



(51)	<b>Int. Cl.</b>		5,876,342 A	3/1999	Chen et al.
	<i>A61B 8/14</i>	(2006.01)	5,891,038 A	4/1999	Seyed-Bolorforosh et al.
	<i>G01S 15/89</i>	(2006.01)	5,892,732 A	4/1999	Gerszenkorn
(56)	<b>References Cited</b>		5,916,169 A	6/1999	Hanafy et al.
			5,919,139 A	7/1999	Lin
			5,920,285 A	7/1999	Benjamin
			5,930,730 A	7/1999	Marfurt et al.
			5,940,778 A	8/1999	Marfurt et al.
			5,964,707 A	10/1999	Fenster et al.
			5,969,661 A	10/1999	Benjamin
			5,999,836 A	12/1999	Nelson et al.
			6,007,499 A	12/1999	Martin et al.
			6,013,032 A	1/2000	Savord
			6,014,473 A	1/2000	Hossack et al.
			6,048,315 A	4/2000	Chiao et al.
			6,049,509 A	4/2000	Sonneiland et al.
			6,050,943 A	4/2000	Slayton et al.
			6,056,693 A	5/2000	Haider
			6,058,074 A	5/2000	Swan et al.
			6,077,224 A	6/2000	Lang et al.
			6,092,026 A	7/2000	Bahorich et al.
			6,122,538 A	9/2000	Sliwa, Jr. et al.
			6,123,670 A *	9/2000	Mo ..... 600/447
			6,129,672 A	10/2000	Seward et al.
			6,135,960 A	10/2000	Holmberg
			6,138,075 A	10/2000	Yost
			6,148,095 A	11/2000	Prause et al.
			6,162,175 A	12/2000	Marian, Jr. et al.
			6,166,384 A	12/2000	Dentinger et al.
			6,166,853 A	12/2000	Sapia et al.
			6,193,665 B1	2/2001	Hall et al.
			6,196,739 B1	3/2001	Silverbrook
			6,200,266 B1	3/2001	Shokrollahi et al.
			6,210,335 B1	4/2001	Miller
			6,213,958 B1	4/2001	Winder
			6,221,019 B1	4/2001	Kantorovich
			6,231,511 B1	5/2001	Bae
			6,238,342 B1	5/2001	Feleppa et al.
			6,246,901 B1	6/2001	Benaron
			6,251,073 B1	6/2001	Imran et al.
			6,264,609 B1	7/2001	Herrington et al.
			6,266,551 B1	7/2001	Osadchy et al.
			6,278,949 B1	8/2001	Alam
			6,289,230 B1	9/2001	Chaiken et al.
			6,304,684 B1	10/2001	Niczyzporuk et al.
			6,309,356 B1	10/2001	Ustuner et al.
			6,324,453 B1	11/2001	Breed et al.
			6,345,539 B1	2/2002	Rawes et al.
			6,361,500 B1	3/2002	Masters
			6,363,033 B1	3/2002	Cole et al.
			6,374,185 B1	4/2002	Taner et al.
			6,394,955 B1	5/2002	Perlitz
			6,423,002 B1	7/2002	Hossack
			6,436,046 B1	8/2002	Napolitano et al.
			6,449,821 B1	9/2002	Sudol et al.
			6,450,965 B2	9/2002	Williams et al.
			6,468,216 B1	10/2002	Powers et al.
			6,471,650 B2	10/2002	Powers et al.
			6,475,150 B2	11/2002	Haddad
			6,480,790 B1	11/2002	Calvert et al.
			6,487,502 B1	11/2002	Taner
			6,499,536 B1	12/2002	Ellingsen
			6,508,768 B1	1/2003	Hall et al.
			6,508,770 B1	1/2003	Cai
			6,517,484 B1	2/2003	Wilk et al.
			6,526,163 B1	2/2003	Halmann et al.
			6,543,272 B1	4/2003	Vitek
			6,547,732 B2	4/2003	Jago
			6,551,246 B1	4/2003	Ustuner et al.
			6,565,510 B1	5/2003	Haider
			6,585,647 B1	7/2003	Winder
			6,604,421 B1	8/2003	Li
			6,614,560 B1	9/2003	Silverbrook
			6,620,101 B2	9/2003	Azzam et al.
			6,652,461 B1	11/2003	Levkovitz
			6,668,654 B2	12/2003	Dubois et al.
			6,672,165 B2	1/2004	Rather et al.
			6,681,185 B1	1/2004	Young et al.
			6,690,816 B2	2/2004	Aylward et al.

(56)	References Cited						
U.S. PATENT DOCUMENTS							
6,692,450	B1	2/2004	Coleman	8,007,439	B2	8/2011	Specht
6,695,778	B2	2/2004	Golland et al.	8,057,392	B2	11/2011	Hossack et al.
6,702,745	B1	3/2004	Smythe	8,057,393	B2	11/2011	Yao et al.
6,719,693	B2	4/2004	Richard	8,079,263	B2	12/2011	Randall et al.
6,728,567	B2	4/2004	Rather et al.	8,079,956	B2	12/2011	Azuma et al.
6,752,762	B1	6/2004	DeJong et al.	8,088,067	B2	1/2012	Vortman et al.
6,755,787	B2	6/2004	Hossack et al.	8,088,068	B2	1/2012	Yao et al.
6,780,152	B2	8/2004	Ustuner et al.	8,088,071	B2	1/2012	Hwang et al.
6,790,182	B2	9/2004	Eck et al.	8,105,239	B2	1/2012	Specht
6,837,853	B2	1/2005	Marian	8,135,190	B2	3/2012	Bae et al.
6,843,770	B2	1/2005	Sumanaweedra	8,157,737	B2	4/2012	Zhang et al.
6,847,737	B1	1/2005	Kouri et al.	8,182,427	B2	5/2012	Wu et al.
6,854,332	B2	2/2005	Alleyne	8,202,219	B2	6/2012	Luo et al.
6,932,767	B2	8/2005	Landry et al.	8,277,383	B2	10/2012	Specht
7,033,320	B2	4/2006	Von Behren et al.	8,279,705	B2	10/2012	Choi et al.
7,087,023	B2	8/2006	Daft et al.	8,412,307	B2	4/2013	Willis et al.
7,104,956	B1	9/2006	Christopher	8,419,642	B2	4/2013	Sandrin et al.
7,217,243	B2	5/2007	Takeuchi	8,478,382	B2	7/2013	Burnside et al.
7,221,867	B2	5/2007	Silverbrook	8,532,951	B2	9/2013	Roy et al.
7,231,072	B2	6/2007	Yamano et al.	8,582,848	B2	11/2013	Funka-Lea et al.
7,269,299	B2	9/2007	Schroeder	8,627,724	B2	1/2014	Papadopoulos et al.
7,283,652	B2	10/2007	Mendonca et al.	8,634,615	B2	1/2014	Brabec
7,285,094	B2	10/2007	Nohara et al.	8,672,846	B2	3/2014	Napolitano et al.
7,313,053	B2	12/2007	Wodnicki	2002/0035864	A1	3/2002	Palfield et al.
7,366,704	B2	4/2008	Reading et al.	2002/0087071	A1	7/2002	Schmitz et al.
7,402,136	B2	7/2008	Hossack et al.	2002/0111568	A1	8/2002	Bukshpan
7,410,469	B1	8/2008	Talish et al.	2002/0161299	A1	10/2002	Prater et al.
7,415,880	B2	8/2008	Renzel	2003/0028111	A1	2/2003	Vaezy et al.
7,443,765	B2	10/2008	Thomenius et al.	2003/0040669	A1	2/2003	Grass et al.
7,444,875	B1	11/2008	Wu et al.	2003/0228053	A1	12/2003	Li et al.
7,447,535	B2	11/2008	Lavi	2004/0054283	A1	3/2004	Corey et al.
7,448,998	B2	11/2008	Robinson	2004/0068184	A1	4/2004	Trahey et al.
7,466,848	B2	12/2008	Metaxas et al.	2004/0100163	A1	5/2004	Baumgartner et al.
7,469,096	B2	12/2008	Silverbrook	2004/0111028	A1	6/2004	Abe et al.
7,474,778	B2	1/2009	Shinomura et al.	2004/0122313	A1	6/2004	Moore et al.
7,481,577	B2	1/2009	Ramamurthy et al.	2004/0122322	A1	6/2004	Moore et al.
7,491,171	B2	2/2009	Barthe et al.	2004/0127793	A1	7/2004	Mendlein et al.
7,497,828	B1	3/2009	Wilk et al.	2004/0138565	A1	7/2004	Trucco
7,497,830	B2	3/2009	Li	2004/0144176	A1	7/2004	Yoden
7,510,529	B2	3/2009	Chou et al.	2004/0236217	A1	11/2004	Cerwin et al.
7,514,851	B2	4/2009	Wilser et al.	2004/0236223	A1	11/2004	Barnes et al.
7,549,962	B2	6/2009	Dreschel et al.	2005/0004449	A1	1/2005	Mitschke et al.
7,574,026	B2	8/2009	Rasche et al.	2005/0053035	A1	3/2005	Li et al.
7,625,343	B2	12/2009	Cao et al.	2005/0054910	A1	3/2005	Tremblay et al.
7,637,869	B2	12/2009	Sudol	2005/0090743	A1	4/2005	Kawashima et al.
7,668,583	B2	2/2010	Fegert et al.	2005/0090745	A1	4/2005	Steen
7,674,228	B2	3/2010	Williams et al.	2005/0111846	A1	5/2005	Steinbacher et al.
7,682,311	B2	3/2010	Simopoulos et al.	2005/0113689	A1	5/2005	Gritzky
7,699,776	B2	4/2010	Walker et al.	2005/0113694	A1	5/2005	Haugen et al.
7,722,541	B2	5/2010	Cai	2005/0124883	A1	6/2005	Hunt
7,744,532	B2	6/2010	Ustuner et al.	2005/0131300	A1	6/2005	Bakircioglu et al.
7,750,311	B2	7/2010	Daghlian	2005/0147297	A1	7/2005	McLaughlin et al.
7,785,260	B2	8/2010	Umemura et al.	2005/0165312	A1	7/2005	Knowles et al.
7,787,680	B2	8/2010	Ahn et al.	2005/0203404	A1	9/2005	Freiburger
7,806,828	B2	10/2010	Stringer	2005/0215883	A1	9/2005	Hundley et al.
7,819,810	B2	10/2010	Stringer et al.	2005/0240125	A1	10/2005	Makin et al.
7,822,250	B2	10/2010	Yao et al.	2005/0252295	A1	11/2005	Fink et al.
7,824,337	B2	11/2010	Abe et al.	2005/0281447	A1	12/2005	Moreau-Gobard et al.
7,833,163	B2	11/2010	Cai	2005/0288588	A1	12/2005	Weber et al.
7,837,624	B1	11/2010	Hossack et al.	2006/0062447	A1	3/2006	Rinck et al.
7,846,097	B2	12/2010	Jones et al.	2006/0074313	A1	4/2006	Slayton et al.
7,850,613	B2	12/2010	Stribling	2006/0074315	A1	4/2006	Liang et al.
7,862,508	B2	1/2011	Davies et al.	2006/0074320	A1	4/2006	Yoo et al.
7,876,945	B2	1/2011	Lötjönen	2006/0079759	A1	4/2006	Vaillant et al.
7,887,486	B2	2/2011	Ustuner et al.	2006/0079778	A1	4/2006	Mo et al.
7,901,358	B2	3/2011	Mehi et al.	2006/0079782	A1	4/2006	Beach et al.
7,907,758	B2	3/2011	Hill et al.	2006/0094962	A1	5/2006	Clark
7,914,451	B2	3/2011	Davies	2006/0111634	A1	5/2006	Wu
7,919,906	B2	4/2011	Cerofolini	2006/0122506	A1	6/2006	Davies et al.
7,926,350	B2	4/2011	Krönig et al.	2006/0173327	A1	8/2006	Kim
7,927,280	B2	4/2011	Davidson	2006/0262291	A1	11/2006	Hess et al.
7,972,271	B2	7/2011	Johnson et al.	2006/0262961	A1	11/2006	Holsing et al.
7,984,637	B2	7/2011	Ao et al.	2007/0016022	A1	1/2007	Blalock et al.
7,984,651	B2	7/2011	Randall et al.	2007/0016044	A1	1/2007	Blalock et al.
8,002,705	B1	8/2011	Napolitano et al.	2007/0036414	A1	2/2007	Georgescu et al.
				2007/0055155	A1	3/2007	Owen et al.
				2007/0078345	A1	4/2007	Mo et al.
				2007/0088213	A1	4/2007	Poland
				2007/0138157	A1	6/2007	Dane et al.

(56)	References Cited					
U.S. PATENT DOCUMENTS						
2007/0161898 A1	7/2007	Hao et al.	2010/0106431 A1	4/2010	Baba et al.	
2007/0161904 A1	7/2007	Urbano	2010/0109481 A1	5/2010	Buccafusca	
2007/0167752 A1	7/2007	Proulx et al.	2010/0121193 A1	5/2010	Fukukita et al.	
2007/0167824 A1	7/2007	Lee et al.	2010/0121196 A1	5/2010	Hwang et al.	
2007/0232914 A1	10/2007	Chen et al.	2010/0130855 A1	5/2010	Lundberg et al.	
2007/0238985 A1	10/2007	Smith et al.	2010/0168566 A1	7/2010	Bercoff et al.	
2007/0242567 A1	10/2007	Daft et al.	2010/0168578 A1	7/2010	Garson, Jr. et al.	
2008/0110261 A1	5/2008	Randall et al.	2010/0174194 A1	7/2010	Chiang et al.	
2008/0110263 A1	5/2008	Klessel et al.	2010/0217124 A1	8/2010	Cooley	
2008/0112265 A1	5/2008	Urbano et al.	2010/0240994 A1	9/2010	Zheng	
2008/0114241 A1	5/2008	Randall et al.	2010/0249570 A1	9/2010	Carson et al.	
2008/0114245 A1	5/2008	Randall et al.	2010/0249596 A1	9/2010	Magee	
2008/0114246 A1	5/2008	Randall et al.	2010/0256488 A1	10/2010	Kim et al.	
2008/0114247 A1	5/2008	Urbano et al.	2010/0262013 A1	10/2010	Smith et al.	
2008/0114248 A1	5/2008	Urbano et al.	2010/0266176 A1	10/2010	Masumoto et al.	
2008/0114249 A1	5/2008	Randall et al.	2010/0268503 A1	10/2010	Specht et al.	
2008/0114250 A1	5/2008	Urbano et al.	2010/0286525 A1	11/2010	Osumi	
2008/0114251 A1	5/2008	Weymer et al.	2010/0286527 A1	11/2010	Cannon et al.	
2008/0114252 A1	5/2008	Randall et al.	2010/0310143 A1	12/2010	Rao et al.	
2008/0114253 A1	5/2008	Randall et al.	2010/0324418 A1	12/2010	El-Aklouk et al.	
2008/0114255 A1	5/2008	Schwartz et al.	2010/0324423 A1	12/2010	El-Aklouk et al.	
2008/0125659 A1	5/2008	Wilser et al.	2010/0329521 A1	12/2010	Beymer et al.	
2008/0181479 A1	7/2008	Yang et al.	2011/0005322 A1	1/2011	Ustuner	
2008/0183075 A1	7/2008	Govari et al.	2011/0016977 A1	1/2011	Guracar	
2008/0188747 A1	8/2008	Randall et al.	2011/0021915 A1	1/2011	Feng	
2008/0188750 A1	8/2008	Randall et al.	2011/0021920 A1	1/2011	Shafir et al.	
2008/0194957 A1	8/2008	Hector et al.	2011/0021923 A1	1/2011	Daft et al.	
2008/0194958 A1	8/2008	Lee et al.	2011/0033098 A1	2/2011	Richter et al.	
2008/0194959 A1	8/2008	Wang et al.	2011/0044133 A1	2/2011	Tokita	
2008/0208061 A1	8/2008	Halmann	2011/0066030 A1	3/2011	Yao	
2008/0242996 A1	10/2008	Hall et al.	2011/0098565 A1	4/2011	Masuzawa	
2008/0249408 A1	10/2008	Palmeri et al.	2011/0112400 A1	5/2011	Emery et al.	
2008/0255452 A1	10/2008	Entrekkin	2011/0112404 A1	5/2011	Gourevitch	
2008/0269604 A1	10/2008	Boctor et al.	2011/0125017 A1	5/2011	Ramamurthy et al.	
2008/0269613 A1	10/2008	Summers et al.	2011/0178400 A1	7/2011	Specht et al.	
2008/0275344 A1	11/2008	Glide-Hurst et al.	2011/0201933 A1	8/2011	Specht et al.	
2008/0285819 A1	11/2008	Konofagou et al.	2011/0270088 A1	11/2011	Shiina	
2008/0287787 A1	11/2008	Sauer et al.	2011/0301470 A1	12/2011	Sato et al.	
2008/0294045 A1	11/2008	Ellington et al.	2011/0306886 A1	12/2011	Daft et al.	
2008/0294050 A1	11/2008	Shinomura et al.	2011/0319764 A1	12/2011	Okada et al.	
2008/0294052 A1	11/2008	Wilser et al.	2012/0004545 A1	1/2012	Ziv-Ari et al.	
2008/0306382 A1	12/2008	Guracar et al.	2012/0035482 A1	2/2012	Kim et al.	
2008/0306386 A1	12/2008	Baba et al.	2012/0036934 A1	2/2012	Krönig et al.	
2008/0319317 A1	12/2008	Kamiyama et al.	2012/0057428 A1	3/2012	Specht et al.	
2009/0010459 A1	1/2009	Garbini et al.	2012/0085173 A1	4/2012	Papadopoulos et al.	
2009/0012393 A1	1/2009	Choi	2012/0095343 A1	4/2012	Smith et al.	
2009/0016163 A1	1/2009	Freeman et al.	2012/0095347 A1	4/2012	Adam et al.	
2009/0018445 A1	1/2009	Schers et al.	2012/0101378 A1	4/2012	Lee	
2009/0024039 A1	1/2009	Wang et al.	2012/0114210 A1	5/2012	Kim et al.	
2009/0036780 A1	2/2009	Abraham	2012/0116226 A1	5/2012	Specht	
2009/0043206 A1	2/2009	Towfig et al.	2012/0121150 A1	5/2012	Murashita	
2009/0048519 A1	2/2009	Hossack et al.	2012/0137778 A1	6/2012	Kitazawa et al.	
2009/0069681 A1	3/2009	Lundberg et al.	2012/0141002 A1	6/2012	Urbano et al.	
2009/0069686 A1	3/2009	Daft et al.	2012/0165670 A1	6/2012	Shi et al.	
2009/0069692 A1	3/2009	Cooley et al.	2012/0179044 A1	7/2012	Chiang et al.	
2009/0099483 A1	4/2009	Rybyanets	2012/0226201 A1	9/2012	Clark et al.	
2009/0112095 A1	4/2009	Daigle	2012/0235998 A1	9/2012	Smith-Casem et al.	
2009/0131797 A1	5/2009	Jeong et al.	2012/0243763 A1	9/2012	Wen et al.	
2009/0143680 A1	6/2009	Yao et al.	2012/0253194 A1	10/2012	Tamura	
2009/0148012 A1	6/2009	Altmann et al.	2012/0265075 A1	10/2012	Pedrizzetti et al.	
2009/0150094 A1	6/2009	Van Velsor et al.	2012/0277585 A1	11/2012	Koenig et al.	
2009/0182237 A1	7/2009	Angelsen et al.	2013/0035595 A1	2/2013	Specht	
2009/0198134 A1	8/2009	Hashimoto et al.	2013/0076207 A1	3/2013	Krohn et al.	
2009/0203997 A1	8/2009	Ustuner	2013/0079639 A1	3/2013	Hector et al.	
2009/0208080 A1	8/2009	Grau et al.	2013/0083628 A1	4/2013	Qiao et al.	
2009/0259128 A1	10/2009	Stribling	2013/0088122 A1	4/2013	Krohn et al.	
2009/0264760 A1	10/2009	Lazebnik et al.	2013/0116561 A1	5/2013	Rothberg et al.	
2009/0306510 A1	12/2009	Hashiba et al.	2013/0131516 A1	5/2013	Katsuyama	
2009/0326379 A1	12/2009	Daigle et al.	2013/0144165 A1	6/2013	Ebbini et al.	
2010/0010354 A1	1/2010	Skerl et al.	2013/0204136 A1	8/2013	Duric et al.	
2010/0016725 A1	1/2010	Thiele	2013/0204137 A1	8/2013	Roy et al.	
2010/0063397 A1	3/2010	Wagner	2013/0247350 A1	9/2013	Specht et al.	
2010/0063399 A1	3/2010	Walker et al.	2013/0258805 A1	10/2013	Hansen et al.	
2010/0069751 A1	3/2010	Hazard et al.	2013/0261463 A1	10/2013	Chiang et al.	
2010/0069756 A1	3/2010	Ogasawara et al.	2014/0073921 A1	3/2014	Specht et al.	
			2014/0135626 A1	5/2014	Specht	
			2014/0243673 A1	8/2014	Anand et al.	
			2015/0045668 A1	2/2015	Smith et al.	

(56)	References Cited							
U.S. PATENT DOCUMENTS								
FOREIGN PATENT DOCUMENTS								
EP	1949856	A1	7/2008	WO	WO2012/160541	A2		
EP	2058796	A2	5/2009	WO	WO2013/059358	A2		
EP	2101191	A2	9/2009	WO	WO2013/109965	A1		
EP	2182352	A2	5/2010	WO	WO2013/116807	A1		
EP	2187813	A1	5/2010	WO	WO2013/116809	A1		
EP	2198785	A1	6/2010	WO	WO2013/116851	A1		
EP	1757955	B1	11/2010	WO	WO2013/116854	A1		
EP	2325672	A1	5/2011	WO	WO2013/116866	A1		
EP	1462819	B1	7/2011	WO	WO2013/128301	A2		
EP	2356941	A1	8/2011	OTHER PUBLICATIONS				
EP	1979739		10/2011	Specht et al.; U.S. Appl. No. 14/279,052 entitled "Ultrasound imaging using apparent point-source transmit transducer," filed May 15, 2014.				
EP	2385391	A2	11/2011	Specht et al.; U.S. Appl. No. 13/773,340 entitled "Determining Material Stiffness Using Multiple Aperture Ultrasound," filed Feb. 21, 2013.				
EP	2294400		2/2012	Call et al.; U.S. Appl. No. 13/850,823 entitled "Systems and methods for improving ultrasound image quality by applying weighting factors," filed Mar. 26, 2013.				
EP	2453256	A2	5/2012	Belevich et al.; U.S. Appl. No. 13/964,701 entitled "Calibration of Multiple Aperture Ultrasound Probes," filed Aug. 12, 2013.				
EP	1840594	B1	6/2012	Call et al.; U.S. Appl. No. 13/971,689 entitled "Ultrasound Imaging System Memory Architecture," filed Aug. 20, 2013.				
EP	2514368	A1	10/2012	Cristianini et al.; An Introduction to Support Vector Machines; Cambridge University Press; pp. 93-111; Mar. 2000.				
EP	1850743	B1	12/2012	Du et al.; User parameter free approaches to multistatic adaptive ultrasound imaging; 5th IEEE International Symposium; pp. 1287-1290, May 2008.				
EP	1594404	B1	9/2013	Feigenbaum, Harvey, M.D.; Echocardiography; Lippincott Williams & Wilkins; Philadelphia; 5th Ed.; pp. 428, 484; Feb. 1994.				
EP	2026280	B1	10/2013	Haykin, Simon; Neural Networks: A Comprehensive Foundation (2nd Ed.); Prentice Hall; pp. 156-187; Jul. 16, 1998.				
FR	2851662	A1	8/2004	Kramb et al.,; Considerations for using phased array ultrasonics in a fully automated inspection system. Review of Quantitative Nondestructive Evaluation, vol. 23, ed. D. O. Thompson and D. E. Chimenti, pp. 817-825, (year of publication is sufficiently earlier than the effective U.S. filed and any foreign priority date) 2004.				
JP	S49-11189	A	1/1974	Ledesma-Carbayo et al.; Spatio-temporal nonrigid registration for ultrasound cardiac motion estimation; IEEE Trans. on Medical Imaging; vol. 24; No. 9; Sep. 2005.				
JP	S54-44375	A	4/1979	Leotta et al.; Quantitative three-dimensional echocardiography by rapid imaging . . . ; J American Society of Echocardiography; vol. 10; No. 8; pp. 830-839; Oct. 1997.				
JP	S55-103839	A	8/1980	Morrison et al.; A probabilistic neural network based image segmentation network for magnetic resonance images; Proc. Conf. Neural Networks; Baltimore, MD; vol. 3; pp. 60-65; Jun. 1992.				
JP	59-101143	A	6/1984	Nadkarni et al.; Cardiac motion synchronization for 3D cardiac ultrasound imaging; Ph.D. Dissertation, University of Western Ontario; Jun. 2002.				
JP	S59-174151	A	10/1984	Press et al.; Cubic spline interpolation; §3.3 in "Numerical Recipes in Fortran: The Art of Scientific Computing", 2nd Ed.; Cambridge, England; Cambridge University Press; pp. 107-110; Sep. 1992.				
JP	S60-13109	U	1/1985	Sakas et al.; Preprocessing and volume rendering of 3D ultrasonic data; IEEE Computer Graphics and Applications; pp. 47-54, Jul. 1995.				
JP	S60-68836	A	4/1985	Sapia et al.; Deconvolution of ultrasonic waveforms using an adaptive wiener filter; Review of Progress in Quantitative Nondestructive Evaluation; vol. 13A; Plenum Press; pp. 855-862; (year of publication is sufficiently earlier than the effective U.S. filed and any foreign priority date) 1994.				
JP	2-501431	A	5/1990	Sapia et al.; Ultrasound image deconvolution using adaptive inverse filtering; 12 IEEE Symposium on Computer-Based Medical Systems, CBMS, pp. 248-253; Jun. 1999.				
JP	4-67856		3/1992	Sapia, Mark Angelo; Multi-dimensional deconvolution of optical microscope and ultrasound imaging using adaptive least-mean-square (LMS) inverse filtering; Ph.D. Dissertation; University of Connecticut; Jan. 2000.				
JP	05-042138	A	2/1993	Smith et al.; High-speed ultrasound volumetric imaging system. 1. Transducer design and beam steering; IEEE Trans. Ultrason., Ferroelectr., Freq. Contr.; vol. 38; pp. 100-108; Mar. 1991.				
JP	6-125908	A	5/1994					
JP	7-051266	A	2/1995					
JP	08-252253		10/1996					
JP	9-103429	A	4/1997					
JP	9-201361	A	8/1997					
JP	10-216128	A	8/1998					
JP	11-089833	A	4/1999					
JP	2001-245884	A	9/2001					
JP	2002-209894	A	7/2002					
JP	2002-253548	A	9/2002					
JP	2002-253549	A	9/2002					
JP	2004-167092	A	6/2004					
JP	2004-215987		8/2004					
JP	2004-337457		12/2004					
JP	2004-351214		12/2004					
JP	2005-523792		8/2005					
JP	2005-526539		9/2005					
JP	2006-122657	A	5/2006					
JP	2008-122209		5/2008					
JP	2008-513763	A	5/2008					
JP	2008-259541	A	10/2008					
JP	20105375		1/2010					
KR	1020090103408	A	10/2009					
WO	WO 92/18054	A1	10/1992					
WO	WO 98/00719	A2	1/1998					
WO	WO02/084594	A2	10/2002					
WO	WO2005/009245	A1	2/2005					
WO	WO 2006/114735	A1	11/2006					
WO	WO 2007/127147	A2	11/2007					
WO	WO2009/060182	A2	5/2009					
WO	WO 2010/017445	A2	2/2010					
WO	WO 2010/095094	A1	8/2010					
WO	WO2011/057252	A1	5/2011					
WO	WO2011/064688	A1	6/2011					
WO	WO2011/100697	A1	8/2011					
WO	WO2011/123529	A1	10/2011					
WO	WO2012/028896	A1	3/2012					
WO	WO2012/049124	A2	4/2012					
WO	WO2012/049612	A2	4/2012					
WO	WO2012/078639	A1	6/2012					
WO	WO2012/091280	A1	7/2012					
WO	WO2012/112540	A2	8/2012					
WO	WO2012/131340	A2	10/2012					

(56)

## References Cited

## OTHER PUBLICATIONS

Specht et al.; Deconvolution techniques for digital longitudinal tomography; SPIE; vol. 454; presented at Application of Optical Instrumentation in Medicine XII; pp. 319-325; Jun. 1984.

Specht et al.; Experience with adaptive PNN and adaptive GRNN; Proc. IEEE International Joint Conf. on Neural Networks; vol. 2; pp. 1203-1208; Orlando, FL; Jun. 1994.

Specht, D.F.; A general regression neural network; IEEE Trans. on Neural Networks; vol. 2.; No. 6; Nov. 1991.

Specht, D.F.; Blind deconvolution of motion blur using LMS inverse filtering; Lockheed Independent Research (unpublished); Jun. 23, 1975.

Specht, D.F.; Enhancements to probabilistic neural networks; Proc. IEEE International Joint Conf. on Neural Networks; Baltimore, MD; Jun. 1992.

Specht, D.F.; GRNN with double clustering; Proc. IEEE International Joint Conf. Neural Networks; Vancouver, Canada; Jul. 16-21, 2006.

Specht, D.F.; Probabilistic neural networks; Pergamon Press; Neural Networks; vol. 3; pp. 109-118; Feb. 1990.

Von Ramm et al.; High-speed ultrasound volumetric imaging-System. 2. Parallel processing and image display; IEEE Trans. Ultrason., Ferroelect., Freq. Contr.; vol. 38; pp. 109-115; Mar. 1991.

Wells, P.N.T.; Biomedical ultrasonics; Academic Press; London, New York, San Francisco; pp. 124-125; Mar. 1977.

Widrow et al.; Adaptive signal processing; Prentice-Hall; Englewood Cliffs, NJ; pp. 99-116; Mar. 1985.

Specht et al.; U.S. Appl. No. 13/690,989 entitled "Motion Detection Using Ping-Based and Multiple Aperture Doppler Ultrasound," filed Nov. 30, 2012.

Hendee et al.; Medical Imaging Physics; Wiley-Liss, Inc. 4th Edition; Chap. 19-22; pp. 303-353; © 2002 (year of pub. sufficiently earlier than effective US filed and any foreign priority date).

Li et al.; An efficient speckle tracking algorithm for ultrasonic imaging; 24; pp. 215-228; Oct. 1, 2002.

UCLA Academic Technology; SPSS learning module: How can I analyze a subset of my data; 6 pages; retrieved from the internet ([http://www.ats.ucla.edu/stat/spss/modules/subset\\_analyze.htm](http://www.ats.ucla.edu/stat/spss/modules/subset_analyze.htm)) Nov. 26, 2001.

Wikipedia; Point cloud; 2 pages; retrieved Nov. 24, 2014 from the internet ([https://en.wikipedia.org/w/index.php?title=Point\\_cloud&oldid=472583138](https://en.wikipedia.org/w/index.php?title=Point_cloud&oldid=472583138)).

Wikipedia; Curve fitting; 5 pages; retrieved from the internet ([http://en.wikipedia.org/wiki/Curve\\_fitting](http://en.wikipedia.org/wiki/Curve_fitting)) Dec. 19, 2010.

Smith et al.; U.S. Appl. No. 14/595,083 entitled "Concave ultrasound transducers and 3D arrays," filed Jan. 12, 2015.

Specht et al.; U.S. Appl. No. 14/078,311 entitled "Imaging with Multiple Aperture Medical Ultrasound and Synchronization of Add-On Systems," filed Nov. 12, 2013.

Specht, D. F.; U.S. Appl. No. 14/157,257 entitled "Method and Apparatus to Produce Ultrasonic Images Using Multiple Apertures," filed Jan. 16, 2014.

Wikipedia; Speed of sound; 17 pages; retrieved from the internet ([http://en.wikipedia.org/wiki/Speed\\_of\\_sound](http://en.wikipedia.org/wiki/Speed_of_sound)) Feb. 15, 2011.

Abeysekera et al.; Alignment and calibration of dual ultrasound transducers using a wedge phantom; Ultrasound in Medicine and Biology; 37(2); pp. 271-279; Feb. 2011.

Carson et al.; Measurement of photoacoustic transducer position by robotic source placement and nonlinear parameter estimation; Biomedical Optics (BiOS); International Society for Optics and Photonics (9th Conf. on Biomedical Thermoacoustics, Optoacoustics, and Acousto-optics; vol. 6856; 9 pages; Feb. 28, 2008.

Chen et al.; Maximum-likelihood source localization and unknown sensor location estimation for wideband signals in the near-field; IEEE Transactions on Signal Processing; 50(8); pp. 1843-1854; Aug. 2002.

Chen et al.; Source localization and tracking of a wideband source using a randomly distributed beamforming sensor array; International Journal of High Performance Computing Applications; 16(3); pp. 259-272; Fall 2002.

Fernandez et al.; High resolution ultrasound beamforming using synthetic and adaptive imaging techniques; Proceedings IEEE International Symposium on Biomedical Imaging; Washington, D.C.; pp. 433-436; Jul. 7-10, 2002.

Gazor et al.; Wideband multi-source beamforming with array location calibration and direction finding; Conference on Acoustics, Speech and Signal Processing ICASSP-95; Detroit, MI; vol. 3 IEEE; pp. 1904-1907; May 9-12, 1995.

Heikkila et al.; A four-step camera calibration procedure with implicit image correction; Proceedings IEEE Computer Society Conference on Computer Vision and Pattern Recognition; San Juan; pp. 1106-1112; Jun. 17-19, 1997.

Hsu et al.; Real-time freehand 3D ultrasound calibration; CUED/F-INFENG/TR 565; Department of Engineering, University of Cambridge, United Kingdom; 14 pages; Sep. 2006.

Khamene et al.; A novel phantom-less spatial and temporal ultrasound calibration method; Medical Image Computing and Computer-Assisted Intervention—MICCAI (Proceedings 8th Int. Conf.); Springer Berlin Heidelberg; Palm Springs, CA; pp. 65-72; Oct. 26-29, 2005.

Slavine et al.; Construction, calibration and evaluation of a tissue phantom with reproducible optical properties for investigations in light emission tomography; Engineering in Medicine and Biology Workshop; Dallas, TX; IEEE pp. 122-125; Nov. 11-12, 2007.

Urban et al.; Implementation of vibro-acoustography on a clinical ultrasound system; IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control; 58(6); pp. 1169-1181; Jun. 2011 (Author Manuscript).

Urban et al.; Implementation of vibro-acoustography on a clinical ultrasound system; IEEE Ultrasonics Symposium (IUS); pp. 326-329; Oct. 14, 2010.

Wang et al.; Photoacoustic tomography of biological tissues with high cross-section resolution: reconstruction and experiment; Medical Physics; 29(12); pp. 2799-2805; Dec. 2002.

Yang et al.; Time-of-arrival calibration for improving the microwave breast cancer imaging; 2011 IEEE Topical Conf. on Biomedical Wireless Technologies, Networks, and sensing Systems (BioWireless); Phoenix, AZ; pp. 67-70; Jan. 16-19, 2011.

Opretzka et al.; A high-frequency ultrasound imaging system combining limited-angle spatial compounding and model-based synthetic aperture focusing; IEEE Transactions on Ultrasonics, Ferroelectrics and Frequency Control, IEEE, US; 58(7); pp. 1355-1365; Jul. 2, 2011.

\* cited by examiner

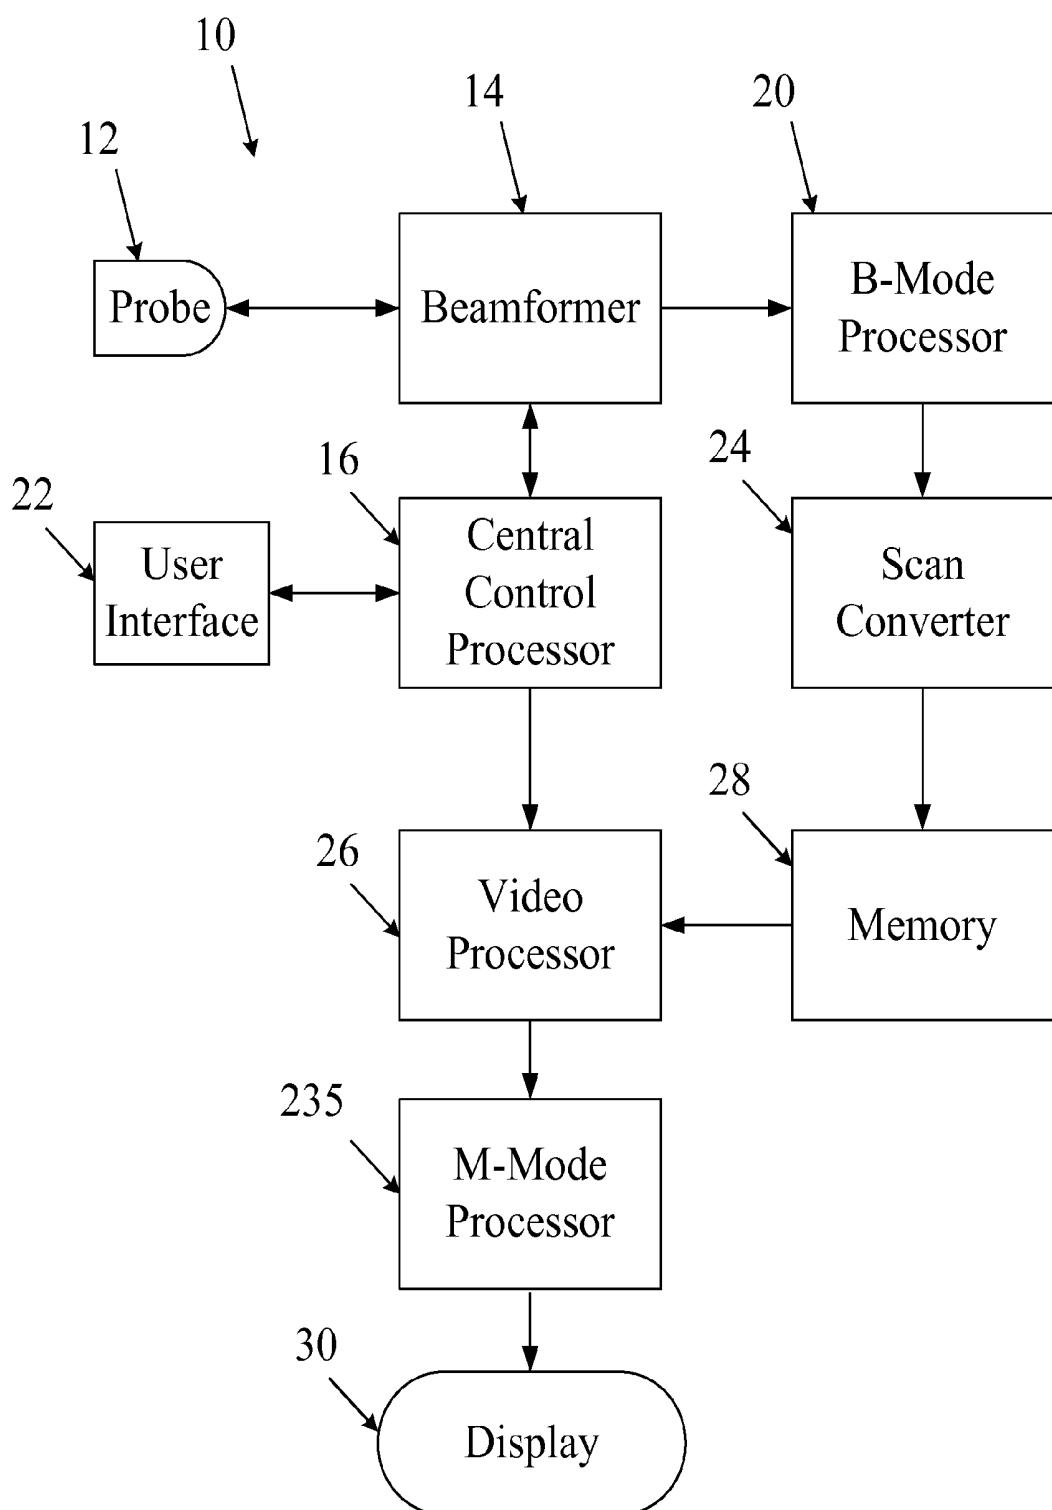
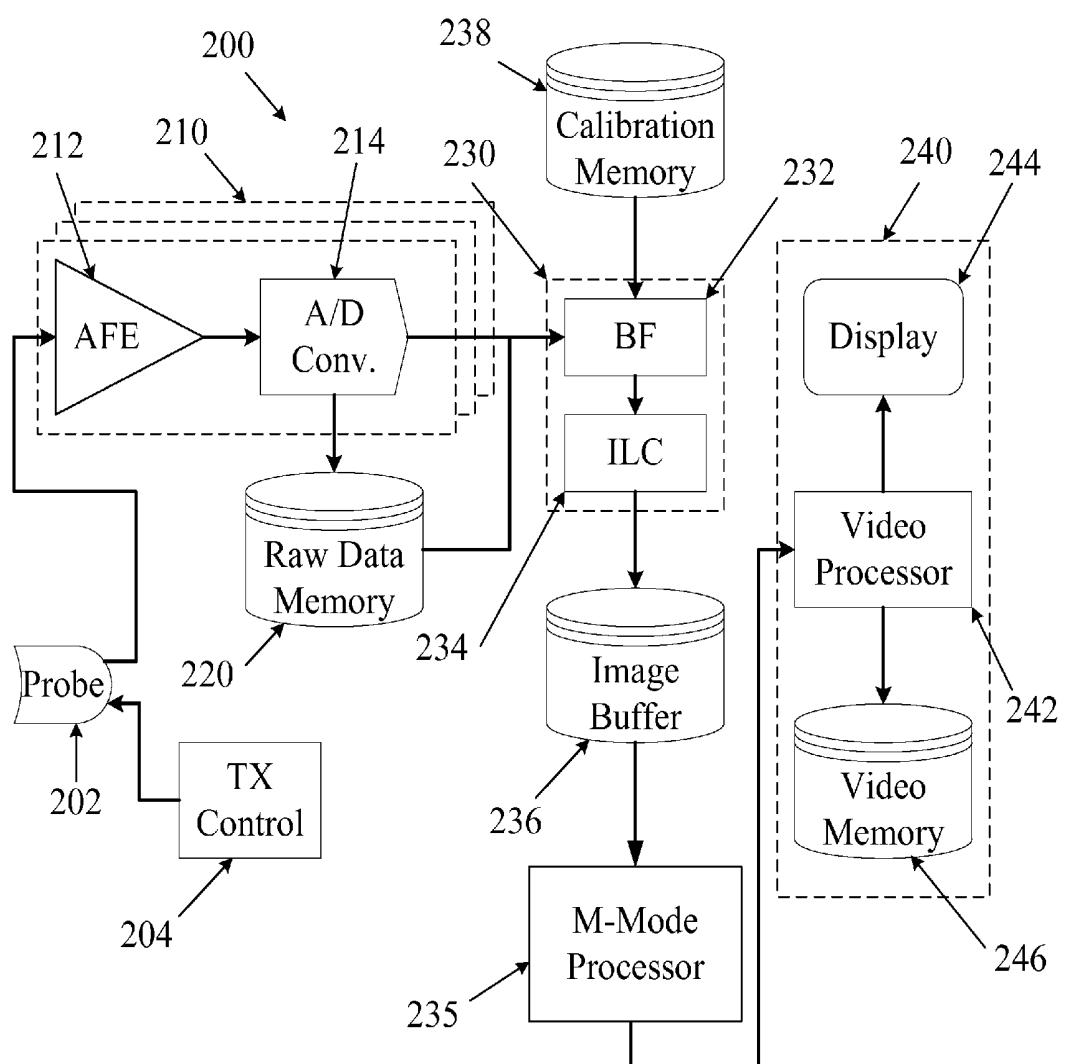
**Fig. 1A**

Fig. 1B



50

Fig. 2

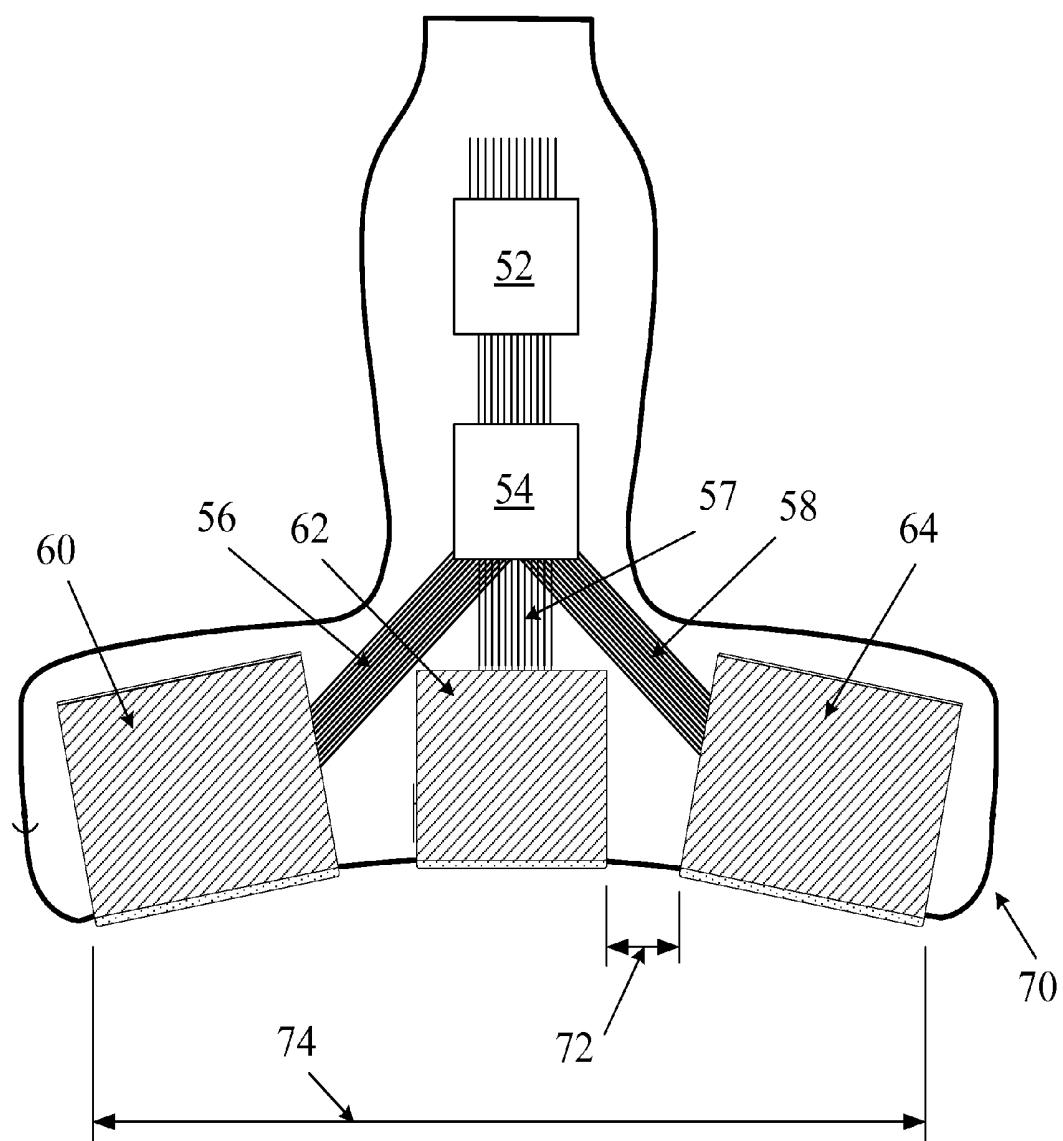
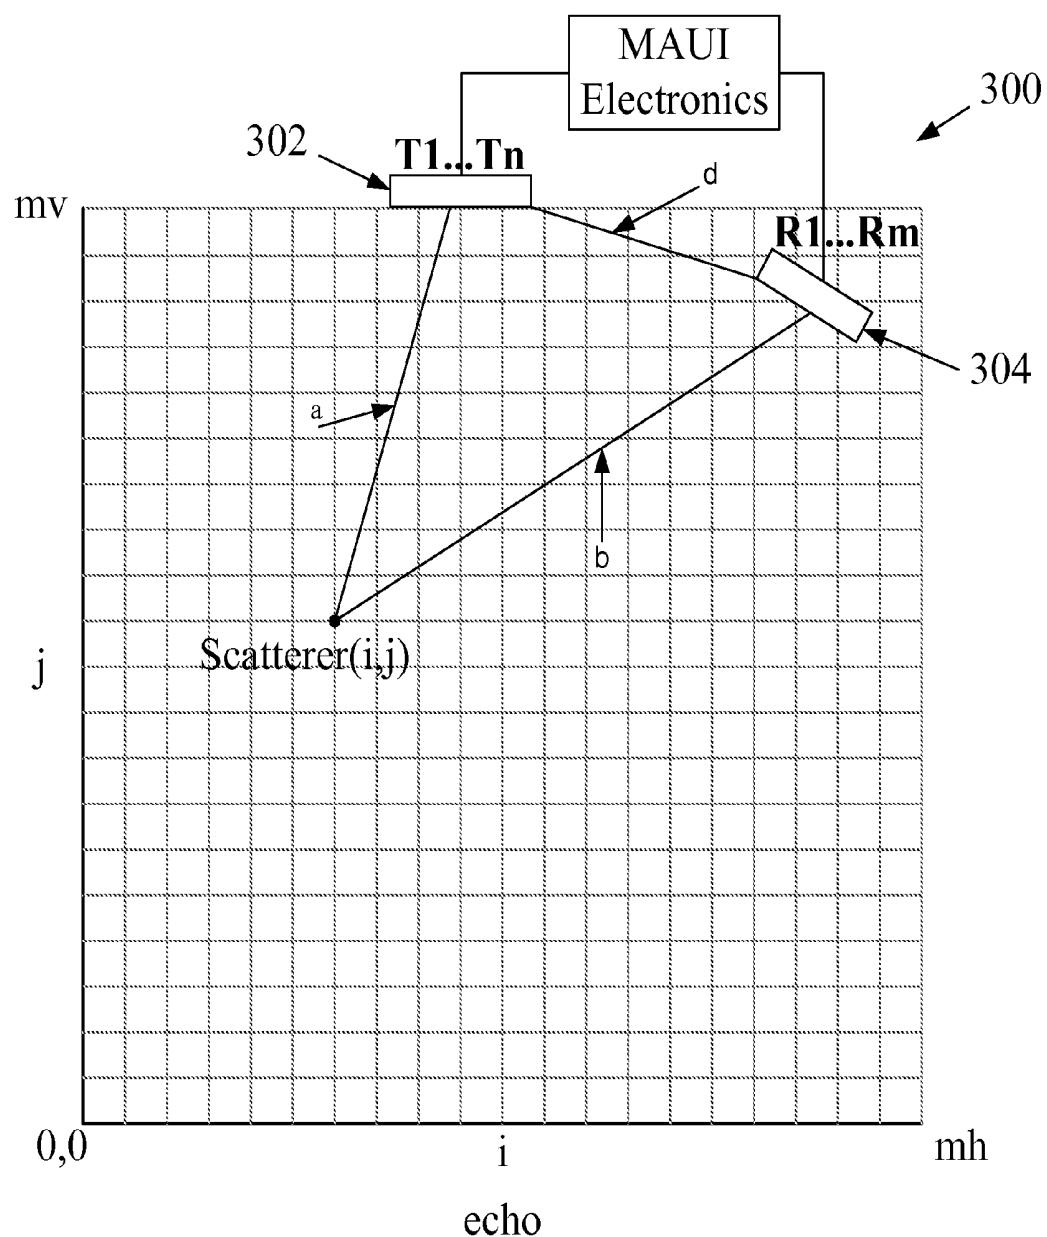
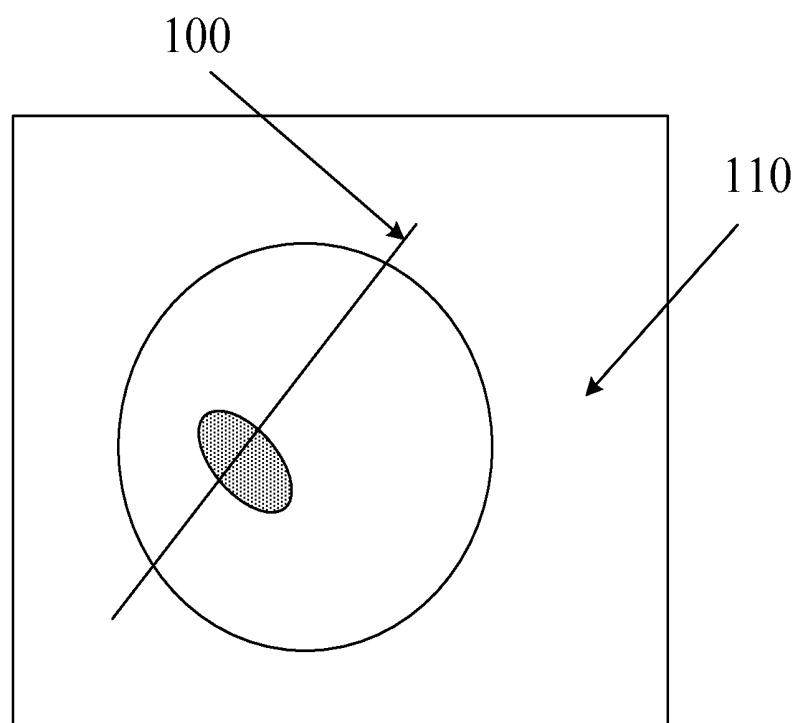
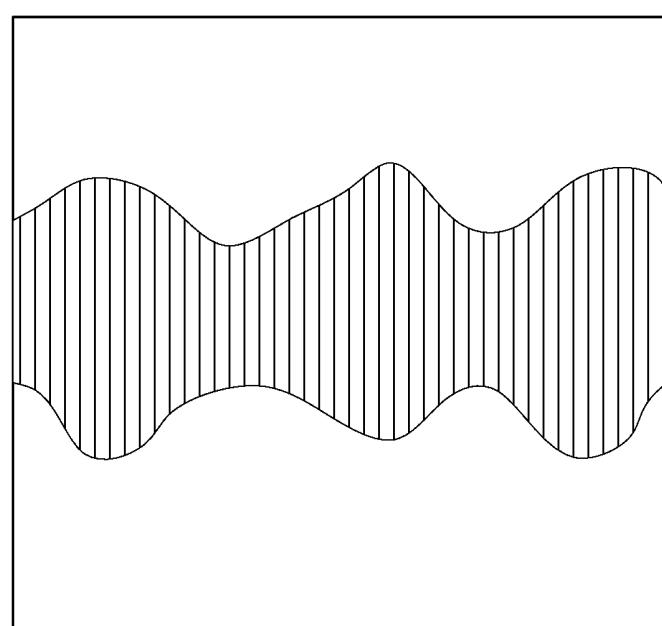
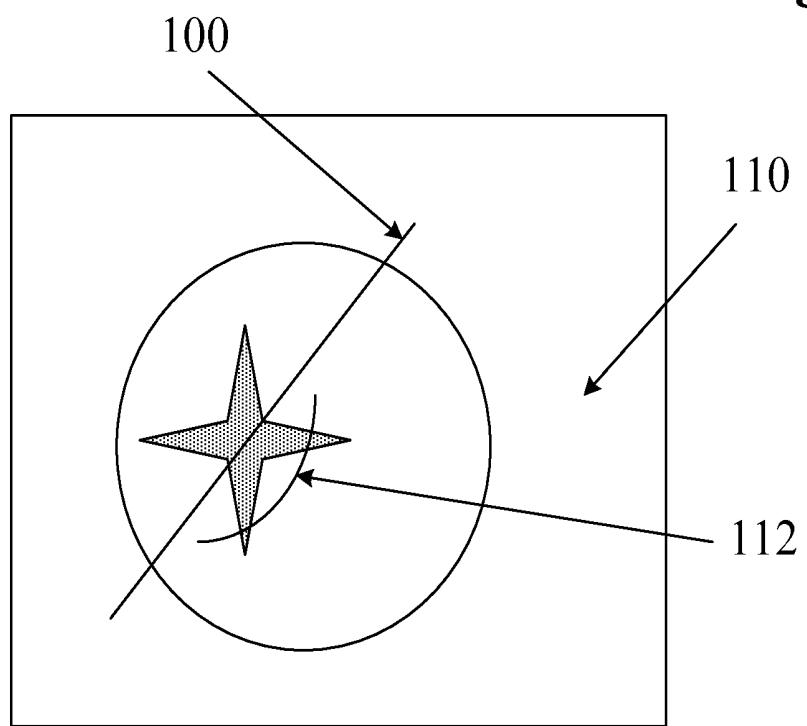
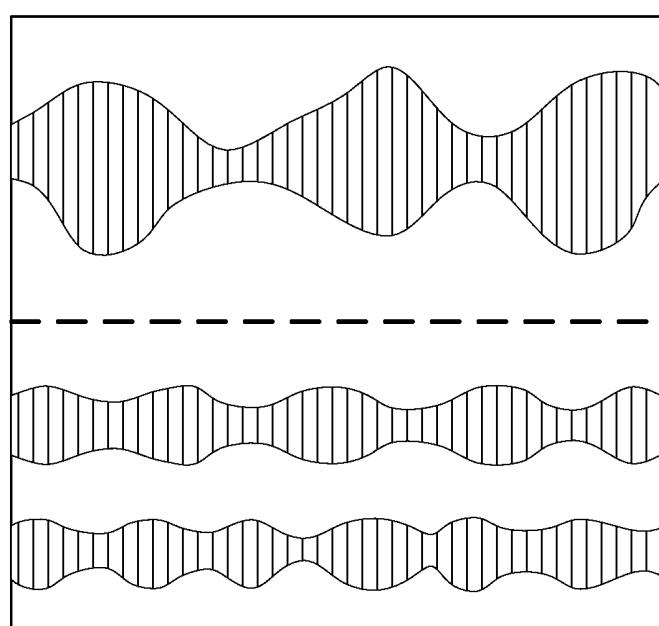


Fig. 3



**Fig. 4A****Fig. 4B**

**Fig. 5A****Fig. 5B**

## M-MODE ULTRASOUND IMAGING OF ARBITRARY PATHS

### CROSS REFERENCE TO RELATED APPLICATIONS

This application claims the benefit of U.S. Provisional Patent Application No. 61/581,583, titled "M-Mode Ultrasound Imaging Of Arbitrary Paths," filed on Dec. 29, 2011, and U.S. Provisional Patent Application No. 61/691,717, titled "Ultrasound Imaging System Memory Architecture," filed on Aug. 21, 2012, both of which are incorporated herein by reference.

### INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

### FIELD

This invention generally relates to ultrasound imaging, and more particularly to M-mode imaging of arbitrary paths.

### BACKGROUND

Conventional ultrasound (or "scanline based" ultrasound as used herein) utilizes a phased array controller to produce and steer a substantially linear transmit waveform. In order to produce a B-mode image, a sequence of such linear waveforms (or "scanlines") may be produced and steered so as to scan across a region of interest. Echoes are received along each respective scanline. The individual scanlines from a complete scan may then be combined to form a complete image (sometimes referred to as a "sector scan" image).

A display method known as M-mode (or motion mode) imaging is commonly used in cardiology and other fields where it is desirable to view the motion of imaged objects. In some forms of M-mode imaging, echoes from a one-dimensional line are displayed over time relative to a static reference point in order to allow a clinician to evaluate movement of a particular structure (such as a cardiac wall or valve) over time. Because a traditional scanline-based ultrasound path is directional (along the scanline axis), available M-mode lines tend to be limited to paths along a scanline.

Generally, M-mode imaging provides a graphic indication of positions and movements of structures within a body over time. In some cases, a single stationary focused acoustic beam is fired at a high frame rate and the resulting M-mode images or lines are displayed side-by-side, providing an indication of the function of a heart over multiple heart cycles.

### SUMMARY OF THE DISCLOSURE

A method of defining and displaying an m-mode path for display in an ultrasound imaging system, the method comprising transmitting an ultrasound signal from a transmitting transducer element into a region of interest including a structure of interest, receiving echoes with at least one receiving transducer element, producing an image of the region of interest from the received echoes, displaying the image of the region of interest including the structure of interest to a user, defining a one-pixel-wide path through the structure of interest, where the path does not lie along a line that intersects the

transmitting transducer element or the receiving transducer element, and displaying a graph of a magnitude of pixels along the path over time.

In some embodiments, the path is non-linear. In other embodiments, the path has at least one curved segment. In one embodiment, the path has at least one linear segment and at least one curved segment. In another embodiment, the path has at least two linear segments that intersect at an angle other than 180 degrees. In some embodiments, the path has at least two discontinuous segments.

In one embodiment, the transmitting transducer element lies on a separate physical transducer array from an array containing the at least one receiving transducer element.

In another embodiment, the transmitting transducer is configured to transmit an unfocused ping ultrasound signal into the region of interest.

In some embodiments, the method further comprises receiving echoes from the entire region of interest with the at least one receiving transducer element, receiving echoes from the entire region of interest with a second receiving transducer element, and producing an image of the region of interest by combining echoes received at the first and second transducer elements.

In some embodiments, defining a path through the structure of interest is performed substantially concurrently with said transmitting and receiving.

In another embodiment, the transmitting transducer is configured to insonify a phased array scan line.

A method of ultrasound imaging is also provided, comprising transmitting ultrasound signals into a region of interest and receiving echoes of the transmitted ultrasound signals with an ultrasound probe, defining a first image window as a portion of the region of interest, identifying an M-mode path intersecting a feature visible in the first image window, displaying data representing the M-mode path on a common display with a B-mode image of the first image window, defining a second image window as a portion of the region of interest that is different than the first image window, and displaying the data representing the M-mode path on a common display with a B-mode image of the second image window.

In one embodiment, all of the method steps are performed during a live real-time imaging session.

In another embodiment, the M-mode path includes at least one non-linear segment. In one embodiment, the M-mode path is not a line intersecting the probe.

In another embodiment, all of the method steps are performed using stored raw echo data retrieved from a raw data memory device.

In some embodiments, the first image window is smaller than and lies entirely within the second image window. In another embodiment, the second image window does not overlap the first image window.

In an additional embodiment, the method further comprises simultaneously displaying the data of the M-mode path on a common display with B-mode images of both the first image window and the second window.

In some embodiments, the M-mode path has at least two discontinuous segments.

A multi-aperture M-mode ultrasound imaging system is also provided, comprising a transmitting transducer element configured to transmit an ultrasound signal into a region of interest including a structure of interest, a receiving transducer element separate from the transmitting transducer element, the receiving transducer element configured to receive echoes from the ultrasound signal, a controller configured to produce an image of the region of interest from the received

echoes, an input mechanism configured to receive a user input defining a one-pixel-wide path through the structure of interest, where the path does not lie along a line that intersects the transmitting transducer element or the receiving transducer element, and a display configured to display the region of interest including the structure of interest, the display also configured to display a graph of a magnitude of pixels along the path over time.

In some embodiments, the transmitting transducer is configured to transmit an unfocused ping ultrasound signal into the region of interest.

In another embodiment, the transmitting transducer is configured to transmit an unfocused spherical ping ultrasound signal into the region of interest. In some embodiments, the transmitting transducer is configured to insonify a phased array scan line.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The novel features of the invention are set forth with particularity in the claims that follow. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying drawings of which:

Having thus summarized the general nature of the invention, embodiments and modifications thereof will become apparent to those skilled in the art from the detailed description below with reference to the attached figures.

FIG. 1A is a block diagram illustrating components of an ultrasound imaging system.

FIG. 1B is a block diagram illustrating another embodiment of an ultrasound imaging system.

FIG. 2 is a section view of a multiple aperture ultrasound imaging probe.

FIG. 3 is a schematic illustration of a multiple aperture ultrasound imaging process using a point-source transmit signal.

FIG. 4A is an illustration of a B-mode ultrasound image with an M-mode path defined through a portion of an imaged object.

FIG. 4B is an illustration of an M-mode graph of the data along the M-mode path of FIG. 4A.

FIG. 5A is an illustration of a B-mode ultrasound image with multiple M-mode paths defined through a portion of an imaged object.

FIG. 5B is an illustration of an M-mode graph of the data along the multiple M-mode paths of FIG. 5A.

#### DETAILED DESCRIPTION

In traditional ultrasound systems, images are generated by combining echoes from a series of pulses transmitted as phased array scan lines. In such scanline-based ultrasound imaging systems, the coordinate system used by the user interface usually lies along the scan lines. As a result, in such systems, a user interface for selecting an M-mode line typically involves selecting a desired segment of one of the scan lines. However, requiring the use of scan lines as M-mode lines means that the sonographer must position and hold the probe such that at least one of the scanlines intersects an anatomical feature through which an M-mode line is desired. In practice, this may be difficult and/or time consuming, and may limit the field of view.

Embodiments below provide systems and methods for obtaining M-mode data substantially in real-time along an

arbitrary and/or user-defined path that does not necessarily lie along an ultrasound scan line. In some embodiments, the path may be a one-dimensional straight line. In other embodiments, the path may comprise a zig-zag pattern, a curved path, or any other non-linear path. As used herein the term “one-dimensional” may refer to a narrow path, whether linear, curved, or otherwise shaped. In some embodiments, a one-dimensional path may have a width of a single display pixel. In other embodiments, a one-dimensional path may have a width greater than one display pixel (e.g., 2 or 3 pixels), but may still have a length that is substantially greater than its width. As will be clear to the skilled artisan, the relationship between actual dimensions of represented objects and image pixels may be any value defined by the imaging system. In some embodiments, the M-mode path is not necessarily a straight line, and may include components at any orientation within the scan plane.

In some embodiments, an ultrasound imaging system may be configured to obtain three-dimensional (3D) image data, in which case an M-mode path may be selected from a displayed 3D volume. For example, an M-mode path may be defined in a 3D volume by selecting a desired plane through the 3D volume, and then defining an M-mode path within the selected 2D plane using any of the systems and methods described herein.

Some embodiments of systems and methods for specifying and displaying arbitrary M-mode lines may be used in conjunction with ping-based and/or multiple aperture ultrasound imaging systems. In other embodiments, systems and methods for specifying and displaying arbitrary M-mode lines as shown and described herein may also be used in conjunction with scanline-based imaging systems.

#### Ultrasound Imaging System Components

FIG. 1A is a block diagram illustrating components of an ultrasound imaging system that may be used with some embodiments of M-mode imaging systems and methods. The ultrasound system 10 of FIG. 1A may be particularly suited for scanline-based imaging and may be configured for acquiring real-time cardiac images either as 2D tomographic slices or as volumetric image data. The system may include a central controller/processor configured to control the other system components, including the probe 12 which includes one or more transducer arrays, elements of which may transmit and/or receive ultrasound signals. In some embodiments, the transducer array(s) may include a 1D, 2D or other dimensional arrays formed from any suitable transducer material. The probe may generally be configured to transmit ultrasonic waves and to receive ultrasonic echo signals. In some embodiments, such transmission and reception may be controlled by a controller which may include a beamformer 14. The echo information from the beamformer 14 may then be processed by a B-mode processor 20 and/or other application-specific processors as needed (e.g., Doppler processors, contrast signal processors, elastography processors, etc.).

The B-Mode processor 20 may be configured to perform functions that include but are not limited to filtering, frequency and spatial compounding, harmonic data processing and other B-Mode functions. In some embodiments, the processed data may then be passed through a scan converter 24 configured to geometrically correct the data from a linear or polar geometry used by a phased-array scanning probe into a Cartesian format (x,y or x,y,z) with appropriate scaling in each dimension. In some embodiments, such as the embodiment described below with reference to FIGS. 2 and 3, a scan converter 24 may be omitted from the system.

Data for each 2D image or 3D volume may then be stored in a memory 28. The memory 28 may be volatile and/or

non-volatile memory configured to store a few seconds up to several minutes or more of 2D or 3D echo image data. The video processor 26 may be configured to take the echo data stored in memory 28 and instructions from the central controller 16 to form video images, including any added graphic overlays and/or text annotation (e.g. patient information). Processed video data may then be passed on to the display 30 for presentation to the operator. The central controller 16 can direct the video processor 26 to display the most recently acquired data in memory as a real-time display, or it can replay sequences of older stored 2D slice or 3D volume data.

An M-mode processor 235 may also be provided to receive a definition of an M-mode path from a user interface and to form the images displaying the selected M-mode data in a desired output format. In some embodiments, an M-mode processor 235 may also include a (volatile or non-volatile) memory device for storing the defined M-mode path. In some embodiments, an M-mode processor 235 may be logically positioned between the video processor 26 and the display 30 in the diagram of FIG. 1A. In other embodiments, an M-mode processor 235 may be a set of functions built into the video processor 26 or another component of the system.

FIG. 1B illustrates another embodiment of an ultrasound imaging system 200 comprising an ultrasound probe 202 which may include a plurality of individual ultrasound transducer elements, some of which may be designated as transmit elements, and others of which may be designated as receive elements. In some embodiments, each probe transducer element may convert ultrasound vibrations into time-varying electrical signals and vice versa. In some embodiments, the probe 202 may include any number of ultrasound transducer arrays in any desired configuration. A probe 202 used in connection with the systems and methods described herein may be of any configuration as desired, including single aperture and multiple aperture probes.

The transmission of ultrasound signals from elements of the probe 202 may be controlled by a transmit controller 204. Upon receiving echoes of transmit signals, the probe elements may generate time-varying electric signals corresponding to the received ultrasound vibrations. Signals representing the received echoes may be output from the probe 202 and sent to a receive subsystem 210. In some embodiments, the receive subsystem may include multiple channels, each of which may include an analog front-end device ("AFE") 212 and an analog-to-digital conversion device (ADC) 214. In some embodiments, each channel of the receive subsystem 210 may also include digital filters and data conditioners (not shown) after the ADC 214. In some embodiments, analog filters prior to the ADC 214 may also be provided. The output of each ADC 214 may be directed into a raw data memory device 220. In some embodiments, an independent channel of the receive subsystem 210 may be provided for each receive transducer element of the probe 202. In other embodiments, two or more transducer elements may share a common receive channel.

In some embodiments, an analog front-end device 212 (AFE) may perform certain filtering processes before passing the signal to an analog-to-digital conversion device 214 (ADC). The ADC 214 may be configured to convert received analog signals into a series of digital data points at some pre-determined sampling rate. Unlike most ultrasound systems, some embodiments of the ultrasound imaging system of FIG. 1B may then store digital data representing the timing, phase, magnitude and/or the frequency of ultrasound echo signals received by each individual receive element in a raw

data memory device 220 before performing any further beamforming, filtering, image layer combining or other image processing.

In order to convert the captured digital samples into an image, the data may be retrieved from the raw data memory 220 by an image generation subsystem 230. As shown, the image generation subsystem 230 may include a beamforming block 232 and an image layer combining ("ILC") block 234. In some embodiments, a beamformer 232 may be in communication with a calibration memory 238 that contains probe calibration data. Probe calibration data may include information about the precise acoustic position, operational quality, and/or other information about individual probe transducer elements. The calibration memory 238 may be physically located within the probe, within the imaging system, or in location external to both the probe and the imaging system.

In some embodiments, after passing through the image generation block 230, image data may then be stored in an image buffer memory 236 which may store beamformed and (in some embodiments) layer-combined image frames. A video processor 242 within a video subsystem 240 may then retrieve image frames from the image buffer, and may process the images into a video stream that may be displayed on a video display 244 and/or stored in a video memory 246 as a digital video clip, e.g. as referred to in the art as a "cine loop".

An M-mode processor 235 may also be provided to receive a definition of an M-mode path from a user interface and to form the images displaying the selected M-mode data in a desired output format. In some embodiments, an M-mode processor 235 may also include a (volatile or non-volatile) memory device for storing the defined M-mode path. In some embodiments, an M-mode processor 235 may be logically positioned between the image buffer 236 and the video processor 242 in the diagram of FIG. 1B. In other embodiments, an M-mode processor 235 may be a set of functions built into the image generation subsystem 230 or the video processor 242 or any other suitable component of the system.

In some embodiments, raw echo data stored in a memory device may be retrieved, beamformed, processed into images, and displayed on a display using a device other than an ultrasound imaging system. For example, such a system may omit the probe 202, the transmit controller 204 and the receive sub-system 210 of FIG. 1B, while including the remaining components. Such a system may be implemented predominantly in software running on general purpose computing hardware. Such alternative processing hardware may comprise a desktop computer, a tablet computer, a laptop computer, a smartphone, a server or any other general purpose data processing hardware.

#### Introduction to Ping-Based Imaging

Some embodiments of ultrasound imaging systems to be used in combination with the systems and methods described herein may use point source transmission of ultrasound signals during the transmit pulse. An ultrasound wavefront transmitted from a point source (also referred to herein as a "ping") illuminates the entire region of interest with each circular or spherical wavefront. Echoes from a single ping received by a single receive transducer element may be beamformed to form a complete image of the insonified region of interest. By combining data and images from multiple receive transducers across a wide probe, and by combining data from multiple pings, very high resolution images may be obtained.

As used herein the terms "point source transmission" and "ping" may refer to an introduction of transmitted ultrasound energy into a medium from a single spatial location. This may be accomplished using a single ultrasound transducer ele-

ment or combination of adjacent transducer elements transmitting together. A single transmission from one or more element(s) may approximate a uniform spherical wave front, or in the case of imaging a 2D slice, may create a uniform circular wavefront within the 2D slice. In some cases, a single transmission of a circular or spherical wavefront from a point source transmit aperture may be referred to herein as a “ping” or a “point source pulse” or an “unfocused pulse.”

Point source transmission differs in its spatial characteristics from a scanline-based “phased array transmission” or a “directed pulse transmission” which focuses energy in a particular direction (along a scanline) from the transducer element array. Phased array transmission manipulates the phase of a group of transducer elements in sequence so as to strengthen or steer an insonifying wave to a specific region of interest.

Images may be formed from such ultrasound pings by beamforming the echoes received by one or more receive transducer elements. In some embodiments, such receive elements may be arranged into a plurality of apertures in a process referred to as multiple aperture ultrasound imaging.

Beamforming is generally understood to be a process by which imaging signals received at multiple discrete receptors are combined to form a complete coherent image. The process of ping-based beamforming is consistent with this understanding. Embodiments of ping-based beamforming generally involve determining the position of reflectors corresponding to portions of received echo data based on the path along which an ultrasound signal may have traveled, an assumed-constant speed of sound and the elapsed time between a transmit ping and the time at which an echo is received. In other words, ping-based imaging involves a calculation of distance based on an assumed speed and a measured time. Once such a distance has been calculated, it is possible to triangulate the possible positions of any given reflector. This distance calculation is made possible with accurate information about the relative positions of transmit and receive transducer elements (As discussed in Applicants' previous applications referenced above, a multiple aperture probe may be calibrated to determine the acoustic position of each transducer element to at least a desired degree of accuracy.) In some embodiments, ping-based beamforming may be referred to as “dynamic beamforming.”

A dynamic beamformer may be used to determine a location and an intensity for an image pixel corresponding to each of the echoes resulting from each transmitted ping. When transmitting a ping signal, no beamforming need be applied to the transmitted waveform, but dynamic beamforming may be used to combine the echoes received with the plurality of receive transducers to form pixel data.

The image quality may be further improved by combining images formed by the beamformer from one or more subsequent transmitted pings. Still further improvements to image quality may be obtained by combining images formed by more than one receive aperture. An important consideration is whether the summation of images from different pings or receive apertures should be coherent summation (phase sensitive) or incoherent summation (summing magnitude of the signals without phase information). In some embodiments, coherent (phase sensitive) summation may be used to combine echo data received by transducer elements located on a common receive aperture resulting from one or more pings. In some embodiments, incoherent summation may be used to combine echo data or image data received by receive apertures that could possibly contain cancelling phase data. Such may be the case with receive apertures that have a combined

total aperture that is greater than a maximum coherent aperture width for a given imaging target.

As used herein the terms “ultrasound transducer” and “transducer” may carry their ordinary meanings as understood by those skilled in the art of ultrasound imaging technologies, and may refer without limitation to any single component capable of converting an electrical signal into an ultrasonic signal and/or vice versa. For example, in some embodiments, an ultrasound transducer may comprise a piezoelectric device. In some alternative embodiments, ultrasound transducers may comprise capacitive micromachined ultrasound transducers (CMUT). Transducers are often configured in arrays of multiple elements. An element of a transducer array may be the smallest discrete component of an array. For example, in the case of an array of piezoelectric transducer elements, each element may be a single piezoelectric crystal.

As used herein, the terms “transmit element” and “receive element” may carry their ordinary meanings as understood by those skilled in the art of ultrasound imaging technologies. The term “transmit element” may refer without limitation to an ultrasound transducer element which at least momentarily performs a transmit function in which an electrical signal is converted into an ultrasound signal. Similarly, the term “receive element” may refer without limitation to an ultrasound transducer element which at least momentarily performs a receive function in which an ultrasound signal impinging on the element is converted into an electrical signal. Transmission of ultrasound into a medium may also be referred to herein as “insonifying.” An object or structure which reflects ultrasound waves may be referred to as a “reflector” or a “scatterer.”

As used herein the term “aperture” refers without limitation to one or more ultrasound transducer elements collectively performing a common function at a given instant of time. For example, in some embodiments, the term aperture may refer to a group of transducer elements performing a transmit function. In alternative embodiments, the term aperture may refer to a plurality of transducer elements performing a receive function. In some embodiments, group of transducer elements forming an aperture may be redefined at different points in time.

Generating ultrasound images using a ping-based ultrasound imaging process means that images from an entire region of interest are “in focus” at all times. This is true because each transmitted ping illuminates the entire region, receive apertures receive echoes from the entire region, and the dynamic multiple aperture beamforming process may form an image of any part or all of the insonified region. In such cases, the maximum extent of the image may be primarily limited by attenuation and signal-to-noise factors rather than by the confined focus of a transmit or receive beamforming apparatus. As a result, a full-resolution image may be formed from any portion of a region of interest using the same set of raw echo data. As used herein, the term “image window” will be used to refer to a selected portion of an entire insonified region of interest that is being displayed at any given time. For example, a first image window may be selected to include an entire insonified area, and then a user may choose to “zoom in” on a smaller selected area, thereby defining a new image window. The user may then choose to zoom out or pan the image window vertically and/or horizontally, thereby selecting yet another image window. In some embodiments, separate simultaneous images may be formed of multiple overlapping or non-overlapping image windows within a single insonified region.

## Embodiments of Multiple Aperture Ultrasound Imaging Systems and Methods

Applicant's prior U.S. patent application Ser. No. 11/865,501 filed on Oct. 1, 2007, published as US Patent Application Publication 2008/0103393 and U.S. patent application Ser. No. 13/029,907 ("the '907 application"), published as 2011/0201933, describe embodiments of ultrasound imaging techniques using probes with multiple apertures to provide substantially increased resolution over a wide field of view.

In some embodiments, a probe may include one, two, three or more apertures for ultrasound imaging. FIG. 2 illustrates one embodiment of a multiple aperture ultrasound probe which may be used for ultrasound imaging with a point source transmit signal. The probe of FIG. 2 comprises three transducer arrays 60, 62, 64, each one of which may be a 1D, 2D, CMUT or other ultrasound transducer array. In alternative embodiments, a single curved array may also be used, each aperture being defined logically electronically as needed. In still further embodiments, any single-aperture or multiple-aperture ultrasound imaging probe may also be used. As shown, the lateral arrays 60 and 64 may be mounted in a probe housing 70 at angles relative to the center array 62. In some embodiments, the angle  $\theta$  of the lateral arrays relative to the central array may be between zero and 45 degrees or more. In one embodiment, the angle  $\theta$  is about 30 degrees. In some embodiments, the right and left lateral arrays 60, 64 may be mounted at different angles relative to the center array 62. In some embodiments, the probe 50 of FIG. 2 may have a total width 74 substantially wider than 2 cm, and in some embodiments 10 cm or greater.

In some embodiments as shown in FIG. 2, separate apertures of the probe may comprise separate transducer arrays which may be physically separated from one another. For example, in FIG. 2, a distance 72 physically separates the center aperture 62 from the right lateral aperture 64. The distance 72 can be the minimum distance between transducer elements on aperture 62 and transducer elements on aperture 64. In some embodiments, the distance 72 may be equal to at least twice the minimum wavelength of transmission from the transmit aperture. In some embodiments of a multiple aperture ultrasound imaging system, a distance between adjacent apertures may be at least a width of one transducer element. In alternative embodiments, a distance between apertures may be as large as possible within the constraints of a particular application and probe design.

In some embodiments, a probe such as that illustrated in FIG. 2 may be used with an ultrasound imaging system such as that illustrated in FIG. 1 but omitting the scan converter. As will be described in more detail below, some embodiments of a point-source imaging method negate the need for a scan converter. The probe 50 may also include one or more sensors 52 and/or controllers 54 joined to an ultrasound imaging system and/or to the transducer arrays by cables 56, 57, 58. Embodiments of similar multiple aperture probes 50 are also shown and described in US Patent Application Publication No. 2010/0262013 and U.S. patent application Ser. No. 13/029,907, filed on Feb. 17, 2011, published as 2011/0201933, both of which are incorporated herein by reference.

Embodiments of multiple aperture ultrasound imaging methods using a point-source transmit signal will now be described with reference to FIG. 3. FIG. 3 illustrates a probe 300 with a first aperture 302 and a second aperture 304 directed toward a region of interest represented by the grid below the probe. In the illustrated embodiment, the first aperture is used as a transmit aperture 302, and the second aperture 304 is used for receiving echoes. In some embodiments, an ultrasound image may be produced by insonifying an entire

region of interest to be imaged with a point-source transmitting element in a transmit aperture 302, and then receiving echoes from the entire imaged plane on one or more receive elements (e.g., R1-Rm) in one or more receive apertures 304.

In some embodiments, subsequent insonifying pulses may be transmitted from each of the elements T1-Tn on the transmitting aperture 302 in a similar point-source fashion. Echoes may then be received by elements on the receive aperture(s) 302 after each insonifying pulse. An image may be formed by processing echoes from each transmit pulse. Although each individual image obtained from a transmit pulse may have a relatively low resolution, combining these images may provide a high resolution image.

In some embodiments, transmit elements may be operated in any desired sequential order, and need not follow a prescribed pattern. In some embodiments, receive functions may be performed by all elements in a receive array 302. In alternative embodiments, echoes may be received on only one or a select few elements of a receive array 302.

The data received by the receiving elements is a series of echoes reflected by objects within the target region. In order to generate an image, each received echo must be evaluated to determine the location of the object within the target region 25 that reflected it (each reflected point may be referred to herein as a scatterer). For a scatterer point represented by coordinates (i,j) in FIG. 3, it is a simple matter to calculate the total distance "a" from a particular transmit element Tx to an element of internal tissue or target object T at (i,j), and the 30 distance "b" from that point to a particular receive element. These calculations may be performed using basic trigonometry. The sum of these distances is the total distance traveled by one ultrasound wave.

Assuming the speed of the ultrasound waves traveling 35 through the target object is known, these distances can be translated into time delays which may be used to identify a location within the image corresponding to each received echo. When the speed of ultrasound in tissue is assumed to be uniform throughout the target object, it is possible to calculate 40 the time delay from the onset of the transmit pulse to the time that an echo is received at the receive element. Thus, a given scatterer in the target object is the point for which a+b=the given time delay. The same method can be used to calculate delays for all points in the desired target to be imaged, creating 45 a locus of points. As discussed in more detail in the '907 application, adjustments to time delays may be made in order to account for variations in the speed of sound through varying tissue paths.

A method of rendering the location of all of the scatterers in 50 the target object, and thus forming a two dimensional cross section of the target object, will now be described with reference to FIG. 3 which illustrates a grid of points to be imaged by apertures 302 and 304. A point on the grid is given the rectangular coordinates (i,j). The complete image will be a 55 two dimensional array of points provided to a video processing system to be displayed as a corresponding array of pixels. In the grid of FIG. 3, 'mh' is the maximum horizontal dimension of the array and 'mv' is the maximum vertical dimension. FIG. 3 also illustrates MAUI electronics, which can comprise any hardware and/or software elements as needed, such as those described above with reference to FIG. 1.

In some embodiments, the following pseudo code may be used to accumulate all of the information to be gathered from a transmit pulse from one transmit element (e.g., one element of T1 . . . Tn from aperture 302), and the consequent echoes received by one receive element (e.g., one element of R1 . . . Rm from aperture 304) in the arrangement of FIG. 3.

---

```

for (i = 0; i < mh; i++){
  for (j = 0; j < mv; j++){
    compute distance a
    compute distance b
    compute time equivalent of a+b
    echo[i][j] = echo[i][j]+stored received echo at the computed time
  }
}

```

---

delay.

A complete two dimensional image may be formed by repeating this process for every receive element in a receive aperture 304 (e.g., R1 . . . Rm). In some embodiments, it is possible to implement this code in parallel hardware resulting in real time image formation.

In some embodiments, image quality may be further improved by combining similar images resulting from pulses from other transmit elements. In some embodiments, the combination of images may be performed by a simple summation of the single point source pulse images (e.g., coherent addition). Alternatively, the combination may involve taking the absolute value of each element of the single point source pulse images first before summation (e.g., incoherent addition). Further details of such combinations, including corrections for variations in speed-of-sound through different ultrasound paths, are described in Applicant's prior U.S. Patent Applications referenced above.

As discussed above, because embodiments of an imaging system using a point source transmit signal and a multiple-aperture receive probe are capable of receiving an entire scan-plan image in response to a single insonifying pulse, a scan converter is not needed, and may therefore be omitted from an ultrasound imaging system. Having received a series of image frames in a similar manner, the image data may be processed and sent to a display for viewing by an operator. In addition to ultrasound imaging systems using point-source transmit signals, the following methods of selecting and displaying arbitrary m-mode paths may also be used with any other ultrasound imaging system, including phased array transmit systems, single-aperture probes, 3D probes, and probes in systems using synthetic aperture techniques.

#### Embodiments for Defining and Displaying Arbitrary M-mode Paths

FIG. 4A illustrates an example of an ultrasound image with a specified m-mode path 100 drawn through an imaged object 110. The amplitude of each pixel along the m-mode path may be displayed in a graph (e.g. a bar graph, line graph or any other desired format). Changing pixel amplitude values may be illustrated over time. FIG. 4B illustrates an example of a graph of data taken along the m-mode path 100 of FIG. 4A.

In some embodiments, a sonographer may wish to simultaneously view changes along two or more separate M-mode paths. Thus in some embodiments, a user may define a plurality of M-mode paths 110, 112 as shown in FIG. 5A. The change in pixel values lying along the first and second paths 110, 112 may be displayed simultaneously in a pair of amplitude/time charts as shown for example in FIG. 5B. FIG. 5A also shows an example of a non-linear path 112. As discussed in further detail below, a non-linear M-mode path may have any length and shape as desired.

Multiple discontinuous M-mode paths and/or non-linear M-mode paths may be beneficial in viewing movement of multiple structures simultaneously. For example, a curve M-mode path may be beneficial when imaging a anatomic structures such as a moving valve, such as a tricuspid valve, an aortic valve or a mitral valve. In other embodiments, multiple simultaneous but dis-continuous m-mode lines may be used

to simultaneously view the movement of multiple structures. For example, a first m-mode path may be drawn to view operation of a tricuspid valve, and a second M-mode path may be drawn to view operation of a mitral valve. Viewing the function of both valves simultaneously may provide substantial diagnostic benefits, such as allowing for precise calibration of a pacemaker.

Selection of an M-mode path generally involves identifying a group of image pixel locations which are to be presented over time as an M-mode graph. Identifying a group of pixels for an m-mode path may comprise identifying the coordinates of selected pixels in a coordinate system used by the video processing system. In some embodiments, M-mode selection and display methods as described herein may be performed in real-time using an ultrasound imaging system such as those illustrated in FIGS. 1A and 1B. With reference to FIGS. 1A and 1B, selection of an M-mode path may be performed by a user via a suitable user interface interaction performed in communication with the M-mode processor 235. The identification of selected pixels may be at least temporarily stored in a memory device associated with the M-mode processor 235. The selected pixels defining the M-mode path may then be retrieved from image frames in the image buffer and/or in the video processor, and an M-mode graph or image illustrating the values of the selected pixels may be formed by the M-mode processor 235 and transmitted to the display to be displayed along with the B-mode image. In alternative embodiments, M-mode selection and display methods as described herein may be performed on a workstation playing back stored 2D or 3D image data.

In some embodiments, selection of a group of pixel locations for presentation as an M-mode path may be assisted by or entirely performed automatically, such as by using a computer aided detection (CAD) system configured to identify a desired anatomical or other feature through which an m-mode path may be desired. For example, US Patent Application Publication No. 2011/0021915 describes a system for automatic detection of structures in M-mode ultrasound imaging. In other embodiments, a desired M-mode path may be chosen by a user through any of several possible user interface interactions, several examples of which are provided below.

As will be clear to the skilled artisan, an imaging system or an image display system may include a variety of user interface devices through which a user may input information to or modify information or objects in a displayed image. Such user interface devices may comprise any of the following, trackballs, buttons, keys, keypads, sliders, dials, voice commands, touch screen, joystick, mouse, etc. The use of these and other user input devices will be clear to the skilled artisan.

In some embodiments, any arbitrary line or path in the image plane may be selected by a user as a line for M-mode display. In some embodiments, a linear path of defined length may be selected as an m-mode path. This may be facilitated through a number of user interface interactions, some examples of which are provided below.

In some embodiments, the ultrasound display may include a touch screen, and a user may define an M-mode path by simply drawing the desired path with a finger or stylus directly on the display screen. In other embodiments, a user may draw a freehand path using a separate user interface device such as a mouse or a drawing tablet. In some embodiments, after drawing a path of a desired shape, an M-mode path of the desired shape may be dragged across a display and/or rotated to a desired position.

In one embodiment of a user interface interaction, a linear m-mode path segment may be selected by first defining a line length, then defining a rotation angle, and then translating the

line into a desired position. In some embodiments, further adjustments to the line length, rotation angle, and position may be made as needed. In some embodiments, defining a line length may comprise entering a numeric value with a numeric keypad or increasing/decreasing a numeric line length value with a scroll wheel, track ball, dial, slider, arrow keys or other input device. Similarly, in some embodiments, a rotation angle may be defined by entering a numeric value with a numeric keypad or any other input device. A rotation angle may be defined relative to any suitable coordinate system. For example, in some embodiments, a rotation angle of zero degrees may correspond to a three o-clock position (e.g., assuming the top of the image is 12 o-clock).

In some embodiments, numeric values of line length or rotation angle may not be displayed, instead only changes to a line length or rotation angle of the line may be shown on the display screen. In some embodiments, translating the line up, down, left or right within the image plane may be performed using arrow keys, a track ball, a mouse, touch screen, voice commands or other input devices.

In another embodiment of a user interface interaction, a desired linear m-mode path segment may be selected by defining or adjusting a line length, translating the line until a first end point is in a desired position, fixing the first end point and rotating the second end point until the line is rotated to the desired orientation and position.

In another embodiment of a user interface interaction, a desired linear m-mode path segment may be selected by first selecting a first end point, such as by positioning a cursor at a desired position on the image. A line length and rotation angle may then be defined and adjusted as needed. In some embodiments, a rotation angle may be defined by directing the system to pivot the line about the selected first end point. Alternatively, a user may select the second end point or another point along the line about which to pivot the line in order to define a desired rotation angle.

In another embodiment of a user interface interaction, a desired linear m-mode path segment may be selected by selecting a first end point with a cursor and then dragging the cursor in a desired direction to draw a line. In other embodiments, a line may be defined by selecting first and second end points, defining a line by joining the two points.

In any case, once a line is defined, either automatically or through a user interface interaction such as those described above, the length and rotation angle may be adjustable through further user interface interactions. For example, a user may define a pivot point about which to pivot the line in order to adjust a rotation angle. Similarly, a user may select a fixed point from which to increase or decrease the length of the line. Such fixed points and pivot points may be either one of the end points, or any other point along the line.

In some embodiments, a non-linear M-mode path may be defined through any of the above user interface interactions by joining linear segments to form any desired non-linear path made up of linear segments. In some embodiments, a user may choose to apply a radius to the M-mode path in areas adjacent intersections of linear segments. In some embodiments, such a radius may be applied automatically, or may be increased or decreased through a user interface interaction.

In other embodiments, a non-linear M-mode path may be defined by providing a user with a free-form drawing cursor with which the user may draw any non-linear path as desired. Further adjustments may then be made to the path, such as by selecting and dragging one or more individual points along the path to obtain a desired M-mode path.

As described above, multiple images may be formed for two or more separate simultaneous image windows showing

different overlapping or non-overlapping portions of an insonified region of interest. Thus, in some embodiments, an M-mode path may be defined while a first image window is displayed, and a user may then zoom or pan the image to a second image window. In some embodiments, the system may be configured to continue displaying the data along the defined M-mode path even when the displayed B-mode image is changed to a different image window than the one in which the M-mode path was defined. For example, a user may zoom in to view a heart valve, and may define an M-mode path intersecting the valve in the zoomed-in image window. The user may then choose to zoom out to view the movement of the whole heart (or a different region of the heart) while continuing to monitor data along the M-mode line intersecting the heart valve.

In some embodiments, the system may store a definition of the image window in which the M-mode line was defined, and may allow a user to toggle between a B-mode image of the M-mode defining image window and a B-mode image of at least one other image window. In still further embodiments, the system may be configured to simultaneously display B-mode images of both the M-mode defining window and another image window (e.g., in a picture-in-picture mode or in a side-by-side view).

Any of the above user interface interactions may also be used to define an M-mode path through a displayed 3D volume. In some embodiments, defining an M-mode path from a 3D volume may also involve a step of rotating an image of a 3D volume before after or during any of the M-mode path defining user interface steps described above.

Although various embodiments are described herein with reference to ultrasound imaging of various anatomic structures, it will be understood that many of the methods and devices shown and described herein may also be used in other applications, such as imaging and evaluating non-anatomic structures and objects. For example, the ultrasound probes, systems and methods described herein may be used in non-destructive testing or evaluation of various mechanical objects, structural objects or materials, such as welds, pipes, beams, plates, pressure vessels, layered structures, etc. Therefore, references herein to medical or anatomic imaging targets such as blood, blood vessels, heart or other organs are provided merely as non-limiting examples of the nearly infinite variety of targets that may be imaged or evaluated using the various apparatus and techniques described herein.

Although this invention has been disclosed in the context of certain preferred embodiments and examples, it will be understood by those skilled in the art that the present invention extends beyond the specifically disclosed embodiments to other alternative embodiments and/or uses of the invention and obvious modifications and equivalents thereof. Thus, it is intended that the scope of the present invention herein disclosed should not be limited by the particular disclosed embodiments described above, but should be determined only by a fair reading of the claims that follow. In particular, materials and manufacturing techniques may be employed as within the level of those with skill in the relevant art. Furthermore, reference to a singular item, includes the possibility that there are plural of the same items present. More specifically, as used herein and in the appended claims, the singular forms "a," "and," "said," and "the" include plural referents unless the context clearly dictates otherwise. It is further noted that the claims may be drafted to exclude any optional element. As such, this statement is intended to serve as antecedent basis for use of such exclusive terminology as "solely," "only" and the like in connection with the recitation of claim elements, or use of a "negative" limitation. Unless defined

## 15

otherwise herein, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs.

What is claimed is:

1. A method of defining and displaying an M-mode path for display in an ultrasound imaging system, the method comprising:

transmitting a first unfocused ultrasound signal from a single transmitting transducer element into a region of interest including a structure of interest;

receiving echoes of the first unfocused ultrasound signal with a first group of receiving transducer elements;

receiving echoes of the first unfocused ultrasound signal with a second group of receiving transducer elements;

retrieving position data describing an acoustic position of the single transmitting transducer element, each element of the first group of receiving transducer elements, and each element of the second group of receiving transducer elements;

forming a first image by using the position data to calculate reflector positions for the echoes received with each of the elements of the first group of receiving transducer elements and coherently combining echo data received by the elements of the first group of receiving transducer elements;

forming a second image by using the position data to calculate reflector positions for the echoes received with each of the elements of the second group of receiving transducer elements and coherently combining echo data received by the elements of the second group of receiving transducer elements;

producing an improved-quality image of the region of interest from the received echoes by incoherently combining the first image and the second image;

displaying the improved-quality image of the region of interest including the structure of interest to a user;

defining an arbitrary one-pixel-wide path through the structure of interest; and

displaying a graph of a magnitude of pixels along the path over time.

2. The method of claim 1, wherein the path is non-linear.

3. The method of claim 2, wherein the path has at least one curved segment.

## 16

4. The method of claim 1, wherein the path has at least one linear segment and at least one curved segment.

5. The method of claim 2, wherein the path has at least two linear segments that intersect at an angle other than 180 degrees.

6. The method of claim 1, wherein the path has at least two dis-continuous segments.

7. The method of claim 1, wherein the transmitting transducer element lies on a separate physical transducer array from an array containing the first group of receiving transducer elements.

8. The method of claim 1, wherein defining a path through the structure of interest is performed substantially concurrently with said transmitting and receiving.

9. A method of ultrasound imaging, comprising: transmitting ultrasound signals into a region of interest and receiving echoes of the transmitted ultrasound signals with an ultrasound probe;

defining a first image window as a first portion of the region of interest;

identifying an M-mode path intersecting a feature visible in the first image window;

defining a second image window as a second portion of the region of interested that is different than the first image window; and

displaying the data representing the M-mode path from the first image window on a common display with a B-mode image of the second image window while a B-mode image of the first image window is not displayed; wherein the second portion of the region of interest defining the second image window does not overlap any of the first portion of the region of interest defining the first image window.

10. The method of claim 9, wherein all of the method steps are performed during a live real-time imaging session.

11. The method of claim 9, wherein the M-mode path includes at least one non-linear segment.

12. The method of claim 9, wherein the M-mode path is not a line intersecting the probe.

13. The method of claim 9, wherein the M-mode path has at least two dis-continuous segments.

\* \* \* \* \*

专利名称(译)	任意路径的M模式超声成像		
公开(公告)号	<a href="#">US9265484</a>	公开(公告)日	2016-02-23
申请号	US13/730346	申请日	2012-12-28
[标]申请(专利权)人(译)	BREWER KENNETH D 史密斯戴维M LORENZATO ROZALIN M RITZI布鲁斯 - [R]		
申请(专利权)人(译)	布鲁尔, KENNETH D. 斯密, 大卫M. LORENZATO, ROZALIN M. RITZI, BRUCE R.		
当前申请(专利权)人(译)	MAUI IMAGING, INC.		
[标]发明人	BREWER KENNETH D SMITH DAVID M LORENZATO ROZALIN M RITZI BRUCE R		
发明人	BREWER, KENNETH D. SMITH, DAVID M. LORENZATO, ROZALIN M. RITZI, BRUCE R.		
IPC分类号	A61B8/00 A61B8/08 A61B8/14 G01S15/89		
CPC分类号	A61B8/486 A61B8/14 A61B8/4444 A61B8/463 A61B8/467 G01S15/8927 A61B8/145 A61B8/4477 A61B8/4488 A61B8/5207 G01S15/8913 A61B8/466		
优先权	61/581583 2011-12-29 US 61/691717 2012-08-21 US		
其他公开文献	US20130172743A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

## 摘要(译)

M模式超声成像的系统和方法允许沿用户定义的路径进行M模式成像。在各种实施例中，用户定义的路径可以是非线性路径或弯曲路径。在一些实施例中，用于M模式超声成像的系统可包括具有至少第一发射孔和第二接收孔的多孔探头。接收孔可以与发射孔分开。在一些实施例中，发射孔径可以被配置为将未聚焦的球形超声ping信号发射到感兴趣的区域中。用户定义的路径可以定义感兴趣的区域内的感兴趣结构。

