

(10) **Patent No.:** US 10,117,640 B2
(45) **Date of Patent:** *Nov. 6, 2018

(54) **QUANTITATIVE ELASTOGRAPHY WITH TRACKED 2D ULTRASOUND TRANSDUCERS**

(58) **Field of Classification Search**
CPC A61B 8/485; A61B 8/12; A61B 8/4209;
A61B 8/4263; A61B 8/483; A61B 8/4281
See application file for complete search history.

(71) Applicant: **The University of British Columbia,**
Vancouver (CA)

(56) **References Cited**

(72) Inventors: **Septimiu Edmund Salcudean**, Vancouver (CA); **Caitlin Marie Schneider**, Vancouver (CA); **Robert N. Rohling**, Vancouver (CA); **Ali Baghani**, Vancouver (CA); **Mohammad Honarvar**, Vancouver (CA)

U.S. PATENT DOCUMENTS

5,107,837 A 4/1992 Ophir et al.
5,538,004 A * 7/1996 Bamber G01S 7/52044
128/916

(Continued)

(73) Assignee: **The University of British Columbia,**
Vancouver (CA)

OTHER PUBLICATIONS

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

Huwart, L. et al., "Liver fibrosis: non-invasive assessment with MR elastography", *NMR in Biomedicine* 2006, 19, pp. 173-179.

(Continued)

This patent is subject to a terminal disclaimer.

Primary Examiner — Bo J Peng

(74) *Attorney, Agent, or Firm* — Oyen Wiggs Green & Mutala LLP

(21) Appl. No.: 15/798,186

(57) **ABSTRACT**

(22) Filed: **Oct. 30, 2017**

A method is described for acquiring 3D quantitative ultrasound elastography volumes. A 2D ultrasound transducer scans a volume of tissue through which shear waves are created using an external vibration source, the synchronized measurement of tissue motion within the plane of the ultrasound transducer with the measurement of the transducer location in space, the reconstruction of tissue displacements and/or tissue velocities in time and space over a volume from this synchronized measurement, and the computation of one or several mechanical properties of tissue from this volumetric measurement of displacements. The tissue motion in the plane of the transducer may be measured at a high effective frame rate in the axial direction of the transducer, or in the axial and lateral directions of the transducer. The tissue displacements and/or tissue velocities over the measured volume may be interpolated over a regular grid in order to facilitate computation of mechanical properties.

(65) **Prior Publication Data**

US 2018/0125455 A1 May 10, 2018

Related U.S. Application Data


(63) Continuation-in-part of application No. 14/040,558, filed on Sep. 27, 2013, now Pat. No. 9,801,615.

(Continued)

(51) **Int. Cl.**
A61B 8/08 (2006.01)
A61B 8/00 (2006.01)
A61B 8/12 (2006.01)

(52) **U.S. Cl.**
CPC *A61B 8/485* (2013.01); *A61B 8/12*
(2013.01); *A61B 8/4209* (2013.01);
(Continued)

22 Claims, 12 Drawing Sheets

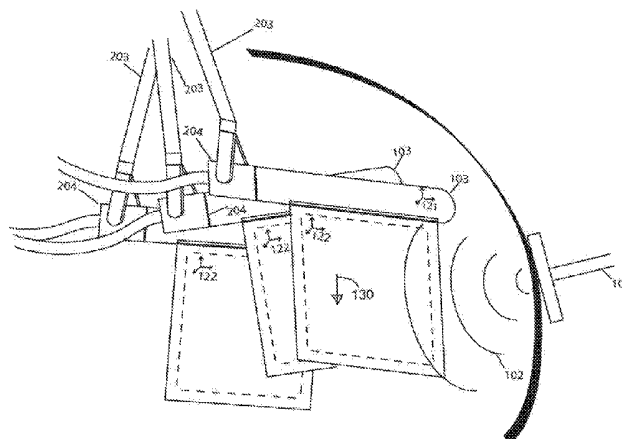

Related U.S. Application Data

- (60) Provisional application No. 61/707,883, filed on Sep. 28, 2012.
- (52) **U.S. Cl.**
CPC *A61B 8/4263* (2013.01); *A61B 8/483* (2013.01); *A61B 8/4281* (2013.01)

(56) References Cited

U.S. PATENT DOCUMENTS

5,825,186	A	10/1998	Ehman et al.	
5,952,828	A	9/1999	Rossmann et al.	
5,977,770	A	11/1999	Ehman	
7,034,534	B2	4/2006	Ehman et al.	
2003/0220556	A1 *	11/2003	Porat	<i>A61B 5/0051</i> 600/407
2005/0252295	A1	11/2005	Fink et al.	
2006/0264736	A1	11/2006	Ehman et al.	
2008/0255444	A1	10/2008	Li	
2009/0209847	A1	8/2009	Li	
2010/0005892	A1	1/2010	Ehman et al.	
2010/0045289	A1	2/2010	Chopra et al.	
2013/0338505	A1	12/2013	Schneider et al.	
2014/0330122	A1	11/2014	Baghani et al.	

OTHER PUBLICATIONS

Yin, M. et al., "Assessment of Hepatic Fibrosis With Magnetic Resonance Elastography", *Journal of Clinical Gastroenterology and Hepatology*, vol. 5, Issue 10, Oct. 2007, pp. 1207-1213.

Sinkus, R. et al., "Viscoelastic shear properties of in vivo breast lesions measured by MR elastography", *Journal of Magnetic Resonance Imaging* vol. 23, 2005, pp. 159-165.

Hamhaber, U. et al., "Three-dimensional analysis of shear wave propagation observed by in vivo magnetic resonance elastography of the brain", *Acta Biomaterialia*, vol. 3, 2007, pp. 127-137.

Dresner, M.A. et al., *Proceedings of the International Society for Magnetic Resonance in Medicine* titled "MR Elastography of the Prostate", 1999.

Sinkus, R. et al., "In-Vivo Prostate MR-Elastography", *Proceedings of International Society of Magnetic Resonance in Medicine*, vol. 11, p. 586, 2003.

Kemper, J. et al., "MR Elastography of the Prostate: Initial In-vivo Application", *Fortschritte auf dem Gebiete der Röntgenstrahlen und der Nuklearmedizin* (Advances in the area of X-ray and Nuclear Medicine), vol. 176, pp. 1094-1099, 2004.

Chopra, R. et al., "In Vivo MR Elastography of the Prostate Gland Using a Transurethral Actuator", *Magnetic Resonance in Medicine*, vol. 62, 2009, pp. 665-671.

Lindop, J. et al., "3D elastography using freehand ultrasound", *Ultrasound in Medicine and Biology*, 32(4), 2006, 529-545.

Baghani, A. et al., "A High-Frame-Rate Ultrasound System for the Study of Tissue Motions", *IEEE Ultrasonics, Ferroelectrics and Frequency Control*, 57(7), 1535-1547 (2010).

Eskandari, H. et al., "Bandpass Sampling of High-Frequency Tissue Motion", *IEEE Transactions on Ultrasonics, Ferroelectrics and Frequency Control*, 58(7), 2011, 1332-1343.

Mercier, L. et al., "A review of calibration techniques for freehand 3-D ultrasound systems", *Ultrasound in Medicine & Biology* 31(2), 143-165 (2005).

Schneider, C. et al., "Remote Ultrasound Palpation for Robotic Interventions using Absolute Elastography", presented at the 15th International Conference on Medical Image Computing and Computer Assisted Intervention, Oct. 2, 2012, Springer LNCS 7510, pp. 42-49.

Schneider, C. et al., "Intra-operative 'Pick-Up' Ultrasound for Robot Assisted Surgery with Vessel Extraction and Registration: A Feasibility Study", *IPCAI 2011*, pp. 122-132.

Doyley, M.M., "Model-based elastography: a survey of approaches to the inverse elasticity problem", *Physics in Medicine and Biology* 57(3), 2012, R35-R73.

Rohling, R. et al., "A comparison of freehand three-dimensional ultrasound reconstruction techniques", *Medical Image Analysis*, 1999, vol. 3, No. 4, pp. 339-359.

Turgay, E. et al., "Identifying the Mechanical properties of Tissue by Ultrasound Strain Imaging", *Ultrasound in Medicine and Biology*, 32(2), pp. 221-235, 2006.

Manduca, A. et al., "Local wavelength estimation for magnetic resonance elastography", *IEEE Conference on Image Processing*, 1996, 527-530.

* cited by examiner

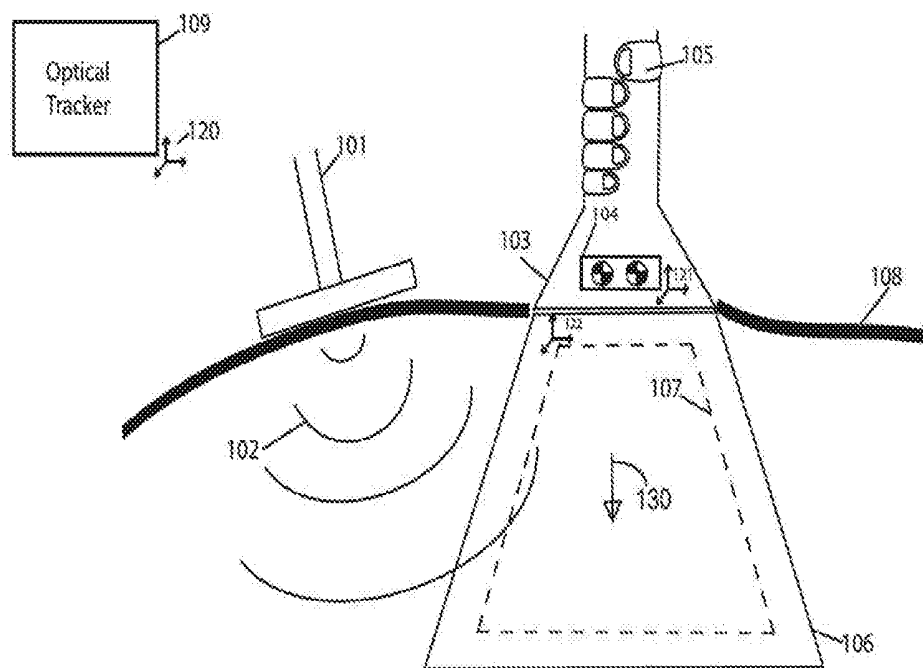


FIG 1

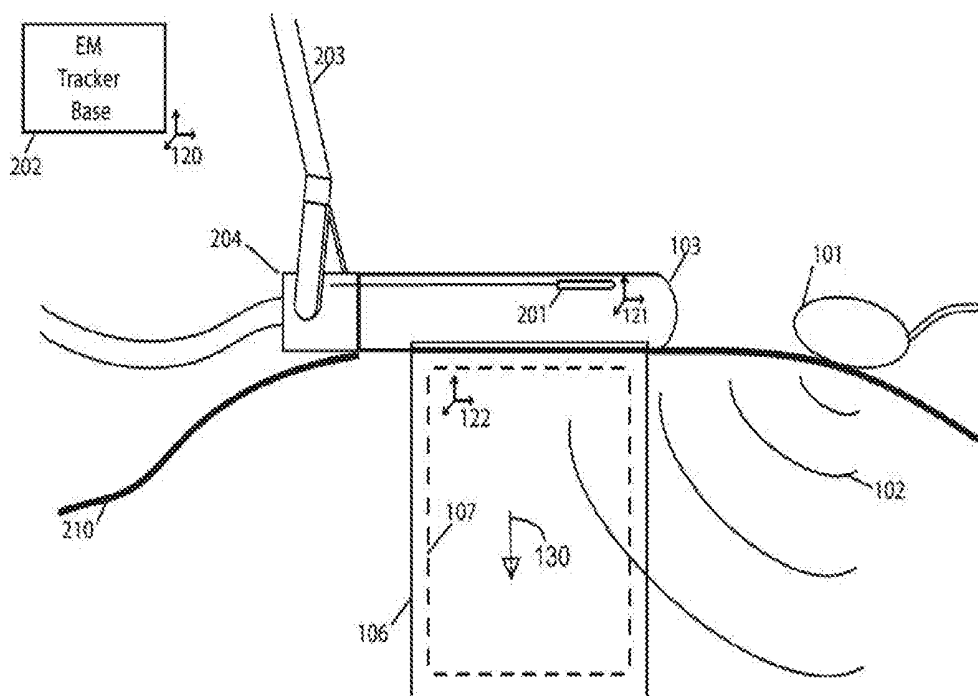


FIG 2

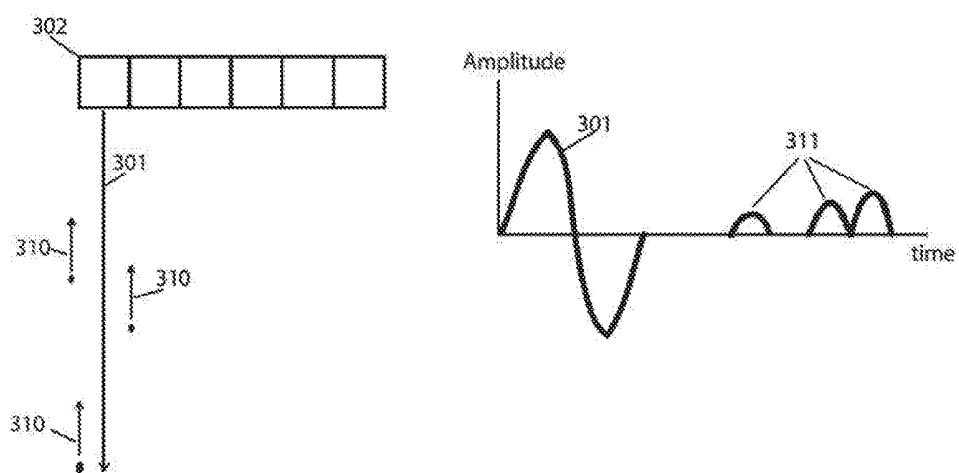


FIG 3

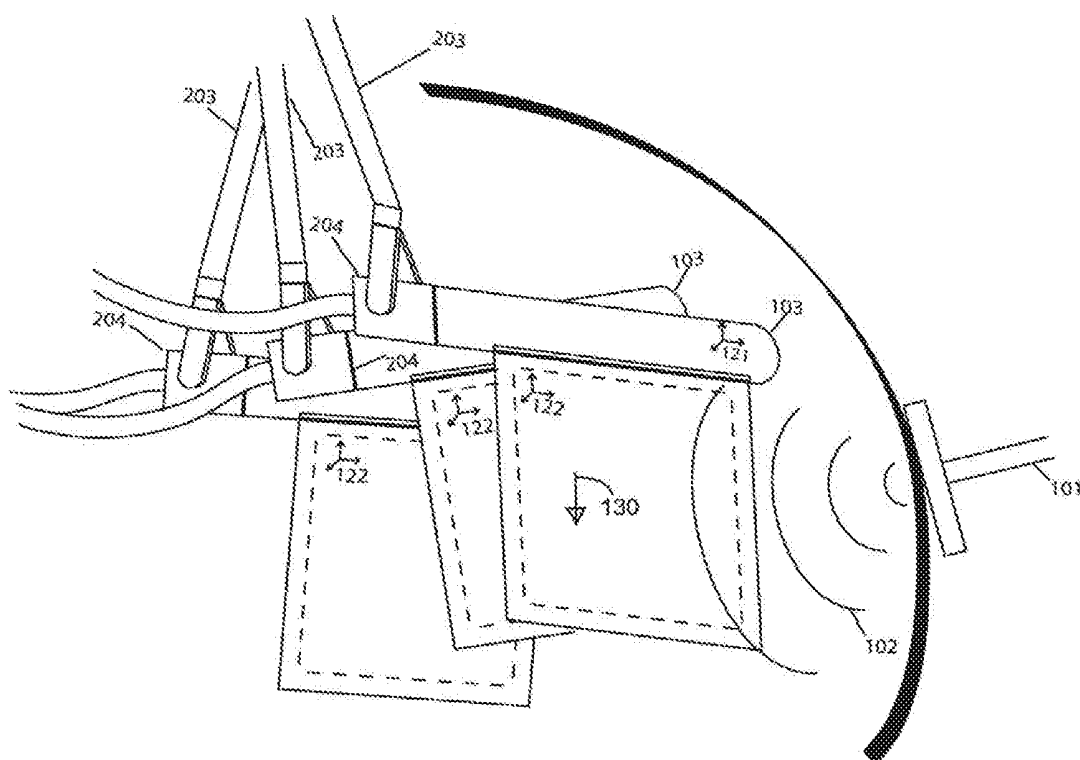


FIG 4

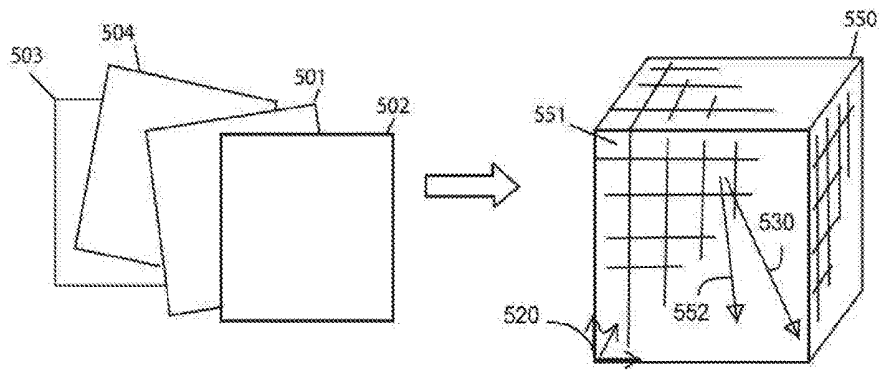
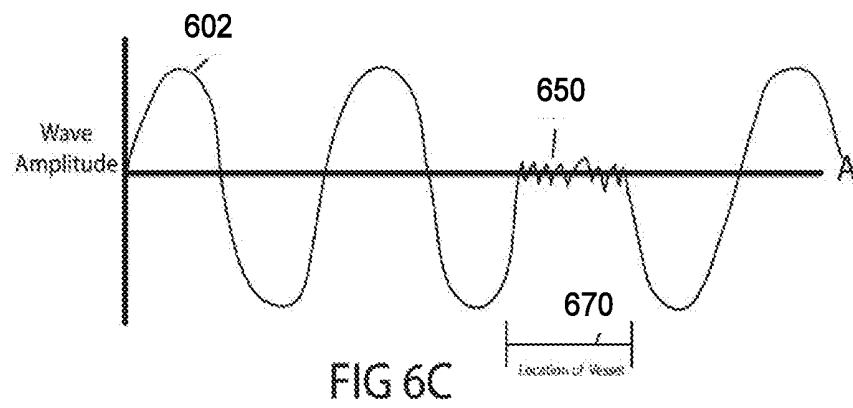
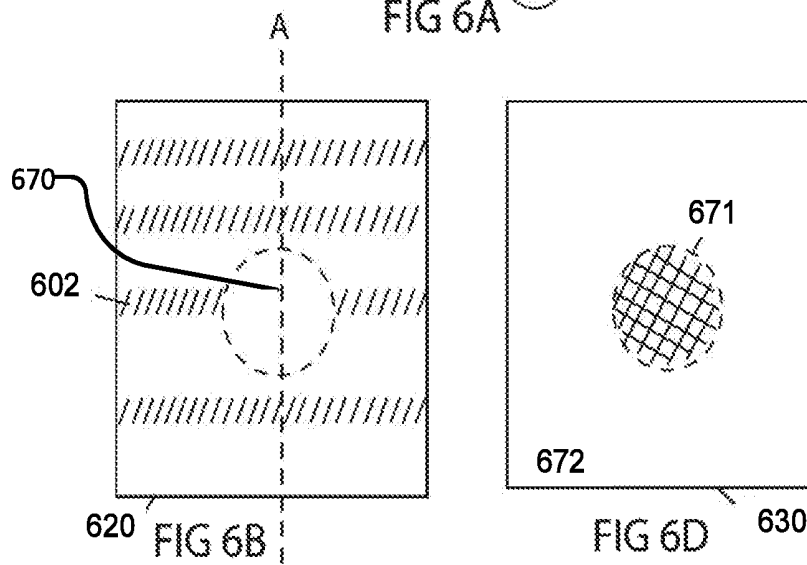
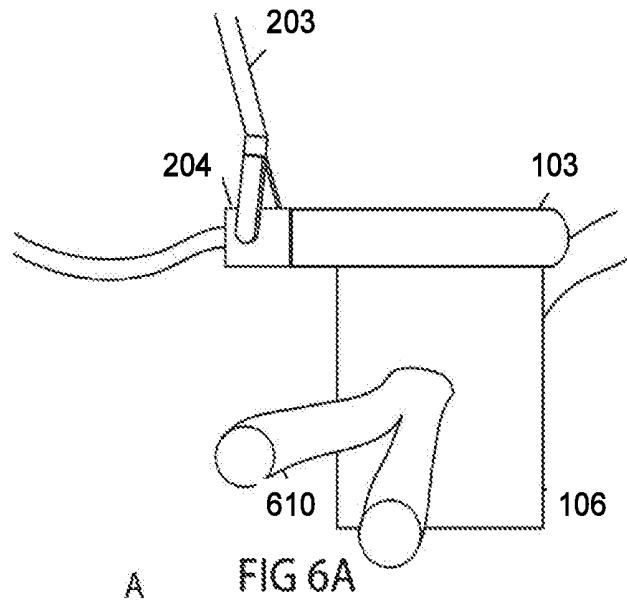
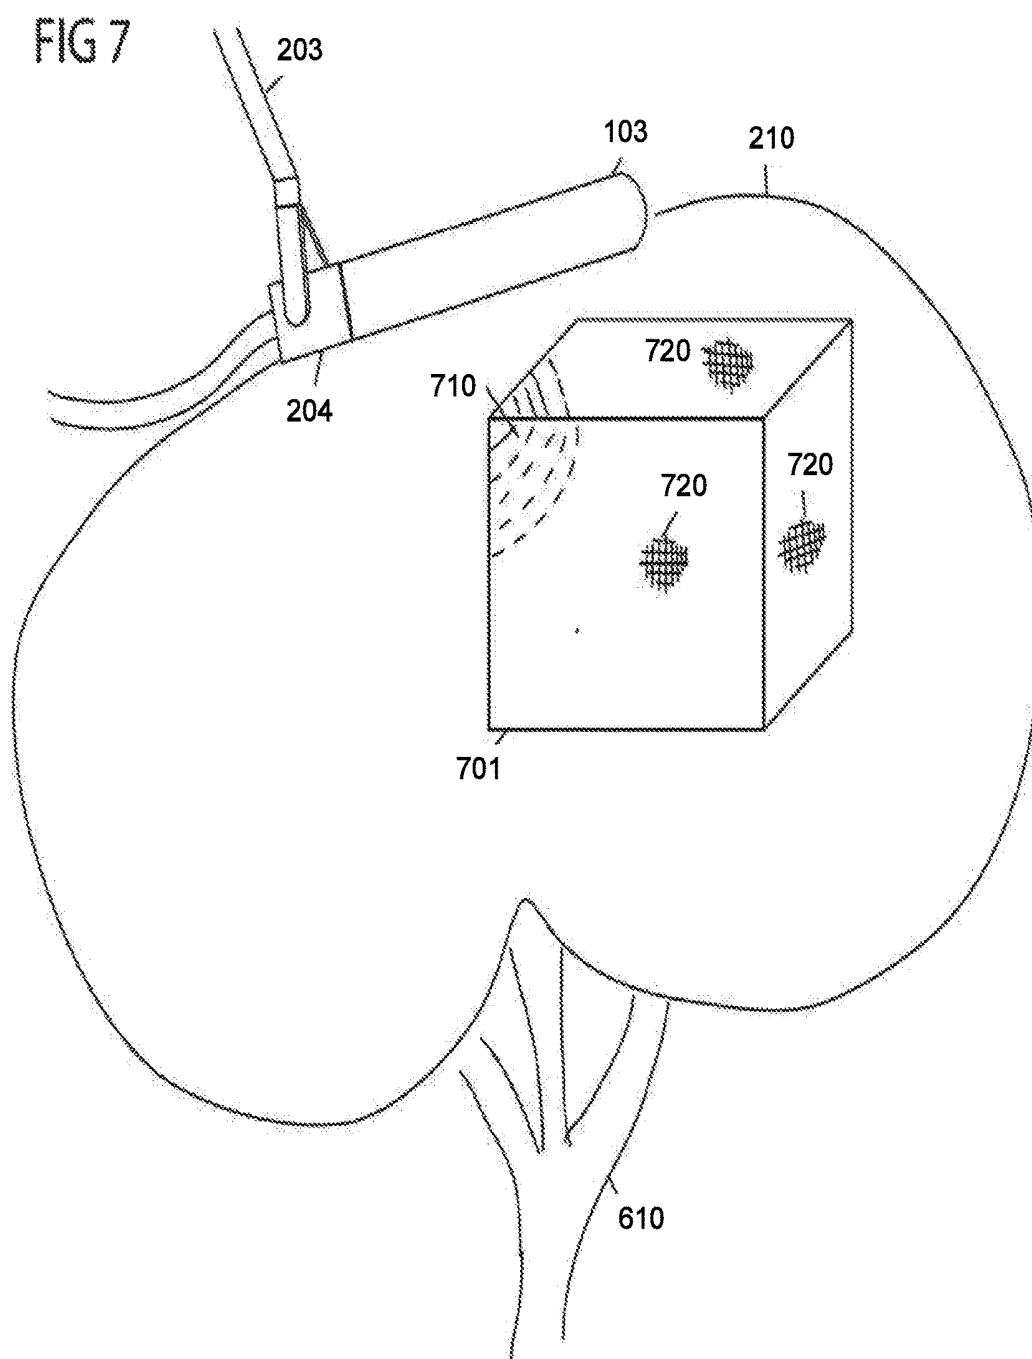
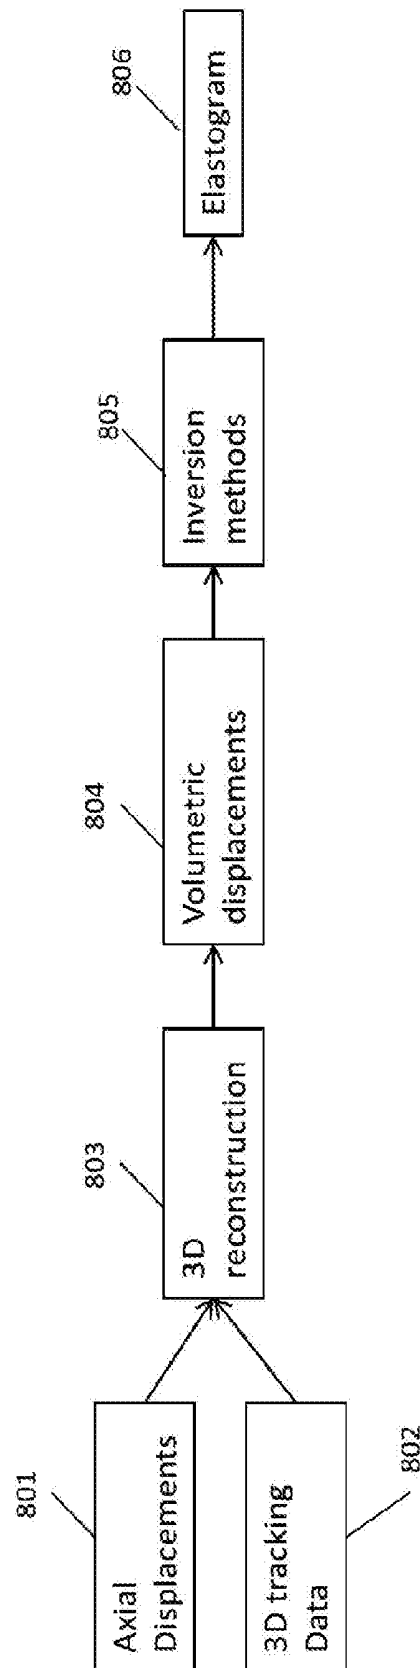


FIG 5





**FIG 8**

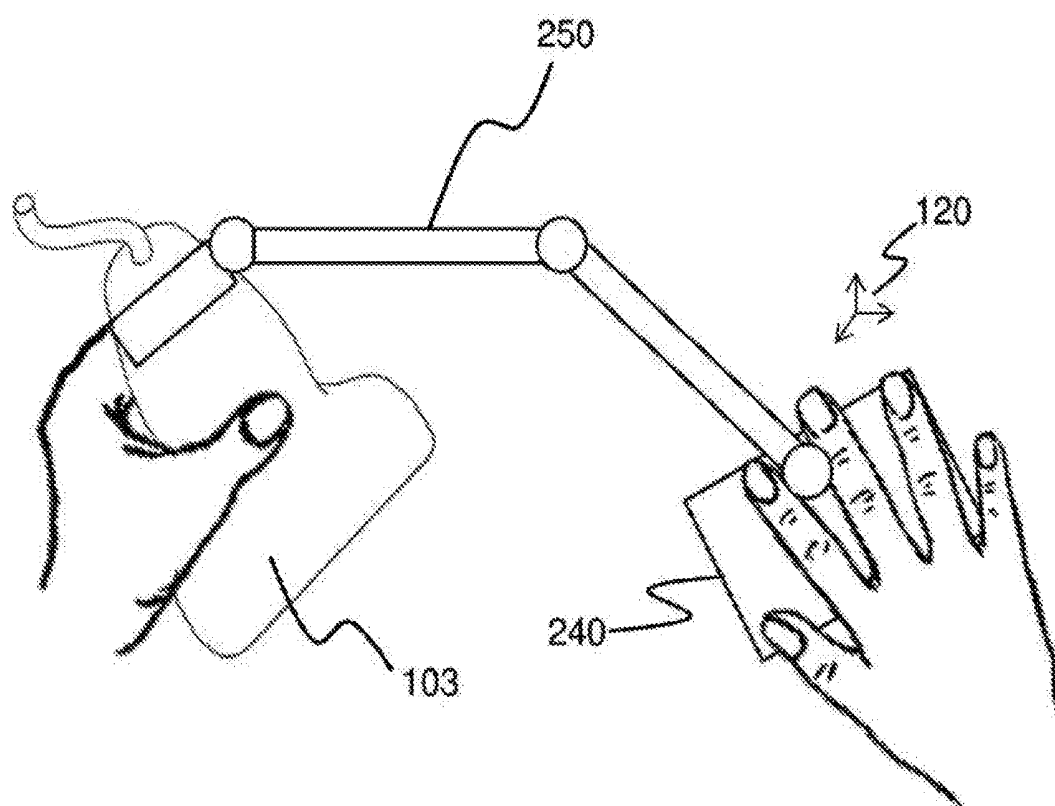


FIG 9

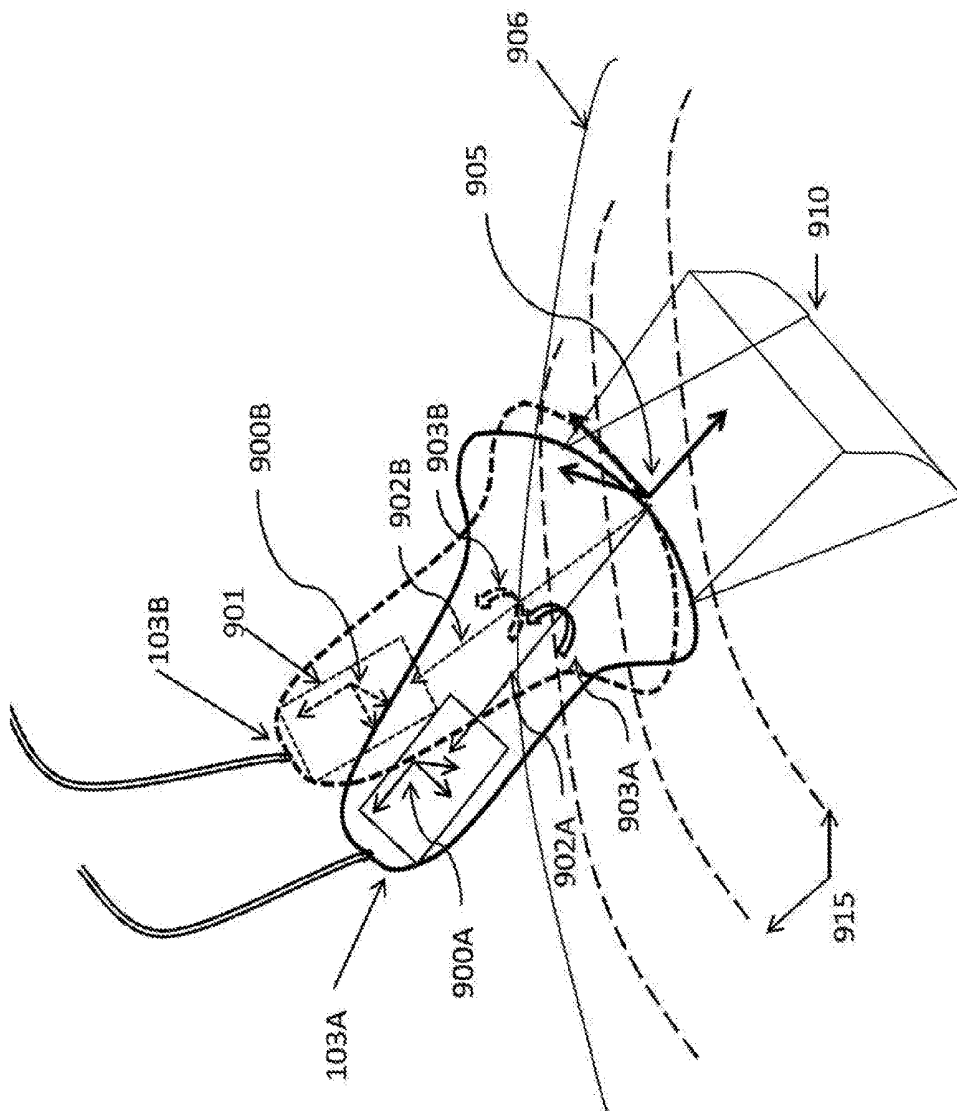


Fig. 10

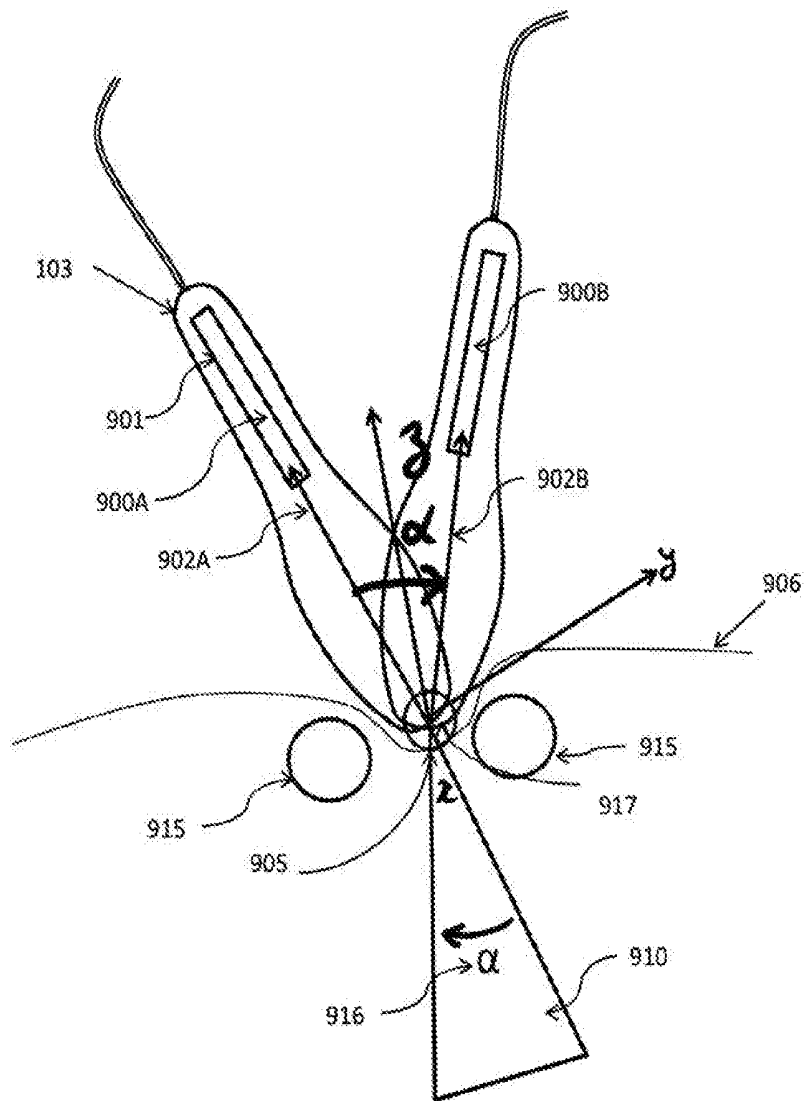
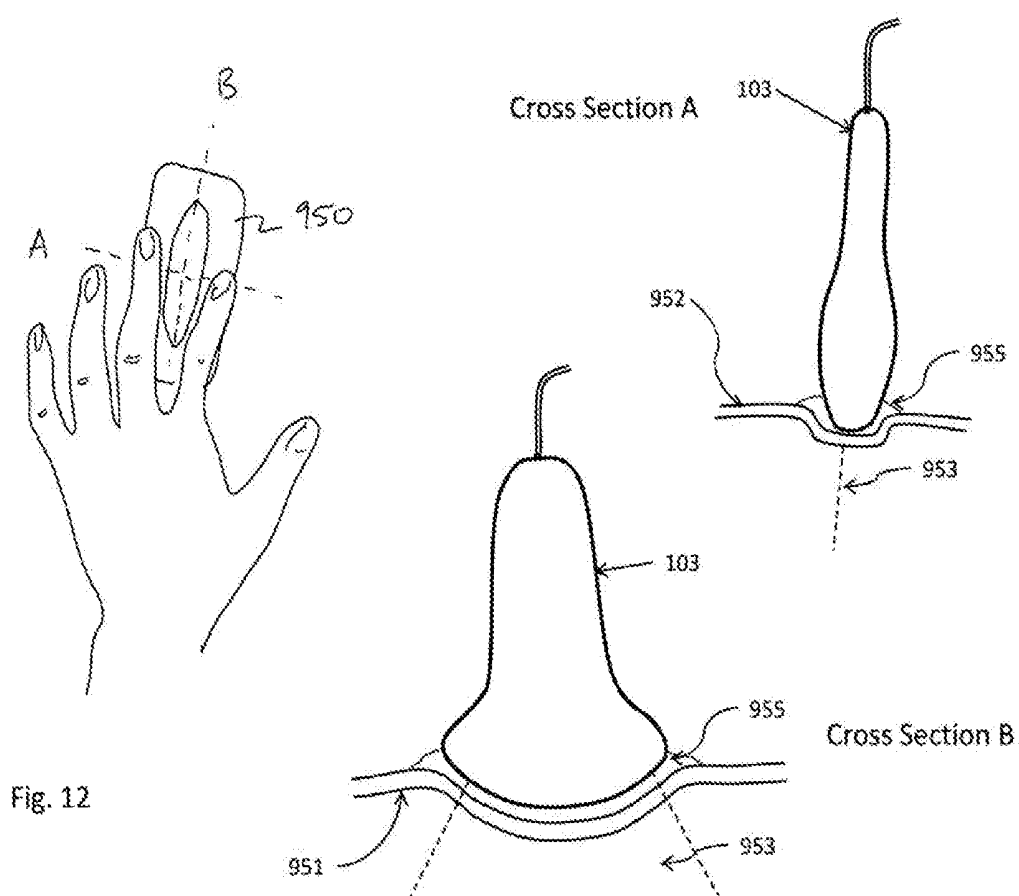


Fig. 11



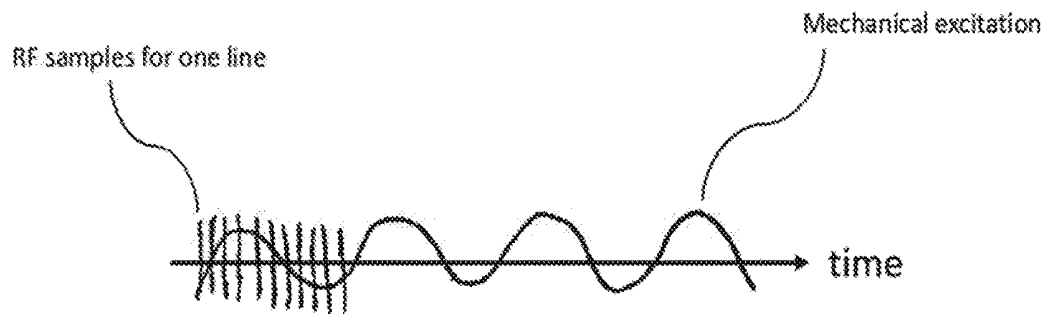


FIG 13a




FIG 13b

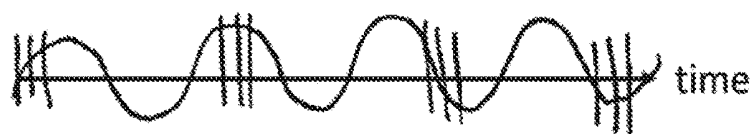


FIG 13c

QUANTITATIVE ELASTOGRAPHY WITH TRACKED 2D ULTRASOUND TRANSDUCERS

This application is a continuation-in-part of U.S. application Ser. No. 14/040,558 filed Sep. 27, 2013, which claims priority under 35 U.S.C. § 119(e) to a U.S. provisional application having Ser. No. 61/707,883, filed Sep. 28, 2012, the entirety of which is hereby incorporated herein by reference for all purposes.

FIELD OF THE INVENTION

This invention relates to medical imaging and, in particular, the measurement of mechanical properties of tissues, also known as elastography.

BACKGROUND OF THE INVENTION

Medical imaging is used in many applications to determine features of the composition of tissue not visible to the naked eye. The images can be displayed to a user, where the intensity or color of the image is a function of some parameter of the tissue composition. For example, computed tomography (CT) displays to the user the absorption of X-rays in the body and ultrasound displays the echo pattern produced in response to a pulsed sound wave. Of particular interest are the mechanical properties of tissue which can also be depicted in images. Changes in the mechanical properties of certain tissues can be an indication of disease. Traditional diagnostic methods have relied on the use of manual palpation to discriminate between healthy tissue and diseased regions because imaging methods were unavailable for detecting changes in mechanical properties. For example, the palpation of stiffer tissue is often the first step in the diagnosis of breast cancer and prostate cancer. A change in the mechanical properties of tissue can also be an indicator of the success or failure of therapy.

Elastography is a medical imaging technique that aims to depict elasticity, a mechanical property of tissue. Elasticity is also referred to as stiffness, or the inverse of compliance. Advanced elastography techniques can also measure the viscoelastic properties of tissue, such as viscosity and relaxation time. For this imaging technique, a mechanical excitation is applied in the proximity of the tissue of interest, such as prostate, breast, liver or any other soft organ in the body, and the resulting deformation is measured. The resulting deformation is measured with ultrasound (the method known as ultrasound elastography or USE) or Magnetic Resonance Imaging (the method known as magnetic resonance elastography or MRE). The deformation is post-processed to extract information such as viscoelastic properties (e.g., shear modulus and viscosity). The deformation or tissue strain, or alternatively, the intrinsic mechanical properties of tissue are then displayed as a map of stiffness (or other meaningful mechanical properties) of the imaged object.

Clinical uses of elastography were first demonstrated in the field of ultrasound as described in U.S. Pat. No. 5,107,837 by Ophir et. al. titled "Method and Apparatus for Measurement and Imaging of Tissue Compressibility and Compliance." Shortly afterwards elastography was introduced in the field of magnetic resonance imaging (MRI) by Ehman and Muthupillai as described in U.S. Pat. No. 5,825,186 titled "Method for Producing Stiffness-Weighted MR Images" and U.S. Pat. No. 5,977,770 by Ehman titled "MR Imaging of Synchronous Spin Motion and Strain

Waves." In the following years elastography was shown to be of clinical value for the detection and staging of hepatic (liver) fibrosis by Sinkus et. al. "Liver fibrosis: non-invasive assessment with MR elastography" in the Journal NMR in Biomedicine 2006, pages 173-179, and Ehman et. al. "Assessment of Hepatic Fibrosis With Magnetic Resonance Elastography" in the Journal of Clinical Gastroenterology and Hepatology, volume 5, Issue 10, October 2007, pages 1207-1213. Elastography imaging of the breast has been successfully demonstrated and published by Sinkus et. al. in "Viscoelastic shear properties of in vivo breast lesions measured by MR elastography" in the Journal of Magnetic Resonance Imaging volume 23, 2005, pages 159-165. Elastography of the brain was also published by Papazoglou and Braun et. al. in "Three-dimensional analysis of shear wave propagation observed by in vivo magnetic resonance elastography of the brain" in Acta Biomaterialia, volume 3, 2007, pages 127-137. More recently, elastography of the lung was demonstrated by Ehman et. al. In U.S. Pat. No. 2006/0264736 titled "Imaging Elastic Properties of the Lung with Magnetic Resonance Elastography". MRE of the prostate ex-vivo was demonstrated first by Dresner, Rossman and Ehman, published in the Proceedings of the International Society for Magnetic Resonance in Medicine titled "MR Elastography of the Prostate" in 1999. MRE of the prostate in-vivo was demonstrated by Sinkus et. al. and published in "In-Vivo Prostate Elastography", Proceedings of International Society of Magnetic Resonance in Medicine, volume 11, page 586, 2003. Prostate elastography was described in U.S. Pat. No. 5,952,828, 2010/0005892, 7,034,534 and the publications referred to above and also by Kemper, Sinkus et. al. "MR Elastography of the Prostate: Initial In-vivo Application." published in Fortschritte auf dem Gebiete der Röntgenstrahlen und der Nuklearmedizin (Advances in the area of X-ray and Nuclear Medicine), volume 176, pages 1094-1099, 2004. An alternative approach to prostate elastography used excitation applied through the rectum or the urethra as described in U.S. Pat. No. and 2009/0209847, 2010/0045289 and the following publication Plewes et. al. "In Vivo MR Elastography of the Prostate Gland Using a Transurethral Actuator" Magnetic Resonance in Medicine, volume 62, 2009, pages 665-671. Alternatively, the mechanical excitation can be applied by a needle that penetrates the skin as described in U.S. Pat. No. 2008/0255444.

Quantitative elastography is an advanced elastography technique that solves an inverse problem: calculating the stiffness maps in a region of interest given excitation of the tissue and measurement of resulting motion in that region. Inverse problems are better solved over a 3D (volumetric) than a 2D (cross-sectional planar) region of interest, for example with 3D MRI and 3D ultrasound. This is because knowledge of the tissue motion over a 3D region of interest allows a more complete tissue motion model (e.g. 3D wave equation) to be used. Waves can propagate in arbitrary directions so an inverse algorithm should have 3D data in order to properly compute the wave speed, or spatial wavelength, from which the shear modulus is derived.

It should be clear that the mechanical waves induced by external exciters in most of the previous mentioned techniques vary in both space and time. An ideal measurement system would measure all three components (x,y,z) of the displacements instantaneously over a volume of interest, such that a 3D vector field of 3D displacements can be obtained at many instances in time. Such measurements would form a mathematically complete representation of the wave propagation. However, such ideal measurements sys-

tems are currently infeasible, so most previous mentioned works exploit the steady state nature of the wave propagation to build up a representation through multiple measurements over several periods of the waves. This is achieved usually by synchronizing acquisition with the exciter that is creating the waves and assuming perfect periodicity in the excitations. MR imaging is a relatively slow imaging modality, so MR elastography typically requires many minutes of acquisition time. The main advantage is that MR elastography creates high quality quantitative images of the mechanical properties of tissue that are considered the gold standard in the field of elastography. Ultrasound holds promise for faster acquisition yet it poses other challenges to overcome due to the pulse-echo nature of data acquisition and need for multiple pulses, which introduce time delays from both time of flight of the pulses and the delays between pulses. More challenges arise from the desire to acquire data over a 3D volume of interest when using a conventional ultrasound transducer that acquires data from a single 2D cross-sectional plane for a given position of the transducer. It is possible to move a conventional ultrasound transducer over a volume of interest in a freehand fashion, but the set of pulse-echo data will not in general be at equally spaced spatial and temporal locations. This makes it more challenging to use conventional inversion methods to calculate the mechanical properties of tissue from the acquired measurements. There exist methods to interpolate irregularly spaced pulse-echo data of stationary tissue into a regularly spaced volume (see Rohling et al. "Comparison of freehand three-dimensional ultrasound reconstruction techniques" in Medical Image Analysis, 1999), but there are no previous reports of also accommodating the time delays for each pulse-echo step when measuring the displacements of moving tissue. It would be beneficial to invent a method that produces the high quality results of MR elastography with a freehand motion of a conventional ultrasound transducer over a volume of interest, despite the irregular spacing of ultrasound compared to MRI.

Tissue motion, as captured by an ultrasound transducer, usually represents the motion in the axial direction with respect to the ultrasound transducer. The axial direction is defined as the direction of the sound pulse created by the transducer array. The lateral direction is defined in a 2D cross-sectional plane as along the direction of the transducer array, while the elevational direction is defined as orthogonal to the 2D cross-sectional plane. The resolution of an ultrasound image is generally highest in the axial direction and lowest in the elevational direction, so tissue motion in the axial direction is measured with the highest accuracy.

In U.S. Pat. Application No 2012/000779, by A. Baghani et al., "Elastography using ultrasound imaging of a thin volume", the entirety of which is hereby incorporated by reference, a method is presented to acquire volumetric quantitative elastography images using either matrix arrays that can electronically steer a planar beam to form a 3D volume, such as the xMATRIX ultrasound transducer (Philips Healthcare, Andover, Mass.), or using mechanically swept linear ultrasound imaging transducers, such as the 4DL14-5/38 Linear 4D ultrasound transducer (Ultrasonix Medical Corporation, Richmond, BC), that move the imaging plane in the elevational direction in order to acquire a volumetric image. In U.S. Pat. Application No 2012/000779, the sweeping motion of the mechanically swept ultrasound transducers is synchronized with the known frequency of the tissue motion in order to generate a set of tissue displacement estimates that are regularly spaced in time and space. As described in U.S. Pat. Application No. 2012/000779,

these displacement estimates can be used to compute elasticity images using techniques known in the art, such as the local spatial frequency estimator.

However, the majority of transducers used with commercial ultrasound machines create only 2D images, so it would be beneficial to extend the benefits of solutions of 3D inverse problems to machines that acquire 2D images.

A standard 2D ultrasound machine can be used to acquire 3D measurements by adding a position tracker to the transducer and then moving the transducer over a 3D region or volume of interest while acquiring ultrasound images—each tagged with one or more position tracker measurements. If the position tracker provides both position and orientation, we will call the joint set of positions and orientations a "location", as commonly done in the robotics literature. A minimum of six numbers is needed to specify the location of an object in space. In this way, the ultrasound image data is acquired at different temporal and spatial locations. This set of ultrasound data is 3D and can be conceptualized by the analogy to stacking a deck of cards, where each card is a 2D ultrasound image. However, since the ultrasound transducer is moved by hand, the set of images will lie on irregularly spaced parallel cross-sections. What is needed is a novel method and system to use the set of tracked ultrasound data in an inverse technique to obtain quantitative elastography.

Previous work such as that performed by Lindop et al ("3D elastography using freehand ultrasound," Ultrasound in Medicine and Biology, 32(4), 2006) demonstrates the ability to create 3D strain volumes using a freehand scanning technique. Unlike the method described in this invention that solves an inverse problem to produce quantitative elastography images, Lindop et al, have created a method using only axial strain imaging. A 2D ultrasound transducer is tracked in 3D space using an active optical tracker. As the transducer is moved, a series of cross-sectional planes are acquired. Each plane is spaced approximately 0.1 mm from its neighbors. They assume that the de-correlation between cross-sectional planes is small and that the small changes in pressure due to the user's motion will cause enough strain to create an elastogram. The strains are calculated using cross-correlation techniques to track the tissue deformation in the axial direction using the radio frequency ultrasound data. However, the Lindop et al. method does not provide the quantitative mechanical properties of tissue, but instead, provides the relative strain. The image quality provided with that method can also be compromised by the accumulation of de-correlation due to involuntary motion of the user in all five degrees of freedom that violate the assumptions of only axial compression of tissue. Considerable correction techniques should be applied after the original cross-correlation in order to create an interpretable image. It is also only capable of measuring the static mechanical properties, not the dynamic properties that require measurements over time. Such dynamic techniques are typically based on observing wave motion in tissue.

It is often the case that the frequency of tissue motion exceeds the imaging speed of commercially available ultrasound machines. Vibration frequencies can range from 10 to 300 Hz, while most commercial ultrasound machines produce images at approximately 40 Hz, depending on the depth of imaging. In order to overcome this drawback, two main methods have been developed. The first method uses techniques to speed up the effective frame rate. These techniques could include sector based imaging as described by Baghani et al ("A high-frame-rate ultrasound system for the study of tissue motions", IEEE Ultrasonics, Ferroelectrics and Frequency Control. 57(7), 1535-1547 (2010)).

Another technique involves careful selection of imaging frame rates and vibration frequencies and is described by Eskandari et al ("Bandpass sampling of high frequency tissue motion", IEEE Transactions on Ultrasonics, Ferro-electrics and Frequency Control, 58(7), 2011).

A key application of elastography is surgery where elastograms can guide surgery. The prevalence of minimally invasive surgery, where a surgeon could find benefit from elastogram guidance, is growing. This type of surgery involves the surgeon using long instruments through small holes in the patient's skins. The difficulty of using these instruments to complete complicated procedures led to the development of robotic laparoscopic surgery. In particular, Intuitive Surgical Inc. has commercialized the da Vinci™ Surgical system. This surgical robot gives the surgeon 6 degrees of freedom of the position and orientation of the end effector of the tool. This system incorporates a stereo laparoscope, allowing the surgeon to view the surgical scene in 3D. Some embodiments of the invention take advantage of both the dexterity and stereo vision systems of this robot to move and track an ultrasound transducer.

The invention disclosed herein uses a steady-state or periodic excitation to create dynamic motion within a tissue. A tracked 2D ultrasound transducer is used to image the volumetric tissue displacements to create a volume of the mechanical properties of the tissue in real-time without disrupting the natural motion of scanning used by the physician. Tracking of the ultrasound transducer can be achieved, for example, by embedding a magnetic sensor, an inertial measurement unit, or one or several cameras for localization inside the transducer. Note that the scanning motion is described here as arising from the physician's hand, but it could also arise from a robot, where the robot is either moved automatically or controlled by a human operator.

SUMMARY OF INVENTION

One aspect provides a method for measuring the mechanical properties in a volume of tissue. The method comprises applying an excitation to the volume of tissue with a vibration source. In some embodiments an internal excitation is applied to the volume of tissue with a vibration source. The method also comprises scanning the volume of tissue with a tracked ultrasound transducer, measuring the tracked ultrasound transducer locations relative to a base coordinate system, computing a tissue response relative to the tracked ultrasound transducer from echo data measured by the tracked ultrasound transducer, converting the tissue response from the tracked ultrasound transducer coordinate system to the base coordinate system using the tracked ultrasound transducer locations, and calculating the mechanical properties in the volume of tissue from the tissue response in the base coordinate systems. Changing of the coordinate system of the tissue response to the base coordinate system comprises a phase compensation for time delays for one or both of (i) time of flight of ultrasound pulses, and (ii) time delays between subsequent ultrasound pulses. The tissue response comprises one or more of tissue velocities and tissue displacements.

The location of the tracked ultrasound transducer may comprise one or more of a position and an orientation of the transducer. The location may be determined using one or more of: electromagnetic sensing, passive or active optical sensing, robot sensing, sensing by an inertial measurement unit (IMU), and a mechanical linkage between the tracked ultrasound transducer and a tracking base. The location

and/or one or more degrees of freedom of the ultrasound transducer may be constrained by a constraining fixture or linkage.

The location of the tracked ultrasound transducer may be determined based on ultrasound transducer image-based motion estimation. A correlation-based algorithm or a machine learning-based algorithm may be applied to determine the transducer motion within each imaging plane or within and outside each imaging plane, from ultrasound echo data.

In some embodiments, the vibration source is placed on the skin of a patient. In some embodiments, the ultrasound transducer is placed on the skin of a patient. In other embodiments, the ultrasound transducer is placed inside a patient and directly adjacent to an area or organ of interest.

BRIEF DESCRIPTION OF THE FIGURES

FIG. 1: Set-up of embodiment using an external transducer and excitation.

FIG. 2: Embodiment using an intra-operative transducer and internal excitation.

FIG. 3: Description of ultrasound imaging.

FIG. 4: Set-up of the intra-operative ultrasound transducer in motion.

FIG. 5: Shows the reconstruction of multiple ultrasound data acquisition planes into a 3D volume.

FIGS. 6A, 6B, 6C and 6D: Illustrate how vessels can be imaged with elastography.

FIG. 7: Shows a surgical scene including one embodiment of the invention.

FIG. 8: Describes the overall work flow of the processing in this invention.

FIG. 9: Shows tracking using a mechanical arm according to one embodiment.

FIG. 10: Describes volume acquisition using an Inertial Measurement Unit.

FIG. 11: Shows detail of volume acquisition when the ultrasound transducer is constrained to rotate about a particular axis as may be the case when imaging the liver through the ribs.

FIG. 12: Shows detail of volume acquisition with a stabilizer plate.

FIG. 13a illustrates a sector based method in which a tissue displacement is sampled for a short time at a high rate.

FIG. 13b illustrates bandpass sampling in which tissue displacement samples are collected at a lower frame rate.

FIG. 13c illustrates a combined method in which sector samples are collected at a high pulse repetition frequency and groups are repeated at a lower rate.

DESCRIPTION OF THE INVENTION

Detailed descriptions of embodiment of the invention are provided herein. It is to be understood, however, that the present invention may be embodied in various forms. Therefore, the specific details disclosed herein are not to be interpreted as limiting, but rather as a representative basis for teaching one skilled in the art how to employ the present invention in virtually any detailed system, structure, or manner. The descriptions of the embodiment of the invention will be made in the publication by Caitlin Schneider, Ali Baghani, Robert Rohling, Septimiu E. Salcudean titled "Remote Ultrasound Palpation for Robotic Interventions using Absolute Elastography", presented at the 15th International Conference on Medical Image Computing and Computer Assisted Intervention, Oct. 2, 2012, Springer

LNCS 7510, pp. 42-49, the entirety of which is hereby incorporated herein by reference.

According to one aspect of the invention, there is provided a system for imaging the mechanical properties of tissue. The system comprises:

- a) A 2D ultrasound transducer with a linear or curvilinear ultrasound array;
- b) A tracker to measure the position and orientation of the ultrasound transducer;
- c) A mechanical exciter to induce waves in the tissue;
- d) Electronic circuits with inputs of ultrasound echo data and their corresponding 3D position tracker measurements, and outputs for the mechanical exciter, and for the ultrasound transducer pulse transmits;
- e) Software programs that control the mechanical exciter and ultrasound transmits, calculate the delays between exciter and ultrasound echo data, and calculate one or more mechanical properties of the tissue based on the set of ultrasound echo data and 3D position tracker measurements;
- f) Monitor to display to the operator the calculated mechanical properties of tissue over the region of interest.

The ultrasound transducer in this system is non-specific and the system is designed in such a way that any type of ultrasound transducer can be used. In some embodiments of the invention, the ultrasound transducer could have a linear ultrasound transducer array. In some embodiments of the invention, the ultrasound transducer could have a curvilinear ultrasound transducer array. In yet another embodiment, the ultrasound transducer can have a matrix transducer array, exemplified by the xMatrix™. For all types of ultrasound transducers, the geometry of the transducer array is known from the manufacturer's specifications and remains constant. This geometry is needed to calculate the spatial location of each pulse-echo beam that is produced relative to each other and the tracker coordinate frame.

We will describe the invention using the embodiment with a transducer having a linear array transducer for the purpose of clarity but not limiting the invention to this particular type of transducer.

The transducer will be tracked through 3D space. This system can be used with any of multiple types of tracking systems. In some embodiments an electromagnetic ("EM") tracker known in the art, such as those manufactured by Ascension Technology Corporation can be used, in which case the EM sensor is permanently or semi-permanently attached to the ultrasound transducer. In other embodiments of the invention, tracking could be performed using optical tracking, with active markers, as exemplified by the Certus™ optical tracking system (Northern Digital Instruments), or passive markers, as exemplified by the Micron-Tracker™ (Claron Technology Inc.), or by using feature tracking in stereo or mono camera images, through known techniques in the field of image processing, or using robotic kinematics when the transducer is manipulated by a robot. Through calibration techniques (Mercier, et al., "A review of calibration techniques for freehand 3-D ultrasound systems", *Ultrasound in Medicine & Biology* 31(2), 143-165 (2005)) the position and orientation of the sensor can be related to the position and orientation of the ultrasound imaging crystals and thus an ultrasound image can be recorded at a measured location (position and orientation) in 3D space.

In some embodiments, tracking is performed using an Inertial Measurement Unit (IMU). The IMU may comprise accelerometers, gyroscopes, and/or magnetometers to track

the ultrasound transducer. IMUs are available in compact packages from multiple vendors—for example, Bosch Sensortec BMF055 9 Axis Motion Sensor, or STM Microelectronics iNEMO LSM9DS1. Such sensors can be used to track either orientation or orientation and position. Typically, IMUs provide more accurate orientation measurements than position measurements, which have more drift.

FIG. 10 shows an example in which only the transducer orientation obtained from the IMU is used to generate an ultrasound volume. In this embodiment, the ultrasound transducer 103 (held by an operator whose hand is not shown) is shown at two different orientations relative to a coordinate system 905 affixed to the patient's body 906. As the transducer is moved from an initial orientation 900A, to a new orientation 900B, the IMU 901 captures the orientation of the transducer—its axial direction 902, varying from 902A to 902B, and its twist about this axial direction 903, varying from 903A through 903B. Assuming that the transducer face is constrained by the operator's hand, and by natural body features, such as the ribs 915 which form a "ridge" around the transducer face, the range of orientations provided by the IMU and the associated ultrasound image frames can be used to construct an ultrasound volume 910. A different view of the transducer is shown in FIG. 11, where it is assumed that the transducer has its face 917 constrained by the ribs 915 to move about the x-axis of the coordinate system 905. As the transducer rotates through an angle α shown at 916 and between the ultrasound transducer axes 902A and 902B, a sector volume of images 910 over the angle α is acquired.

To stabilize the transducer face position on the patient to allow a volume acquisition through transducer rotation only, an acoustically transparent fixture filled with gel could be used. Such a fixture is shown in FIG. 12, labeled as 950, with cross-sections A shown as 952 and B shown as 951. As the ultrasound operator pushes the ultrasound transducer against the plate 950, the curvatures of the plate shown at 951 and 952 will stabilize the position of the ultrasound transducer as a function of the transducer orientation. The coupling gel allows the ultrasound plane 953 to penetrate through the acoustically transparent plate 950.

Alternatively, in some embodiments, tracking may be performed by coupling a mechanical arm or linkage between the ultrasound transducer and the tracking base unit, and detecting movements in the mechanical arm or linkage, as described in FIG. 9.

Particular embodiments may use the ultrasound image itself to track the locations and orientations of the ultrasound transducer. For example, ultrasound transducer image-based motion estimation may be used. This may comprise determining from the ultrasound echo data the transducer motion within each imaging plane (and in some cases, also outside each imaging plane) using a correlation-based, machine learning-based or other type of algorithm. See, for example, "Nonlocal means filter-based speckle tracking", Afsham, Rasoulzian, Najafi, Abolmaesumi, Rohling. *IEEE Trans. Ultrasonics, Ferroelectrics and Frequency Control*, 62(8), 2015, pp. 1501-1515 for a correlation-based algorithm that may be used for tracking. See, for example, "Deep Learning for Sensorless 3D Freehand Ultrasound Imaging", Prevost, Salehi, Sprung, Bauer, Wein, *Medical Image Computing and Computer Assisted Intervention*, 2017, pp. 628-636 for a machine learning-based algorithm that may be used for tracking. In particular embodiments, one or more of the above-described tracking methods (e.g. electromagnetic, passive or active optical sensing, robot sensing, inertial measurement unit sensing, or mechanical linkages) may be

used in combination with the ultrasound transducer image-based motion estimation to track the locations and orientations of the ultrasound transducer.

The mechanical exciter should produce vibrations up to a few hundred hertz to measure the elasticity of organs such as the liver, the kidney, and the prostate. For stiffer or smaller organs such as the skin, the frequency of actuation may be higher, up to a couple of kilohertz. The mechanical exciter can be a voice coil actuator as used in speakers or disk drives; it could also be a piezo actuator for higher frequencies; it could also be a conventional motor with an asymmetrical inertial load that may generate vibrations in the same way a cell phone vibrator does. The amplitude and frequency can be controlled through computer software. In some embodiments of the invention, the vibration source can be placed on the patient's skin near the area or organ of interest, whereas in other embodiments of the inventions, the vibration source can be placed inside the patient, directly on the area or organ of interest.

The vibration source will create steady-state dynamic waves in the tissue. Using previously described techniques for high speed/high frame rate ultrasound imaging of tissue motion, the axial displacements of the tissue are tracked. Since the transducer is moving during the data acquisition process, the imaging transmit sequence is synchronized to the excitation such that the tissue displacements will be tracked in 3D space and the temporal delays will be calculated and compensated for in order to create a volumetric dataset of the tissue displacements over specific instances in time. From this dataset, the mechanical properties of the tissue, such as elasticity and viscosity are calculated.

Tissue displacements may be converted from the coordinate system of a tracked ultrasound transducer to a base coordinate system. Converting the displacements from the coordinate system of the tracked ultrasound transducer to the base coordinate system may comprise applying phase compensation for time of flight of ultrasound pulses. Converting the displacements from the coordinate system of the tracked ultrasound transducer to the base coordinate system may comprise applying phase compensation for time delays between subsequent ultrasound pulses.

In addition to the measured tissue displacement, a lack of coherent motion can also give insight into the tissue makeup. Because water and low viscosity fluids like blood do not support shear waves (the type of waves that are causing tissue displacement) the lack of coherent motion is also an indicator to the tissue structure. Structures like vessels can therefore be identified inside organs such as the liver and kidney, and cystic lesions can be differentiated from solid tumours.

In summary, the invention has a number of aspects including, without limitation, the following aspects:

A method to measure the mechanical properties of a volume of tissue, the method comprising applying an excitation to the volume of tissue using a vibration source, scanning the volume with a tracked ultrasound transducer, measuring the location of the tracked ultrasound transducer, measuring tissue displacements with respect to the ultrasound transducer from the radiofrequency (RF) transducer echo data, converting these measured displacements to a base coordinate system, and calculating mechanical properties of tissue from the volumetric set of displacements in the base coordinate system.

In some embodiments of the invention, methods of interpolating non-uniform displacement measurements in space

are used to create a volumetric datasets of tissue displacements that are uniformly spaced with respect to a base coordinate system.

In some embodiments of the invention, the excitation generated by the vibration source is steady-state.

In some embodiments of the invention, a variety of tracking systems could be used to measure the location of the tracked ultrasound transducer. These tracking systems include but are not limited to, a passive or active optical tracking system, an electromagnetic tracking system or robot kinematics.

In various embodiments of the invention, the vibration source can be placed either on the patient's skin or internally in the patient on the surface of the organ to be imaged.

In various embodiments of the invention, the ultrasound transducer could either be placed on the patient's skin or placed inside the patient and directly adjacent to the area or organ of interest.

In various embodiments of the invention, the coherence of the tissue displacements with respect to a displacement reference such as the vibration source, the motion of a tissue feature or the spatial average motion of a tissue region is computed and used to determine whether the tissue at a specific location is a fluid, such as a blood vessel or a fluid-filled cyst.

In another embodiment of the invention, the reconstruction of the volumetric dataset includes phase compensation for the time of flight of ultrasound pulses.

In another embodiment of the invention, the reconstruction of the volumetric dataset includes phase compensation for the time delays between subsequent ultrasound pulses.

In another embodiment of the invention, the tracked 2D ultrasound transducer moves in a discrete stepwise fashion wherein each step involves holding the transducer stationary while acquiring tissue displacements from a cross-sectional plane of the volume of interest, and then moving the transducer to an adjacent location, and then repeating.

In another embodiment of the invention, the tracked 2D ultrasound transducer moves in a continuous fashion wherein the transducer is moved without stopping over the volume of interest.

The calculated quantitative mechanical property may be one of, but is not limited to, one of the following: the shear modulus of the tissue, the elasticity of the tissue, the shear wave speed of the tissue, or the shear viscosity of the tissue. The mechanical property calculated using this invention can also include the frequency dependency of a mechanical property, such as those listed above.

FIG. 1 shows apparatus according to one embodiment of the invention. In this embodiment, the ultrasound transducer **103** is being held by the user **105** against the patient's skin **108**. An external exciter **101** is used as a vibration source for elastography imaging. The waves **102** created by the external exciter **101**, propagate through the tissue. The tissue motion caused by these waves **102** is imaged by the ultrasound transducer **103** within the region of interest **107** of the ultrasound image **106**. The region of interest **107** will also be called the volume of interest to stress that we are interested in imaging over a volume. As described in the references enclosed therein and known in the state of the art, these motions are measured by repeated capturing of ultrasound pulse-echo data and computing localized delays between such repeated echo data sets using a variety of techniques such as cross-correlation maximization.

The ultrasound transducer **103** in this embodiment is tracked using an optical tracker **109**. The optical tracker can be either a passive tracker, using distinctively shaped mark-

ers **104** attached to the ultrasound transducer **103**. These markers are detected using computer vision techniques. In some embodiments, the markers could be active markers. Active markers emit some type of signal such as coded infrared light pulses that are detected by the optical tracker base station **109**.

The transformation between the optical marker **104** and the ultrasound image **106** can be calibrated using techniques such as those described in Mercier et. al ("A review of calibration techniques for freehand 3-D ultrasound systems", *Ultrasound in Medicine & Biology* 31(2), 143-165 (2005)) giving a single transformation (T_p) from the marker coordinate frame **121** to the image coordinate frame **122**. The time delay between measurements of the marker position and ultrasound data acquisition, including any lag in either the tracker or ultrasound system, can also be calibrated by one of the techniques described in Mercier et. al.

Markers **104** define the ultrasound transducer's **103** position in space with respect to the coordinate frame **120** of the optical tracker base station **109** as a transformation (T_{ot}). Thus the position of the ultrasound image **106** and any feature within it can be located in space using a chain of transformations (T_{ot})*(T_p), determining the image position with respect to the optical tracker **109**.

In other embodiments, internal excitation may be used. For example, FIG. 2 shows one embodiment of the invention incorporating internal excitation. In this embodiment of the invention the ultrasound transducer **103** is a modified laparoscopic transducer, described in detail in C. Schneider et al, ("Intra-operative "Pick-Up" Ultrasound for Robot Assisted Surgery with Vessel Extraction and Registration: A Feasibility Study", IPCAI 2011, and U.S. patent application Ser. No. 13/525,183, now U.S. Pat. No. 9,155,520). This transducer **103** is designed to be used inside the patient's body and placed directly onto the organ or tissue of interest **210**. In this embodiment of the invention, the transducer **103** can be picked up and manoeuvred by a robotic tool **203** controlled by the surgeon. The tool **203** picks up the ultrasound transducer **103** by a specially designed tool/transducer interface **204**. The control of the ultrasound transducer **103** by the surgeon can either be direct or through tele-operation. In this embodiment, an internal exciter **101** is used to create waves **102** in the tissue. The exciter **101** is placed on or near the organ of interest **210** while ultrasound scans are taking place.

In the embodiment demonstrated by FIG. 2, tracking with respect to a base coordinate system can be completed using an electromagnetic (EM) tracking system, as described in C. Schneider et al, ("Intra-operative "Pick-Up" Ultrasound for Robot Assisted Surgery with Vessel Extraction and Registration: A Feasibility Study", IPCAI 2011 and U.S. patent application Ser. No. 13/525,183). With this type of tracking, an EM sensor **201** is embedded inside the ultrasound transducer **103**. The EM Tracker base **202** is placed outside the patient's body and the position of the ultrasound transducer **103** with respect to the EM transmitter **202** can be measured. Tracking takes place similar to the method described above, where the position of the transducer **103** can be found through the combinations of the transformations between coordinate system **120** of the EM Tracker base **202** (the base coordinate system) and the coordinate system **121** of the sensor **201** and the transformation between the sensor coordinate system **121** and the coordinate system of the ultrasound image **122**.

By placing the ultrasound transducer **103**, the exciter **101** and the organ of interest **210** close together, higher mechani-

cal excitation frequencies can be achieved, because energy dissipation of the waves is less of an issue.

FIG. 3 describes the general principle of conventional ultrasound imaging. A sound pulse **301** is emitted from the piezoelectric crystals **302** that make up part of the ultrasound transducer. The sound energy **301** creates reflections **310** where it comes in contact with changes in acoustic impedance. These reflections **310** reflect back to the crystals **302**, causing an electric 'echo' **311** to be emitted from the crystal **302**. The time delays between the original pulse of sound **301** and receiving the echo **311** define the depth of the change in acoustic impedance.

Changes in the delays in these electrical echoes **311** from tissue motion between repeated imaging sound pulses **301** are measured by delay estimation techniques that are well known in the art, such as cross-correlation. This tissue motion is referred to as the axial motion since it is measured in the axial direction of the transducer **103**.

FIG. 4 shows a method for imaging while the transducer **103** is in motion. The transducer **103** can move with up to 6 degrees of freedom when manipulated by a robotic tool **203**. The ultrasound images **106** must be captured in sequence while the transducer **103** is being moved across the tissue. Once the images are captured, they must be reconstructed (FIG. 5).

In some embodiments of the invention, each ultrasound image **106** is taken when the transducer **103** is held still, such that tissue displacements at one spatial location can be measured over multiple instances of time. For example, in the embodiment described in FIG. 1, the imaging sequence is triggered when the transducer **103** is held in place by the user **105**, which may be a robot. In one embodiment shown in FIG. 2, the acquisition of pulse-echo data is triggered while the robot is in the clutched state, i.e. when the tools **203** are disengaged from the surgeon control, and therefore the transducer **103** is stationary during the pulse-echo data acquisition. In both cases, capturing while in motion, or stationary, the imaging data needs to be reconstructed into a 3D volume for the most accurate elastogram creation.

FIG. 5 shows how several individual 2D ultrasound images, collected in any of the manners described above, can be used to create a volume of displacements. The captured ultrasound image planes **501-504** are used to create a volume of data **550** by techniques known in the art. In certain embodiments of the invention, a thin volume can be created from a few images (5-10), or several seconds of scanning can produce a volume consisting of 50-100 slices. The size of the volume **550** can be determined by the user either before the scan begins, or by terminating the scan. The planes **501-504** can be interpolated into a regularly-spaced volume of data using any of the methods described by Rohling et al ("Comparison of freehand three-dimensional ultrasound reconstruction techniques." *Medical Image Analysis*, 1999). The techniques described by Rohling et al. can be extended by one skilled in the art from a scalar intensity data to vector displacement data such as that represented in the volume of displacements **550**. This can be achieved, for example, by interpolating each of the scalar components of the measured displacement vectors onto the regular grid illustrated in FIG. 5. Thus, at every voxel center **551**, there is an associated displacement vector **552**, which is obtained from the vectors of displacements **130** in the ultrasound transducer coordinate system **121** (FIG. 2), transformed to vectors **530** of the coordinate system **520** of the volume of displacements **550**.

When the displacement vectors **130** in the ultrasound transducer coordinate system **121** are complex vectors or

phasors, then the above vector interpolation approach is repeated for the real part and the imaginary part of the phasor in a similar way. Hence, within the volume **550**, the displacement vectors **552** associated with every voxel center **551** represent the amplitude and phase of tissue motion at each voxel **551** within the volume **550**. The coordinate system **520** of the volume of tissue being imaged either coincides with the coordinate system **120** of the ultrasound transducer tracker, or is selected to be close to, or centered at, the volume of tissue being imaged. The chosen location does not affect the elasticity calculations, as the coordinate transformation between the volume coordinate system **520** and the ultrasound transducer tracker coordinate system **120** is known within the interpolation software (Rohling et al, Medical Image Analysis, 1999) and controllable by the user. Hence when we refer to the “base coordinate system”, we mean either the base of the tracker **120** or an arbitrary but known coordinate system with respect to which the tissue properties are calculated and displayed.

FIG. **6** shows how this method could be used to image a vessel **610**. The vessel **610** is filled with blood. The shear waves **102** that are imaged with this elastography method do not propagate in fluids. The motion tracking methods that are used fail to correctly measure motion since reflections **310** from within the vessel are not moving in a coherent way. The loss in coherent motion relative to the motion in the surrounding tissue creates a contrast in the final elastography volume. The level of coherence of tissue motion relative to a reference displacement (such as the exciter displacement, or the displacement of a tissue feature such as an edge, or the spatially averaged displacement of a tissue region) can be computed in a rigorous manner by using the coherence function as described in E. Turgay, S. E. Salcudean and R. N. Rohling, (“Identifying Mechanical properties of Tissue by Ultrasound”, Ultrasound in Medicine and Biology, 32(2), pp.221-235, 2006), which is herein incorporated by reference. The coherence function can be displayed as an image of intensities between zero and one. A tissue portion could be determined to be incoherent relative to the reference when the image intensity drops below a threshold value. For example, tissue areas in which the coherence is less than 0.5 are likely to be fluid.

FIG. **6A** shows how the transducer **103** would be used in an embodiment as described in FIG. **2**. The transducer is held by the robot tool **203** in such a way that the imaging plane **106** intersects with the vessel **610**. FIG. **6B** shows a wave image **620**, where the grey areas **602** represent the wave fronts of the shear waves **102**. The area **670** in the center of the wave image **620** represents the cross-section of the vessel **610**. The wave fronts **602** are disrupted in this area **670**. The amplitude of the waves **102** along the line **A** are shown in FIG. **6C**. The wave pattern within the area **670** is disrupted.

FIG. **6D** is a representation of the resulting elastography image **630** using the method described above, where the center area **671** defines the area of the vessel **610**. The area **671** of the vessel can be seen in good contrast to the background tissue **672**.

FIG. **7** shows one embodiment of the invention using the da Vinci laparoscopic robot. The stereo-camera of the da Vinci robot allows the surgical scene to be displayed to the surgeon in 3D dimensions. Using this display, a volume of elasticity **701** can be displayed to the surgeon. The surgical scene displayed in this figure shows the robotic tool **203** manipulating the transducer **103** on the surface of the organ of interest **210**, in the embodiment shown, this organ is a kidney, but in other embodiments, the organ of interest could

be the prostate, bowel, or other organ. When the scan has been completed and the volume of elasticity **701** can be seen in the place where it was imaged through the stereo display. Within the volume **701**, features such as a vessel **720** and a potential tumour **710** are displayed.

Using this method of determining the local elastic properties the loss of the haptic feedback that is typically absent in current robot systems can thus be supplemented by imaging.

FIG. **8** describes one embodiment of the overall workflow of this invention. In this described embodiment, the axial displacements **801** are captured using fast ultrasound imaging techniques (Baghani, A. et al, “A high-frame-rate ultrasound system for the study of tissue motions”, IEEE Ultrasonics, Ferroelectrics and Frequency Control. 57(7), 1535-1547 (2010)). The 3D tracking data **802** is combined with the displacements measurements **801** using interpolation methods. The final displacements are reconstructed into a 3D volume **803** to create volumetric displacements **804**. Inversion methods **805** such as local frequency estimation (Manduca, A., et al. “Local wavelength estimation for magnetic resonance elastography”. IEEE Conference on Image Processing, 1996) are used to determine the spatial wave frequency within the volumetric data. And finally an elastogram **806** is created that represents the elastic properties of the tissue that was imaged. The steps in this embodiment are only one possible from a series of algorithms that could be used. A survey of inversion methods for elastography is presented by Doyley et al (“Model-based elastography: a survey of approaches to the inverse elasticity problem”, Physics in Medicine and Biology 57(3), 2012).

In ultrasound imaging, images may be acquired by repeatedly imaging sectors at high frame rates, wherein a sector is a subset of a full ultrasound image. A sector may cover only part of the entire width of the ultrasound transducer array. The time delay between sectors; the time delay between different lines within the same sector; and/or the time delay within each line (as described above for example with reference to FIG. **3** and the time delays between the original pulse of sound **301** and receiving echo **311**), may be computed and processed to image a large (volume) region of interest and to compute tissue displacements relative to the ultrasound transducer. The frame of reference coordinate system for the computed tissue displacements may be changed from the ultrasound transducer coordinate system to a base coordinate system using a phase compensation for time delays for one or both of time of flight of ultrasound pulses, and time delays between subsequent ultrasound pulses.

In addition to the sector-based technique, the bandpass sampling technique described in U.S. Pat. No. 8,668,647, by H. Eskandari et al, and in U.S. Pat. Application No 2012/000779, by A. Baghani et al., can be used to recover tissue displacements, even when sampled at a lower frame rate than the Nyquist sampling rate. In sector based methods all the samples required to reconstruct the tissue displacement phasor are collected at high pulse repetition frequency (PRF), achieved by dividing the image into smaller sectors. As shown in FIG. **13a**, with the sector methods the tissue displacement is sampled for a short period of time at a high sector frame rate. As shown in FIG. **13b**, in bandpass sampling all the tissue displacement samples at a given location are collected at lower frame rate, as in full-frame B-mode imaging. These two methods can be combined. In the combined method (FIG. **13c**) the sector samples are collected at high PRF using the sector method and the groups are repeated at a lower rate as in bandpass method.

With this approach, the tissue velocities or relative displacements can be computed by comparing two consecutive RF lines that are sampled at a high PRF and therefore achieve a lower decorrelation and higher signal-to-noise ratio, at the same time benefiting from bandpass sampling. Indeed, as some of the displacements/velocity samples are placed further apart in time, there is flexibility to be gained in how the frequencies of the mechanical excitation are selected. While only one frequency is shown in FIGS. 13*a*, *b*, and *c*, in practice multiple frequencies are required for reliable elasticity imaging. As with tissue displacement measurements, the frame of reference coordinate system for the computed tissue velocities may be changed from the ultrasound transducer coordinate system to a base coordinate system using a phase compensation for time delays for one or both of time of flight of ultrasound pulses, and time delays between subsequent ultrasound pulses.

FIG. 9 shows an embodiment wherein tracking is performed by coupling a mechanical arm 250 between the ultrasound transducer 103 and a tracking base unit 240. In the illustrated embodiment, mechanical arm 250 comprises a plurality of members pivotally connected to one another and/or to the tracking base unit 240 and the ultrasound transducer 230. Movements are detected in the mechanical arm 250 (e.g. by detecting the degree of rotation of members about each pivot point). Tracking base unit 240 may be moved between different locations to allow the ultrasound transducer 103 to be placed over different locations on the patient. Tracking can be performed similarly to methods described above wherein the position of the transducer 103 can be found through the combinations of the transformations between the base coordinate system (i.e. the coordinate system 120 of the tracking base unit 240) and the coordinate system of the sensor on the ultrasound transducer 103 and the transformation between the sensor coordinate system and the coordinate system of the ultrasound image.

What is claimed is:

1. A method for measuring the mechanical properties in a volume of tissue, the method comprising the steps of:
 - applying an excitation to said volume of tissue with a vibration source;
 - scanning said volume of tissue with a tracked ultrasound transducer;
 - measuring said tracked ultrasound transducer locations relative to a base coordinate system;
 - computing a tissue response relative to said tracked ultrasound transducer from echo data measured by said tracked ultrasound transducer, wherein said tissue response comprises one or more of tissue displacements and tissue velocities;
 - converting said tissue response from said tracked ultrasound transducer coordinate system to said base coordinate system using said tracked ultrasound transducer locations; and
 - calculating said mechanical properties in said volume of tissue from said tissue response in said base coordinate systems;
- wherein said changing of the coordinate system of said tissue response to said base coordinate system comprises a phase compensation for time delays for one or both of (i) time of flight of ultrasound pulses, and (ii) time delays between subsequent ultrasound pulses.
2. A method according to claim 1, wherein calculating said mechanical properties comprises interpolating said tissue response in said base coordinate system onto a uniform grid.

3. A method according to claim 1, wherein said excitation is steady-state.

4. A method according to claim 1, wherein a location of said tracked ultrasound transducer is determined using one or more of:

- (a) electromagnetic sensing,
- (b) passive or active optical sensing,
- (c) robot sensing;
- (d) sensing by an inertial measurement unit; and
- (e) a mechanical linkage between the tracked ultrasound transducer and a tracking base.

5. A method according to claim 4 wherein said location of the tracked ultrasound transducer is constrained by a constraining fixture or linkage.

6. A method according to claim 4 wherein one or more degrees of freedom of the tracked ultrasound transducer is constrained by a constraining fixture or linkage.

7. A method according to claim 4, wherein said location of said tracked ultrasound transducer is determined based on ultrasound transducer image-based motion estimation.

8. A method according to claim 7, wherein the ultrasound transducer image-based motion estimation comprises applying a correlation-based algorithm to determine the transducer motion within each imaging plane or within and outside each imaging plane, from ultrasound echo data.

9. A method according to claim 7, wherein the ultrasound transducer image-based motion estimation comprises applying a machine learning-based algorithm to determine the transducer motion within each imaging plane or within and outside each imaging plane, from ultrasound echo data.

10. A method according to claim 1, wherein said vibration source is placed on the skin of a patient.

11. A method according to claim 1, wherein said tracked ultrasound transducer is placed on the skin of a patient.

12. A method according to claim 1, wherein said tracked ultrasound transducer is placed inside a patient and directly adjacent to an area or organ of interest.

13. A method according to claim 1, wherein the calculation of said mechanical properties of tissue comprises calculation of coherence between said tissue displacements and a reference displacement to distinguish soft tissue from a fluid.

14. A method according to claim 1, wherein said tracked ultrasound transducer is moved in a discrete stepwise fashion over said volume of tissue wherein each step comprises holding said tracked ultrasound transducer stationary while measuring said echo data, and then moving said tracked ultrasound transducer to a different location.

15. A method according to claim 1, wherein said tracked ultrasound transducer is moved in a continuous fashion over said volume of tissue.

16. A method according to claim 1, wherein said mechanical properties comprise a quantitative measure of the shear modulus of tissue.

17. A method according to claim 1, wherein said mechanical properties comprise a quantitative measure of the elasticity of the tissue.

18. A method according to claim 1, wherein mechanical properties comprise a quantitative measure of the shear wave speed of the tissue.

19. A method according to claim 1, wherein said mechanical properties comprise a quantitative measure of the shear viscosity of the tissue.

20. A method according to claim 1, wherein said mechanical properties are calculated as a function of frequency.

17

21. A method according to claim **1**, wherein said tracked ultrasound transducer is a matrix transducer array that is capable of both 2D cross-sectional imaging and 3D volumetric imaging.

22. A method according to claim **1**, wherein said tissue response comprises tissue velocities, and computing said tissue response comprises computing said tissue velocities from a plurality of scans of a sector comprising one or more transducer lines.

* * * * *

10

18

专利名称(译)	定量弹性成像与跟踪2D超声换能器		
公开(公告)号	US10117640	公开(公告)日	2018-11-06
申请号	US15/798186	申请日	2017-10-30
[标]申请(专利权)人(译)	英属哥伦比亚大学		
申请(专利权)人(译)	加拿大不列颠哥伦比亚大学		
当前申请(专利权)人(译)	加拿大不列颠哥伦比亚大学		
[标]发明人	SALCUDEAN SEPTIMIU EDMUND SCHNEIDER CAITLIN MARIE ROHLING ROBERT N BAGHANI ALI HONARVAR MOHAMMAD		
发明人	SALCUDEAN, SEPTIMIU EDMUND SCHNEIDER, CAITLIN MARIE ROHLING, ROBERT N. BAGHANI, ALI HONARVAR, MOHAMMAD		
IPC分类号	A61B8/08 A61B8/00 A61B8/12		
CPC分类号	A61B8/485 A61B8/12 A61B8/4263 A61B8/483 A61B8/4209 A61B8/4281		
优先权	61/707883 2012-09-28 US		
其他公开文献	US20180125455A1		
外部链接	Espacenet		

摘要(译)

描述了一种用于获取3D定量超声弹性成像体积的方法。2D超声换能器扫描使用外部振动源通过其产生剪切波的组织体积，在超声换能器的平面内的组织运动的同步测量，其中测量换能器在空间中的位置，重建组织位移和/或来自该同步测量的体积在时间和空间上的组织速度，以及来自该体积测量位移的组织的一个或多个机械特性的计算。换能器平面中的组织运动可以在换能器的轴向方向上以高的有效帧速率测量，或者在换能器的轴向和横向方向上测量。可以在规则网格上内插测量体积上的组织位移和/或组织速度，以便于计算机械性质。

