



(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2001/0021810 A1**

**Hashimoto**

(43) **Pub. Date: Sep. 13, 2001**

(54) **METHOD OF ULTRASONIC IMAGING AND ULTRASONIC DIAGNOSTIC APPARATUS**

(52) **U.S. Cl. .... 600/458**

(76) **Inventor: Hiroshi Hashimoto, Tokyo (JP)**

(57) **ABSTRACT**

Correspondence Address:  
**MOONRAY KOJIMA**  
**BOX 627**  
**WILLIAMSTOWN, MA 01267 (US)**

An ultrasonic diagnostic apparatus transmits ultrasonic waves at such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and at such a strength as not to disperse the contrast agent for other sonic beams thereby to produce an image for a marking frame from received echo signals of ultrasonic transmission, and subsequently transmits ultrasonic waves successively at such a strength as not to disperse the contrast agent for all sonic beams thereby to produce images continuously for no-marking frames, and, after such a time length that the flow range is present within the view field, produces an image for another marking frame. These operations are repeated to display ultrasonic images by which it is possible to visually recognize at a glance the time-wise change of a blood flow.

(21) **Appl. No.: 09/777,984**

(22) **Filed: Feb. 6, 2001**

(30) **Foreign Application Priority Data**

Mar. 8, 2000 (JP) ..... 2000-63853

**Publication Classification**

(51) **Int. Cl.<sup>7</sup> ..... A61B 8/14**

1 0 0

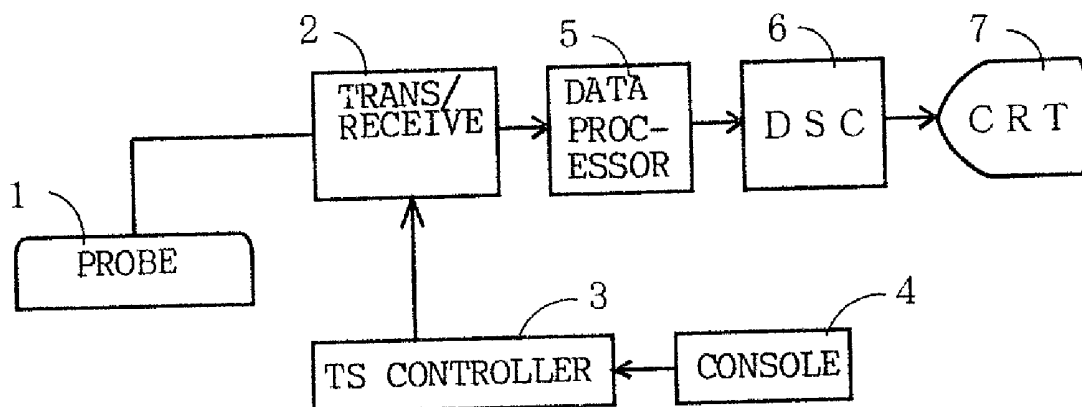


FIG. 1 (PRIOR ART)

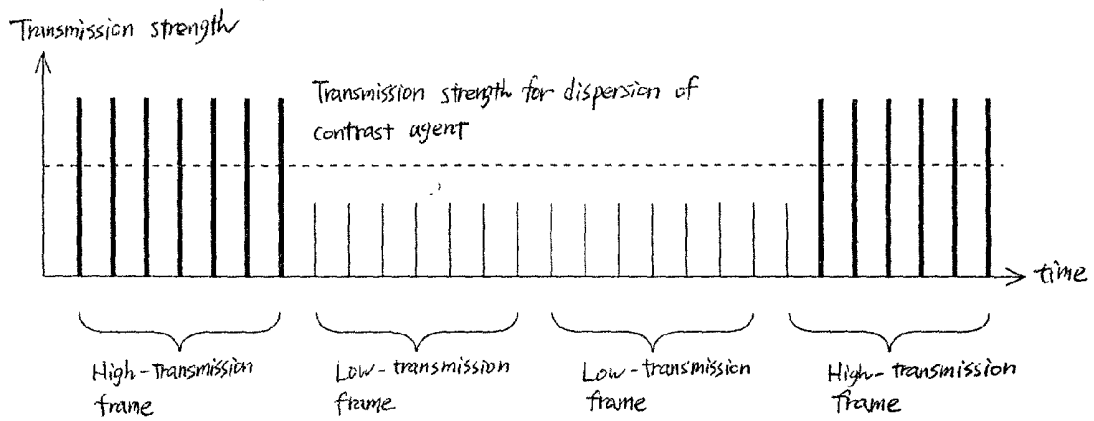


FIG. 2 (a) (PRIOR ART)

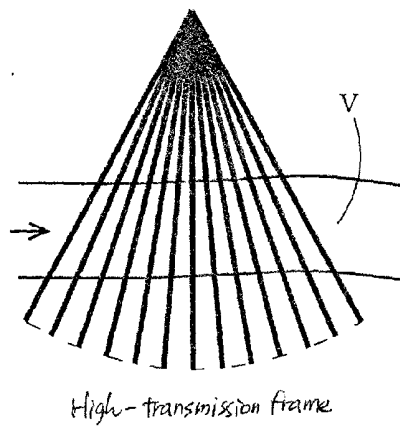


FIG. 2 (b) (PRIOR ART)

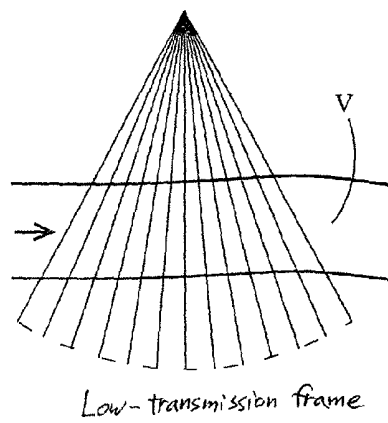


FIG. 3

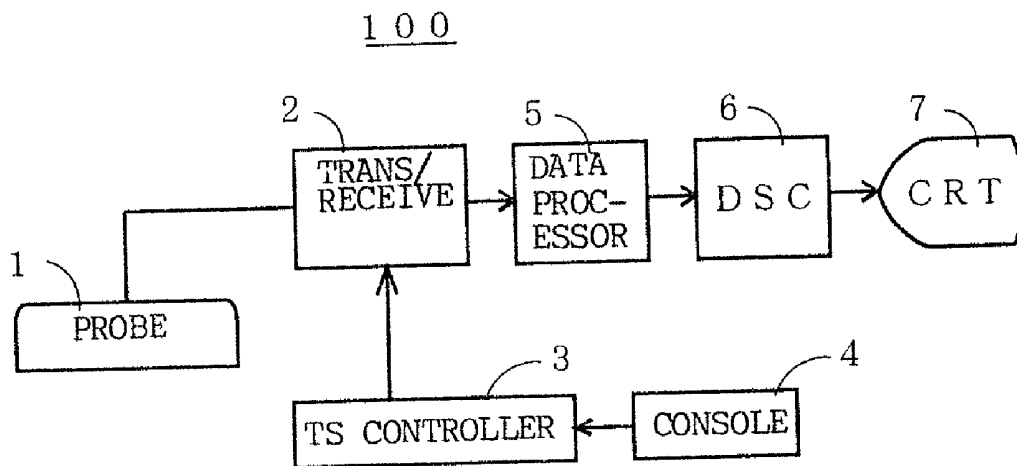


FIG. 4 (a)

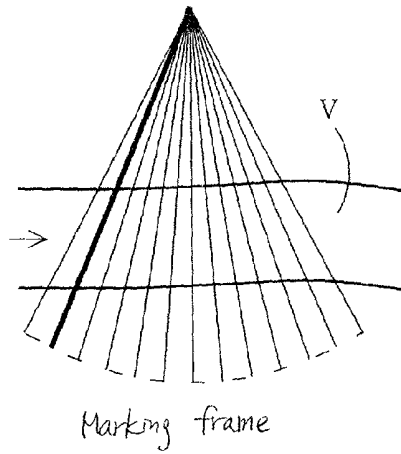


FIG. 4 (b)

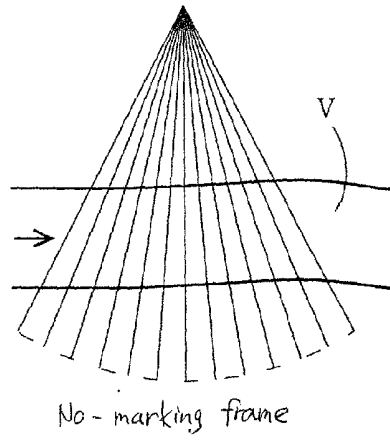


FIG. 5



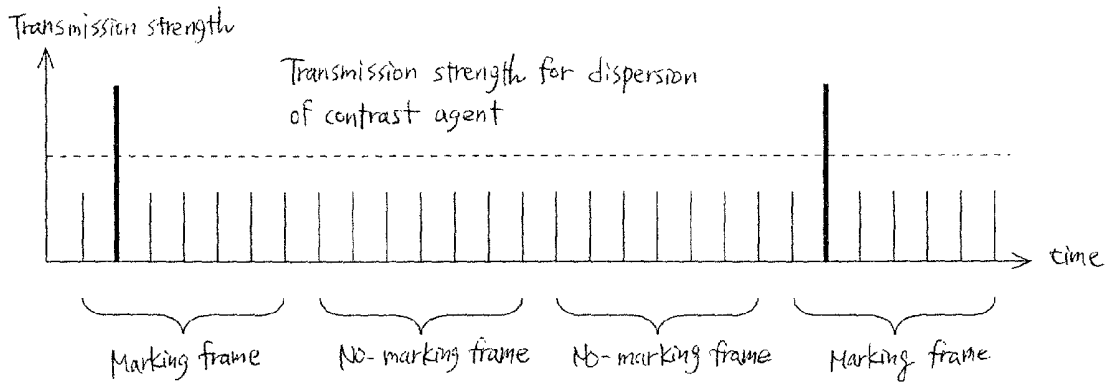


FIG. 6 (a)

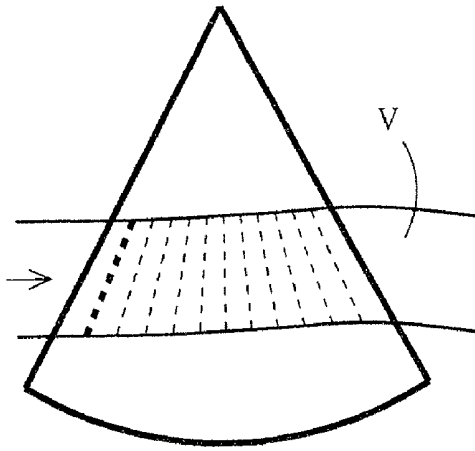


First marking frame

FIG. 6 (b)

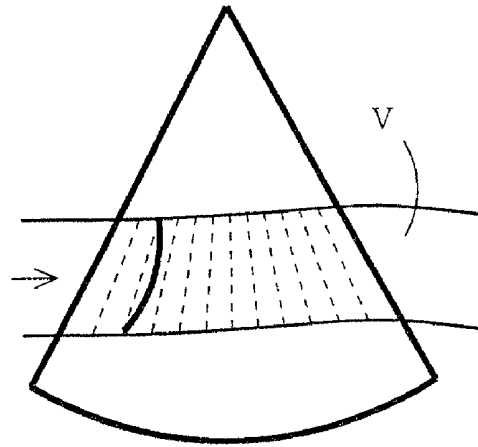

No-marking frame

FIG. 6 (c)

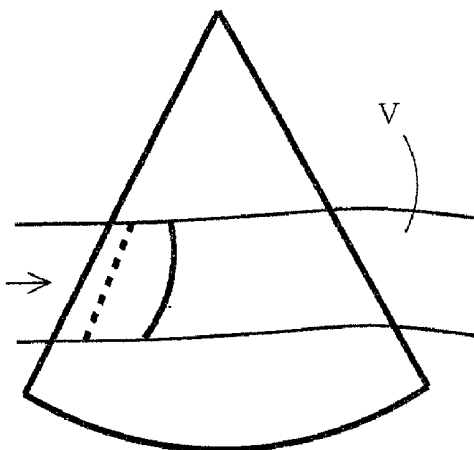

Second marking frame

FIG. 6 (d)

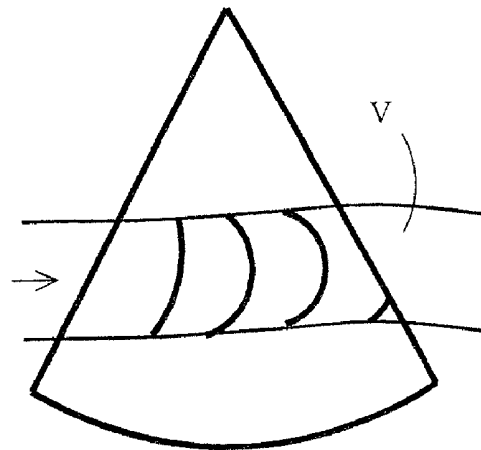


FIG. 7 (a)

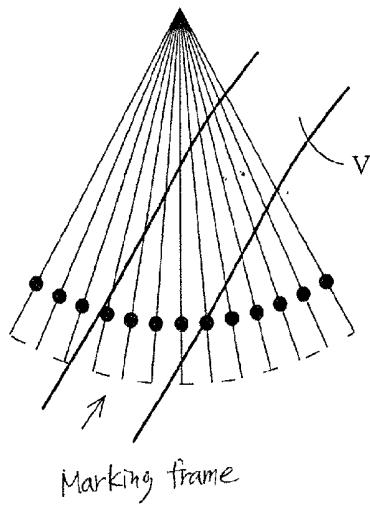


FIG. 7 (b)

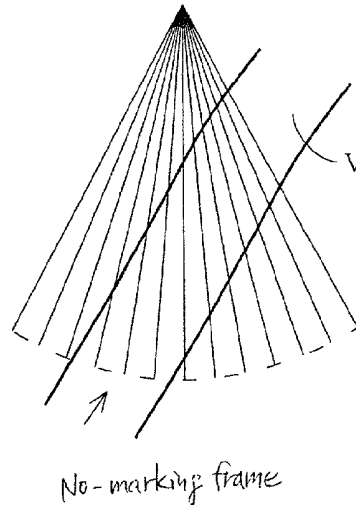


FIG. 8



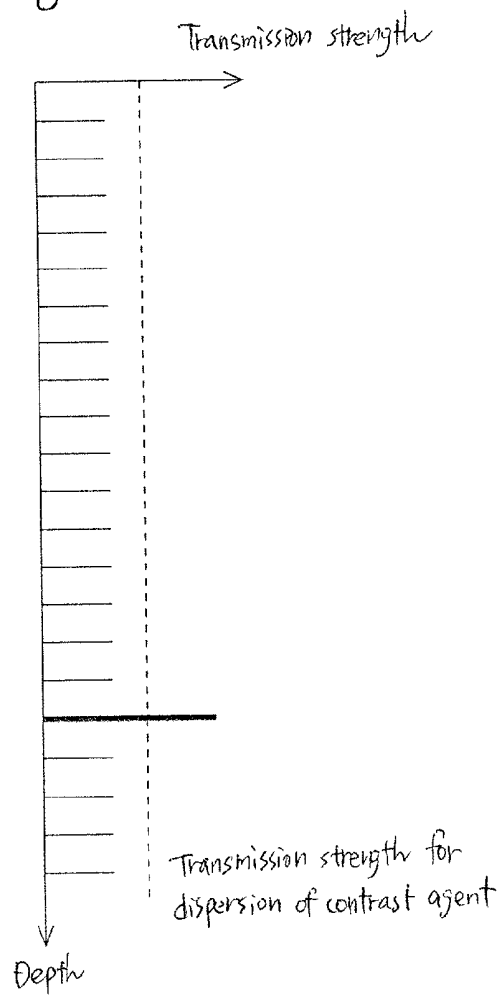


FIG. 9(a)

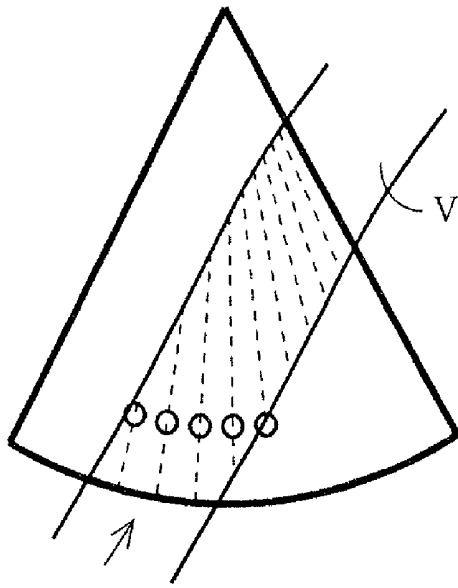


Marking frame

FIG. 9(b)

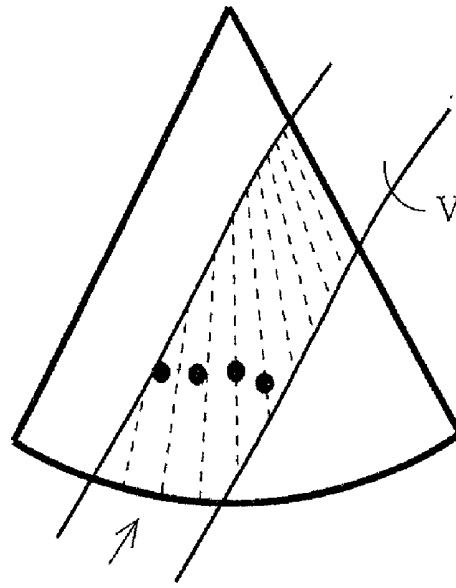

No-marking frame

FIG. 9(c)

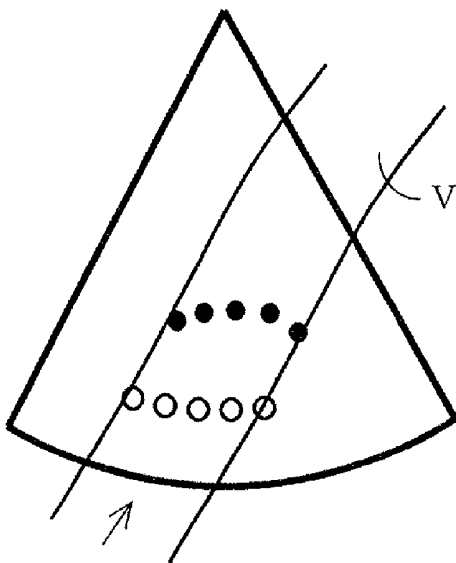

Marking frame

FIG. 9(d)



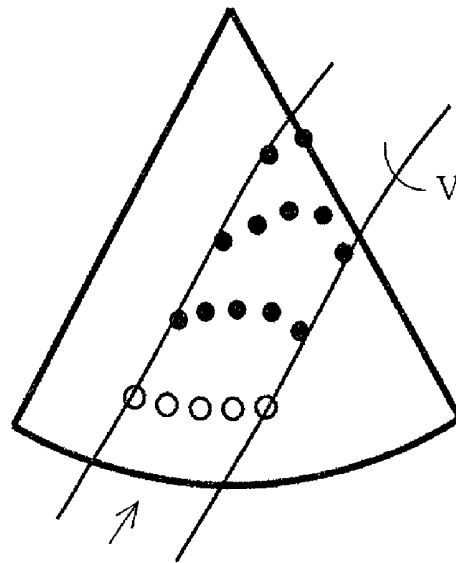


FIG. 10(a)

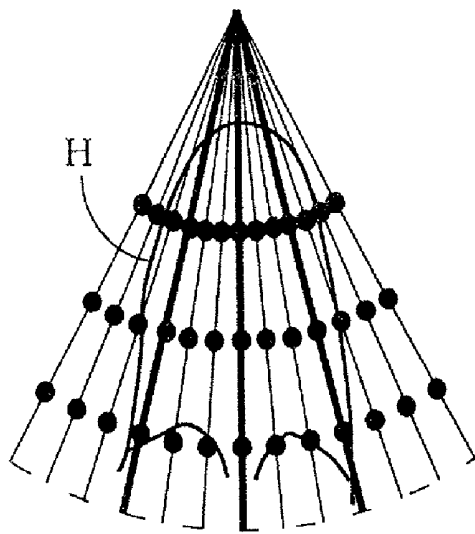


marking frame

FIG. 10(b)

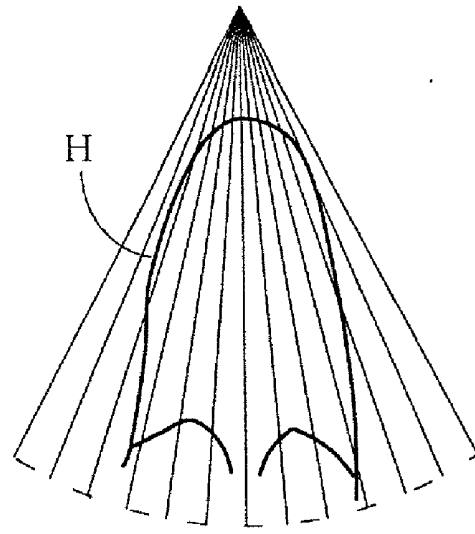

No-marking frame

FIG. 11

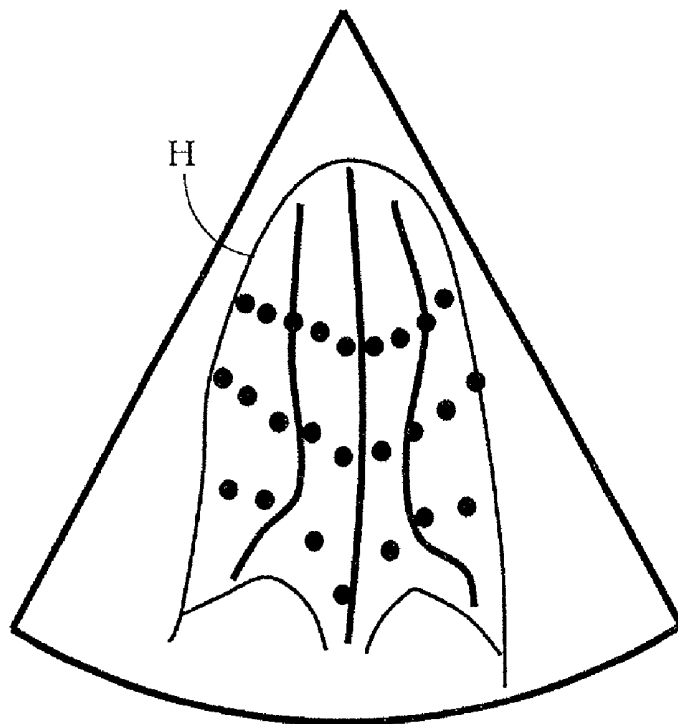

## METHOD OF ULTRASONIC IMAGING AND ULTRASONIC DIAGNOSTIC APPARATUS

### BACKGROUND OF THE INVENTION

[0001] The present invention relates to a method of ultrasonic imaging and an ultrasonic diagnostic apparatus, and more particularly to a method of ultrasonic imaging and an ultrasonic diagnostic apparatus capable of producing ultrasonic images by which it is possible to visually recognize at a glance the time-wise change of a blood flow.

[0002] In obtaining an ultrasonic image of a blood flow, there has been a convention to use small bubbles in blood as the contrast agent. These small bubbles disperse by being hit by a strong ultrasonic wave.

[0003] On this account, after the imaging for a high-transmission frame (a frame taken by use of an ultrasonic wave which is strong enough to disperse the contrast agent), imaging for low-transmission frames (frames taken by use of an ultrasonic wave which is not so strong as to disperse the contrast agent) is carried out continuously, and imaging for another high-transmission frame is carried out on expiration of the time at which the view field is filled with a blood flow including the contrast agent, with these operations being implemented cyclically, as shown in **FIG. 1**.

[0004] In **FIG. 1**, vertical line segments aligning along the time axis represent transmission time points and transmission strengths of sonic beams which form the frames.

[0005] **FIG. 2(a)** shows sonic beams which form a high-transmission frame, and the bold lines signify an ultrasonic wave which is strong enough to disperse the contrast agent. Indicated by **V** is a blood vessel, and the arrow indicates the direction of blood flow.

[0006] In contrast, **FIG. 2(b)** shows sonic beams which form a low-transmission frame, and the thin lines signify an ultrasonic wave which is not so strong as to disperse the contrast agent.

[0007] It has been possible to view the state of a blood flow at one moment in the image of a high-transmission frame which is taken based on the above-mentioned conventional scheme.

[0008] However, this scheme has been problematic in that it cannot provide a view of the time-wise change of a blood flow. Specifically, if it is intended to view the time-wise change of a blood flow, it is necessary to compare images of high-transmission frames taken at different time points, and it necessitates skill.

### SUMMARY OF THE INVENTION

[0009] It is an object of the present invention to provide a method of ultrasonic imaging and an ultrasonic diagnostic apparatus capable of producing ultrasonic images by which it is possible to visually recognize at a glance the time-wise change of a blood flow.

[0010] At a first viewpoint, the present invention provides a method of ultrasonic imaging which is characterized by transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent

for other sonic beams, and producing an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0011] In the ultrasonic imaging method of the first viewpoint, the contrast agent in one part of the image disperses, while the contrast agent in other part does not disperse. Therefore, when another imaging takes place after such a time length that the flow range is present within the view field, the portion with the contrast agent being dispersed moves slightly in its position on the image. When this operation is repeated for a flow which intersects the direction of sonic beam, an effect similar to the tagging in magnetic resonance imaging emerges, and the flow seems to have a stripe pattern indicative of the passing time. As a result, it becomes possible to visually recognize the time-wise change of a blood flow at a glance.

[0012] At a second viewpoint, the present invention provides a method of ultrasonic imaging which is characterized by transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, producing an image for one frame from received signals which correspond to the ultrasonic wave transmission, and interposing the formed frame between frames which are produced by the ultrasonic imaging method mentioned in the first viewpoint.

[0013] In the ultrasonic imaging method of the second viewpoint, a frame without the dispersion of contrast agent is interposed between frames with the dispersion of contrast agent in part of the image, whereby the real-time property of progressive imaging can be improved.

[0014] At a third viewpoint, the present invention provides a method of ultrasonic imaging which is derived from the method of the second viewpoint, and is characterized in that one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

[0015] In the ultrasonic imaging method of the third viewpoint, there is provided a time difference between events of transmission by which the contrast agent is dispersed in part of the image, whereby a pulsing flow can be observed properly.

[0016] At a fourth viewpoint, the present invention provides a method of ultrasonic imaging which is derived from the method of the third viewpoint, and is characterized in that there are in one frame at least two spaced-out sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

[0017] In the ultrasonic imaging method of the fourth viewpoint, the contrast agent disperses at least two spaced-out positions, whereby a number of stripe patterns can be appended to a flow at the same time.

[0018] At a fifth viewpoint, the present invention provides a method of ultrasonic imaging which is characterized by transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from the ultrasonic probe and transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent

for other depths, and producing an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0019] In the ultrasonic imaging method of the fifth viewpoint, the contrast agent in one part of the image disperses, whereas the contrast agent in other part does not disperse. Therefore, when another imaging takes place after such a time length that the flow range is present within the view field, the portion with the contrast agent being dispersed moves slightly in its position on the image. When this operation is repeated for a flow which intersects the direction of sonic beam, an effect similar to the tagging in magnetic resonance imaging emerges, and the flow seems to have a stripe pattern indicative of the passing time. Whereby, it becomes possible to visually recognize at a glance the time-wise change of a blood flow.

[0020] At a sixth viewpoint, the present invention provides a method of ultrasonic imaging which is characterized by transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, producing an image for one frame from received signals which correspond to the ultrasonic wave transmission, and interposing the formed frame between frames which are produced by the ultrasonic imaging method mentioned in the fifth viewpoint.

[0021] In the ultrasonic imaging method of the sixth viewpoint, a frame without the dispersion of contrast agent is interposed between frames with the dispersion of contrast agent in part of the image, whereby the real-time property of progressive imaging can be improved.

[0022] At a seventh viewpoint, the present invention provides a method of ultrasonic imaging which is derived from the method of the sixth viewpoint, and is characterized in that one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

[0023] In the ultrasonic imaging method of the seventh viewpoint, there is provided a time difference between events of transmission by which the contrast agent is dispersed in part of the image, whereby a pulsing flow can be observed properly.

[0024] At an eighth viewpoint, the present invention provides a method of ultrasonic imaging which is derived from the method of the seventh viewpoint, and is characterized in that there are in one frame at least two spaced-out positions of depths for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

[0025] In the ultrasonic imaging method of the eighth viewpoint, the contrast agent disperses at least two spaced-out positions, whereby a number of stripe patterns can be appended to the flow at the same time.

[0026] At a ninth viewpoint, the present invention provides a method of ultrasonic imaging characterized by combining an ultrasonic imaging method of the first through fourth viewpoints and an ultrasonic imaging method of the fifth through eighth viewpoints.

[0027] In the ultrasonic imaging method of the ninth viewpoint, stripe patterns are appended to both of a flow

which intersects the direction of sonic beam and a flow which is virtually parallel to the direction of sonic beam, whereby it is particularly suitable to observe a two-dimensional flow of the cardiac ventricle and atrium.

[0028] At a tenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus characterized by comprising an ultrasonic probe, a transmission/reception means which transmits an ultrasonic wave from the ultrasonic probe and receives a signal which corresponds to the ultrasonic wave transmission, a transmission strength control means which controls the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and have such a strength as not to disperse the contrast agent for other sonic beams, and an image producing means which produces an image for one frame from the received signals.

[0029] The ultrasonic diagnostic apparatus of the tenth viewpoint can suitably carry out the ultrasonic imaging method of the first viewpoint.

[0030] At an eleventh viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from the apparatus of the tenth viewpoint and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that one frame, which is formed at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, is interposed between frames which are formed by the ultrasonic wave transmission at such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for other sonic beams.

[0031] The ultrasonic diagnostic apparatus of the eleventh viewpoint can suitably carry out the ultrasonic imaging method of the second viewpoint.

[0032] At a twelfth viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from the apparatus of the eleventh viewpoint and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

[0033] The ultrasonic diagnostic apparatus of the twelfth viewpoint can suitably carry out the ultrasonic imaging method of the third viewpoint.

[0034] At a thirteenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from an apparatus of the tenth through twelfth viewpoints and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that there are in one frame at least two spaced-out sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

[0035] The ultrasonic diagnostic apparatus of the thirteenth viewpoint can suitably carry out the ultrasonic imaging method of the fourth viewpoint.

[0036] At a fourteenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus characterized by comprising an ultrasonic probe, a transmission/reception means which transmits an ultrasonic wave from the ultrasonic probe and receives a signal which corresponds to the ultrasonic wave transmission, a transmission strength control means which controls the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from the ultrasonic probe and have such a strength as not to disperse the contrast agent for other depths, and an image producing means which produces an image for one frame from the received signals.

[0037] The ultrasonic diagnostic apparatus of the fourteenth viewpoint can suitably carry out the ultrasonic imaging method of the fifth viewpoint.

[0038] At a fifteenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from the apparatus of the fourteenth viewpoint and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that one frame, which is formed by the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, is interposed between frames which are formed by the ultrasonic wave transmission at such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from the ultrasonic probe and at such a strength as not to disperse the contrast agent for other depths.

[0039] The ultrasonic diagnostic apparatus of the fifteenth viewpoint can suitably carry out the ultrasonic imaging method of the sixth viewpoint.

[0040] At a sixteenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from the apparatus of the fifteenth viewpoint and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

[0041] The ultrasonic diagnostic apparatus of the sixteenth viewpoint can suitably carry out the ultrasonic imaging method of the seventh viewpoint.

[0042] At a seventeenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus which is derived from an apparatus of the fourteenth through sixteenth viewpoints and is characterized in that the transmission strength control means controls the ultrasonic wave transmission such that there are in one frame at least two spaced-out positions of depths for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

[0043] The ultrasonic diagnostic apparatus of the seventeenth viewpoint can suitably carry out the ultrasonic imaging method of the eighth viewpoint.

[0044] At an eighteenth viewpoint, the present invention provides an ultrasonic diagnostic apparatus characterized by comprising an ultrasonic probe, a transmission/reception

means which transmits an ultrasonic wave from the ultrasonic probe and receives a signal which corresponds to the ultrasonic wave transmission, a transmission strength control means which controls the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and have for other sonic beams such a strength as to disperse the contrast agent for a certain depth of the sonic beams or a certain depth seen from the ultrasonic probe and have such a strength as not to disperse the contrast agent for other depths, and an image producing means which produces an image for one frame from the received signals.

[0045] The ultrasonic diagnostic apparatus of the eighteenth viewpoint can suitably carry out the ultrasonic imaging method of the ninth viewpoint.

[0046] According to the ultrasonic imaging method and ultrasonic diagnostic apparatus of this invention, which actively utilize the dispersion of contrast agent in the presence of a strong ultrasonic wave, it is possible to produce ultrasonic images which enable to visually recognize at a glance the time-wise change of a blood flow.

[0047] Further objects and advantages of the present invention will be apparent from the following description of the preferred embodiments of the invention as illustrated in the accompanying drawings.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0048] FIG. 1 is an explanatory diagram showing the transmission order for forming high-transmission frames and low-transmission frames based on the conventional scheme.

[0049] FIG. 2 is an explanatory diagram of the high-transmission frame and low-transmission frame based on the conventional scheme.

[0050] FIG. 3 is a block diagram of an ultrasonic diagnostic apparatus based on the first embodiment.

[0051] FIG. 4 is an explanatory diagram of a marking frame and no-marking frame based on the first embodiment.

[0052] FIG. 5 is an explanatory diagram showing the transmission order for forming frames based on the first embodiment.

[0053] FIG. 6 is a set of diagrams showing examples of ultrasonic images produced by the ultrasonic diagnostic apparatus based on the first embodiment.

[0054] FIG. 7 is an explanatory diagram of a marking frame and no-marking frame based on the second embodiment.

[0055] FIG. 8 is an explanatory diagram of the transmission strength for the marking frame based on the second embodiment.

[0056] FIG. 9 is a set of diagrams showing examples of ultrasonic images produced by the ultrasonic diagnostic apparatus based on the second embodiment.

[0057] FIG. 10 is an explanatory diagram of a marking frame and no-marking frame based on the third embodiment.

[0058] FIG. 11 is a diagram of an ultrasonic image produced by the ultrasonic diagnostic apparatus based on the third embodiment.

#### DETAILED DESCRIPTION OF THE INVENTION

[0059] The present invention will be explained in more detail by dealing with the illustrated embodiments.

##### First Embodiment

[0060] FIG. 3 is a block diagram of an ultrasonic diagnostic apparatus 100 based on the first embodiment of this invention.

[0061] This ultrasonic diagnostic apparatus 100 is made up of an ultrasonic probe 1, a transmitter/receiver 2 which transmits an ultrasonic wave at a specified transmission strength, receives the echo of ultrasonic transmission, and produces a reception signal, a transmission strength controller 3 which specifies the transmission strength, an operation console 4 which is used by the operator to instruct the transmission strength controller 3, a data processor 5 which produces an ultrasonic image such as a B-mode image from the reception signal, a DSC (digital scan converter) 6 which converts the ultrasonic image into a display image, and a CRT 7 which displays the display image.

[0062] FIG. 4(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus 100.

[0063] The marking frame is defined to be an image of a frame which is produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for part (shown by the bold lines) of a number of sonic beams which form one frame and the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for other sonic beams (shown by the thin lines), and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0064] FIG. 4(b) is an explanatory diagram of a no-marking frame produced by the ultrasonic diagnostic apparatus 100.

[0065] The no-marking frame is defined to be an image of a frame which is produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0066] FIG. 5 is an explanatory diagram showing the transmission time points and transmission strengths of sonic beams of the ultrasonic diagnostic apparatus 100.

[0067] Vertical line segments aligning along the time axis represent transmission time points and transmission strengths of sonic beams which form the frames.

[0068] Following the imaging for a marking frame, imaging for no-marking frames is carried out continuously, and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0069] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for

a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0070] FIG. 6 is a set of explanatory diagrams of images produced by the ultrasonic diagnostic apparatus 100.

[0071] Shown by (a) is a first marking frame, in which case the contrast agent on the sonic beam (bold dashed line) at the transmission strength for the dispersion of contrast agent disperses, whereas the contrast agent on the sonic beams (thin dashed line) at the transmission strength for no dispersion of contrast agent does not disperse.

[0072] Shown by (b) is a no-marking frame which follows the first marking frame, in which case the portion (bold line) where the contrast agent has dispersed in the first marking frame has a weaker echo than other portion and seems to be the black void. Thin dashed lines represent sonic beams at the transmission strength for no dispersion of contrast agent.

[0073] Shown by (c) is a second marking frame, in which case only the contrast agent on the sonic beam (bold dashed line) at the transmission strength for the dispersion of contrast agent disperses, as in the case of (a). The portion (bold line) where the contrast agent has dispersed in the first marking frame seems to be the black void.

[0074] Shown by (d) is an image after the fifth or later marking frame, in which the portions (bold line) where the contrast agent has dispersed in the preceding marking frames seem to be stripes of the black void.

[0075] The ultrasonic diagnostic apparatus 100 of the foregoing first embodiment presents a stripe pattern appended to a flow which intersects the direction of sonic beams as shown by (d) in FIG. 6, whereby it becomes possible to visually recognize the time-wise change at a glance.

##### Second Embodiment

[0076] The arrangement of an ultrasonic diagnostic apparatus based on the second embodiment of this invention is identical to that shown in FIG. 3.

[0077] FIG. 7(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus of the second embodiment.

[0078] The marking frame is defined to be a frame produced by the concentrated transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for a certain depth (indicated by black dots) of a number of sonic beams (thin lines) which form one frame and the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for other depths, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission. A certain depth on sonic beams may be replaced with a certain depth seen from the ultrasonic probe.

[0079] FIG. 7(b) is an explanatory diagram of a no-marking frame.

[0080] The no-marking frame is defined to be a frame which is produced by the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0081] FIG. 8 is an explanatory diagram showing the depths and transmission strengths of sonic beams used for the marking frame.

[0082] Lateral line segments aligning on the depth axis represent transmission strengths.

[0083] Also in the second embodiment, following the imaging of a marking frame, imaging for no-marking frames is carried out continuously, and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0084] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0085] FIG. 9 is a set of explanatory diagrams of images produced by the ultrasonic diagnostic apparatus of the second embodiment.

[0086] Shown by (a) is a first marking frame, in which case the contrast agent in a portion of the depth (white dots) where the contrast agent is to be dispersed disperses, whereas the contrast agent in other portion does not disperse. Thin dashed lines represent sonic beams at the transmission strength for no dispersion of contrast agent.

[0087] Shown by (b) is a no-marking frame which follows the first marking frame, in which case the portion (black dots) where the contrast agent has dispersed in the first marking frame has weaker echoes than other portion and seems to be the black void.

[0088] Shown by (c) is a second marking frame, in which case only the contrast agent at the depth (white dots) for the dispersion of contrast agent disperses, as in the case of (a). The portion (black dots) where the contrast agent has dispersed in the first marking frame seems to be the black void.

[0089] Shown by (d) is an image after the fourth or later marking frame, in which the portions (black dots) where the contrast agent has dispersed in the preceding marking frames seem to be stripes of the black void.

[0090] The ultrasonic diagnostic apparatus of the foregoing second embodiment presents a stripe pattern appended to a flow which is virtually parallel to the direction of sonic beams as shown by (d) in FIG. 9, whereby it becomes possible to visually recognize the time-wise change at a glance.

#### Third Embodiment

[0091] The arrangement of an ultrasonic diagnostic apparatus based on the third embodiment of this invention is identical to that shown in FIG. 3.

[0092] FIG. 10(a) is an explanatory diagram of a marking frame produced by the ultrasonic diagnostic apparatus of the third embodiment.

[0093] The marking frame is defined to be a frame produced by the transmission of an ultrasonic wave at the strength for the dispersion of contrast agent for two or more spaced-out sonic beams (bold lines) among a number of sonic beams which form one frame and the transmission of an ultrasonic wave for other sonic beams at the strength for the dispersion of contrast agent for two or more spaced-out positions of a certain depth (black dots) and at the strength for no dispersion of contrast agent for other depths, and the formation of an image for one frame from received signals which correspond to the ultrasonic transmission. A certain depth on sonic beams may be replaced with a certain depth seen from the ultrasonic probe.

[0094] FIG. 10(b) is an explanatory diagram of a no-marking frame.

[0095] The no-marking frame is defined to be a frame which is produced by the transmission of an ultrasonic wave at the strength for no dispersion of contrast agent for all of a number of sonic beams which form one frame, and the formation of an image for one frame from received signals which correspond to the ultrasonic wave transmission.

[0096] Also in the third embodiment, following the imaging of a marking frame, imaging for no-marking frames is carried out continuously, and imaging for another marking frame is carried out after such a time length that the flow range is present within the view field, with these operations being repeated.

[0097] Providing a time difference, which is based on the heart beat, between the timing of ultrasonic transmission for a marking frame at the strength for the dispersion of contrast agent and the timing of ultrasonic transmission for the next marking frame at the strength for the dispersion of contrast agent enables the proper observation of a pulsing flow. The time difference based on the heart beat may be a multiple of the period of heart beat measured with an electrocardiograph, or may be a multiple of an approximate heart beat period (e.g., 1 second).

[0098] FIG. 11 is an explanatory diagram of an image produced by the ultrasonic diagnostic apparatus of the third embodiment.

[0099] The portions of marking frames where the contrast agent has dispersed (bold lines and black dots) seem to be a lattice of the black void.

[0100] The ultrasonic diagnostic apparatus based on the third embodiment presents stripe patterns in both the direction orthogonal to the direction of sonic beams and the direction of flow which is virtually parallel to the direction of sonic beams (i.e., in a shape of lattice) as shown in FIG. 11, whereby it becomes possible to visually recognize at a glance the time-wise change of particularly a two-dimensional flow in the cardiac ventricle and atrium.

[0101] Many widely different embodiments of the invention may be configured without departing from the spirit and the scope of the present invention. It should be understood that the present invention is not limited to the specific embodiments described in the specification, except as defined in the appended claims.

1. A method of ultrasonic imaging comprising the steps of:

transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for other sonic beams; and

producing an image for one frame from received signals which correspond to the ultrasonic wave transmission.

2. The method of ultrasonic imaging comprising the steps of:

transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame;

producing an image for one frame from received signals which correspond to the ultrasonic wave transmission; and

interposing the formed frame between frames which are produced by the ultrasonic imaging method of claim 1.

3. The method of ultrasonic imaging of claim 2, wherein one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

4. The method of ultrasonic imaging of claim 1, wherein there are in one frame at least two spaced-out sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

5. A method of ultrasonic imaging comprising the steps of:

transmitting an ultrasonic wave at such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from the ultrasonic probe and transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for other depths; and

producing an image for one frame from received signals which correspond to the ultrasonic wave transmission.

6. The method of ultrasonic imaging comprising the steps of:

transmitting an ultrasonic wave at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame;

producing an image for one frame from received signals which correspond to the ultrasonic wave transmission; and

interposing the formed frame between frames which are produced by the ultrasonic imaging method of claim 5.

7. The method of ultrasonic imaging of claim 6, wherein one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

8. The method of ultrasonic imaging of claim 5, wherein there are in one frame at least two spaced-out positions of depths for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

9. The method of ultrasonic imaging comprising the step of:

combining an ultrasonic imaging method set forth in any of claim 1 through claim 4 and an ultrasonic imaging method set forth in any of claim 5 through claim 8.

10. An ultrasonic diagnostic apparatus by comprising:

an ultrasonic probe;

transmission/reception means for transmitting an ultrasonic wave from said ultrasonic probe and for receiving a signal which corresponds to the ultrasonic wave transmission;

transmission strength control means for controlling the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and have such a strength as not to disperse the contrast agent for other sonic beams; and

image producing means for producing an image for one frame from the received signals.

11. The ultrasonic diagnostic apparatus of claim 10, wherein said transmission strength control means controls the ultrasonic wave transmission such that one frame, which is formed by the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, is interposed between frames which are formed by the ultrasonic wave transmission at such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for other sonic beams.

12. The ultrasonic diagnostic apparatus of claim 11, wherein said transmission strength control means controls the ultrasonic wave transmission such that one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

13. The ultrasonic diagnostic apparatus of claim 10, wherein said transmission strength control means controls the ultrasonic wave transmission such that there are in one frame at least two spaced-out sonic beams for which an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

14. An ultrasonic diagnostic apparatus comprising:

an ultrasonic probe;

transmission/reception means for transmitting an ultrasonic wave from said ultrasonic probe and for receiving a signal which corresponds to the ultrasonic wave transmission;

transmission strength control means for controlling the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from said ultrasonic probe and have such a strength as not to disperse the contrast agent for other depths; and

image producing means for producing an image for one frame from the received signals.

15. The ultrasonic diagnostic apparatus of claim 14, wherein said transmission strength control means controls the ultrasonic wave transmission such that one frame, which is formed by the ultrasonic wave transmission at such a strength as not to disperse the contrast agent for all of a number of sonic beams which form one frame, is interposed between frames which are formed by the ultrasonic wave transmission at such a strength as to disperse the contrast agent for a certain depth of a number of sonic beams which form one frame or a certain depth seen from an ultrasonic probe and at such a strength as not to disperse the contrast agent for other depths.

16. The ultrasonic diagnostic apparatus of claim 15, wherein one timing of ultrasonic wave transmission for one frame at such a strength as to disperse the contrast agent and another timing of ultrasonic wave transmission for a later frame at such a strength as to disperse the contrast agent have a time difference which is based on the heart beat.

17. The ultrasonic diagnostic apparatus of claim 14, wherein said transmission strength control means controls the ultrasonic wave transmission such that there are in one frame at least two spaced-out positions of depths for which

an ultrasonic wave is transmitted at such a strength as to disperse the contrast agent.

18. An ultrasonic diagnostic apparatus comprising:

an ultrasonic probe;

transmission/reception means for transmitting an ultrasonic wave from said ultrasonic probe and for receiving a signal which corresponds to the ultrasonic wave transmission;

transmission strength control means for controlling the ultrasonic wave transmission to have such a strength as to disperse the contrast agent for part of a number of sonic beams which form one frame and have for other sonic beams such a strength as to disperse the contrast agent for a certain depth of the sonic beams or a certain depth seen from an ultrasonic probe and such a strength as not to disperse the contrast agent for other depths; and

image producing means for producing an image for one frame from the received signals.

\* \* \* \* \*

专利名称(译)	超声成像方法和超声诊断设备		
公开(公告)号	<a href="#">US20010021810A1</a>	公开(公告)日	2001-09-13
申请号	US09/777984	申请日	2001-02-06
[标]申请(专利权)人(译)	桥本HIROSHI		
申请(专利权)人(译)	桥本HIROSHI		
当前申请(专利权)人(译)	桥本HIROSHI		
[标]发明人	HASHIMOTO HIROSHI		
发明人	HASHIMOTO, HIROSHI		
IPC分类号	A61B8/00 A61B8/06 A61B8/14 G01S7/52 G01S15/89		
CPC分类号	A61B8/06 A61B8/481 G01S7/52038 G01S7/52041 G01S7/52066 G01S7/52073 G01S15/8979		
优先权	2000063853 2000-03-08 JP		
其他公开文献	US6464644		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

超声波诊断装置以这样的强度发射超声波，以便将造影剂分散成多个声束的一部分，所述声束形成一个帧并且其强度使得不会将造影剂分散到其他声束中从而产生图像。对于来自超声波传输的接收回波信号的标记帧，随后连续发射超声波，其强度使得不会使所有声波束的造影剂分散，从而连续产生无标记帧的图像，并且在这样的时间之后视野中存在流量范围的长度，为另一个标记帧生成图像。重复这些操作以显示超声图像，通过该超声图像可以一目了然地识别血流的时间变化。

