



US 20080146943A1

(19) **United States**

(12) **Patent Application Publication**
Jenkins et al.

(10) **Pub. No.: US 2008/0146943 A1**
(43) **Pub. Date: Jun. 19, 2008**

(54) **INTEGRATED BEAM FORMER AND ISOLATION FOR AN ULTRASOUND PROBE**

(22) Filed: **Dec. 14, 2006**

Publication Classification

(75) Inventors: **David A. Jenkins**, Flanders, NJ (US); **Charles Bryan Byrd**, Medford, NJ (US); **Praveen Dala-Krishna**, Sicklerville, NJ (US)

(51) **Int. Cl.**
A61B 8/00 (2006.01)
(52) **U.S. Cl.** **600/466**

(57) **ABSTRACT**

Correspondence Address:
HANSEN HUANG TECHNOLOGY LAW GROUP, LLP
1725 EYE STREET, NW, SUITE 300
WASHINGTON, DC 20006

A compact, portable ultrasound imaging system includes a combination of an isolation circuit, an ultrasound signal generator, and a beam former within a single unit. The isolation circuit may limit unintended, leakage current from the ultrasound system through the transducer array of the ultrasound system. The signal generator and beam-former may be implemented using large scale integration semiconductor chips. Connections are provided for connecting an ultrasound transducer array, for outputting ultrasound data and for receiving user input and commands.

(73) Assignee: **EP MedSystems, Inc.**, West Berlin, NJ (US)

(21) Appl. No.: **11/610,778**

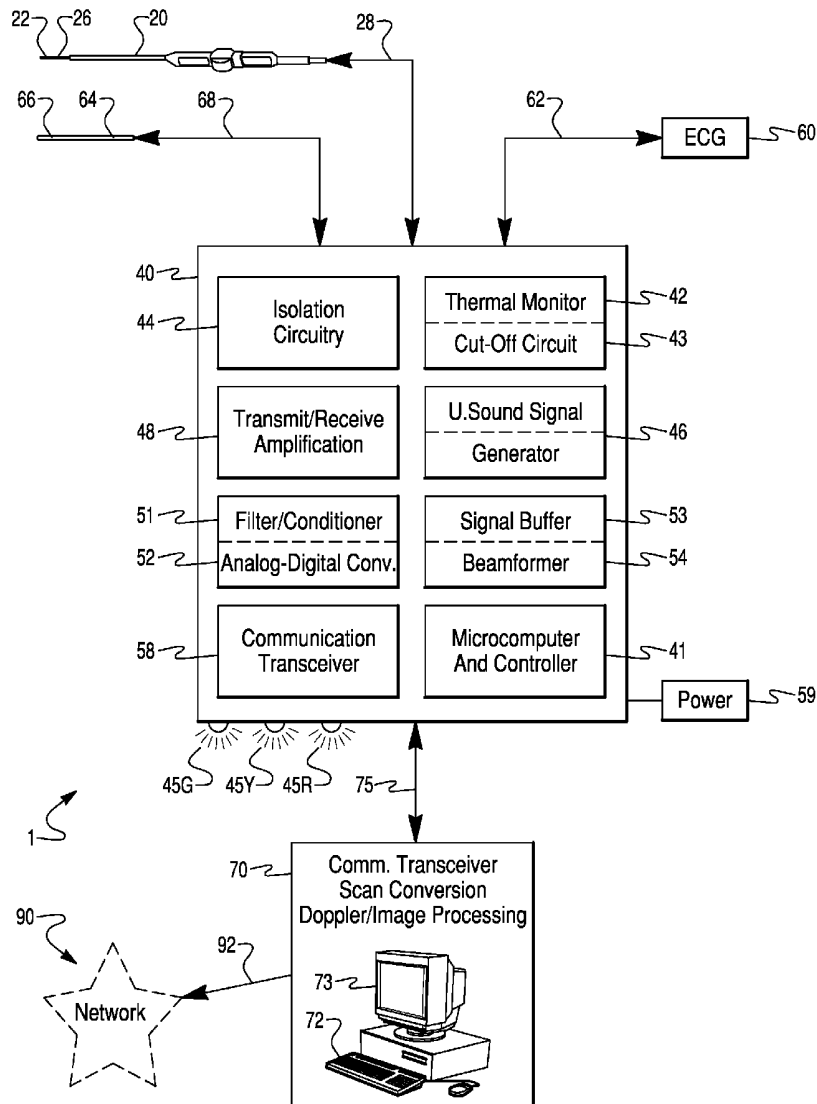


Fig. 1A

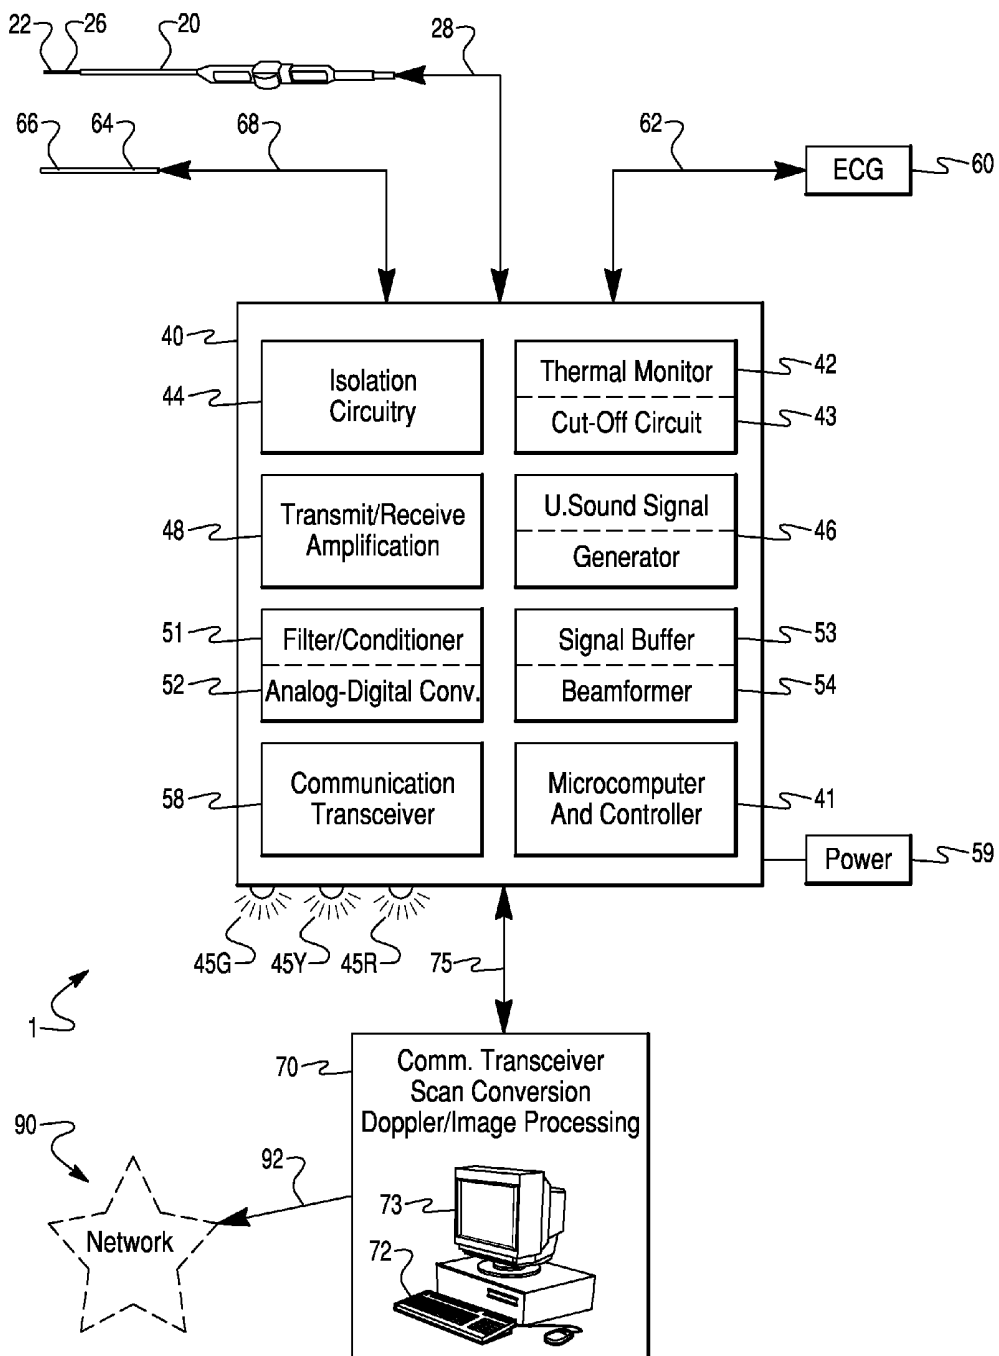


Fig. 1B

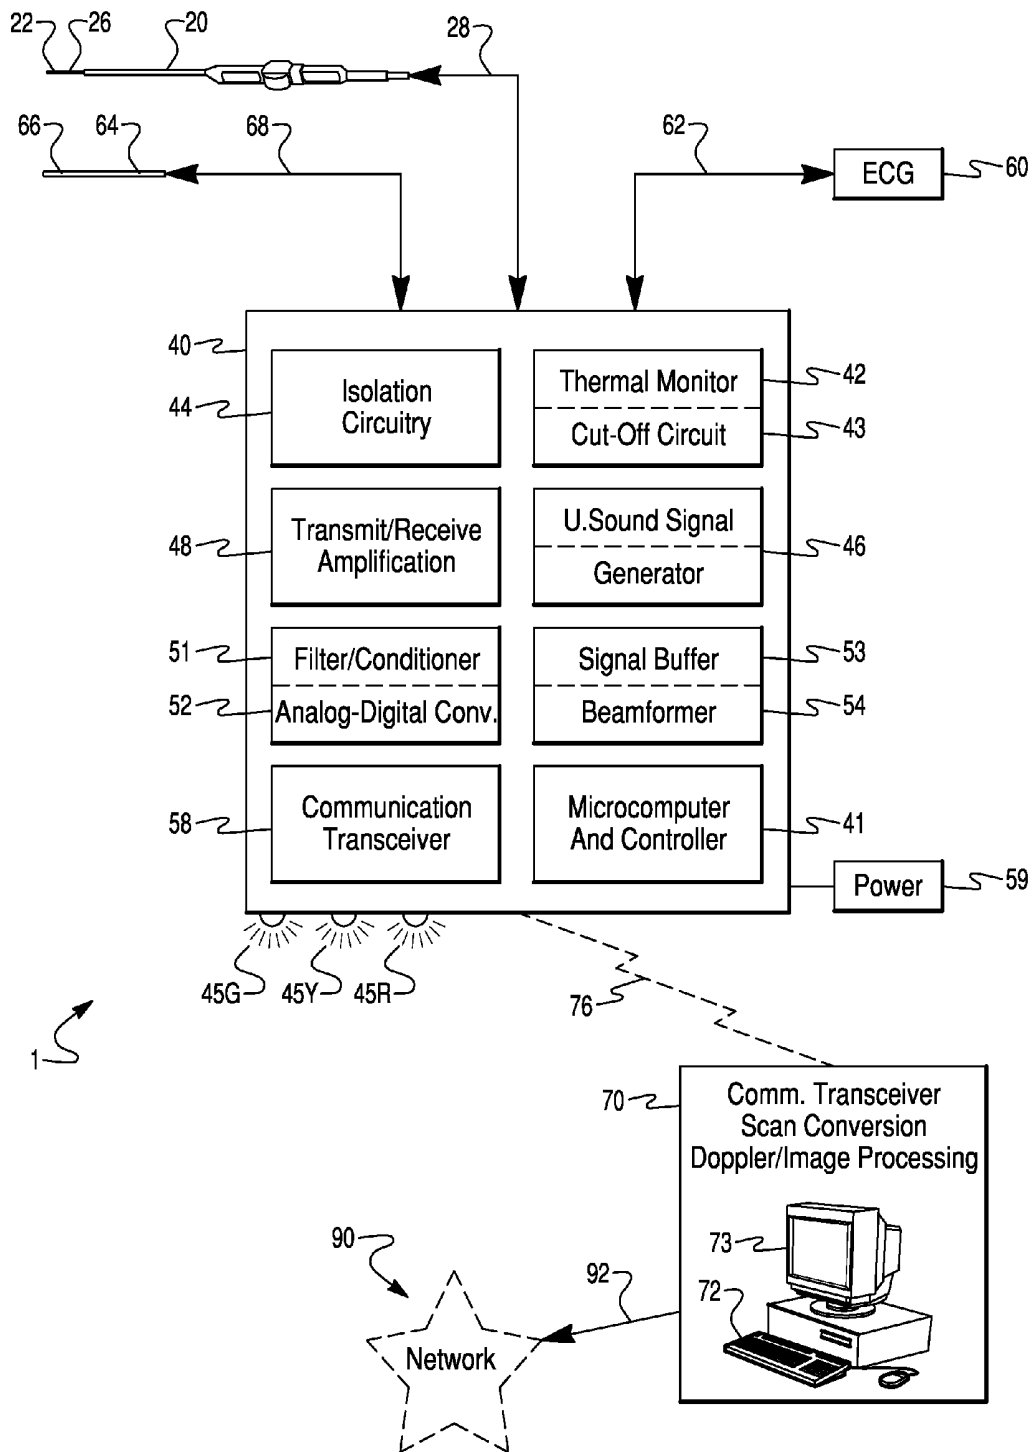


Fig. 2

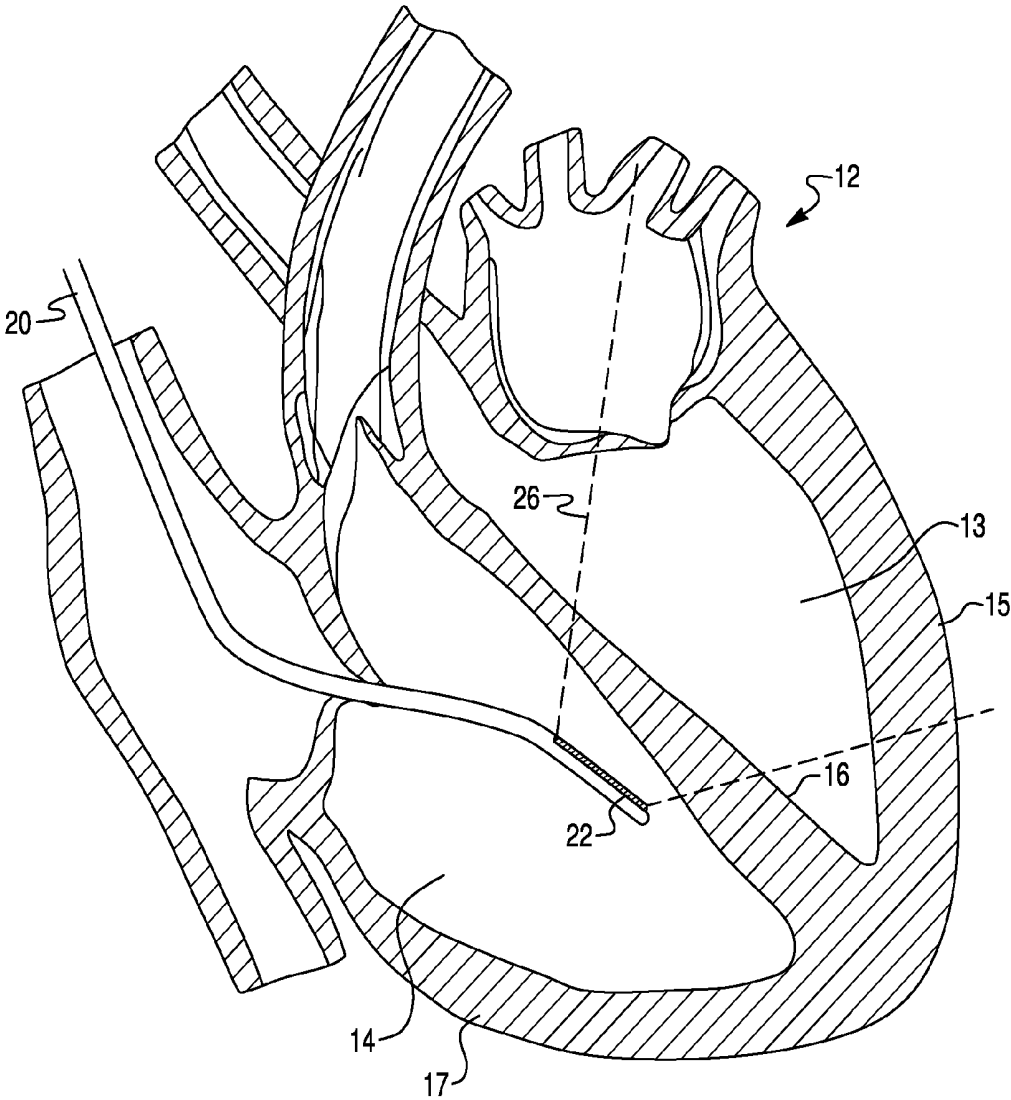


Fig. 3

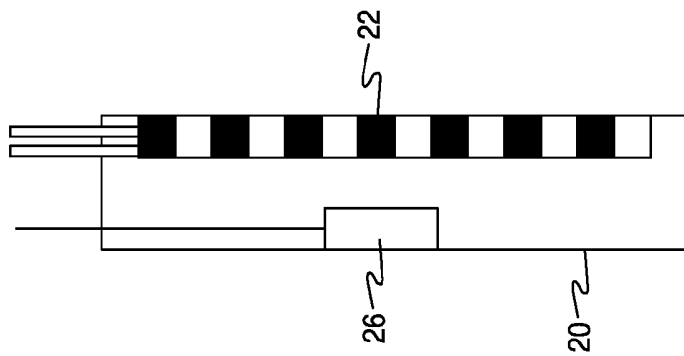


Fig. 4

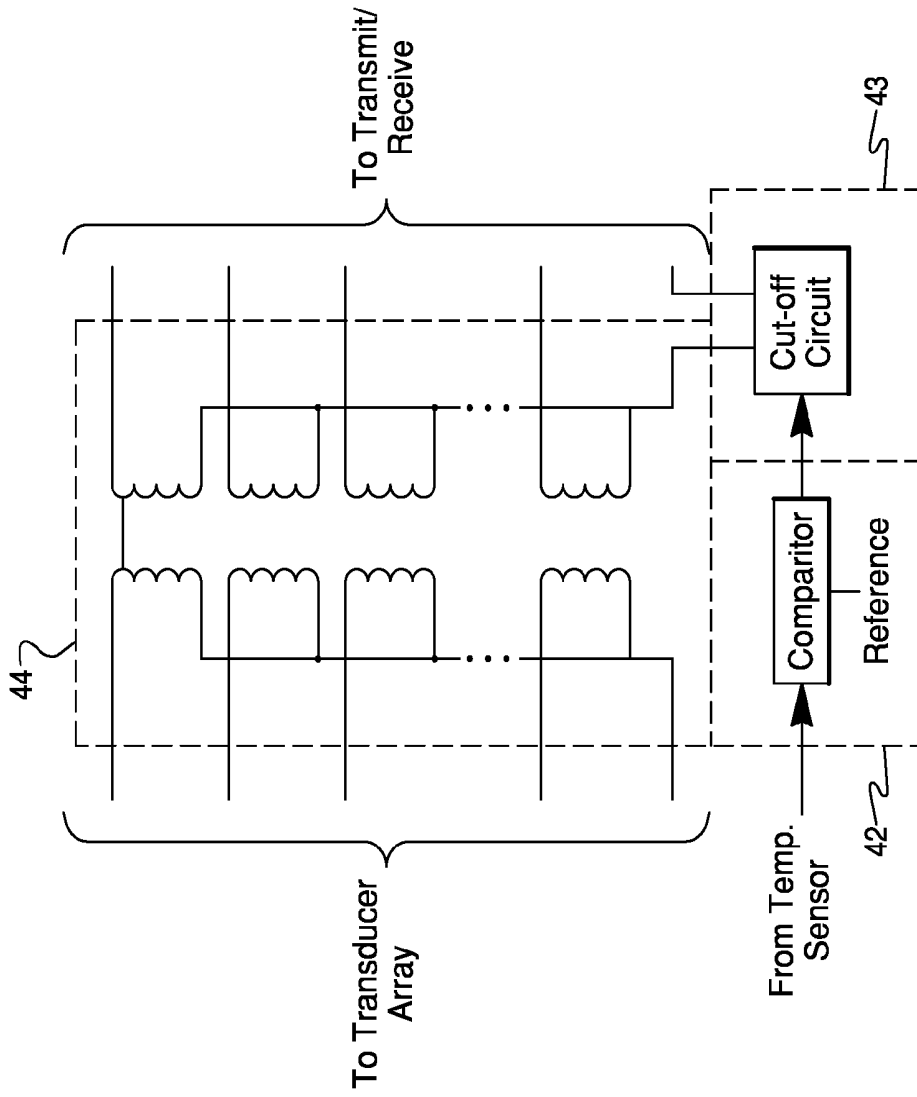


Fig. 5

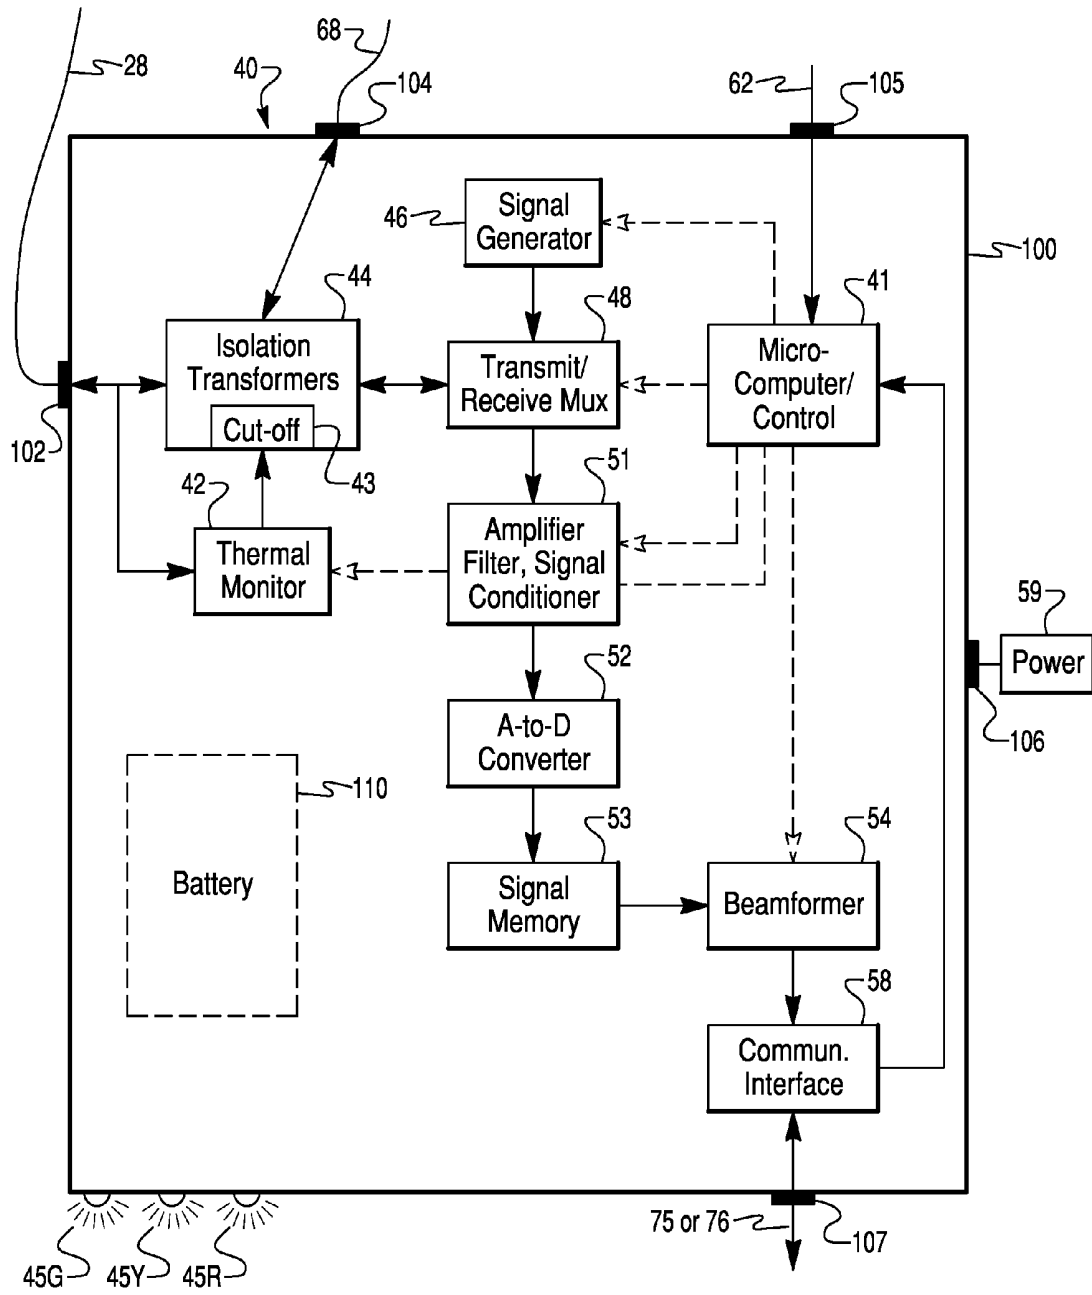


Fig. 6

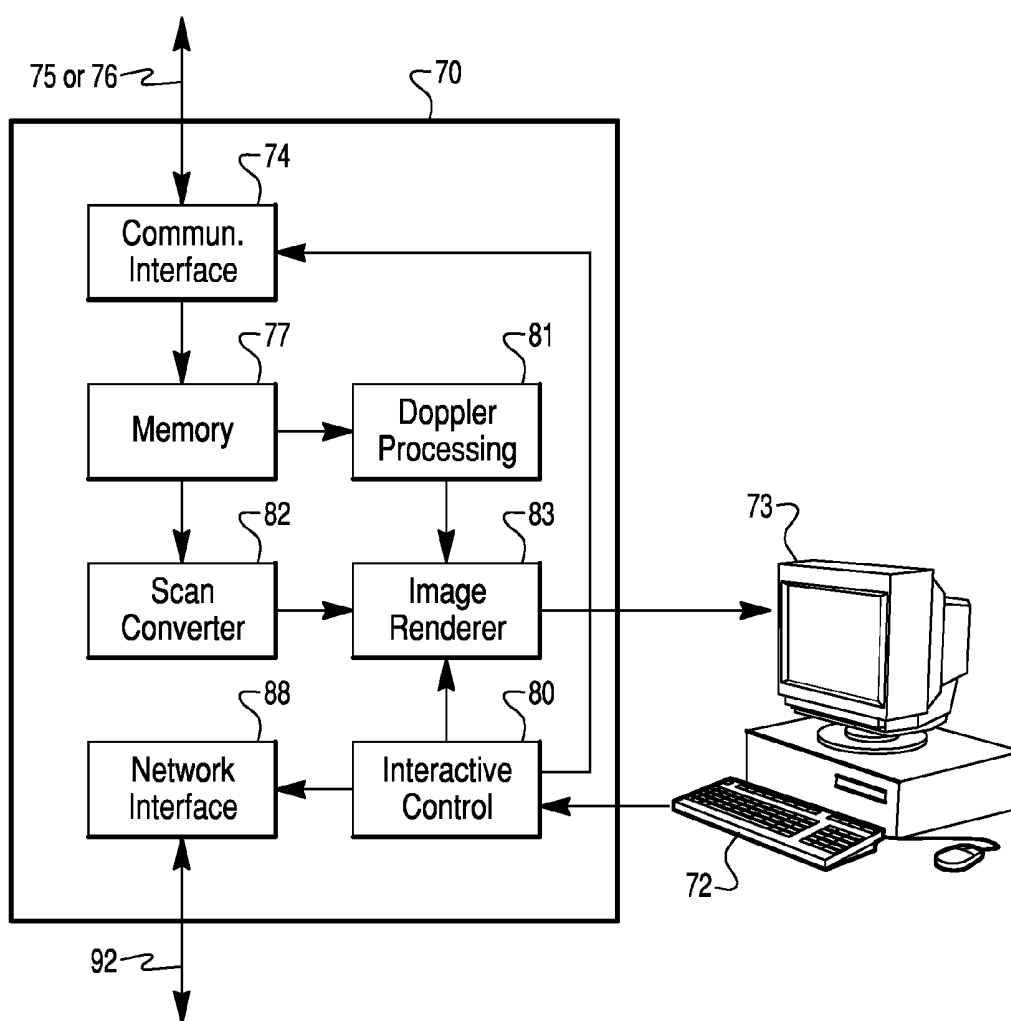


Fig. 7


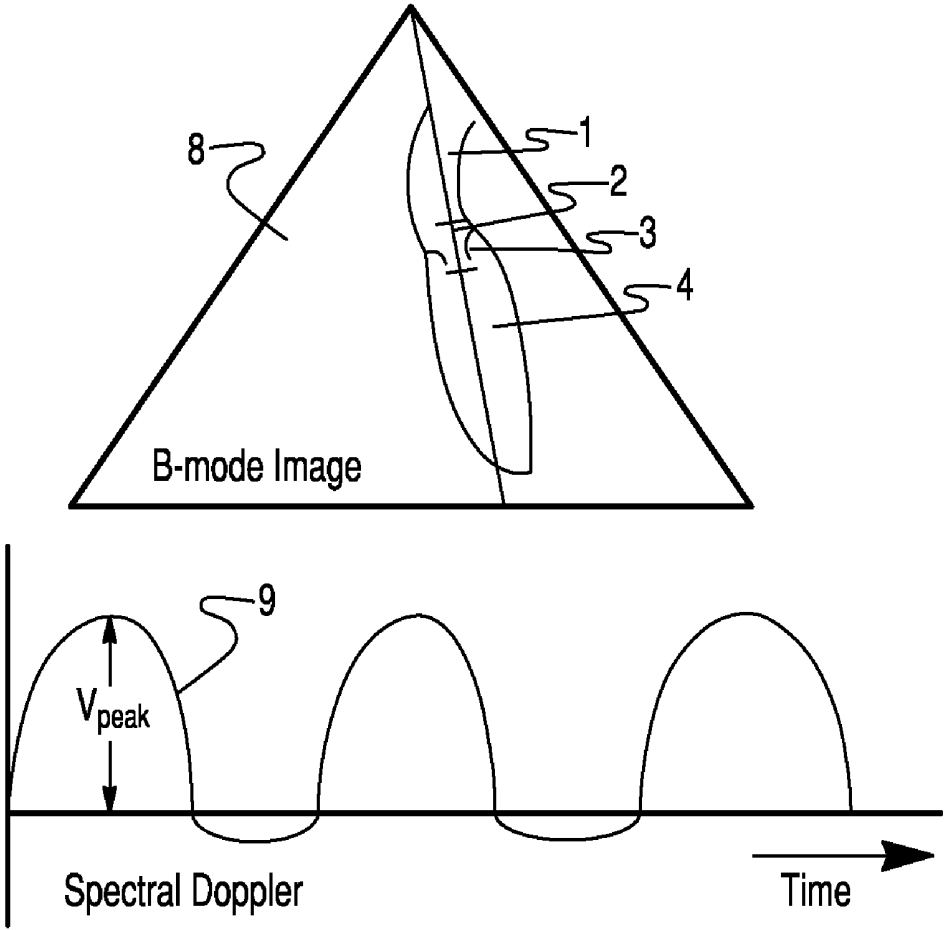


Fig. 9

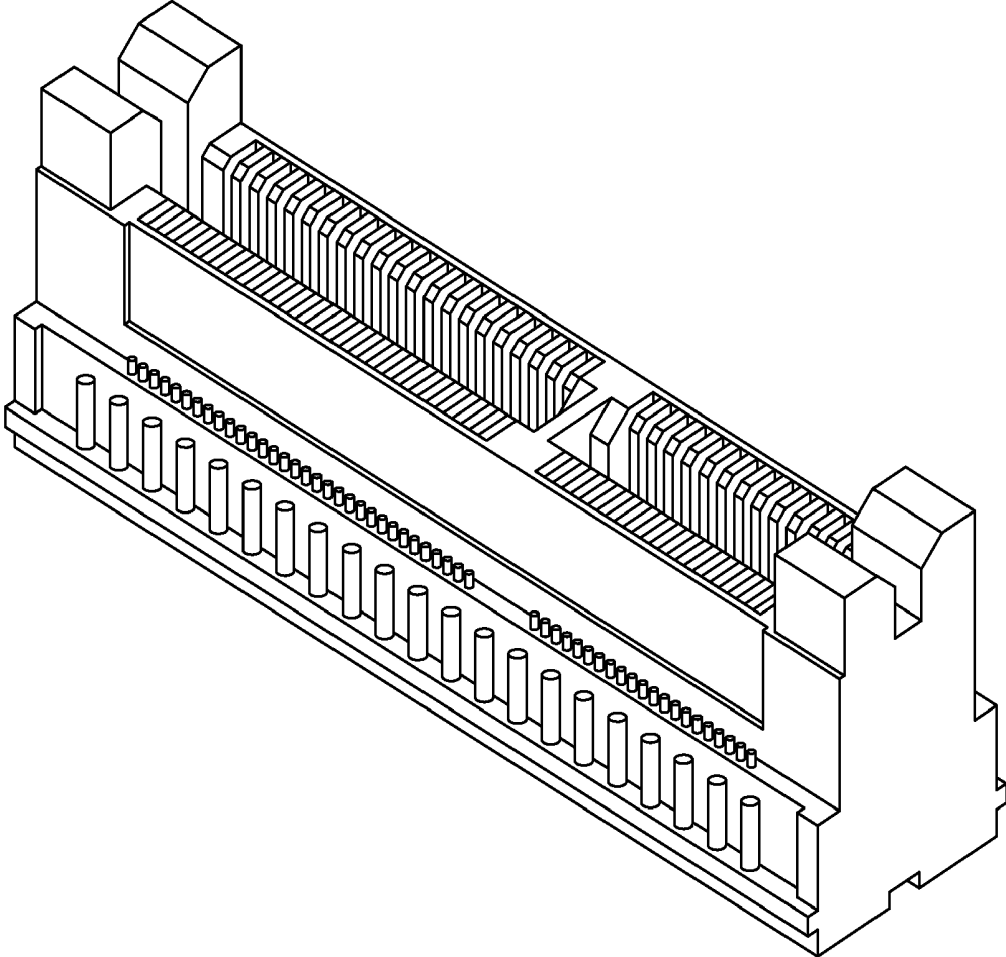

INTEGRATED BEAM FORMER AND ISOLATION FOR AN ULTRASOUND PROBE

FIELD OF THE INVENTION

[0001] The present invention is a medical diagnostic system and method, and more particularly is directed to a compact ultrasound imaging catheter system.

BACKGROUND OF THE INVENTION

[0002] Recent advancements in miniaturization of ultrasound technology has enabled the commercialization of catheters including phased array ultrasound imaging transducers small enough to be positioned within a patient's body via intravenous cannulation. By imaging vessels and organs, including the heart, from the inside, such miniature ultrasound transducers have enabled physicians to obtain diagnostic images available by no other means.

[0003] While ultrasound imaging catheter systems have proven to be invaluable diagnostic tools, the associated cabling and equipment present difficulties for clinicians. For example, the cabling from the ultrasound system to the catheter's proximal connector is heavy, stiff, and limited in length. The length of the cabling required to reach from the ultrasound system to the patient can act as an antenna introducing electronic noise induced from stray electromagnetic radiation in the examination room. The large cart which normally contains the ultrasound system takes up space in the operating room or catheterization lab, and may be difficult to position next to the patient.

SUMMARY OF THE INVENTION

[0004] The present invention is directed toward providing compact, portable ultrasound systems which can improve imaging performance and enhance safety—particularly in connection with intrabody, percutaneous ultrasound probes, such as catheters and endoscopes containing ultrasound transducer arrays.

[0005] An embodiment of the present invention includes a compact, integrated ultrasound pulse generation, beam forming, and electrical isolation unit with connectors for connecting to one or more ultrasound transducer arrays and an image display unit. Any ultrasound transducer array may be connected to the unit. In an embodiment, the ultrasound transducer array is one intended for intrabody use, and in a particular embodiment is a catheter-based ultrasound phased array transducer.

[0006] The integrated ultrasound pulse generation, beam forming, and electrical isolation unit includes the circuitry for generating ultrasound pulses provided to the ultrasound transducer array and for receiving and processing signals received from the ultrasound transducer array. The unit further includes circuitry for communicating the processed ultrasound images to an external image processing and display unit via standard data transmission cables or a wireless data link. The image processing and display unit generally includes a digital processor, memory, and a graphics screen. A conventional laptop computer can embody this image processing and display unit for the present invention. The transducer array can be connected to the ultrasound unit by a multi-conductor electrical cable. The integrated ultrasound pulse generation, beam forming and electrical isolation unit can include electrical isolation components, such as bi-directional optical isolation integrated circuits. Power for the inte-

grated ultrasound pulse generation, beam forming, and electrical isolation unit can be supplied via a cable, such as a data cable with power conductors, from a separate power connector, or from a self contained power source, such as batteries.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] The accompanying drawings, which are incorporated herein and constitute part of this specification, illustrate exemplary embodiments of the invention, and, together with the general description given above and the detailed description given below, serve to explain features of the invention.

[0008] FIG. 1A is a block diagram of an embodiment of the present invention.

[0009] FIG. 1B is a block diagram of another embodiment.

[0010] FIG. 2 is an illustration of an intra-cardiac catheter located in the right ventricular cavity.

[0011] FIG. 3 is a diagram of a catheter transducer array with temperature sensor.

[0012] FIG. 4 is a schematic of the isolation and temperature monitoring circuit according to an embodiment.

[0013] FIG. 5 is a block diagram of an ultrasound unit of an embodiment.

[0014] FIG. 6 is a block diagram of an image processing computer of an embodiment.

[0015] FIG. 7 is a sample display of an ultrasound image from a cardiac ultrasound transducer.

[0016] FIG. 8 is block diagram of another embodiment.

[0017] FIG. 9 is an illustration of an example connector for an embodiment.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

[0018] Various embodiments of the present invention will be described in detail with reference to the accompanying drawings. Wherever possible, the same reference numbers will be used throughout the drawings to refer to the same or like parts.

[0019] As used herein, the terms “about” or “approximately” for any numerical values or ranges indicate suitable dimensional tolerances that allow the part or collection of components to function for their intended purposes as described herein. Also, as used herein, the terms “patient”, “host”, and “subject” refer to any human or animal subject and are not intended to limit the systems or methods to human use. Further, embodiments of the invention will be described for use with an intracardiac ultrasound transducer array catheter. However, the embodiments may be applicable to any medical ultrasound transducer.

[0020] The equipment and cabling historically associated with ultrasound imaging present ergonomic challenges for clinicians. For example, the cabling from the conventional ultrasound machine to the catheter's proximal connector is heavy, stiff, and limited in length. The large cart which normally contains the ultrasound system occupies valued space in the operating room or catheterization lab, and positioning the cart close to the patient may restrict where or how staff or equipment may be stationed. The long cable required to reach from the ultrasound system to the patient can be a source of electronic noise as it may act as an antenna that can pick up stray electromagnetic radiation, such as from utility power and nearby computers, power supplies, displays, pulse gen-

erators, and other equipment. Further, maintaining sterility of the cable connects a non-sterile system with a sterile instrument is a persistent concern.

[0021] To overcome such challenges, various embodiments separate the ultrasound generation and beam-forming circuitry from the image display portion of the system, reduce the size of the ultrasound generation and beam-forming, and integrate the circuitry with electrical isolation circuitry. The result of these innovations is a small, reusable ultrasound unit which houses at least the signal generation, beam-forming, and isolation circuitry in a package can be located adjacent to the patient. As a result, the cable from the ultrasound unit to the catheter can remain relatively short and potentially single-use which may make it easier to keep sterile. Then a lighter weight, inexpensive, disposable cable or a wireless communication interface can connect the ultrasound unit to the image display unit of the system. A shorter cable will be less likely to introduce electronic noise induced by stray electromagnetic radiation. Unlike a conventional ultrasound cart, the small ultrasound unit can be sterilized or placed into a sterile enclosure (e.g., a sterile plastic bag), and the image display unit of the system may be positioned at any convenient location, such as on the bed next to the patient or even on the patient.

[0022] The block diagram in FIG. 1A illustrates main elements of an example embodiment. The embodiment includes an ultrasound transducer array 22 carried by or positioned on a catheter 20 coupled to an ultrasound unit 40 by a signal cable 28. The ultrasound unit 40 is connected to a display, such as a display unit 70, by a wired data interface 75 or a wireless data interface 76 (shown in FIG. 1B).

[0023] A signal cable 28 delivers ultrasound signals from ultrasound unit 40 to each of the transducers in the array 22. Typically, the signal cable 28 will include at least one wire per transducer, and in an embodiment, includes a coaxial cable connected to each transducer in the array 22. In an alternative embodiment, the signal cable 28 includes fewer wires than transducers and a multiplexer circuit (not shown) configured to enable signals to and from the plurality of transducers over the wires. Typically, the signal cable 28 includes an electrical connection plug (e.g., a standard connector) on the proximal end. Providing a plug connector on the end of the cable 28 allows completion of the many electrical connections between the cable conductors and the ultrasound unit 40 since the connection by pressing the plug into a complementary connector in the housing 100 of the ultrasound unit 40.

[0024] The transducers in the array 22 convert the electrical signals from the ultrasound unit 40 into sound waves, which propagate into a portion of a patient's anatomy, such as the heart. The same transducer array 22 also receives ultrasound echoes reflected from anatomic structures and transforms the received sound into electrical signals (e.g., by means of the piezoelectric effect). These electrical signals are conducted via cable 28 back to the ultrasound unit 40.

[0025] The ultrasound unit 40 may include a housing or chassis with exterior connectors for connecting cables to other elements of the embodiment. Ultrasound unit 40 may contain optical and electronic circuitry implementing some or all of the elements described in the following paragraphs. The component elements and interconnecting circuitry of ultrasound unit 40 may include one or more large scale integrated circuits such as VLSI, ASIC, and FPGA chips mounted on one or more circuit boards which are coupled to the connectors.

[0026] Signal generator 46 generates electrical signals of ultrasonic frequencies to be provided to the ultrasound transducer array 22. The signal generator 46 can be configured to produce signals of particular wave forms, frequencies and amplitudes as desired for imaging tissue. The signal generator 46 may also be configured to generate signals with the necessary phase lag to enable the transducer array to generate a focused and steerable sound beam as well known in the art of imaging ultrasound phased array transducers. Alternatively, phase lag may be added by another circuit, such as a beam former circuit 54.

[0027] A transmit/receive multiplexer circuits 48 can be included to direct the signals generated by the generator 46 to isolation circuitry 44 and to separate out echo signals returned from isolation circuitry 44 from the generated signals.

[0028] Isolation circuitry 44 isolates unintended, potentially unsafe electrical currents and voltages from the transducer array 22 which contacts the patient. Examples of suitable isolation circuits are described in U.S. patent application Ser. No. 10/997,898 "Method And Apparatus For Isolating A Catheter Interface", published as U.S. Patent Publication No. 2005/0124898 to Borovsky et al filed on Nov. 29, 2004, the entire contents of which are hereby incorporated by reference. An example of such safety methods and systems is embodied in the ViewMate® catheter ultrasound system from EP MedSystems, Inc. of West Berlin, N.J.

[0029] A thermal monitoring circuit 42 and a cut-off circuit 43 may be included to mitigate possible risks to the patient that can result from excessive local heating by ultrasound. For example, the thermal monitoring circuit 42 may be connected to a temperature sensor (not shown), such as a thermoresistor ("thermistor") positioned on the catheter near the transducer array 22. The thermal monitoring circuit 42 is preferably configured to determine from signals received from the temperature sensor when tissue temperatures in the vicinity of the transducers exceed a safe threshold value and to trigger a safety action when the threshold is exceeded. The safety action may be the output of a cut-off signal to a cut-off circuit 43 which is configured to shut off the signal generation, disconnect transmit circuits from the transmission cable 28, or otherwise discontinue the transmission of ultrasound pulses to the transducer array 22 in response to a cut-off signal. Examples of suitable temperature sensors, thermal monitor circuits and cut off circuits are provided in U.S. patent application Ser. No. 10/998,039 entitled "Safety Systems And Methods For Ensuring Safe Use Of Intra-Cardiac Ultrasound Catheters" published as U.S. Patent Publication No. 2005/0124899 to Byrd et al filed on Nov. 29, 2004, the entire contents of which are hereby incorporated by reference.

[0030] In an embodiment, the thermal monitor circuit 42 is configured to monitor intra-cardiac temperatures as sensed by a thermistor on the catheter, and to transmit to the display unit 70 a temperature value that may be displayed on a monitor. The thermal monitor circuit 42 in such an embodiment may calculate the intracardiac temperature value and transmit this value as digital data to the display unit 70. The thermal monitor circuit 42 may also be configured to transmit a warning when the measured intracardiac temperature exceeds a threshold, such as a temperature that is elevated but still safely below a level at which tissue damage may occur. Such a warning would inform clinicians of a potentially hazardous condition to permit them to take actions to reduce heating, such as adjusting ultrasound power or duty cycle parameters,

in order to avoid damaging tissue and automatic shutoff by the cut-off circuit 43. Such a warning may be transmitted to the display unit 70 as digital data for display on the monitor.

[0031] In another embodiment, a display, such as colored light emitting diode (LED) indicators (45G, 45Y, 45R) on the ultrasound unit 40 are provided to indicate temperature information, in the alternative or in addition to displays on the display unit 70. For example, in such an embodiment three LEDs may be provided, such as a green LED 45G to indicate a safe detected intracardiac temperature, a yellow LED 45Y to indicate an elevated but marginally safe intracardiac temperature, and a red LED 45R to indicate an unsafe or near unsafe intracardiac temperature. In such an embodiment, the thermal monitor circuit 42 includes circuits configured to light the appropriate colored LED based upon the measured intracardiac temperature. This configuration may be accomplished by the thermal monitor circuit 42 testing the sensed temperature against two threshold values, wherein the first threshold corresponds to elevated but still safe intracardiac temperatures and the second threshold corresponds to unsafe or near unsafe intracardiac temperatures. Thus, the thermal monitor circuit can be configured (e.g., with digital switches) to power (i.e., direct a voltage to) the green light emitting diode in response to the temperature input signal indicating a sensed temperature less than the first threshold, power the yellow light emitting diode in response to the temperature input signal indicating a sensed temperature greater than the first threshold but less than the second threshold, and power the red light emitting diode in response to the temperature input signal indicating a sensed temperature greater than the second threshold.

[0032] A filter and conditioner circuit 51 can be included in the ultrasound unit 40 to reject spurious signals that may be induced in or through cable 28.

[0033] An analog-to-digital converter (ADC) 52 can be included in the ultrasound unit 40 to frequently sample and convert the ultrasound signals from analog electrical levels to discrete digital numeric values.

[0034] A signal buffer 53 can be included to store at least a portion of the echo signals, which are returned from the transducer array 22 and which may be processed by other elements of the ultrasound unit 40. In an embodiment, a signal buffer 53 is included to store the echo signals as digital data in a random-access semiconductor memory (RAM).

[0035] Beam former 54 circuits may be included to process signals sent to and received from the transducer array 22 to enable phased-array ultrasound imaging. The beam former 54 may receive ultrasound signals from the signal generator 46 and introduce phase lags for each transducer element so that when the signals are applied to the transducer elements a narrow beam of sound emanates from the array. Also, the beam former 54 may receive signals from the transducer array and process the ultrasound echo signal data to calculate the amplitude and direction of the ultrasound echoes returned to the transducer array 22 from each of many specific angles and distances. The beam former 54 may also determine the frequency or Doppler frequency shift of the signal returned from each of selected angles and distances from the transducer array 22.

[0036] A communications transceiver 58 may be included to prepare ultrasound data for transmission out of ultrasound unit 40, typically in digital form. The communication transceiver 58 may also receive data and commands from outside the ultrasound unit 40 and convert such signals to a form

usable by the ultrasound unit 40. Data transmission may be any high speed (e.g., gigabit per second) data link, such as Ethernet.

[0037] In an embodiment, the communications transceiver 58 may include data encoding or compression capability, such as a microprocessor programmed with data encoding or compression software, so that the ultrasound data can be transmitted in a compressed format. By transmitting data in a compressed format, lower bandwidth communication links (e.g., cable or wireless data link) can be used to transmit data, or more data can be transmitted over a standard cable or wireless data link. Additionally, the control unit 41 or other modules may be configured to filter out data that need not be transmitted, such as signals or data pixels containing little or no data (i.e., pixels where little or no echoes were received), so such data need not be transmitted. In yet a further embodiment, the communications transceiver 58 may include temporary storage capability (e.g., random access memory) and be configured to manage the transmission of data at a maximum data rate consistent with the communication link even when data provided to the transceiver exceeds the maximum data rate. Suitable circuitry and software for encoding, compressing, buffering and filtering data and managing data transmission are well known in the communications arts.

[0038] The ultrasound unit may include a control unit 41 which may be a microcontroller, a microprocessor, a microcomputer, or other controller circuitry (such as programmable firmware or a programmable gate array). The control unit 41 may be configured to coordinate the activity and functionality of the various elements included in the ultrasound unit 40.

[0039] In an embodiment associated with cardiac imaging, the ultrasound unit 40 may also include electrical connections for receiving signals from electrocardiogram (ECG) electrodes and for passing such signals on to an external electrocardiogram (ECG) unit 60 which may be connected to the ultrasound unit 40 through a communications interface 62. The communications interface 62 may be any wired or wireless interface. In an embodiment, the ECG electrodes can be an intracardiac ECG catheter 64 which includes one or more electrodes 66 near a distal end for sensing electrical activity in the heart. Electrical signals sensed by the electrodes 66 can be conveyed to the ultrasound unit 40 by means of an extension of the catheter 64 or a connecting cable 68. In various embodiments, the ECG catheter 64 is connected to the isolation circuitry 44 which isolates the patient from stray or fault voltage from the external ECG equipment 60. In an embodiment, signals sent by the ECG 60 through the interface 62 can be recorded or used to synchronize received ultrasound image data with the heartbeat of the patient. For example, a sequence of images may be associated with a sequence of ECG readings revealing the phases of the cardiac cycle, or images may be captured only at a specified phase of the cardiac cycle.

[0040] In an embodiment in which the ultrasound unit 40 may be packaged within a single housing (see FIGS. 5 and 8) or chassis, the whole unit 40 may be fabricated of components which can withstand a sterilization method. Sterilization methods include subjecting the unit 40 to gas, liquids, heat (dry or steam), radiation, or other known methods. Alternatively, or in addition, the unit 40 may be enclosed in an externally sterile enclosure, such as a plastic bag, with provision for connecting cables through the plastic bag to the unit 40. For example, the connectors may be designed so that the pins of the connector of an external electrical cable (such as

cable 28) are designed to puncture the externally sterile plastic bag locally when mating with the corresponding connector of the unit 40 inside the plastic bag.

[0041] The relationship, function, and interaction of the elements which may be contained in the ultrasound unit 40 of an embodiment will be described further with reference to FIGS. 5 and 8.

[0042] In FIG. 1, the image display unit 70 may be a computer, such as a laptop, which can be configured to perform more sophisticated image processing than is provided by the ultrasound unit 40. Such an embodiment will be described later (with respect to FIG. 6). In an alternative embodiment (which will be discussed later in relation to FIG. 8) image display computer may include a user input device 72, and a video monitor 73.

[0043] Optionally, there may be two (or more) separate communication interfaces 75: one interface for the ultrasound image data communicated to the display unit 70, and a second interface (not shown in FIG. 1A) for communicating configuration parameters and commands from the display unit 70 to the microcomputer 41. These two interfaces 75 may employ the same type of communication hardware and protocol standard or two different types.

[0044] In the embodiment illustrated in FIG. 1A, pixel-based, polar-coordinate oriented ultrasonic image data can be serialized and transmitted to the image display unit 70 over the data communication interface 75. The data interface 75 may be any one or more of several standard high-speed serial or parallel data communication protocols and hardware embodiments. Example embodiments of the serial communication interface 75 include Ethernet, Universal Serial Bus (USB 2.0), FireWire (IEEE-1394), RS-232, or any other existing or future high-speed (e.g., gigabit/second) wired communication interface. As with the communications transceiver 58, the data interface 75 may include circuitry and software for encoding, compressing, buffering and filtering data, as well as managing data transmission to enable the reliable transmission of a large amount of image data through communication links of limited bandwidth. Both the ultrasound unit 40 and the image display unit 70 can contain appropriate corresponding hardware and software communication drivers, data compression and encoders, buffer memory, and data filter circuits and/or software, which are readily available commercially, such as standard off-the-shelf integrated circuits or plug-in circuit cards and well known communication algorithms.

[0045] In an alternative embodiment, the data interface 75 may be an optical cable, such as one or more fiber optic cables. This embodiment is illustrated in FIG. 1A, with the communication transceiver 58 being an optical data link transceiver. Fiber optic data links well known in the art may be used in this embodiment.

[0046] In some embodiments, the communications transceiver 58 and/or the data interface 75 are configured to recognize the particular type of communication link connected to the ultrasound unit 40, and to adapt the communication protocols, data encoding and data transmission rates to match the connected link. Such embodiments may also include software programmed in the microcomputer 41 that enables it to supervise the ultrasound unit 40 consistent with the capabilities and requirements of the connected data link. In such embodiments, the ultrasound unit 40 may include a number of different connection ports for various communication links, such as two or more of a USB port, a FireWire port, a serial

data port, a parallel data port, a telephone band modem and RJ-11 port, a WiFi wireless data link and a BlueTooth wireless data link, for example. Circuitry and/or software operating in the communication modules or microprocessor 41 can be configured to sense when a particular one of the various accommodated communication links is connected, such as by sensing an electrical or radio frequency signal received by the link. Recognizing that a particular link is connected, the communications transceiver 58 and/or the data interface 75 and/or microprocessor 41 can implement the protocol, data encoding and data transmission rate that corresponds to that link. Circuits and methods for recognizing connected data links and adjusting communications protocols accordingly are well known in the digital communication arts. Such embodiments provide flexibility of use, allowing users to connect displays and processors using available or convenient cables or communication links.

[0047] Functionality within the ultrasound unit 40 can be managed and timed by a programmed microcontroller, a microprocessor, a microcomputer 41, equivalent firmware, an ASIC chip, or discrete electronic circuitry, all of which are encompassed by description references to "microcomputer" herein. The microcomputer 41 can respond to configuration parameters and commands sent from the image display unit 70 over communication interface 75. Examples of such configuration parameters and commands include the frequency of the generated ultrasound signals, the mode of operation (continuous or pulsed), depth of imaging, angular width of the active image area, amplifier gain, filter frequencies, details about the transducer array 22 (number and arrangement of transducers), and so forth.

[0048] The hardware layout and software programming needed to implement the design and programming of the ultrasound unit 40 are typical and well known to electrical and software engineers skilled in this art. Similarly, the algorithms programmed into display unit 70 are known to software engineers skilled in mathematics, computer graphics, and graphical-interface operating systems.

[0049] The image display unit 70 can perform any number of several functions. The display unit 70 can process and display the image data provided by the ultrasound unit 40 on a connected monitor 73 or other display, such as a large plasma screen display (not shown) coupled to the display unit 70. The display unit 70 can transmit configuration parameters and control commands to the ultrasound unit 40, where the configuration parameters and commands may be supplied by the operator of the system 1 by means of interactive inputs from a pointing device (mouse or joystick) and keyboard attached to or part of the display unit 70. For example, the operator may inform the display unit 70 about the type of imaging catheter 20 which the display unit 70 may further translate into operational details about the transducer array 22 included in the imaging catheter 20.

[0050] In some embodiments, the image display unit 70 can convert the ultrasound data generated by the beam-former 54 (which may be relative to a transducer-centered polar coordinate system) into an image relative to another set of coordinates, such as a rectangular coordinate system. Such processing may not be necessary in display unit 70, if the conversion was already preformed in the ultrasound unit 40. Techniques for converting image data from one coordinate system into another are well-known in the field of mathematics and computer graphics.

[0051] The display unit **70** may display the rectangular image data as an image on a standard video monitor **73** or within a graphics window managed by the operating system (such as Microsoft Windows XP) of the display unit **70**. In addition, the display unit **70** can display textual data for the operator on the monitor **73**, including, for example, information about the patient, the configuration parameter values in use by the ultrasound unit **40**, and so forth. In an embodiment, the display unit **70** may provide a function that allows measuring the distance between two points on the image, as interactively selected by the operator.

[0052] To analyze and display an indication of the motion—and specifically the velocity—of locations in the image corresponding to tissue and fluid movement (i.e., blood), further Doppler frequency distribution analysis can be performed and translated into a readily understandable graphical representations. Doppler frequency analysis is well-known in the field of ultrasound medical imaging and described in more detail in the patent applications incorporated by reference herein. Fourier analysis may be used, for example, to determine the frequency distribution information and the average Doppler frequency shift for each of all points or selected points in the ultrasound image, and from which to compute the individual velocities of those points.

[0053] The display unit **70** can generate an image in which the Doppler frequency shift information communicated by the unit **40** for each point or pixel is represented by a color hue. Since Doppler shift provides information on the speed and direction of movement of fluids and structures with respect to the transducer, various color hues can be used in the display to correspond to the velocity and direction of motion. For example, red may be used to represent the maximum velocity in one direction, blue to represent the maximum velocity in the opposite direction, and colors between red and blue on the color spectrum to represent velocities in between. In another embodiment, such colors can be superimposed on the B-mode image, which is otherwise rendered as a grayscale image wherein the brightness of each pixel depends on the amplitude of the returned ultrasound echo from the anatomical location corresponding to the pixel. Other modes of display are well known in the art, such as a plot of the distribution of Doppler frequency shifts at the points along a line in the image, and M-mode in which the movement along narrow lines is displayed.

[0054] Optionally, a connection interface **92** may connect the display unit **70** to a clinic or hospital information infrastructure **90** or the Internet. A hospital information infrastructure **90** will typically include a network of attached workstations, graphical displays, database and file servers, and the like. The optional interface **92** typically can be an Ethernet cable, a wireless WiFi interface (IEEE 802.11), or any other high-speed communications physical layer and protocol. For example, an interface **92** can allow the display unit **70** to access information from the Internet, a database, or a hospital network infrastructure **90**. The display unit **70** may also transmit information outward via the interface **92**, such as to store the ultrasound data on a network server or display the ultrasound images elsewhere than the display unit **70**.

[0055] FIG. 1B illustrates another embodiment which electrically isolates the ultrasound unit **40** from the image display unit **70**. The embodiment illustrated in FIG. 1B uses a wireless data communication interface **76** to convey ultrasound image data to the image display unit **70**. This embodiment may have safety advantages, because it electrically isolates

the ultrasound unit **40** from the image display unit **70** and eliminates a data cable which can pick up and conduct stray electrical fields and electronic noise. By removing an electrical conduction path for high voltage or leakage currents, namely the wires or cable of the interface **75** between the ultrasound unit **40** and the display unit **70**, this embodiment provides further patient protection from potential internal or external electrical faults and eliminates a source of electronic noise. Not only does this embodiment provide added protection from faults within display unit **70**, but it can provide protection from lightening or power surges which may occur with an embodiment such as a laptop or desk-top personal computer plugged into a normal AC utility power outlet. Without sufficient isolation circuitry, lighting or surges can send a high voltage spike through the power supply of the display unit **70** and into the rest of the system **1** through any available conductive pathway.

[0056] Commercially available wireless communications systems can be used for the wireless interface **76**. For example, the wireless interface **76** may be an infrared communication interface (such as the IRDA standard), a radio-based communication interface (such as the Bluetooth, Zig-Bee, or 802.11 WiFi or 802.15.4 standards), or both (for example, infrared in one direction and radio in the other direction). To decrease the data processing that must be done in the ultrasound unit **40**, a high speed data transmission system may be used to provide partially processed ultrasound data to the image display unit **70** for further processing. The data transmission may have a data rate of 1 megabit per second or more.

[0057] Common to the embodiments illustrated in FIG. 1A and 1B is a power supply **59** coupled to the ultrasound unit **40**. Electrical power is used both to power the processors and circuits in the ultrasound unit **40** and to provide energy for the electrical pulses which drive the transducer array **22**. Power may be provided through the data cable **75** (as in the case of a USB cable embodiment), via a separate power cable connected to the display unit **70**, via a separate power supply (such as a transformer connected to an AC power source), or via a self contained power source (such as a battery). For an embodiment in which the image display unit **70** does not supply power to the ultrasound unit **40**, such as where the image data is communicated via a wireless data link as illustrated in FIG. 1B, the ultrasound unit **40** can be powered by a separate power source **59**. Non-limiting examples of suitable separate power sources include a rechargeable battery pack, a disposable battery pack, a power supply connected to public utility power lines through an isolation transformer, a power supply engineered for safety compliance isolation from public utility power, a solar cell, a fuel cell, a charged high-capacity storage capacitor, combinations of two or more of such power sources (e.g., a rechargeable battery and a solar cell), and any other source of electrical power which may become known in the art.

[0058] A self-contained power source, such as a battery or solar cell, can provide inherent safety advantages over conventional power sources. This is because a self-contained power source **59** can be used to further isolate the patient from stray and fault currents since there need not be a power cable connected to the beam former unit. This removes the power source (such as hospital main AC power) and the power cord as sources of power spikes and fault currents. Such isolation may be further enhanced by forming the housing or chassis of the ultrasound unit **40** from non-conductive material and

encasing the self-contained power source within the housing or chassis. This configuration effectively presents no return path or common ground between the power source and the patient. That is, even if there is an electrical potential difference between the ultrasound unit **40** and the patient, little current can flow between them. Further, with a self-contained power source, there is very little chance that a patient will receive high voltage from lightening or from a utility power outlet through a failed component, faulty design, or a power surge. A typical self-contained power supply **59** can supply only limited current at limited voltage, further reducing the likelihood of excessive leakage current. Also, using a self-contained power supply **59** can further reduce cables and conductors which can pick up stray electromagnetic radiation and become a source of electronic noise in the system.

[0059] In another embodiment, the power supply **59** may be power conductors parallel to or contained in the communication cable **75** of FIG. 1A, over which the image display unit **70** provides power to the ultrasound unit **40**. The display unit **70** can supply power from its own supply of power such as, for example, if the interface **75** connecting the display unit **70** and the ultrasound unit **40** is embodied by a standard IEEE-1394 (Firewire) cable or a USB cable, both of which contain direct current power conductors.

[0060] If an embodiment does use an electrically conductive cable as part of the communication interface **75**, then in lieu of other measures, the data communication interface **75** can include additional circuits for isolating the ultrasound unit **40** from any source of excessive leakage current or high voltage from or through the display unit **70**—whether or not power is supplied over the interface **75**. National and international safety organizations specify leakage current and breakdown voltage standards for various medical applications: for example, a maximum leakage current of 20 microamperes or a breakdown voltage of at least 5000 volts. By providing electrical isolation circuitry **44** within the ultrasound unit **40**, greater protection for the patient can be provided against high power, power surges, and system overloads, as well as providing greater protection against or filtering of signal artifacts, signal jitter, and signal crosstalk.

[0061] Further patient electrical isolation is provided in embodiments utilizing a fiber optic data cable **75** between the ultrasound unit **40** and the display unit **70**. In an alternative embodiment further isolation may be provided by including an optical isolator module somewhere along each conductor of the interface **75**. An example of an optical isolator module includes a light-emitting diode optically coupled to a photo detector and configured so that electrical signals entering the module are converted into light signals and converted back into electrical signals within the module, thereby conveying the data across an electrically isolating space. In embodiments where the data interface **75** is an optical fiber with suitable optical-electrical converters at each end of the interface **75**, the optical fiber cable can be constructed to prevent or minimize electrical conduction, such as fabricating the covering from non-conducting plastics, thereby providing better electrical isolation. Optical isolation may preclude supplying electrical power through the data interface **75**, so an alternative power supply **59** for the ultrasound unit **40** according to an embodiment described herein may be employed. The use of optical fiber cable or an optical isolation can also help to reduce electronic noise introduced into the ultrasound unit **40** from stray electromagnetic radiation.

[0062] In the various embodiments, the ultrasound unit **40** lies between the patient on one side and power sources and external processors/displays on the other. As such, different levels of isolation may be provided by separate isolation circuitry **44** within the ultrasound unit **40** as appropriate to particular connections. For example, by providing greater electrical isolation on connections to power and/or external processor/displays, such isolation may protect the circuitry of the ultrasound unit **40** as well as the patient from external voltage spikes and fault currents. As another example, isolation circuitry on the patient side of the ultrasound unit **40** circuitry, may reduce hardware and software complications and increase integration efficiency.

[0063] FIG. 2 depicts a simplified cross section of a human heart **12** with an ultrasonic imaging catheter **20** positioned in the right ventricle **14**. The catheter **20** includes an ultrasound transducer array **22**, which may image at least a portion of the heart **12**. For example, the imaging view **26** afforded by the transducer array **22** may allow imaging the left ventricle **13**, the ventricular walls **15,16,17**, and other coronary structures. Usage of an embodiment may include positioning the array **22** at other locations and at other orientations within the heart (such as the right atrium), within a vein, within an artery, or within some other anatomical lumen. Insertion of the catheter **20** into a circulatory system vessel or other anatomical cavity through use of a percutaneous cannula is well known in the medical arts.

[0064] FIG. 3 is a close-up example of an embodiment of a portion of a catheter **20**, carrying an ultrasound transducer array **22**. The array **22** may be located near the distal end of the catheter **20**, but may be located elsewhere within the catheter **20**. Also shown in FIG. 3 is a temperature sensor **26** for connecting to the thermal sensing circuit **42** and cut-off circuit **43** shown in FIGS. 1A and 1B.

[0065] Examples of phased array ultrasound imaging catheters used in performing intracardiac echocardiography and methods of using such devices in cardiac diagnosis are disclosed in the following published U.S. patent applications—each of which is incorporated herein by reference in their entirety.

[0066] 2004/0127798 to Dala-Krishna et al.;

[0067] 2005/0228290 to Borovsky et al.; and

[0068] 2005/0245822 to Dala-Krishna et al.

Commercially available ultrasound catheters are available from EP MedSystems, Inc. of West Berlin, N.J.

[0069] It should be noted that the present invention is not limited to the specific catheter assembly disclosed in the applications cited above, because the invention is applicable to various catheters and instruments designed for intravascular and intracardiac echocardiography and for other physiological uses involving an ultrasound beam former and interfaces with medical instruments and external display equipment

[0070] For all medical imaging technologies, patient safety is of paramount concern. For imaging technologies involving intrabody probes (e.g., ultrasound imaging catheters, electrophysiology (EP) catheters, ablation catheters, etc.), particular attention is paid to protecting the patient from unintended electrical currents and power emissions within the patient's body. For example, testing has shown that leakage currents of sufficient strength can cause muscle stimulation, which may be detrimental to the patient undergoing intrabody imaging. As such, industry approved electrical safety standards (e.g.,

for isolation, grounding, and leakage current) have been established for medical devices, such as national standards set by the Association for Advancement of Medical Instrumentation, limiting leakage currents from intracardiac probes to less than 50 microamperes.

[0071] In typical catheter based probes, electrical shielding or insulation is provided by way of a robust catheter body to satisfy the industry approved electrical safety standards. Shielding alone, however, may be unsatisfactory for some implementations, as substantial shielding increases the thickness of the catheter body. Induced currents may also arise from the catheters acting as an antenna picking up electromagnetic energy radiated by electronic equipment present in a typical electrophysiology lab. In some instances, the shielding may be inadvertently damaged and, thus, not provide adequate protection. Thus, methods and devices that enable intracardiac medical devices to meet or exceed the federally mandated electrical safety standards are highly desirable.

[0072] Published research has revealed that the human heart is more vulnerable to small currents when the currents are introduced within the heart itself, such as by percutaneous catheters. In *Cardiovascular Collapse Caused by Electrocardiographically Silent 60 Hz Intracardiac Leakage Current*, by C. Swerdlow et. al., the authors reported that leakage currents as low as 20 microamps may induce cardiovascular collapse when applied within the heart. Accordingly, percutaneous catheters might require greater electrical isolation than specified in more general standards in order to assure patient safety.

[0073] Such small leakage currents can readily arise, for example, from imperfect electrical insulation, condensation in circuits, faulty electronic components, ambient radio waves, and induction from surrounding circuits and magnetic fields. Further, safety standards require minimum ("creepage") distances (such as 5 millimeters) between certain conductors to isolate a patient from possible high voltage discharges resulting from unlikely but possible component failures.

[0074] FIG. 4 shows an embodiment of the isolation circuitry 44 and thermal monitor circuit 42. In this example embodiment, electrical isolation is accomplished by a transformer circuit for each transducer in the array 22. Transformers do not conduct direct current and small air-core transformers can be used that will not readily pass low frequency alternating current (such as the 50 to 60 hertz of standard utility power outlets). Thus, electrical isolation is provided by presenting high impedance to unintended direct current and to lower frequency alternating currents. Further, if insulated adequately, the transformers will not conduct D.C. voltages below some very high, specified break-down voltage.

[0075] Another example of a safety concern for intrabody ultrasound systems is the sustained power of ultrasound radiated from the transducers, specifically for the higher power employed by color Doppler imaging, wherein the power may locally heat tissue above a safe body temperature. Although the ultrasound generation electronics may indirectly limit the amount of heat an ultrasonic catheter can theoretically induce in tissue at a given power level, direct monitoring of the actual temperature at the transducer array and surrounding tissue is much safer and avoids assumptions about how effectively specific tissues can dissipate the heat. Therefore, a need exists for a safety means either to warn the operator or to curtail the applied power automatically, whenever the measured temperature exceeds some pre-determined limit. An example of a

standard safe temperature limit, as established by FDA in the United States, is 43 degrees Celsius, although the exact limit may depend on the specific environment and use of the catheter.

[0076] Besides the ultrasound transducer array 22, the catheter 20 may optionally further include an electronic temperature sensor 26, such as a thermocouple or thermistor, as shown in FIG. 3. The purpose of the temperature sensor 26 is to measure the increase in temperature resulting from the injection of high-power ultrasound into living tissue. Because the sound energy is most concentrated near the ultrasound transducer array 22, the temperature sensor 26 is best located very close to the array 22, such as on the catheter 20 containing the array 22. Temperatures above a proscribed level (e.g., 43° C.) can permanently damage tissue and must be avoided. Therefore, the temperature sensor 26, together with the thermal monitor circuit 42 of FIG. 4, can be calibrated to detect temperatures above the proscribed level. When the temperature exceeds the proscribed temperature, the cut-off circuit inhibits or at least reduces the generation of the ultrasound signals generated by the signal generator 46.

[0077] FIG. 4 illustrates an example embodiment of the thermal monitor circuit 42 that includes a thermal comparator circuit 42 coupled to a cut-off circuit 43. In this embodiment, signals received from a thermocouple or thermistor 26 positioned near the transducer array 22 can be compared in a comparator circuit to a reference threshold value corresponding to a maximum safe temperature. If the sensed temperature signal exceeds the reference threshold, indicating temperatures in the vicinity of the transducer array 22 exceed a safe temperature, the comparator circuit can generate a cut-off signal that is provided to the cut-off circuit 43. In the circuit embodiment illustrated in FIG. 4A, a common lead is provided to all transformers, particularly on the transmit/receive side (i.e., the portion of isolation circuit connected to the ultrasound unit 40). This circuit permits the cut-off circuit 43 to be a simple switch that opens to disconnect the common lead on the transmit/receive side of the isolation circuit in response to a cut-off signal received from the temperature comparator circuit 42.

[0078] Another example embodiment of the thermal monitor circuit 42 includes a plurality of gate circuits configured to gate the individual leads passing signals to and from each of the transducer elements in the transducer array 22. So long as the temperature measured by the thermistor 26 remains below a safe level (e.g., not more than 43° C.), the gate circuits remain enabled allowing signals to pass to/from the transducer elements. However, should the temperature measured by the thermistor 26 reach or exceed an unsafe level, the thermal monitoring circuit 42 disables the gate circuits, automatically shutting off the transducer array 22. In another example embodiment, the thermal monitor circuit 42 is configured to disable transmission of ultrasound signals from the ultrasound unit 40 by disabling the transmit circuitry by signaling the signal generator 46 through a trigger mechanism, such as a hardware interrupt signal. Other thermal monitor circuit embodiments include circuits that disable an array of multiplexers or transmit channel amplifiers that may be used in the ultrasound unit 40 for generating, controlling, distributing, conditioning and/or transmitting ultrasound pulses to the transducer array 22. The various example embodiments of the thermal monitor and cut-off circuits 42, 43, as well as other suitable circuits, perform the safety function of discontinuing transmission of ultrasound signals from the signal

generator 46 through the isolation circuit 44 upon receiving a cut-off signal or sensing an unsafe temperature in the vicinity of the transducer array 22.

[0079] FIG. 4 also illustrates electrical isolation circuits 44 which electrically isolate the catheter and transducer array from the transmit/receive circuits of the ultrasound unit 40. High frequency ultrasound signals (both transmitted and received) are communicated by means of isolation transformers within the isolation circuits 44, while direct and low frequency AC currents are electrically isolated.

[0080] FIG. 5 illustrates example connections among components of the ultrasound unit 40. The embodiment illustrated in FIG. 5 is not intended to specify the only possible configuration of components and their interconnections but serves as an example of an enabling implementation.

[0081] The signal generator 46 generates electrical signals of ultrasonic frequencies, such as in the range of about 1 megahertz to 10 megahertz, as are commonly used for ultrasound imaging. The signals may be continuous or may be intermittent pulses. The electrical signals may pass through a transmit/receive multiplexer 48, isolation circuits 44, and a cable 28 to reach the transducer array 22. The electrical signals which reach the transducer array 22 cause the transducers to produce ultrasound signals in the same frequency range generated by the generator 46.

[0082] The transmit/receive multiplexer 48 directs the signals generated by the generator 46 through the isolation circuitry 44, which serves to limit unwanted electrical currents and voltages passing into the cable 28.

[0083] Signals which transit the isolation circuitry 44 pass into the signal cable 28 which delivers the signals to each of the transducers in the array 22. The cable 28 may include at least one wire per transducer in the array. The transducers in the array 22 convert the electrical signals into sound waves, which propagate into a portion of a patient's anatomy, such as the heart. As shown in FIG. 5, the same cable 28 (or a separate cable, not shown) may conduct the return ultrasound signals back to the isolation circuitry 44 of the ultrasound unit 40.

[0084] An embodiment of the isolation circuitry 44 is described above with respect to FIG. 4. In an embodiment of ultrasound unit 40, the isolation circuitry may be connected to the cable 28, with no other active circuitry in-between. This arrangement may prevent a possible, compromised path for leakage current caused by other circuitry. An embodiment employs each conductor of cable 28 both to conduct the generated electrical signal to each transducer of array 28 and to conduct the returning echo signal from the transducer. Thus, both the generated signal and the return signal may pass through the same isolation circuit (transformer, bi-directional optical isolator, or other electrical isolation component). In an embodiment there may be at least one isolation circuit for each transducer of array 28.

[0085] Multiplexer 48 may be necessary where the generated signals from the generator 46 and the received echo signals both pass through the same isolation circuitry 44 and the same wires of cable 28. Specifically, the transmit/receive multiplexer 48 may be used to separate out the received echo signals from the generated electrical signals from the generator 46. This may be accomplished by connecting the transducer array to the receiving amplifier circuits between generated ultrasound pulses, so the only signals allowed to pass are the received ultrasound echo signals. Alternatively, the electrical pulses of the transmitted pulses may be subtracted from all signals received from the isolation circuitry to yield

the received ultrasound echo signals. The multiplexer 48 can direct the received ultrasound echo signals to conditioning circuitry 51 to filter and condition the signals as necessary. The signal can also be amplified, such as within the multiplexer 48, within the conditioning circuitry 51, or by a separate amplifier. At some point, the amplified and filtered echo signal can be digitized by an analog-to-digital converter (ADC) and can be temporarily stored in a signal memory buffer 53, such as random access semiconductor memory (RAM).

[0086] For an embodiment which employs separate transducers and conductors for the generated signals and for the received echo signals, separate transformers or mono-directional optical isolators may be used in the isolation circuitry 44. In such an embodiment, the transmit/receive multiplexer 48 may not be included.

[0087] The filter and conditioning circuitry 51 may be provided to reject signal frequencies outside a certain range, such as rejecting spurious signals induced in the cable 28, for example. The echo signals may be amplified as part of this circuitry (before, during, and/or after filtering), as part of the transmit/receive multiplexer 48 or elsewhere in the ultrasound unit 40. Other signal processing may be performed to enhance the desirable properties of the signal returned from the transducer array 22. For example, the signal conditioning circuitry 51 may reject the spurious signals from internal reflections within the catheter.

[0088] The analog-to-digital converter (ADC) 52 can be included to frequently sample the received ultrasound signals, which are received as analog electrical levels, and convert them to discrete digital numeric values. This conversion may be performed before, during, or following the action of the filter and conditioning circuitry 51. The signal may be in either analog or digital form or both during parts of the amplification, filtering, conditioning, and storage of the signal. In other words, the filter and conditioning circuitry 51 may apply well-known analog filtering techniques to the signals before digitization, may apply well-known digital filtering methods to the digitized signals, or do both. Techniques for such digital and analog signal processing are well known. There may be an ADC per transducer, or fewer ADCs may be used with each being time-multiplexed among multiple transducers. Conversion of signals to streams of digital numbers is a convenience based on the current availability and economy of digital processing, but suitable analog circuits can be used in part or all of the ultrasound unit 40.

[0089] Because contemporary electronics routinely store signals in digital form, the embodiment of FIG. 5 may digitize the return signals prior to storage of some portion of the return signals in memory 53, which may be a semiconductor random-access memory (RAM). Methods of storing an analog signal, such as in time delay circuits, may be used instead of or in addition to digital storage. A portion of the memory 53 may store the signal from each transducer of array 22.

[0090] The beam-former 54 processes the returned echo signal data, some or all of which may be stored in memory 53. The beam-former 54 may calculate the amplitude of the ultrasound echo at each of many specific angles and distances from the transducer array. Techniques for beam-forming (either for transmission or for reception) are well known in the fields of ultrasound imaging and in phased array sonar and radar.

[0091] The result of the processing of the data stored in buffer memory 53 by the beam-former 54 typically can be a

pixel-based image relative to a polar-coordinate system. The beam-former 54 may be implemented in very large scale integrated (VLSI) semiconductor circuits. The beam-former 54 may employ substantial parallel processing of the ultrasound signals from the transducers of array 22. For example, there may be simultaneous computations of more than one beam angle and/or more than one distance along a beam angle.

[0092] The amplitude, phase and time of arrival of reflected ultrasound pulses at each transducer in the array 22 can be used by the beam-former 54 to calculate the angle (with respect to the long axis of the transducer array 22) and distance from the array to each echo source. The distance and angle data may then be combined with amplitude (i.e., power of the received echo) to produce (e.g., by processing the data according to an algorithm) a pixel of image data. Alternatively, the beam-former 54 may store or output the processed received ultrasound as data sets comprising data groups of angle, distance and amplitude. In this and like manner, the beam-former 54 can turn the large volume of streaming ultrasound signals into a smaller set of data easily passed over a serial data link 75 for processing or display by a display unit 70. In an embodiment, the beam-former 54 is included in a VLSI chip within the ultrasound unit 40.

[0093] The beam former 54 may compare the frequency of the generated signals with the frequency spectrum of the returned echo signals. The difference in frequency relates directly to the velocity of tissue or blood toward (higher frequency) or away from (lower frequency) the transducer array due to the Doppler effect. The difference in frequency, i.e., the amount of Doppler frequency shift, is indicative of motion of the tissue (including blood) from which the ultrasound reflected. The frequency shift may be determined by mixing the generated signal and received echo signal and detecting the difference frequency. The conversion of the frequency shift to velocity depends on the speed of sound in the body, which is about 1450 to 1600 meters per second in soft tissue, including blood. The conversion of frequency shift to velocity according to well known algorithms may be performed immediately by the beam former 54, or later, such as by an external image processor at the time the image is displayed. If calculated by the beam-former 54, the velocity data (or Doppler shift) may be outputted as a fourth element of the data set, so that echo sources are identified by angle, distance, amplitude and velocity (or frequency or Doppler shift).

[0094] The velocity of echo sources may be computed at each of numerous angles and distances relative to the transducer array 22. The computed velocities may be represented visually as a spectrum of colors, for example, as is conventional in the art. The velocity of numerous points in the tissue or blood may be mapped to colors at the corresponding locations in the final image of the tissue. Image display unit 70, as shown in FIG. 1A, may perform this mapping, although it may be performed alternatively within ultrasound unit 40, as shown in FIG. 8.

[0095] With reference to FIG. 5, an embodiment of a beam former 54 may directly produce an image in rectangular coordinates. Alternatively beam former 54 may directly produce an image in polar coordinates and transform the image into rectangular coordinates. Alternatively, the beam former 54 may simply produce an image in polar coordinates (i.e., angle and distance coordinates) and allow subsequent image processing to perform the coordinate transformation as needed (such as in image display unit 70).

[0096] As also shown in FIG. 5, the buffer memory 53 may make available the return signal data representing the ultrasound echo waves, and the beam-former 54 may access that data and may calculate the amplitude of the ultrasound echo at each of many specific angles and distances from the transducer array. The result of the processing of the data stored in the buffer memory 53 by the beam-former 54 may be a pixel-based image relative to a polar-coordinate system. In an embodiment as illustrated in FIG. 5, polar-coordinate oriented ultrasound echo data may be serialized and may be transmitted to the image display unit 70 over data interface 75. Alternatively, the beam-former 54 may generate data relative to a rectangular coordinate system and transmit that data to display unit 70 over an interface 75.

[0097] A programmed microcontroller, microprocessor, or microcomputer 41 or functionally equivalent discrete electronics can be included to coordinate the activity described above within the ultrasound unit 40. In addition, the microcomputer 41 (or equivalent) may respond to configuration parameters and commands sent from the image display unit 70 (of FIG. 1A) over the communication interface 75 or 76 to the ultrasound unit 40.

[0098] In an embodiment, the ultrasound unit 40 may be configured via software or discrete circuits to adaptively cut and separate each frame of ultrasound image data. Such capability may be used to select and transmit frames for which there is useful information (e.g., changes in position of structures) to limit the bandwidth required for transmitting ultrasound images to external displays. In a normal cardiac cycle, portions of the heart are at rest for significant fractions of the cardiac cycle, so numerous images during such intra-contraction periods will contain the same image information. By not transmitting images in which there has been no change since the previous image, the same clinical information may be transmitted at substantially lower data rates. Such processing of image frames may be accomplished by a segmentation module (not shown).

[0099] In an embodiment associated with cardiac imaging, an external electrocardiogram (ECG) unit 60 (see FIG. 1A or 1B) may be connected to ultrasound unit 40 through an ECG communications interface 62. The signals sent through interface 62 may be used to synchronize the imaging with the heartbeat of the patient. For example, a sequence of images may be associated with a sequence of phases of a cardiac cycle, or images may be captured only at a specified phase of the cardiac cycle. The ECG communications interface 62 may be any wired or wireless interface. The ECG signal may be monitored by the microcomputer 41 to orchestrate the operation and timing of the signal generator 46 in order to image the heart at particular phases of the cardiac cycle.

[0100] Referring to FIGS. 1A and 1B, an embodiment may employ one or more ECG sensors 66 integrated in an intravenous catheter 64 that is coupled to the ultrasound unit 40 by a connecting cable 68. In an embodiment, ECG sensors may be included on the catheter 20 which carries the ultrasound transducer array 22. The ultrasound unit 40 may include connectors for receiving electrical connection plugs for the ECG catheter 64 or connecting the electrical connection plug on the cable 68. Such connectors may route the ECG signals through the isolation circuitry 44 and then out to an external ECG unit 60 via cable 62. This embodiment allows the ultrasound unit 40 to serve as a universal connector for the ultrasound and ECG instruments used in a typical intracardiac examination employing both ECG and ultrasound sensors.

This embodiment reduces the need for multiple cables and connectors, thereby simplifying the procedure.

[0101] In an embodiment, signals from the ECG sensor **66** may be used in lieu of, or in addition to, signals from an external ECG unit **60**, which may have its own ECG sensor or sensors. The ECG sensor signals can be used to record or control the timing of the ultrasound image acquisition relative to the cardiac cycle instead of or in conjunction with signals from an external ECG unit **60**. The signals from an ECG sensor may be included within the data stream outputted by the ultrasound unit **40**.

[0102] Whether an ECG signal is acquired from an external ECG unit **60** or an attached ECG sensor **66**, the interface **60**, **68** or cable **28**, respectively, may be electrically isolated from the ultrasound unit **40** to enhance patient safety and reduce electronic noise in the system. For wired interfaces, the isolation may be accomplished by a transformer isolation circuit **44** or an optical isolator as described herein. Protection against electrical leakage currents and high voltage discharges may be accomplished in an embodiment by using a wireless interface for the ECG interface **62**.

[0103] In addition to including connectors for receiving the input/output connection plugs for ultrasound catheters and ECG sensors or equipment, some embodiments of the ultrasound unit **40** include connections for additional sensors, such as intracardiac percutaneous leads, subcutaneous leads, reference leads and other electrical leads that may be employed during a procedure. As with ultrasound and ECG connections, such additional lead connections can be coupled to isolation circuitry **44** to provide patient protection. By providing such connections with integrated isolation circuitry, the ultrasound unit **40** can serve as a central interface unit for connecting all sensors employed in a procedure.

[0104] Some or all of the electronic circuitry of ultrasound unit **40** may be implemented within one or more large scale integrated circuits such as VLSI, ASIC, or FPGA semiconductor chips, as are well known in the electronics art. The program instructions running in the microcomputer **41** may be stored in some form of random access memory (RAM) or read-only memory (ROM) as software or firmware.

[0105] Portable ultrasound units, which contain compact signal generation and beam-forming circuitry and which are separate from the display unit **70**, are available commercially from Terason, a division of Teratech Corporation (Burlington, Mass.). Some of the details of these portable ultrasound units are described along with associated methods in the following published patent applications—each of which is incorporated herein by reference in its entirety:

[0106] 2005/0228276 to He et al;

[0107] 2005/0018540 to Gilbert et al; and

[0108] 2003/0100833 to He et al.

Also described in the above applications are methods of implementing the beam-forming computations.

[0109] As shown in FIG. 6, the communication interface **74** within the display unit **70** may receive the ultrasound data over the interface **75** or **76** and may temporarily store the data in memory **77** for further processing. The image data at this point may be relative to a polar coordinate system, so scan converter **82** may reformat it into an image relative to a rectangular coordinate system as needed.

[0110] Image data from the scan conversion (and Doppler processing, if any) may be processed by an image renderer **83**, formatted, and displayed as an image on a video monitor **73**.

For example, the rendering circuit **83** may generate a gray-scale image (such as a B-mode image) in which the brightness of each pixel is representative of the amplitude of the ultrasound echo from the anatomical point to which the pixel corresponds.

[0111] Besides responding to operator input of configuration information, the interactive control **80** may also respond to operator input controlling how the image is converted, processed, and rendered on the display **73**.

[0112] The image display unit **70** may perform other functions. For example, the interactive control **80** in the image display unit **70** may transmit configuration parameters and control commands to the ultrasound unit **40**, where the configuration parameters and commands may be supplied by the operator by means of interactive inputs from a pointing device (mouse, trackball, finger pad, or joystick, for example) and a keypad or keyboard **72** attached to display unit **70**.

[0113] Optionally, the interactive control **80** of the image display unit **70** may forward the image and/or raw data to a network file or database server, to the Internet, to display screen, or to a workstation through a communication interface **92**.

[0114] FIG. 7 illustrates example images that can be displayed by an embodiment. Contained within the field of view **8** of the B-mode image is an image of the walls **5** of a ventricular cavity **4**. Also shown in FIG. 7 is a plot **9** of the blood flow velocity as derived from the spectral analysis of the Doppler frequency shifts.

[0115] In an embodiment, the image display unit **70** circuitry may be included within the ultrasound unit **40** housing or chassis. This may be accomplished by simply including the image display unit **70** circuitry as another board or VLSI chip within the ultrasound unit **40**. Alternatively, the circuitry and functionality of the components of the image display unit **70** may be incorporated in a VLSI chip that also encompasses the beam-former **54** and/or microcomputer **41** within the ultrasound unit **40**. In such an embodiment, the ultrasound unit **40** outputs image data as a video signal (e.g., VGA, composite video, conventional television or high-definition video) that can be carried by a cable **75** directly to a display **73** to yield an image on the screen without further processing. In a further embodiment, the ultrasound unit **40** may output image data as a network compatible signal, such as Ethernet or WiFi, that can be directly coupled to a network.

[0116] FIG. 8 is a block diagram of such an embodiment in which most or all of the image processing circuitry is included within the ultrasound unit **40**. That is, most or all of the circuitry of FIG. 6 is compactly incorporated into the chassis of ultrasound unit **40**. This is enabled by readily available circuitry equivalent to a personal computer on a small single circuit board or within a single integrated circuit.

[0117] In the embodiment illustrated in FIG. 8, the communication interface **58**, the communication cable **75** (of FIG. 5) and the communication interface **74** (of FIG. 6) may be simplified or essentially eliminated. Further, the ultrasound unit **40** may directly link to the hospital network and infrastructure **90** (shown in FIG. 1) through wired or wireless link **92** as described above.

[0118] A user input device **72** may be connected to the ultrasound unit **40** to permit a user to provide commands and operating parameters, such as by way of a keyboard, keypad and/or a user pointing device such as a mouse, touch screen, trackball, light pen, or finger pad. The user input device **72** may include a voice recognition device in lieu of or in addi-

tion to a keyboard. The input device 72 may be connected to the ultrasound unit 40 by a cable, an infrared link, a radio link (such as Bluetooth), or the equivalent, each of which are commercially available.

[0119] A display monitor 73 may not be present as part of ultrasound unit 40. Any of many choices, sizes, and styles of a display 73 may be connected to ultrasound unit 40. For example, the external display monitor 73 may be a cathode ray tube, a liquid crystal display, a plasma display screen, "heads up" video goggles, a video projector, or any other graphical display device that may become available. The display monitor 73 may be large and may be located conveniently out of the way, such as a plasma screen hung from the ceiling or on a wall. The display monitor 73 may be positioned for better viewing by the physician. There may be more than one display 73, and a display may be positioned remotely, such as in another room or in a distant facility. The display 73 may be connected to the ultrasound unit 40 by a cable, an infrared link, a radio link (such as Bluetooth), or any equivalent wireless technology.

[0120] In an embodiment, the display monitor 73 and/or the user input device 72 may be embodied by a computer terminal, workstation, or personal computer such as a laptop computer. Such an embodiment can be configured to display the graphical output from the image rendering circuits 83 and to pass user inputs on to the interactive control 80 of the ultrasound unit 40. Alternatively, in an embodiment in which the display monitor 73 and user input device 72 are provided by a computer system, the computer system may operate software enabling it to perform additional image processing on the data received from the ultrasound unit 40.

[0121] The ultrasound unit 40 may need to be powered by an external power source 59, as was previously discussed with respect to FIGS. 1A and 1B. The power source 59 of FIG. 8 may be a separate external power supply with provision to isolate the ultrasound unit 40 from the patient. The power source 59 may be a power source, such as batteries, contained within the ultrasound unit 40. Alternatively, the power source 59 may simply be conductors in a data cable supplying power from input unit 72 or display unit 73.

[0122] Because of the priority of safety for a patient, a wired connection between the ultrasound unit 40 and the user input device 72 may need isolation circuitry to prevent potentially harmful leakage current from flowing from the input device 72 through the ultrasound unit 40 to the patient. This isolation may be provided by the isolation circuits 44 within the ultrasound unit 40 shown in FIGS. 1A, 1B, 4, 6 and 8. Alternatively or in addition, isolation circuits may be provided between the ultrasound unit 40 and the user input device 72, such as an optical fiber data link or optical isolation module as previously described. For example, if the input device 72 is powered from a source which shares a common ground (or other low impedance path) with the patient, there could be unexpected potential differences between the input device 72 and the patient conducted through the ultrasound unit 40. Such a potential difference could produce harmful leakage currents. Such currents are limited by sufficiently high impedance, such as provided by isolation circuitry, such as an optical isolator. The isolator may also protect against unintended high voltages caused by failures in the input device 72, its power source, or by lightning, as well as reduce electronic noise induced by stray electromagnetic radiation.

The same reasoning applies to a wired connection between the display 73 and the ultrasound unit 40, and any connection to a network.

[0123] One way to achieve isolation for the input device 72 or display device 73 is to employ a wireless communication link between device 72 and unit 40 and between device 73 and unit 40. Any wireless communication link of sufficient bandwidth, such as those mentioned previously, may be used in this capacity.

[0124] The embodiment illustrated by FIG. 8 includes an optional connection 68 between the ultrasound unit and an ECG sensor, such as an ECG catheter 64, and an optional connection 62 between the ultrasound unit 40 and an external ECG unit 60. In addition or alternatively, an embodiment may employ an ECG sensor integrated in a catheter 20 with a connection to ultrasound unit 40 through cable 28. The foregoing comments in the discussion of FIG. 5 about ECG signals also apply to an embodiment as illustrated by FIG. 8. Interface 62 may be any wired or wireless communication interface discussed previously.

[0125] As illustrated in FIGS. 5 and 8, various embodiments can be housed within a housing 100 providing environmental and electrical isolation for the circuitry (e.g., circuit boards and integrated circuits) of the ultrasound unit 40. This housing 100 can be fabricated from nonconductive material, such as plastics, to minimize stray currents due to induction. The housing may also be fabricated from materials that can withstand high temperatures and/or gamma radiation so that the housing can be sterilized by heat or exposure to gamma rays.

[0126] Referring to FIGS. 5 and 8, the housing 100 can include electrical connectors to permit the ultrasound unit 40 to be quickly connected to sensors, power, a user interface and displays. For example, one or more multi-contact ultrasound catheter connectors 102 may be provided to enable a reliable electrical connection between an ultrasound phased array catheter 20 cable 28 plug and the ultrasound unit 40 while maintaining an environmental seal. An example of a suitable ultrasound catheter connector 102 is a card edge connector, such as the 0.762 mm Pitch Hi-SpecGS™ Memory Expansion Card Edge Connector manufactured by Molex Corporation (www.molex.com) illustrated in FIG. 9. Such an ultrasound catheter connector 102 can be provided on the interior of the housing 100. The ultrasound catheter connector 102 can be directly connected to the isolation circuits 44, with an electrical lead from a temperature sensor 26 connected to the thermal monitor circuit 42. A card connector (which is a flat plug) on the cable 28 can be used to pass through a sterile plastic barrier to establish an electrical connection with the connector 102. In this manner, a sterile plastic barrier can be used to serve as a boundary between sterile and non-sterile environments, and may be disposable to allow re-use of one or more of the various components. As described above, the plastic barrier may comprise, for example, a plastic sleeve or bag that encloses the housing 100 so the ultrasound unit 40 can be positioned near the patient and within a sterile boundary.

[0127] Additionally, one or more ECG sensor electrical connectors 104 may be provided in the housing 100 to permit electrically connecting ECG sensor connectors 68 to the ultrasound unit 40 without compromising the environmental seal of the housing 100. On the inside of the housing 100, the ECG sensor electrical connectors 104 may be electrically coupled to the isolation circuit 44 or passed through to an

external ECG unit **60** via an ECG unit connector **105**. In an embodiment, the housing **100** includes sixty-four or more contact edge connector type ports **105** for connecting sixty-four individual ECG probe elements.

[0128] Similarly, a power connector **106** may be provided in the housing **100** for accepting a connector to an external power source **59**. Alternatively or in addition, an internal power source, such as an optional battery **110** can be included in the housing **100**. Additionally, an output connector **107** may be provided for connecting to an external computer or display unit **73**. For example, the output connector **107** may be a video connector (e.g., CGI, VGA or composite video) or a standard two-direction serial connector such as USB, FireWire or fiber optic connector. Similarly, an input connector **108** may be provided in the housing **100** to connect to user interface devices, such as a keyboard or computer **72**. Likewise, a network cable connector **109** may be provided for directly connecting the ultrasound unit **40** to a network.

[0129] An advantage to all the embodiments described above is that they enable the use of a short data cable between the ultrasound catheter and the beam former and ultrasound system. Shorter cables significantly reduce the electronic noise that is induced in cables from electromagnetic radiation and magnetic fields within the examination room. By positioning the analog-to-digital conversion electronics (i.e., the electronics which receive ultrasound signals from the transducer and convert the information into digital format) on or next to the patient, the information within the ultrasound signals is converted to noise-resistant digital format with the least amount of induced noise. By reducing the noise in the system, greater sensitivity and better ultrasound image resolution can be obtained. This advantage is further enhanced by embodiments employing a battery powered beam former/isolation ultrasound unit since such embodiments eliminate power cables and connections to the commercial power grid. This advantage is further enhanced by embodiments which employ wireless data links for communicating ultrasound image data to external displays and for receiving control commands from external user interface devices, thereby eliminating data cables connecting to the ultrasound unit.

[0130] Another advantage to all the embodiments described above is that they allow a compact ultrasound unit **40** to be enclosed in a hand-portable housing **100** that can be conveniently located near the patient without occupying a lot of space in the examination or operating room. This arrangement obviates the need for a cumbersome cable extending from the vicinity of the patient out of the sterile field. This arrangement may entirely obviate the need for an ultrasound cart. At most, one or two lighter, more flexible and manageable cable(s), if any, may be used to extend from the ultrasound unit **40** to the display **73** and to the ultrasound unit **40** from the user input device **72**.

[0131] The various embodiments may be used according to the following method, wherein the steps can be performed in an order other than that described below. At least some of the steps may be performed contemporaneously. Some of the steps are optional.

[0132] An ultrasound unit **40**, such as shown in FIG. **8**, may be sterilized or placed inside an externally sterile enclosure. The ultrasound unit **40** may be positioned next to a patient, such as on the examination table on which the patient lies. The ultrasound unit **40** may be connected to an external power source or an internal power source.

[0133] A user input device **72** may be supplied and connected to the ultrasound unit **40**. A display monitor **73** may be supplied and connected to the ultrasound unit **40**. A data interface **92** may be established between the unit **40** and a clinic or hospital infrastructure **90**.

[0134] A sterile, relatively short, ultrasound transducer cable **28** may be connected between the ultrasound unit **40** and an ultrasound imaging catheter **20** which includes an ultrasound transducer array **28**. The catheter **20** may be introduced into a body, such as by percutaneous cannulation, and positioned so the transducer array **28** is at a desired location and orientation, such as guided by use of fluoroscopy. The transducer array **28** may be dynamically repositioned to other locations and orientations.

[0135] The unit **40** may be initialized and configured by an operator, possibly interactively through an input device **72** and video monitor **73**. The configuration may include setting of operational parameters of the ultrasound unit **40**, such as ultrasound frequency, mode of operation, mode of image processing, characteristics of the transducer array **22**, anatomical position of the array **22**, details about the patient, and so forth. The operating parameters may be changed during operation of the invention. For example, the frequency may be changed to increase or decrease the depth of penetration of the ultrasound energy. As another example, the mode of display may be changed from B-mode (which may help the operator position the array **22** with respect to anatomy) to Doppler mode (e.g., color Doppler) to observe and measure the velocity of motion of blood.

[0136] An embodiment includes some or all of the components described herein as a packaged kit with previously sterilized contents. The contents may include, by way of non-limiting example, a catheter **20** bearing an ultrasound transducer array **22**, one or more sterile cables, a sterile enclosure for the ultrasound unit **40**, a battery for the ultrasound unit **40** (if it is battery powered), and instructions. The kit may further include a cable to connect the ultrasound transducer array **22** to the ultrasound unit **40**. The kit may include a cable to connect the ultrasound unit **40** to the display unit **70**, unless the connection between them is wireless. In lieu of just a sterile enclosure for ultrasound unit **40**, an embodiment of the kit may contain the ultrasound unit **40** which has been previously sterilized. Any appropriate method may be used to sterilize the contents, such as gamma radiation, which is typically used to sterilize packaged kits in bulk. Some or all of the contents may be disposable or may be sterilizable for reuse.

[0137] While the present invention has been disclosed with reference to certain exemplary embodiments, numerous modifications, alterations, and changes to the described embodiments are possible without departing from the sphere and scope of the present invention, as defined in the appended claims. Accordingly, it is intended that the present invention not be limited to the described embodiments, but that it have the full scope defined by the language of the following claims, and equivalents thereof.

We claim:

1. A portable integrated ultrasound unit, comprising:
 - a housing;
 - an electrical isolation circuit positioned within the housing;
 - an ultrasound signal generator positioned within the housing and electrically coupled to the electrical isolation circuit; and

- a beam-forming circuit positioned within the housing and electrically coupled to the electrical isolation circuit, the beam-forming circuit configured to receive ultrasound signals from the electrical isolation circuit and output ultrasound data.
2. The portable integrated ultrasound unit according to claim 1, further comprising a microcomputer positioned within the housing and electronically coupled to the ultrasound signal generator and beam-forming circuit.
3. The portable integrated ultrasound unit according to claim 1, further comprising a thermal monitor circuit positioned within the housing, the thermal monitor circuit configured to receive a temperature input signal from a temperature sensor and discontinue transmission of ultrasound signals from the signal generator through the electrical isolation circuit when the temperature input signal indicates a sensed temperature exceeding a threshold.
4. The portable integrated ultrasound unit according to claim 1, further comprising a communication interface circuit positioned within the housing and coupled to the beam former circuit, the communication interface circuit configured to transmit data to an external display.
5. The portable integrated ultrasound unit according to claim 4, further comprising:
- a first connector positioned on the housing and electrically coupled to the isolation circuit, the first connector configured to receive electrical leads from an ultrasound transducer array;
 - a second connector positioned on the housing and electrically coupled to the communication interface circuit, the second connector configured to receive a data transmission cable for connecting to the external display.
6. The portable integrated ultrasound unit according to claim 4, further comprising wireless data link circuit positioned within the housing and coupled to the communication interface circuit, the wireless data link circuit configured to transmit data to the external display by a wireless data link signal.
7. The portable integrated ultrasound unit according to claim 1, further comprising battery enclosed within the housing.
8. The portable integrated ultrasound unit according to claim 5, further comprising a third connector on the housing configured to receive an electrical lead from an electrocardiogram sensor.
9. The portable integrated ultrasound unit according to claim 8, further comprising a fourth connector on the housing coupled to the third connector, the fourth connector configured to receive an electrical cable for connecting to an external electrocardiogram unit.
10. The portable integrated ultrasound unit according to claim 3, wherein the thermal monitor circuit is configured to transmit temperature data to an external image display unit.
11. The portable integrated ultrasound unit according to claim 3, further comprising a light emitting diode coupled to the housing and electrically connected to the thermal monitor circuit, wherein the thermal monitor circuit is further configured to power the light emitting diode in response to temperature data.
12. The portable integrated ultrasound unit according to claim 3, further comprising a green light emitting diode, a yellow light emitting diode and a red light emitting diode each coupled to the housing and each electrically connected to the thermal monitor circuit,
- wherein the thermal monitor circuit is further configured to:
- power the green light emitting diode in response to the temperature input signal indicating a sensed temperature less than a first threshold,
 - power the yellow light emitting diode in response to the temperature input signal indicating a sensed temperature greater than the first threshold but less than a second threshold, and
 - power the red light emitting diode in response to the temperature input signal indicating a sensed temperature greater than the second threshold.
13. The portable integrated ultrasound unit according to claim 9, wherein the ultrasound unit is configured to adapt an electronic transmission protocol to a type of cable coupled to at least one of the first, second, third and fourth connector.
14. An ultrasound system, comprising:
- a catheter including
 - an ultrasound transducer array positioned near a distal end of the catheter,
 - a temperature sensor positioned near the ultrasound transducer array, and
 - electrical leads electrically connecting the ultrasound transducer array to a plug on a proximal end of the catheter;
 - an image display unit; and
 - an integrated ultrasound unit, the ultrasound unit comprising:
 - a housing;
 - an electrical isolation circuit positioned within the housing
 - an ultrasound signal generator positioned within the housing and coupled to the electrical isolation circuit;
 - a beam-forming circuit positioned within the housing and coupled to the electrical isolation circuit;
 - a communication interface circuit positioned within the housing and electronically coupled to the beam forming circuit, the communication interface circuit configured to transmit data to the image display unit; and
 - a first connector positioned on the housing and electrically coupled to the electrical isolation circuit, the first connector configured to receive the catheter electrical plug.
15. The ultrasound system according to claim 14, further comprising a microcomputer positioned within the housing and electronically coupled to the ultrasound signal generator and beam-forming circuit.
16. The ultrasound system according to claim 14, further comprising a thermal monitor circuit positioned within the housing, the thermal monitor circuit configured to receive a temperature input signal from the temperature sensor and discontinue transmission of ultrasound signals from the signal generator through the electrical isolation circuit when the temperature input signal indicates a sensed temperature exceeding a threshold.
17. The ultrasound system according to claim 14, further comprising a second connector positioned on the housing and electrically coupled to the communication interface circuit, the second connector configured to receive a data transmission cable for connecting to the image display unit.
18. The ultrasound system according to claim 14, further comprising a wireless data link circuit positioned within the housing and coupled to the communication interface circuit,

the wireless data link circuit configured to transmit data to the image display unit by a wireless data link signal.

19. The ultrasound system according to claim 14, wherein the image display unit comprises a computer.

20. The ultrasound system according to claim 19, wherein the computer comprises a laptop computer.

21. The ultrasound system according to claim 14, further comprising a battery enclosed within the housing.

22. The ultrasound system according to claim 14, further comprising a third connector on the housing configured to receive an electrical lead from an electrocardiogram sensor.

23. The ultrasound system according to claim 22, further comprising a fourth connector on the housing coupled to the third connector, the fourth connector configured to receive an electrical cable for connecting to an external electrocardiogram unit.

24. The ultrasound system according to claim 16, wherein the thermal monitor circuit is configured to transmit temperature data to an external image display unit.

25. The ultrasound system according to claim 16, further comprising a light emitting diode coupled to the housing and electrically connected to the thermal monitor circuit, wherein the thermal monitor circuit is further configured to power the light emitting diode in response to temperature data.

26. The ultrasound system according to claim 16, further comprising a green light emitting diode, a yellow light emitting diode and a red light emitting diode each coupled to the housing and each electrically connected to the thermal monitor circuit, wherein the thermal monitor circuit is further configured to power the green light emitting diode in response to the temperature input signal indicating a sensed temperature less than a first threshold, power the yellow light emitting diode in response to the temperature input signal indicating a sensed temperature greater than the first threshold but less than a second threshold, and power the red light emitting diode

in response to the temperature input signal indicating a sensed temperature greater than the second threshold.

27. The ultrasound system according to claim 23, wherein the ultrasound unit is configured to adapt an electronic transmission protocol to a type of cable coupled to at least one of the first, second, third or fourth connector.

28. A kit comprising:

a sterile catheter, the catheter including

an ultrasound transducer array positioned near a distal end of the catheter,

a temperature sensor positioned near the ultrasound transducer array, and

electrical leads electrically connecting the ultrasound transducer array to a plug on a proximal end of the catheter; and

an integrated ultrasound unit, the ultrasound unit comprising:

a housing;

an electrical isolation circuit positioned within the housing

an ultrasound signal generator positioned within the housing and coupled to the electrical isolation circuit;

a beam-forming circuit positioned within the housing and coupled to the electrical isolation circuit;

a communication interface circuit positioned within the housing and electronically coupled to the beam forming circuit, the communication interface circuit configured to transmit data to an external image display unit; and

a first connector positioned on the housing and electrically coupled to the electrical isolation circuit, the first connector configured to receive the catheter electrical plug.

* * * * *

专利名称(译)	集成光束成形器和隔离器用于超声探头		
公开(公告)号	US20080146943A1	公开(公告)日	2008-06-19
申请号	US11/610778	申请日	2006-12-14
[标]申请(专利权)人(译)	EP MEDSYST		
申请(专利权)人(译)	EP MedSystems公司, INC.		
当前申请(专利权)人(译)	ST.犹达医疗用品, 房颤DIVISION, INC.		
[标]发明人	JENKINS DAVID A BYRD CHARLES BRYAN DALA KRISHNA PRAVEEN		
发明人	JENKINS, DAVID A. BYRD, CHARLES BRYAN DALA-KRISHNA, PRAVEEN		
IPC分类号	A61B8/00		
CPC分类号	A61B5/042 A61B8/12 A61B8/4405 A61B8/4427 A61B8/565 A61B8/56 A61B2560/0437 A61B5/7232 A61B8/4472		
外部链接	Espacenet USPTO		

摘要(译)

紧凑的便携式超声成像系统包括在单个单元内的隔离电路, 超声信号发生器和波束形成器的组合。隔离电路可以限制来自超声系统的非预期的泄漏电流通过超声系统的换能器阵列。信号发生器和波束形成器可以使用大规模集成半导体芯片来实现。提供连接用于连接超声换能器阵列, 用于输出超声数据和用于接收用户输入和命令。

