



US006579237B1

(12) **United States Patent**
Knoblich

(10) **Patent No.:** **US 6,579,237 B1**
(45) **Date of Patent:** **Jun. 17, 2003**

(54) **DIAGNOSTIC ULTRASONIC IMAGING SYSTEM HAVING ORGANIC LIGHT EMITTING DEVICE DISPLAY**

(75) **Inventor:** **Stan Knoblich**, Everett, WA (US)

(73) **Assignee:** **Koninklijke Philips Electronics NV**, Eindhoven (NL)

(*) **Notice:** Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) **Appl. No.:** **10/022,261**

(22) **Filed:** **Dec. 14, 2001**

(51) **Int. Cl.⁷** **A61B 8/00**

(52) **U.S. Cl.** **600/437**

(58) **Field of Search** 600/437, 441, 600/443, 447; 349/202

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,688,551 A	11/1997	Littman et al.	427/64
5,690,114 A *	11/1997	Chiang et al.	600/447
5,838,416 A *	11/1998	Chen et al.	349/202
5,920,080 A	7/1999	Jones	257/40
5,924,988 A *	7/1999	Burris et al.	600/437
5,929,474 A	7/1999	Huang et al.	257/292

6,048,573 A	4/2000	Tang et al.	427/66
6,066,357 A	5/2000	Tang et al.	427/66
6,069,443 A	5/2000	Jones et al.	313/504
6,117,529 A	9/2000	Leising et al.	428/209
6,191,433 B1	2/2001	Roitman et al.	257/40
6,210,814 B1	4/2001	Thompson et al.	428/690
6,274,979 B1	8/2001	Celii et al.	313/506
6,319,201 B1 *	11/2001	Wilk	600/437

OTHER PUBLICATIONS

Anonymous, "UDC Wins \$1 Million DARPA Program to Develop Flexible OLED Display", (visited Dec. 4, 2001) <<http://www.businesswire.com/webbox/bw.062200/201742456.htm>>.

* cited by examiner

Primary Examiner—Marvin M. Lateef


Assistant Examiner—Ruby Jain


(74) *Attorney, Agent, or Firm*—Dorsey & Whitney LLP

(57) **ABSTRACT**

A diagnostic ultrasonic imaging system includes an ultrasonic scanhead, an ultrasonic system chassis, and an organic light emitting device ("OLED") display. The OLED display has a response time of less than 10 ms, a contrast ratio of at least 1000:1, and a horizontal and vertical viewing angle of at least 160 degrees.

26 Claims, 3 Drawing Sheets

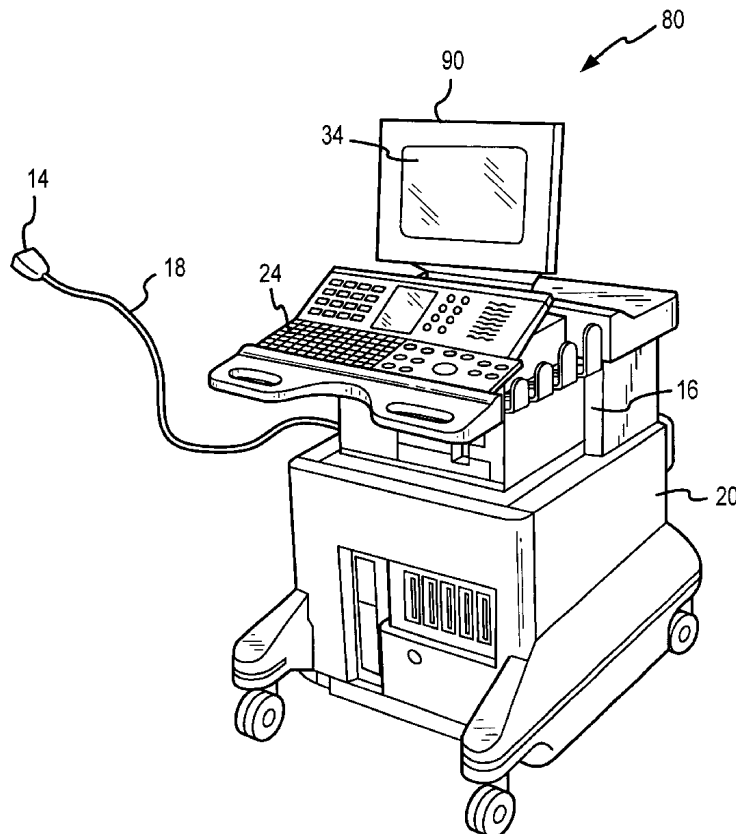

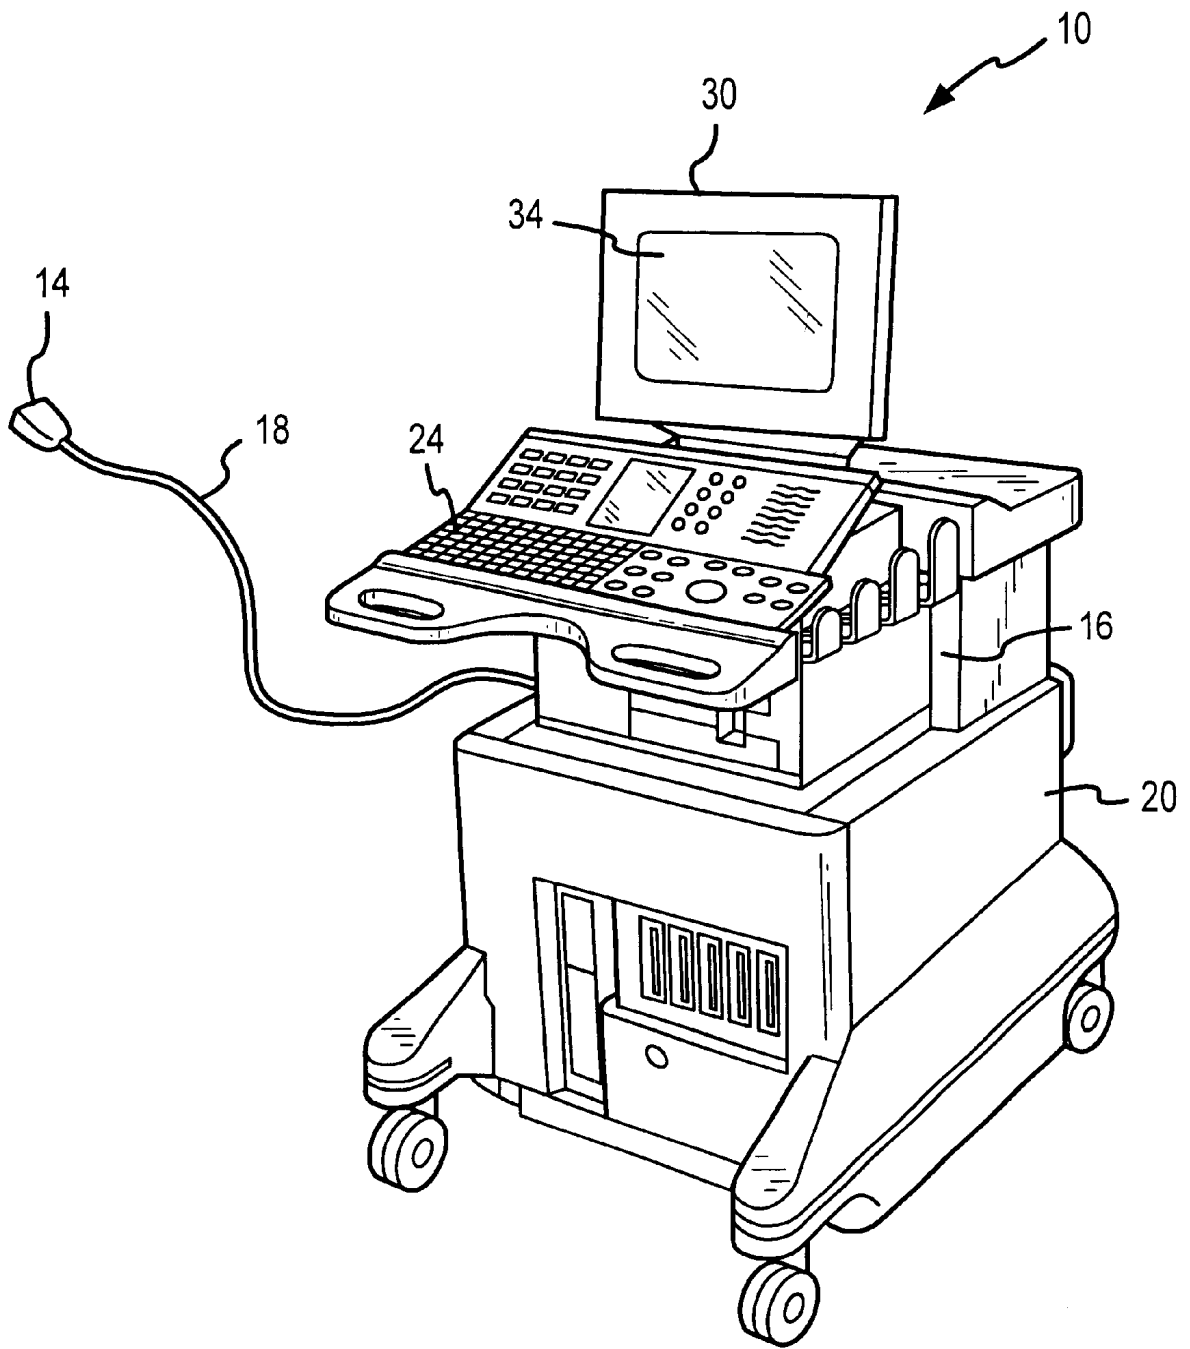

(PRIOR ART)
FIG. 1

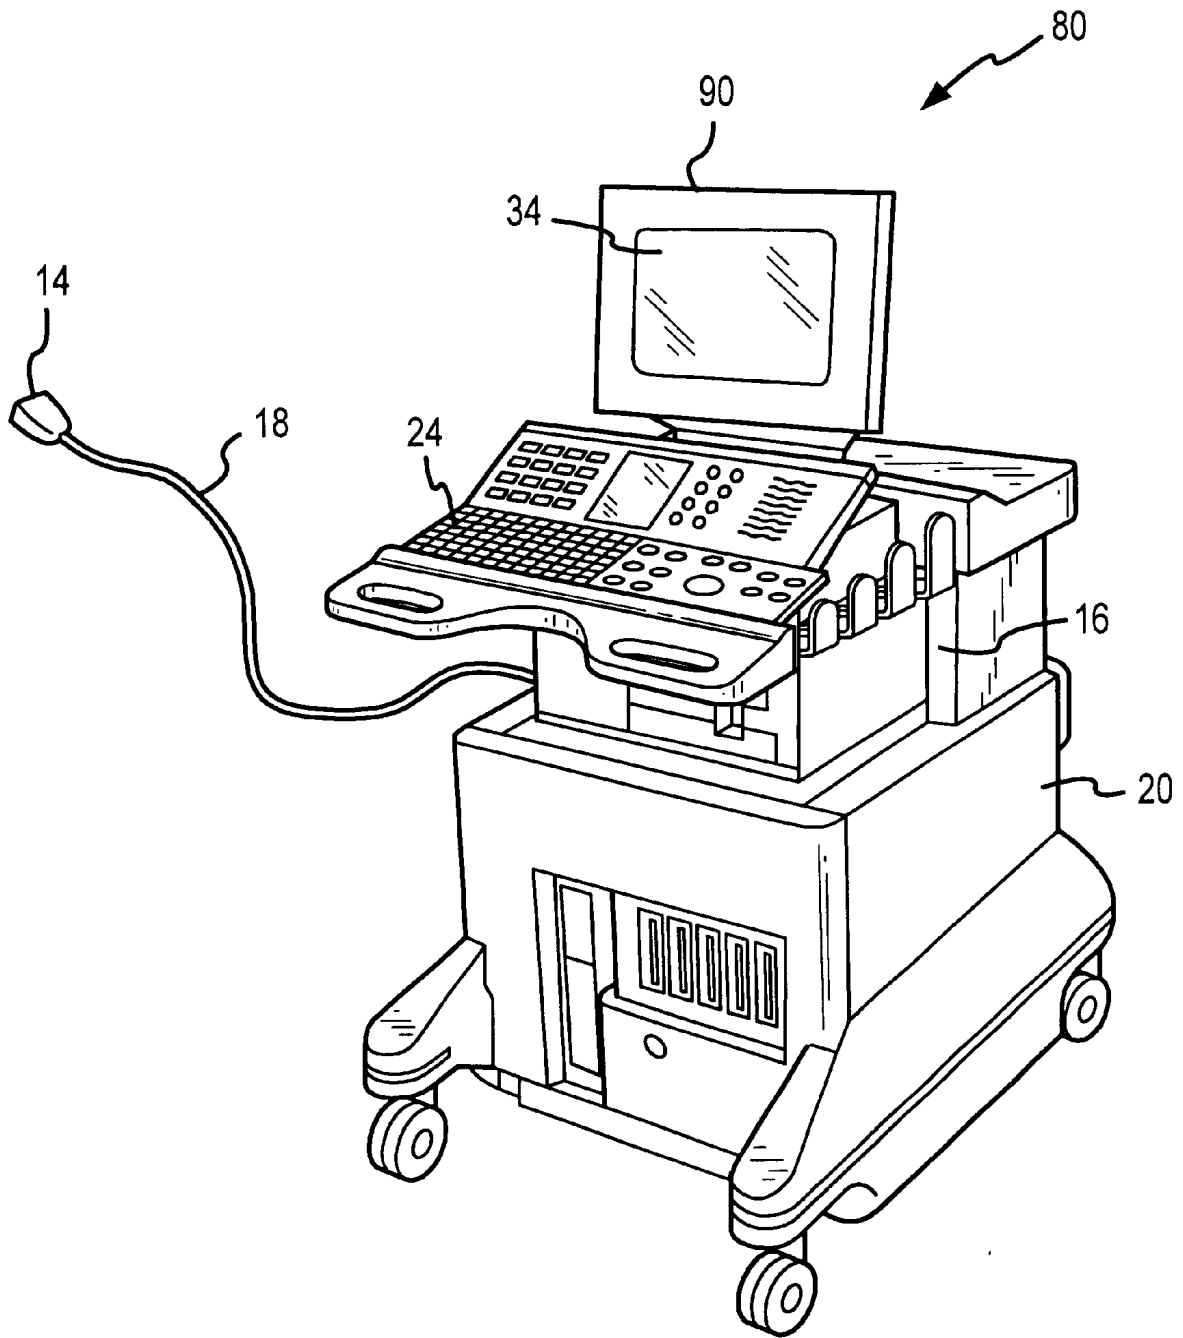


FIG.2

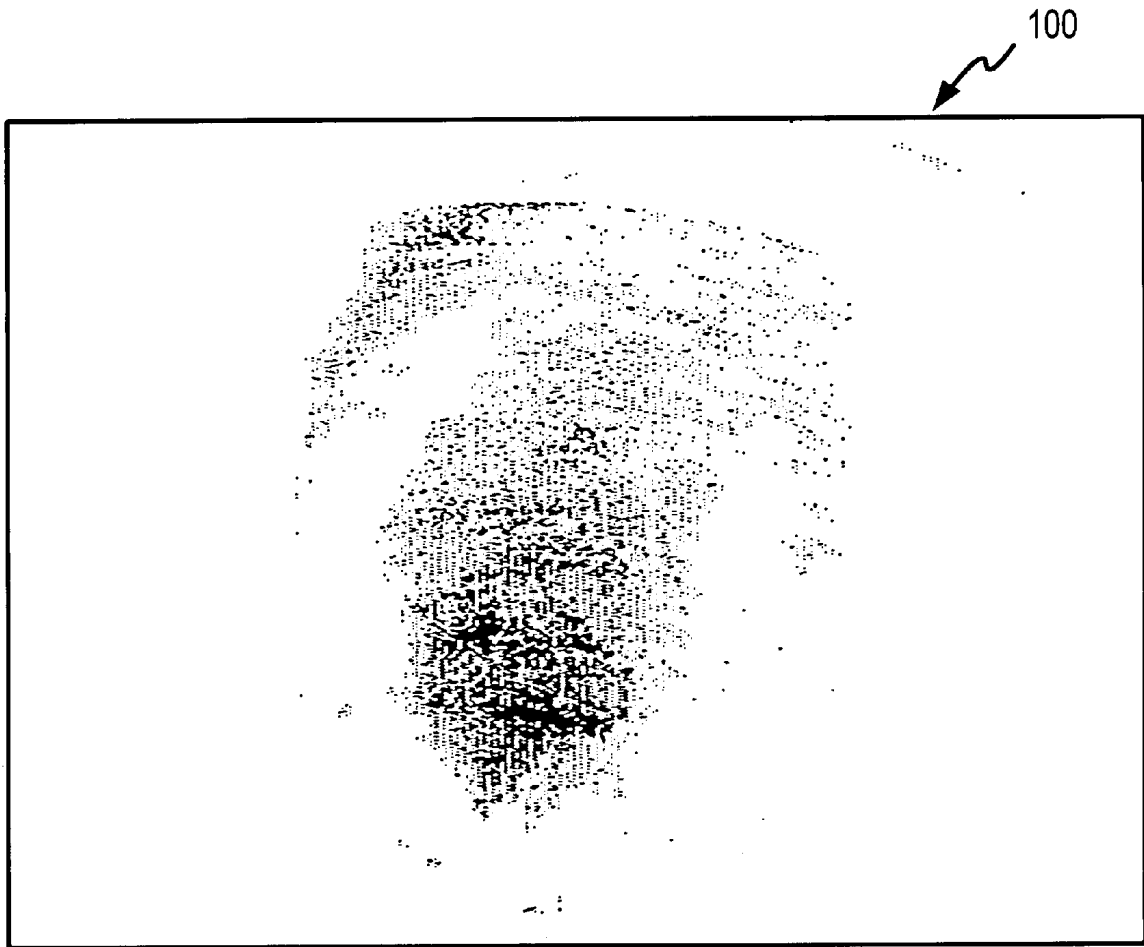


FIG.3

1

DIAGNOSTIC ULTRASONIC IMAGING SYSTEM HAVING ORGANIC LIGHT EMITTING DEVICE DISPLAY

TECHNICAL FIELD

This invention relates to diagnostic ultrasonic imaging systems, and more particularly, to diagnostic ultrasonic imaging systems displays that are optimally suited to displaying ultrasonic images.

BACKGROUND OF THE INVENTION

Diagnostic ultrasonic imaging systems are commonly used to image a wide variety of organs and tissues within the human body. A typical ultrasonic imaging system **10** is shown in FIG. **1**. The imaging system **10** includes an ultrasonic scanhead **14** that is adapted to be placed in contact with a portion of a body that is to be imaged. The scanhead **14** is coupled to a system chassis **16** by a cable **18**. The system chassis **16**, which is mounted on a cart **20**, includes a keyboard **24** by which data may be entered into a processor (not shown) that is included in the system chassis **16**. A display, which may be a cathode ray tube ("CRT") display or a flat panel display **30** having a viewing screen **34**, is placed on an upper surface of the system chassis **16**. Such flat panel displays **30**, such as liquid crystal displays ("LCD"), have been proposed for use in ultrasonic imaging system in, for example, U.S. Pat. No. 5,924,988 to Burris et al., which describes significant advantages that can be achieved by using a relatively thin and lightweight flat panel display.

The images displayed by conventional ultrasonic imaging systems have, in the past, been somewhat static. However, with the development of faster ultrasonic processors, it is possible to display real-time ultrasonic images of rapidly moving tissues and organs, such as a beating heart. However, it has been discovered that flat panel displays, such as liquid crystal displays, suggested for use in, for example, the above-cited patent to Burris et al., cannot optimally portray rapidly moving tissues and organs. This inability is due primarily to the relatively slow response times of conventional flat panel displays proposed for use in ultrasonic imaging systems. Thus, although the small size and light weight of flat panel displays proposed for use in ultrasonic imaging systems would provide many advantages, these advantages can be achieved only by sacrificing the ability to optimally display rapidly moving images.

Another problem that has been discovered with the use of flat panel displays proposed for use in ultrasonic monitoring systems is their lack of dynamic range or contrast ratio. It is often important to be able to discern subtle variations in the intensity of ultrasonic images. For example, it can be important to be able to differentiate an area reflecting substantially no ultrasonic energy, which should appear black, from an area reflecting a slight amount of ultrasonic energy, which should appear almost black. An ultrasonic image displayed on a flat panel display screen with insufficient dynamic range or contrast ratio will be unable to show the area reflecting substantially no ultrasonic energy darkly enough to differentiate that area from the area reflecting a slight amount of ultrasonic energy.

In addition to having a fast response time and a large dynamic range, a flat panel display used to view images in an ultrasonic imaging system should also have a wide viewing angle. The display of an ultrasonic imaging system

2

is often mounted on a cart, but the sonographer or other health care practitioner is often positioned off to the side of the cart next to a patient. Unless the display for the ultrasonic imaging system can be viewed from the side, it may be difficult for the health care practitioner to view the ultrasonic image without taking his or her attention away from the patient. Furthermore, even within the viewing angle of flat panel displays proposed for use in ultrasonic imaging, the color or brightness of the image can vary substantially as the viewing angle is varied.

A need therefore exists for an ultrasonic imaging system having a display that has a response time sufficiently short to display rapidly moving images, a dynamic range or contrast ratio sufficient to discern slight variations in the intensity of ultrasonic echoes, and a view angle that is sufficiently wide that the display can be easily viewed by a health care practitioner while devoting sufficient attention to a patient being examined.

SUMMARY OF THE INVENTION

An ultrasonic imaging system includes a system chassis, an ultrasonic scanhead coupled to the system chassis, and an organic light emitting device display coupled to the system chassis. The display includes a viewing screen on which an ultrasonic image can be displayed with superior response times, contrast ratios, and viewing angles. The response time of the organic light emitting device display is preferably less than 10 ms, and more preferably less than 1 ms. The contrast ratio of the organic light emitting device display is preferably at least 1000:1, and more preferably at least 4000:1. The horizontal and vertical viewing angle of the organic light emitting device display is preferably at least 160 degrees, and more preferably at least 180 degrees.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. **1** is an isometric view of a typical prior art cart-mounted diagnostic ultrasonic imaging system.

FIG. **2** is an isometric view of a cart-mounted diagnostic ultrasonic imaging system using an organic light emitting device ("OLED") display according to one embodiment of the invention.

FIG. **3** is a screen shot of an ultrasonic image displayed using the diagnostic ultrasonic imaging system of FIG. **2**.

DETAILED DESCRIPTION OF THE INVENTION

An ultrasonic imaging system **80** in accordance with one embodiment of the invention is shown in FIG. **2**. The ultrasonic imaging system **80** uses most of the same components as the imaging system **10** of FIG. **1**. Therefore, in the interest of brevity, these components have been provided with the same reference numerals, and an explanation of their operation will not be repeated. The imaging system **80** differs from the imaging system **10** of FIG. **1** in the use of an organic light emitting device ("OLED") display **90**. OLED displays are described in, for example, U.S. Pat. Nos. 5,920,080; 5,929,474; 6,069,443; 6,117,529; 6,191,433; 6,210,814; and 6,274,979, all of which are incorporated herein by reference. As described in detail below, the OLED display **90** provides the ultrasonic imaging system **80** with several advantages over the prior art imaging system **10** having a flat panel display **30**, as shown in FIG. **1**. The OLED display **90** used in the ultrasonic imaging system **80** is a color OLED display. However, it will be understood that the OLED display **90** may alternatively be a monochrome OLED display or an OLED display having a limited range of colors.

OLED displays, such as the OLED display **90** shown in FIG. 2, have a relatively short response time. For example compared with convention LCD flat panel displays, which typically have a response time greater than 20–50 ms, OLED displays have response times less than 1 ms. The OLED display **90** used in the ultrasonic imaging system **80** preferably has a response time of less than 10 ms, and more preferably a response time of less than 1 ms. As a result, the OLED display **90** is able to portray real time images of rapidly moving tissues and organs with significantly greater clarity than the conventional flat panel display **30** proposed for use in ultrasonic imaging systems.

The OLED display **90** also has a significantly wider dynamic range or contrast ratio than the flat panel display **30** shown in FIG. 1. As a result, it is possible to discern subtle differences in brightness of ultrasonic images shown in the display **90** compared to the ultrasonic imaging system **10** of FIG. 1. In part, this increased dynamic range is due to the degree of “blackness” that the display **90** is capable of generating in areas of the displayed image corresponding to areas from which little or no ultrasonic echoes are received. In one embodiment of the ultrasonic imaging system **80**, the OLED display **90** has a contrast ratio of at least 1,000:1, and preferably a contrast ratio of at least 4,000:1.

The OLED display **90** used in the ultrasonic imaging system **80** of FIG. 2 also has the advantage of a wide viewing angle compared to the flat panel display **30** used in the ultrasonic imaging system **10** of FIG. 1. In one embodiment, the OLED display **90** used in the imaging system **80** has a horizontal and vertical viewing angle of at least 160 degrees and, preferably a horizontal and vertical viewing angle of at least 180 degrees. If the OLED display is fabricated on a curved or flexible substrate, viewing angles in excess of 180 degrees are possible, such as viewing angles of 200 degrees. Within these viewing angles, an ultrasonic image presented on the display **90** can not only be viewed, but it can be viewed without substantial shifts in color or brightness as the viewing angle is varied. In contrast, the flat panel display **30**, such as an LCD display, used in the ultrasonic imaging system **10** typically has a horizontal and vertical viewing angle of no more than 160 degrees, and, within this viewing angle, the color and brightness of the displayed image can shift substantially as the viewing angle is varied. As a result, a sonographer or other health care practitioner can view a good quality image on the display **90** with relative ease while devoting adequate attention to a patient being examined.

An example of an ultrasonic image **100** that may be generated using the ultrasonic imaging system **80** is shown in FIG. 3. The image **100** is of a heart of an infant, which, as is known in the art, often beats very rapidly compared to the heart rate of an adult. As a result, the heart moves rapidly commensurate with this rapid heart beat. Despite the rapid heart beat, the image **100** is clearly shown because of the rapid response time, i.e., under 1 ms, of the OLED display **90** used in the system **80**. Furthermore, although not readily apparent in FIG. 3 because of the limitations on graphic rendering, subtle differences in the intensity of the image **100** can be discerned because the image has a contrast ratio of at least 1000:1 made possible by the high contrast ratio capabilities of the OLED display **90**. Finally, although also not apparent from FIG. 3, the horizontal and vertical viewing angle of the image **100** is at least 160 degrees and preferably up to 180 degrees.

While FIG. 2 illustrates the OLED display **90** in use with a cart-borne ultrasound system, it will be appreciated that the OLED display **90** is also well suited for use with smaller,

more portable ultrasound systems and ultrasound image viewing devices where the small size and light weight of the OLED display provides significant advantage. For example, the OLED display **90** may be used with a desktop, hand-carried, and handheld ultrasound systems, as well as with workstations for viewing and manipulating ultrasound images.

From the foregoing it will be appreciated that, although specific embodiments of the invention have been described herein for purposes of illustration, various modifications may be made without deviating from the spirit and scope of the invention. Accordingly, the invention is not limited except as by the appended claims.

What is claimed is:

1. An ultrasonic imaging system, comprising:

a system chassis;

an ultrasonic scanhead coupled to the system chassis; and
an organic light emitting device display coupled to the system chassis, the display having a viewing screen on which an ultrasonic image can be displayed.

2. The ultrasonic imaging system of claim 1, wherein the organic light emitting device display has a response time of less than 10 ms.

3. The ultrasonic imaging system of claim 2, wherein the organic light emitting device display has a response time of less than 1 ms.

4. The ultrasonic imaging system of claim 1, wherein the organic light emitting device display has a contrast ratio of at least 1000:1.

5. The ultrasonic imaging system of claim 4, wherein the organic light emitting device display has a contrast ratio of at least 2000:1.

6. The ultrasonic imaging system of claim 1, wherein the organic light emitting device display has a horizontal and vertical viewing angle of at least 160 degrees.

7. The ultrasonic imaging system of claim 6, wherein the organic light emitting device display has a horizontal and vertical viewing angle of at least 180 degrees.

8. The ultrasonic imaging system of claim 1, wherein the organic light emitting device display comprises a color organic light emitting device display.

9. An ultrasonic imaging system, comprising:

a system chassis;

an ultrasonic scanhead coupled to the system chassis; and
a flat panel display coupled to the system chassis, the flat panel display having a viewing screen on which an ultrasonic image can be displayed, the flat panel display having a response time of less than 10 ms.

10. The ultrasonic imaging system of claim 9, wherein the flat panel display comprises a flat panel display having a response time of less than 1 ms.

11. The ultrasonic imaging system of claim 9, wherein the flat panel display comprises an organic light emitting device display.

12. The ultrasonic imaging system of claim 11, wherein the organic light emitting device display comprises a color organic light emitting device display.

13. An ultrasonic imaging system, comprising:

a ultrasound image processor; and

an organic light emitting device display coupled to the system chassis, the display having a viewing screen on which an ultrasonic image can be displayed.

14. The ultrasonic imaging system of claim 13, wherein the ultrasound image processor comprises a desktop unit.

15. The ultrasonic imaging system of claim 13, wherein the ultrasound image processor comprises a diagnostic image workstation.

5

16. An ultrasonic imaging system, comprising:
a system chassis;

an ultrasonic scanhead coupled to the system chassis; and
a flat panel display coupled to the system chassis, the flat
panel display having a viewing screen on which an
ultrasonic image can be displayed, the flat panel display
having a horizontal and vertical viewing angle of at
least 160 degrees.

17. The ultrasonic imaging system of claim 16, wherein
the flat panel display comprises a flat panel display having
a horizontal and vertical viewing angle of at least 180
degrees.

18. The ultrasonic imaging system of claim 16, wherein
the flat panel display comprises an organic light emitting
device display.

19. The ultrasonic imaging system of claim 18, wherein
the organic light emitting device display comprises a color
organic light emitting device display.

20. A diagnostic ultrasonic image of an object, the image
being shown with a response time of less than 10 ms, a
contrast ratio of at least 1000:1 and a horizontal and vertical
viewing angle of at least 160 degrees.

21. The diagnostic ultrasonic image of claim 20, wherein
the image is shown with a response time of less than 1 ms,
a contrast ratio of at least 4000:1 and a horizontal and
vertical viewing angle of at least 200 degrees.

6

22. A method of displaying an ultrasonic image, compris-
ing:

providing an ultrasonic imaging system, including an
organic light emitting device display having a viewing
screen;

obtaining data corresponding to an ultrasonic image; and
displaying the ultrasonic image on the viewing screen of
the organic light emitting device display.

23. The method of claim 22, wherein the act of providing
an ultrasonic imaging system including an organic light
emitting device display comprises providing an ultrasonic
imaging system including a color organic light emitting
device display.

24. The ultrasonic imaging system of claim 17, wherein
the flat panel display comprises a flat panel display having
a horizontal and vertical viewing angle of at least 200
degrees.

25. The ultrasonic imaging system of claim 25, wherein
the flat panel display comprises a flat panel display having
a horizontal and vertical viewing angle of at least 180
degrees.

26. The ultrasonic imaging system of claim 25, wherein
the flat panel display comprises a flat panel display having
a horizontal and vertical viewing angle of at least 200
degrees.

* * * * *

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 6,579,237 B1
DATED : June 17, 2003
INVENTOR(S) : Stan Knoblich

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page,

Item [56], **References Cited**, OTHER PUBLICATIONS, "Anonymous" reference, reads "OLED Display", visited" should read -- OLED Display" (visited --

Column 1,

Line 29, reads "system in, for example," should read -- systems in, for example, --

Column 2,


Lines 57-58, reads "5,920,080; 5,929,474; 6,069,443; 6,117,529; 6,191,433; 6,210,814; and" should read -- 5,920,080, 5,929,474, 6,069,443, 6,117,529, 6,191,433, 6,210,814 and --

Column 6,

Line 18, reads "system of claim **25**, "wherein" should read -- system of claim **20**, wherein --

Signed and Sealed this

Eighteenth Day of May, 2004

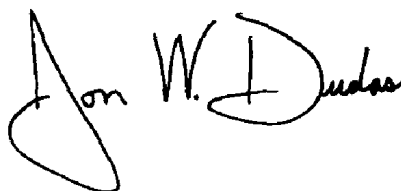

JON W. DUDAS
Acting Director of the United States Patent and Trademark Office

专利名称(译)	诊断超声成像系统具有有机发光装置显示器		
公开(公告)号	US6579237	公开(公告)日	2003-06-17
申请号	US10/022261	申请日	2001-12-14
[标]申请(专利权)人(译)	KNOBLICH STAN		
申请(专利权)人(译)	KNOBLICH STAN		
当前申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
[标]发明人	KNOBLICH STAN		
发明人	KNOBLICH, STAN		
IPC分类号	A61B8/08 G01N29/44 A61B8/00 G01S7/52 G01S15/89		
CPC分类号	A61B8/08 G01S7/52053 A61B8/462 A61B8/4405		
代理机构(译)	德汇律师事务所律师事务所		
助理审查员(译)	JAIN , RUBY		
其他公开文献	US20030114754A1		
外部链接	Espacenet USPTO		

摘要(译)

诊断超声成像系统包括超声扫描头，超声系统底盘和有机发光装置 (“OLED”) 显示器。OLED显示器具有小于10ms的响应时间，至少1000 : 1的对比度，以及至少160度的水平和垂直视角。

