



US 20020151798A1

(19) **United States**(12) **Patent Application Publication**(10) **Pub. No.: US 2002/0151798 A1****Honda**(43) **Pub. Date:****Oct. 17, 2002**

(54) **ULTRASONIC TRANSMISSION/RECEPTION METHOD, ULTRASONIC TRANSMISSION/RECEPTION APPARATUS, ULTRASONIC IMAGING METHOD AND ULTRASONIC IMAGING APPARATUS**

(30) **Foreign Application Priority Data**

Apr. 11, 2001 (JP) 2001-112466

Publication Classification(76) **Inventor: Masayoshi Honda, Tokyo (JP)**(51) **Int. Cl.⁷** **A61B 8/14**(52) **U.S. Cl.** **600/458**

Correspondence Address:

JOHN S. BEULICK**C/O ARMSTRONG TEASDALE, LLP****ONE METROPOLITAN SQUARE****SUITE 2600****ST LOUIS, MO 63102-2740 (US)**(57) **ABSTRACT**

In order to capture an ultrasonic image of high quality using ultrasound having a low sound pressure that does not break a contrast agent, scanning is performed during a pause period of intermittent scanning, using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation; pulse compression is performed on an echo received signal; and an image is produced based on the pulse-compressed echo received signal.

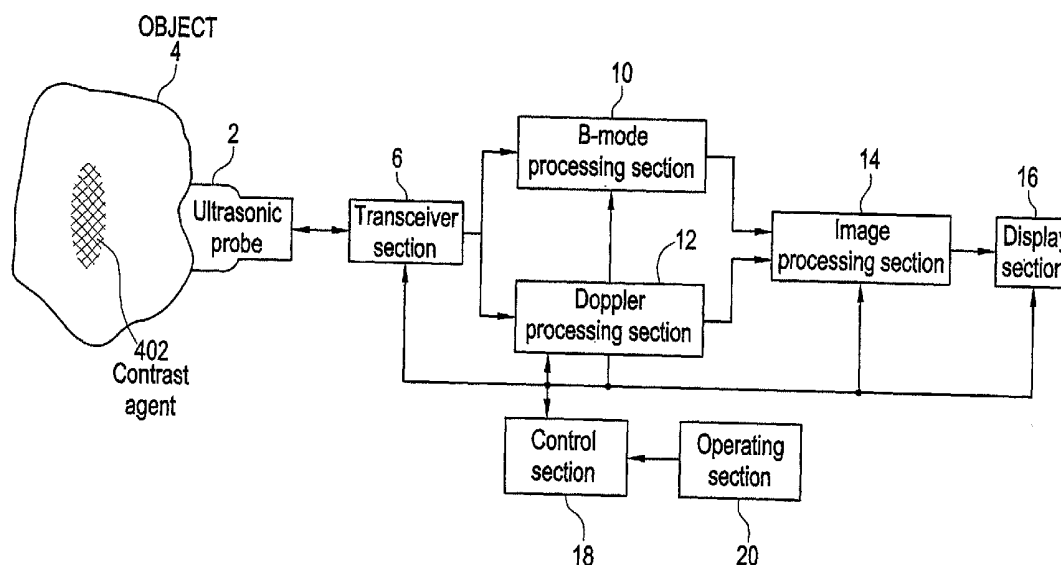
(21) **Appl. No.: 10/119,252**(22) **Filed: Apr. 9, 2002**

FIG. 1

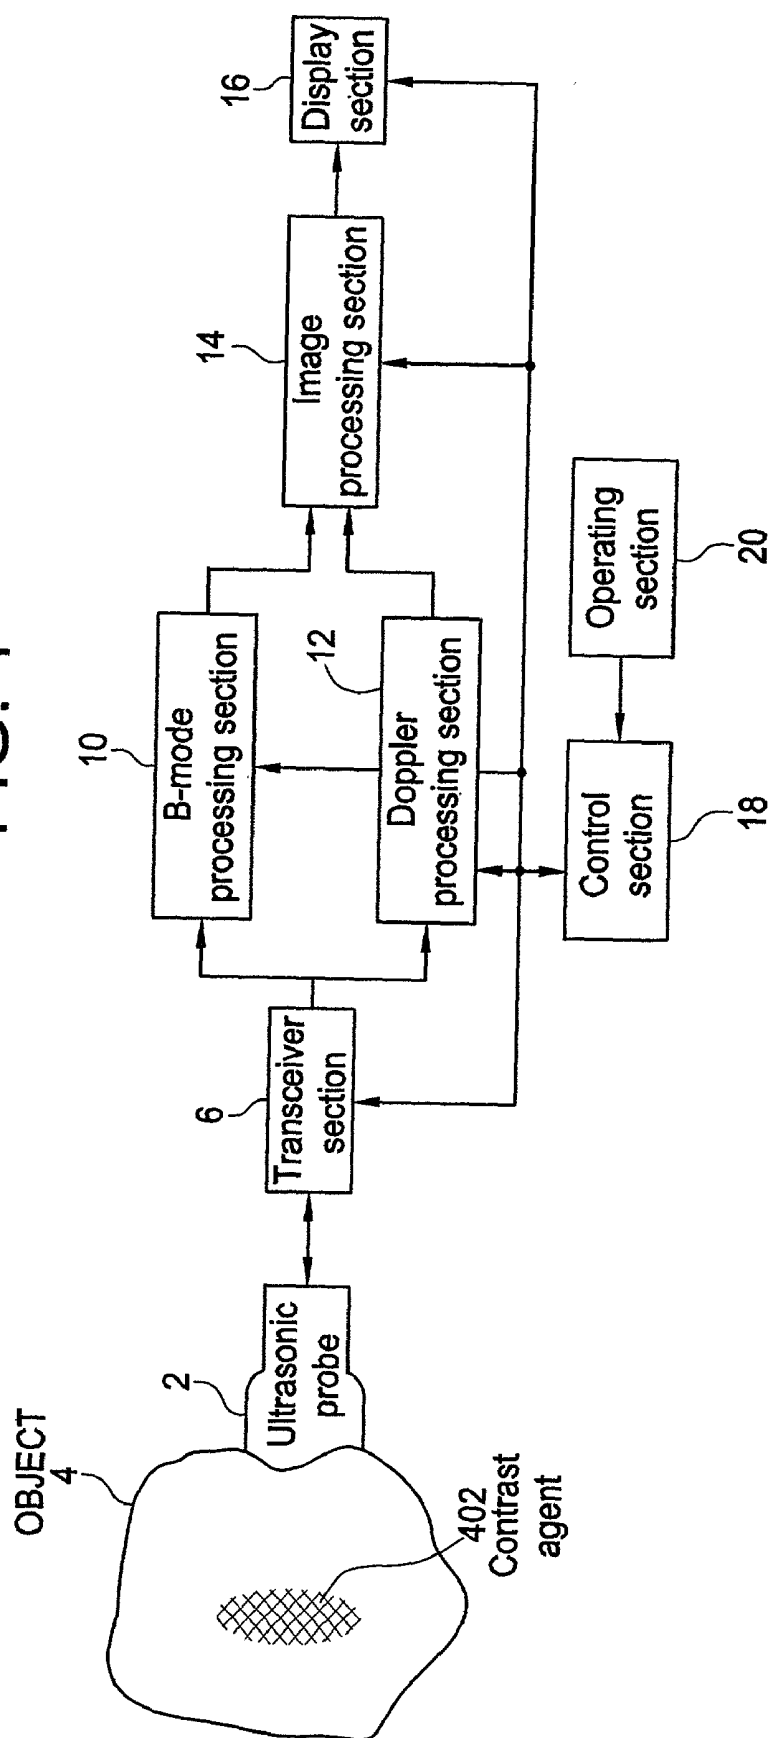


FIG. 2

6

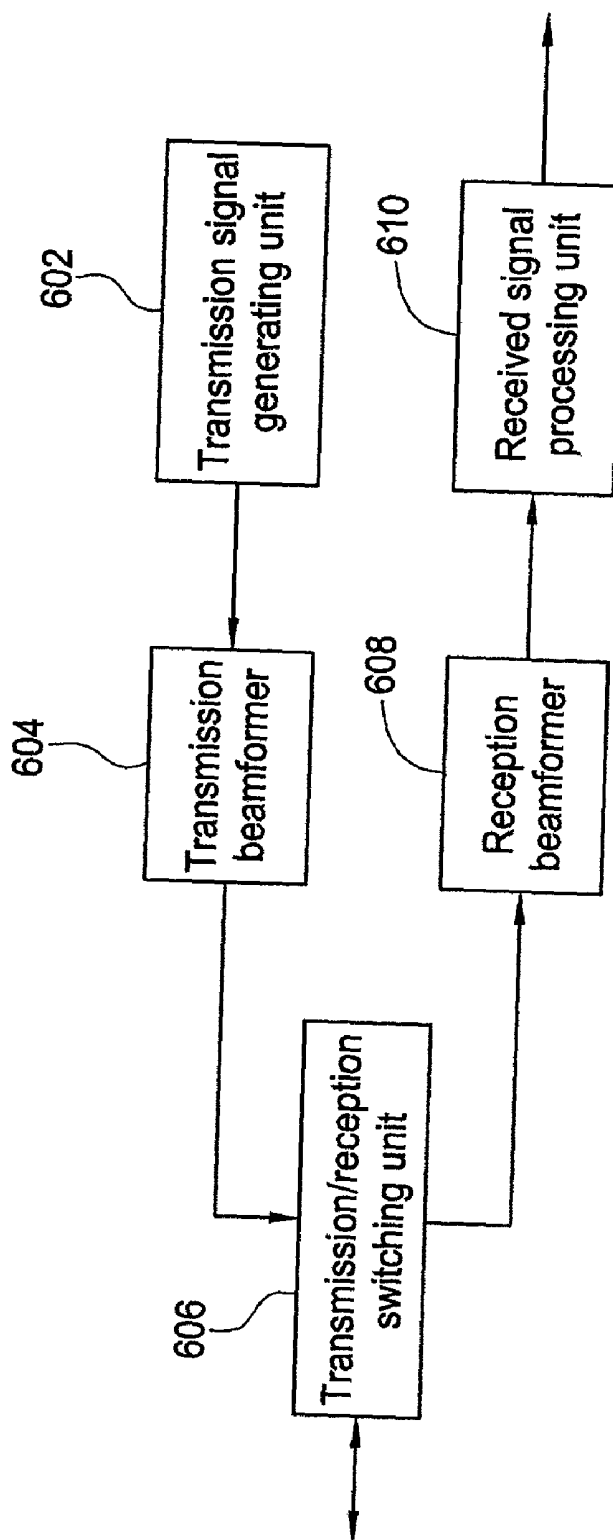


FIG. 3

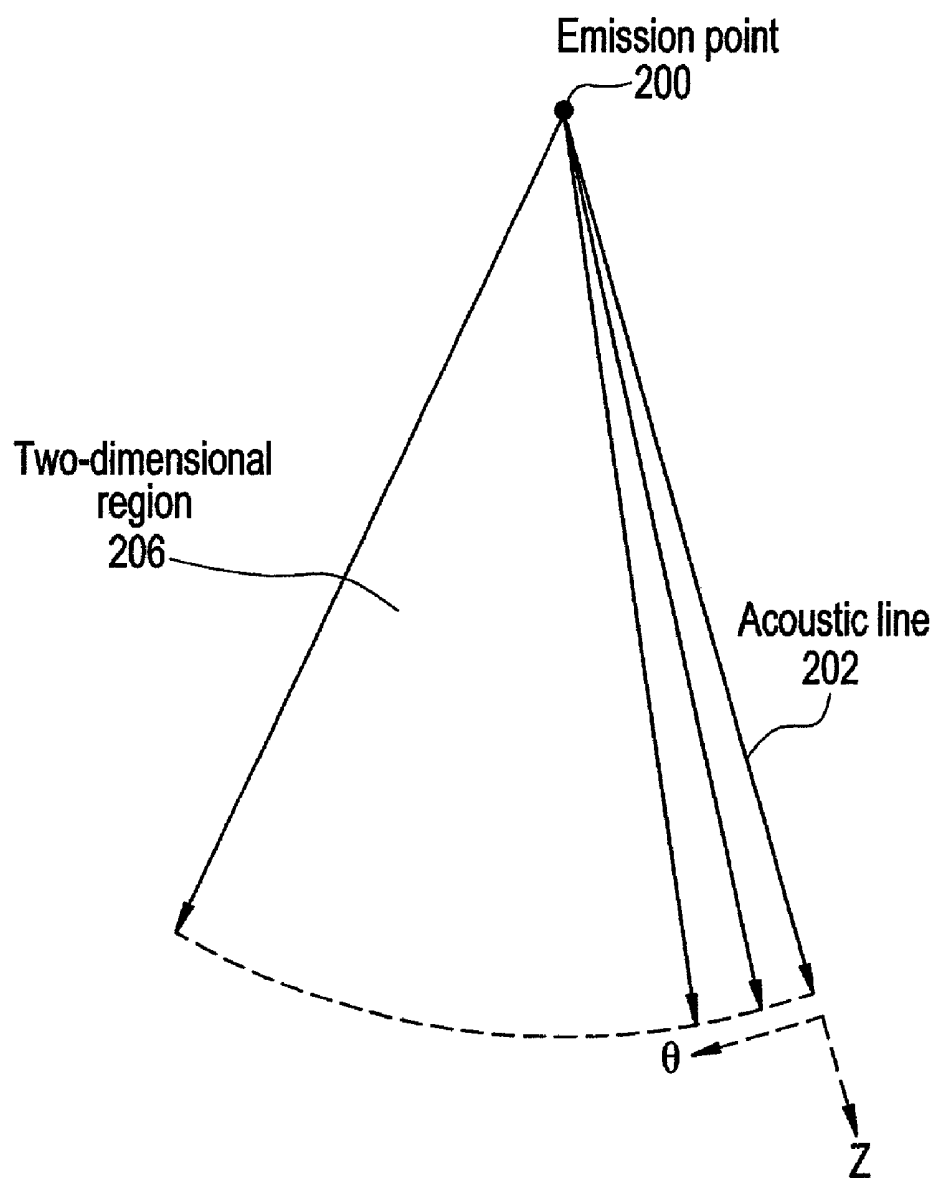


FIG. 4

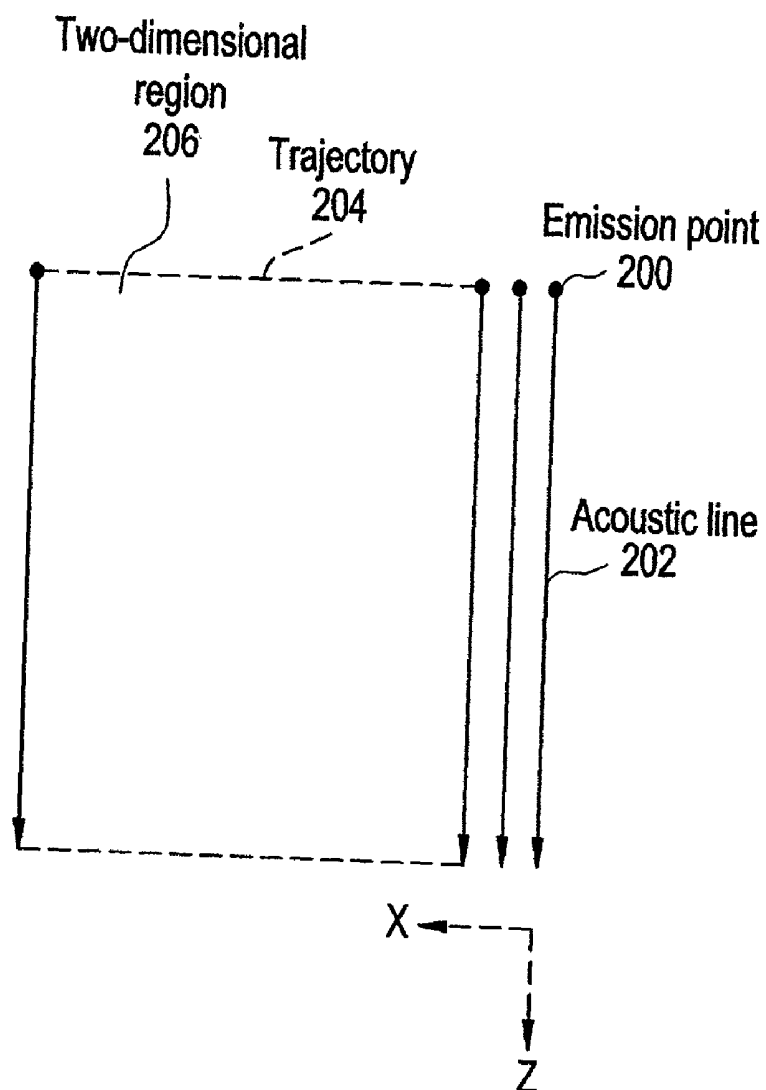


FIG. 5

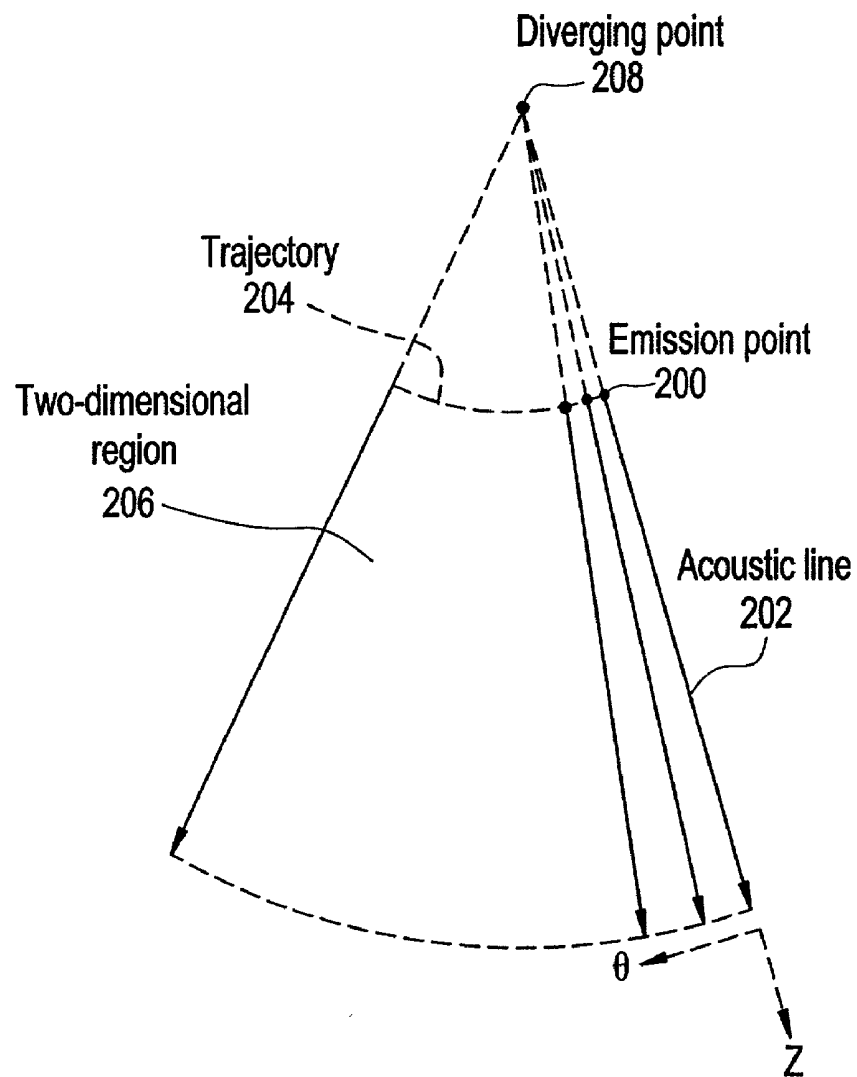


FIG. 6

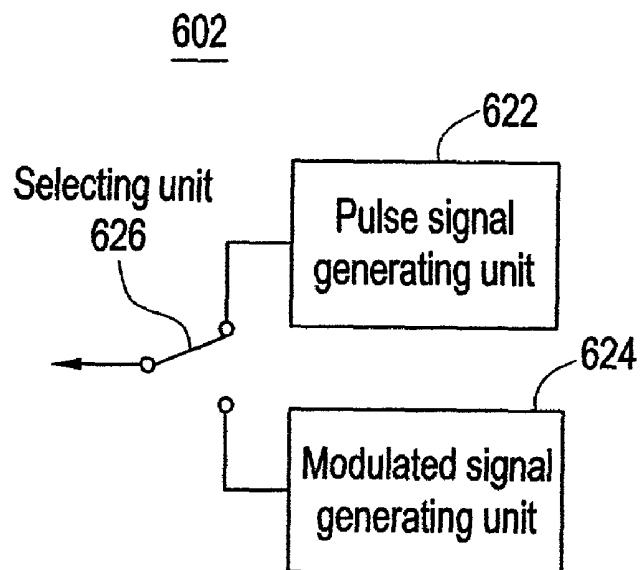


FIG. 7

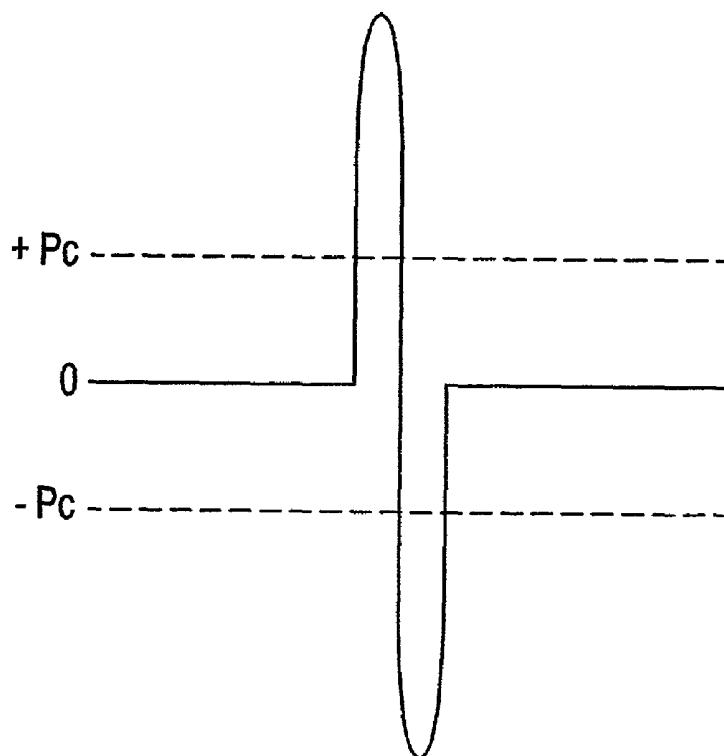


FIG. 8

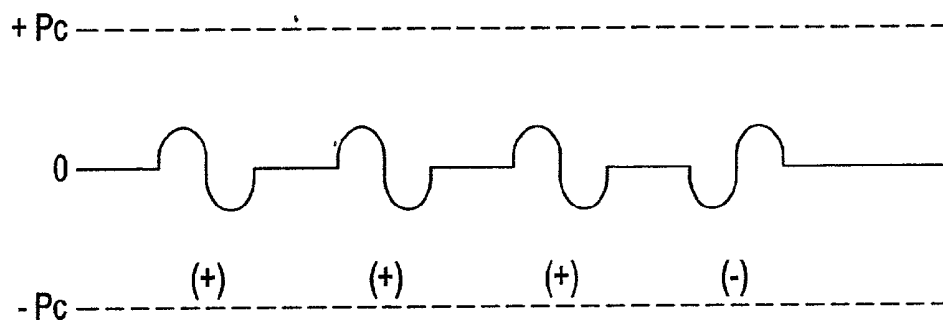
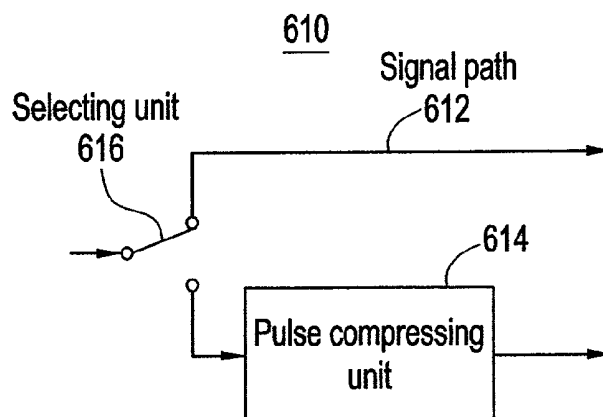


FIG. 9

Code Length	Code Sequence
N=2	++ or +-
N=3	++ -
N=4	++-+ or +++-
N=5	+++ - +
N=7	+++--+-
N=11	+++---+---+-
N=13	+++++---++-+-+

FIG. 10



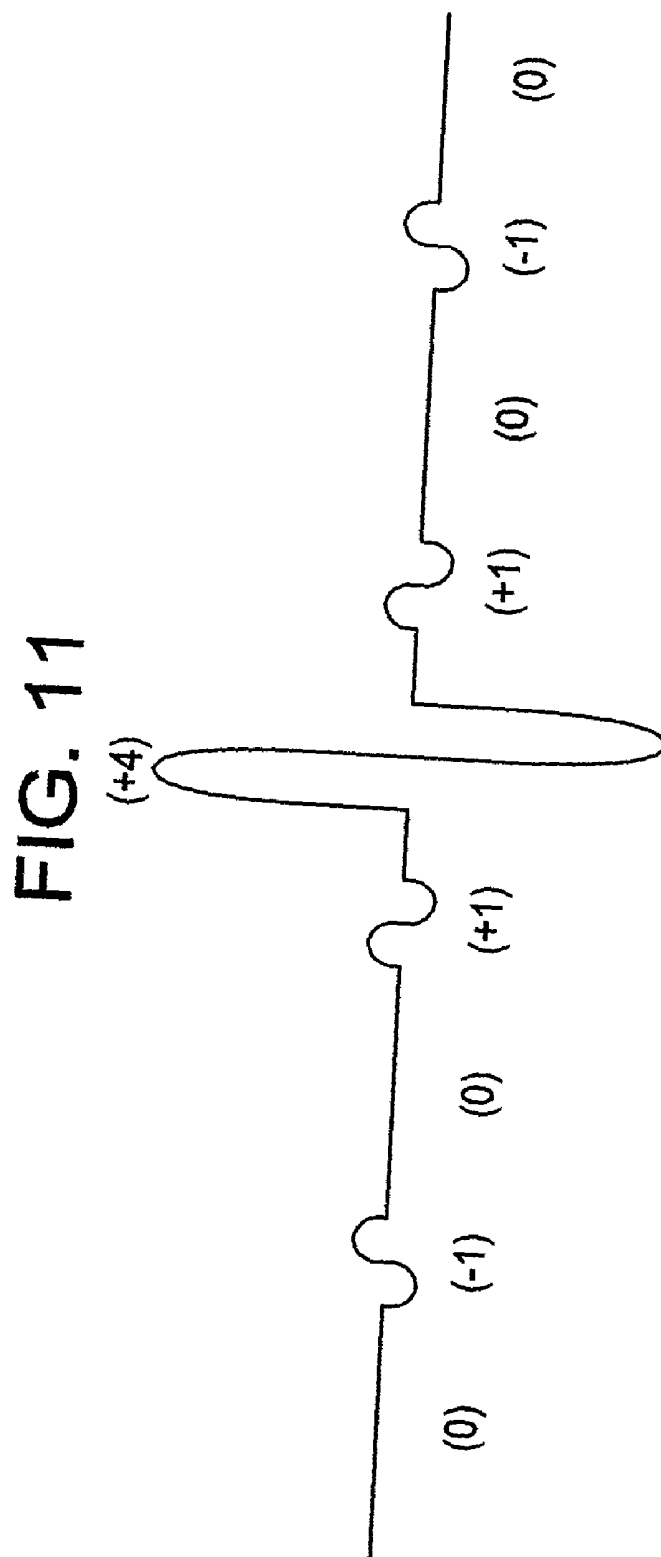


FIG. 12

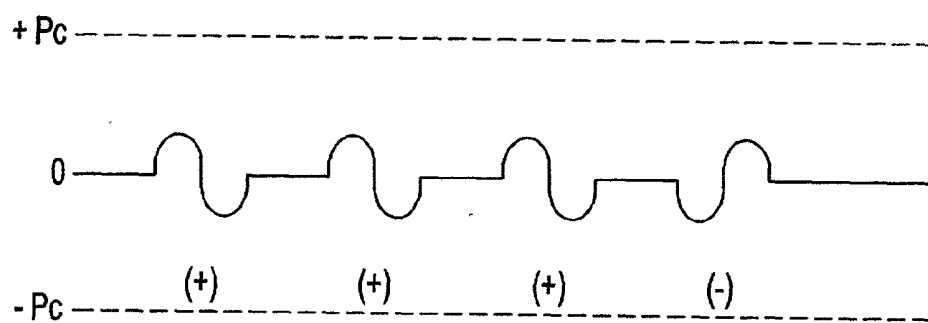


FIG. 13

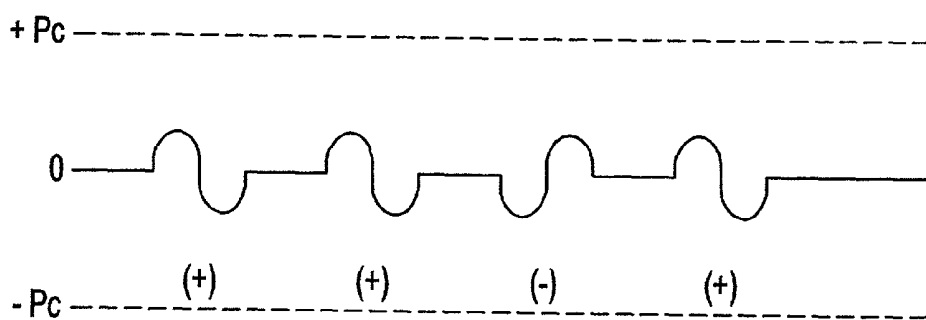


FIG. 14

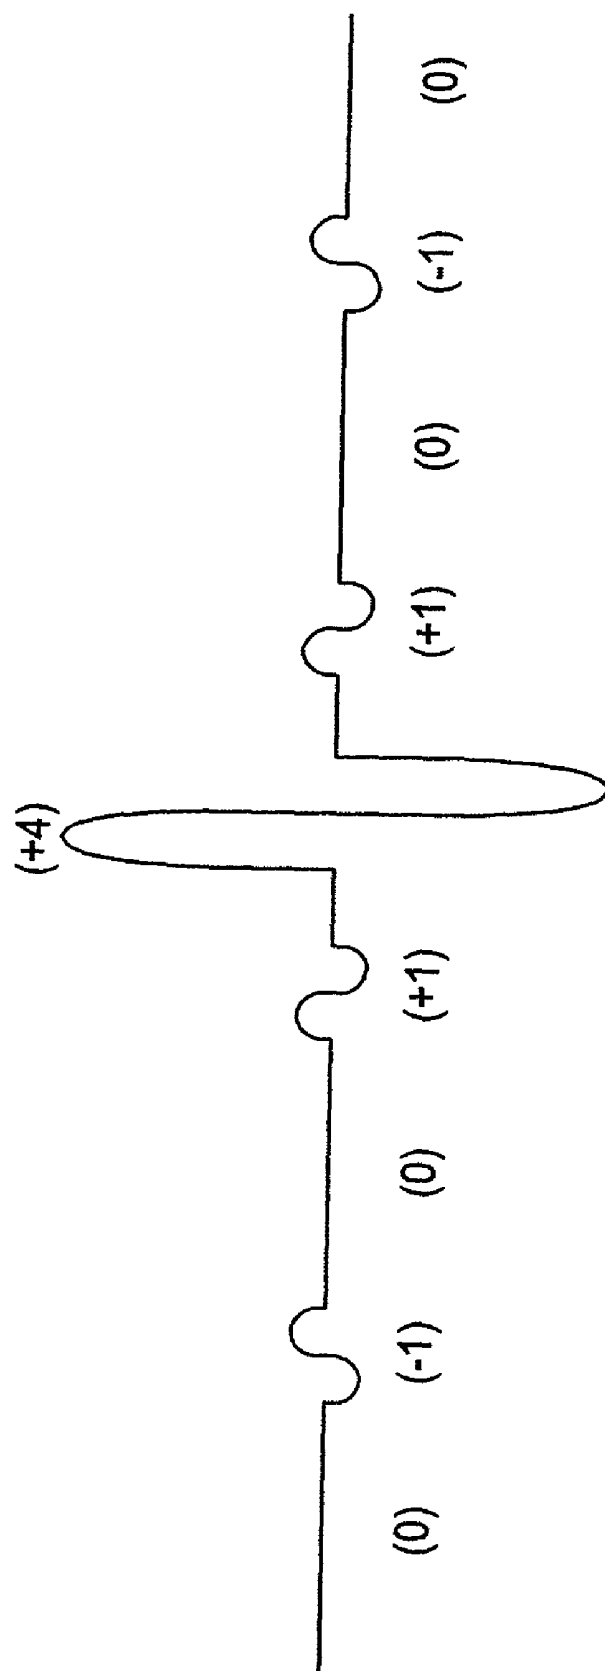


FIG. 15

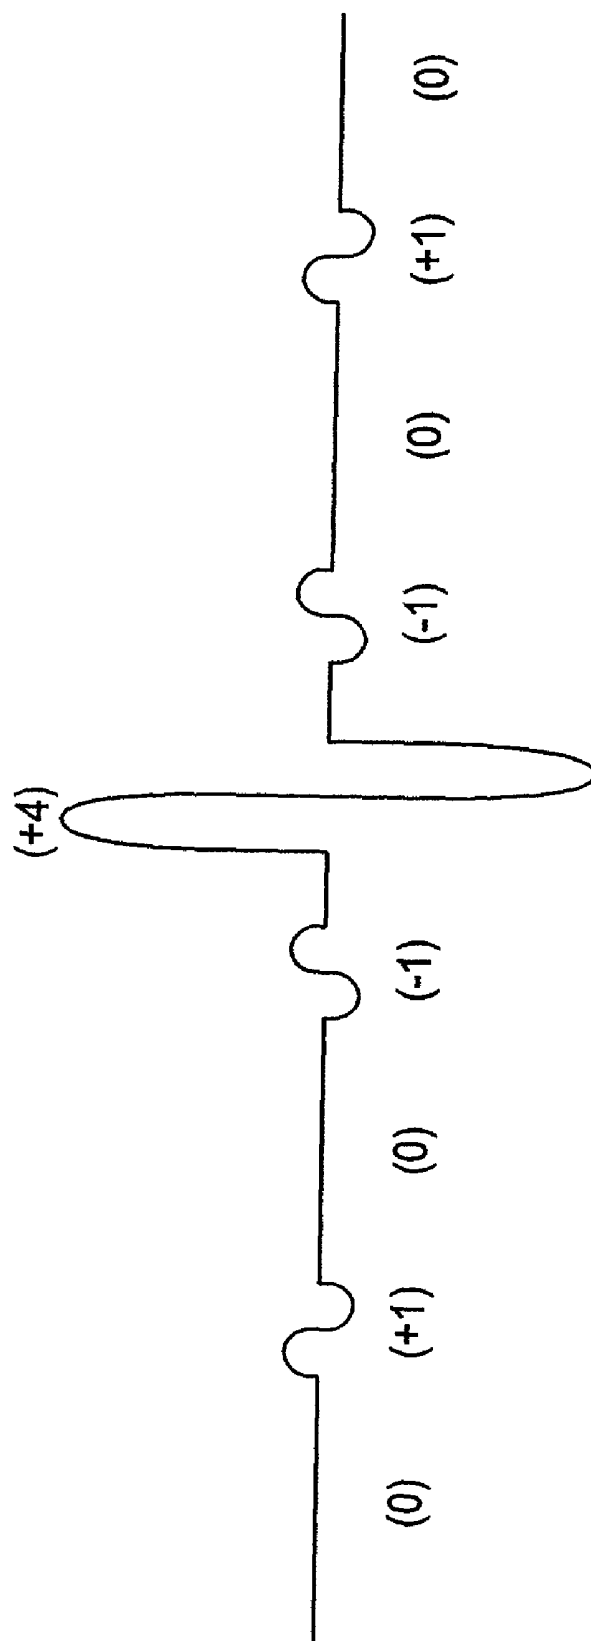


FIG. 16

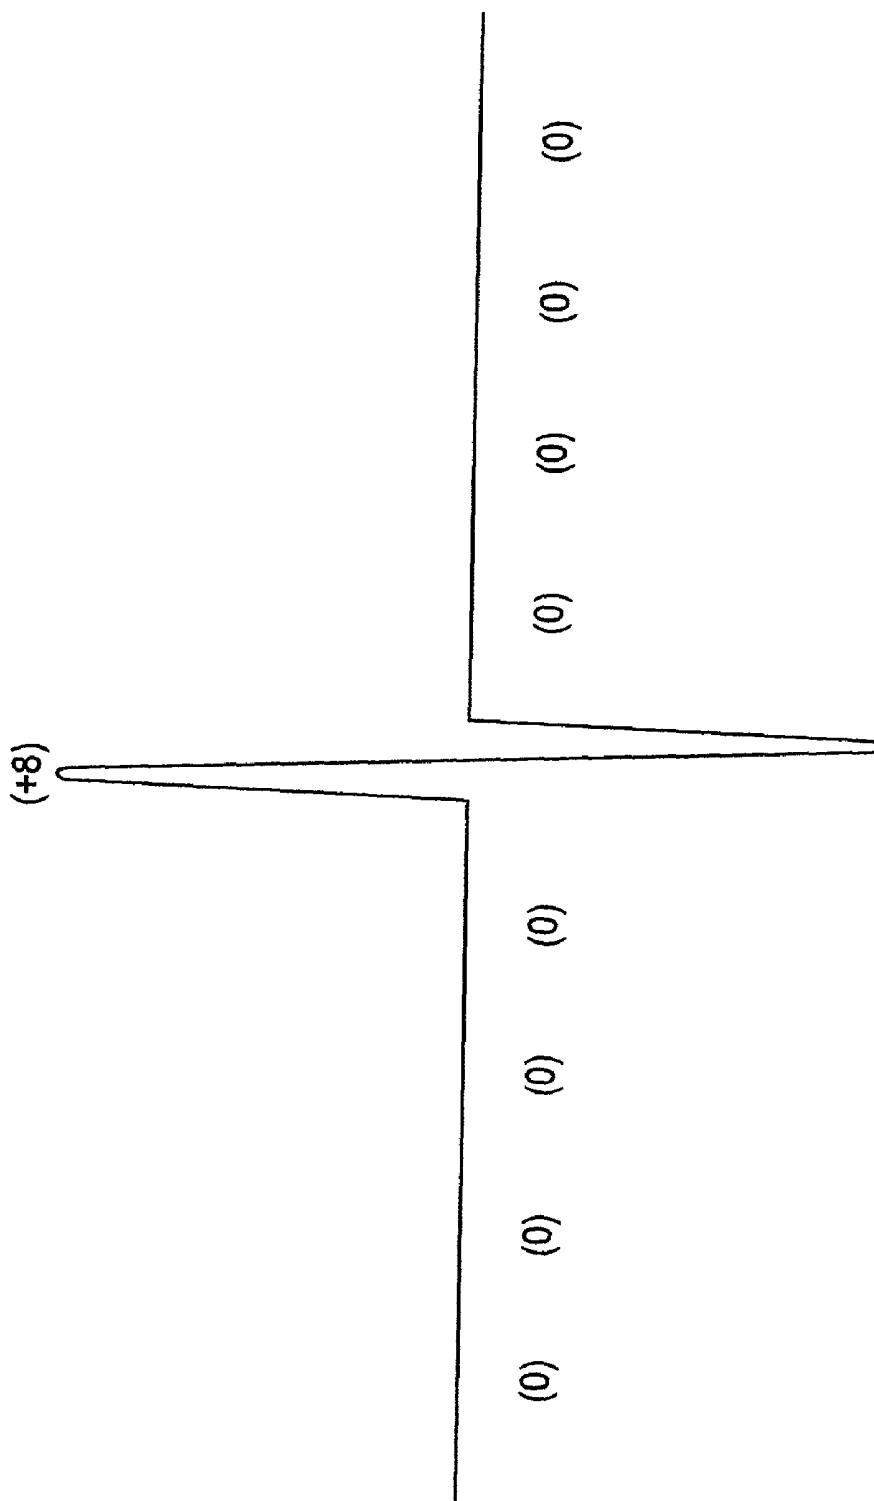


FIG. 17A

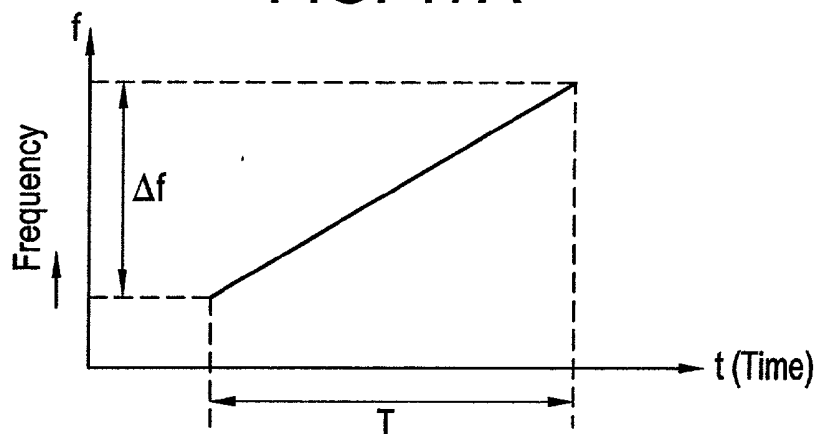


FIG. 17B



FIG. 17C

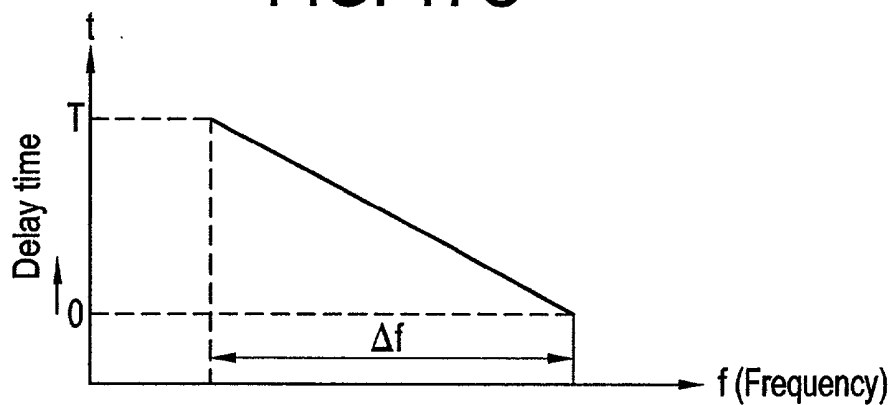


FIG. 17D

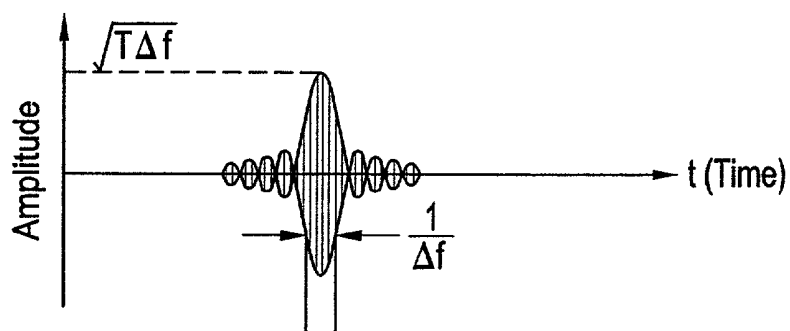
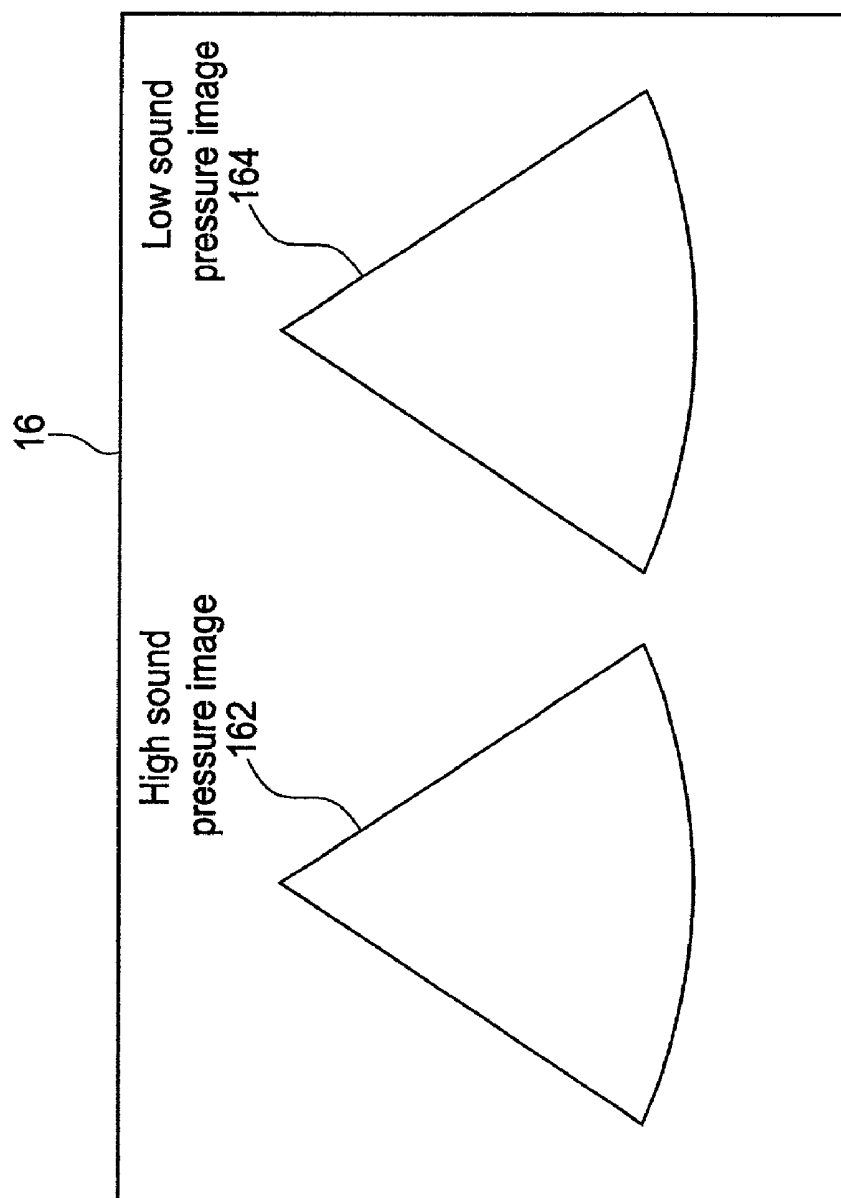


FIG. 18



**ULTRASONIC TRANSMISSION/RECEPTION
METHOD, ULTRASONIC
TRANSMISSION/RECEPTION APPARATUS,
ULTRASONIC IMAGING METHOD AND
ULTRASONIC IMAGING APPARATUS**

BACKGROUND OF THE INVENTION

[0001] The present invention relates to an ultrasonic transmission/reception method, ultrasonic transmission/reception apparatus, ultrasonic imaging method and ultrasonic imaging apparatus, and particularly to an ultrasonic transmission/reception method, ultrasonic transmission/reception apparatus, ultrasonic imaging method and ultrasonic imaging apparatus for imaging an object into which an ultrasonic contrast agent is injected.

RELATED ART

[0002] In ultrasonic imaging, an echo of ultrasound transmitted into an object is used to capture a tomographic image, and the image is displayed as a B-mode image. Moreover, a Doppler shift of the ultrasonic echo is used to capture a dynamic image of blood flow etc., and the image is displayed as a color Doppler image.

[0003] When the signal intensity of the echo needs to be increased, a region of interest (ROI) is infused with a contrast agent using the blood flow. The contrast agent is a collection of microscopic bubbles having a diameter of several micrometers.

[0004] Such a contrast agent is broken up and disappears when exposed to ultrasound having a sound pressure greater than a certain level and will generate no echo next time. Therefore, the next imaging is performed after the contrast agent has again reached the site being imaged.

[0005] For this reason, the ultrasonic imaging using the contrast agent performs intermittent image capture (scanning) with a pause period of, for example, from several seconds to several tens of seconds after every imaging. Each tomographic image obtained from the scanning is displayed as a freeze image and is updated every time the next scanning image is obtained.

[0006] In order to make it possible to observe the state of the imaged site in real time during the pause period, the same region is imaged using ultrasound having a sound pressure reduced to a degree such that it does not break the contrast agent.

[0007] However, the image captured using the ultrasound having a sound pressure reduced to a degree such that it does not break the contrast agent has poor quality because of the low SNR (signal-to-noise ratio) of the echo received signal.

SUMMARY OF THE INVENTION

[0008] It is therefore an object of the present invention is to provide an ultrasonic transmission/reception method, ultrasonic transmission/reception apparatus, ultrasonic imaging method and ultrasonic imaging apparatus that enable an image to be obtained with high quality using ultrasound having a sound pressure reduced to a degree such that it does not break a contrast agent.

[0009] (1) The present invention, in one aspect thereof for solving the aforementioned problem, is an ultrasonic transmission/reception method, comprising the steps of: intermittently scanning an imaged region with a predetermined pause period using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; continuously scanning the same region as the imaged region during the pause period using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; and performing pulse compression on an echo received signal obtained by the continuous scanning.

[0010] (2) The present invention, in another aspect thereof for solving the aforementioned problem, is an ultrasonic transmission/reception apparatus, comprising: first ultrasound transmitting/receiving means for scanning an imaged region using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; second ultrasound transmitting/receiving means for scanning the same region as the imaged region using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; pulse compressing means for performing pulse compression on an echo received signal from the second ultrasound transmitting/receiving means; and control means for causing the first ultrasound transmitting/receiving means to intermittently perform the scanning with a predetermined pause period, and causing the second ultrasound transmitting/receiving means to continuously perform the scanning during the pause period.

[0011] (3) The present invention, in still another aspect thereof for solving the aforementioned problem, is an ultrasonic imaging method, comprising the steps of: intermittently scanning an imaged region with a predetermined pause period using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; continuously scanning the same region as the imaged region during the pause period using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; performing pulse compression on an echo received signal obtained by the continuous scanning; and producing respective images based on an echo received signal obtained by the intermittent scanning and on an echo received signal after the pulse compression.

[0012] (4) The present invention, in still another aspect thereof for solving the aforementioned problem, is an ultrasonic imaging apparatus, comprising: first ultrasound transmitting/receiving means for scanning an imaged region using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; second ultrasound transmitting/receiving means for scanning the same region as the imaged region using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; pulse compressing means for performing pulse compression on an echo received signal from the second ultrasound transmitting/receiving means; control means for causing the first ultrasound transmitting/receiving means to intermittently perform the scanning with a predetermined pause period, and

causing the second ultrasound transmitting/receiving means to continuously perform the scanning during the pause period; and image producing means for producing respective images based on an echo received signal from the first ultrasound transmitting/receiving means and on an echo received signal after the pulse compression from the second ultrasound transmitting/receiving means.

[0013] According to the invention of the aspects as described in (1) and (2), during the pause period, scanning is performed using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, an echo of the ultrasound is received, and the echo received signal is subjected to pulse compression; and therefore, an echo received signal can be obtained with a good SNR even if the transmitted ultrasound has a low sound pressure.

[0014] According to the invention of the aspects as described in (3) and (4), during the pause period, scanning is performed using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and the echo received signal is subjected to pulse compression; and therefore, an echo received signal can be obtained with a good SNR even if the transmitted ultrasound has a low sound pressure. Moreover, since an image is produced based on such an echo received signal, an image of good quality can be obtained.

[0015] Preferably, the modulation is code modulation, in that the modulation of the transmitted ultrasound and the pulse compression of the echo received signal can be effectively performed.

[0016] Preferably, a code sequence for the code modulation is a Barker code, in that such a code has been well-established in practical applications such as radar technology.

[0017] Preferably, a code sequence for the code modulation is a Golay code, in that such a code has been well-established in practical applications such as radar technology, and it generates no side lobe.

[0018] Preferably, the modulation is linear frequency modulation, in that the modulation of the transmitted ultrasound and the pulse compression of the echo received signal can be easily achieved.

[0019] As described above in detail, the present invention can provide an ultrasonic transmission/reception method, ultrasonic transmission/reception apparatus, ultrasonic imaging method and ultrasonic imaging apparatus that enable an image to be obtained with high quality using ultrasound having a sound pressure reduced to a degree such that the ultrasound does not break a contrast agent.

[0020] Further objects and advantages of the present invention will be apparent from the following description of the preferred embodiments of the invention as illustrated in the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021] FIG. 1 is a block diagram of an apparatus in accordance with one embodiment of the present invention.

[0022] FIG. 2 is a block diagram of a transceiver section.

[0023] FIGS. 3-5 are schematic diagrams of acoustic line scanning.

[0024] FIG. 6 is a block diagram of part of the transceiver section.

[0025] FIG. 7 is a waveform diagram of transmitted ultrasound based on an output signal from a pulse signal generating unit.

[0026] FIG. 8 is a waveform diagram of transmitted ultrasound based on an output signal from a modulated signal generating unit.

[0027] FIG. 9 illustrates several code sequences of a Barker code.

[0028] FIG. 10 is a block diagram of part of the transceiver section.

[0029] FIG. 11 illustrates pulse compression by a pulse compressing unit.

[0030] FIGS. 12 and 13 are waveform diagrams of transmitted ultrasound based on an output signal from the modulated signal generating unit.

[0031] FIGS. 14-16 illustrates pulse compression by the pulse compressing unit.

[0032] FIG. 17 illustrates linear frequency modulation and corresponding pulse compression.

[0033] FIG. 18 is a schematic diagram showing an example of a screen displayed on a display section.

DETAILED DESCRIPTION OF THE INVENTION

[0034] Several embodiments of the present invention will now be described in detail with reference to the accompanying drawings. It should be noted that the present invention is not limited to the embodiments. FIG. 1 shows a block diagram of an ultrasonic imaging apparatus, which is an embodiment of the present invention. The configuration of the apparatus represents an embodiment of the apparatus in accordance with the present invention. The operation of the apparatus represents an embodiment of the method in accordance with the present invention.

[0035] As shown in FIG. 1, the present apparatus has an ultrasonic probe 2. The ultrasonic probe 2 has an array of ultrasonic transducers (not shown). The individual ultrasonic transducers are made from a piezoelectric material such as PZT (lead zirconate titanate [Pb—Zr—Ti]) ceramic. The ultrasonic probe 2 is used abutted against an object 4 by a user. A region of interest in the object 4 is supplied with a contrast agent 402 using blood flow.

[0036] The ultrasonic probe 2 is connected to a transceiver section 6. The transceiver section 6 supplies driving signals to the ultrasonic probe 2 to transmit ultrasound. The transceiver section 6 also receives echo signals caught by the ultrasonic probe 2.

[0037] FIG. 2 shows a block diagram of the transceiver section 6. As shown, the transceiver section 6 has a transmission signal generating unit 602. The transmission signal generating unit 602 periodically generates a transmission signal, and inputs the signal to a transmission beamformer

604. The transmission signal generating unit **602** is controlled by a control section **18**, which will be described later.

[0038] The transmission beamformer **604** is for performing beamforming for the transmission, involving generating a beamforming signal for forming an ultrasonic beam in a certain direction based on the transmission signal. The beamforming signal consists of a plurality of driving signals that are given respective time differences corresponding to the direction. The beamforming is controlled by the control section **18**, which will be described later. The transmission beamformer **604** inputs the transmission beamforming signal to a transmission/reception switching unit **606**.

[0039] The transmission/reception switching unit **606** inputs the beamforming signal to the ultrasonic transducer array. A plurality of ultrasonic transducers that constitute a transmission aperture in the ultrasonic transducer array generate ultrasound having respective phase differences corresponding to the time differences in the driving signals. By wavefront synthesis of the ultrasound, an ultrasonic beam is formed along an acoustic line in a certain direction.

[0040] The transmission/reception switching unit **606** is connected with a reception beamformer **608**. The transmission/reception switching unit **606** inputs the echo signals caught by a reception aperture in the ultrasonic transducer array to the reception beamformer **608**. The reception beamformer **608** is for performing beamforming for the reception corresponding to an acoustic line for the transmission, involving imparting time differences to a plurality of received echoes to adjust their phases, and then adding the echoes to form an echo received signal along an acoustic line in a certain direction. The reception beamforming is controlled by the control section **18**, which will be described later.

[0041] The transmission of the ultrasonic beam is repeated at predefined time intervals according to the transmission signal generated by the transmission signal generating unit **602**. Synchronously with the signal, the transmission beamformer **604** and the reception beamformer **608** change the direction of the acoustic line by a predefined amount. Thus, the interior of the object **4** is sequentially scanned by the acoustic line. The transceiver section **6** having such a configuration performs scanning as exemplarily shown in FIG. 3. Specifically, a fan-shaped two-dimensional region **206** is scanned in the θ -direction by an acoustic line **202** extending from an emission point **200** in the z -direction, and so-called sector scanning is carried out.

[0042] When the transmission and reception apertures are formed using part of the ultrasonic transducer array, scanning as exemplarily shown in FIG. 4 can be performed by sequentially shifting the apertures along the array. Specifically, a rectangular two-dimensional region **206** is scanned in the x -direction by translating an acoustic line **202**, which emanates from an emission point **200** in the z -direction, along a linear trajectory **204**, and so-called linear scanning is carried out.

[0043] It will be easily recognized that when the ultrasonic transducer array is a so-called convex array, which is formed along an arc protruding in the direction of ultrasound transmission, a partial fan-shaped two-dimensional region **206** can be scanned in the θ -direction by performing acoustic line scanning similar to that of the linear scanning and

moving an emission point **200** of an acoustic line **202** along an arc-like trajectory **204**, as exemplarily shown in FIG. 5, and so-called convex scanning can thus be carried out.

[0044] The reception beamformer **608** is connected with a received signal processing unit **610**. The received signal processing unit **610** performs processing as described later on an output signal, or an echo received signal, from the reception beamformer **608**.

[0045] Under the control of the control section **18**, which will be described later, scanning as described above is performed using two kinds of ultrasound having different sound pressures. One of the two kinds of ultrasound has a sound pressure sufficient to break the contrast agent, and the other has a sound pressure insufficient to break the contrast agent.

[0046] The scanning using the ultrasound having the higher sound pressure is intermittently performed. The interval between scanings, or the pause period, of the intermittent scanning ranges from several seconds to several tens of seconds. The scanning using the ultrasound having the lower sound pressure is continuously performed during the pause period of the intermittent scanning.

[0047] To perform the scanning using the two kinds of ultrasound, the transmission signal generating unit **602** has two signal generating units, as shown in FIG. 6. One of the two signal generating units is a pulse signal generating unit **622**, and the other is a modulated signal generating unit **624**. One of the output signals from these signal generating units is selected by a selecting unit **626** and input to the transmission beamformer **604**. The selecting unit **626** is controlled by the control section **18**, which will be described later.

[0048] The output signal from the pulse signal generating unit **622** is a signal for causing the ultrasonic transducers to generate ultrasound having a sound pressure greater than a contrast agent breaking sound pressure P_c , as exemplarily shown in FIG. 7.

[0049] The output signal from the modulated signal generating unit **624** is a signal for causing the ultrasonic transducers to generate ultrasound having a sound pressure not greater than the contrast agent breaking sound pressure P_c , as exemplarily shown in FIG. 8.

[0050] As shown in FIG. 8, the output signal from the modulated signal generating unit **624** is modulated. Among other modulation schemes, a code modulation scheme, for example, is employed. As a code sequence for the modulation, there is employed, for example, a Barker code or a Golay code, both of which are practically used in pulse compression radar applications.

[0051] In FIG. 8, a case is illustrated in which the signal is modulated using the Barker code having a code length of four and a code sequence of $[+++-]$. The Barker code includes seven code sequences, as shown in FIG. 9. The code modulation may be achieved by any one of these code sequences.

[0052] To process the two kinds of echo received signals corresponding to the two kinds of transmitted ultrasound, the received signal processing unit **610** has a configuration as shown in FIG. 10. Specifically, as shown, an echo received signal is supplied to one of a through signal path

612 and a pulse compressing unit **614** according to selection by a selecting unit **616**. The selecting unit **616** is controlled by the control section **18**, which will be described later.

[0053] The selecting unit **616** is linked with the selecting unit **626**. When the selecting unit **626** selects the pulse generating unit **622**, the selecting unit **616** selects the through signal path **612**; and when the selecting unit **626** selects the modulated signal generating unit **624**, the selecting unit **616** selects the pulse compressing unit **614**.

[0054] Thus, the echo received signal of ultrasound transmitted based on the output signal from the pulse generating unit **622** is input to the signal path **612**; and the echo received signal of ultrasound transmitted based on the output signal from the modulated signal generating unit **624** is input to the pulse compressing unit **614**.

[0055] The pulse compressing unit **614** performs pulse compression processing on the echo received signal. The pulse compression on the echo received signal of the code-modulated ultrasound is achieved by an autocorrelation calculation.

[0056] By performing the autocorrelation calculation on the echo received signal of the ultrasound modulated as described above, a pulse-compressed signal as shown in **FIG. 11** is obtained. As shown, the pulse-compressed signal has a relative amplitude of 0, -1, 0, +1, +4, +1, 0, -1, 0 along a time axis.

[0057] By such pulse compression, a compressed pulse having a relative amplitude of 4 at the signal center can be obtained. In other words, a signal can be obtained that corresponds to an echo of transmitted ultrasound having a sound pressure four times that of the actually transmitted ultrasound.

[0058] Therefore, even if the sound pressure of the transmitted signal is low to the extent of being not greater than the contrast agent breaking sound pressure, an echo received signal having a good SNR can be obtained that is comparable with that in the case of the transmitted ultrasound having a sound pressure greater than the contrast agent breaking sound pressure.

[0059] The case in which the Golay code is employed is as follows: The Golay code has a pair of two code sequences [+++-] and [++-+]. By using the code sequence pair, two series of transmitted ultrasound are obtained as shown in **FIGS. 12 and 13**.

[0060] For an echo of the transmitted ultrasound shown in **FIG. 12**, the autocorrelation calculation is performed using the code sequence [+++-]; and for an echo of the transmitted ultrasound shown in **FIG. 13**, the autocorrelation calculation is performed using the code sequence [++-+].

[0061] Thus, respective compressed pulses are obtained as shown in **FIGS. 14 and 15**. The compressed pulse shown in **FIG. 14** has a relative amplitude of 0, -1, 0, +1, +4, +1, 0, -1, 0; and the compressed pulse shown in **FIG. 15** has a relative amplitude of 0, +1, 0, -1, +4, -1, 0, +1, 0.

[0062] By calculating the sum of such compressed pulses, a compressed pulse can be obtained having a center signal of +8 and all the other signals of 0, as shown in **FIG. 16**. In other words, a pulse that has an even better SNR than by the Barker code can be obtained. Moreover, such a pulse is

advantageous in that it has no side lobe because all the signals other than the center signal become zero.

[0063] When the Golay code is employed, ultrasound transmission/reception is performed twice for every acoustic line. The first ultrasound transmission/reception is performed using one of the pair of the code sequences, and the second ultrasound transmission/reception is performed using the other. Then, the sum of the first pulse-compressed echo received signal and the second pulse-compressed echo received signal is calculated, and the sum is defined as the echo received signal for one acoustic line. Such transmission/reception is performed while sequentially changing the acoustic line direction.

[0064] In lieu of the code modulation, linear frequency modulation may be employed. **FIG. 17** shows the concept of the linear frequency modulation and corresponding pulse compression. As shown in **FIG. 17(a)**, a frequency modulated signal (b) having a frequency that linearly changes by Δf in a time period T is generated by the modulated signal generating unit **624**, and ultrasound based on the signal (b) is transmitted. Naturally, the sound pressure of the transmitted ultrasound should not be greater than the contrast agent breaking sound pressure P_c .

[0065] By performing the pulse compression on an echo received signal of such ultrasound by the pulse compressing unit **614** having a frequency-delay time characteristic such that the delay time varies from T to 0 in the frequency range Δf , as shown in **FIG. 17(c)**, a compressed pulse having an increased relative amplitude at the signal center can be obtained, as shown in **FIG. 17(d)**.

[0066] A portion consisting of the pulse signal generating unit **622**, selecting unit **626**, transmission beamformer **604**, transmission/reception switching unit **606**, ultrasonic probe **2** and reception beamformer **608** is an embodiment of the first ultrasound transmitting/receiving means of the present invention.

[0067] A portion consisting of the modulated signal generating unit **624**, selecting unit **626**, transmission beamformer **604**, transmission/reception switching unit **606**, ultrasonic probe **2** and reception beamformer **608** is an embodiment of the second ultrasound transmitting/receiving means of the present invention. The pulse compressing unit **614** is an embodiment of the pulse compressing means of the present invention. The control section **18**, which will be described later, is an embodiment of the control means of the present invention.

[0068] The transceiver section **6** as described above is connected to a B-mode processing section **10** and a Doppler processing section **12**, as shown in **FIG. 1**. The echo received signal for each acoustic line output from the transceiver section **6** is input to the B-mode processing section **10** and the Doppler processing section **12**.

[0069] The B-mode processing section **10** is for generating B-mode image data. The B-mode processing section **10** logarithmically amplifies the echo received signal and then detects its envelope to obtain a signal indicating the intensity of the echo at each reflection point on an acoustic line, i.e., an A-scope signal; and generates B-mode image data using the amplitude of the A-scope signal at each instant as the brightness. Image data for the aforementioned two kinds of transmitted ultrasound are individually generated as the B-mode image data.

[0070] The Doppler processing section 12 is for generating Doppler image data. Image data for the aforementioned two kinds of transmitted ultrasound are individually generated as the Doppler image data. The Doppler processing section 12 quadrature-detects the echo received signal and then MTI(moving target indication)-processes the signal to obtain the Doppler shift in the echo signal; and calculates the average flow velocity, variance of the flow velocity, power of the Doppler signal, etc. from an autocorrelation calculation on the Doppler shift. The average flow velocity will sometimes be referred to simply as the flow velocity hereinbelow. Moreover, the variance of the flow velocity will sometimes be referred to simply as the variance, and the power of the Doppler signal simply as the power hereinbelow.

[0071] The Doppler processing section 12 provides data representing the flow velocity, variance and power of an echo source moving inside the object 4 for each acoustic line. The data represents the flow velocity, variance and power at each point (pixel) on an acoustic line. The flow velocity is obtained as a component in an acoustic line direction, and a direction approaching the ultrasonic probe 2 and a direction going away from the ultrasonic probe 2 are distinguished.

[0072] The B-mode processing section 10 and the Doppler processing section 12 are connected to an image processing section 14. The image processing section 14 produces a B-mode image and a color Doppler image based on respective data supplied from the B-mode processing section 10 and the Doppler processing section 12. The B-mode image and the color Doppler image are generated for each of the two kinds of transmitted ultrasound.

[0073] The image processing section 14 is connected with a display section 16, which displays the B-mode and color Doppler images produced by the image processing section 14. A portion consisting of the B-mode processing section 10, Doppler processing section 12, image processing section 14 and display section 16 is an embodiment of the image producing means of the present invention.

[0074] The transceiver section 6, B-mode processing section 10, Doppler processing section 12, image processing section 14 and display section 16 are connected with the control section 18. The control section 18 supplies control signals to these sections for controlling their operation. The control section 18 is supplied with several kinds of notification signals from the controlled sections. The B-mode operation and the Doppler mode operation are executed under the control of the control section 18.

[0075] The control section 18 is connected with an operating section 20. The operating section 20 is operated by the user, and the section 20 inputs appropriate instructions and information to the control section 18. The operating section 20 comprises, for example, a keyboard, pointing device and other operating devices.

[0076] Now the operation of the present apparatus will be described. The user abuts the ultrasonic probe 2 against a desired portion on the object 4, and operates the operating section 20 for performing, for example, B-mode imaging. The imaging is performed under the control of the control section 18.

[0077] The transceiver section 6 performs scanning as shown in FIGS. 3-5 on the interior of the object 4 in an

acoustic-line-sequential manner using the ultrasonic probe 2. Of the aforementioned two kinds of transmitted ultrasound, scanning by the ultrasound having a sound pressure greater than the contrast agent breaking sound pressure is intermittently performed with a pause period of from several seconds to several tens of seconds, and scanning by the ultrasound having a sound pressure not greater than the contrast agent breaking sound pressure is continuously performed during the pause period of the intermittent scanning.

[0078] Thus, two B-mode images are captured. One of the two B-mode images will be sometimes referred to as a high sound pressure image and the other as a low sound pressure image hereinbelow. These images are displayed next to each other on the screen of the display section 16, as exemplarily shown in FIG. 18.

[0079] The high sound pressure image 162 is a contrast image. This image is displayed as a freeze image, and is updated every time a new image is obtained by the intermittent scanning. The low sound pressure image 164 is displayed as a real-time image because it is obtained by the continuous scanning. This image shows the state in real time from the time the contrast agent is broken and to the time it again infuses the site being imaged. Since the image is produced based on the pulse-compressed echo received signal having a high SNR, the image quality is high even if the transmitted ultrasound has a low sound pressure.

[0080] While the present invention has been described with reference to preferred embodiments hereinabove, various changes or substitutions may be made on these embodiments by those ordinarily skilled in the art pertinent to the present invention without departing from the technical scope of the present invention. Therefore, the technical scope of the present invention encompasses not only those embodiments described above but all the embodiments that fall within the scope of the appended claims.

[0081] Many widely different embodiments of the invention may be configured without departing from the spirit and the scope of the present invention. It should be understood that the present invention is not limited to the specific embodiments described in the specification, except as defined in the appended claims.

1. An ultrasonic transmission/reception method, comprising the steps of: intermittently scanning an imaged region with a predetermined pause period using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; continuously scanning the same region as said imaged region during said pause period using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; and performing pulse compression on an echo received signal obtained by said continuous scanning.

2. The ultrasonic transmission/reception method as defined by claim 1, wherein said modulation is code modulation.

3. The ultrasonic transmission/reception method as defined by claim 2, wherein a code sequence for said code modulation is a Barker code.

4. The ultrasonic transmission/reception method as defined by claim 2, wherein a code sequence for said code modulation is a Golay code.

5. The ultrasonic transmission/reception method as defined by claim 1, wherein said modulation is linear frequency modulation.

6. An ultrasonic transmission/reception apparatus, comprising: first ultrasound transmitting/receiving means for scanning an imaged region using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; second ultrasound transmitting/receiving means for scanning the same region as said imaged region using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; pulse compressing means for performing pulse compression on an echo received signal from said second ultrasound transmitting/receiving means; and control means for causing said first ultrasound transmitting/receiving means to intermittently perform the scanning with a predetermined pause period, and causing said second ultrasound transmitting/receiving means to continuously perform the scanning during said pause period.

7. The ultrasonic transmission/reception apparatus as defined by claim 6, wherein said modulation is code modulation.

8. The ultrasonic transmission/reception apparatus as defined by claim 7, wherein a code sequence for said code modulation is a Barker code.

9. The ultrasonic transmission/reception apparatus as defined by claim 7, wherein a code sequence for said code modulation is a Golay code.

10. The ultrasonic transmission/reception apparatus as defined by claim 6, wherein said modulation is linear frequency modulation.

11. An ultrasonic imaging method, comprising the steps of: intermittently scanning an imaged region with a predetermined pause period using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; continuously scanning the same region as said imaged region during said pause period using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; performing pulse compression on an echo received signal obtained by said continuous scanning; and producing respective images based on an echo received signal obtained by said intermittent scanning and on an echo received signal after said pulse compression.

12. The ultrasonic imaging method as defined by claim 11, wherein said modulation is code modulation.

13. The ultrasonic imaging method as defined by claim 12, wherein a code sequence for said code modulation is a Barker code.

14. The ultrasonic imaging method as defined by claim 12, wherein a code sequence for said code modulation is a Golay code.

15. The ultrasonic imaging method as defined by claim 11, wherein said modulation is linear frequency modulation.

16. An ultrasonic imaging apparatus, comprising: first ultrasound transmitting/receiving means for scanning an imaged region using ultrasound that has a sound pressure sufficient to break a contrast agent, and receiving an echo of the ultrasound; second ultrasound transmitting/receiving means for scanning the same region as said imaged region using ultrasound that has a sound pressure insufficient to break the contrast agent and has undergone predetermined modulation, and receiving an echo of the ultrasound; pulse compressing means for performing pulse compression on an echo received signal from said second ultrasound transmitting/receiving means; control means for causing said first ultrasound transmitting/receiving means to intermittently perform the scanning with a predetermined pause period, and causing said second ultrasound transmitting/receiving means to continuously perform the scanning during said pause period; and image producing means for producing respective images based on an echo received signal from said first ultrasound transmitting/receiving means and on an echo received signal after said pulse compression from said second ultrasound transmitting/receiving means.

17. The ultrasonic imaging apparatus as defined by claim 16, wherein said modulation is code modulation.

18. The ultrasonic imaging apparatus as defined by claim 17, wherein a code sequence for said code modulation is a Barker code.

19. The ultrasonic imaging apparatus as defined by claim 17, wherein a code sequence for said code modulation is a Golay code.

20. The ultrasonic imaging apparatus as defined by claim 16, wherein said modulation is linear frequency modulation.

* * * * *

专利名称(译)	超声波发送/接收方法，超声波发送/接收装置，超声波成像方法和超声波成像装置		
公开(公告)号	US20020151798A1	公开(公告)日	2002-10-17
申请号	US10/119252	申请日	2002-04-09
[标]申请(专利权)人(译)	HONDA MASAYOSHI		
申请(专利权)人(译)	HONDA MASAYOSHI		
当前申请(专利权)人(译)	HONDA MASAYOSHI		
[标]发明人	HONDA MASAYOSHI		
发明人	HONDA, MASAYOSHI		
IPC分类号	G01N29/04 A61B8/00 A61B8/14		
CPC分类号	G01N2291/044 A61B8/481		
优先权	2001112466 2001-04-11 JP		
其他公开文献	US6958042		
外部链接	Espacenet USPTO		

摘要(译)

为了使用具有不破坏造影剂的低声压的超声波来捕获高质量的超声波图像，在间歇扫描的暂停期间执行扫描，使用具有不足以破坏造影剂的声压的超声波和经过了预定的调制;对回波接收信号进行脉冲压缩;并且基于脉冲压缩的回波接收信号产生图像。

