



US 20170215838A1

(19) **United States**(12) **Patent Application Publication**
PARK et al.(10) **Pub. No.: US 2017/0215838 A1**(43) **Pub. Date: Aug. 3, 2017**(54) **METHOD AND APPARATUS FOR
DISPLAYING ULTRASOUND IMAGE****Publication Classification**(71) Applicant: **SAMSUNG MEDISON CO., LTD.**,
Hongcheon-gun (KR)(72) Inventors: **Jin-ki PARK**, Hongcheon-gun (KR);
Sung-wook PARK, Hongcheon-gun
(KR); **Jin-yong LEE**, Hongcheon-gun
(KR)(73) Assignee: **SAMSUNG MEDISON CO., LTD.**,
Hongcheon-gun (KR)(21) Appl. No.: **15/258,421**(22) Filed: **Sep. 7, 2016**(30) **Foreign Application Priority Data**

Feb. 1, 2016 (KR) 10-2016-0012456

(51) **Int. Cl.****A61B 8/08** (2006.01)**A61B 8/00** (2006.01)(52) **U.S. Cl.**CPC **A61B 8/0891** (2013.01); **A61B 8/463**(2013.01); **A61B 8/466** (2013.01); **A61B 8/483**(2013.01); **A61B 8/5246** (2013.01)

(57)

ABSTRACT

Provided are methods and apparatuses for displaying ultrasound images. Methods and apparatuses for displaying ultrasound images according to one or more embodiments may determine a stenosis cross-section from ultrasound data with respect to an object including a blood vessel and display at least two cross-sections related to stenosis of the blood vessel and a stenosis index value representing a degree of stenosis of the blood vessel, thereby improving diagnostic usability for a user.

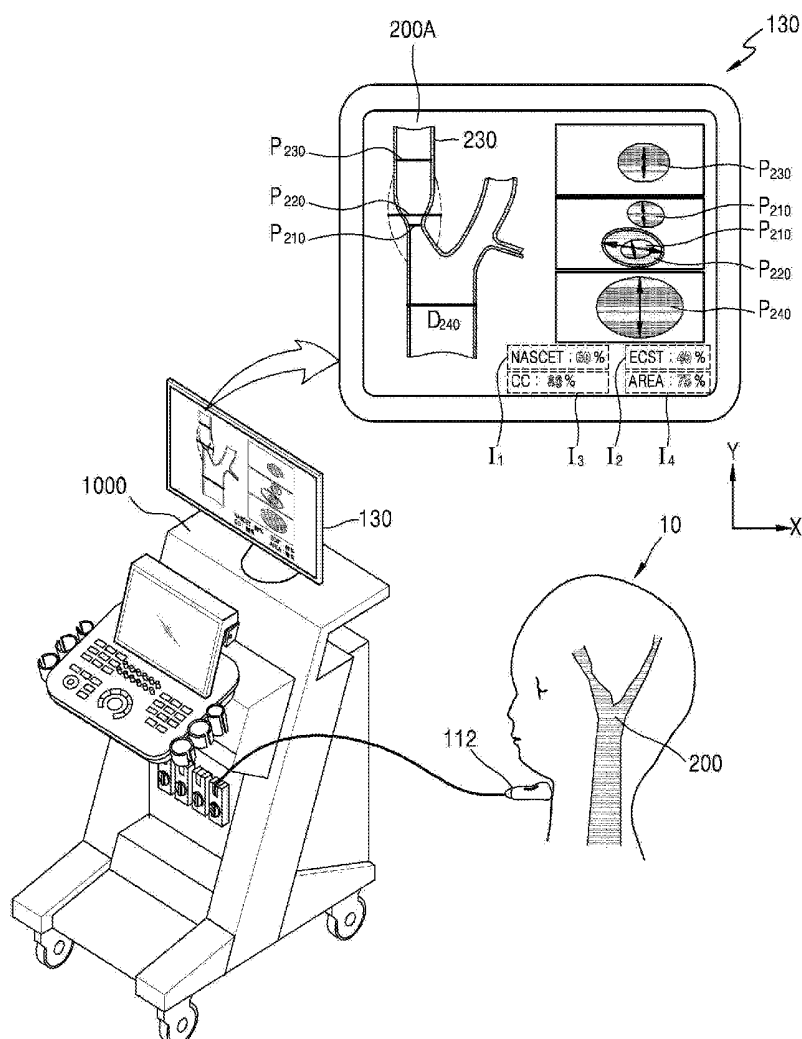


FIG. 1

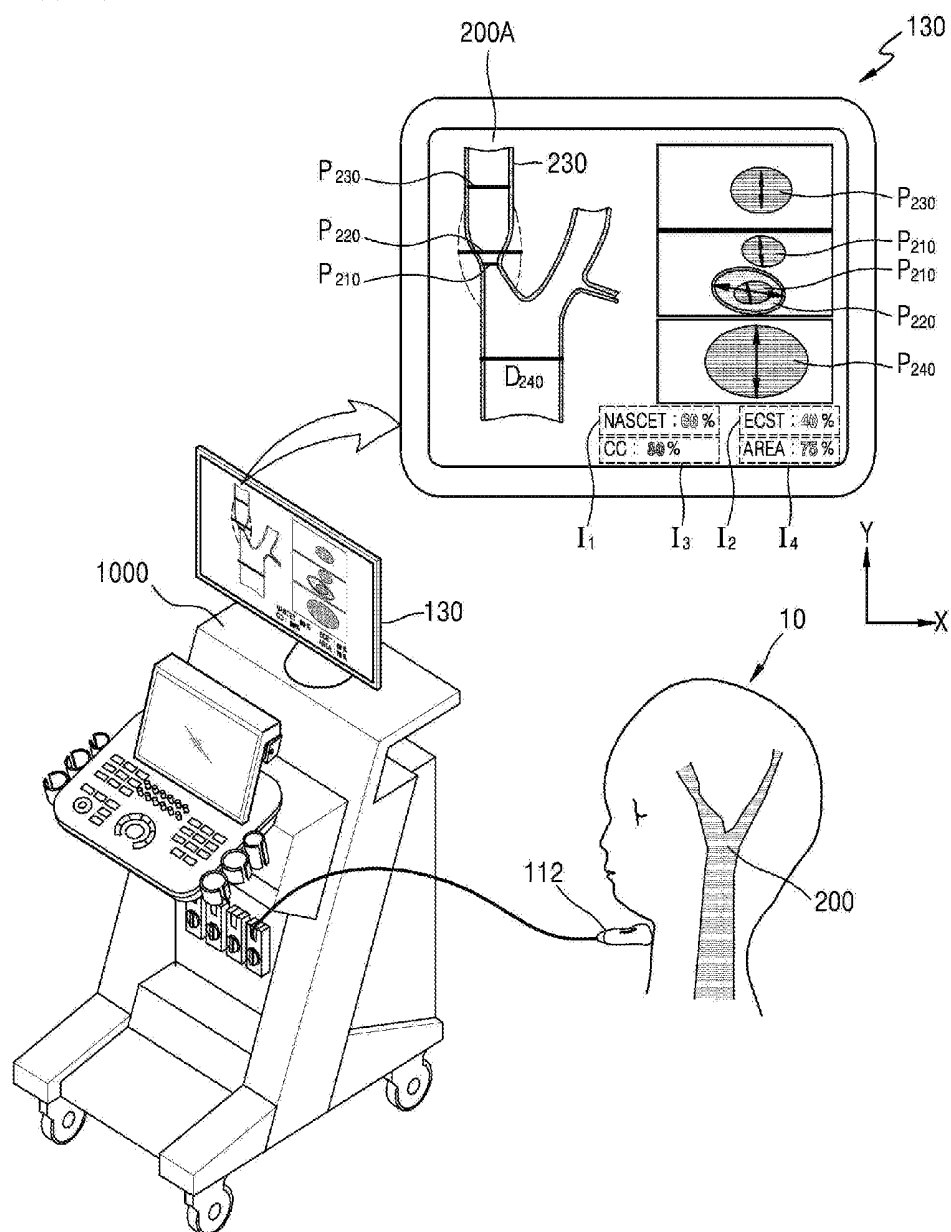


FIG. 2

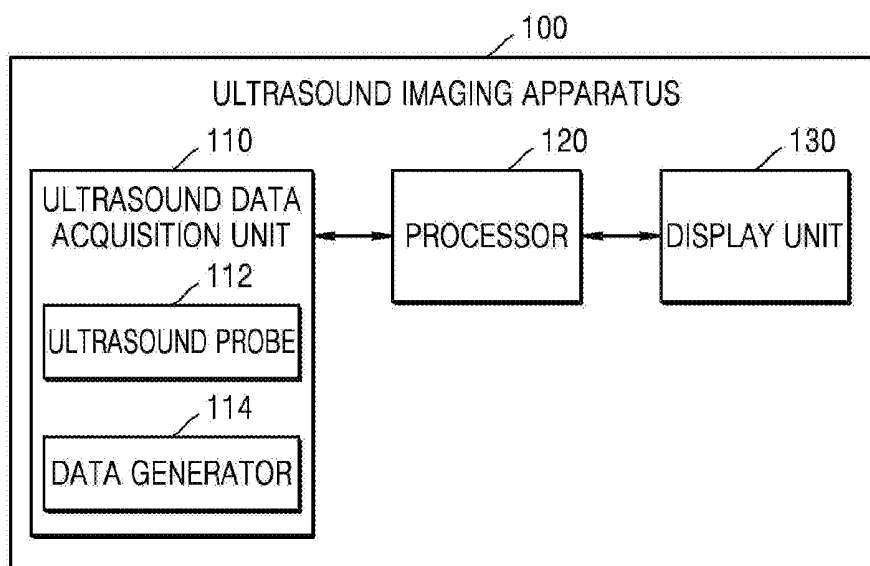


FIG. 3

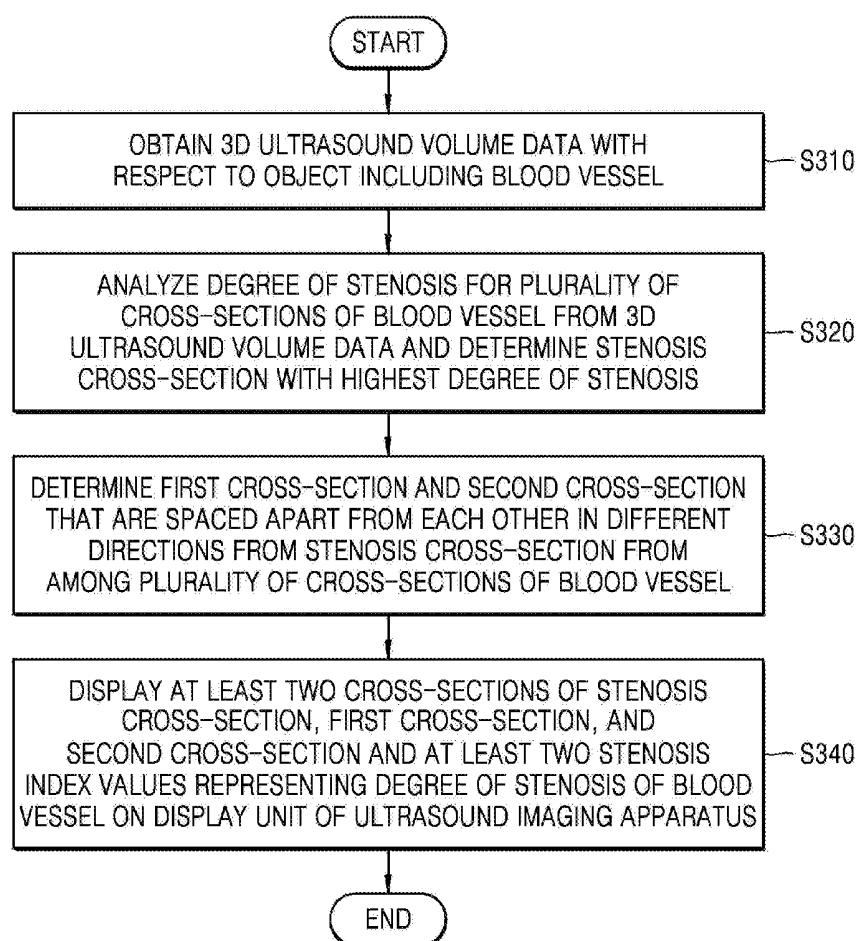


FIG. 4A

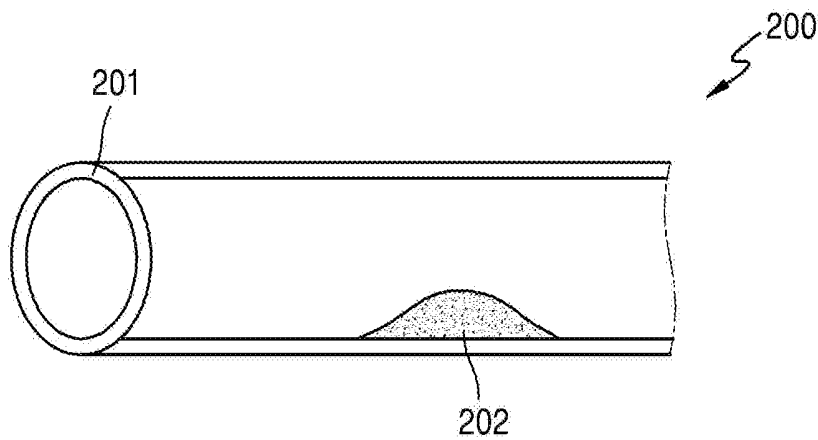


FIG. 4B

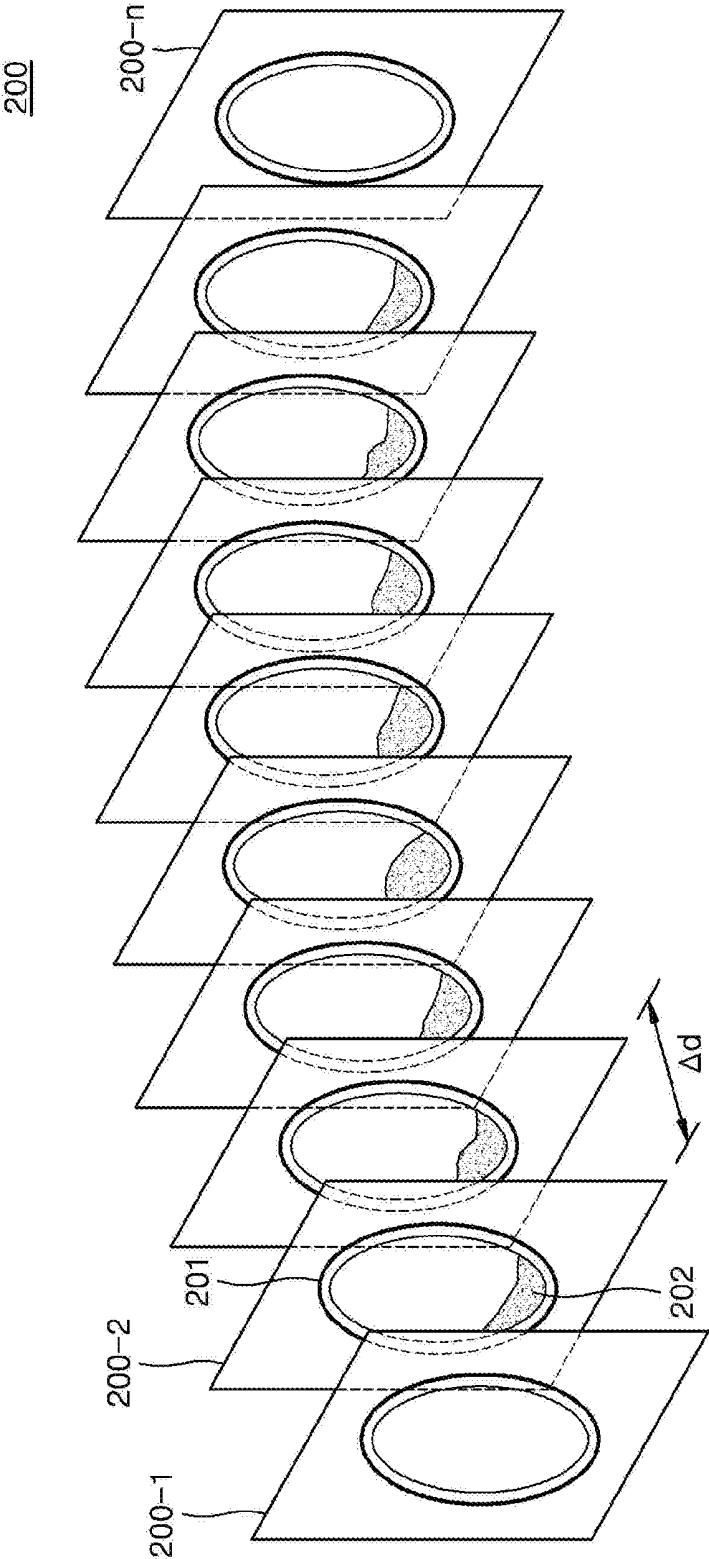


FIG. 4C

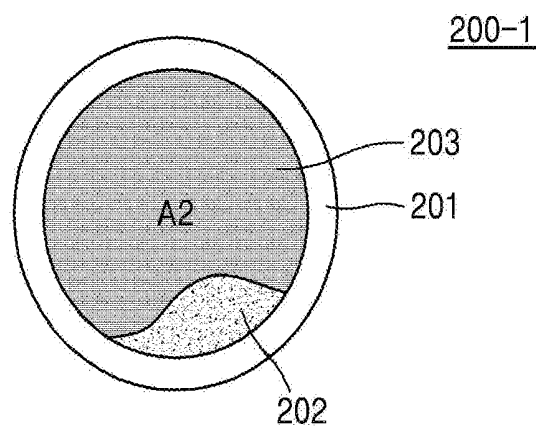


FIG. 5

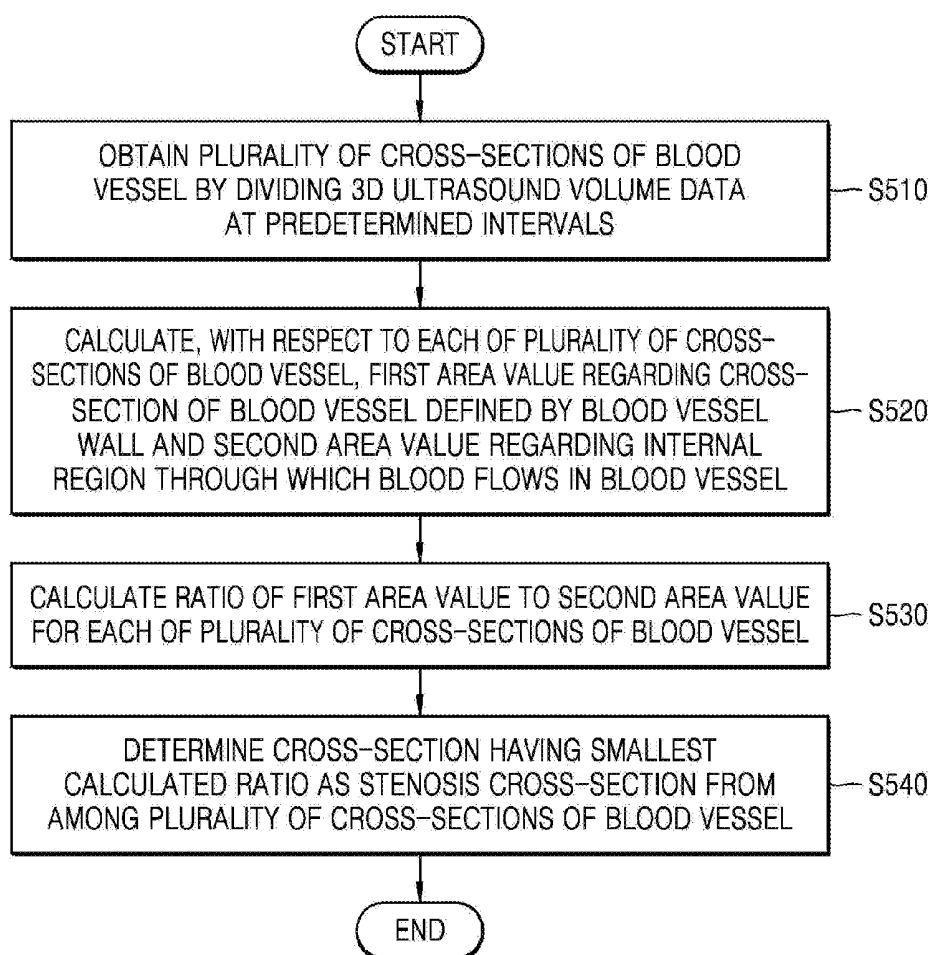


FIG. 6

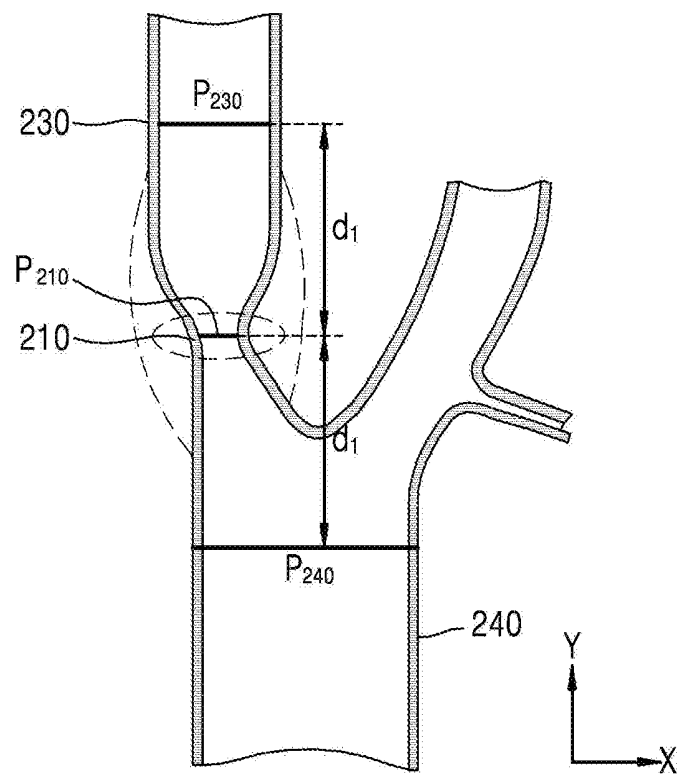


FIG. 7

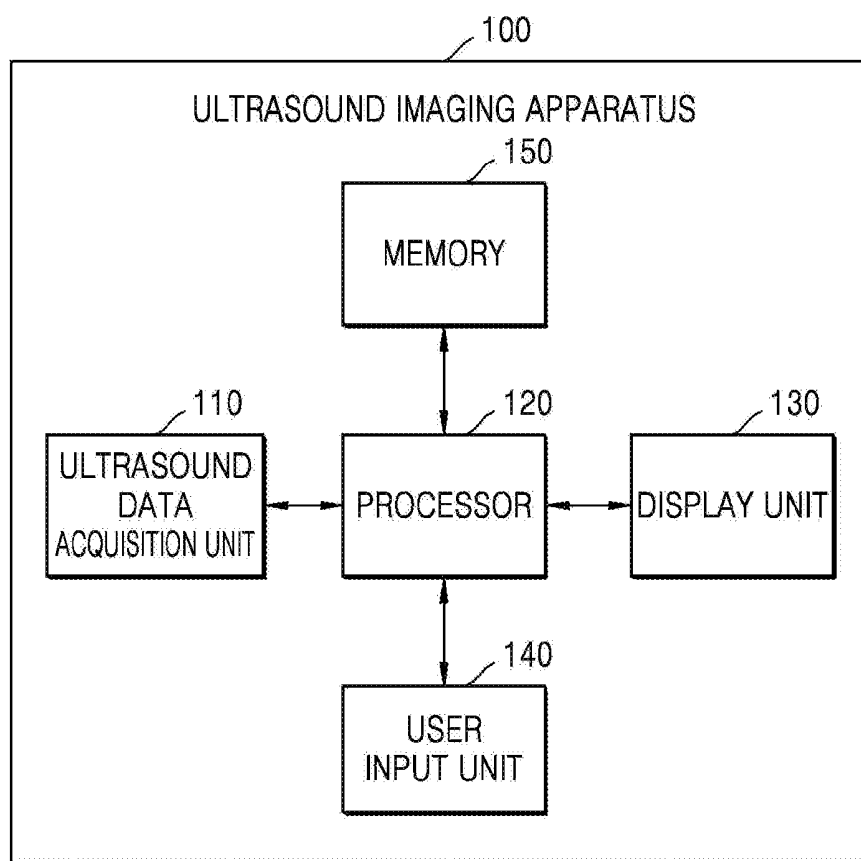


FIG. 8

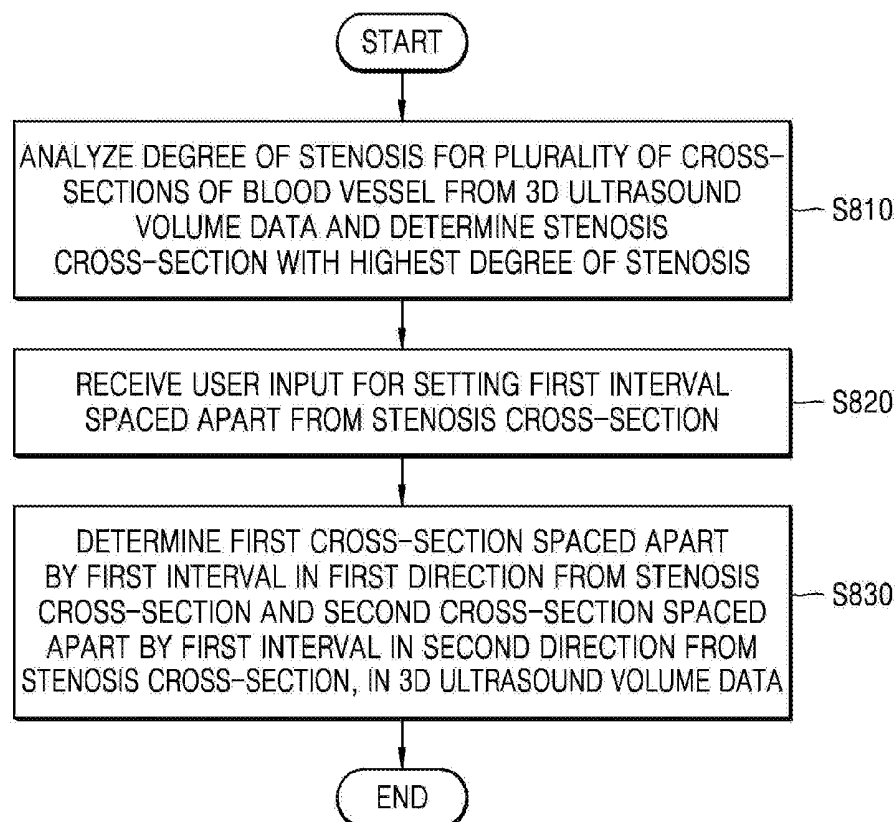


FIG. 9

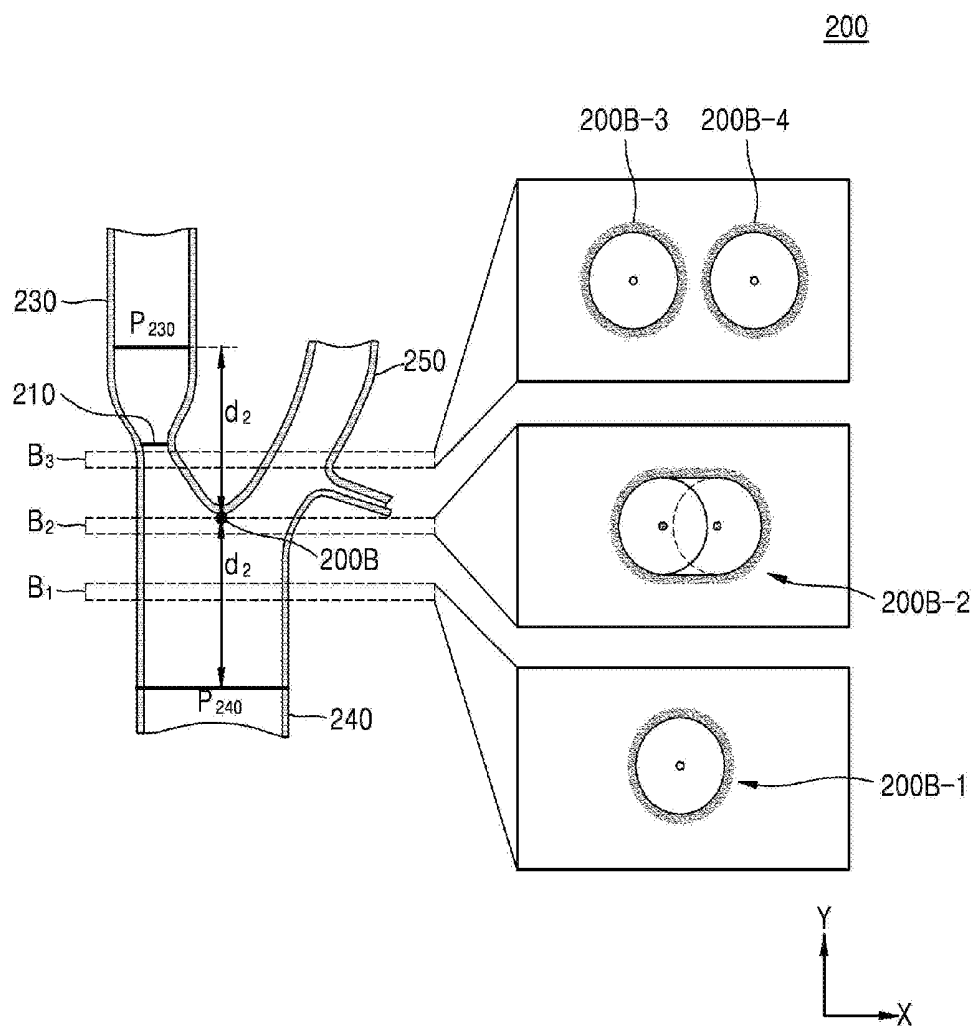


FIG. 10

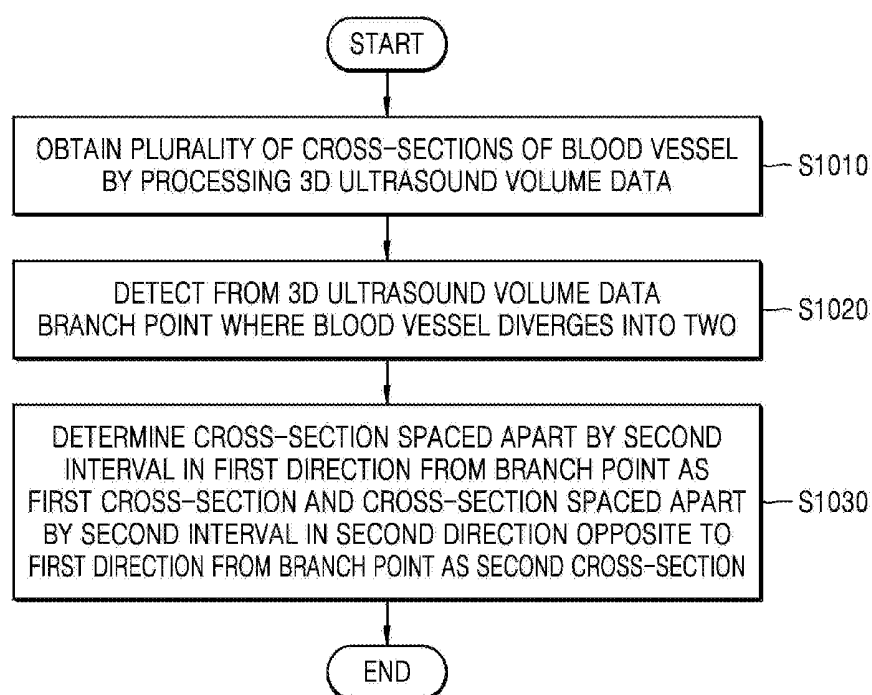


FIG. 11A

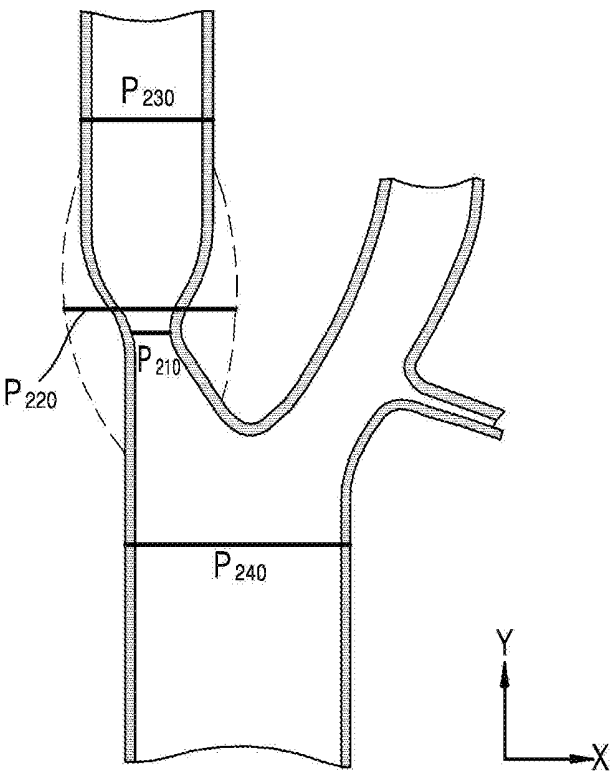


FIG. 11B

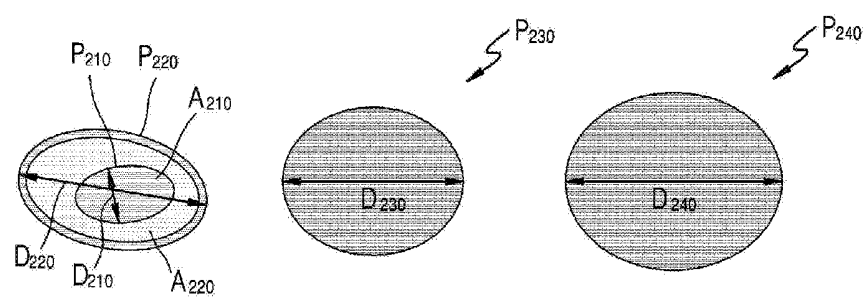


FIG. 12A

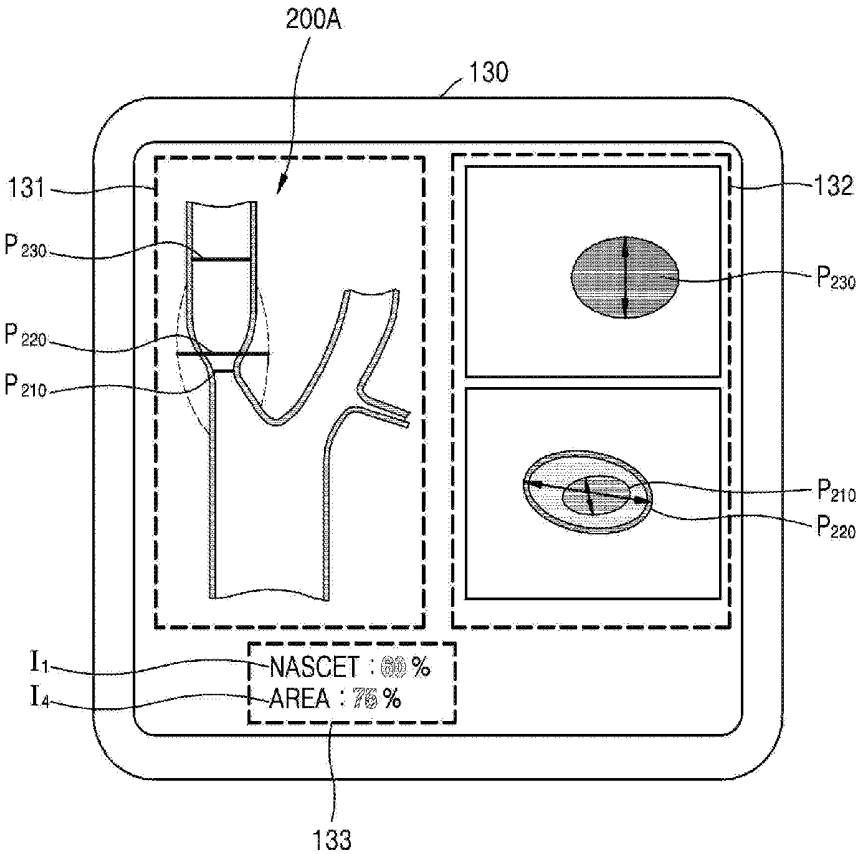


FIG. 12B

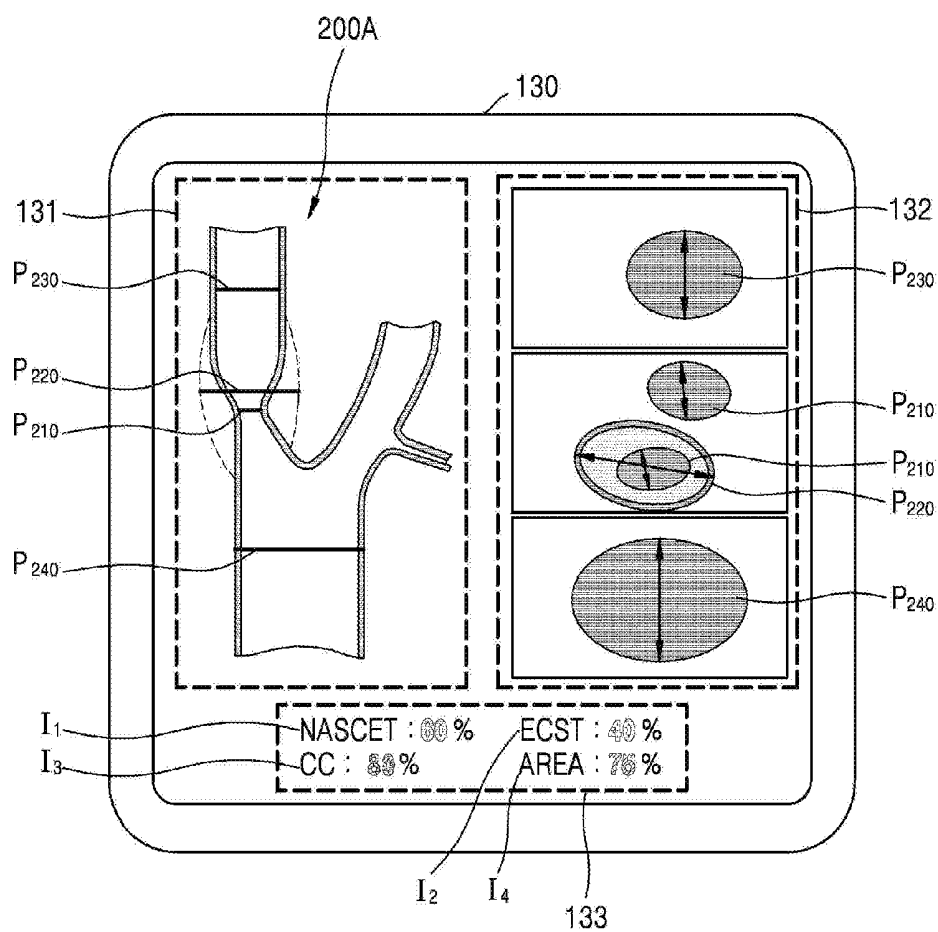


FIG. 12C

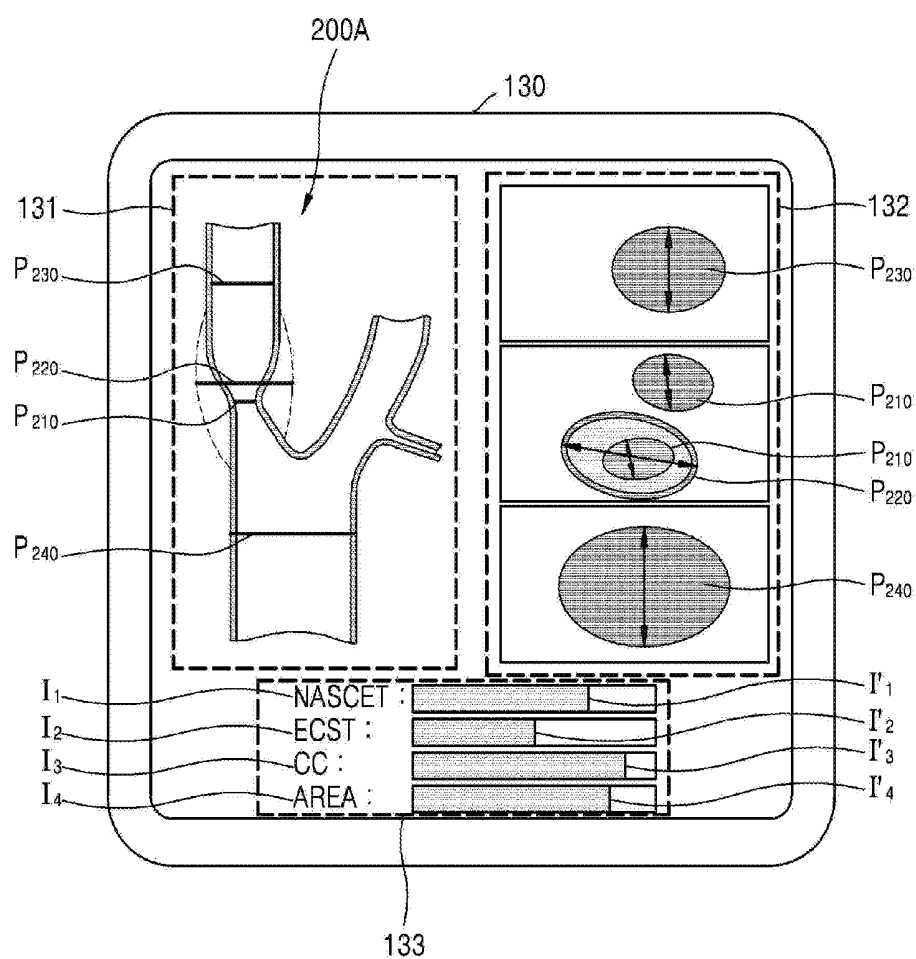


FIG. 12D

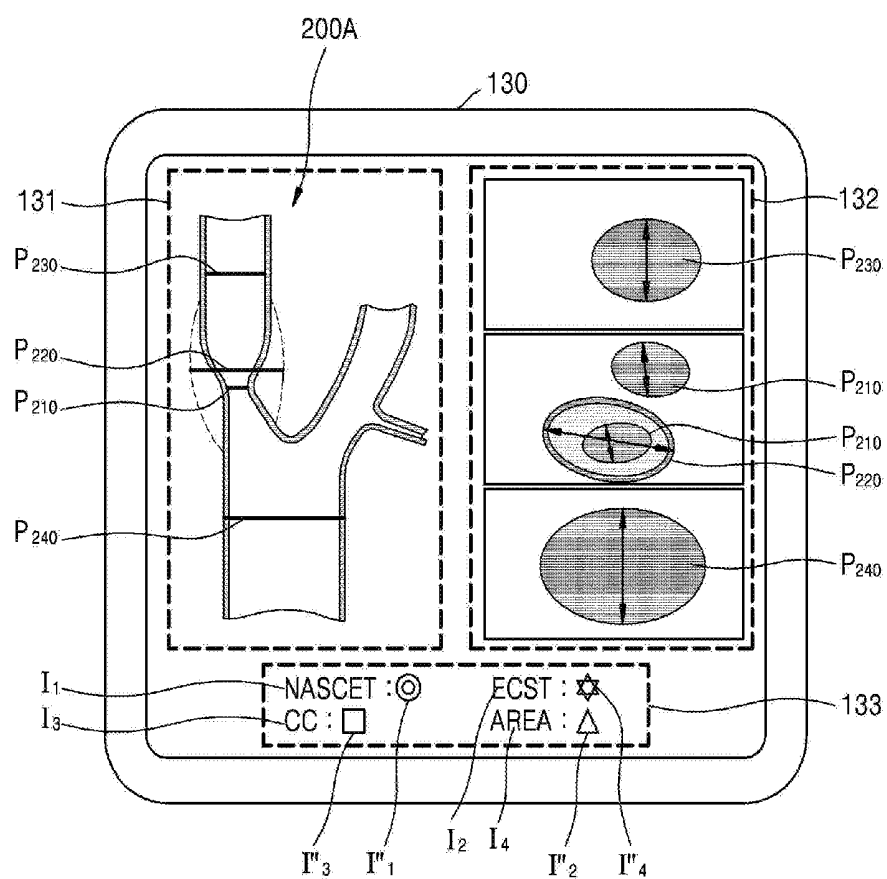


FIG. 13


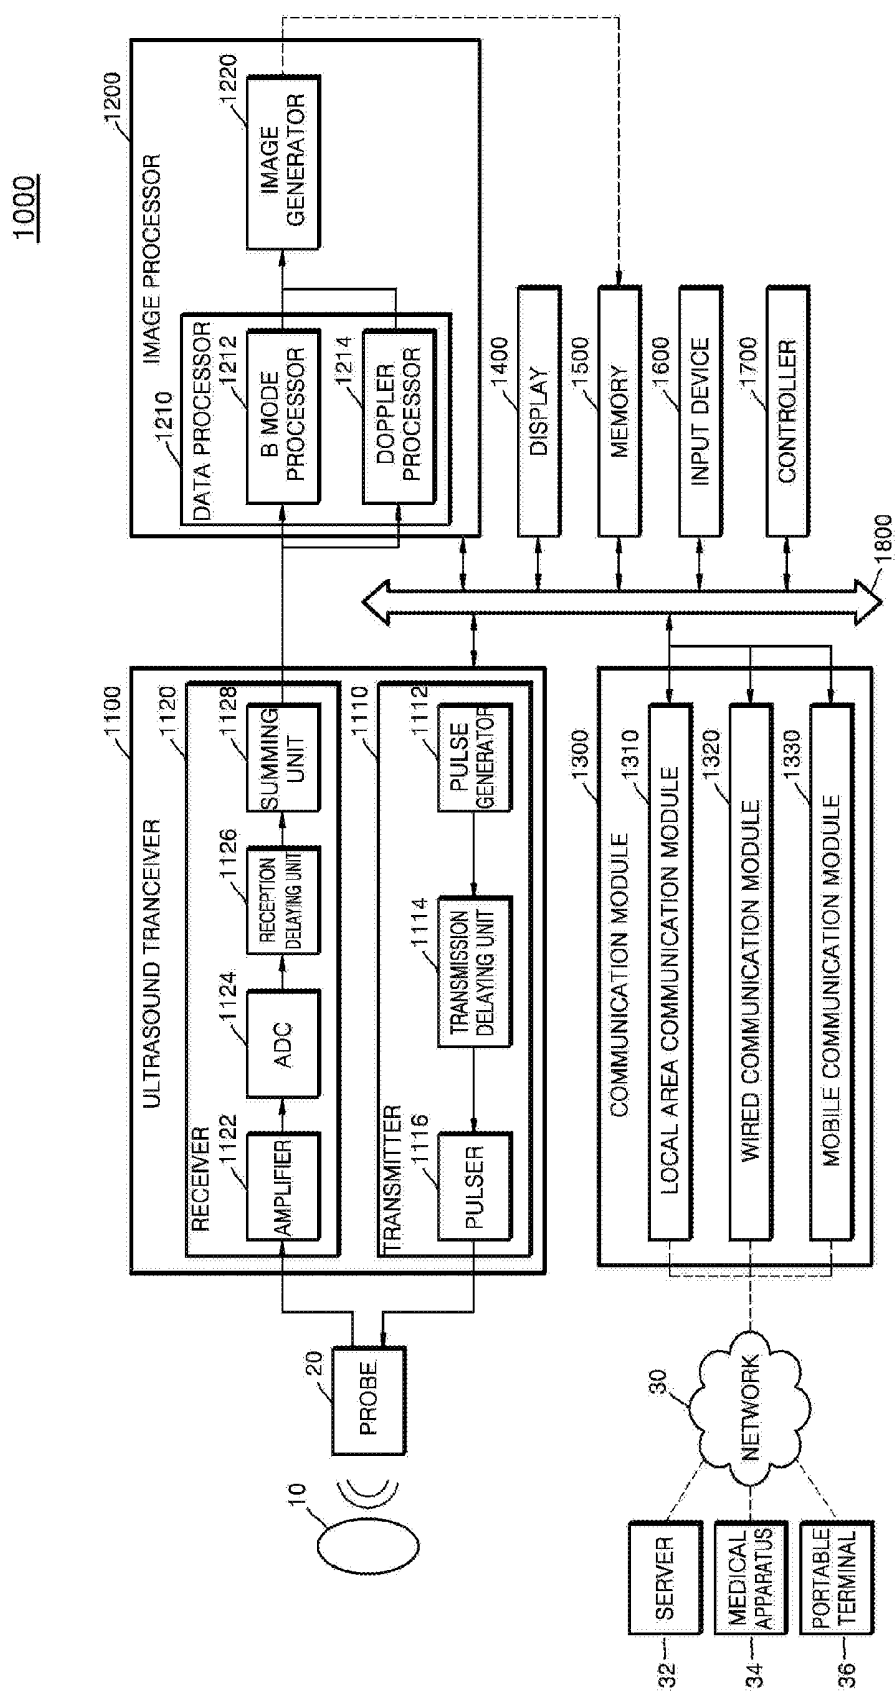


FIG. 14

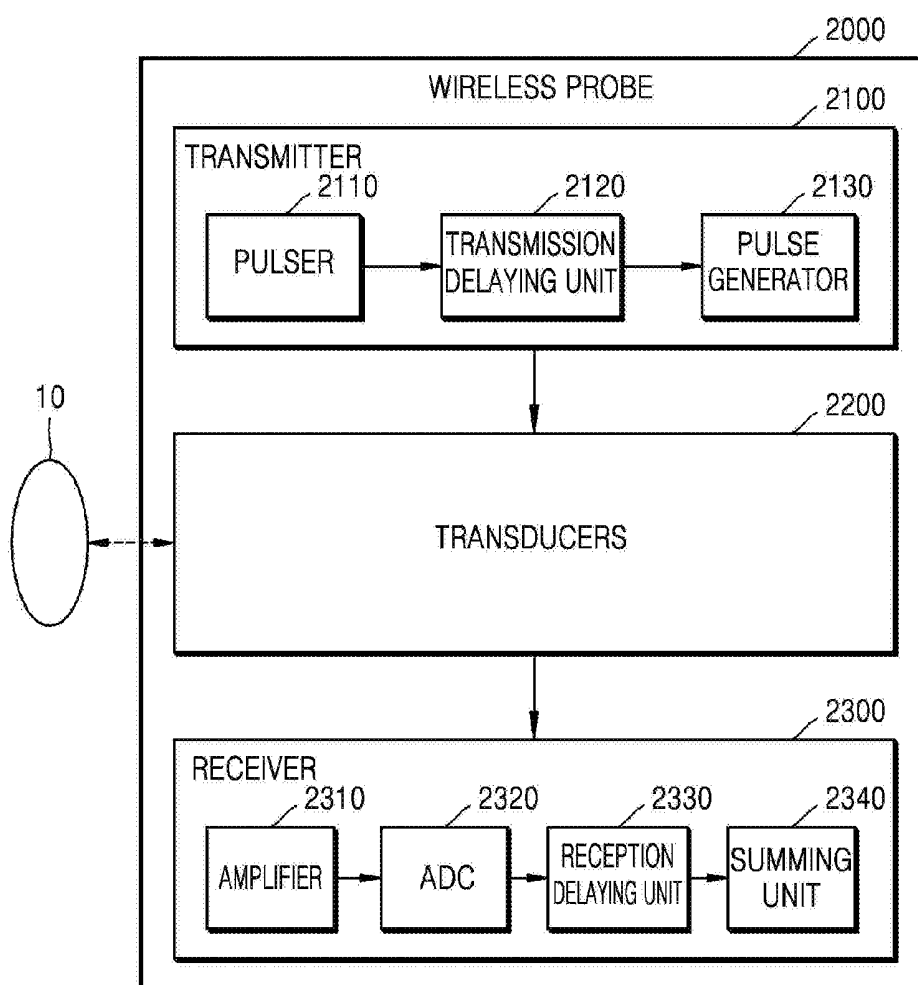

METHOD AND APPARATUS FOR DISPLAYING ULTRASOUND IMAGE

CROSS-REFERENCE TO RELATED APPLICATION

[0001] This application claims the benefit of Korean Patent Application No. 10-2016-0012456, filed on Feb. 1, 2016, in the Korean Intellectual Property Office, the disclosure of which is incorporated herein in its entirety by reference.

BACKGROUND

[0002] 1. Field

[0003] The present disclosure relates to methods and apparatuses for displaying ultrasound images, and more particularly, to methods and apparatuses for determining a plurality of blood vessel cross-sections related to measurement of a degree of stenosis of the blood vessel from three dimensional (3D) ultrasound volume data and displaying a stenosis index value representing a degree of stenosis of a plurality of blood vessel cross-sections of and of the blood vessel.

[0004] 2. Description of the Related Art

[0005] Due to its non-invasive and non-destructive nature, an ultrasound system has become widely used in many medical fields that require information about the inside of an object. The ultrasound system also plays a critical role in medical diagnosis since it can provide high-resolution images of an inner area of an object to a medical practitioner without the need for performing a surgical procedure to directly incise the object for observation.

[0006] In order to measure a degree of stenosis of a blood vessel by using an ultrasound system, an ultrasound probe may be moved over a portion of a patient's body including the blood vessel to find plural cross-sections of the blood vessel, followed by measurement of a diameter or an area of a blood vessel cross-section. As an index for measuring a degree of stenosis by using a diameter of a blood vessel cross-section, North American Symptomatic Carotid Endarterectomy Trial (NASCET), European Carotid Surgery Trial (ECST), or a common carotid method (CC) may be used.

SUMMARY

[0007] Provided are methods and apparatuses for displaying ultrasound images of a plurality of blood vessel cross-sections, which are related to measurement of a degree of stenosis of the blood vessel and are obtained from 3D ultrasound volume data, and a stenosis index value calculated from the plurality of cross-sections of the blood vessel, enabling a user to easily recognize the degree of stenosis of the blood vessel, thereby improving diagnostic usability for a user.

[0008] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0009] According to an aspect of an embodiment, a method, performed by an ultrasound imaging apparatus, of displaying an ultrasound image with respect to an object including a blood vessel, includes obtaining three-dimensional (3D) ultrasound volume data with respect to the object; analyzing a degree of stenosis for a plurality of cross-sections of the blood vessel from the 3D ultrasound volume data and determining a stenosis cross-section with a highest degree of stenosis; determining a first cross-section

and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among the plurality of cross-sections of the blood vessel; and displaying at least two cross-sections of the stenosis cross-section, the first cross-section, the second cross-section, and at least two stenosis index values showing a degree of stenosis of the blood vessel on a display unit of the ultrasound imaging apparatus.

[0010] The displaying of at least two stenosis index values may include displaying at least two index values from among a first index value representing a ratio of a diameter of the first cross-section to a difference between the diameter of the first cross-section and a diameter of the stenosis cross-section, a second index value representing a ratio of an entire blood vessel diameter defined by a blood vessel wall of the stenosis cross-section to a difference between the entire blood vessel diameter and the diameter of the stenosis cross-section, a third index value representing a ratio of a diameter of the second cross-section to a difference between the diameter of the second cross-section and the diameter of the stenosis cross-section, and a fourth index value representing a ratio of a cross-sectional area of the entire blood vessel of the stenosis cross-section to an area of the stenosis cross-section.

[0011] The blood vessel may be a carotid artery, the first cross-section may be a cross-section of an internal carotid artery (ICA), and the second cross-section may be a cross-section of a common carotid artery (CCA).

[0012] The ultrasound imaging method may further include rendering the 3D ultrasound volume data to generate a 3D ultrasound image of the object, wherein the displaying of the at least two cross-sections and the at least two stenosis index values may include displaying the at least two cross-sections, the at least two stenosis index values, and the 3D ultrasound image on the display unit.

[0013] The displaying of the at least two cross-sections and the at least two stenosis index values may include displaying a user interface that displays at least one of different colors, graphs, and figures based on sizes of the at least two stenosis index values, along with the at least two stenosis index values.

[0014] The obtaining of the 3D ultrasound volume data with respect to the object may include transmitting ultrasound signals to the object; receiving ultrasound echo signals reflected by the object; and obtaining the 3D ultrasound volume data from the received ultrasound echo signals.

[0015] The determining of the stenosis cross-section may include obtaining the plurality of cross-sections of the blood vessel by segmenting the 3D ultrasound volume data at predetermined intervals; calculating, with respect to each of the plurality of cross-sections of the blood vessel, a first area value regarding a cross-section defined by a blood vessel wall of the blood vessel and a second area value regarding a cross-section through which blood flows in the blood vessel; calculating, with respect to each of the plurality of cross-sections of the blood vessel, a ratio of the first area value to the second area value; and determining a cross-section having a smallest calculated ratio as a stenosis cross-section from among the plurality of cross-sections of the blood vessel.

[0016] The calculating of the second area value may include obtaining a brightness value for each of the plurality of cross-sections of the blood vessel; determining an area of a region whose obtained brightness value may be less than

a predetermined brightness value as a second area; and calculating an area value of the second area.

[0017] The first cross-section may be spaced apart by a predetermined first interval in a first direction from the stenosis cross-section and the second cross-section may be spaced apart by the first interval in a second direction that may be opposite to the first direction from the stenosis cross-section.

[0018] The determining of the first cross-section and the second cross-section may include receiving a user input for setting a second interval that may be spaced apart from the stenosis cross-section, wherein the first cross-section may be spaced apart by the second interval in a first direction from the stenosis cross-section and the second cross-section may be spaced apart by the second interval in a second direction that may be opposite to the first direction from the stenosis cross-section.

[0019] The determining of the first cross-section and the second cross-section may include detecting from the 3D ultrasound volume data a branch point where the blood vessel diverges into two; and determining a cross-section spaced apart by a third interval in a first direction from the branch point as the first cross-section and determining a cross-section spaced apart by the third interval in a second direction that may be opposite to the first direction from the branch point as the second cross-section.

[0020] According to another aspect of an embodiment, an ultrasound imaging apparatus displaying an ultrasound image with respect to an object including a blood vessel includes an ultrasound data acquisition unit configured to obtain 3D ultrasound volume data with respect to the object; a processor configured to analyze a degree of stenosis for a plurality of cross-sections of the blood vessel from the 3D ultrasound volume data, determine a stenosis cross-section with a highest degree of stenosis and determine a first cross-section and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among the plurality of cross-sections of the blood vessel; and a display unit configured to display at least two cross-sections of the stenosis cross-section, the first cross-section, the second cross-section, and at least two stenosis index values showing a degree of stenosis of the blood vessel.

[0021] The processor may further be configured to calculate at least two index values from among a first index value representing a ratio of a diameter of the first cross-section to a difference between the diameter of the first cross-section and a diameter of the stenosis cross-section, a second index value representing a ratio of an entire blood vessel diameter defined by a blood vessel wall of the stenosis cross-section to a difference between the entire blood vessel diameter and the diameter of the stenosis cross-section, a third index value representing a ratio of a diameter of the second cross-section to a difference between the diameter of the second cross-section and the diameter of the stenosis cross-section, and a fourth index value representing a ratio of a cross-sectional area of the entire blood vessel of the stenosis cross-section to an area of the stenosis cross-section, and the display unit may further be configured to display at least two index values from among the first index value, the second index value, the third index value, and the fourth index value.

[0022] The blood vessel may be a carotid artery, the first cross-section may be a cross-section of an ICA, and the second cross-section may be a cross-section of a CCA.

[0023] The processor may further be configured to render the 3D ultrasound volume data to generate a 3D ultrasound image of the object; and the display unit may further be configured to display the at least two cross-sections, the at least two stenosis index values, and the 3D ultrasound image on the display unit.

[0024] The display unit may further be configured to display a user interface that displays at least one of different colors, graphs, and figures based on sizes of the at least two stenosis index values, along with the at least two stenosis index values.

[0025] The ultrasound data acquisition unit may further be configured to transmit ultrasound signals to the object, receive ultrasound echo signals reflected by the object, and obtain the 3D ultrasound volume data from the received ultrasound echo signals.

[0026] The processor may further be configured to obtain the plurality of cross-sections of the blood vessel by segmenting the 3D ultrasound volume data at predetermined intervals, calculate, with respect to each of the plurality of cross-sections of the blood vessel, a first area value regarding a cross-section defined by a blood vessel wall of the blood vessel and a second area value regarding a cross-section through which blood flows in the blood vessel, calculate, with respect to each of the plurality of cross-sections of the blood vessel, a ratio of the first area value to the second area value, and determine a cross-section having a smallest calculated ratio as a stenosis cross-section from among the plurality of cross-sections of the blood vessel.

[0027] The processor may further be configured to obtain a brightness value for each of the plurality of cross-sections of the blood vessel, determine an area of a region whose obtained brightness value may be less than a predetermined brightness value as a second area, and calculate an area value of the second area.

[0028] The first cross-section may be spaced apart by a predetermined first interval in a first direction from the stenosis cross-section and the second cross-section may be spaced apart by the first interval in a second direction that may be opposite to the first direction from the stenosis cross-section.

[0029] The ultrasound imaging apparatus may further include a user input unit configured to receive a user input for setting a second interval that may be spaced apart from the stenosis cross-section, wherein the processor may further be configured to determine the first cross-section spaced apart by the second interval in a first direction from the stenosis cross-section and the second cross-section spaced apart by the second interval in a second direction that may be opposite to the first direction from the stenosis cross-section.

[0030] The processor may further be configured to detect from the 3D ultrasound volume data a branch point where the blood vessel diverges into two, determines a cross-section spaced apart by a third interval in a first direction from the branch point as the first cross-section, and determine a cross-section spaced apart by the third interval in a second direction that may be opposite to the first direction from the branch point as the second cross-section.

[0031] A non-transitory computer-readable recording medium may have recorded thereon a program for executing the method on a computer.

BRIEF DESCRIPTION OF THE DRAWINGS

[0032] These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

[0033] FIG. 1 is a conceptual view for explaining a method, performed by an ultrasound imaging apparatus, of obtaining an ultrasound image with respect to a blood vessel and displaying a plurality of cross-sections of the blood vessel for measurement of a degree of stenosis of the blood vessel and a plurality of stenosis index values, according to an embodiment;

[0034] FIG. 2 is a block diagram showing a configuration of an ultrasound imaging apparatus according to an embodiment;

[0035] FIG. 3 is a flowchart of a method of displaying a plurality of blood vessel cross-sections related to measurement of a degree of stenosis of the blood vessel and stenosis index values by an ultrasound imaging apparatus according to an embodiment;

[0036] FIG. 4A is a diagram for explaining a structure of a blood vessel that is stenosed;

[0037] FIG. 4B is a diagram for explaining a method, performed by an ultrasound imaging apparatus, of obtaining a plurality of blood vessel cross-sections from 3D ultrasound volume data, according to an embodiment;

[0038] FIG. 4C is a diagram for explaining a method, performed by an ultrasound imaging apparatus, of calculating a degree of stenosis for a plurality of blood vessel cross-sections, according to an embodiment;

[0039] FIG. 5 is a flowchart of a method, performed by an ultrasound imaging apparatus, of determining a stenosis cross-section from among a plurality of blood vessel cross-sections, according to an embodiment;

[0040] FIG. 6 is a diagram for explaining a method, performed by an ultrasound imaging apparatus, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel, according to an embodiment;

[0041] FIG. 7 is a block diagram showing a configuration of an ultrasound imaging apparatus according to an embodiment;

[0042] FIG. 8 is a flowchart of a method, performed by an ultrasound imaging apparatus, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel, according to an embodiment;

[0043] FIG. 9 is a diagram for explaining a method, performed by an ultrasound imaging apparatus, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel according to an embodiment;

[0044] FIG. 10 is a flowchart of a method, performed by an ultrasound imaging apparatus, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel, according to an embodiment;

[0045] FIG. 11A is a diagram for explaining a method, performed by an ultrasound imaging apparatus, of calculating a stenosis index value representing a degree of stenosis of a blood vessel, according to an embodiment;

[0046] FIG. 11B is a cross-sectional view of a blood vessel for explaining a method, performed by an ultrasound imaging apparatus, of calculating a degree of stenosis of the blood vessel, according to an embodiment;

[0047] FIGS. 12A to 12D are diagrams for explaining a method, performed by an ultrasound imaging apparatus, of displaying a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel and at least two stenosis index values representing the degree of stenosis of the blood vessel, according to an embodiment;

[0048] FIG. 13 is a block diagram showing a configuration of an ultrasound diagnosis apparatus according to an embodiment; and

[0049] FIG. 14 is a block diagram showing a configuration of a wireless probe according to an embodiment.

DETAILED DESCRIPTION

[0050] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to like elements throughout. In this regard, the present embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Accordingly, the embodiments are merely described below, by referring to the figures, to explain aspects thereof. Expressions such as “at least one of,” when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0051] The attached drawings for illustrating exemplary embodiments of the present disclosure are referred to in order to gain a sufficient understanding of the present disclosure, the merits thereof, and the objectives accomplished by the implementation of the present disclosure. In this regard, the present embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Rather, these embodiments are provided so that this disclosure will be thorough and complete and will fully convey the concept of the present embodiments to one of ordinary skill in the art, and the spirit and scope of the present invention will only be defined by the appended claims.

[0052] Hereinafter, the terms used in the specification will be briefly described, and then the present disclosure will be described in detail.

[0053] The terms used in this specification are those general terms currently widely used in the art in consideration of functions regarding the present disclosure, but the terms may vary according to the intention of those of ordinary skill in the art, precedents, or new technology in the art. Also, some terms may be arbitrarily selected by the applicant, and in this case, the meaning of the selected terms will be described in detail in the detailed description of the present specification. Thus, the terms used in the specification should be understood not as simple names but based on the meaning of the terms and the overall description of the invention.

[0054] When a part “includes” or “comprises” an element, unless there is a particular description contrary thereto, the part can further include other elements, not excluding the other elements. Also, the term “unit” in the embodiments of the present invention means a software component or hardware component such as a field-programmable gate array (FPGA) or an application-specific integrated circuit (ASIC), and performs a specific function. However, the term “unit” is not limited to software or hardware. The “unit” may be formed so as to be in an addressable storage medium, or may be formed so as to operate one or more processors. Thus, for example, the term “unit” may refer to components such as

software components, object-oriented software components, class components, and task components, and may include processes, functions, attributes, procedures, subroutines, segments of program code, drivers, firmware, micro codes, circuits, data, a database, data structures, tables, arrays, or variables. A function provided by the components and “units” may be associated with the smaller number of components and “units”, or may be divided into additional components and “units”.

[0055] Throughout the specification, an “ultrasound image” refers to an image of an object, which is obtained using ultrasound waves. Furthermore, an “object” may be a human, an animal, or a part of a human or animal. For example, the object may be an organ (e.g., the liver, the heart, the womb, the brain, a breast, or the abdomen), a blood vessel, or a combination thereof. Also, the object may be a phantom. The phantom means a material having a density, an effective atomic number, and a volume that are approximately the same as those of an organism. For example, the phantom may be a spherical phantom having properties similar to a human body.

[0056] Throughout the specification, a “user” may be, but is not limited to, a medical expert, for example, a medical doctor, a nurse, a medical laboratory technologist, or a medical imaging expert, or a technician who repairs medical apparatuses.

[0057] Furthermore, in the present specification, the terms “first”, “second”, “1-1”, etc. are only used to distinguish one component, element, image, pixel, or patch from another component, element, object, image, pixel, or patch. Thus, these terms are not limited to representing the order or priority among elements or components.

[0058] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings. In the following description, well-known functions or constructions are not described in detail so as not to obscure the embodiments with unnecessary detail.

[0059] FIG. 1 is a conceptual view for explaining a method, performed by an ultrasound imaging apparatus 100, of obtaining an ultrasound image with respect to a blood vessel 200 and displaying a plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} , and P_{240} for measurement of a degree of stenosis of the blood vessel 200 and a plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , according to an embodiment.

[0060] Referring to FIG. 1, the ultrasound imaging apparatus 100 may display a three dimensional (3D) ultrasound image 200A of an object 10 including the blood vessel 200, the plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} , and P_{240} , and the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 on a display unit 130. However, embodiments are not limited to the illustration of FIG. 1; and the ultrasound imaging apparatus 100 may display at least two stenosis index values from among the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 .

[0061] In an embodiment, the blood vessel 200 may be a carotid artery located in the neck of the object 10, i.e., a patient. A user using the ultrasound imaging apparatus 100 may scan a neck part of the object 10 by using an ultrasound probe 112 to obtain 3D ultrasound volume data with respect to the blood vessel 200. In particular, the ultrasound probe 112 may transmit ultrasound signals to the object 10, the ultrasound imaging apparatus 100 may receive ultrasound echo signals reflected by the object 10, and the 3D ultra-

sound image 200A may be generated by performing a scan conversion on the received ultrasound echo signals.

[0062] The ultrasound imaging apparatus 100 may obtain a plurality of cross-sections with respect to the blood vessel 200 from 3D ultrasound volume data of the object 10 and determine stenosis cross-sections P_{210} and P_{220} with a highest degree of stenosis by analyzing degrees of stenosis from among a plurality of cross-sections. In an embodiment, the ultrasound imaging apparatus 100 may receive a user input for selecting the stenosis cross-sections P_{210} and P_{220} in the blood vessel 200 and determine the stenosis cross-sections P_{210} and P_{220} based on the user input.

[0063] The ultrasound imaging apparatus 100 may determine a first cross-section P_{230} and a second cross-section P_{240} that may be each spaced apart in different directions from the determined stenosis cross-sections P_{210} and P_{220} . In an embodiment, the first cross-section P_{230} may be spaced apart by a predetermined interval in a first direction Y from the stenosis cross-sections P_{210} and P_{220} and the second cross-section P_{240} may be spaced apart by a predetermined interval in a second direction that is opposite to the first direction Y from the stenosis cross-sections P_{210} and P_{220} .

[0064] The ultrasound imaging apparatus 100 may calculate the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 representing a degree of stenosis of the blood vessel 200 based on a diameter or an area value of the stenosis cross-sections P_{210} and P_{220} , the first cross-section P_{230} , and the second cross-section P_{240} . In an embodiment, the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 may include at least one of North American Symptomatic Carotid Endarterectomy Trial (NASCET), European Carotid Surgery Trial (ECST), and a common carotid method (CC). The plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 are described below in relation to FIGS. 11A and 11B.

[0065] The ultrasound imaging apparatus 100 may display at least two cross-sections of the calculated plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , the stenosis cross-sections P_{210} and P_{220} , the first cross-section P_{230} , and the second cross-section P_{240} on the display unit 130. In an embodiment, the ultrasound imaging apparatus 100 may render 3D ultrasound volume data to generate the 3D ultrasound image 200A with respect to the blood vessel 200 and display the generated 3D ultrasound image 200A on the display unit 130.

[0066] In general, in the case of a two-dimensional (2D) ultrasound imaging apparatus using a one-dimensional (1D) ultrasound probe, in order to obtain ultrasound data for a plurality of cross-sections of the blood vessel 200, the object 10 including the blood vessel 200 may be scanned several times. Even in the case of a 3D ultrasound imaging apparatus, in order to obtain ultrasound data for a plurality of cross-sections of the blood vessel 200, it is inconvenient to manually adjust the position of a cross-section.

[0067] The ultrasound imaging apparatus 100 according to an embodiment may obtain ultrasound data for the stenosis cross-sections P_{210} and P_{220} , with a highest degree of stenosis in the blood vessel 200 and automatically obtain the first cross-section P_{230} and the second cross-section P_{240} with respect to the stenosis cross-sections P_{210} and P_{220} . In addition, the ultrasound imaging apparatus 100 according to an embodiment may display the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 calculated based on a diameter or an area value of the stenosis cross-sections P_{210} and P_{220} , the first cross-section P_{230} , and the second cross-section P_{240} .

together on the display unit **130**, enabling a user to determine a degree of stenosis of the blood vessel **200** and improving diagnostic usability for the user.

[0068] FIG. 2 is a block diagram showing a configuration of an ultrasound imaging apparatus **100** according to an embodiment. In the ultrasound imaging apparatus **100** of FIG. 2, only elements that are related to the present embodiment are illustrated. Therefore, it will be appreciated that other generic components may further be included, in addition to the elements shown in FIG. 2, by those of ordinary skill in the art.

[0069] Referring to FIG. 2, the ultrasound imaging apparatus **100** may include an ultrasound data acquisition unit **110**, a processor **120**, and the display unit **130**. In an embodiment, the ultrasound imaging apparatus **100** may be a cart type apparatus or a portable type apparatus. Examples of portable the ultrasound imaging apparatus **100** may include, but are not limited to, a picture archiving and communication system (PACS) viewer, a smartphone, a laptop computer, a personal digital assistant (PDA), and a tablet personal computer (PC).

[0070] The ultrasound data acquisition unit **110** may obtain ultrasound volume data with respect to the object **10** including the blood vessel **200** of FIG. 1. In an embodiment, the ultrasound data acquisition unit **110** may obtain 3D ultrasound volume data with respect to a carotid artery.

[0071] The term “ultrasound volume data” may refer to data consisting of a plurality of voxels. The ultrasound volume data with respect to the object **10** may include spatial information about the object **10** or clinical information, e.g., information about anatomical configurations of tissues or organs included in the object **10**.

[0072] In an embodiment, the ultrasound data acquisition unit **110** may generate 3D ultrasound volume data with respect to the object **10** using the ultrasound data obtained from the object **10**. In some embodiments, the ultrasound data acquisition unit **110** may obtain 3D ultrasound volume data from an external device via a communication module (see FIG. 13).

[0073] In an embodiment, the ultrasound data acquisition unit **110** may include the ultrasound probe **112** of FIG. 1 that directly transmits or receives ultrasound to or from the object **10**. The ultrasound probe **112** may transmit ultrasound signals from the object **10** and receive echo signals from the object **10**. The ultrasound probe **112** may transmit ultrasound signals to the object **10** in response to a driving signal applied to the ultrasound probe **112** and may receive echo signals reflected by the object **10**.

[0074] The ultrasound probe **112** includes a plurality of transducers, and the plurality of transducers oscillate in response to electric signals and generate acoustic energy, that is, ultrasound waves. Furthermore, the ultrasound probe **112** may be connected to the main body of the ultrasound imaging apparatus **100** by wire or wirelessly, and according to embodiments, the ultrasound imaging apparatus **100** may include a plurality of ultrasound probes **112**. In an embodiment, the ultrasound data acquisition unit **110** may include a 3D probe.

[0075] In an embodiment, the ultrasound probe **112** may transmit ultrasound plane waves to the object **10** and may receive ultrasound echo signals reflected by the object **10**, based on the transmitted ultrasound signals.

[0076] The ultrasound data acquisition unit **110** may further include a data generator **114** that obtains ultrasound data from ultrasound echo signals received from the ultrasound probe **112**.

[0077] In some embodiments, the ultrasound data acquisition unit **110** may receive ultrasound data with respect to the object **10** from an external source. The ultrasound data acquisition unit **110** may generate ultrasound data from an external apparatus connected to the ultrasound imaging apparatus **100** by wire or wirelessly.

[0078] The processor **120** may be at least one of a central processing unit (CPU), a graphic processing unit (GPU), and a micro processor. In an embodiment, the processor **120** may consist of hardware, such as FPGA or ASIC.

[0079] In an embodiment, the processor **120** may generate a 3D ultrasound image with respect to the object **10** by performing rendering with respect to 3D ultrasound volume data provided from the ultrasound data acquisition unit **110**. The term ‘rendering’ as used herein denotes generating and displaying 2D projection image of a 3D discretely sampled data set, such as 3D ultrasound volume data. In an embodiment, the processor **120** may perform rendering using ray casting projection.

[0080] The processor **120** may analyze a degree of stenosis of a plurality of cross-sections of the blood vessel **200** included in the object **10** from the ultrasound data acquisition unit **110** and may determine a stenosis cross-section with the a highest degree of stenosis from among the plurality of cross-sections. In an embodiment, the processor **120** may obtain a plurality of blood vessel cross-sections by segmenting 3D ultrasound volume data with respect to the blood vessel **200** at constant intervals. In an embodiment, the processor **120** may calculate, with respect to each of the plurality of cross-sections, a first area value regarding a cross-section defined by a blood vessel wall of the blood vessel **200** and a second area value regarding a cross-section through which blood flows in the blood vessel **200**; and may calculate, with respect to each of the plurality of cross-sections of the blood vessel **200**, a ratio of the first area value to the second area value. The processor **120** may determine a cross-section having the smallest calculated ratio as a stenosis cross-section from among a plurality of blood vessel cross-sections. Methods of determining a stenosis cross-section will be described in detail in relation to FIGS. 4B, 4C, and 5.

[0081] The processor **120** may determine a first cross-section and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among a plurality of cross-sections of the blood vessel **200**. In an embodiment, the processor **120** may determine a first cross-section and a second cross-section that are spaced apart by the same interval in opposite directions from the stenosis cross-section. In an embodiment, the processor **120** may detect a branch point where the blood vessel **200** diverges into two from the 3D ultrasound volume data with respect to the blood vessel obtained from the ultrasound data acquisition unit **110** and may determine a first cross-section and a second cross-section spaced apart by the same interval on different directions from the detected branch point. The method of determining a first cross-section and a second cross-section by the processor **120** will be described in detail in relation to FIGS. 6 to 10.

[0082] The processor **120** may calculate at least two stenosis index values, which numerically represent a degree

of stenosis of the blood vessel **200**, from a diameter or a cross-sectional area of each of the determined stenosis cross-section, first cross-section, and second cross-section. In an embodiment, the processor **120** may calculate at least two index values, which may be selected from NASCET, ECST, and CC. The stenosis index values will be described in detail in relation to FIG. 11.

[0083] The display unit **130** may display at least two cross-sections of the stenosis cross-section, the first cross-section, and the second cross-section and at least two stenosis index values. In an embodiment, the display unit **130** may display a 3D ultrasound image with respect to the object **10** alongside the stenosis cross-section, the first cross-section, the second cross-section, and a plurality of stenosis index values. In an embodiment, the display unit **130** may display a plurality of stenosis index values along with a user interface that displays at least one of different colors, graphs, and figures, based on sizes of at least two stenosis index values. Displaying at least two stenosis index values on the display unit **130** will be described in detail in relation to FIGS. 12A to 12D.

[0084] The ultrasound imaging apparatus **100** according to an embodiment may determine a stenosis cross-section of the blood vessel **200** with a highest degree of stenosis from 3D ultrasound volume data of the blood vessel **200** of FIG. 1 included in the object **10**, determine a first cross-section and a second cross-section that are spaced apart in different directions from the stenosis cross-section of the blood vessel **200**, and may calculate at least two stenosis index values representing a degree of stenosis of the blood vessel **200**, based on a diameter or a cross-section area size of the stenosis cross-section, the first cross-section, and the second cross-section. In addition, the ultrasound imaging apparatus **100** may display the stenosis cross-section, the first cross-section, and the second cross-section and the at least two stenosis index values on the display unit **130**, improving diagnostic usability for the user. Furthermore, the ultrasound imaging apparatus **100** may display at least two stenosis index values by using at least one of different colors, graphs, and figures, enabling a user to quickly and accurately recognize the degree of stenosis of a blood vessel.

[0085] The method of determining a stenosis cross-section, a first cross-section, and a second cross-section and the method of displaying at least two stenosis index values in the ultrasound imaging apparatus **100**, according to an embodiment, will be described in detail hereinafter.

[0086] FIG. 3 is a flowchart of a method, performed by the ultrasound imaging apparatus **100**, of displaying a plurality of blood vessel cross-sections related to measurement of a degree of stenosis of a blood vessel and stenosis index values, according to an embodiment.

[0087] In operation S310, the ultrasound imaging apparatus **100** may obtain 3D ultrasound volume data with respect to an object including a blood vessel. In an embodiment, the ultrasound imaging apparatus **100** may include an ultrasound probe, and the ultrasound probe may transmit ultrasound signals to an object and may receive ultrasound echo signals reflected by the object. The ultrasound imaging apparatus **100** may obtain 3D ultrasound volume data from the received ultrasound echo signals.

[0088] In operation S320, the ultrasound imaging apparatus **100** may analyze a degree of stenosis for a plurality of blood vessel cross-sections from 3D ultrasound volume data and determine a stenosis cross-section with a highest degree

of stenosis. In an embodiment, the ultrasound imaging apparatus **100** may obtain a plurality of blood vessel cross-sections by segmenting 3D ultrasound volume data with respect to the blood vessel at constant intervals. The ultrasound imaging apparatus **100** may calculate, with respect to each of the plurality of blood vessel cross-sections, a ratio of an area value of a cross-section of the entire blood vessel defined by the blood vessel wall to an area value of a cross-section through which blood flows in the blood vessel and determine a cross-section having the smallest calculated ratio as a stenosis cross-section.

[0089] In operation S330, the ultrasound imaging apparatus **100** may determine a first cross-section and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among a plurality of blood vessel cross-sections. In an embodiment, the ultrasound imaging apparatus **100** may determine a first cross-section and a second cross-section that are spaced apart by the same interval in opposite directions from the stenosis cross-section determined in operation S320.

[0090] In operation S340, the ultrasound imaging apparatus **100** may display at least two cross-sections of the stenosis cross-section, the first cross-section, and the second cross-section and at least two stenosis index values representing the degree of stenosis of the blood vessel. In an embodiment, the ultrasound imaging apparatus **100** may calculate the at least two stenosis index values representing a degree of stenosis of the blood vessel, based on a diameter or a cross-section area of the stenosis cross-section, the first cross-section, and the second cross-section. In an embodiment, the ultrasound imaging apparatus **100** may render 3D ultrasound volume data with respect to the object obtained in operation S310 to generate a 3D ultrasound image with respect to the blood vessel and display the generated 3D ultrasound image alongside the stenosis cross-section, the first cross-section, the second cross-section, and the at least two stenosis index values on the display unit **130** in FIGS. 1 and 2.

[0091] FIG. 4A is a diagram for explaining a structure of a blood vessel that is stenosed.

[0092] Referring to FIG. 4A, the ultrasound imaging apparatus **100** may generate and display an ultrasound image of the blood vessel **200**, e.g., a carotid artery. The image generated by the ultrasound imaging apparatus **100** may include plaque **202** deposited on and accumulated in the blood vessel wall **201**. The image displayed on a display of the ultrasound imaging apparatus **100**, which shows the plaque **202**, may have a variation in at least one of a size, a shape, and a position of the plaque **202**, depending on a degree of stenosis of the blood vessel. Depending on the size, the shape, and the position of the plaque **202** deposited in the blood vessel **200**, the size of region through which the blood can actually flow in the entire area of the blood vessel defined by the blood vessel wall **201** may vary.

[0093] FIG. 4B is a diagram for explaining a method, performed by the ultrasound imaging apparatus **100**, of obtaining a plurality of blood vessel cross-sections from 3D ultrasound volume data, according to an embodiment.

[0094] Referring to FIG. 4B, the ultrasound imaging apparatus **100** may obtain a plurality of blood vessel cross-sections **200-1** to **200-n** from 3D ultrasound volume data with respect to the blood vessel **200**. In an embodiment, the ultrasound imaging apparatus **100** may obtain the plurality

of blood vessel cross-sections **200-1** to **200-n** by segmenting 3D ultrasound volume data with respect to the blood vessel **200** at predetermined intervals Δd . The plurality of blood vessel cross-sections **200-1** to **200-n** may each include the blood vessel wall **201** and the plaque **202**. The plaque **202** included in the plurality of blood vessel cross-sections **200-1** to **200-n** may vary in size and shape.

[0095] The ultrasound imaging apparatus **100** may determine a cross-section, which may have the largest area ratio of the entire area of the blood vessel defined by the blood vessel wall **201** to plaque **202**, as a stenosis cross-section from among the plurality of blood vessel cross-sections **200-1** to **200-n**. The degree of stenosis of a cross-section of the blood vessel **200** may mean the degree of constriction of the blood vessel **200** due to accumulation of deposited plaque on the blood vessel wall **201**. The degree of stenosis of a cross-section of the blood vessel **200** may be measured by comparing an area of a reference region defined by the blood vessel wall **201** with an area of an internal region through which the blood flows. The internal region may mean an area of a blood vessel through which the blood actually flows with the exception of the plaque **202** accumulated on the blood vessel wall **201**. The ultrasound imaging apparatus **100** may deduct the cross-section area, through which the blood flows, from the reference region to thereby measure a ratio of the plaque **202** accumulated on the blood vessel wall.

[0096] The method, performed by the ultrasound imaging apparatus **100**, of determining a stenosis cross-section from among the plurality of blood vessel cross-sections **200-1** to **200-n** will be described with reference to FIG. 4C.

[0097] FIG. 4C is a diagram for explaining a method, performed by the ultrasound imaging apparatus **100**, of calculating a degree of stenosis for a plurality of blood vessel cross-sections, according to an embodiment.

[0098] FIG. 4C is a cross-sectional view of a cross-section **200-1** from among the plurality of blood vessel cross-sections **200-1** to **200-n**. The blood vessel wall **201**, the plaque **202**, and an internal region **203** through which the blood flows in the blood vessel **200** are depicted in FIG. 4C. The ultrasound imaging apparatus **100** may obtain a brightness value from ultrasound data for the plurality of blood vessel cross-sections **200-1** to **200-n** in FIG. 4B. In an embodiment, the ultrasound imaging apparatus **100** may determine an area of a region where the obtained brightness value is less than a predetermined brightness value as the internal region **203**.

[0099] The ultrasound imaging apparatus **100** may calculate a first area value regarding the entire region defined by the blood vessel wall **201**, and calculate a second area value regarding an area **A 2** of the internal region **203** through which the blood flows excluding the plaque **202**. The ultrasound imaging apparatus **100** may calculate a first area value and a second area value with respect to each of the plurality of blood vessel cross-sections **200-1** to **200-n** and a ratio of the first area value to the second area value with respect to each of the plurality of blood vessel cross-sections **200-1** to **200-n**.

[0100] The ultrasound imaging apparatus **100** may determine a cross-section having the smallest calculated ratio with respect to the plurality of blood vessel cross-sections **200-1** to **200-n** as a stenosis cross-section. In other words, a blood vessel cross-section having the smallest ratio of the

plaque **202** in the cross-sectional area of the entire blood vessel defined by the blood vessel wall **201** is determined as a stenosis cross-section.

[0101] FIG. 5 is a flowchart of a method, performed by the ultrasound imaging apparatus **100**, of determining a stenosis cross-section from among a plurality of cross-sections of a blood vessel, according to an embodiment.

[0102] In operation S510, the ultrasound imaging apparatus **100** may obtain a plurality of blood vessel cross-sections by segmenting 3D ultrasound volume data with respect to an object including a blood vessel at constant intervals.

[0103] In operation S520, the ultrasound imaging apparatus **100** may calculate, with respect to each of the plurality of cross-sections of the blood vessel, a first area value regarding a cross-section of the blood vessel defined by a blood vessel wall and a second area value regarding an internal region through which the blood flows in the blood vessel. The blood vessel may include plaque deposited on the blood vessel wall, and the second area value for the plurality of cross-sections of the blood vessel may vary due to the difference in size and shape of the plaque.

[0104] The ultrasound imaging apparatus **100** may obtain a brightness value from ultrasound volume data with respect to each of the plurality of cross-sections of the blood vessel and determine an area of a region where the obtained brightness value is less than a predetermined brightness value as the internal region. The ultrasound imaging apparatus **100** may calculate the second area value regarding the determined internal region.

[0105] In operation S530, the ultrasound imaging apparatus **100** may calculate a ratio of the first area value to the second area value for each of the plurality of blood vessel cross-sections.

[0106] In operation S540, the ultrasound imaging apparatus **100** may determine a cross-section having the smallest calculated ratio as a stenosis cross-section from among the plurality of blood vessel cross-sections.

[0107] FIG. 6 is a diagram for explaining a method, performed by the ultrasound imaging apparatus **100**, of determining the plurality of blood vessel cross-sections P_{230} and P_{240} for measurement of a degree of stenosis of the blood vessel **200**, according to an embodiment. In an embodiment, the blood vessel **200** may be a carotid artery, and a stenosis section **210** may be formed between an internal carotid artery **230** and a common carotid artery **240**.

[0108] Referring to FIG. 6, the ultrasound imaging apparatus **100** may determine the stenosis cross-section P_{210} from 3D ultrasound volume data with respect to the blood vessel **200** and determine the first cross-section P_{230} and the second cross-section P_{240} spaced apart from each other in different directions from the stenosis cross-section P_{210} . The ultrasound imaging apparatus **100** may determine the stenosis cross-section P_{210} from among the plurality of blood vessel cross-sections **200-1** to **200-n** in FIG. 4B by using the method described with reference to FIGS. 4B, 4C, and 5, but embodiments are not limited thereto. In an embodiment, the ultrasound imaging apparatus **100** may receive a user input for setting the stenosis cross-sections P_{210} from among the plurality of blood vessel cross-sections **200-1** to **200-n** and determine the stenosis cross-sections P_{210} based on the user input.

[0109] In an embodiment, the ultrasound imaging apparatus **100** may determine the first cross-section P_{230} spaced apart by a predetermined first interval $d1$ in the first direction

Y from the determined stenosis cross-section P_{210} and the second cross-section P_{240} spaced apart by the first interval $d1$ in a second direction opposite to the first direction Y from the stenosis cross-section P_{210} . In an embodiment, the first interval $d1$ may be 1 cm or less, but embodiments are not limited thereto. The ultrasound imaging apparatus **100** may automatically determine the first cross-section P_{230} and the second cross-section P_{240} , once the determination of the stenosis cross-section P_{210} is complete. However, embodiments are not limited thereto; and the ultrasound imaging apparatus **100** may receive a user input for setting the first cross-section P_{230} and the second cross-section P_{240} and determine the first cross-section P_{230} and the second cross-section P_{240} based on the received user input.

[0110] The first interval $d1$ may be predetermined, embodiments are not limited thereto. In an embodiment, the ultrasound imaging apparatus **100** may receive a user input for setting the first interval $d1$ and determine the first interval $d1$ based on the received user input.

[0111] In an embodiment, the blood vessel **200** may be a carotid artery, the first cross-section P_{230} determined by the ultrasound imaging apparatus **100** may be a cross-section of an internal carotid artery (ICA), and the second cross-section P_{240} may be a cross-section of a common carotid artery (CCA). However, these are for illustrative purposes only; and the blood vessel **200** is not limited thereto.

[0112] FIG. 7 is a block diagram showing a configuration of an ultrasound imaging apparatus **100** according to another embodiment.

[0113] Referring to FIG. 7, the ultrasound imaging apparatus **100** may include the ultrasound data acquisition unit **110**, the processor **120**, the display unit **130**, a user input unit **140**, and a memory **150**. The ultrasound data acquisition unit **110**, the processor **120**, and the display unit **130** may be the same as those described above in relation to FIG. 2; and thus descriptions thereof will be omitted here.

[0114] The user input unit **140** may receive a user input for controlling the ultrasound imaging apparatus **100**. For example, the user input unit **140** may include hardware components, such as a keypad, a mouse, a touch pad, a touch screen, a track ball, and a jog switch. However, embodiments are not limited thereto. In an embodiment, the user input unit **140** may receive a user input for setting the stenosis cross-section P_{210} in FIG. 6 from among a plurality of blood vessel cross-sections of 3D ultrasound volume data obtained from the ultrasound data acquisition unit **110**. Furthermore, in an embodiment, the user input unit **140** may receive a user input for setting the first interval $d1$ in FIG. 6 spaced apart from the stenosis cross-section P_{210} for determination of the first and second cross-sections P_{230} and P_{240} in FIG. 6. In addition, in an embodiment, the user input unit **140** may receive a user input for setting the first cross-section P_{230} and the second cross-section P_{240} .

[0115] The memory **150** stores various data processed by the ultrasound imaging apparatus **100**. The memory **1500** may be any of various storage media, e.g., a flash memory, a hard disk drive, EEPROM, etc, but embodiments are not limited thereto. In an embodiment, the memory **150** may store information about the stenosis cross-section P_{210} , the first cross-section P_{230} , and the second cross-section P_{240} according to a user input received from the user input unit **140**. Additionally, in an embodiment, the memory **150** may store a value of the first interval $d1$ received from the user input unit **140**.

[0116] In an embodiment, the memory **150** may store a 3D ultrasound image generated by volume rendering in the processor **120**.

[0117] FIG. 8 is a flowchart of a method, performed by the ultrasound imaging apparatus **100**, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel, according to an embodiment.

[0118] In operation S810, the ultrasound imaging apparatus **100** may analyze a degree of stenosis for a plurality of blood vessel cross-sections from 3D ultrasound volume data and determine a stenosis cross-section with a highest degree of stenosis. Operation S810 is the same as operation S320 described above in relation to FIG. 3, and thus descriptions thereof will be omitted here.

[0119] In operation S820, the ultrasound imaging apparatus **100** may receive a user input for setting a first interval spaced apart from the stenosis cross-section. The user input unit **140** in FIG. 7 of the ultrasound imaging apparatus **100** may receive a user input for setting a first interval and the received first interval value may be stored in the memory **150** in FIG. 7.

[0120] In operation S830, the ultrasound imaging apparatus **100** may determine a first cross-section spaced apart by the first interval in a first direction from the stenosis cross-section and a second cross-section spaced apart by the first interval in a second direction from the stenosis cross-section, in 3D ultrasound volume data. The first cross-section and the second cross-section may be spaced apart in opposite directions from each other. That is, the second direction may be opposite to the first direction. When a stenosis cross-section is determined in operation S810, the ultrasound imaging apparatus **100** may automatically determine a first cross-section and a second cross-section based on a user input for setting the first interval, but embodiments are not limited thereto. In an embodiment, the ultrasound imaging apparatus **100** may receive a user input for setting the first cross-section and the second cross-section and determine the first cross-section and the second cross-section based on the received user input.

[0121] FIG. 9 is a diagram for explaining a method, performed by the ultrasound imaging apparatus **100**, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel **200**, according to an embodiment.

[0122] Referring to FIG. 9, the ultrasound imaging apparatus **100** may obtain the plurality of blood vessel cross-sections **200-1** to **200-4** from 3D ultrasound volume data with respect to the blood vessel **200** and determine the first cross-section P_{230} and the second cross-section P_{240} from among the plurality of blood vessel cross-sections **200-1** to **200-4**.

[0123] The ultrasound imaging apparatus **100** may analyze the shape of the blood vessel **200** in the plurality of blood vessel cross-sections **200-1** to **200-4** to detect a branch point **200B** where the blood vessel **200** diverges into two. In an embodiment, the ultrasound imaging apparatus **100** may track cross-sections of the blood vessel **200** from the lower side in a Y direction to analyze the shape of the blood vessel **200**. For example, the ultrasound imaging apparatus **100** may detect a first point cross-section **200B-1** with respect to the blood vessel **200** at a first point B_1 . The first point cross-section **200B-1** may mean a cross-section of the blood vessel **200** in an X direction at the first point B_1 from among a plurality of points segmented at constant intervals in the Y

direction. Likewise, the ultrasound imaging apparatus 100 may detect a second point cross-section 200B-2 with respect to the blood vessel 200 at a second point B₂ and third point cross-sections 200B-3 and 200B-4 with respect to the blood vessel 200 at a third point B₃. The ultrasound imaging apparatus 100 may detect the third point cross-sections 200B-3 and 200B-4, which may be blood vessel cross-sections that are divided at the third point B₃. As shown in FIG. 9, the ultrasound imaging apparatus 100 may detect a branch point 200B where the blood vessel 200 diverges into two branches, in which the branch point 200B may be between the second point B₂ and the third point B₃.

[0124] The ultrasound imaging apparatus 100 may determine, about the branch point 200B, the first cross-section P₂₃₀ spaced apart by a second interval d₂ in the first direction Y and the second cross-section P₂₄₀ spaced apart by the second interval d₂ in a second direction opposite to the first direction Y. In an embodiment, the second interval d₂ may be predetermined. The second interval d₂ may be stored in the memory 150. In an embodiment, the ultrasound imaging apparatus 100 may receive a user input for setting the second interval d₂ and determine the second interval d₂ based on the received user input. In an embodiment, the second interval d₂ may have a value of about 1 cm or less, but embodiments are not limited thereto.

[0125] In an embodiment, the blood vessel 200 may be a carotid artery, the first cross-section P₂₃₀ determined by the ultrasound imaging apparatus 100 may be a cross-section of an ICA, and the second cross-section P₂₄₀ may be a cross-section of a CCA. However, these are for illustrative purposes only; and the blood vessel 200 is not limited thereto.

[0126] FIG. 10 is a flowchart of a method, performed by the ultrasound imaging apparatus 100, of determining a plurality of blood vessel cross-sections for measurement of a degree of stenosis of the blood vessel, according to an embodiment.

[0127] In operation S1010, the ultrasound imaging apparatus 100 may obtain a plurality of blood vessel cross-sections by processing 3D ultrasound volume data with respect to an object including a blood vessel. Operation S1010 is the same as operation S320 explained in relation to FIG. 3, and thus descriptions thereof will be omitted.

[0128] In operation S1020, the ultrasound imaging apparatus 100 may detect from the 3D ultrasound volume data a branch point where the blood vessel diverges into two. The ultrasound imaging apparatus 100 may obtain, from the 3D ultrasound volume data, a plurality of blood vessel cross-sections that are segmented at constant intervals in the first direction Y at a plurality of points. The ultrasound imaging apparatus 100 may analyze the plurality of blood vessel cross-sections to detect a branch point where the blood vessel diverges into two. In an embodiment, the ultrasound imaging apparatus 100 may detect the branch point by the change of the number of blood vessels included in the plurality of blood vessel cross-sections.

[0129] In operation S1030, the ultrasound imaging apparatus 100 may determine a cross-section spaced apart by a second interval in the first direction Y from the branch point detected in operation S1020 as a first cross-section and a cross-section spaced apart by the second interval in a second direction opposite to the first direction Y from the branch point as a second cross-section. The value of the second interval may be a predetermined value, but embodiments are not limited thereto. The ultrasound imaging apparatus 100

may receive a user input for setting a value of the second interval and determine the second interval based on the received user input.

[0130] FIG. 11A is a diagram for explaining a method, performed by the ultrasound imaging apparatus 100, of calculating a stenosis index value representing a degree of stenosis of the blood vessel 200, according to an embodiment. FIG. 11B is a cross-sectional view of the blood vessel 200 for explaining a method, performed by the ultrasound imaging apparatus 100, of calculating a degree of stenosis of the blood vessel 200, according to an embodiment. In FIGS. 11A and 11B, the blood vessel 200 may be a carotid artery, but embodiments are not limited thereto.

[0131] Referring to FIGS. 11A and 11B, the ultrasound imaging apparatus 100 may determine the stenosis cross-sections P₂₁₀ and P₂₂₀, the first cross-section P₂₃₀, and the second cross-section P₂₄₀ from 3D ultrasound volume data with respect to the blood vessel 200. The stenosis cross-sections P₂₁₀ and P₂₂₀ shown in FIG. 11B may include the first stenosis cross-section P₂₁₀ with respect to an internal region through which the blood flows in the blood vessel 200 and plaque, and the second stenosis cross-section P₂₂₀, which is a cross-section of the entire blood vessel defined by the blood vessel wall.

[0132] The ultrasound imaging apparatus 100 may calculate at least two of the plurality of stenosis index values I₁, I₂, I₃, and I₄ representing a degree of stenosis of the blood vessel 200 based on a diameter or a cross-section area value of each of the stenosis cross-sections P₂₁₀ and P₂₂₀, the first cross-section P₂₃₀, and the second cross-section P₂₄₀.

[0133] In particular, the ultrasound imaging apparatus 100 may calculate the first index value I₁ representing a ratio of a diameter D₂₃₀ of the first cross-section P₂₃₀ to a difference between the diameter D₂₃₀ of the first cross-section P₂₃₀ and a diameter D₂₁₀ of the first stenosis cross-section P₂₁₀, as in Equation 1.

$$I_1 = \frac{D_{230} - D_{210}}{D_{230}} \times 100 \quad \text{Equation 1}$$

[0134] In an embodiment, the first index value I₁ may be a NASCET index value.

[0135] The ultrasound imaging apparatus 100 may calculate the second index value I₂ representing a ratio of a diameter D₂₂₀ of the second stenosis cross-section P₂₂₀ to a difference between the diameter D₂₂₀ of the second stenosis cross-section P₂₂₀ and the diameter D₂₁₀ of the first stenosis cross-section P₂₁₀, as in Equation 2.

$$I_2 = \frac{D_{220} - D_{210}}{D_{220}} \times 100 \quad \text{Equation 2}$$

[0136] In an embodiment, the second index value I₂ may be an ECST index value.

[0137] The ultrasound imaging apparatus 100 may calculate the third index value I₃ representing a ratio of a diameter D₂₄₀ of the second cross-section P₂₄₀ to a difference between the diameter D₂₄₀ of the second cross-section P₂₄₀ and the diameter D₂₁₀ of the first stenosis cross-section P₂₁₀, as in Equation 3.

$$I_3 = \frac{D_{240} - D_{210}}{D_{240}} \times 100 \quad \text{Equation 3}$$

[0138] In an embodiment, the third index value I_3 may be a CC index value.

[0139] The ultrasound imaging apparatus 100 may calculate the fourth index value I_4 representing a ratio of an area value A_{220} of the second stenosis cross-section P_{220} to an area value A_{210} of the first stenosis cross-section P_{210} , as in Equation 4.

$$I_4 = \frac{A_{210}}{A_{220}} \times 100 \quad \text{Equation 4}$$

[0140] The ultrasound imaging apparatus 100 may obtain brightness values of each of a plurality of blood vessel cross-sections obtained from 3D ultrasound volume data with respect to the blood vessel 200 and determine an area of a region where the obtained brightness value is less than a predetermined brightness value as the stenosis cross-section P_{210} to calculate the fourth index value I_4 . This has been described in detail in relation to FIGS. 4C and 5, and thus a repeated description thereof will be omitted here. In an embodiment, the fourth index value I_4 may be an area reduction index value.

[0141] FIGS. 12A to 12D are diagrams for explaining a method, performed by the ultrasound imaging apparatus 100, of displaying the plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} and P_{240} for measurement of a degree of stenosis of the blood vessel 200 and the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 representing the degree of stenosis of the blood vessel 200, according to an embodiment.

[0142] Referring to FIG. 12A, the ultrasound imaging apparatus 100 may display the 3D ultrasound image 200A with respect to the blood vessel 200, the plurality of blood vessel cross-sections P_{210} , P_{220} , and P_{230} , and the plurality of stenosis index values I_1 and I_4 on the display unit 130. In an embodiment, the 3D ultrasound image 200A may be displayed on a first region 131 of the display unit 130, the stenosis cross-sections P_{210} and P_{220} and the first cross-section P_{230} may be displayed on a second region 132 of the display unit 130, and the two stenosis index values I_1 and I_4 may be displayed on a third region 133 of the display unit 130.

[0143] In FIG. 12A, it is illustrated that the first stenosis cross-section P_{210} , the second stenosis cross-section P_{220} , and the first cross-section P_{230} are all displayed on the second region 132, but embodiments are not limited thereto. At least two cross-sections of the first stenosis cross-section P_{210} , the second stenosis cross-section P_{220} , the first cross-section P_{230} , and the second cross-section P_{240} may be displayed on the second region 132. In an embodiment, a user interface representing a diameter of each of the first stenosis cross-section P_{210} , the second stenosis cross-section P_{220} , and the first cross-section P_{230} may be displayed on the second region 132.

[0144] In an embodiment, the 3D ultrasound image 200A may be an ultrasound image of a carotid artery and the first cross-section P_{230} may be a cross-section of ICA.

[0145] In FIG. 12A, it is illustrated that the first index value I_1 and the fourth index value I_4 are displayed on the third region 133, but embodiments are not limited thereto. In an embodiment, at least two index values of the first index value I_1 as a NASCET value, the second index value I_2 as an ECST value, the third index value I_3 as a CC value, and the fourth index value I_4 as an area reduction value may be displayed on the third region 133. For example, three index values including the first index value I_1 , the second index value I_2 , and the third index value I_3 may be displayed on the third region 133.

[0146] In the embodiment illustrated in FIG. 12A, the ultrasound imaging apparatus 100 may display the stenosis cross-sections P_{210} and P_{220} , the first cross-section P_{230} , and the two stenosis index values I_1 and I_4 representing a degree of stenosis of the blood vessel 200 on the display unit 130, enabling a user to easily recognize the degree of stenosis of the blood vessel 200 and improving diagnostic usability for the user. Furthermore, the ultrasound imaging apparatus 100 may display the 3D ultrasound image 200A with respect to the blood vessel 200 alongside the stenosis cross-sections P_{210} and P_{220} , the first cross-section P_{230} , and the two stenosis index values I_1 and I_4 on the display unit 130, enabling a user to easily recognize a degree of stenosis in accordance with the structure of the blood vessel 200.

[0147] Referring to FIG. 12B, the ultrasound imaging apparatus 100 may display the 3D ultrasound image 200A with respect to the blood vessel 200, the plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} , and P_{240} and the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 on the display unit 130. In the embodiment illustrated in FIG. 12A, the four stenosis index values I_1 , I_2 , I_3 , and I_4 are shown; however this is for illustrative purposes only and three stenosis index values of the four stenosis index values I_1 , I_2 , I_3 , and I_4 may be displayed. In an embodiment, the ultrasound imaging apparatus 100 may select any three stenosis index values to be displayed on the display unit 130 from the four stenosis index values I_1 , I_2 , I_3 , and I_4 . The plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 to be displayed on the display unit 130 may be the same as those described in relation to FIG. 12A, and thus descriptions thereof will be omitted here.

[0148] In an embodiment, the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 to be displayed on the third region 133 may be displayed in different colors depending on the size of each of the index values. For example, when the size of the first index value I_1 is in a range of 0% to 40%, the first index value I_1 may be displayed in blue; when the size thereof is in a range of 40% to 60%, the first index value I_1 may be displayed in yellow; and when the size thereof is in a range of 60% to 90%, the first index value I_1 may be displayed in red. In such a manner, the first index value I_1 may be displayed in different colors depending on the size of the index value. However, the correspondences between the foregoing numerical values and the colors are merely examples for explaining color displaying according to a size of an index value, and thus, the scope of the present disclosure is not limited thereto.

[0149] Referring to FIG. 12C, a user interface including a plurality of graphs I_1' , I_2' , I_3' , and I_4' may be displayed on the third region 133 of the display unit 130, in which the plurality of graphs I_1' , I_2' , I_3' , and I_4' each corresponds to the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , respectively. The 3D ultrasound image 200A displayed on the first

region 131 and the plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} , and P_{240} displayed on the second region 132 may be the same as those described in connection with FIG. 12A, and thus, descriptions thereof will be omitted here.

[0150] The plurality of graphs I_1' , I_2' , I_3' , and I_4' may each be distinctively displayed depending on a size of the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , respectively. For example, when a size of the first index value I_1 is about 60%, the first graph I_1' may be displayed at about 60% of the full size. Although bar graphs are shown in FIG. 12C, the type of the graphs are not limited thereto, and a pie chart, a graph of broken lines, or histogram, may also be used.

[0151] Referring to FIG. 12D, a user interface including a plurality of figures I_1'' , I_2'' , I_3'' , and I_4'' each having distinct shapes may be displayed on the third region 133, in which the plurality of figures I_1'' , I_2'' , I_3'' , and I_4'' respectively correspond to the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 . The 3D ultrasound image 200A displayed on the first region 131 and the plurality of blood vessel cross-sections P_{210} , P_{220} , P_{230} , and P_{240} displayed on the second region 132 may be the same as those described in connection with FIG. 12A, and thus, descriptions thereof will be omitted here.

[0152] The plurality of figures I_1'' , I_2'' , I_3'' , and I_4'' may each be distinctively displayed depending on a size of the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , respectively. For example, when a size of the first index value I_1 is about 60%, and a size of the second index value I_2 is about 90%, the first figure I_1'' and the second figure I_2'' may have different shapes from each other. For example, the first figure I_1'' may be in a circular shape figure, and the second figure I_2'' may be in a star shape figure. However, figures shown in FIG. 12D are for illustrative purposes only; and the shapes of figures representing the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 are not limited thereto.

[0153] In the embodiments of FIGS. 12C and 12D, the ultrasound imaging apparatus 100 may display graphs or figures for the plurality of stenosis index values I_1 , I_2 , I_3 , and I_4 , which represent a degree of stenosis of the blood vessel 200, enabling a user to intuitively recognize the degree of stenosis of the blood vessel 200.

[0154] FIG. 13 is a block diagram showing a configuration of an ultrasound diagnosis apparatus 1000 according to an embodiment. Referring to FIG. 13, the ultrasound diagnosis apparatus 1000 may include a probe 20, an ultrasound transceiver 1100, an image processor 1200, a communication module 1300, a display 1400, a memory 1500, an input device 1600, and a controller 1700, which may be connected to one another via buses 1800.

[0155] The ultrasound imaging apparatus 100 illustrated in FIG. 2 may include the same configuration as the ultrasound diagnosis apparatus 1000 illustrated in FIG. 13. In an embodiment, the ultrasound transceiver 1100 may be equivalent to the ultrasound data acquisition unit 110 shown in FIG. 2, the image processor 1200 may be equivalent to the processor 120 shown in FIG. 2, and the display 1400 may be equivalent to the display unit 130 shown in FIG. 2.

[0156] The ultrasound diagnosis apparatus 1000 may be a cart type apparatus or a portable type apparatus. Examples of portable ultrasound diagnosis apparatuses may include, but are not limited to, a PACS viewer, a smartphone, a laptop computer, a PDA, and a tablet PC.

[0157] The probe 20 transmits ultrasound waves to an object 10 in response to a driving signal applied by the ultrasound transceiver 1100 and receives echo signals

reflected by the object 10. The probe 20 includes a plurality of transducers, and the plurality of transducers oscillate in response to electric signals and generate acoustic energy, that is, ultrasound waves. Furthermore, the probe 20 may be connected to the main body of the ultrasound diagnosis apparatus 1000 by wire or wirelessly, and according to embodiments, the ultrasound diagnosis apparatus 1000 may include a plurality of probes 20.

[0158] A transmitter 1110 supplies a driving signal to the probe 20. The transmitter 110 includes a pulse generator 1112, a transmission delaying unit 1114, and a pulser 1116. The pulse generator 1112 generates pulses for forming transmission ultrasound waves based on a pulse repetition frequency (PRF), and the transmission delaying unit 1114 delays the pulses by delay times necessary for determining transmission directionality. The pulses which have been delayed correspond to a plurality of piezoelectric vibrators included in the probe 20, respectively. The pulser 1116 applies a driving signal (or a driving pulse) to the probe 20 based on timing corresponding to each of the pulses which have been delayed.

[0159] A receiver 1120 generates ultrasound data by processing echo signals received from the probe 20. The receiver 120 may include an amplifier 1122, an analog-to-digital converter (ADC) 1124, a reception delaying unit 1126, and a summing unit 1128. The amplifier 1122 amplifies echo signals in each channel, and the ADC 1124 performs analog-to-digital conversion with respect to the amplified echo signals. The reception delaying unit 1126 delays digital echo signals output by the ADC 124 by delay times necessary for determining reception directionality, and the summing unit 1128 generates ultrasound data by summing the echo signals processed by the reception delaying unit 1126. In some embodiments, the receiver 1120 may not include the amplifier 1122. In other words, if the sensitivity of the probe 20 or the capability of the ADC 1124 to process bits is enhanced, the amplifier 1122 may be omitted.

[0160] The image processor 1200 generates an ultrasound image by scan-converting ultrasound data generated by the ultrasound transceiver 1100. The ultrasound image may be not only a grayscale ultrasound image obtained by scanning an object in an amplitude (A) mode, a brightness (B) mode, and a motion (M) mode, but also a Doppler image showing a movement of an object via a Doppler effect. The Doppler image may be a blood flow Doppler image showing flow of blood (also referred to as a color Doppler image), a tissue Doppler image showing a movement of tissue, or a spectral Doppler image showing a moving speed of an object as a waveform.

[0161] A B mode processor 1212 included in a data processor 1210 extracts B mode components from ultrasound data and processes the B mode components. An image generator 1220 may generate an ultrasound image indicating signal intensities as brightness based on the extracted B mode components 1212.

[0162] Similarly, a Doppler processor 1214 included in the data processor 1210 may extract Doppler components from ultrasound data, and the image generator 1220 may generate a Doppler image indicating a movement of an object as colors or waveforms based on the extracted Doppler components.

[0163] According to an embodiment, the image generator 1220 may generate a 3D ultrasound image via volume-rendering with respect to volume data and may also generate

an elasticity image by imaging deformation of the object **10** due to pressure. Furthermore, the image generator **1220** may display various pieces of additional information in an ultrasound image by using text and graphics. In addition, the generated ultrasound image may be stored in the memory **1500**.

[0164] A display **1400** displays the generated ultrasound image. The display **1400** may display not only an ultrasound image, but also various pieces of information processed by the ultrasound diagnosis apparatus **1000** on a screen image via a graphical user interface (GUI). In addition, the ultrasound diagnosis apparatus **1000** may include two or more displays **1400** according to embodiments.

[0165] The communication module **1300** is connected to a network **30** by wire or wirelessly to communicate with an external device or a server. The communication module **1300** may exchange data with a hospital server or another medical apparatus in a hospital, which is connected thereto via a PACS. Furthermore, the communication module **1300** may perform data communication according to the digital imaging and communications in medicine (DICOM) standard.

[0166] The communication module **1300** may transmit or receive data related to diagnosis of an object, e.g., an ultrasound image, ultrasound data, and Doppler data of the object, via the network **30** and may also transmit or receive medical images captured by another medical apparatus, e.g., a computed tomography (CT) apparatus, a magnetic resonance imaging (MRI) apparatus, or an X-ray apparatus. Furthermore, the communication module **1300** may receive information about a diagnosis history or medical treatment schedule of a patient from a server and utilizes the received information to diagnose the patient. Furthermore, the communication module **1300** may perform data communication not only with a server or a medical apparatus in a hospital, but also with a portable terminal of a medical doctor or patient.

[0167] The communication module **1300** is connected to the network **30** by wire or wirelessly to exchange data with a server **32**, a medical apparatus **34**, or a portable terminal **36**. The communication module **1300** may include one or more components for communication with external devices. For example, the communication module **1300** may include a local area communication module **1310**, a wired communication module **1320**, and a mobile communication module **1330**.

[0168] The local area communication module **1310** refers to a module for local area communication within a predetermined distance. Examples of local area communication techniques according to an embodiment may include, but are not limited to, wireless LAN, Wi-Fi, Bluetooth, ZigBee, Wi-Fi Direct (WFD), ultra wideband (UWB), infrared data association (IrDA), Bluetooth low energy (BLE), and near field communication (NFC).

[0169] The wired communication module **1320** refers to a module for communication using electric signals or optical signals. Examples of wired communication techniques according to an embodiment may include communication via a twisted pair cable, a coaxial cable, an optical fiber cable, and an Ethernet cable.

[0170] The mobile communication module **1330** transmits or receives wireless signals to or from at least one selected from a base station, an external terminal, and a server on a mobile communication network. The wireless signals may

be voice call signals, video call signals, or various types of data for transmission and reception of text/multimedia messages.

[0171] The memory **1500** stores various data processed by the ultrasound diagnosis apparatus **1000**. For example, the memory **1500** may store medical data related to diagnosis of an object, such as ultrasound data and an ultrasound image that are input or output, and may also store algorithms or programs which are to be executed in the ultrasound diagnosis apparatus **1000**.

[0172] The memory **1500** may be any of various storage media, e.g., a flash memory, a hard disk drive, EEPROM, etc. Furthermore, the ultrasound diagnosis apparatus **1000** may utilize web storage or a cloud server that performs the storage function of the memory **1500** online.

[0173] The input device **1600** refers to a means via which a user inputs data for controlling the ultrasound diagnosis apparatus **1000**. The input device **1600** may include hardware components, such as a keypad, a mouse, a touch pad, a touch screen, and a jog switch. However, embodiments are not limited thereto, and the input device **1600** may further include any of various other input units including an electrocardiogram (ECG) measuring module, a respiration measuring module, a voice recognition sensor, a gesture recognition sensor, a fingerprint recognition sensor, an iris recognition sensor, a depth sensor, a distance sensor, etc.

[0174] The controller **1700** may control all operations of the ultrasound diagnosis apparatus **1000**. In other words, the controller **1700** may control operations among the probe **20**, the ultrasound transceiver **1100**, the image processor **1200**, the communication module **1300**, the display **1400**, the memory **1500**, and the input device **1600** shown in FIG. 13.

[0175] All or some of the probe **20**, the ultrasound transceiver **1100**, the image processor **1200**, the communication module **1300**, the display **1400**, the memory **1500**, the input device **1600**, and the controller **1700** may be implemented as software modules. Furthermore, at least one selected from the ultrasound transceiver **1100**, the image processor **1200**, and the communication module **1300** may be included in the controller **1700**. However, embodiments of the present invention are not limited thereto.

[0176] FIG. 14 is a block diagram showing a configuration of a wireless probe **2000** according to an embodiment. As described above with reference to FIG. 13, the wireless probe **2000** may include a plurality of transducers, and, according to embodiments, may include some or all of the components of the ultrasound transceiver **2100** shown in FIG. 13.

[0177] The wireless probe **2000** according to the embodiment shown in FIG. 2 includes a transmitter **2100**, a transducer **2200**, and a receiver **2300**. Since descriptions thereof are given above with reference to FIG. 13, detailed descriptions thereof will be omitted here. In addition, according to embodiments, the wireless probe **2000** may selectively include a reception delaying unit **2330** and a summing unit **2340**.

[0178] The wireless probe **2000** may transmit ultrasound signals to the object **10**, receive echo signals from the object **10**, generate ultrasound data, and wirelessly transmit the ultrasound data to the ultrasound diagnosis apparatus **1000** shown in FIG. 13.

[0179] The above-described embodiments of the present disclosure may be written as computer programs and may be

implemented in general-use digital computers that execute the programs using a non-transitory computer-readable recording medium.

[0180] Examples of the non-transitory computer-readable recording medium include magnetic storage media (e.g., ROM, floppy disks, hard disks, etc.), optical recording media (e.g., CD-ROMs, or DVDs), etc), and transmission media such as Internet transmission media.

[0181] It should be understood that embodiments described herein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each embodiment should typically be considered as available for other similar features or aspects in other embodiments.

[0182] While the present disclosure has been particularly shown and described with reference to exemplary embodiments thereof, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope as defined by the following claims. Accordingly, the above embodiments and all aspects thereof are examples only and are not limiting.

What is claimed is:

1. A method, performed by an ultrasound imaging apparatus, of displaying an ultrasound image with respect to an object comprising a blood vessel, the method comprising:

obtaining three-dimensional (3D) ultrasound volume data with respect to the object;

analyzing a degree of stenosis for a plurality of cross-sections of the blood vessel from the 3D ultrasound volume data and determining a stenosis cross-section with a highest degree of stenosis;

determining a first cross-section and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among the plurality of cross-sections of the blood vessel; and

displaying at least two cross-sections of the stenosis cross-section, the first cross-section, the second cross-section, and at least two stenosis index values showing a degree of stenosis of the blood vessel on a display unit of the ultrasound imaging apparatus.

2. The ultrasound imaging method of claim 1, wherein the displaying of at least two stenosis index values comprises displaying at least two index values from among a first index value representing a ratio of a diameter of the first cross-section to a difference between the diameter of the first cross-section and a diameter of the stenosis cross-section, a second index value representing a ratio of an entire blood vessel diameter defined by a blood vessel wall of the stenosis cross-section to a difference between the entire blood vessel diameter and the diameter of the stenosis cross-section, a third index value representing a ratio of a diameter of the second cross-section to a difference between the diameter of the second cross-section and the diameter of the stenosis cross-section, and a fourth index value representing a ratio of a cross-sectional area of the entire blood vessel of the stenosis cross-section to an area of the stenosis cross-section.

3. The ultrasound imaging method of claim 1, wherein the blood vessel is a carotid artery, the first cross-section is a cross-section of an internal carotid artery (ICA), and the second cross-section is a cross-section of a common carotid artery (CCA).

4. The ultrasound imaging method of claim 1, further comprising rendering the 3D ultrasound volume data to generate a 3D ultrasound image of the object, wherein the displaying of the at least two cross-sections and the at least two stenosis index values comprises displaying the at least two cross-sections, the at least two stenosis index values, and the 3D ultrasound image on the display unit.

5. The ultrasound imaging method of claim 1, wherein the displaying of the at least two cross-sections and the at least two stenosis index values comprises displaying a user interface that displays at least one of different colors, graphs, and figures based on sizes of the at least two stenosis index values, along with the at least two stenosis index values.

6. The ultrasound imaging method of claim 1, wherein the obtaining of the 3D ultrasound volume data with respect to the object comprises:

transmitting ultrasound signals to the object;

receiving ultrasound echo signals reflected by the object; and

obtaining the 3D ultrasound volume data from the received ultrasound echo signals.

7. The ultrasound imaging method of claim 1, wherein the determining of the stenosis cross-section comprises:

obtaining the plurality of cross-sections of the blood vessel by segmenting the 3D ultrasound volume data at predetermined intervals;

calculating, with respect to each of the plurality of cross-sections of the blood vessel, a first area value regarding a cross-section defined by a blood vessel wall of the blood vessel and a second area value regarding a cross-section through which blood flows in the blood vessel;

calculating, with respect to each of the plurality of cross-sections of the blood vessel, a ratio of the first area value to the second area value; and

determining a cross-section having a smallest calculated ratio as a stenosis cross-section from among the plurality of cross-sections of the blood vessel.

8. The ultrasound imaging method of claim 7, wherein the calculating of the second area value comprises:

obtaining a brightness value for each of the plurality of cross-sections of the blood vessel;

determining an area of a region whose obtained brightness value is less than a predetermined brightness value as a second area; and

calculating an area value of the second area.

9. The ultrasound imaging method of claim 1, wherein the first cross-section is spaced apart by a predetermined first interval in a first direction from the stenosis cross-section and the second cross-section is spaced apart by the first interval in a second direction that is opposite to the first direction from the stenosis cross-section.

10. The ultrasound imaging method of claim 1, wherein the determining of the first cross-section and the second cross-section comprises receiving a user input for setting a second interval that is spaced apart from the stenosis cross-section,

wherein the first cross-section is spaced apart by the second interval in a first direction from the stenosis cross-section and the second cross-section is spaced apart by the second interval in a second direction that is opposite to the first direction from the stenosis cross-section.

11. The ultrasound imaging method of claim 1, wherein the determining of the first cross-section and the second cross-section comprises:

detecting from the 3D ultrasound volume data a branch point where the blood vessel diverges into two; and determining a cross-section spaced apart by a third interval in a first direction from the branch point as the first cross-section and determining a cross-section spaced apart by the third interval in a second direction that is opposite to the first direction from the branch point as the second cross-section.

12. An ultrasound imaging apparatus displaying an ultrasound image with respect to an object comprising a blood vessel, the ultrasound imaging apparatus comprising:

an ultrasound data acquisition unit configured to obtain 3D ultrasound volume data with respect to the object; a processor configured to analyze a degree of stenosis for a plurality of cross-sections of the blood vessel from the 3D ultrasound volume data, determine a stenosis cross-section with a highest degree of stenosis and determine a first cross-section and a second cross-section that are spaced apart from each other in different directions from the stenosis cross-section from among the plurality of cross-sections of the blood vessel; and

a display unit configured to display at least two cross-sections of the stenosis cross-section, the first cross-section, the second cross-section, and at least two stenosis index values showing a degree of stenosis of the blood vessel.

13. The ultrasound imaging apparatus of claim 12, wherein the processor is further configured to calculate at least two index values from among a first index value representing a ratio of a diameter of the first cross-section to a difference between the diameter of the first cross-section and a diameter of the stenosis cross-section, a second index value representing a ratio of an entire blood vessel diameter defined by a blood vessel wall of the stenosis cross-section to a difference between the entire blood vessel diameter and the diameter of the stenosis cross-section, a third index value representing a ratio of a diameter of the second cross-section to a difference between the diameter of the second cross-section and the diameter of the stenosis cross-section, and a fourth index value representing a ratio of a cross-sectional area of the entire blood vessel of the stenosis cross-section to an area of the stenosis cross-section, and the display unit is further configured to display at least two index values from among the first index value, the second index value, the third index value, and the fourth index value.

14. The ultrasound imaging apparatus of claim 12, wherein the blood vessel is a carotid artery, the first cross-section is a cross-section of an ICA, and the second cross-section is a cross-section of a CCA.

15. The ultrasound imaging apparatus of claim 12, wherein

the processor is further configured to render the 3D ultrasound volume data to generate a 3D ultrasound image of the object; and

the display unit is further configured to display the at least two cross-sections, the at least two stenosis index values, and the 3D ultrasound image on the display unit.

16. The ultrasound imaging apparatus of claim 12, wherein the display unit is further configured to display a user interface that displays at least one of different colors, graphs, and figures based on sizes of the at least two stenosis index values, along with the at least two stenosis index values.

17. The ultrasound imaging apparatus of claim 12, wherein the ultrasound data acquisition unit is further configured to transmit ultrasound signals to the object, receive ultrasound echo signals reflected by the object, and obtain the 3D ultrasound volume data from the received ultrasound echo signals.

18. The ultrasound imaging apparatus of claim 12, wherein the processor is further configured to obtain the plurality of cross-sections of the blood vessel by segmenting the 3D ultrasound volume data at predetermined intervals, calculate, with respect to each of the plurality of cross-sections of the blood vessel, a first area value regarding a cross-section defined by a blood vessel wall of the blood vessel and a second area value regarding a cross-section through which blood flows in the blood vessel, calculate, with respect to each of the plurality of cross-sections of the blood vessel, a ratio of the first area value to the second area value, and determine a cross-section having a smallest calculated ratio as a stenosis cross-section from among the plurality of cross-sections of the blood vessel.

19. The ultrasound imaging apparatus of claim 18, wherein the processor is further configured to obtain a brightness value for each of the plurality of cross-sections of the blood vessel, determine an area of a region whose obtained brightness value is less than a predetermined brightness value as a second area, and calculate an area value of the second area.

20. The ultrasound imaging apparatus of claim 12, wherein the first cross-section is spaced apart by a predetermined first interval in a first direction from the stenosis cross-section and the second cross-section is spaced apart by the first interval in a second direction that is opposite to the first direction from the stenosis cross-section.

21. The ultrasound imaging apparatus of claim 12, further comprising a user input unit configured to receive a user input for setting a second interval that is spaced apart from the stenosis cross-section,

wherein the processor is further configured to determine the first cross-section spaced apart by the second interval in a first direction from the stenosis cross-section and the second cross-section spaced apart by the second interval in a second direction that is opposite to the first direction from the stenosis cross-section.

22. The ultrasound imaging apparatus of claim 12, wherein the processor is further configured to detect from the 3D ultrasound volume data a branch point where the blood vessel diverges into two, determines a cross-section spaced apart by a third interval in a first direction from the branch point as the first cross-section, and determine a cross-section spaced apart by the third interval in a second direction that is opposite to the first direction from the branch point as the second cross-section.

23. A non-transitory computer-readable recording medium having recorded thereon a program for executing the method of claim 1 on a computer.

* * * * *

专利名称(译)	用于显示超声图像的方法和设备		
公开(公告)号	US20170215838A1	公开(公告)日	2017-08-03
申请号	US15/258421	申请日	2016-09-07
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	PARK JIN KI PARK SUNG WOOK LEE JIN YONG		
发明人	PARK, JIN-KI PARK, SUNG-WOOK LEE, JIN-YONG		
IPC分类号	A61B8/08 A61B8/00		
CPC分类号	A61B8/0891 A61B8/463 A61B8/5246 A61B8/483 A61B8/466 A61B8/145 A61B8/5207 A61B8/5223		
优先权	1020160012456 2016-02-01 KR		
外部链接	Espacenet USPTO		

摘要(译)

提供了用于显示超声图像的方法和设备。根据一个或多个实施例的用于显示超声图像的方法和装置可以确定关于包括血管的对象的超声数据的狭窄横截面，并且显示与血管狭窄和狭窄相关的至少两个横截面。表示血管狭窄程度的指标值，从而提高了用户的诊断可用性。

