



US006524252B1

(12) **United States Patent**
Yu et al.

(10) **Patent No.:** **US 6,524,252 B1**
(b4) **Date of Patent:** **Feb. 25, 2003**

(54) **METHOD AND SYSTEM FOR GENERATING ULTRASOUND FRAMES WITH DECORRELATED SPECKLE PATTERNS AND GENERATING A COMPOUND ULTRASOUND IMAGE THEREFROM**

(75) Inventors: **Zengpin Yu**, Palo Alto, CA (US); **Danhua Zhao**, Milpitas, CA (US); **Shengtz Lin**, Cupertino, CA (US); **Feng Yin**, Palo Alto, CA (US)

(73) Assignee: **U-Systems, Inc.**, Los Altos, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 28 days.

(21) Appl. No.: **09/721,889**

(22) Filed: **Nov. 24, 2000**

(51) Int. Cl.⁷ **A61B 8/00**

(52) U.S. Cl. **600/443**

(58) Field of Search 600/437, 440-447, 600/458; 128/916

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,887,306 A	12/1989	Hwang et al.	
5,353,354 A	10/1994	Keller et al.	
5,632,277 A	5/1997	Chapman et al.	
5,653,235 A	* 8/1997	Teo	600/447
5,709,209 A	1/1998	Friemel et al.	
5,782,766 A	7/1998	Weng et al.	
5,924,991 A	* 7/1999	Hossack et al.	128/916
5,928,151 A	* 7/1999	Hossack et al.	128/916
5,957,852 A	* 9/1999	Hossack et al.	600/458
6,110,115 A	* 8/2000	Ustuner et al.	600/443
6,117,081 A	9/2000	Jago et al.	
6,126,598 A	10/2000	Entrekkin et al.	
6,126,599 A	10/2000	Jago et al.	
6,135,956 A	10/2000	Schmiesing et al.	
6,193,663 B1	* 2/2001	Napolitano et al.	600/447
6,358,209 B1	* 3/2002	Ustuner et al.	600/443

OTHER PUBLICATIONS

U.S. Application Serial No. 09/224,635, filed Dec. 31, 1998.
U.S. Application Serial No. 09/449,095, filed Nov. 24, 1999.

* cited by examiner

Primary Examiner—Marvin M. Lateef


Assistant Examiner—Ali M. Imam

(74) Attorney, Agent, or Firm—Cooper & Dunham LLP

(57) **ABSTRACT**

An ultrasound system that generates compound images from component frames having decorrelated speckle patterns. Successive sets of distinct, speckle-affecting parameters are used to generate successive component frames for compounding, and are selected such that the successive component frames have decorrelated speckle patterns. The speckle-affecting parameters that are changed from frame to frame may be selected from a wide variety of parameters, including transmit beamformer parameters, receive beamformer parameters, and demodulator parameters. According to a preferred embodiment, the successive sets of speckle-affecting parameters differ from each other by at least two speckle-affecting parameters. According to another preferred embodiment, the amount by which each of the multiple speckle-affecting parameters is changed is less than a decorrelation threshold for that parameter, that is, by less than the amount that speckle-affecting parameter alone would be required to change in order to yield decorrelated speckle patterns if no other parameters were changed. When more speckle-affecting parameters are changed, each speckle-affecting parameter can be changed by an amount less than its decorrelation threshold, and yet decorrelated speckle patterns can still be obtained. Moreover, because two different types of speckle-affecting parameters tend to alter the spatial resolution of the component frames in different ways, the spatial resolution of the compounded image can be better as compared to the scenario in which only one speckle-affecting parameter is altered by its decorrelation threshold.

20 Claims, 6 Drawing Sheets

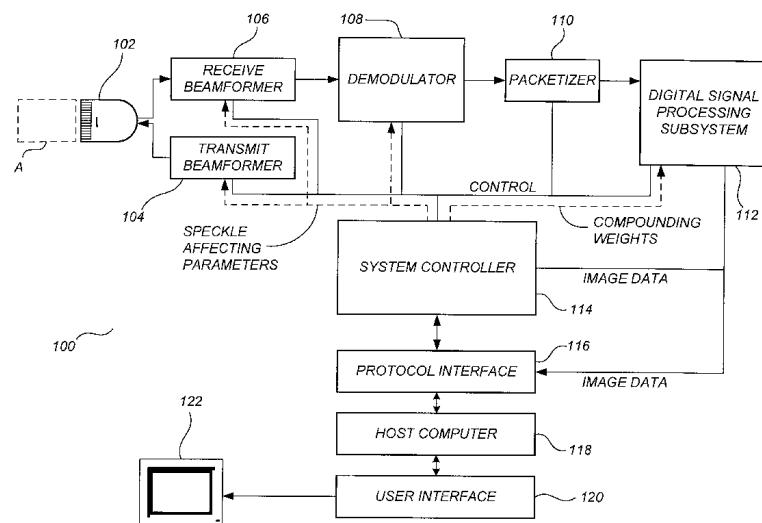

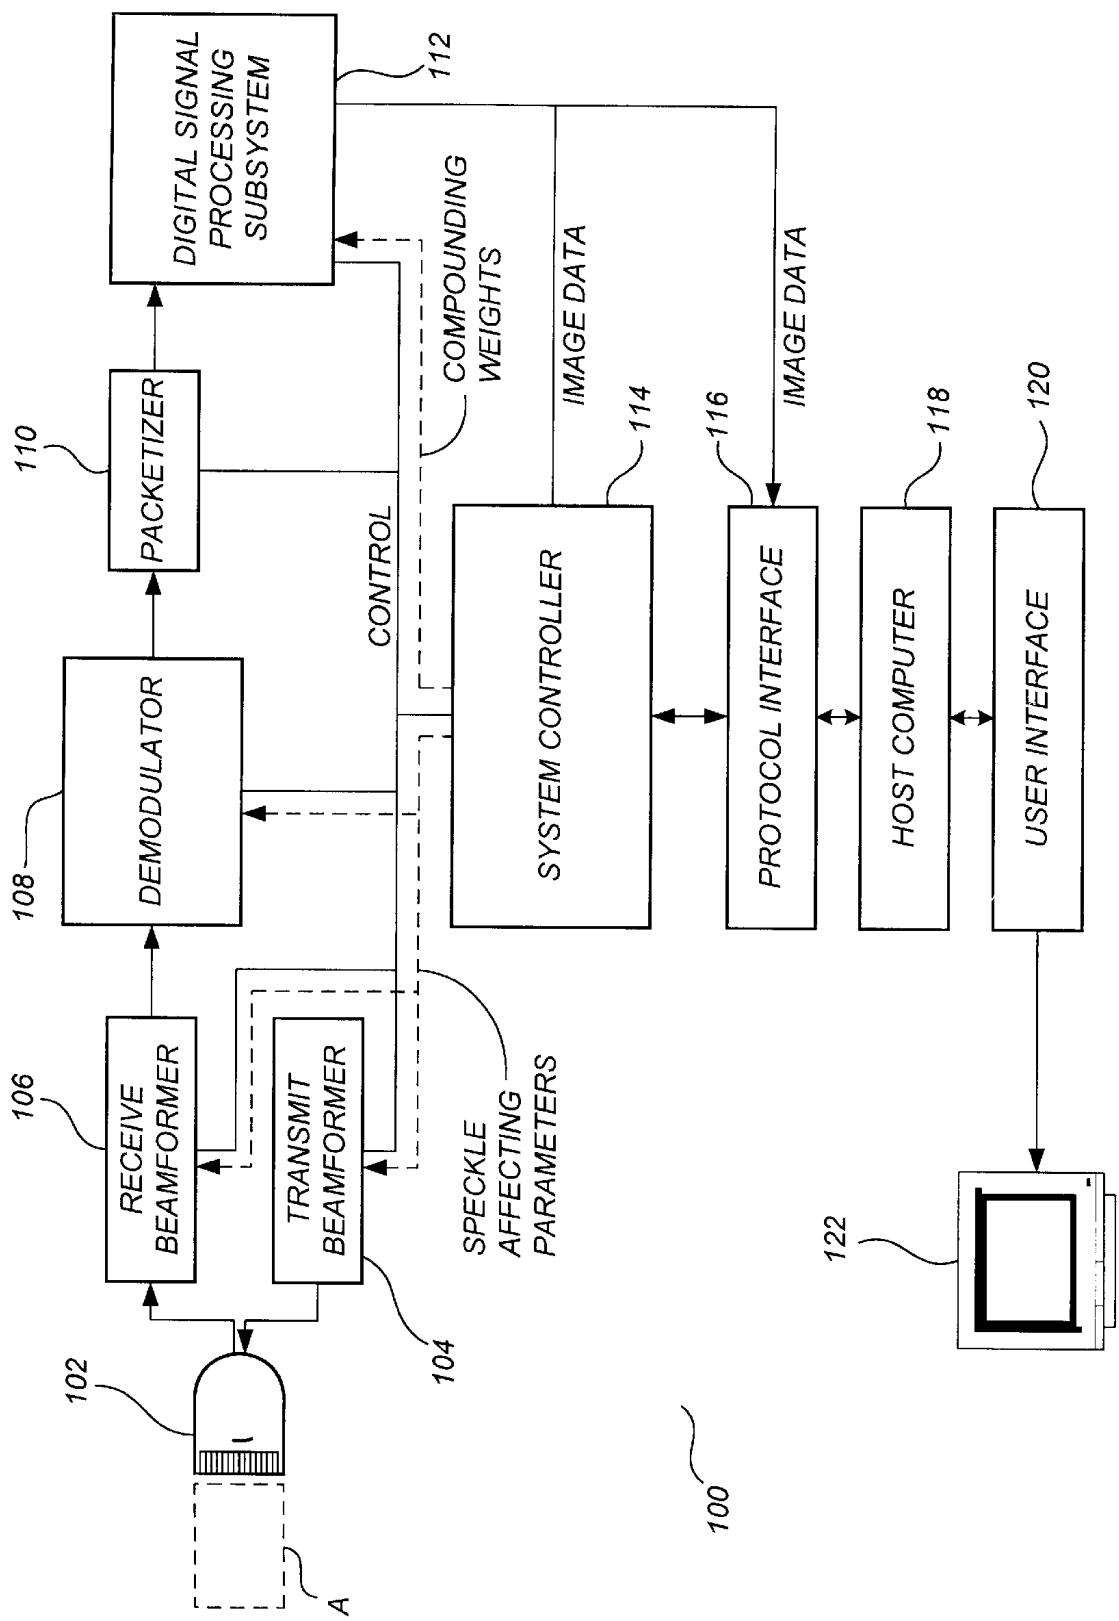


FIG. 1

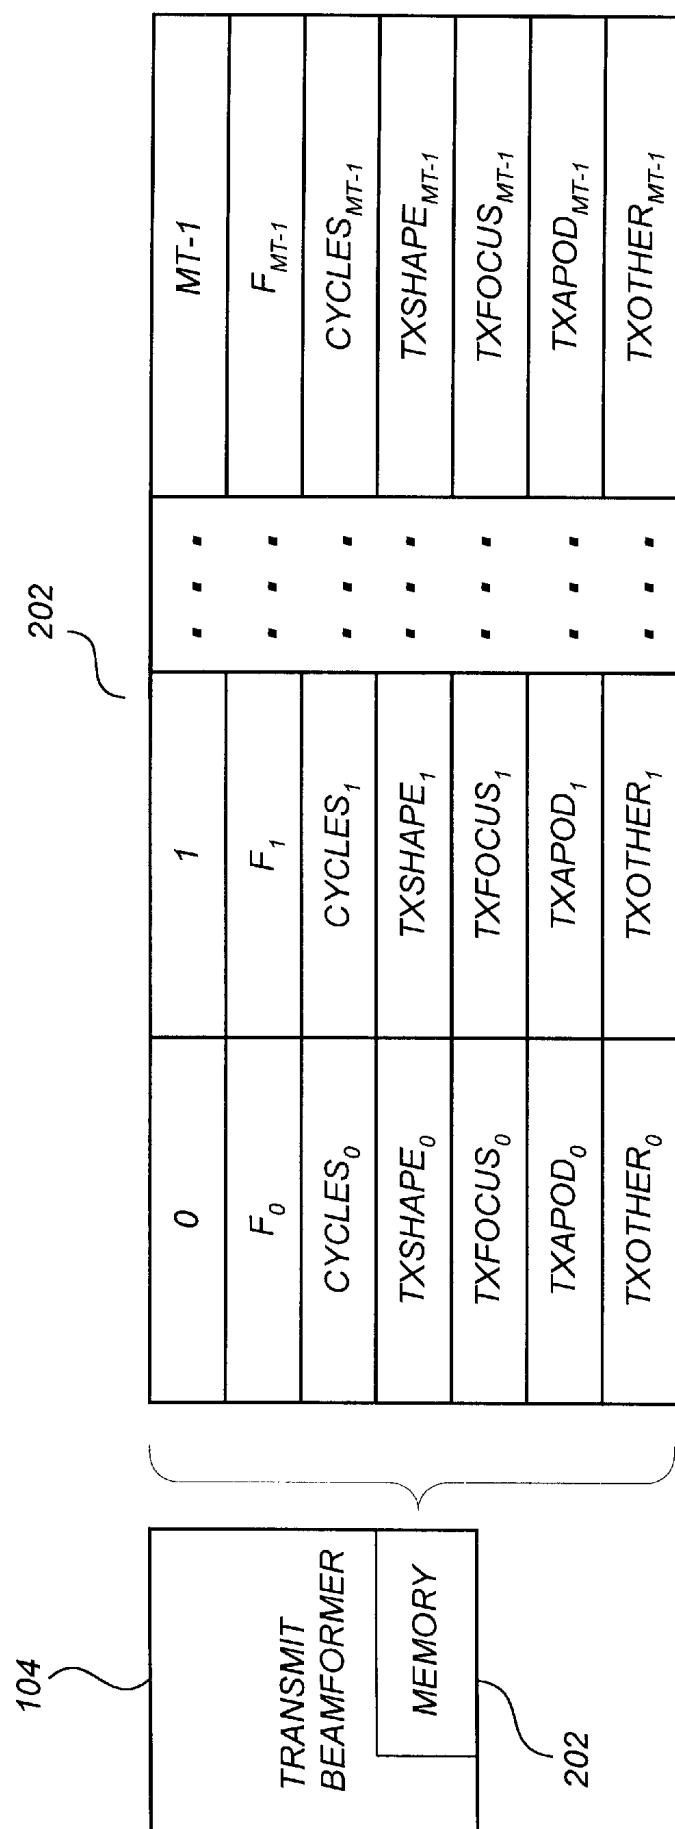


FIG. 2

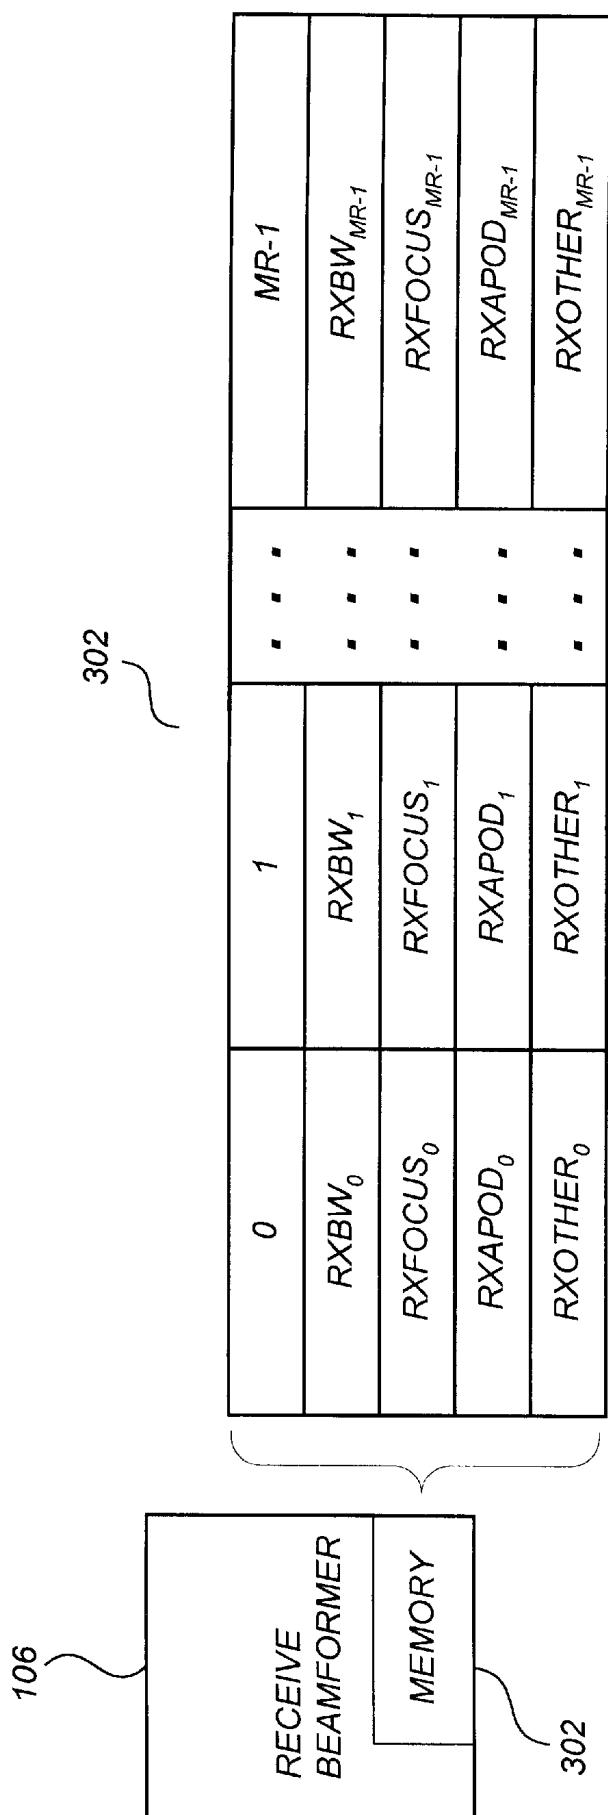


FIG. 3

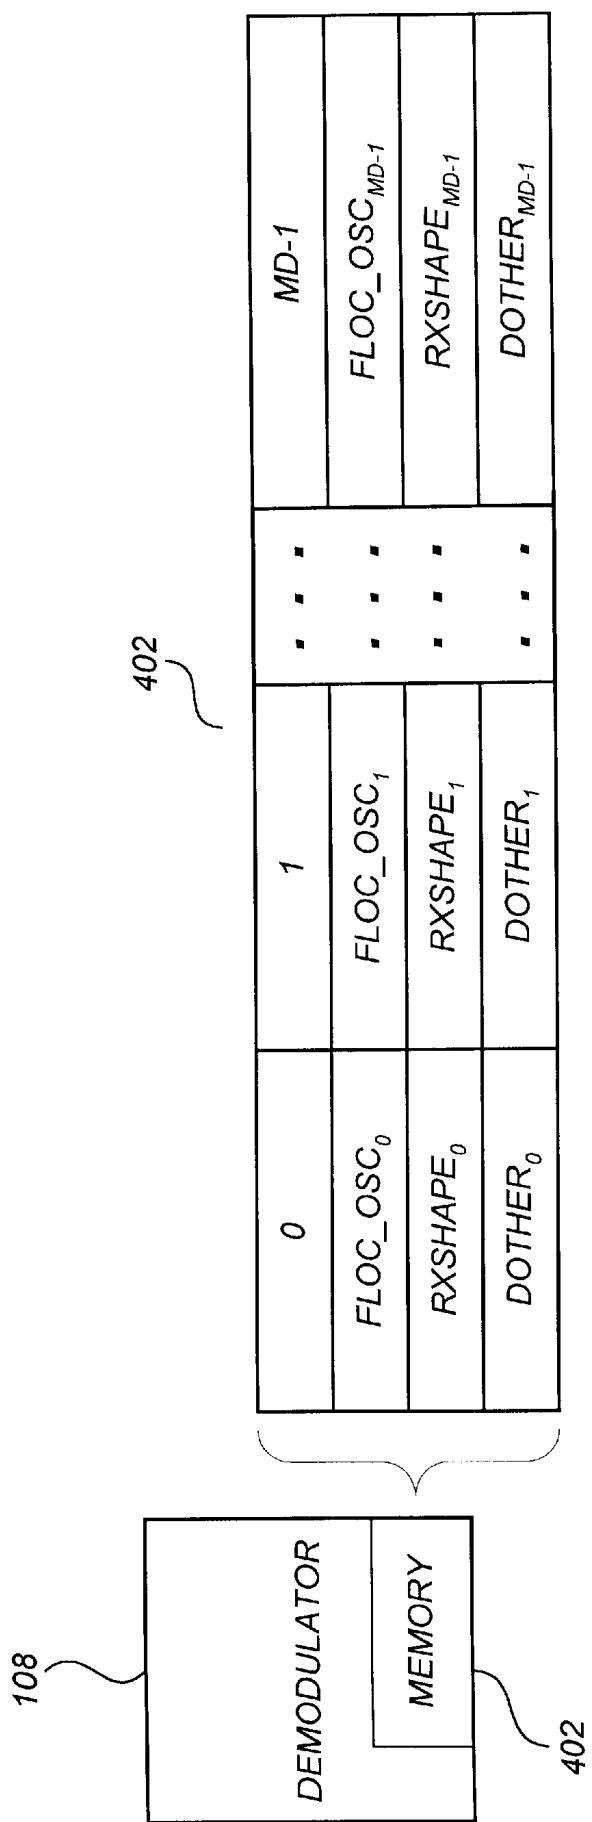


FIG. 4

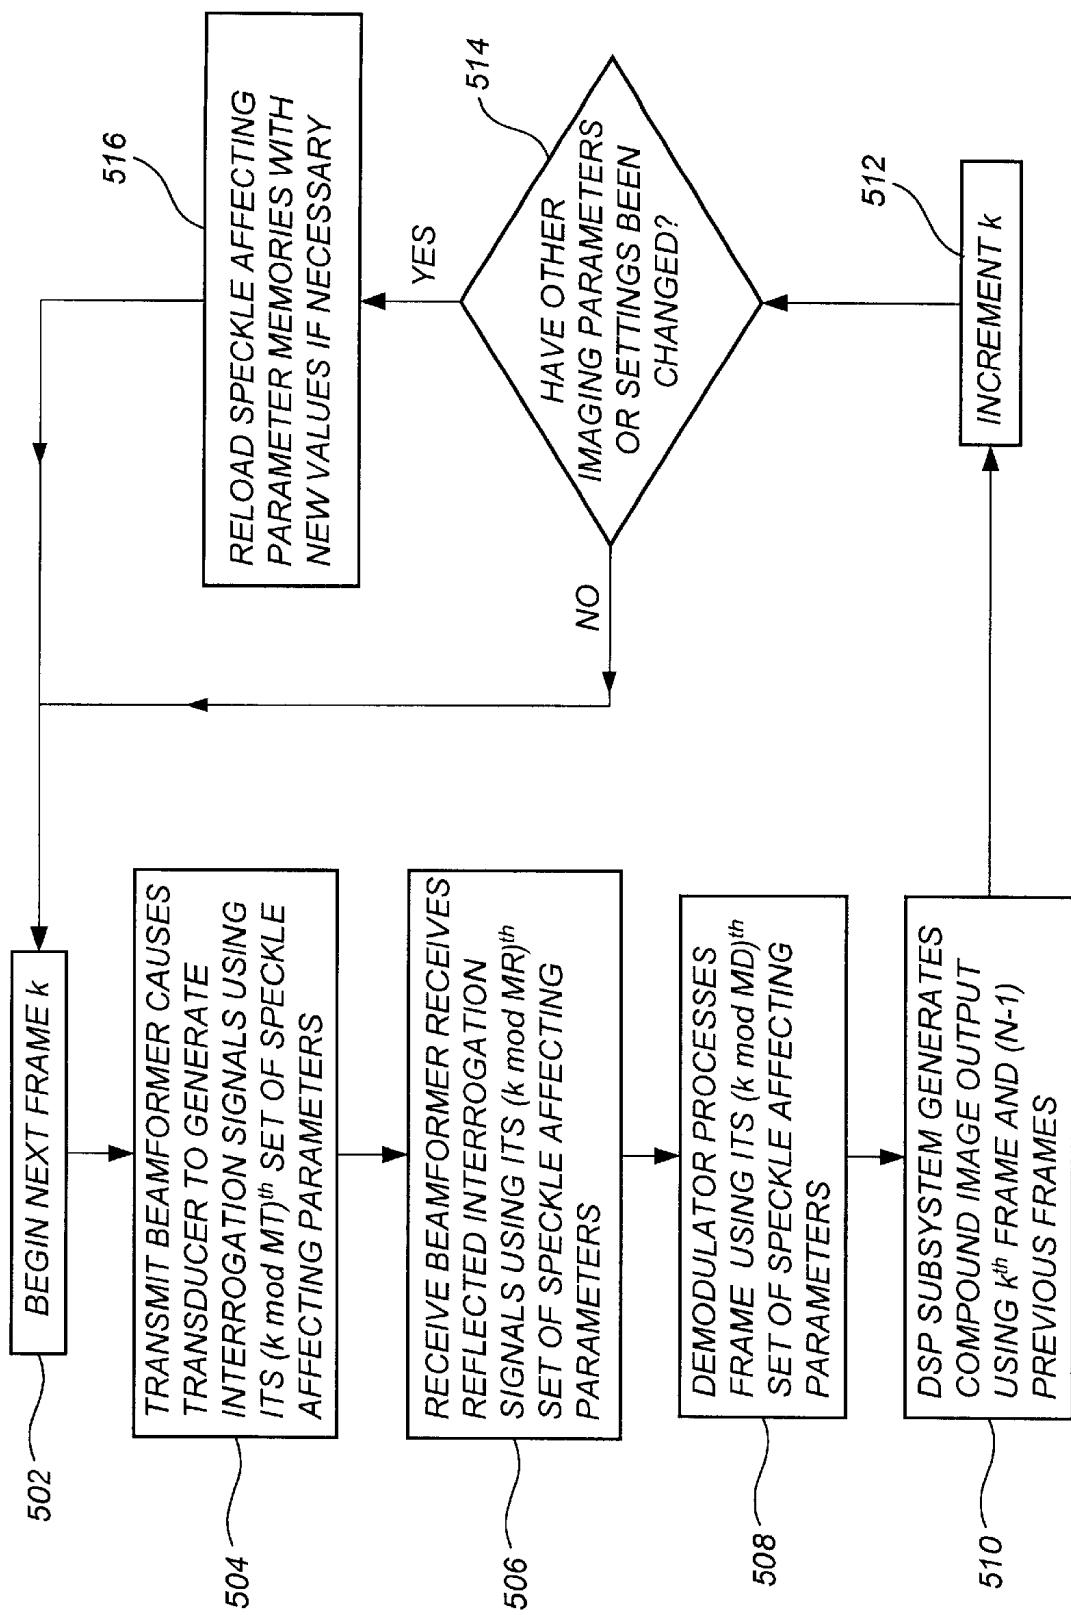


FIG. 5

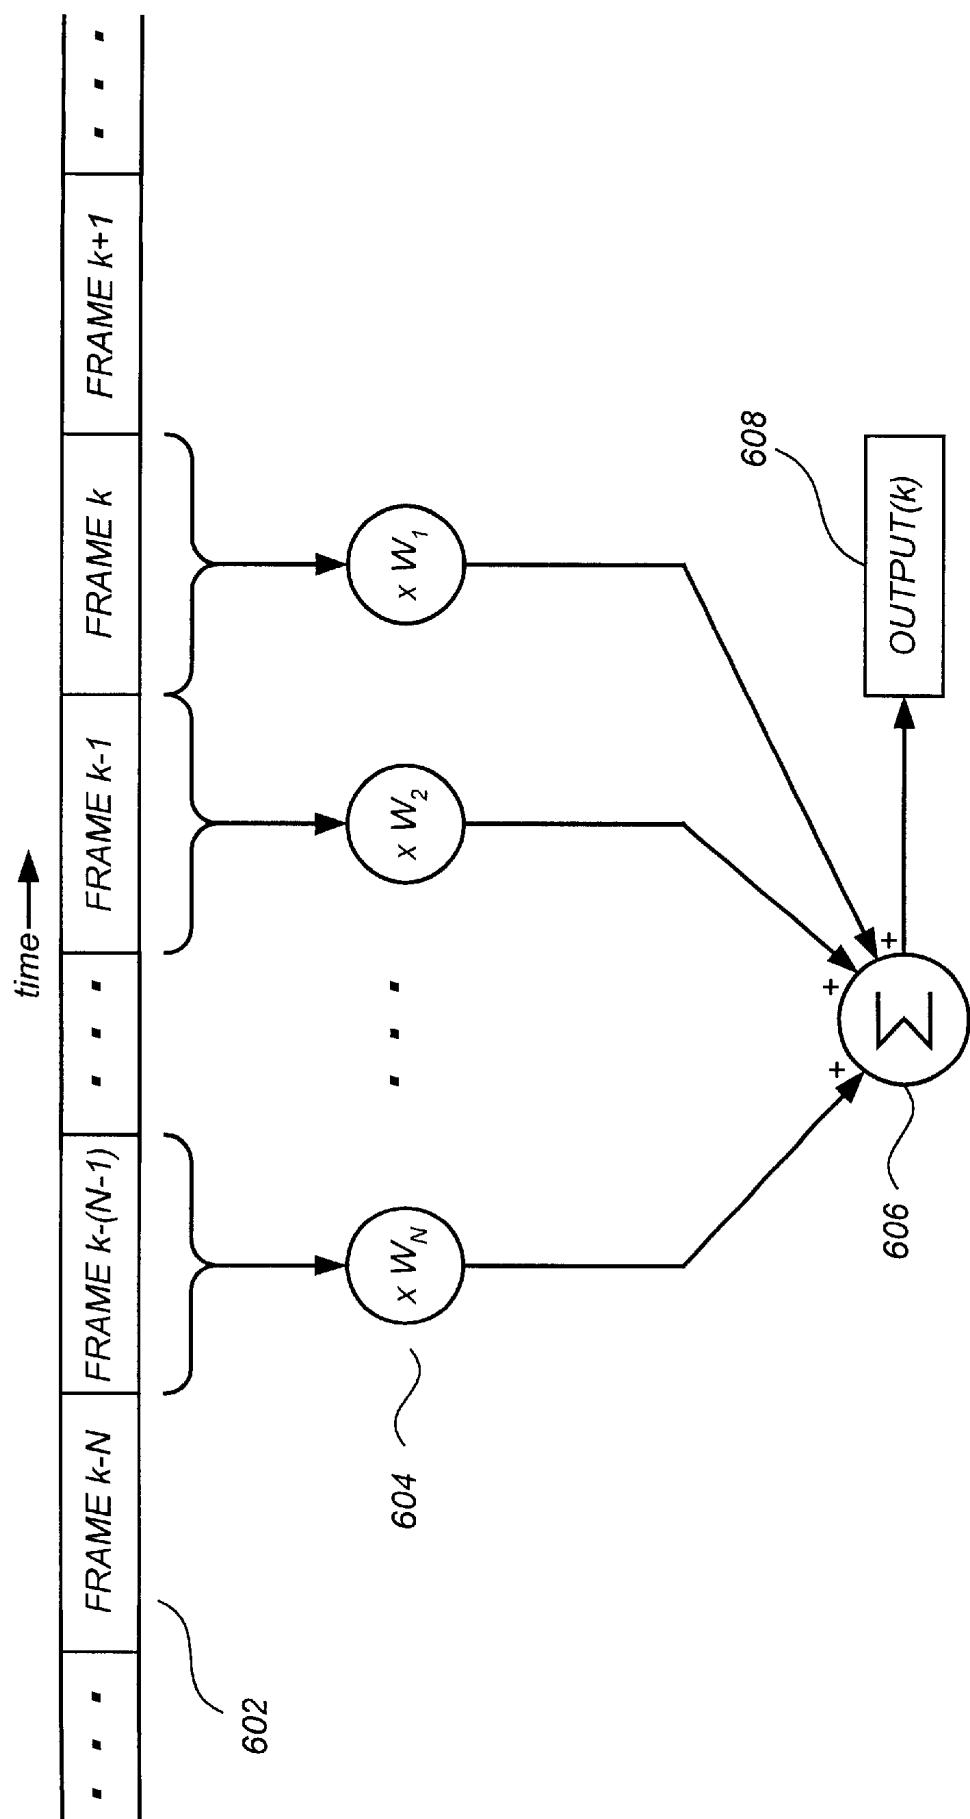


FIG. 6

**METHOD AND SYSTEM FOR GENERATING
ULTRASOUND FRAMES WITH
DECORRELATED SPECKLE PATTERNS AND
GENERATING A COMPOUND ULTRASOUND
IMAGE THEREFROM**

FIELD

This patent specification relates to the field of ultrasound information processing systems. In particular, it relates to a method and system for generating ultrasound frames having decorrelated speckle patterns and generating compound ultrasound images therefrom.

BACKGROUND

Ultrasound imaging systems have become increasingly popular for use in medical diagnosis because they are non-invasive, easy to use, capable of real-time operation, and do not subject patients to the dangers of electromagnetic radiation. Instead of electromagnetic radiation, an ultrasound imaging system transmits sound waves of very high frequency (e.g., 1 MHz to 15 MHz) into the patient and processes echoes scattered from structures in the patient's body to derive and display information relating to these structures.

One factor that currently limits the output quality of ultrasound imaging systems is the phenomenon of speckle. Speckle arises from the use of coherent signals to acoustically interrogate a target. Complex interference patterns arise from phase variations in the coherent signals as they propagate through, and reflect from, the many large and small acoustic reflectivity boundaries in the target. These phase variations may be caused by diffuse scatterers, by multiple scattering, by a non-homogeneous propagation medium which distorts the phase of the received wave, or by other factors.

Speckle appears to the viewer like random noise superimposed on the output image, and degrades the contrast resolution of the image (i.e., the accurate portrayal of the acoustic reflectivity of respective target locations). A speckle pattern will change in a visually recognizable (although complex) way upon a small displacement or rotation of the ultrasound transducer relative to the target, or upon small movements of the target tissue.

One common approach to reducing speckle involves image compounding, i.e., the combining of multiple component frames into an output image, the component frames having decorrelated, or at least partially decorrelated, speckle patterns. Most generally, decorrelation of the speckle patterns relates to how similar they are, or the degree to which their grainy structures appear to be derived from one another. As applied to image compounding, decorrelation of the speckle patterns relates to the degree to which compounding would reduce the speckle effects. Thus, for example, the compounding of two entirely correlated speckle patterns would cause little reduction in the amount of speckle. However, as the decorrelation of the speckle patterns is increased, compounding the patterns would result in speckle reduction, up to a maximum value when the two patterns became entirely decorrelated. It can be shown that, where direct frame averaging is used, this maximum value for speckle reduction is $\sqrt{2}$, or more generally \sqrt{N} for N component frames. Mathematically, decorrelation of the two speckle patterns can be expressed by a measure such as a correlation coefficient, wherein a correlation coefficient of 1.0 corresponds to entirely correlated speckle patterns and a

correlation coefficient of 0.0 corresponds to entirely decorrelated, speckle patterns.

Spatial compounding refers to the compounding of frame data from different sub-apertures and/or angular viewpoints for a given target location. Examples of spatial compounding from different angular viewpoints ("look angles") can be found in U.S. Pat. No. 6,117,081 (Jago et. al.), U.S. Pat. No. 6,126,598 (Entrekkin et. al.), U.S. Pat. No. 6,126,599 (Jago et. al.), and U.S. Pat. No. 6,135,956 (Schmiesing et. al.), which are incorporated by reference herein. There is a trade-off between speckle reduction and spatial resolution in such systems. For example, when using different sub-apertures, it is generally required that the relative translation of the sub-apertures be more than one-half the size of the sub-apertures to yield decorrelated speckle patterns. However, if more sub-apertures were formed to achieve this spacing, there would be a corresponding decrease in the spatial resolution of each component frame as the size of each aperture is decreased. Alternatively, if panoramic or extended view imaging is used to achieve a speckle reduction effect, image registration errors substantially reduce the spatial resolution.

Similar disadvantages are incurred in angular compounding systems such as those listed above, in which frames are taken from different "look angles" and compounded. As described therein, it is required that the "look angles" of the component frames be at least several degrees apart to achieve sufficiently decorrelated speckle patterns. However, as the angular separation of the "look angles" increases, there are beam steering and registration errors that reduce spatial resolution, as well as effective aperture reductions that reduce spatial resolution. Moreover, these errors get worse as the angles deviate further from the normal to the transducer, because small beam steering errors take on increased significance at these angles. Finally, these angular compounding systems suffer from grating lobes due to aliasing effects.

Frequency compounding is accomplished by dividing the bandwidth of the imaging system into multiple bands, and then processing and compounding signals from the different frequency bands. There is a trade-off between axial resolution and speckle reduction in these systems. For increased speckle reduction, it is desirable that the frequency bands of the interrogating pulses have lesser overlap in the frequency domain. However, to achieve this lesser overlap, the bandwidth of the interrogating pulses needs to be narrower, which corresponds to increased pulse length in the time domain and therefore reduced axial resolution. Frequency compounding also causes lateral resolution degradation due to contributions from the lower frequency component, thereby further decreasing spatial resolution.

Temporal compounding involves averaging successive frames together into a compound image. Because only one acoustic pulse can be sent into the target at a time, the above spatial compounding and frequency compounding techniques inherently involve temporal compounding as well. In theory, "pure" temporal compounding—in which no locations, angles, or frequencies are changed between frames—may not reduce speckle at all because the speckle pattern should not change between frames. In practice, however, many tissues and scattering structures incur a small amount of movement between component frames (e.g., through respiratory movements, gastric movements, small muscle movements, etc.) such that speckle patterns can change continually between component frames. Because no transducer movement, angle changes, or frequency changes are incurred between component frames, "pure" temporal compounding involves little or no loss of spatial resolution.

However, spatial compounding, frequency compounding, and temporal compounding each involve an additional trade-off between speckle reduction and temporal resolution, i.e., the ability to “keep up” with moving tissue and/or a moving transducer. As more frames “N” are compounded to reduce speckle, the output image becomes increasingly blurry for locations of relative movement between the transducer and the target tissue, and/or the output frame rate is decreased.

Proposals have been made for dealing with the undesirable tradeoffs between speckle reduction and spatial and/or temporal resolution. For example, the '598 patent supra proposes a dynamic trade off between the blurring effect and the speckle effect, wherein the number of spatially compounded frames “N” is automatically reduced during fast tissue or transducer motion. The '081 patent supra proposes a substitute tradeoff, one between the blurring effect and the frame rate, wherein the “N” frames being compounded are first corrected for misregistration prior to compounding, albeit causing a concomitant reduction in output frame rate, and calling for a substantial increase in processing power and system complexity.

However, it is believed that these and other such proposals can be seen as representing “patches” for fundamental shortcomings in the current ways that speckle is dealt with. In accordance with the preferred embodiments, it is believed that speckle effects can be more effectively reduced by systematically dealing with the many parameters that affect the speckle patterns themselves.

Accordingly, it would be desirable to provide an ultrasound imaging system that provides for reduced speckle while reducing the degradation in spatial resolution associated with image compounding.

It would be further desirable to provide an ultrasound imaging system that provides for reduced speckle while reducing the degradation in temporal resolution associated with image compounding.

It would be further desirable to provide an ultrasound imaging system that provides for reduced speckle that does not substantially increase the complexity of conventional image-compounding ultrasound systems.

SUMMARY

In accordance with a preferred embodiment, an ultrasound system that generates compound images from component frames having decorrelated speckle patterns is provided. Successive sets of distinct, speckle-affecting parameters are used to generate the successive component frames for compounding, and are selected such that the successive component frames have decorrelated speckle patterns. The speckle-affecting parameters that are changed from frame to frame can be selected from a wide variety of parameters, including transmit beamformer parameters, receive beamformer parameters, and demodulator parameters. The speckle-affecting parameters that are changed from frame to frame include, but are not limited to, transmit frequency, number of transmit cycles, number of transmit zones, transmit pulse shape, transmit focus profile, transmit focal point, transmit steering angle, transmit F-number, transmit focus algorithm identifier, transmit aperture setting, transmit apodization profile, receive bandwidth, receive focus profile, receive focal point, receive steering angle, receive F-number, receive focus algorithm identifier, receive aperture setting, receive apodization profile, local oscillator frequency, and receive pulse shape.

According to a preferred embodiment, the successive sets of speckle-affecting parameters differ from each other by at

least two speckle-affecting parameters for enhancing the decorrelation of the successive component frames, thereby providing for improved contrast resolution in the compounded image. According to another preferred embodiment, the amount by which each of the multiple speckle-affecting parameters is changed is less than a decorrelation threshold for that parameter. A decorrelation threshold relates to an amount that a speckle-affecting parameter alone would be required to change in order to yield decorrelated speckle patterns, if no other parameters were changed. It has been found that when more speckle-affecting parameters are changed, each speckle-affecting parameter can be changed by an amount less than its decorrelation threshold, and yet decorrelated speckle patterns can still be obtained. Moreover, because two different types of speckle-affecting parameters tend to alter the component frames in different ways, it has been found that the spatial resolution of the compounded image can be better as compared to the scenario in which only one speckle-affecting parameter is altered by its decorrelation threshold.

In one example of the above preferred embodiment, a partial frequency compounding method and system is provided. According to a preferred method, the difference in transmit frequency between successive frames is only a partial fraction of the difference that would otherwise be required to establish speckle pattern decorrelation if only transmit frequency, and no other parameter, were changed. However, according to a preferred method, an additional speckle-affecting parameter is also changed between successive frames by an amount sufficient to yield decorrelated speckle patterns when changed in conjunction with the transmit frequency. Thus, as a conceptual example, if the transmit frequency would alone need to be changed from f_0 to $1.5f_0$ to establish decorrelated speckle patterns, then according to the preferred embodiments, the transmit frequency could be only changed from f_0 to $1.2f_0$ as long as the number of transmit cycles, for example, were changed from n_0 to $1.5n_0$ at the same time. Moreover, because the resulting component frames are changed in different ways by the transmit frequency change versus the transmit cycle change, the spatial resolution of the compounded result can be better than if only the transmit frequency were changed from f_0 to $1.5f_0$ between component frames.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 shows a block diagram of an ultrasound imaging system in accordance with a preferred embodiment;

FIG. 2 shows a transmit beamformer as adapted for use in the system of FIG. 1, along with an array of transmit beamformer speckle-affecting parameters in accordance with a preferred embodiment;

FIG. 3 shows a receive beamformer as adapted for use in the system of FIG. 1, along with an array of receive beamformer speckle-affecting parameters in accordance with a preferred embodiment;

FIG. 4 shows a demodulator as adapted for use in the system of FIG. 1, along with an array of demodulator speckle-affecting parameters in accordance with a preferred embodiment;

FIG. 5 shows overall steps carried out by the system of FIG. 1 in generating compound ultrasound images and managing speckle-affecting parameters in accordance with a preferred embodiment; and

FIG. 6 shows a conceptual diagram illustrating the creation of compound images using decorrelated component frames in accordance with a preferred embodiment.

DETAILED DESCRIPTION

FIG. 1 shows a block diagram of an ultrasound imaging system **100** in accordance with a preferred embodiment. Ultrasound imaging system **100** comprises a transducer **102**, a transmit beamformer **104**, a receive beamformer **106**, a demodulator **108**, a packetizer **110**, a digital signal processing (DSP) subsystem **112**, a system controller **114**, a protocol interface **116**, a host computer **118**, a user interface **120**, and a display **122**. Although many ultrasound system architectures may be readily adapted for use in accordance with the preferred embodiments, ultrasound imaging system **100** is preferably similar to the those described in the commonly assigned U.S. Ser. No. 09/224,635, filed Dec. 31, 1998, and U.S. Ser. No. 09/449,095 filed Nov. 24, 1999, which are incorporated herein by reference.

Transducer **102** comprises an array of transducer elements that transmits focused acoustic signals into a target responsive to signals generated by the transmit beamformer **104**. In a preferred embodiment, transducer **102** transmits acoustic pulses into an area A that is fixed relative to the transducer. It has been found that using methods of the preferred embodiments, the use of angular spatial compounding, in which component frames are taken at different angles relative to the transducer, can be avoided. In the preferred embodiment in which angular spatial compounding is avoided, several disadvantages associated with angular spatial compounding that degrade spatial resolution in the compound image are avoided. Nevertheless, it is possible to use angular spatial compounding methods in conjunction with the preferred embodiments for other reasons.

Responsive to control signals and parameters received from system controller **114**, transmit beamformer **104** generates signals that are converted into acoustic interrogation signals by transducer **102** and introduced into the target. Transducer **102** also receives acoustic echoes from the target and converts them into signals for forwarding to receive beamformer **106**. Receive beamformer **106** receives the signals and converts them into a single-channel RF signal. Demodulator **108** receives the single-channel RF signal and generates component frames therefrom, which are then packetized by packetizer **110** and fed to DSP subsystem **112**. In accordance with control signals and compounding weights received from system controller **114**, DSP subsystem **112** continuously generates compound output images by compounding "N" component frames at a time. The output image data is transferred to protocol interface **116**, but may optionally be further processed by system controller **114**. The compound output image frames are then transferred to host computer **118** which performs scan conversion on the signals for transmission to user interface **120** and ultimate display by display **122**.

The transmit beamformer **104**, receive beamformer **106**, and demodulator **108** perform their processing functions on successive component frames in accordance with a plurality of successive sets of speckle-affecting parameters. Speckle-affecting parameters relate to settings or other parameters used by the ultrasound system **100** which, if changed, would result in a change in the speckle pattern of the generated component frames. Speckle-affecting parameters are provided by system controller **114** to each of the transmit beamformer **104**, receive beamformer **106**, and demodulator **108** either dynamically or in a fixed predetermined sequence. It has been found that the alternating use of as few as two sets of speckle-affecting parameters between component frames, each differing by as little as two individual speckle-affecting parameters, may provide for an increased

quality output having increased spatial resolution as compared to a scenario in which only one individual speckle-affecting parameter is changed between component frames.

According to a preferred embodiment, the amount by which each of the multiple speckle-affecting parameters is changed is less than a decorrelation threshold for that parameter. A decorrelation threshold relates to an amount that a speckle-affecting parameter alone would be required to change in order to yield decorrelated speckle patterns, if no other parameters were changed. By way of nonlimiting conceptual example, in a system having an initial transmit frequency of f_0 , it may be found that the transmit frequency needs to be changed to at least $1.5f_0$ in order to yield decorrelated speckle patterns between the two resulting frames. In such case, the decorrelation threshold for the transmit frequency parameter at f_0 would be $0.5f_0$. Generally speaking, decorrelation thresholds for each of the many speckle-affecting parameters may be empirically determined by holding all other speckle-affecting parameters constant while varying that parameter, and evaluating whether the resulting component frames are sufficiently decorrelated. The decorrelation threshold for a given speckle-affecting parameter may also vary depending on the magnitude of that parameter. However, given the present disclosure, a person skilled in the art will be readily able to determine the relevant decorrelation thresholds for the speckle-affecting parameters of a given ultrasound system configuration.

In accordance with a preferred embodiment, when multiple speckle-affecting parameters are changed between component frames, each individual speckle-affecting parameter may be changed by an amount less than its decorrelation threshold, and yet decorrelated speckle patterns can still be obtained. Importantly, because two different types of speckle-affecting parameters tend to alter the component frames in different ways, it has been found that the spatial resolution of the compound image is better as compared to the scenario in which only one speckle-affecting parameter is altered by its decorrelation threshold. Thus, continuing the above conceptual example, the transmit frequency might be changed between frames only by an amount $0.2f_0$ (which is less than the above decorrelation threshold of $0.5f_0$), as long as another speckle-affecting parameter, for example, the number of transmit cycles, were changed as well, e.g., from n_0 to $1.5n_0$. In this example, since the transmit frequency is changed by a smaller amount $0.2f_0$, there is a lesser change in the axial resolution of the respective component frames as compared to a transmit frequency change of $0.5f_0$. Furthermore, the change in the number of transmit cycles by $0.5n_0$, while affecting the component frames in some way, will generally affect the component frames in a way that is different than the change in axial resolution. When the compound image is formed by the component frames, it is found that the spatial resolution of the resulting compound image can be better than the compound image resulting if only the transmit frequency were changed from f_0 to $1.5f_0$ between frames.

It is to be appreciated that the above example is a conceptual example only and is introduced to clearly communicate the features and advantages of the preferred embodiments. The actual speckle-affecting parameter selection and the actual speckle-affecting parameter values will be highly system dependent, and therefore the above numerical examples may, or may not, be effective in any given specific ultrasound system. However, upon reading the present disclosure, a person skilled in the art will be readily able to identify which sets of speckle-affecting parameters, and which values and value changes thereof,

will result in enhance spatial resolution of the compound image in any specific ultrasound system without undue experimentation.

Advantageously, because decorrelation of the component frames is enhanced by the toggling of several speckle-affecting parameters at once, the number of component frames “N” needed generate a reduced-speckle compounded result may be decreased. Accordingly, the temporal resolution of an ultrasound system in accordance with the preferred embodiments may likewise be increased as compared to prior art systems.

FIG. 2 shows transmit beamformer 104 as adapted for use in the system of FIG. 1 comprising a memory 202 for storing transmit beamformer speckle-affecting parameters in accordance with a preferred embodiment. As shown in FIG. 2, memory 202 comprises a predetermined number MT of sets of speckle-affecting parameters. In a configuration in which receive beamformer and demodulator speckle-affecting parameters are not varied between component frames, the predetermined number MT may be as little as 2, or may be several times greater as may be empirically determined to yield the best results for specific machines or systems. For a first component frame k, the 0th column of speckle-affecting parameters from memory 202 is used; for a second component frame k+1, the 1st column is used, and so on up to component frame k+MT-1, in which case the (MT-1)st column is used. For the frame k+MT, the 0th column is re-used, and so on. In general, for a kth component frame, the (k mod MT)th column of speckle-affecting parameters from memory 202 is used to process that frame. It is to be appreciated, however, that if receive beamformer and/or demodulator speckle-affecting parameters are varied between component frames, the number MT may be 1, representing the case in which transmit beamformer speckle-affecting parameters are not varied between frames.

For a given column “i” of memory array 202, the transmit beamformer speckle-affecting parameters include a transmit frequency F_i and a number of transmit cycles CYCLES_i. For single-zone transmitting, the transmit frequency F_i and number of transmit cycles CYCLES_i are scalar quantities used for the entire frame. For multi-zone transmitting, in which the component frame is formed from a number ntz_i of separate transmit zones, F_i and CYCLES_i are linear arrays of length ntz_i, each element representing the transmit frequency and number of transmit cycles, respectively, for its respective transmit zone.

The transmit beamformer speckle-affecting parameters further include a transmit pulse shape parameter, an array TXSHAPE_i. For single-zone transmitting, TXSHAPE_i is a linear array of nts_i elements, where nts_i represents the number of transmit cycles being weighted. In general, nts_i will be related to CYCLES_i. Generally, the values of TXSHAPE_i are weightings applied to the transmit pulses that may form different pulse shapes, such as rectangular (the default), Gaussian, Hamming, cosine, triangular, or other shapes. As an alternative to setting the transmit pulse shape parameter by specific weightings, the transmit beamformer 104 may store a number of pre-set transmit pulse shapes, which may then simply be identified by scalar indicators such RECTANGULAR, GAUSSIAN₁, GAUSSIAN₂, HAMMING₁, HAMMING₂, and so on. For multi-zone transmitting, the array TXSHAPE_i will be a two-dimensional array having ntz_i rows, each row representing the transmit pulse shape parameter for its respective transmit zone.

The transmit beamformer speckle-affecting parameters further include a transmit focus profile, an array TXFO-

CUS_i. In its most general form, for single-zone transmitting TXFOCUS_i will be a linear array of ntd_i members, where ntd_i corresponds to the number of transducer elements and each member of TXFOCUS_i corresponds to delay amounts for each transducer element. However, as a more common alternative to directly setting the individual delays, the transmit beamformer 104 may store a number of preset parameter sets corresponding to different transmit focus profile characteristics, which may then be represented by a simple identifier or scalar parameter in the array TXFOCUS_i. Transmit focus profile parameters include, for example, a transmit focal point relating to a focusing distance, a transmit steering angle, a transmit F-number relating to beam width, a transmit focus algorithm identifier (e.g., spherical, line, etc.), and a transmit aperture setting relating to which transducer elements are active. For multi-zone transmitting, TXFOCUS_i will have an additional dimension of length ntz_i, where ntz_i is the number of transmit zones.

The transmit beamformer speckle-affecting parameters further include a transmit apodization profile, an array TXAPOD_i. For single-zone transmitting, TXAPOD_i is a linear array of nta_i elements, where nta_i represents the number of transducer elements being weighted. As an alternative to setting the individual transducer element weightings, the transmit beamformer 104 may store a number of preset apodization profiles, which may then simply be identified by their type. For multi-zone transmitting, the array TXAPOD_i will be a two-dimensional array having ntz_i rows, each row representing the apodization profile for its respective transmit zone. The transmit beamformer speckle-affecting parameters further include other parameters TXOTHER_i, known to affect the speckle pattern of the component frames.

FIG. 3 shows a receive beamformer 106 as adapted for use in the system of FIG. 1 comprising a memory 302 for storing receive beamformer speckle-affecting parameters in accordance with a preferred embodiment. The memory 302 of FIG. 3 comprises a predetermined number MR of sets of speckle-affecting parameters. Similar to the operation of transmit beamformer 104, the (k mod MR)th column of speckle-affecting parameters from memory 302 is used to process the kth component frame. In a configuration in which transmit beamformer and demodulator speckle-affecting parameters are not varied between component frames, the predetermined number MR may be as little as 2, or may be several times greater as may be empirically determined to yield the best results. However, if MT is greater than 1 and/or demodulator speckle-affecting parameters are varied between component frames, the number MR may be 1, representing the case in which receive beamformer speckle-affecting parameters are not varied between frames.

For a given column “i” of memory array 302, the receive beamformer speckle-affecting parameters include a receive bandwidth RXBW_i. For single-zone receiving, the receive bandwidth RXBW_i is a scalar quantity used for the entire frame. For multi-zone receiving, in which the component frame is formed from a number nrz_i of separate receive zones, RXBW_i is a linear array of length nrz_i, each element representing the receive bandwidth for its respective receive zone.

The receive beamformer speckle-affecting parameters further include a receive focus profile, an array RXFOCUS_i, that is a receive beamformer counterpart to the transmit focus profile TXFOCUS_i. In its most general form, for single-zone receiving RXFOCUS_i will be a linear array of nrd_i members. As with the transmit beamformer, the receive

focus profile RXFOCUS_i may comprise individual delay values, or as a more common alternative to directly setting the individual delays, the receive beamformer **106** may store a number of preset parameter sets corresponding to different receive focus profile characteristics, which may then be represented by a simple identifier or scalar parameter in the array RXFOCUS_i . Receive focus profile parameters include, for example, a receive focal point relating to a focusing distance, a receive steering angle, a receive F-number relating to beam width, a receive focus algorithm identifier (e.g., spherical, line, etc.), and a receive aperture setting relating to which transducer elements are active. For multi-zone receiving, RXFOCUS_i will have an additional dimension of length nrz_i , where nrz_i is the number of receive zones.

The receive beamformer speckle-affecting parameters further include a receive apodization profile, an array RXAPOD_i . For single-zone receiving, RXAPOD_i is a linear array of nra_i elements, where nra_i represents the number of transducer elements being weighted. As an alternative to setting the individual transducer element weightings, the receive beamformer **106** may store a number of preset apodization profiles, which may then simply be identified by their type. For multi-zone receiving, the array RXAPOD_i will be a two-dimensional array having nrz_i rows, each row representing the apodization profile for its respective receive zone. The receive beamformer speckle-affecting parameters further include other parameters RXOTHER_i known to affect the speckle pattern of the component frames.

FIG. 4 shows a demodulator **108** as adapted for use in the system of FIG. 1 comprising a memory **402** for storing demodulator speckle-affecting parameters in accordance with a preferred embodiment. The memory **402** of FIG. 4 comprises a predetermined number MD of sets of speckle-affecting parameters. Similar to the operation of transmit beamformer **104** and receive beamformer **106**, the $(k \bmod \text{MD})^{\text{th}}$ column of speckle-affecting parameters from memory **402** is used to process the k^{th} component frame. In a configuration in which transmit beamformer and receive beamformer speckle-affecting parameters are not varied between component frames, the predetermined number MD may be as little as 2, or may be several times greater as may be empirically determined to yield the best results. However, if MT is greater than 1 and/or MR is greater than 1, the number MD may be 1, representing the case in which demodulator speckle-affecting parameters are not varied between frames.

For a given column "i" of memory array **402**, the demodulator speckle-affecting parameters include a local oscillator frequency $\text{FLOC}_{13 \text{ osc}_i}$. For single-zone receiving, the local oscillator frequency $\text{FLOC}_{13 \text{ osc}_i}$ is a scalar quantity used for the entire frame. For multi-zone receiving, in which the component frame is formed from a number nrz_i of separate receive zones, $\text{FLOC}_{13 \text{ osc}_i}$ is a linear array of length nrz_i , each element representing the local oscillator frequency for its respective receive zone.

The demodulator speckle-affecting parameters further include a receive pulse shape parameter, an array RXSHAPE_i of nrs_i elements analogous to the array TXSHAPE_i of transmit beamformer **104**. The demodulator speckle-affecting parameters further include other parameters DXOTHER_i known to affect the speckle pattern of the component frames.

FIG. 5 shows overall main steps carried out by the system of FIG. 1 in generating a compound ultrasound image and managing speckle-affecting parameters in accordance with a preferred embodiment. At step **502**, processing of a next frame k begins. At step **504**, using the values in its memory **202**, transmit beamformer **104** causes transducer **102** to generate interrogation signals using its $(k \bmod \text{MT})^{\text{th}}$ set of speckle-affecting parameters. At step **506**, receive beam-

former **106** receives signals corresponding to reflected acoustic signals from the transducer **102** and, using the values in its memory **302**, generates a single channel RF signal using its $(k \bmod \text{MR})^{\text{th}}$ set of speckle-affecting parameters. At step **508**, demodulator **108** processes the received signal into a k^{th} component frame using its $(k \bmod \text{MD})^{\text{th}}$ set of speckle-affecting parameters.

At step **510**, DSP subsystem **112** generates the compound image output using the k^{th} frame in conjunction with $(N-1)$ previous component frames, where N is the number of component frames being compounded. The preferred compounding method is described infra with respect to FIG. 6, although other compounding methods may be used. At step **512**, the frame counter k is incremented. At step **514**, the system controller **114** determines whether other imaging parameters or settings in the ultrasound system **100** have been changed. If not, processing of the next frame continues at step **502**. If so, at step **516**, new speckle-affecting parameters are loaded into the respective memories **202**, **302**, and **402** if necessary to correspond to the new system parameters. In one preferred embodiment, the system controller computes a new value for "N," the number of frames being compounded, based on the new imaging parameters or settings, and then changes the speckle-affecting parameters in the respective memories **202**, **302**, and **402** according to the new value for "N." As an example, the number "N" may be varied to maintain a given output frame rate which, in turn, can be dependent on a variety of factors, such as display depth, number of transmit focal zones, display mode (e.g. B-mode, color Doppler, power Doppler), or other factors.

FIG. 6 shows a conceptual diagram illustrating the creation of compound images using statistically decorrelated component frames in accordance with a preferred embodiment. Preferably, as shown in FIG. 6, the decorrelated component frames are compounded by DSP subsystem **112** using a finite impulse response (FIR)-like method, such that the output frame rate of the compounded images is as great as the acquisition frame rate of the component frames. Shown in FIG. 6 is a time sequence of frames **602** which, at a point in time k , are independently weighted by the weighting factors **604** as shown in FIG. 6, and then summed by an accumulation device **606** to produce the k^{th} compound output image **608**. While the next frame $k+1$ is included in the computation of the $(k+1)^{\text{st}}$ compound output image, the $[k-(N-1)]^{\text{th}}$ frame is dropped from inclusion in the compounding step. In this way, the output frame rate of the compounded images is as high as the acquisition frame rate of the component frames. The weighting factors **604** may be scalar amounts, or may alternatively be two-dimensional arrays for weighting the frames on a per-location basis.

Tables 1 and 2 below show exemplary sets of speckle-affecting parameters, along with frame weightings, that may be used in accordance with the preferred embodiments. These particular numerical values are useful in a system having the commercial designation USI-2000 by U-Systems, Inc. of Los Altos, Calif.

TABLE 1

Speckle-Affecting Parameter Changes and Compounding Weights
($\text{MT} = 2$; $\text{MR} = 1$; $\text{MD} = 1$; 7.5 MHz Transducer)

Frame Id	Parameters Adjusted	Weighting Parameter
1	Focus = 2 cm, 4 cm, 6 cm F number = 2.0 Number of transmit cycles = 1 Apodization = HAMMING1	0.5

TABLE 1-continued

Speckle-Affecting Parameter Changes and Compounding Weights (MT = 2; MR = 1; MD = 1; 7.5 MHz Transducer)		
Frame Id	Parameters Adjusted	Weighting Parameter
2	Focus = 3 cm, 5 cm, 7 cm F number = 2.5 Number of transmit cycles = 2 Apodization = HAMMING2	0.5

TABLE 2

Speckle Affecting Parameter Changes and Compounding Weights (MT = 4; MR = 1; MD = 1; 10 MHz Transducer)		
Frame Id	Parameters Adjusted	Weighting Parameter
1	Focus = 1 cm, 3 cm Transmit Frequency = 7 MHz	0.2
2	Focus = 2 cm, 4 cm Transmit Frequency = 8 MHz	0.2
3	Focus = 1.5 cm, 3.5 cm Transmit frequency = 9 MHz	0.3
4	Focus = 2.5 cm, 4.5 cm Transmit Frequency = 10 MHz	0.3

Again, it is to be appreciated that the above examples are introduced only to clearly communicate the features and advantages of the preferred embodiments. The actual speckle-affecting parameter selection and the actual speckle-affecting parameter values will be highly system dependent, and therefore the above numerical examples may, or may not, be effective in any given specific ultrasound system. However, upon reading the present disclosure, a person skilled in the art will be readily able to identify which sets of speckle-affecting parameters, and which values and value changes thereof, will result in enhance spatial resolution of the compound image in any specific ultrasound system.

In one alternative preferred embodiment in which the concept of speckle-affecting parameter toggling is taken one step further, the frame quality may be increased by the altering the “tuning” of certain speckle-affecting parameters with respect to each other within a single firing. Normally, certain speckle-affecting parameters in one component of the ultrasound system, e.g., the local oscillator frequency used by demodulator 108, is “tuned” to a different speckle-affecting parameter used by a different component of the ultrasound system 100, e.g., the transmit frequency used by transmit beamformer 104. It has been found that such intra-frame parameters may be “detuned” from each other to alter the speckle patterns. In one example of this alternative preferred embodiment, subharmonic frequency compounding is used, wherein the local oscillator frequency used by the demodulator 108 is selected to be near a subharmonic, say $0.5f_0$, of the transmit frequency f_0 of the transmit beamformer 104. When compounded with other component frames generated without using a subharmonic local oscillator frequency, the result may be further enhanced. In one preferred embodiment, the component frame generated using a location oscillator frequency of $0.5f_0$ may be combined with a component frame generated using a harmonic of f_0 , say, $2f_0$ and then compounded to form a compound output image.

In another preferred embodiment, more than one receive beamformer and/or demodulator may be implemented in

parallel for processing signals corresponding to the k^{th} component frame using different speckle-affecting parameters, with the results being compounded together and also compounded with the results for component frames $k-1$, $k-2$, etc., which were in turn processed using different speckle-affecting parameters. Thus, for example, a first receive beamformer having two sets of speckle-affecting parameters ($SP1_0$ and $SP1_1$) in its memory may process component frames k and $k+1$ using the speckle-affecting parameter sets $SP1_0$ and $SP1_1$, respectively. The single-channel RF signals are processed by a first parallel demodulator to form two frames $FSP1(k)$ and $FSP1(k+1)$, respectively. At the same time, a second receive beamformer, positioned in parallel with the first receive beamformer and having two other sets of speckle-affecting parameters ($SP2_0$ and $SP2_1$) in its memory, processes the same component frames k and $k+1$ using the speckle-affecting parameter sets $SP2_0$ and $SP2_1$, respectively. The single-channel RF signals are processed by a second parallel demodulator to form two frames $FSP2(k)$ and $FSP2(k+1)$, respectively. According to a preferred embodiment, the frames $FSP1(k)$ and $FSP2(k)$ are combined to form a frame $FSP(k)$, and the frames $FSP1(k+1)$ and $FSP2(k+1)$ are combined to form a frame $FSP(k+1)$. The frames $FSP(k)$ and $FSP(k+1)$ are compounded (along with frames $FSP(k+2)$, $FSP(k+3)$, . . . similarly formed) using the compounding methods described supra with respect to FIG. 6.

In another example of the above preferred embodiment, intra-frame harmonic compounding may be combined with decorrelated inter-frame compounding to produce an output with a desirable amount of speckle reduction. In particular, in an ultrasound system in which the transmit beamformer has a transmit frequency of f_0 , three parallel demodulators having local oscillator frequencies of $0.5f_0$ (a subharmonic of the transmit frequency), f_0 (the transmit frequency), and $2f_0$ (a harmonic of the transmit frequency), respectively, may be used to form the frames $FSP1(k)$, $FSP2(k)$, and $FSP3(k)$, respectively, for the k^{th} frame. For the next frame $k+1$, the three demodulators produce the frames $FSP1(k+1)$, $FSP2(k+1)$, and $FSP3(k+1)$ also using local oscillator frequencies of $0.5f_0$, f_0 , and $2f_0$, respectively. Importantly, at least one other speckle-affecting parameter used by the transmit beamformer, receive beamformer, or demodulator is different for frame $(k+1)$ than for frame k . According to a preferred embodiment, the frames $FSP1(k)$, $FSP2(k)$, and $FSP3(k)$ are combined to form a frame $FSP(k)$, and the frames $FSP1(k+1)$, $FSP2(k+1)$, and $FSP3(k+1)$ are combined to form a frame $FSP(k+1)$. The frames $FSP(k)$ and $FSP(k+1)$ are compounded (along with frames $FSP(k+2)$, $FSP(k+3)$, . . . similarly formed) using the compounding methods described supra with respect to FIG. 6.

Whereas many alterations and modifications of the present invention will no doubt become apparent to a person of ordinary skill in the art after having read the foregoing description, it is to be understood that the particular embodiments shown and described by way of illustration are in no way intended to be considered limiting. For example, a system in accordance with the preferred embodiments may be used with color Doppler systems, power Doppler systems, and other systems. In a Doppler system, for example, the transmit beamformer, receive beamformer, and demodulator may additionally use varying Doppler parameters for successive component frames to enhance their statistical decorrelation. Therefore, reference to the details of the preferred embodiments are not intended to limit their scope, which is limited only by the scope of the claims set forth below.

13

What is claimed is:

1. A method for generating a compound ultrasound image, comprising the steps of:
 - generating a first component frame using a first set of speckle-affecting parameters;
 - generating a second component frame using a second set of speckle-affecting parameters, wherein said first and second sets differ by at least two speckle-affecting parameters; and
 - forming the compound ultrasound image using said first and second component frames;

wherein each of said speckle-affecting parameters is an ultrasound system setting that, if changed in isolation between two otherwise identical ultrasound system configurations, would cause the ultrasound system to generate frames having at least partially decorrelated speckle patterns,

each of said speckle-affecting parameters being associated with a decorrelation threshold, said decorrelation threshold being characterized in that, if said speckle-affecting parameter were changed in isolation by an amount less than said decorrelation threshold between two otherwise identical ultrasound system configurations, the ultrasound system would generate frames having only partially decorrelated speckle patterns, said decorrelation threshold being further characterized in that, if said speckle-affecting parameter were changed in isolation by an amount greater than said decorrelation threshold between two otherwise identical ultrasound system configurations, the ultrasound system would generate frames having substantially decorrelated speckle patterns, wherein said at least two speckle-affecting parameters of said first and second sets each differ by an amount less than their corresponding decorrelation thresholds.

2. The method of claim 1, further comprising the step of generating a third component frame using a third set of speckle-affecting parameters, wherein said first, second, and third sets each differ from each other by at least two speckle-affecting parameters, and wherein said third component frame is also used in said step of forming the compound ultrasound image.

3. The method of claim 1, further comprising the step of generating (N-3) additional component frames using an additional (N-3) sets of speckle-affecting parameters, wherein each of said N sets each differ from each other by at least two speckle-affecting parameters, and wherein all N component frames are used in said step of forming the ultrasound image.

4. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of at least one transmit beamformer parameter and at least one receive beamformer parameter.

5. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of at least one receive beamformer parameter and at least one demodulator parameter.

6. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of at least one transmit beamformer parameter and at least one demodulator parameter.

7. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of: transmit frequency, number of transmit cycles, number of transmit zones, transmit pulse shape, transmit focus profile, transmit focal point, transmit steering angle, transmit

14

F-number, transmit focus algorithm identifier, transmit aperture setting, and transmit apodization profile.

- 5 8. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of: receive bandwidth, receive focus profile, receive focal point, receive steering angle, receive F-number, receive focus algorithm identifier, receive aperture setting, and receive apodization profile.

- 10 9. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of local oscillator frequency and receive pulse shape.

- 15 10. The method of claim 1, wherein said speckle-affecting parameters are selected from the group consisting of: transmit frequency, number of transmit cycles, number of transmit zones, transmit pulse shape, transmit focus profile, transmit focal point, transmit steering angle, transmit F-number, transmit focus algorithm identifier, transmit aperture setting, transmit apodization profile, receive bandwidth, receive focus profile, receive focal point, receive steering angle, receive F-number, receive focus algorithm identifier, receive aperture setting, receive apodization profile, local oscillator frequency, and receive pulse shape.

- 20 11. The method of claim 10, wherein first and second sets of speckle-affecting parameters differ by said transmit frequency parameter and said transmit focal point parameter.

- 25 12. The method of claim 1, wherein said component frames are compounded using a finite-impulse-response (FIR) method and N distinct weighting factors, whereby an output frame rate of said compounded images is equal to an acquisition frame rate of said component frames.

- 30 13. The method of claim 12, wherein N is equal to 4.

- 35 14. A method for generating a compound output image in an ultrasound system using partial frequency compounding, comprising the steps of:

- 40 generating a first component frame using a first transmit frequency and a first type of speckle-affecting parameter set at a first value;

- 45 generating a second component frame using (i) a second transmit frequency that differs from said first transmit frequency by an amount less than a decorrelation threshold, and (ii) said first type of speckle-affecting parameter set at a second value different than said first value; and

- 50 forming the compound ultrasound image using said first and second component frames;

- 55 wherein said decorrelation threshold corresponds to a minimum transmit frequency shift required to establish two frames having decorrelated speckle patterns if no other ultrasound system parameters were changed;

- 60 and wherein said second value of said first type of speckle-affecting parameter differs from said first value by an amount sufficient to establish two frames having decorrelated speckle patterns even though said first and second transmit frequencies differ by less than said decorrelation threshold;

- 65 whereby said ultrasound system is capable of generating a reduced-speckle compound image without incurring spatial resolutions losses as great as those associated with inter-frame frequency differences greater than said decorrelation threshold.

- 70 15. The method of claim 14, wherein said step of generating said first component frame also uses a second speckle-affecting parameter set at a third value, and wherein said step of generating said second component frame also uses said second speckle-affecting parameter set at a fourth value different than said third value, whereby said first and second

15

values of said first speckle-affecting parameter may be closer together in achieving said decorrelated speckle patterns than if said second speckle-affecting parameter were not varied between the component frames.

16. The method of claim **15**, wherein said first speckle-affecting parameter is selected from the group consisting of at least one receive beamformer parameter and at least one demodulator parameter. 5

17. The method of claim **15**, wherein said first and second speckle-affecting parameters are selected from the group consisting of: at least one transmit beamformer parameter other than transmit frequency, at least one receive beamformer parameter; and at least one demodulator parameter. 10

18. The method of claim **15**, wherein said first and second speckle-affecting parameters are selected from the group consisting of: number of transmit cycles, number of transmit zones, transmit pulse shape, transmit focus profile, transmit focal point, transmit steering angle, transmit F-number, transmit focus algorithm identifier, transmit aperture setting, transmit apodization profile, receive bandwidth, receive 15 focus profile, receive focal point, receive steering angle, receive F-number, receive focus algorithm identifier, receive aperture setting, receive apodization profile, local oscillator frequency, and receive pulse shape.

19. A method for use with an ultrasound imaging system comprising: 25

generating a first ultrasound frame using a first set of speckle-affecting parameters;

16

generating a second ultrasound frame using a second set of speckle-affecting parameters;

wherein said first and second sets of speckle-affecting parameters differ from each other in at least two speckle-affecting parameters; and

using said first and second ultrasound frames to form at least one ultrasound image;

wherein each of said at least two speckle-affecting parameters is changed between the first and second ultrasound frames; and

wherein the change in each of said at least two speckle-affecting parameters is by an amount that, when only one of said at least two parameters is changed between the first and second frames generated with said system in an ultrasound examination of a body, and no other changes are made, two respective images derived therefrom show no perceptible difference in visible speckle, and when each of said at least two parameters is changed by said amount, and the second frame is generated under conditions that are otherwise the same as for the first frame, said images show a perceptible difference in visible speckle.

20. A method as in claim **19** including using at least said first and second frames to form and display a compound ultrasound image.

* * * * *

专利名称(译)	用于生成具有去相关散斑图案的超声帧并从其生成复合超声图像的方法和系统		
公开(公告)号	US6524252	公开(公告)日	2003-02-25
申请号	US09/721889	申请日	2000-11-24
[标]申请(专利权)人(译)	U系统公司		
申请(专利权)人(译)	U-SYSTEMS INC.		
当前申请(专利权)人(译)	U-SYSTEMS INC.		
[标]发明人	YU ZENGPIN ZHAO DANHUA LIN SHENTZ YIN FENG		
发明人	YU, ZENGPIN ZHAO, DANHUA LIN, SHENTZ YIN, FENG		
IPC分类号	G01S7/52 A61B8/00		
CPC分类号	G01S7/52074 G01S7/52046		
代理机构(译)	COOPER & DUNHAM LLP		
外部链接	Espacenet USPTO		

摘要(译)

一种超声系统，其从具有去相关散斑图案的分量帧生成复合图像。连续组的不同的，散斑影响参数用于生成用于复合的连续分量帧，并且被选择成使得连续分量帧具有去相关的散斑图案。可以从各种参数中选择从帧到帧改变的斑点影响参数，包括发射波束形成器参数，接收波束形成器参数和解调器参数。根据优选实施例，连续的斑点影响参数组彼此相差至少两个斑点影响参数。根据另一个优选实施例，多个斑点影响参数中的每一个被改变的量小于该参数的去相关阈值，即，小于仅影响斑点的参数将需要改变的量。如果没有其他参数改变，则产生去相关的散斑图案。当更多斑点影响参数改变时，每个影响斑点的参数可以改变小于其去相关阈值的量，并且仍然可以获得去相关的斑点图案。此外，因为两种不同类型的散斑影响参数倾向于以不同方式改变分量帧的空间分辨率，所以与仅影响一个散斑影响参数的情况相比，复合图像的空间分辨率可以更好。通过其去相关阈值。

