




US 20030208124A1

(19) **United States**(12) **Patent Application Publication**  
**Poland**(10) **Pub. No.: US 2003/0208124 A1**(43) **Pub. Date: Nov. 6, 2003**(54) **ULTRASONIC DIAGNOSTIC IMAGING  
WITH STEERED IMAGE PLANE**09/641,306, filed on Aug. 17, 2000, now Pat. No.  
6,443,896.(76) **Inventor: McKee Dunn Poland, Andover, MA  
(US)****Publication Classification**(51) **Int. Cl.<sup>7</sup> ..... A61B 8/00**(52) **U.S. Cl. .... 600/437**


Correspondence Address:

**ATL ULTRASOUND****P.O. BOX 3003****22100 BOTHELL EVERETT HIGHWAY****BOTHELL, WA 98041-3003 (US)**(21) **Appl. No.: 10/448,518**(22) **Filed: May 30, 2003****Related U.S. Application Data**(63) Continuation-in-part of application No. 10/437,834,  
filed on May 12, 2003, which is a continuation-in-part  
of application No. 10/231,704, filed on Aug. 29, 2002,  
which is a continuation-in-part of application No.(57) **ABSTRACT**


A two-dimensional array transducer probe is used to image regions of the body that are acoustically obstructed from conventional view by objects such as the lungs or ribs. The probe is located against the body at an acoustic window which provides acceptable ultrasonic transmissivity between the transducer array and the body. While maintaining the probe at its acoustic window, an image plane location is manipulated by adjusting the beam steering directions. The image plane can be tilted in the elevation direction, moved laterally, and/or rotated about a center axis to position the image plane so that the obstructed anatomy is effectively imaged for diagnosis.

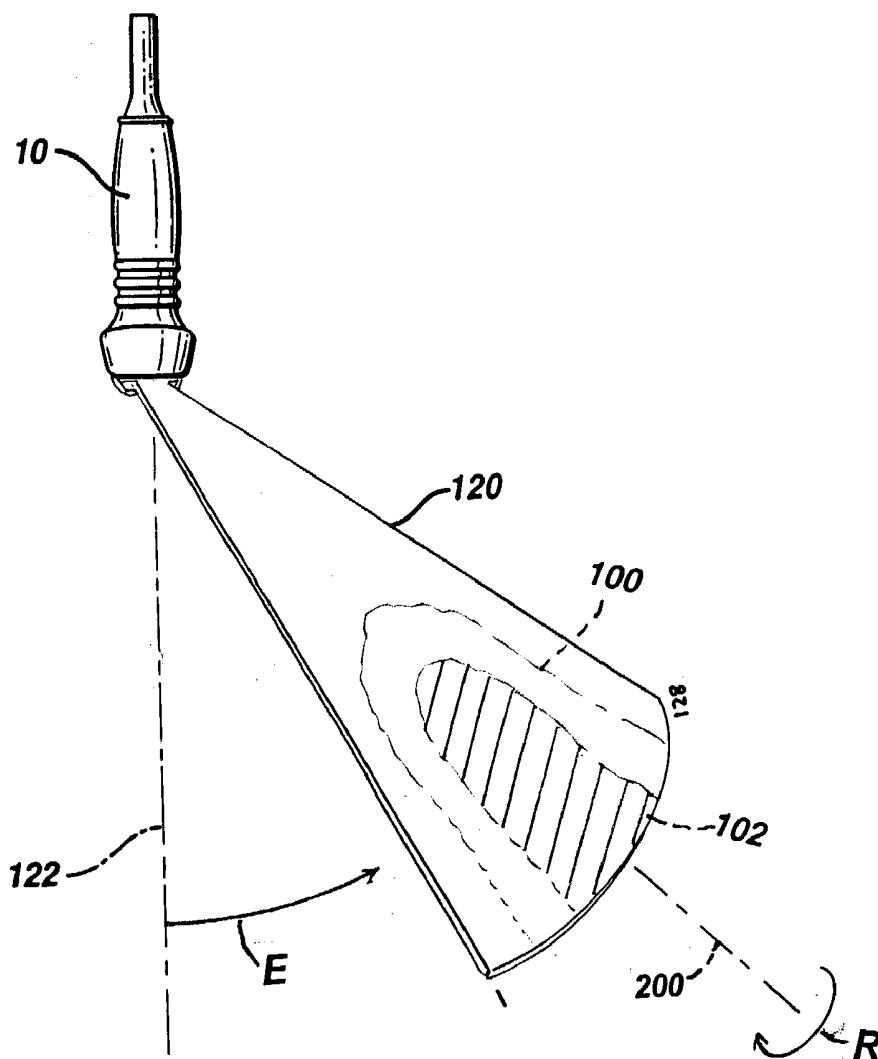


**FIG. 1**

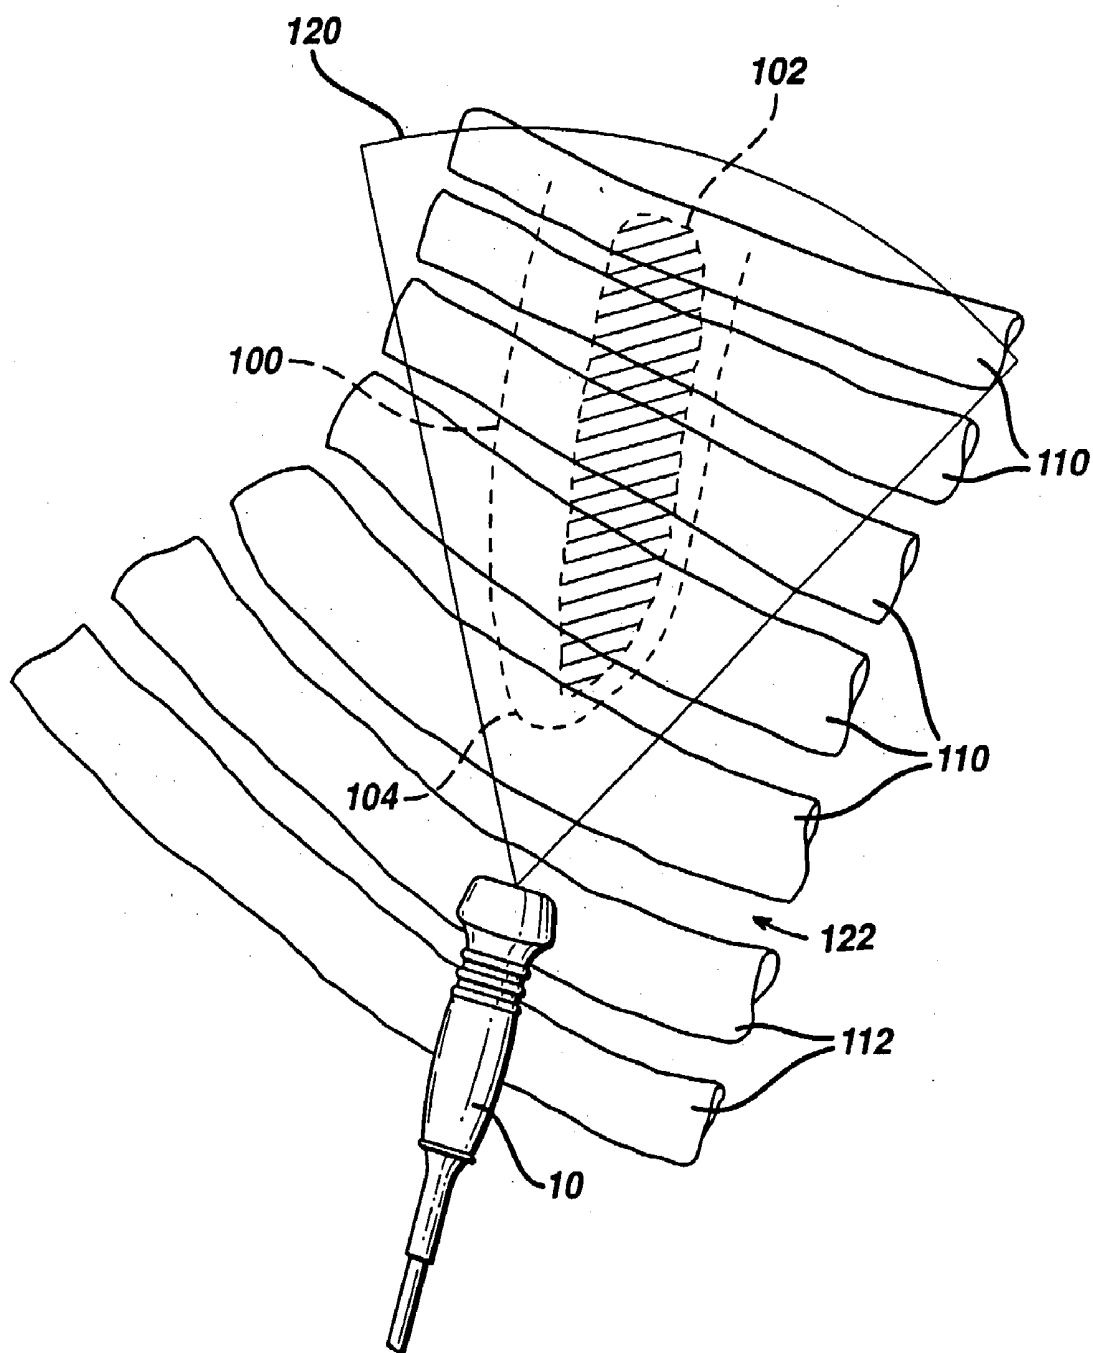


**FIG. 2a**

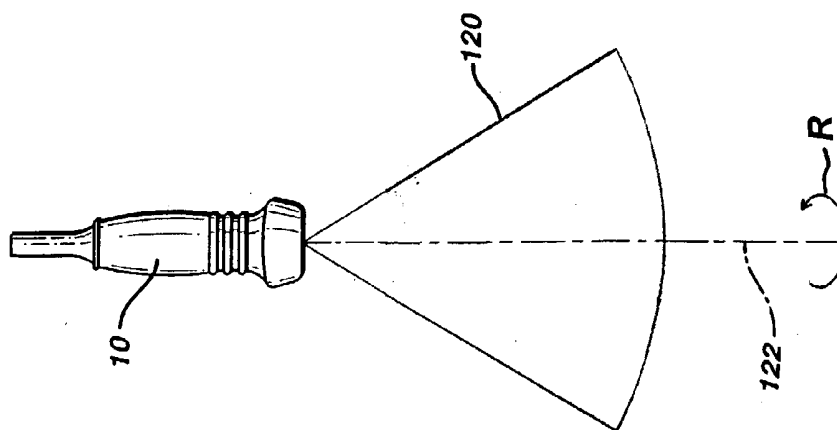


**FIG. 2b**

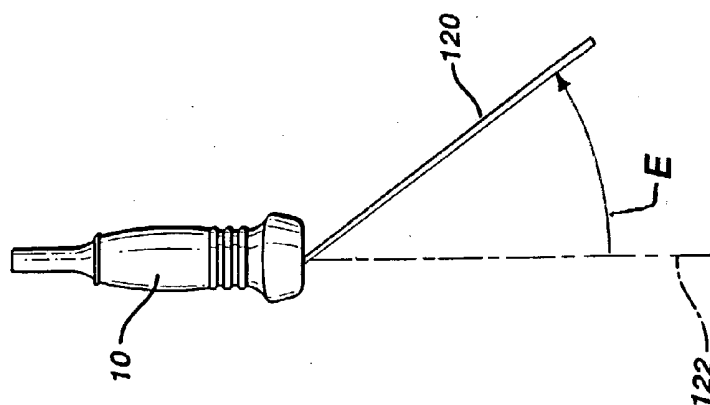

**FIG. 2c**

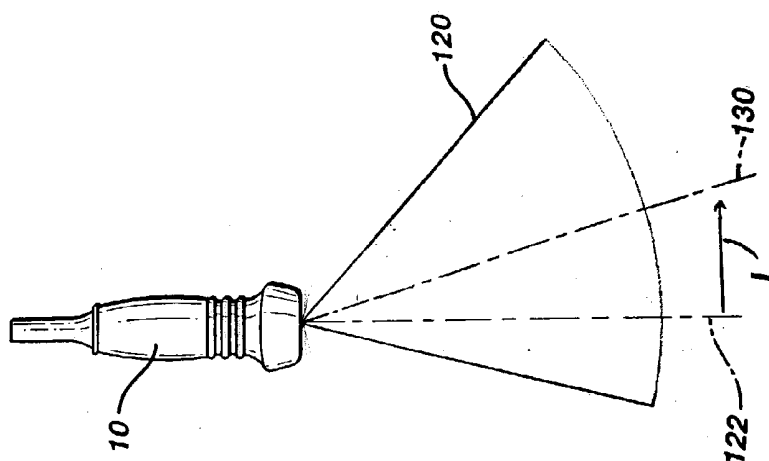

**FIG. 2d**

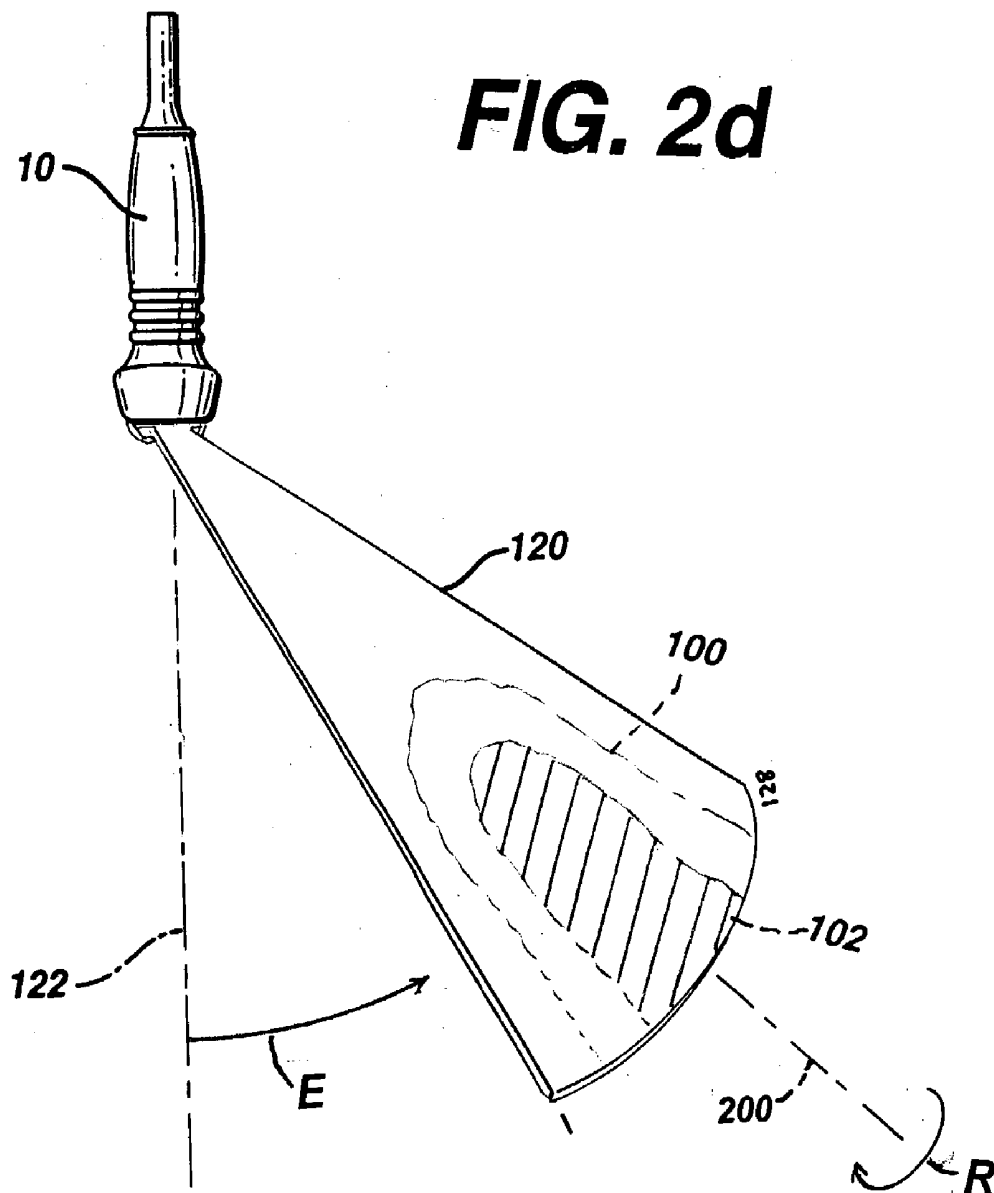


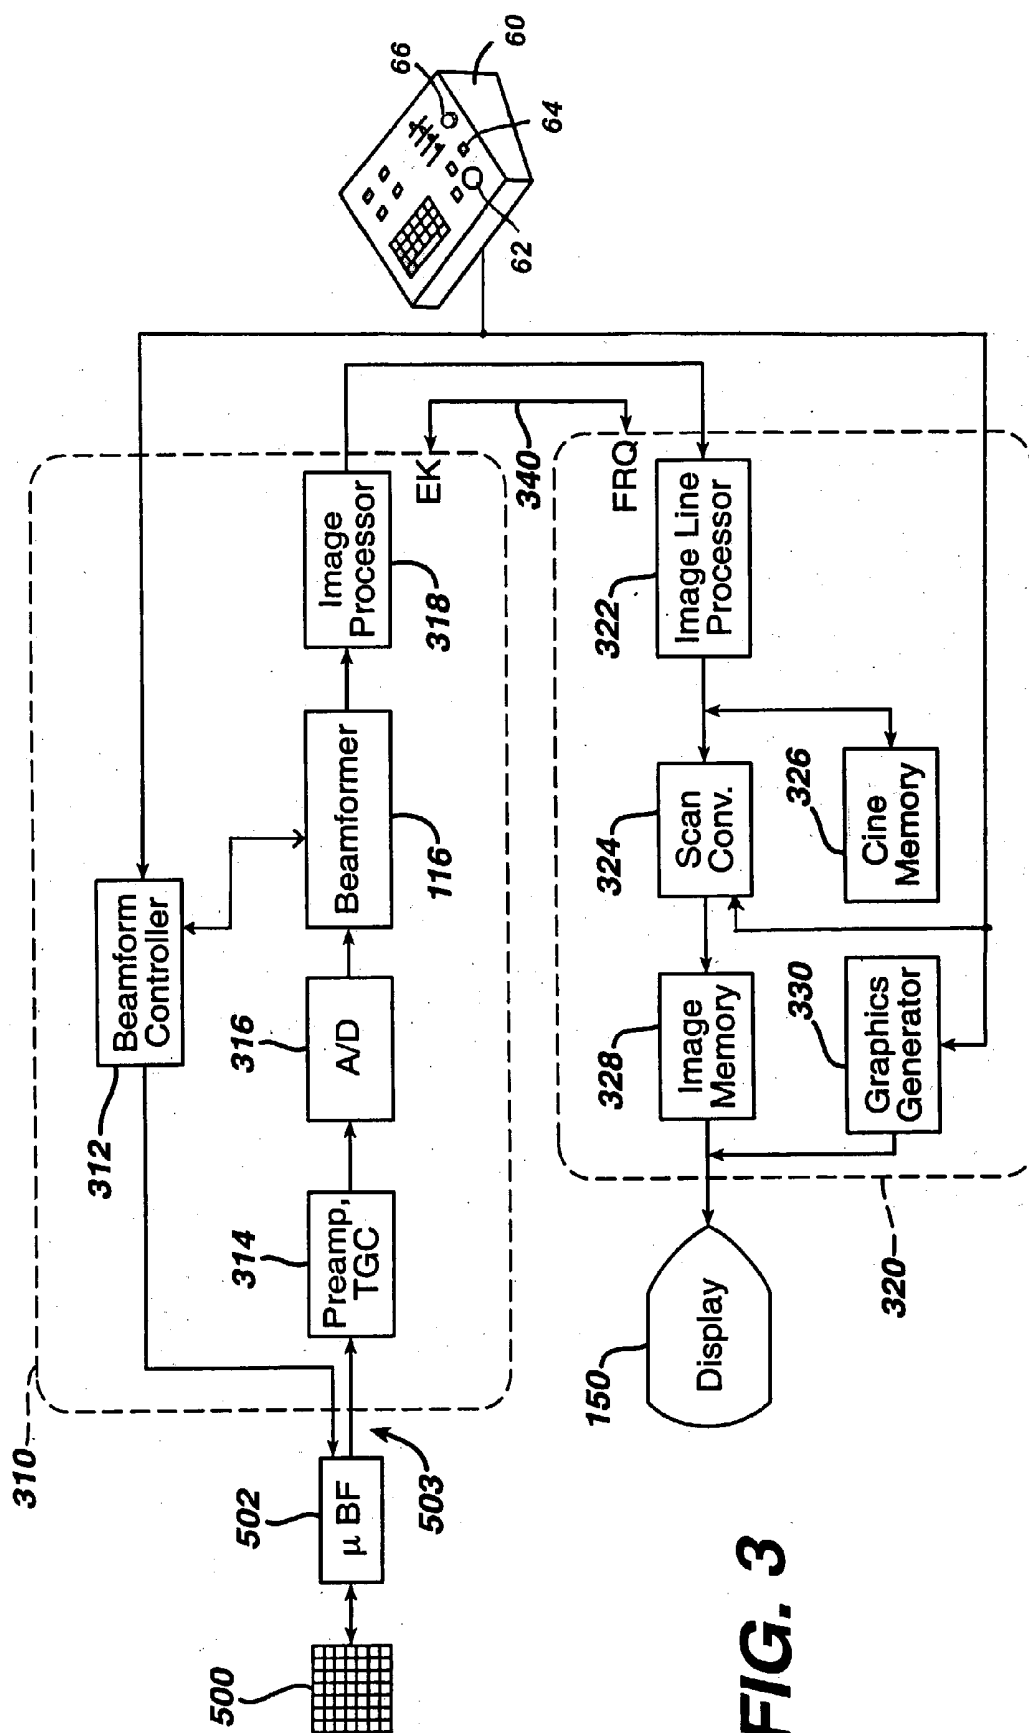


FIG. 3

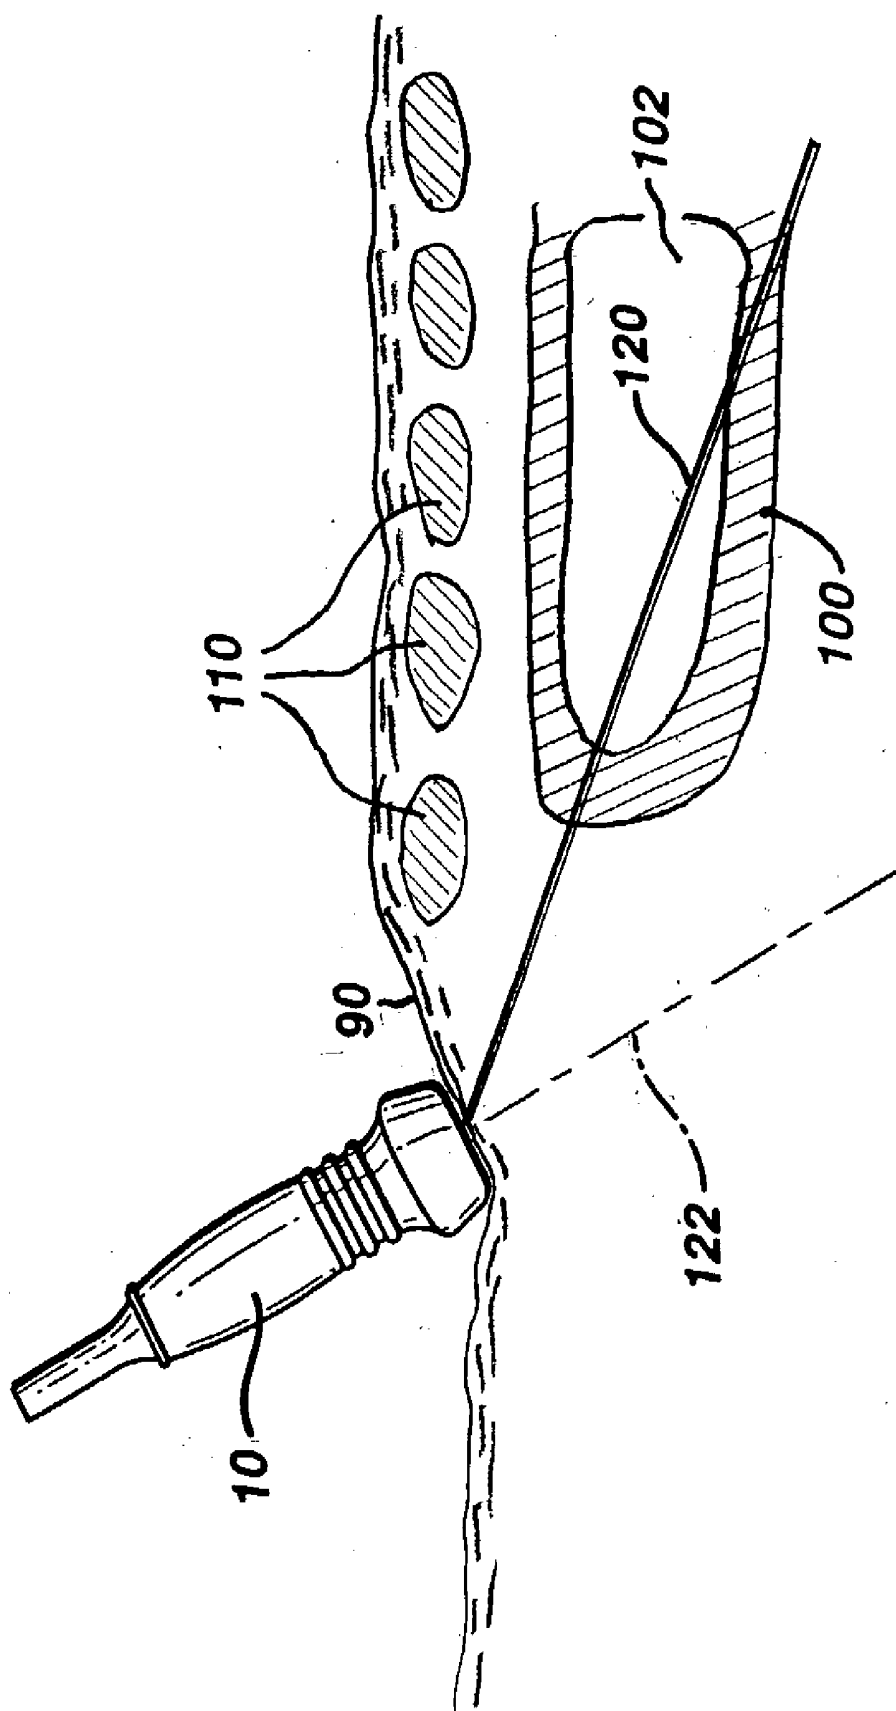

**FIG. 4**

## ULTRASONIC DIAGNOSTIC IMAGING WITH STEERED IMAGE PLANE

**[0001]** This is a continuation in part application of U.S. patent application Ser. No. 10/437,834, filed May 12, 2003, which is a continuation in part application of U.S. patent application Ser. No. 10/231,704, filed Aug. 29, 2002, which is a continuation in part application of U.S. patent application Ser. No. 09/641,306, filed Aug. 17, 2000 and now U.S. Pat. No. 6,443,896.

**[0002]** This invention relates to ultrasonic diagnostic imaging, and more particularly, to ultrasound systems that enable the image plane to be steered while maintaining a good acoustic window for the probe.

**[0003]** Medical diagnostic imaging systems produce highly diagnostic images of soft tissue of the body. However, tissue and organs which need to be observed are frequently obscured by parts of the body which are not highly transmissive of ultrasound such as bones and the air-filled lungs. An example of such a situation is shown in **FIG. 1**. In this illustration the heart **100**, shown in partial outline behind the rib cage **110,112**, is located behind the left side of the rib cage. Outlined within the heart and cross-hatched is the left ventricle **102** of the heart **100**, which is frequently the subject of ultrasonic diagnosis for the assessment of cardiac function. The left ventricle can be accessed transthoracically for ultrasonic imaging by scanning the heart from between the ribs **110,112** for adult patients. The ultrasound beams access the heart through an intercostals space **122** between the ribs **110,11**. The probe **10** scans the heart from the heart apex **104** as indicated by the outline **120** of the image sector scanned by the probe **10**. This technique may be ineffective for some pediatric patients because the intercostals space may be too small. The technique may also be ineffective for some adult patients where the intercostals spaces suitable for beam passage do not allow the probe to be angled for access to the region of the heart which must be imaged. When these problems arise other approaches must be tried, such as scanning upward to the heart from below the lowest rib **112**. However this requires that the probe be tilted against the body to aim the image plane upward to the heart while maintaining sufficient physical contact with the skin so that a good acoustic window is maintained between the probe and the skin. These demands are frequently in conflict, so that it can become impossible to aim the image plane in the desired direction while maintaining proper contact with the skin for acoustic transmission into the body. Another solution to this difficulty is to image the heart from the esophagus by use of a transesophageal echocardiography (TEE) probe. While affording excellent acoustic access to the heart by reason of the absence of any intervening rib structure, this is an invasive procedure requiring great care and which often causes patient discomfort as the TEE probe is inserted and retracted from the patient's throat. Accordingly it would be desirable to be able to image regions of the body which are difficult to access, maintaining good acoustic access to the body while obviating the need for complex imaging procedures.

**[0004]** In accordance with the principles of the present invention, an ultrasonic diagnostic imaging system and method are provided in which an image plane can be steered from an ultrasound probe without the need to physically relocate the probe against the skin of the patient. This

permits the clinician to establish good acoustic contact with the body of the patient, then to scan the region of interest of the patient by steering the image plane without altering the acoustic window. The illustrated embodiments show image planes with multiple degrees of freedom so as to acquire the most diagnostically useful images of the region of interest under study.

**[0005]** In the drawings:

**[0006]** **FIG. 1** illustrates intercostals scanning of the heart;

**[0007]** **FIGS. 2a-2c** illustrate numerous degrees of freedom of image plane adjustment;

**[0008]** **FIG. 2d** illustrates an ultrasonic probe of the present invention with two degrees of freedom of image plane adjustment;

**[0009]** **FIG. 3** illustrates an ultrasonic diagnostic imaging system constructed in accordance with the principles of the present invention; and

**[0010]** **FIG. 4** illustrates a method of imaging the heart in accordance with the principles of the present invention.

**[0011]** Referring to **FIGS. 2a-2c**, an ultrasound probe **10** is shown with several image plane adjustments in **FIG. 2a** the probe **10** is seen to scan a sector image **120**. A conventional one-dimensional array transducer will scan a sector which is directly in front of the array transducer. That is, the sector plane is normal to the face of the probe **10** and evenly distributed on both sides of an axis **122** which is normal to the center of the transducer. A probe **10** of the present invention utilizes a two-dimensional array transducer with the elements of the array being controlled to transmit beams of an image in various directions through the volumetric region in front of the probe. This means, as discussed in further detail below, that the image plane **120** can be rotated around a scanline of the image or the normal axis **122** as indicated by the rotational arrow R. Thus, one degree of freedom which a probe of the present invention may exhibit is the ability to rotate the image plane around the center line or other scanline of the image.

**[0012]** In **FIG. 2a** the image plane **120** is depicted in the plane of the drawing. In **FIG. 2b** the image plane **120** is viewed orthogonal to the plane of the drawing, that is, the image plane is viewed "edge-on." If this were a conventional one-dimensional array probe, the image plane would be aligned with the center axis **122**, extending normal to the face of the probe and transducer array. In accordance with this second embodiment of a probe of the present invention, the position of the image plane exhibits a second degree of freedom in which the image plane **120** can be steered in the elevation direction with respect to the nominal plane alignment with axis **122**, as indicated by elevational arrow E. As used herein, elevation tilt or translation refers to an image plane orientation which is not co-planar with a reference plane such as the starting position of a plane change. The image plane **120** in **FIG. 2b** is tilted in the elevation dimension with respect to the position of the p lane of a conventional one-dimensional array probe.

**[0013]** In the third embodiment of **FIG. 2c** the image plane exhibits a third degree of freedom of translation. In this embodiment the image plane **120** is not centered about the axis **122**, but is steered laterally as indicated by the lateral arrow L. In this position the center line **130** of the

image is steered off of the normal probe axis **122** with the image plane **120** capturing lateral areas of the volumetric region which are outside of the area of the conventionally located image plane. This degree of freedom, where the position of an image does not change its plane but is steered in a different direction in the plane, is referred to herein as lateral tilt or translation.

[0014] The embodiment of **FIG. 2d** illustrates a probe **10** scanning an image plane **120** which exhibits two degrees of freedom of translation. In this perspective view the image plane **120** has been elevated away from the normal axis **122** as indicated by the elevational arrow **E**. The image plane **120** has also been rotated about its center axis **200** as indicated by the rotational arrow **R**. Even though the probe is aimed in the direction of the normal axis **122**, its image plane **120** is still able to capture the heart **100** and the left ventricle **102** in the image by reason of the steering of the image beams transmitted and received by the two dimensional array transducer of the probe **10**.

[0015] It will be understood by those skilled in the art that the order of translation operations may be changed as well as their angular extent, to achieve different overall translations of the image plane **120** in three dimensional space. For example, image plane **120** may first be rotated about a central axis **122** by some rotation angle **R**, and then elevated away from that axis by angle **E**. The resulting position of image plane **120** is different than that shown in **FIG. 2d**. In general, by combining two or more rotation and elevation operations, any arbitrary image plane position may be realized, within the practical electro-acoustic beamforming limits of the ultrasound scanner **310**. The translation operations may be combined into a single computational step by beamformer controller **312**, so that the user is not aware of the geometric decomposition.

[0016] Although the scan lines of the image plane **120** are shown in the figures to have a common apex, other co-planar scan line arrangements are possible, such as rectangular or trapezoidal scan line patterns.

[0017] **FIG. 3** illustrates in block diagram form an ultrasound system constructed in accordance with the principles of the present invention. In this embodiment the probe **10** includes a two-dimensional array transducer **500** and a subarray processor or micro-beamformer **502**. The micro-beamformer contains circuitry which control the signals applied to groups of elements ("patches") of the array transducer **500** and does some processing of the echo signals received by elements of each group. Micro-beamforming in the probe advantageously reduces the number of conductors in the cable **503** between the probe and the ultrasound system and is described in U.S. Pat. No. 5,997,479 (Savord et al.) and in U.S. Pat. No. 6,436,048 (Pesque).

[0018] The probe **10** is coupled to the scanner **310** of the ultrasound system. The scanner includes a beamformer controller **312** which is responsive to a user control **60** and provides control signals to the microbeamformer **502** instructing the probe as to the timing, frequency, direction and focusing of transmit beams. The beamformer controller also controls the beamforming of received echo signals by its coupling to analog-to-digital (A/D) converters **316** and a beamformer **116**. Echo signals received by the probe are amplified by preamplifier and TGC (time gain control) circuitry **314** in the scanner, then digitized by the A/D

converters **316**. The digitized echo signals are then formed into beams by a beamformer **116**. The echo signals are processed by an image processor **318** which performs digital filtering, B mode detection, and Doppler processing, and can also perform other signal processing such as harmonic separation, speckle reduction through frequency compounding, and other desired image processing.

[0019] The echo signals produced by the scanner **310** are coupled to the digital display subsystem **320**, which processes the echo signals for display in the desired image format. The echo signals are processed by an image line processor **322**, which is capable of sampling the echo signals, splicing segments of beams into complete line signals, and averaging line signals for signal-to-noise improvement or flow persistence. The image lines are scan converted into the desired image format by a scan converter **324** which performs R-theta conversion as is known in the art. The image is then stored in an image memory **328** from which it can be displayed on a display **150**. The image in memory is also overlayed with graphics to be displayed with the image, which are generated by a graphics generator **330** which is responsive to the user control for the input of patient identifying information or the movement of cursors, for example. Individual images or image sequences can be stored in a cine memory **326** during capture of image loops.

[0020] For real-time volumetric imaging the display subsystem **320** also includes the 3D image rendering processor (not shown) which receives image lines from the image line processor **322** for the rendering of a real-time three dimensional image which is displayed on the display **150**.

[0021] In accordance with the principles of the present invention, the user interface **60** includes controls **62-66** for control of the orientation of the image plane scanned by the two dimensional array probe. When the user wants to rotate an image about its centerline the user does so by turning a control knob **66**. The lateral and elevational steering of the image plane are both "tilt" modes for purposes of this embodiment. The user toggles between the elevational tilt mode and the lateral tilt mode by depressing tilt key **64** on the user interface **60**. When the system is in the elevation tilt mode, the image plane can be manipulated as illustrated in **FIG. 2b** by rolling a trackball **62** to one side or the other. When the tilt key **64** is depressed the system switches to the lateral tilt mode and the user can move the image plane to the left or right laterally by manipulating the trackball **62**.

[0022] As the user manipulates these controls, signals from the controls are coupled to the beamformer controller **312**. The beamformer controller **312** responds to the user's selection of a new image plane orientation by programming the sequence of beams to be transmitted and received by the beamformer **116** or the microbeamformer **502** in a frame table. The beamformer controller reprograms a frame table for both images by recalculating or selecting the proper sequence of focusing coefficients for transmit and receive beamforming in the directions needed to scan the plane in the location specified by the user. The transmit beams are transmitted and focused in the desired directions through the volume in front of the transducer array **500** under control of a transmit beamformer in the microbeamformer **502** or the beamformer **116**. **FIG. 2d** shows the beam at the left side of the image plane **120** labeled "1" and the beam at the right side of the image plane labeled "128." The data of the frame



table causes the **128** beams of the image plane **120** to be transmitted, received and processed repetitively until the user changes the image plane orientation again or alters another imaging parameter. For instance, the user may be scanning blood flow in a color box in a particular area of the image, in which case Doppler ensembles will be transmitted to and received from the color box area for the processing and display of blood flow. The frame table contains the necessary data for the transmission and reception of the beams necessary to produce the desired image in the desired orientation.

[0023] The B mode echoes from each received scanline are processed by amplitude detection in the image processor **318**, and the Doppler echo ensembles are Doppler processed in the image processor for the production of display signals depicting flow or tissue motion. The processed B mode and/or Doppler signals are then coupled to the display subsystem **320** for display.

[0024] The selection of the desired image planes is also coupled to the display subsystem **320**, where the scan converter **324** and the graphics generator **330** are informed of the design of the images. This enables the scan converter to anticipate and then properly locate the Doppler information along the scanlines of a specified color box area, and enables the graphics generator to outline or highlight the color box if desired. The final image is then displayed on the display **150**.

[0025] **FIG. 4** illustrates an application of the present invention for imaging the heart **100**. Rather than image the heart transcostally through the ribs **110**, the probe **10** is placed against the skin **90** of the abdomen below the ribs. The probe is generally coupled to the body by an acoustic couplant (a gel) which is spread over the skin **90**. A good acoustic window is established when the image plane is imaging the interior of the body without obstruction of the ultrasonic waves. Usually the procedure will commence with the image plane directed in the conventional normal orientation to the probe, which is along axis **122** in the drawing. The probe is then held in place against the favorable acoustic window and the user interface is used to adjust the orientation of the plane. In this example the image plane **120** is tilted in the elevation direction so that it intersects the left ventricle **102** of the heart **100** which is below the ribs. The image plane may, if desired, be tilted laterally and/or rotated until it intersects the heart in the cross-section which is to be imaged. Thus, the clinician is able to acquire diagnostically useful images of an organ, the heart in this example, by manipulating the orientation of the image plane in the body while maintaining a favorable acoustic window with the body.

[0026] The present invention has particular utility for telemedicine, when a skilled diagnostician is not present at the patient's location. For instance, a medic can hold the ultrasound probe against the body of an accident victim who is suspected to have internal injuries or bleeding. The image data can be radioed or otherwise communicated to a facility where the image is displayed for a skilled diagnostician. The diagnostician can manipulate the user controls at his location, with the manipulation of the controls being communicated back to the ultrasound system at the site of the accident. The orientation of the image plane is adjusted correspondingly. While the medic holds the probe stationary

against the accident victim, the diagnostician can manipulate the image plane remotely to survey the suspected injury area and recommend treatment from the remote location. An ultrasound system by which the user controls can be operated remotely for such a procedure is described in U.S. Pat. No. 5,715,823.

[0027] While the present invention finds great utility when embodied in transthoracic and other probes which are intended to be used from outside the body, indwelling probes may also benefit from the present invention. For example, a TEE probe may be fabricated with the ability to steer the plane orientation as described above. Multiplane (omniplane) TEE probes provide the ability to reorient the image plane by moving the probe up and down in the esophagus, twisting the insertion tube in the esophagus, articulating the probe tip, and rotating the array transducer. However, even greater versatility is provided by providing the degrees of freedom of image plane orientation of the present invention, which can also obviate the need for some of the mechanical plane adjustments presently needed for TEE probes.

[0028] Although the user controls in the embodiment of **FIG. 3** are shown located on an ultrasound system user interface, it will be appreciated that the user controls may also be located on the probe. This would enable the user to manipulate the image plane orientation from the probe, without the need to access the ultrasound system scanner or cart.

[0029] The ultrasound image on the display **150** may also be accompanied by an icon which depicts the position of the image plane with respect to the probe. Icons such as those shown in the parent application 10/437,834 or similar icons may be used for this purpose.

What is claimed is:

1. A method of ultrasonically imaging with a two-dimensional array transducer a region of interest of a body which may be obstructed from the view of an image plane extending normal to the face of a transducer comprising:

placing the probe in contact with the body to create an acceptable acoustic window for the probe; and

tilting the image plane from its normal orientation to the face of the transducer to image a region of interest while maintaining the acoustic window.

2. The method of claim 1, wherein placing further comprises using an acoustic gel to create an acceptable acoustic window.

3. The method of claim 1, wherein tilting further comprises manipulating an ultrasound system control to steer the image plane toward the region of interest while maintaining the probe stationary with respect to the acoustic window of the body.

4. The method of claim 3, wherein tilting comprises one of steering the image plane in an elevation plane different from a plane normal to the face of the transducer, or steering the plane laterally with respect to a plane centered about an axis centered with respect to the face of the transducer.

5. The method of claim 4, further comprising rotating the image plane about an axis of the image plane.

6. The method of claim 3, wherein tilting further comprises manipulating a control of an ultrasound system which is remotely located from the location of the probe.

7. The method of claim 6, wherein the control comprises a plurality of control devices.

8. The method of claim 7, wherein at least one of the control devices comprises a trackball control device.

9. A method of ultrasonically imaging with a two-dimensional array transducer probe a region of interest of a body which may be obstructed from the view of an image plane which is fixed in a normal orientation to the face of a transducer comprising:

placing the probe in contact with the body to create an acceptable acoustic window for the probe; and

manipulating the image plane from its normal orientation to the face of the transducer by two or more of the actions of rotating the image plane about an axis, moving the image plane laterally from a center axis, and tilting the image plane in the elevation direction.

10. The method of claim 9, wherein manipulating is performed while maintaining the array transducer in a substantially stationary position with respect to the body.

11. The method of claim 9, wherein manipulating further comprises manipulating a control of an ultrasound system to effect the actions.

12. The method of claim 11, wherein the control comprises a plurality of control devices.

13. The method of claim 11, wherein manipulating further comprises manipulating a control of an ultrasound system which is located on the probe to effect the actions.

14. The method of claim 9, wherein manipulating further comprises manipulating a control of an ultrasound system which is remotely located from the location of the probe.

15. The method of claim 11, wherein at least one of the control devices comprises a trackball control device.

\* \* \* \* \*

专利名称(译)	具有转向图像平面的超声诊断成像		
公开(公告)号	<a href="#">US20030208124A1</a>	公开(公告)日	2003-11-06
申请号	US10/448518	申请日	2003-05-30
[标]申请(专利权)人(译)	波兰MCKEE DUNN		
申请(专利权)人(译)	波兰MCKEE DUNN		
当前申请(专利权)人(译)	皇家飞利浦电子N. V.		
[标]发明人	POLAND MCKEE DUNN		
发明人	POLAND, MCKEE DUNN		
IPC分类号	G01S7/52 G01S15/89 A61B8/00		
CPC分类号	G01S7/52046 G01S7/52063 G01S7/52073 G01S7/52074 G01S15/8993 G01S7/52085 G01S15/8925 G01S15/8936 G01S7/5208		
其他公开文献	US7037264		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

#### 摘要(译)

二维阵列换能器探头用于对身体的区域进行成像，所述区域在诸如肺或肋之类的物体的声学上被传统视野阻挡。探头在声窗处靠着身体定位，在换能器阵列和身体之间提供可接受的超声波透射率。在将探头保持在其声窗口的同时，通过调节光束转向方向来操纵图像平面位置。图像平面可以在仰角方向上倾斜，横向移动和/或围绕中心轴旋转以定位图像平面，从而有效地对阻塞的解剖结构进行成像以用于诊断。

