



US010209352B2

(12) **United States Patent**  
**van Rens**

(10) **Patent No.:** **US 10,209,352 B2**  
(45) **Date of Patent:** **Feb. 19, 2019**

(54) **ULTRASOUND TRANSDUCER ASSEMBLY**

(52) **U.S. Cl.**

(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,  
Eindhoven (NL)

CPC ..... **G01S 7/52047** (2013.01); **A61B 8/0883**  
(2013.01); **A61B 8/4488** (2013.01); **G01S**  
**7/5208** (2013.01); **G01S 15/8915** (2013.01);  
**G01S 15/8993** (2013.01); **G10K 11/346**  
(2013.01)

(72) Inventor: **Antonia Cornelia van Rens**, Nuenen  
(NL)

(58) **Field of Classification Search**

CPC ..... G01S 7/52; G01S 15/8993; G01S 7/5208;  
G01S 15/8915; A61B 8/4488; A61B  
8/0883; G10K 11/346

(73) Assignee: **Koninklijke Philips N.V.**, Eindhoven  
(NL)

USPC ..... 73/625  
See application file for complete search history.

(\* ) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 109 days.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

(21) Appl. No.: **15/314,301**

4,140,022 A 2/1979 Maslak  
4,790,320 A 12/1988 Perten et al.  
(Continued)

(22) PCT Filed: **Jun. 8, 2015**

(86) PCT No.: **PCT/EP2015/062709**

§ 371 (c)(1),

(2) Date: **Nov. 28, 2016**

**FOREIGN PATENT DOCUMENTS**

EP 2944976 A1 11/2015

(87) PCT Pub. No.: **WO2015/189149**

PCT Pub. Date: **Dec. 17, 2015**

*Primary Examiner* — J M Saint Surin

(65) **Prior Publication Data**

US 2018/0180726 A1 Jun. 28, 2018

(57) **ABSTRACT**

An ultrasound transducer assembly (30) is disclosed, comprising: a plurality of ultrasound transducer elements (34, 36, 38) for receiving ultrasound waves and for providing transducer signals (X2, X3, X4) corresponding to the respectively received ultrasound waves. The assembly comprises a plurality of signal combiners (42, 44; 60, 62, 64) for providing different output signals (Y1, Y2) on the basis of the transducer signals, and a plurality of timing elements (48, 52; 68, 70; 72, 74) for providing different time shifts ( $\tau$ ) to the transducer signals. Each of the ultrasound transducer elements is connected to a plurality of the signal combiners for providing the transducer signals including the different time shifts to different of the signal combiners.


(30) **Foreign Application Priority Data**

Jun. 12, 2014 (EP) ..... 14172046

(51) **Int. Cl.**

**A61B 8/08** (2006.01)  
**G10K 11/34** (2006.01)  
**G01S 7/52** (2006.01)  
**A61B 8/00** (2006.01)  
**G01S 15/89** (2006.01)

**15 Claims, 6 Drawing Sheets**

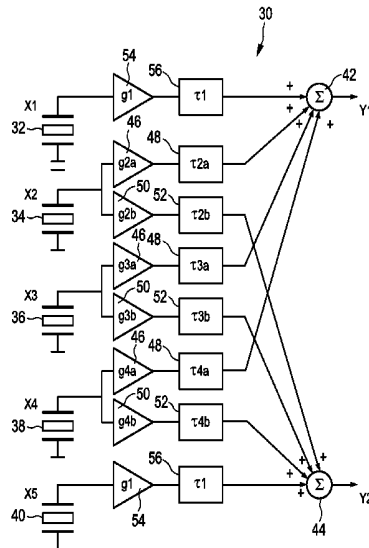

(56)

**References Cited**

U.S. PATENT DOCUMENTS

5,544,655 A \* 8/1996 Daigle ..... G01S 7/52095  
600/447  
5,676,147 A 10/1997 Petrofsky et al.  
5,832,923 A 11/1998 Engeler et al.  
5,908,390 A \* 6/1999 Matsushima ..... G01S 7/52023  
600/447  
5,997,479 A 12/1999 Savord et al.  
8,194,876 B2 \* 6/2012 Kim ..... H04B 13/005  
381/151  
8,690,782 B2 \* 4/2014 Colby ..... G01S 7/52023  
600/437  
2015/0025385 A1 \* 1/2015 Ikeda ..... A61B 8/5207  
600/443

\* cited by examiner

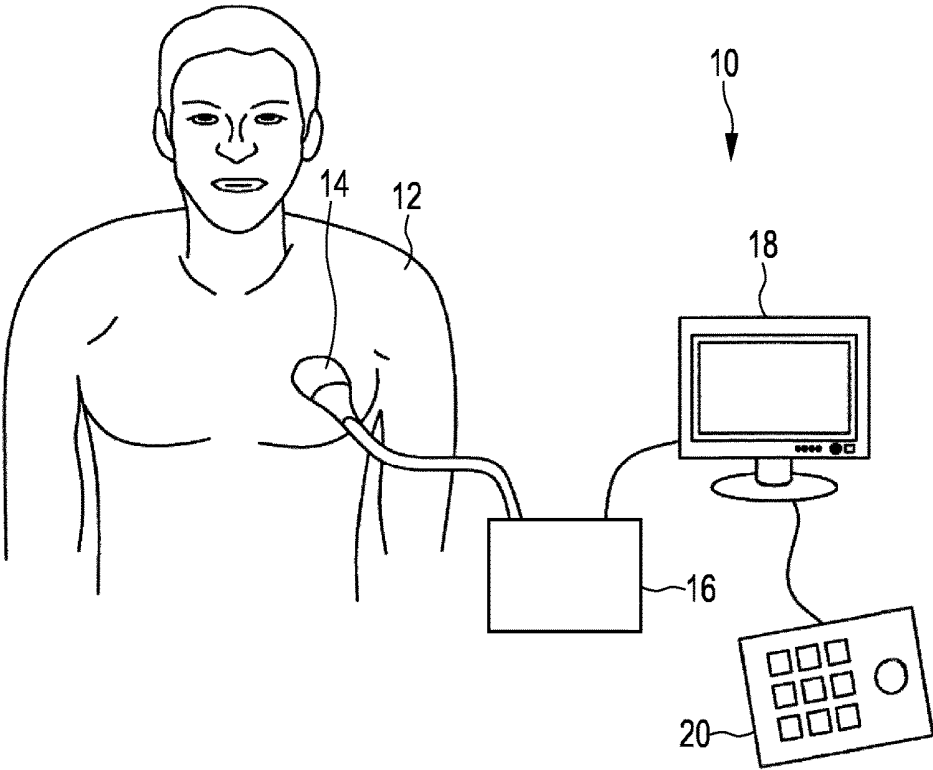


FIG. 1

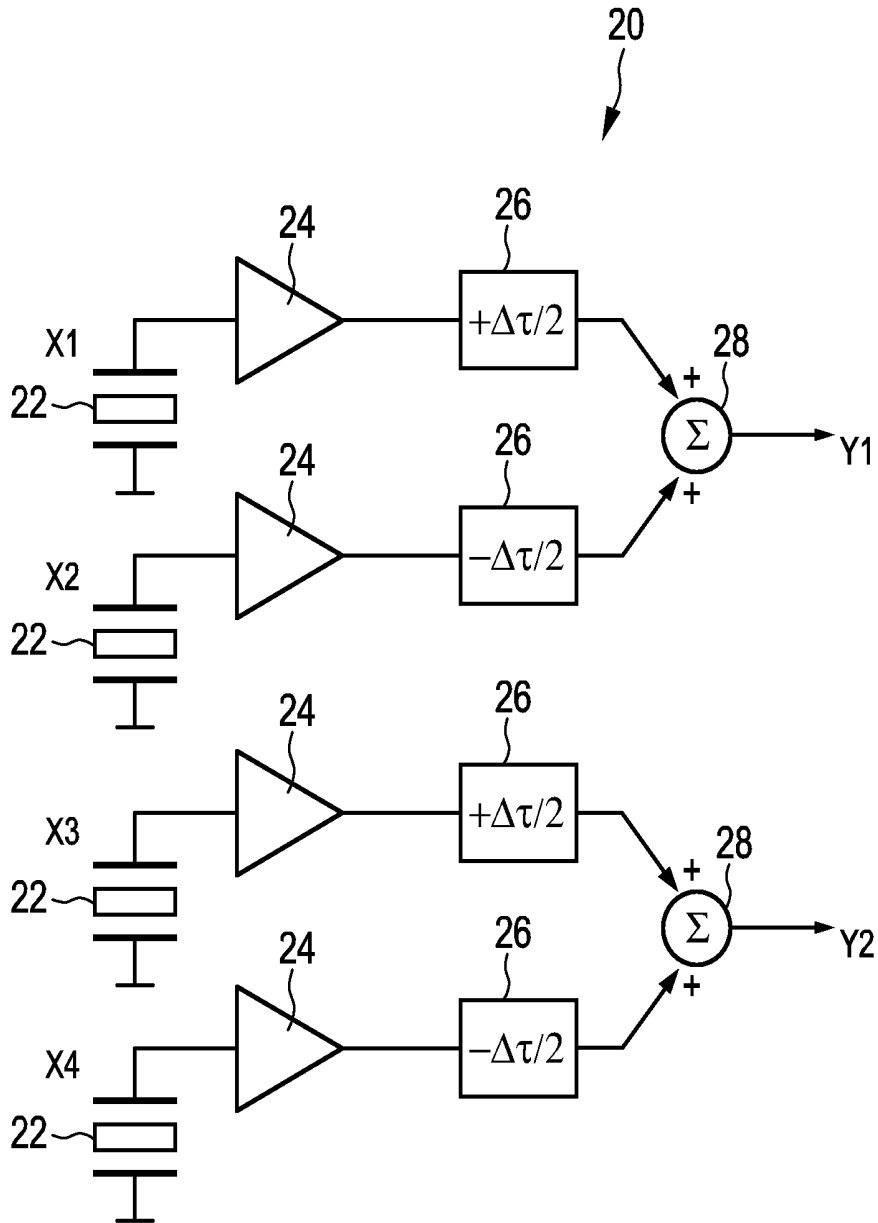


FIG. 2

-prior art-

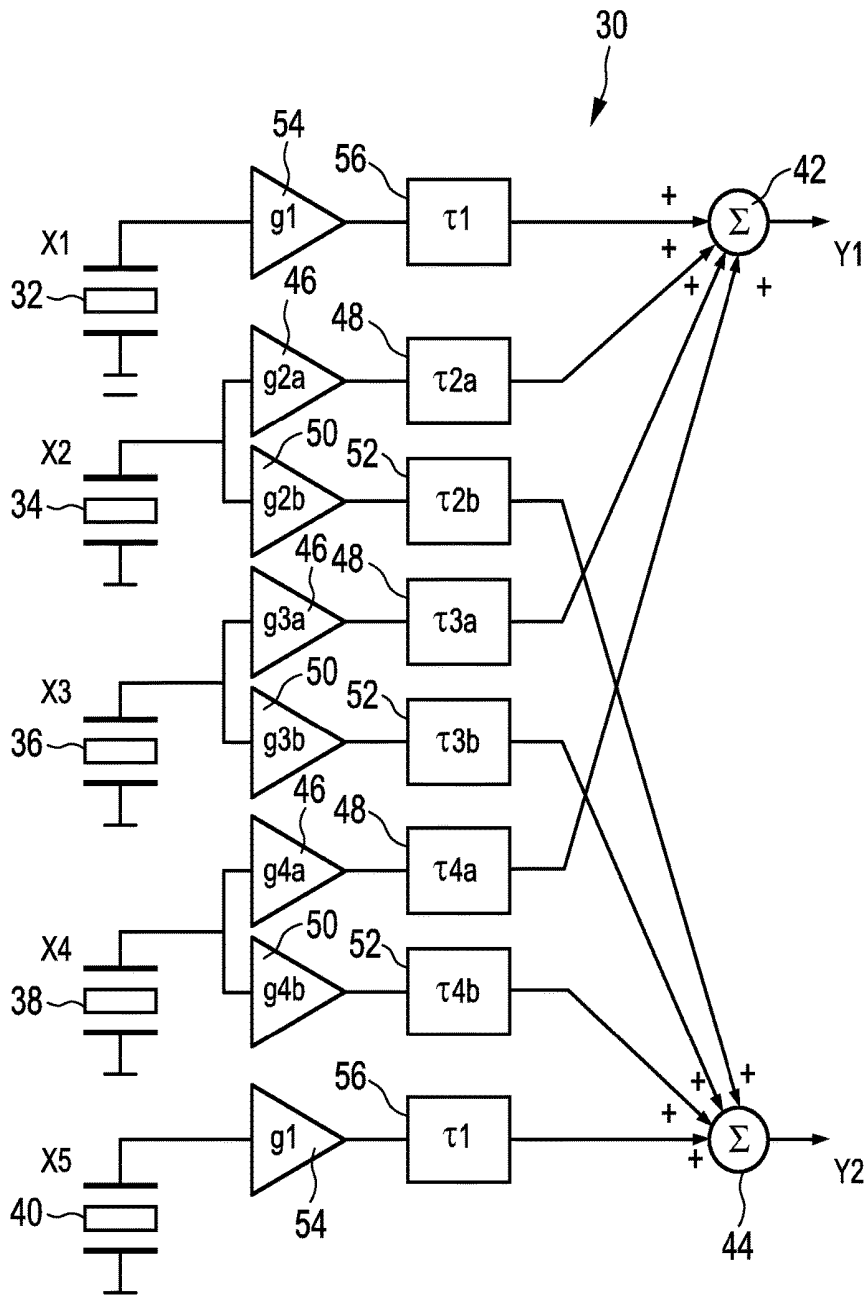


FIG. 3

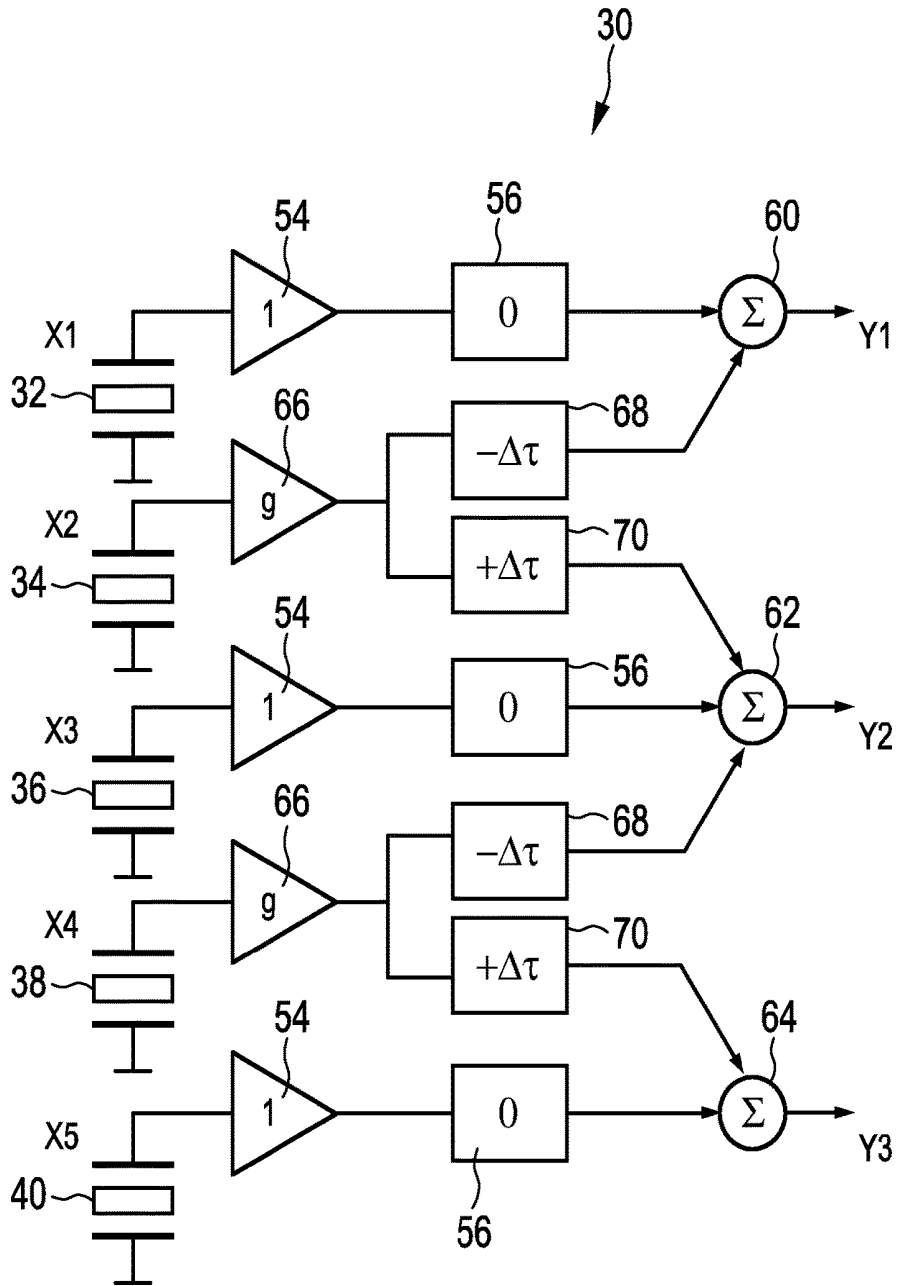


FIG. 4

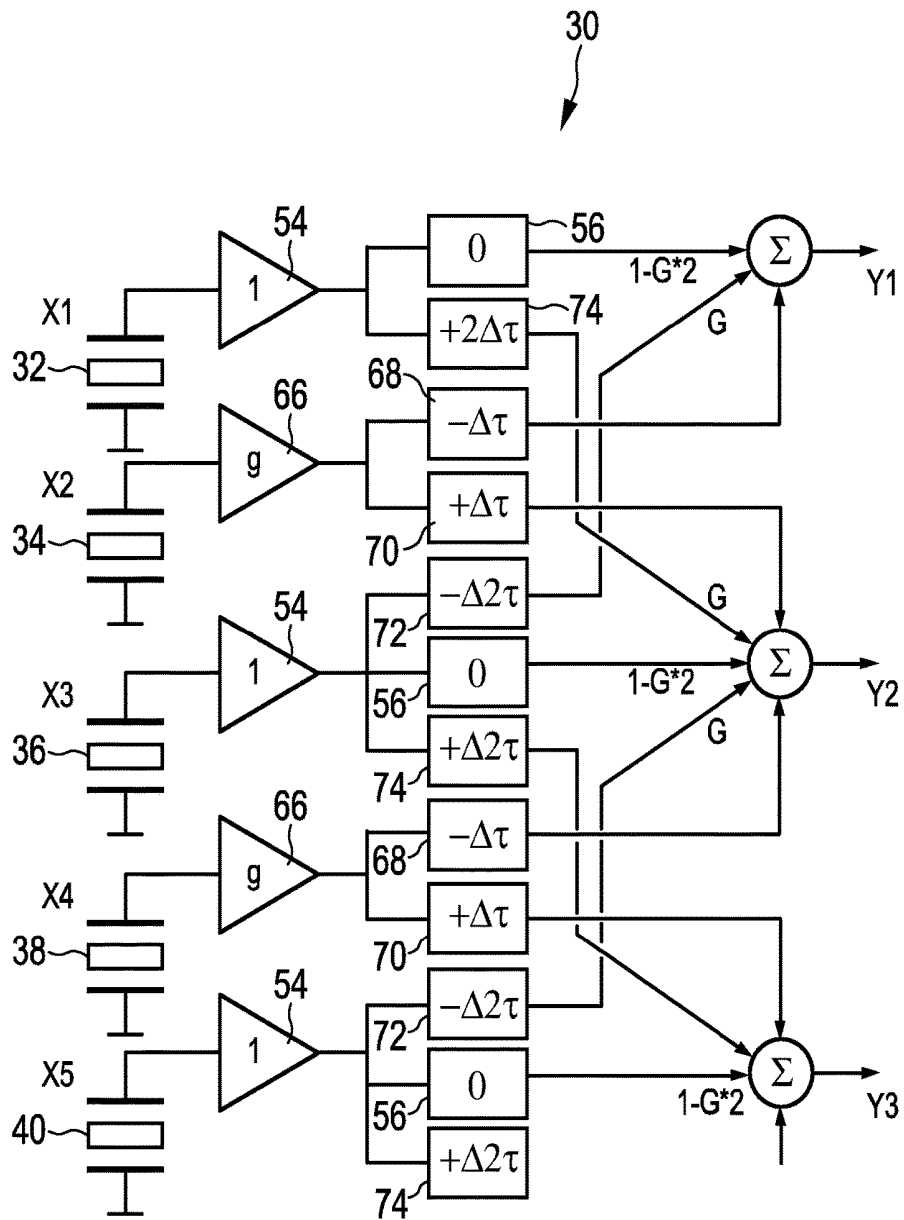


FIG. 5

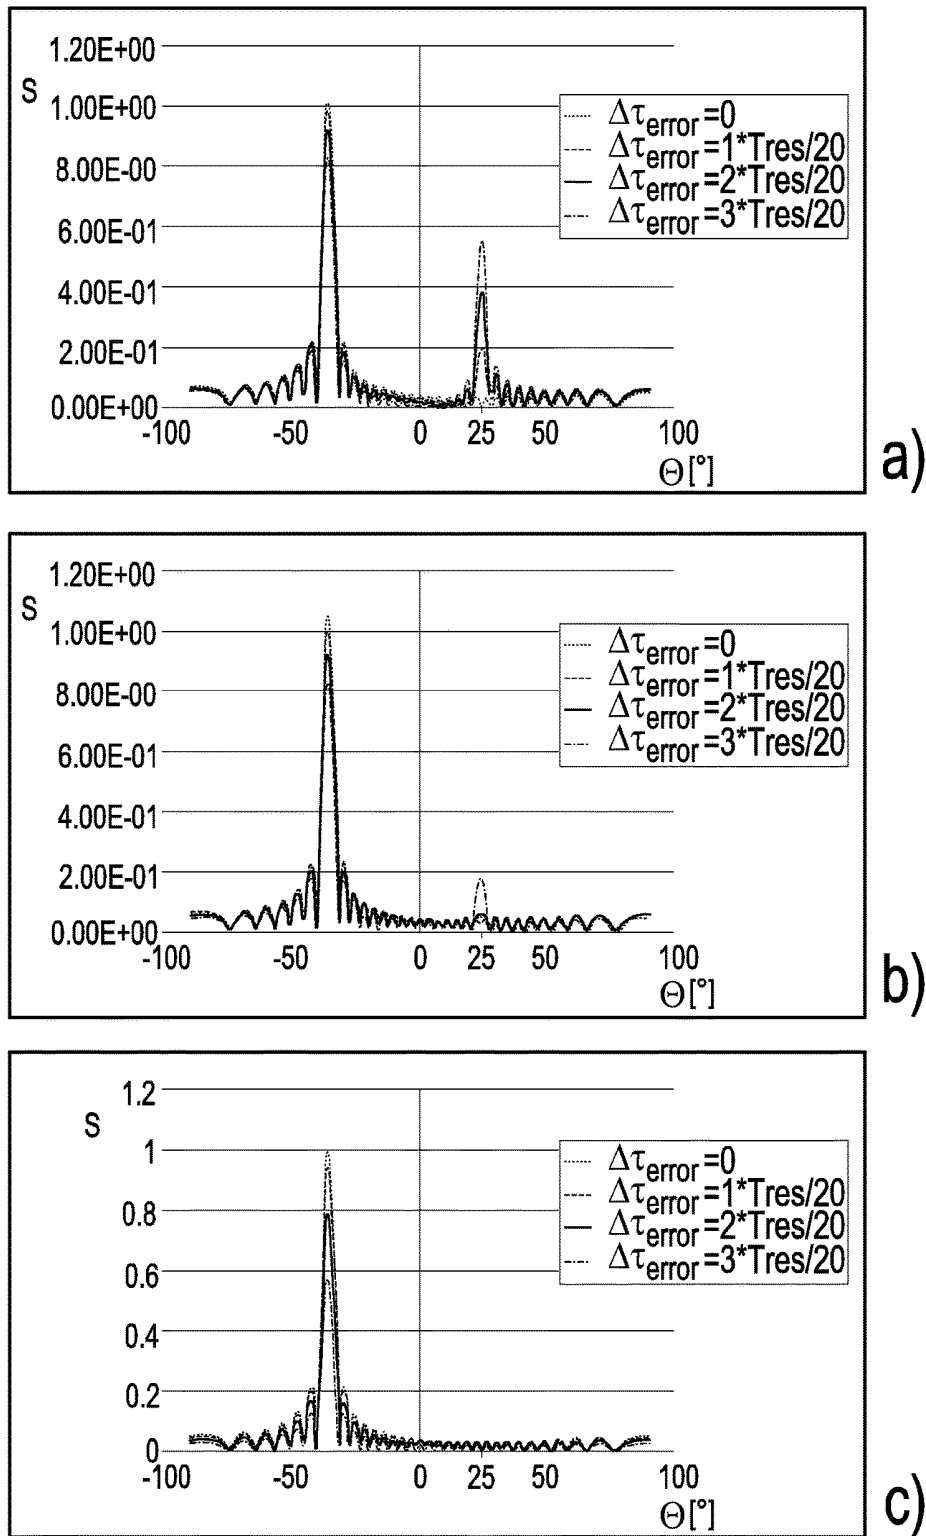


FIG. 6

## ULTRASOUND TRANSDUCER ASSEMBLY

This application is the U.S. National Phase application under 35 U.S.C. § 371 of International Application No. PCT/EP2015/062709, filed on Jun. 8, 2015, which claims the benefit of European Application Serial No. 14172046.6, filed Jun. 12, 2014. These applications are hereby incorporated by reference herein.

## FIELD OF THE INVENTION

The present invention relates to an ultrasound transducer assembly, in particular an ultrasound beamformer for receiving ultrasound waves.

The present invention further relates to an ultrasound imaging system, in particular for in-body ultrasound imaging like cardiovascular or transesophageal echocardiography imaging.

## BACKGROUND OF THE INVENTION

Ultrasound imaging systems are generally known producing real-time images of internal portions of a tissue of a human body or the like. Such imaging systems include a multiple channel transmit beamformer and a multiple channel receive beamformer either coupled to a single array of ultrasonic transducers using a transmit and receive switch or coupled separately to a transmit transducer array and a receive transducer array. The transmit beamformer generates timed electrical pulses and applies them to individual transducer elements to generate an ultrasound beam to a portion of interest to be analyzed. A portion of the acoustic energy is scattered back towards the transducer array from the tissues structures. An array of received transducers, which may be the same as the transmit transducers converts the pressure pulses into corresponding electrical pulses. The receive beamformer usually has a plurality of processing channels with compensating delay elements, wherein a delay value for each channel is selected to collect ultrasound waves from a selected area of interest or from a selected steering direction.

A corresponding ultrasound receive beamformer with phased sub-arrays is e.g. known from U.S. Pat. No. 5,676,147.

The ultrasound penetration depth and, therefore, the area of interest is inversely proportional to the resonance frequency of the ultrasound waves, so that the field of view is close to the transducer array for high ultrasound frequencies. In order to provide high quality images of a field of view, fine and precise timing delays are required for these high ultrasound frequencies. Further, parasitic system-related time delays have an increased impact on the final image quality for these frequencies.

U.S. Pat. No. 4,790,320 discloses an apparatus for parallel processing of ultrasonic information to derive simultaneously multiple vectors of ultrasonic information per ultrasonic transmission. The apparatus includes in a transducer array for each transducer element an analog to digital converter and a delay processing subsystem associated with each analog to digital converter. The output of each first incremental delay means of all of the delay processing subsystems is applied to a first summing network and, simultaneously, the output of each of the second incremental delay means is applied to a second summing network which produces a second vector of time synchronized echo information.

## SUMMARY OF THE INVENTION

It is an object of the present invention to provide an improved ultrasound transducer assembly providing a higher image quality with low technical effort.

It is furthermore an object of the present invention to provide a corresponding ultrasound imaging system.

In a first aspect of the present invention, an ultrasound transducer assembly is presented that comprises:

10 a plurality of ultrasound transducer elements for receiving ultrasound waves and for providing transducer signals corresponding to the respectively received ultrasound waves,

a plurality of signal combiners for providing different output signals on the basis of the transducer signals, and

15 a plurality of timing elements for providing different time shifts to the transducer signals,

wherein each of the ultrasound transducer elements is connected to a plurality of the signal combiners for providing the transducer signals including the different time shifts to different of the signal combiners, respectively.

In a further aspect of the present invention, ultrasound imaging system is presented comprising an ultrasound transducer array including a plurality of ultrasound transducer elements for transmitting and receiving ultrasound waves and an ultrasound transducer assembly of this kind.

Preferred embodiments of the invention are defined in the dependent claims.

The present invention is based on the idea to provide an ultrasound transducer assembly having a plurality of transducer elements, wherein different transducer signals of the transducer elements are differently time shifted and provided to different signal combiners. Parasitic delays or timing errors of the transducer signals can be compensated when the different output signals of the signal combiners are combined. Hence, a time delay of the transducer signals leads to a small amplitude error of the micro-beamformed output signal of the transducer assembly but not to a steering angle error so that the image quality of the overall beamformer can be improved with low technical effort.

The plurality of ultrasound transducer elements, which are each connected to a plurality of the signal combiners form a group of first transducer elements of the ultrasound transducer assembly.

In a preferred embodiment, each of the ultrasound transducer elements is connected to a plurality of the timing elements for providing the different time shifts to each of the transducer signals. This is a possibility to achieve individual time shifts and to provide the transducer signal including the different time shifts to the different signal combiners.

In a preferred embodiment, a plurality of secondary transducer signals is formed from the transducer signal of each of the ultrasound transducer elements and wherein each of the split transducer signals is provided to one of the signal combiners, respectively. The secondary transducer signals are identical to the transducer signals and preferably formed by splitting or copying the transducer signal. Since the transducer signals of each of the transducer elements are provided to different signal combiners and since the transducer signals are differently time shifted, the timing errors and/or propagation delays included in the transducer signals can compensate each other, effectively.

In a preferred embodiment, the signal combiners each comprise an adder. This is a possibility to combine the plurality of transducer signals with a low technical effort.

In a preferred embodiment, the transducer signals of the plurality of transducer elements provided to the different signal combiners are weighted by means of different weight

factors. This is a possibility to adjust the output signals combined at the signal combiners individually, since the differently time shifted transducer signals can be weighted individually. By means of the different weight factors a precise compensation of the timing errors can be achieved.

In a preferred embodiment, an amplifier or an attenuator device is associated to each of the transducer elements to provide different gain factors to the transducer signals. It shall be understood that the gain factors may be larger than one or smaller than one so that the transducer signals are either attenuated or amplified. This is a further possibility to individually set the transducer signals to an individual value so that a precise compensation of the error delays and an improved imaging can be achieved.

In a preferred embodiment, the gain factors of the transducer signals provided to one of the signal combiners having different absolute values. This is a possibility to individually set the output signal of the different signal combiners to an optimal combination of the transducer signal.

In a preferred embodiment, the ultrasound transducer assembly further comprises a second plurality of transducer elements, wherein a delay element is associated to each of the second plurality of transducer elements for providing a fixed time delay to the respective transducer signals of the second plurality of transducer elements. This is a possibility to achieve positive and negative time shifts to the individual transducer signals since a fixed time delay is provided to all transducer signals.

In a preferred embodiment, each of the second plurality of transducer elements is connected to one of the signal combiners. The second plurality of transducer elements form a second group of transducer elements of the ultrasound transducer assembly. These transducer elements can form a reference signal for the first transducer elements which are connected to two of the signal combiners.

In a preferred embodiment, the plurality of second transducer elements and the respectively connected delay elements are virtual elements. This is a possibility to reduce the technical effort, since these reference elements can be simulated including the fixed time delay.

In a preferred embodiment, the time shift provided to the transducer signals include a fixed time delay and a relative time shift. This is a possibility to individually set the time shift to positive or negative values.

In a preferred embodiment, the relative time shift of the transducer signals provided to a first of the signal combiners is a positive time shift and the relative time shift of the transducer signals provided to a second of the signal combiners is a negative time shift. This is a possibility that the timing errors of the transducer signals can compensate each other, since the relative time shift provided to the signal combiners are positive and negative time shifts of the same transducer signals.

In a preferred embodiment, the time shifts of the transducer signals provided to one of the signal combiners have different absolute values. This is a further possibility to achieve a precise compensation of the timing errors.

In a further preferred embodiment, the time shifts of the transducer signals provided to one of the signal combiners are multiples of on first time shift.

In a further preferred embodiment, the time shifts of the transducer signals provided to different of the signal combiners have different polarities.

The plurality of signal combiners are connected to each other to combine the plurality of output signals to an overall output signal of the transducer assembly. This is a possibility

to achieve a single error-compensated output signal of the ultrasound transducer assembly.

In a further preferred embodiment, the plurality of ultrasound transducer elements are connected to the signal combiners in parallel to each other. This is a possibility to combine the transducer signals to different output signals so that a timing error compensation can be achieved.

As mentioned above, the ultrasound transducer assembly according to the present invention can compensate timing errors and/or parasitic delays of the transducer signals with low technical effort, since the transducer signals are individually time shifted and provided to different signal combiners, so that the timing errors are correspondingly compensated by each other in the resulting output signal. Hence, the timing errors lead only to an amplitude error of the micro-beamformed output signal but not in a steering angle error so that the image quality can be improved.

#### BRIEF DESCRIPTION OF THE DRAWINGS

These and other aspects of the invention will be apparent from and elucidated with reference to the embodiment(s) described hereinafter. In the following drawings

FIG. 1 shows a schematic representation of an ultrasound imaging system in use to scan a volume of a patient's body;

FIG. 2 shows a schematic block diagram of a known two-to-one channel receive beamformer of an ultrasound system;

FIG. 3 shows an embodiment of a receive beamformer for timing error compensation;

FIG. 4 shows a further embodiment of a two-to-one channel receive beamformer for timing error compensation;

FIG. 5 shows a further embodiment of a two-to-one channel receive beamformer; and

FIG. 6 shows different sensitivity diagrams for different receive beamformers and different timing errors.

#### DETAILED DESCRIPTION OF THE INVENTION

FIG. 1 shows a schematic illustration of an ultrasound system **10** according to an embodiment, in particular a medical three-dimensional (3D) ultrasound imaging system. The ultrasound imaging system **10** is applied to inspect a volume of an anatomical site, in particular an anatomical site of a patient **12**. The ultrasound system comprises an ultrasound probe **14** having at least one transducer array having a multitude of transducer elements for transmitting and/or receiving ultrasound waves. In one example, the transducer elements each can transmit ultrasound waves in form of at least one transmit impulse of a specific pulse duration, in particular a plurality of subsequent transmit pulses. The transducer elements may be arranged in a one-dimensional array or a two-dimensional array, in particular for providing a multi-planar or three-dimensional images.

An ultrasound scan typically involves emitting ultrasound waves that illuminate a particular volume within a body, which may be designated as target volume. This can be achieved by emitting ultrasound waves at multiple different angles. A set of volume data is then obtained by receiving and processing reflected waves. A steering of the ultrasound transducer is achieved by a receive beamformer which provides individual delays to the individual ultrasound signals.

It shall be understood that the ultrasound probe **14** may either be used in a non-invasive manner (as shown in FIG. 1) or in an invasive manner (not shown) as this is usually

done in two-dimensional transesophageal echocardiography (TEE). The ultrasound probe **14** may be hand-held by the user of the system, for example medical staff or a doctor. The ultrasound probe **14** is supplied to the body of the patient **12** so that an image of an anatomical site, in particular an anatomical object of the patient **12** is provided.

Further, the ultrasound system **10** may comprise a control unit **16** that controls the provision of ultrasound image via the ultrasound system **10**. A control unit **16** controls the acquisition of data via the transducer array of the ultrasound probe **14** and controls the signal and image processing that form the ultrasound images out of the echoes of the ultrasound beams received by the transducer array of the ultrasound probe **14**.

The ultrasound system **10** may further comprise a display **18** for displaying the 3D images to the user. Still further, an input device **20** may be provided connected to the display **18** or directly to the control unit **16**.

The ultrasound system **10** comprises in general a beamformer, which is provided for steering the transducer elements to a focal point within the anatomical site to be inspected. The individual transducer elements are steered to the focal point by providing individual time delays to the transducer signals so that the transit time of the ultrasound waves from the focal point to the different transducer elements can be compensated. By means of these individual time delays provided by the beamformer, a steered ultrasound transducer can be provided.

The beamformer comprises a micro-beamformer, which is located in the ultrasound probe **14** close to the transducer array. The beamformer may further comprise a system-beamformer integrated in the control unit **16** and connected to the micro-beamformer for coarse beamforming. The ultrasound system **10** further comprises an analog-to-digital converter (ADC), which is preferably connected between the micro-beamformer and the system-beamformer.

FIG. 2 shows an ultrasound transducer known from the prior art which is generally denoted by **20**. The ultrasound transducer **20** comprises a two-to-one channel receive micro-beamformer which is adapted to reduce the effects of timing errors by combining differently time shifted signals. The ultrasound transducer **20** comprises a plurality of transducer elements **22**, which are adapted to receive ultrasound waves and to transform the ultrasound waves into an electrical transducer signal X1-X4. The transducer elements **22** are each connected to an amplifier **24** for amplifying the electrical transducer signals X1-X4, wherein the amplifiers **24** are preferably formed as operational amplifiers. The transducer elements **22** are each further connected to a timing element **26**, which are adapted to provide a defined time shift to the electrical signals X1-X4 received from the transducer elements **22**. Two of the transducer elements **22** are connected to one signal adder **28** in order to combine the electrical signals to one output signal Y1, Y2 which are combined by a coarse beamformer to an overall output signal of the ultrasound transducer (not shown).

The timing elements **26**, which are connected to one of the signal adders **28** are adapted to provide a positive and a negative time shift to the electrical transducer signals X1-X4, respectively, so that timing errors can be compensated at the signal adder **28**. In practice, all timing elements **26** provide a fixed positive time delay to the electrical transducer signals X1-X4 and the additional relative time shift so that a positive and a negative time shift can be implemented.

The disadvantage of these standard two-to-one channel receive beamformers is that the time delay must be set very

precisely and that a grating lobe is generated already for moderate timing errors so that the resulting image quality is affected.

FIG. 3 shows an ultrasound transducer assembly according to one embodiment of the present invention which is generally denoted by **30**. The ultrasound transducer assembly **30** comprises a plurality of transducer elements **32, 34, 36, 38, 40** for receiving ultrasound waves and for providing electrical transducer signals, which are generally denoted by X1, X2, X3, X4, X5. The ultrasound transducer assembly **30** further comprises in general an ultrasound beamformer connected to the ultrasound transducer elements **32-40**. The ultrasound beam former shown in FIG. 3 is formed as a four-to-one channel micro-beamformer. The ultrasound beamformer provides steering and focussing of the ultrasound transducer elements **32-40** to a point by providing a time shift to the electrical transducer signals X1-X5 as described in the following. The ultrasound transducer elements **32-40** may be arranged in a one-dimensional or a two-dimensional array of transducer elements in order to provide a two-dimensional or a three-dimensional ultrasound image.

The ultrasound transducer assembly **30** and in particular the ultrasound micro-beamformer comprises a first signal combiner **42** and a second signal combiner **44** which provide a first output signal Y1 and a second output signal Y2. The signal combiners **42, 44** are formed as signal adders which combine electrical signals on the basis of the ultrasound transducer signals X1-X4 and X2-X5 to form the output signals Y1, Y2. The signal combiners **42, 44** are each connected to the transducer elements **34, 36, 38** so that the transducer elements **34, 36, 38** are connected in parallel to each other.

The transducer elements **34, 36, 38**, which form a first group of transducer elements are each connected via a first gain element **46** and a first timing element **48** to the first adder **42**. The transducer elements **34, 36, 38** are further connected via a second gain element **50** and a second timing element **52** to the second signal combiner **44**. A plurality—in this case—two secondary ultrasound signals are formed of the ultrasound transducer signals X2, X3, X4 preferably by splitting or copying the ultrasound transducer signals X2, X3, X4 and the secondary signals are provided with a gain factor  $g$  by means of the gain elements **46, 50** to the timing elements. The secondary ultrasound signals are identical to the respective ultrasound transducer signals X2, X3, X4. The secondary transducer signals are further provided with a time shift  $\tau$  by means of the timing elements **48, 52**. The gain elements **46, 50** and the timing elements **48, 52** provide different gain factors and different time shifts  $\tau$  to the ultrasound transducer signals X2-X4 corresponding to the position of the respective transducer element **34-36** and corresponding to which of the signal combiners **42, 44** the respectively gained and time shifted signal is provided.

The transducer elements **32, 40** are each connected via a gain element **54** and a timing element **56** to only one of the signal combiners **42, 44**. The transducer elements **32, 40**, which are respectively connected to one of the signal combiners **42, 44** belong to a second group of transducer elements. The gain elements **54** provide a reference gain to the respective ultrasound transducer signal X1, X5 and the timing elements **56** provide a fixed time delay  $\tau_1$  to the ultrasound transducer signal X1, X5. The first and the second timing elements **48, 52** each provide the fixed delay  $\tau_1$  to the respective ultrasound transducer signal X2, X3, X4 and an additional time shift, which is positive in the case of the first timing elements **48** and negative in the case of the

second timing elements **52**. Hence, the signals provided to the first signal combiner **42** have a negative time shift relative to the fixed time delay  $\tau_1$  and the signals provided to the second signal combiner **44** have a positive time shift with respect to the fixed delay  $\tau_1$ . The output signals **Y1, Y2** are finally combined e.g. by the system-beamformer to an overall output signal (not shown) of the transducer assembly **30**.

The signals provided to the signal combiners **42, 44** may be provided with a weight factor in order to weigh the respective signals individually so that the respective individual transducer signals **X1-X5** have an individual influence on the wave form of the output signals **Y1, Y2**.

Due to the combination of the differently time shifted and differently weighted ultrasound transducer signals **X1-X5** combined by different signal combiners **42, 44**, the resulting overall output signal is less sensitive to timing errors on the programmed delay profiles than the ultrasound beamformers known from the prior art.

The gain factors  $g$  and the time shifts  $\tau$  of the gain elements **46, 50, 54** and the timing elements **48, 52, 56** have different values. The time shifts and the gain factors primarily are:

$$\tau_1 = \text{fixed delay, sufficiently large to make all delays effectively positive}$$

$$\tau_{2a} = \tau_1 - \Delta\tau$$

$$\tau_{2b} = \tau_1 + (N-1)\Delta\tau$$

$$\tau_{3a} = \tau_1 - 2\Delta\tau$$

$$\tau_{3b} = \tau_1 + (N-2)\Delta\tau$$

$$\tau_{4a} = \tau_1 - 3\Delta\tau$$

$$\tau_{4b} = \tau_1 + (N-3)\Delta\tau$$

$$g_1 = \text{reference gain}$$

$$g_{2a} = (N-1)/N * g_1$$

$$g_{2b} = 1/N * g_1$$

$$g_{3a} = (N-2)/N * g_1$$

$$g_{3b} = 2/N * g_1$$

...

$$g_{Na} = 1/N * g_1$$

$$g_{Nb} = (N-1)/N * g_1,$$

wherein  $\Delta\tau$  is the incremental correction for the calculated signal propagation delay difference and  $N$  is the number of transducer elements **32-38** in a sub-channel, in this example  $N=4$ . The structure can be used to provide any  $N$ -to-1 channel receive beamformer with  $N$  being any natural number larger than one.

In a certain embodiment, the ADC may be integrated in the micro-beamformer and connected between the transducer elements and the gain elements **54, 46, 50**. In a certain embodiment, the ADC is preceded by a low noise amplifier with a fixed gain for all channels.

In a further embodiment, the transducer elements **32, 40** of the second group of elements which are only connected to one of the signal combiners **42, 44** can be implemented as virtual transducer elements, wherein the fixed time delay of

the first group of transducer elements are aligned to the fixed time delay of the virtual transducer elements.

In this case, the time shifts and the gain factors will primarily be:

$$\tau_1 = \text{fixed delay, sufficiently large to make all delays effectively positive}$$

$$\tau_{2a} = \tau_1 - 0.5 * \Delta\tau$$

$$\tau_{2b} = \tau_1 + (N-0.5)\Delta\tau$$

$$\tau_{3a} = \tau_1 - 1.5\Delta\tau$$

$$\tau_{3b} = \tau_1 + (N-1.5)\Delta\tau$$

$$\tau_{4a} = \tau_1 - 2.5\Delta\tau$$

$$\tau_{4b} = \tau_1 + (N-2.5)\Delta\tau$$

$$g_1 = \text{reference gain}$$

$$g_{2a} = (N)/(N+1) * g_1$$

$$g_{2b} = 1/(N+1) * g_1$$

$$g_{3a} = (N-1)/(N+1) * g_1$$

$$g_{3b} = 2/(N+1) * g_1$$

...

$$g_{Na} = (1)/(N+1) * g_1$$

$$g_{Nb} = (N)/(N+1) * g_1$$

wherein  $\Delta\tau$  is the incremental correction for the calculated signal propagation delay difference and  $N$  is the number of non-virtual (real) transducer elements **34, 36, 38** in a sub-channel (in this example,  $N=3$ ).

**FIG. 4** shows an embodiment of the ultrasound transducer assembly **30** including a two-to-one channel micro-beamformer. In this embodiment, the ultrasound transducer assembly **30** comprises three or more signal combiners **60, 62, 64**, which combine signals based on the ultrasound transducer signals **X1-X5** of two or three transducer elements **32-40**. The signal combiners **60, 62, 64** are preferably formed as signal adders and provide the output signals **Y1, Y2, Y3** of the micro-beamformer which are combined to an overall output signal by the (coarse) system-beamformer (not shown). In this embodiment, the transducer elements **32, 36, 40**, which belong to the second group of transducer elements are connected via the gain element **54** and the timing element **56** directly to one of the signal combiners **60, 62, 64**, respectively. The transducer elements **34, 38**, which belong to the first group of transducer elements are connected to a gain element **66** for providing a gain factor  $g$  to the respective ultrasound transducer signal **X2, X4**, wherein two separate secondary transducer signals are formed from the ultrasound transducer signals **X2, X4** including the gain factor  $g$ . The secondary transducer signals are formed by splitting or copying the transducer signals **X2, X4**, wherein the secondary transducer signals are identical with the secondary transducer signals except for the gain factor. The two secondary transducer signals are time shifted by means of a first timing element **68** and a second timing element **70**, respectively, wherein the two secondary transducer signals are provided to different of the signal combiners **60, 62, 64**. Consequently, the transducer elements **32, 36, 40** which belong to the second group of transducer elements and which are in this row the odd transducer elements are

directly connected to one of the signal combiners 60, 62, 64 and the transducer elements 34, 38 which are the even transducer elements are connected to two of the signal combiners 60, 62, 64.

As described above, the timing elements 56 provide a fixed delay  $\tau$  to the respective ultrasound transducer signal X1, X3, X5 and the timing elements 68, 70 provide the fixed delay  $\tau$  and additionally a relative time shift  $-\Delta\tau$ ,  $+\Delta\tau$  to the ultrasound transducer signals X2, X4, wherein the timing element 68 provide a negative time shift  $-\Delta\tau$  and the timing element 70 provide a positive time shift  $+\Delta\tau$  to the respective ultrasound transducer signal X2, X4.

Since the ultrasound transducer signals X2, X4 are differently time shifted and gained by means of the gain factor g, the overall output signal is less sensitive to timing errors on the programmed delay profiles than the beamformer known from the prior art so that a more precise steering and a more precise imaging of the transducer assembly can be achieved.

In a certain embodiment, the ADC may be integrated in the micro-beamformer and connected between the transducer elements and the gain elements 54, 56 (in practice, the ADC will be preceded by a low noise amplifier with a fixed gain for all channels in this case)

FIG. 5 shows a further embodiment of the ultrasound transducer assembly 30. In this embodiment, the transducer assembly 30 comprises the three or more signals combiners 60, 62, 64 which receive each signals on the basis of different ultrasound transducer signals X1-X5 provided by the different ultrasound transducer elements 32-40.

Identical with the embodiment of FIG. 4, the ultrasound transducer signals X2, X4 of the ultrasound transducer elements 34, 38 are provided with a gain factor g and split into two split signals, which are differently time shifted (positive and negative) by means of the timing elements 68, 70 and provided to the respectively neighbored signal combiner 60, 62, 64.

The ultrasound transducer signals X1, X3, X5 of the ultrasound transducer elements 32, 36, 40 are provided with a gain factor g by means of the gain element 54 and split into two or three split signals, wherein one split signal is provided with the fixed time delay by means of the timing element 56 and the so delayed signal is provided to one of the signal combiners 60, 62, 64. The other split signals are time shifted by means of a first timing element 72 and a second timing element 74, wherein the so differently time shifted signals are provided to different of the signal combiners 60, 62, 64. The first timing elements 72 provide the fixed time delay  $\tau$  and a negative time shift to the respective split signal and the second timing elements 74 provide the fixed delay  $\tau$  and a positive time shift to the split signal. In this certain embodiment, three secondary transducer signals are formed of the ultrasound transducer signals X3, X5 by splitting or copying and provided with different time shifts to three of the signal combiners, wherein the ultrasound transducer signals X2, X4 are split into two split signals and provided with different time shifts to two of the signal combiners 60, 62, 64.

Additionally the split signals are weighted by means of weight factors (G, 1-2G) at the signal combiners 60, 62, 64 in order to individually form the output signals Y1, Y2, Y3 on the basis of the ultrasound transducer signals X1-X5. Since the signals of three or more transducer elements 32-40 are combined at the signal combiners 60, 62, 64, the micro-beamformer output signal provided by this embodiment of the ultrasound transducer assembly is less sensitive to timing errors on the programmed delay profiles than a simple two-to-one channel micro-beamformer.

In a certain embodiment, the ADC may be integrated in the micro-beamformer and connected between the trans-

ducer elements and the gain elements 54, 66 and in practice, the ADC is preferably preceded by a low noise amplifier with a fixed gain for all channels in this case.

In the following, the amplitude of grating lobes of the overall output signal of the ultrasound transducer assembly 20 of FIG. 2 and the ultrasound transducer assemblies 30 of FIGS. 4 and 5 are calculated in order to determine the sensitivity to programmed timing errors.

In practice the generated micro-beamformer delay will not be exactly equal to the desired delay. The difference between the two delays is  $\Delta\tau_{\text{error}}$ :

$$+\Delta\tau_{\text{gen}} = +\Delta\tau + \Delta\tau_{\text{error}}$$

$$-\Delta\tau_{\text{gen}} = -\Delta\tau - \Delta\tau_{\text{error}}$$

Note that it is assumed that the error on the positive delay is equal in magnitude but with a negative sign relative to the error on the negative delay. This is realistic since the delays are generated on the same ASIC using the same type of circuitry.

It is assumed that the ultrasound reflections of the two transducer elements can be modeled by a narrowband signal around the resonance frequency  $\omega_{\text{RES}}$  according to:

$$X1(t) = A(t - \Delta\tau_{\text{real}}/2) * \sin(\omega_{\text{RES}}(t - \Delta\tau_{\text{real}}/2))$$

$$X2(t) = A(t + \Delta\tau_{\text{real}}/2) * \sin(\omega_{\text{RES}}(t + \Delta\tau_{\text{real}}/2))$$

With  $+\Delta\tau_{\text{real}}$ =signal propagation delay difference of ultrasound signals X1 and X2 for the actual reflection and  $+\Delta\tau$  if the actual reflection arrives from the steering and focusing direction

$$A(t) = \text{amplitude of the envelope as a function of time.}$$

The output signal Y1\_1 of the ultrasound transducer assembly shown in FIG. 2 (prior art) can be described as follows:

$$\begin{aligned} Y1_1(t) &= X1(t + \Delta\tau_{\text{gen}}/2) + X2(t - \Delta\tau_{\text{gen}}/2) \\ &= A(t - \Delta\tau_{\text{real}}/2 + \Delta\tau_{\text{gen}}/2) * \sin(\omega_{\text{RES}}(t - \Delta\tau_{\text{real}}/2 + \\ &\quad \Delta\tau_{\text{gen}}/2)) + A(t + \Delta\tau_{\text{real}}/2 - \Delta\tau_{\text{gen}}/2) * \\ &\quad \sin(\omega_{\text{RES}}(t + \Delta\tau_{\text{real}}/2 - \Delta\tau_{\text{gen}}/2)) \end{aligned}$$

For acoustic energy coming from the steering direction (Y1\_1s), this formula can be rewritten to:

$$\begin{aligned} Y1_1s(t) &= A(t + \Delta\tau_{\text{error}}/2) * \sin(\omega_{\text{RES}}(t + \Delta\tau_{\text{error}}/2)) + \quad (\text{eq. 1}) \\ &\quad A(t - \Delta\tau_{\text{error}}/2) * \sin(\omega_{\text{RES}}(t - \Delta\tau_{\text{error}}/2)) \\ Y1_1s(t) &\approx A(t) * 2 * \cos(\Delta\tau_{\text{error}}/2) * \sin(\omega_{\text{RES}} t) \\ &\approx A(t) * (2 - (\omega_{\text{RES}} \Delta\tau_{\text{error}}/2)^2) * \sin(\omega_{\text{RES}} t) \end{aligned}$$

For acoustic energy coming from the direction that causes the first grating lobe (Y1\_1g), this formula can be rewritten to:

$$\begin{aligned} Y1_1g(t) &= A(t + \Delta\tau_{\text{error}}/2) * \sin(\omega_{\text{RES}}(t + \Delta\tau_{\text{error}}/2)) - \quad (\text{eq. 2}) \\ &\quad A(t - \Delta\tau_{\text{error}}/2 + T/2) * \sin(\omega_{\text{RES}}(t - \Delta\tau_{\text{error}}/2)) \\ Y1_1g(t) &\approx A(t) * 2 * \sin(\Delta\tau_{\text{error}}/2) * \cos(\omega_{\text{RES}} t) \\ &\approx A(t) * \Delta\tau_{\text{error}} * \cos(\omega_{\text{RES}} t) \end{aligned}$$

In case of the ultrasound transducer 30 shown in FIG. 4, the beamformer is transparent to all odd (even) transducer

## 11

signals. The even (odd) signals are transferred to two signal combiners. E.g. the signal of transducer element X2 is visible in outputs Y1 and Y2 according to:

$$Y1\_2(t) = \text{gain} * A(t - \Delta\tau\_gen) * \sin(\omega_{RES}(t - \Delta\tau\_gen))$$

$$Y2\_2(t) = \text{gain} * A(t + \Delta\tau\_gen) * \sin(\omega_{RES}(t + \Delta\tau\_gen)) \quad (\text{eq. 3})$$

Typically gain factors (gain) are 0.5 . . . 0.6. In the system beamformer (not shown) the signals are combined according to:

$$Y_{total\_2}(t) = Y1\_2(t + \Delta\tau\_sys) + Y2\_2(t - \Delta\tau\_sys) \quad (\text{eq. 4})$$

wherein  $\Delta\tau\_sys$  is the delay generated in the system beamformer, located externally in the imaging system. It is assumed that this system generates the correct steering or focusing delays (the system beamformer typically has much more calculation power than the micro-beamformer), so

$$+\Delta\tau\_sys = +\Delta\tau = +\Delta\tau\_gen - \Delta\tau\_error$$

$$-\Delta\tau\_sys = -\Delta\tau = -\Delta\tau\_gen + \Delta\tau\_error$$

Rewriting equation 3 and 4 gives:

$$Y_{total\_2}(t) = \text{gain} * (A(t - \Delta\tau\_error) * \sin(\omega_{RES}(t - \Delta\tau\_error)) + A(t + \Delta\tau\_error) * \sin(\omega_{RES}(t + \Delta\tau\_error))) * \text{gain} * 2 * A(t) * \cos(\omega_{RES} * \Delta\tau\_error) * \sin(\omega_{RES} * t) \quad (\text{eq. 5})$$

Now it is possible to calculate the effective contribution of odd and even transducer signals provided by the first and second group of transducer elements to the output:

$$Y12\_2(t) = X1(t - \Delta\tau\_real/2 + \Delta\tau\_sys/2) + Y_{total\_2}(t + \Delta\tau\_real/2 - \Delta\tau\_sys/2)$$

For acoustic energy coming from the steering direction (Y12\_2s), this formula can be reduced to:

$$Y12\_2s(t) \approx A(t) * (1 + g * 2 * \cos(\omega_{RES} * \Delta\tau\_error)) * \sin(\omega_{RES} * t) \approx (\text{eq. 6})$$

$$A(t) * (2 - 0.5 * (\omega_{RES} * \Delta\tau\_error)^2) * \sin(\omega_{RES} * t); [g = 0.5]$$

For acoustic energy coming from the direction that causes the first grating lobe (Y12\_2g), the formula can be rewritten to:

$$Y12\_2s(t) \approx (\text{eq. 7})$$

$$A(t) * (1 - \text{gain} * 2 * \cos(\omega_{RES} * \Delta\tau\_error)) * \sin(\omega_{RES} * t) \approx$$

$$A(t) * (0.5 * (\omega_{RES} * \Delta\tau\_error)^2 * \sin(\omega_{RES} * t)); [-g = 0.5]$$

Eq. 7 shows that the amplitude of the grating lobes of the proposed ultrasound transducer including the beamformer for moderate timing errors is lower than the amplitude of the grating lobes of the standard beamformer (eq. 2). Timing errors result into a phase error between odd and even ultrasound signals in case of the standard micro-beamformer while timing errors result into an amplitude error for the proposed micro-beamformer. As all timing errors result into a reduced amplitude of the split or copied secondary transducer signals (eq. 5), it is attractive for imaging performance to choose gain factor  $\text{gain} > 0.5$ , e.g.  $g = [0.5 \dots 0.6]$ .

In case of the second embodiment of the proposed ultrasound transducer 30 shown in FIG. 5, the effect of the timing error is further reduced. Processing of the even transducer signals remains the same, typical value for gain  $g = 0.5$ . The beamformer remains transparent for a major fraction of the odd signals.

## 12

A small fraction of the odd signals is transferred to neighbor output nodes. For example, the signal of transducer element X3 is visible in output Y1, Y2 and Y3 according to:

$$Y1\_3(t) = G * A(t - 2\Delta\tau\_gen) * \sin(\omega_{RES}(t - 2\Delta\tau\_gen))$$

$$Y2\_3(t) = (1 - 2 * G) * A(t) * \sin(\omega_{RES} * t)$$

$$Y3\_3(t) = G * A(t + 2\Delta\tau\_gen) * \sin(\omega_{RES}(t + 2\Delta\tau\_gen)) \quad (\text{eq. 8})$$

Typically gain factor  $g = 0.5$  and  $G = 0.1667$ . In the system beamformer in imaging system (not shown) the signals are combined again according to:

$$Y_{total\_3}(t) = Y1\_3(t + 2\Delta\tau\_sys) + Y2\_3(t) + Y1\_3(t - 2\Delta\tau\_sys) \quad (\text{eq. 9})$$

wherein  $\Delta\tau\_sys$  is the incremental delay generated in the system beamformer, located externally in the imaging system. It is assumed that this system generates the correct steering or focusing delays:

$$+\Delta\tau\_sys = +\Delta\tau = +\Delta\tau\_gen - \Delta\tau\_error$$

$$-\Delta\tau\_sys = -\Delta\tau = -\Delta\tau\_gen + \Delta\tau\_error$$

Rewriting equation 8 and 9 gives:

$$Y_{total\_3}(t) = G * (A(t - 2\Delta\tau\_error) * \sin(\omega_{RES}(t - 2\Delta\tau\_error)) + (1 - 2G) * A(t) * \sin(\omega_{RES} * t) + G * (A(t + 2\Delta\tau\_error)) * \sin(\omega_{RES}(t + 2\Delta\tau\_error)))$$

$$\approx A(t) * (1 + G * 2 * (\cos(\omega_{RES} * 2\Delta\tau\_error) - 1)) * \sin(\omega_{RES} * t) \quad (\text{eq. 10})$$

Now it is possible to calculate the effective contribution of odd and even signals to the output:

$$Y12\_3(t) = Y_{total\_3}(t - \Delta\tau\_real/2 + \Delta\tau\_sys/2) + Y_{total\_2}(t + \Delta\tau\_real/2 - \Delta\tau\_sys/2)$$

For acoustic energy coming from the steering direction (Y12\_3s), this formula can be reduced to:

$$Y12\_3s(t) \approx A(t) * (1 + G * 2 * (\cos(\omega_{RES} * 2\Delta\tau\_error) - 1) + \text{gain} * 2 * \cos(\omega_{RES} * \Delta\tau\_error)) * \sin(\omega_{RES} * t)$$

$$\approx A(t) * (2 - 1.2 * (\omega_{RES} * \Delta\tau\_error)^2) * \sin(\omega_{RES} * t); [g = 0.5, G = 0.1667] \quad (\text{eq. 11})$$

For acoustic energy coming from the direction that causes the first grating lobe (Y12\_3g), the formula can be rewritten to:

$$Y12\_2g(t) \approx A(t) * (1 + G * 2 * (\cos(\omega_{RES} * 2\Delta\tau\_error) - 1) - \text{gain} * 2 * \cos(\omega_{RES} * \Delta\tau\_error)) * \sin(\omega_{RES} * t)$$

$$\ll A(t) * 0.1 * (\omega_{RES} * \Delta\tau\_error)^2 * \sin(\omega_{RES} * t); [g = 0.5, G = 0.1667] \quad (\text{eq. 12})$$

From equation 12 it is clear that the grating lobes are less dependent on the timing error and, therefore, the ultrasound transducer assembly 30 is less sensitive for timing errors in general.

In FIG. 6a-c, the angle sensitivity of the ultrasound transducer assembly 20, 30 of FIGS. 2, 4 and 5 are shown for different values of the timing error. The sensitivity is calculated for a steering angle of  $-36^\circ$  and a grating lobe is generated at an angle of  $+25^\circ$ .

All cases refer to far field sensitivity of the transducer array including the respective ultrasound beamformer. Course delays have been programmed so that the beam is steered to an angle of  $-36^\circ$ . The simulated sensitivity is shown for beamformer timing errors of  $0.1 \cdot T_{res}/20$ ,  $2 \cdot T_{res}/20$  and  $3 \cdot T_{res}/20$  wherein  $T_{res}$  is the period time of the transducer resonance frequency.

As shown in FIG. 6a, the sensitivity of the transducer assembly 20 shown in FIG. 2 including the standard two-to-one beamformer has no grating lobe for zero timing error while the amplitude of the first grating lobe (happening at  $+25$  degrees) increases for increasing timing errors.

FIG. 6b is a simulation of the ultrasound transducer assembly shown in FIG. 4, wherein the grating lobe at  $25^\circ$  is merely visible for a timing error of  $3 \cdot T_{res}/20$ . For smaller timing errors, the grating lobe amplitude reduces rapidly.

FIG. 6c shows a simulation of the sensitivity of the ultrasound transducer using the micro-beamformer of FIG. 5. The simulation diagram shows that an error of the timing does reduce the sensitivity at the steering angle  $-36^\circ$  but that does not show any grating lobe

Consequently, the ultrasound transducer assemblies 30 according to the present invention provides a reduced sensitivity to timing errors than the transducer assemblies known from the prior art.

While the invention has been illustrated and described in detail in the drawings and foregoing description, such illustration and description are to be considered illustrative or exemplary and not restrictive; the invention is not limited to the disclosed embodiments. Other variations to the disclosed embodiments can be understood and effected by those skilled in the art in practicing the claimed invention, from a study of the drawings, the disclosure, and the appended claims.

In the claims, the word "comprising" does not exclude other elements or steps, and the indefinite article "a" or "an" does not exclude a plurality. A single element or other unit may fulfill the functions of several items recited in the claims. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage.

Any reference signs in the claims should not be construed as limiting the scope.

The invention claimed is:

1. An ultrasound transducer assembly, comprising:

a plurality of ultrasound transducer elements for receiving ultrasound waves and for providing transducer signals corresponding to the respectively received ultrasound waves,

a plurality of signal combiners for providing different output signals on the basis of the transducer signals, and

a plurality of timing elements for providing different time shifts to the transducer signals,

wherein each of the ultrasound transducer elements is connected to a plurality of the signal combiners for providing the transducer signals including the different time shifts to different of the signal combiners, and

wherein the plurality of signal combiners are connected to an overall combiner configured to combine the plurality of output signals to an overall output signal of the transducer assembly.

2. The ultrasound transducer assembly as claimed in claim 1, wherein each of the ultrasound transducer elements is connected to a plurality of the timing elements for providing the different time shifts to each of the transducer signals.

3. The ultrasound transducer assembly as claimed in claim 1, wherein a plurality of secondary transducer signals is formed of the transducer signal of each of the ultrasound transducer elements and wherein each of the secondary transducer signals is provided to one of the signal combiners, respectively.

4. The ultrasound transducer assembly as claimed in claim 1, wherein the signal combiners each comprise a signal adder.

5. The ultrasound transducer assembly as claimed in claim 1, wherein the transducer signals of the plurality of transducer elements provided to the different signal combiners are weighted by means of different weight factors.

6. The ultrasound transducer assembly as claimed in claim 1, wherein an amplifier or an attenuator device is associated to each of the transducer elements to provide different gain factors to the transducer signals.

7. The ultrasound transducer assembly as claimed in claim 6, wherein the gain factors of the transducer signals provided to one of the signal combiners have different absolute values.

8. The ultrasound transducer assembly as claimed in claim 1, further comprising a second plurality of transducer elements, wherein a delay element is associated to each of the second plurality of transducer elements for providing a fixed time delay to each of the respective transducer signals of the second plurality of transducer elements.

9. The ultrasound transducer assembly as claimed in claim 8, wherein each of the second plurality of transducer elements is connected to only one of the signal combiners.

10. The ultrasound transducer assembly as claimed in claim 8, wherein the plurality of second transducer elements and the respectively connected delay elements are virtual elements.

11. The ultrasound transducer assembly as claimed in claim 1, wherein the time shift provided to the transducer signals include a fixed time delay and a relative time shift.

12. The ultrasound transducer assembly as claimed in claim 11, wherein the relative time shift of the transducer signals provided to a first of the signal combiners is a positive time shift and the relative time shift of the transducer signals provided to a second of the signal combiners is a negative time shift.

13. The ultrasound transducer assembly as claimed in claim 11, wherein the time shifts of the transducer signals provided to one of the signal combiners have different absolute values.

14. The ultrasound transducer assembly as claimed in claim 1, wherein the plurality of ultrasound transducer elements are connected to the signal combiners in parallel to each other.

15. An ultrasound imaging system comprising the ultrasound transducer assembly as claimed in claim 1.

\* \* \* \* \*

专利名称(译)	超声换能器组件		
公开(公告)号	<a href="#">US10209352</a>	公开(公告)日	2019-02-19
申请号	US15/314301	申请日	2015-06-08
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	荷兰皇家飞利浦V, N.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	VAN RENS ANTONIA CORNELIA		
发明人	VAN RENS, ANTONIA CORNELIA		
IPC分类号	A61B8/08 G10K11/34 G01S7/52 A61B8/00 G01S15/89		
CPC分类号	G10K11/346 G01S15/8915 G01S15/8993 G01S7/5208 G01S7/52047 A61B8/0883 A61B8/4488		
优先权	2014172046 2014-06-12 EP		
其他公开文献	US20180180726A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

公开了一种超声换能器组件 ( 30 ) , 包括 : 多个超声换能器元件 ( 34,36,38 ) , 用于接收超声波并提供换能器信号 ( X 对应于分别接收的超声波 ,  $X_2$  ,  $X_3$  ,  $X_4$  ) 。该组件包括多个信号组合器 ( 42,44 ; 60,62,64 ) , 用于提供不同的输出信号 (  $Y_1$  ,  $Y_2$  ) 基于换能器信号和多个定时元件 ( 48,52 ; 68,70 ; 72,74 ) , 用于向换能器信号提供不同的时移 (  $\tau$  ) 。每个超声换能器元件连接到多个信号组合器 , 用于提供换能器信号 , 包括到不同信号组合器的不同时移。

