



US 20080009739A1

(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2008/0009739 A1**

Chiang et al.

(43) **Pub. Date:** **Jan. 10, 2008**

(54) **ULTRASOUND 3D IMAGING SYSTEM**

(22) **Filed:** **Jun. 23, 2006**

(76) **Inventors:** **Alice M. Chiang**, Weston, MA
(US); **Michael Brodsky**,
Brookline, MA (US); **Xingbai He**,
Andover, MA (US); **William M.**
Wong, Milton, MA (US)

Publication Classification

(51) **Int. Cl.** **A61B 8/14** (2006.01)


(52) **U.S. Cl.** **600/459**

(57) **ABSTRACT**

The present invention relates to an ultrasound imaging system in which the scan head either includes a beamformer circuit that performs far field subarray beamforming or includes a sparse array selecting circuit that actuates selected elements. When used with second stage beamforming system, three dimensional ultrasound images can be generated.

Correspondence Address:
WEINGARTEN, SCHURGIN, GAGNEBIN &
LEBOVICI LLP
TEN POST OFFICE SQUARE
BOSTON, MA 02109

(21) **Appl. No.:** **11/474,098**

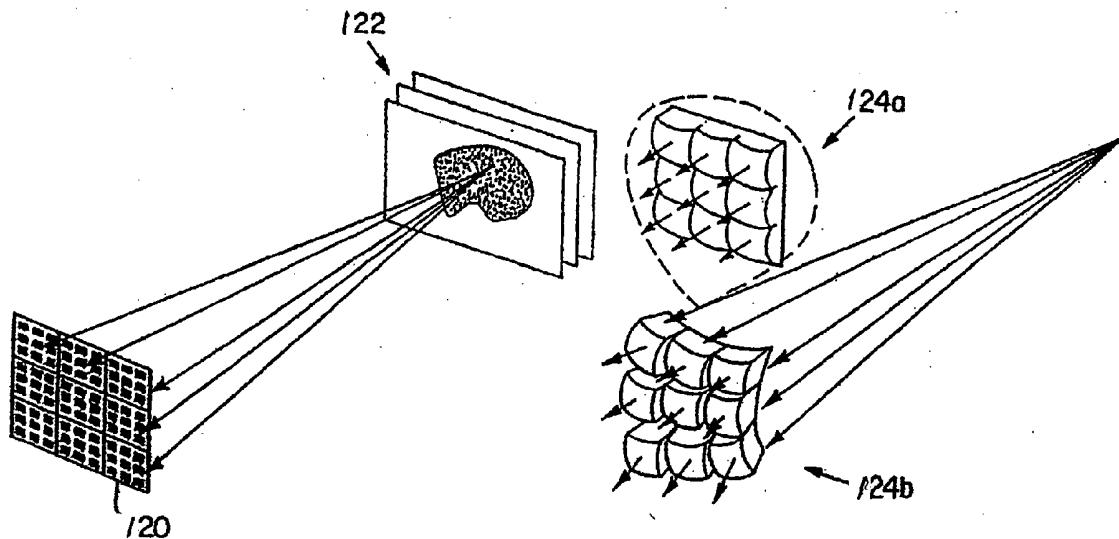

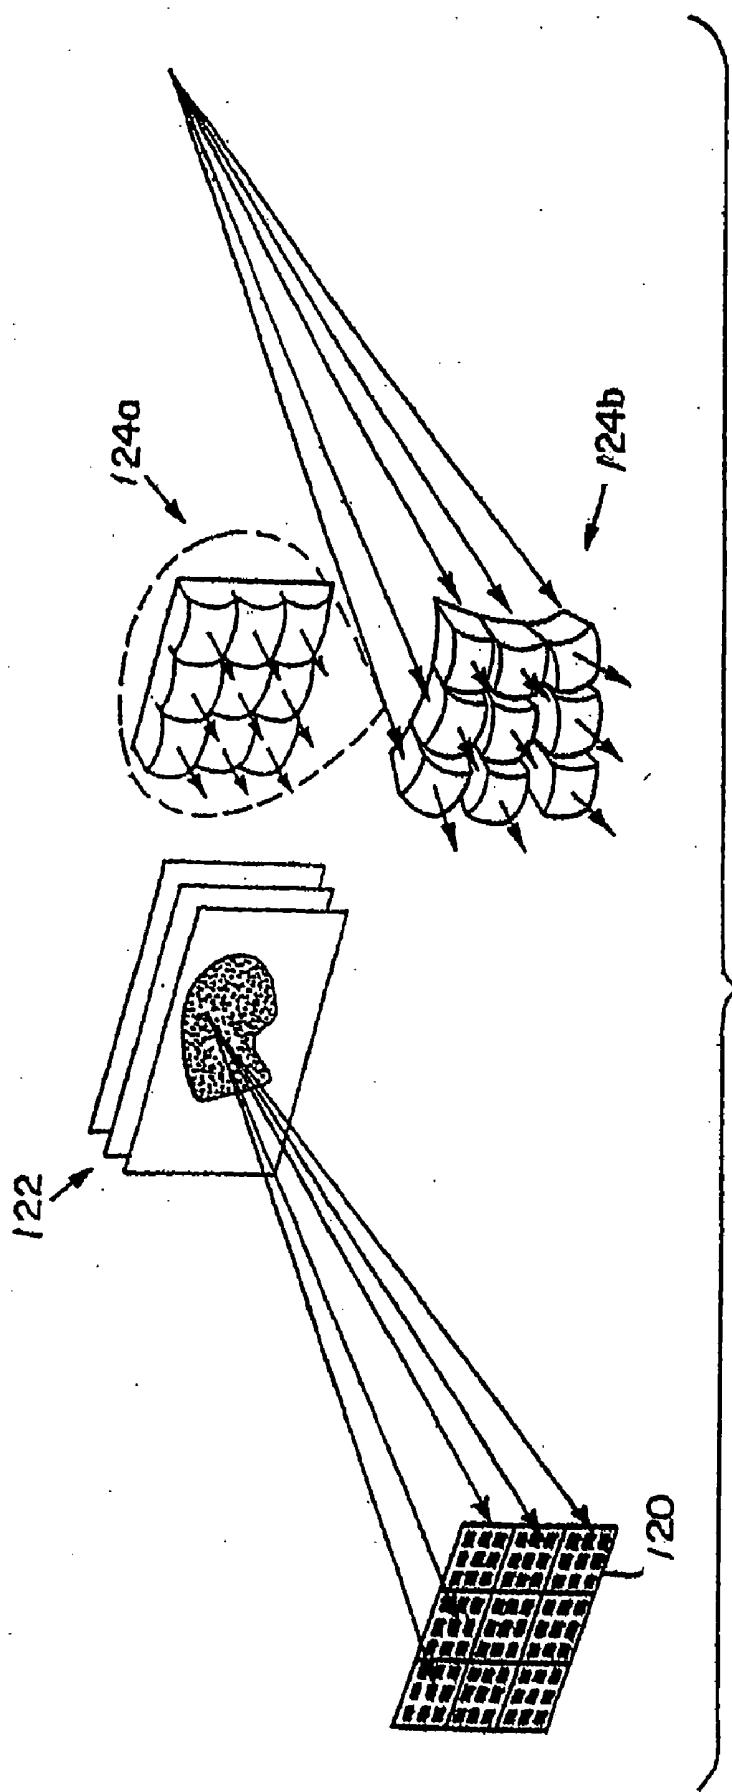


FIG. 1

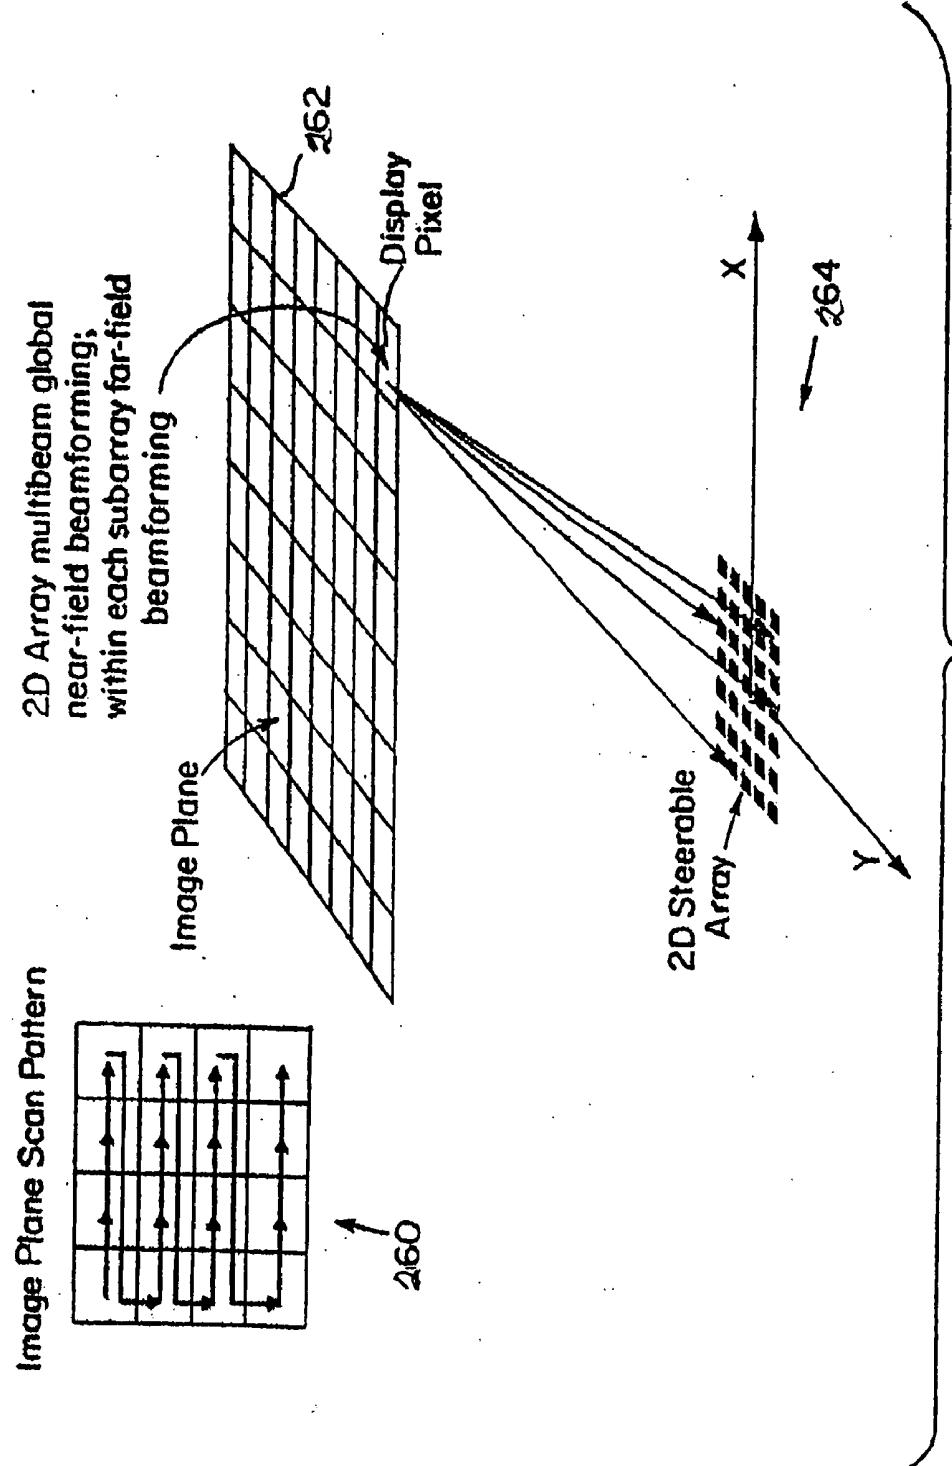


FIG. 2

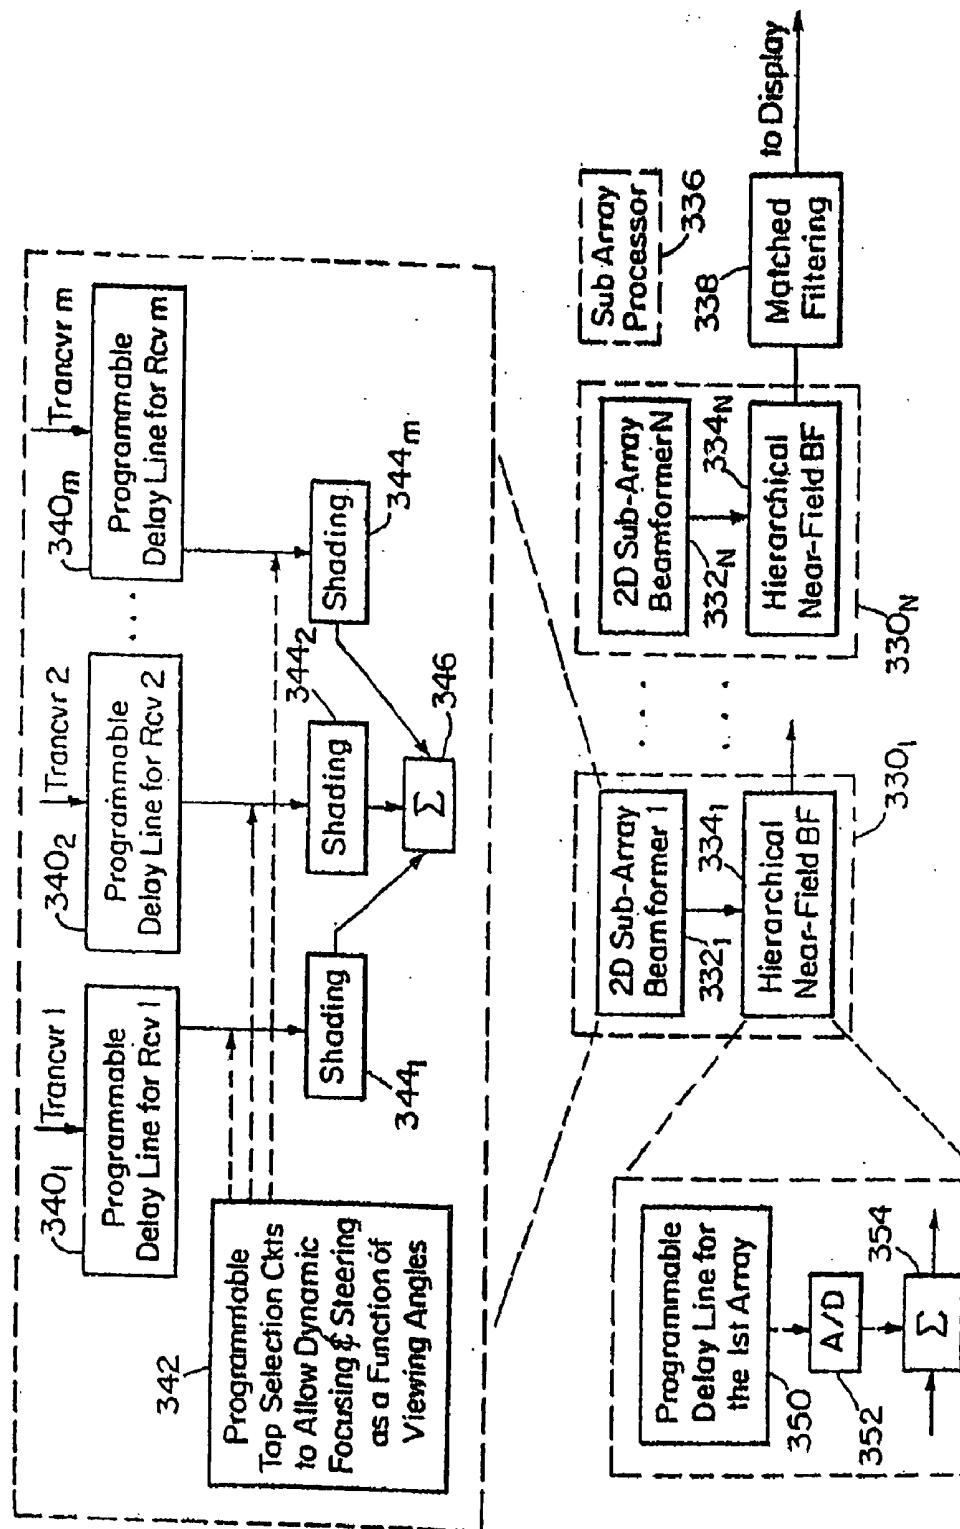


FIG. 3A

ELECTRONICALLY-CONTROLLED ACOUSTIC CONFORMAL LENS

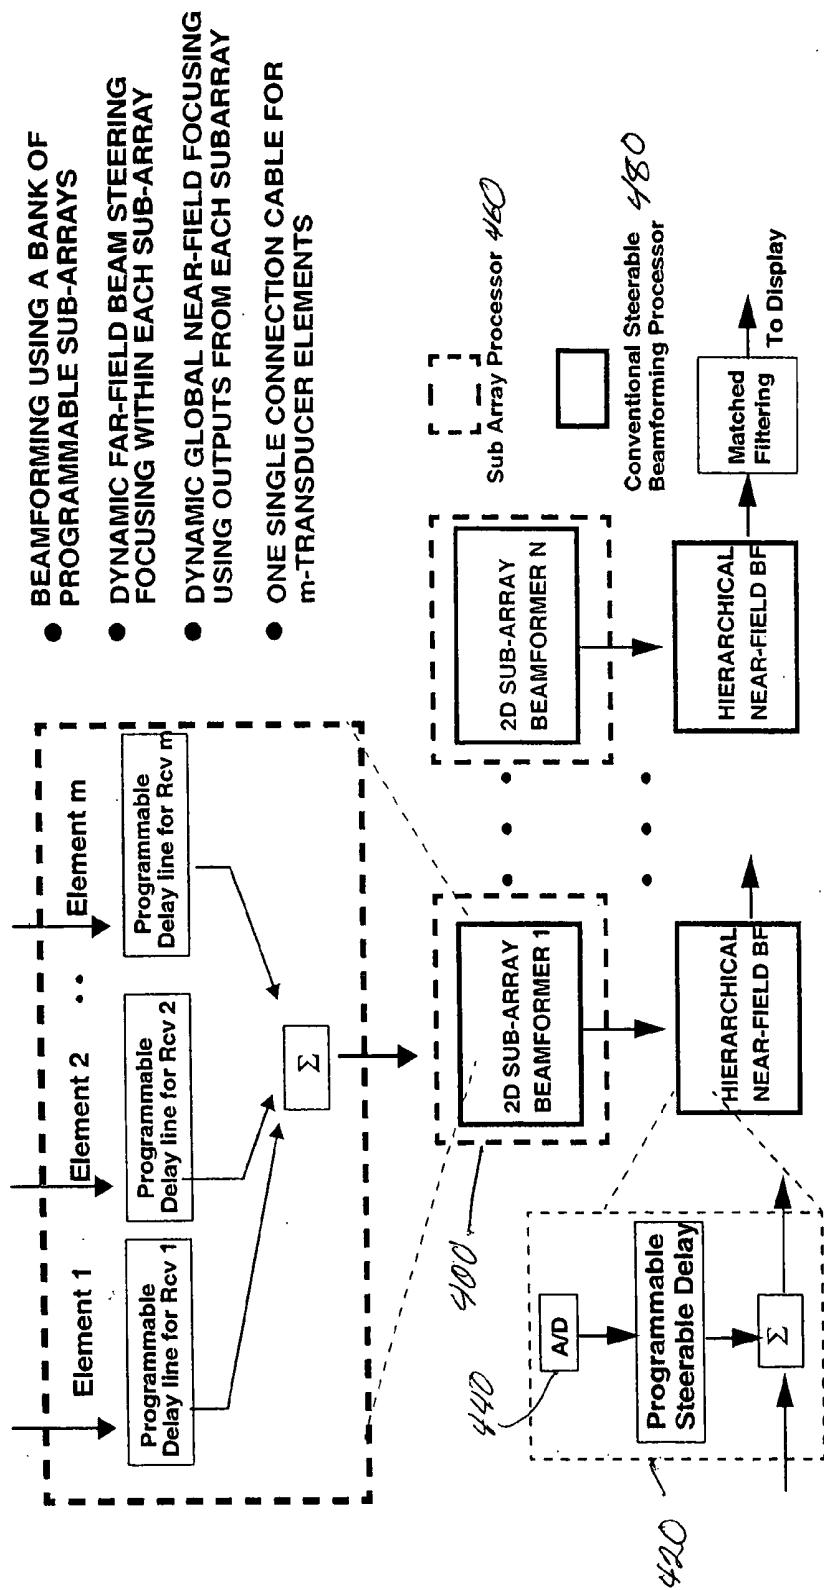


Fig. 3B

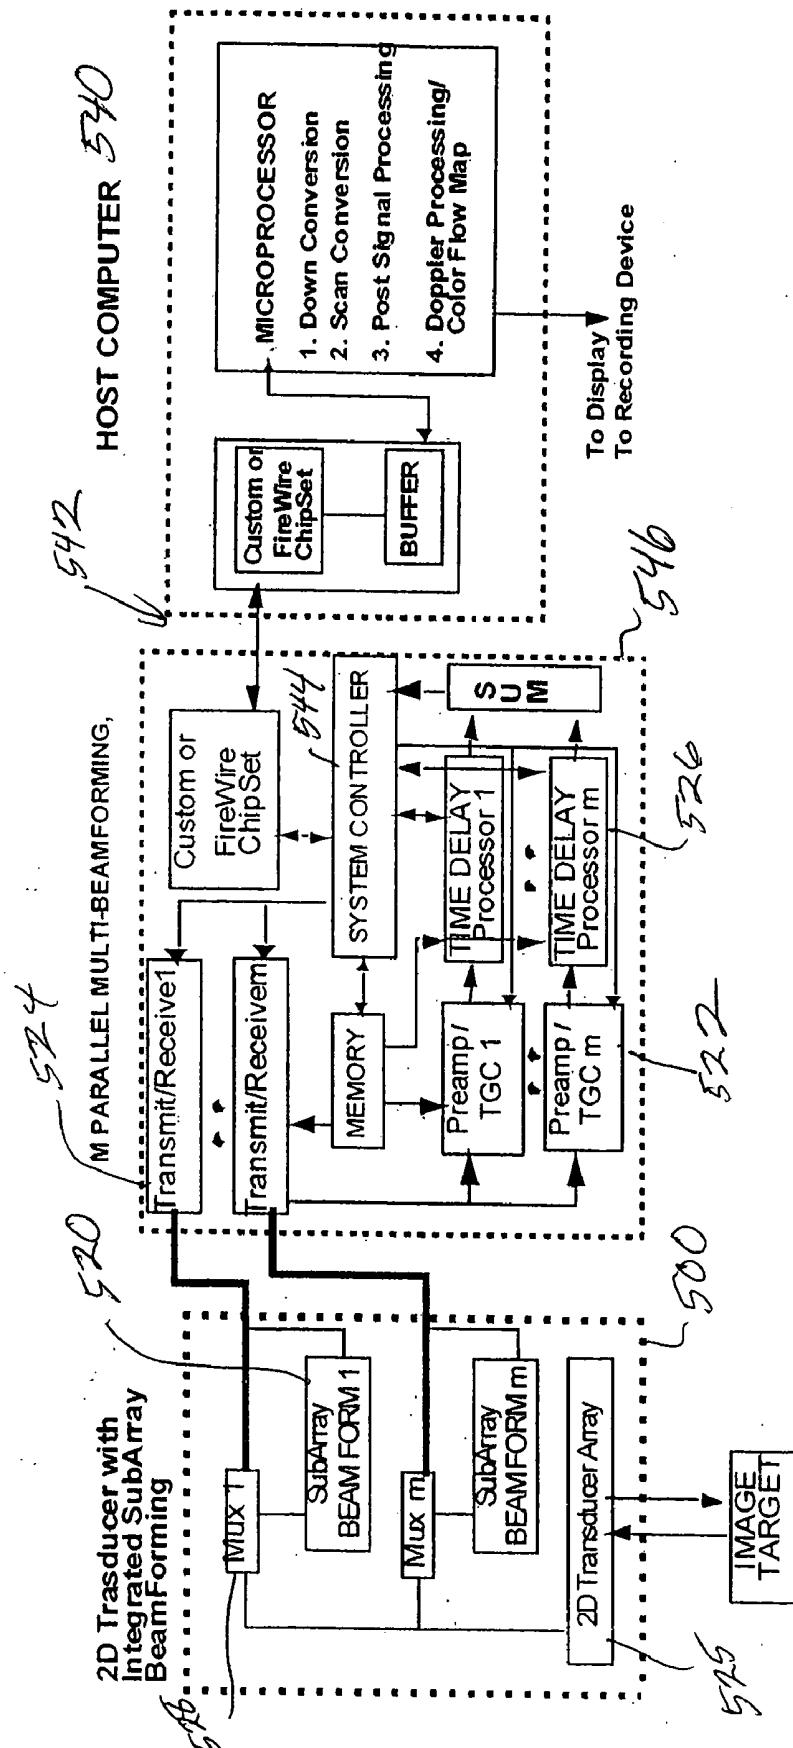
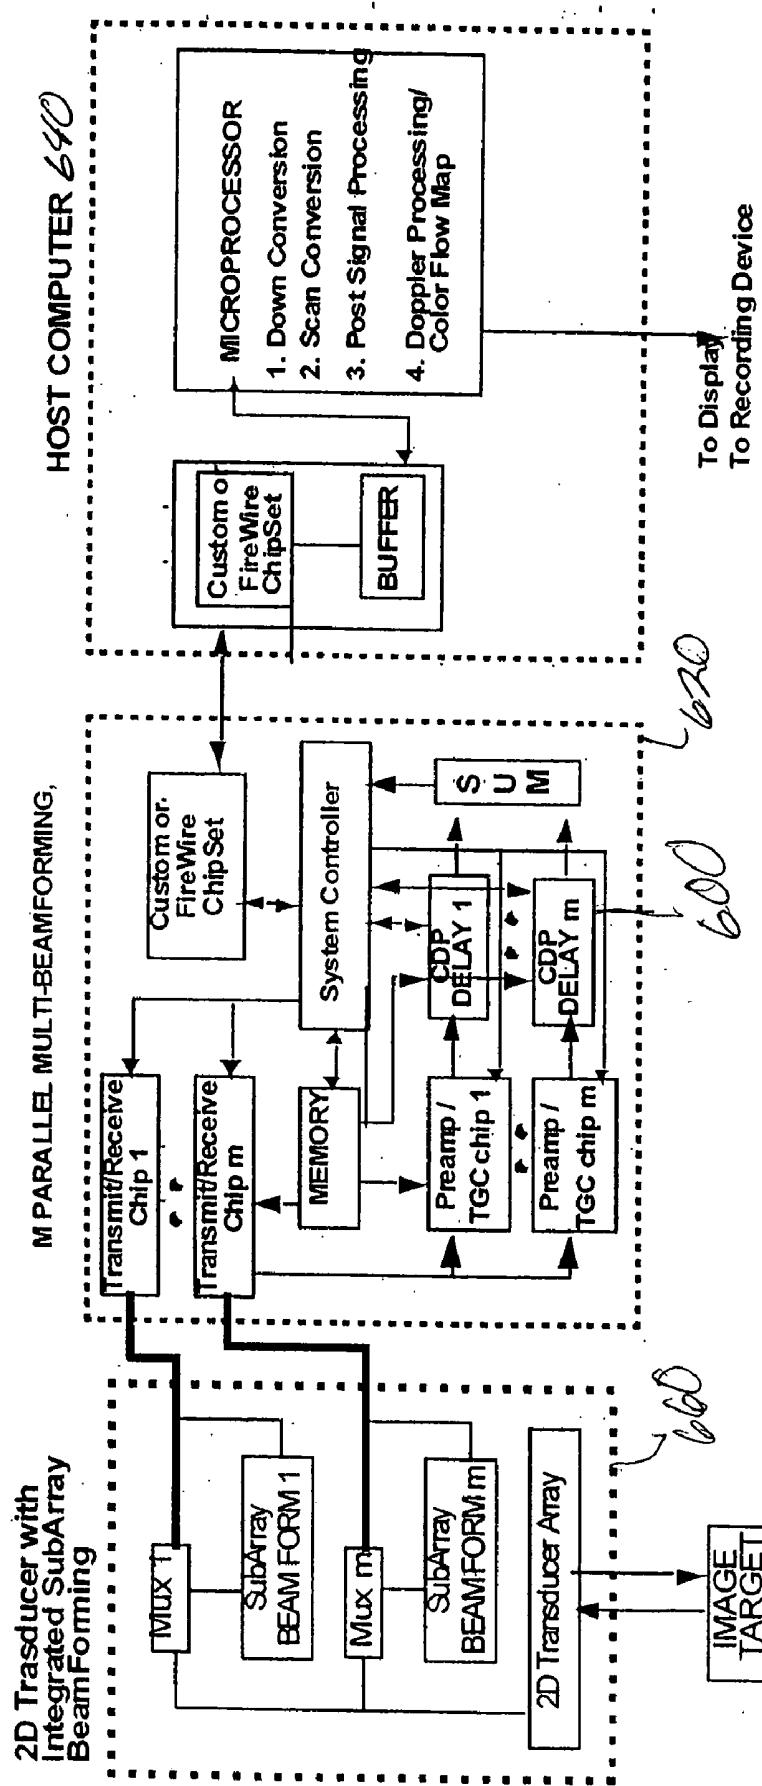


Figure 4



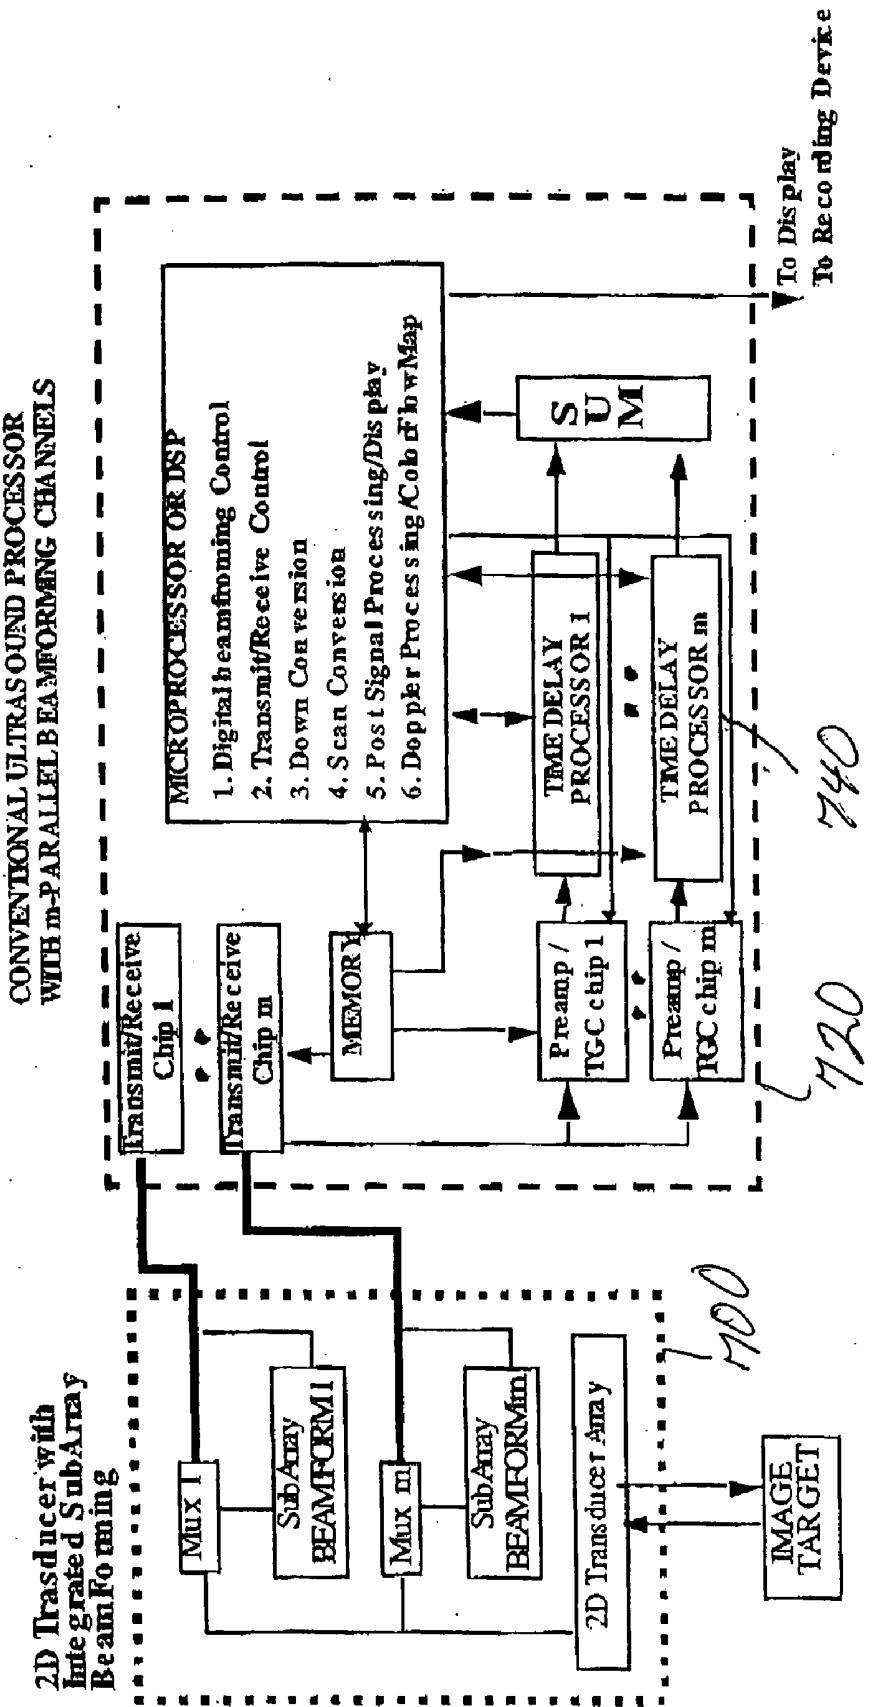
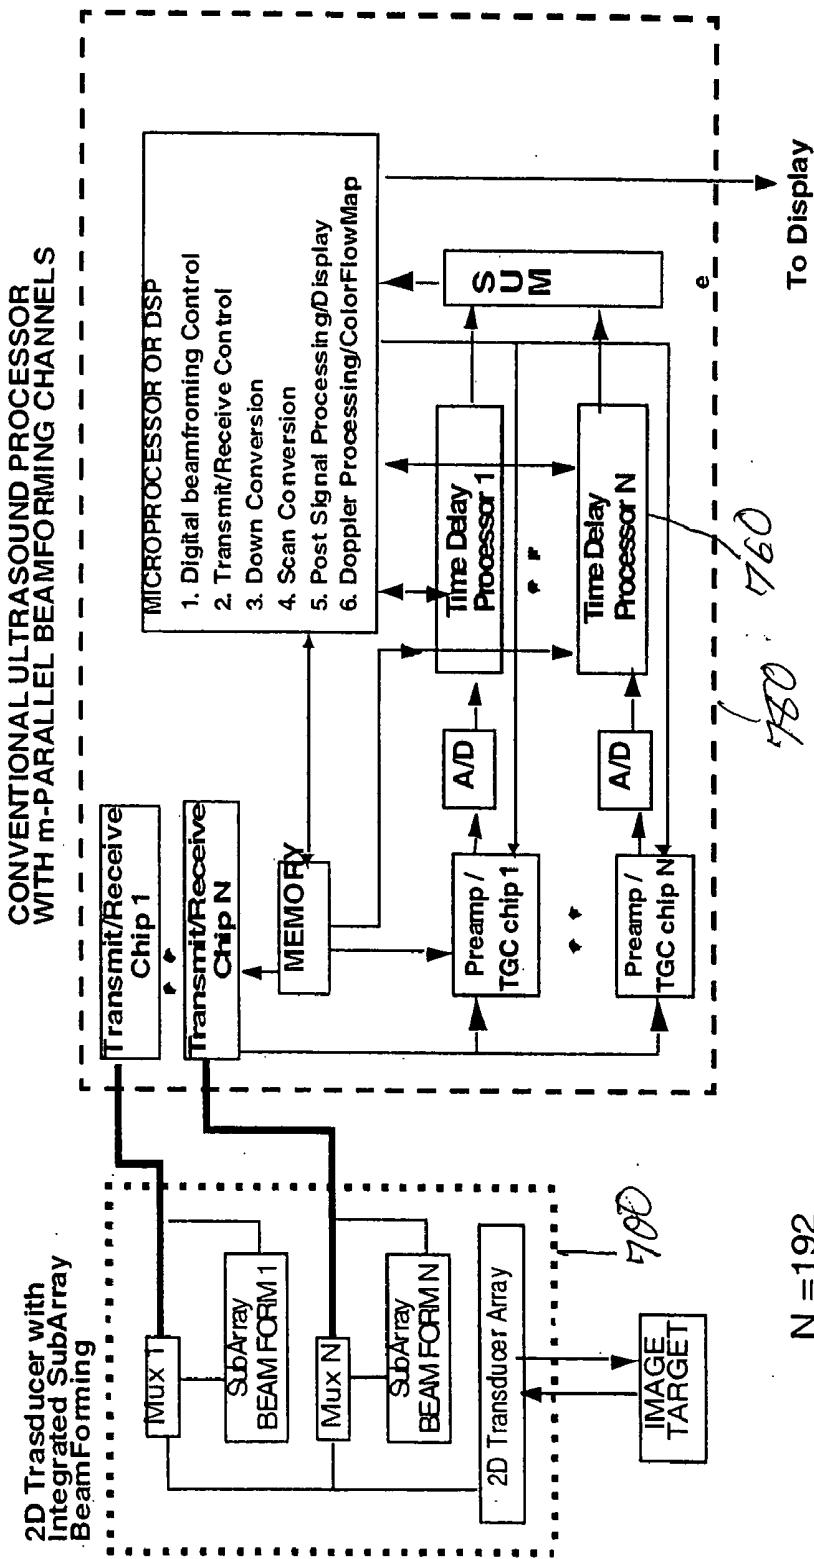
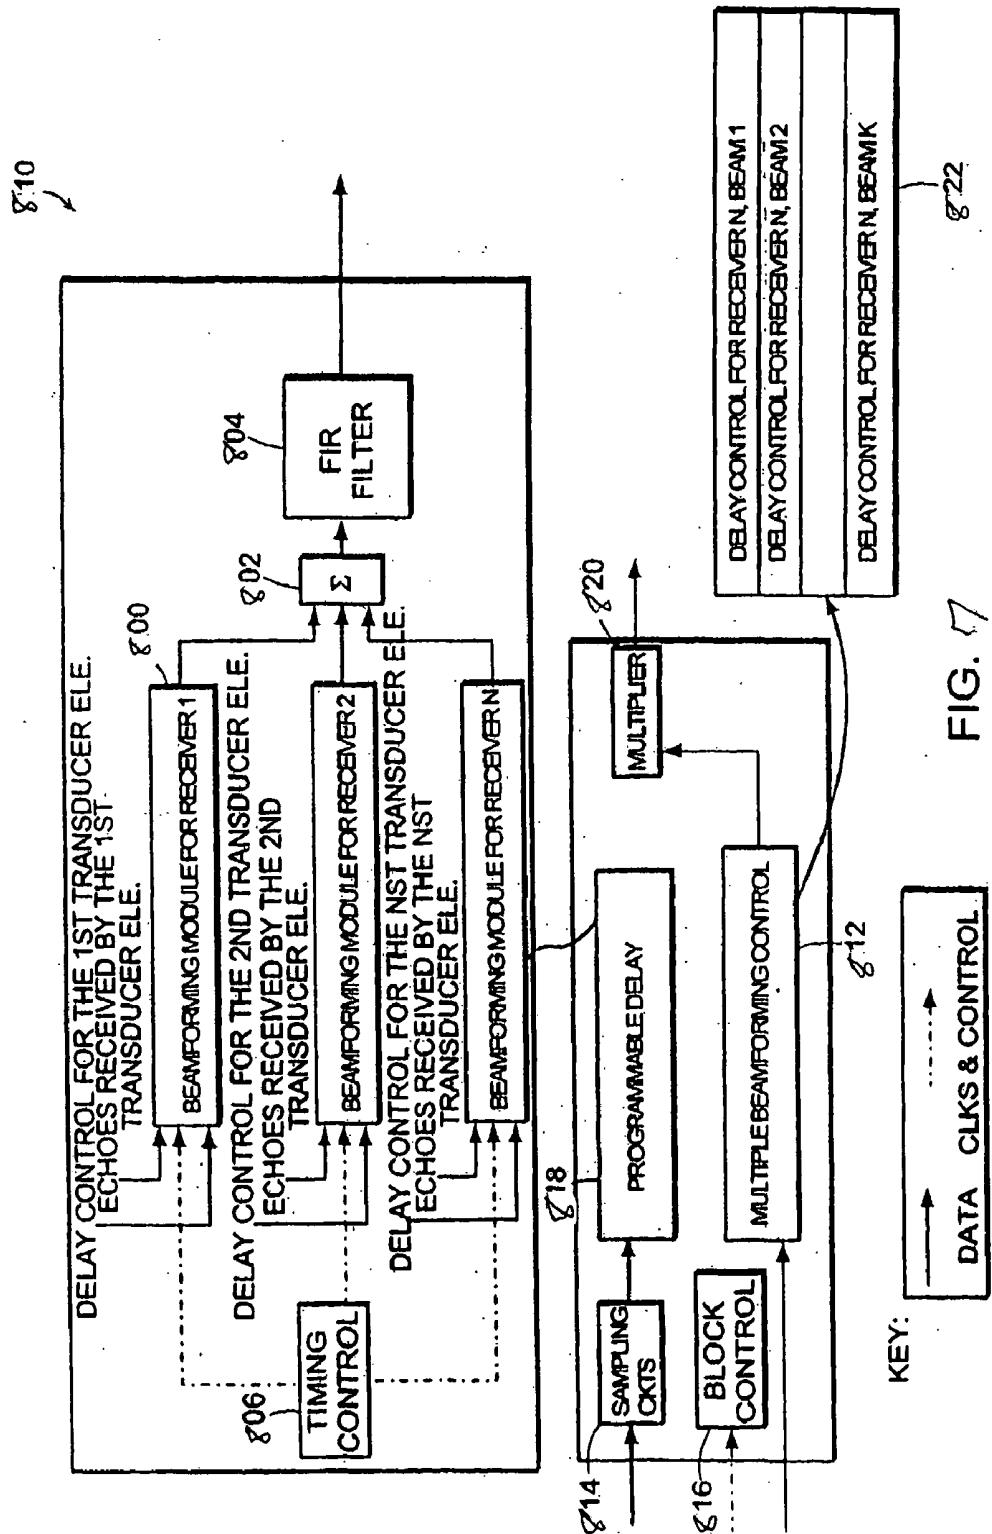


Fig. 6A

Real-Time 3D/4D Imaging





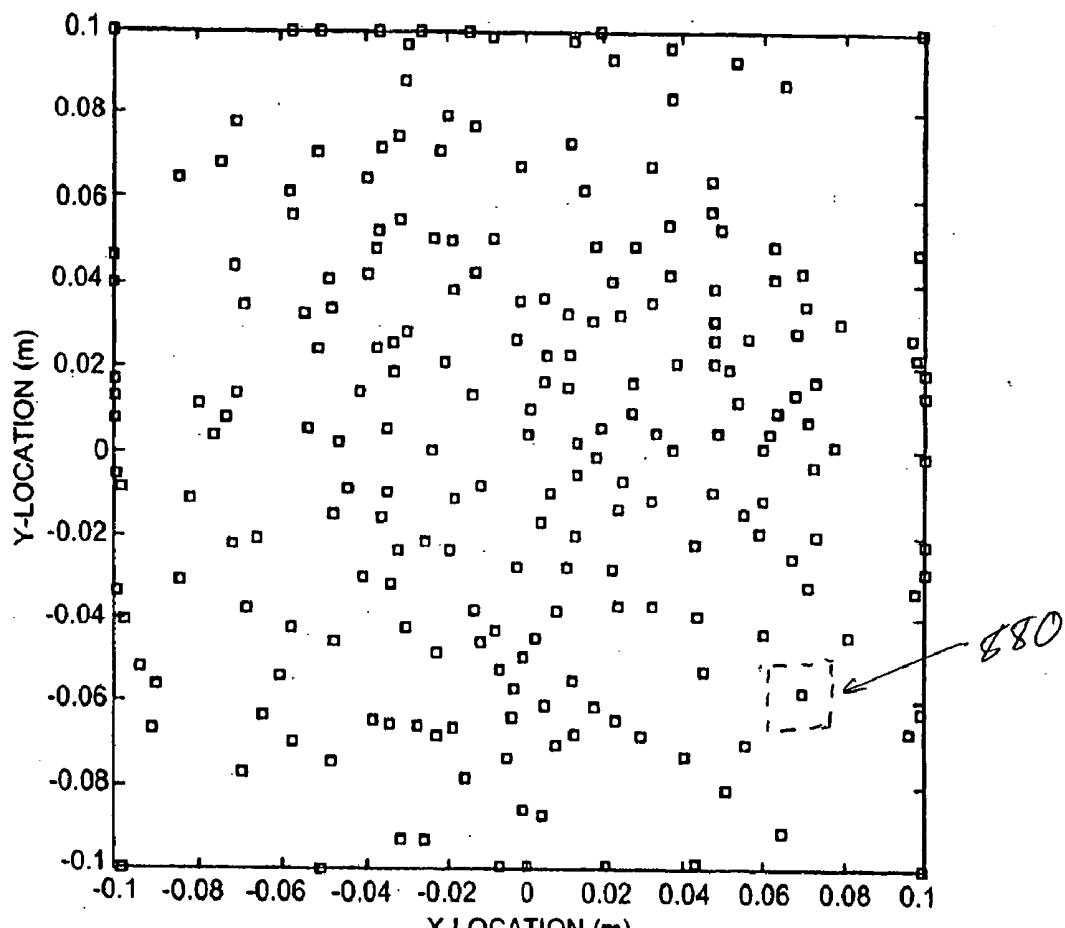


FIG. 8A

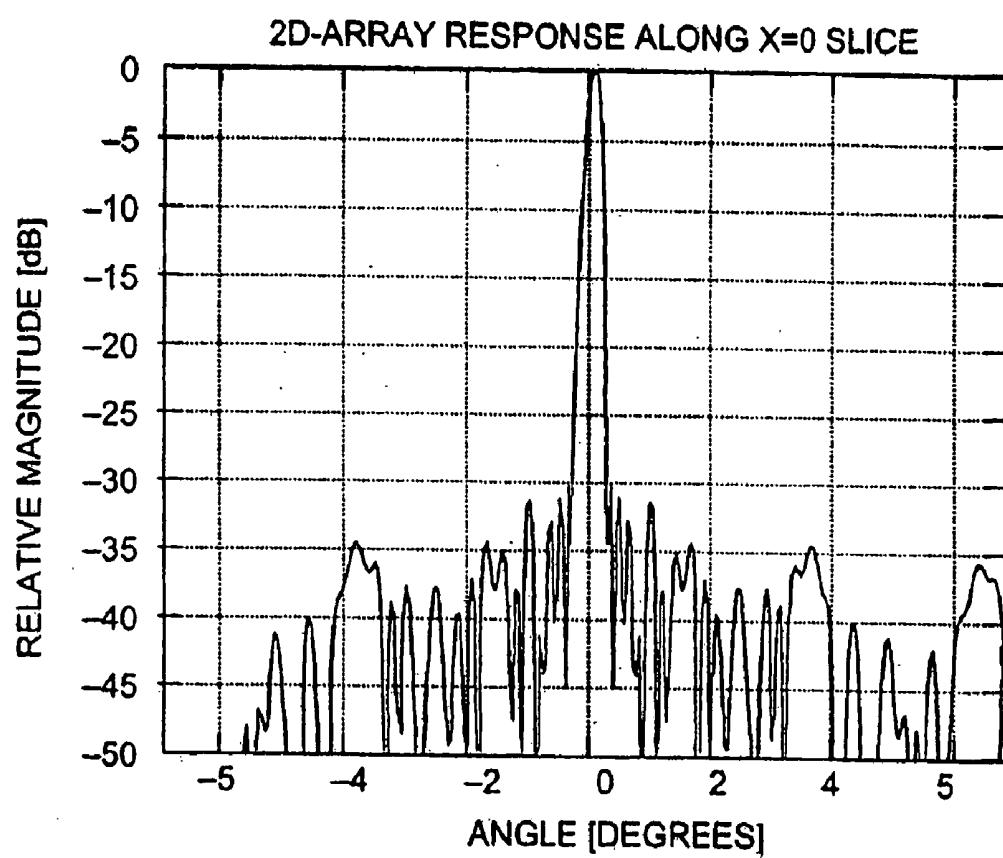


FIG. 8B



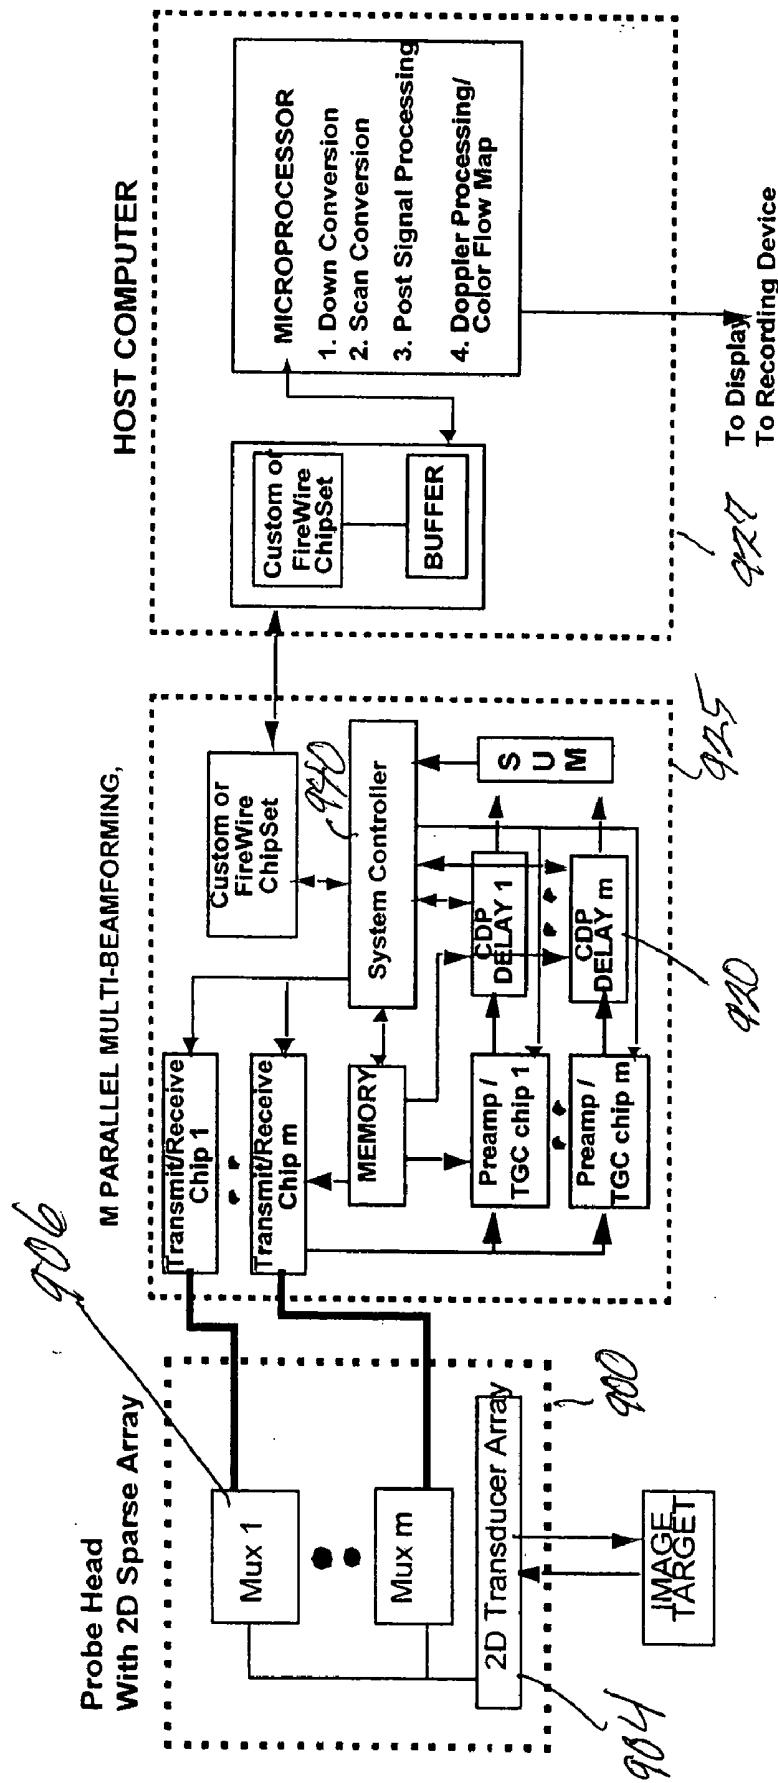


Fig. 9A

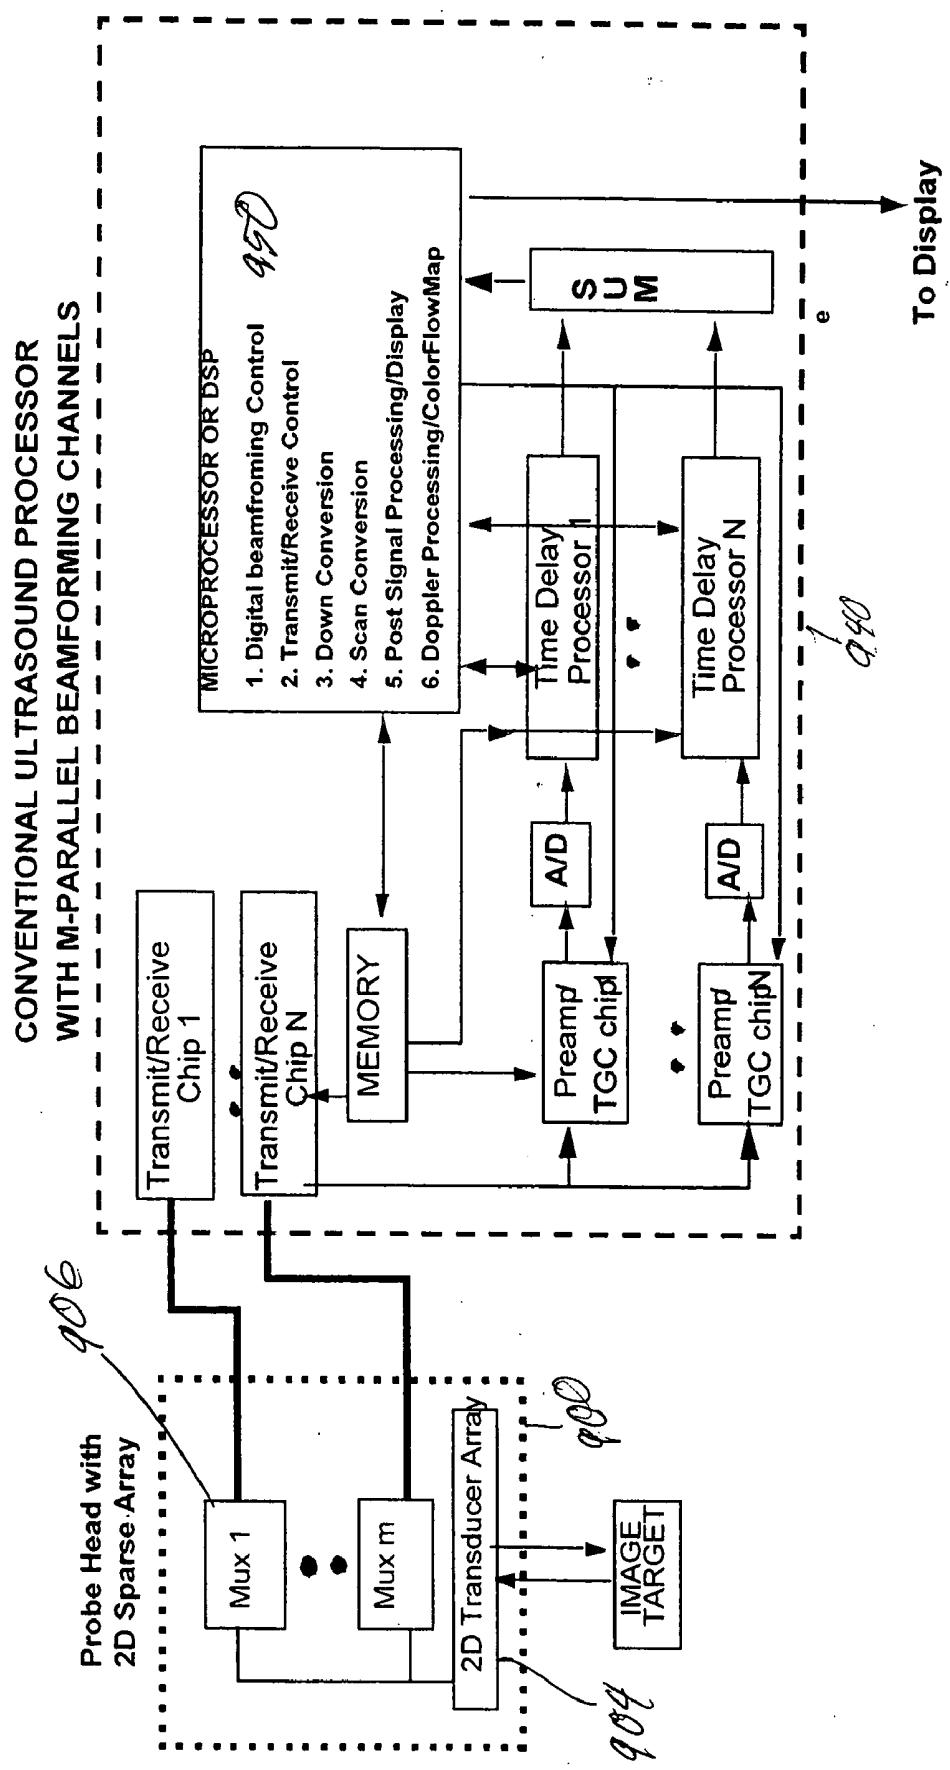

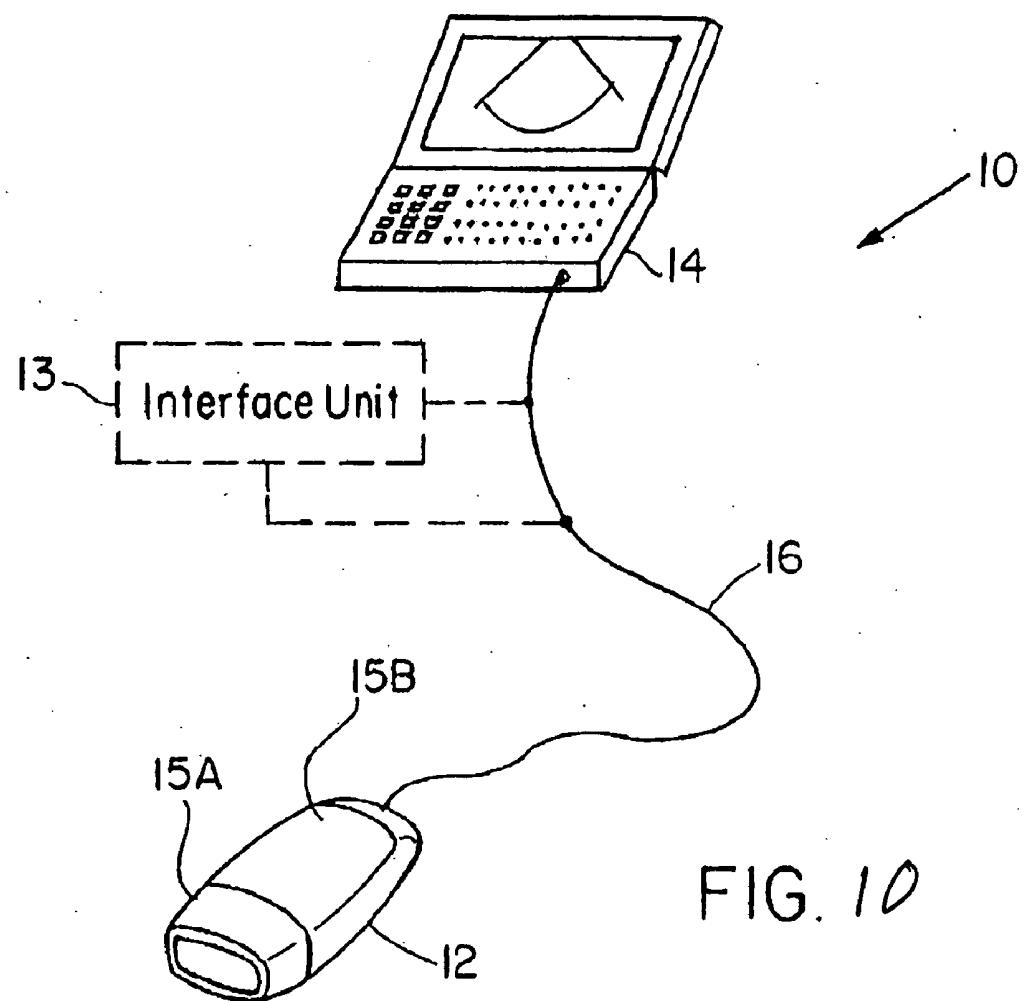

ULTRASOUND 3D IMAGING SYSTEM

BACKGROUND OF THE INVENTION

[0001] Medical ultrasound imaging has become an industry standard for many medical imaging applications. Techniques have been developed to provide three dimensional (3D) images of internal organs and processes using a two dimensional (2D) transducer array. These systems require thousands of beamforming channels. The power required to operate such systems has resulted in the use of an analog phase shift technique with a digital delay beamformer that results in a compromise of image quality.

[0002] There is a continuing need for further improvements in ultrasound imaging technologies enabling improved real-time three dimensional imaging capability. In addition, this improved capability should support continuous real-time display for a fourth dimensional 4D function.

SUMMARY OF THE INVENTION

[0003] The present invention relates to a system for ultrasound medical imaging that provides three dimensional (3D) imaging using a two dimensional (2D) array of transducer elements in a probe housing. In a preferred embodiment, the probe housing contains a first beamforming circuit that transmits beamformed data to a second housing having a second beamforming circuit. The first beamforming circuit provides a far-field subarray beamforming operation. The resulting beamformed data is transmitted from the scan head to a second housing having the second beamforming circuit that provides near-field beamsteering and beamfocusing.

[0004] A preferred embodiment provides a scan head that can be connected to a conventional ultrasound system in which the scan head provides the inputs to the conventional beamforming processing function. The scan head beamformer can utilize a low power charge domain processor having at least 32 beamforming channels.

[0005] An alternative preferred embodiment of the invention employs a sparse array where only a fraction of the transducer elements need to be activated. By selecting the four corner elements of the array to provide proper mean lobe bandwidth, minimizing average sidelobe energy and clutter, eliminating periodicity and maximizing peak to side lobe ratio, quality images are produced. To steer the beams across the volume or region of interest, different transducer elements must be actuated in proper sequence to maintain the peak to sidelobe ratio. The system processor can be programmed to provide the desired sequence for transducer actuation to direct the beam at different angles. Alternatively, a discrete controller can be used to control sparse array actuation. A preferred embodiment provides a scan head with integrated switching circuits for sequentially selecting sparse array actuation elements for sequential multiple beamforming. The scan head can be connected to a conventional ultrasound system in which the scan head provides the inputs to the conventional beamforming processing functions.

[0006] In addition to the three dimensional (3D) display capability, a fourth dimension or time resolved image display can be used to record and display a sequence of images recorded at 10 frames per second or higher, for example. This enables viewing of rapidly changing features such as

blood or fluid flow; heart wall movement etc. at video frames rates of 30 frames per second.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] FIG. 1 illustrates the use of a two dimensional tiled array for ultrasound imaging in accordance with the invention.

[0008] FIG. 2 illustrates a steerable two dimensional array in accordance with the invention.

[0009] FIG. 3A illustrates the use of a first beamformer device for far field beamsteering and focusing and a second time delay beamformer for near field beamforming.

[0010] FIG. 3B illustrates a first analog subarray beamformer forwarding data to a digital beamformer near field beamformer.

[0011] FIG. 4 illustrates a preferred embodiment of a three dimensional imaging system in accordance with the integrated Subarray scan head invention.

[0012] FIG. 5 illustrates a preferred embodiment of the integrated Subarray scan head invention using a charge domain processor for the 2nd time delay beamforming.

[0013] FIG. 6A illustrates the use of the integrated subarray scan head probe of the present invention with a second stage beamforming ultrasound processor.

[0014] FIG. 6B illustrates use of the integrated Subarray scan head with a digital beamforming processor.

[0015] FIG. 7 illustrates an ultrasound system in accordance with the invention.

[0016] FIG. 8A illustrates a sparse array used in accordance with the invention.

[0017] FIG. 8B graphically illustrates the sparse array performance.

[0018] FIG. 9A illustrates the use of the integrated sparse array scan head probe of the present invention connected to a host system with charge-domain beamforming processing. FIG. 9B illustrates the use of the integrated sparse array scan head probe of the present invention connected to a conventional digital ultrasound system with m-parallel beamforming components.

[0019] FIG. 10 illustrates a scan head connected to a portable computer in accordance with a preferred embodiment of the invention.

DETAILED DESCRIPTION OF THE INVENTION

[0020] The objective of the beamforming system is to focus signals received from an image point onto a transducer array. By inserting proper delays in a beamformer to wavefronts that are propagating in a particular direction, signals arriving from the direction of interest are added coherently, while those from other directions do not add coherently or cancel. For real-time three-dimensional applications, separate electronic circuitry is necessary for each transducer element. Using conventional implementations, the resulting electronics rapidly become both bulky and costly as the number of elements increases. Traditionally, the cost, size, complexity and power requirements of a high-resolution beamformer have been avoided by "work-around" system approaches. For real-time three-dimensional high-resolution ultrasound imaging applications, an electronically steerable two-dimensional beamforming processor based on a delay-and-sum computing algorithm is chosen.

[0021] The concept of an electronically-adjustable acoustic conformal lens is to divide the surface of a 2D transducer array into plane “tiles” of relatively small subarrays. As described in U.S. Pat. No. 6,292,433 the entire contents of which incorporated herein by reference, and illustrated in FIG. 1 the tiles/subarrays 120 are made small enough so that when an object is placed within the field-of-view of the imaging system, the incident radiation 122 from the object toward each “tile” can be treated using a far-field approximation. Additional delay elements are incorporated as second-stage processing to allow all subarrays to be coherently summed (i.e., global near-field beamforming can be achieved by simply delaying and then summing the outputs from all subarrays.) The delay-and-sum beamformer allows each subarray to “look” for signals radiating from a particular direction. By adjusting the delays associated with each element of the array, the array’s look direction can be electronically steered toward the source of radiation. Thus instead of looking in one direction as seen at 124a, the direction of tiles 120 can be steered in different direction 124b. The delay line requirement for each element in the sub-array can be less than a hundred stages. Only long delays for global summing are needed for the final near field focusing.

[0022] To scan an image plane using a steerable beamformer system a process such as that shown in FIG. 2 can be used. A raster scan 260 can be used to scan an image plane 262 using a 2D steerable transducer array 264.

[0023] A detailed diagram of an electronically-controlled beamforming system in accordance with the invention is shown in FIG. 3A. This system consists of a bank of parallel time-delay beamforming processors 330, -330N. Each processor 330 consists of two components: a 2D sub-array beamformer 332 for far-field beamsteering/focusing and an additional time delay processor 334 to allow hierarchical near-field beamforming of outputs from each corresponding subarray. The sub-arrays 332 include in-programmable delay lines 340 with tap selectors 342, multiplexers 344 and summed 346 output. As can be seen in FIG. 3A, for a system with n-sub-arrays, n-parallel programmable 2nd-stage near field time delays are needed for individual delay adjustment which are converted with A/D converter 352 to allow all n-parallel outputs be summed 354 coherently, in turn, this summed output is filtered 338 and provides the 3D images of the targeted object. A processor 336 controls sub-array operation. Use of the scan head with a second stage digital beamformer is shown in FIG. 3B. In this embodiment, a plurality of N sub-array beamformers 400 each receive signals from m transducer elements that have separate delay lines whose outputs are summed and provided to near-field beamformers 420 so that this beamformer can be a conventional system with conventional processor 480. A separate sub-array processor 460 controls beamformers 400.

[0024] Without using this hierarchical subarray far-field and then near-field beamforming approach, for an 80×80 element 2D array, a cable consisting of six thousand and four hundred wires is needed to connect the transducer array to a conventional beamforming system. As shown in FIG. 3A, the number of inputs to each subarray processor equals the total number of delay elements in the subarray, each subarray only has a single output. The number of inputs to the subarray bank equals the number of 2D array elements, and the number of outputs from the subarray bank equals to the total transducer array element number divided by the sub-

array element number, i.e., the number of outputs from the subarray bank reference to the number of inputs is reduced by a factor equal to the size of the subarray. For example, if one selects to use a 5×5 subarray to implement this hierarchical beamforming concept, after the first stage subarray beamforming, the total number of wires needed to connect to the 2nd stage near-field beamforming is reduced by a factor of 25. More specifically, as mentioned above, without using this 2D subarray beamforming, 6400 wires are needed to connect an 80×80-el 2D transducer array to a conventional back-end beamforming. Using a 5×5 subarray processing bank first, the number of wires required to connect to the backend beamforming system is reduced to 256. Based on the current invention, a bank of 256 5×5 element subarrays Beamformer can be integrated with a 80×80 element 2D array in the scan head, so a cable consisting of 256 wires is adequate to connect the integrated scan head with the back-end near-field beamforming system. It is important to note that 5×5 subarray far-field beamforming processors can be easily integrated in a small size Si integration circuit, eight of such 5×5 subarray beamforming can be integrated on one chip. Only 32 chips integrated into the scan head, it can reduce the cable size from 6,400 wires down to 256 wires.

[0025] A preferred embodiment of the invention for a 2D array beamforming, each minimizing noise and cable loss with improved S/N performance, are described in FIG. 4, 5 and 6. In all three implementations, the bank of m parallel subarray beamforming processors 520 and multiplexers 528 are integrated with the 2D transducer array 525 to create a compact, low-noise, scan head 500. FIG. 4 depicts a system that the compact scan head is connected to a dedicated processing module, in which the m-parallel preamp/TGCs 522 transmit/received chips 524 and the 2nd stage time delay processing units 526 are housed. This dedicated processing module communicates with a host computer 540 via FireWire or USB or PCI bus 542. Control and synchronization is performed by the system controller 544 located in the processing module or housing 546. FIG. 5 depicts the same architecture as stated in FIG. 4, except, inside the dedicated processing module, the 2nd stage time delay processing units are specifically implemented by using charge-domain programmable (CDP) time-delay lines 600 in housing 620 that is connected to handheld probe 660 and computer housing 648. FIG. 6B depicts a system that the compact sparse array scan head 700 is connected to a conventional, commercially available time-domain digital ultrasound imaging system 700 with n-parallel beamforming channels 760. It is easy to see that in FIG. 6A, the time-delay processor 720 can also be implemented by using CDP time-delay lines 740. In these embodiments the near-field beamforming is housed 720, 780 in the same housing with other image processing functions.

[0026] By systematically varying beamformer delays and shading along a viewing angle of a 2D transducer array, returned echoes along the line of sight representing the 3D radiation sources can be used to create the scanned image at the scanned angle. The system can provide continuous real-time large area scanned images throughout a large field of view at 20 frames/s or more. At this frame rate, the system can be used to display continuous 3D images vs. time, thus providing 4D information of the scanned object. As shown in FIG. 7 a CDP beamforming chip 810, a time multiplexed computing structure can be used to generate multiple beams,

i.e., for each transmit pulse, the bank of 2D subarray beamformers **818** and its corresponding 2nd stage near-field time-delay line are capable of providing multiple beams sequentially. The computing circuits sequentially generate the delays required for forming K beams. The device operates as follows. Once a set of sampled returned-echoes are loaded in the delay lines with sampling circuits **814**, at time t_1 , the delays required for forming beam **1** are computed **812** within each module **822** and applied in parallel to all delay lines. The sampled return-echoes with proper delays are coherently summed **802** and filtered **804** to form the first beam. At time t_2 , the delays required for forming beam **2** are computed within each module and applied in parallel to all delay lines. The sampled return-echoes with proper delays are coherently summed to form the second beam. The procedure repeats until the Kth beam is coherently formed.

[0027] For example, if a computing circuit with 16-serial addressable outputs is built in with the CDP subarray and the 2nd stage time delay lines, for each transmit pulse, 16 beams or scan lines each along a different scan angle can be created. For 256-pulses with a down-range depth of 15 cm, the system can generate a 4096-beams with a 64×64 pixel resolution at a frame rate of 20 frames/s. The system is fully programmable; the beamforming electronics can be adjusted to zoom-in to a smaller field-of-view for high-resolution or higher frame rate images. For example, using 192-transmit pulses with the same down-range depth of 15 cm, the system can generate a 3072-beams with a 64×48 pixel resolution at a 30 frame/s frame rate.

[0028] The array described addresses ultrasound imaging applications using a two-dimensional 2 cm×2 cm array at a frequency of 3 MHZ. The need for resolution on the order of less than half the wavelength dictates as large an aperture as possible that can be housed within a compact package. To interrogate a 90 degree scanning volume and also minimize the impact of grating lobes, an element pitch or separation of less than 0.25 mm is desirable, leading to a 80×80 element array. Using the subarray processing technique described above, a scan head with integrated subarray beamforming circuits followed by a 2nd stage near-field beamsteering/beamfocusing system provides a practical implementation. However, the implementation still requires at least 32 subarray chips to be integrated on a scan head. An alternative pseudo random array design approach can be used to achieve this resolution with a much less amount of processing components in the scanned head.

[0029] To make a sparse array practical, the combination of low insertion loss and wide bandwidth performance is important for realizing acceptable imaging performance with low illumination levels. Quarter-wave matching layers with low acoustic impedance, but physically solid backing results in a robust array that loses only 3-4 dB in the conversion of received signal energy to electrical energy. Array band-widths of 75% or more are typical of this design and construction process. Also, the transducer array employs element positioning and an interconnect system suitable for the beamformer circuitry. The electronics are mounted on printed-circuit boards that are attached to the transducer elements via flexible cables. In practice, a majority of the array elements are connected to outputs using the flexible cables. However, only a small fraction of the total number of elements are wired to the circuit boards. Nevertheless, the

large number of array element connections are sufficient to insure a unique pattern of active-element locations in the final array.

[0030] As an example of a sparse array, assuming a 2×2 cm array with 256 active elements, the resulting filling factor is 4%. The output signal to noise ratio of the array is proportional to the number of active elements, so this filling factor corresponds to a loss in sensitivity of -13 dB when compared to a filled array of the same dimensions. To compensate for this loss, a transmitted signal of wider bandwidth is chosen to increase array sensitivity. In the approach presented here, the sensitivity is increased on the order of 10 dB. Further details regarding sparse array devices can be found in U.S. Pat. No. 6,721,235, the contents of which is incorporated herein by reference.

[0031] Positioning the elements of the array follows the approach in which care must be taken to eliminate any periodicity that would produce grating lobes that compete with the main lobe. Pseudorandom or random arrays can be used (FIG. 8A). The geometry of activated element placement has been developed to maximize the efficiency of the beamformers while minimizing grating and side lobe clutter. Switching between a plurality of different array patterns is used to provide the most efficient beam pattern at different beam angles relative to the region or volume of interest being scanned. Thus, a first pattern can utilize that illustrated in FIG. 8A, which is then switched to a second pattern for a different scan angle. This can involve selecting a transducer element within a neighborhood **880** surrounding a given element to scan at a second angle.

[0032] The primary goal of the optimization method is to minimize the average side lobe energy. Specifically, this is done by interactively evaluating the optimization criterion:

$$J = \frac{1}{2u_{max}^2} \int \int_s W(u_x, u_y) B(u_x, u_y) d u_x d u_y, \quad (1)$$

where the weighting function, $W(u_x, u_y)$, applies more weight to regions in the array response that require side lobe reduction. The optimization method begins with no weighting (i.e., $W(u_x, u_y)=1$) and proceeds by choosing successively better weighting functions that satisfy the optimization criterion. Since the side lobes that require the greatest reduction are related to the previously computed beam pattern, $B(u_x, u_y)$, the weighting is chosen such that $W(u_x, u_y) = B(u_x, u_y)$. This is done in an interactive manner until convergence.

[0033] Basically, a random array is capable of producing an imaging point spread function that has a main lobe to average side lobe ratio of N, where N is the total number of active elements in the array. For the 256-element sparse array example, the resulting ratio is -13 dB. Using a wide bandwidth approach improves this ratio by 10 dB. Based on the preceding optimization criterion, a pseudorandom placement of the array elements was generated (FIG. 8A).

[0034] FIG. 8B is a plot of the array performance, sensitivity versus cross range, for a 256-element sparsely-sampled array at 3 MHZ. The peak to maximum side lobe level is approximately 30 dB. To improve this performance, the system is configured to achieve the maximum main lobe to clutter level ratio possible, which has been independently verified.

[0035] FIG. 9B depicts a system that the sparse array scan head 900 is connected to a conventional, commercially available time-domain digital ultrasound imaging system 940 with m-parallel beamforming channels. It is easy to see that in FIG. 9A, the time-delay processor can also be implemented by using CDP time-delay lines 920 in housing 925 that is connected to a separate computer 927. An array of m multiplexers 906 is used to switch between a sequence of scan patterns executed using a software program and system controller 940 or processor 950. The sequence of sparse array patterns is thus selected to scan at different scan angles of an object being imaged to provide 3D ultrasound imaging thereof.

[0036] A commercially available window-based 3D visualization software can be used to visualizing, manipulating, and analyzing the 3D multiple-beams volume image data generated by the electronically-adjustable acoustic conformal lens system. Traditionally, a clinician with 2D ultrasound images for diagnosis would look at the 2D scanned images slice by slice and mentally reconstruct the information into a 3D representation to judge the anatomy of the patient. This procedure requires the clinician to have well-founded experience as well as a highly sophisticated understanding of human anatomy. To create a “complete” image to the 3D structures, the clinician has to take all available slices into account. Looking at hundreds of slices is too time-consuming, even for a single patient. 3D visualization based on 3D volume data can help overcome this problem by providing the clinician with a 3D representation of the patient’s anatomy reconstructed from the set of multiple-scanned beamforming data.

[0037] A commercially available software tool such as KB-Vol3D of KB-VIS technologies, Chennai, India, provides display or viewing 3D features such as:

[0038] Fast Volume-Rendering

[0039] Shaded Surface Display

[0040] Shaded-Surface module allows easy visualization of surfaces in the volume. Surfaces may be created by intensity-based thresholding. Alternatively, the Seeding option allows selection of specific connected structures of interest.

[0041] MIP (Maximum Intensity Projection) with Radials

[0042] MPR (Multiple-Plane-Reformatting) with Oblique & Double-Oblique and 3D correlation

[0043] MRP Slabs & Multi-Cuts

[0044] Curved MPR

[0045] Color & Opacity Presets with Editor

[0046] Region-Growing and Volume Measurements

[0047] Cutaway Viewing with Slab-Volume and Interactive Real-time VOI

[0048] Volume-interiors are easily visualized using the “Cutaway-Viewing” tool. A Cut-Plane is used to slice through the volume, revealing the interior regions. The cut-plane is easily positioned and oriented using the mouse.

[0049] The VOI (Volume-of-Interest) tool allows interactive, real-time Volume-of-Interest display. The user can isolate and view sub-volumes of interest very easily and in real-time, using easy click-and-drag mouse operation.

[0050] Image Save in Multiple Formats

[0051] Images displayed by KB-Vol3D can be captured to various image formats (including DICOM, JPEG, and BMP etc.)

[0052] Movie Capture in AVI Format

[0053] Visualization operations can also be captured to an AVI movie .le and played on Windows Media Player, QuickTime, and Real Player etc.

[0054] The invention can be implemented using a scan head 12 connected to a portable computer 14 as shown in FIG. 10. the ultrasound system 10 can also include a cable 16 to connect the probe 12 to the processor housing 14. Certain embodiments can employ an interface unit 13 which can include a beamformer device. Scan head 12 can include a transducer array 15A (2D) and a circuit housing 15B which can house multiplexer and/or beamforming components as described in detail in U.S. Pat. Nos. 6,106,472 and 6,869,401, the entire contents being incorporated herein by reference.

[0055] The claims should not be read as limited to the recited order or elements unless stated to that effect. All embodiments that come within the scope and spirit of the following claims and equivalents thereto are claimed as the invention.

What is claimed is:

1. A medical ultrasound imaging system comprising: a two dimensional array of transducer elements in a probe housing;

a first beamformer device in the probe housing; a second beamformer device in a second housing, the second beamformer being in communication with the probe housing to receive beamformed data from the first beamformer device.

2. The system of claim 1 wherein the first beamformer device comprises a plurality of beamformer elements and a corresponding plurality of multiplexer elements.

3. The system of claim 1 further comprising a processor housing having an image processor programmed to perform 3D imaging Processing and Doppler processing.

4. The system of claim 3 wherein the second housing is connected to the probe housing with a first cable and is connected to the processor housing with a second cable.

5. The system of claim 1 wherein the two dimensional array has at least 256 elements.

6. The system of claim 1 wherein the first beamformer device comprises a plurality of sub-array beamforming channels.

7. The system of claim 1 wherein the second beamformer device comprises a digital beamformer.

8. The system of claim 1 wherein the first beamformer comprises a charge domain processor.

9. The system of claim 1 further comprising a processor programmed to actuate the system to collect at least 10 images per second.

10. A medical ultrasound scan head comprising: a two dimensional array of transducer elements in a probe housing; and

a first beamformer device in the probe housing, the first beamformer device having a plurality of sub-arrays.

11. The scan head of claim 10 wherein the first beamformer device comprises a plurality of multiplexer elements.

12. The scan head of claim 10 wherein the probe housing is connected to a processor housing with a first cable.

13. The scan head of claim 10 wherein the two dimensional array comprises a sparse array.

14. The scan head of claim 10 wherein the first beamformer device comprises a charge domain processor.

15. A medical ultrasound imaging system comprising:
a two dimensional array of transducer elements in a probe housing;
a switching device in the probe housing that switches the array from a first sparse array pattern to a second sparse array pattern; and
a processor programmed to sparsely actuate the transducer array.

16. The system of claim **15** wherein the probe housing contains a plurality of multiplexer elements that switches the array between a plurality of sparse array patterns.

17. The system of claim **15** further comprising a processor housing connected to the probe housing, the process housing having an image processor programmed to perform 3D imaging processing and Doppler processing and having a controller to sequentially actuate sparsely selected array elements.

18. The system of claim **15** wherein the two dimensional array comprises a sparse array having at least 256 transducer elements.

19. The system of claim **15** wherein the first pattern corresponds to a first scan angle and the second pattern corresponds to a second scan angle different from the first scan angle.

20. A medical ultrasound imaging system comprising:
a two dimensional array of transducer elements in a probe housing;
a multiplexing network in the probe housing to sparsely actuate the array elements;
a beamformer device in a second housing, the beamformer being in communication with the probe housing to transmit and receive data from selectively activated transducer elements; and
a controller in the second housing in communication with the probe housing to sequentially activate selected transducer elements.

* * * * *

专利名称(译)	超声3D成像系统		
公开(公告)号	US20080009739A1	公开(公告)日	2008-01-10
申请号	US11/474098	申请日	2006-06-23
[标]申请(专利权)人(译)	泰拉科技公司		
申请(专利权)人(译)	TERATECH CORPORATION		
当前申请(专利权)人(译)	TERATECH CORPORATION		
[标]发明人	CHIANG ALICE M BRODSKY MICHAEL HE XINGBAI WONG WILLIAM M		
发明人	CHIANG, ALICE M. BRODSKY, MICHAEL HE, XINGBAI WONG, WILLIAM M.		
IPC分类号	A61B8/14		
CPC分类号	A61B8/4483 A61B8/483 G01S7/52085 G01S7/52095 G01S15/8925 A61B8/4477 G01S15/8993 G10K11/346 G01S7/52082 G01S7/5208 A61B8/145 G01S15/8927 G01S15/8959 G01S15/8961		
其他公开文献	US7874991		
外部链接	Espacenet USPTO		

摘要(译)

超声成像系统技术领域本发明涉及一种超声成像系统，其中扫描头或者包括执行远场子阵列波束成形的波束形成器电路，或者包括激励所选元件的稀疏阵列选择电路。当与第二级波束形成系统一起使用时，可以生成三维超声图像。

