



(19) **United States**

(12) **Patent Application Publication**
Jensen et al.

(10) **Pub. No.: US 2012/0289828 A1**

(43) **Pub. Date: Nov. 15, 2012**

(54) **ULTRASOUND IMAGING SYSTEM**

(52) **U.S. Cl. 600/437**

(75) **Inventors:** **Ole Christian Jensen**, Vaerlose (DK); **Johannes Anders Smith**, Hellerup (DK); **Kaj E. Dunkan**, Stenlille (DK); **Torben Svanberg Nielsen**, Kobenhavn S (DK)

(57) **ABSTRACT**

An ultrasound imaging system includes a console and a key pad. The console includes a two dimensional display region having a vertical dimension and a horizontal dimension, wherein the horizontal dimension is smaller than the vertical dimension. The display region includes an upper portion configured to display image data and a lower portion configured to display, concurrently with displaying the image data in the upper portion, a touch screen menu including a set of soft controls that are respectively configured to control a secondary set of ultrasound imaging functions. The key pad includes a set of physical controls that are respectively configured to control a primary set of ultrasound imaging functions, wherein the key pad has a width that is less than a width of the console. In one embodiment, the key pad is hermetically sealed, and is easily cleanable, disinfected and/or sterilizable.


(73) **Assignee:** **ANALOGIC CORPORATION**, Peabody, MA (US)

(21) **Appl. No.:** **13/106,127**

(22) **Filed:** **May 12, 2011**

Publication Classification

(51) **Int. Cl.**
A61B 8/00 (2006.01)

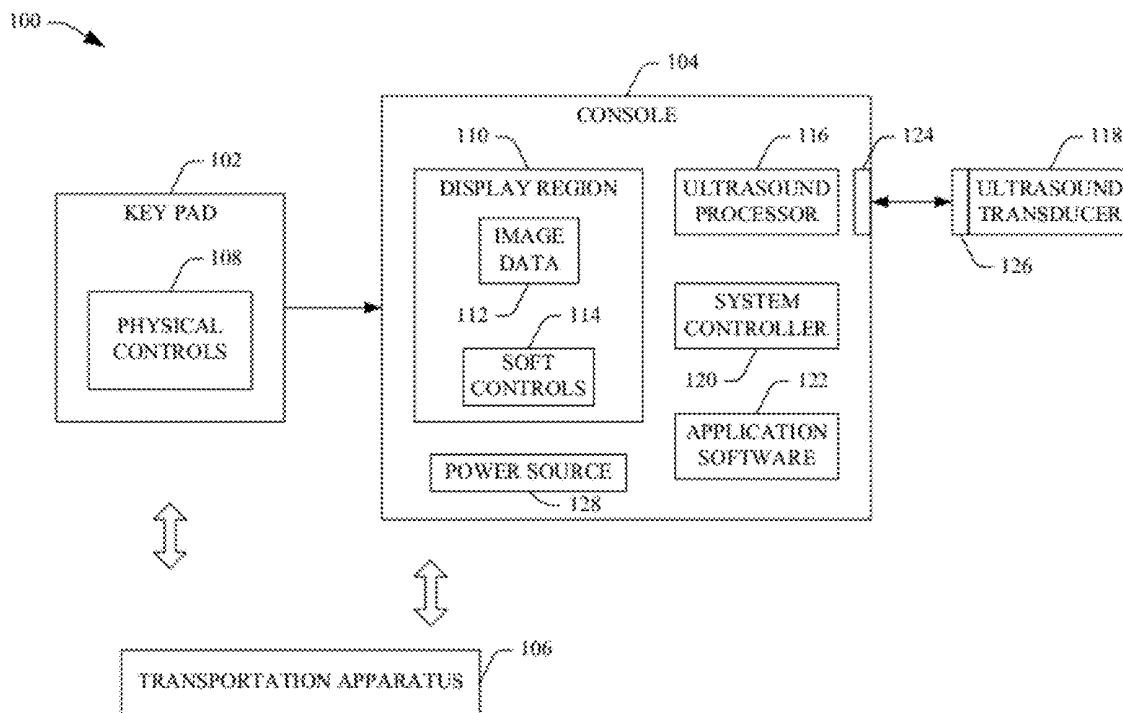

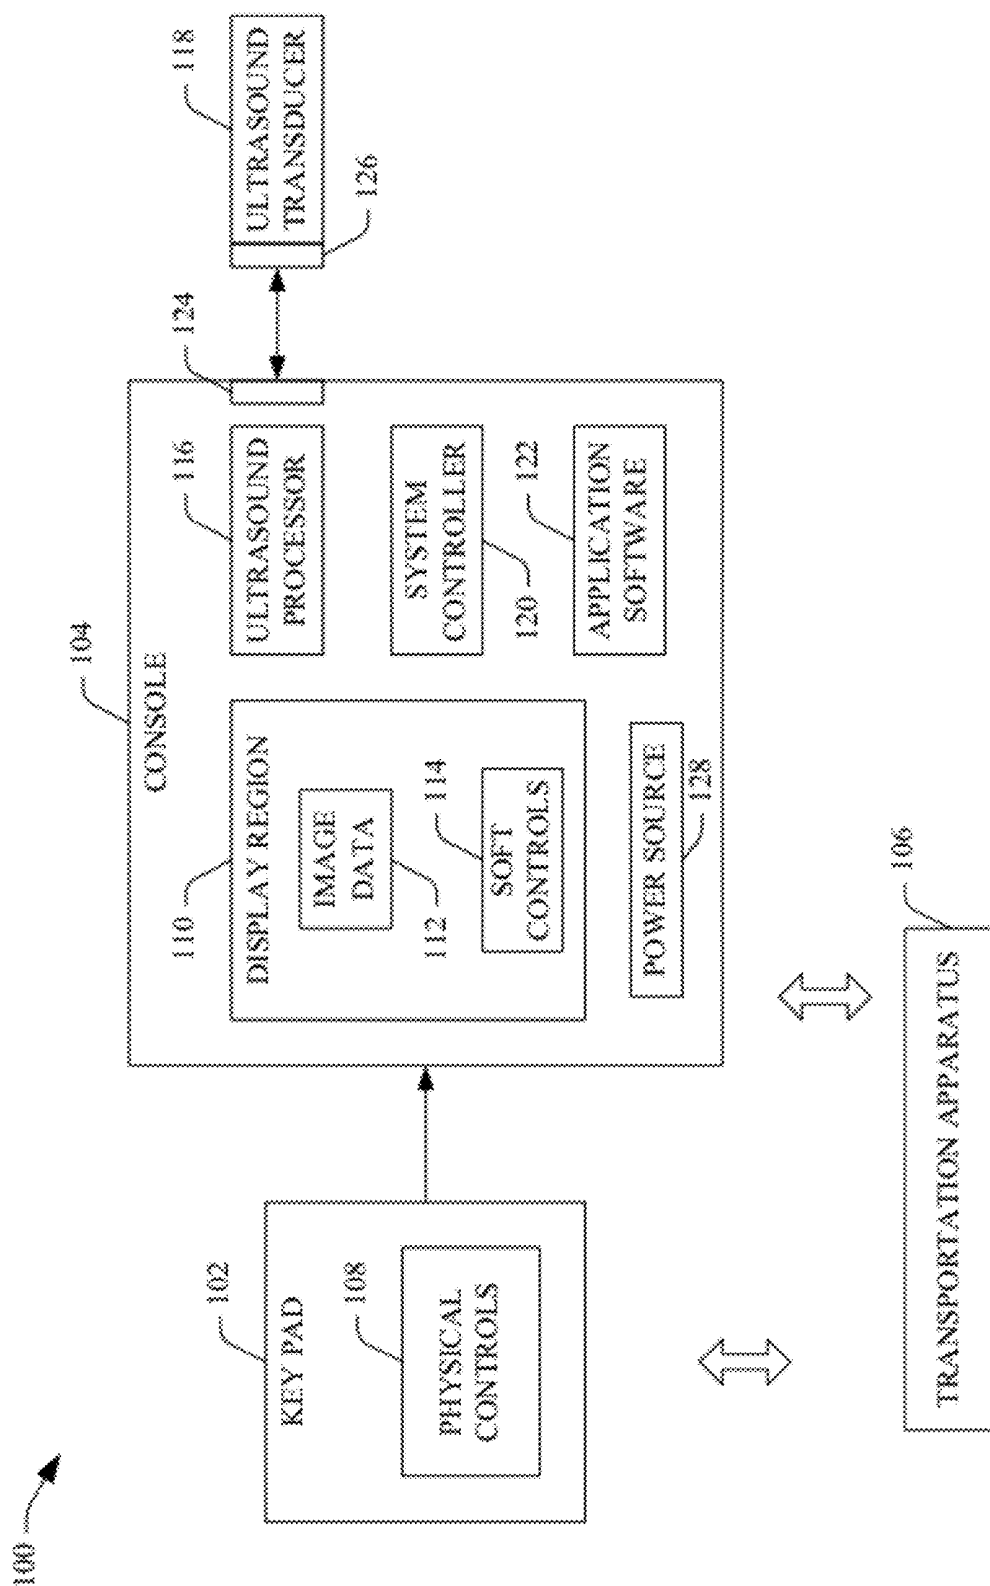


FIGURE 1


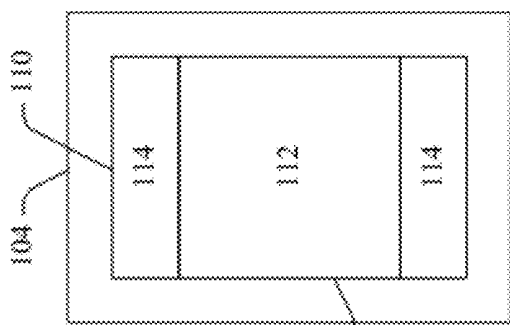


FIGURE 2


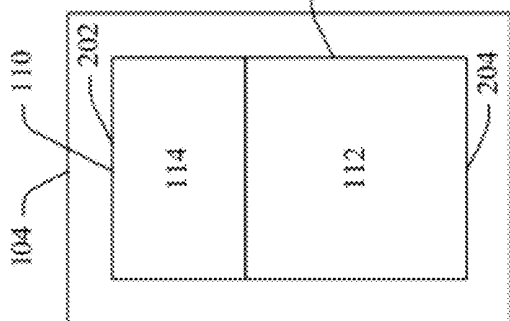


FIGURE 3

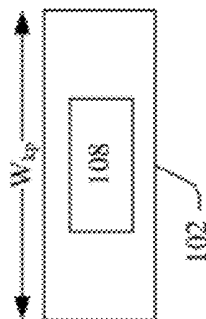
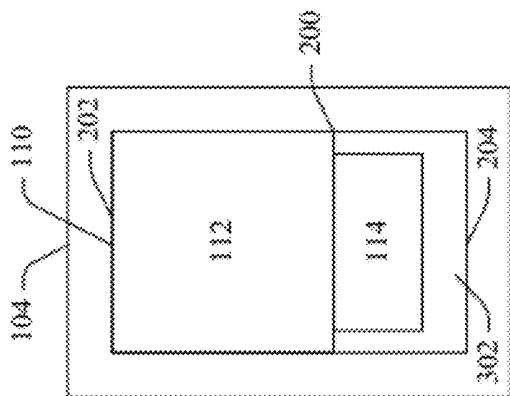


FIGURE 4


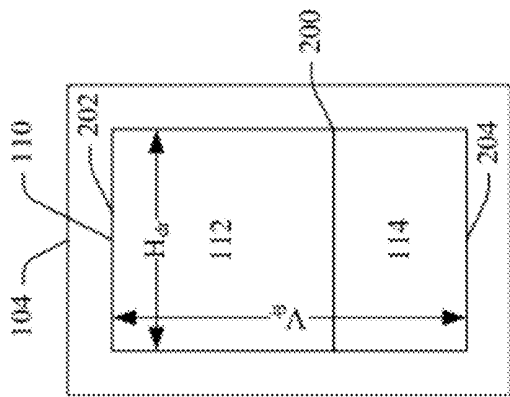


FIGURE 5

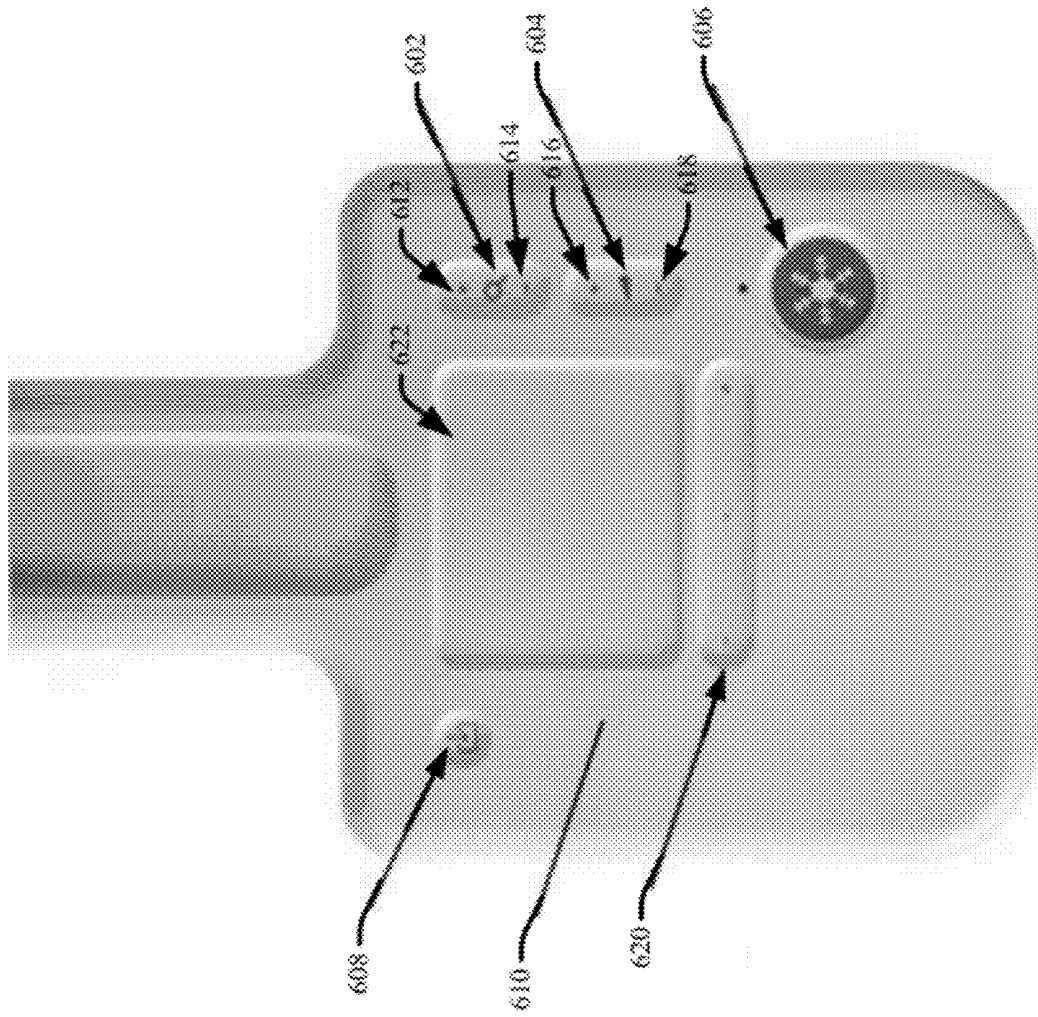


FIGURE 6

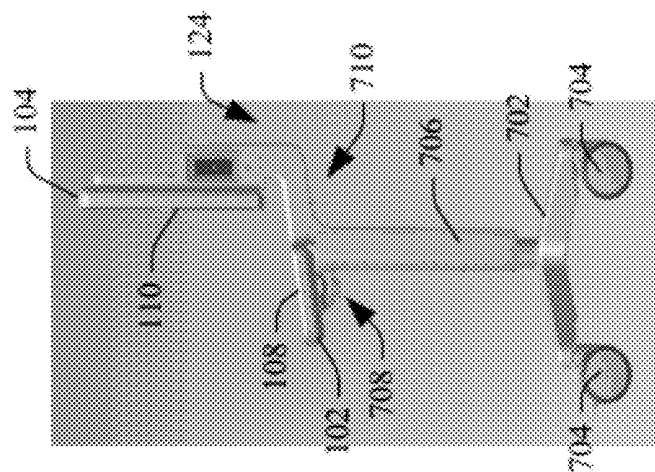


FIGURE 7

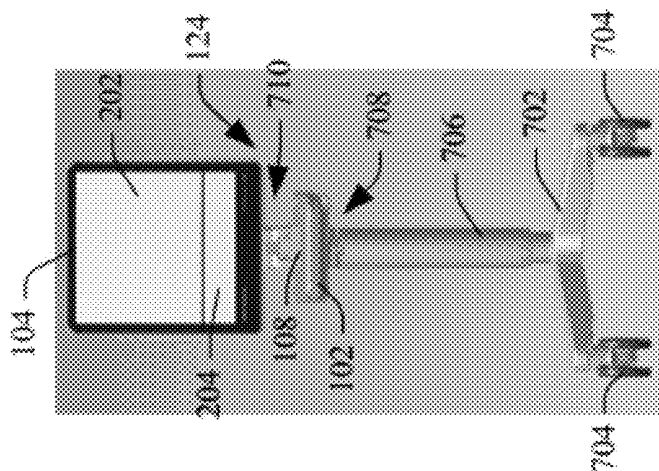


FIGURE 8

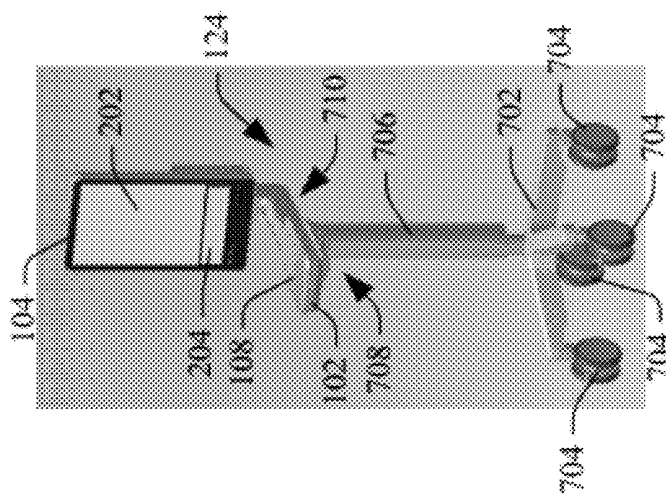


FIGURE 9

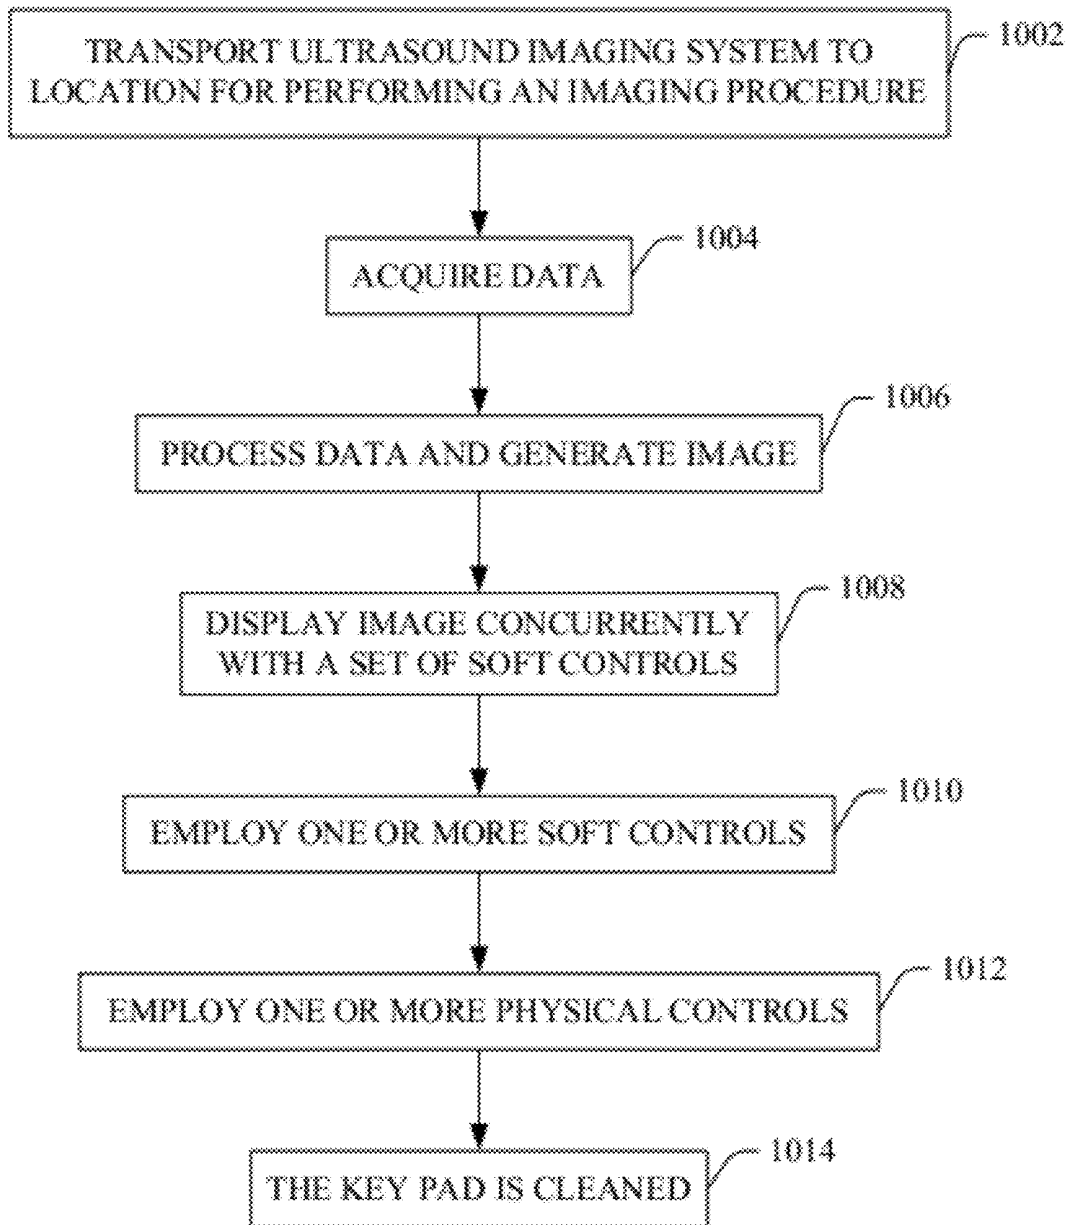


FIGURE 10

ULTRASOUND IMAGING SYSTEM

TECHNICAL FIELD

[0001] The following generally relates to ultrasound imaging and more particularly to a console and key pad of an ultrasound imaging system.

BACKGROUND

[0002] Ultrasound scanners provide useful information about the interior characteristics of an object under examination. In medical applications, clinicians have used ultrasound scanners to examine human subjects in settings such as hospitals, physician's offices, and other locations. Ultrasound scanners have been alternately used in the emergency room, operating room, radiology department, patient room, and similar environments. As such, it is sometimes desirable to transport the scanner from room-to-room. To this end, ultrasound scanners have been equipped with wheeled carts that allow the scanner to be rolled along the floor.

[0003] In a typical environment, a user of the scanner places the transducer on the body over the tissue of interest and begins scanning. A monitor displays the information sensed by the transducer. The user may desire to change scanner parameters or settings, or determine a characteristic about the displayed information. For example, the user may want to increase the gain, adjust depth, change the zoom factor, etc. Such actions have required user interaction with a keyboard of the ultrasound scanner. For example, a conventional ultrasound scanner has included a keyboard with twenty or more keys, and the user activates a corresponding key to invoke a desired function.

[0004] Unfortunately, with twenty or more keys, it may not be readily convenient or easy for the user to locate and activate the key for the desired function. Furthermore, in such environments, the scanner may also come into contact with bodily fluids, which may get on and/or between keyboard keys, making it more difficult to clean the system after the procedure. Applications for these scanners may also place a premium on size. For example, in an operating room, space is often at a premium. Unfortunately, keyboards with twenty or more keys can be wider than the monitor, making the footprint of the system wider than needed to view images.

SUMMARY

[0005] Aspects of the application address the above matters, and others.

[0006] In one aspect, an ultrasound imaging system includes a console and a key pad. The console includes a two dimensional display region having a vertical dimension and a horizontal dimension, wherein the horizontal dimension is smaller than the vertical dimension. The display region includes an upper portion configured to display image data and a lower portion configured to display, concurrently with displaying the image data in the upper portion, a touch screen menu including a set of soft controls that are respectively configured to control a secondary set of ultrasound imaging functions. The key pad includes a set of physical controls that are respectively configured to control a primary set of ultrasound imaging functions, wherein the key pad has a width that is less than a width of the console.

[0007] In another aspect, an ultrasound imaging system includes a console with a display region arranged in a portrait orientation, wherein the display region concurrently presents

ultrasound image data generated by the system and a set of soft secondary ultrasound imaging controls in different portions of the display region. The system further includes a key pad including a set of primary ultrasound imaging controls. The system further includes an interface configured to electrically communicate with a complementary interface of an ultrasound transducer.

[0008] In another aspect, a method includes concurrently displaying ultrasound image data and a set of soft controls vertically with respect to each other in a same display region of a console of an ultrasound imaging system, wherein a set of physical controls are part of a key pad of the ultrasound imaging system, which is narrower than the console of the ultrasound imaging system.

[0009] Those skilled in the art will recognize still other aspects of the present application upon reading and understanding the attached description.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The application is illustrated by way of example and not limitation in the figures of the accompanying drawings, in which like references indicate similar elements and in which:

[0011] FIG. 1 illustrates an example ultrasound imaging system including a key pad and a console;

[0012] FIG. 2 illustrates an example display region of the console in which a set of soft controls is visually presented below image data;

[0013] FIG. 3 illustrates an example display region of the console in which at least one of image data or a set of soft controls is scalable and/or positionable within the display region;

[0014] FIG. 4 illustrates an example display region of the console in which a set of soft controls is presented above image data;

[0015] FIG. 5 illustrates an example display region of the console in which image data is presented between two sets of soft controls;

[0016] FIG. 6 illustrates an example of the key pad, including physical controls thereof;

[0017] FIG. 7 illustrates a perspective view of an example of the ultrasound imaging system;

[0018] FIG. 8 illustrates a front view of an example of the ultrasound imaging system;

[0019] FIG. 9 illustrates a side view of an example of the ultrasound imaging system; and

[0020] FIG. 10 illustrates an example method for using the ultrasound imaging system.

DETAILED DESCRIPTION

[0021] FIG. 1 illustrates an ultrasound imaging system **100**, which includes a key pad **102**, a console **104**, and a transportation apparatus **106** to which the key pad **102** and the console **104** are affixed.

[0022] The key pad **102** includes a set of physical controls **108** configured to activate and/or control at least one imaging function of the ultrasound imaging system **100**. In one non-limiting instance, the set of physical controls **108** make up a primary set of controls (which is a sub-set of the total number of controls), which include a set of controls that are generally used more often and/or frequently for performing imaging procedures than other controls.

[0023] As described in greater detail below, in one instance, the set of physical controls **108** includes less than ten, less

than five, or other non-zero number of controls configured to activate at least one imaging function, which allows for a relatively narrow key pad **102**, relative to a configuration in which the key pad **102** includes more controls. The set of physical controls **108** can also be configured such that they are part of a hermetically sealed surface of the key pad **102**.

[0024] The console **104** includes a human readable display region **110**, which is configured to concurrently display both image data **112** and a touch screen menu including a soft controls **114** configured to activate and/or control at least one imaging function. In one non-limiting instance, the set of soft controls **114** make up a secondary set of controls (which is another sub-set of the total number of controls), which include a set of controls that are generally used less often and/or frequently than the primary controls.

[0025] As described in greater detail below, the display region **110** is configured such that a spatial orientation of the image data **112** and the soft controls **114**, with respect to each other, provides for narrow console footprint with a large image display and easily visualized and readily accessible soft controls **114**. For example, in one instance, the set of soft controls **114** are visually presented concurrently with and below the image data **112** in the display region **110**.

[0026] It is to be appreciated that the large image display facilitates viewing a relatively large distance like across a surgical bed, allows for presentation of details without loss of overview without zooming in, allows for display of two planes/views in near fill size, additional images or information like Doppler spectrums, 3D cubes, measurements, etc. A narrow footprint allows for using the system **100** in small rooms such as operating rooms, easily transporting the system **100** in hallways, crowded elevators, from room to room, etc.

[0027] The console **104** further includes an ultrasound processor **116** configured to interface with an ultrasound transducer **118** that transmits ultrasound signals and receives echoes when utilized to perform an ultrasound procedure. The ultrasound processor **116** generates, based on the received echoes, two dimensional (2D), three-dimensional (3D) or other ultrasound image data indicative of an object under examination.

[0028] A system controller **120** controls the console **104** including one or more components thereof based on application software **122** stored on physical memory thereof and/or accessible thereto. For example, the system controller **120** can control the console **104** such that the ultrasound image data is the image data **112** displayed in the display region **110**. In another example, the system controller **120** can control the console **104** such that the soft controls **114** are based on one or more instructions of the application software **122**.

[0029] The console **104** further includes an interface **124** configured to connect with a complementary interface **126** of the ultrasound transducer **118**. The interfaces **124** and **126** include suitable pathways and/or connectors for conveying control and/or data signals between the console **104** and the transducer **118**.

[0030] A suitable ultrasound transducer **118** includes a single element transducer or a multiple element transducer array, which captures information for two dimensional, three dimensional, four dimensional, Doppler, and/or other ultrasound imaging modes. The interface **124** may be configured to alternately interface with other probes, for example, different frequency probes, probes with different capabilities, and/or other probes.

[0031] The transportation apparatus **106** includes wheels or the like. As such, the transportation apparatus **106** and hence the key pad **102**, the console **104**, and the ultrasound transducer **118** can be transported from one room to another room and/or within a room.

[0032] A power source **128** includes a power converter for converting power from an outside source such as a power cube, a power supply, an AC receptacle, or other power source for powering electrical components of the imaging system **100**. The power source **128** may additionally or alternatively include a primary (non-rechargeable) battery, a secondary (rechargeable) battery, a super capacitor, and/or the like that supplies power for one or more of the components of the imaging system.

[0033] FIGS. 2-5 illustrate various non-limiting examples of the display region **110** of the console **104** in connection with the key pad **102** and the physical controls **108**. Initially referring to FIG. 2, the console **104** includes a monitor **200**, such as a liquid crystal display (LCD), plasma, light emitting diode (LED), cathode ray tube (CRT), or other monitor, which is integrated in and is part of the console **104**.

[0034] The display region **110** is two dimensional and includes a vertical dimension V_{dr} and a horizontal dimension H_{dr} , which is less than the vertical dimension V_{dr} . Generally, this orientation can be considered as "portrait" in contrast to "landscape" in which the horizontal dimension is greater than the vertical dimension. A first or upper portion **202** of the display region **110** is configured to visually present the image data **112**. In the illustrated embodiment, the portion **202** is generally quadratic in shape. A second or lower portion **204** is configured to visually present the soft controls **114**.

[0035] This configuration of upper and lower portions **202** and **204** allows for a narrow footprint (with respect to the horizontal dimension of the system) with a large image display covering the horizontal footprint of the display region **110** with the soft controls **114** located just below the image data **112** such that the user can identify and employ the soft controls **114** without moving his/her eyes way from the image data. In addition, positioning the soft controls **114** as such shortens the distance between the image data **112** and the soft controls **114**.

[0036] The key pad **102** is located below (with respect to the vertical dimension V_{dr}) the console **104** and has a width W_{kp} , which is less than a width W_c of the console **104**, and, thus, does not increase the footprint in the horizontal direction relative to the console **104**. Note that the key pad **102** can be smaller relative to a configuration in which all of the controls are part of the key pad **102**. In addition, the key pad **102** and lower portion **204** provide the feel as is one is an extension of the other or that they are part of the same set of controls.

[0037] FIG. 3 is substantially similar to FIG. 2 except that the soft controls **114** do not occupy the entire lower portion **204**. In this example, a region **302** not occupied by the soft controls can be used to present other information or no information at all. Furthermore, the window of the soft controls may be moveable and/or scalable within the lower portion **204**. Although not shown, this may also apply to the image data **112** and the upper portion **202**. In this example, the key pad width W_{kp} is about a same size as the console W_c . In another instance, W_{kp} can be greater than W_c .

[0038] FIG. 4 shows another embodiment in which the upper portion **202** presents the soft controls **114** and the lower portion **204** presents the image data **112**. FIG. 5 shows another embodiment in which one sub-portion of the soft

controls **114** is located above the image data **112** and another sub-portion of the soft controls **114** is located below the image data **112**. In another instance, the display region **110** is configured such that the user can variously position the image data **112** and/or the soft controls **104** within the display region **110**.

[0039] FIG. 6 illustrates an example key pad **102** and physical controls **108**.

[0040] In this example, the physical controls **108** includes four (4) function controls—a gain function control **604**, a depth function control **602**, a freeze function control **606**, and a print/store function control **608**. A region over each of the controls **602-608** includes a visual graphic or indicia representing the control. In the illustrated embodiment, the visual graphic or indicia are located in a recess in the surface **610**. The visual graphic allows the user to easily visually identify a particular control offered through the key pad **102**.

[0041] The gain function control **604** includes dedicated increase and decrease adjusters **616** and **618**, and the depth function control **602** includes dedicated increase and decrease adjusters **612** and **614**. A shared increase and decrease adjuster **620** can also be used to increase and decrease the gain and depth. The adjuster **620** can further be used to adjust a soft control **114**, which is selected by hovering the screen cursor over a function of interest and/or otherwise.

[0042] The adjusters **612-620** respectively include proximity sensors (e.g., capacitive, magnetic, etc.) and/or touch sensitive areas located under or behind a surface **610** of the key pad **110**. A region over each of the sensor includes a visual graphic or indicia representing the corresponding function (e.g., “+” or “-”). In the illustrated embodiment, the sensor indicia are located in the recess in the surface **610** (along with the control indicia). The sensor visual graphics allow the user to easily visually identify and employ a particular function for a control. The adjusters **612-620** can be actuated by bringing a finger close to the sensors, touching the sensors, and/or sliding the finger along the sensors in a recess.

[0043] A touch pad **622** is used to move a graphical cursor or pointer presented in the display region **110**. Likewise, the touch pad **622** is located in a recess of and behind the surface **610**.

[0044] In the illustrated embodiment, the surface **610** is sealed (e.g., hermetically). This facilitates preventing foreign matter such as bodily fluids, liquids, dirt, etc. from entering the key pad **102** through the surface **610** such as in connection with the various controls **602-608**, adjusters **612-620** and touch pad **622**. The sealed surface and the recesses in the surface **610** render the surface **610** easily cleanable. In one instance, this include disinfectable and/or sterilizable.

[0045] In an alternative embodiment, the key pad **102** also includes one or more indicators such as a visual indicator (e.g., a light emitting diode (LED)), an audible indicator, etc. to provide feedback to an operator. Suitable feedback may relate to a currently activated function control, sensed touch, power status, etc.

[0046] It is to be understood that the set of controls illustrated in this example are provided for explanatory purposes and is not limiting. As such, in other embodiment, more, less the same and/or different controls may be part of the controls **108**. Examples of other controls include, but are not limited to, controls for setting parameters, making measurements, controlling operation, selecting a scanning mode, initiate

scanning, etc. One or more of these and/or other functions may additionally or alternatively be part of the set of soft controls **104**.

[0047] FIGS. 7-9 illustrate an example of the key pad **102** and the console **104** in connection with the transportation apparatus **106**. FIG. 7 illustrates a perspective view, FIG. 8 illustrates a front view, and FIG. 9 illustrates a side view.

[0048] In this example, the transportation apparatus **106** includes a base portion **702** with four (4) or other desired number of wheels **704**, which allow the imaging system **100** to be rolled from location to location such as operating room to operating room or other location. One end of a post **706** is affixed to the base portion and the other end of the post **706** includes a first region **708** to which the key pad **102** attaches and a second region **710** to which the console **104** attaches. The post **708** may be a fixed height or include a telescoping or otherwise height adjustable member, which can be used to adjust the height of the key pad **102** and the console **104**.

[0049] In the illustrated embodiment, the console **104** attaches to the second region **710** such that the surface of the display region **110** and upper and lower regions **202** and **204** is generally perpendicular to the floor. The key pad **102** attaches to the first region **708** such that the key pad runs at a slight angle downward horizontally from the console **104** from just below the display region **110** away from the console **104**. In one instance, the relative position of the key pad **102** and/or the console **104** is adjustable in that they can pivot, rotate and/or translate.

[0050] In another embodiment, the key pad **102** and/or the console **104** are removeably affixed to the transportation apparatus **124** or affixed to another apparatus such as a generally stationary apparatus mounted to a floor, wall, ceiling and/or the like. In the illustrated embodiment, the console **104** includes an LCD monitor. In another embodiment, the console **104** can include a plasma, CRT, or other monitor.

[0051] FIG. 10 illustrates an example method for employing the imaging system **100**.

[0052] It is to be understood that the following acts are provided for explanatory purposes and are not limiting. As such, one or more of the acts may be omitted, one or more acts may be added, one or more acts may occur in a different order (including simultaneously with another act), etc.

[0053] At **1002**, an ultrasound imaging system is transported to a location for performing an imaging procedure. As discussed herein, the narrow footprint of the key pad **102** and the console **104** allows the system **100** to be used in areas with limited space such as an operating room.

[0054] At **1004**, ultrasound data is acquired.

[0055] At **1006**, the ultrasound data is processed, generating at least one image.

[0056] At **1008**, the image is presented in a display region concurrently with a set of soft controls. As described herein, the display orientation can be a portrait orientation as shown FIG. 2 and/or other figures, which allows for display of a large image in an upper portion **202** of the display region **110** and the soft controls in a lower portion **202** of the display portion **110**, which is below the upper portion **202**.

[0057] At **1010**, optionally, one or more of the soft controls are employed to invoke one or more secondary ultrasound imaging functions.

[0058] At **1012**, optionally, one or more physical controls **108** of the key pad **102** are employed to invoke one or more primary ultrasound imaging functions. As described herein,

the physical controls **108** on the key pad **102** provide extremely simple and fast access to primary functions.

[0059] At **1014**, after the imaging procedure, the key pad **102** is cleaned. As discussed herein, the fully sealed surface with the controls **108** is easily cleaned.

[0060] The application has been described with reference to various embodiments. Modifications and alterations will occur to others upon reading the application. It is intended that the invention be construed as including all such modifications and alterations, including insofar as they come within the scope of the appended claims and the equivalents thereof.

What is claimed is:

1. An ultrasound imaging system, comprising:
a console includes a two dimensional display region having a vertical dimension and a horizontal dimension, wherein the horizontal dimension is smaller than the vertical dimension, and the display region includes an upper portion configured to display image data and a lower portion configured to display, concurrently with displaying the image data in the upper portion, a touch screen menu including a set of soft controls that are respectively configured to control a secondary set of ultrasound imaging functions; and
a key pad including a set of physical controls that are respectively configured to control a primary set of ultrasound imaging functions, wherein the key pad has a width that is less than a width of the console.
2. The system of claim 1, wherein the set of physical controls includes less than ten physical controls configured to activate different ultrasound imaging functions.
3. The system of claim 1, wherein the set of physical controls includes less than five physical controls configured to activate different ultrasound imaging functions.
4. The system of claim 3, wherein the set of physical controls are configured to adjust a level of at least one of gain or depth.
5. The system of claim 4, wherein the set of physical controls are configured to control at least one soft control that visually presented in the two dimensional display region.
6. The system of claim 1, the key pad, further comprising: a hermetically sealed surface that includes regions for activating the set of physical controls.
7. The system of claim 6, wherein the regions are part of the hermetically sealed surface and are recessed portions of the hermetically sealed surface.
8. The system of claim 7, further including touch sensitive areas that sense tactition of the recessed regions and generate a signal indicative thereof.
9. The system of claim 6, wherein the hermetically sealed surface is at least one of disinfectable or sterilizeable.
10. The system of claim 1, wherein the display region is part of a single monitor that is integrated in and part of the console.

11. The system of claim 1, wherein the display region is configured in a portrait orientation.

12. The system of claim 1, wherein the secondary set of ultrasound imaging functions are utilized less frequently than the primary set of ultrasound imaging functions.

13. An ultrasound imaging system, comprising:

a console with a display region arranged in a portrait orientation, wherein the display region concurrently presents ultrasound image data generated by the system and a set of soft secondary ultrasound imaging controls in different portions of the display region;

a key pad including a set of primary ultrasound imaging controls; and

an interface configured to electrically communicate with a complementary interface of an ultrasound transducer.

14. The system of claim 13, wherein the set of primary ultrasound imaging controls includes four or less controls configured to control different ultrasound imaging functions.

15. The system of claim 14, wherein the set of primary ultrasound imaging controls is part of a hermetically sealed surface of the key pad.

16. The system of claim 15, wherein the set of primary ultrasound imaging controls control at least one of gain, depth, freeze or print/store functions.

17. The system of claim 16, wherein a width of the key pad is narrower than the a width of the display region.

18. A method, comprising:

concurrently displaying ultrasound image data and a set of soft controls vertically with respect to each other in a same display region of a console of an ultrasound imaging system, wherein a set of physical controls are part of a key pad of the ultrasound imaging system, which is narrower than the console of the ultrasound imaging system.

19. The method of claim 18, wherein the set of physical controls includes four or less controls configured to control different ultrasound imaging functions.

20. The method of claim 18, wherein the set of physical controls is part of a hermetically sealed surface of the key pad.

21. The method of claim 18, further comprising:

receiving an input indicative of a user selected one of the soft controls; and

invoking a corresponding ultrasound imaging function in response to receiving the input.

22. The method of claim 18, further comprising:

receiving an input indicative of a user selected one of the physical controls; and

invoking a corresponding ultrasound imaging function in response to receiving the input.

* * * * *

专利名称(译)	超声成像系统		
公开(公告)号	US20120289828A1	公开(公告)日	2012-11-15
申请号	US13/106127	申请日	2011-05-12
申请(专利权)人(译)	ANALOGIC CORPORATION		
当前申请(专利权)人(译)	B-k医疗APS		
[标]发明人	JENSEN OLE CHRISTIAN SMITH JOHANNES ANDERS DUNKAN KAJ E NIELSEN TORBEN SVANBERG		
发明人	JENSEN, OLE CHRISTIAN SMITH, JOHANNES ANDERS DUNKAN, KAJ E. NIELSEN, TORBEN SVANBERG		
IPC分类号	A61B8/00		
CPC分类号	A61B8/4405 A61B8/467 A61B8/463 A61B8/461		
其他公开文献	US9119586		
外部链接	Espacenet USPTO		

摘要(译)

超声成像系统包括控制台和键盘。控制台包括具有垂直尺寸和水平尺寸的二维显示区域，其中水平尺寸小于垂直尺寸。显示区域包括：上部，被配置为显示图像数据；以及下部，被配置为与在上部显示图像数据同时显示包括一组软控制的触摸屏菜单，所述软控制被分别配置为控制次级组。超声成像功能。键盘包括一组物理控件，其分别被配置为控制一组主要的超声成像功能，其中键盘的宽度小于控制台的宽度。在一个实施例中，键盘是气密封的，并且易于清洁，消毒和/或消毒。

