



US 20150080735A1

(19) **United States**(12) **Patent Application Publication**
HYUN et al.(10) **Pub. No.: US 2015/0080735 A1**(43) **Pub. Date: Mar. 19, 2015**(54) **METHOD AND APPARATUS FOR
PROVIDING ULTRASOUND INFORMATION
BY USING GUIDELINES****G06T 7/20** (2006.01)**A61B 8/06** (2006.01)(52) **U.S. Cl.**CPC . **A61B 8/488** (2013.01); **A61B 8/06** (2013.01);**A61B 8/5269** (2013.01); **A61B 8/463**(2013.01); **G06T 7/20** (2013.01); **G06T 2200/24**(2013.01); **G06T 2207/10132** (2013.01); **G06T****2207/20104** (2013.01); **G06T 2207/30101**

(2013.01)

USPC **600/454**; 600/453; 382/103(71) Applicant: **SAMSUNG MEDISON CO., LTD.**,
Gangwon-Do (KR)(72) Inventors: **Dong-Gyu HYUN**, Gangwon-do (KR);
Seok-Won CHOI, Gangwon-Do (KR)(21) Appl. No.: **14/485,650**(22) Filed: **Sep. 12, 2014**(30) **Foreign Application Priority Data**

Sep. 13, 2013 (KR) 10-2013-0110613

Publication Classification(51) **Int. Cl.****A61B 8/08** (2006.01)**A61B 8/00** (2006.01)(57) **ABSTRACT**

Disclosed are an ultrasound information providing method and apparatus. The ultrasound information providing method includes generating a Doppler image from Doppler data of an object, acquiring a guideline indicating a moving path of the object in the Doppler image, correcting the Doppler data on the basis of an angle between the guideline and a beam axis of a probe, and displaying a Doppler image generated from the corrected Doppler data.

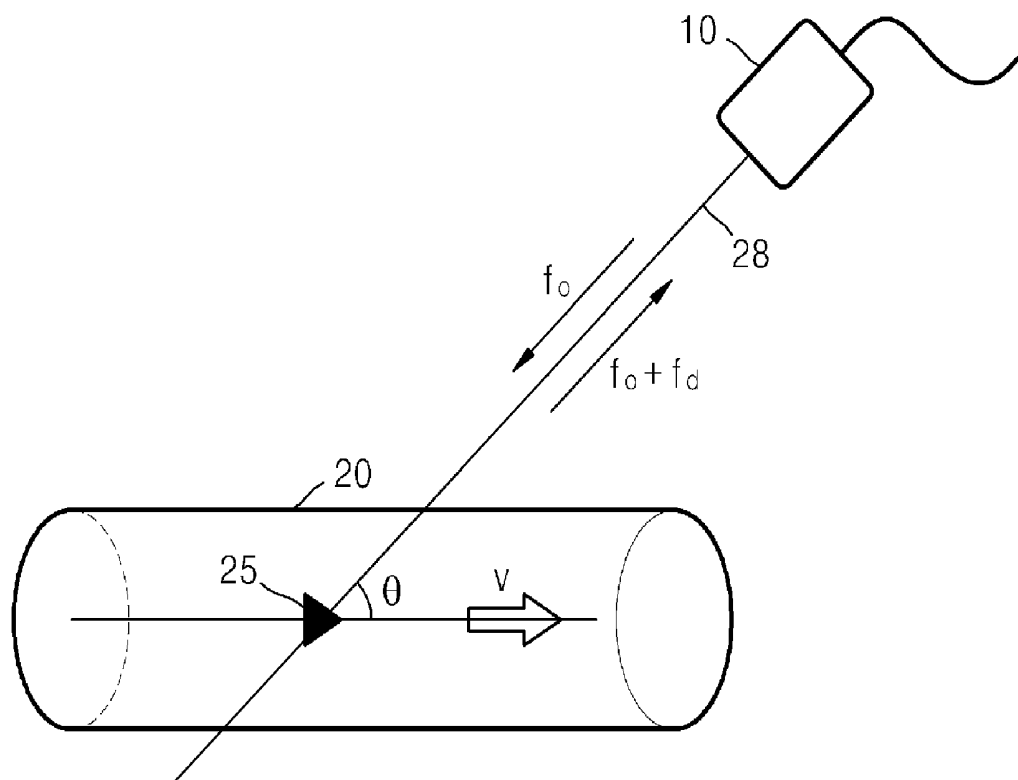


FIG. 1

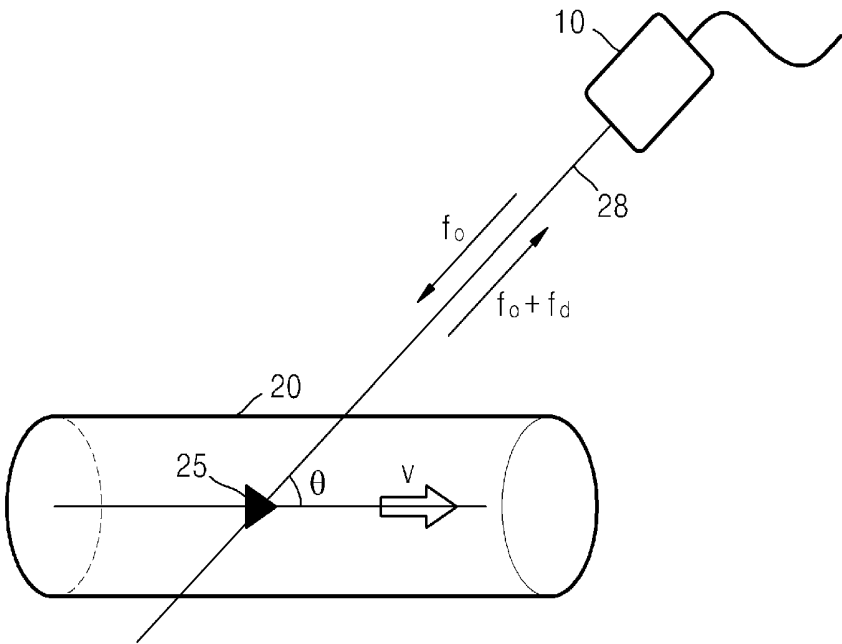


FIG. 2

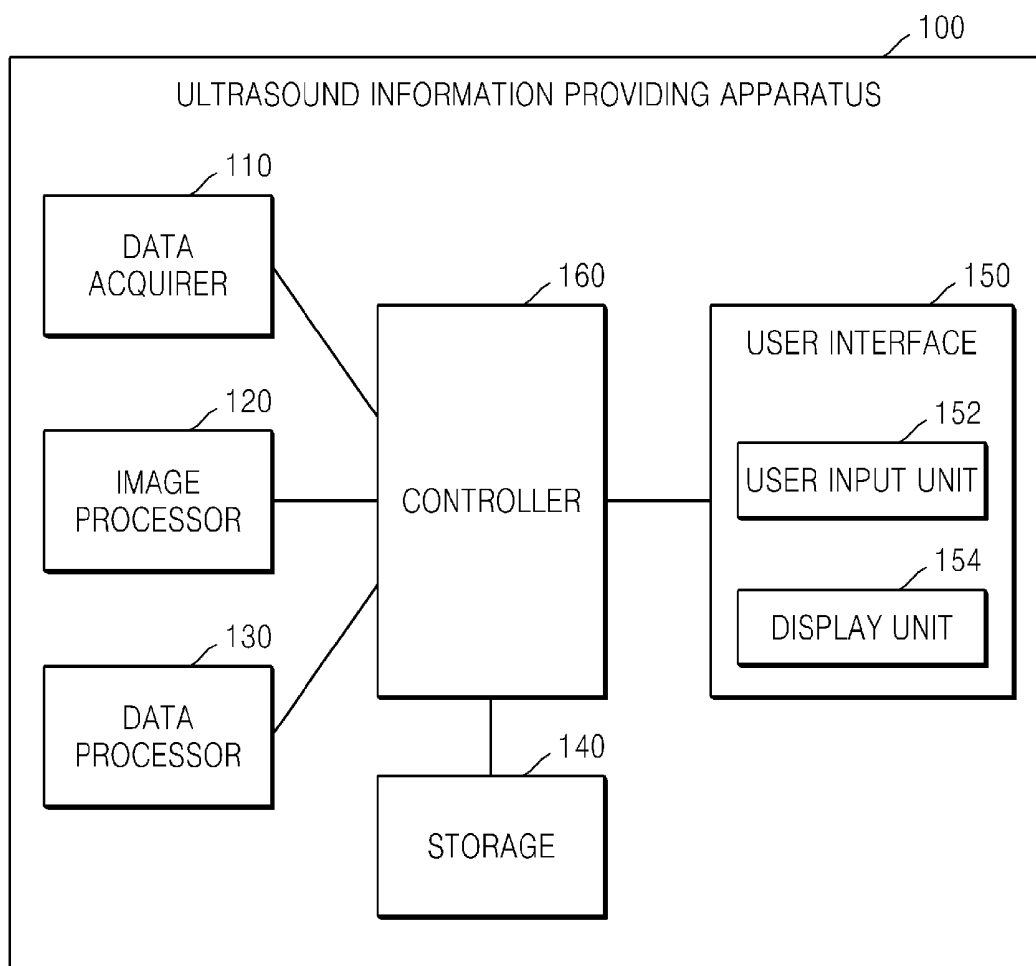


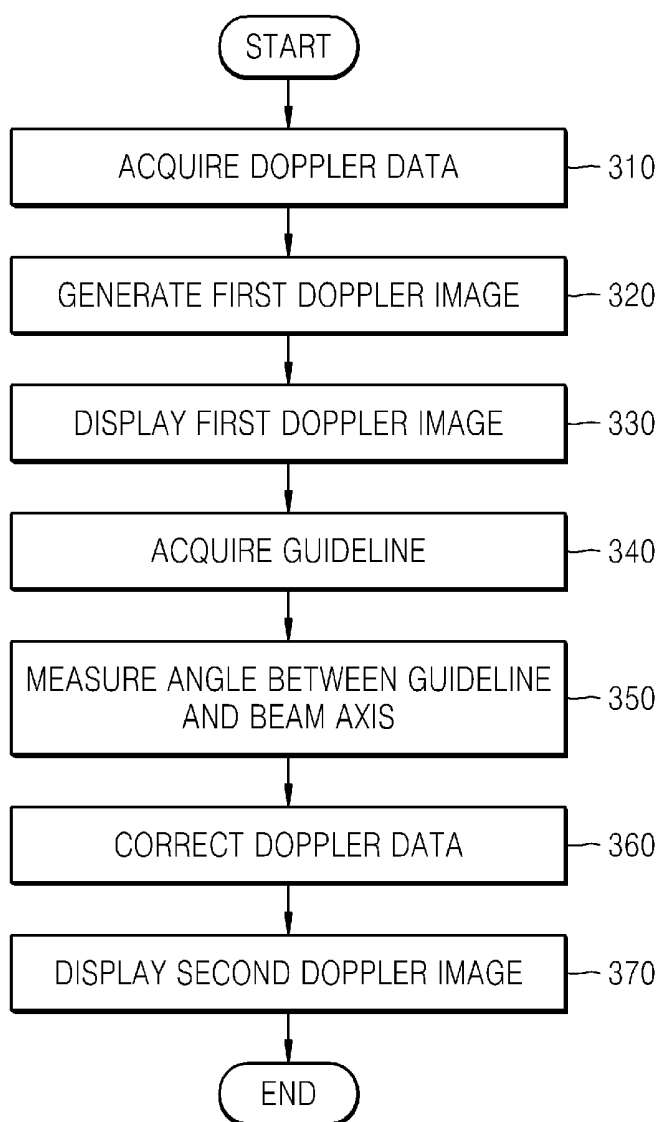
FIG. 3

FIG. 4

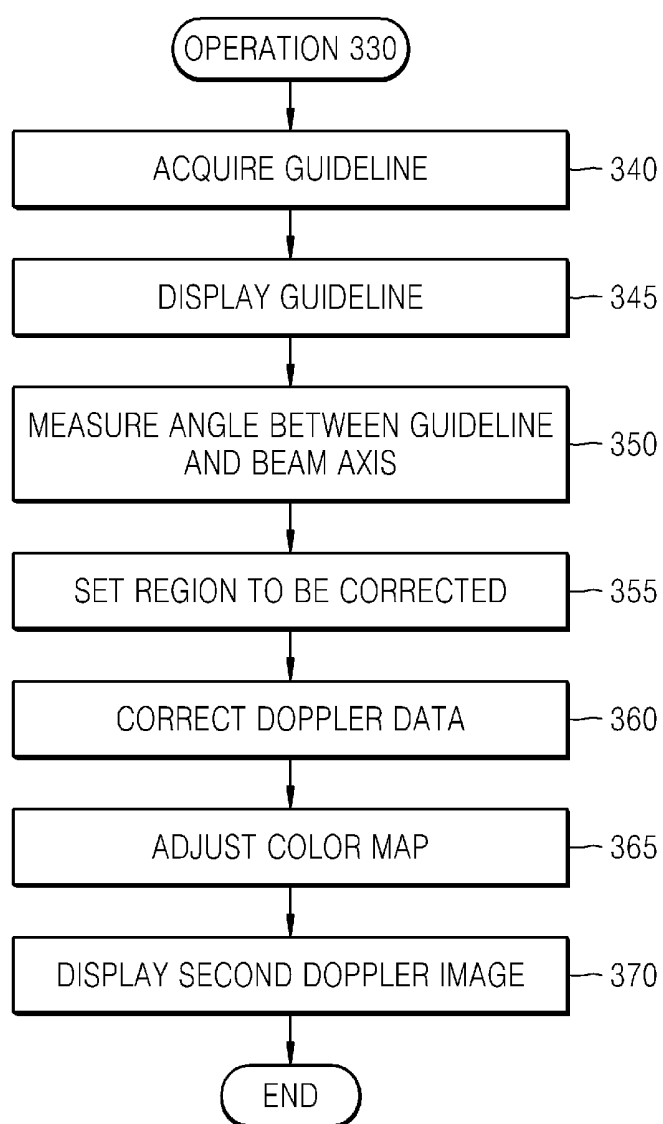


FIG. 5

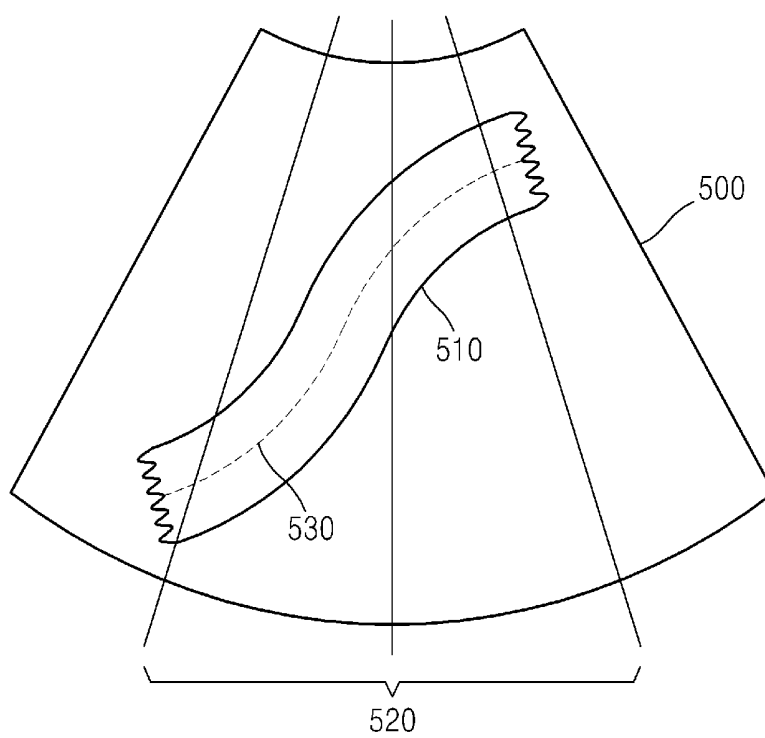


FIG. 6A

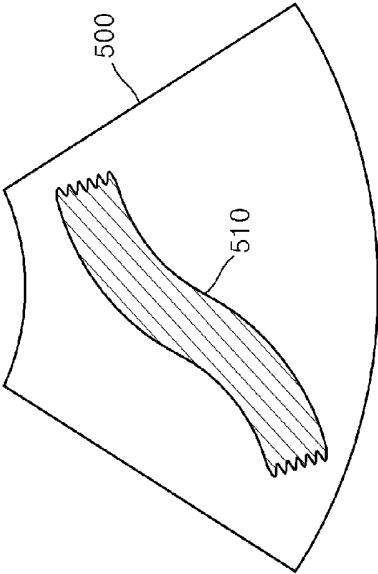


FIG. 6B

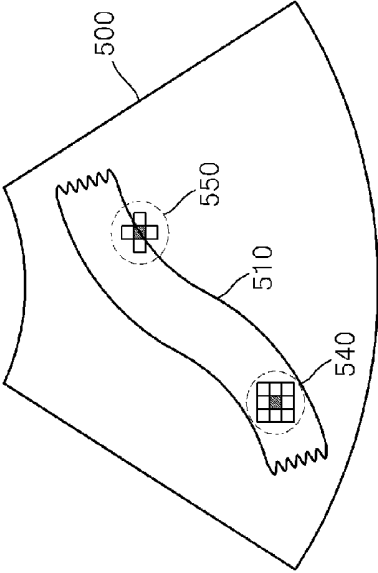


FIG. 6C

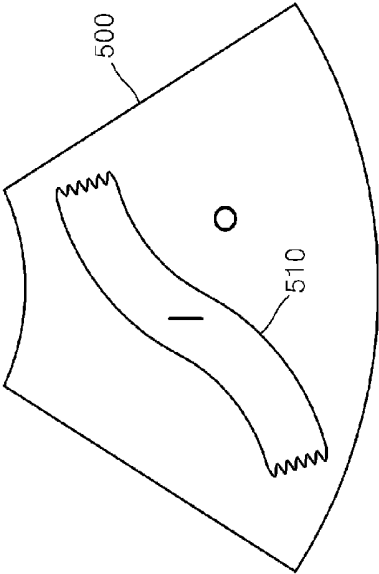


FIG. 6D

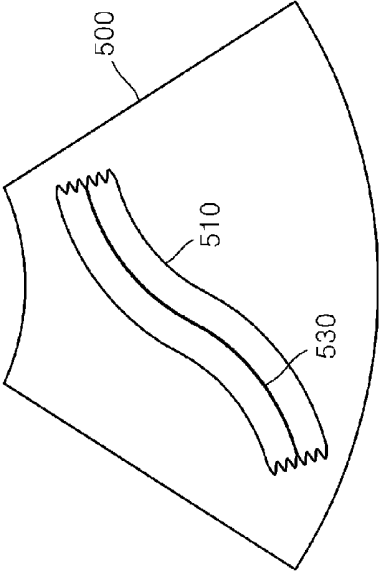


FIG. 7A

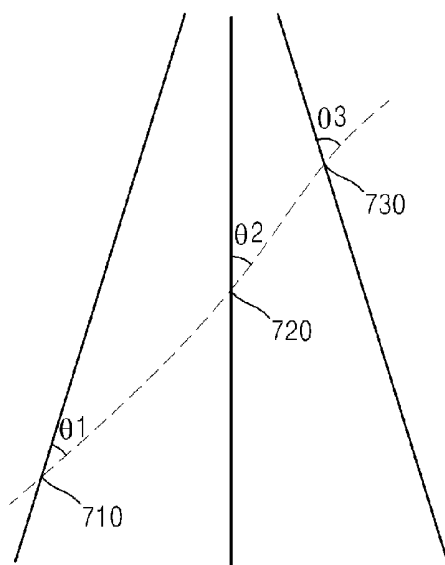


FIG. 7B

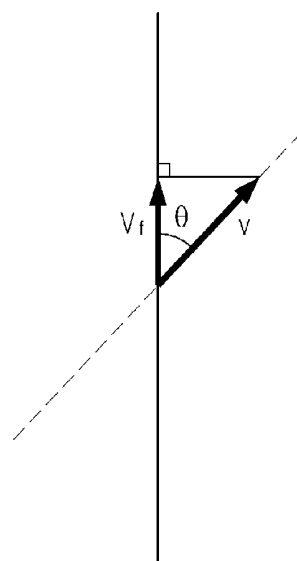


FIG. 8

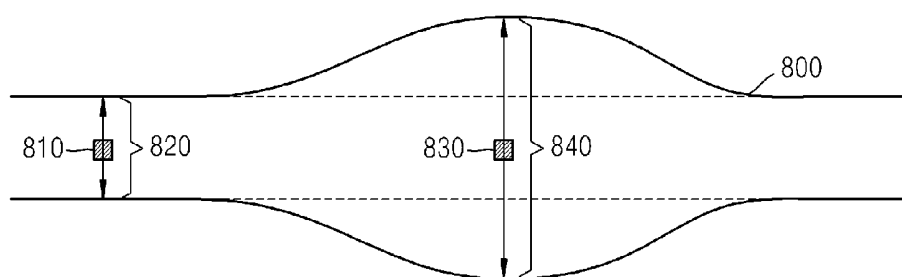


FIG. 9A

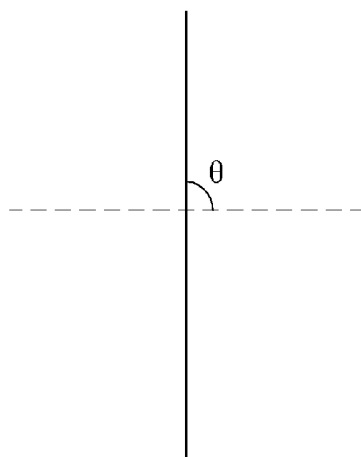


FIG. 9B

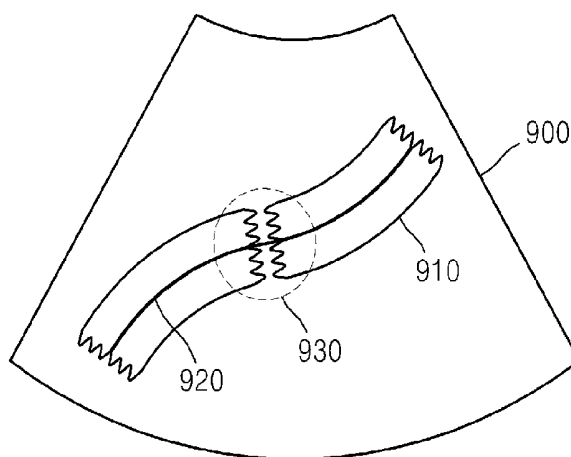


FIG. 10A

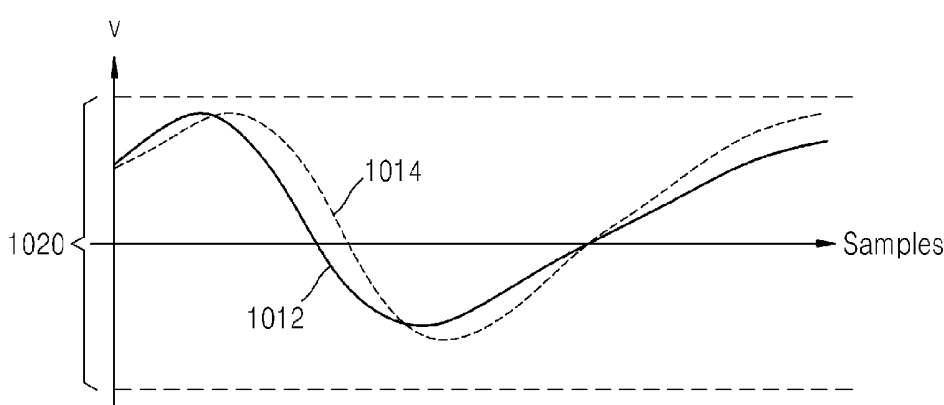


FIG. 10B

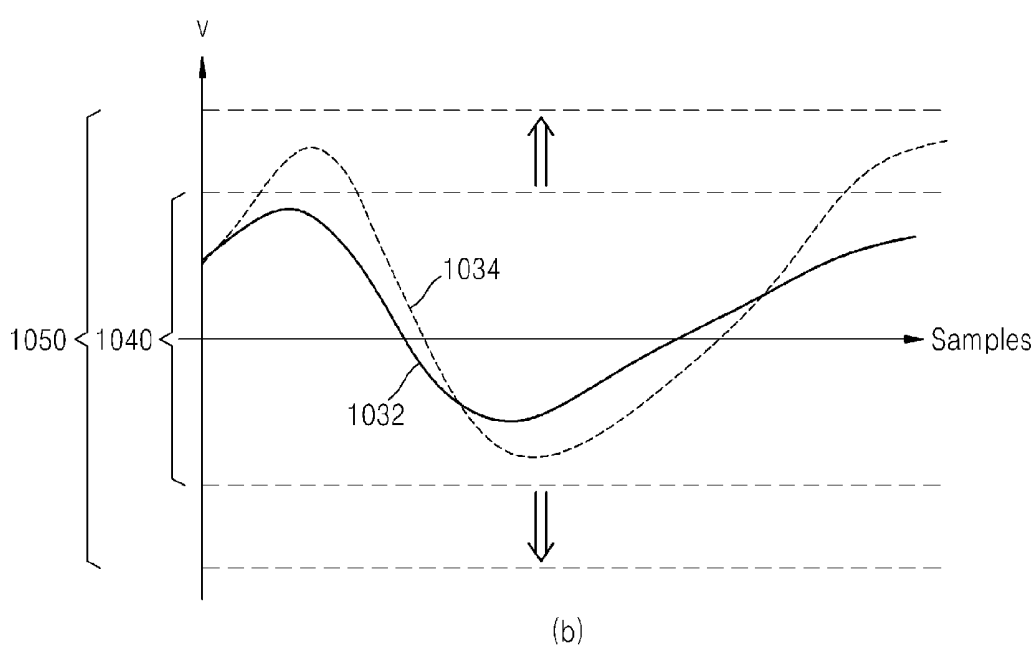


FIG. 11

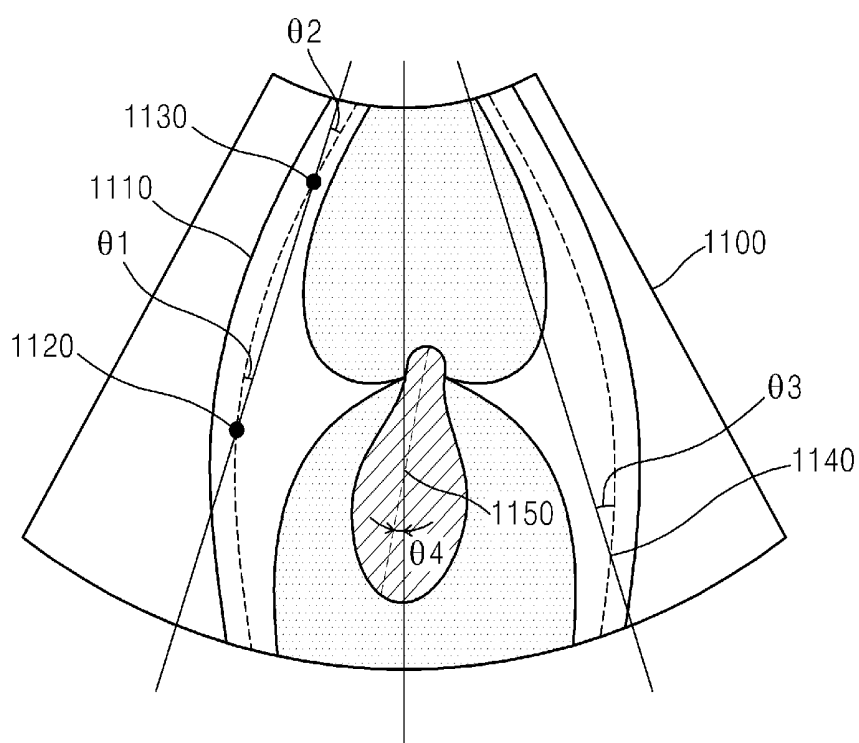
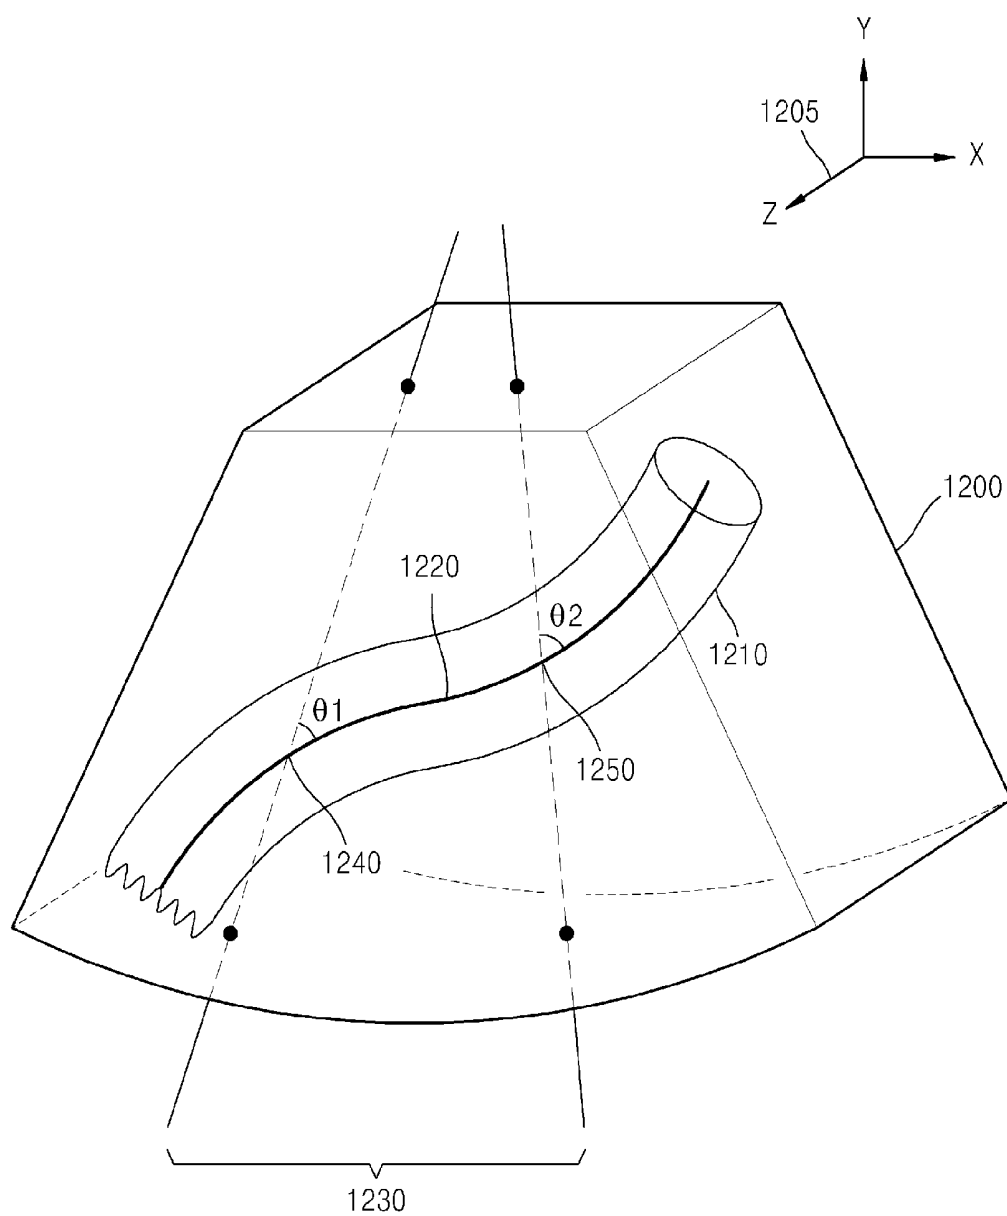


FIG. 12



METHOD AND APPARATUS FOR PROVIDING ULTRASOUND INFORMATION BY USING GUIDELINES

RELATED APPLICATIONS

[0001] This application claims the benefit of Korean Patent Application No. 10-2013-0110613, filed on Sep. 13, 2013, in the Korean Intellectual Property Office, the disclosure of which is incorporated herein in its entirety by reference.

BACKGROUND

[0002] 1. Field

[0003] One or more embodiments of the present invention relate to a method and apparatus for providing information about a diagnosis of an object on a screen by using an ultrasound information providing apparatus, and more particularly, to a method and apparatus for accurately and efficiently displaying a motion of an object by using a guideline of a Doppler image.

[0004] 2. Description of the Related Art

[0005] Ultrasound diagnostic apparatuses transmit an ultrasound signal (generally having a frequency of 20 kHz or more) to an internal part of an object by using a probe, and obtain an image of the internal part of the object by using information of an echo signal reflected from the object. In particular, the ultrasound diagnostic apparatuses are used for medical purposes such as inspecting the inner area of an object, detecting a foreign material in a body, and assessing an injury. The ultrasound diagnostic apparatuses have a higher stability than diagnostic apparatuses using X-rays, display an image in real time, and are safe because there is no exposure to radioactivity, and thus, may be widely used along with other image diagnostic apparatuses.

[0006] An image (hereinafter referred to as an ultrasound image) obtained from an ultrasound diagnostic apparatus may be displayed by the ultrasound diagnostic apparatus, or may be stored in a storage medium and displayed by another image display device. For example, a size of an ultrasound image may be reduced by a portable terminal, a portable electronic device, a personal digital assistant (PDA), a tablet personal computer (PC), or the like, and the ultrasound image may be displayed on a screen.

[0007] Doppler imaging enables a user to know that an object becomes closer to or farther away from a probe which transmits and receives an ultrasound signal, and thus is mainly used to detect a motion of the object.

SUMMARY

[0008] One or more embodiments of the present invention include a method and apparatus for providing ultrasound information about a motion of an object by using guidelines.

[0009] One or more embodiments of the present invention include a non-transitory computer-readable storage medium storing a program for executing the method in a computer.

[0010] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0011] According to one or more embodiments of the present invention, an ultrasound information providing method includes: generating a first Doppler image from Doppler data of an object; acquiring a guideline indicating a moving path of the object in the first Doppler image; correct-

ing the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and displaying a second Doppler image generated from the corrected Doppler data.

[0012] The acquiring may include acquiring the guideline on a basis of a user input, which draws a line on the first Doppler image, or a guideline detecting algorithm.

[0013] The ultrasound information providing method may further include displaying the guideline.

[0014] The displaying of the guideline may include displaying the guideline on at least one of the first and second Doppler images.

[0015] The correcting may include correcting the Doppler data to data previous to projection onto the beam axis by using the angle.

[0016] The angle may include an acute angle between the guideline and the beam axis.

[0017] The ultrasound information providing method may further include setting a region of which the Doppler data is to be corrected.

[0018] The region may include a thickness of the object.

[0019] The setting may include setting the region on a basis of a user input or a blood vessel region detecting algorithm.

[0020] The correcting may include, when the angle is within a predetermined range, correcting the Doppler data by using spatially near Doppler data.

[0021] The ultrasound information providing method may further include, when the corrected Doppler data is not within a range of a color map matched with the Doppler data previous to the correction, scaling up the color map.

[0022] The Doppler data may include two-dimensional (2D) Doppler data or three-dimensional (3D) Doppler data.

[0023] The Doppler data may include at least one of color Doppler data indicating blood flow and tissue Doppler data indicating a motion of a tissue.

[0024] According to one or more embodiments of the present invention, an ultrasound information providing method includes: acquiring a guideline indicating a moving path of an object from Doppler data of the object; correcting the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and displaying a Doppler image generated from the corrected Doppler data.

[0025] According to one or more embodiments of the present invention, an ultrasound information providing apparatus includes: a data acquirer that acquires Doppler data of an object; an image processor that generates a first Doppler image from the Doppler data of the object, and acquires a guideline indicating a moving path of the object in the first Doppler image; a data processor that corrects the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and a display unit that displays a second Doppler image generated from the corrected Doppler data.

[0026] According to one or more embodiments of the present invention, an ultrasound information providing apparatus includes: a data acquirer that acquires Doppler data of an object; an image processor that acquires a guideline indicating a moving path of the object from the Doppler data; a data processor that corrects the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and a display unit that displays a Doppler image which is generated by the image processor by using the corrected Doppler data.

[0027] According to one or more embodiments of the present invention, provided is a non-transitory computer-readable storage medium storing a computer program for executing the ultrasound information providing method.

BRIEF DESCRIPTION OF THE DRAWINGS

[0028] These and/or other aspects will become apparent and more readily appreciated from the following description of the embodiments, taken in conjunction with the accompanying drawings in which:

[0029] FIG. 1 is a diagram for describing a Doppler angle and a Doppler frequency according to an embodiment of the present invention;

[0030] FIG. 2 is a block diagram of an ultrasound information providing apparatus according to an embodiment of the present invention;

[0031] FIG. 3 is a flowchart of an ultrasound information providing method according to an embodiment of the present invention;

[0032] FIG. 4 is a flowchart of an ultrasound information providing method according to another embodiment of the present invention;

[0033] FIG. 5 is a diagram for describing a guideline according to an embodiment of the present invention;

[0034] FIGS. 6A-6D are diagrams for describing an operation of automatically detecting a guideline, according to an embodiment of the present invention;

[0035] FIGS. 7A-7B are diagrams for describing an operation of correcting Doppler data by using an angle between a guideline and a beam axis, according to an embodiment of the present invention;

[0036] FIG. 8 is a diagram for describing an operation of setting a region of which Doppler data is to be corrected, according to an embodiment of the present invention;

[0037] FIGS. 9A-9B are diagrams for describing an operation of correcting Doppler data by using nearby Doppler data, according to an embodiment of the present invention;

[0038] FIGS. 10A-10B are graphs for describing an operation of scaling up a color map matched with Doppler data, according to an embodiment of the present invention;

[0039] FIG. 11 is a diagram for describing an operation of correcting color Doppler data and tissue Doppler data, according to an embodiment of the present invention; and

[0040] FIG. 12 is a diagram for describing an operation of correcting three-dimensional (3D) Doppler data, according to an embodiment of the present invention.

DETAILED DESCRIPTION

[0041] Reference will now be made in detail to embodiments, examples of which are illustrated in the accompanying drawings, wherein like reference numerals refer to like elements throughout. In this regard, the present embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein. Accordingly, the embodiments are merely described below, by referring to the figures, to explain aspects of the present description. Expressions such as “at least one of,” when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0042] The terms used in the present invention have been selected as general terms widely used at present, in consideration of the functions of the present invention, but may be altered according to the intent of an operator skilled in the art, conventional practice, or introduction of new technology. Also, if a term is arbitrarily selected by the applicant in a specific case, a meaning of the term in this specific case will be described in detail in a corresponding description portion of the present invention. Therefore, the terms should be

defined on the basis of the entire content of this specification instead of a simple name of each of the terms.

[0043] In the disclosure below, when it is described that one device comprises (or includes or has) some elements, it should be understood that the device may comprise (or include or has) only those elements, or it may comprise (or include or have) other elements as well as those elements if there is no specific limitation. Moreover, each term such as “... unit”, “... apparatus” and “module” described in specification denotes an element for performing at least one function or operation, and may be implemented via hardware, software, or a combination of hardware and software.

[0044] The term “ultrasound image” used herein denotes an image of an object acquired by using an ultrasound wave. Also, the term “object” used herein may include a person, an animal, a part of the person, or a part of the animal. For example, an object may include an organ such as a liver, a heart, a womb, a brain, breasts, an abdomen, or the like, or a blood vessel. Also, the term “object” may include a phantom. The phantom denotes a material having a volume that is very close to a density and effective atomic number of an organism, and may include a spherical phantom having a characteristic similar to a physical body.

[0045] Moreover, the term “user” used herein is a medical expert, and may be a doctor, a nurse, a medical technologist, a medical image expert, or the like, or may be an engineer who repairs a medical apparatus. However, the user is not limited thereto.

[0046] Hereinafter, embodiments of the present invention will be described in detail with reference to the accompanying drawings.

[0047] FIG. 1 is a diagram for describing a Doppler angle and a Doppler frequency according to an embodiment of the present invention.

[0048] A probe 10 of FIG. 1 transmits an ultrasound signal to an object 25 which moves through a blood vessel 20, and receives an ultrasound signal (an echo signal) reflected from the object 25. The probe 10 transmits the ultrasound signal having a frequency “ f_0 ” to the object 25 which moves at a speed “ v ” in the blood vessel 20. The ultrasound signal transmitted by the probe 10 may focus on the object 25, and the focused ultrasound signal may be expressed as one axis. Hereinafter, a central axis of the ultrasound signal transmitted by the probe 10 is referred to as a beam axis 28.

[0049] The object 25 scatters the ultrasound signal transmitted by the probe 10 to generate an echo signal that has a frequency “ $f_0 + f_d$ ”. Hereinafter, a Doppler frequency denotes a difference frequency “ f_d ” between a frequency of the ultrasound signal transmitted by the probe 10 and a frequency of the echo signal received by the probe 10. That is, the Doppler frequency “ f_d ” may denote a frequency which is Doppler-shifted by the object 25.

[0050] A Doppler angle denotes an angle “ e ” between the beam axis 28 and a moving direction (for example, a central axis of the blood vessel 20) of the object 25. In this case, the Doppler frequency “ f_d ” may be expressed as the following Equation (1):

$$f_d = (2 * f_0 * v * \cos \theta) / c \quad (1)$$

where f_0 denotes a frequency of the transmitted ultrasound signal, v denotes a moving speed of the object 25, c denotes a speed of sound, and e denotes the Doppler angle. That is, the

Doppler frequency is relevant to the moving speed and Doppler angle of the object **25** as well as a transmission ultrasound frequency.

[0051] The Doppler frequency " f_d " is expressed as a component which is obtained by projecting the moving speed of the object **25** onto the beam axis **28**. Therefore, a Doppler image obtained by imaging Doppler data may be differently expressed according to the Doppler angle " θ " even when measuring the same object **25**.

[0052] As the Doppler angle becomes closer to 0, namely, as the moving direction of the object **25** becomes closer to a direction toward the probe **10**, the Doppler frequency " f_d " expresses the moving speed of the object **25** well. In other words, there are a few errors between a Doppler imaging result using the Doppler data and an actual moving speed of the object **25**. On the other hand, as the Doppler angle becomes closer to 90 degrees, $\cos \theta$ becomes closer to 0, and thus, there are many errors between the Doppler frequency " f_d " and an actual speed " v ". That is, the actual moving speed of the object **25** is not reflected well in the Doppler data.

[0053] FIG. 2 is a block diagram of an ultrasound information providing apparatus **100** according to an embodiment of the present invention. Referring to FIG. 2, the ultrasound information providing apparatus **100** according to an embodiment may include a data acquirer **110**, an image processor **120**, a data processor **130**, a storage **140**, a user interface **150**, and a controller **160**. The elements included in the ultrasound information providing apparatus **100** are not limited thereto, and the ultrasound information providing apparatus **100** may further include other general-use elements.

[0054] The ultrasound information providing apparatus **100** provides an ultrasound image, obtained by scanning an object, to a user. The ultrasound image may include a 3D image as well as a two-dimensional (2D) image indicating a cross-sectional surface of the object, and include a Doppler image that expresses a motion of an object in colors by using Doppler data, in addition to a grayscale ultrasound image that is generated by scanning the object according to an amplitude (A) mode, a brightness (B) mode, and a motion (M) mode.

[0055] The ultrasound information providing apparatus **100** may display various kinds of Doppler images to provide ultrasound information to a user. The Doppler image according to an embodiment may include a color Doppler image (also called a blood Doppler image) indicating blood flow, a tissue Doppler image indicating a motion of tissue, and a spectral Doppler image that expresses a moving speed of an object as a waveform.

[0056] Although specifically described below, the ultrasound information providing apparatus **100** may provide ultrasound diagnostic information that is generated by directly scanning an object, but may receive ultrasound diagnostic information from an external device or server connected thereto over a network to provide the ultrasound diagnostic information. In the former, the ultrasound information providing apparatus **100** may be implemented as a fixed/mobile ultrasound diagnostic apparatus. In the latter, however, the ultrasound information providing apparatus **100** may be implemented in various types that include a screen for providing ultrasound information.

[0057] For example, the ultrasound information providing apparatus **100** may be implemented in various types, which include a screen for providing ultrasound information, such as work stations, picture archiving and communication system (PACS) viewers, portable phones, smartphones, smart

televisions (TVs), Internet protocol (IP) TVs, digital TVs, personal computers (PCs), notebook computers, laptop computers, tablet PCs, e-book terminals, personal digital assistants (PDAs), portable multimedia players (PMPs), navigation terminals, consumer electronic (CE) devices, etc.

[0058] The data acquirer **110** acquires ultrasound diagnostic information of an object. The ultrasound diagnostic information according to an embodiment may include the above-described Doppler data. The data acquirer **110** may scan the object and process an echo signal by using a probe, thereby acquiring ultrasound diagnostic information. Also, the data acquirer **110** may acquire ultrasound diagnostic information from an external device or server over a network which is connected thereto in a wired manner or a wireless manner.

[0059] When the data acquirer **110** scans an object to acquire ultrasound diagnostic information, one or more probes may be used. That is, the data acquirer **110** may acquire ultrasound diagnostic information by using various kinds of probes such as a linear array probe, a convex array probe, a phased array probe, a matrix array probe.

[0060] On the other hand, when the data acquirer **110** acquires ultrasound diagnostic information over a network, various types of communication units may be used. For example, the data acquirer **110** may be connected to the network through a wired connection, such as a USB cable, a data cable, or an optical fiber cable, or a wireless connection such as Bluetooth, Wi-Fi, near field communication (NFC), or a 2G/3G/4G network. The data acquirer **110** may acquire ultrasound diagnostic information from an external device, a hospital server, or a cloud server. The data acquirer **110** may acquire data from the other internal device or server of the hospital server connected to a PACS. The ultrasound diagnostic or Doppler data acquired by the data acquirer **110** may be stored in the below-described storage **140**.

[0061] The Doppler data acquired by the data acquirer **110** may include information about a moving direction and speed of the object. The Doppler data, as described above, may include color Doppler data or tissue Doppler data depending on a kind of the object, and include two kinds of Doppler data.

[0062] The Doppler data may include three-dimensional space Doppler (3D Doppler) data in addition to two-dimensional space Doppler (2D Doppler) data depending on a type of an echo signal. Also, the Doppler data may include Doppler data of a continuous image such as a moving image, in addition to Doppler data of a still image.

[0063] The image processor **120** processes the ultrasound diagnostic information acquired by the data acquirer **110** to generate an ultrasound image. The image processor **120**, as described above, may generate various kinds of ultrasound images such as a grayscale ultrasound image and a Doppler image indicating a motion of an object. The image processor **120** may perform 2D rendering or 3D rendering for providing information on a screen.

[0064] The image processor **120** according to an embodiment may match a color map with the Doppler data included in the ultrasound diagnostic information to generate a Doppler image. That is, the image processor **120** may match a color with a component of a moving speed of the object that is included in the Doppler data, and visually provide information of a moving object to a user.

[0065] The image processor **120** may acquire a guideline in addition to the above-described ultrasound image, and perform imaging on the guideline. The guideline may denote a moving route of the object which is displayed on the ultra-

sound image, and the image processor **120** may generate the guideline to be displayed by using a graphical user interface (GUI).

[0066] The image processor **120** according to an embodiment may acquire the guideline on the basis of a user input. That is, the image processor **120** may generate the guideline on the basis of a user input that draws a line, such as a straight line, a curve, or the like, on the ultrasound image or the Doppler image. Alternatively, the image processor **120** may generate the guideline on the basis of a pre-stored guideline detecting algorithm. An embodiment, in which the image processor **120** acquires and generates the guideline, will be described in detail with reference to FIGS. **5** and **6**.

[0067] The image processor **120** may acquire the guideline by using at least one of the Doppler image and the Doppler data. That is, the image processor **120** may acquire the guideline on the basis of a user input for the Doppler image, and may acquire the guideline by applying the guideline detecting algorithm to the Doppler data. Also, the image processor **120** may acquire the guideline by using the Doppler image and the Doppler data.

[0068] The image processor **120** may generate a 3D guideline of a 3D image in addition to a guideline of a 2D image. The 3D guideline may denote a straight line or a curve which is displayed on a 3D space.

[0069] In addition to the above-described details, the image processor **120** may perform imaging on a variety of information displayed on a screen of the ultrasound information providing apparatus **100**. For example, the image processor **120** may generate elements and a variety of information about an ultrasound diagnosis of the object by using a user interface (UI) or a GUI.

[0070] The data processor **130** processes the ultrasound diagnostic information received from the data acquirer **110**. The data processor **130** may correct the Doppler data included in the ultrasound diagnostic information. Although specifically described below with reference to FIG. **7**, the data processor **130** may correct the Doppler data by using the above-described guideline, and correct the Doppler data on the basis of an angle between the guideline and a beam axis of the probe. The data processor **130** may correct the Doppler data to data previous to projection onto the beam axis of the probe.

[0071] The ultrasound diagnostic information (i.e., the corrected Doppler data) obtained through processing by the data processor **130** may be stored in the below-described storage **140**, and the image processor **120** may generate an ultrasound image by using the processed ultrasound diagnostic information.

[0072] The data processor **130** may set a detailed region, of which ultrasound diagnostic information is to be processed, before processing the ultrasound diagnostic information as described above. For example, the data processor **130** may set a region (i.e., a region of interest (ROI)) of which Doppler data is to be corrected, on the basis of a user input, a blood vessel region detecting algorithm, or a tissue region detecting algorithm. Subsequently, the data processor **130** may correct the Doppler data of the set region in a whole region. The region to be corrected may be a partial or whole region of an object, and for example, when the object is a blood vessel, the region to be corrected may be a thickness of the blood vessel.

[0073] The data processor **130** may use Doppler data at a spatially near position in an operation of correcting specific Doppler data. As described above with reference to FIG. **1**,

when a Doppler angle is within a certain range, many errors occur in a Doppler imaging result, and thus, the data processor **130** may correct the Doppler data by using information of an ambient space. A detailed embodiment will be described below with reference to FIG. **9**.

[0074] Moreover, the data processor **130** may scale up or down a color map in correcting Doppler data. That is, when the corrected Doppler data is not within a range of the color map matched with Doppler data previous to the correction, the data processor **130** may adjust the color map so as to prevent aliasing from occurring. A detailed embodiment will be described below with reference to FIG. **10**.

[0075] The storage **140** stores a variety of information obtained through processing by the ultrasound information providing apparatus **100**. For example, the storage **140** may store medical data, such as input/output ultrasound data, ultrasound diagnostic information, and ultrasound images, associated with a diagnosis of an object, and may also store an algorithm or a program which is executed in the ultrasound information providing apparatus **100**.

[0076] The storage **140** may include at least one type of storage medium of a flash memory, a hard disk, a multimedia micro card, a card type memory (a secure digital (SD) card, an extreme digital (XD) card, or the like), random access memory (RAM), static random access memory (SRAM), read-only memory (ROM), electrically erasable programmable read-only memory (EEPROM), and programmable read-only memory (PROM). Also, the ultrasound information providing apparatus **100** may use a web storage or a cloud server which performs a storage function of the storage **140** on the Web.

[0077] The user interface **150** provides ultrasound diagnostic information to a user, and receives various kinds of inputs for controlling the ultrasound information providing apparatus **100** from the user. The user interface **150**, as illustrated in FIG. **2**, may include a user input unit **152** and a display unit **154**.

[0078] The user input unit **152** receives an external input signal for controlling the ultrasound information providing apparatus **100** from the user. That is, the user input unit **152** may receive a user input through various input units such as a keypad, a mouse, a touch panel, a touch screen, a trackball, a jog wheel, a jog switch, etc., and moreover receive a remote input through a remote control unit. For example, the user input unit **152** may receive a user input, which draws a guideline, and a user input that sets a region of which Doppler data is to be corrected.

[0079] A touch panel may detect a proximity touch in which a pointer, which is separated from a screen by a certain distance, approaches a position on the screen, in addition to a real touch in which the pointer actually touches a screen. The pointer used herein denotes a touch instrument for really touching or proximity-touching a specific portion of the touch panel. Examples of the pointer include a stylus pen or a body part, such as a finger or the like, of a human body.

[0080] Moreover, the touch panel may be implemented as a touch screen which forms a layer structure including the display unit **154**. The touch screen may be implemented in various types such as a contact capacitive type, a press resistive type, an infrared sensing type, a surface ultrasonic conductive type, an integration tension measurement type, and a piezo effect type.

[0081] Although not shown, the touch panel may include various sensors which are provided inside or near a touch

screen, for detecting a touch input. An example of a sensor for sensing a touch of the touch panel is a tactile sensor. The tactile sensor denotes a sensor that senses a touch by a specific object by a degree, at which a user feels, or more. The tactile sensor may sense various pieces of information such as a roughness of a touched surface, a stiffness of a touched object, a temperature of a touched point, etc.

[0082] Moreover, an example of a sensor for sensing a touch of the touch panel is a proximity sensor. The proximity sensor denotes a sensor that detects an object approaching a detection surface or an object near the detection surface by using an electromagnetic force or infrared light without mechanical contact. Examples of the proximity sensor include a transmissive photosensor, a directly reflective photosensor, a mirror reflective photosensor, a high frequency oscillation-type proximity sensor, a capacitive proximity sensor, a magnetic proximity sensor, and an infrared proximity sensor.

[0083] The display unit 154 may display a GUI associated with a function setting of the ultrasound information providing apparatus 100, or display ultrasound diagnostic information and an ultrasound image, thereby providing visual information to a user. For example, the display unit 154 may display a variety of information, such as a 2D or 3D ultrasound image, a Doppler image, and a guideline, on a screen.

[0084] The display unit 154 may include at least one of a liquid crystal display (LCD), a thin film transistor-liquid crystal display, an organic light-emitting diode (OLED) display, a flexible display, and a 3D display. Also, the ultrasound information providing apparatus 100 may include two or more display units 154 depending on an implementation type of the ultrasound information providing apparatus 100.

[0085] As described above, the display unit 154 may be configured with the touch screen which forms the layer structure including the user input 152. That is, the display unit 154 may be used as an output unit and an input unit, in which case the display unit 154 may receive a touch input by using a stylus pen or a body part of a human body.

[0086] The controller 160 controls an overall operation of the ultrasound information providing apparatus 100. That is, the controller 160 may control operations between the data acquirer 110, the image processor 120, the data processor 130, the storage 140, and the user interface 150 of FIG. 2.

[0087] For example, the controller 160 may control the image processor 120 so as to generate a Doppler image from Doppler data acquired by the data acquirer 110. Alternatively, the controller 160 may control the storage 140 so as to store Doppler data obtained through correction by the data processor 130, or control the data processor 130 so as to correct the Doppler data on the basis of a user input received by the user interface 150.

[0088] Hereinafter, a method in which the elements included in the ultrasound information providing apparatus 100 provide ultrasound information by using guidelines will be described in detail with reference to FIGS. 3 and 4.

[0089] A flowchart of each of FIGS. 3 and 4 includes a plurality of operations that are performed in time series by the data acquirer 110, the image processor 120, the data processor 130, the storage 140, the user interface 150, and the controller 160 of the ultrasound information providing apparatus 100 illustrated in FIG. 2. Thus, although not described below, the above-described details of the elements of FIG. 2 may be applied to the methods of FIGS. 3 and 4.

[0090] FIG. 3 is a flowchart of an ultrasound information providing method according to an embodiment of the present invention.

[0091] In operation 310, the ultrasound information providing apparatus 100 acquires Doppler data. The ultrasound information providing apparatus 100 may scan an object with a probe to directly acquire the Doppler data, or receive the Doppler data through communication with an external device or server over a network.

[0092] As described above, the Doppler data may include 2D or 3D Doppler data, and include at least one of color Doppler data and tissue Doppler data.

[0093] In operation 320, the ultrasound information providing apparatus 100 generates a first Doppler image by using the Doppler data which is received in operation 310. The ultrasound information providing apparatus 100 may map a color map to a component of a moving speed of the object that is included in the Doppler data, thereby expressing a motion of the object in colors. In spectral Doppler data, the ultrasound information providing apparatus 100 may express a motion of the object as a waveform.

[0094] Subsequently, in operation 330, the ultrasound information providing apparatus 100 displays the first Doppler image which is generated in operation 320.

[0095] In operation 340, the ultrasound information providing apparatus 100 acquires a guideline. As described above with reference to FIG. 2, the guideline may denote a moving route of the object in the Doppler image. The guideline according to an embodiment may be disposed in a region which is displayed in colors according to the Doppler data in the Doppler image.

[0096] The ultrasound information providing apparatus 100 may sense a user input for the first Doppler image which is displayed in operation 330, and acquire the guideline on the basis of the user input. For example, when the user draws a line on the first Doppler image through a touch screen or a touch panel, the ultrasound information providing apparatus 100 may generate the guideline according to the user input.

[0097] Alternatively, the ultrasound information providing apparatus 100 may apply the guideline detecting algorithm to the first Doppler image to automatically generate the guideline. This will be described in detail with reference to FIG. 6.

[0098] In operation 350, the ultrasound information providing apparatus 100 measures angles between the guideline and beam axes. The ultrasound information providing apparatus 100 measures the angles between the guideline (which is acquired in operation 340) and the beam axes with respect to one position of the first Doppler image. According to an embodiment, the ultrasound information providing apparatus 100 may select and measure an acute angle from the angles between the guideline and the beam axes.

[0099] In operation 360, the ultrasound information providing apparatus 100 corrects the Doppler data. The ultrasound information providing apparatus 100 may correct Doppler data at the position, where the angles are measured in operation 350, to data previous to projection according to Equation (1), which has been described above with reference to FIG. 1. Therefore, the ultrasound information providing apparatus 100 may correct the Doppler data to data close to an actual moving speed of the object, and provide information about a diagnosis of the object, thereby reducing an error.

[0100] In operation 370, the ultrasound information providing apparatus 100 displays a second Doppler image on the basis of the Doppler data which is obtained through the cor-

rection in operation 360. In other words, the ultrasound information providing apparatus 100 may newly generate the second Doppler image by using the corrected Doppler data, and display the second Doppler image. That is, the ultrasound information providing apparatus 100 provides a diagnosis result, in which an influence of the Doppler angle on the Doppler data is minimized, to the user.

[0101] FIG. 4 is a flowchart of an ultrasound information providing method according to another embodiment of the present invention. In FIG. 4, an operation subsequent to operations 310 to 330 described above with reference to FIG. 3 will now be described.

[0102] In operation 340, the ultrasound information providing apparatus 100 acquires the guideline. As described above with reference to FIG. 3, the ultrasound information providing apparatus 100 may acquire the guide line on the basis of the user input or the guideline detecting algorithm.

[0103] In operation 345, the ultrasound information providing apparatus 100 may display the acquired guideline on a screen. In FIG. 3, the acquired guideline is merely used for measuring the angles between the guideline and the beam axes, and is not displayed on the screen. On the other hand, the ultrasound information providing apparatus 100 may display the guideline on the first Doppler image. Therefore, the user of the ultrasound information providing apparatus 100 visually checks the guideline, and easily understands a moving route of the object.

[0104] In operation 350, the ultrasound information providing apparatus 100 measures the angles between the guideline and the beam axes. A detailed description on this is as described above with reference to FIG. 3.

[0105] In operation 355, the ultrasound information providing apparatus 100 sets a region, of which Doppler data is to be corrected, in the displayed first Doppler image. The ultrasound information providing apparatus 100, as described above with reference to FIG. 2, may set a region of which ultrasound diagnostic information is to be processed, and set the region of which the Doppler data is to be corrected, on the basis of a user input or a blood vessel region detecting algorithm. The region to be corrected may be a partial or whole region of the object, and will be described below with reference to FIG. 8.

[0106] In operation 360, the ultrasound information providing apparatus 100 corrects the Doppler data. In addition to the details which have been described in operation 360 of FIG. 3, the ultrasound information providing apparatus 100 may correct the Doppler data of the region which is set in operation 355.

[0107] In operation 365, the ultrasound information providing apparatus 100 may adjust a color map matched with the Doppler data and the Doppler image. As described above with reference to FIG. 2, when the corrected Doppler data is not within a range of the color map matched with the Doppler data previous to the correction, the ultrasound information providing apparatus 100 may scale up the color map so as to prevent aliasing from occurring.

[0108] In operation 370, the ultrasound information providing apparatus 100 displays the second Doppler image by using the adjusted Doppler data.

[0109] FIG. 5 is a diagram for describing a guideline according to an embodiment of the present invention.

[0110] A Doppler image 500 of FIG. 5 is a Doppler image of a blood vessel 510, and the ultrasound information providing apparatus 100 displays the Doppler image 500, generated

based on the Doppler data, on a screen. Three solid lines across the Doppler image 500 respectively indicate beam axes 520 of a probe that transmits an ultrasound signal to the blood vessel 510. The beam axes 520 of FIG. 5 may have a fan shape along a scan line, or unlike the illustrated details, the beam axes 520 may be disposed in parallel with each other in a rectangular ultrasound image.

[0111] The ultrasound information providing apparatus 100 acquires a guideline 530 indicating a moving path of blood flow in the blood vessel 510. As described above, the ultrasound information providing apparatus 100 may acquire and generate the guideline 530 according to a received user input.

[0112] For example, when a user draws a line along a central line of the blood vessel 510 via a touch input by using a body part of the user, a mouse, or a trackball, the ultrasound information providing apparatus 100 may generate the guideline 530 according to a sensed position of the user input.

[0113] The ultrasound information providing apparatus 100 may display the acquired guideline 530 on the Doppler image 500. In FIG. 5, the guideline 530 is illustrated as a dashed line. However, present embodiment is not limited thereto, and the ultrasound information providing apparatus 100 may display the guideline 530 as various line types such as a dotted line, a dashed line, a solid line, or a double line.

[0114] On the other hand, the ultrasound information providing apparatus 100 may internally use the acquired guideline 530 in a system without displaying the acquired guideline 530 on the Doppler image 500. The ultrasound information providing apparatus 100, as described above, corrects the Doppler data by using angles between the guideline 530 and the beam axes 520. That is, the ultrasound information providing apparatus 100 may internally use the guideline 530 in the system so as to measure an angle, without displaying the guideline 530 on a screen.

[0115] FIG. 6 are diagrams for describing an operation of automatically detecting a guideline, according to an embodiment of the present invention. The ultrasound information providing apparatus 100, as described above with reference to FIG. 5, may acquire a guideline on the basis of a user input, but may acquire the guideline through a guideline detecting algorithm. Hereinafter, the guideline detecting algorithm will be described with reference to FIGS. 6A to 6D.

[0116] In FIG. 6A, a region 510, which is darkly displayed on a Doppler image, is a region including Doppler data which indicates a motion of an object. In FIGS. 6B to 6D, an operation of classifying the region 510 from the Doppler image 500 will be described.

[0117] In FIG. 6B, the ultrasound information providing apparatus 100 analyzes the Doppler data on the basis of a connected component analysis (CCA) algorithm. That is, the ultrasound information providing apparatus 100 detects the region 510 from the Doppler image 500 according to a plurality of spatially near pixels including Doppler data, in a pixel or a pixel group having a certain size.

[0118] As illustrated in FIG. 6B, the ultrasound information providing apparatus 100 applies an 8-CCA algorithm to a pixel group 540. That is, the ultrasound information providing apparatus 100 may analyze eight pixels disposed close to a top, bottom, left, and right of a pixel, which is darkly displayed at the center, and four-direction diagonal lines in the pixel group 540, and determine whether the pixel group 540 includes Doppler data. The ultrasound information providing apparatus 100 applies a 4-CCA algorithm to a pixel

group 550. That is, the ultrasound information providing apparatus 100 may analyze four pixels close to an up direction, down direction, left direction, and right direction of a pixel, which is darkly displayed at the center in the pixel group 550.

[0119] Therefore, the ultrasound information providing apparatus 100 may detect a boundary of a region including the Doppler data in the Doppler image 500. Subsequently, the ultrasound information providing apparatus 100 may separate the region including the Doppler data from a region including no Doppler data to detect the region 510.

[0120] In FIG. 6C, the ultrasound information providing apparatus 100 displays the analyzed result of the Doppler image 500 as a value of 1 and a value of 0. By using the result analyzed with a CCA algorithm in FIG. 6B, the ultrasound information providing apparatus 100 may store a value of 1 for the region 510 including the Doppler data, and store a value of 0 for the other regions. That is, the ultrasound information providing apparatus 100 may perform a masking operation on the Doppler image 500 to detect a region including information about a motion of an object.

[0121] In FIG. 6D, when a region including the Doppler data is detected, the ultrasound information providing apparatus 100 may acquire a guideline 530 through a skeletonization algorithm. The skeletonization algorithm may denote an algorithm that reduces a thickness of a figure so as to extract a shape of a line, having a thickness equal to or less than a certain thickness, from the figure.

[0122] The ultrasound information providing apparatus 100 may acquire the guideline 530 through a morphology operation algorithm, in addition to the skeletonization algorithm. That is, when the region 510 is detected, the ultrasound information providing apparatus 100 may detect the guideline 530 by repeatedly applying at least one of a dilation algorithm that enlarges the region 510 and an erosion algorithm that reduces the region 510.

[0123] The above-described details of the guideline detecting algorithm that detects the guideline 530 of the region 510 are merely related to an embodiment, but the present embodiment is not limited thereto. The ultrasound information providing apparatus 100 may detect the guideline 530 on the basis of various schemes. The ultrasound information providing apparatus 100 according to an embodiment may detect the longest path included in the region 510 including the Doppler data, and acquire the longest path as the guideline 530.

[0124] FIG. 7 are diagrams for describing an operation of correcting Doppler data by using an angle between a guideline and a beam axis, according to an embodiment of the present invention.

[0125] In FIG. 7A, three height-direction solid lines indicate beam axes of the probe, as described above with reference to FIG. 5, and a width-direction dashed line indicates a guideline. In FIG. 7A, the ultrasound information providing apparatus 100 measures angles between the guideline and the beam axes. The ultrasound information providing apparatus 100 may measure the angles (which are formed along the guideline) between the guideline and the beam axes in a region including Doppler data. The ultrasound information providing apparatus 100 may select an acute angle from among the angles between the guideline and the beam axes.

[0126] In FIG. 7A, an embodiment in which the angles between the guideline and the beam axes are respectively measured at positions 710, 720 and 730 is illustrated. The ultrasound information providing apparatus 100 may acquire

information about the beam axes from information of an ultrasound signal transmitted by the probe. Alternatively, the ultrasound information providing apparatus 100 may acquire beam-axis information about a Doppler image from beam-axis information about ultrasound data previous to scan conversion.

[0127] In FIG. 7B, when the angles between the beam axes and the guideline are measured, the ultrasound information providing apparatus 100 corrects Doppler data at a position, where an angle is measured, by using the measured angles. The ultrasound information providing apparatus 100 may correct Doppler data previous to projection of Doppler data onto the beam axes, by using the angles.

[0128] To provide a detailed description, as described above with reference to FIG. 1, when an actual moving speed of the object is “v” in FIG. 7B, the moving speed of the object that is included in the Doppler data is shown as “v_f” that is a component projected onto a corresponding beam axis according to a Doppler angle.

[0129] The following Equation (2) may be deduced from the above-described Equation (1). Each term of Equation (2) denotes the same term as that of Equation (1).

$$v = \frac{c * f_d}{2 * f_o * \cos \theta} \quad (2)$$

[0130] The ultrasound information providing apparatus 100 may acquire the actual moving speed “v” of the object by using the transmission frequency, the Doppler frequency, and the Doppler angle “θ”. Since the guideline is a line indicating a moving path of the object, the ultrasound information providing apparatus 100 may use the angles which are measured in FIG. 7A, instead of the Doppler angle of Equation (2). That is, the ultrasound information providing apparatus 100 may measure the moving speed “v” of the object by using the angles (which are measured in FIG. 7A) between the guideline and the beam axes.

[0131] The ultrasound information providing apparatus 100 may correct “v_f”, which is a component projected onto a corresponding beam axis, to “v” which is measured by using the angles between the guideline and the beam axes, in Doppler data. Subsequently, the ultrasound information providing apparatus 100 may generate and output a Doppler image by using the corrected Doppler data, thus accurately providing information about a motion of the object to a user.

[0132] The ultrasound information providing apparatus 100 may display a Doppler image based on the corrected Doppler data, and newly display the guideline on the Doppler image.

[0133] FIG. 8 is a diagram for describing an operation of setting a region of which Doppler data is to be corrected, according to an embodiment of the present invention. A solid line of FIG. 8 indicates a blood vessel 800.

[0134] The ultrasound information providing apparatus 100 may set a region, of which Doppler data is to be corrected, in a region including Doppler data. As described above in FIG. 2, the ultrasound information providing apparatus 100 may set a region to be corrected on the basis of a user input or a blood vessel region detecting algorithm. The region to be corrected may include a blood vessel or a thickness of tissue which is an object.

[0135] To describe FIG. 8 as an example, the ultrasound information providing apparatus 100 may determine a region

to be corrected as a thickness **820**, for a position **810**. That is, the ultrasound information providing apparatus **100** may select a total thickness of the blood vessel **800**, which is the region including the Doppler data, as the region to be corrected.

[0136] According to an embodiment, the ultrasound information providing apparatus **100** may determine a region to be corrected according to a user input that selects the thickness **820**. That is, the ultrasound information providing apparatus **100** may receive a user input that selects a boundary or thickness of the blood vessel **800**, and determine a region to be corrected according to the received user input.

[0137] According to another embodiment, the ultrasound information providing apparatus **100** may detect the thickness **820** of the blood vessel **800** on the basis of a blood vessel region detecting algorithm, and determine the detected thickness **820** as the region to be corrected. For example, the algorithm that detects the region **510** described above with reference to FIG. 6 may be used as the blood vessel region detecting algorithm.

[0138] Next, an embodiment in which the ultrasound information providing apparatus **100** corrects Doppler data according to a preset region will be described. First, the ultrasound information providing apparatus **100** corrects Doppler data at the position **810** by using an angle between a guideline and a beam axis for the position **810**. Then, the ultrasound information providing apparatus **100** may apply the measured angle at the position **810** to all Doppler data of the thickness **820** of the blood vessel **800** to correct the Doppler data. That is, the ultrasound information providing apparatus **100** may apply the Doppler data at the position **810** to the Doppler data of the thickness **820**.

[0139] Similarly, at a position **830**, the ultrasound information providing apparatus **100** may apply an angle (which is measured at the position **830**) between a guideline and a beam axis to Doppler data of a thickness **840**.

[0140] As illustrated in FIG. 8, another embodiment may be applied at the position **830**. That is, at the position **830**, the blood vessel **800** is thicker than the position **810**, and thus, the ultrasound information providing apparatus **100** may apply the angle measured at the position **830** to only the thickness **820** set at the position **810** without applying the angle measured at the position **830** to the thickness **840**. In other words, the ultrasound information providing apparatus **100** may arbitrarily set a region to be corrected, and correct Doppler data with the set region being maintained. However, since the thickness of the blood vessel **800** (an object) changes, the ultrasound information providing apparatus **100** may automatically change a region to be corrected, and correct Doppler data.

[0141] FIG. 9 are diagrams for describing an operation of correcting Doppler data by using nearby Doppler data, according to an embodiment of the present invention. As described above with reference to FIG. 1, as a Doppler angle becomes closer to 90 degrees, a cosine function result of the Doppler angle becomes close to 0, causing a reduction in reliability of Doppler data. Therefore, when a measured angle between a guideline and a beam axis is within a predetermined range, the ultrasound information providing apparatus **100** may use Doppler data at a position which is spatially close to a measured position.

[0142] As illustrated in FIG. 9A, the ultrasound information providing apparatus **100** may previously determine a certain range, which enables data of an ambient space to be

used, with respect to an angle between a guideline illustrated as a dashed line and a beam axis illustrated as a solid line. According to an embodiment, the ultrasound information providing apparatus **100** may set the certain range to an angle of 85 degrees to less than 95 degrees.

[0143] In FIG. 9B, a guideline **920** of a blood vessel **910** is displayed on a Doppler image **900**. A Doppler angle of a region **930** is close to 90 degrees, and thus, the blood vessel **910** is illustrated as being discontinuous on the Doppler image **900**. The ultrasound information providing apparatus **100** may measure an angle between the guideline and the beam axis in the region **930**, and determine whether the measured angle is within the range set in FIG. 9A.

[0144] When the angle measured in the region **930** is within the previously determined range, by using Doppler data at a position which is spatially close to a position where the angle within the previously determined range is measured, the ultrasound information providing apparatus **100** may correct Doppler data at the position where the angle is measured. For example, the ultrasound information providing apparatus **100** may use Doppler data at a position previous or subsequent to the position where the angle within the previously determined range is measured, where angles are measured in a region including the Doppler data. The ultrasound information providing apparatus **100** may correct the Doppler data at the position where the angle within the previously determined range is measured, by using ambient Doppler data according to an interpolation technique.

[0145] FIG. 10 are graphs for describing an operation of scaling up a color map matched with Doppler data, according to an embodiment of the present invention. In the graphs of FIGS. 10A and 10B, the abscissa axis indicates samples of corrected Doppler data, and the ordinate axis indicates a moving speed of an object. Also, a waveform illustrated as a solid line illustrates a moving speed of the object included in Doppler data previous to correction, and a waveform illustrated as a dashed line illustrates a moving speed of the object included in corrected Doppler data, namely, a moving speed previous to projection onto a beam axis.

[0146] In FIG. 10A, a moving speed of the object that is illustrated as a waveform **1012** is corrected by using an angle between a guideline and a beam axis for each of the samples of the Doppler data. The moving speed of the object that is included in the corrected Doppler data is illustrated as a waveform **1014**.

[0147] An upper limit line and lower limit line of FIG. 10A indicate a range of a color map which is used to generate a Doppler image by using the Doppler data. That is, in the color map, the moving speed of the object is matched in a color. In a color map according to an embodiment of FIG. 10A, a speed within a range **1020** may be matched in a color.

[0148] In FIG. 10B, the ultrasound information providing apparatus **100** corrects a moving speed of the object that is illustrated as a waveform **1032** to a waveform **1034**. The color map, matched for the Doppler data previous to correction, is matched for a speed within a range **1040**. Therefore, the waveform **1034** indicating a moving speed subsequent to correction is not within a range that enables the matched color map to be applied, the waveform **1034** may be expressed in an undesired color due to aliasing, which occurs in a Doppler image.

[0149] Therefore, when the Doppler data subsequent to correction is not within a color range of the color map matched with the Doppler data previous to correction, the

ultrasound information providing apparatus **100** may scale up the range of the color map from the range **1040** to the range **1050**, thereby enabling the scaled-up range to cover the moving speed that is illustrated as the corrected waveform **1034**.

[0150] FIG. **11** is a diagram for describing an operation of correcting color Doppler data and tissue Doppler data, according to an embodiment of the present invention. FIG. **11** illustrates a Doppler image **1100** of a heart **1110**. In darkly illustrated parts of FIG. **11**, an upper part indicates a left atrium (LA), a lower part indicates a left ventricle (LV), and a part connecting the LA and the LV indicates a mitral valve (MV). A part illustrated as an oblique line indicates blood which flows to the LV when the LA contracts. A part illustrated white in the heart **1110** indicates a myocardium surrounding the heart **1110**.

[0151] The ultrasound information providing apparatus **100**, as illustrated, may display at least one of a color Doppler image and a tissue Doppler image on a screen. That is, the ultrasound information providing apparatus **100** may simultaneously generate the color Doppler image and the tissue Doppler image, and display the color Doppler image and the tissue Doppler image on the screen. For example, the ultrasound information providing apparatus **100** may display the tissue Doppler image obtained by processing tissue Doppler data for the myocardium, and display the color Doppler image obtained by processing color Doppler data for blood flowing to the LV.

[0152] As described above, the ultrasound information providing apparatus **100** may correct the color Doppler data by using an angle “ $\theta 4$ ” between a guideline and a beam axis at a position **1150**, for blood.

[0153] The ultrasound information providing apparatus **100** may correct the tissue Doppler data for the myocardium through an operation similar to that of the blood. That is, the ultrasound information providing apparatus **100** acquires a guideline for the myocardium on the basis of a user input or a guideline detecting algorithm. Then, the ultrasound information providing apparatus **100** measures an angle “ $\theta 1$ ” between a guideline and a beam axis at a position **1120**, an angle “ $\theta 2$ ” between a guideline and the beam axis at a position **1130**, and an angle “ $\theta 3$ ” between a guideline and a beam axis at a position **1140**. The ultrasound information providing apparatus **100** may correct the tissue Doppler data to a value previous to projection onto the beam axis, on the basis of each of the angles, and display a new tissue Doppler image based on the corrected Doppler data on a screen.

[0154] FIG. **12** is a diagram for describing an operation of correcting 3D Doppler data, according to an embodiment of the present invention. A 3D Doppler image **1200** of FIG. **12** displays a blood vessel **1210** disposed in a space by using 3D coordinates **1205**.

[0155] The ultrasound information providing apparatus **100**, as described above, may acquire a guideline **1220** of the blood vessel **1210** displayed on the 3D Doppler image **1200** according to a user input or the guideline detecting algorithm. The ultrasound information providing apparatus **100** may display the generated guideline **1220** on the 3D Doppler image **1200**, or may internally use the guideline **1220** in the system without visually displaying the guideline **1220**. The guideline **1220** of the 3D Doppler image **1200** may be a straight line or a curve disposed in a 3D space.

[0156] The ultrasound information providing apparatus **100** measures an angle “ $\theta 1$ ” between the guideline **1220** and a beam axis **1230** of a probe at a position **1240** and an angle

“ $\theta 2$ ” between the guideline **1220** and the beam axis **1230** at a position **1250**. The ultrasound information providing apparatus **100** may correct 3D Doppler data on the basis of the measured angles, and display a 3D Doppler image based on the corrected 3D Doppler data on a screen.

[0157] As described above, according to the one or more of the above embodiments of the present invention, the ultrasound information providing apparatus and method minimize errors in a moving speed of an object and Doppler data generated according to a Doppler angle. Therefore, a user accurately diagnoses the object, and efficiently reads out a Doppler image. In addition, the ultrasound information providing apparatus and method minimize a degree by which a result of a Doppler image is changed depending on a user’s workmanship, thus enhancing accessibility to the Doppler image.

[0158] The above-described method may be written as computer programs and may be implemented in general-use digital computers that execute the programs using computer-readable recording media. The information used in the aforementioned embodiments may be recorded in computer-readable recording media through various members. Program storage devices usable for describing a storage device including executable computer code for performing various methods of the present invention should not be understood as including transitory targets like signals. Examples of the computer-readable recording medium include magnetic storage media (e.g., ROM, floppy disks, hard disks, etc.) and optical recording media (e.g., CD-ROMs or DVDs).

[0159] It should be understood that the exemplary embodiments described therein should be considered in a descriptive sense only and not for purposes of limitation. Descriptions of features or aspects within each embodiment should typically be considered as available for other similar features or aspects in other embodiments.

[0160] While one or more embodiments of the present invention have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various changes in form and details may be made therein without departing from the spirit and scope of the present invention as defined by the following claims.

What is claimed is:

1. An ultrasound information providing method comprising:
 - generating a first Doppler image from Doppler data of an object;
 - acquiring a guideline indicating a moving path of the object in the first Doppler image;
 - correcting the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and
 - displaying a second Doppler image generated from the corrected Doppler data.
2. The ultrasound information providing method of claim 1, wherein the acquiring comprises acquiring the guideline on a basis of a user input, which draws a line on the first Doppler image, or a guideline detecting algorithm.
3. The ultrasound information providing method of claim 1, further comprising displaying the guideline.
4. The ultrasound information providing method of claim 3, wherein the displaying of the guideline comprises displaying the guideline on at least one of the first and second Doppler images.

5. The ultrasound information providing method of claim 1, wherein the correcting comprises correcting the Doppler data to data previous to projection onto the beam axis by using the angle.

6. The ultrasound information providing method of claim 1, wherein the angle comprises an acute angle between the guideline and the beam axis.

7. The ultrasound information providing method of claim 1, further comprising setting a region of which the Doppler data is to be corrected.

8. The ultrasound information providing method of claim 7, wherein the region comprises a thickness of the object.

9. The ultrasound information providing method of claim 7, wherein the setting comprises setting the region on a basis of a user input or a blood vessel region detecting algorithm.

10. The ultrasound information providing method of claim 1, wherein the correcting comprises, when the angle is within a predetermined range, correcting the Doppler data by using spatially near Doppler data.

11. The ultrasound information providing method of claim 1, further comprising, when the corrected Doppler data is not within a range of a color map matched with the Doppler data previous to the correction, scaling up the color map.

12. The ultrasound information providing method of claim 1, wherein the Doppler data comprises two-dimensional (2D) Doppler data or three-dimensional (3D) Doppler data.

13. The ultrasound information providing method of claim 1, wherein the Doppler data comprises at least one of color Doppler data indicating blood flow and tissue Doppler data indicating a motion of tissue.

14. An ultrasound information providing apparatus comprising:

- a data acquirer that acquires Doppler data of an object;
- an image processor that generates a first Doppler image from the Doppler data of the object, and acquires a guideline indicating a moving path of the object in the first Doppler image;
- a data processor that corrects the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and
- a display unit that displays a second Doppler image by using the corrected Doppler data.

15. The ultrasound information providing apparatus of claim 14, wherein the image processor acquires the guideline on a basis of a user input, which draws a line on the first Doppler image, or a guideline detecting algorithm.

16. The ultrasound information providing apparatus of claim 14, wherein the display unit displays the guideline.

17. The ultrasound information providing apparatus of claim 16, wherein the display unit displays the guideline on at least one of the first and second Doppler images.

18. The ultrasound information providing apparatus of claim 14, wherein the image processor corrects the Doppler data to data previous to projection onto the beam axis by using the angle.

19. The ultrasound information providing apparatus of claim 14, wherein the angle comprises an acute angle between the guideline and the beam axis.

20. The ultrasound information providing apparatus of claim 14, wherein the image processor sets a region of which the Doppler data is to be corrected.

21. The ultrasound information providing apparatus of claim 20, wherein the region comprises a thickness of the object.

22. The ultrasound information providing apparatus of claim 20, wherein the image processor sets the region on a basis of a user input or a blood vessel region detecting algorithm.

23. The ultrasound information providing apparatus of claim 14, wherein when the angle is within a predetermined range, the image processor corrects the Doppler data by using spatially near Doppler data.

24. The ultrasound information providing apparatus of claim 14, wherein when the corrected Doppler data is not within a range of a color map matched with the Doppler data previous to the correction, the image processor scales up the color map.

25. The ultrasound information providing apparatus of claim 14, wherein the Doppler data comprises two-dimensional (2D) Doppler data or three-dimensional (3D) Doppler data.

26. The ultrasound information providing apparatus of claim 14, wherein the Doppler data comprises at least one of color Doppler data indicating blood flow and tissue Doppler data indicating a motion of tissue.

27. A non-transitory computer-readable storage medium storing a computer program for executing the ultrasound information providing method of claim 1.

28. An ultrasound information providing method comprising:

- acquiring a guideline indicating a moving path of an object from Doppler data of the object;
- correcting the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and
- displaying a Doppler image generated from the corrected Doppler data.

29. An ultrasound information providing apparatus comprising:

- a data acquirer that acquires Doppler data of an object;
- an image processor that acquires a guideline indicating a moving path of the object from the Doppler data;
- a data processor that corrects the Doppler data on a basis of an angle between the guideline and a beam axis of a probe; and
- a display unit that displays a Doppler image which is generated by the image processor by using the corrected Doppler data.

* * * * *

专利名称(译)	通过使用指南提供超声信息的方法和装置		
公开(公告)号	US20150080735A1	公开(公告)日	2015-03-19
申请号	US14/485650	申请日	2014-09-12
[标]申请(专利权)人(译)	三星麦迪森株式会社		
申请(专利权)人(译)	三星MEDISON CO. , LTD.		
当前申请(专利权)人(译)	三星MEDISON CO. , LTD.		
[标]发明人	HYUN DONG GYU CHOI SEOK WON		
发明人	HYUN, DONG-GYU CHOI, SEOK-WON		
IPC分类号	A61B8/08 A61B8/00 G06T7/20 A61B8/06		
CPC分类号	A61B8/488 A61B8/06 A61B8/5269 A61B8/463 G06T2207/30101 G06T2200/24 G06T2207/10132 G06T2207/20104 G06T7/20 A61B8/085 A61B8/0858 A61B8/0883 A61B8/0891 A61B8/467 A61B8/469 A61B8/483 A61B8/5207 A61B8/5223 G06T5/006		
优先权	1020130110613 2013-09-13 KR		
外部链接	Espacenet USPTO		

摘要(译)

公开了一种超声信息提供方法和设备。超声信息提供方法包括从对象的多普勒数据生成多普勒图像，获取指示多普勒图像中的对象的移动路径的指南，基于指南与光束轴之间的角度校正多普勒数据。探测器，并显示由校正的多普勒数据产生的多普勒图像。

