



(19) **United States**

(12) **Patent Application Publication**
Wang et al.

(10) **Pub. No.: US 2012/0203103 A1**

(43) **Pub. Date: Aug. 9, 2012**

(54) **PHOTOACOUSTIC CONTRAST AGENT
BASED ACTIVE ULTRASOUND IMAGING**

Publication Classification

(75) Inventors: **Yao Wang**, Arlington, VA (US);
William Tao Shi, Briarcliff Manor,
NY (US)

(51) **Int. Cl.**
A61B 8/14 (2006.01)
(52) **U.S. Cl.** **600/431**

(73) Assignee: **KONINKLIJKE PHILIPS
ELECTRONICS N.V.**,
EINDHOVEN (NL)

(57) **ABSTRACT**

Electromagnetic energy is applied to thereby oscillate a bubble that is then insonified to produce an echo (260) for reception and analysis to afford imaging of the region of the bubble. To create the bubble, the energy may be applied to a nano particle (232) of a contrast agent whose consequent internal nano- or micro-bubbles offer, with novel pulsing techniques, greater sensitivity, and which can permeate outside vasculature (216) prior to being energized thereby affording quantification of vascular permeability and delivery of targeting molecules. The particle can include an absorbing and an evaporating parts, the irradiation (204), as by near-infrared laser, causing the phase change that gives rise to the bubble. The echo may occur in response to ultrasound interrogation (220) of the activated contrast agent, which could entail pulse inversion, power modulation or contrast pulse sequence imaging, with persistence processing. The contrast agent might be mixed with microbubble based ultrasound contrast agent to facilitate the timing of bubble activation.

(21) Appl. No.: **13/501,683**


(22) PCT Filed: **Oct. 11, 2010**

(86) PCT No.: **PCT/IB2010/054595**

§ 371 (c)(1),
(2), (4) Date: **Apr. 12, 2012**

Related U.S. Application Data

(60) Provisional application No. 61/252,214, filed on Oct. 16, 2009.

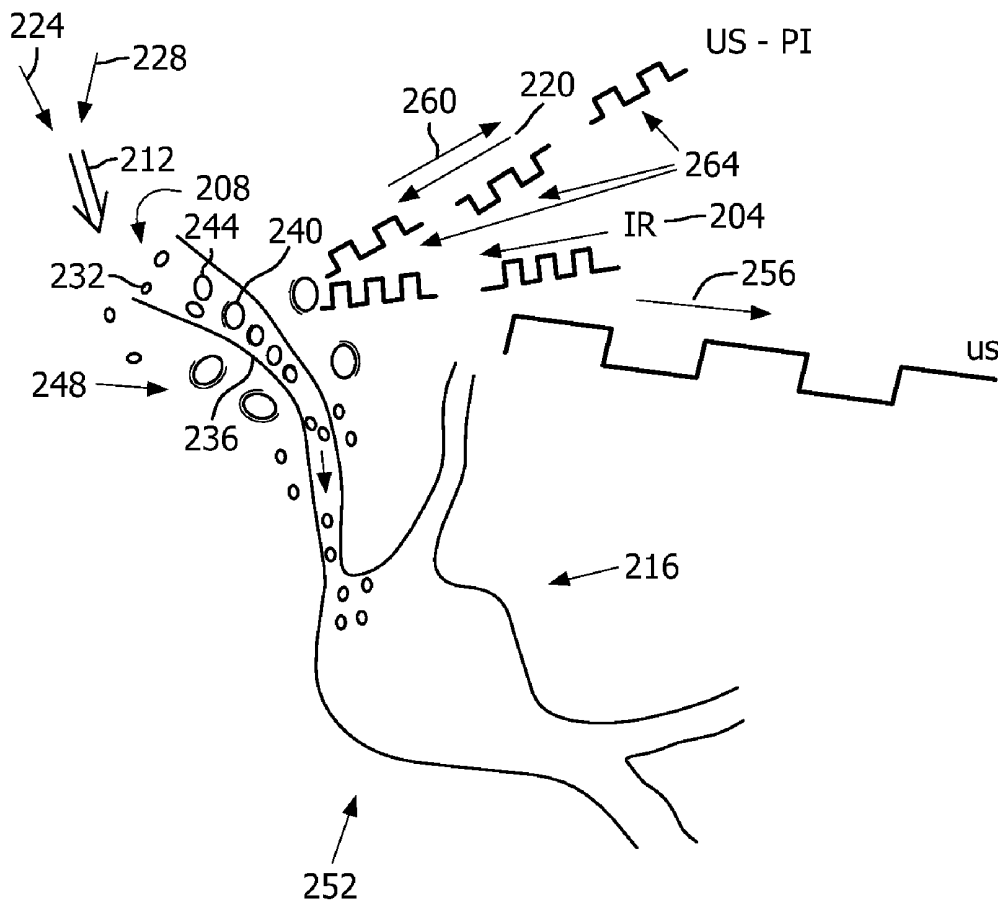

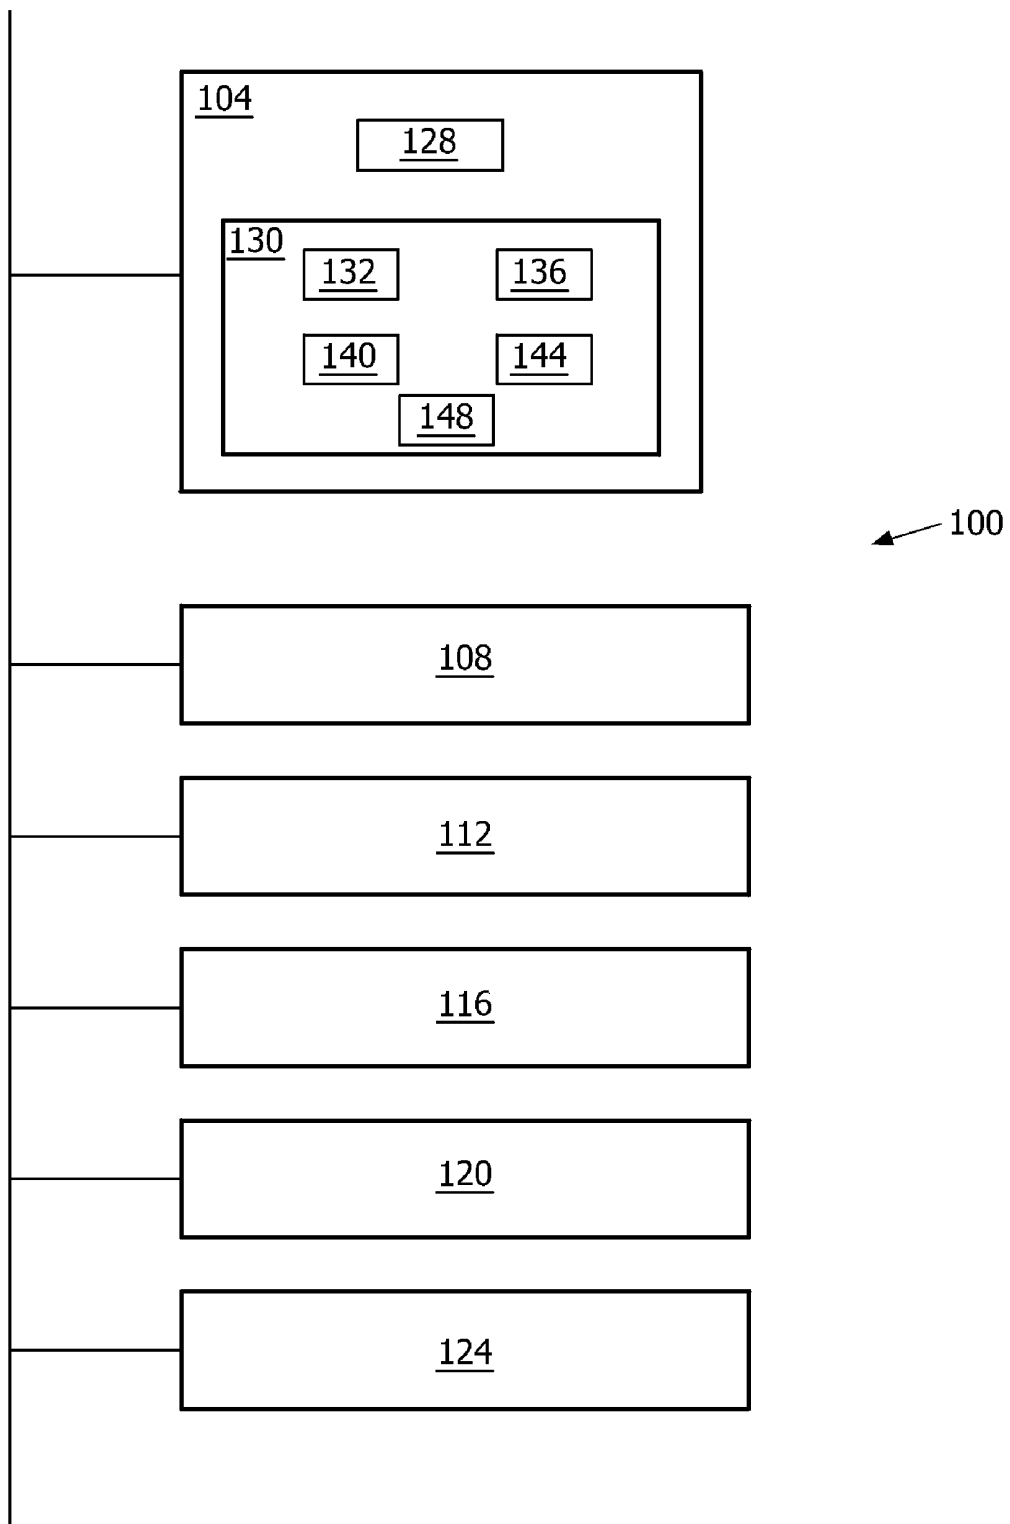


FIG. 1

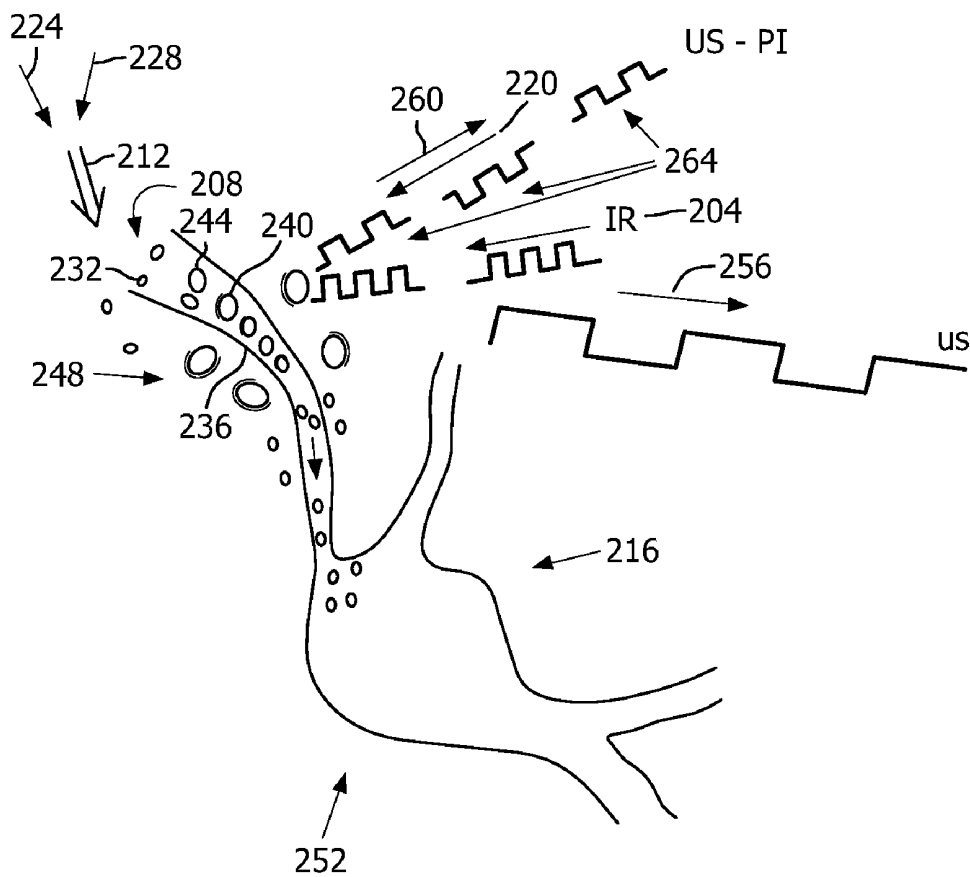


FIG. 2

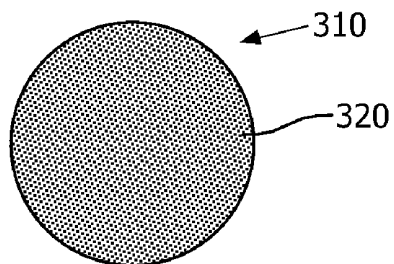


FIG. 3

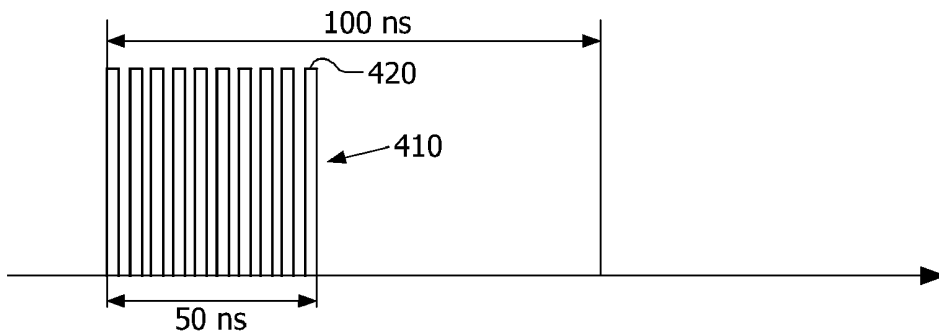


FIG. 4

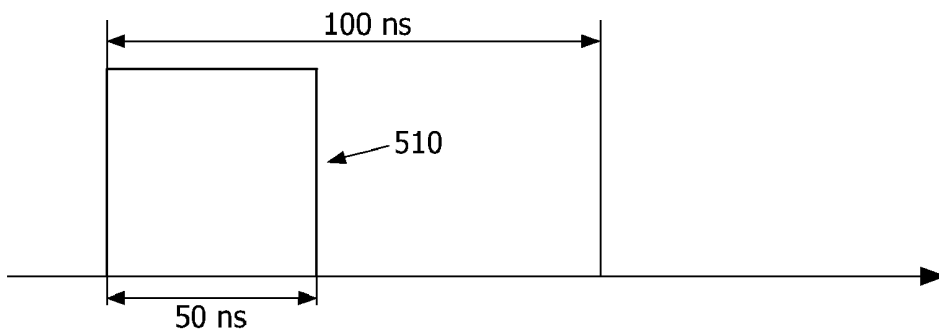


FIG. 5

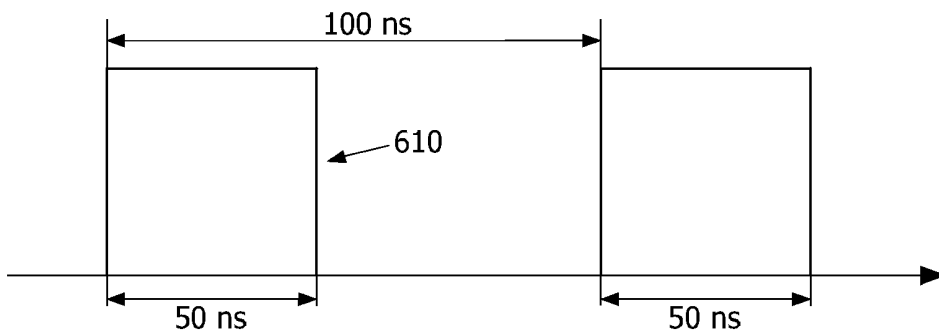


FIG. 6

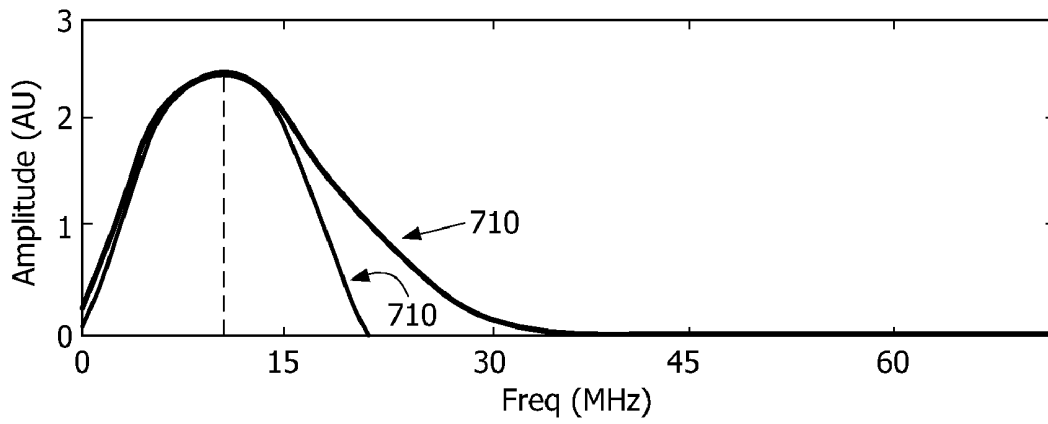


FIG. 7

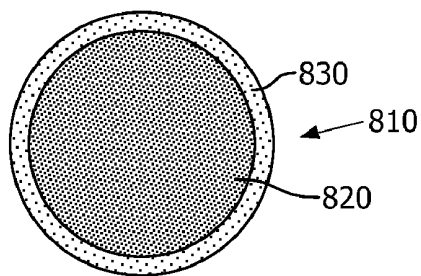


FIG. 8

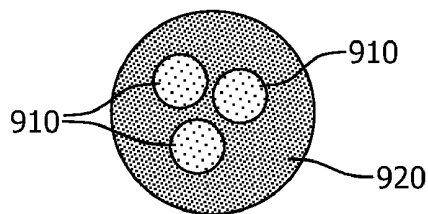


FIG. 9

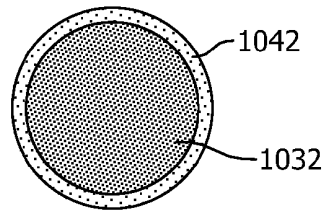


FIG. 10a

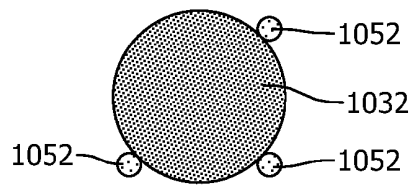


FIG. 10b

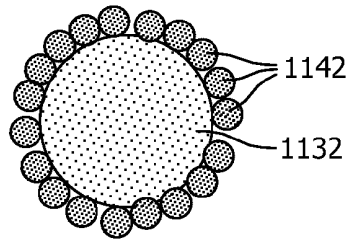


FIG. 11a

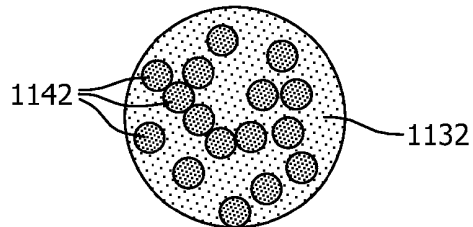


FIG. 11b

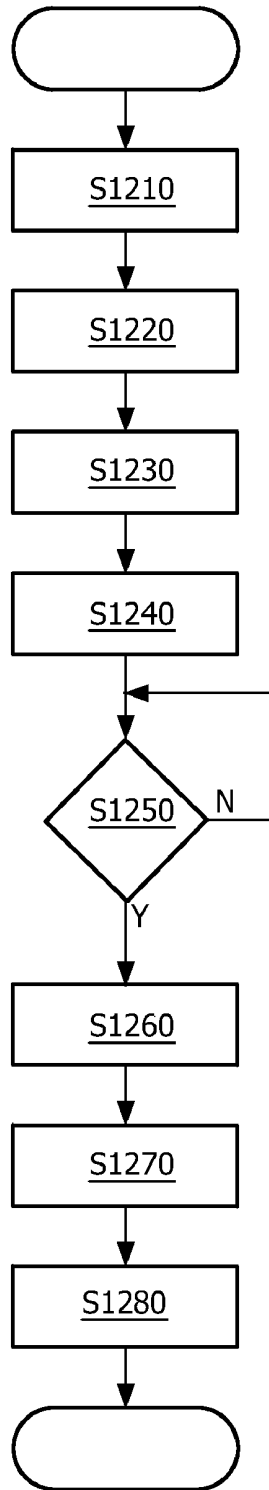


FIG. 12

PHOTOACOUSTIC CONTRAST AGENT BASED ACTIVE ULTRASOUND IMAGING

FIELD OF THE INVENTION

[0001] The present invention is directed to applying electromagnetic energy for imaging and, more particularly, to energizing a substance serving as an ultrasound contrast agent.

BACKGROUND OF THE INVENTION

[0002] Photoacoustic (PA) imaging is a noninvasive imaging technique that may be used in medical environments, e.g., to detect, inter alia, vascular disease, skin abnormalities and some types of cancer. PA imaging generally involves flashing a laser at low energy with a near-infrared wavelength onto a target area or region. Infrared light penetrates relatively deeply into the body. This creates a large radiated area for a more detailed picture. Rapid absorption of laser energy expands the tissue (composed of microscopic absorbers) through transient thermo-elastic expansion. The pulsating expansion creates ultrasonic acoustic waves that can be detected by ultrasound detectors of appropriate sensitivity, e.g., ultrasound transducers. The transducer readings can be processed and interpreted using different mathematical equations/algorithms to create two- or three-dimensional images of the target area, showing the tissue structure via spatial distribution of microscopic absorbers or the flow of a blood-stream carrying the absorbers.

[0003] PA imaging is effective in anatomical applications based on its unique contrast mechanism. Typically, each tissue or target region absorbs different amounts of the laser energy, making each different target region or tissue potentially unique from a PA imaging standpoint. For purposes of blood vessel-related imaging, hemoglobin generally exhibits high optical contrast when a near-infrared wavelength is applied. This contributes to the sensitivity of blood vessel imaging with PA techniques, enabling doctors/health care providers to see abnormalities in the skin, vascular disease and cancer which can then be treated directly. PA images can be combined with those from other modalities (e.g., ultrasound) to create highly detailed depictions of the target area with complementing contrast. For example, the generated images may facilitate valuable diagnostics, e.g., allowing clinicians to identify small lesions that may be difficult to pick up using other techniques/technologies.

[0004] Recently, there have been developed PA contrast agents whose constituent particles are dimensioned down to the nanometer level and are considerably smaller than the microbubbles used in ultrasound imaging.

[0005] A PA contrast agent based on particles of nanometer proportion that can diffuse through blood vessels has been used to endocytose cells outside the vasculature. See U.S. Patent Publication No. 2008/0160090 to Oraevsky et al., entitled "Laser-Activated Nanothermolysis of Cells," (hereinafter referred to as the "'090 publication"), the disclosure of which is incorporated by reference in its entirety.

[0006] However, this PA contrast agent and other PA contrast agents based on particles of nanometer dimension currently available and under development suffer from low sensitivity due to their low acoustical emission, owing to their small particle size.

[0007] Furthermore, incident optical pulsing is generally out of the reception bandwidth of ultrasound instrumentation and, thus, the optical energy is inefficiently converted into ultrasound signals.

[0008] Sufficiently energetic laser irradiation of "'090 publication" nanoparticles sufficiently large, or joined in big enough clusters, can produce surrounding microbubbles which would increase acoustical emission, but emergence of the microbubbles requires energizing to a level that thermo-mechanically destroys local tissue, in accordance with the tumor ablation function of that technique.

[0009] Microbubble-based ultrasound contrast agents offer certain recognized advantages in enhancing regular backscatter signals and generating distinct backscatter signals (e.g., super-harmonics and sub-harmonics of incident ultrasound waves) within the ultrasound receive passband. (See, e.g., Shi W T, Forsberg F, Liu J B, Merritt C R B, Goldberg B B: "New US media boosts imaging quality," Diagnostic Imaging Global: Special Supplement, November 2000, pp 8-12.)

[0010] However, the relatively large size, i.e., of a microbubble, makes known microbubble-based contrast agents unavailable for measuring vascular parameters, such as permeability.

[0011] The use of nano-bubbles—which potentially would overcome the limitations associated with known microbubble-based agents—in ultrasound backscatter imaging has not been realized for several reasons. For example, the lifetime of a nano-bubble is too short for intravenous injection and subsequent human circulation, mainly because of the tremendous surface tension against the shell material in this size range. Additionally, the backscatter cross-section of such nano-bubbles is very small. Since backscatter cross-section is determined by the 6th power on scatterer size, a factor of 10 reduction in bubble diameter may lead to a 10⁶ times (60 dB) reduction in backscatter power, which is a diminishing return.

SUMMARY OF THE INVENTION

[0012] Firstly, it is observed by the present inventors that existing PA agents were primarily developed for optical purposes and rely on increased optical absorption alone to be effective and operable. To date, insufficient attention has been directed to PA agents that improve upon the conversion of absorbed optical energy to in-band ultrasound signals. This lack of effective conversion functionality is a hindrance to the overall effectiveness and applicability of PA agents and PA imaging techniques.

[0013] One or more of the above concerns and shortcomings of the prior art are addressed in commonly-assigned International Patent Publication No. 2009/057021, entitled "Photoacoustic Imaging Contrast Agent and System for Converting Optical Energy to In-Band Acoustic Emission," (hereinafter the "'021 publication") to the present inventors, the disclosure of which is incorporated herein by reference in its entirety. The "'021 publication" reveals PA contrast agents that are optimally tuned for the ultrasonic receive passband of the PA transducer to provide more effective imaging systems. In addition, the contrast agents constituents disclosed therein are sufficiently small to permeate capillary walls and like anatomical structures. This permits an expansion of PA imaging/measurement applications, e.g., to vascular parameters such as permeability. These contrast agents are sufficiently stable for advantageous clinical use, e.g., by intravenous injection and circulatory migration to desired locations/regions.

[0014] What is proposed herein utilizes the PA contrast agents disclosed in the “’021 publication,” and represents an improvement as to systems and methods.

[0015] The present inventors have realized that going beyond passive reception of ultrasound can offer even greater sensitivity and therefore more accurate imaging. The echo from an ultrasound transmit can be utilized, for example, to better distinguish blood flow information from that pertaining to the surrounding tissue such as vascular walls. It can also be used to more reliably identify motion, such as by organs due to the heartbeat or respiration. Ultrasound pulsing methods proposed herein advantageously cater to the relatively small acoustic returns by nano-bubbles and microbubbles produced in accordance with the instant disclosure.

[0016] In one aspect of the present invention, electromagnetic energy is applied to thereby oscillate a bubble in a region. The oscillating bubble is insonified to produce an echo for reception and analysis to afford imaging of the region.

[0017] In one other aspect, the applying causes a phase change in a particle to thereby create the bubble from its particle.

[0018] In a different aspect, the particle comprises an elastic coating.

[0019] In a further aspect, the phase change occurs in response to absorption of the energy by the particle.

[0020] In yet another aspect, the applying comprises applying the energy to an ultrasound contrast medium based on nanoparticles small enough to pass through a vascular wall thereby creating the bubble in a respective one of the nanoparticles.

[0021] In a related version, the applying entails applying energy to oscillate a plurality of bubbles that includes the bubble. The insonifying is performed with low mechanical index.

[0022] In yet further aspect, the applying is commenced, and the imaging is performed, at a time at which a portion of inflow of the bubbles into vasculature has permeated outside the vasculature.

[0023] In some sub-versions, the imaging at that time is performed with persistence processing.

[0024] In some sub-versions, the insonifying is performed according to pulse inversion imaging.

[0025] In some sub-versions, the insonifying is performed according to power modulation imaging.

[0026] In some sub-versions, the insonifying is performed according to contrast pulse sequence imaging.

[0027] In a particular aspect, parameters of a contrast agent are tuned to allow conformance of a power spectrum of bubble oscillation to an ultrasound transducer receive spectral sensitivity curve.

[0028] In another, related aspect, inflow of microbubbles into vasculature is detected, and the applying is commenced responsive to the detecting.

[0029] In a particular embodiment, the method further includes receiving the echo and analyzing the received echo to afford the imaging.

[0030] In some embodiments, the insonifying includes firing a plurality of ultrasound pulses in a common direction, and the analyzing entails coherently combining data echoed back from the pulses.

[0031] In other embodiments, the insonifying produces a plurality of echoes that are received, and the analyzing comprises combining signals based on the echoes and analyzing the combined signals.

[0032] In another alternative aspect, an ultrasonic device features a transmission activator configured for delivering electromagnetic energy to excite a substance in a region so as to enhance utility of the substance as an ultrasound contrast agent, and for delivering, to the excited substance, ultrasound to afford imaging of the region.

[0033] In a related alternative aspect, the delivering of electromagnetic energy includes issuing separate bursts of electromagnetic pulses that propagate to the region and, in accordance with a tunable parameter of the substance, match a frequency of consequent energy absorption by the substance to a target frequency of bubble oscillation in the region by the energy.

[0034] In other, further aspects, the substance includes a nanoparticle-based contrast medium comprising a nanoparticle. Delivering electromagnetic energy expands the nanoparticle into a particle that includes a bubble oscillated by the energy, the bubble serving as an interrogation target for the imaging.

[0035] According to other different aspects, the ultrasonic device further includes an ultrasound transducer with a spectral sensitivity curve, the exciting being such as would cause by itself, without the delivered ultrasound, emission of an acoustic signal whose power spectrum is overlapped, area-wise, by the curve by more than half.

[0036] In some yet further versions, a computer software product for medical analysis incorporates a computer readable storage medium embodying a computer program that includes instructions executable by a processor to perform at least the acts of: applying electromagnetic energy to thereby oscillate a bubble in a region; and insonifying the oscillating bubble to produce an echo for reception and analysis to afford imaging of the region.

[0037] In other still further versions, an article of manufacture comprises a machine-accessible storage medium having instructions encoded thereon for enabling a processor to perform medical analysis by executing acts, including: applying electromagnetic energy to thereby oscillate a bubble in a region; and insonifying the oscillating bubble to produce an echo for reception and analysis to afford imaging of the region.

[0038] In one, yet, additional aspect, the present disclosure features a mixture of nanoparticle-based contrast agent and microbubble-based ultrasound contrast agent.

[0039] Details of the novel, photoacoustic contrast agent based active ultrasound imaging are set forth further below, with the aid of the following drawings, which are not drawn to scale.

BRIEF DESCRIPTION OF THE DRAWINGS

[0040] FIG. 1 is a schematic diagram demonstrating, by example, a design for a photoacoustic contrast agent based active ultrasound imaging system;

[0041] FIG. 2 is a schematic diagram depicting structurally and conceptually an example of an instance of laser irradiation responsive to detection of the inflow of mixed contrast agent into vasculature, and ultrasound interrogation concurrent with the irradiation;

[0042] FIG. 3 illustrates an exemplary contrast agent droplet according to the present disclosure;

[0043] FIG. 4 illustrates an exemplary laser pulse train for use in PA imaging systems of the present disclosure, the pulse train including 50 ns laser irradiation that is made up of 10 individual laser pulses;

[0044] FIG. 5 illustrates an exemplary laser irradiation waveform for use in PA imaging of the present disclosure that represents continuous laser irradiation for 50 ns;

[0045] FIG. 6 illustrates an exemplary embodiment of a laser irradiation waveform that advantageously matches the contrast agent response with the bandwidth (or “passband shape”) of a PA transducer;

[0046] FIG. 7 illustrates, as an example, exciting, by laser irradiation, such as would cause by itself, without the delivered ultrasound, emission of an acoustic signal whose power spectrum is overlapped by the ultrasound transducer spectral sensitivity curve by more than half;

[0047] FIG. 8 illustrates an exemplary contrast agent according to the present disclosure that includes a bi-layered nanoparticle with a core of absorbing and evaporating material and an outer shell of an elastic coating material, where, alternatively, the core may be an evaporating material only, while the elastic shell may be an optically absorbing material;

[0048] FIG. 9 illustrates an exemplary contrast agent composed of a two-liquid emulsion of nano-droplets, wherein the smaller evaporating droplets are embedded inside a larger droplet;

[0049] FIGS. 10a, 10b illustrate respectively an exemplary contrast agent made of optically absorbing particles covered with a coating (FIG. 10a) or droplets (FIG. 10b) of evaporating material according to the present disclosure;

[0050] FIGS. 11a, 11b illustrate an exemplary contrast agent consisting of a complex of an evaporation droplet and optically absorbing particles, where in FIG. 11a the evaporation droplet is covered by absorbing particles and, in FIG. 11b, multiple absorbing particles are embedded inside each droplet; and

[0051] FIG. 12 is a flow chart illustrating an exemplary process of the novel, photoacoustic contrast agent based active ultrasound imaging.

DETAILED DESCRIPTION OF EMBODIMENTS

[0052] FIG. 1 offers, by way of illustrative and non-limitative example, a design for a photoacoustic (PA) contrast agent based active ultrasound imaging system 100. The imaging system 100 features a processing module 104, a contrast medium injector 108, a Q-switched laser 112, a laser-diode type laser 116, a transducer 120 and a display 124, the components being communicatively connected by wire or wirelessly. The processing module 104, implementable with one or more integrated circuits and/or computer software for example, includes a transmission activator 128; a multiple pulse processor 130 including but not limited to one or more of a pulse inversion (PI) processor 132, a power modulation (PW) processor 136, and a contrast pulse sequence (CPS) processor 140; a persistence processor 144; and storage 148 that includes working storage and control storage.

[0053] Irradiation by the laser 112, 116 is commenced by the transmission activator 128 at the appropriate time to activate in-situ the nanoparticle-based contrast agent. At this time, the activator 128 can further activate the transducer 120 to interrogate oscillating bubbles, whose genesis and oscillating occurs as a result of the pulsed laser irradiation. Alternatively, the ultrasound interrogation 220 can be already ongoing at the onset of laser irradiation.

[0054] FIG. 2 depicts structurally and conceptually an example of an instance of infrared (IR) or near-infrared laser irradiation 204, by the Q-switched laser 112, responsive to detection of an inflow 208 of mixed contrast agent 212 into

vasculature 216. Further depicted is ultrasound interrogation 220, by means of the transducer 120, concurrent with the irradiation.

[0055] The mixed contrast agent 212, as originally injected into a subject, e.g., human or animal, in vivo, ex vivo or in vitro, is a mixture in a saline solution, of a nanoparticle-based PA contrast agent 224, as described in the “’021 publication,” and any, i.e., typical, microbubble-based ultrasound contrast agent 228. Mixing with the microbubble-based ultrasound contrast agent 228 makes detection of the inflow 208 easier, since irradiation 204 to activate nanoparticles 232 is delayed until the nanoparticles have had a chance to permeate through vasculature walls 236. Once the inflow 208 is detectable, permeation has already occurred or is underway. As mentioned in the “’021 publication,” selected nanoparticle-based PA contrast agents 224 may be used in combination with conventional microbubble generating media 228 so as to realize the benefits of both contrast agents 224, 228. The mixture 212 may be injected by means of the contrast medium injector 108. Activation of the nanoparticle-based agent 224 is delayed to afford permeation through tissue and blood vessel walls 236, e.g., for purposes of quantifying vascular permeability. The permeation can also serve the molecular imaging/diagnostics purpose of delivering targeting molecules conjugated to the nanoparticles 232.

[0056] In the absence of ultrasound interrogation 220, and in the way of background and as discussed in the “’021 publication,” the resonance of the nano-bubbles (and/or microbubbles) 240 produced as a result of the near-infrared-irradiation 204 of the nanoparticles is advantageously adapted to function as an efficient acoustic radiator, i.e., an ultrasonic source for purposes of PA imaging systems. (Although its nanoparticle is not shown in FIG. 2, the oscillating bubble 240 is shown with an adjacent contour to represent oscillation, i.e., due to the ongoing, on and off energy absorption of the nanoparticle. It is noted that a microbubble 244 of the microbubble-based medium 228, not having an absorbing part of its own, does not oscillate.)

[0057] The novel systems, devices and techniques of the “’021 publication” are enhanced by the instant proposal wherein the resonating bubbles 240 serve well as scatterers whose echoes are robustly processed using compatible ultrasound pulsing/imaging techniques afforded by the processing module 104.

[0058] Moreover, as seen in FIG. 2, a portion 248 of the inflow 208 that has diffused outside the vasculature 216 has been activated, under the influence of the infrared irradiation 204, to produce oscillating bubbles detectable by means of the interrogating ultrasound 220.

[0059] As mentioned in the “’021 publication,” the laser irradiation 204 is absorbed by an absorbing part of a nanoparticle 232 and thereby heated, typically by only a few degrees Celsius, to cause a part of the nanoparticle to undergo a phase change, i.e., evaporation. This results in a bubble 240, and consequent spatial expansion of its nanoparticle. Pulsed application of the laser 112, 116, and the consequent energy absorption, causes the bubbles 240 that arise to oscillate.

[0060] The nanoparticle-based contrast agent/contrast medium 224 may be defined by a nanoparticle 232, e.g., gold nano-sphere, nano-rod, or the like, that is encapsulated and/or coated by a coating material. The coating material may be a perfluorocarbon material/composition, with a low boiling point, and is typically optically transparent, while exhibiting

mechanical elasticity, thereby allowing the droplet to advantageously expand during phase change.

[0061] For delivery purposes, the nanoparticle-based contrast agent/contrast medium **224** may be suspended in a carrier solution, alone or mixed with microbubble-based contrast medium **228**, for injection with respect to a target tissue region **252**. The carrier solution can be a saline-based solution, such as phosphate buffered saline (PBS). Due to the relatively small size, e.g., between about 50 nm and 500 nm in particle diameter, the medium **224** is free to permeate through capillary walls **236** and the like.

[0062] The acoustic signal generated due to bubble oscillation is characterized by a frequency that can be tuned by changing parameters associated with the contrast agent **224**, e.g., droplet size, materials of fabrication, coating/encapsulation materials/thickness, properties of multilayered droplets, and the like. The acoustic signals generated are typically characterized by a target frequency or frequency range. The bubbles (e.g., nano-bubbles and/or microbubbles) **232** resonate at frequencies that advantageously match (or substantially match) the spectral sensitivity curve of a receiving ultrasound transducer **120**. More particularly, nano-bubble and/or microbubble formation leads to generation of signature PA signals that correspond to the droplet size(s) of the contrast medium **224**.

[0063] As mentioned above in connection with the instant proposal, the resonating bubbles are actively interrogated by ultrasound pulsing techniques designed to detect and robustly process the small-amplitude oscillations.

[0064] With reference to FIG. 3 and as disclosed in the "021 publication," a first exemplary embodiment of the nanoparticle-based contrast agent **224** is depicted. The contrast agent **224** is formed of nanoparticle-based droplets **310** of optically absorbing material. The nanoparticle-based droplet **310** is further configured to undergo a phase change, i.e., evaporation, upon absorption of the requisite optical energy, for example laser energy associated with the laser **112**, **116**. Droplet sizes may vary in the same contrast agent **224** or as between different contrast agents, although the range between 50 nm and 500 nm or a distribution that includes this range is typical.

[0065] The nanoparticles **232** that define (in whole or in part) the exemplary droplet **310** of FIG. 3 may take the form of nano-spheres, nano-rods and the like. The nanoparticles **232** are generally optically stimulated by laser energy, thereby generating localized heat that in turn induces a phase change to the droplet **310**, i.e., converts the contrast medium **224** from liquid to gas. Such phase change conversion creates nano-bubbles and/or microbubbles. Thus, with further reference to FIG. 3, evaporation occurs inside the spherical droplet **310** once sufficient light is absorbed. Accordingly, the droplet **310** of the first embodiment comprises absorbing and evaporating material **320**.

[0066] In one example, the absorption cross-section of a gold nanoparticle **232** (e.g., a nano-sphere that is 40 nm in diameter or a nano-rod that is 25 nm in diameter and 100 nm in length) is in the range 10^{-11} to 10^{-9} cm². The gold nanoparticle **232** has a volume in the range 10^{-16} to 10^{-17} cc, a density of 19.3 g/cc and heat capacity of 0.128 J/g°C.

[0067] FIG. 4 shows an exemplary laser pulse train **410** including 50 ns laser irradiation that includes 10 individual laser pulses **420**. Each laser pulse **420** has a temporal duration of 3 ns (e.g., Philips™ Nd:YAG laser source defines this specification). The process may be controlled so that the

resultant gas-filled bubbles may resonate at a target frequency, here 10 MHz. The Q-switched laser **112** issues separate bursts **410** of electromagnetic pulses that, in accordance with one or more tunable parameters (e.g., droplet size, materials of fabrication, coating/encapsulation materials/thickness, properties of multilayered droplets) of the PA contrast medium **224**, match a frequency, e.g., 10 MHz, of consequent energy absorption by the medium to a target frequency of bubble oscillation.

[0068] Depending on the optical and thermal diffusivity of a selected material, the actual thermal expansion drive on the contrast agent **224** may resemble a prolonged (approximately 50 ns) impact, as shown in FIG. 5, which can also serve as an exemplary laser irradiation waveform. In an exemplary embodiment, the conversion efficiency can be increased to about 50%. FIG. 5 illustrates a possible laser irradiation waveform representing a single 50 ns pulse **510** of continuous irradiation. This form of excitation may be more easily achieved with the laser-diode type laser **116** of the type commonly used in telecommunications applications. The 50 ns pulse **510** can be repeated at 100 ns intervals as shown in FIG. 6.

[0069] FIG. 6 shows a further laser irradiation waveform that further matches the contrast agent response with the passband shape of the receiving transducer **120**. The irradiation waveform of FIG. 6 includes an initial 50 ns laser waveform **610** and one or more repetitions every 100 ns which achieves an upward modulation of the spectrum into the receive spectral sensitivity curve of the transducer **120**. The receive spectral sensitivity curve of an ultrasound detector generally resembles a Gaussian or Lorentian shape (with different receiver sensitivities at different frequencies) more than a rectangular window. The waveform excitation associated with FIG. 6 shifts the spectral centroid upward and away from the direct current (DC), thereby achieving an improved coupling in shape.

[0070] FIG. 7 illustrates, as an example, exciting, by laser irradiation **204**, such as would cause by itself, without the delivered ultrasound **220**, emission of an acoustic signal **256** whose power spectrum **710** is overlapped, area-wise, by a spectral sensitivity curve **720** of the receive passband of the ultrasound transducer **120** by more than half. Here, in FIG. 7, the overlap is seen to be substantially more than half.

[0071] FIG. 8 illustrates an exemplary contrast agent **224** that includes a bi-layered nanoparticle **810** with a core **820** of absorbing and evaporating material and an outer shell **830** of an elastic coating material, where, alternatively, the core may be an evaporating material only, while the elastic shell may be an optically absorbing material. The outer shell **830** avoids the possibility of the nano-bubble or microbubble **240** bursting as a result of the laser irradiation **204**. The size and resonant properties/frequency of the nano-bubble/microbubble **240** formed in and by means of the multi-layer/bi-layer nanoparticle **810** of FIG. 8 are akin to those described above with reference to FIG. 3.

[0072] Another exemplary embodiment is schematically depicted in FIG. 9. Instead of one liquid with both optical absorption and evaporation capabilities (e.g., as in FIG. 3), the exemplary agent **224** of FIG. 9 is an emulsion with two liquids. The emulsion includes at least one evaporating smaller nano-drop **910** inside a larger absorbing nano-drop **920**. Two-liquid emulsion droplets can be produced by various techniques, e.g., mechanical stirring, ultrasound sonification, etc.

[0073] As schematically depicted in FIGS. 10a, 10b, a further exemplary implementation includes an optically absorbing core 1032 (e.g., nano-spheres, nano-rods, etc.) encapsulated or covered with a thin, evaporating, coating material 1042, such as perfluorocarbon chemical(s). The liquid coating 1042 may shrink into tiny droplets 1052 on certain surface pockets (e.g., dents, concave defects and the like) of the core 1032, as seen in FIG. 10b.

[0074] In a further exemplary embodiment, as depicted in FIGS. 11a, 11b, a nanoparticle core 1132 of evaporating material such as perfluorocarbon chemical(s) may be covered by optically absorbing material 1142 such as nano-spheres, nano-rods, etc. Alternatively, the optically absorbing material 1142 may be embedded inside the core 1132 of evaporating material, as seen in FIG. 11b.

[0075] It is noted that attachment of absorbing particles to evaporating droplets can be achieved based on various chemical and/or physical interactions, e.g., based on chemical affinity, molecular or biological conjugation, etc. For example, particles can be bound by ligands that are embedded on the surface of droplets. With respect to this type of conjugation, use may be made of a specific technique which is based on an avidin-biotin adhesion, as this conjugation provides an extremely strong non-covalent interaction between a protein and a ligand, with an affinity of 10^{15} M^{-1} at pH 5. See Journal of Controlled Release, 2007.

[0076] With reference to multi-layer/bi-layer contrast agent embodiments, after phase change/evaporation is effected, a gas-filled nano-bubble or microbubble with a shell of optically transparent material is generally created. The size of the bubble-containing droplets may be on the order of 500 nm to 5000 nm, although the instant disclosure is not limited to these values. In an exemplary embodiment, the nano-bubbles or microbubbles may have a resonant frequency of about 5 to 15 MHz, although the present disclosure is not limited to these figures.

[0077] FIG. 12 shows an exemplary process 1200 of the novel, photoacoustic contrast agent based active ultrasound imaging. Parameters of the PA contrast agent 224 are tuned to allow conformance of the power spectrum 710 of bubble oscillation to the ultrasound transducer receive spectral sensitivity curve 720 (step S1210). The PA contrast agent 224 is mixed, in for instance a saline solution, with a microbubble-based ultrasound contrast agent 228 to facilitate detection of the inflow 208 into target vasculature 216. This event is indicative of the occurrence of permeation of the PA agent 224 outside the vasculature (step S1220). The ultrasound probe 120 and the laser 112, 116 are positioned for imaging the target region 252 (step S1230). The mixed contrast medium 212 is injected into the medical subject (step S1240). When the inflow 208 of the mixed contrast medium 212 is detected (step S1250), application of the electromagnetic, i.e., near-infrared laser, energy is commenced. (Laser activation of the PA contrast medium 224 may be performed at a body extremity of the subject, such as an arm or leg, rather than merely at the region 252 of interest to quantify vascular permeability. The laser need not be external, and may be introduced into the body by means of an intravascular applicator or from outside the vasculature.) Concurrent with the laser irradiation 204, ultrasound interrogation 220 of the target region 216 begins, to quantify vascular permeability for example. Low mechanical index (MI) imaging is at low power so that bubble destruction is avoided and non-linear imaging techniques can be used which are particularly sensi-

tive to the low acoustic returns from nano-bubble and microbubble oscillation. Among the low MI, multiple pulse processing techniques usable for ultrasound interrogation 204, in accordance with the instant proposal, is pulse inversion (PI) imaging. This method is described in commonly-assigned U.S. Pat. No. 5,706,819 entitled "Ultrasonic Diagnostic Imaging with Harmonic Contrast Agents," to Hwang et al., hereinafter referred to as the "819 patent." PI imaging avoids the problem of segmenting the fundamental component of bubble echoes 260 from a harmonic when the fundamental and harmonic overlap. It also alleviates the need for a bandwidth-limited filter. U.S. Pat. No. 6,095,980, entitled "Pulse Inversion Doppler Ultrasonic Diagnostic Imaging," to Burns et al. focuses on accounting for tissue motion in PI imaging, and further discusses the alternative non-linear methods of power modulation (PM) imaging and contrast pulse sequence (CPS) imaging. The latter method is more fully described in U.S. Pat. No. 6,494,841, entitled "Medical Diagnostic Ultrasound System Using Contrast Pulse Sequence Imaging," to Thomas et al. An approach to PI imaging that reduces artifacts and improves sensitivity is found in commonly-owned U.S. Pat. No. 6,508,767, entitled "Ultrasonic Harmonic Image Segmentation," to Burns et al. All of these non-linear techniques emit ultrasound interrogation pulses 264 in a common direction and coherently combine the echoed back data 260. As seen in FIG. 2, the interrogation pulses 264 are on paths that are either coincident, or adjacent and parallel. Adding or subtracting linear combinations of echoed back data 220 from different emitted pulses 264 is an example of coherent combining. The non-linear imaging method is supplemented with persistence processing, which has the effect of delaying a change in a real-time image. The fast attack, slow decay persistence technique is discussed in the "819 patent" (step S1260). As a result of the ultrasound interrogation 220 and response 260 processed by a non-linear, low MI imaging technique, vascular wall permeability can be quantified (step S1270). At this point, or any time after step S1240, molecular imaging or diagnostics are afforded by virtue of the small size of pre-activated nanoparticles 232 and consequent ability to diffuse through vascular walls and tissue, and by virtue of the ability to conjugate targeting molecules to the nanoparticles (step S1280). Targeted molecular imaging and diagnostics are available, for example, in HerII selectively targeting of breast cancer, see the "090 publication," $\alpha_v\beta_3$ selectively targeting of endothelium inflammation associated with cardiovascular diseases and rheumatoid arthritis, see U.S. Pat. No. 6,548,046, entitled "Site Specific Binding System, Imaging Compositions and Method," to Lanza et al., and heat shock protein targeting of endothelium transduction, see U.S. Pat. No. 7,575,738, entitled "Heat Shock Protein as a Targeting Agent for Endothelium-Specific In Vivo Transduction," to Syud et al. All of the patents cited above in this paragraph are incorporated herein by reference in their entirety.

[0078] Electromagnetic energy is applied to thereby oscillate a bubble that is then insonified to produce an echo for reception and analysis to afford imaging of the region of the bubble. To create the bubble, the energy may be applied to a particle of a contrast agent whose consequent internal nano- or micro-bubbles offer, with novel pulsing techniques, greater sensitivity, and which can permeate outside vasculature prior to being energized thereby affording quantification of vascular permeability and delivery of targeting molecules. The particle can include an absorbing and an evaporating parts,

the irradiation, as by near-infrared laser, causing the phase change that gives rise to the bubble. The echo may occur in response to ultrasound interrogation of the activated contrast agent, which could entail pulse inversion, power modulation or contrast pulse sequence imaging, with persistence processing. The contrast agent might be mixed with microbubble based ultrasound contrast agent to facilitate the timing of bubble activation.

[0079] It should be noted that the above-mentioned embodiments illustrate rather than limit the invention, and that those skilled in the art will be able to design many alternative embodiments without departing from the scope of the appended claims. For example, as an alternative to mixing the novel PA contrast agent with microbubble based ultrasound contrast agent to aid detection of inflow into vasculature, the inflow timing might be gauged based on empirical data. In the claims, any reference signs placed between parentheses shall not be construed as limiting the claim. Use of the verb "to comprise" and its conjugations does not exclude the presence of elements or steps other than those stated in a claim. The article "a" or "an" preceding an element does not exclude the presence of a plurality of such elements. The invention may be implemented by means of hardware comprising several distinct elements, and by means of a suitably programmed computer having a computer readable storage medium and/or by means of an integrated circuit having a machine-accessible storage medium. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage.

1. A photoacoustic contrast agent based active ultrasound imaging method, comprising:

applying pulsed electromagnetic energy to a nanoparticle-based photoacoustic contrast medium that comprises nanoparticles located in a region (i) to cause a phase change in an evaporation part of the nanoparticles that results in bubbles and (ii) to further produce oscillating bubbles, due to an ongoing on and off energy absorption of an absorbing part of the nanoparticles in response to the pulsed electromagnetic energy, that resonate at a frequency of 10 MHz detectable by an interrogating ultrasound; and

insonifying the oscillating bubbles to produce echoes for reception and analysis to afford active ultrasound imaging of said region.

2. (canceled)

3. The method of claim 1, wherein said particle comprises an elastic coating.

4. (canceled)

5. The method of claim 1, wherein the contrast medium further comprises an ultrasound contrast medium, wherein the nanoparticles are small enough to pass through a vascular wall, and wherein bubbles are created in respective ones of said nanoparticles.

6. The method of claim 1, wherein said insonifying is performed with low mechanical index.

7. The method of claim 6, wherein said applying being commenced, and said imaging being performed, at a time at which a portion of inflow of the plural bubbles into vasculature of the region has permeated outside said vasculature.

8. The method of claim 7, wherein said imaging at said time being performed with persistence processing.

9. The method of claim 1, wherein said insonifying being performed according to pulse inversion imaging.

10. The method of claim 1, wherein said insonifying being performed according to power modulation imaging.

11. The method of claim 1, wherein said insonifying being performed according to contrast pulse sequence imaging.

12. The method of claim 1, further comprising tuning parameters of the contrast medium to allow conformance of a power spectrum of bubble oscillation to an ultrasound transducer receive spectral sensitivity curve.

13. The method of claim 1, further comprising:
detecting inflow of microbubbles of a microbubble-based ultrasound contrast agent into vasculature of the region, said applying being commenced responsive to said detecting.

14. The method of claim 1, further comprising:
receiving the echoes; and
analyzing the received echoes to afford said active ultrasound imaging.

15. The method of claim 14, wherein said insonifying comprises firing a plurality of ultrasound pulses in a common direction, and said analyzing comprises coherently combining data echoed back from the plural pulses.

16. The method of claim 14, wherein said insonifying produces a plurality of echoes that are received, said plurality including said echoes and said analyzing comprises combining signals based on the plural echoes and analyzing the combined signals.

17. A photoacoustic contrast agent based active ultrasonic device comprising:

a transmission activator configured for delivering pulsed electromagnetic energy to excite a nanoparticle-based photoacoustic contrast substance that comprises nanoparticles located in a region so as to enhance utility of said substance as an ultrasound contrast agent (i) to cause a phase change in an evaporation part of the nanoparticles that results in bubbles and (ii) to further produce oscillating bubbles, due to an ongoing on and off energy absorption of an absorbing part of the nanoparticles in response to the pulsed electromagnetic energy, that resonate at a frequency of 10 MHz detectable by an interrogating ultrasound, and for delivering, to the excited substance of oscillating bubbles, ultrasound to produce echoes for reception and analysis to afford active ultrasound imaging of said region.

18. The device of claim 17, wherein said delivering electromagnetic energy comprises issuing separate bursts of electromagnetic pulses that propagate to said region and, in accordance with a tunable parameter of said substance, match a frequency of consequent energy absorption by said substance to a target frequency of bubble oscillation in said region by said energy.

19. The device of claim 17, wherein said applying pulsed electromagnetic energy expands said nanoparticles into particles that include bubbles oscillated by said energy, said bubbles serving interrogation targets for said active ultrasound imaging.

20. The device of claim 17, further comprising an ultrasound transducer with a spectral sensitivity curve, the exciting being such as would cause by itself, without the delivered ultrasound, emission of an acoustic signal whose power spectrum is overlapped, area-wise, by said curve by more than half.

21. A computer software product for medical analysis, said product comprising a non-transitory computer readable storage medium embodying a computer program that includes

instructions executable by a processor to perform a plurality of acts, said plurality comprising the acts of:

applying pulsed electromagnetic energy to a nanoparticle-based photoacoustic contrast medium that comprises nanoparticles located in a region (i) to cause a phase change in an evaporation part of the nanoparticles that results in bubbles and (ii) to further produce oscillating bubbles, due to an ongoing on and off energy absorption of an absorbing part of the nanoparticles in response to the pulsed electromagnetic energy, that resonate at a frequency of 10 MHz detectable by an interrogating ultrasound; and

insonifying the oscillating bubbles to produce echoes for reception and analysis to afford active ultrasound imaging of said region.

22. An article of manufacture, comprising a non-transitory machine-accessible storage medium having instructions

encoded thereon for enabling a processor to perform medical analysis by executing acts, including:

applying pulsed electromagnetic energy to a nanoparticle-based photoacoustic contrast medium that comprises nanoparticles located in a region (i) to cause a phase change in an evaporation part of the nanoparticles that results in bubbles and (ii) to further produce oscillating bubbles, due to an ongoing on and off energy absorption of an absorbing part of the nanoparticles in response to the pulsed electromagnetic energy, that resonate at a frequency of 10 MHz detectable by an interrogating ultrasound; and

insonifying the oscillating bubbles to produce echoes for reception and analysis to afford active ultrasound imaging of said region.

23. (canceled)

* * * * *

专利名称(译)	基于光声造影剂的主动超声成像		
公开(公告)号	US20120203103A1	公开(公告)日	2012-08-09
申请号	US13/501683	申请日	2010-10-11
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦电子N.V.		
当前申请(专利权)人(译)	皇家飞利浦电子N.V.		
[标]发明人	WANG YAO SHI WILLIAM TAO		
发明人	WANG, YAO SHI, WILLIAM TAO		
IPC分类号	A61B8/14		
CPC分类号	A61B8/481 A61B5/0095		
优先权	61/252214 2009-10-16 US		
其他公开文献	US9037218		
外部链接	Espacenet USPTO		

摘要(译)

施加电磁能从而振荡气泡，然后气泡被声穿透以产生用于接收和分析的回波（260），以提供气泡区域的成像。为了产生气泡，可以将能量施加到造影剂的纳米颗粒（232）上，所述造影剂随后产生内部纳米或微气泡，具有新颖的脉冲技术，更高的灵敏度，并且可以在之前渗透到脉管系统外部（216）。通电，从而提供血管通透性的定量和靶向分子的递送。颗粒可以包括吸收和蒸发部分，照射（204），如通过近红外激光，引起产生气泡的相变。回波可以响应于激活的造影剂的超声询问（220）而发生，其可能需要脉冲反转，功率调制或对比脉冲序列成像，具有持久性处理。造影剂可以与基于微泡的超声造影剂混合以促进气泡活化的时间。

