



US006488627B1

(12) **United States Patent**  
**Kim**

(10) **Patent No.:** **US 6,488,627 B1**  
(45) **Date of Patent:** **Dec. 3, 2002**

(54) **ULTRASONIC IMAGE SEARCHING APPARATUS AND ULTRASONIC IMAGE TRANSMISSION AND RECEPTION SYSTEM ADOPTING THE SAME**

5,997,478 A \* 12/1999 Jackson et al. .... 600/437  
6,032,678 A \* 3/2000 Rottem ..... 600/437  
2001/0043729 A1 \* 11/2001 Giger et al. .... 382/128

\* cited by examiner

(75) Inventor: **Sang Hyun Kim**, Seoul (KR)

*Primary Examiner*—Francis J. Jaworski

(73) Assignee: **Medison Co., Ltd.** (KR)

(74) *Attorney, Agent, or Firm*—Bourque & Associates P.A.

(\*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(57) **ABSTRACT**

An ultrasonic image searching apparatus is provided, which includes an input unit for inputting a key word for selecting an object to be searched and an ultrasonic image, a feature extraction unit for extracting the feature of the ultrasonic image inputted via the input unit, a storage unit for storing a plurality of previously acquired ultrasonic images and a database of commentary information and image feature information with respect to each ultrasonic image, a display, and a controller for comparing the key word input from the input unit or the feature extracted from the feature extraction unit with the commentary information and the image feature information in the storage unit and outputting the ultrasonic images contained in the storage unit on the display according to a degree of similarity. Thus, a massive amount of the prestored ultrasonic images can be efficiently searched, and connection with the network such as a web server provides an effect of searching the ultrasonic image.

(21) Appl. No.: **09/621,924**

(22) Filed: **Jul. 24, 2000**

(30) **Foreign Application Priority Data**

Nov. 26, 1999 (KR) ..... 99-52913

(51) **Int. Cl.**<sup>7</sup> ..... **A61B 8/00**

(52) **U.S. Cl.** ..... **600/437**

(58) **Field of Search** ..... 600/437, 443;  
382/128; 709/217-219, 230; 707/316

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,899,999 A \* 5/1999 De Bonet ..... 600/443

**18 Claims, 3 Drawing Sheets**

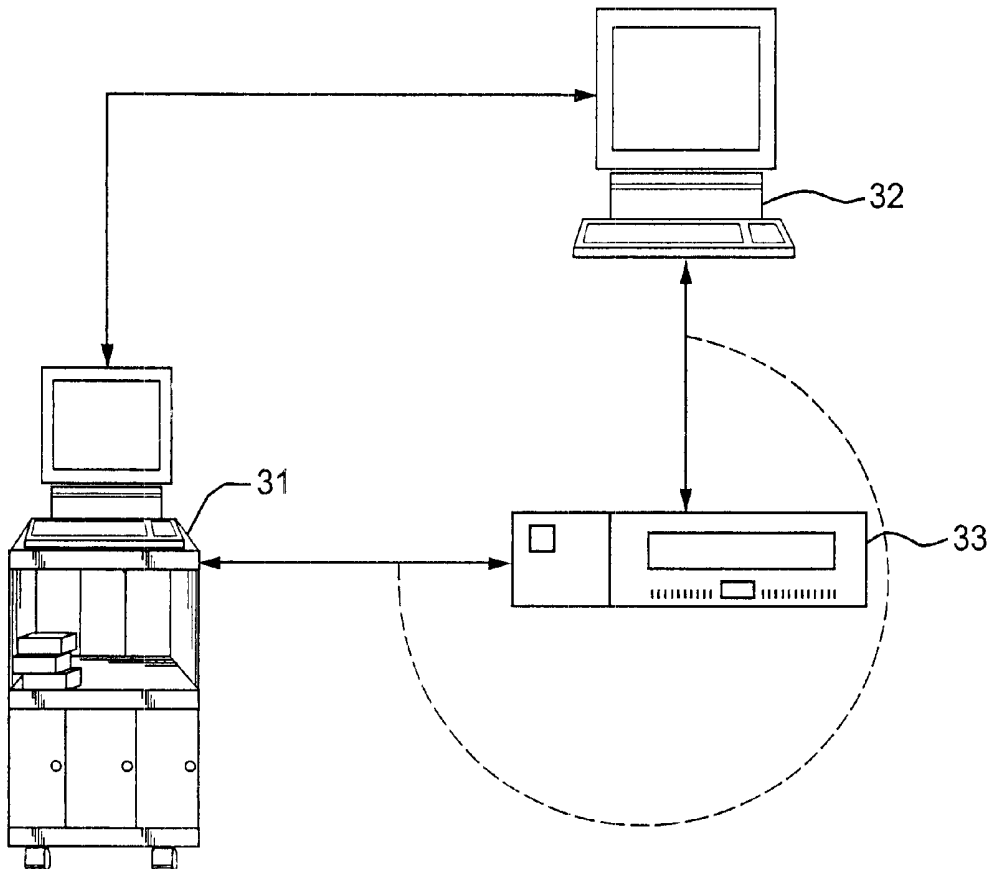


FIG. 1

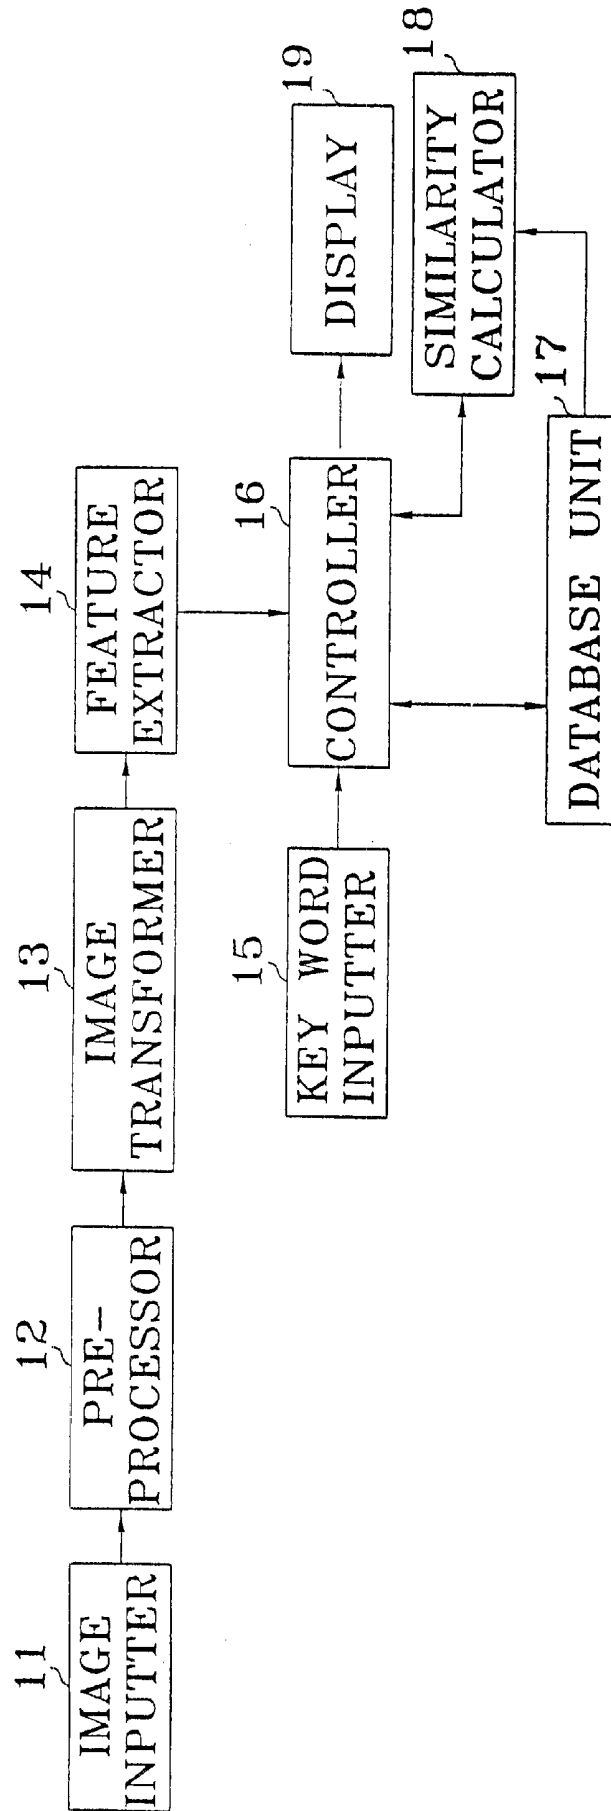
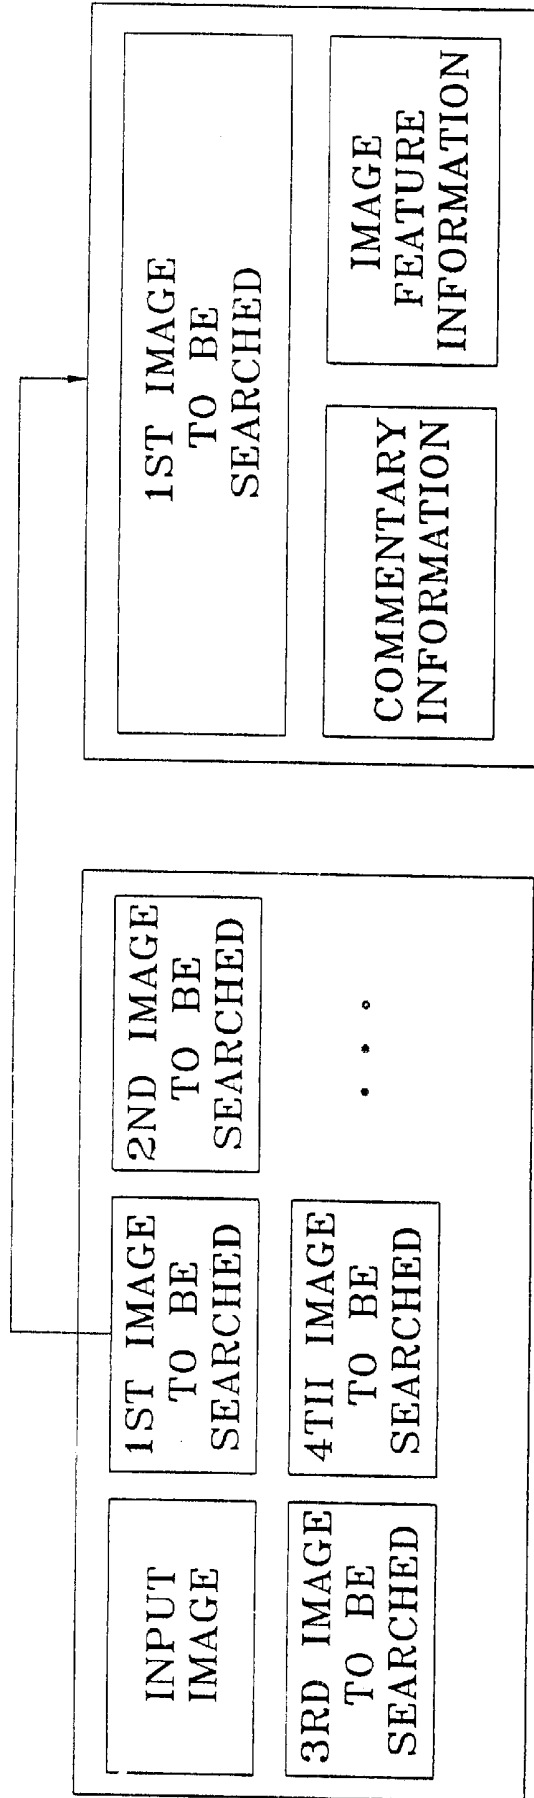


FIG. 2



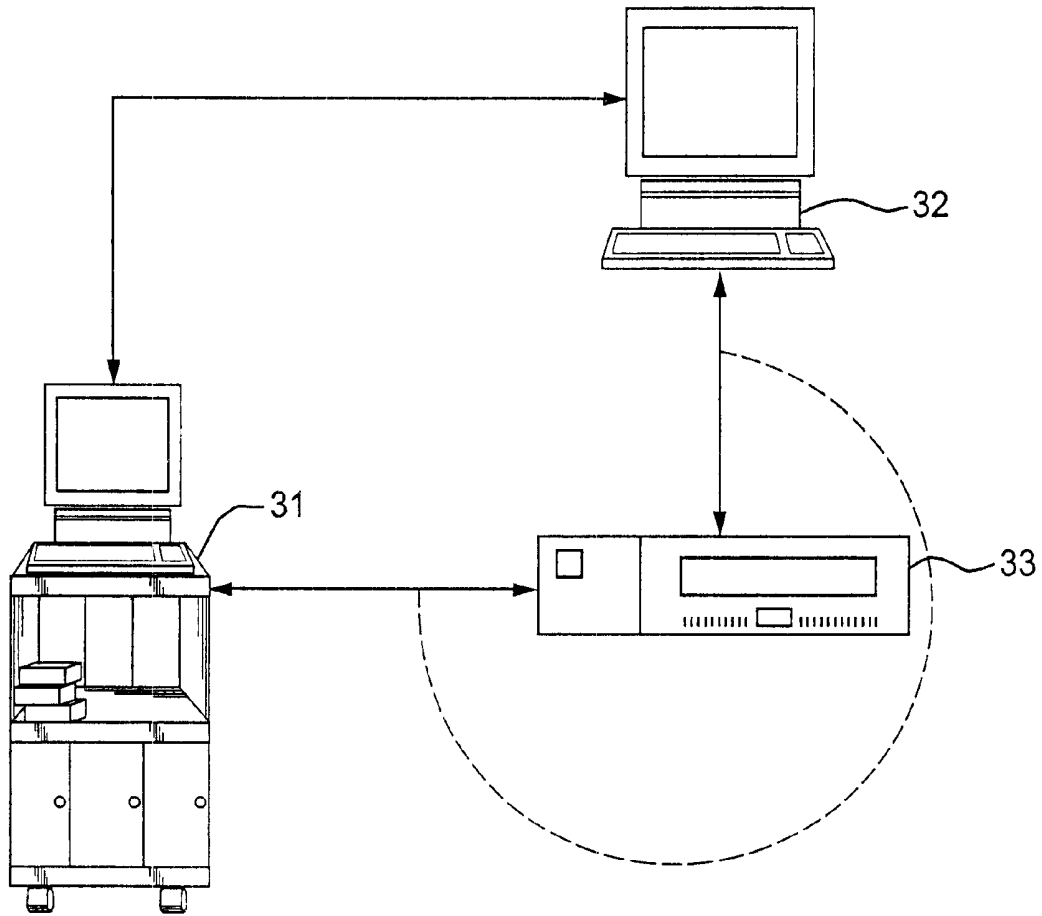


FIG. 3

**ULTRASONIC IMAGE SEARCHING  
APPARATUS AND ULTRASONIC IMAGE  
TRANSMISSION AND RECEPTION SYSTEM  
ADOPTING THE SAME**

**BACKGROUND OF THE INVENTION**

1. Field of the Invention

The present invention relates to an ultrasonic image diagnostic system, and more particularly, to an ultrasonic image searching apparatus and an ultrasonic image transmission and reception system adopting the same, in which an ultrasonic image to be desired by a user is searched among ultrasonic images prestored in an ultrasonic image diagnostic system, and the searched results are displayed in order similar to the desired ultrasonic image.

2. Description of the Related Art

According to development of the electronic engineering field, a number of changes have occurred in an ultrasonic image technological field. Among them, a representative one is to process and store images in digital form. Thus, since ultrasonic images are processed digitally, the ultrasonic diagnostic system can process and store an enormous amount of ultrasonic images. A research for searching a desired image among the enormous amount of the stored ultrasonic images is briskly under progress. In particular, in the MPEG (Moving Pictures Expert Group) standard for a moving image compression method, an image searching method for searching a particular image among successive frames is being under studied. Also, in the medical imaging field, a method for searching an image using a frequency conversion method with respect to MRI images, is being researched.

However, most of the existing image searching methods of which the objects are general images in the world of nature, are applied chiefly to personal computers. The existing image searching methods have been applied only to the case where directionality of images is fixed at the time of searching medical images. Thus, there has been no ultrasonic image searching system which is applicable to the ultrasonic image diagnostic system where position of a probe is adjusted to obtain an ultrasonic image.

**SUMMARY OF THE INVENTION**

To solve the above problems, it is an object of the present invention to provide an ultrasonic image searching apparatus for effectively searching an ultrasonic image.

It is another object of the present invention to provide an ultrasonic image transmission and reception system for searching an ultrasonic image including an ultrasonic image searching apparatus which is connected to a network such as a web server.

To accomplish the above object of the present invention, there is provided an ultrasonic image searching apparatus comprising: an input unit for inputting a key word and an ultrasonic image for selecting an object to be searched; a feature extraction unit for extracting the feature of the ultrasonic image inputted via the input unit; a storage unit for storing a plurality of previously acquired ultrasonic images and a database of commentary information and image feature information with respect to each ultrasonic image; a display; and a controller for comparing the key word input from the input unit or the feature extracted from the feature extraction unit with the commentary information and the image feature information in the storage unit and

outputting the ultrasonic images contained in the storage unit on the display according to a degree of similarity.

There is also provided an ultrasonic image transmission and reception system according to the present invention, comprising: a requester for requesting an ultrasonic image to be searched; and a provider connected to the requester on a network, for constructing a separate database storing ultrasonic images, searching an ultrasonic image which has been requested from the requester, and providing the searched result.

**BRIEF DESCRIPTION OF THE DRAWINGS**

The above objects and other advantages of the present invention will become more apparent by describing the preferred embodiments thereof in more detail with reference to the accompanying drawings in which:

FIG. 1 is a block diagram showing an ultrasonic image searching apparatus according to an embodiment of the present invention;

FIG. 2 shows an exemplary screen state illustrating the ultrasonic image searching results of the FIG. 1 apparatus; and

FIG. 3 shows an application on the web Internet in which the ultrasonic image searching apparatus of FIG. 1 is connected to a personal computer (PC).

**DETAILED DESCRIPTION OF THE  
PREFERRED EMBODIMENTS**

A preferred embodiment of the present invention will be described with reference to the accompanying drawings.

Referring to FIG. 1, an ultrasonic image searching apparatus according to an embodiment of the present invention includes an image inputter **11** for inputting an ultrasonic image and a key word inputter **15** for inputting a key word. Also, the FIG. 1 apparatus includes a pre-processor **12** for pre-processing the ultrasonic image input from the image inputter **11**, an image transformer **13** for image-transforming the pre-processed ultrasonic image, and a feature extractor **14** for extracting the features of the image-transformed ultrasonic image. A controller **16** connected to the output end of the feature extractor **14** is connected to the key word inputter **15** to receive the input key word. Here, the key word can be in the form of both characters and sounds. Hereinafter, characters are input as key words, by way of an example. Also, the controller **16** is connected to a database unit **17** and a similarity calculator **18** in order to transmit and receive signals mutually, and is connected to a display **19** in order to display the images thereon.

The operation of the FIG. 1 ultrasonic image searching apparatus having the above configuration will be described with reference to FIG. 2.

In FIG. 1, a user inputs an image or a key word, to thereby search a desired ultrasonic image. That is, the user inputs characters via the key matrix of the key word inputter **15**, or inputs the ultrasonic image via the image inputter **11**, to thereby search a desired image. In order to search a desired ultrasonic image from the input image or the key word, the database unit **17** stores commentary information and image feature information which are image information corresponding to each ultrasonic image, as well as pre-stored ultrasonic images. Here, the commentary information is for searching an image in the case that a user inputs a key word. Also, the image feature information is for searching an image in the case that a user inputs an image, that is, statistical information such as signal distribution of images or a histogram of frequency components.

The two cases for inputting characters or images in order to search a user desired ultrasonic image will be described in more detail.

First, in the case of image searching according to character inputs, a user inputs a key word using the key matrix of the key word inputter **15**. When a key word signal for image searching is input to the controller **16**, the controller **16** outputs the key word signal to the similarity calculator **18**. Also, the controller **16** controls image information corresponding to the pre-stored ultrasonic image of the database unit **17** to be output to the similarity calculator **18**. The similarity calculator **18** compares the key word signal input from the controller **16** with the commentary information among the image information output from the database unit **17**, to thereby output a degree of similarity to the controller **16**. The controller **16** reads out the ultrasonic image having a degree of similarity input from the similarity calculator **18** from the database unit **17**. The controller **16** outputs the ultrasonic images read out from the database unit **17** in order of a higher degree of similarity. The display **19** displays the image signal input from the controller **16** thereon as shown in FIG. 2. That is, the searched images are output in order of a higher degree of similarity. In the case that a first searched image is selected, the corresponding image is displayed together with the commentary information and the image feature information.

Secondly, in the case that image searching is performed using an ultrasonic image, the user inputs the ultrasonic image which is currently ultrasonic-scanned using a probe. The image inputter **11** outputs the ultrasonic image signal from the probe to the pre-processor **12**. The pre-processor **12** makes the brightness and the contrast of the ultrasonic image from the image inputter **11** equal to those of the ultrasonic image prestored in the database unit **17**, and performs pre-processing operations such as noise cancellation of the ultrasonic image signal and sorting of the significant portions in the ultrasonic image. The image transformer **13** receives the pre-processed ultrasonic image signal from the pre-processor **12**, and image-transforms it so that feature extraction of the ultrasonic image signal is facilitated. That is, the image transformer **13** transforms the pre-processed ultrasonic image from a spatial region to a frequency region, and classifies the frequency components contained in the ultrasonic image systematically to then output the result. Here, the image transforming method can employ a Wavelet transform, a discrete cosine transform (DCT), and so on. The feature extractor **14** extracts the features of the ultrasonic image from the image transformed ultrasonic image signal input from the image transformer **13**. That is, the feature extractor **14** receives the frequency components output from the image transformer **13** and makes them into a histogram to extract the features. Besides, features can be extracted using signal distribution and pattern and motion vector information in the transform region and spatial region. The feature extractor **14** outputs the histogram information of the frequency components in the ultrasonic image signal to the controller **16**. The controller **16** receives the histogram information and outputs it to the similarity calculator **18**. Also, the controller **16** controls the image information of the prestored ultrasonic images in the database unit **17** so as to be output to the similarity calculator **18**. The similarity calculator **18** compares the histogram information input from the controller **16** with that of the prestored ultrasonic images in the database unit **17** and outputs the obtained similarity to the controller **16**. The controller **16** reads out from the database unit **17** the ultrasonic images having the similarity output from the similarity calculator **18**. The

controller **16** outputs the ultrasonic images read out from the database unit **17** in order of a higher similarity. The display **19** displays the image signal input from the controller **16** on a screen as shown in FIG. 2. Here, in the case that diagnostic information is stored together in the database unit **17**, the diagnostic information can be also displayed on the screen together with a plurality of searched resultant image. That is, the searched image is output in order of the higher similarity. When a first searched image is selected, the corresponding image is displayed together with the commentary information and the image feature information.

Also, the above-described ultrasonic image searching apparatus is independently used in the ultrasonic image diagnostic system, and connected on the web via the network, to thereby enable image searching, as well. These are shown in FIG. 3. In the FIG. 3 apparatus, a web server **33** is coupled to an ultrasonic image searching apparatus **31** and a PC **32**, to thus receive and transmit the data for searching an ultrasonic image and the searched resultant image, mutually. The web server **33** constructs a database prestoring the ultrasonic images to be searched. Thus, the web server **33** receives a request of a desired ultrasonic image from the ultrasonic image searching apparatus **31** and the PC **32**, and finds out the requested ultrasonic image among the prestored ultrasonic images, to then transmit the searched result in order of similarity. Also, the present invention enables an ultrasonic image searching among a plurality of ultrasonic image searching apparatuses which are connected to the Internet or Intranet. Further, a PC is connected to a plurality of ultrasonic image searching apparatuses, to thereby enable an ultrasonic image requested by the PC to be searched in the plurality of ultrasonic image searching apparatuses to then be transmitted.

In the above-described embodiment, the image transformer **13** has been used for extracting the features through an image transformation in order to extract the features of the ultrasonic image. As another embodiment of the present invention, the image transformer **13** can be replaced by an image emphasize (not shown), to perform the same function. Referring to FIG. 1, the image emphasize (not shown) is coupled between the pre-processor **12** and the feature extractor **14**, instead of the image transformer **13**. The image emphasize (not shown) receives the pre-processed ultrasonic image from the pre-processor **12**, and emphasizes the feature of the image in the spatial region via image division or contour extraction, to then output the emphasized ultrasonic image. Then, the feature extractor **14** receives the image emphasized ultrasonic image from the image emphasize and extracts the feature of the ultrasonic image. The image searching process is same as that of the FIG. 1 description.

The ultrasonic images applied to the above-described embodiments can be two-dimensional ultrasonic images, three-dimensional ultrasonic images, and four-dimensional ultrasonic images.

Also, the above-described embodiment has been described with respect to the cases that the key word is input and the ultrasonic image is input to select an object to be searched, respectively. However, the key word and the ultrasonic image can be simultaneously received, to thereby enable both the commentary information and the image feature information to be searched together, and combine two similarities to complementarily search the ultrasonic image. That is, sum of the similarity of the commentary information and that of the image feature information is used to search the ultrasonic image.

Thus, the present invention can efficiently search a massive amount of the prestored ultrasonic images, and provides

an effect of searching the ultrasonic image through connection with the network such as a web server.

What is claimed is:

- 1. An ultrasonic image searching apparatus comprising:
  - an input unit for inputting a key word and an ultrasonic image for selecting an object to be searched;
  - a feature extraction unit for extracting at least one feature of said ultrasonic image inputted via said input unit, said feature extraction unit comprising:
    - a pre-processor for manipulating at least one quality of said input ultrasonic image;
    - an image transformer connected to said pre-processor, said image transformer transforming said preprocessed ultrasonic image from a spatial region to a frequency region having frequency components and classifying said frequency components contained in said ultrasonic image; and
    - a feature extractor connected to said image transformer, said feature extractor receiving said frequency components and extracting said features of said ultrasonic image by creating a histogram;
    - a storage unit for storing a plurality of previously acquired ultrasonic images and a database of commentary information and image feature information with respect to each ultrasonic image;
    - a display; and
    - a controller for comparing said key word input from said input unit or said feature extracted from said feature extraction unit with said commentary information and said image feature information in said storage unit and outputting said ultrasonic images contained in said storage unit on said display according to degree of similarity.
- 2. The ultrasonic image searching apparatus according to claim 1, wherein said input unit comprises:
  - a key word inputter for inputting a key word of an image to be searched in the form of characters and sounds; and
  - an image inputter for inputting an ultrasonic image.
- 3. The ultrasonic image searching apparatus according to claim 1, wherein said feature extraction unit extracts image feature information in correspondence to that of the pre-stored ultrasonic image.
- 4. The ultrasonic image searching apparatus according to claim 3, wherein said controller compares the key word input with the commentary information, if the key word has been input from said inputter and compares the ultrasonic image with the image feature information if the ultrasonic image has been input therefrom, to thereby calculate a degree of similarity.
- 5. The ultrasonic image searching apparatus according to claim 6, wherein said controller comprises:
  - a similarity calculator for calculating a degree of similarity by comparing the input key word and ultrasonic image with the commentary information and the image feature information; and
  - a controller for controlling the ultrasonic images to be output in order of similarity input from said similarity calculator.
- 6. The ultrasonic image searching apparatus according to claim 3, wherein said controller compares the key word input from said inputter with the commentary information,

and compares the ultrasonic image with the image feature information respectively, to thereby calculate a degree of similarity based on the comparison results.

- 7. The ultrasonic image searching apparatus according to claim 6, wherein said controller comprises:
  - a similarity calculator for calculating a degree of similarity by comparing the input key word and ultrasonic image with the commentary information and the image feature information; and
  - a controller for controlling the ultrasonic images to be output in order of similarity input from said similarity calculator.
- 8. The ultrasonic image searching apparatus according to claim 1, wherein said feature extraction unit comprises:
  - a pre-processor for pre-processing the input ultrasonic image so as to be equal to the conditions of the ultrasonic images prestored in said storage unit;
  - an image emphasize for receiving the pre-processed ultrasonic image from said pre-processor and image-emphasizing the input pre-processed ultrasonic image; and
  - a feature extractor for extracting the feature of the ultrasonic image based on the image-emphasized ultrasonic image signal.
- 9. The ultrasonic image searching apparatus according to claim 1, wherein said controller for controlling an ultrasonic image selected among a plurality of ultrasonic images displayed on the display so as to be displayed together with the commentary information and the image feature information.
- 10. The ultrasonic searching apparatus according to claim 1, wherein said object to be searched is a two-dimensional, or four-dimensional ultrasonic image.
- 11. The ultrasonic image searching apparatus as claimed in claim 1 wherein said image transformer uses a Wavelet transform.
- 12. The ultrasonic image searching apparatus as claimed in claim 1 wherein said image transformer uses a discrete cosine transform.
- 13. The ultrasonic image searching apparatus as claimed in claim 1 wherein said feature extractor extracts said features using signal distribution and pattern and motion vector.
- 14. The ultrasonic image searching apparatus as claimed in claim 1 wherein said storage unit comprises a server.
- 15. The ultrasonic image searching apparatus as claimed in claim 1 wherein said storage unit comprises a personal computer.
- 16. The ultrasonic image searching apparatus as claimed in claim 1 wherein said storage unit comprises a plurality of ultrasonic image searching apparatuses.
- 17. The ultrasonic image searching apparatus as claimed in claim 1 wherein said pre-processor manipulates said at least one quality of said input ultrasonic image using noise cancellation techniques.
- 18. The ultrasonic image searching apparatus as claimed in claim 1 wherein said pre-processor manipulates said at least one quality of said input ultrasonic image to adjust the brightness and contrast of said input ultrasonic image to approximate the brightness and contrast of said plurality of previously acquired ultrasonic images.

专利名称(译)	超声波图像搜索装置和采用其的超声波图像发送和接收系统		
公开(公告)号	<a href="#">US6488627</a>	公开(公告)日	2002-12-03
申请号	US09/621924	申请日	2000-07-24
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	KIM SANG HYUN		
发明人	KIM, SANG HYUN		
IPC分类号	G06F17/30 A61B8/00 G06Q50/22 G06Q50/24 G06T1/00 G16H10/60		
CPC分类号	G06F17/30247 G06F17/30265 G06F19/321 G06F16/58 G06F16/583		
优先权	1019990052913 1999-11-26 KR		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

提供一种超声波图像检索装置，包括：输入单元，用于输入用于选择待搜索物体的关键词和超声波图像；特征提取单元，用于提取经由输入单元输入的超声波图像的特征，存储装置用于存储多个先前获取的超声图像的单元和关于每个超声图像的评论信息和图像特征信息的数据库，显示器和用于比较从输入单元输入的关键词或从特征提取的特征的控制器提取单元，其具有存储单元中的评论信息和图像特征信息，并根据相似度在显示器上输出包含在存储单元中的超声图像。因此，可以有效地搜索大量预先存储的超声图像，并且与诸如网络服务器的网络的连接提供了搜索超声图像的效果。

