



US 20190239856A1

(19) **United States**

(12) **Patent Application Publication**
LEE et al.

(10) **Pub. No.: US 2019/0239856 A1**
(43) **Pub. Date: Aug. 8, 2019**

(54) **ULTRASOUND DIAGNOSIS APPARATUS AND METHOD OF OPERATING SAME**

Publication Classification

(71) Applicant: **SAMSUNG MEDISON CO., LTD.**,
Hongcheon-gun (KR)

(51) **Int. Cl.**
A61B 8/08 (2006.01)
A61B 8/06 (2006.01)

(72) Inventors: **Jin-yong LEE**, Seongnam-si (KR);
Jong-sik KIM, Seongnam-si (KR)

(52) **U.S. Cl.**
CPC *A61B 8/5223* (2013.01); *A61B 8/488*
(2013.01); *A61B 8/0866* (2013.01); *A61B*
8/5246 (2013.01); *A61B 8/0883* (2013.01);
A61B 8/06 (2013.01)

(73) Assignee: **SAMSUNG MEDISON CO., LTD.**,
Hongcheon-gun (KR)

(57) **ABSTRACT**

(21) Appl. No.: **16/155,168**

Provided are an ultrasound diagnosis apparatus and a method of operating the same. The method includes: transmitting an ultrasound signal to the heart of the fetus and receiving an echo signal reflected from the heart; acquiring first Doppler data and second Doppler data respectively with respect to first and second setting ranges by using the echo signal; and displaying a first resulting image obtained based on the first Doppler data and the second Doppler data.

(22) Filed: **Oct. 9, 2018**

(30) **Foreign Application Priority Data**

Feb. 2, 2018 (KR) 10-2018-0013432

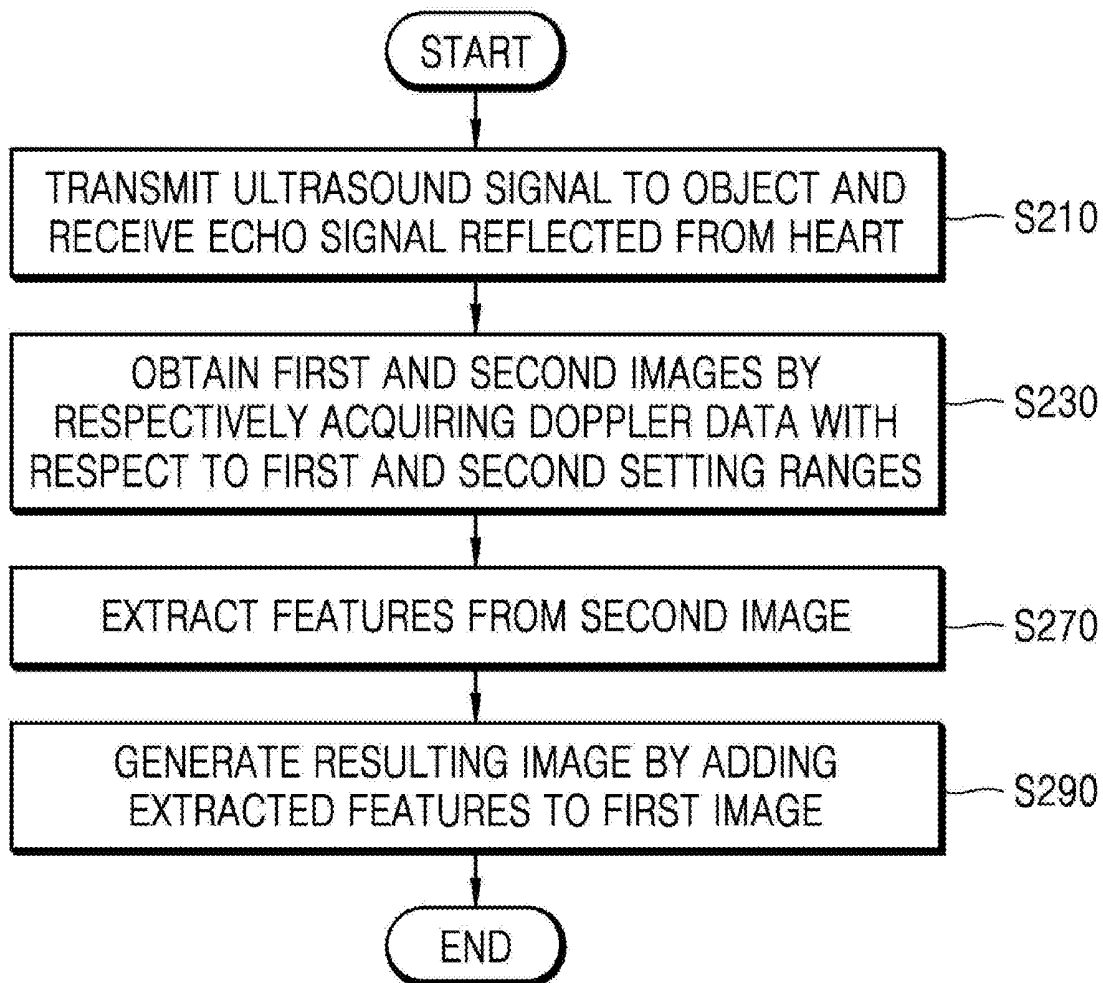


FIG. 1

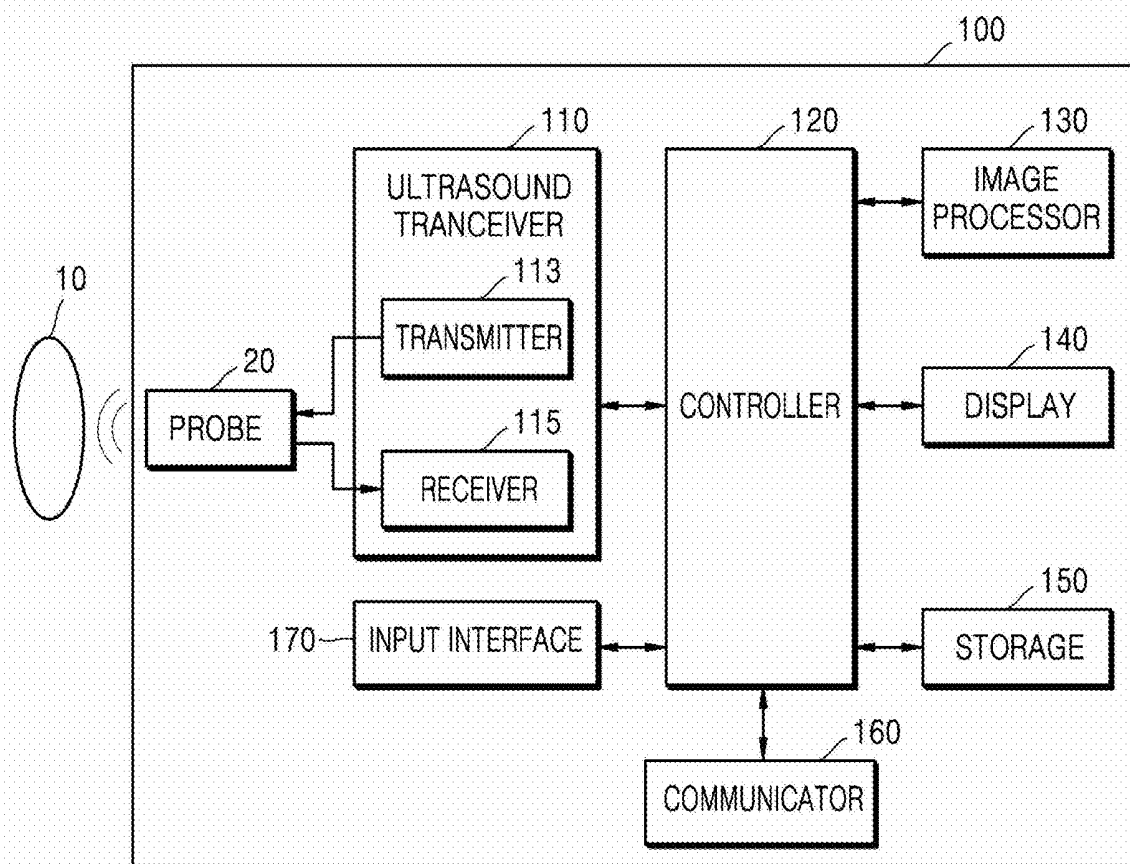


FIG. 2C

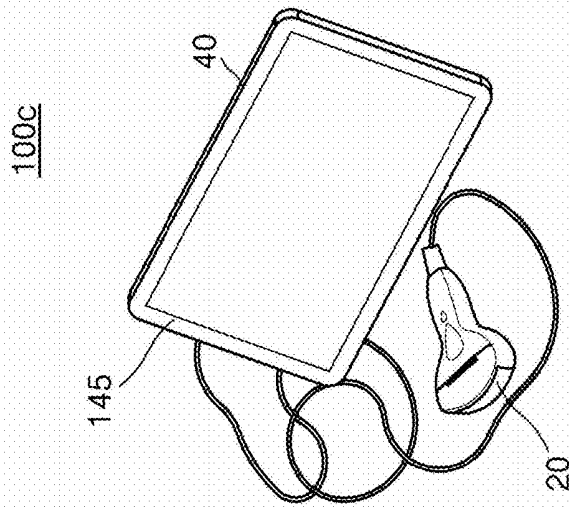


FIG. 2B

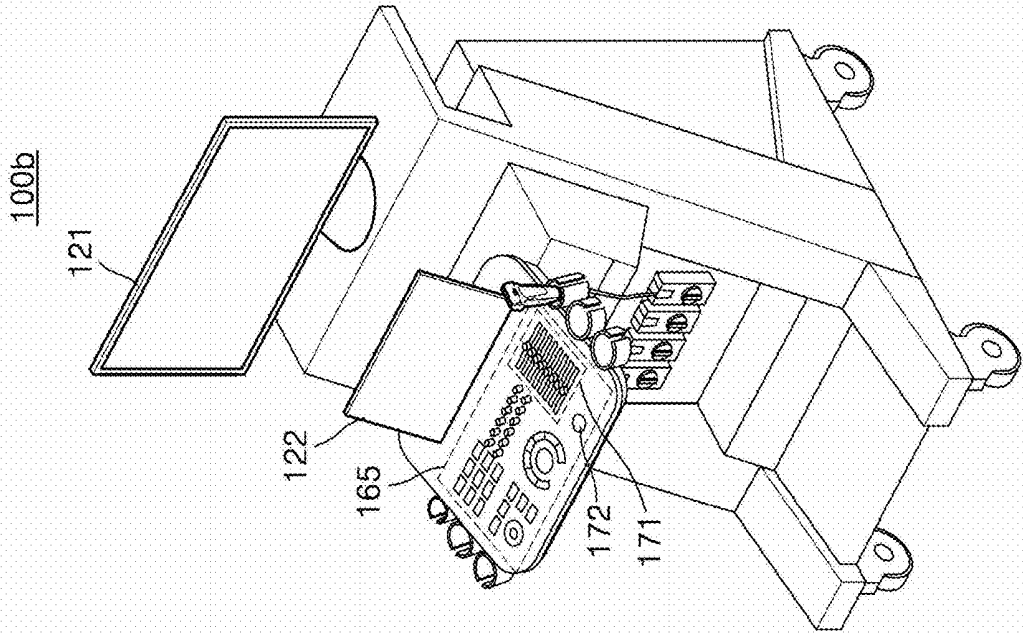


FIG. 2A

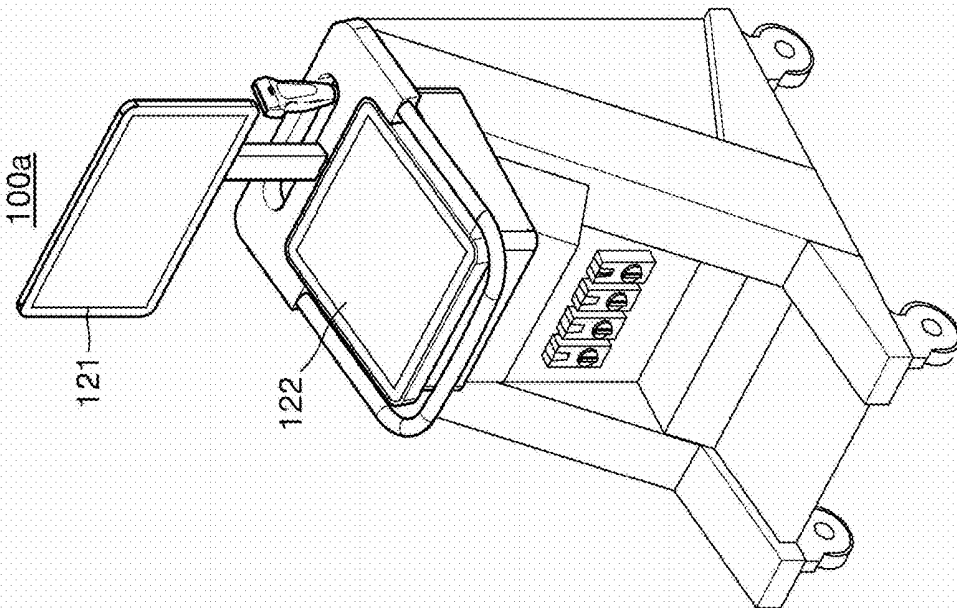


FIG. 3

300

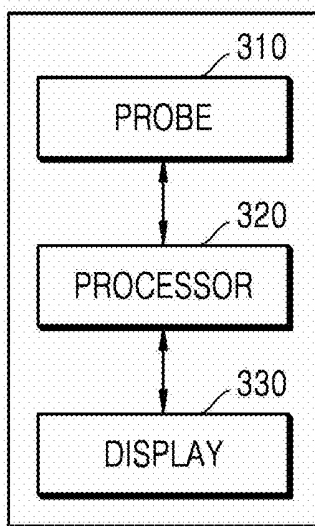


FIG. 4

400

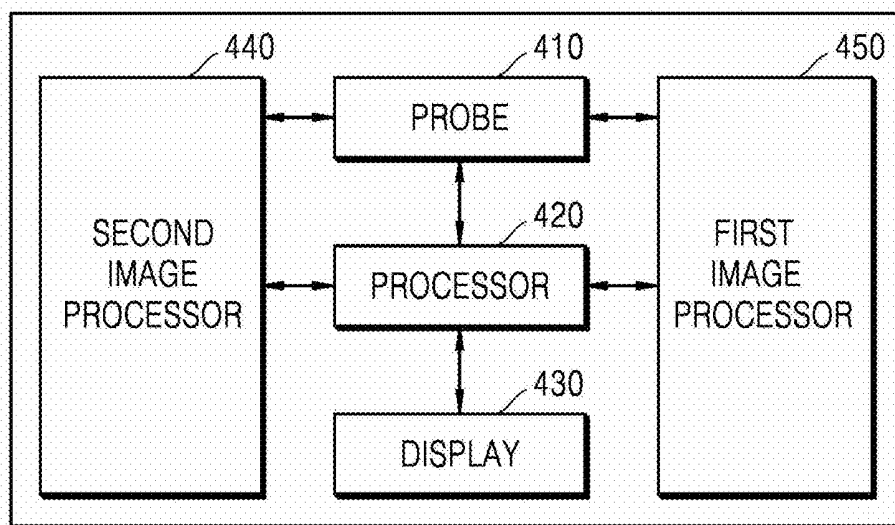


FIG. 5

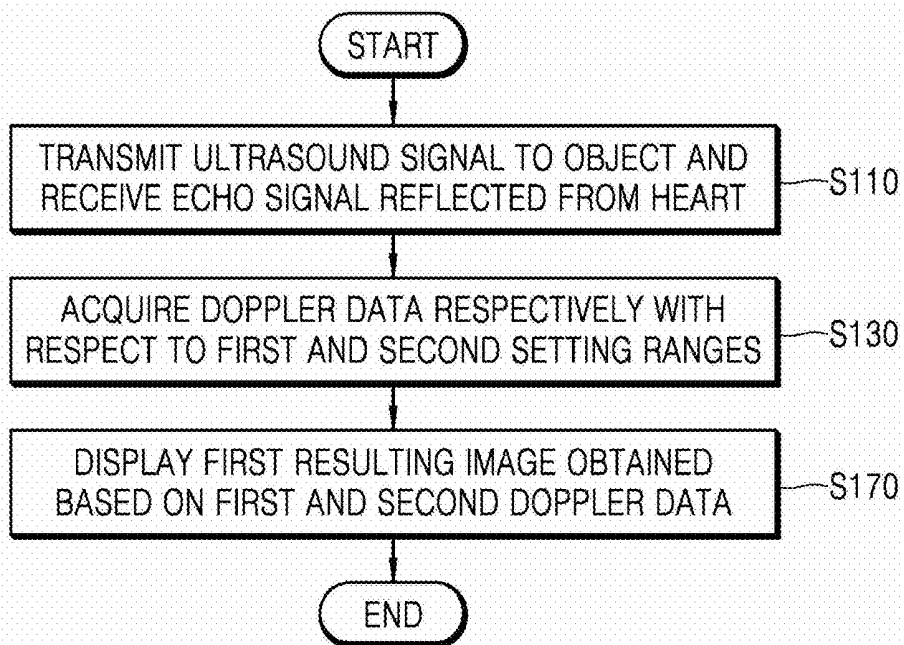


FIG. 6A

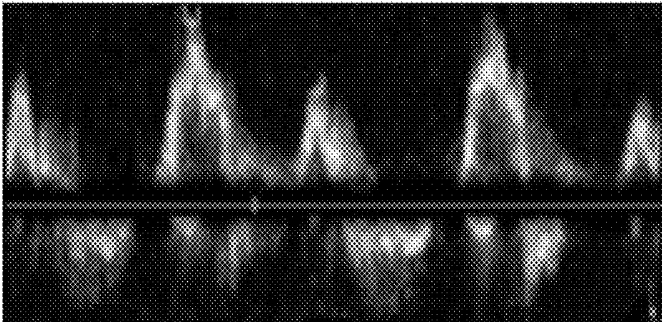


FIG. 6B

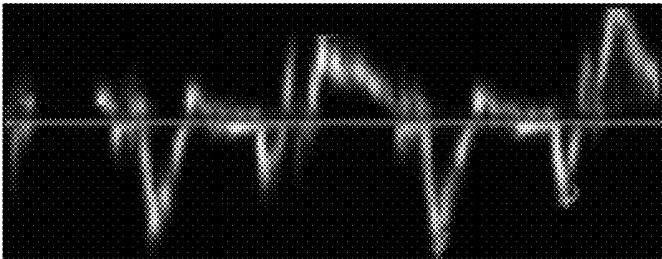


FIG. 7A

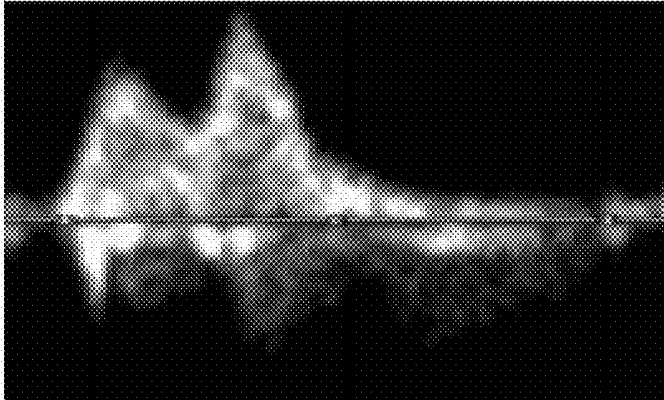


FIG. 7B

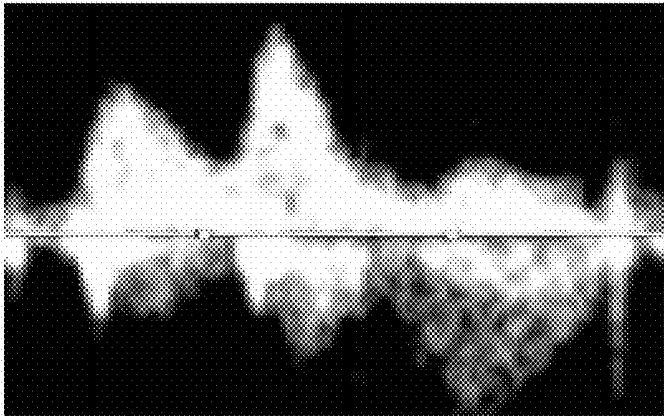


FIG. 8

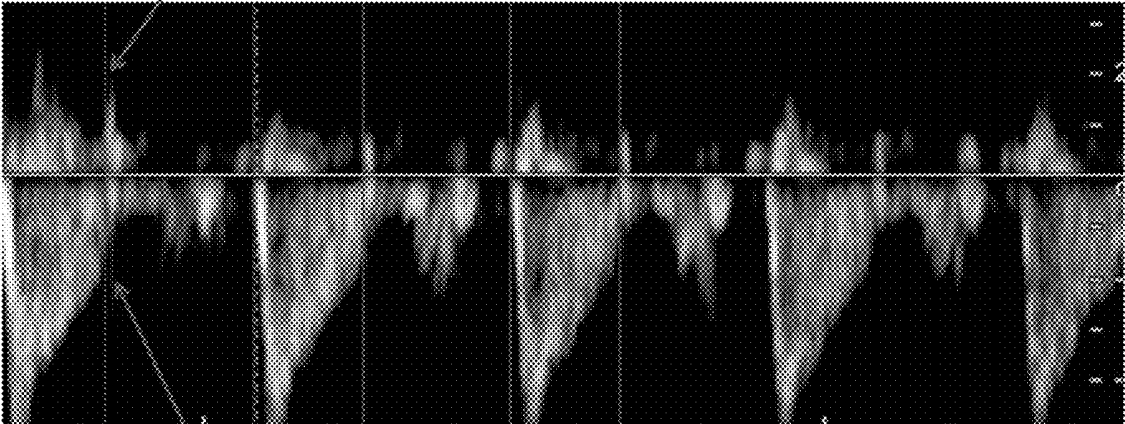


FIG. 9A

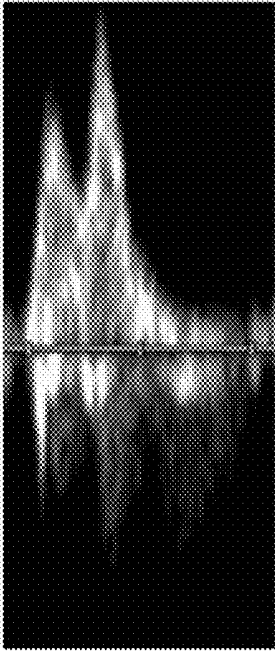


IMAGE 1

FIG. 9B


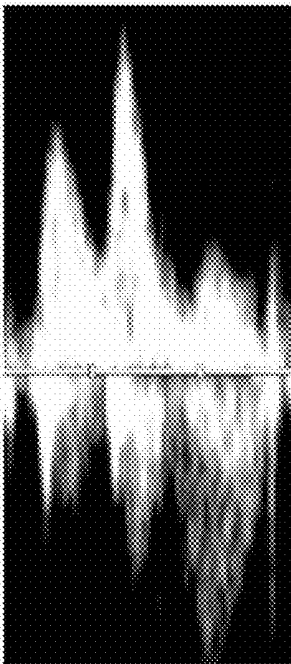


IMAGE 2

FIG. 9C

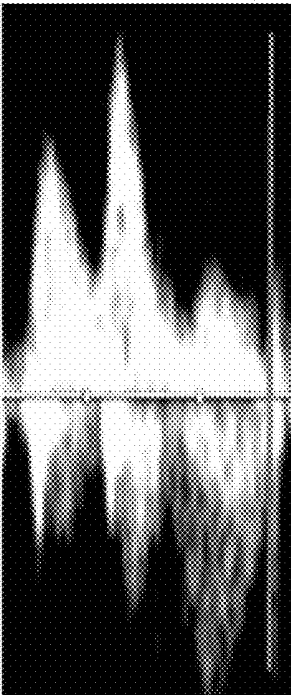

FEATURE EXTRACTION

FIG. 9D

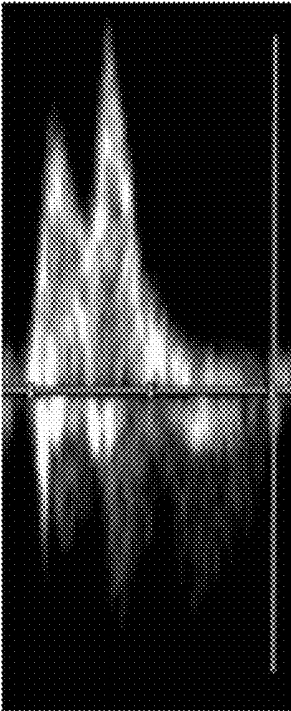


IMAGE REPRESENTATION

FIG. 10

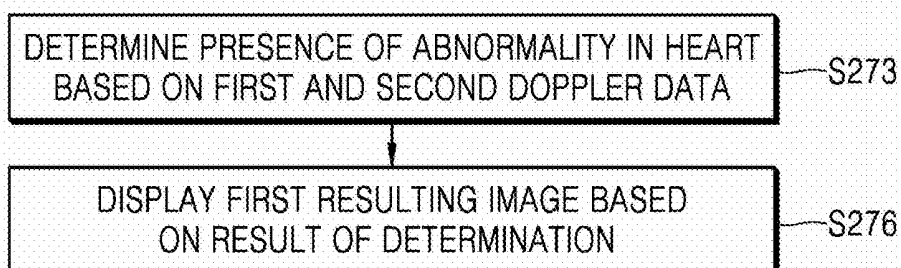


FIG. 11

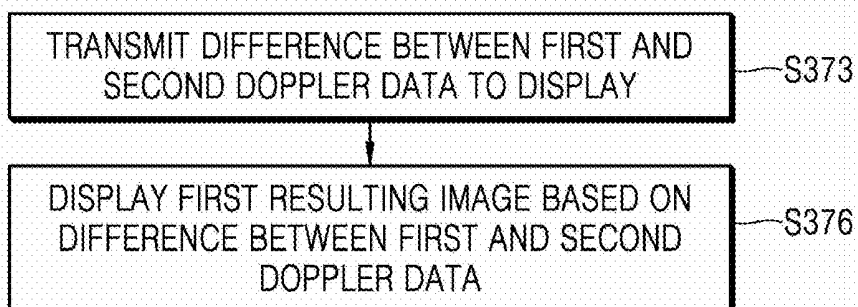


FIG. 12


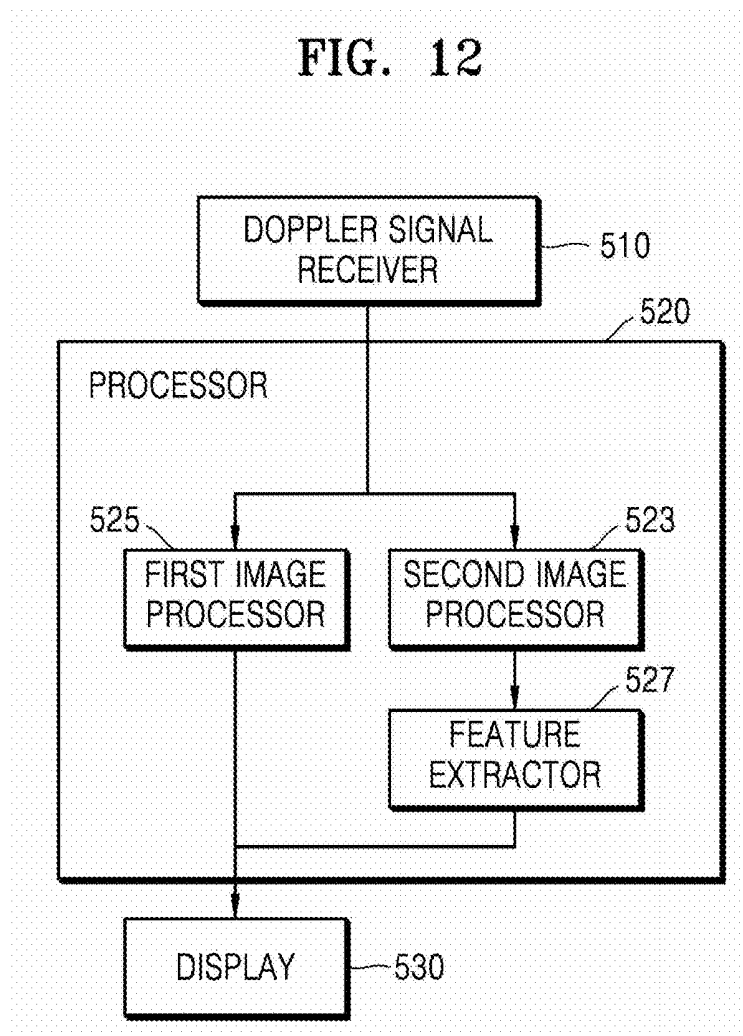


FIG. 13

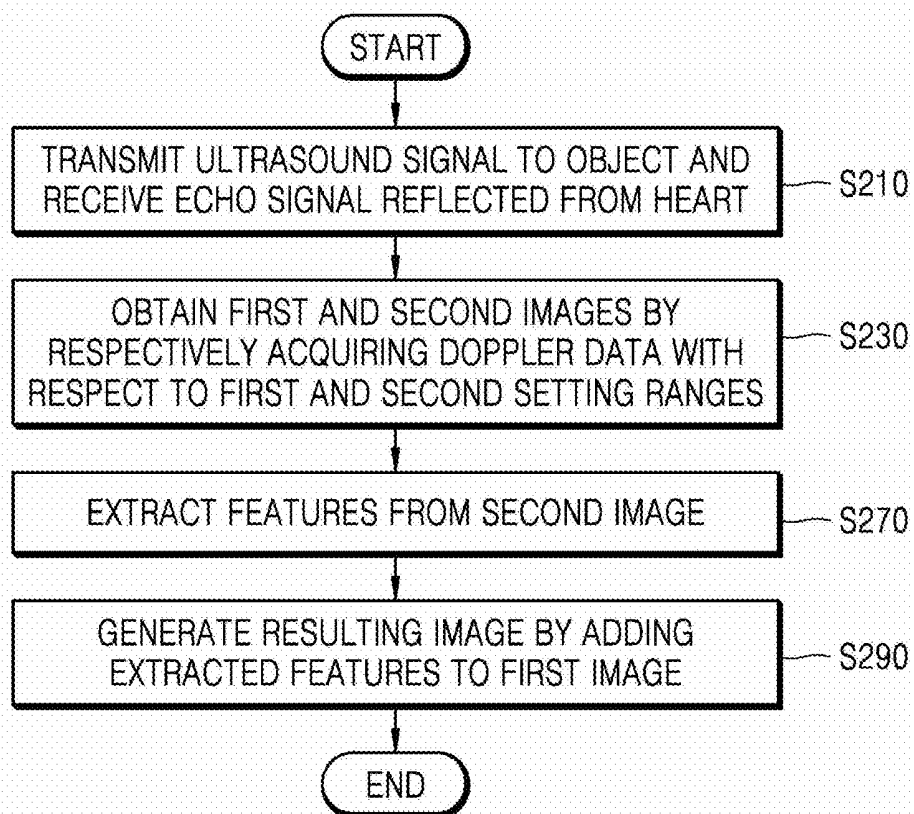

ULTRASOUND DIAGNOSIS APPARATUS AND METHOD OF OPERATING SAME

CROSS-REFERENCE TO RELATED APPLICATION(S)

[0001] This application is based on and claims priority under 35 U.S.C. § 119 to Korean Patent Application No. 10-2018-0013432, filed on Feb. 2, 2018, in the Korean Intellectual Property Office, the disclosure of which is incorporated by reference herein in its entirety.

BACKGROUND

1. Field

[0002] The disclosure relates to ultrasound diagnosis apparatuses and methods of operating the same.

2. Description of Related Art

[0003] Ultrasound diagnosis apparatuses transmit ultrasound signals generated by transducers of a probe to an object and receive information about echo signals reflected from the object, thereby obtaining an image of an internal part of the object. In particular, ultrasound diagnosis apparatuses are used for medical purposes including observing an internal area of an object, detecting foreign substances, and assessing injuries. Such ultrasound diagnosis apparatuses exhibit high stability, display images in real time, and are safe due to lack of radiation exposure, compared to diagnostic X-ray apparatuses. Therefore, ultrasound diagnosis apparatuses have been widely used together with other types of imaging diagnosis apparatuses.

SUMMARY

[0004] Provided are methods and apparatuses for ultrasound diagnosis apparatuses and methods that are used to further facilitate ultrasound diagnosis.

[0005] Additional aspects will be set forth in part in the description which follows and, in part, will be apparent from the description, or may be learned by practice of the presented embodiments.

[0006] In accordance with an aspect of the disclosure, a method of operating an ultrasound diagnosis apparatus includes: transmitting an ultrasound signal to the heart of the fetus and receiving an echo signal reflected from the heart; acquiring first Doppler data and second Doppler data respectively with respect to first and second setting ranges by using the echo signal; and displaying a first resulting image obtained based on the first Doppler data and the second Doppler data.

[0007] The first Doppler data may be data regarding blood flow of the heart, and the second Doppler data is data regarding valves of the heart.

[0008] The displaying of the first resulting image may include: determining presence of an abnormality in the heart based on the first Doppler data and the second Doppler data; and displaying the first resulting image, based on a result of the determining.

[0009] The determining of the presence of the abnormality in the heart may include determining the presence of the abnormality in the heart by calculating an isovolumic interval in a cardiac cycle of the heart.

[0010] The determining of the presence of the abnormality in the heart may include determining the presence of the

abnormality in the heart by determining whether the isovolumic interval is less than or equal to a predetermined time.

[0011] The displaying of the first resulting image may include: transmitting a difference between the first Doppler data and the second Doppler data to a display; and displaying the first resulting image based on the difference between the first Doppler data and the second Doppler data.

[0012] The displaying of the first resulting image may include: generating first image data and second image data respectively based on the first Doppler data and the second Doppler data; and generating feature extraction data representing properties of the heart, based on the first image data and the second image data.

[0013] The first resulting image may be represented such that a user recognizes the properties of the heart from the feature extraction data.

[0014] The first and second setting ranges may each include a range of a magnitude of a signal and a range of a velocity of blood flow, and the first and second Doppler data may each be data in which the magnitude of the signal is within a predetermined range, and the velocity of the blood flow is within a predetermined range.

[0015] The method may further include mixing the first Doppler data with the second Doppler data according to a predetermined method to obtain the first resulting image.

[0016] In accordance with another aspect of the disclosure, an ultrasound diagnosis apparatus for performing diagnosis with respect to a heart of a fetus includes: a probe configured to transmit an ultrasound signal to the heart of the fetus and receive an echo signal reflected from the heart; a processor configured to respectively acquire first Doppler data and second Doppler data with respect to first and second setting ranges by using the echo signal; and a display configured to display a first resulting image obtained based on the first Doppler data and the second Doppler data.

[0017] In accordance with another aspect of the disclosure, a non-transitory computer-readable recording medium has recorded thereon a program for performing a method of operating an ultrasound diagnosis apparatus, the method including: transmitting an ultrasound signal to a heart of a fetus and receiving an echo signal reflected from the heart; acquiring first Doppler data and second Doppler data respectively with respect to first and second setting ranges by using the echo signal; and displaying a first resulting image obtained based on the first Doppler data and the second Doppler data.

BRIEF DESCRIPTION OF THE DRAWINGS

[0018] The above and other aspects, features, and advantages of certain embodiments of the present disclosure will be more apparent from the following description taken in conjunction with the accompanying drawings, in which:

[0019] FIG. 1 is a block diagram illustrating an ultrasound diagnosis apparatus according to an embodiment;

[0020] FIGS. 2A, 2B, and 2C are diagrams respectively illustrating ultrasound diagnosis apparatuses according to an embodiment;

[0021] FIG. 3 is a block diagram of a configuration of an ultrasound diagnosis apparatus according to an embodiment;

[0022] FIG. 4 is a block diagram of a configuration of an ultrasound diagnosis apparatus according to another embodiment;

[0023] FIG. 5 is a flowchart of a method of operating an ultrasound diagnosis apparatus, according to an embodiment;

[0024] FIGS. 6A and 6B show images obtained by changing a setting range according to a target area being examined;

[0025] FIGS. 7A and 7B show images obtained by an ultrasound diagnosis apparatus by adjusting a setting range;

[0026] FIG. 8 shows an image for explaining a method, performed by an ultrasound diagnosis apparatus, of acquiring Doppler data with respect to a heart of an object;

[0027] FIGS. 9A through 9D are images for explaining a first resulting image provided by an ultrasound diagnosis apparatus, according to an embodiment;

[0028] FIG. 10 is a detailed flowchart of a method of operating an ultrasound diagnosis apparatus, according to an embodiment;

[0029] FIG. 11 is a detailed flowchart of a method of operating an ultrasound diagnosis apparatus, according to an embodiment;

[0030] FIG. 12 is a block diagram of a configuration of an ultrasound diagnosis apparatus according to another embodiment; and

[0031] FIG. 13 is a detailed flowchart of a method of operating an ultrasound diagnosis apparatus, according to an embodiment.

DETAILED DESCRIPTION

[0032] Hereinafter, the terms used in the specification will be briefly described, and then the present invention will be described in detail. The terms used in this specification are those general terms currently widely used in the art in consideration of functions regarding the present invention, but the terms may vary according to the intention of those of ordinary skill in the art, precedents, or new technology in the art. Also, specified terms may be selected by the applicant, and in this case, the detailed meaning thereof will be described in the detailed description of the invention. Thus, the terms used in the specification should be understood not as simple names but based on the meaning of the terms and the overall description of the invention.

[0033] Throughout the specification, it will also be understood that when a component “includes” an element, unless there is another opposite description thereto, it should be understood that the component does not exclude another element and may further include another element. In addition, terms such as “. . . unit”, “. . . module”, or the like refer to units that perform at least one function or operation, and the units may be implemented as hardware or software or as a combination of hardware and software.

[0034] Also, the term “unit” in the specification means a software component or hardware component such as a field-programmable gate array (FPGA) or an application-specific integrated circuit (ASIC), and performs a specific function. However, the term “unit” is not limited to software or hardware. The “unit” may be formed so as to be in an addressable storage medium, or may be formed so as to operate one or more processors. Thus, for example, the term “unit” may refer to components such as software components, object-oriented software components, class components, and task components, and may include processes, functions, attributes, procedures, subroutines, segments of program code, drivers, firmware, micro codes, circuits, data, a database, data structures, tables, arrays, or variables. A

function provided by the components and “units” may be associated with a smaller number of components and “units”, or may be divided into additional components and “units”.

[0035] It will be understood that, although the terms “first”, “second”, etc. may be used herein to describe various elements and/or components, these elements and/or components should not be limited by these terms. These terms are only used to distinguish one element or component from another element or component. For example, a first element or component may be termed a second element or component or vice versa without departing from the teachings of embodiments. As used herein, the term “and/or” includes any and all combinations of one or more of the associated listed items. Expressions such as “at least one of,” when preceding a list of elements, modify the entire list of elements and do not modify the individual elements of the list.

[0036] Throughout the specification, an “image” may mean multi-dimensional data formed of discrete image elements (e.g., pixels in a two-dimensional (2D) image and voxels in a three-dimensional (3D) image).

[0037] Throughout the specification, an “ultrasound image” refers to an image of an object, which is obtained using ultrasound waves. An ultrasound image may be an image obtained by transmitting ultrasound signals generated by transducers of a probe to an object and receiving information about echo signals reflected from the object. Furthermore, an ultrasound image may take different forms. For example, the ultrasound image may be at least one of an amplitude (A) mode image, a brightness (B) mode image, a color (C) mode image, and a Doppler (D) mode image. In addition, an ultrasound image may be a 2D or 3D image.

[0038] Furthermore, an “object” may be a human, an animal, or a part of a human or animal. For example, the object may be an organ (e.g., the liver, the heart, the womb, the brain, a breast, or the abdomen), a blood vessel, or a combination thereof. Furthermore, the object may be a phantom. The phantom means a material having a density, an effective atomic number, and a volume that are approximately the same as those of an organism. For example, the phantom may be a spherical phantom having properties similar to a human body.

[0039] Furthermore, throughout the specification, a “user” may be, but is not limited to, a medical expert, such as a medical doctor, a nurse, a medical laboratory technologist, a medical image expert, or a technician who repairs a medical apparatus

[0040] Embodiments will be described more fully hereinafter with reference to the accompanying drawings so that they may be easily implemented by one of ordinary skill in the art. However, the embodiments may have different forms and should not be construed as being limited to the descriptions set forth herein.

[0041] Embodiments of the invention now will be described more fully hereinafter with reference to the accompanying drawings, in which illustrative embodiments of the invention are shown.

[0042] FIG. 1 is a block diagram illustrating a configuration of an ultrasound diagnosis apparatus 100, i.e., a diagnostic apparatus, according to an embodiment.

[0043] Referring to FIG. 1, the ultrasound diagnosis apparatus 100 may include a probe 20, an ultrasound transceiver 110, a controller 120, an image processor 130, one or more

displays **140**, a storage **150**, e.g., a memory, a communicator **160**, i.e., a communication device or an interface, and an input interface **170**.

[0044] The ultrasound diagnosis apparatus **100** may be of a cart-type or a portable-type ultrasound diagnosis apparatus which is portable, moveable, mobile, or hand-held. Examples of a portable-type ultrasound diagnosis apparatus may include a smart phone, a laptop computer, a personal digital assistant (PDA), and a tablet personal computer (PC), each of which may include a probe and a software application, but embodiments are not limited thereto.

[0045] The probe **20** may include a plurality of transducers. The plurality of transducers may transmit ultrasound signals to an object **10** in response to transmitting signals received by the probe **20**, from a transmitter **113**. The plurality of transducers may receive ultrasound signals reflected from the object **10** to generate reception signals. In addition, the probe **20** and the ultrasound diagnosis apparatus **100** may be formed in one body (e.g., disposed in a single housing), or the probe **20** and the ultrasound diagnosis apparatus **100** may be formed separately (e.g., disposed separately in separate housings) but linked wirelessly or via wires. In addition, the ultrasound diagnosis apparatus **100** may include one or more probes **20** according to embodiments.

[0046] The controller **120** may control the transmitter **113** for the transmitter **113** to generate transmitting signals to be applied to each of the plurality of transducers based on a position and a focal point of the plurality of transducers included in the probe **20**.

[0047] The controller **120** may control the ultrasound receiver **115** to generate ultrasound data by converting reception signals received from the probe **20** from analogue to digital signals and summing the reception signals converted into digital form, based on a position and a focal point of the plurality of transducers.

[0048] The image processor **130** may generate an ultrasound image by using ultrasound data generated from the ultrasound receiver **115**.

[0049] The display **140** may display a generated ultrasound image and various pieces of information processed by the ultrasound diagnosis apparatus **100**. The ultrasound diagnosis apparatus **100** may include two or more displays **140** according to the present embodiment. The display **140** may include a touch screen in combination with a touch panel.

[0050] The controller **120** may control the operations of the ultrasound diagnosis apparatus **100** and flow of signals between the internal elements of the ultrasound diagnosis apparatus **100**. The controller **120** may include a memory for storing a program or data to perform functions of the ultrasound diagnosis apparatus **100** and a processor and/or a microprocessor (not shown) for processing the program or data. For example, the controller **120** may control the operation of the ultrasound diagnosis apparatus **100** by receiving a control signal from the input interface **170** or an external apparatus.

[0051] The ultrasound diagnosis apparatus **100** may include the communicator **160** and may be connected to external apparatuses, for example, servers, medical apparatuses, and portable devices such as smart phones, tablet personal computers (PCs), wearable devices, etc., via the communicator **160**.

[0052] The communicator **160** may include at least one element capable of communicating with the external apparatuses. For example, the communicator **160** may include at least one among a short-range communication module, a wired communication module, and a wireless communication module.

[0053] The communicator **160** may receive a control signal and data from an external apparatus and transmit the received control signal to the controller **120** so that the controller **120** may control the ultrasound diagnosis apparatus **100** in response to the received control signal.

[0054] The controller **120** may transmit a control signal to the external apparatus via the communicator **160** so that the external apparatus may be controlled in response to the control signal of the controller **120**.

[0055] For example, the external apparatus connected to the ultrasound diagnosis apparatus **100** may process the data of the external apparatus in response to the control signal of the controller **120** received via the communicator **160**.

[0056] A program for controlling the ultrasound diagnosis apparatus **100** may be installed in the external apparatus. The program may include command languages to perform part of operation of the controller **120** or the entire operation of the controller **120**.

[0057] The program may be pre-installed in the external apparatus or may be installed by a user of the external apparatus by downloading the program from a server that provides applications. The server that provides applications may include a recording medium where the program is stored.

[0058] The storage **150** may store various data or programs for driving and controlling the ultrasound diagnosis apparatus **100**, input and/or output ultrasound data, ultrasound images, applications, etc.

[0059] The input interface **170** may receive a user's input to control the ultrasound diagnosis apparatus **100** and may include a keyboard, button, keypad, mouse, trackball, jog switch, knob, a touchpad, a touch screen, a microphone, a motion input means, a biometrics input means, etc. For example, the user's input may include inputs for manipulating buttons, keypads, mice, trackballs, jog switches, or knobs, inputs for touching a touchpad or a touch screen, a voice input, a motion input, and a bioinformation input, for example, iris recognition or fingerprint recognition, but an embodiment is not limited thereto.

[0060] An example of the ultrasound diagnosis apparatus **100** according to the present embodiment is described below with reference to FIGS. 2A, 2B, and 2C.

[0061] FIGS. 2A, 2B, and 2C are diagrams illustrating ultrasound diagnosis apparatuses **100a**, **100b**, and **100c** according to an embodiment.

[0062] Referring to FIGS. 2A and 2B, the ultrasound diagnosis apparatus **100a** and the ultrasound diagnosis apparatus **100b** may include a main display **121** and a sub-display **122**. At least one among the main display **121** and the sub-display **122** may include a touch screen. The main display **121** and the sub-display **122** may display ultrasound images and/or various information processed by the ultrasound diagnosis apparatus (**100a**, **100b**). The main display **121** and the sub-display **122** may provide graphical user interfaces (GUI), thereby receiving user's inputs of data to control the ultrasound diagnosis apparatus (**100a**, **100b**). For example, the main display **121** may display an ultrasound image and the sub-display **122** may display a control panel

to control display of the ultrasound image as a GUI. The sub-display 122 may receive an input of data to control the display of an image through the control panel displayed as a GUI. The ultrasound diagnosis apparatus 100a may control the display of the ultrasound image on the main display 121 by using the input control data.

[0063] Referring to FIG. 2B, the ultrasound diagnosis apparatus 100b may include a control panel 165. The control panel 165 may include buttons, trackballs, jog switches, or knobs, and may receive data to control the ultrasound diagnosis apparatus 100 from the user. For example, the control panel 165 may include a time gain compensation (TGC) button 171 and a freeze button 172. The TGC button 171 is to set a TGC value for each depth of an ultrasound image. Also, when an input of the freeze button 172 is detected during scanning an ultrasound image, the ultrasound diagnosis apparatus 100 may keep displaying a frame image at that time point.

[0064] The buttons, trackballs, jog switches, and knobs included in the control panel 165 may be provided as a GUI to the main display 121 or the sub-display 122.

[0065] Referring to FIG. 2C, the ultrasound diagnosis apparatus 100c may be implemented as a portable ultrasound diagnosis apparatus. An example of the portable ultrasound diagnosis apparatus may include, for example, smart phones including probes and applications, laptop computers, personal digital assistants (PDAs), or tablet PCs, but an embodiment is not limited thereto.

[0066] The ultrasound diagnosis apparatus 100 may include the probe 20 and a main body 40. The probe 20 may be connected to one side of the main body 40 by wire or wirelessly. The main body 40 may include a touch screen 145. The touch screen 145 may display an ultrasound image, various pieces of information processed by the ultrasound diagnosis apparatus 100, and a GUI.

[0067] FIG. 3 is a block diagram of a configuration of an ultrasound diagnosis apparatus 300 according to an embodiment.

[0068] Referring to FIG. 3, the ultrasound diagnosis apparatus 300 according to the present embodiment may include a probe 310, a processor 320, and a display 330. However, all of the components shown in FIG. 3 are not essential components. The ultrasound diagnosis apparatus 300 may include more or fewer components than those shown in FIG. 3. Configurations and operations of the probe 310, the processor 320, and the display 330 will now be described in detail.

[0069] The probe 310 may include a plurality of transducers that convert ultrasound signals into electrical signals or vice versa. In other words, the probe 310 may include a transducer array consisting of a plurality of transducers. The plurality of transducers may be arranged in a one-dimensional (1D) or 2D array, and each of the plurality of transducers generates ultrasound signals separately or simultaneously. An ultrasound signal transmitted by each transducer is reflected off a discontinuous impedance surface within an object. Each transducer may convert a received reflected echo signal into an electrical reception signal. The probe 310 may transmit ultrasound signals to the heart of an object and receive echo signals reflected therefrom. In this case, the object may be a human. In detail, the object may include an adult, a child, a fetus, etc.

[0070] The processor 320 may receive an echo signal from the probe 310. The processor 320 may then acquire first

Doppler data with respect to a first setting range based on the received echo signal. Furthermore, the processor 320 may acquire second Doppler data with respect to a second setting range based on the echo signal. In this case, the first Doppler data may refer to data regarding blood flow of the heart, and the second Doppler data may refer to data regarding valves of the heart.

[0071] The processor 320 may acquire data regarding a first resulting image to be displayed on the display 330. The processor 320 may acquire the data regarding the first resulting image based on the first Doppler data and the second Doppler data. For example, the processor 320 may acquire data regarding the first resulting image by using a difference between the first Doppler data and the second Doppler data. The processor 320 may then transmit the data regarding the first resulting image to the display 330.

[0072] The display 330 displays a predetermined screen. In detail, the display 330 may display a predetermined screen according to control by the processor 320. The display 330 includes a display panel (not shown) on which a resulting image (e.g., an ultrasound image or diagnostic image), etc. may be displayed.

[0073] The ultrasound diagnosis apparatus 300 may include a central arithmetic processor that controls all operations of the probe 310, the processor 320, and the display 330. The central arithmetic processor may be implemented as an array of a plurality of logic gates or a combination of a general purpose microprocessor and a memory for storing a program that can be run on the general purpose microprocessor. Furthermore, it will be appreciated by those of ordinary skill in the art that the central arithmetic processor may be formed by different types of hardware.

[0074] FIG. 4 is a block diagram of a configuration of an ultrasound diagnosis apparatus 400 according to another embodiment.

[0075] Referring to FIG. 4, the ultrasound diagnosis apparatus 400 according to the present embodiment may include a probe 410, a processor 420, a display 430, a first image processor 450, and a second image processor 440.

[0076] Since the probe 410, the processor 420, and the display 430 included in the ultrasound diagnosis apparatus 400 of FIG. 1 respectively correspond to the probe 310, the processor 320, and the display 330 in the ultrasound diagnosis apparatus 300 described with reference to FIG. 3, descriptions that are provided above with respect to FIG. 3 will be omitted below. The ultrasound diagnosis apparatus 400 may include more or fewer components than those shown in FIG. 4.

[0077] The ultrasound diagnosis apparatus 400 may include the first and second image processors 450 and 440. The first image processor 450 may acquire first Doppler data with respect to a first setting range based on an echo signal. The second image processor 440 may acquire second Doppler data with respect to a second setting range based on the same echo signal that is used by the first image processor 450. The first and second image processors 450 and 440 may respectively process and transform the first Doppler data and the second Doppler data and transmit the results to the processor 420. Unlike in FIG. 4, the first and second image processors 450 and 440 may be included in the processor 420.

[0078] For example, the first image processor 450 may generate data regarding a first image based on the first Doppler data. For example, the first image processor 450

may generate data regarding the first image by extracting data that satisfies the first setting range among the first Doppler data.

[0079] For example, the second image processor 440 may generate data regarding a second image based on the second Doppler data. For example, the second image processor 440 may generate data regarding the second image by extracting data that satisfies the second setting range among the second Doppler data.

[0080] In this case, the first Doppler data and the second Doppler data are acquired by transforming the same echo signal or are generated therefrom. Thus, the ultrasound diagnosis apparatus 400 according to the present embodiment may generate a resulting image via one-time diagnosis, thereby making it convenient for a user to perform diagnosis.

[0081] For example, the processor 420 may extract features by comparing the data regarding the first image with the data regarding the second image. The processor 420 may generate the first resulting image by adding the extracted features to the first image. The first resulting image may be generated using other various methods.

[0082] For example, the first or second setting range may mean a range of a setting value including at least one of a gain, a sensitivity, a power, and a blood flow velocity.

[0083] The ultrasound diagnosis apparatus 400 may further include a user interface (not shown). The user interface may refer to a device via which data for controlling the ultrasound diagnosis apparatus 400 is received from the user.

[0084] The processor 420 may control the display 430 to generate and output a user interface screen for receiving a predetermined command or data from the user. The display 430 may display, on the display panel, an input screen for respectively setting landmarks corresponding to predetermined movements of the heart in the first and second Doppler data. In this case, the predetermined movements may be an opening movement of heart valves and flow of blood through the heart.

[0085] For example, the ultrasound diagnosis apparatus 400 may further include a communicator (not shown). The communicator may receive and/or transmit data from and/or to an external device. For example, the communicator may transmit synchronized first and second Doppler data to an external terminal. Furthermore, the communicator may transmit at least one piece of data related to a function of the heart to the external terminal. In this case, the external terminal may be a patient's terminal. Furthermore, the external device a server for providing may be a relay server of an application for providing health information to a patient or a server that manages medical records of the patient. The communicator may connect to a wireless probe or an external device via a communication network based on Wi-Fi or Wi-Fi Direct (WFD) technology. In detail, examples of a wireless communication network to which the communicator can connect may include, but are not limited to, Wireless LAN (WLAN), Wi-Fi, Bluetooth, ZigBee, WFD, Ultra Wideband (UWB), Infrared Data Association (IrDA), Bluetooth Low Energy (BLE), and Near Field Communication (NFC).

[0086] The ultrasound diagnosis apparatus 400 may further include a memory (not shown). The memory may store data related to an ultrasound image (e.g., an ultrasound image, ultrasound data, scan-related data, data related to

diagnosis of a patient, etc.), data transmitted from an external device to the ultrasound diagnosis apparatus 400, etc. The data transmitted from the external device may include patient-related information, data necessary for diagnosis and treatment of a patient, a patient's past medical history, a medical work list corresponding to instructions regarding diagnosis on a patient, and the like.

[0087] Furthermore, the memory may store a program for executing a method of operating the ultrasound diagnosis apparatus 400. The memory may include a code representing a method of operating the ultrasound diagnosis apparatus 400.

[0088] The ultrasound diagnosis apparatus 400 may include a central arithmetic processor that controls all operations of the probe 410, the processor 420, the display 430, the first image processor 450, the second image processor 440, and the memory. The central arithmetic processor may be implemented as an array of a plurality of logic gates or a combination of a general purpose microprocessor and a memory for storing a program that can be executed on the general purpose microprocessor. Furthermore, it will be appreciated by those of ordinary skill in the art that the central arithmetic processor may be formed by different types of hardware.

[0089] Hereinafter, various operations performed by the ultrasound diagnosis apparatus 300 (400) and applications thereof will be described in detail. Although none of the probe 310 (410), the processor 320 (420), the display 330 (430), the user interface, the communicator, and the memory are specified, features and aspects that would be clearly understood by and are obvious to those of ordinary skill in the art may be considered as a typical implementation. The scope of the present disclosure is not limited by a name of a particular component or a physical/logical structure.

[0090] FIG. 5 is a flowchart of a method of operating an ultrasound diagnosis apparatus, according to an embodiment.

[0091] The method according to the present embodiment may include operations of: transmitting an ultrasound signal to an object and receiving an echo signal reflected from the heart (S110); acquiring first Doppler data with respect to a first setting range and second Doppler data with respect to a second setting range (S130); and displaying a first resulting image obtained based on the first and second Doppler data (S170).

[0092] For example, in operations S130 and S170, the first and second setting ranges may each be ranges of a magnitude of a signal and a velocity of blood flow. Furthermore, the first Doppler data may be data in which a magnitude of a signal is within a first range, and a velocity of blood flow is within a second range. The second Doppler data may be data in which the magnitude of the signal is within a third range, and the velocity of blood flow is within a third range.

[0093] According to an embodiment, the first Doppler data may be acquired with respect to the first setting range by using an echo signal. Furthermore, the second Doppler data may be acquired with respect to the second setting range by using the same echo signal.

[0094] According to an embodiment, in operation S170, to obtain the first resulting image, the processor 420 may mix the first Doppler data with the second Doppler data according to a predetermined method.

[0095] FIGS. 6A and 6B show images obtained by changing a setting range according to a target area being observed.

[0096] For example, FIG. 6A may show an image obtained by optimizing a setting range for observation of a blood flow velocity, and FIG. 6B may show an image obtained by optimizing a setting range for observation of movement of an organ. In this way, the type of an image that can be obtained by the user varies according to a setting range. However, it may be inconvenient for a user to observe a plurality of these images or individually generate and observe the images.

[0097] According to an embodiment, as shown in FIG. 4, an ultrasound diagnosis apparatus may include first and second image processors that respectively acquire pieces of Doppler data with respect to two or more setting ranges based on one ultrasound signal (or echo signal). By combining together the acquired two or more pieces of Doppler data according to a predetermined method, it is possible to provide important information to the user.

[0098] FIGS. 7A and 7B show images obtained by an ultrasound diagnosis apparatus by adjusting a setting range.

[0099] Doppler is a method of observing a blood flow velocity using ultrasound waves. Furthermore, pulsed wave Doppler or continuous wave Doppler may be generally used for relatively accurate measurement of blood flow velocity. In this case, various setting values may be used to predict a range of a blood flow velocity or to obtain a user's desired image. However, use of these setting values or setting ranges may cause the user to miss important information. Furthermore, when the user changes a setting to observe more information, unimportant information may be included and thus, the user may miss actual important information.

[0100] For example, FIG. 7A may be an image obtained by generally adjusting a setting range for observation of blood flow, and FIG. 7B may be an image obtained by excessively adjusting a setting range. In other words, both general setting as shown in FIG. 7A and excessive setting as shown in FIG. 7B may make it difficult for the user to identify important information.

[0101] According to an embodiment, an ultrasound diagnosis apparatus may respectively acquire pieces of Doppler data with respect to two setting ranges and process the acquired Doppler data by using a predetermined method, thereby enabling a user to easily identify important information. According to another embodiment, an ultrasound diagnosis apparatus may respectively acquire pieces of Doppler data with respect to two or more setting ranges.

[0102] FIG. 8 shows an image for explaining a method, performed by an ultrasound diagnosis apparatus, of acquiring Doppler data with respect to a heart of an object.

[0103] A waveform shown in FIG. 8 represents a pulsed wave Doppler signal. The pulsed wave Doppler signal may be used to display a blood flow image. A click signal is indicated by arrows and may be used to detect a valve signal. However, since the click signal is not clearly identified, it may not be easy to clearly provide a valve signal to the user. Hereinafter, an example in which such a valve signal is extracted from a blood flow image and provided to the user according to an embodiment will be described.

[0104] FIGS. 9A through 9D show images for explaining a first resulting image provided by an ultrasound diagnosis apparatus, according to an embodiment.

[0105] FIG. 9A illustrates a first image obtained based on first Doppler data, and FIG. 9B illustrates a second image obtained based on second Doppler data.

[0106] FIG. 9C illustrates a feature extraction image obtained from a second image, and FIG. 9D illustrates a first resulting image obtained by adding the feature extraction image to the first image.

[0107] For example, the processor 420 may obtain the feature extraction image of FIG. 9C from the first image of FIG. 9A and the second image of FIG. 9B. The processor 420 may also obtain the first resulting image of FIG. 9D by adding the feature extraction image of FIG. 9C to the first or second image.

[0108] FIG. 10 is a detailed flowchart of a method of operating the ultrasound diagnosis apparatus 400, according to an embodiment.

[0109] Operation S170 described with reference to FIG. 5 may include operations S273 and S276. Referring to FIG. 10, the processor 420 may determine the presence of an abnormality in the heart based on the first and second Doppler data (S273). In this case, to do so, the processor 420 may calculate an isovolumic interval in a cardiac cycle of the heart. For example, the processor 420 may determine the presence of an abnormality in the heart by determining a length of the isovolumic interval. In detail, the processor 420 may determine the presence of an abnormality in the heart by determining whether the length of the isovolumic interval is less than or equal to a reference value.

[0110] The processor 420 may display a first resulting image based on a result of the determining in operation S273 (S276). For example, when any abnormality of the heart is present, the processor 420 may indicate the presence of an abnormality in the heart on the first resulting image by displaying a separate marker. For example, the processor 420 may indicate the presence of an abnormality in the heart on the first resulting image based on an input received via the user interface.

[0111] FIG. 11 is a detailed flowchart of a method of operating the ultrasound diagnosis apparatus 400, according to an embodiment.

[0112] Operation S170 described with reference to FIG. 5 may include operations S373 and S376. Referring to FIG. 11, the processor 420 may transmit a difference between the first Doppler data and the second Doppler data to the display 430 (S373). The processor 430 may then display a first resulting image based on the difference between the first and second Doppler data (S376).

[0113] FIG. 12 is a block diagram of a configuration of an ultrasound diagnosis apparatus according to another embodiment.

[0114] Referring to FIG. 12, the ultrasound diagnosis apparatus according to the present embodiment may include a Doppler signal receiver 510, a processor 520, and a display 530. The processor 520 may include a first image generator 525, a second image generator 523, and a feature extractor 527.

[0115] FIG. 13 is a detailed flowchart of a method of operating the ultrasound diagnosis apparatus of FIG. 12, according to an embodiment.

[0116] The Doppler signal receiver 510 may receive an ultrasound signal to an object and receive an echo signal reflected from the heart (S210).

[0117] The first image generator 525 may obtain a first image by acquiring Doppler data with respect to a first setting range, and the second image generator 523 may obtain a second image by acquiring Doppler data with respect to a second setting range (S230).

[0118] For example, the first image generator 525 may generate first Doppler data by transforming an echo signal received from a fetus's heart only within the first setting range and obtain the first image based on the first Doppler data. The second image generator 523 may generate second Doppler data by transforming the same echo signal that is used to obtain the first image only within the second setting range and obtain the second image based on the second Doppler data.

[0119] By performing these operations, image 1 as shown in FIG. 9A and image 2 as shown in FIG. 9B may be obtained.

[0120] The feature extractor 527 may extract features from the second image (S270). By performing operation S270, a feature extraction image as shown in FIG. 9C may be obtained. The processor 520 may generate a resulting image by adding the extracted features to the first image (S290). By performing operation S290, an image representation as shown in FIG. 9D may be obtained.

[0121] According to various embodiments, the first and second images may be processed using various methods. Furthermore, the number of images being processed is not limited to two (2) but may be implemented in various ways.

[0122] According to various embodiments, the processor 520 may extract features by combining pieces of data regarding a plurality of images in various ways and generate a resulting image by combining the extracted features with differently processed data.

[0123] The ultrasound diagnosis apparatuses described above may be implemented using hardware components, software components, and/or a combination thereof. For example, the apparatuses and components illustrated in the embodiments may be implemented using one or more general-purpose or special-purpose computers, such as a processor, a controller, an arithmetic logic unit (ALU), a digital signal processor, a microcomputer, a field programmable array (FPA), a programmable logic unit (PLU), a microprocessor, or any other device capable of responding to and executing instructions.

[0124] A processing device may run an operating system (OS) and one or more software applications running on the OS. The processing device may also access, store, manipulate, process, and create data in response to execution of software.

[0125] Although a single processing device may be illustrated for convenience, one of ordinary skill in the art will appreciate that a processing device may include a plurality of processing elements and/or a plurality of types of processing elements. For example, a processing device may include a plurality of processors or a processor and a controller. In addition, the processing device may have different processing configurations such as parallel processors.

[0126] Software may include a computer program, a piece of code, a command, or one or more combinations thereof and independently or collectively instruct or configure the processing device to operate as desired.

[0127] Software and/or data may be embodied permanently or temporarily in any type of machine, component, physical equipment, virtual equipment, computer storage medium or device, or in a transmitted signal wave so as to be interpreted by the processing device or to provide commands or data to the processing device. The software may also be distributed over network-coupled computer systems

so that the software is stored and executed in a distributed fashion. The software and data may be stored in one or more computer-readable recording media.

[0128] The methods according to the embodiments may be recorded in non-transitory computer-readable recording media including program instructions to implement various operations embodied by a computer. The non-transitory computer-readable recording media may also include, alone or in combination with the program instructions, data files, data structures, and the like. The program instructions recorded in the non-transitory computer-readable recording media may be designed and configured specially for the embodiments or be known and available to those of ordinary skill in computer software.

[0129] Examples of non-transitory computer-readable recording media include magnetic media such as hard disks, floppy disks, and magnetic tape, optical media such as CD-ROM discs and DVDs, magneto-optical media such as floptical discs, and hardware devices that are specially configured to store and perform program instructions, such as ROM, RAM, flash memory, and the like.

[0130] Examples of program instructions include both machine code made by a compiler and a high-level programming language to be executed in the computer by using an interpreter.

[0131] The above-described hardware devices may be configured to act as one or more software modules in order to perform the operations of the above-described embodiments, or vice versa.

[0132] While one or more embodiments have been described with reference to the figures, it will be understood by those of ordinary skill in the art that various modifications and changes in form and details may be made from the above descriptions without departing from the spirit and scope as defined by the following claims. For example, adequate effects may be achieved even if the above techniques are performed in a different order than that described above, and/or the aforementioned elements, such as systems, structures, devices, or circuits, are combined or coupled in different forms and modes than those described above or are replaced or supplemented by other components or their equivalents.

[0133] Thus, the scope of the present disclosure is defined not by the detailed description thereof but by the appended claims and their equivalents.

What is claimed is:

1. A method of operating an ultrasound diagnosis apparatus for performing diagnosis with respect to a heart of a fetus, the method comprising:

transmitting an ultrasound signal to the heart of the fetus and receiving an echo signal reflected from the heart; acquiring first Doppler data and second Doppler data respectively with respect to first and second setting ranges by using the echo signal; and

displaying a first resulting image obtained based on the first Doppler data and the second Doppler data.

2. The method of claim 1, wherein the first Doppler data is data regarding blood flow of the heart, and the second Doppler data is data regarding valves of the heart.

3. The method of claim 1, wherein the displaying of the first resulting image comprises:

determining presence of an abnormality in the heart based on the first Doppler data and the second Doppler data; and

displaying the first resulting image, based on a result of the determining.

4. The method of claim 3, wherein the determining of the presence of the abnormality in the heart comprises determining the presence of the abnormality in the heart by calculating an isovolumic interval in a cardiac cycle of the heart.

5. The method of claim 4, wherein the determining of the presence of the abnormality in the heart comprises determining the presence of the abnormality in the heart by determining whether the isovolumic interval is less than or equal to a predetermined time.

6. The method of claim 1, wherein the displaying of the first resulting image comprises:

transmitting a difference between the first Doppler data and the second Doppler data to a display; and displaying the first resulting image based on the difference between the first Doppler data and the second Doppler data.

7. The method of claim 1, wherein the displaying of the first resulting image comprises:

generating first image data and second image data respectively based on the first Doppler data and the second Doppler data; and

generating feature extraction data representing properties of the heart, based on the first image data and the second image data.

8. The method of claim 7, wherein the first resulting image is represented such that a user recognizes the properties of the heart from the feature extraction data.

9. The method of claim 1, wherein the first and second setting ranges each include a range of a magnitude of a signal and a range of a velocity of blood flow, and

wherein the first and second Doppler data are each data in which the magnitude of the signal is within a predetermined range, and the velocity of the blood flow is within a predetermined range.

10. The method of claim 1, further comprising mixing the first Doppler data with the second Doppler data according to a predetermined method to obtain the first resulting image.

11. An ultrasound diagnosis apparatus for performing diagnosis with respect to a heart of a fetus, the ultrasound diagnosis apparatus comprising:

a probe configured to transmit an ultrasound signal to the heart of the fetus and receive an echo signal reflected from the heart;

a processor configured to respectively acquire first Doppler data and second Doppler data with respect to first and second setting ranges by using the echo signal; and a display configured to display a first resulting image obtained based on the first Doppler data and the second Doppler data.

12. The ultrasound diagnosis apparatus of claim 11, wherein the first Doppler data is data regarding blood flow of the heart, and the second Doppler data is data regarding valves of the heart.

13. The ultrasound diagnosis apparatus of claim 11, wherein the processor is further configured to determine

presence of an abnormality in the heart, based on the first Doppler data and the second Doppler data, and

wherein the display is further configured to display the first resulting image based on a result of the determining.

14. The ultrasound diagnosis apparatus of claim 13, wherein the processor is further configured to determine the presence of the abnormality in the heart by calculating an isovolumic interval in a cardiac cycle of the heart.

15. The ultrasound diagnosis apparatus of claim 14, wherein the processor is further configured to determine the presence of the abnormality in the heart by determining whether the isovolumic interval is less than or equal to a predetermined time.

16. The ultrasound diagnosis apparatus of claim 11, wherein the processor is further configured to transmit a difference between the first Doppler data and the second Doppler data to the display, and

wherein the display is further configured to display the first resulting image based on the difference between the first Doppler data and the second Doppler data.

17. The ultrasound diagnosis apparatus of claim 11, wherein the processor is further configured to respectively generate first image data and second image data, based on the first Doppler data and the second Doppler data and produce feature extraction data representing properties of the heart, based on the first image data and the second image data.

18. The ultrasound diagnosis apparatus of claim 17, wherein the display is further configured to represent the first resulting image such that a user recognizes the properties of the heart from the feature extraction data.

19. The ultrasound diagnosis apparatus of claim 11, wherein the first and second setting ranges each include a range of a magnitude of a signal and a range of a velocity of blood flow, and

wherein the first and second Doppler data are each data in which the magnitude of the signal is within a predetermined range, and the velocity of the blood flow is within a predetermined range.

20. The ultrasound diagnosis apparatus of claim 11, wherein the processor is further configured to mix the first Doppler data with the second Doppler data according to a predetermined method to obtain the first resulting image.

21. A non-transitory computer-readable recording medium having recorded thereon a program for performing a method of operating an ultrasound diagnosis apparatus, the method comprising:

transmitting an ultrasound signal to a heart of a fetus and receiving an echo signal reflected from the heart;

acquiring first Doppler data and second Doppler data respectively with respect to first and second setting ranges by using the echo signal; and

displaying a first resulting image obtained based on the first Doppler data and the second Doppler data.

* * * * *

| | | | |
|----------------|--|---------|------------|
| 专利名称(译) | 超声诊断设备及其操作方法 | | |
| 公开(公告)号 | US20190239856A1 | 公开(公告)日 | 2019-08-08 |
| 申请号 | US16/155168 | 申请日 | 2018-10-09 |
| [标]申请(专利权)人(译) | 三星麦迪森株式会社 | | |
| 申请(专利权)人(译) | 三星MEDISON CO. , LTD. | | |
| 当前申请(专利权)人(译) | 三星MEDISON CO. , LTD. | | |
| [标]发明人 | LEE JIN YONG KIM JONG SIK | | |
| 发明人 | LEE, JIN-YONG KIM, JONG-SIK | | |
| IPC分类号 | A61B8/08 A61B8/06 | | |
| CPC分类号 | A61B8/5223 A61B8/488 A61B8/06 A61B8/5246 A61B8/0883 A61B8/0866 | | |
| 优先权 | 1020180013432 2018-02-02 KR | | |
| 外部链接 | Espacenet USPTO | | |

摘要(译)

提供一种超声波诊断装置及其操作方法。该方法包括：将超声信号发送到胎儿的心脏并接收从心脏反射的回声信号；通过使用回波信号分别获取关于第一和第二设定范围的第一多普勒数据和第二多普勒数据；并显示基于第一多普勒数据和第二多普勒数据获得的第一结果图像。

