



US 20050154311A1


(19) **United States**(12) **Patent Application Publication** (10) **Pub. No.: US 2005/0154311 A1**
(43) **Pub. Date: Jul. 14, 2005**(54) **CONNECTION APPARATUS AND METHOD
FOR CONTROLLING AN ULTRASOUND
PROBE****Related U.S. Application Data**(63) Continuation-in-part of application No. 10/756,231,
filed on Jan. 13, 2004.(76) Inventor: **Reinhold Bruestle, Zipf (AT)****Publication Classification**(51) **Int. Cl.⁷** **A61B 8/14**(52) **U.S. Cl.** **600/459**

(57)

ABSTRACT

A connection apparatus and method for controlling an ultrasound probe are provided. The ultrasound probe includes a first chamber, a second chamber and a sealing member between the first and second chambers. The ultrasound probe further includes a connection member within the second chamber having a rigid portion and a flexible portion, with the rigid portion forming at least part of the sealing member.

Correspondence Address:

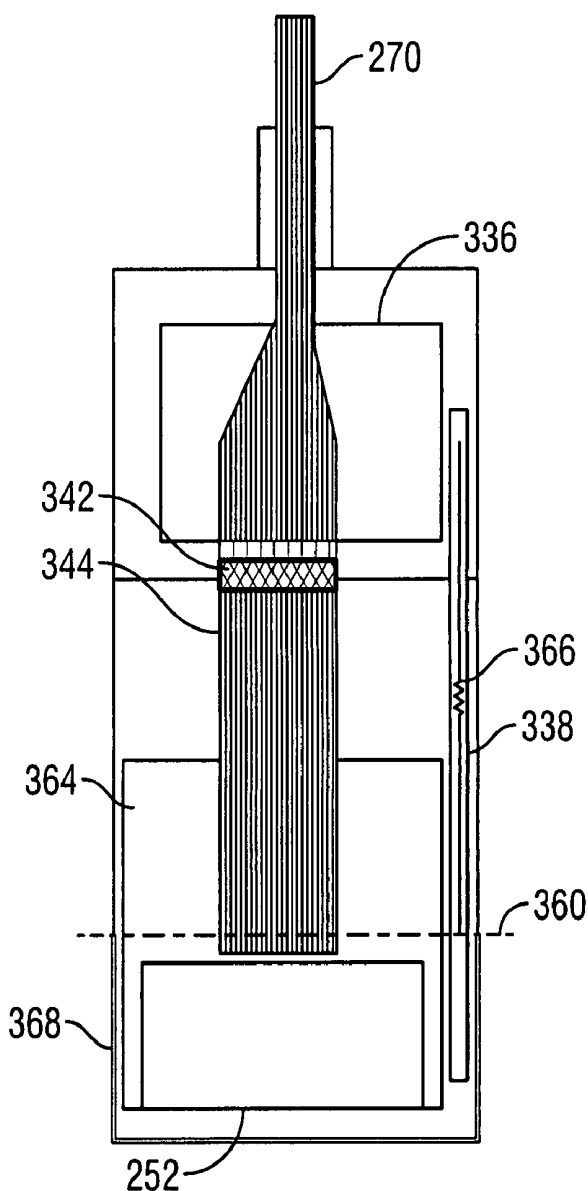Dean D. Small**Armstrong Teasdale LLP****Suite 2600****One Metropolitan Square****St. Louis, MO 63102 (US)**(21) Appl. No.: **10/767,585**(22) Filed: **Jan. 29, 2004**

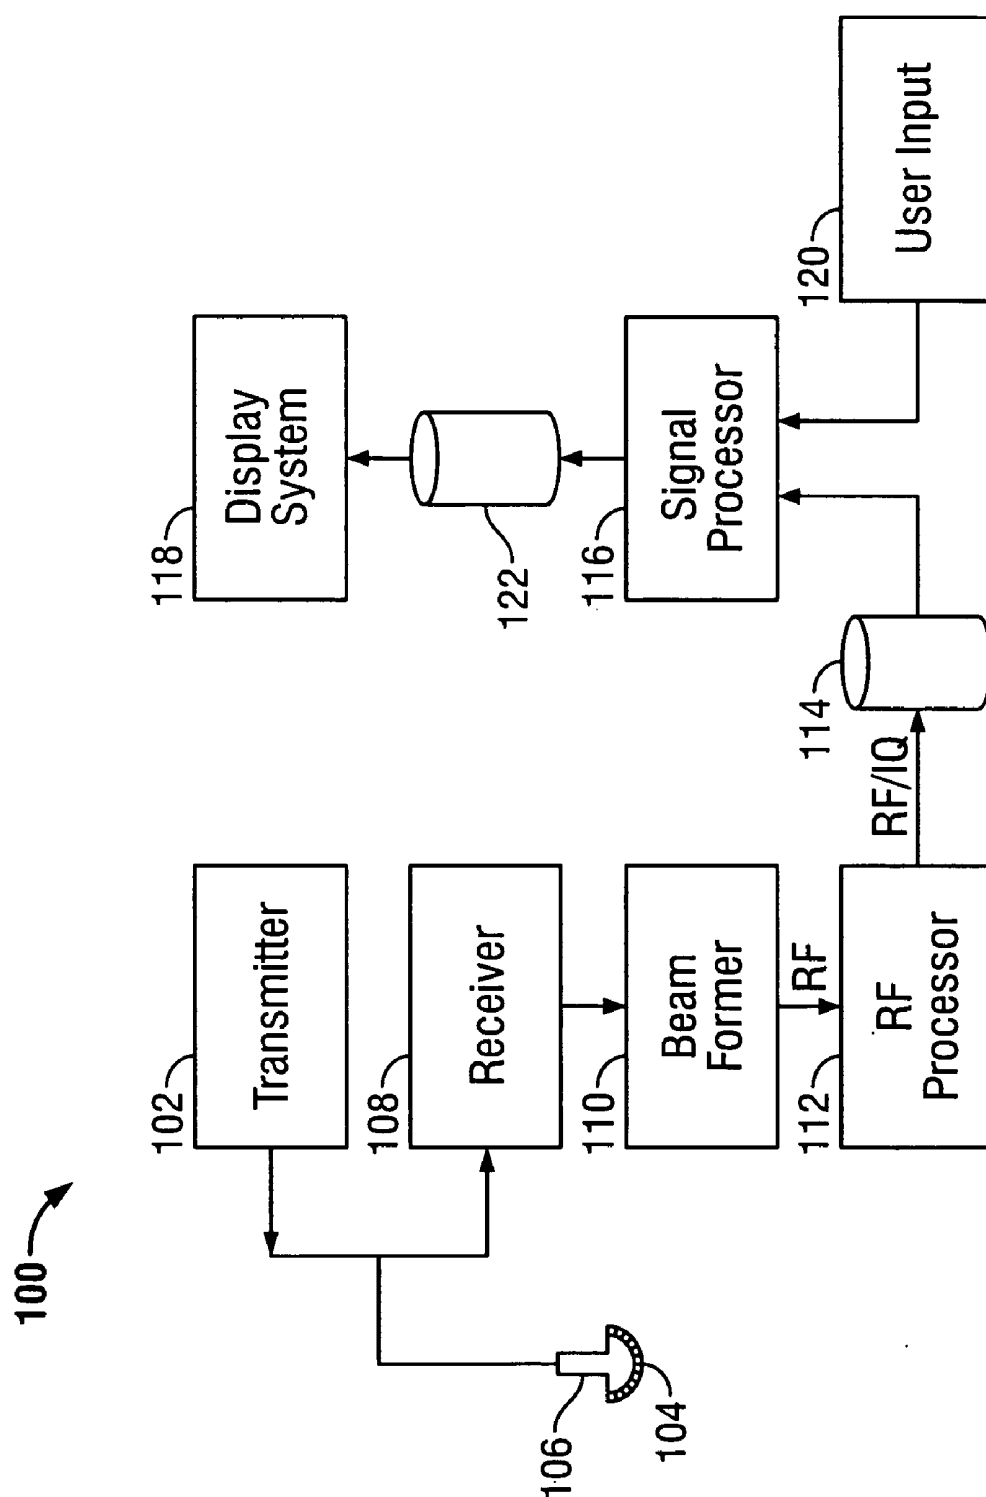


FIG. 1

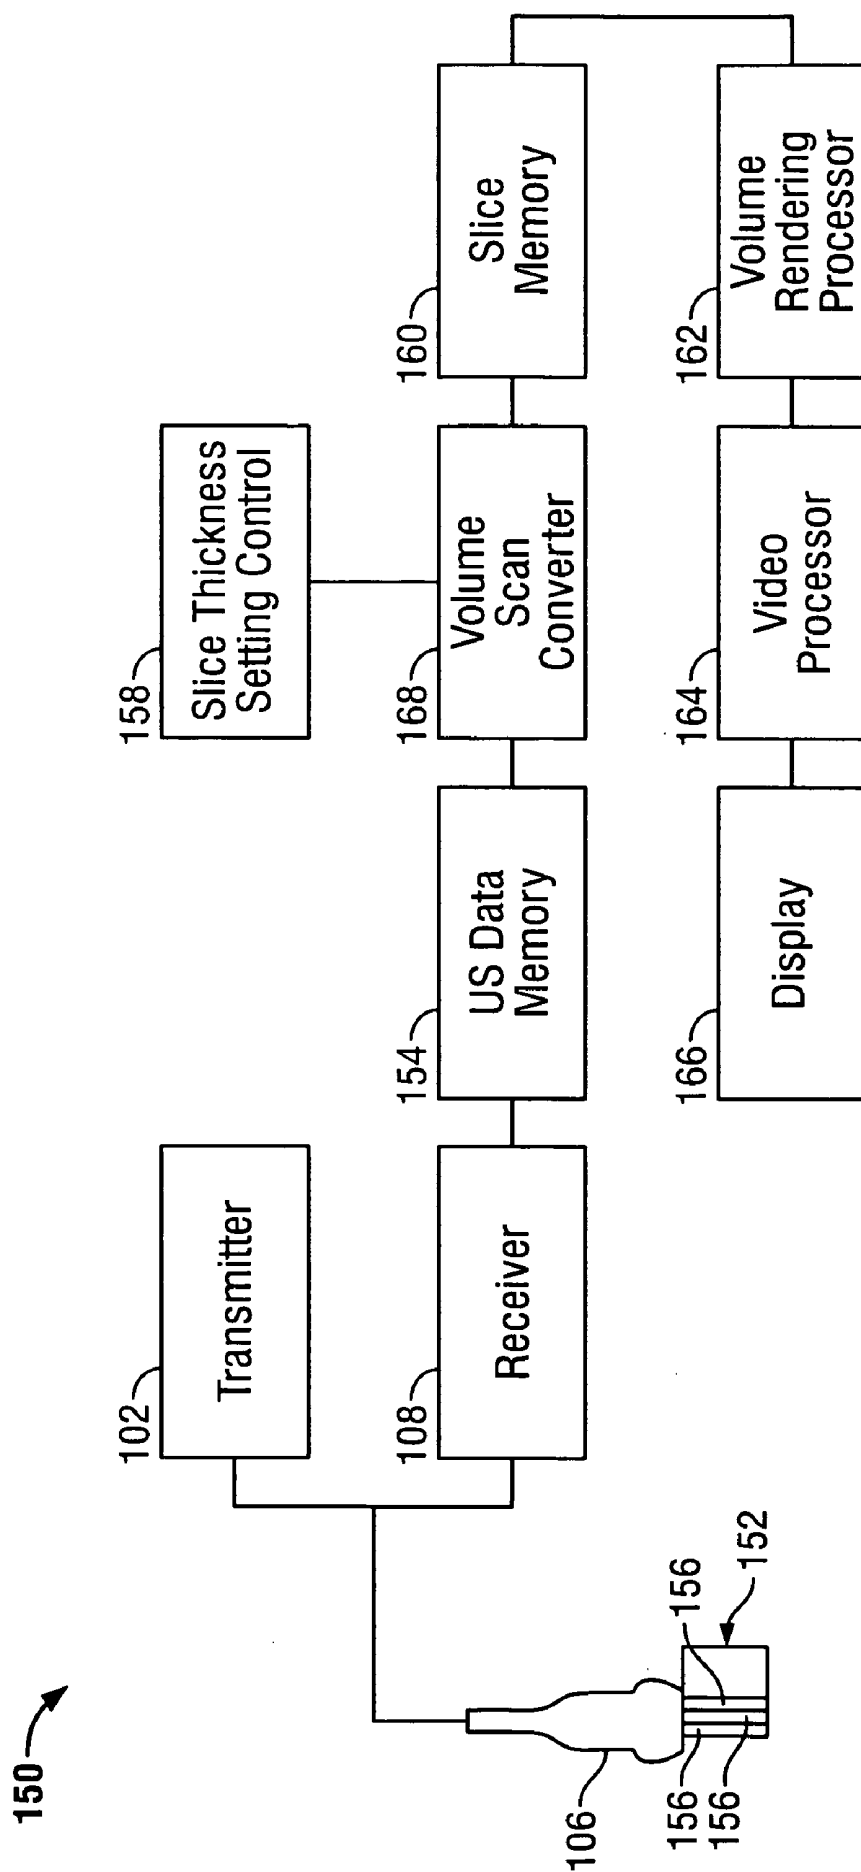


FIG. 2

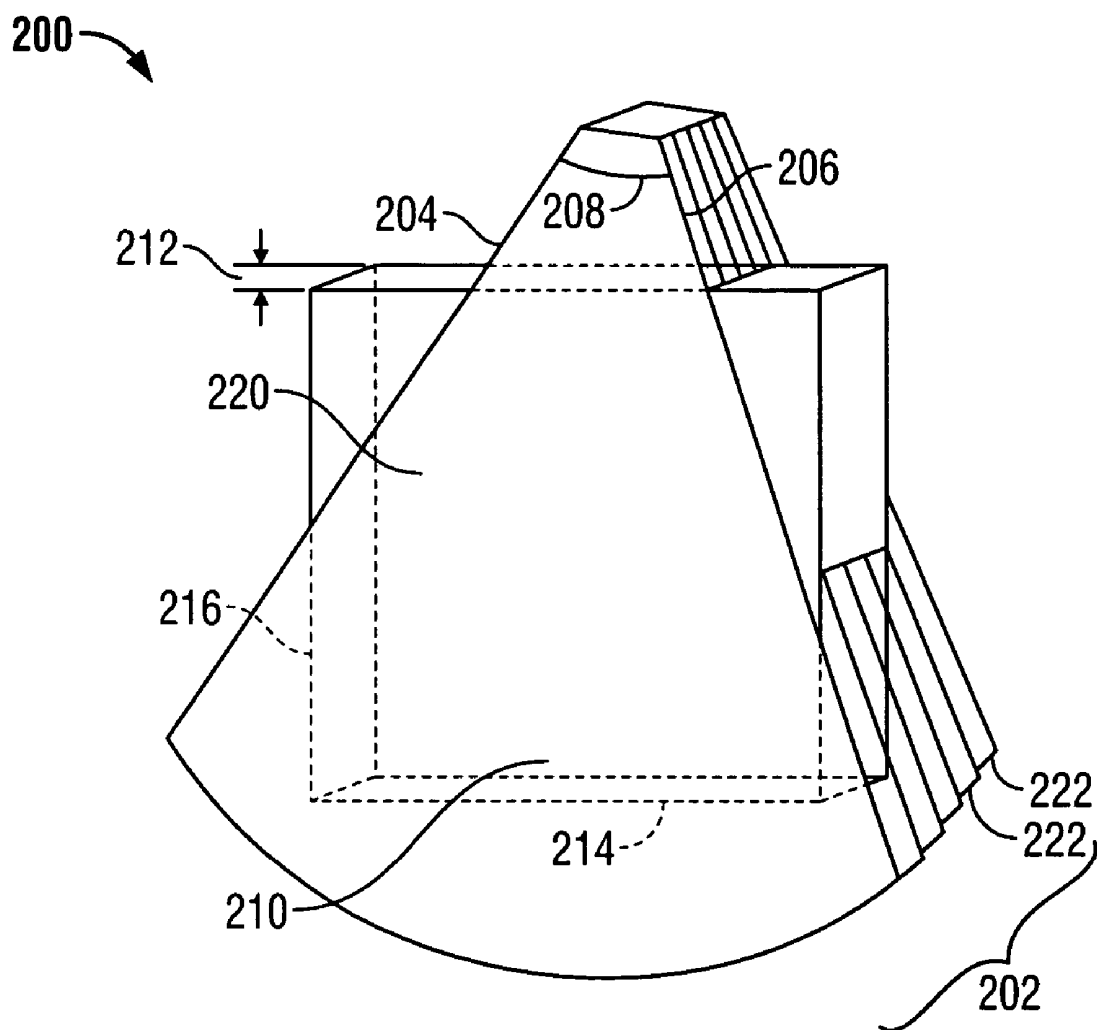


FIG. 3

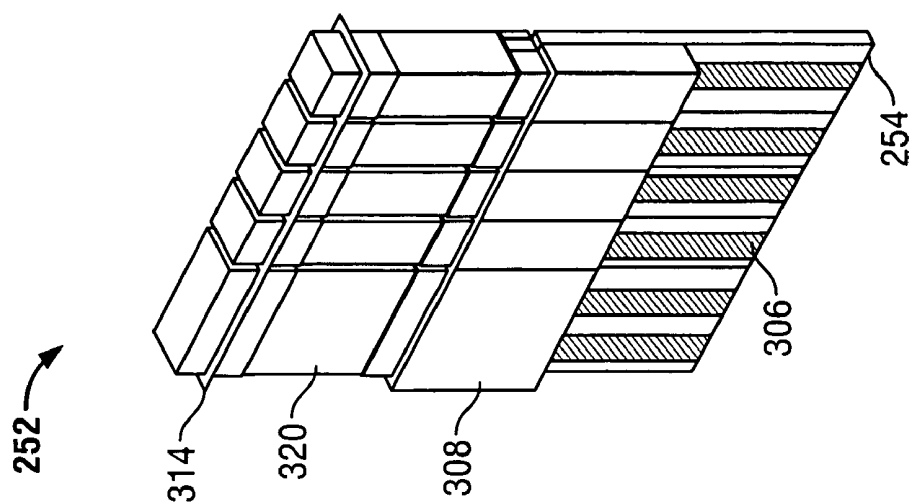


FIG. 6

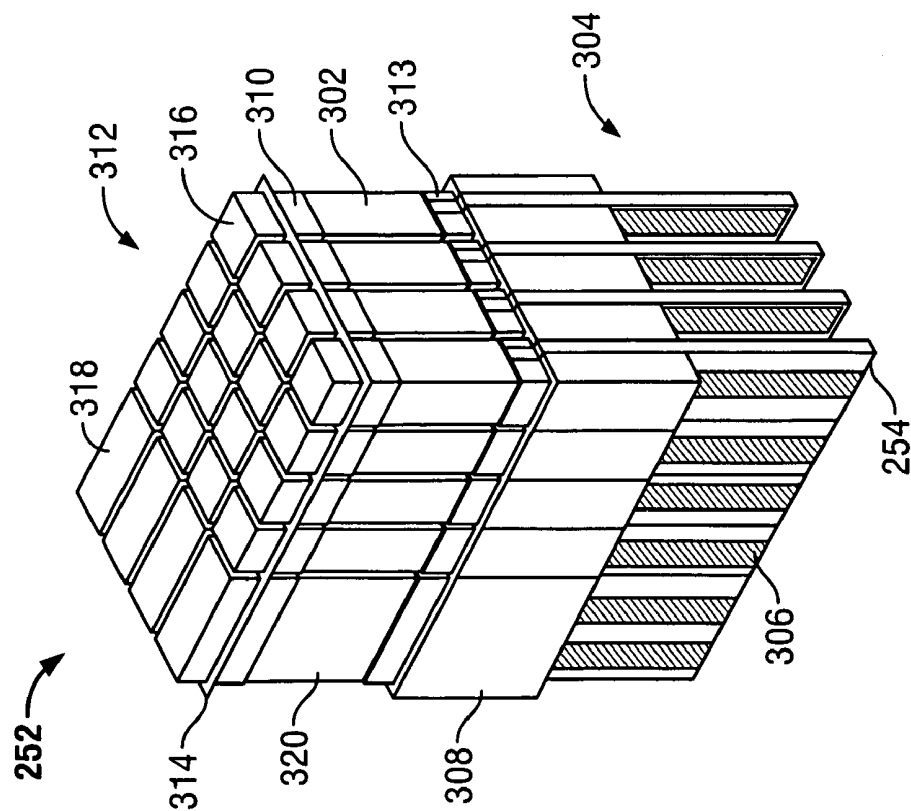
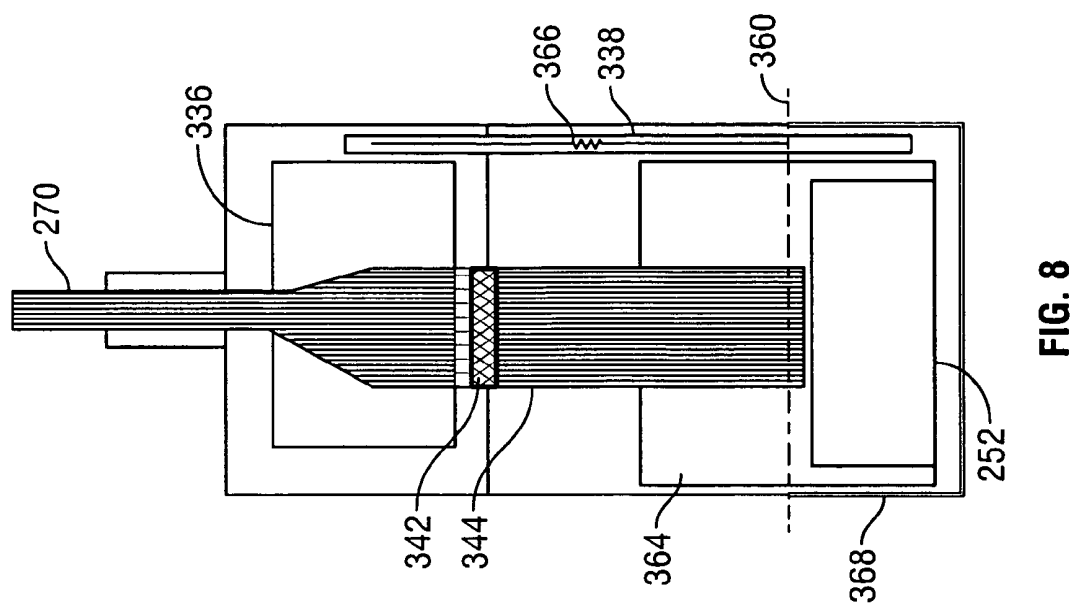
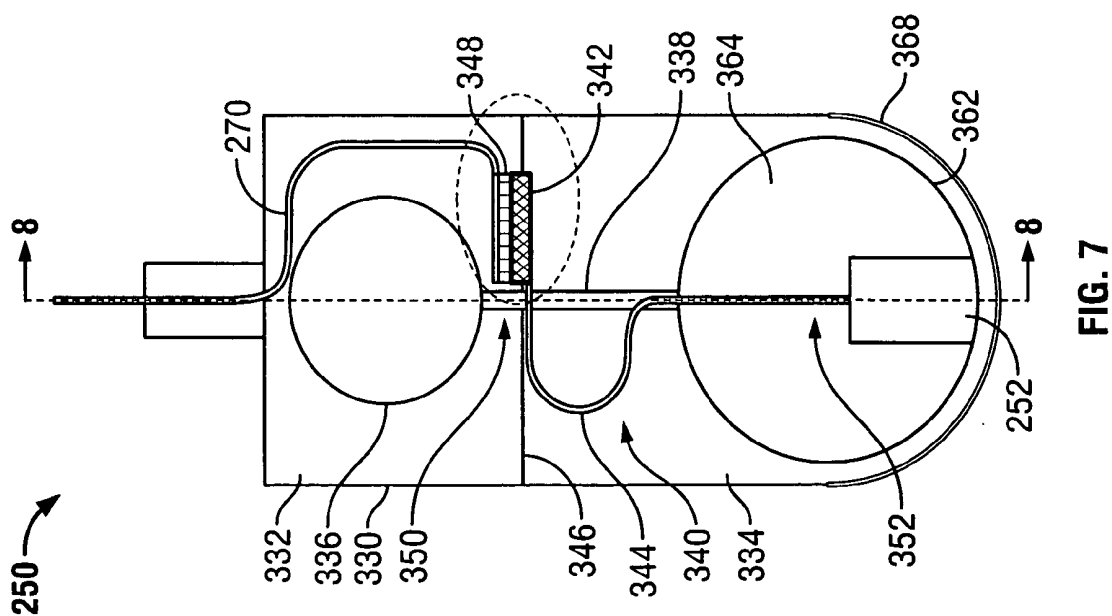


FIG. 5



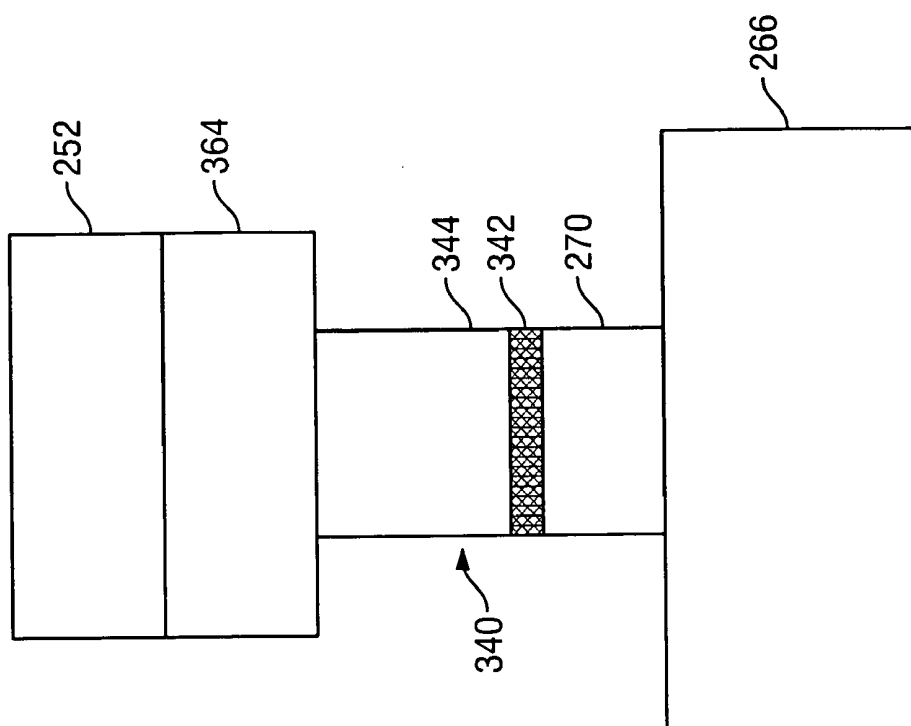


FIG. 10

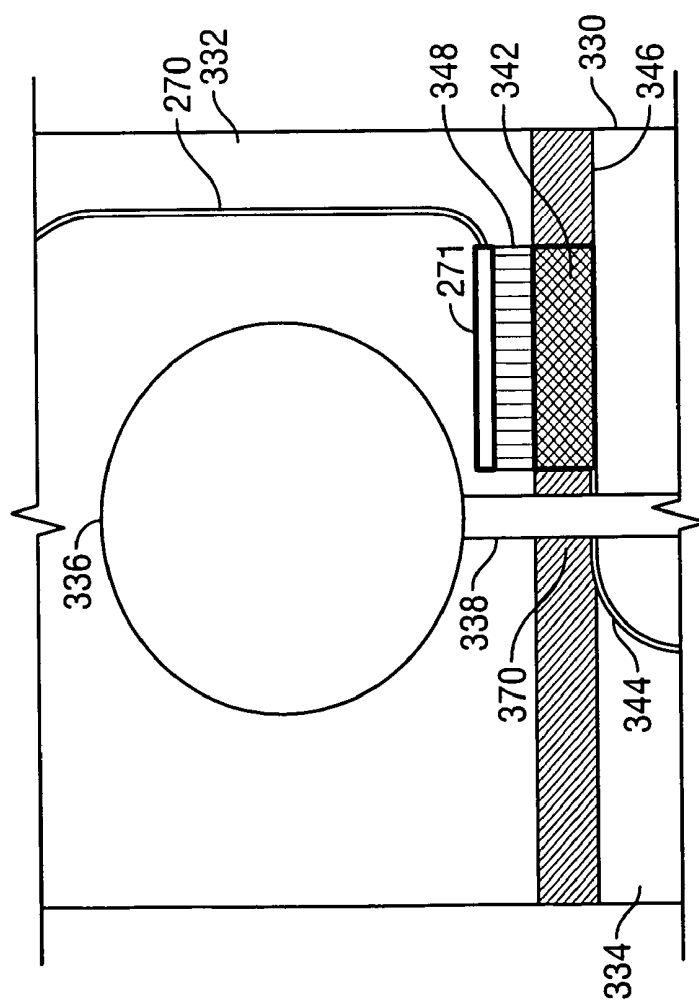


FIG. 9

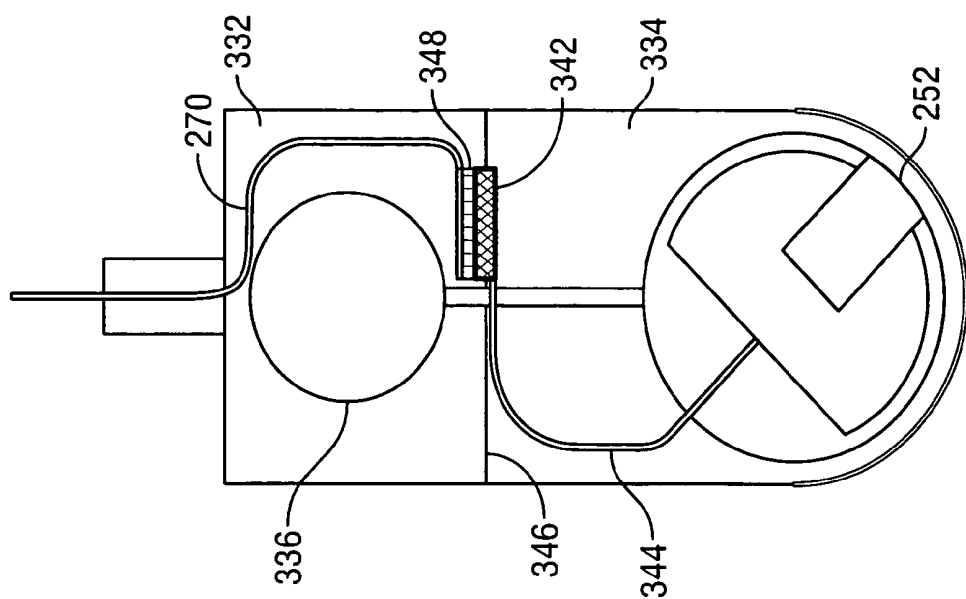


FIG. 11

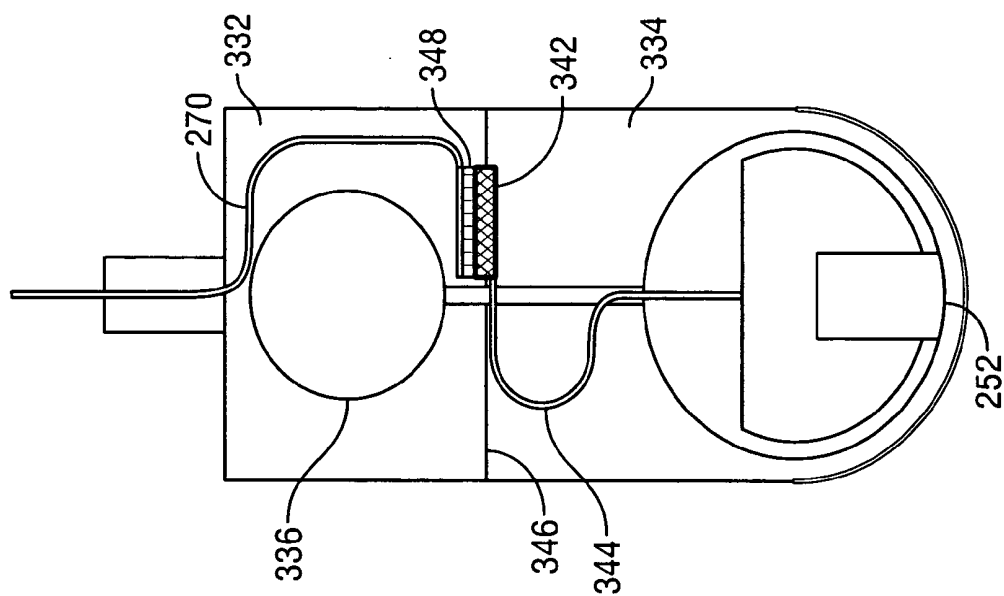


FIG. 12

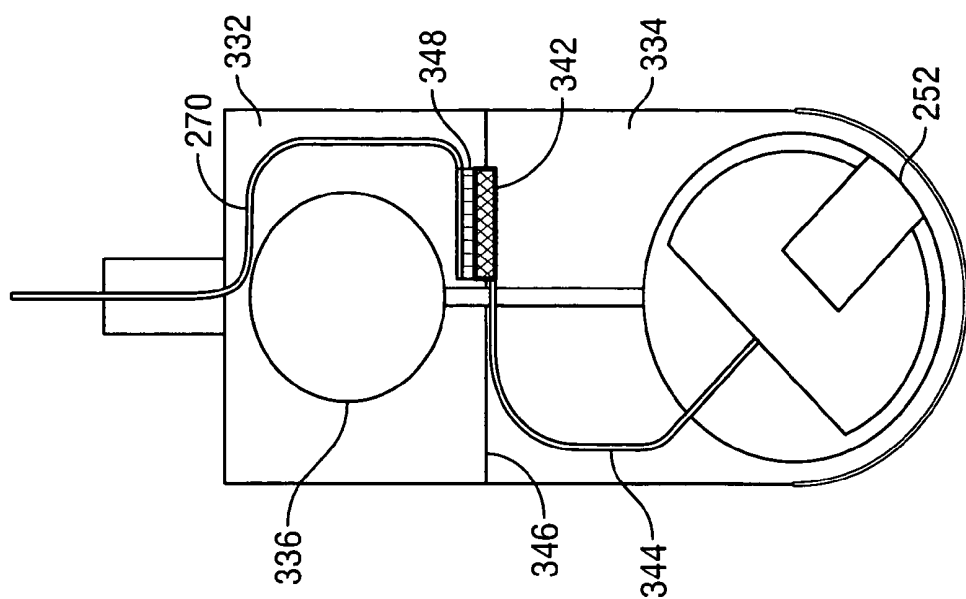


FIG. 13

CONNECTION APPARATUS AND METHOD FOR CONTROLLING AN ULTRASOUND PROBE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part and claims priority to U.S. patent application Ser. No. 10/756,231 filed Jan. 13, 2004 for "APPARATUS AND METHOD FOR CONTROLLING AN ULTRASOUND PROBE," which is hereby incorporated by reference herein in its entirety.

BACKGROUND OF THE INVENTION

[0002] This invention relates generally to ultrasound systems and, more particularly, to probes for ultrasound medical imaging systems.

[0003] Ultrasound systems typically include ultrasound scanning devices, such as, ultrasound probes having different transducers that allow for performing various different ultrasound scans (e.g., different imaging of a volume or body). The ultrasound probes are typically connected to an ultrasound system for controlling the operation of the probes. The probes include a scan head having a plurality of transducer elements (e.g., piezoelectric crystals), which may be arranged in an array. The ultrasound system drives the transducer elements within the array during operation, such as, during a scan of a volume or body, which may be controlled based upon the type of scan to be performed. The ultrasound system includes a plurality of channels for communicating with the probe. For example, the channels may transmit pulses for driving the transducer elements and for receiving signals therefrom.

[0004] In volume probes, wherein the scan head mechanically moves during scan operation, a separate wet and dry chamber are typically provided. In particular, the scan head moves (e.g. rotates) in a sealed wet chamber having an acoustic membrane surrounding a scan head housing that contacts a patient during a scan. The wet chamber is typically filled with an acoustic liquid to allow acoustic coupling during scanning (e.g., during transmissions). The wet chamber is sealed from the dry chamber and may include control components for controlling the operation of the scan head in the wet chamber. The control components communicate with and control the scan head, for example, control the operation of transducer elements within the scan head. The communication between the control components and scan head may be provided by different communication lines (e.g., coaxial or other flexible cable). These communication lines traverse the seal between the wet and dry chambers, requiring the use of sealing members to maintain the liquid tight seal between the chambers. Each sealing member that is required increases the likelihood of a failure, for example, an increased likelihood of liquid leaking into the dry chamber through one of the sealing members. Further, the sealing members add complexity in design and cost to the probe. For example, additional components (e.g., brackets) between the wet and dry chambers may be needed to maintain the position and sealing engagement of the sealing members.

BRIEF DESCRIPTION OF THE INVENTION

[0005] In one exemplary embodiment, an ultrasound probe is provided. The ultrasound probe includes a first

chamber, a second chamber and a sealing member between the first and second chambers. The ultrasound probe further includes a connection member within the second chamber having a rigid portion and a flexible portion, with the rigid portion forming at least part of the sealing member.

[0006] In another exemplary embodiment, a method for controlling an ultrasound probe is provided. The method includes communicating between at least one transducer array and a host system via a connection member, with the connection member formed of a rigid portion and a flexible portion. The flexible portion is configured to connect to the at least one transducer array and the rigid portion forms at least part of a wall between a wet chamber having the at least one transducer array therein and a dry chamber having a system cable therein. The rigid portion is also configured to connect to the system cable, with the system cable connected to the host system. The method further includes controlling elements of the at least one transducer array with the communicating.

BRIEF DESCRIPTION OF THE DRAWINGS

[0007] FIG. 1 is a block diagram of an ultrasound system in accordance with one exemplary embodiment of the present invention.

[0008] FIG. 2 is a block diagram of an ultrasound system in accordance with another exemplary embodiment of the present invention.

[0009] FIG. 3 is a perspective view of an image of an object acquired by the systems of FIGS. 1 and 2 in accordance with an exemplary embodiment of the present invention.

[0010] FIG. 4 is a block diagram of an ultrasound probe in communication with a host system in accordance with an exemplary embodiment of the present invention.

[0011] FIG. 5 is a perspective view of an exemplary transducer stack including an array of transducer elements that may be used in the ultrasound probe shown in FIG. 4.

[0012] FIG. 6 is a perspective view of another exemplary transducer stack including an array of transducer elements that may be used in the ultrasound probe shown in FIG. 4.

[0013] FIG. 7 is a cross-sectional elevation view of a probe in accordance with an exemplary embodiment of the present invention.

[0014] FIG. 8 is an elevation view taken along the line 8-8 of FIG. 7.

[0015] FIG. 9 is a partial cross-sectional elevation view of an ultrasound probe in accordance with an exemplary embodiment of the present invention showing a rigid portion of a connection member forming part of a wall between chambers of the ultrasound probe.

[0016] FIG. 10 is a block diagram showing a connection arrangement for an ultrasound probe in accordance with an exemplary embodiment of the present invention.

[0017] FIGS. 11-13 are cross-sectional elevation views of an ultrasound probe in accordance with an exemplary embodiment of the present invention showing a moving scan head.

DETAILED DESCRIPTION OF THE INVENTION

[0018] Exemplary embodiments of ultrasound systems and methods for controlling ultrasound probes are described in detail below. In particular, a detailed description of exemplary ultrasound systems will first be provided followed by a detailed description of various embodiments of methods and systems for controlling ultrasound probes. A technical effect of the various embodiments of the systems and methods described herein include at least one of improving the sealing arrangement between chambers of an ultrasound probe and allowing for easier maintenance and assembly of the ultrasound probe.

[0019] FIG. 1 illustrates a block diagram of an exemplary embodiment of an ultrasound system 100 that may be used, for example, to acquire and process ultrasonic images. The ultrasound system 100 includes a transmitter 102 that drives an array of elements 104 (e.g., piezoelectric crystals) within or formed as part of a transducer 106 to emit pulsed ultrasonic signals into a body or volume. A variety of geometries may be used and one or more transducers 106 may be provided as part of a probe (not shown). The pulsed ultrasonic signals are back-scattered from density interfaces and/or structures, for example, in a body, like blood cells or muscular tissue, to produce echoes that return to the elements 104. The echoes are received by a receiver 108 and provided to a beamformer 110. The beamformer performs beamforming on the received echoes and outputs an RF signal. The RF signal is then processed by an RF processor 112. The RF processor 112 may include a complex demodulator (not shown) that demodulates the RF signal to form IQ data pairs representative of the echo signals. The RF or IQ signal data then may be routed directly to an RF/IQ buffer 114 for storage (e.g., temporary storage).

[0020] The ultrasound system 100 also includes a signal processor 116 to process the acquired ultrasound information (i.e., RF signal data or IQ data pairs) and prepare frames of ultrasound information for display on a display system 118. The signal processor 116 is adapted to perform one or more processing operations according to a plurality of selectable ultrasound modalities on the acquired ultrasound information. Acquired ultrasound information may be processed in real-time during a scanning session as the echo signals are received. Additionally or alternatively, the ultrasound information may be stored temporarily in the RF/IQ buffer 114 during a scanning session and processed in less than real-time in a live or off-line operation.

[0021] The ultrasound system 100 may continuously acquire ultrasound information at a frame rate that exceeds fifty frames per second, which is the approximate perception rate of the human eye. The acquired ultrasound information is displayed on the display system 118 at a slower frame-rate. An image buffer 122 may be included for storing processed frames of acquired ultrasound information that are not scheduled to be displayed immediately. In an exemplary embodiment, the image buffer 122 is of sufficient capacity to store at least several seconds of frames of ultrasound information. The frames of ultrasound information may be stored in a manner to facilitate retrieval thereof according to their order or time of acquisition. The image buffer 122 may comprise any known data storage medium.

[0022] A user input device 120 may be used to control operation of the ultrasound system 100. The user input

device 120 may be any suitable device and/or user interface for receiving user inputs to control, for example, the type of scan or type of transducer to be used in a scan.

[0023] FIG. 2 illustrates a block diagram of another exemplary embodiment of an ultrasound system 150 that may be used, for example, to acquire and process ultrasonic images. The ultrasound system 150 includes the transducer 106 in communication with the transmitter 102 and receiver 108. The transducer 106 transmits ultrasonic pulses and receives echoes from structures inside a scanned ultrasound volume 152. A memory 154 stores ultrasound data from the receiver 108 derived from the scanned ultrasound volume 152. The scanned ultrasound volume 152 may be obtained by various techniques, including, for example, 3D scanning, real-time 3D imaging, volume scanning, scanning with transducers having positioning sensors, freehand scanning using a Voxel correlation technique, 2D scanning or scanning with a matrix of array transducers, among others.

[0024] The transducer 106 is moved, such as along a linear or arcuate path, while scanning a region of interest (ROI). At each linear or arcuate position, the transducer 106 obtains a plurality of scan planes 156. The scan planes 156 are collected for a thickness, such as from a group or set of adjacent scan planes 156. The scan planes 156 are stored in the memory 154, and then provided to a volume scan converter 168. In some exemplary embodiments, the transducer 106 may obtain lines instead of the scan planes 156, with the memory 154 storing lines obtained by the transducer 106 rather than the scan planes 156. The volume scan converter 168 receives a slice thickness setting from a slice thickness setting control 158, which identifies the thickness of a slice to be created from the scan planes 156. The volume scan converter 168 creates a data slice from multiple adjacent scan planes 156. The number of adjacent scan planes 156 that are obtained to form each data slice is dependent upon the thickness selected by the slice thickness setting control 158. The data slice is stored in a slice memory 160 and accessed by a volume rendering processor 162. The volume rendering processor 162 performs volume rendering upon the data slice. The output of the volume rendering processor 162 is provided to a video processor 164 that processes the volume rendered data slice for display on a display 166.

[0025] It should be noted that the position of each echo signal sample (Voxel) is defined in terms of geometrical accuracy (i.e., the distance from one Voxel to the next) and one or more ultrasonic responses (and derived values from the ultrasonic response). Suitable ultrasonic responses include gray scale values, color flow values, and angio or power Doppler information. It should be noted that the ultrasound system 150 also may include a user input or user interface for controlling the operation of the ultrasound system 150.

[0026] It should be noted that the ultrasound systems 100 and 150 may include additional or different components. For example, the ultrasound system 150 may include a user interface or user input 120 (shown in FIG. 1) to control the operation of the ultrasound system 150, including, to control the input of patient data, scan parameters, a change of scan mode, and the like.

[0027] FIG. 3 illustrates an exemplary image of an object 200 that may be acquired by the ultrasound systems 100 and

150. The object **200** includes a volume **202** defined by a plurality of sector shaped cross-sections with radial borders **204** and **206** diverging from one another at an angle **208**. The transducer **106** (shown in **FIGS. 1 and 2**) electronically focuses and directs ultrasound firings longitudinally to scan along adjacent scan lines in each scan plane **156** (shown in **FIG. 2**) and electronically or mechanically focuses and directs ultrasound firings laterally to scan adjacent scan planes **156**. The scan planes **156** obtained by the transducer **106**, and as illustrated in **FIG. 1**, are stored in the memory **154** and are scan converted from spherical to Cartesian coordinates by the volume scan converter **168**. A volume comprising multiple scan planes **156** is output from the volume scan converter **168** and stored in the slice memory **160** as a rendering region **210**. The rendering region **210** in the slice memory **160** is formed from multiple adjacent scan planes **156**.

[**0028**] The rendering region **210** may be defined in size by an operator using a user interface or input to have a slice thickness **212**, width **214** and height **216**. The volume scan converter **168** (shown in **FIG. 2**) may be controlled by the slice thickness setting control **158** (shown in **FIG. 2**) to adjust the thickness parameter of the slice to form a rendering region **210** of the desired thickness. The rendering region **210** defines the portion of the scanned ultrasound volume **152** that is volume rendered. The volume rendering processor **162** accesses the slice memory **160** and renders along the slice thickness **212** of the rendering region **210**.

[**0029**] Referring now to **FIGS. 1 and 2**, during operation, a slice having a pre-defined, substantially constant thickness (also referred to as the rendering region **210**) is determined by the slice thickness setting control **158** and is processed in the volume scan converter **168**. The echo data representing the rendering region **210** (shown in **FIG. 3**) may be stored in the slice memory **160**. Predefined thicknesses between about 2 mm and about 20 mm are typical, however, thicknesses less than about 2 mm or greater than about 20 mm may also be suitable depending on the application and the size of the area to be scanned. The slice thickness setting control **158** may include a control member, such as a rotatable knob with discrete or continuous thickness settings.

[**0030**] The volume rendering processor **162** projects the rendering region **210** onto an image portion **220** of an image plane(s) **222** (shown in **FIG. 3**). Following processing in the volume rendering processor **162**, pixel data in the image portion **220** may be processed by the video processor **164** and then displayed on the display **166**. The rendering region **210** may be located at any position and oriented at any direction within the volume **202**. In some situations, depending on the size of the region being scanned, it may be advantageous for the rendering region **210** to be only a small portion of the volume **202**.

[**0031**] **FIG. 4** illustrates a block diagram of an exemplary embodiment of an ultrasound probe **250** that may be used in connection with the ultrasound systems **100** or **150**. The ultrasound probe **250** includes a transducer array and backing stack **252** (the "transducer array **252**"), transducer flex cables **254**, which may be formed as a scan head cable, and multiple processing boards **256** that support processing electronics. Each processing board **256** may include a location memory **258** (which may include geometry RAM,

encoder RAM, location registers and control registers as noted below) and signal processors **260**. A location memory controller **262** (e.g., a general purpose CPU, microcontroller, PLD, or the like) also may be provided and includes a communication interface **264**.

[**0032**] The communication interface **264** establishes data exchange with a host system **266** over communication lines **268** (e.g., digital signal lines) and through a system cable **270**. Additionally, in an exemplary embodiment, the system cable **270** includes coaxial cables **272** that connect to the processing boards **256** to communicate transmit pulse waveforms to the transducer array **252** and communicate receive signals, after beamforming, to the host system **266**. The probe **250** also may include a connector **274**, through which the probe **250** connects to the host system **266**.

[**0033**] A clamp **276** may be provided to hold the transducer flex cables **254** against the processing boards **256**. The clamp **276** thereby aids in establishing electrical connectivity between the transducer flex cables **254** and the processing boards **256**. The clamp **276** may include a dowel pin **278** and a bolt **280**, although other implementations are also suitable.

[**0034**] The transducer array **252** is bonded onto the backing stack, as will be described in more detail below with regard to **FIG. 5**. The transducer flex cables **254** provide electrical signal connections through the backing stack. In one exemplary embodiment, there are forty-two transducer flex cables **254**, each with fifty signal connections. Thus, the transducer flex cables **254** support transmit and receive signal connections for as many as **2100** transducer elements in the transducer array **252**, although fewer may be used. For example, each processing board **256** may couple to six transducer flex cables **254**, and thereby includes signal connections for **300** transducer elements.

[**0035**] The processing boards **256** may, like the flex cables **254**, be formed from a flex material, such as, for example, polyimide, polyester, etc. The processing boards **256** include the processing electronics for the transducer array **252**, including the signal processors **260** that perform beamforming on the receive apertures in the transducer array **252**.

[**0036**] Each signal processor **260** may handle, for example, four receive apertures defined at selected spatial locations on the transducer array **252**. The receive apertures may be triangular apertures that include fifteen acoustic transducer elements arranged, for example, as a row of five elements above a row of four elements above a row of three elements above a row of two elements above a row of one element. Furthermore, each processing board **256** may include five signal processors **260**. Thus, in the receive direction, each processing board **256** may process twenty receive apertures, each including fifteen acoustic transducer elements.

[**0037**] For every ultrasound beam, the location memory controller **262** connects via digital signal lines **273** (e.g., carried by a separate flex cable) to each location memory **258** on each processing board **256**. The location memory controller **262** communicates the spatial location information into each location memory **258** for each receive aperture processed by the signal processors **260** on the processing boards **256**. The digital signal lines **273** may include, for example, a clock line for each processing board **256**, a serial

command data line for each processing board **256**, two data lines (for a total of fourteen data lines) connected to each processing board **256**, an output enable for one or more of the signal processors **260**, and a test signal.

[0038] The location memory controller **262** communicates with the host system **266** over the digital signal lines **273** that may form part of, for example, a synchronous serial port. To that end, the communication interface **264** and digital signal lines **273** may implement a low voltage differential signal interface, for example, including a coaxial cable with a grounded shield and center signal wire. The location memory controller **262** includes a block of cache memory **275**, for example, 1-8 MBytes of static random access memory (SRAM).

[0039] FIG. 5 shows one exemplary embodiment of the transducer array **252**. The transducer array **252** includes piezoelectric ceramic **302** that converts electrical-to-acoustic and acoustic-to-electrical energy. The piezoelectric ceramic **302** is located within the center of the transducer array **252**. On the signal side, the piezoelectric ceramic **302** is attached to a z-axis backing block **304** comprised of alternating layers of transducer flex cables **254** and acoustic absorbing material **308** bonded into the solid backing block **304**.

[0040] The backing block **304** is cut in a direction perpendicular to the orientation of the transducer flex cables **254** thereby exposing the ends of the individual transducer flex cable **254** circuit traces **306** to provide for high density signal connection. The ceramic **302**, an electrically conductive inner acoustic matching layer **310** (e.g., a metal filled graphite such as Antimony-Graphite), and the top surface of the backing block **304** are diced in one operation to form discrete acoustic transducer elements **312** centered over each of the flex circuit traces **306** in the transducer flex cables **254**. Thus, there is a signal plane **313** on the z-axis backing block **304**.

[0041] Each circuit trace **306** contacts the bottom, or signal side, of one transducer element **312**. A ground metal layer **314** is coated onto one side of the outer acoustic matching layer **316**, which may be formed from a plastic. This matching layer **316** is attached to the top of each element **312** to form a ground connection across the face of the transducer array **252**. The outer matching layer **316** is partially diced to separate it into discrete elements, thereby improving the acceptable angle of the transducer element **312**. In one exemplary embodiment, however, the dicing does not penetrate to the ground metal layer **314**.

[0042] The electrical ground connection to each transducer element **312** is made via the outermost elements **318** in the transducer. A wraparound ground **320** on the ceramic **302** is also provided. Once the transducer array **252** is mounted into a scan head or head shell, a thin silicone protective facing may be applied.

[0043] It should be noted that different transducer arrays that may have different interconnections may be used as desired or needed (e.g., based upon the probe type or application). For example, FIG. 5 shows an interconnection configuration suitable for arrays requiring an electrical interface of very high density (e.g., two-dimensional (2D) arrays). However, other types of arrays, for example, one-dimensional (1D) arrays, do not require electrical interfaces

of this high density and other interconnection configurations may be more suitable. For example, as shown in FIG. 6, in a 1D array application, the 1D array includes a single transducer flex cable **254** wherein the circuit traces **306** contact the elements of the transducer array **252**. The elements of the transducer array **252** are positioned adjacent each other as the circuit traces **306** on the transducer flex cable **254** are positioned adjacent each other. Similar configurations with a single transducer flex cable **254** may be used, for example, with 1.25D, 1.5D or 1.75D arrays.

[0044] FIGS. 7 and 8 illustrate an exemplary embodiment of the probe **250**, and in particular, a volume imaging probe, having a transducer array **252** in communication with a host system **266** (shown in FIG. 4). The probe **250** includes a housing **330** having a first chamber **332** (e.g., a dry chamber) and a second chamber **334** (e.g., a wet chamber). The first chamber **332** and second chamber **334** may be formed as a single unit (e.g., unitary construction) or may be formed as separate units connected together (e.g. modular design). In an exemplary embodiment, the first chamber **332** is a dry or air chamber having contained therein drive means for mechanically controlling the transducer array **252** and communication means for electrically controlling the transducer array **252**. The drive means generally includes a motor **336** (e.g., stepper motor) and a gear arrangement **338**, such as a two-stage gear arrangement having a belt drive and a rope drive. The communication means generally includes the system cable **270** that communicates with the host system **266** to drive the elements of the transducer array **252** (e.g., selectively activate the elements of the transducer array **252**).

[0045] It should be noted that although the drive means and communication means are described herein having specific component parts, they are not so limited. For example, the drive means may have a different gear arrangement and the communication means may have different connection members or transmission lines.

[0046] In this exemplary embodiment, the second chamber **334** is a wet chamber (e.g., chamber having acoustic liquid therein) having contained therein transducer driving means for moving (e.g., rotating) the transducer array **252** and transducer control means for selectively driving elements of the transducer array **252** (e.g., the piezoelectric ceramics **302**). The transducer driving means generally includes a drive shaft **360** in connection with a scan head housing **362**, supported, for example, on brackets (not shown), that operates to move the transducer array **252** as part of a scan head **364** when driven by the drive means. A support member (not shown) also may be provided for supporting the scan head housing **362** and a biasing spring **366** may be provided, for example, to ensure proper tension on the drive means and transducer drive means. It should be noted that an acoustic membrane **368** may be provided surrounding the scan head housing **362** and formed as part of the housing **330**.

[0047] The transducer control means generally includes a connection member **340** having one or more communication lines for connecting the system cable **270** and the transducer array **252**, and providing communication therebetween. In one exemplary embodiment, the connection member **340** is formed from a printed circuit board having a rigid portion **342** (e.g., rigid printed circuit board portion) and a flexible

portion **344** (e.g., flexible printed circuit board portion). However, it should be noted that the connection member **340** may be formed of any suitable material and/or component parts as desired or needed. In general, the rigid portion **342** and the flexible portion **344** are formed to have a flexibility/rigidity as desired or needed, for example, based upon the type of probe or application. For example, the elastic modulus or mean elastic modulus of the rigid portion **342** and the flexible portion **344** may be determined by the wiring layout of the printed circuit board portion as a result of the distribution of metal layers on the printed circuit board, which may be selected based upon the type of probe. Thus, the material flexibility/rigidity of the rigid portion **342** and flexible portion **344** may be varied as desired or needed. In general, the rigid portion **342** is formed such that it provides sufficient stability from its stiffness or rigidity (e.g., rigid printed circuit board portion) to ensure proper sealing and/or functioning of a probe (e.g., fluid impervious seal between the first chamber **332** and the second chamber **334**). In general, the flexible portion **344** is formed such that it provides sufficient flexibility and durability to ensure proper functioning and/or operation of a probe (e.g., to ensure proper and reliable interconnection between the rigid portion **342** and a moving transducer array **252**).

[0048] The rigid portion **342** forms part of a sealing member **346**, such as, for example, a wall (e.g., fluid impervious wall) between the first chamber **332** and second chamber **334**. The rigid portion **342** may be integrally formed with the sealing member **346** or may be provided in sealing engagement therewith, for example, using adhesive sealing (e.g., epoxy) or other sealing members (e.g., O-rings). In the various exemplary embodiments, the rigid portion **342** and sealing member **346** are a single unitary structure. It should be noted that additional members (e.g., brackets) may be provided in connection with the sealing member **346** to provide mechanical stability for bearing mechanical loads that may be applied to the rigid portion **342** and provide additional pressure on the sealing member **346**. For example, a mechanical load may be applied to the rigid portion **342** by the flexible portion **344** or an interconnection member **348**. The mechanical load may result, for example, from the movement of the flexible portion **344** as described herein, by a differential pressure between the first chamber **332** and second chamber **334**, and by tensions of the system cable **270** that are induced into the rigid portion **342** via the interconnection member **348**, among others.

[0049] At a first portion **350** (e.g., first end) of the connection member **340**, the rigid portion **342** is connected via the interconnection member **348** (e.g., board-to-board connector) to the system cable **270**. At a second portion **352** (e.g., second end) of the connection member **340**, the flexible portion **344** is connected to the transducer array **252**. It should be noted that additional or different connectors may be used to connect to the first portion **350** and second portion **352**. The connection member **340** thereby provides communication between the transducer array **252** and the host system **266** via the system cable **270**. However, additional or different control members may be provided, such as, for example, multiplexing circuits connected to the transducer array **252** for controlling the operation of the elements of the transducer array **252**.

[0050] It should be noted that although the transducer driving means and transducer control means are described

herein having specific component parts, they are not so limited. For example, the transducer driving means may have a different shaft arrangement and the transducer control means may have different control circuits or transmission lines. It also should be noted that additional or different component parts may be provided in connection with the probe **250** as needed or desired, and/or based upon the particular type and application of the probe **250**. For example, a lens covering the transducer array **252** may be provided based upon the type of probe **250**.

[0051] In an exemplary embodiment, and as shown in FIG. 9, the first chamber **332** and second chamber **334** are separated by the sealing member **346** (e.g., fluid impervious wall), with the rigid portion **342** forming a part of the sealing member **346**. The sealing member **346** provides a liquid tight sealing arrangement between the first chamber **332** and the second chamber **334** and may be integrally formed as part of one of the first and second chambers **332** and **334**. One or more slots or openings **370** may be provided as part of the sealing member **346** to allow for passage there-through, for example, of a portion of the drive means (e.g., rope portion of a rope drive). The slots or openings **370** are sealed, for example, with a sealing gasket, epoxy or other suitable sealing member to ensure proper sealing between the first chamber **332** and second chamber **334**. It should be noted that the system cable **270** may include a connector end **271** for connection to the interconnection member **348**.

[0052] Thus, as shown in FIG. 10, the transducer array **252** is connected via the connection member **340** to the system cable **270**. Specifically, the flexible portion **344** connects to the transducer array **252** and the rigid portion **342** connects to the system cable **270**. The system cable **270** then connects to the host system **266**.

[0053] The connection member **340** allows for communication with and control of the operation of the elements of a moving transducer array **252** (e.g., selectively driving the elements of the transducer array **252**) as shown in FIGS. 11-13. The connection member **340** also provides an improved sealing arrangement and more modular probe design (e.g., two chambers removably connectable). It should be noted that the transducer array **252** may be configured for operation in different modes, such as, for example, a 1D, 1.25D, 1.5D, 1.75D and 2D mode of operation.

[0054] While the invention has been described in terms of various specific embodiments, those skilled in the art will recognize that the invention can be practiced with modification within the spirit and scope of the claims.

What is claimed is:

1. An ultrasound probe comprising:

a first chamber;

a second chamber;

a sealing member between the first and second chambers; and

a connection member within the second chamber having a rigid portion and a flexible portion, the rigid portion forming at least part of the sealing member.

2. An ultrasound probe in accordance with claim 1 wherein the sealing member comprises a wall between the first and second chambers.

3. An ultrasound probe in accordance with claim 1 wherein the first chamber is a dry chamber and the second chamber is a wet chamber.

4. An ultrasound probe in accordance with claim 1 wherein the connection member comprises a printed circuit board.

5. An ultrasound probe in accordance with claim 1 wherein the rigid portion comprises a rigid printed circuit board and the flexible portion comprises a flexible printed circuit board.

6. An ultrasound probe in accordance with claim 1 wherein the rigid portion is configured to connect to a system cable in the first chamber and the flexible portion is configured to connect to a transducer array in the second chamber.

7. An ultrasound probe in accordance with claim 1 wherein the rigid portion is configured to connect to a system cable in the first chamber and the flexible portion is configured to connect to a transducer array in the second chamber, the transducer array provided as part of a scan head configured to move within the second chamber.

8. An ultrasound probe in accordance with claim 1 wherein the rigid portion is integrally formed with the sealing member.

9. An ultrasound probe in accordance with claim 1 wherein the rigid portion is sealingly engaged with the sealing member.

10. An ultrasound probe in accordance with claim 1 further comprising an interconnection member to connect the rigid portion to a system cable within the first chamber.

11. An ultrasound probe in accordance with claim 1 wherein the sealing member comprise at least one opening.

12. An ultrasound probe in accordance with claim 1 wherein the first and second chambers are formed in a unitary construction.

13. An ultrasound probe in accordance with claim 1 wherein the first and second chambers are formed in a modular construction.

14. An ultrasound probe in accordance with claim 1 wherein the ultrasound probe is configured to operate in at least one of a 1D, 1.25D, 1.5D, 1.75D and 2D mode of operation.

15. An ultrasound probe comprising:

a dry chamber having drive means for mechanically controlling at least one transducer and communication means for electrically controlling the at least one transducer; and

a wet chamber having a connection member formed of a rigid portion and a flexible portion, the rigid portion forming at least part of a wall between the wet and dry chambers and configured to connect to the communication means, and the flexible portion configured to connect to the at least one transducer.

16. An ultrasound probe in accordance with claim 15 wherein the communication means comprises a system cable.

17. An ultrasound probe in accordance with claim 15 wherein the drive means comprises a motor and gear arrangement.

18. An ultrasound probe in accordance with claim 15 wherein the connection member further comprises a printed circuit board.

19. An ultrasound probe in accordance with claim 15 wherein the dry and wet chambers are configured to connect in a modular arrangement.

20. A connection member for an ultrasound probe, the connection member comprising:

a flexible portion within a wet chamber configured to connect to at least one transducer; and

a rigid portion forming at least part of a sealing member between the wet chamber and a dry chamber, the rigid portion configured to connect to a system cable in the dry chamber.

21. A connection member in accordance with claim 20 wherein the flexible portion and rigid portion each comprise a printed circuit board.

22. A method for controlling an ultrasound probe, the method comprising:

communicating between at least one transducer array and a host system via a connection member, the connection member formed of a rigid portion and a flexible portion, the flexible portion configured to connect to the at least one transducer array, the rigid portion forming at least part of a wall between a wet chamber having the at least one transducer array therein and a dry chamber having a system cable therein, the rigid portion configured to connect to the system cable, with the system cable connected to the host system; and

controlling elements of the at least one transducer array with the communicating.

23. A method in accordance with claim 22 wherein the connection member comprises a printed circuit board.

* * * * *

专利名称(译)	连接装置和用于控制超声探头的方法		
公开(公告)号	US20050154311A1	公开(公告)日	2005-07-14
申请号	US10/767585	申请日	2004-01-29
[标]申请(专利权)人(译)	BRUESTLE REINHOLD		
申请(专利权)人(译)	BRUESTLE REINHOLD		
当前申请(专利权)人(译)	通用电气医疗系统全球性技术公司，有限责任公司		
[标]发明人	BRUESTLE REINHOLD		
发明人	BRUESTLE, REINHOLD		
IPC分类号	A61B8/00 A61B8/14 G01S7/521 G01S15/89 G10K11/35		
CPC分类号	A61B8/14 G01S7/52079 G01S15/8915 G10K11/352 G01S15/8925		
其他公开文献	US7494469		
外部链接	Espacenet USPTO		

摘要(译)

提供了一种用于控制超声探头的连接装置和方法。超声探头包括第一腔室，第二腔室和位于第一腔室和第二腔室之间的密封构件。超声探头还包括在第二腔室内的连接构件，该连接构件具有刚性部分和柔性部分，刚性部分形成密封构件的至少一部分。

