



US006641540B2

(12) **United States Patent**
Fleischman et al.

(10) **Patent No.:** **US 6,641,540 B2**
(45) **Date of Patent:** **Nov. 4, 2003**

(54) **MINIATURE ULTRASOUND TRANSDUCER**

- (75) Inventors: **Aaron J. Fleischman**, University Heights, OH (US); **Shuvo Roy**, Cleveland, OH (US); **Geoffrey R. Lockwood**, Kingston (CA)
- (73) Assignee: **The Cleveland Clinic Foundation**, Cleveland, OH (US)
- (*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 12 days.

(21) Appl. No.: **09/948,068**

(22) Filed: **Sep. 6, 2001**

(65) **Prior Publication Data**

US 2002/0077551 A1 Jun. 20, 2002

Related U.S. Application Data

- (60) Provisional application No. 60/250,775, filed on Dec. 1, 2000.

(51) **Int. Cl.⁷** **A61B 8/14**

(52) **U.S. Cl.** **600/459; 600/462; 600/466; 73/587**

(58) **Field of Search** **600/437-472**

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,917,097 A	4/1990	Proudian, deceased et al.	
5,167,233 A	12/1992	Eberle et al.	
5,311,095 A	5/1994	Smith et al.	
5,938,615 A	8/1999	Eberle et al.	
6,011,855 A	1/2000	Selfridge et al.	
6,049,158 A	4/2000	Takeuchi et al.	
6,070,468 A *	6/2000	Degertekin et al.	73/644
6,151,967 A *	11/2000	McIntosh et al.	73/514.32
6,221,015 B1	4/2001	Yock	
6,246,898 B1	6/2001	Vesely et al.	
6,328,696 B1 *	12/2001	Fraser	600/459
6,328,697 B1 *	12/2001	Fraser	600/459
6,443,901 B1 *	9/2002	Fraser	600/459

OTHER PUBLICATIONS

Ladabaum, I., Jin, X., Soh, H.T., Atalar, A., Khuri-Yakub, B.T., Surface Micromachined Capacitive Ultrasonic Transducers, IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control, vol. 45, No. 3, May 1998, p. 678-690.*
Jin, X.C.; Ladabaum, I.; Khuri-Yakub, B.T., Surface micro-machined capacitive ultrasonic immersion transducers, Micro Electro Mechanical Systems, 1998. MEMS 98. Proceedings., The Eleventh Annual International Workshop on, 1998, p. 649-654.*

Bauer, F.; Simonne, J. J.; and Audaire, L., Ferroelectric Copolymer and IR Sensor Technology Applied to Obstacle Detection, in IEEE, pp. 27-30 (1992).

Fiorillo, A.; Dario, P.; Van Der Spiegel, J.; Domenici, C.; and Foo, J., Spinned P(VDF-TrFE) CoPolymer Layer for a Silicon-Piezoelectric Integrated US Transducer, in Ultrasonics Symposium, pp. 667-670 (1987).

Fiorillo, A. S.; Van Der Spiegel, J.; Bloomfield, P. E.; and Esmail-Zandi, D., A P(VDF-TrFE)-Based Integrated Ultrasonic Transducer, in Sensors and Actuators, pp. 719-725 (1990).

(List continued on next page.)

Primary Examiner—Marvin M. Lateef


Assistant Examiner—William C. Jung

(74) *Attorney, Agent, or Firm*—Tarolli, Sundheim, Covell & Tummino L.L.P.

(57) **ABSTRACT**

An ultrasonic transducer (108) for use in medical imaging comprises a substrate (300) having first and second surfaces. The substrate (300) includes an aperture (301) extending from the first surface to the second surface. Electronic circuitry (302) is located on the first surface. A diaphragm (304) is positioned at least partially within the aperture (301) and in electrical communication with the electronic circuitry (302). The diaphragm (304) has an arcuate shape, formed by applying a differential pressure, that is a section of a sphere. A binder material (314) is in physical communication with the diaphragm (304) and the substrate (300).

33 Claims, 12 Drawing Sheets

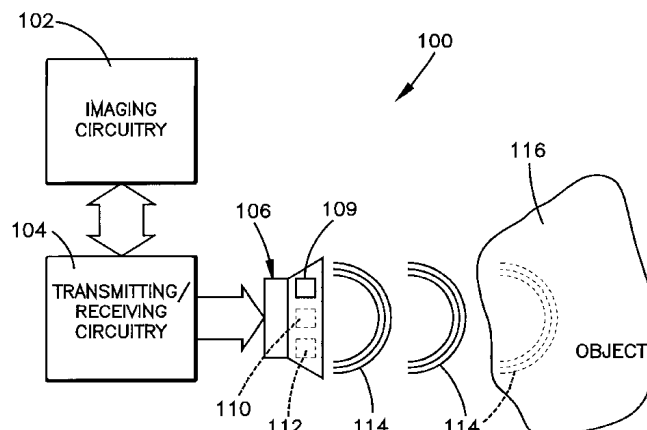

OTHER PUBLICATIONS

Lockwood, G. R.; Ryan, L. K.; Hunt, J. W. ;and Foster, F. S., Measurement of the Ultrasonic Properties of Vascular Tissues and Blood from 36–65 MHz, in *Ultrasound in Med. & Biol.*, vol. 17, No. 7, pp. 653–666.

Mo, Jian-Hua; Robinson, Andrew L.; Fitting, Dale W.; Terry, Jr., Fred L.; and Carson, Paul L., Micromachining for Improvement of Integrated Ultrasonic Transducer Sensitivity, in *IEEE Transactions on Electron Devices*, vol. 37, No. 1, pp. 134–139 (1990).

Mo, Jian-Hua; Fowlkes, J. Brian; Robinson, Andrew L.; and Carson, Paul L., Crosstalk Reduction with a Micromachined Diaphragm Structure for Integrated Ultrasound Transducer Arrays, in *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 39, No. 1, pp. 48–53 (1992).

Seip, Ralf; VanBaren, Philip; and Ebbini, Emad S., Dynamic Focusing in Ultrasound Hyperthermia Treatments Using Implantable Hydrophone Arrays, in *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 41, No. 5, pp. 706–713 (1994).

Sherar, M. D. and Foster, F. S., The Design and Fabrication of High Frequency Poly(Vinylidene Fluoride) Transducers, in *Ultrasonic Imaging*, vol. 11, pp. 75–94 (1989).

Sleva, Michael Z.; Hunt, William D.; and Briggs, Ronald D., Focusing Performance of Epoxy– and Air–Backed Polyvinylidene Fluoride Fresnel Zone Plates, in *J. Acoust. Soc. Am.*, vol. 96, No. 3, pp. 1627–1633 (1994).

Swartz, Robert G. and Plummer, James D., Integrated Silicon–PVF2 Acoustic Transducer Arrays, in *IEEE Transactions on Electron Devices*, vol. ED–26, No. 12, pp. 1921–1931 (1979).

Waller, D. and Safari, A., Corona Poling of PZT Ceramics and Flexible Piezoelectric Composites, in *Ferroelectrics*, vol. 87, pp. 189–195 (1988).

Sleva, Michael Z.; Briggs, Ronald D.; and Hunt, William D., A Micromachined Poly(vinylidene Fluoride–trifluoroethylene) Transducer for Pulse–Echo Ultrasound Applications, in *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, vol. 43, No. 2, pp. 257–262, Mar. 1996.

* cited by examiner

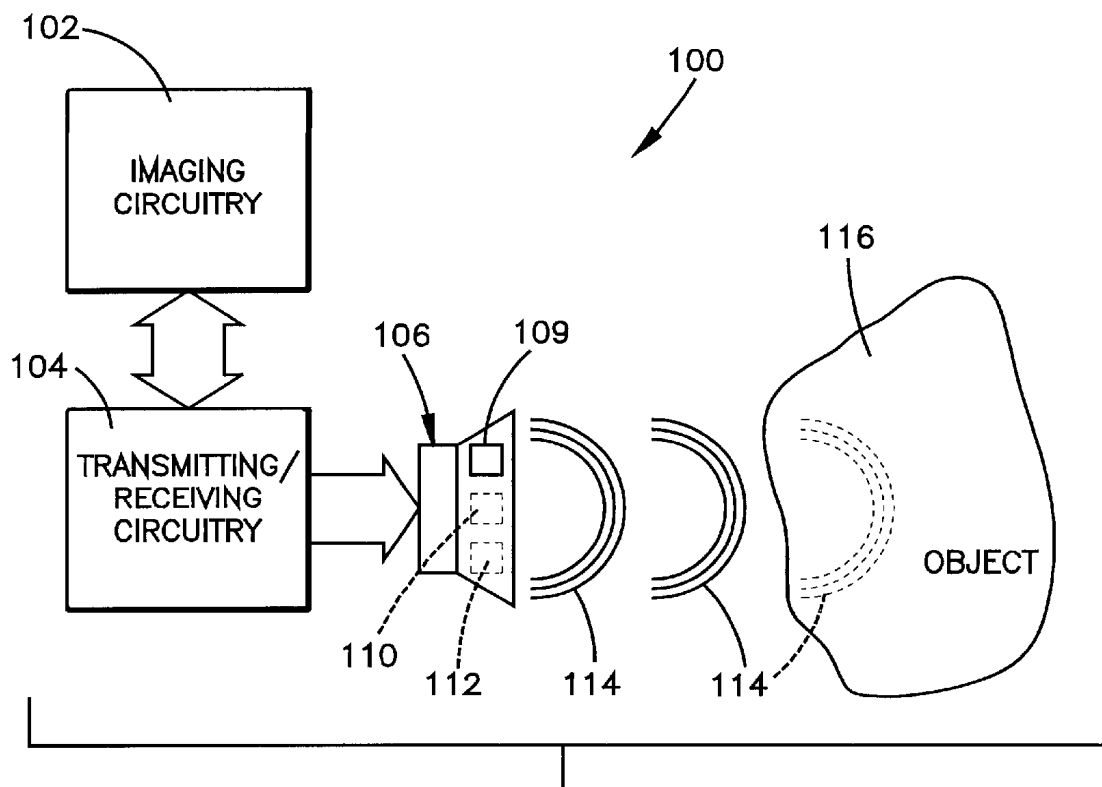


Fig.1

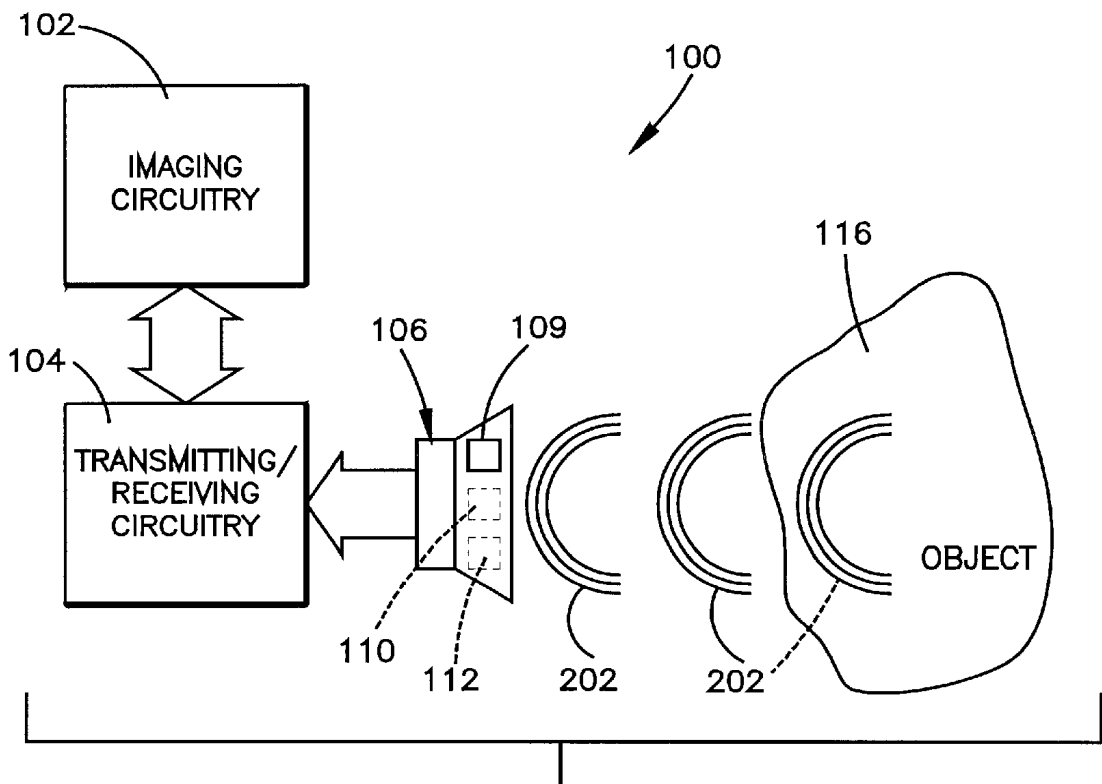


Fig.2

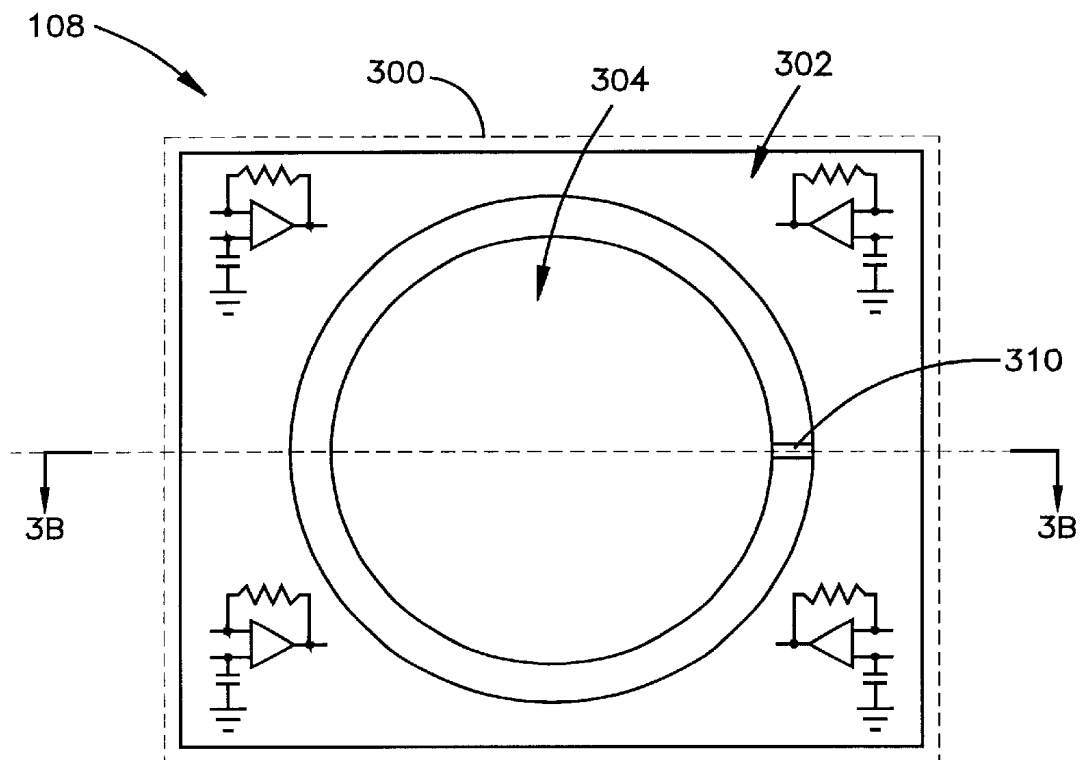


Fig.3A

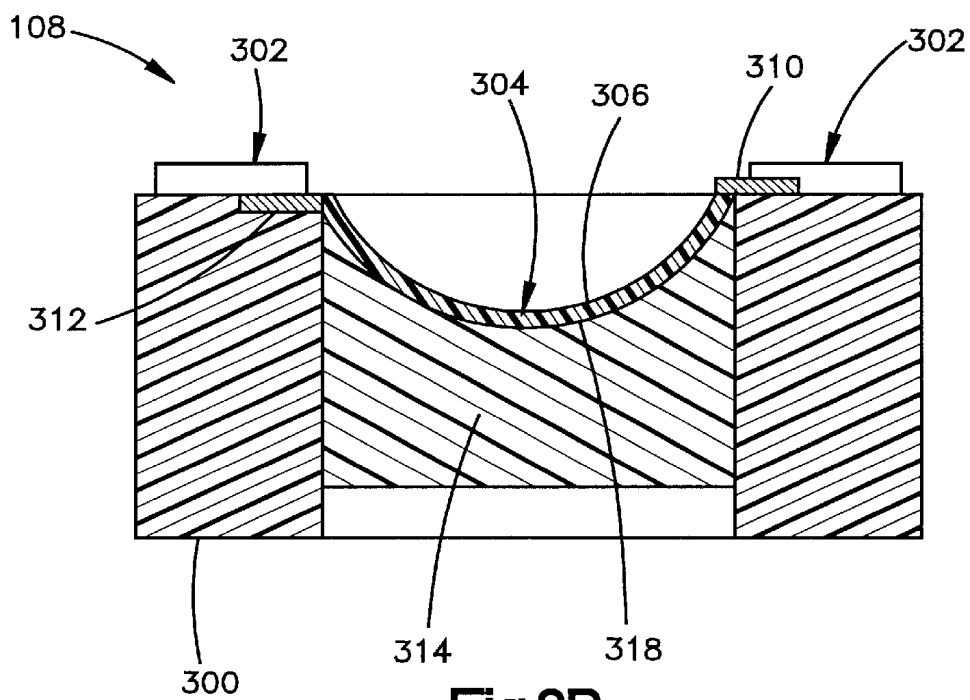
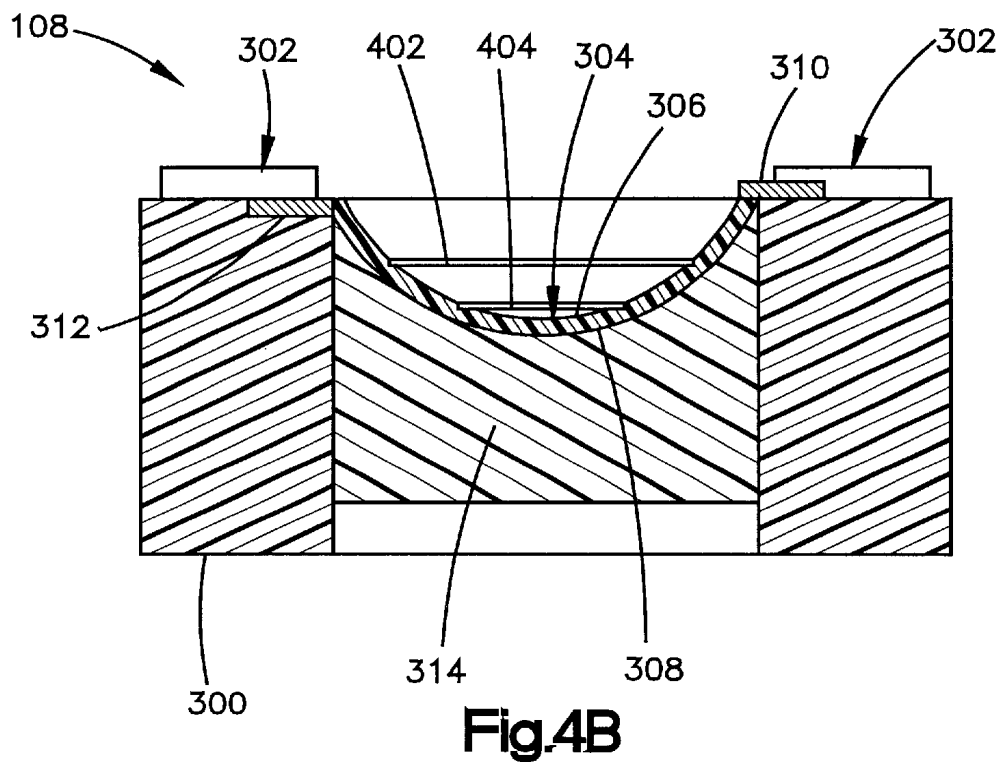
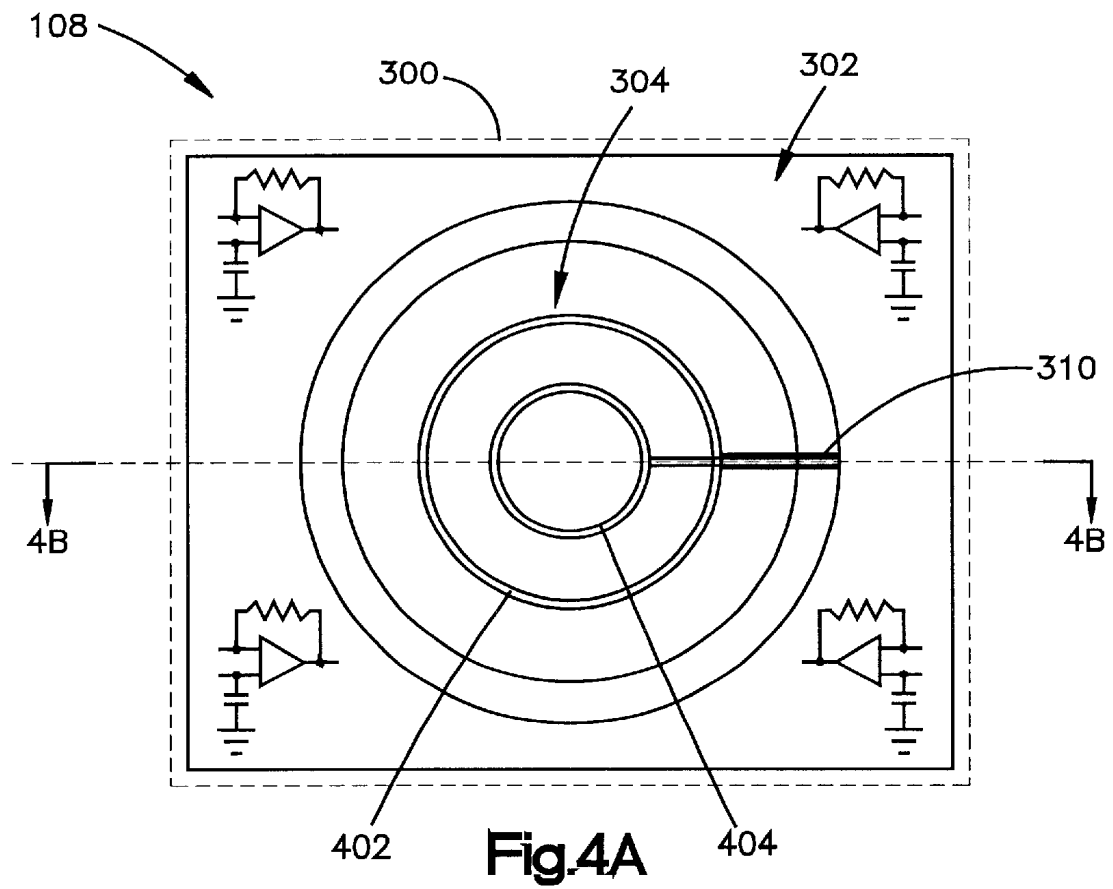


Fig.3B



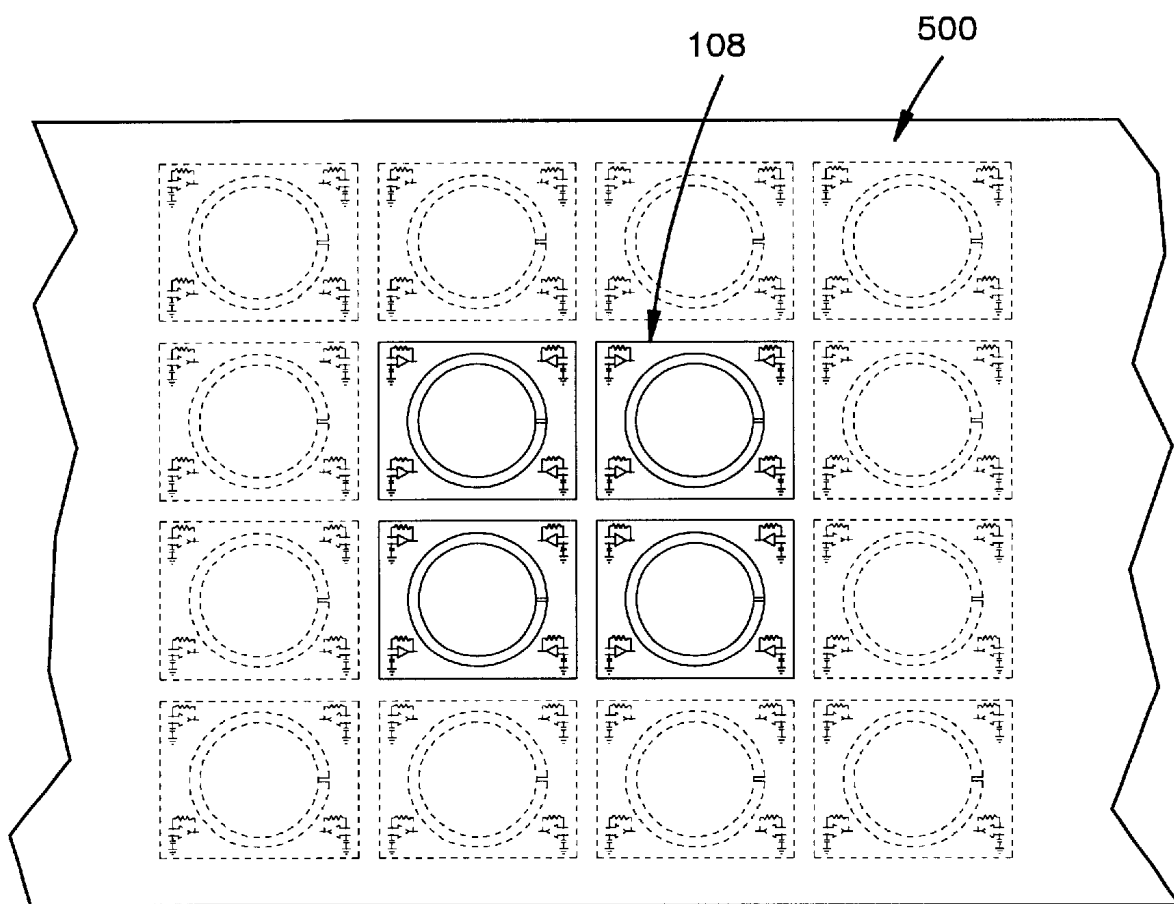


Fig.5

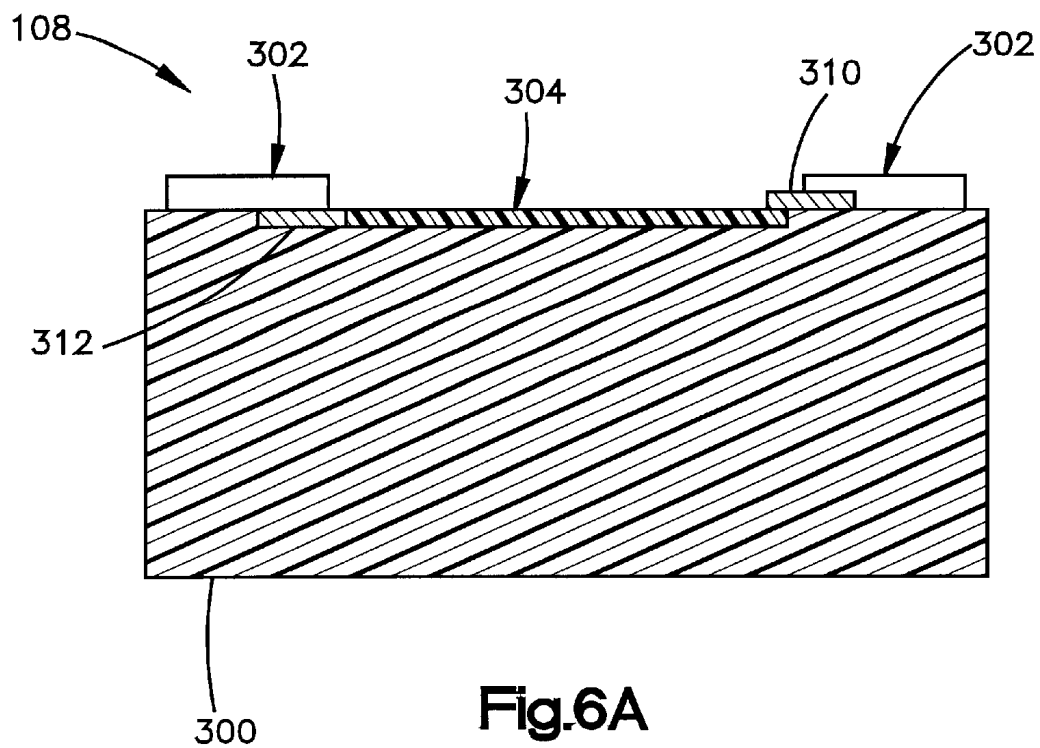


Fig.6A

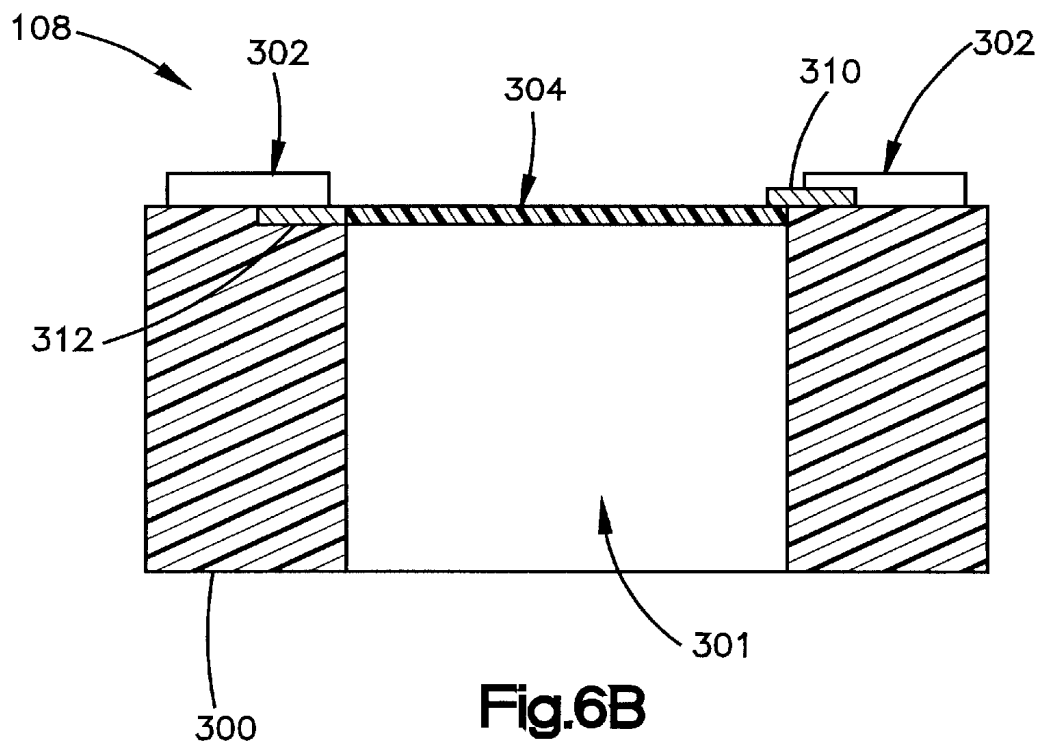
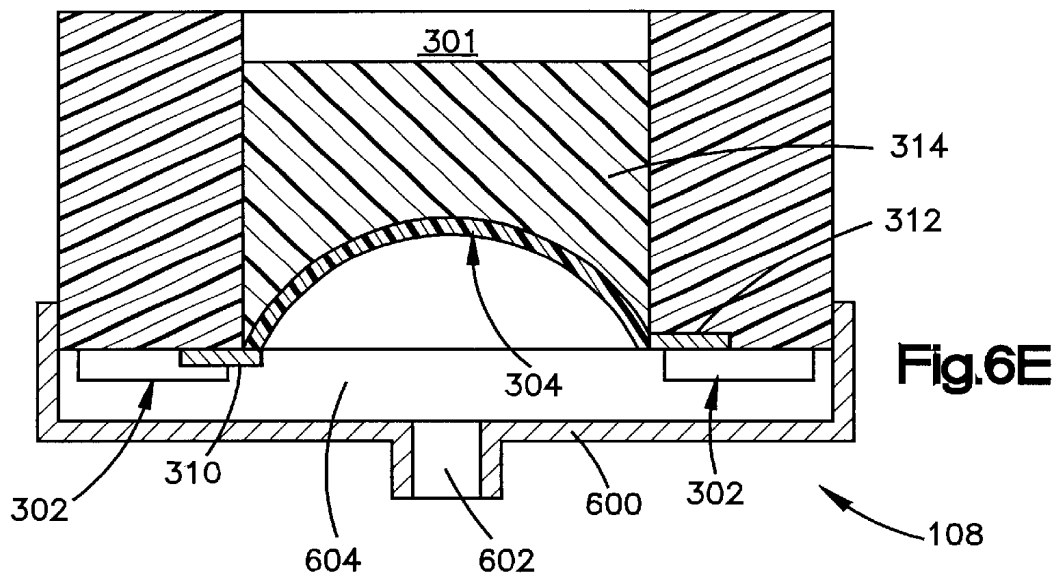
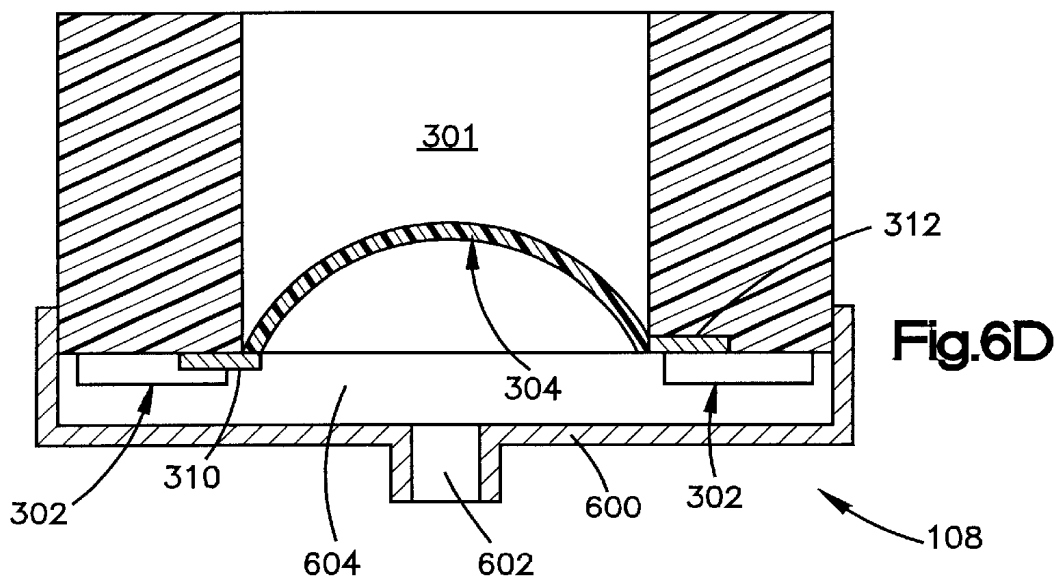
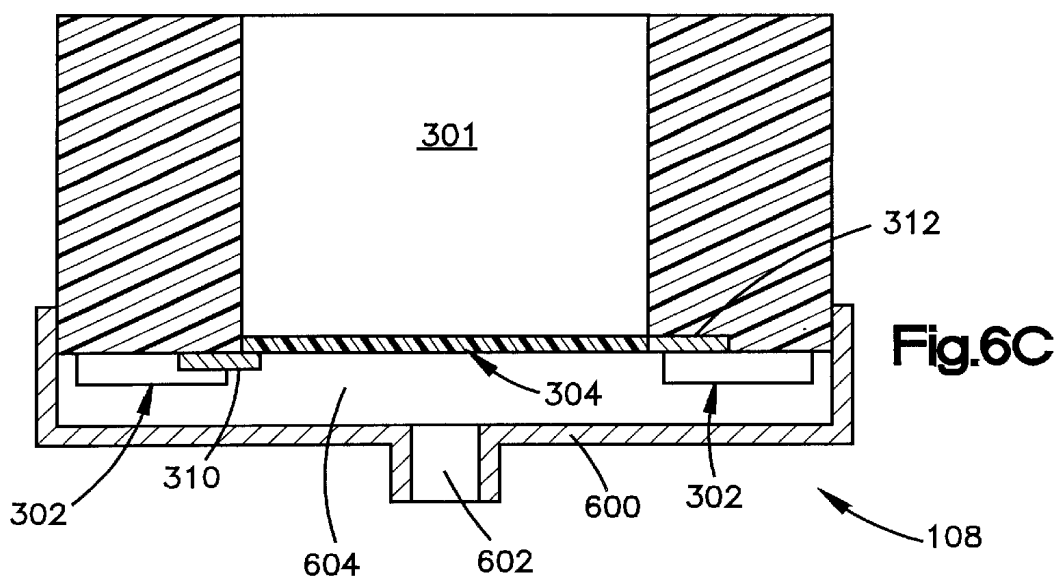
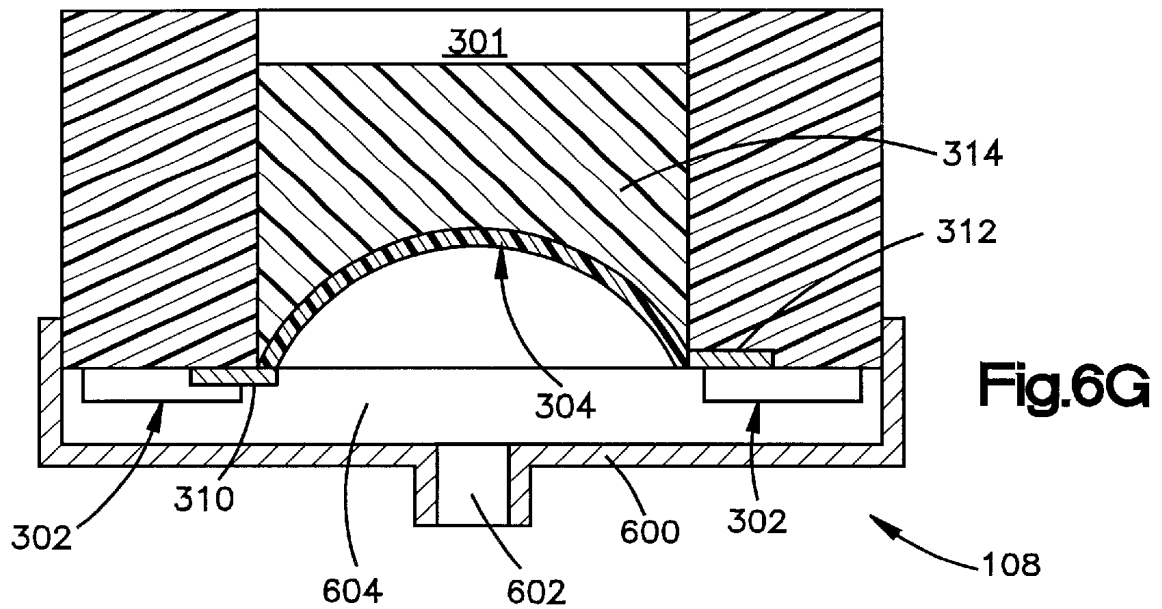
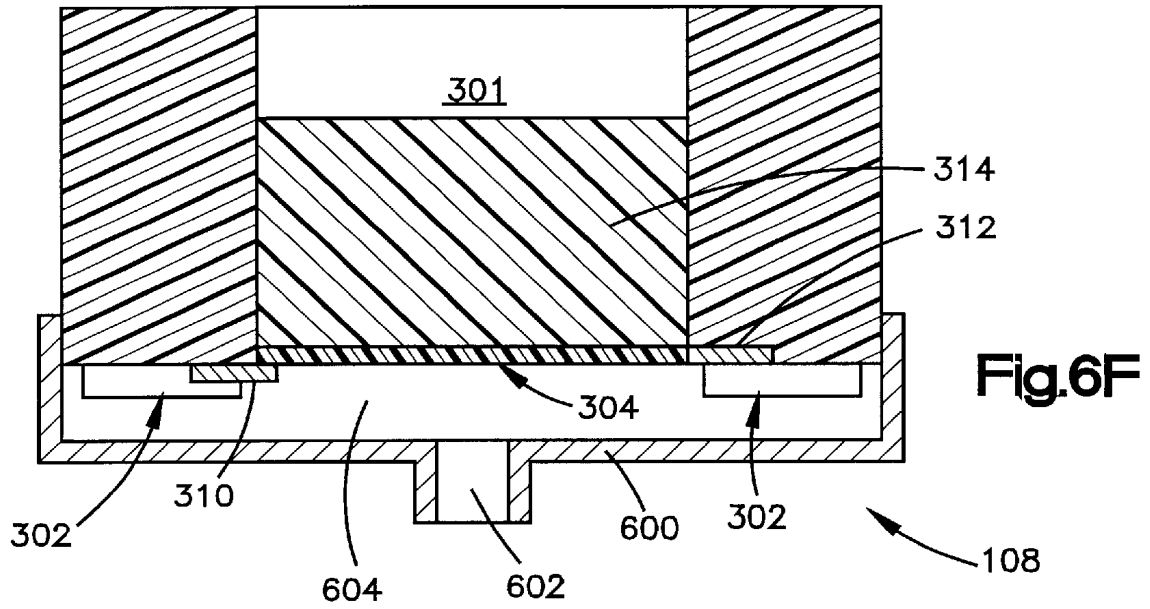


Fig.6B





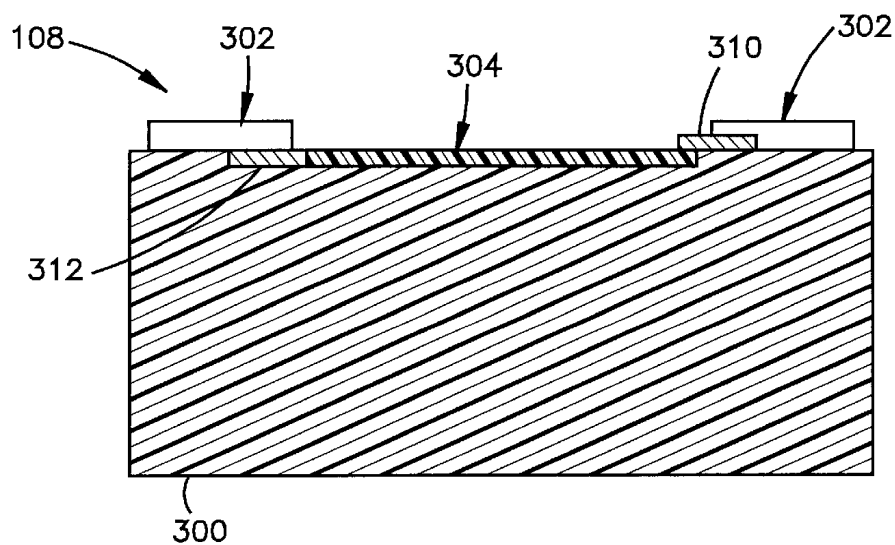


Fig.7A

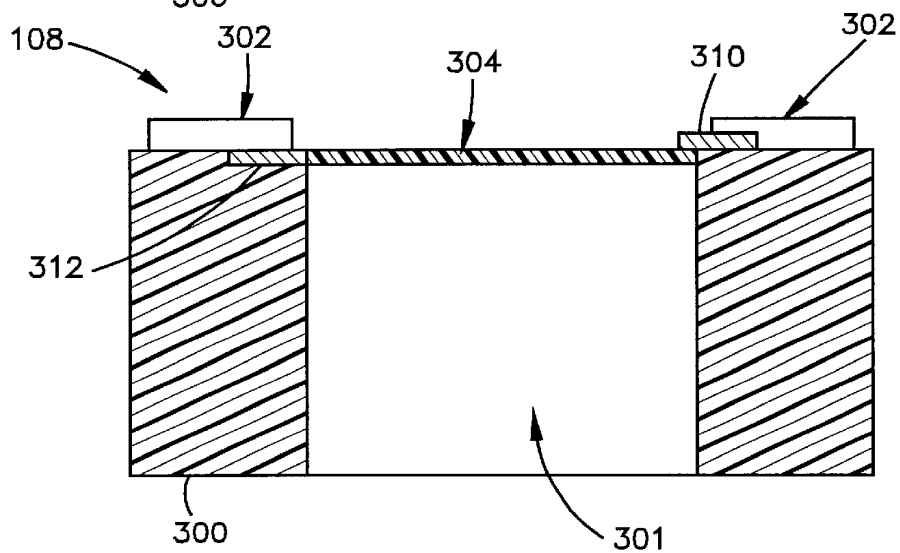


Fig.7B











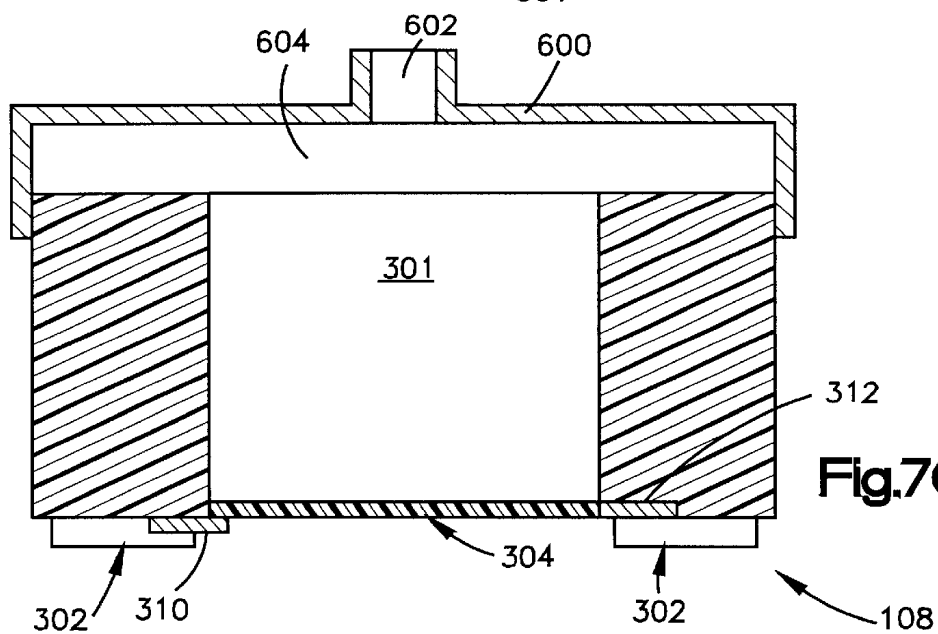


Fig.7C

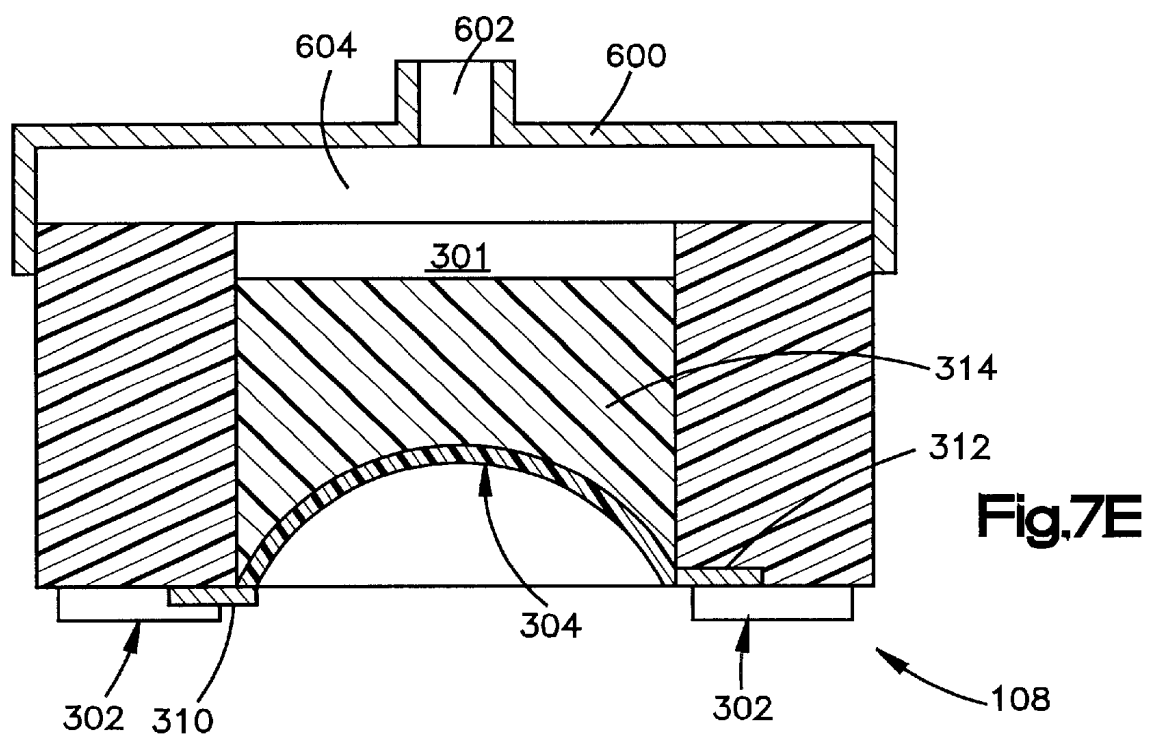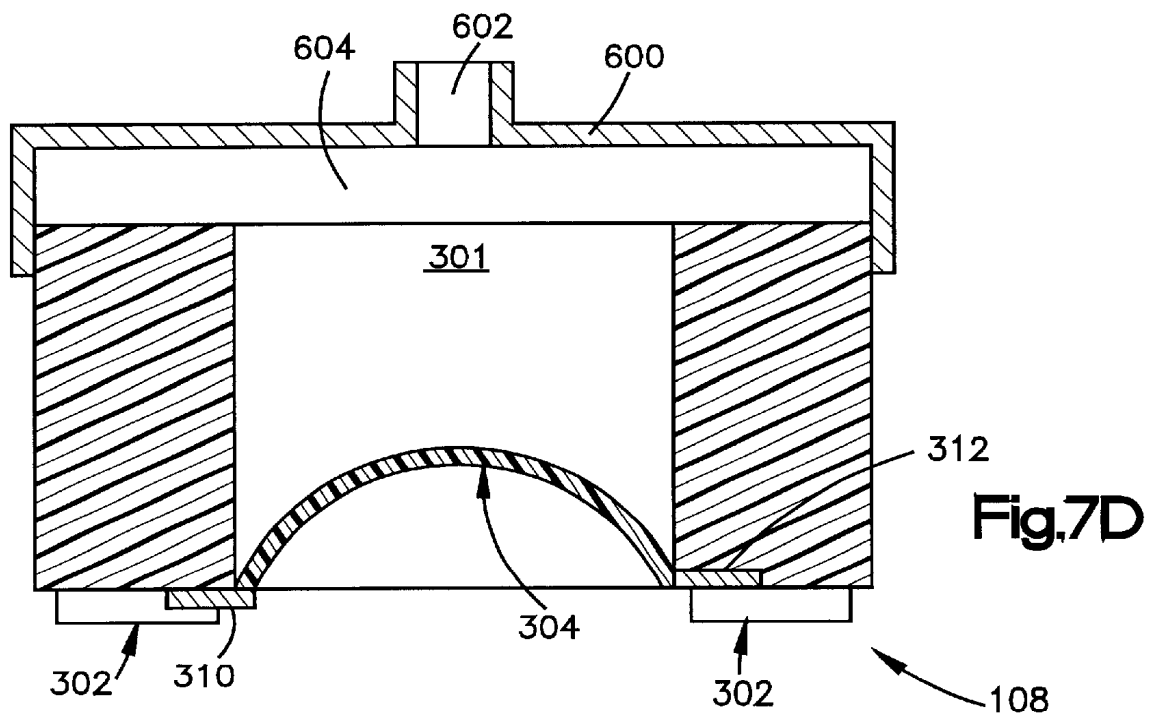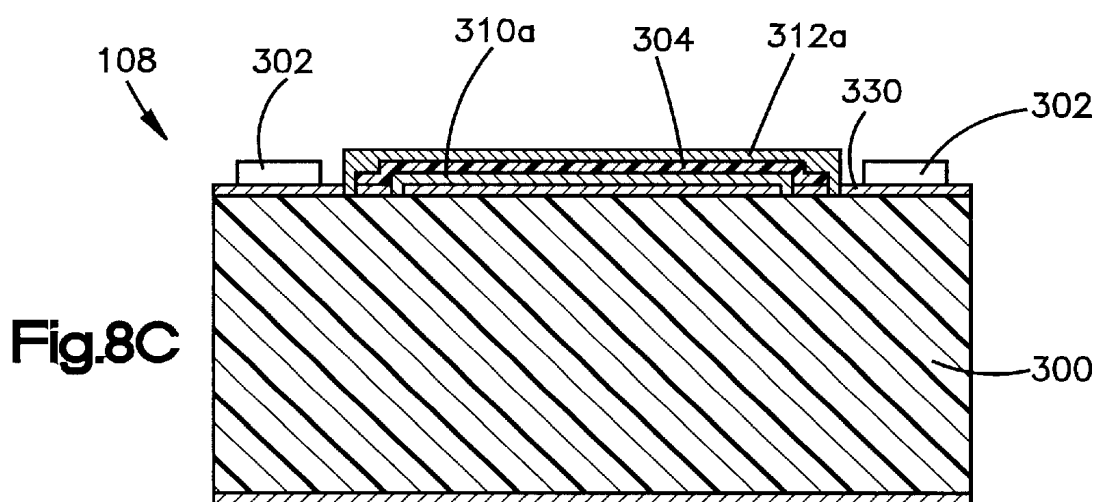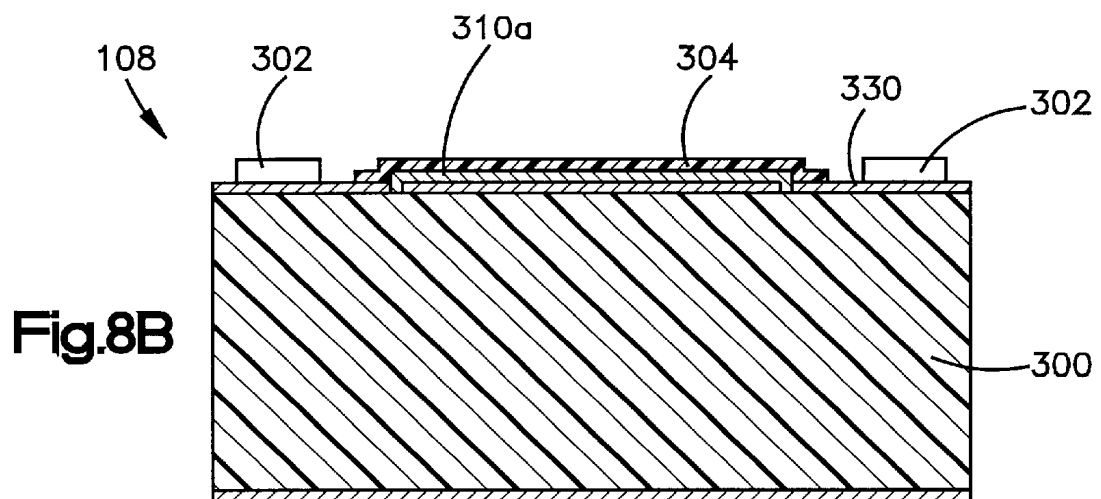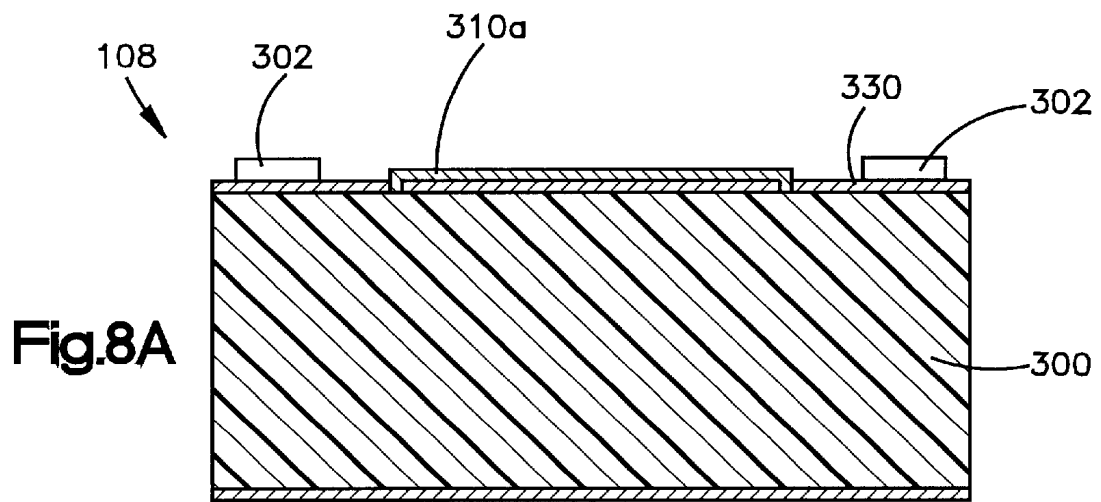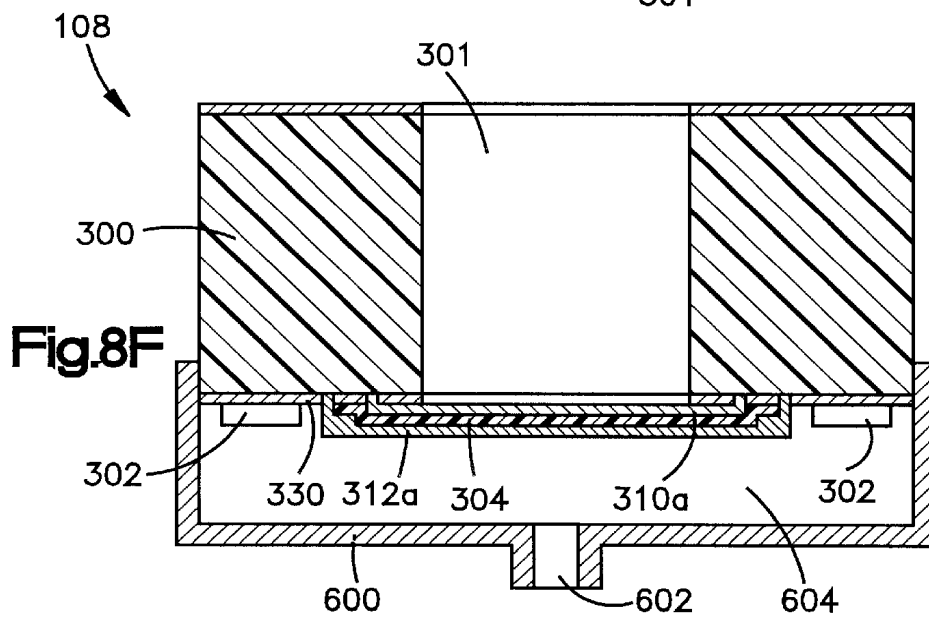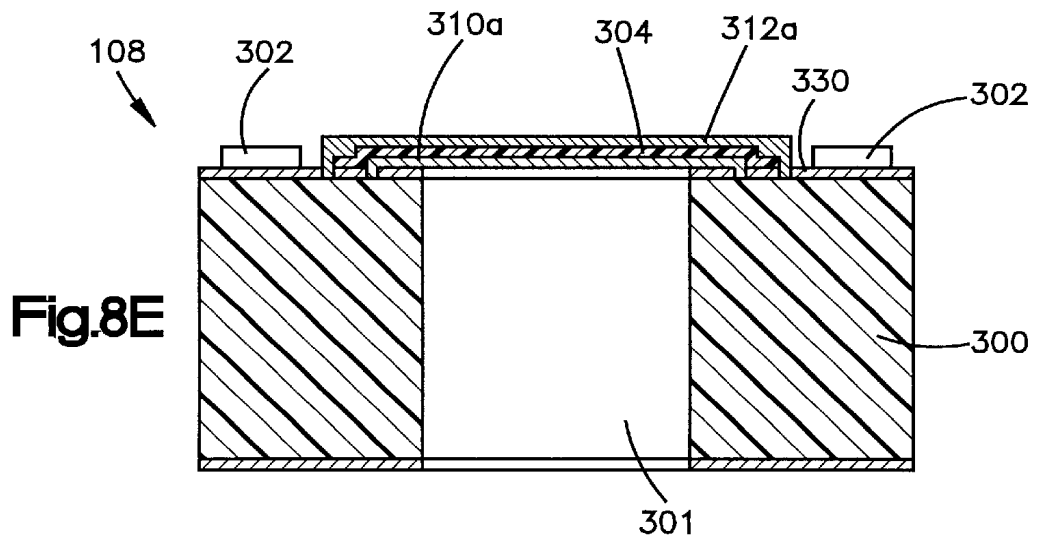

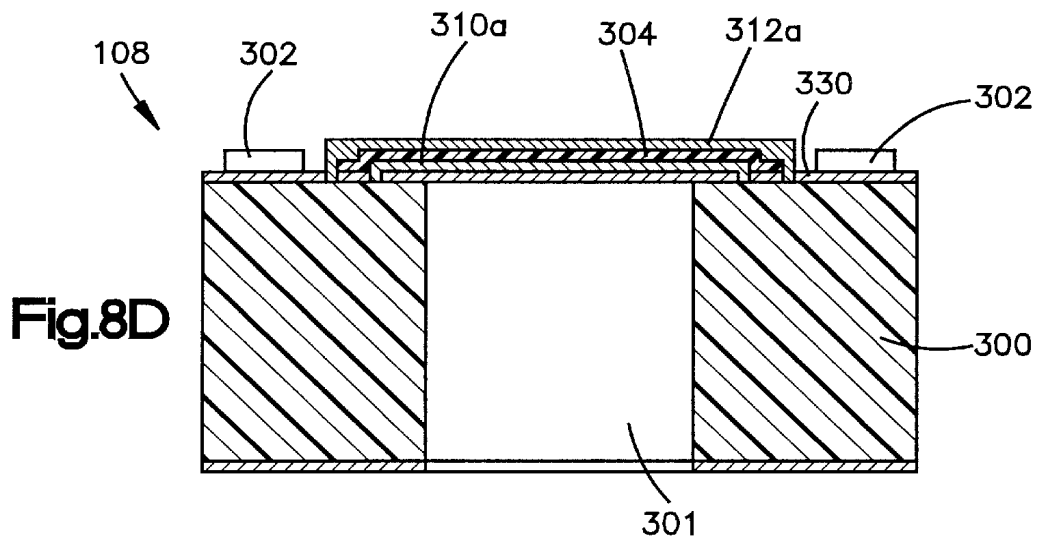

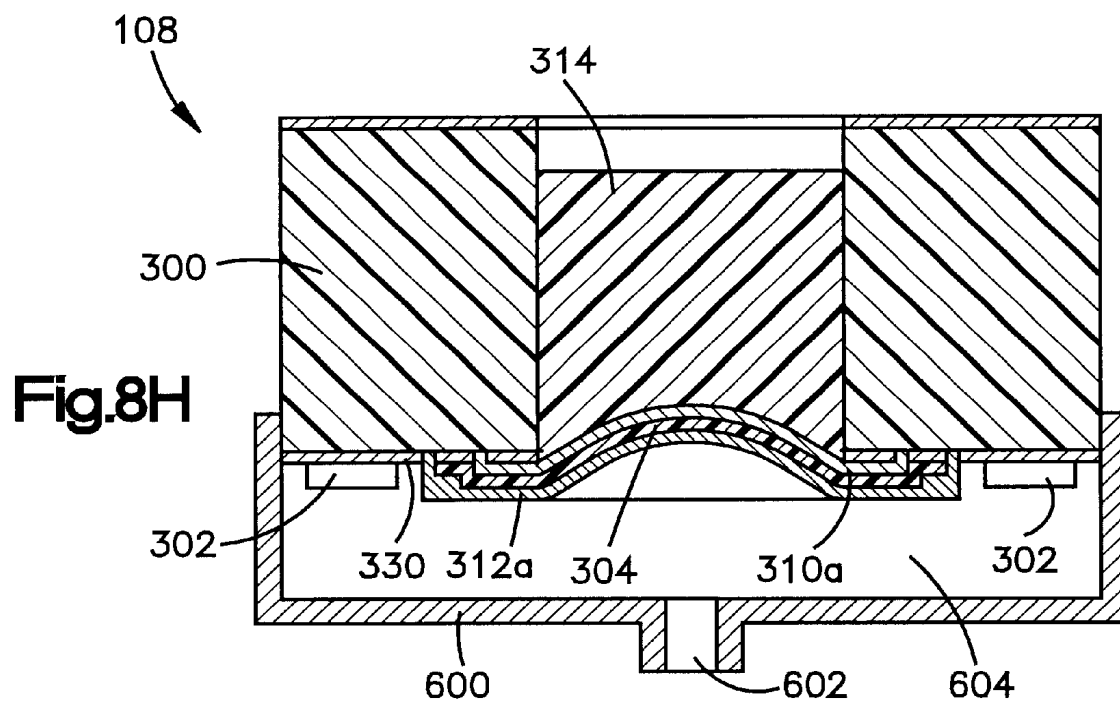

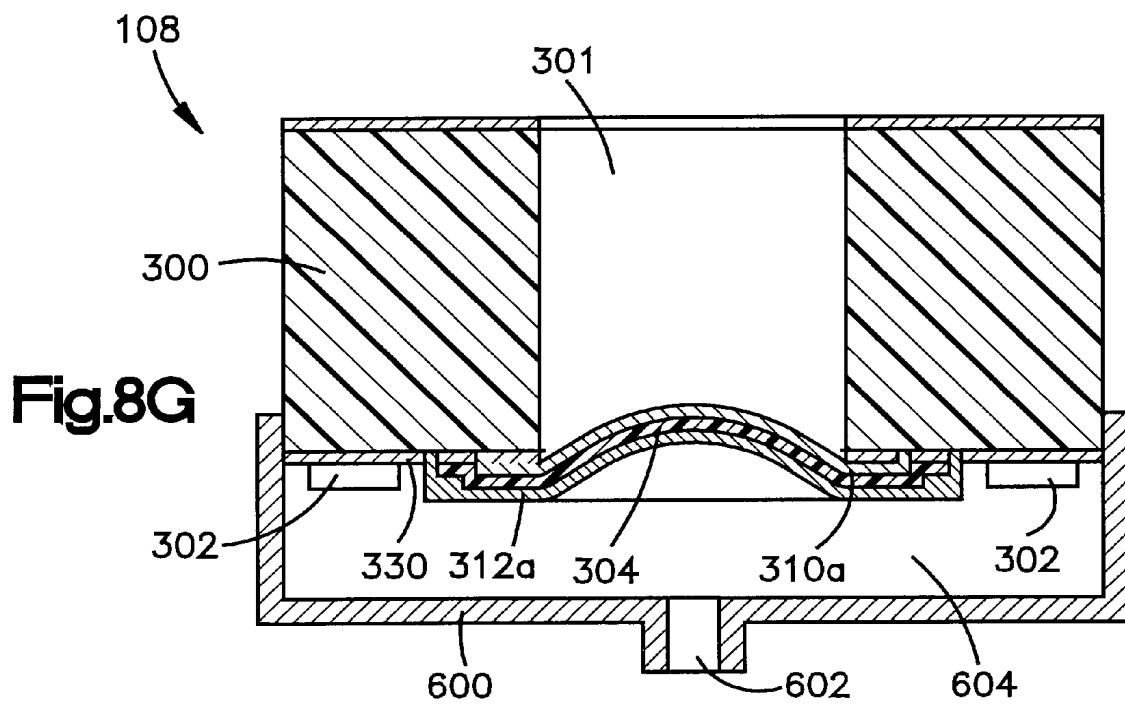

1

MINIATURE ULTRASOUND TRANSDUCER

This application claims the benefit of Provisional Application No. 60/250,775, filed Dec. 1, 2000.

FIELD OF THE INVENTION

The invention relates generally to an ultrasound transducer, and more particularly, to a miniature ultrasound transducer fabricated using microelectromechanical system (MEMS) technology.

BACKGROUND OF THE INVENTION

Ultrasound transducers use high-frequency sound waves to construct images. More specifically, ultrasonic images are produced by sound waves as the sound waves reflect off of interfaces between mechanically different structures. The typical ultrasound transducer both emits and receives such sound waves.

It is known that certain medical procedures do not permit a doctor to touch, feel, and/or look at tumor(s), tissue, and blood vessels in order to differentiate therebetween. Ultrasound systems have been found to be particularly useful in such procedures because the ultrasound system can provide the desired feedback to the doctor. Additionally, such ultrasound systems are widely available and relatively inexpensive.

However, present ultrasound systems and ultrasound transducers tend to be rather physically large and are therefore not ideally suited to all applications where needed. Moreover, due to their rather large size, ultrasound transducers cannot be readily incorporated into other medical devices such as, for example, catheters and probes. Hence, an ultrasound system and, more particularly, an ultrasound transducer of a relatively small size is desirable. MEMS technology is ideally suited to produce such a small ultrasonic transducer.

SUMMARY OF THE INVENTION

The present invention is an ultrasonic transducer for use in medical imaging. The ultrasonic transducer comprises a substrate having first and second surfaces. The substrate includes an aperture extending from the first surface to the second surface. Electronic circuitry is located on the first surface. A diaphragm is positioned at least partially within the aperture and in electrical communication with the electronic circuitry. The diaphragm has an arcuate shape that is a section of a sphere. The transducer further comprises a binder material in physical communication with the diaphragm and the substrate.

In accordance with another aspect of the present invention, a method of forming an ultrasonic transducer is provided. The method comprises the steps of providing a substrate with an aperture, covering the aperture with a film, and applying a differential pressure across the film to form a diaphragm having a shape that is a section of a sphere. The method further comprises the step of applying binding material to the diaphragm to maintain the spherical section shape of the diaphragm.

In accordance with another aspect, the present invention is a medical device for insertion into a mammalian body. The medical device comprises an insertable body portion and an ultrasonic transducing section on the body portion. The ultrasonic transducing section has a plurality of ultrasonic transducers. Each of the plurality of ultrasonic transducers comprises a substrate having first and second surfaces. The

2

substrate includes an aperture extending from the first surface to the second surface. Electronic circuitry is located on the first surface. A diaphragm is located at least partially within the aperture and in electrical communication with the electronic circuitry. The diaphragm has an arcuate shape that is a section of a sphere. Each ultrasonic transducer further comprises a binder material in physical communication with the diaphragm and the substrate.

BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing and other features of the present invention will become apparent to those skilled in the art to which the present invention relates upon reading the following description with reference to the accompanying drawings, in which:

FIGS. 1 and 2 are block diagrams illustrating the operating principles of the present invention;

FIGS. 3A and 3B are illustrations of a first embodiment of an ultrasound transducer constructed in accordance with the present invention;

FIGS. 4A and 4B are illustrations of a second embodiment of an ultrasound transducer constructed in accordance with the present invention;

FIG. 5 is an illustration of a portion of a medical device having an array of ultrasound transducers according to the present invention;

FIGS. 6A–6E illustrate the process of fabricating an ultrasound transducer in accordance with the present invention;

FIGS. 6F and 6G illustrate an alternate process for fabricating an ultrasonic transducer in accordance with the present invention;

FIGS. 7A–7E illustrate another alternate process for fabricating an ultrasonic transducer in accordance with the present invention; and

FIGS. 8A–8H illustrate yet another alternate process for fabricating an ultrasonic transducer in accordance with the present invention.

DETAILED DESCRIPTION OF ILLUSTRATED EMBODIMENTS

Referring to FIGS. 1 and 2, block diagrams of an ultrasound system **100** according to the present invention are shown. More specifically, FIG. 1 illustrates the system **100** during a sound wave emitting cycle and FIG. 2 illustrates the system **100** during a sound wave receiving cycle. The system **100** includes imaging circuitry **102**, transmitting/receiving circuitry **104**, and an ultrasound transducer **106**. The imaging circuitry includes a computer based system (not shown) having appropriate logic or algorithms for driving and interpreting the sound echo information emitted and received from the transducer **106**. The transmitting/receiving circuitry **104** includes interfacing components for placing the imaging circuitry **102** in circuit communication with the transducer **106**. As described in more detail below, the transducer **106** has at least one transducing device **108**, and optionally includes a plurality of such transducing devices as indicated by reference numbers **110** and **112**. Each transducing device **108**, **110**, and **112** includes a transducing element and electronic circuitry for simplifying the communication between the transducer **106** and the imaging circuitry **102**.

In operation, the imaging circuitry **102** drives the transducer **106** to emit sound waves **114** at a frequency in the range of 35 to 65 MHz. It should be understood that frequencies of any other desired range could also be emitted

by the transducer **106**. The sound waves **114** penetrate an object **116** to be imaged. As the sound waves **114** penetrate object **116**, the sound waves reflect off of interfaces between mechanically different structures within the object **116** and form reflected sound waves **202** illustrated in FIG. 2. The reflected sound waves **202** are received by the transducer **106**. The emitted sound waves **114** and the reflected sound waves **202** are then used to construct an image of the object **116** through the logic and/or algorithms within the imaging circuitry **102**.

FIGS. 3A and 3B illustrate a first embodiment of the ultrasound transducing device **108** in plan view and in cross-sectional view, respectively. The transducing device **108** is formed on a substrate **300** that is approximately 1 mm³ in size or smaller, although it should be understood that the transducing device **108** could be larger or smaller than 1 mm³. The substrate **300** is made of silicon and has a topside and a backside surface. The topside surface has electronic circuitry **302** formed thereon. The electric circuitry **302** is formed through conventional processes such as Complementary Metal Oxide Silicon (CMOS) fabrication. The electronic circuitry **302** can include a large number of possible circuit designs and components including, but not limited to, signal conditioning circuitry, buffers, amplifiers, drivers, and analog-to-digital converters. The substrate **300** further has a hole or aperture **301** formed therein for receiving a diaphragm or transducing element **304**. The aperture **301** is formed through either conventional Computer Numerical Control (CNC) machining, laser machining, micromachining, microfabrication, or a suitable MEMS fabrication process such as Deep Reactive Ion Etching (DRIE). The aperture **301** can be circular or another suitable shape, such as an ellipse.

The transducing element **304** is made of a thin film piezoelectric material, such as polyvinylidene fluoride (PVDF) or another suitable polymer. The PVDF film may include trifluoroethylene to enhance its piezoelectric properties. Alternatively, the transducing element **304** could be made of a non-polymeric piezoelectric material such as PZT or ZrO. The PVDF film is spun and formed on the substrate **300**. A free standing film could also be applied to the substrate **300** in lieu of the aforementioned spin coating process. The transducing element **304** can be between 1000 angstroms and 100 microns thick. In the illustrated embodiment, the transducing element **304** is approximately five to fifteen micrometers thick. However, as described below, the thickness of the transducing element **304** can be modified to change the frequency of the transducing device. The PVDF film is then made piezoelectric through corona discharge polling or similar methods.

The transducing element **304** has topside and backside surfaces **306** and **308**, respectively. The topside surface **306** is in electrical communication with an electrode **310** and the backside surface **308** is in electrical communication with an electrode **312**. The electrodes **310** and **312** provide an electrical pathway from the circuitry **302** to the transducing element **304**. The electrodes **310** and **312** are formed, using a known micromachining, microfabrication, or MEMS fabrication technique such as surface micromachining, from conductive material such as a chrome-gold material or another suitable conductive material.

The transducing element **304** is capable of being mechanically excited by passing a small electrical current through the electrodes **310** and **312**. The mechanical excitation generates sound waves at a particular frequency in the high-frequency or ultrasound range between 35 and 65 MHz. The exact frequency depends upon, among other

things, the thickness of the transducing element **304** between the topside and backside surfaces **306** and **308**, respectively. Hence, by controlling the thickness of the transducing element **304**, the desired transducing frequency can be obtained. In addition to being excited by current passed through the electrodes **310** and **312**, the transducing element **304** can also be mechanically excited by sound waves which then generate a current and/or voltage that can be received by the electrodes **310** and **312**.

A binding material **314** preferably in the form of a potting epoxy is applied to the backside surface **308** of the transducing element **304**. The binding material **314** is electrically conductive and mechanically maintains the shape of the transducing element **304**. The binding material **314** also provides attenuation of sound emissions at the backside surface **308**.

FIGS. 4A and 4B illustrate a second embodiment of the ultrasound transducing device **108** in plan view and in cross-sectional view, respectively. The second embodiment is substantially similar to the first embodiment of FIGS. 3A and 3B, except that the transducing device **108** according to the second embodiment includes one or more annular electrodes **402** and **404** operatively coupled between the electrodes **310** and **312**. The annular electrodes **402** and **404** provide the transducing element **304** with the ability to form focused or directed sound waves. The annular electrodes **402** and **404** are made of standard metals and formed on the surface of the transducing element **304** by known microfabrication or MEMS fabrication techniques, such as photolithography, prior to deformation of the transducing element.

Referring now to FIG. 5, an array **500** of ultrasound transducers **108** according to the present invention are shown. The array **500** can include transducers **108** of the variety shown in FIGS. 3A and 3B or FIGS. 4A and 4B, or combinations thereof. The array **500** is illustrated as being located on a probe for inserting into a human body, but could be located on a wide variety of other medical devices. An input and output bus (not shown) is coupled to each ultrasound transducer for carrying power, input, and output signals.

Referring now to FIGS. 6A through 6D, fabrication of the present invention will now be discussed. Before discussing the particulars, it should be noted that present invention is preferably fabricated on a wafer-scale approach. Nevertheless, less than wafer-scale implementation can also be employed such as, for example, on a discrete transducer level. The following description discusses a discrete transducer fabrication, but can also be implemented on a wafer-scale approach using known microfabrication, micromachining, or other MEMS fabrication techniques to produce several thousand transducers from a single four inch silicon wafer.

Referring now particularly to FIG. 6A, the substrate **300** is provided from a conventional circuit foundry with the desired circuitry **302** already fabricated thereon. The advantage of using substrates with circuitry already fabricated thereon is that existing circuit processing technologies can be used to form the required circuitry. The transducing element **304** is then spin-coated onto the substrate **300**, followed by the metallization of a thin-film (not shown) thereon. The transducing element **304** is then "polled", via corona-discharge or similar method, to render the film piezoelectric.

Referring now to FIG. 6B, the backside of the substrate **300** is machined away to form the aperture **301**. The

machining process can be conventional CNC machining, laser machining, micromachining, or a MEMS fabrication process such as DRIE. The transducing device **108** is then turned upside-down as shown in FIG. 6C. Next, a pressure jig **600** is placed over the now downwardly-facing surface of the substrate **300**. The pressure jig **600** includes a pressure connection **602** and a vacuum space **604**. The pressure connection **602** connects the pressure jig **600** to a source of pressurized air or other gas. The pressure jig **600** creates a seal against the substrate **300** and forms a pressurized space **604** for pressurizing the aperture **301**. The pressurized space **604** permits the creation of a differential pressure across the transducing element **304** which causes the transducing element to be drawn into the aperture **301**. As shown in FIG. 6D, the differential pressure results in the transducing element **304** being deformed from a planar shape into an arcuate shape that is a substantially spherical section. The spherical section shape of the transducer element **304** is preferably less than hemispherical as may be seen in FIG. 6D, but could be hemispherical or another shape.

It should be understood that the pressure jig **600** shown in FIGS. 6C–6E could be a portion of a larger jig for performing simultaneous pressurization of hundreds or even thousands of transducing devices **108** formed on a single silicon wafer.

Referring now to FIG. 6E, the binding material **314** is introduced into the aperture **301**. The binding material **314** can be any shape once applied. The binding material **314** is a fluid or semi-solid when applied to the backside surface **308** of the transducing element **304** and the contacts the walls of the aperture **301** in the substrate **300**. The binding material **314** subsequently dries to a solid. The binding material **314** is a suitable form of potting epoxy, which can be either conductive or nonconductive. As described, the binding material **314** functions to maintain the substantially hemispheric shape of transducing element **304**. The binding material **314** further acts to absorb sound waves generated by transducing element **304** that are not used in the imaging process.

FIGS. 6F and 6G illustrate an alternate process for fabricating the ultrasonic transducing device **108**. The alternate process shown on FIGS. 6F and 6G is similar to the process steps shown in FIGS. 6C–6E, except that the binding material **314** is placed in the aperture **301** behind the transducing element **304** before, rather than after, the differential pressure is applied to the transducing element by the pressure jig **600**. The liquid or semi-solid binding material **314** is then deflected along with the transducing element **304** by the differential pressure and, once solidified, mechanically supports the transducing element.

FIGS. 7A–7E illustrate another alternate process for fabricating the ultrasonic transducing device **108**. The alternate process of FIGS. 7A–7E is similar to the process shown in FIGS. 6A–6E, except that the pressure jig **600** brought down over the upwardly-facing surface of the substrate **300** and the pressure source **602** pulls a vacuum, rather than applying increased pressure, in the aperture **301** to cause the desired deflection of the transducing element **304**. Once the transducing element **304** is deflected as desired, the binding material **314** is applied as discussed previously.

FIGS. 8A–8E illustrate another alternate process for fabricating the ultrasonic transducing device **108**. In FIGS. 8A–8E, components that are similar to components shown in FIGS. 6A–6E use the same reference numbers, but are identified with the suffix “a”. Referring now particularly to FIG. 8A, the silicon substrate **300** is provided from a

conventional circuit foundry and the desired circuitry **302** already fabricated thereon. The substrate **300** is already coated with a field oxide layer **330** which is then used to pattern the electrodes **310a** and **312a** (FIG. 8C) on the substrate. After the electrode **310a** is deposited on the substrate **300** and operatively coupled to the circuitry **302**, the transducing element **304** is then spin-coated over the electrode **310a**, as shown in FIG. 8B. The electrode **312a** is then deposited over the transducing element **304**, as shown in FIG. 8C.

Referring now to FIG. 8D, the backside of the substrate **300** is etched, using a DRIE process, to form the aperture **301**. A second etching process is then employed to remove the oxide inside the aperture **301** (FIG. 8E).

The transducing device **108** is then turned upside-down as shown in FIG. 8F. Next, a pressure jig **600** is placed over the now downwardly-facing surface of the substrate **300**. The pressure jig **600** includes a pressure connection **602** and a vacuum space **604**. The pressure connection **602** connects the pressure jig **600** to a source of pressurized air or other gas. The pressure jig **600** creates a seal against the substrate **300** and forms a pressurized space **604** for pressurizing the aperture **301**. The pressurized space **604** permits the creation of a differential pressure across the transducing element **304** which causes the transducing element to be drawn into the aperture **301**. As shown in FIG. 8G, the differential pressure results in the transducing element **304** being deformed from a planar shape into an arcuate shape that is a substantially spherical section. The spherical section shape of the transducer element **304** is preferably less than hemispherical as may be seen in FIG. 6G, but could be hemispherical or another shape. The transducing element **304** is then “polled”, via corona-discharge or similar method, to render the film piezoelectric.

It should be understood that the pressure jig **600** shown in FIGS. 8F–8G could be a portion of a larger jig for performing simultaneous pressurization of hundreds or even thousands of transducing devices **108** formed on a single silicon wafer.

Referring now to FIG. 8H, the binding material **314** is introduced into the aperture **301**. The binding material **314** can be any shape once applied. The binding material **314** is a fluid or semi-solid when applied to the backside surface **308** of the transducing element **304** and the contacts the walls of the aperture **301** in the substrate **300**. The binding material **314** subsequently dries to a solid. The binding material **314** is a suitable form of potting epoxy and should be non-conductive. As described, the binding material **314** functions to maintain the substantially hemispheric shape of transducing element **304**. The binding material **314** further acts to absorb sound waves generated by transducing element **304** that are not used in the imaging process.

From the above description of the invention, those skilled in the art will perceive improvements, changes and modifications. For example, it is contemplated that the shape of the transducing element **304** could be a section of an ellipse, rather than a section of a sphere, in order to provide a different focus for the transducing device **108** and/or alter the frequency of the transducing device. Such an elliptical section shape could be produced by varying the configuration of the aperture **301** in the substrate **300** or by varying the thickness of the transducing element **304**. Further, the annular electrodes **402** and **404** could also be formed to have a shape that is a section of an ellipse. Such improvements, changes and modifications within the skill of the art are intended to be covered by the appended claims.

Having described the invention, we claim:

1. An ultrasonic transducer for use in medical imaging, said ultrasonic transducer comprising:
 - a substrate having oppositely disposed first and second outer surfaces, said substrate including an aperture extending from said first outer surface to said second outer surface;
 - a diaphragm positioned at least partially within said aperture, said diaphragm having an arcuate shape that is a section of a sphere for focusing ultrasonic waves emitted from the diaphragm;
 - a plurality of electrodes in physical communication with said diaphragm; and
 - a binder material in physical communication with said diaphragm and said substrate.
2. The ultrasonic transducer of claim 1 wherein said diaphragm comprises a thin film piezoelectric material.
3. The ultrasonic transducer of claim 2 wherein said thin film piezoelectric material is a polyvinylidene fluoride film.
4. The ultrasonic transducer of claim 2, wherein said thin film piezoelectric material is film comprising polyvinylidene fluoride and trifluoroethylene.
5. The ultrasonic transducer of claim 1 wherein said diaphragm comprises a free-standing film.
6. The ultrasonic transducer of claim 1 wherein said binding material comprises a conductive material.
7. The ultrasonic transducer of claim 1 wherein said binding material comprises a non-conductive material.
8. The ultrasonic transducer of claim 1 wherein said binder material is located at least partially within said aperture, said binder material abutting and supporting said diaphragm and attenuating sound waves generated by said diaphragm.
9. The ultrasonic transducer of claim 1 wherein said diaphragm has a thickness between 1000 angstroms and 100 microns.
10. The ultrasonic transducer of claim 9 wherein said diaphragm has a thickness of approximately five to fifteen micrometers.
11. The ultrasonic transducer of claim 1 wherein at least one of said plurality of electrodes is an annular electrode formed on a surface of said diaphragm and operative to further focus emitted sound waves.
12. The ultrasonic transducer of claim 1 wherein said diaphragm resonates at a frequency between 30 and 120 Mhz.
13. The ultrasonic transducer of claim 1 wherein said first surface of said substrate comprises a surface area of about 1 mm².
14. The ultrasonic transducer of claim 1 wherein said substrate is fabricated from silicon.
15. A method for forming an ultrasonic transducer comprising the steps of:
 - providing a silicon substrate, having oppositely disposed first and second outer surfaces;
 - creating an aperture in the substrate extending from the first surface to the second surface via a micromachining, microfabrication, or MEMS fabrication process;
 - covering the aperture with a film;
 - forming a plurality of electrodes in physical communication with the film via a micromachining, microfabrication, or MEMS fabrication process;
 - applying a differential pressure across the film to form a diaphragm having a shape that is a section of a sphere; and

- applying binding material to the diaphragm to maintain the spherical section shape of the diaphragm.
16. The method of claim 15 wherein the electrodes are formed via surface micromachining.
17. The method of claim 15 wherein the aperture is provided via deep reactive ion etching.
18. The method of claim 15 wherein the step of applying binding material is done before the differential pressure is applied.
19. The method of claim 15 wherein the step of applying binding material is done after the differential pressure is applied.
20. The method of claim 15 further comprising the step of: forming at least one annular electrode on a surface of the diaphragm.
21. The method of claim 15 further comprising the step of: rendering the diaphragm piezoelectric.
22. The method of step 21 where the step of rendering the diaphragm piezoelectric comprises corona discharge polling of the diaphragm.
23. A medical device for insertion into a mammalian body, said medical device comprising:
 - an insertable body portion; and
 - an ultrasonic transducing section on said insertable body portion, said ultrasonic transducing section having at least one ultrasonic transducer, each of said at least one ultrasonic transducer comprising:
 - a substrate having oppositely disposed first and second outer surfaces, said substrate including an aperture extending from said first outer surface to said second outer surface;
 - a diaphragm positioned at least partially within said aperture, said diaphragm having an arcuate shape that is a section of a sphere for focusing ultrasonic waves emitted from said diaphragm;
 - a plurality of electrodes in physical communication with said diaphragm; and
 - a binder material in physical communication with said diaphragm and said substrate.
24. The medical device of claim 23 wherein said diaphragm comprises a thin film piezoelectric material.
25. The medical device of claim 24, wherein said thin film piezoelectric material is a polyvinylidene fluoride film.
26. The medical device of claim 24, wherein said thin film piezoelectric material is a film comprising polyvinylidene fluoride and trifluoroethylene.
27. The medical device of claim 23 wherein said diaphragm comprises a free-standing film.
28. The medical device of claim 23 wherein said binding material comprises a conductive material.
29. The medical device of claim 23 wherein said binding material comprises a non-conductive material.
30. The medical device of claim 23 wherein at least one of said plurality of electrodes is an annular electrode formed on a surface of said diaphragm and operative to further focus sound waves emitted by said at least one transducer.
31. The medical device of claim 23 wherein said binder material is located at least partially within said aperture, said binder material abutting and supporting said diaphragm and attenuating sound waves generated by said diaphragm.
32. The medical device of claim 23 wherein said first surface of said substrate comprises a surface area of about 1 mm².
33. The medical device of claim 23 wherein said substrate is fabricated from silicon.

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : 6,641,540 B2
APPLICATION NO. : 09/948068
DATED : November 4, 2003
INVENTOR(S) : Aaron J. Fleischman, Shuvo Roy and Geoffrey R. Lockwood

Page 1 of 1


It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Column 8, line 3, after "wherein" delete "the electrodes are formed" and insert --said forming of electrodes is achieved--.

Column 8, line 5, after "wherein" delete "the aperture is provided via deep reactive ion etching" and insert --an etching of deep reactive ion creates the aperture--.

Signed and Sealed this

Ninth Day of January, 2007

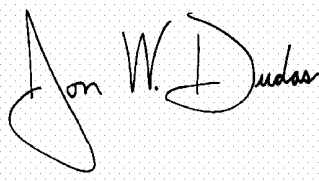A handwritten signature in black ink on a light gray dotted background. The signature reads "Jon W. Dudas" in a cursive, stylized script. The "J" is large and loops around the "on". The "W" and "D" are also stylized.

JON W. DUDAS
Director of the United States Patent and Trademark Office

专利名称(译)	微型超声换能器		
公开(公告)号	US6641540	公开(公告)日	2003-11-04
申请号	US09/948068	申请日	2001-09-06
[标]申请(专利权)人(译)	克里夫兰诊所基金会		
申请(专利权)人(译)	克利夫兰诊所基金会		
当前申请(专利权)人(译)	克利夫兰诊所基金会，		
[标]发明人	FLEISCHMAN AARON J ROY SHUVO LOCKWOOD GEOFFREY R		
发明人	FLEISCHMAN, AARON J. ROY, SHUVO LOCKWOOD, GEOFFREY R.		
IPC分类号	B06B1/06 A61B8/00 H04R3/00 A61B8/14		
CPC分类号	B06B1/0688 B06B1/0651		
优先权	60/250775 2000-12-01 US		
其他公开文献	US20020077551A1		
外部链接	Espacenet USPTO		

摘要(译)

用于医学成像的超声换能器 (108) 包括具有第一和第二表面的基板 (300)。基板 (300) 包括从第一表面延伸到第二表面的孔 (301)。电子电路 (302) 位于第一表面上。隔膜 (304) 至少部分地定位在孔 (301) 内并与电子电路 (302) 电连通。隔膜 (304) 具有弧形形状，通过施加差压形成，该差压是球体的一部分。粘合剂材料 (314) 与隔膜 (304) 和基板 (300) 物理连通。

