



US006936008B2

(12) **United States Patent**
Tarakci et al.

(10) **Patent No.:** **US 6,936,008 B2**
(45) **Date of Patent:** **Aug. 30, 2005**

(54) **ULTRASOUND SYSTEM WITH CABLELESS COUPLING ASSEMBLY**

(75) Inventors: **Umit Tarakci**, Hayward, CA (US); **Mir A. Imran**, Los Altos Hills, CA (US); **Glen McLaughlin**, Saratoga, CA (US); **Xufeng Xi**, Mountain View, CA (US)

(73) Assignee: **Zonare Medical Systems, Inc.**, Mountain View, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 144 days.

(21) Appl. No.: **10/039,910**

(22) Filed: **Oct. 20, 2001**

(65) **Prior Publication Data**

US 2002/0138002 A1 Sep. 26, 2002

Related U.S. Application Data

(63) Continuation-in-part of application No. 09/860,209, filed on May 18, 2001, now Pat. No. 6,569,102, which is a continuation of application No. 09/378,175, filed on Aug. 20, 1999, now Pat. No. 6,251,073.

(51) **Int. Cl.**⁷ **A61B 8/00**
(52) **U.S. Cl.** **600/437**; 600/459
(58) **Field of Search** 600/437, 443, 600/447, 459; 73/625, 626; 310/334–336, 367; 29/25.35

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,409,982 A 10/1983 Plesset et al.
4,803,990 A 2/1989 Bonnefous et al.
4,853,904 A 8/1989 Pesque
4,917,097 A * 4/1990 Proudian et al. 600/463
5,119,342 A 6/1992 Harrison, Jr. et al.
5,140,558 A 8/1992 Harrison, Jr. et al.
5,267,221 A * 11/1993 Miller et al. 367/140
5,278,757 A 1/1994 Hocter et al.
5,291,090 A 3/1994 Dias

5,295,485 A 3/1994 Shinomura et al.
5,329,498 A * 7/1994 Greenstein 367/155
5,483,963 A 1/1996 Butler et al.
5,505,203 A 4/1996 Deitrich et al.

(Continued)

OTHER PUBLICATIONS

Intermec Technologies Corporation, Intermec Technical Glossary ("ribbon cable") <http://home.intermec.com/eprise/main/Intermec/Content/About/Glossary> (accessed Jan. 14, 2005).

University of Oxford, Oxford Physics, "Flexible Ribbon Cable," <http://www.physics.ox.ac.uk/electronics/pfu/ribbon-hm.htm> (accessed Jan. 14, 2005).

Tech-Etch, Inc., Flexible Circuits, "Flexible Circuit Photo Gallery," <http://www.tech-etch.com/flex/2layer.html> (accessed Jan. 14, 2005).

GC Aero Flexible Printed Circuitry, About Flex, <http://www.gcaero.com/hm/aboutflex.htm> (accessed Jan. 14, 2005).

A. Pesavento et al., "Compression of Ultrasonic RF Data," IEEE Proc. Ultrasonics Symposium, 1997.

K. Rigby, et al., "Real Time Adaptive Imaging," IEEE Ultrasonics Symposium, pp. 1603–1606, 1988.

(Continued)

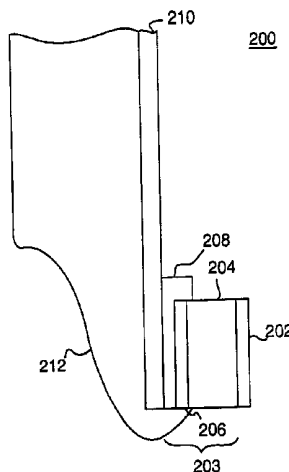
Primary Examiner—Francis J. Jaworski

(74) *Attorney, Agent, or Firm*—Carr & Ferrell LLP

(57) **ABSTRACT**

An ultrasound imaging device having a cableless coupling for coupling a two-dimensional array of ultrasound transducers to a signal generating and receiving unit such as a motherboard. The coupling includes an acoustically attenuating and electrically conductive structure, which can include posts that are electrically conductive or electrically insulative having a conductor embedded or mounted on the outer surface. There can also be a high density connector allowing coupling and de-coupling the two dimensional array to and from the motherboard.

24 Claims, 17 Drawing Sheets



U.S. PATENT DOCUMENTS

5,541,468 A 7/1996 Frey et al.
 5,559,388 A * 9/1996 Lorraine et al. 310/334
 5,590,658 A 1/1997 Chiang et al.
 5,617,862 A 4/1997 Cole et al.
 5,648,942 A * 7/1997 Kunkel, III 367/176
 5,667,373 A 9/1997 Wright et al.
 5,690,114 A * 11/1997 Chiang et al. 600/447
 5,722,412 A 3/1998 Pflugrath et al.
 5,738,099 A 4/1998 Chang
 5,740,806 A 4/1998 Miller
 5,744,898 A * 4/1998 Smith et al. 310/334
 5,782,769 A 7/1998 Hwang et al.
 5,793,701 A 8/1998 Wright et al.
 5,795,297 A * 8/1998 Daigle 600/447
 5,817,024 A 10/1998 Ogle et al.
 5,839,442 A 11/1998 Chiang et al.
 5,851,186 A 12/1998 Wood et al.
 5,873,830 A 2/1999 Hossack et al.
 5,893,363 A 4/1999 Little et al.
 5,897,501 A 4/1999 Wildes et al.
 5,904,652 A 5/1999 Gilbert et al.
 5,905,692 A 5/1999 Dolazza et al.
 5,919,138 A 7/1999 Ustuner
 5,925,967 A 7/1999 Toda
 5,951,479 A 9/1999 Holm et al.
 5,957,846 A * 9/1999 Chiang et al. 600/447
 5,964,709 A 10/1999 Chiang et al.
 5,970,025 A 10/1999 Cole et al.
 5,973,438 A 10/1999 Toda
 6,043,590 A * 3/2000 Gilmore 310/367
 6,055,861 A 5/2000 Banta, Jr. et al.
 6,063,030 A 5/2000 Vara et al.
 6,089,096 A 7/2000 Alexandru
 6,113,545 A 9/2000 Chiao et al.
 6,126,608 A 10/2000 Kemme et al.
 6,135,960 A 10/2000 Holmberg
 6,135,961 A 10/2000 Pflugrath et al.
 6,138,513 A * 10/2000 Barabash et al. 73/602
 6,139,498 A 10/2000 Katsman et al.
 6,174,286 B1 1/2001 Ramamurthy et al.
 6,203,498 B1 3/2001 Bunce et al.
 6,230,043 B1 5/2001 Johnson

6,238,346 B1 5/2001 Mason
 6,251,073 B1 6/2001 Imran et al.
 6,483,228 B2 * 11/2002 Hashimoto 310/336
 6,524,254 B2 * 2/2003 Erikson 600/447
 6,546,803 B1 4/2003 Ptchelintsev et al.
 6,551,248 B2 * 4/2003 Miller 600/459
 6,569,102 B2 * 5/2003 Imran et al. 600/459

OTHER PUBLICATIONS

C.M. Fabian, et al., "Development of a Parallel Acquisition System of Ultrasound Research," IEEE Proc. Ultrasonics Symposium, 2001.

C. M. Fabian, "Development of a Parallel Acquisition System for Ultrasound Research," Department of Electrical Eng., University of Virginia, (data unknown), pp. 1-9.

U.S. Appl. No. 09/860,209, filed May 18, 2001, Mir Imran, Miniaturized Ultrasound Apparatus and Method.

U.S. Appl. No. 09/872,541, filed May 31, 2001, Glen McLaughlin, System and Method for Phase Inversion Ultrasonic Imaging.

U.S. Appl. No. 10/039,858, filed Oct. 20, 2001, Umit Tarakci, A System and Method for Acoustic Imaging at Two Focal Lengths with a Single Lens.

U.S. Appl. No. 10/039,862, filed Oct. 20, 2001, Ting-Lan Ji, Simultaneous Multi-Mode and Multi-Band Ultrasonic Imaging.

U.S. Appl. No. 10/039,922, filed Oct. 20, 2001, Xufeng Xi, Block Switching in Ultrasound Imaging.

U.S. Appl. No. 29/147,576, filed Aug. 31, 2001, Ian Felix, Handheld Ultrasonic Display Device.

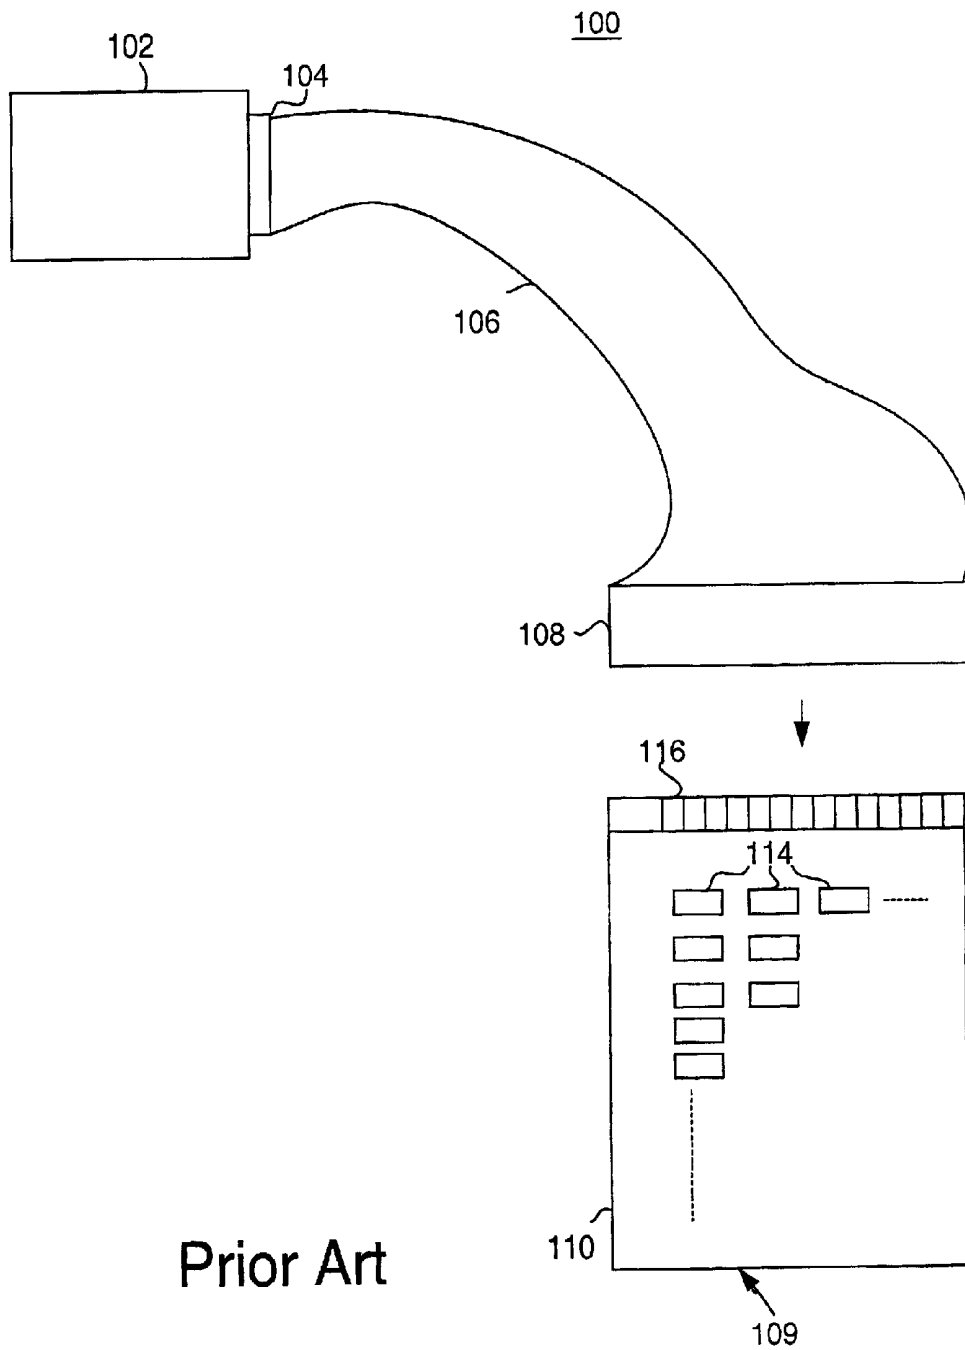
U.S. Appl. No. 29/147,660, filed Aug. 31, 2001, Ian Felix, Handheld Ultrasonic Display Device with Cover.

U.S. Appl. No. 29/148,421, filed Sep. 19, 2001, Ian Felix, Handheld Ultrasonic Transducer with Curved Bulb Grip.

U.S. Appl. No. 29/148,532, filed Sep. 19, 2001, Ian Felix, Handheld Ultrasonic Transducer with Bulb Grip.

U.S. Appl. No. 29/149,730, filed Oct. 15, 2001, Ian Felix, Docking Station.

* cited by examiner



Prior Art

FIG. 1

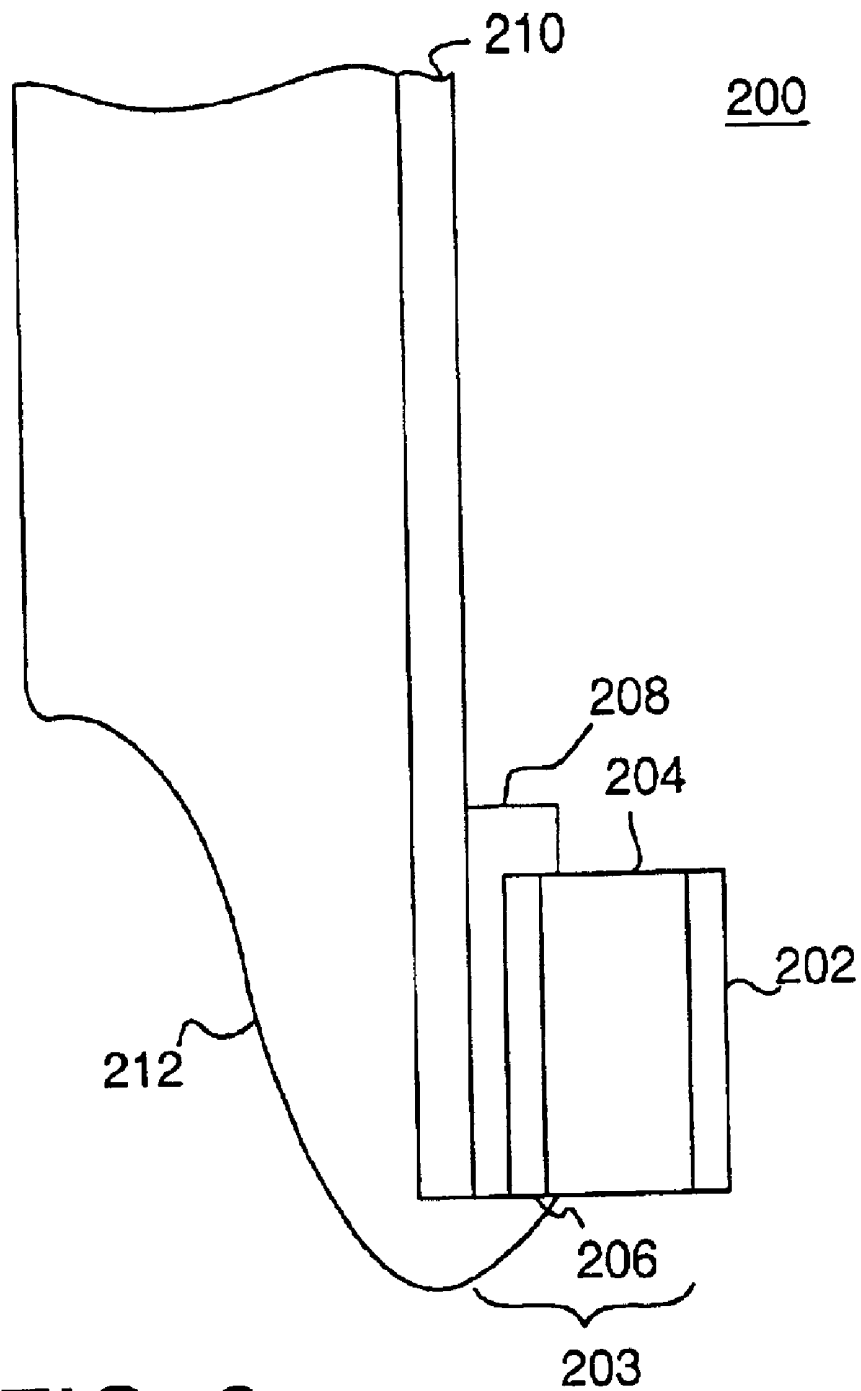


FIG. 2

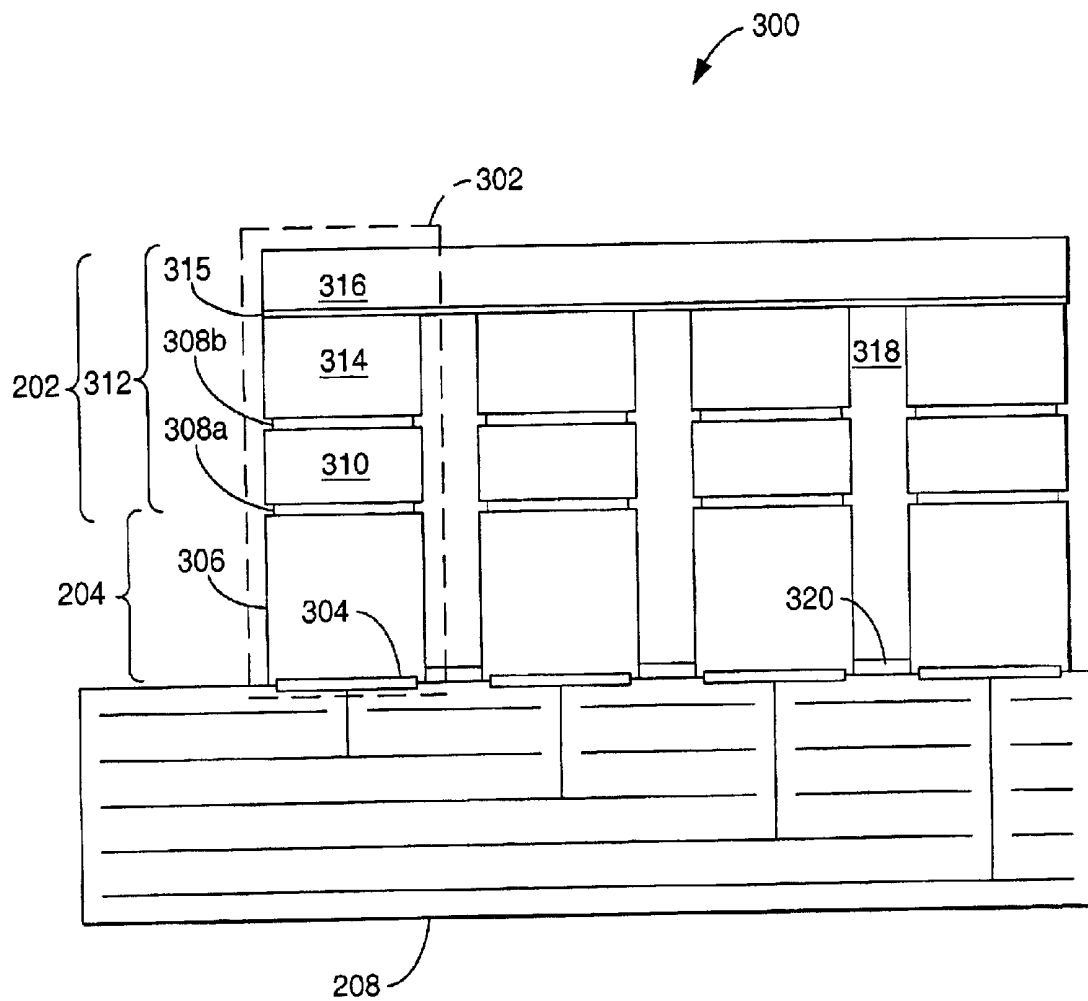


FIG. 3

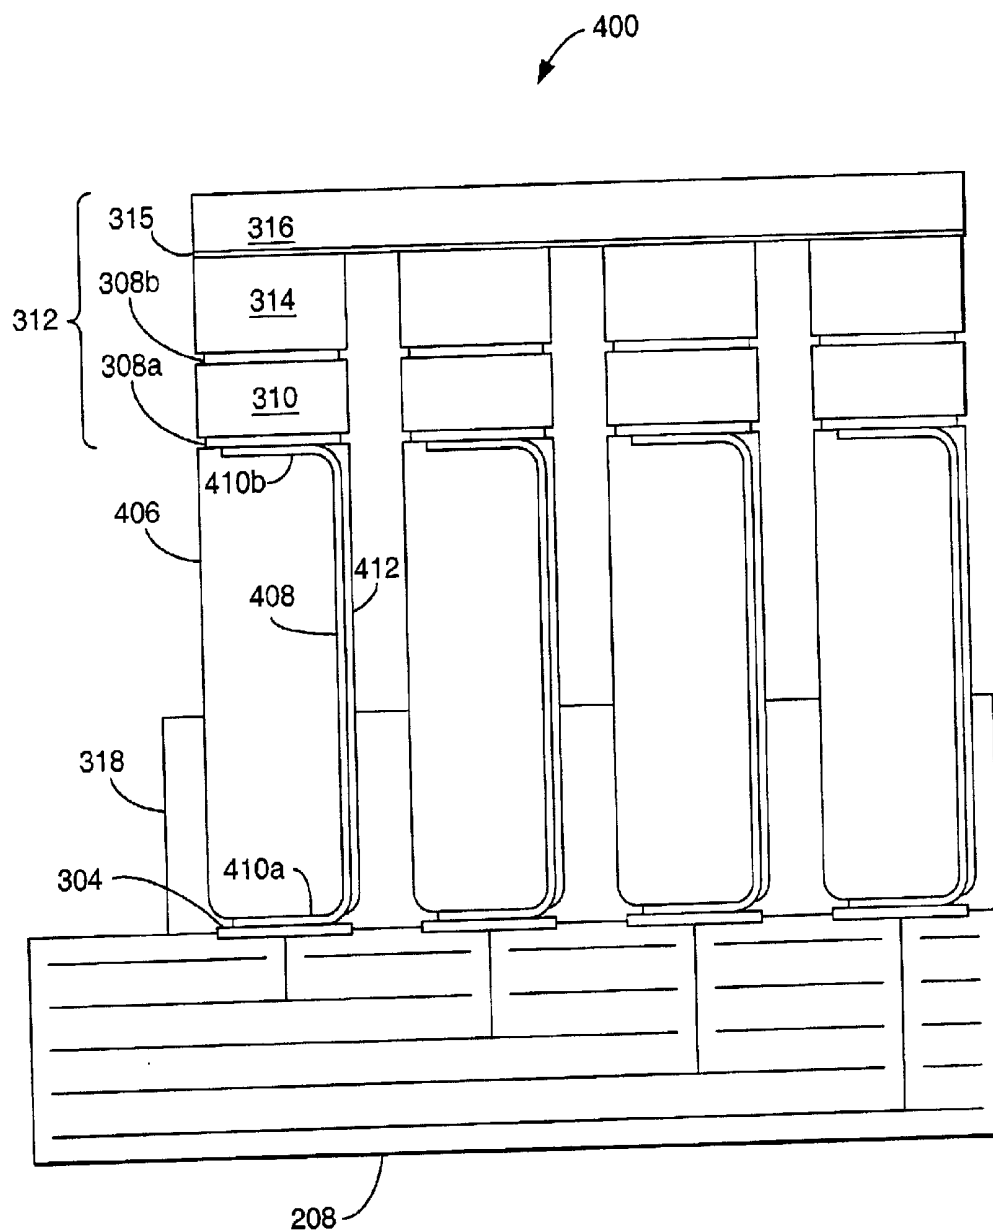


FIG. 4

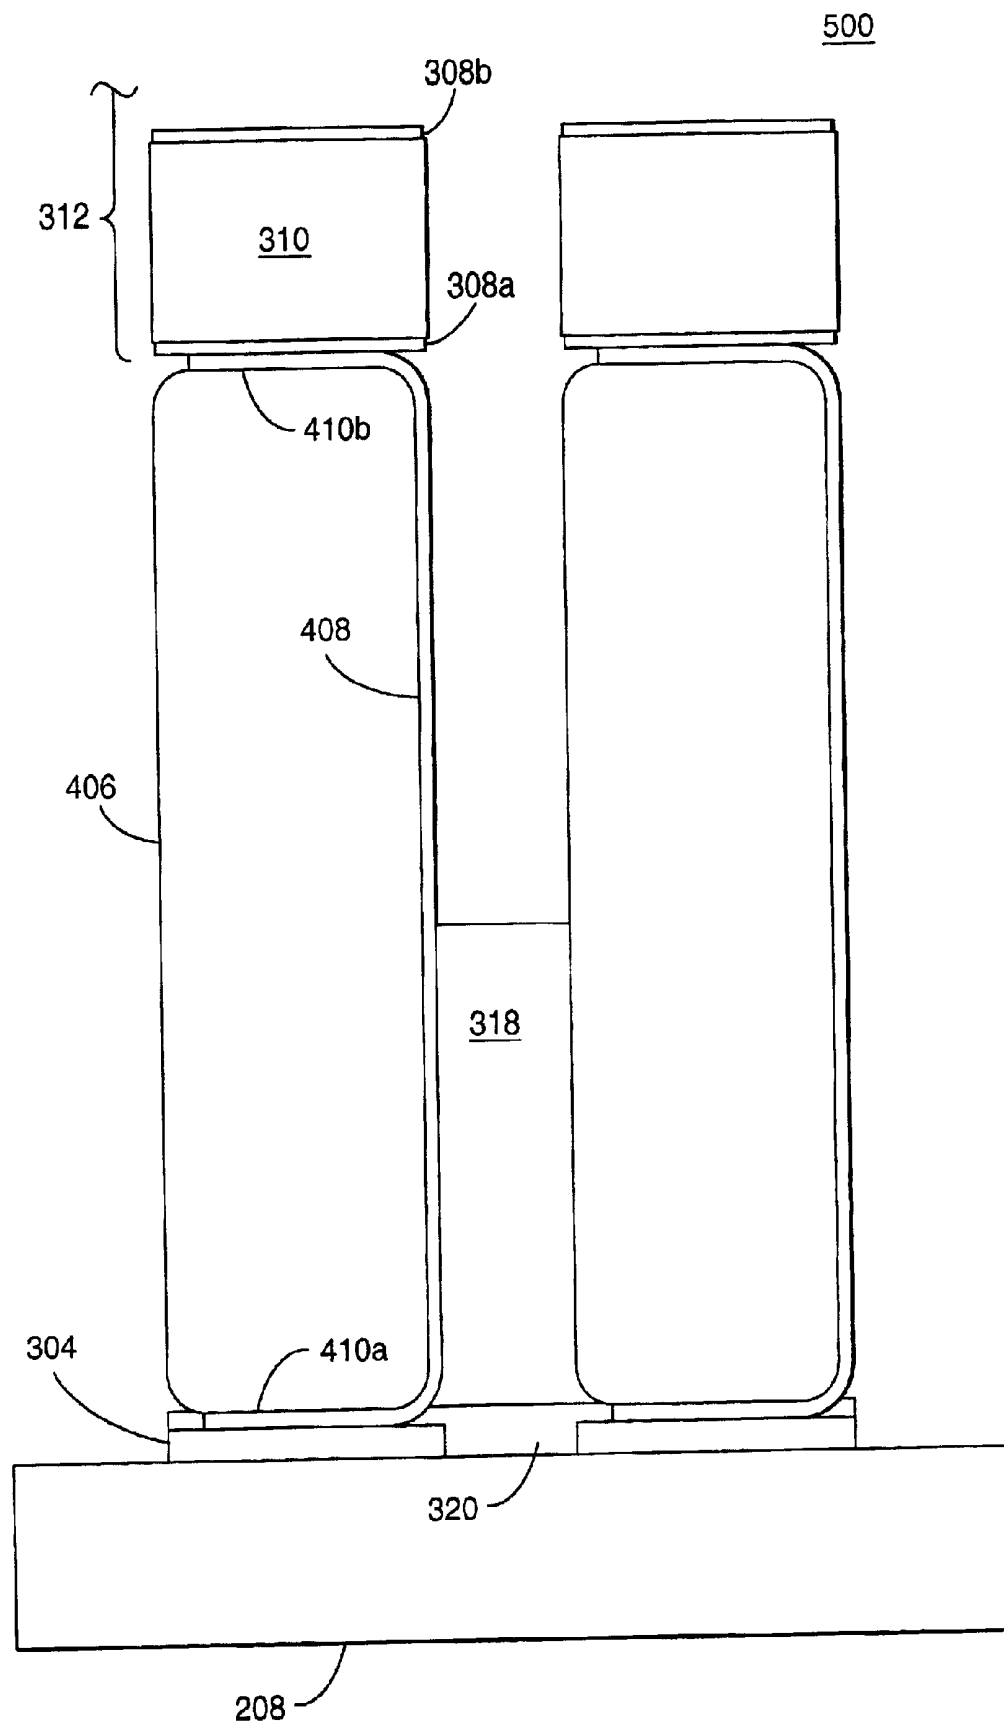


FIG. 5

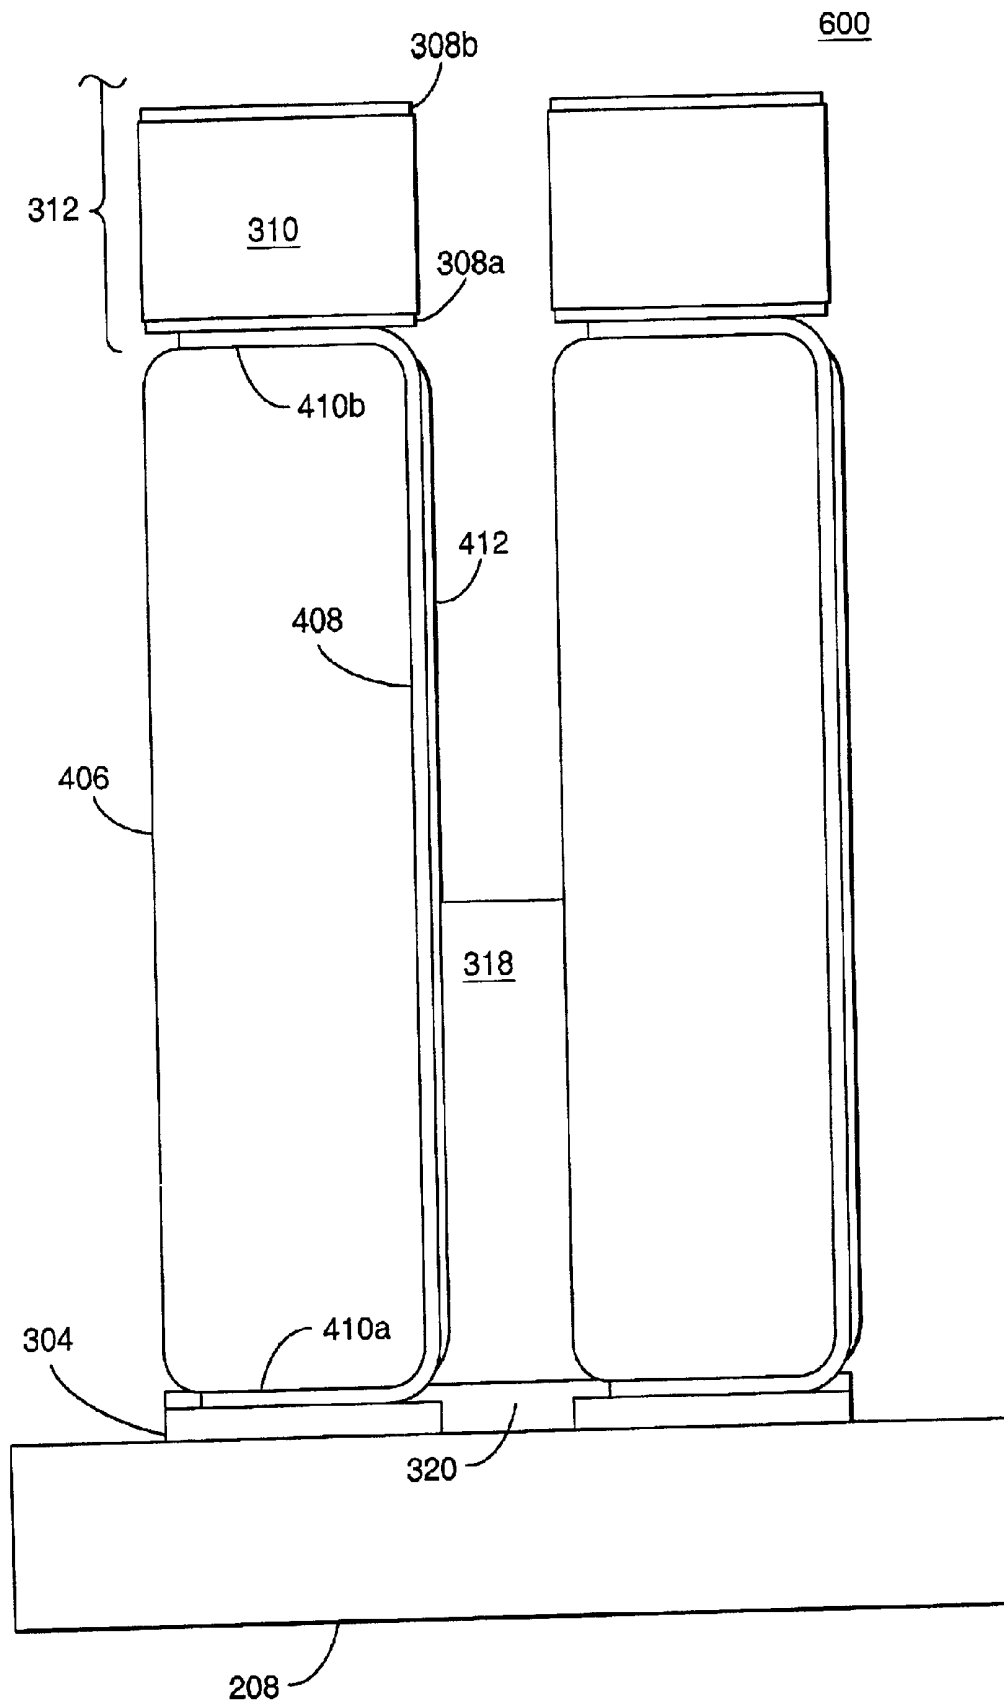


FIG. 6

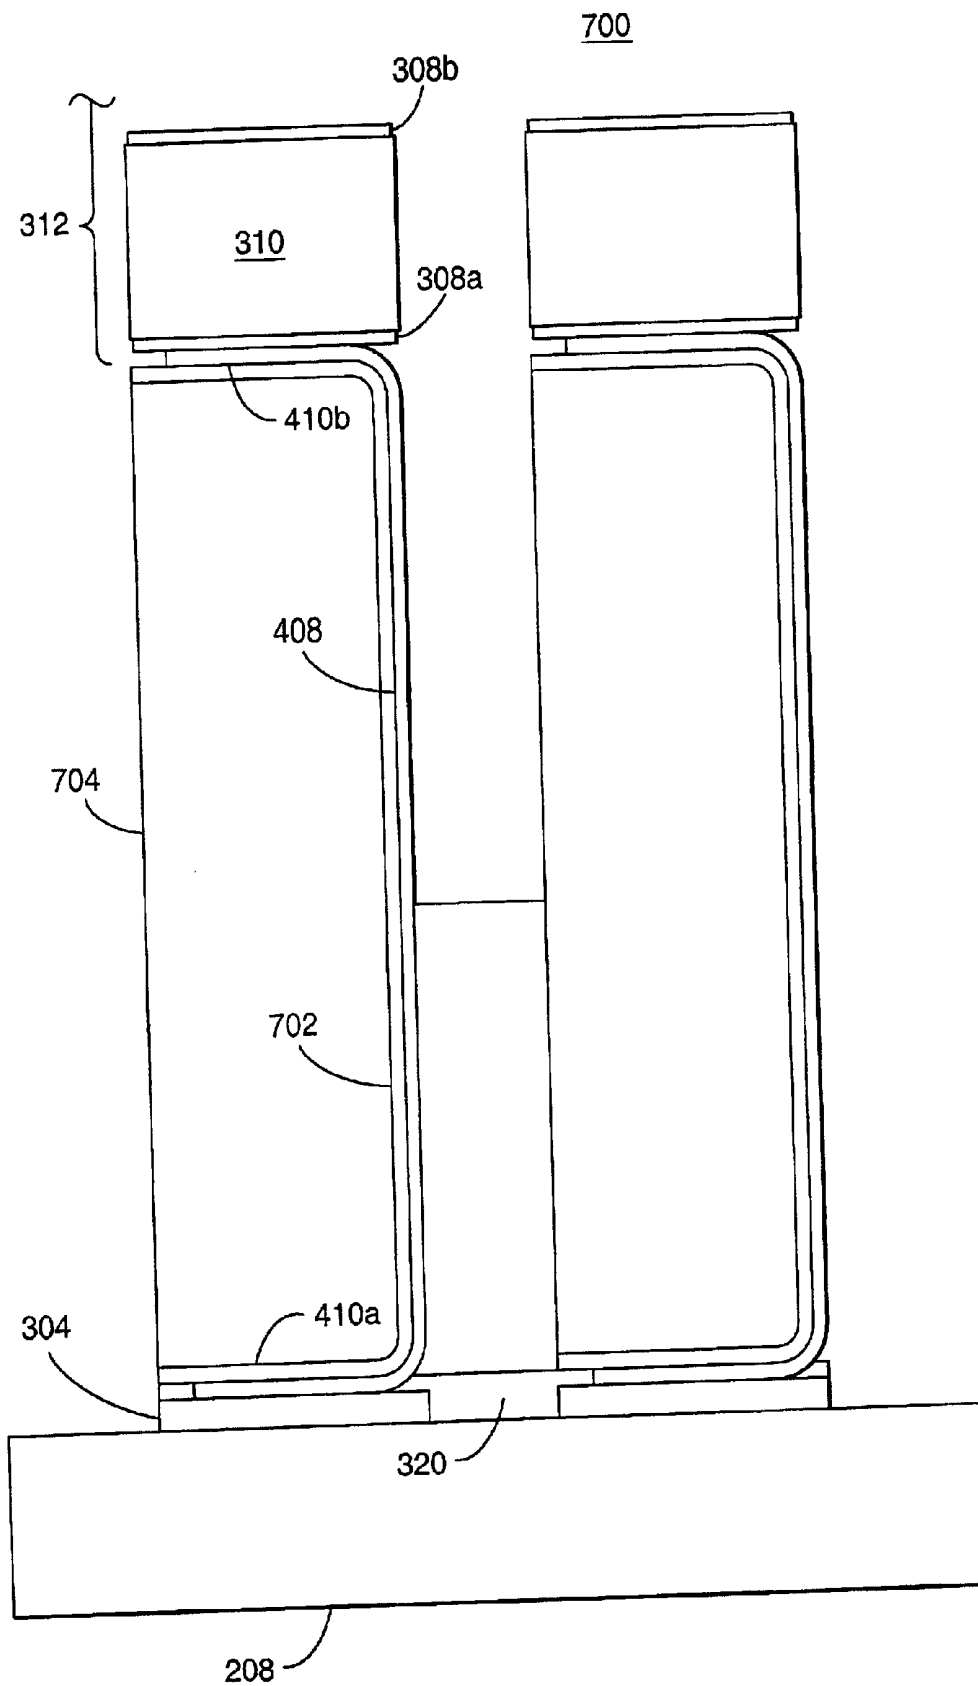


FIG. 7

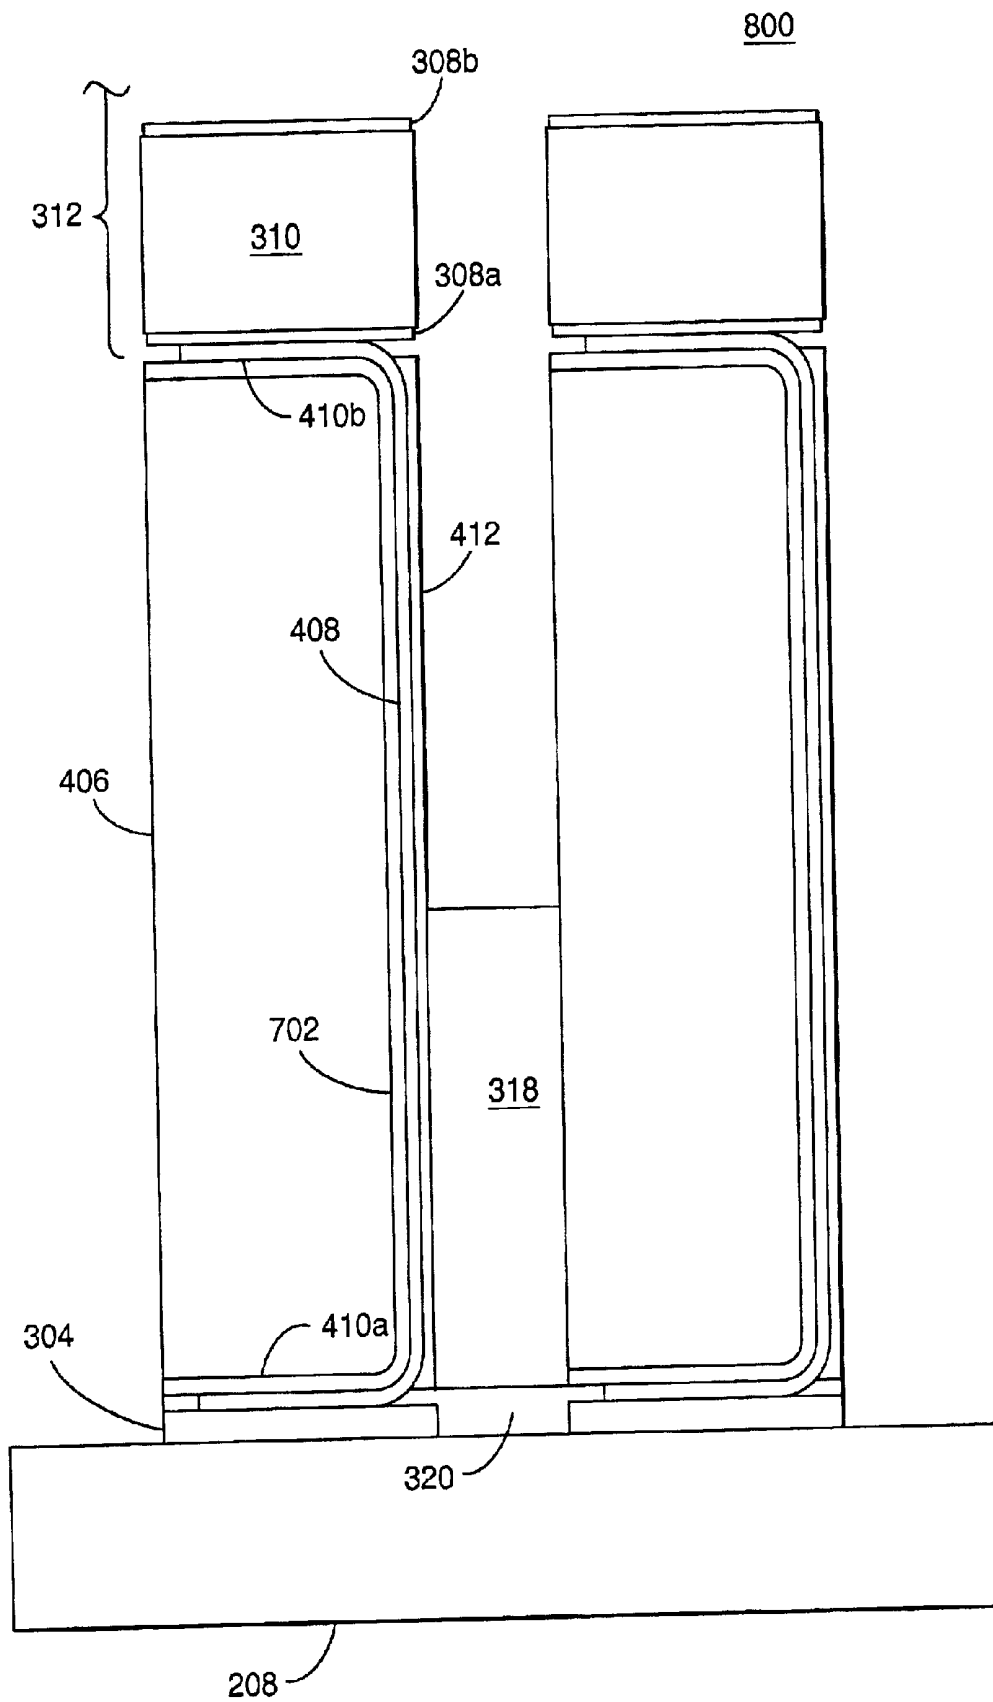


FIG. 8

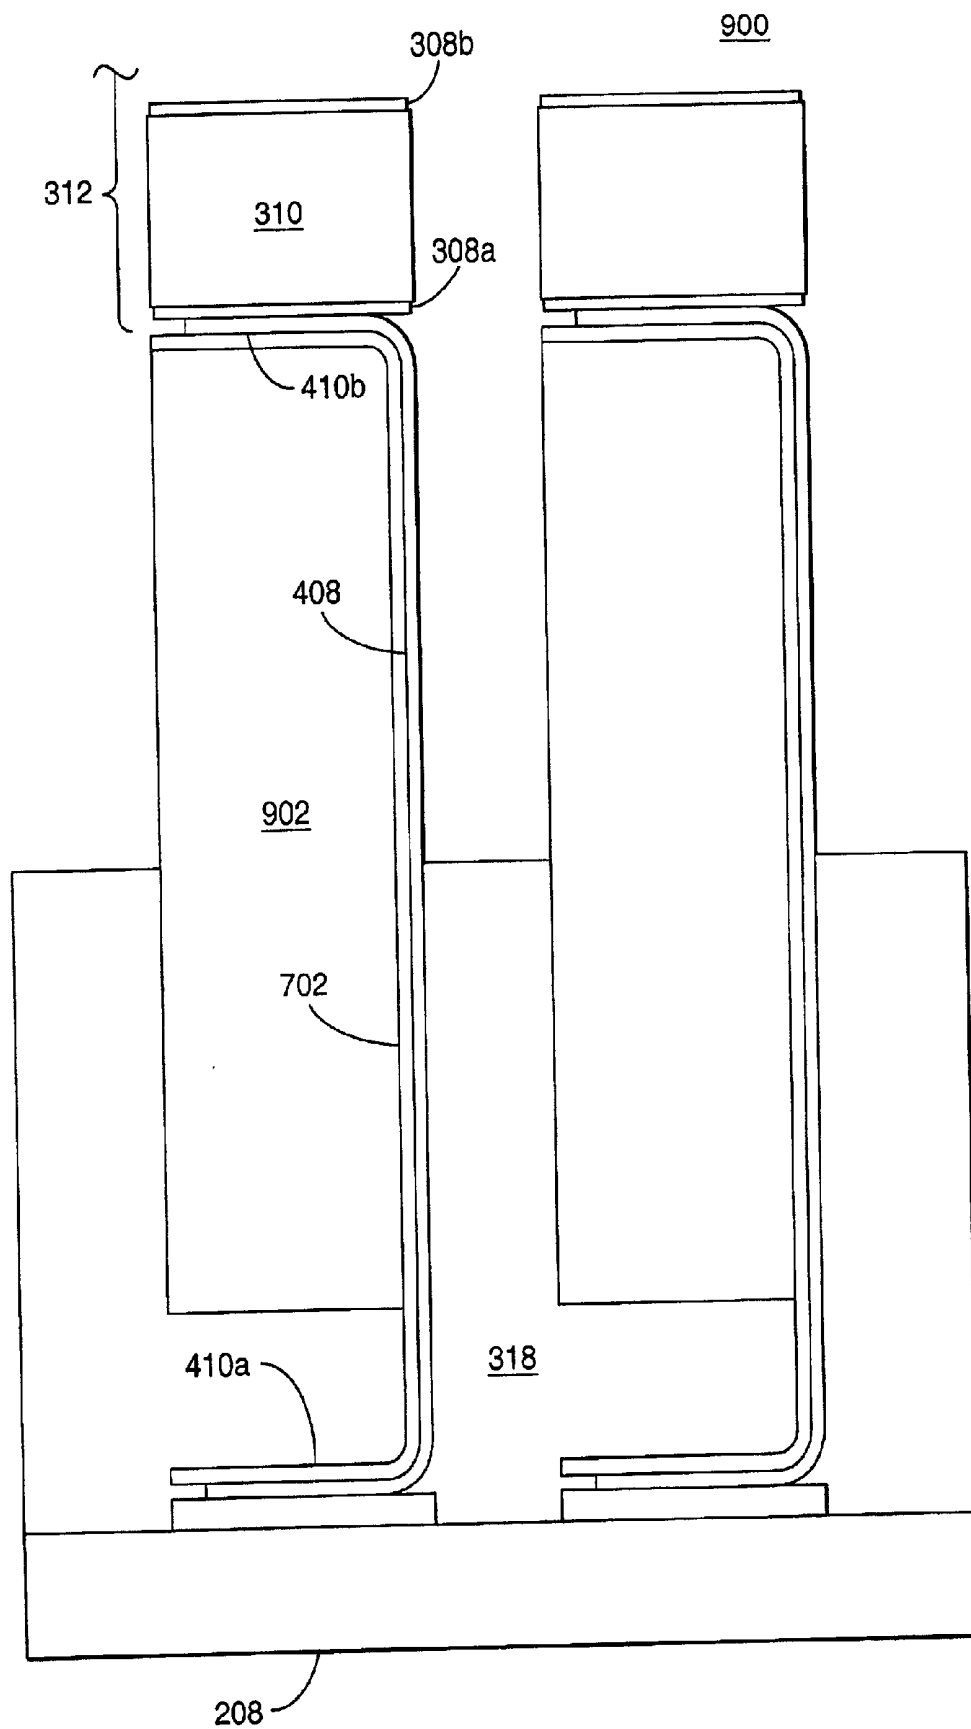


FIG. 9

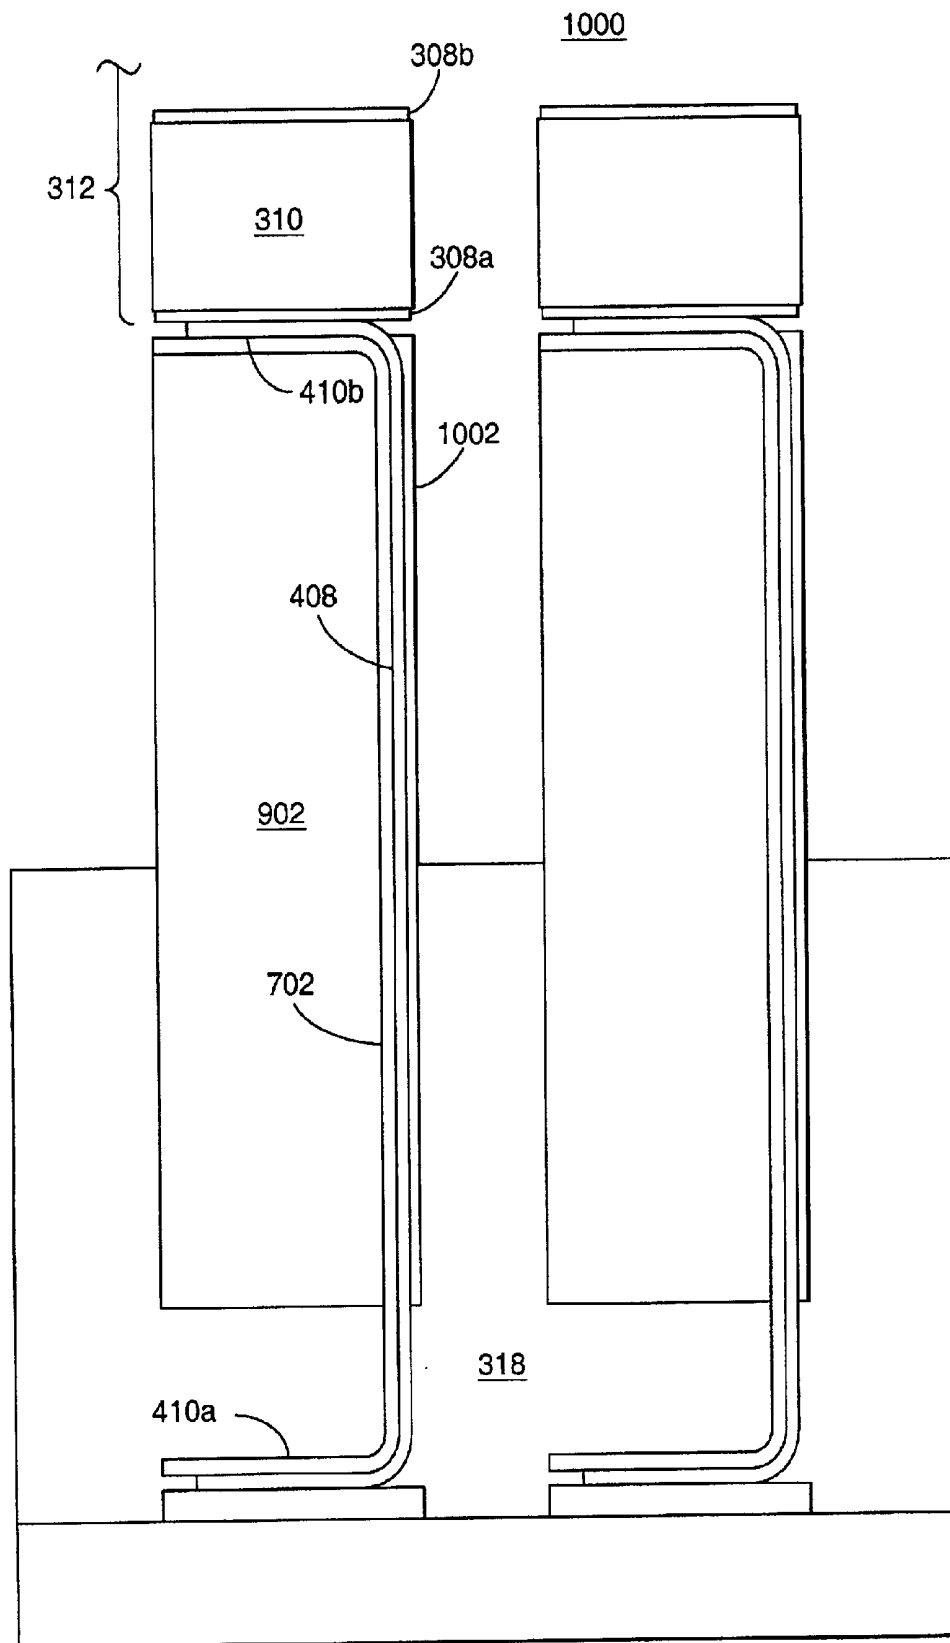


FIG. 10

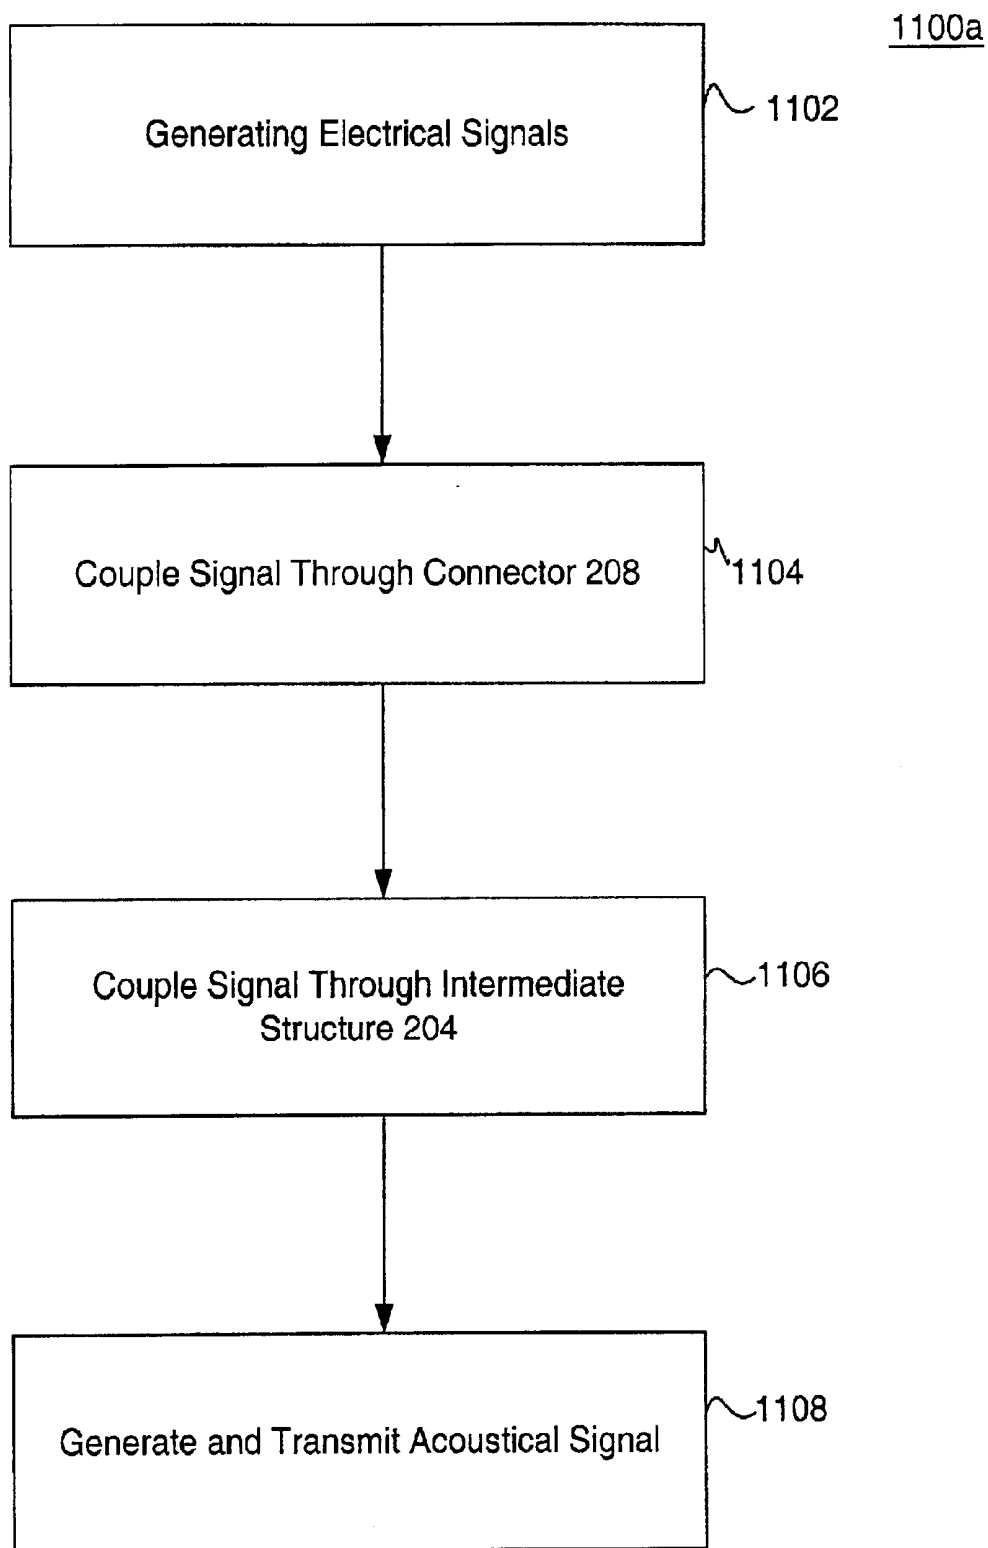


FIG. 11A


1100b

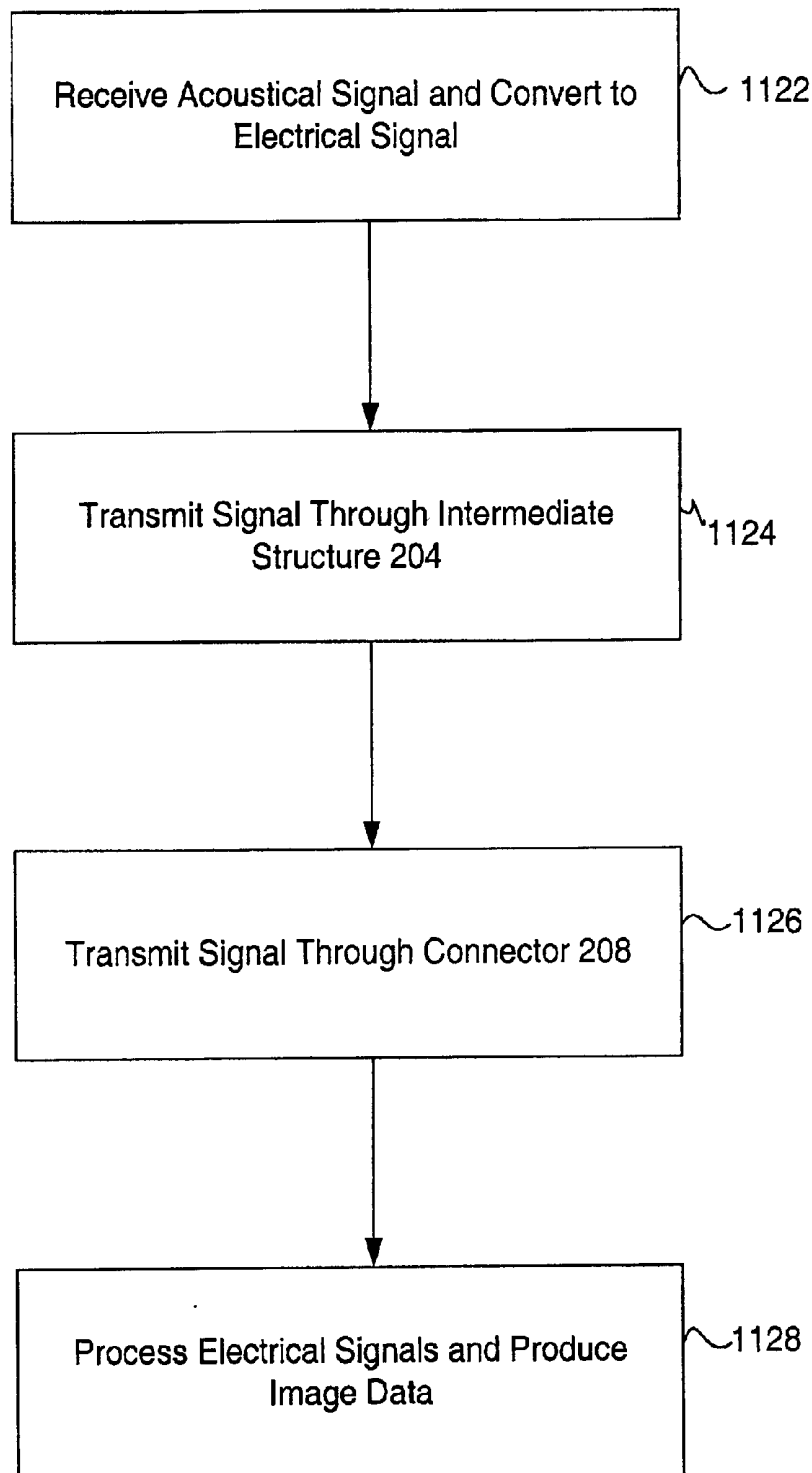FIG. 11B


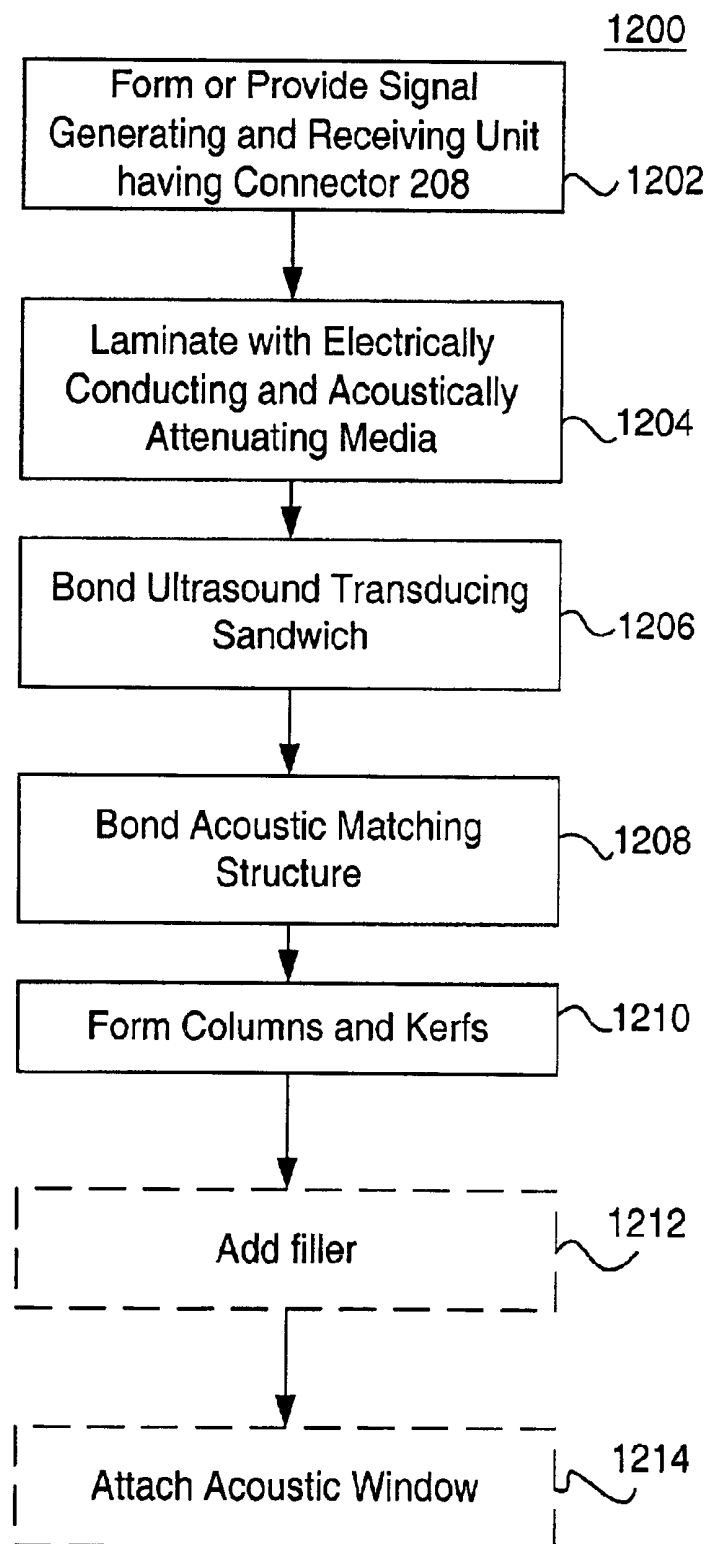


FIG. 12A

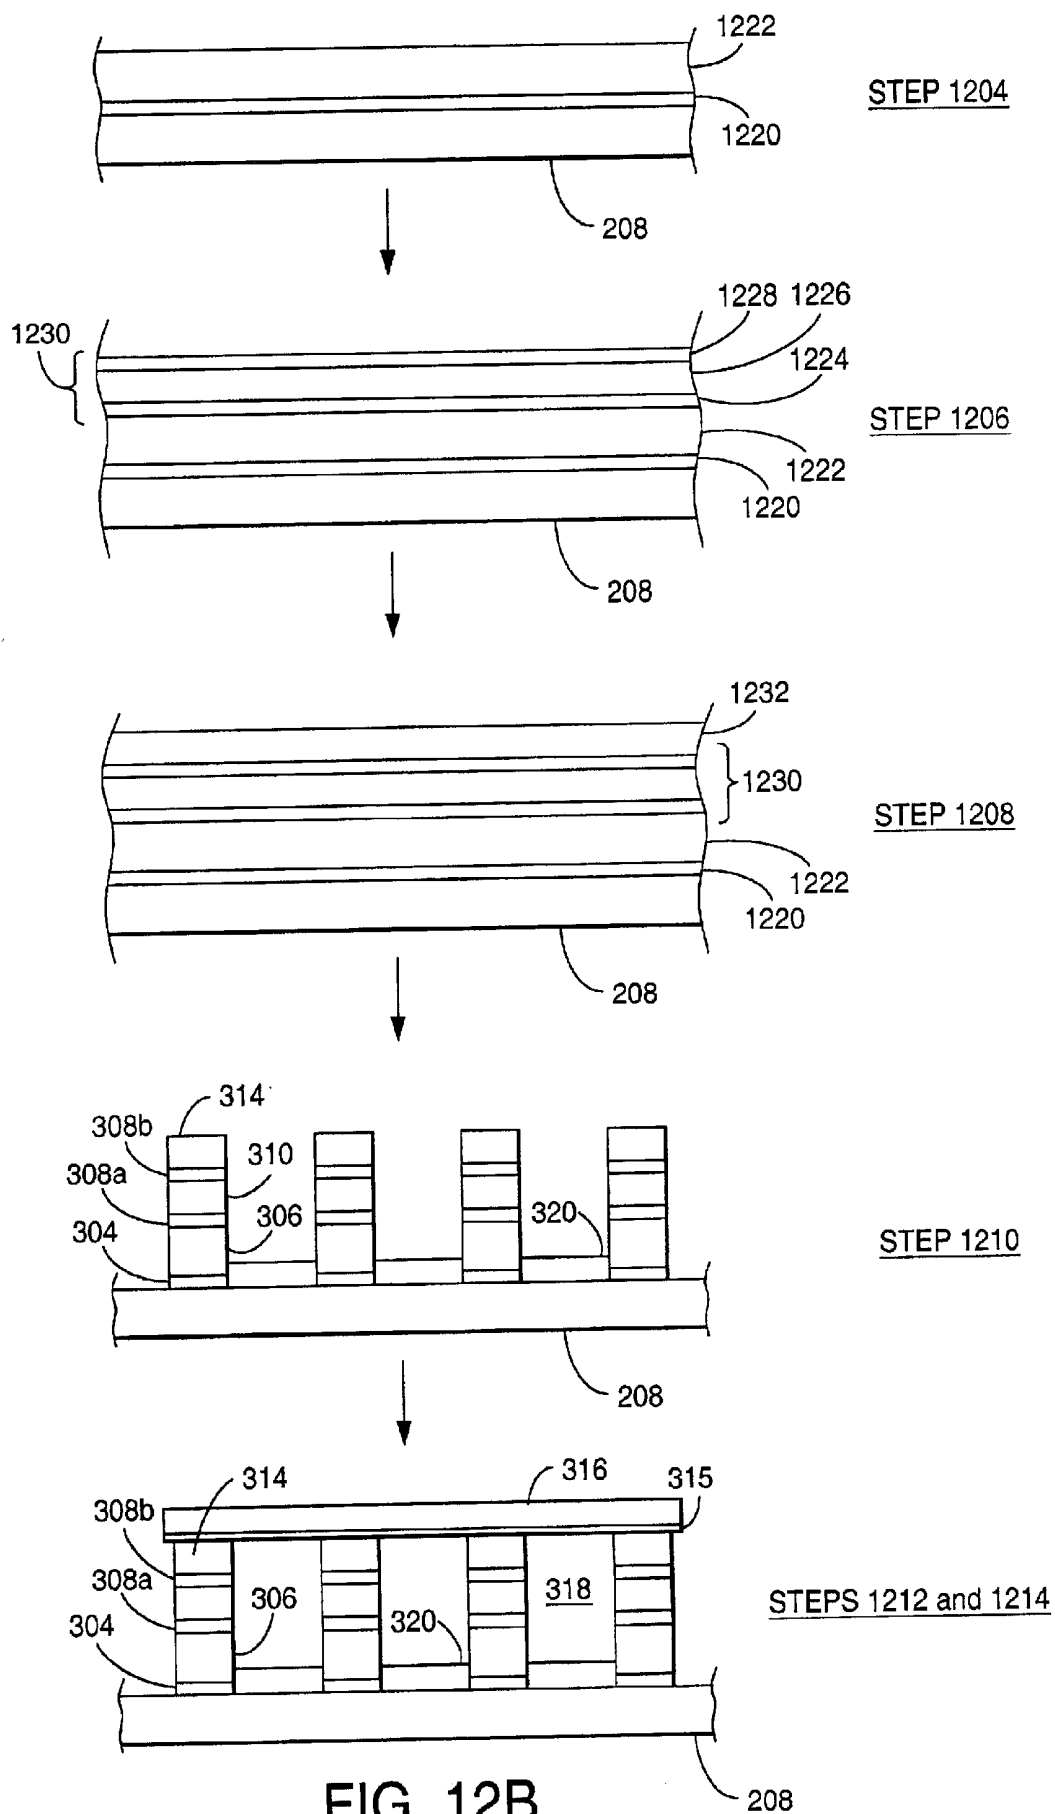

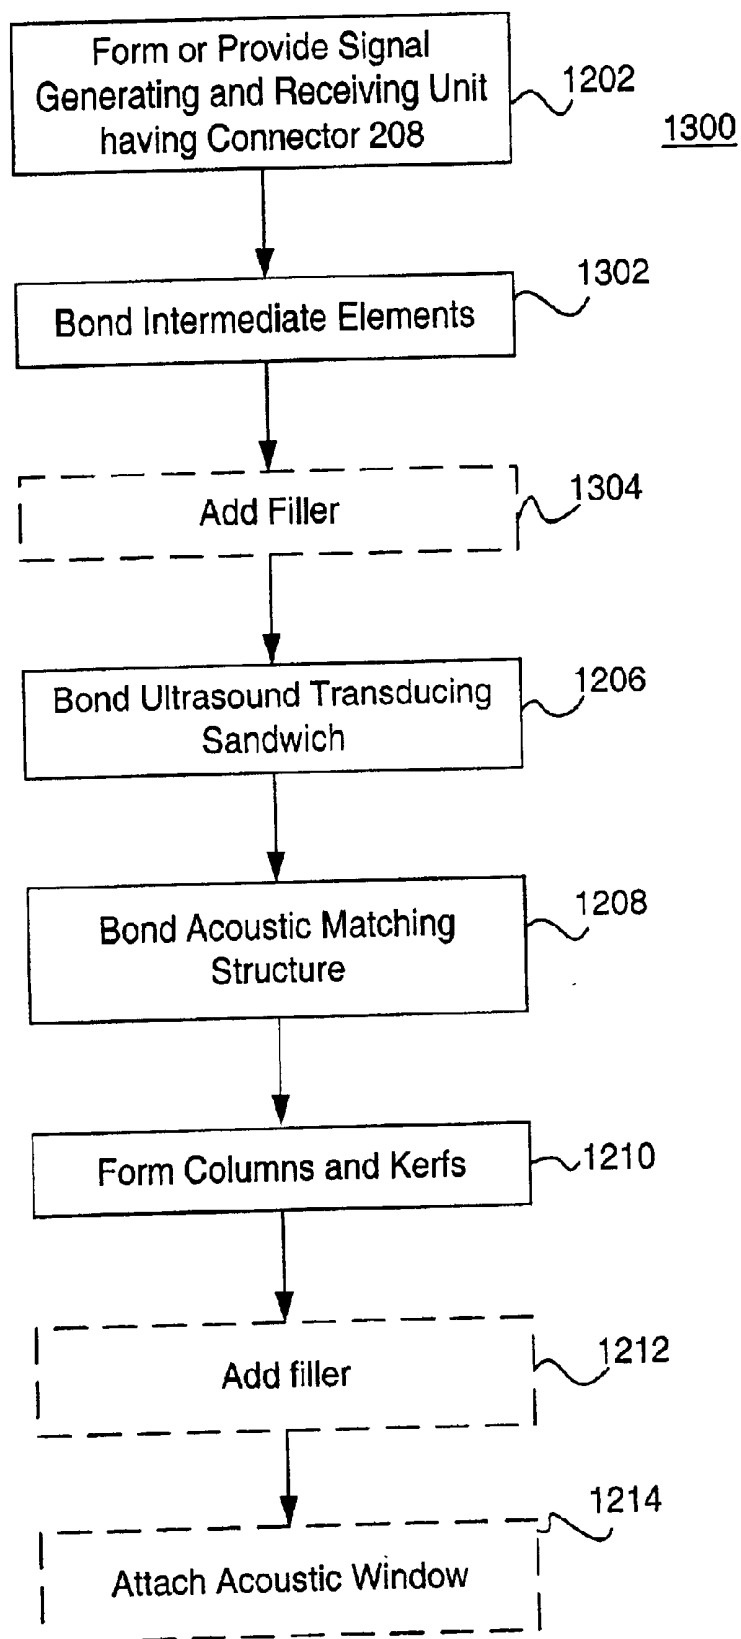


FIG. 13A

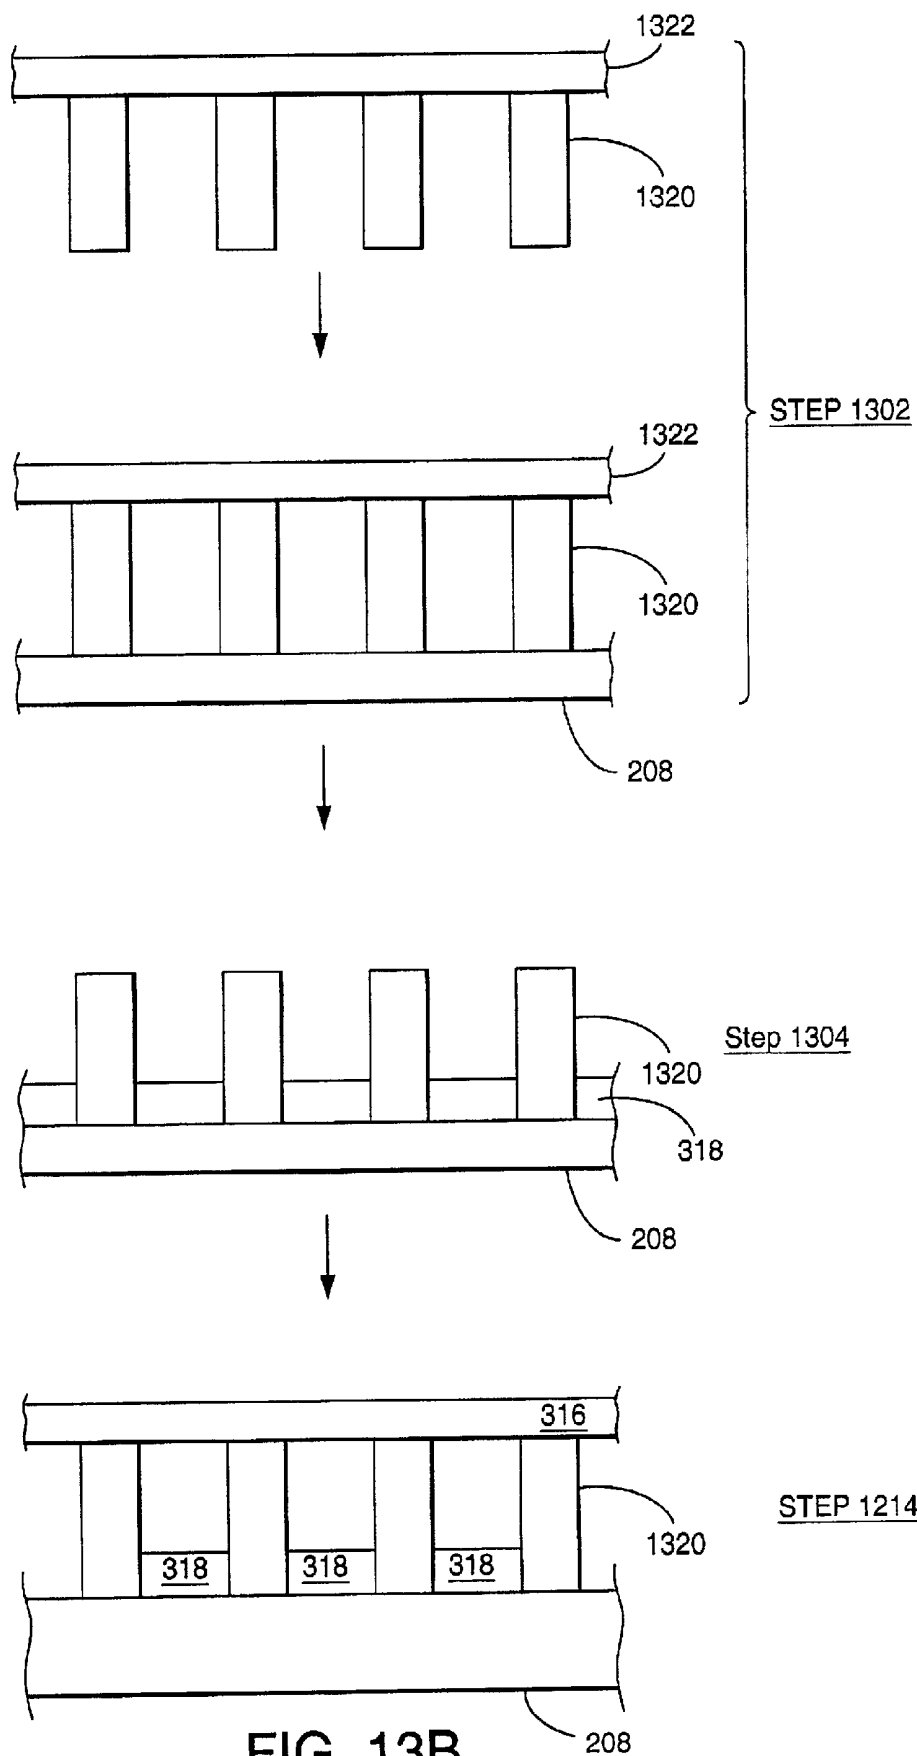


FIG. 13B

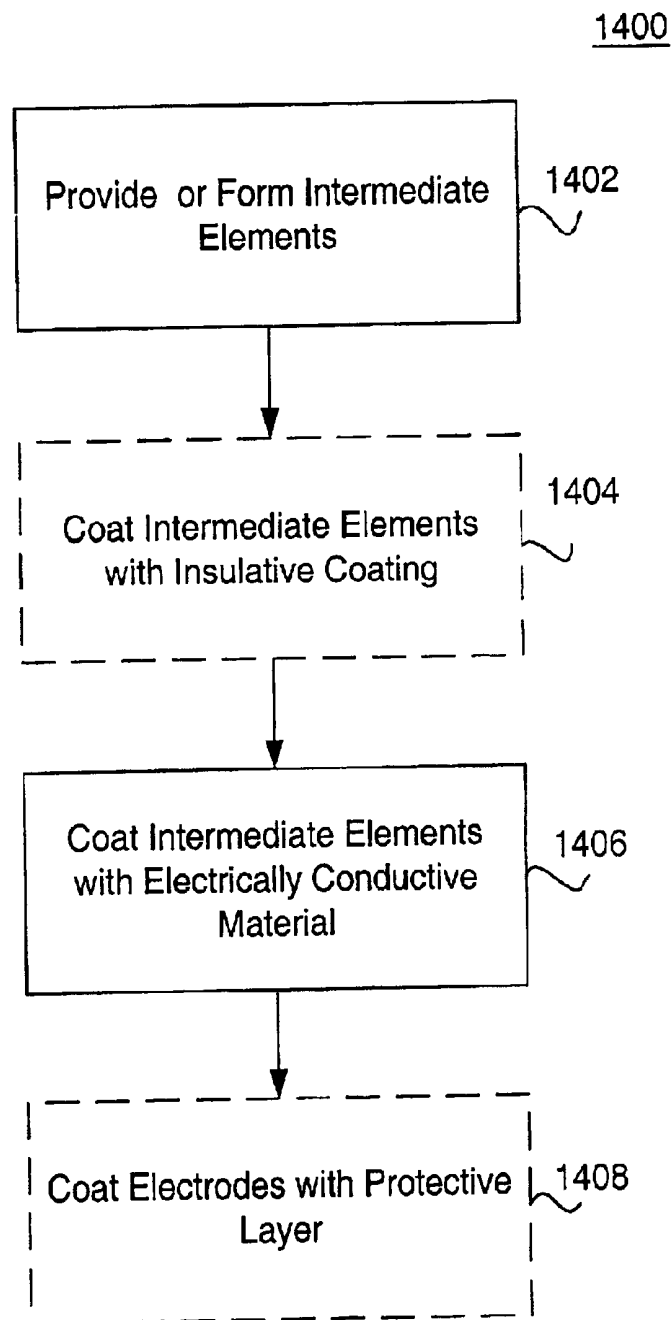


FIG. 14

ULTRASOUND SYSTEM WITH CABLELESS COUPLING ASSEMBLY

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part application of the U.S. patent application Ser. No. 09/860,209, entitled "Miniaturized Ultrasound Apparatus and Method," filed May 18, 2001 and now U.S. Pat. No. 6,569,102, which is a continuation application of U.S. Pat. application Ser. No. 09/378,175, entitled "Miniaturized Ultrasound Apparatus and Method," filed Aug. 20, 1999 and now U.S. Pat. No. 6,251,073. This application is also related to U.S. patent application Ser. No. 10/211,391, entitled "Broad Beam Imaging," and now U.S. Pat. No. 6,685,245.

BACKGROUND OF THE INVENTION

1. Field of the Invention

The invention is in the field of imaging devices and more particularly in the field of portable high-resolution three-dimensional ultrasonic imaging.

2. Description of Prior Art

Ultrasonic imaging is a frequently used method of analysis. The technique is used to examine a wide range of materials and is especially common in medicine because of its relatively non-invasive nature, low cost, and fast response times. Typically, ultrasonic imaging is accomplished by generating and directing ultrasonic waves into a material under investigation. This ultrasonic imaging uses a set of ultrasound generating transducers and then observing reflections generated at the boundaries of dissimilar materials, such as tissues within a patient, also uses a set of ultrasound receiving transducers. The receiving and generating transducers may be arranged in arrays and are typically different sets of transducers but may differ only in the circuitry to which they are connected. The reflections are converted to electrical signals by the receiving transducers and then processed, using techniques known in the art, to determine the locations of echo sources. The resulting data is displayed using a display device, such as a monitor.

The beam intensity as a function of position may oscillate rather than fall off monotonically as a function of distance from the center of the beam. These oscillations in beam intensity are often called "side lobes." In the prior art, the term "apodisation" refers to the process of affecting the distribution of beam intensity to reduce side lobes. However, in the remainder of this specification the term "apodisation" is used to refer to tailoring the distribution of beam intensity for a desired beam characteristic such as having a Gaussian or sinc function distribution of beam intensity (without the side lobes).

Steering refers to changing the direction of a beam. Aperture refers to the size of the transducer or group of transducers being used to transmit or receive an acoustic beam.

The prior art process of producing, receiving, and analyzing an ultrasonic beam is called beam forming. The production of ultrasonic beams optionally includes apodisation, steering, focusing, and aperture. Using a prior art data analysis technique each ultrasonic beam is used to generate a one dimensional set of echolocation data. In a typical implementation, a plurality of ultrasonic beams are used to scan a multi-dimensional volume.

Typically, the ultrasonic signal transmitted into the material under investigation is generated by applying continuous

or pulsed electronic signals to a transducer. The transmitted ultrasound is commonly in the range of 40 kHz to 10 MHz. The ultrasonic beam propagates through the material under investigation and reflects off of structures such as boundaries between adjacent tissue layers. As it travels, the ultrasonic energy may be scattered, resonated, attenuated, reflected, or transmitted. A portion of the reflected signals are returned to the transducers and detected as echoes. The detecting transducers convert the echo signals to electronic signals for processing using simple filters and signal averagers. After beam forming, an image scan converter uses the calculated positional information to generate two dimensional data that can be presented as an image. In prior art systems the image formation rate (the frame rate) is limited by at least the return time of an ultrasonic pulse. The pulse return time is the time between the transmission of ultrasound into the media of interest and the detection of the last reflected signals.

As an ultrasonic pulse propagates through a material of interest, additional harmonic frequency components are generated, which are analyzed and associated with the visualization of boundaries, or image contrast agents designed to re-radiate ultrasound at specific harmonic frequencies. Unwanted reflections within the ultrasound device can cause noise and the appearance of artifacts in the image.

One-dimensional acoustic arrays have a depth of focus that is usually determined by a nonadjustable passive acoustic focusing means that is affixed to each transducer. This type of focusing necessitates using different transducers for different applications with different depths of focus.

Two-dimensional transducer arrays used for high-speed three-dimensional imaging applications suffer from sensitivity loss caused by coupling multiple signal transfer and distribution systems to ultrasound systems. Two-dimensional transducers used for high-speed three-dimensional imaging applications must have a large number of pixels for two-dimensional steering capability with high resolution. High numbers of radiating/receiving pixels inevitably result in high electrical impedances per pixel in many types of transducers (e.g., piezoelectric, capacitive Micro ElectroMechanical (MEM) transducers), making high-resolution two-dimensional arrays impractical.

To reduce the impedance, many prior art devices use a limited number of elements, or a one-dimensional array. In typical ultrasound systems, these high impedance elements are driven by a typical coaxial cable bundle carrying as many micro-coaxial cables as the number of pixels, with each micro-coaxial cable usually having 50-75 Ohm impedance. These cables do not directly interconnect to the individual elements of the two-dimensional array. Another level of interconnection in the form of multi-layer Printed Circuit Boards (PCBs) co-fired ceramic boards or multi-layer flexes must transfer the signal to the transducer elements. The transducer elements are grouped into pixels each containing one or more transducer elements. For example, each pixel may contain one transmitting and one receiving transducer element. Systems including cables suffer from drawbacks that include, (1) the large number of required micro-coaxial elements makes the cable bundle unwieldy, and (2) the 50-75 ohm cable impedance cannot efficiently interface with or match the high electrical impedances of the individual transducer elements. These drawbacks result in impractically low sensitivity levels. The use of an additional multilayer transition device to connect from cables to transducer elements, introduces additional capacitive loading and crosstalk.

FIG. 1 shows a prior art ultrasonic imaging device 100, including a system 102, a first connector 104, a cable 106,

a second connector **108**, and a hand held unit **109**, which includes a multilayer structure **110** for transmitting the signal, interposing electrical connector structure (not shown), acoustic elements **114**, and pins **116**. System **102** may include a systems motherboard. The multilayer structure **110** could be a PCB, co-fired ceramic board, or flex circuits, for example. The interposing electrical connector structure (not shown) could be an interposing media for carrying signals from the multilayer structure **110** to acoustic elements **114**. The device of FIG. **1** is bulky and can be difficult to move and manipulate because cable **106** has many wires in it and therefore interferes with movement. Cable **106** also needs to be thick and therefore does not bend easily. Handheld unit **109** has electrical contact pads **116** for individually powering the acoustic elements **114**.

SUMMARY OF THE INVENTION

An embodiment of the invention provides a miniaturized ultrasound system generating and receiving unit such as a motherboard with two-dimensional signal addressing capability whereby first connector **104**, cable **106**, and second connector **108** of the prior art device in FIG. **1** can be eliminated. The system may have a system motherboard coupled via a cableless coupling to a transducer array. In one embodiment, the cableless coupling is also wireless (e.g., using the radio-frequency spectrum for transmitting and receiving data and signals). The system may include a two-dimensional surface interconnection between the transducer array and the signal generation and/or detection system, which eliminates the impractically thick and heavy cable. In one embodiment, the signal generation and/or detection system may be electrically matched to the transducer elements increasing the sensitivity more than were transducer elements not matched to the signal generation and/or detection system. The two-dimensional interconnection on the motherboard may be used without any other two-dimensional interconnection. In another embodiment, the electrical connection to the two-dimensional array elements are made via many flex circuits (e.g., printed circuit patterns using a layer of copper foil over a polymer base allowing for multidimensionality whereby the circuit may move, bend and twist without damage to the conductor), each coming from one row of elements, which may be terminated directly on the motherboard row of pads. Flex circuits should not be confused with ribbon cables (e.g., those cables made of normal, round insulated wires arranged side-by-side and fastened together by a cohesion process to form a flexible ribbon).

The two-dimensional array may perform multiple tasks. The motherboard system and the transducers may be designed to provide a sufficient percentage of the bandwidth for multiple frequency operations. For example, for many ultrasound transducers 100% of the bandwidth is necessary for multiple frequency operations. In an embodiment, the depth of focus is not fixed by the physical construction of the array, but is controlled by the area forming electronics and the system software, by active electrical phasing of the two-dimensional array elements. Alternatively, different transducers for different applications with different depths of focus can be used. Changing from one transducer to another can be facilitated by having a high density connector (i.e., a connector having a high density of connector contact pads, one pad for each transducer element (e.g., pixel) of the two-dimensional array) between the two-dimensional array and the system motherboard.

The invention may provide acoustically attenuating mounting posts with low electrical resistance, for example,

and allow the two-dimensional arrays of acoustical elements to have a higher sensitivity than were the posts not present. The height of the posts allows the transducer to be oriented for convenient use even though it is an integral part of the motherboard, an other interconnection device, or an other system for example. The permanent connection with the motherboard requires the design of the transducer to provide sufficient bandwidth for multiple frequency operation.

In one embodiment the two-dimensional array is permanently integrated with the motherboard. The depth of focus of the two-dimensional array is not fixed by the physical construction of the array, but is controlled by the area forming electronics and system software, which determine the active phasing of the two-dimensional array elements. This method of control eliminates the necessity of using different transducers for different applications with different fixed depths of focus and allows one transducer affixed to the motherboard, for example, to perform multiple tasks. In another embodiment of this invention different two-dimensional arrays with different depths of focus, frequency, and other characteristics can be plugged to the system motherboard without an intervening cable via the high density connector.

Broad beam technologies refer to systems and methods that include or take advantage of techniques for generating ultrasound and analyzing detected echoes such that multidimensional spatial information obtainable from a single ultrasonic pulse.

Area forming is the process of producing, receiving, and analyzing an ultrasonic beam, that optionally includes apodisation, steering, focusing, and aperture control, where a two dimensional set of echolocation data can be generated using only one ultrasonic beam. Nonetheless, more than one ultrasonic beam may still be used with the area forming even though only one is necessary. Area forming is a process separate and distinct from beam forming. Area forming may yield an area of information one transmit and/or receive cycle, in contrast to beam forming that typically only processes a line of information per transmit and/or receive cycle. Alternatively, beam forming can be used instead of area forming electronics throughout this application.

Volume forming is the process of producing, receiving, and analyzing an ultrasonic beam, that optionally includes apodisation, steering, focusing, and aperture control, where a three dimensional set of echolocation data can be generated using only one ultrasonic beam. Nonetheless, multiple ultrasonic beams may be used although not necessary. Volume forming is a superset of area forming.

Multidimensional forming is the process of producing, receiving, and analyzing an ultrasonic beam, that optionally includes apodisation, steering, focusing, and apertures, wherein a two or more dimensional set of spatial echolocation data can be generated using only one ultrasonic beam. Nonetheless, multiple ultrasonic beams may be used although not necessary. Multidimensional forming optionally includes non-spatial dimensions such as time and velocity.

In the above discussion although the motherboard is specified as the signal generating and receiving unit, it is only by way of example and any signal generating and receiving unit can be used.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. **1** is a prior art ultrasound device;

FIG. **2** is an overview of an embodiment of the invention;

FIG. **3** shows the details of the structure of FIG. **2** according to an embodiment of the invention;

FIG. 4 is an alternative embodiment of the structure of FIG. 2;

FIG. 5 is a more detailed illustration of FIG. 4;

FIG. 6 is another embodiment of the structure of FIG. 2;

FIG. 7 is another embodiment of the structure of FIG. 2;

FIG. 8 is another embodiment of the structure of FIG. 2;

FIG. 9 is another embodiment of the structure of FIG. 2;

FIG. 10 is another embodiment of the structure of FIG. 2;

FIG. 11A is a flowchart of a method of transmitting an acoustic signal;

FIG. 11B is a flowchart of a method of receiving an acoustic signal;

FIG. 12A is a flowchart of a method of making an embodiment of the invention;

FIG. 12B illustrates the structure at various stages of the method of FIG. 12A;

FIG. 13A is a flowchart of a method of making an embodiment of the invention of FIGS. 4-10;

FIG. 13B illustrates the structure at various stages of the method of FIG. 13A; and

FIG. 14 is a flowchart of a method for making intermediate elements of an embodiment of the invention.

DETAILED DESCRIPTION OF THE INVENTION

FIG. 2 is an overview of one embodiment of the invention. FIG. 2 shows a handheld ultrasound device 200 that includes an ultrasound transducing structure 202 coupled via a cableless coupling 203 to a signal generating and receiving unit 210. The cableless coupling 203 includes an intermediate structure 204, an electrically conducting structure 206, a connector 208. The connector 208 is coupled to the signal generating and receiving unit 210, which are secured within housing 212, and cooperates with cableless coupling 203.

The signals from or to intermediate structure 204 pass through electrically conducting structure 206, connector 208, and the signal generating and receiving unit 210. Ultrasound transducing structure 202 generates, or pulses, in response to signals received via intermediate structure 204, or receives ultrasonic waves and converts them to electrical signals, then sends them to intermediate structure 204.

In an embodiment cableless coupling 203 is also wireless. Signal generating and receiving unit 210 can be an integrated circuit or a system including a motherboard and may also include one or more child boards, for example. Intermediate structure 204 is an electrically coupled and acoustically isolating structure that serves to reduce crosstalk between the elements of the ultrasound transducing structure 202. Additionally, intermediate structure 204 protects ultrasound transducing structure 202 from external or internal acoustical noise and conducts the electrical signal to ultrasound transducing structure 202.

Ultrasound transducing structure 202, intermediate structure 204, and electrically conducting structure 206 may be divided into multiple elements that may be arranged in a periodic lattice. The lattice may be rectangular or hexagonal, for example. Electrically conducting structure 206 may be pads or may be interlocking male and female pins, for example, joining intermediate structure 204 and connector 208. Signal generating and receiving unit 210 may be a system motherboard, for example, and may have a connector 208 that can be a Printed Circuit Board (PCB), co-fired ceramic board, or the like, for signal transmission and distribution. Connector 208 may be a separate component

attached to signal generating and receiving unit 210 or may be an integral part of signal generating and receiving unit 210. For example, connector 208 may be a connector region coupled to or on a motherboard. (Throughout this specification the word "on" is to be understood as generic to being an integral part of and to being a separate structure that allows two structures to be attached together. Thus, whenever the specification discusses the connector 208 being "on" signal generating and receiving unit 210 it is to be read as generic to connector 208 being an integral part of and being a separate structure attached to signal generating and receiving unit 210.) Signal generating and receiving unit 210 may include one or more signal processors. The small size of the handheld ultrasound device may allow ultrasound transducing structure 202 to be easily positioned for imaging at a variety of angles.

Alternatively, a section of housing 212 can be made of a flexible material to allow the positioning of the transducer structure 202. Signal generating and receiving unit 210 may be kept small enough and/or may have a section that is made from flexible material to allow handheld ultrasound unit 200 to be flexed, thereby allowing ultrasound transducing structure 202 to be easily positioned for imaging.

FIG. 3 shows the details of the structure of FIG. 2 according to one embodiment of the invention. The FIG. 3 embodiment, which is a first embodiment 300, includes transducer 302 having electrical pads 304, intermediate elements 306, electrical contacts 308 *a* and *b*, which sandwich therebetween an active acoustic element 310, acoustic transducing element 312, acoustic matching element 314, ground sheet 315, optional acoustic window 316, optional filler 318, and optional adhesive 320.

Connector 208 on signal generating and receiving unit 210 of the ultrasound system is coupled to transducer 302. The collection of electrical pads 304 are one embodiment of electrically conducting structure 206. In an embodiment, a two-dimensional array of all electrical pads 304 make up electrically conducting structure 206, and are coupled to intermediate elements 306, which make up intermediate structure 204. Electrical pads 304 can be pure materials, alloys, or any mixture of chromium, nickel, silver, copper, gold, tin, tin oxide, indium and/or indium oxide, or any conductive material, for example. Acoustic transducing element 312 includes electrical contacts 308 *a* and *b*, which sandwich therebetween an active acoustic element 310. Active acoustic element 310 can be made with any acoustically active material (i.e., any material capable of converting a sound signal to an electrical signal and visa versa) such as piezoelectric materials such as quartz, lithium niobate, lithium sulfate, ceramic materials, lead zirconate titanate, barium titanate, and lead metaniobate, or other sound generating devices such as micromachined structures. Electrical contacts 308 *a* and *b* can be made from materials including, pure materials, alloys, or any mixture of chromium, nickel, silver, copper, gold, tin, tin oxide, indium and/or indium oxide, or any conductive material, for example.

The sandwich of active acoustic element 310 and electrical contacts 308 *a* and *b* form an acoustic transducing element 312 for generating and/or receiving ultrasound. In the case of a micro-machined device, the sandwich of active acoustic element 310 and electrical contacts 308 *a* and *b* may be replaced by the micro-machined element and its contacts, which may or may not have a sandwich structure. Acoustic transducing element 312 may also include an acoustic matching element 314 and an optional acoustic window 316. Optional acoustic window 316 may provide electrical isolation protecting a media of interest, such as a patient, from

electrical shock. Optionally, acoustic matching element **314** may provide electrical isolation instead of, or in addition to, the electrical isolation provided by optional acoustic window **316**. Acoustic matching element **314** may be an assembly of acoustic matching sub-elements. For example, acoustic matching element **314** may have several different layers. Acoustic matching element **314** may be made from materials or mixtures of materials with acoustic matching properties. In an embodiment, acoustic matching element **314** electrically couples electrical contact **308b** to ground sheet **315** thereby providing a return to ground. Alternatively, ground sheet **315** need not be included because optional acoustic window **316** can be made from a conductive material and act as a ground sheet. Further, alternatively, electrical contacts **308b** may be electrically coupled together forming one sheet, for example, that may be used for a return to ground. In this alternative embodiment, acoustic matching element **314** may or may not be conductive. Joining electrical contacts **308b** into one sheet increases the difficulty of acoustically isolating transducers **302**. But if the acoustical impedance of the conductive material joining electrical contacts **308b** is mismatched, for example, acoustic isolation can be achieved despite the joining material. Optional filler **318** may be placed between intermediate elements **306**, completely or partially filling the voids or kerfs (i.e., the spaces between transducers **302**). Optional filler **318** may be epoxy resin or other polymers and may include additives to modify filler characteristics. An optional adhesive **320** may be used to secure transducer **302** via electrical pads **304** to connector **208**. Optional adhesive **320** may be insulating or conducting adhesives such as epoxy, polyurethane, or silicone with or without various additives for different properties.

Transducers **302** differ from prior art transducers in that they are mounted directly to connector **208** of signal generating and receiving unit **210**. Alternatively, structures of intermediate elements **306** that are different from the prior art may also be used.

In another embodiment transducer **302** is mounted on a high density connector (not shown), which is plugged into a corresponding connector **208** of the signal generating and receiving unit **210**. The high density connector allows the acoustic transducing element **312** to be positioned further from connector **208**. Structures of intermediate elements **306** are further discussed below. Also, the close proximity of transducers **302** to connector **208** may affect the structural, acoustical, and electrical requirements of transducers **302**. Consequently, the set of elements that produce optimal performance for transducers **302** may be different than those of similar prior art transducers.

Intermediate elements **306** may serve as posts or columns, and can have a cross section of any shape. For example, the cross section of intermediate elements **306** can be square, rectangular, circular, oval, triangular, diamond-like, trapezoidal, rhombus-like, or polygonal in shape. Intermediate elements **306** can be a mixture of any of, any combination of, or all of epoxy, polyurethane, and/or silicone, for example. Intermediate elements **306** may also contain heavy particles of any shape or spheres made from material such as tungsten, and may further contain light particles, bubbles, and/or microspheres, which help attenuate sound. The light particles and microspheres can be made from glass and/or plastic, for example. Additionally, intermediate elements **306** may contain graphite or other electrically conductive particles, which also help attenuate sound. Electrically conductive particles could be used as some or all of the heavy and/or light particles, depending on the ranges of density of the conducting particles chosen.

The signal from signal generating and receiving unit **210** is brought through the layers and structures of connector **208** to electrical pads **304** on connector **208**'s surface. Electrical pads **304**, intermediate elements **306**, and acoustic transducing elements **312** may be stacked one on top of the other and form the above-mentioned two-dimensional lattice. Acoustic transducing elements **312** may transform the electrical signals to sound waves, or may convert acoustic sound waves to electrical signals. Acoustic transducing elements **312** may be arranged in the same lattice as electrical pads **304**, and electrically addressed via signal distribution within signal generating and receiving unit **210**.

Intermediate elements **306** form an interconnecting backing media that transmits electrical signals between electrical pads **304**, on connector **208** of signal generating and receiving unit **210**, and electrical contacts **308a**, on acoustic transducing elements **312**. Intermediate elements **306** may have an electrical conductivity that is high enough to minimize signal loss. The signal loss due to the intermediate element **306** is the power loss (I^2R , where I is the total current flowing through the array of intermediate elements **306** and R is effective resistance of the array of intermediate elements **306**) caused by the resistance of the intermediate element. For example, in an embodiment the conductivity of the intermediate element is adjusted so that the signal loss is kept less than 1 DB.

The total length of the interconnecting media in the direction perpendicular to connector **208** on signal generating and receiving unit **210** and the resistivity of this media are the main factors determining the total resistance of each electrical coupling between acoustic transducing elements **312** and electrical pads **304**. Thus, the resistivity of the intermediate elements **306** limit the elements' length, which in turn limits the intermediate structure **204**'s thickness. Intermediate elements **306** may have adequate acoustical attenuation or impedance to avoid sound reflections from connector **208** of the signal generating and receiving unit **210** that would otherwise reach acoustic transducing elements **312**. Intermediate elements **306** may provide mechanical integrity and positioning accuracy of acoustic transducing elements **312** and connector **208** of signal generating and receiving unit **210**.

The interconnecting backing media used for intermediate elements **306** may be an electrically anisotropic conducting media that conducts electricity in a direction perpendicular to the surface of the electrical pads **304**. The interconnecting backing media may be used to bond acoustic transducing elements **312** to electrical pads **304** on connector **208** of signal generating and receiving unit **210**. Intermediate elements **306** may be made from an electrically conductive and acoustically lossy media. An appropriate anisotropic electrical conduction media can be made by incorporating a sparse concentration of conducting elements and/or particles into an electrically insulating medium. The density of the sparse concentration is such that the conducting elements and/or particles do not touch each other in a direction perpendicular to the flow of electrical current due to their low density. The conducting elements and/or particles may have an elongated shape, and the conducting elements are oriented with their longer dimension to reach and make electrical contact on either side of the insulating medium in which they are located. The elements can be whiskers, wires, or arbitrary shapes of conducting media tending to extend the entire length of intermediate element **306**. Alternatively, the conducting elements and/or particles may be significantly shorter than and kept relatively parallel to the long direction of intermediate elements **306**. The conductive

elements should be long enough so that at least a significant number of them tend to touch one another along the length of the particles, but not along the width. The use of an anisotropic conductor reduces the chances of shorting between adjacent intermediate elements **306** when compared to an isotropic conductor.

Alternatively, an isotropic electrically conducting and acoustically appropriate medium may be used to bond the array of acoustic transducing elements **312** to the two-dimensional array of electrical pads **304**. Electrical shorts between the intermediate elements **306** can be removed by eliminating the excess media causing the short via mechanical dicing, various ion, electron, plasma, chemical erosion, or other processes.

Optional filler **318** may be an insulator that helps minimize electrical shorting and may have suitable acoustical impedance to prevent crosstalk between transducers **302**. It may be desirable to minimize crosstalk by leaving the kerfs near transducers **302** void of filler. Optional filler **318** can be an acoustically attenuating material or a material with a highly mismatched acoustical impedance to transducer **302**.

Optional adhesive **320** can be conductive or insulative. If optional adhesive **320** is conductive, it is placed primarily between electrical pads **304** and intermediate element **306**. Typically any excess optional adhesive **320** would be removed from the kerfs. However, it is not necessary to remove all of optional adhesive **320** from the kerfs even if it is conductive. The thinner a conductive film the more resistive it is to currents traveling in a plane. Also, the thinner a conductive film the more breaks, or discontinuities, it is likely to have in it. Consequently, if any of optional adhesive **320** is conductive and is in the kerfs, the optional adhesive **320** must be thin enough or have enough breaks so that it will act as an insulator in a direction parallel to the surface of connector **208** having electrical pads **304**, and the optional adhesive **320** must not cause any shorting.

Similarly, if optional adhesive **320** is insulative, it is placed primarily in the kerfs. Typically, all of optional adhesive **320** on electrical pads **304** is removed. However it is not necessary to remove all of optional adhesive **320** from the electrical pads **304**, even if it is insulative. The thinner an insulative film, the more likely it will be able to support a current traveling perpendicular to its surface via arcing, tunneling, or breaks in the insulative film, for example. Consequently, if optional adhesive **320** is insulative, the portion placed on electrical pads **304** must be thin enough or have enough holes in it to allow the flow of a current through it (such as by contact, arcing, or tunneling). Pressure applied while bonding intermediate elements **306** can be used to squeeze excess adhesive out from between the electrical pads **304** and the intermediate elements **306**.

In FIGS. 4–10 like components have been given the same alphanumeric labels. To simplify the drawings FIGS. 5–10 show no acoustic matching element **314**, ground sheet **315**, or optional acoustic window **316**, although they are present as in FIGS. 3 and 4. FIGS. 4–10 also share the same ultrasound transducing structure **202** and signal generating and receiving unit **210** as in FIG. 3. FIGS. 5–10 differ from one another primarily in the make up of intermediate structure **204**.

FIG. 4 is an alternative embodiment **400** of the structure of FIG. 2. Embodiment **400** has intermediate elements **406**, which are insulative and coated with a conductor **408** on any number of sides greater than two, including conductive pads **410a** and **b** located at both ends. Specifically, to explain what is meant by conductor **408** being coated on any number of

sides greater than two, conductive pads **410a** and **b** cover intermediate elements **406** on at least part of each of two of its ends. A portion of conductor **408** must also be placed at least partially on a third side of intermediate elements **406** to form an electrical coupling between conductive pads **410a** and **b**. Intermediate elements **406** may be columns or posts made from a mixture of any of, any combination of, or all of, epoxy, polyurethane, and/or silicone containing dense particles or spheres made from material such as, but not limited to, tungsten and bubbles, low density particles, and/or microspheres. The low density particles and microspheres may be made from glass and/or plastic, for example. Conductor **408** may be a thin film that provides electrical interconnection between acoustic transducing elements **312** and electrical pads **304** to which it is bonded or soldered. The conductor **408** may be exposed or covered. If conductor **408** is covered, it may be embedded within, intermediate elements **406** and/or covered by optional film **412**. Optional film **412** allows for the removal of any subsequently introduced optional filler **318** by mechanical means, such as dicing wheels, without the danger of damaging conductor **408**. Optional film **412** may be a thin film of insulating material or the same material as intermediate elements **406**. Conductor **408** may be replaced by conducting wires or whiskers that may be placed along the edges of, or embedded within intermediate elements **406**. Optional filler **318** may encapsulate conductor **408** completely, or partially, as shown in FIG. 4. Optional filler **318** may serve the purposes of providing structural integrity and acoustically isolating individual acoustic transducing elements **312**. Optional filler **318** may be of the same material as the posts used for intermediate elements **406** as long as it is insulative, or does not short transducers **302**; The higher the electrical conductivity of conductor **408**, the lower the signal's loss. In one embodiment, the electrical conductivity provided by conductor **408** may be made high enough to minimize signal loss. The total length of intermediate elements **406** in the direction perpendicular to the signal generating and receiving unit **210**, and the per length resistance of conductor **408**, will determine the total resistance of the individual couplings between the acoustic transducing elements **312** and electrical pads **304**. Due to the relatively high conductivity of metallic films or wires, it is practical to increase the thickness of intermediate structure **204**, to position the acoustic array surface to touch the patient in a comfortable way. Intermediate elements **406** may serve as posts or columns and can have a cross section of any shape. Intermediate elements **406** can have essentially the same mechanical and acoustical properties as intermediate elements **306**, and therefore may have the same composition, except for the lack of the conducting particles in intermediate elements **406**. Because intermediate elements **406** may have a lower resistance, intermediate elements **406** may be made taller than intermediate elements **306**. The mechanical properties of intermediate layer **406** may also be slightly different.

Conductor **408** and the bonding material (such as adhesives, solders, and welding material) should not cause acoustic reflections or perturbations. To avoid acoustic reflections or perturbations, the thickness and size of perturbing items within the acoustic path may be small compared to the acoustic wavelengths of interest. Conductor **408** should adhere to the insulating media well enough to retain the structure's mechanical. The insulating media used for intermediate elements **406** should have adequate acoustical attenuation to avoid sound reflections from connector **208** of signal generating and receiving unit **210** that would other-

wise reach acoustic transducing element **312**. The insulating media used for intermediate elements **406** should have suitable acoustic impedance for optimum performance. The insulating media of intermediate elements **406** may provide mechanical integrity and positioning accuracy of acoustic transducing element **312** and connector **208** of the signal generating and receiving unit **210**.

FIGS. **5** and **6** are the same as FIG. **4** except that the FIGS. **5** and **6** embodiments include optional adhesive **320**. Also, in the FIG. **5** embodiment conductor **408** is exposed, while in the FIG. **6** embodiment, conductor **408** is covered with optional film **412**.

FIG. **7** is another embodiment **700** having a coating of an insulative coating **702** made from Kapton™, or Mylar™, for example, on any number of sides greater than two including both ends, and having conductor **408** laminated thereon. The intermediate elements **704** can be the same as intermediate elements **406**, or can be a conductor.

FIG. **8** is another embodiment **800**, which is the same as that of embodiment **700** of FIG. **7**, except that an optional film **412** covers the exposed portion of conductor **408** and is intermediate conductor **408** and optional filler **318**.

Although FIGS. **6–8** show optional adhesive **320**, it does not need to be present.

FIGS. **9** and **10** are the same as FIGS. **7** and **8**, respectively, except that intermediate element **902** and optional film **1002** do not extend all the way down to conductive pads **410 a**, leaving a gap. The gap may be filled with optional filler **318**. If optional filler **318** is not used, the couplings to electrical pads **304** will remain flexible, thereby providing vibration isolation. If optional filler **318** is used, it provides mechanical integrity and holds the intermediate elements in place. The couplings to the rows and/or columns of electrical pads can be done at any stage of the construction of the interconnection-backing media, or after its completion. Intermediate elements **902** may be posts and can have a cross section of any shape. Intermediate elements **902** can have essentially the same mechanical and acoustical properties as intermediate elements **406** except that since intermediate elements **902** do not extend to conductive pads **410 a**, the mechanical properties can be slightly different.

Although FIGS. **9** and **10** do not show optional adhesive **320**, it could be included.

FIGS. **11A** and **B** show flow charts of methods **1100 a** and **b**, respectively, of using an embodiment of the invention. FIG. **11A** is a method of transmitting acoustic signals, and FIG. **11B** is a method of receiving acoustic signals.

Referring to FIG. **11A**, in step **1102** the signal generating and receiving unit **210** generates an electrical signal. In step **1104**, the electrical signal is cablelessly coupled via connector **208** and through a possible connector (not shown) and electrical pads **304** to intermediate structure **204**. In step **1106**, the electrical signal is coupled through intermediate structure **204** to acoustic transducing element **312**. In step **1108**, acoustic transducing element **312** generates an acoustic signal that is then transmitted via acoustical matching element **314** through optional acoustic window **316**.

Referring to FIG. **11B**, the ultrasonic signals from step **1108** (FIG. **11A**) are modified (e.g., reflected and/or transmitted) by the media of interest. In step **1122**, the modified ultrasonic signals are received. Optionally the reception includes transmitting the ultrasonic signals through the optional acoustical window **316**, and receiving them via acoustic matching element **314** by typically a different combination of acoustic transducing elements **312** because the direction of the incident and reflected ultrasound

signals is typically different. However, in an embodiment each acoustic transducing element **312** can be used both for receiving and transmitting the modified ultrasonic signal. In another embodiment each acoustic transducing elements **312** may be grouped into pixels having a receiving half and a transmitting half. The acoustic transducing elements **312** convert the ultrasonic signal into an electrical signal. In step **1124**, the electrical signals are sent through intermediate structure **204**. In step **1126**, the signals from intermediate structure **204** are sent via electrically conducting structure **206** through connector **208**. In step **1128**, the signals from connector **208** are sent back to signal generating and receiving unit **210** for processing to produce an image on a monitor or store as data for producing an image on a monitor. The receiving step may include attenuating reflections within the handheld ultrasound unit **200** such as with the use of optional filler **318** and acoustically the attenuating materials used in intermediate elements **306**, **406**, and **902**.

FIGS. **12A** and **B** show a method **1200** of making an embodiment of the invention, and some of the temporary structures formed at various stages of the process. In step **1202**, signal generating and receiving unit is formed or provided, and connector **208** is coupled to or formed on signal generating and receiving unit **210**. The rest of signal generating and receiving unit **210** can be formed, assembled, or constructed at anytime relative to forming or coupling connector **208** on signal generating and receiving unit **210**. In step **1204** an electrically conductive layer **1220** could be deposited on connector **208** for forming electrical pads **304**. Also in step **1204**, an electrically conductive and acoustically attenuating media **1222** is laminated on an electrically conductive layer **1220**. Further in step **1206**, a first conductive layer **1224**, an acoustically active layer **1226** and a second conductive layer **1228** form an acoustic transducing sandwich **1230**. Acoustic transducing sandwich **1230** is bonded to electrically conductive and acoustically attenuating media **1222**. Acoustic transducing sandwich **1230** could be first constructed and then bonded to electrically conductive acoustically attenuating layer **1222**, or it could be laminated layer by layer directly upon electrically conductive and acoustically attenuating media **1222**. In step **1208**, an acoustic matching layer **1232** is bonded to one side of acoustic transducing sandwich **1230**. Acoustic matching layer **1232** may include multiple layers and/or have significant structure to improve acoustic matching. In step **1210**, material is removed from the composite structure leaving columns and forming the kerfs. A small amount of connector **208** may also be removed during step **1210** in order to be certain that all of the conductive material between electrical pads **304** is removed, and optional adhesive **320** may be added. In step **1212**, optional filler **318** is added to the kerfs and allowed to harden. In step **1214**, optional acoustic window **316** is bonded to acoustic matching element **314**. Optional acoustic window **316** may have ground sheet **315** formed on it by metalization or deposition for example before being secured to acoustic matching element **314**.

FIGS. **13A** and **B** show a method **1300** of making an embodiment of the invention and some of the temporary structures formed at various stages of the process. In step **1202**, signal generating and receiving unit is formed or provided, and connector **208** is coupled to or formed on signal generating and receiving unit **210**, as in method **1200**. In step **1302**, electrically conductive and acoustically attenuating pillars that form intermediate elements **406** or **902** are attached to connector **208**. Although not shown in FIG. **13B**, intermediate elements **406** or **902** are formed with conductor **408**, optional film **412** or **1002**, and insulative coating **702**

13

attached thereto. Although also not shown in FIG. 13B, when intermediate elements 406 or 902 are attached to connector 208, intermediate elements 406 or 902 are bonded to electrical pads 304 on connector 208. Intermediate elements 406 or 902 with conductor 408, optional film 412 or 1002, and insulative coating 702 attached thereto may be formed as structures 1320 on a sheet 1322 so that they can be fixed in positions relative to one another and aligned with electrical pads 304. Structures 1320 may be first formed and then attached to sheet 1322 or may be formed on sheet 1322. The formation of structures 1320 is described in more detail in relation to FIG. 14, below. Alternatively, electrical pads 304 may be included in structures 1320, for example. After bonding structures 1320, to connector 208, sheet 1322 is detached. In optional step 1304, optional filler 318 may be added as a liquid and allowed to harden. In step 1206, an acoustic transducing sandwich is bonded to intermediate structure 204. The acoustic transducing sandwich includes a first conductive film, an acoustically active layer, and a second conductive film. The acoustic transducing sandwich could be first constructed and then bonded to the electrically conductive acoustically attenuating media, or could be laminated layer by layer directly upon the electrically conductive and acoustically attenuating media. Next in step 1206, material is removed from the transducing sandwich to form acoustic transducing elements 312. Alternatively, acoustic transducing elements 312 could also be formed on the same sheet 1322 while making the intermediate elements as part of structures 1320. Method 1300 then proceeds as in method 1200 with steps 1208, 1210, 1212, and 1214. Method 1300 may include neither of or just one of steps 1304 and 1212. Alternatively, part of the optional filler 318 may be added during step 1304 and part may be added during step 1212.

FIG. 14 shows a flowchart of method 1400 for making the intermediate elements of an embodiment of the invention. In step 1402 method 1400 starts with providing or forming intermediate elements 406 or 902, which may be formed on sheet 1322 or formed separately and then attached to sheet 1322 after the completion of method 1400. If structures 1320 (which form intermediate elements 406 or 902) are formed on sheet 1322 a conductive layer (not shown) is first be deposited on sheet 1322 and then an insulative layer (not shown) is deposited from the composite structure leaving columns to form conductive pads 410b attached to intermediate elements 406 or 902. Conductive pads 410b form a first part of conductor 408. Some material from sheet 1322 may also be removed or alternatively the conductive layer (not shown) may be left exposed and not separated into conductive pads 410 b. Optionally, in step 1404, intermediate elements 406 are coated with an insulative coating 702 some of which may be removed to expose the conductive layer (not shown) or conductive pads 410b. In step 1406, intermediate elements 406 are coated with conductor 408. However, if structures 1320 were formed on sheet 1322 then the part of conductor 408 that forms conductive pad 410b will already be present. The conductor 408 may be attached to insulating coating 702 or embedded within insulating coating 702 first and then attached to intermediate elements 406 via insulative coating 702. The conductive layer (not shown) is separated into conductive pads 410b if not already separated in step 1402. In optional step 1408, the conductor 408 is covered with optional film 412 or 1002. Optional film 412 or 1002 provides an insulating and protective coating thereby embedding conductor 408 in the composite structure formed by intermediate elements 406 or 902 and optional film 412 or 1002, respectively.

Although the word "structure" is used to describe many elements, these elements could also be assemblies, which in

14

this Application is generic to the word "structure" but also includes assemblies or collections of parts. The word "coupling" in this application is generic to direct connection and a connection made via an intermediate element as well as any other type of coupling, link or way of attaching elements together.

The invention could also be constructed using other signals, such as optical signals rather than electrical signals. In an optical embodiment electrically conducting structure 206 may be replaced with an optical connection, for example. Although the acoustic transducing elements 312 are depicted as having electrical contacts 308a and b, they are only necessary if electrical energy is used to excite the active acoustic elements 310. If the active acoustic elements 310 are excited by other forms of energy such as by using electric magnetic waves or mechanical energy, the electrical contacts 308a and b may not be used or may be replaced by coupling contacts for securing the active acoustic element in place.

Although the invention has been described with reference to specific embodiments, it will be understood by those skilled in the art that various changes may be made and equivalents may be substituted for elements thereof without departing from the true spirit and scope of the invention. In addition, modifications may be made without departing from the essential teachings of the invention.

What is claimed is:

1. An ultrasound system comprising:

a signal generating and receiving unit;

a cableless coupling assembly, the cableless coupling assembly comprising intermediate elements coupled to electrical pads wherein the intermediate elements comprise electrically conductive particles, and is configured to attenuate sound; and

an ultrasound transducing assembly coupled via the cableless coupling assembly to the signal generating and receiving unit wherein the ultrasound transducing assembly comprises:

at least one transducer configured to provide sufficient bandwidth for multiple frequency operation, the at least one transducer configured to be electrically matched to the signal generating and receiving unit.

2. An ultrasound system comprising:

at least one transducer configured to provide sufficient bandwidth for multiple frequency operation, the transducer comprising:

acoustic transducing elements; and

an acoustically isolating assembly connected to the acoustic transducing elements; and

a signal generating and receiving unit connected to the acoustically isolating assembly wherein the transducers are directly connected to the signal generating and receiving unit via a cableless connector and the signal generating and receiving unit is electrically matched to the at least one transducer.

3. The system of claim 2 wherein the acoustic transducing elements include at least an acoustically active material between two electrical contacts.

4. The system of claim 3 wherein the acoustic transducing elements include an acoustic matching assembly coupled to one of the two electrical contacts and an acoustic window coupled to the acoustic matching assembly.

5. The system of claim 2 wherein the signal generating and receiving unit includes a motherboard.

6. The system of claim 2 wherein a filler material is placed within kerfs formed by the acoustically isolating assembly.

15

7. The system of claim 2 wherein the acoustically isolating assembly includes posts of an electrically conductive and acoustically attenuating material.

8. The system of claim 7 wherein the posts are anisotropic conductors.

9. The system of claim 7 wherein the posts are isotropic conductors.

10. The system of claim 2 wherein the acoustically isolating assembly includes insulating posts having conductors for conducting electrical signals.

11. The system of claim 10 wherein the conductors are partially embedded within the posts.

12. The system of claim 10 wherein the conductors are attached to the outside of the posts.

13. The system of claim 10 wherein the conductors have an insulative backing that is coupled with the posts.

14. The system of claim 10 wherein the conductors are longer than and extend beyond the posts.

15. An ultrasound system comprising:

circuitry having a signal generating and receiving unit;

acoustic transducing elements configured to provide sufficient bandwidth for multiple frequency operation, and electrically matched to the circuitry, the acoustic transducing elements comprising:

an acoustically active material between two electrical contacts;

an acoustic matching assembly coupled to one of the two electrical contacts; and

an acoustic window coupled to the acoustic matching assembly;

a cableless coupling assembly coupled to the signal generating and receiving unit and the acoustic transducing elements wherein a transducer is directly connected to the signal generating and receiving unit via a connector, the cableless coupling assembly comprising: an acoustically isolating assembly having posts configured to be electrically conductive and acoustically attenuating, isolating the acoustic transducing elements; and

16

a filler material placed within kerfs formed by the acoustically isolating assembly.

16. The system of claim 15 wherein the posts are anisotropic conductors.

17. The system of claim 15 wherein the posts are isotropic conductors.

18. The system of claim 15 wherein the acoustically isolating assembly includes conductors for conducting electrical signals coupled to the posts.

19. The system of claim 18 wherein the conductors are partially embedded within the posts.

20. The system of claim 18 further comprising an acoustical index matching element.

21. The system of claim 18 wherein the conductors are attached to the outside of the posts.

22. The system of claim 18 wherein the conductors have an insulative backing that is coupled with the posts.

23. The system of claim 18 wherein the conductors are longer than and extend beyond the posts.

24. An ultrasound system comprising:

signal generating and receiving means;

ultrasound transducing means configured to provide sufficient bandwidth for multiple frequency operation, and electrically matched to the signal generating and receiving means;

cableless coupling means connected to the signal generating and receiving means and to the ultrasound transducing means wherein the ultrasound transducing means are directly connected to the signal generating and receiving means via connection means, including means for acoustically isolating the ultrasound transducing means from the signal generating and receiving means, and

means for conducting electricity; and

acoustic backing means for attenuating acoustic reflections.

* * * * *

专利名称(译)	超声波系统，带无线耦合组件		
公开(公告)号	US6936008	公开(公告)日	2005-08-30
申请号	US10/039910	申请日	2001-10-20
[标]申请(专利权)人(译)	TARAKCI UMIT IMRAN Mir上 MCLAUGHLIN GLEN 十一旭峰		
申请(专利权)人(译)	TARAKCI UMIT IMRAN MIR A. MCLAUGHLIN GLEN 十一旭峰		
当前申请(专利权)人(译)	深圳迈瑞生物医疗电子股份有限公司.		
[标]发明人	TARAKCI UMIT IMRAN MIR A MCLAUGHLIN GLEN XI XUFENG		
发明人	TARAKCI, UMIT IMRAN, MIR A. MCLAUGHLIN, GLEN XI, XUFENG		
IPC分类号	A61B8/08 G01S15/89 G01S15/00 A61B8/06 G01N29/24 A61B8/00 G01S7/521 H04R1/02		
CPC分类号	A61B8/08 A61B8/4438 A61B8/4455 A61B8/4472 A61B8/462 A61B8/463 A61B8/465 A61B8/467 G01S7/52034 G01S7/52079 G01S7/5208 G01S7/52082 G01S7/52084 G01S7/52096 G01S15/8981 A61B8/06 A61B8/0833 A61B8/0866 A61B8/13 A61B8/468 A61B8/488 G01S15/8979		
其他公开文献	US20020138002A1		
外部链接	Espacenet USPTO		

摘要(译)

一种超声成像设备，具有无线耦合，用于将二维超声换能器阵列耦合到诸如母板的信号产生和接收单元。该耦合包括声学衰减和导电结构，其可以包括导电或电绝缘的柱，其具有嵌入或安装在外表面上的导体。还可以存在高密度连接器，允许二维阵列与主板耦合和分离。

