



US 20100256490A1

(19) **United States**

(12) **Patent Application Publication**

Makin et al.

(10) **Pub. No.: US 2010/0256490 A1**

(43) **Pub. Date: Oct. 7, 2010**

(54) **MEDICAL SYSTEM HAVING AN  
ULTRASOUND SOURCE AND AN ACOUSTIC  
COUPLING MEDIUM**

(76) Inventors: **Inder Raj S. Makin**, Loveland, OH (US); **T. Douglas Mast**, Cincinnati, OH (US); **Michael H. Slayton**, Tempe, AZ (US); **Peter G. Barthe**, Phoenix, AZ (US); **Jeffrey D. Messerly**, Cincinnati, OH (US); **Waseem Faidi**, Clifton Park, NY (US); **Megan M. Runk**, Cincinnati, OH (US)

Correspondence Address:

**PHILIP S. JOHNSON**  
**JOHNSON & JOHNSON**  
**ONE JOHNSON & JOHNSON PLAZA**  
**NEW BRUNSWICK, NJ 08933-7003 (US)**

(21) Appl. No.: **12/818,261**

(22) Filed: **Jun. 18, 2010**

**Related U.S. Application Data**

(63) Continuation of application No. 10/848,550, filed on May 18, 2004.


**Publication Classification**

(51) **Int. Cl.** *A61N 7/00* (2006.01)  
*A61B 8/00* (2006.01)

(52) **U.S. Cl.** ..... **600/439**

(57) **ABSTRACT**

An ultrasound medical system has an end effector including a medical ultrasound transducer and an acoustic coupling medium. The acoustic coupling medium has a transducer-proximal surface and a transducer-distal surface. The medical ultrasound transducer is positioned to emit medical ultrasound through the acoustic coupling medium from the transducer-proximal surface to the transducer-distal surface. The end effector is adapted to change a property (such as the shape and/or the temperature) of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient. In one example, such changes are used to change the focus and/or beam angle of the emitted ultrasound during the medical procedure.

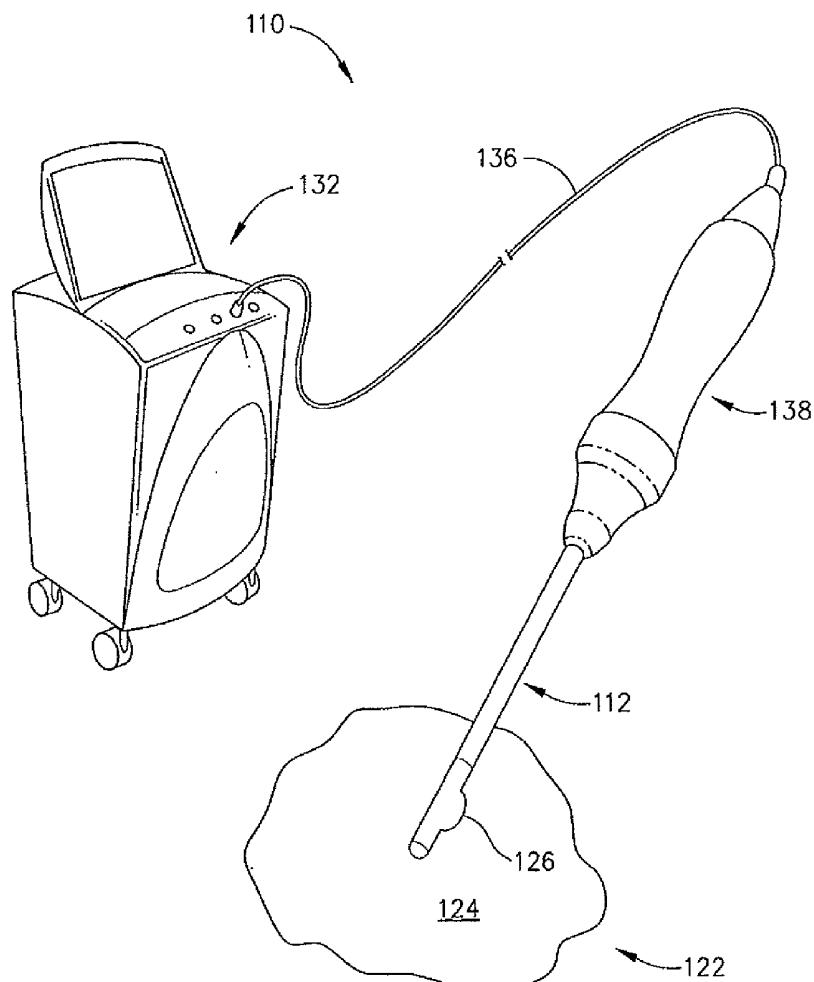

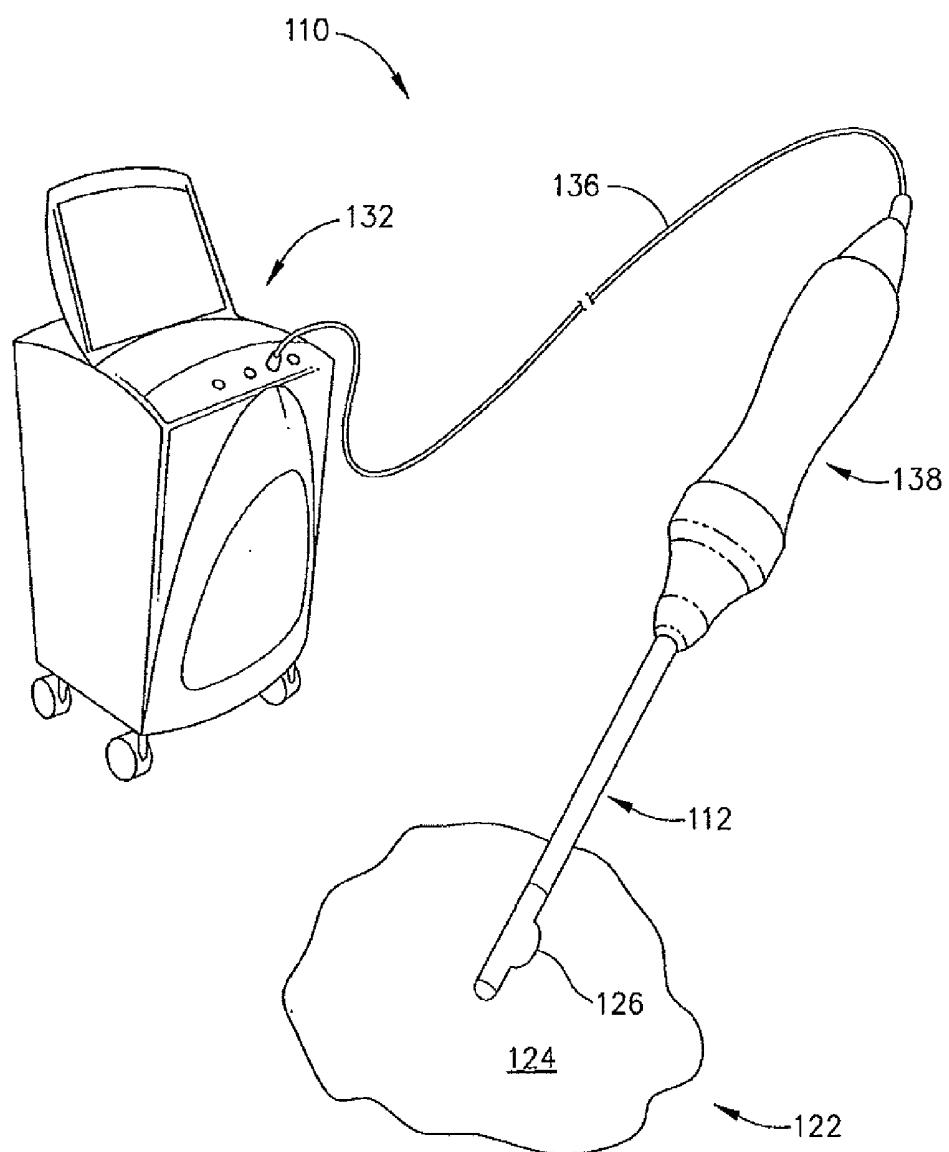


FIG. 1

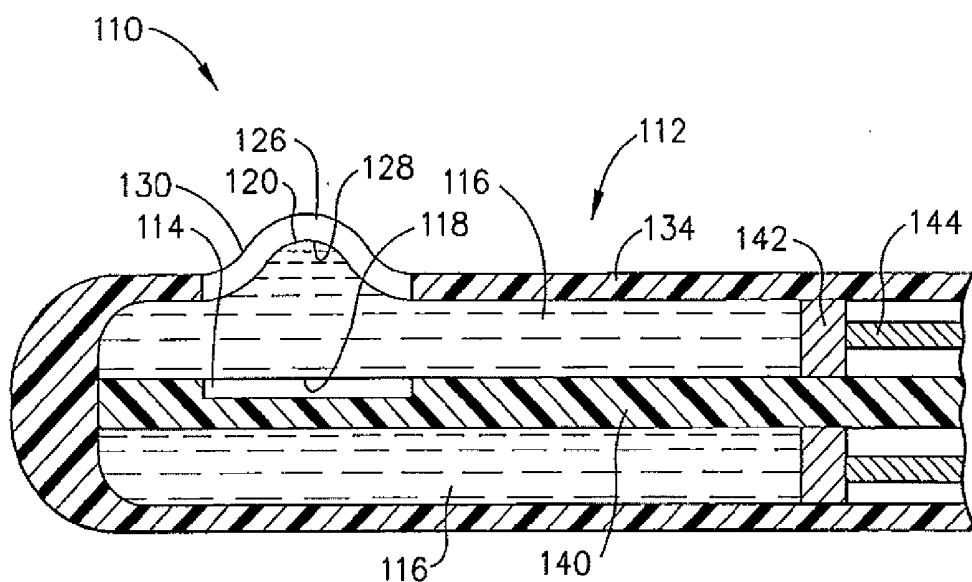


FIG. 2

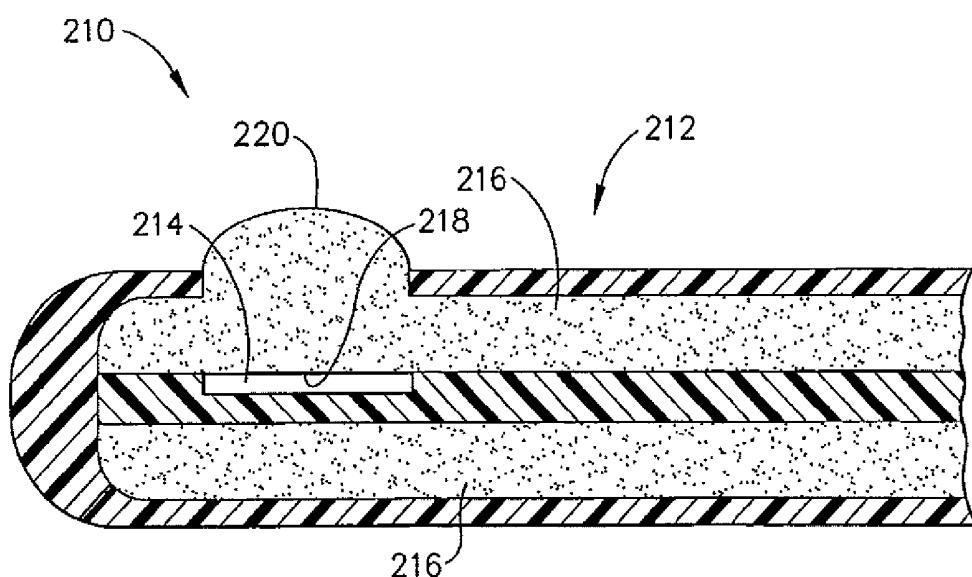


FIG. 3

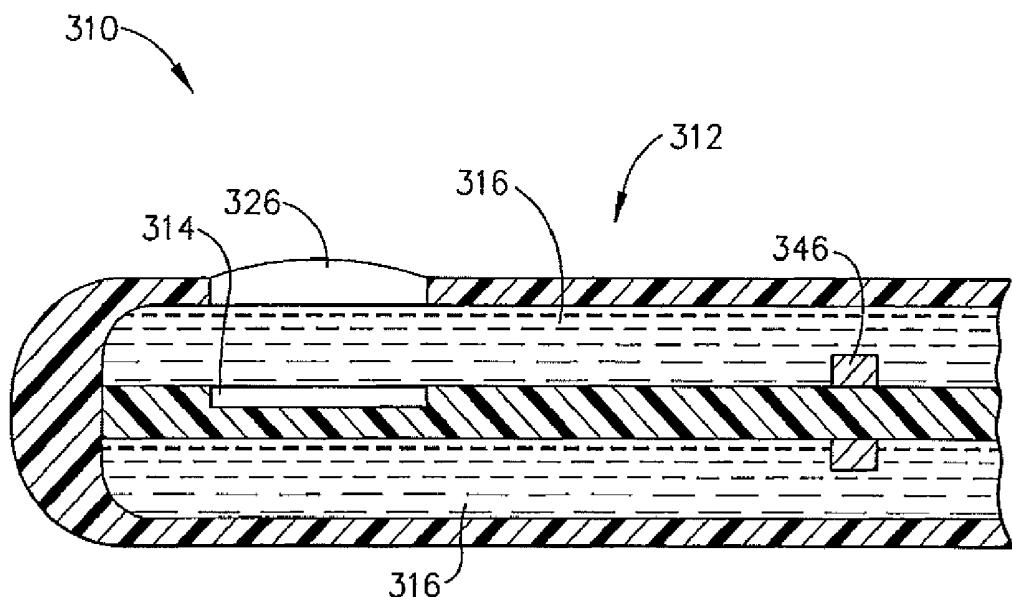


FIG. 4

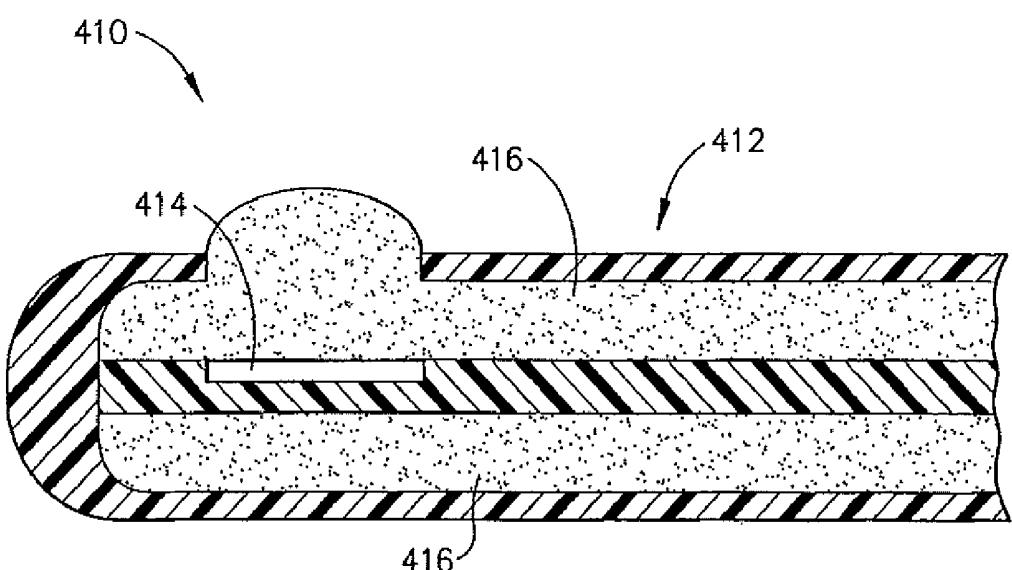


FIG. 5

## MEDICAL SYSTEM HAVING AN ULTRASOUND SOURCE AND AN ACOUSTIC COUPLING MEDIUM

### REFERENCE TO RELATED APPLICATIONS

[0001] The present application is a continuation of U.S. patent Ser. No. 10/848,550 filed May 18, 2004, the contents of which are incorporated herein by reference.

### FIELD OF THE INVENTION

[0002] The present invention relates generally to ultrasound, and more particularly to an ultrasound medical system having an ultrasound source and an acoustic coupling medium.

### BACKGROUND OF THE INVENTION

[0003] Known ultrasound medical methods include using ultrasound imaging (at low power) of patients to identify patient tissue for medical treatment and include using ultrasound (at high power), from the same or a different ultrasound transducer, to ablate identified patient tissue by heating the tissue.

[0004] Known ultrasound medical systems and methods include deploying an end effector having an ultrasound transducer outside the body to break up kidney stones inside the body, endoscopically inserting an end effector having an ultrasound transducer in the rectum to medically destroy prostate cancer, laparoscopically inserting an end effector having an ultrasound transducer in the abdominal cavity to medically destroy a cancerous liver tumor, intravenously inserting a catheter end effector having an ultrasound transducer into a vein in the arm and moving the catheter to the heart to medically destroy diseased heart tissue, and interstitially inserting a needle end effector having an ultrasound transducer needle into the tongue to medically destroy tissue to reduce tongue volume to reduce snoring.

[0005] Conventional ultrasound medical systems include a system having an end effector including a medical ultrasound transducer, a sheath, and a water acoustic coupling medium. The end effector is inserted into a patient, and a balloon portion (which acts as an acoustic window) of the sheath is expanded by increasing water pressure until the balloon portion contacts patient tissue. Then, the medical ultrasound transducer emits medical ultrasound through the balloon portion via the water to image and/or treat the patient tissue.

[0006] Still, scientists and engineers continue to seek improved ultrasound medical systems.

### SUMMARY OF THE INVENTION

[0007] A first expression of an embodiment of the invention is an ultrasound medical system having an end effector including a medical ultrasound transducer and an acoustic coupling medium. The acoustic coupling medium has a transducer-proximal surface and a transducer-distal surface. The medical ultrasound transducer is positioned to emit medical ultrasound through the acoustic coupling medium from the transducer-proximal surface to the transducer-distal surface. The end effector is adapted to change at least one property of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient.

[0008] A second expression of an embodiment of the invention is an ultrasound medical system having a controller and an end effector. The end effector includes a medical ultrasound transducer and an acoustic coupling medium. The acoustic coupling medium has a transducer-proximal surface and a transducer-distal surface. The medical ultrasound transducer is positioned to emit medical ultrasound having a focus and a beam angle through the acoustic coupling medium from the transducer-proximal surface to the transducer-distal surface. The end effector is adapted to change at least one property of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient. The controller controls the end effector to change the property to change the focus and/or the beam angle.

[0009] A third expression of an embodiment of the invention is an ultrasound medical system having a controller and an end effector. The end effector includes a medical ultrasound transducer, an acoustic coupling medium, and a sheath. The sheath includes an expandable acoustic window, wherein the acoustic coupling medium is placed in direct contact with the medical ultrasound transducer and the acoustic window. The medical ultrasound transducer is positioned to emit medical ultrasound through the acoustic window via the acoustic coupling medium. The controller controls the end effector to change the shape of the acoustic window, by changing the pressure exerted by the acoustic coupling medium against the acoustic window, during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient.

[0010] Several benefits and advantages are obtained from one or more of the expressions of an embodiment of the ultrasound medical system of the invention. The acoustic coupling medium also acts as an acoustic lens, wherein the end effector is adapted to change at least one property (such as the shape and/or the temperature) of the acoustic coupling medium which will change the focus and/or the beam angle of emitted ultrasound, with such changes occurring during emission, and/or between emissions, of ultrasound while performing a medical procedure on a patient.

[0011] The present invention has, without limitation, application in conventional endoscopic, laparoscopic, and open surgical instrumentation as well as application in robotic-assisted surgery.

### BRIEF DESCRIPTION OF THE FIGURES

[0012] FIG. 1 is a perspective view of a first embodiment of an ultrasound medical system of the invention including a controller and an end effector, wherein the end effector is seen inserted into a patient (only a portion of whom is shown) and has an acoustic window, and wherein the end effector is adapted to change the shape of the acoustic window during a medical procedure by increasing the pressure of an acoustic coupling medium located inside the end effector;

[0013] FIG. 2 is a schematic cross-sectional view of the end effector of the ultrasound medical system of FIG. 1, wherein the adaptation of the end effector is shown and includes a movable piston which exerts pressure on the acoustic coupling medium;

[0014] FIG. 3 is a schematic cross-sectional view of an end effector of a second embodiment of an ultrasound medical system of the invention, wherein the end effector has an acoustic coupling medium, and wherein the end effector is

adapted to change the shape of the medium-patient interface during a medical procedure, such adaptation being omitted for clarity;

[0015] FIG. 4 is a schematic cross-sectional view of an end effector of a third embodiment of an ultrasound medical system of the invention, wherein the end effector has an acoustic window and has an acoustic coupling medium located inside the end effector, wherein the end effector is adapted to change the temperature of the acoustic coupling medium during a medical procedure, and wherein the adaptation of the end effector includes a heater; and

[0016] FIG. 5 is a schematic cross-sectional view of an end effector of a fourth embodiment of an ultrasound medical system of the invention, wherein the end effector has an acoustic coupling medium and is adapted to change the temperature of the acoustic coupling medium during a medical procedure, such adaptation being omitted for clarity.

#### DETAILED DESCRIPTION OF THE INVENTION

[0017] Before explaining the present invention in detail, it should be noted that the invention is not limited in its application or use to the details of construction and arrangement of parts illustrated in the accompanying drawings and description. The illustrative embodiments of the invention may be implemented or incorporated in other embodiments, variations and modifications, and may be practiced or carried out in various ways. Furthermore, unless otherwise indicated, the terms and expressions employed herein have been chosen for the purpose of describing the illustrative embodiments of the present invention for the convenience of the reader and are not for the purpose of limiting the invention.

[0018] It is understood that any one or more of the following-described embodiments, examples, etc. can be combined with any one or more of the other following-described embodiments, examples, etc.

[0019] Referring now to the drawings, FIGS. 1-2 illustrate an embodiment of the present invention. A first expression of the embodiment of FIGS. 1-2 is an ultrasound medical system 110 comprising an end effector 112 including a medical ultrasound transducer 114 and an acoustic coupling medium 116. The acoustic coupling medium 116 has a transducer-proximal surface 118 and a transducer-distal surface 120. The medical ultrasound transducer 114 is disposed to emit medical ultrasound through the acoustic coupling medium 116 from the transducer-proximal surface 118 to the transducer-distal surface 120. The end effector 112 is adapted to change at least one property of the acoustic coupling medium 116 during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer 114 during a medical procedure on a patient 122. The terminology "ultrasound medical system" includes an ultrasound medical imaging system, an ultrasound medical treatment system, and an ultrasound medical imaging and ultrasound medical treatment system. The terminology "medical procedure" includes an imaging procedure, a treatment procedure, and an imaging and treatment procedure.

[0020] In an enablement of the first expression of the embodiment of FIGS. 1-2, the at-least-one property includes shape, and the end effector 112 is adapted to change the shape (such as the curvature) of the transducer-distal surface 120 during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer 114 during the medical procedure.

[0021] In one variation of this enablement, as shown in the embodiment of FIG. 3, the transducer-distal surface 220 of the acoustic coupling medium 216 is disposable in direct contact with patient tissue. In one modification, the end effector 212 of the ultrasound medical system 210 changes the pressure exerted by the acoustic coupling medium 216 against the patient tissue when the transducer-distal surface 220 of the acoustic coupling medium 216 is disposed in direct contact with patient tissue during the medical procedure. In one construction, the medical ultrasound transducer 214 is disposed in direct contact with the transducer-proximal surface 218 of the acoustic coupling medium 216. In one application, ultrasound imaging from the medical ultrasound transducer 214 or another ultrasound transducer is used to determine the shape of the interface between the transducer-distal surface 220 of the acoustic coupling medium 216 and the patient tissue. It is noted that the interface acts as an acoustic lens surface, and that changing the shape of the interface during the medical procedure can be used to change the focus and/or the beam angle of the ultrasound emitted from the medical ultrasound transducer 214 during the medical procedure when such ultrasound non-perpendicularly passes through the interface. In one option, ultrasound strain imaging of patient tissue is performed by the ultrasound medical system 210.

[0022] In a different variation of this enablement, as shown in the embodiment of FIGS. 1-2, the end effector 112 also includes an expandable acoustic window 126 having an interior surface 128 in direct contact with the transducer-distal surface 120 of the acoustic coupling medium 116 and having an exterior surface 130 disposable in direct contact with patient tissue 124. In one modification, the end effector 112 changes the pressure exerted by the acoustic coupling medium 116 against the acoustic window 126 when the exterior surface 130 of the acoustic window 126 is disposed in direct contact with patient tissue 124 during the medical procedure. In one construction, the medical ultrasound transducer 114 is disposed in direct contact with the transducer-proximal surface 118 of the acoustic coupling medium 116. In one application, ultrasound imaging from the medical ultrasound transducer 114 or another ultrasound transducer is used to determine the shape of the interface between the transducer-distal surface 120 of the acoustic coupling medium 116 and the interior surface 128 of the acoustic window 126 and the shape of the interface between the exterior surface 130 of the acoustic window 126 and the patient tissue 124. In one variation, the acoustic window 126 is a fully-circumferential acoustic window and in another variation it is not. In one option, ultrasound strain imaging of patient tissue 124 is performed by the ultrasound medical system.

[0023] It is noted that the interfaces act as acoustic lens surfaces, and that changing the shape of the interfaces during the medical procedure can be used to change the focus and/or the beam angle of the ultrasound emitted from the medical ultrasound transducer 114 during the medical procedure when such ultrasound non-perpendicularly passes through the interfaces. In one application, the acoustic coupling medium 116 is circulating water, wherein changing the flow rate of the circulating water changes the pressure exerted by the acoustic coupling medium 116 against the acoustic window 126. It is also noted that a change in shape (such as a change in curvature) of the acoustic window 126 typically is accompanied by a change in thickness of the acoustic window

**126** and a change in the distance between the medical ultrasound transducer **114** and the acoustic window **126** which can also effect focus and/or beam angle as is understood by those skilled in the art. In one implementation, the acoustic window **126** is provided with a transducer-distal surface **120** which is rippled (not shown) for use in beam angle steering as is within the level of skill of the artisan.

**[0024]** In the same or a different enablement, as shown in the embodiment of FIG. 4, the at-least-one property includes temperature, and the end effector **312** of the ultrasound medical system **310** is adapted to change the temperature of the acoustic coupling medium **316** during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer **314** during the medical procedure. Changing the temperature of the acoustic coupling medium **316** changes the speed of sound of the emitted ultrasound in the acoustic coupling medium **316** which can be used by those skilled in the art to change the focus and/or the beam angle of the emitted ultrasound when non-perpendicularly passing through a transmission medium interface. It is noted that the embodiment of FIG. 4 includes a rigid or expandable acoustic window **326**, and that the embodiment of the ultrasound medical system **410** of FIG. 5 is identical to that of FIG. 4 except that the end effector **412** of FIG. 5 lacks an acoustic window.

**[0025]** In one example of any one or more or all of the embodiments of FIGS. 1-5, the medical ultrasound transducer **114**, **214**, **314** and/or **414** is chosen from the group consisting of a medical-imaging-only ultrasound transducer, a medical-treatment-only ultrasound transducer, and a medical-imaging-and-treatment ultrasound transducer. In one variation, the medical ultrasound transducer has a single transducer element having a planar or a curved ultrasound-emitting surface. In another variation, the medical ultrasound transducer has an array of transducer elements whose planar or curved ultrasound-emitting surfaces are together disposed to define a curved array surface or whose planar ultrasound-emitting surfaces are together disposed to define a planar array surface. In one modification, the transducer element array is also electronically focused and/or steered as is within the routine capabilities of those skilled in the art. In one extension, the end effector has one or more additional medical ultrasound transducers.

**[0026]** In the same or a different example, the acoustic coupling medium **116**, **216**, **316** and/or **416** is chosen from the group consisting of a liquid, a gel, and a colloid. In one variation, the acoustic coupling medium is a circulating acoustic coupling medium and in a different variation it is not circulating. Examples of liquids include, without limitation, water, a saline solution, glycerol, castor oil, and mineral oil. Other examples of liquids and examples of gels and colloids and other acoustic coupling media are left to the artisan.

**[0027]** In one implementation any one or more or all of the embodiments of FIGS. 1-5, the end effector **112**, **212**, **312** and/or **412** is disposable against an outside surface of the patient. In another implementation, the end effector is insertable into the patient.

**[0028]** A second expression of the embodiment of FIGS. 1-2 is an ultrasound medical system **110** comprising a controller **132** and an end effector **112**. The end effector **112** includes a medical ultrasound transducer **114** and an acoustic coupling medium **116**. The acoustic coupling medium **116** has a transducer-proximal surface **118** and a transducer-distal surface **120**. The medical ultrasound transducer **114** is dis-

posed to emit medical ultrasound through the acoustic coupling medium **116** from the transducer-proximal surface **118** to the transducer-distal surface **120**. The end effector **112** is adapted to change at least one property of the acoustic coupling medium **116** during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer **114** during a medical procedure on a patient **122**. The controller **132** controls the end effector **112** to change the property to change ultrasound focus and/or ultrasound beam angle. In one extension of the embodiments of FIGS. 3-5, and in any one or more or all of the enablements, examples, etc. thereof, the ultrasound medical systems of FIGS. 3-5 also include the controller of the second expression of the embodiment of FIGS. 1-2.

**[0029]** A third expression of the embodiment of FIGS. 1-2 is an ultrasound medical system **110** comprising a controller **132** and an end effector **112**. The end effector **112** includes a medical ultrasound transducer **114**, an acoustic coupling medium **116**, and a rigid or flexible sheath **134**. The sheath **134** includes an expandable acoustic window **126**. The acoustic coupling medium **116** is disposed in direct contact with the medical ultrasound transducer **114** and the acoustic window **126**. The medical ultrasound transducer **114** is disposed to emit medical ultrasound through the acoustic window **126** via the acoustic coupling medium **116**. The controller **132** controls the end effector **112** to change the shape of the acoustic window **126**, by changing (directly or indirectly) the pressure exerted by the acoustic coupling medium **116** against the acoustic window **126**, during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer **114** during a medical procedure on a patient **122**.

**[0030]** In one example of the third expression of the embodiment of FIGS. 1-2, a piston is used to directly change the pressure of an essentially static acoustic coupling medium. In another example, a valve is used to change the flow rate (and hence is used to indirectly change the pressure) of a flowing acoustic coupling medium. In one employment of the third expression of the embodiment of FIGS. 1-2, the controller **132** controls the end effector **112** to change the thickness of the acoustic window **126**, by changing the pressure exerted by the acoustic coupling medium **116** against the acoustic window **126**, during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer **114** during a medical procedure on a patient **122**.

**[0031]** In one arrangement of the embodiment of FIGS. 1-2, the ultrasound medical system **110** also includes a cable **136**, a handpiece **138**, and a rigid or flexible shaft **140**. In this arrangement, the cable **136** operatively connects the controller **132** to the handpiece **138**, the handpiece **138** is operatively connected to the end effector **112**, and the shaft **140** supports the medical ultrasound transducer **114** and is operatively connected to the handpiece **138**. The shaft **140** can be rotatable or non-rotatable with respect to the handpiece **138**. Other arrangements are left to the artisan.

**[0032]** In one construction of the third expression of the embodiment of FIGS. 1-2, a thinner part of the sheath acts as the acoustic window. In another construction, the acoustic window is made from a different material or materials than the material or materials of the non-acoustic-window portion of the sheath. In an additional construction, the entire sheath acts as the acoustic window. Other constructions are left to the artisan.

**[0033]** Examples of acoustically-transmissive materials for acoustic windows include, without limitation, PET [polyeth-

ylene terephthalate] (such as 0.001-inch-thick PET for a fully-circumferential acoustic window), Nylon 6, 11 or 12, TPX [methylpentene copolymer] and fluropolymers such as PTFE [polytetrafluoroethylene], FEP [fluorinated ethylene propylene], PFA [perfluoroalkoxy], PVDA [polyvinylidene acetate], ETFE [ethylene tetrofluoroethylene], polyurethane and polyethylene (high and low density). Shaft and sheath materials, for flexible shafts and sheaths, include, without limitation, Nitinol, polyimide, reinforced polyimide, Nylon, Pebax, silicone, reinforced silicone, polyurethane, polyethylene, fluropolymers and coiled metals (e.g., coiled stainless steel).

[0034] In one deployment of the ultrasound medical system 110 of FIGS. 1-2, the end effector 112 is adapted to change the shape of the transducer-distal surface 120 of the acoustic coupling medium 116 by having the end effector 112 include an annular piston 142, movable by an attached annular piston rod 144. The movable piston 142 is used to change the pressure of a non-circulating acoustic coupling medium 116 to change the curvature of the transducer-distal surface 120 of the acoustic coupling medium 115 (which changes the curvature of the acoustic window 126). In a different deployment, not shown, the end effector 112 is adapted by having the end effector 112 include a channel for the acoustic coupling medium 116 extending from the area of the acoustic window 126 to an orifice connectable to a variable-pressure-exerting device.

[0035] In one deployment of the ultrasound medical system 310 of FIG. 4, the end effector 312 is adapted by having the end effector 312 include a heater 346 which is used to change the temperature of the acoustic coupling medium 316. In a different deployment, not shown, the end effector 312 is adapted by having the end effector 312 include a channel for the acoustic coupling medium 316 extending from the area of the acoustic window 326 to an orifice connectable to a heating device.

[0036] In a further deployment of the ultrasound medical systems of FIGS. 1-2 and FIG. 5, a tube (not shown) surrounds the shaft, is radially spaced apart from the shaft and the sheath, and longitudinally extends proximate the acoustic window with, for example, circulating water as the acoustic coupling medium which enters the ultrasound transducer-acoustic window area from the channel between the shaft and the tube and which exits the ultrasound transducer-acoustic window area from the channel between the tube and the sheath. In one variation, a pump (not shown) varies the flow rate of the water. In such adaptation of the end effector, an increasing flow rate increases the pressure of the circulating acoustic coupling medium which changes the shape of the transducer-distal surface of the acoustic coupling medium (in both the FIGS. 1-2 and FIG. 5 ultrasound medical systems) and hence the shape of the acoustic window (in the FIGS. 1-2 ultrasound medical system). Other deployments are left to the artisan.

[0037] Several benefits and advantages are obtained from one or more of the expressions of an embodiment of the ultrasound medical system of the invention. The acoustic coupling medium also acts as an acoustic lens, wherein the end effector is adapted to change at least one property (such as the shape and/or the temperature) of the acoustic coupling medium which will change the focus and/or the beam angle of emitted ultrasound, with such changes occurring during emission, and/or between emissions, of ultrasound while performing a medical procedure on a patient.

[0038] While the present invention has been illustrated by a description of several embodiments, it is not the intention of the applicants to restrict or limit the spirit and scope of the appended claims to such detail. Numerous other variations, changes, and substitutions will occur to those skilled in the art without departing from the scope of the invention. For instance, the ultrasound medical system of the invention has application in robotic assisted surgery taking into account the obvious modifications of such systems, components and methods to be compatible with such a robotic system. It will be understood that the foregoing description is provided by way of example, and that other modifications may occur to those skilled in the art without departing from the scope and spirit of the appended Claims.

What is claimed is:

1. An ultrasound medical system comprising an end effector including a medical ultrasound transducer and an acoustic coupling medium, wherein the acoustic coupling medium has a transducer-proximal surface and a transducer-distal surface, wherein the medical ultrasound transducer is disposed to emit medical ultrasound through the acoustic coupling medium from the transducer-proximal surface to the transducer-distal surface, and wherein the end effector is adapted to change at least one property of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient.

2. The ultrasound medical system of claim 1, wherein the at-least-one property includes shape, and wherein the end effector is adapted to change the shape of the transducer-distal surface during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during the medical procedure.

3. The ultrasound medical system of claim 2, wherein the transducer-distal surface of the acoustic coupling medium is disposable in direct contact with patient tissue.

4. The ultrasound medical system of claim 3, wherein the end effector changes the pressure exerted by the acoustic coupling medium against the patient tissue when the transducer-distal surface of the acoustic coupling medium is disposed in direct contact with patient tissue during the medical procedure.

5. The ultrasound medical system of claim 2, wherein the end effector also includes an expandable acoustic window having an interior surface in direct contact with the transducer-distal surface of the acoustic coupling medium and having an exterior surface disposable in direct contact with patient tissue.

6. The ultrasound medical system of claim 5, wherein the end effector changes the pressure exerted by the acoustic coupling medium against the acoustic window when the exterior surface of the acoustic window is disposed in direct contact with patient tissue during the medical procedure.

7. The ultrasound medical system of claim 1, wherein the at-least-one property includes temperature, and wherein the end effector is adapted to change the temperature of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during the medical procedure.

8. The ultrasound medical system of claim 1, wherein the medical ultrasound transducer is chosen from the group consisting of a medical-imaging-only ultrasound transducer, a medical-treatment-only ultrasound transducer, and a medical-imaging-and-treatment ultrasound transducer.

**9.** The ultrasound medical system of claim **1**, wherein the acoustic coupling medium is chosen from the group consisting of a liquid, a gel, and a colloid.

**10.** The ultrasound medical system of claim **1**, wherein the end effector is disposable against an outside surface of the patient.

**11.** The ultrasound medical system of claim **1**, wherein the end effector is insertable into the patient.

**12.** An ultrasound medical system comprising a controller and an end effector, wherein the end effector includes a medical ultrasound transducer and an acoustic coupling medium, wherein the acoustic coupling medium has a transducer-proximal surface and a transducer-distal surface, wherein the medical ultrasound transducer is disposed to emit medical ultrasound through the acoustic coupling medium from the transducer-proximal surface to the transducer-distal surface, wherein the end effector is adapted to change at least one property of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient, and wherein the controller controls the end effector to change the property to change ultrasound focus and/or ultrasound beam angle.

**13.** The ultrasound medical system of claim **12**, wherein the at-least-one property includes shape, and wherein the end effector is adapted to change the shape of the transducer-distal surface during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during the medical procedure.

**14.** The ultrasound medical system of claim **12**, wherein the at-least-one property includes temperature, and wherein the end effector is adapted to change the temperature of the acoustic coupling medium during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during the medical procedure.

**15.** The ultrasound medical system of claim **12**, wherein the medical ultrasound transducer is chosen from the group consisting of a medical-imaging-only ultrasound transducer, a medical-treatment-only ultrasound transducer, and a medical-imaging-and-treatment ultrasound transducer.

**16.** The ultrasound medical system of claim **12**, wherein the acoustic coupling medium is chosen from the group consisting of a liquid, a gel, and a colloid.

**17.** The ultrasound medical system of claim **12**, wherein the end effector is disposable against an outside surface of the patient.

**18.** The ultrasound medical system of claim **12**, wherein the end effector is insertable into the patient.

**19.** An ultrasound medical system comprising a controller and an end effector, wherein the end effector includes a medical ultrasound transducer, an acoustic coupling medium, and a sheath, wherein the sheath includes an expandable acoustic window, wherein the acoustic coupling medium is disposed in direct contact with the medical ultrasound transducer and the acoustic window, wherein the medical ultrasound transducer is disposed to emit medical ultrasound through the acoustic window via the acoustic coupling medium, and wherein the controller controls the end effector to change the shape of the acoustic window, by changing the pressure exerted by the acoustic coupling medium against the acoustic window, during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient.

**20.** The ultrasound medical system of claim **19**, wherein the controller controls the end effector to change the thickness of the acoustic window, by changing the pressure exerted by the acoustic coupling medium against the acoustic window, during emission, and/or between emissions, of medical ultrasound from the medical ultrasound transducer during a medical procedure on a patient.

\* \* \* \* \*

|                |   |         |            |
|----------------|---|---------|------------|
| 专利名称(译)        | 具有超声源和声耦合介质的医疗系统  |         |            |
| 公开(公告)号        | <a href="#">US20100256490A1</a>   | 公开(公告)日 | 2010-10-07 |
| 申请号            | US12/818261   | 申请日     | 2010-06-18 |
| [标]申请(专利权)人(译) | MAKIN因德尔RAJ小号<br>MAST T DOUGLAS<br>斯雷顿MICHAEL ^ h<br>BARTHE PETER摹<br>梅瑟利JEFFREY D<br>FAIDI克瓦<br>RUNK MEGAN中号                                 |         |            |
| 申请(专利权)人(译)    | MAKIN因德尔RAJ小号<br>MAST T DOUGLAS<br>斯雷顿MICHAEL ^ h<br>BARTHE PETER摹<br>梅瑟利JEFFREY D<br>FAIDI克瓦<br>RUNK MEGAN中号                                 |         |            |
| 当前申请(专利权)人(译)  | ETHICON LLC   |         |            |
| [标]发明人         | MAKIN INDER RAJ S<br>MAST T DOUGLAS<br>SLAYTON MICHAEL H<br>BARTHE PETER G<br>MESSERLY JEFFREY D<br>FAIDI WASEEM<br>RUNK MEGAN M              |         |            |
| 发明人            | MAKIN, INDER RAJ S.<br>MAST, T. DOUGLAS<br>SLAYTON, MICHAEL H.<br>BARTHE, PETER G.<br>MESSERLY, JEFFREY D.<br>FAIDI, WASEEM<br>RUNK, MEGAN M. |         |            |
| IPC分类号         | A61N7/00 A61B8/00 A61B17/22 A61H1/00 A61N7/02   |         |            |
| CPC分类号         | A61B2017/2253 A61N7/022 A61B8/12 A61N2007/0052 A61B8/4444 A61B8/546 A61N7/00 A61B8/4272 A61B8/4281  |         |            |
| 外部链接           | <a href="#">Espacenet</a> <a href="#">USPTO</a>   |         |            |

## 摘要(译)

超声医疗系统具有末端执行器，该末端执行器包括医学超声换能器和声耦合介质。声耦合介质具有换能器近侧表面和换能器远侧表面。医学超声换能器定位成通过声耦合介质从换能器近侧表面到换能器远侧表面发射医学超声。末端执行器适于在患者的医疗过程期间在医疗超声换能器的发射期间和/或发射之间改变声学耦合介质的性质(诸如形状和/或温度)。在一个示例中，这种改变用于在医疗过程期间改变发射的超声的焦点和/或光束角。

