



(19) **United States**

(12) **Patent Application Publication**  
**Kim**

(10) **Pub. No.: US 2007/0073148 A1**

(43) **Pub. Date: Mar. 29, 2007**

(54) **ULTRASOUND DIAGNOSTIC SYSTEM AND METHOD FOR ROTATING ULTRASOUND IMAGE**

**Publication Classification**

(51) **Int. Cl.**  
*A61B 8/00* (2006.01)  
(52) **U.S. Cl.** ..... **600/437**

(75) **Inventor: Nam Woong Kim, Seoul (KR)**

Correspondence Address:  
**OBLON, SPIVAK, MCCLELLAND, MAIER & NEUSTADT, P.C.**  
**1940 DUKE STREET**  
**ALEXANDRIA, VA 22314 (US)**

(57) **ABSTRACT**

The present invention relates to an ultrasound diagnostic system and a method for rotating an ultrasound image displayed on a display by using a 3D position sensor and/or a joystick attached to a probe. A method for rotating the ultrasound image comprises the steps of: a) activating the probe and the 3D position sensor and/or the joystick; b) forming and displaying the ultrasound image based on ultrasound echo signals acquired through the probe; c) receiving information for rotating the displayed ultrasound image through the 3D position sensor and/or the joystick; and d) rotating the ultrasound image based on the information.

(73) **Assignee: Medison Co., Ltd., Hongchun-gun (KR)**


(21) **Appl. No.: 11/401,324**

(22) **Filed: Apr. 11, 2006**

(30) **Foreign Application Priority Data**

Sep. 14, 2005 (KR) ..... 10-2005-85562

100

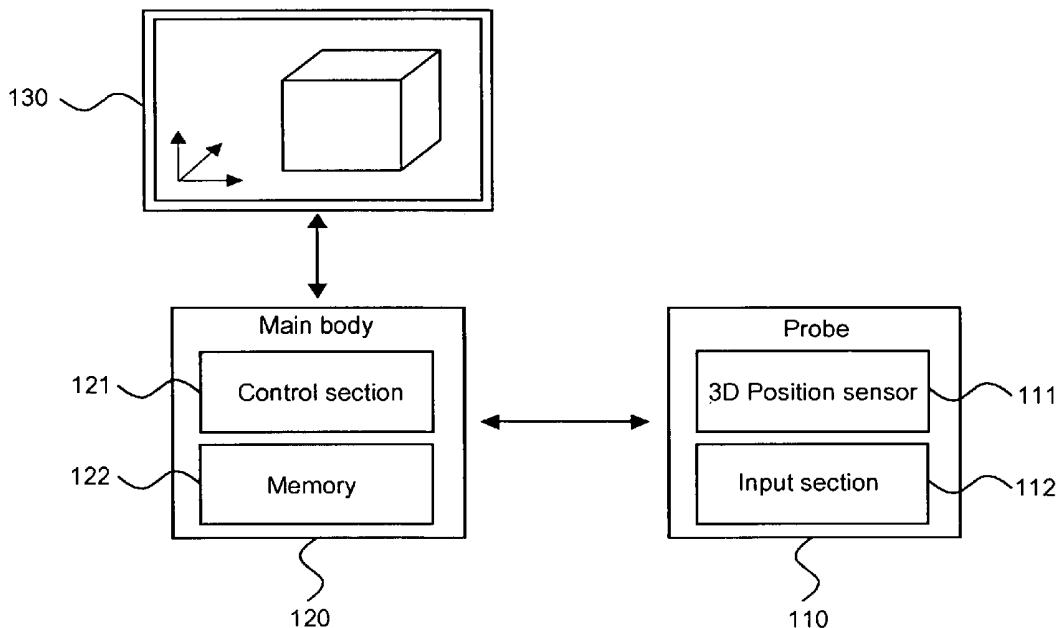

**Fig. 1**

100


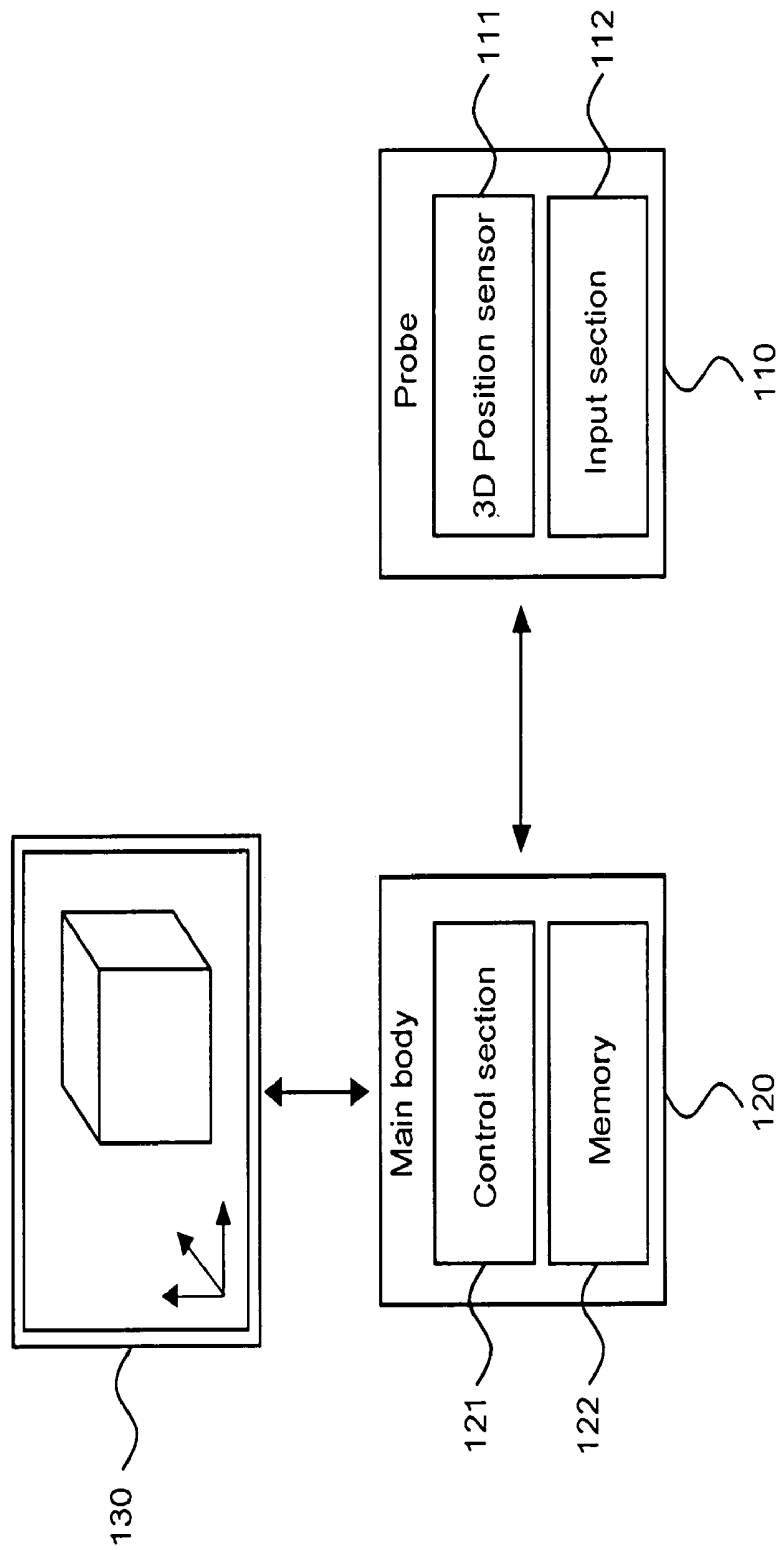


Fig. 2

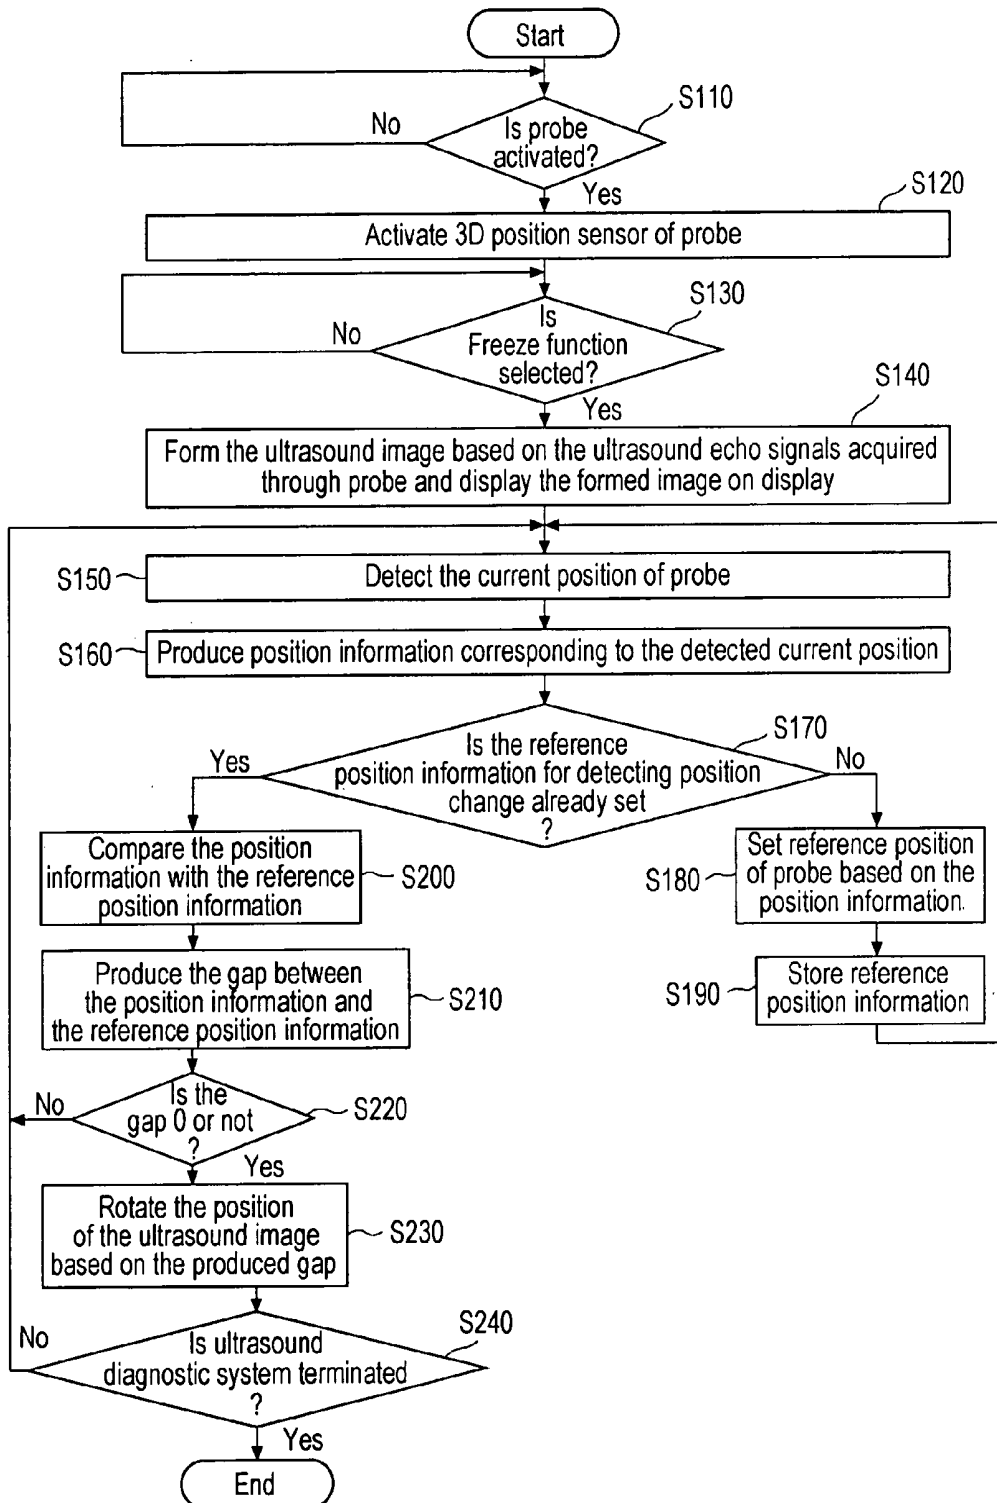

**Fig. 3**

300



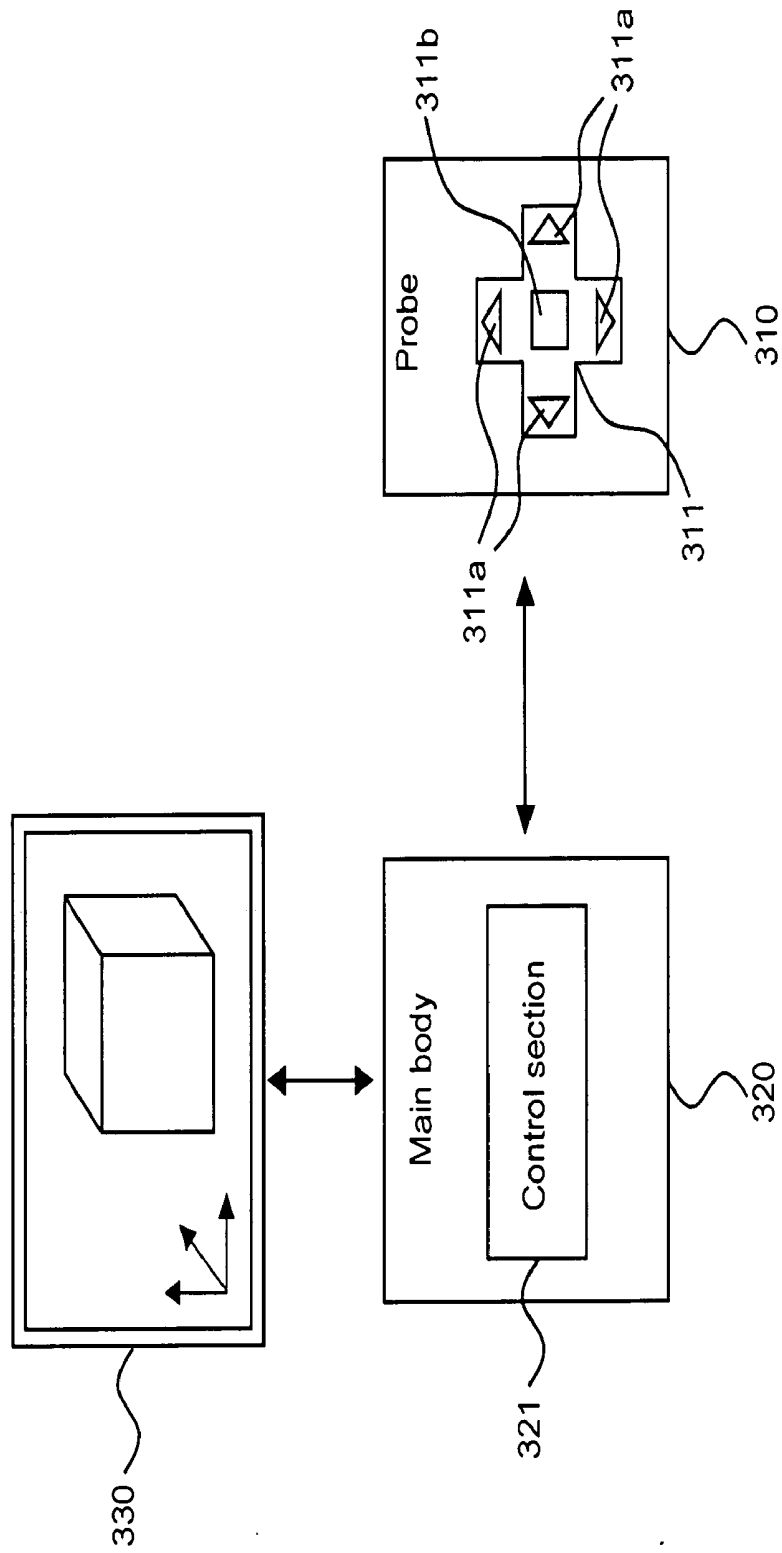


Fig. 4

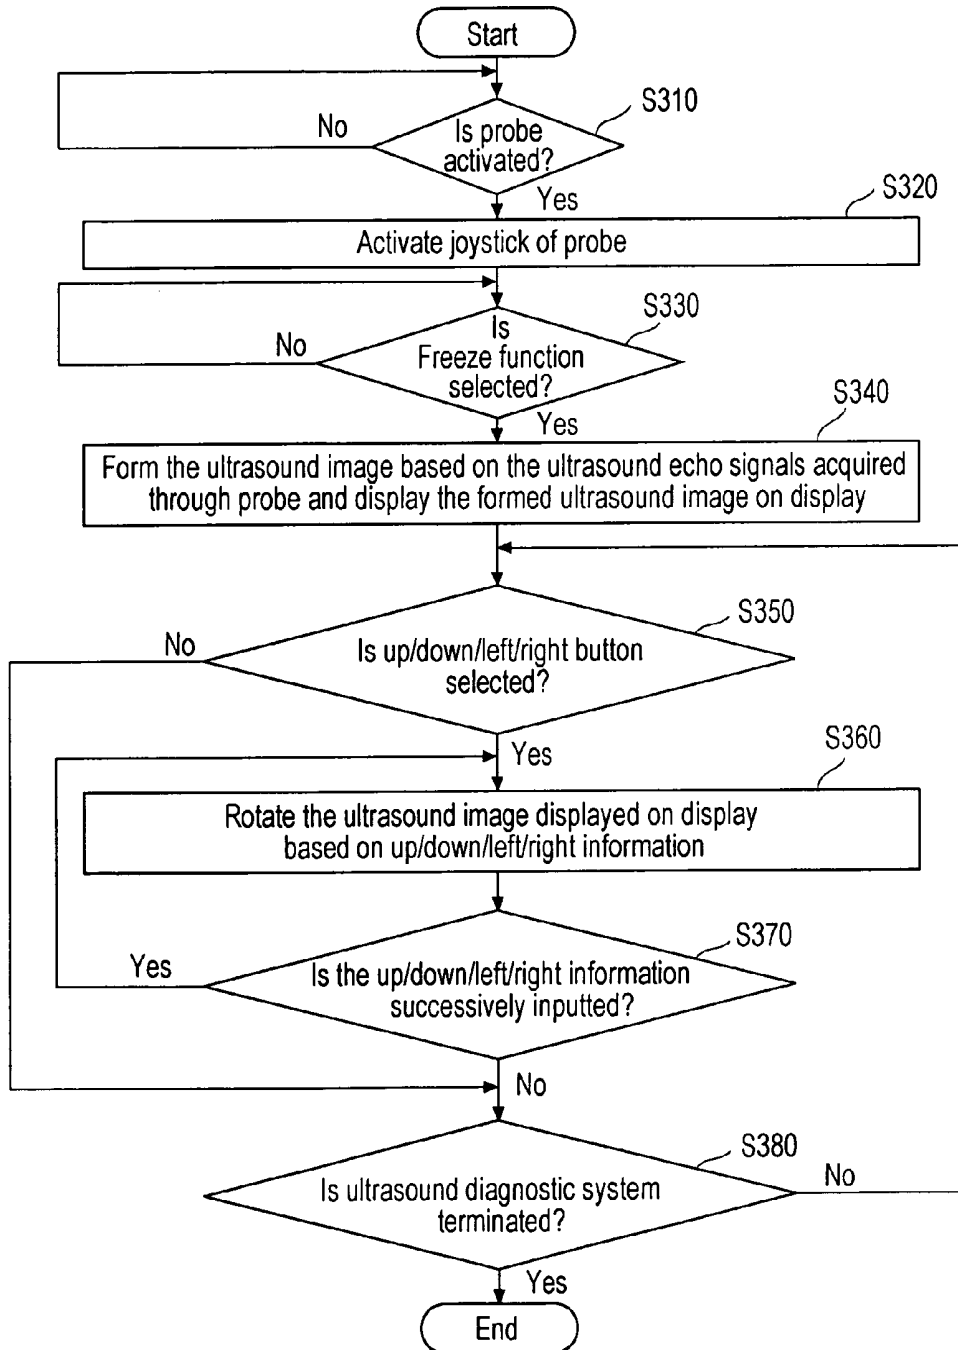

**Fig. 5**

500

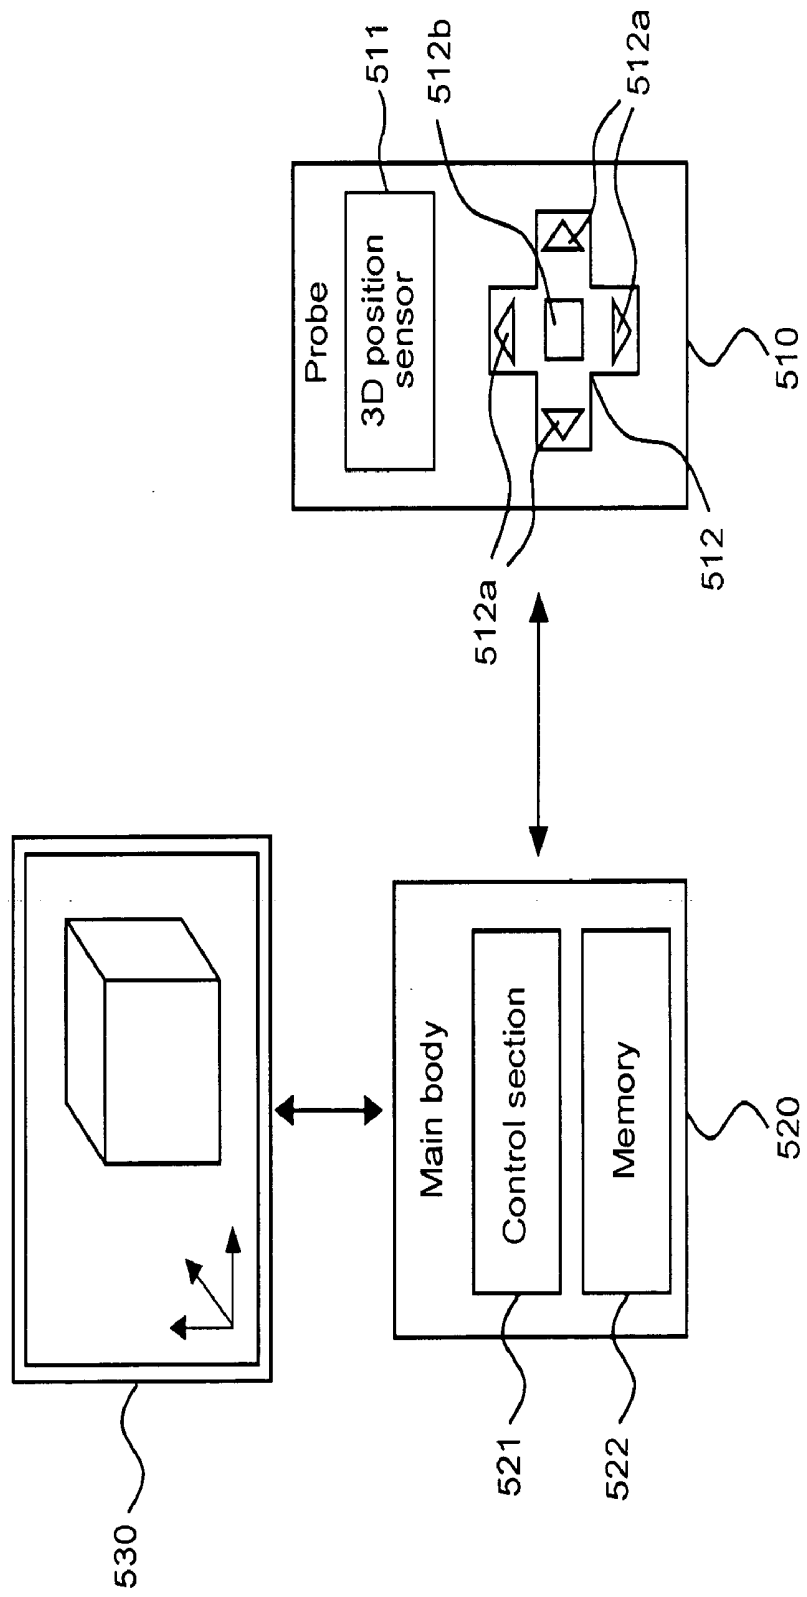

**Fig. 6**



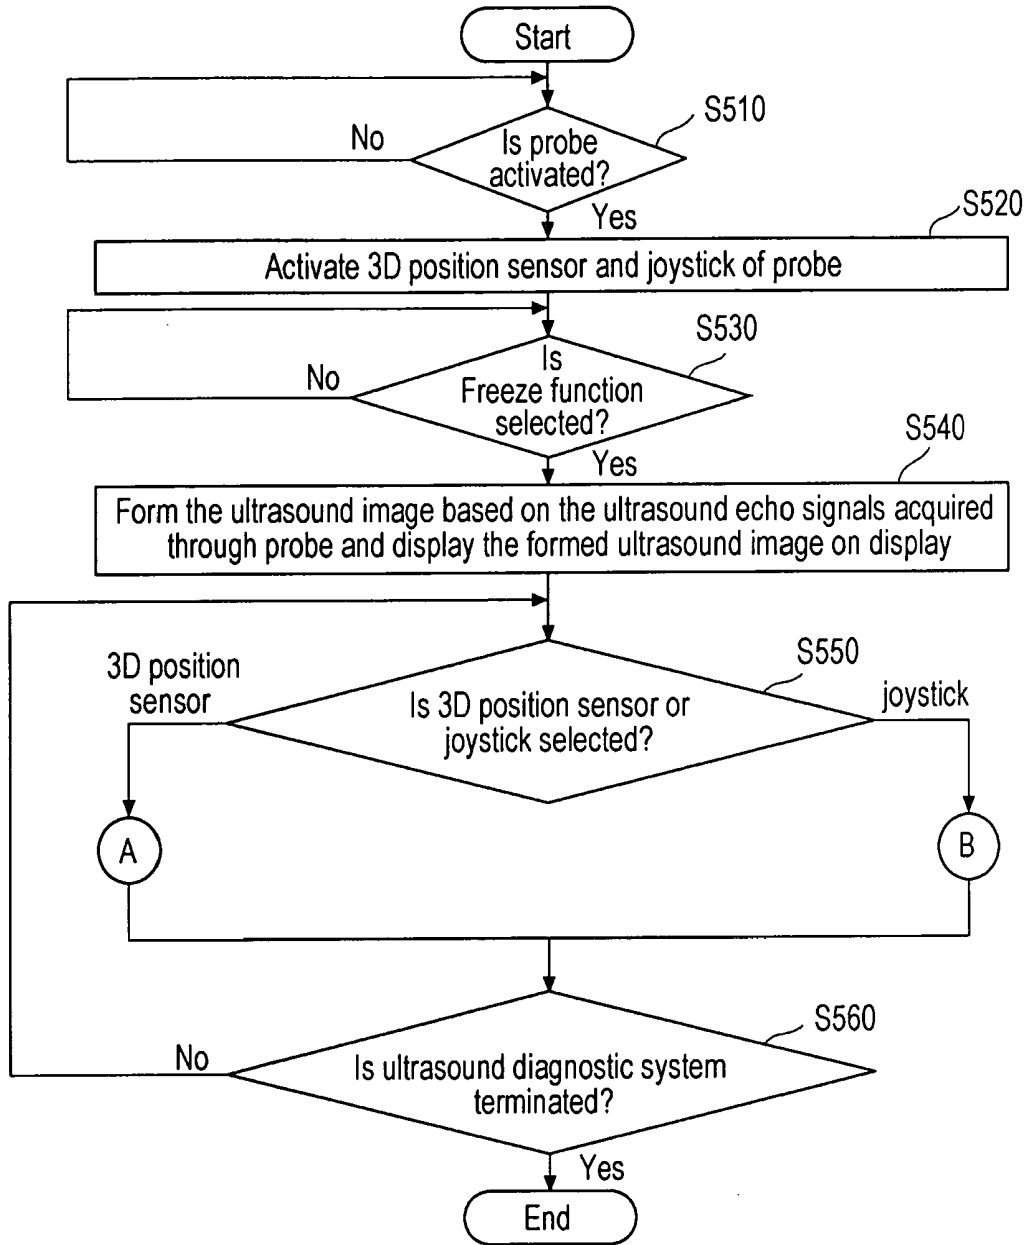


Fig. 7

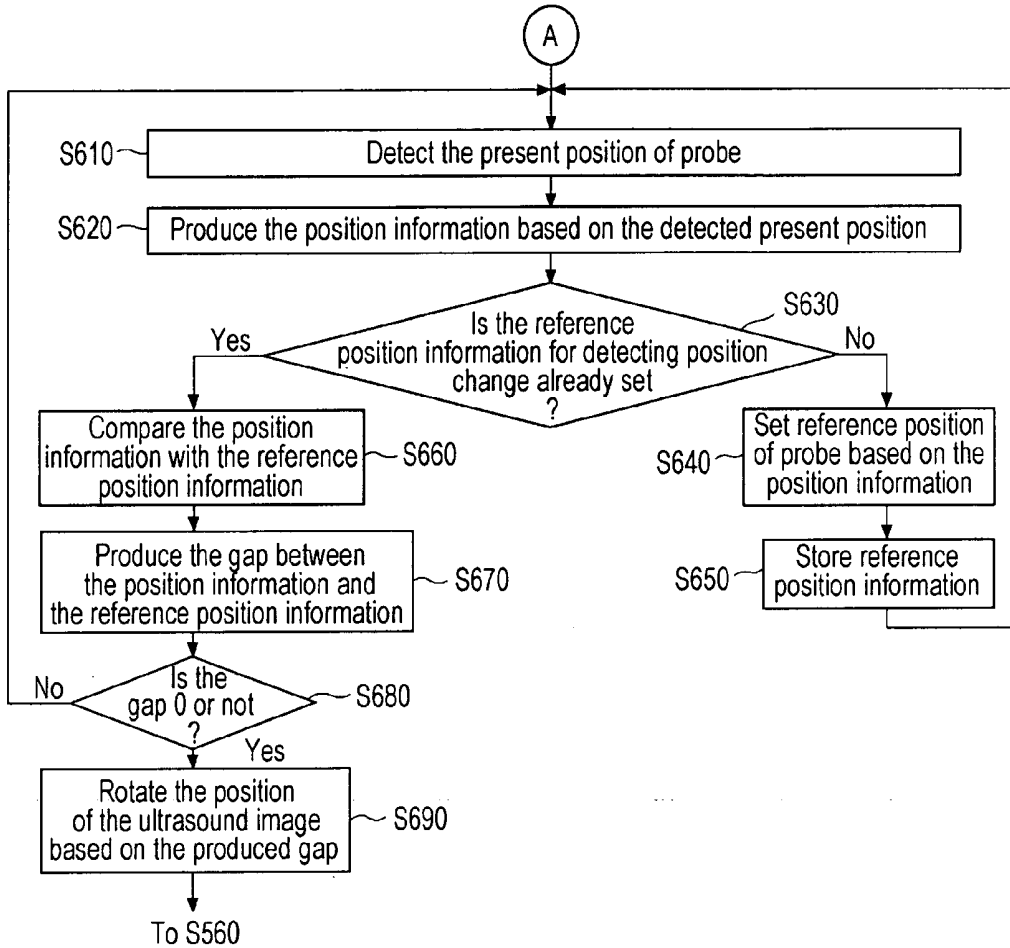

**Fig. 8**

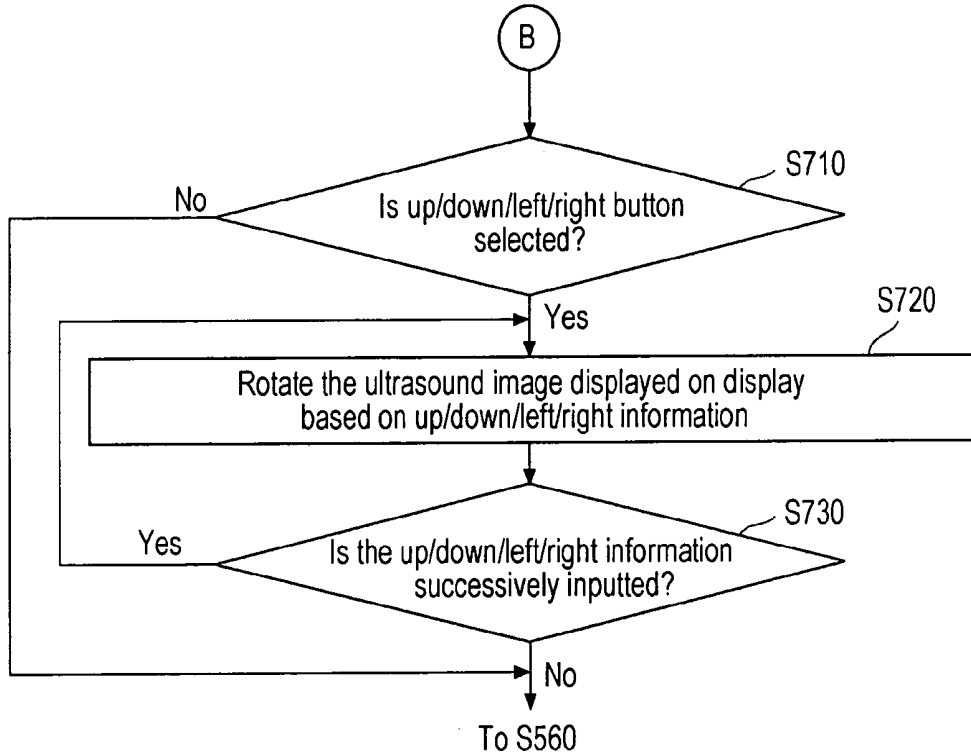

## ULTRASOUND DIAGNOSTIC SYSTEM AND METHOD FOR ROTATING ULTRASOUND IMAGE

### FIELD OF THE INVENTION

[0001] The present invention generally relates to an ultrasound diagnostic system, and more particularly to an ultrasound diagnostic system and a method for rotating an ultrasound image by using a three-dimensional (“3D”) position sensor or a joystick attached to a probe.

### BACKGROUND OF THE INVENTION

[0002] Generally, an ultrasound diagnostic system is used to obtain an image of soft tissue dislocation or blood flow by irradiating ultrasound signals from a surface of the object to a desired portion and using the information acquired from reflected ultrasound signals (ultrasound echo signals). When compared to other image diagnostic devices such as an X-ray diagnostic device, an X-ray Computerized Tomography (“CT”) Scanner, a Magnetic Resonance Image (“MRI”) and a nuclear medicine diagnostic device, the ultrasound diagnostic system is relatively small and inexpensive. Further, the ultrasound diagnostic system can display the ultrasound image in real time and is fairly safe since there is no exposure to X-rays. Thus, the ultrasound diagnostic system is widely used for diagnosing a heart, an abdomen, a urinary organ and obstetrics.

[0003] Particularly, the ultrasound diagnostic system comprises at least one probe, which has a plurality of one-dimensional (“1D”) or two-dimensional (“2D”) transducers and properly adjusts the timing of applying input pulses to the transducers in order to transmit the condensed ultrasound beam along a transmission scan line to a target. Then, the ultrasound echo signals reflected from the target are inputted to the transducers at different timing. Each transducer then outputs the ultrasound echo signals to a beam former.

[0004] As illustrated above, the conventional ultrasound diagnostic system forms an ultrasound image (preferably a 3D ultrasound image) based on the ultrasound echo signals acquired through the probe. It can also display the formed ultrasound image on a display.

[0005] In the conventional ultrasound diagnostic system, however, a user typically handles the probe with one hand while using the other hand to handle the control panel of the ultrasound diagnostic system. After displaying the obtained ultrasound image on a display, the user then handles the track ball and a number of buttons on the control panel in order to rotate the displayed ultrasound image to a certain direction or predetermined angle. Therefore, the conventional ultrasound diagnostic system is disadvantageous since it is difficult to rotate the displayed ultrasound image to the predetermined direction or angle.

[0006] In order to solve the above deficiency, there is provided an ultrasound diagnostic system and a method for rotating the ultrasound image, which is displayed on a display, based on the position information outputted from a 3D position sensor and/or a joystick that are attached to a probe.

### SUMMARY OF THE INVENTION

[0007] The ultrasound diagnostic system of the present invention comprises: a probe; input means attached to the

probe for receiving information for use in rotating an ultrasound image in a predetermined direction; and control means for rotating the ultrasound image based on the information from the input means.

[0008] A method of the present invention for rotating an ultrasound image by using input means attached to a probe for receiving information to rotate an ultrasound image comprises the steps of: a) activating the probe and the input means; b) forming and displaying the ultrasound image based on ultrasound echo signals acquired through the probe; c) receiving information for rotating the displayed ultrasound image through the input means; and d) rotating the ultrasound image based on the information.

[0009] In accordance with the present invention, it is possible for a user to easily rotate the displayed ultrasound image with one hand by using the 3D position sensor and/or the joystick, which are attached to the probe.

### BRIEF DESCRIPTION OF THE DRAWINGS

[0010] The above and other objects and features of the present invention will become apparent from the following description of preferred embodiments given in conjunction with the accompanying drawings, in which:

[0011] FIG. 1 is a block diagram showing an ultrasound diagnostic system according to the first embodiment of the present invention.

[0012] FIG. 2 is a flowchart for describing the operation of an ultrasound diagnostic system according to the first embodiment of the present invention.

[0013] FIG. 3 is a block diagram for describing an ultrasound diagnostic system according to the second embodiment of the present invention.

[0014] FIG. 4 is a flowchart for describing the operation of an ultrasound diagnostic system according to the second embodiment of the present invention.

[0015] FIG. 5 is a block diagram for describing an ultrasound diagnostic system according to the third embodiment of the present invention.

[0016] FIG. 6 is a flowchart for describing the operation of an ultrasound diagnostic system according to the third embodiment of the present invention.

[0017] FIG. 7 is a flowchart for describing the operation of rotating an ultrasound image by using a 3D position sensor according to the third embodiment of the present invention.

[0018] FIG. 8 is a flowchart for describing the operation of rotating an ultrasound image by using a joystick according to the third embodiment of the present invention.

### DETAILED DESCRIPTION OF THE PRESENT INVENTION

[0019] (The First Embodiment)

[0020] FIG. 1 is a block diagram showing an ultrasound diagnostic system, which is constructed in accordance with the first embodiment of the present invention.

[0021] The ultrasound diagnostic system 100, which is shown in FIG. 1, comprises a probe 110, a main body 120 and a display 130. The probe 110 comprises a 3D position

sensor **111** and an input section **112**. The probe **110** also comprises a plurality of 1D, 2D or 3D transducers (not shown), which can send a condensed ultrasound beam along the transmission scan line to a target (not shown) by properly delaying the timing of applying input pulses. Such transducers further receive ultrasound echo signals reflected from the target at different timing of reception.

[0022] The 3D position sensor **111** detects the present position of the probe **110** and generates position information of the probe **110**. As for the 3D position sensor **111**, any device may be used as long as the device can detect the position of the probe **110**. For example, a gyro can be used as the 3D position sensor **111**. The input section **112** receives ultrasound image information and reference position setting information of the probe **110**.

[0023] The main body **120** comprises a control section **121** and a memory **122** for composing an ultrasound image based on the ultrasound echo signals acquired through the probe **110**. It is further configured to display the composed ultrasound image on a display **130** and rotate the ultrasound image on the display **130** according to the position change, that is, the rotation of the probe **110**. The main body **120** also comprises a beam former, an image signal processor, a scan converter and an image processor (not shown).

[0024] The control section **121** controls the overall operation of the ultrasound diagnostic system **100**. Particularly, the control section **121** rotates the ultrasound image displayed on the display **130** based on the position information transmitted from the 3D position sensor **111** of the probe **110**. The memory **122** stores the reference position information for determining the position change of the probe **110**. The reference position information will be described below in detail.

[0025] The operation of the ultrasound diagnostic system, which is in accordance with the first embodiment of the present invention, will be described below in view of FIGS. **1** and **2**. FIG. **2** is a flowchart for describing the operation of the ultrasound diagnostic system, which is in accordance with the first embodiment of the present invention.

[0026] As illustrated in FIG. **2**, if a user activates the probe **110** by operating the ultrasound diagnostic system **100** (step **S110**), the control section **121** activates the 3D position sensor **111** of the probe **110** (step **S120**). If the user then selects the Freeze function for obtaining the ultrasound image through the input section **112** (step **S130**), then the control section **121** forms the ultrasound image based on the ultrasound echo signals acquired through the probe **110** and displays the formed image on the display **130** (step **S140**).

[0027] Subsequently, if the 3D position sensor **111** detects the current position of the probe **110** (step **S150**), then the control section **121** produces the position information corresponding to the detected current position (step **S160**). The control section **121** also checks whether the reference position information for detecting the position change is already set (step **S170**).

[0028] In step **S170**, if it is determined that the reference position of the probe **110** is not set, then the control section **121** sets the reference position of the probe **110** based on the position information transmitted from the 3D position sensor **111** (step **S180**) and stores the information related to the

set reference position (hereinafter referred to as the reference position information) into the memory **122** (step **S190**).

[0029] On the other hand, if it is determined that the reference position is already set (step **S170**), then the control section **121** compares the position information transmitted from the 3D position sensor **111** with the reference position information stored in the memory **122** and produces the gap between the position information and the reference position information (step **S210**). The control section **121** then checks whether the position information is the same as the reference position information, that is, whether the gap is 0 or not (step **S220**). If it is determined that the position information is the same as the reference position information, then the process goes back to step **S150**. Otherwise, the control section **121** changes, that is, the position of the ultrasound image displayed on the display **130** rotates based on the produced gap (step **S230**).

[0030] The control section **121** checks whether the ultrasound diagnostic system **100** is terminated. If it is determined that the ultrasound diagnostic system **100** is terminated, all the processes are terminated. Otherwise, the process goes back to step **S150**.

[0031] (The Second Embodiment)

[0032] FIG. **3** is a block diagram for describing an ultrasound diagnostic system **300**, which is constructed in accordance with the second embodiment of the present invention.

[0033] As shown in FIG. **3**, the ultrasound diagnostic system **300** of the second embodiment comprises a probe **310**, a main body **320** and a display **330**. The probe **310** comprises a joystick **311**. The probe **310** also comprises a plurality of 1D or 2D transducers (not shown), which can send a condensed ultrasound beam along the transmission scan line to a target (not shown) by properly adjusting the timing of applying input pulses to the transducers. Such transducers are also configured to receive the ultrasound echo signals reflected from the target at different timing.

[0034] The joystick **311** is used to rotate the ultrasound image, which is displayed on the display **330**, in a plurality of directions (i.e., up, down, left and right). The joystick **311** comprises a button **311a** for rotating the ultrasound image in up, down, left and right directions. It also comprises a selection button **311b** for acquiring an ultrasound image and adjusting the acquired ultrasound image.

[0035] The main body **320** comprises a control section **321**. The main body **320** also comprises a beam former, an image signal processor, a scan converter and an image processor (not shown).

[0036] The control section **321** controls the overall operation of the ultrasound diagnostic system **300**. Particularly, the control section **321** is configured to perform the following: form an ultrasound image based on the ultrasound echo signals acquired from the probe **310**; display the formed ultrasound image on the display **330**; and change the position of (i.e., rotates) the ultrasound image displayed on the display **330** based on the input information of the joystick **311**.

[0037] The operation of the ultrasound diagnostic system, which is in accordance with the second embodiment of the present invention, will be described below in view of FIGS. **3** and **4**. FIG. **4** is a flowchart for describing the operation of

the ultrasound diagnostic system, which is in accordance with the second embodiment of the present invention.

[0038] As illustrated in FIG. 4, if a user activates the probe 310 by operating the ultrasound diagnostic system 300 (step S310), the control section 321 activates the joystick 311 of the probe 310 (step S320). If the user then selects the Freeze function for obtaining the ultrasound image through a selection button 311b of the joystick 311 (step S330), then the control section 321 forms the ultrasound image based on the ultrasound echo signals acquired through the probe 310 and displays the formed ultrasound image on the display 330 (step S340).

[0039] Subsequently, the control section 312 checks whether the user selects the directional button 311a of the joystick 311. If the user selects the directional button 311a of the joystick 311 in step S350, then the control section 321 rotates the ultrasound image, which is displayed on the display 330, based on the information corresponding to the selected direction button 311a (hereinafter referred to as the "up/down/left/right information") (step S360). However, if the directional button 311a is not selected in step S350, then the process goes to step S380.

[0040] In step S370, the control section 321 checks whether the up/down/left/right information is successively inputted or not. If it is determined that the up/down/left/right information is successively inputted, step S360 is performed. If it is determined that the up/down/left/right information is not successively inputted, the process goes to step S380. In step S380, it is checked whether the ultrasound diagnostic system 300 is terminated or not. If it is determined that the ultrasound diagnostic system 300 is terminated, all the processes are terminated. If it is determined that the ultrasound diagnostic system 300 is not terminated, the process goes back to step S350.

[0041] (The Third Embodiment)

[0042] FIG. 5 is a block diagram for describing an ultrasound diagnostic system 500, which is constructed in accordance with the third embodiment of the present invention. As shown in FIG. 5, the ultrasound diagnostic system 500 of the third embodiment comprises a probe 510, a main body 520 and a display 530. The probe 510 comprises a 3D position sensor 511 and a joystick 512. The probe 510 also comprises a plurality of 1D or 2D transducers (not shown), which can send a condensed ultrasound beam along the transmission scan line to a target (not shown) by properly adjusting the timing of applying input pulses to the transducers. Such transducers are further configured to receive the ultrasound echo signals reflected from the target at different timing.

[0043] The 3D position sensor 511 detects the present position of the probe 510 and generates the position information of the probe 510. Any device may be used as the 3D position sensor 511 so long as the device can detect the position of the probe 510. For example, a gyro can be used as the 3D position sensor 511.

[0044] The joystick 512 is used to rotate the ultrasound image displayed on the display 530 in various directions (i.e., up, down, left and right). The joystick 512 comprises an up/down/left/right button 512a for rotating the ultrasound image in a number of directions, as well as a selection button 512b for acquiring an ultrasound image and adjusting the acquired ultrasound image.

[0045] The main body 520 comprises a control section 521 and a memory 522. The main body 520 is configured to perform the following: form the ultrasound image based on the ultrasound echo signals acquired from the probe 510; display the formed ultrasound image on the display 530; and rotate the ultrasound image displayed on the display 530 according to the change of position, that is, the rotation of the probe 510. The main body 520 also comprises a beam former, an image signal processor, a scan converter and an image processor (not shown).

[0046] The control section 521 controls the overall operation of the ultrasound diagnostic system 500. Particularly, the control section 521 rotates the ultrasound image displayed on the display 530 based on the position information transmitted from the 3D position sensor 511 of the probe 510 and the up/down/left/right information transmitted from the up/down/left/right button 512a of the joystick 512. The memory 522 stores the reference position information for determining the position change of the probe 510. The reference position information will be described below in detail.

[0047] The operation of the ultrasound diagnostic system, which is in accordance with the second embodiment of the present invention, will be described below in view of FIGS. 5 to 8. FIG. 6 is a flowchart for describing the operation of the ultrasound diagnostic system, which is constructed in accordance with the third embodiment of the present invention.

[0048] As illustrated in FIG. 6, if a user activates the probe 510 by operating the ultrasound diagnostic system 500 (step S510), then the control section 521 activates the 3D position sensor 511 and the joystick 512 of the probe 510 (step S520). If the user then selects the Freeze function for obtaining the ultrasound image through a selection button 512b of the joystick 512 (step S530), then the control section 521 forms the ultrasound image based on the ultrasound echo signals acquired through the probe 510 and displays the formed ultrasound image on the display 530 (step S540).

[0049] Subsequently, the control section 521 checks whether the user selects the 3D position sensor 511, that is, whether the user rotates the probe 510, or whether the user selects the joystick 512, that is, whether the user selects the buttons 512a and 512b of the joystick 512 (step S550).

[0050] In step S550, if it is determined that the user selected the 3D position sensor 511, then process A is performed. If it is determined that the user selected the joystick 512, then process B is performed. Processes A and B will be described below in detail while referring to FIGS. 7 and 8.

[0051] Subsequently, the control section 521 checks whether the ultrasound diagnostic system 500 is terminated or not (step S560). If it is determined that the ultrasound diagnostic system 500 is terminated, all the processes are terminated. If it is determined that the ultrasound diagnostic system 500 is not terminated, the process goes back to step S550.

[0052] FIG. 7 is a flowchart for describing the operation of rotating the ultrasound image by using the 3D position sensor according to the third embodiment of the present invention. As illustrated in FIGS. 6 and 7, if the user selects the 3D position sensor 511, the control section 521 enables

the 3D position sensor **511** to detect the present position of the probe **510** (step **S610**) and produce the position information corresponding to the detected present position (step **S620**). Subsequently, the control section **521** checks whether the reference position information for sensing the change of the position of the probe **510** is already set or not (step **S630**).

[**0053**] If it is determined that the reference position is not set, then the control section **521** sets the reference position of the probe **510** based on the position information transmitted from the 3D position sensor **511** (step **S640**) and stores the set reference position information into the memory **522** (step **S650**).

[**0054**] On the other hand, if it is determined that the reference position is set, then the control section **521** compares the position information transmitted from the 3D position sensor **511** with the reference position information stored in the memory **522** (step **S660**). It then produces the gap between the position information and the reference position information (step **S670**). The control section **121** then checks whether the position information is the same as the reference position information, that is, whether the gap is 0 or not (step **S680**). If it is determined that the position information is the same as the reference position information, then the process goes back to step **S610**. Otherwise, the control section **521** changes, that is, the position of the ultrasound image displayed on the display **530** is rotated based on the produced gap (step **S690**).

[**0055**] FIG. 8 is a flowchart for describing the operation of rotating the ultrasound image by using the joystick according to the third embodiment of the present invention. As illustrated in FIG. 8, if the user selects the joystick **512**, the control section **521** checks whether the up/down/left/right button **512a** of the joystick **512** is selected or not (step **S710**).

[**0056**] If it is determined that the up/down/left/right button **512a** is not selected, then the process goes back to step **S560**. Otherwise, the control section **521** rotates the ultrasound image displayed on the display **530** based on the up/down/left/right information corresponding to the selected up/down/left/right button **512a** (step **S720**).

[**0057**] In step **S730**, the control section **5021** checks whether the up/down/left/right information is successively inputted or not. If it is determined that the up/down/left/right information is successively inputted, step **S720** is performed. If it is determined that the up/down/left/right information is not successively inputted, the process goes to step **S560**.

[**0058**] While the present invention has been described and illustrated with respect to a preferred embodiment of the invention, it will be apparent to those skilled in the art that variations and modifications are possible without deviating from the broad principles and teachings of the present invention which should be limited solely by the scope of the claims appended hereto.

What is claimed is:

1. An ultrasound diagnostic system, comprising:
  - a probe;

input means attached to the probe for receiving information for use in rotating an ultrasound image in a predetermined direction; and

control means for rotating the ultrasound image based on the information from the input means.

2. The ultrasound diagnostic system as recited in claim 1, wherein the input means comprises:

a joystick for receiving up/down/left/right information to rotate the ultrasound image in up/down/left/right directions.

3. The ultrasound diagnostic system as recited in claim 1, wherein the input means comprises:

a position sensor for generating position information of the probe by detecting position of the probe.

4. The ultrasound diagnostic system as recited in claim 1, wherein the input means comprises:

a joystick for receiving up/down/left/right information to rotate the ultrasound image in up/down/left/right directions; and

a position sensor for generating position information of the probe by detecting position of the probe.

5. The ultrasound diagnostic system as recited in claim 3, wherein the position sensor comprises:

a reference position information generation section for determining a reference position of the probe and generating reference position information corresponding to the determined reference position; and

a position information generation section for generating position information of the probe based on the reference position information.

6. The ultrasound diagnostic system as recited in claim 4, wherein the position sensor comprises:

a reference position information generation section for determining a reference position of the probe and generating reference position information corresponding to the determined reference position; and

a position information generation section for generating position information of the probe based on the reference position information.

7. The ultrasound diagnostic system as recited in claim 5, further comprising:

storage means for storing the reference position information.

8. The ultrasound diagnostic system as recited in claim 6, further comprising:

storage means for storing the reference position information.

9. A method for rotating an ultrasound image by using input means attached to a probe for receiving information for use in rotating an ultrasound image, comprising the steps of:

- a) activating the probe and the input means;
- b) forming and displaying the ultrasound image based on ultrasound echo signals acquired through the probe;
- c) receiving information for rotating the displayed ultrasound image through the input means; and
- d) rotating the ultrasound image based on the information.

10. The method as recited in claim 9, wherein the step c) comprises the step of:

receiving information for rotating the ultrasound image in up/down/left/right directions.

11. The method as recited in claim 9, wherein the step c) comprises the steps of:

c1) generating reference position information by determining a reference position of the probe;

c2) generating present position information by detecting a present position of the probe; and

c3) generating rotation information for rotating the ultrasound image based on the reference position information and the present position information.

12. The method as recited in claim 9, wherein the step c) comprises the steps of:

e1) analyzing information inputted through the input means;

e2) if the information is information for rotating the ultrasound image in up/down/left/right directions, performing the step d);

e3) if the information is position information of the probe, generating reference position information by determining a reference position of the probe;

e4) generating present position information by detecting a present position of the probe; and

e5) generating rotation information for rotating the ultrasound image based on the reference position information and the present position information.

\* \* \* \* \*

专利名称(译)	超声诊断系统和旋转超声图像的方法		
公开(公告)号	<a href="#">US20070073148A1</a>	公开(公告)日	2007-03-29
申请号	US11/401324	申请日	2006-04-11
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	KIM NAM WOONG		
发明人	KIM, NAM WOONG		
IPC分类号	A61B8/00		
CPC分类号	A61B8/00 A61B8/461 G01S15/8993 G01S15/899 A61B8/467 A61B8/466		
优先权	1020050085562 2005-09-14 KR		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

摘要(译)

超声诊断系统和方法技术领域本发明涉及一种超声诊断系统和一种用于通过使用附接到探头的3D位置传感器和/或操纵杆来旋转显示在显示器上的超声图像的方法。一种用于旋转超声图像的方法包括以下步骤：a) 激活探头和3D位置传感器和/或操纵杆；b) 基于通过探头获取的超声回波信号形成和显示超声图像；c) 接收用于通过3D位置传感器和/或操纵杆旋转显示的超声图像的信息；d) 根据信息旋转超声图像。

