



US 20080071175A1

(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2008/0071175 A1**

LEE et al.

(43) **Pub. Date:** **Mar. 20, 2008**

(54) **ULTRASOUND SYSTEM AND METHOD FOR FORMING ULTRASOUND IMAGES**

(75) Inventors: **Jae Keun LEE**, Seoul (KR); **Chi Young Ahn**, Seoul (KR)

Correspondence Address:

OBLON, SPIVAK, MCCLELLAND MAIER & NEUSTADT, P.C.
1940 DUKE STREET
ALEXANDRIA, VA 22314

(73) Assignee: **Medison Co., Ltd.**, Hongchun-gun (KR)

(21) Appl. No.: **11/759,703**

(22) Filed: **Jun. 7, 2007**

(30) **Foreign Application Priority Data**

Sep. 19, 2006 (KR) 10-2006-0090671

Publication Classification

(51) **Int. Cl.**
A61B 8/00 (2006.01)

(52) **U.S. Cl.** **600/443**

(57) **ABSTRACT**

The present invention provides an ultrasound system for forming an ultrasound image by using a plurality of sub-frames, comprising: a plurality of transducers for transmitting and receiving ultrasound signals along a plurality of scan lines to obtain sub-frames; a determination unit for locating a common point where extensions of said scan lines with respect to the transducers intersect, determine a plurality of virtual common points based on the located common point and determine a plurality of transducer groups, steering angles and a plurality of scan-line groups; a controller responsive to a change of the sub-frames to select scan lines corresponding to the changed sub-frame and adjust steering angles of the selected scan lines based on the plurality of transducer groups, the steering angles and the plurality of scan-line groups; and a processor for synthesizing the plurality of sub-frames to form an ultrasound image.

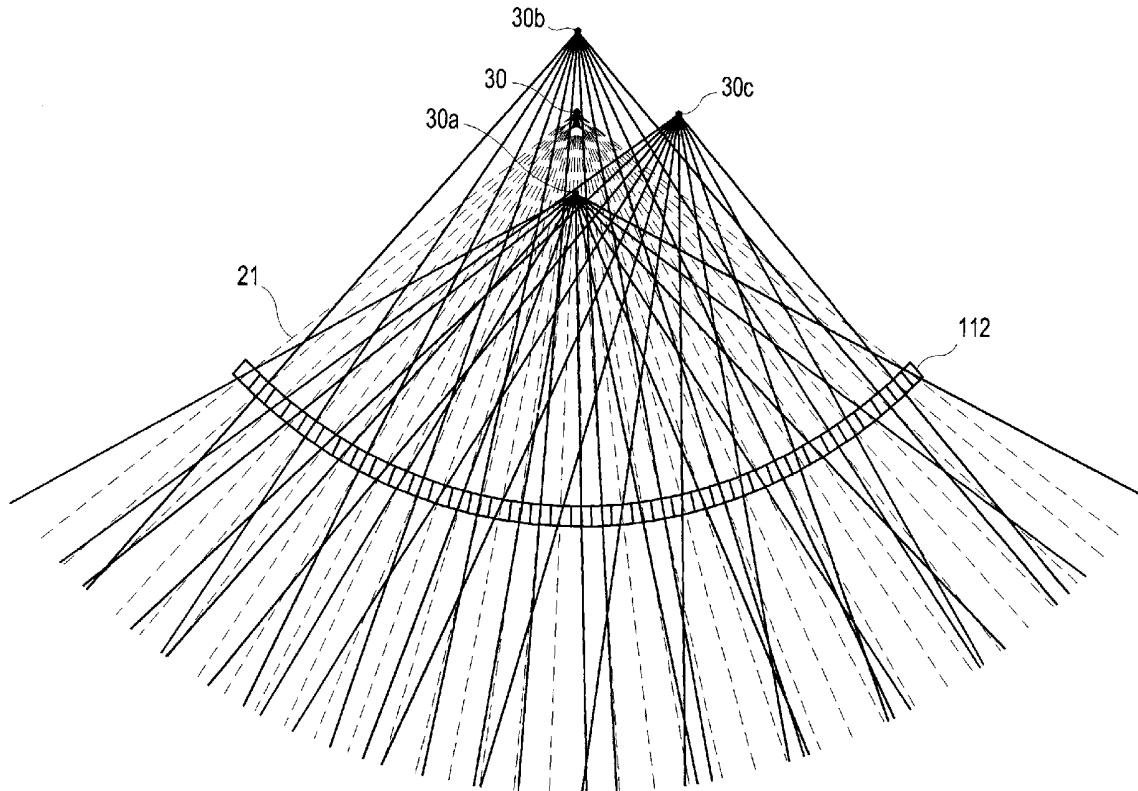


FIG. 1
(PRIOR ART)

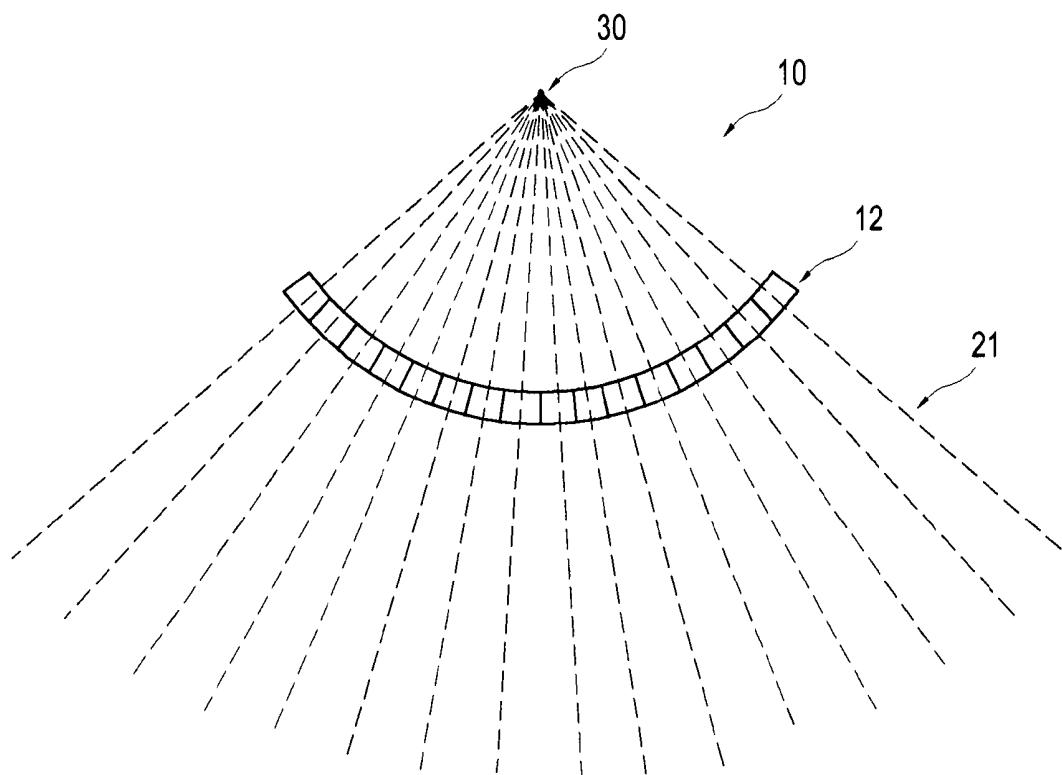


FIG. 2
(PRIOR ART)

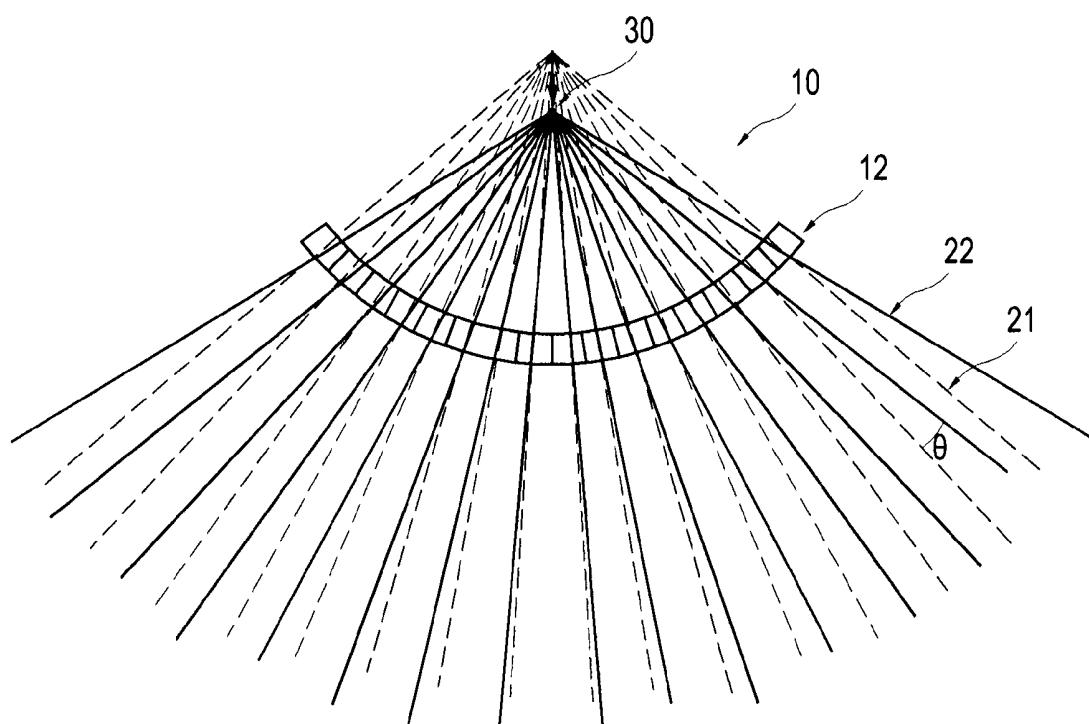


FIG. 3

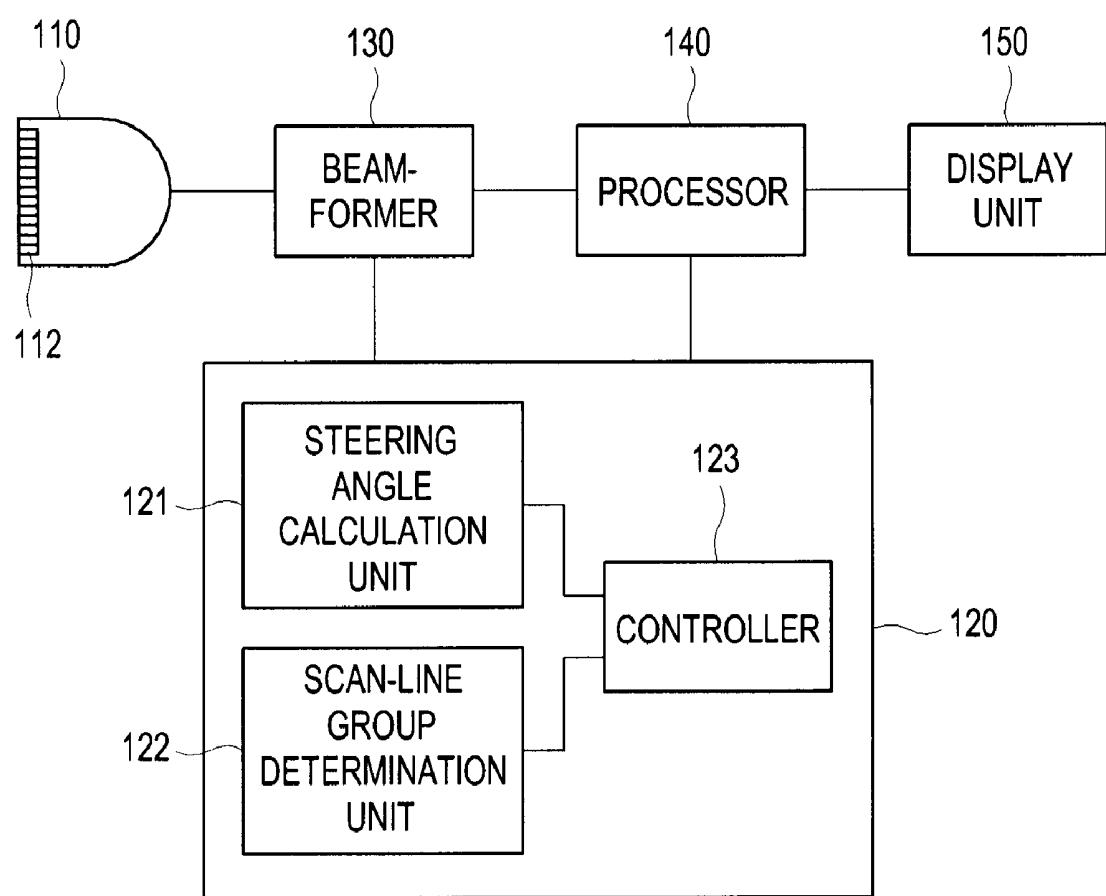


FIG. 4

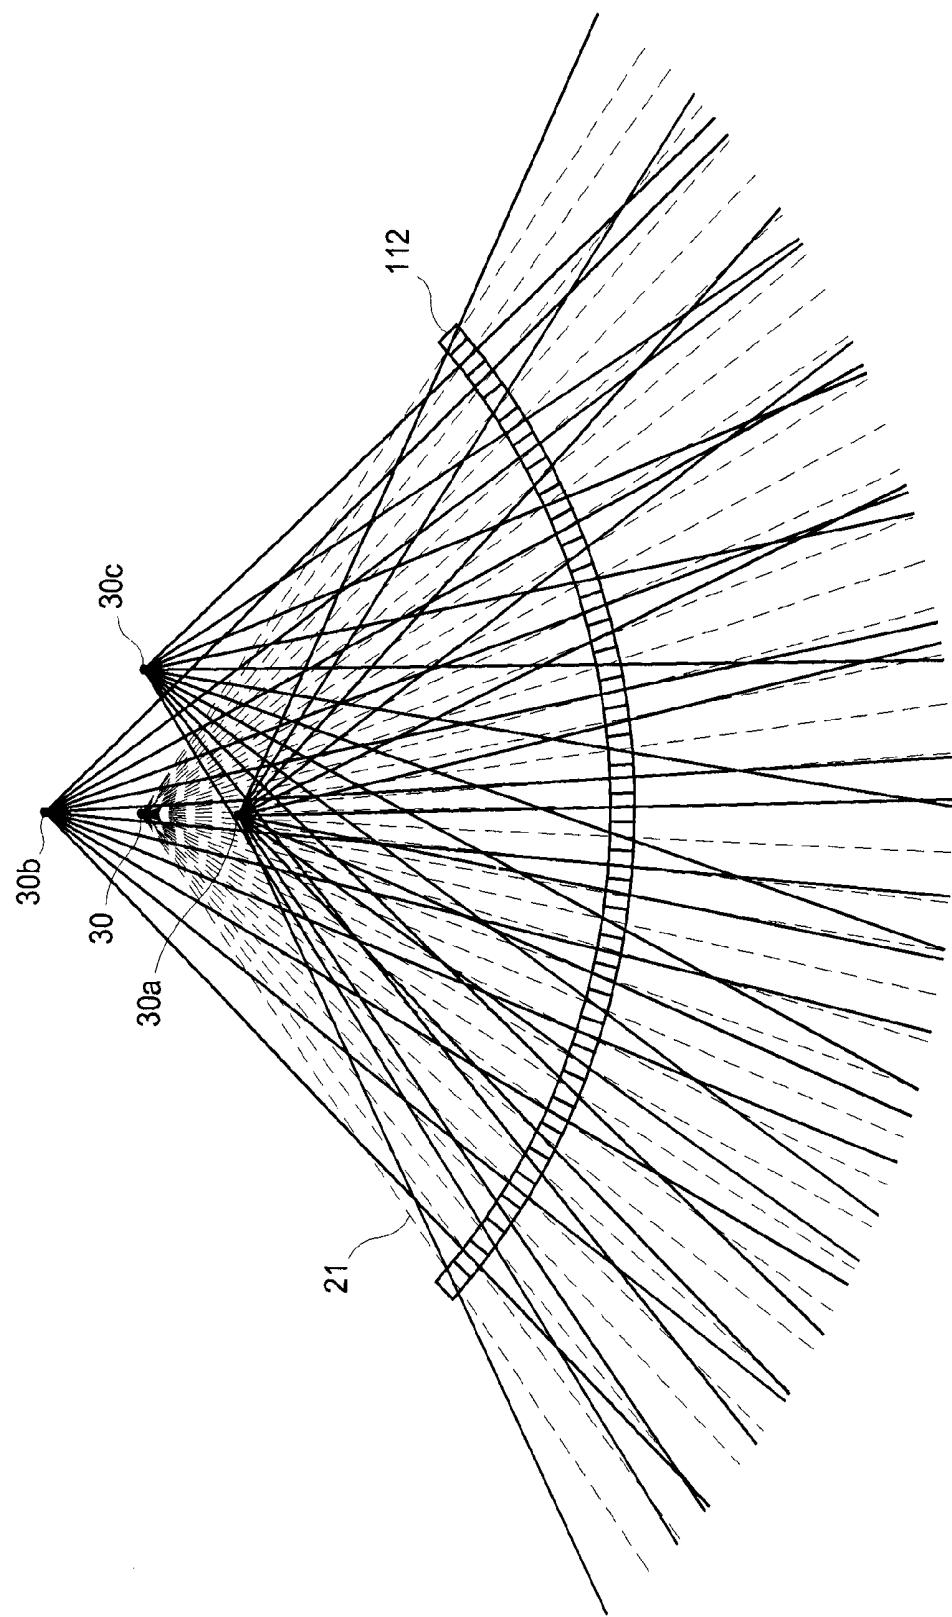


FIG. 5

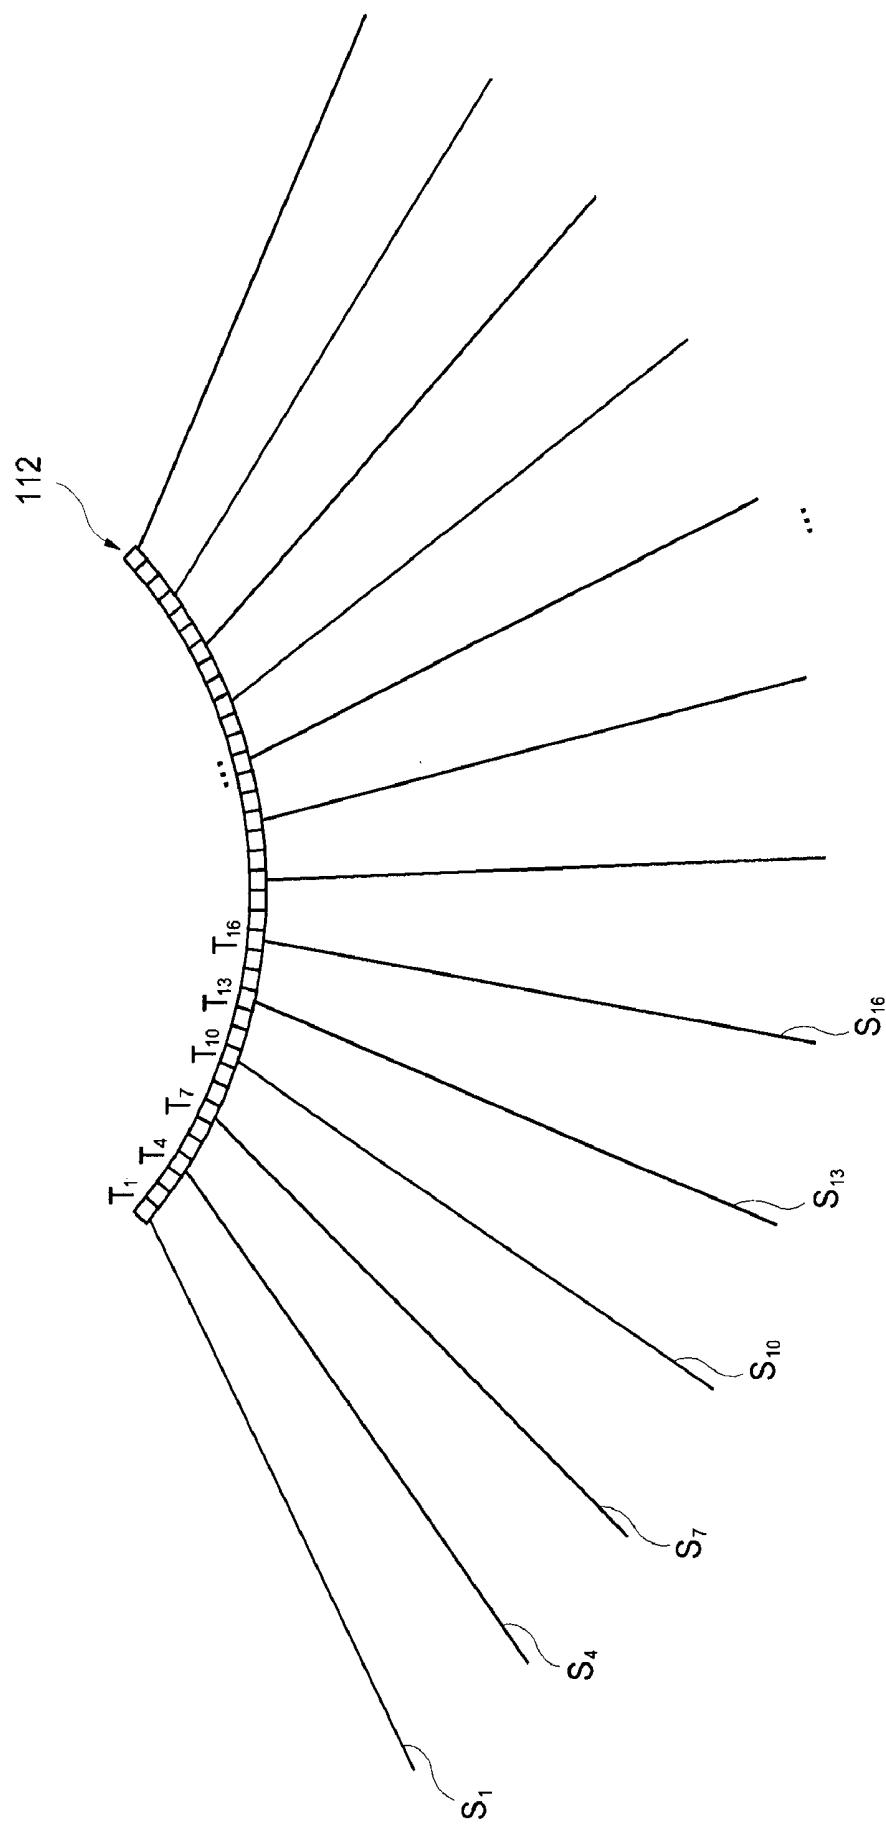


FIG. 6

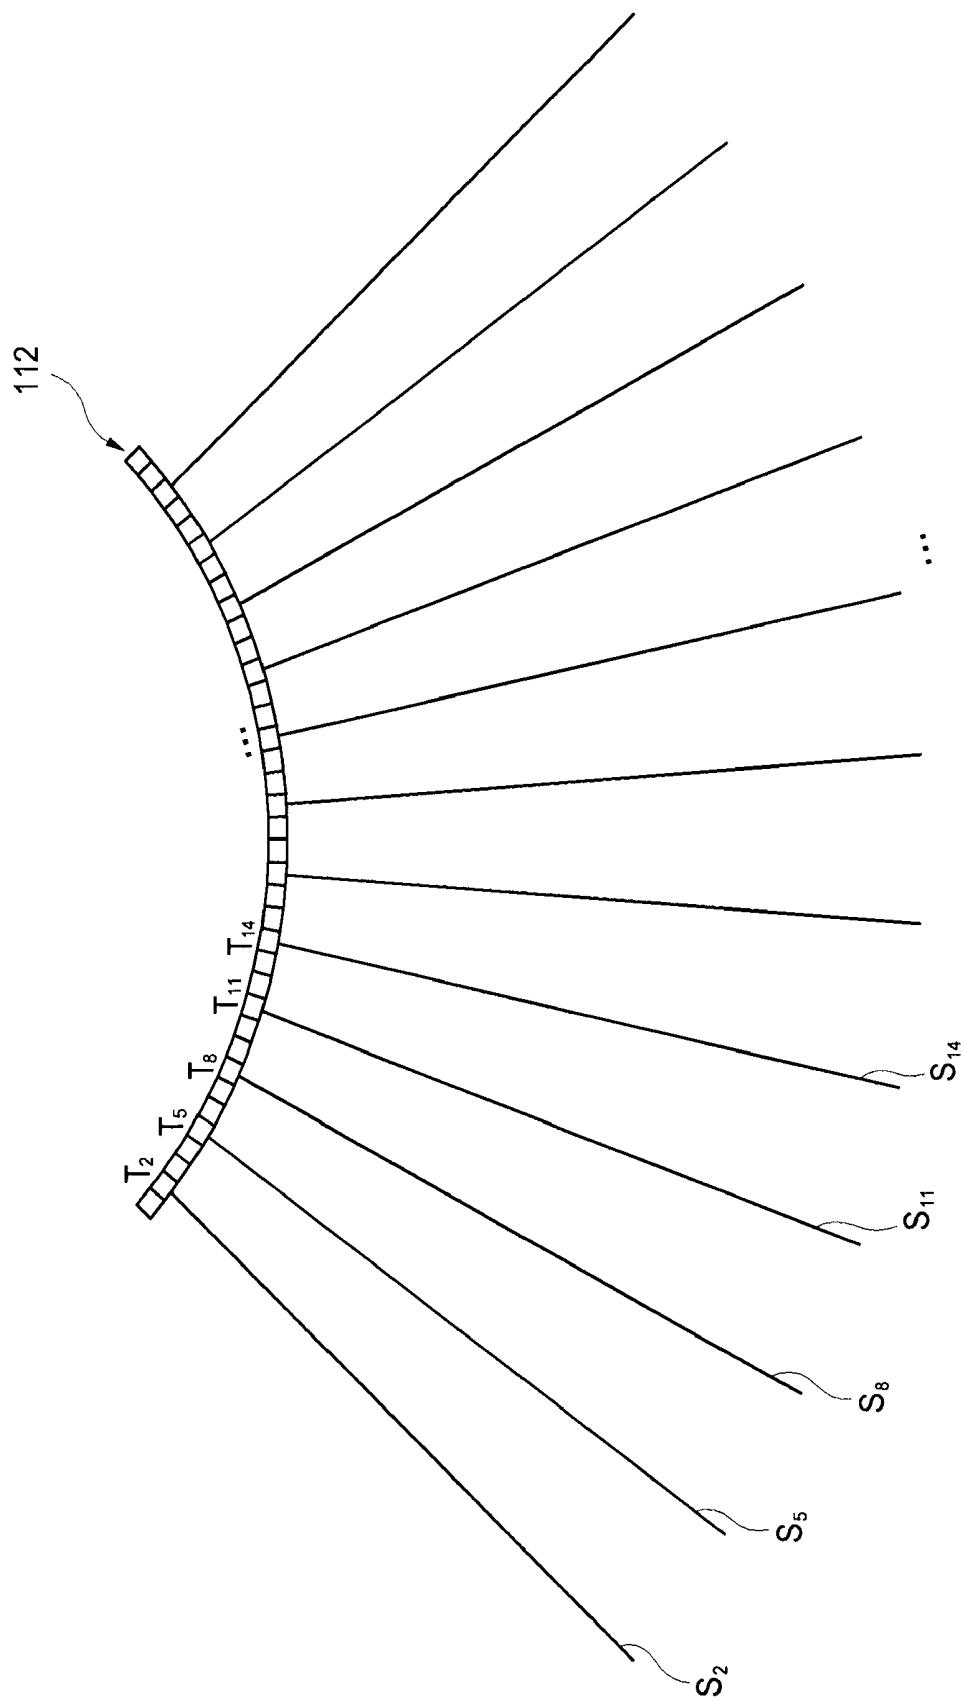


FIG. 7

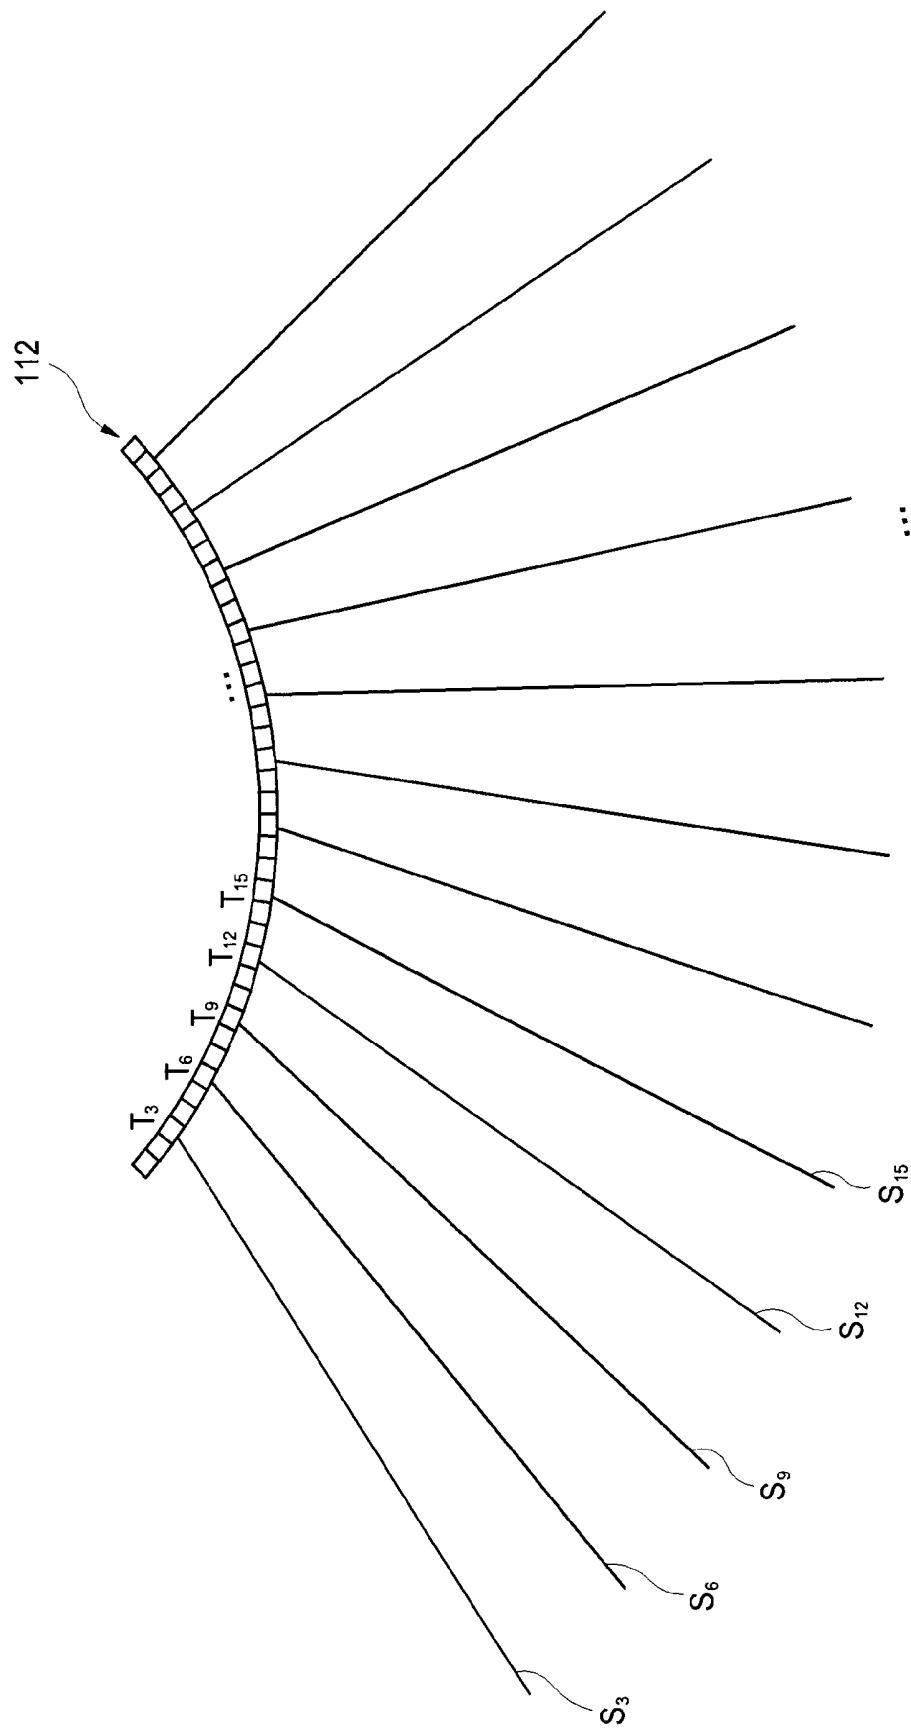


FIG. 8

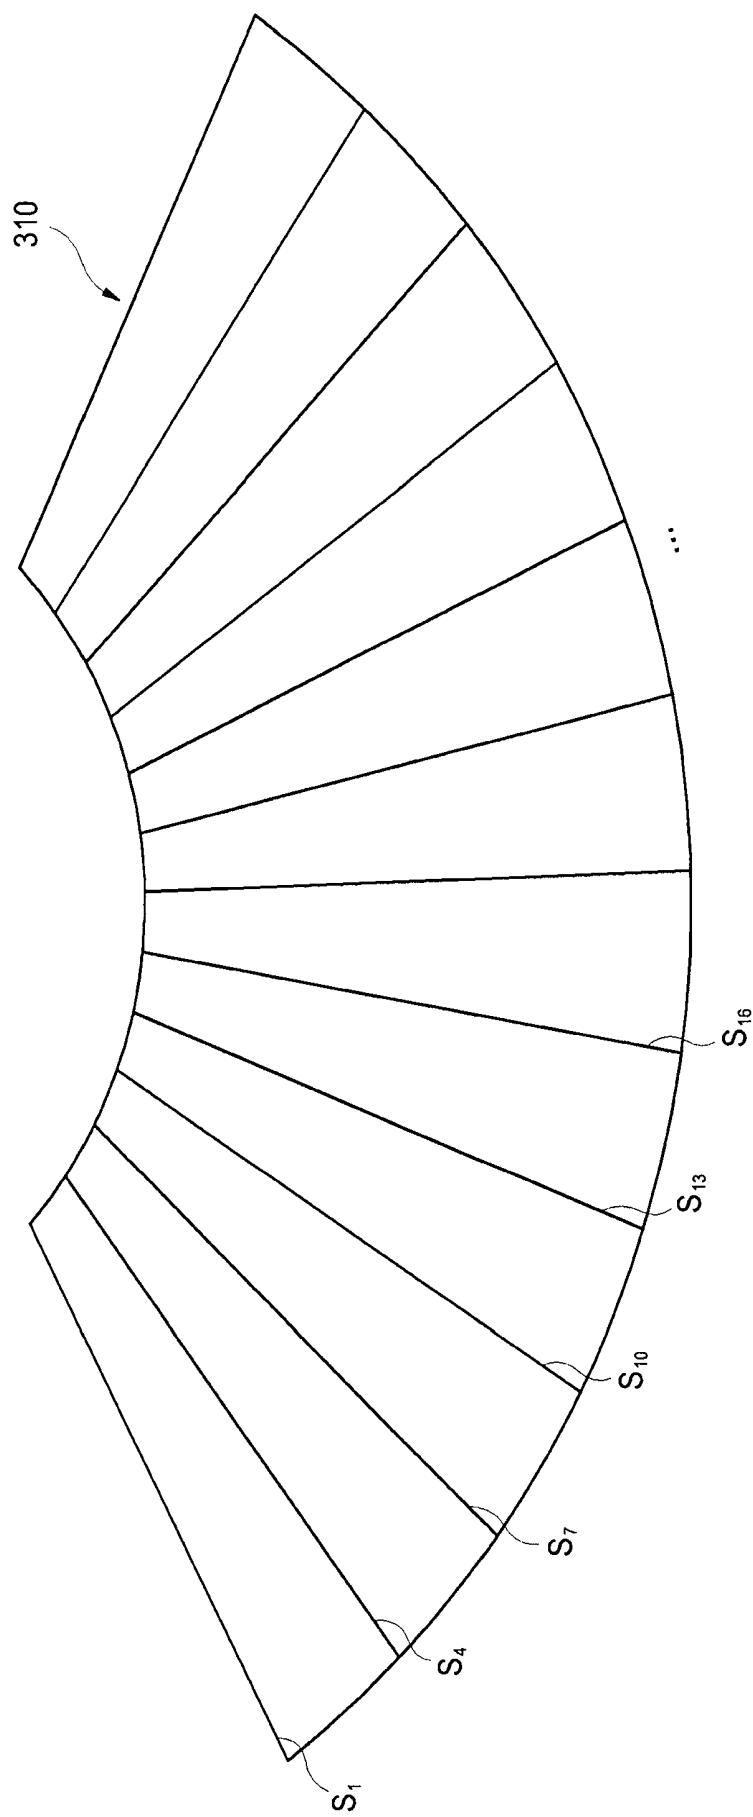


FIG. 9

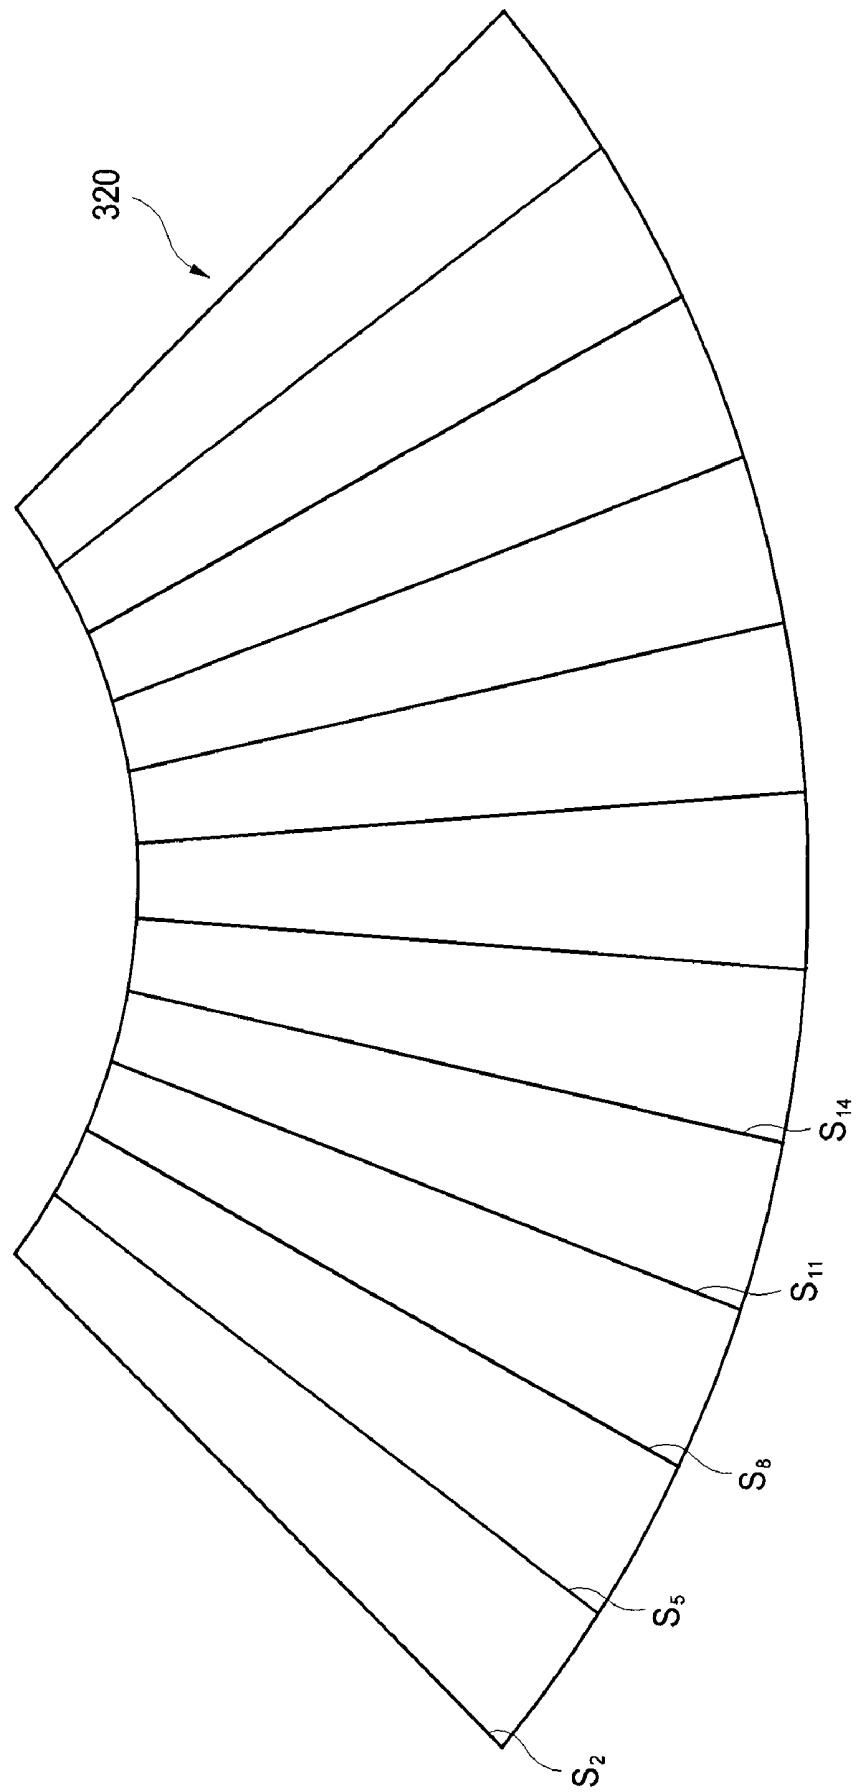


FIG. 10


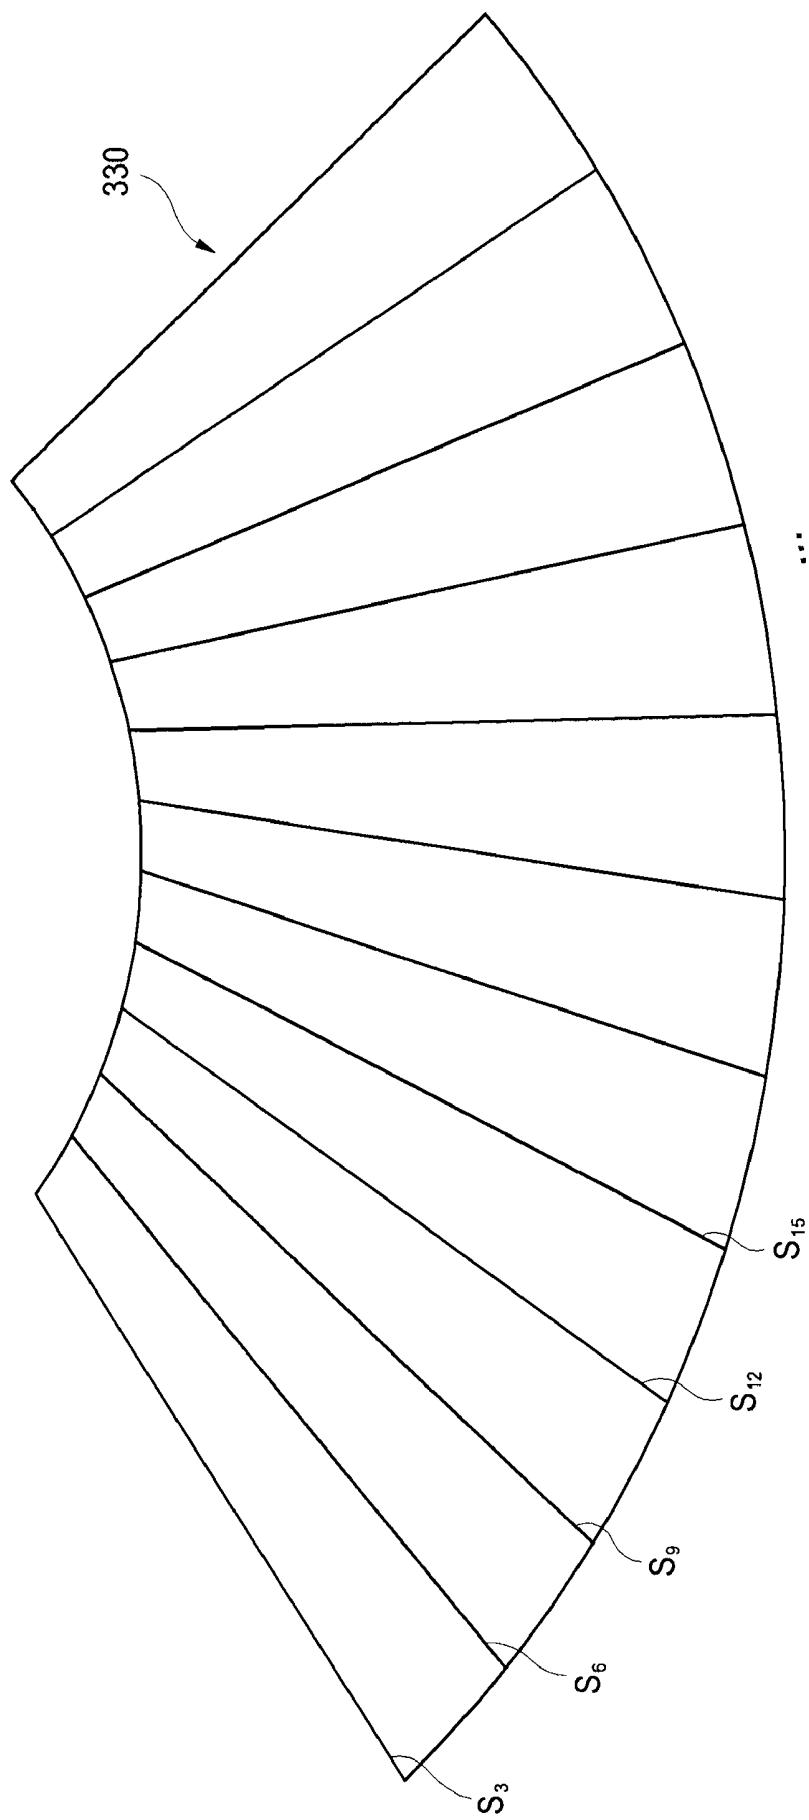


FIG. 11

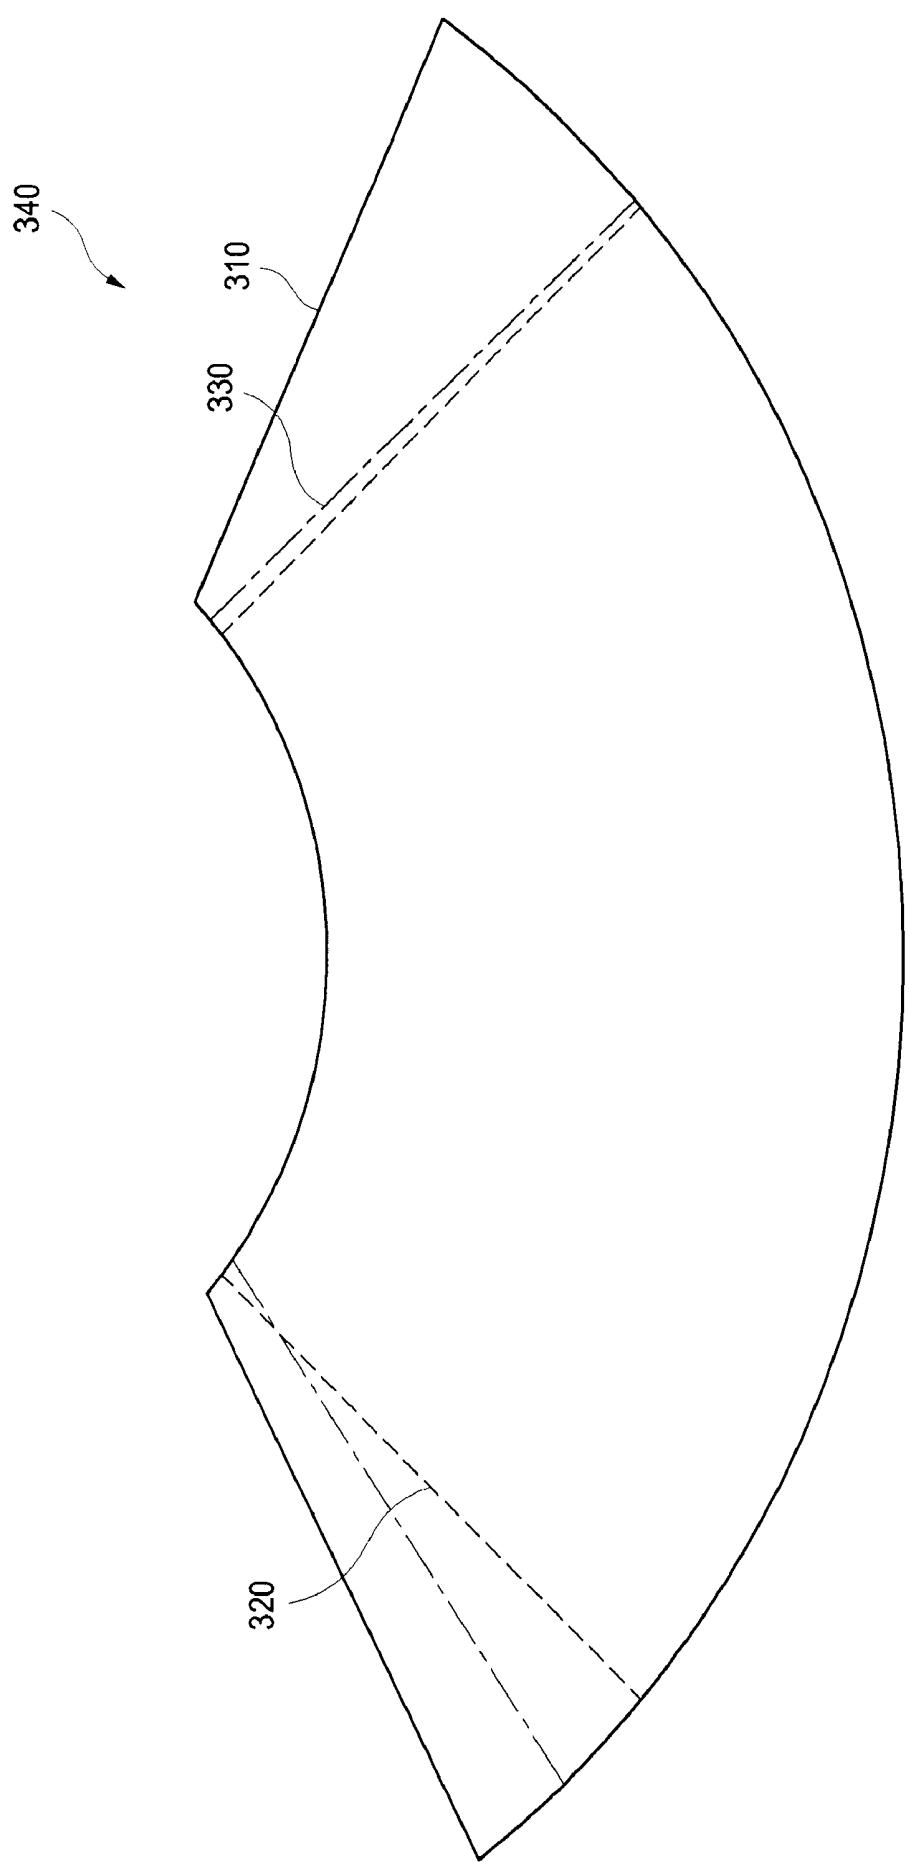

ULTRASOUND SYSTEM AND METHOD FOR FORMING ULTRASOUND IMAGES

[0001] The present application claims priority from Korean Patent Application No. 10-2006-0090671 filed on Sep. 19, 2006, the entire subject matter of which is incorporated herein by reference.

BACKGROUND

[0002] 1. Field

[0003] The present invention generally relates to an ultrasound system, and more particularly to an ultrasound system and method for forming an ultrasound image.

[0004] 2. Background

[0005] An ultrasound system has become an important and popular diagnostic tool since it has a wide range of applications. Specifically, due to its non-invasive and non-destructive nature, the ultrasound system has been extensively used in the medical profession. Modern high-performance ultrasound systems and techniques are commonly used to produce two or three-dimensional diagnostic images of internal features of an object (e.g., human organs).

[0006] The probe of an ultrasound system generally includes transducers for transmitting and receiving broadband ultrasound signals. When the transducers are electrically stimulated, ultrasound signals are generated and transmitted to the object. Signals reflected from the object and delivered to the transducers, which may be referred to as ultrasound echo signals, are electrically transformed. By performing amplification and signal processing on the transformed electrical signals, ultrasound image data can be generated.

[0007] In particular, a number of ultrasound systems employ a curved linear probe to transmit and receive ultrasound signals. Since the curved linear probe transmits ultrasound signals in radial directions, it can obtain an ultrasound image in an area wider than the size of the probe. FIG. 1 shows a geometrical structure of scan lines for the respective transducers in a curved linear probe. As illustrated in FIG. 1, when the respective scan lines 21 are extended back to the rear of the transducers 12, there appears a point 30, through which all the scan lines pass (hereinafter referred to as a "common point"). Conversely, steering angles of the respective scan lines 21 can be determined once the location of the common point 30 is determined. As shown in FIG. 2, when the common point 30 moves, the steering angles of the respective scan lines 21 change. Thereafter, by constructing new scan lines 22 according to the newly determined steering angles, an ultrasound image having a wider view angle can be obtained.

[0008] However, in a conventional ultrasound system, gaps formed between the scan lines become greater as the common point moves for a wider view angle. This deteriorates the quality of the ultrasound image, and more particularly the quality of the object located around the center of the ultrasound image.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] Arrangements and embodiments may be described in detail with reference to the following drawings in which like reference numerals refer to like elements and wherein:

[0010] FIG. 1 shows a geometrical structure of scan lines for respective transducers of a curved linear probe;

[0011] FIG. 2 shows a geometrical structure of scan lines for respective transducers of a conventional curved linear probe with adjusted steering angles;

[0012] FIG. 3 shows a configuration of an ultrasound system constructed in accordance with an embodiment of the present invention;

[0013] FIG. 4 shows an example of determining steering angles in accordance with an embodiment of the present invention;

[0014] FIGS. 5 to 7 show an example of determining groups of scan lines in accordance with an embodiment of the present invention;

[0015] FIGS. 8 to 10 show an example of sub-frames of the respective scan-line groups in accordance with an embodiment of the present invention; and

[0016] FIG. 11 shows an example of a frame formed by spatially synthesizing sub-frames in accordance with an embodiment of the present invention.

DETAILED DESCRIPTION

[0017] A detailed description may be provided with reference to the accompanying drawings. One of ordinary skill in the art may realize that the following description is illustrative only and is not in any way limiting. Other embodiments of the present invention may readily suggest themselves to such skilled persons having the benefit of this disclosure.

[0018] An ultrasound system constructed in accordance with an embodiment of the present invention includes a plurality of transducers, a determination unit, a controller and a processor. The transducers transmit and receive ultrasound signals along a plurality of scan lines to obtain sub-frames. The determination unit locates a common point where extensions of the scan lines with respect to the transducers intersect, and determines a plurality of virtual common points based on the located common point. The determination unit then determines a plurality of transducer groups, steering angles and a plurality of scan-line groups. Based on the transducer groups, the steering angles and the scan-line groups, the controller selects scan lines corresponding to the changed sub-frames and adjusts steering angles of the selected scan lines as the sub-frame changes. The processor synthesizes the sub-frames to form an ultrasound image.

[0019] Hereinafter, an embodiment of the present invention will be described with reference to FIGS. 3 to 11. As shown in FIG. 3, an ultrasound system 100 constructed in accordance with an embodiment of the present invention includes a probe 110, a scan-line determination unit 120, a beam-former 130, a processor 140 and a display unit 150.

[0020] The probe 110 includes a transducer array 112 comprising a plurality of transducers. The probe 110 transmits ultrasound signals to an object along scan lines and receives ultrasound signals reflected by the object. In an embodiment, the probe 110 may be a curved linear probe.

[0021] The scan-line determination unit 120 includes a steering angle calculation unit 121, a scan-line group determination unit 122 and a controller 123. The steering angle calculation unit 121 locates a plurality of virtual common points based on the common point where extensions of original scan lines for the respective transducers intersect. It then partitions a plurality of transducers into several groups

based on the number of located virtual common points. Thereafter, the steering angle calculation unit 121 matches virtual common points to the respective transducer groups and calculates adjusted steering angles of the scan lines for the respective transducers.

[0022] In an embodiment shown in FIG. 4, based on the location of the common point 30 where extensions of the original scan lines 21 with respect to the respective transducers intersect, the steering angle calculation unit 121 may locate: a first virtual common point 30a by moving the common point 30 toward the transducer array 112; a second virtual common point 30b by moving the common point 30 far from the transducer array 112; and a third virtual common point 30c by moving the common point 30 in parallel with the transducer array 112. It may then partition a plurality of scan lines into 3 groups according to the number of the located virtual common points. That is, among a plurality of transducers T₁ to T_n, the steering angle calculation unit 121 may determine: transducers {T₁, T₄, T₇, T₁₀, . . . } as a first transducer group; transducers {T₂, T₅, T₈, T₁₁, . . . } as a second transducer group; and transducers {T₃, T₆, T₉, T₁₂, . . . } as a third transducer group. The steering angle calculation unit 121 may determine: the first virtual common point 30a as a virtual common point corresponding to the first transducer group; the second virtual common point 30b as a virtual common point corresponding to the second transducer group; and the third virtual common point 30c as a virtual common point corresponding to the third transducer group. Thereafter, the steering angle calculation unit 121 calculates steering angles of the scan lines for the respective transducers based on the location of the corresponding virtual common points.

[0023] Although the above embodiment partitions a plurality of transducers into three groups based on three virtual common points, the present invention is not limited thereto. It is also possible to locate N number of virtual common points and to partition a plurality of transducers T₁ to T_n based on the number N of the located virtual common points. For example, the plurality of transducers T₁ to T_n may be partitioned so that the transducers {T₁, T_{N+1}, T_{2N+1}, T_{3N+1}, . . . } constitute a first transducer group, the transducers {T₂, T_{N+2}, T_{2N+2}, T_{3N+2}, . . . } constitute a second transducer group, and {T_N, T_{2N}, T_{3N}, T_{4N}, . . . } constitute an Nth transducer group.

[0024] Further, in the above embodiment, the common point is moved into vertical and horizontal directions to locate a plurality of virtual common points. However, the present invention is not limited thereto. That is, the common point may be moved in various directions to locate a plurality of virtual common points.

[0025] The scan-line group determination unit 122 determines scan-line groups to obtain a plurality of sub-frames. Assume that three virtual common points 30a, 30b and 30c are located by the steering angle calculation unit 121 and transducer groups are determined based on the three located virtual common points 30a, 30b and 30c in accordance with an embodiment of the present invention. Then, the scan-line group determination unit 122 may determine, among a plurality of scan lines S₁ to S_n; scan lines {S₁, S₄, S₇, S₁₀, . . . } corresponding to the first transducer group as a first scan-line group to obtain a first sub-frame; scan lines {S₂, S₅, S₈, S₁₁, . . . } corresponding to the second transducer group as a second scan-line group to obtain a second sub-frame; and scan lines {S₃, S₆, S₉, S₁₂, . . . } as a third

scan-line group to obtain a third sub-frame. Although the above embodiment describes partitioning a plurality of scan lines into three scan-line groups based on the three virtual common points, the present invention is not limited thereto. For example, it is also possible to partition a plurality of scan lines S₁ to S_n based on the number N of located virtual common points. As a further example, the scan lines S₁ to S_n may be partitioned so that the scan lines {S₁, S_{N+1}, S_{2N+1}, S_{3N+1}, . . . } constitute a first scan-line group, the scan lines {S₂, S_{N+2}, S_{2N+2}, S_{3N+2}, . . . } constitute a second scan-line group, and {S_N, S_{2N}, S_{3N}, S_{4N}, . . . } constitute an Nth scan-line group.

[0026] In order to obtain a plurality of sub-frames, the controller 123 performs control whenever the frame changes so that ultrasound signals are transmitted along the scan lines of the scan-line groups corresponding to the respective sub-frames. In an embodiment of the present invention, in order to obtain a first sub-frame 310 as shown in FIG. 8, the controller 123 performs control so that ultrasound signals are transmitted along the respective scan lines {S₁, S₄, S₇, . . . , S_{n-2}} of the first scan-line group as shown in FIG. 5. The controller 123 further performs control so that ultrasound signals are transmitted along the respective scan lines {S₂, S₅, S₈, . . . , S_{n-1}} of the second scan-line group as shown in FIG. 6. This is in order to obtain a second sub-frame 320 as shown in FIG. 9. Further, the ultrasound signals are transmitted along the respective scan lines {S₃, S₆, S₉, . . . , S_n} of the third scan-line group as shown in FIG. 7 in order to obtain a third sub-frame 330 as shown in FIG. 10. The controller 123 also controls the processor 140 to synthesize a plurality of sub-frames based on the virtual common points, the steering angles, the transducer groups and the scan-line groups, thereby forming one frame of the ultrasound image.

[0027] Under the control of the controller 123, the beam-former 130 delays and sums up the ultrasound signals, which are transmitted and received by the transducers along scan lines corresponding to each of the scan-line groups. The processor 140 forms one frame by spatially synthesizing a plurality of sub-frames provided by the beam-former 130 under the control of the controller 123. It then forms an ultrasound image signal based on the synthesized frame. In an embodiment of the present invention, the processor 140 spatially synthesizes sub-frames 310 to 330 as shown in FIGS. 8 to 10 to form a frame 340 as shown in FIG. 11. In such a case, the processor 140 may perform the synthesizing by calculating average of each pixel (e.g., averaged intensity of each pixel) through a plurality of sub-frames 310 to 330, or by providing different weights on the sub-frames. The processor 140 may further perform interpolation processing on each sub-frame using a variety of image interpolation methods before spatially synthesizing the sub-frames. The processor 140 may also include a storage unit to temporarily store the sub-frames. The display unit 150 receives the ultrasound image signal from the processor 140 and displays the ultrasound image.

[0028] Any reference in this specification to "one embodiment," "an embodiment," "example embodiment," etc., means that a particular feature, structure or characteristic described in connection with the embodiment is included in at least one embodiment of the invention. The appearances of such phrases in various places in the specification are not necessarily all referring to the same embodiment. Further, when a particular feature, structure or characteristic is

described in connection with any embodiment, it is submitted that it is within the purview of one skilled in the art to affect such feature, structure or characteristic in connection with other ones of the embodiments.

[0029] Although embodiments have been described with reference to a number of illustrative embodiments thereof, it should be understood that numerous other modifications and embodiments can be devised by those skilled in the art that will fall within the spirit and scope of the principles of this disclosure. More particularly, various variations and modifications are possible in the component parts and/or arrangements of the subject combination arrangement within the scope of the disclosure, the drawings and the appended claims. For example, although the embodiments have been described as employing a curved linear probe, the present invention is not limited thereto, and it is also possible to use a linear probe, in which case a plurality of virtual common points may be formed by moving a common point located in an infinite point. In addition to variations and modifications in the component parts and/or arrangements, alternative uses will also be apparent to those skilled in the art.

What is claimed is:

1. An ultrasound system for forming an ultrasound image by using a plurality of sub-frames, comprising:

a plurality of transducers for transmitting and receiving ultrasound signals along a plurality of scan lines to obtain sub-frames;

a determination unit for locating a common point where extensions of the scan lines with respect to the transducers intersect and determine a plurality of virtual common points based on the located common point, the determination unit further being configured to determine a plurality of transducer groups, steering angles and a plurality of scan-line groups;

a controller for being responsive to a change of the sub-frames to select scan lines corresponding to the changed sub-frame and adjust steering angles of the selected scan lines based on the plurality of transducer groups, the steering angles and the plurality of scan-line groups; and

a processor for synthesizing the plurality of sub-frames to form an ultrasound image.

2. The ultrasound system of claim 1, wherein the determination unit includes:

a first determination unit for determining the plurality of transducer groups by grouping the plurality of transducers according to the number of the virtual common points;

a second determination unit for matching the virtual common points with the plurality of transducer groups and determine the steering angles of the scan lines for the respective transducers; and

a third determination unit for determining the plurality of scan-line groups by grouping the scan lines corresponding to the respective transducer groups.

3. The ultrasound system of claim 1, wherein the processor includes:

a unit for calculating an averaged intensity of each pixel through the plurality of sub-frames and form the ultrasound image by synthesizing the plurality of sub-frames based on the calculated average intensity.

4. The ultrasound system of claim 1, wherein the processor includes:

a unit for providing different weights on the plurality of sub-frames and form the ultrasound image by synthesizing the plurality of sub-frames provided with the different weights.

5. A method of forming an ultrasound image by using a plurality of sub-frames formed with a plurality of transducers to transmit and receive ultrasound signals along a plurality of scan lines, comprising the steps of:

(a) determining a plurality of virtual common points based on a common point where extensions of a plurality of scan lines intersect;

(b) determining a plurality of transducer groups, steering angles and a plurality of scan-line groups based on the plurality of virtual common points;

(c) in response to a change of sub-frames, selecting scan lines corresponding to the changed sub-frame and adjusting steering angles of the selected scan lines based on the plurality of transducer groups, the steering angles and the plurality of scan-line groups;

(d) forming a plurality of sub-frames by transmitting and receiving ultrasound signals along the scan lines with the adjusted steering angles; and

(e) forming an ultrasound image by synthesizing the plurality of sub-frames.

6. The method of claim 5, wherein the step (b) includes:

(b1) determining the plurality of transducer groups by grouping a plurality of transducers according to the number of the virtual common points;

(b2) matching the virtual common points with the plurality of transducer groups and determining the steering angles of the scan lines for the respective transducers; and

(b3) determining the plurality of scan-line groups corresponding to the respective transducer groups.

7. The method of claim 5, wherein the step (e) includes: calculating averaged intensity of each pixel through the plurality of sub-frames and forming the ultrasound image by synthesizing the plurality of sub-frames based on the calculated average intensity.

8. The method of claim 5, wherein the step (e) includes:

providing different weights on the plurality of sub-frames and forming the ultrasound image by synthesizing the plurality of sub-frames provided with the different weights.

* * * * *

专利名称(译)	超声系统和形成超声图像的方法		
公开(公告)号	US20080071175A1	公开(公告)日	2008-03-20
申请号	US11/759703	申请日	2007-06-07
申请(专利权)人(译)	MEDISON CO. , LTD.		
当前申请(专利权)人(译)	MEDISON CO. , LTD.		
[标]发明人	LEE JAE KEUN AHN CHI YOUNG		
发明人	LEE, JAE KEUN AHN, CHI YOUNG		
IPC分类号	A61B8/00		
CPC分类号	G01S7/52085 G01S15/8995 G01S15/8927		
优先权	1020060090671 2006-09-19 KR		
其他公开文献	US7766835		
外部链接	Espacenet USPTO		

摘要(译)

本发明提供一种超声系统，用于通过多个子帧形成超声图像，包括：多个换能器，用于沿多条扫描线发送和接收超声信号，以获得子帧；确定单元，用于定位所述扫描线相对于换能器的延伸相交的公共点，基于所定位的公共点确定多个虚拟公共点，并确定多个换能器组，转向角和多个扫描 - 线组；控制器响应于子帧的改变以选择对应于改变的子帧的扫描线，并基于多个换能器组，转向角和多个扫描线组调整所选扫描线的转向角；处理器，用于合成多个子帧以形成超声图像。

