



US 20190015072A1

(19) **United States**

(12) **Patent Application Publication**
DELADI et al.

(10) **Pub. No.: US 2019/0015072 A1**
(43) **Pub. Date: Jan. 17, 2019**

(54) **MEDICAL DEVICE WITH FORWARD AND
SIDEWARD ABLATION MONITORING
ULTRASOUND TRANSDUCERS**

A61B 34/20 (2016.01)
A61B 8/08 (2006.01)
B06B 1/06 (2006.01)
A61B 90/00 (2016.01)
G01S 15/46 (2006.01)
A61B 18/00 (2006.01)
A61B 18/14 (2006.01)

(71) Applicant: **KONINKLIJKE PHILIPS N.V.**,
Eindhoven (NL)

(72) Inventors: **Szabolcs DELADI**, Veldhoven (NL);
**Cornelius Antonius Nicolaas Maria
VAN DER VLEUTEN**, Liempde (NL);
**Antonius Johannes Josephus
RADEMAKERS**, Eindhoven (NL)

(52) **U.S. Cl.**
CPC *A61B 8/4483* (2013.01); *A61B 18/1492*
(2013.01); *A61B 34/20* (2016.02); *A61B*
8/0883 (2013.01); *A61B 8/445* (2013.01);
B06B 1/0629 (2013.01); *A61B 2034/2063*
(2016.02); *Y10T 29/42* (2015.01); *A61B*
2034/2051 (2016.02); *A61B 2090/3782*
(2016.02); *G01S 2015/465* (2013.01); *A61B*
2018/00738 (2013.01); *A61B 2018/00839*
(2013.01); *A61B 2090/364* (2016.02); *A61B*
8/12 (2013.01)

(21) Appl. No.: **16/129,837**

(22) Filed: **Sep. 13, 2018**

Related U.S. Application Data

(62) Division of application No. 13/885,796, filed on Feb.
4, 2014, filed as application No. PCT/IB2011/054330
on Oct. 3, 2011.

Foreign Application Priority Data


Nov. 18, 2010 (EP) 10191687.2

Publication Classification

(51) **Int. Cl.**
A61B 8/00 (2006.01)
A61B 8/12 (2006.01)

(57) **ABSTRACT**

The invention relates to ultrasound imaging method and apparatus suitable for minimally invasive ultrasound diagnostic devices in cardiac ablation monitoring and in tumor ablation monitoring. The present invention proposes an assembly of forward and side-facing transducers and a system of embedded forward and side-facing transducers in apertures on surfaces of the assembly. This provides control of the acoustic properties of the transducer and improved ablation monitoring when the assembly is incorporated in a medical device.

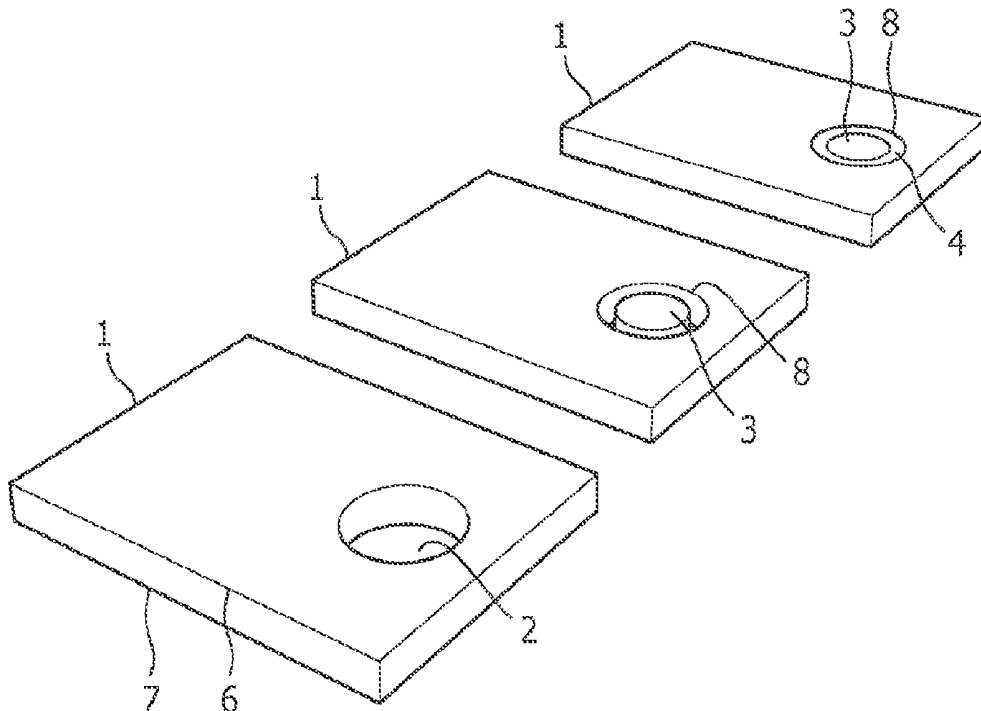

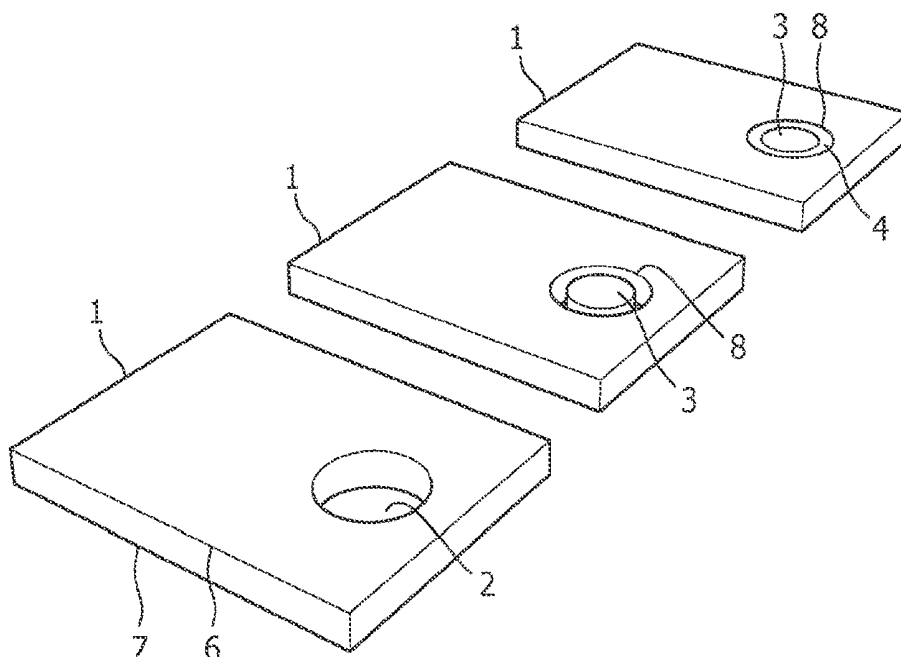


FIG. 1

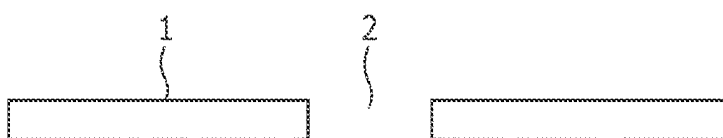


FIG. 2a

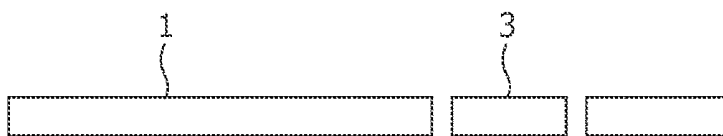


FIG. 2b

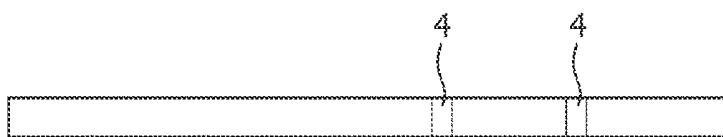


FIG. 2c

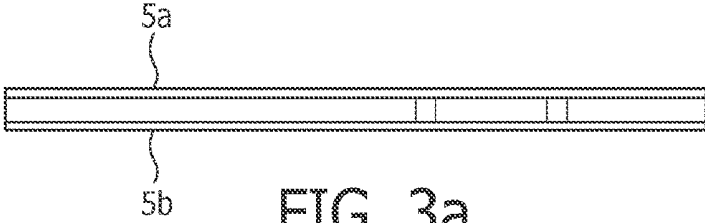


FIG. 3a

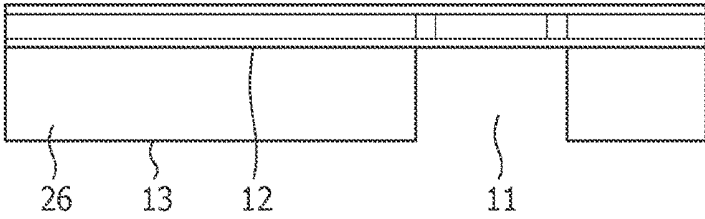


FIG. 3b

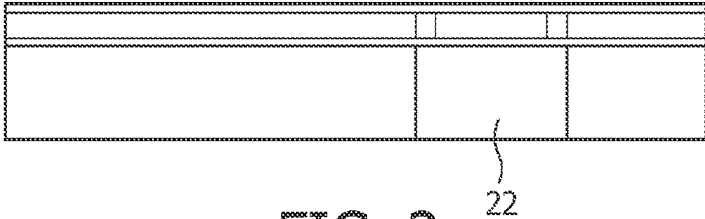


FIG. 3c

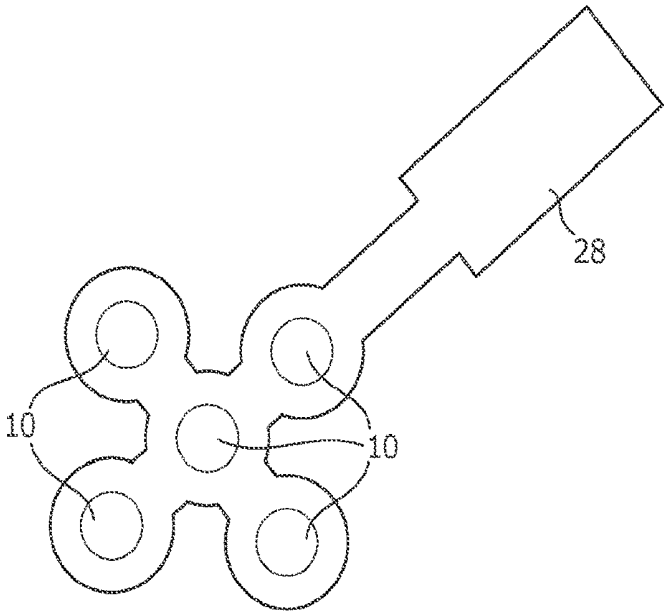


FIG. 5

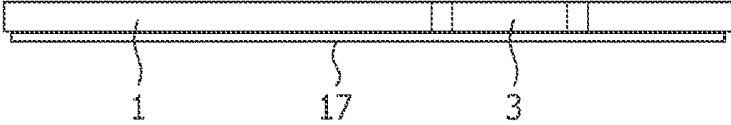


FIG. 4a

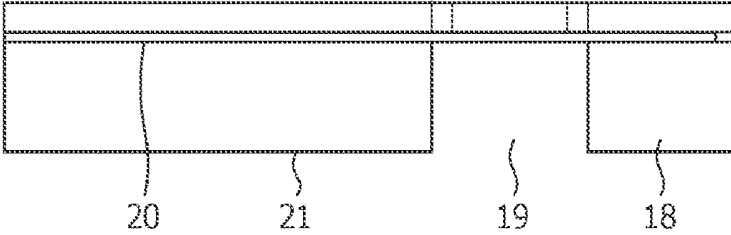


FIG. 4b

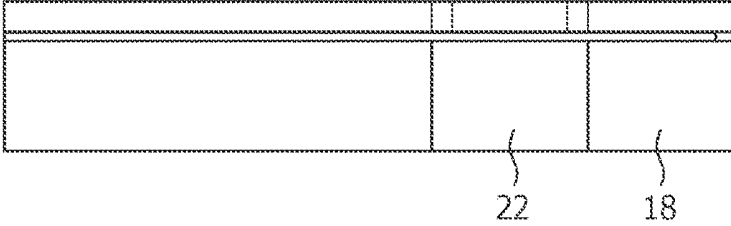


FIG. 4c

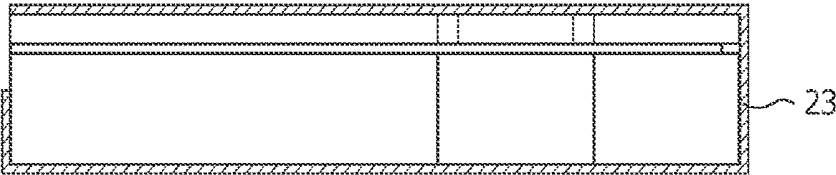


FIG. 4d

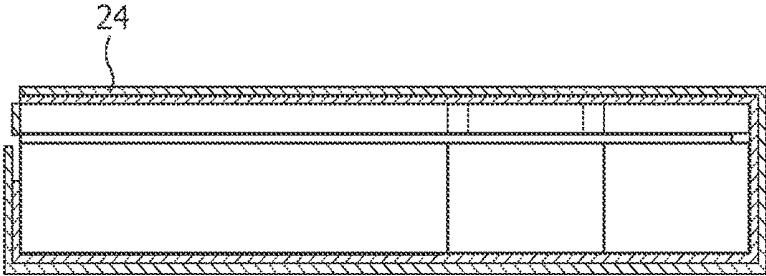


FIG. 4e

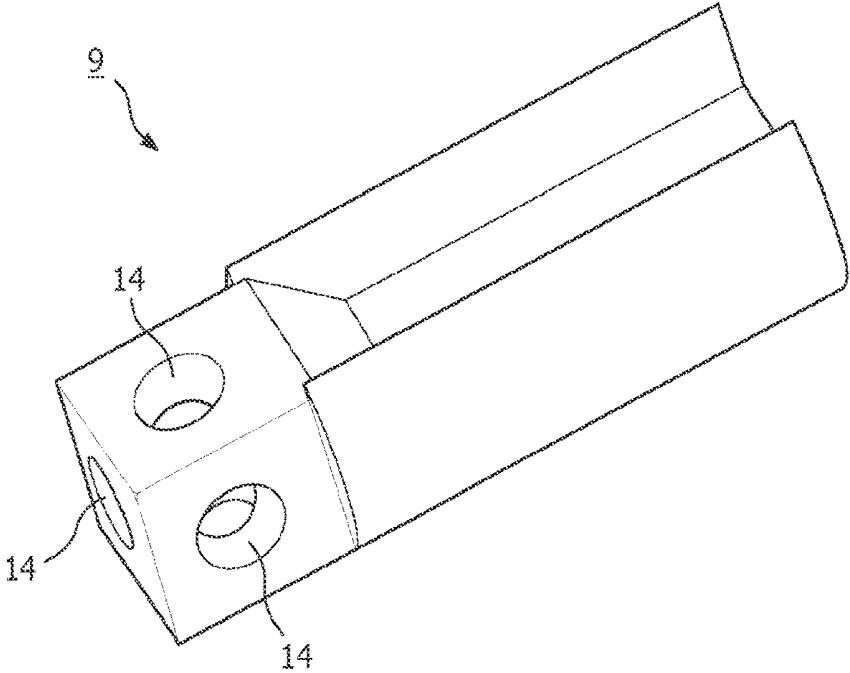


FIG. 6

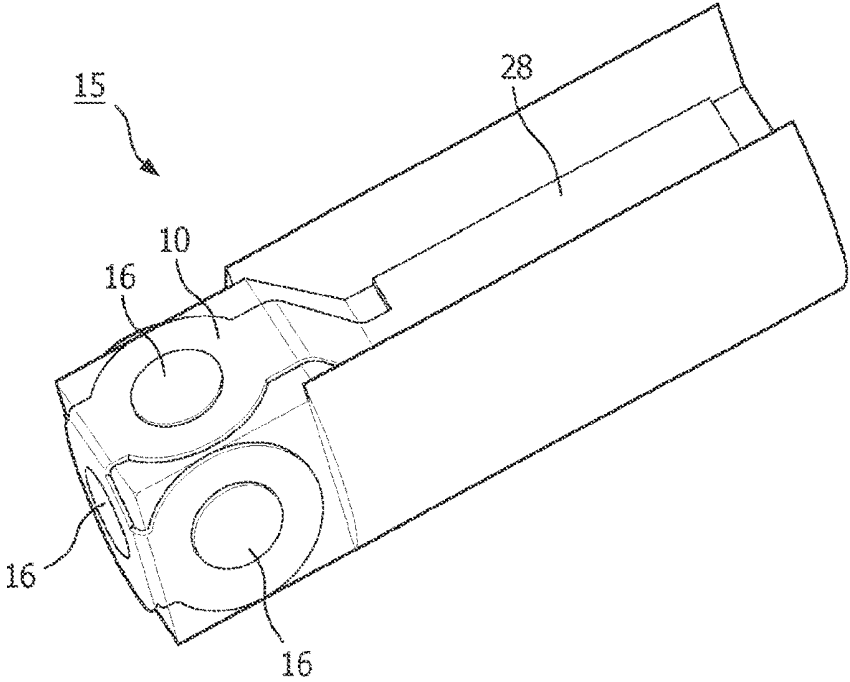


FIG. 7

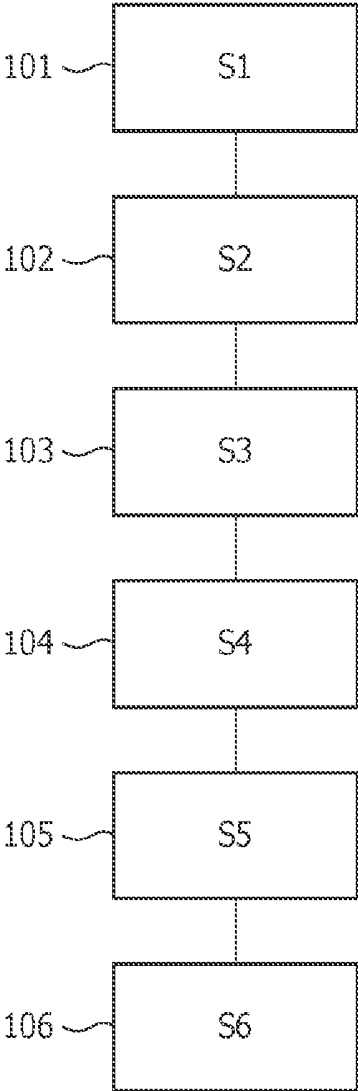


FIG. 8

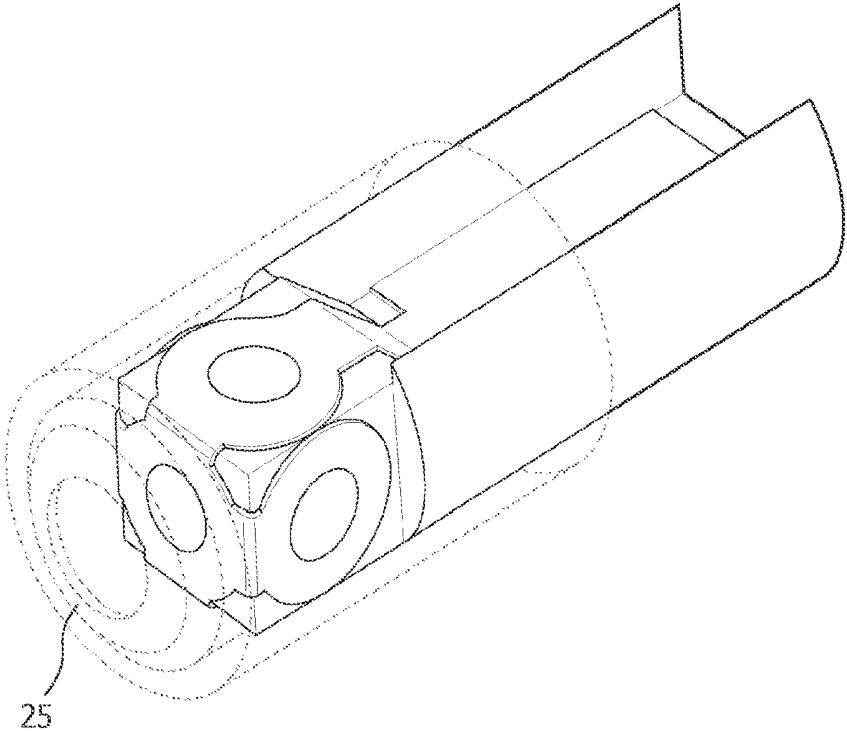


FIG. 9

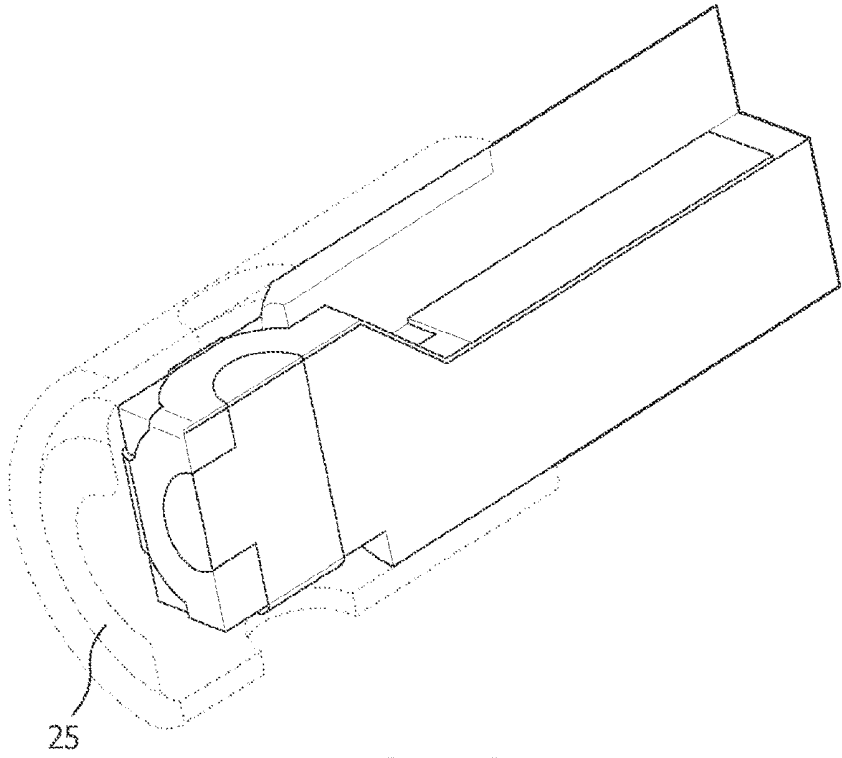


FIG. 10

MEDICAL DEVICE WITH FORWARD AND SIDEWARD ABLATION MONITORING ULTRASOUND TRANSDUCERS

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a divisional of prior application Ser. No. 13/885,796 filed Feb. 4, 2014, entitled “Medical Device with Ultrasound Transducers Embedded in Flexible Foil” which is a national stage entry of PCT/IB11/54330, filed Oct. 3, 2011. These applications claim priority to EP 10191687.2, filed Nov. 18, 2010, which is incorporated by reference herein in its entirety for all purposes.

FIELD OF THE INVENTION

[0002] The invention relates to ultrasound imaging apparatus suitable for minimally invasive ultrasound diagnostic devices. The invention can be used for fabrication of interventional devices used in cardiac ablation monitoring and in cancer ablation monitoring.

BACKGROUND OF THE INVENTION

[0003] Radiofrequency (RF) catheter ablation is an invasive procedure used to remove faulty electrical pathways from patients who are prone to develop cardiac arrhythmias such as atrial fibrillation (AF). In AF ablation procedures, complete electrical isolation of the pulmonary veins is targeted and this is achieved by creating lesion lines with an ablation catheter.

[0004] The majority of the catheter ablation procedures are performed with “single-point ablation catheters”. Lesion lines can be created with such catheters by sequential point by point ablation. To achieve complete electrical isolation of the pulmonary veins lesion lines are created meeting the two requirements of being transmural and continuous.

[0005] A requirement for RF catheters is a more adequate control. A system that can provide a real-time feedback of the lesion development in the tissue, and can provide real-time information about the depth of the lesion with respect to the thickness of the tissue at the treatment site, would prevent injury and potential death from overheating in (RF) catheter ablation procedures, while insufficient heating results in recurrence of arrhythmia. It has been shown that high-frequency ultrasound can be used to monitor the progression of the lesion boundary in M-mode imaging.

[0006] Embedding ultrasound transducers in ablation catheters enables real-time feedback on lesion front progression.

[0007] U.S. Pat. No. 7,846,101 discloses an intravascular ultrasound imaging apparatus comprising a transducer assembly. The assembly includes a flexible circuit comprising transducer elements attached to a flexible substrate. However, as the flexible substrate is part of the material stack forming the assembly, the flexible foil may produce acoustical effect adverse to the transducer elements performance.

[0008] The inventor of the present invention has appreciated that an improved transducer assembly is of benefit, and has in consequence devised the present invention. In particular it would be advantageous to realize a transducer assembly having acoustic properties depending only on the transducer element material. It would also be desirable to

enable the user of RF catheter to access real-time feedback of the lesion development in tissue during RF catheter ablation procedure.

SUMMARY OF THE INVENTION

[0009] In general, the invention preferably seeks to mitigate, alleviate or eliminate one or more of the above mentioned disadvantages singly or in any combination. In particular, it may be seen as an object of the present invention to provide a method that solves the above mentioned problems, or other problems, of the prior art.

[0010] To better address one or more of these concerns, in a first aspect of the invention an ultrasound transducer assembly is presented that comprises a flexible foil having openings extending from a top to a bottom surface of the flexible foil; one or more piezoelectric elements contained into the openings and fastened to the internal rim of the openings; one or more conductive layers deposited on the flexible foil and on the one or more piezoelectric elements.

[0011] By placing piezoelectric elements into the openings of the flexible foil, the properties of piezoelectric elements are not influenced by the material of the flexible foil and therefore desired tuning of the performance of the transducer assembly can be obtained. As the transducer assembly comprises one or more piezoelectric elements embedded into the flexible foil, the flexible foil does not influence the acoustical performance of the transducer. The inside edge, i.e. the internal rim of the opening of the flexible foil is fastened to the piezoelectric element, i.e. the external edge of the piezoelectric element.

[0012] The flexible foil maybe e.g. a Kapton foil, metalized with, e.g. copper, having openings, i.e. holes to contain piezoelectric elements. The piezoelectric elements are, e.g. piezoelectric patches.

[0013] In some embodiments the flexible foil comprises metallization tracks.

[0014] In some embodiments the one or more conductive layers is/are deposited on the top and the bottom surface of the flexible foil and on the top and the bottom surface of the one or more piezoelectric elements.

[0015] In some other embodiments the one or more conductive layers are two layers, the first layer deposited on the top surface of the flexible foil and on the top of the one or more piezoelectric elements and the second layer deposited on the bottom surface of the flexible foil and on the bottom surface of the one or more piezoelectric elements. Through the deposition of these conductive layers, the assembly is provided with a top electrode on the piezoelectric elements, which is connected to the top metallization layer of the flexible foil and a bottom electrode on the piezoelectric element which is connected to the bottom metallization layer of the flexible foil.

[0016] In some other embodiments the one or more conductive layers is one layer deposited on the bottom surface of the flexible foil and on the bottom surface of the one or more piezoelectric elements. This provides great advantages for protection of the electrical signal of the transducer from adverse external perturbations and is useful in the realization of the Faraday cage around the bottom electrode avoiding RF signal interference with ultrasound signal during ablation.

[0017] In a second aspect of the invention an ultrasound transducer system is presented that comprises: an ultrasound transducer assembly according to the first aspect of the

invention placed in a base structure; the base structure comprising cavities, wherein the cavities are filled with backing material; a coating layer deposited on the external surface of the ultrasound transducer assembly.

[0018] In some embodiments at least one of the cavities of the ultrasound transducer system extends from the top to the bottom surface of the base structure. The cavities of the base structure may be considered as apertures in the base structure, providing access to the back side or back surface of the piezoelectric element placed on the base structure. The cavities in the base structure may communicate with each other, e.g. in presence of multiple piezoelectric elements or can be accessed individually.

[0019] The ultrasound transducer assembly placed on the base structure may be glued on and around the base structure. When the ultrasound transducer assembly is placed on the base structure, the empty cavities located at the backside, i.e. at the bottom surface, of the transducer elements are filled with backing material. In this way the performance of the transducer are only dependent on the piezoelectric and the backing materials, and are not influenced by the flexible foil. The flexible foil is not supporting the piezoelectric elements and the piezoelectric elements are embedded into it.

[0020] In placing the ultrasound transducer assembly onto the base structure, the openings of the flexible foil in which the piezoelectric elements are fasten, e.g. by means of glue, are located in positions corresponding to the cavities of the base structure. The back side or bottom surface of the piezoelectric elements is therefore accessible through the cavities of the base structure. The modality of addition of the backing material allows for freedom and good control of the appropriate choice of the material. For example, the filling material can be dispensed into the cavities by injection in a fluidic state through conducts in the base structure. Examples of filling materials comprises adhesive which can rapidly bond to plastics and metal upon exposure to UV and/or visible light. Filling materials compositions may also comprise microspheres, such as ceramic or glass sphere, which can be hollow, lightweight and with a high compressive strength.

[0021] In some other embodiments of the ultrasound transducer assembly according to the first aspect of the invention, the fastening comprises at least a side wall of one or more piezoelectric elements glued to the internal rim of the openings. By gluing only the side or later wall of the piezoelectric elements the piezoelectric elements the acoustic properties of the piezoelectric system are not influenced by the flexible foil.

[0022] The invention is of great advantage in particular in the fabrication of high frequency (HF) transducers. In traditional HF transducers, the flexible foil is included in the transducer stack and the transducer elements are place onto the flexible foil. As the higher the frequency, the lower the thickness of the piezoelectric elements, traditional HF transducers have a high chance of failure due to high risk of breakdown as the electrodes from the front side and the backside of the piezoelectric material are becoming too close with respect to each other. The invention, by embedding the piezoelectric elements into the flexible foil, provides a solution which is therefore particularly advantageous for HF transducers.

[0023] In some embodiments the one or more piezoelectric elements is/are glued with non-conductive glue.

[0024] In some embodiments the one or more piezoelectric elements is/are fastened to the internal rim of the openings by an isolation layer, i.e. a layer having isolating properties.

[0025] In some other embodiments the ultrasound transducer assembly according to the first aspect of the invention further comprises an isolation layer deposited onto the external surface of the ultrasound transducer assembly. This electrical isolation layer may be a matching layer coating the ultrasound transducer assembly for maximizing the acoustic performance of the transducer elements.

[0026] In a third aspect of the invention a catheter tip is presented that comprises an ultrasound transducer assembly according to the first aspect of the invention.

[0027] In a fourth aspect of the invention a catheter tip is presented that comprises an ultrasound transducer system according to the second aspect of the invention.

[0028] The catheter tip may have irrigation holes through which the ultrasound transducer system communicates externally towards the environment, e.g. a pulmonary vein.

[0029] The catheter tip may also have other openings through which the ultrasound transducers system can follow the ablation procedure of tissue unobstructed, e. g. for optical fibers. Alternatively, in case an ultrasound transparent medium is used for ablation e.g. polymethylpentene coated with a thin platinum layer then the tip should not necessarily contain openings.

[0030] When the ultrasound transducers are embedded in ablation catheters for enable real-time feedback on lesion front progression, the ablation cap can be mounted on the catheter body after the ultrasound transducers system is electrically connected and fixed in the catheter tip.

[0031] In a fifth aspect of the invention a method for fabricating an ultrasound transducer assembly is presented that comprises: providing a flexible foil having openings extending from the top to the bottom surface of the flexible foil; mounting one or more piezoelectric elements into the openings; depositing one or more conductive layers on the flexible foil and the one or more piezoelectric elements.

[0032] In some embodiments according to the fifth aspect of the invention the mounting comprises inserting the one or more piezoelectric elements into the openings and gluing said one or more piezoelectric elements to the internal rim of the openings.

[0033] In some embodiments according to the fifth aspect of the invention the depositing comprises depositing one or more conductive layers on the top and bottom surface of the flexible foil and on the top and the bottom surface of the one or more piezoelectric elements.

[0034] In a sixth aspect of the invention a method for fabricating an ultrasound transducer system is presented that comprises: positioning the ultrasound transducer assembly according to the first aspect of the invention onto a base structure, the base structure comprising cavities; filling the cavities with backing material; depositing a coating layer on the external surface of the ultrasound transducer assembly.

[0035] In some embodiments according to this last aspect the positioning comprises folding into a 3D structure the flexible foil containing the one or more piezoelectric elements and gluing the folded flexible foil around the base structure.

[0036] In some embodiments according to this last aspect the filling comprises dispensing backing material in a fluidic state and hardening the backing material.

[0037] In general the various aspects of the invention may be combined and coupled in any way possible within the scope of the invention. These and other aspects, features and/or advantages of the invention will be apparent from and elucidated with reference to the embodiments described hereinafter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0038] Embodiments of the invention will be described, by way of example only, with reference to the drawings.

[0039] FIG. 1 shows a perspective view of a flexible foil with patterned openings according to embodiments of the invention.

[0040] FIG. 2a shows a cross section of the flexible foil as shown in FIG. 1.

[0041] FIG. 2b shows a cross section of the flexible foil including a piezoelectric element according to embodiments of the invention.

[0042] FIG. 2c shows a cross section of the flexible foil including a piezoelectric element glued into the opening of the flexible foil according to embodiments of the invention.

[0043] FIG. 3a shows a cross section of the flexible foil as shown in FIG. 2c where conducting electrodes are deposited.

[0044] FIG. 3b shows a cross section of the flexible foil as shown in FIG. 3a positioned on a base or supporting structure.

[0045] FIG. 3c shows a cross section of the transducer assembly as shown in FIG. 3b where the cavities in the base structure are filled with backing material.

[0046] FIG. 4a shows a cross section of the flexible foil as shown in FIG. 2c where a single conducting electrode is deposited on the back surface of the flexible foil and piezoelectric element.

[0047] FIG. 4b shows a cross section of the flexible foil as shown in FIG. 4a positioned on a base or supporting structure.

[0048] FIG. 4c shows a cross section of the transducer assembly as shown in FIG. 4b where the cavities in the base structure are filled with backing material.

[0049] FIG. 4d shows a cross section of the transducer system as shown in FIG. 4c where a conducting electrode is deposited around the transducer system.

[0050] FIG. 4e shows a cross section of the transducer system as shown in FIG. 4d where a matching or electrical isolation layer is deposited around the transducer system.

[0051] FIG. 5 shows a top view of a patterned flexible foil including transducer elements according to embodiments of the invention.

[0052] FIG. 6 shows a perspective view of a base element according to embodiments of the invention.

[0053] FIG. 7 shows an ultrasound transducer system according to embodiments of the invention.

[0054] FIG. 8 shows the flowchart of a method for fabricating an ultrasound transducer system according to one aspect of the invention.

[0055] FIG. 9 shows a prospective view of an ultrasound transducer system according to embodiments of the invention comprising an ablation cap.

[0056] FIG. 10 shows a cross section view of an ultrasound transducer system according to embodiments of the invention comprising an ablation cap.

DESCRIPTION OF EMBODIMENTS

[0057] FIG. 1 shows three steps of the method for fabricating an ultrasound transducer according to one aspect of the invention. On the flexible foil 1 a desired patterned is produced, e.g. opening 2, extending from the top surface 6 to a bottom surface 7. Piezoelectric elements, e.g. piezoelectric element 3, are located in into the openings, e.g. opening 2 and fastened to the internal rim 8 of opening 2. Non-conductive glue 4 may be used to fasten the piezoelectric element 3 to the internal rim 8 of opening 2.

[0058] FIG. 2a shows a cross section of the flexible foil 1 before including the piezoelectric elements. The opening 2 is filled, as shown in FIG. 2b by a piezoelectric element 3. The mounting of the piezoelectric element 3, e.g. a piezoelectric patch, is achieved by gluing the patches in the designated areas at the rim or edge of the opening 2. In some embodiments the mounting of the piezoelectric element 3 may be achieved by gluing a thin peripheral annular region of the piezoelectric patch 3 on the flexible foil 1.

[0059] FIG. 2b shows the flexible foil 1 with opening 2 where the piezoelectric element 3 is located into the opening 2.

[0060] FIG. 2c shows the transducer assembly of FIG. 2b where the piezoelectric element 3, i.e. the external edge of the piezoelectric element 3, is fastened to the inside edge, i.e. the internal rim of the opening 2 of the flexible foil 1 by means of glue 4. The glue may be non-conductive glue so as to provide isolation of the piezoelectric element 3, e.g. piezoelectric patch from the flexible foil 1.

[0061] FIG. 3a shows the transducer assembly of FIG. 2c after conductive layers 5 are deposited on the flexible foil 1 and on the piezoelectric element 2. In particular conductive layer 5a is deposited on the top surface of the flexible foil 1 and of the piezoelectric element 2 providing the top electrode, while the conductive layer 5b is deposited on the bottom surface of the flexible foil 1 and of the piezoelectric element 2 providing the bottom electrode.

[0062] In FIG. 3b the transducer assembly of FIG. 3a is then placed onto a base structure 6, characterized by cavities 11 extending from the top surface 12 to the bottom surface 13 of the base structure 6. The transducer assembly is filled with backing material 7 as shown in FIG. 3c.

[0063] In some other embodiments one layer is deposited on the bottom surface of the flexible foil and on the bottom surface of the one or more piezoelectric element. FIG. 4a shows a cross section of the flexible foil as shown in FIG. 2c where a single conducting layer 17 is deposited on the back surface of the flexible foil 1 and piezoelectric element 3. The transducer assembly of FIG. 4a is then placed onto a base structure 18, characterized by cavities 19 extending from the top surface 20 to the bottom surface 21 of the base structure 18 as shown in FIG. 4b.

[0064] The transducer assembly placed on the base structure 18 is filled with backing material 22 as shown in FIG. 4c.

[0065] In FIG. 4d a coating layer 23 is deposited at least partially around the transducer system as shown in FIG. 4c. The transducer system as shown in FIG. 4d can be further coated by a matching or electrical isolation layer 24 deposited around the transducer system.

[0066] The embodiment shown in FIG. 4 is an alternative to the embodiments shown in FIG. 3 and provides great advantages for electrical signal isolation purposes.

[0067] FIG. 5 shows a top view of a patterned flexible foil including transducer elements according to an embodiment of the invention. The flexible foil 28 is patterned so as to have a cross-shape having five openings 10 in which piezoelectric elements 16 are going to be introduced. Shape and number of openings depend on the base structure to be used and on the number of piezoelectric elements to be fastened. This is within the knowledge of the person skilled in the art. The flexible foil 28 is designed so as to be folded in a three-dimensional structure with matches, e.g. in one embodiment the shape of the base structure 9 having cavities 14 as shown in FIG. 6. By folding and gluing the ultrasound transducer assembly onto the base structure the ultrasound transducer system 15 is produced as shown in FIG. 7. The piezoelectric elements 16 fastened into the openings 10 of the flexible foil 28 are positioned so as to face the cavities 14 of the base structure 9. The cavities 14 are then filled with backing materials. The filling may be achieved through injection of backing material in fluidic state followed by hardening. Hardening may be achieved e.g. by curing in air, through exposure to high temperature, exposure to UV light or through the use of chemicals, such as chemical catalyst. In case of hardening with UV exposure, the base structure 9 is made of UV transparent material.

[0068] A further coating layer is deposited on the external surface of the ultrasound transducer assembly 15 so as to provide electrical isolation from external disturbance, e.g. RF ablation.

[0069] In cardiac ablation monitoring, the ultrasound transducer system can be connected and fixed in a catheter tip of a catheter allowing for forward and sideward monitoring during ablation. After the ultrasound transducer system is electrically connected and fixed in the catheter tip, the ablation cap, e.g. a platinum ablation cap 25 as shown in FIGS. 9 and 10, can be mounted on the catheter body. The ablation tip may have apertures through which the ultrasound transducer system can follow the ablation procedure. Alternatively a material, such as polymethylpentene coated with thin platinum layer, which is transparent to ultrasound may be used. This avoids the need of apertures in the ablation tip.

[0070] FIG. 8 shows the flowchart of a method for fabricating an ultrasound transducer system according to one aspect of the invention.

[0071] In step (S1) 101, a flexible foil having openings extending from the top to the bottom surface is provided. The flexible foil may have metallization, e.g. copper) on front and backsides or alternatively has patterned metallization tracks on one of the sides for the front and backside of the piezoelectric material, e.g. PZT.

[0072] In step (S2) 102, one or more piezoelectric elements is/are mounted into the flexible foil openings. Mounting comprises inserting the one or more piezoelectric elements into the openings of the flexible foil and fastening, e.g. by gluing the one or more piezoelectric elements to the internal rim of the openings of the flexible foil.

[0073] In step (S3) 103, one or more conductive layers is/are deposited on the flexible foil and on the one or more piezoelectric elements. Depositing comprises depositing one or more conductive layers on the top and/or bottom surface of the flexible foil and on the top and/or the bottom surface of the one or more piezoelectric elements.

[0074] In step (S4) 104, the ultrasound transducer assembly produced in the first three steps is positioned onto a base structure which comprises cavities. Positioning the ultra-

sound transducer assembly on the base structure comprises folding into a 3D structure the flexible foil containing the one or more piezoelectric elements and gluing the folded flexible foil around the base structure.

[0075] In step (S5) 105, the cavities of the base structure are filled with backing material. The filling comprises dispensing backing material in a fluidic state and hardening the backing material. In step (S6) 106, a coating layer is deposited on the external surface of the ultrasound transducer assembly.

[0076] While the invention has been illustrated and described in detail in the drawings and foregoing description, such illustration and description are to be considered illustrative or exemplary and not restrictive; the invention is not limited to the disclosed embodiments. Other variations to the disclosed embodiments can be understood and effected by those skilled in the art in practicing the claimed invention, from a study of the drawings, the disclosure, and the appended claims. In the claims, the word "comprising" does not exclude other elements or steps, and the indefinite article "a" or "an" does not exclude a plurality. A single processor or other unit may fulfill the functions of several items recited in the claims. The mere fact that certain measures are recited in mutually different dependent claims does not indicate that a combination of these measures cannot be used to advantage. A computer program may be stored/distributed on a suitable medium, such as an optical storage medium or a solid-state medium supplied together with or as part of other hardware, but may also be distributed in other forms, such as via the Internet or other wired or wireless telecommunication systems. Any reference signs in the claims should not be construed as limiting the scope.

1-15. (canceled)

16. A combined ablation and ultrasound imaging catheter for insertion within a body, the catheter having a catheter tip comprising:

- an ablation cap having a distal-facing aperture and a plurality of lateral-facing apertures formed through the ablation cap, wherein the plurality of lateral-facing apertures are located proximal of the distal facing aperture, and are arrayed around a circumference of the ablation cap;

- an ultrasound transducer system fixed within the ablation cap and having:

- a first ultrasound transducer element configured to follow an ablation procedure in a first direction through the distal-facing aperture of the ablation cap, the first direction orientated primarily distally away from the catheter tip;

- a plurality of second ultrasound transducer elements located proximal to the first ultrasound transducer element, the plurality of second ultrasound transducer elements arrayed about the circumference of the ablation cap and configured to follow the ablation procedure through the plurality of lateral-facing apertures of the ablation cap in a plurality of second directions, respectively, the plurality of second directions orientated laterally away from the catheter tip and different from the first direction.

17. The catheter of claim 16, wherein the ablation electrode comprises an RF ablation electrode.

18. The catheter of claim 16, wherein the first and second ultrasound transducer elements are mounted on a base structure and are entirely within the ablation cap.

19. The catheter of claim 16, wherein the plurality of apertures are evenly spaced about the circumference of the ablation cap.

20. The catheter of claim 16, wherein each of the second ultrasound transducer elements are located along a curved portion of the ablation cap.

21. The catheter of claim 16, wherein the plurality of second ultrasound transducer elements are four ultrasound elements evenly arrayed at angles of 90° about the circumference of the ablation cap.

22. The catheter of claim 16, wherein the ablation cap is a platinum ablation cap.

23. The catheter of claim 16, wherein the ablation cap is a cylindrical shell.

24. The catheter of claim 16, wherein the ultrasound transducer system comprises:

a flexible foil having openings extending from the top to the bottom surface of said flexible foil;

the first ultrasound transducer element contained into a first opening of said openings and fastened to the internal rim of said first opening;

the plurality of second ultrasound transducer elements contained into the remaining openings and fastened to the internal rim of said remaining openings;

a base structure comprising cavities, wherein said cavities are filled with backing material.

25. A method of manufacturing a combined ablation and ultrasound imaging catheter for insertion within a body, comprising:

providing an ultrasound transducer system having a base structure and comprising a first ultrasound transducer element located distal on the base structure and a plurality of second ultrasound transducer elements located sideward on the base structure;

providing an ablation cap having a distal-facing aperture formed through the ablation cap and a plurality of lateral-facing apertures formed through the ablation cap and located proximal of the distal facing aperture, the plurality of lateral-facing apertures arrayed around a circumference of the ablation cap;

fixing the ultrasound transducer system within the ablation cap, so that a catheter tip is formed, in which the first ultrasound transducer element is capable of following an ablation procedure in a first direction through

the distal-facing aperture of the ablation cap, and the plurality of second ultrasound transducer elements are capable of following the ablation procedure through the plurality of lateral-facing apertures of the ablation cap in a plurality of second directions, respectively, the plurality of second directions orientated laterally away from the catheter tip and different from the first direction.

26. An ablation catheter comprising:

a ultrasound transducer assembly placed in a base structure, and

a catheter having a catheter tip,

wherein the base structure comprises two or more openings containing ultrasound transducers,

wherein ultrasound transducers of at least one of the openings face an end of the base structure and ultrasound transducers of at least a second opening of the base structure face outward from a length of the base structure, and

wherein the ultrasound transducer assembly is connected and fixed in the catheter tip.

27. The ablation catheter of claim 26 further comprising an ablation cap mounted on the catheter.

28. The ablation catheter of claim 27, wherein the ablation cap comprises a material transparent to ultrasound.

29. The ablation catheter of claim 27, wherein the ablation cap comprises platinum.

30. The ablation catheter of claim 27 wherein the ablation cap comprises apertures aligned with the ultrasound transducers.

31. The ablation catheter of claim 26 wherein the catheter tip comprises a material that is transparent to ultrasound.

32. The ablation catheter of claim 26 wherein the ultrasound transducers comprise piezoelectric elements.

33. A catheter tip comprising an ultrasound transducer assembly placed in a base structure, wherein the base structure comprises two or more openings containing ultrasound transducers, and

wherein ultrasound transducers of at least one of the openings face an end of the base structure and ultrasound transducers of at least a second opening of the base structure face outward from a length of the base structure.

* * * * *

专利名称(译)	具有前向和侧向消融监测超声换能器的医疗装置		
公开(公告)号	US20190015072A1	公开(公告)日	2019-01-17
申请号	US16/129837	申请日	2018-09-13
[标]申请(专利权)人(译)	皇家飞利浦电子股份有限公司		
申请(专利权)人(译)	皇家飞利浦N.V.		
当前申请(专利权)人(译)	皇家飞利浦N.V.		
[标]发明人	DELADI SZABOLCS VAN DER VLEUTEN CORNELIUS ANTONIUS NICOLAAS MARIA RADEMAKERS ANTONIUS JOHANNES JOSEPHUS		
发明人	DELADI, SZABOLCS VAN DER VLEUTEN, CORNELIUS ANTONIUS NICOLAAS MARIA RADEMAKERS, ANTONIUS JOHANNES JOSEPHUS		
IPC分类号	A61B8/00 A61B8/12 A61B34/20 A61B8/08 B06B1/06 A61B18/00 A61B18/14 A61B90/00 G01S15/46		
CPC分类号	A61B34/20 A61B2034/2051 A61B2090/364 A61B2090/3782 A61B2034/2063 G01S2015/465 B06B1/0629 A61B2018/00839 A61B2018/00738 A61B18/1492 A61B8/4483 A61B8/445 A61B8/12 A61B8/0883 Y10T29/42		
优先权	2010191687 2010-11-18 EP 13/885796 2014-02-04 US PCT/IB2011/054330 2011-10-03 WO		
外部链接	Espacenet USPTO		

摘要(译)

本发明涉及适用于心脏消融监测和肿瘤消融监测中的微创超声诊断装置的超声成像方法和装置。本发明提出了一种前向和侧向换能器的组件以及在组件表面上的孔中嵌入的前向和侧向换能器的系统。当组件结合在医疗装置中时，这提供了对换能器的声学特性的控制和改进的消融监测。

