

(19)



(11)

EP 1 887 961 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
11.01.2012 Bulletin 2012/02

(51) Int Cl.:
A61B 19/00 (2006.01) A61B 8/00 (2006.01)

(21) Application number: **06784595.8**

(86) International application number:
PCT/US2006/021852

(22) Date of filing: **05.06.2006**

(87) International publication number:
WO 2007/030173 (15.03.2007 Gazette 2007/11)

(54) LAPAROSCOPIC ULTRASOUND ROBOTIC SURGICAL SYSTEM

LAPAROSKOPISCHES ULTRASCHALL-ROBOTERSYSTEM FÜR CHIRURGISCHE ZWECKE
SYSTÈME CHIRURGICAL ROBOTIQUE ULTRASONORE LAPAROSCOPIQUE

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI
SK TR**

(30) Priority: **06.06.2005 US 688013 P**

(43) Date of publication of application:
20.02.2008 Bulletin 2008/08

(60) Divisional application:
**11150207.6 / 2 289 452
11150208.4 / 2 289 453
11150209.2 / 2 289 454**

(73) Proprietor: **Intuitive Surgical Operations, Inc.
Sunnyvale, CA 94086 (US)**

(72) Inventors:
• **HASSER, Christopher
Sunnyvale, CA 94086 (US)**
• **TAYLOR, Russell
Baltimore, MD 21218 (US)**
• **CHOTI, Michael
Baltimore, MD 21218 (US)**
• **LEVEN, Josh
Baltimore, MD 21218 (US)**

(74) Representative: **MacDougall, Alan John Shaw et al
Mathys & Squire LLP
120 Holborn
London
EC1N 2SQ (GB)**

(56) References cited:
**US-A1- 2003 013 949 US-A1- 2003 220 541
US-B1- 6 425 865**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 887 961 B1

Description**FIELD OF THE INVENTION**

[0001] The present invention generally relates to robotic surgical systems and in particular, to a laparoscopic ultrasound robotic surgical system useful for performing minimally invasive surgical procedures.

BACKGROUND OF THE INVENTION

[0002] Minimally invasive surgery offers many benefits over traditional open surgery techniques, including less pain, shorter hospital stays, quicker return to normal activities, minimal scarring, reduced recovery time, and less injury to tissue. Consequently, demand for minimally invasive surgery using robotic surgical systems is strong and growing.

[0003] Laparoscopy is a type of minimally invasive surgery in which a small incision is made in the abdominal wall through which an instrument called a laparoscope is inserted to permit anatomic structures within the abdomen and pelvis to be seen. The abdominal cavity is commonly distended and made visible by the instillation of absorbable gas such as carbon dioxide. Tubes may be pushed through the same or different incisions in the skin so that probes or other instruments can be introduced to a surgical site. In this way, a number of surgical procedures can be performed without the need for a large or open cavity surgical incision.

[0004] One disadvantage of laparoscopy, however, is the inability to manually palpate hidden or solid organs. Laparoscopic Ultrasound ("LUS") allows the surgeon to overcome this limitation by providing visualization of deeper structures. In fact, even when open cavity operations are performed, intraoperative ultrasonography may be significantly more sensitive at detecting otherwise occult lesions within anatomic structures than bimanual palpation.

[0005] As an example, intraoperative ultrasonography of the liver is useful in a variety of clinical settings during laparoscopic surgery. These include: staging and assessment of the liver, including ultrasound-guided needle biopsy, liver tumor ablation, and evaluation of the liver prior to laparoscopic liver resection.

[0006] For resection procedures, surgeons should have the ability to perform accurate staging of the liver and other sites to rule out metastatic disease prior to resection. The addition of LUS to standard laparoscopy improves the diagnosis of metastases over conventional preoperative diagnostic methods.

[0007] Ultrasound-directed liver biopsy is an important component of hepatic staging and assessment. When a lesion is identified by ultrasound, needle biopsy is necessary to confirm the findings histologically. Current practice requires manual free-hand LUS in conjunction with free-hand positioning of the biopsy needle under ultrasound guidance.

[0008] For the treatment of unresectable metastases, increasing interest has been focused on ablative approaches such as radiofrequency ("RF"), cryotherapy, microwave, or chemical ablation. While interstitial ablation can be performed percutaneously or during open surgery, laparoscopic ablation has significant advantages. First, unlike percutaneous therapy, laparoscopy can identify both hepatic and extrahepatic metastases not visualized on preoperative imaging, which misses significant tumors in about 10% to 20% of patients with colorectal liver metastases. Second, laparoscopic or operative ultrasound ("US") has been shown to be significantly more accurate than transabdominal US, CT or MR at visualizing liver lesions. Further, operative approaches, including laparoscopy, permit mobilization of structures away from a surface tumor that may be thermally injured during RF ablation. Percutaneous ablation and laparoscopic ablation both typically require general anesthesia and an overnight hospital stay. Laparoscopy, on the other hand, does not impose a significantly greater burden on the patient.

[0009] While ablation promises advantages compared to other approaches, the technical difficulty of manipulating the ultrasound probe, aligning the ultrasound probe with the ablation probe, and placement of the ablation probe demands considerable expertise. The surgeon must precisely place the ablation probe tip within the volumetric center of the tumor in order to achieve adequate destruction of the tumor and a 1 cm zone of surrounding normal parenchyma. Tumors are identified by preoperative imaging, primarily CT and MR, and then laparoscopically localized by LUS.

[0010] One major limitation of ablative approaches is the lack of accuracy in probe tip placement within the center of the tumor. This is particularly important, as histologic margins cannot be assessed after ablation as is done with hepatic resection. In addition, manual guidance often requires multiple passes and repositioning of the probe tip, further increasing the risk of bleeding and tumor dissemination. Intraoperative ultrasound provides excellent visualization of tumors and provides guidance for RF probe placement, but its 2D-nature and dependence on the sonographer's skill limit its effectiveness.

[0011] Although laparoscopic instrumentation and techniques are beginning to be extended to resection of the liver, loss of the surgeon's tactile sense makes it difficult to assess the safe margins of resection necessary for safe parenchymal transection. Lack of clear visualization and mapping of intrahepatic structures with current LUS techniques could result in catastrophic injury to major adjacent structures. The surgeon must carefully examine the liver by ultrasound prior to resection in order to rule out additional tumors which may preclude curative therapy. Surgeons also require ultrasound to determine and plan safe and complete resection with sufficient surgical margin clearance.

[0012] Despite its theoretical advantages, intraoperative LUS is not widely practiced for such uses as laparoscopic liver cancer surgery. To expand usage in this and other applications, advances in LUS robotic surgical systems that improve surgeon efficiency in performing minimally invasive surgical procedures, as well as the ease of using those systems is desirable.

[0013] For example, optimization of LUS for hepatic surgery may significantly improve the clinical management of patients. In addition to minimizing morbidity and discomfort, an improved LUS robotic surgical system may significantly reduce costs. Faster, more accurate, and more complete assessment of the liver may be performed by experts, as well as potentially by surgeons who are not experts in intraoperative ultrasonography of the liver.

[0014] Image-guided biopsy of sometimes small and inaccessible liver lesions may be facilitated. Advanced LUS robotic tools could increase the use of resection as a definitive treatment for larger and less favorably placed tumors. Improved real-time guidance for planning, delivery and monitoring of ablative therapy may also provide the missing tool needed to allow accurate and effective application of this promising therapy.

[0015] US 2003/0220541 describes a robotically surgical system in which an ultrasound probe may be attached to a robotic arm and swept across a surgical site to capture cuts for three-dimensional rendering in response to either operator movement of a master control device or a pre-programmed sequence in a computer program.

SUMMARY OF THE INVENTION

[0016] According to an aspect of the present invention, there is provided a laparoscopic ultrasound robotic surgical system comprising: a first robotic arm mechanically coupled to an ultrasound probe; a second robotic arm mechanically coupled to a surgery related device; a master manipulator; a control switch having user selectable first and second modes; and a processor configured to cause the second robotic arm to be locked in position and the first robotic arm to move the ultrasound probe according to user manipulation of the master manipulator when the control switch is in the first mode, and to cause the second robotic arm to manipulate the surgery related device according to manipulation of the master manipulator and the first robotic arm to move the ultrasound probe according to stored instructions upon detection of a user command associated with the stored instructions when the control switch is in the second mode.

[0017] Additional features and advantages of the various aspects of the present invention will become apparent from the following description of its preferred embodiment, which description should be taken in conjunction with the accompanying drawings

[0018] BRIEF DESCRIPTION OF THE DRAWINGS

[0019] FIG. 1 illustrates a top view of an operating room employing a laparoscopic ultrasound robotic surgical system utilizing aspects of the present invention.

[0020] FIG. 2 illustrates a block diagram of a laparoscopic ultrasound robotic surgical system utilizing aspects of the present invention.

[0021] FIG. 3 illustrates a laparoscopic ultrasound probe utilizing aspects of the present invention.

[0022] FIG. 4 illustrates a flow diagram of a method for training a LUS robotic surgical system to robotically move a LUS probe in a trained manner upon command, utilizing aspects of the present invention.

[0023] FIG. 5 illustrates a flow diagram of a method for generating a clickable thumbnail image that allows a user to command that a LUS probe be automatically moved to a position and orientation from which the image was captured, utilizing aspects of the present invention.

[0024] FIG. 6 illustrates a flow diagram of a method for automatically moving a LUS probe to a position and orientation associated with a clickable thumbnail image, utilizing aspects of the present invention.

[0025] FIG. 7 illustrates a flow diagram of a method for robotically assisted needle guidance to a marked lesion of a cancerous structure, utilizing aspects of the present invention.

[0026] FIG. 8 illustrates a perspective view of a 3D ultrasound image of an anatomic structure in a camera reference frame with selectable 2D image slices as used in a medical robotic system utilizing aspects of the present invention.

[0027] FIG. 9 illustrates a perspective view of a 3D camera view of an anatomic structure in a camera reference frame as used in a medical robotic system utilizing aspects of the present invention.

[0028] FIG. 10 illustrates a perspective view of a frontal 2D slice of a 3D ultrasound view of an anatomic structure that overlays a 3D camera view of the anatomic structure, as displayable in a medical robotic system utilizing aspects of the present invention.

[0029] FIG. 11 illustrates a perspective view of an inner 2D slice of a 3D ultrasound view of an anatomic structure that overlays a 3D camera view of the anatomic structure, as displayable in a medical robotic system utilizing aspects of the present invention.

[0030] DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0031] FIG. 1 illustrates, as an example, a top view of an operating room employing a robotic surgical system. The robotic surgical system in this case is a Laparoscopic Ultrasound Robotic Surgical System 100 including a Console ("C") utilized by a Surgeon ("S") while performing a minimally invasive diagnostic or surgical procedure with assistance from

one or more Assistants ("A") on a Patient ("P") who is reclining on an Operating table ("O").

[0032] The Console includes a Master Display **104** (also referred to herein as a "Display Screen") for displaying one or more images of a surgical site within the Patient as well as perhaps other information to the Surgeon. Also included are Master Input Devices **107** and **108** (also referred to herein as "Master Manipulators"), one or more Foot Pedals **105** and **106**, a Microphone **103** for receiving voice commands from the Surgeon, and a Processor **102**. The Master Input Devices **107** and **108** may include any one or more of a variety of input devices such as joysticks, gloves, trigger-guns, hand-operated controllers, or the like. The Processor **102** is preferably a personal computer that may be integrated into the Console or otherwise connected to it in a conventional manner.

[0033] The Surgeon performs a minimally invasive surgical procedure by manipulating the Master Input Devices **107** and **108** so that the Processor **102** causes their respectively associated Slave Arms **128** and **129** (also referred to herein as "Slave Manipulators") to manipulate their respective removably coupled and held Surgical Instruments **138** and **139** (also referred to herein as "Tools") accordingly, while the Surgeon views three-dimensional ("3D") images of the surgical site on the Master Display **104**.

[0034] The Tools **138** and **139** are preferably Intuitive Surgical's proprietary EndoWrist™ articulating instruments, which are modeled after the human wrist so that when added to the motions of the robot arm holding the tool, they allow a full six degrees of freedom of motion, which is comparable to the natural motions of open surgery. Additional details on such tools may be found in commonly owned U.S. Pat. No. 5,797,900 entitled "Wrist Mechanism for Surgical Instrument for Performing Minimally Invasive Surgery with Enhanced Dexterity and Sensitivity,". At the operating end of each of the Tools **138** and **139** is a manipulatable end effector such as a clamp, grasper, scissor, stapler, blade, needle, or needle holder.

[0035] The Master Display **104** has a high-resolution stereoscopic video display with two progressive scan cathode ray tubes ("CRTs"). The system offers higher fidelity than polarization, shutter eyeglass, or other techniques. Each eye views a separate CRT presenting the left or right eye perspective, through an objective lens and a series of mirrors. The Surgeon sits comfortably and looks into this display throughout surgery, making it an ideal place for the Surgeon to display and manipulate 3-D intraoperative imagery.

[0036] A Stereoscopic Endoscope **140** (also referred to as a "Laparoscope") provides right and left camera views to the Processor **102** so that it may process the information according to programmed instructions and cause it to be displayed on the Master Display **104**. A Laparoscopic Ultrasound ("LUS") Probe **150** provides two-dimensional ("2D") ultrasound image slices of an anatomic structure to the Processor **102** so that the Processor **102** may generate a 3D ultrasound computer model of the anatomic structure and cause the 3D computer model (or alternatively, 2D "cuts" of it) to be displayed on the Master Display **104** as an overlay to the endoscope derived 3D images or within a Picture-in-Picture ("PIP") in either 2D or 3D and from various angles and/or perspectives according to Surgeon or stored program instructions.

[0037] Each of the Tools **138** and **139**, as well as the Endoscope **140** and LUS Probe **150**, is preferably inserted through a cannula or trocar (not shown) or other tool guide into the Patient so as to extend down to the surgical site through a corresponding minimally invasive incision such as Incision **166**. Each of the Slave Arms **121-124** is conventionally formed of linkages which are coupled together and manipulated through motor controlled joints (also referred to as "active joints"). Setup Arms (not shown) comprising linkages and setup joints are used to position the Slave Arms **121-124** vertically and horizontally so that their respective surgical related instruments may be coupled for insertion into the cannulae.

[0038] The number of surgical tools used at one time and consequently, the number of slave arms being used in the System **100** will generally depend on the diagnostic or surgical procedure and the space constraints within the operating room, among other factors. If it is necessary to change one or more of the tools being used during a procedure, the Assistant may remove the tool no longer being used from its slave arm, and replace it with another tool, such as Tool **131**, from a Tray ("T") in the Operating Room.

[0039] Preferably, the Master Display **104** is positioned near the Surgeon's hands so that it will display a projected image that is oriented so that the Surgeon feels that he or she is actually looking directly down onto the surgical site. To that end, an image of the Tools **138** and **139** preferably appear to be located substantially where the Surgeon's hands are located even though the observation points (i.e., that of the Endoscope **140** and LUS Probe **150**) may not be from the point of view of the image.

[0040] In addition, the real-time image is preferably projected into a perspective image such that the Surgeon can manipulate the end effector of a Tool, **138** or **139**, through its associated Master Input Device, **107** or **108**, as if viewing the workspace in substantially true presence. By true presence, it is meant that the presentation of an image is a true perspective image simulating the viewpoint of an operator that is physically manipulating the Tools. Thus, the Processor **102** transforms the coordinates of the Tools to a perceived position so that the perspective image is the image that one would see if the Endoscope **140** was looking directly at the Tools from a Surgeon's eye-level during an open cavity procedure.

[0041] The Processor **102** performs various functions in the System **100**. One important function that it performs is

to translate and transfer the mechanical motion of Master Input Devices **107** and **108** to their associated Slave Arms **121** and **122** through control signals over Bus **110** so that the Surgeon can effectively manipulate their respective Tools **138** and **139**. Another important function is to implement the various methods described herein providing a robotic assisted LUS capability.

[0042] Although described as a processor, it is to be appreciated that the Processor **102** may be implemented in practice by any combination of hardware, software and firmware. Also, its functions as described herein may be performed by one unit, or divided up among different components, each of which may be implemented in turn by any combination of hardware, software and firmware.

[0043] Prior to performing a minimally invasive surgical procedure, ultrasound images captured by the LUS Probe **150**, right and left 2D camera images captured by the stereoscopic Endoscope **140**, and end effector positions and orientations as determined using kinematics of the Slave Arms **121-124** and their sensed joint positions, are calibrated and registered with each other.

[0044] In order to associate the ultrasound image with the rest of the surgical environment, both need to be expressed in the same coordinate frame. Typically, the LUS Probe **150** is either labeled with markers and tracked by a tracking device such as the Optotrak® position sensing system manufactured by Northern Digital Inc. of Ontario, Canada, or held by a robot with precise joint encoders. Then the rigid transformation between the ultrasound image and the frame being tracked is determined (which is typically referred to as the ultrasound calibration).

[0045] For example, using the Optotrak® frame for the ultrasound calibration, the ultrasound image generated by the LUS Probe **150** is calibrated to an Optotrak® rigid body using an $AX=XB$ formulation. " $AX=XB$ " is a rubric for a class of calibration/registration problem commonly encountered in computer vision, surgical navigation, medical imaging, and robotics. The mathematical techniques are well known. See, e.g., E. Boctor, A. Viswanathan, M. Chioti, R. Taylor, G. Fichtinger, and G. Hager, "A Novel Closed Form Solution for Ultrasound Calibration," International Symposium on Biomedical Imaging, Arlington, VA, 2004, pp. 527-530.

[0046] "A" and "B" in this case, are transformations between poses of the Optotrak® rigid body (A) and the ultrasound image (B). Thus, "X" is the transformation from the ultrasound image to the rigid body.

[0047] To perform the ultrasound calibration, the LUS Probe **150** may be placed in three known orientations defined by the $AX=XB$ calibration phantom. The ultrasound image frame may then be defined by three fiducials which appear in each of the three poses. The three poses allow three relative transformations based on Optotrak® readings (A) and three relative transformations based on the ultrasound images (B) for the $AX=XB$ registration.

[0048] Camera calibration is a common procedure in computer vision applications. As an example, in order to determine the intrinsic and extrinsic parameters of the Endoscope **140**, a checkerboard phantom with a multi-plane formulation provided by the Caltech Camera Calibration Toolbox may be used. To construct the phantom, Optotrak® markers are added to a typical checkerboard video calibration phantom, and each corner of the checkerboard is digitized using a calibrated Optotrak® pointer. Thus, the corner positions may be reported with respect to the Optotrak®.

[0049] The calibration may then be performed by placing the phantom in view of the Endoscope **140** in several dozen orientations, and recording both stereo image data and Optotrak® readings of the four checkerboard corners. The images may then be fed into the calibration toolbox, which determines the intrinsic and extrinsic camera parameters, as well as the 3D coordinates of the grid corners in the camera frame. These coordinates may then be used with the Optotrak® readings to perform a point-cloud to point-cloud registration between the Endoscope **140** rigid body and camera frame.

[0050] The Controller **102** is configured to use the robot kinematics to report a coordinate frame for the LUS Probe **150** tip relative to the Endoscope **140**. However, due to inaccuracies in the setup joint encoders, both of these coordinate frames may be offset from their correct values. Thus, it may be necessary to register the offsets between the real camera frame of the Endoscope **140** and the camera frame calculated from the kinematics as well as between the real and kinematic LUS Probe **150** frames. With this complete, the kinematics may be used in place of the Optotrak® readings to determine ultrasound image overlay placement.

[0051] As long as the position of the Endoscope **140** doesn't overly change, a constant transformation may be assumed between the kinematic tool tip and the laparoscopic Optotrak® rigid body. Using an $AX=XB$ formulation, the LUS Probe **150** may be moved, for example, to several positions, and the static offset between the tool tip and Optotrak® rigid body registered. Knowing this offset, the Endoscope **140** offset may be calculated directly:

$$C_{CD} = D_{LusD} (C_{LusUrb})^{-1} T_{OUrb} (T_{OErb})^{-1} F_{CErb} \quad (1)$$

[0052] where C_{CD} is the camera offset from the real Endoscope **140** (also referred to herein simply as the "camera") frame to the camera frame calculated from the kinematics, F_{CErb} is the transformation from the camera to the endoscope rigid body, $T_{ourb} \cdot (T_{OErb})^{-1}$ is the transformation from the camera rigid body to the LUS rigid body, C_{LusUrb} is the

transformation from the LUS rigid body to the kinematic ultrasound tool tip, and D_{LUSD} is the reading from the Controller **102** giving the transformation from the kinematic ultrasound tool tip to a fixed reference point associated with the Slave Arms **121-124**.

[0053] However, the aforescribed registration should be redone each time the camera is moved, thus making it best suited for pre-operative calibration and registration. For intra-operative, the registration may be better performed using video tracking of a visual marker on the LUS Probe **150** instead of the Optotrak® readings. Thus, if the camera were moved while using tool tracking, the registration can be corrected on the fly as the tool is tracked. For additional details on tool tracking, see, e.g., commonly owned U.S. patent application US2006258938 with serial no. 11/130,471 entitled "Methods and system for performing 3-D tool tracking by fusion of sensor and/or camera derived data during minimally invasive surgery," filed May 16, 2005. In addition to, or alternatively, manual registration of ultrasound and camera images may be performed using conventional grab, move and rotate actions on a 3D ultrasound computer model of an anatomic structure, so that the computer model is properly registered over a camera model of the anatomic structure in the Master Display **104**.

[0054] Slave Arms **123** and **124** may manipulate the Endoscope **140** and LUS Probe **150** in similar manners as Slave Arms **121** and **122** manipulate Tools **138** and **139**. When there are only two master input devices in the system, however, such as Master Input Devices **107** and **108** in the System **100**, in order for the Surgeon to manually control movement of either the Endoscope **140** or LUS Probe **150**, it may be required to temporarily associate one of the Master Input Devices **107** and **108** with the Endoscope **140** or the LUS Probe **150** that the Surgeon desires manual control over, while its previously associated Tool and Slave Manipulator are locked in position.

[0055] FIG. 2 illustrates, as an example, a block diagram of the LUS Robotic Surgical System **100**. In this system, there are two Master Input Devices **107** and **108**. Master Input Device **107** controls movement of either a Tool **138** or a stereoscopic Endoscope **140**, depending upon which mode its Control Switch Mechanism **211** is in, and Master Input Device **108** controls movement of either a Tool **139** or a LUS Probe **150**, depending upon which mode its Control Switch Mechanism **231** is in.

[0056] The Control Switch Mechanisms **211** and **231** may be placed in either a first or second mode by a Surgeon using voice commands, switches physically placed on or near the Master Input Devices **107** and **108**, Foot Pedals **105** and **106** on the Console, or Surgeon selection of appropriate icons or other graphical user interface selection means displayed on the Master Display **104** or an auxiliary display (not shown).

[0057] When Control Switch Mechanism **211** is placed in the first mode, it causes Master Controller **202** to communicate with Slave Controller **203** so that manipulation of the Master Input **107** by the Surgeon results in corresponding movement of Tool **138** by Slave Arm **121**, while the Endoscope **140** is locked in position. On the other hand, when Control Switch Mechanism **211** is placed in the second mode, it causes Master Controller **202** to communicate with Slave Controller **233** so that manipulation of the Master Input **107** by the Surgeon results in corresponding movement of Endoscope **140** by Slave Arm **123**, while the Tool **138** is locked in position.

[0058] Similarly, when Control Switch Mechanism **231** is placed in the first mode, it causes Master Controller **222** to communicate with Slave Controller **223** so that manipulation of the Master Input **108** by the Surgeon results in corresponding movement of Tool **139** by Slave Arm **122**. In this case, however, the LUS Probe **150** is not necessarily locked in position. Its movement may be guided by an Auxiliary Controller **242** according to stored instructions in Memory **240**. The Auxiliary Controller **242** also provides haptic feedback to the Surgeon through Master Input **108** that reflects readings of a LUS Probe Force Sensor **247**. On the other hand, when Control Switch Mechanism **231** is placed in the second mode, it causes Master Controller **222** to communicate with Slave Controller **243** so that manipulation of the Master Input **222** by the Surgeon results in corresponding movement of LUS Probe **150** by Slave Arm **124**, while the Tool **139** is locked in position.

[0059] Before switching back to the first or normal mode, the Master Input Device **107** or **108** is preferably repositioned to where it was before the switch to the second mode of Control Switch **211** or **231**, as the case may be, or kinematic relationships between the Master Input Device **107** or **108** and its respective Tool Slave Arm **121** or **122** is readjusted so that upon switching back to the first or normal mode, abrupt movement of the Tool **138** or **139** does not occur. For additional details on control switching, see, e.g., commonly owned U.S. Pat. No. 6,659,939 "Cooperative Minimally Invasive Telesurgical System."

[0060] The Auxiliary Controller **242** also performs other functions related to the LUS Probe **150** and the Endoscope **140**. It receives output from a LUS Probe Force Sensor **247**, which senses forces being exerted against the LUS Probe **150**, and feeds the force information back to the Master Input Device **108** through the Master Controller **222** so that the Surgeon may feel those forces even if he or she is not directly controlling movement of the LUS Probe **150** at the time. Thus, potential injury to the Patient is minimized since the Surgeon has the capability to immediately stop any movement of the LUS Probe **150** as well as the capability to take over manual control of its movement.

[0061] Another key function of the Auxiliary Control **242** is to cause processed information from the Endoscope **140** and the LUS Probe **150** to be displayed on the Master Display **104** according to user selected display options. As will be described in more detail below, such processing includes generating a 3D ultrasound image from 2D ultrasound

image slices received from the LUS Probe **150** through an Ultrasound Processor **246**, causing either 3D or 2D ultrasound images corresponding to a selected position and orientation to be displayed in a picture-in-picture window of the Master Display **104**, and causing either 3D or 2D ultrasound images of an anatomic structure to overlay a camera captured image of the anatomic structure being displayed on the Master Display **104**.

[0062] Although shown as separate entities, the Master Controllers **202** and **222**, Slave Controllers **203**, **233**, **223**, and **243**, and Auxiliary Controller **242** are preferably implemented as software modules executed by the Processor **102**, as well as certain mode switching aspects of the Control Switch Mechanisms **211** and **231**. The Ultrasound Processor **246** and Video Processor **236**, on the other hand, are separate boards or cards typically provided by the manufacturers of the LUS Probe **150** and Endoscope **140** that are inserted into appropriate slots coupled to or otherwise integrated with the Processor **102** to convert signals received from these image capturing devices into signals suitable for display on the Master Display **104** and/or for additional processing by the Auxiliary Controller **242** before being displayed on the Master Display **104**.

[0063] FIG. 3 illustrates a side view of one embodiment of the LUS Probe **150**. The LUS Probe **150** is a dexterous tool with preferably two distal degrees of freedom, permitting reorientation of LUS Sensor **301** through, for example, approximately $\pm 80^\circ$ in distal "pitch" and "yaw", and $\pm 240^\circ$ in "roll" about a ball joint type, pitch-yaw mechanism **311** (functioning as and also referred to herein as a "Wrist" mechanism). Opposing pairs of Drive Rods or Cables (not shown) physically connected to a proximal end of the LUS Sensor **301** and extending through an internal passage of Elongated Shaft **312** mechanically control pitch and yaw movement of the LUS Sensor **301** using conventional push-pull type action. This flexibility of the LUS Probe **150** (provided by the pitch/yaw wrist mechanism) is especially useful in optimally orienting the LUS Probe **150** for performing ultrasonography on an anatomic structure during a minimally invasive surgical procedure.

[0064] The LUS Sensor **301** captures 2D ultrasound slices of a proximate anatomic structure, and transmits the information back to the Processor **102** through LUS Cable **304**. Although shown as running outside of the Elongated Shaft **312**, the LUS Cable **304** may also extend within it. A Clamshell Sheath **321** encloses the Elongate Shaft **312** and LUS Cable **304** to provide a good seal passing through a Cannula **331** (or trocar). Fiducial Marks **302** and **322** are placed on the LUS Sensor **301** and the Sheath **321** for video tracking purposes.

[0065] A force sensing capability is provided by Strain Gauges **303** which provide direct feedback of how hard the LUS Probe **150** is pushing on a structure being sonographed, supplementing whatever limited feedback is available from joint motor torques. Potential uses of this information include: providing a redundant safety threshold check warning the Surgeon or preventing motion into the structure if forces get too great; providing the Surgeon with an approved haptic appreciation of how hard he or she is pushing on a structure; and possibly permitting some measure of compensation for unmodeled deflections of the pitch-Yaw or "Wrist" Mechanism **311** which are not detected for some reason by joint position sensors or encoders. The Strain Gauges **303** in this case serve the function of the LUS Probe Force Sensor **247** as previously described in reference to FIG. 2.

[0066] Robotic assisted LUS has the potential to reduce variability in the ultrasound images produced, compared to freehand scanning, and can reduce operator workload and difficulty. Behaviors as simple as rocking the LUS Probe **150** back and forth can maintain an updated 3D ultrasound image without operator intervention. More complicated behaviors can include movement of the LUS Probe **150** along the surface of a target anatomical structure in a methodical pattern to generate a full image of the target, or reliably returning to a previously scanned probe location and orientation.

[0067] FIG. 4 illustrates, as an example, a flow diagram of a method for training the Auxiliary Controller **242** (i.e., providing it with stored instructions) to cause the LUS Probe **150** to be robotically moved in the trained manner upon command, in order to capture a sequence of 2D ultrasound image slices of an anatomic structure, which are used by the Auxiliary Controller **242** to generate a 3D computer model of the structure. Prior to performing the training, the Control Switch Mechanism **231** is placed in its second mode so that the Surgeon may move the LUS Probe **150** for training purposes by manipulating the Master Input Device **108**. After performing training, the Control Switch Mechanism **231** is then placed back into its first or normal mode so that the Surgeon may manipulate the Tool **139** to perform a minimally invasive surgical procedure using the Master Input Device **108**.

[0068] In **401**, the training module is initially idle (i.e., it is not being executed by the Processor **102**). In **402**, the Processor **102** (or a training module agent running in the background) may periodically check whether a start of training indication is received. Alternatively, the start of training indication may act as an interrupt which initiates running of the training module. The start of training indication may be initiated by a Surgeon through a recognized voice command, selection of a training option on a graphical user interface displayed on the Master Display **104**, a switch mechanism that may physically be located on the corresponding Master Control Input **108** or other convenient location accessible to the Surgeon, or any other conventional means.

[0069] After the start of training indication is detected, in **403**, the training module records or stores the current LUS Probe **150** position and orientation, and periodically (or upon Surgeon command) continues to do so by looping around **403** and **404** until a stop training indication is detected or received. The stop training indication in this case may also be initiated by the Surgeon in the same manner as the start of training indication, or it may be initiated in a different, but

other conventional manner. After the stop training indication is detected or received, a last position and orientation of the LUS Probe **150** is recorded or stored.

[0070] Between the start and stop of training, the Surgeon moves the LUS Probe **150** and the Processor **102** stores its trajectory of points and orientations so that they may be retraced later upon command. In one type of training, the Surgeon moves the LUS Probe **150** back and forth near an anatomic structure in order to capture a sequence of 2D ultrasound image slices from which a 3D version (or computer model) of the anatomic structure may be rendered by the Processor **102**. In another type of training, the Surgeon move the LUS Probe **150** once or more times along the surface of the anatomic structure in order to capture a different sequence of 2D ultrasound image slices from which a 3D version (or computer model) of the anatomic structure may be rendered by the Processor **102**.

[0071] Although described as recording the positions and orientations of the LUS Probe **150**, in practice, the active joint positions of its Slave Arm **124** are stored instead since their measurements are directly obtainable through encoders attached to each of the joints and their positions correspond to the LUS Probe **150** positions and orientations.

[0072] After storing the trajectory of positions and orientations of the LUS Probe **150** in the Memory **240**, the trajectory is then associated with a means for the Surgeon to command the Auxiliary Controller **242** to move the LUS Probe **150** in the desired fashion. For example, the trajectory may be associated with a voice command which upon its detection, the Auxiliary Controller **242** causes the Slave Arm **124** to move the LUS Probe **150** back and forth along the stored trajectory of positions and orientations. Likewise, the trajectory may also be associated with a user selectable option on a graphical user interface displayed on the Master Display **104**, or it may be associated with a switch mechanism such as a button or unused control element on the Master Input Device **108**. It may also be associated with the depression of the Foot Pedal **106**, so that the Auxiliary Controller **242** causes the Slave Arm **124** to move the LUS Probe **150** back and forth along the stored trajectory of positions and orientations as long as the Foot Pedal **106** is being depressed, and stops such motion once the Surgeon takes his or her foot off the Foot Pedal **106**.

[0073] FIG. 5 illustrates, as an example, a flow diagram of a method for generating clickable thumbnail images corresponding to LUS Probe **150** positions and orientations that are stored in Memory **240**, so that when the Surgeon clicks on one of the thumbnail images, the Auxiliary Controller **242** causes the Slave Arm **124** to move the LUS Probe **150** to its stored position and orientation. This allows the Surgeon to move the LUS Probe **150** to see different views of an anatomic structure while the Control Switch Mechanism **231** is in its first or normal mode. Thus, the Surgeon can continue to perform a minimally invasive surgical procedure by manipulating Tool **139** using the Master Input Device **108**. The method may then be combined with that described in reference to FIG. 4 in order to generate a sequence of 2D ultrasound image slices starting from that position and orientation, from which the Auxiliary Controller **242** may generate a 3D computer model rendition of the anatomic structure.

[0074] Prior to performing the method, however, the Control Switch Mechanism **231** is placed in its second mode so that the Surgeon may move the LUS Probe **150** into the desired positions and orientations by manipulating the Master Input Device **108**. After generating the clickable thumbnail images, the Control Switch Mechanism **231** is then placed back into its first or normal mode so that the Surgeon may manipulate the Tool **139** to perform the minimally invasive surgical procedure using the Master Input Device **108**.

[0075] In **501**, the Auxiliary Controller **242** receives a snapshot command from the Surgeon. The snapshot command may be, for example, a voice command, graphical user interface selection, or switch position. In **502**, the Auxiliary Controller **242** causes the LUS Probe **150** to capture a 2D ultrasound image slice, and in **503**, a thumbnail of the image is generated. The thumbnail in this case may include a simple JPEG or GIF file of the captured image. In **504**, the current position and orientation of the LUS Probe **150** is stored in Memory **240** along with information of its association with the thumbnail. In **505**, a clickable version of the thumbnail is displayed on the Master Display **104**, so that the Surgeon may command the Auxiliary Controller **242** to cause the LUS Probe to be positioned and oriented at the stored position and orientation at any time upon clicking with his or her mouse or other pointing device on the clickable thumbnail. The Surgeon may then move the LUS Probe **150** to other positions and/or orientations, and repeat **501-505** to generate additional thumbnail images.

[0076] FIG. 6 illustrates, as an example, a flow diagram of a method for automatically moving the LUS Probe **150** to a position and orientation associated with a clickable thumbnail upon command to do so by a Surgeon while performing a minimally invasive surgical procedure using Tool **139**. In **601**, the clicking of a thumbnail generated by the method described in reference to FIG. 5 is detected by, for example, a conventional interrupt handling process. Upon such detection, in **602**, the Auxiliary Controller **242** is instructed by, for example, stored instructions corresponding to the interrupt handling process, to retrieve the position and orientation stored in Memory **240** which is associated with the thumbnail. The Auxiliary Controller **242** then causes the LUS Probe **150** to move to that position and orientation by appropriately controlling Slave Arm **124**. Thus, the Surgeon is able to move the LUS Probe **150** to a desired position without having to change modes of the Control Switch Mechanism **231** and halt operation of the Tool **139** until the LUS Probe **150** is moved.

[0077] FIG. 7 illustrates, as an example, a flow diagram of a method for robotically assisted needle guidance and penetration into a marked lesion of a cancerous structure, which allows appreciation for the aspects of robotic assisted

LUS described herein. In **701**, a selected 2D ultrasound image slice view of a cancerous structure such as a liver is displayed at the proper depth on the Master Display **104** as an overlay to a 3D camera view of the cancerous structure. The selected 2D ultrasound image slice view may be a frontal view or an inner slice view as taken from a previously generated 3D ultrasound computer model of the cancerous structure.

[0078] As an example clarifying the **701** process, **FIG. 8** illustrates a simplified perspective view of a 3D ultrasound computer model **800** of the cancerous structure, which has been generated, for example, using the method described in reference to **FIG. 4**, and has been translated into the camera reference frame (EX, EY, EZ). **FIG. 9**, on the other hand, illustrates a simplified perspective view of a 3D camera view **900** of the cancerous structure as taken by the stereoscopic Endoscope **140**. If the Surgeon selects a frontal slice **801** of the 3D ultrasound computer model **800** to be viewed as an overlay to the 3D camera view **900**, then the overlay will appear as shown in **FIG. 10**. On the other hand, if the Surgeon selects one of the inner slices **802-804** of the 3D ultrasound computer model **800**, such as inner slice **803**, to be viewed as an overlay to the 3D camera view **900**, then the overlay will appear as shown in **FIG. 11** with the 2D ultrasound image slice **803** displayed at the proper depth. To avoid confusion, the portion of the 3D camera view above that depth is made transparent.

[0079] Alternatively, in **701**, the surgeon may manually control movement of the LUS Probe **150** so that 2D ultrasound image slices captured by it appear as emanating in proper perspective and direction from the 3D camera image of the LUS Probe **150** in the Master Display **104**. Preferably, the emanated 2D image slices being displayed in the Master Display **104** do not occlude the anatomic structure being probed. This manual approach may be particularly useful to the Surgeon for quickly spotting lesions in the anatomic structure.

[0080] In **702**, the Surgeon marks lesions on the cancerous structure displayed as a result of **701**. Each marked lesion is preferably marked using a designated color in order to clearly show that the Surgeon has already identified it, thereby avoiding double counting. The location in the camera reference frame (EX, EY, EZ) of each marked lesion is stored in Memory **240**, and in **703**, the Processor **102** determines an optimal needle tip path to that location.

[0081] In **703**, the Processor **102** generates a virtual fixture to help guide the needle to the marked lesion. To generate the virtual fixture, local kinematic constraints on the Slave Arm manipulating the needle Tool may be specified by providing a table of constraints of the form:

$$\left(\vec{x} - \vec{x}_0 \right)^T A_K \left(\vec{x} - \vec{x}_0 \right) + \vec{b}_K \left(\vec{x} - \vec{x}_0 \right) \leq c \quad (2)$$

[0082] where $\vec{x}$ represents, in simplified terms, the current 6 DOF kinematic pose of a master arm, or, in more general terms, a parameterization of a Cartesian pose F linearized about some nominal pose F_0 so that $(\vec{x} - \vec{x}_0) = F_0^{-1} F$. The tables are to be updated periodically based on visual feedback, user interaction, etc.

[0083] As can be appreciated, equation (2) can be easily checked and enforced.

[0084] Similarly, a simple table-driven interface for surgeon interaction forces can be implemented approximately as follows:

$$\vec{f} \leftarrow 0; \quad y \leftarrow \vec{x} - \vec{x}_0; \quad (3)$$

for $k \leftarrow 1$ to N do

$$\{ \epsilon \leftarrow \vec{y}^T C_K \vec{y} + \vec{d}_k \vec{y} - e_k;$$

$$\text{if } \epsilon > 0 \text{ then } \{ \vec{g} \leftarrow 2 C_K \vec{y} \vec{d}_k; \vec{f} \leftarrow \vec{f} + f(\epsilon) \vec{g} / \|\vec{g}\|; \};$$

$\};$

output $\vec{f}$ (after limiting & spacing)

[0085] where ϵ corresponds, roughly, to a distance from a surface in state space and the function $f(\epsilon)$ corresponds to a (non-linear) stiffness.

[0086] The above formulation suffices to support a variety of virtual chamfers, virtual springs, detents, etc. It is also easily extended to virtual dampers by adding velocity terms.

[0087] Now, more particularly, in the present case where it is desired to help aim an injection needle at a target in a live ultrasound image, let:

$$\vec{P}_{\text{TROCAR}} = \text{position where needle enters patient} \quad (4)$$

$$= \text{"RCM" point for needle insertion arm}$$

$$\mathbf{R}_{\text{NEEDLE}} = \mathbf{R}_0 \mathbf{R}(\vec{\alpha}) = \text{orientation of needle arm} \quad (5)$$

$$\vec{\alpha} = \text{vector representation for small rotation} \quad (6)$$

$$\mathbf{F}_{\text{LUS}} = [\mathbf{R}_{\text{LUS}}, \vec{P}_{\text{LUS}}] = \text{pose of LUS sensor} \quad (7)$$

$$\mathbf{V}_{\text{TARGET}} = \text{position of target wrt LUS sensor} \quad (8)$$

[0088] Then the basic constraint is that the needle axis (which is assumed for this example to be the $\vec{Z}$ axis of the needle driver) should be aimed at the target lesion, which will be given by $\mathbf{F}_{\text{LUS}} \vec{V}_{\text{TARGET}}$. One metric for the aiming direction error will be:

$$\epsilon_{\text{AIMING}}(\vec{\alpha}) = \left\| \left(\mathbf{R}_{\text{NEEDLE}} \vec{z} \right) \times \left(\mathbf{F}_{\text{LUS}} \vec{V}_{\text{TARGET}} - \vec{P}_{\text{TROCAR}} \right) \right\|^2 \quad (9)$$

$$= \left\| \left(\mathbf{R}(\vec{\alpha}) \vec{z} \right) \times \mathbf{R}_0^{-1} \left(\mathbf{F}_{\text{LUS}} \vec{V}_{\text{TARGET}} - \vec{P}_{\text{TROCAR}} \right) \right\|^2$$

[0089] which can be approximated as a quadratic form in $\vec{\alpha}$ and converted to a virtual fixture using the method described above. Similarly, if the position of the needle tip is $\vec{P}_{\text{TIP}}$, the penetration depth beyond the LUS target will be given by:

$$\epsilon_{\text{BEYOND}} = \left(\mathbf{R}_0 \mathbf{R}(\vec{\alpha}) \vec{z} \right) \cdot \left(\mathbf{F}_{\text{LUS}} \vec{V}_{\text{TARGET}} - \vec{P}_{\text{TIP}} \right) \quad (10)$$

[0090] which can easily be transcribed into a virtual detent or barrier preventing over-penetration. Alternatively, a simple spherical attractor virtual fixture can be developed to minimize $\|\mathbf{F}_{\text{LUS}} \vec{V}_{\text{TARGET}} - \vec{P}_{\text{TIP}}\|$.

[0091] In 705, the Processor 102 determines the needle tip position as it moves towards the target lesion, and in 706, the Processor 102 determines the distance between the needle tip position and the target lesion. The needle tip position may be determined from the Slave Arm kinematics and/or through visual tracking in the camera image.

[0092] In 707, the color of the lesion or some other object in the display changes as the needle tip gets closer to the target. For example, the color may start off as blue when the needle tip is still far away from the target, and it may change through color spectrum so that it becomes red as it nears the target. Alternatively, a bar graph or other visual indicator

may be used to give a quick sense of the distance.

[0093] In **708**, a determination is made whether the distance has reached a threshold distance (usually specified as some distance close to or even at the surface of the target lesion). If the threshold has not been reached, then the method loops back to **705** and continually repeats **705-708** until the threshold is reached. Once the threshold is reached, in **709**, a 90 degree view of the cancerous structure and the approaching needle is shown in a picture-in-picture window of the Master Display **104**. The method may then go back to **705** and repeat **705-708** as the needle penetrates the cancerous structure or withdraws back to its start position.

[0094] Although the various aspects of the present invention have been described with respect to a preferred embodiment, it will be understood that the invention is entitled to full protection within the full scope of the appended claims.

Claims

1. A laparoscopic ultrasound robotic surgical system (100) comprising:

a first robotic arm (124) mechanically coupled to an ultrasound probe (150);
 a second robotic arm (122) mechanically coupled to a surgery related device (139);
 a master manipulator (108);
 a control switch (231) having user selectable first and second modes; and
 a processor (102) configured to cause the second robotic arm (122) to be locked in position and the first robotic arm (124) to move the ultrasound probe (150) according to user manipulation of the master manipulator (108) when the control switch (231) is in the first mode, and to cause the second robotic arm (122) to manipulate the surgery related device (139) according to manipulation of the master manipulator (108) and the first robotic arm (124) to move the ultrasound probe (150) according to stored instructions upon detection of a user command associated with the stored instructions when the control switch (231) is in the second mode.

2. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the surgery related device (139) is a surgical tool.

3. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the user command is a voice command.

4. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the user command derives from user selection of an option provided in a graphical user interface.

5. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the user command derives from a selection indicated by a switch position.

6. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the stored instructions instruct the processor (102) to cause the first robotic arm (124) to move the ultrasound probe (150) so that 2D ultrasound image slices captured by the ultrasound probe (150) while moving provide information for the processor (102) to generate a 3D computer model of at least part of an anatomic structure during a minimally invasive surgical procedure.

7. The laparoscopic ultrasound robotic surgical system (100) according to claim 6, wherein the stored instructions instruct the processor (102) to cause the first robotic arm (124) to move the ultrasound probe (150) along a trajectory of stored points.

8. The laparoscopic ultrasound robotic surgical system (100) according to claim 7, wherein the stored instructions instruct the processor (102) to cause the first robotic arm (124) to repetitively move the ultrasound probe (150) back and forth along the trajectory of stored points.

9. The laparoscopic ultrasound robotic surgical system (100) according to claim 7, wherein the trajectory of stored points include points on a surface of the anatomic structure.

10. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the stored instructions instruct the processor (102) to cause the first robotic arm (124) to move the ultrasound probe (150) so as to be positioned and oriented at a stored position and orientation.

11. The laparoscopic ultrasound robotic surgical system (100) according to claim 10, wherein the stored position and orientation correspond to a clickable thumbnail of an ultrasound image generated by the ultrasound probe (150) at the position and orientation.

12. The laparoscopic ultrasound robotic surgical system (100) according to claim 11, wherein the processor (102) is configured to cause the first robotic arm (124) to move the ultrasound probe (150) to the stored position and orientation upon receiving an indication that a user has clicked the clickable thumbnail.

13. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the surgery related device (139) is a surgical tool, and further comprising:

an endoscope (140) for capturing images of a surgical site in a patient;
wherein the processor (102) is configured to display the captured images in a picture section of a display screen (104) and an ultrasound image captured by the ultrasound probe (150) within a picture-in-picture section of the display screen (104).

14. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the surgery related device (139) is a surgical tool, and further comprising:

an endoscope (140) for capturing video images;
wherein the processor (102) is configured to spatially register ultrasound images captured by the ultrasound probe (150) with the video images captured by the endoscope (140).

15. The laparoscopic ultrasound robotic surgical system (100) according to claim 14, wherein the processor (102) is configured to determine positions and orientations of the ultrasound images relative to a frame of reference associated with the endoscope (140), and display the ultrasound images so as to overlay the video images at the determined positions and orientations on a display screen (104).

16. The laparoscopic ultrasound robotic surgical system (100) according to claim 15, wherein the endoscope (140) is a stereoscopic endoscope (140) for capturing right and left 2D camera views including captured images of the ultrasound probe (150), the display screen (104) is a 3D display screen (104), and the processor (102) is configured to: generate a 3D camera image from the captured right and left 2D camera views, and display the 3D camera images in the 3D display screen (104) with 2D ultrasound image slices captured by the ultrasound probe (150) overlaid in the 3D camera images so as to appear as emanating in proper perspective from the ultrasound probe (150).

17. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the control switch (231) is placed in the first or second mode by a user voice command.

18. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the control switch (231) is placed in the first or second mode by user selection of an option provided in a graphical user interface.

19. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the control switch (231) is placed in the first or second mode by a user selected switch position.

20. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the ultrasound probe (150) includes a force sensor (247) configured to sense forces exerted against the ultrasound probe (150) and to provide information of the sensed forces to the processor (102), and the processor (102) is configured to reflect information of the sensed forces back to the master manipulator (108) so as to be felt by a user while manipulating the master manipulator (108).

21. The laparoscopic ultrasound robotic surgical system (100) according to claim 1, wherein the ultrasound probe (150) comprises:

an ultrasound sensor (301);
an elongated shaft (312); and
a wrist mechanism (311) coupling the ultrasound sensor (301) to the elongated shaft (312) so as to allow pitch and yaw movement of the ultrasound sensor (301) relative to an axis running along a length of the elongated

shaft (312).

22. The laparoscopic ultrasound robotic surgical system (100) according to claim 21, wherein the ultrasound probe (150) further comprises:

a first pair of cables coupled to the ultrasound sensor (301) such that the ultrasound sensor (301) moves in a yaw direction by pulling on only one of the first pair of cables and moves in an opposite yaw direction when pulling on only the other of the first pair of cables.

23. The laparoscopic ultrasound robotic surgical system (100) according to claim 22, wherein the ultrasound probe (150) further comprises:

a second pair of cables coupled to the ultrasound sensor (301) such that the ultrasound sensor (301) moves in a pitch direction by pulling on only one of the second pair of cables and moves in an opposite pitch direction when pulling on only the other of the second pair of cables.

Patentansprüche

1. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall, wobei vorgesehen sind:

ein erster Roboterarm (124), der mechanisch an eine Ultraschallsonde (150) gekoppelt ist;
 ein zweiter Roboterarm (122), der mechanisch an eine chirurgische Vorrichtung (139) gekoppelt ist;
 ein Master-Manipulator (108),
 ein Steuerschalter (231), der eine erste und eine zweite Betriebsart, von einem Benutzer auswählbar, aufweist;
 und
 ein Prozessor (102), der dazu ausgebildet ist, den zweiten Roboterarm (124) zu veranlassen, in seiner Position verriegelt zu sein, und den ersten Roboterarm (124) zu veranlassen, die Ultraschallsonde (150) entsprechend einer Betätigung durch den Benutzer des Master-Manipulators (108) zu bewegen, wenn sich der Steuerschalter (231) in der ersten Betriebsart befindet, und den zweiten Roboterarm (122) zu veranlassen, die chirurgische Vorrichtung (139) entsprechend der Betätigung des Master-Manipulators (108) zu betätigen, und den ersten Roboterarm (124), die Ultraschallsonde (150) entsprechend gespeicherten Instruktionen zu bewegen, nach Erfassung eines Benutzerbefehls, welcher den gespeicherten Instruktionen zugeordnet ist, wenn sich der Steuerschalter (231) in der zweiten Betriebsart befindet.

2. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die chirurgische Vorrichtung (139) ein chirurgisches Werkzeug ist.

3. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Benutzerbefehl ein Sprachbefehl ist.

4. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Benutzerbefehl von einer Benutzerauswahl einer Option herrührt, die in einer graphischen Benutzerschnittstelle vorgesehen ist.

5. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Benutzerbefehl von einer Auswahl herrührt, die durch eine Schalterposition angezeigt wird.

6. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die gespeicherten Instruktionen den Prozessor (102) anweisen, den ersten Roboterarm (124) zu veranlassen, die Ultraschallsonde (150) zu bewegen, so dass zwei 2D-Ultraschallbildscheiben, die von der Ultraschallsonde (150) während der Bewegung aufgenommen werden, Information für den Prozessor (102) bereitstellen, um ein 3D-Computermodell zumindest eines Teils einer anatomischen Struktur während einer minimal-invasiven chirurgischen Prozedur zu erzeugen.

7. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 6, bei welchem die gespeicherten Instruktionen den Prozessor (102) anweisen, den ersten Roboterarm (124) dazu zu veranlassen, die Ultraschallsonde (150) entlang einer Trajektorie gespeicherter Punkte zu bewegen.

8. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 7, bei welchem die gespeicherten Instruktionen den Prozessor (102) anweisen, den ersten Roboterarm (124) dazu zu veranlassen, die Ultraschallsonde (150) wiederholt rückwärts und vorwärts entlang der Trajektorie gespeicherter Punkte zu bewegen.

9. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 7, bei welchem die Trajektorie gespeicherter Punkte auf einer Oberfläche der anatomischen Struktur enthält.

10. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die gespeicherten Instruktionen den Prozessor (102) anweisen, den ersten Roboterarm (124) dazu zu veranlassen, die Ultraschallsonde (150) so zu bewegen, dass sie an einer gespeicherten Position und Orientierung angeordnet bzw. orientiert ist.

11. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 10, bei welchem die gespeicherte Position und Orientierung einem anklickbaren Vorschaubild eines Ultraschallbildes entsprechen, das von der Ultraschallsonde (150) bei der Position und Orientierung erzeugt wird.

12. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 11, bei welchem der Prozessor (102) dazu ausgebildet ist, den ersten Roboterarm (124) dazu zu veranlassen, die Ultraschallsonde (150) zu der gespeicherten Position und Orientierung zu bewegen, nach Empfang einer Anzeige, dass ein Benutzer das anklickbare Vorschaubild angeklickt hat.

13. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die chirurgische Vorrichtung (139) ein chirurgisches Werkzeug ist, wobei weiterhin vorgesehen ist:

ein Endoskop (240) zur Aufnahme von Bildern eines Operationssitus in einem Patienten;
wobei der Prozessor (102) dazu ausgebildet ist, die aufgenommenen Bilder in einem Bildabschnitt eines Anzeigebildschirms (104) anzuzeigen, und ein Ultraschallbild, das von der Ultraschallsonde (150) aufgenommen wurde, innerhalb eines Bild-im-Bild-Abschnitts des Anzeigebildschirms (104).

14. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die chirurgische Vorrichtung (139) ein chirurgisches Werkzeug ist, und weiterhin vorgesehen ist:

ein Endoskop (140) zur Aufnahme von Videobildern;
wobei der Prozessor (102) dazu ausgebildet ist, räumlich Ultraschallbilder, die von der Ultraschallsonde (150) aufgenommen werden, mit den Videobildern auszurichten, die von dem Endoskop (140) aufgenommen werden.

15. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 14, bei welchem der Prozessor (102) dazu ausgebildet ist, Positionen und Orientierungen der Ultraschallbilder relativ zu einem Bezugsrahmen zu bestimmen, der dem Endoskop (140) zugeordnet ist, und die Ultraschallbilder so anzuzeigen, dass sie die Videobilder an den festgelegten Positionen und Orientierungen auf einem Anzeigebildschirm (104) überlagern.

16. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 15, bei welchem das Endoskop (140) ein stereoskopisches Endoskop (140) zur Aufnahme rechter und linker 2D-Kamerabilder ist, welche aufgenommene Bilder der Ultraschallsonde (150) enthalten, der Anzeigebildschirm (104) ein 3D-Anzeigebildschirm (104) ist, und der Prozessor (102) dazu ausgebildet ist, um: ein 3D-Kamerabild aus den aufgenommenen rechten und linken 2D-Kamerabildern zu erzeugen, und die 3D-Kamerabilder in dem 3D-Anzeigebildschirm (104) anzuzeigen, mit 2D-Ultraschallbildscheiben, die von der Ultraschallsonde (150) aufgenommen werden, überlagert in den 3D-Kamerabildern, und so erscheinen, als gingen sie in ordnungsgemäßer Perspektive von der Ultraschallsonde (150) aus.

17. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Steuerschalter (231) in der ersten oder zweiten Betriebsart durch einen Benutzer-Sprachbefehl angeordnet wird.

18. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Steuerschalter (231) in der ersten oder zweiten Betriebsart durch eine Benutzerauswahl einer Option angeordnet wird, die in einer graphischen Benutzerschnittstelle vorgesehen ist.

19. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem der Steuerschalter (231) in der ersten oder zweiten Betriebsart durch eine von einem Benutzer ausgewählte Schalterposition angeordnet

wird.

20. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die Ultraschallsonde (150) einen Kraftsensor (247) aufweist, der dazu ausgebildet ist, Kräfte zu erfassen, die gegen die Ultraschallsonde (150) einwirken, und Information bezüglich der erfassten Kräfte den Prozessor (102) zur Verfügung zu stellen, und der Prozessor (102) dazu ausgebildet ist, Information bezüglich der erfassten Kräfte zurück zum Master-Manipulator (108) zu reflektieren, so dass sie von einem Benutzer während der Benutzung des Master-Manipulators (108) gefühlt werden.

21. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 1, bei welchem die Ultraschallsonde (150) aufweist:

ein Ultraschallsensor (301);
eine längliche Welle (312); und
einen Handgelenkmechanismus (311), welcher den Ultraschallsensor (301) mit der länglichen Welle (312) so koppelt, dass eine Nickbewegung und eine Gierbewegung des Ultraschallsensors (301) relativ zu einer Achse ermöglicht werden, die entlang der Länge der länglichen Welle (312) verläuft.

22. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 21, bei welchem die Ultraschallsonde (150) weiterhin aufweist:

ein erstes Paar von Kabeln, die an den Ultraschallsensor (301) so gekoppelt sind, dass sich der Ultraschallsensor (301) in einer Gierrichtung bewegt, durch Ziehen nur eines der Kabel des ersten Paares von Kabeln, und sich in einer entgegengesetzten Gierrichtung bewegt, wenn nur das andere Kabel des ersten Paares von Kabeln gezogen wird.

23. Chirurgierobotersystem (100) mit laparoskopischem Ultraschall nach Anspruch 22, bei welchem die Ultraschallsonde (150) weiterhin aufweist:

ein zweites Paar von Kabeln, das so an den Ultraschallsensor (301) gekoppelt ist, dass sich der Ultraschallsensor (301) in einer Nickrichtung bewegt, durch Ziehen nur eines Kabels des zweiten Paares von Kabeln, und sich in einer entgegengesetzten Nickrichtung bewegt, beim Ziehen nur des anderen Kabels des zweiten Paares von Kabeln.

Revendications

1. Système chirurgical robotique ultrasonore laparoscopique (100) comprenant :

un premier bras robotique (124) couplé mécaniquement à une sonde ultrasonore (150) ;
un deuxième bras robotique (122) couplé mécaniquement à un dispositif associé à la chirurgie (139) ;
un manipulateur principal (108) ;
un commutateur de commande (231) ayant des premier et deuxième modes pouvant être sélectionnés par l'utilisateur ; et
un processeur (102) configuré pour entraîner le blocage du deuxième bras robotique (122) dans une position et le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) selon la manipulation effectuée par l'utilisateur du manipulateur principal (108) lorsque le commutateur de commande (231) est en premier mode et pour entraîner la manipulation par le deuxième bras robotique (122) du dispositif associé à la chirurgie (139) selon la manipulation du manipulateur principal (108) et le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) selon les instructions mémorisées après détection d'une commande utilisateur associée aux instructions mémorisées lorsque le commutateur de commande (231) se trouve en deuxième mode.

2. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le dispositif associé à la chirurgie (139) est un outil chirurgical.

3. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel la commande utilisateur est une commande vocale.

4. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel la commande utilisateur provient de la sélection par l'utilisateur d'une option se trouvant dans une interface graphique utilisateur.
5. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel la commande utilisateur provient d'une sélection indiquée par une position du commutateur.
6. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel les instructions mémorisées indiquent au processeur (102) d'entraîner le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) de sorte que des coupes d'images ultrasonores en 2D capturées par la sonde ultrasonore (150) pendant le déplacement fournissent des informations pour que le processeur (102) génère un modèle informatique en 3D d'au moins une partie d'une structure anatomique pendant une intervention chirurgicale mini-invasive.
7. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 6, dans lequel les instructions mémorisées indiquent au processeur (102) d'entraîner le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) le long d'une trajectoire de points mémorisés.
8. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 7, dans lequel les instructions mémorisées indiquent au processeur (102) d'entraîner le déplacement répétitif par le premier bras robotique (124) de la sonde ultrasonore (150) en va-et-vient le long de la trajectoire de points mémorisés.
9. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 7, dans lequel la trajectoire de points mémorisés comprend des points sur une surface de la structure anatomique.
10. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel les instructions mémorisées indiquent au processeur (102) d'entraîner le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) de façon à être positionnée et orientée sur une position et dans une orientation mémorisée.
11. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 10, dans lequel la position et l'orientation mémorisées correspondent à une image en réduction, sur laquelle on peut cliquer, d'une image ultrasonore générée par la sonde ultrasonore (150) sur la position et l'orientation.
12. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 11, dans lequel le processeur (102) est configuré pour entraîner le déplacement par le premier bras robotique (124) de la sonde ultrasonore (150) à la position et l'orientation mémorisées après avoir reçu une indication selon laquelle un utilisateur a cliqué sur l'image en réduction sur laquelle on peut cliquer.
13. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le dispositif associé à la chirurgie (139) est un outil chirurgical et comprenant en outre :
 - un endoscope (140) pour capturer des images d'un site chirurgical chez un patient ;
 - dans lequel le processeur (102) est configuré pour afficher les images capturées dans une section d'image d'un écran d'affichage (104) et une image ultrasonore capturée par la sonde ultrasonore (150) dans une section d'incrustation d'image de l'écran d'affichage (104).
14. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le dispositif associé à la chirurgie (139) est un outil chirurgical et comprenant en outre :
 - un endoscope (140) pour capturer des images vidéo ;
 - dans lequel le processeur (102) est configuré pour enregistrer spatialement les images ultrasonores capturées par la sonde ultrasonore (150) avec les images vidéo capturées par l'endoscope (140).
15. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 14, dans lequel le processeur (102) est configuré pour déterminer des positions et des orientations des images ultrasonores par rapport à un cadre de référence associé à l'endoscope (140) et afficher les images ultrasonores de façon à superposer les images vidéo sur les positions et orientations déterminées sur un écran d'affichage (104).
16. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 15, dans lequel l'endoscope (140) est un endoscope stéréoscopique (140) pour la capture des vues de la caméra de droite et gauche en 2D

comprenant les images capturées de la sonde ultrasonore (150), l'écran d'affichage (104) est un écran en 3D (104) et le processeur (102) est configuré pour : générer une image de caméra en 3D à partir des vues capturées de la caméra de droite et de gauche en 2D et afficher les images de la caméra en 3D sur l'écran d'affichage en 3D (104) avec des coupes d'image ultrasonore en 2D capturées par la sonde ultrasonore (150) superposées dans les images de la caméra en 3D de façon à apparaître comme provenant en perspective correcte de la sonde ultrasonore (150).

17. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le commutateur de commande (231) est placé en premier ou deuxième mode par la commande vocale d'un utilisateur.

18. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le commutateur de commande (231) est placé en premier ou deuxième mode par la sélection par l'utilisateur d'une option figurant dans une interface graphique utilisateur.

19. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel le commutateur de commande (231) est placé en premier ou deuxième mode par une position du commutateur choisie par l'utilisateur.

20. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel la sonde ultrasonore (150) comprend un capteur de force (247) configuré pour capter les forces exercées contre la sonde ultrasonore (150) et pour fournir des informations sur les forces captées au processeur (102) et le processeur (102) est configuré pour renvoyer les informations sur les forces captées au manipulateur principal (108) de façon à être perçues par un utilisateur lorsqu'il manipule le manipulateur principal (108).

21. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 1, dans lequel la sonde ultrasonore (150) comprend :

un capteur ultrasonore (301) ;
une tige allongée (312) ; et
un mécanisme de poignet (311) couplant le capteur ultrasonore (301) à la tige allongée (312) de façon à permettre un mouvement de tangage et de lacet du capteur ultrasonore (301) par rapport à un axe s'étendant le long de la tige allongée (312).

22. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 21, dans lequel la sonde ultrasonore (150) comprend en outre :

une première paire de câbles couplés au capteur ultrasonore (301) de telle sorte que le capteur ultrasonore (301) se déplace dans une direction de lacet en tirant uniquement sur un câble de la première paire de câbles et se déplace dans une direction de lacet opposée en tirant uniquement sur l'autre câble de la première paire de câbles.

23. Système chirurgical robotique ultrasonore laparoscopique (100) selon la revendication 22, dans lequel la sonde ultrasonore (150) comprend en outre :

une deuxième paire de câbles couplés au capteur ultrasonore (301) de telle sorte que le capteur ultrasonore (301) se déplace dans une direction de tangage en tirant uniquement sur un câble de la deuxième paire de câbles et se déplace dans une direction de tangage opposée en tirant uniquement sur l'autre câble de la deuxième paire de câbles.

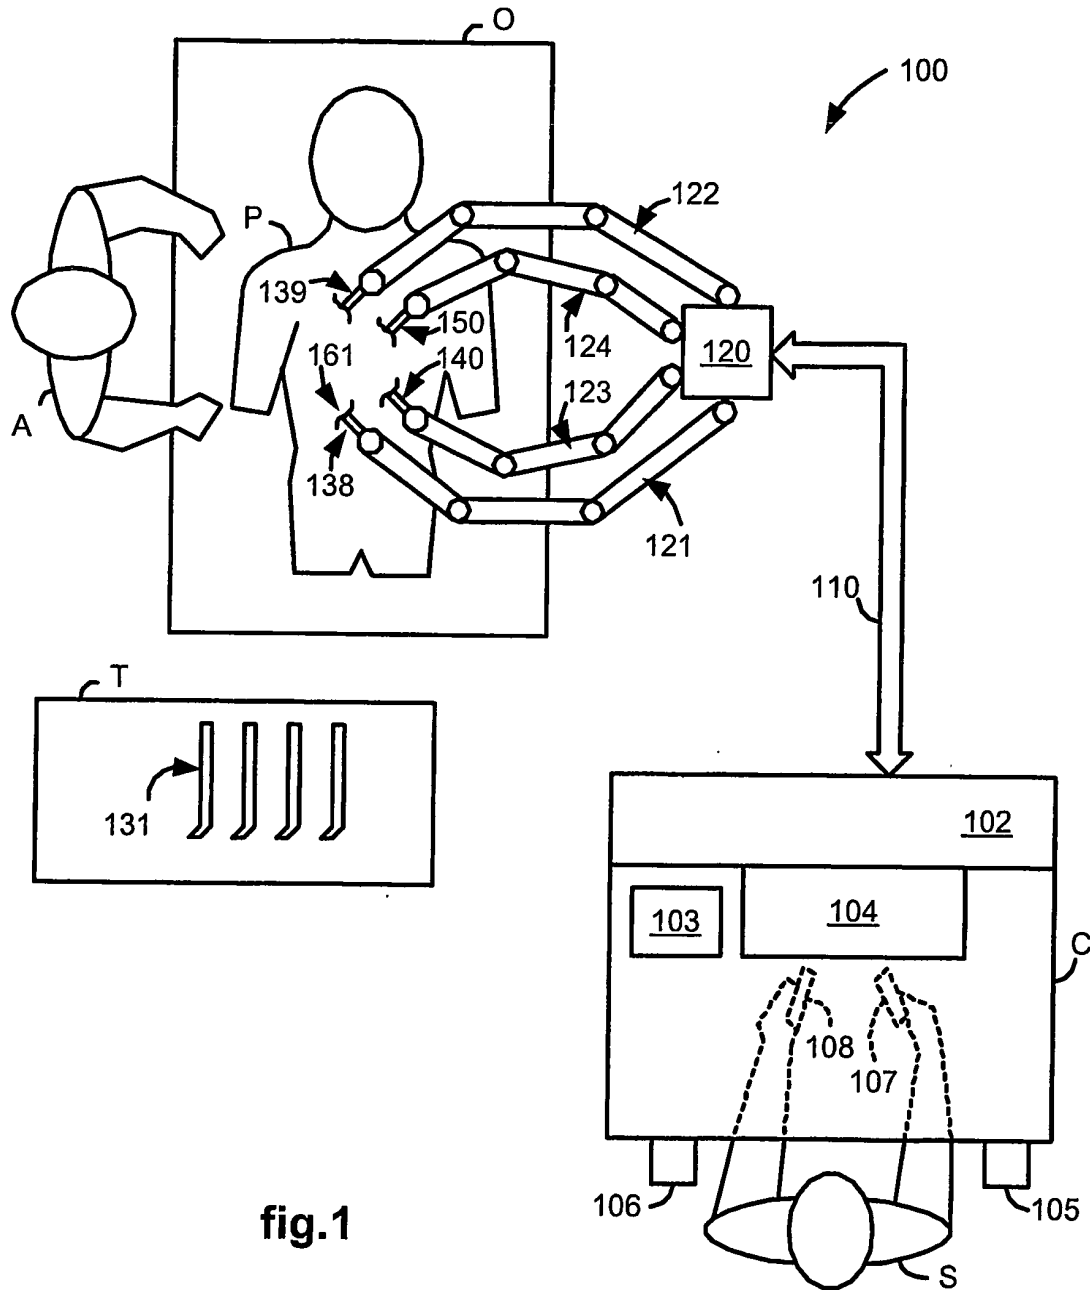


fig.1

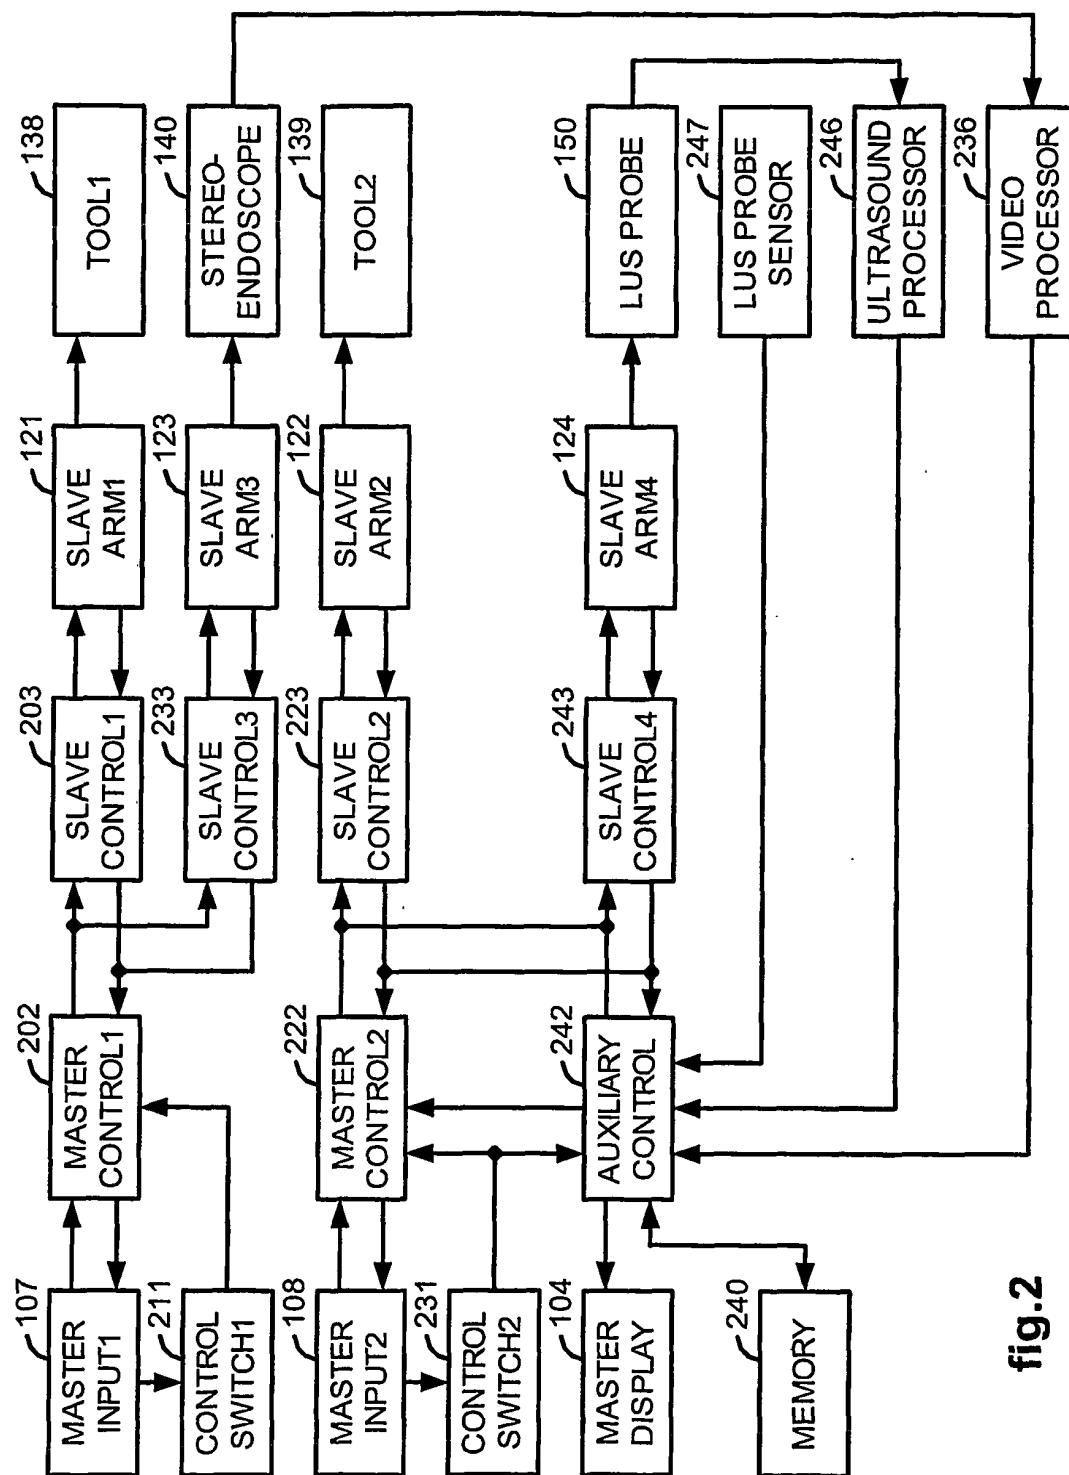


fig.2

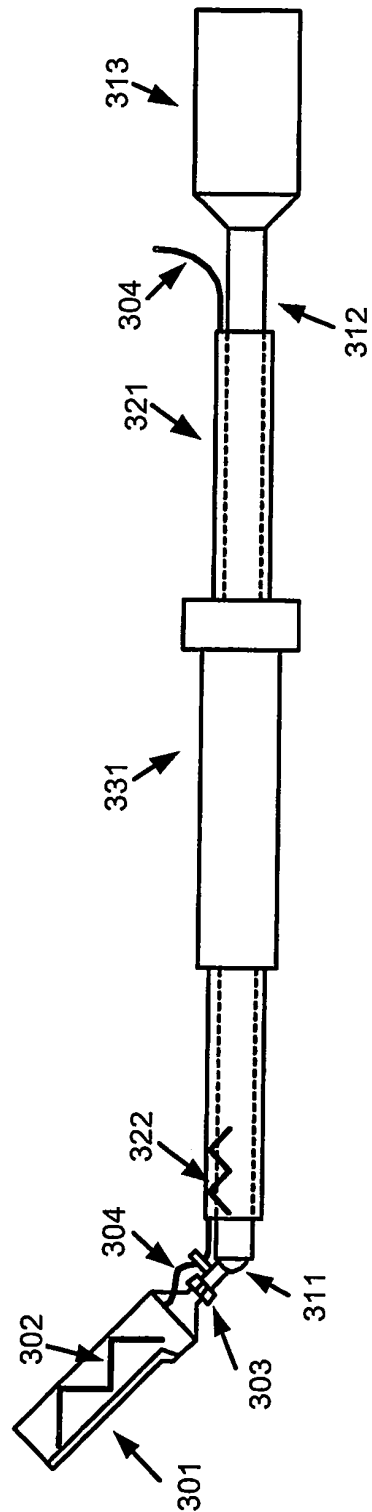


fig. 3

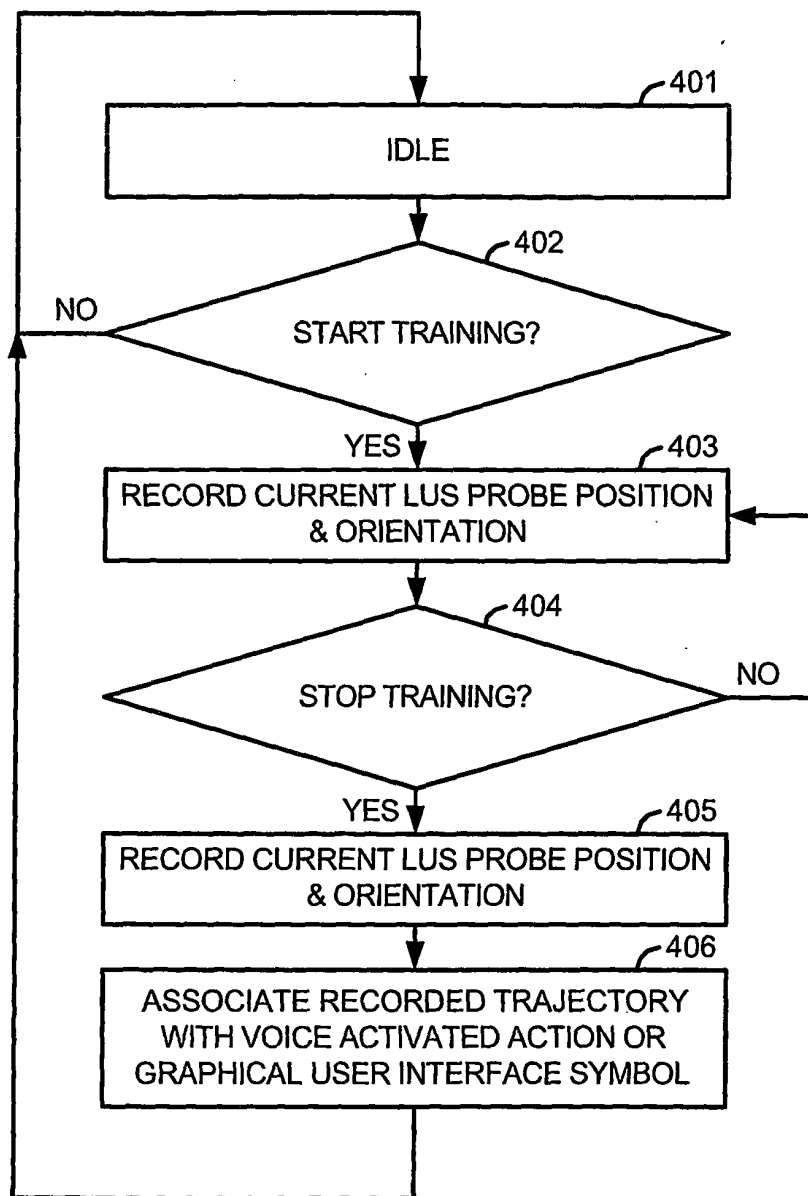


fig.4

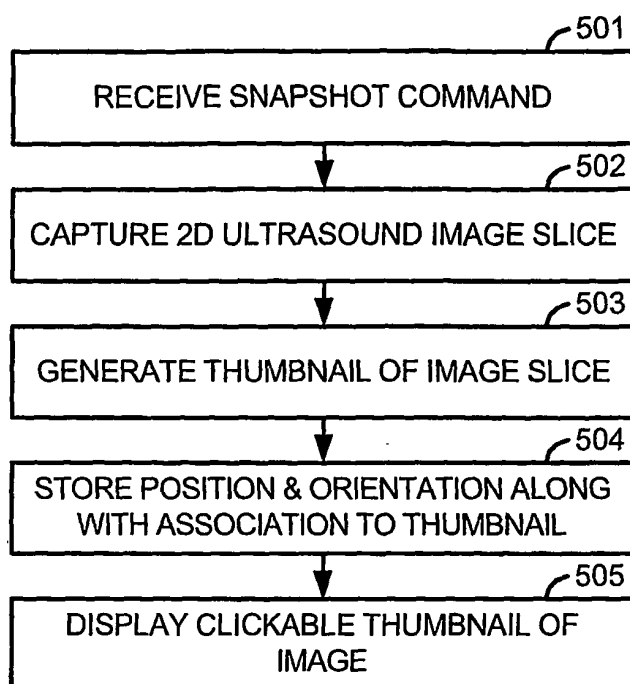


fig.5

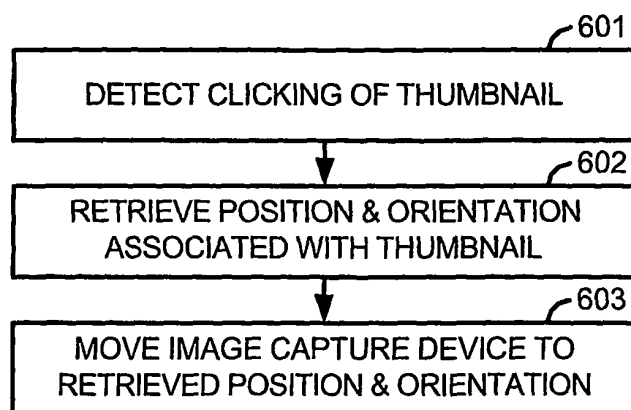


fig.6

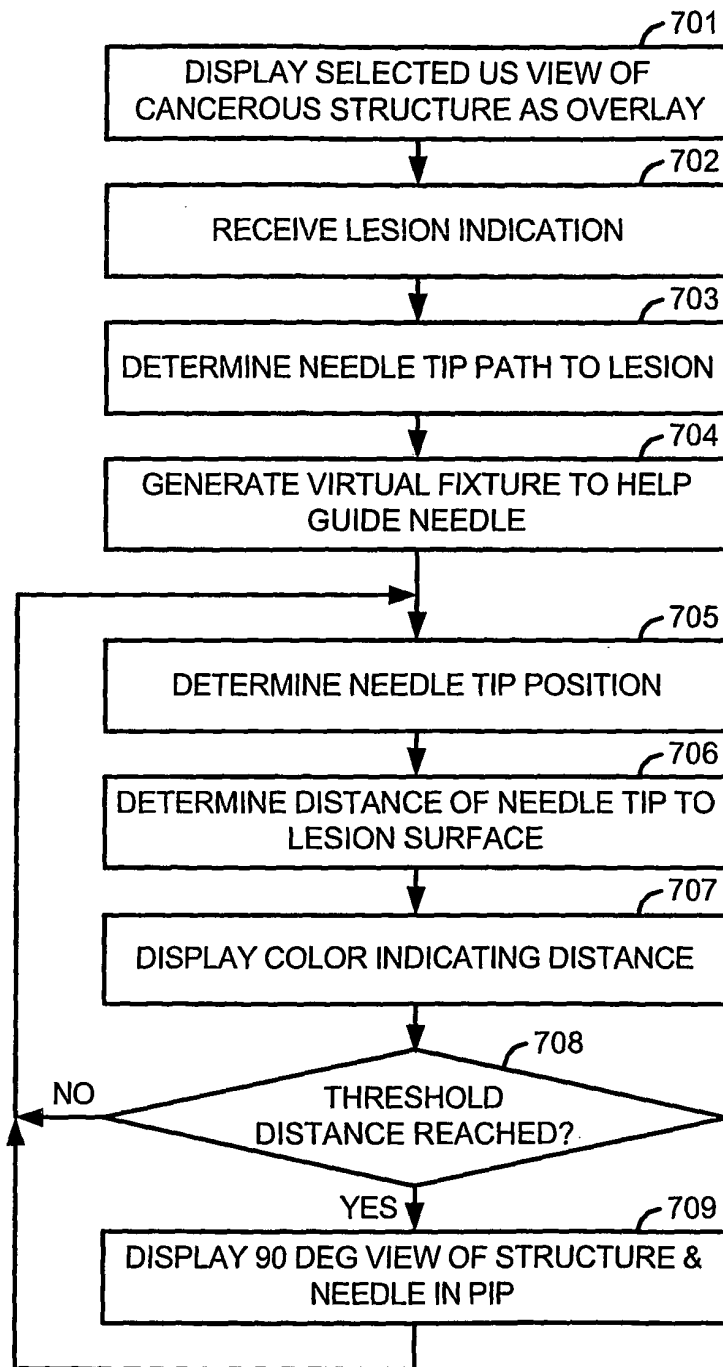


fig.7

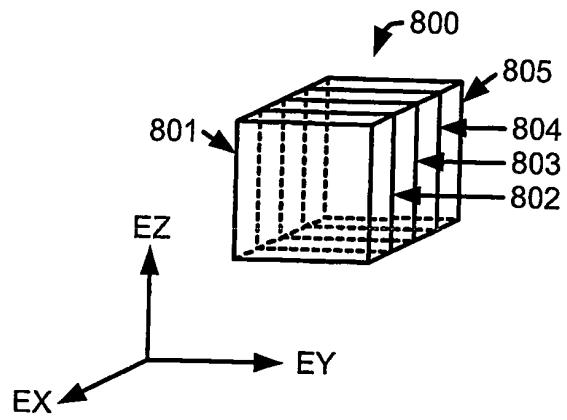


fig.8

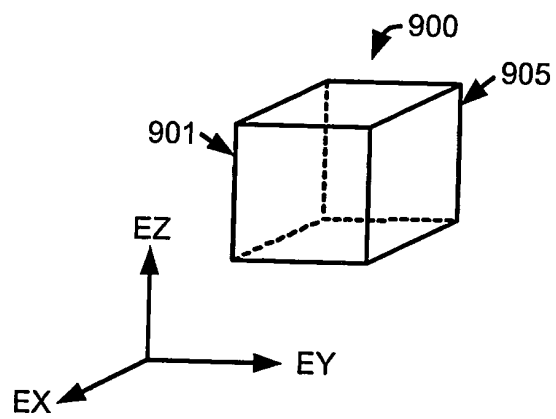


fig.9

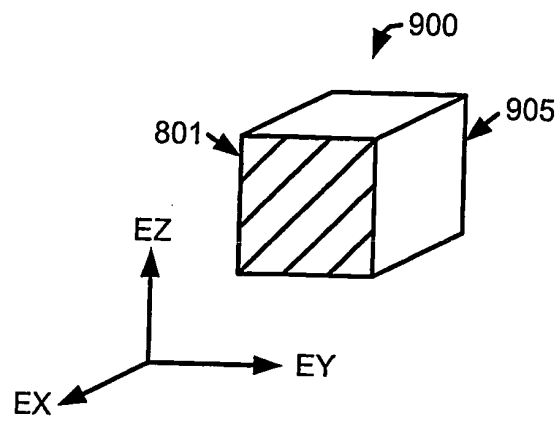


fig.10

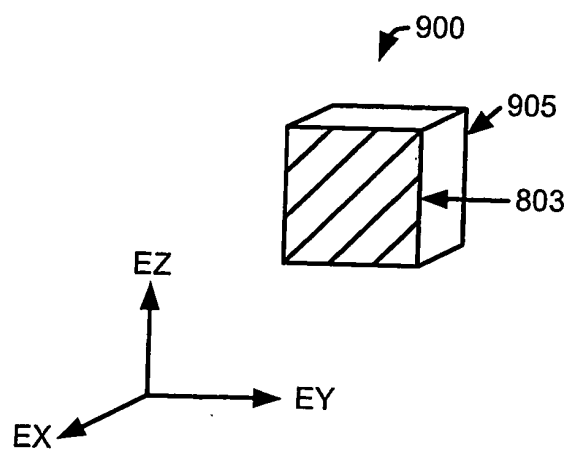


fig.11

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 20030220541 A [0015]
- US 5797900 A [0034]
- US 2006258938 A [0053]
- US 11130471 B [0053]
- US 6659939 B [0059]

Non-patent literature cited in the description

- **E. BOCTOR ; A. VISWANATHAN ; M. CHIOTI ; R. TAYLOR ; G. FICHTINGER ; G. HAGER.** A Novel Closed Form Solution for Ultrasound Calibration. *International Symposium on Biomedical Imaging*, 2004, 527-530 [0045]

专利名称(译)	腹腔镜超声机器人手术系统		
公开(公告)号	EP1887961B1	公开(公告)日	2012-01-11
申请号	EP2006784595	申请日	2006-06-05
[标]申请(专利权)人(译)	直观外科手术公司		
申请(专利权)人(译)	Intuitive Surgical公司 , INC.		
当前申请(专利权)人(译)	Intuitive Surgical公司运营 , INC.		
[标]发明人	HASSER CHRISTOPHER TAYLOR RUSSELL CHOTI MICHAEL LEVEN JOSH		
发明人	HASSER, CHRISTOPHER TAYLOR, RUSSELL CHOTI, MICHAEL LEVEN, JOSH		
IPC分类号	A61B19/00 A61B8/00		
CPC分类号	A61B8/00 A61B8/12 A61B8/4218 A61B8/4245 A61B34/25 A61B34/30 A61B34/37 A61B34/70 A61B34/76 A61B90/03 A61B90/361 A61B2017/00203 A61B2034/107 A61B2090/364 A61B2090/365 A61B2090/378 A61B1/3132 A61B8/461 A61B90/37 A61B2034/305		
优先权	60/688013 2005-06-06 US		
其他公开文献	EP1887961A1		
外部链接	Espacenet		

摘要(译)

LUS机器人手术系统可由外科医生训练以在命令时以期望的方式自动移动LUS探针，使得外科医生在微创外科手术期间不必手动操作。由LUS探针根据存储的指令捕获的2D超声图像切片序列可处理成解剖结构的3D超声计算机模型，其可以显示为摄像机视图的3D或2D覆盖或者通过选择的PIP显示。外科医生或编程以协助外科医生检查解剖结构的异常情况。虚拟固定装置是可定义的，以便帮助外科医生将工具准确地引导到所显示的超声图像上的目标。

