



(11)

EP 2 648 603 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:

05.02.2020 Bulletin 2020/06

(51) Int Cl.:

A61B 1/313 ^(2006.01) **A61B 1/00** ^(2006.01)
A61B 1/05 ^(2006.01) **A61B 1/06** ^(2006.01)
A61M 13/00 ^(2006.01)

(21) Application number: **11846608.5**

(86) International application number:

PCT/US2011/063948

(22) Date of filing: **08.12.2011**

(87) International publication number:

WO 2012/078872 (14.06.2012 Gazette 2012/24)

(54) **PORTABLE LAPAROSCOPE SYSTEM**

TRAGBARES LAPAROSKOPSYSTEM

SYSTÈME DE LAPAROSCOPE PORTABLE

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

- **ARE, Madhuri**
Omaha, NE 68116 (US)
- **ALEXANDER, Dennis**
Lincoln, NE 68516 (US)

(30) Priority: **08.12.2010 US 420901 P**

(74) Representative: **Hamer, Christopher K.**
Mathys & Squire LLP
The Shard
32 London Bridge Street
London SE1 9SG (GB)

(43) Date of publication of application:
16.10.2013 Bulletin 2013/42

(73) Proprietor: **The Board of Regents of
the University of Nebraska**
Lincoln, NE 68583-0745 (US)

(56) References cited:
WO-A2-2010/088135 US-A- 5 785 644
US-A1- 2005 197 536 US-A1- 2008 033 450
US-A1- 2009 005 636 US-B1- 6 387 043

(72) Inventors:

- **ARE, Chandrakanth**
Omaha, NE 68116 (US)

EP 2 648 603 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

BACKGROUND

[0001] Medical professionals employ laparoscopes to perform minimally invasive surgery on a patient's abdominal cavity for diagnostic and treatment purposes. Generally, laparoscopes comprise an instrument configured to pass through a small incision (e.g., in the abdominal wall) and capture images (e.g., video) of areas within a patient. The captured images are normally displayed by large monitors that are positioned proximate to the laparoscopic procedure area (e.g., suspended from the ceiling of the operating room around the operating table). During use, laparoscopes require a myriad of associated equipment, such as power sources, insufflators and so on, which are coupled to the laparoscope via a wiring/tube harness, and so forth. Consequently, laparoscopes are confined to use in dedicated surgical environments, such as a laparoscopic operating room in a hospital.

[0002] Prior art document US 5,785,644 discloses a portable laparoscope system which is used in combination with a source of insufflation such as an insufflation needle in a trocar.

SUMMARY

[0003] A portable laparoscope is disclosed. The portable laparoscope is capable of providing laparoscopic imaging functionality to medical personnel in unconventional environments (e.g., environments other than a dedicated laparoscopic operating room, including environments such as but not necessarily limited to: rural areas, combat zones, and so on). In implementations, the portable laparoscope includes a housing and an elongated tube coupled to the housing. A lighting source and an image capture device are disposed proximate to an end of the elongated tube opposite the housing. The image capture device is configured to capture an image in a viewing area that is illuminated by light provided by the lighting source. The portable laparoscope includes an image display apparatus configured to display the images acquired by the image capture device and/or to transmit the images to a remote display device. The portable laparoscope may be configured to position and hold an insufflator.

[0004] The invention is defined in the appended claims 1 - 13.

DRAWINGS

[0005] The detailed description is described with reference to the accompanying figures. The use of the same reference numbers in different instances in the description and the figures may indicate similar or identical items. It should be noted that the drawings are not necessarily to scale.

FIG. 1 is a block diagram illustrating an example portable laparoscope in accordance with example implementations of the present disclosure.

FIG. 2 is a diagrammatic isometric view illustrating a portable laparoscope used in a non-dedicated surgical environment in accordance with example implementations of the present disclosure.

FIG. 3 is a diagrammatic isometric view of the portable laparoscope illustrated in FIG. 2, where a light source and a camera are disposed proximate to an end of an elongated tube of the portable laparoscope.

FIG. 4A is a diagrammatic isometric view illustrating a portable laparoscope configured with a flip screen display device in accordance with example implementations of the present disclosure.

FIG. 4B is a diagrammatic isometric view illustrating a portable laparoscope configured to employ a mobile device for display of images in accordance with example implementations of the present disclosure.

FIG. 4C is a diagrammatic isometric view illustrating a portable laparoscope including a display device configured to articulate to provide multiple viewing angles in accordance with example implementations of the present disclosure.

FIG. 4D is a diagrammatic isometric view illustrating a portable laparoscope including a fixed display device in accordance with example implementations of the present disclosure.

FIG. 4E is a diagrammatic isometric view illustrating a portable laparoscope coupled with a detachable display device in accordance with example implementations of the present disclosure.

FIG. 4F is a partial diagrammatic isometric view illustrating an end of an elongated tube of a portable laparoscope, where a light source and a camera array is disposed at the end of the elongated tube in accordance with example implementations of the present disclosure.

FIG. 4G is a diagrammatic view illustrating a portable laparoscope including a housing configured with a display device and a handle to assist with operating the portable laparoscope in accordance with example implementations of the present disclosure.

FIG. 5 is a diagrammatic isometric view of a portable laparoscope as used in a surgical environment, where the portable laparoscope includes a gas cartridge, a trocar-hookup, and a trocar in accordance with example implementations of the present disclosure.

FIG. 6 is a diagrammatic side elevation view of the portable laparoscope illustrated in FIG. 5.

DETAILED DESCRIPTION

Overview

[0006] Laparoscopes are generally used to perform

minimally invasive surgeries. Laparoscopes employ a variety of detached equipment such as power sources, insufflators, monitors, and so on, which are coupled to the laparoscope via a wiring/tube harness, or the like. For example, laparoscopic equipment is generally connected to a bank of large display screens arranged within a dedicated operating room in order to provide a physician with as large and as detailed a view of a patient's internal organs as possible. Consequently, laparoscopes are very expensive, cumbersome and time consuming to set-up. Thus, laparoscopes have been confined to use in dedicated surgical environments such as a laparoscopic operating room in a hospital, surgical center, or the like.

[0007] In many instances, access to a dedicated surgical environment can be difficult or even impossible, especially when multiple patients must be evaluated and/or treated in a short span of time, such as during a mass casualty event. For example, in the case of an individual who has been subjected to multiple traumatic injuries, there may be a high risk of internal bleeding. Instant triage evaluation of this type of polytrauma patient in the emergency room itself may be difficult, compounded by the fact that diagnosing internal bleeding is very time sensitive in order to provide effective intervention. Although a technique such as Focused Assessment with Sonography for Trauma (FAST) can provide some information, it lacks the ability to fully visualize internal organs in an ambulatory setting, which can help significantly in triaging patients. Further, in the Intensive Care Unit (ICU), diagnosing the onset of internal bleeding or other internal maladies is often complicated because polytraumatic patients are difficult to move or immobile. Thus, in both triage and ICU settings, imaging devices such as Computed Tomography (CT) devices or Magnetic Resonance Imaging (MRI) devices are not feasible solutions, especially when patients are hemodynamically stable and cannot be moved and such equipment is unavailable. With abdominal trauma, the use of CT with contrast may be preferred. As discussed, neither a triage nor an ICU setting lends itself to CT scanning due to a critical condition of patients, lack of patient mobility, and/or time constraints.

[0008] Accordingly, a portable laparoscope is disclosed. In one or more implementations, the portable laparoscope includes a housing and an elongated tube coupled to the housing. The portable laparoscope can be configured to support an insufflator. A lighting source and an image capture device (e.g., a camera) are disposed proximate to an end of the elongated tube opposite the housing. The camera is configured to capture an image in a viewing area that is illuminated by light provided by the lighting source. The portable laparoscope includes an image display apparatus configured to display the images acquired by the camera and/or to transmit the images to a remote display device. In one example, the image display apparatus may comprise a display such as a Liquid Crystal Display (LCD) for displaying captured

images and/or captured video of a patient's internals, such as an abdominal cavity, and so forth. In another example, the image display apparatus includes a transmitter disposed in the housing that is configured to transmit images and/or video captured by the camera to a receiver. The receiver is configured to receive the images and/or video for display by a display device communicatively coupled to the receiver.

[0009] The portable laparoscope is capable of providing laparoscopic imaging functionality to medical personnel in unconventional environments (e.g., environments other than a dedicated laparoscopic operating room). Thus, the portable laparoscope may be configured to be used in a variety of environments. For example, the portable laparoscope may be used in remote areas, such as, but not necessarily limited to: military field hospitals or rural areas, in a hospital environment outside of the operating room, or in areas where sophisticated and expensive medical equipment is generally not available. Further, the portable laparoscope may be used in applications other than surgical intervention, such as for surgical evaluation outside of an operating room.

[0010] The portable laparoscope may be used for determining the presence and/or extent of abdominal trauma. This information can then be used to determine an appropriate course of action in treatment, making conservative management of abdominal injury possible by providing information more accurate than that provided by a CT scan. Further, because portable laparoscopy can provide direct visualization of an abdominal cavity, resolution may not significantly influence diagnostic fidelity. However, using a portable laparoscope for abdominal trauma is provided by way of example only and is not meant to be restrictive of the present disclosure. Thus, a portable laparoscope can also be used for ischemic bowel, which may otherwise be difficult to diagnose, and often frustrates radiographic evaluation. Portable laparoscopy at a bedside in the ICU may dramatically ease diagnosis of ischemic bowel with much higher fidelity. In addition to the triage bay and ICU, portable laparoscopy may also be performed in multiple locations outside of the operating room. For example, most medical clinics have a clean space to perform procedures such as lumbar puncture or colonoscopy. Such rooms may also be utilized for laparoscopic evaluation using a portable laparoscope in accordance with the present disclosure. In the following discussion, an example portable laparoscope is described.

Example Environment

[0011] It will be understood that when an element is referred to as being "connected," "coupled," "operatively coupled," and/or "communicatively coupled" to another element, it can be directly connected or coupled to the other element, or intervening elements may be present. In contrast, when an element is referred to as being "directly connected" or "directly coupled" to another ele-

ment, there are no intervening elements present. Additionally, like numbers refer to like elements throughout. Reference will now be made in detail to the subject matter disclosed, which is illustrated in the accompanying figures.

[0012] FIGS. 1 through 6 illustrate an example portable laparoscope 100. As shown, the portable laparoscope 100 includes a housing 102 and an elongated tube 104 coupled to the housing 102. The housing can be configured to support an insufflator 106. A light source 108 and a camera 110 are disposed proximate to a first end 112 of the elongated tube 104 coupled to the housing 102. The housing 102 is also configured to hold image display apparatus 114, that can be configured to display the images acquired by the camera 110 and/or transmit the images to a remote display device. A power source 116 is disposed in the housing 102 to provide sufficient operational power to the electronic devices disposed in the portable laparoscope 100 (e.g., light source 108, camera 110, image display apparatus 114, etc.). The housing 102 may be fabricated of a medical grade material such as titanium. However, titanium is provided by way of example only, and is not meant to be restrictive of the disclosure. Thus, other materials medical grade materials may be used to construct the housing 102, the elongated tube 104, and so forth.

[0013] The elongated tube 104 may be configured in a variety of ways. As shown, the elongated tube 104 includes a first end 112 and a second end 118. The first end 112 is defined by the end of the elongated tube 104 distal from the housing 102. In implementations, a light source 108 and a camera 110 are disposed of the elongated tube 104 proximate to the first end 112. In some implementations, the light source 108 and/or the camera 110 can be disposed of the elongated tube 104 proximate to the second end 118. In this type of configuration, lenses, fiber optic cables, and the like can be used to direct light to and from the light source 108 and/or the camera 110 along the length of the elongated tube 104. The light source 108 and/or the camera 110 can also be positioned within the housing 102. A window formed of generally transparent material is disposed at the first end 112 to provide a protective cover for the light source 108 and the camera 110 and other equipment within the elongated tube 104. In embodiments, the generally transparent material may be comprised of quartz, or the like.

[0014] The second end 118 of the elongated tube 104 is coupled to the housing 102 using, for example, a threaded fitting. The fitting can be used to provide articulation between the housing 102 and the elongated tube 104. For example, the fitting can be implemented as a joint. The second end 118 may also be welded to or fastened to the threaded fitting. In an implementation, the elongated tube 104 may comprise an approximately fourteen inch (14") (355.6 millimeters) long tube that is ten millimeters (10 mm) (0.39 inches) in diameter. The elongated tube 104 may also be comprised of a rigid material (e.g., titanium), a flexible material (e.g., medical nylon),

or other medical grade materials. In some implementations, the elongated tube 104 can be configured to extend and retract. For example, the elongated tube 104 can be configured to telescope, and/or to retract into the housing 102.

[0015] The insufflator 106 is used to supply a gas (e.g., CO₂) to the abdominal cavity to lift abdominal integument from the internal organs proximate to the first end 112 of the elongated tube 104. The insufflator 106 is either a cartridge-based insufflator, a gas cylinder-based insufflator or an infusion balloon-based insufflator. The insufflator 106 can be disposed or housed within the housing 102.

[0016] The light source 108 may assume a variety of configurations. For example, the light source 108 may be comprised of a light emitting diode (LED), a laser diode, quantum dots, multiple light emitting diodes, multiple laser diodes, or the like. In an implementation, the light source 108 is disposed at the first end 112 proximate to a camera 110, and the power source 116 is coupled (e.g., wired configuration, etc.) to the light source 108 to provide sufficient operational power to the light source 108. When the portable laparoscope 100 is in use, the light source 108 is configured to emit a light to illuminate an area within a field of view of the camera 110.

[0017] The camera 110 may be configured in a variety of ways. The camera 110 may, for example, be comprised of: a pin hole camera, a charge coupled device (CCD) camera, a fiber optic coupled camera, a video camera, and so forth. The camera 110 is configured to capture an image in the camera's field of view. The camera 110 is disposed proximate to the first end 112 and coupled to the power source 116. In an implementation, the camera 110 may be part of a group of multiple cameras 110 disposed proximate to the first end 112 and coupled to the power source 116. As illustrated in FIG. 4F, multiple cameras 110 can be disposed at different locations of the first end 112 to capture multiple images from different angles. The multiple cameras 110 may also be arranged in such a configuration that provides a stereoscopic view of the captured images when displayed.

[0018] The camera 110 is configured to communicate with image display apparatus 114. For example, one or more cameras 110 may be communicatively coupled to an electronic device (e.g. a display 122, etc.) via a wired configuration, a fiber optic communication, a transmitter/receiver link, or the like. In an implementation, the camera 110 is configured to transfer the captured image data to an image display apparatus 114 disposed of the housing 102.

[0019] The image display apparatus 114 may assume a wide variety of configurations, as illustrated in FIGS. 4A through 4E. The image display apparatus 114 is configured to display images captured by cameras 110 and/or to transmit the images to a remote display device. For example, the image display apparatus 114 may include, but is not necessarily limited to: a transmitter 120 configured to transmit captured images; a display 122,

such as a liquid crystal display (LCD) device or a projection device; and so forth. The camera 110 and the image display apparatus 114 are communicatively coupled together via a wired configuration, a wireless configuration, a fiber optic configuration, or the like.

[0020] In an implementation, the image display apparatus 114 may be configured as a display 122 disposed of (e.g., housed within) the housing 102. For example, the display 122 may be a flip-screen display device, as illustrated in FIG. 4A. As shown, the flip-screen display device may be configured to pivot from a substantially folded position for transportation and storage to a substantially upright position for viewing purposes. In another example, the display 122 may be coupled to the elongated tube 104 (shown in FIGS. 4C, 4D, and 4G). For instance, the housing 102 may include an aperture to allow viewing of the display portion of the display 122. It is contemplated that the display 122 may be a display device of varying dimensions. For example, the display 122 may be comprised of an approximately 2.5 inch (6.35 centimeter) diagonal LCD device, an approximately 5.8 inch (14.73 centimeters) diagonal LCD device, and so forth. The display 122 may present the captured image(s) as individual images for a predetermined amount of time. The captured images may also be presented as a sequence of images (e.g., video). In another implementation, the display 122 may comprise a projection device, such as a liquid crystal display (LCD) projector, or the like. The housing 102 may be configured to house the projection device. In an implementation, the projection device is configured to project images as a virtual screen to a viewing area. The viewing area may include, but is not necessarily limited to: a projection screen, a wall, or another projection viewing medium.

[0021] As illustrated in FIG. 1, the image display apparatus 114 may comprise a transmitter 120. The transmitter 120 may be configured in a variety of ways. For example, the transmitter 120 may be a Radio Frequency (RF) transmitter configured to transmit one or more images captured by camera 110 via a RF network (e.g., Bluetooth, Wi-Fi, etc.). In another example, the transmitter 120 may comprise a laser diode configured to transmit one or more image(s) via a free-space optical network. The transmitter 120 may be housed within the housing 102 and coupled to power source 116.

[0022] The transmitter 120 can be configured to transmit one or more captured image(s) to a remote display device. The remote display device may be configured in a variety of ways. In an implementation, the remote display device may be comprised of an image display device 124. The image display device 124 may be a monitor (e.g., LCD device, High Definition (HD) display device, etc.) communicatively coupled (e.g., wired configuration, wireless configuration, etc.) to a receiver 126. A receiver 126 is configured to receive the one or more image(s) transmitted by the transmitter 120 and to provide the one or more image(s) to the image display device 124. The receiver 126 may be implemented in a number of ways.

For example, the receiver 126 may be a RF receiver configured to receive images from a RF transmitter. In another example, the receiver 126 may be an avalanche photodiode configured to receive images from a laser diode.

[0023] In an implementation, the receiver 126 is configured to receive the image(s) transmitted by the transmitter 120 and to furnish the images to the image display device 124 via a wired configuration. For example, the receiver 126 and image display device 124 may be located in a separate area (e.g., building, room, etc.) from the transmitter 120 and portable laparoscope 100.

[0024] It is contemplated that a mobile device 128 may be used to view the image(s) furnished by camera 110. In an implementation, mobile device 128 may be coupled to elongated tube 104 via a wired configuration as illustrated in FIG. 4B. In another implementation, the transmitter 120 may be configured to transmit the captured image(s) to a detachable mobile device 128 via a network 130 as illustrated in FIG. 4E. The mobile device 128 may be configured in a variety of ways. For instance, the mobile device 128 may be configured as a mobile phone, a smart phone, a laptop computing device, and so forth. The mobile device 128 may include a display 132. In an implementation, the display 132 may be integral with the mobile device 128. In another implementation, the display 132 may be coupled to the mobile device 128 via a wired configuration. For example, the transmitter 120 may transmit the captured image(s) to a mobile phone 128 via the network 130. The mobile phone 128 furnishes the captured image(s) to the display 132 for display. In another example, the transmitter 120 may transmit the captured image(s) to a laptop computer 128 via the network 130. The laptop 128 furnishes the captured image(s) to the display 132 for display.

[0025] The network 130 is representative of a variety of different communication pathways and network connections that may be employed, individually or in combinations, to communicate among the components of the portable laparoscope 100. Further, network 130 is representative of a variety of different types of networks and connections that are contemplated including, but not necessarily limited to: the Internet; an intranet; a satellite network; a cellular network; a mobile data network; wired and/or wireless connections; and so forth.

[0026] Examples of wireless networks include, but are not necessarily limited to: a free-space optical transmission network, a wireless LED network, as well as networks configured for communications according to: one or more standard of the Institute of Electrical and Electronics Engineers (IEEE), such as 802.11 or 802.16 (Wi-Max) standards; Wi-Fi standards promulgated by the Wi-Fi Alliance; Bluetooth standards promulgated by the Bluetooth Special Interest Group; and so on. Wired communications are also contemplated such as through universal serial bus (USB), Ethernet, serial connections, and so forth. As illustrated in FIG. 1, the portable laparoscope 100 includes a power source 116. In an implementation,

the power source 116 may comprise a battery that is configured to provide sufficient operational power to the various electronic components associated with or coupled to the portable laparoscope 100. For instance, in an implementation, the battery provides sufficient operational power to operate the image display apparatus 114, the insufflator 106, the camera 110, and the light source 108. It is contemplated that sufficient operational power may be defined as each electronic device powered by the battery receiving enough power to be fully operational according to the specifications of each device for a definite amount of time.

[0027] In FIG. 1, the laparoscope 100 is depicted as including a processor 134 and a memory 136. The processor 134 provides processing functionality for the portable laparoscope 100 and may include any number of processors, micro-controllers, or other processing systems and resident or external memory for storing data and other information accessed or generated by portable laparoscope 100. The processor 134 is configured to execute one or more software program(s). The processor 134 is not limited by the materials from which it is formed or the processing mechanisms employed therein and, as such, may be implemented via semiconductor(s) and/or transistors (e.g., electronic Integrated Circuits (ICs)), and so forth.

[0028] The memory 136 is an example of tangible computer-readable media that provides storage functionality to store various data associated with the operation of the portable laparoscope 100, such as the software program and code segments mentioned above, or other data to instruct the processor 134 and other elements of the portable laparoscope 100 to perform the steps described herein. Although a single memory 136 is shown, a wide variety of types and combinations of memory may be employed. The memory 136 may be integral with the processor 134, stand-alone memory, or a combination of both. The memory may include, for example, removable and non-removable memory elements such as Random Access Memory (RAM), Read Only Memory (ROM), Flash memory (e.g., an SD Card, a mini-SD card, a micro-SD Card), magnetic memory, optical memory, USB memory devices, and so forth.

[0029] As depicted in FIG. 1, the housing 102 includes a memory interface 138. The memory interface 138 provides removable storage functionality to portable laparoscope 100. For instance, the memory interface 138 is configured to detect when a removable memory element has been positioned or inserted into memory interface 138. The memory interface 138 is configured to receive the image(s) and/or the video from the camera 110 and furnish the image(s) and/or the video to the removable memory element for storage. The image(s) may be transferred via a protocol implemented in software, hardware, and/or firmware. The removable memory elements may include, but are not necessarily limited to: SD Cards, mini-SD cards, micro-SD Cards, USB drives, or the like. In this configuration, processor 134 may be housed in the

housing 102 as a standalone processor, a processor integral with the camera 110, or a processor integral with the memory interface 138. The processor 134 may provide processing functionality to the portable laparoscope 100, the camera 110, and/or the memory interface 138.

[0030] FIGS. 2 and 3 illustrate example implementations of portable laparoscopes in accordance with the present disclosure. FIG. 2 depicts a portable laparoscope 100 used in a non-dedicated surgical environment. For instance, medical personnel (not shown) may use laparoscope 100 to perform a laparoscopic procedure on a patient. Medical personnel may insert end 112 through an incision made in patient. As shown in FIG. 3, end 112 includes light source 108 and camera 110. As described above, the light source will provide illumination to the area within the camera's 110 field of view. The camera 110 furnishes one or more image(s) to the image display apparatus 114 (depicted as display 122 in FIGS. 2 and 3) for medical personnel to view. In another implementation, as illustrated in FIG. 4C, portable laparoscope 100 may be manipulated by medical personnel to provide further camera 110 views and so forth. Moreover, portable laparoscope 100 may implemented with ergonomic designs. For instance, as illustrated in FIG. 4G, a handle 142 may be coupled to display 122.

[0031] Referring now to FIGS. 5 and 6, the insufflator 106 comprises a portable gas supply 144 coupled to a gas tube 140. The portable gas supply 144 may comprise a portable gas cartridge, a portable gas tank, or the like. A gas regulator 146 is disposed between the portable gas supply 144 and the gas tube 140. The gas regulator 146 is configured to interface with the portable gas supply 144 and to regulate the gas flow released into the gas tube 140 from the portable gas supply 144. In an implementation, the gas regulator 146 may be comprised of a high pressure gas regulator or the like. For example, a high pressure gas regulator may include a FISHER-BRAND Multistage Cylinder Regulator, or the like. In an implementation, the gas regulator 146 may be configured to reduce the flow rate of the gas to low variable pressures. In a further implementation, the gas regulator 146 may be coupled, or connected, to a flow meter (not shown) to monitor the flow rate of the insufflator 106. The flow meter may comprise a Smith Flowmeter Regulator, or the like. In one implementation, the gas tube 140 may be disposed, or housed, within the elongated tube 104. In another implementation, the gas tube 140 may be a standalone gas tube 140.

[0032] In an implementation, as illustrated in FIGS. 5 and 6, the laparoscope 100 may also include a trocar hook-up 148 and a trocar 150. The trocar hook-up 148 provides an interface with the gas tube 140 proximate to the first end 112 of the elongated tube 104. The trocar 150 is configured to make an incision in a patient and is also coupled proximate to the elongated tube 104 and the trocar hook-up 148. Once an incision has been created, the first end 112 of the elongated tube 104 may then be inserted through the incision to allow the camera

110 to provide imagery of the body cavity. It is contemplated that the trocar 150 may be any trocar known in the art and may be interchangeable with other types of trocars. In a further implementation, as illustrated in FIG. 6, the light source 108 and the camera 110 may be disposed proximate to the trocar 150. For instance, the trocar 150 may include the light source 108 and the camera 110 and provide illumination functionality and image capture functionality once the trocar 150 has been inserted through the incision in the patient.

Conclusion

[0033] Although the subject matter has been described in language specific to structural features and/or process operations, it is to be understood that the subject matter defined in the appended claims is not necessarily limited to the specific features or acts described above. Rather, the specific features and acts described above are disclosed as example forms of implementing the claims.

Claims

1. A portable laparoscope system (100) comprising:

a housing (102);
 an elongated tube (104) comprising a first end (112) and a second end (118), the second end (118) of the elongated tube coupled to the housing (102), the elongated tube configured for at least partial insertion into a body cavity;
 an image capture device (110) disposed at the first end (112) of the elongated tube, the image capture device (110) configured to capture an image within a field of view of the image capture device (110);
 a light source (108) disposed at the first end (112) of the elongated tube, the light source (108) configured to emit a light proximate to an area within the field of view of the image capture device (110);
 an insufflator (106) configured to supply and provide a gas for inflating a body cavity into which the elongated tube is inserted, said insufflator (106) comprising a portable gas supply (144); a gas tube (140) for transporting gas from the portable gas supply; and a gas regulator (146) disposed between the portable gas supply (144) and the gas tube (140); and said insufflator (106) being cartridge-based, gas cylinder-based or infusion balloon-based;
 an image display apparatus (114) disposed of the housing (102) and coupled with the image capture device (110) for at least one of displaying or transmitting an image of a body cavity captured by the image capture device (110);
 a power source (116) disposed in the housing

(102) and coupled to the light source (108), the image capture device (110), the insufflator (106), and the image display apparatus (114), the power source (116) configured to provide a sufficient operational power to the light source (108), the image capture device (110), the insufflator (106), and the image display apparatus (114); and wherein the power source (116) comprises a battery.

2. The portable laparoscope system (100) as recited in claim 1, wherein the image display apparatus (114) comprises a transmitter (120) communicatively coupled to the image capture device (110), the transmitter (120) being configured to transmit the image to a receiver (126) communicatively coupled to an image display device (124).

3. The portable laparoscope system (100) as recited in claim 1, wherein the image display apparatus (114) comprises a display (122) configured to display the image.

4. The portable laparoscope system (100) as recited in claim 3, wherein the display (122) comprises a liquid crystal display device.

5. The portable laparoscope system (100) as recited in claim 2, wherein the transmitter (120) is configured to transmit the image via a wireless network (130); preferably wherein the wireless network (130) conforms to 802.11 standards and, preferably, the wireless network (130) comprises a free-space optical transmission network.

6. The portable laparoscope system (100) as recited in claim 1, the insufflator (106) further comprising:

a gas tube (140) for transporting gas from the portable gas supply (144); and
 a gas regulator (146) disposed between the portable gas supply (144) and the gas tube (140).

7. The portable laparoscope system (100) as recited in claim 1, wherein the insufflator (106) is disposed in the housing (102).

8. The portable laparoscope system (100) as recited in claim 1, further comprising:
 a memory interface (138) disposed of the housing (102), the memory interface (138) configured to receive a removable memory element.

9. The portable laparoscope system (100) as recited in claim 1, wherein the image display apparatus (114) comprises a projection device.

10. The portable laparoscope system (100) as recited in

claim 1, wherein the image display apparatus (114) and the image capture device (110) are communicatively coupled via a wired configuration.

11. A portable laparoscope system (100) comprising:

an elongated tube (104) comprising a first end (112) and a second end (118), the first end of the elongated tube (104) configured for at least partial insertion into a body cavity;

a housing (102) for supporting the elongated tube (104), the housing (102) coupled with the second end (118) of the elongated tube (104); an image capture device (110) disposed at the first end (112) of the elongated tube (104), the image capture device (110) configured to capture an image within a field of view of the image capture device (110);

a light source (108) disposed at the first end (112) of the elongated tube (104), the light source (108) configured to emit a light proximate to an area within the field of view of the image capture device (110);

an insufflator (106) configured to supply and provide a gas for inflating a body cavity into which the elongated tube (104) is inserted, said insufflator (106) comprising a portable gas supply (144); a gas tube (140) for transporting gas from the portable gas supply; and a gas regulator (146) disposed between the portable gas supply (144) and the gas tube (140); and said insufflator (106) being cartridge-based, gas cylinder-based or infusion balloon-based;

a transmitter (120) disposed of the housing (102) and communicatively coupled with the image capture device (110) for transmitting an image of a body cavity captured by the image capture device (110) to a receiver (126) coupled to an image display device (124); and

a power source (116) disposed in the housing (102) and coupled to the light source (108), the image capture device (110), the insufflator (106) and the transmitter (120), the power source (116) configured to provide a sufficient operational power to the light source (108), the image capture device (110), the insufflator (106) and the transmitter (120); and wherein the power source (116) comprises a battery.

12. The portable laparoscope system (100) as recited in claim 11, wherein the transmitter (120) is configured to transmit the image via a wireless network (130).

13. The portable laparoscope system (100) as defined in claim 12, wherein the wireless network (130) comprises a free-space optical transmission network.

Patentansprüche

1. Tragbares Laparoskopsystem (100), das Folgendes umfasst:

ein Gehäuse (102);

eine längliche Röhre (104) mit einem ersten Ende (112) und einem zweiten Ende (118), wobei das zweite Ende (118) der länglichen Röhre mit dem Gehäuse (102) gekoppelt ist, wobei die längliche Röhre zum zumindest teilweisen Einführen in eine Körperhöhle konfiguriert ist;

eine Bilderfassungsvorrichtung (110), die am ersten Ende (112) der länglichen Röhre angeordnet ist, wobei die Bilderfassungsvorrichtung (110) so konfiguriert ist, dass sie ein Bild innerhalb eines Sichtfeldes der Bilderfassungsvorrichtung (110) erfasst;

eine Lichtquelle (108), die am ersten Ende (112) der länglichen Röhre angeordnet ist, wobei die Lichtquelle (108) so konfiguriert ist, dass sie ein Licht in der Nähe eines Bereichs innerhalb des Sichtfeldes der Bilderfassungsvorrichtung (110) ausstrahlt;

einen Insufflator (106), der so konfiguriert ist, dass er ein Gas zum Aufblasen einer Körperhöhle, in die die längliche Röhre eingeführt ist, zuführt und bereitstellt, wobei der genannte Insufflator (106) eine tragbare Gasversorgung (144); eine Gasröhre (140) für den Transport von Gas aus der tragbaren Gasversorgung; und einen Gasregler (146) umfasst, der zwischen der tragbaren Gasversorgung (144) und der Gasröhre (140) angeordnet ist; und der genannte Insufflator (106) Kartuschen-, Gasflaschen- oder Infusionsballon-basiert ist;

eine Bildanzeigeeinheit (114), die an dem Gehäuse (102) angeordnet und mit der Bilderfassungsvorrichtung (110) gekoppelt ist, um ein von der Bilderfassungsvorrichtung (110) erfasstes Bild einer Körperhöhle anzuzeigen und/oder zu übertragen;

eine Stromquelle (116), die im Gehäuse (102) angeordnet und mit der Lichtquelle (108), der Bilderfassungsvorrichtung (110), dem Insufflator (106) und der Bildanzeigeeinheit (114) gekoppelt ist, wobei die Stromquelle (116) so konfiguriert ist, dass sie die Lichtquelle (108), die Bilderfassungsvorrichtung (110), den Insufflator (106) und die Bildanzeigeeinheit (114) mit einer ausreichenden Betriebsenergie versorgt; und wobei die Stromquelle (116) eine Batterie umfasst.

2. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei die Bildanzeigeeinheit (114) einen Sender (120) umfasst, der mit der Bilderfassungsvorrichtung (110) in Verbindung steht, wobei der Sender

- (120) so konfiguriert ist, dass er das Bild zu einem Empfänger (126) überträgt, der kommunikativ mit einer Bildanzeigevorrichtung (124) gekoppelt ist.
3. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei die Bildanzeigevorrichtung (114) ein Display (122) umfasst, das zum Anzeigen des Bildes konfiguriert ist. 5
 4. Tragbares Laparoskopsystem (100) nach Anspruch 3, wobei das Display (122) eine Flüssigkristallanzeigevorrichtung umfasst. 10
 5. Tragbares Laparoskopsystem (100) nach Anspruch 2, wobei der Sender (120) so konfiguriert ist, dass er das Bild über ein drahtloses Netzwerk (130) überträgt; wobei das drahtlose Netzwerk (130) vorzugsweise 802.11-Standards entspricht und das drahtlose Netzwerk (130) vorzugsweise ein optisches Freiraumübertragungsnetzwerk umfasst. 15 20
 6. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei der Insufflator (106) ferner Folgendes umfasst: 25
 - eine Gasröhre (140) für den Transport von Gas aus der tragbaren Gasversorgung (144); und
 - einen Gasregler (146), der zwischen der tragbaren Gasversorgung (144) und der Gasröhre (140) angeordnet ist. 30
 7. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei der Insufflator (106) im Gehäuse (102) angeordnet ist. 35
 8. Tragbares Laparoskopsystem (100) nach Anspruch 1, das ferner Folgendes umfasst: 40
 - eine Speicherschnittstelle (138), die an dem Gehäuse (102) angeordnet ist, wobei die Speicherschnittstelle (138) zur Aufnahme eines entfernbaren Speicherelements konfiguriert ist. 45
 9. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei die Bildanzeigevorrichtung (114) eine Projektionsvorrichtung umfasst. 50
 10. Tragbares Laparoskopsystem (100) nach Anspruch 1, wobei die Bildanzeigevorrichtung (114) und die Bilderfassungsvorrichtung (110) über eine verdrahtete Konfiguration kommunikativ gekoppelt sind. 55
 11. Tragbares Laparoskopsystem (100), das Folgendes umfasst:
 - eine längliche Röhre (104), die ein erstes Ende (112) und ein zweites Ende (118) umfasst, wobei das erste Ende der länglichen Röhre (104) für ein zumindest teilweises Einführen in eine

Körperhöhle konfiguriert ist;
 ein Gehäuse (102) zum Tragen der länglichen Röhre (104), wobei das Gehäuse (102) mit dem zweiten Ende (118) der länglichen Röhre (104) gekoppelt ist;
 eine Bilderfassungsvorrichtung (110), die am ersten Ende (112) der länglichen Röhre (104) angeordnet ist, wobei die Bilderfassungsvorrichtung (110) so konfiguriert ist, dass sie ein Bild innerhalb eines Sichtfeldes der Bilderfassungsvorrichtung (110) erfasst;
 eine Lichtquelle (108), die am ersten Ende (112) der länglichen Röhre (104) angeordnet ist, wobei die Lichtquelle (108) so konfiguriert ist, dass sie ein Licht in der Nähe eines Bereichs innerhalb des Sichtfeldes der Bilderfassungsvorrichtung (110) ausstrahlt;
 einen Insufflator (106), der so konfiguriert ist, dass er ein Gas zum Aufblasen einer Körperhöhle, in die die längliche Röhre (104) eingeführt ist, zuführt und bereitstellt, wobei der genannte Insufflator (106) eine tragbare Gasversorgung (144); eine Gasröhre (140) für den Transport von Gas aus der tragbaren Gasversorgung; und einen Gasregler (146) umfasst, der zwischen der tragbaren Gasversorgung (144) und der Gasröhre (140) angeordnet ist; und der genannte Insufflator (106) Kartuschen-, Gasflaschen- oder Infusionsballon-basiert ist;
 einen Sender (120), der an dem Gehäuse (102) angeordnet und mit der Bilderfassungsvorrichtung (110) kommunikativ gekoppelt ist, um ein von der Bilderfassungsvorrichtung (110) erfasstes Bild einer Körperhöhle zu einem Empfänger (126) zu übertragen, der mit einer Bildanzeigevorrichtung (124) gekoppelt ist; und
 eine Stromquelle (116), die in dem Gehäuse (102) angeordnet und mit der Lichtquelle (108), der Bilderfassungsvorrichtung (110), dem Insufflator (106) und dem Sender (120) gekoppelt ist, wobei die Stromquelle (116) so konfiguriert ist, dass sie die Lichtquelle (108), die Bilderfassungsvorrichtung (110), den Insufflator (106) und den Sender (120) mit einer ausreichenden Betriebsenergie versorgt; und wobei die Stromquelle (116) eine Batterie umfasst.

12. Tragbares Laparoskopsystem (100) nach Anspruch 11, wobei der Sender (120) so konfiguriert ist, dass das Bild über ein drahtloses Netzwerk (130) übertragen wird.
13. Tragbares Laparoskopsystem (100) nach Anspruch 12, wobei das drahtlose Netzwerk (130) ein optisches Freiraumübertragungsnetzwerk umfasst.

Revendications

1. Système de laparoscope portable (100) comprenant :

un boîtier (102) ;
 un tube allongé (104) comprenant une première extrémité (112) et une deuxième extrémité (118), la deuxième extrémité (118) du tube allongé couplé au boîtier (102), le tube allongé configuré pour une insertion au moins partielle jusque dans une cavité corporelle ;
 un dispositif de capture d'image (110) disposé au niveau de la première extrémité (112) du tube allongé, le dispositif de capture d'image (110) configuré pour capturer une image au sein d'un champ de vision du dispositif de capture d'image (110) ;
 une source de lumière (108) disposée au niveau de la première extrémité (112) du tube allongé, la source de lumière (108) configurée pour émettre une lumière à proximité d'une zone au sein du champ de vision du dispositif de capture d'image (110) ;
 un insufflateur (106) configuré pour acheminer et fournir un gaz destiné à gonfler une cavité corporelle jusque dans laquelle le tube allongé est inséré, ledit insufflateur (106) comprenant une alimentation en gaz portable (144) ; un tube à gaz (140) destiné à transporter du gaz à partir de l'alimentation en gaz portable ; et un régulateur de gaz (146) disposé entre l'alimentation en gaz portable (144) et le tube à gaz (140) ; et ledit insufflateur (106) étant à base de cartouche, à base de cylindre de gaz ou à base de ballonnet de perfusion ;
 un appareil d'affichage d'image (114) disposé sur le boîtier (102) et couplé avec le dispositif de capture d'image (110) destiné à au moins une action parmi l'affichage ou l'émission d'une image d'une cavité corporelle capturée par le dispositif de capture d'image (110) ;
 une source de puissance (116) disposée dans le boîtier (102) et couplée à la source de lumière (108), au dispositif de capture d'image (110), à l'insufflateur (106), et à l'appareil d'affichage d'image (114), la source de puissance (116) configurée pour fournir une puissance de fonctionnement suffisante à la source de lumière (108), au dispositif de capture d'image (110), à l'insufflateur (106), et à l'appareil d'affichage d'image (114) ; et dans lequel la source de puissance (116) comprend une batterie.

2. Système de laparoscope portable (100) selon la revendication 1, dans lequel l'appareil d'affichage d'image (114) comprend un émetteur (120) couplé en communication au dispositif de capture d'image

(110), l'émetteur (120) étant configuré pour émettre l'image à un récepteur (126) couplé en communication à un dispositif d'affichage d'image (124).

3. Système de laparoscope portable (100) selon la revendication 1, dans lequel l'appareil d'affichage d'image (114) comprend un affichage (122) configuré pour afficher l'image.

4. Système de laparoscope portable (100) selon la revendication 3, dans lequel l'affichage (122) comprend un dispositif d'affichage à cristaux liquides.

5. Système de laparoscope portable (100) selon la revendication 2, dans lequel l'émetteur (120) est configuré pour émettre l'image via un réseau sans fil (130) ; préférentiellement dans lequel le réseau sans fil (130) est conforme aux normes 802.11 et, préférentiellement, le réseau sans fil (130) comprend un réseau d'émission optique en espace libre.

6. Système de laparoscope portable (100) selon la revendication 1, l'insufflateur (106) comprenant en outre :

un tube à gaz (140) destiné à transporter du gaz à partir de l'alimentation en gaz portable (144) ; et
 un régulateur de gaz (146) disposé entre l'alimentation en gaz portable (144) et le tube à gaz (140) .

7. Système de laparoscope portable (100) selon la revendication 1, dans lequel l'insufflateur (106) est disposé dans le boîtier (102).

8. Système de laparoscope portable (100) selon la revendication 1, comprenant en outre : une interface mémoire (138) disposée sur le boîtier (102), l'interface mémoire (138) configurée pour recevoir un élément de mémoire amovible.

9. Système de laparoscope portable (100) selon la revendication 1, dans lequel l'appareil d'affichage d'image (114) comprend un dispositif de projection.


10. Système de laparoscope portable (100) selon la revendication 1, dans lequel l'appareil d'affichage d'image (114) et le dispositif de capture d'image (110) sont couplés en communication via une configuration câblée.

11. Système de laparoscope portable (100) comprenant :

un tube allongé (104) comprenant une première extrémité (112) et une deuxième extrémité (118), la première extrémité du tube allongé

(104) configurée pour une insertion au moins partielle dans une cavité corporelle ;
 un boîtier (102) destiné à supporter le tube allongé (104), le boîtier (102) couplé avec la deuxième extrémité (118) du tube allongé (104) ;
 un dispositif de capture d'image (110) disposé au niveau de la première extrémité (112) du tube allongé (104), le dispositif de capture d'image (110) configuré pour capturer une image au sein d'un champ de vision du dispositif de capture d'image (110) ;
 une source de lumière (108) disposée au niveau de la première extrémité (112) du tube allongé (104), la source de lumière (108) configurée pour émettre une lumière à proximité d'une zone au sein du champ de vision du dispositif de capture d'image (110) ;
 un insufflateur (106) configuré pour acheminer et fournir un gaz destiné à gonfler une cavité corporelle jusque dans laquelle le tube allongé (104) est inséré, ledit insufflateur (106) comprenant une alimentation en gaz portable (144) ; un tube à gaz (140) destiné à transporter du gaz à partir de l'alimentation en gaz portable ; et un régulateur de gaz (146) disposé entre l'alimentation en gaz portable (144) et le tube à gaz (140) ; et ledit insufflateur (106) étant à base de cartouche, à base de cylindre de gaz ou à base de ballonnet de perfusion ;
 un émetteur (120) disposé sur le boîtier (102) et couplé en communication avec le dispositif de capture d'image (110) destiné à émettre une image d'une cavité corporelle capturée par le dispositif de capture d'image (110) à un récepteur (126) couplé à un dispositif d'affichage d'image (124) ; et
 une source de puissance (116) disposée dans le boîtier (102) et couplée à la source de lumière (108), au dispositif de capture d'image (110), à l'insufflateur (106) et à l'émetteur (120), la source de puissance (116) configurée pour fournir une puissance de fonctionnement suffisante à la source de lumière (108), au dispositif de capture d'image (110), à l'insufflateur (106) et à l'émetteur (120) ; et dans lequel la source de puissance (116) comprend une batterie.

12. Système de laparoscope portable (100) selon la revendication 11, dans lequel l'émetteur (120) est configuré pour émettre l'image via un réseau sans fil (130) .
13. Système de laparoscope portable (100) tel que défini dans la revendication 12, dans lequel le réseau sans fil (130) comprend un réseau d'émission optique en espace libre.

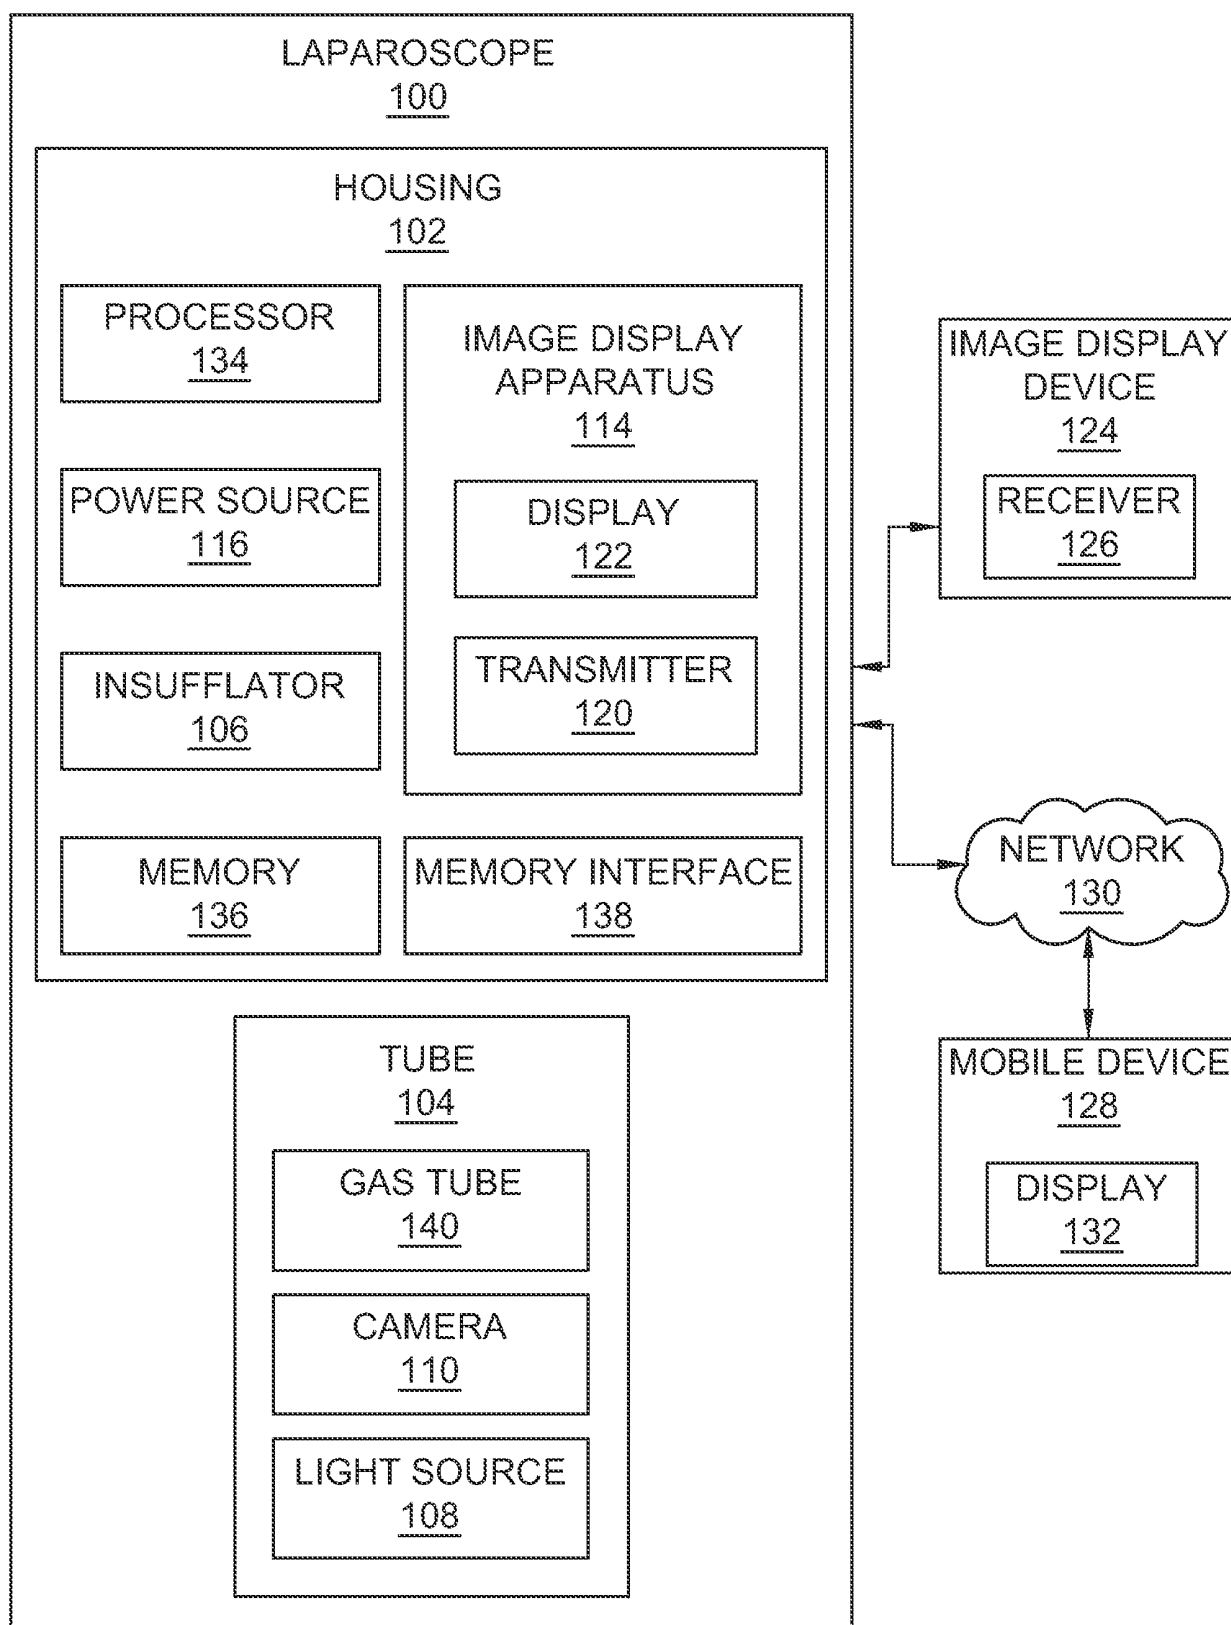**FIG. 1**

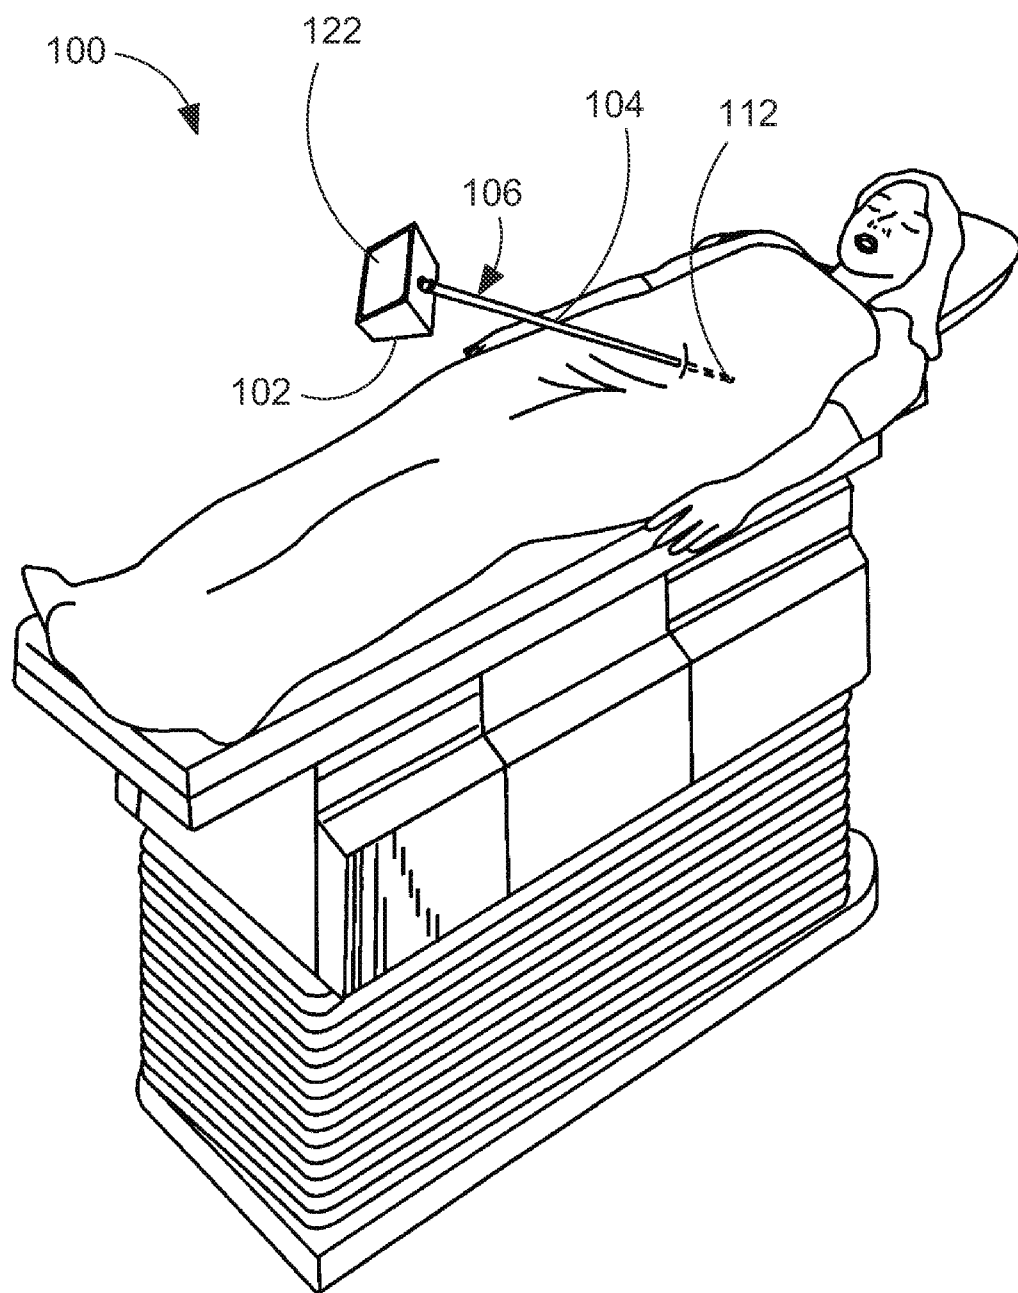
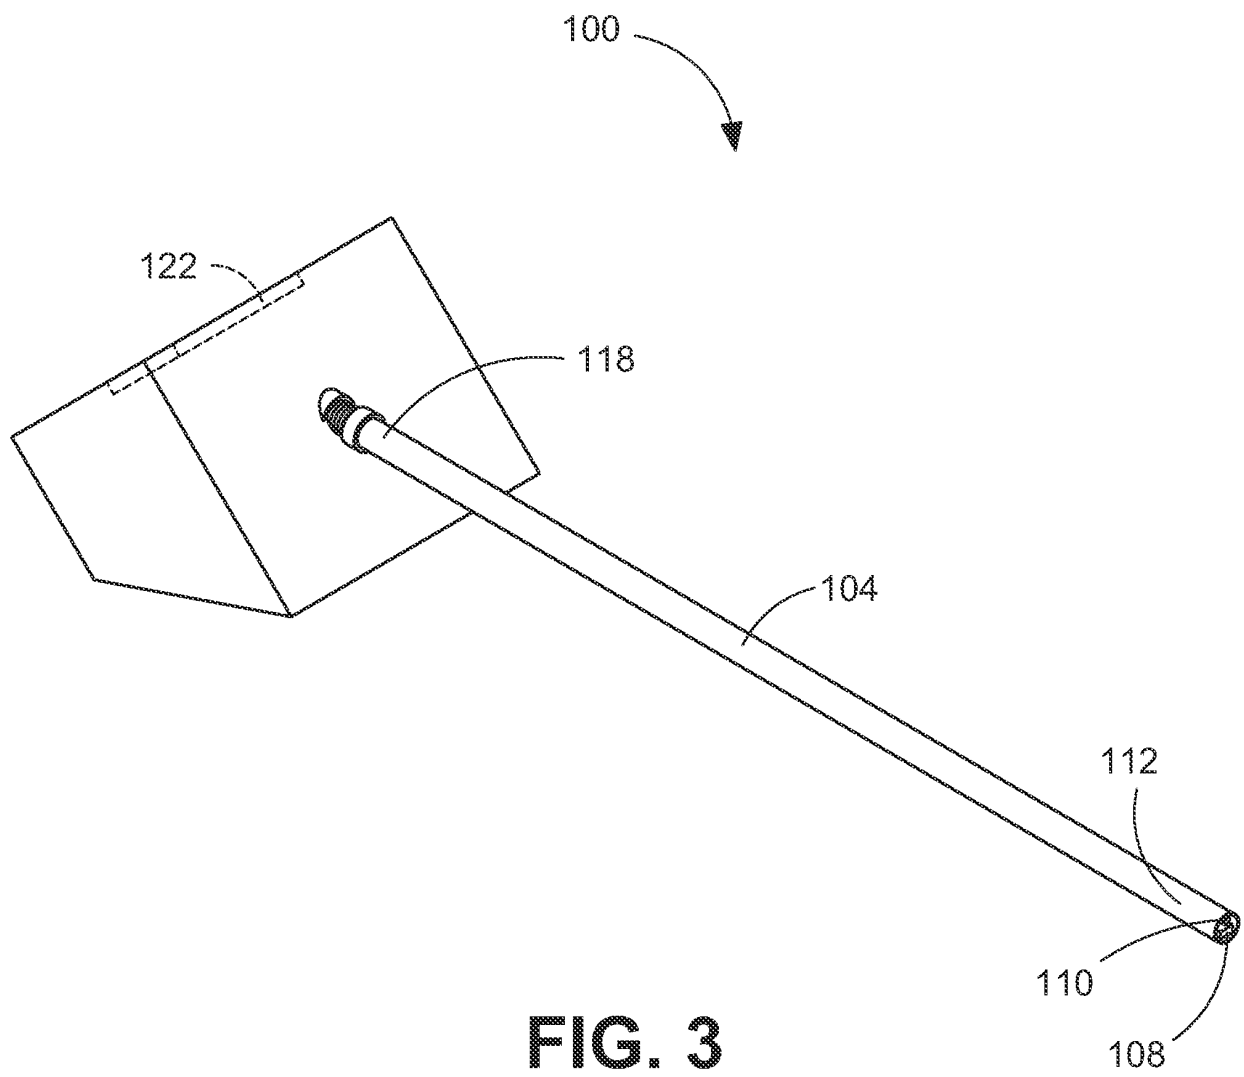


FIG. 2



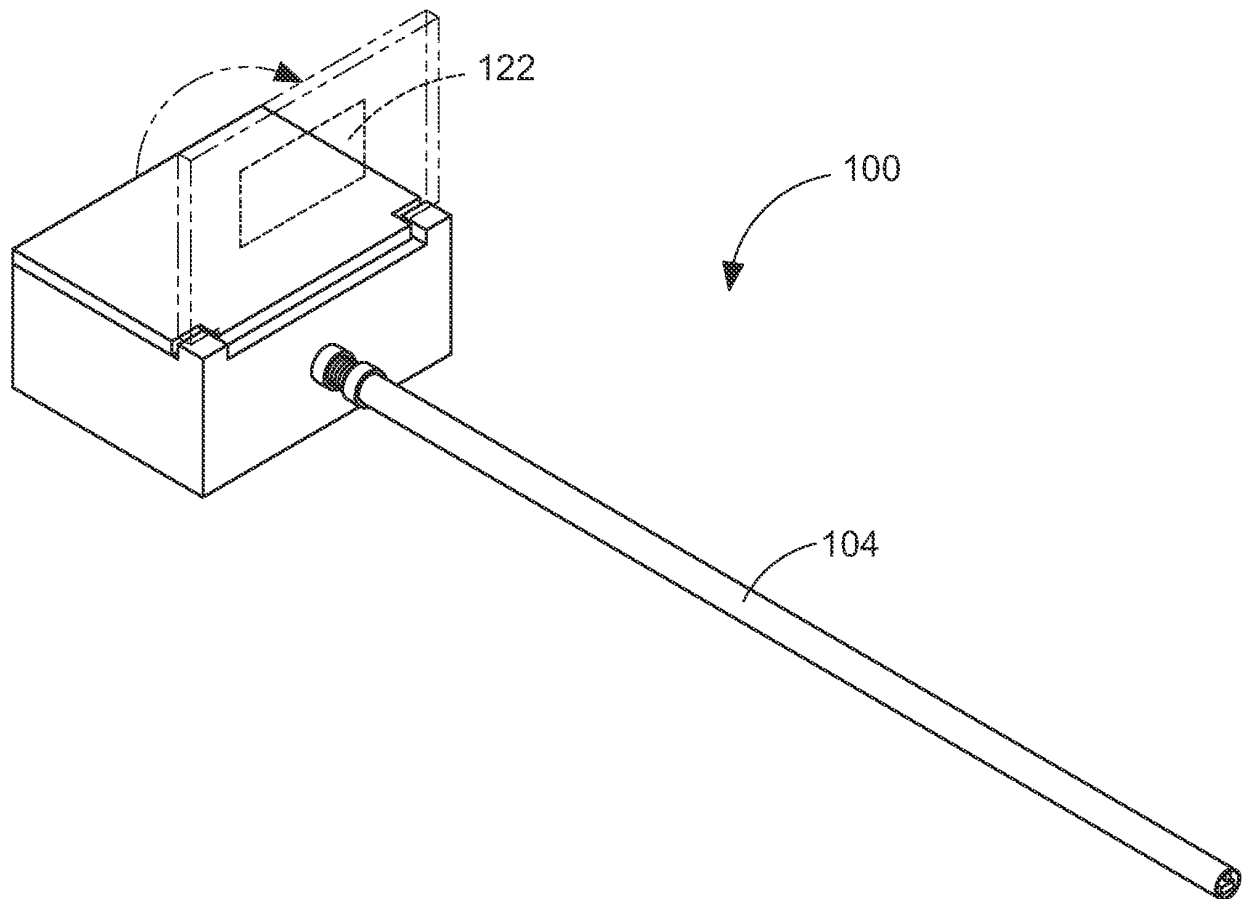


FIG. 4A

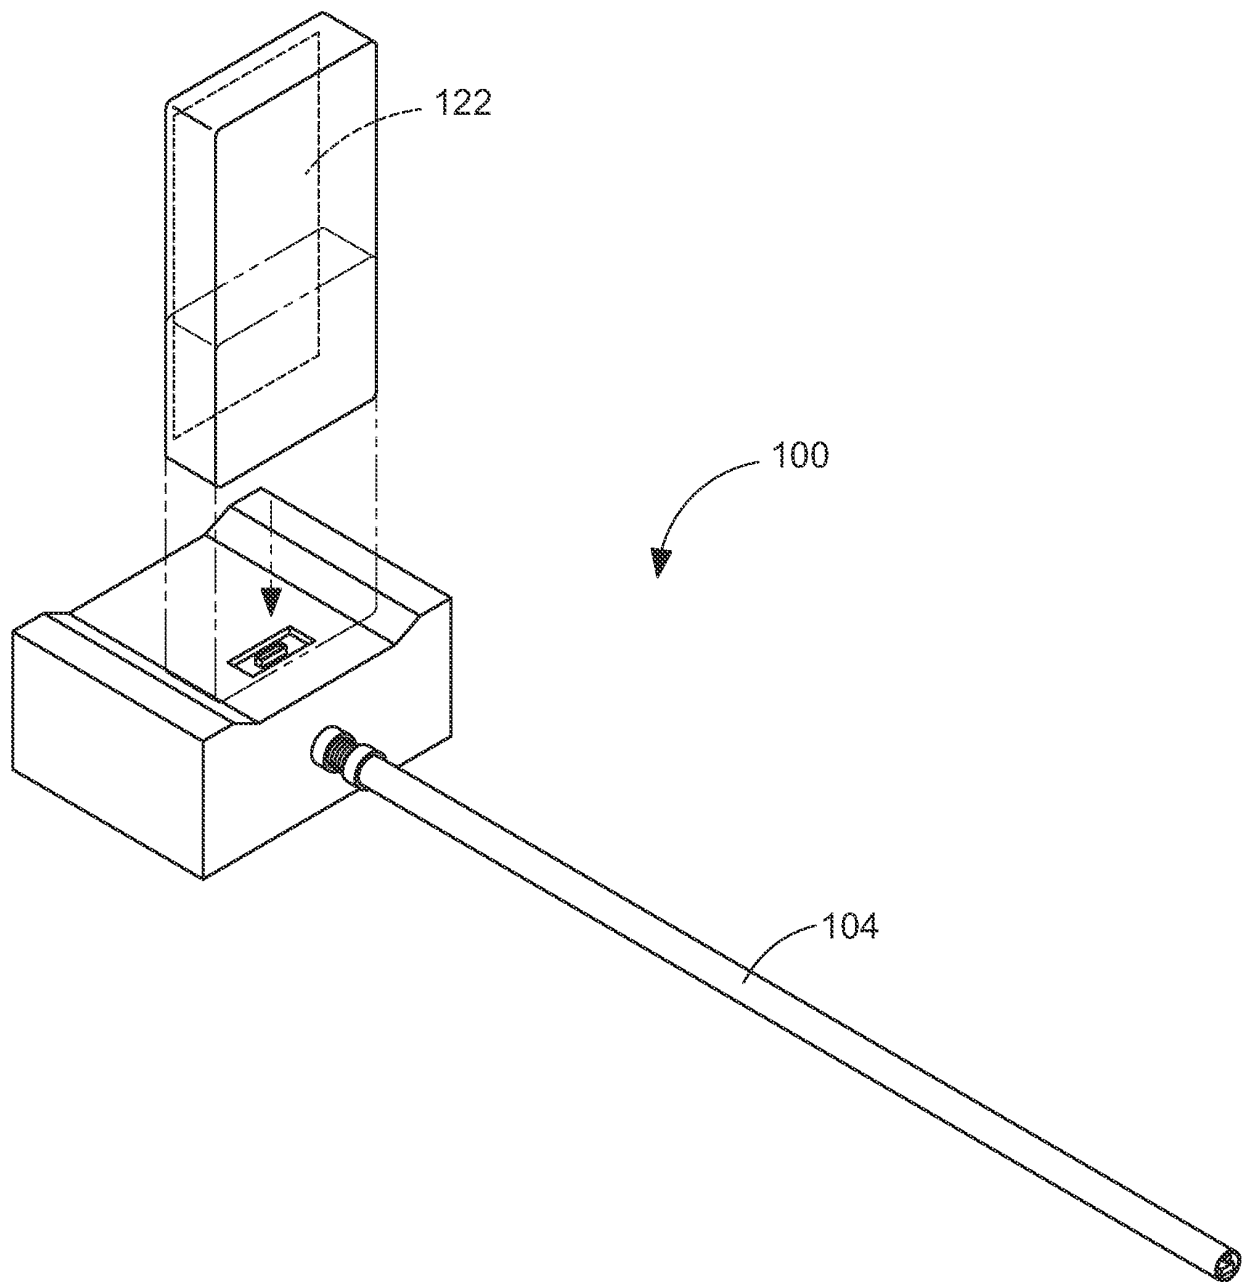


FIG. 4B

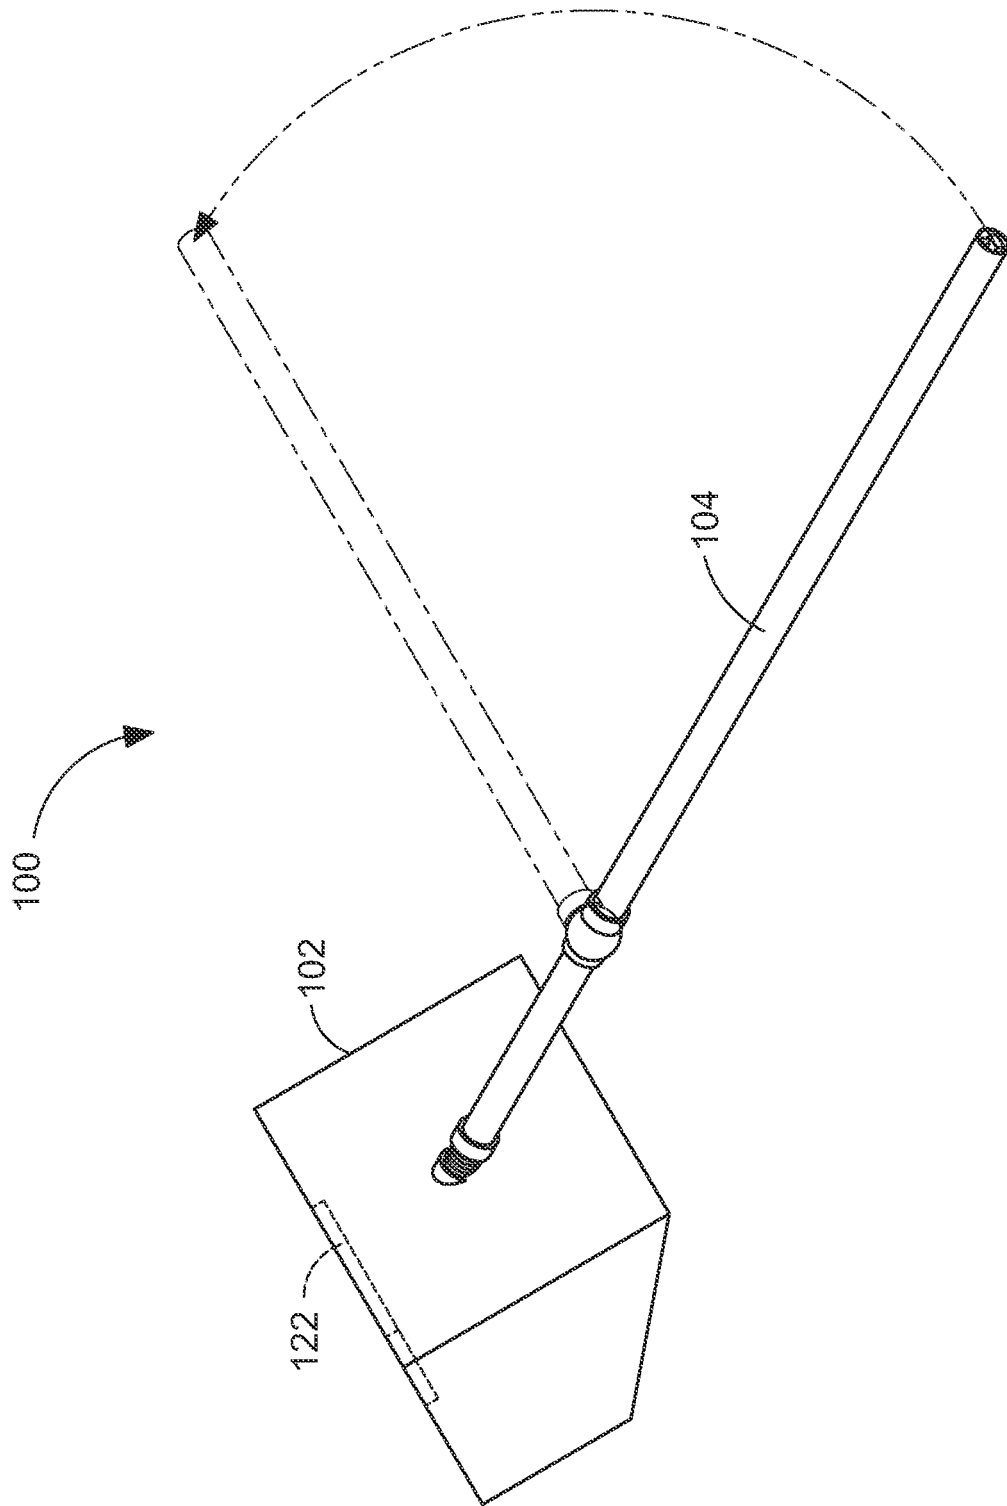


FIG. 4C

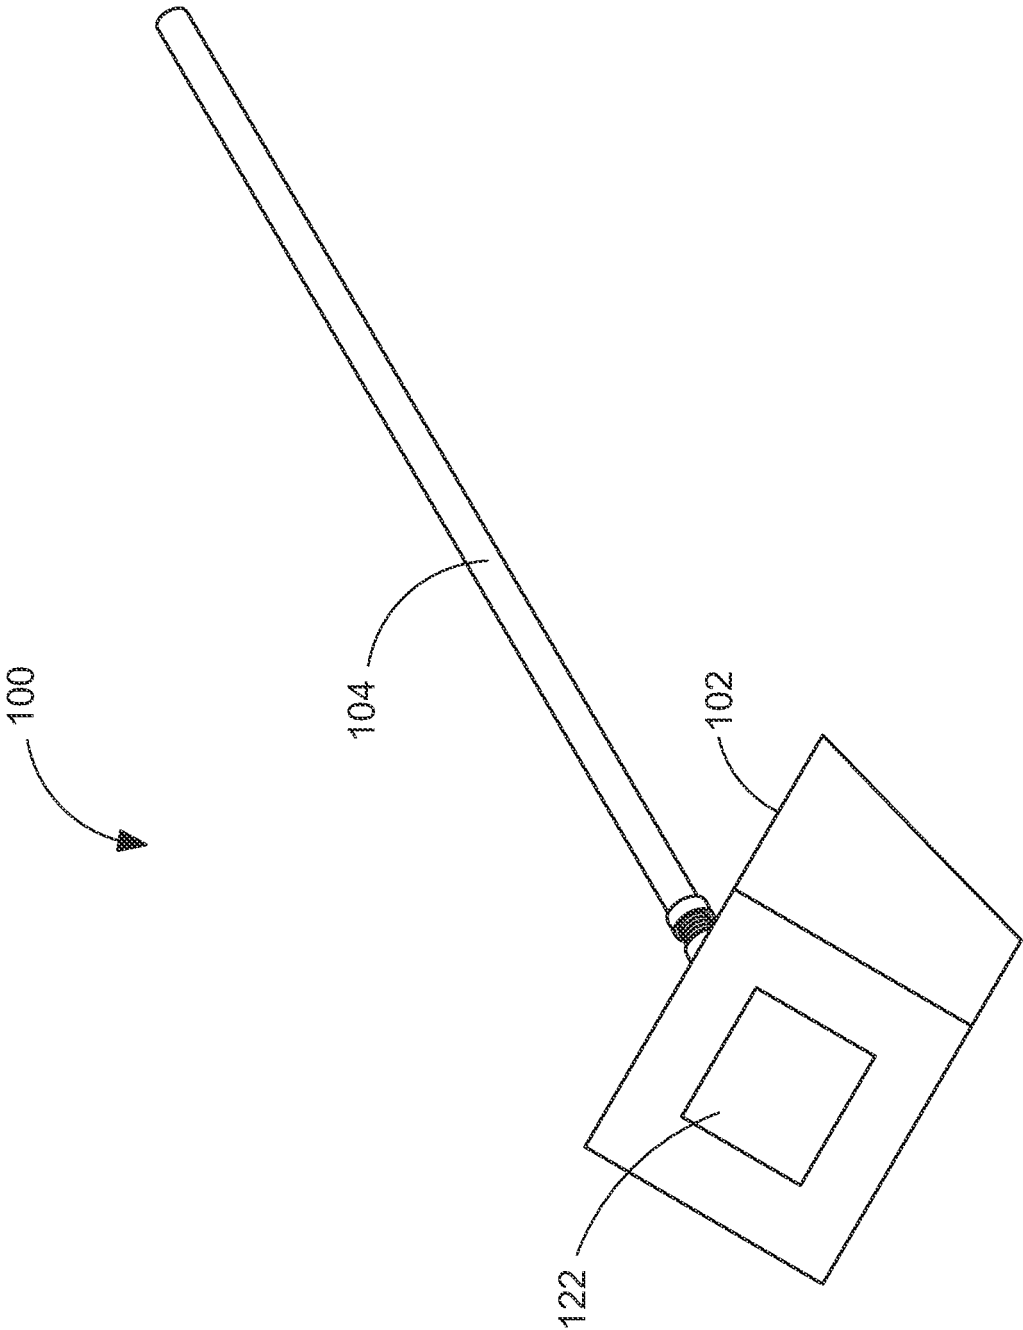


FIG. 4D

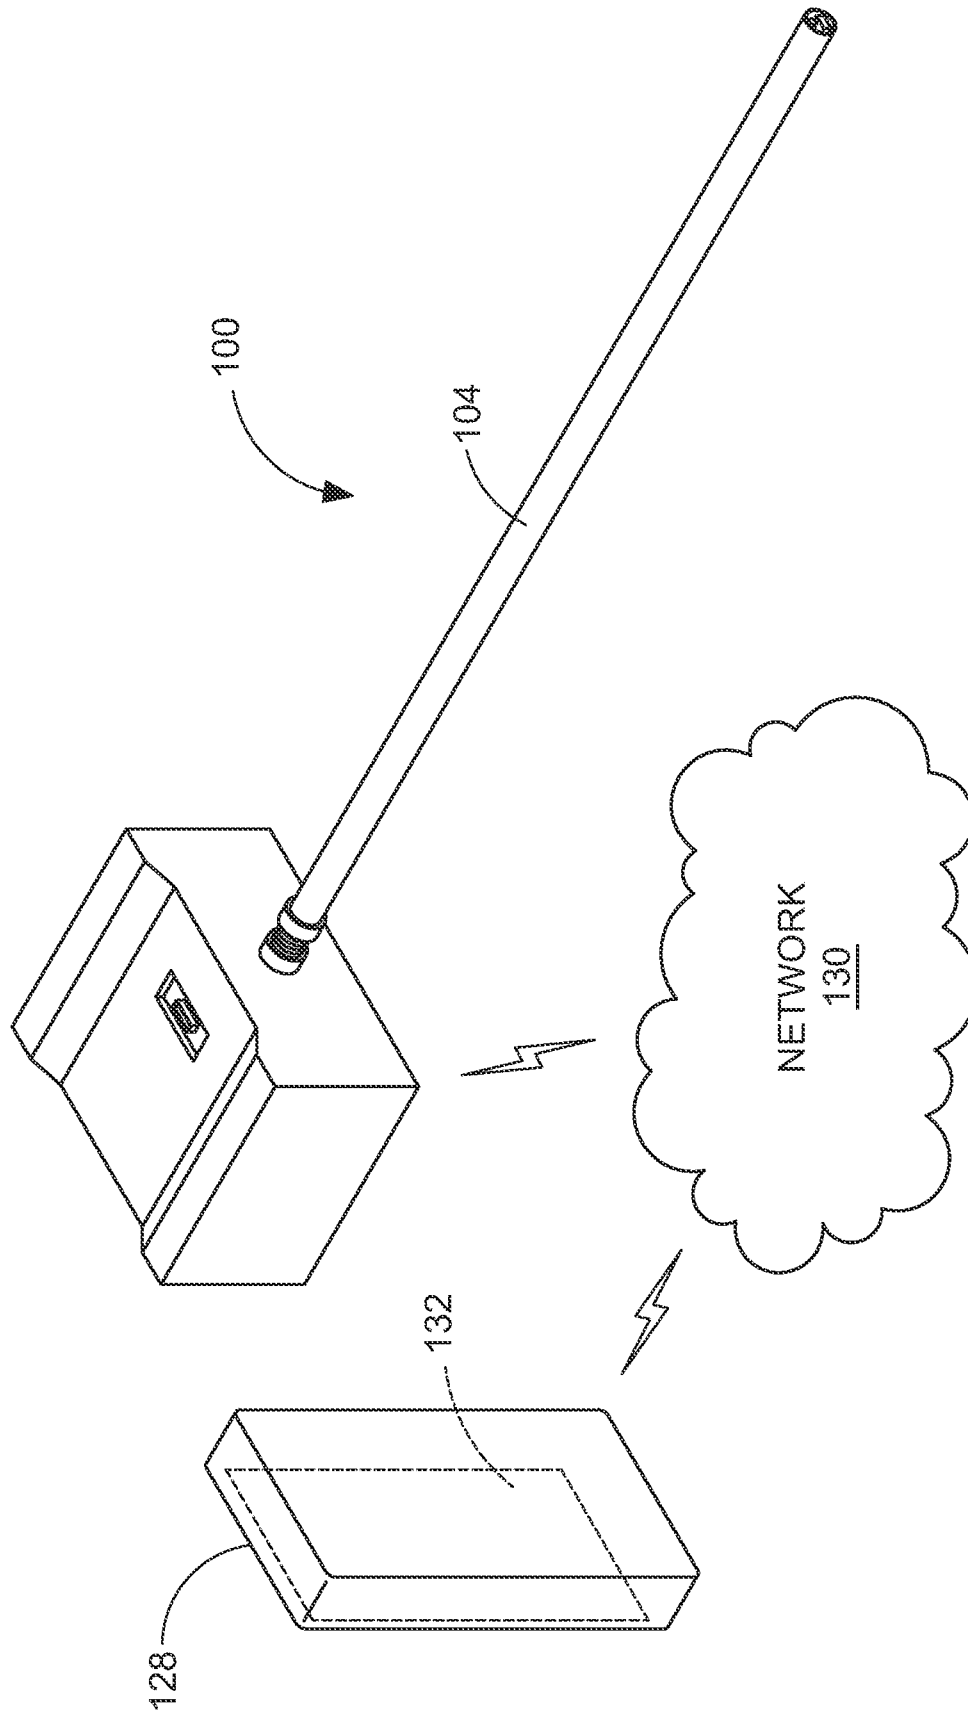
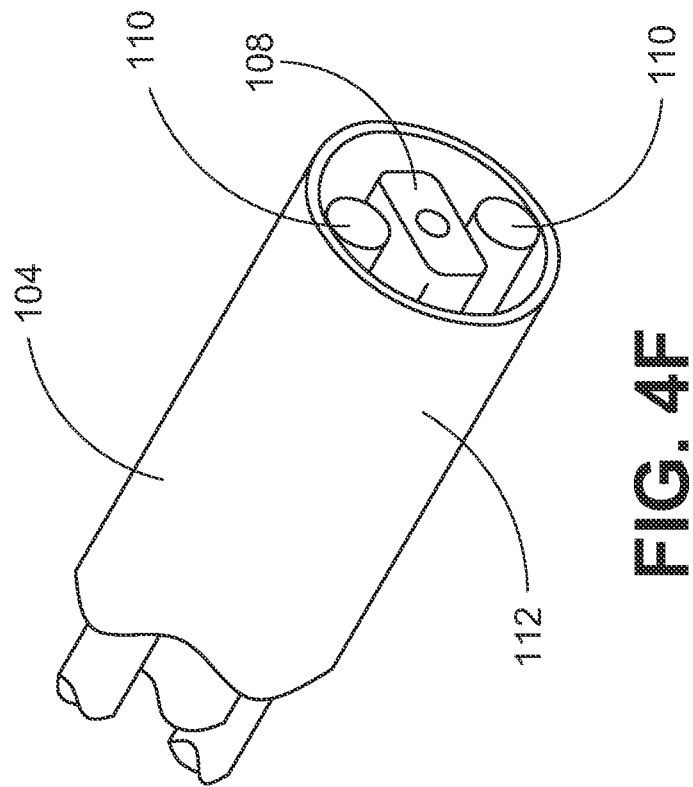


FIG. 4E



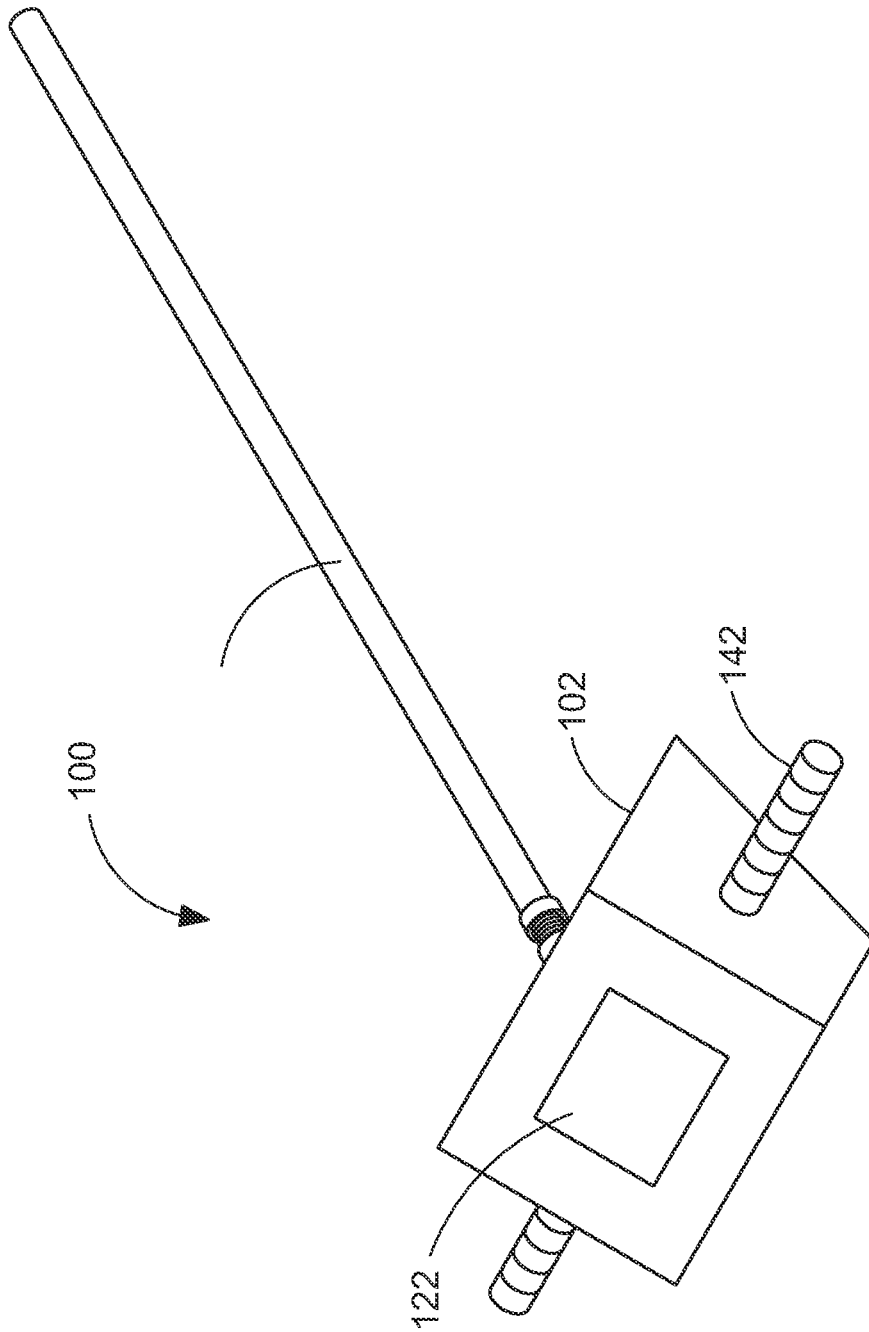


FIG. 4G


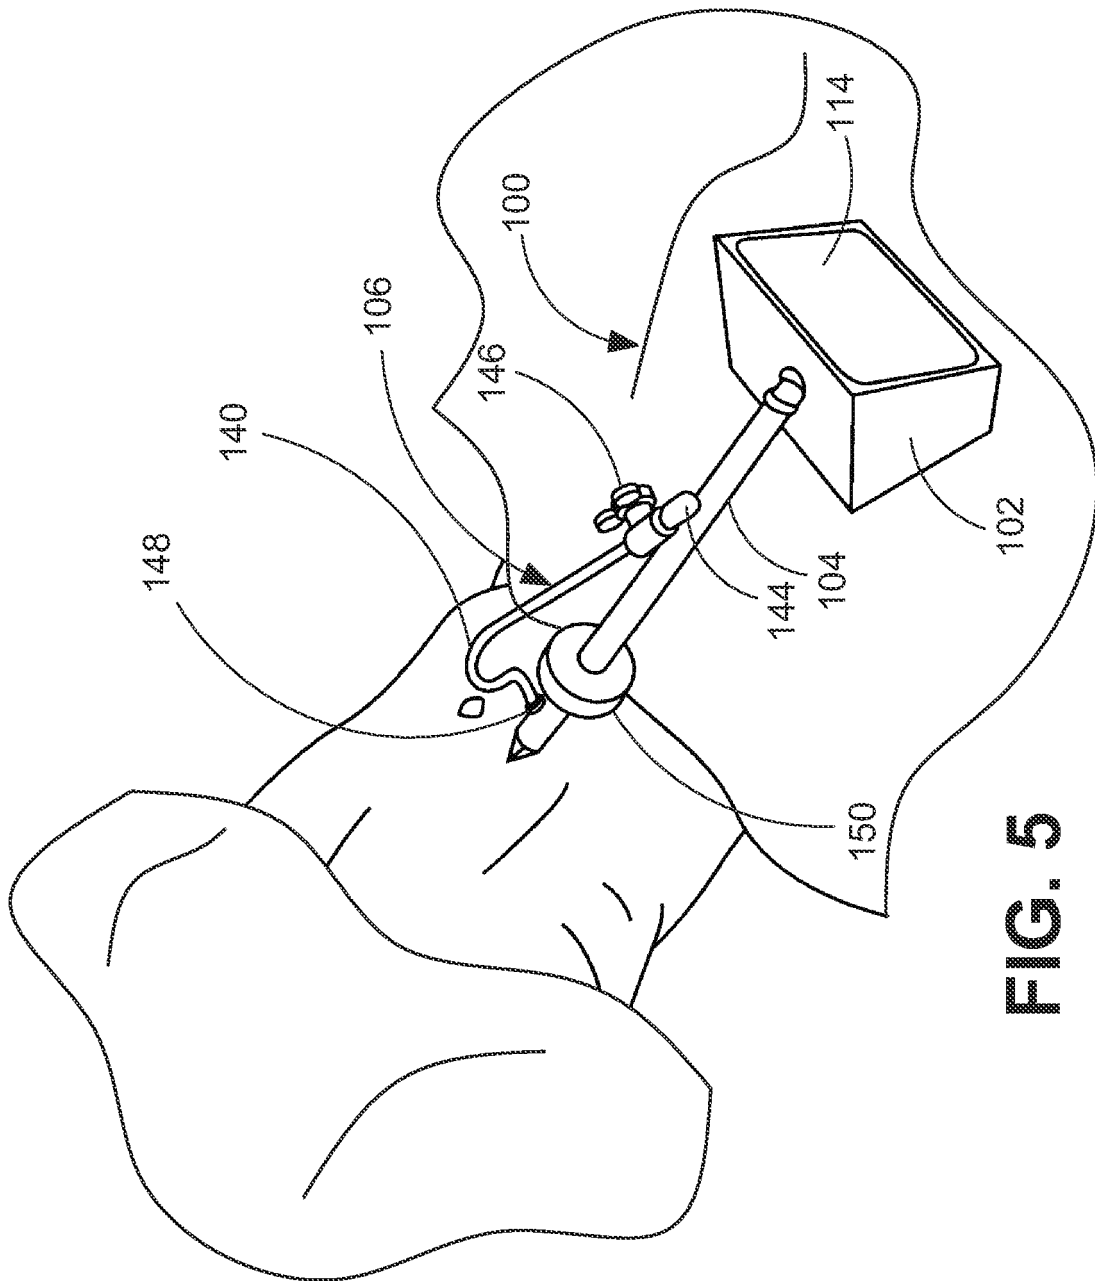


FIG. 5

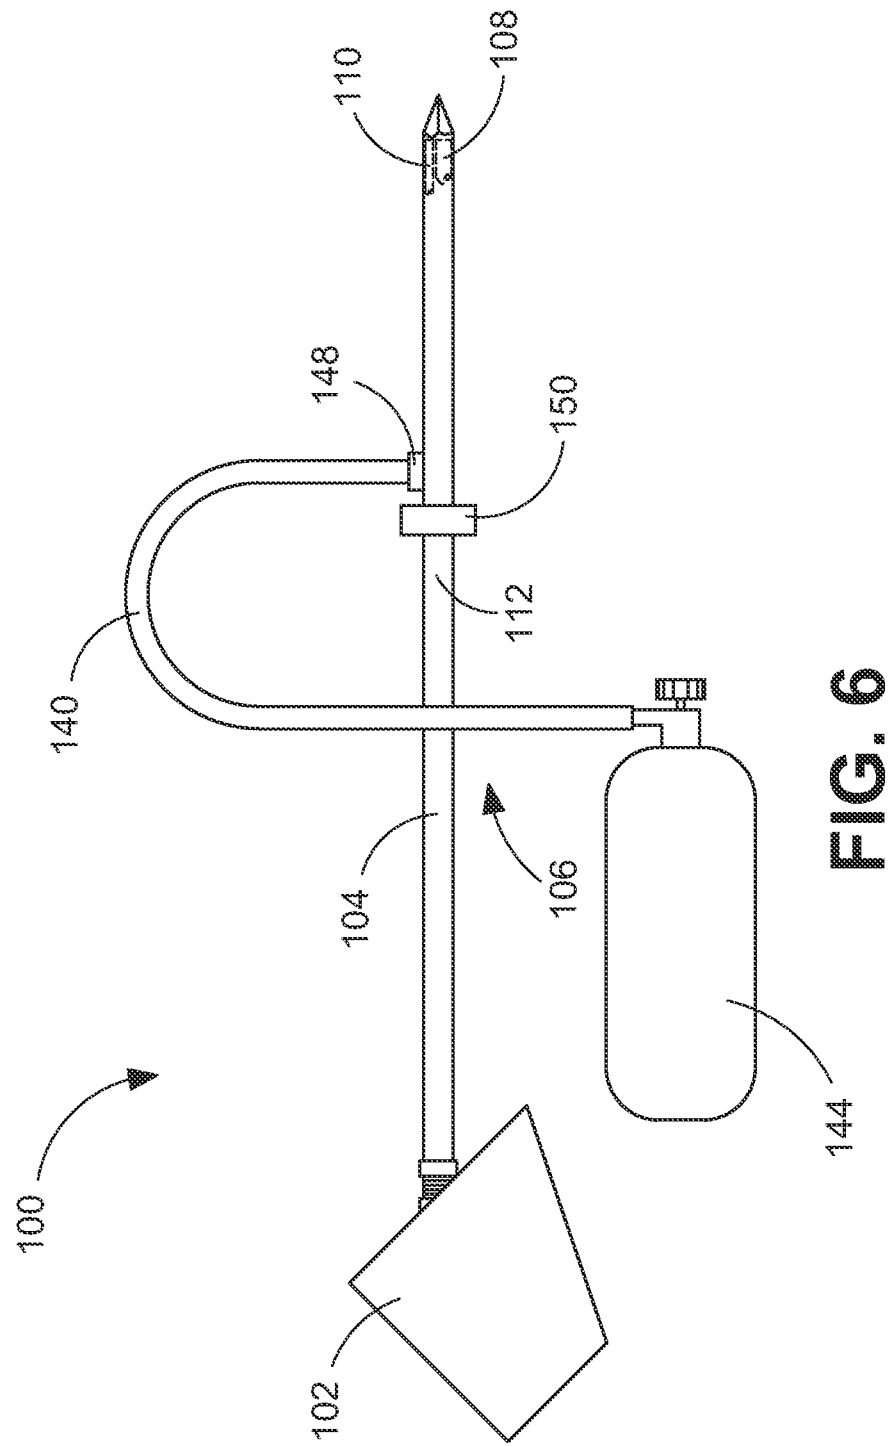

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5785644 A [0002]

专利名称(译)	便携式腹腔镜系统		
公开(公告)号	EP2648603B1	公开(公告)日	2020-02-05
申请号	EP2011846608	申请日	2011-12-08
申请(专利权)人(译)	内布拉斯加大学的校董会		
当前申请(专利权)人(译)	内布拉斯加大学的校董会		
[标]发明人	ARE CHANDRAKANTH ARE MADHURI ALEXANDER DENNIS		
发明人	ARE, CHANDRAKANTH ARE, MADHURI ALEXANDER, DENNIS		
IPC分类号	A61B1/313 A61B1/00 A61B1/05 A61B1/06 A61M13/00		
CPC分类号	A61B1/00013 A61B1/00016 A61B1/00052 A61B1/00108 A61B1/00183 A61B1/05 A61B1/0676 A61B1/3132 A61M13/003		
优先权	61/420901 2010-12-08 US		
其他公开文献	EP2648603A2 EP2648603A4		
外部链接	Espacenet		

摘要(译)

公开了一种便携式腹腔镜。在实施方式中，便携式腹腔镜包括壳体和联接至壳体的细长管。光源和照相机靠近细长管的与壳体相对的一端设置。相机被配置为在由光源提供的光照射的观看区域中捕获图像。便携式腹腔镜包括图像显示装置，该图像显示装置被配置为显示由照相机获取的图像和/或将图像发送到远程显示装置。壳体可以被构造保持和定位吹入器。

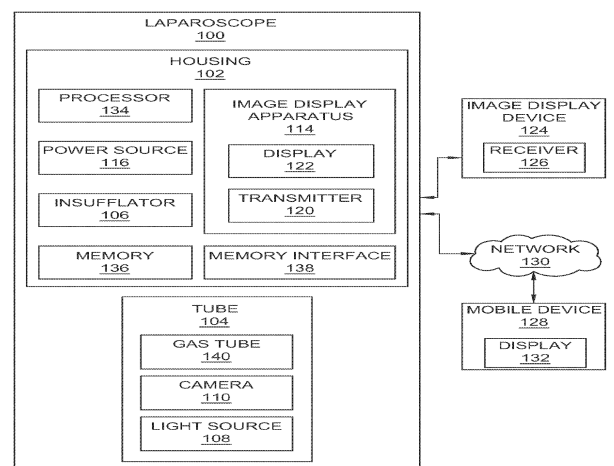


FIG. 1