



(11) EP 1 437 601 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
20.06.2007 Bulletin 2007/25

(51) Int Cl.:
G01R 33/28 (2006.01) **A61B 5/055 (2006.01)**
G01R 33/032 (2006.01)

(21) Application number: **03000554.0**(22) Date of filing: **10.01.2003****(54) Apparatus for detecting the position and the orientation of an invasive device**

Vorrichtung zur Ermittlung von Ort und Orientierung eines invasiven Geräts

Dispositif pour déterminer la localisation et l'orientation d'un appareil invasif

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PT SE SI SK TR**

- **Umathum, Reiner**
69115 Heidelberg (DE)
- **Zabel, Hans-Joachim**
69126 Heidelberg (DE)

(43) Date of publication of application:
14.07.2004 Bulletin 2004/29

(74) Representative: **Isenbruck, Günter**
Patentanwälte,
Isenbruck - Bösl - Hörschler - Wichmann - Huhn,
Theodor-Heuss-Anlage 12
68165 Mannheim (DE)

(73) Proprietor: **Deutsches Krebsforschungszentrum**
Stiftung des öffentlichen Rechts
69120 Heidelberg (DE)

(56) References cited:
WO-A-02/086526 **US-A- 5 318 025**
US-A- 5 592 939 **US-A1- 2002 058 868**
US-B1- 6 223 066

(72) Inventors:
• **Bock, Michael**
69115 Heidelberg (DE)

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates to an assembly for detecting the position and the orientation of an interventional device, using a Faraday sensor.

5 [0002] Modern interventional and surgical procedures aim to treat the affected tissue by causing minimal injury to healthy tissue structures. Special instruments are delivered to the target region via a minimal surgical opening and the affected tissue is treated.

10 [0003] The target of the minimally invasive operation is often not directly visible for the interventionist, thus the operations are done under imaging guidance. X-ray fluoroscopy, computed tomography, ultrasound and optical endoscopy are currently the most frequently used imaging methods. However, magnetic resonance imaging (MRI) is a state of the art imaging modality for medical diagnostics and it has potential to become a superior guidance method. Knowing the accurate position of the instrument tip inside the patient is essential, since the surgeon should be able to accurately guide the instrument to the target.

15 [0004] Within an MR-imaging apparatus, interventional device tracking has so far been done either by evaluating the change (gain or destruction) of the MR-signal at the position of the interventional device or by attaching an electrical conductor or a high-frequency antenna to the device.

20 [0005] The change of MR-signal caused by the device itself can only be used to measure the position of the device, if the device is positioned within the imaging frame. Furthermore, if the contrast between the device and its surroundings is too low, it cannot be detected. Visualisation of an interventional device could depend upon its being coated with an 25 MR contrast agent, or upon its effect on the MR image by nature of its chemical make-up. However, compounds and materials considered MR-compatible, and even MR contrast agents, can produce significant distortion artifacts that obscure the anatomy and physiology of the imaged tissue. Initial attempts to visualise endovascular devices in MR imaging were based on passive susceptibility artifacts produced by the device when exposed to the MR field. US 5,154,179 and US 4,989,608 disclose the incorporation of paramagnetic material into endovascular devices to make the devices visible under MR imaging.

30 [0006] If the device is connected to an electrical conductor with one or more windings and if these windings are passed by a direct current, a local distortion of the magnetic field of the MR-imaging apparatus is caused. This distortion causes a local alteration of the MR image. By taking two MR images, one with and one without a direct current flowing through the conductor, the position of the interventional device can be determined by the difference of the signals in the two MR images. This method is described in US 5,868,674. Within the magnetic radio frequency field of the MR-imaging apparatus, electric coupling of the wires, which are used as a current supply for the electrical conductor can lead to severe heating under certain circumstances. If the heat is not dissipated, it might result in the destruction of the device and it could be hazardous to the patient.

35 [0007] Another possibility for measuring the position of the interventional device is the application of a high-frequency antenna, which is attached to the device. This antenna is tuned to the resonance frequency of the MR-imaging apparatus. Therefore, the antenna is not compatible to all MR imagers. Furthermore, dangerous RF-heating can take place and the MR technique has to be adapted to this kind of device tracking.

40 [0008] Exemplary of methods for active MR visualisation of implanted medical devices is US 5,211,165, which discloses an MR tracking system for a catheter based on transmit/receive microcoils positioned near the end of the catheter by which the position of the device can be tracked and localised. US 5,375,596 discloses a method for locating catheters and other tubular medical devices implanted in the human body using an integrated system of wire transmitters and receivers. US 4,572,198 also provides for conductive elements, such as electrode wires, for systematically disturbing the magnetic field in a defined portion of a catheter to yield increased MR visibility of that region of the catheter. However, the presence of conductive elements in the catheter also introduces increased electronic noise and the possibility of 45 Ohmic heating, and these factors have the overall effect of degrading the quality of the MR image and raising concerns about the patient's safety. US 5,882,305 therefore replaces long lead wires, which can cause heating during MR imaging and may distort an MR image, by at least one optical fibre. Consequently, electrical signals have to be converted into modulated optical signals and vice versa by two transducer circuits.

50 [0009] Another possible way of finding the position of an interventional device is to localise it independently of the MR imaging, by using several cameras and light-emitting or reflecting reference marks. For this technique, a free field of view between the reference marks and the cameras is required. Unfortunately, the field of view is very limited when the interventional device is inside a patient's body and when the MR-imaging apparatus is closed.

55 [0010] US 6,223,066 B1 refers to an apparatus for determining the position of an object, comprising: a light source; a magnetic-field responsive optical element coupled to the object, which receives light from the light source and rotates the plane of polarisation of the light responsive to an external magnetic field; a detector, which receives at least a portion of the modulated light from the magnetic field responsive optical element and generates signals responsive thereto; and signal processing circuitry, which receives the signals from the detector and processes the signals to determine the position of the object.

[0011] Accordingly, it is the object of the present invention to provide an apparatus for detecting the position and the orientation of an interventional device, which overcome the drawbacks mentioned above.

[0012] In accordance with the object of the present invention, there is provided an apparatus as set out in claim 1, This apparatus is used for measuring the position and the orientation of an interventional device within a magnetic resonance imaging apparatus, the magnetic resonance imaging apparatus providing a static magnetic field B_0 , and magnetic field gradients with known magnetic flux densities and directions, comprising the steps of

(A) attaching a Faraday sensor to the interventional device, the Faraday sensor being connected to an optical measuring device,

(B) using the optical measuring device for measuring the rotation of the plane of polarisation of linearly polarised light in the Faraday sensor, while exposing the interventional device

(i) to the static magnetic field B_0 and

(ii) to the field gradients in all three directions of space in addition to the static magnetic field B_0

and

(C) determining the position and the orientation of the interventional device by evaluating the measured rotation of the plane of polarisation of the linearly polarised light.

[0013] The apparatus according to the invention takes advantage of the magnetic fields provided by a magnetic resonance (MR) imaging apparatus. Compared to X-ray systems, which work with significant levels of radiation, MR does not utilise ionising radiation and there are no known long-term adverse effects on biological tissues from MR, as used in clinical MR imaging environment.

[0014] A Faraday sensor is attached to the interventional device. A Faraday sensor uses the Faraday effect, which consists in the rotation of the plane of polarisation of a light beam by a magnetic field. The magnitude of rotation (rotation angle Φ) depends upon the strength of the magnetic field (magnetic flux density B), the length of the transmitting substance 1 and Verdet constant V , which is a property of the transmitting substance, its temperature and the frequency of the transmitted light. If the light path and the direction of the applied magnetic field are parallel, the plane of polarisation is rotated according to the following form:

$$\Phi = V B l.$$

[0015] If the light path is oriented in an angle α with respect to the direction of the magnetic field, the rotation angle of the plane of polarisation is

$$\Phi = V B l \cos\alpha.$$

[0016] Therefore, by measuring the angle of rotation Φ and if V and l are known (and $\alpha = 0$), the magnetic flux density of the magnetic field can be determined. Furthermore, by measuring the angle of rotation Φ and if V , B and l are known, the angle α can be determined. The present invention profits of these correlations in order to measure the local magnetic field and thereby the position and orientation of the interventional device, to which the Faraday sensor is attached.

[0017] For measuring Φ , an active material, typically a crystal, is placed in a light beam between a polarizer and an analyzer and Φ is given by the relative angle between the polarizer and the analyzer at maximum light transmission. At a constant angle between the polarizer and the analyzer, the angle of rotation can be determined by measuring the light intensity transmitted by the analyzer, which depends upon the rotation angle Φ . Changes in the magnetic field result in a modulation of the transmitted light and can be measured e.g. using a fast photo detector. The polarizer, the analyzer and the fast photo detector can be part of the optical measuring device of the present invention.

[0018] One advantage of using a Faraday sensor for interventional device tracking is that it does not contain any conducting material. As a result, a dangerous heating of the position sensor is avoided.

[0019] The rotation of the plane of polarisation of linearly polarised light in the Faraday sensor is measured with the help of the optical measuring device. As mentioned above, the angle of rotation is a function of the strength of the magnetic field. As a result, measuring the angle of rotation means measuring the strength of the magnetic field, if all other variables are known. According to the present invention, the magnetic resonance imaging apparatus provides defined magnetic fields, the strength and direction of which are known and are different at every point of the measurement

space. Therefore, the Faraday sensor can be localised by determining the magnetic field strength at its position.

[0020] The interventional device (together with the Faraday sensor) is exposed to a static and homogeneous magnetic field B_0 (step (i)) in order to determine its orientation. If the light path inside the Faraday sensor is not parallel to the lines of electric flux of this magnetic field, the rotation of the plane of polarisation is different than with the light path and the lines of electric flux being parallel (see above formula). The magnetic field is the same for any position of the Faraday sensor within the static and homogeneous magnetic field B_0 . Consequently, the angle of rotation Φ is not dependent upon the position of the Faraday sensor, but only upon the angle α between the direction of the magnetic field and the light path within the sensor.

[0021] Further (during step (ii)), the interventional device is exposed to field gradients in all three directions of space in addition to the static and preferably homogeneous magnetic field B_0 . The magnetic field gradient is a variation in the magnetic field with respect to position. By applying field gradients in all three directions (at the same time or one after the other), the three coordinates giving the position of the Faraday sensor (and the interventional device) can be determined. The steps (i) and (ii) can also be carried out in reverse order.

[0022] One advantage of the present invention is that no visual contact with the Faraday sensor is necessary. Furthermore, localising the sensor is not dependent upon MR imaging and the corresponding image formation, since it is carried out only by determining the local magnetic field at the position of the sensor with the help of field gradients.

[0023] In one preferred embodiment of the present invention, the Faraday sensor is a reflection type sensor. In this kind of sensor, the light passes through the active material (e.g. the crystal) of the Faraday sensor, is reflected and passes through the active material again in the other direction. The direction of rotation of the plane of polarisation is the same for both paths of the light. Therefore, if the same beam of light is reflected back and forth through the active medium, the rotation of its plane of polarisation is increased each time. The reflection of the light beam can either take place at a mirror behind the active medium of the Faraday sensor or at the end surface of the active medium itself. The reflection type sensor is advantageous because of its possible miniaturisation, allowing the Faraday sensor to be integrated easily into very small interventional devices.

[0024] The magnetic resonance imaging apparatus provides the magnetic fields for MR imaging and for the method according to the invention. The magnetic fields applied for MR imaging, particularly the field gradients, are usually very complex. The magnetic fields used for determining the position and the orientation of an interventional device can be chosen much simpler, in order to keep the evaluation of the measured data simple.

[0025] In a preferred embodiment of the present invention, the magnetic fields provided by the magnetic resonance imaging apparatus are used for both, the MR imaging and the measurement of the position and the orientation of the interventional device. By using the same magnetic fields for both purposes, the time for getting MR images and the information about the position and orientation of the interventional device is reduced. Long scan times limit the applicability of MR-imaging techniques to the general patient population. In particular, long scan times lead to artifacts in the MR images due to involuntary patient movements and motion of the interventional device. Therefore the scan time should be reduced as much as possible.

[0026] In a preferred embodiment of the present invention, an image of the interventional device is superimposed upon independently acquired diagnostic images at the position of the interventional device determined according to the invention. The position of the interventional device (and possibly its orientation) is displayed on display means by superposition of a graphic symbol on a conventional MR image. In alternative embodiments of the invention, a graphic symbol representing the interventional device is superimposed on diagnostic images obtained with other imaging systems such as a computer tomography (CT) scanner, an ultrasound scanner or a positron emission tomography (PET) system. Other embodiments of the invention display the position and the orientation of the interventional device numerically or as a graphic symbol without reference to a medical diagnostic image.

[0027] Preferably the interventional device, the position and orientation of which are measured according to the present invention, is a guide wire, a catheter, an endoscope, a laparoscope, a biopsy needle, surgical implement, therapy delivery implement, an intravascular catheter, a radiofrequency ablation device, a cryo-cooling device or a similar device.

[0028] In a preferred embodiment of the present invention the Faraday sensor is aligned within a static homogeneous magnetic field B_0 prior to its use. In this context, aligning means setting a particular angle of orientation α between the direction of the magnetic field and the light path within the sensor, e.g. an angle of 0° . The Faraday rotation angle ϕ_{cal} is measured with the aligned sensor and stored. In the next step (for example during an interventional procedure) the rotation angle ϕ_0 within the static homogeneous magnetic field B_0 in the absence of field gradients is determined. From the phase difference $\phi_0 - \phi_{cal}$ the actual orientation angle α is computed.

[0029] The interventional device is exposed to a magnetic field gradient in each direction of space (x,y,z). In a magnetic resonance tomography apparatus the field gradient G is typically designed to modulate the component of the magnetic flux parallel to the static magnetic field B_0 :

$$\mathbf{B}(\mathbf{x}, \mathbf{y}, \mathbf{z}) = \mathbf{B}_0 + \mathbf{G}_x(t) \cdot \mathbf{x} + \mathbf{G}_y(t) \cdot \mathbf{y} + \mathbf{G}_z(t) \cdot \mathbf{z}$$

5 [0030] The position of the Faraday sensor (and the interventional device) is then calculated by the difference of the angle of rotation of linearly polarised light caused by the different magnetic field gradients $\phi_{x,y,z}$ and the rotation angle measured without the presence of the gradients ϕ_0 :

$$10 \quad x = \frac{\Phi_x - \Phi_0}{V \cdot l \cdot G_x \cdot \cos \alpha}, \quad y = \frac{\Phi_y - \Phi_0}{V \cdot l \cdot G_y \cdot \cos \alpha}, \quad z = \frac{\Phi_z - \Phi_0}{V \cdot l \cdot G_z \cdot \cos \alpha}.$$

15 [0031] A measurement of the position and orientation of the sensor therefore requires the measurement of four Faraday rotation angles ($\phi_0, \phi_x, \phi_y, \phi_z$) and an initial calibration of the sensor (ϕ_{cal}).

[0032] In a further preferred embodiment of the present invention the relative angle of rotation is increased using a minimum of two magnetic field gradients with opposite polarities in each spatial direction. The two gradients are applied successively and the phase difference is measured.

[0033] In another preferred embodiment of the present invention, the optical measuring device uses a lock-in technique for measuring the rotation of the plane of polarisation of the linearly polarised light in the Faraday sensor caused by the magnetic field gradients. The angle of rotation of the plane of polarisation of the linearly polarised light is preferably determined by measuring the light intensity of the linearly polarised light after passing through an analyzer. If the magnetic field, to which the Faraday sensor is exposed, is composed of a strong static magnetic field B_0 and a small field gradient, the angle of rotation is mainly influenced by the strong static magnetic field. The small field gradients generate the position information, however, the small position signal is obscured by noise in the received signal. One of the most useful devices for improving the signal-to-noise ratio is the lock-in amplifier. A lock-in amplifier takes a periodic reference signal and a noisy input signal and extracts only that part of the signal whose frequency and phase match the reference. Therefore, the signal to be measured has to be modulated (e.g. chopped) with the reference frequency. For the present invention, the field gradients are modulated with a reference frequency, resulting in a modulated intensity signal of the linearly polarised light after passing through the Faraday sensor and the analyzer.

[0034] The method of detecting the position and orientation of an object within a defined magnetic field with the help of a Faraday sensor is not limited to medical applications within an MR-imaging apparatus. It can also be used for non-medical applications within an MR-scanner or for position detection in a known magnetic field, which is not provided by an MR-imaging apparatus. Examples for non-medical applications within an MR-scanner are materials science investigations with an MR-independent position signal (e.g. studies on parmesan cheese). Position detection with a known magnetic field, which is not provided by an MR-imaging apparatus, can be carried out in a room with special coils for generating the magnetic fields for spatial encoding.

[0035] The present invention may be best understood by reference to the following description in conjunction with the accompanying drawing in which:

40 Fig. 1a is a schematic drawing showing an optical measuring device with a transmission type Faraday sensor suitable for the present invention,

45 Fig. 1b is a schematic drawing showing an optical measuring device with a reflection type Faraday sensor suitable for the present invention,

Fig. 1c is a schematic drawing showing an optical measuring device with a transmission type Faraday sensor with an etalon suitable for the present invention,

50 Fig. 2 is a schematic illustration showing an optical measuring device with a transmission type Faraday sensor being suitable for the present invention and

Fig. 3 is a timing diagram showing the consecutive measurement steps to determine the orientation and the position of the sensor.

55 [0036] The Faraday sensor as shown in fig. 1a contains a magneto-optically active medium in the form of a crystal 1. Within a magnetic field the polarisation of a light beam is rotated when the beam is traversing the crystal 1. The rotation angle at the end of the crystal 1 depends upon the length L of the active material, the Verdet constant and the magnetic

field strength. To measure the rotation angle, the crystal 1 is placed between a polarizer 3 and an analyzer 4. The polarizer 3 and the analyzer 4 are formed by polarisation foils, which are arranged at a constant angle to each other. The optical fibre 5 is used to couple light, which is emitted by a light source 7, into the crystal 1, after having passed the polarizer 3. A second optical fibre 6 is used to transmit the light beam coming out of the Faraday sensor to a detector (not shown) for measuring the light intensity. The Faraday sensor as shown in fig. 1a is a transmission type sensor. The light beam passes through this sensor only in one direction.

[0037] In an alternative implementation the Faraday sensor is constructed as a reflection type sensor as shown in fig. 1b. The reflection type sensor has the advantage that the same optical fibre 5 can be used to transmit the light from the light source 7 to the sensor and to guide the reflected light to an external detector (not shown). Furthermore, the rotation angle in a reflection type sensor is doubled as compared to a transmission type sensor of the same length L due to the doubled optical path length. Therefore, a mirror 9 is attached to the end of the crystal 1 to reflect the light coming from the light source 7 passing in forward direction through the polarizer 3 and the crystal 1. The light reflected by mirror 9 is passing in backward direction through the crystal 1 and the polarizer 3, which is now acting as an analyzer 4, and is guided through the fibre 5 to a beam splitter 2. At the beam splitter 2, the reflected light beam is separated from the incident light beam 8. The reflected light beam 19 is then transmitted to a detector (not shown).

[0038] In an alternative implementation the Faraday sensor is constructed as an etalon type sensor as shown in fig. 1c. The etalon type sensor is a modification of the reflection type sensor shown in fig. 1b where a second, semi-transparent mirror 11 is placed between the polarizer 3 and the crystal 1 in addition to the reflecting first mirror 10 at the end of the crystal 1.

[0039] In summary, the optical measuring device, which is suitable for the present invention preferably comprises a light source 7, a polarizer 3, an analyzer 4 and a photo detector. The light source 7 is preferably a laser, especially a diode laser. Since the Verdet constant depends upon the frequency of the light passing through the magneto-optically active material, the method according to the present invention should be operated with a monochromatic light source.

[0040] In a preferred embodiment of the present invention, the light source 7 is an intensity-stabilized light source in order to avoid intensity fluctuations of the light beam, which would cause errors of measurement. Another possibility of eliminating the unwanted effect of intensity fluctuations of the light beam emitted by the light source 7 would be decoupling part of the light beam to be used in the Faraday sensor without its plane of polarisation being rotated in the Faraday sensor, the decoupled light beam serving as a reference beam.

[0041] The Faraday sensor is preferably connected to the optical measuring device by at least one optical fibre 5, 6. By using optical fibres 5, 6, the light source 7 and the photo detector can be placed outside of the magnetic fields, advantageously avoiding any influence of the fields on the functioning of these devices. The Faraday sensor preferably comprises a crystal 1 containing at least one of the following magneto-optically active materials: terbium-gallium-garnet or rare earth (III) aluminum garnets (cf. Rubinsetin CB, Van Uitert LG, Grodkiewicz WH: Magneto-optical properties of rare earth (III) aluminum garnets, J. Appl. Phys. 35, 3069-70 (1964)).

[0042] Fig. 2 shows a transmission type Faraday sensor, which is suitable for the present invention, being placed within a static magnetic field and in magnetic field gradients and connected to a signal evaluation unit. A light source 7 emits a beam of light, which passes through an optical fibre 5. The light is coupled into a polarizer 3 and a crystal 1 which turns its plane of polarisation in the presence of magnetic fields created by a magnet 13 and by magnetic field gradient coils 12. The transmitted light is passed through an analyzer 4 at the end of the crystal 1. The close proximity of polarizer 3 and analyzer 4 to the crystal 1 ensures that the plane of polarisation is not rotated additionally within the optical fibres 5 and 6 which would generate an unwanted additional polarisation rotation. If polarisation-maintaining fibres are used, taking this measure is not necessary. The light beam at the end of the analyzer 4 is coupled into a second optical fibre 6 which guides the light to the photo detector 14. The photo detector 14 creates a signal proportional to the intensity of the light having passed the Faraday sensor.

[0043] For measuring the orientation of the sensor with respect to the static magnetic field created by the magnet 13 in the absence of magnetic field gradients created by the gradient coils 12, the signal amplitude measured by the photo detector 14 is compared with the signal amplitude measured with the aligned sensor, which is oriented parallel to the static magnetic field.

[0044] For measuring the position of the Faraday sensor a magnetic field gradient in one spatial direction created by the gradient coils 12 is applied. Preferably the gradient amplitude is modulated in the form of a sine wave. The modulated gradient field creates an intensity modulation of the light beam passing through the sensor. To evaluate the amplitude of modulation, the signal output of the photo detector 14 is passed to a lock-in amplifier 18. To eliminate unwanted effects of signal fluctuations, the photo detector signal is passed through a low-pass filter 16 to determine a reference signal which does not show the modulation created by the gradients. This reference signal is used for normalization of the lock-in amplifier signal 18. The photo detector output signal is also passed to the lock-in amplifier 18 through a high-pass filter 15. The high-pass filter 15 is chosen so that the modulation frequency created by the gradient coils 12 is not lost in the filtering process. This signal is then compared in the lock-in amplifier 18 with the modulation signal of the gradients provided by the gradient controller 17. The demodulated and normalized output signal of the lock-in amplifier

18 is a measure of the position along the direction of the applied gradient.

[0045] Fig. 3 shows four different measurement steps during the manipulation of the interventional device (and therefore the Faraday sensor). During a first time period only the static magnetic field is acting upon the sensor and the signal at the photo detector is used to determine the orientation of the device. In the next three following steps a sinusoidally modulated waveform is applied to the magnetic field gradient in the first, the second and the third spatial direction. During each of these time periods the photo detector signal is evaluated using the lock-in amplifier for signal analysis.

Example 1

[0046] As the magneto-optically active material for the position sensor a 7.5 mm-long crystal of Terbium-Gallium-garnet (TGG) was chosen, which offers a high Verdet constant of about 7 deg/T/mm at $\lambda = 675$ nm. A diode laser (DLS15, Linos, Germany) was used as a light source and the light was coupled into the crystal through an optical fibre (core diameter: 63 μ m) and a polarising foil. A rotatable analyzer was placed directly behind the crystal and the power of the transmitted light was measured far away from the sensor using again an optical fibre for light transmission and a photo detector (transmission type sensor). Several different experiments were carried out: (a) The sensor was placed at the patient table of a commercial whole body 1.5 T MR scanner (Siemens Magnetom Symphony) and the Faraday rotation was measured with the sensor as a function of z-position and compared to the magnetic flux measurement of a Hall detector. (b) At the magnet's iso-center the sensor was rotated relative to the B_0 -field direction and the change in Faraday rotation was assessed. (c) Trapezoidal gradients of variable duration (1-2 ms) and amplitude (20 and 30 mT/m) were applied at different positions in the gradient field and the change in light transmission was detected with a lock-in amplifier, which compared the gradient control signal with the signal of the fast photo detector. Since the output power of the laser diode was not constant over the measurement period, the detected signal was normalised to the low frequency component of the laser diode signal.

[0047] The magnetic field measurement with the optical sensor showed that the response of the sensor was linear up to $B_0 = 1.5$ T. At this field strength a total rotation angle of 65.8° was measured, which corresponds to a measured Verdet constant of 5.9 deg/T/mm. The expected cosine-law for the rotation against the main magnetic field $\Phi = V L B \cos(\alpha)$ could be reproduced. The normalised demodulated lock-in amplifier signal U_n showed a linear dependency of the position of the sensor. For a gradient strength of $G = 30$ mT/m a sensitivity of $(0.31 \pm 0.02) \times 10^{-3}$ was achieved (fig. 2) so that with this set-up the precision of the localisation is about 1.5 cm. With the current proto-type sensor both position and one orientation angle can be measured. Using this technique e.g. in an intravascular catheter demands the sensor be integrated into an optical fibre and be operated in reflection mode, so that a single fibre can be used and the sensitivity is doubled. Furthermore, special gradient cycles for optical position detection must be incorporated into MRI pulse sequences.

Reference Numbers

[0048]

| | |
|----|----------------------|
| 1 | crystal |
| 2 | beam splitter |
| 3 | polarizer |
| 4 | analyzer |
| 5 | first optical fibre |
| 6 | second optical fibre |
| 7 | light source |
| 8 | incident light beam |
| 9 | mirror |
| 10 | first mirror |
| 11 | second mirror |
| 12 | gradient coils |
| 13 | magnet |
| 14 | photo detector |
| 15 | high pass filter |
| 16 | low pass filter |
| 17 | gradient controller |
| 18 | lock-in amplifier |
| 19 | reflected light beam |

Claims

1. An apparatus containing

5 a magnetic resonance imaging apparatus for providing a homogenous and static magnetic field B_0 and magnetic field gradients with known magnetic flux densities in three different directions of space; an interventional device provided with a Faraday sensor attached thereto; and an optical measuring device connected to the Faraday sensor, said device being arranged to measure the rotation of the plane of polarisation of linearly polarised light in the Faraday sensor, said magnetic resonance imaging apparatus being arranged to expose the interventional device

10 (i) to said homogenous and static magnetic field B_0 , in the absence of the magnetic field gradients, and (ii) to said magnetic field gradients in addition to the homogenous and static magnetic field B_0 ,

15 and the apparatus being arranged to determine the position and the orientation of the interventional device by evaluating the rotation of the plane of polarisation of the linearly polarised light measured in cases (i) and (ii).
2. The apparatus as claimed in claim 1, wherein the Faraday sensor is a reflection type sensor, an etalon type sensor or a transmission type sensor.
- 20 3. The apparatus as claimed in claim 1 or 2, wherein the magnetic fields provided by the magnetic resonance imaging apparatus are provided for both, MR imaging and determining the position and the orientation of the interventional device.
4. The apparatus as claimed in one of claims 1 to 3, comprising a display means for superimposing an image of the 25 interventional device upon independently acquired medical diagnostic images at the determined position.
5. The apparatus as claimed in one of claims 1 to 4, wherein the optical measuring device comprises a light source (7), a polarizer (3), an analyzer (4) and at least one photo detector (14).
- 30 6. The apparatus as claimed in claim 5, wherein the light source (7) is a diode laser.
7. The apparatus as claimed in one of claims 1 to 6, wherein the Faraday sensor is connected to the optical measuring device by at least one optical fibre (5, 6).
- 35 8. The apparatus as claimed in one of claims 1 to 7, wherein the Faraday sensor comprises a crystal (1) containing at least one of the following magneto-optically active materials: terbium-gallium-garnet or rare earth aluminum garnets.
9. The apparatus as claimed in one of claims 1 to 8, wherein the interventional device is a guide wire, a catheter, an 40 endoscope, a laparoscope, a biopsy needle, surgical implement, therapy delivery implement, an intravascular catheter, a radiofrequency ablation device or a cryo-cooling device.
10. The apparatus as claimed in one of claims 1 to 9, wherein the optical measuring device uses a lock-in technique 45 for measuring the rotation of the plane of polarisation of the linearly polarised light in the Faraday sensor, caused by the magnetic field gradients.

Patentansprüche

- 50 1. Ein Apparat enthaltend

einen Kernspintomographen zum Bereitstellen eines homogenen und statischen Magnetfeldes B_0 und magnetischer Feldgradienten mit bekannten magnetischen Flussdichten in drei verschiedenen Raumrichtungen; ein Interventionsinstrument, das mit einem Faraday-Sensor ausgestattet ist, der daran befestigt ist; und ein optisches Messgerät, das mit dem Faraday-Sensor verbunden ist, wobei das Gerät so angeordnet ist, um die Rotation der Polarisationsebene von linear polarisiertem Licht in dem Faraday-Sensor zu messen; wobei der Kernspintomograph angeordnet ist, um das Interventionsinstrument

(i) dem homogenen und statischen Magnetfeld B_0 in Abwesenheit der magnetischen Feldgradienten und

(ii) den magnetischen Feldgradienten zusätzlich zu dem homogenen und statischen Magnetfeld B_0

auszusetzen und wobei der Apparat angeordnet ist, um die Position und die Orientierung des Interventionsinstruments durch Auswerten der Rotation der Polarisationsebene des linear polarisierten Lichtes gemessen in den Fällen 5 (i) und (ii) zu bestimmen.

2. Der Apparat gemäß Anspruch 1, wobei der Faraday-Sensor ein Sensor vom Reflexionstyp, ein Sensor vom Etalon-Typ oder ein Sensor vom Transmissionstyp ist.
- 10 3. Der Apparat gemäß Anspruch 1 oder 2, wobei die durch den Kernspintomographen bereitgestellten Magnetfelder sowohl für die Kernspintomographie als auch zur Bestimmung der Position und Orientierung des Interventionsinstruments bereitgestellt werden.
- 15 4. Der Apparat gemäß einem der Ansprüche 1 bis 3, umfassend ein Anzeigemittel zum Überlagern eines Bildes des Interventionsinstruments mit unabhängig gewonnenen medizinischen diagnostischen Bildern an der bestimmten Position.
- 20 5. Der Apparat gemäß einem der Ansprüche 1 bis 4, wobei das optische Messgerät eine Lichtquelle (7), einen Polarisator (3), einen Analysator (4) und mindestens einen Photodetektor (14) enthält.
- 25 6. Der Apparat gemäß Anspruch 5, wobei die Lichtquelle (7) ein Diodenlaser ist.
7. Der Apparat gemäß einem der Ansprüche 1 bis 6, wobei der Faraday-Sensor an das optische Messgerät durch mindestens eine optische Faser (5, 6) angeschlossen ist.
- 30 8. Der Apparat gemäß einem der Ansprüche 1 bis 7, wobei der Faraday-Sensor einen Kristall (1) enthält, der mindestens eines der folgenden magnetooptisch aktiven Materialien enthält: Terbium-Crallium-Granat oder Seltenerd-Aluminiumgranat.
9. Der Apparat gemäß einem der Ansprüche 1 bis 8, wobei das Interventionsinstrument ein Führungsdräht, ein Katheter, ein Endoskop, ein Laparoskop, eine Biopsienadel, ein chirurgisches Hilfsmittel, ein Therapieabgabehilfsmittel, ein intravaskulärer Katheter, ein Hochfrequenz-Ablationsgerät oder ein Cryokühlgerät ist.
- 35 10. Der Apparat gemäß einem der Ansprüche 1 bis 9, wobei das optische Messgerät eine Lock-In-Technik verwendet, um die Rotation der Polarisationsebene von linear polarisiertem Licht in dem Faraday-Sensor zu messen, die durch die magnetischen Feldgradienten verursacht wird.

Revendications

1. Un dispositif comportant :

- un appareil d'imagerie par résonance magnétique pour obtenir un champ magnétique B_0 homogène et statique et des gradients de champ magnétique qui présentent des densités connues de flux magnétique selon trois directions différentes de l'espace ;
45 - un organe d'intervention muni d'un capteur de Faraday qui lui est fixé; et
- un organe optique de mesure connecté au capteur de Faraday, ledit organe étant agencé pour mesurer la rotation du plan de polarisation de la lumière polarisée linéairement dans le capteur de Faraday ;

50 ledit appareil d'imagerie par résonance magnétique étant agencé pour exposer l'organe d'intervention :

- audit champ magnétique B_0 homogène et statique, en l'absence des gradients de champ magnétique, et
- audit gradient de champ magnétique en plus du champ magnétique homogène et statique B_0 ,

55 et le dispositif étant agencé pour déterminer la position et l'orientation de l'organe d'intervention en évaluant la rotation du plan de polarisation de la lumière polarisée linéairement mesurée dans les cas (i) et (ii).

2. Le dispositif selon la revendication 1, dans lequel le capteur de Faraday est un capteur du type réflexion, un capteur

du type étalon ou un capteur du type transmission.

3. Le dispositif selon la revendication 1 ou 2, dans lequel les champs magnétiques générés par l'appareil d'imagerie par résonance magnétique sont fournis à la fois pour l'imagerie MR (par résonance magnétique) et pour déterminer la position et l'orientation de l'organe d'intervention.
4. Le dispositif selon l'une des revendications 1 à 3, comprenant des moyens d'affichage pour superposer une image de l'organe d'intervention à des images de diagnostic médical acquises indépendamment, à la position déterminée.
- 10 5. Le dispositif selon l'une des revendications 1 à 4, dans lequel l'organe de mesure optique comprend une source (7) de lumière, un polariseur (3), un analyseur (4) et au moins un photodétecteur (14).
6. Le dispositif selon la revendication 5, dans lequel la source (7) de lumière est une diode laser.
- 15 7. Le dispositif selon l'une des revendications 1 à 6, dans lequel le capteur de Faraday est connecté à l'organe de mesure optique par au moins une fibre optique (5, 6).
8. Le dispositif selon l'une des revendications 1 à 7, dans lequel le capteur de Faraday comprend un cristal (1) contenant au moins l'un parmi les matériaux suivants actifs sur le plan magnéto-optique : terbium-gallium-grenat ou grenats de terres rares à l'aluminium.
- 20 9. Le dispositif selon l'une des revendications 1 à 8, dans lequel l'organe d'intervention est un fil-guide, un cathéter, un endoscope, un laparoscope, une aiguille de biopsie, un instrument chirurgical, un instrument de délivrance de thérapie, un cathéter intravasculaire, un organe d'ablation par radiofréquence ou un organe de cryo-refroidissement.
- 25 10. Le dispositif selon l'une des revendications 1 à 9, dans lequel l'organe de mesure optique utilise une technique de synchronisation (*lock-in*) pour mesurer la rotation du plan de polarisation de la lumière polarisée linéairement dans le capteur de Faraday, provoquée par les gradients de champ magnétique.

30

35

40

45

50

55

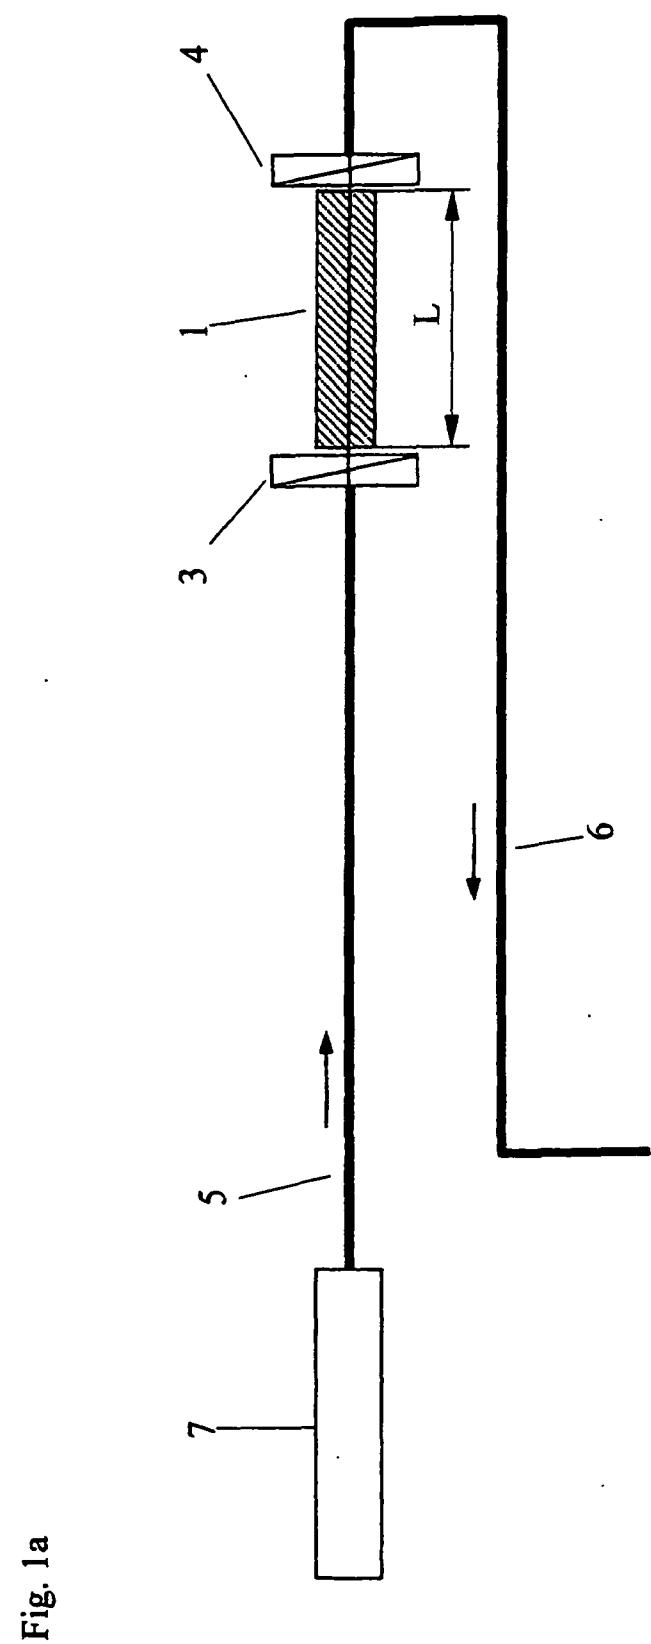


Fig. 1a

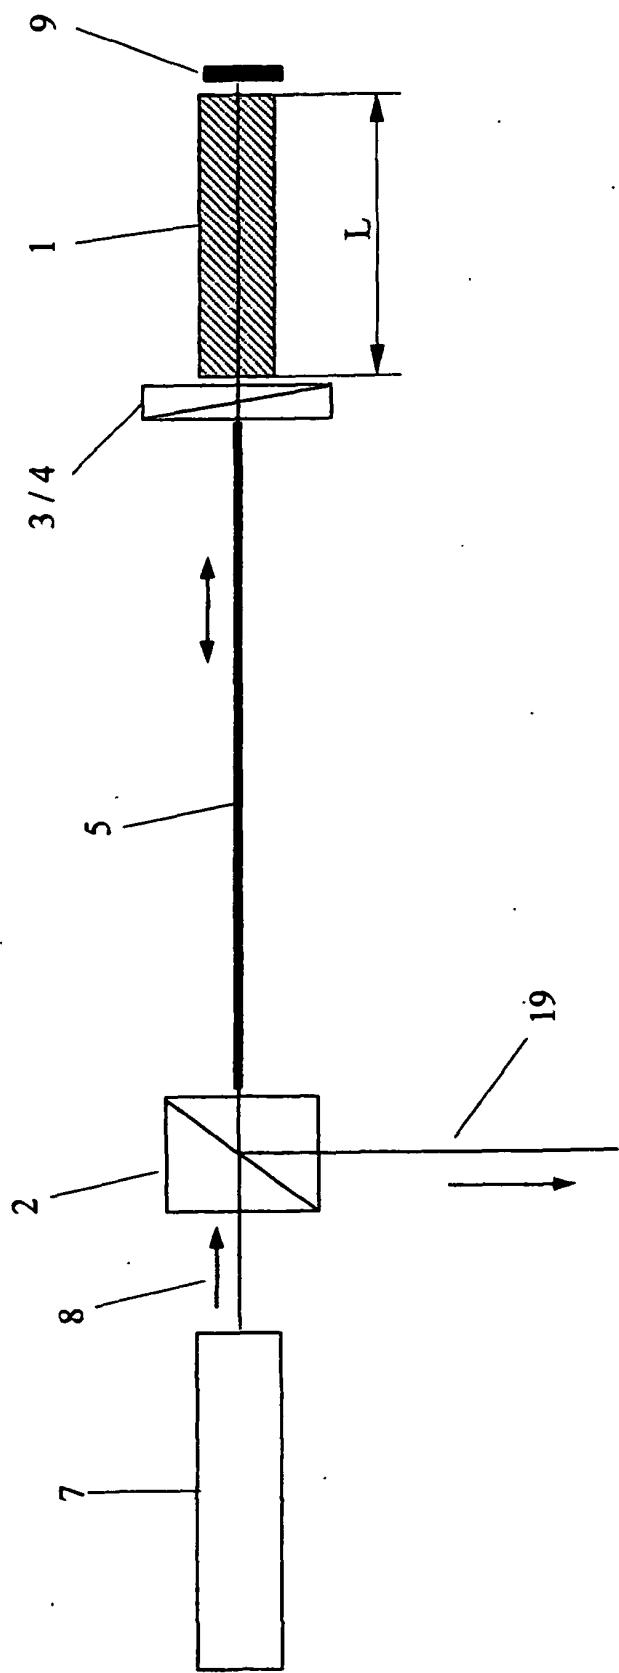


Fig. 1b

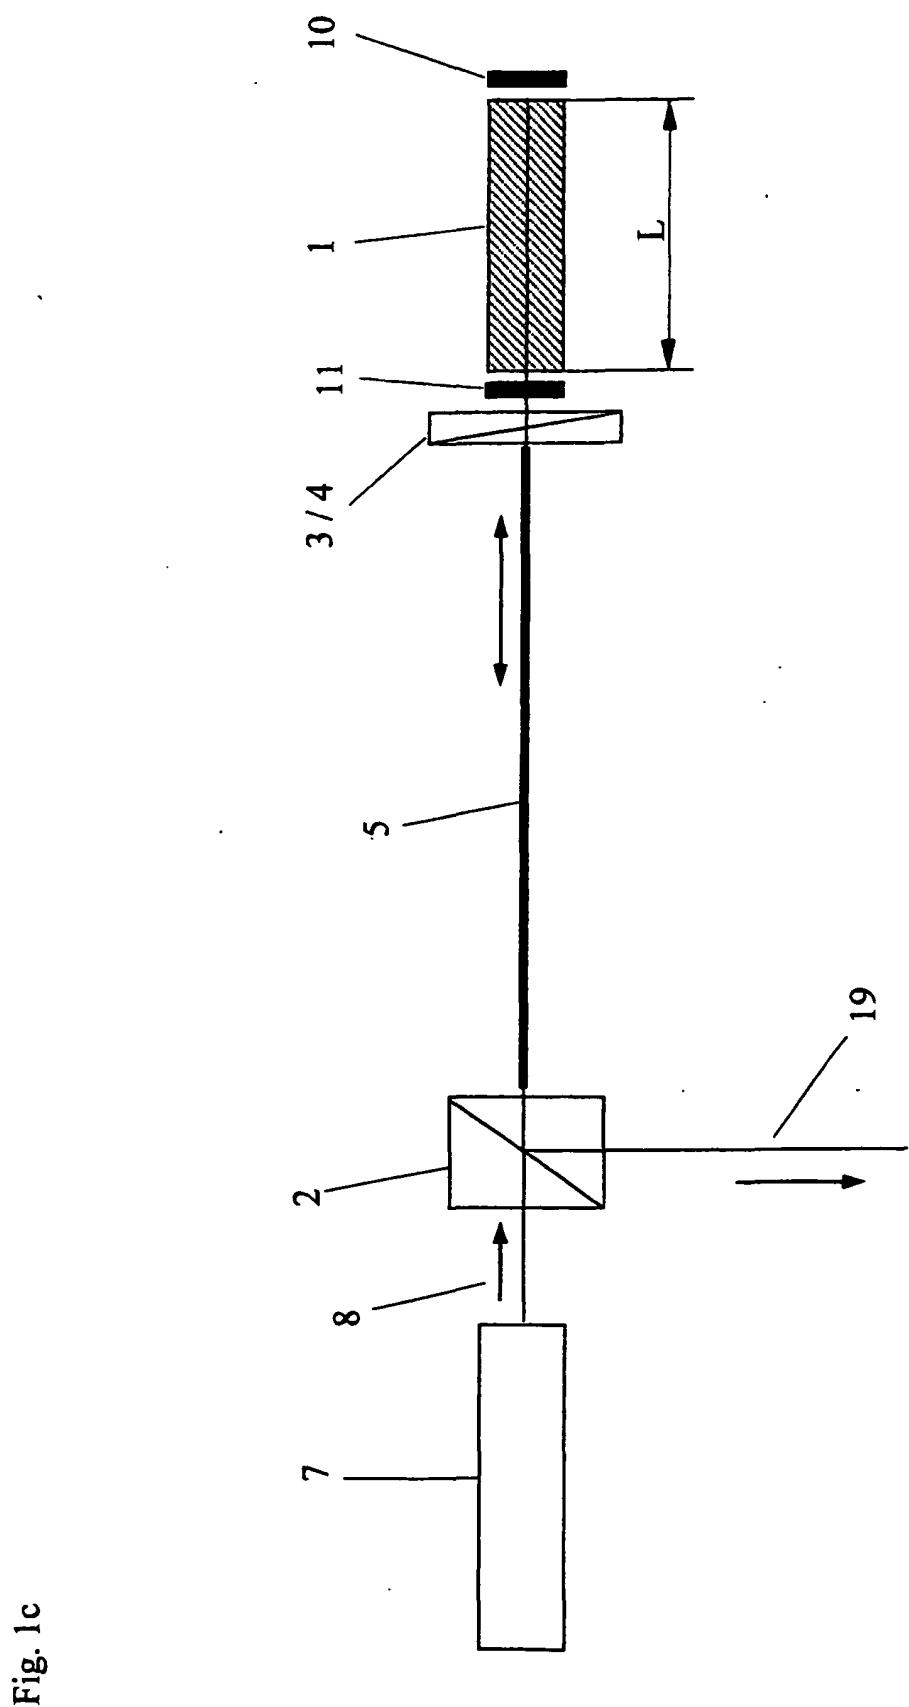


Fig. 1c

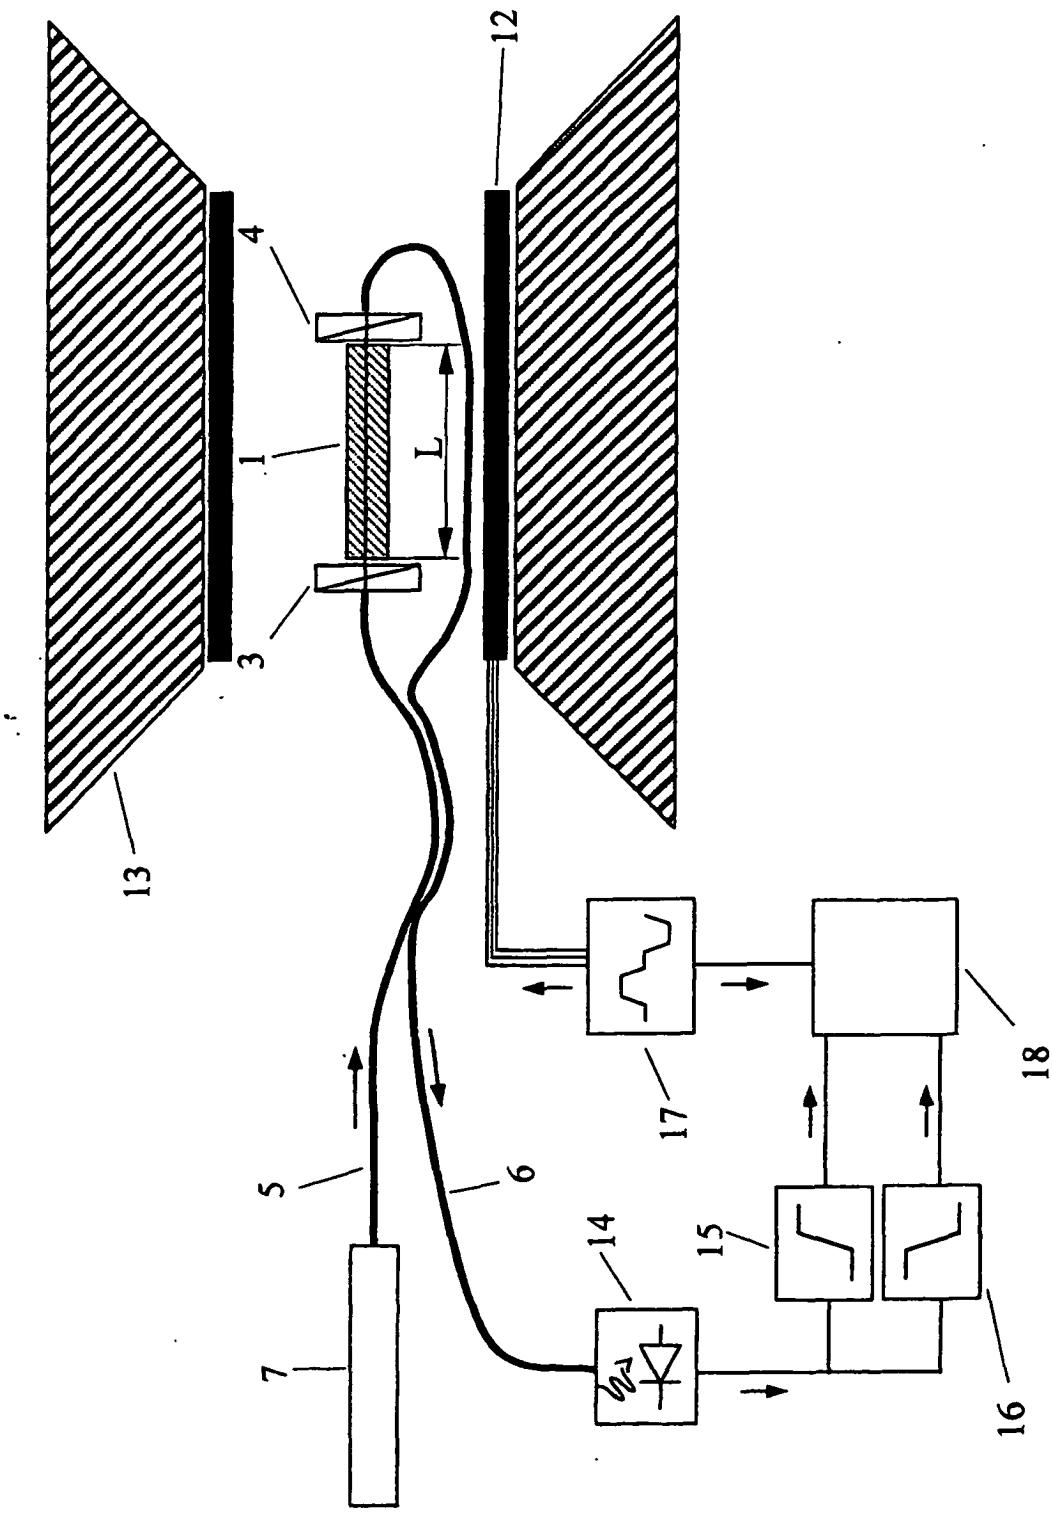


Fig. 2

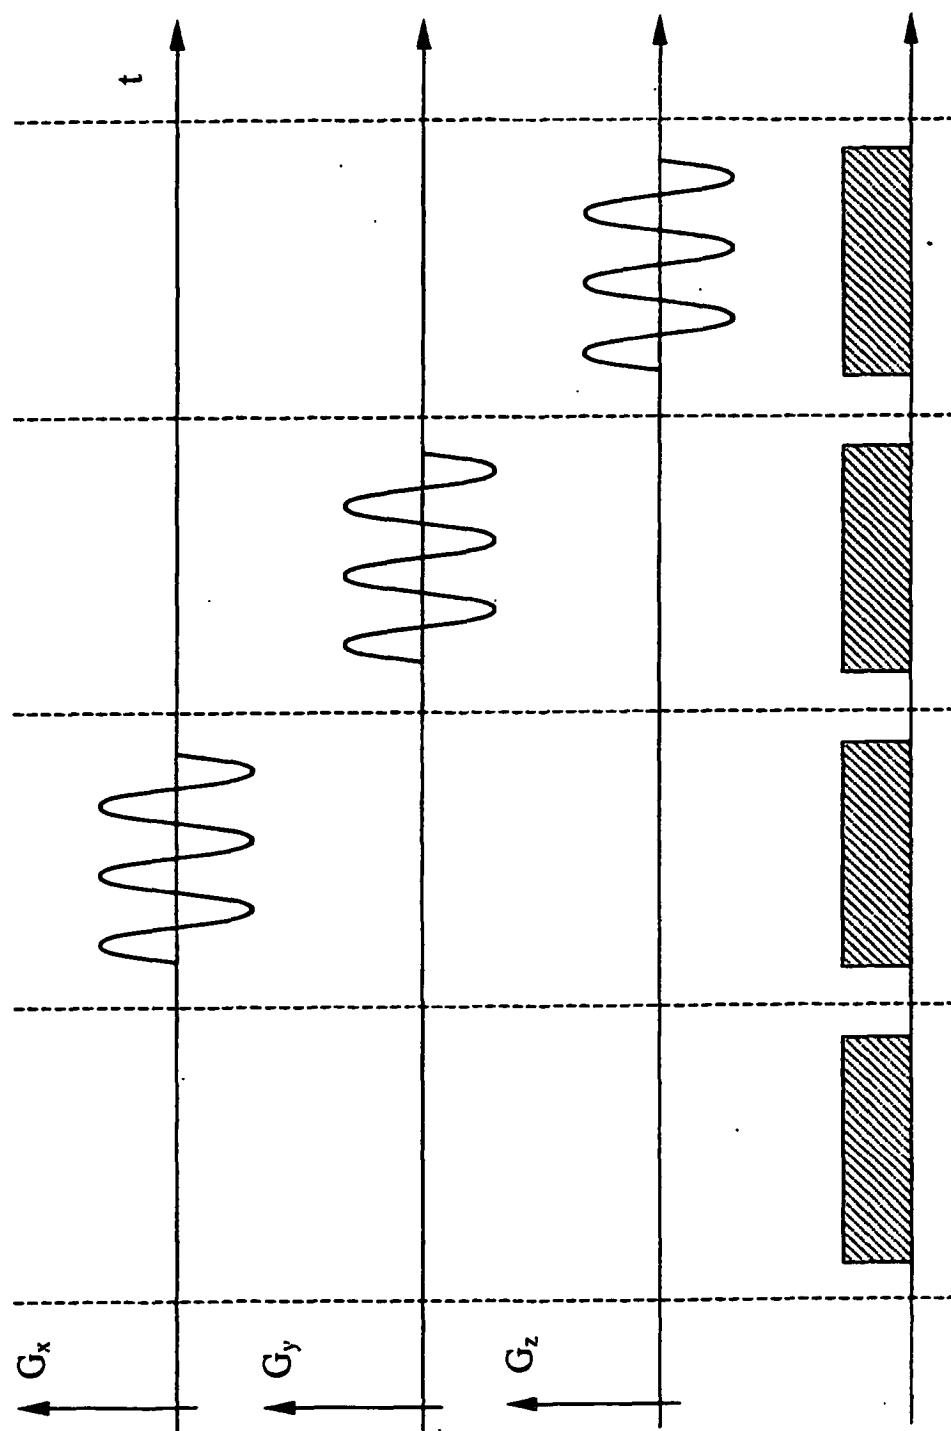


Fig. 3

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5154179 A [0005]
- US 4989608 A [0005]
- US 5868674 A [0006]
- US 5211165 A [0008]
- US 5375596 A [0008]
- US 4572198 A [0008]
- US 5882305 A [0008]
- US 6223066 B1 [0010]

Non-patent literature cited in the description

- **RUBINSETIN CB ; VAN UITERT LG ; GRODKIEWICZ WH.** Magneto-optical properties of rare earth (III) aluminum garnets. *J. Appl. Phys.*, 1964, vol. 35, 3069-70 [0041]

| | | | |
|----------------|---|---------|------------|
| 专利名称(译) | 用于检测侵入装置的位置和取向的装置 | | |
| 公开(公告)号 | EP1437601B1 | 公开(公告)日 | 2007-06-20 |
| 申请号 | EP2003000554 | 申请日 | 2003-01-10 |
| [标]申请(专利权)人(译) | 德国癌症研究公共权益基金会 | | |
| 申请(专利权)人(译) | DEUTSCHES KREBSFORSCHUNGSZENTRUM STIFTUNG DESÖFFENTLICHENRECHTS | | |
| 当前申请(专利权)人(译) | DEUTSCHES KREBSFORSCHUNGSZENTRUM STIFTUNG DESÖFFENTLICHENRECHTS | | |
| [标]发明人 | BOCK MICHAEL UMATHUM REINER ZABEL HANS JOACHIM | | |
| 发明人 | BOCK, MICHAEL UMATHUM, REINER ZABEL, HANS-JOACHIM | | |
| IPC分类号 | G01R33/28 A61B5/055 G01R33/032 | | |
| CPC分类号 | G01R33/287 G01R33/0322 | | |
| 其他公开文献 | EP1437601A1 | | |
| 外部链接 | Espacenet | | |

摘要(译)

本发明涉及一种用于测量磁共振成像设备内介入设备的位置和方向的方法和设备，该磁共振成像设备提供静磁场B0和具有已知磁通密度和方向的磁场梯度，包括以下步骤：(A)将法拉第传感器连接到介入装置，法拉第传感器连接到光学测量装置，(B)使用光学测量装置测量线性偏振光的偏振平面的旋转。法拉第传感器，同时将介入装置(i)暴露于静磁场B0，以及(ii)除了静磁场B0和(C)确定位置和方向之外，在所有三个空间方向上的场梯度。通过评估线性偏振光的偏振面的测量旋转来介入设备。

$\phi = VB_1$