

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
6 May 2004 (06.05.2004)


PCT

(10) International Publication Number
WO 2004/037102 A1

- (51) International Patent Classification⁷: A61B 18/18
- (21) International Application Number: PCT/IB2003/004459
- (22) International Filing Date: 9 October 2003 (09.10.2003)
- (25) Filing Language: Italian
- (26) Publication Language: English
- (30) Priority Data: PI2002A000059 22 October 2002 (22.10.2002) IT
- (71) Applicant and
(72) Inventor: LONGO, Iginio [IT/IT]; Largo Duca D'Aosta, 11, I-56123 Pisa (IT).
- (72) Inventor; and
(75) Inventor/Applicant (for US only): TOSORATTI, Nevio [IT/IT]; Via R. Alessandri, 50, I-00151 Roma (IT).
- (74) Agent: CELESTINO, Marco; ABM Agenzia Brevetti & Marchi, Viale Giovanni Pisano, 31, I-56123 Pisa (IT).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Published:**
- with international search report
 - before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: INTERSTITIAL MICROWAVE ANTENNA WITH LATERAL EFFECT FOR TISSUES HYPERTHERMIA IN MINIMAL INVASIVE SURGERY

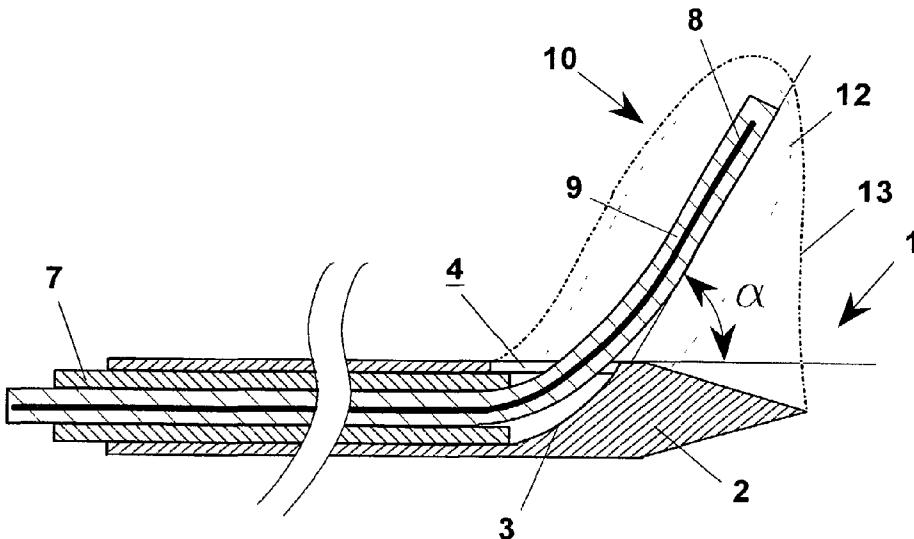

(57) **Abstract:** Application device (1), for example, a metal needle or a plastic catheter that has in the end portion (2) of the free end a gradually increasing thickness to form substantially a chute guide (3) which ends at a side opening (4) made on the application device (1). This way, an interstitial antenna (10) is obtained formed by a co-axial tube having an external conductor (7), by a dielectric layer (9) and by a central conductor (8) embedded in the dielectric layer (9) that insulates it from the external conductor (7). The antenna (10) can be put in a target tissue, along an actuation direction forming an angle α with the introduction direction. This way, the antenna (10) achieves an actual surface isothermal, i.e. a mass of tissue actually coagulated within a curved surface (13), since the tip of the application device (1) is connected electrically with the external conductor (7) and increases its area of action.

WO 2004/037102 A1

- 1 -

TITLE

INTERSTITIAL MICROWAVE ANTENNA WITH LATERAL EFFECT FOR TISSUES HYPERTHERMIA IN MINIMAL INVASIVE SURGERY

Field of the invention

The present invention relates to mininvasive surgery 5 techniques, for hyperthermia of solid deep wounds for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, especially in oncology. More precisely, the present invention relates to a microwave co-axial antenna 10 particularly indicated for hyperthermia of large tissue masses. Furthermore, the invention relates to a method for manufacturing such an antenna.

Description of the prior art

Hyperthermia in oncology is a method that has been 15 used for over 30 years for treatment of cancer (Hahn GM, Hyperthermia and Cancer, Plenum Press, in the York, 1982). It consists in heating cancer cells to obtain their necrosis either directly or with additional use of other methods such as radiotherapy, chemotherapy or other 20 surgery techniques.

For heating tissues, in particular for treatment of surface lesions, firstly electromagnetic waves have been used produced by a source located out of the human body.

More recently thin appliances have been used among 25 which microwave antennas, operating between several hundreds of MHz and several thousands of MHz, typically at 2450 MHz, created with a co-axial tube, for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications, suitable for the local treatment of deep 30 lesions (Iskander MF & Tumeh AM, Design Optimization of Interstitial Antennas, IEEE Transactions on Biomedical Engineering, 1989, 238-246).

- 2 -

Such antennas are usually inserted within the lesion to treat using catheters or metal needles, under computerised imaging techniques such as echographic guiding, TAC, NMR or other. They are suitable for being 5 used in combination with other actions such as drugs, ionizing waves and/or surgery ablation.

These microwave antennas, normally, are manufactured using a flexible or semi-rigid co-axial tube, suitably modified at one end, for conveying microwave power into 10 the tissues to cause hyperthermia.

The use of the minimally invasive microwaves coagulation therapy (TCMM) for percutaneous, laparoscopic applications, etc., is well known and widely documented in many industrial extra-European countries (USA, Japan, 15 Canada, China, etc.).

Such therapy provides introducing a small diameter co-axial antenna up to directly the centre of a lesion, of cancerous or hypertrophic tissue, normally through a introduction metal needle or a plastic catheter.

20 In figure 1 an axial cross section is shown of an antenna 100 integrated with a biopsy needle 100 of known art. The active part of the antenna, in the right side of the drawing, is suitably configured as a radiating dipole or monopole. More precisely, 107 is the external conductor 25 of the co-axial tube, 109 is the dielectric layer that insulates the external conductor from the central conductor 108. Isothermal surfaces having a rotationally symmetric configuration can be obtained by heating a biological tissue (not crossed by large blood vessels) 30 with a normal antenna 100, that for example is made by cutting at an end the portion of the external conductor 107 of the co-axial tube and leaving dielectric layer 109 uncovered as described in figure 1.

- 3 -

Once put within the lesion, the active end of the antenna exceeding the needle 101 emits microwave power (typically 60 W, at the frequency of 2450 MHz) sufficient to obtain in a few minutes the necrosis of a mass of 5 tissue of spheroidal shape 112: for example, for coagulating 10 ml of aqueous tissue 2-3 minutes are required. The coagulative necrosis induced by the treatment destroys the tissue, which, normally, remains in its position where it is subject to a fibrotic process, it 10 shrinks and does not affect further the adjacent zones. However, as the duration of the treatment and/or of the power supplied by the microwave antenna increase, the coagulated mass does not grow proportionally its volume, since the subtraction of heat by the blood circulation and 15 by diffusion for conductivity increases proportionally to the surface of the treated volume: the consequence is that with an antenna of conventional type it is possible to treat, in a single application, lesions with a diameter not more than 2-3 cm.

20 With the existing technology, to treat lesions of larger diameter (>3 cm), the application has to be repeated through successive insertions of a single antenna 100 as shown in figure 2A, or the simultaneous introductions of several antennas 100. As shown in figure 25 2B, in this case the use is known of a multiple support 120 to guide together all the needles (as an array). In both cases, the traumatic aspects of the hyperthermia treatments and the soreness immediately felt by the patient increase substantially.

30 It must be noted that if a single TCMM application is sufficient for treatment of a lesion of 3 cm of diameter, a lesion of 8 cm of diameter requires between 20 and 30 single operations, considering a 1 cm overlap safety factor. Then, the use of an array of antennas is

- 4 -

justified only if the lesion can be treated with not too many antennas, since otherwise the rate of invasivity is, in fact, comparable to that of a conventional surgical operation, and the same happens in case of a treatment 5 with a large number of consecutive insertions of a single applicator in different points.

Always as shown in figure 2A, by treating hepatic lesions in a percutaneous way using antenna 100 of conventional type, whereas lesion 20 can be treated even 10 if requiring numerous insertions for coagulating the whole mass, it is not instead possible to treat lesion 21 next to a large blood vessel 25 for high risk of perforating or coagulating the vessel same.

Furthermore, lesions of irregular shape or that 15 cannot be crossed longitudinally by the applicator are a further difficulty for conventional applicators presently in use.

Summary of the invention

It is a feature of the present invention to provide 20 a microwave co-axial antenna for applications in medicine and surgery for further reducing treatment invasivity of a minimally invasive microwaves coagulation therapy with respect to the prior art, avoiding both a multiplication of the number of applications required for treating large 25 lesions with a single antenna of conventional design (through repeated extraction and reintroduction of the applicator at different points of the tissue) both a requirement of an array of antennas.

It is also a feature of the present invention to 30 provide an antenna that is inserted into a lesion and proceeds in a direction lateral/oblique with respect to the axis of the application needle and with an adjustable angle.

- 5 -

It is a further a feature of the present invention to provide a method for the production of such an antenna and of its application device.

These and other features are accomplished with one exemplary antenna for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, in species for applications of acute hypertermia in oncology, comprising:

- 10 - an inner conductor,
- a dielectric layer that covers the inner conductor for all its length,
- an external conductor that covers coaxially the dielectric layer except from an end portion,
- a tubular application device for coaxially 15 guiding the antenna in a target tissue along an introduction direction,

whose characteristic is that the application device has in the end portion a side opening and a chute guide suitable for guiding the antenna through the side opening 20 causing it to enter the target tissue, along an actuation direction forming an angle α with the application device same.

Preferably, the application device is a metal needle or a plastic catheter which, in the end portion, has a 25 stiff blocking material, for example metal, having a tapered inner face forming said chute guide and a sharp external face.

Alternatively, the application device in the end portion has a gradually increasing thickness in order to 30 form said chute guide.

Advantageously, for allowing the introduction of the antenna in the target tissue along the actuation direction a metal flexible mandrel is provided sliding in the application device before introducing the antenna and

- 6 -

suitable for protruding from it through the side opening for making an inlet hole in the tissue to treat according to the actuation direction.

Once made the hole along the actuation direction, 5 the mandrel is extracted from the application device and replaced by the co-axial antenna that is inserted in the hole made previously by the mandrel for a length suitable for allowing a correct operation. When the treated zone has reached a predetermined temperature, the antenna is 10 withdrawn and can be inserted then in another position after having rotated the application device a certain angle or after having translated it along the introduction direction, without the need of making other inlet holes. This way, it is possible to apply hyperthermia to a mass 15 of tissue having an axial symmetry or to masses of irregular shape.

Furthermore, such an antenna allows to heat lesions located laterally with respect to the application device without that these are necessarily crossed by the needle. 20 This feature allows to treat lesions extending near large blood vessels, that cannot be treated with the antennas of prior art owing to a high risk of perforating the vessel.

In particular, it is possible to replace the needle with another having a different angle α for the actuation 25 direction with respect to the introduction direction. Within certain limits, the length can also be changed of the portion of antenna exceeding the opening. This way, the shape of the area of operation can be changed as preferred.

30 Brief description of the drawings

Further characteristics and advantages of the interstitial antenna, according to the present invention will be made clearer with the following description of an exemplary embodiment thereof, exemplifying but not

- 7 -

limitative, with reference to the further attached drawings wherein:

- figures 3 and 4 show a cross sectional axial view of an application device for an interstitial antenna, according 5 to the invention;
- figures 5 and 6 show in axial cross section an interstitial antenna, according to the invention;
- figure 7 shows a cross sectional axial view of an alternative exemplary embodiment for the application 10 device of figure 3;
- figure 8 shows diagrammatically a possible use of the interstitial antenna of figures 5 and 6.

Description of a preferred exemplary embodiment

In figure 3, an application device 1 according to 15 the invention is shown, in an axial cross section, for example a metal needle or a plastic catheter that has in the end portion 2 of its free end a gradually increasing thickness to form substantially a chute guide 3 which ends at a side opening 4 made on application device 1. This 20 way, an interstitial antenna 10 is obtained (figure 6) formed by a co-axial tube having an external conductor 7, by a dielectric cable 9 and by a central conductor 8 embedded in the dielectric cable 9 that insulates it from the external conductor 7. The antenna 10 can be put in a 25 target tissue, along an actuation direction forming an angle α with the introduction direction.

With reference to figure 4, for allowing the introduction of cable 9 in the target tissue along the actuation direction a metal flexible mandrel is provided 30 5, suitably shaped, sliding in application device 1 and capable of protruding from it through the side opening 4 for making an inlet hole in the tissue to treat according to the actuation direction forming an angle α with the introduction direction.

- 8 -

Then, once made the hole along the actuation direction, the mandrel 5 is extracted from application device 1 and replaced by cable 9 that is inserted in the hole made previously by the mandrel 5 for a length 5 suitable for allowing a correct operation (figure 6).

In particular, a calculated isothermal surface obtained by the antenna is indicated in figure 6 by a curved dashed line 12, whereas the actual isothermal surface, i.e. the mass of tissue actually coagulated is 10 enclosed within a curved line 13, since the tip of application device 1 is connected electrically with the external conductor 7 and increases its area of action.

When the treated zone has reached a predetermined temperature, cable 9 is withdrawn and it can be put 15 forward again after having rotated application device 1 of a certain angle or after having translated it along the introduction direction, without the need of making other inlet holes 11, as shown in figure 8. It is sufficient to repeat the above operations with mandrel 5 and then cable 20 9. This way, it is possible to reduce remarkably the treatment invasivity avoiding both to multiply the number of applications required for treating large lesions 20 with a single antenna 100 of conventional design (figure 2A) both to use an array of antennas (figure 2B), which 25 requires a single hole but of much larger diameter.

Furthermore, the antenna 10, according to the invention, allows to heat lesions located laterally with respect to application device 1 without that they are crossed by a hole. This feature allows to treat lesions 21 30 extending near a large blood vessel 25, that cannot be treated with the antennas of prior art (figure 2A), for high risk of perforating the vessel 25 same.

In figure 7 an alternative exemplary embodiment is shown for application device 1. This embodiment provides

- 9 -

that the metal needle or the plastic catheter 1 are associated to a block 6 of stiff material, for example metal, having a side opening 4, a tapered inner face forming the chute guide 3 and a sharp external face. 5 Needle 1 and block 6 are releasably engaged, for example, by a screw threaded coupling 1a-1b. This way, it is possible to change as desired the shape of the area of operation simply replacing the block 6 for adjusting the angle α of the actuation direction with respect to the 10 introduction direction.

The foregoing description of a specific embodiment will so fully reveal the invention according to the conceptual point of view, so that others, by applying current knowledge, will be able to modify and/or adapt for 15 various applications such an embodiment without further research and without parting from the invention, and it is therefore to be understood that such adaptations and modifications will have to be considered as equivalent to the specific embodiment. The means and the materials to 20 realise the different functions described herein could have a different nature without, for this reason, departing from the field of the invention. It is to be understood that the phraseology or terminology employed herein is for the purpose of description and not of 25 limitation.

- 10 -

CLAIMS

1. Microwave device for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, in species for applications of acute hypertermia in oncology, comprising:

- an inner conductor,
- a dielectric layer that covers said inner conductor for all its length,
- an external conductor that covers coaxially said dielectric layer except from an end portion, forming together with said dielectric layer and said inner conductor a co-axial antenna,
- a tubular application device for coaxially guiding said antenna in a target tissue along an introduction direction,

characterised in that said application device has in the end portion a side opening and a chute guide, said chute guide guiding said antenna through said side opening causing it to enter the target tissue along an actuation direction that forms an angle α with respect to said application device.

2. Microwave device for interstitial applications, according to claim 1, wherein said application device is a metal needle or a plastic catheter which, in the end portion, has a stiff blocking material, for example metal, having a tapered inner face forming said chute guide and a sharp external face.

3. Microwave device for interstitial applications, according to claim 1, wherein said application device is a hollow needle, blind in the end portion and having said side opening, wherein at said side opening a gradually increasing thickness is provided in order to form said chute guide.

- 11 -

4. Microwave device for interstitial applications, according to claim 1, wherein for the introduction of the antenna in the target tissue along the actuation direction a metal flexible mandrel is provided sliding in said application device before introducing the antenna and suitable for protruding from it through said side opening for making an inlet hole in the tissue to treat according said actuation direction.

- 1/4 -

Fig. 1
(prior art)

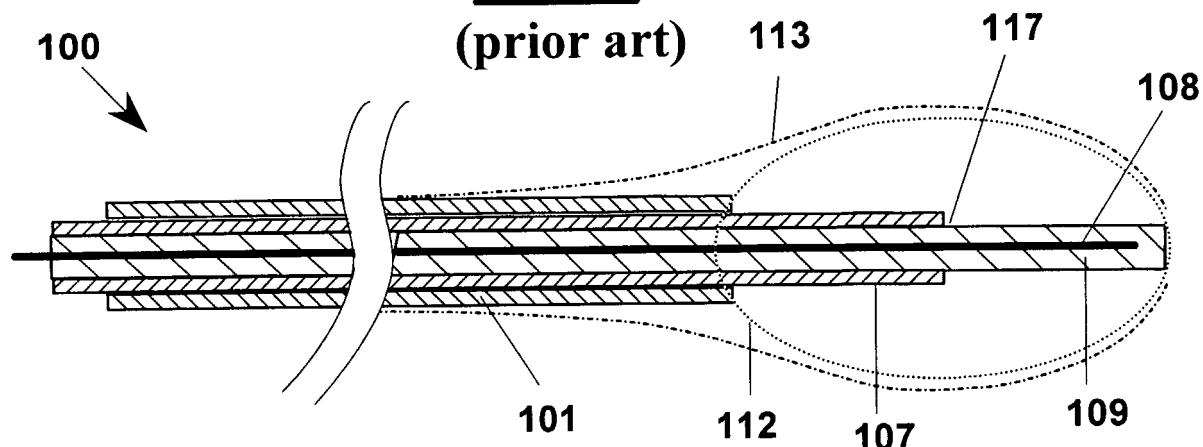


Fig. 2A

(prior art)




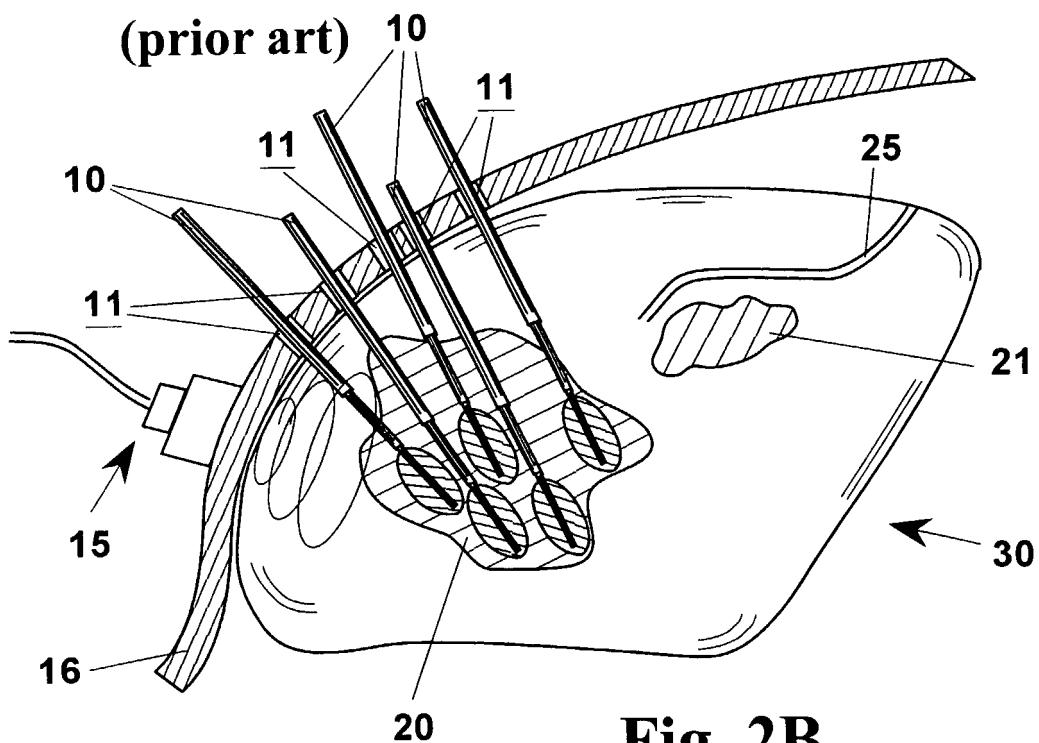


Fig. 2B



(prior art)

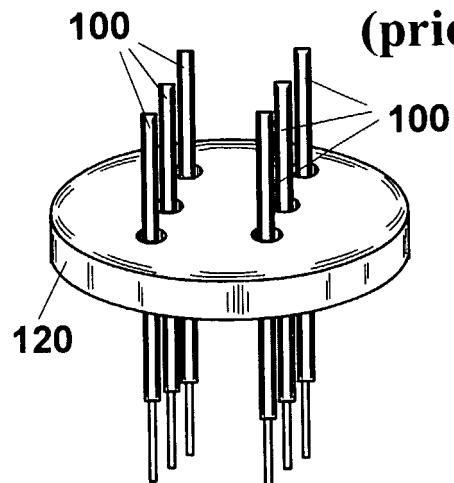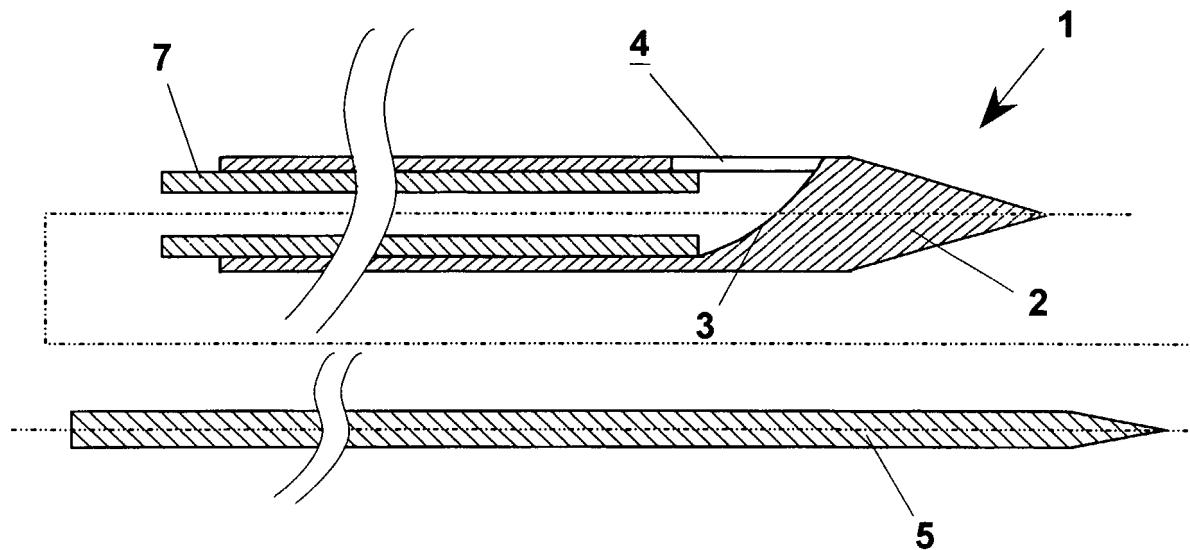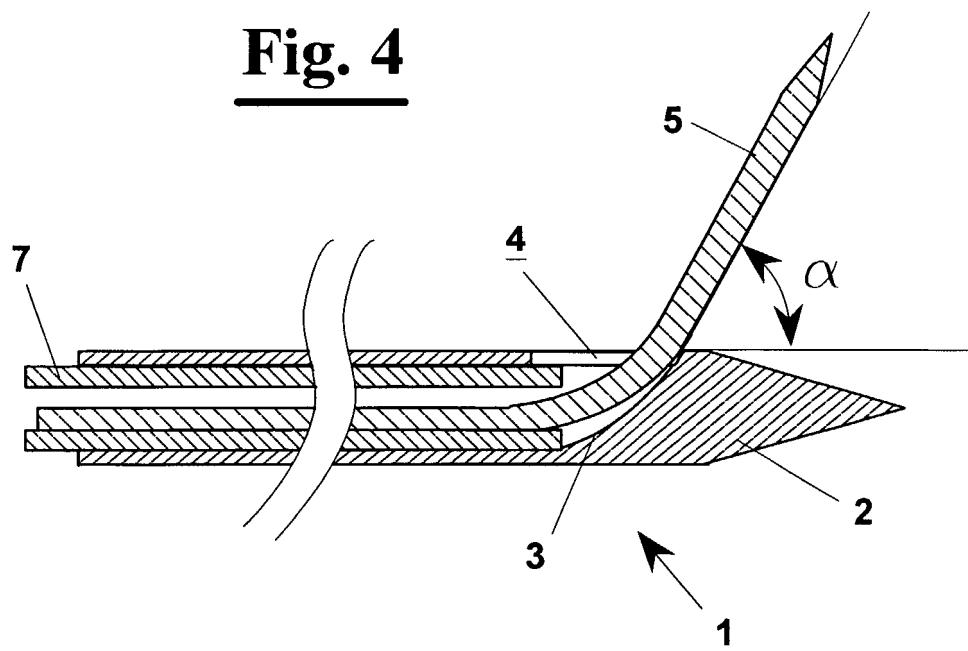

- 2/4 -

Fig. 3**Fig. 4**

- 3/4 -

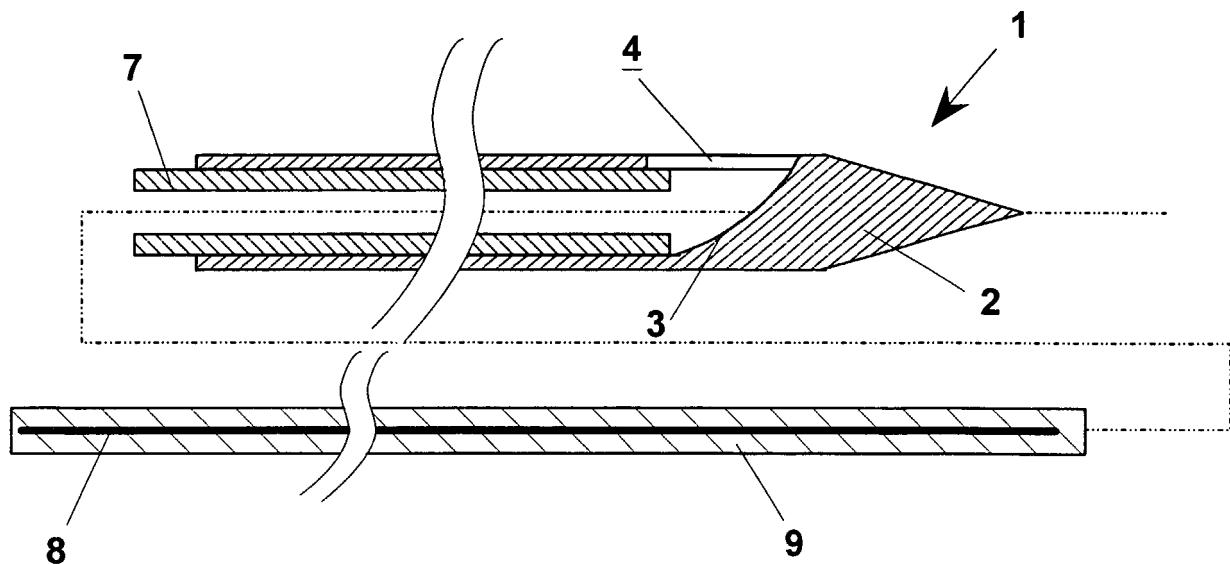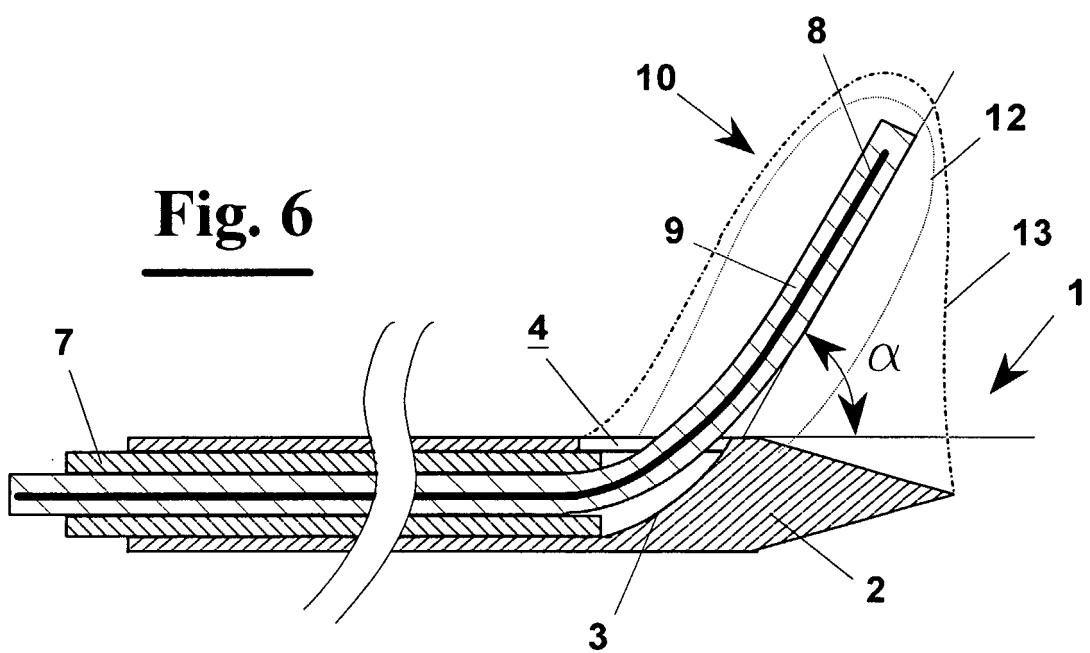Fig. 5**Fig. 6**

- 4/4 -

Fig. 7


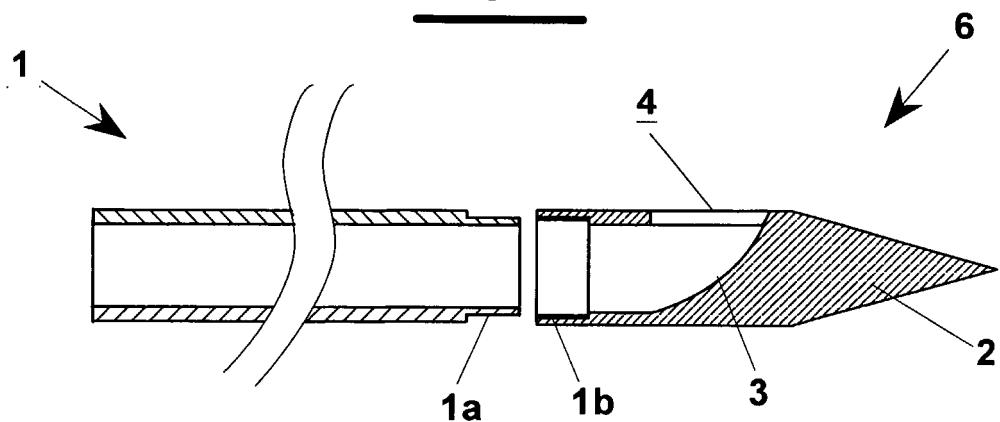


Fig. 8

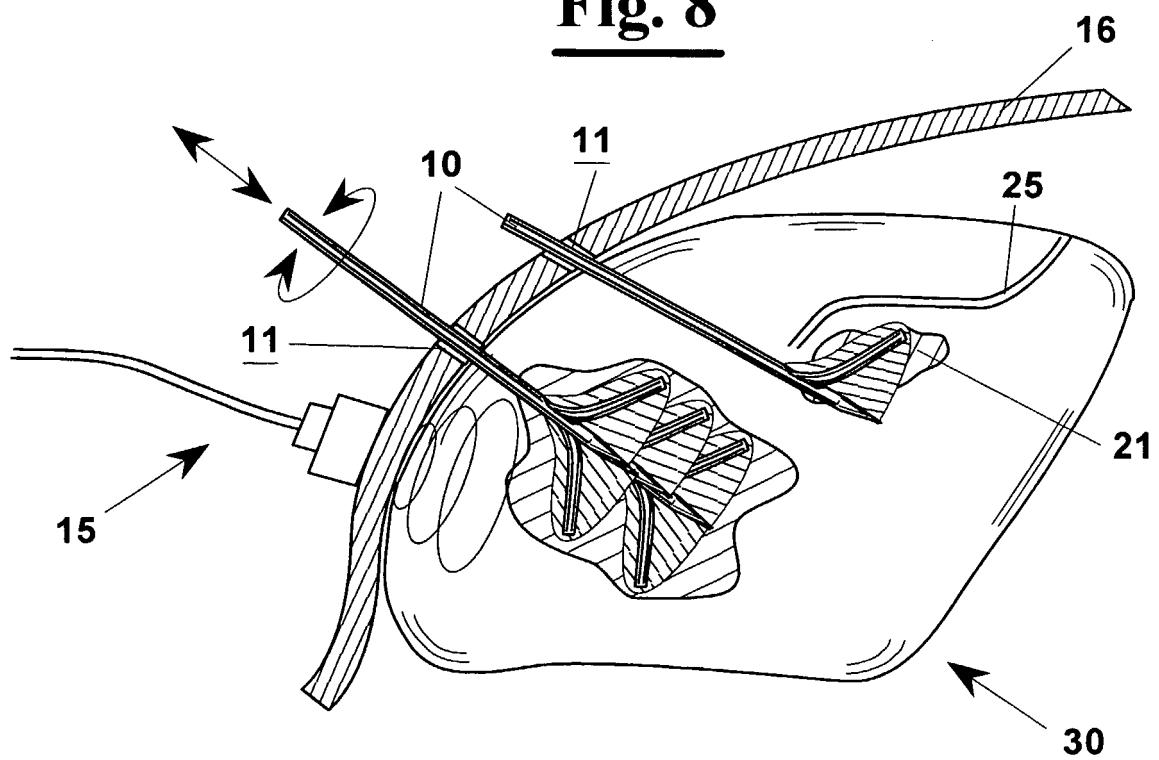

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB 03/04459

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B18/18

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, WPI Data, PAJ

C. DOCUMENTS CONSIDERED TO BE RELEVANT

| Category [*] | Citation of document, with indication, where appropriate, of the relevant passages | Relevant to claim No. |
|-----------------------|--|-----------------------|
| X | US 5 599 294 A (LUNDQUIST INGEMAR H ET AL) 4 February 1997 (1997-02-04) column 7, line 29 -column 8, line 16; figures 5,7-9 --- | 1, 3 |
| Y | WO 95 10253 A (UROLOGIX INC) 20 April 1995 (1995-04-20) page 9, line 1 - line 5 page 6, line 8 - line 13; figure 3 --- | 2, 4 |
| X | US 6 044 846 A (EDWARDS STUART D) 4 April 2000 (2000-04-04) column 5, line 42 - line 65; figures 6,7 --- | 1, 3 |
| X | US 2002/058932 A1 (MOORMAN JACK W ET AL) 16 May 2002 (2002-05-16) paragraphs '0046!, '0055!; figure 2 --- | 1 |
| Y | US 2002/058932 A1 (MOORMAN JACK W ET AL) 16 May 2002 (2002-05-16) paragraphs '0046!, '0055!; figure 2 --- | 4 |
| | | -/- |

Further documents are listed in the continuation of box C.

Patent family members are listed in annex.

^{*} Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

19 February 2004

Date of mailing of the international search report

27/02/2004

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl
Fax: (+31-70) 340-3016

Authorized officer

Mayer-Martenson, E

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB 03/04459

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

| Category | Citation of document, with indication, where appropriate, of the relevant passages | Relevant to claim No. |
|----------|--|-----------------------|
| Y | US 5 456 662 A (DOUGLASS DAVID L ET AL) 10 October 1995 (1995-10-10) column 4, line 35 - line 41; figures 5,6 ----- | 2 |

INTERNATIONAL SEARCH REPORT

International

Application No

PCT/IB 03/04459

| Patent document cited in search report | Publication date | Patent family member(s) | Publication date |
|--|------------------|--|--|
| US 5599294 | A 04-02-1997 | AT 132046 T AU 671405 B2 AU 2047595 A AU 657235 B2 AU 4999893 A BR 9306893 A CA 2121032 A1 CA 2226484 A1 DE 4305663 A1 DE 69301143 D1 DE 69325164 D1 DE 69325164 T2 EP 0611314 A1 EP 0629382 A1 EP 0893101 A2 ES 2084510 T3 ES 2134295 T3 FI 950584 A FR 2694700 A1 GB 2269538 A , B IL 104647 A JP 7503645 T JP 3128242 B2 KR 273015 B1 MX 9304905 A1 NZ 255687 A US 5370675 A US 2001031941 A1 US 5385544 A US 5421819 A US 6022334 A US 5435805 A US 6102886 A WO 9404220 A1 US 6241702 B1 US 5409453 A US 2002183740 A1 US 5470308 A US 5366490 A US 5556377 A US 5720718 A US 5542915 A US 5470309 A US 5554110 A US 5549644 A US 5484400 A US 6206847 B1 US 6129726 A US 5630794 A | 15-01-1996 22-08-1996 10-08-1995 02-03-1995 15-03-1994 08-12-1998 03-03-1994 03-03-1994 17-02-1994 08-02-1996 08-07-1999 25-05-2000 24-08-1994 21-12-1994 27-01-1999 01-05-1996 01-10-1999 04-04-1995 18-02-1994 16-02-1994 31-12-1995 20-04-1995 29-01-2001 01-12-2000 29-04-1994 20-12-1996 06-12-1994 18-10-2001 31-01-1995 06-06-1995 08-02-2000 25-07-1995 15-08-2000 03-03-1994 05-06-2001 25-04-1995 05-12-2002 28-11-1995 22-11-1994 17-09-1996 24-02-1998 06-08-1996 28-11-1995 10-09-1996 27-08-1996 16-01-1996 27-03-2001 10-10-2000 20-05-1997 |
| WO 9510253 | A 20-04-1995 | AU 8099794 A WO 9510253 A1 | 04-05-1995 20-04-1995 |
| US 6044846 | A 04-04-2000 | US 5964755 A US 5575788 A US 5558672 A US 5569241 A US 5505730 A | 12-10-1999 19-11-1996 24-09-1996 29-10-1996 09-04-1996 |

INTERNATIONAL SEARCH REPORT

International Application No.
PCT/IB 03/04459

| Patent document cited in search report | Publication date | Patent family member(s) | | Publication date |
|--|------------------|-------------------------|------------------|------------------|
| US 6044846 | A | AU 2882199 A | | 15-09-1999 |
| | | WO 9943262 A1 | | 02-09-1999 |
| | | US 2003135206 A1 | | 17-07-2003 |
| | | US 2003024538 A1 | | 06-02-2003 |
| | | WO 0176495 A1 | | 18-10-2001 |
| | | US 6024743 A | | 15-02-2000 |
| | | US 6302898 B1 | | 16-10-2001 |
| | | US 6006755 A | | 28-12-1999 |
| | | US 6009877 A | | 04-01-2000 |
| | | US 6056744 A | | 02-05-2000 |
| | | US 6092528 A | | 25-07-2000 |
| | | US 2003109866 A1 | | 12-06-2003 |
| | | US 6002968 A | | 14-12-1999 |
| | | US 6254598 B1 | | 03-07-2001 |
| | | US 6315776 B1 | | 13-11-2001 |
| | | US 6405732 B1 | | 18-06-2002 |
| | | US 2001034518 A1 | | 25-10-2001 |
| | | US 2002115991 A1 | | 22-08-2002 |
| | | US 2002103483 A1 | | 01-08-2002 |
| | | AU 2871795 A | | 19-01-1996 |
| | | NL 1000670 C2 | | 22-04-1996 |
| | | NL 1000670 A1 | | 27-12-1995 |
| | | WO 9600041 A1 | | 04-01-1996 |
| | | US 5681308 A | | 28-10-1997 |
| | | US 5769846 A | | 23-06-1998 |
| | | AU 707548 B2 | | 15-07-1999 |
| | | AU 2998195 A | | 19-01-1996 |
| | | CA 2193964 A1 | | 04-01-1996 |
| | | EP 0767629 A1 | | 16-04-1997 |
| | | WO 9600042 A1 | | 04-01-1996 |
| | | US 2003144659 A1 | | 31-07-2003 |
| | | US 2002091381 A1 | | 11-07-2002 |
| | | US 5827273 A | | 27-10-1998 |
| | | US 5800429 A | | 01-09-1998 |
| | | US 5746224 A | | 05-05-1998 |
| | | US 5823197 A | | 20-10-1998 |
| | | US 5843077 A | | 01-12-1998 |
| US 2002058932 | A1 | 16-05-2002 | US 6306132 B1 | 23-10-2001 |
| | | | US 2003195500 A1 | 16-10-2003 |
| | | | US 2001039416 A1 | 08-11-2001 |
| US 5456662 | A | 10-10-1995 | US 5370675 A | 06-12-1994 |
| | | | US 5435805 A | 25-07-1995 |
| | | | US 5421819 A | 06-06-1995 |
| | | | US 5385544 A | 31-01-1995 |
| | | | US 6152143 A | 28-11-2000 |
| | | | US 6179803 B1 | 30-01-2001 |
| | | | US 5514131 A | 07-05-1996 |
| | | | US 6416491 B1 | 09-07-2002 |
| | | | US 5674191 A | 07-10-1997 |
| | | | US 5707349 A | 13-01-1998 |
| | | | US 5718702 A | 17-02-1998 |
| | | | US 5743870 A | 28-04-1998 |
| | | | US 5730719 A | 24-03-1998 |
| | | | US 5817049 A | 06-10-1998 |
| | | | US 5843021 A | 01-12-1998 |
| | | | US 5486161 A | 23-01-1996 |

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB 03/04459

| Patent document cited in search report | Publication date | Patent family member(s) | Publication date |
|--|------------------|-------------------------|------------------|
| US 5456662 | A | AT 132046 T | 15-01-1996 |
| | | AU 671405 B2 | 22-08-1996 |
| | | AU 2047595 A | 10-08-1995 |
| | | AU 657235 B2 | 02-03-1995 |
| | | AU 4999893 A | 15-03-1994 |
| | | AU 685086 B2 | 15-01-1998 |
| | | AU 6133194 A | 29-08-1994 |
| | | AU 718834 B2 | 20-04-2000 |
| | | AU 6189698 A | 09-07-1998 |
| | | BR 9306893 A | 08-12-1998 |
| | | CA 2121032 A1 | 03-03-1994 |
| | | CA 2155217 A1 | 18-08-1994 |
| | | CA 2226484 A1 | 03-03-1994 |
| | | CN 1119418 A | 27-03-1996 |
| | | DE 4305663 A1 | 17-02-1994 |
| | | DE 69301143 D1 | 08-02-1996 |
| | | DE 69325164 D1 | 08-07-1999 |
| | | DE 69325164 T2 | 25-05-2000 |
| | | EP 0611314 A1 | 24-08-1994 |
| | | EP 0629382 A1 | 21-12-1994 |
| | | EP 0631514 A1 | 04-01-1995 |
| | | EP 0893101 A2 | 27-01-1999 |
| | | ES 2084510 T3 | 01-05-1996 |
| | | ES 2134295 T3 | 01-10-1999 |
| | | FI 950584 A | 04-04-1995 |
| | | IL 104647 A | 31-12-1995 |
| | | IL 108532 A | 13-07-1997 |
| | | JP 7503645 T | 20-04-1995 |
| | | JP 3128242 B2 | 29-01-2001 |
| | | JP 8506259 T | 09-07-1996 |
| | | KR 273015 B1 | 01-12-2000 |
| | | MX 9304905 A1 | 29-04-1994 |
| | | NZ 255687 A | 20-12-1996 |
| | | US 2001031941 A1 | 18-10-2001 |

| | | | |
|----------------|------------------------------------|---------|------------|
| 专利名称(译) | 间质微波天线对微创手术组织热疗有侧向作用 | | |
| 公开(公告)号 | EP1553885A1 | 公开(公告)日 | 2005-07-20 |
| 申请号 | EP2003748430 | 申请日 | 2003-10-09 |
| [标]申请(专利权)人(译) | LONGO IGINIO | | |
| 申请(专利权)人(译) | LONGO , IGINIO | | |
| 当前申请(专利权)人(译) | LONGO , IGINIO | | |
| [标]发明人 | LONGO IGINIO TOSORATTI NEVIO | | |
| 发明人 | LONGO, IGINIO TOSORATTI, NEVIO | | |
| IPC分类号 | A61B18/18 | | |
| CPC分类号 | A61B18/18 A61B18/1815 A61B2018/183 | | |
| 优先权 | 102002901056955 2002-10-22 IT | | |
| 其他公开文献 | EP1553885B1 | | |
| 外部链接 | Espacenet | | |

摘要(译)

涂敷装置 (1) , 例如金属针或塑料导管 , 其在自由端的端部 (2) 中具有逐渐增加的厚度 , 以形成基本上在侧面开口处终止的斜槽引导件 (3) (4)) 在应用设备 (1) 上制作。这样 , 通过具有外部导体 (7) 的同轴管 , 通过介电层 (9) 和嵌入在介电层 (9) 中的中心导体 (8) 形成间隙天线 (10) 。使其与外部导体 (7) 绝缘。天线 (10) 可沿着与引入方向形成角度 α 的致动方向放入目标组织中。这样 , 由于施加装置 (1) 的尖端与外部导体 (7) 电连接 , 因此天线 (10) 实现了实际的表面等温 , 即在曲面 (13) 内实际凝结的大量组织。增加其行动领域。