



(51) International Patent Classification:

A61B 17/03 (2006.01) A61M 31/00 (2006.01)
A61B 17/34 (2006.01) A61F 2/84 (2006.01)

(21) International Application Number:

PCT/US2010/030531

(22) International Filing Date:

9 April 2010 (09.04.2010)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/212,296 9 April 2009 (09.04.2009) US
61/277,359 21 September 2009 (21.09.2009) US
61/280,896 9 November 2009 (09.11.2009) US

(71) Applicant (for all designated States except US): **CARDIOVASCULAR SYSTEMS, INC.** [US/US]; 4574 Country Lane, Livermore, CA 94550 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **HOUSER, Russell, A.** [US/US]; 4574 Country Lane, Livermore, CA 94550 (US). **BOWER, John, Hunter** [US/US]; 651 South N. Street, Livermore, CA 94550 (US). **DO, Paul, L.**

[US/US]; 1001 South 7th Street, San Jose, CA 95112 (US).

(74) Agent: **O'REGAN, Cecily, A.**; Greenberg Traurig LLP, 2450 Colorado Avenue, Suite 400 E., Santa Monica, CA 90404 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, SM,

[Continued on next page]

(54) Title: TISSUE CLOSURE DEVICES, DEVICE AND SYSTEMS FOR DELIVERY, KITS AND METHODS THEREFOR

(57) Abstract: The present invention relates to wound closure devices, devices and systems for delivery, kits and methods therefor. The wound closure devices can achieve wound closure in lieu of compression and can be configured to be quickly deployable by an introducer or from outside the body.

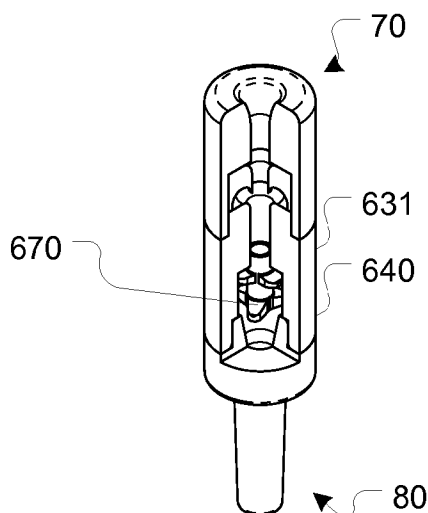


FIG. 65A



TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, **Published:**
ML, MR, NE, SN, TD, TG).

— *without international search report and to be republished
upon receipt of that report (Rule 48.2(g))*

TISSUE CLOSURE DEVICES, DEVICE AND SYSTEMS FOR DELIVERY, KITS AND METHODS THEREFOR

RELATED APPLICATIONS

[0001] This application claims priority to and the benefit of U.S. Provisional Patent Applications **61/212,296**, filed April 9, 2009, entitled "Introducer Sheath Adapter for the Atraumatic Delivery of a Medical Device," **61/277,359** filed September 21, 2009, entitled "Tissue Closure Device Systems and Methods," and **61/280,896** filed November 9, 2009, entitled "Bioabsorbable Plug Tissue Closure System," the disclosures of which are hereby incorporated by reference herein in their entirety and made a part of the present specification.

[0002] This application contains related disclosure to the following U.S. applications: U.S. Patent Application Serial Nos. **12/327,655** filed December 3, 2008, titled "Guided Tissue Cutting Device, Method of Use and Kits Therefor," **12/263,322** filed October 31, 2008, titled "Vascular Closure Devices, Systems, and Methods of Use," Provisional Applications **61/005,435**, filed December 3, 2007 and entitled "Guided Tissue Cutting Device and Method of Use," **61/190,100**, filed August 26, 2008 and entitled "Tissue Closure Devices, Systems and Methods of Use," and which in turn is a continuation in-part of **10/183,396** filed June 28, 2002, now U.S. Patent **6,726,696**, Application **10/127,714**, filed April 23, 2002 and entitled "Arteriotomy Closure Devices and Techniques," and Provisional Patent Application Nos. **60/286,269**, filed April 24, 2001 and entitled "Percutaneous Vessel Access Closure Device and Method," **60/300,892**, filed June 25, 2001 and entitled "Percutaneous Vessel Access Closure Device and Method," **60/302,255**, filed June 28, 2001 and entitled "Percutaneous Vessel Access Closure Device and Method (Hemostatic Patch or Collar)," the disclosures of which are hereby incorporated by reference herein in their entirety and made a part of the present specification.

BACKGROUND OF THE INVENTION

A. FIELD OF THE INVENTION

[0003] The invention generally relates to medical devices and techniques, and more particularly to cardiovascular tissue closure devices, systems, techniques and kits.

B. DESCRIPTION OF THE RELATED ART

[0004] In most cardiology and radiology procedures, a catheter is inserted into an artery, such as the femoral artery, through a vascular introducer. When the procedure is complete, the physician removes the catheter from the introducer and then removes the introducer from the arteriotomy or incision or opening into the lumen in the vessel. The physician then must prevent or limit the amount of blood that leaks through the arteriotomy so that the patient can be discharged.

Physicians currently use a number of methods to close the arteriotomy, such as localized compression, sutures, collagen plugs, adhesives, gels, foams, clips, and similar materials.

[0005] In performing localized compression, the physician presses down against the vessel to allow the arteriotomy to naturally clot. This method, however, can take a significant amount of time, and requires the patient to remain immobilized and kept in the hospital for observation. Moreover, clots at the puncture site may also be dislodged. The amount of time necessary for the compression can significantly increase depending upon how much heparin, glycoprotein IIb/IIA antagonists, or other anti-clotting agents were used during the procedure. Sutures and collagen plugs can have procedure variability, can require time to close the vessel, and can necessitate a separate deployment device. Adhesives, gels, foams, and clips can have negative cost factors, can necessitate a complicated deployment process, and can have procedure variability.

SUMMARY OF THE INVENTION

[0006] An aspect of the disclosure is directed to a closure device. The closure device comprises: a distal flexible cap; one or more proximally positioned radial extending elements; a stem positioned between the distal flexible cap and the one or more radial extending element, wherein the distal flexible cap is formable toward an axis. In at least some configurations, the distal flexible cap can be configured such that it has at least one of a substantially flat distal surface and a substantially flat proximal surface, a substantially flat distal surface and a substantially concave proximal surface, a substantially flat distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially flat proximal surface, a substantially convex distal surface and a substantially concave proximal surface, a substantially convex distal surface and a substantially convex proximal surface, a substantially concave distal surface and a substantially flat proximal surface, a substantially concave distal surface and a substantially concave proximal surface, and a substantially concave distal surface and a substantially convex proximal surface. Additionally, the distal flexible cap can have at least one of a uniform thickness in a cross-section or a variable thickness in a cross-section. In some configurations, the proximal surface of the distal flexible cap has one of more of at least one of anchoring protrusions, nibs or ribs. The distal flexible cap can also be configured to have a shape selected from round, triangular, oval, ovoid, elliptical, square, and saucer. The flexible cap shape can have rounded edges. Additionally, the stem can be positioned on a proximal surface of the flexible cap at least one of centrally and non-centrally. A proximally accessible stem bore can also be provided. Additionally, a clip can be positionable within the proximal bore. The proximally accessible stem bore can also have at least one of internal threads along an interior surface, parallel walls along its length, non-parallel walls along its length, an undercut in the bore at a location along its length, and a bent bore along its length. Additionally, the bore can be configured to extend from the proximal end of the device to the proximal end of the flexible cap. A wide variety of configurations for the stem are possible as will be appreciated. A few

of the configurations include, for example, cross-sectional profile shapes selected from the group comprising square, triangular, arrowhead, trapezoidal, rectangular, J, Y, hook, and bulbous. The stem can further comprise a proximally positioned aperture therethrough, one or more exterior features adapted and configured to achieve anchoring the stem in vivo, one or more slots along at least a portion of its length parallel to a stem longitudinal axis beginning at its proximal end, a configuration which enables it to open away from the longitudinal axis from its proximal end, a proximal end adapted and configured to form a clasp, a socket, a breakable stem, a tearable stem, and/or at least one of the distal flexible cap and stem are in releasable communication with a tether. Additionally, a tether can be provided. The tether can be one or more of a wire, a spring, a thread, a ribbon, and a tube. Wire can at least be one of a bent wire, a curved wire, a wavy wire, and a helical wire.

[0007] Another aspect of the disclosure is directed to a delivery capsule. The delivery capsule comprises: a cartridge body; a tapered distal tip; a compressible section; a clear section; a lumen extending therethrough, wherein the clear section is adapted and configured to house a closure device. The delivery capsule can be further adapted and configured to comprise a valve, one or more proximally positioned detent features on an exterior surface of the cartridge body, one or more distally positioned undercuts, an exterior groove in the cartridge body, a one-way snap feature, an undercut central bore, and/or a central aperture adapted and configured to receive a plunger. Where the capsule receives a plunger it can further be configured to permit the plunger to move in a first axial direction and resist movement in a second axial direction different than the first direction. One or more collets can also be provided.

[0008] Still another aspect of the disclosure is directed to a wound closure delivery system. The wound closure delivery system comprises: an introducer; a wound closure delivery cartridge; a guide and seal assembly; and a plunger wherein the introducer is adapted and configured to releasably engage the wound closure delivery cartridge at a proximal end, the wound closure delivery cartridge is adapted and configured to releasably engage the guide and seal assembly at a proximal end, and the plunger is adapted and configured to be advanced through a lumen in each of the guide and seal assembly, the wound closure delivery cartridge and the introducer. In at least some configurations, the distal flexible cap can be configured such that it has at least one of a substantially flat distal surface and a substantially flat proximal surface, a substantially flat distal surface and a substantially concave proximal surface, a substantially flat distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially flat proximal surface, a substantially convex distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially concave proximal surface, a substantially concave distal surface and a substantially flat proximal surface, a substantially concave distal surface and a substantially concave proximal surface, and a substantially concave distal surface and a substantially convex proximal surface. Additionally, the distal flexible cap can have at least one of a uniform thickness in a cross-section or a variable thickness in a cross-section. In some configurations, the proximal surface of the

distal flexible cap has one of more of at least one of anchoring protrusions, nibs or ribs. The distal flexible cap can also be configured to have a shape selected from round, triangular, oval, ovoid, elliptical, square, and saucer. The flexible cap shape can have rounded edges. Additionally, the stem can be positioned on a proximal surface of the flexible cap at least one of centrally and non-centrally. A proximally accessible stem bore can also be provided. Additionally, a clip can be positionable within the proximal bore. The proximally accessible stem bore can also have at least one of internal threads along an interior surface, parallel walls along its length, non-parallel walls along its length, an undercut in the bore at a location along its length, and a bent bore along its length. Additionally, the bore can be configured to extend from the proximal end of the device to the proximal end of the flexible cap. A wide variety of configurations for the stem are possible as will be appreciated. A few of the configurations include, for example, cross-sectional profile shapes selected from the group comprising square, triangular, arrowhead, trapezoidal, rectangular, J, Y, hook, and bulbous. The stem can further comprise a proximally positioned aperture therethrough, one or more exterior features adapted and configured to achieve anchoring the stem in vivo, one or more slots along at least a portion of its length parallel to a stem longitudinal axis beginning at its proximal end, a configuration which enables it to open away from the longitudinal axis from its proximal end, a proximal end adapted and configured to form a clasp, a socket, a breakable stem, a tearable stem, and/or at least one of the distal flexible cap and stem are in releasable communication with a tether. Additionally, a tether can be provided. The tether can be one or more of a wire, a spring, a thread, a ribbon, and a tube. Wire can at least be one of a bent wire, a curved wire, a wavy wire, and a helical wire. The delivery capsule can be further adapted and configured to comprise a valve, one or more proximally positioned detent features on an exterior surface of the cartridge body, one or more distally positioned undercuts, an exterior groove in the cartridge body, a one-way snap feature, an undercut central bore, and/or a central aperture adapted and configured to receive a plunger. Where the capsule receives a plunger it can further be configured to permit the plunger to move in a first axial direction and resist movement in a second axial direction different than the first direction. One or more collets can also be provided.

[0009] Yet another aspect of the disclosure is directed to a method of closing a wound. Suitable methods comprise: assembling a wound closure system comprising a guide and seal assembly, a closure device delivery capsule, and an introducer; inserting the assembled wound closure system percutaneously; centering a mammalian vessel with a distal tip of a tubular sheath of the introducer; and inserting a plunger into a proximal aperture in the guide and seal assembly; advancing the plunger through the guide and seal assembly into the closure device delivery capsule; engaging the closure device at the tip of the plunger; advancing the closure device into a tapered tip and reducing a profile of the closure device in at least one plane; advancing the closure device beyond the distal tip of the tubular sheath of the introducer and into the vessel; and withdrawing the system until a proximal surface of a face plate of the closure device comes in contact with an interior surface of the mammalian vessel; disengaging the closure device from the interior of the introducer. Additionally, at

least one of the steps of pulling a tether connected to a proximal end of the closure device , and releasing the tether connected to the proximal end of the closure device.

[0010] Still other aspects are directed to a kit for a percutaneous procedure comprising a closure device delivery capsule housing a closure device; an introducer; a guide and seal assembly; and a plunger. The kit can further comprise one or more items selected from the group consisting of needles, hypo tubes, guidewires, electrode wires, intravenous wires, vascular introducers, catheters, laparoscopes, endoscopes, trocars, and cannulas, one or more compounds for delivery to a tissue, and/or one or more items selected from the group consisting of a pair of scissors, a scalpel, a swab, a syringe, a hemostat, a lubricant, a needle, a snare, an antiseptic, and an anesthetic. Suitable compounds include, for example, one or more of a sclerosing agent, an antibiotic, and an anti-inflammatory agent.

INCORPORATION BY REFERENCE

[0011] All publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application was specifically and individually indicated to be incorporated by reference.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] The novel features of the invention are set forth with particularity in the appended claims. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are used, and the accompanying drawings of which:

[0013] **FIG. 1** shows a perspective view of an embodiment of a vessel closure system;

[0014] **FIG. 2** shows a perspective view of an embodiment of a vascular closure clip in an open or pre-deployed configuration;

[0015] **FIG. 3** shows a perspective view of the clip of **FIG. 2** in a closed or deployed configuration;

[0016] **FIG. 4** shows a side view of the clip of **FIG. 2** in an open configuration;

[0017] **FIG. 5** shows a side view of the clip of **FIG. 2** in a closed configuration;

[0018] **FIG. 6** shows a bottom view of the clip of **FIG. 2** in a closed configuration;

[0019] **FIG. 7** shows a perspective view of a deployment instrument preloaded with a vascular closure clip;

[0020] **FIG. 8** shows a close-up view of the distal end of the deployment instrument of **FIG. 7**;

[0021] **FIG. 9** shows a perspective view of an inner tubular member portion of the deployment instrument of **FIG. 7**;

[0022] **FIG. 10** shows a side view of the inner tubular member of **FIG. 9**;

- [0023] FIG. 11 shows a distal end view of the inner tubular member of FIG. 9;
- [0024] FIG. 12 shows a perspective view of an outer tubular member portion of the deployment instrument of FIG. 7;
- [0025] FIG. 13 shows a distal end view of the outer tubular member of FIG. 12;
- [0026] FIG. 14 shows a side view of the outer tubular member of FIG. 12;
- [0027] FIG. 15 shows a close-up side view of an intermediate portion of the outer tubular member of FIG. 12;
- [0028] FIG. 16 shows another close-up side view of an intermediate portion of the outer tubular member of FIG. 12;
- [0029] FIG. 17 shows a perspective view of a pressure element of the deployment instrument of FIG. 7;
- [0030] FIG. 18 shows a perspective view of the deployment instrument of FIG. 7 loaded onto a vascular introducer that has been inserted into a patient's blood vessel;
- [0031] FIG. 19 shows a perspective view of the deployment instrument of FIG. 7 which has been advanced over the vascular introducer until its distal end encounters the vessel wall;
- [0032] FIG. 20 shows a close-up view of the deployment instrument of FIG. 19 showing the pressure element in an initial, relaxed position;
- [0033] FIG. 21 shows a perspective view of the deployment instrument of FIG. 7 with the pressure element fully advanced;
- [0034] FIG. 22 shows a close-up view of the deployment instrument of FIG. 21 showing the fully advanced pressure element;
- [0035] FIG. 23 shows a close-up side view of the deployment instrument of FIG. 7 in a partially-deployed state showing the clip's tines penetrating the vessel wall;
- [0036] FIG. 24 shows a perspective view of the deployment instrument of FIG. 7 in a partially-deployed state;
- [0037] FIG. 25 shows a close-up view of the distal end of the deployment instrument of FIG. 24;
- [0038] FIG. 26 shows a close-up bottom view of the proximal end of the deployment instrument of FIG. 24 showing the handle engaging the stop element;
- [0039] FIG. 27 shows a side view of the proximal end of the deployment instrument of FIG. 24 showing the handle engaging the stop element;
- [0040] FIG. 28 shows a side view of the deployment instrument of FIG. 24 in a partially deployed state after withdrawing the vascular introducer;
- [0041] FIG. 29 shows a side view of the proximal end of the deployment instrument of FIG. 27 showing how the stop element can be overcome;
- [0042] FIG. 30 shows a perspective view of the deployment instrument of FIG. 7 in a fully deployed configuration;

[0043] FIG. 31 shows a side view of the deployment instrument of FIG. 7 in a fully deployed configuration which shows the vascular closure clip closing the arteriotomy;

[0044] FIG. 32 shows a side view of the deployment instrument of FIG. 7 showing the deployment instrument being removed from the patient's body following deployment;

[0045] FIG. 33 shows a side view of a vascular closure procedure using a removable clip, showing the deployment instrument being advanced over the vascular introducer;

[0046] FIG. 34 shows a side view of the procedure of FIG. 33 showing the deployment instrument being removed after deploying the clip;

[0047] FIG. 35 shows a side view of the vascular closure procedure of FIG. 33 showing the vascular closure clip being removed from the patient's body following hemostasis;

[0048] FIG. 36 shows a perspective view of a clip loading mechanism;

[0049] FIG. 37 shows a perspective view of the clip loading mechanism of FIG. 36 fully inserted into the distal end of the deployment instrument;

[0050] FIG. 38 shows a perspective view of a pusher tool configured to mate with a vascular closure clip to fully advance the clip over the clip loading mechanism of FIG. 36 and onto the distal end of the deployment instrument;

[0051] FIG. 39 shows a perspective view of the pusher tool of FIG. 38 fully advancing the clip onto the distal end of the deployment instrument;

[0052] FIG. 40 shows a bottom view of a slidable tissue cutter;

[0053] FIG. 41 shows a perspective view of the slidable tissue cutter of FIG. 40;

[0054] FIG. 42 shows a bottom view of a frame which can constitute a first component of the slidable tissue cutter of FIG. 40;

[0055] FIG. 43 shows a distal end view of the frame of FIG. 42;

[0056] FIG. 44 shows a perspective view of a slidable tissue dilator;

[0057] FIG. 45 shows a distal end view of the slidable tissue dilator of FIG. 44;

[0058] FIG. 46 shows a side view of the slidable tissue dilator of FIG. 44;

[0059] FIG. 47A shows a perspective view of another embodiment of a vascular closure clip in an open configuration;

[0060] FIG. 47B shows a perspective view of the vascular closure clip of FIG. 47A in a closed configuration;

[0061] FIG. 47C shows a bottom view of the vascular closure clip of FIG. 47A in a closed configuration;

[0062] FIG. 47D shows a side view of the vascular closure clip of FIG. 47A in a closed configuration;

[0063] FIG. 48A shows a perspective view of another embodiment of a vascular closure clip in a closed configuration;

- [0064] FIG. 48B shows a perspective view of the vascular closure clip of FIG. 48A in an open configuration;
- [0065] FIG. 49A shows a perspective view of another embodiment of a vascular closure clip in an open configuration;
- [0066] FIG. 49B shows a perspective view of the vascular closure clip of FIG. 49B in a closed configuration;
- [0067] FIG. 50A shows a perspective view of another embodiment of a vascular closure clip in an open configuration;
- [0068] FIG. 50B shows a perspective view of the vascular closure clip of FIG. 50A in a closed configuration;
- [0069] FIG. 51A shows a perspective view of another embodiment of a vascular closure clip in an open configuration; FIG. 51B shows a perspective view of the vascular closure clip of FIG. 51A in a closed configuration; FIG. 51C shows a side view of the vascular closure clip of FIG. 51A in an open configuration; FIG. 51D shows a side view of the vascular closure clip of FIG. 51A in a closed configuration; FIG. 51E shows a top view of the vascular closure clip of FIG. 51A in a closed configuration;
- [0070] FIG. 52 shows a circuit diagram of a circuit using direct resistive element heating to heat tissue surrounding the arteriotomy;
- [0071] FIG. 53 shows a circuit diagram of a circuit using ohmic tissue heating to heat tissue surrounding the arteriotomy;
- [0072] FIG. 54 shows a distal end view of another embodiment of an inner tubular member that can form one component of a deployment instrument;
- [0073] FIG. 55 shows a proximal end view of the inner tubular member of FIG. 54;
- [0074] FIG. 56A shows a perspective view another embodiment of a deployment instrument which can be used with a vascular closure plug; FIG. 56B shows a perspective view of the deployment instrument of FIG. 56A preloaded with a vascular closure plug; FIG. 56C shows a perspective view of the deployment instrument of FIG. 56A after deploying the vascular closure plug;
- [0075] FIG. 57 shows a side view of the deployment instrument of FIG. 56B being advanced over a vascular introducer that has been inserted into a patient's blood vessel;
- [0076] FIG. 58 shows a side view of the deployment instrument of FIG. 57 positioning the distal end of the vascular closure plug against the arteriotomy;
- [0077] FIG. 59 shows a side view of the deployment instrument of FIG. 57 holding the plug against the arteriotomy after removing the vascular introducer;
- [0078] FIG. 60 shows a side view of the deployment instrument of FIG. 57 showing the exposed portions of the plug beginning to swell;
- [0079] FIG. 61 shows a side view of a deployed plug as the deployment instrument of FIG. 57 is removed;

[0080] FIG. 62 shows a side view of the deployed plug of FIG. 61 which is continuing to swell; and

[0081] FIG. 63 shows a side view of the deployed plug of FIG. 61 which has begun to be absorbed by the patient's body;

[0082] FIGS. 64A-H shows a closure system and various embodiments for locking mechanism; FIGS. 64A-B illustrate an exterior view of the system and a cross-section of the exterior view along the lines B-B, respective; FIG. 64C illustrates a close-up of the cross-section of the proximal section of the system shown in FIG. 64b; FIG. 64D illustrates a close-up of the distal end of the device; FIGS. 64E-F are close-ups of cross-sections of the proximal end of the device;

[0083] FIGS. 65A-G shows a delivery capsule with a cut away in FIG. 65A, an exterior side view FIG. 65B, a cross-section along the lines C-C in FIG. 65C, a view down the distal barrel end in FIG. 65E, a cross-section along the lines F-F in FIG. 65F and a cross-section with a directional indication for pressure in FIG. 65G;

[0084] FIGS. 66A-D shows a proximal cross-section of the delivery system illustrating embodiments of mechanisms of engaging a part of a portion of the delivery system with another part;

[0085] FIGS. 67A-E shows a plug deployment system in use with a currently available introducer with cross-sections of the proximal end (FIG. 67D) and expanded views (FIG. 67C);

[0086] FIGS. 68A-B shows an exterior view of plug deployment system in use with another currently available introducer;

[0087] FIGS. 69A-B shows an exterior view of another plug deployment system in use with yet another currently available introducer;

[0088] FIGS 70A-G shows a plug delivery capsule from an exterior view, a longitudinal cross-section along the lines B-B of FIG. 70C, a view down the distal end (FIG. 70C), and the delivery capsule collet from an exterior view (FIG. 70D), cross-sectional view along the lines F-F before machining FIG. 70E and after machining FIG. 70F to create the fingers or legs, and a view down the proximal barrel (FIG. 70G);

[0089] FIGS. 71A-C shows a collet cartridge insert from an exterior view (FIG. 71A), a cross-sectional view along the lines B-B (FIG. 71B) and a view down the barrel from the proximal end (FIG. 71C);

[0090] FIGS. 72A-E shows a capsule configuration from a side perspective view (FIG. 72A), a longitudinal cross-sectional view along the lines B-B (FIG. 72B), a view down the barrel from the distal end (FIG. 72C), a side view (FIG. 72D), and a view down the barrel from the proximal end (FIG. 72E);

[0091] FIGS. 73A-E shows another capsule configuration in a perspective shadow view (FIG. 73A), a longitudinal cross-sectional view along the lines B-B (FIG. 73B), a view down distal end (FIG. 73C), a cross-sectional view in shadow (FIG. 73D), and a view down the proximal end (FIG. 73E);

[0092] FIGS. 74A-D shows a plunger grip from a perspective view (FIG. 74A), a cross-sectional side view along the lines B-B (FIG. 74B), a side view (FIG. 74C) and a view down the distal end (FIG. 74D);

[0093] FIGS 75 A-C shows another plunger grip configuration with the plunger grip in a proximal shadow view (FIG. 75A), a cross-sectional side view along the lines B-B (FIG. 75B) and a view down the distal end (FIG. 75C);

[0094] FIGS. 76A-B shows a tether line configuration;

[0095] FIGS. 77A-B shows another tether line configuration;

[0096] FIGS. 78A-E shows a plunger tip from a perspective view (FIG. 78A), a longitudinal cross-section along the lines B-B (FIG. 78B), a view from the proximal end (FIG. 78C), a view from the distal end (FIG. 78D), and a cross-sectional view of the plunger tip and plunger (FIG. 78E);

[0097] FIGS. 79A-J shows two plug configuration, the first configuration from a perspective view (FIG. 79A), a top view from a distal end (FIG. 79B), a bottom view from a proximal end (FIG. 79C), a side view (FIG. 79D), and a longitudinal cross-sectional view along the lines E-E (FIG. 79E), and the second configuration from a perspective view (FIG. 79F), a top view from a distal end (FIG. 79G), a bottom view from a proximal end (FIG. 79H), a side view (FIG. 79I), and a longitudinal cross-sectional view along the lines E-E (FIG. 79J);

[0098] FIGS. 80A-C shows plug and locking configurations in operation with a stem portion of the plug in removeable communication with the plate;

[0099] FIGS. 81A-N shows additional plug mating configurations employing wires, variably configured longitudinal apertures in the stem, hooks, clasps, perpendicular apertures through the stem;

[0100] FIGS. 82A-B shows releasable plug configurations which can be torn or separated along the stem;

[0101] FIGS. 83A-D shows tethered plug configurations which include a ball or radiopaque marker;

[0102] FIGS. 84A-D shows tethered plug configurations with a ball and socket connection;

[0103] FIGS. 85A-R shows plug stem variations having a wide variety of geometric shapes;

[0104] FIGS. 86A-E shows plug with petals design;

[0105] FIGS. 87A-B shows disc configurations for the face plate of the plugs;

[0106] FIGS. 88A-F shows alternative disc configurations for the face plate of the plugs;

[0107] FIGS. 89A-G shows disc configurations with ribs and nibs;

[0108] FIGS. 90A-E illustrates hemostatic plug capsule designs;

[0109] FIGS. 91A-I illustrates stem and capsule mating designs; and

[0110] FIGS. 92A-T illustrate the system component interactions and operations when deploying a vessel closure device using a system as disclosed.

DETAILED DESCRIPTION

[00111] The following description provides examples of certain embodiments for purposes of illustration. The inventions as claimed should not be limited to these examples. Moreover, although the examples are provided in the context of vessel closure, the invention also has broad application to other types of tissue closure. U.S. Patent No. **7,025,776** to Houser et al., the entirety of which is incorporated herein by reference, discloses a variety of additional vessel closure devices and methods with features that can be used in combination with or instead of features of the embodiments disclosed herein.

[00112] As will be appreciated by those skilled in the art, the components of the vessel closure systems described herein can be sized to accommodate an introducer sized from 6French to 22French, and any size therein. Ranges have been provided for purposes of illustration only and to facilitate a better understanding of the disclosure. Additional values, provided for illustration purposes only, are contained in Table 1.

TABLE 1

Component	System Size	Inner Diameter	Outer Diameter	Length	Additional Considerations
closure system	≤ 6F 16F 22F			0-50 mm > introducer length	OAL and typically dependent on introducer length
plunger grip	≤ 6F 16F 22F		2.0 - 35.0 mm 6 - 50 mm 7 - 75 mm	10 - 75 mm 15 - 75 mm 15 - 125 mm	ID typically a function of tube and capsule proximal end
deployment plunger	≤ 6F 16F 22F		0.5 - 3 mm 1 - 6 mm 2 - 8 mm	0-50 mm > introducer length	OAL and typically dependent on introducer length
plunger tube	≤ 6F 16F 22F	0.3 - 2.0 mm 0.3 - 5.5 mm 0.3 - 7.5 mm	0.5 - 3 mm 1 - 6 mm 2 - 8 mm	0-50 mm > introducer length	OAL and typically dependent on introducer length
plunger tip	≤ 6F 16F 22F		0.3 - 1.5 mm 0.3 - 4.5 mm 0.3 - 6.5 mm	1 - 10 mm 1 - 15 mm 1 - 25 mm	
delivery capsule collet	≤ 6F 16F	0.48 min 0.80 min	1.5 - 20 mm 1.5 - 35 mm	2 - 15 mm 4 - 35 mm	Nominally 0.02 mm; typically a smaller ID than the plunger tube OD

Component	System Size	Inner Diameter	Outer Diameter	Length	Additional Considerations
	22F	1.80 mm	2.0 - 75 mm	5 - 50 mm	
central lumen	≤ 6F 16F 22F				Per mfg specs, nominally the "French size" of the introducer i.e. 6F = 2mm
collet cartridge insert	≤ 6F 16F 22F	0.48 min 0.80 min 1.80 mm	2 - 20 mm 2 - 35 mm	2 - 25 mm 2 - 50 mm 3 - 75 mm	Nominally 0.5 mm larger ID than collet OD
capsule	≤ 6F 16F 22F	2 - 12 mm 3 - 15 mm 5 - 25 mm	3 - 35 mm 4 - 50 mm 6 - 75 mm	4 - 35 mm 4 - 75 mm 4 - 155 mm	
capsule exterior surface	≤ 6F 16F 22F	2 - 12 mm 3 - 15 mm 5 - 25 mm	3 - 35 mm 4 - 50 mm 6 - 75 mm	4 - 35 mm 4 - 75 mm 4 - 155 mm	
cartridge body	≤ 6F 16F 22F	2 - 12 mm 3 - 15 mm 5 - 25 mm	3 - 35 mm 4 - 50 mm 6 - 75 mm	4 - 35 mm 4 - 75 mm 4 - 155 mm	
detent	≤ 6F 16F 22F	6 - 35 mm 16 - 55 mm 22 - 75 mm		0.5 - 25 mm 0.5 - 55 mm 0.5 - 75 mm	ID typically not less than "French size" of system
tapered tip	≤ 6F 16F 22F				ID nominally equal to introducer lumen size OD tapers to fit introducer cap diameter
re-entrant nose	≤ 6F 16F 22F				length and OD are a function of particular dimensions of the introducer ID tapers nominally to introducer lumen ID
hemostatic valve (on capsule)	≤ 6F 16F 22F	0 - 7 mm 0 - 17 mm 0 - 23 mm	depends on mfg depends on mfg depends on mfg	depends on mfg depends on mfg depends on mfg	full closed to larger than introducer size, see mfg specs

Component	System Size	Inner Diameter	Outer Diameter	Length	Additional Considerations
side walls	≤ 6F	0.48 min	na/	2 - 25 mm	nominally equal to OD and length of collet cartridge insert
	16F	0.80 min	n/a	2 - 50 mm	
	22F	1.80 mm	n/a	3 - 75 mm	
base	≤ 6F 16F 22F				nominally equal to OD of collet cartridge insert

I. VESSEL CLOSURE SYSTEMS

[00113] Referring to **FIG. 1**, a vessel closure system **100** can generally include a vessel closure device such as clip **102** or plug and a deployment or advancement instrument **104**. The plugs or closure devices can also be referred to as sealing devices, implants, vessel access closure devices, arteriotomy closure device, vascular closure devices, and tissue closure devices. As depicted, clip **102** is loaded onto a distal end **105** of deployment instrument **104**. The deployment instrument **104** is slidably mounted to or advanced along and generally guided by a vascular introducer **108** or other tubular medical device such as a catheter which has been inserted into a blood vessel **18**. In certain embodiments, a narrow opening in the skin initially created for the insertion of the vascular introducer **108** can be expanded or enlarged by a guided slidable tissue cutter **106** to form a percutaneous opening **12** sufficiently large to easily permit passage of the deployment instrument **104** into the body.

[00114] The deployment instrument **104** can be guided by a tube section **110** of vascular introducer **108** through the percutaneous opening **12** until it reaches arteriotomy site **14**. The deployment instrument **104** is configured to deploy a vascular closure clip **102** to close the arteriotomy **14**. The deployment instrument **104** can then be withdrawn.

(a) Deployment Instrument

[00115] A variety of deployment instruments are depicted and described herein. Persons of skill in the art will appreciate that the modifications to the designs disclosed can be performed without departing from the scope of the disclosure.

[00116] Turning now to **FIG. 8** a more detailed view of the distal end **105** of a deployment instrument **104** from **FIG. 1** is illustrated, which is configured to receive clip **102** and generally maintain it in an open configuration until deployed. In the illustrated embodiment, the tines **126a**, **126b** are substantially parallel with a central axis of the inner tubular member **154**, and the distal ends **127a**, **127b** of the tines **126a**, **126b** are substantially aligned with the distal end **165** of the inner tubular member **154**. In other embodiments, the distal ends **127a**, **127b** of the tines **126a**, **126b** can extend slightly beyond the distal end **165** of the inner tubular member **154**. Alternatively, clip **102** can be located more proximally while the deployment instrument **104** is in its initial configuration

with the distal ends *127a*, *127b* of the tines *126a*, *126b* being proximally spaced from the distal end *165* of the inner tubular member *154*. As will be described in more detail below, the inner diameter of the base *120* of the clip *102* can be positioned close to or in contact with the outer diameter of the distal end *165* of the inner tubular member *154*, and the outer diameter of the base *120* of the clip *102* can be positioned close to or in contact with the inner diameter of the distal end *173* of the outer tubular member *156*. A radially inwardly directed restoring force exerted by the tines *126a*, *126b* in the open configuration increases the friction between the inner surfaces of the clip *102* and the outer surface of the inner tubular member *154*, generally preventing the clip *102* from readily sliding away from its position between the inner and outer tubular members *154*, *156*.

[00117] Distal end *173* of outer tubular member *156* can include an interior ledge or countersink *174* configured to receive and abut against the base *120* of clip *102*. As will be explained in more detail below, when the assembled deployment instrument *104* is advanced to the tissue closure site and the inner tubular member *154* is axially withdrawn in the proximal direction from the outer tubular member *156*, a distally directed reaction force is exerted by countersink *174* against the base *120* of the clip *102*, preventing the clip *102* from also moving in the proximal direction. When the distal end *165* of the inner tubular member *154* is moved in the proximal direction past the base *120* of the clip *102*, the contacting or adjacent relationship between the clip *102* and the inner and outer tubular members *154*, *156* is interrupted and the clip *102* is released from the deployment instrument *104*. In certain embodiments, the use of countersink *174* can permit the outer tubular member *156* to avoid contact with or otherwise to protect all or a portion of clip *102* during advancement prior to deployment. In other embodiments, countersink *174* can be omitted and the distal-most surface of outer tubular member *156* can be configured to contact base *120* to force off or otherwise permit removal of the clip *102* from the deployment instrument *104*.

[00118] FIGS. 9 - 11 are illustrations of an example of the inner tubular member *154* separated from the outer tubular member *156* before the configuration illustrated in FIGS. 7 - 8 is assembled. Inner tubular member *154* defines an inner lumen *166* which is configured to receive a tubular medical device such as a vascular introducer *108*. Elongate slot *162* allows at least a portion of the deployment instrument *104* to be tilted away from and axially separated from the proximal portion of the vascular introducer *108* by a medical professional without detaching the instrument *104* entirely from the tube section *110*. See, e.g., FIG. 1. This configuration permits the medical professional to position the deployment instrument *104* out of the way while the desired interventional or diagnostic procedure is performed. In the illustrated embodiment, axial grooves *160* run along the length of the outer surface of inner tubular member *154* and are configured to mate with axial protrusions *168* (see FIG. 13) formed on an inner surface of outer tubular member *156*. This mating configuration can prevent inner tubular member *154* from rotating relative to outer tubular member *156* and can help to align elongate slot *162* of inner tubular member *154* and elongate slot *170* of outer tubular member *156*.

[00119] The proximal end of inner tubular member **154** can include a handle **164** which may be gripped by the medical professional, for example, to withdraw inner tubular member **154** during deployment. The handle is generally configured for handling by a user and for enabling a user to achieve motion or operation of a distal end in response to the user's control of the handle. As illustrated, handle **164** can be generally circular with a flattened lower end to facilitate delatching of the stop mechanism during complete deployment as explained below. Other shapes and configurations can also be used. The upper portion of handle **164** includes a cut-out portion **350** which is aligned with and merges with elongate slot **162**. Lower portion of handle **164** includes a recess **169** to accommodate tab **172** of the outer tubular member **156**. The distal end of handle **164** includes distal faces **354** which can be substantially flat. Faces **354** are configured to abut the proximal-most edge of the tube section of outer tubular member **156** to prevent over-insertion of inner tubular member **154** into outer tubular member **156**. Proximal faces **167** of handle **164** can be substantially flat and are configured to abut stops **175** on tab **172** during partial deployment. Lower portion of the handle **164** can include angled surfaces **352**.

[00120] FIGS. 12 - 16 illustrate an example of an outer tubular member **156** separated from the inner tubular member **154** before the configuration illustrated in FIGS. 7 - 8 is assembled. Outer tubular member **156** defines an inner lumen **171** configured to receive inner tubular member **154**. An elongate slot **170** runs along a length of outer tubular member **156** and provides access to the interior of inner lumen **171**. Elongate slot **170** of outer tubular member **156** is configured to align with elongate slot **162** of inner tubular member **154**. Distal end **173** of outer tubular member **156** can include one or more slots **176** to provide side access to clip **102** while deployment instrument **104** is in its initial configuration.

[00121] A securing or movement-limiting structure such as tab **172** extends from a proximal end of outer tubular member **156**. Tab **172** includes stop surfaces **175** configured to abut the proximal faces **167** on handle **164** during partial deployment as explained in more detail below. Tab **172** can include two tapered arms **181** surrounding a window portion **177** to facilitate assembly of the deployment instrument **104** as explained further below. Tab **172** can also include a recessed, weakened, or hinge portion **186** to facilitate bending. In certain embodiments, tab **172** can be relatively rigid with the exception of weakened portion **186**. In certain embodiments, bending of tab **172** can be configured to occur substantially at weakened portion **186**. In certain embodiments, tab **172** can be relatively long. For example, tab **172** can be at least about 20 mm. A long tab **172** can facilitate handling by the medical professional. A long tab **172** can also increase the leverage applied by the medical professional to effectuate bending.

[00122] The deployment instrument can include a pressure sensitive structure which can comprise, in one example, pressure tapers **178** formed on an outer surface of outer tubular member **156** and flexible tabs **188** of pressure element **158**. Outer tubular member **156** can also include a pressure sensitive structure such as an axial protrusion **185** extending from a proximally-located outer

surface. As illustrated, axial protrusion **185** can be located in a substantially diametrically opposite position from elongate slot **170**, although other configurations are possible. A ramp or one-way tapered lock **184** extends from axial protrusion **185**. A stop, **182** which can be generally annular in shape, extends from an outer surface of outer tubular member **156**. The outer surface of outer tubular member **156** also includes pressure tapers **178**. Pressure tapers **178** can terminate in substantially flat surfaces **180**. Surfaces **180** can be adjacent to and in contact with annular stop **182**. As illustrated in **FIG. 16**, outer tubular member **156** can include two pressure tapers **178** located in a substantially diametrically opposite position from one another on the generally circular outer tubular member **156**. Also as illustrated, pressure tapers **178** can be positioned at approximately equal circumferential distances from elongate slot **170** and axial protrusion **185**. Other configurations are possible.

[00123] **FIG. 17** provides a detailed illustration of a pressure element **158**, which in some embodiments can be a generally ring-shaped element configured to be received on an outer surface of outer tubular member **156**. In certain embodiments, as illustrated, pressure element **158** can be a separate element from outer tubular member **156**. In other embodiments, pressure element **158** can be integrally formed with outer tubular member **156**. As described in more detail below, pressure element **158** can be used to confirm that the medical professional is applying generally sufficient but not excessive pressure to safely begin deployment of the clip **102**. Pressure element **158** can include a cut-out portion **105** aligned with elongate slots **162**, **170** of the inner and outer tubular members **156**, **154**. Recess **190** can be configured to mate with axial protrusion **185** of outer tubular member **156** to keep the pressure element **158** properly aligned. An inner surface of pressure element **158** includes one or more flexible tabs **188**. Flexible tabs **188** are configured to align with, and be advanced over, pressure tapers **178** of outer tubular member **156**.

[00124] During assembly of deployment instrument **104**, pressure element **158** can be advanced over the proximal end of outer tubular member **156** and over one-way tapered lock **184**. Recessed portion **190** and/or lock **184** can be configured to flex or temporarily deform sufficiently to accommodate this procedure. Alternatively, lock **184** or other locking means can be formed on, or secured to, outer tubular member **156** after positioning of pressure element **158**. Tapered lock **184** prevents pressure element **158** from moving too far in a proximal direction with respect to outer tubular member **156**. Inner tubular member **154** can then be inserted into the inner lumen **171** of outer tubular member **156** from the outer tubular member's proximal end. As the inner tubular member **154** is inserted into outer tubular member **156**, inner surfaces **183** (see **FIG. 11**) of the lower portion of handle **164** adjacent to recess **169** begin to come into contact with tapered arms **181** of tab **172**. The continued advancement of inner tubular member **154** distally causes surfaces **183** to apply an inwardly-directed force to arms **181**. Window **177** permits arms **181** to resiliently flex inwardly until handle **164** has been advanced distally of stops **175**. Inner tubular member **154** can then be advanced further until distal faces of handle **354** contact the proximal-most edge of the tube section of outer tubular member **156**.

[00125] In another example of a deployment instrument forming part of a closure system or kit, a vessel closure system **600** is shown in **FIGS. 64A-E**. The vessel closure system **600** is adapted and configured to further provide three sections in communication with each other: a plunger **610**, a capsule **630** and an introducer **650**. The plunger **610** further includes a deployment plunger **612**, and a guide and seal assembly **614**. The deployment plunger **612** is a rod, such as a cylindrical or substantially cylindrical rod, configured to be housed within an aperture formed in the guide and seal assembly **614**. The plunger **612** is configured such that it is capable of a movement in at least one direction along a central axis **A**. The plunger can terminate in a plunger tip **620** which may, in some configurations, be removeable.

[00126] The closure device capsule **630** engages the plunger at a proximal end **70** and an introducer at a distal end **80**. The capsule **630** includes a deployment cartridge body **632**, and a compressible section **634**. In some configurations, the capsule **630** is adapted and configured to snap fit within an least a portion of the introducer cap.

[00127] The introducer **650** further is adapted to receives a part of the capsule **630**. A re-entrant nose **646** of the capsule **630** is positioned to align within an aperture of an introducer bore to minimize cocking of the closure device **670** during deployment. A central aperture **656** is provided through which the clip, plug or closure device **670** contained in the capsule **630** can travel during deployment. In this configuration a hemostasis valve **652** is provided on the introducer which maintains the closure device **670** in position within the capsule during delivery.

[00128] Once the introducer, capsule **630** and plunger have been assembled, the components will not separate during use. This feature prevents inadvertent disassembly once the clip, plug or closure device **670** is deployed in the vessel. For example, if the entire deployment assembly and introducer are not withdrawn as a single unit, the clip, plug or closure device **670** could be stripped off the plunger. This could result in the clip, plug or closure device **670** being deployed in the vessel without properly seating at the arteriotomy site. As shown in **FIG. 64C**, the capsule **630** snap fits over the introducer **650** at its proximal end and the capsule **630** snap fits within the introducer at its proximal end. Additional flanges **675** can be provided on the distal end **80** of the cap **616** or arms extending from the plunger **610** which fit within a detent **636** provided on the exterior surface **631** of the capsule **630** when the plunger **610** is fully positioned on the capsule **630**.

[00129] Each component can be configured to provide a one-way snap feature, as shown in more detail in **FIGS. 64E-H**. In **FIGS. 64E-F** the plunger grip **610** has been snapped onto the capsule **630** and the system is provided with internal locking feature shown are characterized in that the proximal end **70** of the introducer **650** has a cap **656** or arms that extend radially from the axis **A** and then curve and extend along an axis parallel to, or substantially parallel, the axis **A** to engage and mate with an exterior surface of the distal end **80** of the capsule **630**. The capsule **630** features a tapered tip **636** at its distal end **80** which can further be provided with an undercut that is configured to fit within an interior recess of the introducer.

[00130] An example of an external lock feature is shown in more detail in **FIG. 64G-H**. As with the previous illustration, the plunger grip **610** has been snapped onto the capsule **630**. Where external locking features are provided, the proximal end of the introducer **650** has a flange into which the capsule **630** fits and which further includes fingers **660** that fit within a groove **642** formed on an exterior surface **631** of the capsule **630**.

[00131] Tissue clips and plugs, described in more detail below, can be deployed using the system by providing the clip, plug or closure device **670** within a capsule **630** as shown, for example, in **FIGS. 65A-G**. The capsule **630** has a tubular exterior surface **631** with a first diameter at a proximal end **70** and a smaller diameter at a distal end **80**. As will be appreciated by those skilled in the art, the tubular capsule can take a variety of cross-sectional configurations including circular, oval, polygon, D shape, etc. For purposes of illustration, dimensions are provided for a circular cross-sectional shape in order to provide a context for the sizes and volumes involved. Additionally, the sizes may change as a result of the size of the introducers used. Persons of skill in the art will appreciate that introducers can vary from 8 French to 20 French (and values therein). Thus dimensions would likely be proportional to the French size of the introducer. Thus, for example, a typical diameter of the first diameter could be from about 4mm to 25mm, more preferably about 8mm, or any value therein to about 100th of a mm. Typical diameter of the second diameter range from about 1mm to about 3mm, more preferably about 2mm, or any value therein to about 100th of a mm. The overall length of the capsule ranges from about 12mm to about 50mm or up to 100mm, more preferably about 35mm, or any value therein to about the 100th of a mm. The capsule **630** includes a clear tubular section **640** approximately mid-length through the presence of the clip, plug or closure device can be observed through which fluid flow can be observed as the clip, plug or closure device **670** contained within the capsule **630** is deployed. As shown in the cross-section along the lengthwise axis **A**, the capsule body **632** includes a proximal end **70**, a distal end **80** and a mid-section. An aperture **638**, **638'** is provided in both the proximal body section and the distal body section. A valve **648** can be provided as shown. The closure device **670** is positioned within the interior of the capsule **630** at a position where the capsule body **632** is configured such that a user can see the clip, plug or closure device **670** within the capsule body **632**. The re-entrant nose **646** the plunger grip **610** has been snapped onto the capsule **630** and the system is provided with internal locking feature shown are characterized in that the proximal end **70** of the introducer **650** can be tapered along its length such that its diameter at its proximal end **70** and its distal end **80** are not substantially the same. Additionally, the elongated aperture **638'** within the nose **646** can also change in diameter along its length. The tapered end tip **646** at the distal end is configured to dilate the hemostatic valve **652** within the introducer **650** such that the valve can at least temporarily be opened, allowing the clip, plug or closure device **670** to be advanced through the valve without potentially damaging the clip, plug or closure device **670**, or dislodging the clip, plug, closure device from the distal end of the plunger **612**. By altering the cross-section of the elongated aperture within the nose **654** through which the clip, plug or closure device

670 travels during deployment, the clip, plug or closure device **670** can thereby be manipulated to achieve a reduced profile as the clip, plug or closure device **670** is advanced forward. The see-through chamber allows a fluid, such as blood, to flow, confirming that the proper location of the introducer sheath has been achieved. The capsule **630** may further be configured to include a guide for the insertion of a tool to contact and advance the clip, plug or closure device **670**. In the configuration depicted here, the legs of the clip, plug or closure device **670** are positioned to sit on an edge of the bore on the distal section.

[00132] Turning to **FIGS. 66A-D**, additional configurations of capsule **630** and plunger assemblies configured to present disassembly are provided. The configurations illustrated are adapted and configured to prevent inadvertent separation of a deployment assembly from an introducer once the clip, plug or closure device is fully extended into the vessel. Some configurations can be adapted and configured to enable a deliberate override by a physician, if necessary. As with the previous configuration, the vessel closure system **600** is adapted and configured to further provide three sections in communication with each other: a plunger **610**, a capsule **630** and an introducer **650**. The plunger **610** further includes a deployment plunger **612**, and a guide and seal assembly **614**. The deployment plunger **612** is a rod, such as a cylindrical or substantially cylindrical rod, configured to be housed within an aperture formed in the guide and seal assembly **614**. The plunger **612** is configured such that it is capable of a movement along a central axis **A** in a first direction and a second direction. The plunger **610** fits over and snaps onto the proximal end **70** of the capsule **630**. Alternatively, an internal lock feature can be provided wherein a male section of the plunger **610** slides into a mating female recess in the proximal end of the capsule **630** and locks in place as shown in **FIG. 66D**. In some configurations, a separate seal is not provided. Rather hemostasis is achieved by the closure device itself as it seals within the capsule. Thus, provision of a separate seal in any of these configurations is optional.

[00133] An additional aspect of the deployment system is that it can be used with a variety of commercially available introducer systems, such as those available from Cordis (**FIGS. 67** and **69**), and St. Jude Medical (**FIG. 68**). As shown in **FIGS. 67A-E, 68A-B** and **69A-B** each of the systems **600** includes a plunger **610**, a delivery capsule **630** in combination with a plunger **612**, a plunger tube **618**, a collet cartridge insert **623**, a delivery cap collet **621**, a bioabsorbable closure device **670**, a tether **662**, a tether drag element **664**. A plunger tip **613** can also be provided as shown in **FIGS. 68** and **69**. The introducers depicted herein typically range from about 120 mm to about 170 mm in length, or any length therein to the 100th of a mm. The plunger tubes typically are from 15mm to 50mm longer than the length of the commercially available introducers for which they are configured to mate, e.g., a deployment system configured to work with a 120mm introducer would have a plunger from about 135mm to about 170 mm in length, or any length therein and have an inner diameter (for 6 French introducers) of from about 1.0 mm to about 2.4mm. The system may be configured to enable simple

and easy, non-surgical closure of hemodialysis vascular access sites (including, for example, fistulae and/or grafts) that will no longer be used because of occlusion or other reason.

[00134] A suitable configuration for the delivery capsule **630** is shown in further detail in **FIGS. 70A-F**. The delivery capsule **630** has an outer diameter from about 4mm to 12mm on its distal end **80** and from about 3mm to about 11mm on its proximal end **70** or any size therein to about the 100th of a mm. Where the devices are volume manufactured, the distal tip and the capsule can be configured as a single component. The proximal end **70** has an aperture into which the guide assembly fits (as shown above in **FIG. 64**) and an aperture therethrough through which the deployment plunger can travel as it pushes the closure device to the delivery site. The distal end **80** has a smaller outer diameter to facilitate engaging the introducer (which fits around the exterior surface **631** of the capsule **630** until it reaches the wall. From **FIG. 70C**, which is a view down the barrel of the capsule **630** from the distal end **80**, the central aperture **644** can be seen and the bottom face **649'** formed from the counterbore which is characterized by side walls and a base surface. The delivery capsule collet **621** shown in **FIGS. 70D-E** has a first diameter ranges from about 3mm to about 4mm, or any size therein to about the 100th of a mm and the second diameter ranges from about 2.7mm to about 3.0mm, or any size therein to about the 100th of a mm. An inner diameter of the aperture ranges from about 1.5mm to about 1.9mm at its proximal end and about 1.3mm to about 1.7mm at its distal end, or any size therein to about the 100th of a mm. From **FIG. 70F**, the exterior taper of the outer surface of the collet **621** from a proximal end (wider) to a distal end (narrower) has a value of from about 0.4° to about 8°, or more preferably about 5°, or any value therein.

[00135] The collet cartridge insert **623** is shown in **FIGS. 71A-C**. The collet cartridge insert is a slotted cylindrical clamp that is inserted into the tapered interior of the delivery capsule to hold the capsule. The collet cartridge insert has a cylindrical profile with an aperture therethrough along an axis **A**. The aperture has a tapered dimension as illustrated in **FIG. 71B**. **FIG. 71C** is an end-view of the collet cartridge insert from a distal end **80**. The collet typically has a first outer diameter at a proximal end **70** and a second outer diameter at a distal end **80**. The first diameter ranges from about 4.4mm to about 5.0mm, or any size therein to about the 100th of a mm and the second diameter ranges from about 4.7mm to about 5.0mm, or any size therein to about the 100th of a mm. An inner diameter of the aperture ranges from about 3.3mm to about 3.9mm at its proximal end and about 1.5mm to about 1.8mm at its distal end, or any size therein to about the 100th of a mm. The exterior taper of the interior aperture of the collet cartridge insert from a proximal end (wider) to a distal end (narrower) has a value of from about 0.4° to about 8°, or more preferably about 5°, or any value therein.

[00136] The delivery capsule **630** distal tip **654** is shown in more detail in **FIGS. 72A-E**. The delivery capsule **630** distal tip **654** has a stem with an aperture **636** therethrough. The stems can also be referred to as a core, column, vertical section, mid-section, center, post or shaft without departing from the scope of the disclosure. The aperture ranges in diameter from about 3.8mm to about 4.2mm at its proximal end, more preferably about 4.02 mm, or any value therein to about the 100th of a mm

and then tapers down to a diameter of about 2.4 mm to about 2.6 mm, or more preferably about 2.51 mm, or any value therein to about the 100th of a mm along its tapered tip **638**. The length of the distal tip ranges from about 4.0mm to about 25.0mm, more preferably about 18mm, or any length therein to about 100th of a mm. In some configurations lengths greater than 35mm may be appropriate. The outer diameter of the delivery capsule distal tip is about 3.0mm to about 4.0mm, more preferably 3.2mm, or any value therein to about the 100th of a mm. Outer diameters can be, in some instances up to 35mm or more. The outer diameter of the widest section is about from 4.5mm to about 10.0mm, more preferably about 5.7mm, or any value therein to about 100th of a mm. In some configurations, the widest section can be up to 35mm or greater. The proximal section has an outer diameter of about 4.5mm to about 10.0mm, more preferably about 5.7mm, or any value therein to about the 100th of a mm. An internal tapered section **634** is located near a proximal end **70**. The distal tip has an intermediate body with a radius larger than the radius of the neck. A proximal section is provided which has a radius larger than the distal tip but less than the intermediate body. The proximal transparent module section of the delivery capsule **630** is shown in more detail in **FIGS. 73A-E**. The transparent section has body with an aperture **637** therethrough. The body is configured to provide an outer diameter at its proximal end **70** sized to engage the distal end **80** of the plunger and an outer diameter at its distal end **80** sized to engage the proximal end **70** of the delivery mechanism. As illustrated, the outer diameter of the proximal end **70** is larger than the diameter of an intermediate section, but smaller than a diameter of the distal section. The aperture at the distal end **80** is large enough to enable the proximal end **70** of the delivery mechanism to fit within a recess and abut against a distally facing surface. The proximal end **70** of the aperture has a diameter that flares as it reaches the proximal end **70** of the module.

[00137] The capsule contains the sealing element or vessel closure device and protects the device from damage during the delivery process. As a result of the configuration of the capsule, the capsule also initiates reduction of the cross-sectional diameter of the vessel closure device prior to the vessel closure device entering the introducer. The capsule achieves a reduction in the cross-sectional diameter of the vessel closure device by, for example, deflecting a radially extending section of the vessel closure device. The capsule also facilitates in confirming that the introducer sheath is positioned within the target vessel, by the presence of blood viewable in the capsule.

[00138] The plunger grip **610** is shown in **FIGS. 74A-D**. The plunger grip **610** is configured to provide a variable external surface facilitating engagement by a user. The proximal end **70** has a knob-like shape which tapers into a narrower neck before widening at its distal end **80**. A central lumen **622** is provided along an axis **a**, through a portion of its length, terminating prior to the proximal end **70**. A perpendicular aperture can be provided near the distal end **80** which is in communication with the central lumen. The perpendicular aperture can, for example, be a threaded hole for use with a set screw to allow adjustment of the overall length of the plunger. The length of the plunger grip is about 12mm to about 45mm, or more preferably 25 mm, or any value therein to the

100th of a mm. The outer diameter of the plunger grip ranges from about 3.0mm to about 12mm along its length, more preferably about 10mm at its widest section and about 6mm at its narrowest section, or any value therein to about the 100th of a mm. The concave central portion of the plunger, particularly has varying outer diameter along its length over a range of from about 5mm of the length to about 20 mm of the length, or more preferably 7 mm to about 15 mm, or any value therein to about the 100th of a mm. Although this feature is optional, it improves the physician's grasp on the proximal end. The central lumen is for engagement with the plunger rod or tube.

[00139] An alternate embodiment of a plunger grip is shown in **FIGS. 75A-C**. As depicted the plunger grip **610** does not have a concave section along its length. The plunger grip has a central lumen **622** having a first inner diameter and a second inner diameter, and a length of about 10mm to about 35mm, more preferably about 16mm, or any value therein to about the 100th of a mm. The first inner diameter of the lumen is from about 6.3mm to about 7.7 mm, more preferably about 7 mm, while the outer diameter of the plunger grip is from about 7.6mm to about 8.9mm, more preferably about 8mm, or any value therein to about the 100th of a mm. The second inner diameter is from about 1.2mm to about 1.8mm, more preferably 1.6mm, or any value therebetween to about the 100th of a mm. The length of the lumen of the first diameter section ranges from about 5.0mm to about 7.6mm, more preferably about 6.4mm, or any value therein to about the 100th of a mm, while the length of the lumen of the second diameter section ranges from about 7.6mm to about 11.4mm, more preferably about 9.4mm, or any value therein to about the 100th of a mm.

[00140] In some configurations of the system, tether lines **672** can be employed. Tethers can also be referred to as leashes, temporary or removeable plug attachment mechanisms, suture lines, threads, wires, lines, containment members, containment elements, safety elements and capture elements without departing from the scope of the disclosure. Suitable tether line configurations are shown in **FIGS. 76A-B** and **77A-B**. The tether line **672** can be a continuous loop as shown in **FIG. 76A** or can be a wire forming a tether **674** as shown in **FIGS. 81A-D**. In some configurations, such as those depicted in **FIGS. 68** and **69**, a plunger tip **662** is employed without a tether line. A suitable configuration of a plunger tip is illustrated in **FIGS. 78A-E**. The plunger tip **662** has a round distal **80** tip and a tapered proximal **70** end adapted to snap fit within a suitable mating recess **676** as shown in **FIG. 79E** in the proximal end of the vascular closure. **FIGS. 68, 69** and **78E** shows the plunger tip within the plunger stem. The overall length of the plunger tip is, for example, from about 7.6mm to about 11.4mm, more preferably about 9.5mm, or any length therein to about the 100th of a mm. The proximal end has a trapezoidal cross-section **664** with a first width of about 1.02mm to about 1.27mm, more preferably 1.14mm or any diameter therein to about the 100th mm. Over a length of about 0.76mm to about 1.02mm, more preferably about 0.89mm, the trapezoidal cross-section widens to a diameter of about 1.02mm to about 1.27mm, more preferably 1.14mm, or any diameter therein to about the 100th mm. An intermediate narrowed neck section **666** follows having a diameter similar to the proximal end of the trapezoidal section and a length of about 0.76 mm to about 1.02mm, more

preferably about 0.89mm. The main body **668** of the plunger tip has a diameter of about 1.77mm to about 2.29mm, more preferably about 1.98mm, or any diameter therein to about 100th of a mm. From the view looking at the plug from a proximal end shown in **FIG. 78C**, the three varying diameters of the proximal end of the trapezoidal cross-section, the wider diameter of the trapezoidal section and the main body are visible. The diameter of the intermediate narrowed neck is not visible. After the main body **668**, a stem section **665** narrows from a proximal end towards a distal end along a length of from about 3.05mm to about 4.32mm, more preferably about 4.04mm, or any value therein to about the 100th of a mm. The stem section **665** ends distally with the formation of a bulbous end **667**. The bulbous end has a diameter of about 1.02mm to about 1.17mm, more preferably about 1.14mm, or any length therein to about the 100th of a mm. As viewed from the distal end, shown in **FIG. 78D**, the diameter of the bulbous end is visible and the main body. As will be appreciated from reviewing **FIG. 78E**, the plunger fits within an aperture in the distal end of the plunger stem **618**, which is connected to the handle at its proximal end.

(b) Tissue Clips, Plugs and Closure Devices

[00141] Tissue clips, plugs and closure devices disclosed herein are disclosed in the context of delivery into a mammalian body for purposes of closing, for example, an artery. However, as will be appreciated by those skilled in the art, other applications are possible. For example, the clips, plugs and closure devices could be sized such that they do not require delivery by a delivery system but rather are delivered in the field in the context of a trauma - such as a knife wound or gunshot wound - as an alternative to compression to stop bleeding. A variety of elements can be used in conjunction with the closure devices either on an exterior surface or an interior surface including, but not limited to, edges, ridges, flanges, wings, petals, radially extending members, and horizontal protrusion.

[00142] **FIG. 2** is a perspective view of an embodiment of a clip **102** in a pre-deployed or open configuration. Clip **102** can include a base portion **120**. Base portion **120** can be generally or completely annular, forming a partial or complete circle. In some embodiments, a base portion **120** with a continuous or substantially continuous circle along its upper edge as illustrated can provide increased strength and resistance to contortion or bending in either or both of the open and closed configurations. A generally circular base portion **120** can allow the tines **126a-b** to move or bend during the transition between the open and closed configurations while generally resisting a substantial change in shape or orientation of the base portion **120**. The height **135** of the base portion **120** can be selected to achieve a desired amount of stiffness or flexibility.

[00143] Fingers **122** and **124** can be configurable to extend from base portion **120** and support a plurality of tissue-engaging elements such as tines **126a-b**. In some embodiments, as illustrated, the fingers **122** and **124** can be positioned in a substantially opposing arrangement, for example wherein finger **122** is positioned in a substantially diametrically opposite location on the generally circular base **120** from finger **124**. As explained below, many other positions and configurations can be used.

[00144] In the illustrated example of FIG. 2, each finger 122, 124 includes three tines: one central tine 126a and two outer tines 126b. The outer tines 126b can be substantially the same length 132 from the respective tips 127b to the respective junctures with the forward surface 134 of each finger 122, 124. In some embodiments, the forward surface 134 can be substantially perpendicular to the tines 126a, 126b and substantially parallel with the plane of the base 120 in the open configuration. Surfaces 134 can generally act as substantially blunt stops to prevent over-insertion of clip 102 into the vessel wall 16. In some embodiments, the length 133 of the central tines 126a can be slightly greater than the length 132 of the outer tines 126b. This length differential can assist in producing an increased leverage and an increased force along a central line generally bisecting the base 120 between the two opposing central tines 126a to help pull generally opposing sides of a tissue slit opening together.

[00145] In some embodiments, the lengths 132, 133 can be selected so that the tines 126a, 126b pierce but do not completely penetrate through a vessel wall 16 of average thickness into the interior region of the vessel 18. For example, the length 132 may be greater than or equal to about 1 mm, and/or the length 132 may be less than or equal to about 4 mm, and the length 133 may be greater than or equal to about 1 mm, and/or the length 133 may be less than or equal to about 5 mm. In some embodiments, the length 132 is about 3 mm, and the length 133 is about 3 mm. In other embodiments, the tines 126a, 126b can be configured to penetrate the vessel wall, but generally not long enough to contact or penetrate the vessel wall 17 on the opposite side of the vessel 18. The lengths of the tines 126a, 126b are generally greater than the height 135 of the base portion 120. In the illustrated embodiment, fingers 122 and 124 are generally symmetrical about a central axis. In other embodiments, the fingers 122, 124 can be asymmetrical or include a different number or configuration of tissue-engaging elements.

[00146] Fingers 122, 124 can include one or more bend-facilitating regions 125, such as narrowed regions, indentations, articulating joints, or window portions as illustrated. The size, shape, and placement of the bend-facilitating regions 125 can be adjusted to assist in achieving a desired amount of closure force for the clip 102. As illustrated, the contours of the bend-facilitating regions 125 can be generally smooth to avoid additional trauma to the vessel wall. In some embodiments, an upper edge 129 of a bend-facilitating region 125 can be positioned in general alignment with a lower edge 131 of the base portion 120 to maintain a desired height 135 of the base portion 120. As illustrated, the width of the bend-facilitating region can be smaller than the height 135 of the base portion 120.

[00147] FIG. 3 shows a perspective view of clip 102 in a closed or deployed configuration. Clip 102 is preferably biased into a closed configuration. As shown in FIGS. 1 and 2, clip 102 can be temporarily maintained in an open or pre-deployed state by deployment instrument 104 until it is deployed and returns to substantially the same configuration illustrated in FIG. 3. Clip 102 can be configured to automatically close upon deployment to close the arteriotomy. In certain embodiments,

the closing of clip **102** can be accomplished substantially via changes in flexion regions **400**. In some embodiments, the dimensions, shape, and/or orientation of other portions of clip **102** can remain substantially unchanged between the pre-deployed and deployed states.

[00148] FIG. 4 is a side view of clip **102** in an open configuration. The respective heights **135**, **136**, **401**, of the base portion **120**, the support portion **141**, and the bend-facilitating region **125**, can have many different values, depending on the particular application of the clip **102** and other design preferences. Moreover, these heights **135**, **136**, **401** can be constant or can vary in some embodiments. By way of example, the height **135** of the base portion **120** may be greater than or equal to about 0.5 mm and/or may be less than or equal to about 2 mm; the height **136** of the support portion **141** may be greater than or equal to about 0.5 mm and/or may be less than or equal to about 4 mm; and the height **401** of the bend-facilitating region **125** may be greater than or equal to about 0.2 mm and/or may be less than or equal to about 2 mm or any size therein to about the 100th of a mm. In some embodiments, the height **135** of the base portion **120** is about 0.5 mm, 0.6 mm, 0.7 mm, 0.8 mm, 0.9 mm, 1.0 mm, 1.1 mm, 1.2 mm, 1.3 mm, 1.4 mm, 1.5 mm, 1.6 mm, 1.7 mm, 1.8 mm, 1.9 mm or 2.0 mm. In some embodiments, the height **136** of the support portion **141** is about 0.5 mm, 0.6 mm, 0.7 mm, 0.8 mm, 0.9 mm, 1.0 mm, 1.1 mm, 1.2 mm, 1.3 mm, 1.4 mm, 1.5 mm, 1.6 mm, 1.7 mm, 1.8 mm, 1.9 mm, 2.0 mm, 2.1 mm, 2.2 mm, 2.3 mm, 2.4 mm, 2.5 mm, 2.6 mm, 2.7 mm, 2.8 mm, 2.9 mm, 3.0 mm, 3.1 mm, 3.2 mm, 3.3 mm, 3.4 mm, 3.5 mm, 3.6 mm, 3.7 mm, 3.8 mm, 3.9 mm, or 4.0 mm or any size therein to about the 100th of a mm. In some embodiments, the height **401** of the bend-facilitating region **125** is about 0.2 mm, 0.3 mm, 0.4 mm, 0.5 mm, 0.6 mm, 0.7 mm, 0.8 mm, 0.9 mm, 1.0 mm, 1.1 mm, 1.2 mm, 1.3 mm, 1.4 mm, 1.5 mm, 1.6 mm, 1.7 mm, 1.8 mm, 1.9 mm or 2.0 mm or any size therein to about a 100th of a mm. In some embodiments, the height **135** is about 1 mm, the height **136** is about 2 mm, and the height **401** is about 0.8 mm. Other suitable heights can also be used.

[00149] As illustrated in FIGS. 2-4, the height **136** of the support portions **141** of fingers **122** and **124** can be less than the length **133** of central tines **126a** (for example, less than about 80%). This can permit the base portion **120** of the clip **102** to be positioned relatively close to the outer surface of the vessel wall **16** when the clip **102** is attached. In some embodiments, the support portions **141** can have different sizes or may be eliminated (e.g., with the tines **126a,b** attaching directly to the base portion **120**). In other embodiments, height **136** can be approximately equal to or greater than the length **133** of central tines **126a**. The support portions **141** can include smoothly contoured sides **143**, as illustrated, to diminish the likelihood that the support portions **141** will pierce the vessel wall **16** and/or cause trauma to the vessel wall **16**. In the illustrated embodiment, the outer surface of the support portions **141** is curved (e.g., similar in curvature to the outer surface of the base portion **120**). In some embodiments, the outer surface of the support portions **141** can be flat or can be shaped in a way different from the outer surface of the base portion **120**.

[00150] FIG. 5 is a side-view of clip **102** in a closed configuration. In a deployed state, clip **102** can define an angle **2 130** between a central axial line or an edge in fingers **122, 124** and a peripheral surface or an edge **131** of base **120**. Angle **2 130** can be selected to assist in determining the applied closure force and to facilitate removal of clip **102** in embodiments using temporary closure, as explained further below. Angle **2 130** also can be selected to assist in determining the overall depth of penetration by the tines **126a, 127b** into the vessel wall **16**. For example, a smaller angle will generally produce a more shallow penetration and a larger angle will generally produce a deeper penetration. In some embodiments, Angle **2 130** can be greater than or equal to about 30° and/or less than or equal to about 70°. In some embodiments, Angle **2 130** can be about 30°, 35°, 40°, 45°, 50°, 55°, 60°, 65°, or 70° or any angle value therein to a 100th of a degree. In a particular example, Angle **2 130** can be about 50°. Other appropriate angles can also be used. In some embodiments, as illustrated, the flexion regions **400** can bend while other structures remain substantially unchanging or intact.

[00151] FIG. 6 is a bottom view of clip **102** in a closed configuration. As illustrated, opposed pairs of tines **126a, 126b** can be configured to contact one another or to draw very close to each other (e.g., within a distance equivalent to about the thickness **137** of each tine **126a, 126b**) in the closed configuration. In other embodiments, the tines **126a, 126b** need not be configured to move very close to each other in the closed configuration. In some embodiments, base portion **120** has a side thickness **138** which can be greater than or equal to about 0.1 mm and/or less than or equal to about 0.5 mm. In some embodiments, base portion **120** has a side thickness **138** of about 0.1 mm, 0.2 mm, 0.3 mm, 0.4 mm or 0.5 mm or any size therein to about the 100th of a mm. In some embodiments, base portion **120** has a side thickness **138** of about 0.2 mm. As illustrated, in some embodiments, all portions of the clip **102** can share approximately the same thickness. The thickness can also vary between different portions of the clip **102** in appropriate circumstances. For example, referring to FIG. 4, tines **126a-b** can have a thickness **137** which can be less than thickness **138** of the base portion **120** to facilitate penetration of the vessel wall **16**.

[00152] Base portion **120** can define an outer diameter and an inner diameter. For example, the outer diameter can be greater than or equal to about 3 mm and/or less than or equal to about 7 mm, and the inner diameter can be greater than or equal to about 2.5 mm and/or less than or equal to about 6.5 mm. In some embodiments, the outer diameter is about 3.0 mm, 3.5 mm, 4.0 mm, 4.5 mm, 5.0 mm, 5.5 mm, 6.0 mm, 6.5 mm or 7.0 mm. In some embodiments, the inner diameter is about 2.5 mm, 3.0 mm, 3.5 mm, 4.0 mm, 4.5 mm, 5.0 mm, 5.5 mm, 6.0 mm or 6.5 mm or any size therein to about the 100th of a mm. In some embodiments, the outer diameter is about 5.3 mm and the inner diameter is about 4.8 mm. Other suitable diameters can also be used. Different size clips can be used depending on the specific tissue compression or closure application for which they are being used and to account for different anatomical sizes, such as differences in the thickness or diameter of the vessel

wall **16**. In some instances, a plurality of different-sized clips **102** can be provided to health care professionals to allow for variability and increased precision in diminishing trauma and increasing the appropriate closure force for a particular patient. Moreover, a clip size also can be selected to accommodate the tubular medical device over which the clip will be advanced. In embodiments effecting arteriotomy closure, the clip's inner diameter should be large enough to be advanced over a standard commercial introducer.

[00153] As illustrated in **FIG. 6**, the tines can have straight edges **145** and define an inner angle α **405**. Angle α **405** can be selected to help adjust an insertion force required to cause penetration of the tines **126a**, **126b** into or withdrawal of the tines **126a**, **126b** from the vessel wall **16**. In some embodiments, angle α **405** can be greater than or equal to about 3° and/or less than or equal to about 15°. In some embodiments, angle α **405** can be about 3°, 4°, 5°, 6°, 7°, 8°, 9°, 10°, 11°, 12°, 13°, 14° or 15° or any value therein to about 100th of a degree. In some embodiments, angle α **405** can be about 9°. Other suitable angles can also be used. The widths of the tips **127a**, **127b** of tines **126a**, **126b** can also be adjusted to determine a required insertion force. In certain embodiments, the width of tips **127a**, **127b** can be greater than or equal to about 0.03 mm, and/or less than or equal to about 0.09 mm. In certain embodiments, the width of tips **127a**, **127b** can be about 0.03, 0.04, 0.05, 0.06, 0.07, 0.08 or 0.09 mm or any size therein to about the 100th of a mm. In certain embodiments, the width of tips **127a**, **127b** can be about 0.06 mm. Other suitable tip widths can also be used. In certain embodiments, the edges of the tines **126a**, **126b** can be curved, segmented, or define different angles at different portions. In certain embodiments, the tines **126a**, **126b** can include barbs, protrusions, or other elements configured to resist withdrawal from the vessel wall **16**. The barbs can be sized or configured to provide sufficient resistive force to prevent accidental removal of the clip **102** during partial deployment of the clip **102** as explained in more detail below. In certain embodiments, the resistive force provided by the barbs can also be sufficiently small to permit atraumatic removal of the clip **102**.

[00154] For embodiments in which the base **120** is substantially circular, arc **406** corresponds to the circumferential width of fingers **122** and **124**. In the illustrated embodiment, arc **406** subtends an approximately 90° angle. In some embodiments, arc **406** can subtend an angle greater than or equal to about 60° and/or less than or equal to about 90°. In some embodiments, arc **406** can subtend an angle of about 60°, 65°, 70°, 75°, 80°, 85°, or 90° or any value therein to about 100th of a degree. Other angles can also be used. Arc **403** corresponds to a circumferential width of window portions **125**. In some embodiments, arc **403** can subtend an angle between greater than or equal to about 15° and less than or equal to about 30°. In some embodiments, arc **403** can subtend an angle of about 15°, 16°, 17°, 18°, 19°, 20°, 21°, 22°, 23°, 24°, 25°, 26°, 27°, 28°, 29° or 30° or any value therein to about 100th of a degree. In certain embodiments, arc **403** can be less than or equal to about one-half the length of arc **406**. Connecting portions of fingers **122** and **124** adjacent to the window portions **125** can have widths defined by arcs **402** and **404**. Arc **139** corresponds to the separation distance

between fingers **122** and **124**. In the illustrated embodiment, arc **139** subtends an angle of approximately 90°. In some embodiments, arc **139** can subtend an angle greater than or equal to about 60° and/or less than or equal to about 90°. In some embodiments, arc **139** can subtend an angle of about 60°, 65°, 70°, 75°, 80°, 85°, or 90° or any value therein to about 100th of a degree. Other angles can also be used. In some embodiments, as illustrated, the shape and/or orientation of the base portion are substantially or entirely unchanged in the transition between an open or pre-deployed state and a closed or deployed state.

[00155] **FIG. 7** is a perspective view of deployment instrument **104** with clip **102** in the open or pre-deployed position attached to a distal end thereof. The configuration illustrated in **FIG. 7** is generally an initial or starting configuration before insertion of the deployment instrument **104** into a patient. The deployment instrument **104** with a pre-loaded clip **102** can be provided to the physician in a sterilized package in this general configuration. In certain embodiments, the deployment instrument **104** can be constructed with three basic components: inner tubular member **154**, outer tubular member **156**, and pressure element **158**.

[00156] **FIGS. 47A-D** illustrate another embodiment of a vascular closure clip **350**. Clip **350** as illustrated can be similar in many respects to clip **102** except as described below. A primary difference between clip **350** and clip **102** is that the arrangement of fingers **252**, **254** on clip **350** is asymmetric: the number of tines **256**, **258** on each side is not equal. For example, as illustrated, a first finger **252** can include three tines **256**. A second finger **254** can include two tines **258**. Tines **256** and tines **258** can be offset from one another and configured to interlace when clip **350** is in a closed configuration as seen in **FIGS. 47B-D**. For some applications, this interlacing configuration can provide certain advantages over the configuration of clip **102**. For example, fingers **252** and **254** can be configured to apply greater compression to tissue and to more completely close the arteriotomy **14**, by attempting to draw generally opposing sides of tissue past one another. In addition, the interlaced configuration can in some embodiments, permit a smaller angle **2 259** to be formed between a central axial line or an edge in fingers **252**, **254** and a peripheral surface or an edge **253** of a base portion **251** for a given length of fingers **252**, **254**. In some embodiments, angle **2 259** can be greater than or equal to about 10° and/or less than or equal to about 50°. In some embodiments, angle **2 259** can be about 10°, 15°, 20°, 25°, 30°, 35°, 40°, 45°, or 50° or any value therein to about 100th of a degree. In a particular example, angle **2 259** can be about 30°. Other suitable angles may also be used. In the illustrated example of **FIG. 47C**, fingers **252** and **254** do not contact one another when clip **350** is in its closed or deployed configuration. In other embodiments, fingers **252** and **254** can be configured to contact one another in the deployed configuration. For example, tines **258** can be configured to rest on forward surfaces **253** of finger **252**. Tines **256** can be configured to rest on forward surfaces **255** of finger **254**.

[00157] **FIGS. 48A-B** illustrate another embodiment of a vascular closure clip **260**. Clip **260** can be similar to other clips disclosed herein, except as described below. Clip **260** includes three symmetrical fingers **262** extending from annular base **261**. As illustrated, fingers **262** can be uniformly spaced around the circumference of base **261**. Each finger **262** can include two tines **264**. Distal ends of tines **264** are configured to meet when clip **260** is in its closed configuration as illustrated in **FIG. 48B**.

[00158] **FIGS. 49A-B** illustrate another embodiment of a vascular closure clip **270**. Clip **270** can include three symmetrical fingers **272** which can be uniformly spaced around the circumference of annular base **271**. Clip **270** can be similar in many respects to clip **260**. A primary difference between clip **270** and clip **260** is that the tines **274** of clip **270** are configured to overlap tines **274** of adjacent fingers when clip **270** is in a closed configuration.

[00159] **FIGS. 50A-B** illustrate another embodiment of a vascular closure clip **280**. Clip **280** can be similar to other clips disclosed herein. Clip **280** can include three fingers **282**, which can be substantially uniformly spaced around the circumference of annular base **281**. Each finger **282** includes two tines **284** which are offset to one side from a central portion of the finger **282**. This configuration can permit fingers to bend to a greater degree in the closed configuration without overlapping.

[00160] **FIGS. 51A-E** illustrate another embodiment of a vascular closure clip **290**. Clip **290** can be similar to other clips disclosed herein, except as described below. Clip **290** includes six fingers **292** substantially uniformly spaced around a circumference of base portion **291**. In some embodiments, each finger **292** includes only a single tine **294**. Tines **294** are configured to fold to a substantially flat configuration, best seen in **FIG. 49D**. Such a configuration permits clip **299** to have a relatively low interior profile. Tines **294** are not configured to contact one another when clip **290** is in a closed configuration. In other embodiments, tines **294** can be configured to meet at or close to a central point, or other point. Tines **294** include a distal-most portion **295** and a second more-proximal portion **296**. Portion **295** defines a first interior angle which can be smaller than an interior angle defined by portion **296**. Such a configuration gives tines **294** a relatively "sharp" tip and can facilitate the tines' initial penetration of vessel wall **16**. Base portion has a height **298**. As illustrated height **298** can be relatively small and can be, for example, approximately equal to or less than one fifth of a radius defined by annular base portion **291**. A relatively small height **298** permits the clip **290** to have a relatively low external profile when implanted.

[00161] Clip **290** can provide more complete circumferential closure by being configured to engage tissue on substantially all sides of arteriotomy. In certain embodiments, it can be more desirable to use such clips **290** for permanent implantation and other clips for temporary implantation. For example, the use of only two opposed fingers can facilitate removal. The use of only two opposed fingers can create a "pinching"-type closing action which can be advantageously simple and predictable.

[00162] In certain embodiments, heat can be used to facilitate the closure of arteriotomy **14**. **FIG. 52** illustrates a circuit 500 using direct resistive element heating to heat tissue surrounding the arteriotomy **14**. In certain embodiments, selected tissue surrounding the arteriotomy can be heated to a temperature which can be equal to about 40°C, between about 40°C and 45°C, or greater than about 45°C. In certain embodiments, selected tissue surrounding the arteriotomy can be heated to a temperature of about 35°C, 36°C, 37°C, 38°C, 39°C, 40°C, 41°C, 42°C, 43°C, 44°C, 45°C, 46°C, 47°C, 48°C, 49°C, or 50°C or any value therein to about 100th of a degree. Other suitable temperatures may also be used. At these temperatures, tissue being compressed together by a vascular closure clip can undergo cellular changes that tend to fuse tissue together to close the arteriotomy.

[00163] Other clip variations are also possible. The tissue compression can be modified by adjusting one or more of several tissue engagement element design attributes, such as the length, width, thickness, angle, number and location of the elements, etc. The proximal edge of the clip can have a straight, sinusoidal, notched, keyed, combination or other suitable design. The proximal edge geometry can mate with a contacting surface of the advancement and deployment instrument. Clips can be made from one or more of a tubing, sheet, wire, strip, band, rod, combination or other suitable material.

[00164] **FIGS. 56A-C** illustrate an additional embodiment of a vessel closure system. In one embodiment, a swellable plug **310** which can be bioabsorbable is loaded onto the distal end of a plug deployment instrument **300**. Plug deployment instrument **300** can include an inner tubular member **302** with handle **306** and an outer tubular member **304** with handle **308**. The proximal end **312** of plug **310** can be received by the distal end of outer tubular member **304**. Intermediate stop portion **314** of plug **310** can have a larger outer diameter than either proximal end **312** or distal end **316** and is received against the distal end of the outer tubular member **304**. As illustrated, stop portion **314** can have a generally circular geometry. However, other suitable shapes or geometries can be used. For example, in certain embodiments stop portion **314** can have a flared or tapered shape, a general 'X' shape, an inverted general 'T' shape, a combination or any other suitable shape or geometry. In certain embodiments, stop portion **314** can be slotted or ribbed to facilitate flexing during advancement. Proximal end **312** can be relatively long to facilitate plug kinking as will be described below. In certain embodiments, proximal end **312** can have a length that is greater than or equal to about twice the length of distal end **316**, and/or greater than or equal to about five times the length of distal end **316**. Plug **310** can include a longitudinal channel **318** allowing the deployment instrument **300** and plug **310** to be advanced over a tubular medical device in a similar fashion to that described above with respect to deployment instrument **104**. Inner tubular member **306** can be advanced distally by applying pressure to handle **306** and/or by pulling handle **308** in a proximal direction. A stop means such as a removable element affixed to the outer tubular member **302** between handles **306** and **308** can maintain separation of handles **306** and **308** until the medical professional is ready to begin deployment. Once the medical professional has confirmed proper placement of the distal end of the

deployment instrument **300**, the stop means can be overcome by for example removing the removable element in order to begin deployment. The distal end of inner tubular member **306** pushes plug **310** free of the outer tubular member **304** to effect deployment. The deployment instrument **300** can be configured such that the plug **310** will be fully deployed when the handles **306** and **308** have been brought together.

[00165] Swellable plug **310** can be partially or completely fabricated from materials that swell or expand when they are exposed to a fluid, such as blood or subcutaneous fluid, or another fluid, for example, that can be added by the physician to cause the material to swell. These materials include hydrophilic gels (hydro gels), regenerated cellulose, polyethylene vinyl acetate (PEVA), as well as composites and combinations thereof and combinations of other biocompatible swellable or expandable materials. Upon deployment, swellable plug **310** can swell causing longitudinal channel **318** to be occluded and sealing the arteriotomy. In certain embodiments, plug **310** can be partially or completely fabricated from a lyophilized hydrogel, such as, for example polyethylene glycol (PEG) or other polymer carrier. The polymer used in the carrier can include hydrolytically degradable chemical groups, thereby permitting in vivo degradation. Hydrophilic polymeric materials suitable for use in forming hydrogels include poly(hydroxyalkyl methacrylate), poly(electrolyte complexes), poly(vinylacetate) cross-linked with hydrolysable bonds, water-swallowable N-vinyl lactams polysaccharides, natural gum, agar, agarose, sodium alginate, carrageenan, fucoidan, furcellaran, laminaran, hypnea, eucheuma, gum Arabic, gum ghatti, gum karaya, gum tragacanth, locust bean gum, arabinogalactan, pectin, amylopectin, gelatin, hydrophilic colloids such as carboxymethyl cellulose gum or alginate gum crosslinked with a polyol such as propylene glycol, and the like. Several formulations of previously known hydrogels are described in U.S. Patent No. **3,640,741** to Etes, U.S. Patent No. **3,865,108** to Hartop, U.S. Patent No. **3,992,562** to Denzinger et al., U.S. Patent No. **4,002,172** to Manning et al., U.S. Patent No. **4,014,335** to Arnold, U.S. Patent No. **4,207,893** to Michaels, and in Handbook of Common Polymers, (Scott and Roff, Eds.) Chemical Rubber Company, Cleveland, Ohio, all of which disclosures in the foregoing patents and publication regarding hydrogels are incorporated herein by reference.

[00166] An example of a method for using plug deployment instrument **300** and plug **310** will now be described with reference to **FIGS. 57-63**. The deployment instrument **300** loaded with plug **310** can be advanced over a previously installed tubular medical device **108** as shown in **FIG. 57** until the distal end **316** encounters vessel wall **16**. In certain embodiments, as illustrated, distal end **316** can be received within the arteriotomy **14**. In other embodiments, distal end **316** can be received against an outer surface of vessel wall **316**. Intermediate portion **314** can be configured to act as a stop to prevent over-insertion of plug **310** into the vessel. The introducer sheath can then be removed from the vessel as shown in **FIG. 59**.

[00167] As shown in **FIG. 60**, the deployment instrument **300** can be held in place against the vessel wall **316** while the exposed portions of plug **310** begin to swell. The swelling can be initiated

or accelerated by various events, such as coming into contact with blood and/or subcutaneous fluid. In certain embodiments, the enlargement of distal end **316** can help to secure the plug **310** in place within the arteriotomy **14**. The swelling of plug **310** can occlude longitudinal channel **318**, tending to seal or otherwise partially or entirely fill the arteriotomy **14**. Alternatively or additionally, the channel **318** can be occluded via kinking of proximal portion **312**. Once the plug **310** is secured to the vessel wall **16**, deployment instrument **300** can be removed as shown in **FIG. 61**. Fatty tissue that was previously displaced by the deployment instrument **300** may begin to fill in the tissue tract. This tissue can thus apply pressure to proximal portion **312** tending to kink or occlude it. Patient movement and/or externally or internally applied pressure can also be used to cause the proximal portion **312** to kink. Deployment of plug **310** at an acute angle to the vessel wall, as illustrated, can also increase the tendency of proximal portion **312** to kink. In certain embodiments, the inner surface of the longitudinal channel **318** can be configured to stick to itself when one region of it contacts another region. For example, in certain embodiments inner surfaces of longitudinal channel **318** can be coated with an adhesive or other appropriate coating to assist in occluding the longitudinal channel **318**. In certain embodiments, the adhesive or coating can be configured to avoid or to diminish adherence to the deployment instrument **300**. **FIG. 62** shows an embodiment of the deployed plug **310** in a fully swollen state. Plug **310** can be completely or partially bioabsorbable. In certain embodiments, plug **310** can be configured to be completely absorbed by the patient's body after about 4 weeks. Other suitable times may also be used. **FIG. 63** shows the plug **310** in a partially-dissolved state.

[00168] Swellable plug **310** can be shielded from unintended contact with fluid (blood, saline, etc.), before insertion into the body, by a removable wrapper or dissolvable coating. Swellable plug **310** can include a relatively rigid outer coating that begins to dissolve upon exposure to fluids such as blood, thus providing time for the medical professional to position the plug **310** within the arteriotomy. In some embodiments, a plug can be configured to be advanced directly over the tubular medical device **108** and deployment instrument **310** can be replaced with a pusher instrument. In certain embodiments, a plug can include a longitudinal slit or spiral allowing the plug to be attached to the tubular medical device or deployment instrument from the side. In certain embodiments, the deployment instrument can also include a slot allowing attachment from the side.

[00169] The vascular closure device can incorporate one or more coatings, materials, compounds, substances, drugs, therapeutic agents, etc., that positively affect healing at the site, at and or near where the device is deployed, either incorporated into the structure forming the device, incorporated into a coating, or both. Thrombo-resistance materials, antiproliferative materials, or other coatings intended to prevent thrombosis (acute and or chronic), hyperplasia, platelet aggregation, or other negative response, at or near the attachment of the device within the body. The coatings, materials, compounds, substances, drugs, therapeutic agents, etc., can be used by themselves, and/or contained in a carrier such as a polymeric matrix, starch, or other suitable material

or method. The coatings can be liquid, gel, film, uncured, partially cured, cured, combination or other suitable form.

[00170] Additional configurations of closure devices or clip, plug or closure device **670** are illustrated in **FIGS. 79A-E**. The clip, plug or closure device **670** has a plate section, wings or petals at a first end, an elongated neck section which is the core, stem, vertical section, mid-section, post or shaft, and a set of flanges **675** extending from the neck at an opposing end which are radially extending members, wings, petals or horizontal protrusions. As illustrated, the face plate is triangular and has three petal shapes on its distal end (the end within the wound) which meet centrally at a center point along the face plate and extend outwardly. The petals can be raised sections with scoring, or whatever configuration assists in allowing the face plate to bend toward the inner axis **A** during deployment. Additionally, a fewer or greater number of scored or raised petals can be provided. Additionally, the shape of the face plate may result in a different number of petals being used on the surface. The clip, plug or closure device **670** may further include an aperture or bore **676** through at least a portion of the elongated neck section or stem **672**. Horizontal grooves can be provided around the core to reduce bleeding and for added sealing. The plug may also be coated in lubricant to assist vessel contact opening and to reduce the force required to advance the plug through the capsule and introducer sheath tubing or into the target site. The wound or vessel contacting surfaced may vary in thickness, profile and geometry and the middle plug core or stem may vary in thickness, profile, geometry, and/or any other aspect. Additionally, the middle plug section may be at least partially hollow. Moreover, any surface of the plug may be configured to have at least one smooth, textured, patterned, grooved, or a combination thereof. The plug may have at least one of a hole, notch, void, dimple, groove, slot, indentation, concave section, or any other desired configuration. Plug sections can be made from a single piece or multiple pieces. Where separate pieces are used, the separate pieces can be fixed or moveable. For example the plug may be configured so that the outer vessel contacts can be moved toward the inner vessel contacts, contacting (and compressing, if desired), the vessel. The moveable outer vessel contacts may be configured to maintain its position, relative to the vessel wall and/or inner vessel contacting area, by any suitable technique, including a single or two way ratched and/or one or more of either or both of bump(s) or protrusion(s) between the core (column) and the outer vessel contacts, enabling a custom or optimized fit between the inner and outer vessel contacts. The plug may have at least one of a radially extending inner vessel element, and a radially extending outer vessel element. The outer vessel element may be located at any point on the center (e.g., at axis **A**) or core of the plug, and may not necessarily be in direct or close contact with the outer vessel wall surface. The inner vessel member and one or more vertical cores, when deployed (unconstrained), upper ends of the core may move (all together, independently, or a combination) to an open position into an expended or larger cross-section from the constrained or deflected position during advancement using a tubular medical device.

[00171] The triangular plate section or face plate **680** is adapted and configured to be placed on an interior surface of a tissue layer to be sealed, with the elongated neck **672** extending through the wound, and two or more flanges **675** positioned exteriorly to the wound and proximal to the deployment device. The face plate can be configured such that it is flat on a proximal side and convex on a posterior side. With the face plate further being scored along its posterior face to facilitate conforming the face plate into a low profile configuration for delivery. The stem or core can be straight, curves, angled or a combination thereof. Moreover the stem can assist in achieving plug contact and/or attachment to the vessel. Additionally, the device may be substantially straight during deployment or advancement through the introducer sheath, and then moved to another configuration when it is no longer constrained within the tubular medical device (such as an introducer sheath). The devices and systems can be configured to provide a partial or complete circumferential closure device to secure an implantable device, such as a ventricular assist device. Rotation and/or detent may be incorporated into the system for a final plunger forward advancement movement and confirmation that the plug is fully deployed and the sheath is ready to be withdrawn.

[00172] For purposes of illustration in the context of a device that is delivered *in situ*, a suitable configuration of the plugs disclosed herein provides for a length of about 3.81mm to about 5.08mm, or more preferably about 4.39mm, or any value therein to about the 100th of a mm. The bore has a length of about 2.92mm to about 3.94mm, or more preferably about 3.43mm, or any value therein to about the 100th of a mm. The width of the bore is about 0.76mm to about 1.27mm, or preferably about 1.00mm, or any value therein to about the 100th of a mm. The stem of the plug between the cap and the flanges **675** ranges from about 3.30mm to about 3.81mm, more preferably 3.48mm, or any value therein to about the 100th of a mm. The overall diameter of the device ranges from about 3.81mm to about 4.57mm, or more preferably 4.27mm, or any value therein to about the 100th of a mm. As shapes are not necessarily circular, these value can represent, for example, a diameter of a two-dimensional circular shape that encompasses the flanges **675** or the face plate. Devices that are used from outside the body (e.g., to repair an external wound in lieu of compression, would be sized larger).

[00173] Additional configurations of closure devices or clip, plug or closure device **670** are illustrated in **FIGS. 79F-J**. The clip, plug or closure device **670** has a plate section, wings or petals at a first end, an elongated neck section which is the core, stem, vertical section, mid-section, post or shaft, and proximal bail or loop **675'** extending from the neck at an opposing end for attachment to a tether line, where the tether is looped through the bail and when the tether loop is cut it pulls out through the loop **675'**. The clip, plug or closure device **670** may further include an aperture or bore **676** through at least a portion of the elongated neck section or stem **672**.

[00174] The clip, plug or closure device **670** can be deployed in combination with, for example, a removeable tether. The use of a tether allows confirmation of proper placement and sealing of the seal and reduces inadvertent manipulation of a deployed clip, plug or closure device **670**

. The tether can be, for example, a thread, wire, and/or coil. The tether can be made from cotton, polymer, metal, metal alloy, and may be compliant, semi-rigid, rigid or of a changing rigidity. The tether may be pre-shaped, using nitinol for example, or any suitable material including silk, metal or metal alloy or polymer. The pre-shaped tether may be configured to hold the plug during deployment, and then pulled out or away from the plug, separating from the plug and withdrawing from the body. Additionally, the tether may be a separate component, and/or integrated into the design of the plug, and may include at least one weakened section designed to separate from the plug at a specific section. In some configurations, the tether may be adapted to separate from the plug by pulling, pushing, twisting, or combinations thereof or any other separation mechanism. Moreover, the tether may be configured to be separable, as shown in some embodiments herein, by a weakened area, the strength of the tether, the strength of the attachment between the tether and the plug or combinations thereof.

[00175] As shown in **FIGS. 80A-C** the clip, plug or closure device **670** can be configured to provide a collapsible clip, plug or closure device **670** with a distal end **80** that fits within an opening on the proximal end **70** of the clip, plug or closure device **670** and is attached to a tether or wire **674** at its proximal end **70** that, when pulled, causes the clip, plug or closure device **670** to collapse. The delivery system and wire **674** are then withdrawn through the delivery device and the entire delivery system is completely disengaged, leaving the clip, plug or closure device **670** deployed *in vivo*. **FIGS. 81A-N** illustrates other removeable configurations wherein a tether or wire **674** is used to allow confirmation of proper placement and seating of the clip, plug or closure device **670**. As shown in **FIG. 81A**, a bent wire **674** is routed through a central bore **676** in the clip, plug or closure device **670**. The wire **674** is configured such that a force required to straighten the wire and pull it through the bore **676** is equal to a release force. As shown in **FIG. 81B** the wire **674** can be configured to spring away from a central axis **A** as the wire **674** is pulled proximally toward the user and away from the clip, plug or closure device **670**. In **FIG. 81C** the wire **674** is configured with a wavy bend such that the apex of the bends engages the side walls **678** of the tubular channel **678'** formed in the clip, plug or closure device **670**. The distal end **80** of the wire **674** can engage the plug face plate **680** in a semi-permanent configuration such that a force is required to disengage the wire **674** from the clip, plug or closure device **670** and withdraw it through the channel. As shown in **FIG. 81D** the channel can include a groove or well into which a bend in the wire extends forming a detent **636**. A suture line can be used as shown in **FIG. 81E**. The suture line **674** can be configured to disengage from the clip, plug or closure device **670** as shown. Other configurations include, for example, a bent wire **674** configuration as shown in **FIG. 81F**, where a helical coiled wire **674** is configured to decrease in outer diameter when tension is applied. **FIG. 81G** illustrates a staggered or bent bore or channel **678** in the clip, plug or closure device **670** through which a strained wire **674** is positioned. The strained wire **674**, thus must flex through the staggered or bent bore or channel **678**. In **FIG. 81H** the wire **674** is configured to have an elongated S curve with a sharp tip that points away from the pull direction (e.g.,

toward the distal end **80**). As shown in **Figs. 81e-h**, a portion of the line **674** can extend through the distal surface of the cap **680** taking a variety of configurations parallel to the cap **680** surface or coiled.

[00176] Other concepts include, for example, tethered clip, plug or closure device **670** concepts where, for example, a tether **674** in the form of a loose thread passes through an aperture **679** on a proximal end **70** of the clip, plug or closure device **670** as shown in **FIG. 81I**. Alternatively, the proximal end **70** of the clip, plug or closure device **670** could be in the form of a safety pin clasp as shown in **FIG. 81J** which unhinges to release the tether **674**. A pincher clasp could likewise be used, as shown in **FIG. 81K**, or a snap and ball socket as shown in **FIG. 81L**. A molded-in break point could also be used such that the bolded break point breaks when tension is applied from a proximal end **70** as shown in **FIG. 81M**. In another configuration a ribbon section is used as shown in **FIG. 81N**.

[00177] Additional release concepts are shown with respect to **FIGS. 82A-B**. The configuration illustrated in **FIG. 82A** relies on an overstretch section at a weak point along the length of the stem of the closure device **670**. Over-stretch can be combined with a twist action that results in a snap of the stem **672** along its length. In some configurations, as shown in **FIG. 82B**, tear notches can be provided which enable the stem **672** to be separated using a tear motion, which then tears along the tear notches, and releases the clip, plug or closure device **670**. A cutter can be used in combination with a tether tube **678'**. As will be appreciated by those skilled in the art, a radiopaque marker can be employed, such as a tungsten ball, such that the device can be seen on an x-ray monitor or other imaging device. The radiopaque marker can be positioned such that it is part of a break-away portion of the plug such that it can be removed when it is no longer clinically necessarily or desirable to have the marker in place.

[00178] Tethered clip, plug or closure device **670** are also contemplated. Tether clip, plug or closure device **670** can use, for example, a ball-and-socket design as shown in **FIG. 83A**. In this configuration, a molded ball is provided on the plug stem. The molded ball socket has one or more splits. When opened, the splits form finger than can easily open to release the ball within the socket. As shown in **FIG. 83B** a tether line **674** can be provided in combination with a tether tube **682**. The tether tube restrains the fingers formed in the molded ball socket and restrains the fingers from opening. This maintains a secure grip on the ball until the tether line **674** and tube **682** are retracted. When the tether tube and line are retracted, as shown in **FIGS. 83C-D**, the ball is withdrawn as well. This configuration has very high grip security on the plug via the tether line until the user slides the tether tube **682** from the end.

[00179] In another configuration, the tethered clip, plug or closure device **670** can be used in conjunction with a ball-socket tether tube **682**-tether line **674** as shown in **FIG. 84A**. The ball can be positioned such that it is fixed in relation to the ball and tether tube **682** end. A release button **684** configuration can be used to lock the tether tube **682** in place, wherein movement of the tether tube **682** along an axis **A** stops when the one or more buttons reach a detent **636**. As shown in **FIG. 84B** the

tether tube **682** can retract past the end of the clip, plug or closure device **670**, for example when the release button is pushed. The diameter of such a configuration is about 1.0 to 2.5 mm, or more preferably about 1.5 to 2.0 mm, or any diameter therein to about 100th of a mm. In a snip-off design shown in **FIGS. 84C-D**, the tether tube **682** travels to a button stop **684**, similar to the configuration shown in **FIG. 84A** and then is snipped at a cut line near a proximal end **70**.

[00180] Further to the designs depicted in **FIGS. 79-84** a variety of clip, plug or closure device **670** profiles is also contemplated. As shown in **FIG. 85A** the closure device **670** can have a round or substantially round disk or face plate **680** at a distal end **80** with a stem **672** protruding from a proximal surface of the disk. The stem **672** can be a locating, centering and/or anchoring stem. As will be appreciated by those skilled in the art, the stem **672** can have a variety of configurations as shown in more detail in **FIGS. 85B-R**. The stem **672** can be configured to have a square or rectangular cross-section as shown in **FIG. 85B** which could then be a variety of cross-sections along its perpendicular axis to the one depicted (e.g., round, square, etc.), a triangular cross-section as shown in **FIG. 85C** which could then be, for example, pyramidal or conical in three dimensions, a stem with an arrow-head as shown in **FIG. 85D** with the same three -dimensional considerations previously described, have a concave proximal surface as shown in **FIG. 85E**, a convex proximal surface as shown in **FIG. 85F**, a combination of a stem with an arrow-head having a concave surface adapted to receive a mating ball as shown in **FIG. 85G**, a stem with an aperture perpendicularly through the stem to receive, for example, a wire, as shown in **FIG. 85H**, a stem with flanges **675** tapered distally as shown in **FIG. 85I**, a stem shaped as a trapezoid with its wide edge being positioned proximally and its narrow edge adjacent the disc portion of the closure device. In another configuration, the stem is shaped as a hook in cross-section with a rounded hook as shown in **FIG. 85K** or a catch as shown in **FIG. 85L**. Additionally, effective is the use of a protuberance as part of a detent **636** system as shown in **FIG. 85M**, or a channel which opens to receive a mating element having a wider head as shown in **FIG. 85N**. A variety of screw configurations can also be employed for the stem **672**, as shown in **FIGS. 85O-P**. Standard threading of the stem **672** can be used, as shown in **FIG. 85O**. Alternatively, internal threading in a bore of the stem **672** can be used as shown in **FIG. 85P**. A bi-stable geometry can also be used as shown in **FIG. 85Q-R**.

[00181] The closure device can also be configured to provide for inner petals as shown in **FIGS. 86A-E**. The stem **672** of such a configuration could have a small diameter under 1mm with an optional suture line. Various stem options are included which illustrate ribs and nibs on both sides of the distal sealing surface or skirt. As shown in **FIG. 86A**, the stem **672** can have bulbous sections along its length which have a diameter greater than the small diameter of the stem. Alternatively, the neck can be less than 1mm, or any value to 10mm as shown in **FIG. 86B** but end with a flat disk **680** at its proximal end **70** in communication with a suture line **674**. As shown in **FIGS. 86C-D** a closure device **670** could be pressed into place with the disk **680** configured such that the outer edges can move towards a central axis **A** as the device **670** is pressed through a wound, and then open up once

in, for example, the vessel with the disc placing pressure on the vessel wall to retain its position. As shown in **FIG. 86E**, the device **670** can be configured to have a hollow plunger which seats under the cap of the device. A variety of configurations of the disk can be employed and post configuration on the surface of the disk can be employed without departing from the scope of the disclosure as will be appreciated by reviewing **FIGS. 87A-B** and **FIGS. 88A-F**. As shown in **FIGS. 87A-B** the device **670** comprises a disk **680** that can be substantially flat from a side view and substantially round from an end view, with a post or stem **672** and/or tether or suture line **674** centrally positioned on the disk **680**. As shown in **FIGS. 88A-F** the disk **680** can be round, triangular, oval, ovoid, square, triangular and elongated (with wings). Typically these shapes will also have rounded edges, for example, a square or triangular shape could be rounded at the corners as shown in **FIGS. 88B**. Moreover, the sides can be bent inward toward a central point such that, for example, a triangular shape becomes closer to a Y shape as shown in **FIG. 88C**. Additionally, a variety of side profiles can be employed as shown in **FIGS. 88D-F**, for example flat, concave, convex, flat on one side and convex or concave on the opposing side, with or without an interior chamber as shown in **FIG. 88E**. In some configurations, ribs and nibs **686** can be provided on one or more surfaces to facilitate anchoring the device *in situ* as shown in **FIGS. 88F** and **89A-G** which illustrate embodiments and embodiments deployed *in situ*. Nibs **686** on a proximal surface will, when the device **670** is inserted into, for example, the vessel, engage the interior surface of the vessel to prevent withdrawal of the device **670** and to minimize or eliminate movement of the device *in situ*.

(c) **Guided Tissue Cutter**

[00182] **FIGS. 40-42** illustrate an example of a tissue opening widener such as a guided slidable tissue cutter **106**, which can be used in a vessel closure system **100** in certain embodiments. After completing the desired medical procedure, the medical professional can temporarily attach tissue cutter **106** by clipping it onto the tube section **110** of the vascular introducer **108** as shown in **FIG. 1**. The tissue cutter **106** can then be slidably advanced along the vascular introducer sheath **108**. The cutter **106** can be configured to make an incision of a precise depth and width at the site of the percutaneous opening **12** using sharp distal edges **203** of blades **202**. The cutter **106** generally positions the edges **203** of the blades **202** at a specific orientation and distance from the tube **110** to permit a consistently and modestly sized entry point for the deployment instrument **104**. A ledge such as mechanical stops **208** can ensure that the incision is not any deeper than needed to facilitate entry of the deployment instrument **104**. Using the existing introducer sheath **108** as a guide for the slidable tissue cutter **106** also assists in ensuring proper placement of the incision. After making the incision, the slidable tissue cutter **106** can be removed from the side of the vascular introducer.

[00183] **FIGS. 41-43** illustrate an example of a frame portion **200** which can form a component of a slidable tissue cutter **106**. In certain embodiments, scalpel blades **202** can be secured to frame portion **200**. In other embodiments, the cutter **106** can use specialized blades and/or be formed from a single piece. As illustrated, slidable cutter **106** includes two blades **202** positioned on

lateral sides, such as in a diametrically opposite position from one another. In other embodiments, a single blade or three or more blades can be used. In certain embodiments, the cutting surfaces of each blade **202** can be static and configured to cut tissue without requiring interaction with a second cutting surface. In other embodiments, dynamic blades can be used.

[00184] Slidable cutter **106** can include a channel **206** with a partial circumferential cross-sectional geometry as shown in **FIG. 43**. This geometry enables a "snap-on" feature permitting the cutter **106** to be easily and temporarily attached to the tubular medical device and facilitating removal of the cutter **106** once the desired tissue has been cut. In other embodiments, a slidable cutter can use two mating pieces that clamp or snap together to facilitate temporary attachment and removal. In a preferred embodiment, channel **206** is sized so as to be compatible with any commercialized introducer sheath. The ends **208** of the frame portion **200** act as mechanical stops to control the depth of the incision. In some embodiments, handle portions **204** can extend beyond the end of channel **206** to facilitate handling by the medical professional at a distance from the sharp edges **203**.

Advantageously, such a configuration can facilitate the medical professional's control of the instrument without requiring an increase in the length **205** of channel **206**. Most commercially available vascular introducers are between 11 and 13 cm long. Once inserted into a patient's vessel, the exposed portion of the introducer's tube section can be relatively small. Thus, it can be desirable to limit the amount of tube section that is taken up by the attached cutter and hence to reduce the length **205** of channel **206**. The proximal ends of the handle portions **204** can be flared outwardly as illustrated to provide increased space between the cutter **106** and the tube **110** for improved manual access and manipulation, and to permit the deployment instrument **104** to be positioned as close axially as possible to the generally short exposed length of tube **110**. The lateral edges of the cutter **106** can be tapered as illustrated.

[00185] Frame **200** can include recesses **210** sized to receive scalpel blades **202**. The recesses **210** can be used to shield portions of the blades **202** not intended to cut tissue. Scalpel blades **202** can be secured to frame **200** via one or more of a variety of known methods such as, for example, friction-fitting, mechanical interference fitting, sonic welding, adhesives, screws, clamps, and the like. As illustrated, scalpel blades **202** are configured to angle inward toward one another slightly. Such a configuration can help to ensure that the blades **202** cut tissue immediately adjacent to the percutaneous opening **12**. In other embodiments, scalpel blades **202** can be oriented in a substantially parallel configuration. In some embodiments, the blades **202** can be adjustable, allowing a medical professional to adjust one or more of the incision's depth, width, and angle, and/or a collection of cutters **106** of different sizes can be provided for different applications. In certain embodiments, slidable tissue cutter **106** is configured to cut substantially only the patient's skin. Fatty tissue located beneath the skin will generally move out of the way of the deployment instrument **104** with minimal resistance. Accordingly, a deeper incision may not be necessary in some embodiments.

[00186] The cutter **106** can be made from one or more of the following materials: polymers, including Nylon, polyamide, polycarbonate (e.g., Makrolon®), acrylonitrile butadiene styrene (ABS), polyester, polyethyleneterephthalate (PET), polyetheretherketone (PEEK™), polyimide, superelastic / shape memory polymers and metals, including spring steel, stainless steel, shape memory metal alloys including nickel titanium alloys (Nitinol), 17-7 PH, cobalt-chromium-nickel alloy (Elgiloy®), and nickel based alloys with chromium and iron (Inconel®). Other appropriate materials can also be used. In embodiments using a "snap-on" feature the frame **200** can be sufficiently flexible to allow the walls of the channel to bend outwardly to accommodate the tubular medical device **108**. The slidable cutter **106** can be completely or partially fabricated using one or more of the following methods: casting, laminating, machining, molding (injection or other), sintering, stereo lithography. Other suitable methods can also be used. Advantageously, the slidable tissue cutter **106** can be inexpensive to produce and designed for one-time use. In other embodiments, the tissue cutter **106** can be designed for repeated use following sterilization. An additional advantage of slidable tissue cutter **106** is that it allows for greater precision and ease of use than a hand-held scalpel and is less dependent upon the medical professional's skill and care.

(d) Guided Tissue Dilator

[00187] FIGS. 44-46 illustrate an example of a guided slidable tissue dilator **220** which can be used in a vessel closure system **100** in certain embodiments. Tissue dilator **220** can be configured to dilate the tissue tract before the deployment instrument **104** and can be moved through the opening in the skin. Tissue dilator **220** can be generally tube-shaped and configured to snap onto and off of the existing introducer sheath. Dilating the tissue before the advancement of deployment instrument **104** creates a temporary pathway through the tissue, making it easier to advance the deployment instrument **104** forward to the vessel wall **16**. After dilating the tissue tract, the tissue dilator **220** is then slid backwards and removed from around the introducer sheath.

[00188] Tissue dilator **220** can include an elongate tubular portion **223** with a channel **222**. Tubular portion **223** can include a tapered distal end **226** to facilitate insertion of tissue dilator **220** through the percutaneous opening **12**. Tissue dilator **220** can include a base **221** with handle portions **224** extending beyond the end of channel **222**. As illustrated, surfaces of handles **224** can be positioned in a plane generally parallel to a longitudinal axis of tubular portion **223**. In other embodiments, handles **224** can be positioned at an appropriate angle, such as, for example, an angle of at least approximately 90 degree angle. Angled handles can advantageously provide a surface to push on that is perpendicular to the direction of applied force. As with the cutter **106**, ends **228** of base **221** can act as mechanical stops to limit the depth of insertion. The medical professional can advance tissue dilator **220** until its distal end **226** encounters the resistance of the vessel wall **16**. As with the cutter **106**, channel **222** can have a partial circumferential cross-sectional geometry enabling it to "snap on" to an introducer sheath or other medical device. In other embodiments, a tissue dilator can use two mating pieces that clamp or snap together to facilitate temporary attachment and removal. In

the illustrated embodiment, tubular section **221** includes a distal section **230** and a proximal section **232**. Distal section **230** has a greater partial-circumferential cross-section than proximal section **232**. In other embodiments, tubular section **221** can be substantially uniform along its length. Tissue dilator **220** can be made from materials and methods similar to those described above with reference to tissue cutter **106**.

(e) **Heated Systems**

[00189] Heat can be used with any of the vascular closure clips described above, such as, for example clip **102**. A power source **502** such as an RF power source is provided. Other suitable power sources such as a DC power source can be used. Power source **502** is connected to a resistive element **508** via conductors **504** and **506**. Clip **102** can function as the circuit's resistive element **508**. In certain embodiments, only a portion of clip **102** will function as the resistive element. Clip **102** can be treated to increase its resistance value by, for example, being covered with a resistive coating. An increased resistance can reduce the power level necessary to effectuate a given amount of heating. In certain embodiments, portions of the clip **102** are covered with a thermally and/or electrically insulative coating. The remaining, uncovered portions of clip **102** can be configured to transfer thermal energy to the tissue being heated. In certain embodiments, only the tines or a distal portion of the tines are configured to transfer the thermal energy to the tissue. Conductors **504** and **506** can include wires made from a suitable electrically-conductive material such as copper-clad steel. In certain embodiments, conductors **504** and **506** can also function as tethering elements to allow removal of clip **102**. Conductors **504** and **506** can be covered with an insulating cover or coating. A thermocouple **512** can be mounted to the clip to monitor the temperature of the clip and/or the surrounding tissue. The recorded temperature can be provided to a user display **510** and/or controller **514**. Controller **514** permits the medical professional to adjust the amount of power delivered to the resistive element **508**. In certain embodiments, the power delivered can be less than about 2 W, between about 2 and about 50 W, or greater than 50 W. In certain embodiments, the power delivered can be about 2 W, 3 W, 4 W, 5 W, 6 W, 7 W, 8 W, 9 W, 10 W, 11 W, 12 W, 13 W, 14 W, 15 W, 16 W, 17 W, 18 W, 19 W, 20 W, 21 W, 22 W, 23 W, 24 W, 25 W, 26 W, 27 W, 28 W, 29 W, 30 W, 31 W, 32 W, 33 W, 34 W, 35 W, 36 W, 37 W, 38 W, 39 W, 40 W, 41 W, 42 W, 43 W, 44 W, 45 W, 46 W, 47 W, 48 W, 49 W, or 50 W or any wattage therebetween. Other suitable wattages may also be used. The medical professional can maintain the tissue at the desired temperature for a certain length of time. In some embodiments, heat can be applied to the tissue for a period less than or equal to about 30 seconds, or greater than 30 seconds. Other suitable times may also be used.

[00190] Following the application of heat, the conductors **504**, **506** can be disconnected from clip **102** in many ways. For example, a twisting, cutting, or other manipulative action can be used to remove the conductors. In embodiments using temporary or removable clips, conductors **504**, **506** can be used as a primary or backup tethering element to remove the clip **102** following hemostasis. In certain embodiments, conductors **504**, **506** can be connected to the clip **102** via spot welding,

mechanical fit, soldering, combination, or other suitable method. Conductors **504**, **506** can be fabricated from many different materials, such as copper, platinum, stainless steel, or a composite of materials (e.g. copper clad steel or platinum and silver combined by a drawn filled tubing process). In certain embodiments, conductors **504**, **506** can include composite signal wires using silver as the inner core to better transmit, for example, radiofrequency or direct current energy. Conductors **504**, **506** can be fabricated with a circular, elliptical, rectangular (flat), or other geometry which may depend on the space available on the clip **102**. Conductors **504**, **506** can be covered or jacketed with an insulative material such as polyimide, polyamide, polyurethane, polyester, nylon, or other suitable material.

[00191] In certain embodiments, a special tip can be placed over a standard electrosurgical tool such as, e.g., a Bovie Instrument (i.e., digital electrosurgical generator and accessories by Bovie Medical Corporation), to insert through the skin and make contact with the closure device and/or tissue. In certain embodiments, alternative heating means can be provided to heat the clip and/or the adjacent tissues including, for example, ultrasound energy, microwave energy, etc.

[00192] **FIG. 53** illustrates a circuit using ohmic tissue heating to heat tissue. A power source **502** such as a radiofrequency (RF) or direct current (DC) power source is provided. Power source **502** is connected to an active electrode **524** via conductor **526**. Clip **102** can function as the active electrode **524**. Alternatively, only a portion of clip **102** can function as the active electrode **524**. For example, in certain embodiments, one or more of the clip's tines or only a portion of the clip's tines such as the distal-most portion can function as the active electrode **524**. In certain embodiments, remaining portions of the clip **524** are covered with an electrically insulating cover or coating. A second conductor **528** connects power source **502** to an indifferent electrode **522**. The indifferent electrode **522** can be, for example, an electrode plate or large surface area indifferent ground pad applied to the patient's skin. The indifferent electrode **522** can be placed on the patient's back, thigh or other location. The indifferent electrode **522** can be applied to a portion of the patient's skin generally opposite the percutaneous opening. The power supply **502** applies a voltage differential across the active and indifferent electrodes **524**, **522** causing current to flow through the intervening tissue thus heating the tissue. The heat is generally concentrated at tissue adjacent to the active electrode **524**. Controller **514** can permit the medical professional to adjust the amount of power delivered.

[00193] In another embodiment (not shown), a first portion of the clip can act as a first electrode and a second portion of the clip can act as a second electrode. The first and second portions of the clip can be electrically insulated from one another. For example, a first finger or a portion of the first finger such as one or more tines can act as the first electrode and a second finger or a portion of the second finger can act as the second electrode. A power source applies a voltage differential across the first and second electrodes causing current to flow between them and heat intervening tissue.

[00194] An electrode-enabled closure device can also be used to confirm contact between the closure device and the tissue surface, such as by comparing the impedance between an electrode element and a return path (indifferent electrode or second electrode). When an electrode surface contacts only or primarily blood, the measured impedance can be substantially higher than when a small or substantial portion of the electrode surface contacts tissue.

[00195] FIGS. 54-55 show another embodiment of an inner tubular member 154' which can form one component of a deployment instrument. Inner tubular member 154' can be similar to inner tubular member 154 described above. A primary difference between inner tubular member 154' and inner tubular member 154 is the inclusion of recessed portions 550 on handle 164'. Connecting channels 552 can be relatively thin and can permit access from an exterior surface of handle 164' to an interior of recessed portions 550. Recessed portions 550 can receive the proximal ends of suture lines 234. For example, the proximal ends of suture lines 234 can be tied to or looped around portions 554 of handle 164'. A removable clip can be implanted using the procedure described above. Prior to removal of the deployment instrument, the suture lines 234 can be removed from portions 554 of handle 164'. Following hemostasis, the proximal ends of the suture lines 234 can be grasped to withdraw the clip from the vessel and out of the patient.

II. METHODS OF USING AND DEPLOYING CLIPS AND/OR PLUGS

[00196] In certain embodiments, the distal end of inner tubular member can have at least one section with a larger circumferential diameter or flare to cause clip tines to deflect outward (during forward movement during deployment), capturing more tissue (than without the increased diameter section) as the clip is advanced forward, for greater tissue compression and sealing. The distal end of the inner tubular member can also have a non circumferential enlargement such as at least one bump or raised surface arranged around the circumference. This design can be used to cause only some of the clip tines to be opened or deflected outward during advancement and deployment, or some to deflect more than others.

[00197] In certain embodiments, the deployment instrument can be configured so that the clip is deployed by advancing the outer tubular member distally relative to the inner tubular member instead of by proximally withdrawing the inner tubular member. The pressure element or other pressure sensing means can be secured to the inner tubular member, such as for example at a proximal end of the inner tubular member.

[00198] In certain embodiments, suction can be used to temporarily attach the deployment instrument to the vessel wall, and/or to confirm contact with the desired tissue. The deployment instrument can be configured to enable local and/or remote suction. In certain embodiments, an elongate suction tube or lumen can be secured to and/or located within the deployment instrument. The suction tube can include an opening on or near the distal end of the deployment instrument, and a valve or fitting (such as, for example, a Luer fitting) on the side or proximal end of the tool, to which a syringe, bulb, or other suction device could be attached and/or integrally formed. In certain

embodiments, local suction can be accomplished without attachment to an external vacuum source. Local suction can be accomplished, for example, using a syringe or other physician manipulated device to pull a vacuum, creating the desired suction. A Luer-lock or stopcock then can be used to close the suction tube or lumen containing the vacuum to maintain a suction condition. In certain embodiments, a remote vacuum suction system can be attached to a vacuum line. The vacuum system can include a means for limiting the amount of vacuum/suction which can be created in order to prevent trauma to the tissue adjacent to the distal suction port.

[00199] The slidable tissue cutter can be adapted to use heat to cut skin and or other tissue by making the leading edge an electrode and attaching at least one electrical conductor to the electrode. Direct resistive element heating or ohmic tissue heating can be used. Biocompatible materials (e.g., gold, platinum, platinum/iridium, stainless steel, nitinol and other suitable materials) can be used for the electrode and connected to a suitable (e.g., electrical and biocompatible) conductor. For ohmic tissue heating, one conductor can be connected to an RF power source. Another conductor is connected to a ground pad placed on the patient's body, and also connected to the power source. For direct resistive element heating, both conductors from the power source are connected to an electrode.

[00200] In certain embodiments, the cutting elements of slidable tissue cutter can be designed to cut tissue or to both cut and remove tissue. In some cut-and-remove embodiments, the cutting element can be circular, diagonal, angled, or other blade. The slidable tissue cutter can be designed and used to cut any body tissue including, but not limited to, skin, fat ligaments, cartilage, bone, or vessels. The cutting element can be of any desirable type, including thermal (laser, RF, etc.), chemical, ultrasonic, combination, or other.

[00201] An example of a method for using deployment instrument **104** and clip **102** will now be described. **FIG. 18** illustrates a deployment instrument **104** in an initial configuration loaded onto a vascular introducer **108** that has been inserted into a patient's blood vessel **18**. The deployment instrument **104** can also be configured for use with other medical devices such as, for example, tubular or elongate dilators, trocars, endoscopes, catheters, guide wires, needles, tubes, sheaths, combination or other. The tubular medical device **108** is first inserted through the inner diameter of the deployment instrument **104** which has been loaded with clip **102**. The tubular medical device **108** can then be inserted through the skin and into the desired vessel **18** using any of a number of known methods, such as, for example, the Seldinger method. The desired interventional or diagnostic procedure is then performed. The deployment instrument **104** can be temporarily moved to the side as illustrated so as not to interfere with the medical procedure. For example, the deployment instrument **104** can be moved toward the back or proximal end of the introducer sheath **108** as shown in **FIG. 18**. Slots **162** and **170** (see **FIGS. 7** and **12**) facilitate this positioning.

[00202] With reference to **FIGS. 19-20**, deployment instrument **104** is advanced forward along the introducer sheath through the percutaneous opening **12** until the distal end **105** of the deployment instrument **104** contacts the vessel wall **16**. At this state along the pressure sensitive structure on the

outside of outer tubular member **156**, pressure element **158** is in its initial, non-advanced configuration as shown in **FIG. 20**. In certain embodiments, a dilator that was previously removed or a new dilator or other elongate member can be inserted into the inner lumen of the vascular introducer **108** to provide mechanical support and resistance to kinking of the introducer **108**. Reinsertion of the dilator may thus facilitate the advancement of deployment instrument **104** over the introducer **108**.

[00203] With reference to **FIGS. 21-22**, pressure element **158** is then manually advanced distally until it reaches stop **182**, indicating to the medical professional that appropriate force is being applied between the deployment instrument **104** and the vessel wall **16** to begin deployment. **FIG. 22** is a close up view of the pressure element **158** in its fully advanced configuration. As the pressure element **158** is advanced distally, flexible tabs **188** are subjected to greater flexion as they advance up pressure tapers **178**. Thus, advancing the pressure element **158** can require an increasing amount of applied force. Pressure tapers **178** generally flare outward until reaching flat surfaces **180**. Stop **182** generally prevents pressure element **158** from advancing distally beyond this point. The amount of applied force required to fully advance the pressure element **158** can be adjusted by altering one or more of the number, size, width and rigidity of tabs **188**, the angle of incline of pressure tapers **178** and the height of surfaces **180**. In certain embodiments, the deployment instrument **104** can require at least about 10 ounces of force to safely begin deployment of the clip **102**. Thus, in certain embodiments, pressure element **158** can require at least about 10 ounces of force to be fully advanced. In other embodiments, the deployment instrument **104** can require between about 3 ounces of force and about 64 ounces of force to safely begin deployment of the clip **102**. In some embodiments, less than about 3 ounces of force is required. In other embodiments, the deployment instrument **104** can require about 3 ounces of force, about 4 ounces of force, 5 ounces of force, about 6 ounces of force, about 7 ounces of force, about 8 ounces of force, about 9 ounces of force, about 10 ounces of force, about 11 ounces of force, about 12 ounces of force, about 13 ounces of force, about 14 ounces of force, about 15 ounces of force, about 16 ounces of force, about 17 ounces of force, about 18 ounces of force, about 19 ounces of force, about 20 ounces of force, about 21 ounces of force, about 22 ounces of force, about 23 ounces of force, about 24 ounces of force, about 25 ounces of force, about 26 ounces of force, about 27 ounces of force, about 28 ounces of force, about 29 ounces of force, about 30 ounces of force, about 31 ounces of force, about 32 ounces of force, about 33 ounces of force, about 34 ounces of force, about 35 ounces of force, about 36 ounces of force, about 37 ounces of force, about 38 ounces of force, about 39 ounces of force, about 40 ounces of force, about 41 ounces of force, about 42 ounces of force, about 43 ounces of force, about 44 ounces of force, about 45 ounces of force, about 46 ounces of force, about 47 ounces of force, about 48 ounces of force, about 49 ounces of force, about 50 ounces of force, about 51 ounces of force, about 52 ounces of force, about 53 ounces of force, about 54 ounces of force, about 55 ounces of force, about 56 ounces of force, about 57 ounces of force, about 58 ounces of force, about 59 ounces of force, about 60 ounces of force, about 61 ounces of force, about 62 ounces of force, about 63 ounces of force, or

about 64 ounces of force, or any value up to about 100 ounces, or any value therein, measured to a value of about 100th of an ounce, to safely begin deployment of the clip **102**. In certain embodiments, the deployment instrument can be configured to make an audible "click" or otherwise produce an audio, visual, or tactile signal when the pressure element **158** has fully advanced.

[00204] In some embodiments, other pressure-sensitive structures such as a pressure or force gauge can be used to verify that adequate pressure is applied. The deployment instrument can use a spring in place of, or in addition to, a taper element. A first end of the spring can be secured to a slidable element. A second end can be attached to a distal point on the outer tubular member. The slidable element can be used to compress the spring, thus applying force to the outer tubular member. A combination or other means to confirm sufficient contact and pressure between the deployment instrument and vessel can also be included. In certain embodiments, the deployment instrument can include a grasping tool configured to assist in securing the distal end of the deployment instrument to the vessel. In certain embodiments, the medical professional can observe a backflow of blood through a channel or window in the deployment instrument following removal of the tubular medical device to confirm proper placement on the vessel. Blood can be configured to flow through the central channel of the deployment instrument. In certain embodiments, a clear channel or clear tubular section **640** can be provided to receive blood flow. One or more sensors can be provided to verify proper placement and/or pressure.

[00205] **FIG. 23** shows the deployment instrument **104** with clip **102** in a partially-deployed configuration. In a partially-deployed state, tines **126a**, **126b** can pierce the vessel wall **16** and the clip **102** remains attached to the deployment instrument **104** in a substantially open configuration. The medical professional partially deploys the clip **102** by beginning to withdraw inner tubular member **154**. The medical professional can maintain adequate pressure on pressure element **158** (e.g. pressure sufficient to maintain pressure element **158** in its fully advanced configuration) while withdrawing inner tubular member **154**. Handle **164** can be used to withdraw the inner tubular member **154**. For example, the medical professional can apply distally-directed pressure to the pressure element **158** with one hand while partially withdrawing handle **164** with the remaining hand. The ledge or countersink **174** on outer tubular member **156** prevents clip **102** from being withdrawn along with the inner tubular member **154**. Thus, as the inner tubular member **154** is withdrawn, the tines **126a,b** begin to extend beyond the distal end **165** of inner tubular member **154**. The continued application of pressure on pressure element **158** (and thus outer tubular member **156**) generally forces the tines **126a,b** to pierce the vessel wall **16**. In certain embodiments, the pressure element **158** can include a means to prevent inner tubular member **154** from being withdrawn unless and until pressure element **158** is fully advanced.

[00206] **FIGS. 24-29** illustrate an example of a method of producing partial deployment. **FIG. 24** shows a perspective view of the deployment instrument **104** in a partially-deployed state, and **FIG. 25** shows a close-up view of the distal end **105** of the deployment instrument **104** in its partially-

deployed state. Handle **164** can be withdrawn until the proximal face **167** of handle **164** contacts the stops **175**, generally arresting further withdrawal as shown in **FIGS. 26** and **27**. Stops **175** generally prevent the medical professional from fully deploying the clip prematurely and ensure the clip **102** is partially deployed to an appropriate depth. Stop **175** is configured to allow the handle **164** to travel a known, limited distance **179**. In embodiments where the tips **127a,b** of tines **126a,b** are initially aligned with distal end **165** of inner tubular member **154**, distance **179** can correspond to a depth of the tines' insertion into the vessel wall **16**. In certain embodiments, distance **179** can be greater than or equal to about 0.5 mm and/or less than or equal to about 4 mm. In certain embodiments, distance **179** can be about 0.5 mm, 0.6 mm, 0.7 mm, 0.8 mm, 0.9 mm, 1.0 mm, 1.1 mm, 1.2 mm, 1.3 mm, 1.4 mm, 1.5 mm, 1.6 mm, 1.7 mm, 1.8 mm, 1.9 mm, 2.0 mm, 2.1 mm, 2.2 mm, 2.3 mm, 2.4 mm, 2.5 mm, 2.6 mm, 2.7 mm, 2.8 mm, 2.9 mm, 3.0 mm, 3.1 mm, 3.2 mm, 3.3 mm, 3.4 mm, 3.5 mm, 3.6 mm, 3.7 mm, 3.8 mm, 3.9 mm, or 4.0 mm or any size therein to about the 100th of a mm. In certain embodiments, distance **179** can be about 2 mm. Other suitable distances can also be used. Distance **179** can be different depending on the specific application or clip being used.

[00207] With the clip **102** partially deployed in the vessel wall **16**, the tubular medical device **108** is no longer needed to guide the deployment instrument **104** to the arteriotomy and hence the tubular medical device **108** can then be removed from the vessel **18** as shown in **FIG. 28**. Removing the tubular medical device **108** prior to full deployment prevents the clip **102** from closing over the tubular medical device **108**. Partially deploying the clip **102** helps to position the deployment instrument **104** more accurately and temporarily secure it in place while the tubular medical device **108** is removed.

[00208] Once the tubular medical device **108** is removed from the vessel, the stops **175** can be overcome by bending tab **172** in the direction of the arrow **189** shown in **FIG. 29** to allow full linear movement of the inner tubular member **154**. Tab **172** can thus operate as a releasing element, permitting the stops **175** to be overcome. Recessed or weakened portion **186** of tab **172** may facilitate bending. The flattened bottom portion and angled faces **352** of handle **164** can reduce the amount that tab **172** is required to bend in order to overcome stops **175**. In some embodiments where deployment instrument **104** is disposable and configured for one-time use, tab **175** may be configured to snap off. Other appropriate stop means and methods for overcoming the stop means can be used.

[00209] With reference to **FIGS. 30-31**, the medical professional then continues to withdraw inner tubular member **154** until the clip **102** is forced off of or advanced past the distal end **105** of the deployment instrument **104**. The opposed fingers **122**, **124** of the clip **102** fold inwardly, drawing together sides of the vessel tissue from an outside surface of the vessel to close the arteriotomy **14** as shown in **FIG. 31**. Closing the arteriotomy can, but does not necessarily, result in complete mechanical closure of the opening. Instead, the term "close" in this context can refer to any facilitation of hemostasis. Thus, in certain embodiments, sides of the vessel tissue may not

necessarily touch. Generally, the sides of the vessel tissue are brought closer together to reduce the size of the opening **14** in the vessel **18** and thereby facilitate hemostasis.

[00210] FIG. 32 shows the deployment instrument **104** being withdrawn following successful deployment of the clip **102**. Clip **102** can be biocompatible and configured for permanent implantation. Accordingly, in certain embodiments a patient may be discharged following confirmation of successful clip deployment and hemostasis.

[00211] In some embodiments, vascular closure system **100** can be completely or substantially extravascular in that the deployment instrument or closure device is not required to penetrate into the interior region of blood vessel **18**. This can reduce or eliminate the amount of foreign material introduced into contact with the patient's blood stream, thus reducing the risk of infection, blockage, or other complications. For example, in certain embodiments a posterior support is not required during deployment of the clip. In some systems, the use of posterior support may disadvantageously require that a portion of the deployment tool or closure device be positioned in the blood vessel during or following deployment. The use of a posterior support element within the vessel may require complicated mechanisms to facilitate its removal following deployment. The safe deployment of the clip without requiring posterior support can be facilitated through use of a partial deployment technique as described above and by the application of a controlled amount of external pressure via a pressure element or other pressure sensing means. In addition, the use of a clip with appropriately-sized tines to prevent over-insertion can also facilitate deployment without posterior support.

[00212] The system **100** described above can also be compatible with standard commercially available introducers already used in standard vascular interventional or diagnostic procedures. This can eliminate the need to purchase and use specialized and costly additional or different equipment or to change the way that the interventional or diagnostic procedures are performed, thus reducing the accompanying risks.

[00213] FIGS. 33-35 illustrate an example of a method of temporarily implanting a clip **102**. In certain embodiments, a vessel closure clip **102** can be removable and configured for temporary implantation as illustrated in FIG. 33. In embodiments using temporary closure, one or more suture lines **234** or other suitable tethering means can be secured to the clip **102** and positioned along the outer surface of the outer tubular member **156** prior to insertion. The suture lines **234** can be tied to the clip **102** or looped through window portions **125** or other openings provided on the clip **102** for this purpose or attached in some other way. In certain embodiments, the clip **102** and deployment instrument **104** may be provided to the medical professional with suture lines **234** attached. In other embodiments, suture lines **234** may be attached by the medical professional prior to use. Slots **176** on the distal end **173** of outer tubular member **156** (see FIG. 8) can facilitate access to the clip **102** for the purposes of securing the suture lines **234** to the clip **102** after it is loaded onto the deployment instrument **104**. The distal ends of axial grooves **160** on inner tubular member **154** can allow the suture lines to be passed under base portion **120**. In certain embodiments, the suture lines **234** can be

tied or secured to the clip before it is loaded on the deployment instrument **104**. The suture lines **234** can run along the outer surface of outer tubular member **156** as shown in **FIG. 33**. In other embodiments, the suture lines **234** can run along an interior of the deployment instrument **104**. In certain embodiments, the deployment instrument **104** can include channels specifically adapted to accommodate suture lines **234**.

[00214] The removable clip **102** can be temporarily implanted using the procedure outlined above. The proximal ends of the suture lines **234** can be left extending outside of the patient's body while the clip **102** remains implanted. After a period of time sufficient to achieve hemostasis, the medical professional can pull on the suture lines **234** to remove the clip as seen in **FIG. 35**. The closure force of the clip can be configured so that force applied to the suture lines **234** causes the fingers **122**, **124** to temporarily open, allowing the clip **102** to be safely removed without reopening the arteriotomy **14** or damaging the vessel wall **16**. In certain embodiments, the clip **102** can include another or alternative release mechanism that can be triggered via the suture lines **234**. The release mechanism can cause the fingers **122**, **124** to open to facilitate removal of the clip **102**. In embodiments using a shape memory clip, the clip can be cooled until it transforms to its martensite phase, making it more easily deformed and lowering the amount of force required to open the clip's fingers and withdraw it. The clip **102** can be cooled via insertion of a cold probe or via application of an externally-applied cold source such as an ice pack. In addition or in the alternative, an infusing syringe can be used to deliver a cooled liquid such as chilled saline to the clip. In certain embodiments, the clip **102** can exhibit a two-way shape memory effect and cooling the clip **102** can return it to its second memorized configuration which can be, for example, an open configuration. The clip's composition and treatment can be selected to achieve desired phase transition temperatures to facilitate such an approach.

[00215] The time required to achieve hemostasis can vary from patient to patient depending on a variety of factors including the patient's age, sex, medical condition, medications, and the presence of anti-clotting agents that can have been used during the medical procedure. Under certain conditions, clip **102** can be removed after about 10 minutes, after about 15 minutes, after about 20 minutes, after about 25 minutes, after about 30 minutes, after about 35 minutes, after about 40 minutes, after about 45 minutes, after about 50 minutes, after about 55 minutes, or after about 60 minutes or any suitable time therein measured to about 100th of a second. In some embodiments, clip **102** can be removed after about 1 h or more. Other suitable times can also be used.

[00216] In some embodiments, it can be desirable to use suture lines **234** even in clips intended for permanent implantation in order to enable emergency removal. In this arrangement, the medical professional can deploy the clip using the procedure described above. Once it is determined that the clip has been successfully deployed, the medical professional can cut the suture lines **234** and completely withdraw them from around the clip.

[00217] This disclosure has provided certain examples of closure devices including clips and plugs. However, other types of closure devices can be used. In certain embodiments, a closure device can be smaller in an initial configuration or in a deployed configuration. In certain embodiments, the closure device can close a tissue opening by bringing closer together sides of the tissue opening and/or by partially or completely occluding the opening. The closure device can be partially or completely made from one or more of a polymer, rubber, silicone, metal, metal alloy, superelastic / shape memory polymers and metallic alloys, or other suitable material or materials.

[00218] In some embodiments, the closure device may be partially or completely fabricated from a biodegradable/bioabsorbable material, including but not limited to one or more of starch, modified cellulose, collagen, fibrin, fibrinogen, fibronectin, elastin, vitronectin, laminin, thrombin, albumin and gelatin or other connective proteins or natural materials, polymers or copolymers such as polyvinyl pyrrolidone, polylactide [poly-L-lactide (PLLA), poly-D-lactide (PDLA)], polyglycolide, polydioxanone, polycaprolactone, polygluconate, polylactic acid (PLA), polylactic acid-polyethylene oxide copolymers, poly(hydroxybutyrate), polyanhydride, polyphosphoester, poly(amino acids), poly(alpha-hydroxy acid) poly d,l-lactic acid (PLA) and copolymers of lactic acid and glycolic acid (PLGA), or related copolymers of these materials as well as composites and combinations thereof and combinations of other biodegradable/bioabsorbable materials. In some embodiments, the closure device can be partially or completely fabricated from a biocompatible material, such as expanded polytetrafluoroethylene (ePTFE), polyester, polyurethane, silicone, rubber, Dacron, and/or urethane.

[00219] In some embodiments, the closure device can include one or more coatings and/or be partially or completely formed from one or more of the following: swellable materials, bioabsorbable materials, and biocompatible materials.

[00220] In some embodiments, the closure device can have a biocompatible contact surface such as adhesives, bonding compounds, or other solutions, including those intended to delay swelling or expansion of at least one section of the closure device once it comes in contact with a fluid. The biocompatible contact surface can be located on any surface or all surfaces of the closure device. The contact surface can be applied or integrated into the device in many ways, such as during the manufacturing process, just prior to deployment, or after the device has been deployed. The bonding materials can be in the form of a liquid, semi solid, or solid. Suitable bonding materials can include gels, foams and microporous mesh. Suitable adhesives can include acrylates, cyanoacrylates, epoxies, fibrin-based adhesives, other biological based adhesives, UV light and/or heat activated or other specialized adhesives. The contact surface can bond on initial contact, or after a longer period of time to allow repositioning of the closure device if desired. Such a contact surface can include a crystalline polymer that changes from a non-tacky crystalline state to an adhesive gel state, such as when the temperature is raised from room temperature to body temperature. An example of such material is available under the trade name Intillemer™ adhesive, available from Landec Corp., as well as composites and combinations thereof and combinations of other materials. Suppliers of

biocompatible adhesives include, but are not limited to, Plasto (Dijon, France), Haemacure (Montreal, Canada), Cohesion (Palo Alto, Calif.), Cryolife (Kennesaw, Ga.), TissueLink (Dover, N.H.), and others. To increase the work time of the contact surface and/or to allow repositioning of the closure device after it has been deployed, the contact surface can be blended with a material such as a starch or other material, that retards or delays bonding to allow repositioning of the device after it has been deployed. A degradable coating can be placed over the contact surface so that it degrades and exposes the adhesive. Other contact surfaces can include composites-based adherents and combinations of the above materials and other suitable materials as are known in the art.

[00221] The closure devices, systems, and methods can be used for any suitable cardiovascular, gastrointestinal, neurological, reproductive, lymphatic, respiratory, orthopedic, combination or other applications where partial or complete, temporary, removable, or permanent closure, compression, sealing, bringing together, cinching, anchoring, and/or reinforcement, tissue modification, stabilization, tissue access, tissue reforming, tissue connection (e.g., to other tissue or between tissue and a medical device), and/or tissue resizing is desired. Additionally, the closure devices, systems, and methods can be used in connection with any lumen, duct, organ, hollow body organ or cavity, or other bodily structures or tissues, where partial or complete, temporary, removable, or permanent sealing, crimping, compression, plugging, reinforcement or other purpose is desired. For example, some applications include, but are not limited to, the following: cerebral aneurysm treatment, shortening the chordae tendinae to treat mitral valve prolapse, reversible or permanent sterilization for women by occluding the fallopian tubes, and for men by occluding the vas ducts or tubes, closure of septal (or other) defects in the heart or anywhere else in the body, patent foramen ovale (PFO) closure, post-biopsy tissue closure, tissue closure following minimally invasive surgical or transluminal procedures, general tissue ligation, and localized therapeutic elution. Other applications include closing an access puncture of the heart following a diagnostic or interventional procedure, such as, for example, minimally invasive, percutaneous heart valve reinforcement or replacement procedures using devices and systems such as those from Edwards Lifesciences (Irvine, CA).

[00222] A tissue closure system can enable the advancement / deployment of the sealing element over and/or alongside other than tubular medical devices, including tools used during medical procedure such as, for example, hemostats, cutters, tweezers, probes, biopsy devices, etc. A deployment instrument and/or sealing element can be configured to be advanced over and/or alongside additional medical devices, such as, for example, needles, hypo tubes, guide wires, electrode wires, intravenous (IV) tubes, vascular introducers, catheters, laparoscopes, endoscopes, trocars, cannulas, combination or other suitable medical devices. The disclosed systems can be packaged on or with the medical devices or tools. A deployment instrument and/or sealing element can be configured to work with medical devices of all sizes, including devices having an outer diameter of less than or equal to about 6 French, greater than or equal to about 20 French, and all sizes

in between. In some embodiments, a deployment instrument and/or sealing element can be configured to work with medical devices having an outer diameter of about 6 French, 7 French, 8 French, 9 French, 10 French, 11 French, 12 French, 13 French, 14 French, 15 French, 16 French, 17 French, 18 French, 19 French or 20 French. Other suitable sizes may also be used.

[00223] In certain embodiments, a tissue closure system can be configured to operate as a stand-alone surgical system. For example, in certain embodiments a tissue closure system can be configured to operate without being advanced over or alongside or otherwise being guided by an elongate medical device.

[00224] A deployed element can be used as a temporary or permanent spacer, shim, or to displace and/or support, stabilize, reinforce, or occlude any tissue or tissues, including bone. The deployed element can be partially or completely made from many different types of materials, including, for example, a polymer, sponge, metal, metal alloy, superelastic / shape memory materials (including polymers and metallic alloys), or any other suitable material or materials. The deployed element can be deployed through a tube with a pusher element, e.g., a stylet, plunger, inner tubular member or rod, and allowed to expand before, during and/or after deployment. The deployment element can be biased in an expanded configuration. The deployed element can be maintained in a compressed configuration during positioning of the element, and allowed to expand to an expanded configuration when no longer constrained. In general, the closure device may be constrained in a smaller cross section profile, and allowed to self-expand once a constraining force is removed. In addition, the closure device may be constrained in an open position, and allowed to self-close once the opening force is removed.

[00225] The general components and/or disclosed systems, with desired modifications, can be used to temporarily or permanently close, and/or reinforce tissue access for medical procedures such as minimally invasive biopsy, other tissue removal, or diagnostic or therapeutic procedures including locations on, through, or inside the heart, locations for procedures including electrophysiology, congestive heart failure, valve related treatment (including, for example, dilation, valve reinforcement, replacement, papillary muscle treatment, chordae tendineae, and other related structures, combination and or other purposes) and/or any other locations on organs or tissue, including skin.

[00226] The systems of the present invention can facilitate less invasive surgery involving thorascopic access and visualization to the target location. In some embodiments, the systems of the invention can be suitable for use through a median sternotomy, lateral thoracotomy, intercostals port-access, mini-sternotomies, other less invasive approaches involving xiphoid access, inguinal approaches, or sub-thoracic approaches adjacent the diaphragm. In other embodiments, the systems of the present invention can be configured for catheter-based applications by elongating the shaft and altering the diameters and other feature dimensions for intravascular access.

[00227] The systems of the present invention are capable of being deployed through a thoracostomy, thoracotomy, median sternotomy, mini-sternotomy, mini-thoracotomy, xiphoid access,

subthoracic access, arthroscopic, or laparoscopic approach, thereby potentially eliminating the need for long incisions to access the soft tissue and corresponding anatomic structures.

[00228] The closure devices, systems and methods can be used for temporary or permanent tissue reshaping, reforming and/or resizing. Tissues which can be reshaped and/or resized include organs, such as the stomach, lungs, etc., and other structures, such as the esophagus and structures of the heart and/or valves. For example, in certain embodiments one or more clips may alone be sufficient to reshape, reform and/or resize tissue by one or more of accessing, gathering, pursing, bunching, cinching or holding tissue. In other embodiments, multiple clips can be connected together by a suitable tether, e.g., static or elastic, from the outer or inner surface of a tissue structure or organ. In certain embodiments, the tether can be tightened following implantation of the clips to achieve additional resizing, reforming and/or reshaping of tissue. In certain embodiments, one or more clips and/or a suitable tether can be used to resize and/or reinforce the Lower Esophageal Sphincter (LES) for gastrointestinal uses, or to resize the tissue around a heart valve.

[00229] The disclosed clips and/or delivery systems can also be configured to anchor implanted stent grafts by securing the graft to the tissue wall to prevent the graft from moving. For example, stent grafts (such as those devices and systems from W.L. Gore, Cook, Medtronic, etc.) can be used to treat an abdominal aortic aneurysm by reinforcing the aortic wall to prevent rupture. One or more clips can be deployed on the inside of the stent graft and/or on the outside of the abdominal aorta, and may be in contact with the graft and/or act to limit potential graft movement. The disclosed devices, systems and methods relating to anchoring or attachment of stent grafts, endoprosthesis, or other structures or devices, can also be used for any other locations on or inside the body.

[00230] The general closure systems can be configured to be used with robotically or computer controlled medical procedures, including surgical systems such as those available from Intuitive Surgical, Inc. (Sunnyvale, CA), and catheter-based technologies from Stereotaxis (St. Louis, MO) and Hansen Medical (Mountain View, CA).

[00231] The closure systems can be used to close the vessel access in larger sized catheter-based percutaneous, transluminal procedures, including heart valve reinforcement / replacement procedures, such as those from CoreValve (Irvine, CA), Edwards Lifesciences (Irvine, CA), Sadra Medical Inc. (Campbell, CA), etc.

[00232] As shown in further detail in **FIGS. 90A-E** with respect to deployment of the plug device from the capsule **630** having a hemostatic design, the plug sits within a capsule **630** that is positioned between an introducer and a guide seal assembly as previously shown. Looking down the barrel of the capsule **630** from the distal end **80**, **FIG. 90B**, the walls of the capsule **630** can be seen with the positioned plug down within the aperture. A skirt area of the plug covers a bore and hemostatic pressure forces the skirt face to seal against the housing thus creating a seal which prevents leakage of fluid through the capsule **630** as shown in **FIGS. 90C-E**. In operation, the introducer is advanced to the site in vivo where the plug is to be deployed. A plunger is then advanced

in a distal direction through the plunger stem, capsule body **634** and introducer pushing the plug through the introducer to the site as shown in **FIG. 91A**.

[00233] To assist in controlling the direction of travel of the plunger grip, a locking split bushing can be incorporated in the design as shown in **FIGS. 91B-I**. The conical split bushing configuration has a conical taper on the stem and a split conical bushing which engages the conical taper and causes self-locking when backward (proximally directed) motion is attempted, but releases moving forward (distally directed). In another configuration, a canted disk which locks and releases can be used as shown in **FIGS. 91D-E**. As the disk tilts back and forth it either allows movement of the stem in a forward directed or locks the stem to prevent backward motion. Still another configuration is a ratchet configuration as shown in **FIGS. 91F-G** where the stem is notched and engages locking fingers which allow forward direction but prevent backward direction. Yet another configuration uses a silent ratchet as shown in **FIGS. 91H-I** where fingers are provided that dig into the stem.

[00234] As shown in **FIGS. 92A-T** the introducer is advanced into the vessel such that the tip of the introducer crosses the vessel wall and the distal end **80** of the introducer is positioned within the lumen of the vessel. As shown in **FIGS. 92A-B** the hemostasis valve is closed and keeps the sealing device in place within the capsule **630**. Once the introducer is positioned at a desired location crossing, for example, the vessel wall the plunger is inserted into the proximal opening of the capsule **630** at the introducer cap as shown in **FIGS. 92C-D**. As the plunger is advanced through the capsule **630**, the plunger tube comes into contact with the tether, a collet insert and the collet which places a slight drag on the plunger to allow forward motion but not backward motion. The collet can be configured from a helically wound braid or a biaxial braid which results in relaxation when the plunger is pushed through it but tightens to prevent backward motion when the plunger is retracted by reducing the radial distance between opposing sides and the overall circumference or a collar around the plunger such that it exerts a strong clamping force when it is tightened via a tapered outer collar, as shown here. The plunger and cartridge is then inserted into the proximal end **70** of the introducer as shown in **FIGS. 92E-F**. The combination is then advanced into the introducer and seated within the introducer as shown in **FIGS. 92G-H** and the hemostasis valve is in an opened configuration. From that point the plunger is advanced within the collet advancing the plug forward (still in the capsule **630**) as shown in **FIGS. 92I-J**. The plunger is then advanced further into the introducer pushing the plug into the inner lumen of the introducer device as shown in **FIGS. 92K-L**. At this point, the side wings of the plug are bent backwards so that the plug assumes a smaller cross-sectional profile configuration having an outer diameter less than the interior diameter of the introducer while advancing through the introducer device. As shown in **FIGS. 92M-N** the plug is now advanced approximately 80% through the introducer toward the distal end **80** of the introducer (which is positioned within the lumen of the vessel). The plug is then advanced beyond the distal end **80** of the introducer at which point the plug is no longer constrained and restores to its original profile with a diameter of the distal end **80** of the

plug being greater than the diameter of the introducer as shown in **FIGS. 92O-P**. Thereafter the introducer is withdrawn. As the introducer is withdrawn, the plug is pulled into a position wherein the stem of the plug traverses the vessel wall opening and the plug face conformably engages the interior of the vessel wall. Once the introducer exits the vessel, the proximal end **70** of the plug stem is observable from the exterior of the vessel and may, in some configurations, extend beyond the interior surface of the vessel wall as shown in **FIGS. 92Q-R**. Additional close up detail of the plug being positioned within the vessel is shown in **FIGS. 92S-T**. If a tether has been used the tether extends from the plug enabling the user to ensure that the stem of the plug is properly advanced through the opening of the vessel wall. The tether can then be removed, if desired. The plug is held securely in place by the interior fluid pressure forcing the inner distal surface of the plug against the interior vessel wall. This force proportionally increases with fluid pressure, improving the security of the plug. No other features are required to achieve hemostasis of the plug. The function of the stem is essentially three fold. First, it brings the inner vessel contacting element in contact with the inner wall of the vessel, creating a momentary hemostasis that is then self activated. Second, it acts as a centering element to center the vessel contacting about the puncture site (e.g., where the stem is positioned at a central point and not positioned off-center). Lastly, it prevents the plug from shifting away from the puncture site due to the force exerted by the blood flow through the vessel. A simple stem configuration can be as illustrated in **FIGS. 85A-B**.

III. METHODS OF MANUFACTURE

[00235] The deployment instrument **104** can be partially or completely made from one or more of the following materials: polymers, including Nylon, polyamide, polycarbonate (e.g., Makrolon®), acrylonitrile butadiene styrene (ABS), polyester, polyethyleneterephthalate (PET), polyetheretherketone (PEEK™), polyimide, superelastic / shape memory polymers and metals, including spring steel, stainless steel, shape memory metal alloys including nickel titanium alloys (Nitinol), 17-7 PH, cobalt-chromium-nickel alloy (Elgiloy®), and nickel based alloys with chromium and iron (Inconel®). Other suitable materials can be used. The deployment instrument **104** can be completely or partially fabricated using one or more of the following methods: casting, extrusion, laminating, machining, molding (injection or other), sintering, or stereo lithography. Other suitable methods can be used.

[00236] As illustrated, in certain embodiments, the deployment instrument **104** can be constructed using relatively few components, e.g., an inner tubular member, an outer tubular member, and a pressure element. Each of the components can be produced inexpensively via injection molding. In certain embodiments, the deployment instrument **104** can be disposable and designed for single use. Alternatively, the deployment instrument **104** can be designed for repeated use following sterilization.

[00237] In certain embodiments the advancement / deployment tool can contain more than one clip, with the ability to deploy one or more clips at a time, and can include an indexing or other

means to controllably deploy only one (or more) clips at a time. A multiple-clip embodiment can include at least two or more of the clips tethered together with a suitable tether. The tether can be elastic and/or able to be tensioned or otherwise configured to permit tissue between the two or more deployed clips to be pursed as the deployed clips are pulled (or drawn) towards one another. The tether can be permanently or temporarily tightened and secured at, for example, one or more ends of the tether to maintain the tension.

[00238] A method for loading the clip **102** onto the deployment instrument **104** will now be described with reference to **FIGS. 36-39**. A loading mechanism **240** can be used to facilitate loading the clip **102** onto the distal end **165** of inner tubular member **154**. Loading mechanism **240** includes a proximal section **244** which mates with the inner tubular member's inner lumen as seen in **FIG. 37**. Clip **102** is then advanced over tapered distal section **242** of loading mechanism **240**. Distal section **242** gradually forces apart the clip's fingers **122, 124** as shown in **FIG. 38**. The loading mechanism **240** can also include an intermediate section **245** with a substantially constant circumference which can be substantially equal to that of inner tubular member **154**. A pusher mechanism **249** can be used to advance the clip over the loading mechanism **240** and onto the deployment instrument **104**. Pusher mechanism **249** can include an end geometry configured to mate with the distal end of clip **102** as seen in **FIG. 39**. Once the clip **102** has been fully loaded onto the deployment instrument **104**, the pusher mechanism **249** and loading mechanism **240** can be removed. In embodiments using a superelastic or shape memory clip, the clip **102** can be cooled until it undergoes a martensite phase transformation in order to facilitate the clip's deformation. During its martensite phase, the clip **102** is more easily deformed and thus the fingers **122, 124** can be more readily spread apart in order to load the clip **102** onto the deployment instrument **104**. Such an approach can be used as an alternative to or in addition to the loading procedure described above.

[00239] Post device fabrication coating methods can include, but are not limited to, spin coating, RF-plasma polymerization, dipping, spraying, brushing, submerging the devices into a beaker containing a therapeutic solution while inside a vacuum chamber to permeate the device material, etc.

[00240] Alternatively, or in combination with the above therapeutic substances, one or more materials such as platinum, gold, tantalum, tin, tin-indium, zirconium, zirconium alloy, zirconium oxide, zirconium nitrate, phosphatidyl-choline, pyrolytic carbon, combination or other material, can be deposited onto the closure device surface using electroplating, sputtering vacuum evaporation, ion assisted beam deposition, vapor deposition, silver doping, boronation techniques, or other coating process.

[00241] Radiopaque material such as barium sulfate, bismuth trioxide, tantalum, platinum/iridium or other suitable materials can be added to any of the closure devices for enhanced visualization under a fluoroscope or other visualization means commonly used in a catheterization lab or surgical suite. Additionally, such materials can be added to the closure device by sputter coating, ion deposition, vapor deposition, combination, or other suitable processes.

[00242] In certain embodiments, the clip can be configured to be in its malleable martensite phase at room temperature. The clip can be loaded onto a deployment instrument in an open configuration. The clip can be configured to transition to an austenite phase by the application of heat during or after deployment. The application of heat can cause the clip to revert to its memorized, closed configuration. In certain embodiments, the clip can be configured to revert to its closed configuration upon being heated to a temperature near the temperature of the human body. In such embodiments, the clip can be delivered to the arteriotomy and partially deployed or held in place on the exterior of the vessel wall **16** for a period of time sufficient to heat the clip to its austenite transition temperature. In other embodiments, heat may be applied via insertion of a heated probe or remotely via application of focused electromagnetic energy.

[00243] The clip can include at least one (single element) hinge feature to assist with deployment, tissue engagement, compression and or removal from the tissue. The clip can be partially or completely made from one or more of the following materials: superelastic / shape memory polymers, metals including, spring steel and stainless steel, metal alloys including nitinol, 17-7 PH, Elgiloy®, and Inconel®. Other appropriate materials can also be used. In a preferred embodiment, the clip can be partially or completely made from a superelastic and/or shape memory material such as nitinol. A discussion of certain properties of superelastic and/or shape memory materials can be found in U.S. Patent No. **7,182,771**, the entirety of which is hereby incorporated by reference herein and made a part of the present specification. In certain embodiments, such as those using nitinol or other superelastic and/or shape memory materials, it can be desirable for the clip to have a relatively tight bend in a memorized configuration. In some circumstances, it can be advantageous to use a bend sufficiently tight that it would normally exceed the elastic limit of the material and thus permanently deform it. To prevent permanent deformation, a bend can be produced in the device followed by an annealing process to relieve bending stresses within the device. Following this first bend, the device can be bent further to produce an even sharper bend, and then re-annealed to alleviate the stress from this additional bending. This process can be repeated to attain a desired substantial bend, or reduced radii, or reduced angle that would otherwise permanently deform the device if the bend were attempted in a single bending event. In certain embodiments, any surface of the clip that comes in contact with blood and/or tissue can be electropolished, especially metal or metal alloy surfaces, such as a superelastic/shape memory alloy. Electropolishing may be used to produce smooth surfaces. Electropolishing can also beneficially remove or reduces flash and other artifacts from the fabrication of the device.

[00244] The clip can have a completely contiguous cross section, or partial, incomplete contiguous cross section. A discontinuous cross-section can permit certain embodiments of the clips to be loaded from the side of the vascular introducer and/or deployment instrument. In certain embodiments, the deployment instrument can include a slot or opening permitting the deployment instrument to be secured to the tubular medical device from the side. Tissue engagement elements

(e.g., tines, fingers, protrusions, etc.) can be parallel, overlapping, crossing, spiral, combination or other. The clip can include tissue engagement elements with the same, different or combination lengths. The clip can compress tissue on a horizontal plane, vertical plane or a combination of both. The tissue engagement elements can be straight, curved or a combination of both. The tissue attachment motion / direction can be straight, twisted, rotated, combination or other suitable and desirable motion or motions.

[00245] Many different types of delivery features can be incorporated during the manufacturing process for any of the devices and systems disclosed herein, such as coatings on the vascular closure device, can be used to deliver therapeutic agents, including (but are not limited to) one or more of the following: antiproliferative/antimitotic agents including natural products such as vinca alkaloids (i.e. vinblastine, vincristine, and vinorelbine), paclitaxel, epididodophyllotoxins (i.e. etoposide, teniposide), antibiotics (dactinomycin (actinomycin D) daunorubicin, doxorubicin and idarubicin), anthracyclines, mitoxantrone, bleomycins, plicamycin (mithramycin) and mitomycin, enzymes (L-asparaginase which systemically metabolizes L-asparagine and deprives cells which do not have the capacity to synthesize their own asparagine); antiplatelet agents such as G_{II}(GP IIb/IIIa) inhibitors and vitronectin receptor antagonists; antiproliferative/antimitotic alkylating agents such as nitrogen mustards (mechlorethamine, cyclophosphamide and analogs, melphalan, chlorambucil), ethylenimines and methylmelamines (hexamethylmelamine and thiotepa), alkyl sulfonates-busulfan, nitrosoureas (carmustine (BCNU) and analogs, streptozocin), trazenes—dacarbazine (DTIC); antiproliferative/antimitotic antimetabolites such as folic acid analogs (methotrexate), pyrimidine analogs (fluorouracil, floxuridine, and cytarabine), purine analogs and related inhibitors (mercaptopurine, thioguanine, pentostatin and 2-chlorodeoxyadenosine {cladribine}); platinum coordination complexes (cisplatin, carboplatin), procarbazine, hydroxyurea, mitotane, aminoglutethimide; hormones (i.e. estrogen); anticoagulants (heparin, synthetic heparin salts and other inhibitors of thrombin); fibrinolytic agents (such as tissue plasminogen activator, streptokinase and urokinase), aspirin, dipyridamole, ticlopidine, clopidogrel, abciximab; antimigratory; antisecretory (breveldin); anti-inflammatory: such as adrenocortical steroids (cortisol, cortisone, fludrocortisone, prednisone, prednisolone, 6.alpha.-methylprednisolone, triamcinolone, betamethasone, and dexamethasone), non-steroidal agents (salicylic acid derivatives i.e. aspirin; para-aminophenol derivatives i.e. acetaminophen; indole and indene acetic acids (indomethacin, sulindac, and etodolac), heteroaryl acetic acids (tolmetin, diclofenac, and ketorolac), arylpropionic acids (ibuprofen and derivatives), anthranilic acids (mefenamic acid, and meclofenamic acid), enolic acids (piroxicam, tenoxicam, phenylbutazone, and oxyphenthatrazone), nabumetone, gold compounds (auranofin, aurothioglucose, gold sodium thiomalate); immunosuppressives: (cyclosporine, tacrolimus (FK-506), sirolimus (rapamycin), azathioprine, mycophenolate mofetil); angiogenic agents: vascular endothelial growth factor (VEGF), fibroblast growth factor (FGF); angiotensin receptor blockers; nitric oxide donors; anti-sense oligonucleotides and combinations thereof; cell cycle inhibitors,

mTOR inhibitors, and/or growth factor signal transduction kinase inhibitors. Alternatively, a clot promoter can be used, such as protamine sulphate or calcium hydroxide. Endothelial cells can also be added to the vascular closure device.

[00246] One or more of the therapeutic agents can be included in the device in many ways, such as by blending them into the device base materials during fabrication, applying them just prior to deployment, or applying them after the device has been deployed. One or more therapeutic agents can be used on a single device. The delivery feature can be designed to provide benefits rapidly or over an extended period of time. The delivery feature can be stable or eluting. The coatings, materials, compounds, substances, therapeutic agents, etc., can elute from a coated (or embedded) device (or component) over time and enter the surrounding tissue. In certain embodiments, the delivery feature can be effective during a period of at least about three days in some applications, between about seven and about thirty days in other application, and/or up to approximately six months in some applications.

IV. Kits

[00247] A vessel closure system as described above can be sold to end users in the form of a kit. The kits can comprise multiple items, including but not limited to one or more deployment instruments and one or more clips. The kits can further comprise tissue cutters and tissue dilators as described above. In some embodiments, the kits can comprise swellable plugs in addition to or instead of the clips. The deployment instruments can be preloaded with the clips or plugs, or the kits can require assembly by the end user. In some embodiments, the kits can comprise an elongate medical device. In some embodiments, the kits can comprise one or more items selected from the group consisting of needles, hypo tubes, guidewires, electrode wires, intravenous wires, vascular introducers, catheters, laparoscopes, endoscopes, trocars, and cannulas. In some embodiments, the kits can comprise a compound for delivery to a tissue. The compound can be one or more of a sclerosing agent, an antibiotic, or an anti-inflammatory agent. In some embodiments, the kits can comprise one or more of any of a pair of scissors, a scalpel, a swab, a syringe, a hemostat, a lubricant, a needle, a snare, an antiseptic, or an anesthetic. Components of the kits can be designed and intended for single or multiple uses.

[00248] Kits can be configured such that deployment of the kits enables quickly stopping, or significantly reducing bleeding from a blood vessel (artery or vein), organ and/or other tissue where bleeding is present as a result of an impact trauma such as a knife wound or gun shot. Thus, the devices can be configured to be sized for a variety of applications.

[00249] While preferred embodiments of the present invention have been shown and described herein, it will be obvious to those skilled in the art that such embodiments are provided by way of example only. Numerous variations, changes, and substitutions will now occur to those skilled in the art without departing from the invention. It should be understood that various alternatives to the embodiments of the invention described herein may be employed in practicing the

invention. It is intended that the following claims define the scope of the invention and that methods and structures within the scope of these claims and their equivalents be covered thereby.

CLAIMS

WHAT IS CLAIMED IS:

1. A closure device comprising:
 - (a) a distal flexible cap;
 - (b) one or more proximally positioned radial extending elements;
 - (c) a stem positioned between the distal flexible cap and the one or more radial extending element,wherein the distal flexible cap is formable toward an axis.
2. The closure device of claim 1 wherein the distal flexible cap has at least one of a substantially flat distal surface and a substantially flat proximal surface, a substantially flat distal surface and a substantially concave proximal surface, a substantially flat distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially flat proximal surface, a substantially convex distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially concave proximal surface, a substantially concave distal surface and a substantially flat proximal surface, a substantially concave distal surface and a substantially concave proximal surface, and a substantially concave distal surface and a substantially convex proximal surface.
3. The closure device of claim 1 wherein the distal flexible cap has at least one of a uniform thickness in a cross-section or a variable thickness in a cross-section.
4. The closure device of claim 1 wherein the proximal surface of the distal flexible cap has one of more of at least one of anchoring protrusions, nibs or ribs.
5. The closure device of claim 1 wherein the distal flexible cap has a shape selected from round, triangular, oval, ovoid, elliptical, square, and saucer.
6. The closure device of claim 5 wherein the flexible cap shape has rounded edges.
7. The closure device of claim 1 wherein the stem is positioned on a proximal surface of the flexible cap at least one of centrally and non-centrally.
8. The closure device of claim 1 further comprising a proximally accessible stem bore.
9. The closure device of claim 8 wherein a clip is positionable within the proximal bore.
10. The closure device of claim 8 wherein the proximally accessible stem bore has at least one of internal threads along an interior surface, parallel walls along its length, non-parallel walls along its length, an undercut in the bore at a location along its length, and a bent bore along its length.
11. The closure device of claim 8 wherein the bore extend from the proximal end of the device to the proximal end of the flexible cap.
12. The closure device of claim 1 wherein the stem has a cross-sectional profile selected from the group comprising square, triangular, arrowhead, trapezoidal, rectangular, J, Y, hook, and bulbous.

13. The closure device of claim 1 wherein the stem further comprises a proximally positioned aperture therethrough.
14. The closure device of claim 1 wherein the stem further comprises one or more exterior features adapted and configured to achieve anchoring the stem in vivo.
15. The closure device of claim 1 wherein the stem further comprises a one or more slots along at least a portion of its length parallel to a stem longitudinal axis beginning at its proximal end.
16. The closure device of claim 13 wherein the stem is adapted and configured to open away from the longitudinal axis from its proximal end.
17. The closure device of claim 1 wherein the stem has a proximal end adapted and configured to form a clasp, a socket, a breakable stem, a tearable stem.
18. The closure device of claim 1 wherein at least one of the distal flexible cap and stem are in releasable communication with a tether.
19. The closure device of claim 18 wherein the tether is one or more of a wire, a spring, a thread, a ribbon, and a tube.
20. The closure device of claim 19 wherein the wire is at least one of a bent wire, a curved wire, a wavy wire, and a helical wire.
21. A delivery capsule comprising:
 - a cartridge body;
 - a tapered distal tip;
 - a compressible section;
 - a clear section;
 - a lumen extending therethrough,wherein the clear section is adapted and configured to house a closure device.
22. The delivery capsule of claim 21 further comprising a valve.
23. The delivery capsule of claim 21 further comprising one or more proximally positioned detent features on an exterior surface of the cartridge body.
24. The delivery capsule of claim 21 further comprising one or more distally positioned undercuts.
25. The delivery capsule of claim 21 further comprising an exterior groove in the cartridge body.
26. The delivery capsule of claim 21 further comprising a one-way snap feature.
27. The delivery capsule of claim 21 further comprising an undercut central bore.
28. The delivery capsule of claim 21 wherein the capsule is adapted and configured to receive a plunger through a central aperture.
29. The delivery capsule of claim 28 wherein the capsule is adapted and configured to permit the plunger to move in a first axial direction and resist movement in a second axial direction different than the first direction.

30. The delivery capsule of claim 21 further comprising one or more collets.

31. A wound closure delivery system comprising:

an introducer;

a wound closure delivery cartridge;

a guide and seal assembly; and

a plunger

wherein the introducer is adapted and configured to releasably engage the wound closure delivery cartridge at a proximal end, the wound closure delivery cartridge is adapted and configured to releasably engage the guide and seal assembly at a proximal end, and the plunger is adapted and configured to be advanced through a lumen in each of the guide and seal assembly, the wound closure delivery cartridge and the introducer.

32. The wound closure delivery system of claim 31 wherein the system further comprises a closure device within the cartridge having a distal flexible cap; one or more proximally positioned radial extending elements; a stem positioned between the distal flexible cap and the one or more radial extending element, wherein the distal flexible cap is formable toward an axis.

33. The wound closure delivery system of claim 32 wherein the distal flexible cap of the closure device has at least one of a substantially flat distal surface and a substantially flat proximal surface, a substantially flat distal surface and a substantially concave proximal surface, a substantially flat distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially flat proximal surface, a substantially convex distal surface and a substantially convex proximal surface, a substantially convex distal surface and a substantially concave proximal surface, a substantially concave distal surface and a substantially flat proximal surface, a substantially concave distal surface and a substantially concave proximal surface, and a substantially concave distal surface and a substantially convex proximal surface.

34. The wound closure delivery system of claim 32 wherein the distal flexible cap has at least one of a uniform thickness in a cross-section or a variable thickness in a cross-section.

35. The wound closure delivery system of claim 32 wherein the proximal surface of the distal flexible cap has one of more of at least one of anchoring protrusions, nibs or ribs.

36. The wound closure delivery system of claim 32 wherein the distal flexible cap has a shape selected from round, triangular, oval, ovoid, elliptical, square, and saucer.

37. The wound closure delivery system of claim 36 wherein the flexible cap shape has rounded edges.

38. The wound closure delivery system of claim 32 wherein the closure device stem is positioned on a proximal surface of the flexible cap at least one of centrally and non-centrally.

39. The wound closure delivery system of claim 32 further comprising a proximally accessible stem bore.

40. The wound closure delivery system of claim 39 wherein a clip is positionable within the proximal bore of the closure device.
41. The wound closure delivery system of claim 39 wherein the proximally accessible stem bore has at least one of internal threads along an interior surface, parallel walls along its length, non-parallel walls along its length, an undercut in the bore at a location along its length, and a bent bore along its length.
42. The wound closure delivery system of claim 39 wherein the bore extend from the proximal end of the device to the proximal end of the flexible cap.
43. The wound closure delivery system of claim 32 wherein the stem has a cross-sectional profile selected from the group comprising square, triangular, arrowhead, trapezoidal, rectangular, J, Y, hook, and bulbous.
44. The wound closure delivery system of claim 32 wherein the stem further comprises a proximally positioned aperture therethrough.
45. The wound closure delivery system of claim 32 wherein the stem further comprises one or more exterior features adapted and configured to achieve anchoring the stem in vivo.
46. The wound closure delivery system of claim 32 wherein the stem further comprises a one or more slots along at least a portion of its length parallel to a stem longitudinal axis beginning at its proximal end.
47. The wound closure delivery system of claim 46 wherein the stem is adapted and configured to open away from the longitudinal axis from its proximal end.
48. The wound closure delivery system of claim 32 wherein the stem has a proximal end adapted and configured to form a clasp, a socket, a breakable stem, a tearable stem.
49. The wound closure delivery system of claim 32 wherein at least one of the distal flexible cap and stem are in releasable communication with a tether.
50. The wound closure delivery system of claim 49 wherein the tether is one or more of a wire, a spring, a thread, a ribbon, and a tube.
51. The wound closure delivery system of claim 50 wherein the wire is at least one of a bent wire, a curved wire, a wavy wire, and a helical wire.
52. The wound closure delivery system of claim 31 further comprising a delivery capsule having a cartridge body; a tapered distal tip; a compressible section; a clear section; a lumen extending therethrough, wherein the clear section is adapted and configured to house a closure device.
53. The wound closure delivery system of claim 52 wherein at least one of the introducer or the delivery capsule further comprises a valve.
54. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises one or more proximally positioned detent features on an exterior surface of the cartridge body.

55. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises one or more distally positioned undercuts.

56. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises an exterior groove in the cartridge body.

57. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises a one-way snap feature.

58. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises an undercut central bore.

59. The wound closure delivery system of claim 52 wherein the capsule is adapted and configured to receive a plunger through a central aperture.

60. The wound closure delivery system of claim 59 wherein the capsule is adapted and configured to permit the plunger to move in a first axial direction and resist movement in a second axial direction different than the first direction.

61. The wound closure delivery system of claim 52 wherein the delivery capsule further comprises one or more collets.

62. A method closing a wound comprising:

- (a) assembling a wound closure system comprising a guide and seal assembly, a closure device delivery capsule, and an introducer;
- (b) inserting the assembled wound closure system percutaneously;
- (c) entering a mammalian vessel with a distal tip of a tubular sheath of the introducer; and
- (d) inserting a plunger into a proximal aperture in the guide and seal assembly;
- (e) advancing the plunger through the guide and seal assembly into the closure device delivery capsule;
- (f) engaging the closure device at the tip of the plunger;
- (g) advancing the closure device into a tapered tip and reducing a profile of the closure device in at least one plane;
- (h) advancing the closure device beyond the distal tip of the tubular sheath of the introducer and into the vessel; and
- (i) withdrawing the system until a proximal surface of a face plate of the closure device comes in contact with an interior surface of the mammalian vessel;
- (j) disengaging the closure device from the interior of the introducer.

63. The method of claim 62 further comprising the step of pulling a tether connected to a proximal end of the closure device.

64. The method of claim 63 further comprising the step of releasing the tether connected to the proximal end of the closure device.

65. A kit for a percutaneous procedure comprising a closure device delivery capsule housing a closure device; an introducer; a guide and seal assembly; and a plunger.

66. The kit of claim 65 further comprising one or more items selected from the group consisting of needles, hypo tubes, guidewires, electrode wires, intravenous wires, vascular introducers, catheters, laparoscopes, endoscopes, trocars, and cannulas.

67. The kit of claim 65 further comprising a compound for delivery to a tissue.

68. The kit of claim 67 wherein the compound is one or more of a sclerosing agent, an antibiotic, and an anti-inflammatory agent.

69. The kit of claim 65 further comprising one or more items selected from the group consisting of a pair of scissors, a scalpel, a swab, a syringe, a hemostat, a lubricant, a needle, a snare, an antiseptic, and an anesthetic.

1 / 98


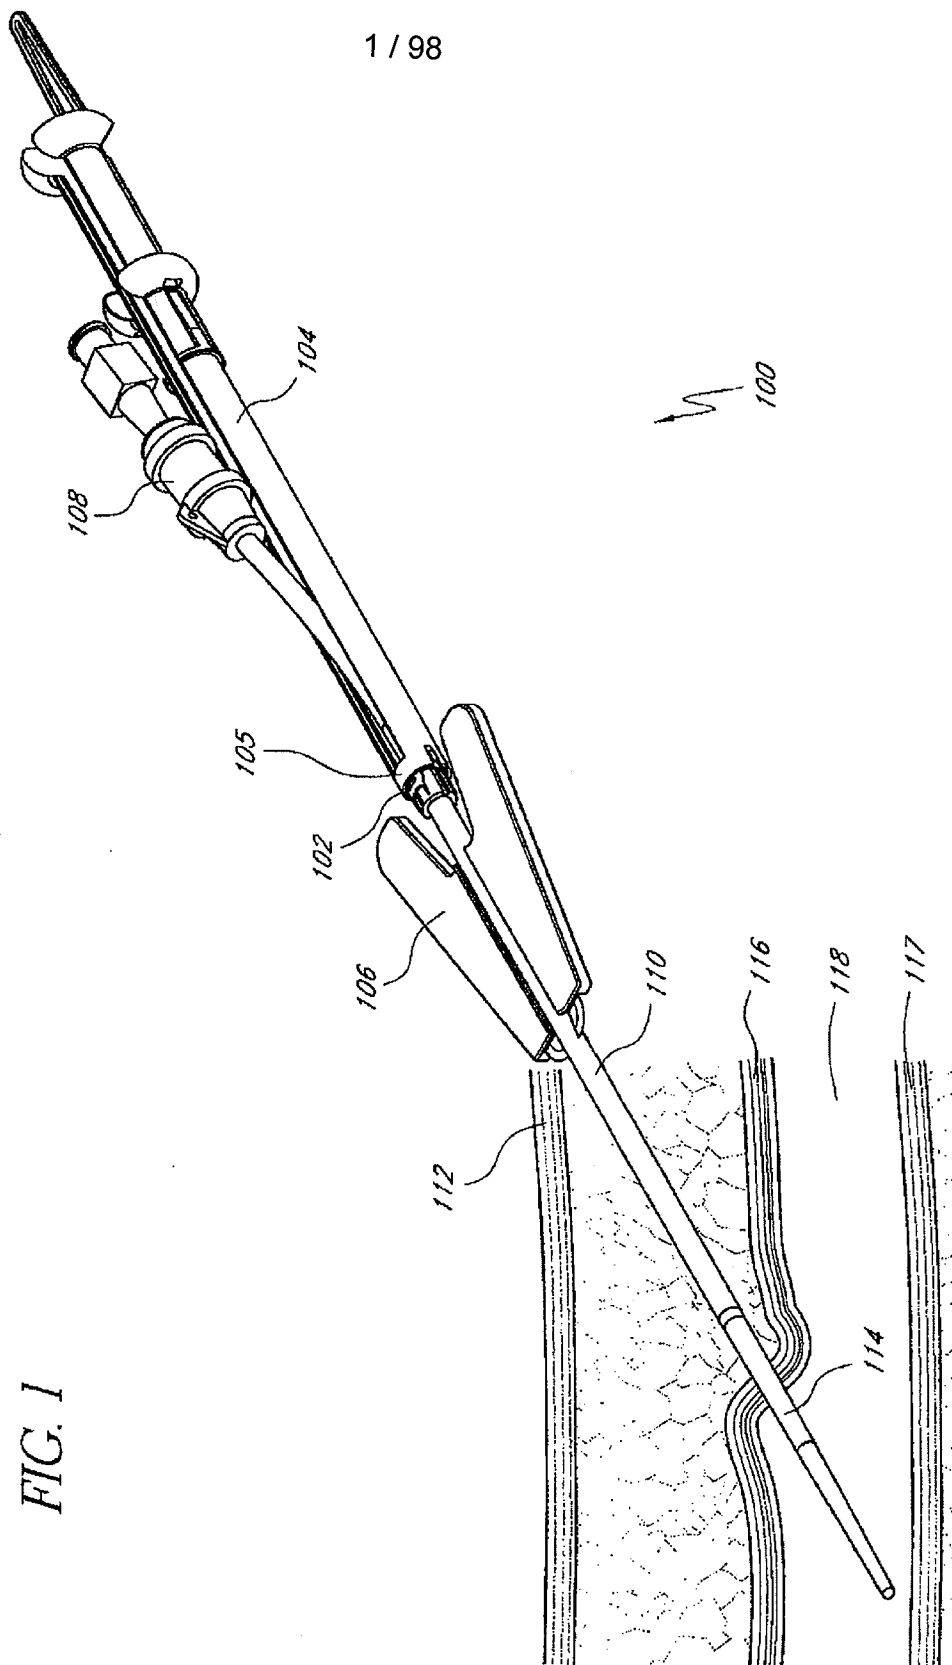


FIG. 1

FIG. 2

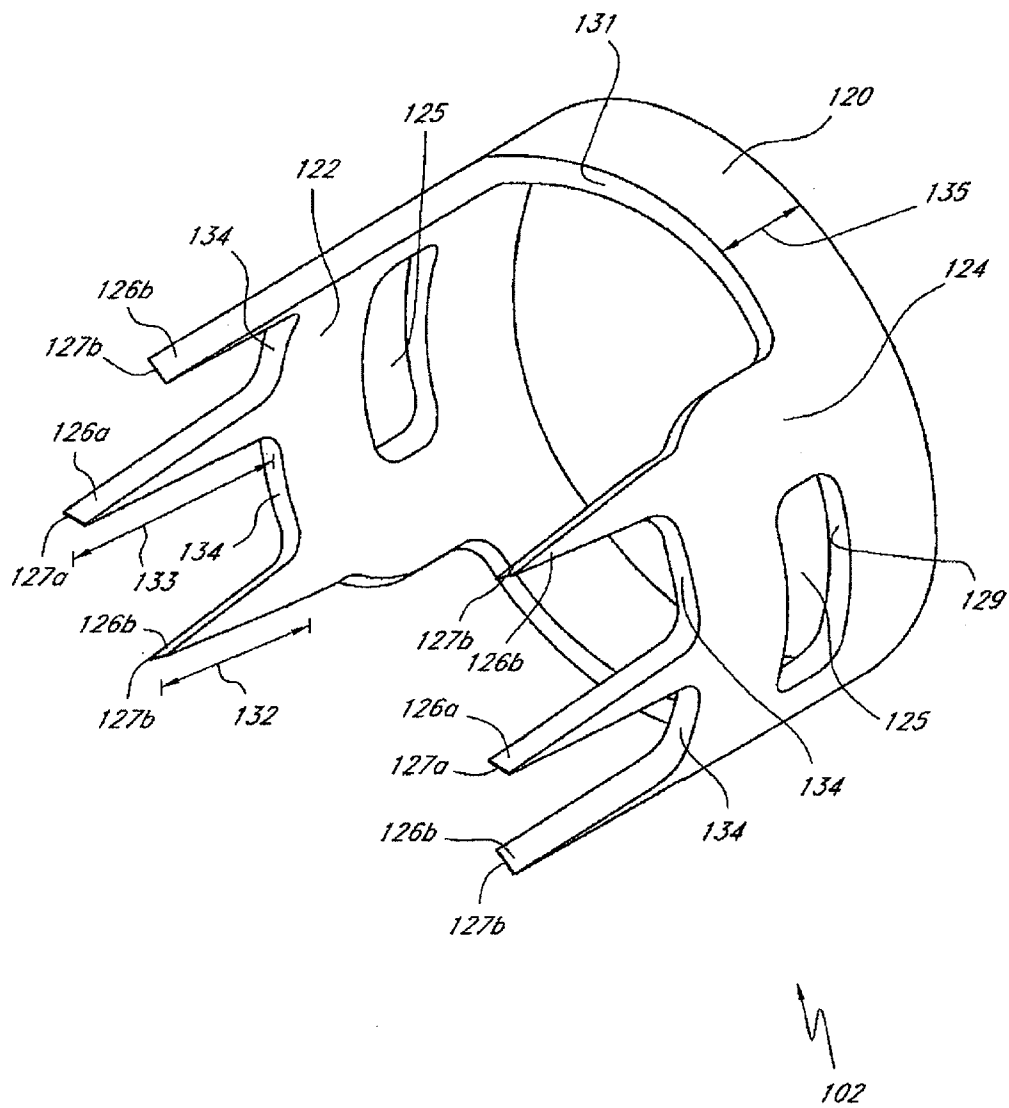

3 / 98

FIG. 3


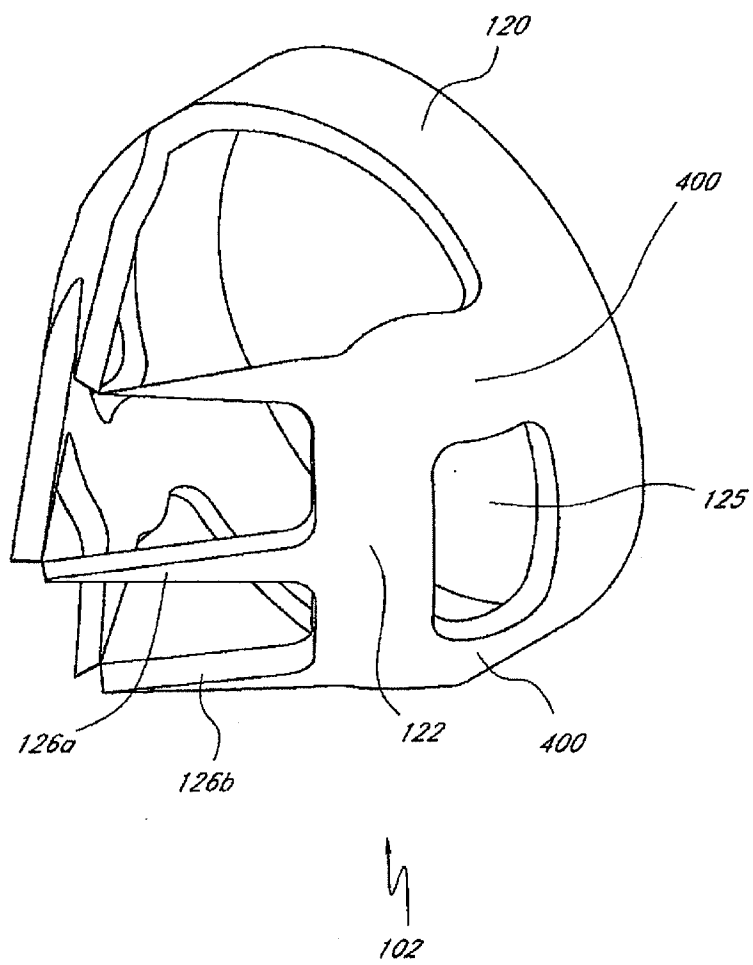


FIG. 4

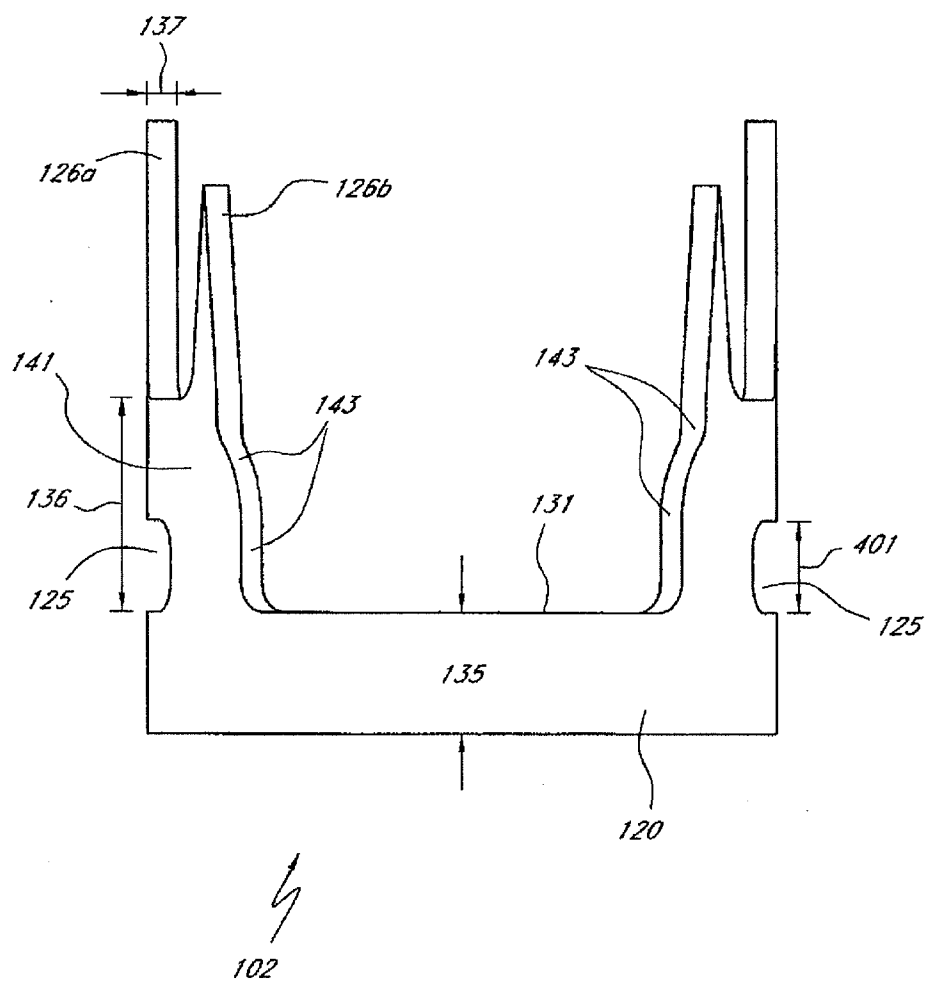

5 / 98

FIG. 5



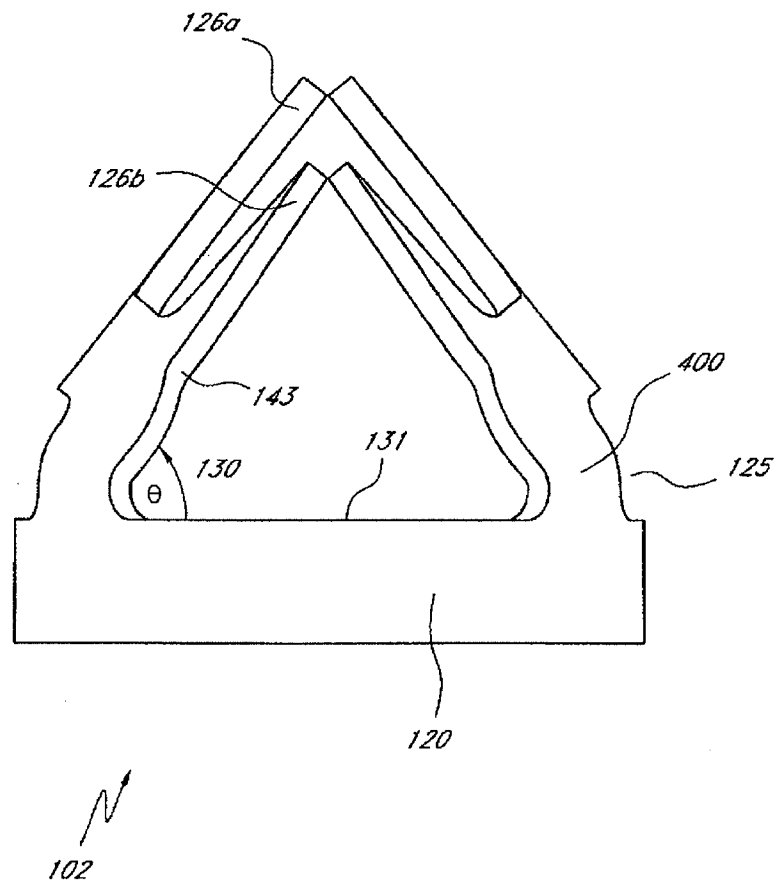


FIG. 6

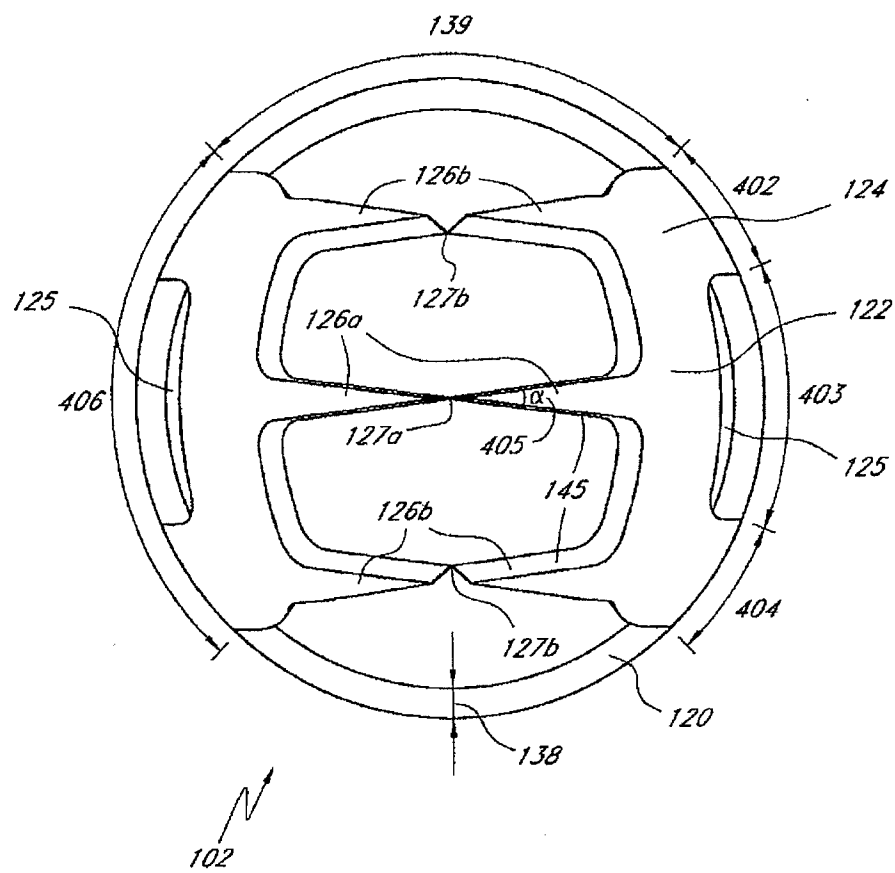


7 / 98

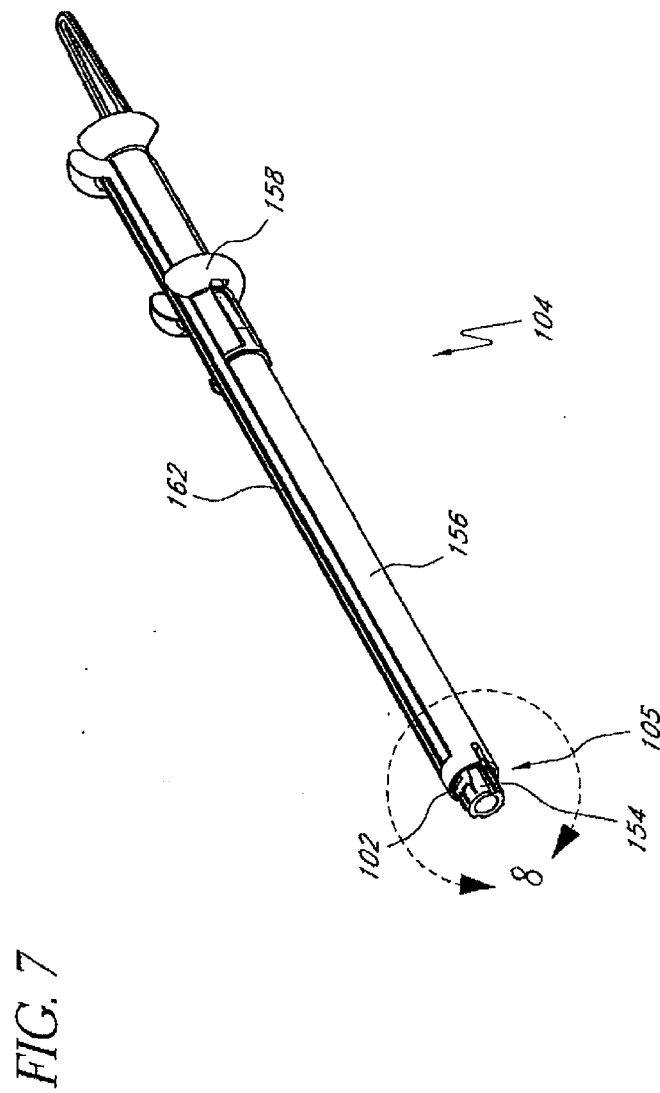


8 / 98

FIG. 8

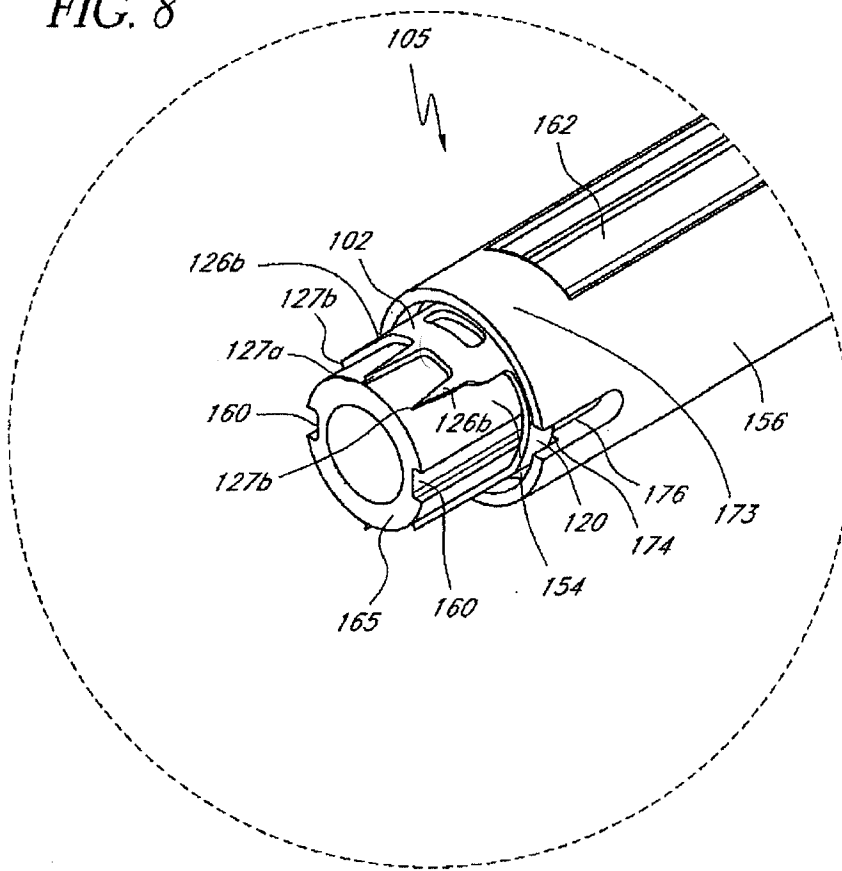


9 / 98

FIG. 9

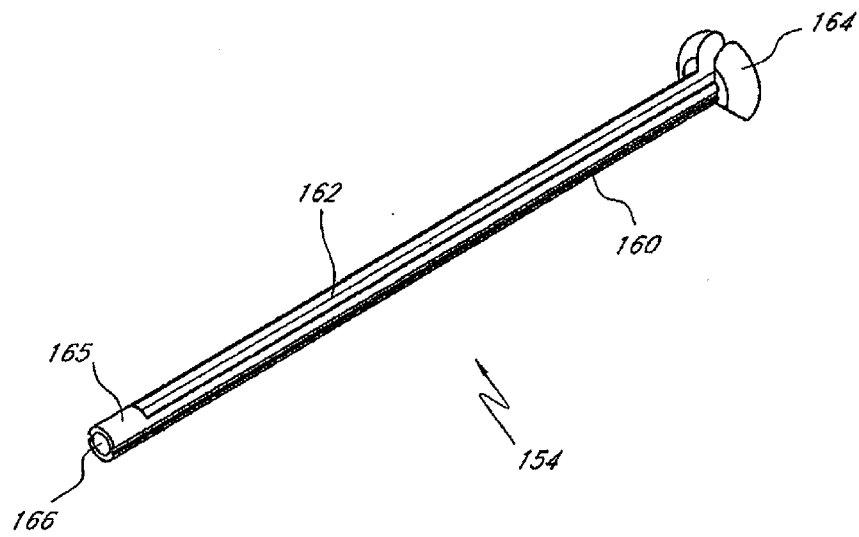


10 / 98

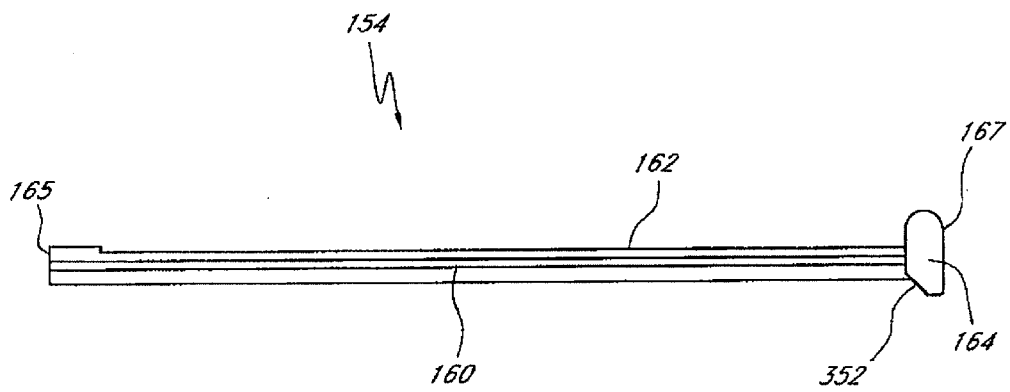FIG. 10


11 / 98

FIG. 11

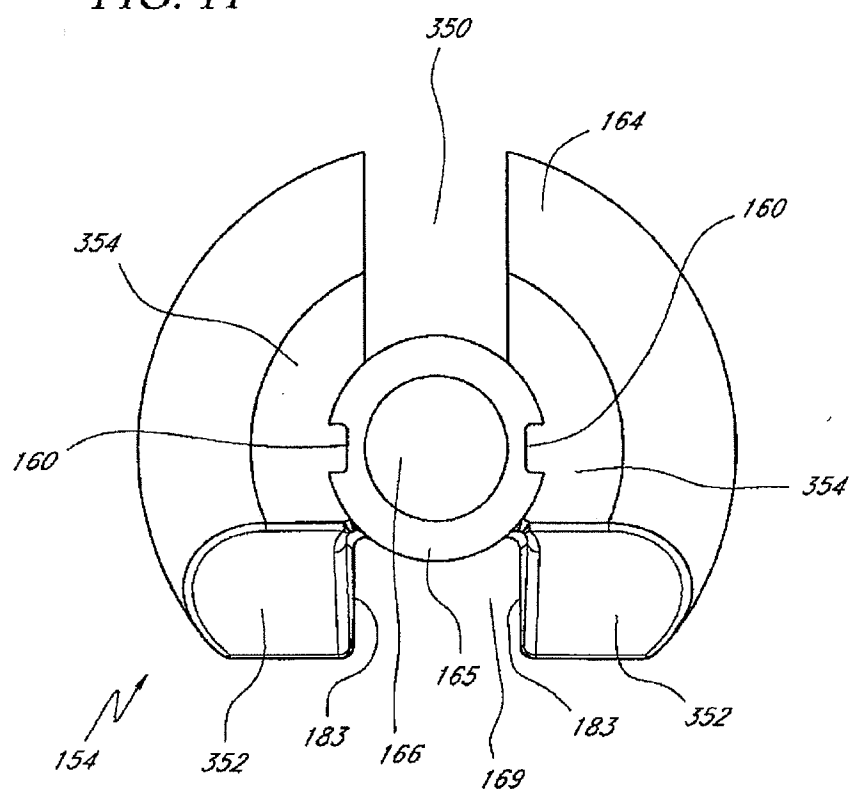

12 / 98

FIG. 12

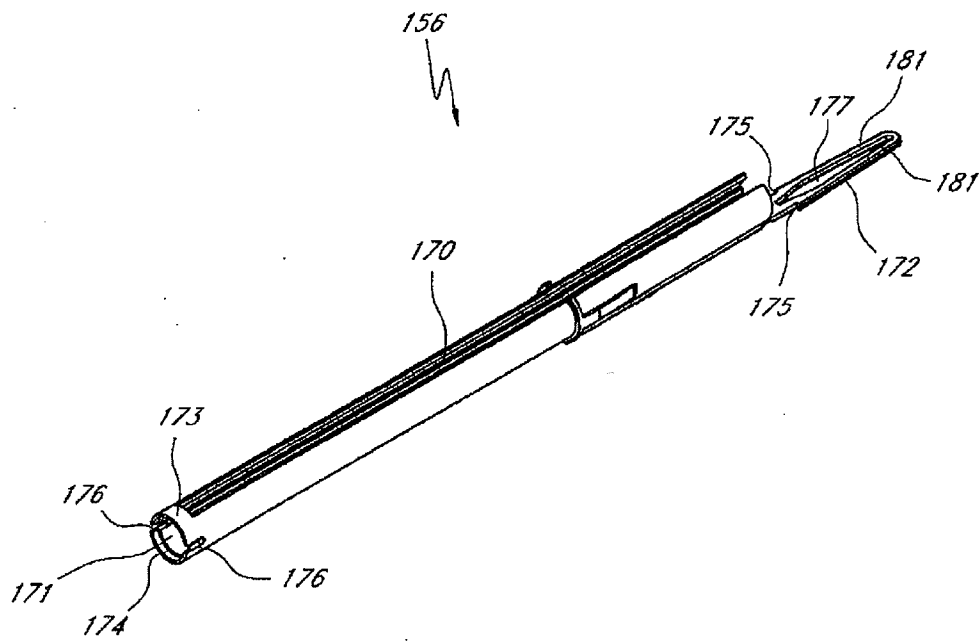

13 / 98

FIG. 13



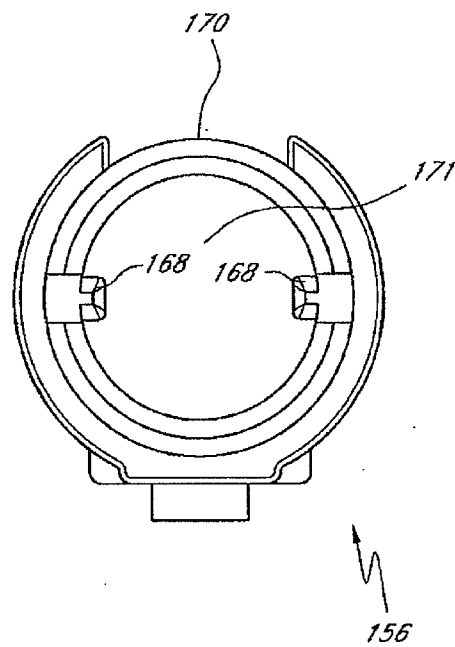


FIG. 14

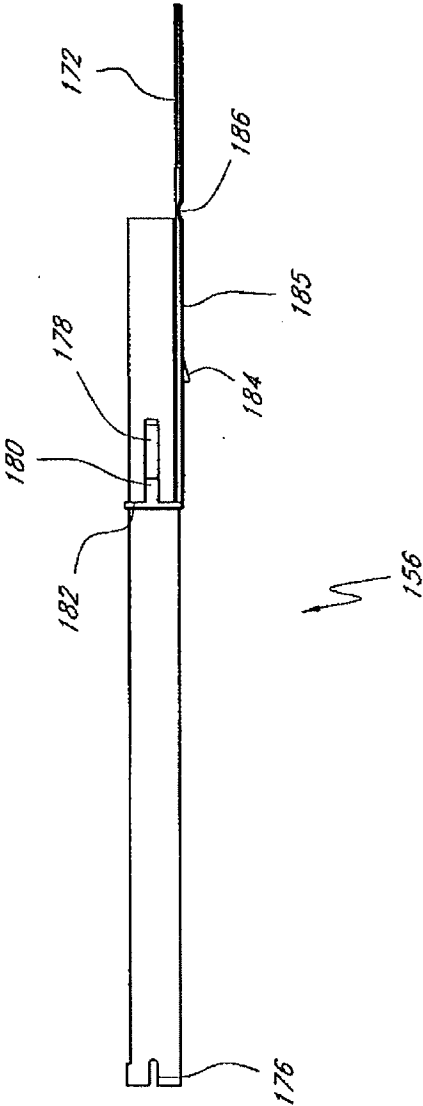


15 / 98

FIG. 15

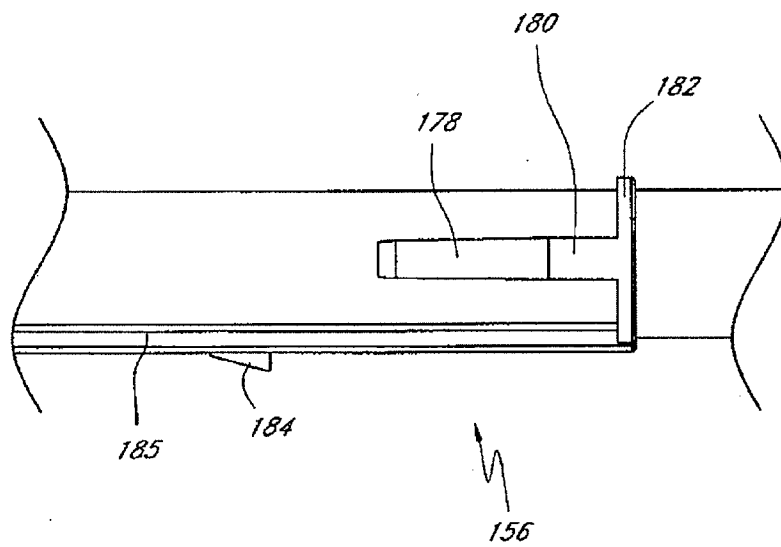


16 / 98

FIG. 16

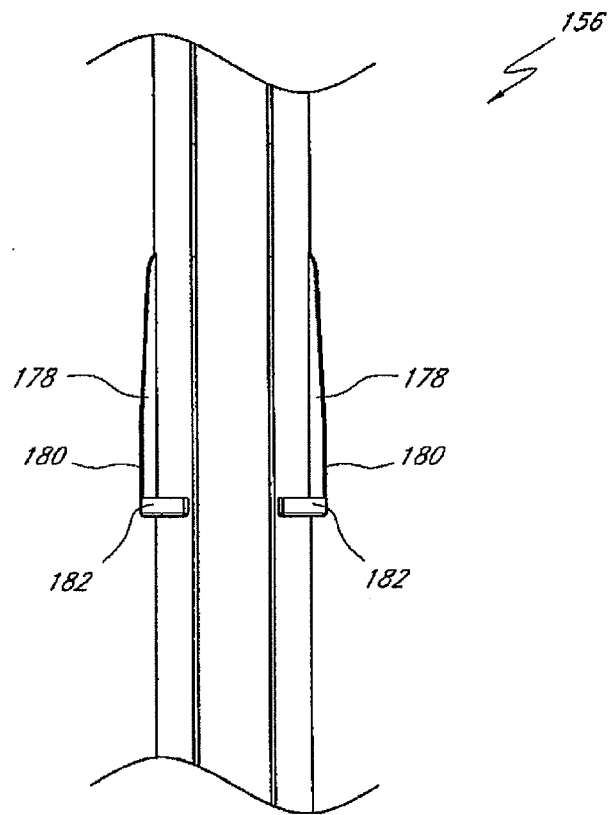


17 / 98


FIG. 17

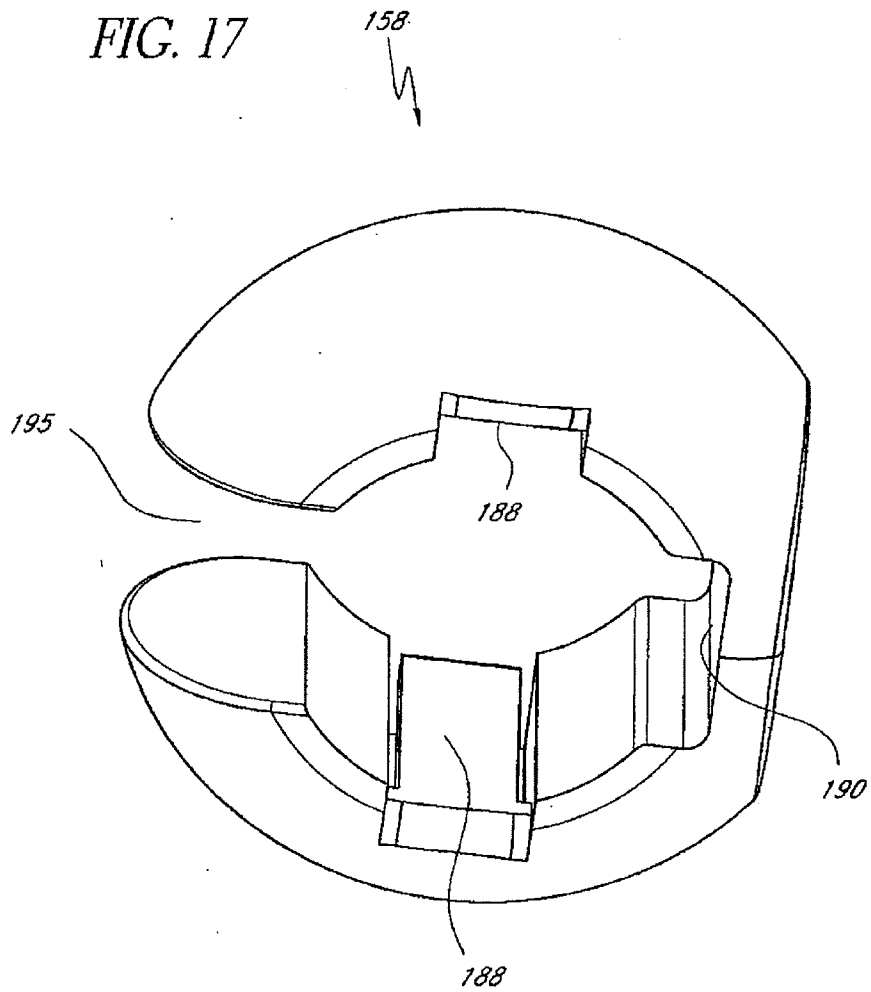


18 / 98

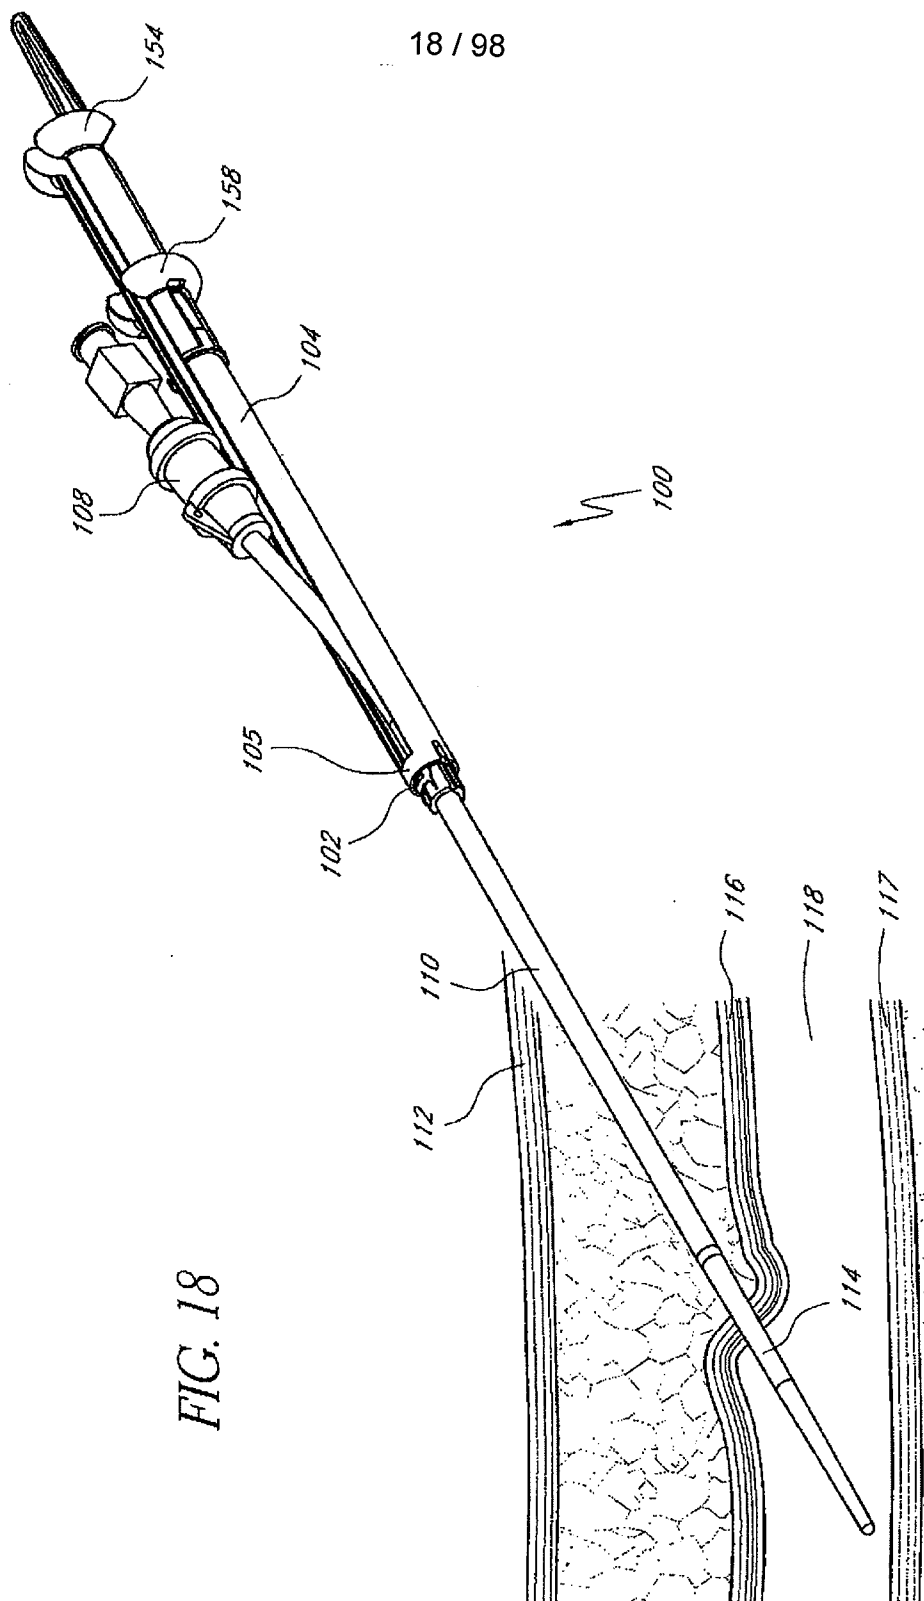

19 / 98

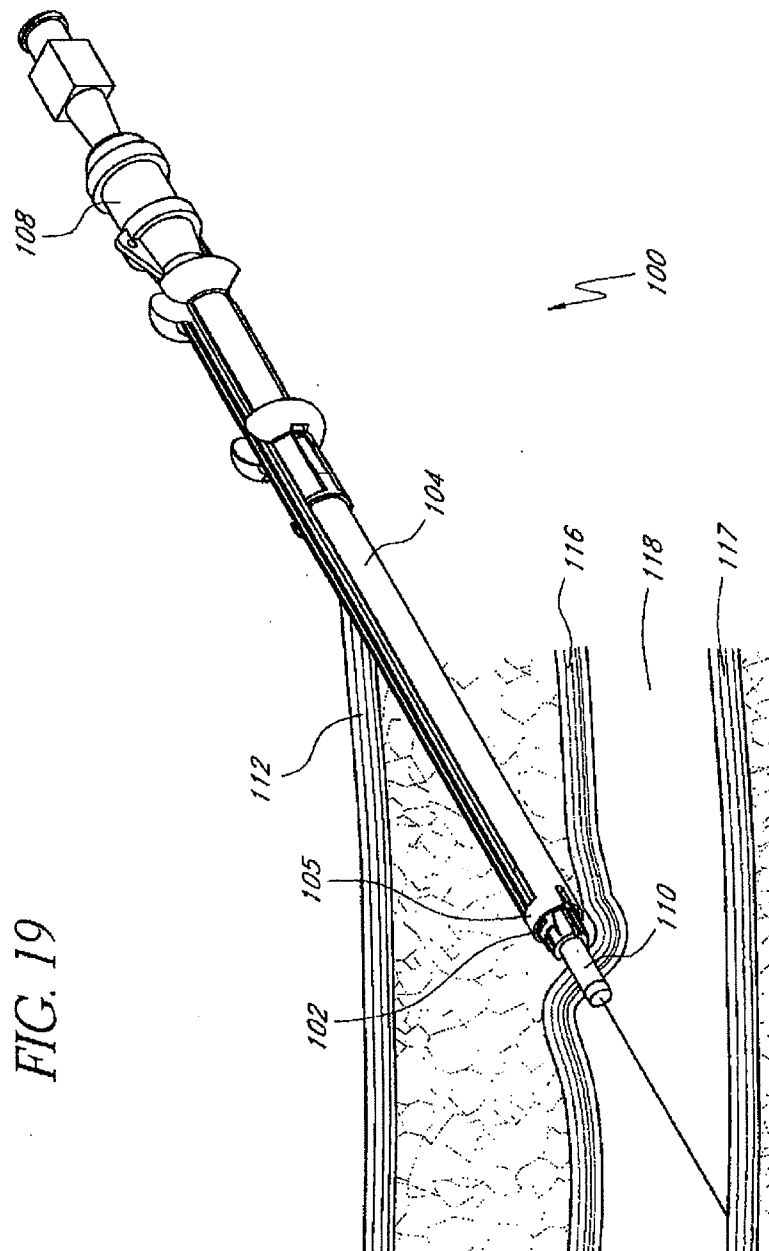

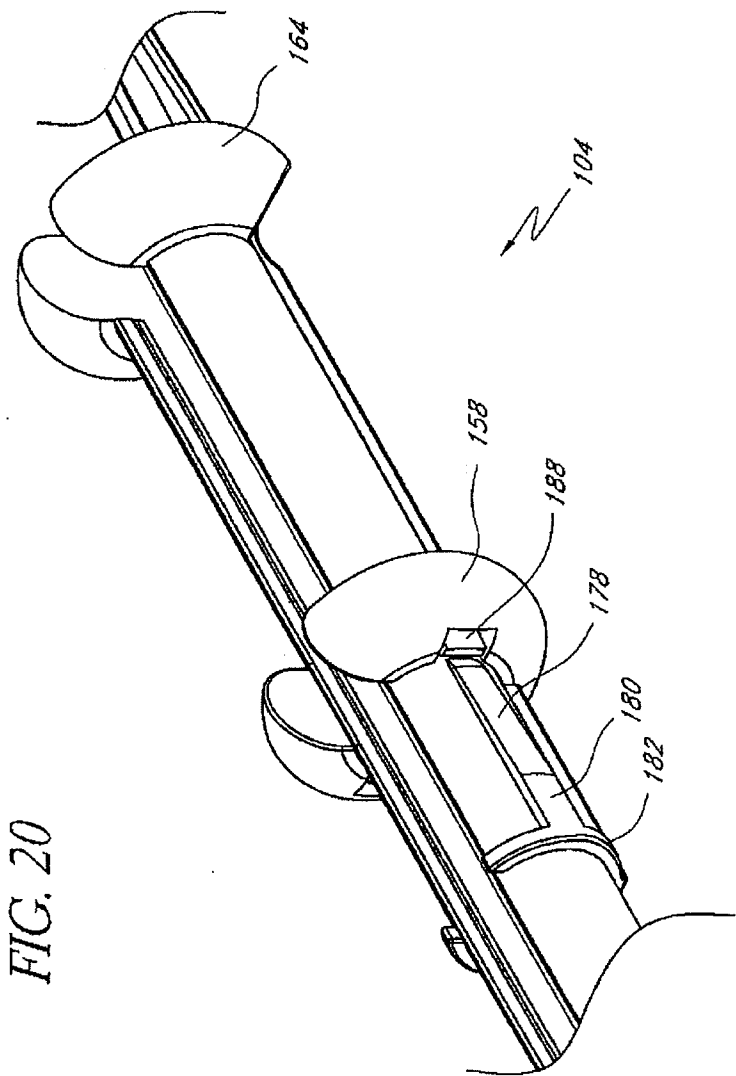

21 / 98


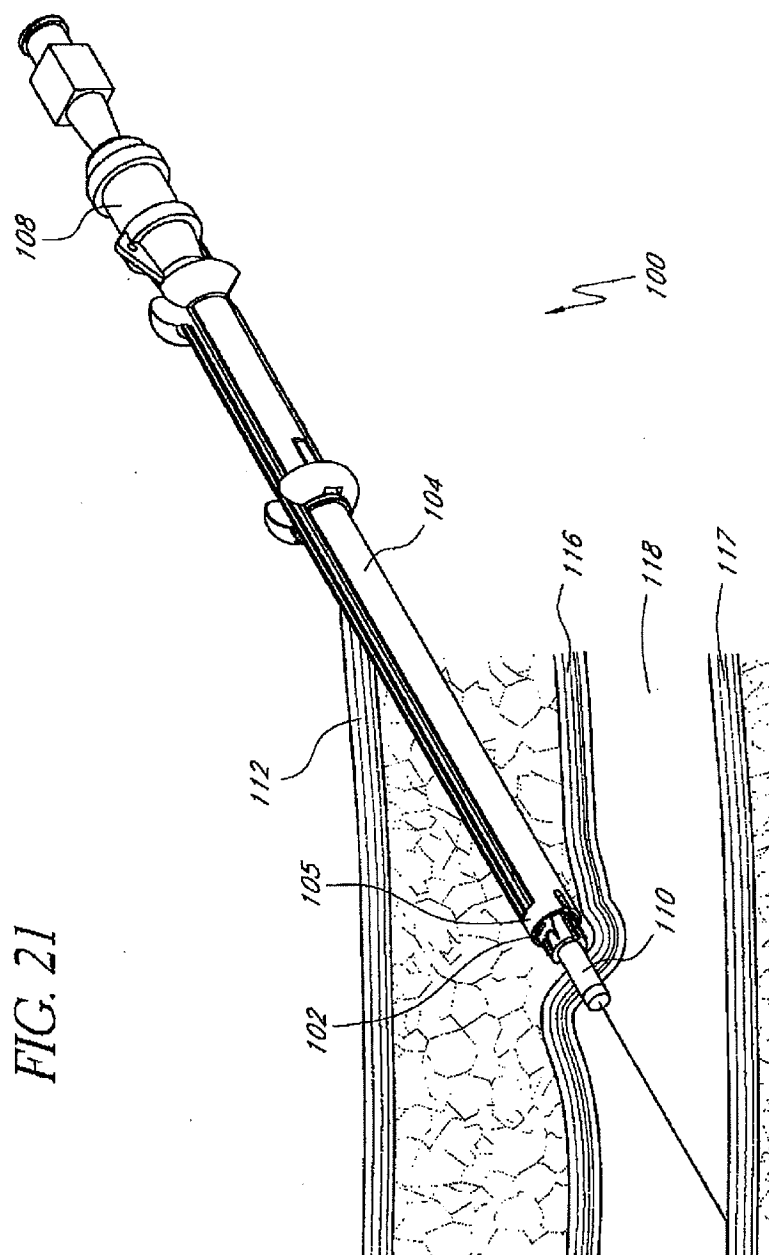


FIG. 21

22 / 98

FIG. 22

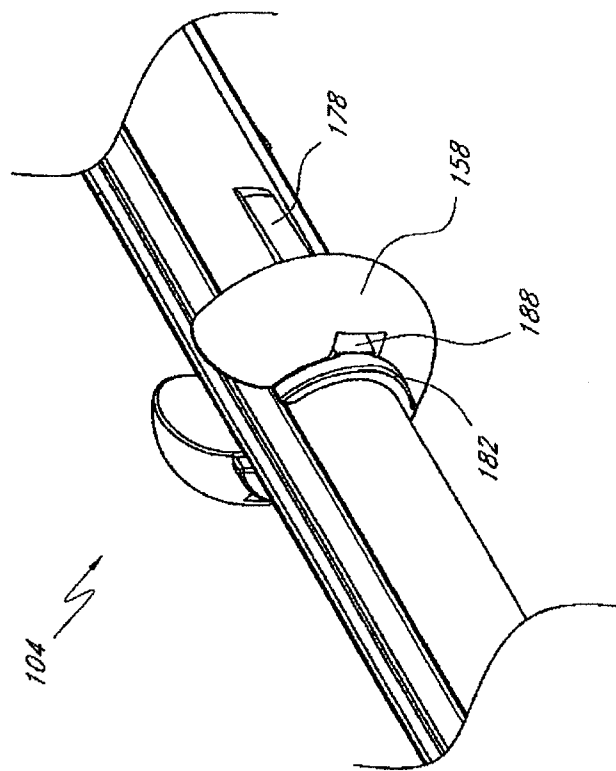

23 / 98

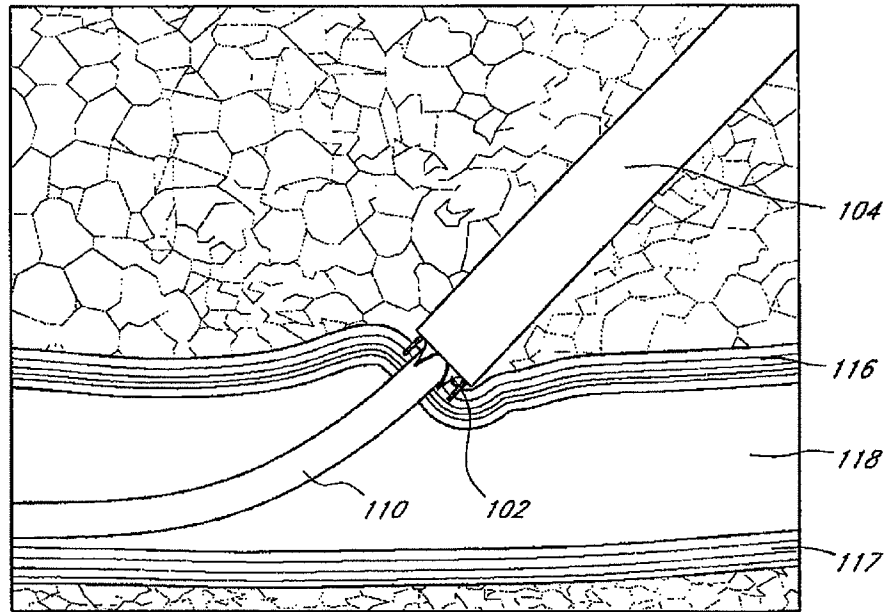


FIG. 23

24 / 98


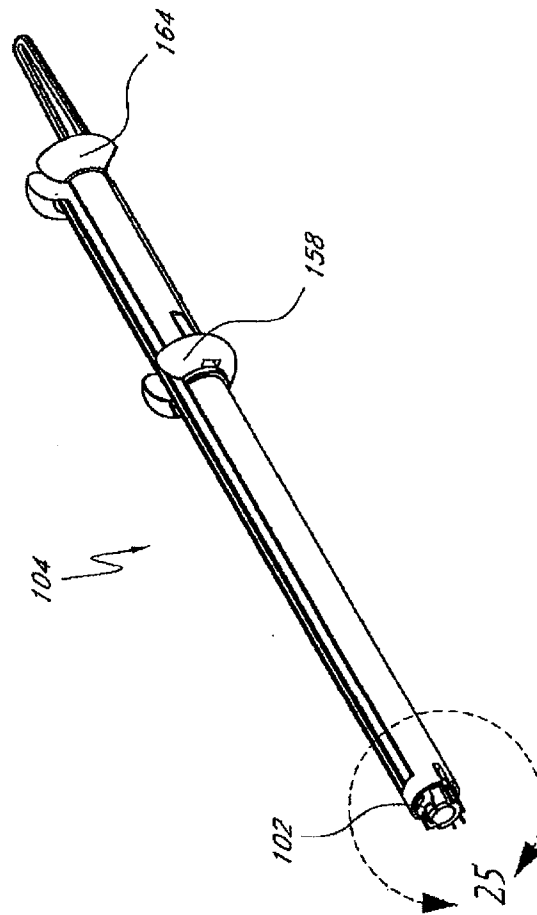


FIG. 24


25 / 98

FIG. 25

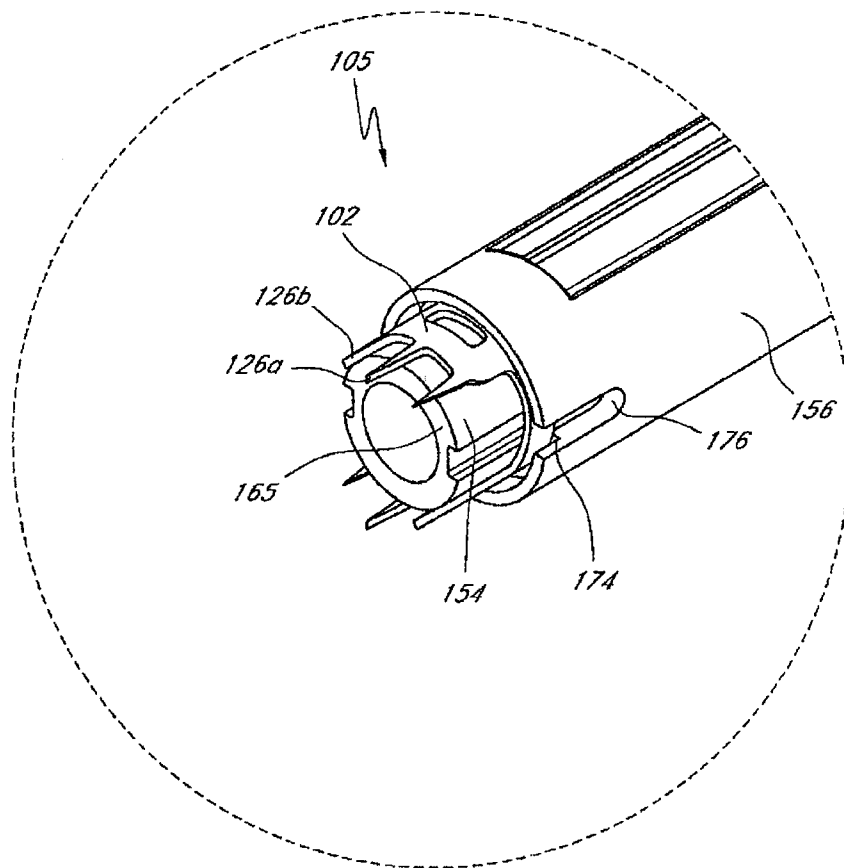

26 / 98

FIG. 26

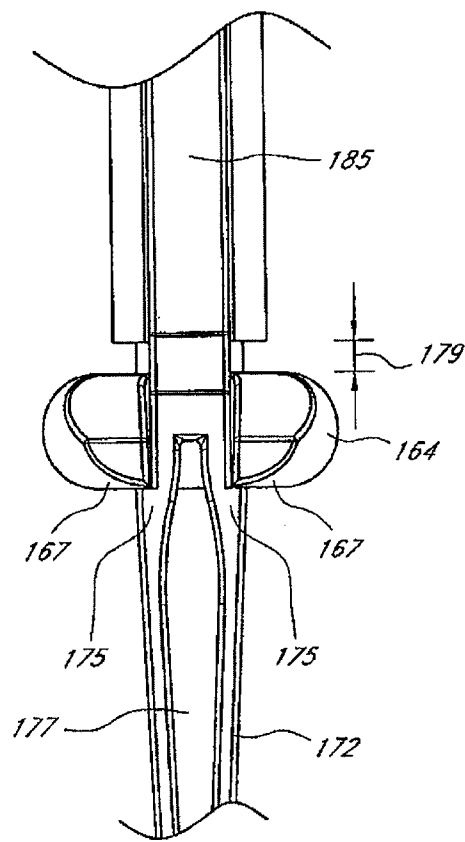

27 / 98

FIG. 27


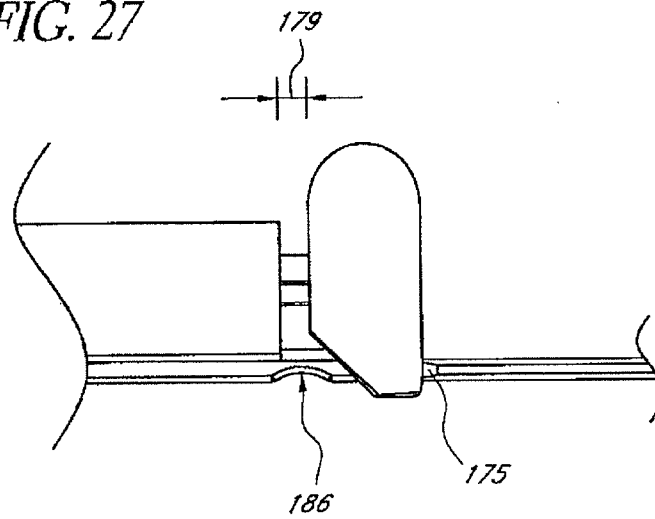


FIG. 29

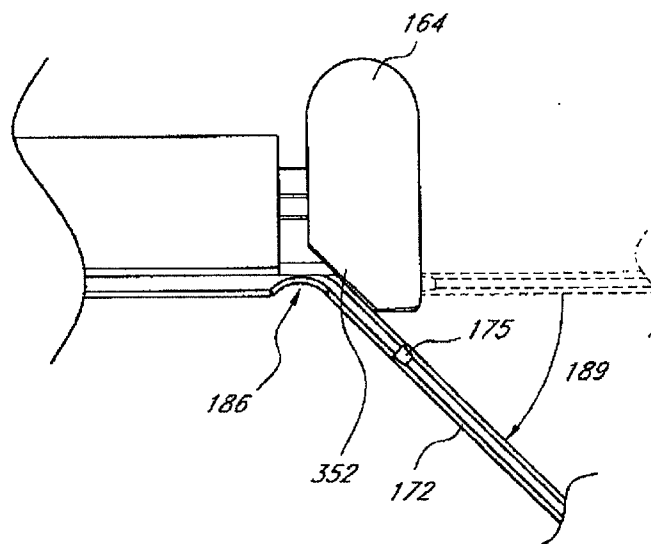

28 / 98

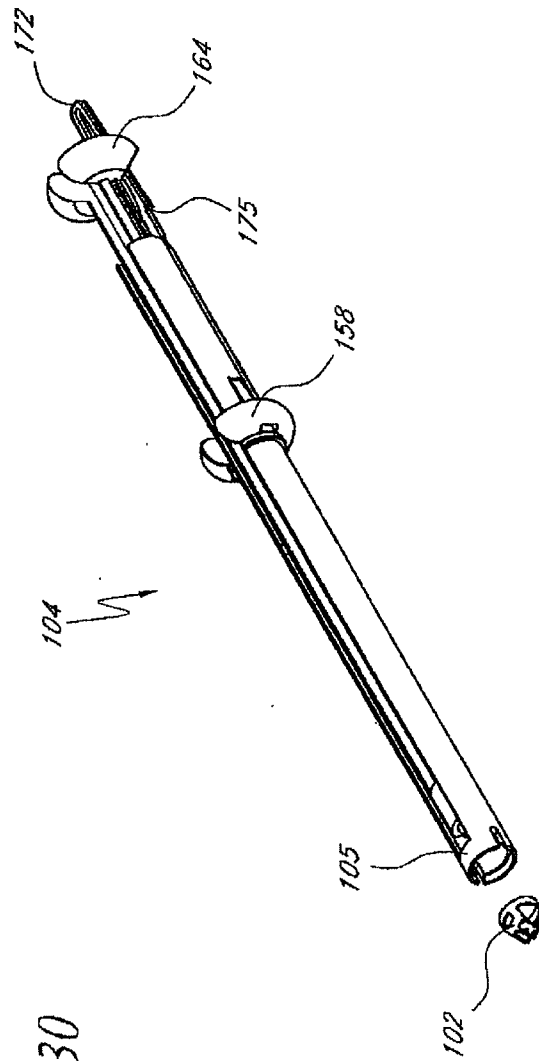


FIG. 30

29 / 98

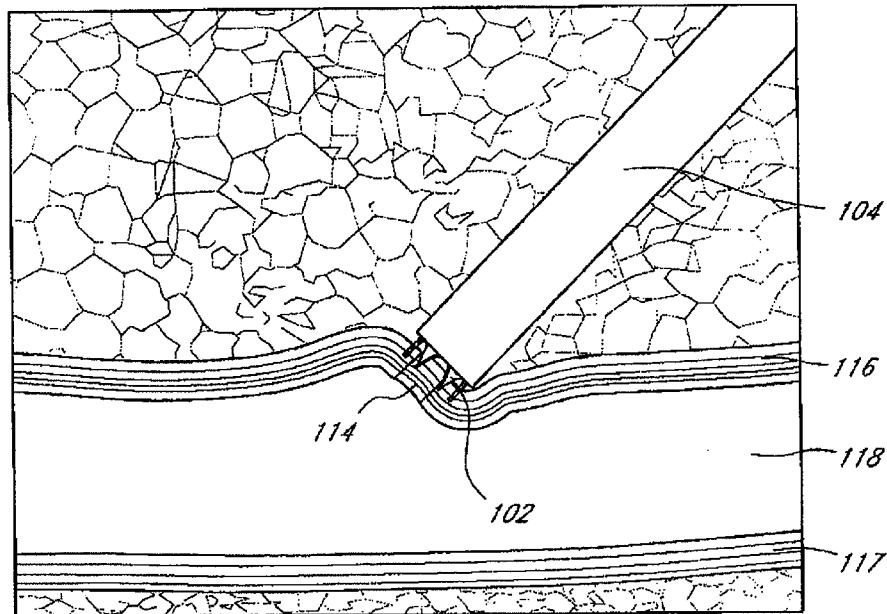


FIG. 28

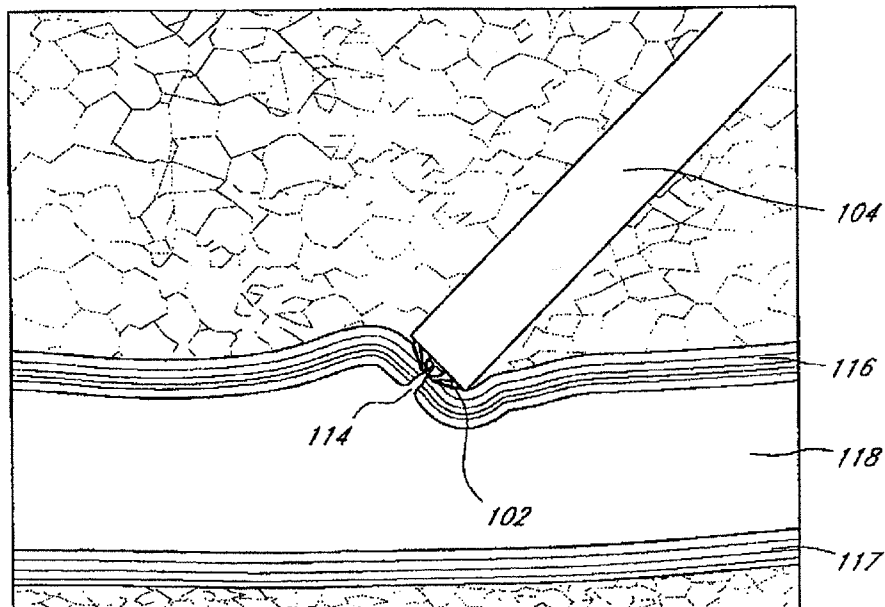


FIG. 31

30 / 98

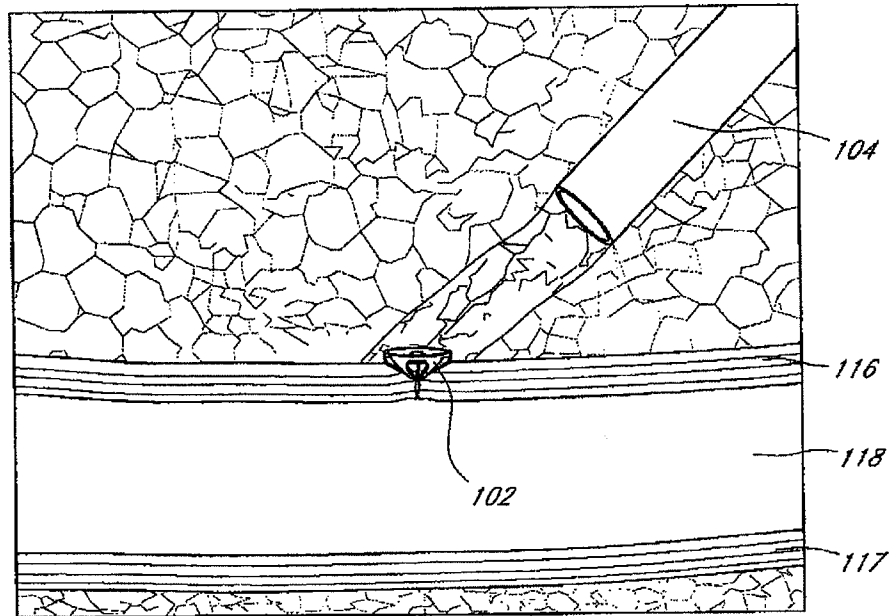


FIG. 32

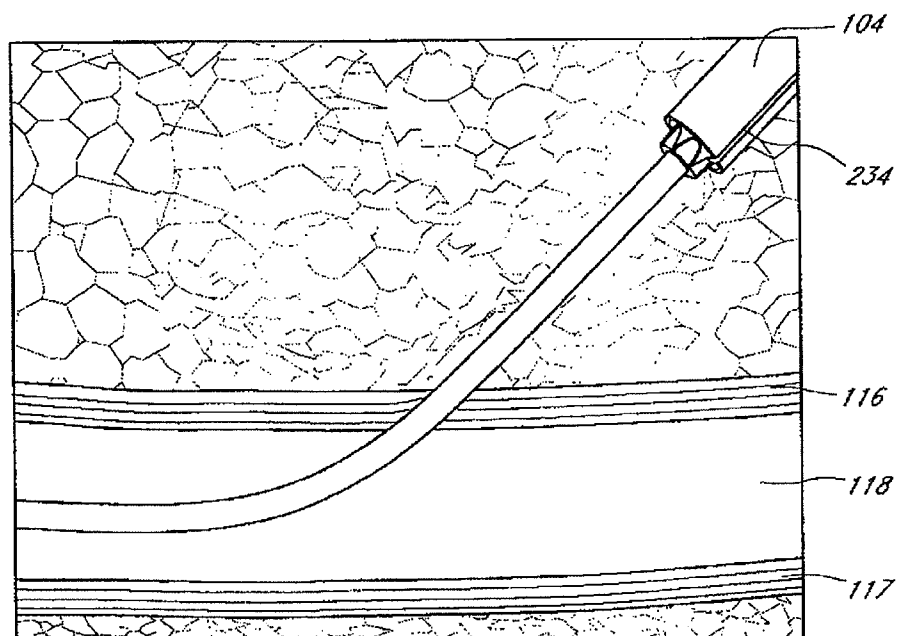


FIG. 33

31 / 98

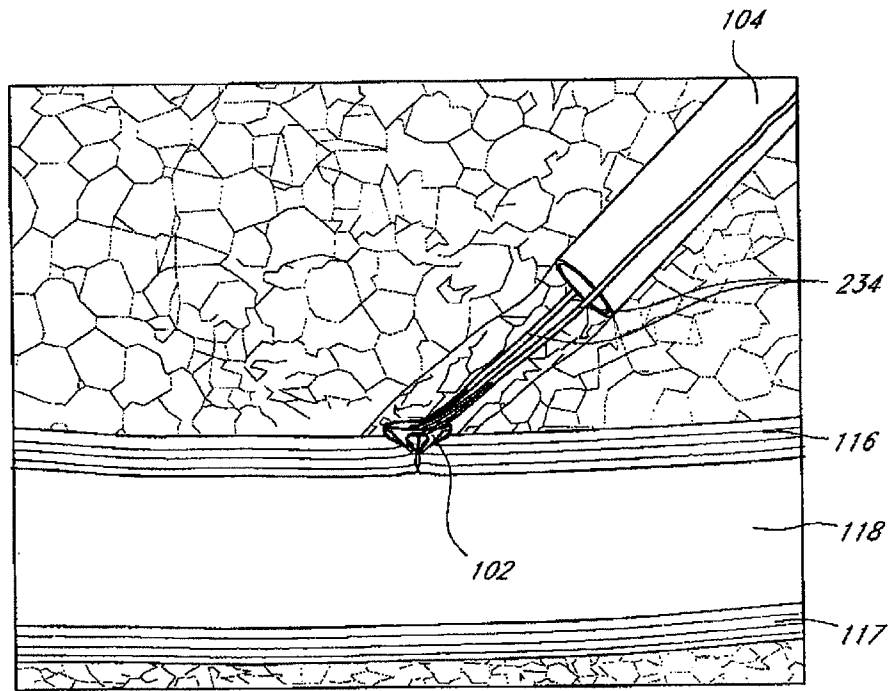


FIG. 34

32 / 98



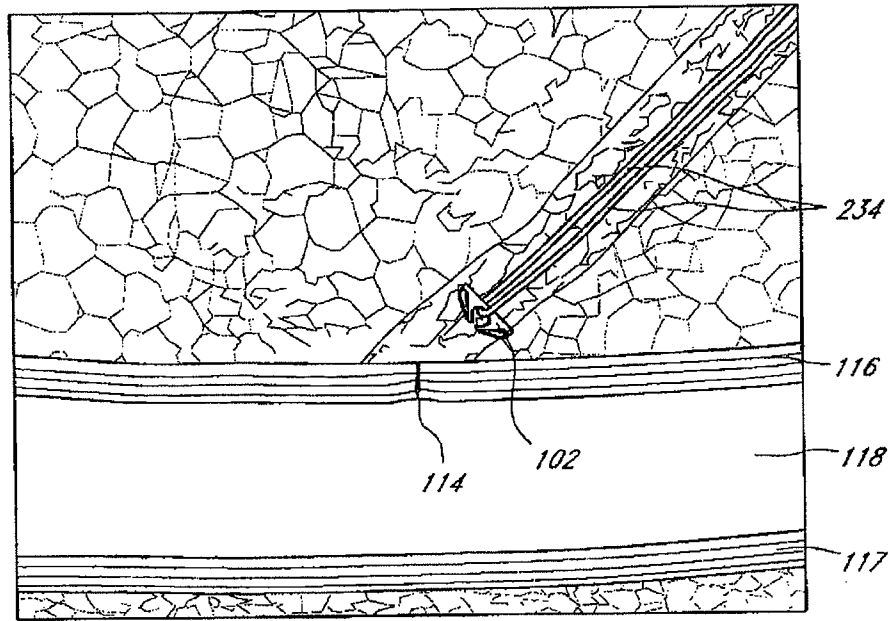


FIG. 35


33 / 98

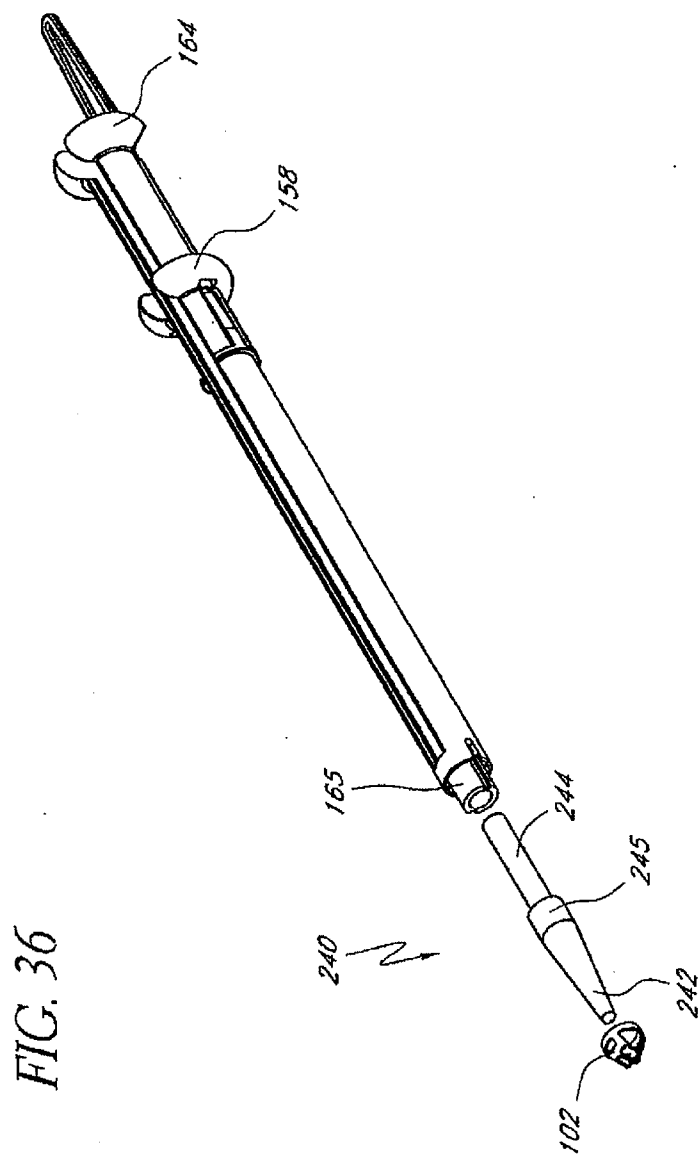


34 / 98

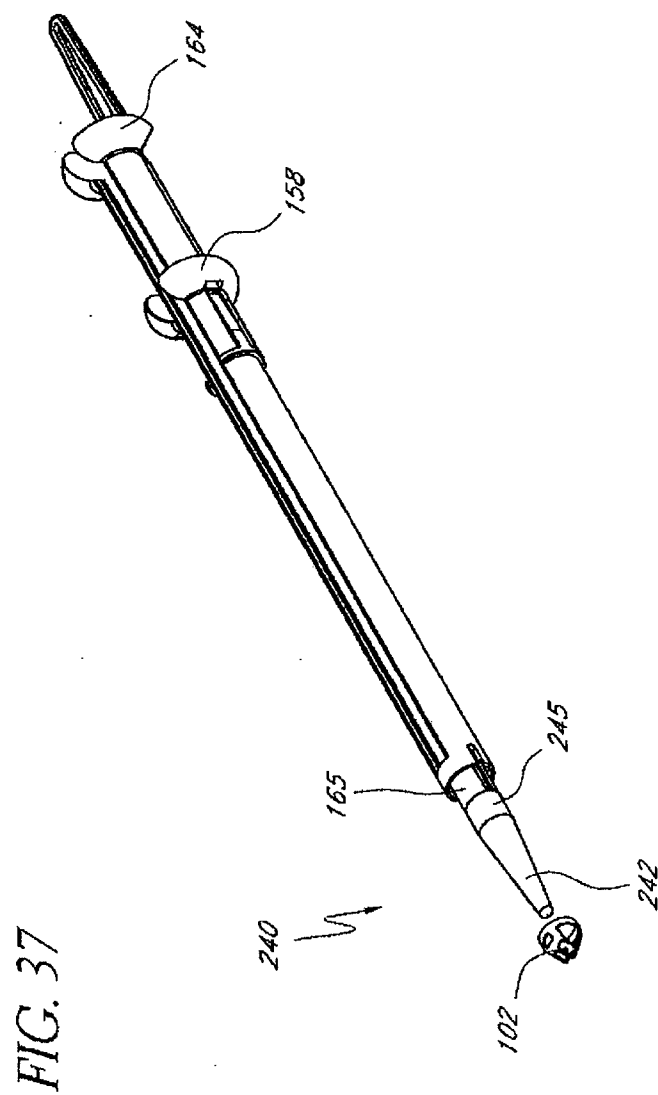


35 / 98

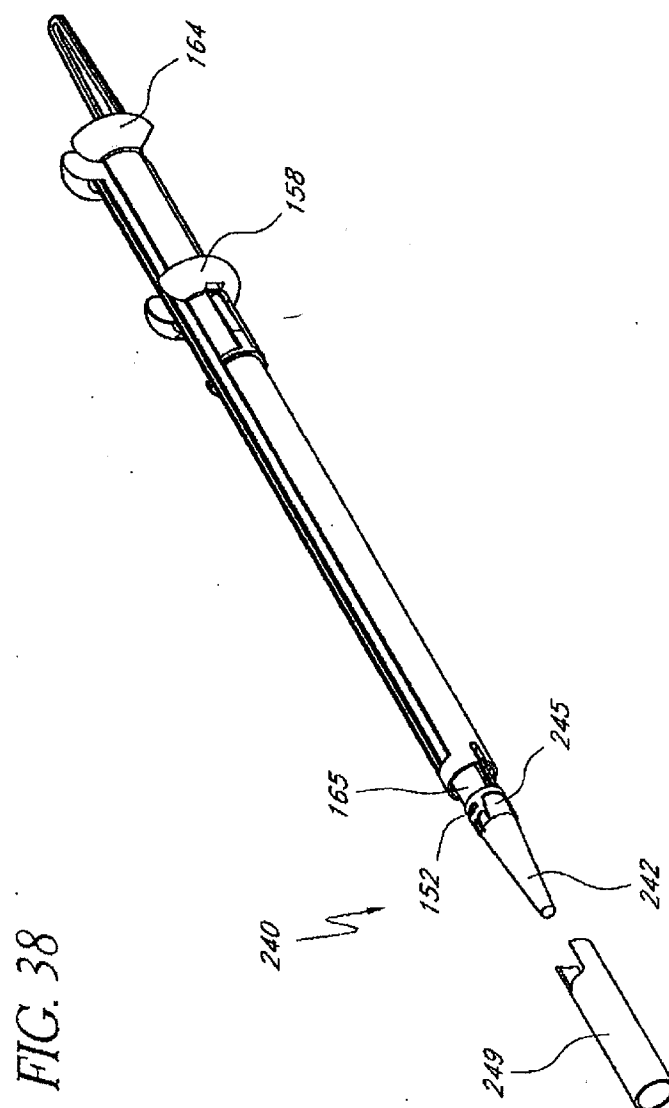

36 / 98

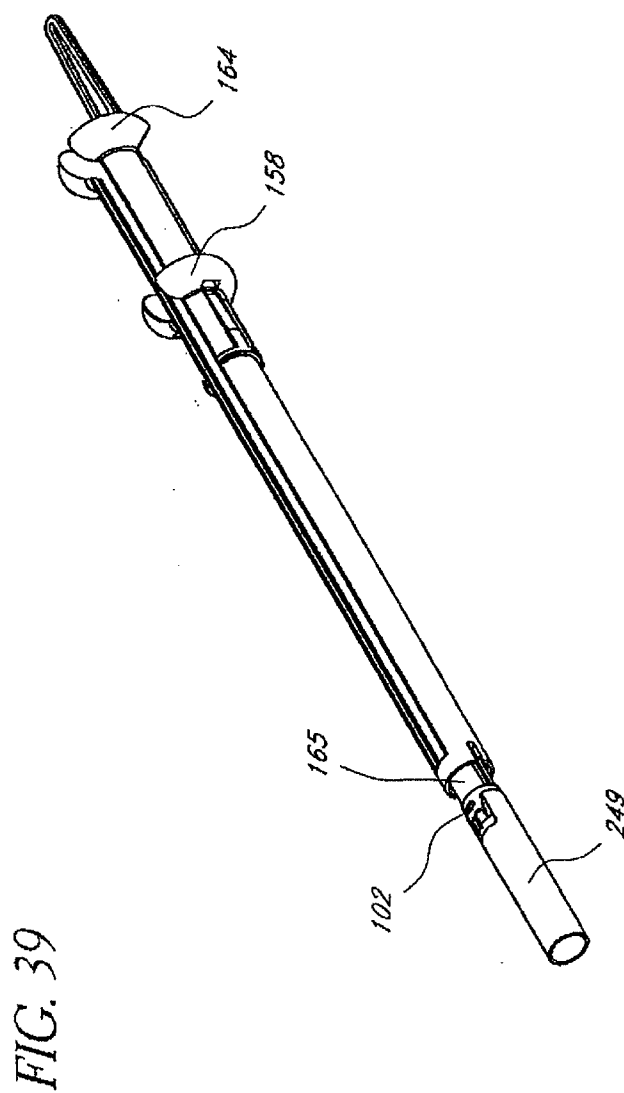


37 / 98

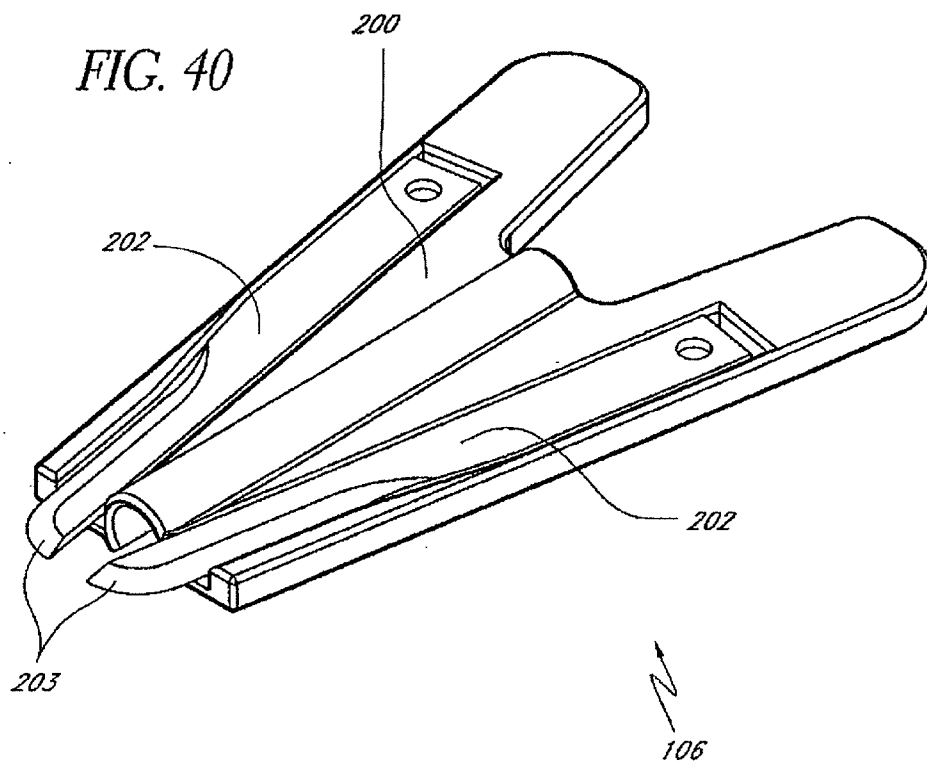


38 / 98

FIG. 41

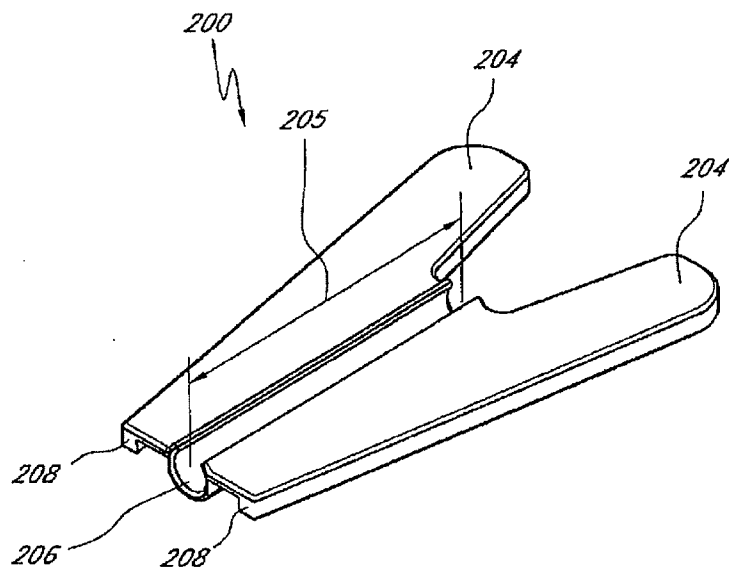


39 / 98

FIG. 42

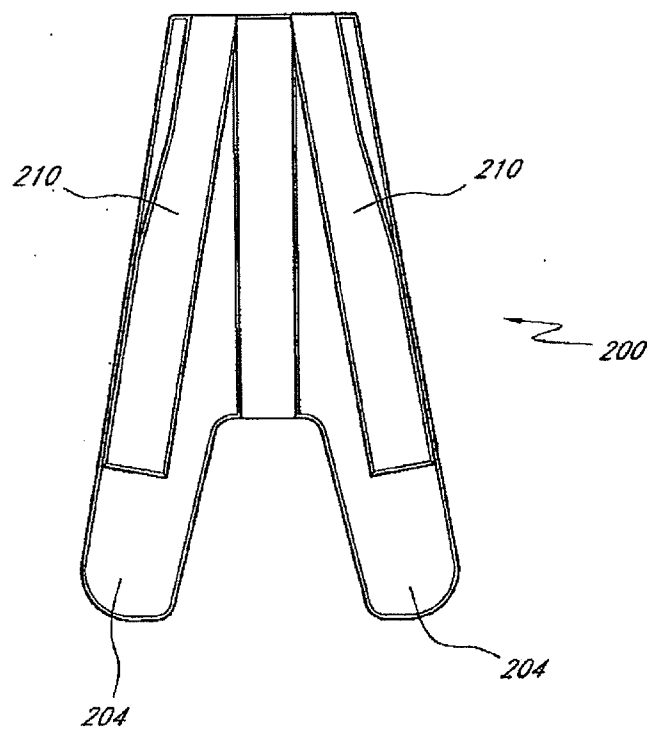

40 / 98

FIG. 43

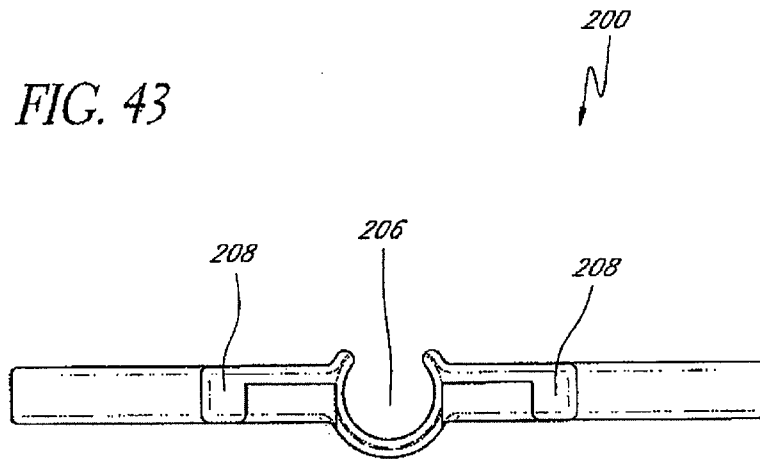

41 / 98

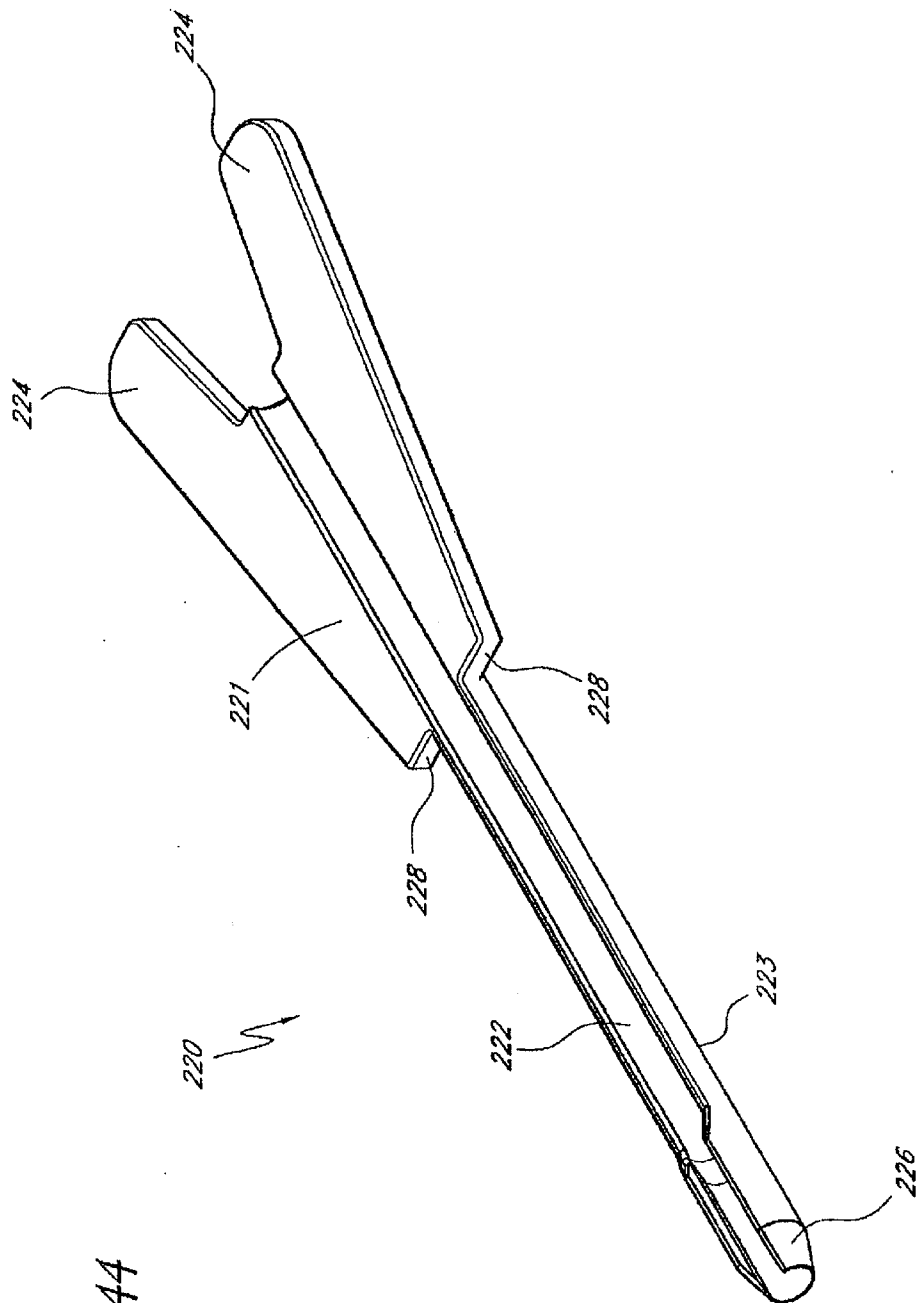


FIG. 44

42 / 98

FIG. 45



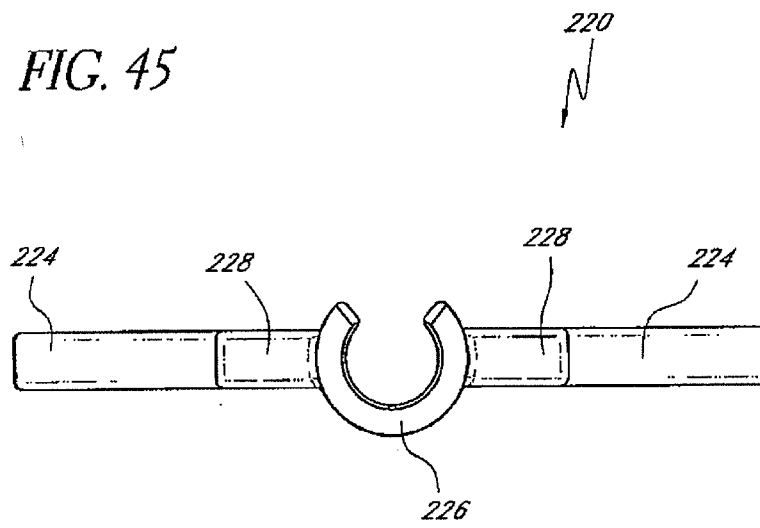


FIG. 46

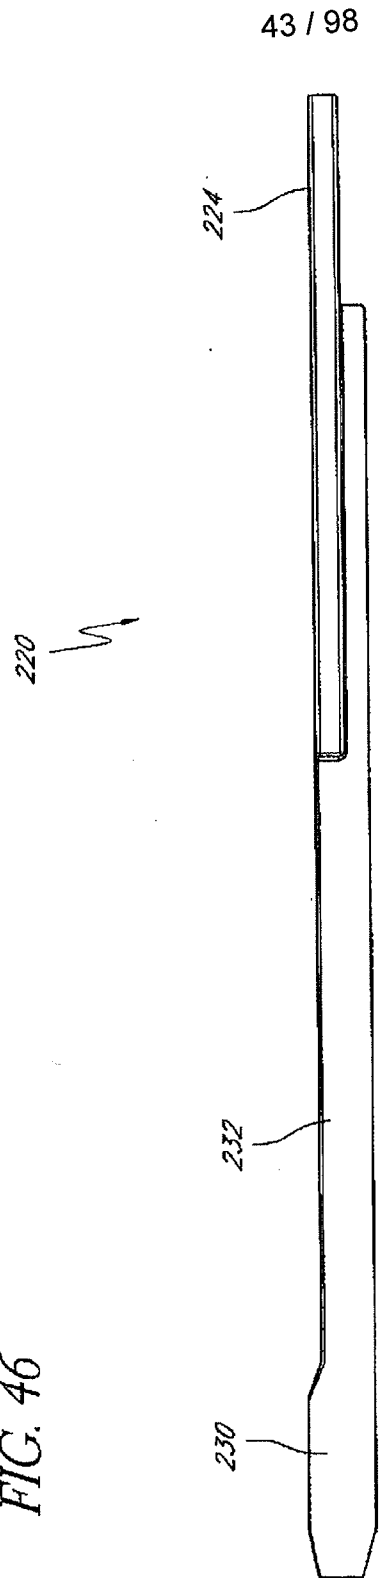

44 / 98

FIG. 47A

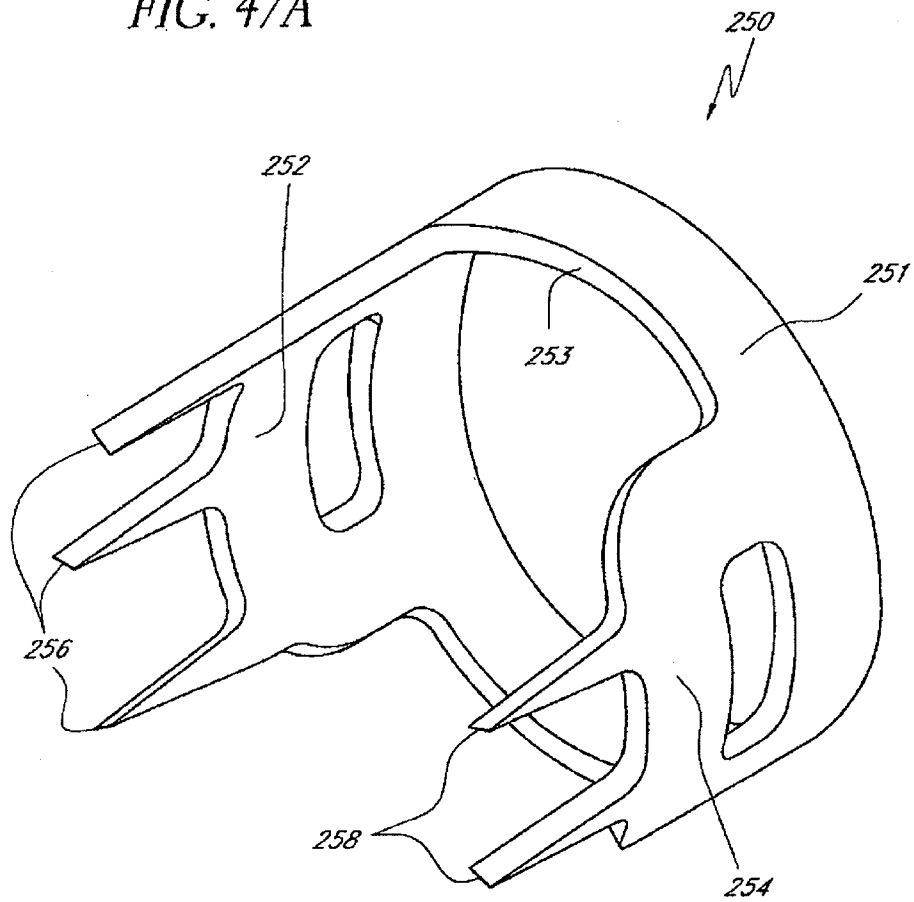

45 / 98

FIG. 47B



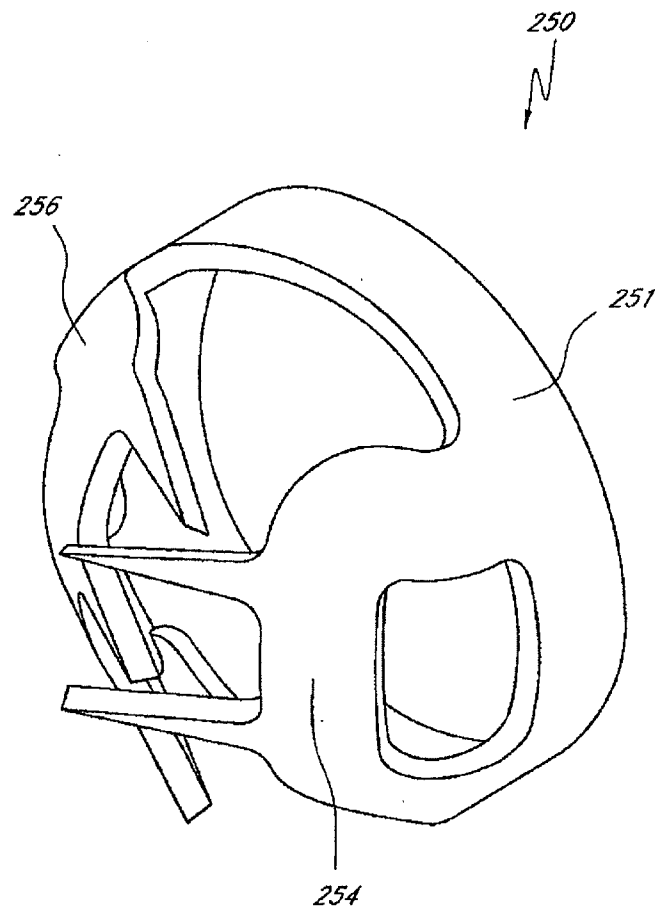


FIG. 47C

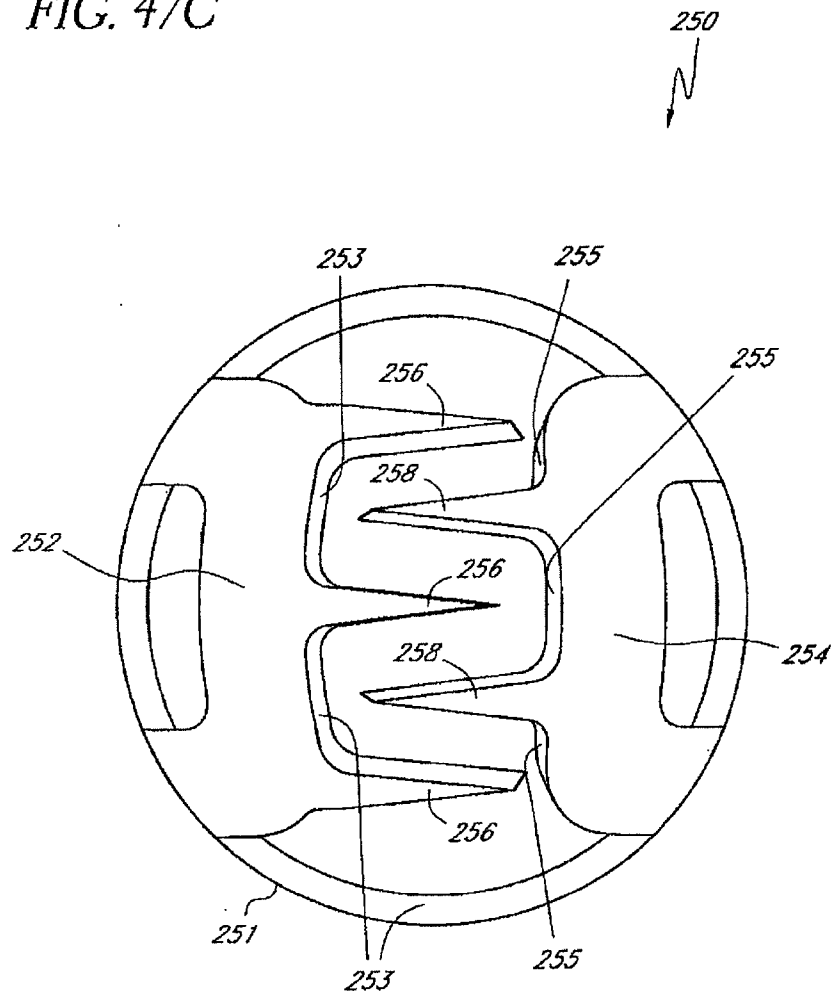


47 / 98

FIG. 47D

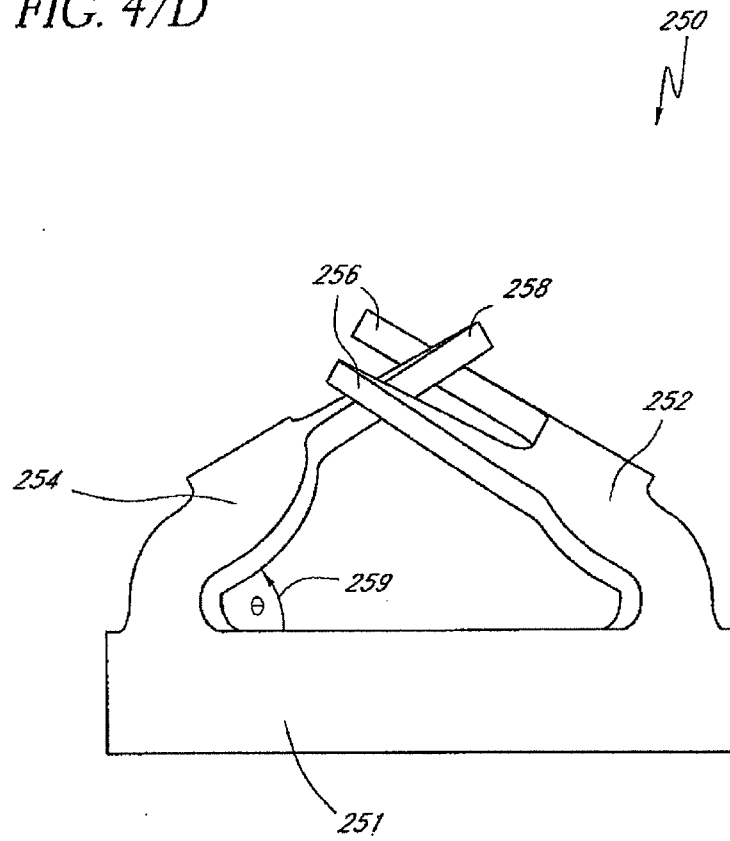


48 / 98

FIG. 48A

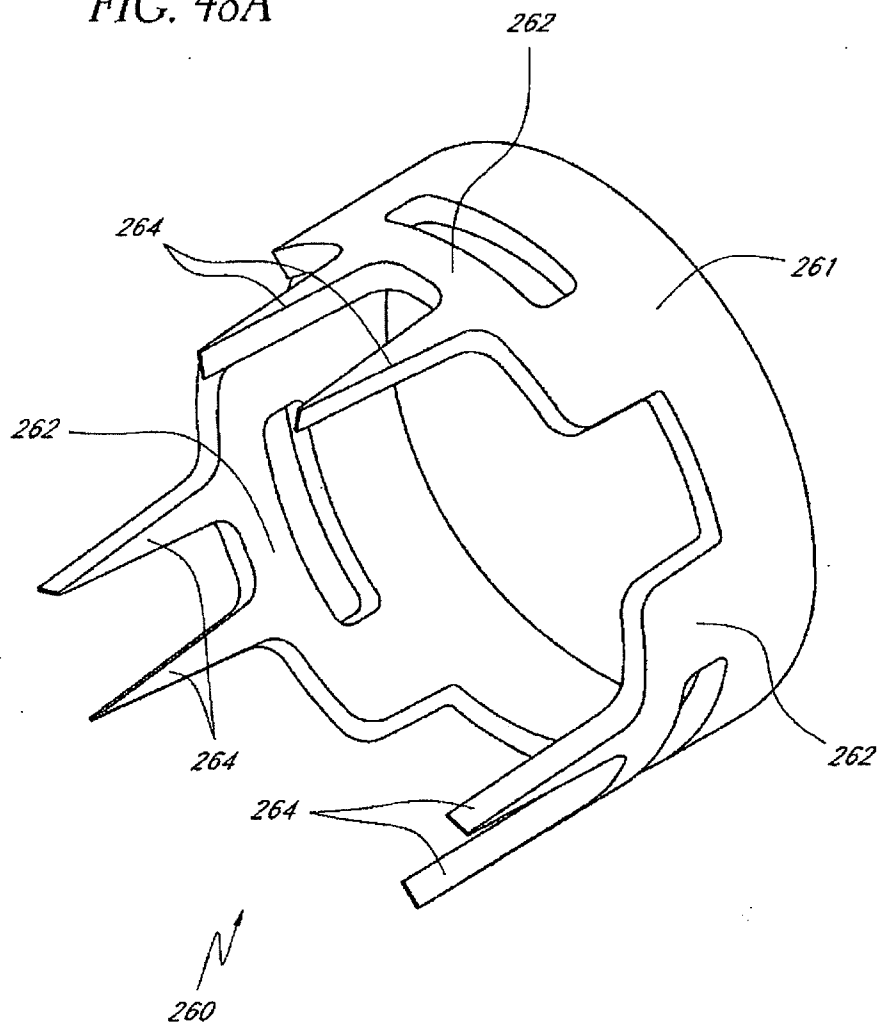


49 / 98

FIG. 48B

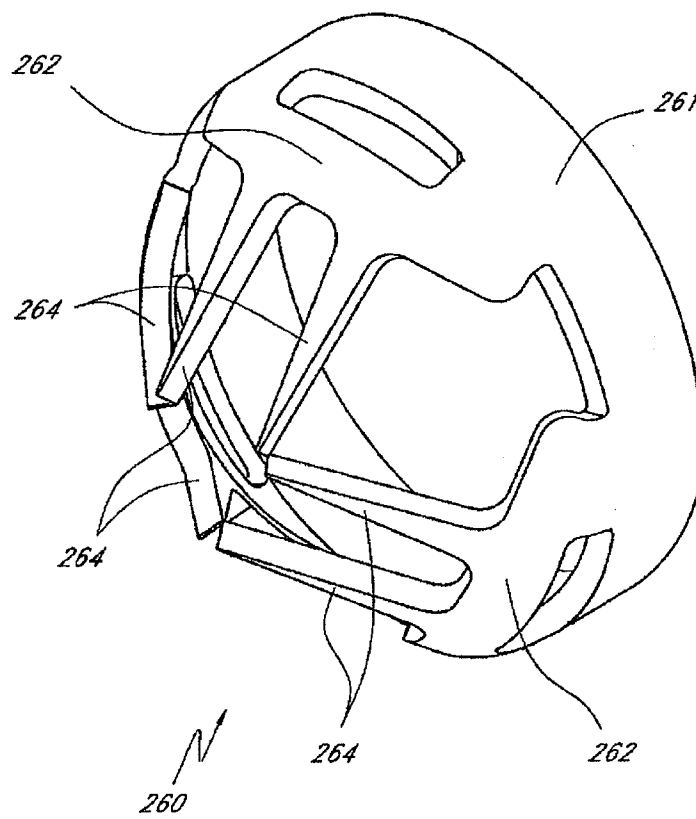


50 / 98

FIG. 49A

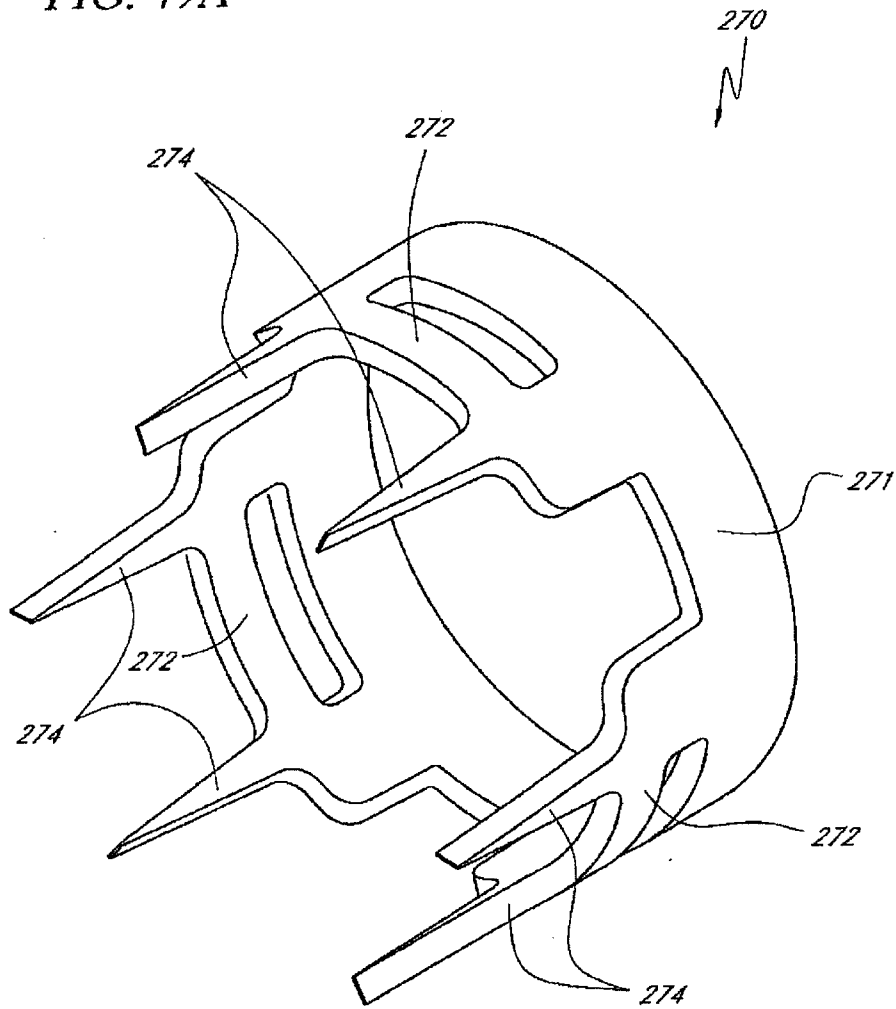


51 / 98

FIG. 49B

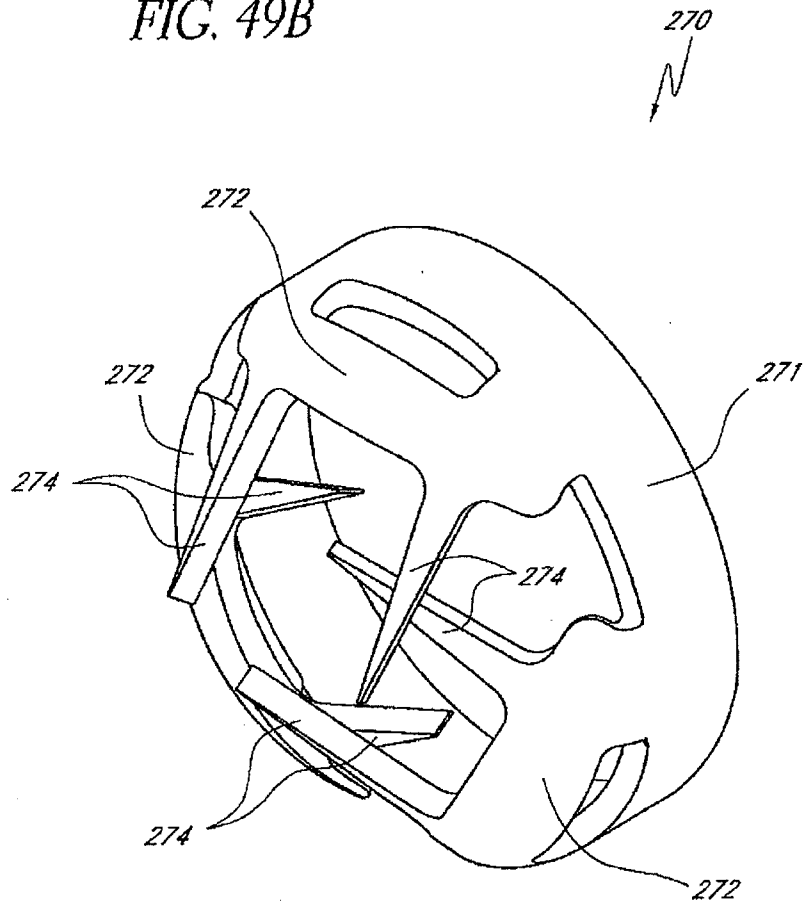


52 / 98

FIG. 50A

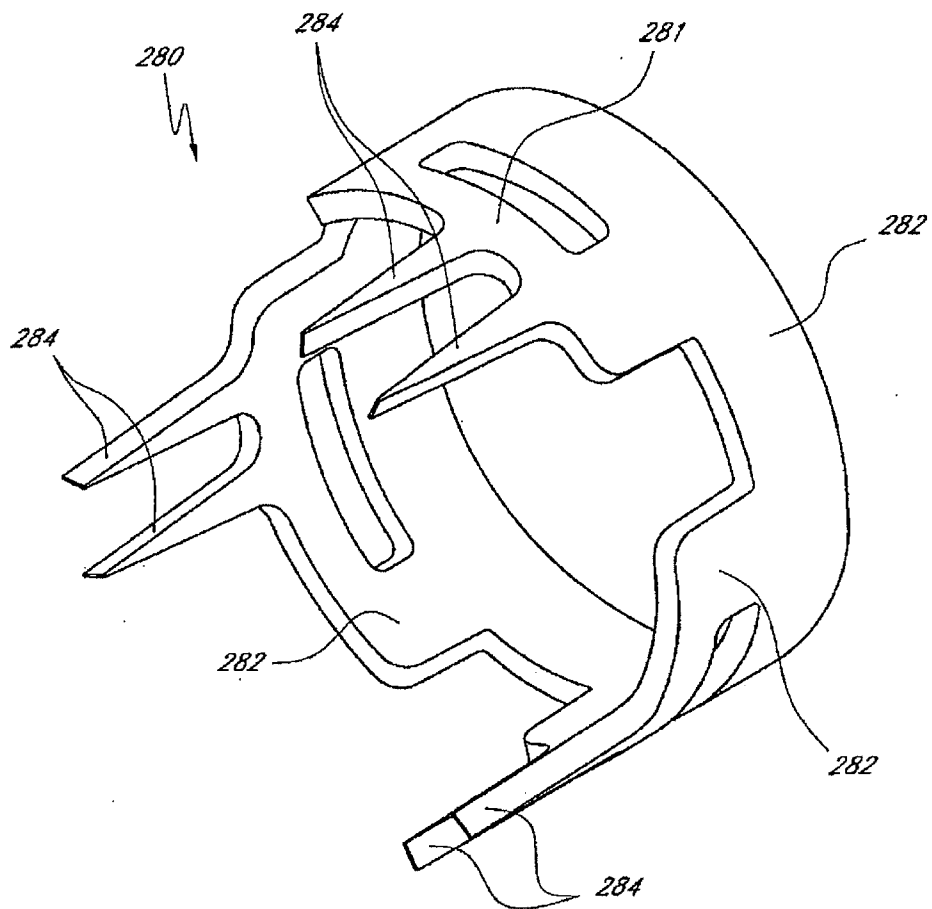


53 / 98

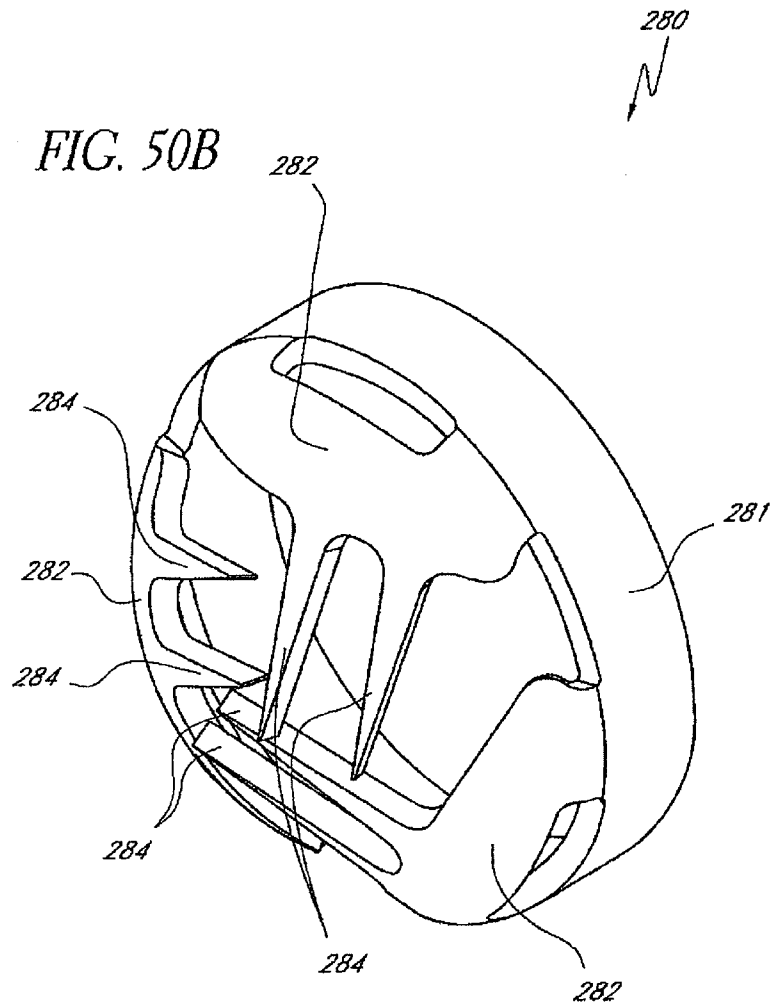


54 / 98

FIG. 51A

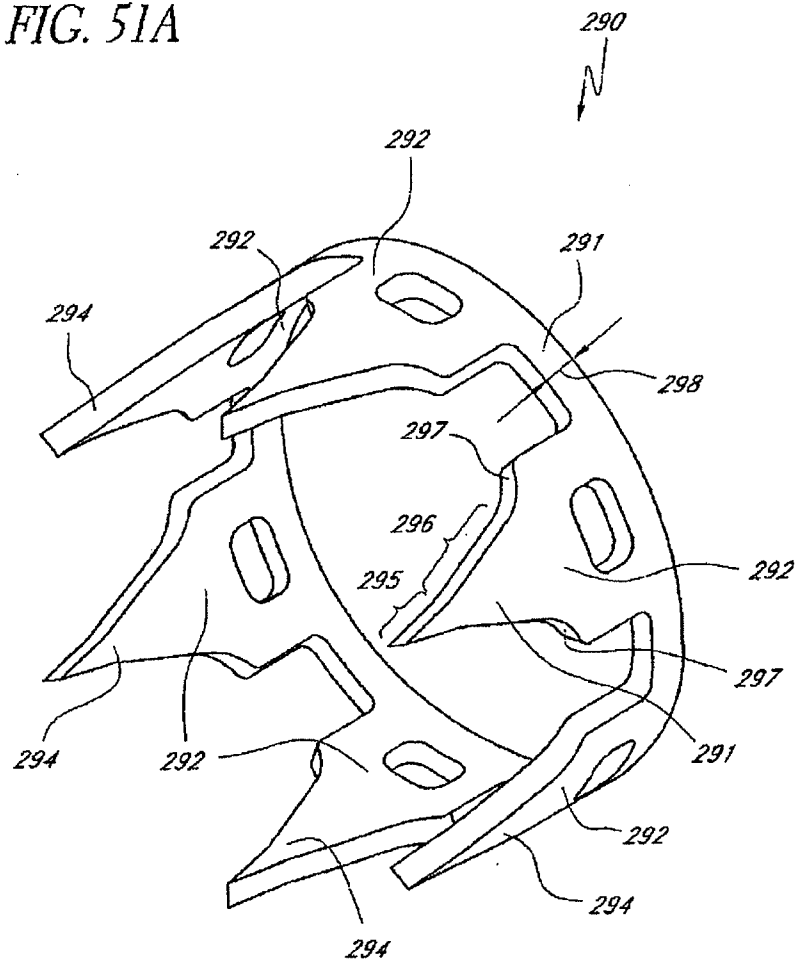


55 / 98

FIG. 51B

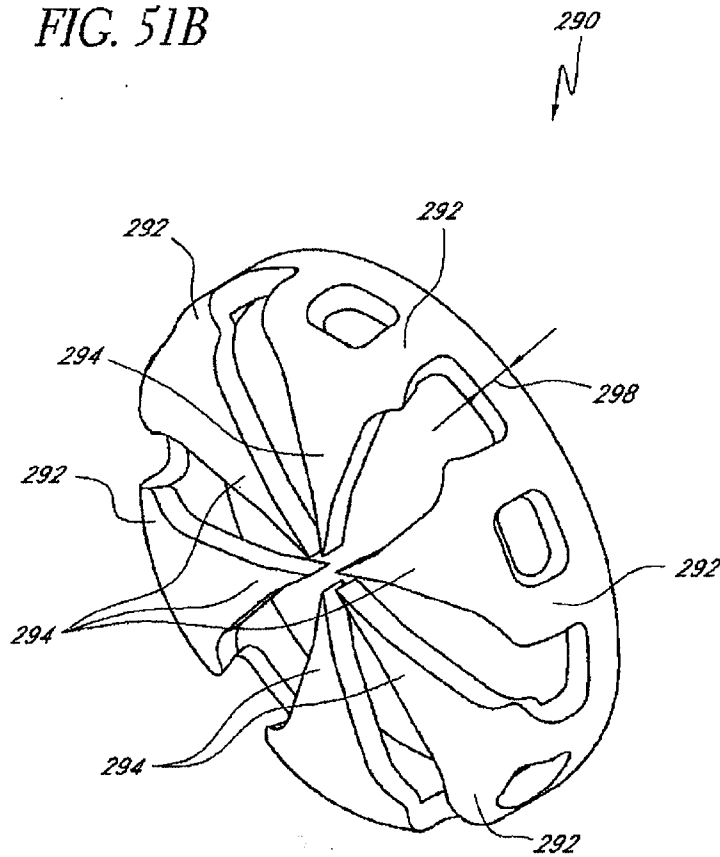



56 / 98

FIG. 51C

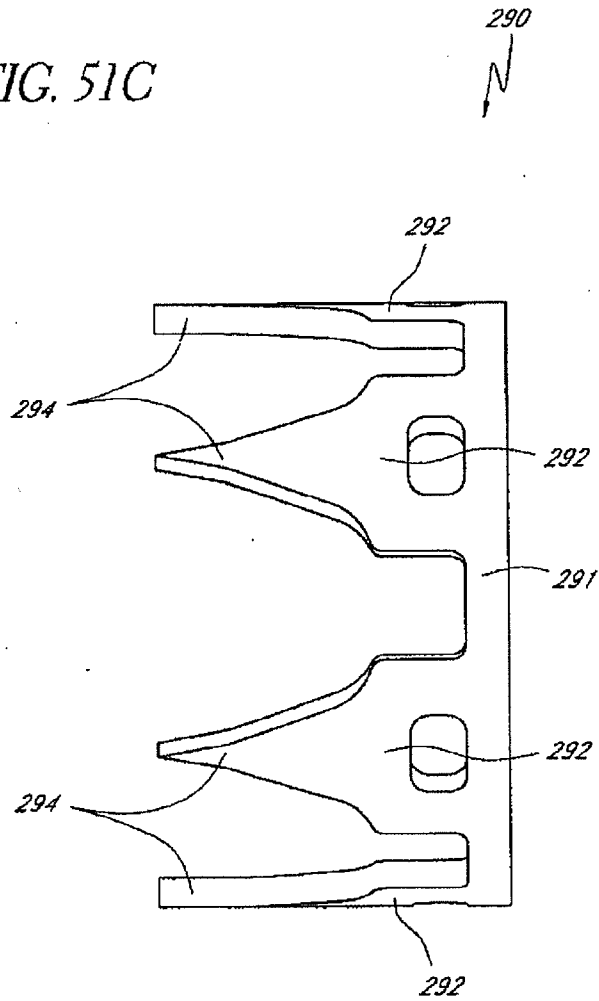


57 / 98

FIG. 51D

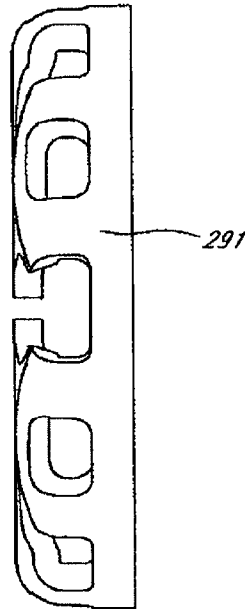

58 / 98

FIG. 51E

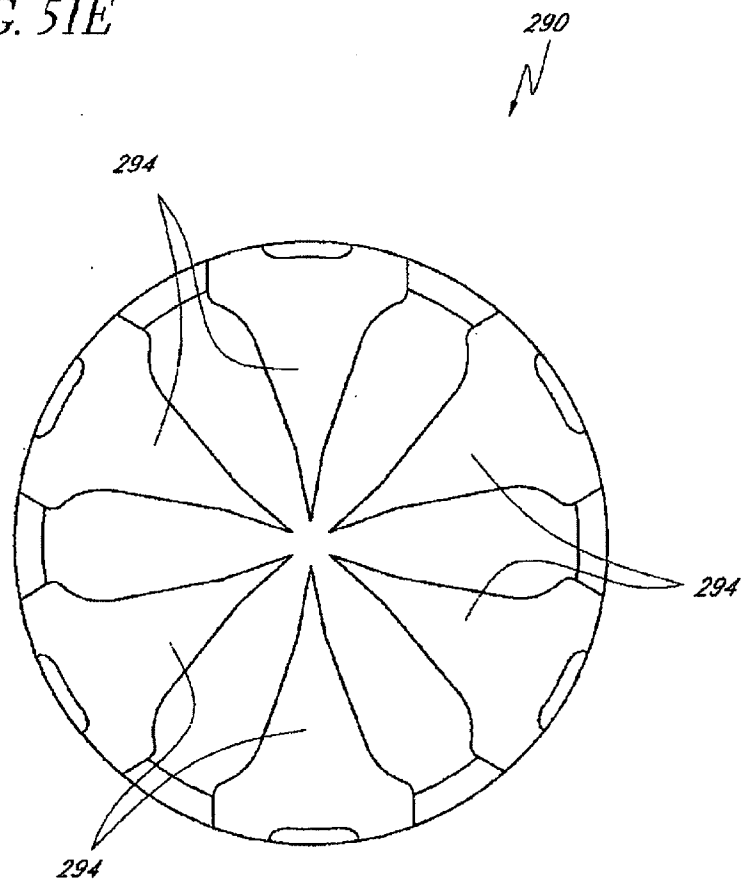

59 / 98

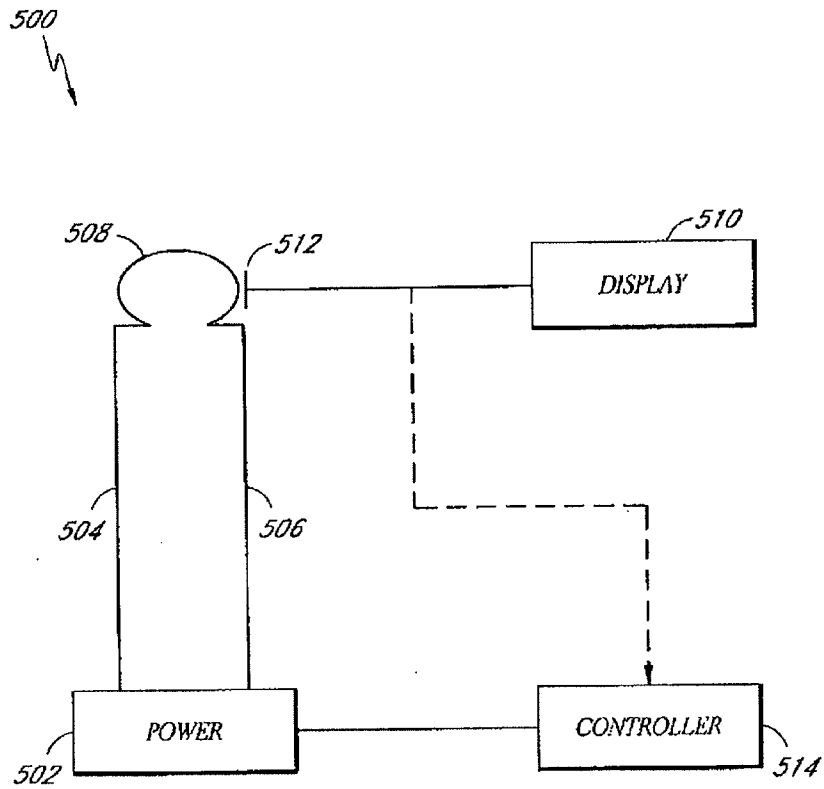


FIG. 52

60 / 98


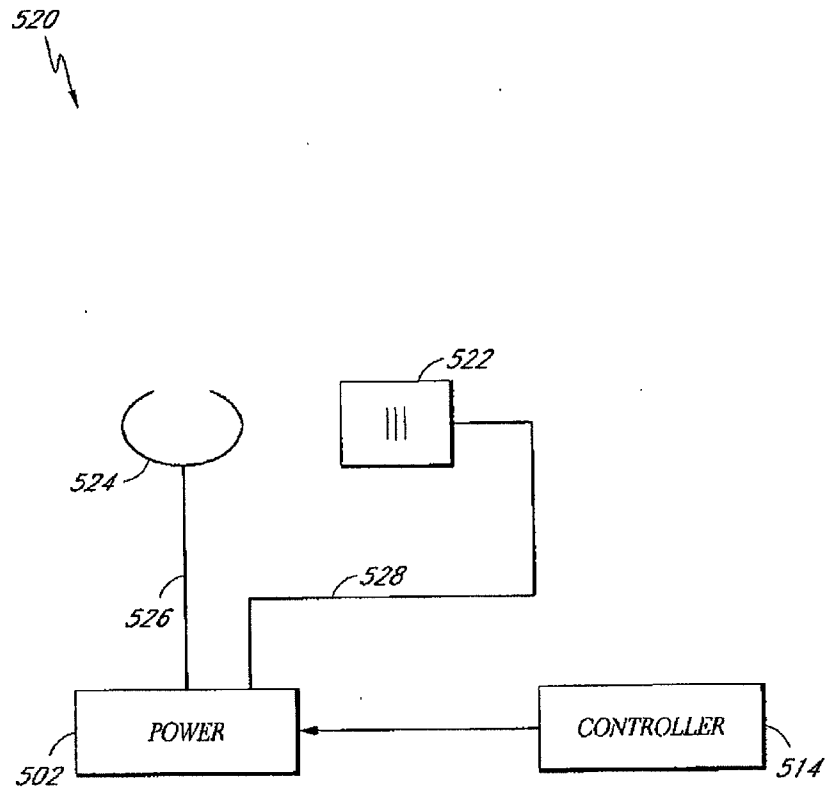



FIG. 53

FIG. 54



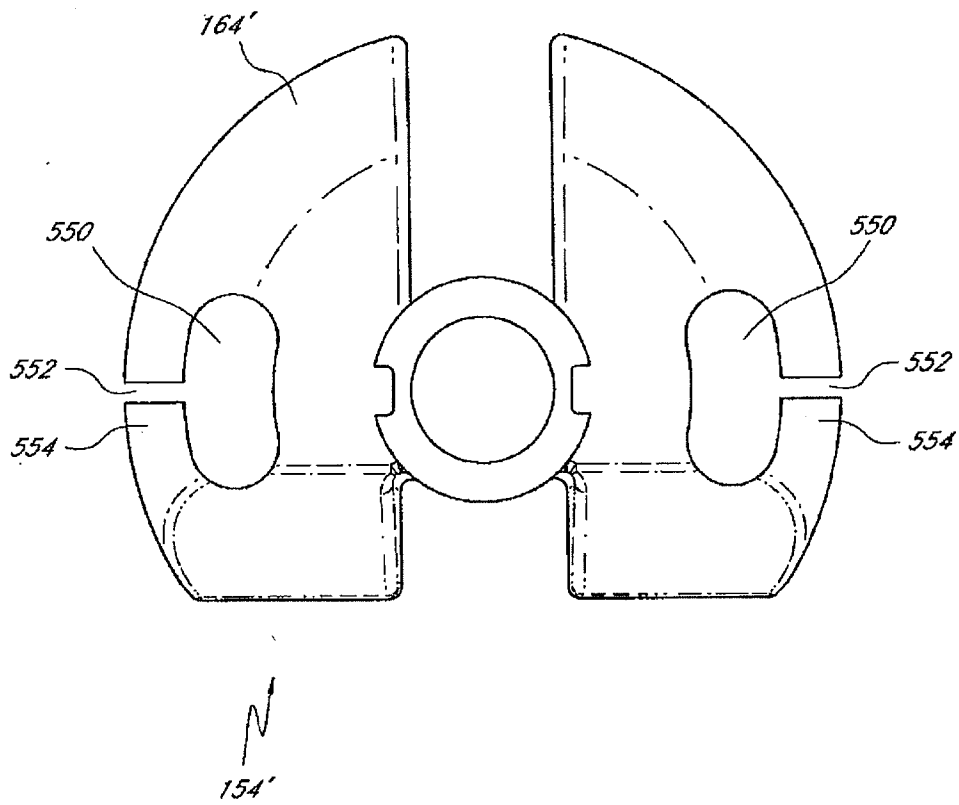


62 / 98

FIG. 55

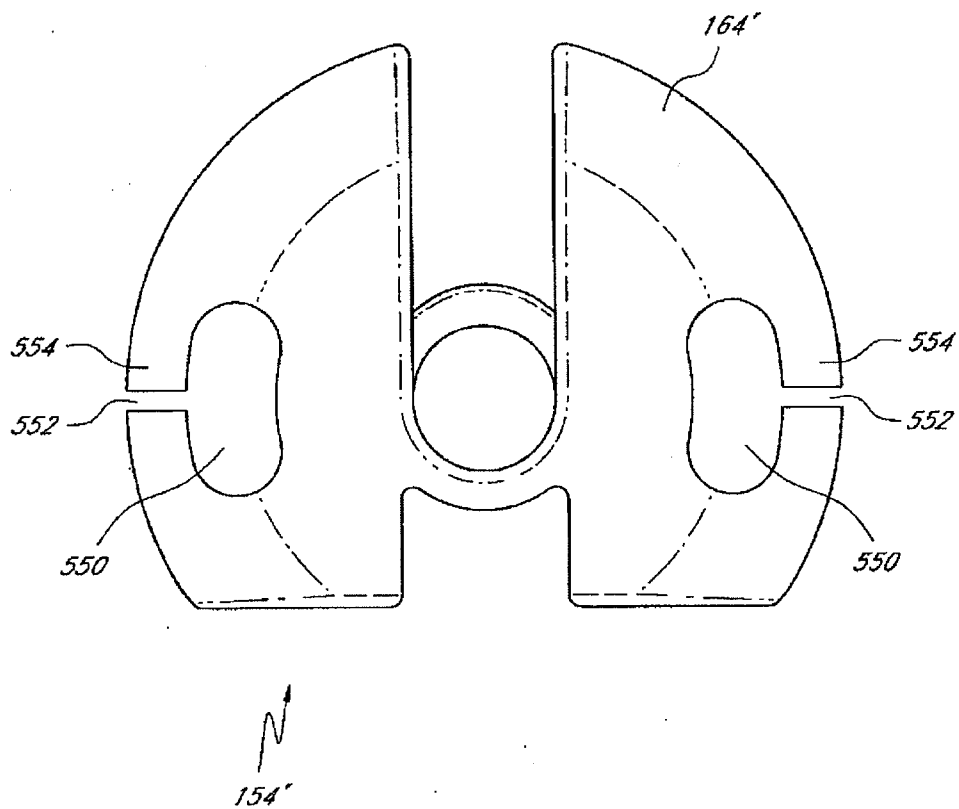

63 / 98

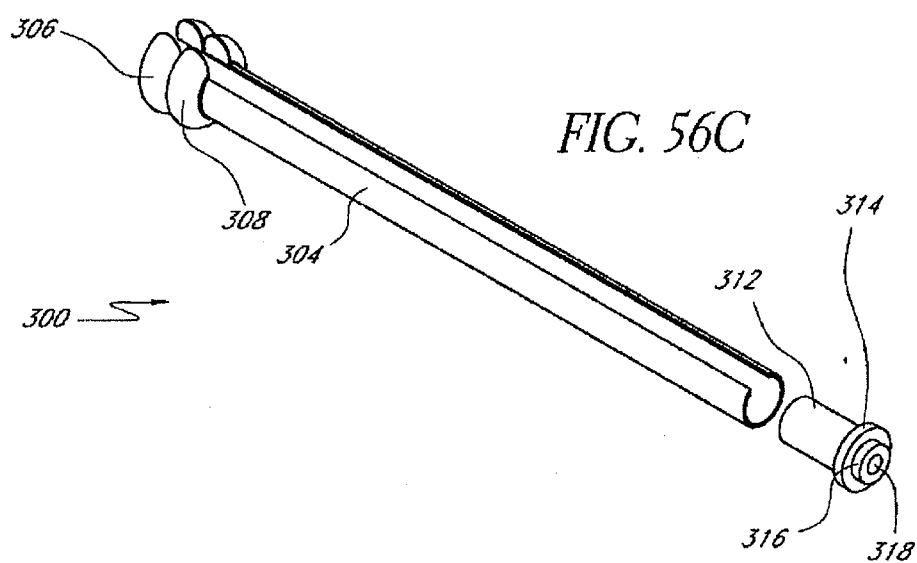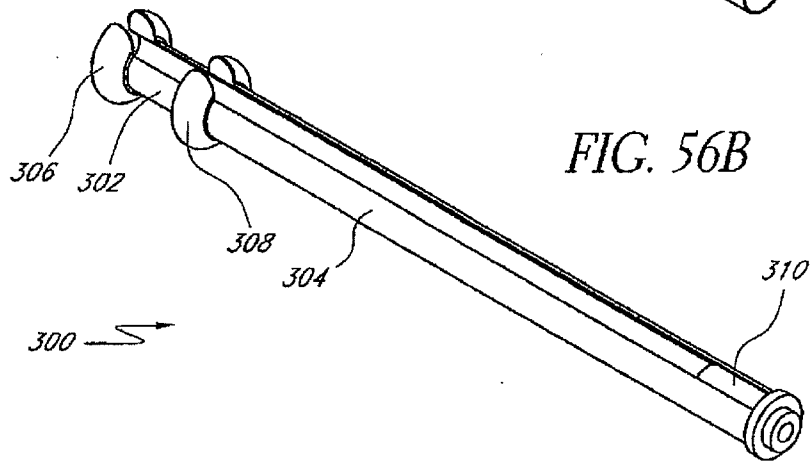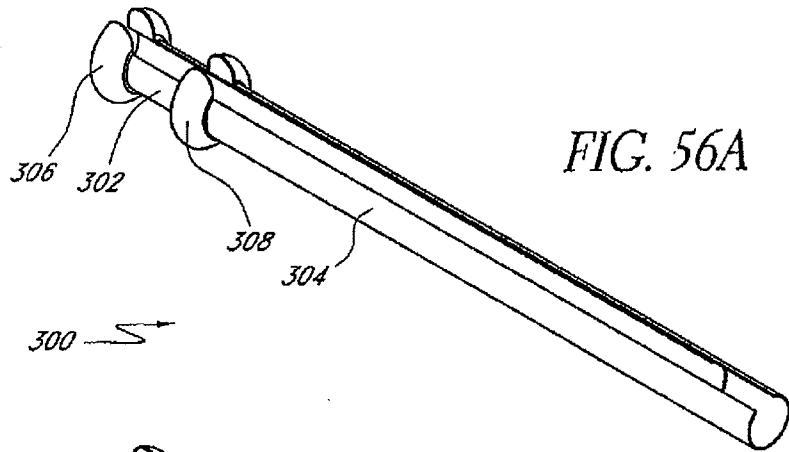

64 / 98

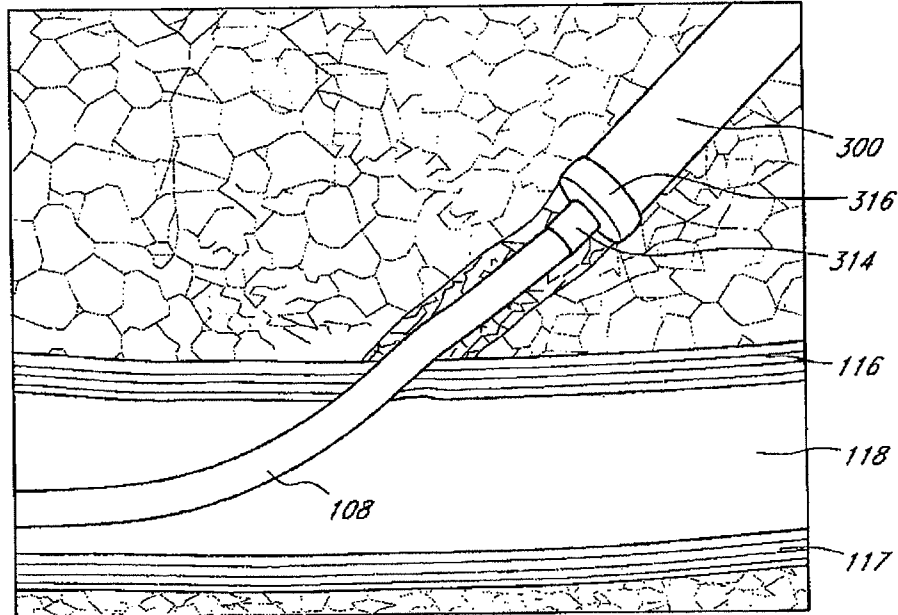


FIG. 57

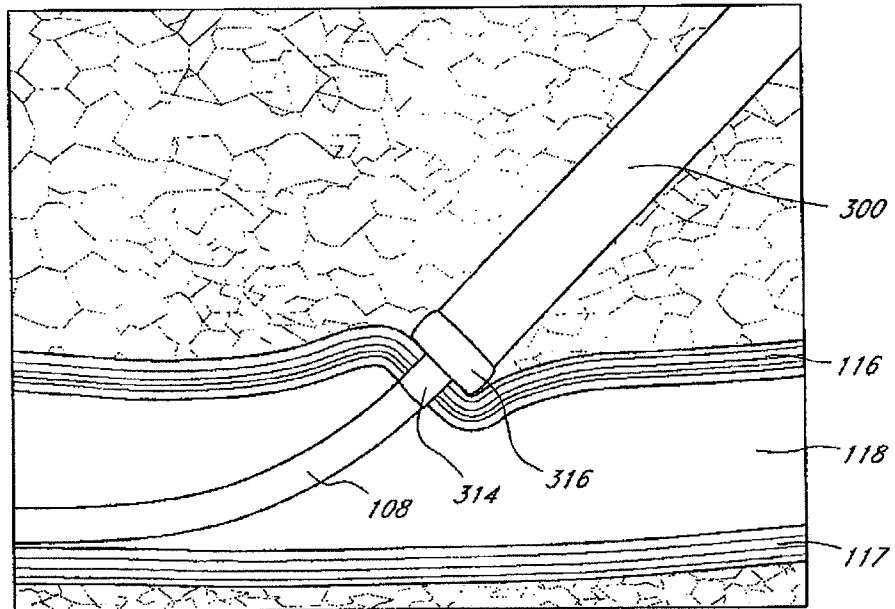


FIG. 58

65 / 98

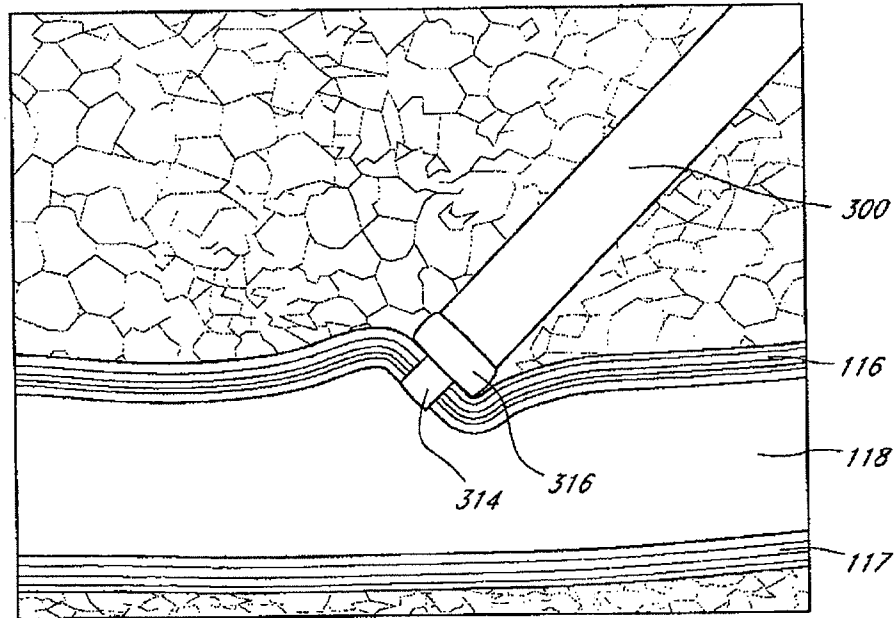


FIG. 59

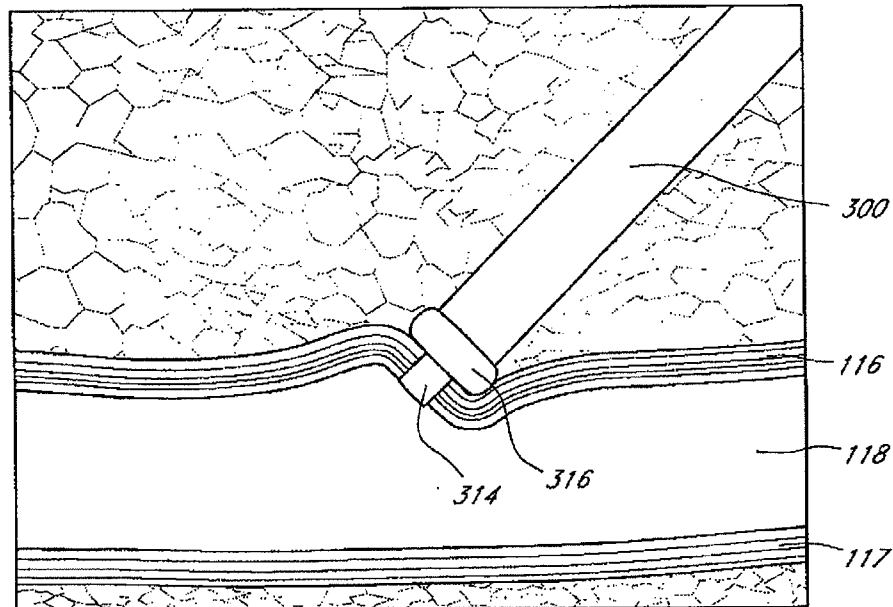


FIG. 60

66 / 98

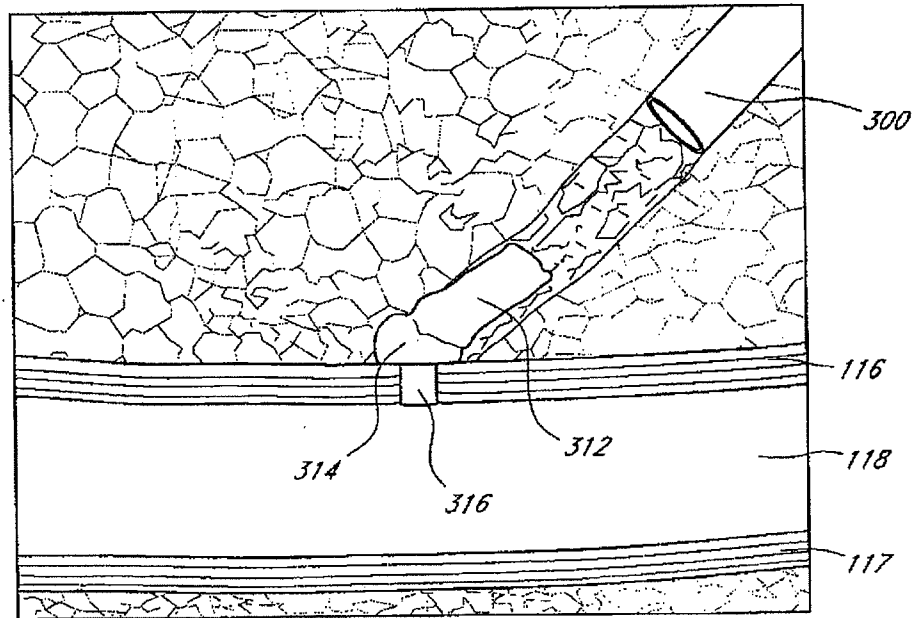


FIG. 61

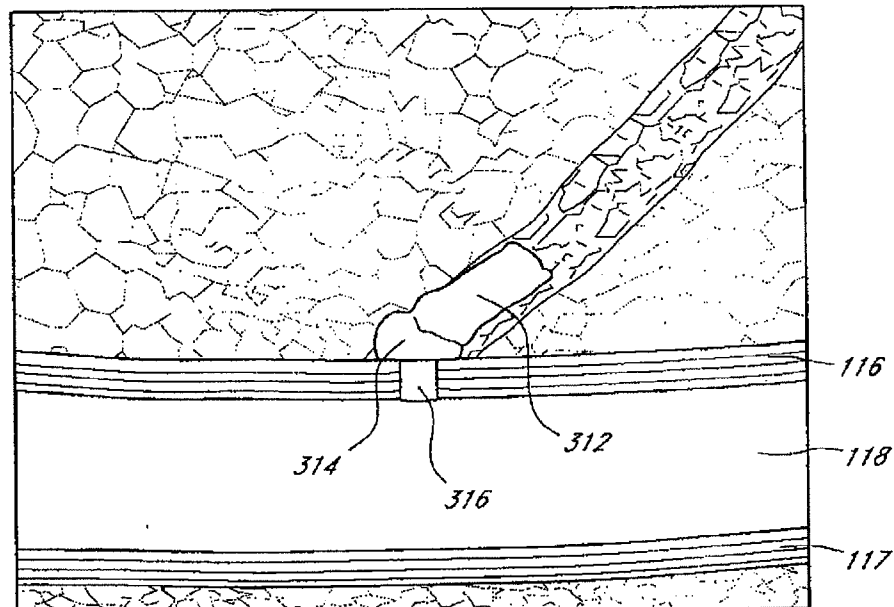


FIG. 62

67 / 98

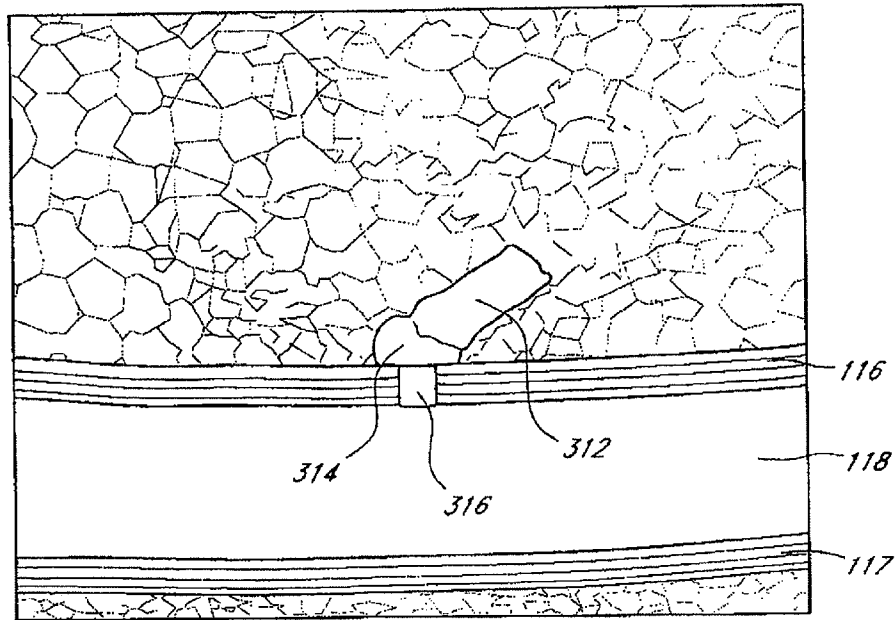
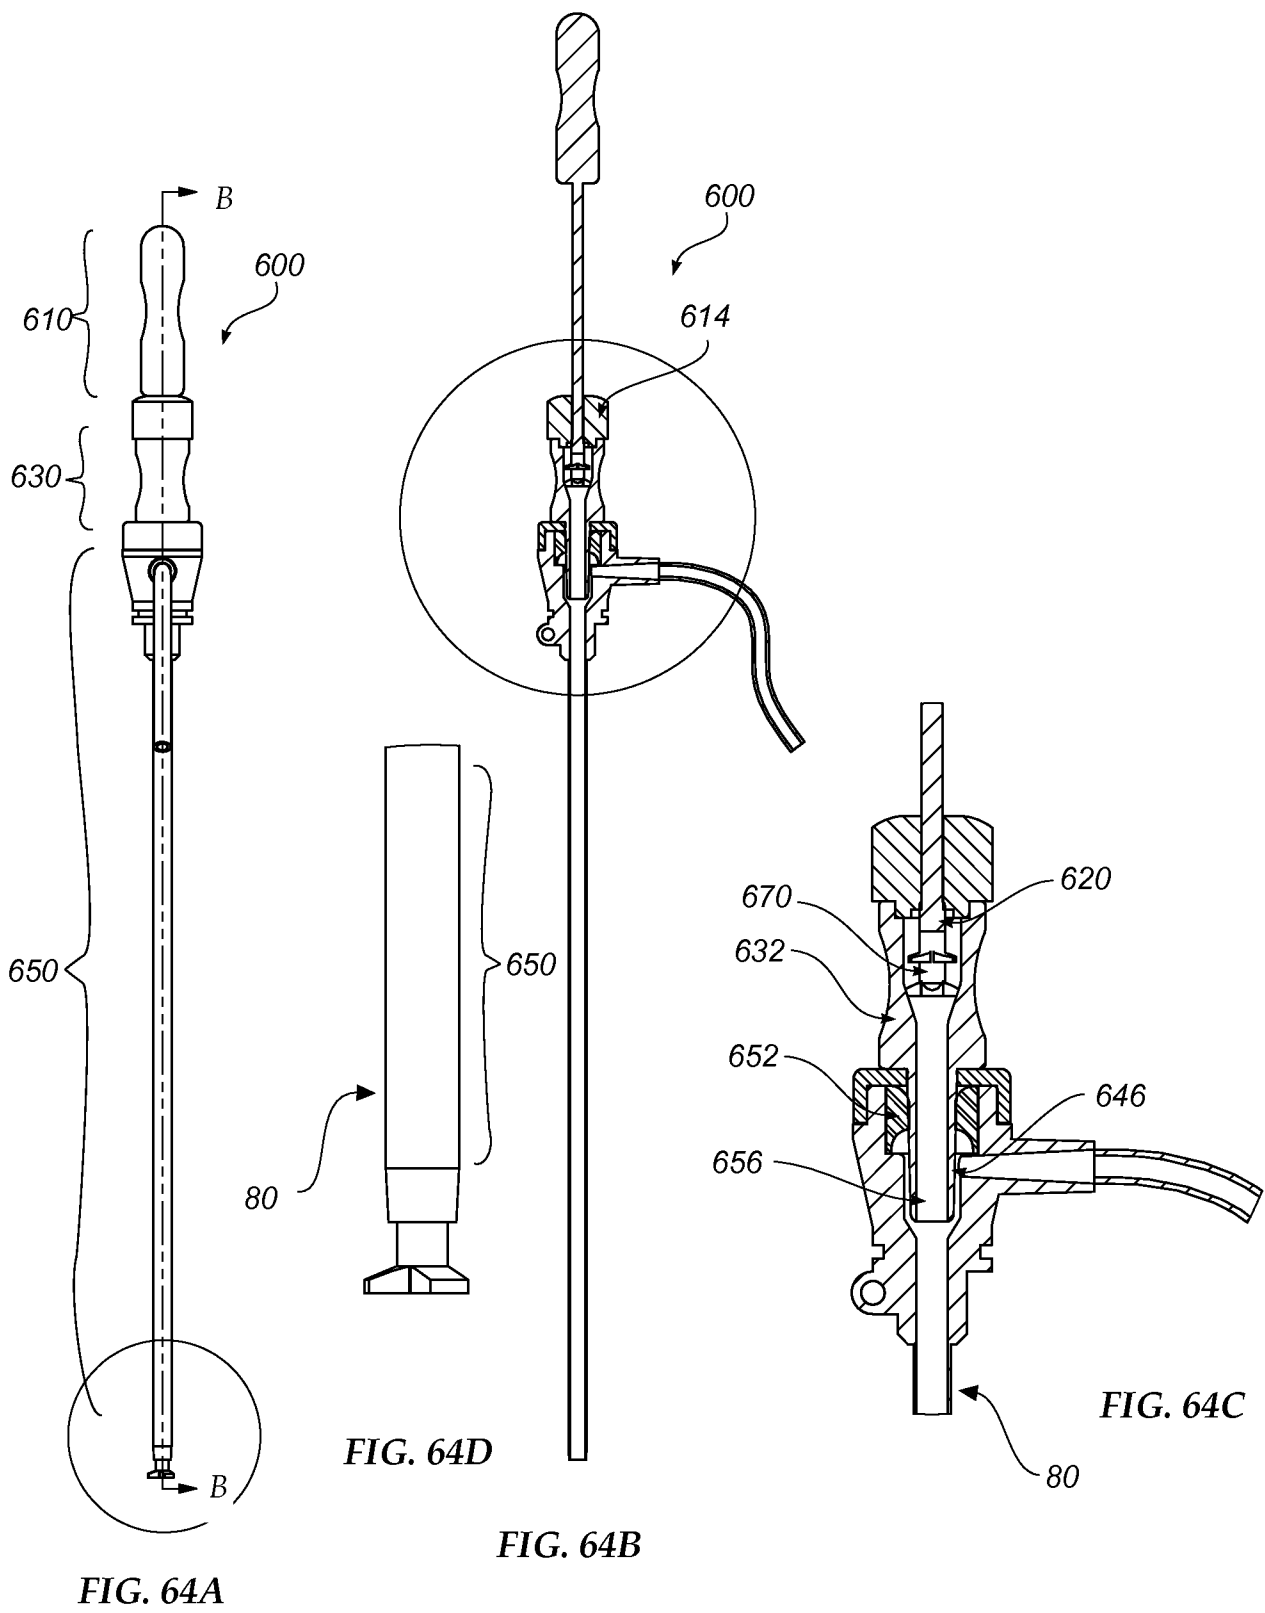


FIG. 63

68/98



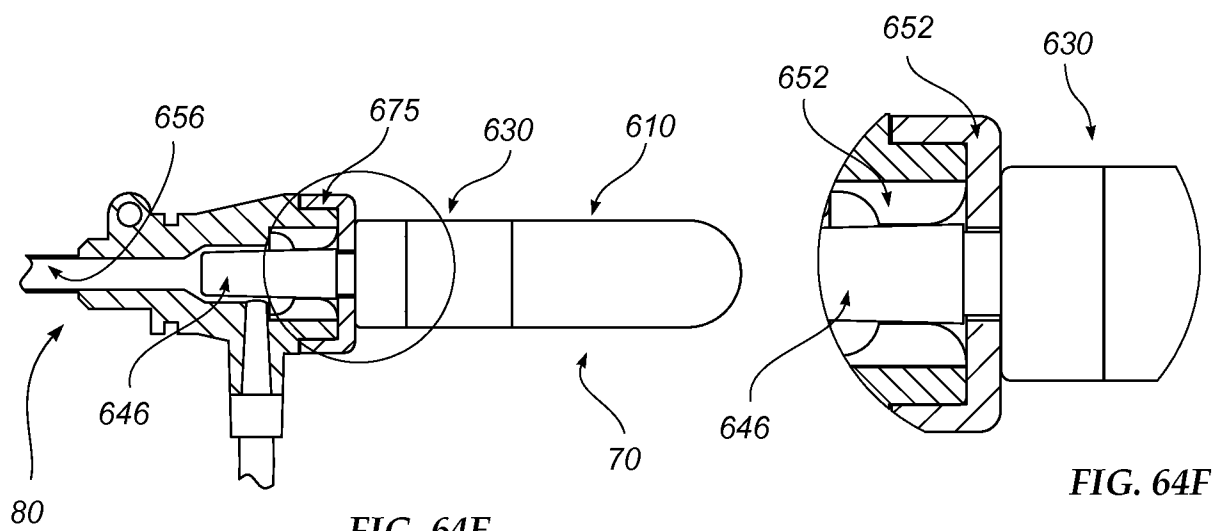


FIG. 64E

FIG. 64F

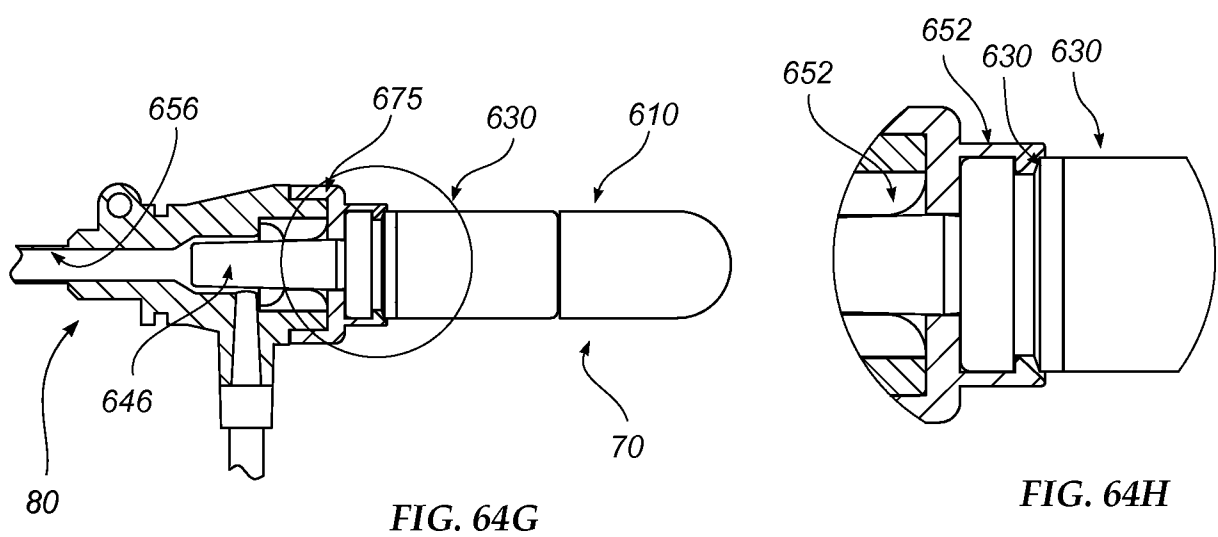


FIG. 64G

FIG. 64H

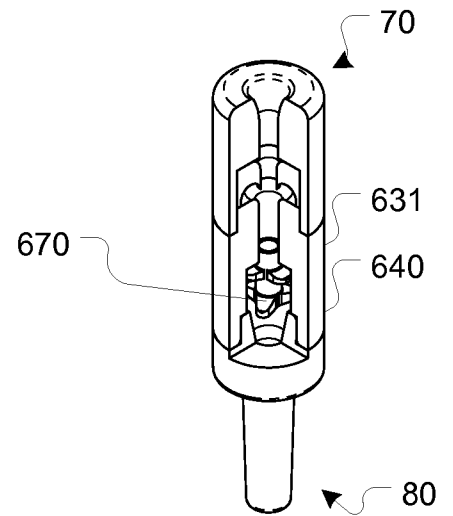


FIG. 65A

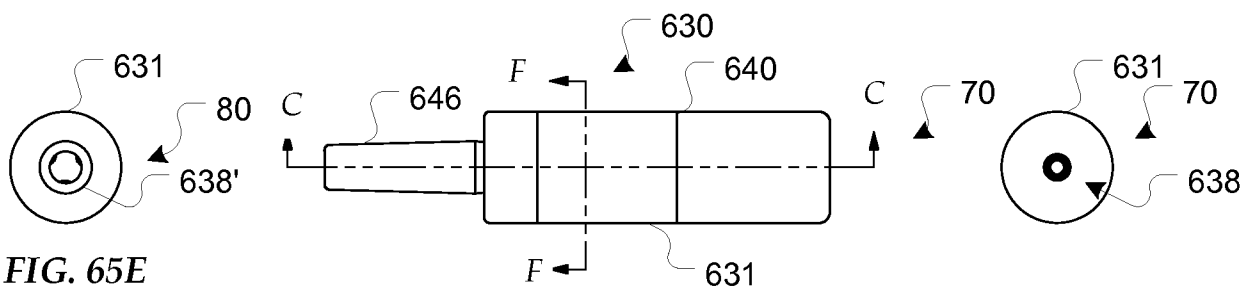


FIG. 65E

FIG. 65B

FIG. 65D

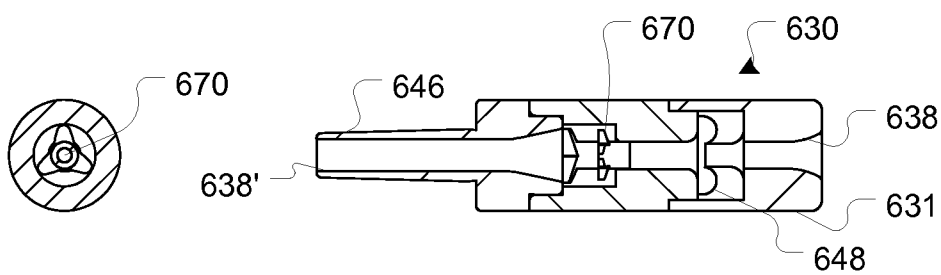


FIG. 65F

FIG. 65C

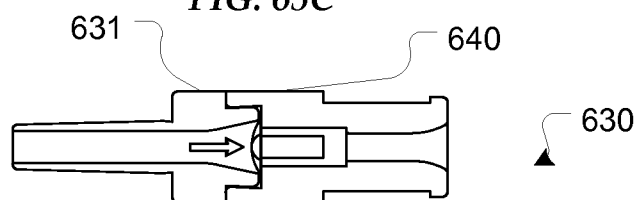
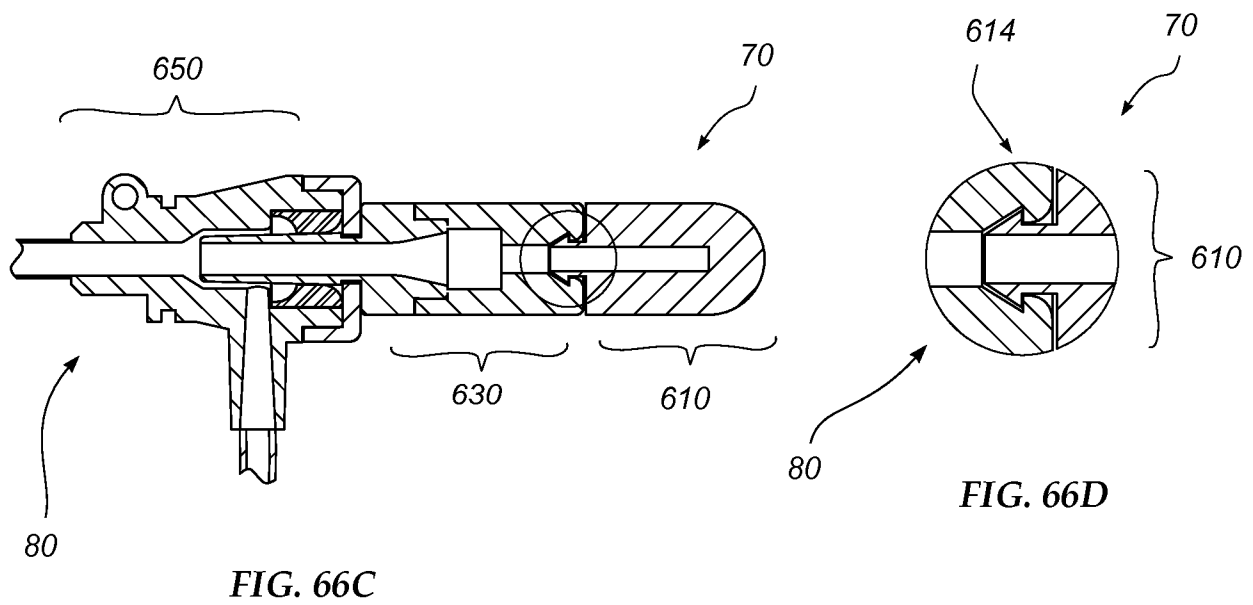
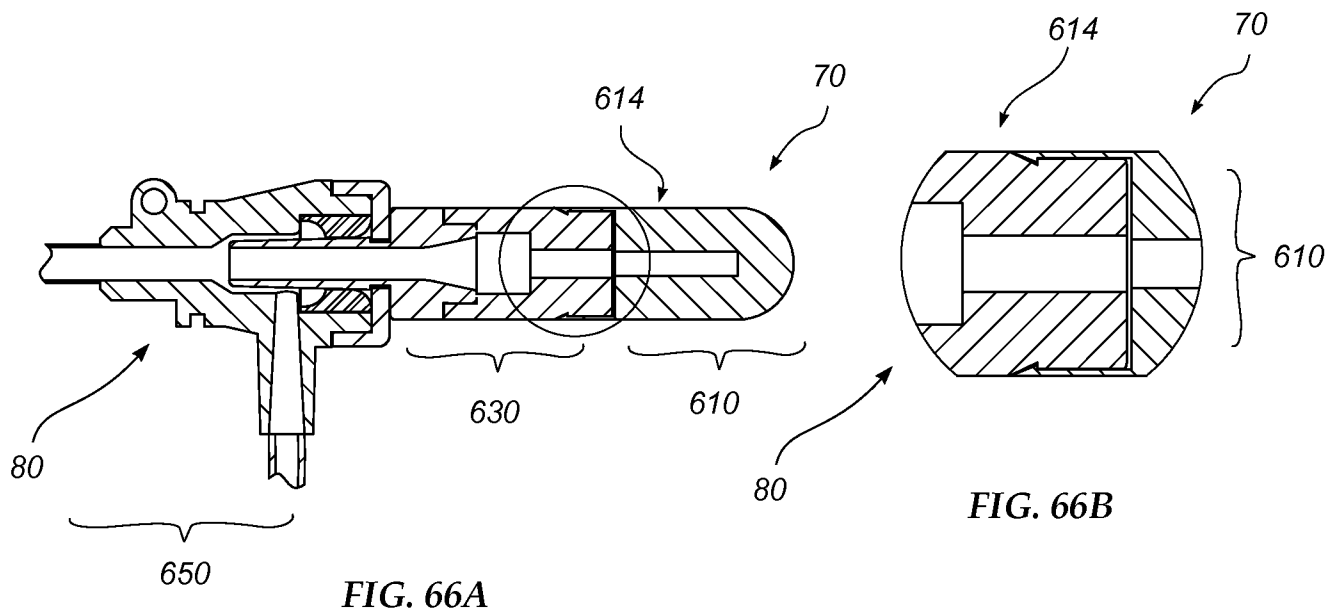


FIG. 65G

71/98



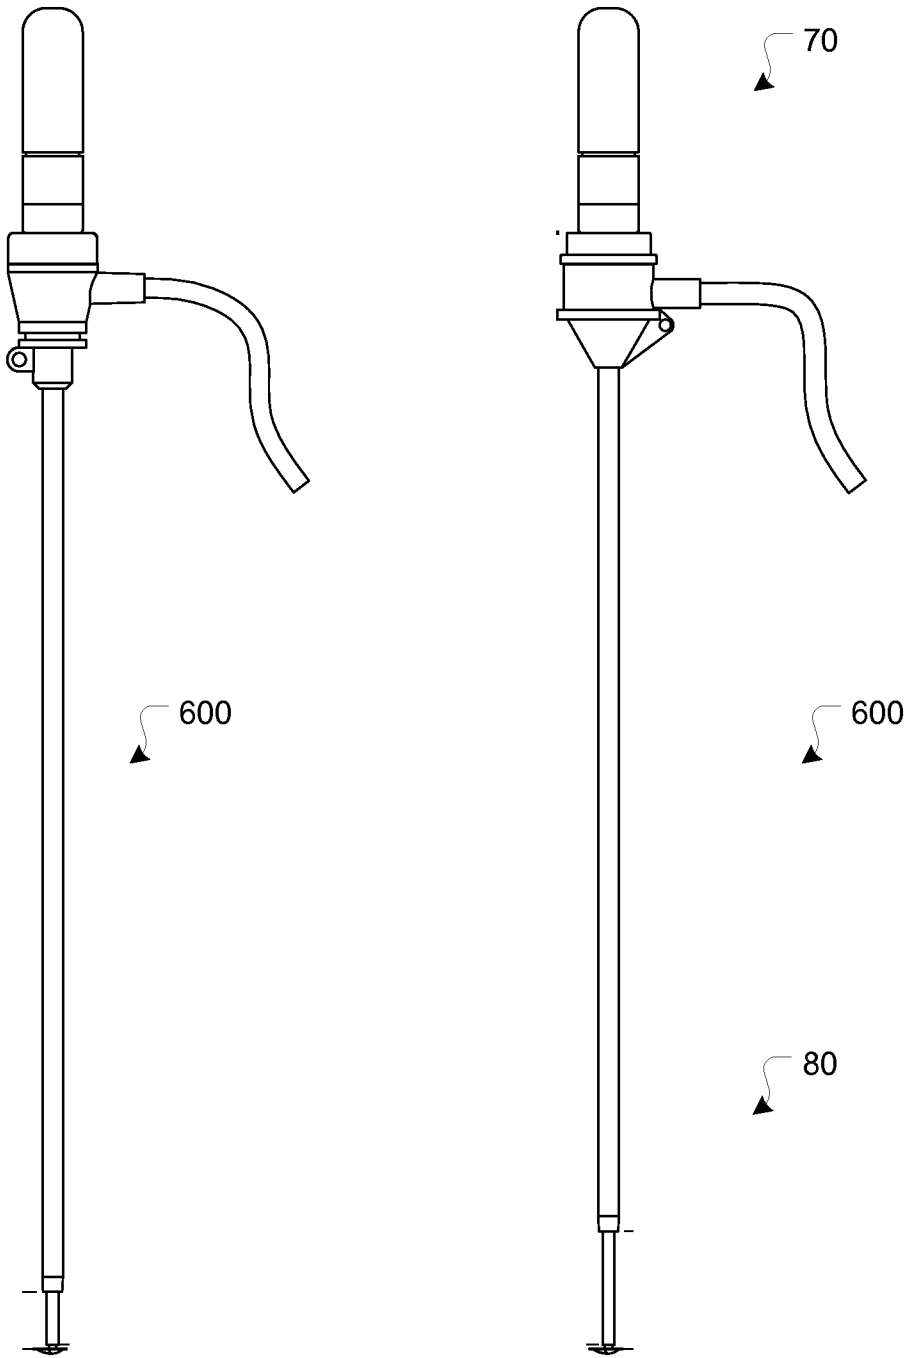


FIG. 67A

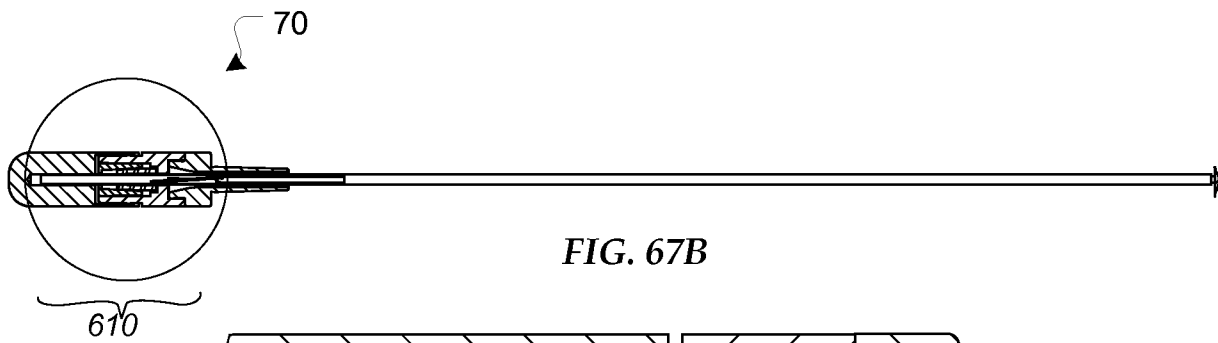


FIG. 67B

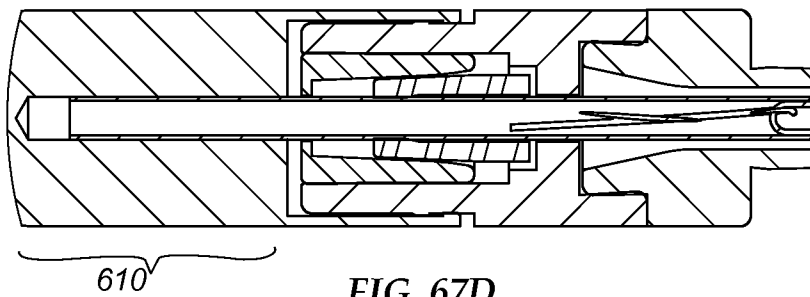


FIG. 67D

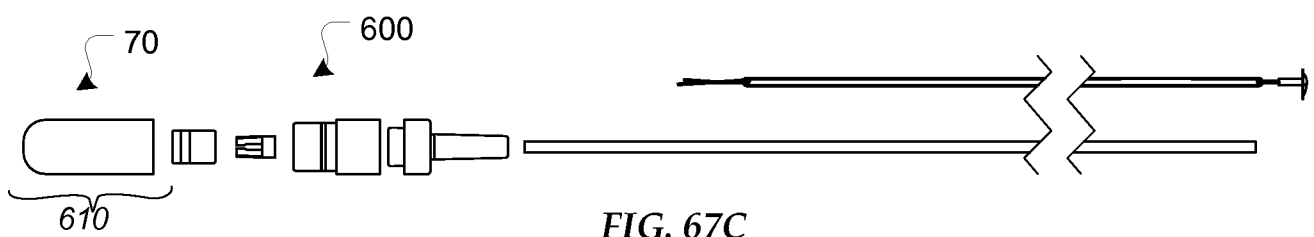


FIG. 67C

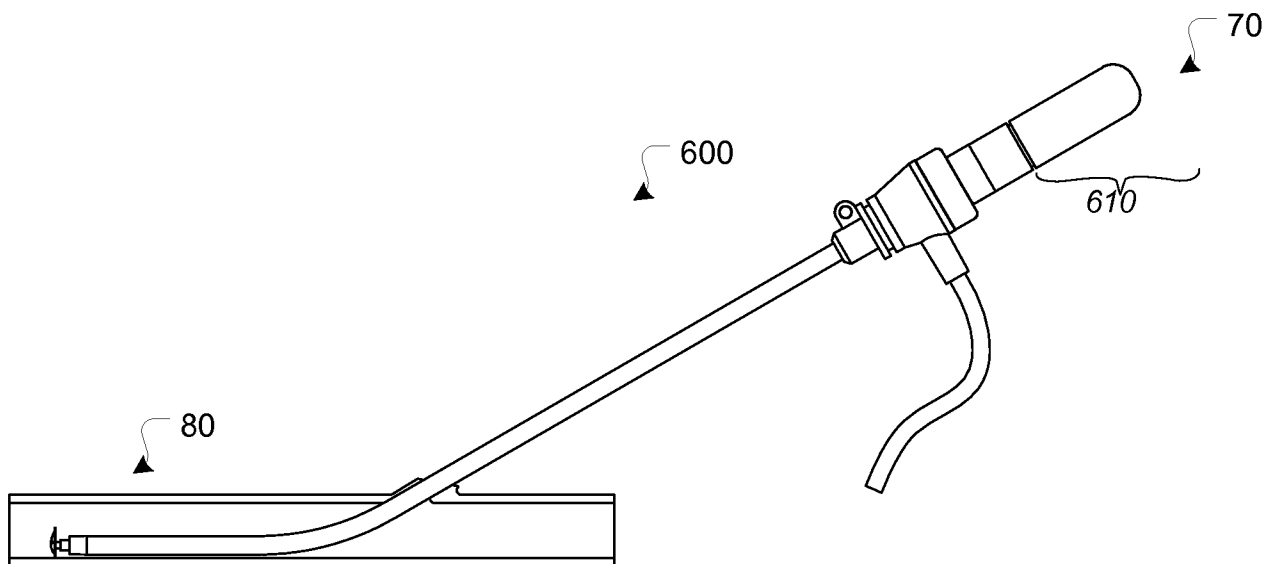


FIG. 67E

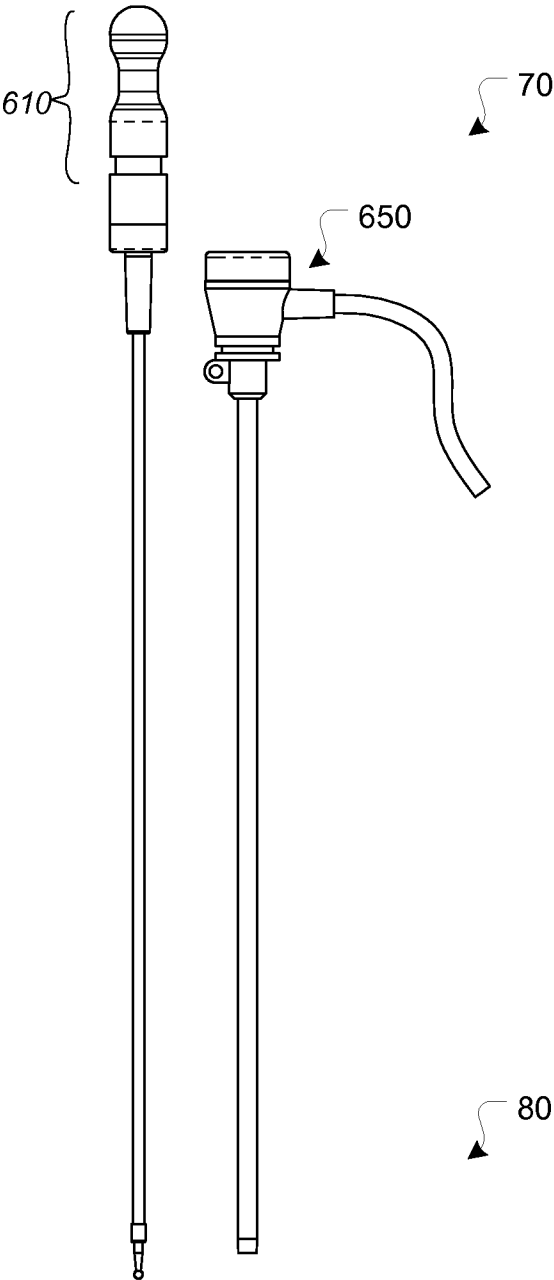


FIG. 68A

FIG. 68B

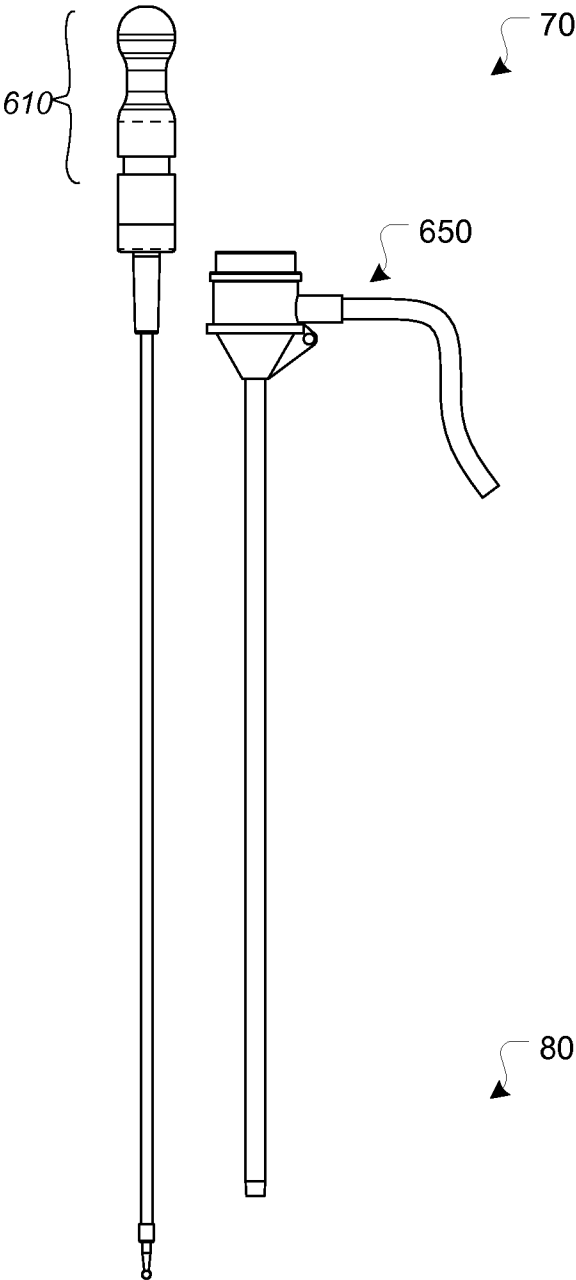


FIG. 69A

FIG. 69B

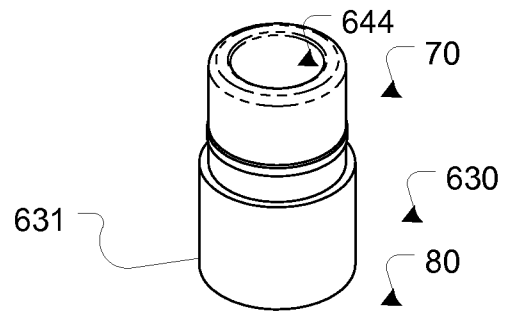


FIG. 70A

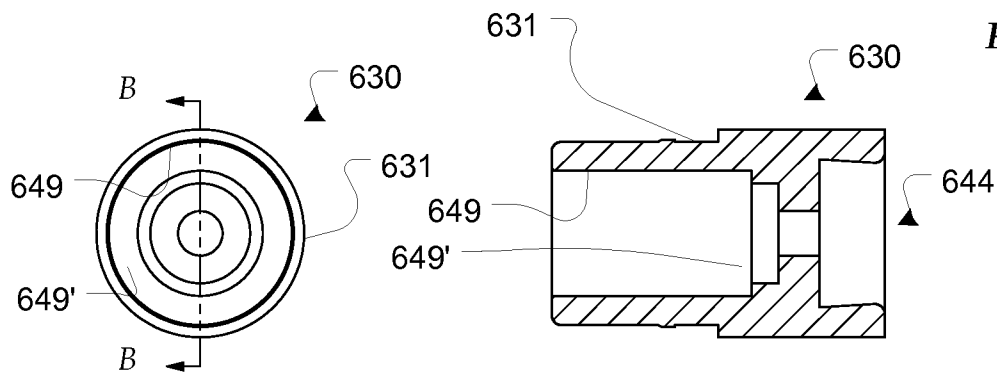


FIG. 70B

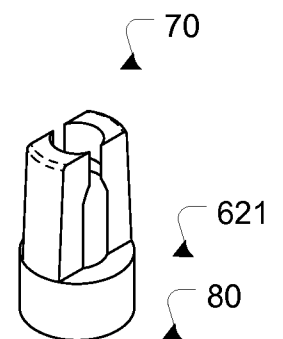


FIG. 70D

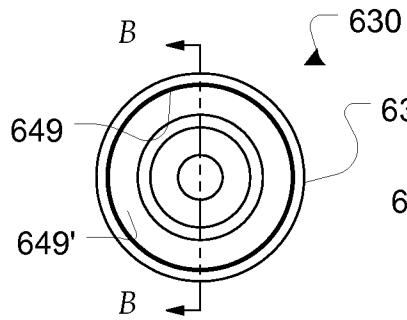


FIG. 70C




FIG. 70G

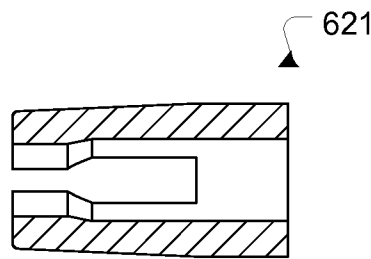


FIG. 70E

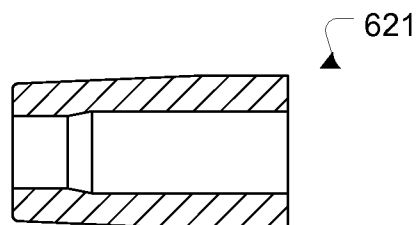


FIG. 70F

76/98

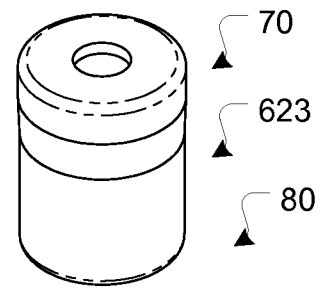


FIG. 71A

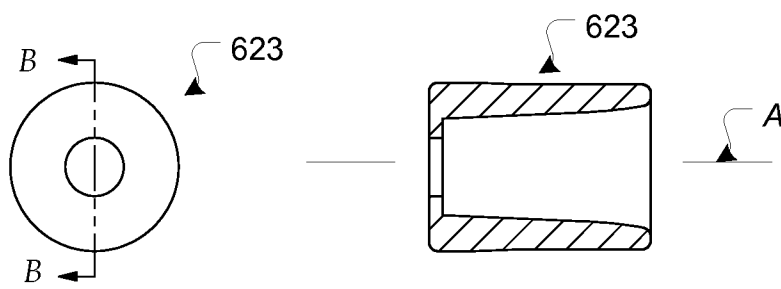


FIG. 71B




FIG. 71C




FIG. 72A

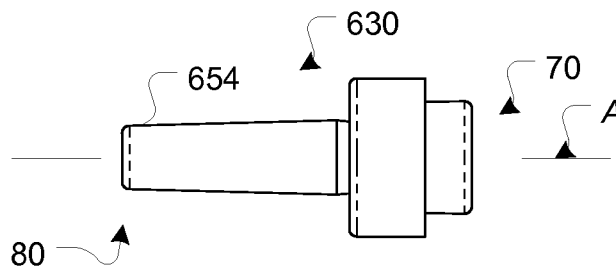


FIG. 72D

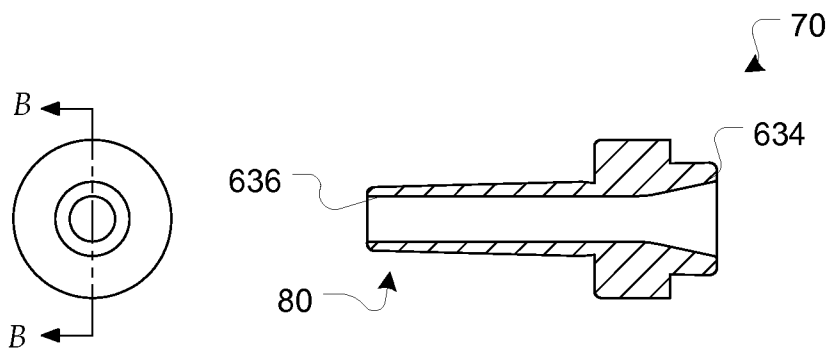


FIG. 72B




FIG. 72C




FIG. 72E

77/98

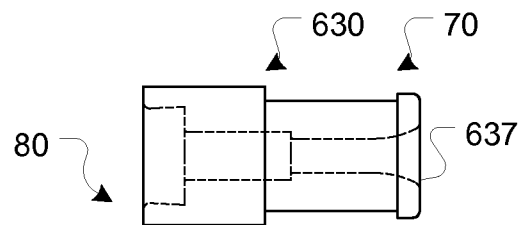


FIG. 73D

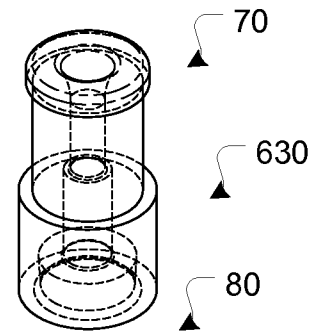


FIG. 73A

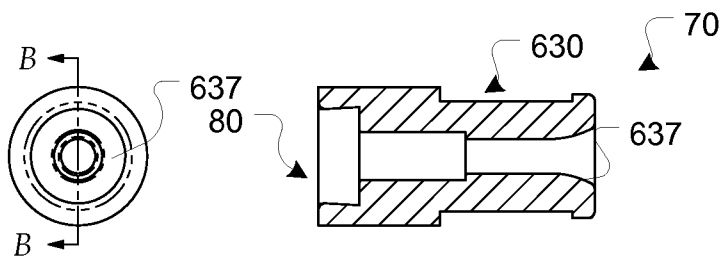


FIG. 73C

FIG. 73b




FIG. 73E

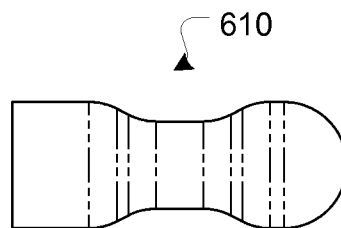


FIG. 74C

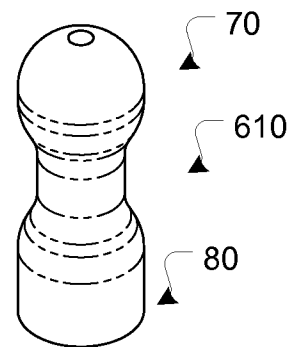


FIG. 74A

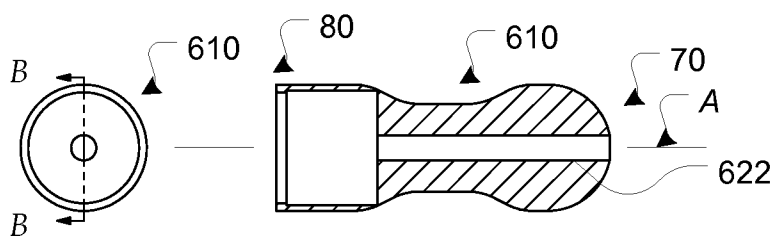


FIG. 74D

FIG. 74B

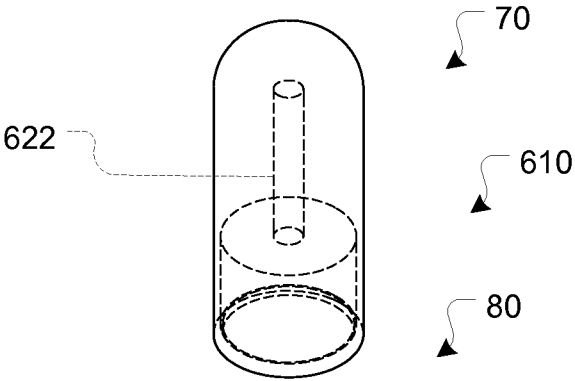


FIG. 75A




FIG. 75C

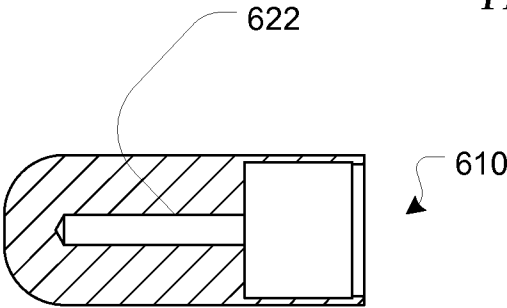


FIG. 75B

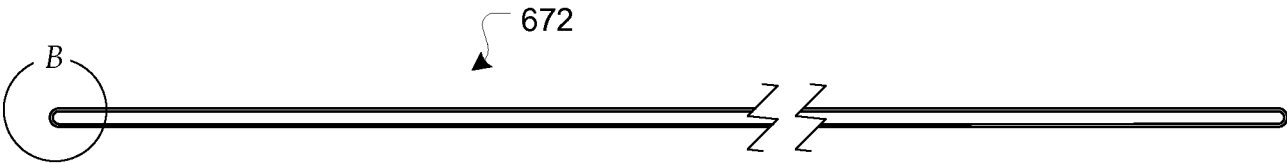


FIG. 76A




FIG. 76B

79/98

FIG. 77A

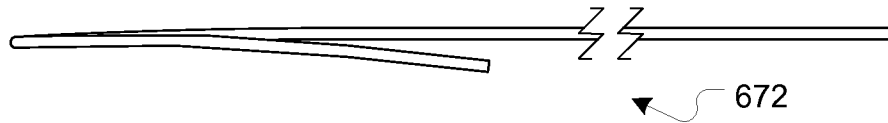


FIG. 77B

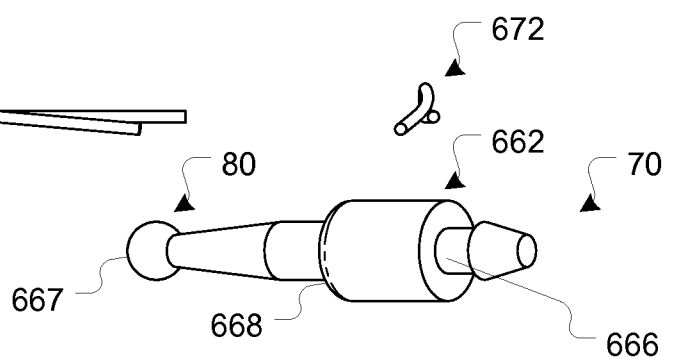
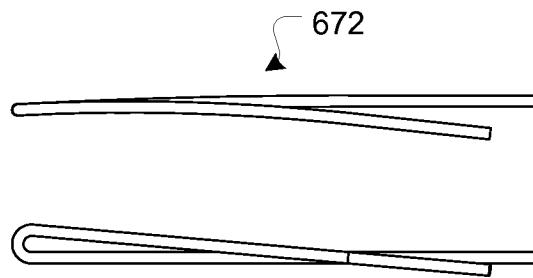


FIG. 78A

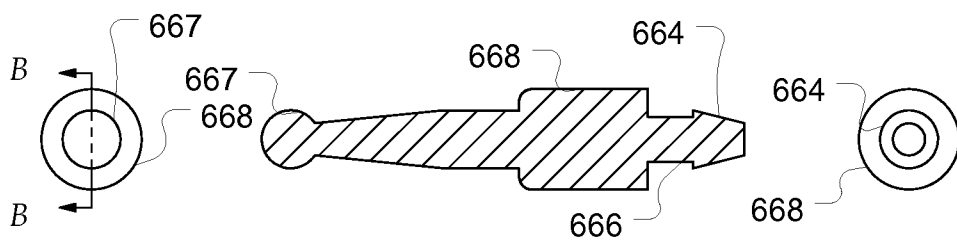


FIG. 78D

FIG. 78B

FIG. 78C

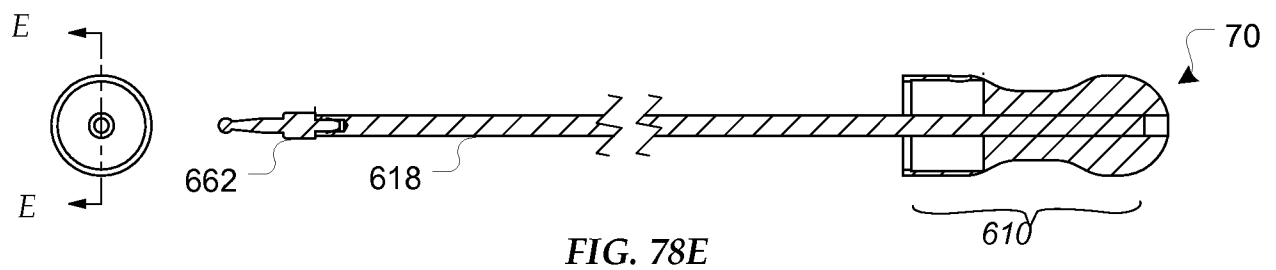


FIG. 78E

80/98

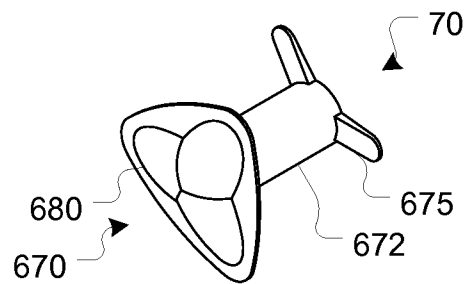


FIG. 79A




FIG. 79B




FIG. 79D

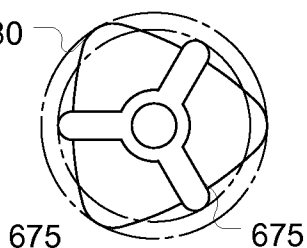


FIG. 79C

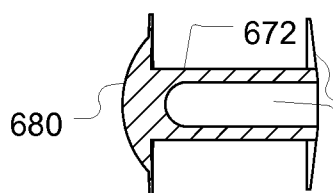


FIG. 79E

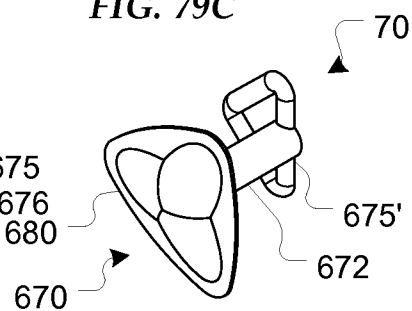


FIG. 79F




FIG. 79G

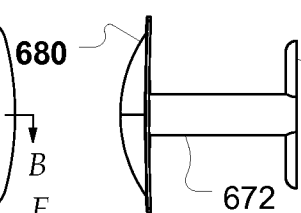


FIG. 79H

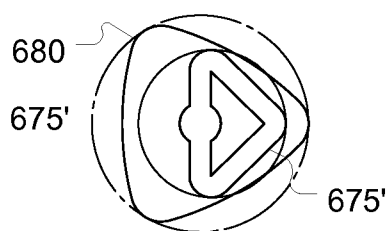


FIG. 79I

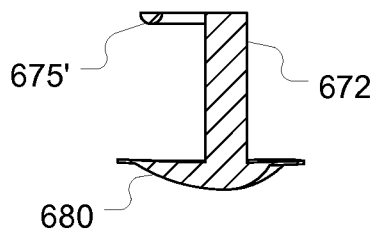


FIG. 79J

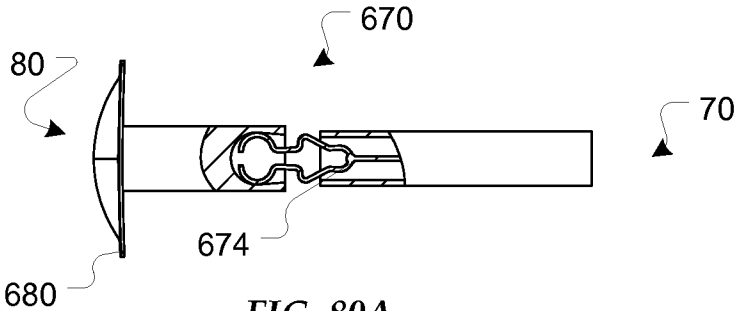



FIG. 80A

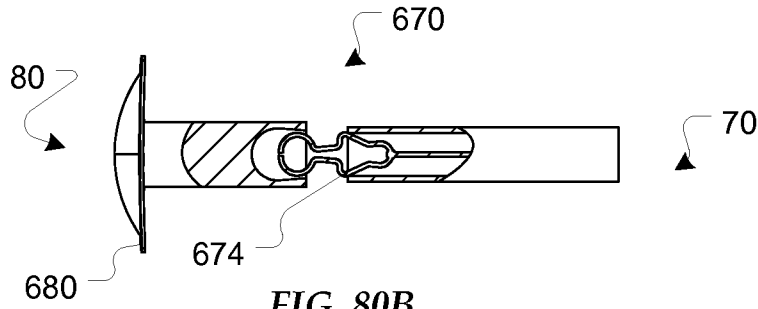



FIG. 80B

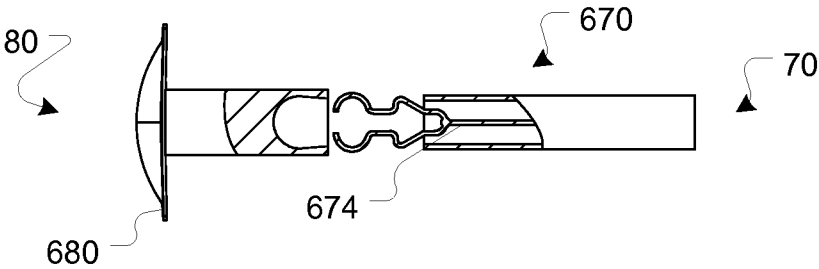



FIG. 80C




FIG. 81A




FIG. 81B




FIG. 81C





FIG. 81D

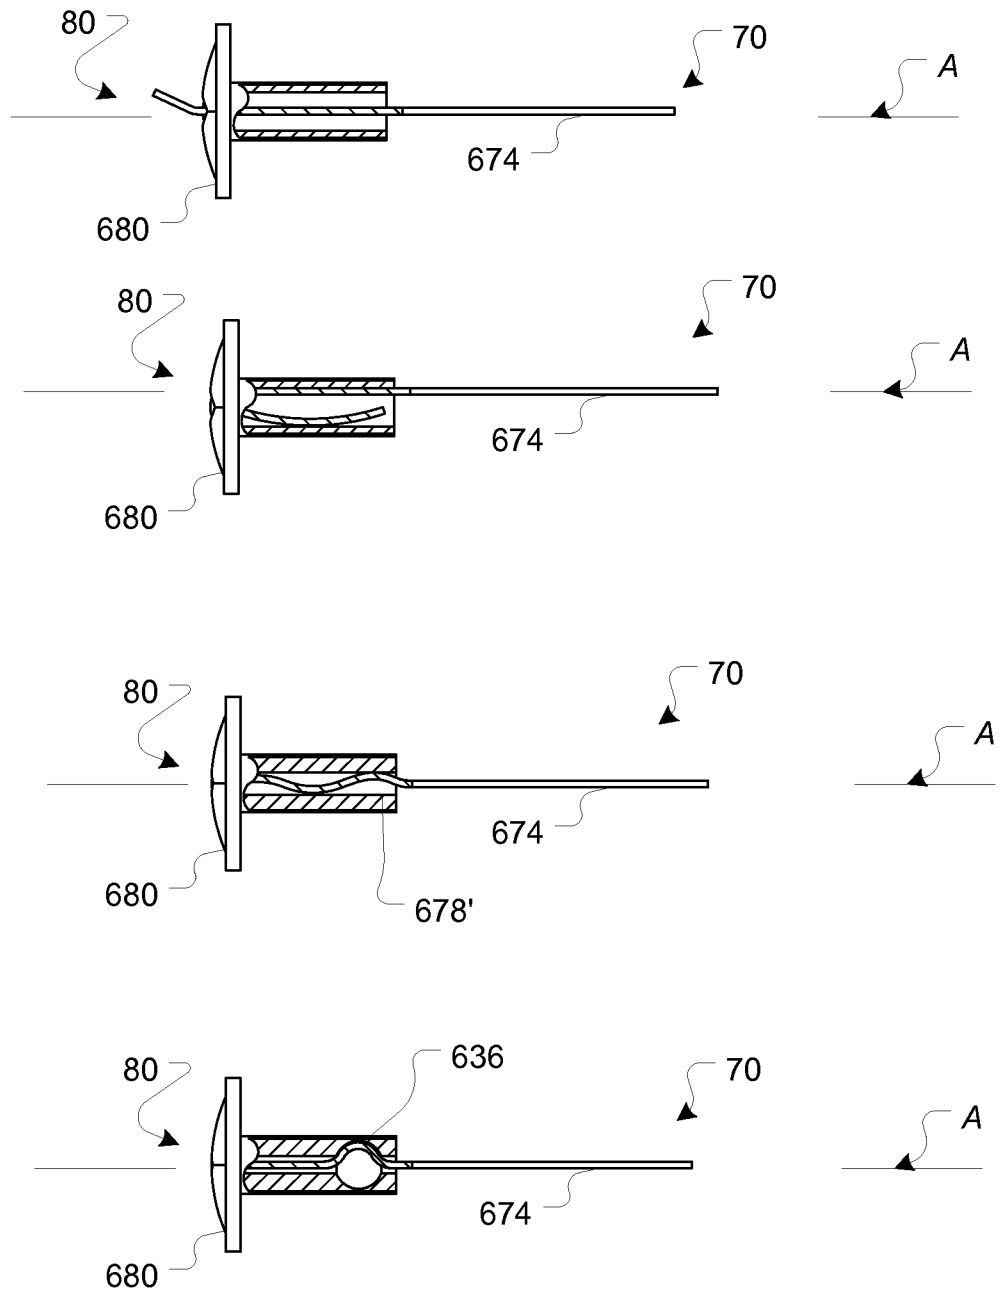

83/98




FIG. 81E




FIG. 81F




FIG. 81G








FIG. 81H

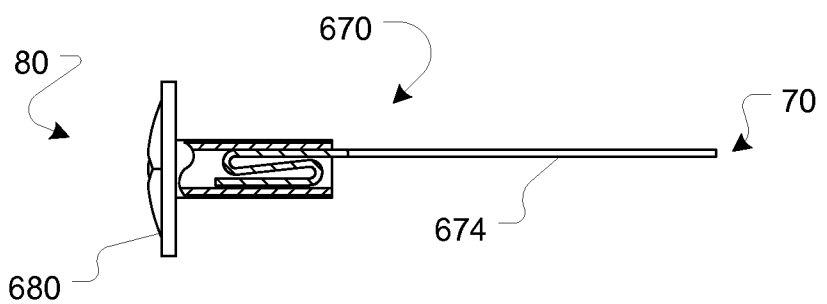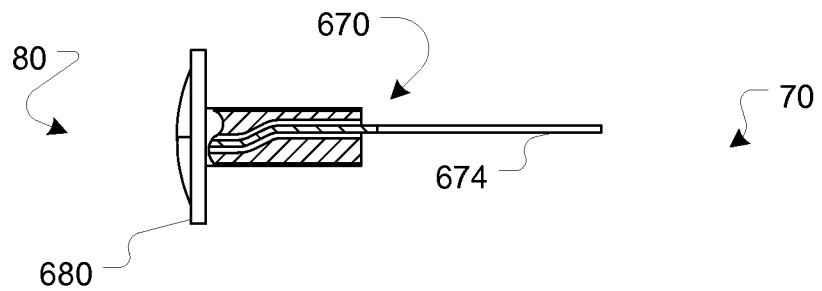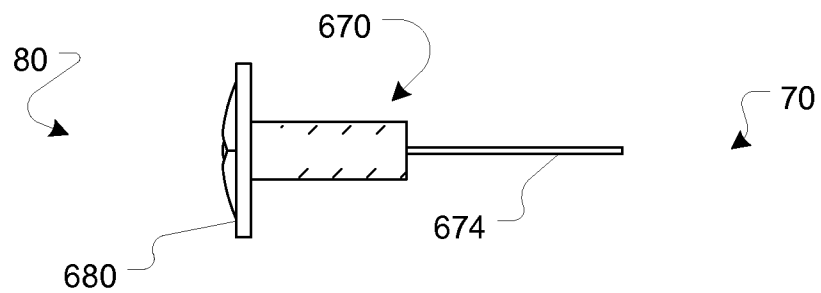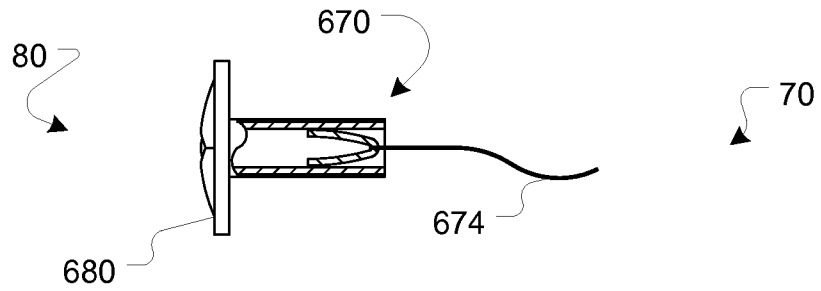

84/98




FIG. 81I


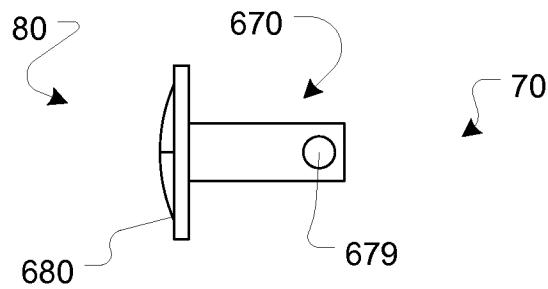


FIG. 81J


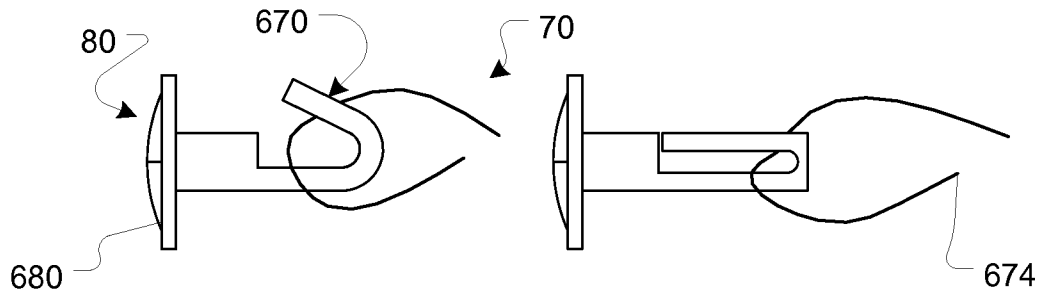


FIG. 81K


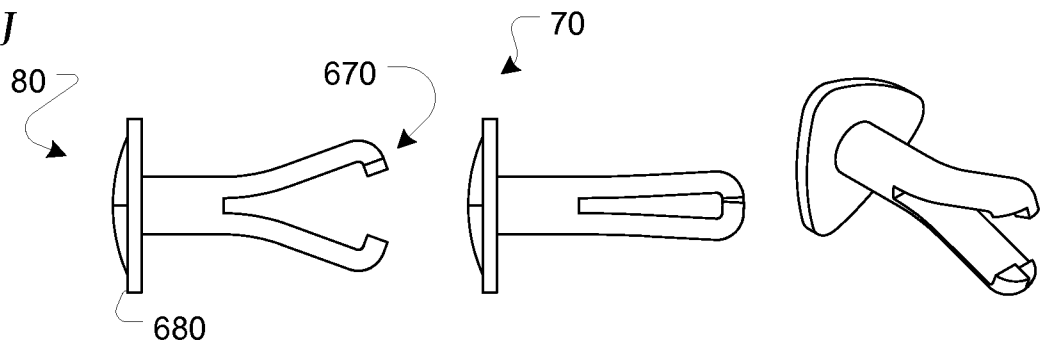


FIG. 81L






FIG. 81M

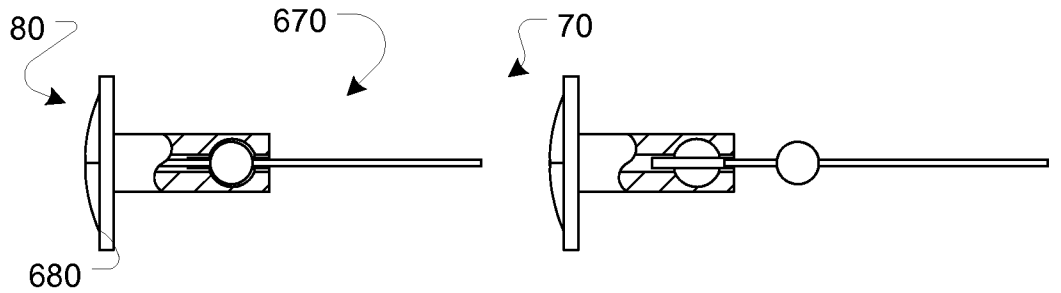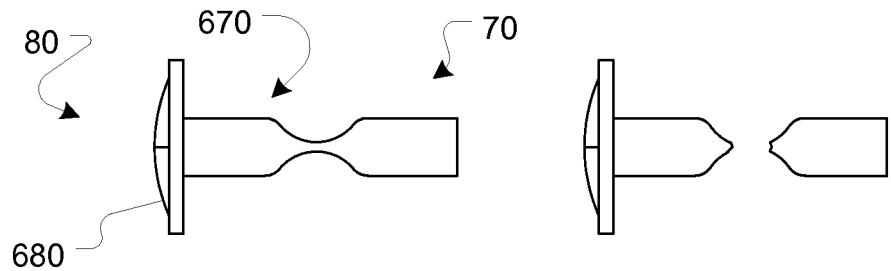

85/98

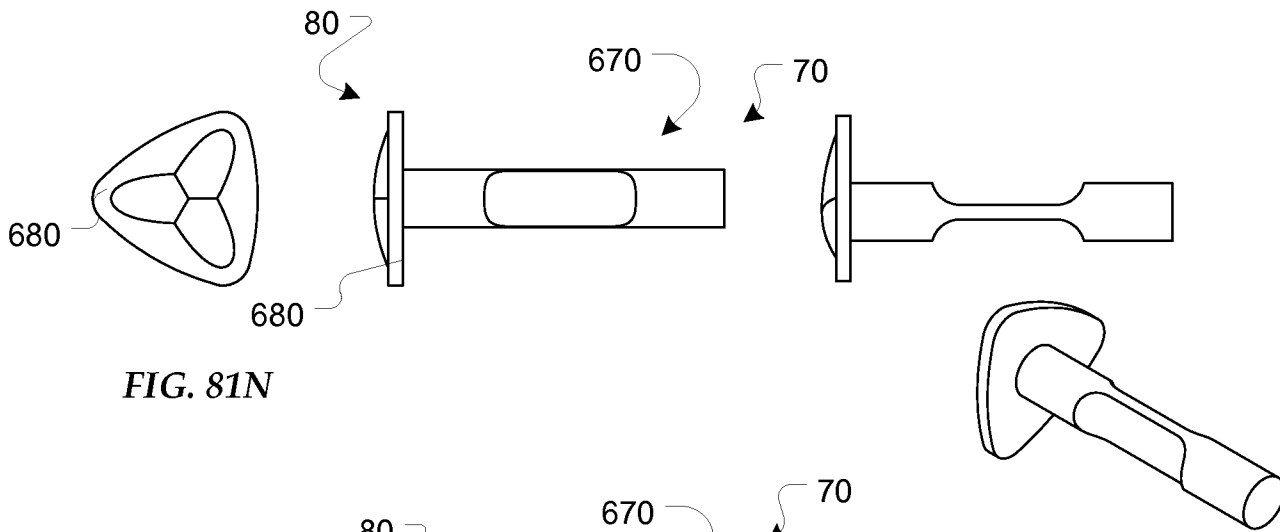


FIG. 81N

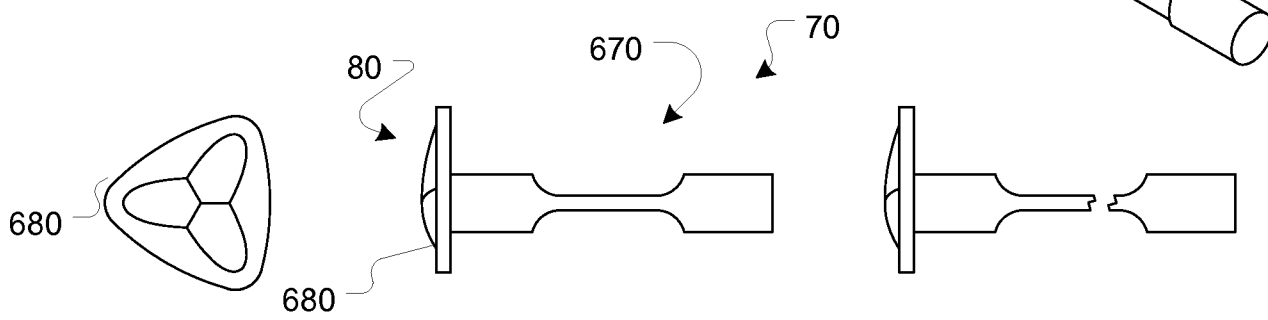


FIG. 82A

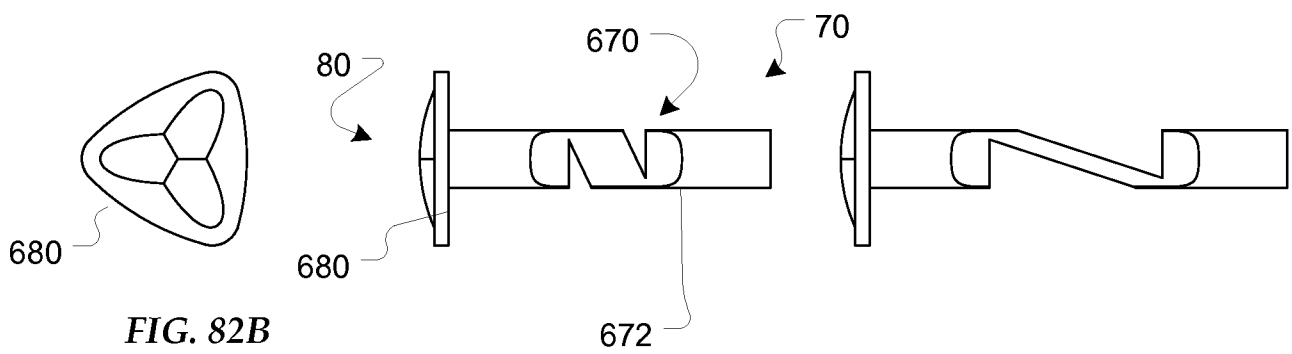


FIG. 82B

86/98

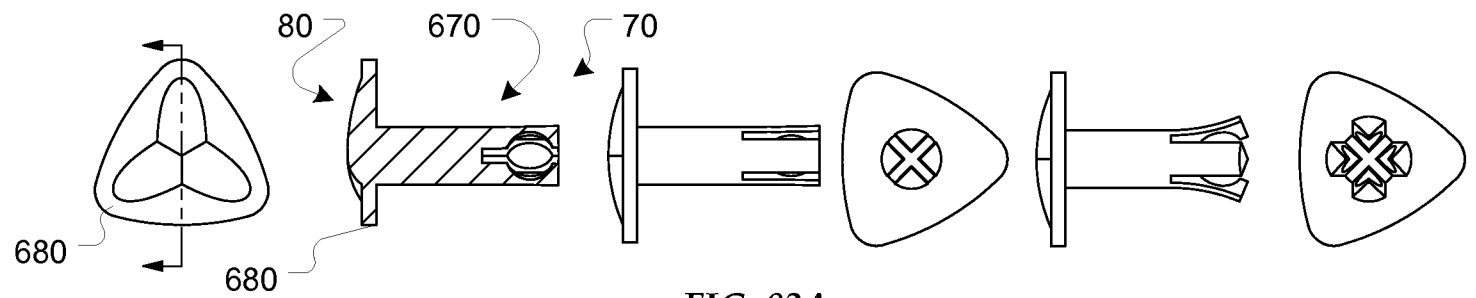


FIG. 83A

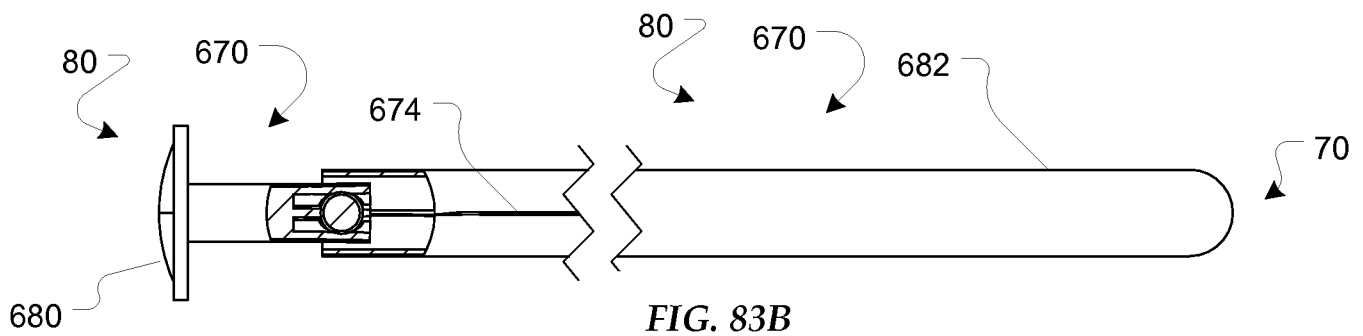


FIG. 83B

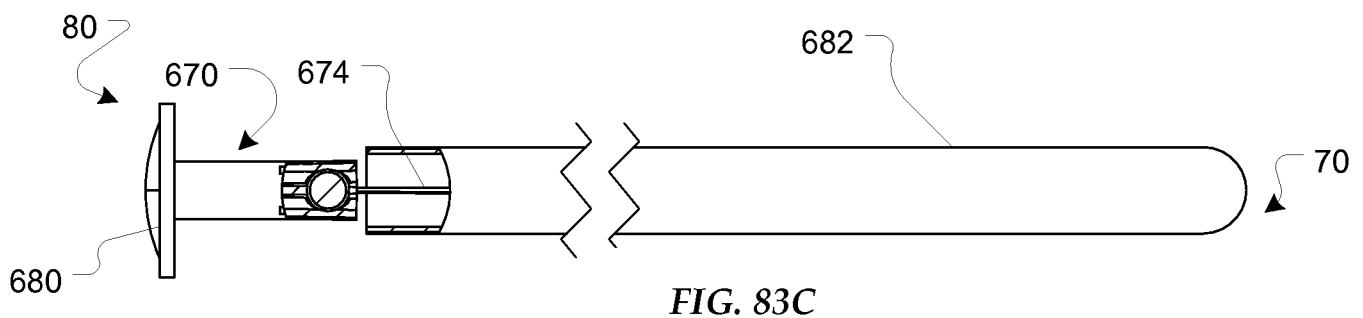


FIG. 83C

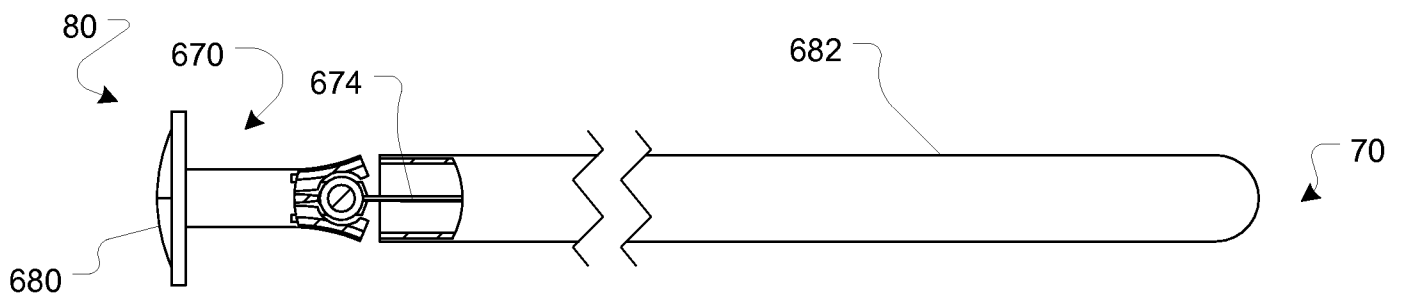
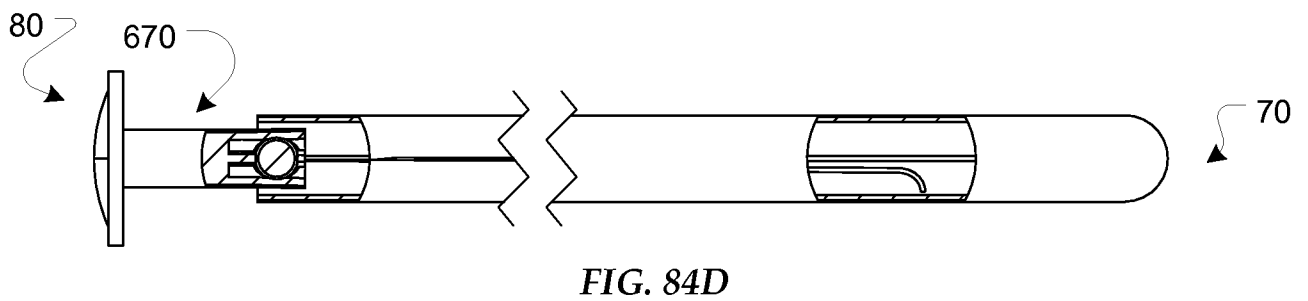
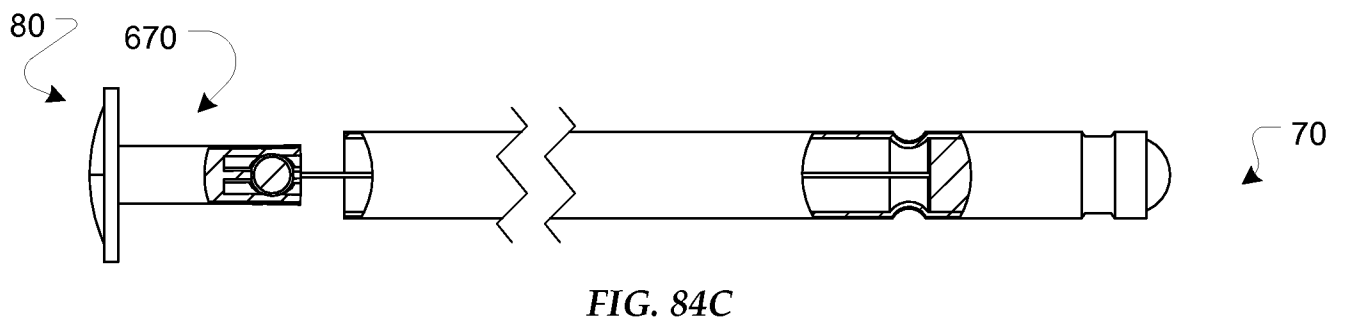
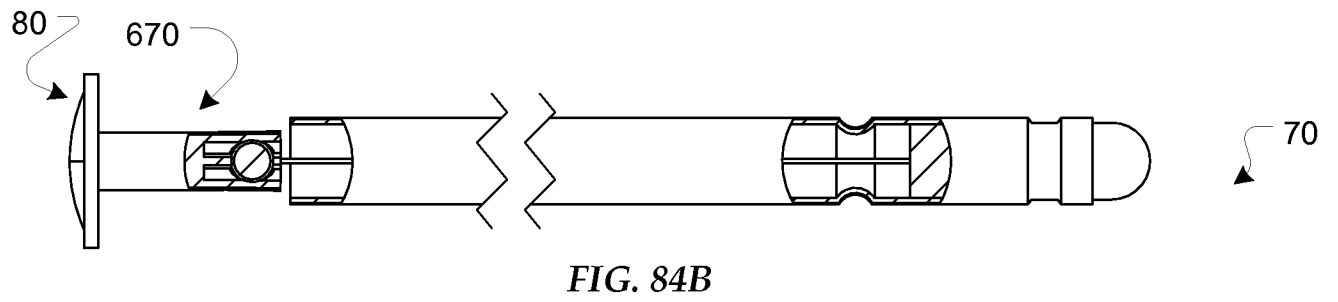
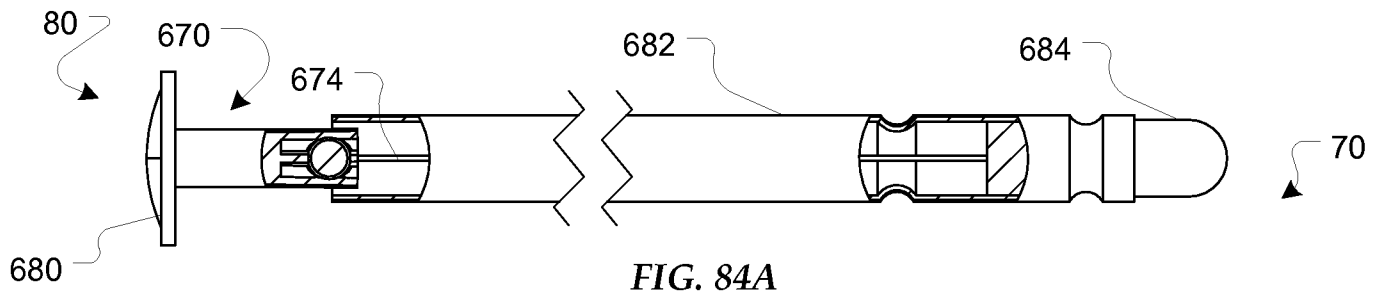


FIG. 83D

87/98






FIG. 85A




FIG. 85B




FIG. 85C




FIG. 85D




FIG. 85E




FIG. 85F




FIG. 85G

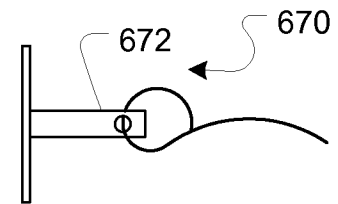


FIG. 85H




FIG. 85I




FIG. 85J

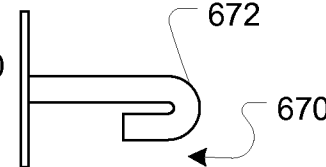


FIG. 85K




FIG. 85L

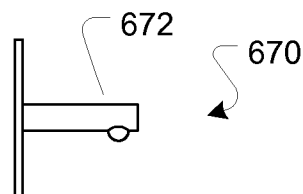


FIG. 85M

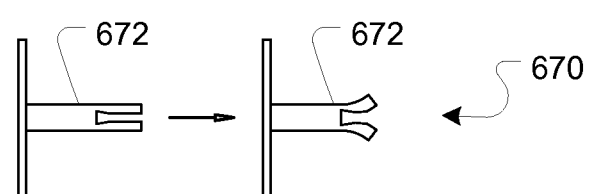


FIG. 85N

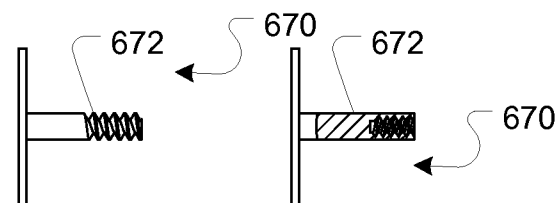


FIG. 85O




FIG. 85P




FIG. 85Q




FIG. 85R

89/98

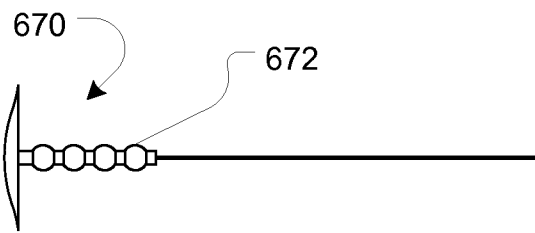


FIG. 86A

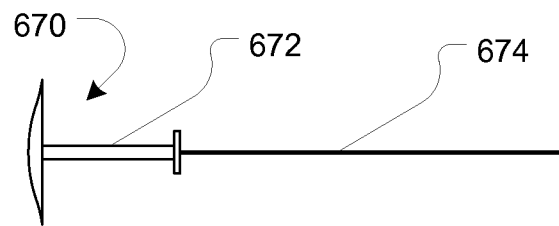


FIG. 86B

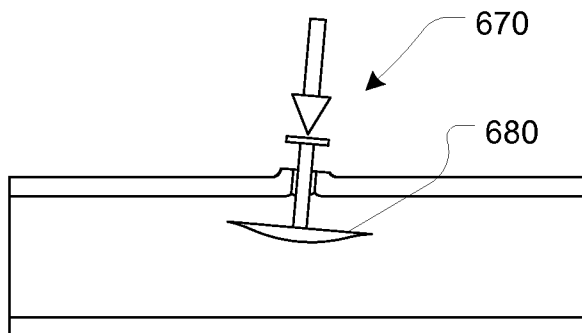


FIG. 86C

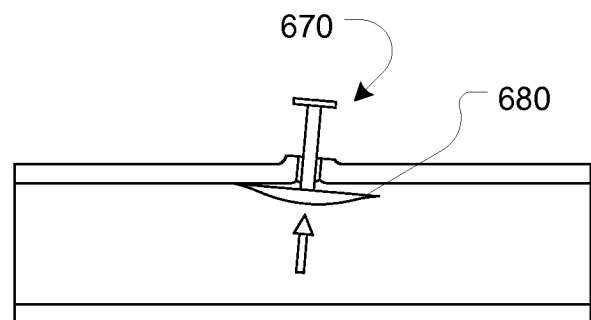


FIG. 86D

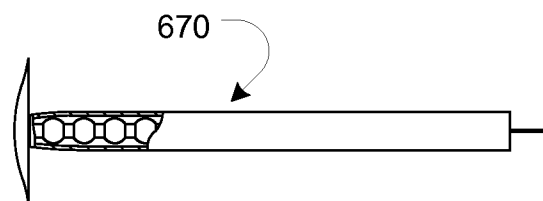
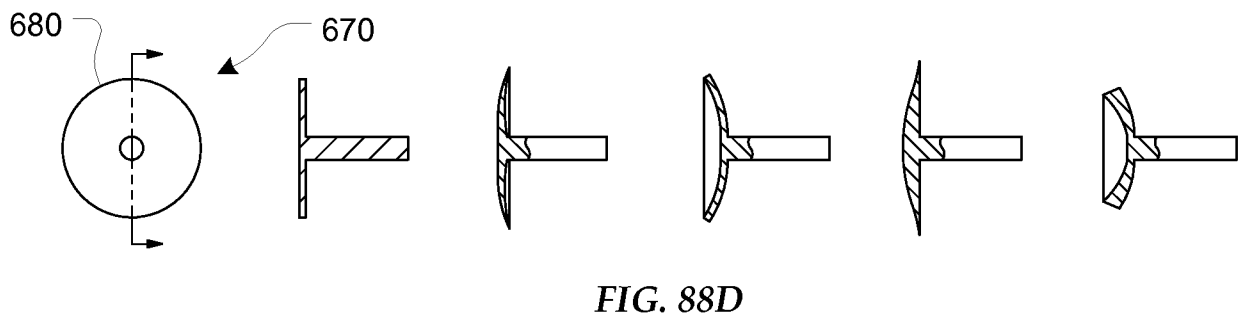
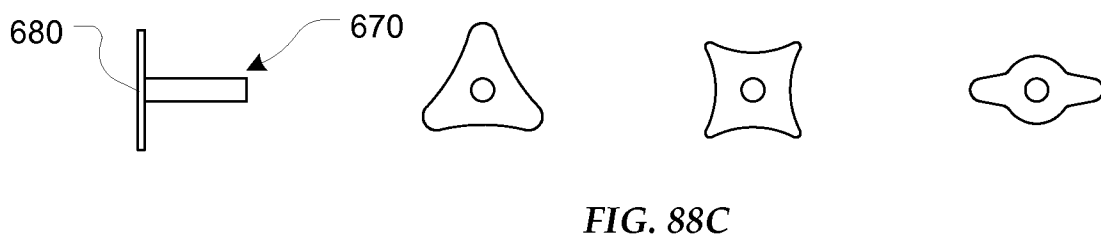
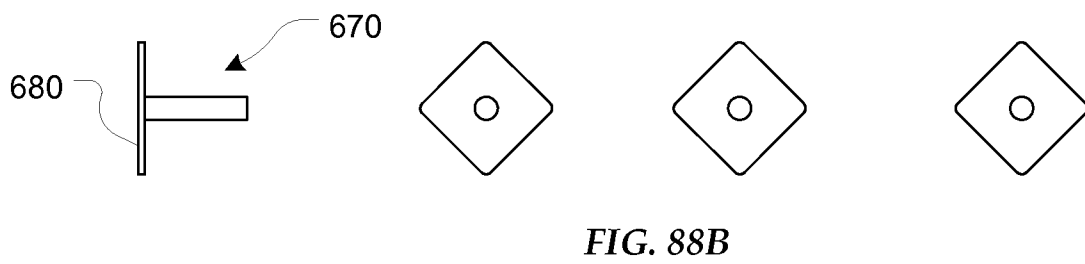
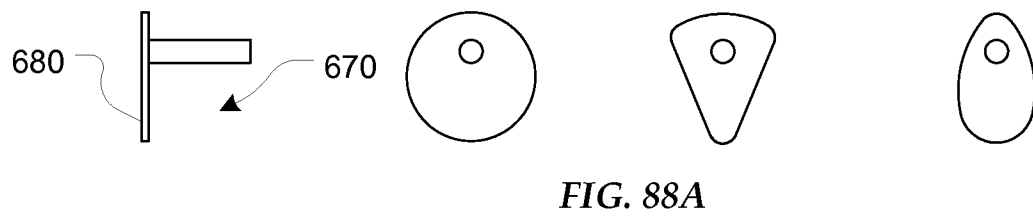
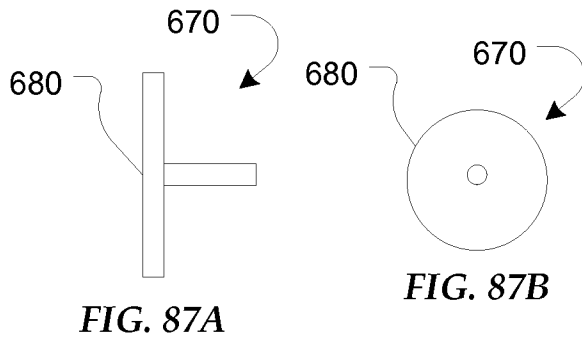


FIG. 86E

90/98



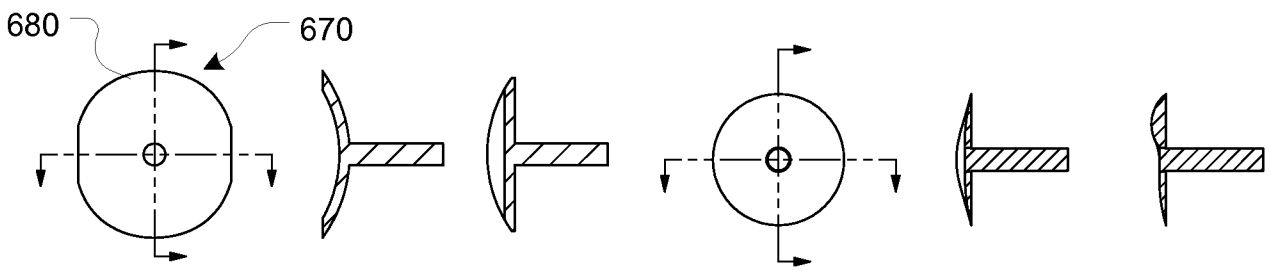


FIG. 88E

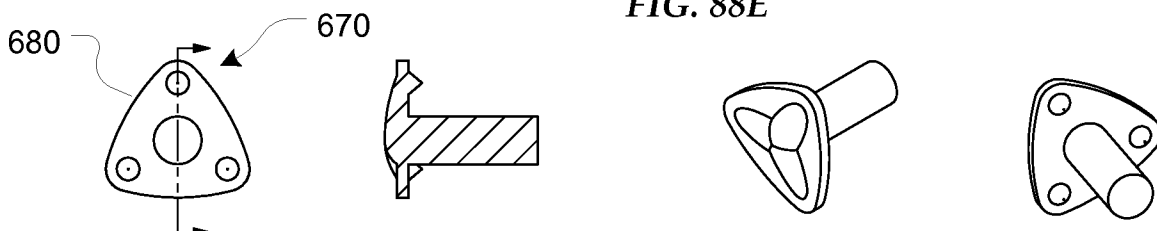


FIG. 88F

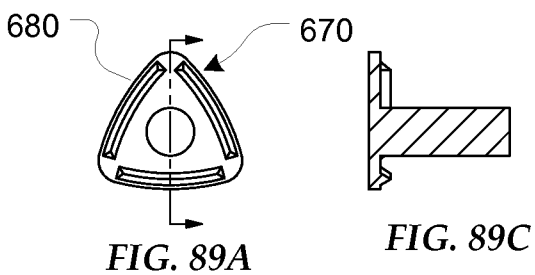


FIG. 89A

FIG. 89C

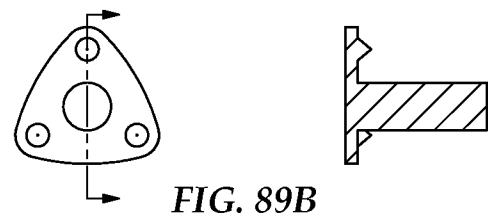


FIG. 89B

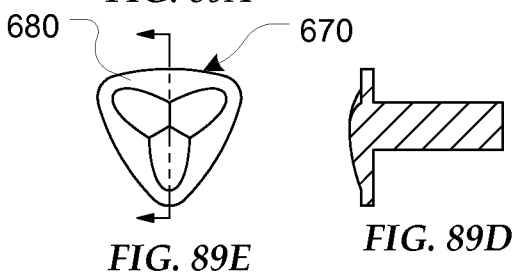


FIG. 89E

FIG. 89D


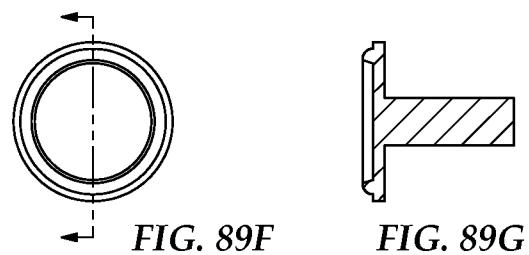


FIG. 89F

FIG. 89G

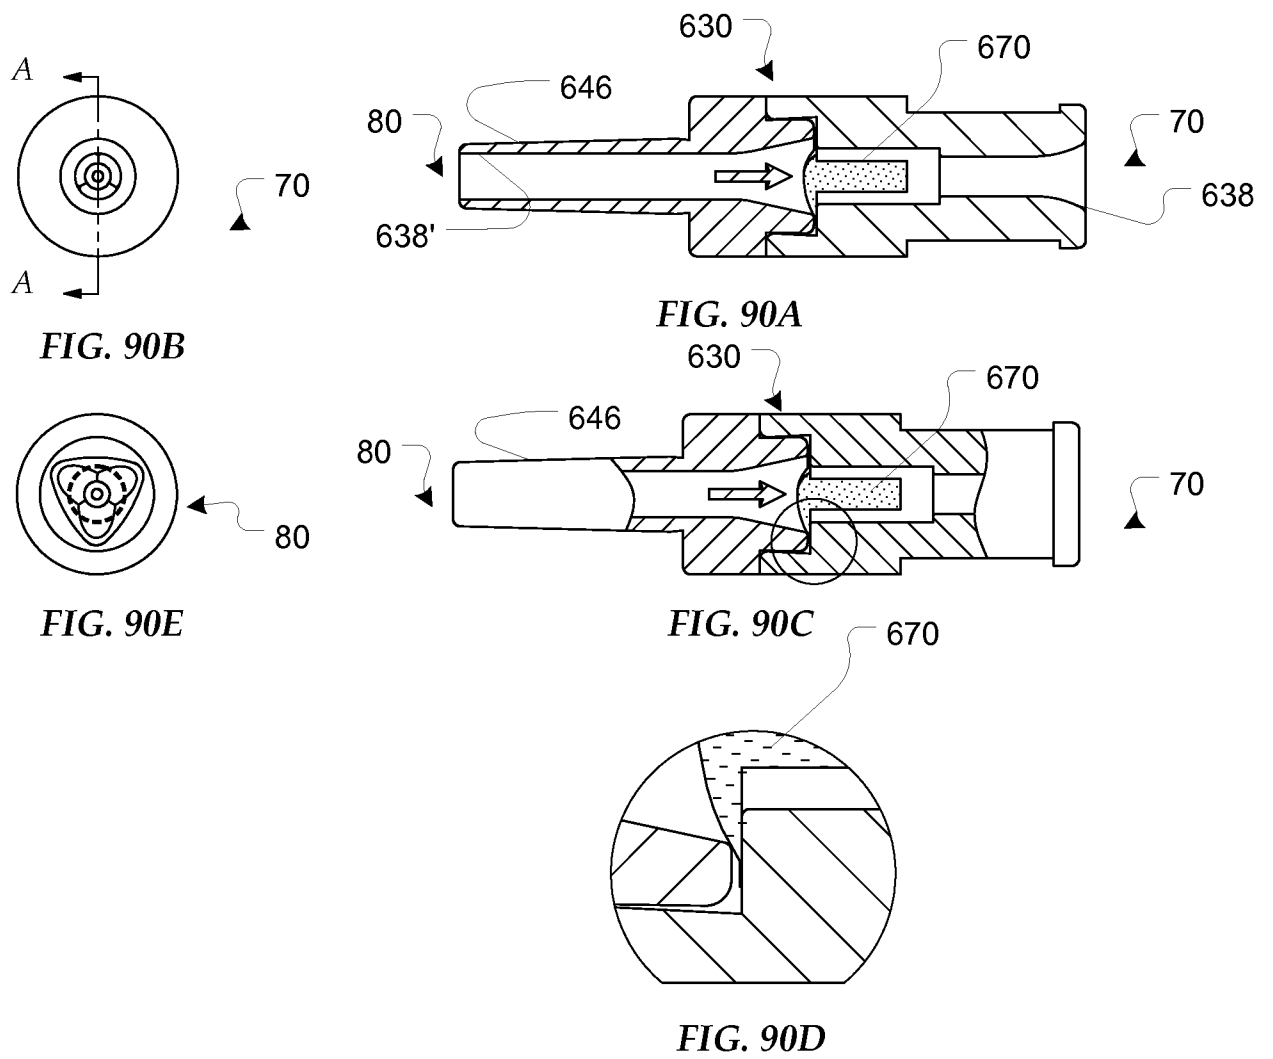

93/98

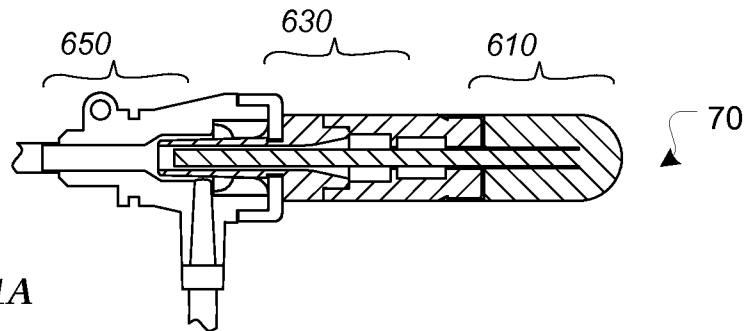


FIG. 91A

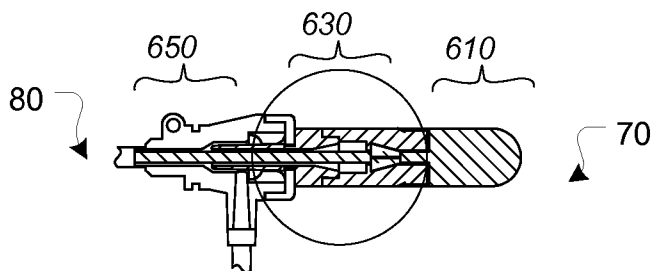


FIG. 91B

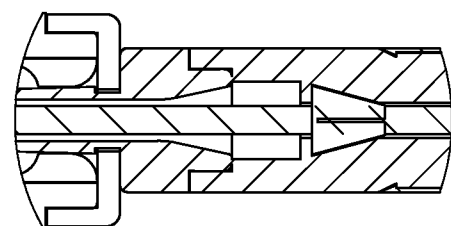


FIG. 91C

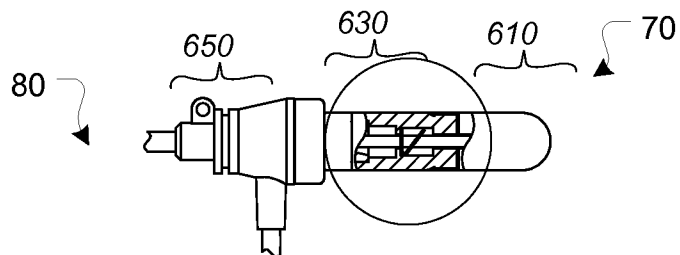


FIG. 91D

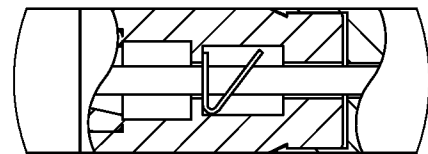


FIG. 91E

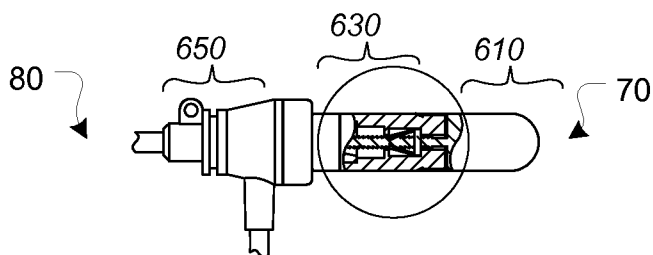


FIG. 91F

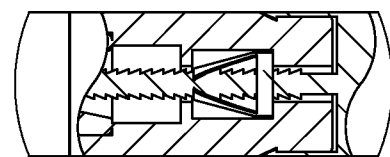


FIG. 91G

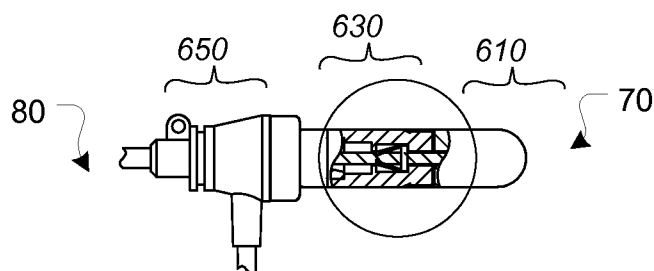


FIG. 91H

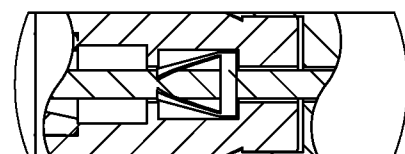


FIG. 91 i

94/98

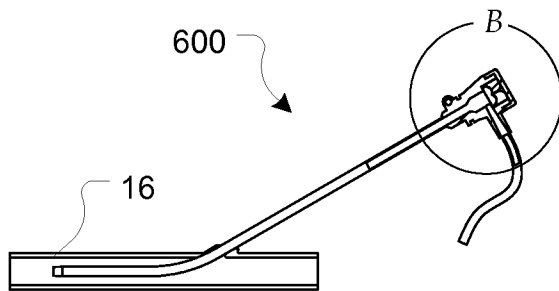


FIG. 92A

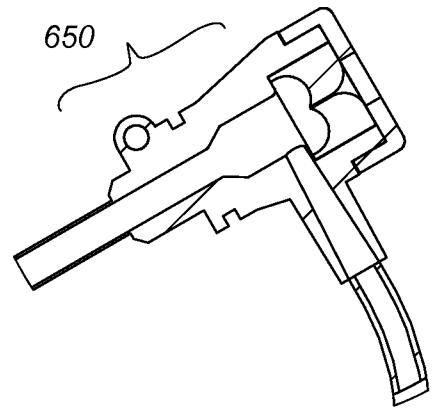


FIG. 92B

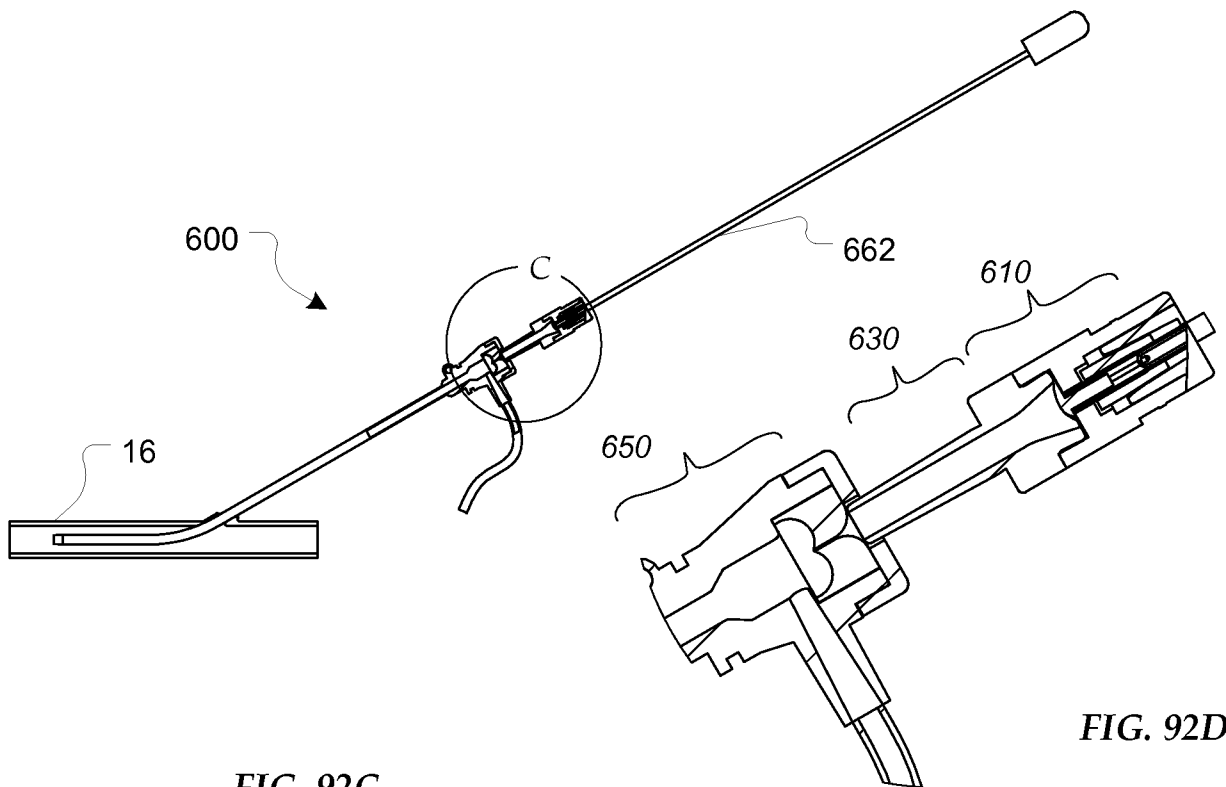


FIG. 92C

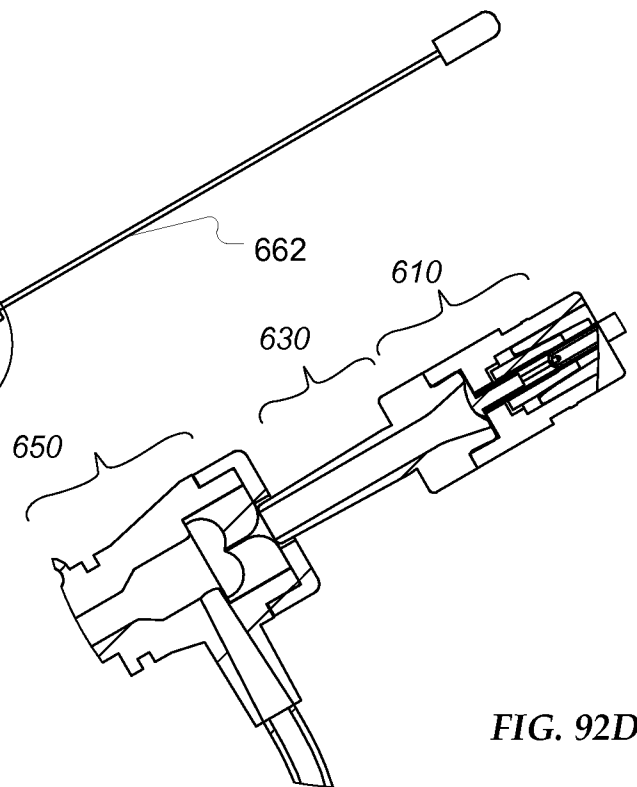


FIG. 92D

95/98

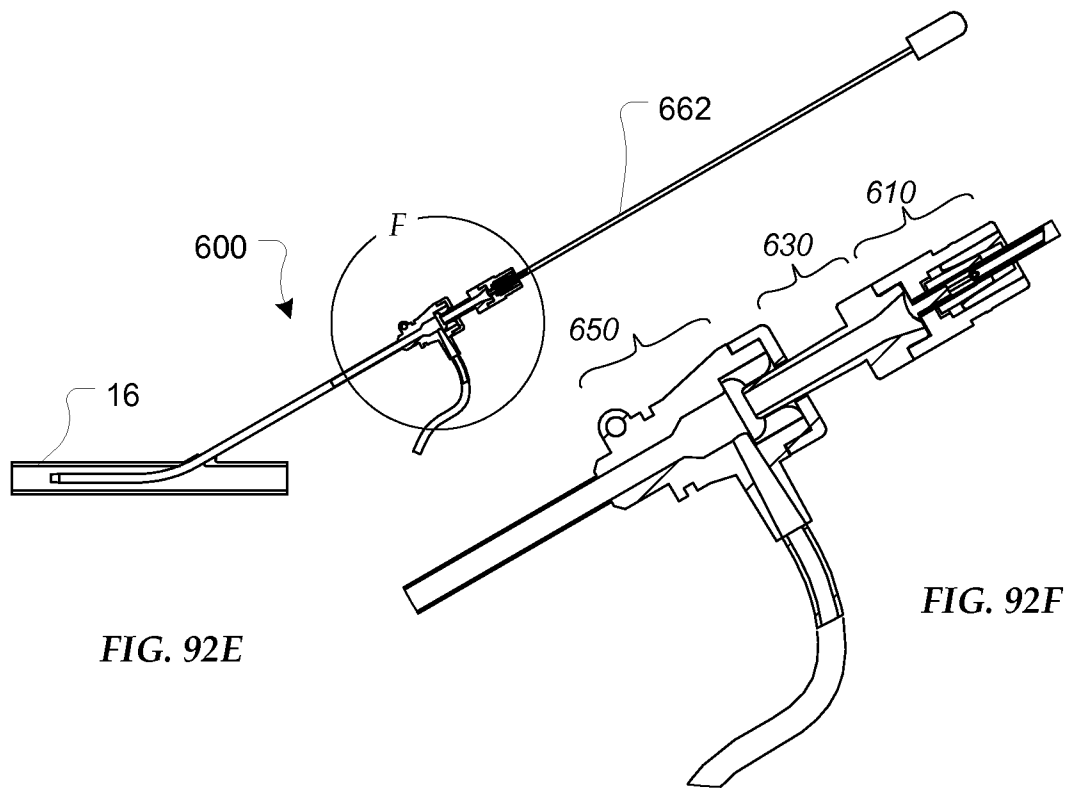


FIG. 92E

FIG. 92F

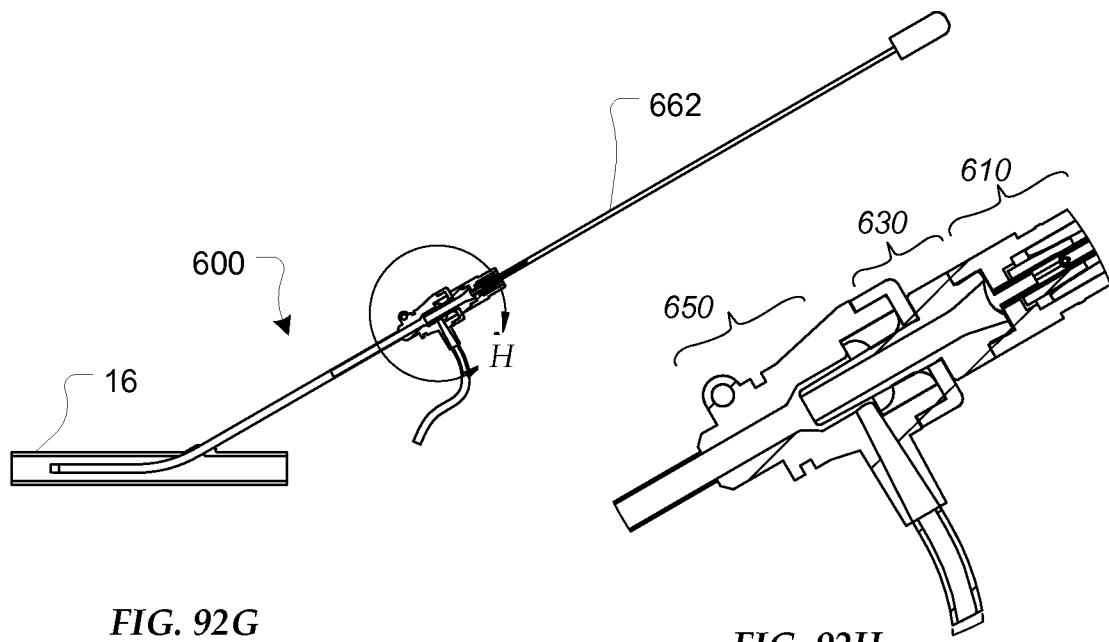


FIG. 92G

FIG. 92H

96/98

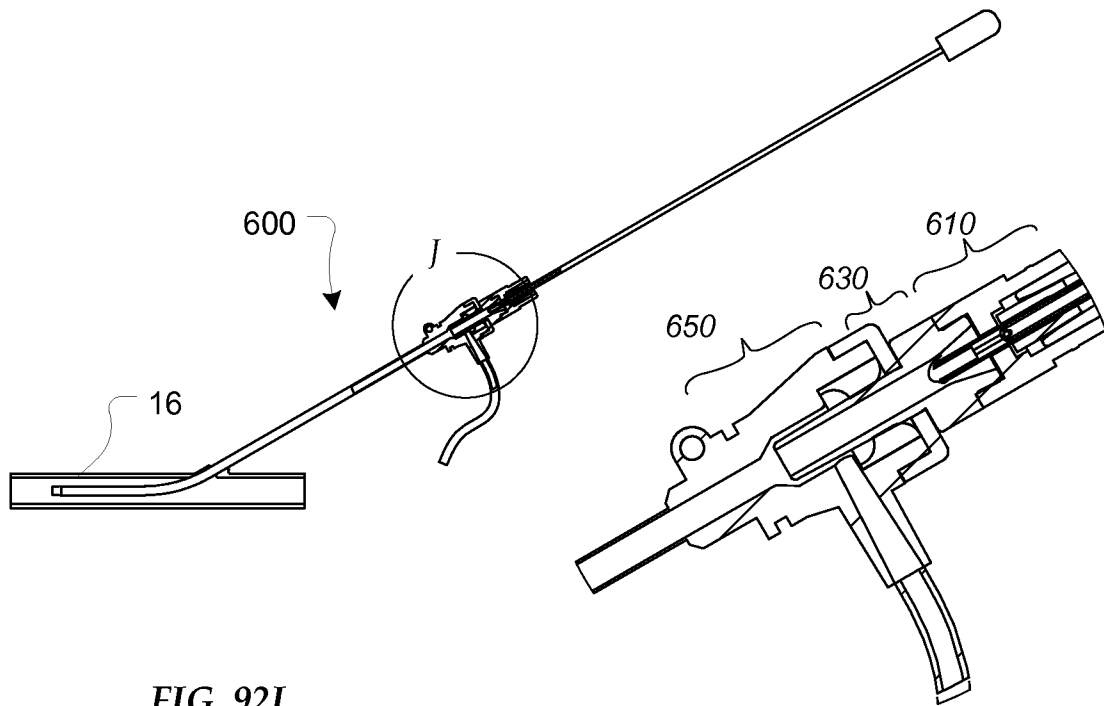


FIG. 92I

FIG. 92J

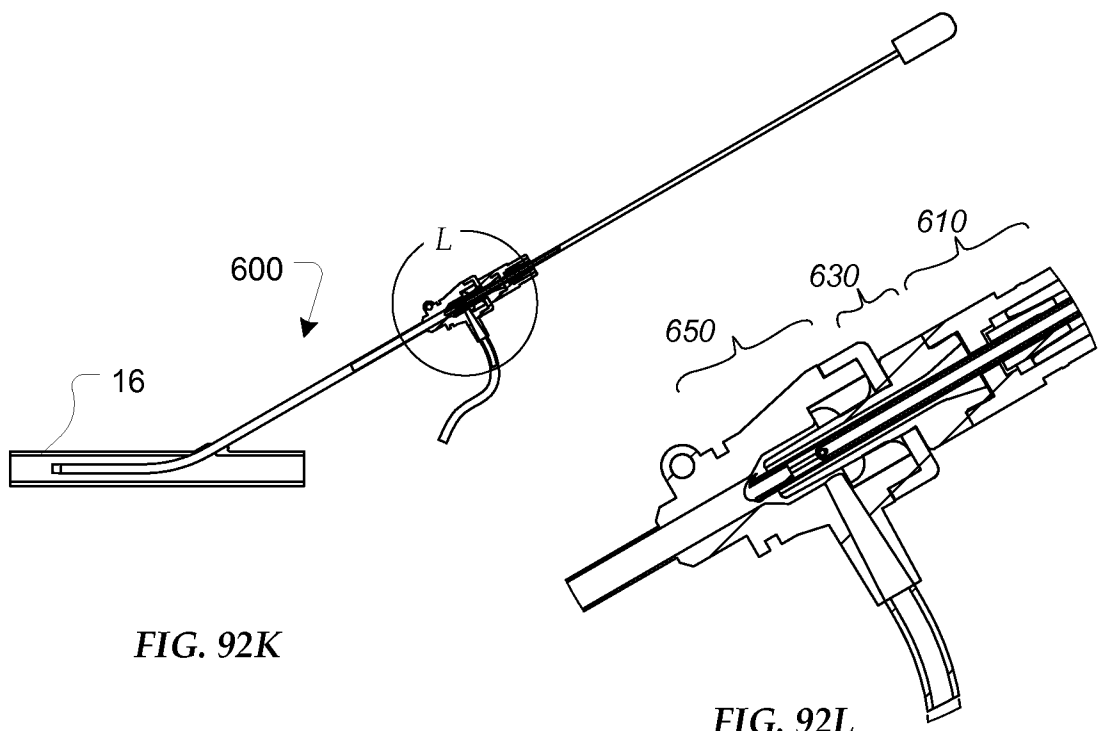


FIG. 92K

FIG. 92L

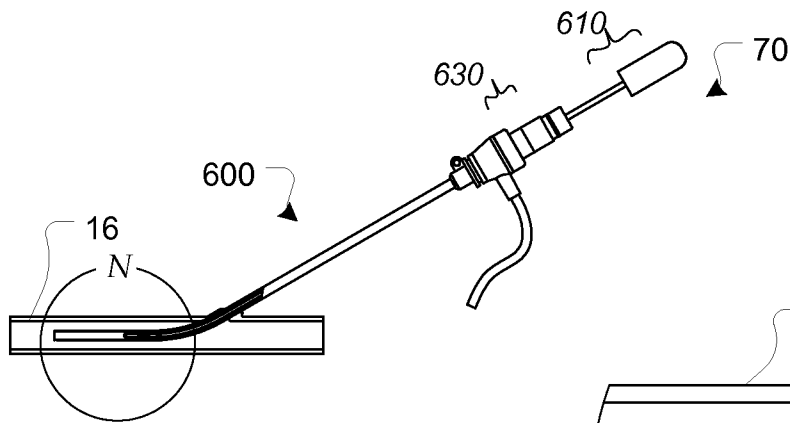


FIG. 92M

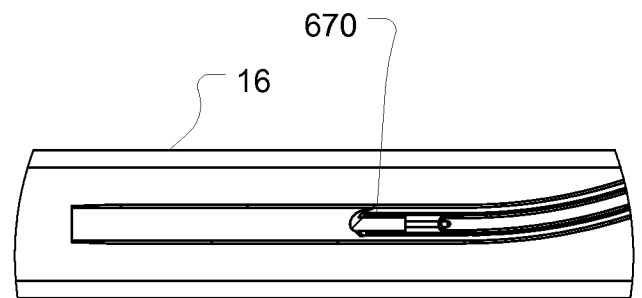


FIG. 92N

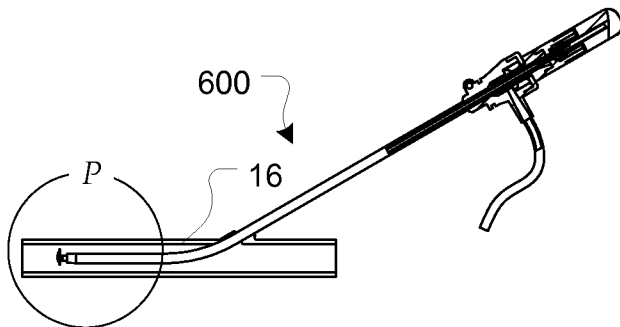


FIG. 92O

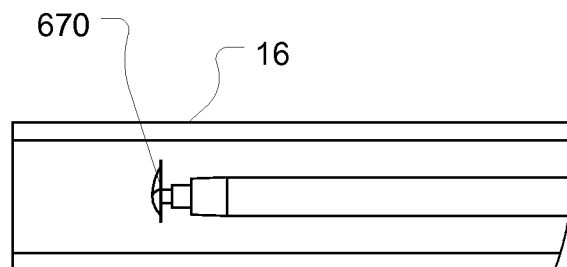


FIG. 92P

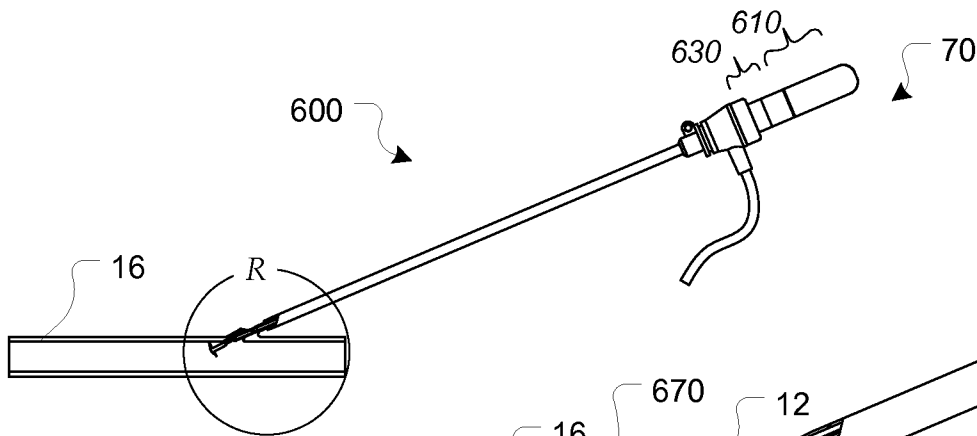


FIG. 92Q

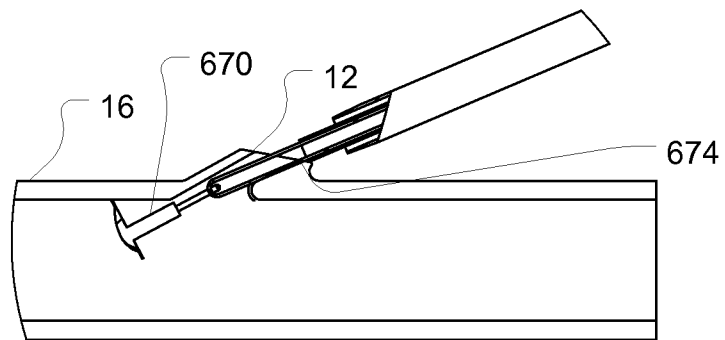


FIG. 92R

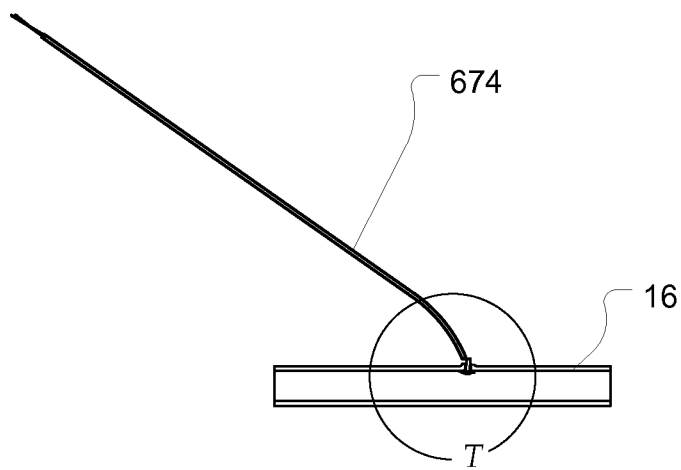


FIG. 92S

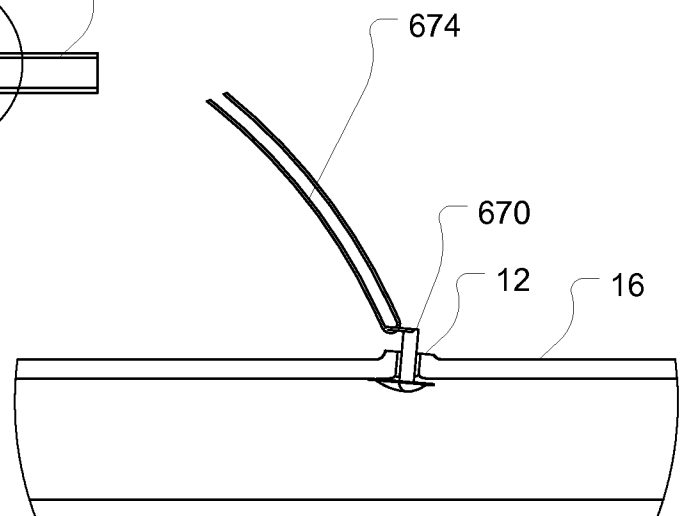


FIG. 92T

专利名称(译)	组织闭合装置，用于递送的装置和系统，试剂盒及其方法		
公开(公告)号	EP2416711A4	公开(公告)日	2017-06-07
申请号	EP2010762492	申请日	2010-04-09
[标]申请(专利权)人(译)	心血管科技股份有限公司		
申请(专利权)人(译)	心血管TECHNOLOGIES , INC.		
当前申请(专利权)人(译)	心血管技术公司		
[标]发明人	HOUSER RUSSELL A BOWER JOHN HUNTER DO PAUL L		
发明人	HOUSER, RUSSELL, A. BOWER, JOHN, HUNTER DO, PAUL, L.		
IPC分类号	A61B17/03 A61B17/34 A61M31/00 A61F2/84		
CPC分类号	A61B17/0057 A61B17/0644 A61B17/12109 A61B17/12172 A61B17/32 A61B17/3209 A61B18/1482 A61B50/30 A61B2017/00477 A61B2017/00615 A61B2017/00623 A61B2017/00659 A61B2017/00668 A61B2017/00672 A61B2017/0462 A61B2017/0641 A61B2018/00601 A61B2018/00916 A61B2018/ /1412 A61B2018/1455 A61B2090/036 A61B2090/037		
优先权	61/212296 2009-04-09 US 61/277359 2009-09-21 US 61/280896 2009-11-09 US		
其他公开文献	EP2416711A2		
外部链接	Espacenet		

摘要(译)

本发明涉及伤口闭合装置，用于递送的装置和系统，试剂盒及其方法。
伤口闭合装置可以实现伤口闭合而不是压缩，并且可以构造成可以通过
导引器或从身体外部快速展开。