

(19)



(11)

EP 1 479 348 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
09.07.2008 Bulletin 2008/28

(51) Int Cl.:
A61B 17/072 (2006.01)

(21) Application number: **04252979.2**

(22) Date of filing: **20.05.2004**

(54) **Surgical stapling instrument having a single lockout mechanism**

Chirurgisches Klammersetzgerät mit einem einzigen Verriegelungsmechanismus

Agrafeuse chirurgicale avec un seul mécanisme de verrouillage

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IT LI LU MC NL PL PT RO SE SI SK TR**

(30) Priority: **20.05.2003 US 441424**

(43) Date of publication of application:
24.11.2004 Bulletin 2004/48

(73) Proprietor: **Ethicon Endo-Surgery, Inc.**
Cincinnati, OH 45242 (US)

(72) Inventors:
• **Shelton, Frederick E. IV**
Hillsboro,
Ohio 45133 (US)

- **Setser, Michael E.**
Burlington,
Kentucky 41005 (US)
- **Weisenburgh, William B.**
Maineville,
Ohio 45039 (US)

(74) Representative: **Tunstall, Christopher Stephen et al**
Carpmaels & Ransford
43-45 Bloomsbury Square
London WC1A 2RA (GB)

(56) References cited:
US-A- 5 465 895 **US-A- 6 109 500**
US-B1- 6 202 914

EP 1 479 348 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Field of the Invention

[0001] The present invention relates in general to surgical stapler instruments that are capable of applying lines of staples to tissue while cutting the tissue between those staple lines and, more particularly, to improvements relating to stapler instruments and improvements in processes for forming various components of such stapler instruments.

Background of the Invention

[0002] Surgical staplers have been used in the prior art to simultaneously make a longitudinal incision in tissue and apply lines of staples on opposing sides of the incision. Such instruments commonly include a pair of cooperating jaw members that, if the instrument is intended for endoscopic or laparoscopic applications, are capable of passing through a cannula passageway. One of the jaw members receives a staple cartridge having at least two laterally spaced rows of staples. The other jaw member defines an anvil having staple-forming pockets aligned with the rows of staples in the cartridge. The instrument includes a plurality of reciprocating wedges which, when driven distally, pass through openings in the staple cartridge and engage drivers supporting the staples to effect the firing of the staples toward the anvil.

[0003] Examples of surgical staplers suitable for endoscopic applications are described in U.S. Pat. No. 5,465,895, and US 6, 202, 914 (upon which the preamble of claim 1 is based), both of which advantageously provide distinct closing and firing actions. Thereby, a clinician is able to close the jaw members upon tissue to position the tissue prior to firing. Once the clinician has determined that the jaw members are properly gripping tissue, the clinician can then fire the surgical stapler, thereby severing and stapling the tissue. The simultaneous severing and stapling avoids complications that may arise when performing such actions sequentially with different surgical tools that respectively only sever or staple.

[0004] It is often advantageous to build an end effector for the surgical stapler that is reusable. For instance, one patient may need a series of severing and stapling operations. Replacing an entire end effector for each operation tends to be economically inefficient. This is especially true if the end effector is built to be strong and reliable over repeated operations. To that end, staple cartridges are fitted into the end effector prior to each operation of the surgical stapler. Thus, a much smaller amount of the surgical staples is discarded after each use.

[0005] While the staple cartridge provides numerous advantages, it is desirable to prevent inadvertent firing of the surgical stapler when an unfired staple cartridge is not present. Otherwise, the severing of tissue may occur without the staples to minimize bleeding.

[0006] It is particularly desirable that preventing such

inadvertent firing be accomplished in a reliable way that is not subject to an intervening malfunction. Moreover, for ease of manufacturing and assembly, it is further desirable that the lockout features be accomplished with a minimum number of components.

[0007] Consequently, a significant need exists for an improved surgical stapling and severing instrument that prevents inadvertent firing (i.e., severing and stapling) when a staple cartridge is not installed or is spent, having been previously fired.

Brief Summary of the Invention

[0008] The invention overcomes the above-noted and other deficiencies of the prior art by providing a single lockout mechanism that prevents firing a surgical stapling and severing instrument when either a staple cartridge is not installed or is spent. In particular, the single lock mechanism prevents distal movement of a firing bar, and thus severing of tissue, in instances where simultaneous stapling would not occur.

[0009] In one aspect of the invention, a surgical instrument includes a handle portion operable to produce a firing motion that actuates an implement portion. This implement portion has an elongate channel that receives a staple cartridge with a firing drive slot defined therebetween. A firing mechanism engages the elongate channel along its longitudinal length and includes an engaging device that traverses the firing drive slot for distally moving a wedge sled in the staple cartridge. A lockout mechanism is advantageously positioned to be moved out of the firing drive slot by the presence of the wedge sled in its unfired, proximal position, and thus allowing the firing bar to fire. When the wedge sled is no longer in the unfired position (i.e., spent cartridge or missing cartridge), the lockout mechanism resiliently moves into the firing drive slot. The proximal and distal sides of the lockout mechanism present in the firing drive slot are shaped to allow the engaging device of the firing bar to return to its proximal, initial position but to thereafter impede distal movement until an unfired staple cartridge is installed.

[0010] These and other objects and advantages of the present invention shall be made apparent from the accompanying drawings and the description thereof.

Brief Description of the Figures

[0011] The accompanying drawings, which are incorporated in and constitute a part of this specification, illustrate embodiments of the invention, and, together with the general description of the invention given above, and the detailed description of the embodiments given below, serve to explain the principles of the present invention.

[0012] FIG. 1 depicts a partially cut-away side elevation view of a surgical stapling and severing instrument in an open position.

[0013] FIG. 2 depicts a cross-sectional side elevation detail view along the line 2-2 of FIG. 1 of an end effector

of the surgical stapling and severing instrument.

[0014] FIG. 3 depicts an enlarged side elevation view of the firing bar of the surgical stapling and severing instrument of FIG. 2.

[0015] FIG. 4 depicts an enlarged front view of the firing bar of the surgical stapling and severing instrument of FIG. 2.

[0016] FIG. 5 depicts a cross-sectional side elevation detail view of an alternative end effector for the surgical stapling and severing instrument of FIG. 1, incorporating a firing bar that lacks a middle pin for preventing pinching of the end effector.

[0017] FIG. 6 depicts a side elevational view of a handle portion of a proximal end of the surgical stapling and severing instrument of FIG. 1 with a left side removed to expose interior parts in an unclamped, unfired ("start") position.

[0018] FIG. 7 depicts a perspective, exploded view of the handle portion of the proximal end of the surgical stapling and severing instrument of FIG. 1.

[0019] FIG. 8 depicts a side elevational view of the handle portion of the proximal end of the surgical stapling and severing instrument of FIG. 1 with the left side removed to expose interior parts in the closed ("clamped") position.

[0020] FIG. 9 depicts a side elevational view of the handle portion of proximal end of surgical stapling and severing instrument of FIG. 1 with the left side removed to expose interior parts in the stapled and severed ("fired") position.

[0021] FIG. 10 depicts an isometric view of the end effector at the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position exposing the staple cartridge and cutting edge of the firing bar.

[0022] FIG. 11 depicts an isometric, exploded view of the implement portion of the surgical stapling and severing instrument of FIG. 1.

[0023] FIG. 12 depicts an isometric view of the end effector at the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position with the cartridge largely removed exposing a single staple driver and a double staple driver as exemplary and the wedge sled in its start position against a middle pin of the firing bar.

[0024] FIG. 13 depicts an isometric view of the distal end of the surgical stapling and severing instrument of FIG. 1 with the anvil in the up or open position with the staple cartridge completely removed and a portion of an elongate channel removed to expose a lowermost pin of the firing bar.

[0025] FIG. 14 depicts a side elevation view in section showing a mechanical relationship between the anvil, elongate channel, and staple cartridge in the closed position of the surgical stapling and severing instrument of FIG. 1, the section generally taken along lines 14-14 of FIG. 10 to expose wedge sled, staple drivers and staples but also depicting the firing bar along the longitudinal

centerline.

[0026] FIG. 15 depicts a section view of the end effector of the surgical stapling and severing instrument with the cartridge and firing bar in the start position taken along line 15-15 of FIG. 10.

[0027] FIG. 16 depicts a section view taken along line 16-16 of FIG. 15 showing the cross-sectional relationship between the firing bar, elongate channel, wedge sled, staple drivers, staples and staple cartridge.

[0028] FIG. 17 depicts a side elevation section view of the surgical stapling and severing instrument of FIG. 1 taken along the longitudinal centerline of the end effector in a partially closed but unclamped position gripping tissue.

[0029] FIG. 18 depicts a partially cut-away side elevational view of the surgical stapling and severing instrument of FIG. 1 in the closed or clamped position.

[0030] FIG. 19 depicts a side elevation view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in the closed or clamped position with tissue properly compressed.

[0031] FIG. 20 depicts a partially cut-away side elevational view of the surgical stapling and severing instrument of FIG. 1 in a partially fired position.

[0032] FIG. 21 depicts a view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in a partially fired position.

[0033] FIG. 22 depicts a partially cut-away side elevational view of the surgical stapling and severing instrument of FIG. 1 in a fully fired position.

[0034] FIG. 23 depicts a view in centerline section of the distal end of the surgical stapling and severing instrument of FIG. 1 in a fully fired position.

[0035] FIG. 24 depicts a perspective view looking distally at the elongate channel of FIG. 1 partially cut away to expose a cartridge body and a single lockout mechanism engaging a middle pin of a firing bar.

[0036] FIGS. 25-28 depict a cross-sectional side detail view of the single lockout mechanism, staple cartridge and firing bar of FIG. 24, sequentially shown in a cartridge loaded and unfired state in FIG. 25, a cartridge being fired state in FIG. 26, a spent cartridge with firing bar being retracted state in FIG. 27, and spent cartridge with firing bar retracted state in FIG. 28.

[0037] FIG. 29 depicts the single lockout mechanism of FIG. 24 further incorporating a lockout trough.

[0038] FIG. 30 depicts a bottom perspective view of an elongate channel of FIG. 1 partially cut away to show another single lockout mechanism engaging the middle pin of a firing bar when a staple cartridge is missing.

[0039] FIGS. 31-34 depict a cross-sectional side detail view of the single lockout mechanism of FIG. 30, sequentially shown in a cartridge loaded and unfired state in FIG. 31, a cartridge being fired state in FIG. 32, a spent cartridge with firing bar being retracted state in FIG. 33, and a spent cartridge with firing bar retracted state in FIG. 34.

Detailed Description of the Invention

[0040] Turning to the Drawings, wherein like numerals denote like components throughout the several views, FIG. 1 and 2 depict a surgical stapling and severing instrument 10 that is capable of practicing the unique benefits of the present invention. The surgical stapling and severing instrument 10 incorporates an end effector 12 having an E-beam firing mechanism ("firing bar") 14 that advantageously controls the spacing of the end effector 12. In particular, an elongate channel 16 and a pivotally translatable anvil 18 are maintained at a spacing that assures effective stapling and severing. Furthermore, firing (i.e., severing and stapling) is prevented from occurring if the instrument is not capable of stapling with a single lockout mechanism, which is described in more detail below.

[0041] The surgical and stapling and severing instrument 10 includes a handle portion 20 connected to an implement portion 22, the latter further comprising a shaft 23 distally terminating in the end effector 12. The handle portion 20 includes a pistol grip 24 toward which a closure trigger 26 is pivotally drawn by the clinician to cause clamping, or closing, of the anvil 18 toward the elongate channel 16 of the end effector 12. A firing trigger 28 is farther outboard of the closure trigger 26 and is pivotally drawn by the clinician to cause the stapling and severing of clamped tissue in the end effector 12.

[0042] It will be appreciated that the terms "proximal" and "distal" are used herein with reference to a clinician gripping a handle of an instrument. Thus, the end effector 12 is distal with respect to the more proximal handle portion 20. It will be further appreciated that for convenience and clarity, spatial terms such as "vertical" and "horizontal" are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

[0043] Closure trigger 26 is actuated first. Once the clinician is satisfied with the positioning of the end effector 12, the clinician may draw back the closure trigger 26 to its fully closed, locked position proximate to the pistol grip 24. Then, the firing trigger 28 is actuated. The firing trigger 28 springedly returns when the clinician removes pressure. A release button 30 when depressed on the proximal end of the handle portion 20 releases any locked closure trigger 26.

[0044] A closure sleeve 32 encloses a frame 34, which in turn encloses a firing drive member 36 that is positioned by the firing trigger 28. The frame 34 connects the handle portion 20 to the end effector 12. With the closure sleeve 32 withdrawn proximally by the closure trigger 26 as depicted, the anvil 18 springedly opens, pivoting away from the elongate channel 16 and translating proximally with the closure sleeve 32.

[0045] The elongate channel 16 receives a staple cartridge 37 that is responsive to the firing bar 14 to drive staples into forming contact with the anvil 18. It will ap-

preciated that although a readily replaceable staple cartridge 37 is advantageously described herein, a staple cartridge 37 consistent with aspects of the present invention may be permanently affixed or integral to the elongate channel 16, for instance when a larger portion of the end effector 12 is replaced after each firing.

E-BEAM FIRING MECHANISM

[0046] With particular reference to FIGS. 2-4, the firing bar 14 includes three vertically spaced pins that control the spacing of the end effector 12 during firing. In particular, an upper pin 38 is staged to enter an anvil pocket 40 near the pivot between the anvil 18 and elongate channel 16. When fired with the anvil 18 closed, the upper pin 38 advances distally within a longitudinal anvil slot 42 extending distally through anvil 18. Any minor upward deflection in the anvil 18 is overcome by a downward force imparted by the upper pin 38.

[0047] Firing bar 14 also includes a lower most pin, or firing bar cap, 44 that upwardly engages a channel slot 45 in the elongate channel 16, thereby cooperating with the upper pin 38 to draw the anvil 18 and the elongate channel 16 slightly closer together in the event of excess tissue clamped therebetween.

[0048] The firing bar 14 advantageously includes a middle pin 46 that passes through a firing drive slot 47 formed in a lower surface of the cartridge 37 and an upward surface of the elongate channel 16, thereby driving the staples therein as described below. The middle pin 46, by sliding against the elongate channel 16, advantageously resists any tendency for the end effector 12 to be pinched shut at its distal end. To illustrate an advantage of the middle pin 46, FIG. 5 depicts an alternative end effector 12' that lacks a middle pin on a firing bar 14'. In this depiction, the end effector 12' is allowed to pinch shut at its distal end, which tends to impair desired staple formation.

[0049] Returning to FIGS. 2-4, a distally presented cutting edge 48 between the upper and middle pins 38, 46 on the firing bar 14 traverses through a proximally presented, vertical slot 49 in the cartridge 37 to sever clamped tissue. The affirmative positioning of the firing bar 14 with regard to the elongate channel 16 and anvil 18 assure that an effective cut is performed.

CAMBERED ANVIL WITH SELECTED CARTRIDGE GAP

[0050] The affirmative vertical spacing provided by the E-Beam firing bar 14 is suitable for the limited size available for endoscopic devices. Moreover, the E-Beam firing bar 14 enables fabrication of an anvil 16 with a camber imparting a vertical deflection at its distal end, similar to the position depicted in FIG. 5. This cambered anvil 16 advantageously assists in achieving the desired gap in the end effector 12 even with an anvil 16 reduced thickness, which is thus more suited to the size limitations of

an endoscopic device.

[0051] The E-Beam firing bar 14 further enables increased applications, especially in combination with a range of configurations of staple cartridges. For instance, a clinician may select a gray staple cartridge yielding a 0.02 mm tissue gap, a white staple cartridge yielding a 0.04 mm tissue gap, a blue cartridge yielding a 0.06 mm tissue gap, or a green cartridge yielding a 0.10 mm tissue gap. The vertical height of each respective staple cartridge in combination with the length of staples and an integral wedge sled (described in more detail below) pre-determines this desired tissue thickness with the anvil 18 appropriately vertically spaced by the E-Beam firing bar 14.

TWO-AXIS HANDLE

[0052] With reference to FIGS. 6-9, the handle portion 20 is comprised of first and second base sections 50 and 52, which are molded from a polymeric material such as a glass-filled polycarbonate. The first base section 50 is provided with a plurality of cylindrical-shaped pins 54. The second base section 52 includes a plurality of extending members 56, each having a hexagonal-shaped opening 58. The cylindrical-shaped pins 54 are received within the hexagonal-shaped openings 58 and are frictionally held therein for maintaining the first and second base sections 50 and 52 in assembly.

[0053] A rotating knob 60 has a bore 62 extending completely through it for engaging and rotating the implement portion 22 about its longitudinal axis. The rotating knob 60 includes an inwardly protruding boss 64 extending along at least a portion of the bore 62. The protruding boss 64 is received within a longitudinal slot 66 formed at a proximal portion of the closure sleeve 32 such that rotation of the rotating knob 60 effects rotation of the closure sleeve 32. It will be appreciated that the boss 64 further extends through frame 34 and into contact with a portion of the firing drive member 36 to effect their rotation as well. Thus, the end effector 12 (not shown in FIGS. 6-9) rotates with the rotating knob 60.

[0054] A proximal end 68 of the frame 34 passes proximally through the rotating knob 60 and is provided with a circumferential notch 70 that is engaged by opposing channel securement members 72 extending respectively from the base sections 50 and 52. Only the channel securement member 72 of the second base section 52 is shown. The channel securement members 72 extending from the base sections 50, 52 serve to secure the frame 34 to the handle portion 20 such that the frame 34 does not move longitudinally relative to the handle portion 20.

[0055] The closure trigger 26 has a handle section 74, a gear segment section 76, and an intermediate section 78. A bore 80 extends through the intermediate section 78. A cylindrical support member 82 extending from the second base section 52 passes through the bore 80 for pivotally mounting the closure trigger 26 on the handle portion 20. A second cylindrical support member 83 ex-

tending from the second base section 52 passes through a bore 81 of firing trigger 28 for pivotally mounting on the handle portion 20. A hexagonal opening 84 is provided in the cylindrical support member 83 for receiving a securement pin (not shown) extending from the first base section 50.

[0056] A closure yoke 86 is housed within the handle portion 20 for reciprocating movement therein and serves to transfer motion from the closure trigger 26 to the closure sleeve 32. Support members 88 extending from the second base section 52 and securement member 72, which extends through a recess 89 in the yoke 86, support the yoke 86 within the handle portion 20.

[0057] A proximal end 90 of the closure sleeve 32 is provided with a flange 92 that is snap-fitted into a receiving recess 94 formed in a distal end 96 of the yoke 86. A proximal end 98 of the yoke 86 has a gear rack 100 that is engaged by the gear segment section 76 of the closure trigger 26. When the closure trigger 26 is moved toward the pistol grip 24 of the handle portion 20, the yoke 86 and, hence, the closure sleeve 32 move distally, compressing a spring 102 that biases the yoke 86 proximally. Distal movement of the closure sleeve 32 effects pivotal translation movement of the anvil 18 distally and toward the elongate channel 16 of the end effector 12 and proximal movement effects closing, as discussed below.

[0058] The closure trigger 26 is forward biased to an open position by a front surface 130 interacting with an engaging surface 128 of the firing trigger 28. Clamp first hook 104 that pivots top to rear in the handle portion 20 about a pin 106 restrains movement of the firing trigger 28 toward the pistol grip 24 until the closure trigger 26 is clamped to its closed position. Hook 104 restrains firing trigger 28 motion by engaging a lockout pin 107 in firing trigger 28. The hook 104 is also in contact with the closure trigger 26. In particular, a forward projection 108 of the hook 104 engages a member 110 on the intermediate section 78 of the closure trigger 26, the member 110 being outward of the bore 80 toward the handle section 74. Hook 104 is biased toward contact with member 110 of the closure trigger 26 and engagement with lockout pin 107 in firing trigger 28 by a release spring 112. As the closure trigger 26 is depressed, the hook 104 is moved top to rear, compressing the release spring 112 that is captured between a rearward projection 114 on the hook 104 and a forward projection 116 on the release button 30.

[0059] As the yoke 86 moves distally in response to proximal movement of the closure trigger 26, an upper latch arm 118 of the release button 30 moves along an upper surface 120 on the yoke 86 until dropping into an upwardly presented recess 122 in a proximal, lower portion of the yoke 86. The release spring 112 urges the release button 30 outward, which pivots the upper latch arm 118 downwardly into engagement with the upwardly presented recess 122, thereby locking the closure trigger 26 in a tissue clamping position, such as depicted in FIG.

8.

[0060] The latch arm 118 can be moved out of the recess 122 to release the anvil 18 by pushing the release button 30 inward. Specifically, the upper latch arm 118 pivots upward about pin 123 of the second base section 52. The yoke 86 is then permitted to move proximally in response to return movement of the closure trigger 26.

[0061] A firing trigger return spring 124 is located within the handle portion 20 with one end attached to pin 106 of the second base section 52 and the other end attached to a pin 126 on the firing trigger 28. The firing return spring 124 applies a return force to the pin 126 for biasing the firing trigger 28 in a direction away from the pistol grip 24 of the handle portion 20. The closure trigger 26 is also biased away from pistol grip 24 by engaging surface 128 of firing trigger 28 biasing front surface 130 of closure trigger 26.

[0062] As the closure trigger 26 is moved toward the pistol grip 24, its front surface 130 engages with the engaging surface 128 on the firing trigger 28 causing the firing trigger 28 to move to its "firing" position. When in its firing position, the firing trigger 28 is located at an angle of approximately 45° to the pistol grip 24. After staple firing, the spring 124 causes the firing trigger 28 to return to its initial position. During the return movement of the firing trigger 28, its engaging surface 128 pushes against the front surface 130 of the closure trigger 26 causing the closure trigger 26 to return to its initial position. A stop member 132 extends from the second base section 52 to prevent the closure trigger 26 from rotating beyond its initial position.

[0063] The surgical stapling and severing instrument 10 additionally includes a reciprocating section 134, a multiplier 136 and a drive member 138. The reciprocating section 134 comprises a wedge sled in the implement portion 22 (not shown in FIG. 6-9) and a metal drive rod 140.

[0064] The drive member 138 includes first and second gear racks 141 and 142. A first notch 144 is provided on the drive member 138 intermediate the first and second gear racks 141, 142. During return movement of the firing trigger 28, a tooth 146 on the firing trigger 28 engages with the first notch 144 for returning the drive member 138 to its initial position after staple firing. A second notch 148 is located at a proximal end of the metal drive rod 140 for locking the metal drive rod 140 to the upper latch arm 118 of the release button 30 in its unfired position.

[0065] The multiplier 136 comprises first and second integral pinion gears 150 and 152. The first integral pinion gear 150 is engaged with a first gear rack 154 provided on the metal drive rod 140. The second integral pinion gear 152 is engaged with the first gear rack 141 on the drive member 138. The first integral pinion gear 150 has a first diameter and the second integral pinion gear 152 has a second diameter which is smaller than the first diameter.

[0066] FIGS. 6, 8 and 9 depict respectively the handle portion 20 in the start position (open and unfired), a

clamped position (closed and unfired) and a fired position. The firing trigger 28 is provided with a gear segment section 156. The gear segment section 156 engages with the second gear rack 142 on the drive member 138 such that motion of the firing trigger 28 causes the drive member 138 to move back and forth between a first drive position, shown in FIG. 8, and a second drive position, shown in FIG. 9. In order to prevent staple firing before tissue clamping has occurred, the upper latch arm 118 on the release button 30 is engaged with the second notch 148 on the drive member 138 such that the metal drive rod 140 is locked in its proximal-most position, as depicted in FIG. 6. When the upper latch arm 118 falls into the recess 122, the upper latch arm 118 disengages with the second notch 148 to permit distal movement of the metal drive rod 140, as depicted in FIG. 9.

[0067] Because the first gear rack 141 on the drive member 138 and the gear rack 154 on the metal drive rod 140 are engaged with the multiplier 136, movement of the firing trigger 28 causes the metal drive rod 140 to reciprocate between a first reciprocating position, shown in FIG. 8, and a second reciprocating position, shown in FIG. 9. Since the diameter of the first pinion gear 150 is greater than the diameter of the second pinion gear 152, the multiplier 136 moves the reciprocating section 134 a greater distance than the drive member 138 is moved by the firing trigger 28. The diameters of the first and second pinion gears 150 and 152 may be changed to permit the length of the stroke of the firing trigger 28 and the force required to move it to be varied.

[0068] It will be appreciated that the handle portion 20 is illustrative and that other actuation mechanisms may be employed. For instance, the closing and firing motions may be generated by automated means.

SEPARATE AND DISTINCT CLOSING AND FIRING END EFFECTOR

[0069] The end effector 12 of the surgical stapling and severing instrument 10 is depicted in further detail in FIGS. 10-16. As described above, the handle portion 20 produces separate and distinct closing and firing motions that actuate the end effector 12. The end effector 12 advantageously maintains the clinical flexibility of this separate and distinct closing and firing (i.e., stapling and severing). In addition, the end effector 12 introduces the aforementioned ability to affirmatively maintain the closed spacing during firing after the clinician positions and clamps the tissue. Both features procedurally and structurally enhance the ability of the surgical stapling and severing instrument 10 by ensuring adequate spacing for instances where an otherwise inadequate amount of tissue is clamped and to enhance the clamping in instances where an otherwise excessive amount of tissue has been clamped.

[0070] FIG. 10 depicts the end effector 12, which is in an open position by a retracted closure sleeve 32, with a staple cartridge 37 installed in the elongate channel

16. On a lower surface 200 of the anvil 18, a plurality of stapling forming pockets 202 are arrayed to correspond to a plurality of stapler apertures 204 in an upper surface 206 of the staple cartridge 37. The firing bar 14 is at its proximal position, with the upper pin 38 aligned in a non-interfering fashion with the anvil pocket 40. The anvil pocket 40 is shown as communicating with the longitudinal anvil slot 42 in the anvil 18. The distally presented cutting edge 48 of the firing bar 14 is aligned with and proximally from removed from the vertical slot 49 in the staple cartridge 37, thereby allowing removal of a spent cartridge and insertion of an unfired cartridge, which is snapfit into the elongate channel 16. Specifically, extension features 208, 210 of the staple cartridge 37 engage recesses 212, 214 (shown in FIG. 12) of the elongate channel 16.

[0071] FIG. 11 shows the implement portion 22 of the surgical stapling and severing instrument 10 in disassembled form. The staple cartridge 37 is shown as being comprised of a cartridge body 216, a wedge sled 218, single and double drivers 220, staples 222, and a cartridge tray 224. When assembled, the cartridge tray 224 holds the wedge sled 218, single and double drivers 220, and staples 222 inside the cartridge body 216.

[0072] Having a wedge sled 218 integral to the staple cartridge 37 enables a number of flexible design options as compared to incorporating camming surfaces onto a firing bar itself. For instance, a number of different staple cartridges may be selected for use in the instrument 10 with each staple cartridge having a different configuration of rows of staples, each thus having a unique wedge sled configured to contact the middle pin 46 of the firing bar 14 while causing the driving of the staples 222. As another example, the integral wedge sled 218 provides an opportunity for a number of lockout features, described in greater detail below.

[0073] The elongate channel 16 has a proximally placed attachment cavity 226 that receives a channel anchoring member 228 on the distal end of the frame 34 for attaching the end effector 12 to the handle portion 20. The elongate channel 16 also has an anvil cam slot 230 that pivotally receives an anvil pivot 232 of the anvil 18. The closure sleeve 32 that encompasses the frame 34 includes a distally presented tab 234 that engages an anvil feature 236 proximate but distal to the anvil pivot 232 on the anvil 18 to thereby effect opening and closing of the anvil 18. The firing drive member 36 is shown as being assembled from the firing bar 14 attached to a firing connector 238 by pins 240, which in turn is rotatably and proximally attached to the metal drive rod 140. The firing bar 14 is guided at a distal end of the frame by a slotted guide 239 inserted therein.

[0074] With particular reference to FIG. 12, a portion of the staple cartridge 37 is removed to expose portions of the elongate channel 16, such as recesses 212, 214 and to expose some components of the staple cartridge 37 in their unfired position. In particular, the cartridge body 216 (shown in FIG. 11) has been removed. The

wedge sled 218 is shown at its proximal, unfired position with a pusher block 242 contacting the middle pin 46 (not shown in FIG. 12) of the firing bar 14. The wedge sled 218 is in longitudinal sliding contact upon the cartridge tray 224 and includes wedges 228 that force upward the single and double drivers 220 as the wedge sled 218 moves distally. Staples 222 (not shown in FIG. 12) resting upon the drivers 220 are thus also forced upward into contact with the anvil forming pockets 202 on the anvil 18 to form closed staples. Also depicted is the channel slot 45 in the elongate channel 16 that is aligned with the vertical slot 49 in the staple cartridge 37.

[0075] FIG. 13 depicts the end effector 12 of FIG. 12 with all of the staple cartridge 37 removed to show the middle pin 46 of the firing bar 14 as well as portion of the elongate channel 16 removed adjacent to the channel slot 45 to expose the firing bar cap 44. In addition, portions of the shaft 23 are removed to expose a proximal portion of the firing bar 14. Projecting downward from the anvil 18 near the pivot, a pair of opposing tissue stops 244 prevent tissue being positioned too far up into the end effector 12 during clamping.

[0076] FIG. 14 depicts the end effector 12 closed in a tissue clamping position with the firing bar 14 unfired. The upper pin 38 is in the anvil pocket 40, vertically aligned with the anvil slot 42 for distal longitudinal movement of the firing bar 14 during firing. The middle pin 46 is positioned to push the wedge sled 218 distally so that wedge 228 sequentially contacts and lifts double drivers 220 and the respective staples 222 into forming contact with staple forming pockets 202 in the lower surface 200 of the anvil 18.

[0077] FIG. 15 depicts the upper surface 206 of the staple cartridge 37 with the firing bar 14 in its unfired, proximal position. The stapler apertures 204 are arrayed on each side of the vertical slot 49 in the staple cartridge 37.

[0078] FIG. 16 depicts the end effector 12 near the pivot showing that the elongate channel 16 has opposing ramp portions 246 to thereby cooperate with the tissue stops 244 of the anvil 18 (not shown in FIG. 16) to prevent tissue from jamming the end effector 12. Also depicted in greater detail are the double drivers 220 and their relation to the staples 222.

OPERATION

[0079] In use, the surgical stapling and severing instrument 10 is used as depicted in FIGS 1, 2, and 17-23. In FIGS. 1-2, the instrument 10 is in its start position, having had an unfired, fully loaded staple cartridge 37 snap-fitted into the distal end of the elongate channel 16. Both triggers 26, 28 are forward and the end effector 12 is open, such as would be typical after inserting the end effector 12 through a trocar or other opening into a body cavity. The instrument 10 is then manipulated by the clinician such that tissue 248 to be stapled and severed is positioned between the staple cartridge 37 and the anvil 18,

as depicted in FIG. 17.

[0080] With reference to FIGS. 18-19, next, the clinician moves the closure trigger 26 proximally until positioned directly adjacent to the pistol grip 24, locking the handle portion 20 into the closed and clamped position. The retracted firing bar 14 in the end effector 12 does not impede the selective opening and closing of the end effector 12, but rather resides within the anvil pocket 40. With the anvil 18 closed and clamped, the E-beam firing bar 14 is aligned for firing through the end effector 12. In particular, the upper pin 38 is aligned with the anvil slot 42 and the elongate channel 16 is affirmatively engaged about the channel slot 45 by the middle pin 46 and the firing bar cap 44.

[0081] With reference to FIGS. 20-21, after tissue clamping has occurred, the clinician moves the firing trigger 28 proximally causing the firing bar 14 to move distally into the end effector 12. In particular, the middle pin 46 enters the staple cartridge 37 through the firing drive slot 47 to effect the firing of the staples 222 (not shown in FIGS. 20-21) via wedge sled 218 toward the anvil 18. The lower most pin, or firing bar cap 44, cooperates with the middle pin 46 to slidably position cutting edge 48 of the firing bar 14 to sever tissue. The two pins 44, 46 also position the upper pin 38 of the firing bar 14 within longitudinal anvil slot 42 of the anvil 18, affirmatively maintaining the spacing between the anvil 18 and the elongate channel 16 throughout its distal firing movement.

[0082] With reference to FIGS. 22-23, the clinician continues moving the firing trigger 28 until brought proximal to the closure trigger 26 and pistol grip 24. Thereby, all of the ends of the staples 222 are bent over as a result of their engagement with the anvil 18. The firing bar cap 44 is arrested against a firing bar stop 250 projecting toward the distal end of the channel slot 45. The cutting edge 48 has traversed completely through the tissue. The process is complete by releasing the firing trigger 28 and by then depressing the release button 30 while simultaneously squeezing the closure trigger 26 to open the end effector 12.

SINGLE LOCKOUT FOR MISSING/SPENT STAPLE CARTRIDGE

[0083] As described above, the E-beam firing bar 14 provides unique capabilities for affirmatively spacing the end effector 12 while simultaneously severing tissue and effecting the forming of staples on each side of the cut. With reference to FIG. 24, preventing the distal movement of the firing bar 14 thus prevents the inadvertent severing of tissue. A single lockout mechanism 270 according to the invention responds to a missing staple cartridge 37 or a spent staple cartridge 37, the latter condition depicted in FIG. 24, by blocking the middle pin 46 of the firing bar (only the middle pin of the firing bar being shown in FIG. 24).

[0084] In particular, the single lockout mechanism 270 is depicted as a pair of bent spring fingers 272 positioned

in the elongate channel 16 to respond to both conditions: missing cartridge and spent cartridge. In particular, the bent spring fingers 272 raise up to block the middle pin 46 of the firing bar 14 when the wedge sled 218 (not shown in FIG. 24) is not present, such as when the cartridge 37 is removed or when the cartridge 37 has been fired.

[0085] FIGS. 25-28 depict the single lockout mechanism 270, according to the claimed invention specifically the bent spring fingers 272 sequentially as the surgical stapling and severing instrument 10 is fired. In Fig. 25, an unfired staple cartridge 37 has been inserted into the elongate channel 16 with the wedge sled 218 depressing the bent spring fingers 272 so that the firing drive slot 47 formed between the cartridge 37 and the elongate channel 16 is unimpeded.

[0086] In FIG. 26, firing of the cartridge 37 has commenced, with the wedge sled 218 and the middle pin 46 of the firing bar 14 having distally traversed off of the bent spring fingers 272, which then spring up into the firing drive slot 47.

[0087] In FIG. 27, the staple cartridge 37 is now spent with the wedge sled 218 fully driven distally and no longer depicted. The firing bar 14 is being retracted proximally. Since the bent spring fingers 272 pivot from a more distal point, the firing bar 14 is able to ride up onto the bent spring fingers 272 during retraction, causing them to be depressed out of the firing drive slot 47.

[0088] In FIG. 28, the firing bar 14 is fully retracted and now confronts a non-depressed pair of bent spring fingers 272 to prevent distal movement. The single lockout mechanism 270 thereby activated remains during the period in which the spent staple cartridge 37 is removed until an unfired staple cartridge 37 is installed.

[0089] FIG. 29 depicts a lockout trough 274 that may advantageously be included in the single lockout mechanism 270 in order to provide increased mechanical strength. In some applications, it may be desirable to resist strong firing motions without damaging the bent spring fingers 272. The lockout trough 274 communicates with the firing drive slot 47 when the bent spring fingers 272 are not depressed. Moreover, the lockout trough 274 is downwardly ramped in a distal direction such that the middle pin 46 of the firing bar 14 is directed toward an abutting surface 276 at a distal end of the lockout trough 274, thereby reacting the distal movement of the firing bar 14 into an elongate channel 16'. In particular, the firing bar 14 in its initial position moves to a distal and lowered position, depicted at 14', wherein the middle pin 46 moves to a position depicted as 46'. It will be appreciated that the upper pin 38 and lower firing bar cap 44, as each moves to distal and lowered positions 38' and 44' respectively, position the middle pin 46 against elongate channel 16 so that the middle pin 46 enters the lockout trough 274.

[0090] It will be further appreciated that the firing bar 14' may be readily retracted from the lockout trough 274. Moreover, insofar as the upper pin 38' would be engaging

the anvil 18 (not shown in FIG. 29) in this position, the clinician would have to retract the firing bar 14' so that the anvil 18 could be opened in order to insert an unfired staple cartridge 37, and thus the firing bar 14 would be fully retracted and would not impede the depressing of the bent spring fingers 272 to their inactivated position.

[0091] FIG. 30 depicts another single lockout mechanism 270, also according to the claimed invention depicted as a pair of lockout hooks 280 having ramped ends 282 distally placed with regard to attachment devices 284 inserted through apertures 286 in the elongate channel 16. The ramped ends 282 lie above a hook recess 288 defined in the elongate channel 16. Thus, when each ramped end 282 is contacted by a wedge sled 218 of an unfired staple cartridge 37 (not shown in FIG. 30), the ramped ends 282 are depressed into the hook recess 288, thereby clearing the way for the middle pin 46 of the firing bar 14 (only the middle pin shown in FIG. 30) to move distally to fire the staple cartridge 37. A thin shaft 290 coupling the attachment devices 284 to respectively to the ramped end 282 of each lockout hook 280 resiliently responds to absence of a wedge sled 218, as depicted, wherein the ramped ends 282 return to impede the firing drive slot 47 to block a retracted middle pin 46 of the firing bar.

[0092] FIGS. 31-34 depict the sequence of operation of the lockout hooks 280. In FIG. 31, the staple cartridge 37 is unfired so that the distally positioned wedge sled 218 depresses the ramped ends 282 into the hook recess 288, allowing the middle pin 46 of the firing bar 14 to move distally during firing, as depicted in FIG. 32. With the wedge sled 218 and middle pin 46 distally removed with respect to the lockout mechanism 270, the ramped ends 282 resiliently raise out of the hook recess 282 to occupy the firing drive slot 47.

[0093] In FIG. 33, the firing bar 14 is being retracted to the point of contacting the ramped ends 282 of the lockout hook 280. Since the distal end of the ramped ends 282 is lower than the proximal part of the ramped ends 282, the middle pin 46 of the firing bar 14 rides over the ramped ends 282, forcing them down into the hook recess 288 until middle pin 46 is past the ramped ends 282, as depicted in FIG. 34, wherein the ramped ends 282 resiliently spring back up to block the middle pin 46. Thus, the firing bar 14 is prevented from distal movement while the spent staple cartridge 37 is replaced with an unfired staple cartridge 37.

[0094] While the present invention has been illustrated by description of several embodiments and while the illustrative embodiments have been described in considerable detail, it is not the intention of the applicant to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications may readily appear to those skilled in the art.

Claims

1. A surgical linear stapling instrument (10) comprising:

5 a handle portion (20) operably configured to produce a firing motion;
 an elongate channel (16) coupled to the handle portion (20);
 10 an anvil (18) pivotally attached to the elongate channel (16);
 a staple device (37) engaged by the elongate channel (16) and including a plurality of staple drivers (220) and a wedge member (218) distally movable through the staple device (37) to cam the staple drivers (220) toward the anvil (18);
 15 a firing device (14) moving distally from a proximalmost position in response to the firing motion to drive the wedge member (218) distally from a proximal position; and
 20 a lockout device (270); preventing firing of the instrument in the absence of an unspent staple device (37); **characterised in that**
 the lockout device (270) is disabled by the wedge member (218) when the wedge member (218) is in the proximal position;
 25 the wedge member (218) is separate from the firing device (14); and arranged such that retraction of the firing device (14) does not retract the wedge member (218); and
 30 the lockout device (270) is operably configured to prevent distal movement of the firing device (14) from its proximalmost position when the wedge member (218) is not in the proximal position.

2. The surgical instrument (10) of claim 1, wherein the staple device (37) comprises a replaceable device.

3. The surgical instrument (10) of claim 1, wherein the staple device (37) includes a firing drive slot (47) through which at least a portion of the firing device (14) distally traverses to drive the wedge member (218), the lockout device (270) resiliently intruding into the firing drive slot (47) from the elongate channel (16).

4. The surgical instrument (10) of claim 3, wherein the lockout device (270) presents a surface in the firing drive slot (47) ramped from the elongate channel (16) proximally.

5. The surgical instrument (10) of claim 4, wherein the lockout device (270) comprises a proximally directed spring finger (272).

6. The surgical instrument (10) of claim 5, wherein the elongate channel (16) includes a recess under the spring finger (272) to receive a portion of the firing

device (14).

7. The surgical instrument (10) of claim 4, wherein the lockout device (270) comprises a spring-biased plunger. 5
8. The surgical instrument (10) of claim 4, wherein the lockout device (270) comprises a ramped hook (104) springedly attached to the elongate channel (16). 10
9. The surgical instrument of claim 1, further comprising:
 - a shaft (23) attached to the handle portion (20) and operably configured for transferring the closing motion and the firing motion; and 15
 - a firing bar (14) coupled to the shaft (23) and responsive to the firing motion to distally traverse between the elongate channel (16) and the anvil (18); 20
 - wherein the handle portion (20) is operably configured to produce a closing motion; the elongate channel (16) is attached to the shaft (23); 25
 - the anvil (18) is responsive to the closing motion; the wedge member (218) is displaced by the firing bar (14) during firing; and 30
 - the lockout device (270) is disabled by a non-displaced wedge member (218). 35
10. The surgical instrument (10) of claim 9, wherein the staple device (37) comprises a replaceable device, 35

Patentansprüche

1. Chirurgisches, lineares Klammersetzgerät (10) umfassend:
 - ein Handteil (20), das derart betriebsgemäß konfiguriert ist, dass eine Schussbewegung erzeugt wird; 40
 - einen langgestreckten Kanal (16), der mit dem Handteil (20) verbunden ist; 45
 - einen Amboss (18), der schwenkbar an dem langgestreckten Kanal (16) angebracht ist; 50
 - eine Klammereinrichtung (37), die den langgestreckten Kanal (16) belegt und mehrere Klammerantriebe (220) und ein Keilbauteil (218) umfasst, das distal durch die Klammereinrichtung (37) bewegbar ist, um die Klammerantriebe (220) hin zu dem Amboss (18) ablaufen zu lassen; 55
 - eine Schusseinrichtung (14), die sich von einer proximalsten Position auf die Schussbewegung hin bewegt, um das Keilbauteil (218) distal von der proximalen Position anzutreiben; und
 - eine Verriegelungseinrichtung (270), die das

Abfeuern des Geräts in der Abwesenheit einer unerschöpften Klammereinrichtung (37) verhindert; **dadurch gekennzeichnet, dass** die Verriegelungseinrichtung (270) durch das Keilbauteil (218) dann deaktiviert ist, wenn das Keilbauteil (218) in der proximalen Position ist; das Keilbauteil (218) von der Schusseinrichtung (14) getrennt und so angeordnet ist, dass eine Rückführung der Schusseinrichtung (14) das Keilbauteil (218) nicht zurückführt; und die Verriegelungseinrichtung (270) betriebsgemäß zum Verhindern der distalen Bewegung der Schusseinrichtung (14) von ihrer proximalsten Position konfiguriert ist, wenn sich das Keilbauteil (218) nicht in der proximalen Position befindet.

2. Klammersetzgerät (10) nach Anspruch 1, bei dem die Klammereinrichtung (37) eine austauschbare Einrichtung umfasst.
3. Klammersetzgerät (10) nach Anspruch 1, bei dem die Klammereinrichtung (37) einen Schussantriebsschlitz (47) umfasst, durch den hindurch sich mindestens ein Abschnitt der Schusseinrichtung (14) distal quer bewegt, um das Keilbauteil (218) anzutreiben, wobei die Verriegelungseinrichtung (270) in den Schussantriebsschlitz (47) von dem langgestreckten Kanal (16) elastisch eindringt.
4. Klammersetzgerät (10) nach Anspruch 3, bei dem die Verriegelungseinrichtung (270) in dem Schussantriebsschlitz (47) eine Fläche aufweist, die sich von dem langgestreckten Kanal (16) proximal ramartig anhebt.
5. Klammersetzgerät (10) nach Anspruch 4, bei dem die Verriegelungseinrichtung (270) einen proximal ausgerichteten Federfinger (272) umfasst.
6. Klammersetzgerät (10) nach Anspruch 5, bei dem der langgestreckte Kanal (16) eine Aussparung unter dem Federfinger (272) umfasst, um einen Abschnitt der Schusseinrichtung (14) aufzunehmen.
7. Klammersetzgerät (10) nach Anspruch 4, bei dem die Verriegelungseinrichtung (270) eine federvorgespannte Stange umfasst.
8. Klammersetzgerät (10) nach Anspruch 4, bei dem die Verriegelungseinrichtung (270) einen sich ramartig anhebenden Haken (104) umfasst, der federförmig an dem langgestreckten Kanal (16) angebracht ist.
9. Klammersetzgerät (10) nach Anspruch 1, umfassend:

- einen Schaft (23), der an dem Handteil (20) angebracht und betriebsgemäß zum Übertragen der Schließbewegung und der Schussbewegung konfiguriert ist; und
 einer Schussstange (14), die mit dem Schaft (23) verbunden ist und auf die Schussbewegung anspricht, um sich zwischen dem langgestreckten Kanal (16) und dem Amboss (18) distal quer zu bewegen;
 wobei das Handteil (20) betriebsgemäß zum Durchführen einer Schließbewegung konfiguriert ist;
 der langgestreckte Kanal (16) an dem Schaft (23) angebracht ist;
 der Amboss auf die Schließbewegung anspricht;
 das Keilbauteil (218) durch die Schussstange (14) während des Abfeuerns verlagert wird; und die Verriegelungseinrichtung (270) durch ein nicht verlagertes Keilbauteil (218) deaktiviert wird.
10. Klammersetzgerät (10) nach Anspruch 9, bei dem die Klammereinrichtung (37) eine austauschbare Einrichtung umfasst.

Revendications

1. Instrument d'agrafage linéaire chirurgical (10) comprenant :
- ♦ une partie formant une poignée (20) configurée fonctionnellement de façon à produire un mouvement de déclenchement ;
 - ♦ un canal allongé (16) couplé à la partie formant une poignée (20) ;
 - ♦ une enclume (18) fixée de façon à pivoter au canal allongé (16) ;
 - ♦ un dispositif à agrafes (37) mis en prise par le canal allongé (16) et comprenant une pluralité d'entraînements d'agrafes (220) et un élément à cale (218) pouvant se déplacer distalement dans le dispositif à agrafes (37) pour entraîner les entraînements d'agrafes (220) vers l'enclume (18) ;
 - ♦ un dispositif de déclenchement (14) se déplaçant distalement d'une position proximale en réponse au mouvement de déclenchement pour entraîner l'élément à cale (218) sur le plan distal à partir d'une position proximale ; et
 - ♦ un dispositif de blocage (270) empêchant le déclenchement de l'instrument en l'absence d'un dispositif à agrafes non utilisé (37) ;

caractérisé en ce que

- ♦ le dispositif de blocage (270) est désactivé

par l'élément à cale (218) lorsque l'élément à cale (218) est en position proximale ;

- ♦ l'élément à cale (218) étant séparé du dispositif de déclenchement (14) et disposé de telle sorte que la rétraction du dispositif de déclenchement (14) ne rétracte pas l'élément à cale (218) ; et
 - ♦ le dispositif de blocage (270) étant configuré fonctionnellement de façon à empêcher un mouvement distal du dispositif de déclenchement (14) de sa position proximale lorsque l'élément à cale (218) n'est pas en position proximale.
2. Instrument chirurgical (10) selon la revendication 1, dans lequel le dispositif à agrafes (37) comprend un dispositif remplaçable.
3. Instrument chirurgical (10) selon la revendication 1, dans lequel le dispositif à agrafes (37) comprend une fente d'entraînement de déclenchement (47) par laquelle au moins une partie du dispositif de déclenchement (14) traverse distalement pour entraîner l'élément à cale (218), le dispositif de blocage (270) entrant de façon élastique dans la fente d'entraînement de déclenchement (47) depuis le canal allongé (16).

4. Instrument chirurgical (10) selon la revendication 3, dans lequel le dispositif de blocage (270) présente une surface dans la fente d'entraînement de déclenchement (47) avançant depuis le canal allongé (16) sur le plan proximal.
5. Instrument chirurgical (10) selon la revendication 4, dans lequel le dispositif de blocage (270) comprend un doigt à ressort dirigé de manière proximale (272).
6. Instrument chirurgical (10) selon la revendication 5, dans lequel le canal allongé (16) comprend une cavité sous le doigt à ressort (272) pour recevoir une partie du dispositif de déclenchement (14).
7. Instrument chirurgical (10) selon la revendication 4, dans lequel le dispositif de blocage (270) comprend un piston dévié par ressort.
8. Instrument chirurgical (10) selon la revendication 4, dans lequel le dispositif de blocage (270) comprend un crochet incliné (104) fixé par ressort au canal allongé (16).
9. Instrument chirurgical selon la revendication 1, comprenant en outre :

- ♦ une tige (23) fixée à la partie à poignée (20) et configurée fonctionnellement pour transférer le mouvement de fermeture et le mouvement de déclenchement ; et

♦ une barre de déclenchement (14) couplée à la tige (23) et répondant au mouvement de déclenchement de façon à traverser distalement entre le canal allongé (16) et l'enclume (18) ;

5

dans lequel la partie formant une poignée (20) est configurée fonctionnellement de façon à produire un mouvement de fermeture ;

le canal allongé (16) est fixé à la tige (23) ;

l'enclume (18) répond au mouvement de fermeture ; 10

l'élément à cale (218) est déplacé par la barre de déclenchement (14) pendant le déclenchement ;

et le dispositif de blocage (270) est désactivé par un élément à cale non déplacé (218).

15

10. Instrument chirurgical (10) selon la revendication 9, dans lequel le dispositif à agrafes (37) comprend un dispositif remplaçable.

20

25

30

35

40

45

50

55

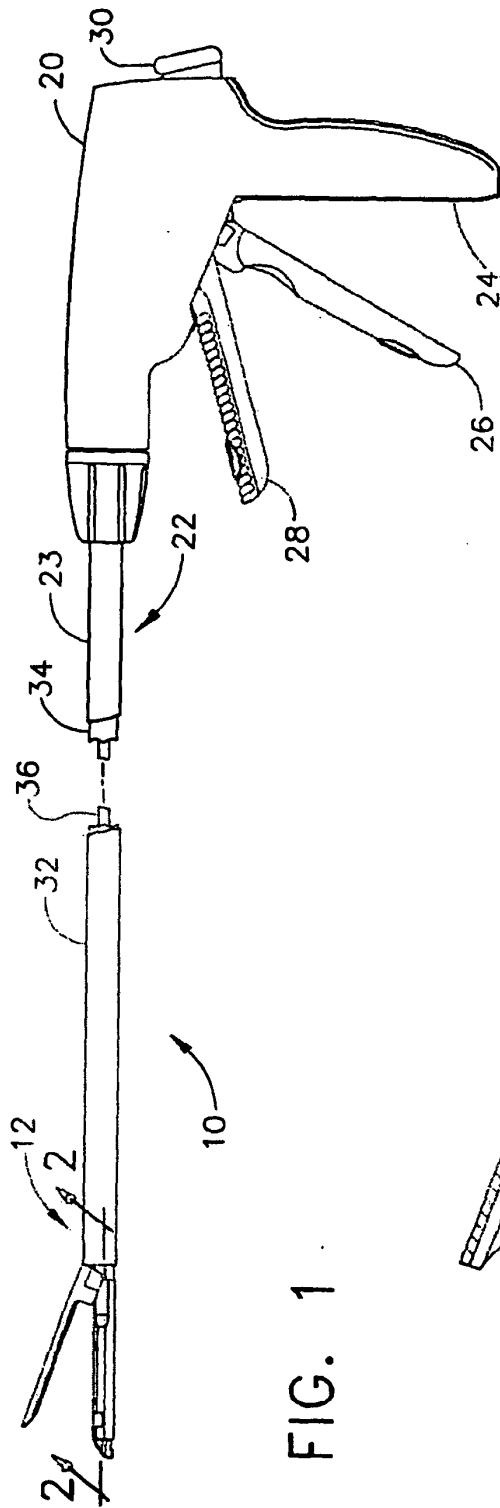


Fig. 1

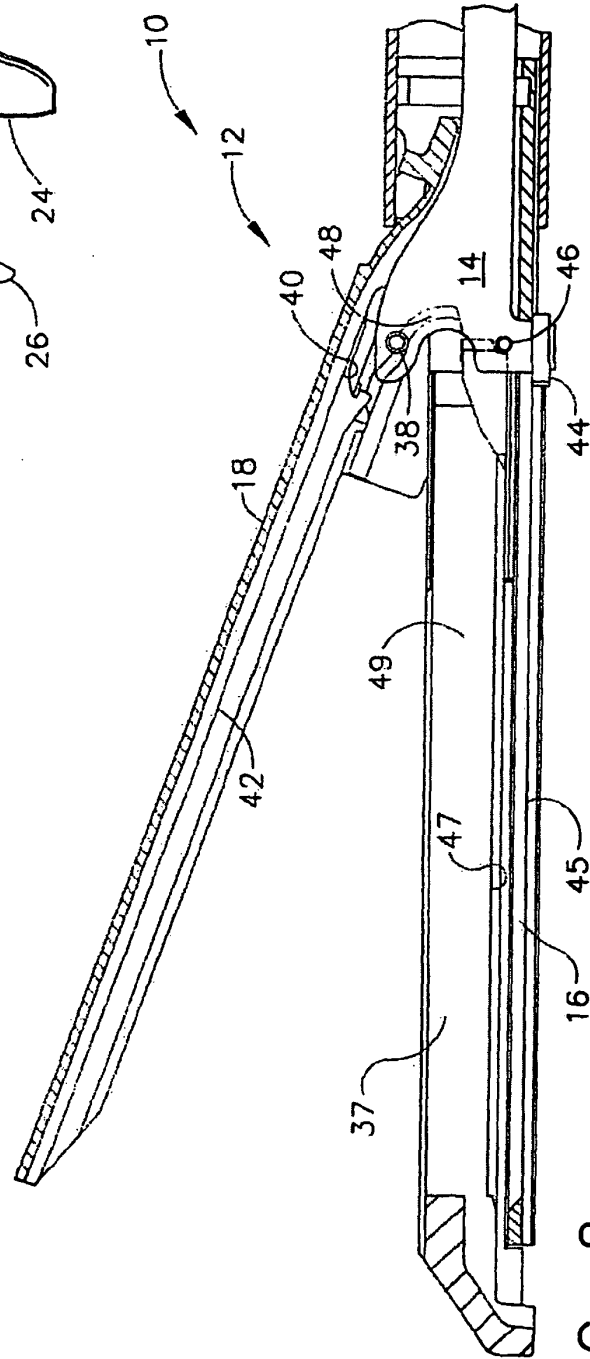


FIG. 2

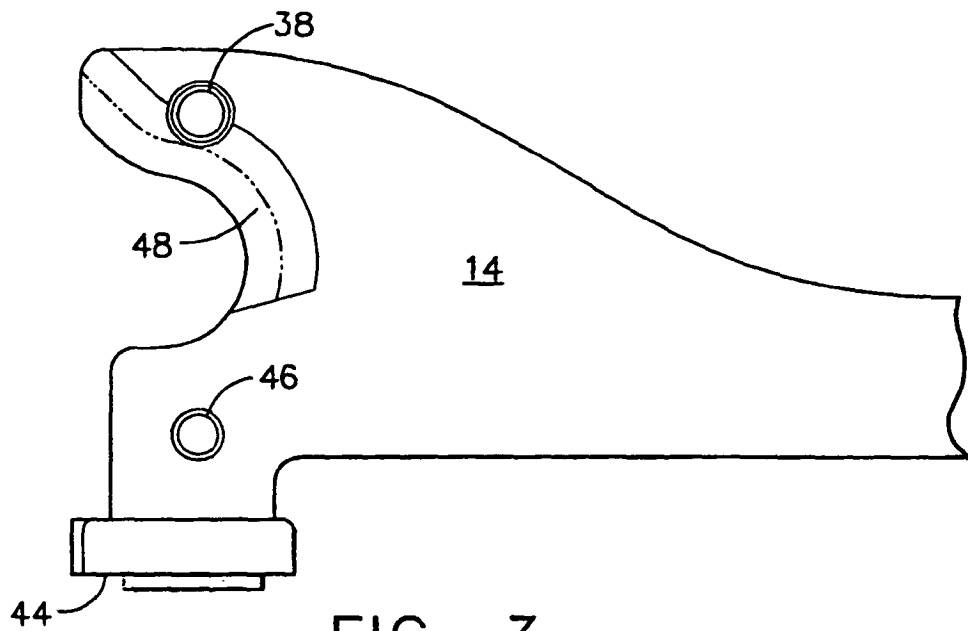


FIG. 3

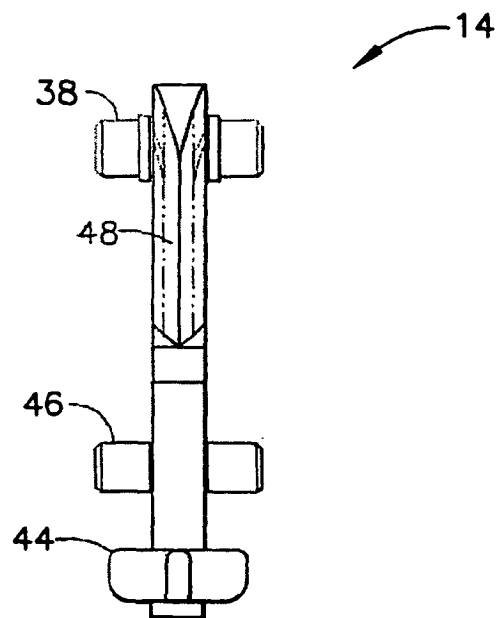


FIG. 4

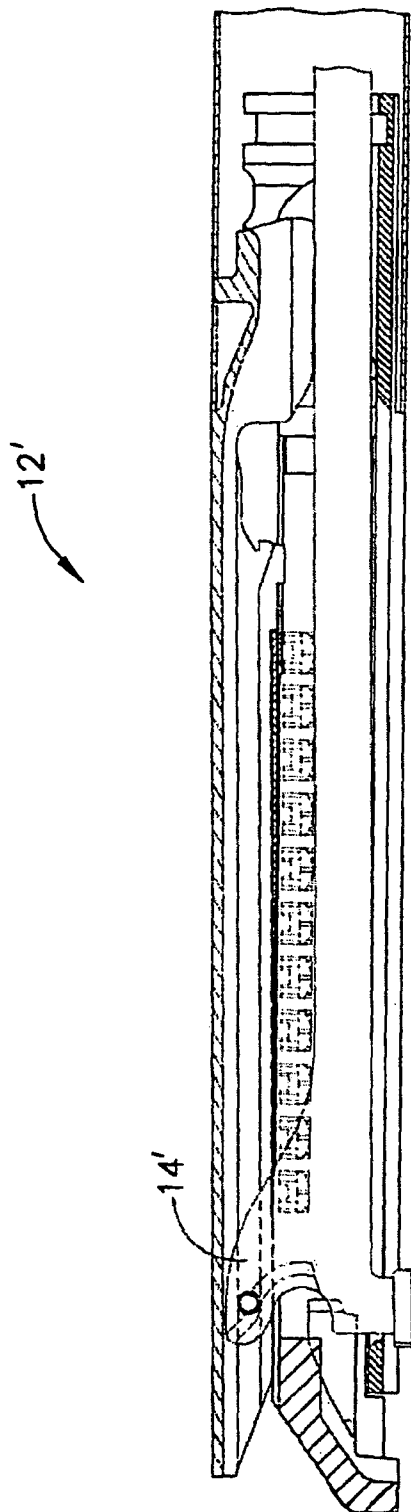


FIG. 5

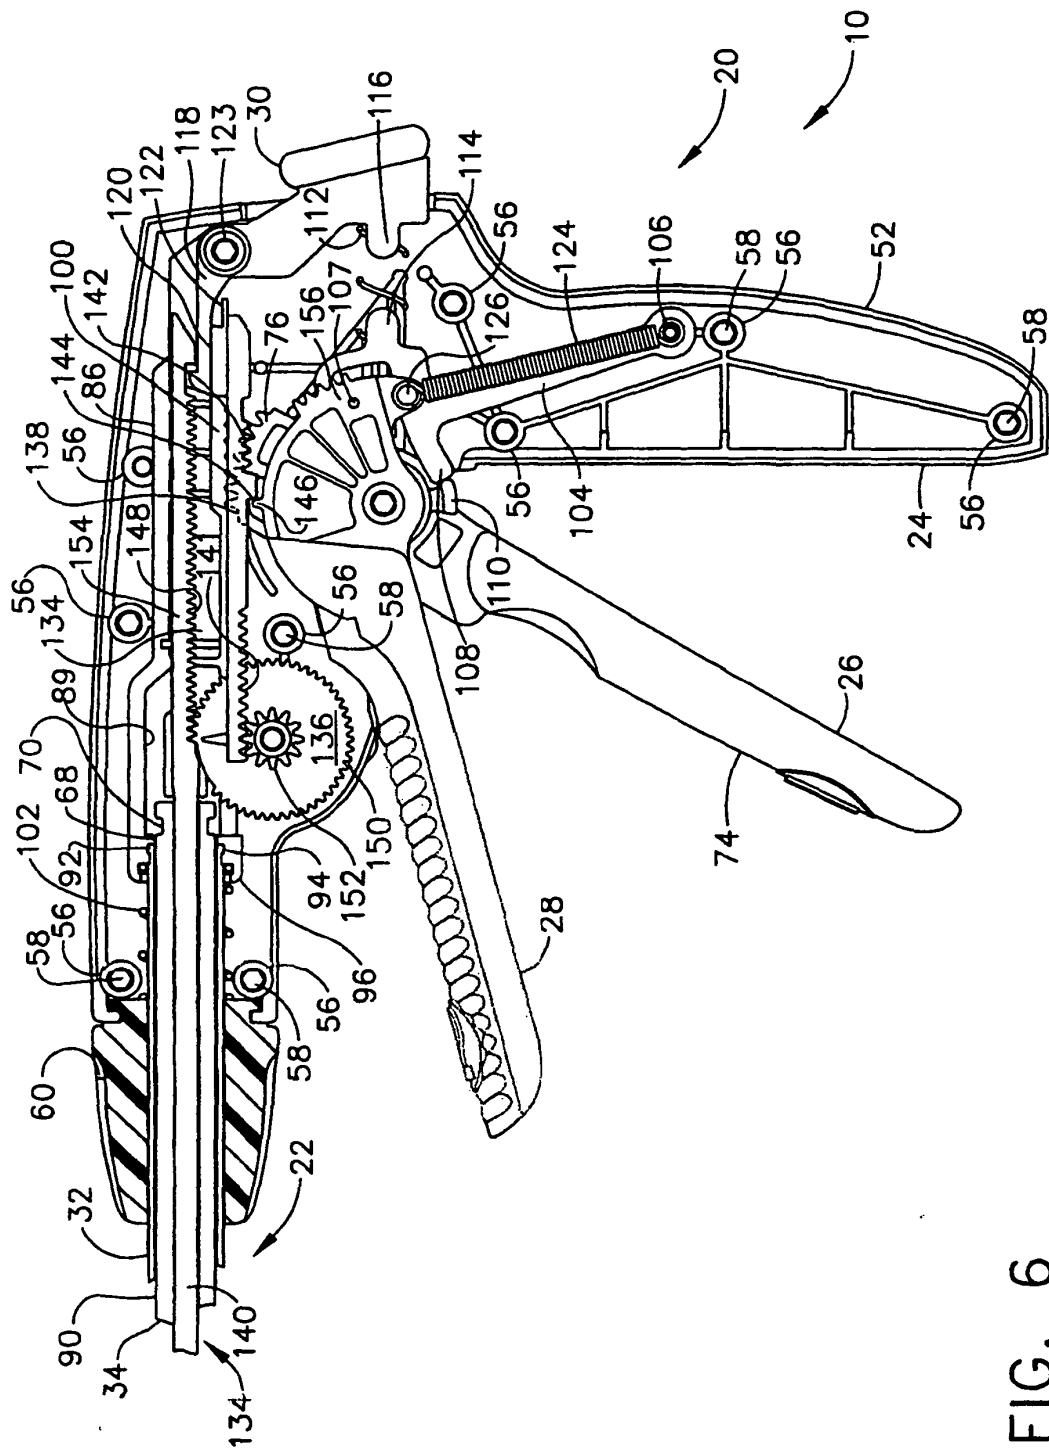


FIG. 6

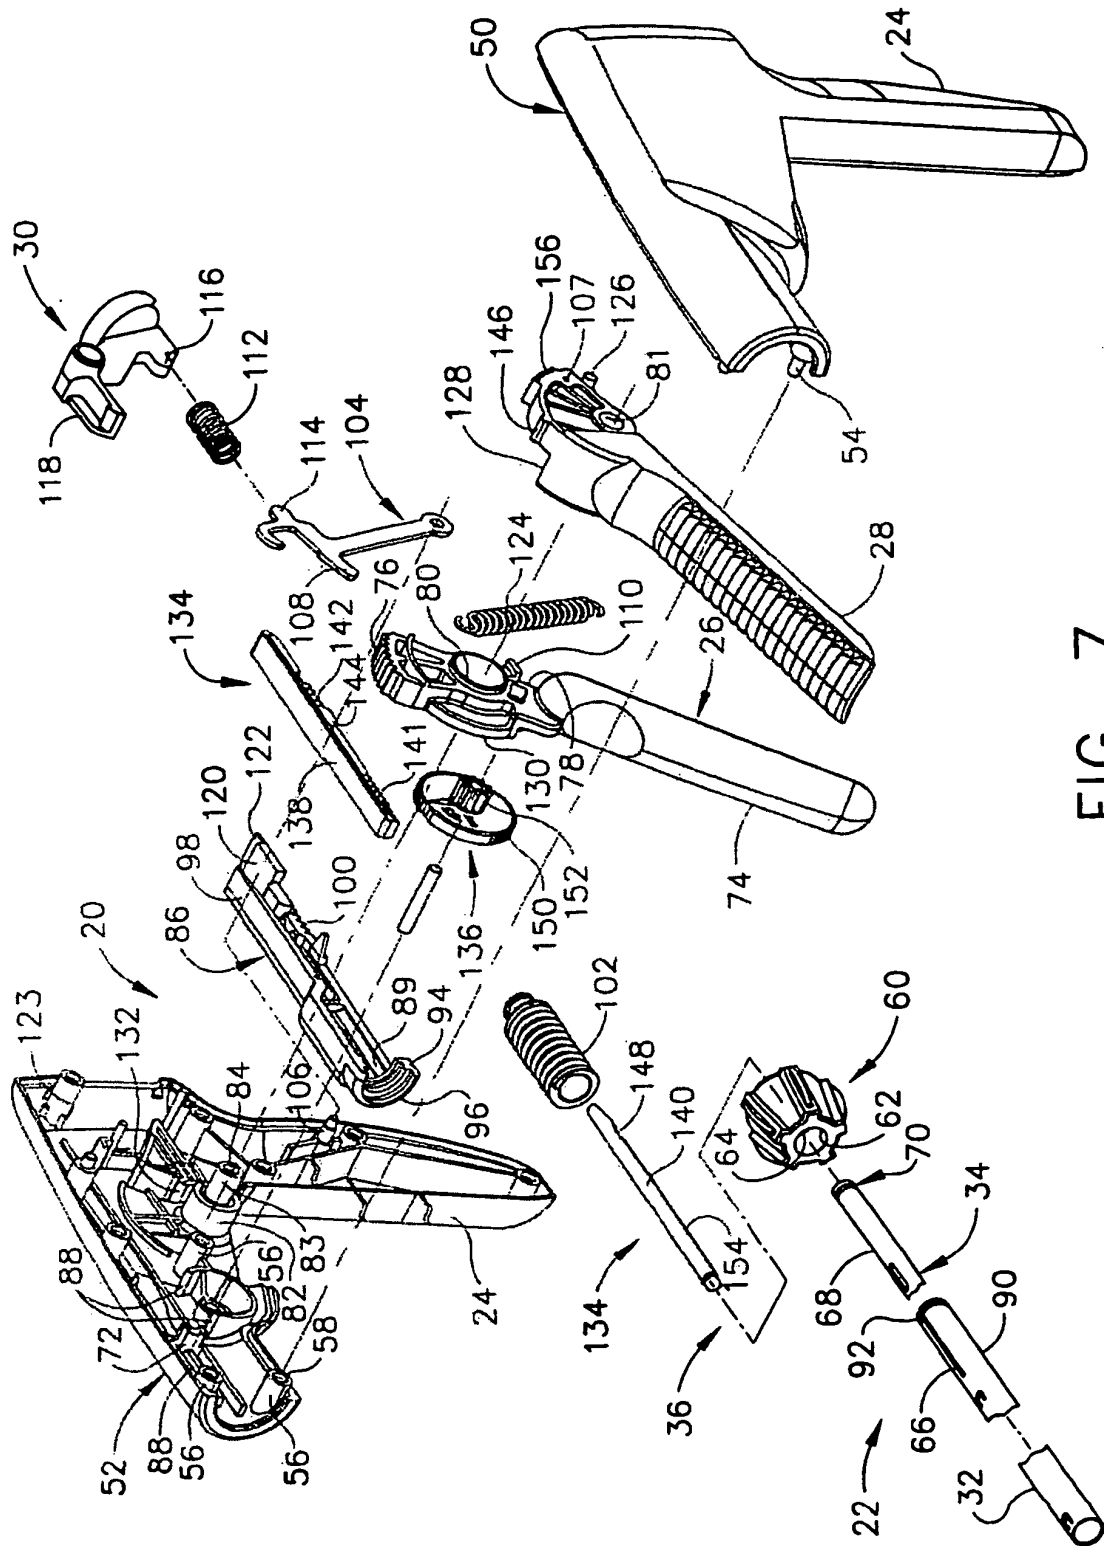


FIG. 7

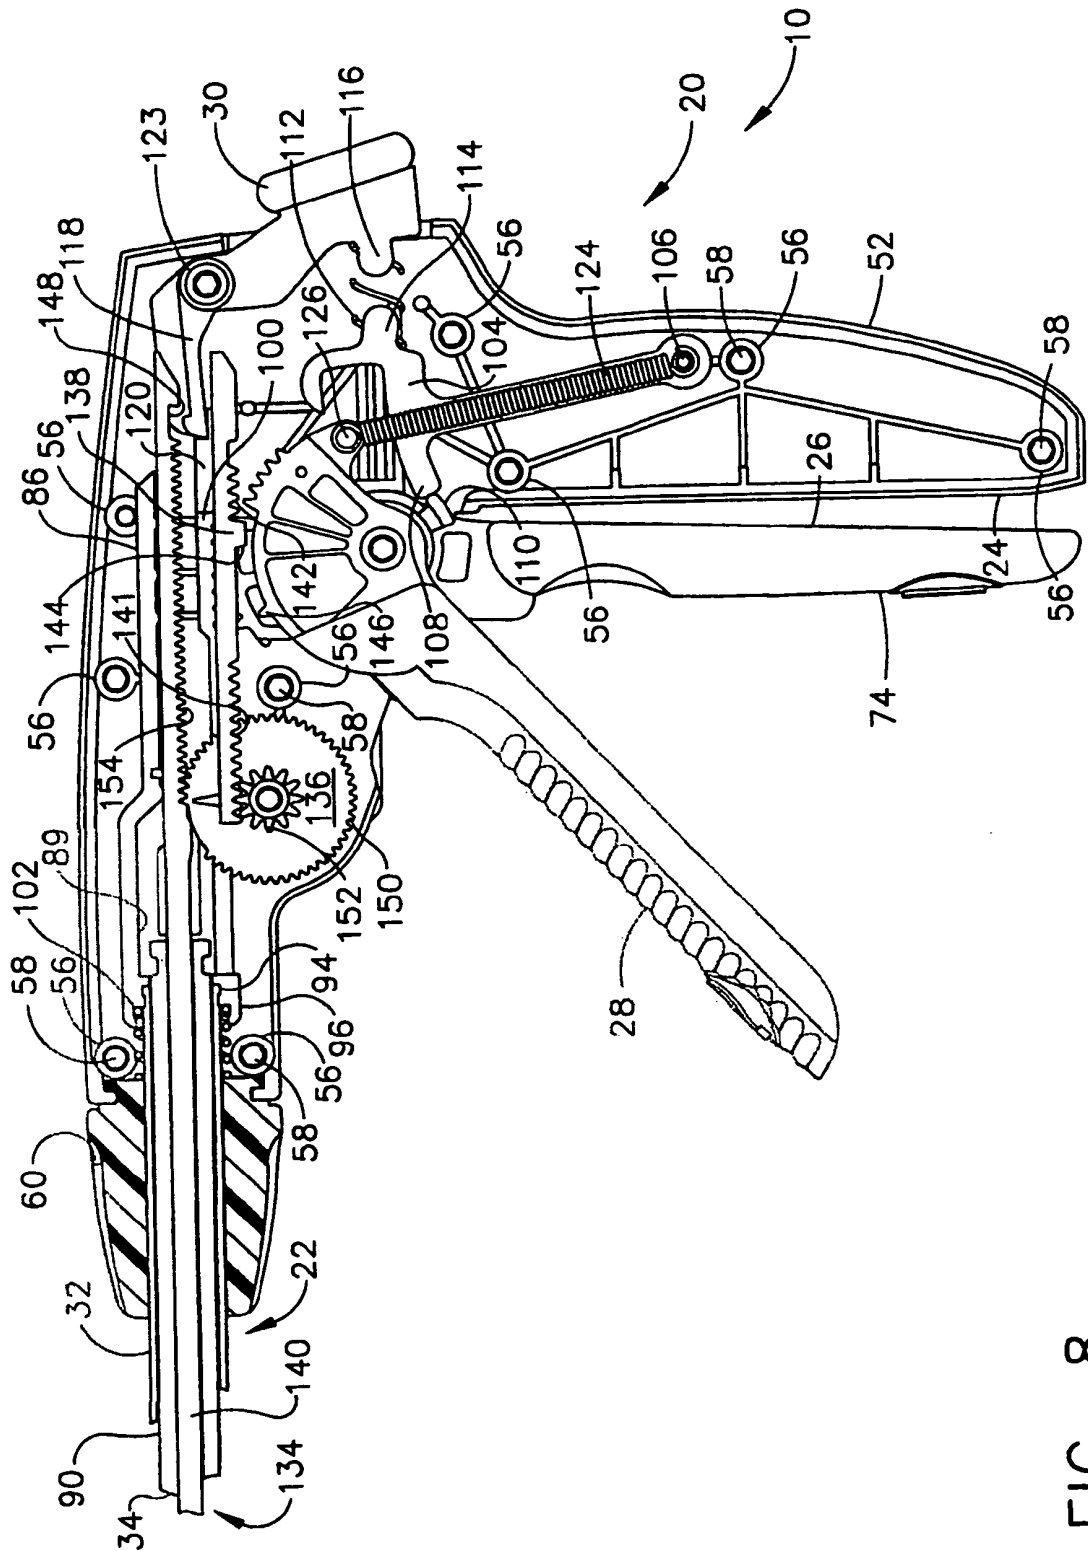


Fig. 8

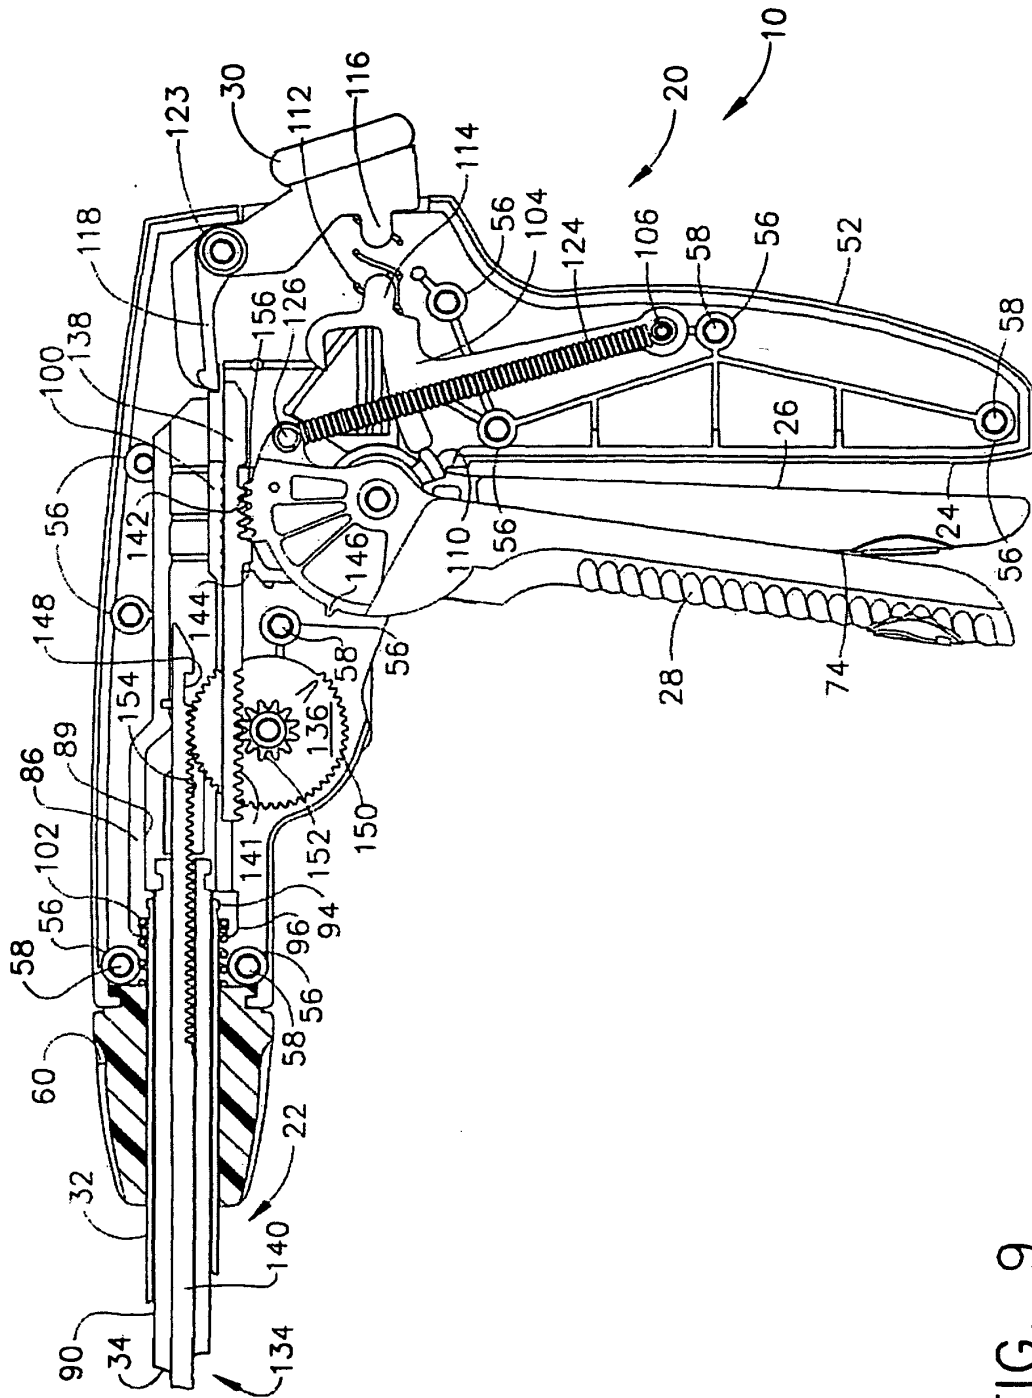


FIG. 9

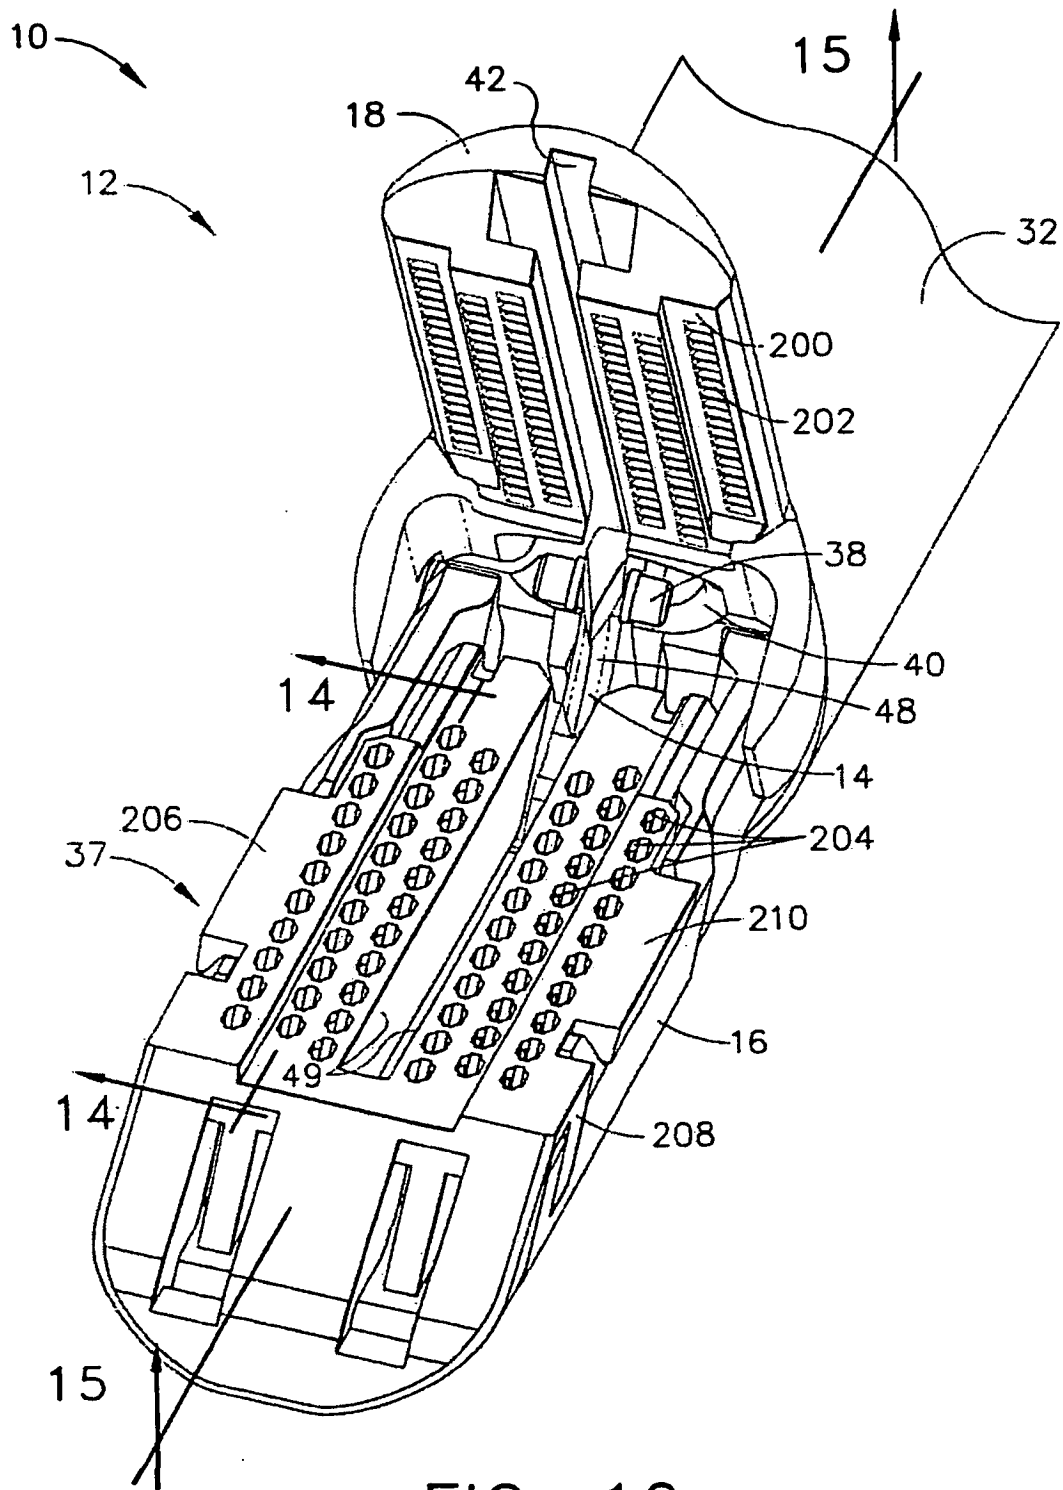


FIG. 10

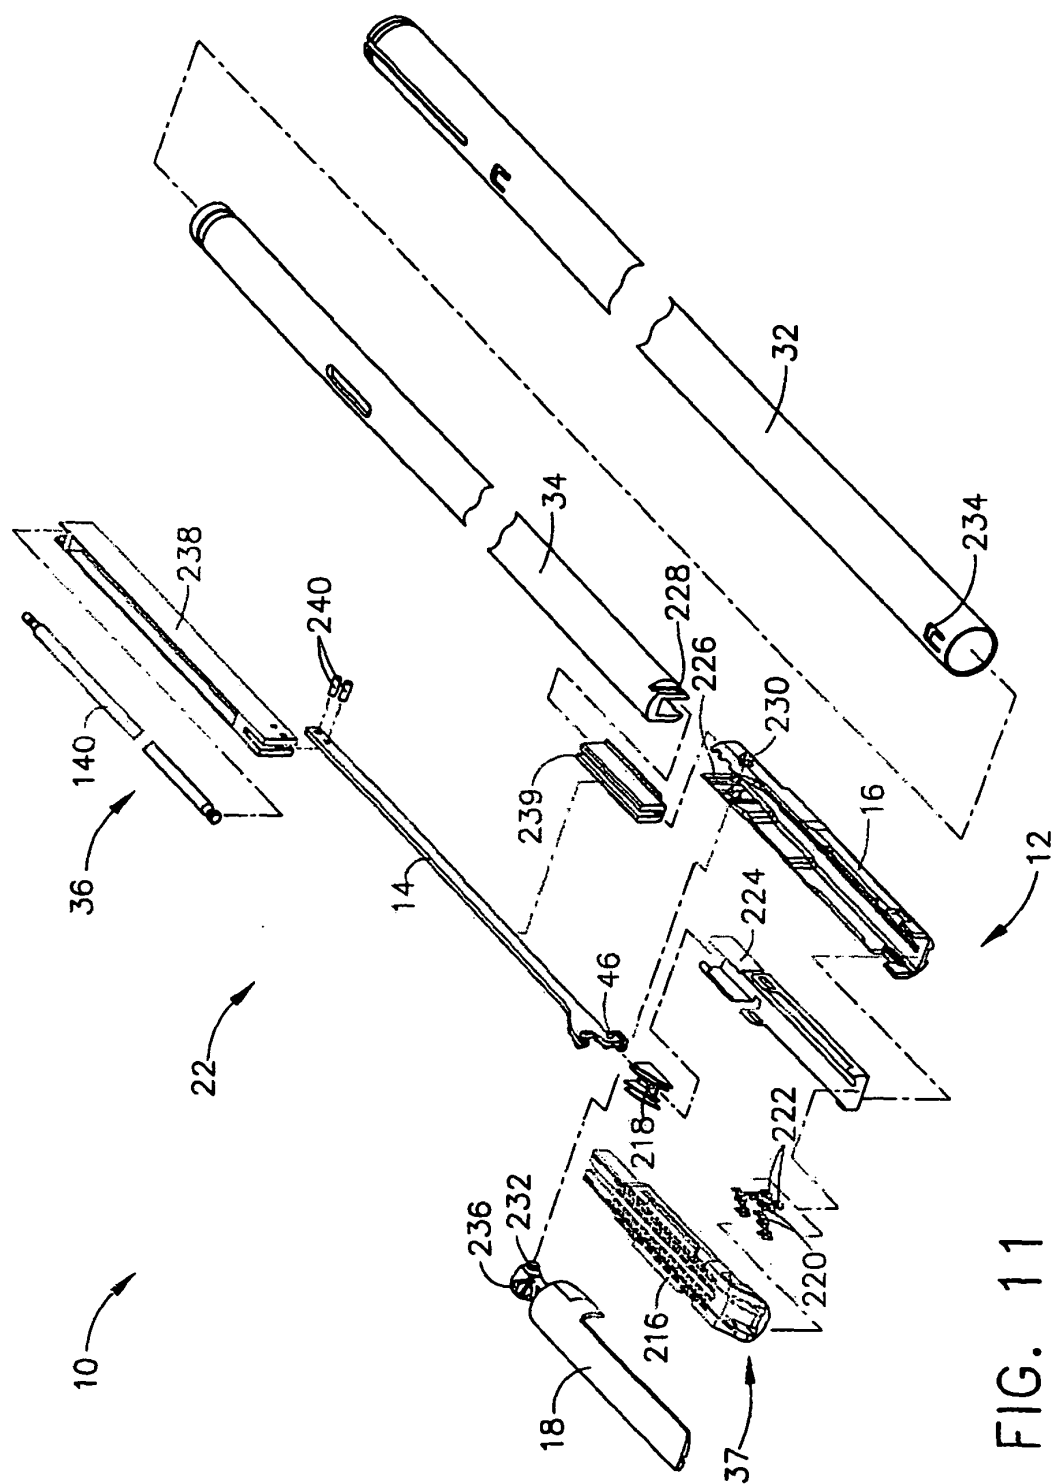


FIG. 11

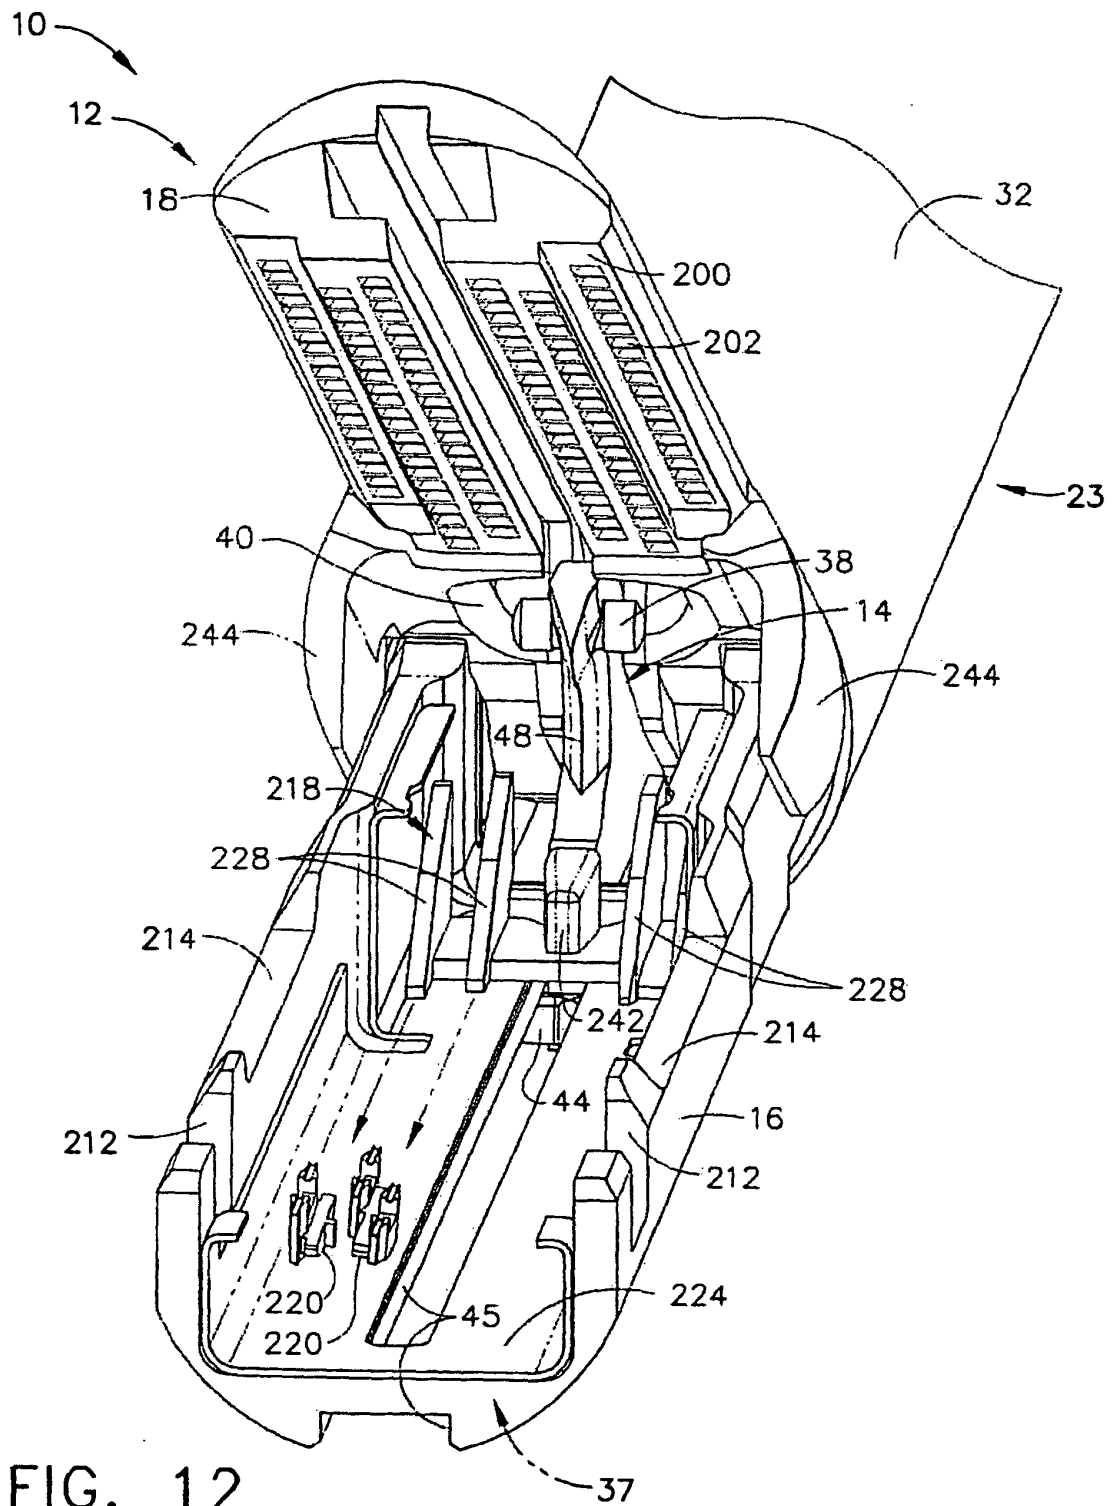


FIG. 12

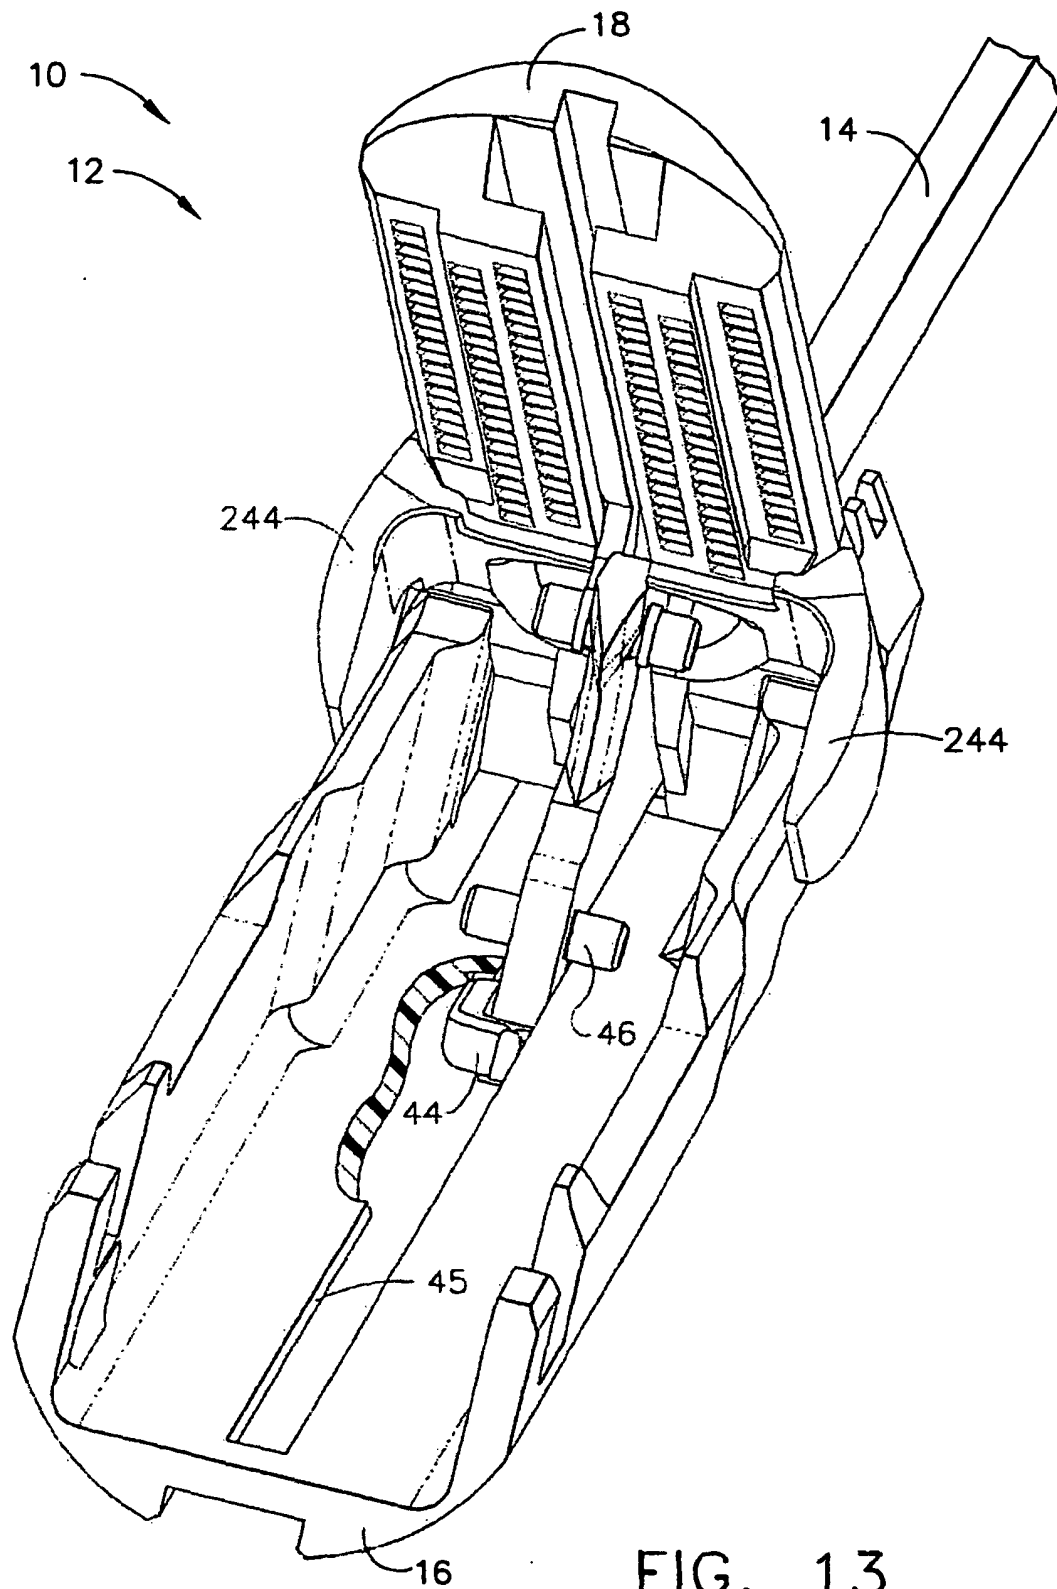


FIG. 13

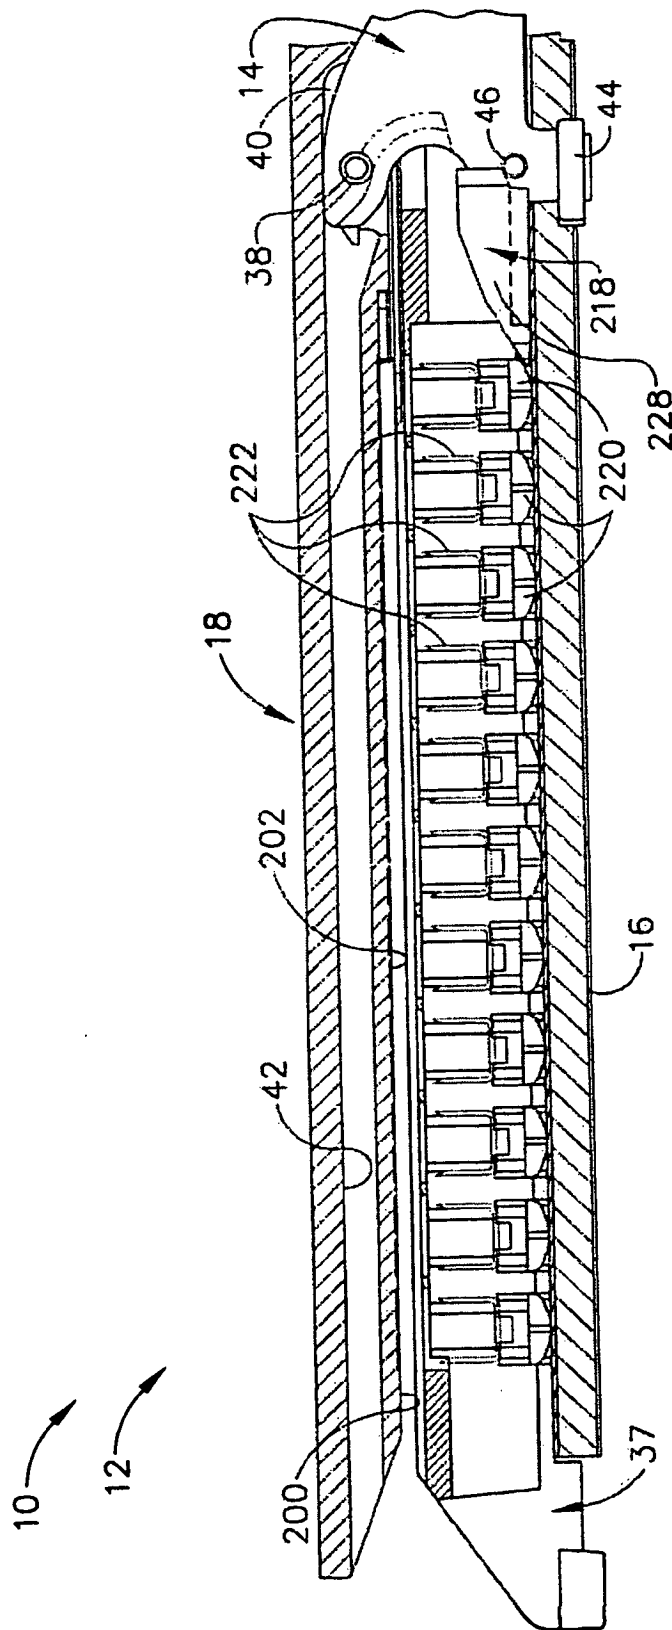
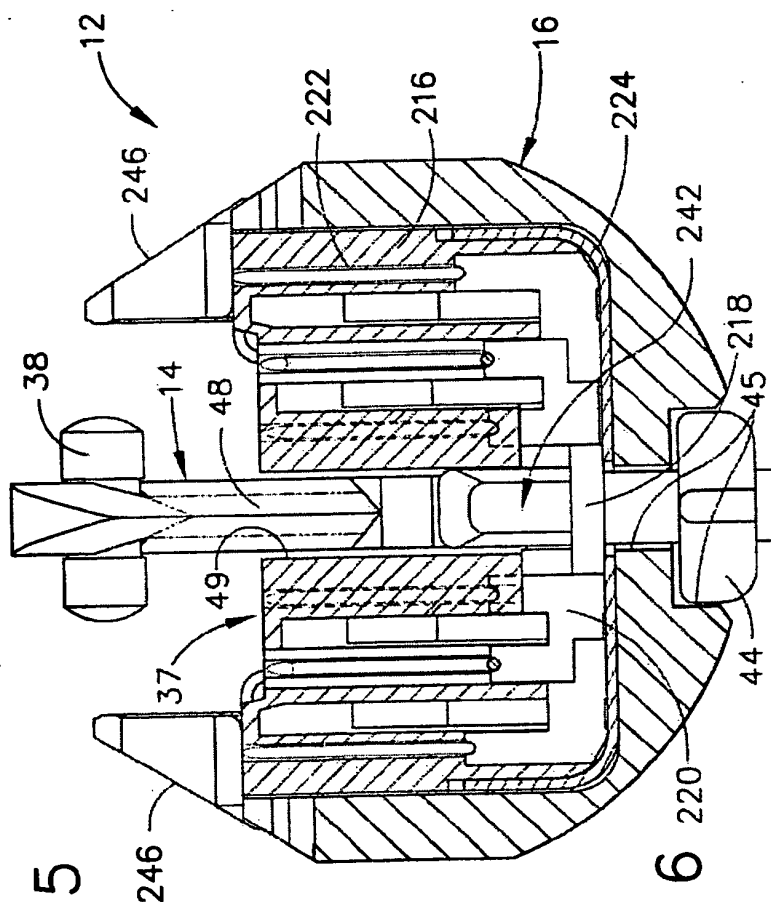
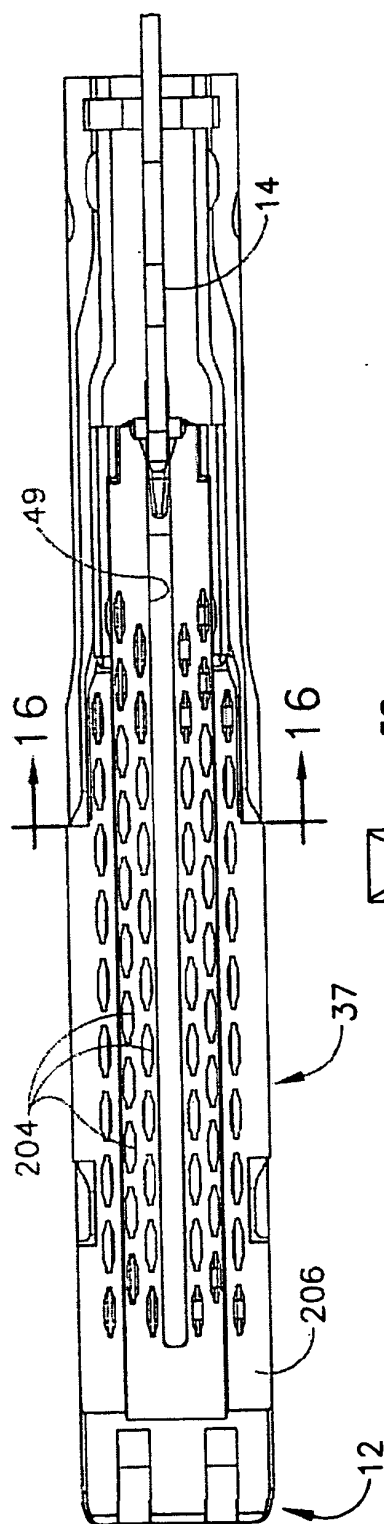


FIG. 14



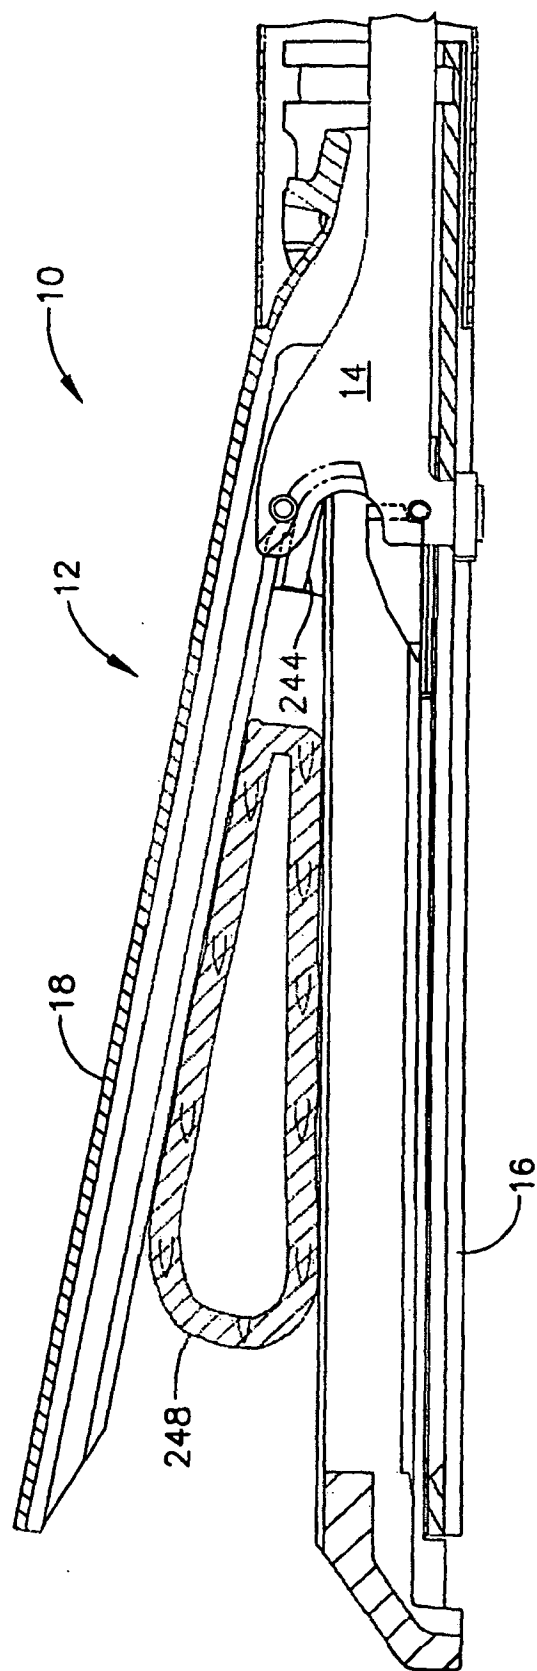
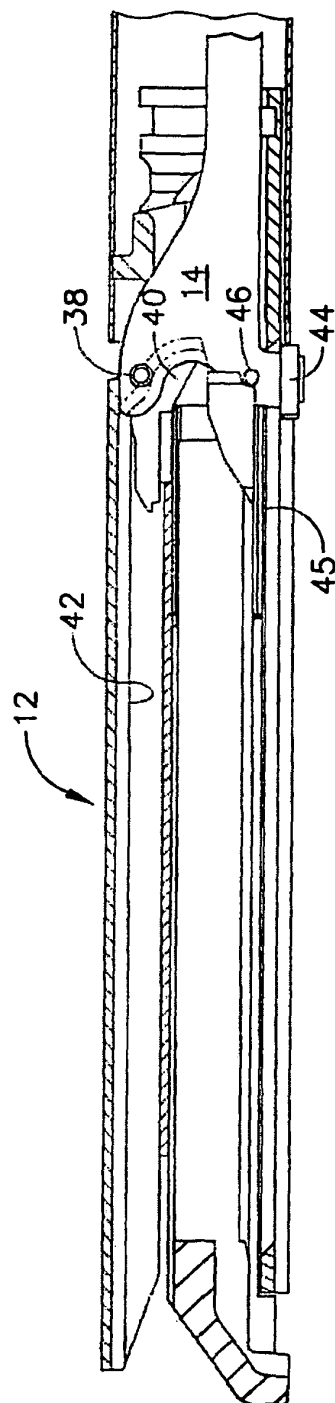
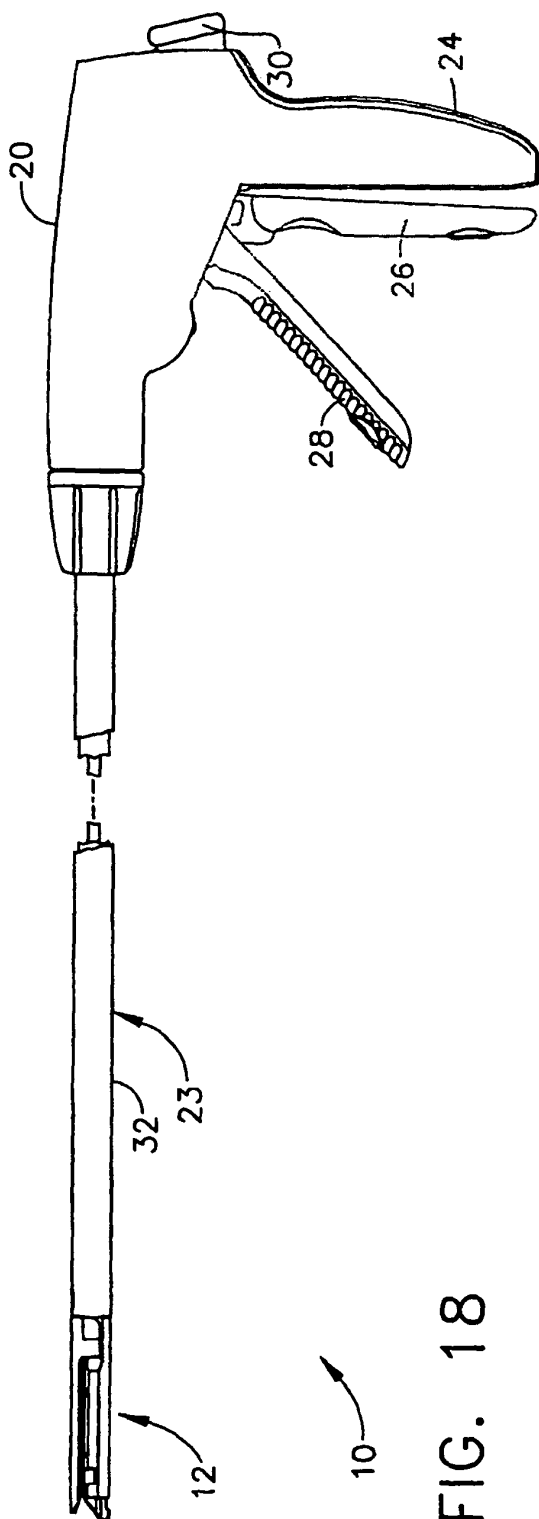


FIG. 17



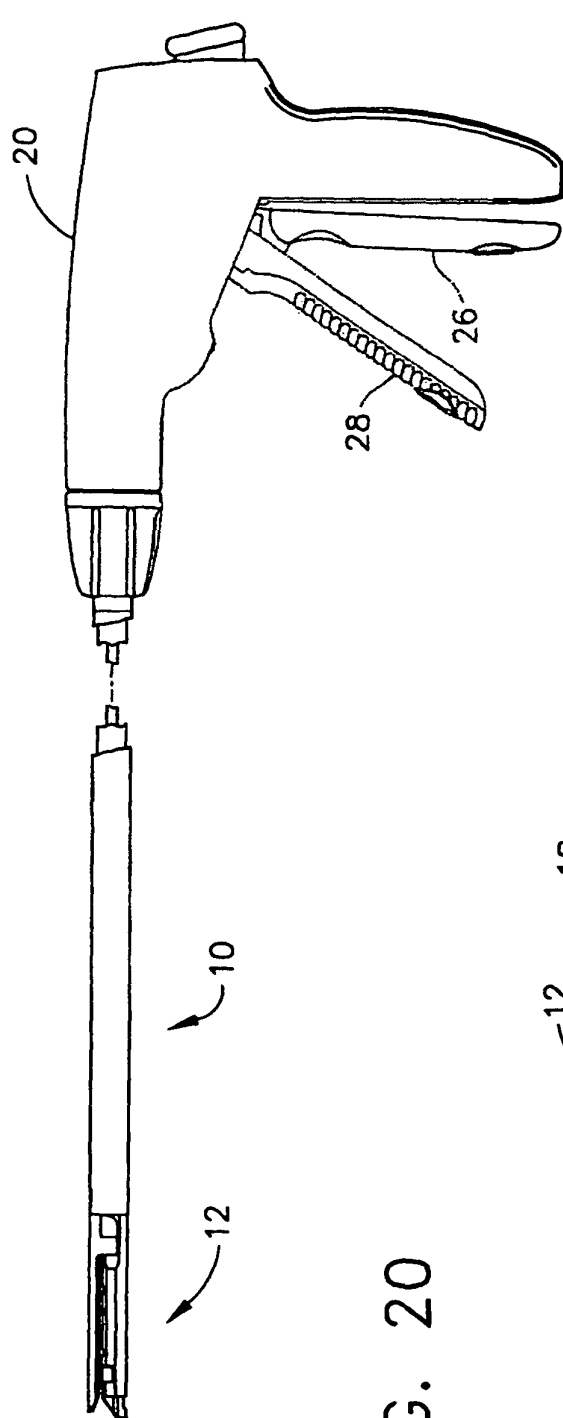


FIG. 20

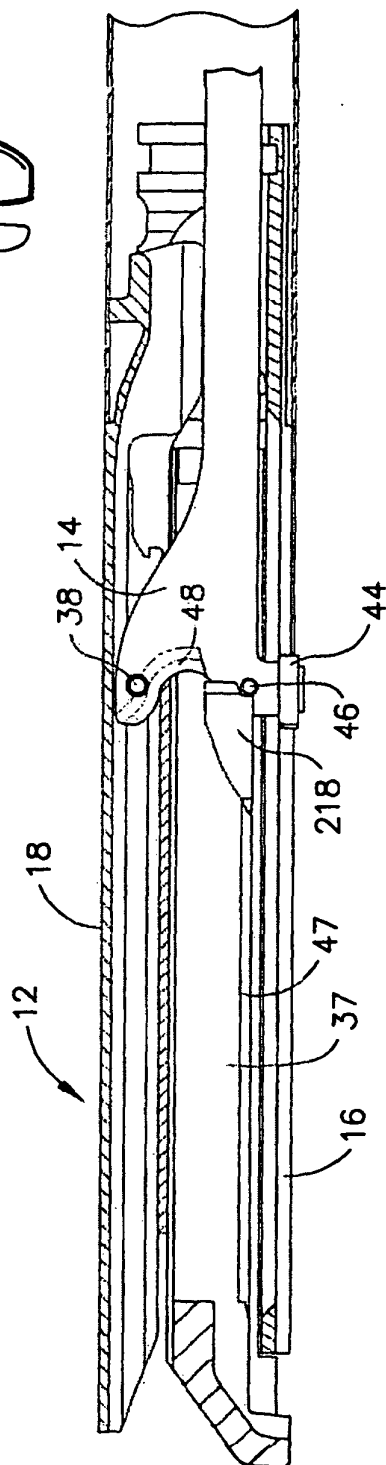


FIG. 21

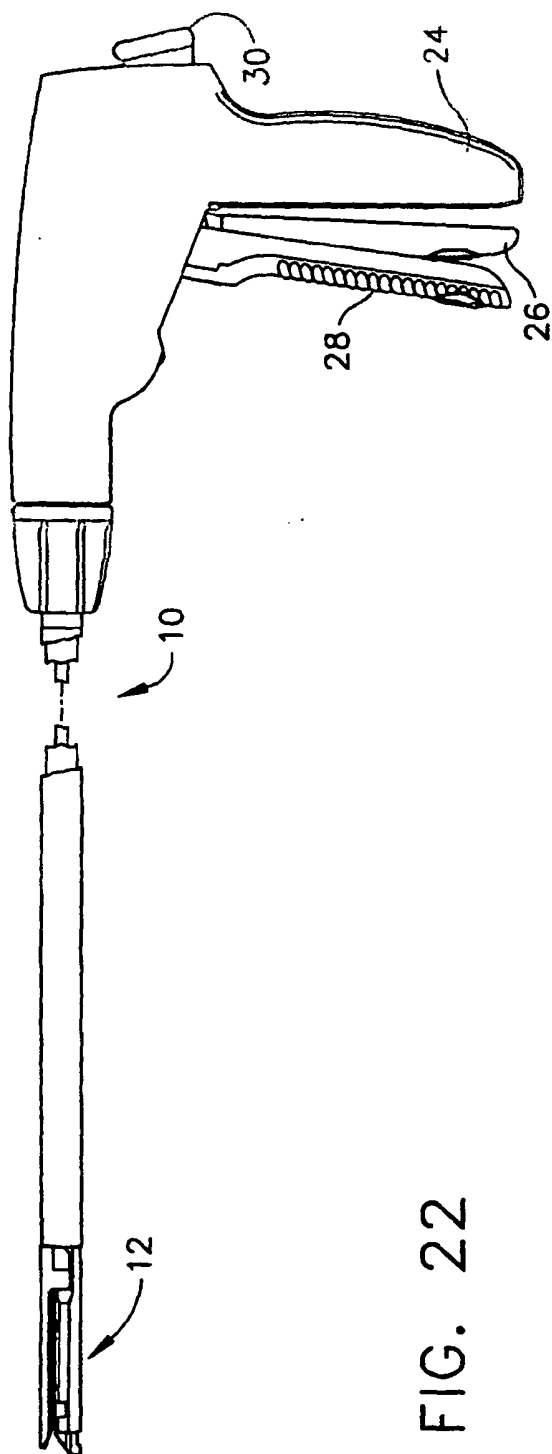


FIG. 22

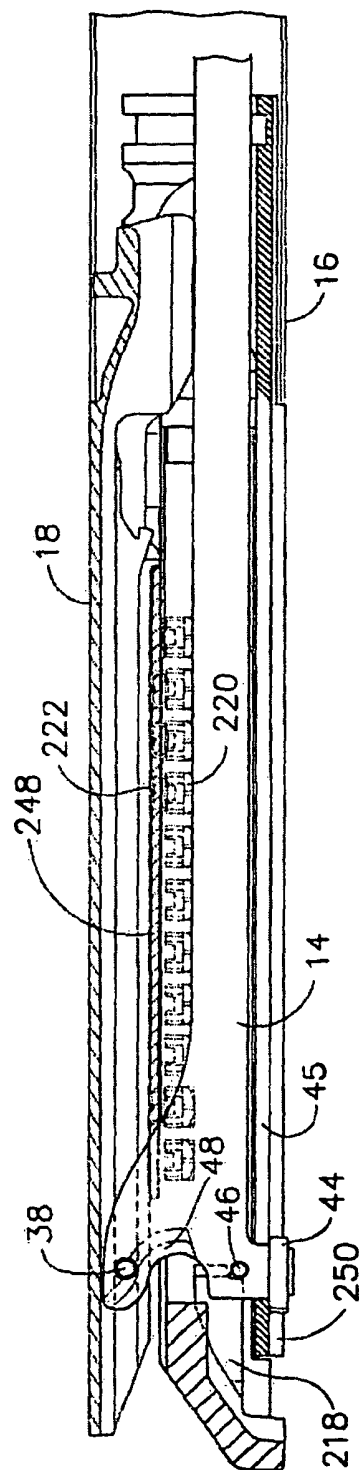


FIG. 23

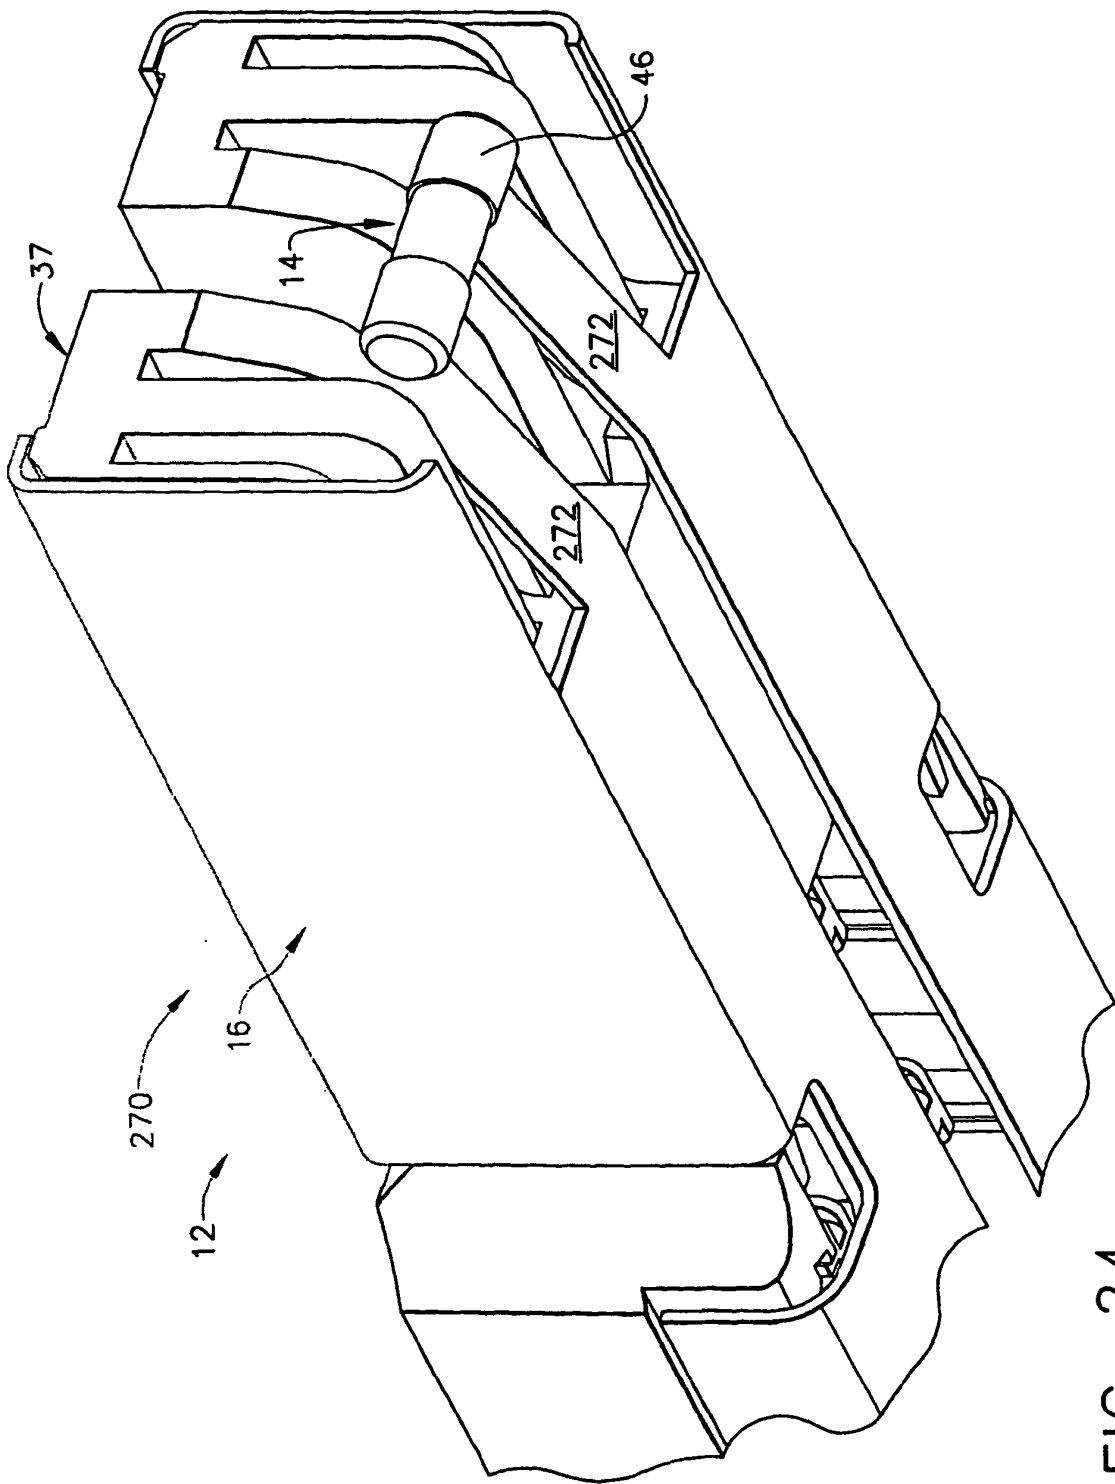
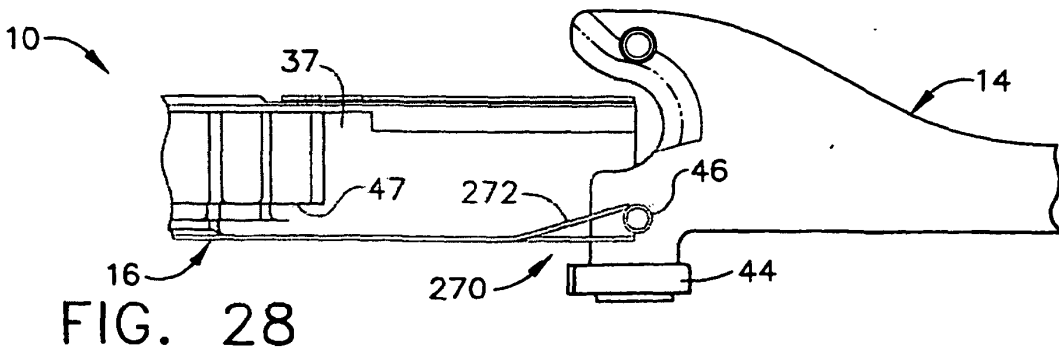
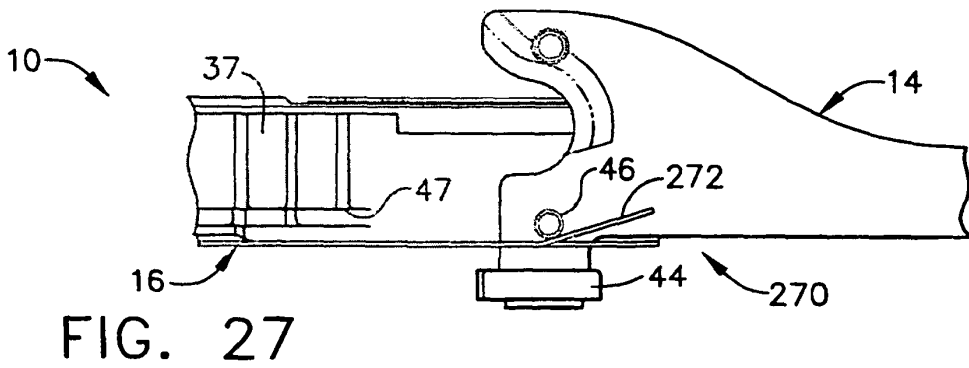
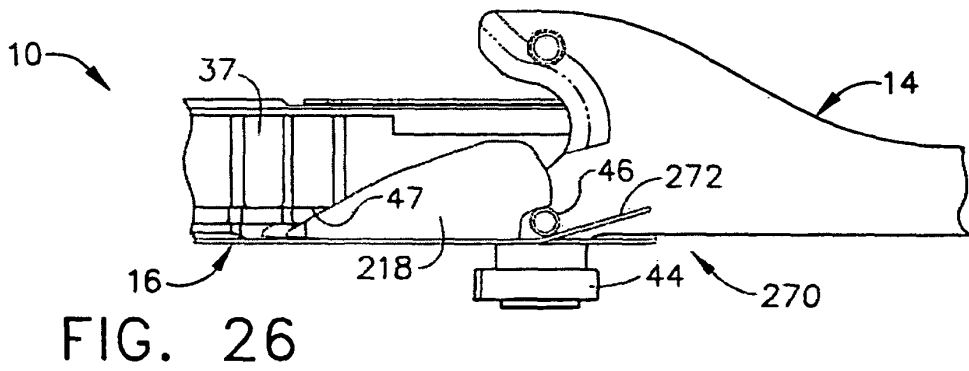
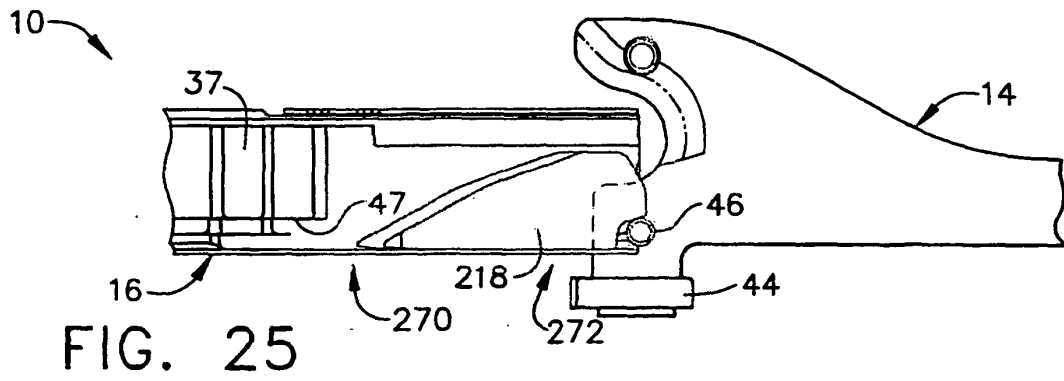


FIG. 24



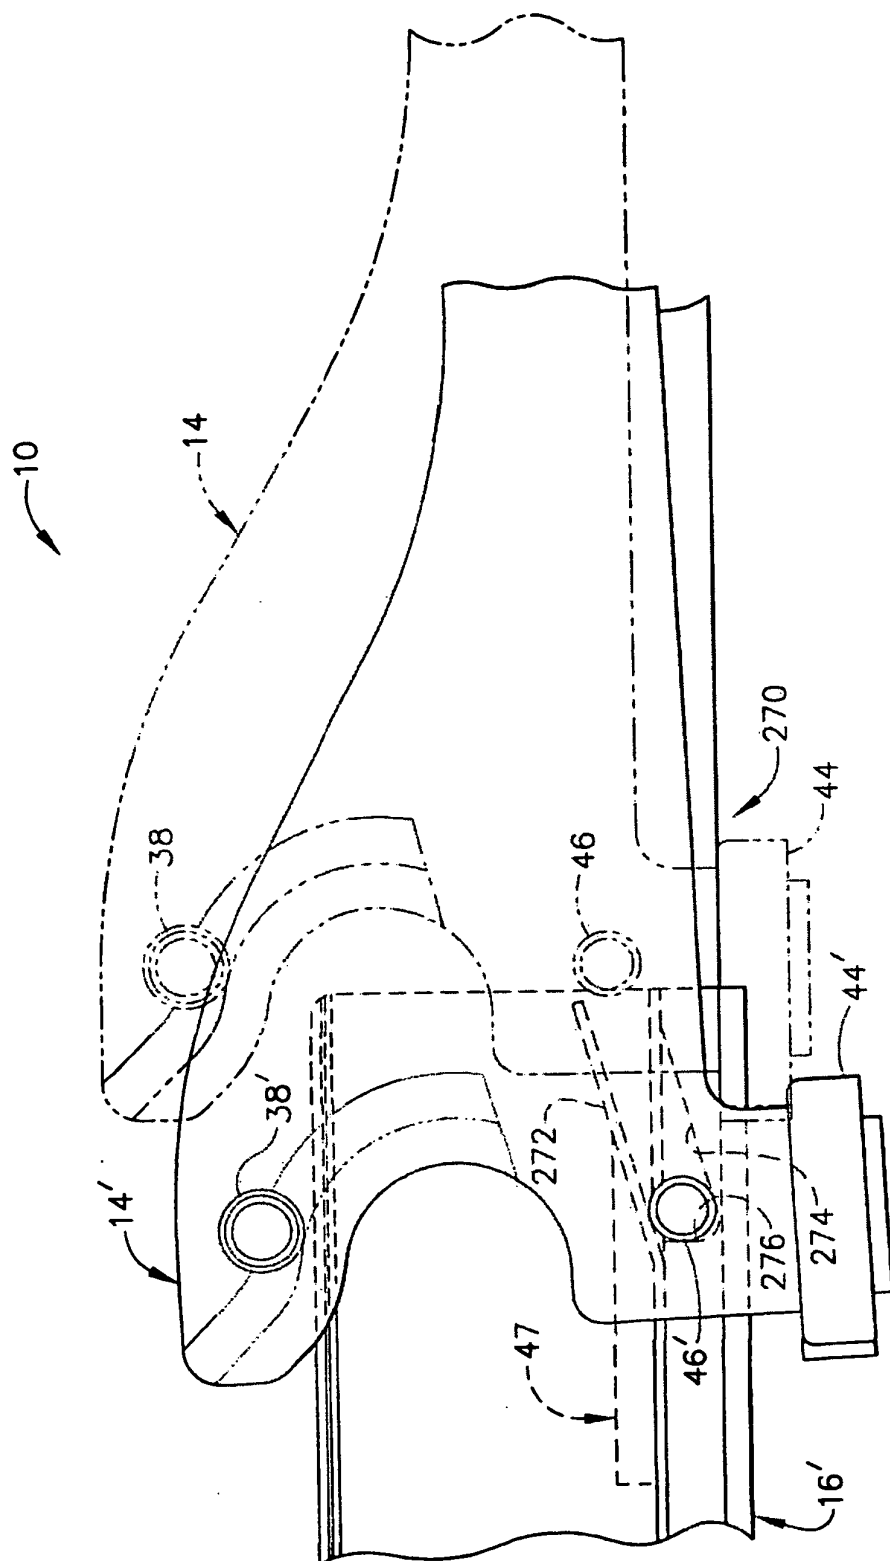


FIG. 29

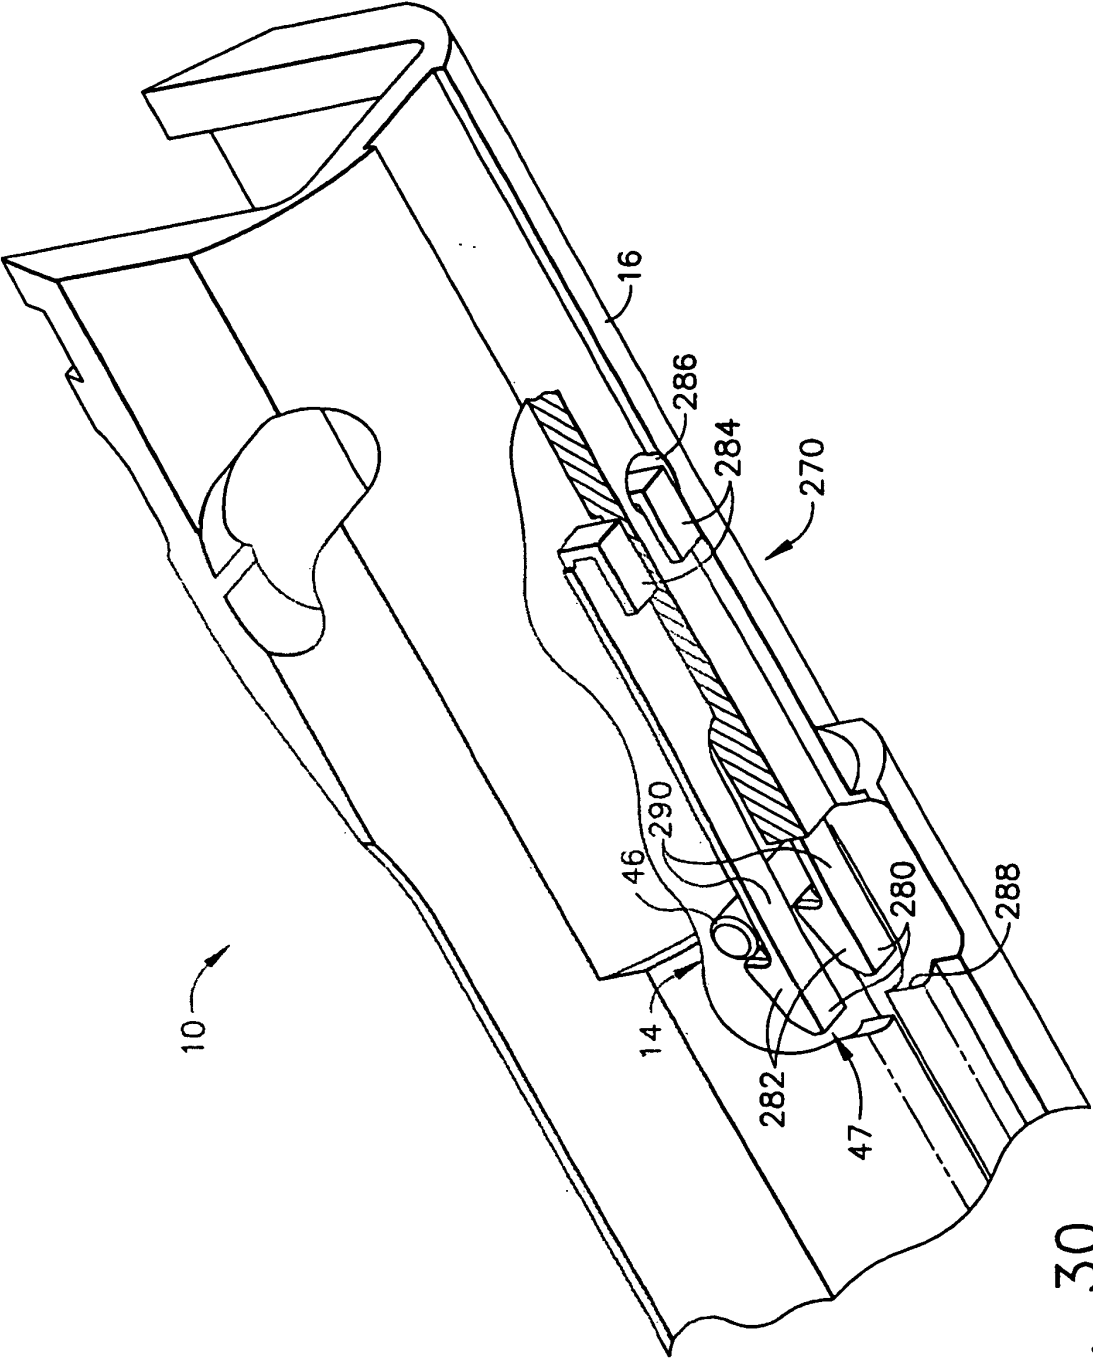


FIG. 30

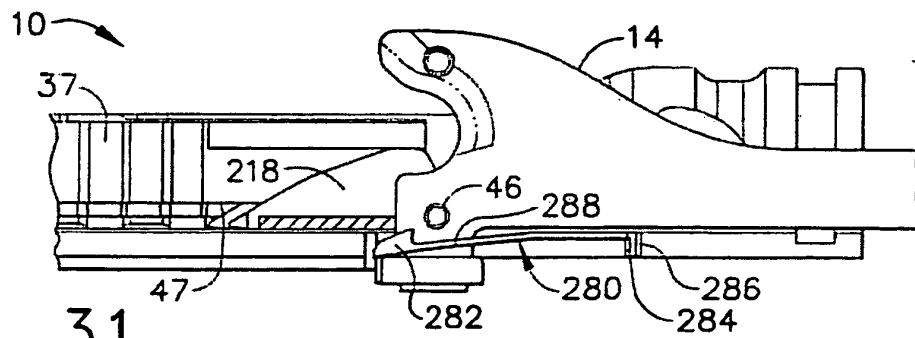


FIG. 31

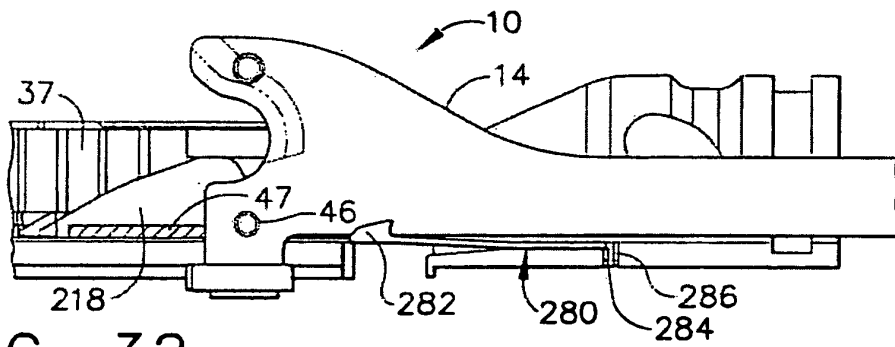


FIG. 32

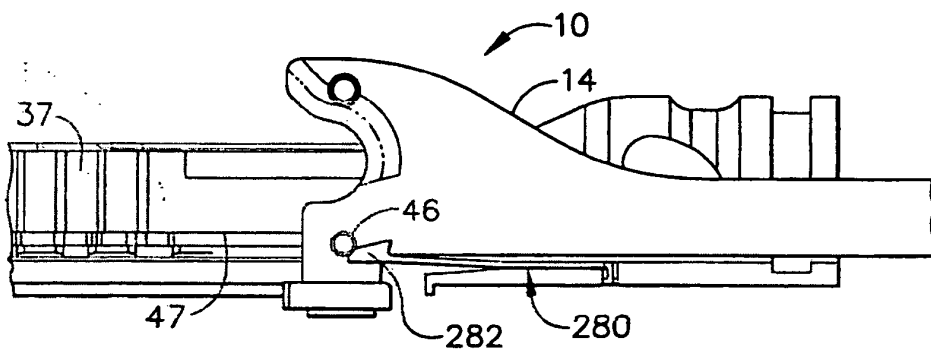


FIG. 33

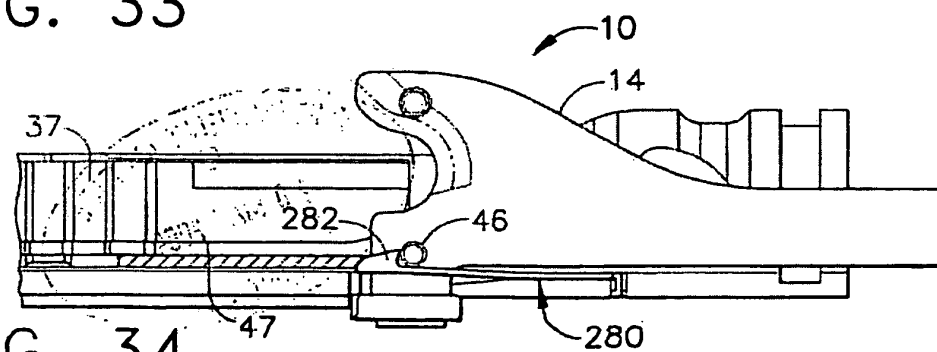


FIG. 34

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 5465895 A [0003]
- US 6202914 B [0003]

专利名称(译)	具有单个锁定机构的外科缝合器械		
公开(公告)号	EP1479348B1	公开(公告)日	2008-07-09
申请号	EP2004252979	申请日	2004-05-20
[标]申请(专利权)人(译)	伊西康内外科公司		
申请(专利权)人(译)	爱惜康内镜外科		
当前申请(专利权)人(译)	爱惜康内镜手术，INC.		
[标]发明人	SHELTON FREDERICK E IV SETSER MICHAEL E WEISENBURGH WILLIAM B		
发明人	SHELTON, FREDERICK E. IV SETSER, MICHAEL E. WEISENBURGH, WILLIAM B.		
IPC分类号	A61B17/072 A61B17/068		
CPC分类号	A61B17/07207 A61B2017/00367 A61B2017/00398 A61B2017/07214 A61B2017/07285 A61B2090/08021 A61B2090/0814		
优先权	10/441424 2003-05-20 US 11/538237 2006-10-03 US		
其他公开文献	EP1479348A1		
外部链接	Espacenet		

摘要(译)

用于腹腔镜和内窥镜临床手术的外科器械同时切断并缝合夹在末端执行器中的组织，该末端执行器包括保持钉仓的细长通道和枢转连接的砧座。电子束击发杆接合通道并在远侧击发运动期间选择性地接合砧座，其中组织被切断并被钉钉从钉仓向上驱动以形成抵靠砧座。特别地，与钉仓成一体的楔形件由击发杆的中间销向远侧驱动以实现钉合。细长通道的单个锁定响应于楔形滑板在其未击发位置的存在，以允许击发杆发射。否则，单个锁定装置可防止在钉仓丢失或耗尽时发射。

