



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
16.06.2010 Bulletin 2010/24

(51) Int Cl.:
A61B 17/122 (2006.01)

(21) Application number: **09015108.5**

(22) Date of filing: **06.10.2004**

(84) Designated Contracting States:
AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IT LI LU MC NL PL PT RO SE SI SK TR

- **Gurskis, Donnell, W.**
Belmont, CA 94002 (US)
- **Bacich, Steven, R.**
Half Moon Bay, CA 94019 (US)

(30) Priority: **08.10.2003 US 681700**

(62) Document number(s) of the earlier application(s) in accordance with Art. 76 EPC:
04816910.6 / 1 670 364

(74) Representative: **Zimmermann & Partner**
Postfach 330 920
80069 München (DE)

(71) Applicant: **Arbor Surgical Technologies, Inc.**
Irvine, CA 92614 (US)

Remarks:

This application was filed on 07-12-2009 as a divisional application to the application mentioned under INID code 62.

(72) Inventors:
• **Drews, Michael J.**
Sacramento, CA 95817 (US)

(54) **Attachment device and methods of using the same**

(57) Devices for attaching a first mass and a second mass and methods of making and using the same are disclosed. The devices can be made from an resilient, elastic or deformable materials. The devices can be used to attach a heart valve ring to a biological annulus. The devices can also be used for wound closure or a variety of other procedures such as anchoring a prosthesis to surrounding tissue or another prosthesis, tissue repair, such as in the closure of congenital defects such as septal heart defects, tissue or vessel anastomosis, fixation of tissue with or without a reinforcing mesh for hernia repair, orthopedic anchoring such as in bone fusing or tendon or muscle repair, ophthalmic indications, laparoscopic or endoscopic tissue repair or placement of prostheses, or use by robotic devices for procedures such as those above performed remotely

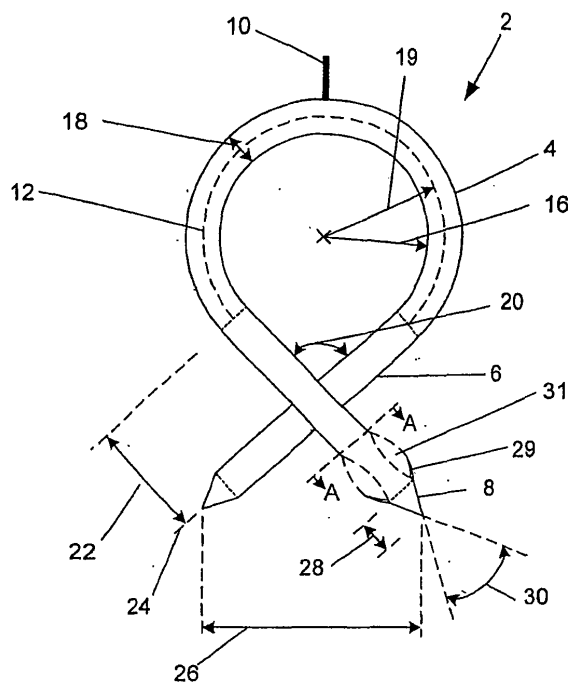


Fig. 1

Description

BACKGROUND OF THE INVENTION

1. Field of the Invention

[0001] The present invention relates generally to a device for attaching a first mass to a second mass and methods of making and using the same.

2. Description of the Related Art

[0002] Prosthetic heart valves can replace defective human valves in patients. Prosthetic valves commonly include sewing rings, suture cuffs or rings that are attached to and extend around the outer circumference of the prosthetic valve orifice.

[0003] In a typical prosthetic valve implantation procedure, the aorta is incised and the defective valve is removed leaving the desired placement site that may include a fibrous tissue layer or annular tissue. Known heart valve replacement techniques include individually passing sutures through the fibrous tissue or desired placement site within the valve annulus to form an array of sutures. Free ends of the sutures are extended out of the thoracic cavity and laid, spaced apart, on the patient's body. The free ends of the sutures are then individually threaded through a flange of the sewing ring. Once all sutures have been run through the sewing ring (typically 12 to 18 sutures), all the sutures are pulled up taught and the prosthetic valve is slid or "parachuted" down into place adjacent the placement site tissue. The prosthetic valve is then secured in place by traditional knot tying with the sutures. This procedure is time consuming as doctors often use three to ten knots per suture.

[0004] The sewing ring is often made of a biocompatible fabric through which a needle and suture can pass. The prosthetic valves are typically attached to the sewing rings which are sutured to a biological mass that is left when the surgeon removes the existing valve from the patient's heart. The sutures are tied snugly, thereby securing the sewing ring to the biological mass and, in turn, the prosthetic valve to the heart.

[0005] During heart valve replacement procedures, the patient is on heart-lung bypass which reduces the patient's oxygen level and creates non-physiological blood flow dynamics. The longer a patient is on heart-lung bypass, the greater the risk for permanent health damage. Existing suturing techniques extend the duration of bypass and increase the health risks due to heart-lung bypass. Furthermore, the fixturing force created by suturing varies significantly from suture to suture, even for the same medical professional.

[0006] In addition, sutures and other attachment devices are used in a variety of medical applications where the use of the device of the present invention would provide an advantage in fixing a first mass to a second mass, where the first mass is a tissue or a device or prosthesis,

and the second mass is a tissue or a device or prosthesis. These applications include anchoring a prosthesis such as a synthetic or autologous graft to surrounding tissue or another prosthesis, tissue repair such as in the closure of congenital defects such as septal heart defects, tissue or vessel anastomosis, fixation of tissue with or without a reinforcing mesh for hernia repair, orthopedic anchoring such as in bone fusing or tendon or muscle repair, ophthalmic indications, laparoscopic or endoscopic tissue repair or placement of prostheses, or use by robotic devices for procedures performed remotely.

[0007] For these indications and others, there is a need for a fixturing device to minimize the time spent fixturing certain devices or conduits, such as a valve prosthesis and a second mass, a vessel to another vessel or anatomical structure, tissue to tissue, surrounding tissue to a second prosthesis, and the like as described above. Furthermore, there is a need for a device that complements existing suturing or attachment devices and methods and reduces fixturing times. Also, there is a need for a fixturing device that can be easily removed. There also exist a need to provide a fixturing device that can provide a consistent fixturing force.

SUMMARY OF THE INVENTION

[0008] A device for connecting a first mass to a second mass is disclosed. The device has a base and a first leg. The base has a base axis, a first end and a second end. The first leg extends from the first end of the base. The device has a first configuration and a second configuration. When the base is rotated with respect to the base axis, the device is in the first configuration. The device can also have a second leg extending from the second end of the base.

[0009] Another device for connecting a first mass to a second mass is disclosed. The device has a base, a first leg and a second leg. The base has a base axis, a first end and a second end. The first leg has a first longitudinal axis and a first leg length. The first leg extends from the first end of the base. The second leg has a second longitudinal axis and a second leg length. The second leg extends from the second end of the base. The first leg length is substantially longer than the second leg length.

[0010] The device can have a first configuration and a second configuration. When the base is rotated with respect to the base axis, the device is in the first configuration.

[0011] Yet another device for connecting a first mass to a second mass is disclosed. The device has a base, a first leg and a second leg. The base is curved. The base has a base diameter, a first end and a second end. The first leg has a first longitudinal axis and a first leg length. The first leg extends from the first end of the base. The second leg has a second longitudinal axis and a second leg length. The second leg extends from the second end of the base. The device has a relaxed configuration. In the relaxed configuration the first leg crosses

the second leg at a leg angle. The leg angle is less than 180 degrees.

[0012] The leg angle can be less than or equal to 90 degrees. The leg angle can be less than or equal to 60 degrees. The base diameter can be less than or equal to 0.13 inches. The base diameter can be greater than or equal to 0.08 inches.

[0013] A method of attaching a first mass to a second mass is disclosed. The method uses an attachment device having a base, a first leg, and a second leg. The base has a first end and a second end. The first leg extends from the first end of the base. The second leg extends from the second end of the base. The attachment device has a first configuration and a second configuration. The method includes holding the attachment device in the first configuration. The method also includes twisting the base of the attachment device to force the attachment device into the second configuration. Further, the method includes inserting the attachment device into the first mass and the second mass. The method also includes releasing the attachment device.

[0014] Twisting the base of the attachment device can occur before inserting the attachment device into the first mass. Inserting the attachment device, at least partially, into the first mass can occur before twisting the base of the attachment device.

[0015] Another method of attaching a first mass to a second mass is disclosed. The method includes forcibly holding an attachment device in a second configuration. The attachment device has a first configuration and the second configuration. The method also includes inserting the attachment device into the first mass and the second mass. The method also includes releasing the attachment device into the first configuration.

[0016] According to the present invention there is provided a device for attaching a first mass to a second mass comprising a base having a base axis, a first end and a second end, a first leg, wherein the first leg extends from the first end of the base, and wherein the device has a first configuration and a second configuration, and wherein the device is in the first configuration when the base is rotated with respect to the base axis.

[0017] Advantageously the device further comprises a second leg, wherein the second leg extends from the second end of the base.

[0018] According to a further aspect of the present invention there is provided a device for attaching a first mass to a second mass comprising a base having a base axis, a first end and a second end, a first leg having a first longitudinal axis and a first leg length, wherein the first leg is attached to the first end of the base, and a second leg having a second longitudinal axis and a second leg length, wherein the second leg extends from the second end of the base, and wherein the first leg length is longer than the second leg length.

[0019] Advantageously the device has a first configuration and a second configuration, and wherein the device is in the first configuration when the base is rotated

with respect to the base axis.

[0020] Advantageously the first leg length is greater than or equal to three times the second leg length.

[0021] According to a yet further aspect of the present invention there is provided a device for attaching a first mass to a second mass comprising a curved base having a base diameter, a first end and a second end, a first leg having a first longitudinal axis and a first leg length, wherein the first leg extends from the first end of the base, and a second leg having a second longitudinal axis and a second leg length, wherein the second leg extends from the second end of the base, wherein the device has a relaxed configuration, and wherein in the relaxed configuration the first leg crosses the second leg at a leg angle, and wherein the leg angle is less than 180 degrees.

[0022] Advantageously the leg angle is less than or equal to 90 degrees. Advantageously the leg angle is less than or equal to 60 degrees. Advantageously the base diameter is less than or equal to 0.13 inches. Advantageously the base diameter is greater than or equal to 0.08 inches.

[0023] According to a yet further aspect of the present invention there is provided a method of attaching a first mass to a second mass using an attachment device comprising a base having a base axis, a first end and a second end, a first leg extending from the first end of the base, and a second leg extending from the second end of the base, wherein the attachment device has a first configuration and a second configuration, the method comprising holding the attachment device in the first configuration, rotating the base about the base axis to force the attachment device into the second configuration, inserting the attachment device into the first mass and the second mass; and releasing the attachment device.

[0024] Advantageously the rotating the base occurs before the inserting the attachment device into the first mass. Advantageously the inserting the attachment device into the first mass occurs before the rotating the base. Advantageously a first object comprises a first section and a second section, and wherein the first section comprises the first mass and the second section comprises the second mass.

[0025] According to a yet further aspect of the present invention there is provided a method of attaching a first mass to a second mass, the method comprising forcibly holding an attachment device in a first configuration, wherein the attachment device has the first configuration and a second configuration; inserting the attachment device into the first mass and the second mass; and releasing the attachment device, wherein the attachment device attempts to form the second configuration when released.

BRIEF DESCRIPTION OF THE DRAWINGS

[0026]

Figure 1 is a front view of an embodiment of the at-

achment device.

Figure 2 is a side view of an embodiment of the attachment device.

Figure 3 is a bottom view of an embodiment of the attachment device.

Figures 4-10 illustrate embodiments of section A-A of the attachment device.

Figure 11 is a front view of an embodiment of the attachment device.

Figure 12 and 13 are bottom views of various embodiments of the attachment device shown in Figure 11.

Figure 14 and 15 are front views of various embodiments of the attachment device.

Figure 16 is a front perspective view of an embodiment of the attachment device.

Figure 17 is a top view of the embodiment of the attachment device shown in Figure 16.

Figure 18 is a side perspective view of an embodiment of the attachment device.

Figure 19 is a side view of the attachment device shown in Figure 18.

Figures 20 and 21 are front views of various embodiments of the attachment device.

Figure 22 is a front perspective view of an embodiment of the attachment device.

Figure 23 is a top view of the embodiment of the attachment device shown in Figure 22.

Figure 24 is a front view of an embodiment of the attachment device.

Figure 25 illustrates an embodiment of a mandrel for manufacturing the attachment device.

Figure 26 and 27 illustrate methods of changing the attachment device from a first configuration to a second configuration.

Figures 28-30 are cross-sections illustrating an embodiment of a method of using the attachment device.

Figures 31-33 are cross-sections illustrating an embodiment of a method of using the attachment device with the pledget shown in full perspective for Figures 31 and 32.

Figures 34-36 are cross-sections illustrating an embodiment of a method of using the embodiment of the attachment device shown in Figure 14. Figures 37-39 are cross-sections illustrating an embodiment of a method of using the embodiment of the attachment device shown in Figures. 18 and 19.

Figures 40-42 are cross-sections illustrating an embodiment of a method of using the attachment device.

Figure 43 is a cross-section illustrating a method of using the flag.

Figure 44 illustrates an embodiment of the tool for deploying the attachment device.

Figure 45 illustrates the end of a tool for deploying the attachment device.

Figures 46 and 47 illustrate using the tip of an em-

bodiment of the tool to deploy the attachment device.

DETAILED DESCRIPTION

[0027] Figures 1 through 3 illustrate an attachment device 2. The attachment device 2 can have a base 4, legs 6, and a tip 8 at the end of each leg 6. (Phantom lines delineate the base 4, legs 6 and tips 8.) The base 4, legs 6 and tips 8 can be separate or integral elements. A flag 10 can be attached to, and extend from, the base 4. The base 4 and/or the legs 6 can be straight or curved.

[0028] The attachment device 2 can be made from a deformable or elastic material or a combination of materials having resulting deformable or elastic properties. The material can be, for example, stainless steel alloys, nickel titanium alloys (e.g., Nitinol), cobalt-chrome alloys (e.g., ELGILOY® from Elgin Specialty Metals, Elgin, IL; CONICHROME® from Carpenter Metals Corp., Wyomissing, PA), polymers such as polyester (e.g., DACRON® from E. I. Du Pont de Nemours and Company, Wilmington, DE), polypropylene, polytetrafluoroethylene (PTFE), expanded PTFE (ePTFE), polyether ether ketone (PEEK), nylon, polyether-block co-polyamide polymers (e.g., PEBAX® from ATOFINA, Paris, France), aliphatic polyether polyurethanes (e.g., TECOFLEX® from Thermedics Polymer Products, Wilmington, MA), polyvinyl chloride (PVC), polyurethane, thermoplastic, fluorinated ethylene propylene (FEP), extruded collagen, silicone, echogenic, radioactive, radiopaque materials or combinations thereof. Examples of radiopaque materials are barium sulfate, titanium, stainless steel, nickel-titanium alloys, tantalum and gold.

[0029] Any or all elements of the attachment device 2 can be a matrix for cell ingrowth or used with a fabric, for example a covering (not shown) that acts as a matrix for cell ingrowth. The fabric can be, for example, polyester (e.g., DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE), polypropylene, PTFE, ePTFE, nylon, extruded collagen, silicone or combinations thereof.

[0030] The attachment device 2 and/or the fabric can be filled and/or coated with an agent delivery matrix known to one having ordinary skill in the art and/or a therapeutic and/or diagnostic agent. These agents can include radioactive materials; radiopaque materials; cytogenic agents; cytotoxic agents; cytostatic agents; thrombogenic agents, for example polyurethane, cellulose acetate polymer mixed with bismuth trioxide, and ethylene vinyl alcohol; lubricious, hydrophilic materials; phosphor cholene; anti-inflammatory agents, for example non-steroidal anti-inflammatories (NSAIDs) such as cyclooxygenase-1 (COX-1) inhibitors (e.g., acetylsalicylic acid, for example ASPIRIN® from Bayer AG, Leverkusen, Germany; ibuprofen, for example ADVIL® from Wyeth, Collegeville, PA; indomethacin; mefenamic acid), COX-2 inhibitors (e.g., VIOXX® from Merck & Co., Inc., Whitehouse Station, NJ; CELEBREX® from Pharmacia Corp., Peapack, NJ; COX-1 inhibitors); immuno-

suppressive agents, for example Sirolimus (RAPA-MUNE®, from Wyeth, , Collegeville, PA), or matrix metalloproteinase (MMP) inhibitors (e.g., tetracycline and tetracycline derivatives) that act early within the pathways of an inflammatory response. Examples of other agents are provided in Walton et al, Inhibition of Prostaglandin E2 Synthesis in Abdominal Aortic Aneurysms, Circulation, July 6, 1999, 48-54; Tambiah et al, Provocation of Experimental Aortic Inflammation Mediators and Chlamydia Pneumoniae, Brit. J. Surgery 88 (7), 935-940; Franklin et al, Uptake of Tetracycline by Aortic Aneurysm Wall and Its Effect on Inflammation and Proteolysis, Brit. J. Surgery 86 (6), 771-775; Xu et al, Sp1 Increases Expression of Cyclooxygenase-2 in Hypoxic Vascular Endothelium, J. Biological Chemistry 275 (32) 24583-24589; and Pyo et al, Targeted Gene Disruption of Matrix Metalloproteinase-9 (Gelatinase B) Suppresses Development of Experimental Abdominal Aortic Aneurysms, J. Clinical Investigation 105 (11), 1641-1649 which are all incorporated by reference in their entireties.

[0031] A base axis 12 can extend longitudinally through the transverse cross-sectional center of the base 4. As shown in Figure 2, when viewed from the side, the base axis 12 can form a base plane angle 14 from about 0° to about 30°, for example about 10°. The base 4 can have a base inner radius 16 from about 0.25 mm (0.010 in.) to about 19.1 mm (0.750 in.), for example about 1.91 mm (0.075 in.). The proximal end of the base 4 can be formed into a table 17. The table 17 can be a flat surface that tapers to the base 4

[0032] The base 4 and legs 6 can have a shaft diameter 18 from about 0.03 mm (0.001 in.) to about 6.35 mm (0.250 in.), for example, about 0.51 mm (0.020 in.). The base 4 and legs 6 can have the same or different shaft diameters 18. A base neutral radius 19 can be the base inner radius 16 and half the shaft diameter 18. As shown in Figure 1, the legs 6 can intersect at a leg angle 20 in or near the plane of the attachment device 2 or in or near the approximate plane of the base 4. An approximate plane is a plane that can be used whether the base 4 does or does not fall on a flat plane. If the base 4 is a straight line or a point, the approximate plane of the base 4 can be calculated using the points of the legs 6 that are nearest the base 4 and out of line with the base 4. The leg angle 20 can be from about 180° to about 10°, more narrowly from about 90° to about 60°, for example about 45° or, for example, about 60°.

[0033] The length from an end of the base 4 to a longitudinal leg axis 24 can be a body length 22. The body length 22 can be from about 0.25 mm (0.010 in.) to about 12.7 mm (0.500 in.), for example about 2.913 mm (0.1147 in.). The length between the distal end of one tip 8 and the distal end of the opposite tip 8 can be a tip distance 26. The tip distance 26 can be from about 0.03 mm (0.001 in.) to about 25.4 mm (1.000 in.), more narrowly about 1.3 mm (0.050 in.) to about 3.18 mm (0.125 in.), for example about 2.3 mm (0.090 in.).

[0034] The tip 8 can have a tip length 28 from about

0.05 mm (0.002 in.) to about 12.7 mm (0.500 in.), for example about 1.0 mm (0.040 in.). The tip 8 can have a tip angle 30 from about 5° to about 90°, for example about 30°. The tips 8 can be straight, pointed ends, curve out of line (shown by alternative tips 8a and 8b, drawn in phantom lines in Figures 2 and 3) from the nearest end of the leg 6, or combinations thereof.

[0035] The tips 8 and/or legs 6 can have retention devices 29. The retention devices 29 can be barbs, spikes, hooks, threads, ribs, splines, a roughened surface, a sintered surface, a covered surface (e.g., with DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE) or combinations thereof. A retention coating 31, for example a biodegradable coating or filler such as gel or gelatin or otherwise removable, can be on and/or around and/or near the retention devices 29. The retention coating 31 (shown in phantom lines) can be configured to render the retention device 29 substantially ineffective until a substantial amount of the retention coating 31 has been biodegraded or otherwise removed.

[0036] The legs 6 can have mechanical interfaces 33, for example, a slot, snap, protrusion, latch, catch or combinations thereof. The interfaces 33 can be aligned so the interface on one leg 6 meets the interface 33 on the other leg 6 at the point where the legs 6 cross. The interfaces 33 can removably attach to each other.

[0037] Figures 4 through 10 illustrate examples of cross-section A-A of the legs 6 and/or the base 4. The cross-section A-A of the legs 6 can be the same or different as the cross-sections of the base 4. The cross-sections of the base 4 and/or legs 6 can be constant or vary along their respective lengths. Figures 4 through 8, respectively, illustrate circular, rectangular (including square), triangular, substantially flat, and star-shaped or irregular cross-sections A-A. Figure 9 illustrates an oval cross-section A-A. A ratio of the shaft diameter 18 to the length of a minor axis 32 can be from about 1:1 to about 20:1, for example 10:1.

[0038] Figure 10 illustrates a cavity 36 inside the cross-section A-A. The cavity 34 can be hollow or can be filled completely or partially. The cavity 34 can be filled with an agent delivery matrix known to one having ordinary skill in the art and/or a therapeutic and/or diagnostic agent and/or echogenic and/or radioactive and/or radiopaque materials, for example, the agents and/or materials listed supra. The type and amount of filling can vary along the length of the base 4 and/or legs 6. The ratio of the shaft diameter 18 to a cavity diameter 36 can be from about 1:1 to about 50:1, for example, about 2:1.

[0039] Figure 11 illustrates an attachment device 2 that can have a leg 6 that can have a first leg segment 38 and a second leg segment 40. The first leg segment 38 can extend from the base 4. The second leg segment 40 can extend on a proximal end from the first leg segment 38. The tip 8 can extend from a distal end of the second leg segment 40. The second leg segment 40 can have a different radius of curvature than the first leg segment 38 and/or form an angle with respect to the first leg seg-

ment 40. Figure 12 illustrates that the second leg segment 40 can form an angle (shown by arrows) with the approximate plane of the base 4. Figure 13 illustrates that the first leg segment 38 can form an angle (shown by arrows) with the approximate plane of the base 4. The second leg segments 40 can be substantially parallel with the approximate plan of the base 4.

[0040] Figure 14 illustrates an attachment device 2 that can have a first leg 6a that can be substantially longer than a second leg 6b. The ratio of a first leg-tip length 22a to a second leg-tip length 22b can be from about 1:1 to about 10:1, for example, about 3:1.

[0041] Figure 15 illustrates an attachment device that can have a first leg radius 42 and a second leg radius 44. The ratio of the first leg radius 42 to the second leg radius 44 can be from about 1:1 to about 50:1, for example about 10:1.

[0042] Figures 16 and 17 illustrate an attachment device 2 that can have a "flat top." The approximate plane of the second leg 6b can form an angle, for example about 90°, with the approximate plane of the base 4. When in use, the flat top can further anchor the attachment device 2 against the first mass and/or second mass. Figures 18 and 19 illustrate an attachment device 2 that can have arms 6 that can wrap around the base axis 12.

[0043] Figure 20 illustrates an attachment device 2 that can have arms 46 that can extend from the base 4 and/or the legs 6. When deployed, the arms 46 can squeeze tissue between the arms 46 and the legs 6 and/or base 4 for additional retention force. Anchors 48 can extend from the arms 46, for example at the distal ends of the arms 46. The anchors 48 can be, for example, hooks, barbs, spikes, staples or combinations thereof. The anchors 48 can extend directly from the base 4 and/or legs 6 with or without arms 46 separately attached to the base 4 and/or legs 6. Figure 21 illustrates an attachment device 2 that can have a straight base 4 and can have the arms 46 extending from the base 4.

[0044] Figures 22 and 23 illustrate an attachment device that can have first, second and third legs 6a, 6b and 6c. The base 4 can be a platform, wire frame, or point attachment which can be spot-welded or brazed, tube crimped or otherwise mechanically connected. The planes of the legs 6a, 6b and 6c can intersect at substantially equal angles, about 120°, or unequal angles.

[0045] Figure 24 illustrates an attachment device that can have a first loop 49 and a second loop 51. The first loop 49 can be formed from the base 4 and a proximal portion of the first leg segments 38. The second loop 51 can be formed from a distal portion of the first leg segments 38 and a proximal portion of the second leg segments 40.

METHODS OF MAKING

[0046] Figure 25 illustrates a mandrel 50 that can be used to form the attachment device 2, for example during heat treatment. The base 4 and/or legs 6 can be held on

the mandrel 50 by a single cylinder 52, a formed path 54, a pressure plate 56, for example a washer under a screw or combinations thereof. Methods for forming shape memory alloys (e.g., Nitinol) are known to those having ordinary skill in the art. The tips 8 can be formed, for example, by grinding, electropolishing, or precision sharpening (e.g., polishing services from Point Technologies, Inc., Boulder, CO) to a satisfactory geometry, including a trocar point, beveled, rounded, tapered, pointed or flattened.

[0047] Other methods known to one having ordinary skill in the art can be used to manufacture the attachment device 2 and/or its elements. For example, manufacturing techniques include molding, machining, casting, forming (e.g., pressure forming), crimping, stamping, melting, screwing, gluing, welding, die cutting, laser cutting, electrical discharge machining (EDM), etching or combinations thereof.

[0048] Any elements, sub-assemblies, or the attachment device 2 as a whole after final assembly, can be coated by dip-coating or spray-coating methods known to one having ordinary skill in the art, utilizing materials such as PTFE (e.g., TEFLON® from E. I. du Pont de Nemours and Company, Wilmington, DE), polyester (e.g., DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE), gelatin, gel, other polymers or combinations thereof. One example of a method used to coat a medical device for vascular use is provided in U.S. Patent No. 6,358,556 by Ding et al. and hereby incorporated by reference in its entirety. Time release coating methods known to one having ordinary skill in the art can also be used to delay the release of an agent in the coating. The coatings can be thrombogenic or anti-thrombogenic.

[0049] The attachment device 2, or any element thereof (e.g., the base 4) can be covered with a fabric, for example polyester (e.g., DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE), polypropylene, PTFE (e.g., TEFLON® from E. I. du Pont de Nemours and Company, Wilmington, DE), ePTFE, nylon, extruded collagen, gel, gelatin, silicone or combinations thereof. Methods of covering an implantable device with fabric are known to those having ordinary skill in the art, for example, sintering, spray coating, adhesion, loose covering, dipping or combinations thereof.

METHODS OF USING

[0050] The attachment device 2 can have a first configuration (e.g., the configuration shown in Figures 26 and 27) and a second configuration (e.g., the configuration shown in Figures 1 through 3). The attachment device 2 can have the second configuration when the attachment device is in a relaxed state, with no external forces applied (e.g., prior to insertion or use). The attachment device 2 can have the first configuration when external forces are applied, such as by a delivery tool prior to delivery. When external forces are removed from the

attachment device 2, the attachment device 2 can revert from the first configuration to the second configuration.

[0051] The attachment device can substantially revert to the second configuration even when some permanent hysteresis deformation occurs and/or when a foreign object (e.g., a first and/or second mass) is obstructing the attachment device 2. When the attachment device 2 has the first configuration, one or both legs 6 can be rotated with respect to the base 4 (e.g., by rotating the base 4 around the base axis 12, one or both legs 6 splay or separate as they are torqued by the twisting or rotating around of the base).

[0052] Figure 26 illustrates a method of forcing the attachment device to have the first configuration. The attachment device 2 can be forced to have the first configuration by the application of a base torque, shown by arrows 58, applied about the base axis 12. The base torque can be directly applied to the base 4. The base torque indirectly becomes, or can be applied as, a leg torque, as shown by arrows 60a and 60b, to the legs 6a and/or 6b about the leg axes 24a and 24b. If approximately two times the base neutral radius 19 is less than the tip distance 26, the legs 6 will splay outward when entering the first mass 68. If approximately two times the base neutral radius 19 is greater than or equal to the tip distance 26, the legs 6 will splay inward or stay vertical when deploying into the first mass 68.

[0053] Figure 27 illustrates a method of forcing the attachment device to have the first configuration. The attachment device 2 can be forced to have the first configuration by the application of a pivot torque, shown by arrows 62, applied about the area where the base 4 attaches to the legs 6, so that the legs 6 are forced to pivot radially outward from each other. The pivot torque can be applied by applying outward translational forces, as shown by arrows 64, to one or both legs 6. The pivot torque can be applied by applying translational forces to the base 4; as shown by arrows 66.

[0054] As illustrated in Figures 28 through 30, the attachment device 2 can be deployed to attach a first mass 68 to a second mass 70. The first mass 68 and/or the second mass 70 can be a prosthesis and/or a tissue, or both tissue or both prostheses. The prosthesis can be, for example, cardiac leads, markers, stents, grafts, stent-grafts, heart valves, annuloplasty rings, autografts, allografts, xenografts or any assemblies thereof or combination thereof. The tissue can be, for example, vessels, valves, organs (e.g., intestine, heart, skin, liver, kidney, urethra, bone mass, tendon, nerve, muscle), calcified soft tissue or any combination thereof.

[0055] Heart valve assemblies disclosed by Griffin et al. in U.S. Patent No. 6,241,765, by Lane in U.S. Patent No. 6,371,983 and by Ritz in U.S. Patent No. 5,976,183, both of which are hereby incorporated in their entireties, can be placed with the use of the device of the present invention. Other heart valve assemblies that can be used include, for example, the Advantage Bileaflet heart valve, Parallel valve, Freestyle stentless aortic valve, Hancock

Porcine heart valve, Hancock apical left ventricular connector model 174A, Hancock valved conduit models 100, 105, 150, Hall Medtronic heart valve, Hall Medtronic valved conduit, MOSAIC® heart valve and Intact porcine tissue valve (by Medtronic, Inc. Minneapolis, MN); Angelini Lamina-flo valve (by Cardio Carbon Company, Ltd., England); Bjork-Shiley single-disk, monostrut and caged-disk valves (Shiley, Inc., now-defunct, previously of CA); Wada-Cutter valve and Chitra Cooley-Cutter valve (by Cutter Biomedical Corp., San Diego, CA); Angioflex trileaflet polyurethane valve (by Abiomed, Inc., Danvers, MA); ATS AP Series heart valve and ATS Standard heart valve (by ATS Medical, Inc., Minneapolis, MN); ANNULOFLO® annuloplasty ring, ANNUFLEX® annuloplasty ring, CARBSEAL® valved conduit, OR-BIS® Universal aortic and mitral valve, pediatric/small adult valve, R series valve, SUMIT® mitral valve, TOP HAT® aortic valve, OPTIFORM® mitral valve, MITROFLOW SYNERGY® PC stented aortic pericardial bioprosthesis and the SYNERGY® ST stented aortic and mitral porcine bioprosthesis (by CarboMedics, Inc., Austin, TX); ON-X® prosthetic heart valve (by MCRI®, LLC, Austin, TX); Starr-Edwards SILASTIC® ball valve, Starr-Edwards 1000, Starr-Edwards 1200, Starr-Edwards 1260, Starr-Edwards 2400, Starr-Edwards 6300, Starr-Edwards 6500, Starr-Edwards 6520, Carpentier-Edwards porcine tissue valve, Carpentier-Edwards pericardial prosthesis, Carpentier-Edwards supra-annular valve, Carpentier-Edwards annuloplasty rings, Duro-medics valve and PERIMOUNT® heart valve (by Edwards Lifesciences Corp., Irvine, CA); Cross-Jones Lenticular disc valve (by Pemco, Inc.); Tissuemed stented porcine valve (by Tissuemed, Ltd., Leeds, England); Tekna valve (by Baxter Healthcare, Corp., Deerfield, IL); Komp-01 mitral retainer ring (by Jyros Medical Ltd., London, England); SJM® Masters Series mechanical heart valve, SJM® Masters Series aortic valved graft prosthesis, ST. JUDE MEDICAL® mechanical heart valves, ST. JUDE MEDICAL® mechanical heart valve Hemodynamic Plus (HP) series, SJM REGENT® valve, TORONTO SPV® (Stentless Porcine Valve) valve, SJM BIOCOR® valve and SJM EPIC® valve (St. Jude Medical, Inc., St. Paul, MN); Sorin Bicarbon, Sorin Carbocast, Sorin Carboseal Conduit, Sorin Pericarbon and Sorin Pericarbon Stentless (by Snia S.p.A.; Italy). The attachment devices of the present invention may be deployed to implant these various devices in the supra-annular position, or infrannular, depending on the geometry and preferred placement of a particular device. Similarly, it may be advantageous to use the attachment devices 2 of the present invention to secure a sewing ring, or first prosthesis by placing them horizontally or vertically within or around the annulus of such ring, prior to placing a second prosthesis including a valve structure, as provided in U.S. Application Serial No. 10/646,639 filed, 22 August 2003, hereby incorporated by reference in its entirety.

[0056] Figure 28 illustrates that the attachment device 2 can be held in the first configuration. The attachment

device 2 can be fed through a pledget 71 before the attachment device 2 is forced into the first mass 68. The pledget 71 can be a piece of fabric, for example, a fabric listed supra. The pledget 71 can be loaded onto the attachment device 2 before use. Figure 29 illustrates that the attachment device 2 can be forced, as shown by arrow 72, into and through the first mass 68 and part of the second mass 70. Figure 30 illustrates that the attachment device 2 can be released from having the first configuration. The attachment device 2 can revert to having substantially the second configuration. A pinching force, shown by arrows, can be applied to the attachment device 2 to encourage additional reversion of the attachment device 2 to having the second configuration. The attachment device 2 shown in Figure 24 can be deployed in the same manner as described supra, except that the attachment device 2 shown in Figure 24 can be rotated sufficiently to straighten the first and second loops, before or during deployment.

[0057] The attachment device 2 can be removed and redeployed at any stage of deployment supra, for example, if the surgeon is unsatisfied with the position of the attachment device 2, or if the prosthesis need replacing or "redoing" at a point in the future. If the attachment device 2 has a retention device 29, when the retention coating 31 sufficiently biodegrades or is otherwise removed, the retention devices 29 will become exposed and can substantially prevent the removal of the attachment device 2 from the deployment site. Removal may still be achieved however, by apply sufficient force (by a tool or other device) to overcome the strength of the secondary retention element.

[0058] Figures 31 through 33 illustrate a method of deploying the attachment device 2 to attach a first mass 68 to a second mass 70. The pledget 71 can be fed over the attachment device 2 before use. The pledget 2 can be formed as a rectangular container with an access opening 73, for example a slit, hole, or aperture, to allow access to the base 4 of the attachment device 2. The attachment device 2 can have the second configuration. The attachment device 2 can be forced, as shown by arrow, so the tips 8 engage the first mass 68. Figure 32 illustrates that, with the tips 8 held by the first mass 68, a longitudinal torque, shown by arrows, applied to the attachment device 2 about a longitudinal axis 74 can then force the attachment device 2 into the first configuration. As illustrated by Figure 33, the attachment device 2 can be forced, shown by arrow, through the first mass 68 and part of the second mass 70. The longitudinal torque (not shown in Figure 33) can be removed during deployment or after the attachment device 2 is completely deployed into the first and second masses 68 and 70. The pledget 71 can be crushed during deployment.

[0059] Figures 34 through 36 illustrate a method of deploying the attachment device shown in Figure 14. The first leg 6a can be forced, as shown by arrow, into and through the first mass 68 and part of the second mass 70. The first leg 6a can have a "paddle" (not shown). The

paddle can be a flat oval or long rectangular cross-sectional shape on one leg. The paddle can increase resistive force with the first and/or second mass 68 and/or 70 when applying torque to the attachment device 2.

[0060] Figure 35 illustrates that the attachment device 2 can be forced into the first configuration by applying a base torque, shown by arrows 58. The second leg 6b can then rotate outwardly from the attachment device 2, as shown by arrow 76.

[0061] Figure 36 illustrates that the attachment device 2 can be forced, shown by arrow, through the first mass 68 and part of the second mass 70. The base torque (not shown in Figure 36) can be removed during deployment or after the attachment device 2 is completely deployed into the first and second masses 68 and 70.

[0062] Figures 37 through 39 illustrate a method of deploying the attachment device 2 shown in Figures 18 and 19. Figure 37 illustrates that the base 4 and the tips 8 can be placed in contact with or near the first mass 68. Figure 38 illustrates that the arms 6 can be rotated, as shown by arrows, about the base axis 12. The arms 6 can be rotated to cause the arms 6 to be forced into the first mass 68. Figure 39 illustrates that the arms 6 can be rotated, as shown by arrows, further about the base axis 12. The arms 6 can be forced into and through the second mass 70. The arms 6 can re-enter the first mass 68.

[0063] Figures 40 through 42 illustrate a method of deploying the attachment device 2 to attach a first mass 68 to a second mass 70. The first mass 68 and the second mass 70 can be two sections of the same object, such as when the attachment device 2 is used to close a wound. Figure 40 illustrates that the attachment device 2 can be held in the first configuration. Figure 41 illustrates that the attachment device 2 can be forced, as shown by arrow 72, so that the first leg 6a inserts into the first mass 68 and that the second leg 6b inserts into the second mass 70. Figure 42 illustrates that the attachment device 2 can be released from having the first configuration. The attachment device 2 can revert to having substantially the second configuration, causing the legs 6a and 6b to rotate inward, shown by arrows 78, applying force, shown by arrows 80, to the first mass 68 and the second mass 70 such that the first and second masses 68 and 70 move toward each other.

[0064] The attachment device 2 can be removed from the second mass 70 and/or the first mass 68, when applicable, by reversing the steps of the deployment methods supra.

[0065] Figure 43 illustrates that, during use, the attachment device 2 can be covered by new tissue growth 82. The flag 10 can extend outside of the new tissue growth 82 (as shown) or be located just below the surface but palpable. The flag 10 can act as a marker, palpable or visible by direct vision or imaging modalities known in the art (e.g., x-ray, magnetic resonance imaging (MRI), ultrasound, computed tomography (CT), echocardiogram) for example to locate the attachment device 2 in

case of removal of the attachment device 2. The flag 10 can be made of, for example, suture material (e.g., Nylon, polyglycolic acid, polyester such as DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE, metals such as those used in the other elements of the attachment device 2, other polymers or combinations thereof). The base 4 can also serve this function (e.g., of a marker) in some applications.

[0066] Figure 44 illustrates a tool 84 for deploying the attachment device 2. The tool 84 can have a first lever 86 and a second lever 88. The first lever 86 can be rotatably attached to the second lever 88 at a pivot 90. The first and second levers 86 and 88 can have a handle 92 at each lever's first end and a pad 94 at each lever's second end. The pads 94 can be used to hold the attachment device 2. When a force is applied to the handles 92, shown by arrows 96, the force is transmitted, shown by arrows 98, to the pads 94.

[0067] A driver shaft 100 can have a driver handle 102 at a first end and grips 104 at a second end. The pivot 90 can have a longitudinal channel 106. The driver shaft 100 can pass through the longitudinal channel 106 and/or be rotatably mounted to a case (not shown) fixed to a lever 86 or 88. The grips 104 can be releasably attached to the attachment device 2. The attachment device 2 can be rotated about the longitudinal axis 2 by releasing the pads 94 and rotating, as shown by arrows 108, the driver handle.

[0068] Figure 45 shows the end of a tool 84 for deploying the attachment device 2 before the attachment device 2 has been loaded into the tool 84. The tool 84 can have a top part 110 and a bottom part 112. The top part 110 can be removably attached to the bottom part, as shown by arrow 114.

[0069] The top part 110 and/or the bottom part 112 can have grooves 116 sized to fit the base 4 and a portion of one or more legs 6 when the attachment device 2 has the first configuration. The attachment device 2 can be forced to have the first configuration and be loaded into the tool 84, as shown by arrow 118. The top part 110 can be attached to the bottom part 112 with the attachment device 2 seated (not shown) in the grooves 116.

[0070] The attachment device 2 can be placed at a desired deployment site by the tool 84. The device 2 can be deployed from the tool 84 by removing the top part 110 from the bottom part 112, and removing the tool 84 from the deployment site.

[0071] Figures 46 illustrates an end of a tool 84. The tool 84 can have a case 120 with an anvil 122 and leg ports 124. The case 120 can be slidably attached to a slide 126. The attachment device 2 can be loaded around the anvil 122. The legs 6 can protrude from the case 120 through the leg ports 124.

[0072] Figure 47 illustrates a method of using the tool 84 of Figure 46 to deploy the attachment device 2. The slide 126 can be forced, as shown by arrow 128, toward the anvil 122. The slide 126 can push the base 4 against the anvil 122, causing the legs 6 to rotate outward, as

shown by arrows 76. The surface geometry of the anvil 122 and the slider 126 can match the surface geometry of the attachment device 2, when the attachment device is fully strained, as shown in Figure 39. The attachment device 2 can then be inserted into the desired deployment site (not shown). When the attachment device 2 is in place, the attachment device 2 can be deployed from the tool 84, for example, by sliding the anvil 122 out of the way (perpendicular to the plane of Figure 47) and forcing the attachment device 2 out the end of the tool 84 with the slide 126.

[0073] The ends of the tools 84 shown in Figures 45 through 47 can be pivoted to the remainder of the tool 84 by methods known to those having ordinary skill in the art. The pivotable end of the tool 84 can improve access to deployment sites not as easily accessible by a non-articulating tool 84. The tool 84 can be non-articulatable. It would also be possible when access to the site of implantation allows, to employ a tool substantially similar to a needle driver tool known to those skilled in the art.

[0074] Additional disclosure is included in U.S. Patent Application Serial Nos. 10/327,821 and 10/646,639, filed 20 December 2002 and 22 August 2003, respectively, which are hereby incorporated by reference in their entireties. It is apparent to one skilled in the art that various changes and modifications can be made to this disclosure, and equivalents employed, without departing from the spirit and scope of the invention. Elements shown with any embodiment are exemplary for the specific embodiment and can be used on other embodiments within this disclosure.

Claims

1. A system for securing a prosthesis to tissue within a patient's body, comprising:

an attachment device (2) comprising a base (4) and a pair of legs (6) extending from the base (4), the attachment device (2) being elastically movable from a first relaxed configuration wherein the legs (6) cross one another and a second delivery configuration wherein the legs (6) extend substantially parallel with one another;

a tool (84) for deploying the attachment device (2), the attachment device (2) being loadable into the tool (84) with the attachment device (2) in the relaxed configuration; and

a prosthesis (68) securable to tissue (70) using the attachment device (2) while applying a force using the tool (84) to place the attachment device (2) in the delivery configuration, the attachment device (2) being releasable from the tool (84) such that the attachment device (2) returns towards the relaxed configuration such that the

- legs (6) cross one another.
2. The system of claim 1, wherein the prosthesis comprises at least one of a stent, a graft, a stent-graft, an annuloplasty ring, an autograft, an allograft, and a xenograft. 5
 3. The system of claim 1, wherein the prosthesis comprises a heart valve prosthesis securable to a tissue annulus using the attachment device. 10
 4. The system of claim 3, wherein the heart valve prosthesis comprises a first prosthesis comprising a sewing ring and a second prosthesis comprising a valve structure, and wherein the attachment device is used to attach the first prosthesis within or around the annulus. 15
 5. The system of claim 4, wherein the tool (84) is configured for securing the heart valve prosthesis to a tissue annulus by inserting a plurality of attachment devices (2) through the sewing ring, wherein each attachment device (2) is delivered by: 20
 - a) holding the attachment device (2) in the tool (84) in the relaxed configuration; 25
 - b) applying a force with the tool (84) to force the attachment device (2) to the delivery configuration; 30
 - c) inserting the legs (6) through the sewing ring into tissue with the attachment device (2) in the delivery configuration; and 30
 - d) deploying the attachment device (2) from the tool (84) such that the attachment device (2) returns towards the relaxed configuration; and 35

thereafter placing the second prosthesis.
 6. The system of claim 5, wherein the tool (84) comprises an anvil (122), and step a) comprises loading the attachment device (2) around the anvil (122) in the relaxed configuration. 40
 7. The system of claim 5, wherein the tool (84) comprises a slide (126) and an anvil (122) for causing the legs (6) of the attachment device (2) to rotate outward to the delivery configuration during step b). 45
 8. The system of claim 7, wherein step d) comprises sliding the anvil (122) out of the way and forcing the attachment device (2) out the end of the tool (84) with the slide (126). 50
 9. The system of claim 5, wherein the tool (84) retains the attachment device (2) in the delivery configuration while the attachment device (2) is inserted through the sewing ring into tissue, whereupon the attachment device (2) is deployed from the tool (84). 55

10. The system of any preceding claim, wherein the legs (6) of the attachment devices (2) comprise tips (8) with straight pointed ends that allow the attachment device (2) to be removed and redeployed at any stage of deployment.
11. The system of any one of claims 1-4, wherein the tool (84) comprises a slide (126) and an anvil (122) for causing the legs (6) of the attachment device (2) to rotate outward to the delivery configuration.
12. The system of claim 11, wherein the attachment device (2) is deployable from the tool (84) by sliding the anvil (122) out of the way and forcing the attachment device (2) out the end of the tool (84) with the slide (126).
13. The system of any preceding claim, wherein the attachment device (2) comprises a curved base (4) having a base diameter, a first end and a second end, a first leg (6) having a first longitudinal axis (24) and a first leg length, wherein the first leg extends from the first end of the base, and a second leg (6) having a second longitudinal axis (24) and a second leg length, wherein the second leg (6) extends from the second end of the base (4), and wherein, in the delivery configuration, the legs (6) splay apart to allow the attachment device (2) to be forced through the prosthesis into the tissue when external forces are applied by the tool (84) and, wherein, in the relaxed configuration, the first leg (6) crosses the second leg (6) at a leg angle (20), and wherein the leg angle is less than 180 degrees.
14. An apparatus for attaching two masses, the apparatus comprising:

an attachment device (2) made from elastic material for securing a prosthesis to tissue; and
a tool (84) for deploying the attachment device (2),

wherein the attachment device (2) comprises:

a curved base (4) having a base diameter, a first end and a second end, a first leg (6) having a first longitudinal axis (24) and a first leg length, wherein the first leg extends from the first end of the base, and a second leg (6) having a second longitudinal axis (24) and a second leg length, wherein the second leg (6) extends from the second end of the base (4); and

wherein the attachment device (2) has a first configuration in which the legs (6) splay apart to allow the attachment device (2) to be forced through the prosthesis into the tissue when external forces are applied by the tool (84) and a second relaxed configuration

ration, wherein the first leg (6) crosses the second leg (6) at a leg angle (20), and wherein the leg angle is less than 180 degrees, the attachment device (2) reverting from the first configuration towards the second relaxed configuration when external forces are removed from the attachment device (2). 5

15. The apparatus of claim 14, further comprising a pledget (71), wherein the attachment device (2) can be fed through a pledget (71) before the attachment device (2) is forced into the prosthesis and tissue. 10

15

20

25

30

35

40

45

50

55

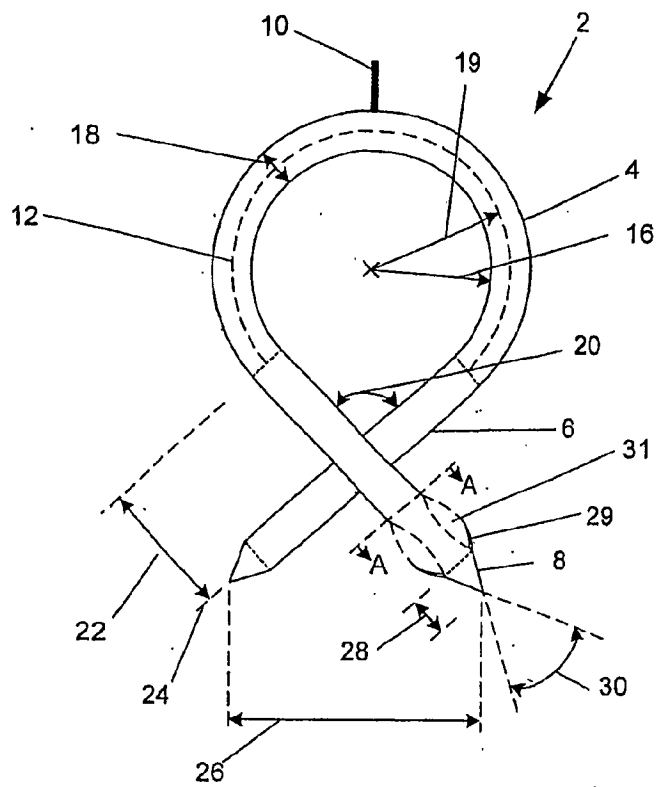


Fig. 1

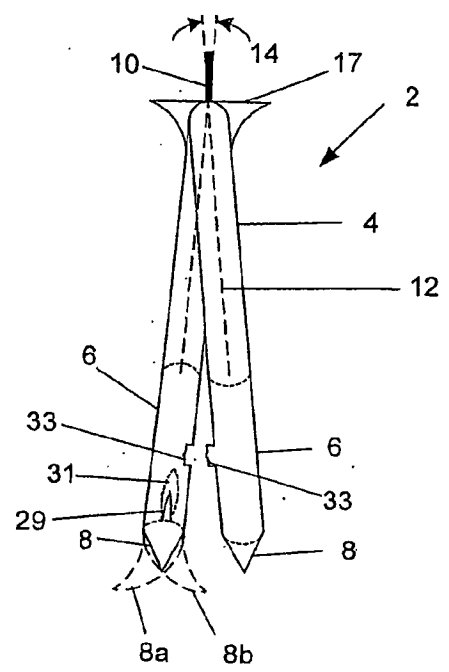


Fig. 2

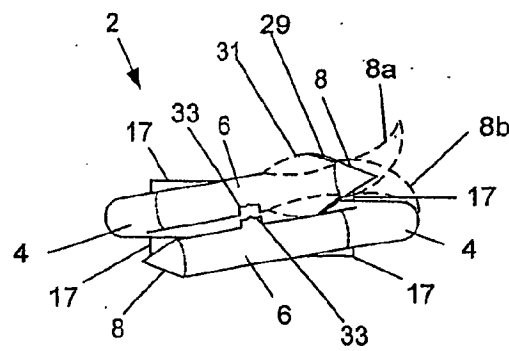


Fig. 3




Fig. 4




Fig. 5



Fig. 6



Fig. 7

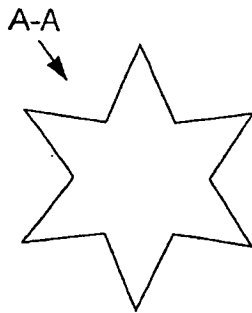


Fig. 8




Fig. 9


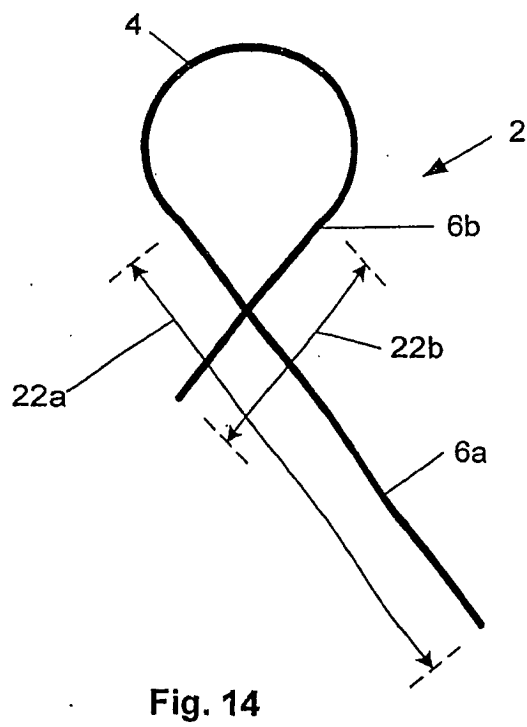
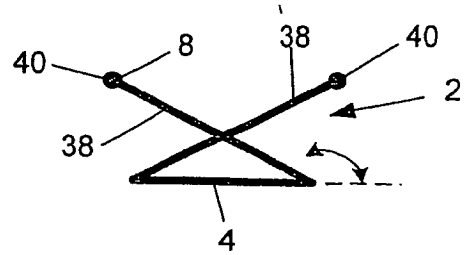
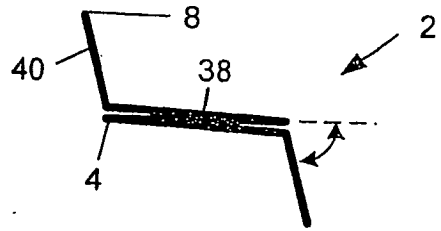
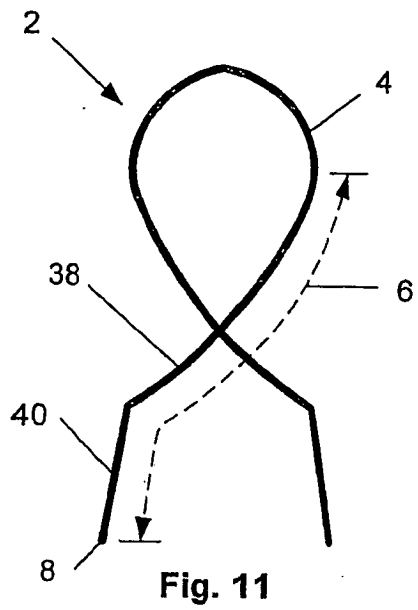


Fig. 10



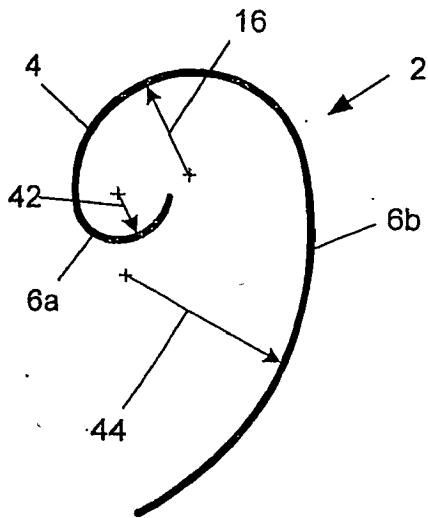


Fig. 15

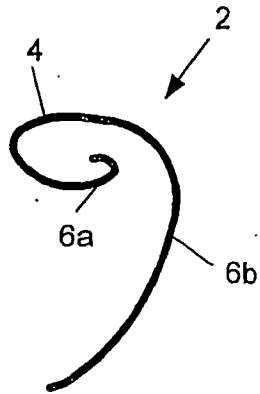


Fig. 16

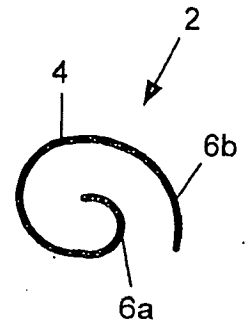


Fig. 17

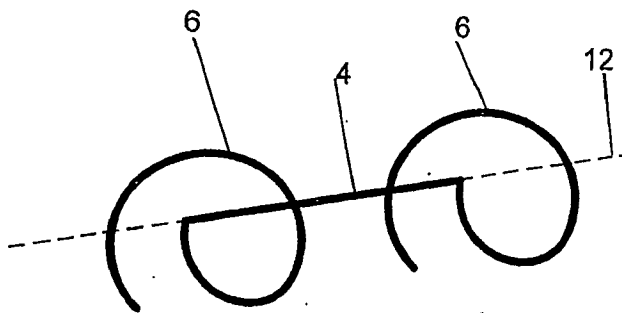


Fig. 18





Fig. 19

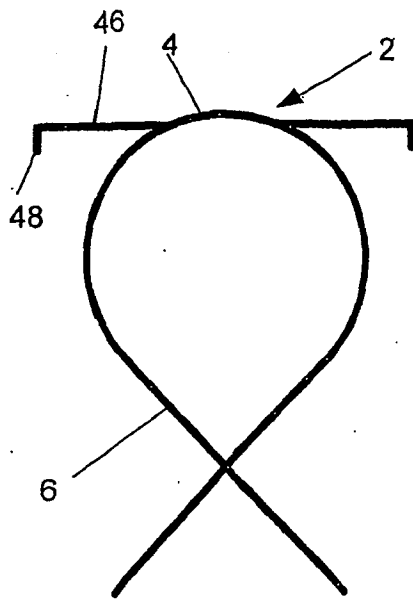

20

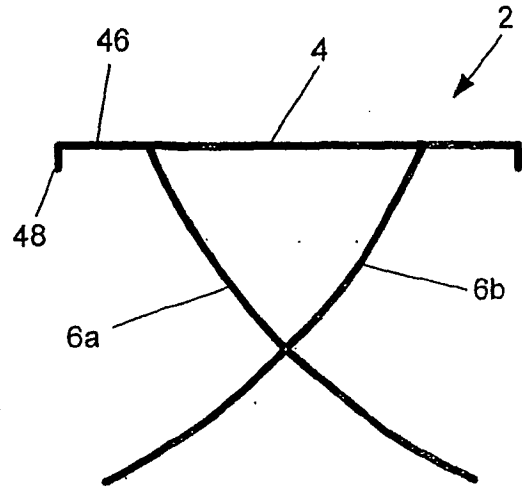


Fig. 21

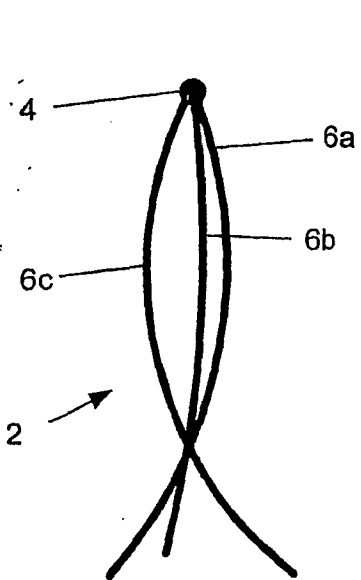


Fig. 22

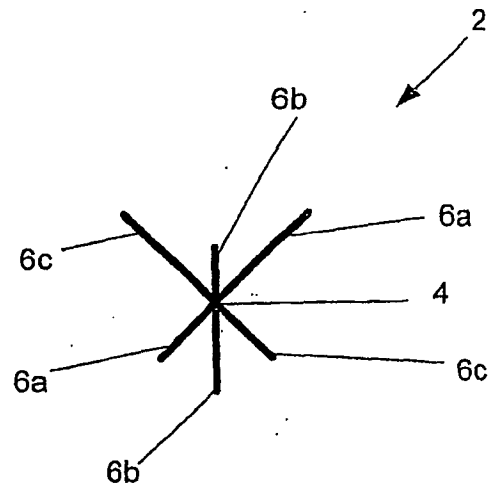


Fig. 23

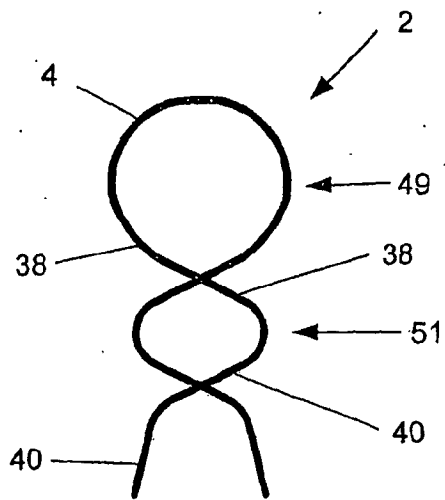


Fig. 24

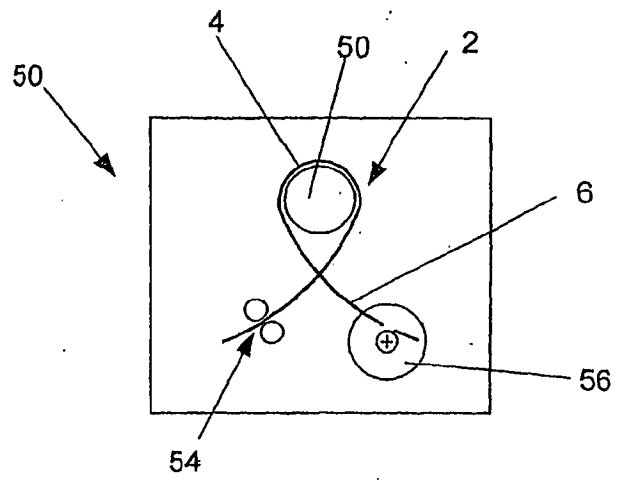


Fig. 25

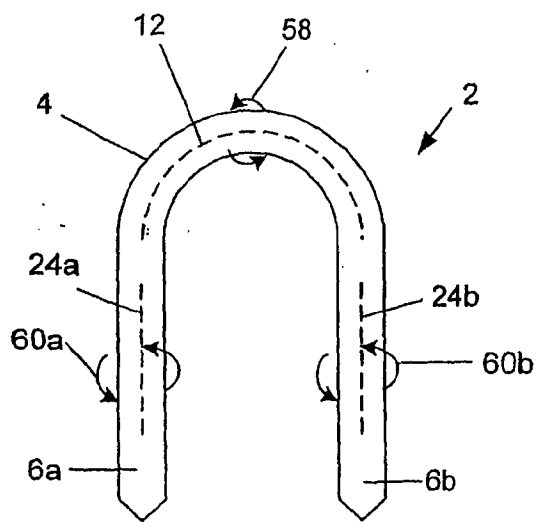


Fig. 26

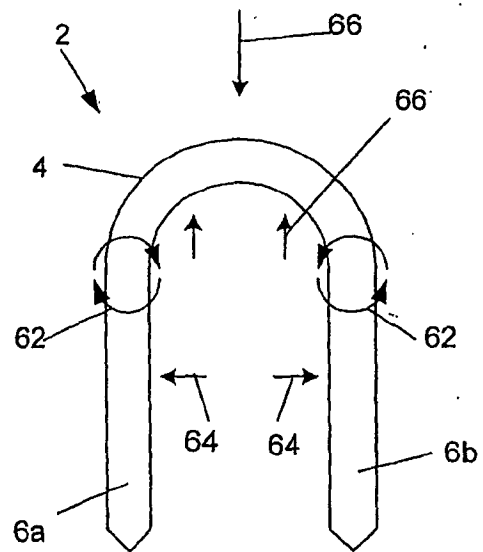


Fig. 27

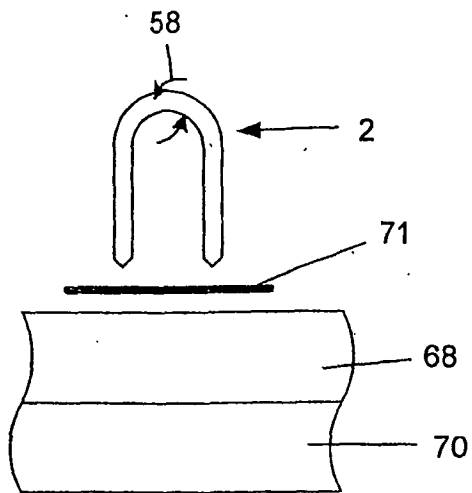


Fig. 28

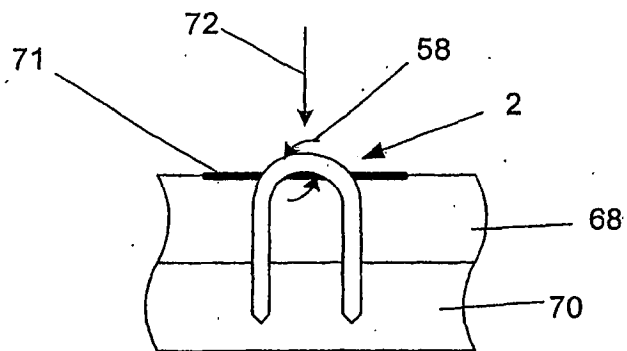


Fig. 29

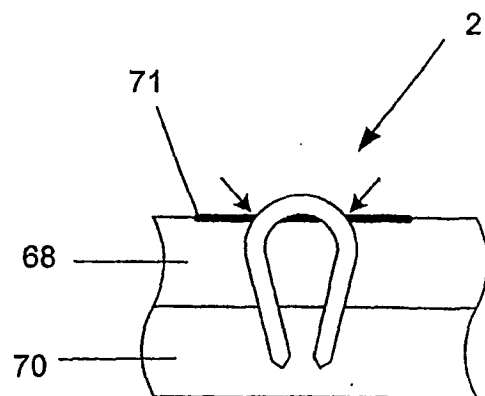


Fig. 30

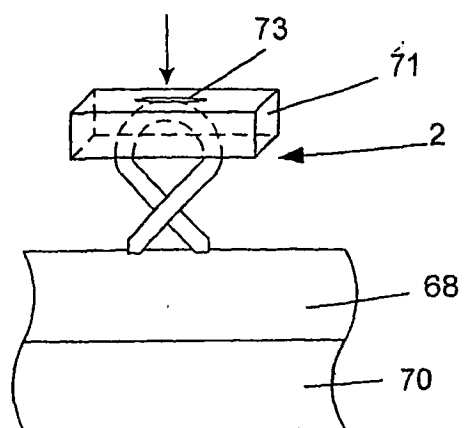


Fig. 31

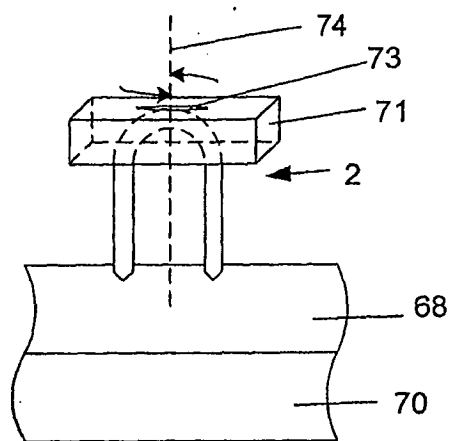


Fig. 32

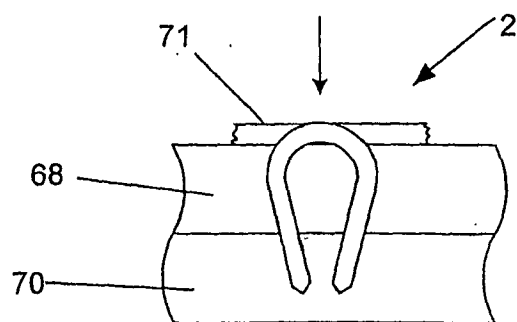


Fig. 33

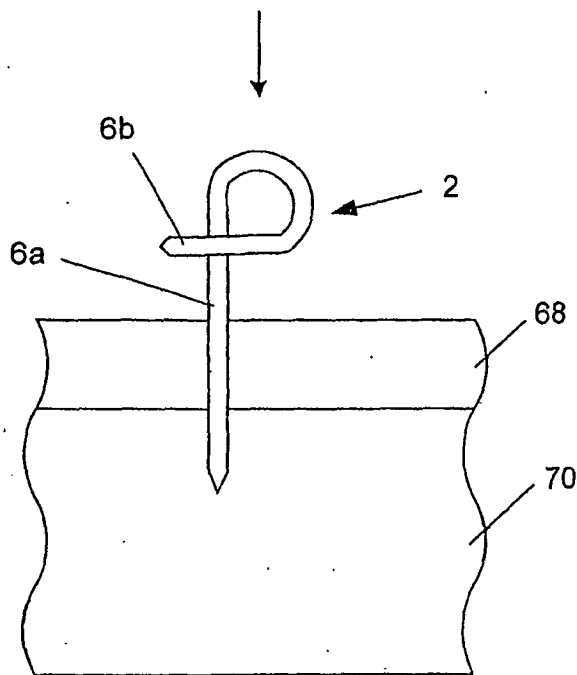


Fig. 34

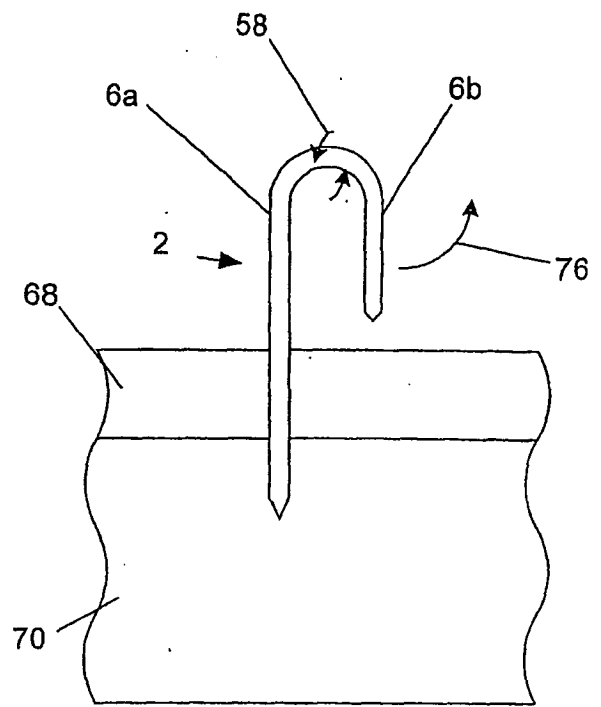


Fig. 35

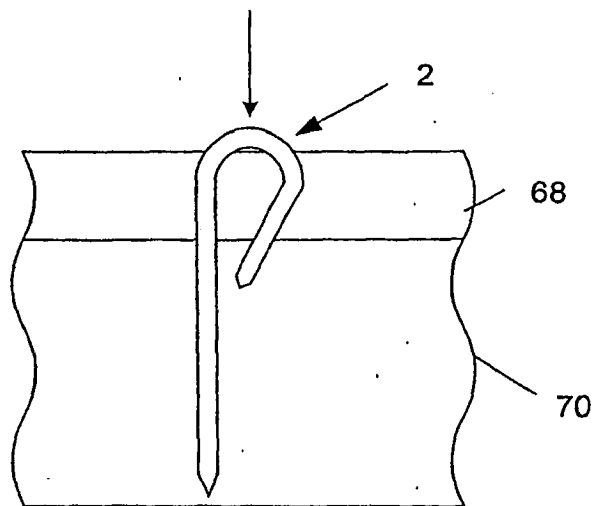


Fig. 36

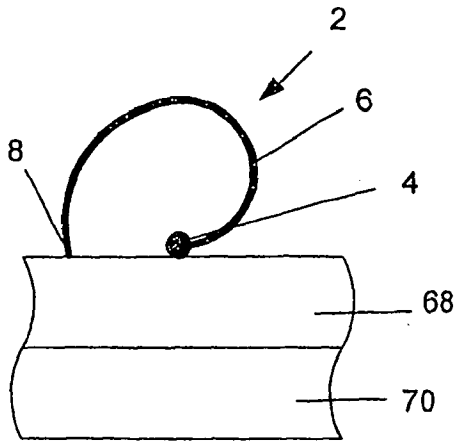


Fig. 37

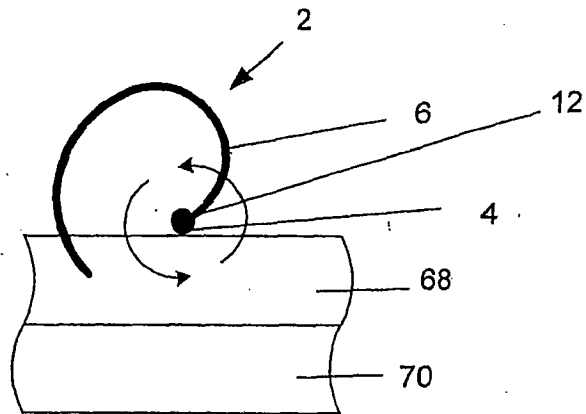


Fig. 38

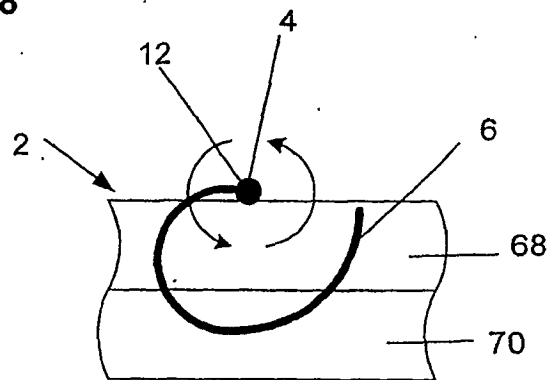


Fig. 39

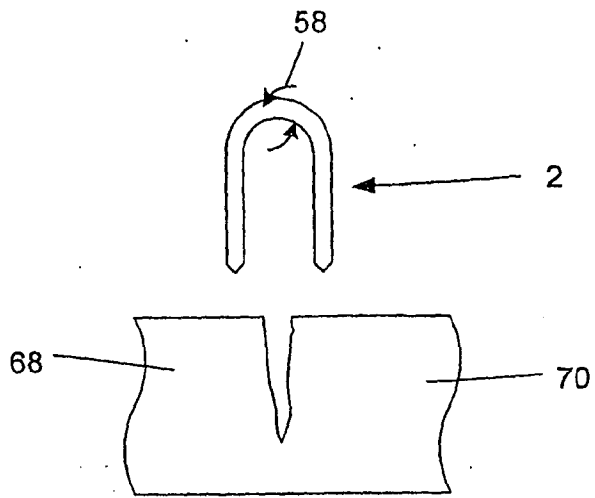


Fig. 40

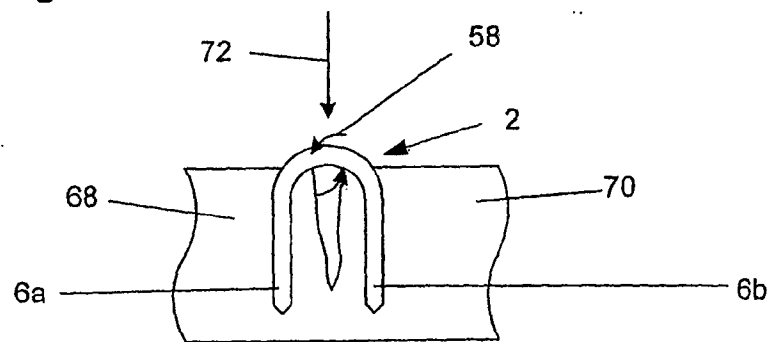


Fig. 41

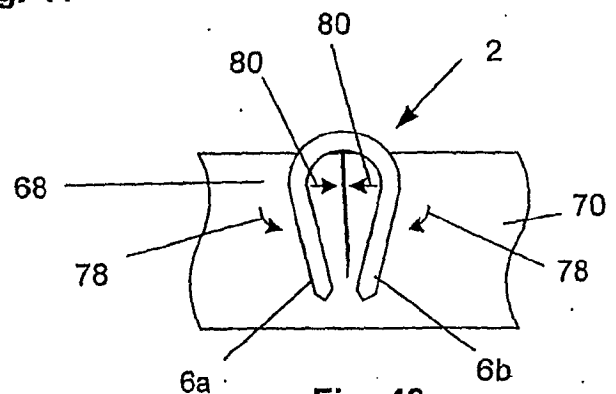


Fig. 42

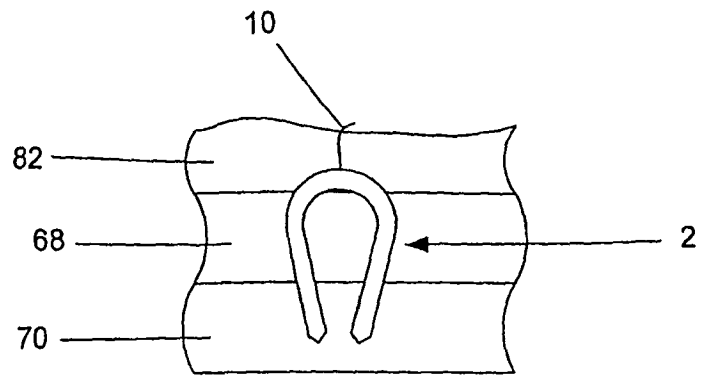


Fig. 43

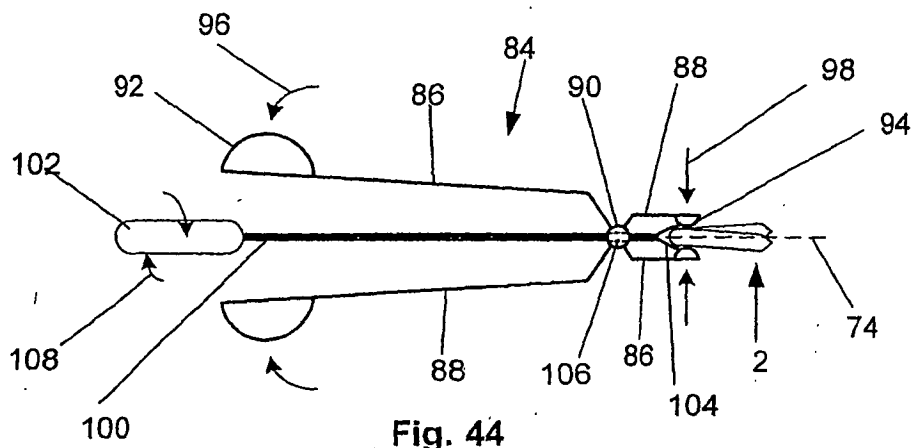


Fig. 44

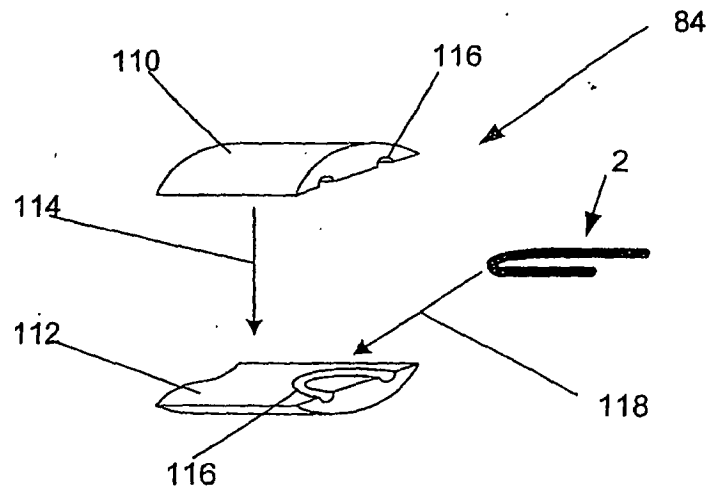


Fig. 45

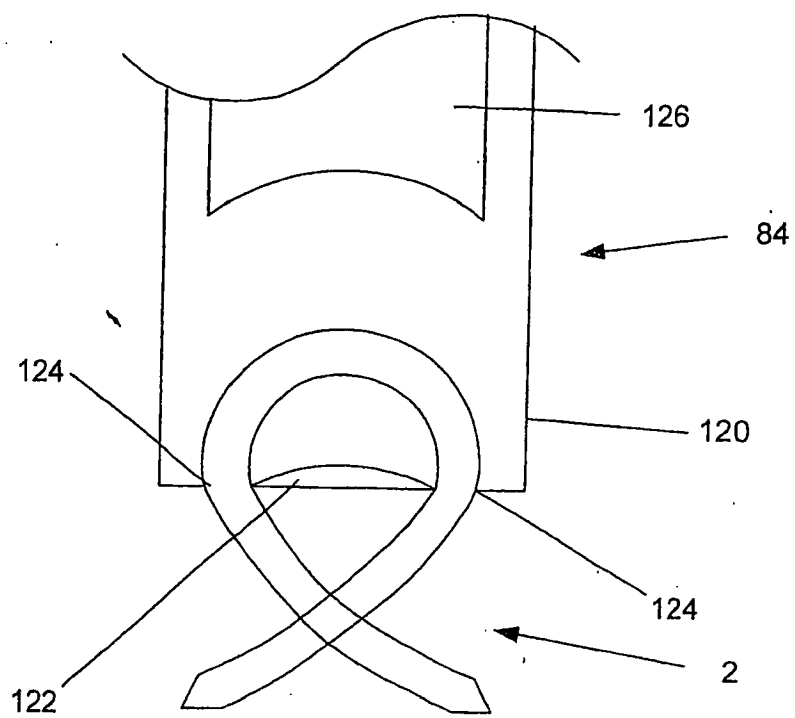


Fig. 46

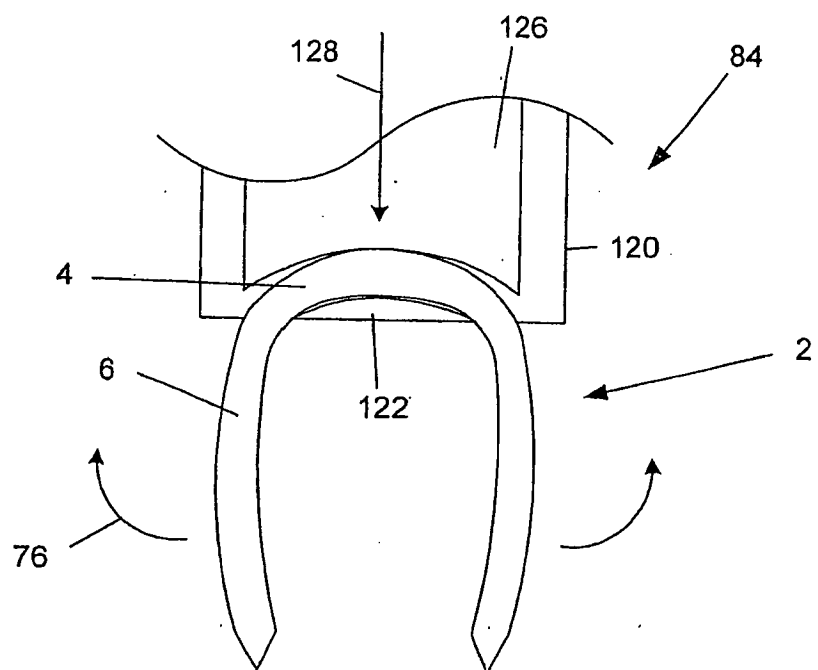


Fig. 47



EUROPEAN SEARCH REPORT

Application Number
EP 09 01 5108

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	WO 97/28745 A1 (HEARTPORT, INC.) 14 August 1997 (1997-08-14)	1,2	INV. A61B17/122
Y	* abstract; figures 12F,12G * * page 29, lines 3-37 *	3-13	
X	WO 03/053289 A (MILO) 3 July 2003 (2003-07-03)	14,15	
Y	* page 9, lines 13-31; figures 4,6a,6b *	3-9,13	
Y	EP 0 826 340 A2 (MEDINOV-AMP ET AL.) 4 March 1998 (1998-03-04)	10-12	
A	WO 97/39688 A2 (VNUS MEDICAL TECHNOLOGIES, INC.) 30 October 1997 (1997-10-30) * abstract; figures 2,3,19-29 * * page 11, lines 23-25 *	1,14	
A	US 5 984 949 A (LEVIN) 16 November 1999 (1999-11-16) * the whole document *	1,14	TECHNICAL FIELDS SEARCHED (IPC) A61B
The present search report has been drawn up for all claims			
Place of search The Hague		Date of completion of the search 4 May 2010	Examiner Giménez Burgos, R
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document</p>			

 3
EPO FORM 1503 03 82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 09 01 5108

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

04-05-2010

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9728745	A1	14-08-1997	AU 2265297 A	28-08-1997
			US 2003114867 A1	19-06-2003
			US 6254615 B1	03-07-2001
			US 2004073240 A1	15-04-2004
			US 2004172050 A1	02-09-2004
			US 2001021858 A1	13-09-2001

WO 03053289	A	03-07-2003	EP 1465555 A1	13-10-2004
			JP 4230915 B2	25-02-2009
			JP 2005523738 T	11-08-2005

EP 0826340	A2	04-03-1998	FR 2752720 A1	06-03-1998

WO 9739688	A2	30-10-1997	AU 2923997 A	12-11-1997
			US 6149660 A	21-11-2000

US 5984949	A	16-11-1999	NONE	

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 6358556 B, Ding [0048]
- US 6241765 B, Griffin [0055]
- US 6371983 B, Lane [0055]
- US 5976183 A, Ritz [0055]
- US 64663903 A [0055]
- US 32782102 A [0074]
- US 10646639 B [0074]

Non-patent literature cited in the description

- **Walton et al.** Inhibition of Prostaglandin E2 Synthesis in Abdominal Aortic Aneurysms. *Circulation*, 06 July 1999, 48-54 [0030]
- **Tambiah et al.** Provocation of Experimental Aortic Inflammation Mediators and Chlamydia Pneumoniae. *Brit. J. Surgery*, vol. 88 (7), 935-940 [0030]
- **Franklin et al.** Uptake of Tetracycline by Aortic Aneurysm Wall and Its Effect on Inflammation and Proteolysis. *Brit. J. Surgery*, vol. 86 (6), 771-775 [0030]
- **Xu et al.** Sp1 Increases Expression of Cyclooxygenase-2 in Hypoxic Vascular Endothelium. *J. Biological Chemistry*, vol. 275 (32), 24583-24589 [0030]
- **Pyo et al.** Targeted Gene Disruption of Matrix Metalloproteinase-9 (Gelatinase B) Suppresses Development of Experimental Abdominal Aortic Aneurysms. *J. Clinical Investigation*, vol. 105 (11), 1641-1649 [0030]

专利名称(译)	附件装置及其使用方法		
公开(公告)号	EP2196159A1	公开(公告)日	2010-06-16
申请号	EP2009015108	申请日	2004-10-06
[标]申请(专利权)人(译)	ARBOR手术TECH		
申请(专利权)人(译)	ARBOR外科技术, INC.		
当前申请(专利权)人(译)	ARBOR外科技术, INC.		
[标]发明人	DREWS MICHAEL J GURSKIS DONNELL W BACICH STEVEN R		
发明人	DREWS, MICHAEL J. GURSKIS, DONNELL, W. BACICH, STEVEN, R.		
IPC分类号	A61B17/122 A61B17/064 A61B17/068 A61B17/08 A61F2/24		
CPC分类号	A61B17/064 A61B17/0682 A61B17/083 A61B17/1227 A61B2017/0641 Y10S623/904 A61F2/2427		
代理机构(译)	ZIMMERMANN & PARTNER		
优先权	10/681700 2003-10-08 US PCT/US2004/033149 2004-10-06 WO		
其他公开文献	EP2196159B1		
外部链接	Espacenet		

摘要(译)

公开了用于附接第一质量和第二质量的装置及其制造和使用方法。该装置可由弹性、弹性或可变形材料制成。该装置可用于将心脏瓣膜环连接到生物环。该装置还可用于伤口闭合或各种其他手术，例如将假体固定到周围组织或其他假体，组织修复，例如关闭先天性缺陷，例如隔膜心脏缺损，组织或血管吻合，固定具有或不具有用于疝修复的增强网的组织，诸如骨融合或肌腱或肌肉修复中的矫形锚固，眼科适应症，腹腔镜或内窥镜组织修复或假体的放置，或机器人装置用于诸如上述执行的程序的组织远程

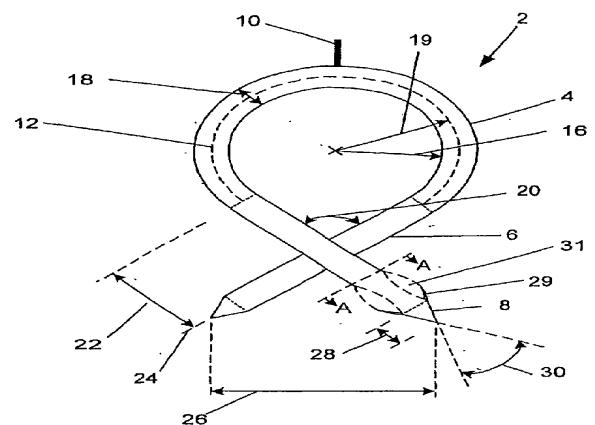


Fig. 1