

(19)



(11)

EP 2 417 925 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
07.12.2016 Bulletin 2016/49

(51) Int Cl.:
A61B 18/12 (2006.01) **A61B 34/00** (2016.01)
A61B 18/14 (2006.01)

(21) Application number: **11176993.1**

(22) Date of filing: **09.08.2011**

(54) Electrosurgical tool having tactile feedback

Elektrochirurgisches Werkzeug mit taktiler Rückmeldung

Outil électrochirurgical doté d'un retour d'informations tactiles

(84) Designated Contracting States:

**AL AT BE BG CH CY CZ DE DK EE ES FI FR GB
GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO
PL PT RO RS SE SI SK SM TR**

(30) Priority: **12.08.2010 US 373009 P**

(43) Date of publication of application:
15.02.2012 Bulletin 2012/07

(73) Proprietor: **Immersion Corporation
San Jose, CA 95134 (US)**

(72) Inventors:

• **Gregorio, Pedro
Verdun, QC H4H 2H6 (CA)**

• **Ullrich, Christopher J.
Ventura, CA 93003 (US)**

(74) Representative: **Hofstetter, Schurack & Partner
Patent- und Rechtsanwaltskanzlei
PartG mbB
Balanstrasse 57
81541 München (DE)**

(56) References cited:
**EP-A1- 1 254 637 EP-A1- 1 852 078
WO-A1-94/24949 WO-A1-2008/033937
US-A- 5 928 159**

EP 2 417 925 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description**FIELD OF THE INVENTION**

[0001] Embodiments hereof relate to surgical tools for treating tissue, wherein information related to the tissue treatment is processed and displayed to a user in one or more feedback modes integrated onto a handle of the tool

BACKGROUND OF THE INVENTION

[0002] As opposed to open surgery in which a surgeon cuts a relatively large incision in the skin of a patient for accessing internal organs, minimally invasive surgical procedures are performed by making relatively small incisions and then inserting tools through the incisions to access the organs. Minimally invasive surgery usually results in shorter hospitalization times, reduced therapy requirements, less pain, less scarring, and fewer complications.

[0003] Although minimally invasive surgical procedures involving small incisions include many advantages over open surgery, minimally invasive surgery can still create challenges to a surgeon. For example, the surgeon must typically rely on a miniature camera introduced through an incision to view the patient's internal organs and see how the movement and operation of the tools affects the organs. The camera transmits images to a visual display, allowing the surgeon to see the internal organs and tissues and to see the effect of other minimally invasive tools on the organs and tissues. In this way, the surgeon is able to perform laparoscopic surgery, dissection, cauterization, endoscopy, telesurgery, and the like.

[0004] Compared to open surgery, however, minimally invasive surgery presents limitations in visual and haptic perceptions, and creates challenges unique to this type of surgery. One of the major concerns is the potential for tissue damage, possibly caused by inappropriate use of force or excessive application of energy/heat. For example, electrosurgical tools operate by stimulating tissue with a high frequency electric current. The frequency of the current controls the action of the tool, which can include heating, ablating/cauterizing, sealing, and/or dissecting. In a minimally invasive procedure, surgeons must rely on experience and indirect visualization to determine when the tissue is dissected, sealed, ablated or when other changes have occurred in the tissue.

[0005] A surgical tool system according to the preamble of present claim 1 is known from the document WO 94/24949, for example. Further surgical tools are described in US 5 928 159, in EP 1 254 637 A1 as well as in WO 2008/033937 A1.

[0006] Based on the foregoing, it is an object of the invention to improve minimally invasive surgical tools and in particular, there is a need for minimally invasive surgical tools having improved feedback related to the surgical procedure.

[0007] According to the invention, this object is solved by the claims of patent claim 1.

BRIEF DESCRIPTION OF DRAWINGS

[0008] The foregoing and other features and advantages of the invention will be apparent from the following description of embodiments hereof as illustrated in the accompanying drawings. The accompanying drawings, which are incorporated herein and form a part of the specification, further serve to explain the principles of the invention and to enable a person skilled in the pertinent art to make and use the invention. The drawings are not to scale.

FIG. 1 is a diagram illustrating a side view of a surgical tool system including a laparoscopic surgical tool and an external control system according to an embodiment hereof.

FIG. 2 is a block diagram of the surgical tool system of FIG. 1.

FIG. 3 is a diagram illustrating a side view of a surgical tool system having haptic and audio feedback mechanisms, according to an embodiment hereof.

FIG. 4 is a diagram illustrating a side view of a surgical tool system having haptic, audio, and visual feedback mechanisms, according to another embodiment hereof.

DETAILED DESCRIPTION OF THE INVENTION

[0009] Specific embodiments of the present invention are now described with reference to the figures, wherein like reference numbers indicate identical or functionally similar elements. The terms "distal" and "proximal" are used in the following description with respect to a position or direction relative to the treating clinician. "Distal" or "distally" are a position distant from or in a direction away from the clinician. "Proximal" and "proximally" are a position near or in a direction toward the clinician.

[0010] The following detailed description is merely exemplary in nature and is not intended to limit the invention or the application and uses of the invention. Furthermore, there is no intention to be bound by any expressed or implied theory presented in the preceding technical field, background, brief summary or the following detailed description.

[0011] The invention is defined by the appended claims

[0012] Embodiments hereof relate to a surgical tool system 101 that includes a laparoscopic surgical tool 100 for heating, ablating/cauterizing, sealing, and/or dissecting tissue, a control system 112 for monitoring impedance of the tissue during treatment thereof, and a tactile feedback system 120 integrated into tool 100 that generates relevant feedback from control system 112 in at

least the form of haptic effects to the user. The tactile feedback provided by feedback system 120 alerts the tool user of changes in tissue properties, *i.e.*, when impedance of the tissue indicates that the treatment procedure is complete. In addition, as will be explained in more detail herein, the tactile feedback provided by feedback system 120 also supplies information relating to the operating status of control system 112 to the user.

[0013] FIG. 1 illustrates an embodiment of an exemplary surgical tool system 101. In this embodiment, surgical tool 100 is shown as a laparoscopic tool which is configured to be inserted through trocar or other minimally invasive access port. Surgical tool 100 includes a handle 102, a shaft 104, and a distal portion 106. Distal portion 106 includes a tip 108. As shown, tip 108 is a grasper or gripper. However, it should be understood that distal portion 106 may include any suitable type of tip having any suitable functionality. Laparoscopic tools in general, like tool 100, are typically thin instruments that each have varied functions (*e.g.*, grippers/graspers, scissors, clip appliers, hook cautery, etc.) and that can be introduced by the surgeon into the abdomen or other areas of the body through trocars, which are hollow tubes with a rubber seal to keep CO₂ from leaking. Shaft 104 is designed to connect handle 102 to distal portion 106 and to communicate mechanical actions of handle 102 to distal portion 106. More particularly, the motion of handle 102 opens and closes grasper tip 108 through an internal mechanical connector (not shown) that runs from handle 102 to grasper tip 108. According to some examples of the embodiment of FIG. 1, shaft 104 may be about 20 cm to 30 cm in length and tip 108 may be about 10 mm to 15 mm in length. In addition the shaft 104 is typically 5 mm in diameter, although tools with 3mm, 10mm and 12mm diameters are also commonly used. By manipulating handle 102, an operator can insert distal portion 106 into the abdomen of the patient and control tip 108 of distal portion 106.

[0014] Surgical tool 100 includes at least one electrical tissue contact element 110 coupled to and mechanically integrated with tip 108. Tissue contact element 110 is capable of applying heat supplied from a power source 114 of control system 112 to tissue. In one embodiment, tissue contact element 110 is a radiofrequency (RF) electrode for heating, ablating, sealing, and/or dissecting tissue and power source 114 is a radiofrequency (RF) generator. The RF electrode may have any suitable configuration capable of creating an ablative lesion within tissue, including but not limited to a flat electrode, a ring electrode, a hook electrode, or a dome-shaped electrode. Tissue contact element 110 may be coupled to the distal end of the grasper as shown in FIG. 1, to the bottom or outer surface of the grasper as shown in FIG. 3, to an interior surface within jaws of the grasper as shown in FIG. 4, or any other location on the grasper that is deemed appropriate. When distal portion 106 is inserted, the surgeon can manipulate handle 102 to control the location and orientation of tip 108 such that tissue contact element

110 is able to contact certain regions of the patient.

[0015] Embodiments hereof are described with respect to an electrosurgical tool having a radiofrequency (RF) electrode for heating, ablating, sealing, and/or dissecting tissue and a radiofrequency (RF) generator for supplying energy thereto. However, it should be understood by those of ordinary skill in the art that power source 114 may generate other types of energy for heating or ablating tissue including electrical energy, ultrasonic energy, cryoablation energy, etc., and in each case, tissue contact element 110 would be a suitable corresponding component to apply the type of energy to tissue. Further, when utilized in conjunction with alternative types of energy, control system 112 may monitor other suitable tissue, system, and/or operating properties rather than impedance to indicate when the treatment procedure is complete.

[0016] Surgical tool 100 further includes a common or indifferent reference electrode 111 that is separately disposed from tissue contact element or RF electrode 110. As shown, surgical tool 100 is a bipolar tool and a complete electrical circuit is formed between RF power source 114, electrodes 110 and 111, and the tissue extending between electrodes 110 and 111, with the tissue between electrodes 110 and 111 having an in-circuit impedance that may be monitored to indicate tissue changes as described in more detail herein.

[0017] Reference electrode 111 may be coupled to and mechanically integrated with tip 108 at a location spaced apart from RF electrode 110. However, as will be apparent to those of ordinary skill in the art, surgical tool 100 may be a monopolar tool in which the reference electrode is a skin patch electrode or grounding plate positionable outside the patient's body (not shown). In a monopolar embodiment, current and/or voltage flows from power source 114, through tissue contact electrode 110, and into the grounding plate or reference electrode exterior to the patient. As such, although tool 100 is illustrated with only one tissue contact element 110, it will be apparent to those of ordinary skill in the art that multiple tissue contact elements may be coupled to the distal end of tool 100. The same current and/or voltage flows through each tissue contact element and into the grounding plate or reference electrode 111 exterior to the patient.

[0018] Electrodes 110, 111 are electrically connected to control system 112 via two electrically conductive leads 113, 115, respectively, that extend through at least one lumen (not shown) of shaft 104. Electrodes 110, 111 may be fixedly attached to the distal ends of the two electrically conductive leads by any suitable means. For example, the electrodes may be attached via welding, soldering, by the use of an electrically conductive adhesive, by the addition of a connecting element there between, or by another mechanical method. Although shown with two leads 113, 115 extending through shaft 104, it will be understood by those of ordinary skill in the art that two leads are only required for bipolar tools having tissue

contact element 110 and reference electrode 111 integrated onto distal portion 106 of tool 100. Conversely in a monopolar tool, only one lead is required to run through shaft 104 for connecting control system 112 to one or more tissue contact elements, while an external lead or ground line is connected the grounding plate or reference electrode exterior to the patient.

[0019] FIG. 2 is a block diagram of surgical tool system 101, further illustrating the relationship between the main components of surgical tool system 101. More particularly, control system 112 includes power source 114, an impedance analyzer 116 for continuously measuring the electrical impedance between RF electrode 110 and reference electrode 111, and a controller or tactile mapping logic 118 configured to process impedance information from impedance analyzer 116 onto tactile feedback signals or commands. The tactile feedback signals are communicated from control system 112 to haptic feedback system 120 on handle 102 of tool 100. Lead 113 electrically connects power supply 114 and RF electrode 110 in order to supply RF power thereto, while lead 115 electrically connects impedance analyzer 116 and reference electrode 111 to communicate impedance measurements between electrodes 110, 111, which preferably include impedance measuring capabilities as will be described in more detail herein. A third lead or tether 117 electrically connects tactile mapping logic 118 to haptic feedback system 120 in handle 102 of tool 100 to control or actuate haptic effects thereto. A fourth lead (not shown) may also be provided between control system 112 and handle 102 to provide an isolated ground line for a low voltage actuator circuit located in handle 102, described in more detail herein.

[0020] In one embodiment, power source 114, impedance analyzer 116, and tactile mapping logic 118 are combined into an integral, external component that is separated from surgical tool 100 and is electrically connected to electrodes 110, 111 and haptic feedback system 120 via internal or external wires. Stated in another way, all of the components of control system 112 may be in the same external instrumentation unit. However, in another embodiment, power source 114, impedance analyzer 116, and/or tactile mapping logic 118 may be separate external components that are electrically connected together. In yet another embodiment, one or more of power source 114, impedance analyzer 116, and tactile mapping logic 118 may be mounted within or on handle 102 of surgical tool 100 and are electrically connected to electrodes 110, 111 and haptic feedback system 120 via only internal wires.

[0021] Power source 114 generates a current sufficient to heat, ablate, seal, and/or dissect tissue. The current is alternating current and may be of any suitable power level and frequency to heat, ablate, seal, and/or dissect tissue as desired. In one embodiment, power source 116 may be a RF power generator manufactured by Pfizer Valley Lab of Boulder, CO, which is capable of providing a high output power between 100 W - 200 W. For exam-

ple, power source 116 may generate 100 W at 50 kHz for ablation, although the frequency and power thereof may be varied during the procedure to allow for ablation, cautery, tissue specificity, etc. In addition, power source

5 114 generates a harmless electric current through lead 110 to allow for the measurement of impedance, as will be described in further detail below. The current is an alternating current (AC) and the selected alternating frequency may be in the range of 1 kHz to 500 kHz or other
10 suitable frequencies known to those of skill in the art of bioelectric impedance. For example, a current of 2 micro-
ampères at 50 KHz may be used.

[0022] Power source 114 and impedance analyzer 116 work together in order to continuously measure impedance 15 of the target tissue in real time. Real-time impedance measurement permits the user to gauge the completeness, *i.e.*, degree of transmurality, of the heat, ablation, sealing, or dissection treatment. Specifically, ablation aims to kill cells at an ablation site while leaving
20 the basic structure of the tissue intact and a transmural lesion that extends through the thickness of the tissue blocks electrical signals because it is nonconductive scar tissue. The ability of the lesion to block electrical signals may be accurately indicated by monitoring the impedance
25 of tissue, which can be measured simultaneously with the creation of the lesion. Accordingly, impedance may be monitored to indicate when ablation is complete and transmural. Monitoring impedance at or adjacent to the ablation site and determining completeness of the
30 treatment can be determined according to any criteria. For example, the detection of a particular value of electrical impedance is disclosed in U.S. Patent Nos. Pat. No. 5,540,681 to Struhal, et al.; the detection of a desired drop in electrical impedance at the electrode site as an
35 indicator of transmurality is disclosed in U.S. Pat. No. 5,562,721 to Marchlinski et al; the detection of an impedance rise or an impedance rise following an impedance fall are disclosed in U.S. Pat. No. 5,558,671 issued to Yates and U.S. Pat. No. 5,540,684 issued to Hassler; the
40 detection of a series of impedance measurements that are relatively constant over a desired period of time or over a defined number of successive impedance measurements or an abrupt rise in impedance as an indicator of transmurality is disclosed in U.S. Pat. Pub. No. 2005/0090815 to Francischelli et al..

[0023] As tool 100 heats, ablates, seals, or dissects tissue via tissue contact element 110, power source 114 generates an AC current between electrodes 110, 111 via two electrically conductive leads 113, 115 that extend
50 between control system 112 and electrodes 110, 111, respectively. While current is flowing, impedance analyzer 116 measures a corresponding resistance between electrodes 110, 111 via two electrically conductive leads 113, 115. Impedance analyzer 116 then arithmetically
55 converts the resistance to an impedance measurement. In order to measure impedance, impedance analyzer 116 may include logic resources, such as a microprocessor, configured to analyze and store impedance information

derived from electrodes 110, 111. For example, impedance analyzer 116 may include a voltage-current converting circuit, an amplifying circuit, an A/D converting circuit, and an impedance arithmetic operation section.

[0024] Impedance may thus be measured between the ablation electrodes or alternatively, between additional electrodes (not shown) located adjacent the ablation electrodes as described in U.S. Patent No. 5,558,671. In yet another embodiment, impedance may be measured between electrodes 110, 111 via impedance analyzer 116 built into the RF generator and in addition, secondary additional sensor(s) may be located adjacent the ablation electrodes for monitoring tissue properties during heating, ablating, sealing, and/or dissecting. Measurements from the secondary sensor(s) may be utilized to reinforce or supplant the impedance measurements produced by impedance analyzer 116.

[0025] Control system 112 further includes controller or tactile mapping logic 118 that processes the impedance information derived from electrodes 110, 111 according to specific algorithms and operator selections. Tactile mapping logic 118 may be a general-purpose or specific-purpose processing device or microcontroller. In one embodiment, tactile mapping logic 118 may be associated with a memory device (not shown) for storing data and/or instructions. The memory device can be any type of storage device or computer-readable medium, such as random access memory ("RAM") or read-only memory ("ROM"). The memory device stores logical instructions, commands, and/or code executed by tactile mapping logic 118. The memory device may also be located internal to control system 112, or any combination of internal and external memory. In another embodiment, logical instructions, commands, and/or code can be implemented in hardware and incorporated in tactile mapping logic 118 using discrete logic circuitry, an application specific integrated circuit ("ASIC"), a programmable gate array ("PGA"), a field programmable gate array ("FPGA"), etc., or any combination thereof. In yet another embodiment, logical instructions, commands, and/or code can be implemented in both hardware in tactile mapping logic 118 and software/firmware stored in the memory.

[0026] Tactile mapping logic 118 is configured to map sensed/calculated impedance values onto tactile feedback signals or commands. Mapping may include a function or lookup table, or may include a more complex algorithm and, if necessary, a finite state machine. Tactile mapping logic 118 determines what haptic effects are to be played and the order in which the effects are played in response to the sensed/calculated impedance values. Tactile mapping logic 118 outputs control signals to haptic feedback system 120 coupled to handle 102 to provide feedback information to an operator when performing a procedure. In general, high-level parameters that define a particular haptic effect include magnitude, frequency and duration. Low-level parameters such as pulse width modulation may also be used to determine a particular

haptic effect.

[0027] In one embodiment, the formation of a transmural lesion may be associated with an impedance change of 10 ohms. A corresponding lookup table may be represented as follows:

Impedance Change (ohm)	Haptic Amplitude (V)
0	0
2	0
4	0
6	1
8	2.5
10	5

[0028] The above example is of a straightforward and non-complex lookup or function table to map sensed/calculated impedance values onto tactile feedback signals or commands provides increasing feedback to the surgeon as the lesion forms. Other lookup functions are possible and may be user-selectable and/or may be utilized to communicate other types of information to the user in the form of haptic effects. The other types of information that may be communicated include operating parameters of control system 112, such as but not limited to the frequency or power settings in the RF generator, as will be described in more detail herein.

[0029] Haptic feedback system 120 includes at least an actuator drive circuit 122 (shown in FIG. 2) which is coupled to a haptic actuator 124 (also shown as FIG. 2) for providing haptic feedback to the operator. In order to provide feedback to the operator, haptic feedback system 120 is electrically connected to control system 112. In one embodiment, in order to communicate commands from tactile mapping logic 118 to haptic actuator 124, impedance analyzer 116 provides a motor voltage along lead or tether 117 to handle 102 of tool 100. As such, tactile mapping logic 118 outputs control signals to drive circuit 122 which includes electronic components and circuitry used to supply haptic actuator 124 with the required electrical current and voltage to cause the desired haptic effects. As mentioned above, a fourth lead (not shown) may also be provided between control system 112 and handle 102 to provide an isolated ground line for a drive circuit 122 in handle 102 such that tactile mapping logic 118 communicates with haptic feedback system 120 via an isolated DC voltage line having two conductors. In one embodiment, haptic actuator 124 is a vibrotactile device that generates vibrations on handle 102 for haptic feedback. Other types of haptic feedback may be generated and provided to the user, including kinesthetic feedback (e.g., active and resistive force feedback), handle deformation, and/or other types of tactile feedback such as texture and heat. As shown in FIG. 1, multiple haptic actuators may be incorporated in handle 102 at

several locations 119 for providing haptic effects to the fingers and thumb of a hand of the surgeon. Haptic actuators 124 may include electromagnetic motors, eccentric rotating mass ("ERM") actuators in which an eccentric mass is moved by a motor, linear resonant actuators ("LRAs") in which a mass attached to a spring is driven back and forth, shape memory alloys, electro-active polymers that deform in response to signals, mechanisms for changing stiffness, vibrotactile actuators, inertial actuators, piezoelectric actuators, or other suitable types of actuating devices. In one embodiment, haptic actuator 124 can be implemented as an inertial actuator to provide vibrotactile feedback to the operator. In another embodiment, kinesthetic haptic feedback may utilize, for example, solenoids to change the stiffness/damping of handle 102, small air bags that change size in handle 102, or shape changing materials. A detailed description of possibly haptic actuators suitable for use herein may be found in US 2009-0088659.

[0030] In one embodiment, tactile feedback system 120 alerts the tool user of changes in tissue properties, i.e., when the impedance of the tissue indicates that the treatment procedure is complete. For example, haptic effects provided by tactile feedback system 120 may include a vibrotactile alert when the tissue has reached a target or predetermined impedance value and/or a kinesthetic barrier on the trigger of handle 102 as the impedance approaches the target impedance value.

[0031] According to the invention, tactile feedback system 120 additionally supplies information relating to the operating status of control system 112 to the user. Haptic effects provided by tactile feedback system 120 provides information about the status of power source 114. The frequency and amplitude settings of the RF generator/power source 114 are mapped into a set of vibrotactile alerts to provide confirmation to the user that the generator is operating in a particular mode. As such, the surgeon would be able to "feel" that tool 100 is in the correct operating mode before engaging in electrosurgical activity.

[0032] In yet another embodiment, tactile mapping logic 118 may output command signals to power source 114. For example, when the impedance of the tissue indicates that ablation is complete, tactile mapping logic 118 may output a command signal to shut down power source 114, thereby preventing delivery of additional energy to the tissue and controlling the behavior of tool 100.

[0033] Referring to FIG. 3, an embodiment incorporating two types or modes of feedback for the operator is shown. Specifically, haptic feedback system 320 provides both haptic and audio feedback via haptic actuator 124 and an audio device or speaker 326. Tactile mapping logic 118 communicates the processed information to one or more of haptic actuator 124 and audio device 326 according to which ones of these feedback mechanisms are enabled and how they are controlled to provide their respective outputs.

[0034] In one embodiment, feedback may be provided

to the operator in a continuous manner as the operator performs the surgery. In another embodiment, feedback may be provided to the operator as an alert to notify or warn the operator when a particular condition is satisfied.

5 Further, one type of feedback may be provided in a continuous manner while another type of feedback is provided as an alert. For example, audio feedback may be provided to the operator in a continuous manner while haptic feedback is provided to the operator as an alert. Continuous 10 audio feedback may inform the operator of the distance of measured/calculated impedance values and a haptic alert may be generated when the measured/calculated impedance values indicate that ablation is complete and transmural.

15 **[0035]** Referring to FIG. 4, an embodiment incorporating three types or modes of feedback for the operator is shown. Specifically, haptic feedback system 420 provides haptic, audio, and visual feedback via haptic actuator 124, audio device or speaker 326, and visual display 428, respectively.

20 Tactile mapping logic 118 communicates the processed information to one or more of haptic actuator 124, audio device 326, visual display 428 according to which ones of these feedback mechanisms are enabled and how they are controlled to provide their 25 respective outputs.

In this embodiment, visual display 428 is a liquid crystal display (LCD) screen on a back region of handle 102. Visual display 428 may be used to display impedance information and/or the operating status of RF power source 114. In one embodiment, an ultrasound transducer (not shown) may be coupled to tip 108 of tool 100 and visual display 428 may be configured to show ultrasound image information to assist the surgeon to position the tool as needed. Visual display 428 can include a touch screen, which can be configured to 30 present information to the operator and can also be configured to sense when the operator presses certain portions of the touch screen. In this way, the touch screen can act as a touchable user interface with graphical presentation capabilities. Visual display 428 may include a 35 graphical user device that enables the surgeon to select different feedback profiles, adjust sensor behavior, modify supplemental information, and the like.

[0036] According to the embodiment of FIG. 4, handle portion 402 of surgical tool 400 may further include one 40 or more buttons 432. Buttons 432 can be configured using any suitable mechanism for allowing an operator to control the nature of the feedback that is provided to the operator. Buttons 432 may include devices for allowing certain levels, intensities, or amplitudes to be adjusted 45 or certain selections to be made regarding the output presented to the operator. In some embodiments, buttons 432 may be configured as switches, such as momentary toggle switches, allowing an operator to select different ways in which sensor information is mapped or 50 provided to respective output devices. Buttons 432 can be implemented as a rocker switch or as a one-dimensional control surface. According to one function of buttons 432, the operator can enable or disable one or more 55

output mechanisms by controlling whether or not output signals based on the sensed signals are provided to the respective output devices. Another function of buttons 432 includes the ability to enable one or more output mechanisms. In this regard, the operator can control if and how feedback is presented in a visual, auditory, and/or haptic fashion. With feedback tailored to the surgeon's preferences, the tool can provide feedback to supplement the operator experience for better operation and performance.

[0037] It will be apparent to those of ordinary skill in the art that embodiments hereof relate to any type of tools that can be manipulated by an operator. More particularly, the tools described in the present disclosure include a handle portion that mechanically controls a distal portion of the tool. According to embodiments hereof, a tissue contact element at a distal end of a device and a haptic feedback system may collectively function to extract impedance or pertinent information regarding the operating status of the control system that is subsequently communicated to the operator as haptic, audio, and/or visual feedback. Although embodiments disclosed are tools for laparoscopic surgery, other embodiments can be used for non-laparoscopic surgeries such as in vascular or other catheterization where information detected from a tissue contact element on the tool-tip can be communicated back to the catheter handle. Further, for endoscopy procedures, information detected from a tissue contact element on a flexible endoscope can be communicated back to the endoscope handle. Other embodiments can be used for telesurgery or telepresence in order to, for example, perform routine external examinations and/or utilize open surgical tools by a remote doctor.

[0038] While various embodiments according to the present invention have been described above, it should be understood that they have been presented by way of illustration and example only, and not limitation. It will be apparent to persons skilled in the relevant art that various changes in form and detail can be made therein without departing from the scope of the invention. Thus, the breadth and scope of the present invention should not be limited by any of the above-described exemplary embodiments, but should be defined only in accordance with the appended claims. It will also be understood that each feature of each embodiment discussed herein, and of each reference cited herein, can be used in combination with the features of any other embodiment.

Claims

1. A surgical tool system comprising:

a surgical tool (100) comprising a handle (102) and an electrical tissue contact element (110) operable to ablate tissue mounted on a distal portion (106) of the tool (100), wherein the distal portion (106) is connected to the handle (102)

via a shaft;

a power source (114) electrically connected to the tissue contact element (110);
an impedance analyzer (116) electrically connected to the tissue contact element (110), wherein the impedance analyzer (116) receives impedance measurement signals from the tissue contact element (110) and calculates tissue impedance;
a tactile mapping logic (118) electrically connected to the impedance analyzer (116), wherein the tactile mapping logic (118) receives calculated impedance information from the impedance analyzer (116) and processes the information into signal commands; and
a feedback system (120) including one or more haptic actuators (124) coupled to the handle (102) and electrically connected to the tactile mapping logic (118), wherein the tactile mapping logic (118) communicates the signal commands to the feedback system (120) and the feedback system (120) uses the signal commands to generate haptic feedback relating to the calculated impedance information to the handle (102),

characterized in that

the haptic feedback generated by the feedback system (120) additionally informs a user about operating parameters of the power source (114), wherein the operating parameters include at least one of a frequency setting and an amplitude setting of the power source (114) that are mapped into a set of vibrotactile alerts to provide confirmation to the user that the power source (114) is operating in a particular mode.

2. The surgical tool system of claim 1, wherein the haptic feedback generated by the feedback system (120) informs a user of the formation of a transmural lesion.

3. The surgical tool system of claim 2, wherein the formation of a transmural lesion may be associated with a tissue impedance change of approximately 10 ohms.

4. The surgical tool system of claim 2, wherein the feedback system (120) generates a vibrotactile or kinesthetic alert upon the formation of a transmural lesion.

5. The surgical tool system of claim 1, wherein the tactile mapping logic (118) further communicates signal commands to the power source (114).

6. The surgical tool system of claim 5, wherein the tactile mapping logic (118) outputs a command signal to shut down the power source (114) upon formation of a transmural lesion.

7. The surgical tool system of claim 1, wherein the feedback system (120) uses the signal commands to further generate audio or visual feedback relating to the calculated impedance information. 5

8. The surgical tool system of claim 1, wherein the feedback system (120) is operable to provide feedback in a continuous manner or wherein the feedback system is operable to provide feedback as an alert to notify the user when a particular condition is satisfied. 10

9. The surgical tool system of claim 1, wherein the tissue contact element (110) is a radiofrequency electrode and the power source (114) is a radiofrequency generator. 15

10. The surgical tool system of claim 1, wherein at least one of the power source (114), impedance analyzer (116), and tactile mapping logic (118) are mounted within or on the handle (102). 20

11. The surgical tool system of claim 1, wherein the tactile mapping logic (118) utilizes a lookup table to process the calculated impedance information into signal commands or wherein the tactile mapping logic utilizes an algorithm to process the calculated impedance information into signal commands. 25

12. The surgical tool system of claim 1, wherein the power source (114), impedance analyzer (116) and tactile mapping logic (118) are combined into an integral, external component that is separated from the surgical tool. 30

Patentansprüche

1. Chirurgisches Instrumentensystem, das umfasst:
 - ein chirurgisches Instrument (100) mit einem Griff (102) und einem elektrischen Gewebekontaktelement (110), das betriebsfähig ist, um Gewebe abzutragen, das an einem distalen Abschnitt (106) des Instruments (100) montiert ist, wobei der distale Abschnitt (106) mit dem Griff (102) über einen Schaft verbunden ist;
 - eine Leistungsquelle (114), die mit dem Gewebekontaktelement (110) elektrisch verbunden ist;
 - einen Impedanzanalysator (116), der mit dem Gewebekontaktelement (110) elektrisch verbunden ist, wobei der Impedanzanalysator (116) Impedanzmesssignale vom Gewebekontaktelement (110) empfängt und die Gewebeimpedanz berechnet;
 - eine taktile Abbildungslogik (118), die mit dem Impedanzanalysator (116) elektrisch verbun-

den ist, wobei die taktile Abbildungslogik (118) berechnete Impedanzinformationen vom Impedanzanalysator (116) empfängt und die Informationen in Signalbefehle verarbeitet; und ein Rückmeldungssystem (120) mit einem oder mehreren haptischen Aktuatoren (124), die mit dem Griff (102) gekoppelt sind und mit der taktilen Abbildungslogik (118) elektrisch verbunden sind, wobei die taktile Abbildungslogik (118) die Signalbefehle zum Rückmeldungssystem (120) übermittelt und das Rückmeldungssystem (120) die Signalbefehle verwendet, um die haptische Rückmeldung in Bezug auf die berechneten Impedanzinformationen für den Griff (102) zu erzeugen,
dadurch gekennzeichnet, dass
 die durch das Rückmeldungssystem (120) erzeugte haptische Rückmeldung zusätzlich einen Benutzer über Betriebsparameter der Leistungsquelle (114) informiert, wobei die Betriebsparameter mindestens eine von einer Frequenzeinstellung und einer Amplitudeneinstellung der Leistungsquelle (114) umfassen, die in einen Satz von vibrotaktilem Alarmen abgebildet werden, um eine Bestätigung zum Benutzer zu liefern, dass die Leistungsquelle (114) in einem speziellen Modus arbeitet.

2. Chirurgisches Instrumentensystem nach Anspruch 1, wobei die haptische Rückmeldung, die durch das Rückmeldungssystem (120) erzeugt wird, einen Benutzer über die Bildung einer transmuralen Läsion informiert.
3. Chirurgisches Instrumentensystem nach Anspruch 2, wobei die Bildung einer transmuralen Läsion einer Gewebeimpedanzänderung von ungefähr 10 Ohm zugeordnet werden kann.
4. Chirurgisches Instrumentensystem nach Anspruch 2, wobei das Rückmeldungssystem (120) einen vibrotaktilem oder kinästhetischen Alarm bei der Bildung einer transmuralen Läsion erzeugt.
5. Chirurgisches Instrumentensystem nach Anspruch 1, wobei die taktile Abbildungslogik (118) ferner Signalbefehle zur Leistungsquelle (114) übermittelt.
6. Chirurgisches Instrumentensystem nach Anspruch 5, wobei die taktile Abbildungslogik (118) ein Befehlssignal ausgibt, um die Leistungsquelle (114) bei der Bildung einer transmuralen Läsion abzuschalten.
7. Chirurgisches Instrumentensystem nach Anspruch 1, wobei das Rückmeldungssystem (120) die Signalbefehle verwendet, um ferner eine akustische oder visuelle Rückmeldung in Bezug auf die berech-

nenen Impedanzinformationen zu erzeugen.

8. Chirurgisches Instrumentensystem nach Anspruch 1, wobei das Rückmeldungssystem (120) betriebs-fähig ist, um eine Rückmeldung in einer kontinuierlichen Weise zu liefern, oder wobei das Rückmeldungssystem betriebsfähig ist, um eine Rückmeldung als Alarm zu liefern, um den Benutzer zu be-nachrichtigen, wenn eine spezielle Bedingung erfüllt ist. 5

9. Chirurgisches Instrumentensystem nach Anspruch 1, wobei das Gewebekontaktelement (110) eine Hochfrequenzelektrode ist und die Leistungsquelle (114) ein Hochfrequenzgenerator ist. 10 15

10. Chirurgisches Instrumentensystem nach Anspruch 1, wobei mindestens eines der Leistungsquelle (114), des Impedanzanalysators (116) und der tak-tilen Abbildungslogik (118) im oder am Griff (102) montiert ist. 20 25

11. Chirurgisches Instrumentensystem nach Anspruch 1, wobei die taktile Abbildungslogik (118) eine Nach-schlagetabelle verwendet, um die berechneten Im-pedanzinformationen in Signalbefehle zu verarbeiten, oder wobei die taktile Abbildungslogik einen Al-gorithmus verwendet, um die berechneten Impedanzinformationen in Signalbefehle zu verarbeiten. 30 35

12. Chirurgisches Instrumentensystem nach Anspruch 1, wobei die Leistungsquelle (114), der Impedanza-nalyse (116) und die taktile Abbildungslogik (118) zu einer integralen, externen Komponente kombi-niert sind, die vom chirurgischen Instrument getrennt ist. 40

Revendications

1. Système formant outil chirurgical, comprenant :

un outil chirurgical (100), comprenant une poi-gnée (102) et un élément de contact tissulaire électrique (110), utilisable pour enlever des tis-sus, monté sur une partie distale (106) de l'outil (100), dans lequel la partie distale (106) est re-liée à la poignée (102) par l'intermédiaire d'un axe ; 45

une source d'énergie (114), reliée électriquement à l'élément de contact tissulaire (110) ;

un analyseur d'impédance (116), relié électriquement à l'élément de contact tissulaire (110), dans lequel l'analyseur d'impédance (116) re-çoit des signaux de mesure d'impédance de l'élément de contact tissulaire (110) et calcule l'impédance des tissus ; 50

une logique de cartographie tactile (118), reliée

électriquement à l'analyseur d'impédance (116), dans lequel la logique de cartographie tactile (118) reçoit des informations sur l'impé-dance calculée provenant de l'analyseur d'im-pédance (116) et traite les informations en com-mandes de signaux et

un système de rétroaction (120), comportant un ou plusieurs actionneurs haptiques (124), cou-plés à la poignée (102) et reliés électriquement à la logique de cartographie tactile (118), dans lequel la logique de cartographie tactile (118) communique les commandes de signaux au système de rétroaction (120) et le système de rétroaction (120) utilise les commandes de si-gnaux pour générer une rétroaction haptique re-lative aux informations sur l'impédance calculée à la poignée (102),

caractérisé en ce que

la rétroaction haptique, générée par le système de rétroaction (120), informe, de plus, un utili-sateur sur les paramètres de service de la sour-ce d'énergie (114), dans laquelle les paramètres de service comportent au moins un réglage par-mi un réglage de fréquence et un réglage d'am-plitude de la source d'énergie (114), qui sont cartographiés en un ensemble d'alertes vibro-tactiles, pour apporter une confirmation à l'utili-sateur, suivant laquelle la source d'énergie (114) fonctionne dans un mode particulier.

2. Système formant outil chirurgical selon la revendi-cation 1, dans lequel la rétroaction haptique, générée par le système de rétroaction (120), informe un utilisateur de la formation d'une lésion transmurale. 40

3. Système formant outil chirurgical selon la revendi-cation 2, dans lequel la formation d'une lésion trans-murale peut être associée à un changement d'impé-dance tissulaire d'approximativement 10 ohms. 45

4. Système formant outil chirurgical selon la revendi-cation 2, dans lequel le système de rétroaction (120) génère une alerte vibrotactile ou kinesthésique lors de la formation d'une lésion transmurale. 50

5. Système formant outil chirurgical selon la revendi-cation 1, dans lequel la logique de cartographie tac-tile (118) communique en outre des commandes de signaux à la source d'énergie (114). 55

6. Système formant outil chirurgical selon la revendi-cation 5, dans lequel la logique de cartographie tac-tile (118) émet un signal de commande pour couper la source d'énergie (114) lors de la formation d'une lésion transmurale.

7. Système formant outil chirurgical selon la revendi-cation 1, dans lequel le système de rétroaction (120)

utilise les commandes de signaux pour générer en outre une rétroaction audio ou visuelle relative aux informations sur l'impédance calculée.


8. Système formant outil chirurgical selon la revendication 1, dans lequel le système de rétroaction (120) est utilisable pour fournir une rétroaction d'une manière continue ou dans lequel le système de rétroaction est utilisable pour fournir une rétroaction sous forme d'une alerte, pour avertir l'utilisateur lorsqu'une condition particulière est remplie. 5
9. Système formant outil chirurgical selon la revendication 1, dans lequel l'élément de contact tissulaire (110) est une électrode à radiofréquence et la source d'énergie (114) est un générateur de radiofréquence. 15
10. Système formant outil chirurgical selon la revendication 1, dans lequel au moins un élément parmi la source d'énergie (114), l'analyseur d'impédance (116) et la logique de cartographie tactile (118) est monté dans ou sur la poignée (102). 20
11. Système formant outil chirurgical selon la revendication 1, dans lequel la logique de cartographie tactile (118) utilise une table de conversion, pour traiter les informations sur l'impédance calculée en commandes de signaux ou dans lequel la logique de cartographie tactile utilise un algorithme pour traiter les informations sur l'impédance calculée en commandes de signaux. 25
12. Système formant outil chirurgical selon la revendication 1, dans lequel la source d'énergie (114), l'analyseur d'impédance (116) et la logique de cartographie tactile (118) sont combinés en un composant externe d'un seul tenant, qui est séparé de l'outil chirurgical. 35

40

45

50

55

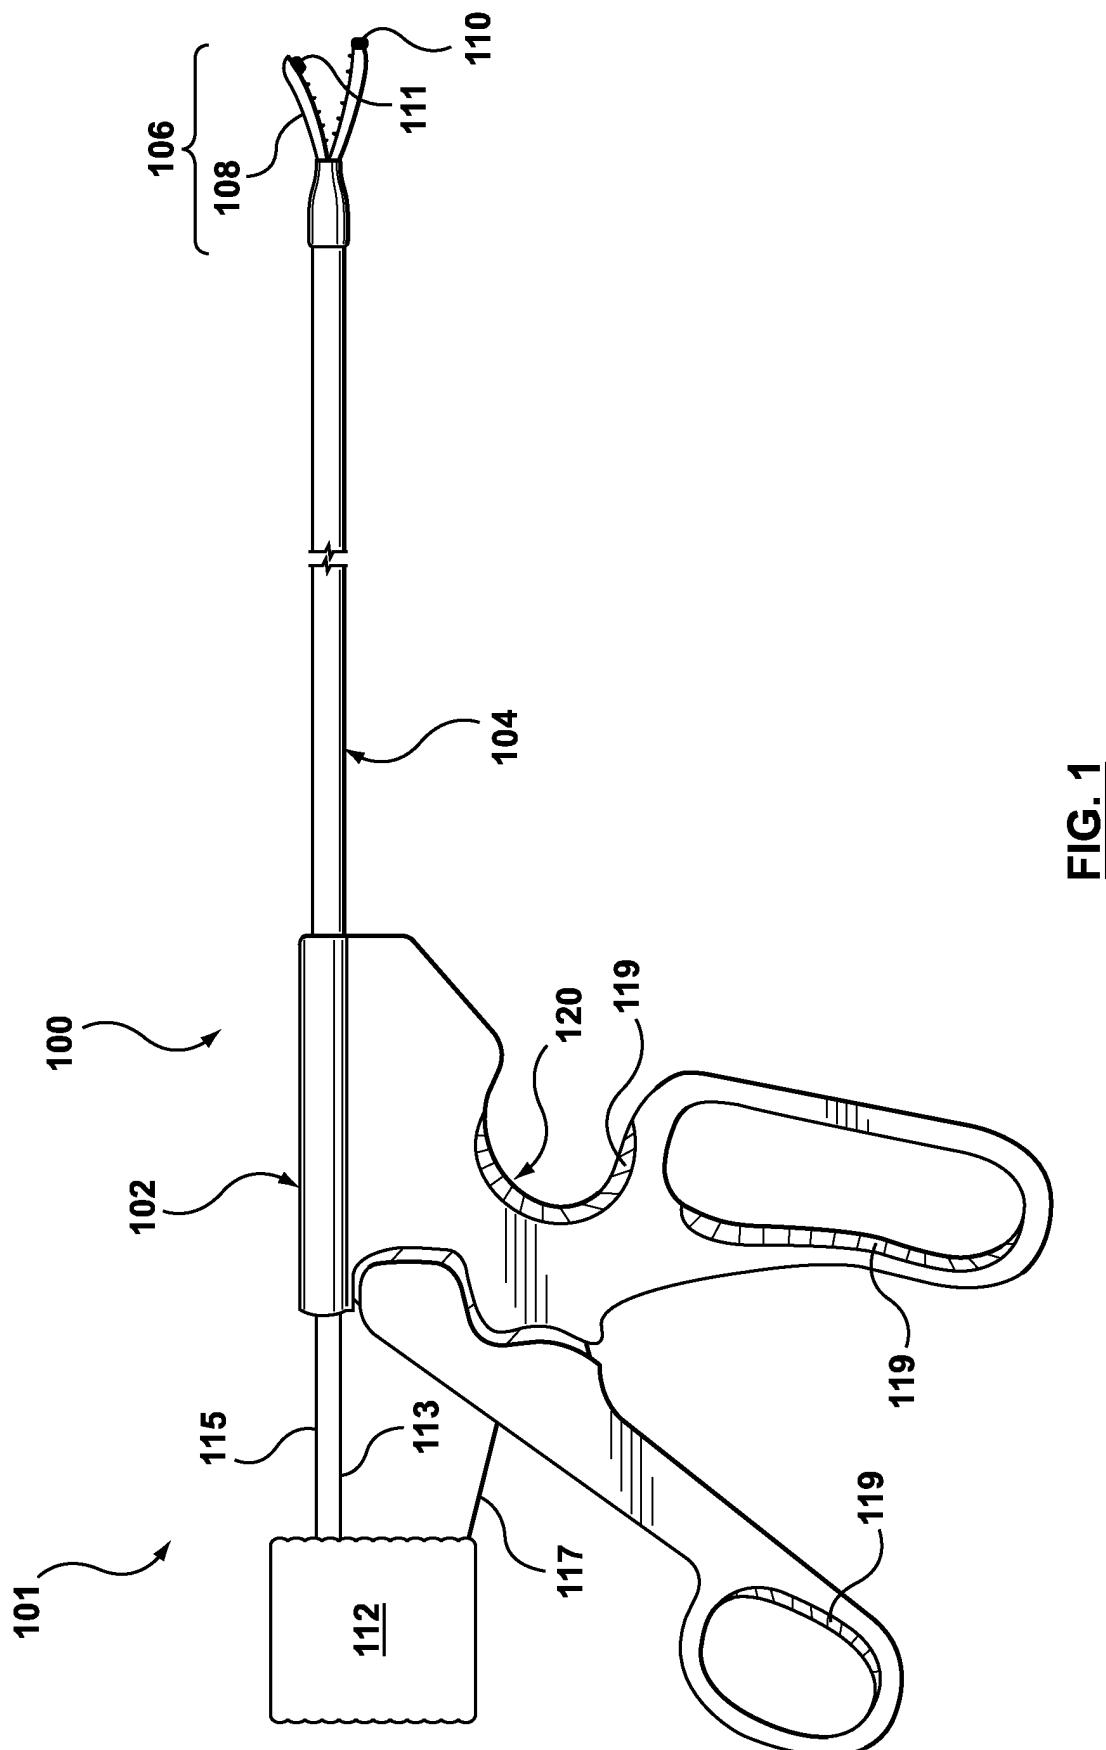

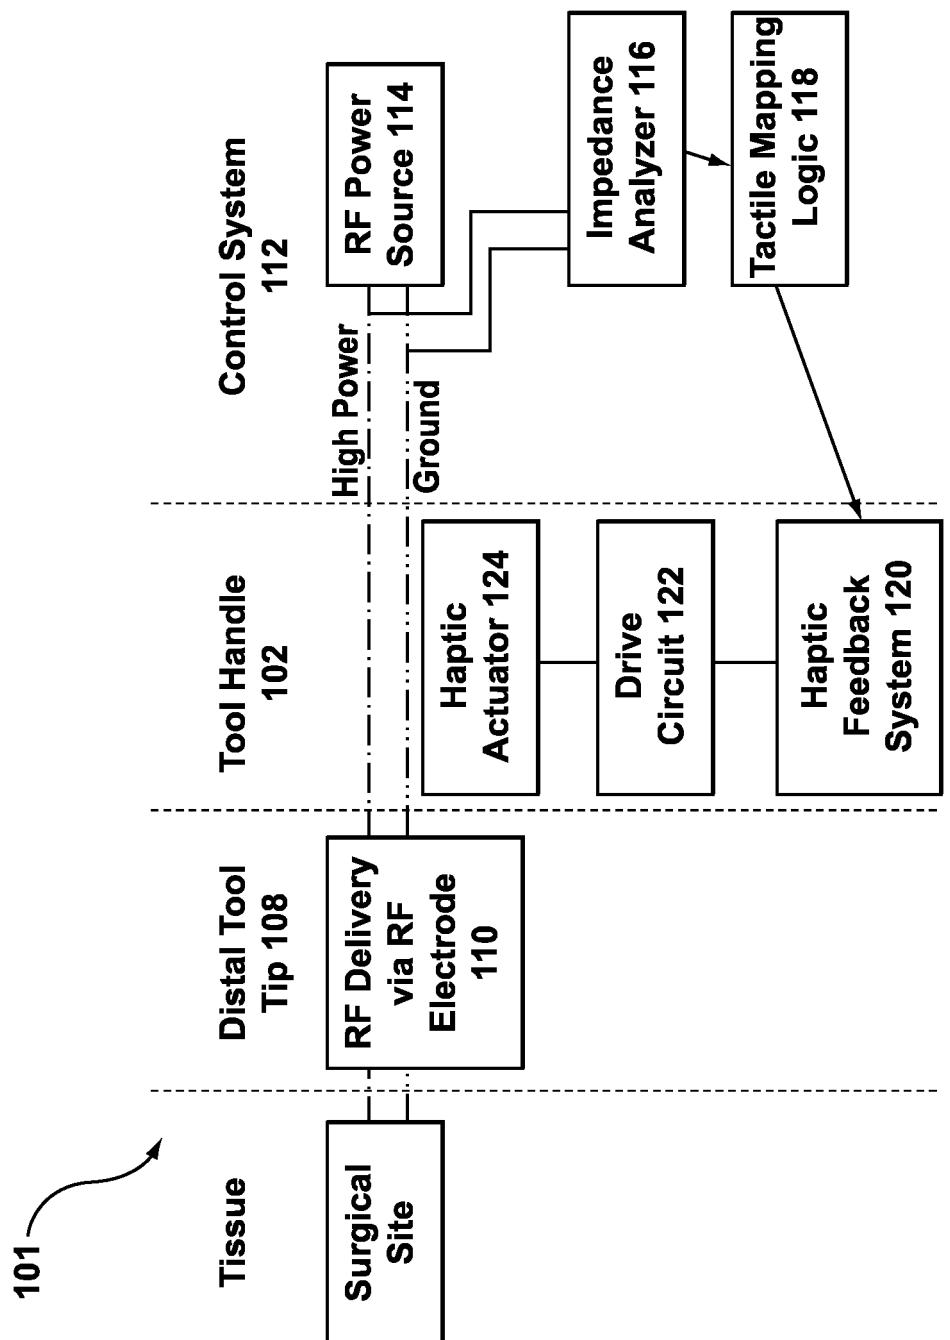


FIG. 2

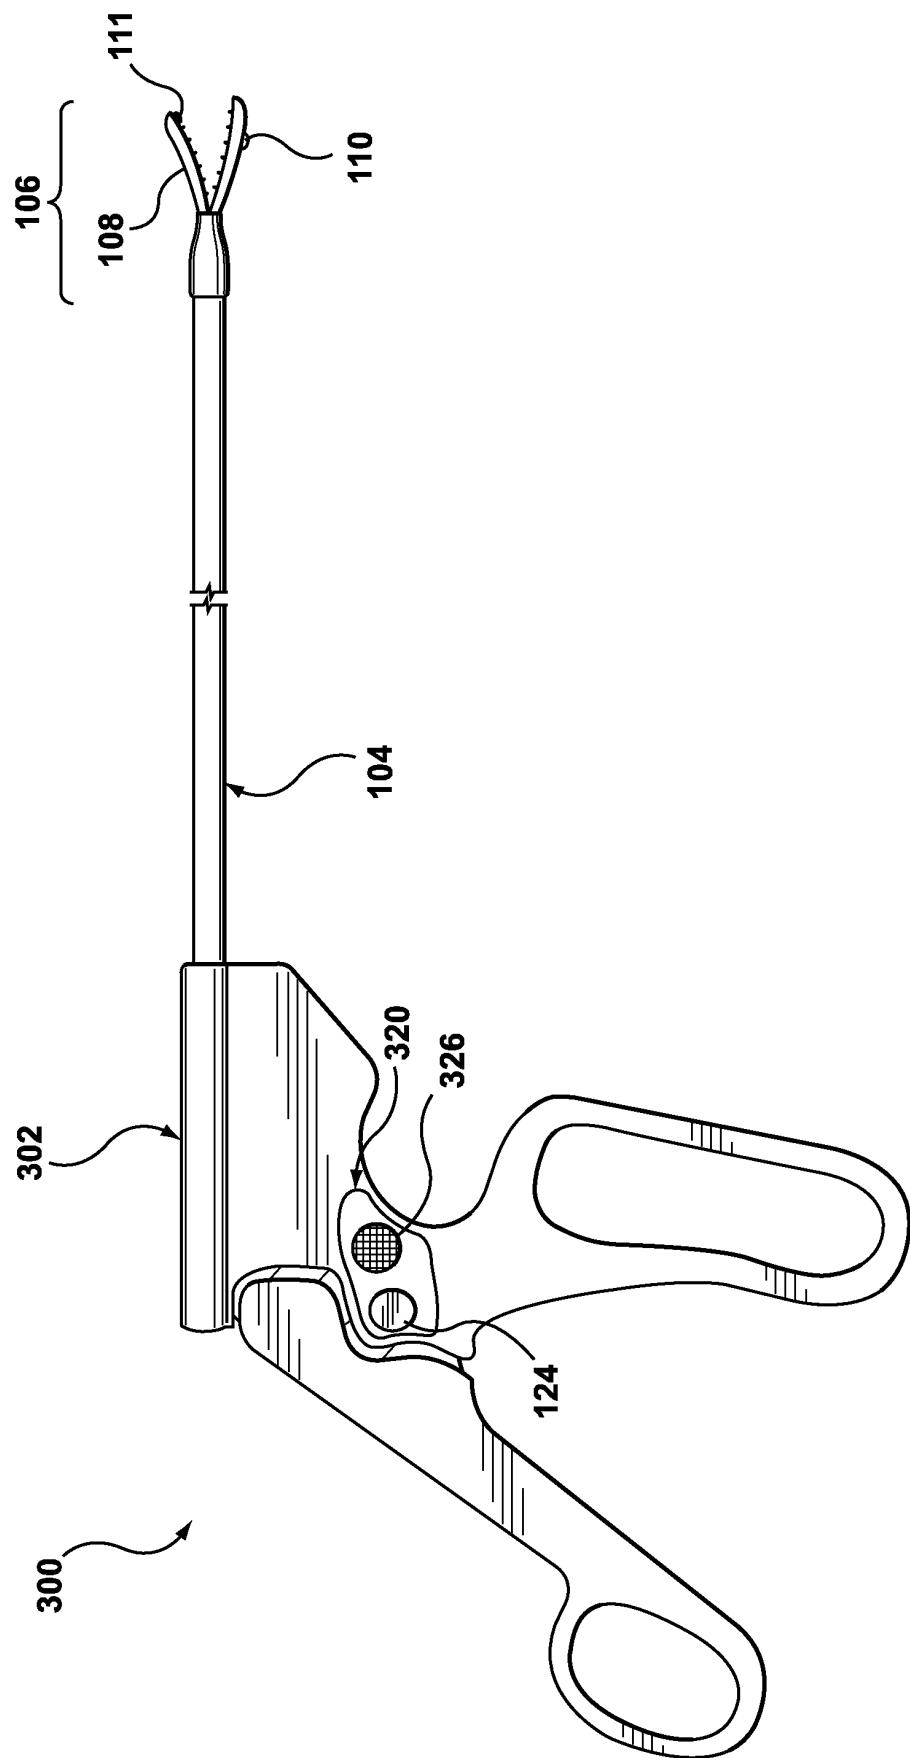


FIG. 3

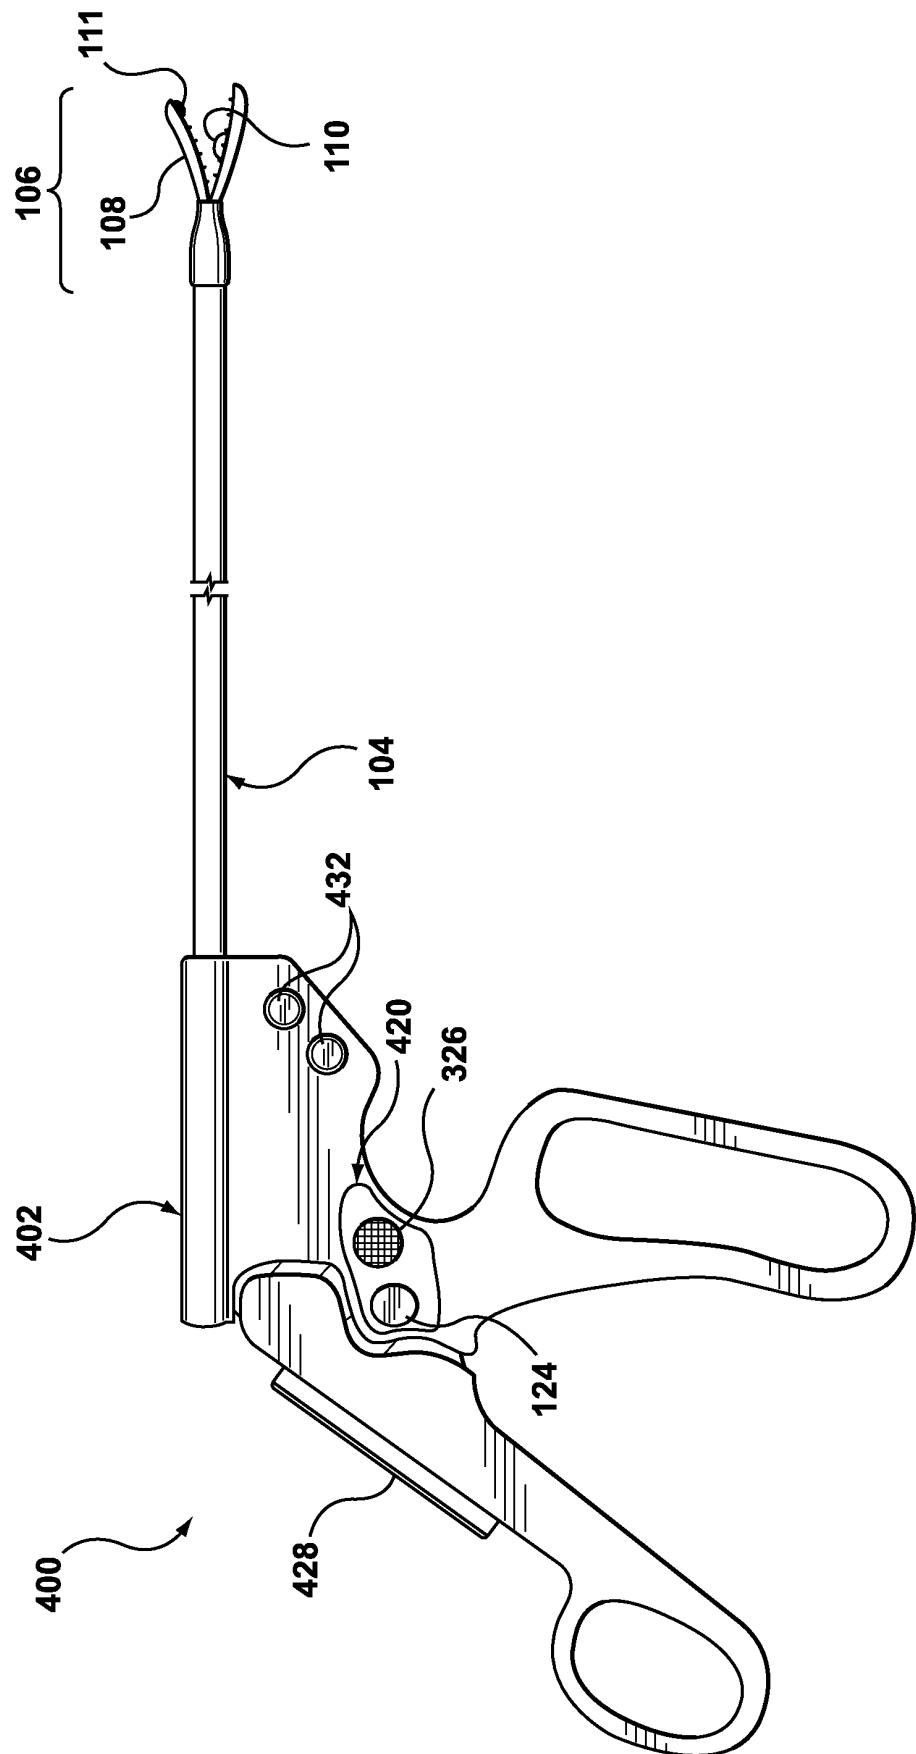


FIG. 4

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 9424949 A [0005]
- US 5928159 A [0005]
- EP 1254637 A1 [0005]
- WO 2008033937 A1 [0005]
- US 5540681 A, Struhi [0022]
- US 5562721 A, Marchlinski [0022]
- US 5558671 A, Yates [0022] [0024]
- US 5540684 A, Hassler [0022]
- US 20050090815 A, Francischelli [0022]
- US 20090088659 A [0029]

专利名称(译)	具有触觉反馈的电外科工具		
公开(公告)号	EP2417925B1	公开(公告)日	2016-12-07
申请号	EP2011176993	申请日	2011-08-09
[标]申请(专利权)人(译)	伊梅森公司		
申请(专利权)人(译)	Immersion公司		
当前申请(专利权)人(译)	Immersion公司		
[标]发明人	GREGORIO PEDRO ULLRICH CHRISTOPHER J		
发明人	GREGORIO, PEDRO ULLRICH, CHRISTOPHER J.		
IPC分类号	A61B18/12 A61B34/00 A61B18/14		
CPC分类号	A61B18/12 A61B18/1206 A61B18/1442 A61B34/76 A61B2018/00303 A61B2018/00684 A61B2018/00875		
优先权	61/373009 2010-08-12 US		
其他公开文献	EP2417925A1		
外部链接	Espacenet		

摘要(译)

外科手术工具系统，包括用于加热，消融，密封和/或解剖组织的腹腔镜外科手术工具，用于在组织的治疗过程中监视组织阻抗的控制系统，以及集成在工具手柄上的触觉反馈系统，其产生相关信息从控制系统以至少触觉效果的形式反馈给用户。触觉反馈提醒工具使用者组织性质的变化，即组织的阻抗指示治疗过程完成时。另外，所提供的触觉反馈可以向用户提供与控制系统的操作状态有关的信息。

