

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
6 October 2011 (06.10.2011)

(10) International Publication Number
WO 2011/123274 A1

(51) International Patent Classification:

A61B 17/22 (2006.01)

(72) Inventors; and

(75) Inventors/Applicants (for US only): **SHOHAT, Shaul** [IL/IL]; Hagiva 69, Kfar Oranim (IL). **TAMIR, Idan** [IL/IL]; Hashoftim 3, Zichron Ya'akov (IL). **KILEMNIK, Ido** [US/IL]; Nordau 35, Herzlia (IL).

(21) International Application Number:

PCT/US2011/029219

(74) Agents: **GOLLADAY, James E.** et al.; Kilpatrick Townsend & Stockton LLP, Two Embarcadero Center, 8th Floor, San Francisco, California 94111 (US).

(22) International Filing Date: 21 March 2011 (21.03.2011)

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:

61/319,931 1 April 2010 (01.04.2010) US

(71) Applicant (for all designated States except US): **XENOLITH MEDICAL LTD.** [IL/IL]; 1 Leshem St., 82000 Kiryat-Gat (IL).

[Continued on next page]

(54) Title: EXPANDABLE DEVICES AND METHODS OF USE

(57) **Abstract:** A sieving device and related methods including an expandable sieve mounted on a surgical guide wire. The expandable sieve may be a self-expandable braided filter which is mounted on the guide wire in an axially fixed position, or moveable in one or more directions. The sieving device is deployable in an obstructed ureter, or other body lumen, such as at the beginning of a stone removal procedure, prior to actual stone defragmentation (lithotripsy) phase. The expandable sieve may be set distal to the obstructive stone and expanded to span the entire local ureter cross section in order to retain stone fragments larger than a predetermined size from migrating distally towards the kidney under high irrigation rates/pressures during lithotripsy.

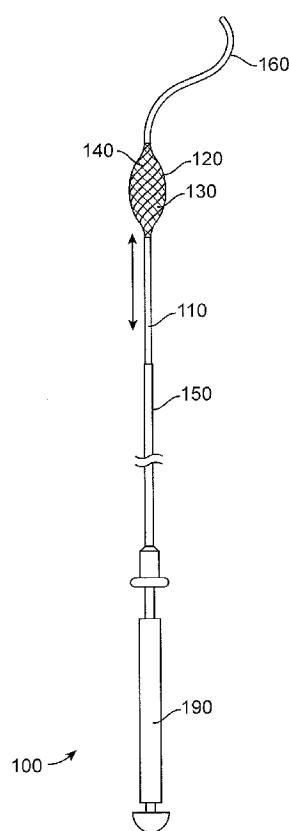


FIG. 1



ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) **Designated States** (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ,

TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

EXPANDABLE DEVICES AND METHODS OF USE

CROSS-REFERENCES TO RELATED APPLICATIONS

[0001] The present application claims the benefit under 35 U.S.C. §119(e) of provisional

5 application Ser. No. 61/319,931 filed April 1, 2010, the contents of which are hereby incorporated herein by reference in their entirety.

BACKGROUND OF THE INVENTION

[0002] Embodiments and methods of the invention may find applicability in the field of ureteral stone retention and retrieval, and other procedures and devices used for preventing or 10 diminishing the migration of harmful debris and other particulates in vessels of the body to organs, such as the kidney, during medical procedures such as, for example, endourological procedures and the like.

[0003] Calculi, stones and the like that are formed in body passages, such as in the ureter and

the kidneys are a common problem affecting between 5-7% of women and 10-12% men in

15 populations worldwide. These formations are usually caused due to increase in the concentration of urine salts resulting in their crystallization. Kidney stones smaller than 4mm are usually self-expelled, while larger ones tend to obstruct the ureter causing great pain and interfere with the passage of urine. The disease manifests itself in a wide spectrum of symptoms from asymptomatic to intense pain that occurs as a result of stone fragments making their way down 20 the urinary tract, recurring infections, and damage to the kidney, which can include reduced to complete loss of kidney function.

[0004] Until the 1980's, the common treatments for kidney stone removal involved painful and invasive procedures. Since then, kidney stone removal procedures have dramatically evolved to include Extracorporeal Shock Wave Lithotripsy (ESWL), a non-invasive procedure that uses

25 externally-applied shock waves to pulverize kidney stones, and ureteroscopy, a minimally-invasive endoscopic procedure that locates and removes kidney stones through their capture and/or pulverization by holmium laser energy (the latter is termed Intracorporeal Shock Wave Lithotripsy - ISWL).

[0005] When the obstructing stone is relatively large, the use of non-invasive techniques to disassemble the stone (e.g. ESWL) is less efficient, so the removal of larger stones typically involves the use of direct concentrated energy to fragment and disintegrate the stones. Such devices may use laser, ultrasonic, electro-shocks, or other fragmenting means. Holmium lasers 5 have been found to be particularly efficient in the field. Typically, the energy source is brought to the target location under endoscopic guidance using a ureteroscope.

[0006] A large percentage of ureteroscopic kidney stone removal procedures involve usage of stone baskets for stone capture and retrieval through the ureteroscope's working channel. In the past, stone baskets have been used to extract entire stones, but with the advent of lithotripsy the 10 use of such baskets has been reduced to extracting hard stones that proved refractory to disintegration by lithotripsy, and to collecting large stone fragments. In the latter case, the disadvantage is that the stone basket is introduced after kidney stone disintegration and, therefore, requires either the retrieval of the laser to allow its introduction, or the existence of an additional working channel in the ureteroscope. Clearly, the introduction of stone baskets after 15 stone fragmentation cannot prevent distal migration of fragments towards the kidney during the fragmentation procedure itself. This may be compounded by the use of high irrigation flow typically needed for ureteroscopic imaging.

[0007] These circumstances can lead to a cumbersome procedure that frequently fails in retrieving all stone fragments, resulting in translocation of the fragments up the ureter and, at 20 times, into the kidney. This commonly necessitates a longer and more aggressive procedure for the retrieval of such stone fragments by the endourologist, which many times results in increased damage to ureter walls and therefore to longer patient recovery time. This increased damage may also require stenting of the ureter, for example by a temporary double J-stent that prevents 25 ureter wall collapse post ureteroscopy. In such circumstances, an additional ureteroscopic post-operative procedure for the removal of these stents may be required.

[0008] Thus, the typical employment of a stone basket post-fragmentation can lead to a prolonged medical procedure, increased intrusiveness, and additional health risks for the patient. These factors result in extended required healing times, and may sometimes necessitate follow-up interventions for removing remaining stones.

[0009] Nonetheless, ureteroscopic procedures have gained wide acceptance and become the standard for kidney stone removal. In past years, some attempts have been made to introduce stone fragment capturing devices before and during lithotripsy and then optionally deploying them to remove the fragments from the ureter. These include devices such as the Stone Cone™
5 Retrieval Coil marketed by Boston Scientific and the NTrap® Stone Entrapment and Extraction Device marketed by Cook Medical. However, none of these devices allow continuous conformation to the narrowing ureter lumen along the extraction path, so fragments may still migrate. Furthermore, these devices may not be applicable for filtering fragments of different sizes, thereby potentially causing less efficient ureteroscopic visualization and irrigation
10 protocols. Additionally, current devices are not applicable for comprehensive filtering but, rather, are used for retaining relatively large stones for direct retrieval. For example, PercSys's Accordion ® and Pluromed's BackStop™ are examples of stone retrieval devices. The first is a Nitinol frame-supported fabric that obstructs the ureter, but is provided in discreet sizes (7 and 10mm) that restrict the ability to fully conform to the ureter's variable diameter. The second is
15 based on Pluromed's proprietary Rapid Transition Polymers™ (RTP™) that are liquid at low temperature and transition to gel at body temperature; the transition is reversible via cooling and the gel is completely dissolvable. The BackStop™ gel forms a plug above the stones in the ureter and prevents stone migration during fragmentation. After the stones are fragmented, the gel is dissolved with saline and exits the body.

20

BRIEF SUMMARY OF THE INVENTION

[0010] The invention provides systems and methods useful for removing obstructions and other debris from body lumen, such as, for example, a ureter and the like. Embodiments of the invention may include medical devices with an elongated support member, such as a wire, a
25 guide wire, throughwire, shaft, etc., and a sheath surrounding at least part of the support member or the like. In embodiments, the sheath may have an outer diameter of, for example, less than or equal to approximately 1.5 mm, or less than or equal to 1.0 mm and/or may be axially moveable in at least one direction along the support member.

[0011] One or more expandable sieves may be attached to the support member and contained
30 at least partially in the sheath. According to aspects of the invention, the expandable sieve may be configured to expand from a collapsed state to an expanded state that substantially conforms

to a transverse cross section of a body lumen. In embodiments, the expanded state may be conformable to a lumen having a diameter in the range of, for example, approximately 0.5 mm and 15 mm, or approximately 1.0 mm to 13 mm. In embodiments, the device may include at least two expandable sieves mounted to the support member that are configured to be expanded 5 independently from one another.

[0012] In embodiments, the expandable sieve may be configured to substantially prevent the passage of particles with a maximum diameter equal or greater than a predetermined size therethrough while in an expanded state, and to substantially allow the passage of particles with a maximum diameter less than the predetermined size while in the expanded state. For example, 10 the expandable sieve may be configured to substantially prevent passage of particles with a maximum diameter greater than, or equal to, 1.0 mm, and to substantially allow the passage of particles with a maximum diameter less than 1.0 mm therethrough. In other embodiments, the expandable sieve may be configured to substantially prevent passage of particles with a maximum diameter greater than, or equal to, 2.0 mm therethrough, and to substantially allow 15 passage of particles with a maximum diameter less than 2.0 mm therethrough. In embodiments, the expandable sieve may also be adjustably positionable along a length of the support member.

[0013] According to further aspects of the invention, the device may be configured to accommodate a stent, or other medical device, being deployed over a free end of the support member and/or past the expandable sieve. In embodiments, the device may be configured to 20 accommodate, for example, a ureteroscope working channel passing thereupon.

[0014] In embodiments, the expandable sieve may be configured to maintain a positioning of the expandable sieve along a length of the body lumen, while subjected to an irrigation flow, by only a radial force exerted by the expandable sieve on a wall of the body lumen while the expandable sieve is in the expanded state. In embodiments, the device may be configured to 25 substantially maintain a position of the expandable sieve against an irrigation flow in a range of, for example, approximately 10 ml/min to 1.0 liter/min, or approximately 50 ml/min to 100 ml/min, by only a radial force exerted by the expandable sieve on a wall of the body lumen while the expandable sieve is in the expanded state.

[0015] In embodiments, device may be configured to maintain a positioning of the expandable sieve along a length of the body lumen, while subjected to an irrigation flow in a range of, for 30

example, approximately 10 ml/min to 1 liter/min, by a radial force exerted by the expandable sieve on a wall of the body lumen, while the expandable sieve is in the expanded state, and a restraining force applied by the support member.

[0016] In embodiments, the sheath may be redeployable over the expandable sieve in the

5 expanded state to return the expandable sieve substantially back to the collapsed state. In embodiments, the expandable sieve may have a compressed diameter of, for example, approximately less than 1.0 mm. The expandable sieve may be configured to expand to an expanded state that is adjustable within a range of, for example, approximately 0.5 mm and 15 mm, or 1.0 mm to 13 mm.

10 **[0017]** According to further aspects of the invention, the expandable sieve maybe configured to maintain an opening size of less than a predetermined diameter, for example, less than 1.0 mm or less than 2.0 mm, throughout an expanded state range of approximately 0.5 mm and 15 mm, or 1.0 mm to 13 mm.

15 **[0018]** Embodiments may also include anchors of various configurations located at a distal end of the device.

[0019] According to further aspects of the invention, devices as described herein may be included in a medical system configured for fragmenting calcified aggregations, such as kidney stones and the like. Exemplary systems may be configured to interface with at least one of a ureteroscope, a fragmentation energy source, and an irrigation source.

20 **[0020]** According to further aspects of the invention, methods of removing an obstruction, calcified aggregations, and/or other debris from a body may employ devices as described herein and may include, for example, inserting an elongated support member, or the like, along with an expandable sieve into a body lumen, e.g. hollow or tubular organs such as but not limited to: urethra, urinary bladder, ureter, kidney pelvis, gastrointestinal tract, biliary ducts, gallbladder, 25 pancreatic ducts, blood vessels, upper respiratory tract or bronchi, salivary ducts, lacrimal ducts, articulations, bursa etc. Methods may include positioning the expandable sieve in a collapsed state distally of an obstruction, such as a kidney stone, or the like, and withdrawing a sheath to expand the expandable sieve from the collapsed state to an expanded state.

[0021] Embodiments may include fragmenting obstructions, calcified aggregations, and the like, such as by fragmentation means such as laser, electro-hydraulic, pneumatic, or ultrasonic lithotripter devices, etc.

[0022] Embodiments may include inducing a liquid flow in the body lumen and/or straining particulates with a diameter greater than an opening size of the expandable sieve from the liquid flow in the body lumen using the expandable sieve. Embodiments may include maintaining a positioning of the expandable sieve along a length of the body lumen during the straining and/or induced liquid flow by only a radial force exerted by the expandable sieve on a wall of the body lumen.

5 [0023] Embodiments may also include advancing the sheath to return the expandable sieve from the expanded state substantially back to the collapsed state.

[0024] Embodiments may include deploying a stent, or other surgical device, to a body lumen over the support member and/or the expandable sieve.

[0025] Additional features, advantages, and embodiments of the invention may be set forth or 15 apparent from consideration of the following detailed description, drawings, and claims.

Moreover, it is to be understood that both the foregoing summary of the invention and the following detailed description are exemplary and intended to provide further explanation without limiting the scope of the invention claimed. The detailed description and the specific examples, however, indicate only preferred embodiments of the invention. Various changes and 20 modifications within the spirit and scope of the invention will become apparent to those skilled in the art from this detailed description.

BRIEF DESCRIPTION OF THE DRAWINGS

[0026] The accompanying drawings, which are included to provide a further understanding of the invention, are incorporated in and constitute a part of this specification, illustrate 25 embodiments of the invention and together with the detailed description serve to explain the principles of the invention. No attempt is made to show structural details of the invention in more detail than may be necessary for a fundamental understanding of the invention and various ways in which it may be practiced. In the drawings:

[0027] FIGURE 1 is a schematic illustration of a first embodiment of an exemplary device with an expandable sieve constructed according to the principles of the invention.

[0028] FIGURE 2 depicts further details of the expandable sieve of Figure 1 in a compressed state.

5 [0029] FIGURE 3 depicts further details of the exemplary expandable sieve of Figure 2 in an expanded state.

[0030] FIGURE 4 depicts a schematic of an exemplary anchorless expandable sieve of the invention.

10 [0031] FIGURES 5A through 5C depict various embodiments of wire distal ends that may be employed as anchors for the expandable sieves of the invention.

[0032] FIGURE 6 depicts another embodiment of an exemplary device that may be used with an expandable sieve of the invention as shown in a ureter.

[0033] FIGURE 7 is a schematic illustration of an exemplary device of the invention with two expandable sieves.

15 [0034] FIGURE 8 is a schematic illustration with further details of an exemplary expandable sieve having a manual positioning and expanding device.

[0035] FIGURE 9 depicts another embodiment of an exemplary device of the invention shown in a ureter having a blockage.

20 [0036] FIGURE 10 depicts an exemplary device and expanded expandable sieve according to the invention as shown in a ureter having a blockage.

[0037] FIGURE 11 depicts a magnified view of an exemplary device of the invention along with an ureteroscope in proximity to a blockage undergoing fragmentation.

[0038] FIGURE 12 depicts an enlarged view of an exemplary sieve device of the invention that traps a fragment between the device and a vessel wall.

25 [0039] FIGURE 13 depicts use of another exemplary device of the invention in proximity to a blockage undergoing fragmentation.

[0040] FIGURE 14 depicts use of the other exemplary device of the invention with a sheath removed.

[0041] FIGURES 15A and 15B depict magnified views of the use of an exemplary device of the invention used for retrieval of fragments.

[0042] FIGURES 16A through 16C depict yet further details of various embodiments of expandable sieves having different shaped expanded states.

5 **[0043]** FIGURE 17 depicts yet another exemplary device of the invention, including an umbrella-shaped expandable sieve.

[0044] FIGURE 18 is a schematic of another exemplary device of the invention, including a detachable expandable sieve.

10 **[0045]** FIGURE 19 is a schematic of another exemplary device of the invention, having a deployable stent being inserted over the wire.

[0046] FIGURE 20 is a schematic illustration of restraining forces exerted by expandable sieves of the invention.

DETAILED DESCRIPTION OF THE INVENTION

[0047] It is understood that the invention is not limited to the particular methodology, 15 protocols, and reagents, etc., described herein, as these may vary as the skilled artisan will recognize. It is also to be understood that the terminology used herein is used for the purpose of describing particular embodiments only, and is not intended to limit the scope of the invention. It also is be noted that as used herein and in the appended claims, the singular forms "a," "an," 20 and "the" include the plural reference unless the context clearly dictates otherwise. Thus, for example, a reference to "a sieve" is a reference to one or more sieves and equivalents thereof known to those skilled in the art.

[0048] Unless defined otherwise, all technical and scientific terms used herein have the same meanings as commonly understood by one of ordinary skill in the art to which the invention pertains. The embodiments of the invention and the various features and advantageous details 25 thereof are explained more fully with reference to the non-limiting embodiments and examples that are described and/or illustrated in the accompanying drawings and detailed in the following description. It should be noted that the features illustrated in the drawings are not necessarily drawn to scale, and features of one embodiment may be employed with other embodiments as the skilled artisan would recognize, even if not explicitly stated herein. Descriptions of well-

known components and processing techniques may be omitted so as to not unnecessarily obscure the embodiments of the invention. The examples used herein are intended merely to facilitate an understanding of ways in which the invention may be practiced and to further enable those of skill in the art to practice the embodiments of the invention. Accordingly, the examples and 5 embodiments herein should not be construed as limiting the scope of the invention, which is defined solely by the appended claims and applicable law. Moreover, it is noted that like reference numerals reference similar parts throughout the several views of the drawings.

[0049] Moreover, provided immediately below is a “Definition” section, where certain terms relating to the invention are defined specifically. Particular methods, devices, and materials are 10 described, although any methods and materials similar or equivalent to those described herein can be used in the practice or testing of the invention. All references referred to herein are incorporated by reference herein in their entirety.

[0050] The terms “treating” and “treatment” as used herein refer to reduction in severity and/or frequency of symptoms, elimination of symptoms and/or underlying cause, prevention of the 15 occurrence of symptoms and/or their underlying cause, and improvement or remediation of damage.

[0051] The term “patient” as in treatment of “a patient” refers to a mammalian individual afflicted with or prone to a condition, disease or disorder as specified herein, and includes both humans and animals.

[0052] The term “sieve” as used herein refers to devices including webs, meshes, perforations, and other assorted combinations of material and openings, through which a liquid mixture including particles of various sizes may be passed to separate particles of a certain size from the liquid mixture. The term broadly includes various sifters, filters, and devices used for similar purposes, unless expressly distinguished. According to embodiments of the invention, particular 25 sieves may be configured to prevent the flow of relatively large and/or harmful particles, such as preventing large calcified particles and fragments from migrating to the kidneys, without accumulating masses of relatively smaller particles and debris that can lead to total occlusion of the filtered cross section. Particular sieves may be configured to allow a higher irrigation flow than conventional filters, which create a higher resistance to fluids passing therethrough. In 30 embodiments, exemplary sieves may be configured to retain particles of particular sizes, for

example, particles with a diameter in a range of approximately 0.5-2.0mm. According to aspects of the invention, designs may retain certain particles without leading to occlusion of a body lumen in which the sieve is positioned and allowing greater overall irrigation flow to be maintained.

5 [0053] The following preferred embodiments may be described in the context of exemplary ureteroscopic procedures for ease of description and understanding. However, the invention is not limited to the specifically described devices and methods, and may be adapted to various clinical applications without departing from the overall scope of the invention. For example, devices and related methods including concepts described herein may be used for preventing migration and

10 or removal of loose bodies, foreign bodies, or concretions such as but not limited to: calcifications, stones, thrombi, loose tissues, plaque fragments, emboli, bone fragments, in any hollow or tubular organs such as but not limited to: urethra, urinary bladder, ureter, kidney pelvis, gastrointestinal tract, biliary ducts, gallbladder, pancreatic ducts, blood vessels, upper respiratory tract or bronchi, salivary ducts, lacrimal ducts, articulations, bursa etc.

15 [0054] As shown in Figure 1, a first embodiment of the invention may include a device 100 having a shaft 110, which is connected toward the distal end 160 to an expandable sieve 120. In embodiments, the shaft 110 may be constructed from various materials, and may be configured, at least partially, as a flexible guide wire, and the like, that is conformable to the path of a vessel into which the guide wire is inserted. In embodiments, the expandable sieve 120, and the like, 20 may be fixed to a guide wire, such as shaft 110, or slideably mounted thereto for movement in one or both axial directions along the length of the shaft 110 as shown by arrow in Figure 1. The expandable sieve 120 is configured to expand to various diameters, e.g. in a range between 0.5 mm and 15 mm, and/or in a range between 1.0 mm and 13 mm, and may substantially conform to a transverse cross section of a body lumen in which the expandable sieve 120 is deployed, as 25 described further herein. Such expandability can be useful in numerous situations. For example, the transverse cross section of the ureter has deviations and changes of diameter along its length, and is also subject to substantial change due to illnesses. Therefore a conforming sieve element such as those described herein may be advantageously used in ureters that range in size, for example, among different patients, along a length of the ureter, and/or according to other 30 physiological circumstances such as illness etc.

[0055] As used herein, sieves that substantially conform to a lumen should be understood as those achieving a conformity that further substantially corresponds to an opening size of the sieve. For example, an expandable sieve with an opening size of 1.0 mm that substantially conforms to a lumen will be considered as also having a physical contour, which may be

5 irregularly shaped, presenting no openings between the lumen and the sieve with a minimum diameter greater than 1.0 mm. An opening size of the sieve (130) may be understood as a maximum diameter of openings in the sieve, including, for example, openings in meshed, braided, or porous materials of the sieve, that are configured to allow liquids, and particles smaller than the respective openings, to pass therethrough.

10 **[0056]** In embodiments, the expandable sieve 120 may be configured as a self-expandable mesh, that is selectively and/or frictionally positionable along a portion of the shaft 110. The portion of the shaft 110 within which the expandable sieve 120 may be positioned, may be bounded, for example by rings, detents, and the like, on the shaft 110. Such adjustability may be advantageous in selective positioning of the expandable sieve along the length of a vessel. In
15 embodiments, the expandable sieve 120 may be moved in the axial direction by various mechanisms, for example, a positioning wire, and/or a sheath, such as sheath 150 described below.

[0057] The device 100 also includes a sheath 150 that is mounted axially about the shaft 110. The sheath 150 may be moveable in the axial direction, and may be configured to at least
20 partially surround the expandable sieve 120. The sheath 150 may include a locking mechanism (not shown) that secures the sheath to the expandable sieve 120, and allows for positioning of the expandable sieve 120 in the axial direction. The sheath 150 may be released from engagement with the expandable sieve 120 to allow the sheath 150 to be withdrawn from the expandable sieve 120.

25 **[0058]** In embodiments, the proximal end of the shaft 110 may be releasably attached to a handle 190 for manipulating the device 100, adding additional devices over the proximal end of the shaft, etc.

[0059] As shown in Figure 2, the expandable sieve 120 may be contained in sheath 150 such that the sheath 150 maintains the expandable sieve 120 in a compressed state. Expandable sieve
30 120 may be expanded from a compressed state to an expanded state by various means. For

example, expandable sieve 120 may include, or be configured with, a self-expanding mechanism such as a self-expanding compressible weave and the like, or it may be expanded by an active mechanical mechanism, such as, for example, a pull wire or an internal balloon. The expandable sieve 120 may be manufactured of a braided mesh including various materials, and combinations 5 of materials, for example, biocompatible materials such as, but not limited to, Nitinol, Co-Cr alloy, stainless steel and/or other metallic or plastic materials. In embodiments, the expandable sieve 120 may be transitioned from the compressed state, e.g. shown in Figure 2, to a partially or fully expanded state by, for example, withdrawing the sheath 150 from the covering position around the expandable sieve 120. For example, as shown in Figure 2, the sheath 150 may be 10 moved in the direction indicated by direction 152 to expose the expandable sieve 120 and remove the restraining force of the sheath 150.

[0060] As discussed herein, the expandable sieve 120, and other embodiments of the invention, may include various shapes in compressed and/or expanded states. In some circumstances, an unconstrained shape will be described, which should be understood as the shape that the 15 particular component will assume in the absence of external force acting on the component. For example, the expandable sieve 120 may be configured such that, when released from the sheath 150, the sieve naturally assumes an unconstrained expandable shape that is substantially spherical. Other configurations are also contemplated.

[0061] For example, as shown in Figure 3, the expandable sieve 120 may assume a dome- 20 shaped configuration when the sheath 150 is fully withdrawn from the expandable sieve 120. Such configurations, in which the distal end of the expandable sieve includes the maximum unconstrained diameter, may be beneficial in better allowing the expandable sieve 120 to expand to a greater, and more effective, diameter when the sheath 150 is partially withdrawn. Expandable sieve 120 may be configured to assume various other unconstrained three- 25 dimensional and two-dimensional shapes, including but not limited to, cylindrical ellipsoid, pear shaped, egg shaped, conical, umbrella shaped, tear shaped, and/or circular, elliptical, triangular, etc. In embodiments, the unconstrained shape may have a radial symmetry that may be substantially preserved at various constrained diameters. Such designs may be advantageous, for example, in order to fit various ureteral diameters and geometries, and to substantially obliterate 30 the corresponding lumen with the expandable sieve by closely conforming to the lumen, and may

assist in preventing, for example, migration of stone fragments towards the kidney during stone fragmentation.

[0062] In embodiments, the expandable sieve 120 may be configured such that the length of the sieve in the collapsed or compressed state is between 50-200 mm, and the length of the sieve in the fully expanded state is between 30-70 mm. In embodiments, the expandable sieve 120 may be configured such that the diameter of the sieve in the collapsed or compressed state is between 0.5-1.0 mm, e.g. 0.9 mm, and the diameter of the sieve in a fully expanded state is between 7-20 mm, e.g. 15 mm. Individual wires of the sieve may be, for example, formed from a metallic, or other material having similar elastic modulus, with a wire diameter of

10 approximately 50-80 μ m. In embodiments, an expandable sieve, such as sieve 120, may include approximately 20-72 wires in a braided structure resulting in a suitable range of opening sizes and/or radial pressure when deployed in a body lumen. For example, embodiments may include expandable sieves with configurations that exert a radial pressure of approximately 85-1200 N/m² on a lumen wall when deployed.

15 **[0063]** As shown in Figure 3, the expandable sieve 120 may be provided with openings 130, the diameters of which may be configured in a range of, for example, 0.5mm to 2mm diameter in the expanded state. In embodiments, the openings 130 may be approximately 1mm in diameter in a partially to fully expanded state of the expandable sieve 120. In embodiments, the expandable sieve may be configured to substantially maintain a maximum diameter of the

20 openings 130 throughout an expanded state range, e.g. a maximum diameter of approximately 1mm throughout an expanded state range of 1.0 mm to 13 mm, without exceeding a maximal opening size or without deviating from an opening sizes range, such as 0.5 to 2 mm. In some situations, this could include a distribution of opening sizes, all less than the maximal opening size, along a sieve's longitudinal axis at a given state of expansion. However, more uniform

25 opening sizes may be achieved using other configurations, for example, by including multiple layers for the sieve, such as one layer that is woven so its openings change with expansion, and another layer that is porous, non-woven and/or non-elastic that may slide over the first layer without stretching or having fibers movable one with respect to the other. Thus, the openings 130 may be used to substantially prevent stone fragments of a predetermined minimal size and the

30 like to enter into, pass through, and/or to migrate distally to, the expandable sieve 120.

[0064] Alternatively, or in combination to the openings 130, the expandable sieve 120 may be provided with a permeable film 140 (see Fig. 1), for example, a liquid permeable film, which covers at least part of the expandable sieve 120, and which prevents stone fragments and the like from entering into, or migrating beyond, the covered portion of expandable sieve 120. An 5 expandable sieve including a permeable film may be used, for example, to reduce a flow of fluid to the kidney pelvis during ureteroscopy and, therefore, reduce the chance for fluid absorption and pain due to distension of the kidney pelvis. Such features may also be used to improve visibility at the stone site. In embodiments, a permeable film, such as film 140, and the like may be configured to be removable from the sieve, whereby the sieving device can be used to present 10 different filtering profiles at different times in the same expanded state. For example, a permeable film may have an opening size of 0.1mm, which may be advantageous for limiting the flow of smaller debris etc. at certain times such as the initial deployment of the device. The sieve may also have an expandable mesh or the like with a different maximum opening size, e.g. approximately 1mm. Therefore, after the permeable film is removed, the sieving device may 15 present an opening size that is, for example, an order of magnitude different than the opening size of the device when the permeable film is attached. Various ways of removing a permeable film and the like are contemplated, such as, connecting the film to a separate control wire that can be independently withdrawn along with the film.

[0065] The sheath 150 may be configured as a hollow tube with dimensions including, for 20 example, an outer diameter equal to or less than 1.5 mm, or, optionally, approximately 1.0 mm. In embodiments, the inner diameter of the sheath 150 may be in a range of 0.3 mm to 1.0 mm, e.g. approximately 0.9 mm, and may be sized according to the shaft 110 and/or a compressed diameter of the expandable sieve 120.

[0066] In embodiments, the sheath 150, or similar overtubes and the like, may be removable 25 from the device 100, such as by fully withdrawing the sheath 150 over the proximal end of the device. In further embodiments, the sheath 150 may also be reinstalled over the shaft 110, and/or the expandable sieve 120. As described further herein, such features may be advantageous, for example, in allowing the device 100 to assume a smaller profile within a ureteroscope and the like for a period of time during a procedure, and also allow for the re- 30 compression of the expandable sieve after other tasks, such as, for example, fragmentation and irrigation, are completed, and/or to reposition the expandable sieve.

[0067] In other embodiments, a sheath, or similar overtube, may be actuated by a separate pull chord, rather than being directly pulled upon. For example, a partial sheath, that extends only partly along a length of the device, may be remotely actuated, and, in embodiments with multiple expandable sieves, one or more sieves may have separate partial sheaths that can be individually actuated to allow for selective expansion of a particular expandable sieve.

[0068] The distal end 160 of the device 100 may take various forms, including, for example, a continuation of a guide wire or the like, extending through the expandable sieve 120, and/or a distal end of the expandable sieve 120 may be attached to a guide wire. In embodiments, guide wires, such as the distal end of the device 100, may include portions that are bendable and/or 10 twistable to form an expanded anchoring portion in a kidney opening.

[0069] As shown in Figure 4, the distal end of the expandable sieve 120 may terminate in a anchorless nub 170, or may be attached with various extensions, anchors and/or ends. For example, as shown in Figures 5A-5C, the device 100 may terminate with a tip, which may be tapered, flexible, floppy, semi-rigid, hydrophilic, etc. The tip may be pre-configured, and/or 15 dynamically shaped, at its distal end to the form of a pig tail 172, a U-shape 174, or an O-shape 176. Such distal ends of the device 100 and guide wire may serve as a retention means, or anchor, of the guide wire in, for example, the kidney pelvis, and prevent its dislodgement during procedures, such as stone fragment evacuation from the ureter, such as shown in Figure 6.

[0070] Figure 6 depicts aspects of an exemplary device 100 as may be used in a procedure 20 requiring insertion into a ureter 610, having lumen 612. As shown in Figure 6, the device 100 is configured to traverse the length of ureter 610 and to enter the kidney pelvis 620. The expandable sieve 120 is located at a position along the length of the ureter 610 within the lumen 612. The device 100 is shown with a distal end including helical shape 178 that may be inserted 25 in the kidney pelvis 610. Additionally, a portion 180 of the proximal end of the guide wire may be configured, such as in a helical pattern, to further prevent dislodgement of the distal end of the guide wire from the kidney pelvis during manipulation of the device. For example, by providing secondary restraining means, such as the helical portion 180, in the ureter, a reduction in force applied to the restraining means in the kidney pelvis, e.g. helical end 178, may be achieved. According to embodiments, sieving devices including expandable meshes and/or braids may also

be used to anchor the device in place with, or without, an additional anchor such as those shown in Figures 5A-5C and 6.

[0071] In embodiments, a device may be provided with more than one, e.g. two, expandable sieves. For example, as shown in Figure 7, a device may include expandable sieves 210 and 220, which may have similar characteristics to expandable sieve 120 depicted in Figures 1-3.

5 Expandable sieves 210 and 220 may be connected, for example, by a connecting filament 230 that may be, for example, straight, helical, or other shapes described herein. In embodiments, expandable sieves 210 and 220 may be separately expandable such that each of the expandable sieves 210 and 220 may be expanded at different times and/or amounts. For example, a sheath, 10 such as sheath 150 shown in Figure 1, may be configured to withdraw from one of the expandable sieves 210 and 220 first, and withdraw from the other of expandable sieves 210 and 220 afterwards. Such configurations may allow, for example, a clinician to position and secure the first expandable sieve at a desired location, and then position and secure the second expandable sieve, at a second desired location, which may be adjustable and/or different than the 15 length of connecting filament 230. More than two expandable sieves are also contemplated and may be achieved using similar methods. Also, one or more expandable sieves may be fixed, and one or more expandable sieves may be adjustable in an axial direction.

[0072] Embodiments may also include locking mechanisms whereby the expandable sieve, 20 such as expandable sieve 120 depicted in Figures 1-3, may be temporarily or permanently locked in an at least partially expanded state through manual means. For example, as shown in Figure 8, the expandable sieve 310 may be provided with a locking means, which may include an internal filament 320 connected to a distal end 330 of the expandable sieve 310. The internal filament 320 may be connected to the expandable sieve 310 from within and pass through a proximal orifice 340, or neck, of the expandable sieve 310. In this configuration, the proximal end 340 of 25 the expandable sieve 310 is fixed to the shaft and the distal end 330 generally moves in an axial direction as a diameter of the expandable sieve 310 is expanded or contracted. For example, as the diameter of the expandable sieve 310 is compressed, the length of expandable sieve 310 increases. Therefore, by fixing, or applying sufficient tension to, internal filament 320, the expandable sieve 310 is restrained, or locked, from returning to the compressed, or more slender, 30 configuration. In other embodiments, the internal filament 320, or the like, may be used as a

positioning rod to move an expandable sieve (which is mounted on the guide wire and moveable along the axial direction) in one or both axial directions.

[0073] In embodiments, a device of the invention, such as the device 100 depicted in Figure 1, may be configured for use in a working channel of a ureterscope. For example, components of

5 the device 100, e.g. sheath 150, shaft 110 and any components distal thereto, may be sized and configured to be inserted into a working channel of a ureterscope, and optionally controlled via controls of the ureterscope. In embodiments, and as discussed further herein, various other components may be used in combination with the disclosed devices and ureterscope, such as stents that may be positioned over the device before or after its insertion into a body lumen.

10 Accordingly, stents, and other devices may be deployed, for example, after the expandable sieve is returned to a compressed state, without removing the device from the body lumen. Further details regarding exemplary uses of the disclosed devices and methods are shown with reference to Figure 9.

[0074] As shown in Figure 9, a device 410 may be introduced through a ureteroscope 420

15 working channel, within the ureter 430. In the example shown in Figure 9, the device 410 is fed past an obstruction 440 in the ureter 430, such as a kidney stone, towards the kidney 450, which may be done, for example, under direct vision and/or fluoroscopy. An expandable sieve (not shown) may be held within the sheath 422 in a compressed state, whereby the expandable sieve may be positioned distal to the obstruction 440. Thus, the sieving device is deployable in an 20 obstructed ureter at the beginning of a stone removal procedure prior to actual stone defragmentation (lithotripsy) phase. As discussed previously, a distal end of the device 410 may be positioned in a kidney pelvis and include means for anchoring the device 410 in the kidney, such as curved, helical and other shaped bends and/or ends. Further details are shown in Figure 10-11.

25 **[0075]** After the device, and expandable sieve(s), are positioned properly, the outer sheath 422 may be retracted revealing a self expandable sieve 460 that, as shown in Figure 10, expands and occupies the ureter 430 above the obstruction 440. The self expandable sieve 460 may expand, for example, up to 30 times its collapsed deployable form (e.g., from about 0.5mm to about 15 mm in diameter) while exerting mild pressure/force onto the vessel, e.g. ureter, walls in various

30 diameters. One advantage of certain embodiments using a fully retractable and removable outer

sheath is that, after the sheath is withdrawn to allow the expandable sieve to manually or self-expand, the now thinner proximal part of the shaft by itself allows more room for irrigation, or other devices, to be run through the ureterscope working channel. Once the filter has been deployed, the clinician can apply irrigation at a higher flow rate, e.g. for improved endoscopic visibility, and the like, thereby allowing better control over the laser. Such irrigation may be applied through the ureterscope's working channel without introduction of other instruments through the ureter.

[0076] As shown in the expanded view in Figure 11, a portion of the guide wire proximal of the expandable sieve extends past the obstruction 440. An end of the ureterscope 420 includes 10 two working channels 424 and 426, although other ureterscopes may be used having one or more than two working channels. The device 410 is routed through working channel 426. In other embodiments, the device may be inserted side-by-side with a ureterscope.

[0077] A fragmentation energy source may be deployed through the same, or different, working channel of the ureterscope. Other actuating means, in addition to the sheath and self-expanding sieve, are also contemplated to expand various different expandable sieves described herein. In the position depicted in Figure 11, the obstruction 440, such as a kidney stone, may be fragmented by standard fragmentation means such as laser, electro-hydraulic, pneumatic or ultrasonic lithotripter devices used in combination with, or separately from, ureterscope 420.

[0078] For example, as also shown in Figure 11, a laser fiber 428 may be included in working 20 channel 424 and energized to promote fragmentation of the obstruction 440. Liquid may also be released into the ureter 430 via working channel 426 to promote washing away of the resulting fragments 490. Consequently, fragments 490 may be dislodged from the obstruction 440 and travel up the ureter toward the expanded expandable sieve 460. Thus, as described above, and as will be apparent to those understanding the concepts described throughout the specification, 25 embodiments may include replacing all, or a portion, of a working channel previously occupied by a sleeve, sheath and the like, with irrigation flow, suction flow, and/or additional tools or instruments, such as a fragmentation device and the like. As mentioned previously, devices according to the invention may also be used, instead, side-by-side with a ureterscope or other device deployed in the body lumen.

[0079] In alternative embodiments, an expandable sieve may be positioned to contact an obstruction (e.g. stone, stone fragment, clot, other solid or semi-solid particle), and to entrap the obstruction between a surface of the expandable sieve and a surface of the body lumen, for example, for the dual purposes of particle retention and subsequent fragmentation. As shown in

5 Figure 12, an expandable sieve, or trapping mechanism 510, may be positioned near obstruction 530. According to embodiments, the obstruction 530, and the like, may be trapped between an artificial surface and a biological surface, for example, surface 512 of the expandable trapping mechanism 510 and a surface 520 of the body lumen in which the trapping mechanism 510 is deployed. Accordingly, a fragmenting mechanism 540, such as a laser, electro-hydraulic, 10 pneumatic or ultrasonic lithotripter device, etc., may be positioned and applied to the obstruction 530, as well as other fragments that may develop and be subsequently trapped by the expandable trapping mechanism 510.

[0080] Other possible surfaces upon which obstructions and other particles may be trapped include, for example, biological surfaces including blood, ureter or other vessel walls, and 15 artificial surfaces including braids, meshes, etc. of the expandable sieves and trapping mechanisms described herein. In embodiments, the artificial surface may be a self expandable braid that exerts force against the biological surface, ensuring their apposition, which facilitates particle entrapment. The artificial surface may include a sieve having openings of a size of a specific pre-determined sizes range, allowing corresponding particle fragment migration through 20 it. For example, according to embodiments, the expandable trapping mechanism 510 may include a surface configured to substantially prevent passage of, and to apply a trapping pressure to, particles with a diameter greater than approximately 1.0 mm, or other therapeutically desirable size depending on the nature of the procedure, particle composition, affected vessel, and/or other relevant organs. Further details regarding exemplary sieving and trapping 25 techniques are described with reference to Figure 13.

[0081] As shown in Figure 13, stone fragments and the like of sizes greater than a predetermined value may be prevented from migrating towards the kidney 450 by the expanded expandable sieve 460 that is situated above the remains of fragments 440. Optionally, the sieve once expanded is configured to allow passage of fragments and particles of, for example, less 30 than 2mm, or optionally less than 1mm, therethrough. Optionally, such passage is only applicable under irrigation of minimal flow rate value. Expandable sieve 460 is shown within

the ureter and occupying its lumen. It should be understood that the expandable sieve 460 closely conforms to a transverse cross section of the lumen such that fragments are prevented from migrating beyond the expandable sieve 460 without passing through it. For example, the remains of obstruction 440, previously shown in Figure 11, must be reduced to an appropriate 5 size, e.g. approximately less than 1mm, in order to pass through the openings of expandable sieve 460. In embodiments, the expandable sieve 460, and the like, may be configured such that no gaps with a minimum diameter greater than 1mm are present between an outer contour of the expandable sieve and the transverse cross section of the body lumen.

[0082] In embodiments, devices according to aspects of the invention may be configured 10 and/or used to withdraw blockages, fragments, debris and the like, in addition to sieving. For example, a device, such as that shown in Figure 13, may be pulled by the shaft 410, filament 470, or other attached mechanism, and the expanded expandable sieve 460 will brush out fragments remaining in the ureter, or trapped in the expandable sieve. In embodiments, after fragmenting the stone to a desired degree, the expandable sieve, optionally together with the 15 ureteroscope, may be withdrawn. The sieve may then serve as a radially changeable wiper that wipes the large fragments towards direction of pull, e.g. toward the bladder, while adjusting and conforming to changes in the dimensions of the vessel, e.g. the narrowing ureter, as it travels distally. Thus, the device may be withdrawn with the fragments or other material, through the bladder, and ureteroscope or introducer sheath, to the bladder. In embodiments in which the 20 device is provided with a locking device including, for example, filament 470, the device may be pulled after tensioning and/or locking the locking device, which may be used to prevent the expandable means from resuming its more slender configuration. This may allow for a more forceful brushing out of the remaining stone fragments.

[0083] The handle 480 and the sheath 482 of the device, shown in Figure 13, may be removed 25 such that only the shaft 410, or other guide wire, that is connected to the expandable sieve 460, remains within the working channel of the ureteroscope 420, or within the introducer sheath. Thus, as shown in Figure 14, the device may be easily reduced to the shaft 410 and expandable sieve 460. The shaft 410 of the device may have a very small diameter, for example, between 0.5 mm and 0.01 mm, and preferentially, between 0.3 mm to 0.1 mm. Such dimensions may be 30 advantageous in leaving additional space within the working channel, for other instruments, irrigation, etc., and/or for deploying other medical devices, such as stents, over the device.

[0084] As previously discussed with respect to Figure 7, a device including more than one expandable sieves, e.g. expandable sieves 210 and 220, may also be used. Such devices may be introduced into the ureter, extending above the obstruction 440, as previously described. Both of expanding sieves 210 and 220 may be expanded to an at least partially expanded state, whereby

5 the ureter is occupied at a distal location, via expandable sieve 220, and a proximal location, via expandable sieve 210. The distal guide wire 160 may be introduced within the kidney pelvis of kidney 450, and serve as retention means for the device. As discussed previously, an obstruction 440 may be fragmented by various means, or the obstruction 440 may be trapped, captured, and/or withdrawn without fragmentation or other reduction techniques. For example, according

10 to embodiments, the obstruction may be fragmented, and the device may thereafter be pulled, such that the proximal expandable sieve 210 brushes out the ureter including substantially all fragments with a diameter larger than an opening size of the proximal expandable sieve 210. The distal expandable sieve 220 may remain within the ureter while the proximal expandable sieve 210 is withdrawn. Thus, the distal expandable sieve 220 may advantageously prevent

15 possible migration towards the kidney 450 of fragments or other debris that may escape the sweep by proximal expandable sieve 210, such as fragments that lodge in the vessel wall or are otherwise not collected by the expandable sieve due to irregularities and/or contortions in the vessel, etc. In embodiments, an opening size of the distal expandable sieve 220 may be different than an opening size of the proximal expandable sieve 210. For example, the distal expandable

20 sieve 220 may have a smaller opening size than that of the proximal expandable sieve 210, such as to allow for a relatively easier retraction of the proximal expandable sieve 210, while still maintaining a desired filtering size at the distal expandable sieve 220.

[0085] In embodiments, a sheath (not shown) may be individually advanced over the proximal expandable sieve 210, and the device pushed again within the ureter, for example, while the

25 distal expandable sieve 220 is still in an expanded state. The proximal expandable sieve 210 may then be re-exposed and expanded by withdrawing the sheath, and additional fragments may be brushed out and/or trapped for further fragmentation or other reduction. This procedure may be repeated as needed and may be particularly suitable in cases involving a large stone burden, or including multiple stones at different locations within the ureter.

30 [0086] According to yet other aspects of the invention, embodiments may include features and methods that allow for trapping particles while the device is inserted in the body lumen. For

example, as shown in Figures 15A-15B, an expandable filter 810 may include an optional stopping mechanism 812 that may be used to hold the expandable filter in a position along the length of guide wire 814 or to withdraw the expandable filter 810. It should be noted that, according to embodiments discussed further herein, a stopper 812, or the like, may not be

5 required to maintain a positioning of the sieving device, such as expandable filter 810, which may be configured to maintain its position using radial forces alone.

[0087] As shown in Figure 15A, a collection of fragments 820 have been trapped by expandable filter 810, and are being prevented from migrating toward the kidney. Turning to Figure 15B, a sleeve 830, such as an access sheath, may be introduced over the guide wire and 10 advanced in the lumen, and/or the expandable filter 810 withdrawn into the sleeve 830, such that the fragments 820 are substantially contained between the expandable filter 810 and the sleeve/access sheath 830. In embodiments, the opening of the sleeve 830 may be expandable and/or adjustable to closely approximate a transverse cross section of the lumen. Once the fragments 820 are substantially contained, the device can be withdrawn to remove the fragments, 15 or the area between the expandable filter 810 and the sleeve 830 can be flushed with irrigation and suction, via the ureteroscope 420, or the like, to remove the fragments. Although various exemplary embodiments are shown with a configuration including a sieve, such as a braid, being passed over a wire, other configurations are also contemplated, for example those in which the sieve attaches at one or more ends with a wire that does not pass through the sieve.

20 [0088] Expandable sieves in accordance with principles described herein may take various forms. For example, as shown in Figure 16A, the expandable sieves may have a substantially spherical configuration in an unconstrained expanded state, that adopts a cylindrical component along sidewalls when constrained in a body lumen. Other configurations may include a dome-shaped configuration in an unconstrained expanded state, which also adopts a cylindrical 25 component along sidewalls when constrained in a body lumen, as shown in Figure 16B. Embodiments may include a closed and convex shape at the proximal end and/or an opened, and optionally concave, shape at the distal end. As shown in Figure 16C, embodiments may include bell-shaped, and other configurations, in which a sieve portion has a contoured shape at its proximal end, which may be used to promote fragment accumulation in specific region(s), e.g. at 30 a sieve periphery, while allowing uninterrupted continuous irrigation flow through its center.

[0089] In embodiments depicted in Figure 17, the expandable filtering means 61 may be conically shaped. Configurations such as shown in Figure 17 may provide advantages, for example, when varying opening sizes are desired, such as larger openings in the distal end of the sieve. Such configurations may, for example, prevent debris accumulation within portions of the 5 braid that could interfere with stenting over the device. In the embodiment depicted in Figure 17, the tip 62 faces distally, e.g. towards the kidney, and the distal rim 63 of the expandable filtering means 61 is connected by one or more, and preferably 3, filaments 64. The shaft 65 may be attached from within to the tip of the expandable means. Such a configuration may be employed to act like an umbrella that can be expanded in a way that only requires a liquid flow 10 to pass through one surface of the sieve, rather than two surfaces such as in a spheroid, or other substantially enclosed-shaped, sieve

[0090] For example, in embodiments, to expand the expandable filtering means 61, the external sheath 66 may be retracted. The shaft 65 and/or filaments 64 may then be adjusted to control an expansion of the filtering means 61. In embodiments the external sheath 66 may be 15 removed during fragmentation of the stone. When the device is expanded within the ureter above the stone or stone fragments, it can capture them and permit their evacuation.

[0091] In another embodiment shown in Figure 18, an expandable device 71 may be detachable from shaft 72, via a securing mechanism 76. Securing mechanism 76 may be, for example, remotely actuated to detach the expandable device 71 from the shaft 72. In 20 embodiments, the expandable device 71 may be configured to be pushed out of an external sheath 73 by shaft 72, in order to, for example, allow the expandable device 71 to undergo a self-expansion to an expanded state. The expanded expandable device 71 may be retrieved by a standard grasper, and the like. Such embodiment may be desirable in order to, for example, prevent stone migration to cavities such as calyxes of the kidney during ureteroscopy and/or 25 percutaneous nephrolithotripsy.

[0092] In embodiments, exemplary devices may also serve as a guide wire for introducing and/or guiding intraluminal devices, such as a catheter, an imaging apparatus such as an ureteroscope, and/or a stent, to a position along the device, e.g. over the device to the kidney pelvis (using introduction techniques sometimes referred to as “over-the-wire” and “rapid 30 exchange”). As known in the art, a ureteral stent, or ureteric stent, may be configured as a thin

tube that is inserted into the ureter to prevent or treat obstruction of the urine flow from the kidney. The length of the stents used in adult patients may vary between 24 and 30 cm. Such stents, and the like, may be used according to aspects of the invention, for example, as shown in Figure 19. Embodiments may include configurations in which the device may be readied to 5 accommodate a stent, or the like, such as by removing handles and/or other large-diameter portions of the device, leaving a free end of the device to receive a stent, such as D-J stent 910, over the sheath and/or shaft of the device. Stent 910 may be a hollow tube with a diameter and gauge sized according to the patient's ureter and/or condition.

[0093] After being placed over the free end of the device, the stent 910 may be guided to a 10 desired position, such as the renal pelvis. In embodiments, the stent may be advanced by the use of, for example, a push tube (not shown), such as a plastic tube that is advanced along the wire and pushes the stent into place. In certain embodiments, a sheath of the device may be removed and the stent advanced over the shaft of the device, including over the expandable sieve 120, and over the distal guide wire 160. In alternative embodiments, the sheath, such as sheath 150 shown 15 in Figure 3 may be advanced over the expandable sieve 120 to re-collapse the expandable sieve 120 before advancing the stent 910 over the sheath 150 and expandable sieve 120.

[0094] Thus, according to aspects of the invention, a device may be used, first, to prevent 20 migration of potentially harmful fragments and the like, and, second, to act as a guide for placement of a stent, such as a ureteral stent. By providing a device that can accomplish both of these functions, trauma to the patient may be reduced by minimizing the number of separate 25 devices that need to be inserted and withdrawn from the patient, while also reducing the overall time associated with these procedures as well as the number of ureteroscope entries into the ureter. This type of dual use may be particularly beneficial in procedures such as kidney stone removal and ureteral stent insertion, which may be required together. For example, ureteral stents may be used to ensure the patency of a ureter that has been compromised by a kidney 2010 stone. In other situations, it may become necessary to place a stent in the ureter if the ureter has been irritated or scratched during stone fragmentation and/or removal.

[0095] As depicted schematically in Figure 20, in embodiments a static friction force "f" may 30 be applied to a throughwire 2010, such as the guide wire, passing through the expandable sieve 2010 to provide a resistive force and maintain the position of the expandable sieve in the lumen

against a flow 2030 containing debris 2040. The expandable sieve 2020 may also be held in place by applying a combined force $F+f$, wherein “F” is the radial force $F(r)$ applied by the expandable sieve and “f” is the static force f applied by the throughwire 2010. In other embodiments, the sieving device may be configured to substantially maintain its position, and to 5 resist a combined pressure from the flow and debris, through the force $F(r)$ only. That is, the device may be configured to substantially maintain a position during operation without a restraining force f being applied by a throughwire or the like.

[0096] According to embodiments, the expandable sieve 2020 may be held in place, by $F(r)$ only, $F+f$, or f only, while countering a debris containing irrigation flow 2030 at various 10 therapeutic levels. For example, according to embodiments, a force $F(r)$ may be exerted by an expandable sieve to resist flows of approximately 1 liter/min, 100 ml/min, or 10 ml/min. Preferable ranges have been found to be, for example, between 50-100 ml/min. For example, in one embodiment the expandable sieve may be held in place in a flow of 1 liter/min by 15 homogenously exerting outward radial force $F(n)$ towards walls of the body lumen, without a force f applied by the throughwire 2010 or the like. In embodiments, the sieve may be configured to exert a radial force of, for example, approximately $85-1200 \text{ N/m}^2$ when deployed.

[0097] The description given above is merely illustrative and is not meant to be an exhaustive list of all possible embodiments, applications or modifications of the invention. Thus, various modifications and variations of the described methods and systems of the invention will be 20 apparent to those skilled in the art without departing from the scope and spirit of the invention. Although the invention has been described in connection with specific embodiments, it should be understood that the invention as claimed should not be unduly limited to such specific embodiments.

Expandable devices.

In a first embodiment, Fig 1, the device is intended for preventing the migration of loose tissue fragments or concretions within hollow cavities or tubular organs such as but not limited to: stone fragments within the ureter. The device comprises a slender shaft 11, which is connected at the distal end to an expandable means 12. The expandable means is designed to conserve its shape at various diameters. It may be expanded by preferably a self expanding mechanism, or it may be expanded by an active mechanical mechanism such as a pull wire or an internal balloon. The preferred shape may be chosen from a list of such shape such as but not limited to spherical, cylindrical ellipsoid, pear shaped, conical, etc. Such shape should preferentially have a radial symmetry and should preserve such symmetry at various diameters. This design is preferred in order to fit at various ureteral diameters and to always completely obliterate its lumen in order to prevent migration of stone fragments proximally towards the kidney during stone fragmentation. The expandable means may be provided with openings 13, whose diameter should be no larger than 1 to 2 mm diameter in the expanded state, in order to prevent stone fragments to enter into the expandable means and to block it in the expanded configuration, or to migrate distally to it. Alternatively, the expandable means may be provided with a film 14, which covers its openings and which prevents stone fragments from entering into it. This coated expandable device may reduce the flow of fluid to the kidney pelvis during ureteroscopy and therefore reduce the chance for fluid absorption and pain due to distension of the kidney pelvis and may improve the visibility at the stone site.

The expandable means may be manufactured of a biocompatible material such as but not limited to Nitinol, stainless steel or other metallic or plastic materials. The expandable means may be self expandable and may be manufactured of such as but not limited to: a self expandable stent or woven mesh material.

The device is covered with a slender sheath 15. The distal end of the expandable means may be attached to a slender flexible guide-wire 16a, or the distal end of the expandable means 12 may be tip-less 16b. Such guide wire may be pre-shaped at its distal end in a pig tail 17a or helical shape 17b, U shaped 17c, or O shaped 17d. Such distal end of the guide wire may serve as a retention means of the guide wire in the kidney pelvis and prevent its dislodgement during stone fragment evacuation from the ureter with the expandable means. Additionally, the proximal end of the guide wire 18 may be helical too to prevent dislodgement of the distal end of the guide wire from the kidney pelvis during manipulation of the device. The proximal end of the shaft may be releasably attached to a handle 19 for manipulating the device.

In another embodiment, Fig 2, the device is provided with 2 expandable means 21 and 22, which are connected by a connecting filament 23 that may be straight or helical.

In another embodiment Fig. 3, the expandable means 31 is provided with a locking means 32, which may be for example an internal filament 32 connected to the distal end 33 of the expandable means 31 from within and passing through a proximal orifice or neck of the expandable means 34. By pulling on this locking filament the expanded expandable means remains in this configuration and can not regain its slender configuration.

The method of use is described in Fig 4a. The device 41 is introduced through a ureteroscope 42 working channel, or through an ureteroscope introducer sheath within the ureter 43 and besides the stone, above the stone 44 towards the kidney 45 under direct vision and/or fluoroscopy.

In Fig. 4b the outer sheath is retracted revealing the self expandable means 46 that will expand and occlude the ureter 43 above the stone 44. The stone is fragmented by standard fragmentation means such as laser, electrohydraulic, pneumatic or ultrasonic lithotripter devices and the stone fragments are prevented from migrating towards the kidney by the expanded expandable means that is situated above the stone within the ureter and is occluding its lumen.

Then, Fig 4c, the device is pulled by the slender shaft 46 and the expanded expandable means will brush out the remaining stone fragments out from the ureter within the urinary bladder or through the introducer sheath outside the patient. Alternatively, in case that the device is provided with a locking filament 47 the device is pulled after tightening and locking the locking filament that will prevent the expandable means to resume its slender configuration and may permit a more forceful brushing out of the remaining stone fragments.

In Fig. 4d, the handle 48 and the sheath 49 of the device is removed and only the slender shaft that is connected to the expandable means remains within the working channel of the ureteroscope or with the introducer sheath. Such shaft may have a very small diameter from 0.5 mm down to 0.01 mm and preferentially, between 0.3 to 0.1 mm and leave more space within the working channel for other instruments and for irrigation.

In Fig. 5a, the device described in embodiment 2, is introduced in a similar way to what was described in Fig. 4 into the ureter above the stone. The distal guide wire 16 is introduced within the kidney pelvis and serves as a retention means for the device during its manipulation. The device is pulled and the proximal 21 expandable means is brushing out the ureter the stone fragments. The distal 22 expandable means remains within the ureter and prevent possible migration towards the kidney or some stone fragments. In Fig. 5b the sheath of the device 15 is advanced again over the proximal expandable means 21 and the entire device is pushed again within the ureter, the proximal expandable means is re-exposed and additional stone fragments may be brushed out. This procedure may be repeated as needed and may be suitable in case of a large stone burden or of multiple stones at different locations within the ureter.

In another embodiment Fig 6a, the expandable means is conical 61, with the pointed tip 62 facing distally towards the kidney and the proximal rim 63 of the conical expandable means is connected by one or more and preferably 2 or 3 slender filaments 64. The slender shaft 65 is attached from within to the tip of the expandable means. Such a device acts like an umbrella that can be flipped over. In order to expand it the external sheath 66 is retracted and then the slender shaft is pushed forward while the filaments 64 are retracted. The slender shaft 65 and slender filaments 64 may be kept together by a very thin sheath 67. In this case the external sheath 66 may be removed during fragmentation of the stone. When the device is expanded within the ureter above the stone or stone fragments, it can capture them and permit their evacuation. When desirable the stone fragments may be disengaged by pulling on the slender shaft against the external sheath,

which will cause the expandable device to flip over and to release the stone fragments Fig 6b.

In another embodiment Fig. 7, the expandable device 71 may be detachable from its slender shaft 72a, or it may be pushed out of the external sheath 73 by a pusher 72b. The expanded device may be retrieved by a standard grasper. Such embodiment may be desirable in order to prevent stone migration to cavities such as calyces of the kidney during ureteroscopy and/or percutaneous nephrolithotripsy.

In a preferred embodiment the device may serve as a guide wire for introducing a D-J stent over it to the kidney pelvis Fig. 8. In order to perform this maneuver, the handle is removed and the D-J stent 81 is introduced over the sheath of the device to the renal pelvis, or the sheath of the device is removed and the stent is advanced over the slender shaft 82 of the device over the expandable device 83 and over the distal guide wire 84.

Such devices may be used for preventing migration and or removal of loose bodies, foreign bodies, or concretions such as but not limited to: calcifications, stones, thrombi, loose tissues, plaque fragments, emboli, bone fragments in any hollow or tubular organs such but not limited: urethra, urinary bladder, ureter, kidney pelvis, gastrointestinal tract, biliary ducts, gallbladder, pancreatic ducts, blood vessels, upper respiratory tract or bronchi, salivary ducts, lacrimal ducts, articulations, bursa etc.

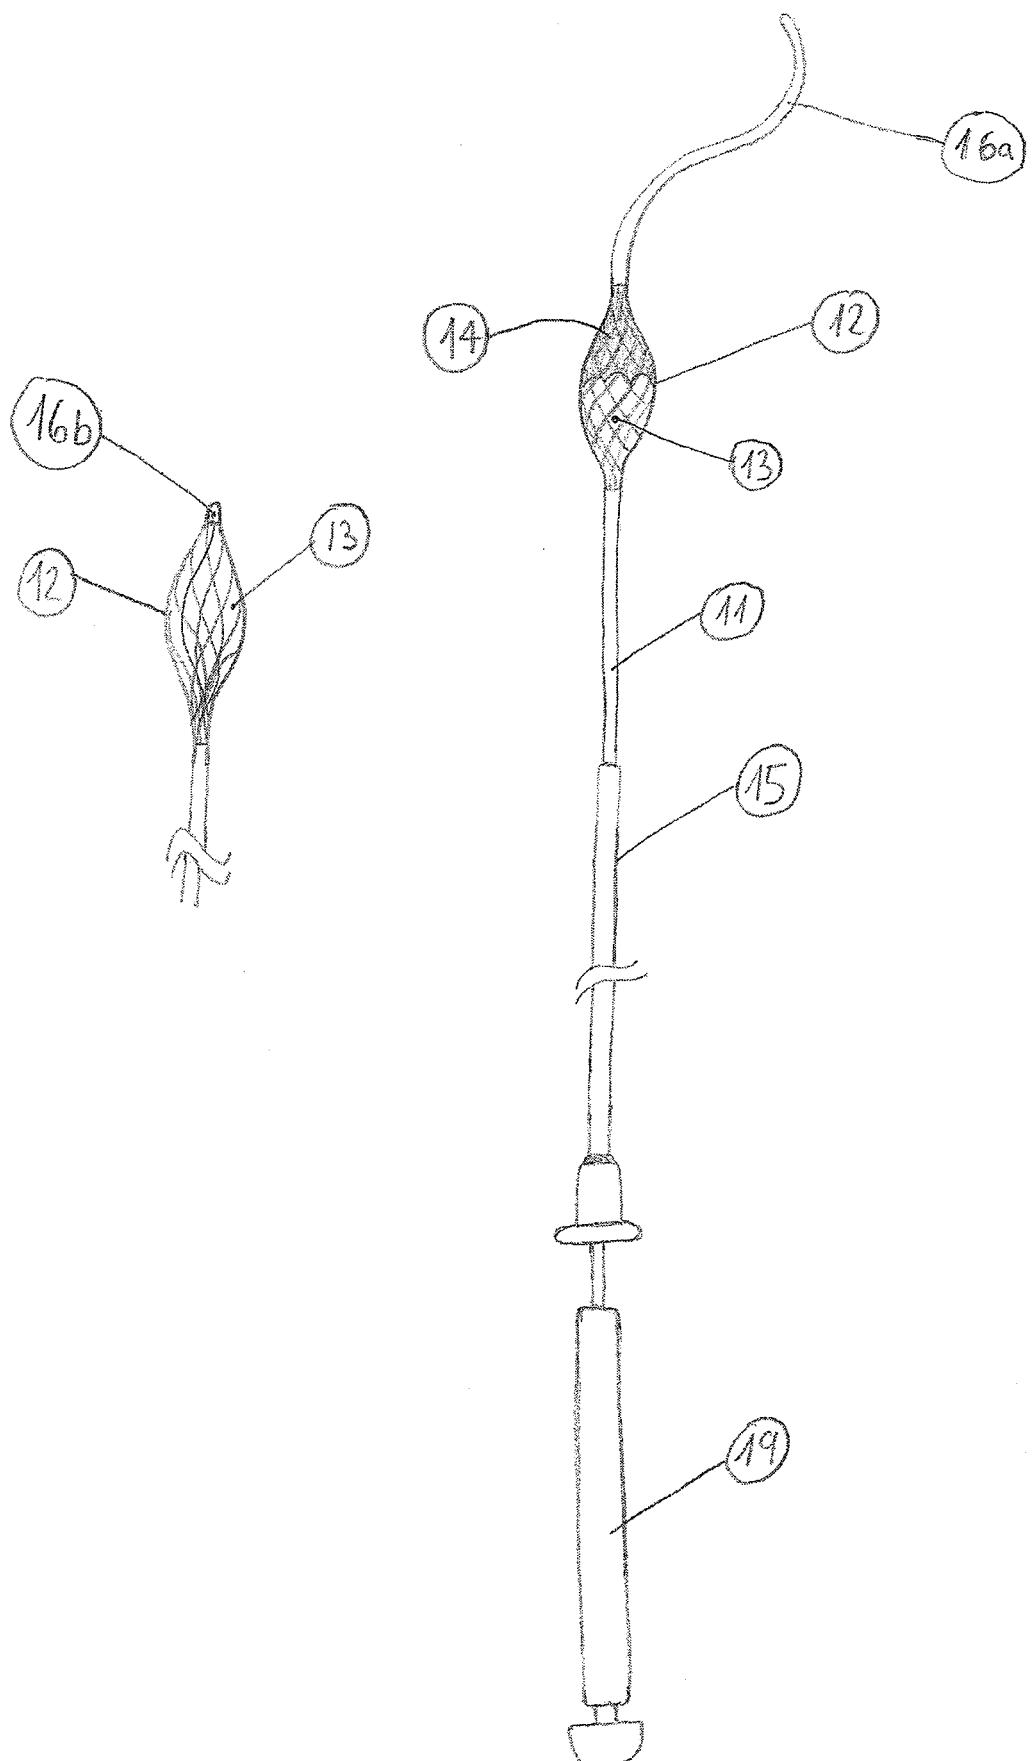


Fig. 1A

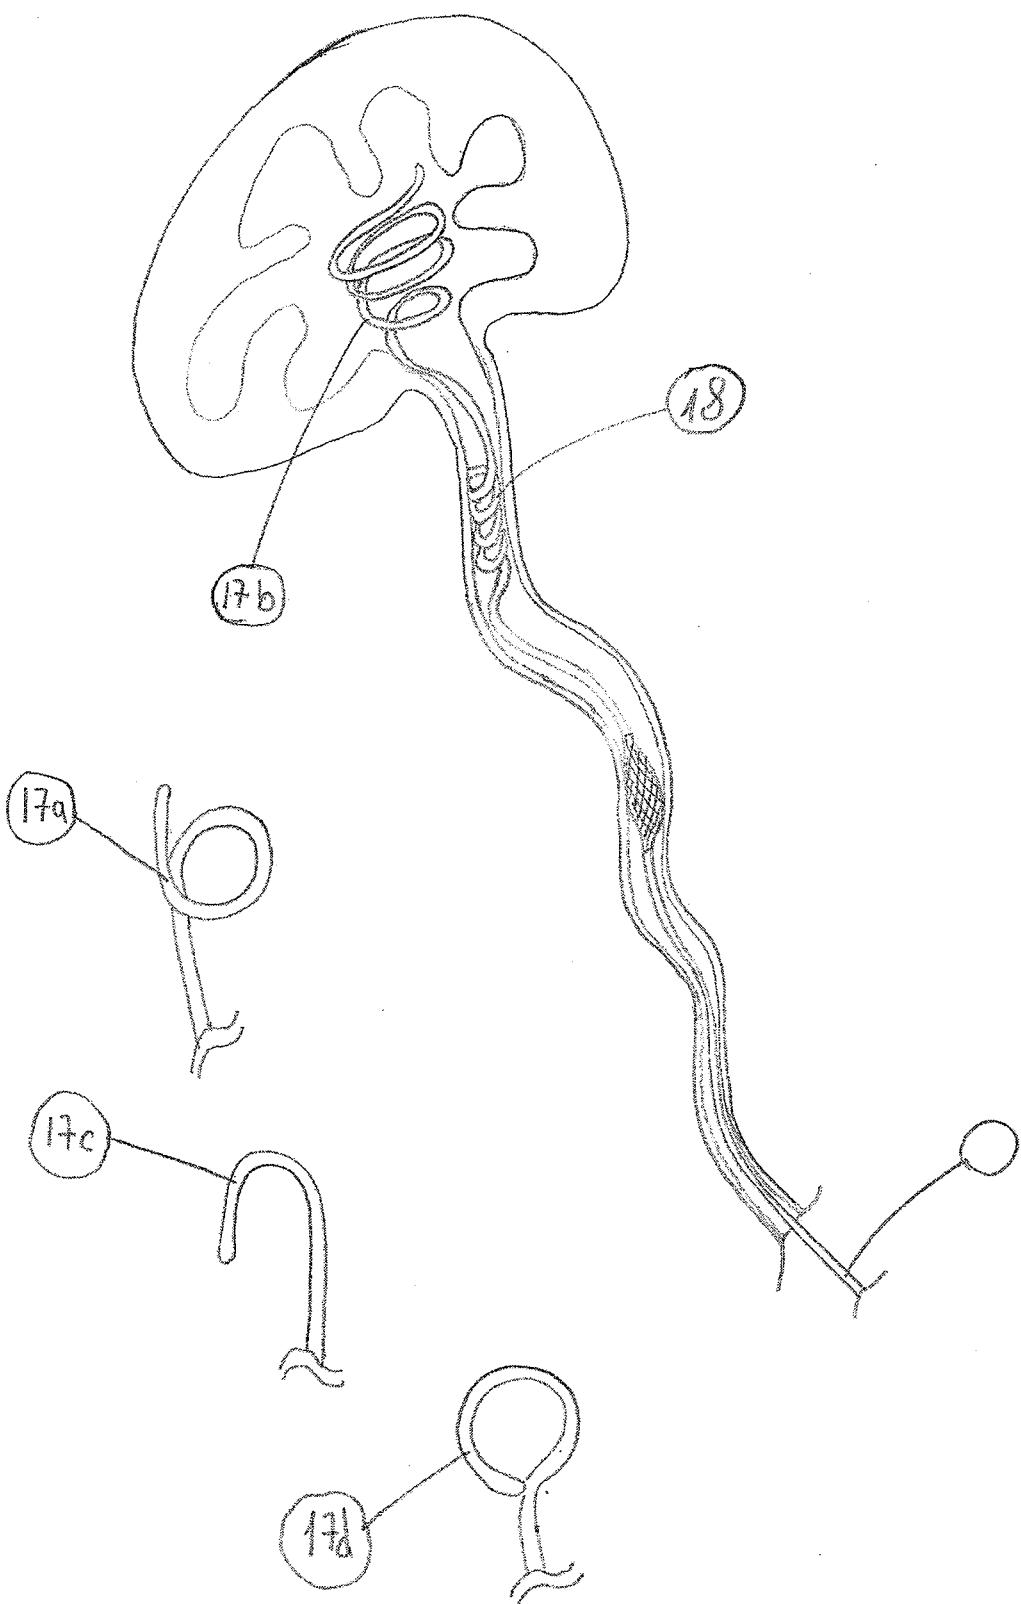


Fig 1B

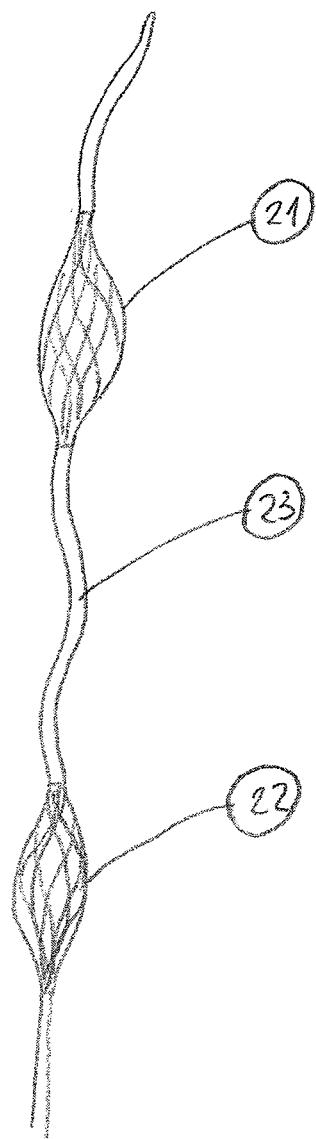


Fig 2

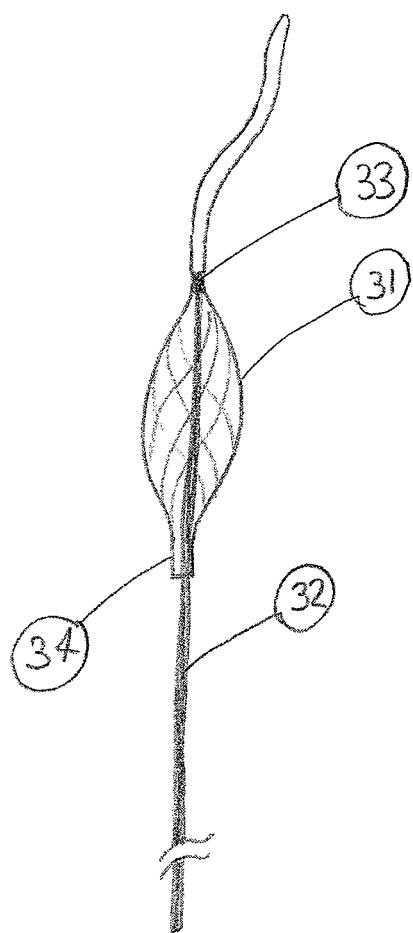


Fig 3

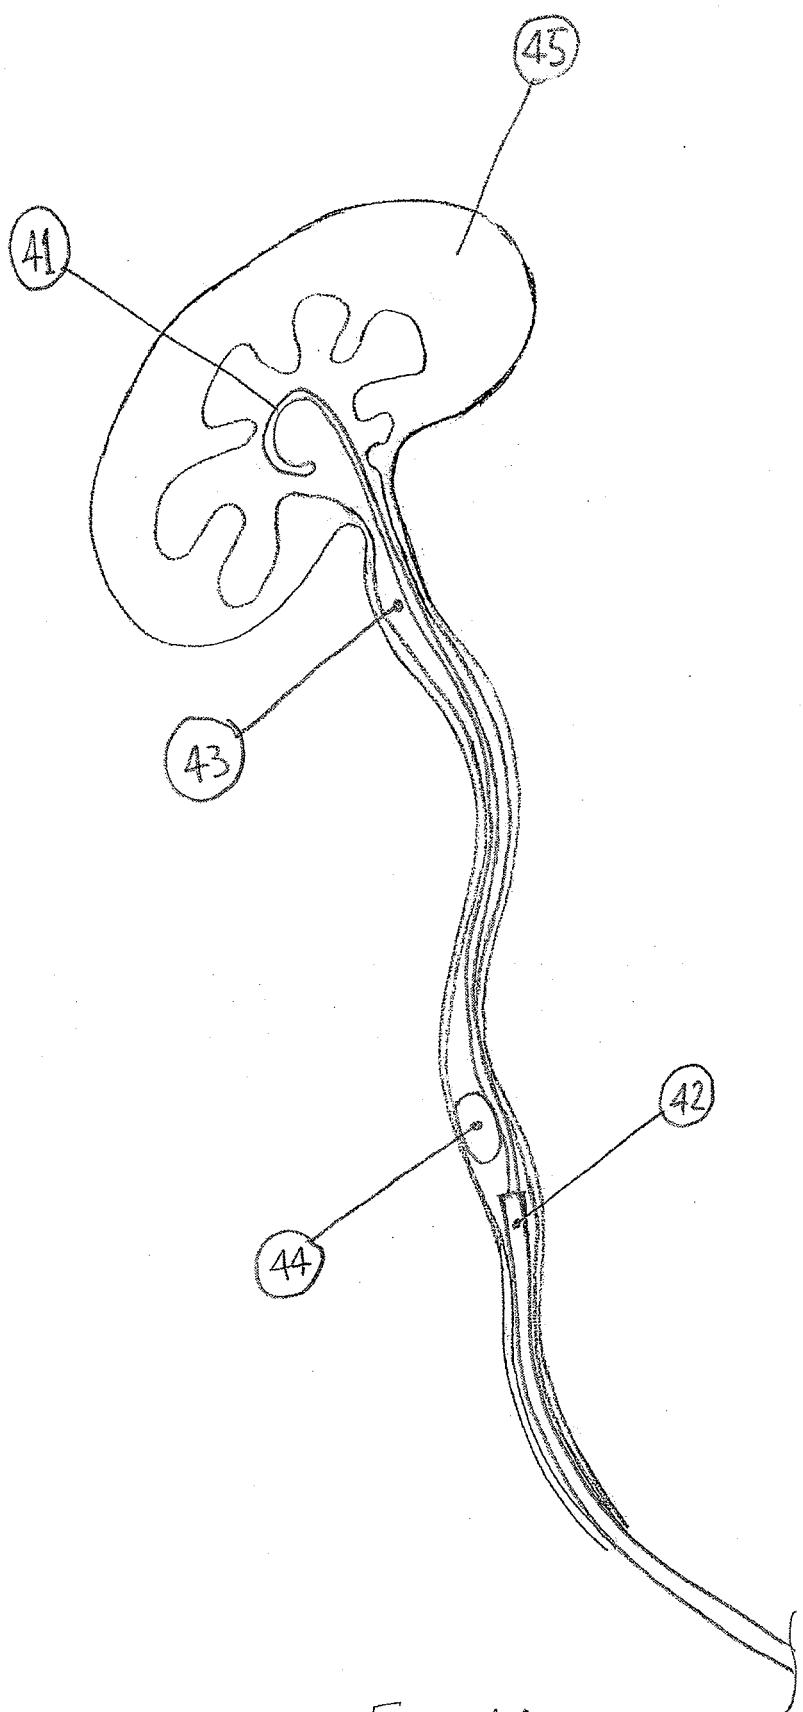


Fig. 4A

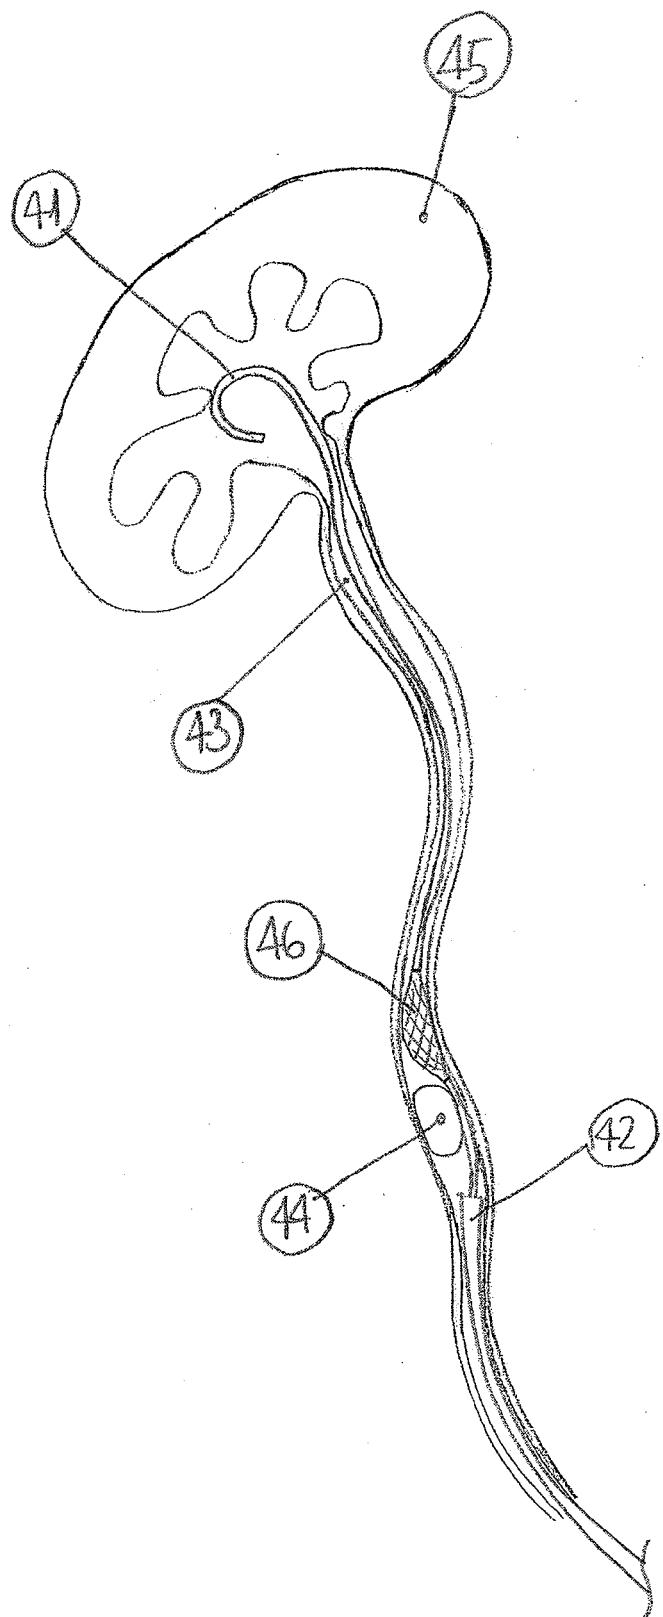
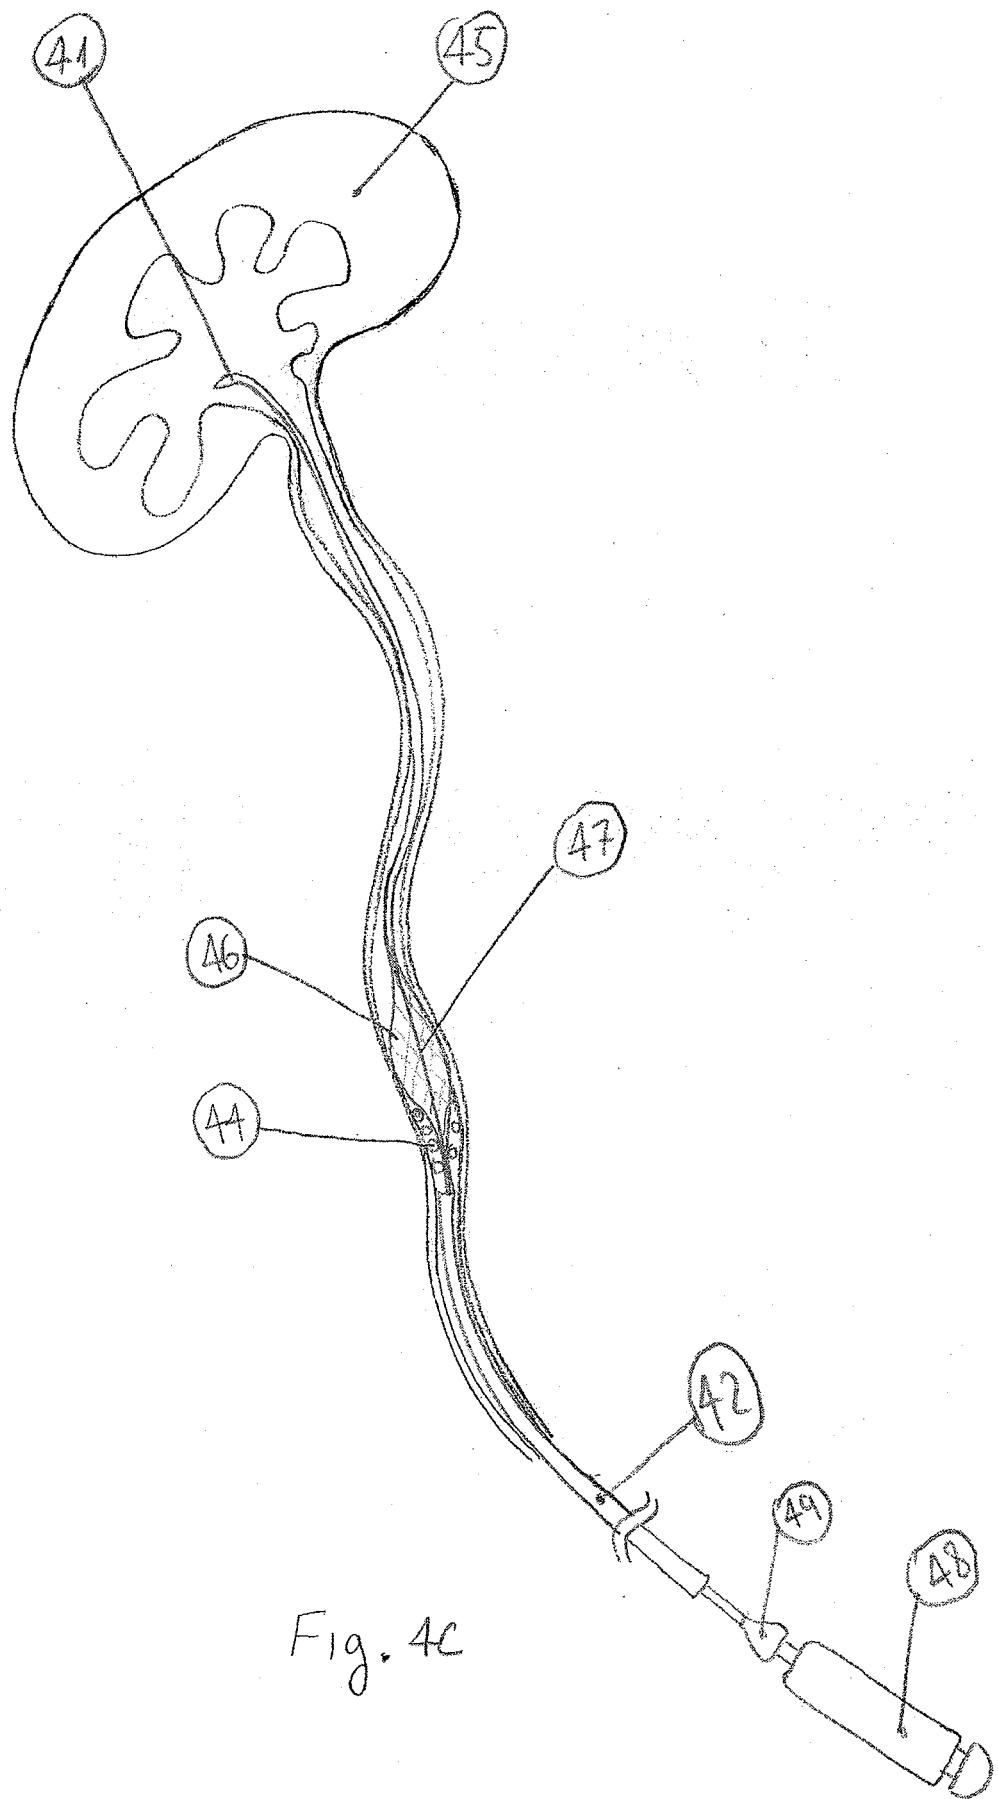


Fig. 4B



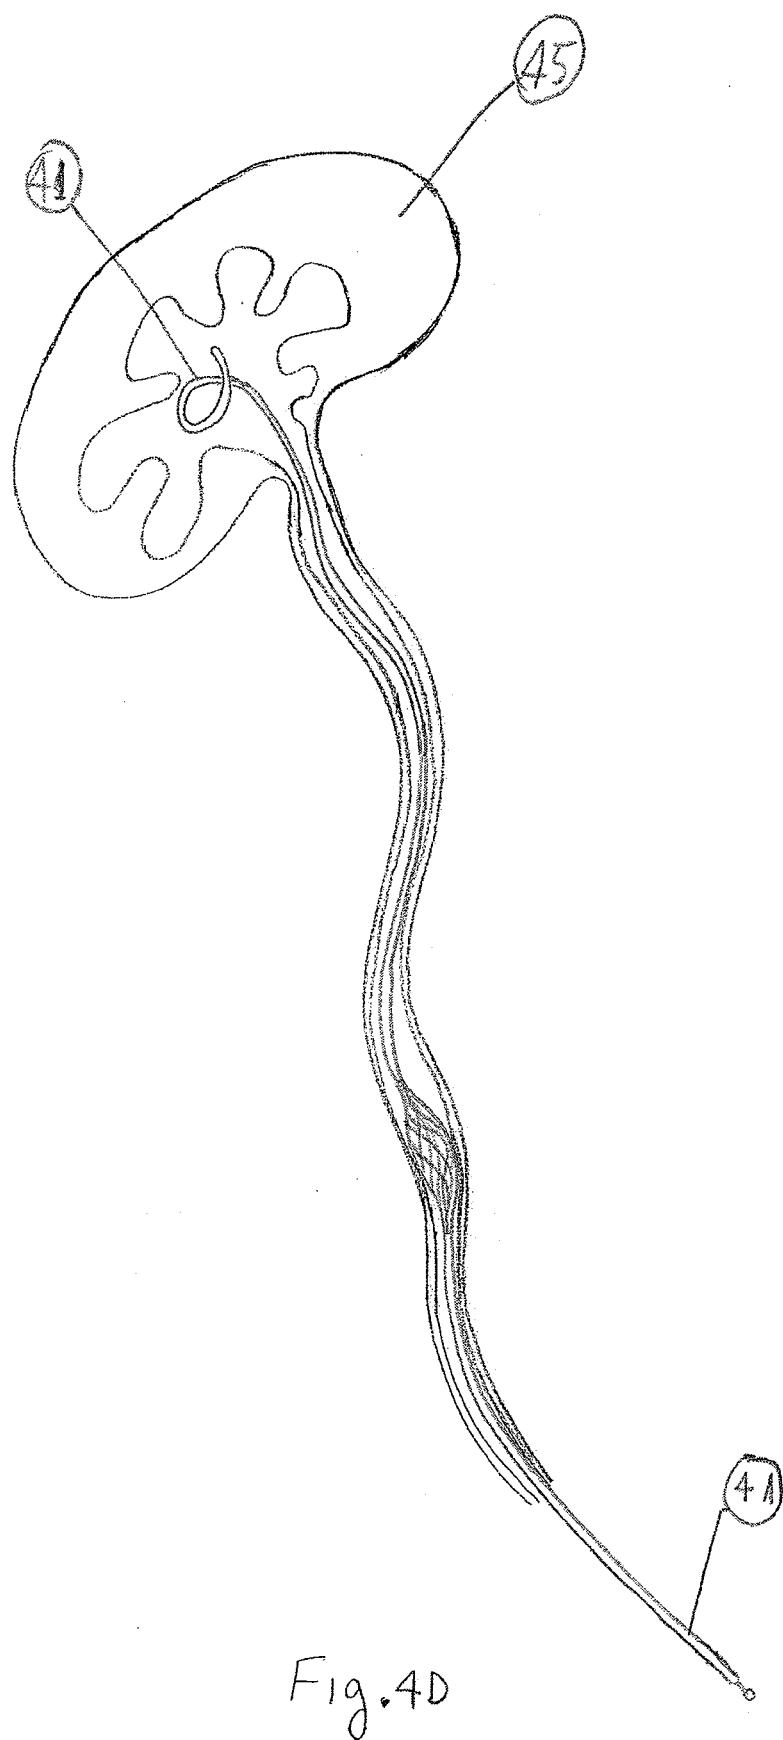


Fig. 4D

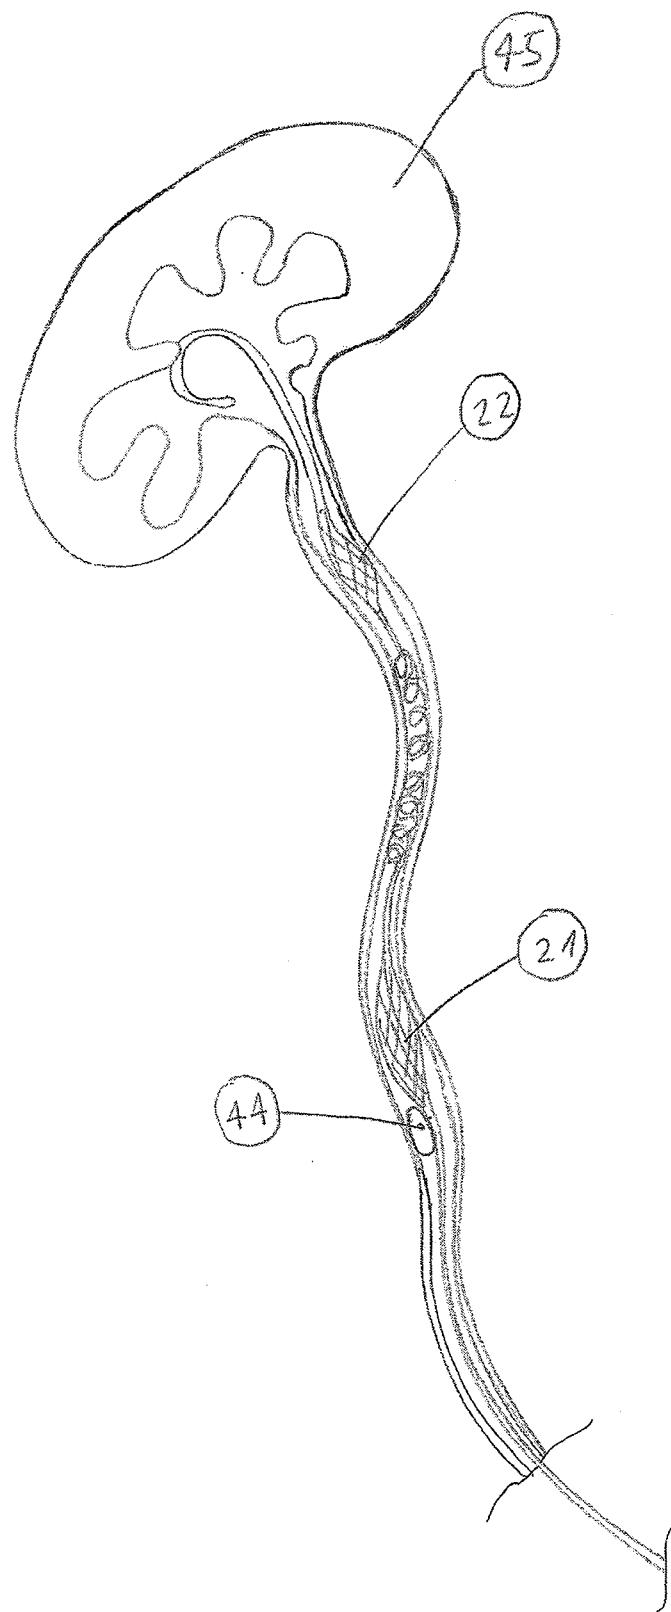


Fig. 5a

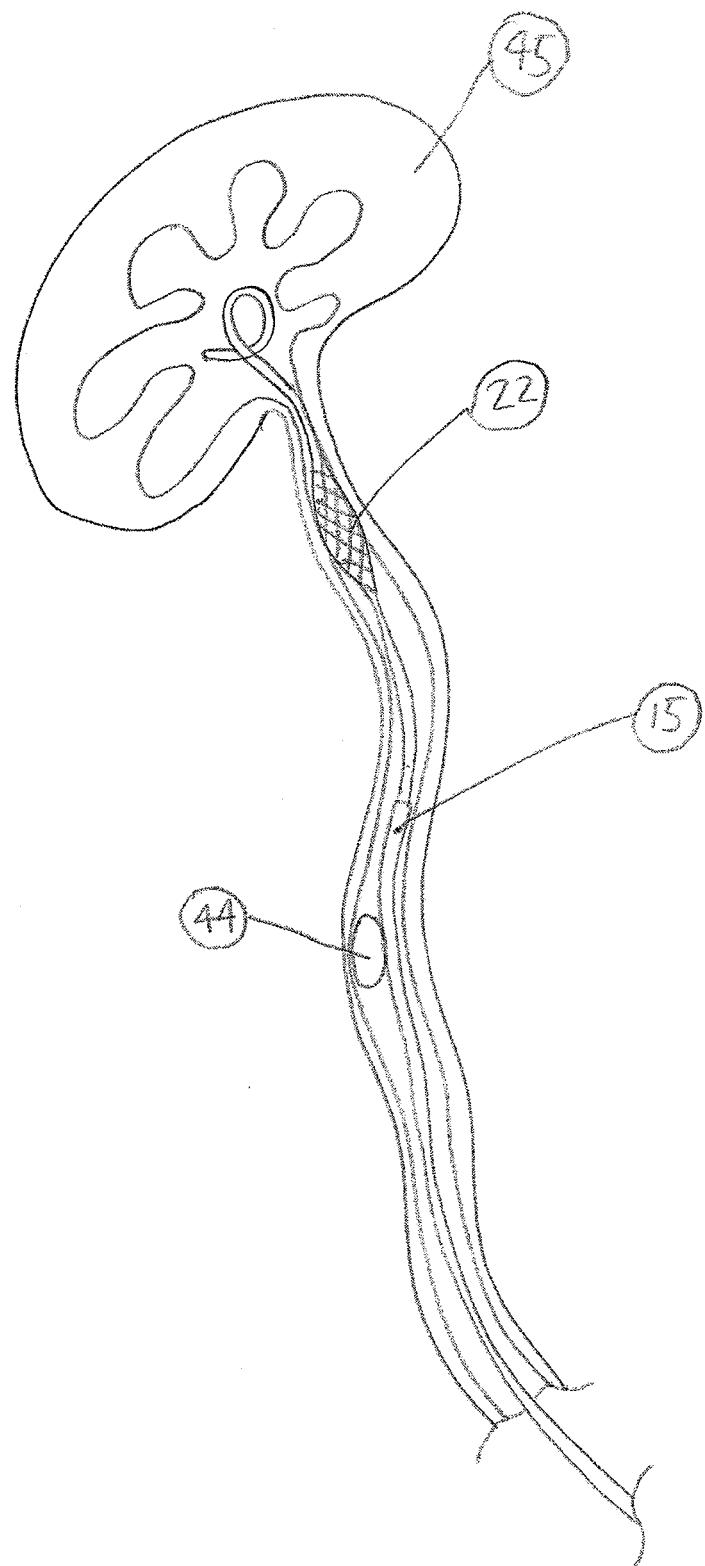


Fig 5b.

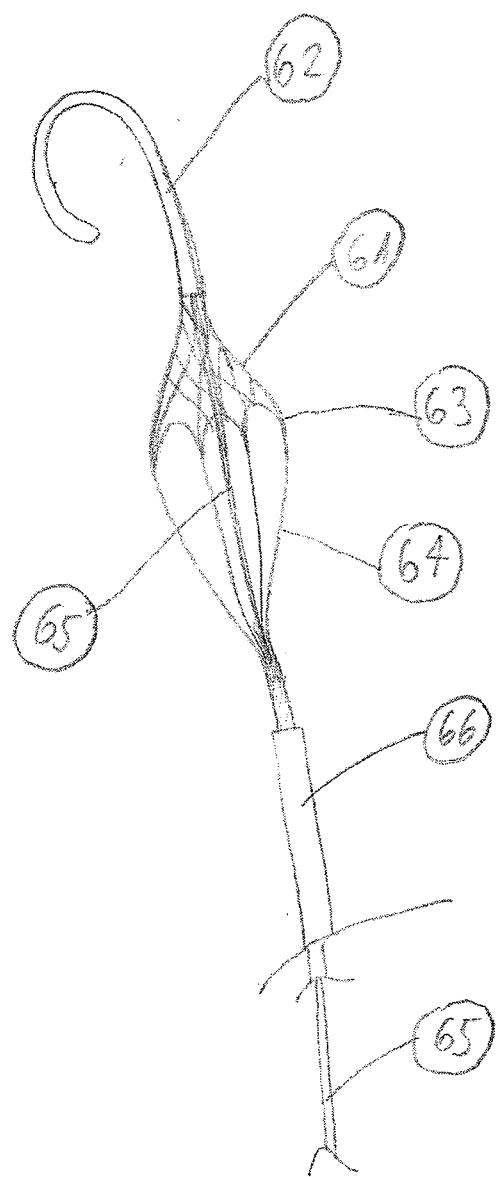


Fig 6a

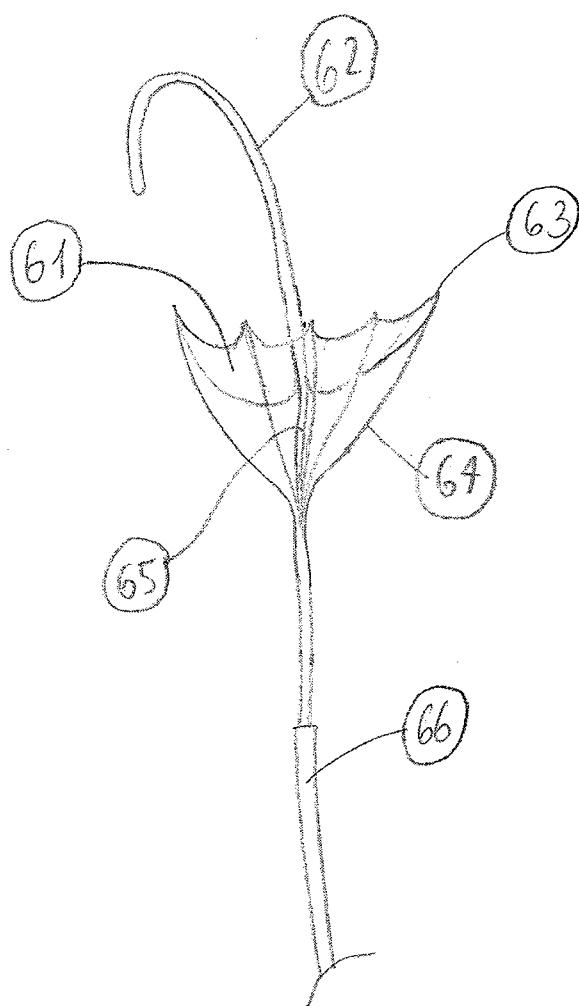


Fig 6 b.

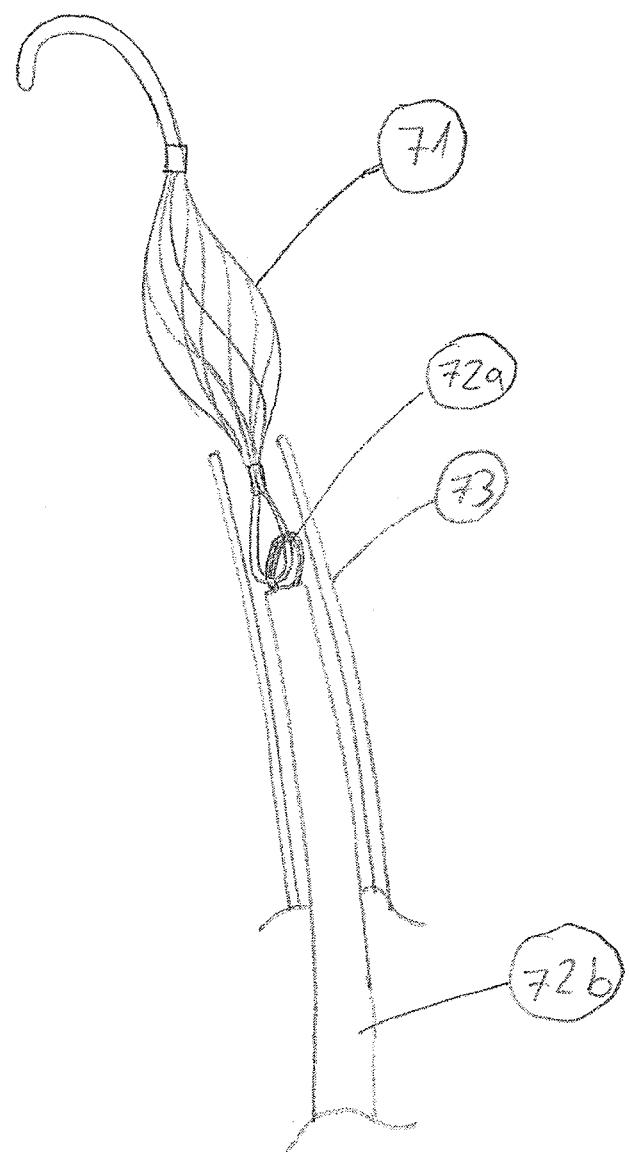


Fig 7

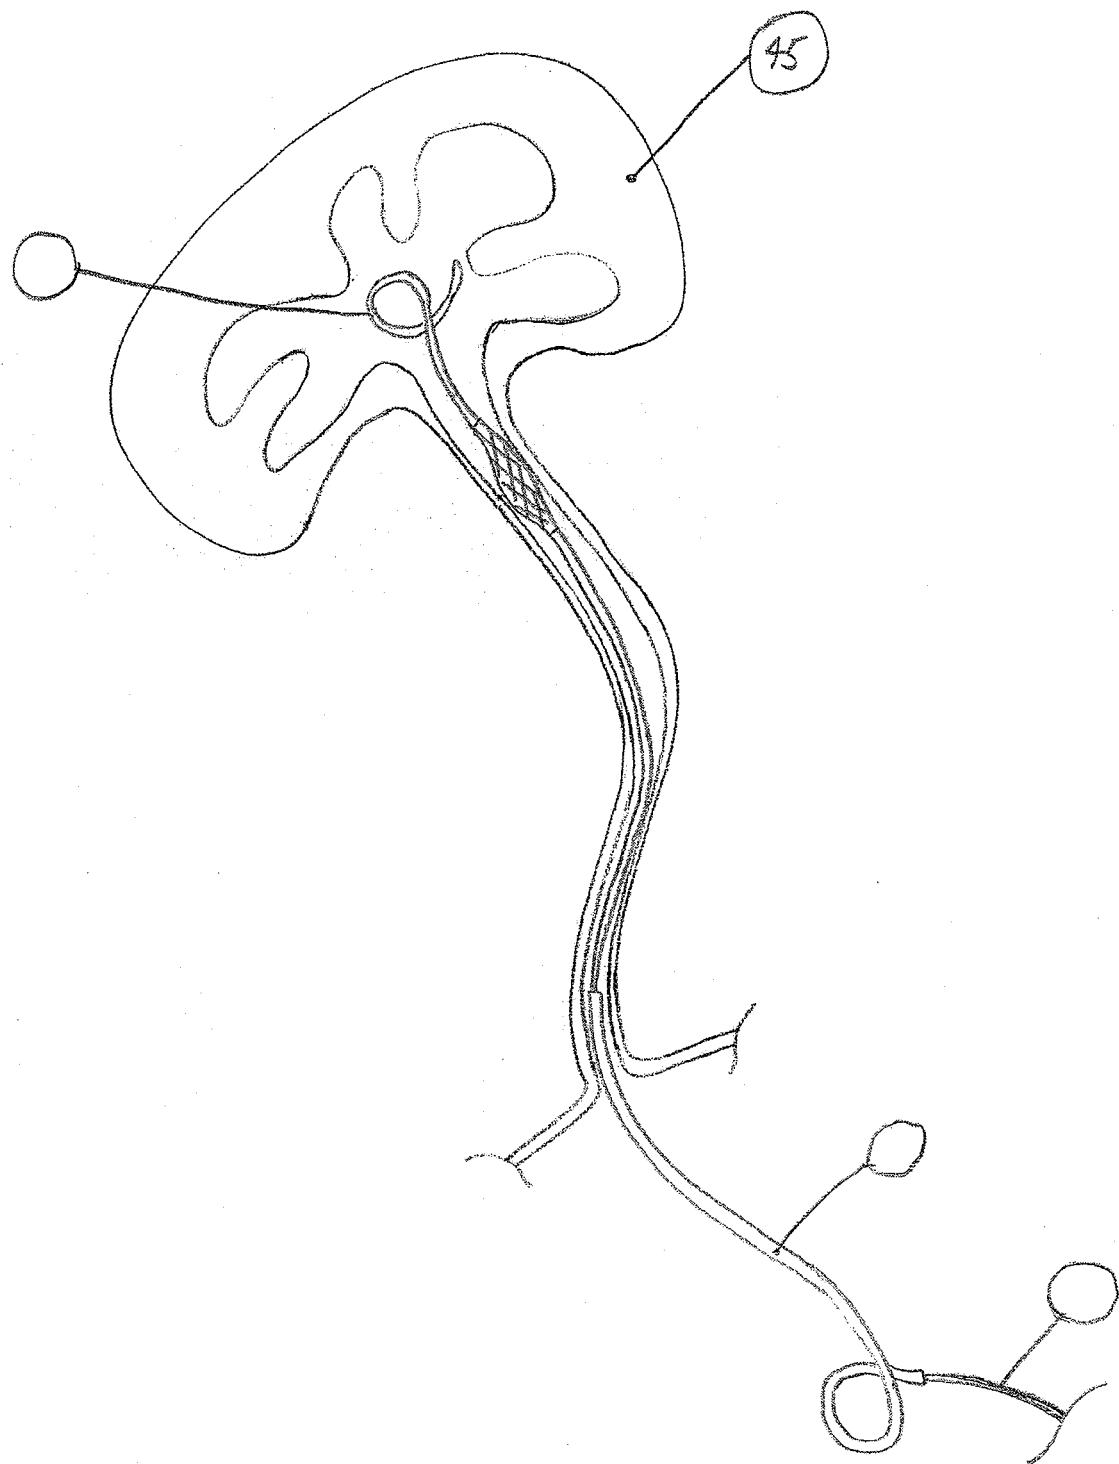


Fig 8a

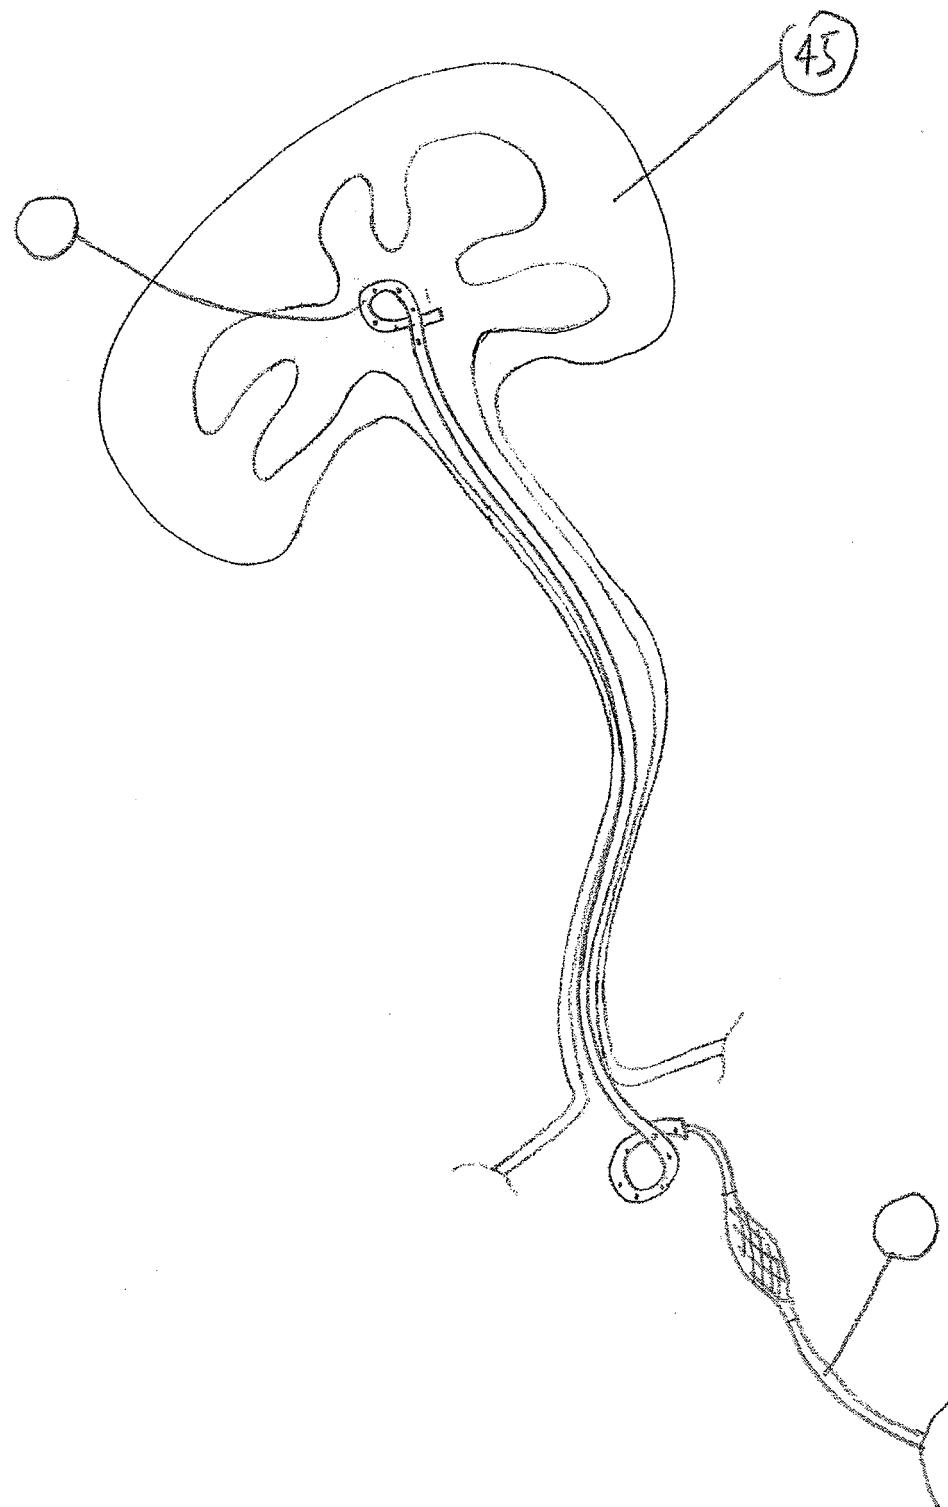


Fig 8b

1 WHAT IS CLAIMED IS:

2

3 1. A medical device comprising:

4 a wire;

5 a sheath surrounding at least part of the wire, the sheath being axially moveable in
6 at least one direction along the wire; and

7 a first expandable sieve contained at least partially in the sheath,

8 wherein, the first expandable sieve is configured to expand from a collapsed state
9 to an expanded state that substantially conforms to a transverse cross section of a body lumen
10 and having a diameter in the range of approximately 0.5 mm and 15 mm.

11

12 2. The device of claim 1, wherein the first expandable sieve is configured to
13 substantially prevent a passage of particles with a maximum diameter greater than, or equal to,
14 1.0 mm therethrough, and to substantially allow a passage of particles with a maximum diameter
15 less than 1.0 mm therethrough.

16

17 3. The device of claim 1, wherein the first expandable sieve is configured to
18 substantially prevent a passage of particles with a maximum diameter greater than, or equal to,
19 2.0 mm therethrough, and to substantially allow a passage of particles with a maximum diameter
20 less than 2.0 mm therethrough.

21

22 4. The device of claim 1, wherein the device is configured to accommodate a
23 stent being deployed over a free end of the wire and past the first expandable sieve.

24

25 5. The device of claim 1, wherein the device is configured to accommodate a
26 ureteroscope working channel passing thereupon.

27

28 6. The device of claim 1, wherein the first expandable sieve is configured to
29 maintain a positioning of the first expandable sieve along a length of the body lumen, while
30 subjected to an irrigation flow in a range of approximately 10 ml/min to 1.0 liter/min, by only a
31 radial force exerted by the first expandable sieve on a wall of the body lumen while the first
32 expandable sieve is in the expanded state.

34 7. The device of claim 1, wherein the first expandable sieve is configured to
35 maintain a positioning of the first expandable sieve along a length of the body lumen, while
36 subjected to an irrigation flow in a range of approximately 50-100 ml/min, by only a radial force
37 exerted by the first expandable sieve on a wall of the body lumen while the first expandable
38 sieve is in the expanded state.

39
40 8. The device of claim 1, wherein the first expandable sieve is configured to
41 maintain a positioning of the first expandable sieve along a length of the body lumen, while
42 subjected to an irrigation flow in a range of approximately 10 ml/min to 1 liter/min, by a radial
43 force exerted by the first expandable sieve on a wall of the body lumen, while the first
44 expandable sieve is in the expanded state, and a restraining force applied by the wire.

45
46 9. The device of claim 1, wherein the sheath is redeployable over the first
47 expandable sieve in the expanded state to return the first expandable sieve substantially back to
48 the collapsed state.

49
50 10. The device of claim 1, wherein the first expandable sieve has a
51 compressed diameter of approximately less than 1.0 mm.

52
53 11. The device of claim 1, wherein the first expandable sieve is configured to
54 expand to an expanded state that is adjustable within a range of approximately 0.5 mm and 15
55 mm.

56
57 12. The device of claim 1, wherein the first expandable sieve is configured to
58 maintain an opening size less than 2.0 mm throughout an expanded state range of approximately
59 1.0-13 mm.

60
61 13. The device of claim 1, wherein the sheath has an outer diameter less than
62 or equal to approximately 1.5 mm.

63
64 14. The device of claim 1, further comprising an anchor located at a distal end
65 of the device.

67 15. The device of claim 1, wherein the first expandable sieve is adjustably
68 positionable along a length of the wire.

69

70 16. The device of claim 1, further comprising a second expandable sieve
71 mounted to the guide wire and that is configured to be expanded independently from the first
72 expandable sieve.

73

74 17. A medical system configured for fragmenting calcified aggregations
75 including the device of claim 1.

76

77 18. The system of claims 17, wherein the system is configured to interface
78 with at least a ureteroscope, a fragmentation energy source, and an irrigation source.

79

80 19. A medical device comprising:
81 an elongated support member;
82 a sheath configured to surround at least part of the support member, the sheath
83 being axially moveable in at least one direction along the support member; and
84 a first expandable sieve configured to be deployed in a body lumen and to be held
85 at least temporarily in a compressed state by the sheath,
86 wherein the first expandable sieve is configured to maintain a positioning of the
87 first expandable sieve along a length of the body lumen, while subjected to an irrigation flow in a
88 range of approximately 10 ml/min to 1.0 liter/min, by only a radial force exerted by the first
89 expandable sieve on a wall of the body lumen while the first expandable sieve is in an expanded
90 state.

91

92 20. The device of claim 19, wherein the first expandable sieve is axially
93 moveable in at least one direction along the support member.

94

95 21. The device of claim 19, wherein the first expandable sieve is configured to
96 substantially prevent a passage of particles with a maximum diameter greater than or equal to 1.0
97 mm therethrough, and to substantially allow a passage of particles with a maximum diameter less
98 than 1.0 mm therethrough.

99

100 22. The device of claim 19, wherein the first expandable sieve is configured to
101 substantially prevent a passage of particles with a maximum diameter greater than or equal to 2.0
102 mm therethrough, and to substantially allow a passage of particles with a maximum diameter less
103 than 2.0 mm therethrough.

104

105 23. The device of claim 19, wherein the sheath is redeployable over the first
106 expandable sieve in the expanded state to return the first expandable sieve substantially back to
107 the collapsed state.

108

109 24. The device of claim 19, wherein the first expandable sieve has a
110 compressed diameter of approximately less than 1.0 mm.

111

112 25. The device of claim 19, wherein the expanded state of the first expandable
113 sieve is conformable to a body lumen with a diameter in a range of approximately 0.5 mm and
114 15 mm.

115

116 26. The device of claim 19, wherein the first expandable sieve is configured to
117 maintain an opening size less than 2.0 mm throughout an expanded state range of approximately
118 1.0-13 mm.

119

120 27. The device of claim 19, further comprising an anchor located at a distal
121 end of the device.

122

123 28. A medical device comprising:
124 a wire;
125 a sheath configured to surround at least part of the support member, the sheath
126 being axially moveable in at least one direction along the support member; and
127 a first expandable sieve configured to be deployed in a body lumen and to be held
128 at least temporarily in a compressed state by the sheath,
129 wherein the device is configured to accommodate a stent being deployed over a
130 free end of the wire and past the first expandable sieve.

131

132 29. A method of removing an obstruction from a body using the device of
133 claim 1, the method comprising:

134 inserting the wire into a body lumen;

135 withdrawing the sheath to expand the first expandable sieve from a collapsed state
136 to an expanded state;

137 inducing a liquid flow in the body lumen; and

138 straining particulates with a diameter greater than an opening size of the first
139 expandable sieve from the liquid flow in the body lumen using the first expandable sieve, while
140 maintaining a positioning of the first expandable sieve along a length of the body lumen by only
141 a radial force exerted by the first expandable sieve on a wall of the body lumen.

142

143 30. A method of removing an obstruction from a body comprising:

144 inserting an elongated support member and a first expandable sieve into a body
145 lumen, the support member and first expandable sieve at least partially surrounded by a sheath;
146 positioning the first expandable sieve in a collapsed state distally of the
147 obstruction;

148 withdrawing the sheath to expand the first expandable sieve from the collapsed
149 state to an expanded state;

150 straining particulates with a diameter greater than an opening size of the first
151 expandable sieve from a liquid flow in the body lumen using the first expandable sieve; and

152 advancing the sheath to return the first expandable sieve from the expanded state
153 substantially back to the collapsed state.

154

155 31. The method of claim 30, further comprising deploying a stent to the body
156 lumen over the support member and the expandable sieve.

157

158 32. The method of claim 30, wherein the obstruction is a kidney stone and the
159 body lumen is a ureter.

160

161 33. A method of treating a calcified aggregation in a body comprising:

162 inserting an elongated support member and a first expandable sieve into a body
163 lumen, the support member and first expandable sieve at least partially surrounded by a sheath;

164 positioning the first expandable sieve in a collapsed state distally of the calcified
165 aggregation;

166 withdrawing the sheath to expand the first expandable sieve from the collapsed
167 state to an expanded state;

168 fragmenting the calcified aggregation; and

169 straining particulates with a diameter greater than an opening size of the first
170 expandable sieve from a liquid flow in the body lumen using the first expandable sieve while
171 maintaining a positioning of the first expandable sieve along a length of the body lumen by only
172 a radial force exerted by the first expandable sieve on a wall of the body lumen.

173

174 34. The method of claim 33, wherein the calcified aggregation is a kidney
175 stone and the body lumen is a ureter.

176

177

1 / 17

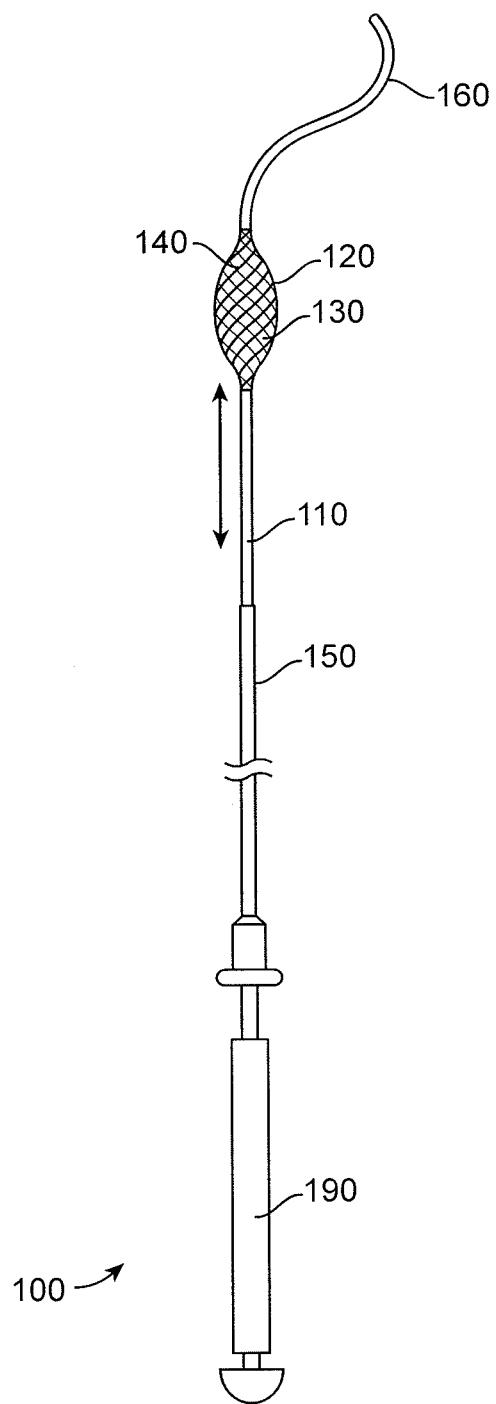


FIG. 1

2 / 17

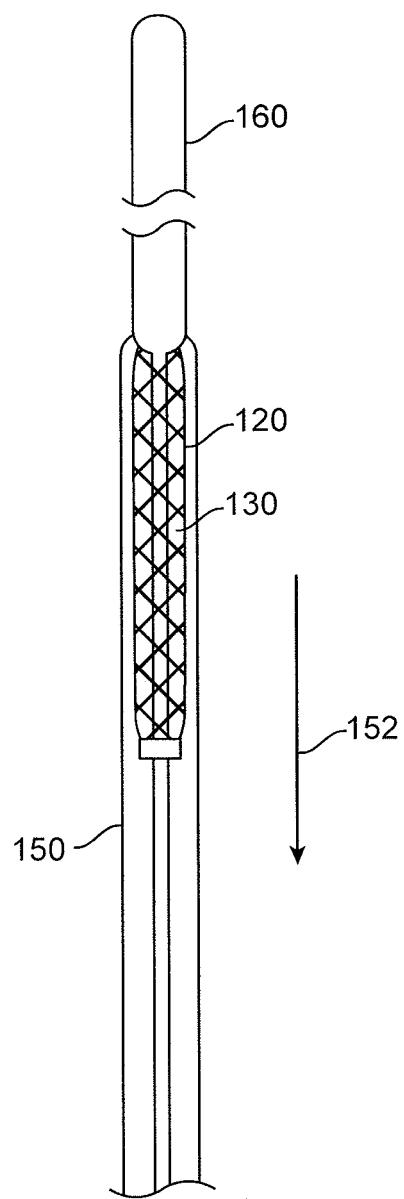


FIG. 2

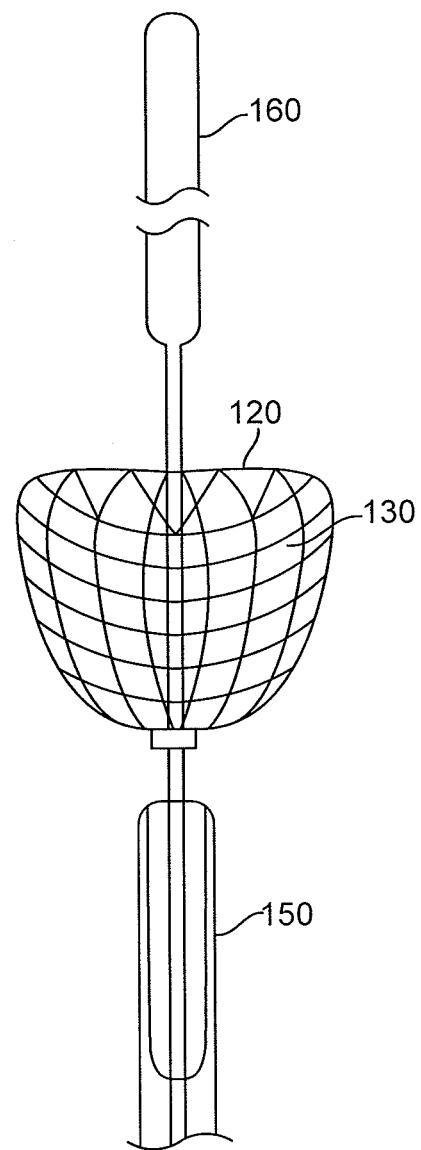


FIG. 3

3 / 17

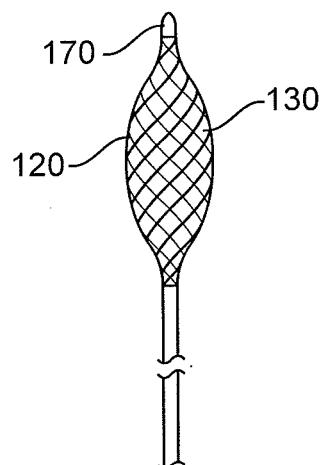


FIG. 4

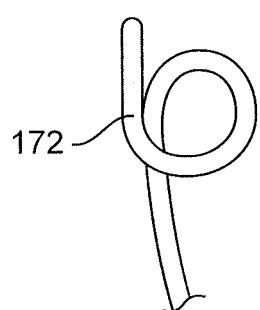


FIG. 5A




FIG. 5B




FIG. 5C

4 / 17

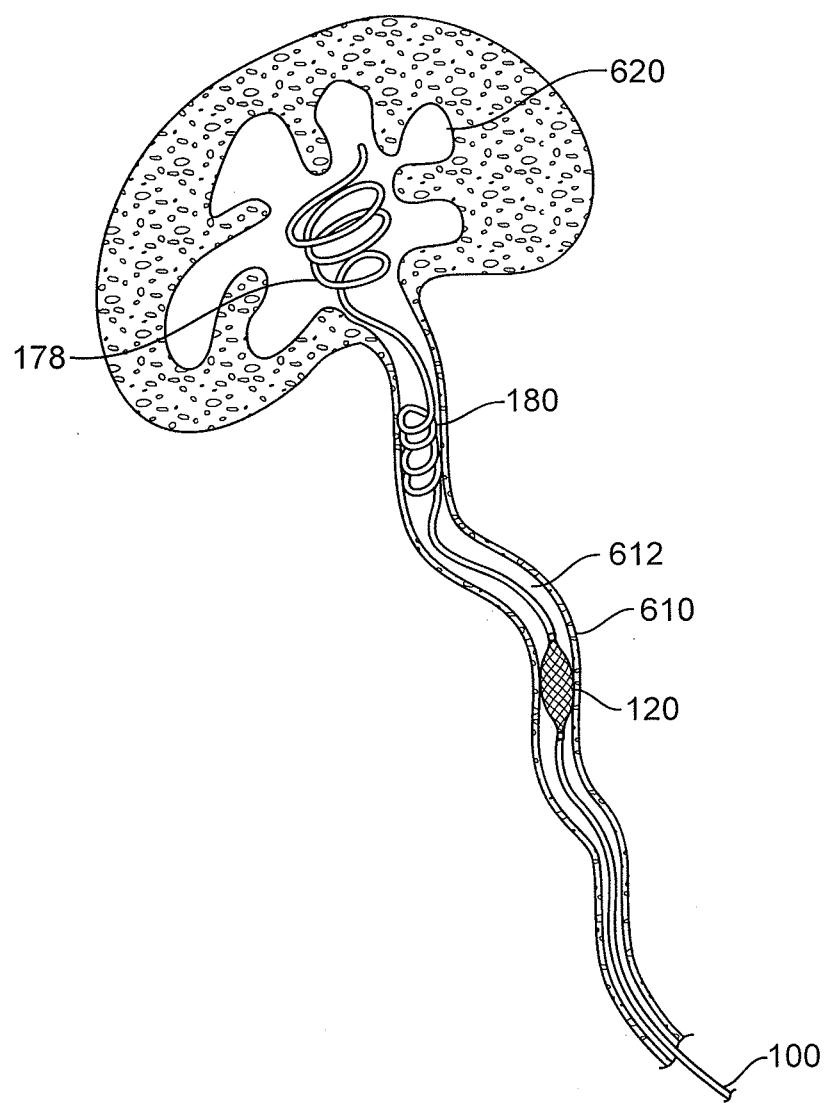


FIG. 6

5 / 17

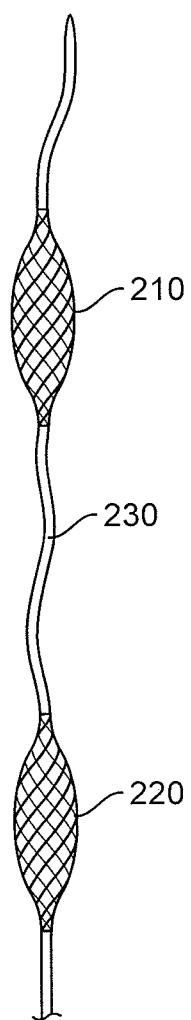


FIG. 7

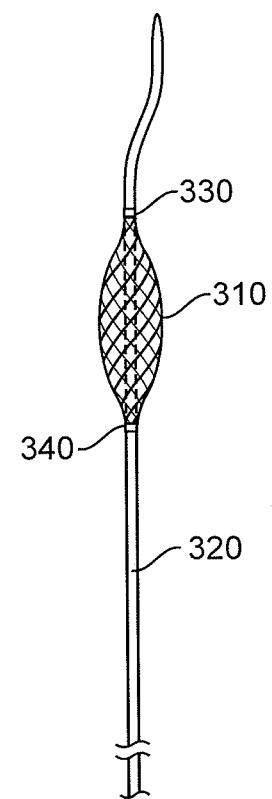


FIG. 8

6 / 17

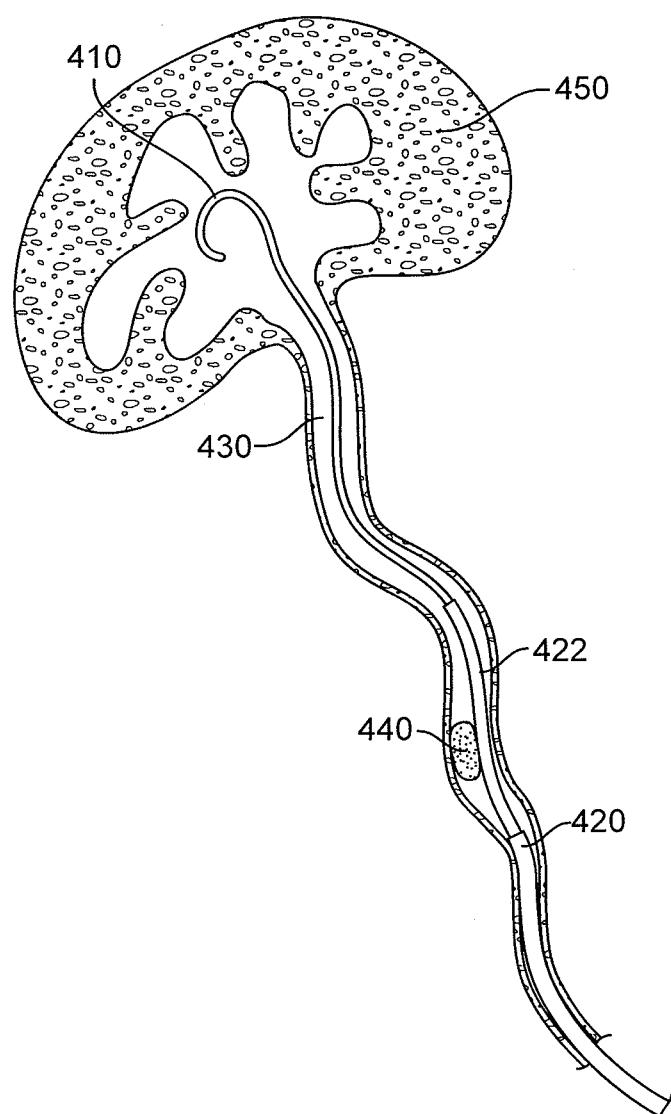


FIG. 9

7 / 17

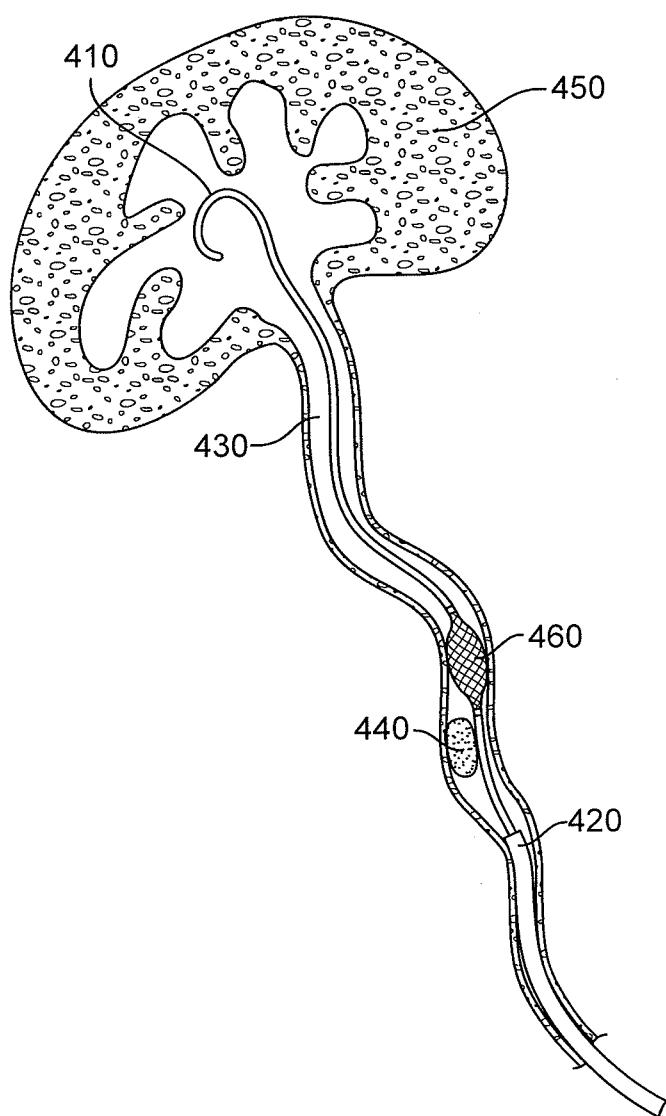


FIG. 10

8 / 17

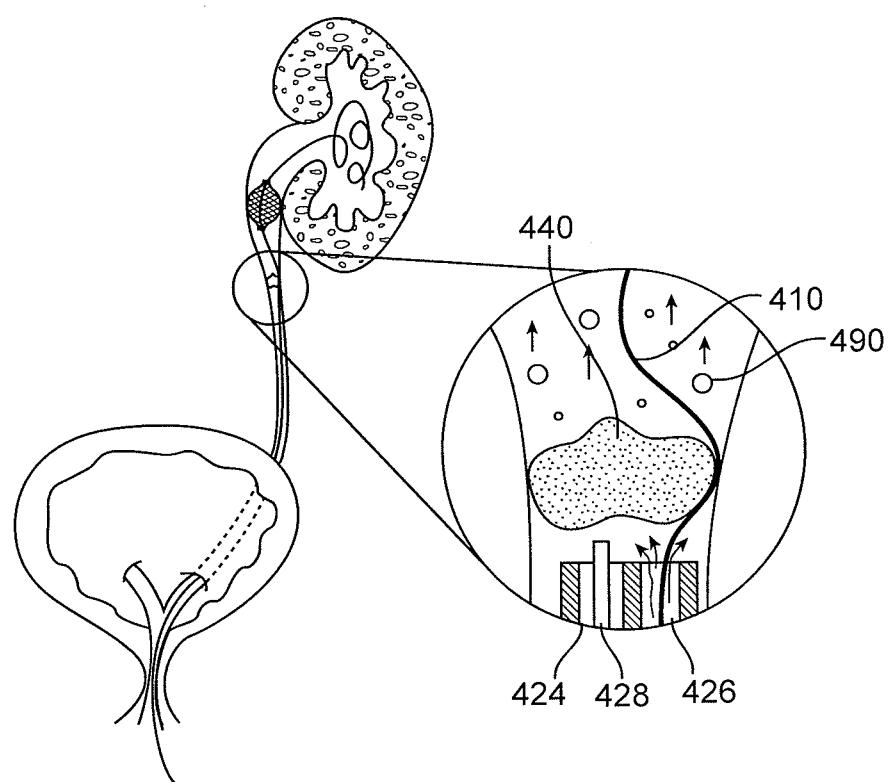


FIG. 11

9 / 17


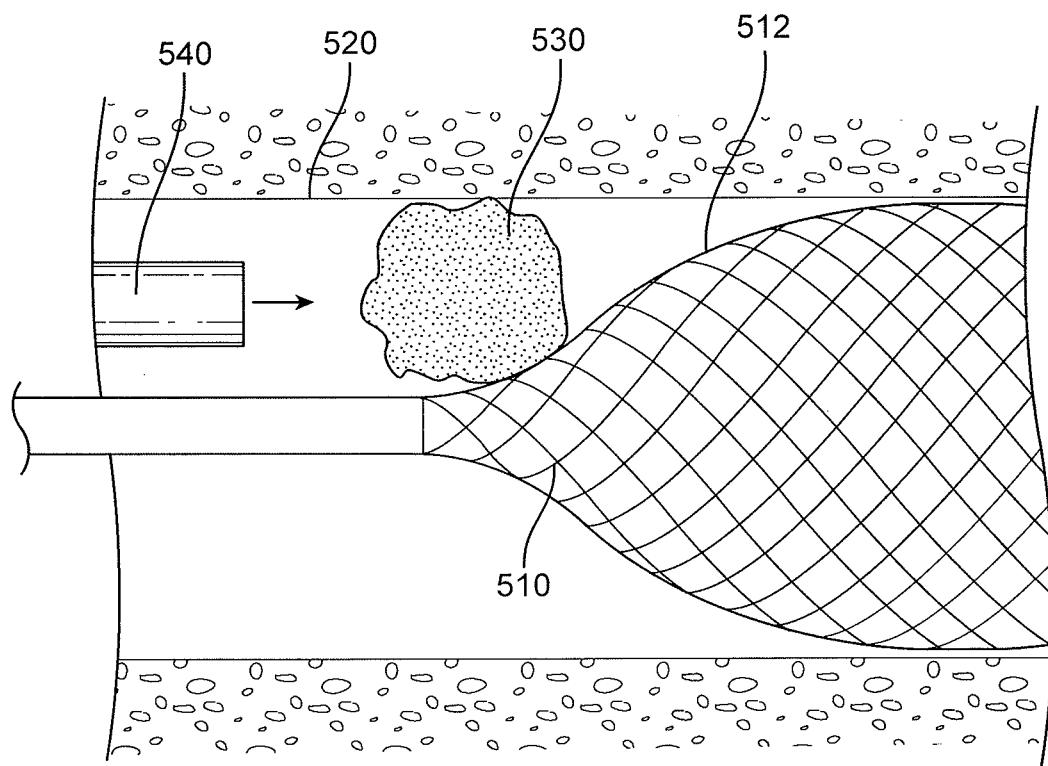


FIG. 12

10 / 17

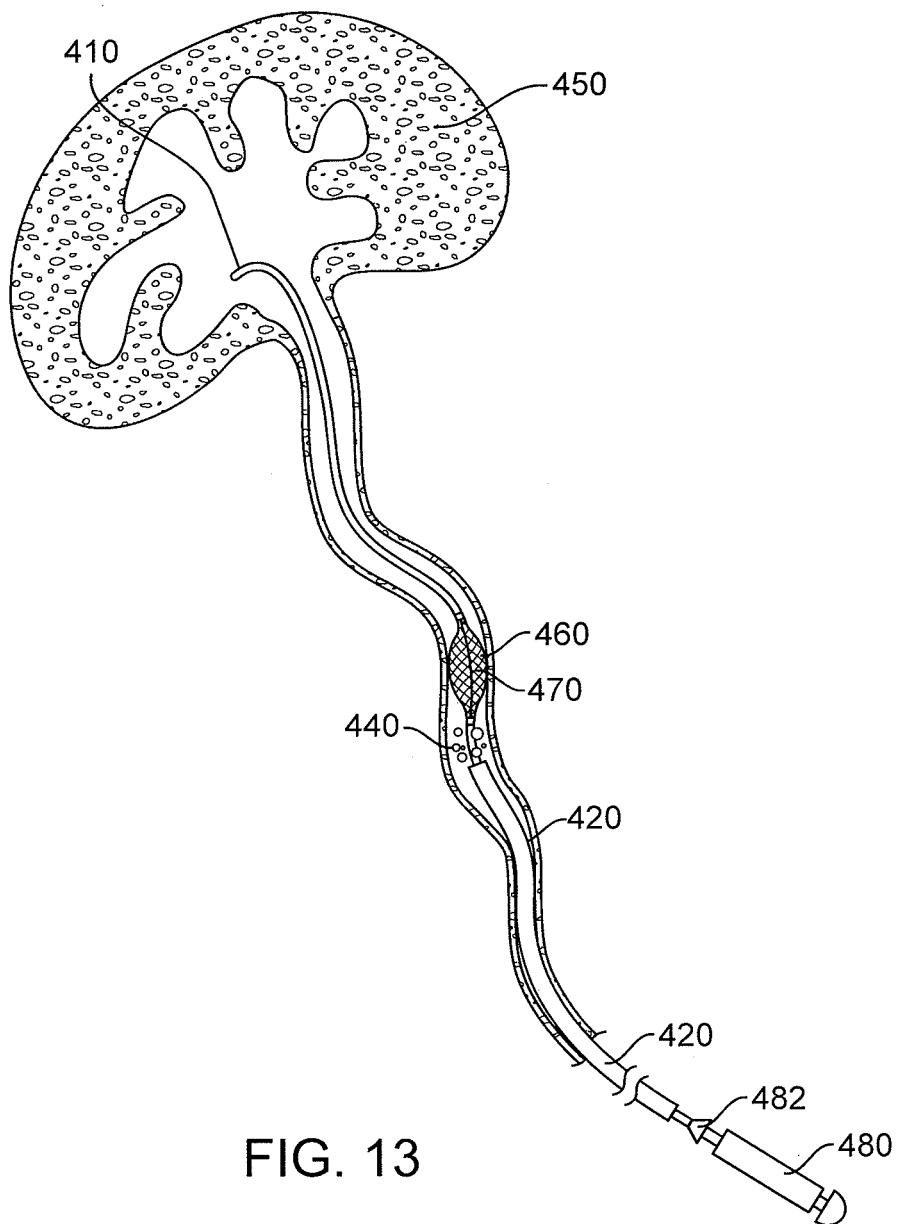

11 / 17

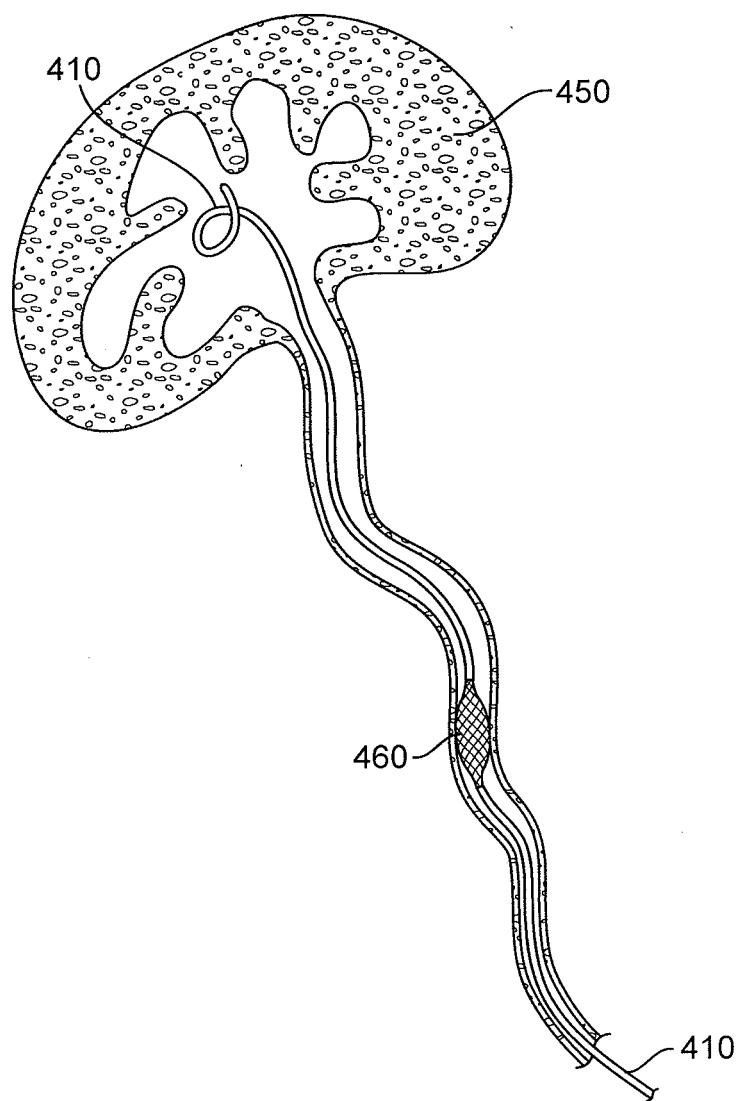


FIG. 14

12 / 17

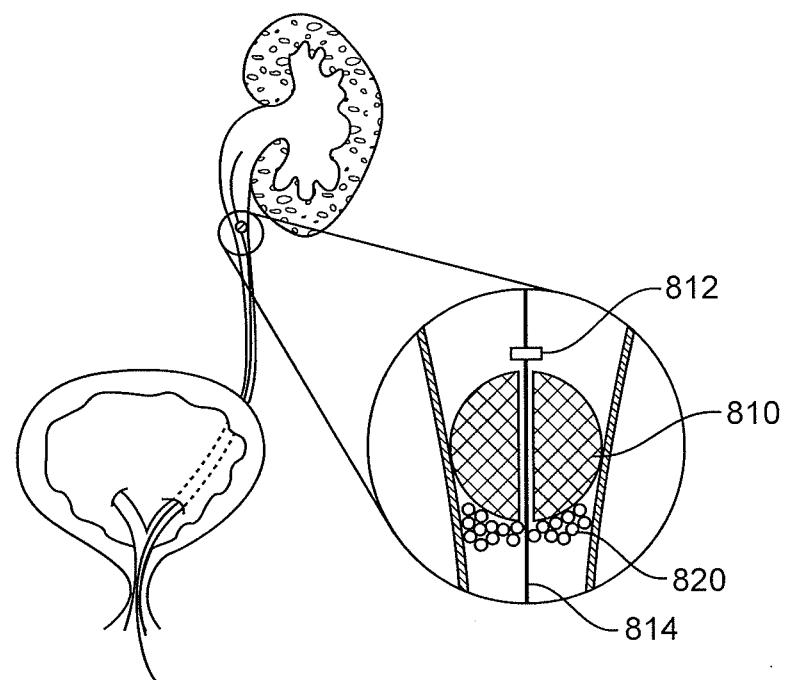


FIG. 15A

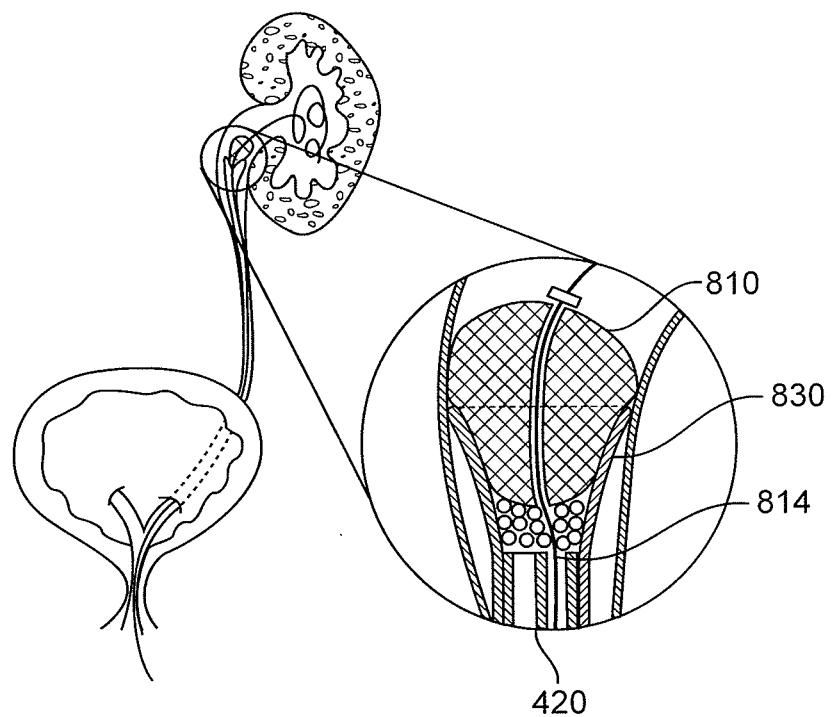


FIG. 15B

13 / 17

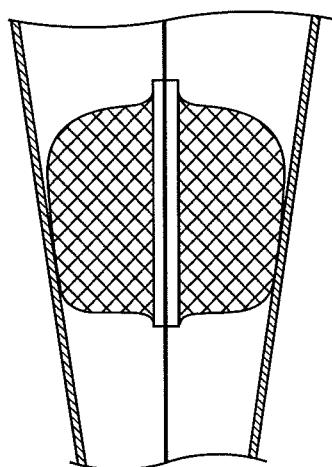


FIG. 16A

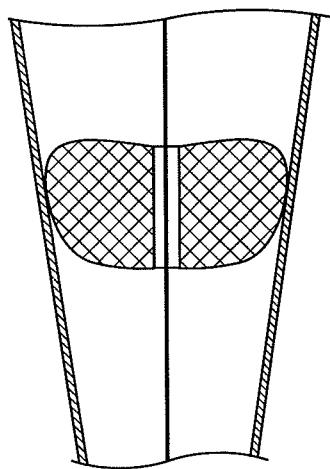


FIG. 16B

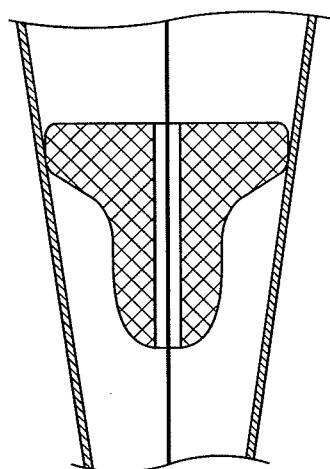


FIG. 16C

14 / 17

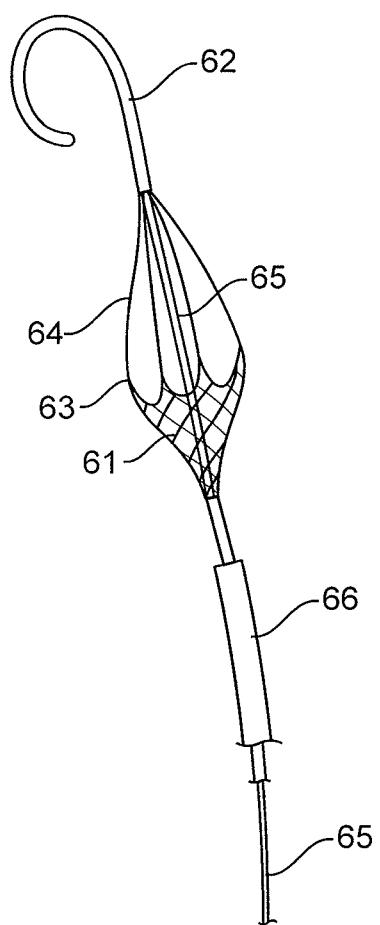


FIG. 17

15 / 17

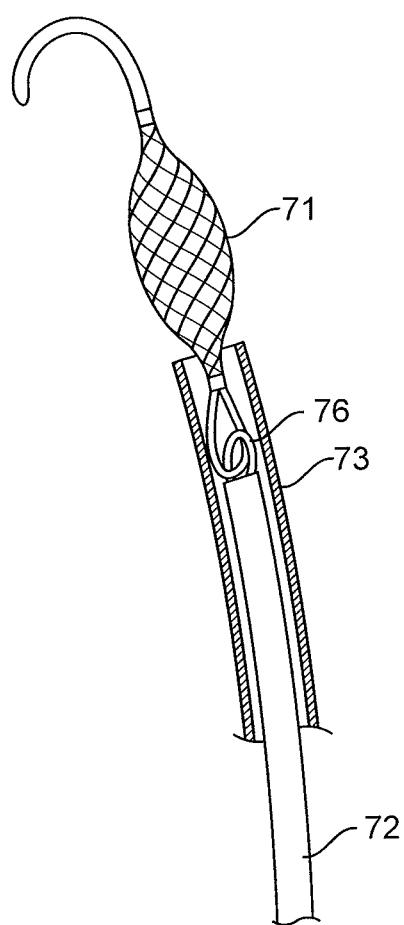


FIG. 18

16 / 17

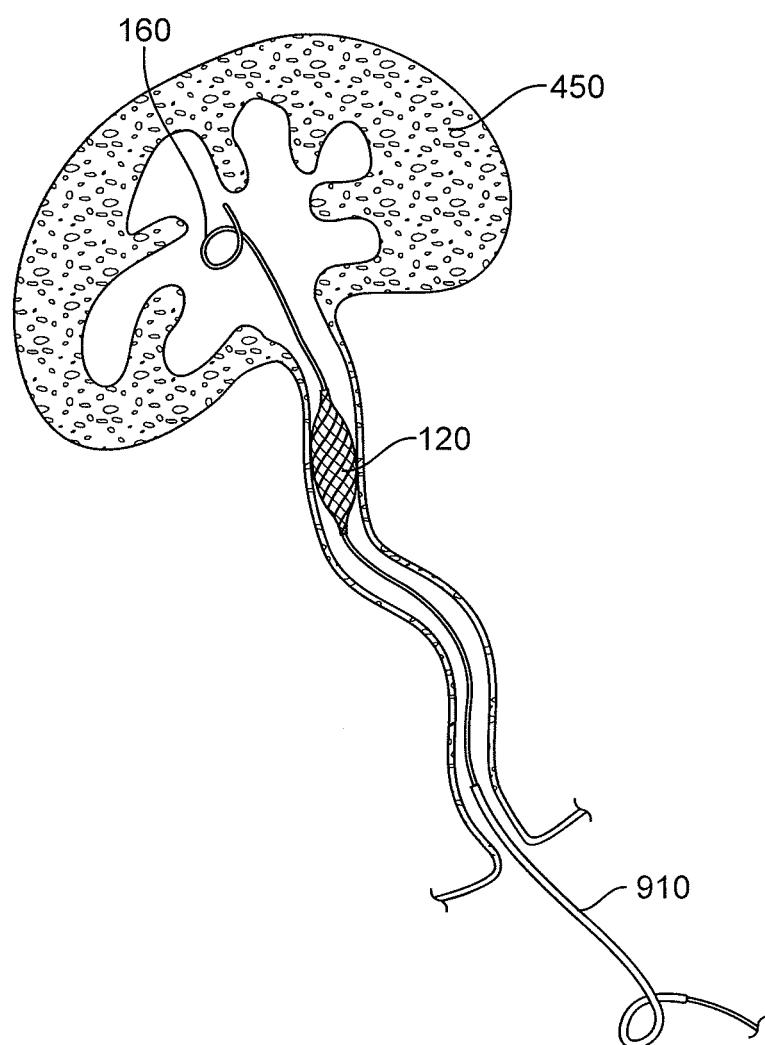


FIG. 19

17 / 17

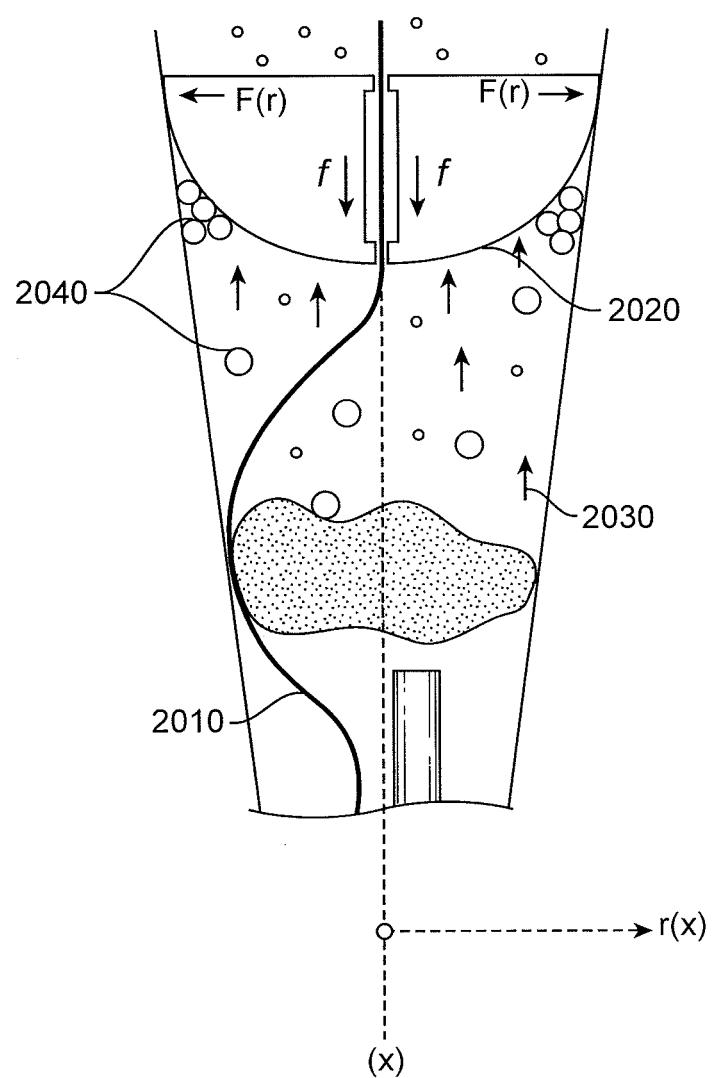


FIG. 20

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2011/029219

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 17/22 (2011.01)

USPC - 606/127

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC(8) - A61B 17/22, 17/94, 17/221; A61M 25/00, 29/00 (2011.01)

USPC - 600/1, 200; 606/127, 159, 198, 200

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

PatBase

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2006/0224178 A1 (CHENG) 05 October 2006 (05.10.2006) entire document	30, 32-34
---		-----
Y		2-3, 5, 12, 18, 21-22, 26, 29, 31
X	US 6,096,053 A (BATES) 01 August 2000 (01.08.2000) entire document	1, 6-7, 9-11, 13, 16-17, 19-20, 23-25
---		-----
Y		2-5, 8, 12, 14-15, 18, 21-22, 26-29
Y	US 7,241,308 B2 (ANDREAS et al) 10 July 2007 (10.07.2007) entire document	4, 28, 31
Y	US 2007/0016244 A1 (BEHL et al) 18 January 2007 (18.01.2007) entire document	8, 14, 27
Y	US 2009/0112253 A1 (NEILAN) 30 April 2009 (30.04.2009) entire document	15

Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance
 "E" earlier application or patent but published on or after the international filing date
 "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
 "O" document referring to an oral disclosure, use, exhibition or other means
 "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
 "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
 "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
 "&" document member of the same patent family

Date of the actual completion of the international search

10 May 2011

Date of mailing of the international search report

20 MAY 2011

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
 P.O. Box 1450, Alexandria, Virginia 22313-1450
 Facsimile No. 571-273-3201

Authorized officer:

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300
 PCT OSP: 571-272-7774

专利名称(译)	可扩展的设备和使用方法		
公开(公告)号	EP2552328A4	公开(公告)日	2017-06-28
申请号	EP2011763223	申请日	2011-03-21
[标]申请(专利权)人(译)	捕虏体MEDICAL		
申请(专利权)人(译)	捕虏体医疗有限公司		
当前申请(专利权)人(译)	捕虏体医疗有限公司		
[标]发明人	SHOHAT SHAUL TAMIR IDAN KILEMNIK IDO		
发明人	SHOHAT, SHAUL TAMIR, IDAN KILEMNIK, IDO		
IPC分类号	A61B17/22		
CPC分类号	A61B17/22 A61B17/221 A61B2017/22042 A61B2017/22047 A61B2017/22074 A61B2017/2212 A61B2017/320716 A61F2/013 A61F2002/015		
代理机构(译)	MAIWALD专利ADVOCATE GMBH		
优先权	61/319931 2010-04-01 US		
其他公开文献	EP2552328A1		
外部链接	Espacenet		

摘要(译)

一种筛分装置和相关方法，包括安装在手术导丝上的可膨胀筛。可膨胀筛可以是自膨胀编织过滤器，其在轴向固定位置安装在导丝上，或者可在多个方向上移动。在实际的石头碎片整理(碎石术)阶段之前，筛分装置可以在阻塞的输尿管或其他体腔中展开，例如在除石过程开始时。可膨胀筛可以设置在阻塞性结石的远侧并且扩展以跨越整个局部输尿管横截面，以便保持大于预定尺寸的石碎片在碎石期间在高灌注速率/压力下向远侧向肾移动。