



US007377920B2

(12) **United States Patent**
Buyse et al.

(10) **Patent No.:** **US 7,377,920 B2**
(45) **Date of Patent:** **May 27, 2008**

(54) **LAPAROSCOPIC BIPOLAR
ELECTROSURGICAL INSTRUMENT**

(75) Inventors: **Steven P. Buyse**, Longmont, CO (US);
Kate R. Lawes, Superior, CO (US);
Dale F. Schmaltz, Fort Collins, CO
(US); **Michael J. Lands**, Louisville,
CO (US); **S. Wade Lukianow**, Boulder,
CO (US); **Kristin D. Johnson**,
Louisville, CO (US); **Gary M.**
Couture, Longmont, CO (US); **Lap P.**
Nguyen, Longmont, CO (US)

(73) Assignee: **Sherwood Services AG**, Schaffhausen
(CH)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 400 days.

(21) Appl. No.: **11/122,346**

(22) Filed: **May 5, 2005**

(65) **Prior Publication Data**
US 2005/0240179 A1 Oct. 27, 2005

Related U.S. Application Data

(63) Continuation of application No. 10/164,654, filed on
Jun. 6, 2002, now abandoned, which is a continua-
tion-in-part of application No. 09/591,330, filed on
Jun. 9, 2000, now Pat. No. 6,451,018, which is a
continuation of application No. 08/970,472, filed on
Nov. 14, 1997, now Pat. No. 6,228,083.

(51) **Int. Cl.**
A61B 18/14 (2006.01)

(52) **U.S. Cl.** **606/50**; 606/46; 606/48;
606/207; 606/208

(58) **Field of Classification Search** 606/46,
606/48-52

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

371,664 A 10/1887 Brannan et al.

(Continued)

FOREIGN PATENT DOCUMENTS

CA 2104423 2/1994

(Continued)

OTHER PUBLICATIONS

Sigel et al. "The Mechanism of Blood Vessel Closure by High
Frequency Electrocoagulation" Surgery Gynecology & Obstetrics,
Oct. 1965 pp. 823-831.


(Continued)

Primary Examiner—Lee S. Cohen

(57) **ABSTRACT**

A laparoscopic bipolar electrosurgical instrument for sealing
tissue includes a handle having an elongated tube affixed
thereto. The tube includes first and second jaw members
having electrically conductive sealing surfaces attached to a
distal end thereof which are movable from a first position for
approximating tissue to a second position for grasping tissue
therebetween. The handle includes a fixed handle and a
handle which is movable relative to the fixed handle to effect
movement of the jaw members from the first position to the
second position for grasping tissue. The jaw members connect
to a source of electrosurgical energy such that the opposable
sealing surfaces are capable of conducting electrosurgical
energy through tissue held therebetween. A stop is included
for maintaining a minimum separation distance between
opposing sealing surfaces. A ratchet is also included to
maintain a closure force in the range of about 7 kg/cm² to
about 13 kg/cm² between opposing sealing surfaces.

8 Claims, 5 Drawing Sheets

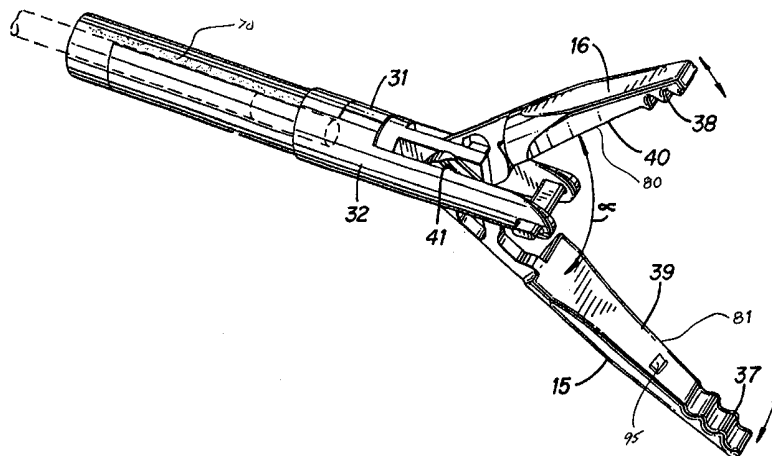

U.S. PATENT DOCUMENTS					
702,472 A	6/1902	Pignolet	5,258,006 A	11/1993	Rydell et al.
728,883 A	5/1903	Downes	5,261,918 A	11/1993	Phillips et al.
1,586,645 A	6/1926	Bierman	5,275,615 A	1/1994	Rose
2,002,594 A	5/1935	Wappler et al.	5,277,201 A	1/1994	Stern
2,011,169 A	8/1935	Wappler	5,282,799 A	2/1994	Rydell
2,031,682 A	2/1936	Wappler et al.	5,290,286 A	3/1994	Parins
2,176,479 A	10/1939	Willis	5,304,203 A	4/1994	El-Mallawany et al.
2,305,156 A	12/1942	Grubel	5,308,357 A	5/1994	Lichtman
2,632,661 A	8/1948	Cristofv	5,318,589 A	6/1994	Lichtman
2,668,538 A	2/1954	Baker	5,324,289 A	6/1994	Eggers
2,796,065 A	6/1957	Kapp	5,330,471 A	7/1994	Eggers
3,459,187 A	8/1969	Pallotta	5,334,183 A	8/1994	Wuchinich
3,643,663 A	2/1972	Sutter	5,334,215 A	8/1994	Chen
3,651,811 A	3/1972	Hildebrandt et al.	5,336,221 A	8/1994	Anderson
3,862,630 A	1/1975	Balamuth	5,342,359 A	8/1994	Rydell
3,866,610 A	2/1975	Kletschka	5,342,381 A	8/1994	Tidemand
3,911,766 A	10/1975	Fridolph et al.	5,342,393 A	8/1994	Stack
3,920,021 A	11/1975	Hiltebrandt	5,352,222 A	10/1994	Rydell
3,921,641 A	11/1975	Hulka	5,354,271 A	10/1994	Voda
3,938,527 A	2/1976	Rioux et al.	5,356,408 A	10/1994	Rydell
3,952,749 A	4/1976	Fridolph et al.	5,366,477 A	11/1994	LeMarie, III et al.
3,970,088 A	7/1976	Morrison	5,368,600 A	11/1994	Failla et al.
3,987,795 A	10/1976	Morrison	5,383,897 A	1/1995	Wholey
4,005,714 A	2/1977	Hiltebrandt	5,389,098 A	2/1995	Tsuruta et al.
4,041,952 A	8/1977	Morrison, Jr. et al.	5,389,104 A	2/1995	Hahnen et al.
4,043,342 A	8/1977	Morrison, Jr.	5,391,166 A	2/1995	Eggers
4,074,718 A	2/1978	Morrison, Jr.	5,391,183 A	2/1995	Janzen et al.
4,088,134 A	5/1978	Mazzariello	5,396,900 A	3/1995	Slater et al.
4,112,950 A	9/1978	Pike	5,403,312 A	4/1995	Yates et al.
4,127,222 A	11/1978	Adams	5,411,519 A	5/1995	Tovey et al.
4,128,099 A	12/1978	Bauer	5,411,520 A	5/1995	Nash et al.
4,165,746 A	8/1979	Burgin	5,413,571 A	5/1995	Katsaros et al.
4,300,564 A	11/1981	Furihata	5,415,657 A	5/1995	Taymor-Luria
4,370,980 A	2/1983	Lottick	5,422,567 A	6/1995	Matsunaga
4,416,276 A	11/1983	Newton et al.	5,423,810 A	6/1995	Goble et al.
4,452,246 A	6/1984	Bader et al.	5,425,739 A	6/1995	Jessen
4,492,231 A	1/1985	Auth	5,429,616 A	7/1995	Schaffer
4,552,143 A	11/1985	Lottick	5,431,674 A	7/1995	Basile et al.
4,574,804 A	3/1986	Kurwa	5,437,292 A	8/1995	Kipshidze et al.
4,597,379 A	7/1986	Kihn et al.	5,438,302 A	8/1995	Goble
4,600,007 A	7/1986	Lahodny et al.	5,441,517 A	8/1995	Kensey et al.
4,655,216 A	4/1987	Tischer	5,443,463 A	8/1995	Stern et al.
4,657,016 A	4/1987	Garito et al.	5,443,464 A	8/1995	Russell et al.
4,662,372 A	5/1987	Sharkany et al.	5,443,480 A	8/1995	Jacobs et al.
4,671,274 A	6/1987	Sorochenko	5,445,638 A	8/1995	Rydell et al.
4,685,459 A	8/1987	Xoch et al.	5,445,658 A	8/1995	Durrrfeld et al.
D295,893 S	5/1988	Sharkany et al.	5,451,224 A	9/1995	Goble et al.
D295,894 S	5/1988	Sharkany et al.	5,456,684 A	10/1995	Schmidt et al.
4,763,669 A	8/1988	Jaeger	5,458,598 A	10/1995	Feinberg et al.
4,827,929 A	5/1989	Hodge	5,460,629 A	10/1995	Shlain et al.
4,887,612 A	12/1989	Esser et al.	5,462,546 A	10/1995	Rydell
4,938,761 A	7/1990	Ensslin	5,472,443 A	12/1995	Cordis et al.
4,985,030 A	1/1991	Melzer et al.	5,478,351 A	12/1995	Meade et al.
5,007,908 A	4/1991	Rydell	5,480,409 A	1/1996	Riza
5,026,370 A	6/1991	Lottick	5,484,436 A	1/1996	Eggers et al.
5,084,057 A	1/1992	Green et al.	5,496,317 A	3/1996	Goble et al.
5,099,840 A	3/1992	Goble et al.	5,496,347 A	3/1996	Hashiguchi et al.
5,116,332 A	5/1992	Lottick	5,499,997 A	3/1996	Sharpe et al.
5,147,357 A	9/1992	Rose et al.	5,509,922 A	4/1996	Aranyi et al.
5,151,102 A	9/1992	Xamiyama et al.	5,514,134 A	5/1996	Rydell et al.
5,176,695 A	1/1993	Dulebohn	5,527,313 A	6/1996	Scott et al.
5,190,541 A	3/1993	Abele et al.	5,531,744 A	7/1996	Nardella et al.
5,196,009 A	3/1993	Kirwan, Jr.	5,536,251 A	7/1996	Evard et al.
5,197,964 A	3/1993	Parins	5,540,684 A	7/1996	Hassler, Jr.
5,215,101 A	6/1993	Jacobs et al.	5,540,685 A	7/1996	Parins et al.
5,217,457 A	6/1993	Delahuerga et al.	5,540,715 A	7/1996	Katsaros et al.
5,217,458 A	6/1993	Parins	5,542,945 A	8/1996	Fritzsche
5,217,460 A	6/1993	Knoepfler	5,558,672 A	9/1996	Edwards et al.
5,219,354 A	6/1993	Choudhury et al.	5,562,699 A	10/1996	Heimberger et al.
5,244,462 A	9/1993	Delahuerga et al.	5,569,241 A	10/1996	Edwardds
5,250,047 A	10/1993	Rydell	5,569,243 A	10/1996	Kortenbach et al.
			5,571,100 A	11/1996	Goble et al.
			5,573,424 A	11/1996	Poppe

5,573,534 A	11/1996	Stone	5,906,630 A	5/1999	Anderhub et al.
5,573,535 A	11/1996	Viklund	5,908,420 A	6/1999	Parins et al.
5,578,052 A	11/1996	Koros et al.	5,911,719 A	6/1999	Eggers
5,582,611 A	12/1996	Tsuruta et al.	5,913,874 A	6/1999	Berns et al.
5,585,896 A	12/1996	Yamazaki et al.	5,921,984 A	7/1999	Sutcu et al.
5,590,570 A	1/1997	LeMaire, III et al.	5,925,043 A	7/1999	Kumar et al.
5,601,601 A	2/1997	Tal et al.	5,935,126 A	8/1999	Riza
5,603,711 A	2/1997	Parins et al.	5,944,718 A	8/1999	Austin et al.
5,603,723 A	2/1997	Aranyi et al.	5,951,549 A	9/1999	Richardson et al.
5,611,798 A	3/1997	Eggers	5,954,720 A	9/1999	Wilson et al.
5,626,578 A	5/1997	Tihon	5,957,923 A	9/1999	Hahnen et al.
5,626,609 A	5/1997	Zvenyatsky et al.	5,961,514 A	10/1999	Long et al.
5,630,833 A	5/1997	Katsaros et al.	5,976,132 A	11/1999	Morris
5,637,110 A	6/1997	Pennybacker et al.	5,984,939 A	11/1999	Yoon
5,643,294 A	7/1997	Tovey et al.	5,989,277 A	11/1999	LeMaire, III et al.
5,647,869 A	7/1997	Goble et al.	6,004,335 A	12/1999	Vaitekunas et al.
5,647,871 A	7/1997	Levine et al.	6,010,516 A	1/2000	Hulka et al.
5,649,959 A	7/1997	Hannam et al.	6,024,741 A	2/2000	Williamson et al.
5,658,281 A	8/1997	Heard	6,024,744 A	2/2000	Kese et al.
5,662,667 A	9/1997	Knodel	6,030,384 A	2/2000	Nezhat
5,665,100 A	9/1997	Yoon	6,033,399 A	3/2000	Gines
5,667,526 A	9/1997	Levin	6,039,733 A	3/2000	Buyse et al.
5,674,220 A	10/1997	Fox et al.	6,041,679 A	3/2000	Slater et al.
5,681,282 A	10/1997	Eggers et al.	6,050,996 A	4/2000	Schmaltz et al.
5,693,051 A	12/1997	Schulze et al.	6,053,914 A	4/2000	Eggers et al.
5,695,522 A	12/1997	LeMaire, III et al.	6,053,933 A	4/2000	Balazs et al.
5,700,261 A	12/1997	Brinkerhoff	D424,694 S	5/2000	Tetzlaff et al.
5,702,390 A	12/1997	Austin et al.	D425,201 S	5/2000	Tetzlaff et al.
5,707,369 A	1/1998	Vaitekunas et al.	6,059,782 A	5/2000	Novak et al.
5,709,680 A	1/1998	Yates et al.	RE36,795 E	7/2000	Rydell
5,716,366 A	2/1998	Yates	6,083,223 A	7/2000	Baker
5,720,744 A	2/1998	Eggleston et al.	6,086,586 A	7/2000	Hooven
5,727,428 A	3/1998	LeMaire, III et al.	6,090,107 A	7/2000	Borgmeier et al.
5,735,848 A	4/1998	Yates et al.	6,096,037 A	8/2000	Mulier et al.
5,743,906 A	4/1998	Parins et al.	6,099,550 A	8/2000	Yoon
5,755,717 A	5/1998	Yates et al.	6,102,909 A	8/2000	Chen et al.
5,766,130 A	6/1998	Selmonosky	6,110,171 A	8/2000	Rydell
5,766,166 A	6/1998	Hooven	6,113,596 A	9/2000	Hooven et al.
5,766,170 A	6/1998	Eggers	6,113,598 A	9/2000	Baker
5,769,849 A	6/1998	Eggers	6,117,158 A	9/2000	Measamer et al.
5,772,655 A	6/1998	Bauer et al.	6,123,701 A	9/2000	Nezhat
5,772,670 A	6/1998	Brosa	H1904 H	10/2000	Yates et al.
5,776,128 A	7/1998	Eggers	6,126,658 A	10/2000	Baker
5,776,130 A	7/1998	Buyse et al.	6,152,923 A	11/2000	Ryan
5,779,701 A	7/1998	McBrayer et al.	6,162,220 A	12/2000	Nezhat
5,792,137 A	8/1998	Carr et al.	6,174,309 B1	1/2001	Wrublewski et al.
5,792,177 A	8/1998	Kaseda	6,179,834 B1	1/2001	Buyse et al.
5,797,927 A	8/1998	Yoon	6,179,837 B1	1/2001	Hooven
5,797,938 A	8/1998	Paraschac et al.	6,183,467 B1	2/2001	Shapeton et al.
5,797,958 A	8/1998	Yoon	6,187,003 B1	2/2001	Buyse et al.
5,800,449 A	9/1998	Wales	6,190,386 B1	2/2001	Rydell
5,807,393 A	9/1998	Williamson, IV et al.	6,193,718 B1	2/2001	Kortenbach et al.
5,810,808 A	9/1998	Eggers	6,206,876 B1	3/2001	Levine et al.
5,810,811 A	9/1998	Yates et al.	6,206,877 B1	3/2001	Kese et al.
5,810,877 A	9/1998	Roth et al.	6,217,602 B1	4/2001	Redmon
5,814,043 A	9/1998	Shapeton	6,221,039 B1	4/2001	Durgin et al.
5,817,093 A	10/1998	Williamson, IV et al.	6,224,593 B1	5/2001	Ryan et al.
5,820,630 A	10/1998	Lind	6,228,080 B1	5/2001	Gines
5,827,271 A	10/1998	Buyse et al.	6,228,083 B1	5/2001	Lands et al.
5,827,279 A	10/1998	Hughett et al.	6,267,761 B1	7/2001	Ryan
5,827,281 A	10/1998	Levin	6,270,497 B1	8/2001	Sekino et al.
5,833,690 A	11/1998	Yates et al.	6,270,508 B1	8/2001	Klieman et al.
5,843,080 A	12/1998	Fleenor et al.	6,273,887 B1	8/2001	Yamauchi et al.
5,849,022 A	12/1998	Sakashita et al.	6,277,117 B1	8/2001	Tetzlaff et al.
5,853,412 A	12/1998	Mayenberger	6,280,458 B1	8/2001	Boche et al.
5,860,976 A	1/1999	Billings et al.	6,283,961 B1	9/2001	Underwood et al.
5,876,401 A	3/1999	Schulze et al.	D449,886 S	10/2001	Tetzlaff et al.
5,891,141 A	4/1999	Rydell	6,322,561 B1	11/2001	Eggers et al.
5,891,142 A	4/1999	Eggers et al.	6,334,860 B1	1/2002	Dorn
5,893,863 A	4/1999	Yoon	6,334,861 B1	1/2002	Chandler et al.
5,893,875 A	4/1999	O'Connor et al.	6,345,532 B1	2/2002	Coudray et al.
5,893,877 A	4/1999	Gampp, Jr. et al.	6,350,264 B1	2/2002	Hooven
5,902,301 A	5/1999	Olig	6,352,536 B1	3/2002	Buyse et al.

US 7,377,920 B2

Page 4

6,358,249 B1	3/2002	Chen et al.	7,135,020 B2	11/2006	Lawes et al.
D457,958 S	5/2002	Dycus et al.	D533,942 S	12/2006	Kerr et al.
D457,959 S	5/2002	Tetzlaff et al.	7,147,638 B2	12/2006	Chapman et al.
6,387,094 B1	5/2002	Eitenmuller	7,150,097 B2	12/2006	Sremcich et al.
6,398,779 B1	6/2002	Buyse et al.	7,150,749 B2	12/2006	Dycus et al.
6,402,747 B1	6/2002	Lindemann et al.	D535,027 S	1/2007	James et al.
6,409,728 B1	6/2002	Ehr et al.	7,156,846 B2	1/2007	Dycus et al.
H2037 H	7/2002	Yates et al.	7,160,298 B2	1/2007	Lawes et al.
6,419,675 B1	7/2002	Gallo, Sr.	7,160,299 B2	1/2007	Baily
6,425,896 B1	7/2002	Baltschun et al.	7,169,146 B2	1/2007	Truckai et al.
6,440,144 B1	8/2002	Bacher	7,179,258 B2	2/2007	Buyse et al.
6,443,952 B1	9/2002	Mulier et al.	7,195,631 B2	3/2007	Dumbauld
6,443,970 B1	9/2002	Schulze et al.	D541,418 S	4/2007	Schechter et al.
6,451,018 B1	9/2002	Lands et al.	7,207,990 B2	4/2007	Lands et al.
6,458,128 B1	10/2002	Schulze	D541,938 S	5/2007	Kerr et al.
6,458,130 B1	10/2002	Frazier et al.	7,223,265 B2	5/2007	Keppel
6,464,701 B1	10/2002	Hooven et al.	7,232,440 B2	6/2007	Dumbauld et al.
6,464,702 B2	10/2002	Schulze et al.	7,241,296 B2	7/2007	Buyse et al.
6,464,704 B2	10/2002	Schmaltz et al.	7,252,667 B2	8/2007	Moses et al.
6,511,480 B1	1/2003	Tetzlaff et al.	7,255,697 B2	8/2007	Dycus et al.
6,527,771 B1	3/2003	Weadock et al.	7,267,677 B2	9/2007	Johnson et al.
6,585,735 B1	7/2003	Frazier et al.	7,270,660 B2	9/2007	Ryan
6,602,252 B2	8/2003	Mollenauer	7,270,664 B2	9/2007	Johnson et al.
6,620,161 B2	9/2003	Schulze et al.	2002/0013583 A1	1/2002	Camran et al.
6,626,901 B1	9/2003	Treat et al.	2002/0049442 A1	4/2002	Roberts et al.
6,641,595 B1	11/2003	Moran et al.	2002/0099372 A1	7/2002	Schulze et al.
6,652,521 B2	11/2003	Schulze	2002/0107517 A1	8/2002	Witt et al.
6,656,177 B2	12/2003	Truckai et al.	2002/0111624 A1	8/2002	Witt et al.
6,660,072 B2	12/2003	Chatterjee	2002/0188294 A1	12/2002	Couture et al.
6,669,696 B2	12/2003	Bacher et al.	2003/0014052 A1	1/2003	Buyse et al.
6,682,527 B2	1/2004	Strul	2003/0014053 A1	1/2003	Nguyen et al.
6,682,528 B2	1/2004	Frazier et al.	2003/0018331 A1	1/2003	Dycus et al.
6,685,724 B1	2/2004	Haluck	2003/0018332 A1	1/2003	Schmaltz et al.
6,695,840 B2	2/2004	Schulze	2003/0032956 A1	2/2003	Lands et al.
6,702,810 B2	3/2004	McClurken et al.	2003/0069571 A1	4/2003	Treat et al.
6,726,068 B2	4/2004	Miller	2003/0078578 A1	4/2003	Truckai et al.
6,726,686 B2	4/2004	Buyse et al.	2003/0109875 A1	6/2003	Tetzlaff et al.
6,733,498 B2	5/2004	Paton et al.	2003/0114851 A1	6/2003	Truckai et al.
6,743,229 B2	6/2004	Buyse et al.	2003/0139741 A1	7/2003	Goble et al.
6,770,072 B1	8/2004	Truckai et al.	2003/0139742 A1	7/2003	Wampler et al.
6,773,434 B2	8/2004	Ciarrocca	2003/0158549 A1	8/2003	Swanson
6,776,780 B2	8/2004	Mulier et al.	2003/0181910 A1	9/2003	Dycus et al.
6,790,217 B2	9/2004	Schulze et al.	2003/0199869 A1	10/2003	Johnson et al.
D496,997 S	10/2004	Dycus et al.	2003/0216732 A1	11/2003	Truckai et al.
6,802,843 B2	10/2004	Truckai et al.	2003/0220637 A1	11/2003	Truckai et al.
D499,181 S	11/2004	Dycus et al.	2003/0229344 A1	12/2003	Dycus et al.
6,818,000 B2	11/2004	Muller et al.	2003/0236325 A1	12/2003	Bonora
6,860,880 B2	3/2005	Treat et al.	2004/0030330 A1	2/2004	Brassell et al.
6,887,240 B1	5/2005	Lands et al.	2004/0030332 A1	2/2004	Knowlton et al.
6,926,716 B2	8/2005	Baker et al.	2004/0049185 A1	3/2004	Latterell et al.
6,929,644 B2	8/2005	Truckai et al.	2004/0064151 A1	4/2004	Mollenauer
6,932,810 B2	8/2005	Ryan	2004/0082952 A1	4/2004	Dycus et al.
6,932,816 B2	8/2005	Phan	2004/0087943 A1	5/2004	Dycus et al.
6,942,662 B2	9/2005	Goble et al.	2004/0115296 A1	6/2004	Duffin
6,960,210 B2	11/2005	Lands et al.	2004/0116924 A1	6/2004	Dycus et al.
6,964,662 B2	11/2005	Kidooka	2004/0116979 A1	6/2004	Truckai et al.
6,994,707 B2	2/2006	Ellman et al.	2004/0122423 A1	6/2004	Dycus et al.
7,011,657 B2	3/2006	Truckai et al.	2004/0143263 A1	7/2004	Schechter et al.
7,033,354 B2	4/2006	Keppel	2004/0147925 A1	7/2004	Buyse et al.
7,052,496 B2	5/2006	Yamauchi	2004/0162557 A1	8/2004	Tetzlaff et al.
D525,361 S	7/2006	Hushka	2004/0176762 A1	9/2004	Lawes et al.
7,083,618 B2	8/2006	Couture et al.	2004/0193153 A1	9/2004	Sarter et al.
7,090,673 B2	8/2006	Dycus et al.	2004/0225288 A1	11/2004	Buyse et al.
7,101,371 B2	9/2006	Dycus et al.	2004/0230189 A1	11/2004	Keppel
7,101,372 B2	9/2006	Dycus et al.	2004/0236325 A1	11/2004	Tetzlaff et al.
7,101,373 B2	9/2006	Dycus et al.	2004/0243125 A1	12/2004	Dycus et al.
7,103,947 B2	9/2006	Sartor et al.	2004/0249371 A1	12/2004	Dycus et al.
7,112,199 B2	9/2006	Cosmesecu	2004/0249374 A1	12/2004	Tetzlaff et al.
D531,311 S	10/2006	Guerra et al.	2004/0250419 A1	12/2004	Sremcich et al.
7,118,570 B2	10/2006	Tetzlaff et al.	2004/0254573 A1	12/2004	Dycus et al.
7,118,587 B2	10/2006	Dycus et al.	2005/0004564 A1	1/2005	Wham et al.
7,131,970 B2	11/2006	Moses et al.	2005/0004568 A1	1/2005	Lawes et al.
7,131,971 B2	11/2006	Dycus et al.	2005/0004570 A1	1/2005	Chapman et al.

2005/0021025 A1	1/2005	Buyse et al.	EP	0623316 A1	11/1994
2005/0021026 A1	1/2005	Baily	EP	0624348 A2	11/1994
2005/0021027 A1	1/2005	Shields et al.	EP	0650701 A1	5/1995
2005/0033278 A1	2/2005	McClurken et al.	EP	0694290 A3	3/1996
2005/0101951 A1	5/2005	Wham et al.	EP	0717966 A1	6/1996
2005/0101952 A1	5/2005	Lands et al.	EP	0754437 A3	3/1997
2005/0107784 A1	5/2005	Moses et al.	EP	853922 A1	7/1998
2005/0107785 A1	5/2005	Dycus et al.	EP	0875209 A1	11/1998
2005/0113818 A1	5/2005	Sartor et al.	EP	0878169 A1	11/1998
2005/0113819 A1	5/2005	Wham et al.	EP	0887046 A3	1/1999
2005/0113826 A1	5/2005	Johnson et al.	EP	0923907 A1	6/1999
2005/0113827 A1	5/2005	Dumbauld et al.	EP	0986990 A1	3/2000
2005/0113828 A1	5/2005	Shields et al.	EP	1034747 A1	9/2000
2005/0119655 A1	6/2005	Moses et al.	EP	1034748 A1	9/2000
2005/0149151 A1	7/2005	Orszulak et al.	EP	1034746 A3	10/2000
2006/0064085 A1	3/2006	Schechter et al.	EP	1035807 A3	10/2000
2006/0079891 A1	4/2006	Arts et al.	EP	1050278 A1	11/2000
2006/0129146 A1	6/2006	Dycus et al.	EP	1053719 A1	11/2000
2006/0161150 A1	7/2006	Keppel	EP	1053720 A1	11/2000
2006/0167450 A1	7/2006	Johnson et al.	EP	1055399 A1	11/2000
2006/0167452 A1	7/2006	Moses et al.	EP	1055400 A1	11/2000
2006/0173452 A1	8/2006	Buyse et al.	EP	1080694 A1	3/2001
2006/0189980 A1	8/2006	Johnson et al.	EP	1082944 A1	3/2001
2006/0189981 A1	8/2006	Dycus et al.	EP	1159926 A2	12/2001
2006/0190035 A1	8/2006	Hushka et al.	EP	1301135 A	4/2003
2006/0217709 A1	9/2006	Couture et al.	EP	1330991 A1	7/2003
2006/0224158 A1	10/2006	Odom et al.	EP	1486177 A2	6/2004
2006/0259036 A1	11/2006	Tetzlaff et al.	EP	1472984 A1	11/2004
2006/0264922 A1	11/2006	Sartor et al.	EP	1530952 A1	5/2005
2006/0264931 A1	11/2006	Chapman et al.	EP	1532932 A1	5/2005
2006/0271038 A1	11/2006	Johnson et al.	EP	1632192 A1	3/2006
2007/0043352 A1	2/2007	Garrison et al.	EP	1645238 A1	4/2006
2007/0043353 A1	2/2007	Dycus et al.	EP	1707143 A1	10/2006
2007/0055231 A1	3/2007	Dycus et al.	GB	2214430 A	6/1989
2007/0062017 A1	3/2007	Dycus et al.	JP	501068	9/1984
2007/0074807 A1	4/2007	Guerra	JP	502328	3/1992
2007/0078456 A1	4/2007	Dumbauld et al.	JP	5-40112	2/1993
2007/0078458 A1	4/2007	Dumbauld et al.	JP	06343644 A2	12/1994
2007/0078459 A1	4/2007	Johnson et al.	JP	07265328 A2	10/1995
2007/0088356 A1	4/2007	Moses et al.	JP	08056955 A2	3/1996
2007/0106295 A1	5/2007	Garrison et al.	JP	08252263 A2	10/1996
2007/0106297 A1	5/2007	Dumbauld et al.	JP	09010223 A2	1/1997
2007/0118111 A1	5/2007	Weinberg	JP	11244298 A2	9/1999
2007/0118115 A1	5/2007	Artale et al.	JP	2000342599 A2	12/2000
2007/0142833 A1	6/2007	Dycus et al.	JP	2000350732 A2	12/2000
2007/0142834 A1	6/2007	Dumbauld	JP	2001008944 A2	1/2001
2007/0156139 A1	7/2007	Schechter et al.	JP	2001029356 A2	2/2001
2007/0156140 A1	7/2007	Baily	JP	2001128990 A2	5/2001
2007/0173811 A1	7/2007	Couture et al.	SU	401367	10/1973
2007/0173814 A1	7/2007	Hixson et al.	SU	401367	11/1974
2007/0179499 A1	8/2007	Garrison	WO	WO89/00757	1/1989
2007/0203485 A1	8/2007	Keppel	WO	WO 92/06642	4/1992
2007/0213706 A1	9/2007	Dumbauld et al.	WO	WO 94/08524 A	4/1994
2007/0213707 A1	9/2007	Dumbauld et al.	WO	WO94/20025	9/1994
2007/0213708 A1	9/2007	Dumbauld et al.	WO	WO 95/02369	1/1995
2007/0213712 A1	9/2007	Buyse et al.	WO	WO 95/07662	3/1995

FOREIGN PATENT DOCUMENTS

DE	2415263	10/1975	WO	WO95/15124	6/1995
DE	2627679	1/1977	WO	WO96/05776	2/1996
DE	8712328	3/1988	WO	WO 96/22056	7/1996
DE	4303882	8/1994	WO	WO 96/13218	9/1996
DE	29616210	1/1997	WO	WO 97/00646	1/1997
DE	19608716	4/1997	WO	WO 97/00647	1/1997
DE	19751106	5/1998	WO	WO97/10764	3/1997
DE	19751108	5/1999	WO	WO 97/10764	3/1997
EP	0364216 A1	4/1990	WO	WO 97/24073	7/1997
EP	518230 A1	12/1992	WO	WO 97/24993	7/1997
EP	0 541 930 B1	5/1993	WO	WO 98/27880	7/1998
EP	0572131	12/1993	WO	WO 99/03407	1/1999
EP	584787 A1	3/1994	WO	WO 99/03408	1/1999
EP	0589453 A2	3/1994	WO	WO 99/03409	1/1999
			WO	WO 99/12488	3/1999
			WO	WO 99/40857	8/1999

WO	WO 99/40881	8/1999
WO	WO 99/51158	10/1999
WO	WO 99/66850	12/1999
WO	WO 99/66850 A	12/1999
WO	WO 00/24330	5/2000
WO	WO 00/24331	5/2000
WO	WO00/24331	5/2000
WO	WO 00/41638	7/2000
WO	WO00/47124	8/2000
WO	WO 00/53112	9/2000
WO	WO 01/17448 A	3/2001
WO	WO 01/54604	8/2001
WO	WO02/07627	1/2002
WO	WO 02/07627	1/2002
WO	WO02/080783	10/2002
WO	WO 02/080783	10/2002
WO	WO 02/080784	10/2002
WO	WO02/080784	10/2002
WO	WO02/080785	10/2002
WO	WO 02/080785	10/2002
WO	WO02/080786	10/2002
WO	WO 02/080786	10/2002
WO	WO 02/080793	10/2002
WO	WO02/080793	10/2002
WO	WO02/080794	10/2002
WO	WO 02/080794	10/2002
WO	WO 02/080795	10/2002
WO	WO 02/080796	10/2002
WO	WO02/080797	10/2002
WO	WO 02/080797	10/2002
WO	WO 02/080798	10/2002
WO	WO 02/080799	10/2002
WO	WO 02/081170	10/2002
WO	WO02/081170	10/2002
WO	WO 03/101311	12/2003
WO	WO2004/032777	4/2004
WO	WO 2004/032777	4/2004
WO	WO 2004/052221	6/2004
WO	WO 2004/073490	9/2004
WO	WO2004/073490	9/2004
WO	WO2004/073753	9/2004
WO	WO 2004/082495	9/2004
WO	WO 2004/098383	11/2004
WO	WO 2004/103156	12/2004
WO	WO2005/004735	1/2005
WO	WO 2005/110264	11/2005

OTHER PUBLICATIONS

Bergdahl et al. "Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator" *J. Neurosurg.* vol. 75, Jul. 1991, pp. 148-151.

Kennedy et al. "High-burst-strength, feedback-controlled bipolar vessel sealing" *Surgical Endoscopy* (1998) 12: 876-878.

Peterson et al. "Comparison of Healing Process Following Ligation with Sutures and Bipolar Vessel Sealing" *Surgical Technology International* (2001).

Linehan et al. "A Phase I Study of the LigaSure Vessel Sealing System in Hepatic Surgery" Section of HPB Surgeon, Washington University School of Medicine, St. Louis MO, Presented at AHPBA, Feb. 2001.

Johnson et al. "Evaluation of the LigaSure Vessel Sealing System in Hemorrhoidectomy" American College of Surgeons (ACS) Clinica Congress Poster (2000).

Sayfan et al. "Sutureless Closed Hemorrhoidectomy: A New Technique" *Annals of Surgery* vol. 234 No. 1 Jul. 2001 pp. 21-24.

Heniford et al. "Initial Results with an Electrothermal Bipolar Vessel Sealer" *Surgical Endoscopy* (2000) 15:799-801.

Heniford et al. "Initial Research and Clinical Results with an Electrothermal Bipolar Vessel Sealer" Oct. 1999.

McLellan et al. "Vessel Sealing for Hemostasis During Pelvic Surgery" Int'l Federation of Gynecology and Obstetrics FIGO World Congress 2000, Washington, D.C.

Levy et al. "Use of a New Energy-based Vessel Ligation Device During Vaginal Hysterectomy" Int'l Federation of Gynecology and Obstetrics (FIGO) World Congress.

Crawford et al. "Use of the LigaSure Vessel Sealing System in Urologic Cancer Surgery" *Grand Rounds in Urology* 1999 vol. 1 Issue 4 pp. 10-17.

Rothenberg et al. "Use of the LigaSure Vessel Sealing System in Minimally Invasive Surgery in Children" Int'l Pediatric Endosurgery Group (IPEG) 2000.

Palazzo et al. "Randomized clinical trial of Ligasure versus open haemorrhoidectomy" *British Journal of Surgery* 2002, 89, 154-157.

"Innovations in Electrosurgery" Sales/Product Literature, Dec. 31, 2000.

LigaSure Vessel Sealing System, the Seal of Confidence in General, Gynecologic, Urologic, and Laparoscopic Surgery Sales/Product Literature, Jan. 2004.

Carbonell et al., "Comparison of the Gyros PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC.

"Reducing Needlestick Injuries in the Operating Room" Sales/Product Literature.

Chung et al., "Clinical Experience of Sutureless Closed Hemorrhoidectomy with LigaSure" *Diseases of the Colon & Rectum* vol. 46, No. 1 Jan. 2003.

Strasberg et al., "Use of a Bipolar Vessel-Sealing Device for Parenchymal Transection During Liver Surgery" *Journal of Gastrointestinal Surgery*, vol. 6, No. 4, Jul./Aug. 2002 pp. 569-574.

Paul G. Horgan, "A Novel Technique for Parenchymal Division During Hepatectomy" *The American Journal of Surgery*, vol. 181, No.3, Apr. 2001 pp. 236-237.

W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery" Sales/Product Literature.

Michael Choti, "Abdominoperineal Resection with the LigaSure Vessel Sealing System and LigaSure Atlas 20 cm Open Instrument" *Innovations That Work*, Jun. 2003.

Craig Johnson, "Use of the LigaSure Vessel Sealing System in Bloodless Hemorrhoidectomy" *Innovations That Work*, Mar. 2000.

Muller et al., "Extended Left Hemicolectomy Using the LigaSure Vessel Sealing System" *Innovations That Work*, Sep. 1999.

Herman et al., "Laparoscopic Intestinal Resection With the LigaSure Vessel Sealing System: A Case Report" *Innovations That Work*, Feb. 2002.

Carus et al., "Initial Experience With The LigaSure Vessel Sealing System in Abdominal Surgery" *Innovations That Work*, Jun. 2002.

Levy et al. "Randomized Trial of Suture Versus Electrosurgical Bipolar Vessel Sealing in Vaginal Hysterectomy" *Obstetrics & Gynecology*, vol. 102, No. 1, Jul. 2003.

Levy et al., "Update on Hysterectomy—New Technologies and Techniques" *OBG Management*, Feb. 2003.

Barbara Levy, "Use of a New Vessel Ligation Device During Vaginal Hysterectomy" FIGO 2000, Washington, D.C.

McLellan et al. "Vessel Sealing For Hemostasis During Gynecologic Surgery" Sales/Product Literature.

Sengupta et al., "Use of a Computer-Controlled Bipolar Diathermy System in Radical Prostatectomies and Other Open Urological Surgery" *ANZ Journal of Surgery* (2001) 71.9 pp. 538-540.

Olsson et al. "Radical Cystectomy In Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3, 2001.


E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Venous Complex" Sales/Product Literature.

Jarrett et al., "Use of the LigaSure Vessel Sealing System for Peri-Hilar Vessels in Laparoscopic Nephrectomy" Sales/Product Literature.

E. David Crawford "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" Sales/Product Literature.

Joseph Ortenberg "LigaSure System Used in Laparoscopic 1st and 2nd Stage Orchiopexy" *Innovations That Work*, Nov. 2002.

- Koyle et al., "Laparoscopic Palomo Varicocele Ligation in Children and Adolescents" *Pediatric Endosurgery & Innovative Techniques*, vol. 6, No. 1, 2002.
- Dulemba et al. "Use of a Bipolar Electrothermal Vessel Sealer in Laparoscopically Assisted Vaginal Hysterectomy" *Sales/Product Literature*; Jan. 2004.
- Johnson et al. "Evaluation of a Bipolar electrothermal Vessel Sealing Device in Hemorrhoidectomy" *Sales/Product Literature*; Jan. 2004.
- Int'l Search Report PCT/US98/18640.
- Int'l Search Report PCT/US98/23950.
- Int'l Search Report PCT/US99/24869.
- Int'l Search Report PCT/US01/11218.
- Int'l Search Report PCT/US01/11340.
- Int'l Search Report PCT/US01/11420.
- Int'l Search Report PCT/US02/01890.
- Int'l Search Report PCT/US02/11100.
- Int'l Search Report PCT/US04/03436.
- Int'l Search Report PCT/US04/13273.
- Int'l Search Report PCT/US04/15311.
- Int'l Search Report EP 98944778.
- Int'l Search Report EP 98958575.
- Int'l Search Report EP 04027314.
- Int'l Search Report EP 04027479.
- Int'l Search Report EP 04027705.
- Int'l Search Report EP 04013772.
- "Innovations in Electrosurgery" *Sales/Product Literature*; Dec. 31, 2000.
- Olsson et al. "Radical Cystectomy in Females" *Current Surgical Techniques in Urology*, vol. 14, Issue 3, 2001.
- Levy et al. "Use of a New Energy-based Vessel Ligation Device During Vaginal Hysterectomy" *Int'l Federation of Gynecology and Obstetrics (FIGO) World Congress* 1999.
- Carbonell et al., "Comparison of theGyrus PlasmaKinetic Sealer and the Valleylab LigaSure Device in the Hemostasis of Small, Medium, and Large-Sized Arteries" *Carolinas Laparoscopic and Advanced Surgery Program, Carolinas Medical Center, Charlotte, NC* 2003.
- "Reducing Needlestick Injuries in the Operating Room" *Sales/Product Literature* 2001.
- W. Scott Helton, "LigaSure Vessel Sealing System: Revolutionary Hemostasis Product for General Surgery" *Sales/Product Literature* 1999.
- McLellan et al. "Vessel Sealing for Hemostasis During Gynecologic Surgery" *Sales/Product Literature* 1999.
- E. David Crawford "Use of a Novel Vessel Sealing Technology in Management of the Dorsal Velnous Complex" *Sales/Product Literature* 2000.
- Jarrett et al., "Use of the LigaSure Vessel Sealing System for Peri-Hilar Vessels in Laparoscopic Nephrectomy" *Sales/Product Literature* 2000.
- E. David Crawford "Evaluation of a New Vessel Sealing Device in Urologic Cancer Surgery" *Sales/Product Literature* 2000.
- International Search Report PCT/US01/11224 dated Nov. 13, 2001.
- International Search Report EP 98958575.7 dated Sep. 20, 2002.
- International Search Report EP 04013772 dated Apr. 1, 2005.
- International Search Report EP 05013895 dated Oct. 14, 2005.
- International Search Report EP 05017281 dated Nov. 16, 2005.
- Int'l Search Report EP 05013463.4 dated Sep. 28, 2005.
- Int'l Search Report EP 05019130.3 dated Oct. 18, 2005.
- Int'l Search Report EP 05020665.5 dated Feb. 16, 2006.
- Int'l Search Report EP 05020666.3 dated Feb. 17, 2006.
- Int'l Search Report EP 05021779.3 dated Jan. 18, 2006.
- Int'l Search Report EP 05021197.8 dated Jan. 31, 2006.
- Int'l Search Report EP 05021937.7 dated Jan. 13, 2006.
- Int'l Search Report—extended- EP 05021937.7 dated Mar. 6, 2006.
- Int'l Search Report EP 05023017.6 dated Feb. 16, 2006.
- Int'l Search Report EP 05021780.1 dated Feb. 9, 2006.
- Int'l Search Report EP 06002279.5 dated Mar. 9, 2006.
- Int'l Search Report EP 05016399 dated Jan. 5, 2006.
- Int'l Search Report EP 06005185.1 dated Apr. 18, 2006.
- Int'l Search Report EP 06008779.8 dated Jun. 13, 2006.
- Int'l Search Report EP 1683496 dated Jun. 13, 2006.
- Int'l Search Report EP 05016399 dated Jan. 5, 2006.
- Int'l Search Report EP 06005185.1 dated Apr. 18, 2006.
- Int'l Search Report EP 06008779.8 dated Jun. 13, 2006.
- Int'l Search Report EP 1683496 dated Jun. 13, 2006.
- Int'l Search Report EP 04013772 dated Apr. 1, 2005.
- Int'l Search Report EP 05013895 dated Oct. 14, 2005.
- Int'l Search Report EP 05017281 dated Nov. 16, 2005.
- Int'l Search Report EP 06006716 dated Aug. 4, 2006.
- Int'l Search Report PCT/US01/11224 dated Nov. 13, 2001.
- Int'l Search Report EP 06014461.5 dated Oct. 20, 2006.
- Int'l Search Report EP 06020584.6 dated Jan. 12, 2007.
- Int'l Search Report EP 06020583.8 dated Jan. 30, 2007.
- Int'l Search Report EP 06020756.0 dated Feb. 5, 2007.
- Int'l Search Report EP 06024123.9 dated Feb. 26, 2007.
- Int'l Search Report EP 04 752343.6 dated Jul. 20, 2007.
- Int'l Search Report EP 06 024122.1 dated Mar. 19, 2007.
- Int'l Search Report EP 07 001480.8 dated Apr. 12, 2007.
- Int'l Search Report EP 07 001488.1 dated May 29, 2007.
- Int'l Search Report —Extended EP 07 009029.5 dated Jul. 12, 2007.
- Int'l Search Report EP 07 009321.6 dated Aug. 17, 2007.

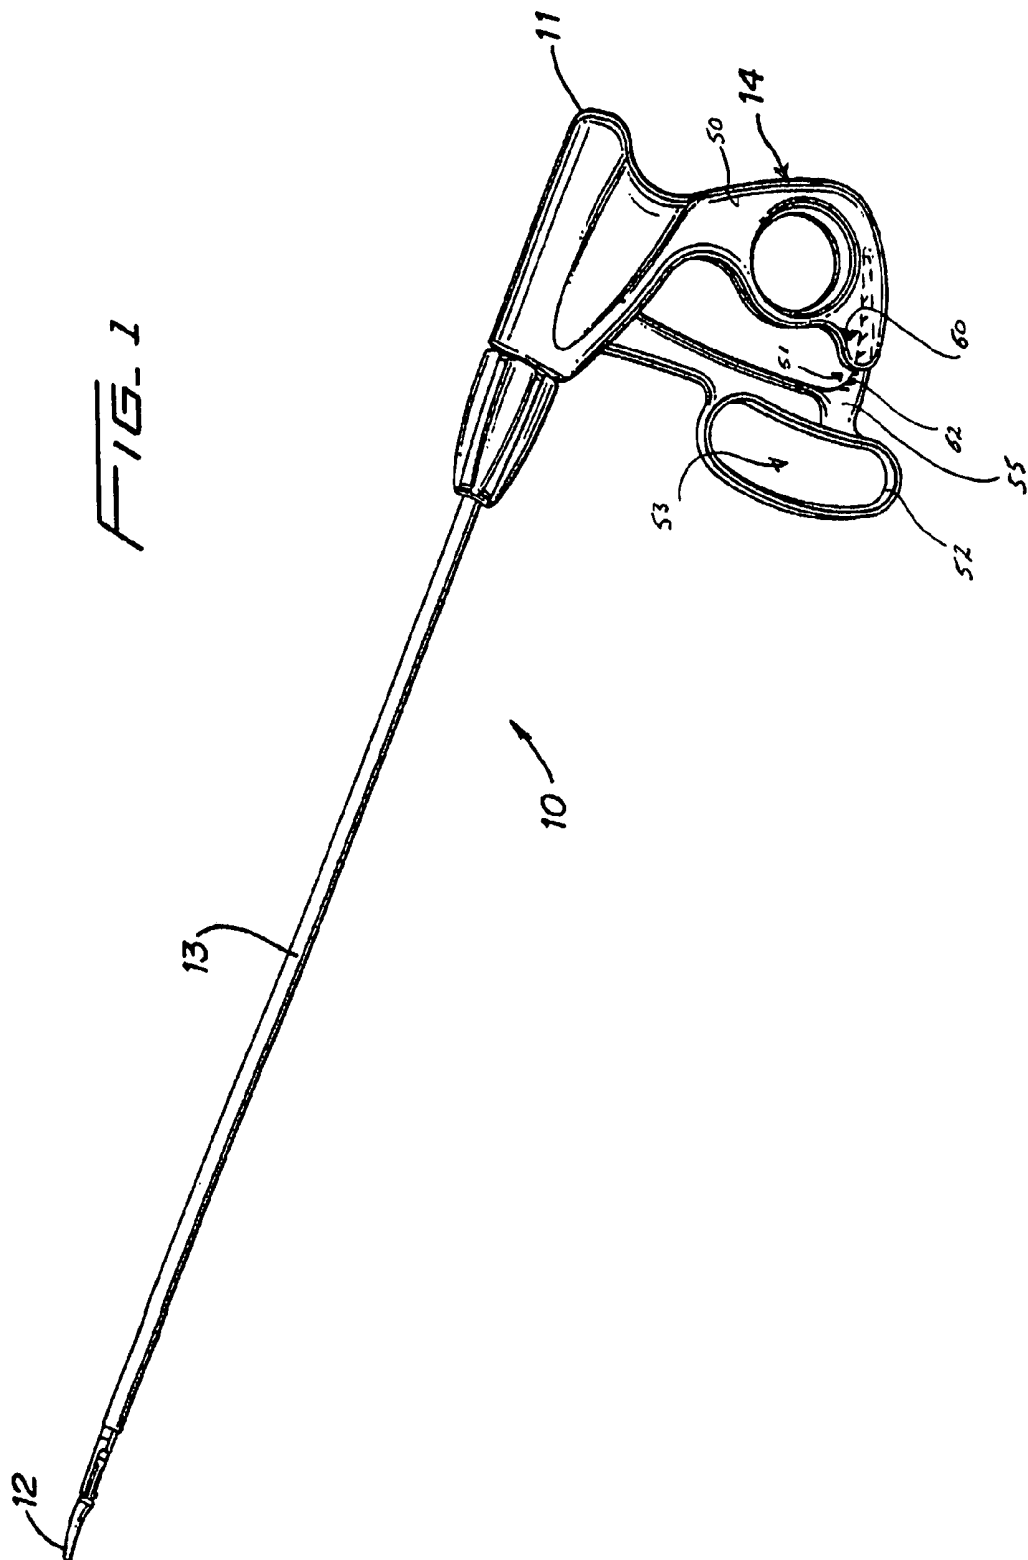

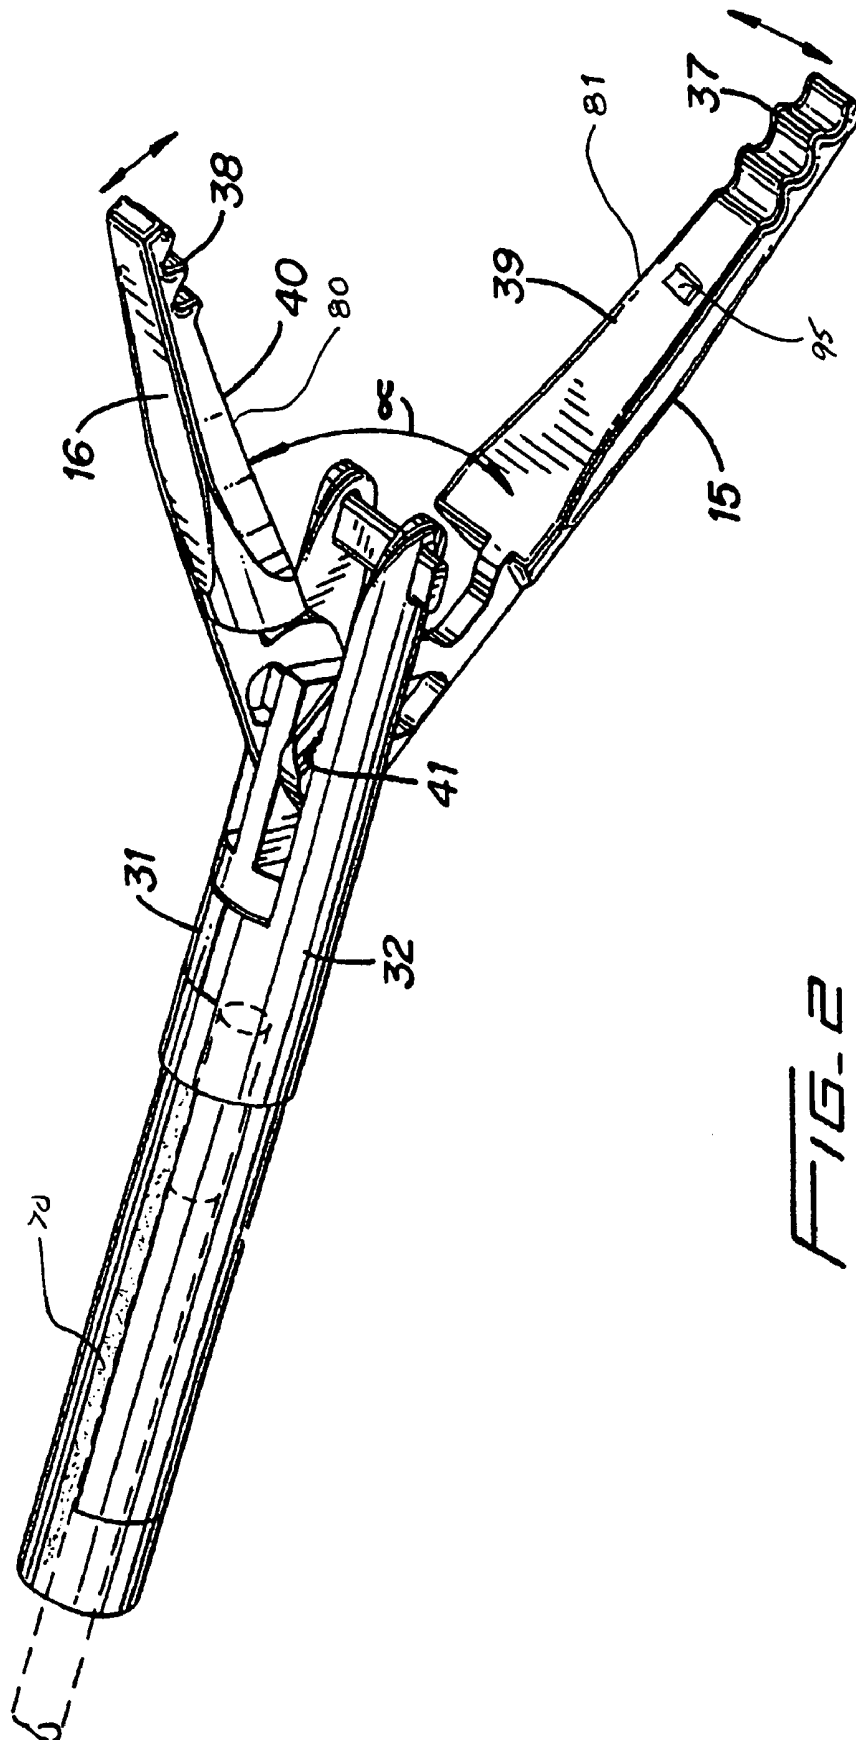


FIG. 2

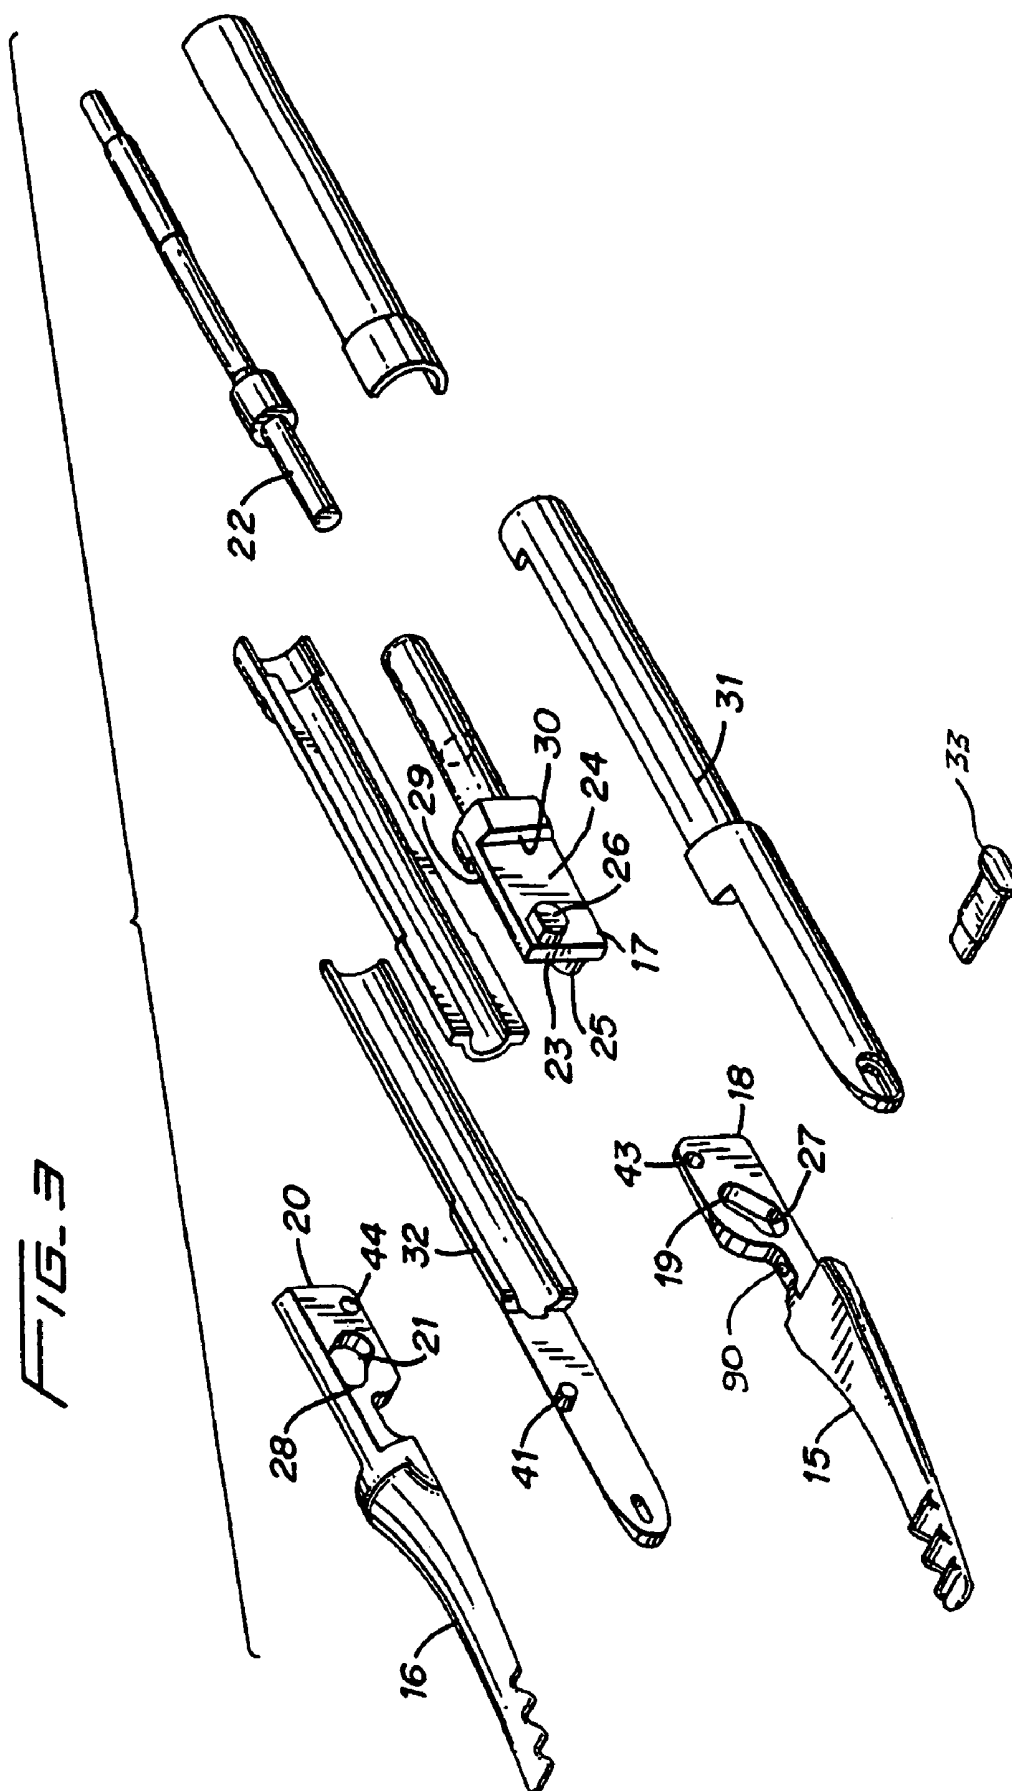


FIG. 4

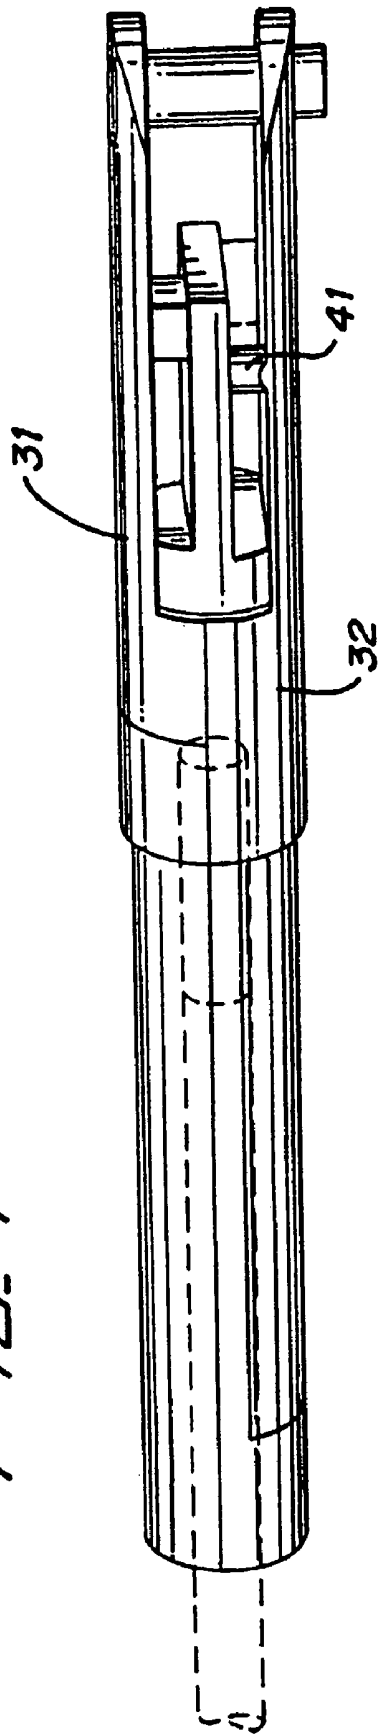


FIG. 5

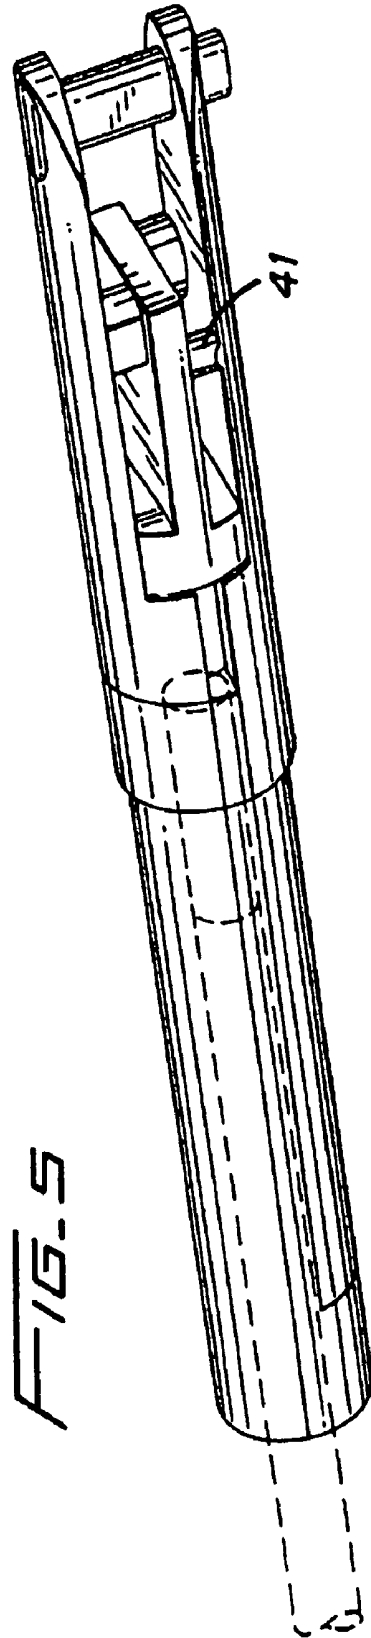


FIG. 6


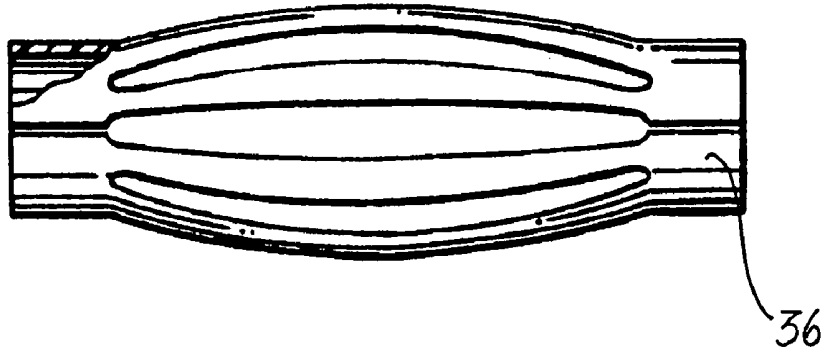


FIG. 7

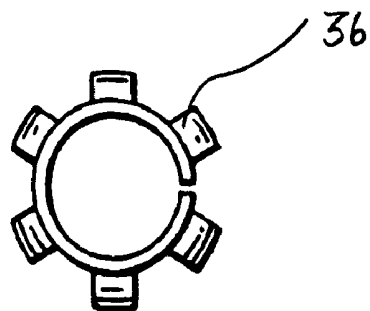

LAPAROSCOPIC BIPOLAR ELECTROSURGICAL INSTRUMENT

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 10/164,654 filed Jun. 6, 2002, now abandoned, which is a continuation-in-part of U.S. application Ser. No. 09/591,330 filed on Jun. 9, 2000 now U.S. Pat. No. 6,451,018, which is a continuation of U.S. application Ser. No. 08/970,472 filed on Nov. 14, 1997, now U.S. Pat. No. 6,228,083, the entire contents of all of which being incorporated by reference herein.

BACKGROUND

1. Field of the Invention

This disclosure relates to an electrosurgical instrument for performing laparoscopic surgical procedures, and more particularly to a laparoscopic electrosurgical instrument that is capable of grasping vessels and vascular tissue with sufficient force between two bipolar jaws to seal the vessel or vascular tissue.

2. Background of Related Art

Laparoscopic surgical instruments are used to perform surgical operation without making large incisions in the patient. The laparoscopic instruments are inserted into the patient through a cannula, or port, that has been made with a trocar. Typical sizes for cannulas range from three millimeters to twelve millimeters. Smaller cannulas are usually preferred, and this presents a design challenge to instrument manufacturers who must find ways to make surgical instruments that fit through the cannulas.

Certain surgical procedures require cutting blood vessels or vascular tissue. This sometimes presents a problem for surgeons because it is difficult to suture blood vessels using laparoscopic tools. Very small blood vessels, in the range below two millimeters in diameter, can often be closed using standard electrosurgical techniques. If a larger vessel is severed, it may be necessary for the surgeon to convert the laparoscopic procedure into an open-surgical procedure and thereby abandon the benefits of laparoscopy.

Several journal articles have disclosed methods for sealing small blood vessels using electrosurgery. An article entitled Studies on Coagulation and the Development of an Automatic Computerized Bipolar Coagulator, J. Neurosurg., Volume 75, July 1991, describes a bipolar coagulator which is used to seal small blood vessels. The article states that it was not possible to safely coagulate arteries with a diameter larger than 2 to 2.5 mm. A second article is entitled Automatically Controlled Bipolar Electrocoagulation—"COACOMP", Neurosurg. Rev. (1984), pp. 187-190. This article describes a method for terminating electrosurgical power to the vessel so that charring of the vessel walls can be avoided.

It has been recently determined that electrosurgical methods may be able to seal larger vessels using an appropriate electrosurgical power curve, coupled with an instrument capable of applying a large closure force to the vessel walls. It is thought that the process of coagulating small vessels is fundamentally different than electrosurgical vessel sealing. Coagulation is defined as a process of desiccating tissue wherein the tissue cells are ruptured and dried. Vessel sealing is defined as the process of liquefying the collagen in the tissue so that it cross-links and reforms into a fused

mass. Thus, coagulation of small vessels is sufficient to permanently close them. Larger vessels need to be sealed to assure permanent closure.

It would be desirable to have a surgical tool capable of applying electrosurgical energy, capable of applying a large closure force to the vessel walls, and also capable of fitting through a cannula. A large closure force between the jaws typically requires a large moment about the pivot for each jaw. This presents a challenge because the first and second pins have a small moment arm with respect to the pivot of each jaw. A large force, coupled with a small moment arm, is undesirable because the large forces may shear the first and second pins. It is also undesirable to increase the moment arm of the first and second pins because the physical size of the yoke might not fit through a cannula.

Several bipolar laparoscopic instruments are known. For example, U.S. Pat. No. 3,938,527 discloses a bipolar laparoscopic instrument for tubal cauterization. U.S. Pat. No. 5,250,047 discloses a bipolar laparoscopic instrument with a replaceable electrode tip assembly. U.S. Pat. No. 5,445,638 discloses a bipolar coagulation and cutting forceps with first and second conductors extending from the distal end. U.S. Pat. No. 5,391,166 discloses a bipolar endoscopic instrument having a detachable working end. U.S. Pat. No. 5,342,359 discloses a bipolar coagulation device.

The present invention solves the problem of providing a large closure force between the jaws of a laparoscopic bipolar electrosurgical instrument, using a compact design that fits through a cannula, without risking structural failure of the instrument yoke.

SUMMARY OF THE INVENTION

The present disclosure relates to a laparoscopic bipolar electrosurgical instrument for sealing tissue and includes a handle having an elongated tube affixed thereto. The tube includes first and second jaw members attached to a distal end thereof which are movable from a first position for approximating tissue to at least one subsequent position for grasping tissue therebetween. Each of the jaw members includes an electrically conductive sealing surface. The handle has a fixed handle and a handle which is movable relative to the fixed handle to effect movement of the jaw members from the first position to the at least one subsequent position for grasping tissue. The jaw members are connected to a source of electrosurgical energy such that the jaw members are capable of conducting bipolar electrosurgical energy through the tissue held therebetween. A stop is included for maintaining a minimum separation distance between opposing sealing surfaces and a ratchet is included for maintaining a closure force in the range of about 3 kg/cm² to about 16 kg/cm² between opposing sealing surfaces.

Preferably, the stop maintains a minimum separation distance of at least about 0.03 millimeters between opposing sealing surfaces. The stop may be disposed on at least one of the electrically conductive sealing surfaces, or alternatively, the stop may be located adjacent one of the electrically conductive sealing surfaces.

In one embodiment according to the present disclosure, the first jaw member is connected to the bipolar electrosurgical energy source by a pushrod and the second jaw member is connected to the bipolar electrosurgical source by a conductive tube.

In another embodiment, the ratchet is disposed within the fixed handle and at least one complimentary interlocking mechanical interface is disposed on the movable handle.

Preferably, the ratchet and the complimentary interlocking mechanical interface provide at least one interlocking position for maintaining a closure force within the range of about 7 kg/cm² to about 13 kg/cm² between opposing sealing surfaces. Ideally, the closure force is in the range of about 4 kg/cm² to about 6.5 kg/cm².

In yet another embodiment according to the present disclosure, the laparoscopic bipolar electrosurgical instrument includes a handle having an elongated tube affixed thereto with first and second jaw members attached to a distal end thereof which each include electrically conductive sealing surfaces. The jaw members are movable from a first position for approximating tissue to at least one subsequent position for grasping tissue therebetween. The handle has a fixed handle and a handle which is movable relative to the fixed handle to effect movement of the jaw members from the first position to the at least one subsequent position for grasping tissue. The sealing surfaces include a non-stick material for reducing tissue adhesion during the sealing process. The first and second jaw members are coupled to a source of bipolar electrosurgical energy and a stop is disposed on at least one of the electrically conductive sealing surfaces to maintain a minimum separation distance between the opposable seal surfaces during sealing. A ratchet is disposed on one of the fixed and movable handles and at least one complimentary interlocking mechanical interface is disposed on the other of the fixed and movable handles. Preferably, the ratchet and the complimentary interlocking mechanical interface include at least one interlocking position which maintains a closure force in the range of about 7 kg/cm² to about 13 kg/cm² between opposable seal surfaces.

In one embodiment, the non-stick material is a coating which is deposited on the opposable sealing surfaces. The non-stick coating may be selected from a group of materials consisting of: nitrides and nickel/chrome alloys. Preferably, the non-stick coating includes one of: TiN; ZrN; TiAlN; CrN; nickel/chrome alloys with a Ni/Cr ratio of approximately 5:1; Inconel 600; Ni200; and Ni201.

In one embodiment according to the present disclosure, the opposable sealing surfaces are manufactured from a non-stick material which is a nickel/chrome alloy. For example, the non-stick material may include nickel/chrome alloys with a Ni/Cr ratio of approximately 5:1, Inconel 600, Ni200 and Ni201.

Preferably, at least one of the jaw members, handles and elongated tube includes an insulative material disposed thereon which may be an insulative coating or an insulative sheath.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a laparoscopic bipolar electrosurgical instrument according to the present disclosure;

FIG. 2 is a perspective view of the distal end and jaws of the instrument in FIG. 1;

FIG. 3 is an exploded view of the distal end shown in FIG. 2;

FIG. 4 is perspective view of the distal end of the instrument with the jaws removed;

FIG. 5 is another perspective of FIG. 4;

FIG. 6 is a side view of an electrical spring contact; and

FIG. 7 is a front view of the spring contact shown in FIG. 6.

DETAILED DESCRIPTION OF THE INVENTION

A laparoscopic bipolar electrosurgical instrument 10 is shown in FIG. 1. The instrument 10 has a proximal end 11 with a handle 14 for holding and manipulating the instrument 10. A distal end 12 on the instrument 10 is used for surgical manipulation of tissue. The instrument 10 comprises an elongate tube 13 that is sized to fit through a cannula for laparoscopic operations, and in different embodiments may be sized to fit through a five to ten millimeter cannulas.

A portion of the distal end 12 of the instrument 10 is shown in FIG. 2. A first jaw 15 and a second jaw 16 are shown in an open position. An angle α is subtended by the jaws 15 and 16. Closing of the jaws 15 and 16 is defined as a reduction of the angle α subtended by the jaws 15 and 16. Similarly, opening of the jaw 15 and 16 is defined as an enlargement of the angle α . The angle α is zero when the jaws 15 and 16 are closed together. The center of rotation for the first jaws 15 is at the first pivot 41, and the center of rotation for the second jaw 16 is at the second pivot 42. The first pivot 41 is located on an outer nose piece 32, and fits in a first pivot hole 43 located on the first flange 18. The second pivot 42 is located on an inner nose piece 31, and fits in a second pivot hole 44 located on the second flange 20.

Pieces that comprise the distal end 12 of the instrument 10 are shown in an exploded view in FIG. 3. The first jaw 15 and the second jaw 16 are shown separated from a yoke 17. The first jaw 15 has a first flange 18 and a first slot 19 therewithin. The second jaw 16 has a second flange 20 and a second slot 21 therewithin. Each jaw 15 and 16 is preferably formed from a single piece of stainless steel or other electrically conductive material.

Referring again to FIG. 3, the yoke 17 is attached to a pushrod 22. The yoke 17 is preferably formed from an electrically insulative material such as plastic. A first side 23 of the yoke 17 faces the first flange 18. A second side 24 of the yoke 17 faces the second flange 20. When the yoke 17 is positioned between the flanges 18 and 20, the yoke 17 also acts to electrically insulate the first jaw 15 from the second jaw 16. In this manner, bipolar electrosurgical current can be conducted through tissue grasped by the jaws 15 and 16 without short circuiting between the flanges 18 and 20.

A first pin 25 is located on the first side 23 which movably engages the first slot 19. Similarly, a second pin 26 is located on the second side 24 to movably engage the second slot 21. Each pin and slot combination works as a cam-follower mechanical linkage. Motion of the pushrod 22 moves the yoke 17 causing pins 25 and 26 to slide within their respective slots 19 and 21. The slots 19 and 21 are angled with respect to the distal ends of the jaws 15 and 16 such that the jaws 15 and 16 move in an arcuate fashion toward and away from each other. The pins 25 and 26 are different from the pivots 41 and 42. The pins 25 and 26 provide a force against the walls of the slots 19 and 21, creating a moment about the pivots 41 and 42.

The slots 19 and 21 are arranged such that distal motion of the pushrod 22 causes the jaws 15 and 16 to move together. Distal motion of the pushrod 22 is defined as motion in the direction of the distal end 12 of the instrument 10. Once the jaws 15 and 16 are closed together, the present invention holds the jaws 15 and 16 together with a compressive force on the pushrod 22.

One of the advantages of this invention is that shear forces on the pins 25 and 26 can be offloaded to prevent mechanical failure when large forces are being transmitted to the jaws 15

and 16. Each slot 19 and 20 has a cul-de-sac 27 and 28, respectively, as shown in FIG. 3. The first cul-de-sac 27 is an enlargement of the first slot 19 near its distal end. The second cul-de-sac 28 is an enlargement of the second slot 21 near its distal end. The cam-follower motion of the pins 25 and 26 in the slots 19 and 21 will bring the pins 25 and 26 into their respective cul-de-sac 27 and 28. This position of the pins 25 and 26 leaves a very small moment arm between the pins 25 and 26 and the pivots 41 and 42. The yoke 17 has shoulders 29 and 30 that can provide a relatively large moment about the pivots 41 and 42 to effect a high closure force between the jaws 15 and 16 without a high shear forces on the pins 25 and 26, as described below.

Once the pins 25 and 26 are in the cul-de-sacs 27 and 28, the force from the yoke is transmitted to the flanges 18 and 20 by a first shoulder 29 and a second shoulder 30. The shoulders 29 and 30 about the proximal end of the flanges 18 and 20 to cause the jaws 15 and 16 to close together. The pivots 41 and 42 are preferably made of metal and can withstand relatively high shear forces. In contrast, pins 25 and 26 are preferably made of plastic and will break under relatively high shear forces. Thus, the shoulders 29 and 30 provide a moment about the pivots 41 and 42, thereby avoiding the necessity of applying high shear forces to the pins 25 and 26 wherein the moment arm from the pins 25 and 26 would be small. There is an angle α at which the pins 25 and 26 enter their respective cul-de-sacs 27 and 28 and the shoulders 29 and 30 about the flanges 18 and 20. The angle α at which the forgoing occurs is preferably around three degrees.

The bipolar electrosurgical instrument 10 has first and second poles of alternating potential that are conducted along the instrument 10 and through tissue that is grasped between the jaws 15 and 16. The first pole is conducted from the proximal end 11 toward the distal end 12 along the pushrod 22. The second pole is conducted from the proximal end 11 toward the distal end 12 along the tube 13. The outer surface of the tube 13 is preferably coated with an electrically insulative material. There is also preferably an electrically insulative barrier between the pushrod 22 and the tube 13 to prevent short circuits in the instrument 10.

In the preferred embodiment, the distal end of the instrument 10 comprises an inner nose piece 31 and an outer nose piece 32, as shown in FIG. 2. The inner nose piece 31 is electrically connected with the pushrod 22, while the outer nose piece is electrically connected with the tube 13. The inner nose piece 31 and the outer nose piece 32 capture the yoke 17, along with the first and second flanges 18 and 20, as shown in FIG. 2. The yoke 17 moves axially, along an axis defined by the tube 13, in a space between the inner and outer nose pieces 31 and 32. A spacer stake 33 maintains the separation of the nose pieces 31 and 32 at their distal ends. The nose pieces 31 and 32 provide lateral support for the flanges 18 and 20 to help ensure that the pins 25 and 26 remain within the slots 19 and 21, respectively.

The preferred embodiment also comprises an inner insulator 34 and an outer insulator 35 for maintaining electrical insulation between the poles. The outer insulator 35 is seated between the tube 13 and the inner nose 31, as shown in FIGS. 2 and 4. The inner insulator 34 is seated between the tube 13 and the pushrod 22. In this manner, the outer nose piece 32 can provide electrical continuity between the tube 13 and the second jaw 16, while the inner nose piece 34 can provide electrical continuity between the pushrod 22 and the first jaw 15. Since the pushrod 22 is slidably mounted within the tube 13, the preferred embodiment has a spring contact 36, as shown in FIGS. 6 and 7, which is mounted on the

pushrod 22 to maintain an electrical connection with the inner nose piece 34 during axial motion.

The first and second jaws 15 and 16 each have ridges 37 and 38 at their distal ends that preferably nest together. The jaws 15 and 16 also have seal surfaces 39 and 40, as shown in FIG. 2. The width of the seal surfaces 39 and 40 is a parameter that affects the quality of the surgical outcome. The closure force between the jaws 15 and 16 varies along the length of the seal surfaces 39 and 40, with the largest force at the distal tip and the smallest force at the proximal end of the seal surfaces 39 and 40. It is known that the amount of pressure exerted on the tissue depends on the surface area of the tissue that is in contact with the seal surfaces. In the one embodiment, the width of each seal surface, e.g., 39, is in the range of about 2 to about 5 millimeters, and preferably 4 millimeters width, while the length of each seal surface 39 and 40 is preferably in the range of about 10 to 30 millimeters.

It has been found through experimentation that good vessel sealing results are obtained when the closure force in grams divided by the width in millimeters is in the range of about 400 to 650 grams per millimeter of seal surface width. Since the closure force varies with the length of the seal surfaces 39 and 40, it has been found to be advantageous to taper the width of the seal surfaces 39 and 40 along their length, with the widest width at the proximal end and the narrowest width at the distal end. For example, if the width of the seal surface 39, 40 is 4 millimeters, the closure force is preferably in the range of about 1600 grams to about 2600 grams. This design allows the jaws 15 and 16 to apply a relatively constant closure force per unit width, preferably 525 grams per millimeter width which yields a closure force of 2100 grams for a 4 millimeter width seal surface 39, 40.

In one embodiment, the handle 14 includes a fixed handle 50 having a channel 51 defined therein which slidably receives a movable handle 52. Movable handle 52 includes a handgrip 53 defined therein which allows a user to move handle 52 relative to fixed handle 50. Movable handle 52 also includes a flange 55 having a series of grooves 62 defined therein which mechanically inter-engage a corresponding ratchet 60 disposed within channel 51. Preferably, the ratchet 60 and groove 62 are dimensioned such that successive ratchet positions will yield pressures within a predetermined working range of about 7 kg/cm² to about 13 kg/cm². In one embodiment, the successive ratchet positions are two millimeters apart.

Experimental results in tissue studies suggest that the magnitude of pressure exerted on the tissue by the seal surfaces 39 and 40 is important in assuring a proper surgical outcome. Tissue pressures within a working range of about 3 kg/cm² to about 16 kg/cm² and, preferably, within a working range of 7 kg/cm² to 13 kg/cm² have been shown to be effective for sealing arteries and vascular bundles. Tissue pressures within the range of about 4 kg/cm² to about 6.5 kg/cm² have proven to be particularly effective in sealing arteries and tissue bundles.

A method of making a laparoscopic bipolar electrosurgical instrument 10 is also herein described. The method comprises the step of forming a first jaw 15 having a first flange 18 with a first slot 19, and a second jaw 16 having a second flange 20 with a second slot 21. The jaws 15 and 16 are preferably formed in a casting process, although it is also possible to machine the jaws 15 and 16 from stock. The casting process may include injecting powdered metal under pressure into a mold, and then applying heat.

Other steps in the method include attaching a yoke 17 to a pushrod 22, and electrically insulating the first flange 18

from the second flange 20 with the yoke 17. The yoke 17 is preferably an injection molded plastic part with features including a first shoulder 29 and a second shoulder 30.

During assembly of the distal portion of the instrument 10, steps in the method include engaging a first pin 25 with the first slot 19, and engaging a second pin 26 with the second slot 21. The slots 19 and 21 are shaped such that a subtended angle α between the first and second jaws 15 and 16 decreases with distal motion of the pushrod 17. The slots 19 and 20 are formed with cul-de-sacs 27 and 28 positioned to relieve shear stresses on the first and second pins 25 and 26 at the subtended angle α approximately where the first and second shoulders 29 and 30 engage the first and second flanges 18 and 20.

Further steps in the method comprise: surrounding at least a portion of the pushrod 22 with an electrically conductive tube 13; electrically insulating the tube 13 from the pushrod 22; electrically connecting an inner nose piece 31 to the pushrod 22, and electrically connecting an outer nose piece 32 to the tube 13, wherein the inner nose piece 31 and the outer nose piece 32 capture the yoke 17 along with the first and second flanges 18 and 20 to conduct bipolar electrosurgical current to the first and second jaws 15 and 16. In the preferred embodiment, there is a step of electrically connecting the pushrod 22 and the inner nose piece 31 with a spring contact 36.

The method of making the instrument 10, in some embodiments, includes the steps of tapering the width of the seal surfaces 39 and 40 along the length of each of the first and second jaws 15 and 16.

An electrically insulative coating 70 may be included to substantially cover the elongated tube 13 to protect the surgeon against electrical arcs. Other parts of the instrument may also be protected by the insulative coating 70. An insulative sheath may also be used to cover tube 13 or other components of the instrument 10, e.g., the proximal end 11, handles 50, 52 and the outer surfaces (non-opposing surfaces) of the jaw members 15, 16.

It is envisioned that the outer surface of the jaw members 15 and 16 may include a nickel-based material, coating, stamping, metal injection molding which is designed to reduce adhesion between the jaw members (or components thereof) with the surrounding tissue during activation and sealing. Moreover, it is also contemplated that other components such as the tube 13 and handles 50, 52 may also be coated with the same or a different "non-stick" material. Preferably, the non-stick materials are of a class of materials that provide a smooth surface to prevent mechanical tooth adhesions.

It is also contemplated that the tissue sealing surfaces 39 and 40 of the jaw members 15 and 16, respectively, may be manufactured from one (or a combination of one or more) of the following "non-stick" materials: nickel-chrome, chromium nitride, MedCoat 2000 manufactured by The Electrolyzing Corporation of OHIO, Inconel 600 and tin-nickel. For example, high nickel chrome alloys and Ni200, Ni201 (~100% Ni) may be made into electrodes or sealing surfaces by metal injection molding, stamping, machining or any like process.

In addition these materials preferably include an optimal surface energy for eliminating sticking due in part to surface texture and susceptibility to surface breakdown due electrical effects and corrosion in the presence of biologic tissues. It is envisioned that these materials exhibit superior non-stick qualities over stainless steel and should be utilized on the instrument in areas where the exposure to pressure and RF energy can create localized "hot spots" more susceptible

to tissue adhesion. As can be appreciated, reducing the amount that the tissue "sticks" during sealing improves the overall efficacy of the instrument.

The tissue sealing surfaces 39 and 40 may also be "coated" with one or more of the above materials to achieve the same result, i.e., a "non-stick surface". For example, Nitride coatings (or one or more of the other above-identified materials) may be deposited as a coating on another base material (metal or nonmetal) using a vapor deposition manufacturing technique.

One particular class of materials disclosed herein has demonstrated superior non-stick properties and, in some instances, superior seal quality. For example, nitride coatings which include, but not are not limited to: TiN, ZrN, TiAlN, and CrN are preferred materials used for non-stick purposes. CrN has been found to be particularly useful for non-stick purposes due to its overall surface properties and performance. Other classes of materials have also been found to reducing overall sticking. For example, high nickel/chrome alloys with a Ni/Cr ratio of approximately 5:1 have been found to significantly reduce sticking in bipolar instrumentation. One particularly useful non-stick material in this class is Inconel 600. Bipolar instrumentation having electrodes made from or coated with Ni200, Ni201 (~100% Ni) also showed improved non-stick performance over typical bipolar stainless steel electrodes.

It has been found experimentally that local current concentrations can result in an uneven tissue effect, and to reduce the possibility of this outcome, each seal surface 39 and 40 may include a radiused edge 80, 81. As mentioned above, a tapered seal surface 39 and 40 has been shown to be advantageous in certain embodiments because the taper allows for a relatively constant pressure on the tissue along the length of the seal surfaces 39 and 40. The width of the seal surfaces 39 and 40 may be adjusted to assure that the closure force divided by the width is approximately constant along the length.

In one embodiment, a stop 90, made from insulative material, is located in the instrument to maintain a minimum separation of at least about 0.03 millimeters between the seal surfaces 39 and 40, as shown in FIG. 3. Preferably, the stop maintains a minimum separation distance in the range of about 0.03 millimeters to about 0.16 millimeters. The stop 90 reduces the possibility of short circuits between the seal surfaces 39 and 40. It is envisioned that stop 90 may be positioned proximate the pivots 41 and 42, proximate the stake 33 or adjacent the opposable seal surfaces 39 and 40.

In another embodiment, the instrument 10 includes a second or alternative stop 95 which is designed to maintain a minimum separation of at least about 0.03 millimeters between the seal surfaces 39 and 40, as shown in FIG. 2. Preferably, the stop 90 and/or the stop 95 maintains a separation distance within the range of about 0.03 millimeters to about 0.16 millimeters. A plurality of stops 90 and/or 95 (or various patterns of stops 90, 95) may also be utilized to accomplish this purpose.

It is to be understood that the above described embodiments are only illustrative of the application of the principles of the present invention. Numerous modifications and alternative arrangements may be devised by those skilled in the art without departing from the spirit and scope of the present invention. The appended claims are intended to cover such modifications and arrangements.

9

What is claimed is:

1. A laparoscopic bipolar electrosurgical instrument for sealing tissue, comprising:

a handle being selectively movable to actuate a pair of first and second opposable jaw members attached to a distal end thereof, the jaw members being movable from a first position for approximating tissue to at least one subsequent position for grasping tissue therebetween, each of the jaw members including an electrically conductive sealing surface and adapted to connect to a source of electrosurgical energy such that the sealing surfaces are capable of conducting electrosurgical energy through tissue held therebetween and each jaw member including: a cam slot defined therein having a cul de sac at a distal end thereof;

a yoke being dimensioned to operatively engage each of the jaw members to affect movement thereof, said yoke including first and second pins extending from the sides thereof which operatively engage a respective cam slot in each of the jaw members, said pins being movable within said cam slots upon actuation of said handle and said pins being dimensioned to enter each cul de sac when said jaw members are disposed at an angle of about 3 degrees relative to one another.

2. A laparoscopic bipolar electrosurgical instrument according to claim 1 wherein said yoke further includes a pair of shoulders which are designed to offload closure pressure of the pins when said pins enter said cul de sac portions of said slots.

10

3. A laparoscopic bipolar electrosurgical instrument according to claim 1 further comprising a stop for maintaining a minimum separation distance of at least about 0.03 millimeters between the sealing surfaces.

4. A laparoscopic bipolar electrosurgical instrument according to claim 3 wherein the stop is disposed on at least one of the sealing surfaces.

5. A laparoscopic bipolar electrosurgical instrument according to claim 3 wherein the stop maintains a minimum separation distance between the sealing surfaces in the range of about 0.03 millimeters to about 0.16 millimeters.

6. A laparoscopic bipolar electrosurgical instrument according to claim 3 further comprising means for maintaining a closure force in the range of about 3 kg/cm² to about 16 kg/cm² between the sealing surfaces.

7. A laparoscopic bipolar electrosurgical instrument according to claim 1 further comprising means for maintaining a closure force in the range of about 3 kg/cm² to about 16 kg/cm² the sealing surfaces.

8. A laparoscopic bipolar electrosurgical instrument according to claim 1 further comprising:

a pushrod adapted to connect the first jaw member to a source of electrosurgical energy; and

a conductive tube adapted to connect the second jaw member to the source of electrosurgical energy.

* * * * *

专利名称(译)	腹腔镜双极电外科仪器		
公开(公告)号	US7377920	公开(公告)日	2008-05-27
申请号	US11/122346	申请日	2005-05-05
[标]申请(专利权)人(译)	Buysse的史蒂芬P 劳斯凯特 - [R 伤感DALE°F 地政MICHAELJ LUKIANOW小号W JOHNSON KRISTIND COUTURE GARY中号 阮LAP P		
申请(专利权)人(译)	Buysse的史蒂芬P 劳斯凯特 - [R 伤感DALE°F 地政MICHAELJ LUKIANOW小号W JOHNSON KRISTIND COUTURE GARY中号 阮LAP P		
当前申请(专利权)人(译)	SHERWOOD SERVICES AG		
[标]发明人	BUYSSE STEVEN P LAWES KATE R SCHMALTZ DALE F LANDS MICHAEL J LUKIANOW S WADE JOHNSON KRISTIN D COUTURE GARY M NGUYEN LAP P		
发明人	BUYSSE, STEVEN P. LAWES, KATE R. SCHMALTZ, DALE F. LANDS, MICHAEL J. LUKIANOW, S. WADE JOHNSON, KRISTIN D. COUTURE, GARY M. NGUYEN, LAP P.		
IPC分类号	A61B18/14 A61B19/00		
CPC分类号	A61B18/1445 A61B2018/00083 A61B2018/0063 A61B2018/00666 A61B2019/304 A61B2090/034		
审查员(译)	COHEN , LEE S.		
其他公开文献	US20050240179A1		
外部链接	Espacenet USPTO		
摘要(译)			

用于密封组织的腹腔镜双极电外科器械包括手柄，手柄具有固定到其上的细长管。所述管包括第一和第二钳口构件，所述第一和第二钳口构件具有附接到其远端的导电密封表面，所述导电密封表面可从用于近似组织的第一位置移动到用于抓握其间的组织的第二位置。手柄包括固定手柄和手柄，手柄可相对于固定手柄移动，以实现钳口构件从第一位置到第二位置的移动，以抓取组织。钳口构件连接到电外科能量源，使得可相对的密封表面能够通过保持在其间的组织传导电外科能量。包括止动件以保持相对的密封表面之间的最小间隔距离。还包括棘轮以在相对的密封表面之间保持约7kg / cm²至约13kg / cm²范围内的闭合力。

