

(56)	References Cited					
U.S. PATENT DOCUMENTS						
3,791,379 A	2/1974	Storz	5,312,425 A	5/1994	Evans et al.	
3,812,855 A	5/1974	Banko	5,312,430 A	5/1994	Rosenbluth et al.	
3,850,162 A	11/1974	Iglesias	5,320,091 A	6/1994	Grossi et al.	
3,945,375 A	3/1976	Banko	5,347,992 A	9/1994	Pearlman et al.	
3,980,252 A	9/1976	Tae	5,350,390 A	9/1994	Sher	
3,995,619 A	12/1976	Glatzer	5,364,395 A	11/1994	West, Jr.	
3,996,921 A	12/1976	Neuwirth	5,374,253 A	12/1994	Burns, Sr. et al.	
4,011,869 A	3/1977	Seiler, Jr.	5,390,585 A	2/1995	Ryuh	
4,108,182 A	8/1978	Hartman et al.	5,392,765 A	2/1995	Muller	
4,146,405 A	3/1979	Timmer et al.	5,395,313 A	3/1995	Naves et al.	
4,198,958 A	4/1980	Utsugi	5,403,276 A	4/1995	Schechter et al.	
4,203,444 A	5/1980	Bonnell et al.	5,409,013 A	4/1995	Clement	
4,210,146 A	7/1980	Banko	5,411,513 A	5/1995	Ireland et al.	
4,246,902 A	1/1981	Martinez	5,425,376 A	6/1995	Banys et al.	
4,247,180 A	1/1981	Norris	5,429,601 A	7/1995	Conley et al.	
4,258,721 A	3/1981	Parent	5,443,476 A	8/1995	Shapiro	
4,261,346 A	4/1981	Wettermann	5,449,356 A	9/1995	Walbrink et al.	
4,294,234 A	10/1981	Matsuo	5,456,689 A	10/1995	Kresch et al.	
4,316,465 A	2/1982	Dotson, Jr.	5,490,819 A	2/1996	Nicholas et al.	
4,369,768 A	1/1983	Vukovic	5,490,860 A	2/1996	Middle et al.	
4,392,485 A	7/1983	Hiltebrandt	5,492,537 A	2/1996	Vancaillie	
4,414,962 A	11/1983	Carson	5,498,258 A	3/1996	Hakky et al.	
4,449,538 A	5/1984	Corbitt et al.	5,527,331 A	6/1996	Kresch et al.	
4,493,698 A	1/1985	Wang et al.	5,549,541 A	8/1996	Muller	
4,517,977 A	5/1985	Frost	5,556,378 A	9/1996	Storz et al.	
4,543,965 A	10/1985	Pack et al.	5,563,481 A	10/1996	Krause	
4,567,880 A	2/1986	Goodman	5,569,164 A	10/1996	Lurz	
4,589,414 A	5/1986	Yoshida et al.	5,569,254 A	10/1996	Carlson et al.	
4,601,290 A	7/1986	Effron et al.	5,569,284 A	10/1996	Young et al.	
4,606,330 A	8/1986	Bonnet	5,591,187 A	1/1997	Dekel	
4,630,598 A	12/1986	Bonnet	5,601,583 A	2/1997	Donahue et al.	
4,644,952 A	2/1987	Patipa et al.	5,601,603 A	2/1997	Illi	
4,649,919 A	3/1987	Thimsen et al.	5,602,449 A	2/1997	Krause et al.	
4,700,694 A	10/1987	Shishido	5,603,332 A	2/1997	O'Connor	
4,706,656 A	11/1987	Kuboto	5,630,798 A	5/1997	Beiser et al.	
4,718,291 A	1/1988	Wood et al.	5,649,547 A	7/1997	Ritchart et al.	
4,737,142 A	4/1988	Heckele	5,669,927 A	9/1997	Boebel et al.	
4,749,376 A	6/1988	Kensey et al.	5,672,945 A	9/1997	Krause	
4,756,309 A	7/1988	Sachse et al.	5,674,179 A	10/1997	Bonnet et al.	
4,819,635 A	4/1989	Shapiro	5,676,497 A	10/1997	Kim	
4,844,064 A	7/1989	Thimsen et al.	5,695,448 A	12/1997	Kimura et al.	
4,850,354 A	7/1989	McGurk-Burleson et al.	5,702,420 A	12/1997	Sterling et al.	
4,856,919 A	8/1989	Takeuchi et al.	5,709,698 A	1/1998	Adams et al.	
4,867,157 A	9/1989	McGurk-Burleson et al.	5,730,752 A *	3/1998	Alden et al. 606/180	
4,924,851 A	5/1990	Ognier et al.	5,733,298 A	3/1998	Berman et al.	
4,940,061 A	7/1990	Terwilliger et al.	5,741,286 A	4/1998	Recuset	
4,950,278 A	8/1990	Sachs et al.	5,741,287 A	4/1998	Alden et al.	
4,955,882 A	9/1990	Hakky	5,749,885 A	5/1998	Sjostrom et al.	
4,986,827 A	1/1991	Akkas et al.	5,749,889 A	5/1998	Bacich et al.	
4,998,527 A	3/1991	Meyer	5,759,185 A	6/1998	Grinberg	
4,998,914 A	3/1991	Wiest et al.	5,772,634 A	6/1998	Atkinson	
5,007,917 A	4/1991	Evans	5,775,333 A	7/1998	Burbank et al.	
5,027,792 A	7/1991	Meyer	5,782,849 A	7/1998	Miller	
5,037,386 A	8/1991	Marcus et al.	5,807,240 A	9/1998	Muller et al.	
5,105,800 A	4/1992	Takahashi et al.	5,807,282 A	9/1998	Fowler	
5,106,364 A	4/1992	Hayafuji et al.	5,810,861 A	9/1998	Gaber	
5,112,299 A	5/1992	Pascaloff	5,814,009 A	9/1998	Wheatman	
5,116,868 A	5/1992	Chen et al.	5,833,643 A	11/1998	Ross et al.	
5,125,910 A	6/1992	Freitas	5,840,060 A	11/1998	Beiser et al.	
5,133,713 A	7/1992	Huang et al.	5,857,995 A	1/1999	Thomas et al.	
5,152,744 A	10/1992	Krause et al.	5,873,886 A	2/1999	Larsen et al.	
5,158,553 A	10/1992	Berry et al.	5,899,915 A	5/1999	Saadat	
5,163,433 A	11/1992	Kagawa et al.	5,911,699 A	6/1999	Anis et al.	
5,169,397 A	12/1992	Sakashita et al.	5,911,722 A	6/1999	Adler et al.	
5,176,677 A	1/1993	Wuchinich	5,913,867 A	6/1999	Dion	
5,195,541 A	3/1993	Obenchain	5,916,229 A	6/1999	Evans	
5,226,910 A	7/1993	Kajiyama et al.	5,925,055 A	7/1999	Adrian et al.	
5,244,459 A	9/1993	Hill	5,928,163 A	7/1999	Roberts et al.	
5,254,117 A	10/1993	Rigby et al.	5,944,668 A	8/1999	Vancaillie et al.	
5,269,785 A	12/1993	Bonutti	5,947,990 A	9/1999	Smith	
5,270,622 A	12/1993	Krause	5,951,490 A	9/1999	Fowler	
5,275,609 A	1/1994	Pingleton et al.	5,956,130 A	9/1999	Vancaillie et al.	
5,288,290 A	2/1994	Brody	5,957,832 A	9/1999	Taylor et al.	
5,304,118 A	4/1994	Trese et al.	6,001,116 A	12/1999	Heisler et al.	
5,312,399 A	5/1994	Hakky et al.	6,004,320 A	12/1999	Casscells et al.	
			6,007,513 A	12/1999	Anis et al.	
			6,024,751 A	2/2000	Lovato et al.	
			6,032,673 A	3/2000	Savage et al.	
			6,039,748 A	3/2000	Savage et al.	

US 9,155,454 B2

Page 3

(56)	References Cited		2009/0270898 A1	10/2009	Chin et al.
U.S. PATENT DOCUMENTS					
6,042,552 A	3/2000	Cornier	DE	3601453 A1	9/1986
6,068,641 A	5/2000	Varsseveld	DE	3615694 A1	11/1987
6,086,542 A	7/2000	Glowa et al.	DE	4038398 A1	6/1992
6,090,123 A	7/2000	Culp et al.	DE	4440035 A1	5/1996
6,113,594 A	9/2000	Savage	DE	19633124 A1	5/1997
6,119,973 A	9/2000	Galloway	DE	102006022827	12/2006
6,120,147 A	9/2000	Vijfinkel et al.	DE A61B 1/00	
6,120,462 A	9/2000	Hibner et al.	DE	102006022827 A1	12/2006
6,132,448 A	10/2000	Perez et al.	EP	0310285 A2	4/1989
6,149,633 A	11/2000	Maaskamp	EP	0557044 A1	8/1993
6,156,049 A	12/2000	Lovato et al.	EP	0582295 A2	2/1994
6,159,160 A	12/2000	Hsei et al.	EP	0606531 A2	7/1994
6,159,209 A	12/2000	Hakky	EP	0621008 A2	10/1994
6,203,518 B1	3/2001	Anis et al.	EP	0806183 A1	5/1997
6,217,543 B1	4/2001	Anis et al.	EP	1681022 A1	7/2006
6,224,603 B1	5/2001	Marino	EP	2093353 A	9/1982
6,244,228 B1	6/2001	Kuhn et al.	GB	2311468 A	10/1997
6,258,111 B1	7/2001	Ross et al.	GB	01-75416	5/1989
6,277,096 B1	8/2001	Cortella et al.	JP	2002-538889	11/2002
6,315,714 B1 *	11/2001	Akiba	JP	2003245247 A	9/2003
6,358,200 B1	3/2002	Grossi	JP	1006944 C2	3/1999
6,358,263 B2	3/2002	Mark et al.	NL	WO 81/01648 A1	6/1981
6,359,200 B1	3/2002	Day	WO	WO 92/11816 A2	7/1992
6,402,701 B1	6/2002	Kaplan et al.	WO	WO 93/07821 A1	4/1993
6,428,486 B2	8/2002	Ritchart et al.	WO	WO 93/15664 A1	8/1993
6,494,892 B1	12/2002	Ireland et al.	WO	WO 94/26181 A1	11/1994
6,585,708 B1	7/2003	Maaskamp	WO	WO 95/05777 A1	3/1995
6,610,066 B2	8/2003	Dinger et al.	WO	WO 95/10981 A1	4/1995
6,626,827 B1	9/2003	Felix et al.	WO	WO 95/10982 A1	4/1995
6,632,182 B1	10/2003	Treat	WO	WO 95/22935 A1	8/1995
6,656,132 B1	12/2003	Ouchi	WO	WO 95/30377 A1	11/1995
6,712,773 B1	3/2004	Viola	WO	WO 96/11638 A1	4/1996
6,837,847 B2 *	1/2005	Ewers et al.	WO	WO 96/26676 A1	9/1996
7,025,732 B2	4/2006	Thompson et al.	WO	WO 97/09922 A1	3/1997
7,150,713 B2	12/2006	Shener et al.	WO	WO 97/17027 A1	5/1997
7,226,459 B2	6/2007	Cesarini et al.	WO	WO 97/19642 A1	6/1997
7,249,602 B1	7/2007	Emanuel	WO	WO 97/24071 A1	7/1997
7,510,563 B2	3/2009	Cesarini et al.	WO	WO 97/34534 A1	9/1997
7,763,033 B2	7/2010	Gruber et al.	WO	WO 97/35522 A1	10/1997
7,922,737 B1	4/2011	Cesarini et al.	WO	WO 98/09569 A1	3/1998
8,061,359 B2	11/2011	Emanuel	WO	WO 98/10707 A1	3/1998
2001/0039963 A1	11/2001	Spear et al.	WO	WO 98/46147 A1	10/1998
2001/0047183 A1	11/2001	Privitera et al.	WO	WO 99/03407 A1	1/1999
2002/0058859 A1	5/2002	Brommersma	WO	WO 99/03409 A1	1/1999
2002/0165427 A1	11/2002	Yachia et al.	WO	WO 99/07295 A1	2/1999
2003/0050603 A1	3/2003	Todd	WO	WO 99/11184 A1	3/1999
2003/0050638 A1	3/2003	Yachia et al.	WO	WO 99/39648 A1	8/1999
2003/0078609 A1	4/2003	Finlay et al.	WO	WO 99/44506 A1	9/1999
2003/0114875 A1	6/2003	Sjostrom	WO	WO 99/60935 A1	12/1999
2005/0043690 A1	2/2005	Todd	WO	WO 00/12010 A1	3/2000
2005/0085692 A1	4/2005	Kiehn et al.	WO	WO 00/28890 A1	5/2000
2006/0036132 A1	2/2006	Renner et al.	WO	WO 00/33743 A1	6/2000
2006/0047185 A1	3/2006	Shener et al.	WO	WO 00/44295 A1	8/2000
2006/0241586 A1	10/2006	Wilk	WO	WO 00/47116 A1	8/2000
2008/0015621 A1	1/2008	Emanuel	WO	WO 00/57797 A1	10/2000
2008/0058588 A1	3/2008	Emanuel	WO	WO 01/35831 A1	5/2001
2008/0058842 A1	3/2008	Emanuel	WO	WO 01/58368 A1	8/2001
2008/0097468 A1	4/2008	Adams et al.	WO	WO 01/95810 A2	12/2001
2008/0097469 A1	4/2008	Gruber et al.	WO	WO 02/069808 A2	9/2002
2008/0097470 A1	4/2008	Gruber et al.	WO	WO 03/022164 A1	3/2003
2008/0097471 A1	4/2008	Adams et al.	WO	WO 03/077767 A1	9/2003
2008/0135053 A1	6/2008	Gruber et al.	WO	WO 2005/060842 A1	7/2005
2008/0146872 A1	6/2008	Gruber et al.	WO	WO 2005/096963 A2	10/2005
2008/0146873 A1	6/2008	Adams et al.	WO	WO 2006/105283 A2	10/2006
2008/0245371 A1	10/2008	Gruber	WO	WO 2006/121968 A2	11/2006
2008/0249366 A1	10/2008	Gruber et al.	WO	WO 2006/121970 A2	11/2006
2008/0249534 A1	10/2008	Gruber et al.	WO	WO 2007/044833 A2	4/2007
2008/0249553 A1	10/2008	Gruber et al.			
2008/0262308 A1	10/2008	Prestezog et al.			
2009/0270812 A1	10/2009	Litscher et al.			
2009/0270895 A1	10/2009	Churchill et al.			
2009/0270896 A1	10/2009	Sullivan et al.			
2009/0270897 A1	10/2009	Adams et al.			

OTHER PUBLICATIONS

ACMI Corporation, "Dolphin II Hysteroscopic Fluid Management Systems," ACMI Corporation, 2002 (1 page).
 ACMI Corporation, "DOLPHIN II and DESTIN-U-FLO Fluid Management Systems for Hysteroscopy", ACMI Corporation, 2002 (1 page).

(56)	References Cited	
	OTHER PUBLICATIONS	
	Action Closing Prosecution for 95/002,058 mailed Aug. 9, 2013 (34 pages). Advisory Action in U.S. Appl. No. 11/929,940 mailed Sep. 10, 2010 (3 pages). Bacsko "Uterine Surgery by Operative Hysteroscopy", European Journal of Obstetrics & Gynecology and Reproductive Biology, vol. 71, pp. 219-222, 1997 (4 pages). Baggish et al., "Diagnostic and Operative Hysterectomy," Mosby, pp. 97-105, 123-125, 127-132, 353-355, and 394-398, 1999 (27 pages). Claim chart for anticipation of claims 1-8 based on Banko US 3,945,375 (4 pages). Claim chart for anticipation of claims 1-8 based on Kresch US 5,456,689 (4 pages). Claim chart for anticipation of claims 1-8 based on Savage US 6,032,673 (13 pages). C.R. Bard, Inc, "The HydroFlex HD System" (1 page). Cravello et al., "Hysteroscopic Resection of Fibroids: Results with a 6-Year Follow-up Period", Journal of Gynecologic Surgery, vol. 15, No. 1, 1-5 1999 (5 pages). Defendant Hologic Inc.'s Preliminary, Non-Binding List of Asserted Prior Art References in <i>Smith & Nephew, Inc. v. Hologic, Inc.</i> Civil Action Nos. 11-CV-12064-RWZ and 10-CV-10951-RWZ, U.S. District Court for the District of Massachusetts, Feb. 8, 2012, (7 pages). Denial of Order for 95/001,955 mailed Jun. 4, 2012 (5 pages). Denial of Petition for 95/001,955 mailed Sep. 28, 2012 (5 pages). Dictionary definition of reciprocate, Merriam-Webster Dictionary, on-line edition, retrieved Mar. 20, 2013 (1 page). Dictionary definition of rotate, Merriam-Webster Dictionary, on-line edition, retrieved Mar. 20, 2013 (1 page). Dictionary definition of translate, Merriam-Webster Dictionary, on-line edition, retrieved Mar. 20, 2013 (1 page). Drews et al., "Surgical Approach to Myomas: Laparoscopy and Hysteroscopy", Seminars in Reproductive Endocrinology, vol. 10, No. 4, pp. 367-377, 1992 (11 pages). Dumesic et al., "A New Approach to Hysteroscopic Cannulation of the Fallopian Tube", Journal of Gynecologic Surgery, vol. 7, No. 1, pp. 7-9, 1991 (3 pages). Emanuel et al., "Long-term Results of Hysteroscopic Myomectomy for Abnormal Uterine Bleeding", Obstetrics & Gynecology, vol. 93, No. 5, Part I, pp. 743-748, 1999 (6 pages). European Patent Office Examination Report for Application No. 05 786 521.4-2305 dated Apr. 21, 2010 (4 pages). European Patent Office Examination Report for Application No. 05 786 521.4-2305 dated Sep. 26, 2010 (5 pages). Executed Expert Declaration of Dr. Henry A. Dominicis in support of Request for Inter Parties Reexamination of U.S. Patent No. 8,061,359, (150 pages). Executed Expert Declaration of Hal Walbrink in support of Request for Inter Parties Reexamination of U.S. Patent No. 8,061,359 (22 pages). Exhibit P to Hologic's Opposition to Smith & Nephew's Motion for Preliminary Injunction, Redacted, <i>Smith & Nephew, Inc. v. Hologic, Inc.</i> Civil Action No. 11-CV-12064-RWZ, filed Dec. 30, 2011 (99 pages). First Office Action for 95/002,058 mailed Sep. 19, 2012 (37 pages). Franchini et al., "Endometrial resection: a diagnostic tool in postmenopausal women", Gynecological Endoscopy, 8, pp. 111-114, 1999 (5 pages). "From Distention to Deficit Monitoring Taking the All-In-One Approach", W.O.M. World of Medicine (1 page). Gerber et al., "The Endoscapel: A new endoscopic instrument for supracervical hysterectomy and morcellation of masses; clinical evaluation", European Journal of Obstetrics & Gynecology and Reproductive Biology, 86, p. S12, 1999 (1 page). Gynecare, "Fluid Management System" Instructions for Use (26 pages). Gynecare "Motor Drive Unit" Instructions for Use (3 pages). Gynecare X-Tract, "Tissue Morcellator", Instructions for Use (3 pages). Gynescopic Corporation "Laser Fiber Director", Advertisement, Journal of Gynecologic Surgery, vol. 6, No. 1, 1990 (2 pages). Hess et al., "Textbook of Bilio-Pancreatic Disease", vol. III, PICCIN, e.g. Fig 6.5.1, pp. 1584-1586, 1997 (5 pages). Hologic's Opposition to Smith & Nephew's Motion for Preliminary Injunction, Redacted, <i>Smith & Nephew, Inc. v. Hologic, Inc.</i> , Civil Action No. 11-CV-12064-RWZ, filed Dec. 30, 2011 (26 pages). "HysteRo-Purator 1143-1 Technical Data" WISAP (2 pages). International Search Report for International Application No. PCT/US2011/053753 mailed on Dec. 20, 2011 (4 pages). International Search Report for International Application No. PCT/US2005/029807 mailed on Jun. 13, 2006 (5 pages). Japanese Office Action in Japanese Patent Application No. 2007-530014, dated Feb. 15, 2011 (10 pages). Karl Storz, Advertisement, Journal of Gynecologic Surgery, vol. 5, No. 4, 1989 (3 pages). Karl Storz, "Pilot a Course to Successful Outcomes", Intermetro Industries Corporation, 2001 (2 pages). Karl Storz "Uterine Resectoscopes for Endometrial Ablation and Resection", Advertisement, Journal of Gynecologic Surgery, vol. 6, No. 1, 1990 (3 pages). Lin et al. "Clinical Applications of a New Fujinon Operating Fiberoptic Hysteroscope", Journal of Gynecologic Surgery, vol. 6, No. 2, pp. 81-87, 1990 (7 pages). Mettler et al., "Pelvicopic uterine surgery" Surgical Endoscopy, 6, pp. 23-31, 1992 (9 pages). Neis et al., "Hysteroscopy: Textbook and Atlas", Thieme Medical Publishers, pp. 91-103, 1994 (13 pages). Nisolle et al., "Endometrial ablation with the Nd-YAG laser in dysfunctional bleeding" Minimally Invasive Therapy, vol. 1, pp. 35-39, 1991 (5 pages). Office Action in U.S. Appl. No. 09/486,977 mailed Sep. 7, 2005 (7 pages). Office Action in U.S. Appl. No. 11/780,759 mailed Jul. 22, 2010 (5 pages). Office Action in U.S. Appl. No. 11/780,759 mailed Jul. 26, 2010 (7 pages). Office Action in U.S. Appl. No. 11/780,759 mailed Jan. 5, 2011 (7 pages). Office Action in U.S. Appl. No. 11/929,938 mailed Jul. 30, 2010 (10 pages). Office Action in U.S. Appl. No. 11/929,938 mailed Jan. 5, 2011 (10 pages). Office Action in U.S. Appl. No. 11/929,940 mailed Dec. 30, 2009 (9 pages). Office Action in U.S. Appl. No. 11/929,940 mailed Jul. 1, 2010 (12 pages). Office Action in U.S. Appl. No. 95/001,933 mailed Jun. 5, 2012 (37 pages). Office Action in U.S. Appl. No. 95/001,933 mailed Apr. 1, 2013 (94 pages). Office Action in U.S. Appl. No. 95/001,933 mailed Sep. 19, 2013 (79 pages). Opening Claim Construction Brief of Defendant Hologic, Inc., from Massachusetts Civil Action No. 1:11-cv-12064-RWZ (Defendant's Opening Markman Brief) (24 pages). Opening Markman Brief of Plaintiff Smith & Nephew, Inc., from Massachusetts Civil Action No. 1:11-cv-12064-RWZ "Plaintiff's Opening Markman Brief" (24 pages). Order Granting Request for Reexam 95/001,933, mailed Jun. 5, 2012 (29 pages). Park et al., "Endoscopic Management of Uterine Myoma", Yonsei Medical Journal, vol. 40, No. 6, pp. 583-588, 1999 (6 pages). Patent Owner's Aug. 3, 2012 Response to Office Action for U.S. Appl. No. 95/001,933 mailed Jun. 5, 2012 (151 pages). Patent Owner's Jun. 3, 2013 Response to Office Action for U.S. Appl. No. 95/001,933 mailed Apr. 1, 2013 (75 pages). Patent Owner's Oct. 21, 2013 Response to Action Closing Prosecution in 95/001,933 mailed Sep. 19, 2013 (218 pages). Patent Owner's Jan. 22, 2013 Response to Office Action for 95/002,058 mailed Sep. 9, 2012 (379 pages). Patent Owner's Sep. 9, 2013 Response to Action Closing Prosecution for 95/002,058 dated Aug. 9, 2013 (7 pages).	

(56)

References Cited

OTHER PUBLICATIONS

Patent Owner's Oct. 25, 2010 Response to Office Action for U.S. Appl. No. 11/780,759 mailed Jul. 26, 2010 (13 pages).

Patent Owner's Mar. 31, 2011 Response to Office Action for U.S. Appl. No. 11/780,759 mailed Jan. 5, 2010 (15 pages).

PCT International Preliminary Report on Patentability for Application No. PCT/US2005/029807 dated Feb. 28, 2007, (9 pages).

Petition for Review for 95/001,955, Jul. 3, 2012 (36 pages).

Reexam Order for 95/002,058 mailed Sep. 19, 2012 (54 pages).

Reexamination Litigation Search Report CRU 3999 filed Apr. 2, 2012 in U.S. Appl. No. 95/001,955 (33 pages).

Reference AQ "Fishing Reel produced and sold by Shimano of Japan in to the U.S. prior to Oct. 26, 2001," filed Oct. 17, 2005 in the prosecution file history of U.S. Appl. No. 09/983,810 (7 pages).

Request for Inter Partes Reexamination of U.S. Patent No. 8,061,359, filed Apr. 2, 2012 (265 pages).

Richard Wolf "Morce- Power 2306" Electronic Morcellator (2 pages).

Richard Wolf "The Fluid Manager" (2 pages).

Right of Appeal Notice mailed Jan. 14, 2014 for U.S. Appl. No. 95/001,933 (58 pages).

Second Office Action for 95/002,058 mailed Jan. 24, 2014 (31 pages).

Sheath et al., "Fiberoptic Light for Oophorectomy at Vaginal Hysterectomy", Journal of Gynecologic Surgery, vol. 14, No. 3, pp. 119-22, 1998 (4 pages).

Sugimoto "A Color Atlas of Hysteroscopy" Springer-Verlag Tokyo, 1999 (17 pages).

Third Party Response to Office Action for U.S. Appl. No. 95/001,933 mailed Apr. 1, 2013 (101 pages).

Third Party Response to Office Action for U.S. Appl. No. 95/001,933 mailed Jun. 5, 2012 (777 pages).

Third Party Response in U.S. Appl. No. 95/001,933 to Action Closing Prosecution mailed Sep. 19, 2013 (38 pages).

Third Party Response to First Office Action for 95/002,058 mailed on Sep. 19, 2012.

Third Party Response in 95/002,058 to Action Closing Prosecution mailed Apr. 1, 2013 (101 pages).

Third Party Response in 95/002,058 to Action Closing Prosecution mailed Aug. 9, 2013 (25 pages).

Valle "Hysteroscopic Removal of Submucous Leiomyomas", Journal of Gynecologic Surgery, vol. 6, No. 1, pp. 89-96, 1990 (9 pages).

Weck "A Direct Path to Diagnostic and Operative Control: The Weck-Baggish Hysteroscopy System" Advertisement, Journal of Gynecologic Surgery, vol. 7, No. 1, 1991 (2 pages).

Williamson et al., Editorial 1 "Complications of hysteroscopic treatments of menorrhagia", British Journal of Anesthesia, vol. 77, No. 3, pp. 305-308, 1996 (4 pages).

European Patent Office Examination Report for Application No. 11 770 261.3-1657 dated Feb. 11, 2014 (4 pages).


PCT International Preliminary Report on Patentability for Application No. PCT/US2011/053753 dated Apr. 2, 2013 (7 pages).

Chinese Office Action for Chinese Application No. 201180046921.6, mailed Dec. 23, 2014, 29 pages, with English language translation.

First Office Action for Japanese Patent Application No. 2013-531779 dated May 18, 2015, with English translation, 6 pages.

Patent Examination Report No. 1 for Australian Patent Application No. 2011308834 dated Jun. 11, 2015, 3 pages.

* cited by examiner

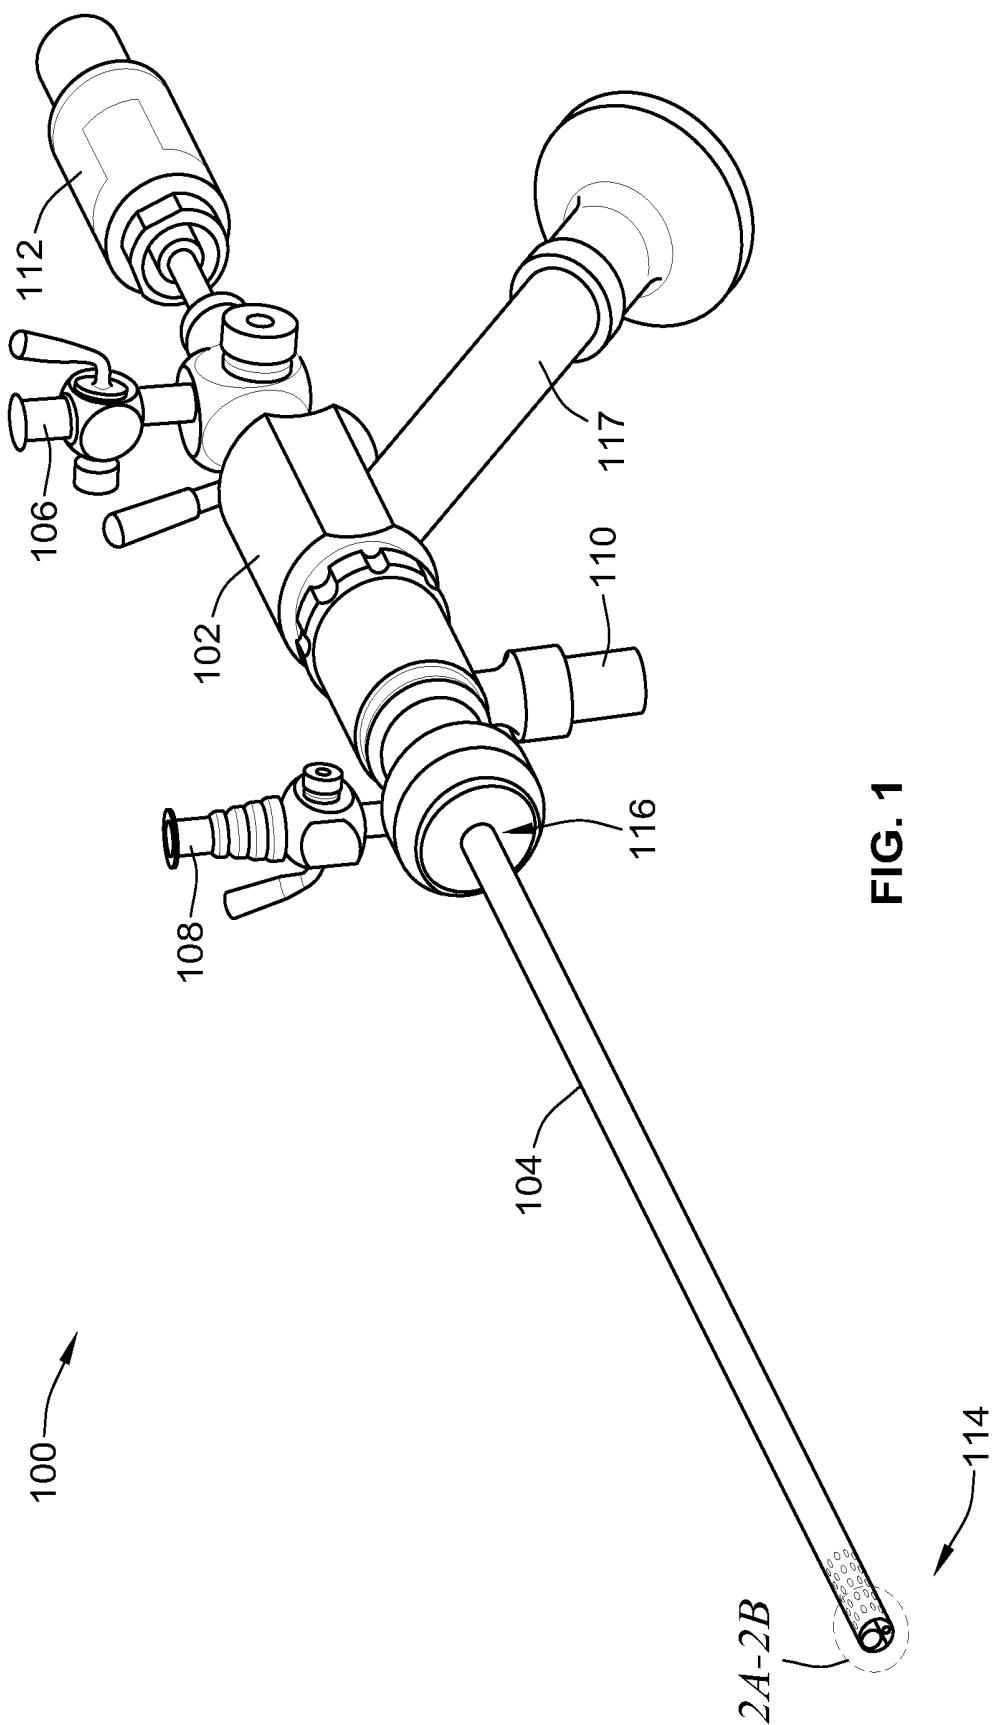

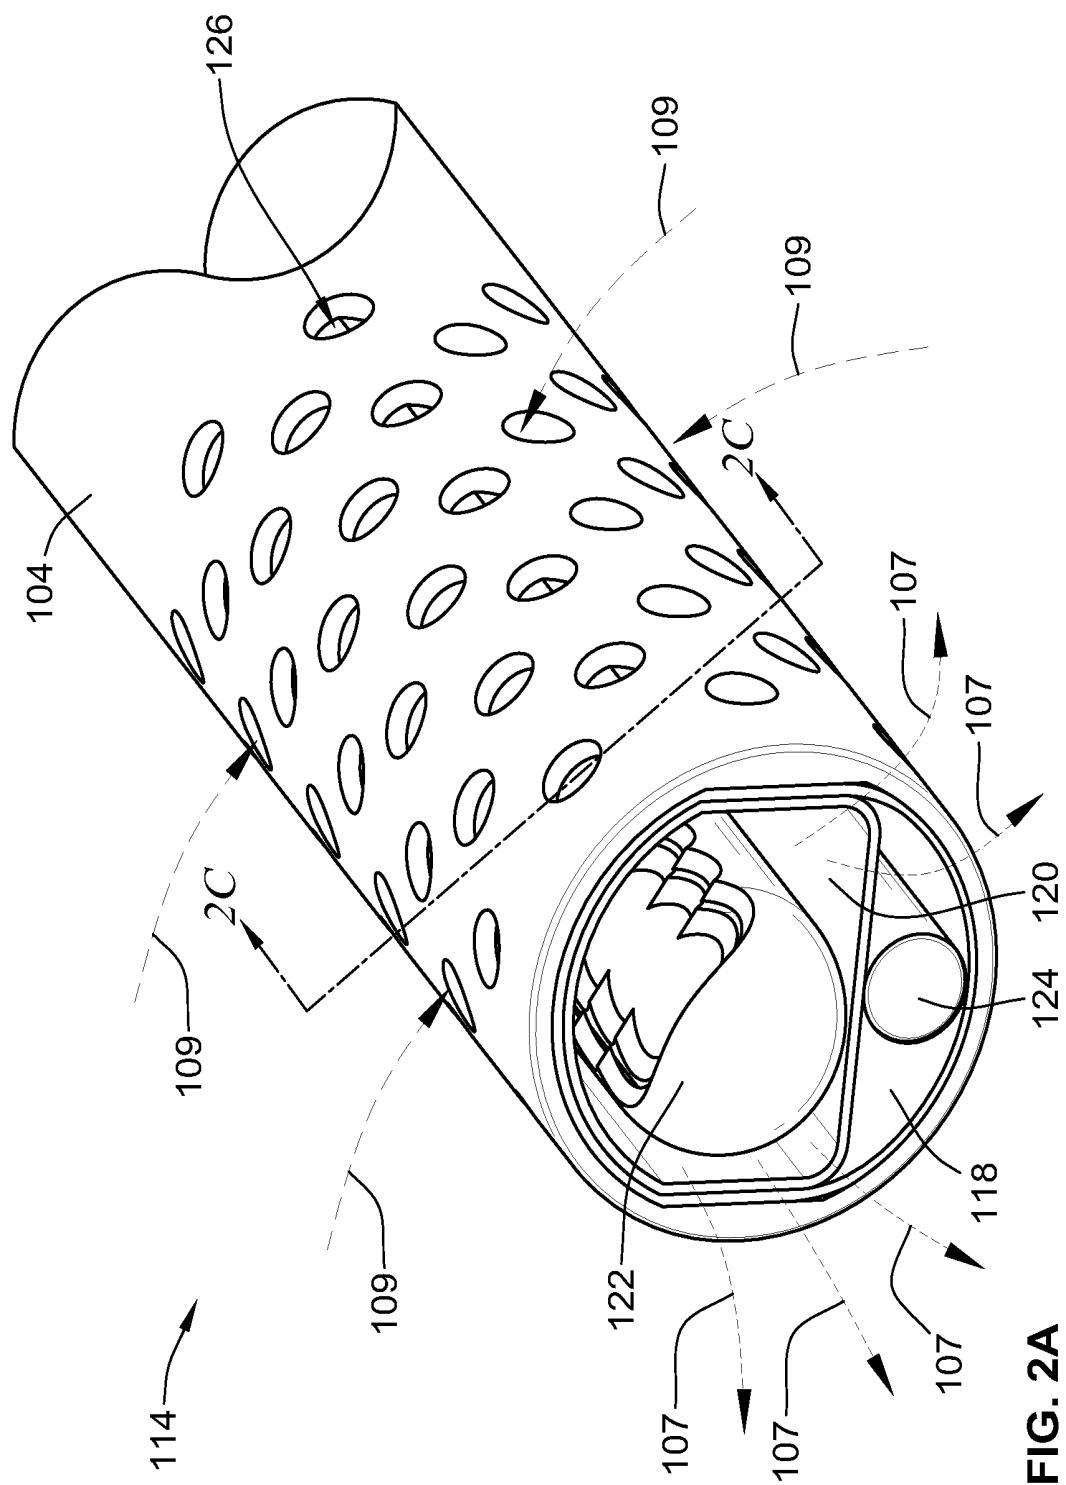


FIG. 2A

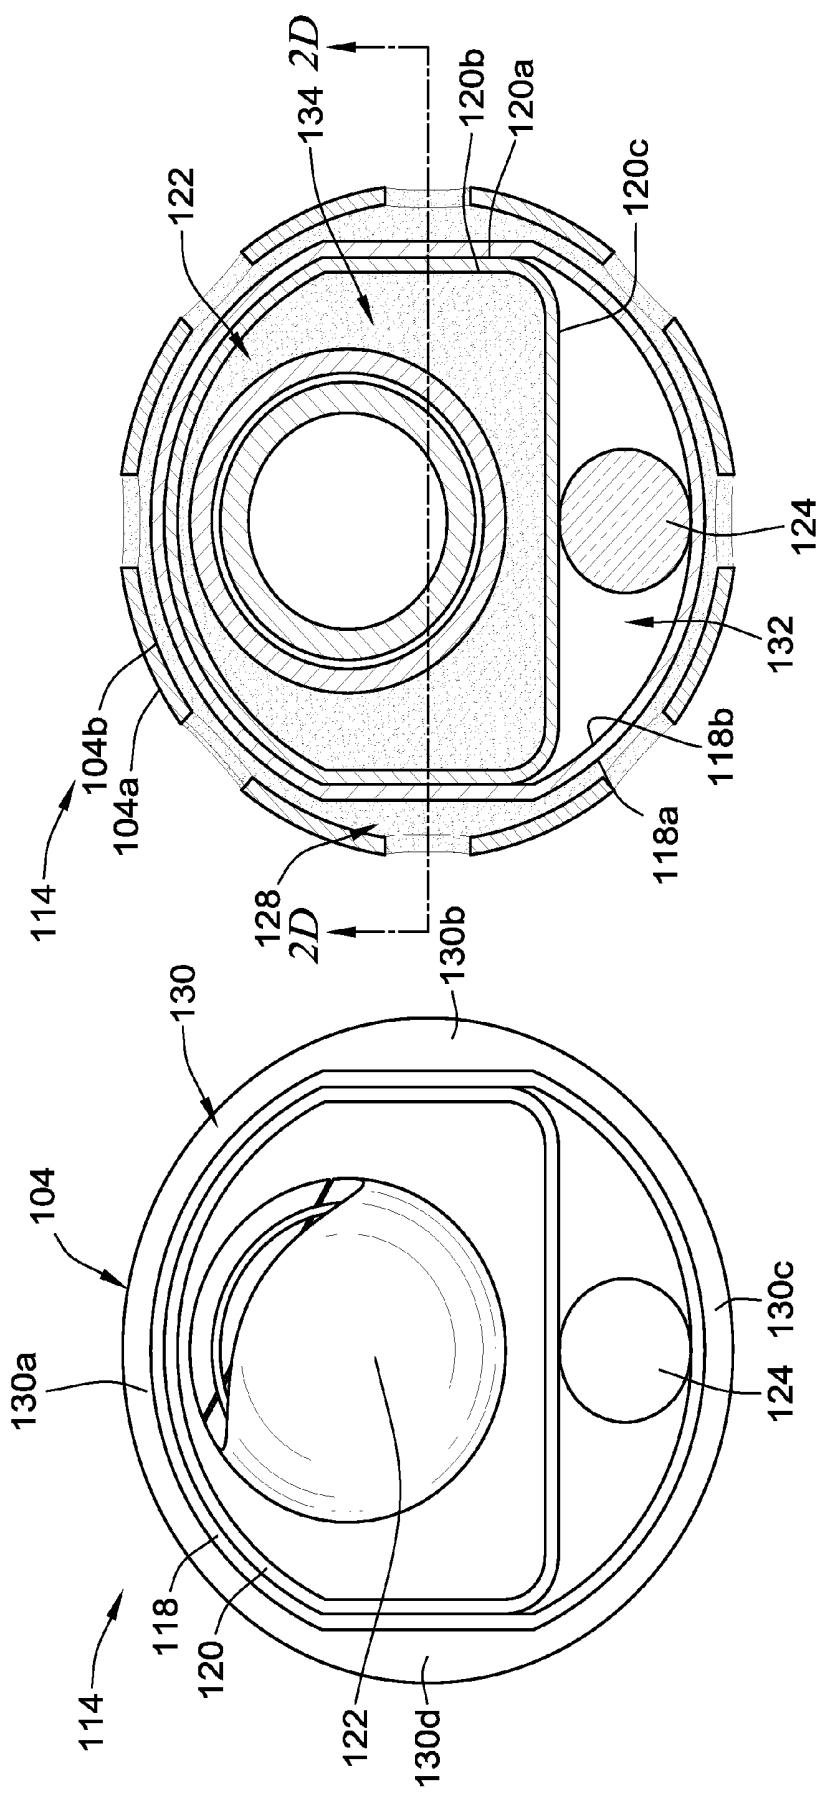


FIG. 2C

FIG. 2B

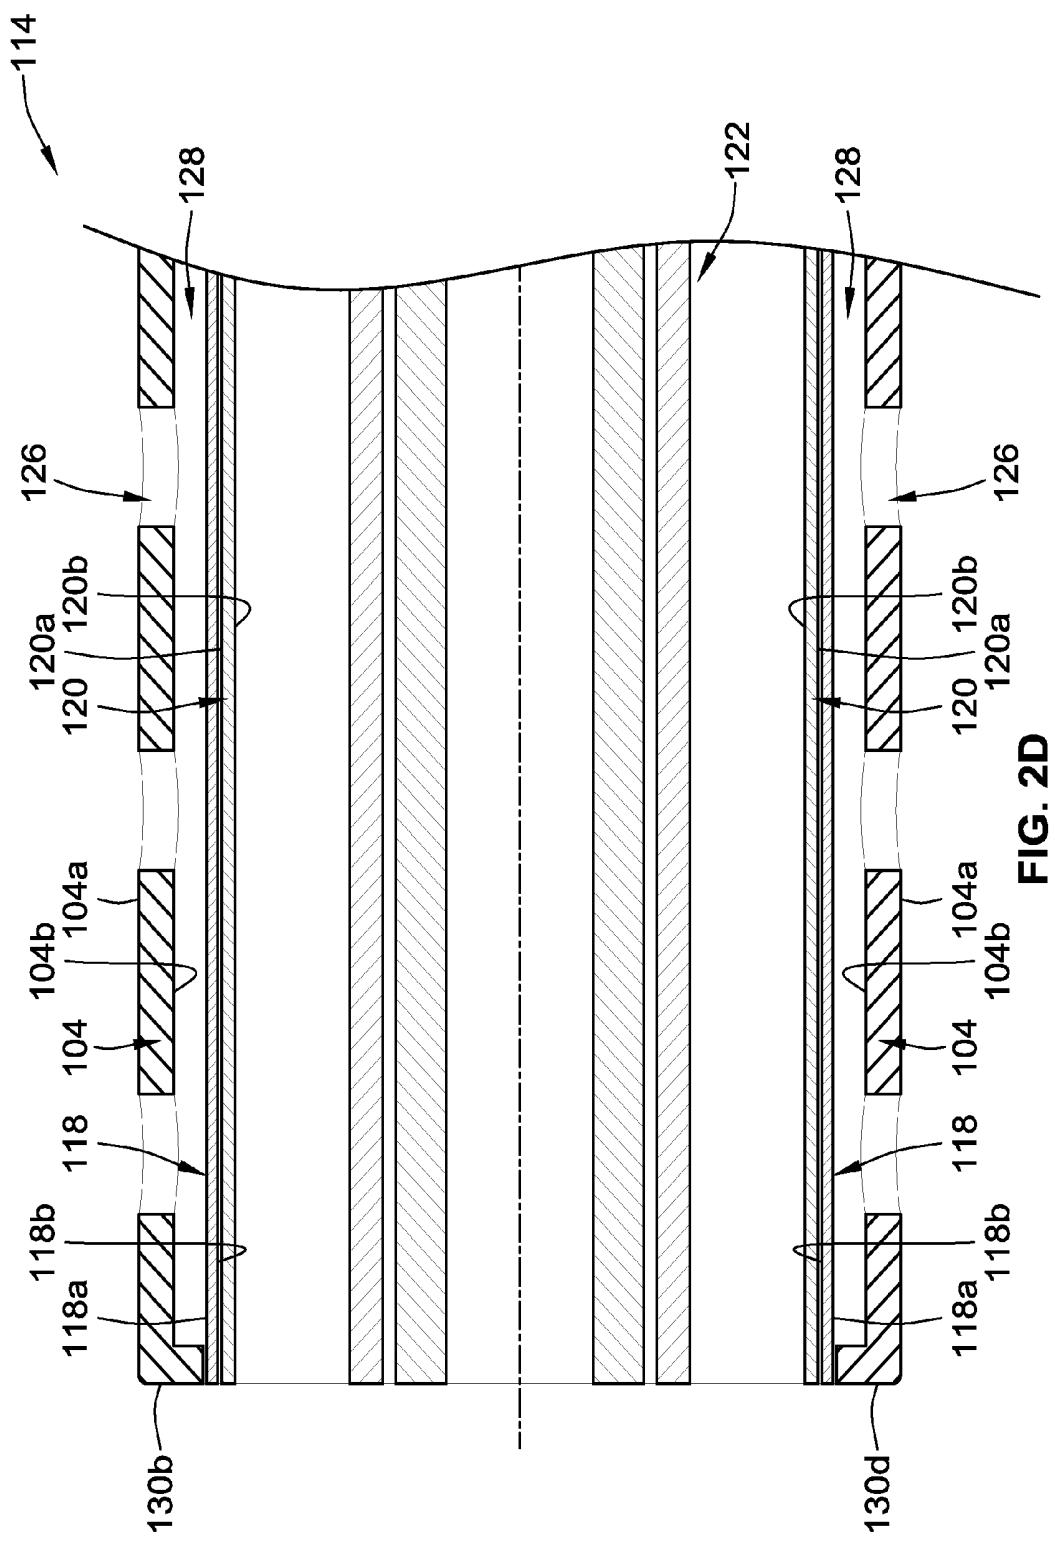


FIG. 2D




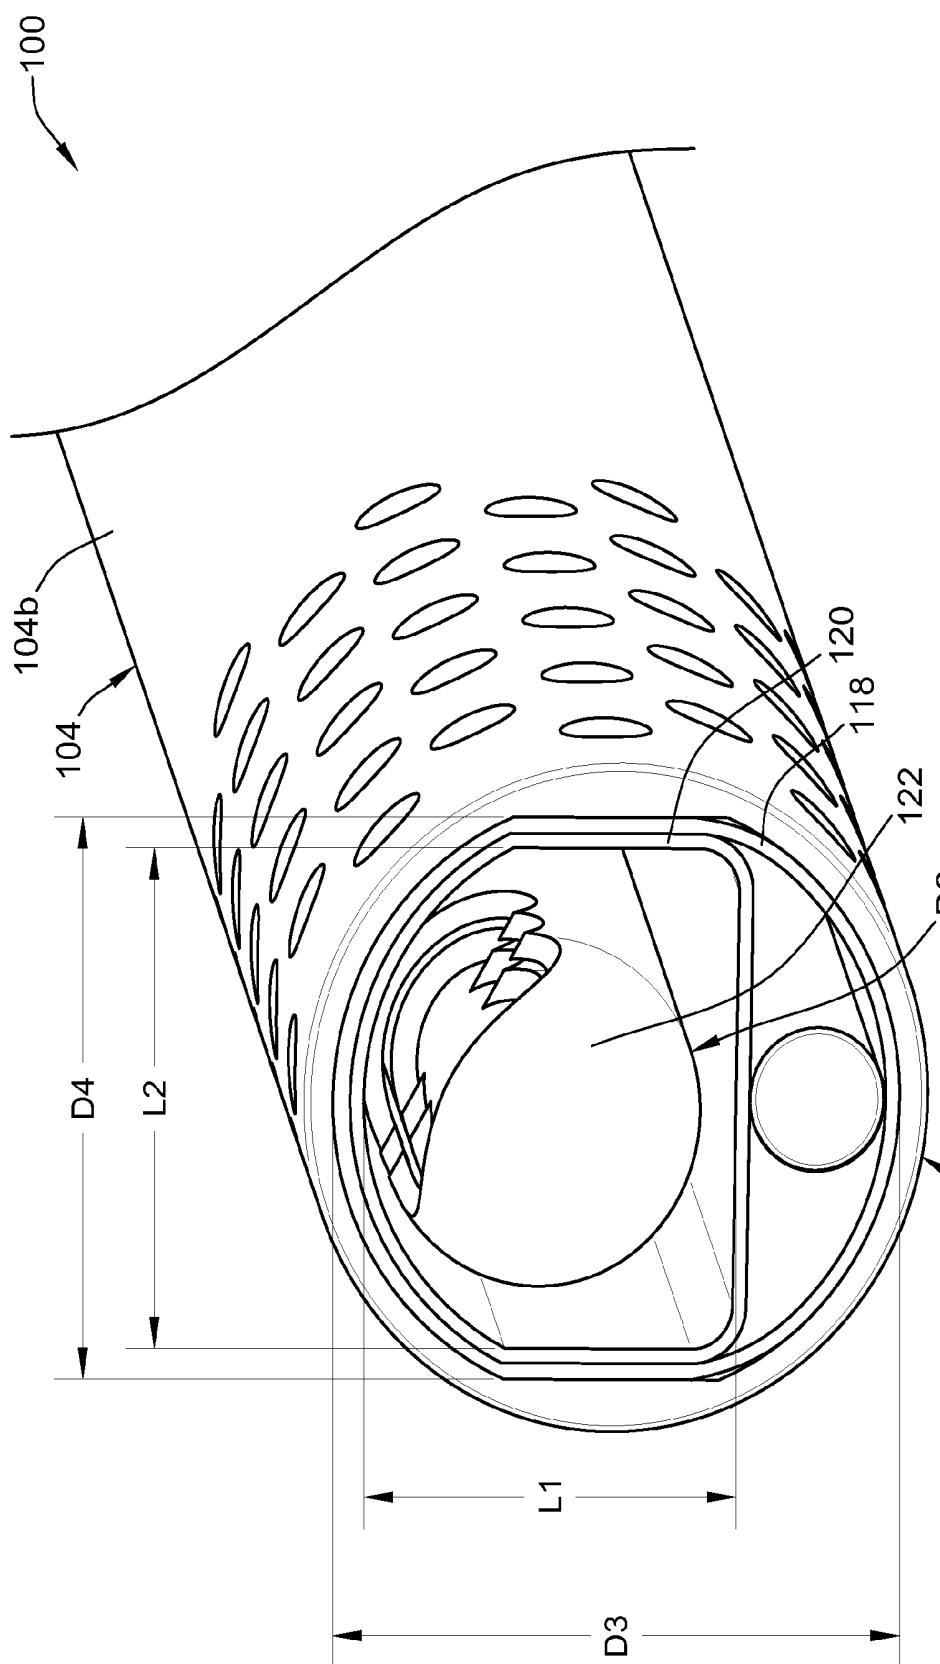


FIG. 3

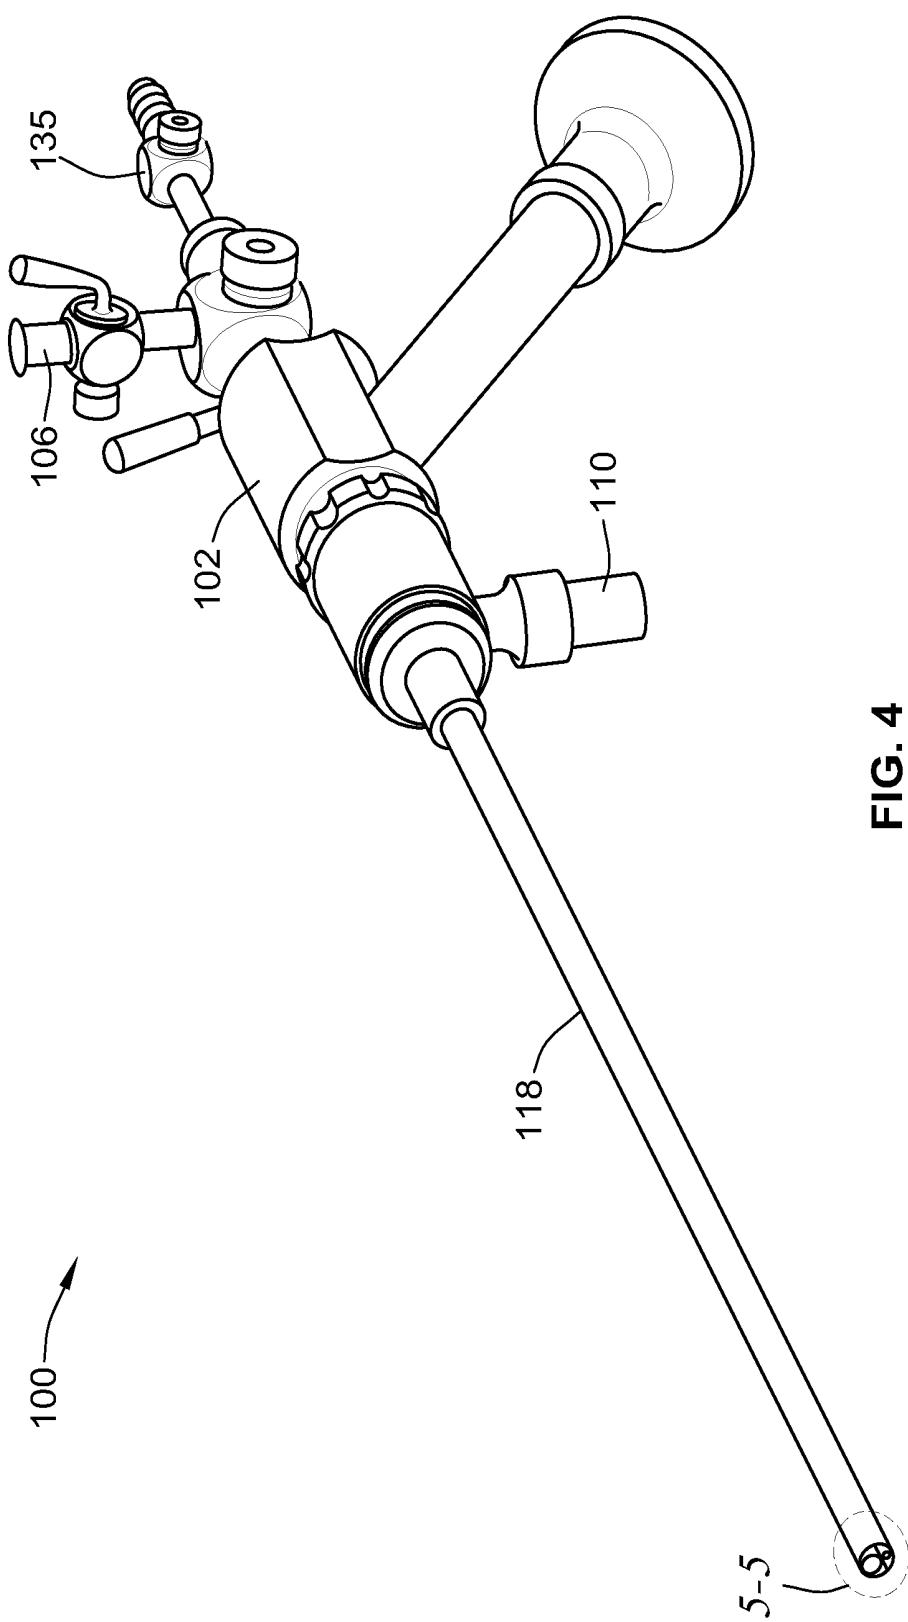

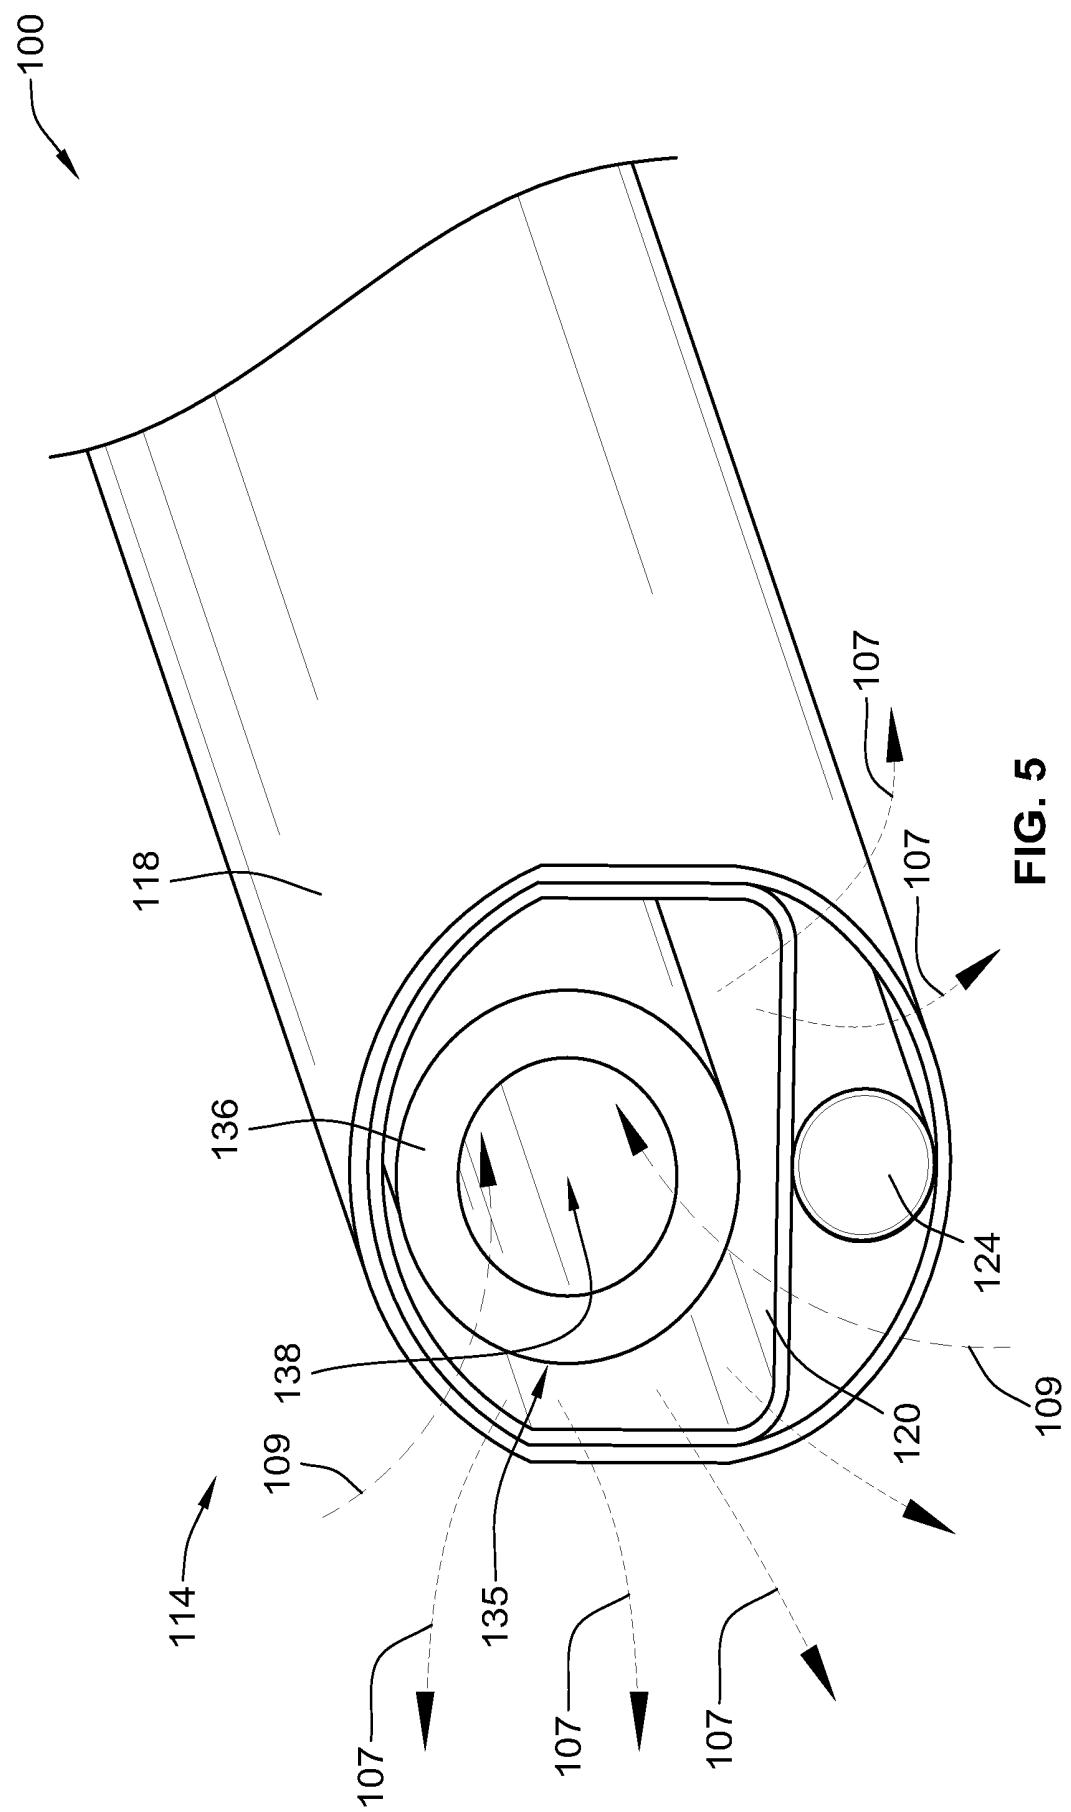

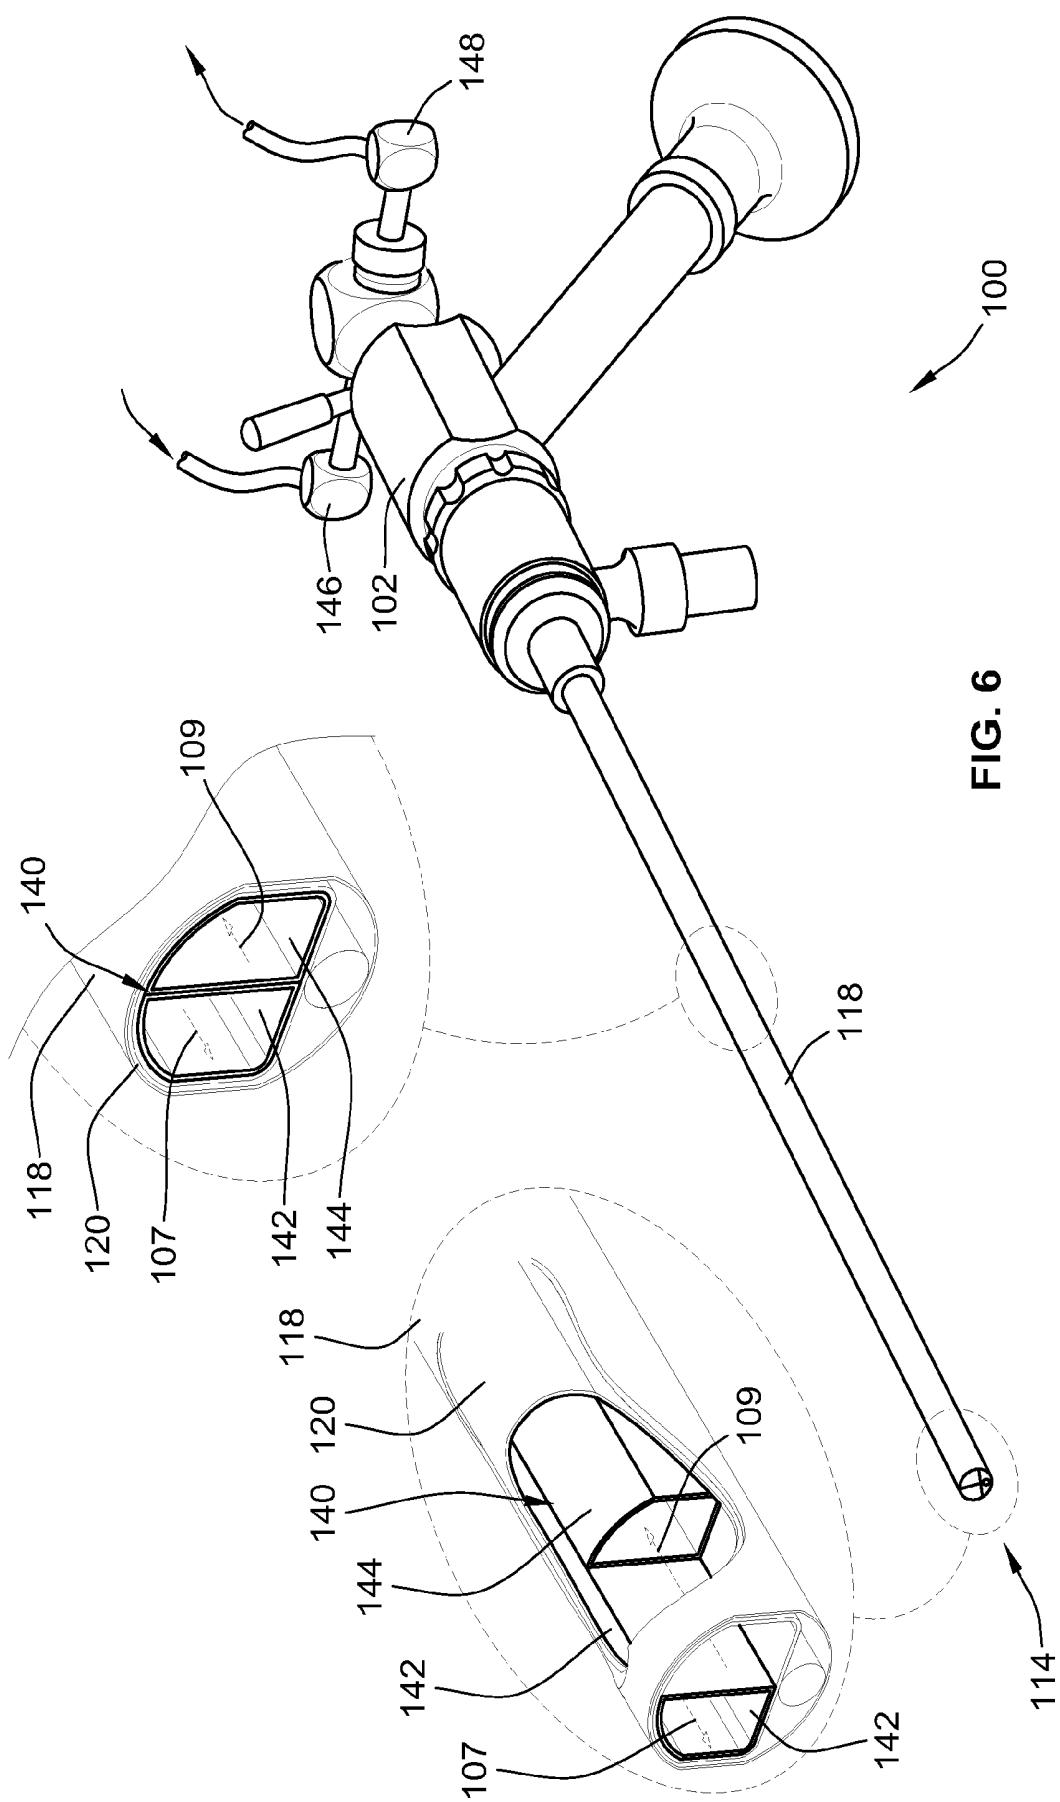

HYSTEROSCOPIC SYSTEM

FIELD OF THE INVENTION

The present invention relates generally to hysteroscopy systems, and, more particularly, to a hysteroscopy system having a small size for use in an office setting.

BACKGROUND OF THE INVENTION

Hysteroscopy refers generally to the inspection of a uterine cavity using a hysteroscope with access through the cervix. As such, hysteroscopy allows diagnosis of intrauterine pathology and, furthermore, can be used for surgical intervention. The hysteroscope typically includes a scope and a sheath.

One problem associated with some current hysteroscopy systems is that they must be used in an operating room setting with the patient being under some type of anesthesia. Anesthesia is required in particular because the size of current hysteroscopes is large and, as such, they can cause discomfort and pain to the patient. For example, a typical hysteroscope may have an outermost diameter of about 9 millimeters. Such hysteroscopes include a scope having a diameter of about 8 millimeters and a sheath having a diameter of about 9 millimeters. In comparison, scientific literature on the subject agrees that hysteroscopy can be performed using a vaginal approach, which can be performed in an office setting, only when the outermost diameter of the hysteroscope is about 6 millimeters or less.

Another problem associated with current scopes is that they typically include a blunt flange at the scope distal end. The flange extends outwardly from the scope and make it difficult, if not impossible, to use the scope without the sheath and/or without an obturator. Accordingly, the size of some current hysteroscopes is limited to the size of the scope and the sheath, e.g., a diameter of 9 millimeters.

What is needed, therefore, is a hysteroscope system for an office setting that addresses the above-stated and other problems.

SUMMARY OF THE INVENTION

According to one aspect of the present invention, a hysteroscopy system is directed to performing a medical procedure in an office setting. The hysteroscopy system includes a scope having an outer surface, an internal channel defined by an inner surface, and a distal end. A sheath is removably coupled to the scope and has a tip at which a distal flange extends internally towards the outer surface of the scope. The sheath also has an inner surface and a plurality of outflow holes near the distal flange. An outflow channel is formed between the inner surface of the sheath and the outer surface of the scope, the distal flange forming a distal end of the outflow channel. An operative channel is formed within the internal channel of the scope for receiving at least one of a surgical tool and an inflow fluid, and a visualization channel is formed adjacent to the operative channel for receiving a visualization device.

According to yet another aspect of the invention, a hysteroscopy system for a medical procedure includes a scope in the form of an elongated tubular member having an outer surface and an internal surface. The internal surface of the scope defines an internal channel of the scope. A sheath is in the form of an elongated tubular member removably coupled to the scope, the sheath having an outer surface and an internal surface. The sheath has a flange extending internally towards

the outer surface of the scope at a distal end of the sheath. An operative member is located within the internal channel of the scope and is in the form of an elongated D-shape tubular member. The operative member has an outer surface and an internal surface, the outer surface being spaced away from the internal surface of the scope to form a visualization channel.

According to yet another aspect of the invention, a hysteroscopy system includes a scope having an outer surface and an internal channel, and a sheath removably coupled to the scope. The sheath has an inner surface and a distal flange, the distal flange extending internally towards the outer surface of the scope. An outflow channel is formed between the inner surface of the sheath and the outer surface of the scope, the distal flange forming a distal end of the outflow channel between the scope and the sheath.

Additional aspects of the invention will be apparent to those of ordinary skill in the art in view of the detailed description of various embodiments, which is made with reference to the drawings, a brief description of which is provided below.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a hysteroscope system.

FIG. 2A is an enlarged perspective view of a distal end of the hysteroscope system.

FIG. 2B is an enlarged side view of the distal end of the hysteroscope system.

FIG. 2C is an enlarged cross-sectional end view of the distal end of the hysteroscope system.

FIG. 2D is an enlarged cross-sectional top view of the distal end of the hysteroscope system.

FIG. 3 shows dimensions associated with the distal end of FIG. 2A.

FIG. 4 is a perspective view of the hysteroscope system having a sheath removed from a scope.

FIG. 5 is an enlarged perspective view of the distal end of the hysteroscope system of FIG. 4.

FIG. 6 is a perspective view of an alternative embodiment of the hysteroscope system.

While the invention is susceptible to various modifications and alternative forms, specific embodiments have been shown by way of example in the drawings and will be described in detail herein. It should be understood, however, that the invention is not intended to be limited to the particular forms disclosed. Rather, the invention is to cover all modifications, equivalents, and alternatives falling within the spirit and scope of the invention as defined by the appended claims.

DETAILED DESCRIPTION

Referring to FIG. 1, a hysteroscope system 100 includes a hysteroscope 102 having, inter alia, a sheath 104, an inflow valve 106, an outflow valve 108, a light post 110, and a morcellator 112. The sheath 104 is a generally an elongated tubular member that has a distal end 114 and a proximal end 116. The hysteroscope system 100 also includes an arm 117 that is connected to an imaging device (e.g., a camera) to capture images received via a visualization device (e.g., visualization device 124).

According to some exemplary embodiments, the hysteroscope system 100 is intended for morcellation of uterine pathology with a scope and accessories having a sufficiently small diameter that can be inserted into a patient's uterus using the vaginal approach. In particular, the hysteroscope system 100 provides a way to minimize patient pain because a tenaculum and speculum are not typically used.

Furthermore, anesthesia is not needed and the medical procedures can be performed in an office setting. This may result, for example, in a quicker surgery with less pain and quicker recovery, and may potentially lower the cost of the surgery. Yet another advantage of the hysteroscope system 100 is that a surgeon has the option to decide if they prefer greater flow instruments (e.g., with a coupled sheath 104) or smaller diameter instruments (e.g., with a removed sheath 104), depending on the patient case.

Referring to FIG. 2A, the sheath 104 is removably coupled to a scope 118, which is generally an elongated tubular member having (similar to the sheath 104) a distal end 114 and a proximal end 116. More specifically, the sheath 104 is slidably fitted in an overlapping manner over the scope 118. The scope 118 includes an operative member 120, which is in the form of an elongated D-shape tubular member.

The operative member 120 receives internally a surgical tool 122, which can be selected from a variety of different tools. For example, the surgical tool 122 can be a rotary morcellator, a reciprocating morcellator, or a morcellator having both reciprocal and rotary capabilities. The scope 118 further includes a visualization device 124. The visualization device 124 is adjacent to the operative member 120 and can include various image devices. For example, the visualization device 124 can include fiber-optic technology for illumination and image transmission.

To maintain continuous outflow, a plurality of outflow holes 126 are formed near the distal end 114 of the sheath 104. The inflow valve 106 (shown in FIG. 1) regulates inflow of a liquid through the operative member 120, as represented by the arrows 107 extending from the operative member 120. The liquid is used, for example, to distend and irrigate the uterus of a patient. Furthermore, the liquid is generally received from an access pump, which delivers the fluid to produce a substantially constant predetermined pressure level within a joint cavity, e.g., a uterus. The outflow valve 108 (shown in FIG. 1) regulates outflow of the liquid through the outflow holes 126 via an outflow channel 128 (shown in FIG. 2C) formed between the sheath 104 and the scope 118. The outflow of the liquid is represented by the arrows 109 extending into the outflow holes 126. The outflow liquid is generally sent to a waste container.

Referring to FIG. 2B, the sheath 104 has at the distal end 114 a flange 130 extending inwardly towards the scope 118 to form a closed end of the outflow channel 128 (shown in FIG. 2C). The flange 130 has a generally oval shape and includes two pairs of opposite sides 130a-130d.

According to the illustrated embodiment, the shape of the flange 130 is non-uniform. For example, a second side 130b extends a greater distance internally towards the center of the scope 118 than a first side 130a. Similarly, based on the symmetric features of this embodiment, a fourth side 130d extends a greater distance internally towards the center of the scope 118 than a third side 130c. In alternative embodiments, the flange 130 can have different shapes and sizes.

Referring to FIGS. 2C-2D, the sheath 104 has an outer surface 104a and an internal surface 104b, and the scope 118 has an outer surface 118a and an internal surface 118b. The internal surface 104b of the sheath 104 defines an internal channel in which the scope 118 and the visualization device 124 are located. The internal surface 118b of the scope 118 defines an internal channel in which the outer member and thus the surgical tool 122 is located.

The operative member 120 has an outer surface 120a, an internal surface 120b, and a flat outer surface 120c (clearly shown in FIG. 2C). The flat outer surface 120c is spaced away from the internal surface 118b of the scope 118 to form a

visualization channel 132 (clearly shown in FIG. 2C) in which the visualization device 124 is located. The visualization channel 132 is only a small part of the larger internal channel of the scope 118.

The outflow channel 128 is formed between the internal surface 104b of the sheath 104 and the outer surface 118a of the scope 118. An inflow channel 134 is formed in the internal channel of the scope 118. If the surgical tool 122 is removed, the inflow channel 134 is simply the entire internal channel of the scope 118. If the surgical tool 122 is in place, the inflow channel 134 is limited to the area between the surgical tool 122 and the internal surface 120b of the operative member 120.

Referring to FIG. 3, the hysteroscopy system 100 is designed to have a size that can be used in an office setting. Specifically, the outer most diameter is designed to be about 6 millimeters or less. According to the illustrated embodiment, the outer diameter D1 of the sheath 104 (which is the same as the diameter of the outer surface 104b) is about 5.6 millimeters. For example, in an alternative embodiment the diameter of the sheath 104 is 5.5 millimeters. The outer diameter D2 of the surgical tool 122 (e.g., morcellator) is about 2.9 millimeters.

The scope 118 has an oval shape with a long diameter D3 of about 5.15 millimeters and a short diameter D4 of about 4.6 millimeters. The operative member 120 has a curvature dimension L1 of about 3.1 millimeters and a flat dimension L2 of about 3.95 millimeters.

The relatively small dimensions of the hysteroscopy system 100 allows a patient to be treated in an office setting. Generally, medical procedures may be provided to a patient with the use of the current hysteroscopy system 100 such that little or no anesthesia may be necessary. Clearly, one advantage of the hysteroscopy system 100 is that it is sufficiently small in diameter to be suitable for the vaginoscopic approach.

Referring to FIG. 4, the hysteroscopy system 100 is also usable without the sheath 104 while still providing continuous flow via a diagnostic cannula 135 (e.g., a cannula having a diameter of about 2.9 millimeters). Specifically, the sheath 104 is removed to allow only the insertion of the scope 118 into a patient, e.g., into an uterus. The removal of the sheath 104 decreases the outermost diameter of the hysteroscopy system 100. For example, in accordance with the dimensions described above in reference to FIG. 3, the outermost diameter decreases to about 5.15 millimeters (the long diameter D3) from about 5.6 millimeters (the outer diameter D1). When the sheath 104 is removed, the outflow can be provided by an operation tool, such as the morcellator 112 described above (shown in FIGS. 1-3), or by the diagnostic cannula 135.

In contrast to previous scopes, the scope 118 does not have a flange extending outwards from its distal end. The outward extending flange of the previous scopes unnecessarily increased the outermost diameter of the respective scopes and created an obtrusive distal end that made it difficult, if not impossible, to introduce into a patient without a sheath and obturator.

Referring to FIG. 5, the hysteroscopy system can be used for diagnostic purposes when the sheath 104 is removed. The sheath 104 is likely to be used in operative cases mostly to clear the visual field before introduction of a morcellator blade. The diagnostic cannula 135, which has a distal end 136, is used to create a smaller overall diameter of the system for diagnostic purposes. According to the dimensions described above, a reduction of approximately 0.5 millimeters can be achieved by removing the sheath 104. Another advantage of the cannula 135 is that it can be made reusable.

Yet another advantage of the cannula 135 is that it can be used to distend and irrigate the patient's uterus during the diagnostic procedure.

The cannula 135 allows for continuous outflow but does not extend beyond the distal end of the scope 118. For example, the cannula 135 provides a replacement for the outflow channel 128, which is removed with the removal of the sheath 104. Specifically, the cannula 135 provides an alternative outflow channel 138 to replace the outflow channel 128 formed by the sheath 104. As such, continuous flow can be maintained even if the sheath 104 is removed.

Referring to FIG. 6, the hysteroscope system 100 alternatively includes a flow device 140 inserted within the operative member 120. The flow device 140 has an inflow tubular element 142 and an outflow tubular element 144, which can be conjoined elements or separate elements.

The distal ends of the tubular elements 142, 144 terminate at different points within the operative member 120. Preferably, the distal end of the inflow tubular element 142 terminates at the distal end 114 of the scope 118, and the distal end of the outflow tubular element 144 terminates some distance away from the distal end 114 within the operative member 120. The termination of tubular elements 142, 144 at different points along the operative member 120 eliminates the possibility of fluid short-circuit and provides better circulation and, hence, irrigation within the uterus.

According to one example, the flow device 140 is made of stainless steel and, as such, can be a reusable device. According to another example, the flow device 140 is made from a much more cost-effective material, such as a polymer. If a polymer is used, the flow device 140 will typically be considered a single-use device.

In practice, for example, a surgeon will insert the flow device 140 into the operative member 120 of the hysteroscope 102 prior to introduction into the uterus of a patient. After hysteroscope introduction into the uterus, an inflow valve 146 of the flow device 140 will be opened and the uterus will be distended. Then, by opening an outflow valve 148 of the flow device 140, irrigation is achieved. In the case of a diagnostic procedure, the flow device 140 could stay in place for the duration of the surgery. In the case of an operative procedure, the flow device 140 is removed and an operative tool (e.g., the morcellator 112) is inserted into the scope 118.

While the best modes for carrying out the present invention have been described in detail, those familiar with the art to which this invention relates will recognize various alternative designs and embodiments for practicing the invention within the scope of the appended claims. For example, the sheath 104, the scope 118, and the surgical tool 122 can be circular, oval, or any other smooth shape (i.e., an unobtrusive shape such as a shape that does not have a outward extending flange). In another example, the operative member 120 can have a circular shape or any other similar shape to the illustrated D-shape.

What is claimed is:

1. A hysteroscopy system, the system comprising:
a scope having an outer surface and an internal channel defined by an inner surface;
a sheath removably coupled to the scope and having a tip at which a distal flange extends internally in a protruding manner towards the outer surface of the scope, the sheath further having an inner surface;
an outflow channel formed between the inner surface of the sheath and the outer surface of the scope, the distal flange extending internally in the protruding manner to form a distal end of the outflow channel between the scope and the sheath;

an operative channel formed within the internal channel of the scope; and
a visualization channel formed adjacent to the operative channel,

wherein the distal flange and the sheath are monolithic, a first edge portion of the distal flange facing towards the scope protrudes a first distance towards the outer surface of the scope in a radial direction, a second edge portion of the distal flange facing towards the scope protrudes a second distance towards the outer surface of the scope in the radial direction, and the first distance is different than the second distance.

2. The hysteroscopy system of claim 1, further comprising a surgical tool inserted within the operative channel, the surgical tool being selected from a group consisting of a rotary morcellator, a reciprocating morcellator, or a rotary and reciprocating morcellator.

3. The hysteroscopy system of claim 1, wherein the visualization channel is configured for receiving a visualization device.

4. The hysteroscopy system of claim 1, further comprising an operative member inserted within the scope, the operative member having an outer surface and an internal channel.

5. The hysteroscopy system of claim 4, wherein the outer surface of the operative member has a generally D-shape.

6. The hysteroscopy system of claim 4, further comprising a tool inserted within the internal channel of the operative member.

7. The hysteroscopy system of claim 6, further comprising a fluid flowing through the internal channel of the operative member, the fluid flowing between the tool and the internal channel of the operative member.

8. The hysteroscopy system of claim 1, wherein the sheath has an outer diameter of about 5.6 millimeters and a long diameter of the scope is about 5.15 millimeters.

9. The hysteroscopy system of claim 1, wherein the distal flange extends internally in the protruding manner towards the outer surface of the scope such that an internal diameter of a proximal end of the sheath is greater than an internal diameter of the distal flange.

10. A hysteroscopy system, the system comprising:
a scope having an outer surface and an inner surface relative to a radial direction of the scope, the inner surface defining an inflow channel and the outer surface being continuous through a distal end of the hysteroscopy system;
a sheath removably coupled to the scope, the sheath having an outer surface and an inner surface relative to the radial direction, the sheath further having a distal flange protruding from the inner surface of the sheath and towards the outer surface of the scope at the distal end of the hysteroscopy system; and
an outflow channel formed between the inner surface of the sheath and the outer surface of the scope, the distal flange engaging the outer surface of the scope to form an end of the outflow channel between the scope and the sheath at the distal end of the hysteroscopy system,
wherein the distal flange and the sheath are monolithic, a first edge portion of the distal flange facing towards the scope protrudes a first distance towards the outer surface of the scope in the radial direction, a second edge portion of the distal flange facing towards the scope protrudes a second distance towards the outer surface of the scope in the radial direction, and the first distance is different than the second distance.

11. The hysteroscopy system of claim 10, wherein the distal flange has an oval shape with a non-uniform diameter.

12. The hysteroscopy system of claim **11**, wherein the oval shape has two opposite sides that extend a greater distance internally towards the center of the scope than two other opposite sides.

13. The hysteroscopy system of claim **10**, wherein the sheath has an outer diameter of about 5.6 millimeters and a long diameter of the scope is about 5.15 millimeters.

14. The hysteroscopy system of claim **10**, wherein the sheath further includes a plurality of outflow holes near the distal flange.

15. The hysteroscopy system of claim **10**, further comprising a visualization channel formed within the internal surface of the scope.

16. The hysteroscopy system of claim **15**, further comprising a visualization device inserted within the visualization channel.

* * * * *

专利名称(译)	宫腔镜系统		
公开(公告)号	US9155454	公开(公告)日	2015-10-13
申请号	US12/892355	申请日	2010-09-28
[标]申请(专利权)人(译)	史密夫和内修有限公司		
申请(专利权)人(译)	施乐辉 , INC.		
当前申请(专利权)人(译)	施乐辉 , INC.		
[标]发明人	SAHNEY MIRA SHENER IRMAKOGLU CEMAL		
发明人	SAHNEY, MIRA SHENER-IRMAKOGLU, CEMAL		
IPC分类号	A61B1/00 A61B1/307 A61B1/018 A61B17/32 A61M5/00 A61B1/12 A61B17/34 A61B1/015 A61B1/303		
CPC分类号	A61B1/015 A61B1/00135 A61B1/018 A61B1/307 A61B17/3421 A61B17/32002 A61B2217/007 A61B1/303 A61B2017/320024 A61B2017/320028 A61B17/3205 A61B17/42 A61B2017/320052 A61B2017/4216 A61B1/00142		
代理机构(译)	尼克松皮博迪律师事务所		
其他公开文献	US20120078038A1		
外部链接	Espacenet USPTO		

摘要(译)

一种子宫镜检查系统，包括具有内部通道的窥视镜，可拆卸地连接到窥视镜的护套和流出通道。护套具有远端凸缘，该远端凸缘在内部朝向窥视镜的外表面延伸。流出通道形成在护套的内表面和窥视镜的外表面之间。远端凸缘形成流出通道的远端，并且通常位于窥视镜和护套之间。

