



US 20110087267A1

(19) **United States**

(12) **Patent Application Publication**

Spivey et al.

(10) **Pub. No.: US 2011/0087267 A1**

(43) **Pub. Date: Apr. 14, 2011**

(54) **METHOD FOR EXCHANGING END EFFECTORS IN VIVO**

(76) Inventors: **James T. Spivey**, Cincinnati, OH (US); **Kevin M. Huey**, Cincinnati, OH (US); **Rudolph H. Nobis**, Mason, OH (US); **Sean P. Conlon**, Loveland, OH (US)

(21) Appl. No.: **12/576,578**

(22) Filed: **Oct. 9, 2009**

**Publication Classification**


(51) **Int. Cl.**

*A61B 17/29* (2006.01)  
*A61B 17/94* (2006.01)

(52) **U.S. Cl. .... 606/205; 606/1**

(57) **ABSTRACT**

A laparoscopic surgical method comprises obtaining a first instrument comprising an elongate shaft with a distal end and a proximal end connected to a first handle. The distal end of the first instrument is passed through a percutaneous incision. A surgical end effector is obtained having a distal end with operable jaws and a proximal end selectively attachable to and detachable from the distal end of the first instrument. A second instrument is obtained comprising a distal end and a proximal end connected to a second handle. The surgical end effector is loaded ex vivo on the distal end of the second instrument. The distal end of the second instrument with the loaded surgical end effector is passed through a second incision spaced from the percutaneous incision. The proximal end of the surgical end effector is attached in vivo to the distal end of the first instrument. Tissue is manipulated by actuating the handle of the first instrument to operate the jaws of the surgical end effector.

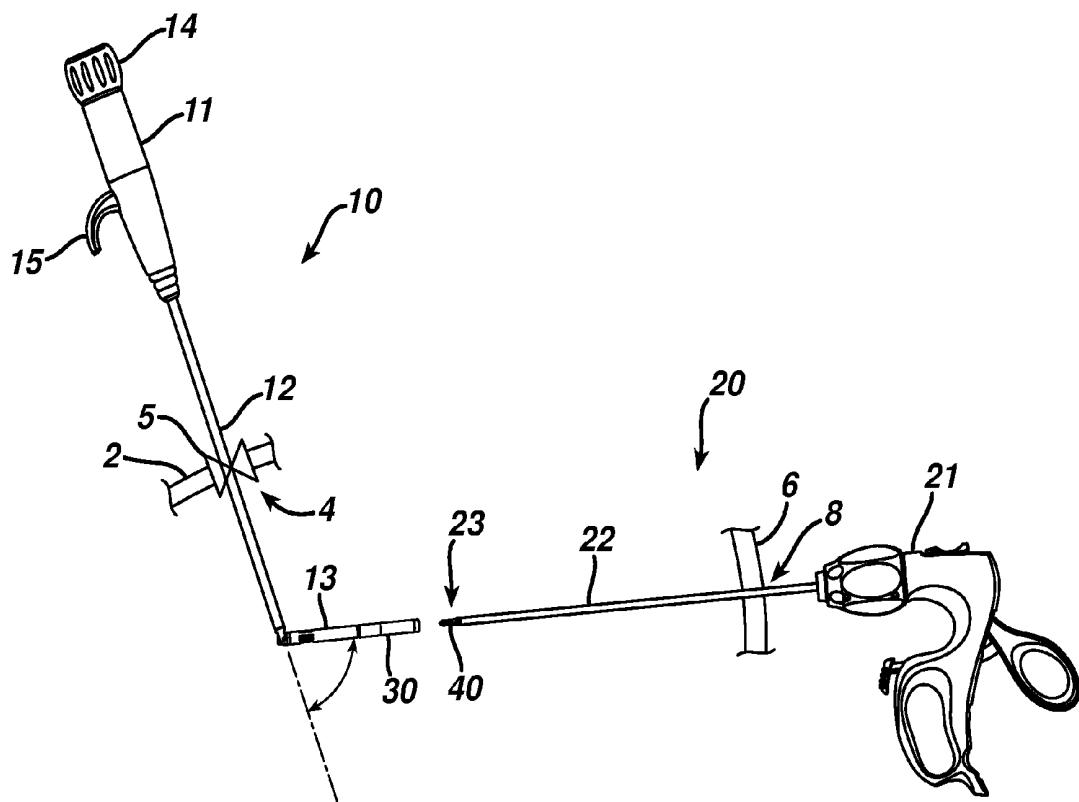

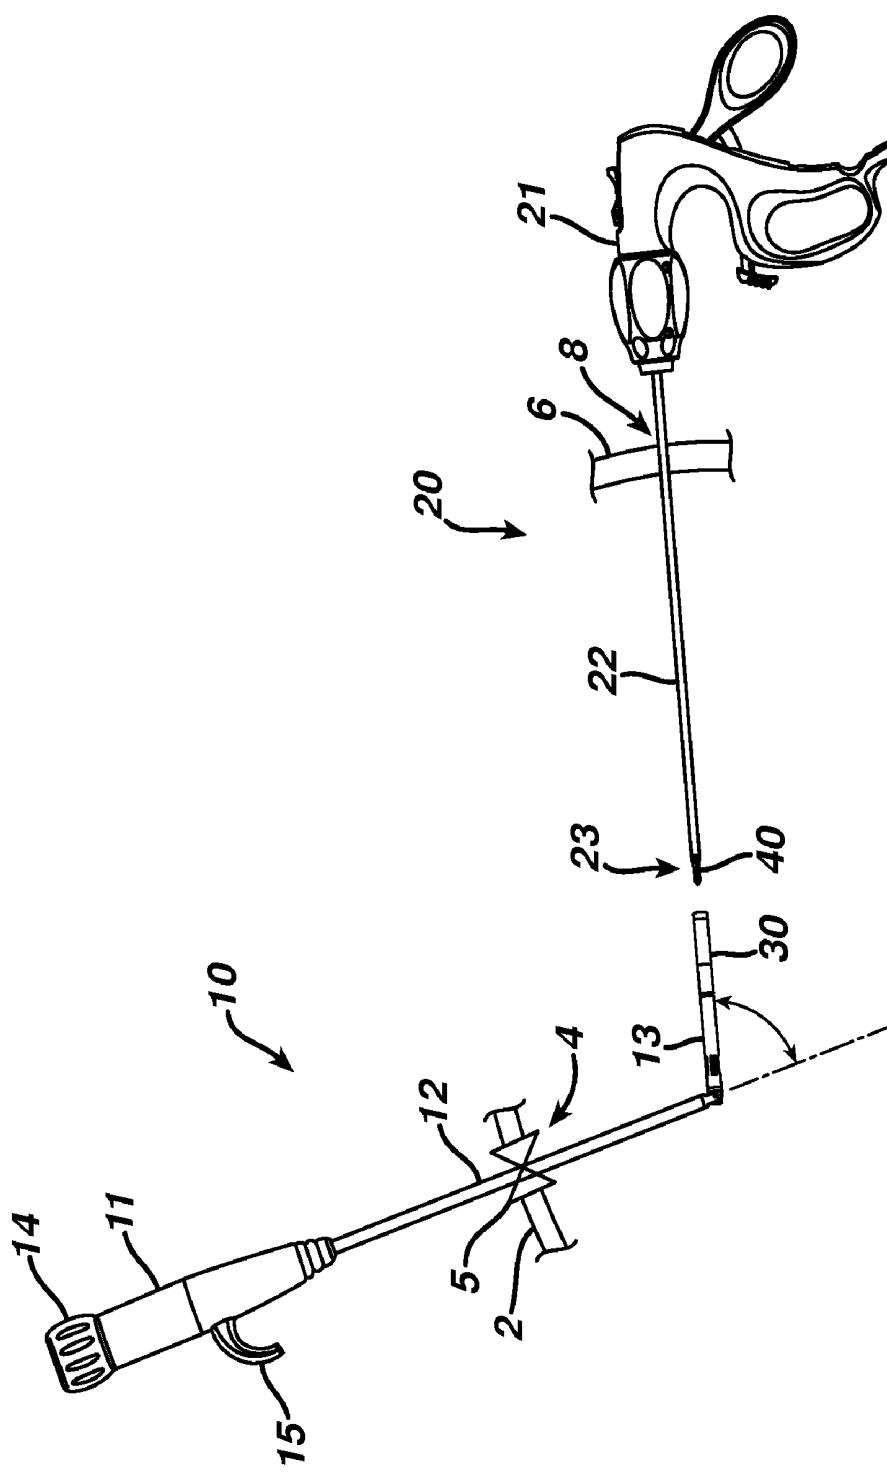


FIG. 1



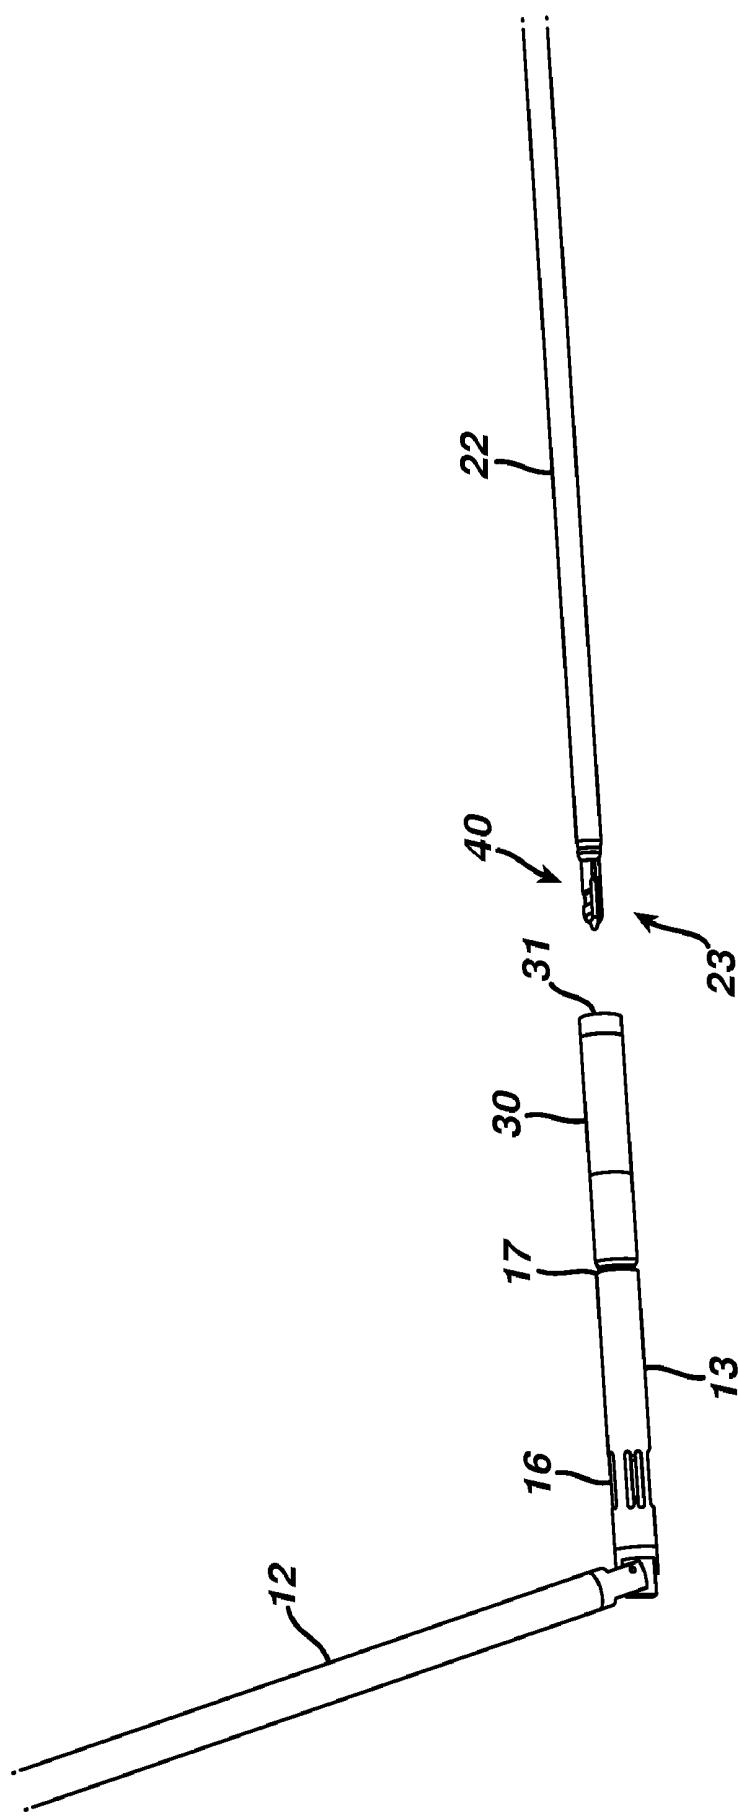



FIG. 2

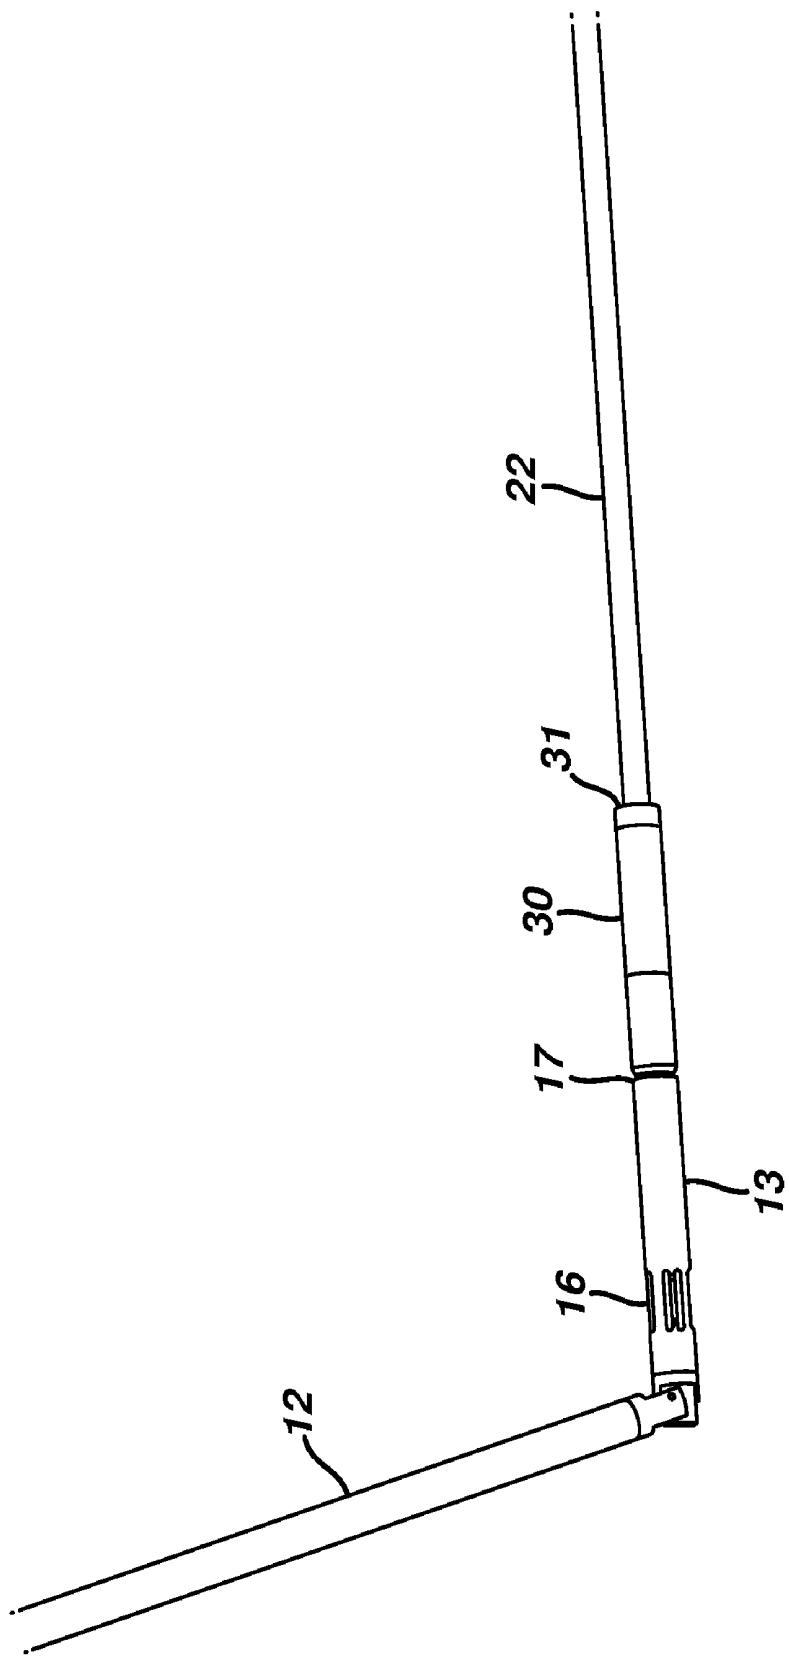

**FIG. 3**

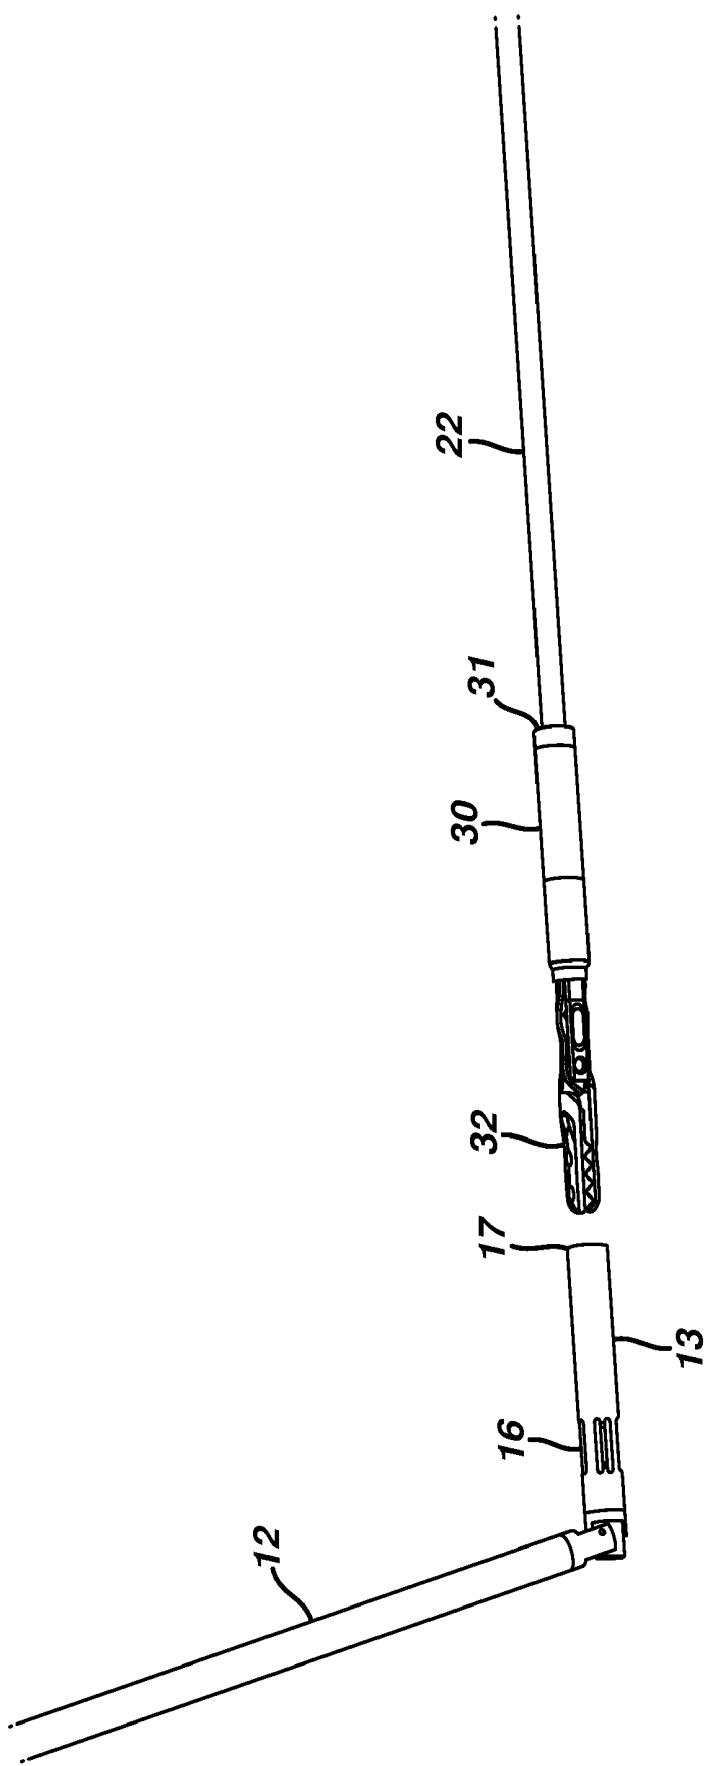



**FIG. 4**

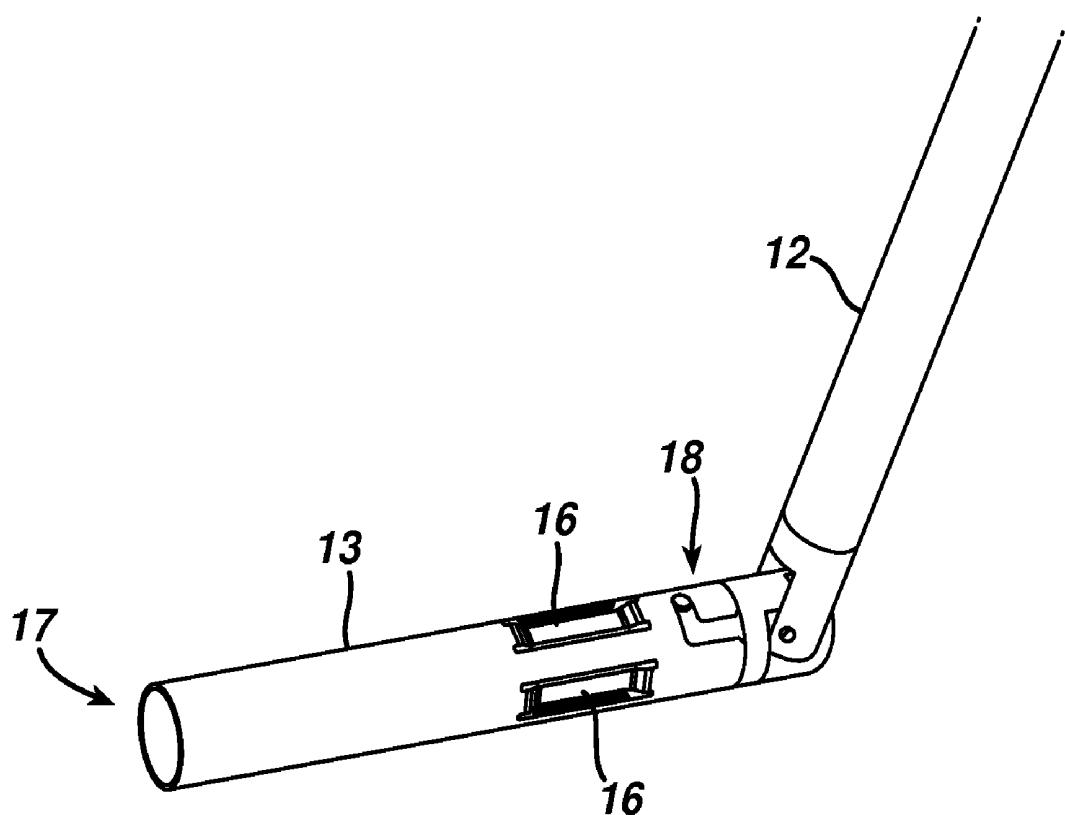


**FIG. 4A**


FIG. 5

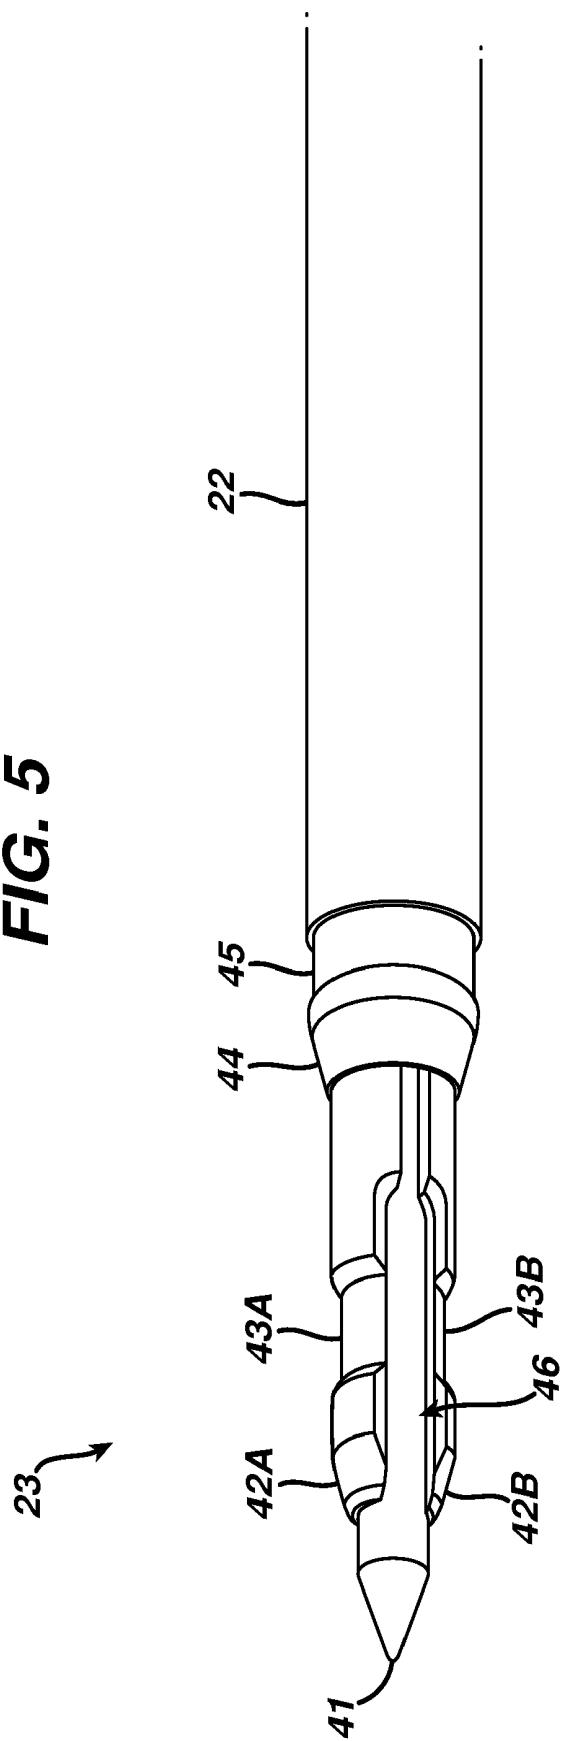

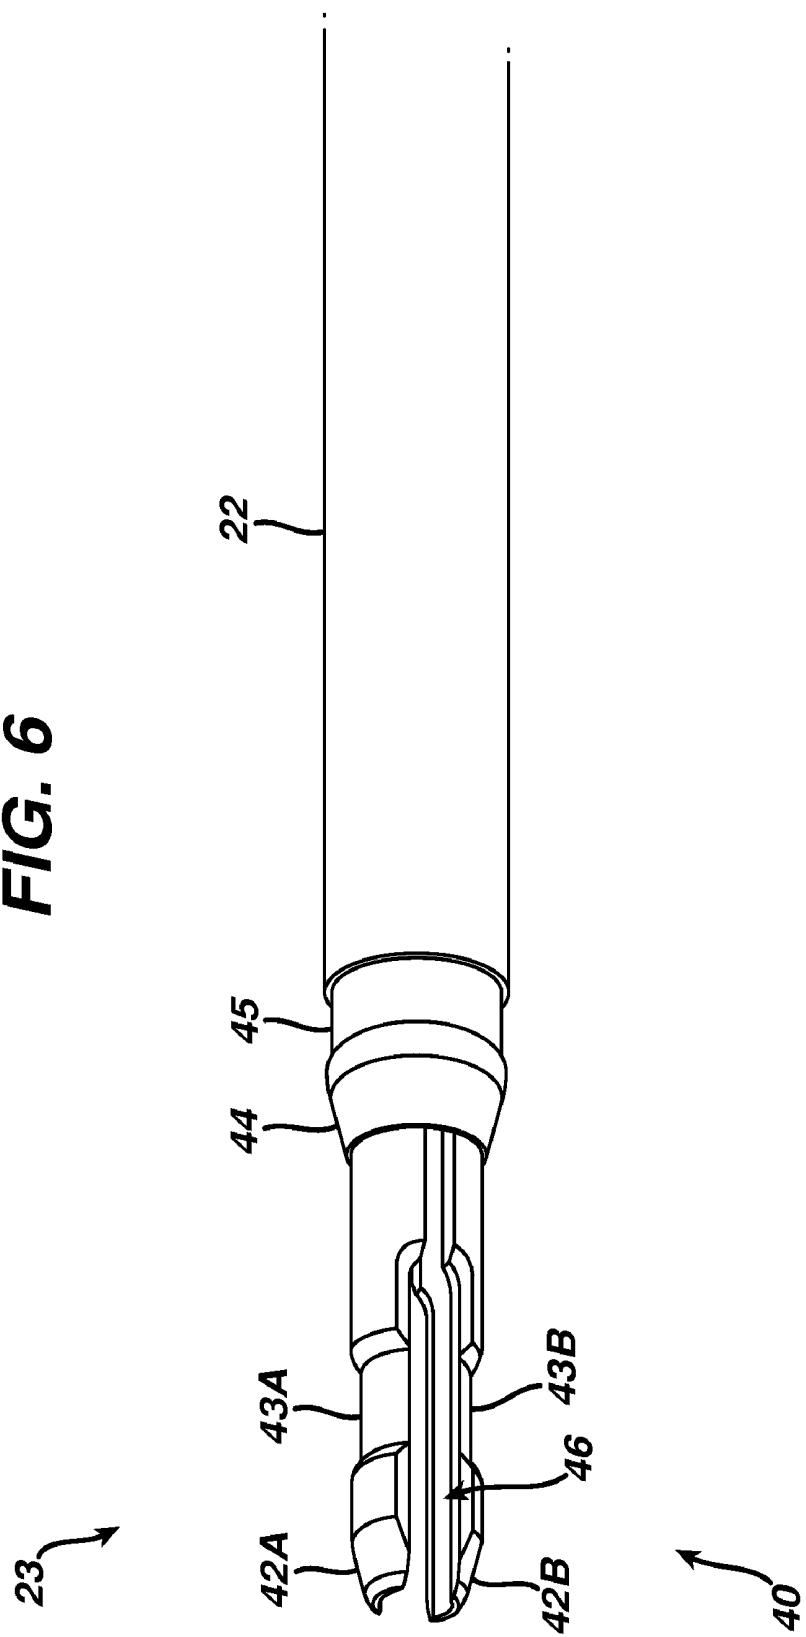
**FIG. 6**




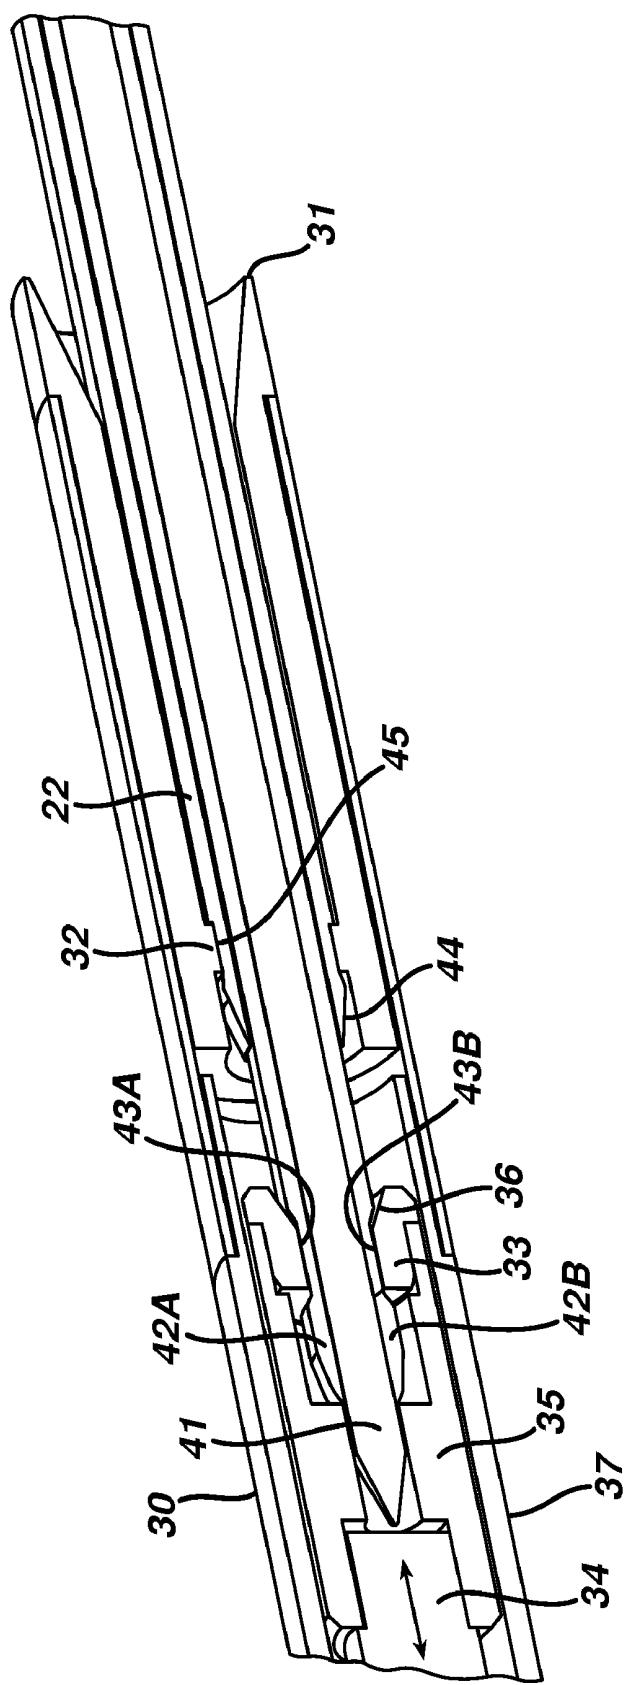
**FIG. 7**

**FIG. 8**

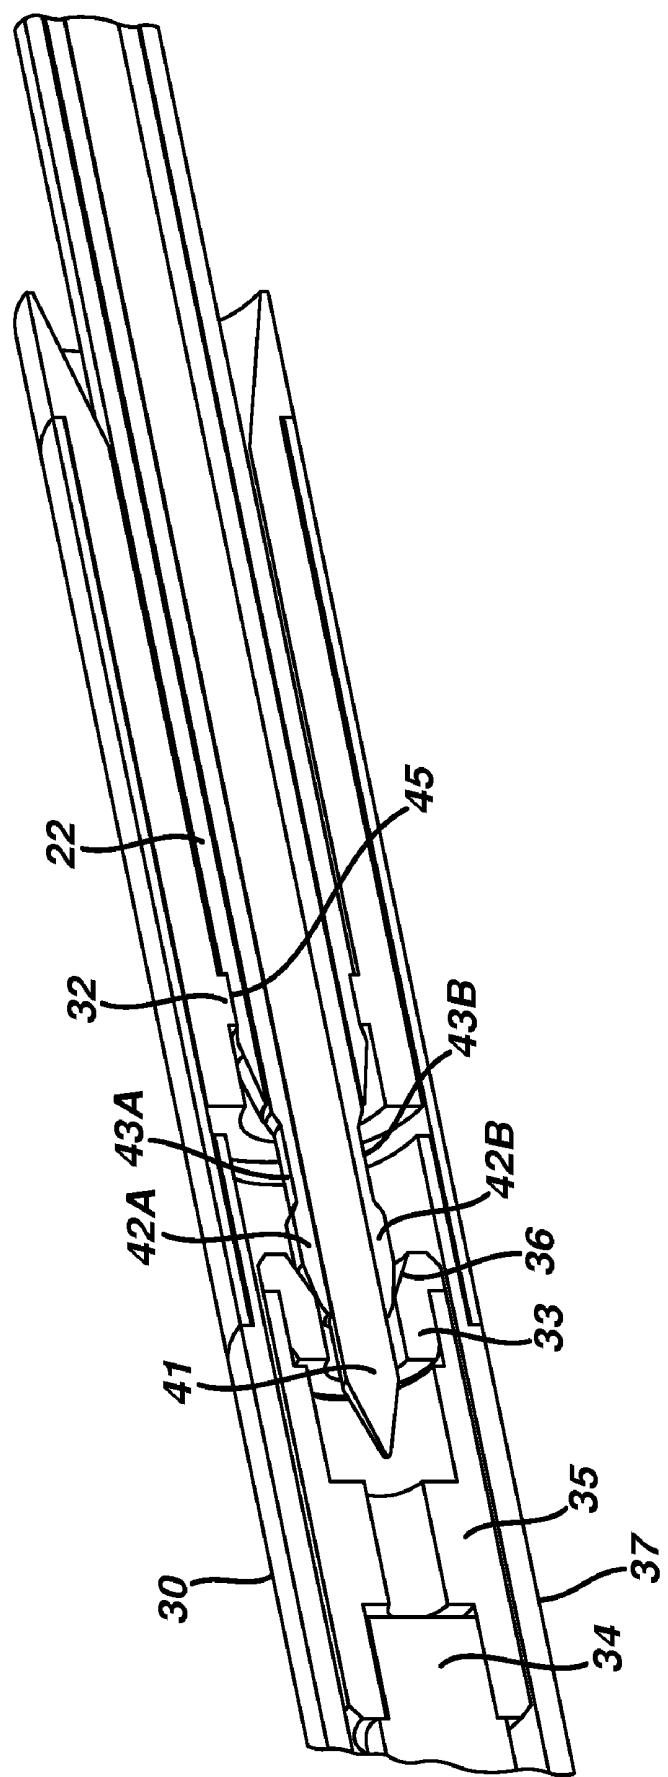

**FIG. 9**

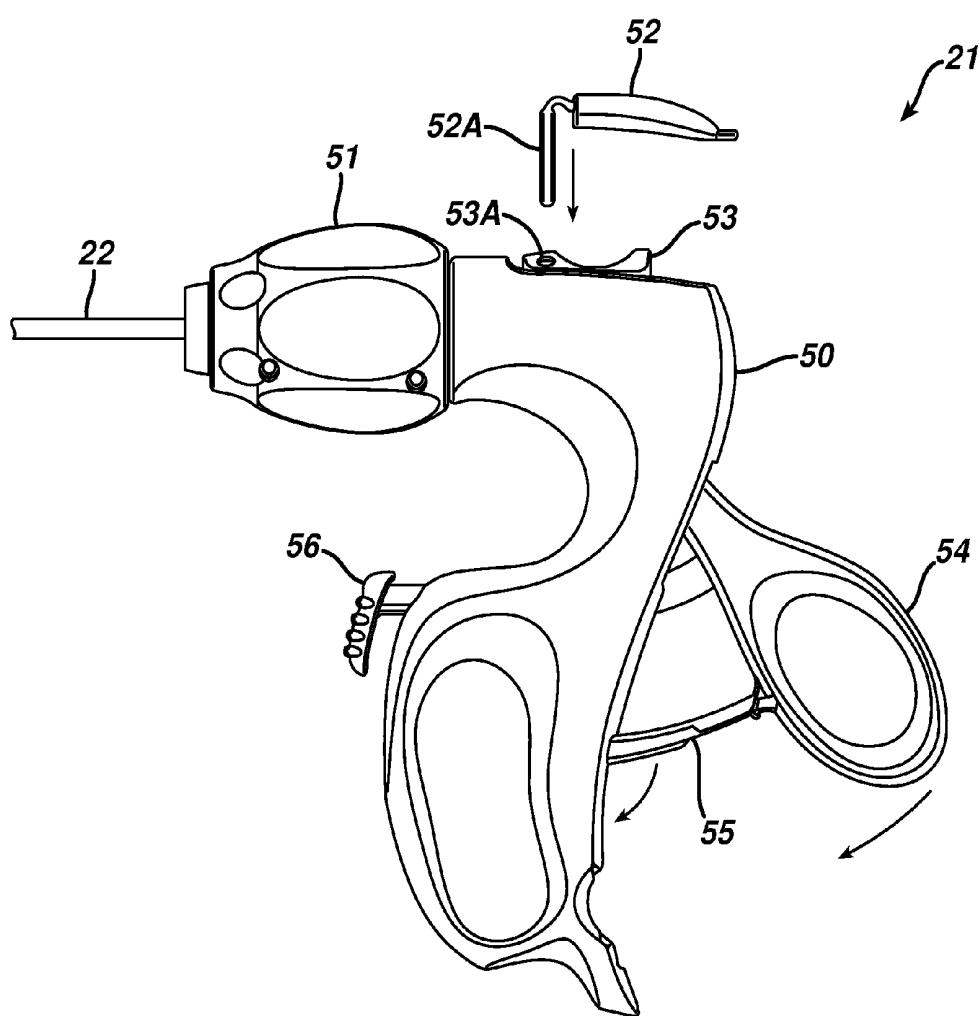

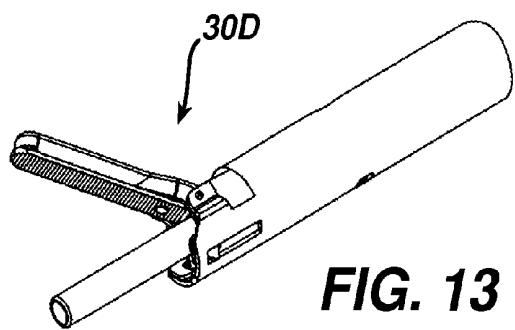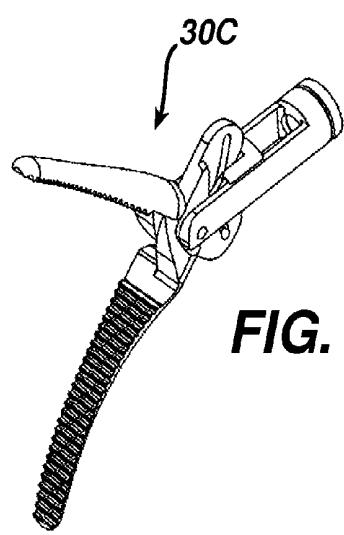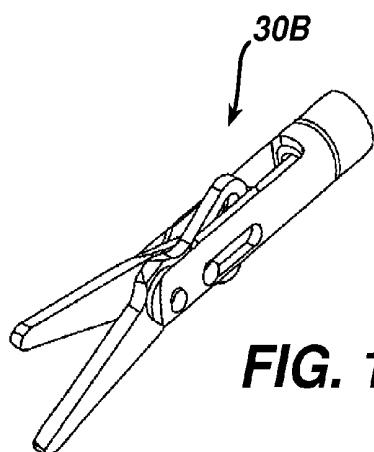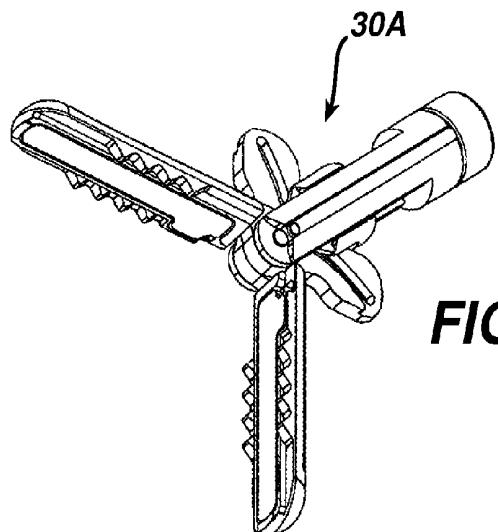

## METHOD FOR EXCHANGING END EFFECTORS IN VIVO

### BACKGROUND

[0001] The present invention relates in general to surgical devices and procedures, and more particularly to minimally invasive surgery.

[0002] Surgical procedures are often used to treat and cure a wide range of diseases, conditions, and injuries. Surgery often requires access to internal tissue through open surgical procedures or endoscopic surgical procedures. The term "endoscopic" refers to all types of minimally invasive surgical procedures including laparoscopic, arthroscopic, natural orifice intraluminal, and natural orifice transluminal procedures. Endoscopic surgery has numerous advantages compared to traditional open surgical procedures, including reduced trauma, faster recovery, reduced risk of infection, and reduced scarring. Endoscopic surgery is often performed with an insufflatory fluid present within the body cavity, such as carbon dioxide or saline, to provide adequate space to perform the intended surgical procedures. The insufflated cavity is generally under pressure and is sometimes referred to as being in a state of pneumoperitoneum. Surgical access devices are often used to facilitate surgical manipulation of internal tissue while maintaining pneumoperitoneum. For example, trocars are often used to provide a port through which endoscopic surgical instruments are passed. Trocars generally have an instrument seal, which prevents the insufflatory fluid from escaping while an instrument is positioned in the trocar.

[0003] While surgical access devices are known, no one has previously made or used the surgical devices and methods in accordance with the present invention.

### BRIEF DESCRIPTION OF DRAWINGS

[0004] While the specification concludes with claims which particularly point out and distinctly claim the invention, it is believed the invention will be better understood from the following description taken in conjunction with the accompanying drawings illustrating some non-limiting examples of the invention. Unless otherwise indicated, the figures are not necessarily drawn to scale, but rather to illustrate the principles of the invention.

[0005] FIG. 1 depicts surgical procedure with an instrument and loader holding an end effector;

[0006] FIG. 2 depicts a close-up view of the distal ends of the instrument and loader in FIG. 1;

[0007] FIG. 3 depicts an instrument being inserted into an end effector;

[0008] FIG. 4 depicts an instrument attached to an end effector being withdrawn from a loader;

[0009] FIG. 4A depicts a loader with removable distal end;

[0010] FIG. 5 depicts an isometric close-up view of the distal end of an instrument in a locked position;

[0011] FIG. 6 depicts an isometric close-up view of the distal end of an instrument in an unlocked position;

[0012] FIG. 7 depicts an isometric cross-sectional view of the distal end of an instrument attached to an end effector;

[0013] FIG. 8 depicts an isometric cross-sectional view of the distal end of an instrument attached to an end effector in a pushed-off configuration;

[0014] FIG. 9 depicts an instrument handle;

[0015] FIG. 10 depicts a bi-polar jawed end effector;

- [0016] FIG. 11 depicts a cutting shears end effector;
- [0017] FIG. 12 depicts a Maryland dissector end effector; and
- [0018] FIG. 13 depicts an ultrasonic shears end effector;

### DETAILED DESCRIPTION

[0019] As shown in FIG. 1, instrument (20) comprises an elongate shaft (22) passing through an incision (8) of a tissue wall (6). A loader (10) comprises an elongate shaft (12) passing through an incision (4) of a tissue wall (2). The surgical end effector (30) is selectively attachable in vivo and detachable in vivo to the attachment mechanism (40) located at the distal end (23) of the instrument (20). In this example, the end effector is a jawed tissue grasper, but a variety of other end effectors could be also be used. The end effector (30) may be loaded ex vivo into the distal end (13) of the shaft (12), and then introduced into the surgical field through the incision (4). The loader (10) holds the end effector (30) during the in vivo attachment to and in vivo detachment from the instrument (20). The loader (10) and instrument (20) each includes ex vivo handles (11, 21) attached to the proximal ends of the shafts (12, 22) that enable surgeons to use the devices.

[0020] The tissue wall (2, 6) anatomies will vary based on the surgical procedure, but some non-limiting examples include percutaneous incisions into the abdomen, thorax, or pelvis. The incisions (4, 8) may be created with a cutting or puncturing instrument, and will typically be spaced from one another. The tissue walls (2, 6) may be the same or different anatomies. For instance, tissue walls (2, 6) may both be the abdominal wall. In another example, tissue wall (2) could be an organ (e.g., stomach, colon, esophagus, etc.) accessed through a natural orifice, while the incision (8) in tissue wall (6) could be percutaneous. In yet another example, incision (4) may provide access to the abdomen, while the incision (8) may provide access to the pelvis. If pneumoperitoneum is desired, the incisions may include instrument seals, such as those commonly found in trocars. In this example, the instrument seal (5) is schematically shown in incision (4) with the loader (10) passing through the seal (5), while the shaft (22) seals directly with the tissue wall (6) by virtue of the resilience of the tissue without the aid of a sealing device.

[0021] The loader shaft (12) in this embodiment is rigid and straight, but the shaft (12) could be curved or flexible, which would be beneficial for natural orifice transluminal introduction of the distal end (13) to the surgical field. The loader (10) may include an articulating distal end (13) controlled by the knob (14). The distal end (13) will typically be introduced and removed through the incision (4) in-line with the shaft (12), and then articulated in vivo to facilitate alignment between the end effector (30) and the shaft (22). The arm (15) is rigidly connected to the handle (11) to facilitate grasping of the handle and rotational orientation of the articulated distal end (13) about the shaft (12) axis. In this embodiment, the distal end (13) of the loader (10) comprises a tube opening at the distal tip (17). The tube is dimensioned to receive the end effector (30). The tube (30) includes an engagement feature (16) for holding the end effector (30). While the engagement feature (16) may vary, in this embodiment a plurality of leaf springs provide an interference fit with the end effector (30) to frictionally hold the end effector in the tube. In this embodiment, when the end effector (30) is loaded in the tube, the distal end (32) is positioned in the tube and the proximal end (31) extends from the tube opening (17). This arrangement prevents the jaws of the end effector from opening. After the

distal end (23) of the instrument (20) is attached to the proximal end (31) of the end effector (30), the end effector (30) can be pulled from the distal end (13) of the loader (10).

[0022] FIG. 4A depicts an alternative embodiment of a loader (10) where the distal end (13) is selectively attachable and detachable to the shaft (12). As shown in this example, this feature is enabled with a bayonet connection (18), but other connections are also contemplated including snap connections, threaded connections, and the like. One advantage of this alternative embodiment is that different distal end (13) configurations may be used to hold end effectors that may not be accommodated by a single sized tube.

[0023] FIGS. 5 and 6 depict a detailed view of one embodiment of an attachment mechanism (40) located at the distal end (23) of the shaft (22). The attachment mechanism (40) comprises a mating feature on the shaft (22), which in this embodiment is a circumferential groove (45) positioned on the lateral surface of the shaft (22). The attachment mechanism (40) also comprises arms (42A, 42B) projecting distally from the distal end (44) of the shaft (22). The arms are axially slideable relative the shaft (22) and are resiliently deflectable medially into the gap (46). The arms each comprise a mating feature, which in this embodiment comprises a stepped lateral notch (43A, 43B). An elongate pin (41) is positioned medially relative the arms (42) and is axially slideable relative the arms (42) between a locked position preventing medial deflection of the arms (an example of which is shown in FIG. 5) and an unlocked position allowing medial deflection of the arms (an example of which is shown in FIG. 6). The pin (41) and arms (42) may each slide independently relative the shaft (22).

[0024] As shown in the embodiment of FIG. 5, the elongate pin (41) may include a pointed obturator tip. In this configuration the distal end (23) may be used to puncture through the tissue wall (6). The distal ends of the arms (42) and distal end (44) of the shaft (22) include tapered surfaces to facilitate passing through the incision (8).

[0025] FIG. 7 shows the attachment mechanism (40) attached to the end effector (30). The groove (45) of the shaft (22) mates the rib (32) of the end effector (30) preventing relative axial motion. The lateral grooves (43) of the arms (42) mate the ring (33) of the end effector (30) preventing relative axial motion. The rib (32) is rigidly connected to the outer housing (37) of the end effector (30), and the ring (33) is rigidly connected to the jaw actuator (34) via the coupling (35). Accordingly, axial movement of the arms (42) relative the shaft (22) will cause axial movement of the jaw actuator (34) relative the housing (37), thereby causing the jaws to open and close.

[0026] The following describes one method for attaching the end effector (30) to the shaft (22). The distal end (23) is introduced into the proximal end (31) of the end effector (30) with the pin (41) in the unlocked position. As the arms (42) are advanced axially into the end effector (30), the chamfered lead (36) of the ring (33) medially deflects the arms (42) until the ring (33) is seated into the lateral notches (43). Simultaneously the shaft (22) advances axially into the end effector (30), and the tapered end (44) aligns the rib (32) to seat into the groove (45). In both cases, the surgeon will feel a tactile "snap" indicating proper engagement. Once fully seated in the end effector (30), the pin (41) may be slid to the locked position thereby attaching the end effector (30) to the instrument (20). Once attached, the surgeon may pull the end effector from the loader (10), and the loader (10) may then be

removed from the surgical field. The surgeon may then manipulate tissue with the end effector (30) as needed for the surgical procedure.

[0027] FIG. 9 shows and example of the handle (21) for the instrument (20). The handle (21) includes a base (50). A knob (51) rotates the attachment mechanism (40) about the axis of the shaft (22), which will also rotate an attached end effector (30). The trigger (54) pivots relative the base (50) causing axial movement of the arms (42) and the pin (41) relative the shaft (22). Operation of the trigger (54) will operate the jaws on an attached end effector (30). The latch (55) pivots relative the base (50) between a locked position (as shown in figure) to prevent operation of the trigger (54) and an unlocked position recessed in the base (50). During seating with the end effector (30), the latch (55) may be locked to maintain the same relative axial spacing of the corresponding mating features (43, 45) as the mating features (33, 32), resulting in resulting in a single "snap" feedback. The trigger lock (56) can lock/unlock the trigger in/from its depressed position. An actuator (53), which in this embodiment is a slider, controls axial movement of the pin (51) relative the arms (42). The distal most position of the actuator (53) relative the base (as shown in the figure) places the pin (51) in its locked position, and the proximal most position places the pin (51) in its unlocked position. The pin lock (52) includes a pin (52A) which when inserted into the hole (53A) maintains the pin (41) and arms (42) in the extended and locked positions as shown in FIG. 5.

[0028] FIGS. 10-13 illustrate some non-limiting examples of alternative end effectors (30A-D) that may attached to the distal end (23) of the instrument (20). In addition to the loader (10) and instrument (20), all or a portion of the end effectors (30, 30A, 30B, 30C, 30D) may be bundled as part of a kit so the surgeon may interchange the attached end effector as needed for a surgical procedure. All the end effectors examples shown here have cooperating jaws; however, non-jawed end effectors could also be employed such as hook knives, snares, and the like. In the case of end effectors that require energy, appropriate energy transmission mechanisms known in the art should be added to the handle (21) and shaft (22). For instance, appropriate electrical connections can be added for the bi-polar forceps end effector (30A). Similarly, an ultrasonic transducer and waveguide can be added for the ultrasonic shears end effector (30D).

[0029] The following describes one method for using the devices during a laparoscopic surgical procedure. An instrument (20) is obtained and passed through incision (8). The incision (8) may be a precutaneous incision formed at least partially by a puncture formed with the obturator on the pin (41) in the configuration shown in FIG. 5. The pin lock (52) and latch (55) may be secured to the slider (53) and trigger (54), respectively. After the puncture, the pin lock (52) may be removed.

[0030] A loader (10) and end effector (30) are obtained. The end effector (30) may be selected from a plurality of end effectors provided in a kit. The end effector (30) is loading ex vivo into the distal end (13) of the loader (10). The distal end (13) of the loader (10) with the loaded end effector (30) is passed through incision (4). The second incision (4) may also be percutaneous incision spaced from the first incision (8), and may include passing the distal end (13) with the loaded end effector (30) through a trocar. The distal end (13) may be articulated to facilitate orientation between the proximal end (31) of the end effector (30) and the attachment mechanism

(40). The actuator (53) is slid proximally to move the pin (41) to its unlocked position. The distal end (23) of the instrument (20) is advanced into the proximal end (31) of the end effector (30) until the respective mating features of the instrument (20) and end effector (30) are engaged. The actuator (53) may then be slid distally thus advancing the pin (41) to its locked position. The end effector (30) has now been attached in vivo to the instrument (20). The end effector (30) may then be pulled from the loader (10) and the latch (55) disengaged from the trigger (54). Tissue is then manipulating by actuating the trigger (54) of the handle (21) to operate the jaws of the end effector (30).

[0031] After completing the surgical procedure, the end effector (30) may be detached from the shaft (22). If previously removed, the loader (10) may be reintroduced through the incision (4) into the surgical field. The distal end (32) of the end effector (30) is seated into the distal end (13) of the loader (10), and the pin (41) moved to its unlocked position. The arms (42) are then proximally withdrawn from the ring (33) and the pin (41) is returned to the locked position. Accordingly, the device will be in the configuration depicted in FIG. 8. Distally advancing the arms (42) will push the ring (33) distally till the rib (32) unseats from the groove (45). This unseating may be facilitated by the jaws of the end effector (30) being held in a closed position by the tube in the loader distal end (13). The distal end (23) may then be withdrawn from the end effector (30) thus detaching the end effector (30) from the instrument (20). The end effector will be held in the loader (10) by virtue of the engagement feature (16). Removal of the loader (10) from the surgical field will remove the end effector (30). A different end effector may then be attached to the instrument (20), or the instrument (20) may be withdrawn from the surgical field.

[0032] Without limitation, the following describe some of the benefits and advantages of the foregoing devices and methods over the prior art. The end effector (30) may have a much larger diameter than the shaft (22); accordingly, the incision (8) can be smaller compared to more traditional laparoscopic instruments resulting in less pain and scarring, and quicker recovery. This also facilitates a small diameter shaft (22) (even less than 3 mm), thus potentially eliminating a trocar in the incision (8). The attachment mechanism (40) provides quick end effector (30) exchanges with the instrument (20), thus decreasing surgical time. The loader (10) also facilitates quick end effector (30) exchanges. A kit of multiple end effectors may reduce instrument costs by consolidating a single shaft (22) and handle (21) for all instruments. Many other benefits will be apparent to those skilled in the art.

[0033] Having shown and described various embodiments and examples of the present invention, further adaptations of the methods and devices described herein can be accomplished by appropriate modifications by one of ordinary skill in the art without departing from the scope of the present invention. Several of such potential modifications have been mentioned, and others will be apparent to those skilled in the art. For instance, the specific materials, dimensions, and the scale of drawings will be understood to be non-limiting examples. Accordingly, the scope of the present invention

should be considered in terms of the following claims and is understood not to be limited to the details of structure, materials, or acts shown and described in the specification and drawings.

1. A laparoscopic surgical method, comprising:
  - a) obtaining a first instrument comprising an elongate shaft with a distal end and a proximal end connected to a first handle;
  - b) passing the distal end of the first instrument through a percutaneous incision;
  - c) obtaining a surgical end effector having a distal end with operable jaws and a proximal end selectively attachable to and detachable from the distal end of the first instrument;
  - d) obtaining a second instrument comprising a distal end and a proximal end connected to a second handle;
  - e) loading ex vivo the surgical end effector on the distal end of the second instrument;
  - f) passing the distal end of the second instrument with the loaded surgical end effector through a second incision spaced from the percutaneous incision;
  - g) attaching in vivo the proximal end of the surgical end effector to the distal end of the first instrument; and
  - h) manipulating tissue by actuating the handle of the first instrument to operate the jaws of the surgical end effector.
2. The laparoscopic surgical method of claim 1, wherein (f) comprises passing the distal end of the second instrument with the loaded surgical end effector through a trocar.
3. The laparoscopic surgical method of claim 1, where the first percutaneous incision is formed at least partially a puncture formed with an obturator on the distal end of the first instrument.
4. The laparoscopic surgical method of claim 1, further comprising, between (f) and (g), articulating the distal end of the second instrument.
5. The laparoscopic surgical method of claim 1, wherein (e) comprises loading ex vivo the surgical end effector on the distal end of the second instrument such that the jaws are prevented from opening.
6. The laparoscopic surgical method of claim 1, wherein (e) comprises loading ex vivo the surgical end effector on the distal end of the second instrument such that the surgical end effector extends distally from the distal end of the second instrument.
7. The laparoscopic surgical method of claim 6, wherein (e) comprises loading ex vivo the surgical end effector on the distal end of the second instrument such that the distal end of the surgical end effector is positioned in the distal end of the second instrument and the proximal end of the surgical end effector extends distally from the distal end of the second instrument.
8. The laparoscopic surgical method of claim 1, wherein (e) comprises obtaining a surgical end effector from a plurality of surgical end effectors each having a distal end with operable jaws and a proximal end selectively attachable to and detachable from the distal end of the first instrument.

\* \* \* \* \*

专利名称(译)	在体内交换末端执行器的方法		
公开(公告)号	<a href="#">US20110087267A1</a>	公开(公告)日	2011-04-14
申请号	US12/576578	申请日	2009-10-09
[标]申请(专利权)人(译)	斯皮维JAMES t HUEY KEVIN中号 NOBIS鲁道尔夫^ h 康伦SEAN P		
申请(专利权)人(译)	斯皮维JAMES t HUEY KEVIN中号 NOBIS鲁道尔夫^ h 康伦SEAN P		
当前申请(专利权)人(译)	斯皮维JAMES t HUEY KEVIN中号 NOBIS鲁道尔夫^ h 康伦SEAN P		
[标]发明人	SPIVEY JAMES T HUEY KEVIN M NOBIS RUDOLPH H CONLON SEAN P		
发明人	SPIVEY, JAMES T. HUEY, KEVIN M. NOBIS, RUDOLPH H. CONLON, SEAN P.		
IPC分类号	A61B17/29 A61B17/94		
CPC分类号	A61B17/29 A61B18/1442 A61B2017/00296 A61B2018/1495 A61B2017/00477 A61B2017/0053 A61B2017/00473		
其他公开文献	US9186203		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

## 摘要(译)

腹腔镜手术方法包括获得包括细长轴的第一器械，细长轴具有远端和连接到第一手柄的近端。第一器械的远端穿过经皮切口。获得外科端部执行器，其具有带有可操作钳口的远端和可选择地附接到第一器械的远端并且可从第一器械的远端拆卸的近端。获得第二器械，其包括远端和连接到第二手柄的近端。外科端部执行器离体装载在第二器械的远端上。具有装载的外科端部执行器的第二器械的远端穿过与经皮切口间隔开的第二切口。外科端部执行器的近端在体内附接到第一器械的远端。通过致动第一器械的手柄来操作组织以操作外科端部执行器的钳口。

