



US007460104B2

(12) **United States Patent**
Rosenberg

(10) **Patent No.:** **US 7,460,104 B2**
(45) **Date of Patent:** **Dec. 2, 2008**

(54) **LAPAROSCOPIC SIMULATION INTERFACE**

4,638,798 A 1/1987 Shelden et al.

(75) Inventor: **Louis B. Rosenberg**, Pleasanton, CA
(US)

(Continued)

(73) Assignee: **Immersion Corporation**, San Jose, CA
(US)

FOREIGN PATENT DOCUMENTS

SU 1124372 11/1984

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 591 days.

(Continued)

(21) Appl. No.: **11/041,992**

OTHER PUBLICATIONS

(22) Filed: **Jan. 26, 2005**

Adelstein, Bernard D. et al., "A High Performance Two Degree-Of-Freedom Kinesthetic Interface", In Human Machine Interfaces for Teleoperators and Virtual Environments, NASA Conference Publication 10071, pp. 108-113, 1991.

(65) **Prior Publication Data**

US 2005/0162383 A1 Jul. 28, 2005

(Continued)

Related U.S. Application Data

Primary Examiner—Prabodh Dharia

(74) *Attorney, Agent, or Firm*—Thelen LLP; David B. Ritchie

(63) Continuation of application No. 09/852,401, filed on May 9, 2001, now Pat. No. 7,023,423, which is a continuation of application No. 08/870,956, filed on Jun. 6, 1997, now Pat. No. 6,246,390, which is a continuation of application No. 08/374,288, filed on Jan. 18, 1995, now Pat. No. 5,731,804.

(57)

ABSTRACT

An apparatus which comprises a manipulandum that is configured as a surgical instrument; a closed loop linkage system which includes a first central member fixedly coupled to a first object coupling and a second central member fixedly coupled to a second object coupling, wherein the first and second object couplings are separately coupled to the manipulandum to allow the manipulandum to be moveable in a plurality of rotary degrees of freedom and an axial degree of freedom; a force feedback system is coupled to the linkage system, wherein the force feedback system selectively applies resistive forces to the manipulandum based on the position of the manipulandum with respect to one or more reference coordinates. In an embodiment, the force feedback system includes an actuator to provide a force to the manipulandum in at least one degree of freedom in response to signals received from a computer system.

(51) **Int. Cl.**
G09G 5/00 (2006.01)

(52) **U.S. Cl.** **345/156**; 345/184


(58) **Field of Classification Search** 345/156-158, 345/161, 162, 179, 184; 318/567; 434/262; 600/1, 167, 139; 227/175.1, 180.1
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,520,060 A 7/1970 Crabtree et al.
3,919,691 A 11/1975 Noll
4,571,834 A 2/1986 Fraser et al.

31 Claims, 10 Drawing Sheets

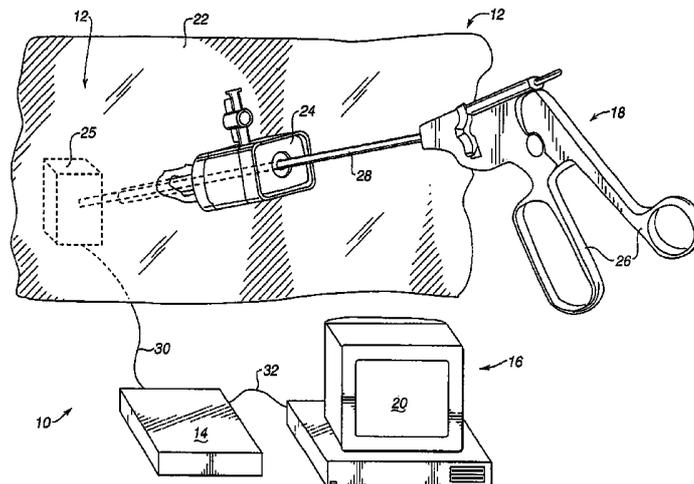

U.S. PATENT DOCUMENTS

4,907,973 A 3/1990 Hon
 5,022,407 A 6/1991 Horch et al.
 5,050,608 A 9/1991 Watanabe et al.
 5,086,401 A 2/1992 Glassman et al.
 5,113,872 A 5/1992 Jahrmarkt et al.
 5,186,629 A 2/1993 Rohen
 5,230,623 A 7/1993 Guthrie et al.
 5,251,127 A 10/1993 Raab
 5,290,276 A 3/1994 Sewell, Jr.
 5,334,017 A 8/1994 Lang et al.
 5,389,865 A 2/1995 Jacobus et al.
 5,397,323 A 3/1995 Taylor
 5,403,191 A 4/1995 Tuason
 5,417,210 A 5/1995 Funda et al.
 5,436,542 A 7/1995 Petelin et al.
 5,445,166 A 8/1995 Taylor
 5,451,924 A 9/1995 Massimino et al.
 5,480,307 A 1/1996 Lang et al.
 5,576,727 A * 11/1996 Rosenberg et al. 345/179
 5,609,485 A 3/1997 Bergman et al.
 5,623,582 A * 4/1997 Rosenberg 700/264
 5,629,594 A * 5/1997 Jacobus et al. 318/568.11
 5,642,469 A * 6/1997 Hannaford et al. 700/264
 5,667,517 A 9/1997 Hooven
 5,701,140 A 12/1997 Rosenberg et al.
 5,720,742 A 2/1998 Zacharias
 5,734,373 A * 3/1998 Rosenberg et al. 345/161
 5,742,278 A 4/1998 Chen et al.
 5,766,016 A 6/1998 Sinclair et al.
 5,767,839 A 6/1998 Rosenberg
 5,805,140 A * 9/1998 Rosenberg et al. 345/161
 5,808,665 A 9/1998 Green
 5,821,920 A 10/1998 Rosenberg et al.
 5,967,980 A 10/1999 Ferre et al.
 6,037,927 A 3/2000 Rosenberg
 6,057,828 A 5/2000 Rosenberg et al.
 6,246,390 B1 6/2001 Rosenberg
 6,620,174 B2 9/2003 Jensen et al.
 6,758,843 B2 7/2004 Jensen
 7,023,423 B2 * 4/2006 Rosenberg 345/161
 7,032,798 B2 * 4/2006 Whitman et al. 227/175.1
 7,061,467 B2 6/2006 Rosenberg
 2001/0020937 A1 * 9/2001 Rosenberg et al. 345/184

2004/0164959 A1* 8/2004 Rosenberg et al. 345/161

FOREIGN PATENT DOCUMENTS

WO WO 91-06935 5/1991

OTHER PUBLICATIONS

Bergamasco, Massimo, "Haptic Interfaces: The Study of Force and Tactile Feedback Systems," IEEE International Workshop on Robot and Human Communication, 1995, pp. 15-20.
 Chen, Elaine Y. et al., "Exos Slip Display Research and Development," DSC-vol. 55-1, Dynamic Systems and Control, vol. , 1994, pp. 265-270.
 Durlach, Nathaniel I. et al., "Virtual Reality: Scientific and Technological Challenges," National Academy Press, Washington, D. C. 1995, pp. 160-205.
 Hon, David, "Ixion's Realistic Medical Simulations" Virtual Reality World, vol. 2, No. 4, Jul./Aug. 1994, pp. 58-62.
 Jackson et al., "Force Feedback and Medical Simulation," Interactive Technology and the New Paradigm, Chapter 24, pp. 147-151, 1995.
 Krueger et al., "The Responsive Workbench," IEEE Computer and Applications, 1994, pp. 12-14.
 Marcus, Beth A. et al., "Making VR Feel Real," in: Proceedings of SRI International Virtual Worlds Conference, Stanford Research Institute, 1991, 7 pages.
 Marcus, Beth, "Touch Feedback in Surgery," Official Proceedings of Virtual Reality and Medicine The Cutting Edge, 1994, pp. 96-97.
 Merrill, Jonathan R. et al., "Virtual Reality for Trade Shows and Individual Physician Training," Medical Applications, 1994, pp. 40-44.
 Rosenberg, Louis B. et al., "Perceptual Decomposition Of Virtual Haptic Surfaces," Proceedings of the IEEE 1993 Symposium on Research Frontiers in Virtual Reality, pp. 46-53, (1993).
 Rosenberg, Louis B., "Virtual Fixtures": Perceptual Overlays Enhance Operator Performance in Telepresence Tasks, Dept. of Mechanical Engineering, Stanford University, Aug. 1994, pp. ii-214.
 Russo, Massimo Andrea, "The Design and Implementation of a Three Degree of Freedom Force Output Joystick," Dept. of Mechanical Engineering, MIT May 1990, 131 pages.
 Satava, Richard M., "The Role of Virtual Reality in Medicine of the 21st Century", Virtual Reality Systems, vol. 1, No. 2, 1994, pp. 64-67.
 Snow et al., "Model-X Force-Reflecting-Hand-Controller", NT Control No. NPO-17851; JPL Case No. 7348, pp. 1-4 with 25 pages of attachments, 1989.
 Tadros, Alfred Heikal, "Control System Design for a Three Degree of Freedom Virtual Environment Simulator Using Motor/Brake Pair Actuators," Dept. of Mechanical Engineering, MIT Feb. 1990, pp. 2-88.
 Taubes, Gary, "Surgery in Cyberspace", Science News Articles Online Technology Magazine Articles, <http://www.discover.com/issues/dec-94>, Dec. 1994, 7 pages.
 Yamakita, M. et al., "Tele Virtual Reality of Dynamic Mechanical Model," Proceedings of the 1992 IEEE/RSJ International Conference on Intelligent Robots and Systems, Jul. 7-10, 1992, pp. 1103-1110.

* cited by examiner

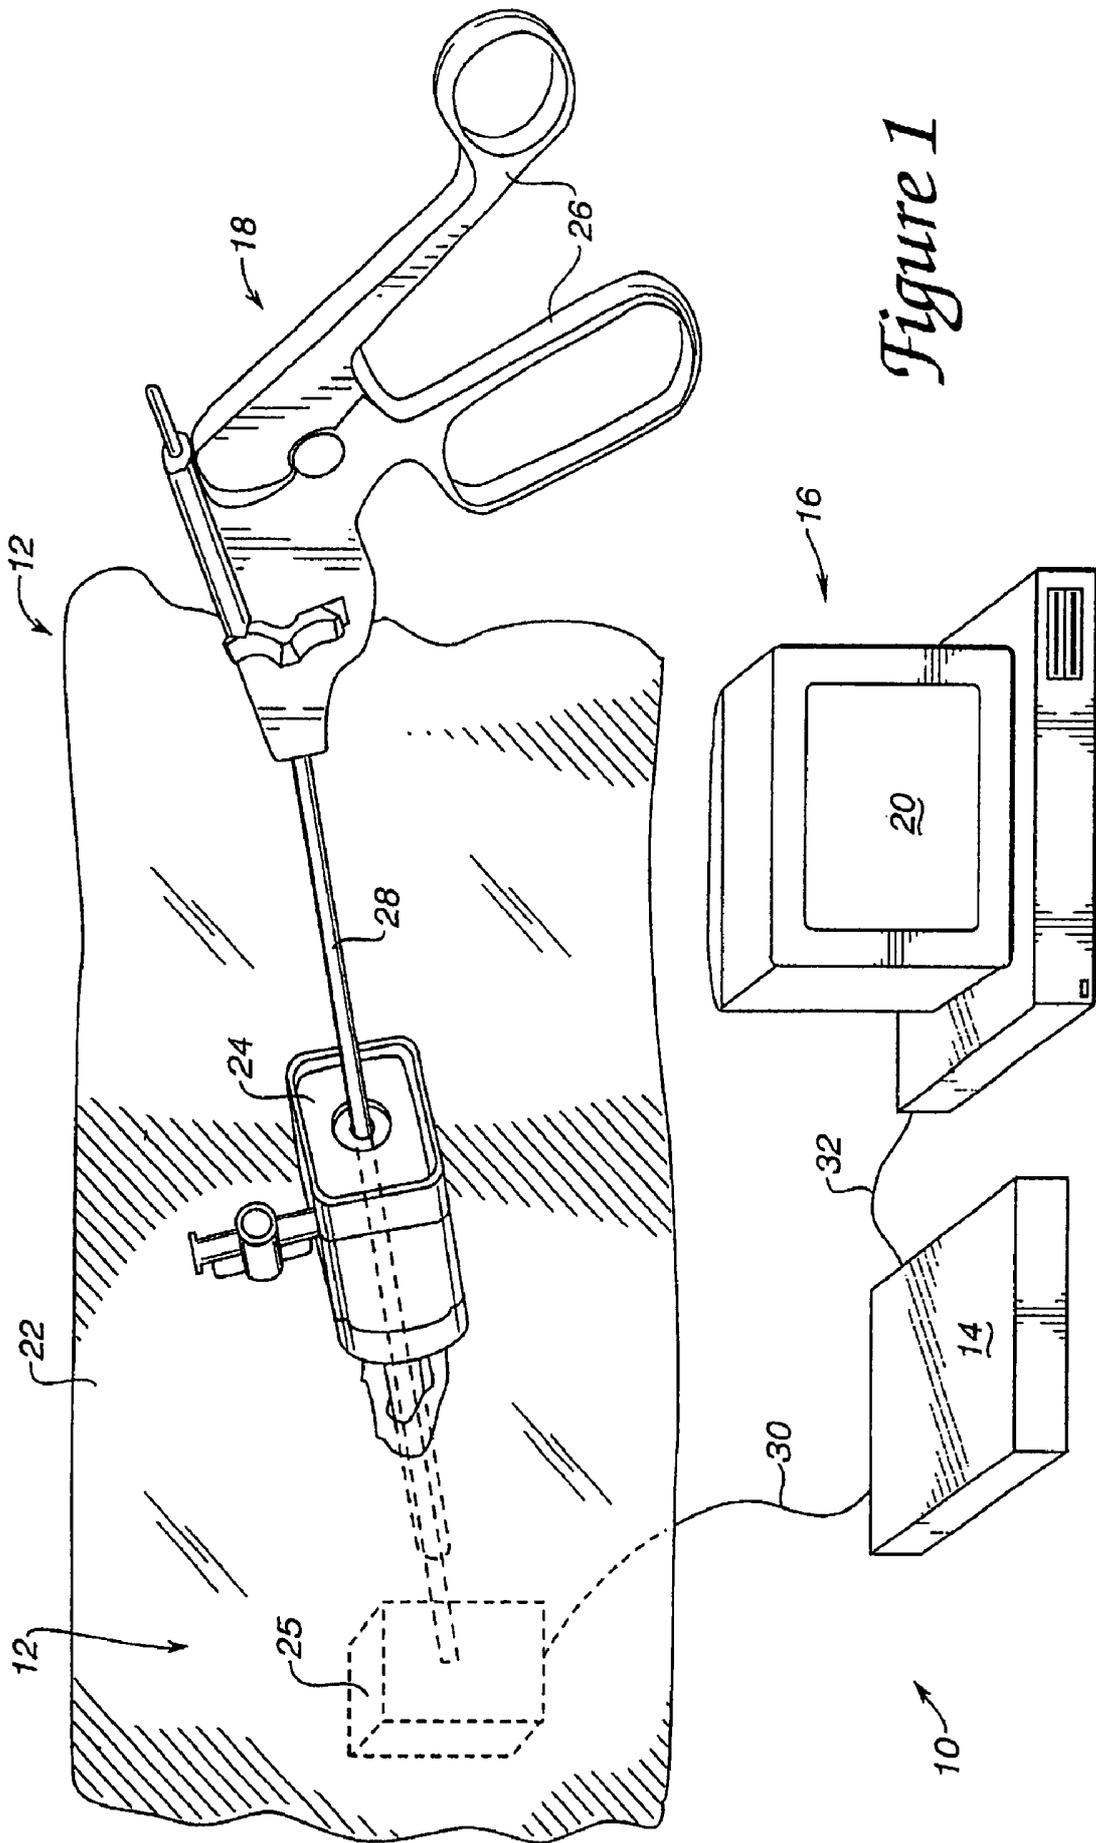


Figure 1

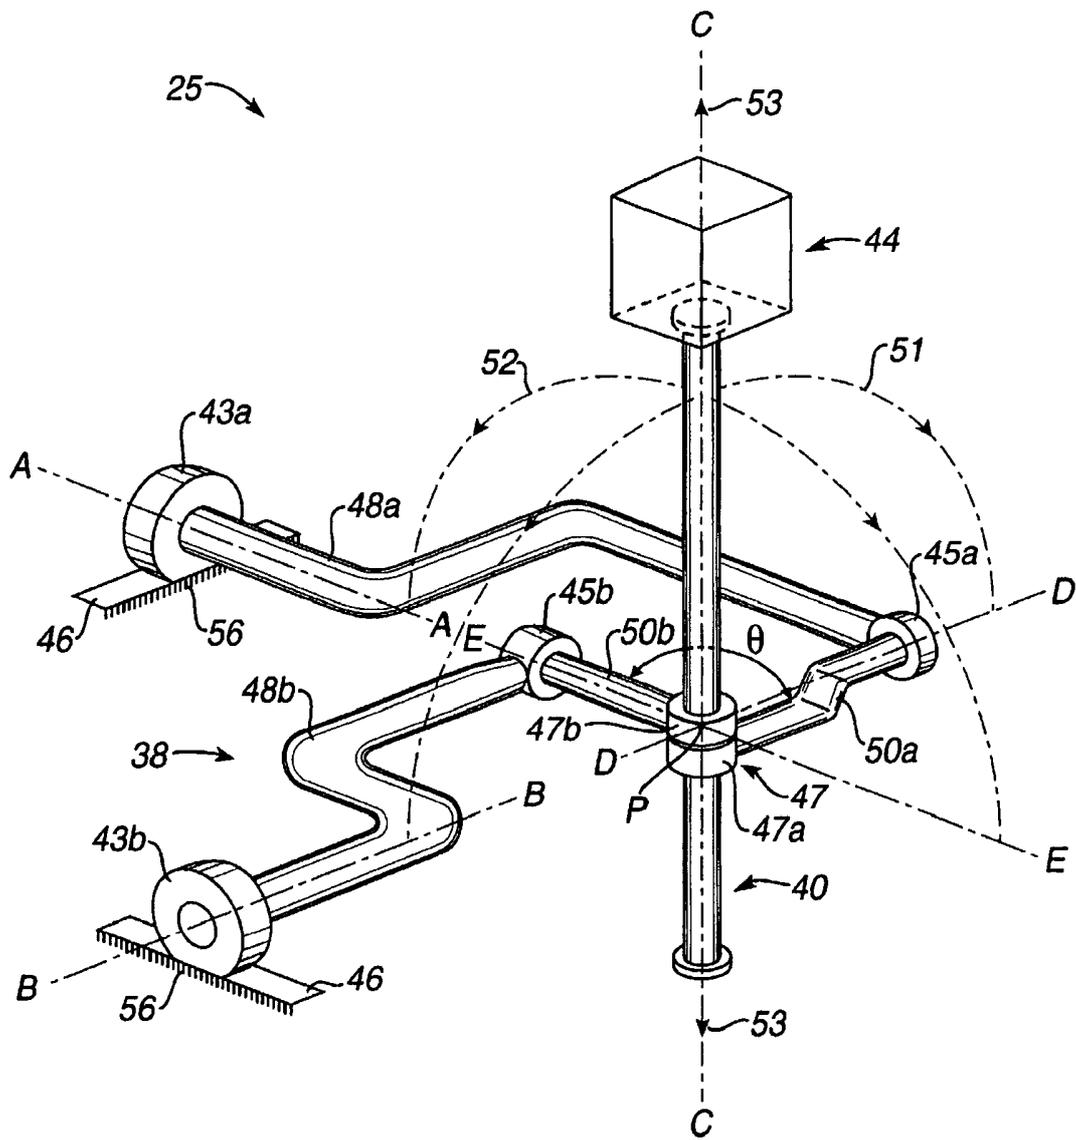
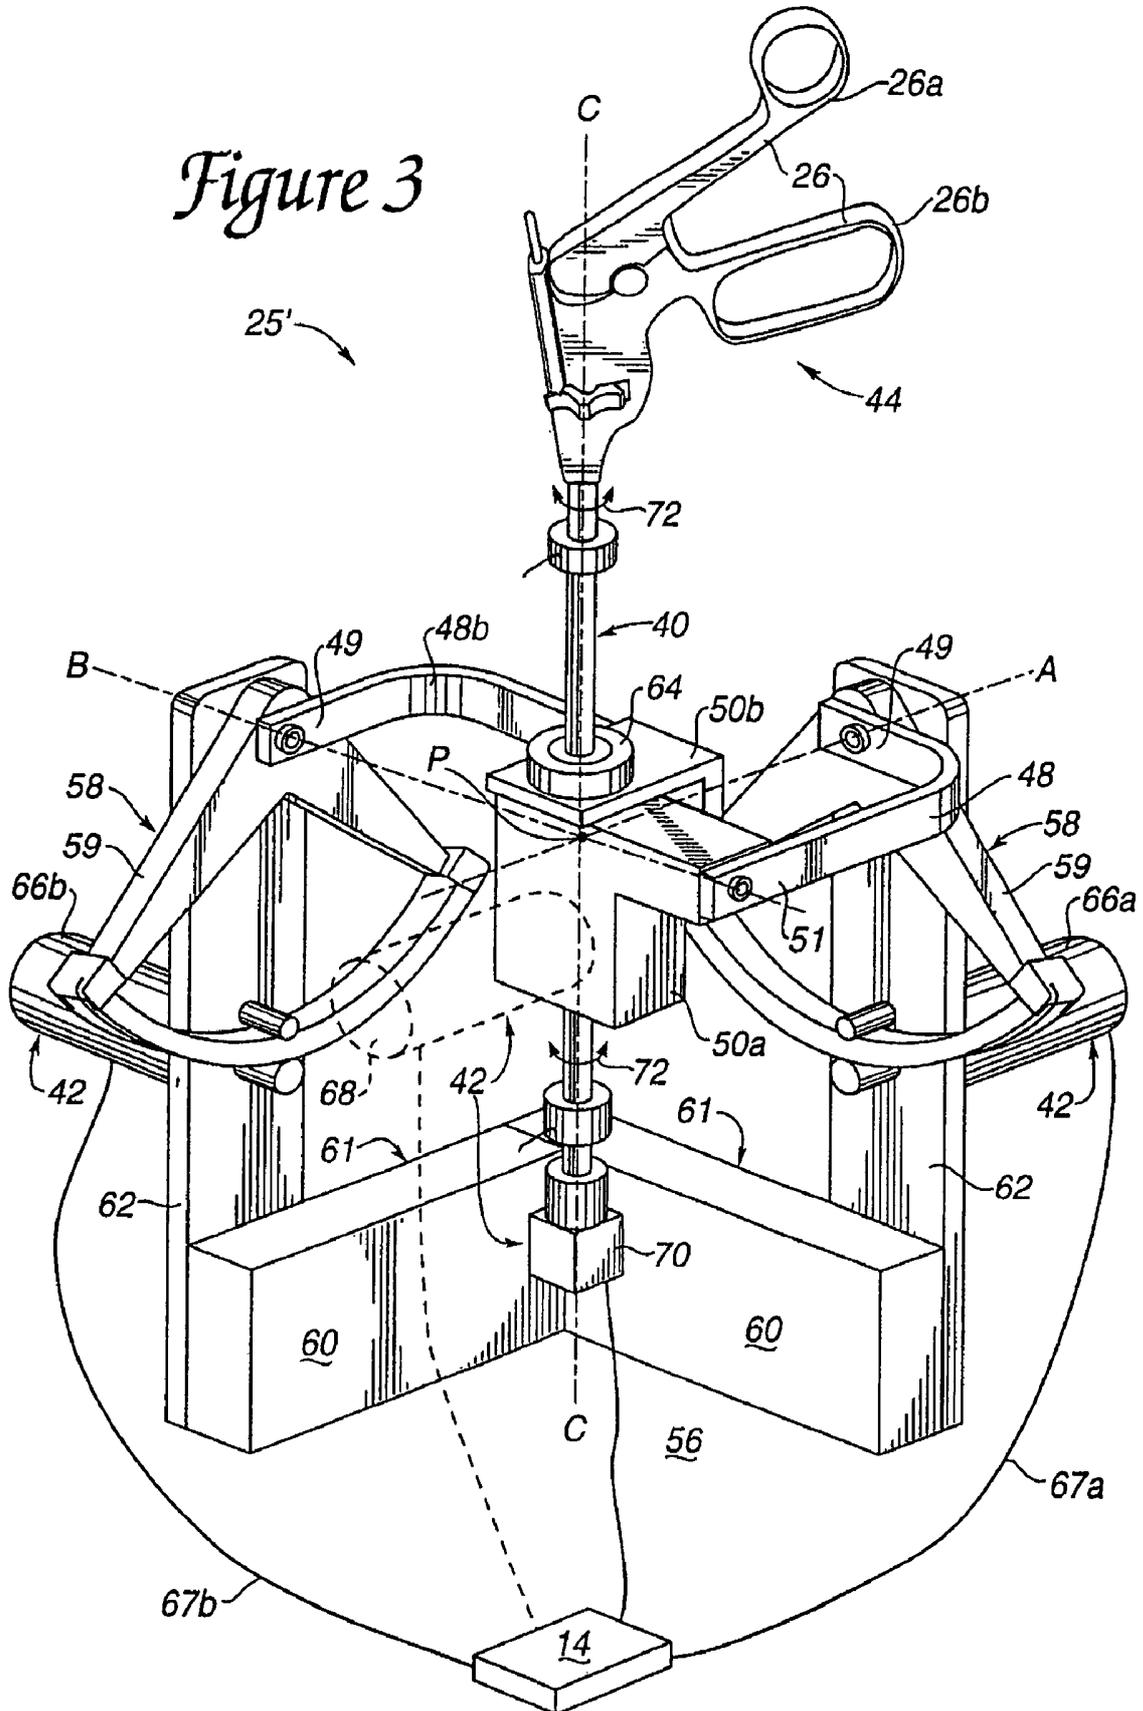


Figure 2

Figure 3



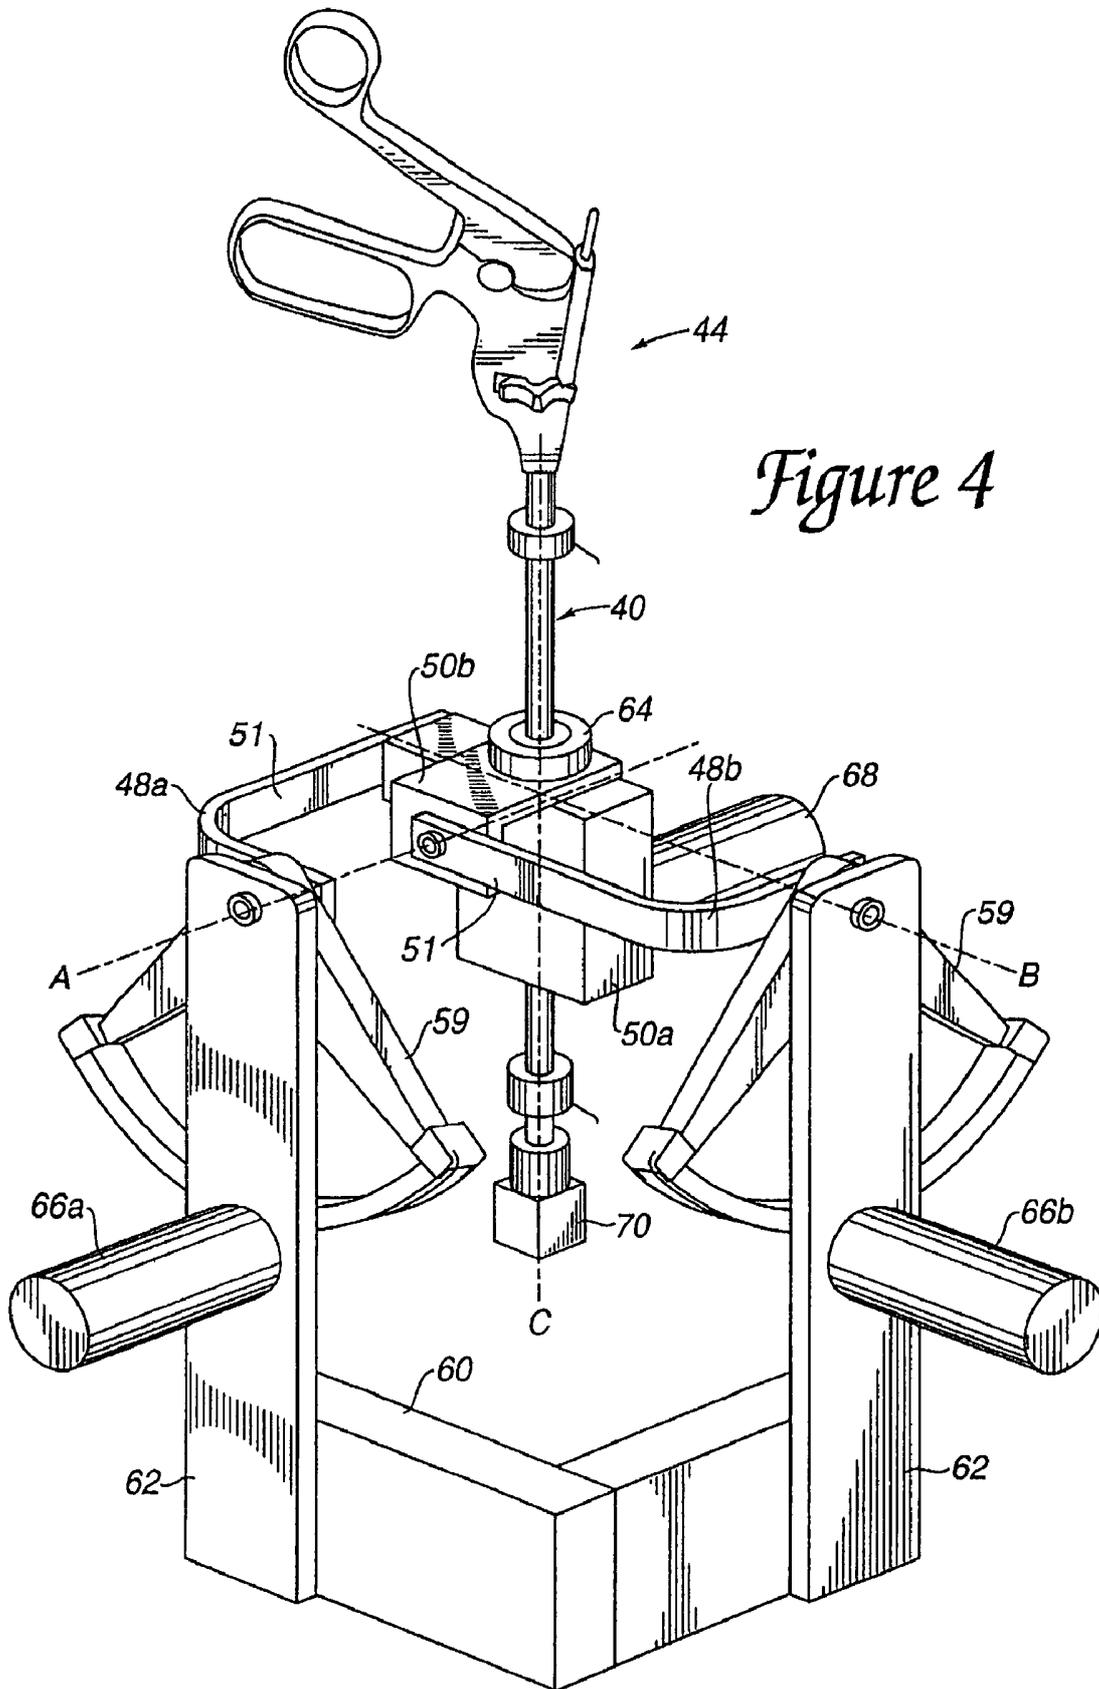
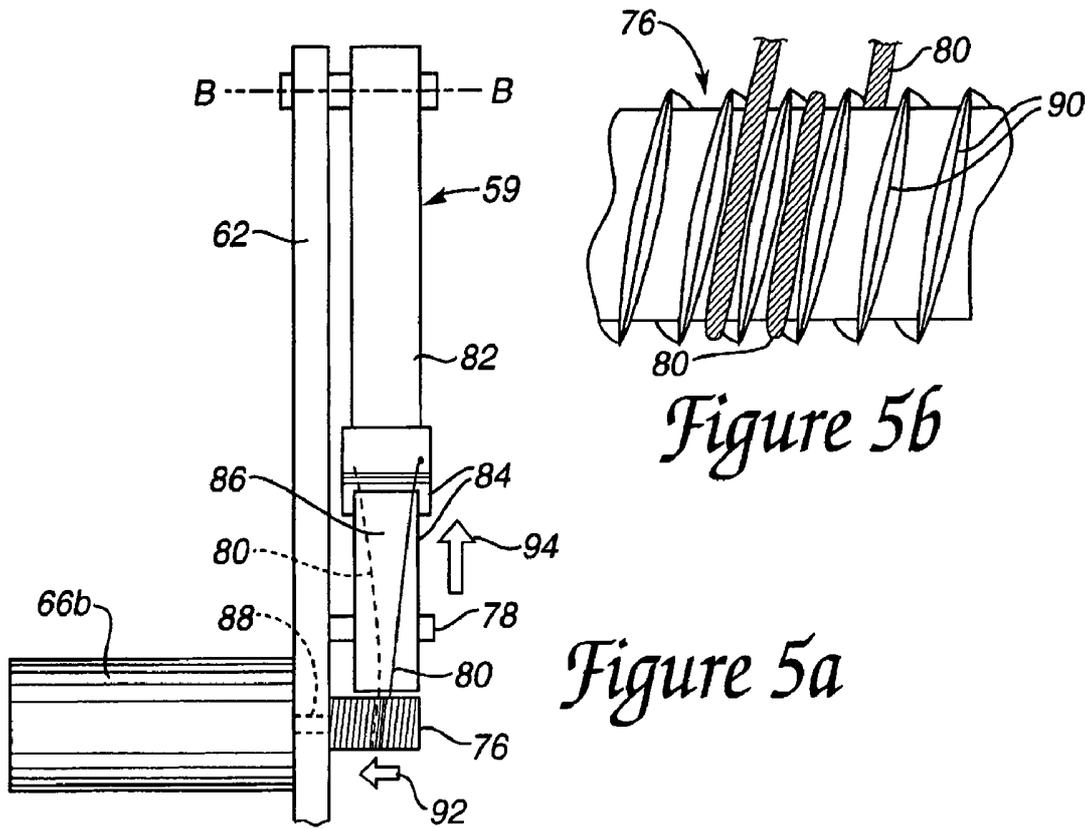
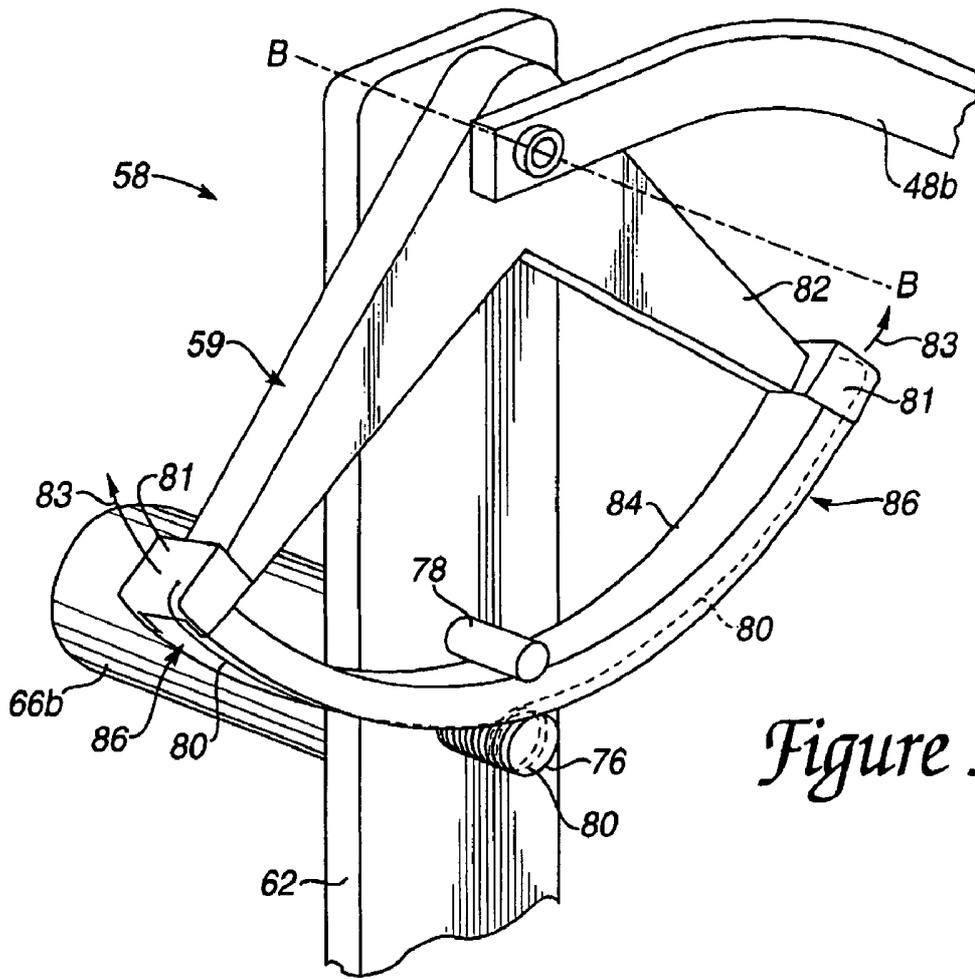
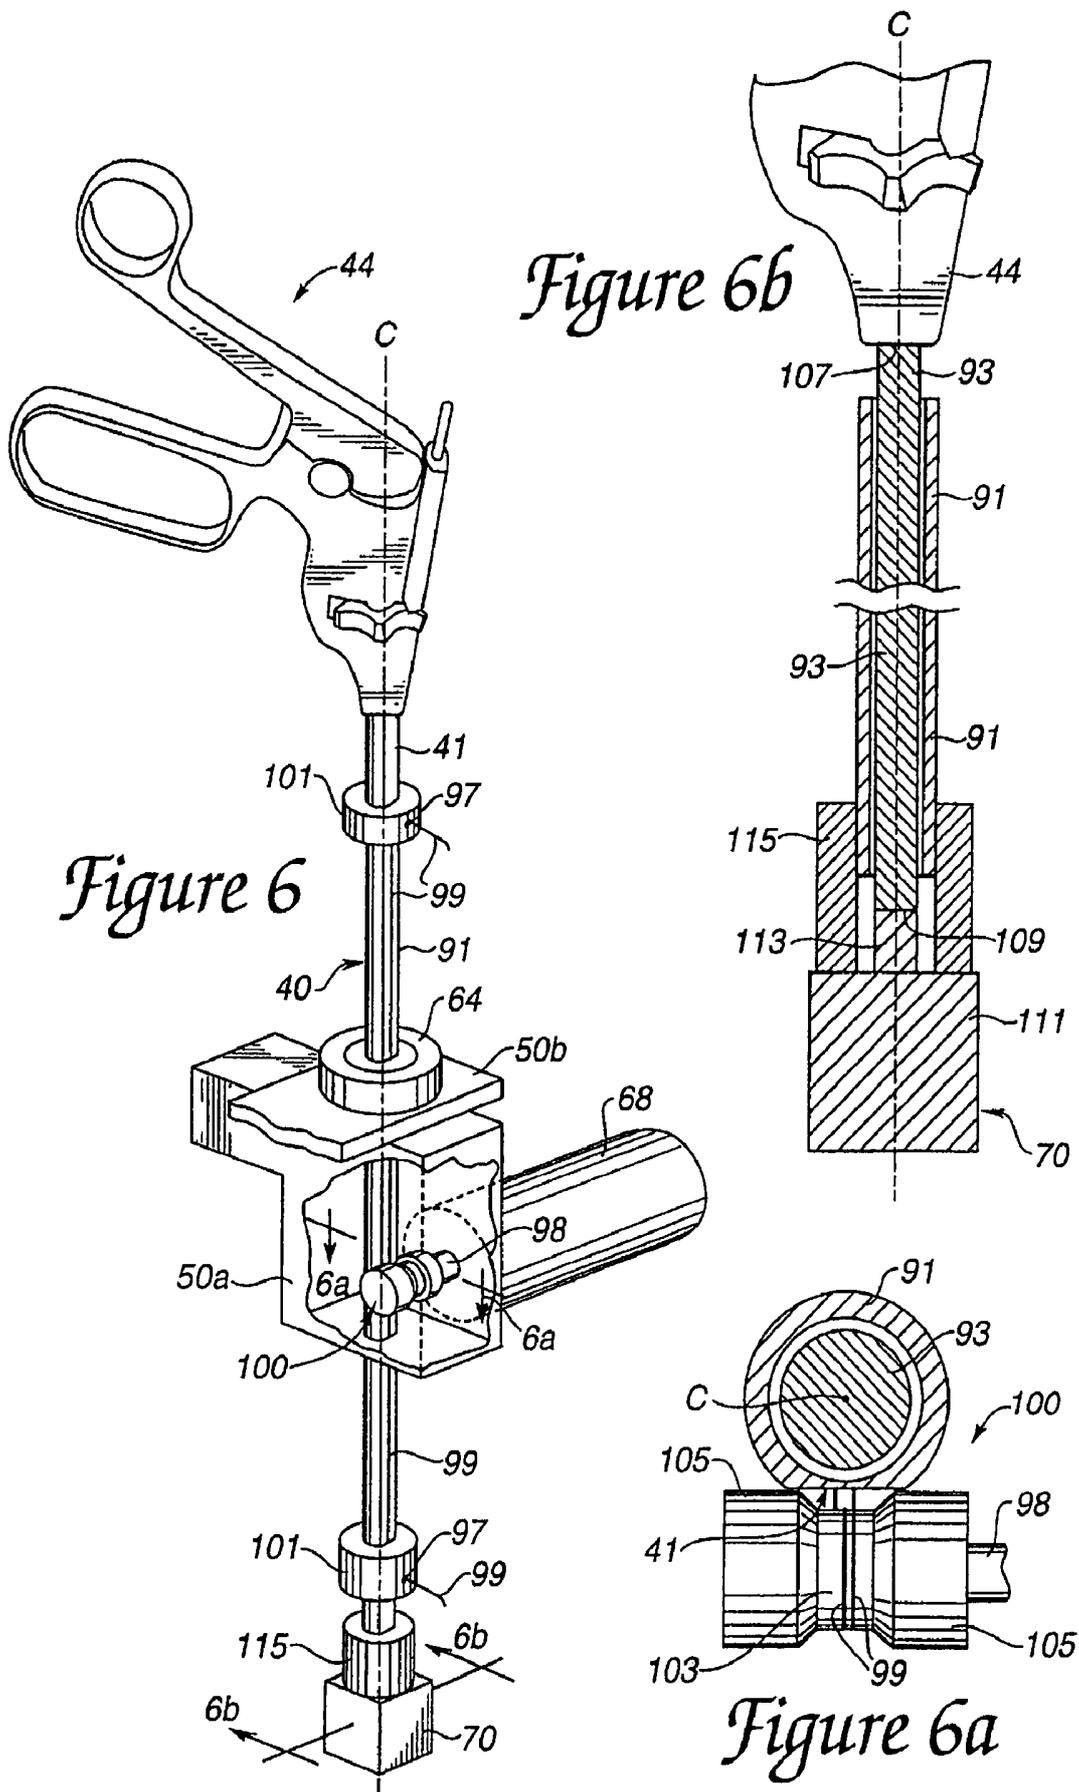


Figure 4





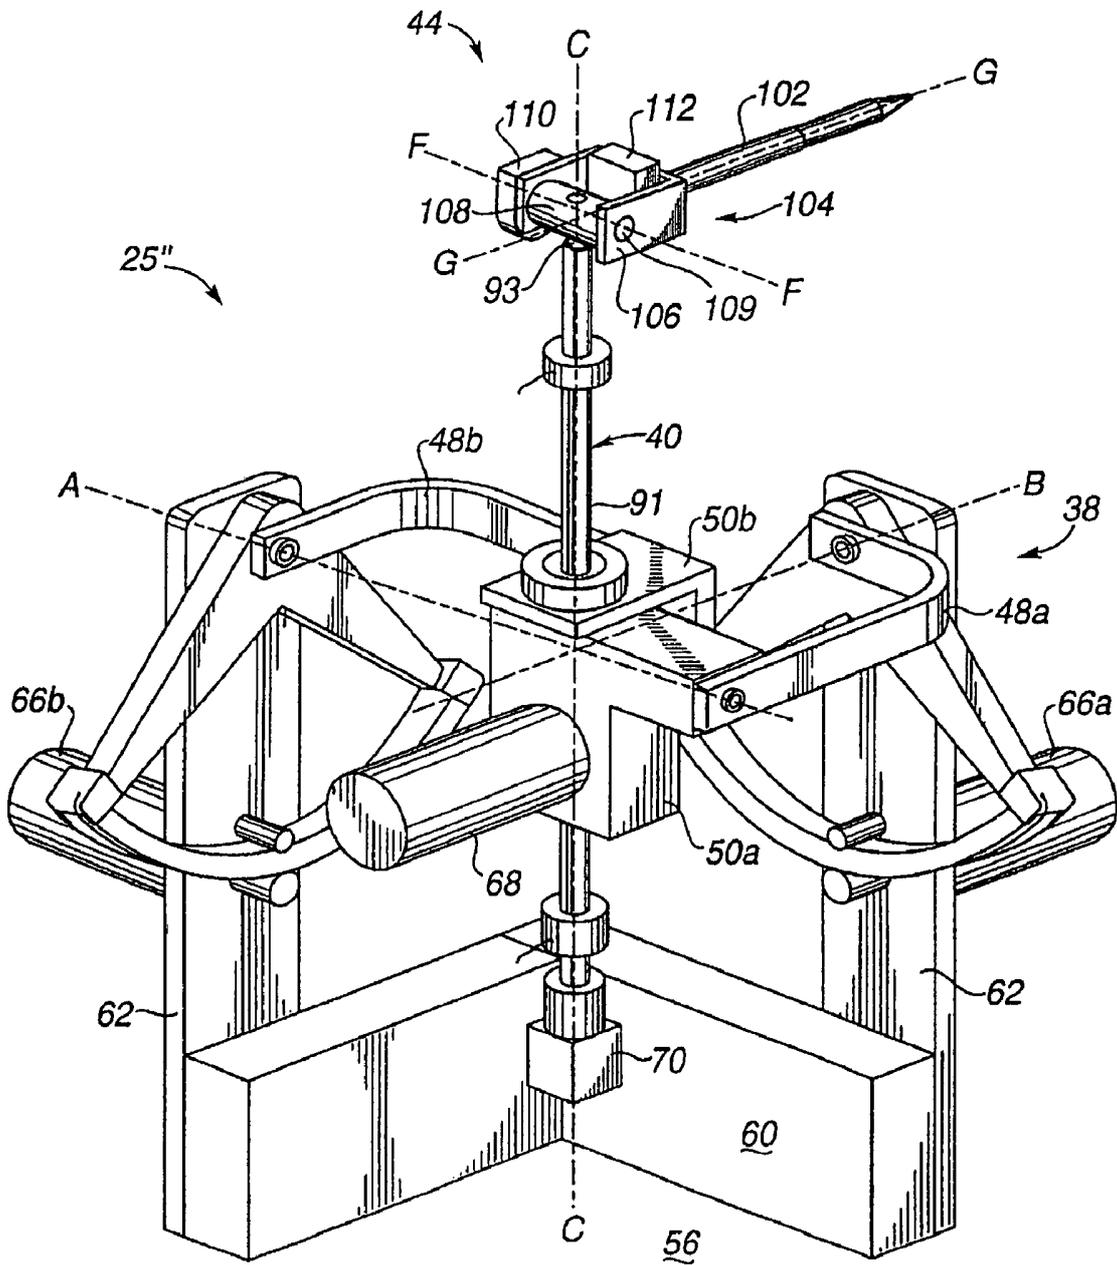


Figure 7

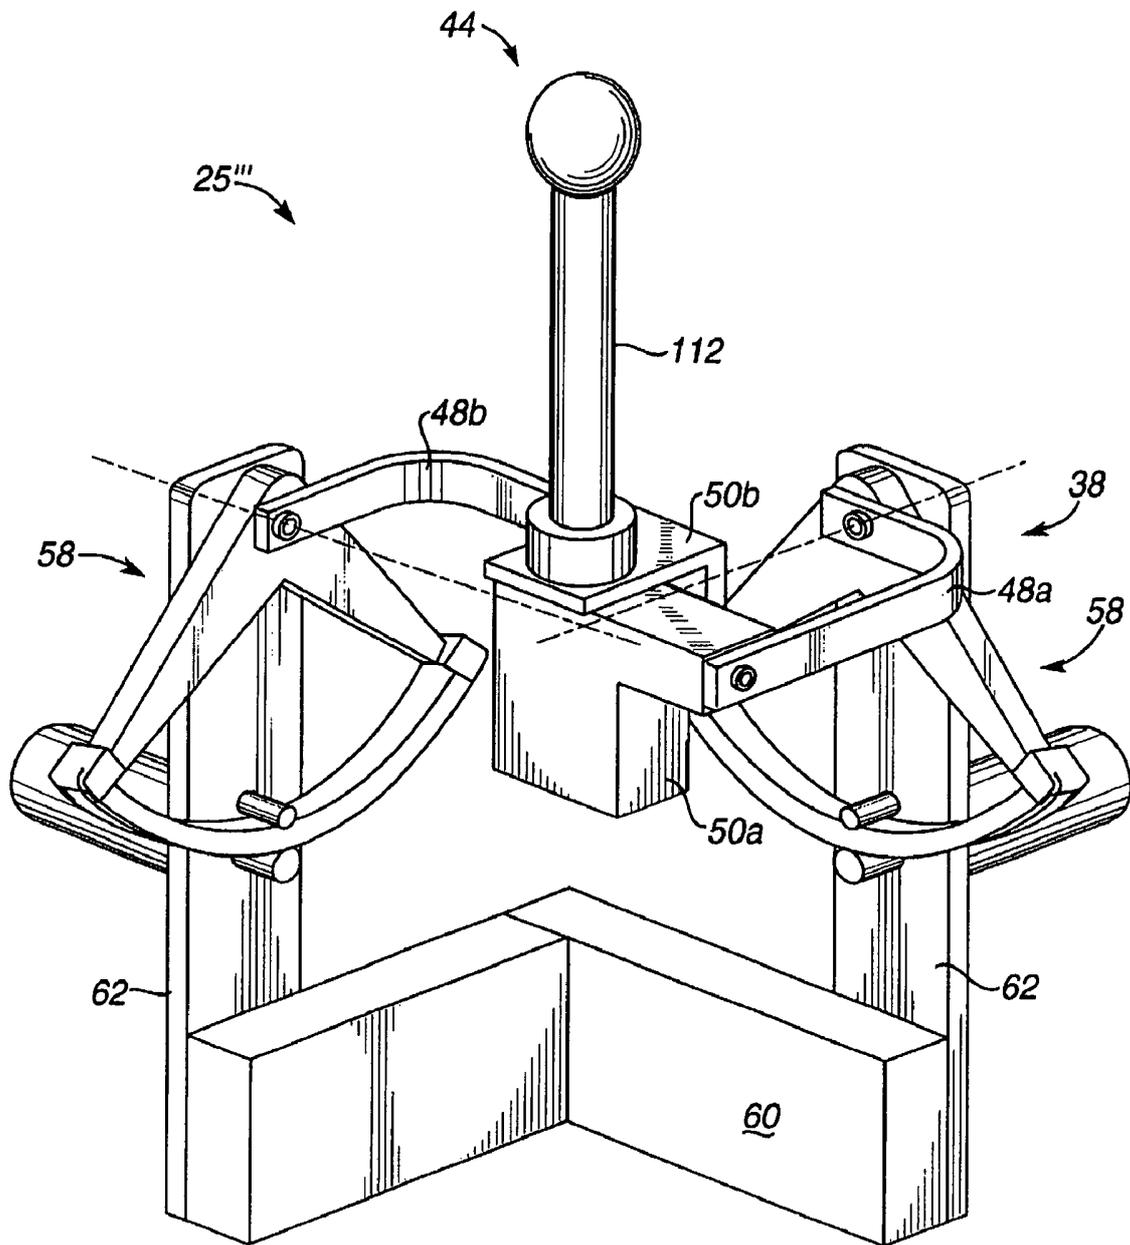


Figure 8

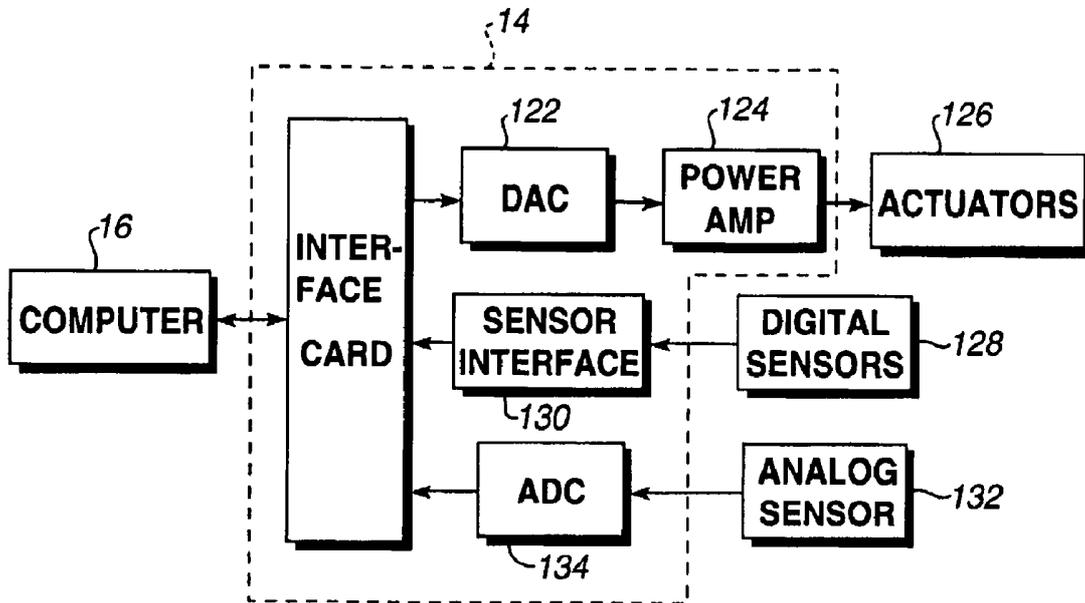


Figure 9

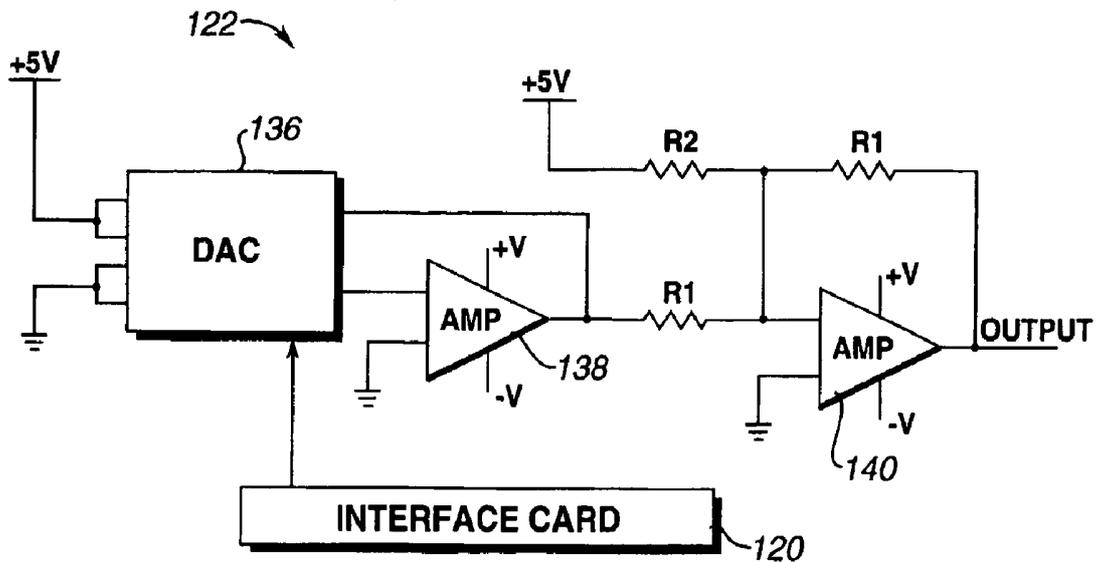


Figure 10

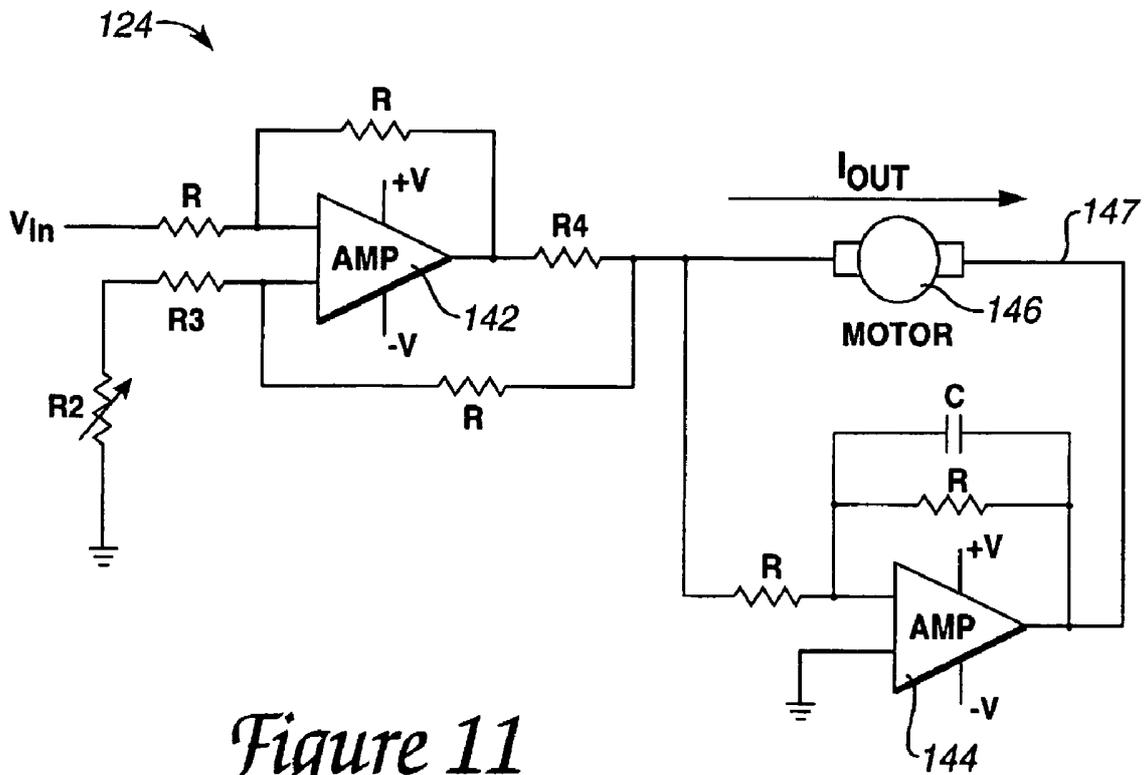


Figure 11

LAPAROSCOPIC SIMULATION INTERFACE

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. application Ser. No. 09/852,401, filed May 9, 2001, now U.S. Pat. No. 7,023, 423 which is a continuation of U.S. application Ser. No. 08/870,956, now U.S. Pat. No. 6,246,390, filed Jun. 6, 1997, which is a continuation of U.S. application Ser. No. 08/374, 288, now U.S. Pat. No. 5,731,804, filed Jan. 18, 1995, the entirety of which are incorporated herein by reference in their entirety.

BACKGROUND

The present invention relates generally to interface devices between humans and computers, and more particularly to computer input devices having three-dimensional input.

Virtual reality computer systems provide users with the illusion that they are part of a "virtual" environment. A virtual reality system will typically include a computer processor, such as a personal computer or workstation, specialized virtual reality software, and virtual reality I/O devices such as head mounted displays, sensor gloves, three dimensional ("3D") pointers, etc.

One common use for virtual reality computer systems is for training. In many fields, such as aviation and vehicle and systems operation, virtual reality systems have been used successfully to allow a user to learn from and experience a realistic "virtual" environment. The appeal of using virtual reality computer systems for training relates, in part, to the ability of such systems to allow trainees the luxury of confidently operating in a highly realistic environment and making mistakes without "real world" consequences. Thus, for example, a trainee pilot or automobile driver can learn to operate a vehicle using a virtual reality simulator without concern for accidents that would cause injury, death and/or property damage in the real world. Similarly, operators of complex systems, e.g., nuclear power plants and weapons systems, can safely practice a wide variety of training scenarios that would risk life or property if performed in reality.

For example, a virtual reality computer system can allow a doctor-trainee or other human operator or user to "manipulate" a scalpel or probe within a computer-simulated "body", and thereby perform medical procedures on a virtual patient. In this instance, the I/O device which is typically a 3D pointer, stylus, or the like is used to represent a surgical instrument such as a scalpel or probe. As the "scalpel" or "probe" moves within a provided space or structure, results of such movement are updated and displayed in a body image displayed on the screen of the computer system so that the operator can gain the experience of performing such a procedure without practicing on an actual human being or a cadaver.

In other applications, virtual reality computers systems allow a user to handle and manipulate the controls of complicated and expensive vehicles and machinery. For example, a pilot or astronaut in training can operate a fighter aircraft or spacecraft by manipulating controls such as a control joystick and other buttons and view the results of controlling the aircraft on a virtual reality simulation of the aircraft flying. In yet other applications, a user can manipulate objects and tools in the real world, such as a stylus, and view the results of the manipulation in a virtual reality world with a "virtual stylus" viewed on a screen, in 3-D goggles, etc.

For virtual reality systems to provide a realistic (and therefore effective) experience for the user, sensory feedback and

manual interaction should be as natural as possible. As virtual reality systems become more powerful and as the number of potential applications increases, there is a growing need for specific human/computer interface devices which allow users to interface with computer simulations with tools that realistically emulate the activities being represented within the virtual simulation. Such procedures as laparoscopic surgery, catheter insertion, and epidural analgesia should be realistically simulated with suitable human/computer interface devices if the doctor is to be properly trained. Similarly, a user should be provided with a realistic interface for manipulating controls or objects in a virtual reality simulation to gain useful experience.

While the state of the art in virtual simulation and medical imaging provides a rich and realistic visual feedback, there is a great need for new human/computer interface tools which allow users to perform natural manual interactions with the computer simulation. For medical simulation, there is a strong need to provide doctors with a realistic mechanism for performing the manual activities associated with medical procedures while allowing a computer to accurately keep track of their actions. There is also a need in other simulations to provide virtual reality users with accurate and natural interfaces for their particular tasks.

In addition to sensing and tracking a user's manual activity and feeding such information to the controlling computer to provide a 3D visual representation to the user, a human interface mechanism should also provide force or tactile ("haptic") feedback to the user. The need for the user to obtain realistic tactile information and experience tactile sensation is extensive in many kinds of simulation. For example, in medical/surgical simulations, the "feel" of a probe or scalpel simulator is important as the probe is moved within the simulated body. It would invaluable to a medical trainee to learn how an instrument moves within a body, how much force is required depending on the operation performed, the space available in a body to manipulate an instrument, etc. In simulations of vehicles or equipment, force feedback for controls such as a joystick can be necessary to realistically teach a user the force required to move the joystick when steering in specific situations, such as in a high acceleration environment of an aircraft. In virtual world simulations where the user can manipulate objects, force feedback is necessary to realistically simulate physical objects; for example, if a user touches a pen to a table, the user should feel the impact of the pen on the table. An effective human interface not only acts as an input device for tracking motion, but also as an output device for producing realistic tactile sensations. A "high bandwidth" interface system, which is an interface that accurately responds to signals having fast changes and a broad range of frequencies as well as providing such signals accurately to a control system, is therefore desirable in these and other applications.

There are number of devices that are commercially available for interfacing a human with a computer for virtual reality simulations. There are, for example, such 2-dimensional input devices such as mice, trackballs, and digitizing tablets. However, 2-dimensional input devices tend to be awkward and inadequate to the task of interfacing with 3-dimensional virtual reality simulations.

Other 3-dimensional interface devices are available. A 3-dimensional human/computer interface tool sold under the trademark Immersion PROBE.TM. is marketed by Immersion Human Interface Corporation of Santa Clara, Calif., and allows manual control in 3-dimensional virtual reality computer environments. A pen-like stylus allows for dexterous 3-dimensional manipulation, and the position and orientation

of the stylus is communicated to a host computer. The Immersion PROBE has six degrees of freedom which convey spatial coordinates (x, y, z) and orientation (roll, pitch, yaw) of the stylus to the host computer.

While the Immersion PROBE is an excellent 3-dimensional interface tool, it may be inappropriate for certain virtual reality simulation applications. For example, in some of the aforementioned medical simulations three or four degrees of freedom of a 3-dimensional human/computer interface tool is sufficient and, often, more desirable than five or six degrees of freedom because it more accurately mimics the real-life constraints of the actual medical procedure. More importantly, the Immersion PROBE does not provide force feedback to a user and thus does not allow a user to experience an entire sensory dimension in virtual reality simulations.

In typical multi-degree of freedom apparatuses that include force feedback, there are several disadvantages. Since actuators which supply force feedback tend to be heavier and larger than sensors, they would provide inertial constraints if added to a device such as the Immersion PROBE. There is also the problem of coupled actuators. In a typical force feedback device, a serial chain of links and actuators is implemented to achieve multiple degrees of freedom in a desired object positioned at the end of the chain, i.e., each actuator is coupled to the previous actuator. The user who manipulates the object must carry the inertia of all of the subsequent actuators and links except for the first actuator in the chain, which is grounded. While it is possible to ground all of the actuators in a serial chain by using a complex transmission of cables or belts, the end result is a low stiffness, high friction, high damping transmission which corrupts the bandwidth of the system, providing the user with an unresponsive and inaccurate interface. These types of interfaces also introduce tactile "noise" to the user through friction and compliance in signal transmission and limit the degree of sensitivity conveyed to the user through the actuators of the device.

Other existing devices provide force feedback to a user. In U.S. Pat. No. 5,184,319, by J. Kramer, an interface is described which provides force and texture information to a user of a computer system. The interface consists of a glove or "exoskeleton" which is worn over the user's appendages, such as fingers, arms, or body. Forces can be applied to the user's appendages using tendon assemblies and actuators controlled by a computer system to simulate force and textual feedback. However, the system described by Kramer is not easily applicable to simulation environments such as those mentioned above where an object is referenced in 3D space and force feedback is applied to the object. The forces applied to the user in Kramer are with reference to the body of the user; the absolute location of the user's appendages are not easily calculated. In addition, the exoskeleton devices of Kramer can be cumbersome or even dangerous to the user if extensive devices are worn over the user's appendages. Furthermore, the devices disclosed in Kramer are complex mechanisms in which many actuators must be used to provide force feedback to the user.

Therefore, a less complex, more compact, and less expensive alternative to a human/computer interface tool having force feedback, lower inertia, higher bandwidth, and less noise is desirable for certain applications.

SUMMARY OF THE INVENTION

The present invention provides a human/computer interface apparatus which can provide from two to six degrees of freedom and highly realistic force feedback to a user of the apparatus. The preferred apparatus includes a gimbal mechanism and linear axis member which provide three degrees of freedom to an object coupled to the apparatus and held by the user. The structure of the apparatus permits transducers to be positioned such that their inertial contribution to the system is very low. In addition, a capstan drive mechanism provides mechanical advantage in applying force feedback to the user, smooth motion, and reduction of friction, compliance, and backlash of the system. The present invention is particularly well suited to simulations of medical procedures using specialized tools and moving an object such as a stylus or joystick in three-dimensional simulations.

An apparatus of the present invention for interfacing the motion of an object with an electrical system includes a gimbal mechanism that provides two revolutive degrees of freedom to an object about two axes of rotation. In the preferred embodiment, the gimbal mechanism is a closed loop five-member linkage including a ground member coupled to a ground surface, first and second extension members, each being coupled to the ground member, and first and second central members, the first central member having an end coupled to the first extension member and the second central member having an end coupled to the second extension member.

A linear axis member is coupled to the gimbal mechanism at the intersection of the two central members, which is at the intersection of the two axes of rotation. The linear axis member is capable of being translated along a third axis to provide a third degree of freedom. The user object is coupled to the linear axis member and is thus translatable along the third axis so that the object can be moved along all three degrees of freedom. Transducers are also coupled between members of the gimbal mechanism and linear axis member to provide an electromechanical interface between the object and the electrical system.

In one embodiment, the linear axis member can be rotated about its lengthwise axis to provide a fourth degree of freedom. Four transducers are preferably provided, each transducer being associated with a degree of freedom. The transducers for the first three degrees of freedom include sensors and actuators, and the transducer for the fourth degree of freedom preferably includes a sensor. The sensors are preferably digital encoders and the actuators are basket wound DC servo motors. The sensors sense the positions of the object along the respective degrees of freedom and provide the sensory information to a digital processing system such as a computer. The actuators impart forces along the respective degrees of freedom in response to electrical signals produced by the computer.

In the preferred embodiment, a capstan drive mechanism is coupled between an actuator and the gimbal mechanism for each degree of freedom of the gimbal mechanism. The capstan drive mechanism transmits the force generated by the transducer to the gimbal mechanism and transmits any forces generated by the user on the gimbal mechanism to the transducer. In addition, a capstan drive mechanism is preferably used between the linear axis member and a transducer to transmit force along the third degree of freedom. The capstan drive mechanisms each preferably include a rotating capstan drum rotatably coupled to the gimbal mechanism, where the capstan drum is coupled to a pulley by a cable and the transducer is coupled to the pulley.

In another embodiment, a floating gimbal mechanism is coupled to the linear axis member to provide fifth and sixth degrees of freedom to an object coupled to the floating gimbal mechanism. Fifth and sixth degree of freedom transducers are coupled to the floating gimbal mechanism to sense the position of the object along the fifth and sixth degrees of freedom.

In one embodiment, the handle or grip of a medical tool such as a laparoscope is used as the object in a medical procedure simulation. In other embodiments, a stylus or a joystick is used as the object.

The gimbal mechanism of the present invention provides a structure allowing transducers associated with two degrees of freedom to be decoupled from each other and instead be coupled to a ground surface. This allows the weight of the transducers to contribute a negligible inertia to the system, providing a low friction, high bandwidth motion system. The addition of a linear axis member and transducer positioned near the center of rotation of the gimbal mechanism allows a third degree of freedom to be added with minimal inertia. The present invention also includes capstan drive mechanisms coupled between the transducers and moving components of the apparatus. The capstan drive provides mechanical advantage while allowing smooth movement to be achieved and providing negligible friction and backlash to the system. These advantages allow a computer system to have more complete and realistic control over force feedback sensations experienced by a user of the apparatus.

These and other advantages of the present invention will become apparent to those skilled in the art upon a reading of the following specification of the invention and a study of the several figures of the drawing.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a perspective view of a virtual reality system which employs an apparatus of the present invention to interface a laparoscope tool handle with a computer system;

FIG. 2 is a schematic diagram of a mechanical apparatus of the present invention for providing mechanical input and output to a computer system;

FIG. 3 is a perspective front view of a preferred embodiment of the mechanical apparatus of FIG. 2;

FIG. 4 is a perspective rear view of the embodiment of the mechanical apparatus of FIG. 3;

FIG. 5 is a perspective detailed view of a capstan drive mechanism used for two degrees of motion in the present invention;

FIG. 5a is a side elevational view of the capstan drive mechanism shown in FIG. 5;

FIG. 5b is a detailed side view of a pulley and cable of the capstan drive mechanism of FIG. 5;

FIG. 6 is a perspective view of a center capstan drive mechanism for a linear axis member of the mechanical apparatus shown in FIG. 3;

FIG. 6a is a cross sectional top view of a pulley and linear axis member used in the capstan drive mechanism of FIG. 6;

FIG. 6b is a cross sectional side view of the linear axis member and transducer shown in FIG. 6;

FIG. 7 is a perspective view of an embodiment of the apparatus of FIG. 2 having a stylus object for the user;

FIG. 8 is a perspective view of an embodiment of the apparatus of FIG. 2 having a joystick object for the user;

FIG. 9 is a block diagram of a computer and the interface between the computer and the mechanical apparatus of FIG. 2;

FIG. 10 is a schematic diagram of a suitable circuit for a digital to analog controller of the interface of FIG. 9; and

FIG. 11 is a schematic diagram of a suitable power amplification circuit for powering the actuators of the present invention as shown in FIG. 9.

DETAILED DESCRIPTION

In FIG. 1, a virtual reality system 10 used to simulate a medical procedure includes a human/computer interface apparatus 12, an electronic interface 14, and a computer 16. The illustrated virtual reality system 10 is directed to a virtual reality simulation of a laparoscopic surgery procedure. The software of the simulation is not a part of this invention and thus will not be discussed in any detail. However, such software is commercially available as, for example, Teleos.TM. from High Techsplinations of Rockville, Md. Suitable software drivers which interface such simulation software with computer input/output (I/O) devices are available from Immersion Human Interface Corporation of Santa Clara, Calif.

The handle 26 of a laparoscopic tool 18 used in conjunction with the present invention is manipulated by an operator and virtual reality images are displayed on a screen 20 of the digital processing system in response to such manipulations. Preferably, the digital processing system is a personal computer or workstation, such as an IBM-PC AT or Macintosh personal computer, or a SUN or Silicon Graphics workstation. Most commonly, the digital processing system is a personal computer which operates under the MS-DOS operating system in conformance with in IBM PC AT standard.

The human/interface apparatus 12 as illustrated herein is used to simulate a laparoscopic medical procedure. In addition to the handle of a standard laparoscopic tool 18, the human/interface apparatus 12 may include a barrier 22 and a standard laparoscopic trocar 24 (or a facsimile of a trocar). The barrier 22 is used to represent portion of the skin covering the body of a patient. Trocar 24 is inserted into the body of the virtual patient to provide an entry and removal point from the body of the patient for the laparoscopic tool 18, and to allow the manipulation of the laparoscopic tool. Laparoscopic tools and trocars 24 are commercially available from sources such as U.S. Surgical of Connecticut. Barrier 22 and trocar 24 can be omitted from apparatus 12 in other embodiments. Preferably, the laparoscopic tool 18 is modified, in the preferred embodiment, the shaft is replaced by a linear axis member of the present invention, as described below. In other embodiments, the end of the shaft of the tool (such as any cutting edges) can be removed. The end of the laparoscopic tool 18 is not required for the virtual reality simulation, and is removed to prevent any potential damage to persons or property. An apparatus 25 for interfacing mechanical input and output is shown within the "body" of the patient in phantom lines.

The laparoscopic tool 18 includes a handle or "grip" portion 26 and a shaft portion 28. The shaft portion is an elongated mechanical object and, in particular, is an elongated cylindrical object, described in greater detail below. In one embodiment, the present invention is concerned with tracking the movement of the shaft portion 28 in three-dimensional space, where the movement has been constrained such that the shaft portion 28 has only three or four free degrees of motion. This is a good simulation of the real use of a laparoscopic tool 18 in that once it is inserted into a trocar 24 and through the gimbal apparatus 25, it is limited to about four degrees of freedom. More particularly, the shaft 28 is constrained at some point of along its length such that it can move with four degrees of freedom within the patient's body.

While one embodiment of the present invention will be discussed with reference to the laparoscopic tool 18, it will be appreciated that a great number of other types of objects can be used with the method and apparatus of the present invention. In fact, the present invention can be used with any mechanical object where it is desirable to provide a human/

computer interface with three to six degrees of freedom. Such objects may include endoscopic or other similar surgical tools used in medical procedures, catheters, hypodermic needles, wires, fiber optic bundles, styluses, joysticks, screw drivers, pool cues, etc. Some of these other objects are described in detail subsequently.

The electronic interface **14** is a component of the human/computer interface apparatus **12** and couples the apparatus **12** to the computer **16**. More particularly, interface **14** is used in preferred embodiments to couple the various actuators and sensors contained in apparatus **12** (which actuators and sensors are described in detail below) to computer **16**. A suitable interface **14** is described in detail with reference to FIG. 9.

The electronic interface **14** is coupled to mechanical apparatus **25** of the apparatus **12** by a cable **30** and is coupled to the computer **16** by a cable **32**. In other embodiments, signal can be sent to and from interface **14** and computer **16** by wireless transmission and reception. In some embodiments of the present invention, interface **14** serves solely as an input device for the computer **16**. In other embodiments of the present invention, interface **14** serves solely as an output device for the computer **16**. In preferred embodiments of the present invention, the interface **14** serves as an input/output (I/O) device for the computer **16**.

In FIG. 2, a schematic diagram of mechanical apparatus **25** for providing mechanical input and output in accordance with the present invention is shown. Apparatus **25** includes, a gimbal mechanism **38** and a linear axis member **40**. A user object **44** is preferably coupled to linear axis member **40**.

Gimbal mechanism **38**, in the described embodiment, provides support for apparatus **25** on a grounded surface **56** (schematically shown as part of member **46**). Gimbal mechanism **38** is preferably a five-member linkage that includes a ground member **46**, extension members **48a** and **48b**, and central members **50a** and **50b**. Ground member **46** is coupled to a base or surface which provides stability for apparatus **25**. Ground member **46** is shown in FIG. 2 as two separate members coupled together through grounded surface **56**. The members of gimbal mechanism **38** are rotatably coupled to one another through the use of bearings or pivots, wherein extension member **48a** is rotatably coupled to ground member **46** and can rotate about an axis A, central member **50a** is rotatably coupled to extension member **48a** and can rotate about a floating axis D, extension member **48b** is rotatably coupled to ground member **46** and can rotate about axis B, central member **50b** is rotatably coupled to extension member **48b** and can rotate about floating axis E, and central member **50a** is rotatably coupled to central member **50b** at a center point P at the intersection of axes D and E. The axes D and E are "floating" in the sense that they are not fixed in one position as are axes A and B. Axes A and B are substantially mutually perpendicular. As used herein, "substantially perpendicular" will mean that two objects or axis are exactly or almost perpendicular, i.e. at least within five degrees or ten degrees of perpendicular, or more preferably within less than one degree of perpendicular. Similarly, the term "substantially parallel" will mean that two objects or axis are exactly or almost parallel, i.e. are at least within five or ten degrees of parallel, and are preferably within less than one degree of parallel.

Gimbal mechanism **38** is formed as a five member closed chain. Each end of one member is coupled to the end of another member. The five-member linkage is arranged such that extension member **48a**, central member **50a**, and central member **50b** can be rotated about axis A in a first degree of freedom. The linkage is also arranged such that extension

member **48b**, central member **50b**, and central member **50a** can be rotated about axis B in a second degree of freedom.

Linear axis member **40** is preferably an elongated rod-like member which is coupled to central member **50a** and central member **50b** at the point of intersection P of axes A and B. As shown in FIG. 1, linear axis member **40** can be used as shaft **28** of user object **44**. In other embodiments, linear axis member **40** is coupled to a different object. Linear axis member **40** is coupled to gimbal mechanism **38** such that it extends out of the plane defined by axis A and axis B. Linear axis member **40** can be rotated about axis A by rotating extension member **48a**, central member **50a**, and central member **50b** in a first revolute degree of freedom, shown as arrow line **51**. Member **40** can also be rotated about axis B by rotating extension member **50b** and the two central members about axis B in a second revolute degree of freedom, shown by arrow line **52**. Being also translatably coupled to the ends of central members **50a** and **50b**, linear axis member **40** can be linearly moved along floating axis C, providing a third degree of freedom as shown by arrows **53**. Axis C can, of course, be rotated about one or both axes A and B as member **40** is rotated about these axes.

Also preferably coupled to gimbal mechanism **38** and linear axis member **40** are transducers, such as sensors and actuators. Such transducers are preferably coupled at the link points between members of the apparatus and provide input to and output from an electrical system, such as computer **16**. Transducers that can be used with the present invention are described in greater detail with respect to FIG. 2.

User object **44** is coupled to apparatus **25** and is preferably an interface object for a user to grasp or otherwise manipulate in three dimensional (3D) space. One preferred user object **44** is the grip **26** of a laparoscopic tool **18**, as shown in FIG. 1. Shaft **28** of tool **18** can be implemented as part of linear axis member **40**. Other examples of user objects are described in subsequent embodiments. User object **44** may be moved in all three degrees of freedom provided by gimbal mechanism **38** and linear axis member **40** and additional degrees of freedom as described below. As user object **44** is moved about axis A, floating axis D varies its position, and as user object **44** is moved about axis B, floating axis E varies its position.

FIGS. 3 and 4 are perspective views of a specific embodiment of a mechanical apparatus **25'** for providing mechanical input and output to a computer system in accordance with the present invention. FIG. 3 shows a front view of apparatus **25'**, and FIG. 4 shows a rear view of the apparatus. Apparatus **25'** includes a gimbal mechanism **38**, a linear axis member **40**, and transducers **42**. A user object **44**, shown in this embodiment as a laparoscopic instrument having a grip portion **26**, is coupled to apparatus **25'**. Apparatus **25'** operates in substantially the same fashion as apparatus **25** described with reference to FIG. 2.

Gimbal mechanism **38** provides support for apparatus **25'** on a grounded surface **56**, such as a table top or similar surface. The members and joints ("bearings") of gimbal mechanism **38** are preferably made of a lightweight, rigid, stiff metal, such as aluminum, but can also be made of other rigid materials such as other metals, plastic, etc. Gimbal mechanism **38** includes a ground member **46**, capstan drive mechanisms **58**, extension members **48a** and **48b**, central drive member **50a**, and central link member **50b**. Ground member **46** includes a base member **60** and vertical support members **62**. Base member **60** is coupled to grounded surface **56** and provides two outer vertical surfaces **61** which are in a substantially perpendicular relation which each other. A vertical support member **62** is coupled to each of these outer

surfaces of base member 60 such that vertical members 62 are in a similar substantially 90-degree relation with each other.

A capstan drive mechanism 58 is preferably coupled to each vertical member 62. Capstan drive mechanisms 58 are included in gimbal mechanism 38 to provide mechanical advantage without introducing friction, and backlash to the system. A capstan drum 59 of each capstan drive mechanism is rotatably coupled to a corresponding vertical support member 62 to form axes of rotation A and B, which correspond to axes A and B as shown in FIG. 1. The capstan drive mechanisms 58 are described in greater detail with respect to FIG. 5.

Extension member 48a is rigidly coupled to capstan drum 59 and is rotated about axis A as capstan drum 59 is rotated. Likewise, extension member 48b is rigidly coupled to the other capstan drum 59 and can be rotated about axis B. Both extension members 48a and 48b are formed into a substantially 90-degree angle with a short end 49 coupled to capstan drum 59. Central drive member 50a is rotatably coupled to a long end 51 of extension member 48a and extends at a substantially parallel relation with axis B. Similarly, central link member 50b is rotatably coupled to the long end of extension member 48b and extends at a substantially parallel relation to axis A (as better viewed in FIG. 4). Central drive member 50a and central link member 50b are rotatably coupled to each other at the center of rotation of the gimbal mechanism, which is the point of intersection P of axes A and B. Bearing 64 connects the two central members 50a and 50b together at the intersection point P.

Gimbal mechanism 38 provides two degrees of freedom to an object positioned at or coupled to the center point P of rotation. An object at or coupled to point P can be rotated about axis A and B or have a combination of rotational movement about these axes.

Linear axis member 40 is a cylindrical member that is preferably coupled to central members 50a and 50b at intersection point P. In alternate embodiments, linear axis member 40 can be a non-cylindrical member having a cross-section of, for example, a square or other polygon. Member 40 is positioned through the center of bearing 64 and through holes in the central members 50a and 50b. The linear axis member can be linearly translated along axis C, providing a third degree of freedom to user object 44 coupled to the linear axis member. Linear axis member 40 can preferably be translated by a transducer 42 using a capstan drive mechanism similar to capstan drive mechanism 58. The translation of linear axis member 40 is described in greater detail with respect to FIG. 6.

Transducers 42 are preferably coupled to gimbal mechanism 38 to provide input and output signal between mechanical apparatus 25' and computer 16. In the described embodiment, transducers 42 include two grounded transducers 66a and 66b, central transducer 68, and shaft transducer 70. The housing of grounded transducer 66a is preferably coupled to vertical support member 62 and preferably includes both an actuator for providing force in or otherwise influencing the first revolute degree of freedom about axis A and a sensor for measuring the position of object 44 in or otherwise influenced by the first degree of freedom about axis A, i.e., the transducer 66a is "associated with" or "related to" the first degree of freedom. A rotational shaft of actuator 66a is coupled to a pulley of capstan drive mechanism 58 to transmit input and output along the first degree of freedom. The capstan drive mechanism 58 is described in greater detail with respect to FIG. 5. Grounded transducer 66b preferably corresponds to grounded transducer 66a in function and operation. Transducer 66b is coupled to the other vertical support member 62

and is an actuator/sensor which influences or is influenced by the second revolute degree of freedom about axis B.

Grounded transducers 66a and 66b are preferably bidirectional transducers which include sensors and actuators. The sensors are preferably relative optical encoders which provide signals to measure the angular rotation of a shaft of the transducer. The electrical outputs of the encoders are routed to computer interface 14 via buses 67a and 67b and are detailed with reference to FIG. 9. Other types of sensors can also be used, such as potentiometers, etc.

It should be noted that the present invention can utilize both absolute and relative sensors. An absolute sensor is one which the angle of the sensor is known in absolute terms, such as with an analog potentiometer. Relative sensors only provide relative angle information, and thus require some form of calibration step which provide a reference position for the relative angle information. The sensors described herein are primarily relative sensors. In consequence, there is an implied calibration step after system power-up wherein the sensor's shaft is placed in a known position within the apparatus 25' and a calibration signal is provided to the system to provide the reference position mentioned above. All angles provided by the sensors are thereafter relative to that reference position. Such calibration methods are well known to those skilled in the art and, therefore, will not be discussed in any great detail herein.

Transducers 66a and 66b also preferably include actuators which, in the described embodiment, are linear current control motors, such as DC servo motors. These motors preferably receive current signals to control the direction and torque (force output) that is produced on a shaft; the control signals for the motor are produced by computer interface 14 on control buses 67a and 67b and are detailed with respect to FIG. 9. The motors may include brakes which allow the rotation of the shaft to be halted in a short span of time. A suitable transducer for the present invention including both an optical encoder and current controlled motor is a 20 W basket wound servo motor manufactured by Maxon of Burlingame, Calif.

In alternate embodiments, other types of motors can be used, such as a stepper motor controlled with pulse width modulation of an applied voltage, or pneumatic motors. However, the present invention is much more suited to the use of linear current controlled motors. This is because voltage pulse width modulation or stepper motor control involves the use of steps or pulses which can be felt as "noise" by the user. Such noise corrupts the virtual simulation. Linear current control is smoother and thus more appropriate for the present invention.

Passive actuators can also be used in transducers 66a, 66b and 68. Magnetic particle brakes or friction brakes can be used in addition to or instead of a motor to generate a passive resistance or friction in a degree of motion. An alternate preferred embodiment only including passive actuators may not be as realistic as an embodiment including motors; however, the passive actuators are typically safer for a user since the user does not have to fight generated forces.

In other embodiments, all or some of transducers 42 can include only sensors to provide an apparatus without force feedback along designated degrees of freedom. Similarly, all or some of transducers 42 can be implemented as actuators without sensors to provide only force feedback.

Central transducer 68 is coupled to central drive member 50a and preferably includes an actuator for providing force in the linear third degree of freedom along axis C and a sensor for measuring the position of object 44 along the third degree of freedom. The rotational shaft of central transducer 68 is

coupled to a translation interface coupled to central drive member **50a** which is described in greater detail with respect to FIG. 6. In the described embodiment, central transducer **68** is an optical encoder and DC servo motor combination similar to the actuators **66a** and **66b** described above.

The transducers **66a**, **66b** and **68** of the described embodiment are advantageously positioned to provide a very low amount of inertia to the user handling object **44**. Transducer **66a** and transducer **66b** are decoupled, meaning that the transducers are both directly coupled to ground member **46** which is coupled to ground surface **56**, i.e. the ground surface carries the weight of the transducers, not the user handling object **44**. The weights and inertia of the transducers **66a** and **66b** are thus substantially negligible to a user handling and moving object **44**. This provides a more realistic interface to a virtual reality system, since the computer can control the transducers to provide substantially all of the forces felt by the user in these degrees of motion. Apparatus **25'** is a high bandwidth force feedback system, meaning that high frequency signals can be used to control transducers **42** and these high frequency signals will be applied to the user object with high precision, accuracy, and dependability. The user feels very little compliance or "mushiness" when handling object **44** due to the high bandwidth. In contrast, in typical prior art arrangements of multi-degree of freedom interfaces, one actuator "rides" upon another actuator in a serial chain of links and actuators. This low bandwidth arrangement causes the user to feel the inertia of coupled actuators when manipulating an object.

Central transducer **68** is positioned near the center of rotation of two revolute degrees of freedom. Though the transducer **68** is not grounded, its central position permits a minimal inertial contribution to the mechanical apparatus **25'** along the provided degrees of freedom. A user manipulating object **44** thus will feel minimal internal effects from the weight of transducers **66a**, **66b** and **68**.

Shaft transducer **70** preferably includes a sensor and is provided in the described embodiment to measure a fourth degree of freedom for object **44**. Shaft transducer **70** is preferably positioned at the end of linear axis member **40** that is opposite to the object **44** and measures the rotational position of object **44** about axis C in the fourth degree of freedom, as indicated by arrow **72**. Shaft transducer **70** is described in greater detail with respect to FIGS. 6 and 6b. Preferably, shaft transducer **72** is implemented using an optical encoder similar to the encoders described above. A suitable input transducer for use in the present invention is an optical encoder model SI marketed by U.S. Digital of Vancouver, Wash. In the described embodiment, shaft transducer **70** only includes a sensor and not an actuator. This is because for typical medical procedures, which is one intended application for the embodiment shown in FIGS. 3 and 4, rotational force feedback to a user about axis C is typically not required to simulate actual operating conditions. However, in alternate embodiments, an actuator such as a motor can be included in shaft transducer **70** similar to transducers **66a**, **66b**, and **68**.

Object **44** is shown in FIGS. 3 and 4 as a grip portion **26** of a laparoscopic tool similar to the tool shown in FIG. 1. Shaft portion **28** is implemented as linear axis member **40**. A user can move the laparoscopic tool about axes A and B, and can translate the tool along axis C and rotate the tool about axis C. The movements in these four degrees of freedom will be sensed and tracked by computer system **16**. Forces can be applied preferably in the first three degrees of freedom by the computer system to simulate the tool impacting a portion of subject body, experiencing resistance moving through tissues, etc.

Optionally, additional transducers can be added to apparatus **25'** to provide additional degrees of freedom for object **44**. For example, a transducer can be added to grip **26** of laparoscopic tool **18** to sense when the user moves the two portions **26a** and **26b** relative to each other to simulate extending the cutting blade of the tool. Such a laparoscopic tool sensor is described in U.S. patent application Ser. No. 08/275,120, now U.S. Pat. No. 5,623,582 filed Jul. 14, 1994 and entitled "Method and Apparatus for Providing Mechanical I/O for Computer Systems" assigned to the assignee of the present invention and incorporated herein by reference in its entirety.

FIG. 5 is a perspective view of capstan drive mechanism **58** shown in some detail. As an example, the drive mechanism **58** coupled to extension arm **48b** is shown; the other capstan drive **58** coupled to extension arm **48a** is substantially similar to the mechanism presented here. Capstan drive mechanism **58** includes capstan drum **59**, capstan pulley **76**, and stop **78**. Capstan drum **59** is preferably a wedge-shaped member having leg portion **82** and a curved portion **84**. Other shapes of member **59** can also be used. Leg portion **82** is pivotally coupled to vertical support member **62** at axis B (or axis A for the opposing capstan drive mechanism). Extension member **48b** is rigidly coupled to leg portion **82** such that when capstan drum **59** is rotated about axis B, extension member **48b** is also rotated and maintains the position relative to leg portion **82** as shown in FIG. 5. Curved portion **84** couples the two ends of leg portion **82** together and is preferably formed in an arc centered about axis B. Curved portion **84** is preferably positioned such that its bottom edge **86** is about 0.030 inches above pulley **76**.

Cable **80** is preferably a thin metal cable connected to curved portion **84** of the capstan drum. Other types of durable cables, cords, wire, etc. can be used as well. Cable **80** is attached at a first end to curved portion **84** near an end of leg portion **82** and is drawn tautly against the outer surface **86** of curved portion **84**. Cable **80** is wrapped around pulley **76** a number of times and is then again drawn tautly against outer surface **86**. The second end of cable **80** is firmly attached to the other end of curved portion **84** near the opposite leg of leg portion **82**. The cable transmits rotational force from pulley **76** to the capstan drum **59**, causing capstan drum **59** to rotate about axis B as explained below. The cable also transmits rotational force from drum **59** to the pulley and transducer **66b**. The tension in cable **80** should be at a level so that negligible backlash or play occurs between capstan drum **59** and pulley **76**. Preferably, the tension of cable **80** can be adjusted by pulling more (or less) cable length through an end of curved portion **84**. Caps **81** on the ends of curved portion **84** can be used to easily tighten cable **80**. Each cap **81** is preferably tightly coupled to cable **80** and includes a pivot and tightening screw which allow the cap to move in a direction indicated by arrow **83** to tighten cable **80**.

Capstan pulley **76** is a threaded metal cylinder which transfers rotational force from transducer **66b** to capstan drum **59** and from capstan drum **59** to transducer **66b**. Pulley **76** is rotationally coupled to vertical support member **62** by a shaft **88** (shown in FIG. 5a) positioned through a bore of vertical member **62** and rigidly attached to pulley **76**. Transducer **66b** is coupled to pulley **76** by shaft **88** through vertical support member **62**. Rotational force is applied from transducer **66b** to pulley **76** when the actuator of transducer **66b** rotates the shaft. The pulley, in turn, transmits the rotational force to cable **80** and thus forces capstan drum **59** to rotate in a direction about axis B. Extension member **48b** rotates with capstan drum **59**, thus causing force along the second degree of freedom for object **44**. Note that pulley **76**, capstan drum **59** and extension member **48b** will only actually rotate if the user is

not applying the same amount or a greater amount of rotational force to object 44 in the opposite direction to cancel the rotational movement. In any event, the user will feel the rotational force along the second degree of freedom in object 44 as force feedback.

The capstan mechanism 58 provides a mechanical advantage to apparatus 25' so that the force output of the actuators can be increased. The ratio of the diameter of pulley 76 to the diameter of capstan drum 59 (i.e. double the distance from axis B to the bottom edge 86 of capstan drum 59) dictates the amount of mechanical advantage, similar to a gear system. In the preferred embodiment, the ratio of drum to pulley is equal to 15:1, although other ratios can be used in other embodiments.

Similarly, when the user moves object 44 in the second degree of freedom, extension member 48b rotates about axis B and rotates capstan drum 59 about axis B as well. This movement causes cable 80 to move, which transmits the rotational force to pulley 76. Pulley 76 rotates and causes shaft 88 to rotate, and the direction and magnitude of the movement is detected by the sensor of transducer 66b. A similar process occurs along the first degree of freedom for the other capstan drive mechanism 58. As described above with respect to the actuators, the capstan drive mechanism provides a mechanical advantage to amplify the sensor resolution by a ratio of drum 59 to pulley 76 (15:1 in the preferred embodiment).

Stop 78 is rigidly coupled to vertical support member 62 a few millimeters above curved portion 84 of capstan drum 59. Stop 78 is used to prevent capstan drum 59 from moving beyond a designated angular limit. Thus, drum 59 is constrained to movement within a range defined by the arc length between the ends of leg portion 82. This constrained movement, in turn, constrains the movement of object 44 in the first two degrees of freedom. In the described embodiment, stop 78 is a cylindrical member inserted into a threaded bore in vertical support member 62.

FIG. 5a is a side elevational view of capstan mechanism 58 as shown in FIG. 5. Cable 80 is shown routed along the bottom side 86 of curved portion 84 of capstan drum 59. Cable 80 is preferably wrapped around pulley 76 so that the cable is positioned between threads 90, i.e., the cable is guided by the threads as shown in greater detail in FIG. 5b. As pulley 76 is rotated by transducer 66b or by the manipulations of the user, the portion of cable 80 wrapped around the pulley travels closer to or further from vertical support member 62, depending on the direction that pulley 76 rotates. For example, if pulley 76 is rotated counterclockwise (when viewing the pulley as in FIG. 5), then cable 80 moves toward vertical support member 62 as shown by arrow 92. Capstan drum 59 also rotates clockwise as shown by arrow 94. The threads of pulley 76 are used mainly to provide cable 80 with a better grip on pulley 76. In alternate embodiments, pulley 76 includes no threads, and the high tension in cable 80 allows cable 80 to grip pulley 76.

Capstan drive mechanism 58 is advantageously used in the present invention to provide transmission of forces and mechanical advantage between transducers 66a and 66b and object 44 without introducing substantial compliance, friction, or backlash to the system. A capstan drive provides increased stiffness, so that forces are transmitted with negligible stretch and compression of the components. The amount of friction is also reduced with a capstan drive mechanism so that substantially "noiseless" tactile signals can be provided to the user. In addition, the amount of backlash contributed by a capstan drive is also negligible. "Backlash" is the amount of play that occurs between two coupled rotat-

ing objects in a gear or pulley system. Two gears, belts, or other types of drive mechanisms could also be used in place of capstan drive mechanism 58 in alternate embodiments to transmit forces between transducer 66a and extension member 48b. However, gears and the like typically introduce some backlash in the system. In addition, a user might be able to feel the interlocking and grinding of gear teeth during rotation of gears when manipulating object 44; the rotation in a capstan drive mechanism is much less noticeable.

FIG. 6 is a perspective view of central drive member 50a and linear axis member 40 shown in some detail. Central drive member 50a is shown in a partial cutaway view to expose the interior of member 50a. Central transducer 68 is coupled to one side of central drive member 50a. In the described embodiment, a capstan drive mechanism is used to transmit forces between transducer 68 and linear axis member 40 along the third degree of freedom. A rotatable shaft 98 of transducer 68 extends through a bore in the side wall of central drive member 50a and is coupled to a capstan pulley 100. Pulley 100 is described in greater detail below with respect to FIG. 6a.

Linear axis member 40 preferably includes an exterior sleeve 91 and an interior shaft 93 (described with reference to FIG. 6b, below). Exterior sleeve 91 is preferably a partially cylindrical member having a flat 41 provided along its length. Flat 41 prevents sleeve 91 from rotating about axis C in the fourth degree of freedom described above. Linear axis member 40 is provided with a cable 99 which is secured on each end of member 40 by tension caps 101. Cable 99 preferably runs down a majority of the length of exterior sleeve 91 on the surface of flat 41 and can be tightened, for example, by releasing a screw 97, pulling an end of cable 99 until the desired tension is achieved, and tightening screw 97. Similarly to the cable of the capstan mechanism described with reference to FIG. 5, cable 99 should have a relatively high tension.

As shown in FIG. 6a, cable 99 is wrapped a number of times around pulley 100 so that forces can be transmitted between pulley 100 and linear axis member 40. Pulley 100 preferably includes a central axle portion 103 and end lip portions 105. Exterior sleeve 91 is preferably positioned such that flat 41 of the sleeve is touching or is very close to lip portions 105 on both sides of axle portion 103. The cable 99 portion around pulley 100 is wrapped around central axle portion 103 and moves along portion 103 towards and away from shaft 98 as the pulley is rotated clockwise and counterclockwise, respectively. The diameter of axle portion 103 is smaller than lip portion 105, providing space between the pulley 100 and flat 41 where cable 99 is attached and allowing free movement of the cable. Pulley 100 preferably does not include threads, unlike pulley 76, since the tension in cable 99 allows the cable to grip pulley 100 tightly. In other embodiments, pulley 100 can be a threaded or unthreaded cylinder similar to capstan pulley 76 described with reference to FIG. 5.

Using the capstan drive mechanism, transducer 68 can translate linear axis member 40 along axis C when the pulley is rotated by the actuator of transducer 68. Likewise, when linear axis member 40 is translated along axis C by the user manipulating object 44, pulley 100 and shaft 98 are rotated; this rotation is detected by the sensor of transducer 68. The capstan drive mechanism provides low friction and smooth, rigid operation for precise movement of linear axis member 40 and accurate position measurement of the member 40.

Other drive mechanisms can also be used to transmit forces to linear axis member and receive positional information from member 40 along axis C. For example, a drive wheel

made of a rubber-like material or other frictional material can be positioned on shaft **98** to contact linear axis member **40** along the edge of the wheel. The wheel can cause forces along member **40** from the friction between wheel and linear axis member. Such a drive wheel mechanism is disclosed in the abovementioned application Ser. No. 08/275,12, now U.S. Pat. No. 5,623,582 well as in U.S. patent application Ser. No. 08/344,148, filed Nov. 23, 1994 and entitled "Method and Apparatus for Providing Mechanical I/O for Computer Systems Interfaced with Elongated Flexible Objects" assigned to the assignee of the present invention and incorporated herein by reference in its entirety. Linear axis member **40** can also be a single shaft in alternate embodiments instead of a dual part sleeve and shaft.

Referring to the cross sectional side view of member **40** and transducer **70** shown in FIG. *6b*, interior shaft **93** is positioned inside hollow exterior sleeve **91** and is rotatably coupled to sleeve **91**. A first end **107** of shaft **93** preferably extends beyond sleeve **91** and is coupled to object **44**. When object **44** is rotated about axis C, shaft **93** is also rotated about axis C in the fourth degree of freedom within sleeve **91**. Shaft **93** is translated along axis C in the third degree of freedom when sleeve **91** is translated. Alternatively, interior shaft **93** can be coupled to a shaft of object **44** within exterior sleeve **91**. For example, a short portion of shaft **28** of laparoscopic tool **18**, as shown in FIG. *1*, can extend into sleeve **91** and be coupled to shaft **93** within the sleeve, or shaft **28** can extend all the way to transducer **70** and functionally be used as shaft **93**.

Shaft **93** is coupled at its second end **109** to transducer **70**, which, in the preferred embodiment, is an optical encoder sensor. The housing **111** of transducer **70** is rigidly coupled to exterior sleeve **91** by a cap **115**, and a shaft **113** of transducer **70** is coupled to interior shaft **93** so that transducer **70** can measure the rotational position of shaft **93** and object **44**. In alternate embodiments, an actuator can also be included in transducer **70** to provide rotational forces about axis C to shaft **93**.

FIG. *7* is a perspective view of an alternate embodiment of the mechanical apparatus **25'** and user object **44** of the present invention. Mechanical apparatus **25'** shown in FIG. *7* operates substantially the same as apparatus **25'** shown in FIGS. *3* and *4*. User object **44**, however, is a stylus **102** which the user can grasp and move in six degrees of freedom. By "grasp", it is meant that users may releasably engage a grip portion of the object in some fashion, such as by hand, with their fingertips, or even orally in the case of handicapped persons. Stylus **102** can be sensed and force can be applied in various degrees of freedom by a computer system and interface such as computer **16** and interface **14** of FIG. *1*. Stylus **102** can be used in virtual reality simulations in which the user can move the stylus in 3D space to point to objects, write words, drawings, or other images, etc. For example, a user can view a virtual environment generated on a computer screen or in 3D goggles. A virtual stylus can be presented in a virtual hand of the user. The computer system tracks the position of the stylus with sensors as the user moves it. The computer system also provides force feedback to the stylus when the user moves the stylus against a virtual desk top, writes on a virtual pad of paper, etc. It thus appears and feels to the user that the stylus is contacting a real surface.

Stylus **102** preferably is coupled to a floating gimbal mechanism **104** which provides two degrees of freedom in addition to the four degrees of freedom provided by apparatus **25'** described with reference to FIGS. *3* and *4*. Floating gimbal mechanism **104** includes a U-shaped member **106** which is rotatably coupled to an axis member **108** by a shaft **109** so that U-shaped member **106** can rotate about axis F. Axis

member **108** is rigidly coupled to linear axis member **40**. In addition, the housing of a transducer **110** is coupled to U-shaped member **106** and a shaft of transducer **110** is coupled to shaft **109**. Shaft **109** is preferably locked into position within axis member **108** so that as U-shaped member **106** is rotated, shaft **109** does not rotate. Transducer **110** is preferably a sensor, such as an optical encoder as described above with reference to transducer **70**, which measures the rotation of U-shaped member **106** about axis F in a fifth degree of freedom and provides electrical signals indicating such movement to interface **14**.

Stylus **102** is preferably rotatably coupled to U-shaped member **106** by a shaft (not shown) extending through the U-shaped member. This shaft is coupled to a shaft of transducer **112**, the housing of which is coupled to U-shaped member **106** as shown. Transducer **112** is preferably a sensor, such as an optical encoder as described above, which measures the rotation of stylus **102** about the lengthwise axis G of the stylus in a sixth degree of freedom.

In the described embodiment of FIG. *7*, six degrees of freedom of stylus **102** are sensed. Thus, both the position (x, y, z coordinates) and the orientation (roll, pitch, yaw) of the stylus can be detected by computer **16** to provide a highly realistic simulation. Other mechanisms besides the floating gimbal mechanism **104** can be used to provide the fifth and sixth degrees of freedom. In addition, forces can be applied in three degrees of freedom for stylus **102** to provide 3D force feedback. In alternate embodiments, actuators can also be included in transducers **70**, **110**, and **112**. However, actuators are preferably not included for the fourth, fifth, and sixth degrees of freedom in the described embodiment, since actuators are typically heavier than sensors and, when positioned at the locations of transducers **70**, **100**, and **112**, would create more inertia in the system. In addition, the force feedback for the designated three degrees of freedom allows impacts and resistance to be simulated, which is typically adequate in many virtual reality applications. Force feedback in the fourth, fifth, and sixth degrees of freedom would allow torques on stylus **102** to be simulated as well, which may or may not be useful in a simulation.

FIG. *8* is a perspective view of a second alternate embodiment of the mechanical apparatus **25''** and user object **44** of the present invention. Mechanical apparatus **25''** shown in FIG. *8* operates substantially the same as apparatus **25'** shown in FIGS. *3* and *4*. User object **44**, however, is a joystick **112** which the user can preferably move in two degrees of freedom. Joystick **112** can be sensed and force can be applied in both degrees of freedom by a computer system and interface similar to computer system **16** and interface **14** of FIG. *1*. In the described embodiment, joystick **112** is coupled to cylindrical fastener **64** so that the user can move the joystick in the two degrees of freedom provided by gimbal mechanism **38** as described above. Linear axis member **40** is not typically included in the embodiment of FIG. *8*, since a joystick is not usually translated along an axis C. However, in alternate embodiments, joystick **112** can be coupled to linear axis member **40** similarly to stylus **102** as shown in FIG. *7* to provide a third degree of freedom. In yet other embodiments, linear axis member **40** can rotate about axis C and transducer **70** can be coupled to apparatus **25''** to provide a fourth degree of freedom. Finally, in other embodiments, a floating gimbal mechanism as shown in FIG. *7*, or a different mechanism, can be added to the joystick to allow a full six degrees of freedom.

Joystick **112** can be used in virtual reality simulations in which the user can move the joystick to move a vehicle, point to objects, control a mechanism, etc. For example, a user can view a virtual environment generated on a computer screen or

in 3D goggles in which joystick **112** controls an aircraft. The computer system tracks the position of the joystick as the user moves it around with sensors and updates the virtual reality display accordingly to make the aircraft move in the indicated direction, etc. The computer system also provides force feedback to the joystick, for example, when the aircraft is banking or accelerating in a turn or in other situations where the user may experience forces on the joystick or find it more difficult to steer the aircraft.

FIG. **9** is a schematic view of a computer **16** and an interface circuit **120** used in interface **14** to send and receive signals from mechanical apparatus **25**. Circuit **120** includes computer **16**, Interface card **120**, DAC **122**, power amplifier circuit **124**, digital sensors **128**, and sensor Interface **130**. Optionally included are analog sensors **132** instead of or in addition to digital sensors **128**, and ADC **134**. In this embodiment, the interface **14** between computer **16** and mechanical apparatus **25** as shown in FIG. **1** can be considered functionally equivalent to the interface circuits enclosed within the dashed line in FIG. **14**. Other types of interfaces **14** can also be used. For example, an electronic interface **14** is described in U.S. patent application Ser. No. 08/092,974, filed Jul. 16, 1993 and entitled "3-D Mechanical Mouse" assigned to the assignee of the present invention, which is the parent of file wrapper continuation application Ser. No. 08/461,170, now U.S. Pat. No. 5,576,727, and incorporated herein by reference in its entirety. The electronic interface described therein was designed for the Immersion PROBE.TM. 3-D mechanical mouse and has six channels corresponding to the six degrees of freedom of the Immersion PROBE.

Interface card **120** is preferably a card which can fit into an interface slot of computer **16**. For example, if computer **16** is an IBM AT compatible computer, interface card **14** can be implemented as an ISA or other well-known standard interface card which plugs into the motherboard of the computer and provides input and output ports connected to the main data bus of the computer.

Digital to analog converter (DAC) **122** is coupled to interface card **120** and receives a digital signal from computer **16**. DAC **122** converts the digital signal to analog voltages which are then sent to power amplifier circuit **124**. A DAC circuit suitable for use with the present invention is described with reference to FIG. **10**. Power amplifier circuit **124** receives an analog low-power control voltage from DAC **122** and amplifies the voltage to control actuators **126**. Power amplifier circuit **124** is described in greater detail with reference to FIG. **11**. Actuators **126** are preferably DC servo motors incorporated into the transducers **66a**, **66b**, and **68**, and any additional actuators, as described with reference to the embodiments shown in FIGS. **3**, **7**, and **8** for providing force feedback to a user manipulating object **44** coupled to mechanical apparatus **25**.

Digital sensors **128** provide signals to computer **16** relating the position of the user object **44** in 3D space. In the preferred embodiments described above, sensors **128** are relative optical encoders, which are electro-optical devices that respond to a shaft's rotation by producing two phase-related signals. In the described embodiment, sensor interface circuit **130**, which is preferably a single chip, receives the signals from digital sensors **128** and converts the two signals from each sensor into another pair of clock signals, which drive a bidirectional binary counter. The output of the binary counter is received by computer **16** as a binary number representing the angular position of the encoded shaft. Such circuits, or equivalent circuits, are well known to those skilled in the art; for example, the Quadrature Chip from Hewlett Packard, California performs the functions described above.

Analog sensors **132** can be included instead of digital sensors **128** for all or some of the transducers of the present invention. For example, a strain gauge can be connected to stylus **130** of FIG. **7** to measure forces. Analog sensors **132** provide an analog signal representative of the position of the user object in a particular degree of motion. Analog to digital converter (ADC) **134**, converts the analog signal to a digital signal that is received and interpreted by computer **16**, as is well known to those skilled in the art.

FIG. **10** is a schematic view of a DAC circuit **122** of FIG. **9** suitable for converting an input digital signal to an analog voltage that is output to power amplifier circuit **124**. In the described embodiment, circuit **122** includes a parallel DAC **136**, such as the DAC1220 manufactured by National Semiconductor, which is designed to operate with an external generic op amp **138**. Op amp **138**, for example, outputs a signal from zero to -5 volts proportional to the binary number at its input. Op amp **140** is an inverting summing amplifier that converts the output voltage to a symmetrical bipolar range. Op amp **140** produces an output signal between -2.5 V and $+2.5$ V by inverting the output of op amp **138** and subtracting 2.5 volts from that output; this output signal is suitable for power amplification in amplification circuit **124**. As an example, $R1=200$ k.OMEGA. and $R2=400$ k.OMEGA. Of course, circuit **122** is intended as one example of many possible circuits that can be used to convert a digital signal to a desired analog signal.

FIG. **11** is a schematic view of a power amplifier circuit **124** suitable for use in the interface circuit **14** shown in FIG. **9**. Power amplifier circuit receives a low power control voltage from DAC circuit **122** to control high-power, current-controlled servo motor **126**. The input control voltage controls a transconductance stage composed of amplifier **142** and several resistors. The transconductance stage produces an output current proportional to the input voltage to drive motor **126** while drawing very little current from the input voltage source. The second amplifier stage, including amplifier **144**, resistors, and a capacitor C, provides additional current capacity by enhancing the voltage swing of the second terminal **147** of motor **146**. As example values for circuit **124**, $R=10$ k.OMEGA., $R2=500$.OMEGA., $R3=9.75$ k.OMEGA., and $R4=1$.OMEGA. Of course, circuit **124** is intended as one example of many possible circuits that can be used to amplify voltages to drive actuators **126**.

While this invention has been described in terms of several preferred embodiments, it is contemplated that alterations, modifications and permutations thereof will become apparent to those skilled in the art upon a reading of the specification and study of the drawings. For example, the linked members of apparatus **25** can take a number of actual physical sizes and forms while maintaining the disclosed linkage structure. In addition, other gimbal mechanisms can also be provided with a linear axis member **40** to provide three degrees of freedom. Likewise, other types of gimbal mechanisms or different mechanisms providing multiple degrees of freedom can be used with the capstan drive mechanisms disclosed herein to reduce inertia, friction, and backlash in a system. A variety of devices can also be used to sense the position of an object in the provided degrees of freedom and to drive the object along those degrees of freedom. Furthermore, certain terminology has been used for the purposes of descriptive clarity, and not to limit the present invention. It is therefore intended that the following appended claims include all such alterations, modifications and permutations as fall within the true spirit and scope of the present invention.

What is claimed is:

1. An apparatus comprising:
a manipulandum configured as a surgical instrument;
a closed loop linkage system including a first central member fixedly coupled to a first object coupling and a second central member fixedly coupled to a second object coupling, wherein the first and second object couplings are separately coupled to the manipulandum to allow the manipulandum to be moveable in a plurality of rotary degrees of freedom and an axial degree of freedom;
a force feedback system coupled to the linkage system, wherein the force feedback system selectively applies resistive forces to the manipulandum based on the position of the manipulandum with respect to one or more reference coordinates.
2. The apparatus according to claim 1 wherein the manipulandum includes a grip portion and an elongated portion.
3. The apparatus according to claim 1 wherein the manipulandum is representative of a laparoscopic instrument.
4. The apparatus according to claim 1 wherein the manipulandum is representative of an endoscopic instrument.
5. The apparatus according to claim 1 wherein the manipulandum is representative of a catheter.
6. The apparatus according to claim 1 wherein the manipulandum is representative of a hypodermic needle.
7. The apparatus according to claim 1 wherein the force feedback system further comprises a sensor configured to detect movement of the manipulandum in at least one degree of freedom with respect to the one or more reference coordinates.
8. The apparatus according to claim 1 wherein the force feedback system further comprises an actuator configured to provide a force to the manipulandum in at least one degree of freedom in response to signals received from a computer system.
9. The apparatus according to claim 1 wherein the force feedback system inputs and receives signals from a simulation program in a computer system, the simulation program providing the one or more reference coordinates.
10. The apparatus according to claim 1 further comprising a capstan drive mechanism coupled to the linkage system, the capstan mechanism to facilitate a transmission of the feedback force from an actuator to the linkage system.
11. The apparatus according to claim 10 wherein the capstan mechanism further comprises
a capstan drum;
a pulley coupled to the capstan drum; and
a cable coupled to the capstan drum and in contact with the pulley.
12. The apparatus according to claim 1 wherein the force feedback system further comprises a sensor configured to detect movement of the manipulandum along at least one of the rotary degrees of freedom.
13. The apparatus according to claim 1 wherein the force feedback system further comprises a sensor configured to detect movement of the manipulandum along the axial degree of freedom.
14. A closed loop linkage system of an apparatus adapted to simulate a surgical instrument comprising:
a ground member;
first and second extension members in contact with the ground member;
a first central member coupled to the first extension member at a first end, the first central member including a first object coupling rigidly attached thereto at a second end, wherein the first object coupling is adapted to receive a portion of a manipulandum; and

- a second central member coupled to the second extension member at a first end, the second central member including a second object coupling rigidly attached thereto at a second end, wherein the second object coupling is coaxial with the first object coupling and is adapted to receive the portion of the manipulandum,
wherein the linkage system allows the manipulandum to be moveable in a plurality of rotary degrees of freedom and an axial degree of freedom.
15. The linkage system according to claim 14 wherein the manipulandum is representative of a laparoscopic instrument.
16. The linkage system according to claim 14 wherein the manipulandum is representative of an endoscopic instrument.
17. The linkage system according to claim 14 wherein the manipulandum is representative of a catheter.
18. The linkage system according to claim 14 wherein the manipulandum is representative of a hypodermic needle.
19. The linkage system according to claim 14, wherein the linkage system is coupled to a force feedback system, the force feedback system capable of selectively applying resistive forces based on the position of the received manipulandum with respect to one or more reference coordinates.
20. The linkage system according to claim 19 wherein the force feedback system further comprises a sensor adapted to detect movement of the manipulandum in at least one degree of freedom with respect to the one or more reference coordinates.
21. The linkage system according to claim 19 wherein the force feedback system further comprises an actuator adapted to provide a force to the manipulandum in at least one degree of freedom in response to signals received from a computer system.
22. The linkage system according to claim 19 wherein the force feedback system inputs and receives signals from a simulation program in a computer system, the simulation program providing the one or more reference coordinates.
23. The linkage system according to claim 14 further comprising a capstan drive mechanism coupled to the linkage system, the capstan mechanism facilitate a transmission of the feedback force from an actuator to the linkage system.
24. The linkage system according to claim 23 wherein the capstan mechanism further comprises
a capstan drum;
a pulley coupled to the capstan drum; and
a cable coupled to the capstan drum and in contact with the pulley.
25. The linkage system according to claim 19 wherein the force feedback system further comprises a sensor configured to detect movement of the manipulandum along at least one of the rotary degrees of freedom.
26. The linkage system according to claim 19 wherein the force feedback system further comprises a sensor configured to detect movement of the manipulandum along the axial degree of freedom.
27. An apparatus comprising:
a housing having an opening; and
an manipulandum configured to simulate a surgical instrument insertable in the opening, the implement capable of being manipulated axially and rotationally relative to the housing;
a frame assembly to restrict axial movement of the manipulandum along a predetermined axis;
a rotation sensor coupled to the manipulandum, wherein the rotation sensor monitors the axial rotation of the manipulandum relative to the housing;

21

a position sensor coupled to the manipulandum, wherein the position sensor monitors the axial position of the manipulandum along the predetermined axis;
a cable coupled to the manipulandum; and
a motor coupled to the cable, the motor capable of selectively applying a torque to the cable to apply a resistive force to the manipulandum along the predetermined axis
28. The apparatus according to claim **27** wherein the manipulandum is representative of a laparoscopic instrument.

22

29. The apparatus according to claim **27** wherein the manipulandum is representative of an endoscopic instrument.
30. The apparatus according to claim **27** wherein the manipulandum is representative of a catheter.
31. The apparatus according to claim **27** wherein the manipulandum is representative of a hypodermic needle.

* * * * *

专利名称(译)	腹腔镜模拟界面		
公开(公告)号	US7460104	公开(公告)日	2008-12-02
申请号	US11/041992	申请日	2005-01-26
[标]申请(专利权)人(译)	ROSENBERG LOUIS B		
申请(专利权)人(译)	ROSENBERG LOUIS B.		
当前申请(专利权)人(译)	Immersion公司		
[标]发明人	ROSENBERG LOUIS B		
发明人	ROSENBERG, LOUIS B.		
IPC分类号	G09G5/00 A61B19/00 A63F13/06 G05G9/047 G06F3/00 G06F3/01 G06F3/038 G09B9/28 G09B23/28 G09G5/08		
CPC分类号	A63F13/06 G05G9/047 G06F3/016 G06F3/0346 G06F3/03545 G06F3/0383 G09B9/28 G09B23/28 A61B19/26 A63F2300/1037 G05G9/04737 G05G2009/0474 G05G2009/04766 G06F2203/015 A61B90/50 A63F13/24 A63F13/285		
其他公开文献	US20050162383A1		
外部链接	Espacenet USPTO		

摘要(译)

一种装置，包括配置为手术器械的操作器；一种闭环连杆机构，包括固定连接于第一物体连接器的第一中心构件和固定连接于第二物体连接器的第二中心构件，其中第一和第二物体连接器分别连接于操作器以允许操作器连接可在多个旋转自由度和轴向自由度上移动；力反馈系统耦合到连杆系统，其中力反馈系统基于操作器相对于一个或多个参考坐标的位置选择性地施加阻力到操作器。在一个实施例中，力反馈系统包括致动器，以响应于从计算机系统接收的信号以至少一个自由度向操作器提供力。

