



US 20130245373A1

(19) **United States**

(12) **Patent Application Publication**  
**Okoniewski**

(10) **Pub. No.: US 2013/0245373 A1**  
(43) **Pub. Date: Sep. 19, 2013**

(54) **SEAL ANCHOR WITH NON-PARALLEL LUMENS**

(71) Applicant: **COVIDIEN LP**, Mansfield, MA (US)

(72) Inventor: **Gregory Okoniewski**, North Haven, CT (US)

(73) Assignee: **Covidien LP**, Mansfield, MA (US)

(21) Appl. No.: **13/891,717**

(22) Filed: **May 10, 2013**

**Related U.S. Application Data**

(63) Continuation of application No. 12/887,847, filed on Sep. 22, 2010.

(60) Provisional application No. 61/247,654, filed on Oct. 1, 2009.

**Publication Classification**

(51) **Int. Cl.**

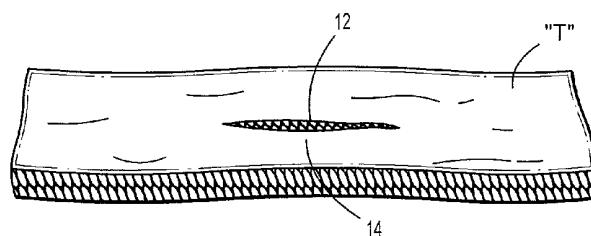
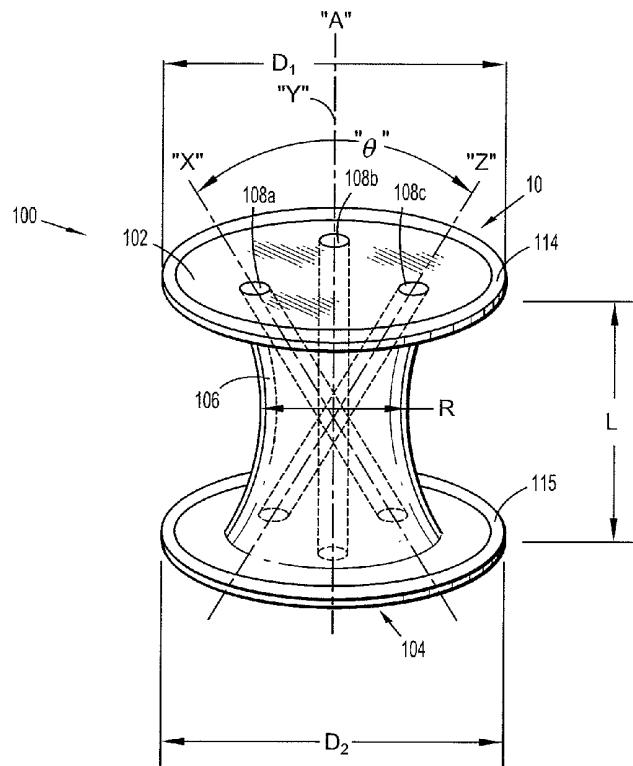
**A61B 17/02** (2006.01)

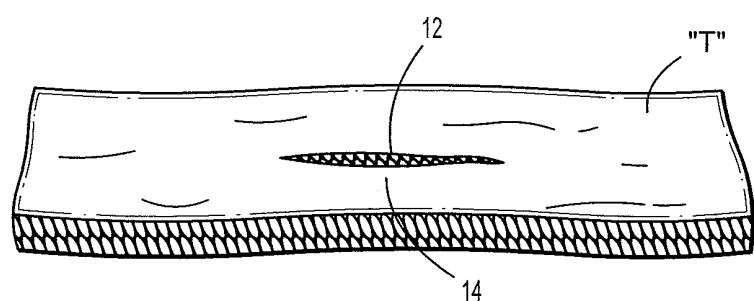
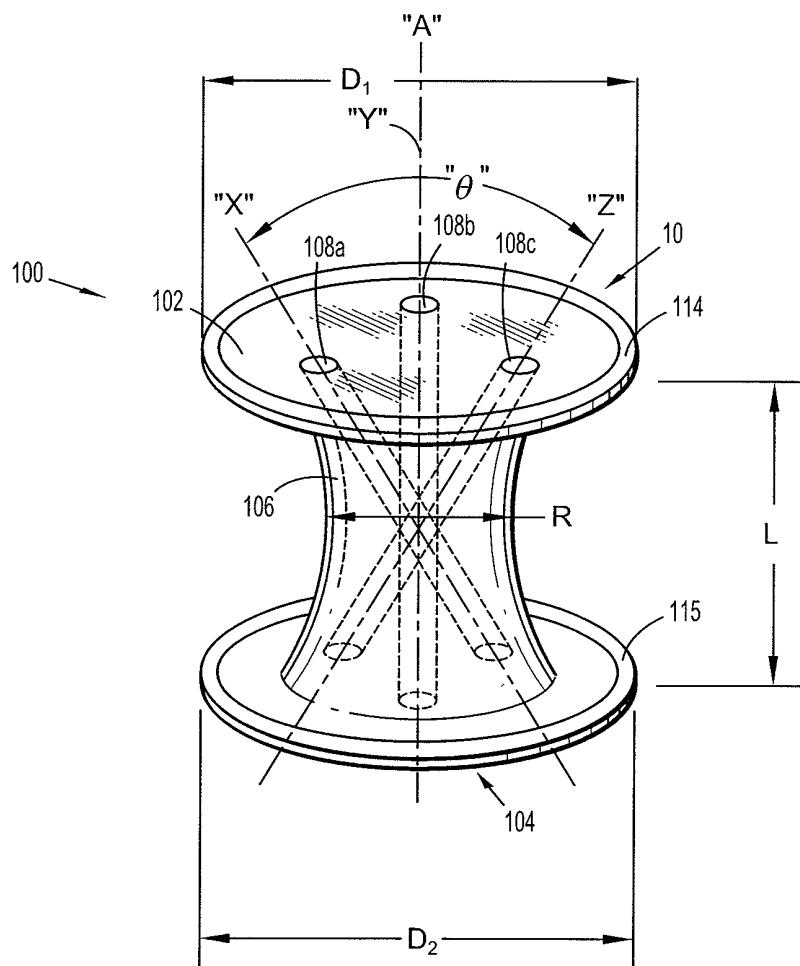
(52) **U.S. Cl.**

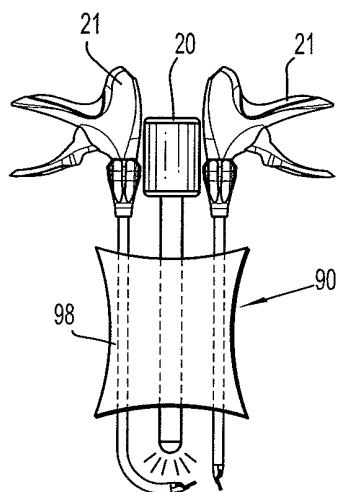
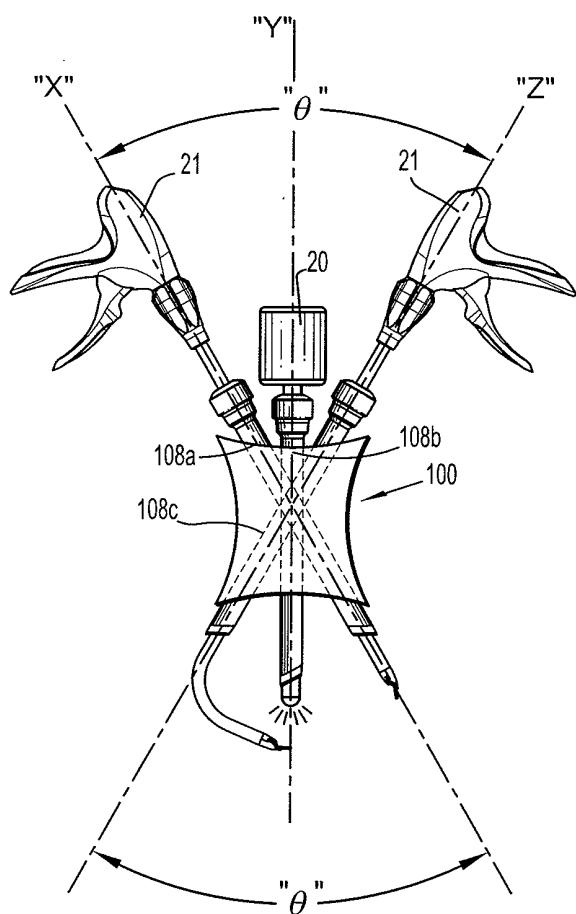
CPC ..... **A61B 17/0218** (2013.01)  
USPC ..... **600/109; 600/208**

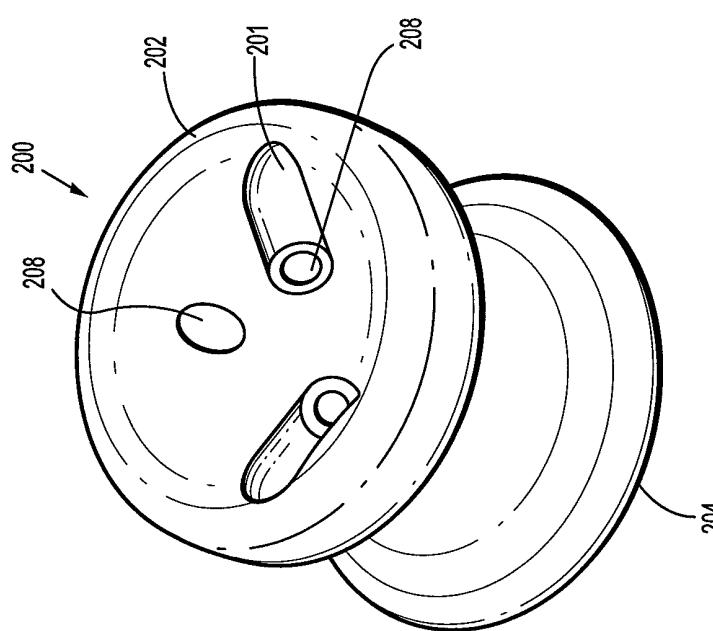
(57) **ABSTRACT**

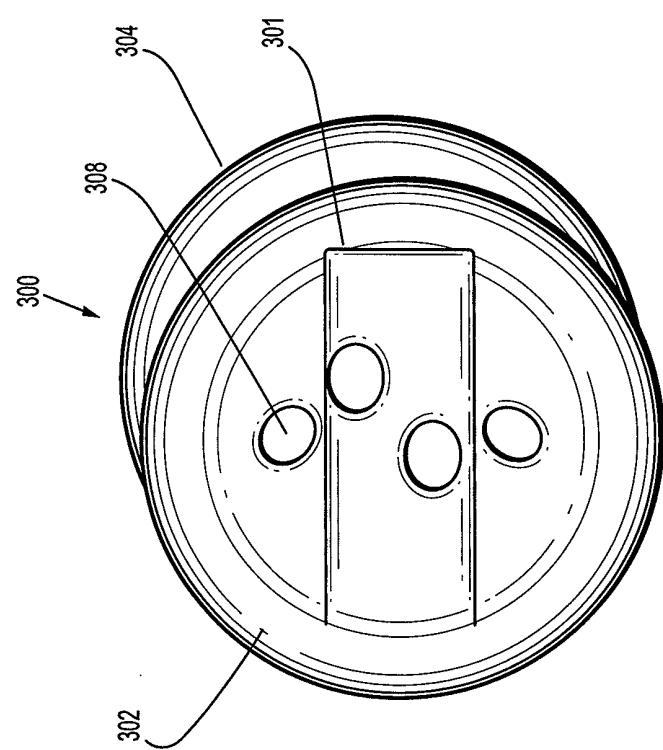
A seal anchor member defines a housing defining a longitudinal axis, the housing having leading and trailing ends, and including a plurality of lumens extending between the leading and trailing ends, each lumen being adapted for substantially sealed reception of an object therein and defining a longitudinal axis, wherein at least two of the lumens define longitudinal axes that are non-parallel to facilitate angled, at-rest placement of multiple instruments within the seal anchor member.



**FIG. 1**

**FIG. 2A****FIG. 2B**

**FIG. 3**

**FIG. 4**

## SEAL ANCHOR WITH NON-PARALLEL LUMENS

### CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 12/887,847, filed Sep. 22, 2010, which claims priority to, and benefit of, U.S. Provisional Application Ser. No. 61/247,654, filed Oct. 1, 2009, the disclosure of which is hereby incorporated by reference in its entirety.

### BACKGROUND

#### [0002] 1. Technical Field

[0003] The present disclosure relates to a seal for use in a surgical procedure. More particularly, the present disclosure relates to a seal anchor member adapted for insertion into an incision in tissue and including a plurality of non-parallel lumens adapted for the sealed reception of one or more surgical objects such that a substantially fluid-tight seal is formed with both the tissue and the surgical object or objects.

#### [0004] 2. Background of the Related Art

[0005] Today, many surgical procedures are performed through small incisions in the skin, as compared to the larger incisions typically required in traditional procedures, in an effort to reduce both trauma to the patient and recovery time. Generally, such procedures are referred to as "endoscopic", unless performed on the patient's abdomen, in which case the procedure is referred to as "laparoscopic". Throughout the present disclosure, the term "minimally invasive" should be understood to encompass both endoscopic and laparoscopic procedures.

[0006] During a typical minimally invasive procedure, surgical objects, such as surgical access devices (e.g., trocar and cannula assemblies) or endoscopes, are inserted into the patient's body through an incision in tissue. In general, prior to the introduction of the surgical object or instrument into the patient's body, insufflation gasses are used to enlarge the area surrounding the target surgical site to create a larger, more accessible work area. Accordingly, the maintenance of a substantially fluid-tight seal is desirable so as to prevent the escape of the insufflation gases and the deflation or collapse of the enlarged surgical site.

[0007] To this end, various valves and seals are used during the course of minimally invasive procedures and are widely known in the art. Various seals have been developed including lumens for the reception of surgical instruments. Depending upon the needs of a particular surgical procedure, instruments may need to be angled with respect to one another for extended periods of time. Holding the instruments at angles with respect to one another and/or overcoming the internal biases of the seal anchor member through which the instruments are inserted may fatigue the surgeon and/or breach the fluid-tight barrier between the seal anchor member and surrounding tissue.

[0008] Accordingly, a continuing need exists for new seal anchor members that can be inserted directly into the incision in tissue and that can accommodate a variety of surgical objects or instruments while maintaining the integrity of an insufflated workspace.

### SUMMARY

[0009] Disclosed herein is a seal anchor member including a housing including leading and trailing ends, and one or

more lumens extending therethrough. Each of the lumens is adapted for receiving a surgical instrument in a substantially sealed reception. The one or more lumens are angled with respect to a longitudinal axis of the housing. At least two of the lumens define axes that are non-parallel with respect to one another. In an embodiment, the housing may include a plurality of lumens, e.g., three lumens, in which one of the lumens is parallel with respect to the longitudinal axis and the other two lumens are non-parallel with respect to each other and the longitudinal axis. As described herein, the lumens, while defining axes that are intersecting, do not cross each other since the lumens are laterally spaced apart, e.g., the axes, not the lumens, are intersecting when the housing is viewed in a side cross-sectional view. This arrangement of the lumens facilitates the simultaneous, non-parallel placement of multiple surgical objects or instruments within the seal anchor member. However, in other embodiments, the lumens may be intersecting.

[0010] Furthermore, the lumens may define openings at the leading end that are radially spaced apart about the trailing end. Alternatively, the lumens may define openings at the leading end that are spaced along a diameter of the trailing end. The openings defined by the lumens may be staggered about an axis of the trailing end or may be positioned along a diameter but offset from that diameter. Alternatively, the openings defined by the lumens may be positioned on a chord or a diameter of the trailing end.

[0011] The housing may be formed from a compressible material to facilitate adjusting the angles between instruments inserted within the lumens and with respect to the longitudinal axis of the housing. In the absence of a force, e.g., a radial force, upon the instruments inserted within the lumens, the lumens are angled, i.e., non-parallel, with respect to each other. During use, the angles of the lumens are adjustable by applying a force.

[0012] The leading end may include a groove, cut-out, or recess that is positioned adjacent to the proximal end of at least one of the lumens. The groove is configured and adapted to facilitate the insertion of the instrument into the lumen by stabilizing the instrument and leading the instrument into the lumen. The groove may be generally arcuate. The groove may narrow from the proximal end to the distal end of the groove. The groove may extend radially outward from the proximal end of the at least one lumen.

[0013] Furthermore, the housing of the seal anchor may be adapted to transition between a first compressed condition to facilitate at least partial insertion of the seal anchor member within a tissue tract, and a second expanded condition to facilitate securing of the seal anchor member within the tissue tract and in substantial sealed relation with tissue surfaces defining the tissue tract. In an embodiment, the housing may be formed from a compressible material or from a foam material. In an embodiment, the foam material may be at least partially constituted of a material selected from the group consisting of polyisoprene, urethane, and silicone. In another embodiment, the housing may be formed from a gel material.

[0014] The housing may also define a substantially arcuate configuration. The housing may define a substantially hour glass shape. Furthermore, the lumens may define openings at the leading end that are radially spaced apart about the trailing end. Alternatively, the lumens may define openings at the leading end that are spaced along a diameter of the trailing end. The openings defined by the lumens may be staggered about an axis of the trailing end or may be positioned along a

diameter but offset from that diameter. Alternatively, the openings defined by the lumens may be positioned on a chord or a diameter of the trailing end.

[0015] These and other features of the apparatus disclosed herein will become more readily apparent to those skilled in the art from the following detailed description of various embodiments of the present disclosure.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0016] Various embodiments of the present disclosure are described hereinbelow with references to the drawings, wherein:

[0017] FIG. 1 is a front perspective view of a seal anchor in accordance with the present disclosure shown relative to tissue;

[0018] FIG. 2A is a front perspective view of a seal anchor member having lumens therein that are parallel to one another;

[0019] FIG. 2B is a front perspective view of the seal anchor of FIG. 1 shown with medical instruments inserted therein;

[0020] FIG. 3 is another embodiment of a seal anchor in accordance with the present disclosure; and

[0021] FIG. 4 is a yet another embodiment of a seal anchor in accordance with the present disclosure.

#### DETAILED DESCRIPTION OF THE EMBODIMENTS

[0022] In the drawings and in the description which follows, in which like references numerals identify similar or identical elements, the term "proximal" will refer to the end of the apparatus which is closest to the clinician during use, while the term "distal" will refer to the end which is furthest from the clinician, as is traditional and known in the art. A seal anchor for use in a surgical procedure is shown and described in U.S. Pat. Pub. 2009-0093752, the entire contents of which are hereby incorporated by reference. The seal anchor member may be used during a minimally invasive procedure in which the seal anchor is inserted into an incision. Alternatively, the seal anchor may be used through a naturally occurring opening (e.g., anus or vagina) or any incision in a patient's skin.

[0023] The use and function of seal anchor member 100 will be discussed during the course of a typical minimally invasive procedure. Initially, the peritoneal cavity (not shown) is insufflated with a suitable biocompatible gas such as, e.g., CO<sub>2</sub> gas, such that the cavity wall is raised and lifted away from the internal organs and tissue housed therein, providing greater access thereto. The insufflation may be performed with an insufflation needle or similar device, as is conventional in the art. Either prior or subsequent to insufflation, a tissue tract 12 is created in tissue "T", the dimensions of which may be varied dependent upon the nature of the procedure.

[0024] A seal anchor 100 will now be described with reference to FIGS. 1 and 2. The seal anchor 100 defines a longitudinal axis "A" and has respective trailing (or proximal) and leading (or distal) ends 102, 104 and an intermediate portion 106 disposed between the trailing and leading ends 102, 104. Seal anchor member 100 includes one or more lumens (or ports) 108a, 108b, 108c disposed between the trailing and leading ends 102, 104 that define corresponding longitudinal axes "X", "Y", "Z". As seen in FIG. 1, the axes

"X", "Y", "Z" defined by the lumens 108a, 108b, 108c, respectively, are non-parallel with respect to one another. To facilitate the simultaneous placement of instruments into each of the lumens 108a, 108b, 108c, the lumens 108a-c do not cross one another. The lumens 108a-c are laterally spaced apart such that, although the lumens 108a-c are angled with respect to one another, the lumens 108a-c do not intersect one another. In other embodiments, however, lumens may be arranged to cross one another. In contrast to seal anchor 100, a seal anchor 90 having parallel, non-intersecting lumens 98 is illustrated in FIG. 2A.

[0025] As seen in FIG. 2B, the lumens 108a-c are adapted to receive instrumentation therein in a substantially sealed manner. The lumens 108a-c are adapted to inhibit the escape of insufflation gasses within a body cavity with or without instrumentation being inserted therein. Accordingly, the lumens 108a-c have diameters that are adapted to contract in the absence of a surgical instrument inserted therein and are adapted to expand to accommodate instrumentation in a substantially sealed manner.

[0026] As shown in FIG. 2B, the instrumentation inserted within the lumens 108 may include, but are not limited to, a camera 20 that may be inserted within one of the lumens 108 and a pair of surgical instruments 21 that are inserted into two of the other lumens 108. Since the axes "X" and "Z" of the two lumens 108a, 108c, through which the pair of surgical instruments 21 are inserted, cross one another, the distance between the distal ends of the surgical instruments 21 is greater than it would be if the axes "X", "Z" were parallel to one another. Since the lumens 108a, 108c define non-parallel axes, manipulation of the surgical instruments 21 is facilitated since there is a lesser probability of the instruments 21 interfering with each other's use. Furthermore, since the at-rest state for the lumens 108a-c is at angles with respect to one another, surgeon fatigue is reduced for those procedures necessitating such positioning for an extended duration of time. Adjustment of the angles of the lumens with respect to one another is facilitated by overcoming the internal biasing force of the seal anchor member 100 by applying a radial force to the surgical instrumentation placed within the lumens 108a-c.

[0027] As previously discussed, FIG. 2A illustrates a seal anchor 90 including lumens 98 that are parallel to one another. Inserted within lumens 98 are surgical instruments 21 and camera 20. As seen in FIG. 2A, the parallel configuration of the lumens 98 hinder camera 20 in obtaining a clear view of the surgical site. It will be appreciated that the non-parallel, intersecting configuration of the lumens 108a-c of seal anchor 100 facilitate obtaining a lesser obstructed field of view than would be obtainable using seal anchor 90. In particular, as shown in FIG. 2B, axes "X" and "Z" define an angle "θ" therebetween. The greater the value of angle "θ", the lesser the probability of surgical instruments 21 obstructing the view of camera 20. Moreover, the greater the angle "θ", the lesser the probability of interference between instruments 21 during the procedure. In addition, the greater the angle "θ", the greater the number of internal structures included within the surgical field and within reach of instruments 21.

[0028] Proximal end 102 of seal anchor member defines a first diameter D<sub>1</sub> and distal end 104 defines a second diameter D<sub>2</sub>. In one embodiment of seal anchor member 100, the respective first and second diameters D<sub>1</sub>, D<sub>2</sub> of the proximal and distal ends 102, 104 are substantially equivalent, as seen in FIG. 1, although an embodiment of seal anchor member

**100** in which diameters  $D_1, D_2$  are different is also within the scope of the present disclosure. As depicted in FIG. 1, proximal and distal ends **102, 104** define substantially planar surfaces. However, embodiments are also contemplated herein in which either or both of proximal and distal ends **102, 104**, respectively, define surfaces that are substantially arcuate to assist in the insertion of seal anchor member **100** within a tissue tract **12** defined by tissue surfaces **14** and formed in tissue “T”, e.g., an incision, as discussed in further detail below.

**[0029]** Intermediate portion **106** defines a radial dimension “R” and extends longitudinally between proximal and distal ends **102, 104**, respectively, to define an axial dimension or length “L”. The radial dimension “R” of intermediate portion **106** varies along the axial dimension, or length, “L” thereof. Accordingly, seal anchor member **100** defines a cross-sectional dimension that varies along its length “L”, which facilitates the anchoring of seal anchor member **100** within tissue “T”, as discussed in further detail below. However, an embodiment of seal anchor member **100** in which the radial dimension “R” remains substantially uniform along the axial dimension “L” thereof is also within the scope of the present disclosure.

**[0030]** The radial dimension “R” of intermediate portion **106** is appreciably less than the respective diameters  $D_1, D_2$  of proximal and distal ends **102, 104** such that seal anchor member **100** defines an “hour-glass” shape or configuration to assist in anchoring seal anchor member **100** within tissue “T”, as discussed in further detail below. However, in an alternate embodiment, the radial dimension “R” of intermediate portion **106** may be substantially equivalent to the respective diameters  $D_1, D_2$  of proximal and distal ends **102, 104**. In cross section, intermediate portion **106** may exhibit any suitable configuration, e.g., substantially circular, oval or oblong.

**[0031]** The seal anchor **100** may be adapted to transition from an expanded condition to a compressed condition so as to facilitate the insertion and securement thereof within tissue tract **12** in tissue “T”. In the expanded condition, seal anchor **100** is at rest and the respective radial dimensions  $D_1, D_2$  of seal anchor **100**, as well as the radial dimension R of the intermediate portion **106** are such that the seal anchor **100** cannot be inserted within tissue tract **12**. However, the seal anchor **100** may transition to a compressed condition such that proximal and distal ends **102, 104**, as well as intermediate portion **106** are dimensioned for insertion into tissue tract **12**.

**[0032]** To facilitate the transition between an expanded and a compressed condition, the seal anchor **100** may be formed from a compressible material having an internal biasing force such that the seal anchor **100** will transition back to an expanded condition upon insertion of the seal anchor **100** within tissue tract **12**, thereby ensuring a seal between the seal anchor **100** and the tissue tract **12**. Seal anchor **100** may be formed from a shape memory material, a foam material, or a gel material, or the like, but may also be formed from other materials. In an embodiment, the seal anchor **100** may be formed from a material selected from the group consisting of polyisoprene, urethane, and silicone.

**[0033]** Positioning members **114, 115** of the trailing and leading ends **102, 104**, respectively, may engage the walls defining the body cavity of the tissue tract **12** to facilitate securement of seal anchor member **100** within the body tissue. For example, positioning member **114** at leading end **104** may engage the internal peritoneal wall and positioning

member **114** adjacent trailing end **102** may engage the outer epidermal tissue adjacent the incision **12** within tissue “T”. In another embodiment of seal anchor member **100**, one or more additional positioning members **114** may be associated with intermediate portion **106**.

**[0034]** The use and function of seal anchor member **100** will be discussed during the course of a typical minimally invasive procedure. Initially, the peritoneal cavity (not shown) is insufflated with a suitable biocompatible gas such as, e.g.,  $\text{CO}_2$  gas, such that the cavity wall is raised and lifted away from the internal organs and tissue housed therein, providing greater access thereto. The insufflation may be performed with an insufflation needle or similar device, as is conventional in the art. Either prior or subsequent to insufflation, a tissue tract **12** is created in tissue “T”, the dimensions of which may be varied dependent upon the nature of the procedure.

**[0035]** Different embodiments of seal anchors will be described with reference to FIGS. 2 and 3. Seal anchors **200, 300** are substantially similar to seal anchor **100**, except in the configuration of lumens and further include structures to stabilize instrumentation inserted within the lumens. Both seal anchor **200** and seal anchor **300**, shown in FIGS. 2 and 3, include lumens defining intersecting axes. Seal anchor **200** includes a trailing end **202** and a distal end **204**. A plurality of lumens **208** is disposed between the trailing and leading ends **202, 204**. Lumens **208** define openings in the trailing end **202** that are radially positioned along the trailing end **202**. A cut-out or groove **201** in the leading end extending outward from at least one lumen **208** facilitates stabilization of instrumentation inserted within the lumen **208**.

**[0036]** In an alternative embodiment, a seal anchor **300** including plurality of lumens disposed between leading and trailing ends **302, 304** is shown in FIG. 4. A cut-out or groove **301** in an arcuate or half-cylindrical configuration is disposed in the trailing end. At least one lumen **308** is disposed within the groove **301**. Groove **301** is adapted to facilitate stabilization of instrumentation inserted within the at least one of the lumens **308** that is disposed within the area defined by the groove **301**.

**[0037]** Although the illustrative embodiments of the present disclosure have been described herein with reference to the accompanying drawings, the above description, disclosure, and figures should not be construed as limiting, but merely as exemplifications of particular embodiments. It is to be understood, therefore, that the disclosure is not limited to those precise embodiments, and that various other changes and modifications may be effected therein by one skilled in the art without departing from the scope or spirit of the disclosure.

What is claimed is:

1. A surgical device comprising:  
a flexible seal anchor member defining a longitudinal axis,  
the seal anchor member including an arcuate distal surface and an arcuate proximal surface, the seal anchor member defining a substantially hour-glass shape when the seal anchor member is in an at-rest condition,  
the seal anchor member defining at least three lumens extending from the proximal surface and through the seal anchor member to the distal surface, the at least three lumens being configured for substantially sealed reception of a surgical object inserted therein, wherein each one of the at least three lumens define a longitudinal axis, and wherein, when the seal anchor member is in the

at-rest condition, at least two lumen cross one another when the seal anchor member is viewed from a side.

**2.** The surgical device of claim **1**, wherein, when the seal anchor member is in an at-rest state, the longitudinal axis of a first lumen of the at least three lumens is parallel relative to the longitudinal axis of the seal anchor member and the longitudinal axes of a second lumen and a third lumen of the at least three lumens are non-parallel relative to the longitudinal axis of the seal anchor member.

**3.** The surgical device of claim **2**, wherein the first lumen is configured for reception of a camera therein, and wherein the second and third lumen are configured for reception of a pair of surgical instruments that, from a side view of the seal anchor member, cross one another within the seal anchor member in the absence of a radial force being exerted on the pair of surgical instruments.

**4.** The surgical device of claim **1**, wherein the anchor seal member comprises at least one of a compressible or a shape memory material.

**5.** The surgical device of claim **1**, wherein the anchor seal member comprises a foam or a gel.

**6.** The surgical device of claim **1**, wherein a relative position of the at least three lumens are adjustable by a force exerted by a surgical instrument within one of the lumen.

**7.** The surgical device of claim **1**, wherein the seal anchor member is adapted to transition between a first condition in which at least a portion of the seal anchor member is insertable within an incision in an abdominal wall of a patient, and a second condition to facilitate securing the seal anchor member within the tissue tract and in substantial sealing relation with tissue surfaces defining the incision.

**8.** The surgical device of claim **1**, wherein the seal anchor member is configured for insertion into an incision during a laparoscopic surgical procedure, and wherein the at least three lumens are configured to inhibit the escape of insufflation gases from within a body cavity.

**9.** The surgical device of claim **8**, wherein the at least three lumens are configured to inhibit the escape of insufflation gases from within a body cavity with or without instrumentation being inserted therein.

**10.** A surgical device comprising:

a compressible seal anchor member defining a longitudinal axis, the seal anchor member including a leading end defining a distal surface, a trailing end defining a proximal surface, and an intermediate portion between the leading and trailing ends, each of the leading and trailing ends having a diameter that is greater than a diameter of the intermediate portion when the seal anchor member is in an at-rest condition,

the seal anchor member defining a plurality of ports extending through the leading end, the intermediate portion and the trailing end, at least two of the plurality of ports being configured for substantially sealed reception of an instrument therein, wherein at least two ports are straight within the seal anchor member and are non-parallel relative to each other and to the longitudinal axis when the seal anchor member is in the at-rest condition, and wherein the at least two ports, when the seal anchor member is viewed from the side, cross one another such that a pair of surgical instruments inserted within the at least two ports cross one another within the seal anchor member in the absence of a force being exerted on the pair of surgical instruments.

**11.** The surgical device of claim **10**, wherein the proximal and distal surfaces are arcuate.

**12.** The surgical device of claim **10**, wherein the compressible material comprises at least one of a foam and a gel.

**13.** The surgical device of claim **10**, wherein a position of the plurality of ports relative to each other is adjustable by a force exerted by at least one instrument when the instrument is within one of the plurality of ports.

**14.** The surgical device of claim **10**, wherein the seal anchor member is adapted to transition between a compressed condition to facilitate at least partial insertion of the seal anchor member within an incision in an abdominal wall of a patient, and an inserted condition to facilitate securing of the seal anchor member within the incision and in sealing relation with tissue surfaces defining the incision.

**15.** The surgical device of claim **10**, wherein the seal anchor member defines a substantially hour-glass shape.

**16.** The surgical device of claim **10**, wherein the seal anchor member is configured for reception of a camera there-through.

**17.** The surgical device of claim **10**, wherein the seal anchor member is configured for insertion into an incision during a minimally invasive surgical procedure, the seal anchor member inhibiting the escape of insufflation gases from within a body cavity.

**18.** A surgical device configured for insertion into an incision during a minimally invasive surgical procedure and to inhibit the escape of insufflation gases from within a body cavity, the surgical device comprising:

a seal anchor member defining a longitudinal axis, the seal anchor member including a leading end defining an arcuate distal surface and a trailing end defining an arcuate proximal surface, the seal anchor member defining a substantially hour-glass shape when the seal anchor member is in an at-rest condition,

the seal anchor member defining at least first, second and third lumens extending through the trailing and leading ends from the proximal surface to the distal surface, each one of the first, second and third lumens being configured for substantially sealed reception of an instrument therein,

wherein, when surgical instruments are in use within the lumen of the seal anchor member, each one of the first, second and third lumens define a longitudinal axis that is straight and that is non-parallel relative to each other, wherein the longitudinal axis of the first lumen is parallel relative to the longitudinal axis of the seal anchor member and is configured for reception of a camera therein, and wherein the longitudinal axes of the second and third lumens are non-parallel relative to the longitudinal axis of the seal anchor member and cross over each other when the seal anchor member is viewed from a side, the second and third lumens configured for reception of a pair of surgical instruments therein.

**19.** The surgical device of claim **18**, wherein, when the seal anchor member is viewed from the side, the longitudinal axes of the second and third lumens cross one another such that, in the absence of a radial force being exerted on a pair of surgical instruments inserted through the second and third lumen, the pair of surgical instruments cross one another within the seal anchor member.

**20.** The surgical device of claim **18**, wherein the seal anchor member is formed from a material that enables the seal anchor member to transition between a first condition in

which at least a portion of the seal anchor member is insertable within an incision in an abdominal wall, and a second condition in which at least a portion of the seal anchor member expands so as to be secured within the incision and so as to be in sealing relation with tissue surfaces defining the incision.

\* \* \* \* \*

专利名称(译)	用非平行流明密封锚		
公开(公告)号	<a href="#">US20130245373A1</a>	公开(公告)日	2013-09-19
申请号	US13/891717	申请日	2013-05-10
[标]申请(专利权)人(译)	柯惠有限合伙公司		
申请(专利权)人(译)	COVIDIEN LP		
当前申请(专利权)人(译)	COVIDIEN LP		
[标]发明人	OKONIEWSKI GREGORY		
发明人	OKONIEWSKI, GREGORY		
IPC分类号	A61B17/02		
CPC分类号	A61B17/3423 A61B17/3462 A61B17/3498 A61B2017/3429 A61B2017/3445 A61M2202/02 A61B2017/3492 A61B17/0218 A61M13/003 A61B2017/00238 A61B2017/3466 A61B17/0293		
优先权	61/247654 2009-10-01 US		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

### 摘要(译)

密封锚定构件限定了限定纵向轴线的壳体，壳体具有前端和尾端，并且包括在前端和尾端之间延伸的多个腔，每个腔适于基本上密封接收其中的物体并限定纵向。轴，其中至少两个管腔限定不平行的纵向轴线，以便于多个器械在密封锚固件内成角度的静止放置。

