



US 20060015161A1

(19) **United States**

(12) **Patent Application Publication**

Longo et al.

(10) **Pub. No.: US 2006/0015161 A1**

(43) **Pub. Date: Jan. 19, 2006**

(54) **INTERSTITIAL MICROWAVE ANTENNA
WITH LATERAL EFFECT FOR TISSUE
HYPERTERMIA IN MINIMAL INVASIVE
SURGERY**

(76) Inventors: **Ignio Longo**, Pisa (IT); **Nevio
Tosoratti**, Roma (IT)

Correspondence Address:
**DENNISON, SCHULTZ, DOUGHERTY &
MACDONALD**
1727 KING STREET
SUITE 105
ALEXANDRIA, VA 22314 (US)

(21) Appl. No.: **10/531,918**

(22) PCT Filed: **Oct. 9, 2003**

(86) PCT No.: **PCT/IB03/04459**

(30) **Foreign Application Priority Data**

Oct. 23, 2002 (IT) P12002A000059

Publication Classification

(51) **Int. Cl.**
A61F 2/00 (2006.01)
A61N 5/02 (2006.01)

(52) **U.S. Cl.** **607/101; 607/156**

(57) **ABSTRACT**

Application device (1), for example, a metal needle or a plastic catheter that has in the end portion (2) of the free end a gradually increasing thickness to form substantially a chute guide (3) which ends at a side opening (4) made on the application device (1). This way, an interstitial antenna (10) is obtained formed by a co-axial tube having an external conductor (7), by a dielectric layer (9) and by a central conductor (8) embedded in the dielectric layer (9) that insulates it from the external conductor (7). The antenna (10) can be put in a target tissue, along an actuation direction forming an angle α with the introduction direction. This way, the antenna (10) achieves an actual surface isothermal, i.e. a mass of tissue actually coagulated within a curved surface (13), since the tip of the application device (1) is connected electrically with the external conductor (7) and increases its area of action.

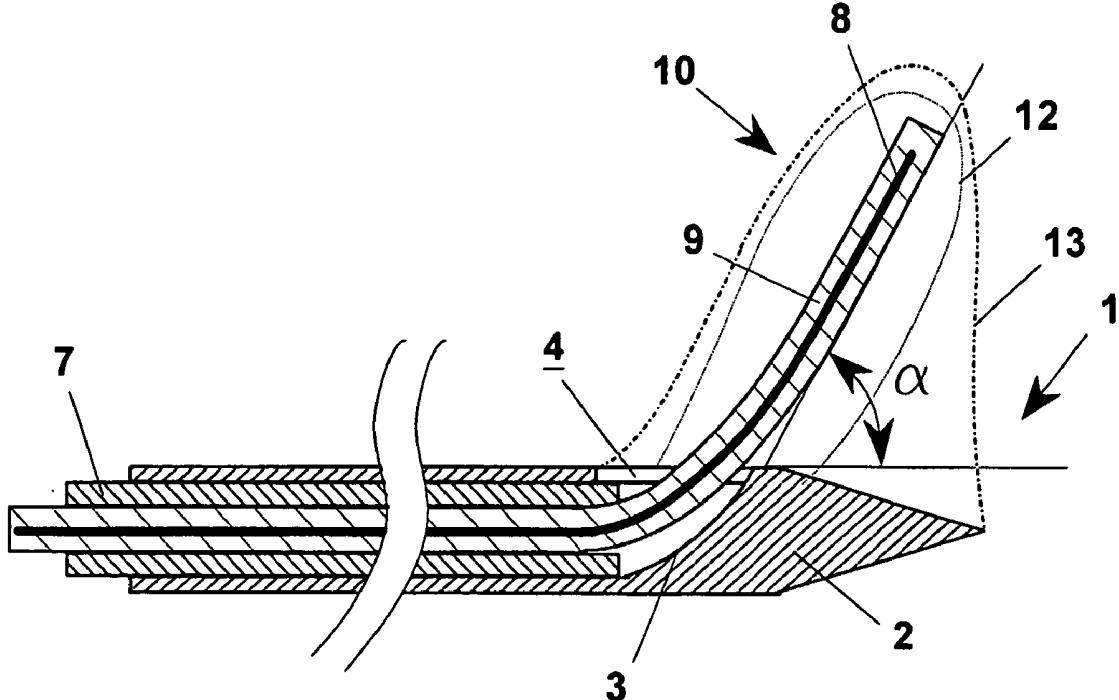


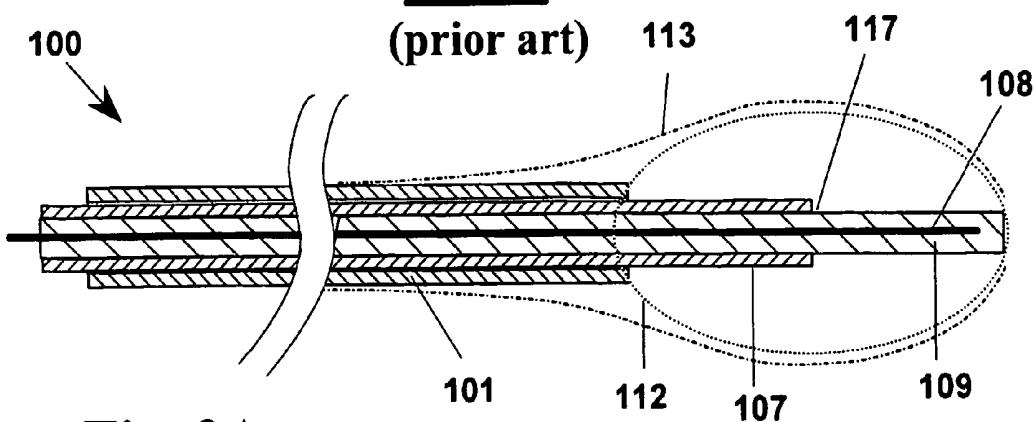
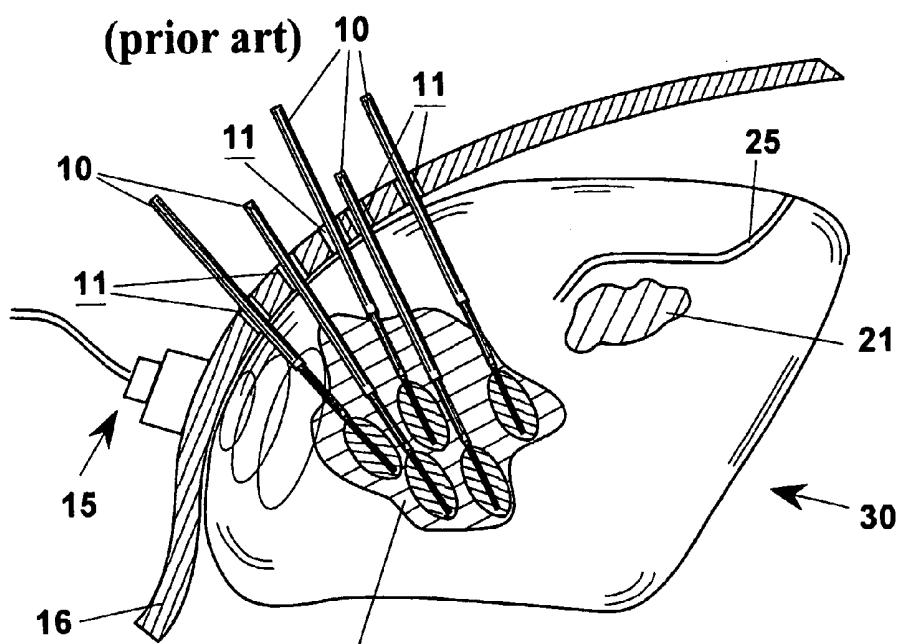
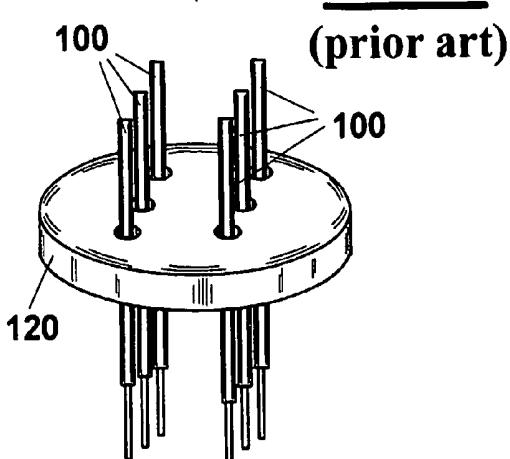
Fig. 1**Fig. 2A****Fig. 2B**

Fig. 3

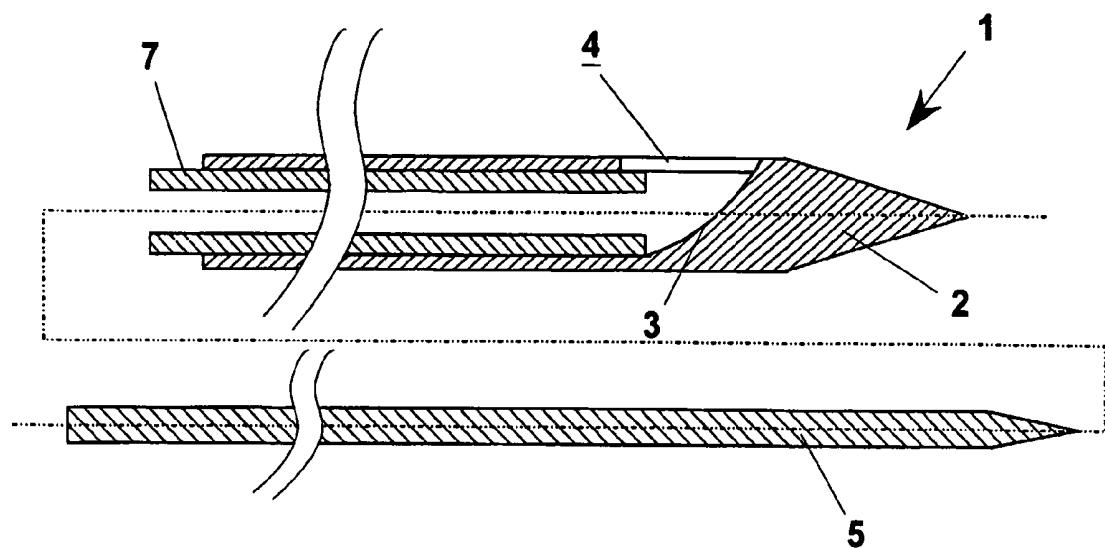


Fig. 4

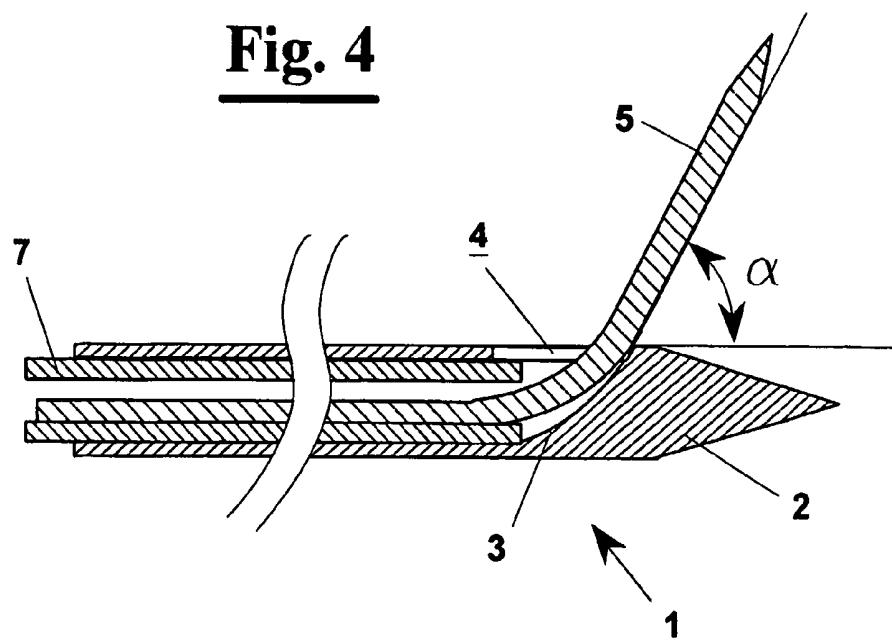


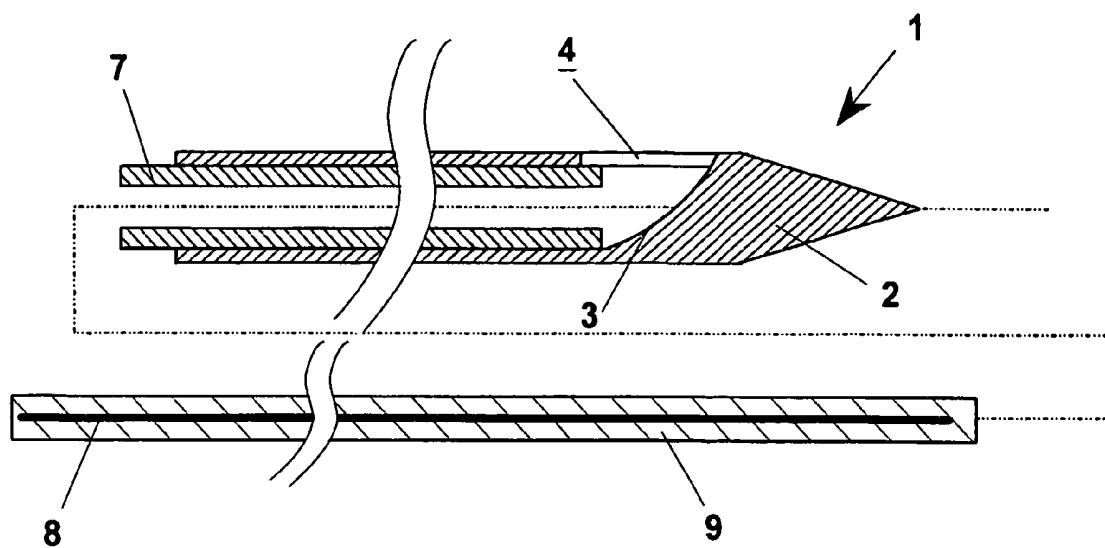
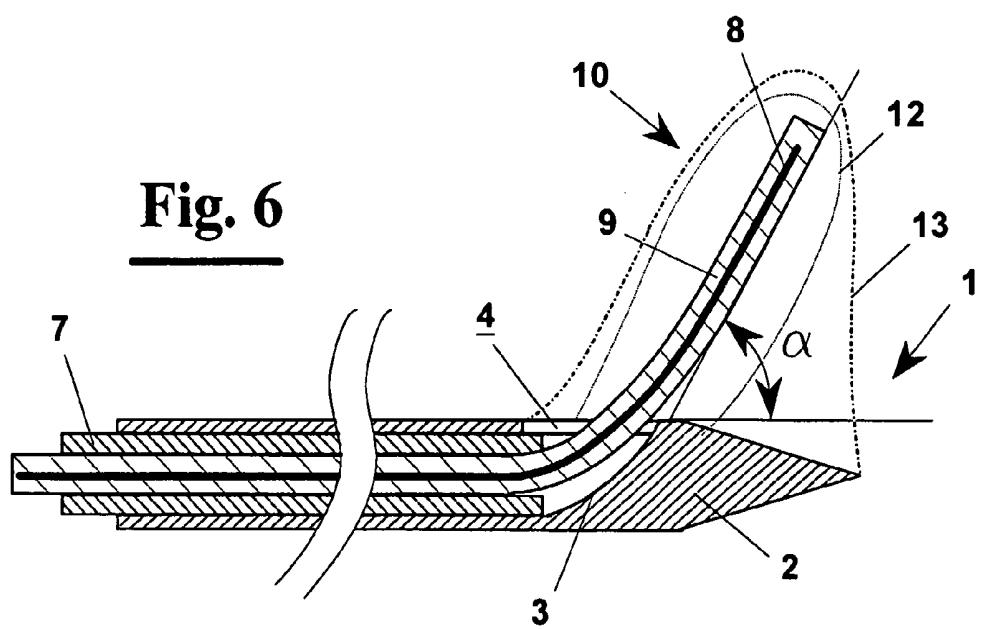
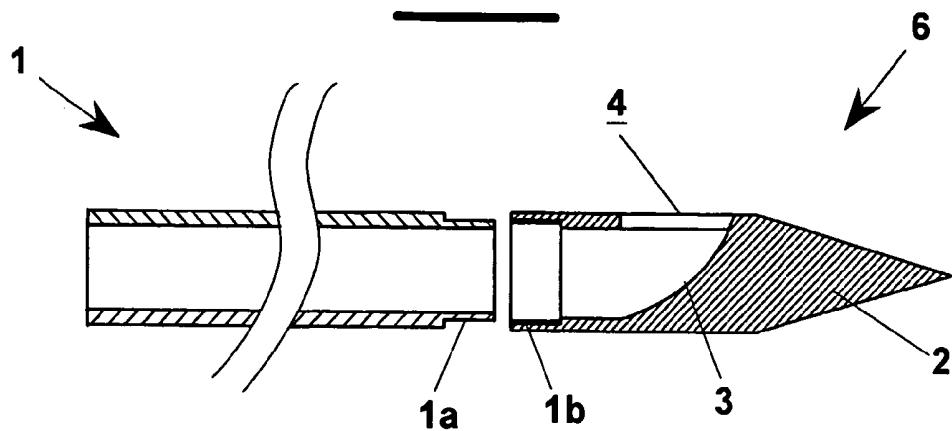
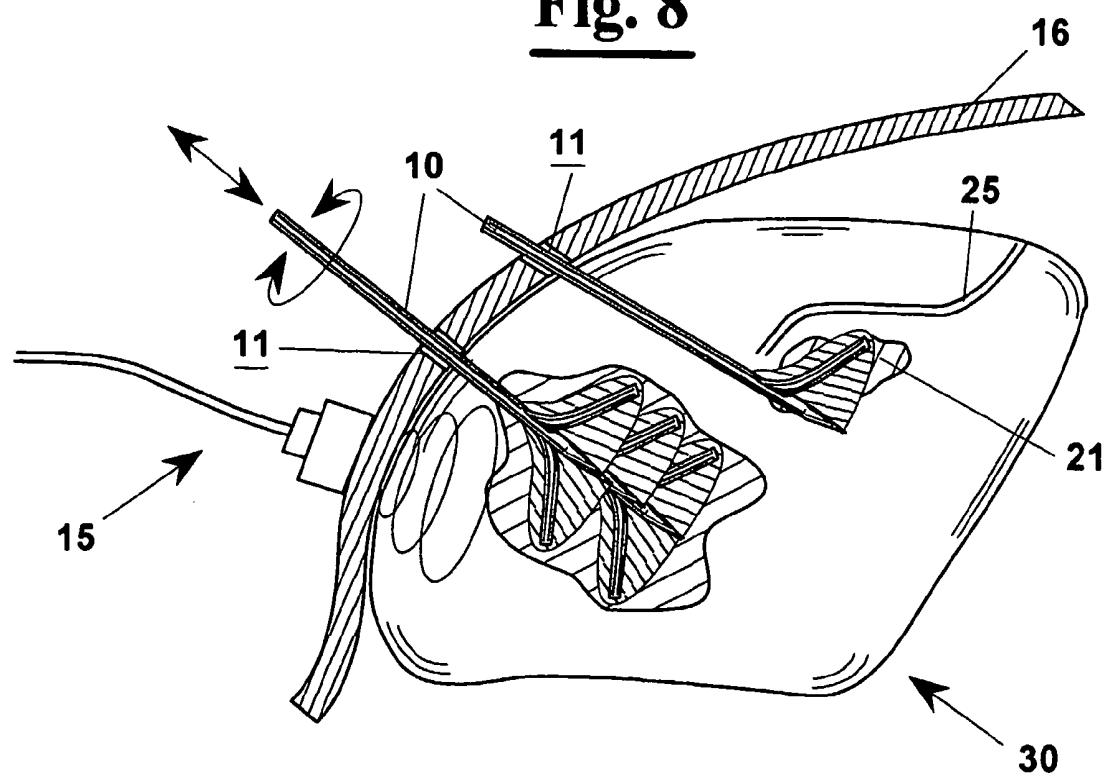
Fig. 5**Fig. 6**

Fig. 7**Fig. 8**

INTERSTITIAL MICROWAVE ANTENNA WITH LATERAL EFFECT FOR TISSUE HYPERHERMIA IN MINIMAL INVASIVE SURGERY

FIELD OF THE INVENTION

[0001] The present invention relates to minimally invasive surgery techniques, for hyperthermia of solid deep wounds for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, especially in oncology. More precisely, the present invention relates to a microwave co-axial antenna particularly indicated for hyperthermia of large tissue masses. Furthermore, the invention relates to a method for manufacturing such an antenna.

DESCRIPTION OF THE PRIOR ART

[0002] Hyperthermia in oncology is a method that has been used for over 30 years for treatment of cancer (Hahn GM, Hyperthermia and Cancer, Plenum Press, in the York, 1982). It consists in heating cancer cells to obtain their necrosis either directly or with additional use of other methods such as radiotherapy, chemotherapy or other surgery techniques.

[0003] For heating tissues, in particular for treatment of surface lesions, firstly electromagnetic waves have been used produced by a source located out of the human body.

[0004] More recently thin appliances have been used among which microwave antennas, operating between several hundreds of MHz and several thousands of MHz, typically at 2450 MHz, created with a co-axial tube, for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications, suitable for the local treatment of deep lesions (Iskander M F & Tumeh A M, Design Optimization of Interstitial Antennas, IEEE Transactions on Biomedical Engineering, 1989, 238-246).

[0005] Such antennas are usually inserted within the lesion to treat using catheters or metal needles, under computerised imaging techniques such as echographic guiding, TAC, NMR or other. They are suitable for being used in combination with other actions such as drugs, ionizing waves and/or surgery ablation.

[0006] These microwave antennas, normally, are manufactured using a flexible or semi-rigid co-axial tube, suitably modified at one end, for conveying microwave power into the tissues to cause hyperthermia.

[0007] The use of the minimally invasive microwaves coagulation therapy (TCMM) for percutaneous, laparoscopic applications, etc., is well known and widely documented in many industrial extra-European countries (USA, Japan, Canada, China, etc.).

[0008] Such therapy provides introducing a small diameter co-axial antenna up to directly the centre of a lesion, of cancerous or hypertrophic tissue, normally through an introduction metal needle or a plastic catheter.

[0009] In FIG. 1 an axial cross section is shown of an antenna 100 integrated with a biopsy needle 100 of known art. The active part of the antenna, in the right side of the drawing, is suitably configured as a radiating dipole or monopole. More precisely, 107 is the external conductor of the co-axial tube, 109 is the dielectric layer that insulates the

external conductor from the central conductor 108. Isothermal surfaces having a rotationally symmetric configuration can be obtained by heating a biological tissue (not crossed by large blood vessels) with a normal antenna 100, that for example is made by cutting at an end the portion of the external conductor 107 of the co-axial tube and leaving dielectric layer 109 uncovered as described in FIG. 1.

[0010] Once put within the lesion, the active end of the antenna exceeding the needle 101 emits microwave power (typically 60 W, at the frequency of 2450 MHz) sufficient to obtain in a few minutes the necrosis of a mass of tissue of spheroidal shape 112: for example, for coagulating 10 ml of aqueous tissue 2-3 minutes are required. The coagulative necrosis induced by the treatment destroys the tissue, which, normally, remains in its position where it is subject to a fibrotic process, it shrinks and does not affect further the adjacent zones. However, as the duration of the treatment and/or of the power supplied by the microwave antenna increase, the coagulated mass does not grow proportionally its volume, since the subtraction of heat by the blood circulation and by diffusion for conductivity increases proportionally to the surface of the treated volume: the consequence is that with an antenna of conventional type it is possible to treat, in a single application, lesions with a diameter not more than 2-3 cm.

[0011] With the existing technology, to treat lesions of larger diameter (>3 cm), the application has to be repeated through successive insertions of a single antenna 100 as shown in FIG. 2A, or the simultaneous introductions of several antennas 100. As shown in FIG. 2B, in this case the use is known of a multiple support 120 to guide together all the needles (as an array). In both cases, the traumatic aspects of the hyperthermia treatments and the soreness immediately felt by the patient increase substantially.

[0012] It must be noted that if a single TCMM application is sufficient for treatment of a lesion of 3 cm of diameter, a lesion of 8 cm of diameter requires between 20 and 30 single operations, considering a 1 cm overlap safety factor. Then, the use of an array of antennas is justified only if the lesion can be treated with not too many antennas, since otherwise the rate of invasiveness is, in fact, comparable to that of a conventional surgical operation, and the same happens in case of a treatment with a large number of consecutive insertions of a single applicator in different points.

[0013] Always as shown in FIG. 2A, by treating hepatic lesions in a percutaneous way using antenna 100 of conventional type, whereas lesion 20 can be treated even if requiring numerous insertions for coagulating the whole mass, it is not instead possible to treat lesion 21 next to a large blood vessel 25 for high risk of perforating or coagulating the vessel same.

[0014] Furthermore, lesions of irregular shape or that cannot be crossed longitudinally by the applicator are a further difficulty for conventional applicators presently in use.

SUMMARY OF THE INVENTION

[0015] It is a feature of the present invention to provide a microwave co-axial antenna for applications in medicine and surgery for further reducing treatment invasiveness of a minimally invasive microwaves coagulation therapy with

respect to the prior art, avoiding both a multiplication of the number of applications required for treating large lesions with a single antenna of conventional design (through repeated extraction and reintroduction of the applicator at different points of the tissue) both a requirement of an array of antennas.

[0016] It is also a feature of the present invention to provide an antenna that is inserted into a lesion and proceeds in a direction lateral/oblique with respect to the axis of the application needle and with an adjustable angle.

[0017] It is a further a feature of the present invention to provide a method for the production of such an antenna and of its application device.

[0018] These and other features are accomplished with one exemplary antenna for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, in species for applications of acute hypertermia in oncology, comprising:

[0019] an inner conductor,

[0020] a dielectric layer that covers the inner conductor for all its length,

[0021] an external conductor that covers coaxially the dielectric layer except from an end portion,

[0022] a tubular application device for coaxially guiding the antenna in a target tissue along an introduction direction,

[0023] whose characteristic is that the application device has in the end portion a side opening and a chute guide suitable for guiding the antenna through the side opening causing it to enter the target tissue, along an actuation direction forming an angle α with the application device same.

[0024] Preferably, the application device is a metal needle or a plastic catheter which, in the end portion, has a stiff blocking material, for example metal, having a tapered inner face forming said chute guide and a sharp external face.

[0025] Alternatively, the application device in the end portion has a gradually increasing thickness in order to form said chute guide.

[0026] Advantageously, for allowing the introduction of the antenna in the target tissue along the actuation direction a metal flexible mandrel is provided sliding in the application device before introducing the antenna and suitable for protruding from it through the side opening for making an inlet hole in the tissue to treat according to the actuation direction.

[0027] Once made the hole along the actuation direction, the mandrel is extracted from the application device and replaced by the co-axial antenna that is inserted in the hole made previously by the mandrel for a length suitable for allowing a correct operation. When the treated zone has reached a predetermined temperature, the antenna is withdrawn and can be inserted then in another position after having rotated the application device a certain angle or after having translated it along the introduction direction, without the need of making other inlet holes. This way, it is possible to apply hyperthermia to a mass of tissue having an axial symmetry or to masses of irregular shape.

[0028] Furthermore, such an antenna allows to heat lesions located laterally with respect to the application device without that these are necessarily crossed by the needle. This feature allows to treat lesions extending near large blood vessels, that cannot be treated with the antennas of prior art owing to a high risk of perforating the vessel.

[0029] In particular, it is possible to replace the needle with another having a different angle α for the actuation direction with respect to the introduction direction. Within certain limits, the length can also be changed of the portion of antenna exceeding the opening. This way, the shape of the area of operation can be changed as preferred.

BRIEF DESCRIPTION OF THE DRAWINGS

[0030] Further characteristics and advantages of the interstitial antenna, according to the present invention will be made clearer with the following description of an exemplary embodiment thereof, exemplifying but not limitative, with reference to the further attached drawings wherein:

[0031] FIGS. 3 and 4 show a cross sectional axial view of an application device for an interstitial antenna, according to the invention;

[0032] FIGS. 5 and 6 show in axial cross section an interstitial antenna, according to the invention;

[0033] FIG. 7 shows a cross sectional axial view of an alternative exemplary embodiment for the application device of FIG. 3;

[0034] FIG. 8 shows diagrammatically a possible use of the interstitial antenna of FIGS. 5 and 6.

DESCRIPTION OF A PREFERRED EXEMPLARY EMBODIMENT

[0035] In FIG. 3, an application device 1 according to the invention is shown, in an axial cross section, for example a metal needle or a plastic catheter that has in the end portion 2 of its free end a gradually increasing thickness to form substantially a chute guide 3 which ends at a side opening 4 made on application device 1. This way, an interstitial antenna 10 is obtained (FIG. 6) formed by a co-axial tube having an external conductor 7, by a dielectric cable 9 and by a central conductor 8 embedded in the dielectric cable 9 that insulates it from the external conductor 7. The antenna 10 can be put in a target tissue, along an actuation direction forming an angle α with the introduction direction.

[0036] With reference to FIG. 4, for allowing the introduction of cable 9 in the target tissue along the actuation direction a metal flexible mandrel is provided 5, suitably shaped, sliding in application device 1 and capable of protruding from it through the side opening 4 for making an inlet hole in the tissue to treat according to the actuation direction forming an angle α with the introduction direction.

[0037] Then, once made the hole along the actuation direction, the mandrel 5 is extracted from application device 1 and replaced by cable 9 that is inserted in the hole made previously by the mandrel 5 for a length suitable for allowing a correct operation (FIG. 6).

[0038] In particular, a calculated isothermal surface obtained by the antenna is indicated in FIG. 6 by a curved dashed line 12, whereas the actual isothermal surface, i.e.

the mass of tissue actually coagulated is enclosed within a curved line **13**, since the tip of application device **1** is connected electrically with the external conductor **7** and increases its area of action.

[0039] When the treated zone has reached a predetermined temperature, cable **9** is withdrawn and it can be put forward again after having rotated application device **1** of a certain angle or after having translated it along the introduction direction, without the need of making other inlet holes **11**, as shown in **FIG. 8**. It is sufficient to repeat the above operations with mandrel **5** and then cable **9**. This way, it is possible to reduce remarkably the treatment invasivity avoiding both to multiply the number of applications required for treating large lesions **20** with a single antenna **100** of conventional design (**FIG. 2A**) both to use an array of antennas (**FIG. 2B**), which requires a single hole but of much larger diameter.

[0040] Furthermore, the antenna **10**, according to the invention, allows to heat lesions located laterally with respect to application device **1** without that they are crossed by a hole. This feature allows to treat lesions **21** extending near a large blood vessel **25**, that cannot be treated with the antennas of prior art (**FIG. 2A**), for high risk of perforating the vessel **25** same.

[0041] In **FIG. 7** an alternative exemplary embodiment is shown for application device **1**. This embodiment provides that the metal needle or the plastic catheter **1** are associated to a block **6** of stiff material, for example metal, having a side opening **4**, a tapered inner face forming the chute guide **3** and a sharp external face. Needle **1** and block **6** are releasably engaged, for example, by a screw threaded coupling **1a-1b**. This way, it is possible to change as desired the shape of the area of operation simply replacing the block **6** for adjusting the angle α of the actuation direction with respect to the introduction direction.

[0042] The foregoing description of a specific embodiment will so fully reveal the invention according to the conceptual point of view, so that others, by applying current knowledge, will be able to modify and/or adapt for various applications such an embodiment without further research and without parting from the invention, and it is therefore to be understood that such adaptations and modifications will have to be considered as equivalent to the specific embodiment. The means and the materials to realise the different functions described herein could have a different nature without, for this reason, departing from the field of the

invention. It is to be understood that the phraseology or terminology employed herein is for the purpose of description and not of limitation.

1. Microwave device for interstitial, percutaneous, laparoscopic, endoscopic and intra-operation applications in medicine and surgery, in species for applications of acute hypertermia in oncology, comprising:

an inner conductor,

a dielectric layer that covers said inner conductor for all its length,

an external conductor that covers coaxially said dielectric layer except from an end portion, forming together with said dielectric layer and said inner conductor a co-axial antenna,

a tubular application device for coaxially guiding said antenna in a target tissue along an introduction direction,

characterised in that said application device has in the end portion a side opening and a chute guide, said chute guide guiding said antenna through said side opening causing it to enter the target tissue along an actuation direction that forms an angle α with respect to said application device.

2. Microwave device for interstitial applications, according to claim 1, wherein said application device is a metal needle or a plastic catheter which, in the end portion, has a stiff blocking material, for example metal, having a tapered inner face forming said chute guide and a sharp external face.

3. Microwave device for interstitial applications, according to claim 1, wherein said application device is a hollow needle, blind in the end portion and having said side opening, wherein at said side opening a gradually increasing thickness is provided in order to form said chute guide.

4. Microwave device for interstitial applications, according to claim 1, wherein for the introduction of the antenna in the target tissue along the actuation direction a metal flexible mandrel is provided sliding in said application device before introducing the antenna and suitable for protruding from it through said side opening for making an inlet hole in the tissue to treat according said actuation direction.

* * * * *

专利名称(译)	间质微波天线具有侧向作用的微创手术组织热疗		
公开(公告)号	US20060015161A1	公开(公告)日	2006-01-19
申请号	US10/531918	申请日	2003-10-09
[标]申请(专利权)人(译)	LONGO IGNIO TOSORATTI NEVIO		
申请(专利权)人(译)	LONGO IGNIO TOSORATTI NEVIO		
当前申请(专利权)人(译)	LONGO IGNIO TOSORATTI NEVIO		
[标]发明人	LONGO IGNIO TOSORATTI NEVIO		
发明人	LONGO, IGNIO TOSORATTI, NEVIO		
IPC分类号	A61F2/00 A61N5/02 A61B18/18		
CPC分类号	A61B18/18 A61B2018/183 A61B18/1815		
优先权	102002901056955 2002-10-23 IT		
外部链接	Espacenet USPTO		

摘要(译)

涂敷装置 (1) , 例如金属针或塑料导管 , 其在自由端的端部 (2) 中具有逐渐增加的厚度 , 以形成基本上在侧面开口处终止的斜槽引导件 (3) (4)) 在应用设备 (1) 上制作。这样 , 通过具有外部导体 (7) 的同轴管 , 通过介电层 (9) 和嵌入在介电层 (9) 中的中心导体 (8) 形成间隙天线 (10) 。使其与外部导体 (7) 绝缘。天线 (10) 可沿着与引入方向形成角度 α 的致动方向放入目标组织中。这样 , 由于施加装置 (1) 的尖端与外部导体 (7) 电连接 , 因此天线 (10) 实现了实际的表面等温 , 即在曲面 (13) 内实际凝结的大量组织。增加其行动领域。

