



US009833259B2

(12) **United States Patent**
McGinley et al.

(10) **Patent No.:** **US 9,833,259 B2**
(45) **Date of Patent:** ***Dec. 5, 2017**

(54) **SURGICAL ACCESS PORT**

(71) Applicant: **APPLIED MEDICAL RESOURCES CORPORATION**, Rancho Santa Margarita, CA (US)

(72) Inventors: **Kimball B. McGinley**, Rancho Santa Margarita, CA (US); **Henry Kahle**, Corona, CA (US); **Scott V. Taylor**, Rancho Santa Margarita, CA (US); **Gary M. Johnson**, Rancho Santa Margarita, CA (US)

(73) Assignee: **Applied Medical Resources Corporation**, Rancho Santa Margarita, CA (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 337 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **14/636,252**

(22) Filed: **Mar. 3, 2015**

(65) **Prior Publication Data**

US 2015/0173792 A1 Jun. 25, 2015

Related U.S. Application Data

(63) Continuation of application No. 13/872,340, filed on Apr. 29, 2013, now Pat. No. 8,968,250, which is a (Continued)

(51) **Int. Cl.**
A61B 17/34 (2006.01)
A61M 13/00 (2006.01)
(Continued)

(52) **U.S. Cl.**
CPC **A61B 17/3423** (2013.01); **A61B 17/0218** (2013.01); **A61B 17/3462** (2013.01);
(Continued)

(58) **Field of Classification Search**

CPC A61B 17/3462; A61B 17/3498; A61B 2017/3464; A61B 17/3423; A61B 17/34;
(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,100,482 A 8/1963 Hett
3,542,380 A 11/1970 Klein et al.
(Continued)

FOREIGN PATENT DOCUMENTS

EP 1 520 540 A1 4/2005
WO WO 94/19052 9/1994
(Continued)

OTHER PUBLICATIONS

European Patent Office, International Search Report and the Written Opinion for International Application No. PCT/US2006/060019, dated May 14, 2005.

(Continued)

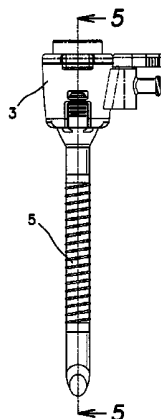
Primary Examiner — Aarti B Berdichevsky

(74) *Attorney, Agent, or Firm* — John F. Heal

(57) **ABSTRACT**

A surgical access port or trocar is provided. The trocar has a trocar seal housing and a trocar cannula with an optical obturator insertable through the trocar seal housing and the trocar cannula. The trocar is configured to access a body cavity, to maintain positive pressure and to prevent loss of surgical insufflation gas used in laparoscopic procedures. The trocar seal housing can be releasably attached to the trocar cannula. The trocar seal housing may also have a shield and/or alignment channel that provide protection or assist in operation of instrument and zero seals housed in the trocar seal housing.

8 Claims, 40 Drawing Sheets



Related U.S. Application Data

- continuation of application No. 11/549,926, filed on Oct. 16, 2006, now Pat. No. 8,430,851.
- (60) Provisional application No. 60/726,825, filed on Oct. 14, 2005, provisional application No. 60/828,515, filed on Oct. 6, 2006.
- (51) **Int. Cl.**
A61B 17/02 (2006.01)
A61B 17/00 (2006.01)
A61M 39/22 (2006.01)
- (52) **U.S. Cl.**
 CPC *A61M 13/003* (2013.01); *A61B 17/3417* (2013.01); *A61B 17/3474* (2013.01); *A61B 2017/0046* (2013.01); *A61B 2017/00477* (2013.01); *A61B 2017/347* (2013.01); *A61B 2017/3419* (2013.01); *A61B 2017/3464* (2013.01); *A61M 39/223* (2013.01); *A61M 2039/229* (2013.01)
- (58) **Field of Classification Search**
 CPC *A61B 2017/347*; *A61B 39/06*; *A61B 2039/0626*; *A61B 2039/0686*; *A61B 2039/0633*; *A61B 2039/229*
 See application file for complete search history.

References Cited

U.S. PATENT DOCUMENTS

3,613,684 A	10/1971	Sheridan	5,458,608 A	10/1995	Wortrich
4,147,184 A	4/1979	Jess	5,458,640 A	10/1995	Gerrone
4,180,542 A	12/1979	Wrasman	5,472,216 A	12/1995	Albertson et al.
4,576,589 A	3/1986	Kraus et al.	5,476,475 A	12/1995	Gadberry
4,655,752 A	4/1987	Honkanen et al.	5,492,304 A	2/1996	Smith et al.
5,043,126 A	8/1991	Thurau	5,496,280 A	3/1996	Vandenbroek et al.
5,053,016 A	10/1991	Lander	5,538,509 A	7/1996	Dunlap et al.
5,112,308 A	5/1992	Olsen et al.	5,545,142 A	8/1996	Stephens et al.
5,116,353 A	5/1992	Green	5,545,150 A	8/1996	Danks et al.
5,186,712 A	2/1993	Kelso et al.	5,549,583 A	8/1996	Sanford et al.
5,197,955 A	3/1993	Stephens et al.	5,554,124 A	9/1996	Alvarado
5,209,737 A	5/1993	Ritchart et al.	5,578,016 A	11/1996	Zinger
5,211,370 A	5/1993	Powers	5,584,850 A	12/1996	Hart et al.
5,224,930 A	7/1993	Spaeth et al.	5,591,192 A	1/1997	Privitera et al.
5,226,891 A	7/1993	Bushatz et al.	5,603,702 A	2/1997	Smith et al.
5,242,412 A	9/1993	Blake, III	5,607,440 A	3/1997	Danks et al.
5,261,888 A	11/1993	Semm	5,616,131 A	4/1997	Sauer et al.
5,273,545 A	12/1993	Hunt et al.	5,618,309 A	4/1997	Green et al.
5,290,245 A	3/1994	Dennis	5,628,732 A	5/1997	Antoon, Jr. et al.
5,295,993 A	3/1994	Green	5,643,301 A	7/1997	Mollenauer
5,300,035 A	4/1994	Clement	5,653,718 A	8/1997	Yoon
5,300,036 A	4/1994	Mueller et al.	5,657,963 A	8/1997	Hinchiffe et al.
5,308,336 A	5/1994	Hart et al.	5,658,306 A	8/1997	Kieturakis et al.
5,312,362 A	5/1994	Pfolsgraf et al.	5,662,615 A	9/1997	Blake, III
5,312,363 A	5/1994	Ryan et al.	5,685,820 A	11/1997	Riek et al.
5,330,497 A	7/1994	Freitas et al.	5,690,664 A	11/1997	Sauer et al.
5,334,150 A	8/1994	Kaali	5,709,664 A	1/1998	Vandenbroek et al.
5,342,315 A	8/1994	Rowe et al.	5,720,759 A	2/1998	Green et al.
5,354,280 A	10/1994	Haber et al.	5,722,958 A	3/1998	Gravener et al.
5,356,421 A	10/1994	Castro	5,727,770 A	3/1998	Dennis
5,360,417 A	11/1994	Gravener et al.	5,738,628 A	4/1998	Sierocuk et al.
5,372,588 A	12/1994	Farley et al.	5,792,113 A	8/1998	Kramer et al.
5,385,552 A	1/1995	Haber et al.	5,797,944 A	8/1998	Obles et al.
5,385,553 A	1/1995	Hart et al.	5,807,338 A	9/1998	Smith et al.
5,385,572 A	1/1995	Nobles et al.	5,817,061 A	10/1998	Goodwin et al.
5,391,153 A	2/1995	Haber et al.	5,820,604 A	10/1998	Fox et al.
5,407,433 A	4/1995	Loomas	5,820,606 A	10/1998	Davis et al.
5,411,483 A	5/1995	Loomas et al.	5,827,228 A	10/1998	Rowe
5,423,761 A	6/1995	Hein et al.	5,855,566 A	1/1999	Dunlap et al.
5,431,151 A	7/1995	Riek et al.	5,860,996 A	1/1999	Urban et al.
5,445,142 A	8/1995	Hassler, Jr.	5,865,812 A	2/1999	Correia
5,454,791 A	10/1995	Tovey et al.	5,871,471 A	2/1999	Ryan et al.
5,456,673 A	10/1995	Ziegler et al.	5,871,473 A	2/1999	Strauss et al.
			5,895,377 A	4/1999	Smith et al.
			5,928,208 A	7/1999	Chu et al.
			5,941,852 A	8/1999	Dunlap et al.
			5,989,224 A	11/1999	Exline et al.
			5,989,228 A	11/1999	Danks et al.
			6,003,553 A	12/1999	Wahlberg
			6,004,326 A	12/1999	Castro et al.
			6,017,356 A	1/2000	Frederick et al.
			6,036,711 A	3/2000	Mozdzierz et al.
			RE36,702 E	5/2000	Green et al.
			6,066,117 A	5/2000	Fox et al.
			6,083,203 A	7/2000	Yoon
			6,099,505 A	8/2000	Ryan et al.
			6,123,689 A	9/2000	To et al.
			6,196,967 B1	3/2001	Lim et al.
			6,197,002 B1	3/2001	Peterson
			6,203,557 B1	3/2001	Chin
			6,206,875 B1	3/2001	Long et al.
			6,228,061 B1	5/2001	Flatland et al.
			6,258,065 B1	7/2001	Dennis et al.
			6,270,454 B1	8/2001	Sano et al.
			6,340,358 B1	1/2002	Bohannon et al.
			6,423,036 B1	7/2002	Van Huizen
			6,482,181 B1	11/2002	Racenet et al.
			6,497,716 B1	12/2002	Green et al.
			6,569,119 B1	5/2003	Haberland et al.
			6,569,120 B1	5/2003	Green et al.
			6,589,212 B1	7/2003	Navis
			6,595,946 B1	7/2003	Pasqualucci
			6,656,198 B2	12/2003	Tsonton et al.
			6,685,630 B2	2/2004	Sauer et al.
			6,695,815 B2	2/2004	Moening
			6,695,816 B2	2/2004	Cassidy, Jr.
			6,702,787 B2	3/2004	Pasqualucci et al.
			6,726,663 B1	4/2004	Dennis
			6,811,546 B1	11/2004	Callas et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,860,869	B2	3/2005	Dennis	
6,923,783	B2	8/2005	Pasqualucci	
6,938,902	B2	9/2005	Devers	
6,942,671	B1	9/2005	Smith	
6,981,966	B2	1/2006	Green et al.	
7,056,303	B2	6/2006	Dennis et al.	
7,083,626	B2	8/2006	Hart et al.	
7,390,317	B2	6/2008	Taylor et al.	
7,717,878	B2	5/2010	Smith	
7,984,730	B2	7/2011	Ziv et al.	
8,968,250	B2 *	3/2015	McGinley A61B 17/3462 604/167.06
2002/0010424	A1	1/2002	Dennis et al.	
2003/0004529	A1	1/2003	Tsonton et al.	
2003/0040711	A1	2/2003	Racenet et al.	
2003/0060770	A1	3/2003	Wing et al.	
2003/0066978	A1	4/2003	Enerson	
2004/0068232	A1	4/2004	Hart et al.	
2004/0106942	A1	6/2004	Taylor	
2004/0147809	A1	7/2004	Kazakevich	
2004/0158126	A1	8/2004	Sauer et al.	
2004/0167473	A1	8/2004	Moening	
2004/0171990	A1	9/2004	Dennis et al.	
2004/0204682	A1	10/2004	Smith	
2004/0210162	A1	10/2004	Wyatt et al.	
2004/0230161	A1	11/2004	Zeiner	
2004/0260244	A1	12/2004	Piechowicz et al.	

2005/0033342	A1	2/2005	Hart et al.
2005/0065475	A1	3/2005	Hart et al.
2005/0065543	A1	3/2005	Kahle et al.
2005/0070850	A1	3/2005	Albrecht
2005/0070851	A1	3/2005	Thompson et al.
2005/0070947	A1	3/2005	Franer et al.
2005/0131349	A1	6/2005	Albrecht et al.
2005/0209608	A1	9/2005	O'Heeron
2005/0212221	A1	9/2005	Smith et al.
2005/0251191	A1	11/2005	Taylor et al.
2008/0077169	A1	3/2008	Taylor et al.
2011/0233435	A1	9/2011	Matsumoto et al.

FOREIGN PATENT DOCUMENTS

WO	WO 2004/032770	4/2004
WO	WO 2005/007024 A2	1/2005

OTHER PUBLICATIONS

European Patent Office, Invitation to Pay Additional Fees and Communication Relating to the Results of the Partial International Search for International Application No. PCT/US2006/060019 dated Mar. 13, 2007.

European Patent Office, European Search Report for European Patent Application No. 08 16 5292, titled Surgical Access Port, dated Jul. 1, 2009.

* cited by examiner

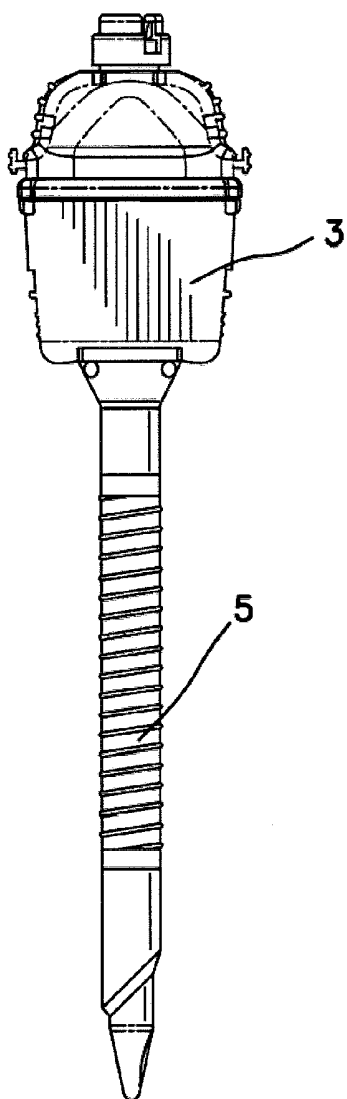


FIG. 1

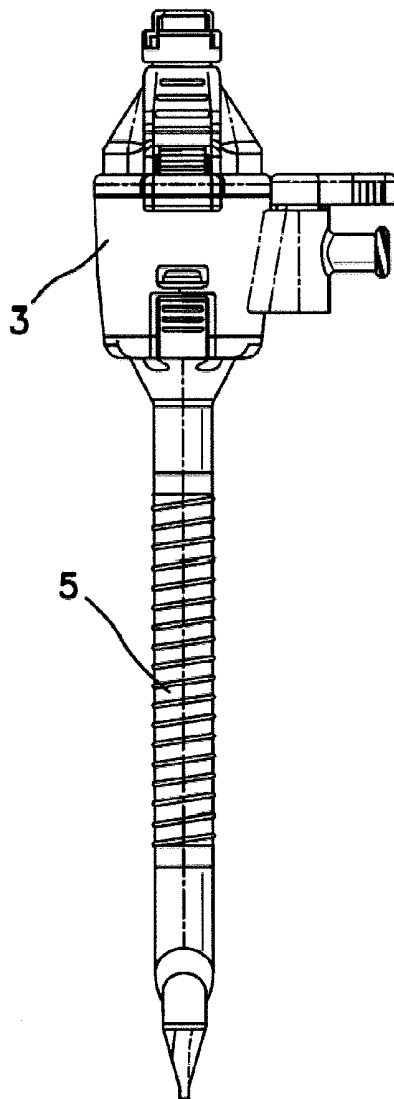


FIG. 2

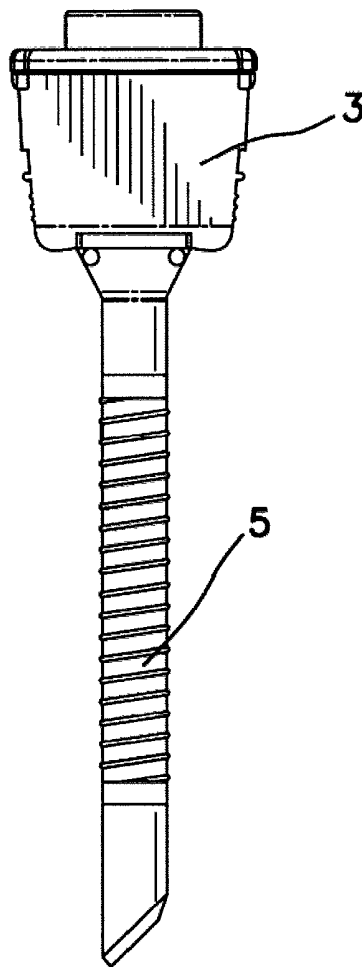


FIG. 3

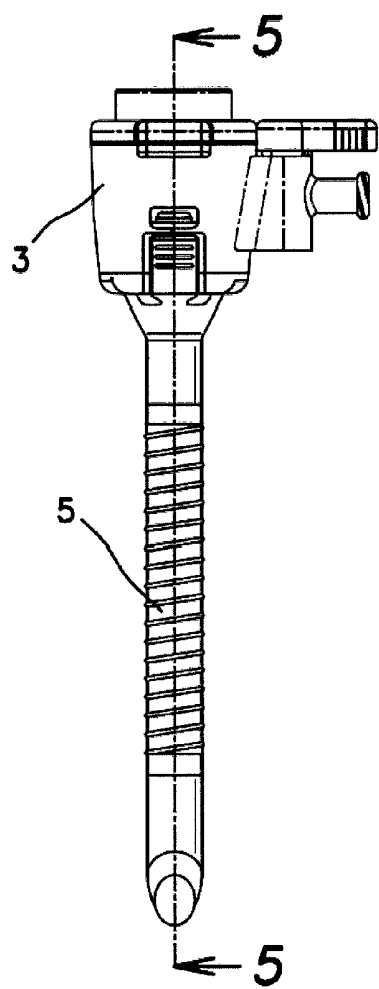


FIG. 4

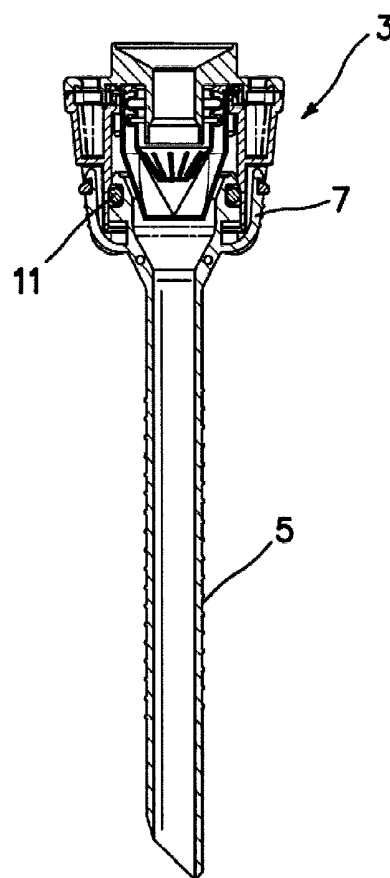
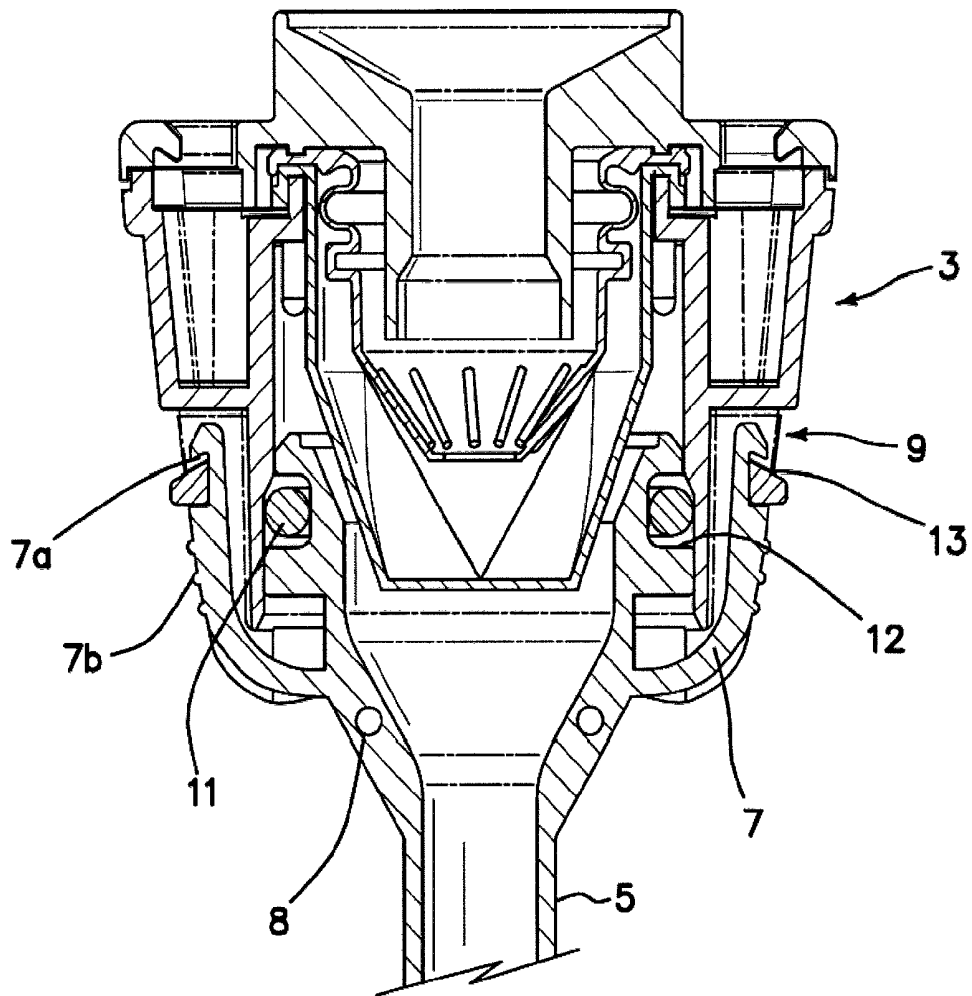


FIG. 5

**FIG. 6**

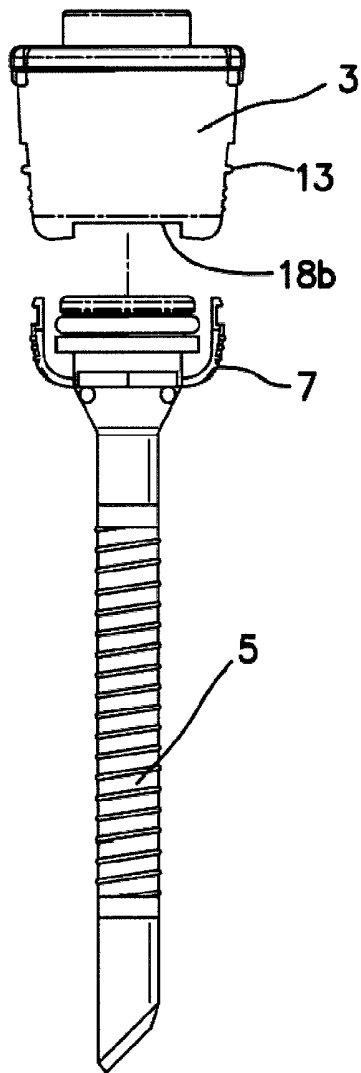


FIG. 7

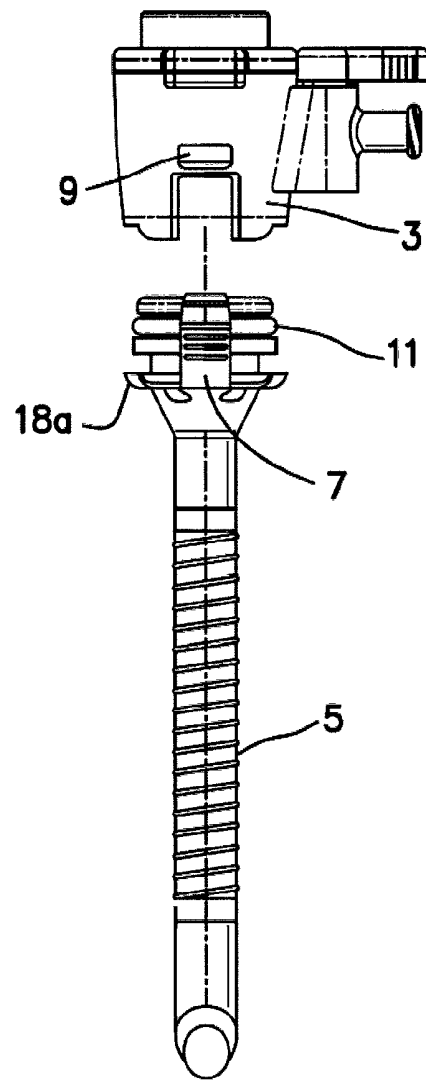


FIG. 8

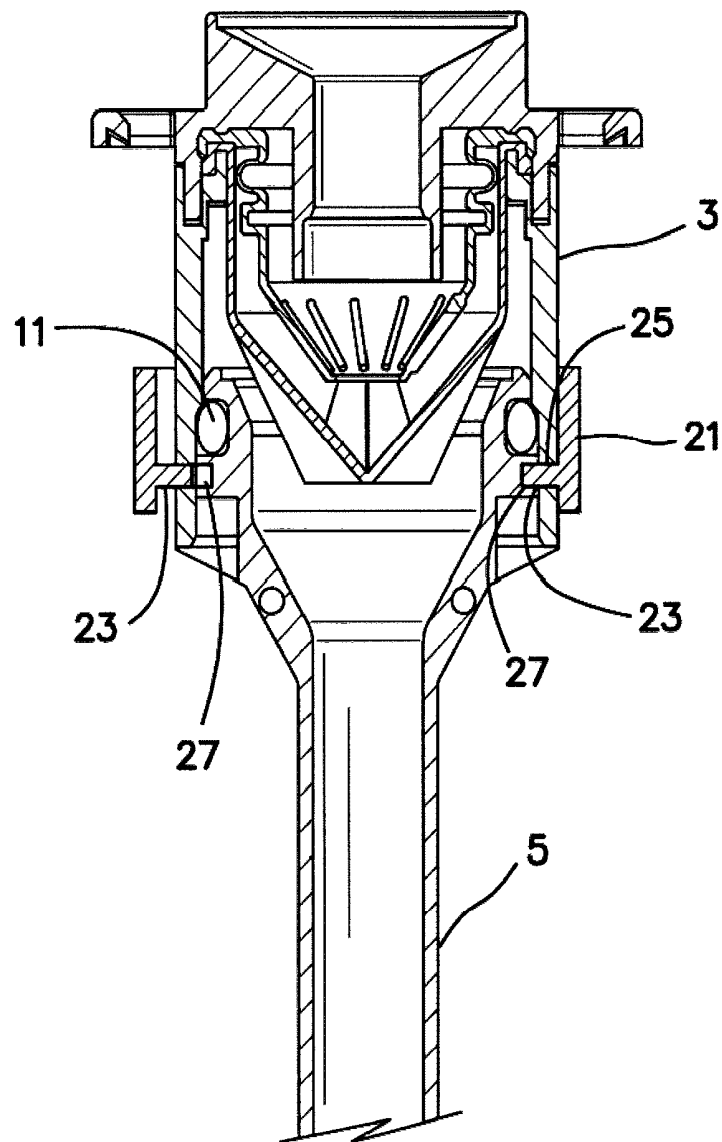
**FIG. 9**

FIG. 10

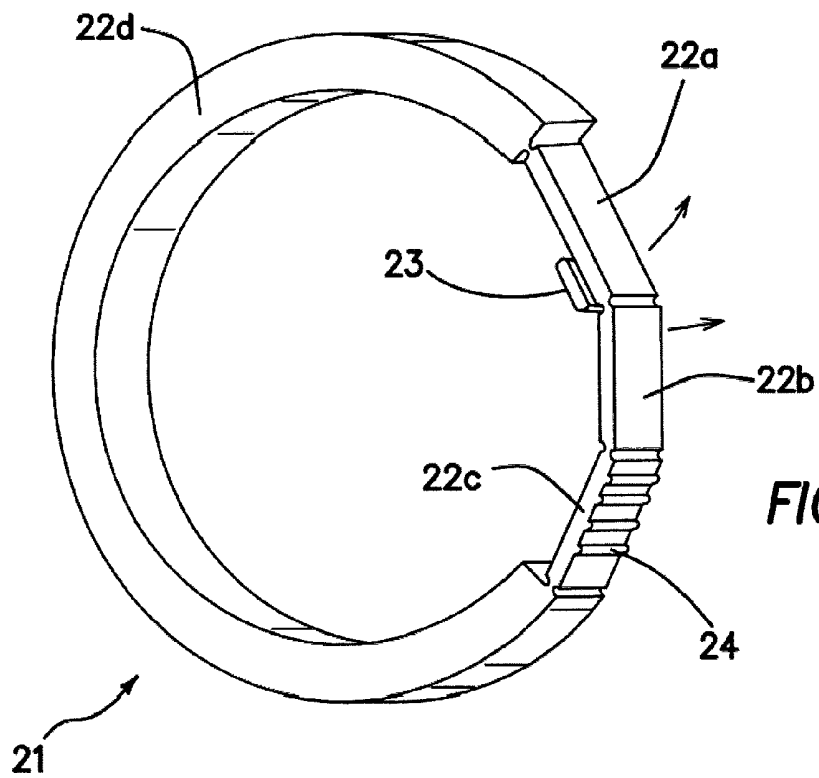
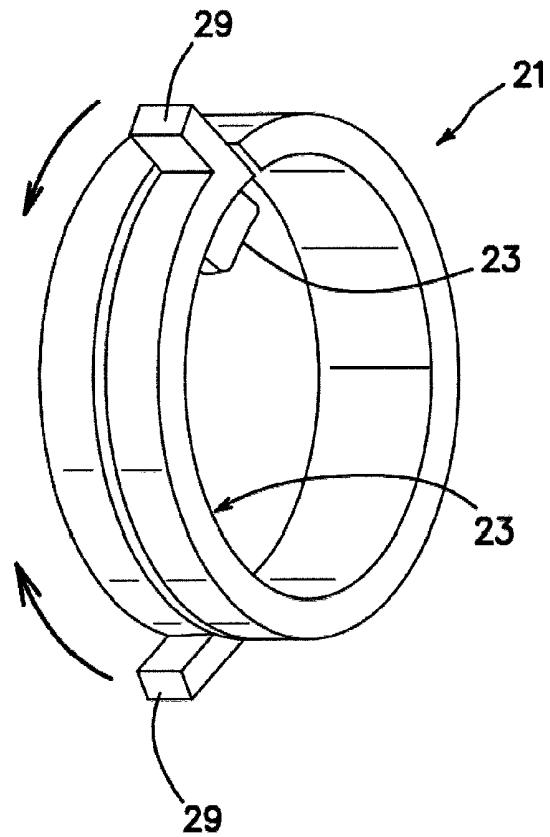
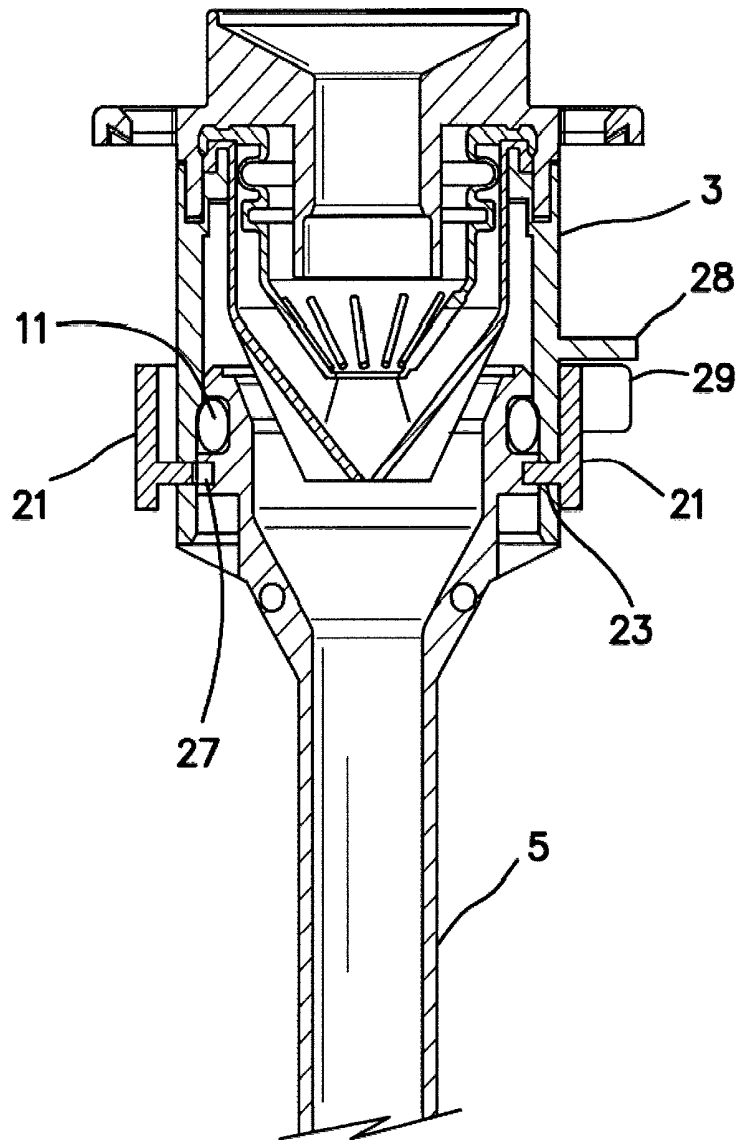


FIG. 12

**FIG. 11**

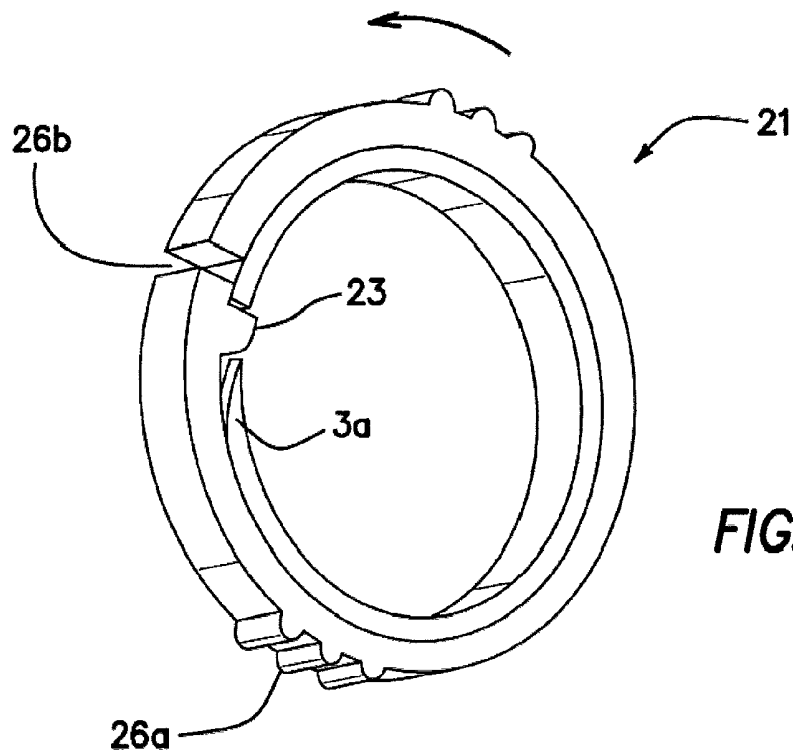


FIG. 13

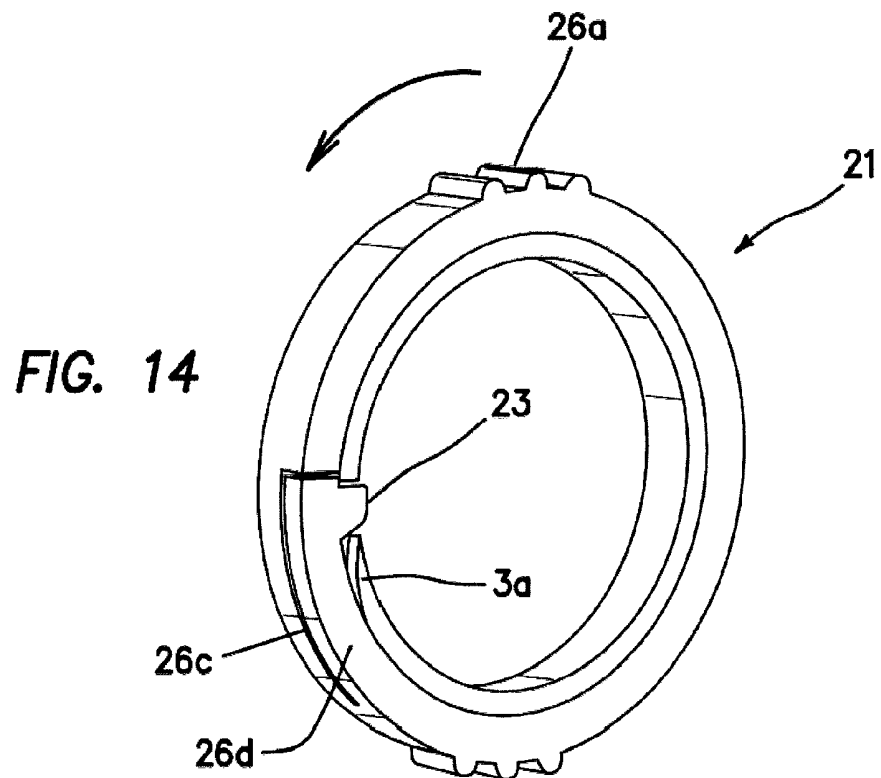
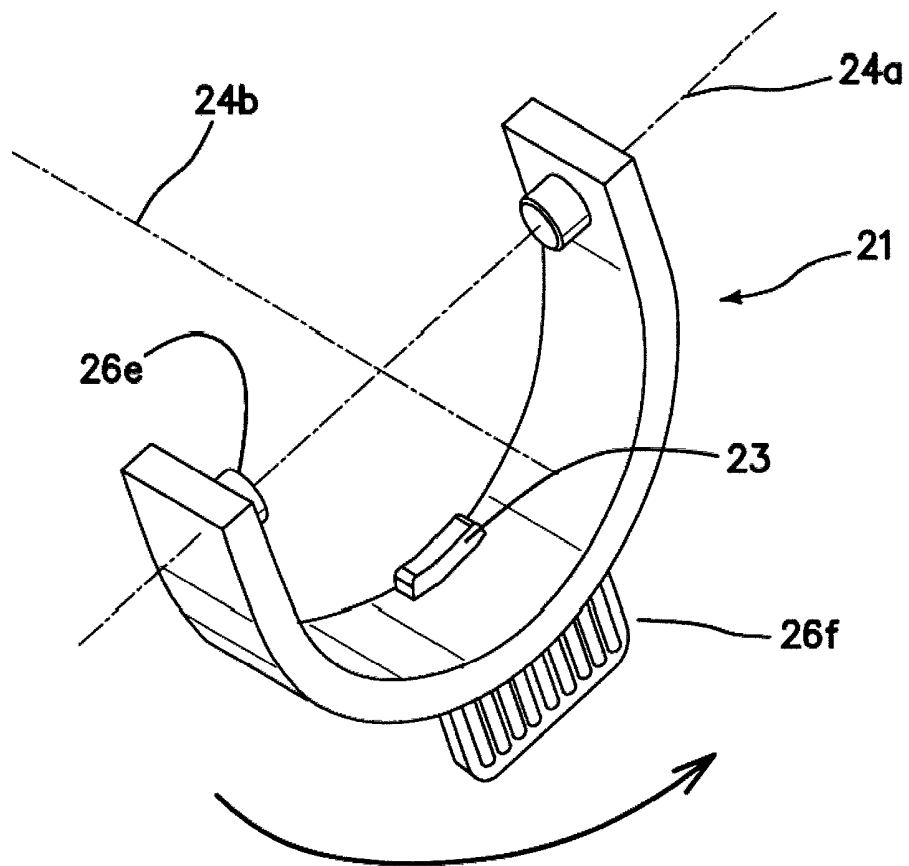
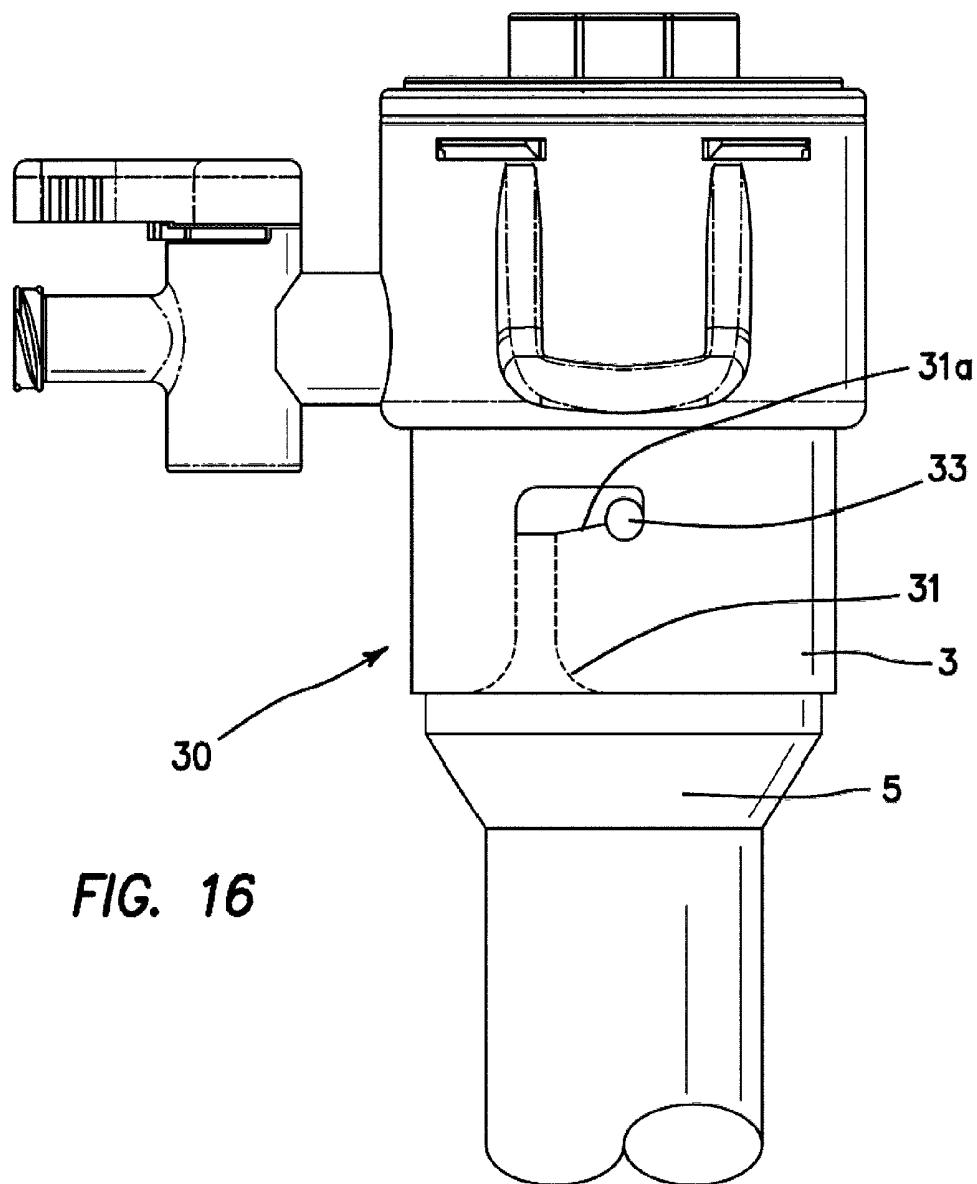
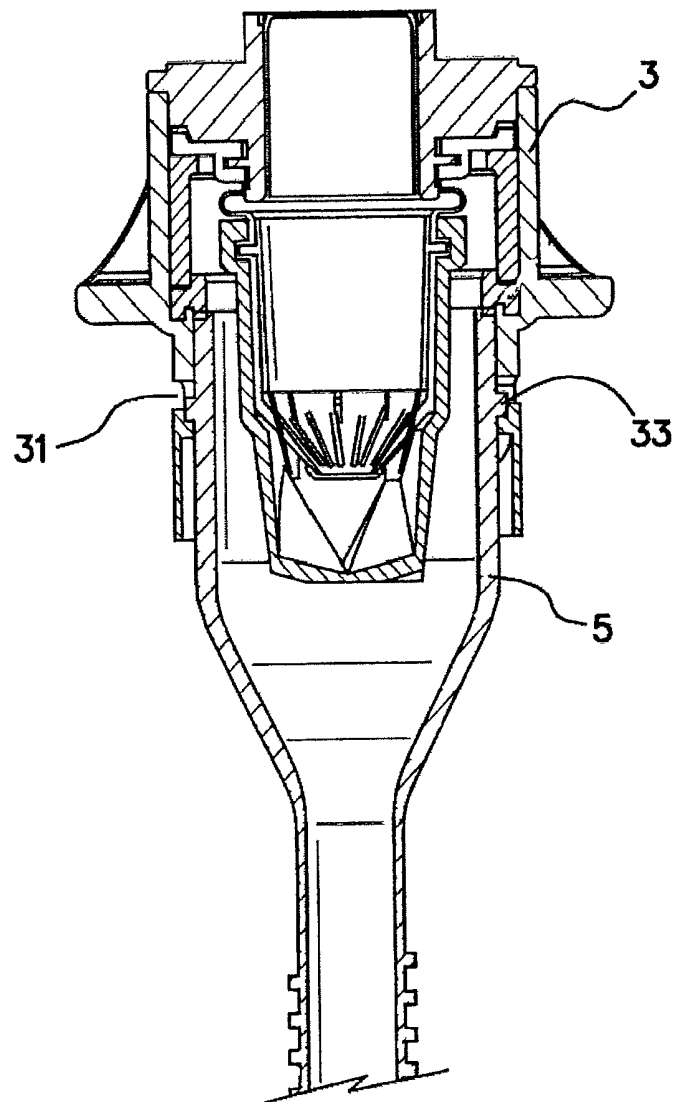
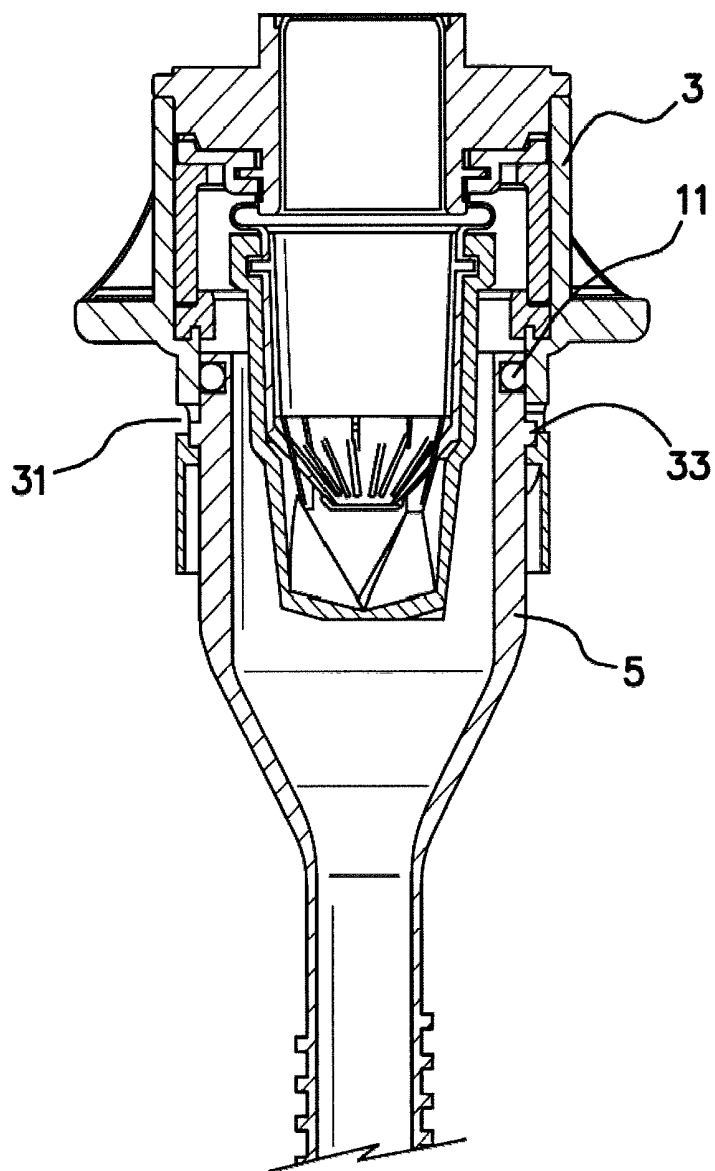


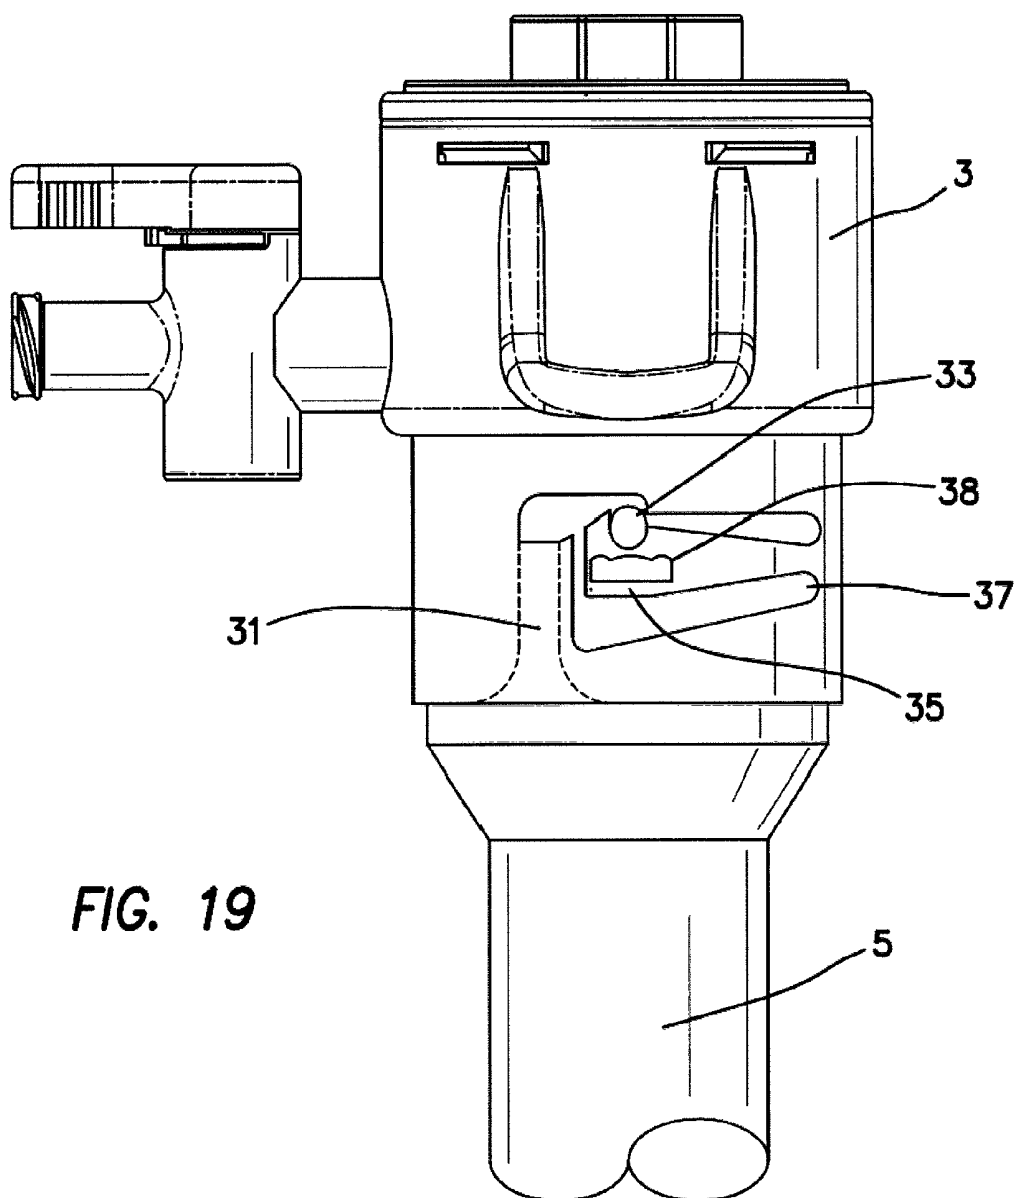
FIG. 14

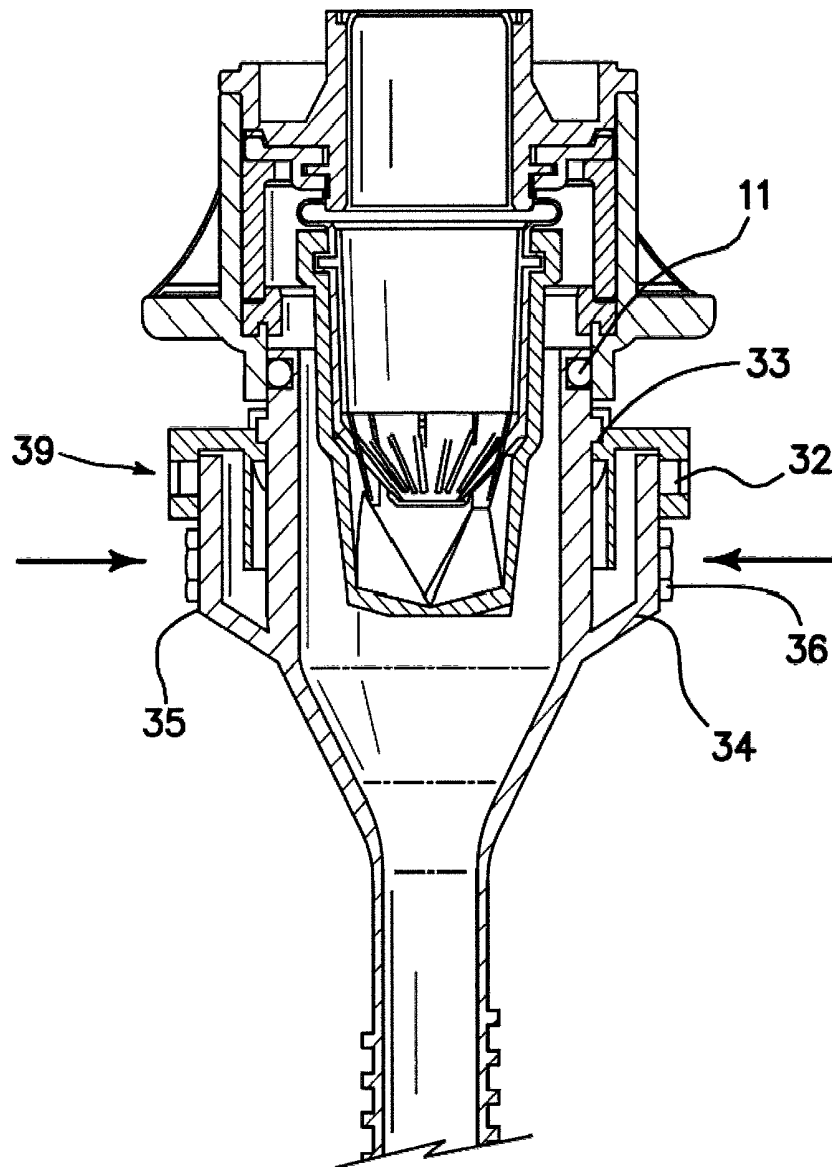
FIG. 15

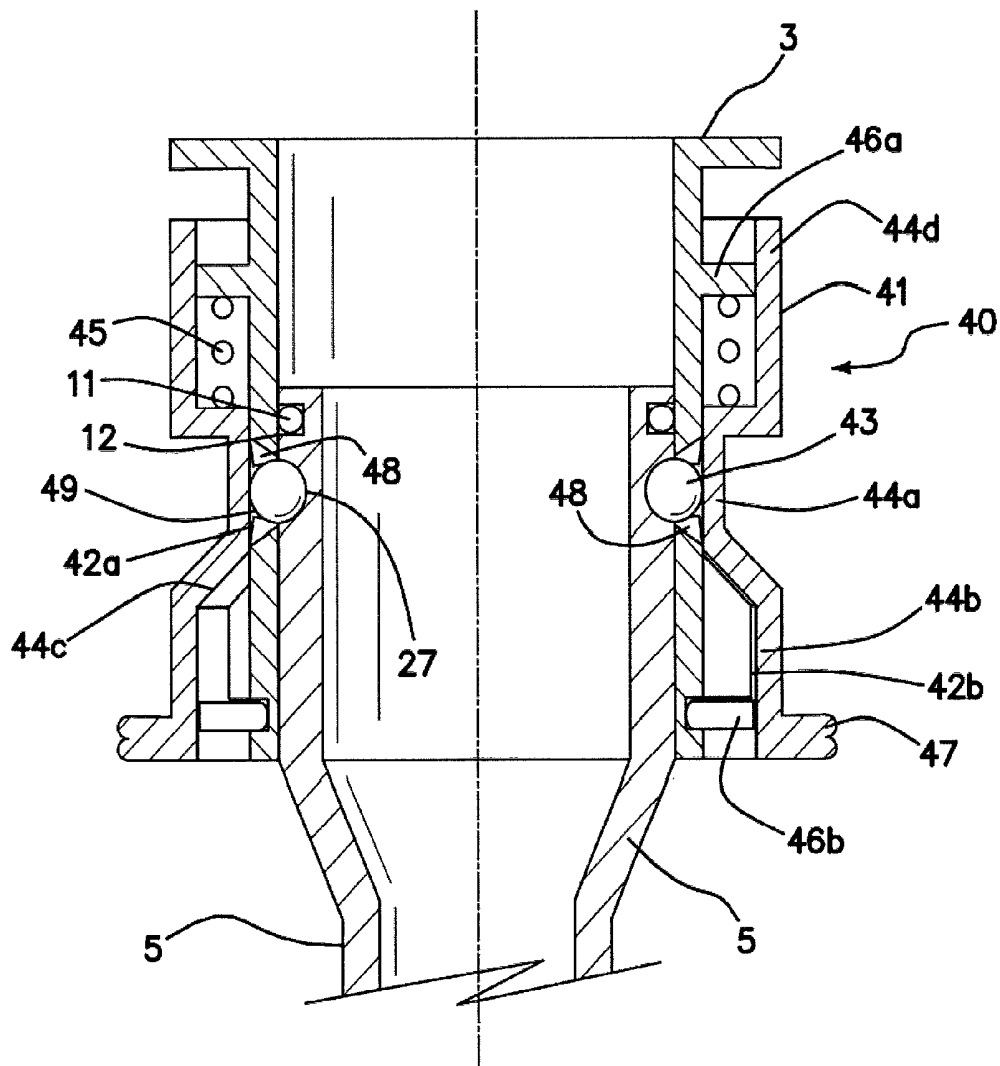
**FIG. 16**

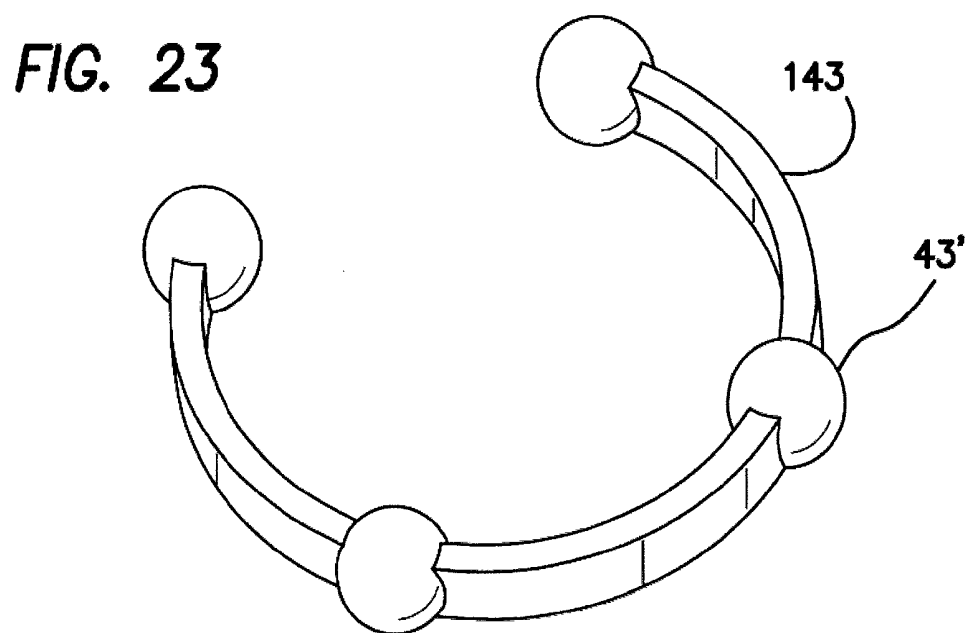
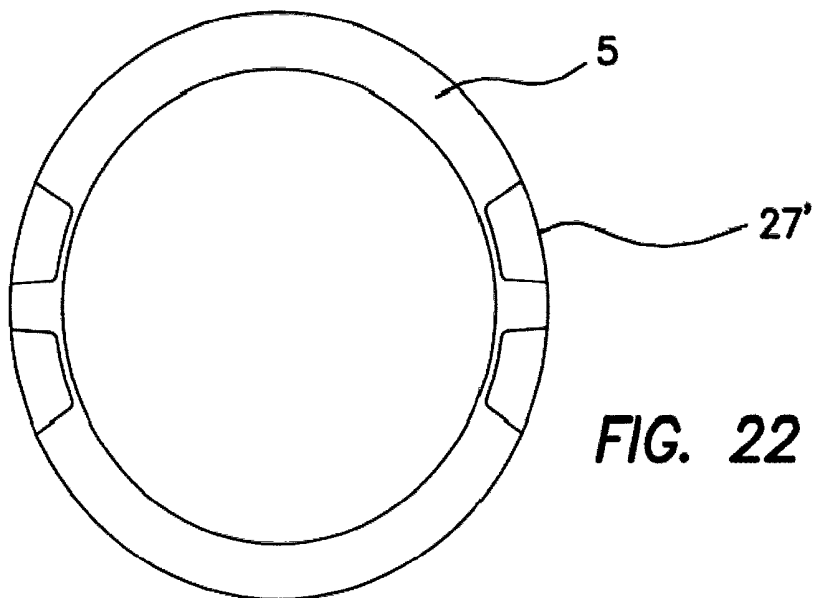
**FIG. 17**

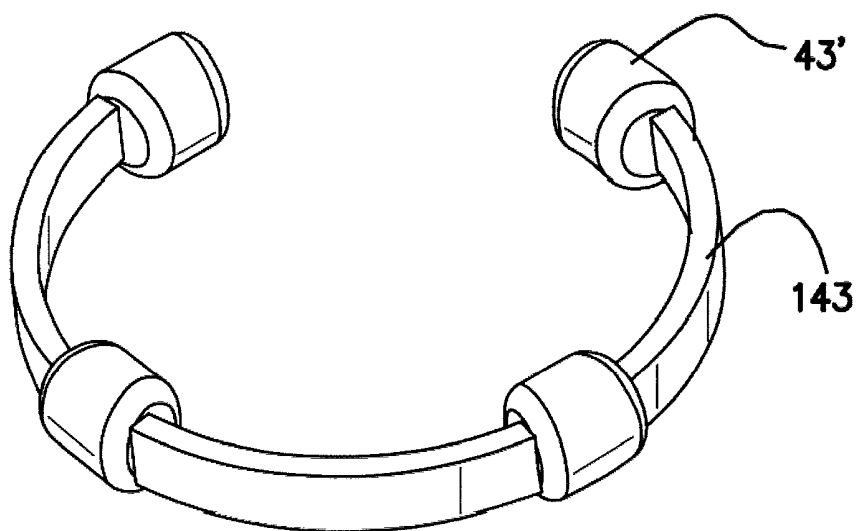
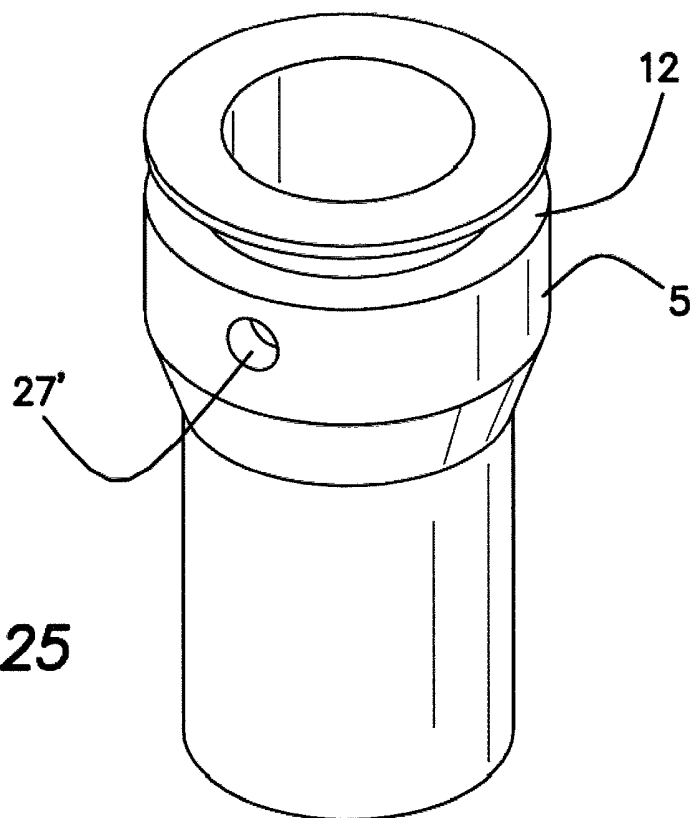
**FIG. 18**

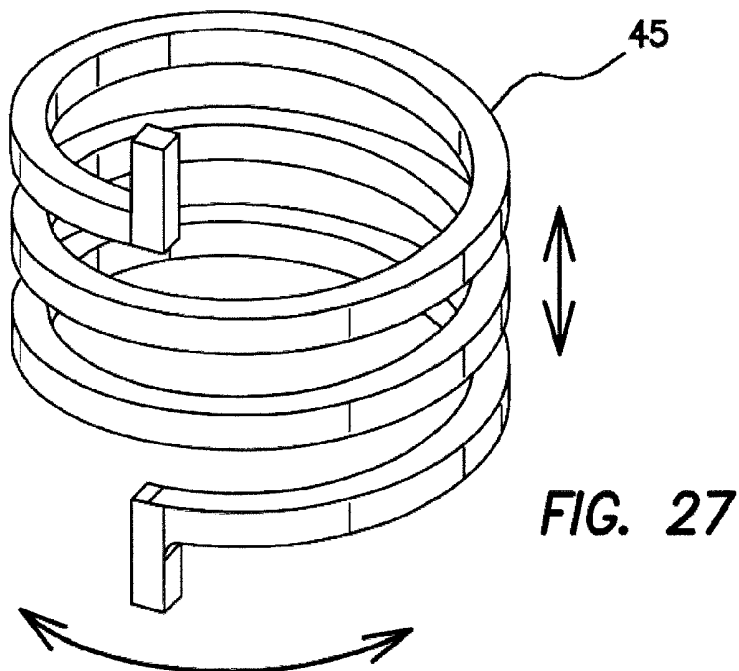
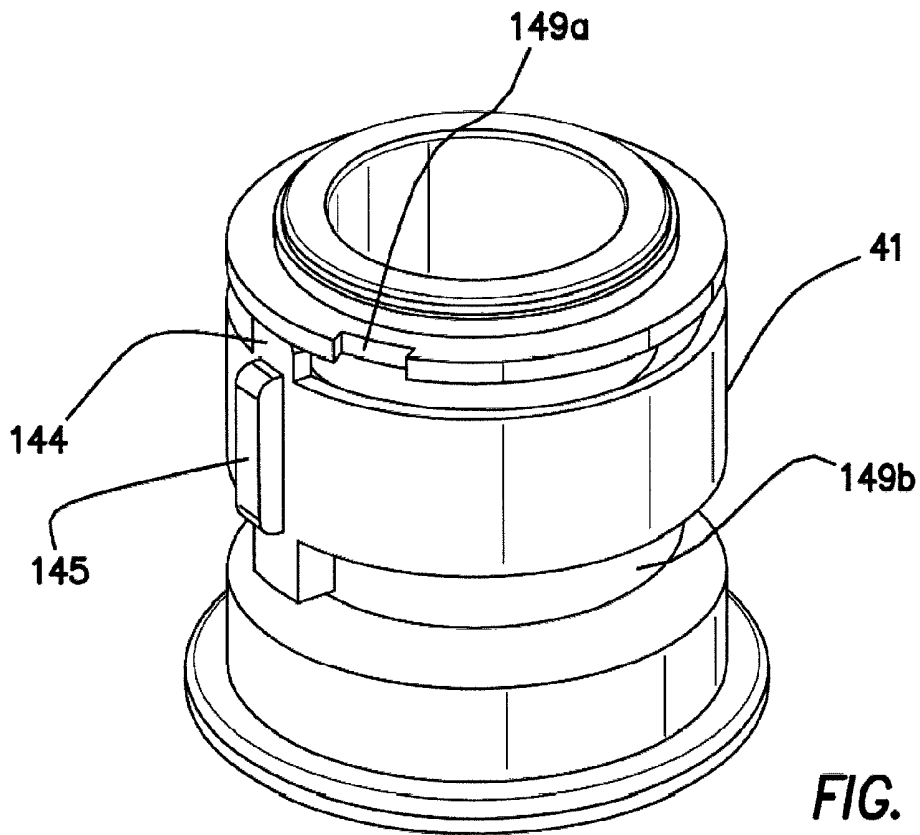


**FIG. 20**

**FIG. 21**



**FIG. 24****FIG. 25**



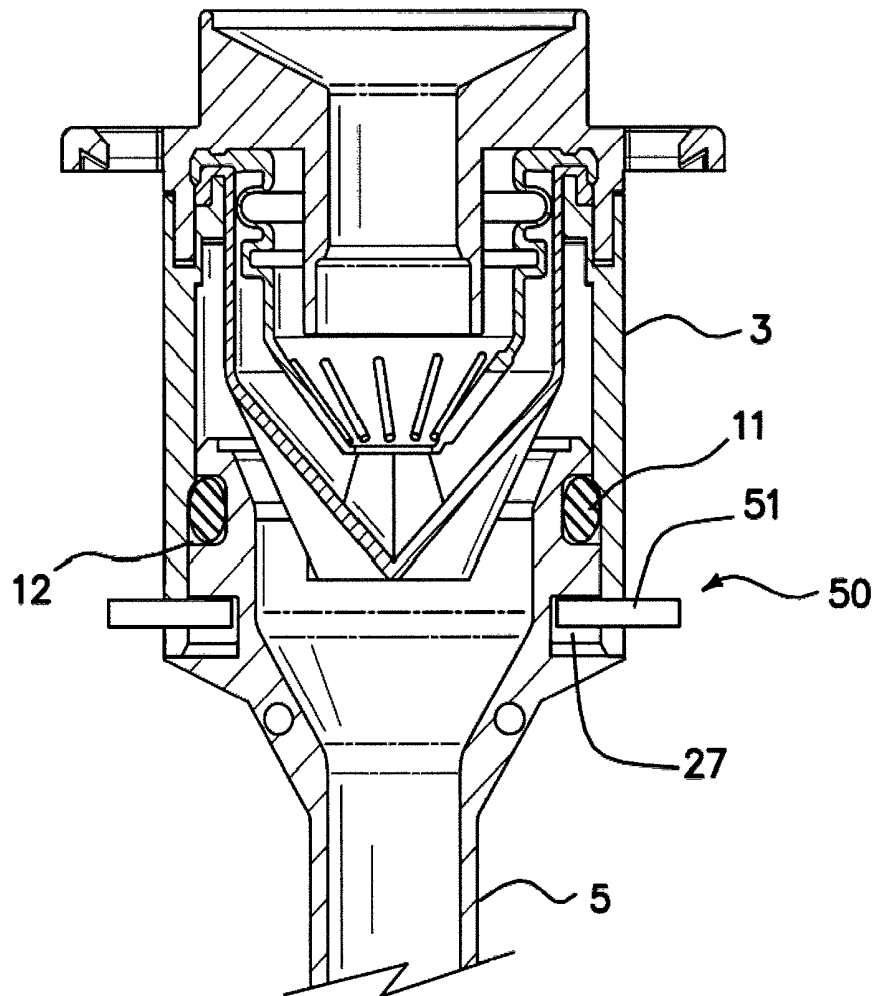
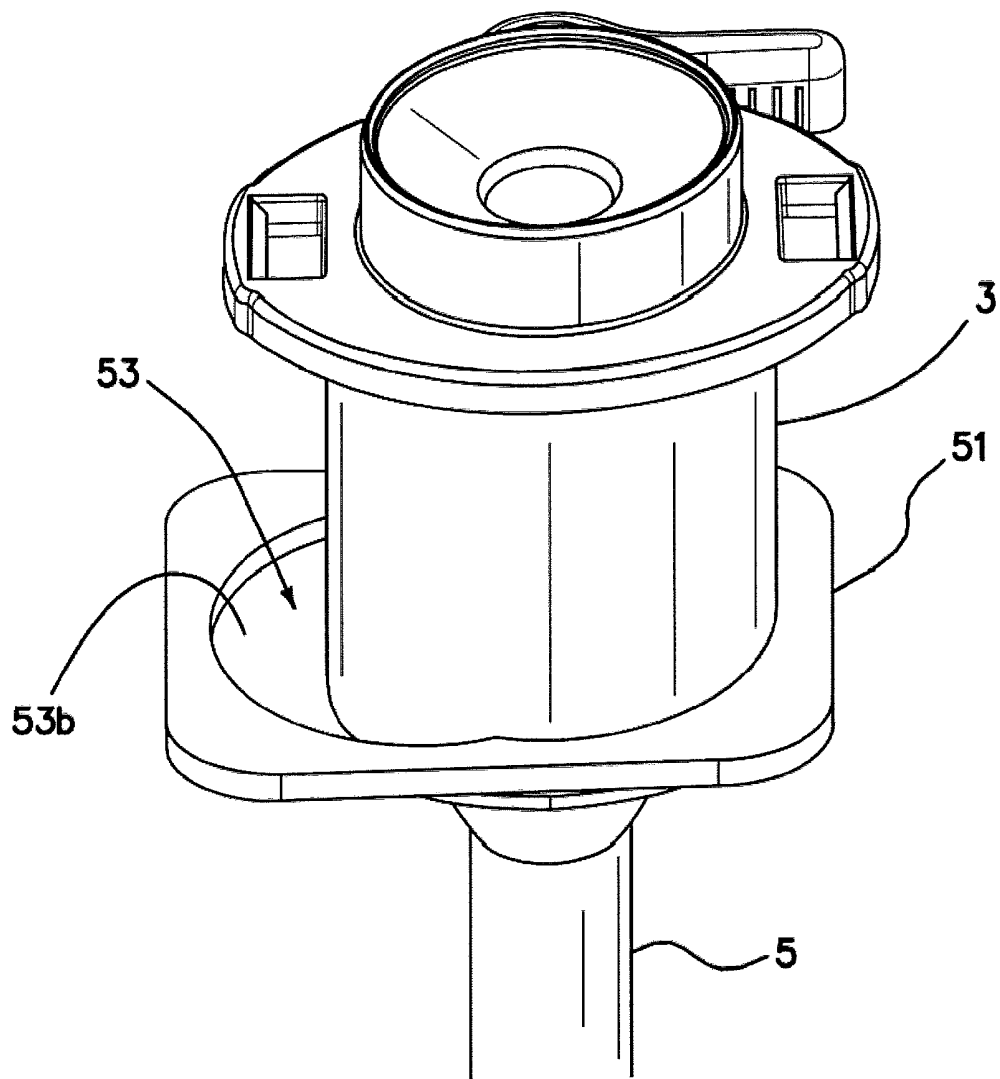


FIG. 28

**FIG. 29**

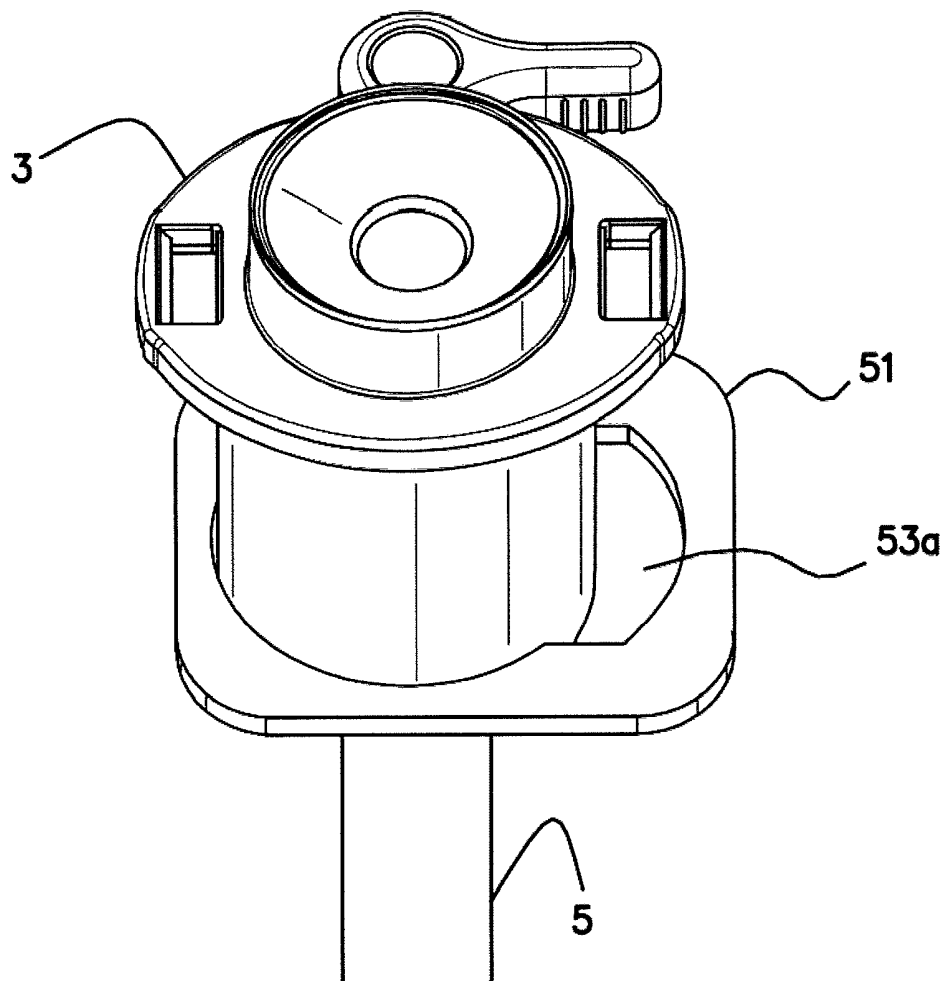
**FIG. 30**

FIG. 31

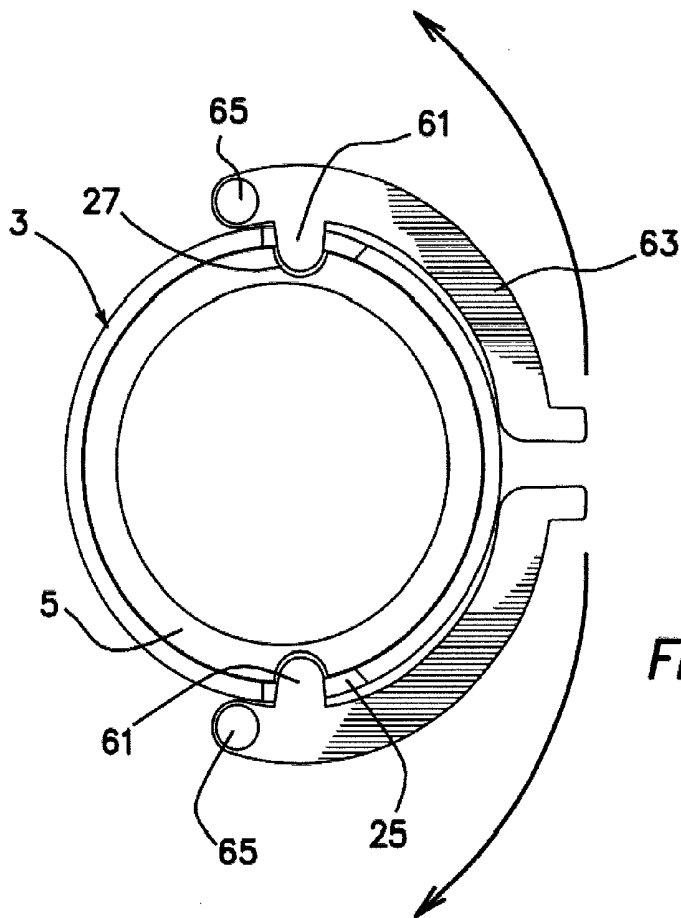
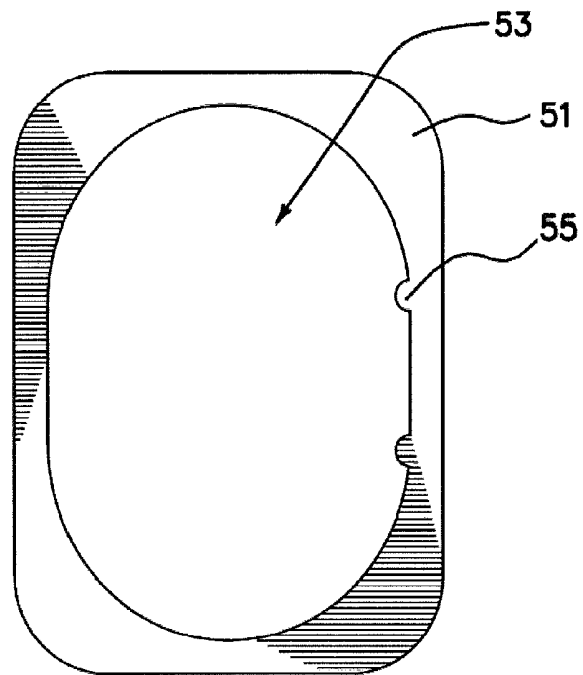
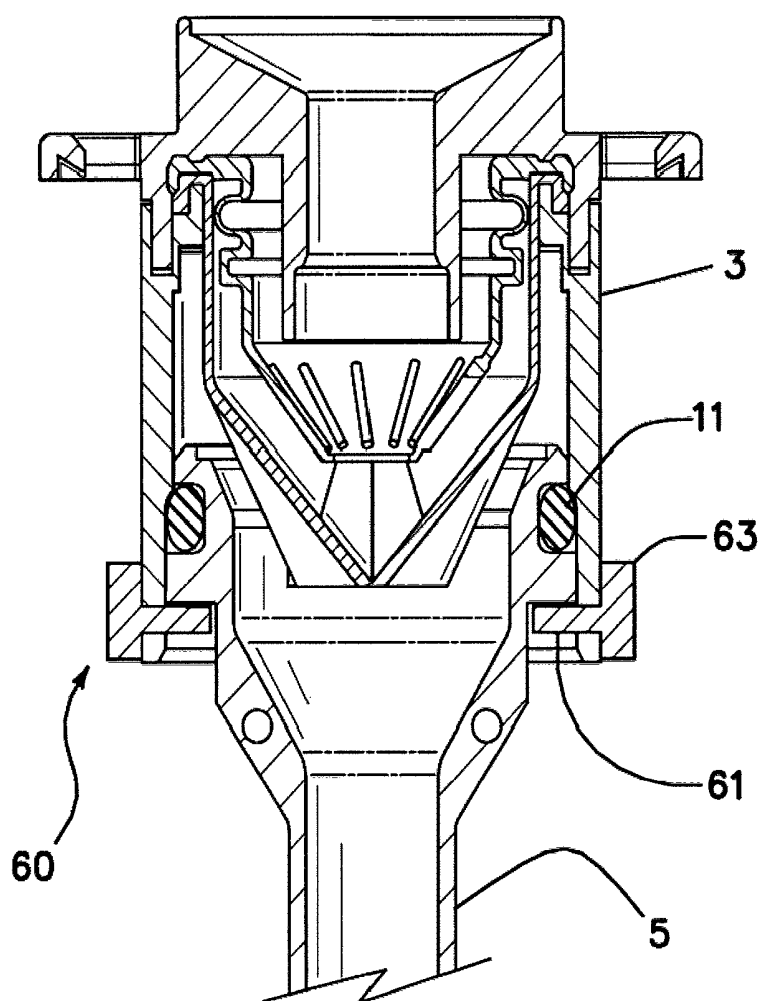
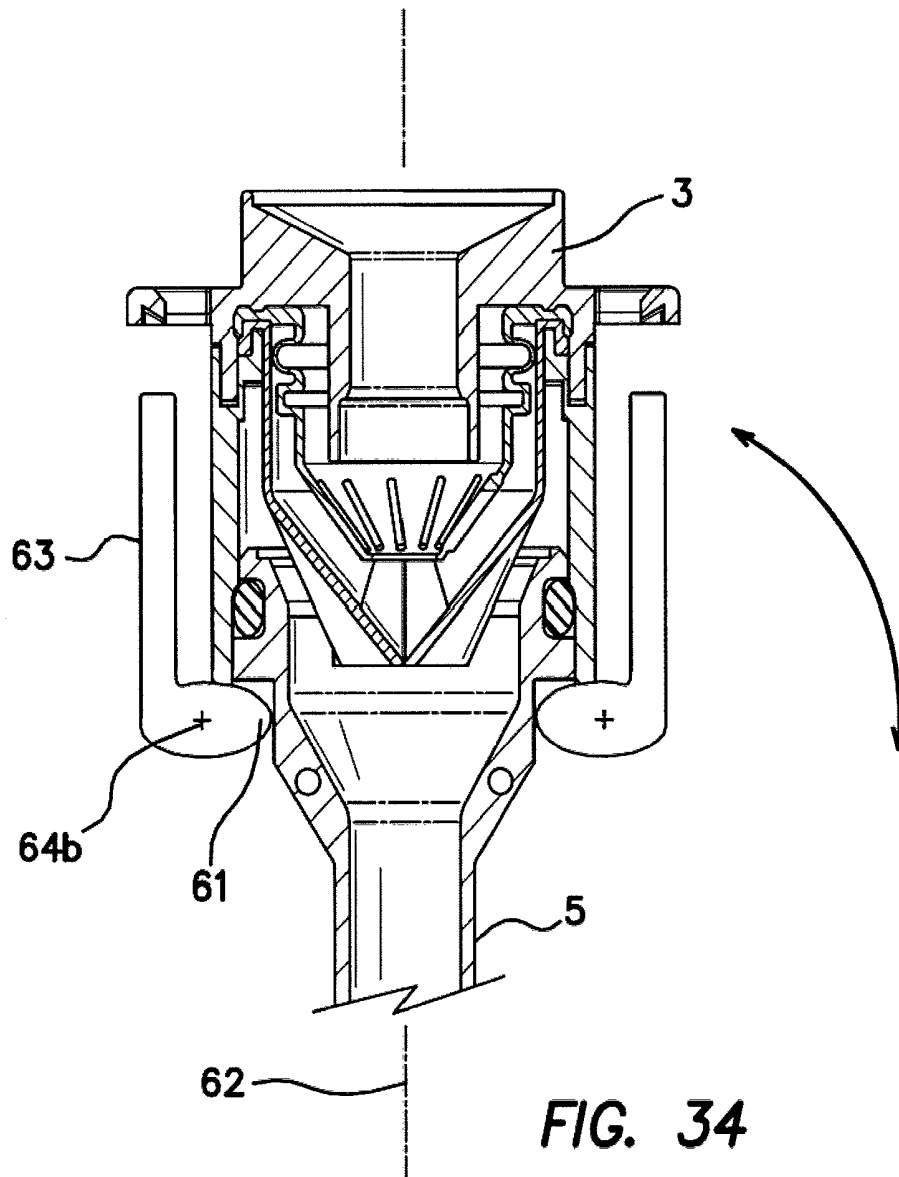
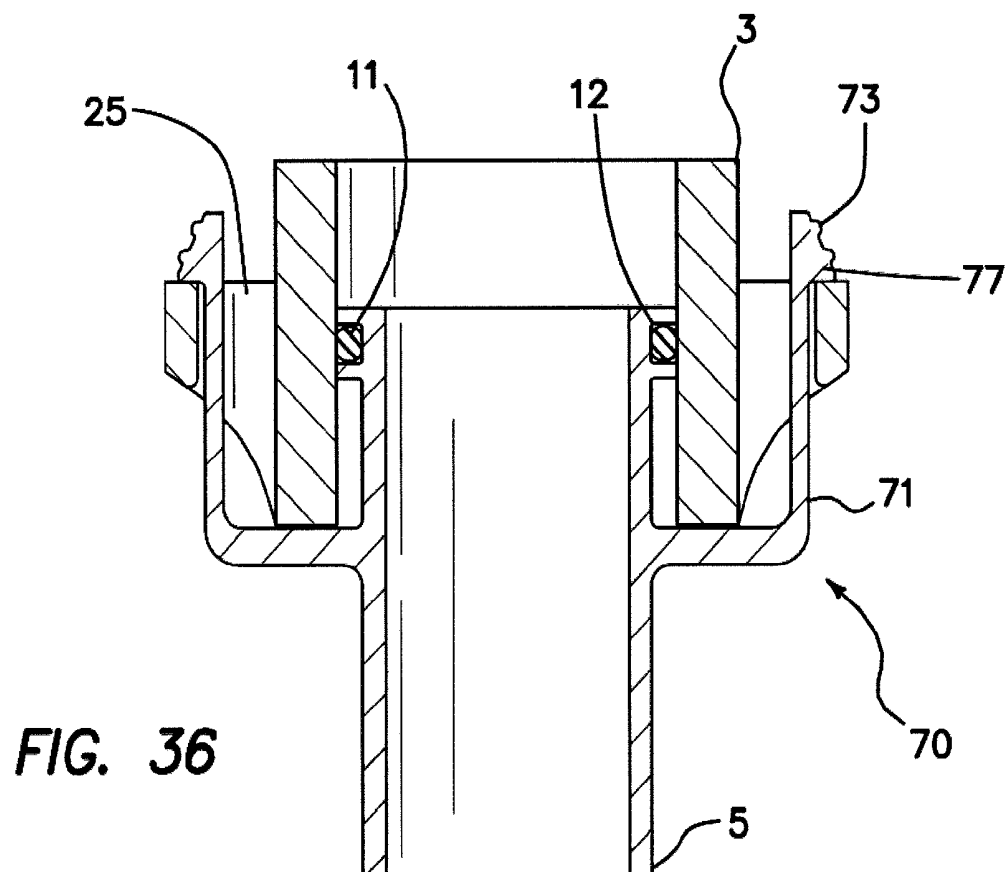
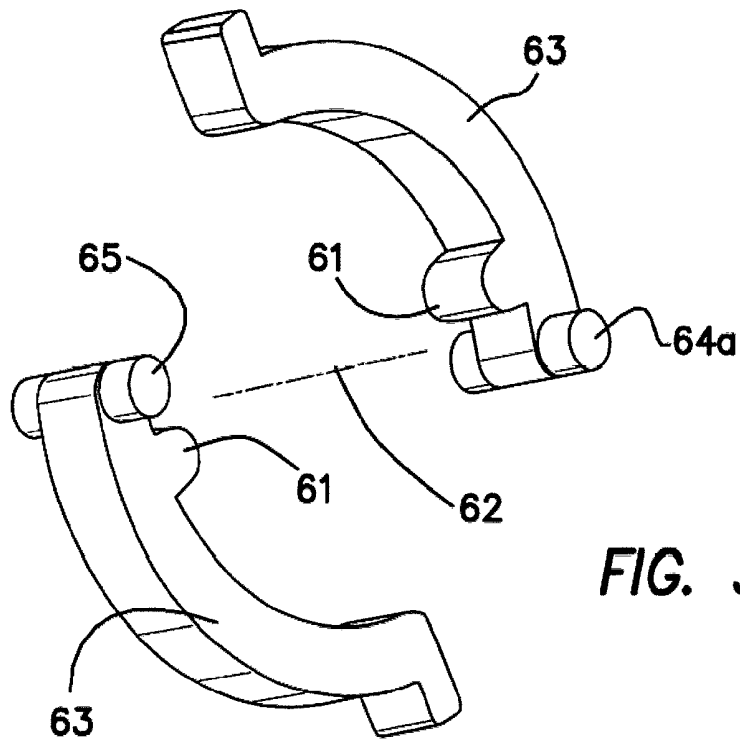


FIG. 33

**FIG. 32**





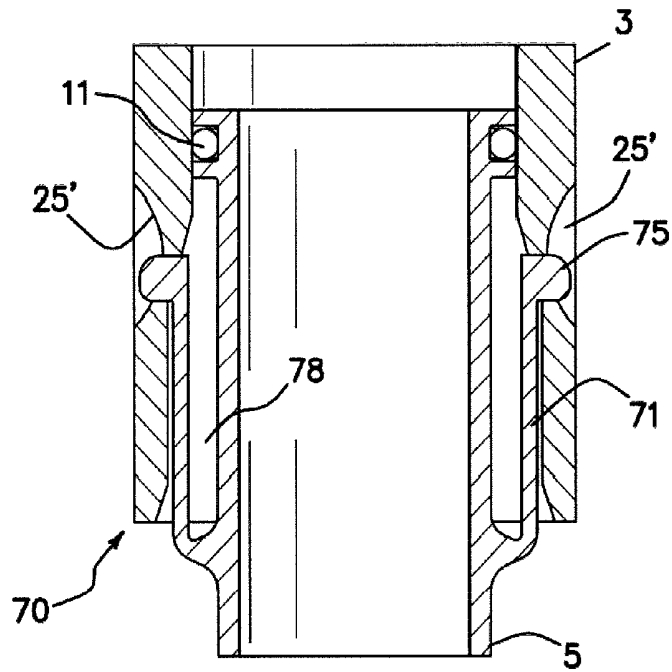


FIG. 37

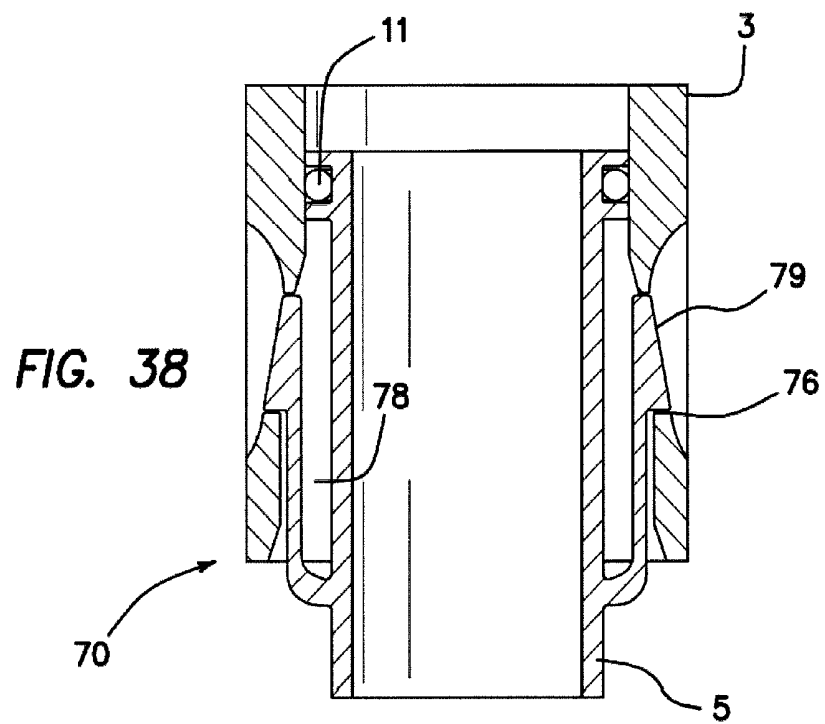
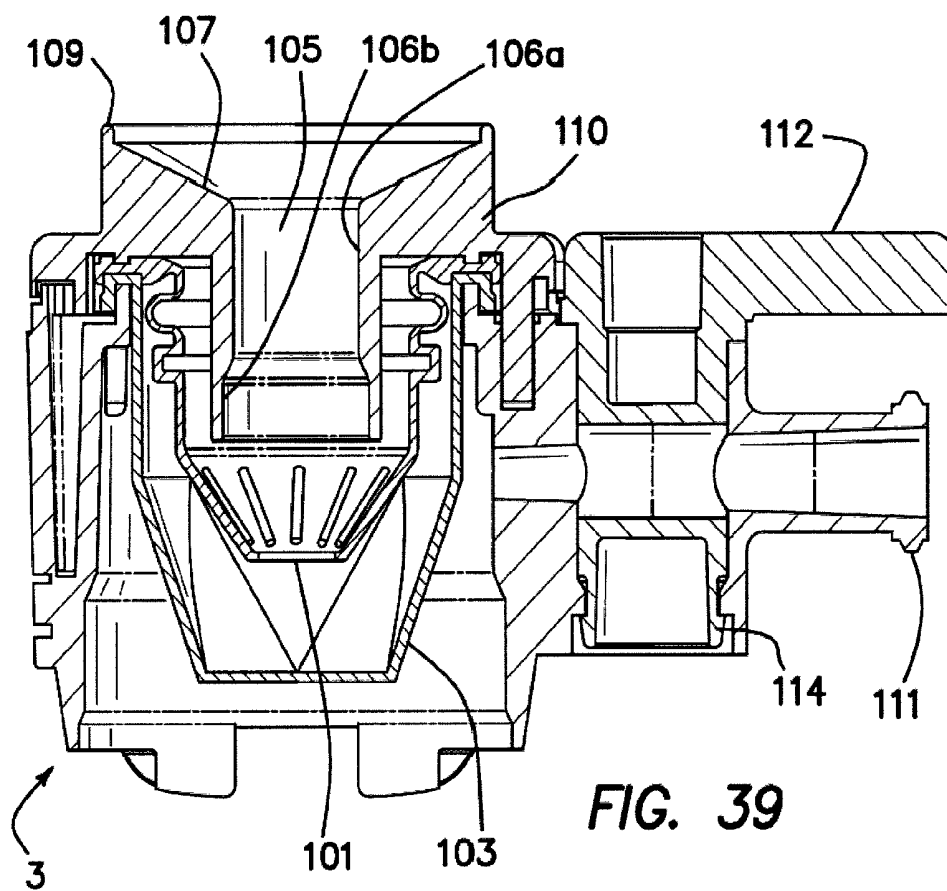


FIG. 38



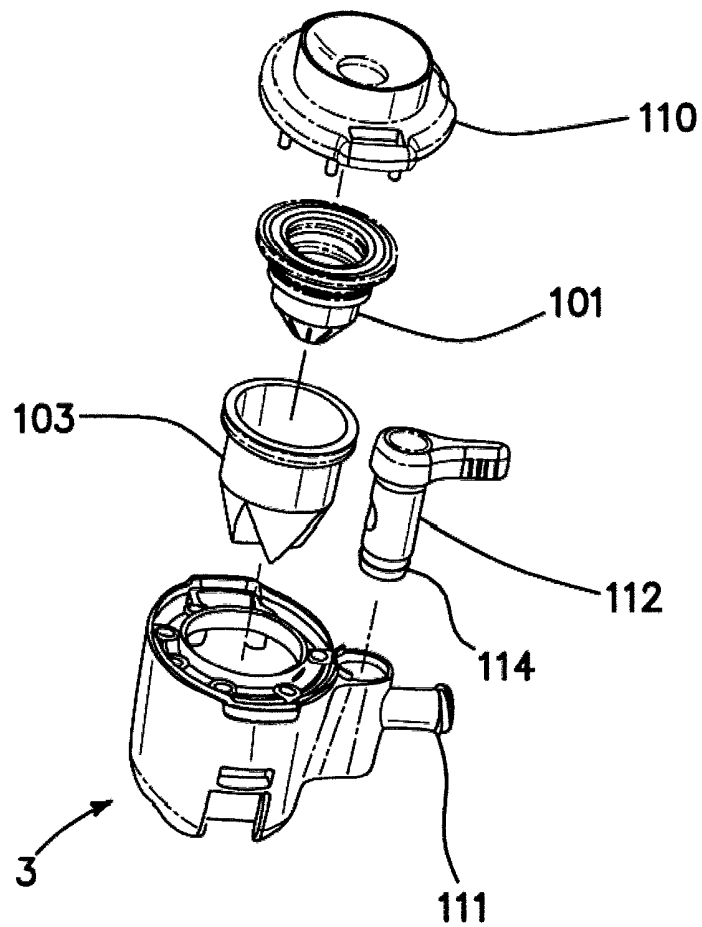
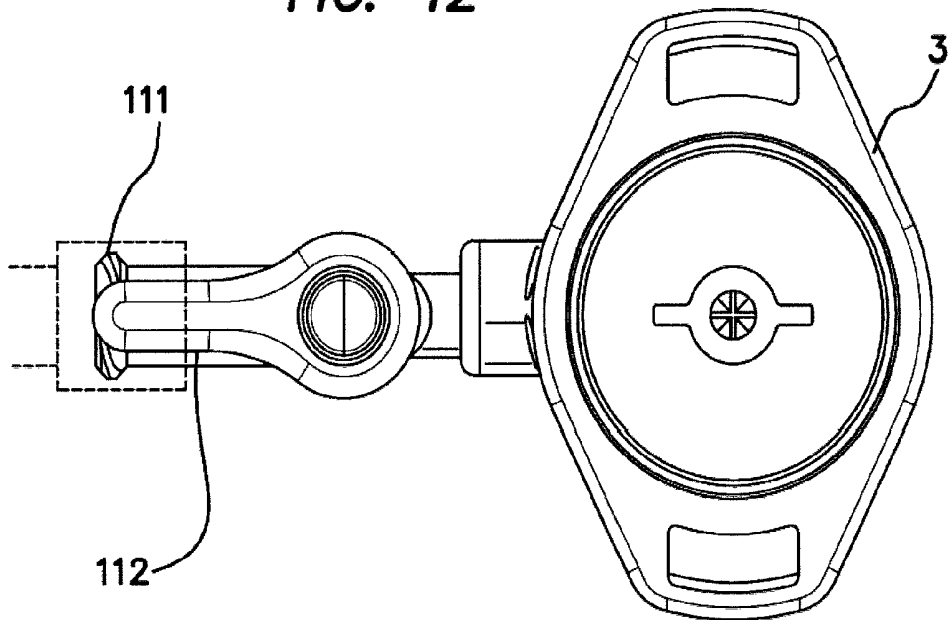
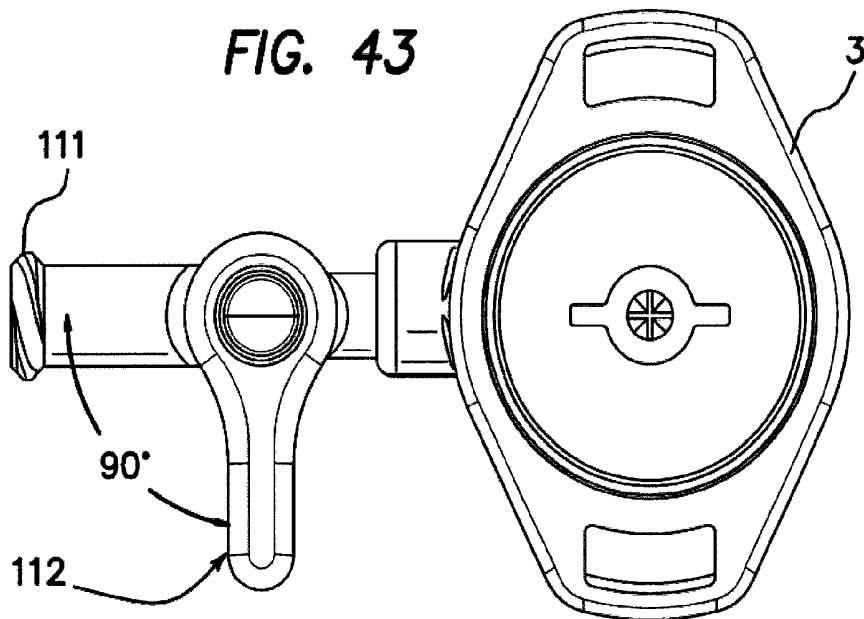
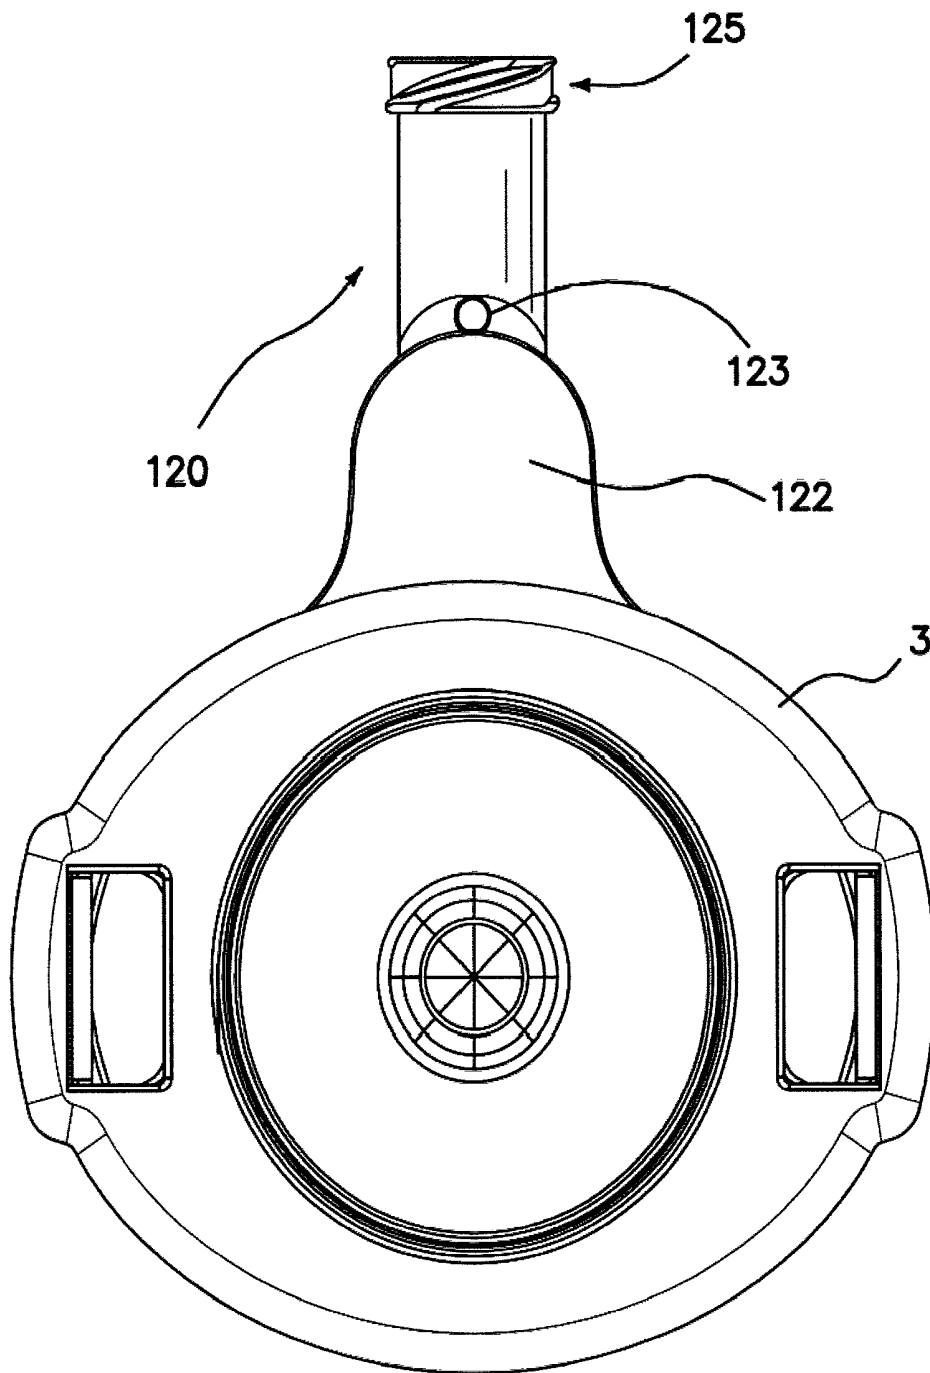
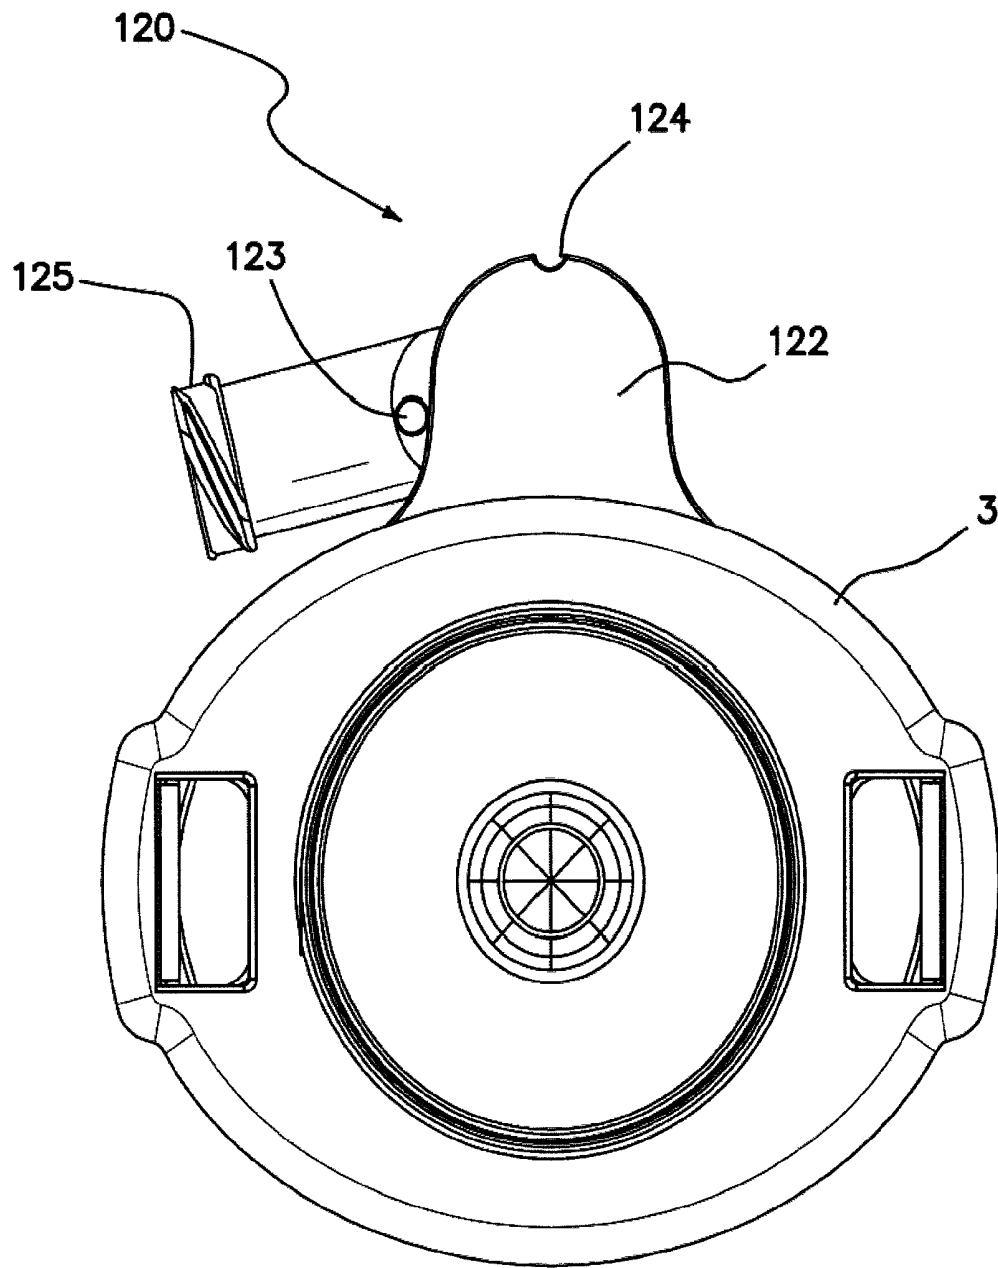
**FIG. 40**

FIG. 41

FIG. 42**FIG. 43**

**FIG. 44**

**FIG. 45**

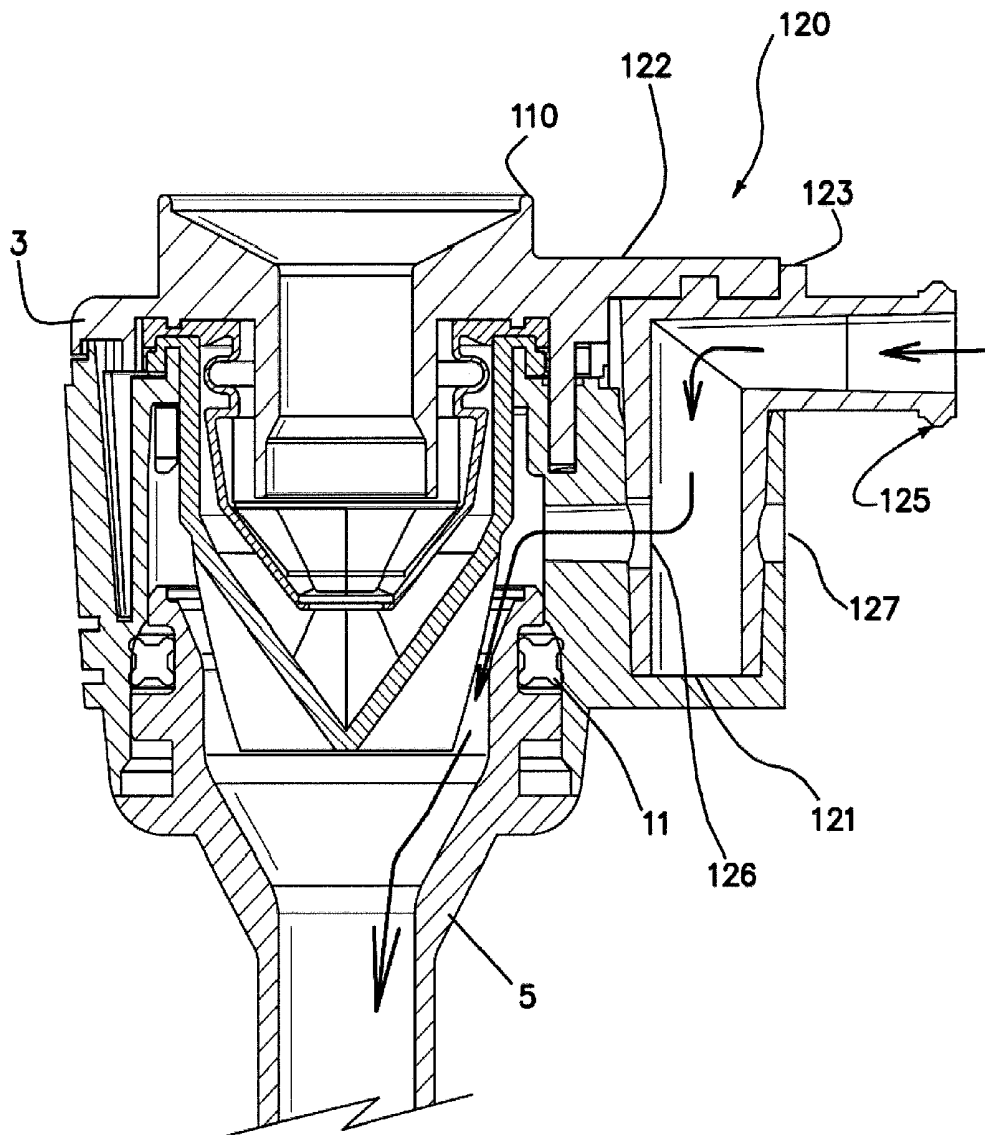


FIG. 46

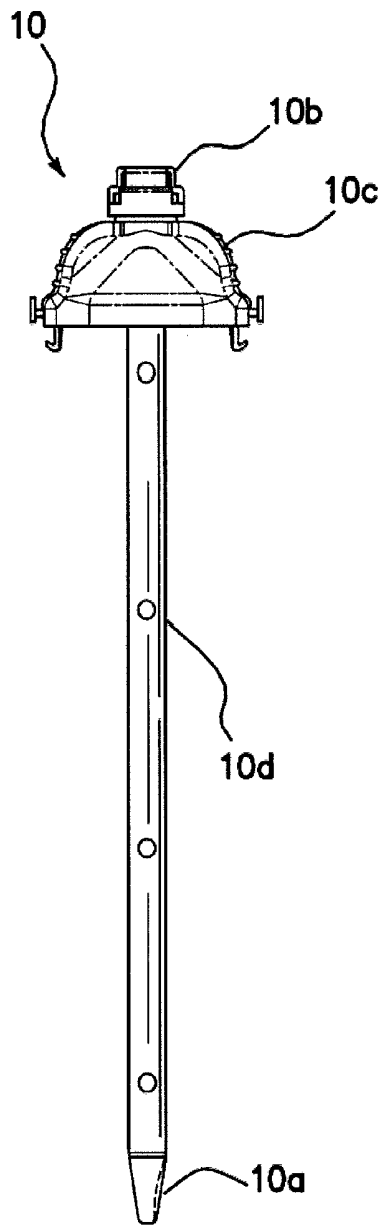


FIG. 47

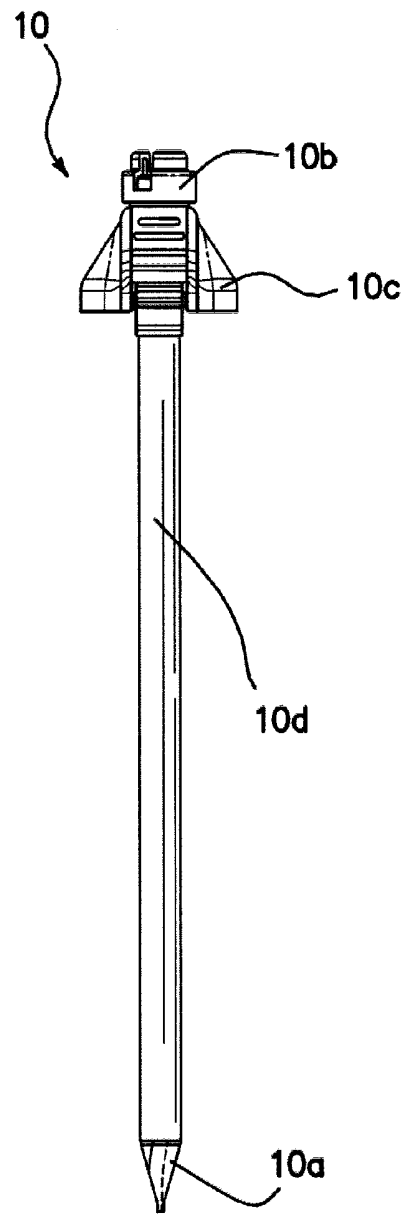
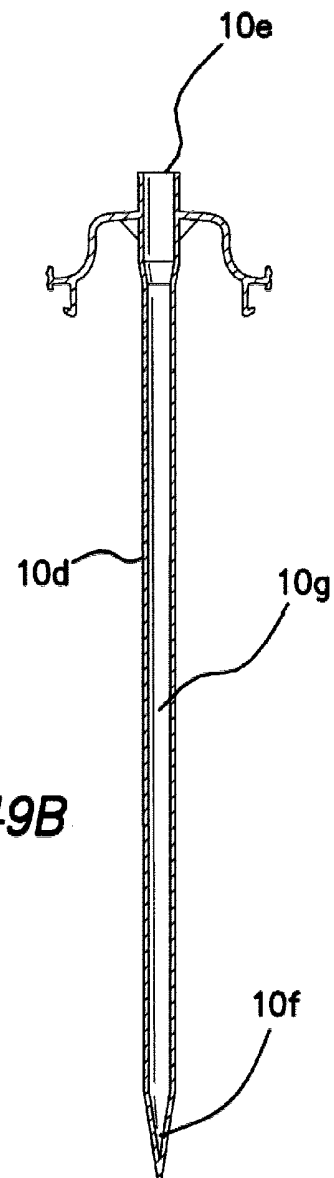
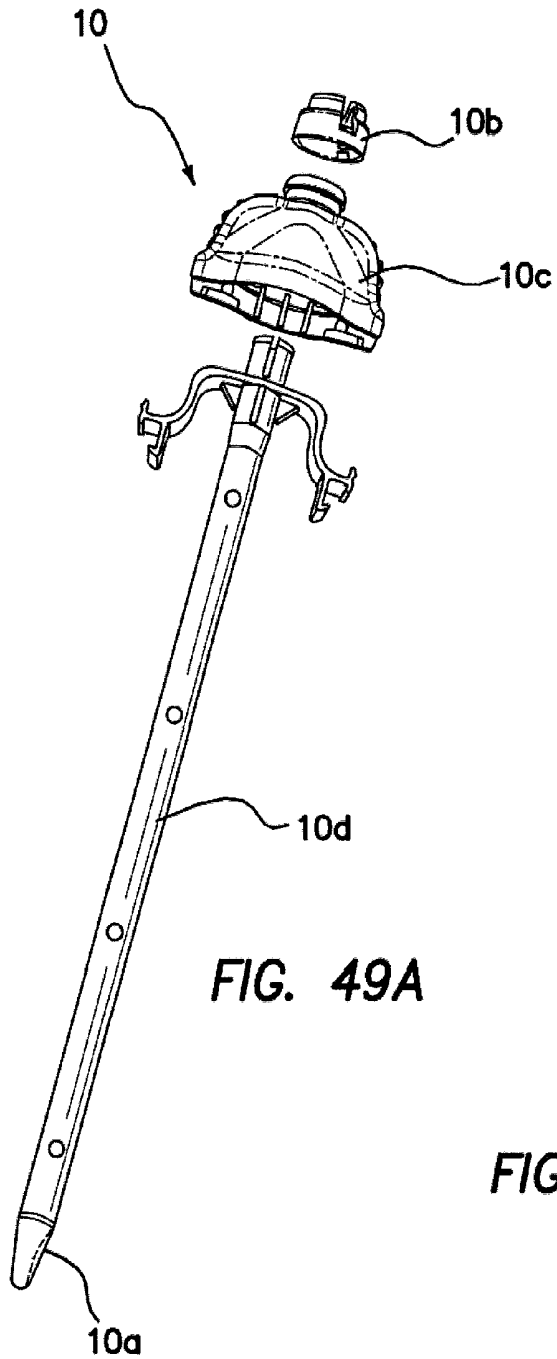
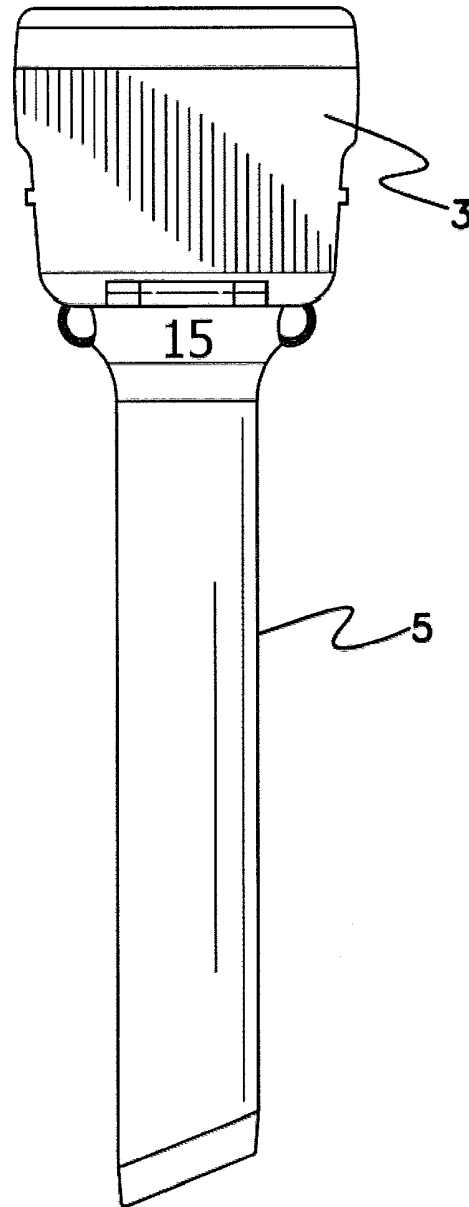


FIG. 48



**FIG. 50**

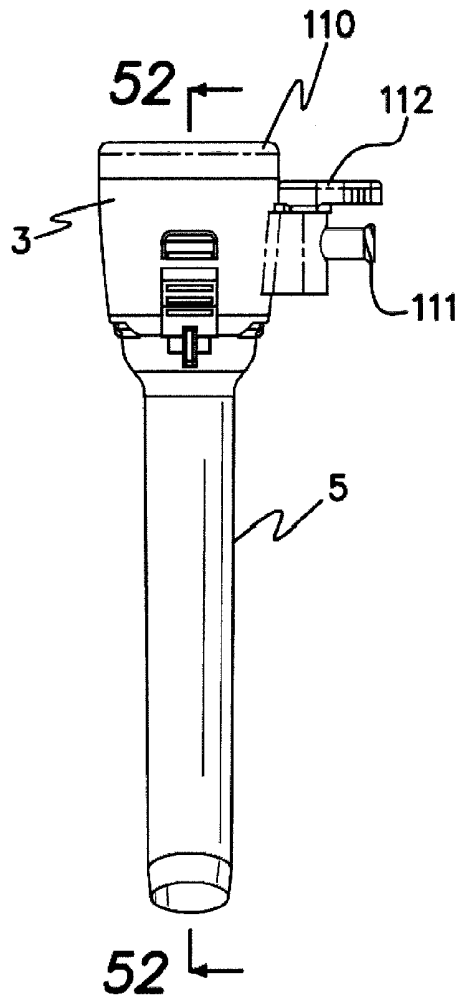


FIG. 51

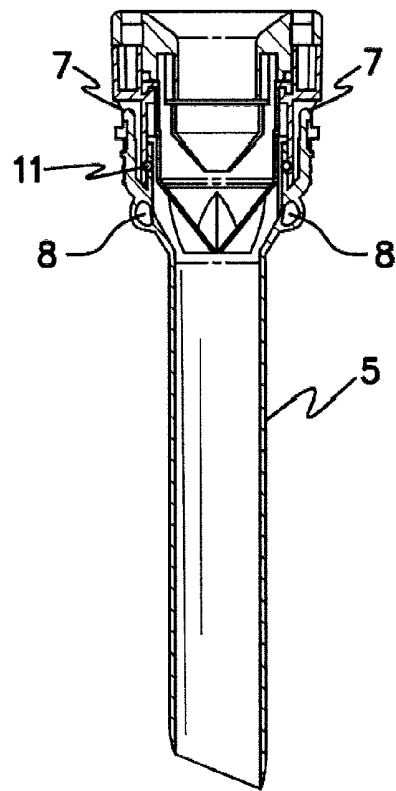
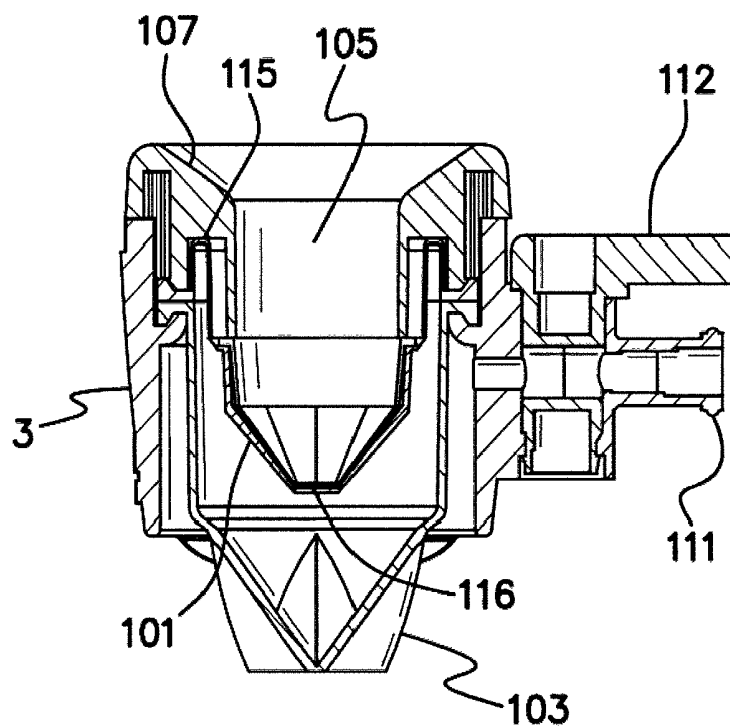


FIG. 52

**FIG. 53**

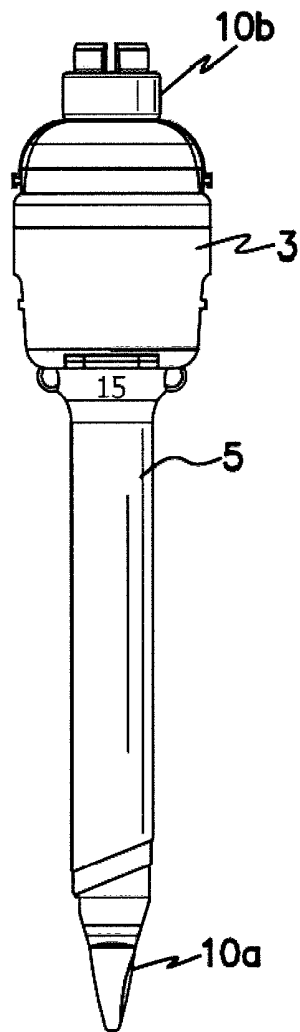


FIG. 54

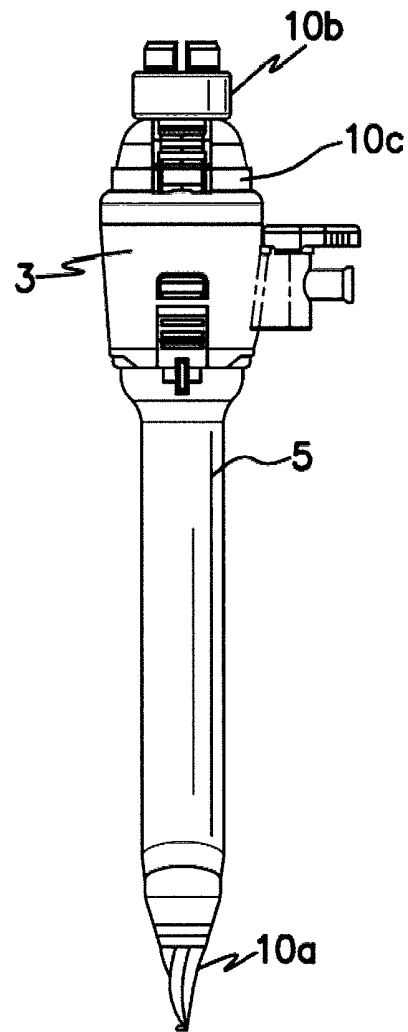


FIG. 55

SURGICAL ACCESS PORT**CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation of U.S. patent application Ser. No. 13/872,340 entitled "SURGICAL ACCESS PORT," filed Apr. 29, 2013, currently pending, which is a continuation of U.S. patent application Ser. No. 11/549,926 entitled "SURGICAL ACCESS PORT," filed Oct. 16, 2006, which issued as U.S. Pat. No. 8,430,851, which claims the benefit of U.S. Provisional Application No. 60/726,825, filed Oct. 14, 2005, and U.S. Provisional Application No. 60/828,515, filed Oct. 6, 2006, the disclosures of all of which are hereby incorporated by reference as if set forth in full herein.

BACKGROUND

Laparoscopic surgery is commonly performed using access ports or trocars, which provide instrument access across an abdominal wall and into a gas pressurized abdominal cavity. Trocar seals within the trocars allow instrument changes with no or minimal loss in gas pressure. Such seals should be very durable even when challenged by the insertion of sharp-pointed instruments. They should be capable of accommodating a wide range of inserted instrumentation without leaking. They should be nearly friction-free so that they do not interfere with the action of the instrument. And they should not damage the inserted instruments. In addition, they should be cost-effective and user-friendly, and not add to the complexity of a surgical procedure. Also, due to the inherent limited confines of laparoscopic surgery, a continuing effort to reduce facial defects and to reduce interference between trocars, smaller or compact trocars are desirable while still providing the above-noted functionalities or enhanced functionalities.

Laparoscopic surgery is an evolving modality. Significant changes in instrumentation continue to challenge the trocar seals presently in use. Accordingly, there remains a continuing need to extend the range, durability and sensitivity of trocar seals.

SUMMARY

Generally, the present invention provides surgical access port or trocar with a low-profile seal housing releasable from a cannula capable of accommodating an optical obturator. In one aspect, a surgical access port comprises a trocar seal housing having at least one seal, a trocar cannula having a lumen, the at least one seal arranged to seal the lumen and a trocar lock releasably connecting the trocar cannula to the seal housing and being one of slidably and pivotably connected to one of the trocar seal housing and trocar cannula.

In one aspect, a surgical access port comprises a trocar seal housing having an instrument seal, a zero seal and an alignment channel with a generally funneled entry. The zero seal is fixed to the trocar seal housing and the instrument seal is positioned between the alignment channel and the zero seal and is pivotably connected to the seal housing and a trocar cannula is attached to the trocar seal housing.

In one aspect, a surgical access port comprises a trocar seal housing having an instrument seal, a zero seal, a shield and an alignment channel with a generally funneled entry. The zero seal is fixed to the trocar seal housing, the instrument seal is positioned between the alignment channel and the zero seal and is connected to the seal housing. The

shield is positioned between the alignment channel and the instrument seal and a trocar cannula is attached to the trocar seal housing.

Many of the attendant features of the present invention will be more readily appreciated as the same becomes better understood by reference to the foregoing and following description and considered in connection with the accompanying drawings in which like reference symbols designate like parts throughout.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a front view of a surgical access port in accordance with various aspects of the present invention;

FIG. 2 is a side view of a surgical access port in accordance with various aspects of the present invention;

FIG. 3 is a front view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 4 is a side view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 5 is a cross-sectional view taken along section lines 5-5 of FIG. 4 in accordance with various aspects of the present invention;

FIG. 6 is an enlarged cross-sectional side view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 7 is front view of a trocar seal housing detached from a trocar cannula in accordance with various aspects of the present invention;

FIG. 8 is side view of a trocar seal housing detached from a trocar cannula in accordance with various aspects of the present invention;

FIG. 9 is a cross-sectional side view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 10 is a perspective view of a lock ring in accordance with various aspects of the present invention;

FIG. 11 is a cross-sectional side view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 12 is a perspective view of a lock ring in accordance with various aspects of the present invention;

FIG. 13 is a perspective view of a lock ring in accordance with various aspects of the present invention;

FIG. 14 is a perspective view of a lock ring in accordance with various aspects of the present invention;

FIG. 15 is a perspective view of a lock ring in accordance with various aspects of the present invention;

FIG. 16 is a side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 17 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 18 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 19 is a side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 20 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 21 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 22 is a top view of a portion of socket lock in accordance with various aspects of the present invention;

FIG. 23 is a perspective view of a socket lock in accordance with various aspects of the present invention;

FIG. 24 is a perspective view of a socket lock in accordance with various aspects of the present invention;

FIG. 25 is a perspective view of a partially shown trocar cannula in accordance with various aspects of the present invention;

FIG. 26 is a perspective view of a trocar seal housing and socket lock in accordance with various aspects of the present invention;

FIG. 27 is a perspective view of a return spring in accordance with various aspects of the present invention;

FIG. 28 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 29 is a perspective view of a surgical access port in a locked condition without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 30 is a perspective view of a surgical access port in an unlocked condition without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 31 is a top view of a gate lock in accordance with various aspects of the present invention;

FIG. 32 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 33 is a cross-sectional top view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 34 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula in accordance with various aspects of the present invention;

FIG. 35 is a perspective view of lock levers in accordance with various aspects of the present invention;

FIG. 36 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula and seal housing in accordance with various aspects of the present invention;

FIG. 37 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula and seal housing in accordance with various aspects of the present invention;

FIG. 38 is a cross-sectional side view of a surgical access port without an optical obturator and partially shown cannula and seal housing in accordance with various aspects of the present invention;

FIG. 39 is a cross-sectional side view of a trocar seal housing in accordance with various aspects of the present invention;

FIG. 40 is an exploded view of a trocar seal housing in accordance with various aspects of the present invention;

FIG. 41 is a cross-sectional side view of a trocar seal housing in accordance with various aspects of the present invention;

FIGS. 42-43 are plan views of a trocar seal housing in accordance with various aspects of the present invention;

FIGS. 44-45 are plan views of a trocar seal housing in accordance with various aspects of the present invention;

FIG. 46 is a cross-sectional side view of a trocar seal housing in accordance with various aspects of the present invention;

FIG. 47 is a front view of an optical obturator in accordance with various aspects of the present invention;

FIG. 48 is a side view of an optical obturator in accordance with various aspects of the present invention;

FIG. 49A is an exploded view of an optical obturator in accordance with various aspects of the present invention;

FIG. 49B is a longitudinal cross section of the shaft of the obturator illustrated in FIG. 49A;

FIG. 50 is a front view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 51 is a side view of a surgical access port without an optical obturator in accordance with various aspects of the present invention;

FIG. 52 is a cross-sectional view taken along section lines 52-52 of FIG. 51 in accordance with various aspects of the present invention;

FIG. 53 is a cross-sectional side view of a trocar seal housing in accordance with various aspects of the present invention;

FIG. 54 is a front view of a surgical access port in accordance with various aspects of the present invention; and

FIG. 55 is a side view of a surgical access port in accordance with various aspects of the present invention.

DETAILED DESCRIPTION

A surgical access port, e.g., a trocar, which comprises a trocar seal housing, a trocar cannula, and/or an optical obturator is provided. In this description, “proximal” or “proximally” refers to that portion of the instrument, component, or element that extends toward the user. “Distal” or “distally” refers to that portion of the instrument, component, or element that extends away from the user. The trocar is configured to access a body cavity and to maintain positive pressure at its distal end to prevent loss of surgical insufflation gas such as carbon dioxide used, for example, in laparoscopic procedures to insufflate the body cavity. The trocar seal and trocar cannula is also configured to sealingly engage surgical instruments of various diameters, which would typically be inserted through the trocar, to prevent loss of surgical gas during use of such instruments. In one aspect, the trocar seal housing is releasably attachable to the trocar cannula to allow the seal to be removed during surgery to enable the extraction of tissue specimens through the trocar. The trocar in one aspect has or is included with an optical obturator having a tip, which includes a smooth outer surface and has a high degree of optical clarity.

Referring now to FIGS. 1-4, the trocar seal housing 3 in one aspect can be easily detached or removed from the trocar cannula 5 and easily attached or re-attached to the trocar cannula 5 for example during a surgical procedure. During surgery, small tissue specimens may be extracted from a body cavity through a trocar to enable pathological analysis of the tissue specimen. The integrity of the tissue specimen can be maintained or the maintenance facilitated by avoiding

or minimizing withdrawal of delicate tissue specimens through a trocar seal. As such, in one aspect, the trocar seal housing 3 is arranged to be removed from the trocar cannula 5 to enable extraction of tissue specimens from a body cavity while maintaining the integrity of the tissue specimen. The trocar seal housing 3 also easily reattaches to the trocar cannula 5 after its initial removal during a surgical procedure.

Also, in one aspect, the trocar seal housing 3 is easily removable from the trocar cannula 5 to enable rapid desufflation of an insufflated body cavity. In one aspect, a trocar lock releasably attaches the trocar cannula to the trocar seal housing. For example, towards the end of a laparoscopic surgical procedure, release of the insufflation gas such as carbon dioxide from the peritoneal cavity of the patient is performed. By opening one or more stopcock valves on the trocar seal, desufflation can be achieved. The flow rate through the stopcock valves, however, can be slow with regard to evacuation of the carbon dioxide from the peritoneal cavity and therefore the time expended to evacuate the insufflation gas can be excessive. By removing the seal housing 3 from the cannula 5, the cannula provides an unobstructed outlet for the insufflation gas to escape thereby decreasing desufflation time.

In FIGS. 5-8, two cantilever arms 7 extend from the cannula 5 which engage mating slots 9 on the trocar seal housing 3. Each of the cantilever arms 7 has a hook 7a on its distal end, which engages a ledge 13 on the trocar seal housing 3 when the trocar seal housing 3 is attached to the trocar cannula 5. The hooks on the cantilever arms maintain the axial position of the trocar seal housing on the trocar cannula and prevent axial dislodgment of the trocar seal housing 3 from the trocar cannula 5.

The cantilever arms 7 in one aspect act as leaf springs resiliently attaching onto the trocar seal housing 3. For example, during attachment of the trocar seal housing 3 onto the trocar cannula 5, the cantilever arms 7 flex inward until the distal ends of the cantilever arms reach slots 9 in the trocar seal housing 3. Once the distal ends of the cantilever arms 7 reach the trocar seal housing slots 9, the cantilever arms 7 spring outward such that the hooks 7a overhang the mating ledges 13 on the trocar seal housing 3. When an axial force is applied to the trocar seal housing 3 relative to the trocar cannula 5, the hooks 7a further engage the ledges 13 on the trocar seal housing and do not allow removal of the trocar seal housing from the trocar cannula. As such, in one aspect, a trocar lock comprises a pair of resilient arms 7 extending from opposing sides of the trocar cannula 5 in a direction parallel to a longitudinal axis of the cannula. The pair of resilient arms operationally engaging the pair of slots 9 on opposing sides of the trocar seal housing 3.

To remove the trocar seal housing 3 from the trocar cannula 5, finger tabs 7b located on the mid-portion of the cantilever arms 7 are depressed causing the cantilever arms to move inward resulting in the disengagement of the hooks 7a from the housing ledges 13. The trocar seal housing 3 can thereby be removed from the trocar cannula 5 by applying an axial force to the trocar seal housing relative to the trocar cannula. The cantilever arms 7 on the trocar cannula 5 also prevent or resist rotation of the trocar seal housing relative to the trocar cannula 5. For example, the cantilever arms 7 prevent the trocar seal housing 3 from being twisted off of the trocar cannula 5 during manipulation of the trocar. In one aspect, the trocar seal housing 3 is prevented from being twisted off by tabs or extended portions 18a of the cannula 5 engaging recesses or slots 18b in the seal housing 3. The trocar seal housing and cannula attachment can also be

threaded and/or bayonet lock connections to attach the trocar seal housing 3 to the trocar cannula 5. However, inadvertently rotating the trocar seal housing 3 relative to the trocar cannula 5 during manipulation of inserted instrumentation or manipulation of connected insufflation gas tubing to the seal housing may result in an unintended detachment of the trocar seal housing 3 from the trocar cannula 5. An unintended detachment of a trocar seal housing from a trocar cannula during a surgical procedure may result in a loss of insufflation gas, a loss of visibility of the operative area, a delay in the procedure, and/or other potential surgical issues.

The trocar cannula 5 in one aspect has a cannula seal or sealing ring 11 positioned in a groove, cavity or gland 12 at its proximal end which forms a seal with the inside diameter of the trocar seal housing. In one aspect, a gland is an o-ring cavity and includes the portion of the cavity, e.g., portions of the trocar cannula and/or housing, that compress the o-ring to create a seal. In one aspect, the groove 12 in a proximal end of the cannula substantially encircles an outer periphery of the cannula 5 and a seal or the sealing ring 11 is disposed in the groove 12. The sealing ring 11, which in one aspect comprises of an o-ring with an "o" cross section, prevents loss of pneumoperitoneum between the trocar seal housing 3 and the trocar cannula 5. To minimize the friction between the sealing ring 11 and the trocar seal housing 3, an x-ring can be used rather than an o-ring. The x-ring has a generally "x" cross section and minimizes the area of contact between the sealing ring and the trocar seal housing 3 resulting in a reduction of static and kinetic frictional forces. Reducing the frictional forces between the sealing ring 11 and the trocar seal housing 3 reduces the axial force utilized to attach and/or detach the trocar seal relative to the trocar cannula 5.

Referring now to FIGS. 9-11, a trocar lock ring 21 releasably connects the trocar seal housing 3 to the trocar cannula 5. The lock ring 21 is shown simultaneously in an unlocked position on the left side of the trocar seal housing and a locked position on the right side of the trocar seal housing 3 for simplicity and ease of discussion. The trocar lock ring 21 in one aspect is substantially cylindrical and outlines a perimeter that generally corresponds to the outer periphery of the trocar seal housing 3. The lock ring 21 positions the trocar seal housing between the lock ring and the trocar cannula. One or more projections, protrusions or tabs 23 extend from the lock ring 21. In one aspect, one or more rectangular tabs extend perpendicularly from an inner surface of the lock ring 21 and the longitudinal axis of the trocar cannula 5. In a lock position, the tabs 23 extend through a corresponding aperture or slot 25 in the trocar seal housing 3 and into a corresponding groove or cavity 27 in the trocar cannula 5 thereby securing the trocar seal housing 3 to the trocar cannula 5. The groove 27 in the trocar cannula is adjacent to, e.g., below or away from the proximal end of the trocar cannula 5, the groove 12 in the trocar cannula holding the cannula seal 11. By moving or withdrawing the tab 23 out of the groove 27 in the trocar cannula 5, i.e., moving the lock ring 21 into an unlock position, the trocar seal housing 3 is released or allowed to be removed from the trocar cannula 5. In one aspect, the tab 23 is completely movable out of the groove 27 of the trocar cannula 5, but is not completely movable out of the corresponding aperture 25 in the trocar seal housing 3. As such, in one aspect, a trocar lock comprises a ring 21 having a tab 23 inwardly extending towards a center of the ring 21. The trocar seal housing 3 has an aperture 25 and the trocar cannula having a groove 27. The tab or tabs are movable from a first position in which the tab is engaged with the aperture, sized to receive the tab, in the trocar seal housing 3 and a second

position in which the tab is engaged with the aperture in the trocar seal housing and the groove, sized to receive the tab, in the trocar cannula 5.

In one operational case, the lock tab 23 protrudes through the wall of the trocar seal housing 3 and into the trocar cannula groove 27, locking the trocar seal housing 3 to the trocar cannula 5. To release the trocar seal housing 3 from the trocar cannula 5, the locking ring 21 is manipulated in specific predetermined manner to prevent accidental operation or unlocking of the trocar seal housing 3 from the trocar cannula 5. The manipulation of the locking ring 21 causes the lock tab 23 to be directly or indirectly withdrawn from the groove 27, thus allowing removal of the trocar seal housing 3 from the trocar cannula 5.

The locking ring in one aspect is arranged with external grip tabs 29 flushed with or extended on an outer surface of the lock ring 21 and positioned on opposing sides of the ring. The grip tabs 29 in one aspect are also positioned on the outer surface of the lock ring 21. In one operation, squeezing the tabs 29 together in the direction shown deforms the lock ring 21 to a generally oval shape manipulates the locking ring and causes withdrawal of the tabs 23 from the groove 27. The grip tabs 29 in one aspect are protected from accidental operation by being positioned under a ledge 28 projecting from the trocar seal housing 3.

In one aspect, as shown in FIG. 12, the locking ring 21 is generally cylindrical and close-fitting to the trocar seal housing 3 with the locking ring 21 having one or more sections forming a portion of the cylinder. One or more projections or tabs 23 extend from the one or more sections of the locking ring 21 towards the seal housing 3. In one aspect, a portion of the locking ring 21 has three sections 22a, b, c each connected successively to each other via living hinges, walls having curved cavities allowing the sections to move away from the center of the locking ring 21. One of the sections, section 22a is connected to the remaining portion 22d of the locking ring 21 at about a mid-point of the remaining portion 22d and another section, section 22c is connected to another end of the remaining portion 22d of the locking ring 21 near the external or outer surface of the locking ring 21. The other section, section 22b is connected between the two sections, sections 22a and 22c. One of the sections, section 22a has a projection or tab 23 extending perpendicularly from the section towards the seal housing 3 to engage the seal housing aperture 25 and the cannula groove 27. The other section, section 22c, has grip tabs 24 extending from an outer surface of the section 22c. In one operation, as shown by the direction arrows, by squeezing one of the sections, e.g., section 22c, inwards towards the center of the locking ring 21 causes the adjoining two sections, sections 22a, b to move or rotate outwards away from the seal housing 3 and cannula 5, thereby pulling or withdrawing the tab 23 from the cannula groove 27. As such, the trocar seal housing 3 is unlocked or can be removed from the trocar cannula 5.

In FIGS. 13-14, in one aspect, the locking ring 21 is rotatable closely around the seal housing 3. The locking ring 21 has an axial split 26b and one or more lock tabs 23 extending from the locking ring 21. The axial split provides for an easily molded part with a single element per ring and allows the ring 21 to flex and thereby facilitate rotation. The seal housing 3 in one aspect has a ramp 3a adjacent to the seal housing aperture 25 to facilitate rotation and thus withdrawal of the tab 23. Grip tabs 26a extending along a portion or portions of the external surface of the locking ring 21 facilitates manipulation of the locking ring 21. The lock ring in one aspect is arranged with multiple local slots or

slits 26c that create or act as a leaf spring 26d to flexibly hold or bias the lock tabs 23 towards the seal housing aperture 25 and cannula groove 27.

In FIG. 15, the lock ring 21 in one aspect pivots or tips about an axis 24a perpendicular to the main or longitudinal axis 24b of the trocar cannula 5. One or more pivot pins 26e extend from or into the locking ring 21 connecting the lock ring 21 to the seal housing 3 and providing pivot points and a pivot axis generally perpendicular to the longitudinal axis 24a of the trocar cannula 5. As the lock ring pivots or tips, as shown by the direction arrow, for example, the lock tabs 23 extending therefrom engage or withdraw the trocar cannula groove 27 and seal housing aperture 25. A grip tab 26f extending from the external surface of the locking ring 21 assists in manipulating the ring 21. In one aspect, a plurality of lock rings and associated tabs and grips or a combination of lock rings described above are used to releasably secure the trocar seal housing 3 to the trocar cannula 5. As such, in one aspect, a trocar lock comprises a ring 21 having a tab 23 inwardly extending towards a center of the ring 21. The trocar seal housing 3 has an aperture 25 and the trocar cannula having a groove 27. The tab or tabs are movable from a first position in which the tab is engaged with the aperture, sized to receive the tab, in the trocar seal housing 3 and a second position in which the tab is engaged with the aperture in the trocar seal housing and the groove, sized to receive the tab, in the trocar cannula 5.

Referring now to FIGS. 16-18, the trocar cannula 5 with a seal 11, such as an o-ring or x-ring, e.g., an elastomeric ring with an x-shaped cross-section, situated in a groove 12 in the cannula 5 with a releasable bayonet lock 30 is shown. The cannula 5 also has one or more pins or tabs 33 that project radially out from an external surface of the cannula away from the longitudinal axis of the cannula 5. The pins 33 engage slots 31 in the seal housing such that as the pins move within the slots, the cannula is rotated (approximately 90° or a quarter of one revolution). Once the cannula 5 has been turned, the pins 33 are surrounded top and bottom, thus locking the cannula 5 to the seal housing 3. The slots 31 in one aspect starts with a ramped or curved opening extending parallel to the longitudinal axis of the cannula and curving towards a generally horizontal direction into a ramped end 31a with a small detent at the end of the ramp.

A cannula seal in one aspect is arranged such that it is axially compressed as the cannula rides up the ramp 31a. This adds friction, which helps prevent the cannula 5 and seal housing 3 from becoming separated unintentionally. However, with the added friction, having to overcome this friction can cause removal of the trocar seal housing from the trocar cannula to be difficult. A bayonet type attachment without additional friction, such as provided by axial seal compression, can reduce the effectiveness of preventing unintended detachment of the seal housing 3 from the cannula 5 during surgery as the instruments are manipulated through the trocar.

In FIG. 19, the lock tab 35 prevents or resists rotation of the seal housing 3 and thus guards against unintended detachment of the seal housing 3 from the trocar cannula 5. As such, the lock tab 35 is manipulated before the seal housing can be rotated and detached. In one aspect, the lock tab 35 is arranged as a leaf spring integral to the seal housing 3 with a grip tab 38 extending from the outer surface of the lock tab 35. The lock tab 35 has a cavity arranged to engage the pin 33 extending from the trocar cannula 5 thereby securing the trocar seal housing 3 to the cannula 5. The lock tab 35 is deflected distally, e.g., pivoted, towards slot 37 in the seal housing to move the tab 35 out of the path of the pin

33 extending from the cannula 5. With the lock tab 35 out of the path of the pin, the seal housing can be rotated and removed from the cannula. As such, in one aspect, a trocar lock comprises a post or pin 33 extending from an external surface of the trocar seal cannula. A slot or slots 31,37 are in the trocar seal housing and a resilient arm or lock tab 35 in the trocar seal housing 3 is adjacent to the slot or slots. The lock tab 35 is movable towards or in a longitudinal direction. As shown in FIG. 20, the lock tab 35 in one aspect comprises a plurality of leaf spring latches 34 integral to the cannula 5 having one or more projections or tabs 32 also extending from the cannula 5. The latches are releasably engagable with the apertures or slots 39 in the seal housing 3. The latches 34 are squeezed towards each other, as shown for example by the direction arrows, using grip tabs 36 moving the projections 32 out of the slots 39 in the seal housing 3 and thereby allowing the seal housing to rotate and be removed from the cannula 5.

Referring to FIG. 21, the trocar cannula 5 with a seal 11, such as an o-ring or x-ring, situated in a groove 12 in the cannula with a releasable socket lock 40 is shown. In one aspect, the cannula 5 has a plurality of apertures or slots or similarly situated groove 27 adjacent to the sealing groove 12 in the cannula 5. Socket lock 40 engages the apertures or groove in the cannula 5 to releasably secure the trocar seal housing 3 with the cannula 5.

In one aspect, the socket lock 40 comprises a plurality of generally circular or cylindrical beads or balls 43. One or more balls 43 protrude through the seal housing 3 and into the cannula groove 27, securing the trocar seal housing 3 to the trocar cannula 5. The balls 43 are held in position by a close fit collar 41. The collar 41 is arranged with two inside diameters 42a,b such that when the collar 41 is moved axially, the balls 43 are free to retract into the larger of the two inside diameters 42b, freeing the attachment of the seal housing 3 from the cannula 5. In one aspect, the collar is generally cylindrical having a first proximal portion 44a with a first diameter 42a and a second distal portion 44b with a second diameter 42b. The first diameter 42a generally corresponds to the diameter of the proximal end of the cannula and is smaller than the second diameter 42b. The second portion 44b is farther away from the proximal end of the cannula 5 than the first portion 44a of the collar 41. The collar 41 in one aspect comprises a ramp 44c connecting the two portions 44a,b and thus the inside diameters 42a,b which assists or facilitates the balls from moving or driving inwardly to the locked position when the collar is moved back to the original position. A return spring 45 axially in-line with a longitudinal axis of the trocar cannula 5 and connected to collar 41 provides a force to bias the collar towards the lock position thereby providing protection against unintended operation and automatic closure or locking of the seal housing 3 onto the cannula 5. As such, in one aspect, the trocar lock comprises a collar 41 and a plurality of balls 43 connected to the collar 41. The balls 43 are engagable with corresponding apertures in the trocar seal housing 3 and the trocar cannula 5. A return spring 45 connected to the collar 41 biases the collar 41 towards a distal end of the trocar cannula 5.

In one aspect, a third or additional proximal portion 44d of the collar 41 along with projections 46a from the seal housing 3 secure the return spring 45 to the collar and the seal housing 3. A retainer 46b, such as a snap or split ring, in conjunction with the second or distal portion 44b of the collar 41 secures the collar 41 to the seal housing 3 and the balls 43 when positioned in contact with the second portion 44b. Grip tabs 47 in one aspect extend from an outer

periphery of the collar to facilitate manipulation of the collar 41. Ramps or cuts 48 adjacent to or part of the apertures 49 of the seal housing 3 facilitate movement of the balls 43 into the locking position or engagement with the seal housing 3.

In one aspect, the balls 43 are loose secured between the collar 41 and seal housing 3. The balls 43 are spaced from each other along a perimeter around the cannula to provide additional strength and reduce unwanted motion. The lock balls 43 in one aspect are spherical, cylindrical, barrel-shaped or otherwise curved. The balls in one aspect are equally spaced or irregularly or randomly spaced. Positioning the balls towards each other, for example, providing two sets of two balls, however can assist in plastic molding operations as this eliminates or reduces the need for slides, which can simplify the mold of the trocar cannula 5 with apertures 27' as shown in FIG. 22. In one aspect, the balls are provided as a molded ring 143 incorporating generally spherical, cylindrical, barrel-shaped or generally curved components 43' movable as loose balls as shown in FIGS. 23-24. Such a molded ring can reduce cost and aid in assembly operations. As such, a ring 143 in one aspect connects the plurality of balls 43 to each other.

In one aspect, the socket lock 40 engages a plurality of discrete apertures 27' in the cannula 5 as shown in FIG. 25 instead of a continuous groove 27. As such, the balls 43 when engaged with the apertures 27' would be locked rotationally as well as axially. However, a continuous groove avoids having to orientate or align the lock with the cannula to first mate the components together.

In one aspect, to protect against unintended operation, a second motion is utilized before the collar 41 is retracted axially. As such, in one aspect, a latch is depressed before the collar 41 can be moved and, in one aspect, the collar 41 is first rotated before being able to be withdrawn axially. In FIG. 26, the collar 41 has one or more tabs 144 extending from the collar parallel to the longitudinal axis of the cannula 5. The collar 41 travels or rotates within a groove or channel 149b to engage/disengage slots 149a in the seal housing 3 or a slots 149a in a ledge extending from the outer periphery of the seal housing 3. In one aspect, the groove 149b extends along the periphery of the collar 41. As such, to first activate the release or unlocking of the seal housing 3 from the trocar cannula 5, the collar 41 is rotated to align the tabs 144 with the slots 149a to allow axial movement of the collar 41. Axially movement of the collar 41 subsequently allows the releasing of the seal housing 3 from cannula 5. Grip tabs 145 in one aspect extending from the collar 41 in-line or adjacent to the tabs 144 facilitate movement of the collar 41.

In one aspect, the return spring 45 also acts as a torsion spring when the collar is rotated before it can be retracted. For example, the spring is of a wound wire construction or a molded plastic part. In one aspect, the return spring 45 comprises a single large coil spring providing two biases, axially and rotationally, as shown for example by the direction arrows in FIG. 27 or multiple springs arranged axially at intervals around the inside of the collar. Multiple springs in one aspect are arranged to deflect sideways when the collar is rotated, thus acting as a torsional return spring.

Referring to FIGS. 28-30, the trocar cannula 5 with a seal 11, such as an o-ring or x-ring, situated in a groove 12 in the cannula 5 with a gate lock 50 is shown. In one aspect, the gate lock 50 engages a pair of parallel grooves 27 in the cannula 5. The gate lock 50 is a generally flat plate 51 with a keyhole-shaped aperture 53 through the plate. The keyhole-shaped aperture has a narrow portion 53a and wide portion 53b. As such, in one aspect, the trocar gate lock 50

11

comprises a substantially flat plate 51 having a keyhole slot 53 with a first aperture 53a being smaller than a second aperture 53b. The gate lock 50 slides from side to side in relation to the longitudinal axis of the trocar cannula 5. When the narrow portion 53a of the gate lock 50 engages the trocar seal housing 3, portions of the flat plate 51 or substantially planar tabs extending from the plate engage the groove 27 in the trocar cannula 5 thereby securing the trocar seal housing 3 to the trocar cannula 5. By moving or sliding the gate lock 50 in the opposite direction or extreme, the narrow portion 53a of the gate lock disengages the trocar cannula 5 as the seal housing 3 is positioned in the wide portion 53b of the gate lock 50. The gate lock 50 remains engaged with the trocar seal housing 3 via, for example, a groove or slot, but is removed or withdrawn from the groove 27 in the trocar cannula 5. Thus, the seal housing 3 can be removed from the trocar cannula 5. As such, the flat plate of the gate lock 50 in one aspect is movable in a direction perpendicular to a longitudinal axis of the trocar cannula from a first position in which the trocar seal housing is within the first aperture 53a and a second position in which the trocar seal housing is within the second aperture 53b. The flat plate 51 being in the first position engages with an aperture in the trocar seal housing 3 and the groove in the trocar cannula 5 and in a second position in which the flat plate 51 is engaged only with the aperture in the trocar seal housing 3.

In one aspect, the gate lock 50 is fitted with a return spring or detents to bias the gate lock 50 to one position, e.g., locked, versus another position, e.g., unlocked. In one aspect, the aperture 53 in the gate lock is generally round or oval in shape with one or more projections or detents 55 extending to the center of the gate lock as shown in FIG. 31.

Referring to FIGS. 32-33, the trocar cannula 5 with a seal 11, such as an o-ring or x-ring, situated in a groove 12 in the cannula 5 with a lever lock 60 is shown. In one aspect, the lever lock 60 engages a groove or slots 27 in the cannula 5 to secure the seal housing 3 to the cannula 5. The lever lock 60 has one or more lever arms 63 with one or more projections or tabs 61 operationally engaged with a corresponding groove or slots 27 in the trocar cannula 5. The trocar seal housing 3 has a corresponding apertures or slots 25 extending through a sidewall of the trocar seal housing 3. The tab 61 of lever lock 60 when engaged with the groove 27 in the trocar cannula 5 through the slot in the seal housing 3 secures the trocar seal housing to the cannula 5. The lever arms 63 are attached to the seal housing via a pivot pin 65 extending from/to one end of the lever arms 63 to/from the seal housing 3. Rotating or pivoting the lever lock from out of a substantially horizontal position as shown for example by the direction arrows causes the tab 61 of arm 63 to withdraw from the groove 27 in the trocar cannula 5 and/or the aperture 25 in the trocar seal housing 3. Thus, the seal housing 3 can be released from the trocar cannula 5. In one aspect, the lever arms 63 are arranged with a pivot axis 64a parallel to the longitudinal axis 62 of the cannula 5 or in one aspect with a pivot axis 64b at 90 degrees to the cannula longitudinal axis 62 as shown in FIG. 34. In one aspect, multiple lever locks are attached to the seal housing 3 and are arranged in like orientations or as mirror images as for example shown in FIG. 35. As such, in one aspect, the trocar lock 60 comprises at least one lever arm 63 pivotably movable relative to the trocar seal housing 3 and having a tab 61 extending from the at least one lever arm. The at least one lever arm is movable from a first position in which the tab engages with the aperture in the trocar seal housing 3 and the groove in the trocar cannula 5 and a second position in

12

which the tab 61 is engaged only with the aperture in the trocar seal housing 3 or is substantially withdrawn from the groove in the trocar cannula 5.

Referring to FIG. 36, the trocar cannula 5 with a seal 11, such as an o-ring or x-ring, situated in a groove 12 in the cannula 5 with a latch lock 70 is shown. In one aspect, the latch lock 70 are twin leaf spring latches 71 integral or attached to the cannula 5 with tabs or projections 77 that engage apertures or slots 25 in the seal housing 3 to secure the seal housing 3 to the cannula 5. The latches 71 are manipulated, e.g., squeezed, to withdraw the latches out of the slots 25 in the seal housing thereby allowing the seal housing 3 to be detached from the cannula 5. Grip tabs 73 extending from the latches 71 assist in manipulation, e.g., squeezing, of the latches. As such, the trocar lock 70 comprises at least one latch with a tab 77. The at least one latch is movable from a first position in which the tab 77 engages with the aperture in the aperture in the trocar seal housing 3 and the groove in the trocar cannula 5 and a second position in which the tab 77 is withdrawn from the groove in the trocar cannula 5.

In FIG. 37, the latch arm 71 has a bulbous head 75 that engages or springs into a recessed area or curved cavity 25' of the seal housing 3. The latch lock 70 in one aspect accommodates both tensile and compressive loads between the seal housing 3 and cannula 5 and therefore serves to position the parts in relation to each other. Additional secondary ledges or stops may also be used to further enhance the locking of the seal housing 3 to the cannula 5. The radii or curve at the top and bottom of the bulbous head 75 assists the latch lock 70 in engaging and disengaging, e.g., hook and unhook, from the seal housing 3. The recess 25' in the seal housing allows the latch lock 70 to be accessed without protruding from the seal housing 3. A release button that protruded could be unintentionally squeezed during normal surgical procedures, possibly resulting in unintended detachment of the seal housing 3 from the cannula 5. The functional or manipulated area 78 of the latch lock 70 relative to the cannula 5, for example, the area allowing the latch lock to flex, in one aspect is larger than the portion of the seal housing 3 that contacts the cannula seal 12. In one aspect, the seal housing 3 inner walls are tapered, ramped or curved. As such, the cannula seal is protected as the cannula 5 passes the latch slots or aperture 25' in the seal housing 3.

In FIG. 38, the latch lock 70 has generally triangular shaped latch heads 79. The triangular shaped latch heads 79 increase or assist in deflection of the latch lock 70 when mating the seal housing 3 and cannula 5. For example, the user would not need to hold the latch open as the parts are mated. The flat bottom 76 of the latch lock 70 ensures a positive lock while requiring a minimum of clearance to achieve the lock. An angled or overlapping latch can provide a more positive lock but may introduce more travel or play between the cannula 5 and seal housing 3. The latch lock 70 comprises of resilient or latches arms arranged external to the cannula seal lumen of the seal housing. As such, the cannula seal 11 and locking tabs or heads are generally in the same horizontal plane, resulting in a shorter seal to cannula joint. A shorter seal can be desirable for cost and ergonomic considerations. The latch lock 70 is tensile capable and as such the seal housing 3 is arranged to bottom out on the horizontal portion 76 of the latches 71.

Referring now to FIGS. 39-40, trocar seal housing 3 holds or encloses an instrument or septum seal 101 and a zero seal 103, e.g., a duckbill seal. The septum seal 101 and the zero seal 103 are coaxially aligned with each other and a longi-

tudinal or central axis of the trocar cannula **5** and seal housing **3**. The septum seal **101** has an aperture with its center substantially in-line with the center of the trocar seal housing **3** and/or cannula **5**. The septum seal **101** forms a seal to maintain pneumoperitoneum around instruments inserted through the seal's aperture while the zero seal **103** forms a seal to maintain pneumoperitoneum when no instrumentation is present in the trocar seal housing **3** and/or trocar cannula **5**. The septum seal **101** in one aspect is free to swing at its distal end in response to the insertion of instrumentation or in response to the manipulation of inserted instrumentation. In one aspect, the septum seal pendulates. For example, the septum seal at its distal end moves along generally curved line or arc in response to the insertion of instrumentation or in response to the manipulation of inserted instrumentation. In one aspect, excess material, levers, bellows, convolutions or other such means pivotally connect the instrument or septum seal **101** to the trocar seal housing **3**.

In one aspect, the zero seal **103** is fixed in place in contrast to the septum seal **101**. In one aspect, the septum seal **101** is pivotally attached to the seal housing **3** and substantially encompassed in the fixed zero seal **103**. In one aspect, the zero seal **103** is a duckbill seal fixed to the trocar seal housing **3**. As such, the zero seal **103** does not swing or pendulate to a large degree, if any, relative to the septum seal **101**. The zero seal **103** in combination with the septum seal **101** enables the trocar to accommodate a wide range of instrumentation diameters while minimizing the overall size of the trocar seal housing and trocar cannula.

A pendulous septum seal **101** with a zero seal attached to the pendulous septum seal can also be provided, such that pendent movement of the septum seal results in pendent movement of the zero seal. However, such a pendent trocar seal configuration can utilize a large amount of space to be accommodated within the trocar seal housing **3** and the trocar cannula **5** to enable the pendent movement of both the septum seal and the zero seal. This may result in a trocar seal with a relatively large axial length and overall diameter. The pendent septum seal **101** and a fixed zero seal **103** allows the trocar seal housing **3** and trocar cannula **5** to be sized with a reduced axial length and a reduced diameter relative to other trocar seals.

In one aspect, an instrument alignment channel **105** is juxtaposed to the septum seal **101**. The alignment channel **105** in one aspect is substantially fixed and/or rigid. In one aspect, the alignment channel **105** is a long tubular channel, which extends from the proximal opening of the trocar seal to above the aperture in the septum seal **101**. The alignment channel **105** serves to align or guide instrumentation during insertion and manipulation. By aligning the instrumentation and restricting the degree to which instrumentation can be manipulated, the alignment channel **105** decreases the likelihood that instrumentation can catch, tear, or otherwise disrupt the septum seal **101**. Also, the alignment channel being fixed restricts the degree to which an inserted instrument can be manipulated. As such, the degree of pendulous movement utilized to accommodate instrumentation with a wide range of diameters is decreased and also the size of the trocar seal can be more compact.

The alignment channel **105** in one aspect also enables the size of the septum seal aperture to be increased. For example, the aperture in the septum seal **101** is sized to prevent cat-eye leakage during extreme lateral movement of the instrumentation. However, with a fixed instrument alignment channel **105**, which is juxtaposed the septum seal **101**, lateral movement of inserted instrumentation is restricted

and a pendulous septum seal **101** accommodates the small amount of lateral instrumentation movement allowed by the alignment channel **105**. As such, the aperture in the pendulous septum seal can be enlarged and/or tolerances relaxed. The increased diameter of the septum seal aperture results in a reduction in the drag force produced during axial movement of inserted instrumentation. A reduction in instrumentation drag force for trocar seals can aid with positioning of instrumentation relative to the operative tissue. A reduction in instrumentation drag force also decreases the likelihood that a trocar seal housing **3** and cannula **5** will be dislodged from a body wall during withdrawal of an instrument. A reduction in instrumentation drag force can also result in less fatigue for the surgeon, for example, during complex surgical procedures.

In one aspect, the alignment channel **105** has a proximal end, a distal end, and a body portion **106a** extending between the proximal end and the distal end. The distal end extends into an outwardly tapered exit. In one aspect, the alignment channel **105** has an enlarged diameter at its distal end. The enlarged diameter allows for inversion of the septum seal **101** adjacent to the alignment channel **105** and prevents binding of the septum seal between the alignment channel and an instrument. For example, during withdrawal of an instrument, the septum seal **101** may invert and pull into the alignment channel **105**. In one aspect, if the alignment channel **105** is not sufficiently sized, a binding or lock up effect may occur which can prevent further withdrawal of the instrument. The alignment channel **105** in one aspect has a first diameter along its body portion **106a** to align instruments and to prevent excessive lateral movement of the inserted instruments. The alignment channel **105** in one aspect has a second diameter at its distal end **106b**, which is larger than the first diameter. The second diameter is sized such that it can accommodate a two wall thicknesses of the septum seal and/or the largest instrument diameter that can pass through the first diameter of the alignment channel. The axial length of the enlarged diameter distal end **106b** is sized such that the septum seal **101** can invert but not extend into a body portion **106a** of the alignment channel with a smaller diameter portion of the alignment channel **105**.

The alignment channel **105** in one aspect has an entry **107** at its proximal end that aids with insertion of instrumentation and serves to guide instrumentation into the alignment channel **105**. In one aspect, the entry is generally funneled and/or tapered. As such, in one aspect, the alignment channel **105** has a proximal end and a distal end. The proximal end extends into an outwardly tapered entry. In one aspect, the tapered entry has a diameter that is larger than the diameter of the outwardly tapered exit. In one aspect, the entry has a matte finish or provides an anti-reflective or non-glare finish, coating or layer. The anti-reflective entry prevents or reduces glare and/or light from a laparoscope from being reflected back or towards the user. The entry in one aspect has a guard rail **109** at the proximal portion of the entry. The guard rail **109** in one aspect comprises a raised wall which generally encircles the top or external surface of the entry extending parallel to the longitudinal cannula axis from an end cap or wall **110** of the trocar seal housing **3**. In one aspect, the trocar seal housing **3** has opening in an end cap of the trocar seal housing and an alignment channel **105** extends from the end cap **110**. The septum seal **101** positioned between the alignment channel **105** and the zero seal **103**. The zero seal **103** is adjacent to a proximal end of the cannula **5**. In one aspect, the guard rail comprises a raised portion substantially outlining a periphery of the generally funneled entry **107**. In one aspect, the guard rail integrated with or separate

from the entry **107** and is a raised portion substantially outlining a periphery of an opening in a proximal end of the seal housing **3**. The guard rail **109** provides a tactile hard stop to limit or prevent a surgeon from laterally sliding an instrument out of the entry **107** or alignment channel **109** during insertion of an instrument into the trocar seal housing **3**.

Referring to FIG. **41**, in one aspect, the pendulous septum seal **101** is protected with a sleeve or shield **108** that is nested into the septum seal **101** and pivots with the septum seal **101**. The shield prevents instruments from catching and/or tearing the septum seal. The shield **108** can also prevent the septum seal from inverting during instrument withdrawal and in one aspect is a polyethylene sleeve. The shield **108** can also reduce the instrumentation drag force and in one aspect is used in combination with the instrument alignment channel **105**. The shield **108** in one aspect partially surrounds the alignment channel **105**. In one aspect, the shield **108** is positioned axially between the alignment channel **105** and the septum seal **101**. In one aspect, the shield **108** extends along the septum seal **101** between the alignment channel **105** and the septum seal **101**.

In one aspect, a trocar seal housing **3** has a stopcock body **112**. For example, the trocar seal housing has an integrally luer fitting inlet or molded integral luer fitting **111** and a snap fitted stopcock body **112**. The stopcock body **112** in one aspect comprises a center bore and a lever. The trocar seal housing **3** with the integral luer fitting **111** is injection molded with polycarbonate. The stopcock body **112** is injection molded with polyethylene. The stopcock center bore in one aspect has a barb **114** at its distal end, which engages with a shelf on the integral luer fitting **111** to secure the stopcock body to the integral luer fitting. The trocar seal housing **3** in one aspect can have a separately assembled stopcock/luer fitting, which is then bonded or ultrasonically welded to the trocar seal housing **3** (e.g., FIG. **42**). However, as shown in FIG. **41**, with the trocar seal housing **3** with an integrally molded luer fitting and stopcock body, bonding or welding the stopcock can be avoided thereby eliminating at least one assembly process and one molded component thereby reducing the overall cost to produce the trocar seal. In one aspect, the integral luer fitting **111** is incorporated with and extends from the trocar seal housing **3** in a first direction for a first distance. The first direction is substantially perpendicular to a longitudinal axis of the trocar cannula **5**. The stopcock **112** has a central bore extending substantially parallel to the longitudinal axis of the trocar cannula **5** and is fitted into the integral luer fitting **111**. The stopcock **112** also has a lever movable by a user and extends in a second direction for a second distance. The first direction corresponds to the second direction and the first distance corresponds to the second distance.

In one aspect, the trocar seal housing **3** has an aperture with a center positioned along a first axis and is arranged to communicate gas to the trocar cannula **5**. The first axis is substantially perpendicular to a longitudinal axis of the trocar cannula. The integral luer fitting **111** has an aperture with a center positioned along the first axis and is arranged to be coupled to an insufflation gas line. The stopcock **112** has a central or center bore that has a first aperture with a center and a second aperture with a center. The center bore is movable from a first position to a second position. In the first position, the center of the first aperture and the center of the second aperture are substantially aligned with the first axis. In the second position, the center of the first aperture and the center of the second aperture are out of alignment with the first axis. Examples of trocars with stopcocks or

configurable with stopcocks are described in U.S. patent application Ser. No. 10/264,550, filed Oct. 4, 2002, U.S. patent application Ser. No. 11/000,123, filed Nov. 30, 2004, and U.S. patent application Ser. No. 10/776,387, filed Feb. 10, 2004, and U.S. Provisional Patent Application No. 60/529,455, filed Dec. 12, 2003, U.S. Provisional Patent Application No. 60/492,949, filed Aug. 6, 2003, U.S. Provisional Patent Application No. 60/312,683, filed Aug. 14, 2001, the entire disclosures of which are hereby incorporated by reference as if set in full herein.

In one aspect, as shown for example in FIGS. **44-46**, a luer fitting is integrated with a stopcock lever to form a spigot **120**. With this configuration, the spigot **120** can double as a handle. As such, the spigot **120** can rotate from a high profile position to a low profile position reducing the overall profile of the trocar seal. A reduced trocar seal profile allows for greater manipulation of the trocar and enables trocars to be more closely spaced on a body wall. For example, the trocar seal housing with an integrated or combined stopcock lever and luer fitting provides a reduced "footprint" (plan view) or the area taken up by the trocar.

In one example, in a laparoscopic surgery three to five trocar ports can be used. Each trocar is provided with a stopcock. However, only one trocar has an open stopcock with an insufflation line attached. The stopcocks on the other the trocar are not used and are therefore closed. As shown for example in FIGS. **42-43**, even though the levers are in the closed position, however, the luer inlet fitting still extends outwardly from the seal and so increases the space occupied by the trocar. In addition, the lever may only be swung 90 degrees to either side and due to geometry conditions, the lever still projects out from the trocar. As such, a closed stopcock can occupy more space than an open stopcock as two objects project outwardly from the trocar. Also, a fixed luer inlet fitting on a trocar can contact the patient's skin during extreme manipulation of the trocar, which can restrict instrument manipulation or trauma to the skin.

In one aspect, a separate stopcock/luer inlet assembly added to the trocar seal housing can result with the stopcock protruding about 1 1/8" from an approximate 1" diameter seal. This changes the footprint to an approximate 1" by 2 1/8" oval versus an approximate 1" circle for a non-stopcock version. In one aspect, a trocar seal housing **3** integrates the stopcock bore and luer fitting inlet into the housing. This reduces the overhang by about 1/4", reducing the footprint. Also, at least one part and at least one assembly operation is eliminated. Overhang is also reduced to about 7/8" versus about 1 1/8". In one aspect, a trocar seal housing **3** is provided which eliminates a fixed inlet **111** which protrudes from the trocar housing even when the valve lever is turned parallel to the body of the trocar housing (off position). In one aspect, the stopcock/inlet assembly is transformed into a combination lever and fitting, spigot **120**. In the "off" position, the spigot **120** protrudes about 3/8" or so from 1" diameter housing, as the spigot can be turned past about 90 degrees to lay alongside the housing. In one aspect, the trocar cap traps the spigot in a valve bore when assembled. As such, a cap ledge in one aspect is provided above the spigot.

The spigot **120** with a reduced profile, especially when it is not in use and therefore closed, in one aspect, comprises a combined lever and luer inlet fitted to pivot to the trocar seal housing **3**. In the open position, the spigot extends directly outward from the housing **3** and occupies an area similar but less than a stopcock and luer inlet fitting. When the spigot **120** is swung to the closed position, it lies closely alongside the trocar housing **3** and occupies a reduced area. In particular, no luer inlet fitting protrudes outwardly from

a closed and unused fitting. In one aspect, the spigot **120** is fitted to a closed ended pivot bore **121** and is retained by a ledge **122** extending locally from the seal housing **3** or an end cap of the seal housing **3**. On the other end of the spigot **120**, an insufflation gas fitting end **125**, e.g., a threaded end, operationally connects to an insufflation gas line. Near the closed ended pivot bore, a insufflation outlet aperture or hole **126** provides gaseous communication between the inlet or insufflation fitting end **125** and the cannula via associated apertures or channels provided in the cannula **5** and seal housing **3**. The opposing end of the closed ended pivot bore has a pivot pin extending into the ledge **122** securing the spigot **120** in a pivotable relation with the seal housing **3**. A hole or aperture **127** may be provided on the seal housing adjacent to spigot **120** to facilitate molding of the seal housing components.

To prevent unintended rotation, in one aspect, one or more detents **123** engaging with a corresponding cavity **124** on the end cap or wall or extended ledge **122** are provided to retain the spigot **120** in a particular positions, e.g., open and closed. In one aspect, the lever is able to rotate more than 90 degrees so as to be positioned more closely along the seal housing and therefore occupy as little space as possible. With the spigot **120** swung over alongside the seal housing, skin contact is diminished. As such, in one aspect, a pivotable spigot **120** is connected to the trocar seal housing **3**. The spigot **120** has an insufflation gas fitting on one end **125** and movable between a first position to position the gas fitting extending away from and/or perpendicularly to a longitudinal axis of the trocar cannula **5** and the trocar seal housing **3** and a second position to position the gas fitting extending close to and/or positioned substantially near the seal housing **3**.

Referring now to FIGS. **47-49B**, an optical obturator **10** in one aspect is configured to separate muscle fibers and tissue during placement of the trocar across a body wall. The trocar seal housing **3** and cannula **5** with the inserted obturator **10** is alternately twisted back and forth as a small axial force is applied to traverse a body wall. The cross sectional profile of the obturator tip **10a** is configured such that its width is greater than its length. Rotation of the obturator **10** causes muscle fibers and tissue to separate along natural planes. The optical obturator **10** in one aspect is formed of a transparent high-flow polycarbonate material to enable visualization of tissue fibers during traversal across a body wall. Visualization can be achieved by inserting a laparoscope with an attached camera into the inside diameter of the obturator **10**. The tissue is viewed through the tip **10a** of the obturator as the trocar traverses a body wall. In one aspect, a laparoscope is allowed to be positioned within a portion of the obturator tip **10a** enhancing visualization. Referring to FIG. **49B**, in one aspect, the obturator **10** has a longitudinally extending lumen **10g** from a proximal open end **10e** to a distal closed end **10f**. The lumen **10g** is sized and arranged to receive a laparoscope and the obturator **10** is sized to be slidably movable in the lumen of the trocar cannula **5**.

In one aspect, the tip portion of the obturator is molded. The injection mold for the obturator is configured such that the distal tip of the obturator, which in one aspect is the portion that contacts and separates body wall tissue, does not include any mold parting lines and/or injection molding gates. The tip **10a** therefore is smooth with a high degree of clarity and is free of any artifacts produced as a result of injection molding such as parting line flash, parting line mismatch, gate recesses, gate remnants, and gate blush. An optical obturator **10** with these artifacts from injection molding may catch body wall tissue such as the peritoneum.

The image produced through the optical obturator is also enhanced, as the tip of the obturator does not include parting lines, a gate remnant, a gate recess, or gate blush, all of which may reduce the optical clarity of an optical obturator.

Referring now to FIGS. **50-55**, the access port comprises a seal housing **3** releasably attached to a cannula **5**. The seal housing **5** holds a pendulous septum seal **101**, which has a convolution **115** of excess material at its proximal end. The convolution **115** enables the septum seal **101** to pivot in response to the insertion of an instrument such that the septum seal can align itself with the inserted instrument. The convolution **115** also allows the septum seal **101** to pivot during off-axis movement of an inserted instrument such that a seal is maintained between the septum seal **101** and the inserted instrument. The septum seal **101** is designed with the convolution **115** such that there are no undercuts on the part. By providing a part with no undercuts, the septum seal **101** can be transfer molded with relatively simple multi-cavity mold tooling. In one aspect, convolutions **115**, excess material, levers, bellows, or other such means pivotally connect the instrument or septum seal **101** to the trocar seal housing **3**.

In one aspect, the trocar seal comprises a septum shield **116** adjacent to the septum seal **101**. The septum shield is arranged such that it abuts the distal portion of the alignment channel **105**. In one aspect, the septum shield **116** has a proximal flat portion in contact with the alignment channel **105**. This minimizes the axial movement of the septum shield **116** during withdrawal of an inserted instrument. The septum seal in one aspect comprises an annular rib positioned between the alignment channel **105** and the septum shield **116**. The annular rib for example abuts the distal portion of the alignment channel **105** and extends perpendicular to the longitudinal axis of the trocar cannula. The annular rib in one aspect holds the shield in place in the septum shield. In one aspect, the septum shield **116** partially surrounds the alignment channel. In one aspect, the septum shield **116** is positioned axially between the alignment channel and the septum seal **101**. In one aspect, the septum shield **116** extends along the septum seal **101** between the alignment channel **105** and the septum seal **101**.

The septum seal **101** in one aspect is configured with varying wall thicknesses in the convolution portion **115** of the seal **101** to minimize axial movement of the septum seal **101** during the insertion or distal advancement of an instrument. For example, the outer wall of the convolution **115** can be configured with a thicker wall than the inner wall of the convolution **115**. This would allow the septum seal **101** to pivot yet would inhibit the axial movement of the septum seal **101** in the distal direction.

The septum seal **101** in one aspect has a plurality of radially spaced vertical ribs on an outside wall or surface of the convolution **115**. The radially spaced ribs allow the septum seal **101** to pivot yet inhibits the axial movement of the septum seal **101** in the distal direction. The most proximal portion of the convolution **115** in one aspect is arranged to have a thinner wall thickness than either the outer wall or the inner wall of the convolution **115**. This enables the septum seal **101** to easily pivot yet inhibits the axial movement of the septum seal **101** in the distal direction. The convolution **115** in one aspect comprises a plurality of radially spaced ribs, which would span the gap between the outer wall of the convolution and the inner wall of the convolution. The ribs would be thin enough to allow the septum seal **101** to pivot yet would inhibit the axial movement of the septum seal **101** in the distal direction. By minimizing or inhibiting the axial movement of the septum

seal **101** in the distal direction this allows or facilitates the trocar seal to be arranged more compactly with a reduced overall height.

In various aspects, the trocar seal housing **3** has opening in an end cap **110** of the trocar seal housing and an alignment channel **105** extends from the end cap **110**. The septum seal **101** is positioned between the alignment channel **105** and the zero seal **103**. The zero seal **103** is also adjacent to a proximal end of the cannula **5**. The access port in one aspect comprises a seal housing **3**, which is releasably attached to the cannula **5** via for example cantilever snap arms **7** to enable removal of tissue specimens and to enable rapid desufflation of a body cavity. Suture ties loops or eyes **8** in one aspect are generally circular apertures extending from opposing sides of the cannula **5**. The access port in one aspect accommodates a blunt optical obturator arranged to be used in conjunction with an inserted laparoscope to allow visualization of tissue during traversal across a body wall. The optical obturator **10** in one aspect has a laparoscope lock **10b** arranged to allow rotation of the laparoscope within the obturator while preventing axial movement of the laparoscope within the obturator.

The trocar seal housing **3** and cannula **5** in one aspect comprises multiple components. The trocar cannula **5** is an injection molded polycarbonate. Attached to the trocar cannula **5** is an EPDM (Ethylene Propylene Diene Monomer) O-ring seal. In one aspect, the cannula seal **11** is overmolded seal comprising of silicone, KRATON, styrene-ethylene/butylene-styrene, copolyester, copolyamide, thermoplastic rubber, thermoplastic vulcanite, C-FLEX, or a thermoplastic elastomeric material molded into a polycarbonate trocar cannula. The trocar seal housing **3** has an injection molded polycarbonate housing, an injection molded polycarbonate cap, an injection molded polycarbonate shield, a compression molded polyisoprene septum seal **101**, a compression molded polyisoprene duckbill valve **103**, and an injection molded polyethylene stopcock body **112**. To assemble the trocar seal, the stopcock lever is snap fitted into the integral luer fitting **111** of the housing **3**. The duckbill valve **103** is seated into the housing **3**. The septum seal **101** is nested into the duckbill valve **103**. The cap is press fitted onto the housing **3**. The assembled trocar seal housing **3** is snap fitted onto the trocar cannula **5**.

The optical obturator **10** in one aspect comprises three components; an injection molded polycarbonate obturator shaft **10d**, an injection molded polycarbonate knob **10c**, and an injection molded polycarbonate scope lock **10b**. The scope lock retains the axial position of an inserted laparoscope. Assembly of the obturator in one aspect comprises snap fitting the knob onto the obturator shaft. The scope lock snap fits onto the knob.

In one aspect, the trocar cannula **5** and o-ring are formed of reusable materials enabling autoclave sterilization and re-use of the cannula and o-ring. In one aspect, the optical obturator shaft is formed of an extruded plastic tube or a metal tube. The tip portion **10a** is bonded to the tube or overmolded onto the tube. In one aspect, the zero seal **103** is a double duckbill valve, a single duckbill, a gel seal, an overlapping flap seal, and/or a slit seal. In one aspect, the septum seal **101** and the zero seal **103** may be coated with parylene, silicone grease, mineral oil, glycerin, Teflon, silicone oil, or a combination thereof to reduce instrument drag forces. The septum seal **101** and zero seal **103** in one aspect is chlorinated or plasma etched to reduce instrument drag forces.

In various aspects, the trocar lock is arranged to resist axial forces directed to separate the trocar cannula from the

trocar seal housing. In one example, a trocar lock has a tab extending from the trocar lock and is movable through an aperture in the trocar seal housing to a groove in the trocar cannula. In one example, a trocar lock extends from the trocar cannula and has a tab that is engagable with a slot in the trocar seal housing. In various aspects, a trocar seal housing is provided which easily attaches to and easily detaches from a trocar cannula, has a pendulous septum seal with a zero seal, a fixed instrument alignment channel, a shield protecting the septum seal, an instrument alignment channel with an enlarged space to allow for inversion of the septum seal, an optical obturator with a tip that has a high degree of optical clarity and/or with an outer surface that is smooth, or any combination thereof. Examples of pendulous seals are described in U.S. patent application Ser. No. 10/264,550, filed Oct. 4, 2002, the entire disclosure of which is hereby incorporated by reference as if set in full herein. Examples of shielded septum seals are described in U.S. patent application Ser. No. 11/000,123, filed Nov. 30, 2004, and U.S. Provisional Patent Application No. 60/529,455, filed Dec. 12, 2003, the entire disclosures of which are hereby incorporated by reference as if set in full herein. Examples of optical obturators are described in U.S. patent application Ser. No. 10/956,167, filed Oct. 1, 2004, and U.S. Provisional Patent Application No. 60/508,390, filed Oct. 3, 2003, the entire disclosures of which are hereby incorporated by reference as if set in full herein.

Although the present invention has been described in certain specific aspects, many additional modifications and variations would be apparent to those skilled in the art. It is therefore to be understood that the present invention may be practiced otherwise than specifically described, including various changes in the size, shape and materials, without departing from the scope and spirit of the present invention. Thus, embodiments of the present invention should be considered in all respects as illustrative and not restrictive.

The invention claimed is:

1. A surgical access port comprising,

a trocar seal housing configured to sealingly engage surgical instruments inserted therethrough, the trocar seal housing defining a central longitudinal axis, and the trocar seal housing comprising:

a valve bore disposed on an external surface of the trocar seal housing; and

an aperture in the external surface of the trocar seal housing, the aperture fluidly coupled to the valve bore;

a spigot pivotally coupled to the valve bore, the spigot comprising a gas fitting end extending from the valve bore, and an aperture end in gaseous communication with the gas fitting end, the aperture end positioned in the valve bore;

and the spigot pivotable between a low profile configuration wherein the gas fitting end is positioned substantially near the external surface of the trocar seal housing and the aperture end is out of alignment with the aperture in the external surface of the trocar seal housing, and an extended configuration wherein the gas fitting end extends away from the trocar seal housing and the aperture end is aligned with the aperture in the external surface of the trocar seal housing to provide gaseous communication between the gas fitting end and the trocar seal housing.

2. The surgical access port of claim 1, further comprising an end cap positioned at a proximal end of the trocar seal housing retaining the spigot within the valve bore the end cap comprising a cavity formed therein, and the spigot

further comprising a detent thereon engageable with the cavity with the spigot in a predetermined position.

3. The surgical access port of claim 2 wherein the end cap comprises a ledge extending therefrom, and wherein the cavity is formed in the ledge.

4. The surgical access port of claim 2, wherein the predetermined position comprises an open position defined by the extended configuration of the spigot.

5. The surgical access port of claim 2, wherein with the spigot in the extended configuration, a gaseous communication path extends generally perpendicularly to the central longitudinal axis adjacent the gas fitting end, generally parallel to the central longitudinal axis within the spigot within the valve bore, and generally perpendicular to the central longitudinal axis through the aperture end and the aperture in the trocar seal housing.

6. The surgical access port of claim 2, further comprising a trocar cannula removably attached to the trocar seal housing.

7. The surgical access port of claim 6, wherein the trocar cannula comprises two cantilever arms extending therefrom and wherein the trocar seal housing comprises two mating slots formed therein, each mating slot positioned to receive a corresponding one of the cantilever arms when the trocar seal housing is attached to the trocar cannula.

8. The surgical access port of claim 7, wherein each of the cantilever arms has a hook at a free end thereof to engage the mating slots of the trocar seal housing.

* * * * *

专利名称(译)	手术入口		
公开(公告)号	US9833259	公开(公告)日	2017-12-05
申请号	US14/636252	申请日	2015-03-03
[标]申请(专利权)人(译)	应用医疗资源		
申请(专利权)人(译)	应用医疗资源CORPORATION		
当前申请(专利权)人(译)	应用医疗资源CORPORATION		
[标]发明人	MCGINLEY KIMBALL B KAHLE HENRY TAYLOR SCOTT V JOHNSON GARY M		
发明人	MCGINLEY, KIMBALL B. KAHLE, HENRY TAYLOR, SCOTT V. JOHNSON, GARY M.		
IPC分类号	A61B17/34 A61M13/00 A61B17/02 A61B17/00 A61M39/22		
CPC分类号	A61B17/3423 A61B17/0218 A61B17/3462 A61M13/003 A61B17/3417 A61B17/3474 A61M2039/229 A61B2017/00477 A61B2017/347 A61B2017/3419 A61B2017/3464 A61M39/223 A61B2017/0046		
优先权	11/549926 2013-04-30 US 60/726825 2005-10-14 US 60/828515 2006-10-06 US		
其他公开文献	US20150173792A1		
外部链接	Espacenet USPTO		

摘要(译)

提供外科进入端口或套管针。套管针具有套管针密封壳体 and 套管针套管，套管针套管具有可通过套管针密封壳体和套管针套管插入的光学填充物。套管针被配置成进入体腔，以维持正压并防止在腹腔镜手术中使用的手术吹入气体的损失。套管针密封壳体可以可释放地连接到套管针套管上。套管针密封壳体还可以具有护罩和/或对准通道，其提供保护或辅助操作仪器和容纳在套管针密封壳体中的零密封。

