



US006881213B2

(12) **United States Patent**  
**Ryan et al.**

(10) **Patent No.:** **US 6,881,213 B2**  
(45) **Date of Patent:** **Apr. 19, 2005**

(54) **DEVICE AND METHOD TO EXPAND  
TREATMENT ARRAY**

(56) **References Cited**

(75) Inventors: **Thomas P. Ryan**, Flemington, NJ (US);  
**David Y. Yuan**, Somerset, NJ (US);  
**Roddi J. Simpson**, Jersey City, NJ  
(US); **Scott A. Ciarrocca**, Stockton, NJ  
(US); **Alexander J. Sinton**,  
Doylestown, PA (US)

(73) Assignee: **Ethicon, Inc.**, Somerville, NJ (US)

(\*) Notice: Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 179 days.

(21) Appl. No.: **10/278,235**

(22) Filed: **Oct. 23, 2002**

(65) **Prior Publication Data**

US 2004/0002748 A1 Jan. 1, 2004

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 10/186,389, filed on  
Jun. 28, 2002, now abandoned.

(51) **Int. Cl.**<sup>7</sup> ..... **A61B 18/18**

(52) **U.S. Cl.** ..... **606/41; 607/101**

(58) **Field of Search** ..... 606/41-50; 607/96,  
607/101, 102

**U.S. PATENT DOCUMENTS**

5,722,401 A	*	3/1998	Pietroski et al. ....	600/374
5,769,880 A		6/1998	Truckai et al.	
5,817,092 A		10/1998	Behl	
5,827,276 A		10/1998	Le Veen et al.	
6,050,992 A		4/2000	Nichols	
6,123,718 A	*	9/2000	Tu et al. ....	607/113
6,488,673 B1	*	12/2002	Laufer et al. ....	604/516
6,589,238 B2	*	7/2003	Edwards et al. ....	606/41
6,625,486 B2	*	9/2003	Lundkvist et al. ....	604/21


\* cited by examiner

*Primary Examiner*—Roy D. Gibson

(57) **ABSTRACT**

A medical device is provided and includes an elongated tube that has a longitudinal axis and an expandable member attached to the tube. The expandable member is expandable from a collapsed configuration to an expanded configuration. A plurality of electrodes is attached to the expandable member. The electrodes are used to emit energy. Each of the electrodes is arranged generally coaxially relative to the tube when the expandable member is in its collapsed and expanded configurations.

**25 Claims, 9 Drawing Sheets**

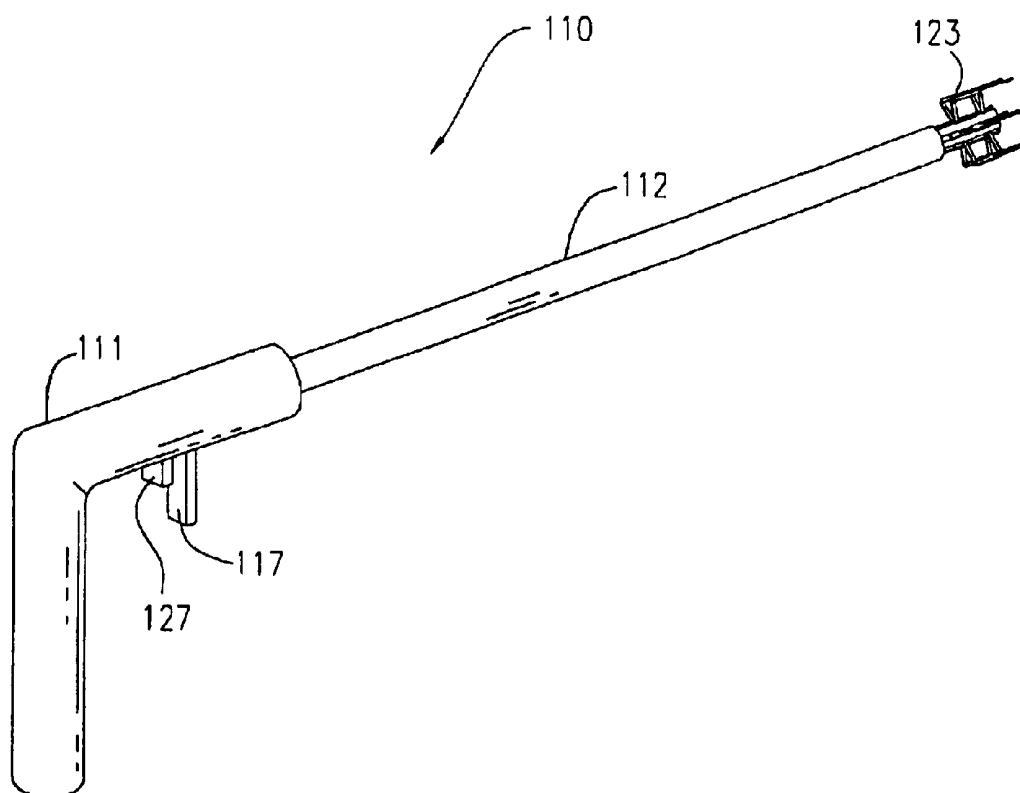

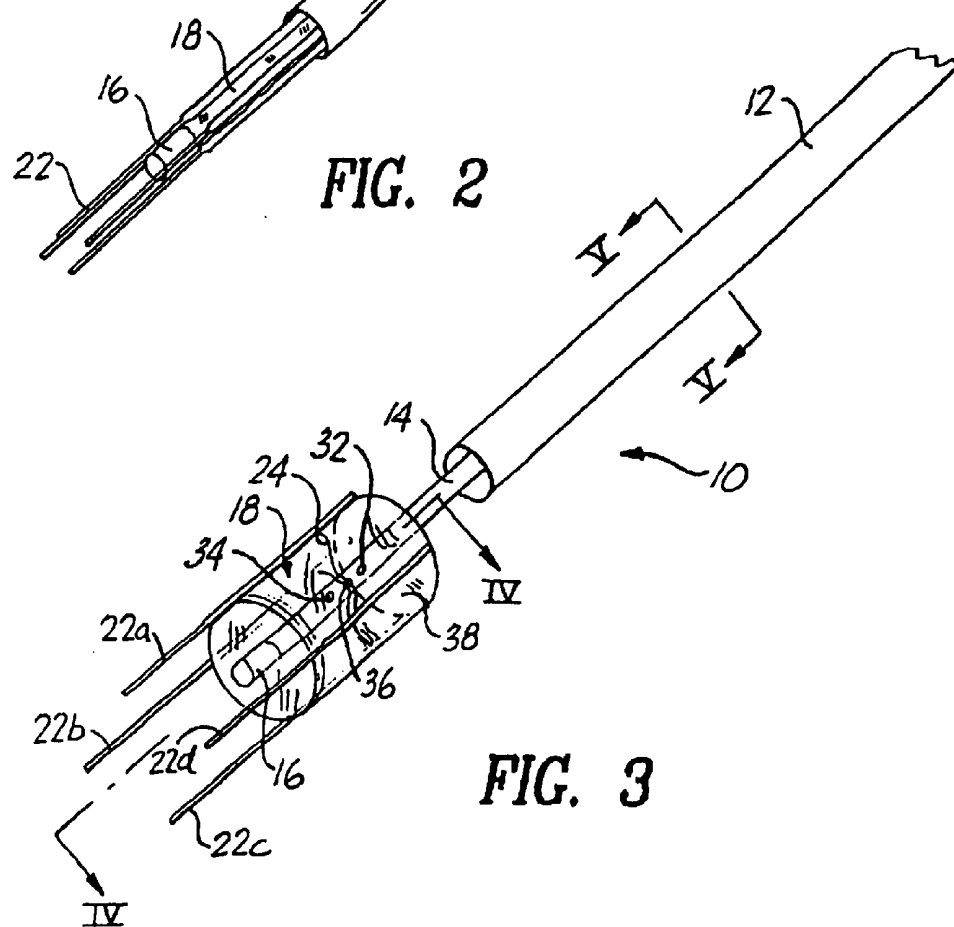
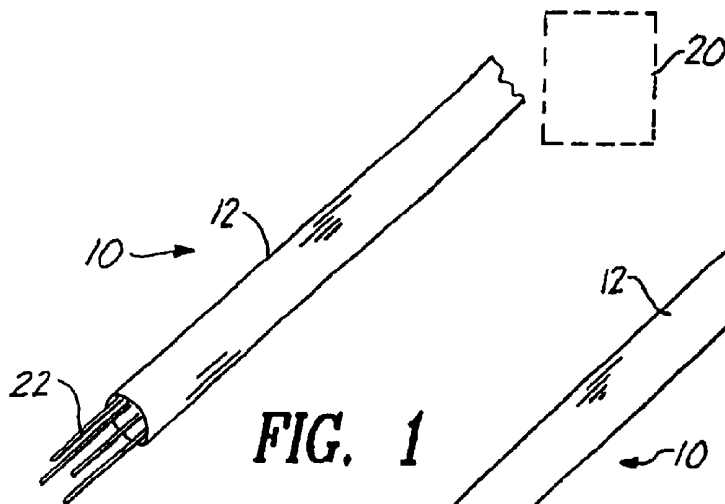


FIG. 3

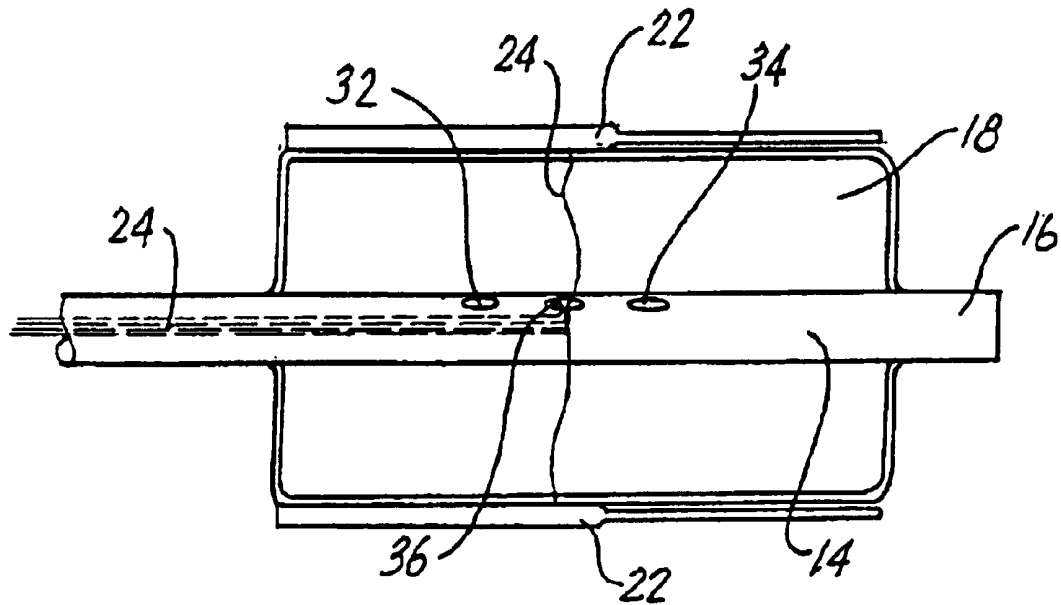


FIG. 4

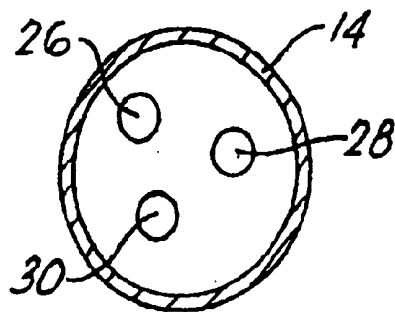


FIG. 5

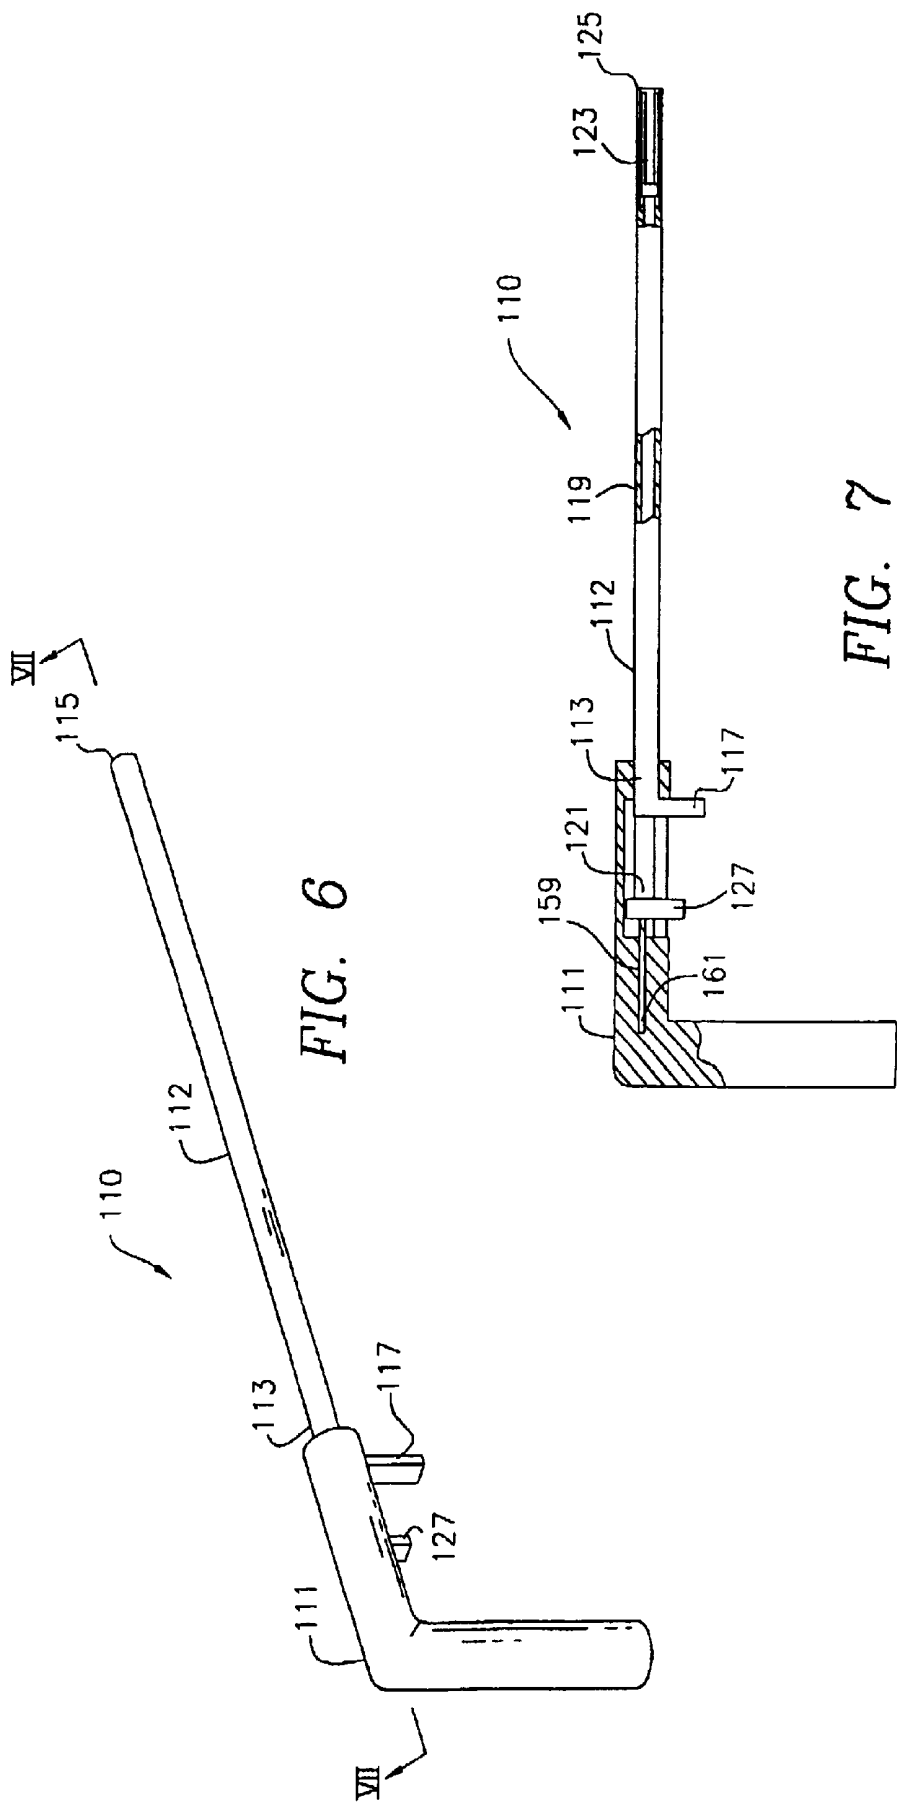
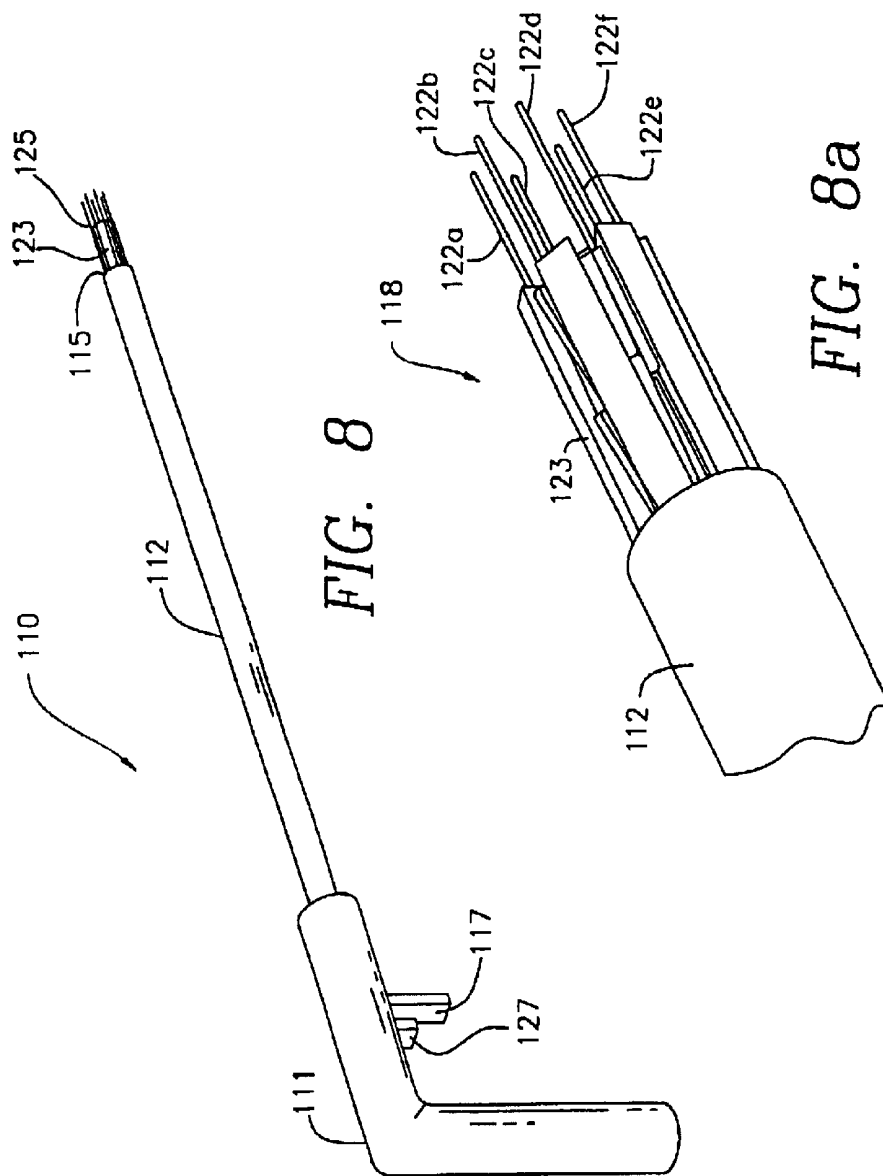


FIG. 6

FIG. 7



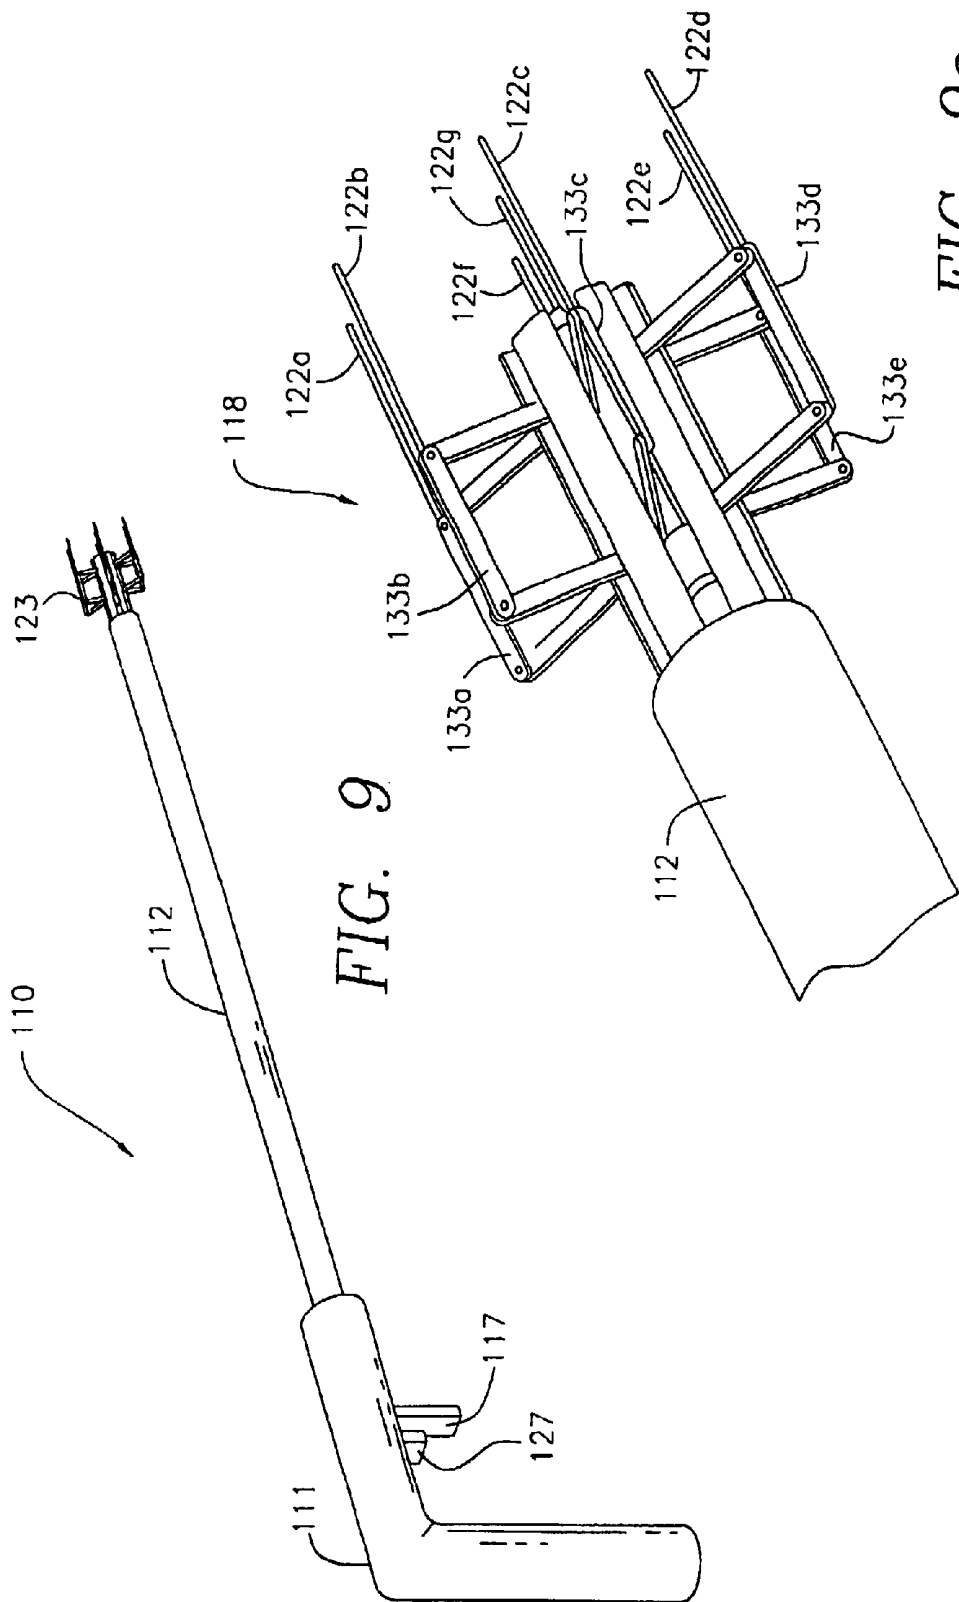


FIG. 9

FIG. 9a

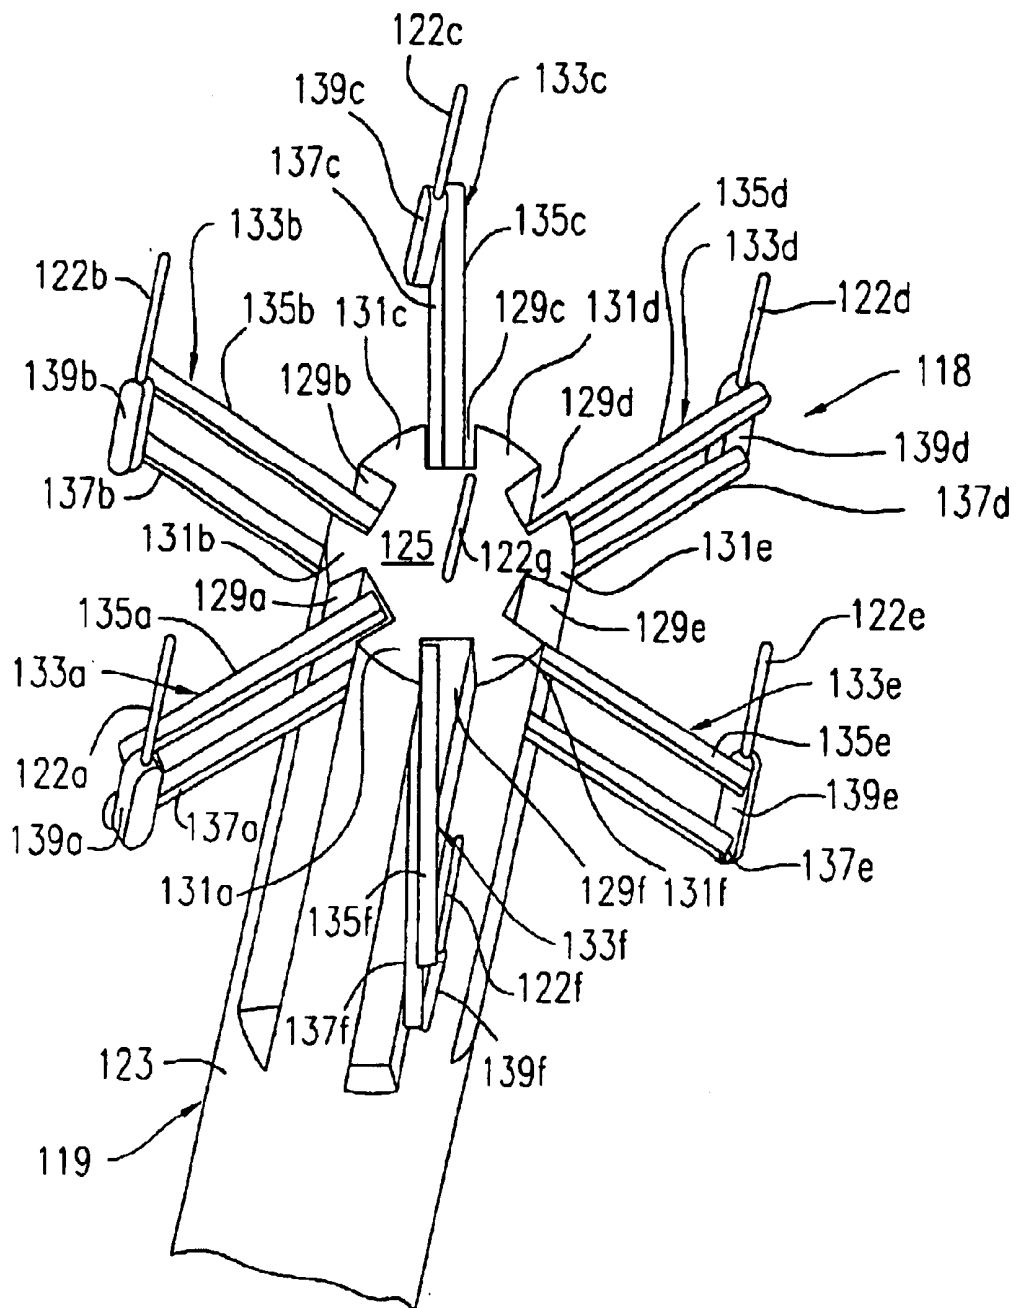


FIG. 9b

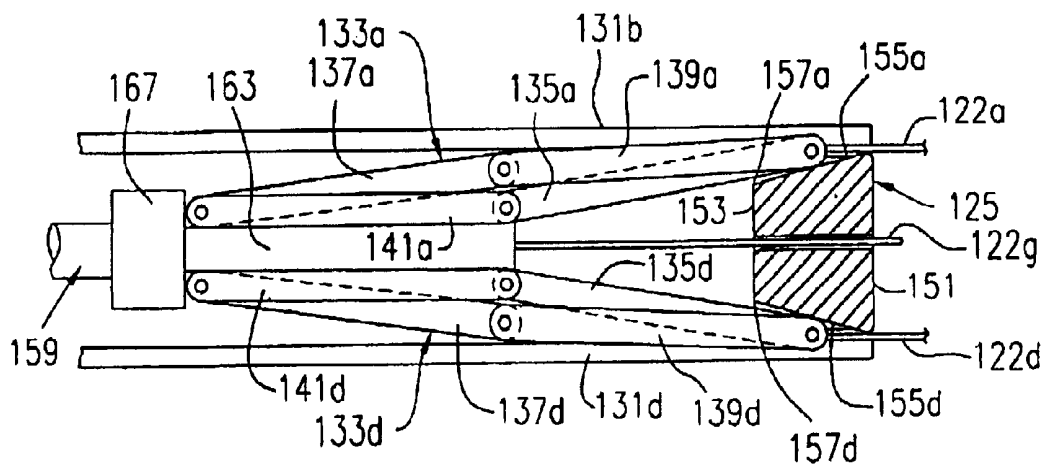


FIG. 10a

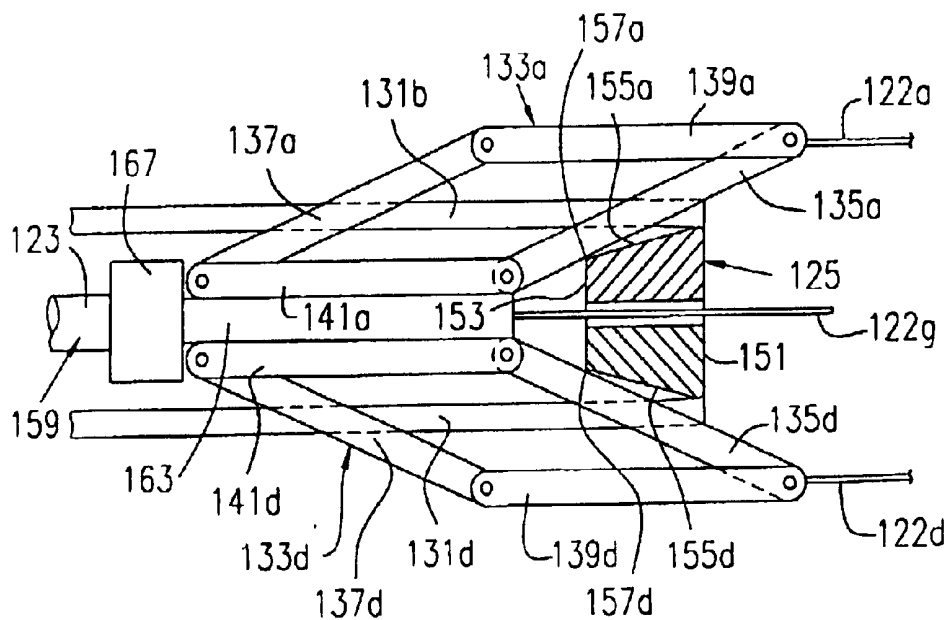


FIG. 10b

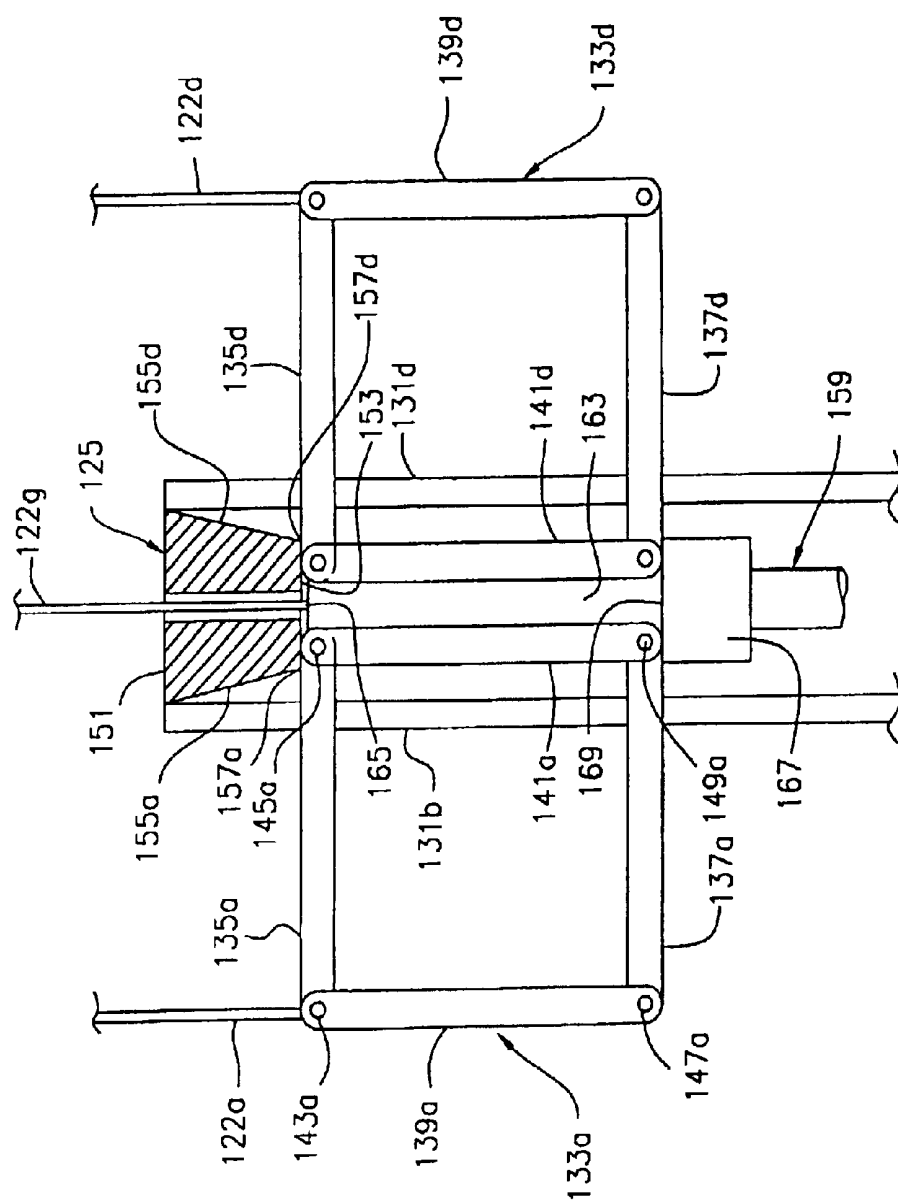
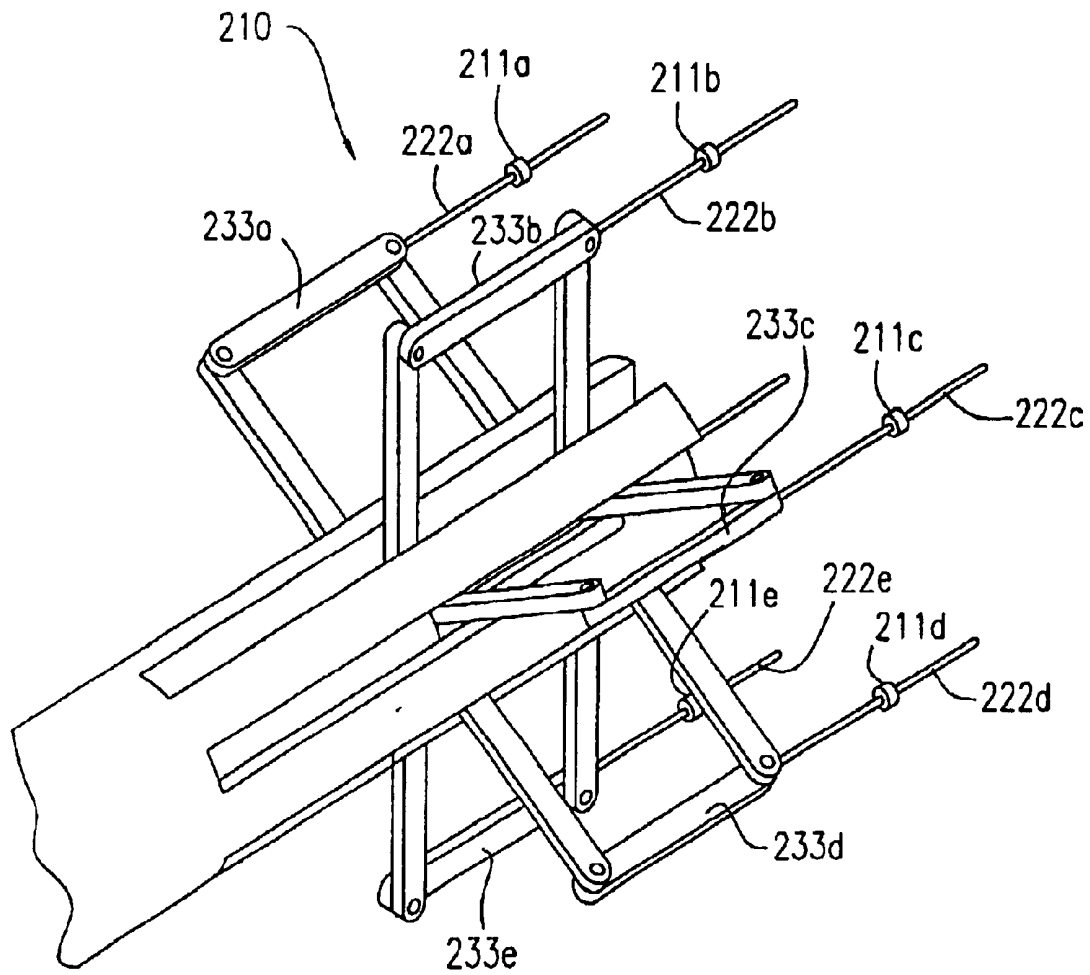


FIG. 10c

*FIG. 11*

## DEVICE AND METHOD TO EXPAND TREATMENT ARRAY

### CROSS REFERENCE TO RELATED APPLICATION

This application is a continuation-in-part of commonly owned U.S. application Ser. No. 10/186,389, entitled "DEVICE AND METHOD TO EXPAND TREATMENT ARRAY" filed Jun. 28, 2002, now abandoned.

### FIELD OF THE INVENTION

The present invention relates to an RF (radio frequency) device for use in the performance of RF thermal treatment of tissue, and more particularly, to an RF device adapted for use during a laparoscopic or percutaneous procedure.

### BACKGROUND OF THE INVENTION

During an RF procedure, a probe is placed into a target tissue for treating malignant and nonmalignant conditions. The probe is typically provided with an array of electrodes so that RF energy can be supplied to the target tissue.

Various RF devices have been employed to treat a large volume of tissue with a single applicator in a single procedure. One such device employs an array of wire electrodes that deploys and assumes an inverted umbrella shape after reaching the target tissue. When deployed, the inverted umbrella shape of the electrode array may be altered by tissue mechanical resistance or calcifications such that the electrode array exhibits a non-uniform pattern of thermal treatment. Such a non-uniform pattern is undesirable because tissue effects will be affected by the changing distance between adjacent electrodes that diverge or converge.

An alternative approach involves the use of an array of electrodes that have a large diameter. Such an approach is also undesirable because the large electrode array cannot be inserted through the body unless an open surgery is performed. Further, the large electrode array cannot be accommodated through a laparoscopic trocar that has a small diameter of 5 to 10 mm.

Accordingly, there is a need for an improved RF device having electrodes that deploy in a uniform and parallel manner along the length of the electrodes and that can be accommodated in a laparoscopic trocar having a small diameter.

### SUMMARY OF THE INVENTION

In accordance with the present invention, there is provided a medical device used for thermal treatment of tissue. The medical device includes an elongated tube that has a longitudinal axis and an expandable member attached to the tube. The expandable member is expandable from a collapsed configuration to an expanded configuration. A plurality of energy-emitting electrodes is attached to the expandable member. Each of the electrodes is arranged generally coaxially relative to the tube when the expandable member is in its collapsed and expanded configurations.

A method is also disclosed for performing thermal treatment of tissue using the medical device. Initially, the tube is placed near the tissue area with the expandable member in its collapsed configuration. In this step, the electrodes are in close proximity to each other and all of the electrodes are arranged generally co-axially relative to the tube. Then, the expandable member is expanded so that it assumes its expanded configuration. In this step, the electrodes are

spaced apart from each other and all of the electrodes are arranged generally coaxially relative to the tube.

Other features and aspects of the present invention will become more fully apparent from the following detailed description of the exemplary embodiment, the appended claims and the accompanying drawings.

### BRIEF DESCRIPTION OF THE DRAWINGS

For a more complete understanding of the present invention, reference is made to the following detailed description of the exemplary embodiment considered in conjunction with the accompanying drawings, in which:

FIG. 1 is a front, perspective view of an RF device constructed in accordance with the present invention, which shows a multi-lumen tube in a retracted position;

FIG. 2 is a view similar to the view shown in FIG. 1, except that the multi-lumen tube is between its retracted and extended positions, and which shows a balloon member in its collapsed configuration;

FIG. 3 is a view similar to the view shown in FIG. 1, except that the multi-lumen tube is in its extended position and the balloon member is in its expanded configuration;

FIG. 4 is a cross-sectional view, taken along section lines IV—IV and looking in the direction of the arrows, of the RF device of FIG. 3;

FIG. 5 is a cross-sectional view, taken along section lines V—V and looking in the direction of the arrows, of the RF device of FIG. 3;

FIG. 6 is a front, perspective view of an RF device constructed in accordance with a second embodiment of the present invention, which shows a sleeve in an extended position;

FIG. 7 is a cross-sectional view, taken along section lines VII—VII and looking in the direction of the arrows, of the RF device of FIG. 6;

FIG. 8 is a view similar to the view shown in FIG. 6, except that the sleeve is in a retracted position and a plurality of arms is in a collapsed configuration;

FIG. 8a is an exploded view of the distal portion of the RF device of FIG. 8;

FIG. 9 is a view similar to the view shown in FIG. 8, except that the arms are in an expanded configuration;

FIG. 9a is an exploded view of the distal portion of the RF device of FIG. 9;

FIG. 9b is a top, perspective view of the RF device of FIG. 9a;

FIGS. 10a–c are sequential, partial cross-sectional views, showing the progressive movement of two of the arms as they move from the collapsed configuration to the expanded configuration; and

FIG. 11 is a front, perspective view of a distal portion of an RF device constructed in accordance with a third embodiment of the present invention.

### DETAILED DESCRIPTION OF THE EXEMPLARY EMBODIMENT

FIG. 1 shows an RF device 10 used for thermal treatment of tissue. The RF device 10 can be applied through 5–10 mm or larger laparoscopic trocar. Alternatively, the RF device 10 can be applied percutaneously to the affected tissue area.

With reference to FIGS. 1 to 3, the RF device 10 includes an outer sheath 12 which is linearly shaped and an elongated multi-lumen tube 14 sized and shaped to be coaxially

received within the outer sheath 12. The multi-lumen tube 14 has a longitudinal axis and is also linearly shaped. The multi-lumen tube 14 is also sized and shaped to move relative to the outer sheath 12 by conventional methods such as by laparoscopic surgical tools (e.g., graspers, forceps, retractors) sliding through a plastic or metal trocar. As shown in FIG. 2, the multi-lumen tube 14 has a distal end 16 that can extend from the outer sheath 12. More particularly, the multi-lumen tube 14 is movable between a retracted position (see FIG. 1), in which the multi-lumen tube 14 retracts into the outer sheath 12, and an extended position (see FIG. 3), in which the multi-lumen tube 14 extends from the outer sheath 12. Alternatively, the outer sheath 12 can be sized and shaped to move relative to the multi-lumen tube 14.

Referring to FIG. 3, the RF device 10 further includes a balloon member 18 attached to the multi-lumen tube 14. The tube 14 extends completely through the balloon member 18. More particularly, the balloon member 18 is positioned along an intermediate length of the tube 14. For reasons to be discussed hereinafter, the balloon member 18 is sized and shaped to inflate into a fully expanded configuration as shown in FIG. 3 and to deflate into a fully collapsed configuration as shown in FIG. 2. Further, when the multi-lumen tube 14 is in its retracted position, the balloon member 18 is in its collapsed configuration and compressed within the outer sheath 12 so as to facilitate insertion into a trocar for delivery to the affected tissue area. When the multi-lumen tube 14 is in its extended position, the balloon member 18 is released from the outer sheath 12 such that it can move between its expanded configuration and collapsed configuration.

The RF device 10 is powered by an RF energy source, such as a conventional electrosurgical generator 20 (shown in phantom in FIG. 1). The operating frequency ranges from 100 to 3,000 kHz, preferably 400 to 700 kHz. As illustrated in FIG. 3, the RF device 10 includes a plurality of generally linearly shaped electrode needles 22 for delivering RF energy. The electrode diameters are between 0.25 and 1.0 mm, preferably 0.5 mm. The tips may be beveled, as a hypodermic needle, or other sharp tip. The polarity of the electrode needles 22 can be regulated such that each of the electrode needles 22 can be activated in various arrangements to be used as an active or return electrode. For example, two adjacent electrode needles 22a, 22b may be active and the remaining two electrode needles 22c, 22d may be return. Alternatively, adjacent electrode needles 22a, 22b may be active and return, making an alternating pattern. Alternatively, all electrode needles 22a, 22b, 22c, and 22d may be active and the return is a ground pad on the patient (not shown). Each of the electrode needles 22 is attached to the outer surface of the balloon member 18 by conventional attaching means, such as a solvent-based glue. It will be understood that although four electrode needles 22 are shown in FIG. 3, the number of electrode needles 22 can vary. The electrosurgical generator 20 is electrically connected to the electrode needles 22 and provides monopolar or bipolar energy to them in order to thermally treat tissue. With reference to FIG. 4, a plurality of wire leads 24 extends through the multi-lumen tube 14 and is electrically connected to the electrosurgical generator 20 and to the electrode needles 22. As shown in FIG. 4, each of the electrode needles 22 is attached to one of the wire leads 24. Although the electrode needles 22 may be connected in various bipolar or monopolar configurations, the order of connections may be changed at time intervals to facilitate the distribution of RF energy and configure the heating field dynamically. The

electrode needles 22 can be used or can be equipped with components to sense tissue properties, such as either temperature, impedance, or other properties. This sensing may determine what the new order of connections will be to alter the heating pattern based on the sensor feedback. The sensors may be temperature sensing, as in thermistors, thermocouples, or fiber optic sensors and may be located on or inside the electrode needles 22.

When the balloon member 18 is in its collapsed configuration, the electrode needles 22 are in a compressed position, in which the electrode needles 22 are proximate to the multi-lumen tube 14 as shown in FIG. 2 so as to facilitate insertion within the outer sheath 22. Further, as the balloon member 18 inflates to its expanded configuration, the electrode needles 22 move to a deployed configuration, in which the electrode needles 22 move radially outward relative to the multi-lumen tube 14 such that each of the electrode needles 22 extends in a substantially parallel relationship relative to the other electrode needles 22 as shown in FIG. 3. The balloon member 18 expands to a diameter of between 10 and 50 mm, preferably 20 mm if four electrode needles 22a, 22b, 22c, 22d are provided and 30 mm if six electrode needles are provided. After extending, each of the electrode needles 22 is substantially spaced from the other electrode needles 22. Because RF energy is applied to the affected tissue area interstitially, having substantial spacing between the electrode needles 22 facilitates the spread of RF energy deposition, thereby treating a large volume of tissue. The electrode needles 22 are arranged generally coaxially relative to the tube 14 when the balloon member 18 is in its collapsed configuration and its expanded configuration.

With reference to FIG. 5, the multi-lumen tube 14 includes a passageway 26 for receiving air or liquid, either of which can be used to inflate the balloon member 18 (see FIG. 3) to its fully expanded configuration (see FIG. 3). This could be simply done with a syringe. A passageway 28 is also provided for receiving a vacuum to evacuate the air or liquid from the balloon member 18, thereby causing it to deflate and assume its fully collapsed configuration as shown in FIG. 2. This could also be done with a syringe. Alternatively, the multi-lumen tube 14 can employ a single passageway (not shown) that can receive air, fluid, and vacuum, rather than having the two separate passageways 26, 28. Further, a passageway 30 is sized and shaped to allow the wire leads 24 (see FIG. 4) to pass therethrough. The air or liquid may be circulating inside the balloon member 18 to cool the electrode needles 22 and the tissue surface that contacts the electrode needles 22. The electrode needles 22 can incorporate heat pipe technology, typically a sealed hollow cylinder, with conductive fluid, whose purpose is to transport heat away from the hottest segments.

Referring to FIG. 3, the multi-lumen tube 14 includes a vent 32 for receiving air/liquid from the passageway 26 (see FIG. 5), a vent 34 for receiving vacuum from the passageway 28 (see FIG. 5), and a plurality of wire vents 36, each of which is sized and shaped to allow one of the wire leads 24 to pass therethrough and connect to one of the electrode needles 22. The vents 32, 34 and the wire vents 36 are located underneath the balloon member 18.

When inflated as shown in FIG. 3, the balloon member 18 has a substantially cylindrically-shaped configuration and includes an interior chamber 38 filled with air or liquid. The balloon member 18 can be made from a material which is selected from a group including silicone, latex, urethane, and other flexible polymers, as commonly used in medical devices.

In operation, a conventional laparoscopic trocar (not shown) is initially placed through the skin. The RF device 10

is then applied through the laparoscopic trocar such that the RF device **10** enters the open body cavity. Note that in the foregoing step, the multi-lumen tube **14** is in its retracted position (see FIG. 1).

As shown in FIG. 2, the multi-lumen tube **14** is then extended from the outer sheath **12**. Turning now to FIG. 3, the balloon member **18** is fully inflated with air or liquid so as to assume its expanded configuration. As the balloon member **18** inflates, the electrode needles **22** move toward their deployed configuration. The array of electrode needles **22** is now placed into the target tissue. Voltage is then supplied to the electrode needles **22** such that RF energy is emitted therefrom to the tissues surrounding each of the electrode needles **22**. After a predetermined time period between 5 and 50 minutes, preferably 15 minutes, the power to the electrode needles **22** is terminated. Next, the RF device **10** is removed from the target tissue and moved to a second treatment zone or from the body cavity by initially deflating the balloon member **18** into its collapsed configuration such that the electrode needles **22** assume their compressed configuration, and then retracting the multi-lumen tube **14** into the outer sheath **12**. Lastly, the device is removed from the body through the trocar.

As is evident from the description above, the present invention provides numerous advantages. For instance, because each of the electrode needles **22** extends in a substantially parallel relationship relative to the other electrode needles **22** as shown in FIG. 3, the heating and electric fields will be homogenous along the length of the electrode needles **22**. Only the desired penetration depth is used since the electrode needles **22** can be inserted into tissue between 5 and 50 mm, preferably 30 mm. Further, the RF device **10** provides a more predictable heating than that of competitive devices. The RF device **10** can thermally treat malignant or benign pathologies without requiring surgery. The electrode needles **22** can be arranged such that the radius of the deployed array has a length such that the heating takes place between the electrode needles **22**, when configured in a bipolar fashion, with alternating polarity between adjacent needles. This radius could be 1 cm if the electrode needles **22** are spaced 1 to 3 mm apart, and any larger radius (1.5 to 3 cm) with the same spaced apart configuration would have the same effect. In summary, with this configuration, only the outside of the treatment area is heated such that a cylindrical shell of volume of necrosis is created.

A second exemplary embodiment of the present invention is illustrated in FIGS. 6 to 10c. Elements illustrated in FIGS. 6 to 10c which correspond to the elements described above with reference to FIG. 1 have been designated by corresponding reference numerals increased by one hundred. In addition, elements illustrated in FIGS. 6 to 10c which do not correspond to the elements described above with reference to FIG. 1 have been designated by odd numbered reference numerals starting with reference number **111**. The embodiment of FIGS. 6 to 10c operates in the same manner as the embodiment of FIG. 1, unless it is otherwise stated.

FIG. 6 shows an RF device **110** having a handle portion **111** and an elongated sleeve **112** attached thereto. The elongated sleeve **112** includes a proximal end **113** received within the handle portion **111** and a distal end **115** sized and shaped to be received within the target tissue for reasons described hereinafter. A finger gripping flange **117** is located at the proximal end **113** of the sleeve **112**, for moving the sleeve **112** between a retracted position (see FIG. 8) and an extended position (see FIG. 6), as will be described below.

Referring to FIG. 7, the RF device **110** also includes a probe sheath **119** coaxially received within the sleeve **112**.

The probe sheath **119** includes a proximal end **121** received within the handle portion **111**, a distal portion **123**, and a distal end **125** sized and shaped to be received within the target tissue for reasons described hereinafter. A flange **127** is located at the proximal end **121** of the probe sheath **119** and utilized to move the probe sheath **119** between a retracted position (see FIG. 9) and an extended position (see FIG. 6), as will be described below.

With reference to FIG. 9B, the distal portion **123** of the probe sheath **119** has six longitudinal grooves **129a-f** on its outer surface so as to form six longitudinally extending bars **131a-f**. The longitudinal groove **129a** is formed between an adjacent pair of the bars **131a-b**, while the longitudinal groove **129b** is formed between an adjacent pair of the bars **131b-c**. Also, the longitudinal groove **129c** is formed between an adjacent pair of the bars **131c-d**, while the longitudinal groove **129d** is formed between an adjacent pair of the bars **131d-e**. The longitudinal groove **129e** is formed between an adjacent pair of the bars **131e-f**, while the longitudinal groove **129f** is formed between an adjacent pair of the bars **131f-a**.

Referring still to FIG. 9B, an expandable member **118** is provided and includes six arms **133a-f**, each of which is expandable between a collapsed configuration (see FIG. 8a) and an expanded configuration (see FIG. 9a) as will be described in further detail hereinafter. A plurality of generally linearly shaped electrode needles **122a-f** is provided for delivering RF energy. More particularly, the needles **122a-f** are attached to the arms **133a-f**, respectively, by conventional attaching means. The polarity of the electrode needles **122a-f** can be regulated such that each of the electrode needles **122a-f** can be activated in various arrangements to be used as an active or return electrode. For example, the three adjacent electrode needles **122a**, **122b**, **122c** may be active and the remaining three electrode needles **122d**, **122e**, **122f** may be return. Alternatively, adjacent electrode needles (e.g., **122a**, **122b**) may be active and return, making an alternating pattern. Alternatively, all of the electrode needles **122a-f** may be active and the return is a ground pad on the patient (not shown).

With reference to FIG. 9b, the arms **133a-f** includes front sections **135a-f**, back sections **137a-f**, needle sections **139a-f**, and side sections (see FIGS. 10a-c) (only side sections **141a**, **141d** are visible in FIGS. 10a-c), respectively. The electrode needles **122a-f** are attached to the needle sections **139a-f**, respectively. For simplicity, only two of the arms **133a**, **133d** are described in detail below with reference to FIGS. 10a-c. It will be understood that the structure and operation of all of the arms **133a-f** are similar. Adjacent sections are hingedly attached to each other. More particularly, with reference to FIG. 10c, the front section **135a** is hingedly attached to the needle section **139a** at a first joint **143a** along one edge of the front section **135a**, and to the side section **141a** at a second joint **145a** along an opposite edge of the front section **135a**. The needle section **139a** is hingedly attached to the front section **135a** at the first joint **143a** along one edge of the needle section **139a**, and to the back section **137a** at a third joint **147a** along an opposite edge of the needle section **139a**. Likewise, the back section **137a** is hingedly attached to the needle section **139a** at the third joint **147a** along one edge of the back section **137a**, and to the side section **141a** at a fourth joint **149a** along an opposite edge of the back section **137a**. The side section **141a** is hingedly attached to the back section **137a** at the fourth joint **149a** along one edge of the side section **141a**, and to the front section **135a** at the second joint **145a** along an opposite edge of the side section **141a**. Similarly, the

front section **135d** is hingedly attached to the needle section **139d** along one edge of the front section **135a**, and to the side section **141d** along an opposite edge of the front section **135d**. The needle section **139d** is hingedly attached to the front section **135d** along one edge of the needle section **139d**, and to the back section **137d** along an opposite edge of the needle section **139d**. Likewise, the back section **137d** is hingedly attached to the needle section **139d** along one edge of the back section **137d**, and to the side section **141d** along an opposite edge of the back section **137d**. The side section **141d** is hingedly attached to the back section **137d** along one edge of the side section **141d**, and to the front section **135d** along an opposite edge of the side section **141d**.

The second joint (e.g., **145a**) of each of the arms **133a-f** has an opening (not shown) through which conventional attaching means pass through so as to connect all of the side sections of the arms **133a-f** along one edge of each side section. Likewise, the fourth joint (e.g., **149a**) of each of the arms **133a-f** has an opening (not shown) through which conventional attaching means pass through so as to connect all of the side sections of the arms **133a-f** along an opposite edge of each side section.

Referring to FIGS. **10a-c**, the distal end **125** of the probe sheath **119** includes a front portion **151**, a back portion **153**, and six inwardly tapered sides (only opposing sides **155a**, **155d** are visible in FIGS. **10a-c**) located within the six longitudinal grooves **129a-f** (see FIG. **9B**), respectively. The back portion **153** is attached to the six inwardly tapered sides along a circumferential edge (only two edge points **157a**, **157d** of which are visible in FIGS. **10a-c**).

Referring back to FIG. **7**, the RF device **110** further includes an elongated tube **159** coaxially received within the probe sheath **119**. The elongated tube **159** has a proximal end **161** received within the handle portion **111** and a distal portion **163** (see FIGS. **10a-c**) sized and shaped to be received within the target tissue. With reference to FIGS. **10a-c**, the distal portion **163** of the elongated tube **159** is located between the six arms **133a-f** (only the arms **133a**, **133d** are visible). The RF device **110** also includes an electrode needle **122g** attached to an end **165** of the distal portion **163**. The elongated tube **159** also includes a cylindrical member **167** connected to an opposite end **169** of the distal portion **163** and connected to the arms **133a-f** of the expandable member **118**.

In operation, a conventional laparoscopic trocar (not shown) is initially placed through the skin in some cases. Alternatively, a percutaneous approach may be used. The RF device **110** is then applied through the laparoscopic trocar such that the RF device **110** enters the open body cavity. Note that in the foregoing step, the sleeve **112** is in its extended position (see FIG. **6**), in which the sleeve **112** covers the probe sheath **119** and the arms **133a-f**.

As shown in FIGS. **8** and **8a**, the finger gripping flange **117** (see FIG. **8**) is retracted such that the sleeve **112** moves in a proximal direction toward the handle portion **111** until it is in contact with the flange **127** of the probe sheath **119** so as to expose the distal portion **123** of the probe sheath **119** and the arms **133a-f**. Turning now to FIGS. **9** and **9a**, the finger gripping flange **117** is further retracted so as to cause the flange **127** to retract toward the handle portion **111**. As the flange **127** retracts, the probe sheath **119** moves from its extended position to its retracted position, such that each of the arms **133a-f** deploys to its expanded configuration as will be described in further detail hereinafter.

The following description will describe the deployment of the arms (only the arms **133a**, **133d** are visible in FIGS.

**10a-c**), i.e., to make the conversion from the collapsed configuration illustrated in FIG. **10a** to the expanded configuration illustrated in FIG. **10c**. Initially as illustrated in FIG. **10a**, the front section **135a** is positioned so as to rest on the side **155a** of the distal end **125** of the probe sheath **119**. In this position, the front section **135a** is adjacent to and substantially parallel to the needle section **139a**, and the side section **141a** is adjacent to and substantially parallel to the back section **137a**. As shown in FIG. **10b**, as the flange **127** (see FIG. **9**) retracts, the distal end **125** of the probe sheath **119** retracts such that contact between the front section **135a** and the edge point **157a** of the distal end **125** allows the front section **135a** to pivot about pivot points **143a**, **145a**. As the front section **135a** pivots, the needle section **139a** and the back section **137a** also pivot. When the pivot point **145a** contacts the edge point **157a**, the arm **133a** is in its expanded configuration such that adjacent sections (e.g., **135a**, **139a**) are substantially perpendicular to each other.

RF energy is then supplied to the electrode needles **122a-g** such that RF energy is emitted therefrom to the tissues surrounding each of the electrode needles **122a-g**. After a predetermined time period between 5 and 50 minutes, preferably 15 minutes, the power to the electrode needles **122a-g** is terminated. Next, the RF device **110** is removed from the target tissue and to the second target location or from the body cavity by extending the finger gripping flange **117** toward the arms **133a-f** such that contact between the sleeve **112** and the back section (e.g., **137a**) of each of the arms **133a-f** moves the arms **133a-f** into their collapsed configuration. Lastly, the RF device **110** is removed from the body through the trocar.

A third exemplary embodiment of the present invention is illustrated in FIG. **11**. Elements illustrated in FIG. **11** which correspond to the elements described above with reference to FIGS. **6** to **10c** have been designated by corresponding reference numerals increased by one hundred. In addition, elements illustrated in FIG. **11** which do not correspond to the elements described above with reference to FIGS. **6** to **10c** have been designated by odd numbered reference numerals starting with reference number **211**. The embodiment of FIG. **11** operates in the same manner as the embodiment of FIGS. **6** to **10c**, unless it is otherwise stated.

FIG. **11** shows an RF device **210** having six movable parts **211a-e** (only five of which are shown) attached to the six needles **222a-e** (only five of which are shown), respectively, of the arms **233a-e**. The movable parts **211a-e** are electrically connected to the six needles **222a-e**, respectively, and may be cylindrical, spherical, hemispherical, etc. In operation, the needles **222a-e** are inserted into tissue to the desired depth, which is in a range of approximately 1 to 4 cm. Then, the needles **222a-e** are inserted further, about 2 to 4 mm, into the tissue and then withdrawn 2 to 4 mm. In this position, the movable parts **211a-e** are 2 to 4 mm away from the tissue surface. Once the needles **222a-e** are activated, the tissue is heated and the power is shut off. Then, the needles **222a-e** are advanced 2 to 4 mm such that the movable parts **211a-e** are in contact with the tissue surface. Power is switched on again and the movable parts **211a-e** heat the tissue at the interface. After approximately 5 to 10 seconds of activation, the tissue interface is sufficiently coagulated. The purpose of the movable parts **211a-e** is to stop any bleeding at the location where the needles **222a-e** enter the tissue.

It should be noted that the RF device **10**, **110**, **210** can have numerous modifications and variations. For instance, the RF device **10**, **110**, **210** can be either disposable or non-disposable. The RF device **10**, **110**, **210** can have

laparoscopic applications and can be used to treat various sites such as the liver, kidney, spine, lung, and fibroids on or in the wall of the uterus. Also, the RF device **10**, **110**, **210** can have percutaneous applications and can be used to treat various sites such as the breast and the prostate. The electrode needles **22a-d**, **122a-g**, **222a-e** can be insulated in sections to regulate the conductive portion and the heating field. In such aspects, RF current will flow only through the needle portion that is not covered by insulation. The RF device **10**, **110**, **210** can employ alternative energy sources such as laser fibers, ultrasound PZT based cylinders, chemical, microwave antennas, and/or a cryogenic device. The foregoing energy sources can include either catheters or needles. It will be understood that although seven electrode needles **122** are shown in FIG. **9b**, the number of electrode needles **122** can vary. Likewise, although six longitudinal grooves **129a-f** and six longitudinally extending bars **131a-f** are shown, the number of grooves **129a-f** and bars **131a-f** can vary. All such variations and modifications are intended to be included within the scope of the invention as defined in the appended claims.

What is claimed is:

**1.** A medical device used for thermal treatment of tissue, comprising an elongated probe sheath having a longitudinal axis; an expandable member attached to said elongated probe sheath, said expandable member being expandable from a collapsed configuration to an expanded configuration; and a plurality of energy-emitting electrodes attached to said expandable member such that each of said electrodes is arranged generally coaxially relative to said probe sheath when said expandable member is in its said collapsed and expanded configurations, said expandable member including a plurality of arms, each of said arms being expandable between a collapsed configuration and an expanded configuration, said probe sheath including a plurality of inwardly tapered sides in cooperation with said arms, and said probe sheath being movable between a retracted position and an extended position.

**2.** The medical device of claim **1**, further comprising a sleeve sized and shaped so as to receive said probe sheath and said expandable member when said expandable member is in its said collapsed configuration.

**3.** The medical device of claim **2**, wherein each of said electrodes moves radially outward from said probe sheath as said expandable member moves from its said collapsed configuration to its said expanded configuration.

**4.** The medical device of claim **3**, wherein said electrodes are in close proximity to each other when said expandable member is in its said collapsed configuration and wherein said electrodes are spaced apart from each other when said expandable member is in its said expanded configuration.

**5.** The medical device of claim **4**, wherein said probe sheath extends completely through said expandable member, whereby said expandable member is positioned along an intermediate length of said probe sheath.

**6.** The medical device of claim **5**, wherein each of said electrodes has a generally linear shape.

**7.** The medical device of claim **6**, wherein said probe sheath is movable between a retracted position, in which said probe sheath retracts into said sleeve, and an extended position, in which said probe sheath extends axially outward from said sheath.

**8.** The medical device of claim **7**, wherein said tube includes a plurality of channels, at least one of said channels being sized and shaped so as to allow a fluid to pass therethrough.

**9.** The medical device of claim **8**, wherein said expandable member is expandable to its said expanded configuration when a fluid is passed through said at least one of said channels.

**10.** The medical device of claim **9**, wherein said expandable member is collapsible to its said collapsed configuration when a vacuum is supplied to said expandable member through at least another of said channels.

**11.** The medical device of claim **10**, further comprising a plurality of wire leads connected to said electrodes.

**12.** The medical device of claim **11**, wherein at least another of said channels is sized and shaped to allow said wire leads to pass therethrough.

**13.** The medical device of claim **12**, wherein said expandable member is a balloon member.

**14.** The medical device of claim **13**, wherein said electrodes emit RF energy.

**15.** The medical device of claim **14**, wherein said balloon member is substantially cylindrically-shaped when it is in its said expanded configuration.

**16.** The medical device of claim **15**, wherein said electrodes surround said tube when said balloon member is in its said expanded configuration.

**17.** The medical device of claim **16**, wherein said expandable member is attached to said tube by a solvent-based glue.

**18.** A method for performing thermal treatment of tissue using a medical device which includes a probe sheath having a plurality of inwardly tapered sides, an expandable member including a plurality of arms, the expandable member attached to the tube and expandable from a collapsed configuration to an expanded configuration, and a plurality of electrodes attached to the expandable member, said method comprising the steps of:

(a) inserting the medical device within a tissue area with the expandable member in its collapsed configuration, in which the electrodes are in close proximity to each other and in which all of the electrodes are arranged generally coaxially relative to the probe sheath; and

(b) moving the arms relative to the inwardly tapered sides of the probe sheath so as to expand the expandable member so that it assumes its expanded configuration, in which the electrodes are spaced apart from each other and in which all of the electrodes are arranged generally coaxially relative to the probe sheath.

**19.** The method of claim **18**, wherein the method is used in a laparoscopic application.

**20.** The method of claim **18**, wherein the method is used in a percutaneous application.

**21.** The medical device of claim **1**, wherein each of said arms moves toward its said expanded configuration as said probe sheath moves from its said extended position to its said retracted position.

**22.** The medical device of claim **21**, further comprising an elongated sleeve coaxially received over said probe sheath, said sleeve being movable between a retracted position and an extended position.

**23.** The medical device of claim **22**, wherein each of said arms moves toward its said collapsed configuration as said sleeve moves from its said retracted position to its said extended position.

**24.** The medical device of claim **23**, wherein the polarity of said electrodes can be selectively varied.

**25.** A medical device used for thermal treatment of tissue, comprising an elongated probe sheath having a longitudinal axis; an expandable member attached to said elongated probe sheath, said expandable member being expandable from a collapsed configuration to an expanded configuration; and a plurality of energy-emitting electrodes attached to said expandable member such that each of said electrodes is arranged generally coaxially relative to said probe sheath when said expandable member is in its said collapsed and

**11**

expanded configurations, said expandable member including a plurality of arms, each of said arms being expandable between a collapsed configuration and an expanded configuration, said arms including a plurality of members

**12**

connected to said electrodes, each of said members movable relative to said electrodes.

\* \* \* \* \*

专利名称(译)	扩展治疗阵列的装置和方法		
公开(公告)号	<a href="#">US6881213</a>	公开(公告)日	2005-04-19
申请号	US10/278235	申请日	2002-10-23
[标]申请(专利权)人(译)	ETHICON. INC		
申请(专利权)人(译)	ETHICON INC.		
当前申请(专利权)人(译)	ETHICON INC.		
[标]发明人	RYAN THOMAS P YUAN DAVID Y SIMPSON RODDI J CIARROCCA SCOTT A SINTON ALEXANDER J		
发明人	RYAN, THOMAS P. YUAN, DAVID Y. SIMPSON, RODDI J. CIARROCCA, SCOTT A. SINTON, ALEXANDER J.		
IPC分类号	A61B18/14 A61B18/18		
CPC分类号	A61B18/1477 A61B18/1482 A61B2018/143 A61B2018/0022 A61B2018/00214		
其他公开文献	US20040002748A1		
外部链接	<a href="#">Espacenet</a> <a href="#">USPTO</a>		

# 摘要(译)

提供了一种医疗装置，其包括细长管，该细长管具有纵向轴线和附接到管的可扩张构件。可扩张构件可从收缩构型扩张到扩张构型。多个电极附接到可扩张构件。电极用于发射能量。当可扩张构件处于其收缩和扩张构型时，每个电极通常相对于管同轴地布置。

