



US008696694B2

(12) **United States Patent**
Belson

(10) **Patent No.:** **US 8,696,694 B2**
(45) **Date of Patent:** ***Apr. 15, 2014**

(54) **APPARATUS AND METHOD FOR
ENDOSCOPIC COLECTOMY**

(71) Applicant: **Intuitive Surgical Operations, Inc.**,
Sunnyvale, CA (US)

(72) Inventor: **Amir Belson**, Los Altos, CA (US)

(73) Assignee: **Intuitive Surgical Operations, Inc.**,
Sunnyvale, CA (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

This patent is subject to a terminal dis-
claimer.

(21) Appl. No.: **13/729,602**

(22) Filed: **Dec. 28, 2012**

(65) **Prior Publication Data**

US 2013/0116712 A1 May 9, 2013

Related U.S. Application Data

(62) Division of application No. 12/027,739, filed on Feb.
7, 2008, now Pat. No. 8,361,090, which is a division of
application No. 10/327,370, filed on Dec. 20, 2002,
now Pat. No. 7,338,505.

(60) Provisional application No. 60/347,674, filed on Jan.
9, 2002.

(51) **Int. Cl.**
A61B 17/11 (2006.01)

(52) **U.S. Cl.**
USPC **606/153**

(58) **Field of Classification Search**
CPC A61B 1/31; A61B 17/1114
USPC 606/150, 153, 154
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

616,672 A 12/1898 Kelling
2,510,198 A 6/1950 Tesmer

(Continued)

FOREIGN PATENT DOCUMENTS

DE 2823025 A1 12/1979
DE 3707787 A1 9/1988

(Continued)

OTHER PUBLICATIONS

Belson et al., U.S. Appl. No. 11/796,220 entitled "Steerable seg-
mented endoscope and method of insertion" filed Apr. 27, 2007.

(Continued)


Primary Examiner — Julian W Woo

Assistant Examiner — Shaun L David

(57) **ABSTRACT**

Apparatus and methods for endoscopic colectomy are described herein. A colectomy device having a first and a second tissue approximation device is mounted on a colonoscope separated from one another. During deployment of the colectomy device, a diseased portion of the colon is positioned inbetween the tissue approximation devices. The tissue approximation devices are radially expanded such that they contact and grasp the colon wall at two sites adjacent to the diseased portion of the colon. The diseased portion is separated from the omentum and is transected using a laparoscope or is drawn into the colonoscope for later removal. The tissue approximation devices are then urged towards one another over the colonoscope to approximate the two free edges of the colon into contact together where they are fastened to one another using the tissue approximation device as a surgical stapler to create an end-to-end anastomosis.

18 Claims, 19 Drawing Sheets

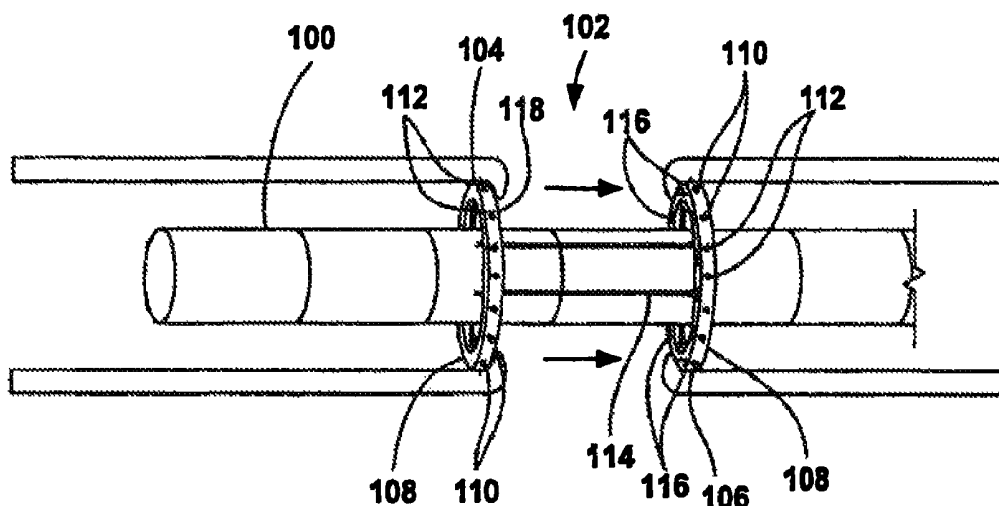

(56)

References Cited

U.S. PATENT DOCUMENTS

2,533,494 A	12/1950	Mitchell, Jr.	4,873,965 A	10/1989	Danieli
2,767,705 A	10/1956	Moore	4,873,990 A	10/1989	Holmes et al.
3,060,972 A	10/1962	Sheldon	4,879,991 A	11/1989	Ogiu
3,071,161 A	1/1963	Ulrich	4,884,557 A	12/1989	Takehana et al.
3,096,962 A	7/1963	Meijs	4,890,602 A	1/1990	Hake
3,162,214 A	12/1964	Bazinet	4,895,431 A	1/1990	Tsujiuchi et al.
3,168,274 A	2/1965	Street	4,899,731 A	2/1990	Takayama et al.
3,190,286 A	6/1965	Stokes	4,904,048 A	2/1990	Sogawa et al.
3,266,059 A	8/1966	Stelle	4,917,114 A	4/1990	Green et al.
3,430,662 A	3/1969	Guarnaschelli	4,919,112 A	4/1990	Siegmund
3,497,083 A	2/1970	Anderson	4,930,494 A	6/1990	Takehana et al.
3,546,961 A	12/1970	Marton	4,949,927 A	8/1990	Madocks et al.
3,610,231 A	10/1971	Takahashi et al.	4,957,486 A	9/1990	Davis
3,625,084 A	12/1971	Siebert	4,969,709 A	11/1990	Sogawa et al.
3,643,653 A	2/1972	Takahashi et al.	4,971,035 A	11/1990	Ito
3,739,770 A	6/1973	Mori	4,977,886 A	12/1990	Takehana et al.
3,773,034 A	11/1973	Burns et al.	4,977,887 A	12/1990	Gouda
3,780,740 A	12/1973	Rhea	4,987,314 A	1/1991	Gotanda et al.
3,858,578 A	1/1975	Milo	5,005,558 A	4/1991	Aomori
3,871,358 A	3/1975	Fukuda et al.	5,005,559 A	4/1991	Blanco et al.
3,897,775 A	8/1975	Furihata	5,014,709 A	5/1991	Bjelkhagen et al.
3,913,565 A	10/1975	Kawahara	5,018,509 A	5/1991	Suzuki et al.
3,946,727 A	3/1976	Okada et al.	5,025,778 A	6/1991	Silverstein et al.
3,990,434 A	11/1976	Free	5,060,632 A	10/1991	Hibino et al.
4,054,128 A	10/1977	Seufert et al.	5,092,901 A	3/1992	Hunter et al.
4,176,662 A	12/1979	Frazer	5,122,156 A *	6/1992	Granger et al. 606/219
4,198,982 A	4/1980	Fortner et al.	5,125,395 A	6/1992	Adair
4,233,981 A *	11/1980	Schomacher 606/153	5,127,393 A	7/1992	McFarlin et al.
4,236,509 A	12/1980	Takahashi et al.	5,159,446 A	10/1992	Hibino et al.
4,240,435 A	12/1980	Yazawa et al.	5,166,787 A	11/1992	Irion
4,273,111 A	6/1981	Tsukaya	5,174,276 A	12/1992	Crockard
4,327,711 A	5/1982	Takagi	5,174,277 A	12/1992	Matsumaru
4,366,810 A	1/1983	Slanetz, Jr.	5,188,111 A	2/1993	Yates et al.
4,393,728 A	7/1983	Larson et al.	5,207,695 A	5/1993	Trout, III
4,432,349 A	2/1984	Oshiro	5,217,001 A	6/1993	Nakao et al.
4,483,326 A	11/1984	Yamaka et al.	5,220,911 A	6/1993	Tamura
4,489,826 A	12/1984	Dubson	5,228,429 A	7/1993	Hatano
4,494,417 A	1/1985	Larson et al.	5,234,448 A	8/1993	Wholey et al.
4,499,895 A	2/1985	Takayama	5,243,967 A	9/1993	Hibino
4,503,842 A	3/1985	Takayama	5,250,058 A	10/1993	Miller et al.
4,543,090 A	9/1985	McCoy	5,251,611 A	10/1993	Zehel et al.
4,551,061 A	11/1985	Olenick	5,253,647 A	10/1993	Takahashi et al.
4,559,928 A	12/1985	Takayama	5,254,127 A *	10/1993	Wholey et al. 606/153
4,566,843 A	1/1986	Iwatsuka et al.	5,254,809 A	10/1993	Martin
4,577,621 A	3/1986	Patel	5,257,617 A	11/1993	Takahashi
4,592,341 A	6/1986	Omagari et al.	5,259,364 A	11/1993	Bob et al.
4,592,354 A	6/1986	Rothfuss	5,271,381 A	12/1993	Ailinger et al.
4,601,283 A	7/1986	Chikama	5,271,382 A	12/1993	Chikama
4,601,713 A	7/1986	Fuqua	5,279,610 A	1/1994	Park et al.
4,621,618 A	11/1986	Omagari	5,282,810 A	2/1994	Allen et al.
4,624,243 A	11/1986	Lowery et al.	5,297,443 A	3/1994	Wentz
4,630,649 A	12/1986	Oku	5,309,927 A	5/1994	Welch
4,643,184 A	2/1987	Mobin-Uddin	5,314,435 A	5/1994	Green et al.
4,646,722 A	3/1987	Silverstein et al.	5,325,845 A	7/1994	Adair
4,648,733 A	3/1987	Merk	5,337,732 A	8/1994	Grundfest et al.
4,651,718 A	3/1987	Collins et al.	5,337,733 A	8/1994	Bauerfeind et al.
4,655,257 A	4/1987	Iwashita	5,343,874 A	9/1994	Picha et al.
4,683,773 A	8/1987	Diamond	5,347,987 A	9/1994	Feldstein et al.
4,686,963 A	8/1987	Cohen et al.	5,348,259 A	9/1994	Blanco et al.
4,712,969 A	12/1987	Kimura	5,364,389 A *	11/1994	Anderson 606/8
4,726,355 A	2/1988	Okada	5,370,108 A	12/1994	Miura et al.
4,753,222 A	6/1988	Morishita	5,383,467 A	1/1995	Auer et al.
4,753,223 A	6/1988	Bremer	5,383,852 A	1/1995	Stevens-Wright
4,754,909 A	7/1988	Barker et al.	5,389,222 A	2/1995	Shahinpoor
4,784,117 A	11/1988	Miyazaki	5,394,864 A	3/1995	Kobayashi et al.
4,787,369 A	11/1988	Allred, III	5,395,030 A	3/1995	Kuramoto et al.
4,788,967 A	12/1988	Ueda	5,400,769 A	3/1995	Tanii et al.
4,793,326 A	12/1988	Shishido	5,402,768 A	4/1995	Adair
4,796,607 A	1/1989	Allred, III	5,411,508 A *	5/1995	Bessler et al. 606/153
4,799,474 A	1/1989	Ueda	5,413,108 A	5/1995	Alfano
4,800,890 A	1/1989	Cramer	5,421,337 A	6/1995	Richards-Kortum et al.
4,807,593 A	2/1989	Ito	5,425,738 A	6/1995	Gustafson et al.
4,815,450 A	3/1989	Patel	5,429,118 A	7/1995	Cole et al.
4,832,473 A	5/1989	Ueda	5,439,000 A	8/1995	Gunderson et al.
4,834,068 A	5/1989	Gottesman	5,451,221 A	9/1995	Cho et al.
			5,456,714 A	10/1995	Owen
			5,460,166 A	10/1995	Yabe et al.
			5,460,168 A	10/1995	Masubuchi et al.
			5,469,840 A	11/1995	Tanii et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

5,482,029 A	1/1996	Sekiguchi et al.	5,993,447 A	11/1999	Blewett et al.
5,487,757 A	1/1996	Truckai et al.	5,996,346 A	12/1999	Maynard
5,489,256 A	2/1996	Adair	6,016,440 A	1/2000	Simon et al.
5,503,635 A	4/1996	Sauer et al.	6,033,359 A	3/2000	Doi
5,507,287 A	4/1996	Palcic et al.	6,036,636 A	3/2000	Motoki et al.
5,507,717 A	4/1996	Kura et al.	6,036,702 A	3/2000	Bachinski et al.
5,531,664 A	7/1996	Adachi et al.	6,042,155 A	3/2000	Lockwood
5,551,945 A	9/1996	Yabe et al.	6,048,307 A	4/2000	Grundl et al.
5,558,619 A	9/1996	Kami et al.	6,063,022 A	5/2000	Ben-Haim
5,558,665 A	9/1996	Kieturakis	6,066,102 A	5/2000	Townsend et al.
5,577,992 A	11/1996	Chiba et al.	6,066,132 A	5/2000	Chen et al.
5,586,968 A	12/1996	Grundl et al.	6,068,638 A	5/2000	Makower
5,590,660 A	1/1997	MacAulay et al.	6,096,289 A	8/2000	Goldenberg
5,601,087 A	2/1997	Gunderson et al.	6,099,464 A	8/2000	Shimizu et al.
5,602,449 A	2/1997	Krause et al.	6,099,465 A	8/2000	Inoue
5,620,408 A	4/1997	Vennes et al.	6,099,485 A	8/2000	Patterson
5,624,380 A	4/1997	Takayama et al.	6,106,510 A	8/2000	Lunn et al.
5,624,381 A	4/1997	Kieturakis	6,117,148 A	9/2000	Ravo et al.
5,626,553 A	5/1997	Frassica et al.	6,119,913 A	9/2000	Adams et al.
5,645,520 A	7/1997	Nakamura et al.	6,129,667 A	10/2000	Dumoulin et al.
5,647,368 A	7/1997	Zeng et al.	6,129,683 A	10/2000	Sutton et al.
5,651,769 A	7/1997	Waxman et al.	6,141,577 A	10/2000	Rolland et al.
5,653,690 A	8/1997	Booth et al.	6,149,581 A	11/2000	Klingenstein
5,658,238 A	8/1997	Suzuki et al.	6,162,171 A	12/2000	Ng et al.
5,662,585 A	9/1997	Willis et al.	6,174,280 B1	1/2001	Oneda et al.
5,662,587 A	9/1997	Grundfest et al.	6,174,291 B1	1/2001	McMahon et al.
5,665,050 A	9/1997	Benecke	6,179,776 B1	1/2001	Adams et al.
5,667,476 A	9/1997	Frassica et al.	6,185,448 B1	2/2001	Borovsky
5,669,918 A	9/1997	Balazs et al.	6,201,989 B1	3/2001	Whitehead et al.
5,679,216 A	10/1997	Takayama et al.	6,203,493 B1	3/2001	Ben-Haim
5,728,044 A	3/1998	Shan	6,203,494 B1	3/2001	Moriyama
5,733,245 A	3/1998	Kawano	6,210,337 B1	4/2001	Dunham et al.
5,749,828 A	5/1998	Solomon et al.	6,221,006 B1	4/2001	Dubrul et al.
5,752,912 A	5/1998	Takahashi et al.	6,241,657 B1	6/2001	Chen et al.
5,759,151 A	6/1998	Sturges	6,249,076 B1	6/2001	Madden et al.
5,762,613 A	6/1998	Sutton et al.	6,264,086 B1	7/2001	McGuckin, Jr.
5,765,561 A	6/1998	Chen et al.	6,270,453 B1	8/2001	Sakai
5,769,792 A	6/1998	Palcic et al.	6,306,081 B1	10/2001	Ishikawa et al.
5,772,597 A	6/1998	Goldberger et al.	6,309,346 B1	10/2001	Farhadi
5,773,835 A	6/1998	Sinofsky	6,315,714 B1	11/2001	Akiba
5,779,624 A	7/1998	Chang	6,319,197 B1	11/2001	Tsuji et al.
5,807,241 A	9/1998	Heimberger	6,327,492 B1	12/2001	Lemelson
5,810,715 A	9/1998	Moriyama	6,332,089 B1	12/2001	Acker et al.
5,810,716 A	9/1998	Mukherjee et al.	6,348,058 B1	2/2002	Melkent et al.
5,810,717 A	9/1998	Maeda et al.	6,366,799 B1	4/2002	Acker et al.
5,810,776 A	9/1998	Bacich et al.	6,402,687 B1	6/2002	Ouchi
5,813,976 A	9/1998	Filipi et al.	6,408,889 B1	6/2002	Komachi
5,827,190 A	10/1998	Palcic et al.	6,428,203 B1	8/2002	Danley
5,827,265 A	10/1998	Glinsky et al.	6,443,888 B1	9/2002	Ogura et al.
5,839,639 A	11/1998	Sauer et al.	6,453,190 B1	9/2002	Acker et al.
5,842,973 A	12/1998	Bullard	6,459,481 B1	10/2002	Schaack
5,860,581 A	1/1999	Robertson et al.	6,468,203 B2	10/2002	Belson
5,860,914 A	1/1999	Chiba et al.	6,482,149 B1	11/2002	Torii
5,868,760 A	2/1999	McGuckin, Jr.	6,485,413 B1	11/2002	Boppert et al.
5,876,329 A	3/1999	Harhen	6,485,496 B1	11/2002	Suyker et al.
5,876,373 A	3/1999	Giba et al.	6,490,467 B1	12/2002	Bucholz et al.
5,885,208 A	3/1999	Moriyama	6,503,259 B2 *	1/2003	Huxel et al. 606/153
5,893,369 A	4/1999	LeMole	6,511,417 B1	1/2003	Taniguchi et al.
5,897,417 A	4/1999	Grey	6,511,418 B2	1/2003	Shahidi et al.
5,897,488 A	4/1999	Ueda	6,517,477 B1	2/2003	Wendlandt
5,902,254 A	5/1999	Magram	6,527,706 B2	3/2003	Ide
5,906,591 A	5/1999	Dario et al.	6,537,211 B1	3/2003	Wang et al.
5,908,381 A	6/1999	Aznoian et al.	6,544,215 B1	4/2003	Bencini et al.
5,916,147 A	6/1999	Boury	6,554,793 B1	4/2003	Pauker et al.
5,921,915 A	7/1999	Aznoian et al.	6,569,173 B1 *	5/2003	Blatter et al. 606/153
5,928,136 A	7/1999	Barry	6,616,600 B2	9/2003	Pauker
5,941,815 A	8/1999	Chang	6,638,213 B2	10/2003	Ogura et al.
5,941,908 A	8/1999	Goldsteen et al.	6,641,528 B2	11/2003	Torii
5,957,833 A	9/1999	Shan	6,656,110 B1	12/2003	Iron et al.
5,968,052 A	10/1999	Sullivan, III	6,699,183 B1	3/2004	Wimmer
5,971,767 A	10/1999	Kaufman et al.	6,736,822 B2	5/2004	McClellan et al.
5,976,074 A	11/1999	Moriyama	6,743,239 B1 *	6/2004	Kuehn et al. 606/139
5,989,182 A	11/1999	Hori et al.	6,761,685 B2	7/2004	Adams et al.
5,989,230 A	11/1999	Frassica	6,800,056 B2	10/2004	Tartaglia et al.
5,993,381 A	11/1999	Ito	6,808,499 B1	10/2004	Churchill et al.
			6,808,520 B1	10/2004	Fourkas et al.
			6,817,973 B2	11/2004	Merril et al.
			6,837,846 B2	1/2005	Jaffe et al.
			6,837,849 B2	1/2005	Ogura et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

6,843,793	B2	1/2005	Brock et al.	
6,850,794	B2	2/2005	Shahidi	
6,858,005	B2	2/2005	Ohline et al.	
6,869,396	B2	3/2005	Belson	
6,875,170	B2	4/2005	Francois et al.	
6,890,297	B2	5/2005	Belson	
6,902,528	B1	6/2005	Garibaldi et al.	
6,960,161	B2	11/2005	Amling et al.	
6,974,411	B2	12/2005	Belson	
6,984,203	B2	1/2006	Tartaglia et al.	
7,018,331	B2	3/2006	Chang et al.	
7,087,013	B2	8/2006	Belson et al.	
7,338,505	B2	3/2008	Belson	
8,361,090	B2	1/2013	Belson	
2002/0016607	A1	2/2002	Bonadio et al.	
2002/0062062	A1	5/2002	Belson et al.	
2002/0082625	A1 *	6/2002	Huxel et al.	606/153
2002/0091398	A1	7/2002	Galdonik et al.	
2002/0120254	A1	8/2002	Julian et al.	
2002/0147385	A1	10/2002	Butler et al.	
2002/0151767	A1	10/2002	Sonnenschein et al.	
2002/0169361	A1	11/2002	Taniguchi et al.	
2002/0193662	A1	12/2002	Belson	
2003/0083550	A1	5/2003	Miyagi	
2003/0130598	A1	7/2003	Manning et al.	
2003/0167007	A1	9/2003	Belson	
2003/0171775	A1 *	9/2003	Belson	606/213
2003/0195387	A1	10/2003	Kortenbach et al.	
2003/0236505	A1	12/2003	Bonadio et al.	
2003/0236549	A1	12/2003	Bonadio et al.	
2004/0019254	A1	1/2004	Belson et al.	
2004/0106852	A1	6/2004	Windheuser et al.	
2004/0176683	A1	9/2004	Whitin et al.	
2004/0193008	A1	9/2004	Jaffe et al.	
2004/0193009	A1	9/2004	Jaffe et al.	
2004/0210109	A1	10/2004	Jaffe et al.	
2004/0220450	A1	11/2004	Jaffe et al.	
2005/0020901	A1	1/2005	Belson et al.	
2005/0085693	A1	4/2005	Belson et al.	
2005/0124855	A1	6/2005	Jaffe et al.	
2005/0154258	A1	7/2005	Tartaglia et al.	
2005/0154261	A1	7/2005	Ohline et al.	
2005/0165276	A1	7/2005	Belson et al.	
2005/0203339	A1	9/2005	Butler et al.	
2005/0209506	A1	9/2005	Butler et al.	
2005/0209509	A1	9/2005	Belson	
2005/0222497	A1	10/2005	Belson	
2005/0222498	A1	10/2005	Belson	
2006/0009678	A1	1/2006	Jaffe et al.	
2006/0052664	A1	3/2006	Julian et al.	
2006/0235457	A1	10/2006	Belson	
2006/0235458	A1	10/2006	Belson	
2006/0258912	A1	11/2006	Belson et al.	
2007/0043259	A1	2/2007	Jaffe et al.	
2007/0093858	A1	4/2007	Gambale et al.	
2007/0135803	A1	6/2007	Belson	
2007/0161291	A1	7/2007	Swinehart et al.	
2007/0161857	A1	7/2007	Durant et al.	
2007/0249901	A1	10/2007	Ohline et al.	
2007/0270650	A1	11/2007	Eno et al.	
2008/0154288	A1 *	6/2008	Belson	606/150

FOREIGN PATENT DOCUMENTS

DE	4102211	A1	8/1991
DE	19626433	A1	1/1998
DE	19729499	A1	1/1999
EP	165718	A2	12/1985
EP	382974	A1	8/1990
EP	497781	B1	1/1994
EP	993804	A1	4/2000
EP	1101442	A2	5/2001
FR	2732225	A1	10/1996
GB	2347685	A	9/2000

JP	63136014	A2	6/1988
JP	63272322	A2	11/1988
JP	1152413	A2	6/1989
JP	1229220	A2	9/1989
JP	1262372	A2	10/1989
JP	2246986	A2	10/1990
JP	2296209	A2	12/1990
JP	3136630	A2	6/1991
JP	4054970	A2	2/1992
JP	5011196	A2	1/1993
JP	5111458	A2	5/1993
JP	5305073	A2	11/1993
JP	6007287	A2	1/1994
JP	8322786	A2	12/1996
JP	9028662	A2	2/1997
JP	10337274	A2	12/1998
JP	11042258	A2	2/1999
JP	21046318	A2	2/2001
SU	871786	A1	10/1981
SU	1256955	A1	9/1986
SU	1301701	A1	4/1987
WO	9317751	A1	9/1993
WO	9419051	A1	9/1994
WO	9504556	A2	2/1995
WO	9509562	A1	4/1995
WO	9605768	A1	2/1996
WO	9710746	A1	3/1997
WO	9725101	A2	7/1997
WO	9729701	A1	8/1997
WO	9729710		8/1997
WO	9824017	A2	6/1998
WO	9849938	A1	11/1998
WO	9916359	A1	4/1999
WO	9933392	A1	7/1999
WO	9951283	A2	10/1999
WO	9959664	A1	11/1999
WO	0010456	A1	3/2000
WO	0027462	A1	5/2000
WO	0054653	A1	9/2000
WO	0074565	A1	12/2000
WO	0149353	A2	7/2001
WO	0167964	A2	9/2001
WO	0170096	A1	9/2001
WO	0170097	A1	9/2001
WO	0174235	A1	10/2001
WO	0180935	A1	11/2001
WO	0239909	A1	5/2002
WO	0247549	A1	6/2002
WO	02064028	A1	8/2002
WO	02068988	A1	9/2002
WO	02069841	A2	9/2002
WO	02089692	A1	11/2002
WO	02096276	A1	12/2002
WO	03028547	A2	4/2003
WO	2004019769	A1	3/2004
WO	2004084702	A2	10/2004

OTHER PUBLICATIONS

Berger, W. L. et al., "Sigmoid Stiffener for Decompression Tube Placement in Colonic Pseudo-Obstruction," Endoscopy, 2000, vol. 32, Issue 1, pp. 54-57.

Durant, et al.; U.S. Appl. No. 12/036,976 entitled "Systems and methods for articulating an elongate body," filed Feb. 25, 2008.

Hasson, H.M., "Technique of Open Laparoscopy," (from step 1 to step 9), May 1979, 2424 North Clark Street, Chicago, Illinois 60614, 3 pages.

Ireland Application No. 2000/0225, filed Mar. 22, 2000, Inventor Declan B., et al.

Ireland Application No. 2000/0559, filed Jul. 11, 2000, Inventor Declan B., et al.

Lee, Thomas S. et al., "A highly redundant robot system for inspection," Proceedings of Conference on Intelligent Robotics in Field, Factory, Service, and Space (CIRFFSS '94), Mar. 21-24, 1994, vol. 1, pp. 142-148. Houston, Texas.

(56)

References Cited

OTHER PUBLICATIONS

McKernan, J.B. et al., "Laparoscopic general surgery," Journal of the Medical Association of Georgia, Mar. 1990, vol. 79, Issue 3, pp. 157-159.

Slatkin, A.B. et al., "The development of a robotic endoscope," Proceedings 1995 IEEE/RSJ International Conference on Intelligent Robots and Systems, Aug. 5-9, 1995, vol. 2, pp. 162-171, Pittsburgh, Pennsylvania.

Vertut, Jean and Phillipe Coiffet, Robot Technology: Teleoperation and Robotics Evolution and Development, English translation, Prentice-Hall, Inc., Inglewood Cliffs, NJ, USA 1986, vol. 3A, 332 pages.

Woodley et al., U.S. Appl. No. 11/871,104 entitled "System for managing bowden cables in articulating instruments," filed Oct. 11, 2007.

* cited by examiner

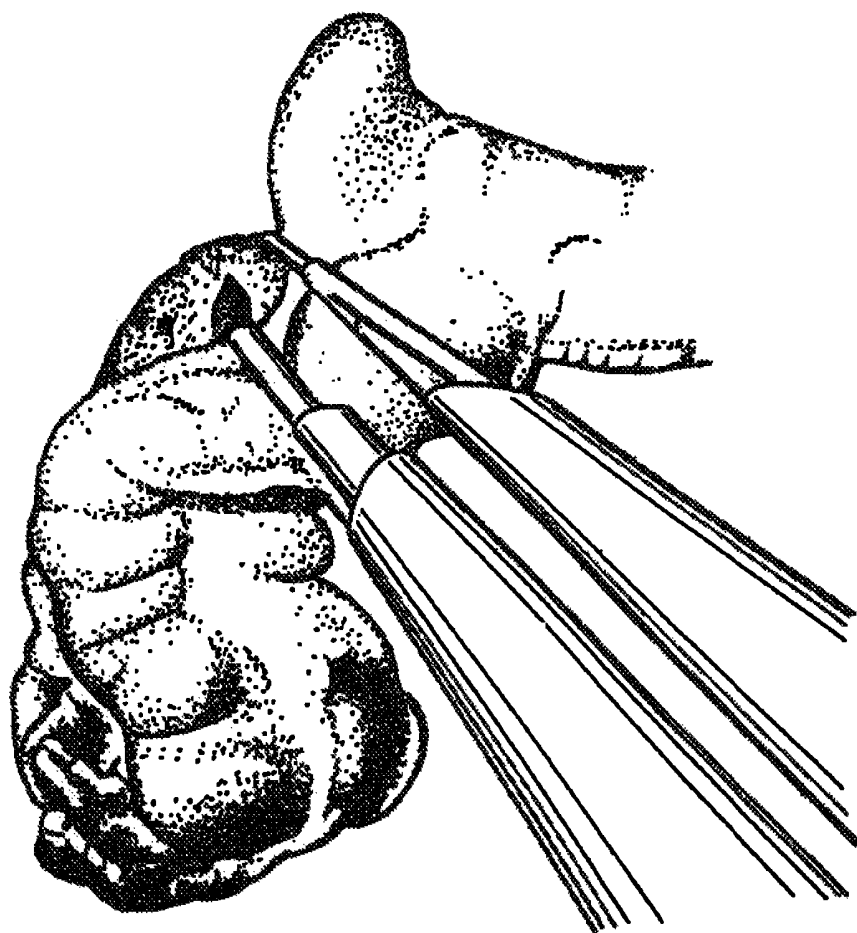


FIG. 1

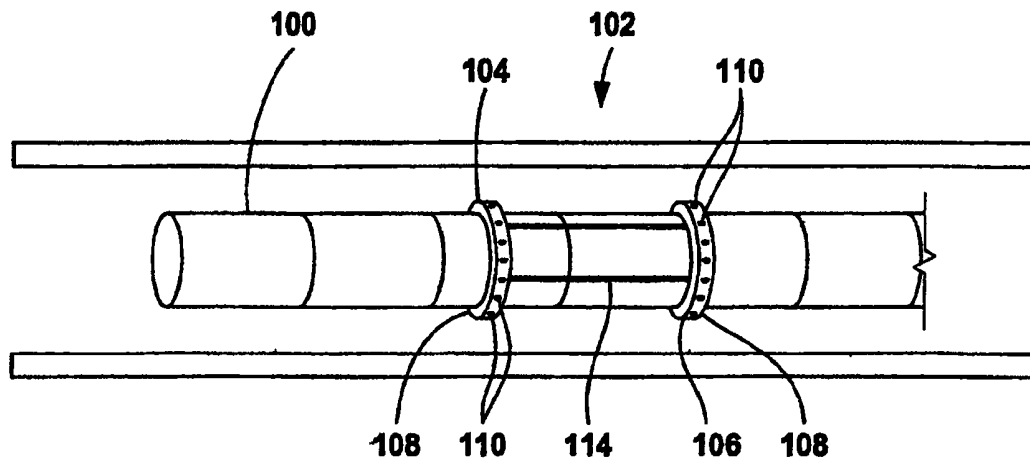


FIG 2

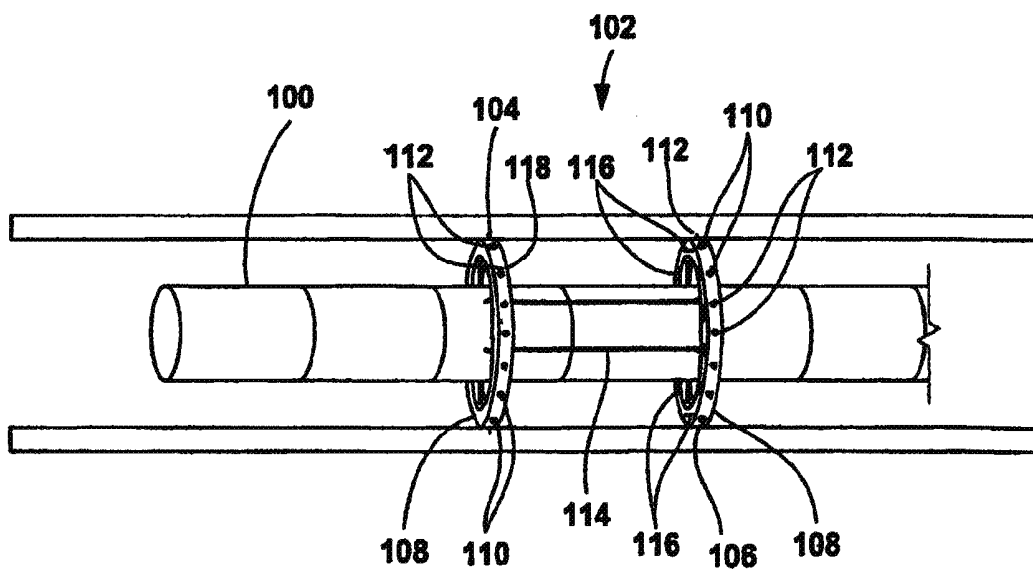
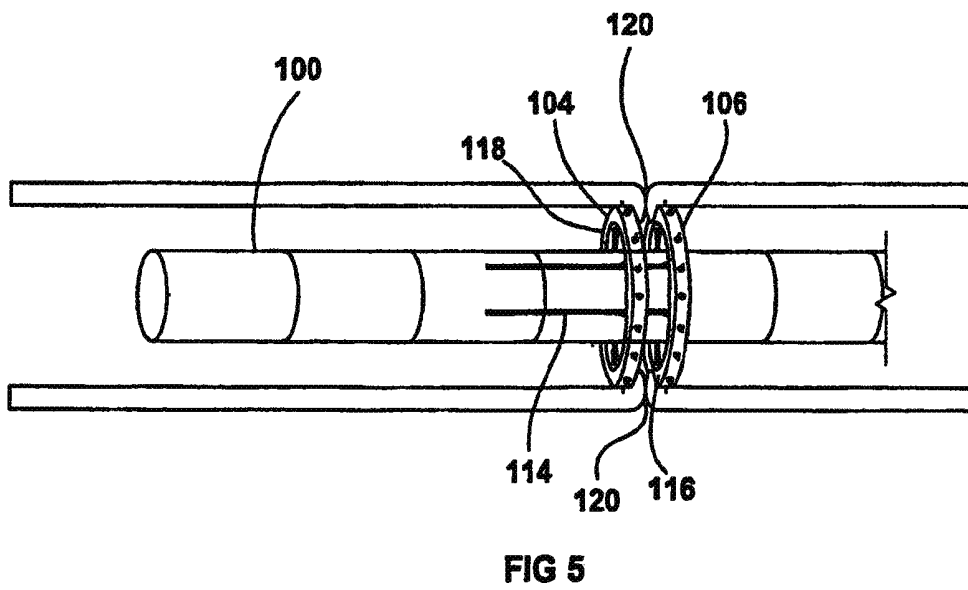
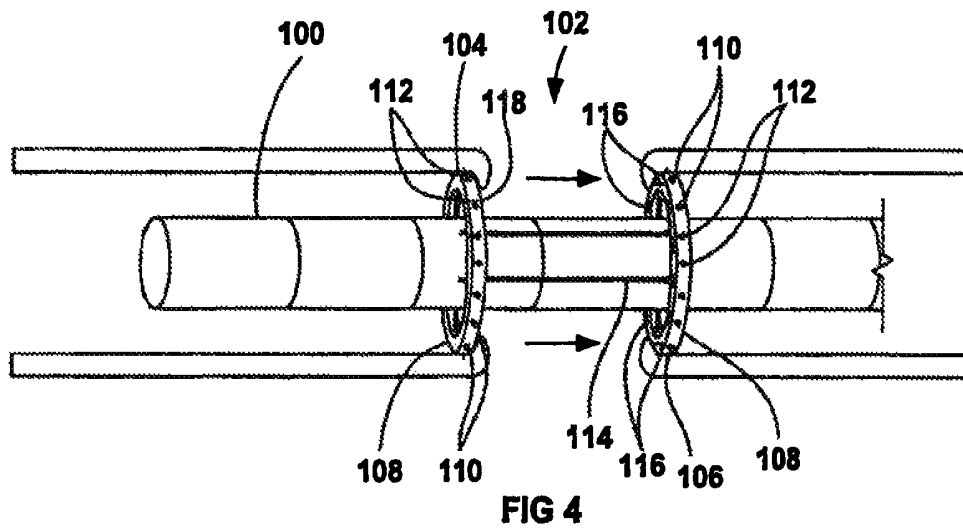


FIG 3



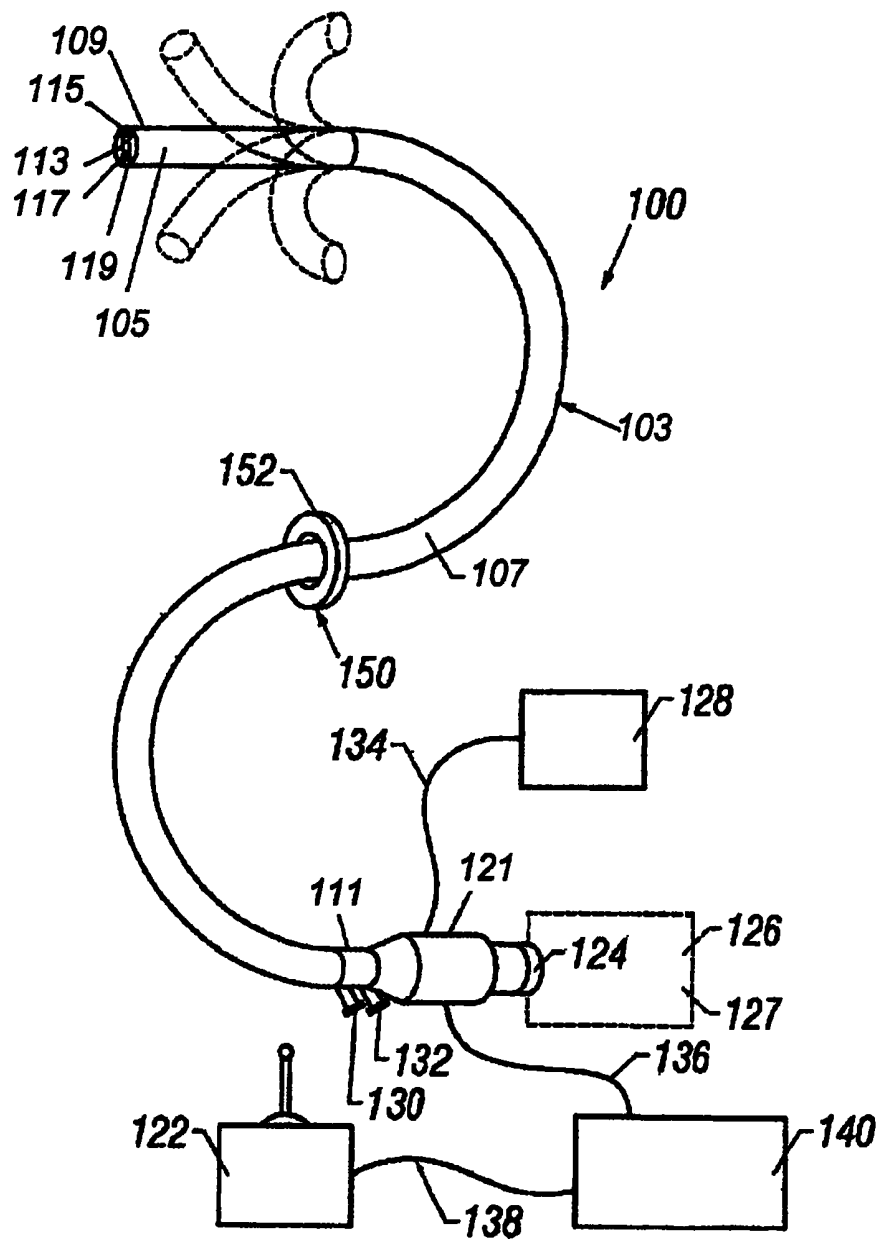


FIG. 6

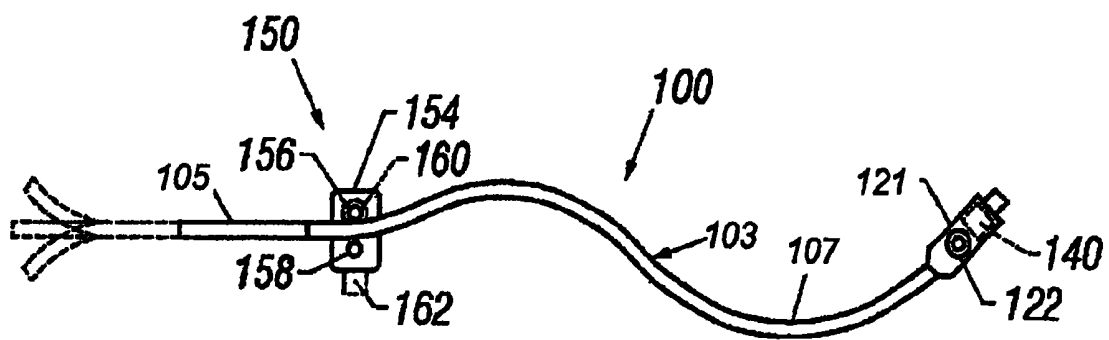


FIG. 7

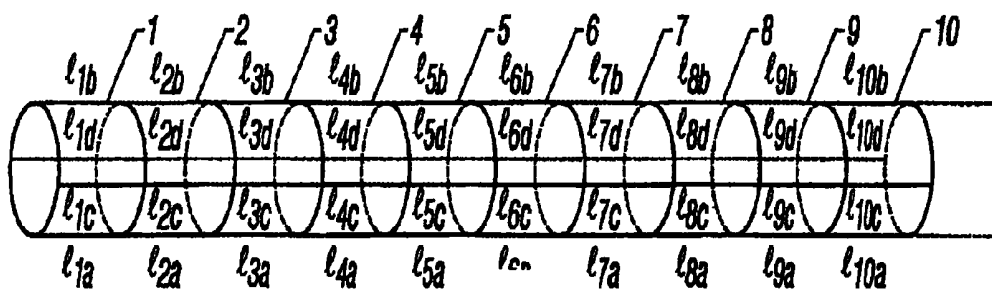


FIG. 8

103

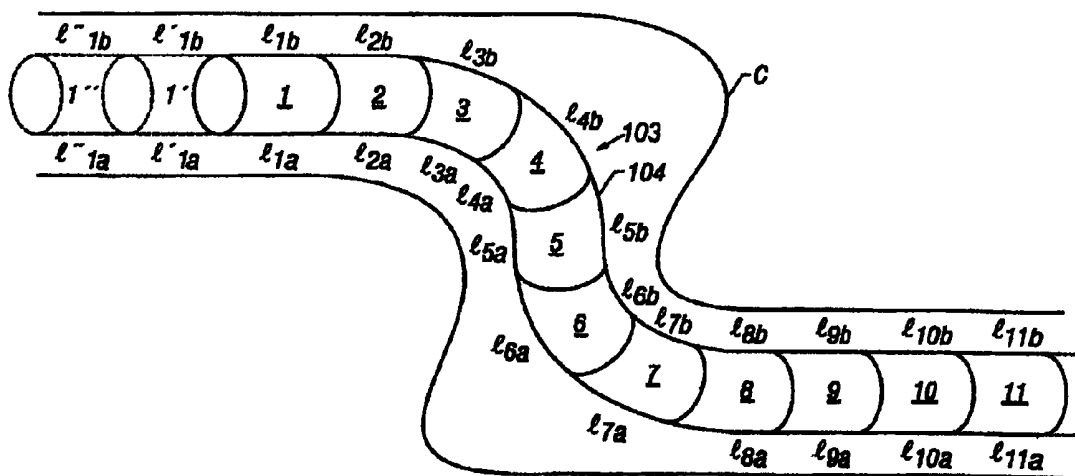


FIG. 9

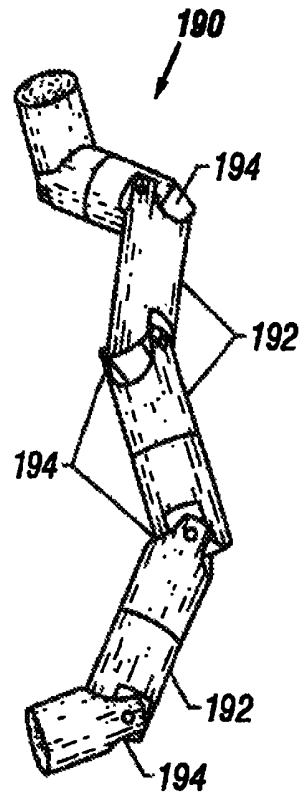


FIG. 10

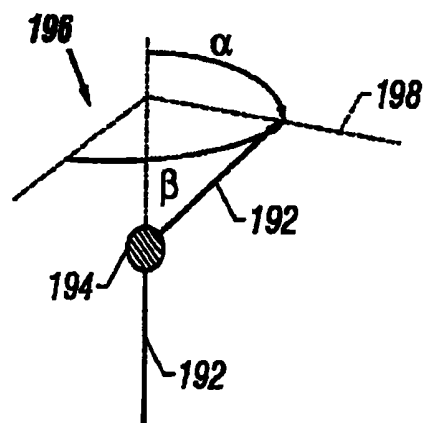


FIG. 11

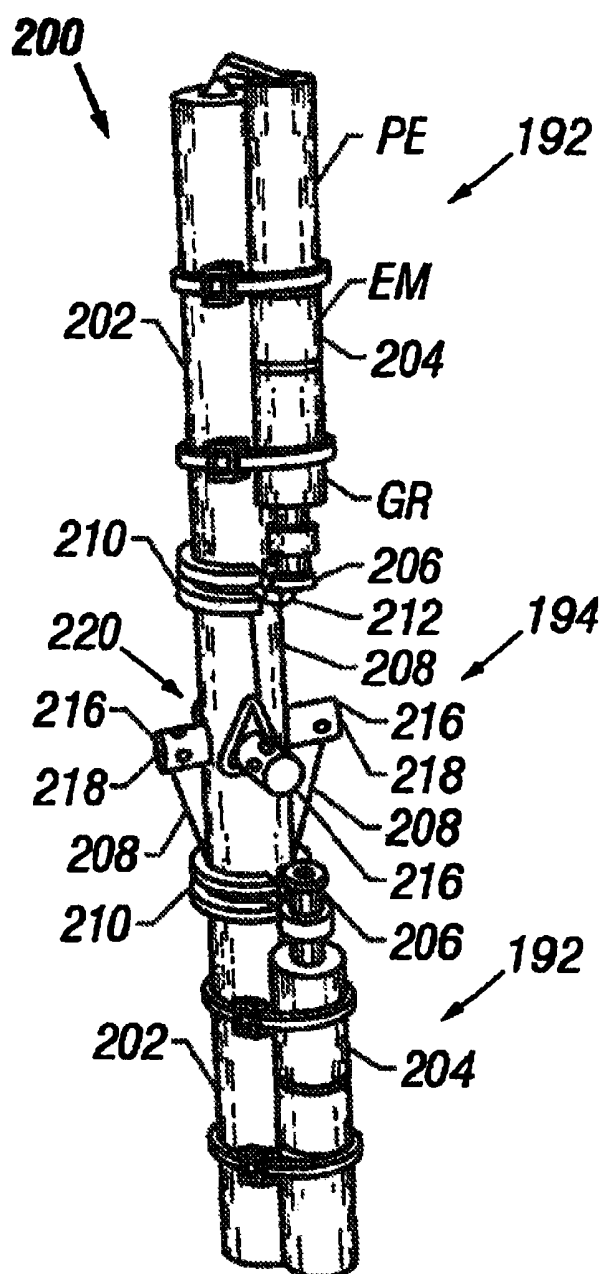


FIG. 12

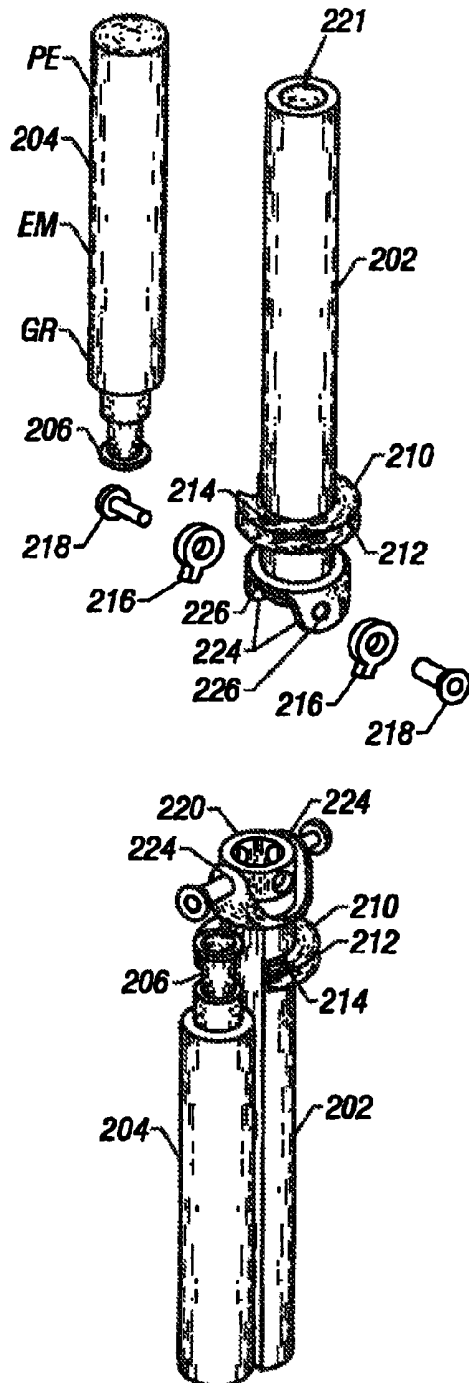


FIG. 13A

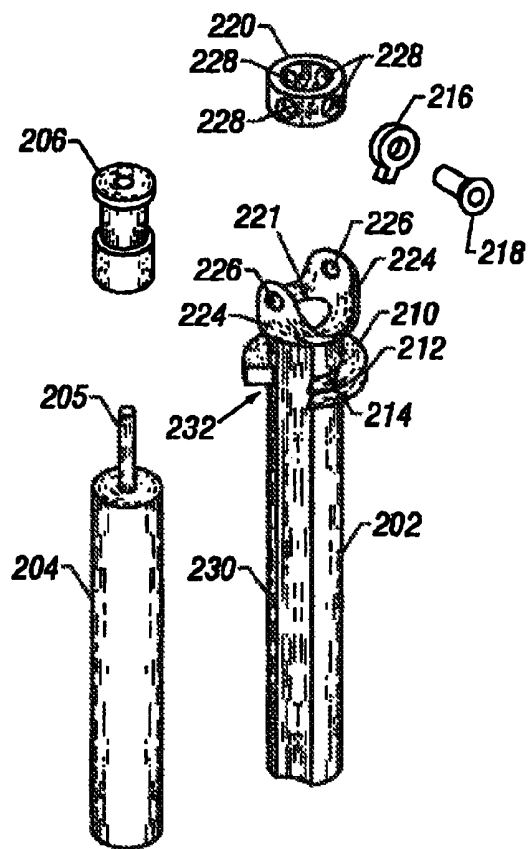


FIG. 13B

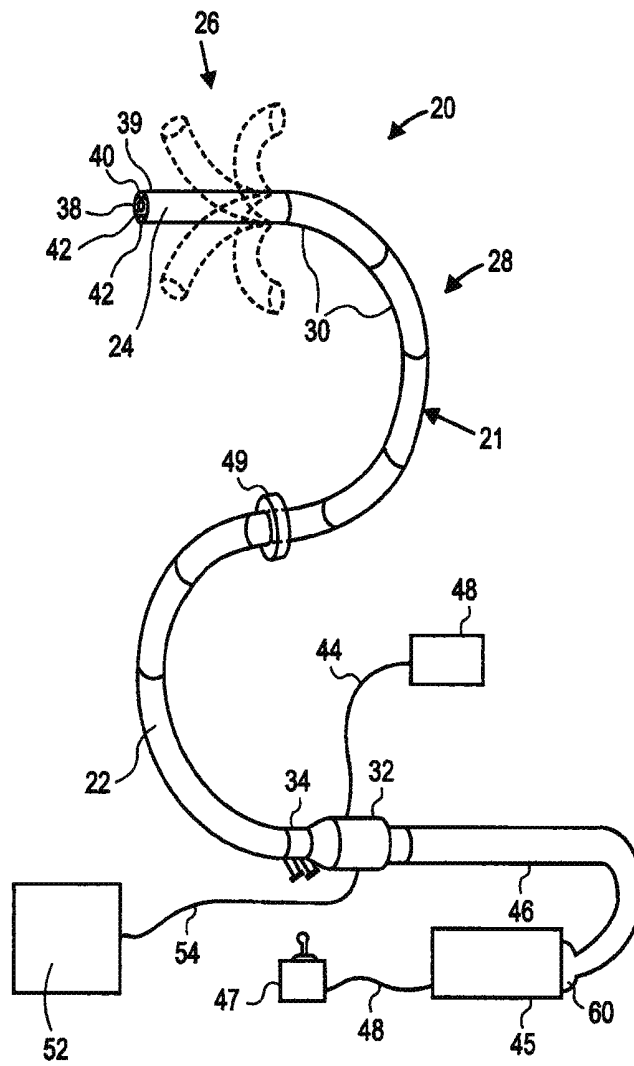


FIG. 14

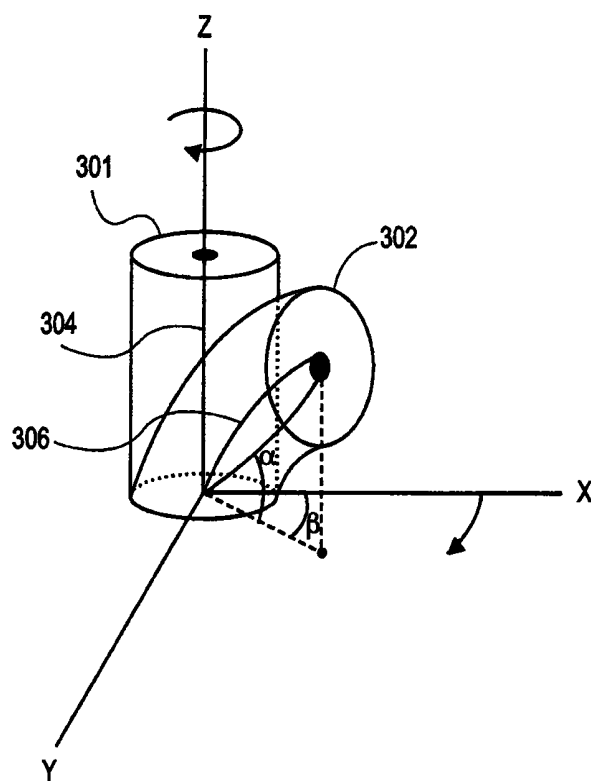


FIG. 15A

FIG. 15B

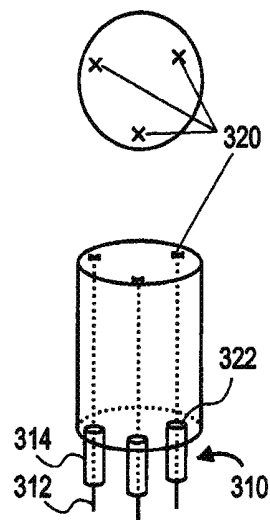


FIG. 15C

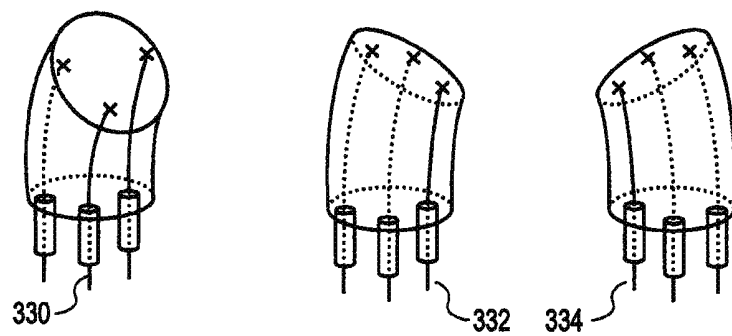


FIG. 15D

FIG. 15E

FIG. 15F

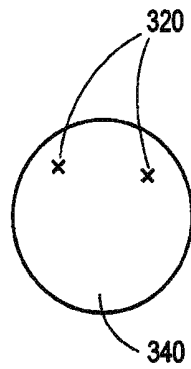


FIG. 16A

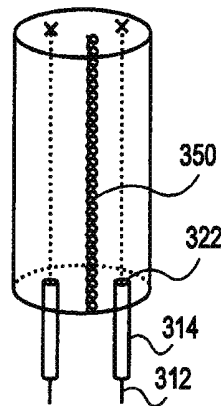


FIG. 16B

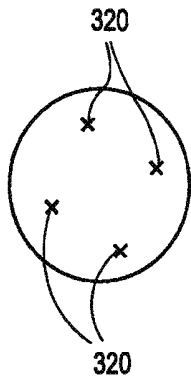


FIG. 16C

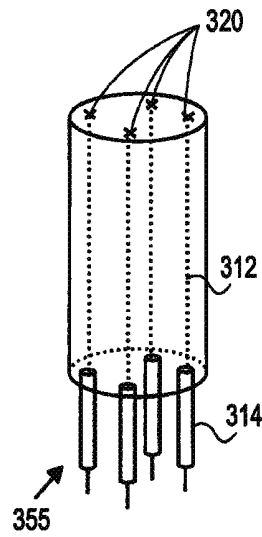
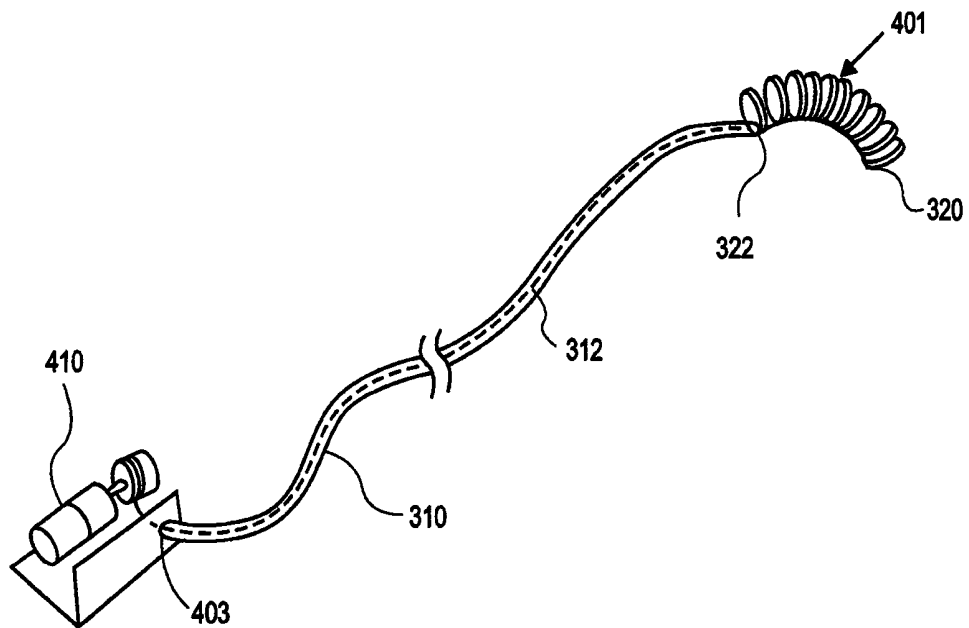


FIG. 16D

FIG. 17



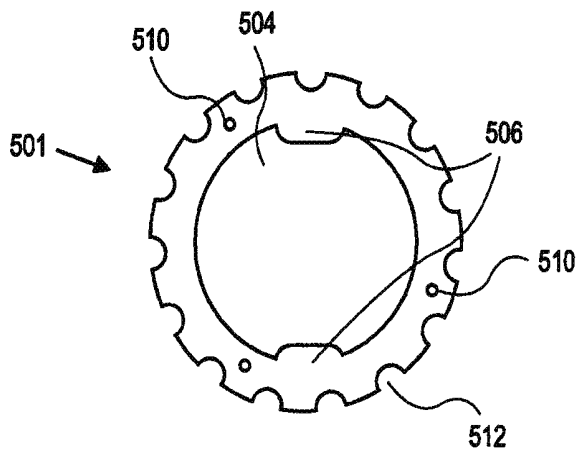


FIG. 18A

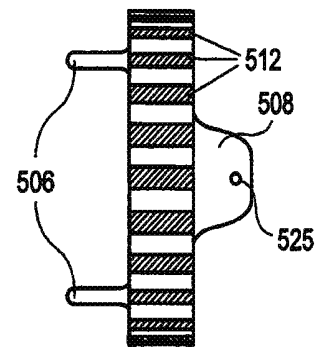


FIG. 18B

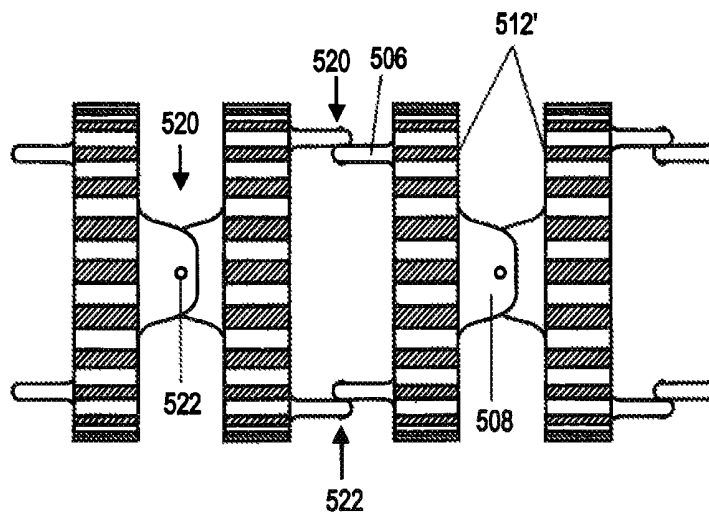


FIG. 18C

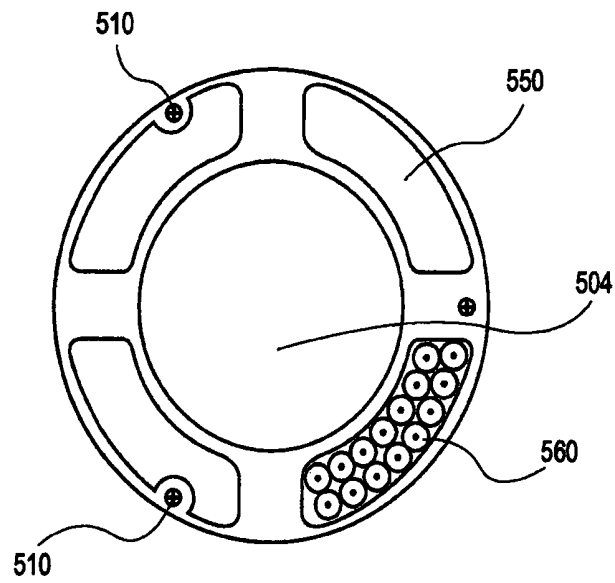


FIG. 18D

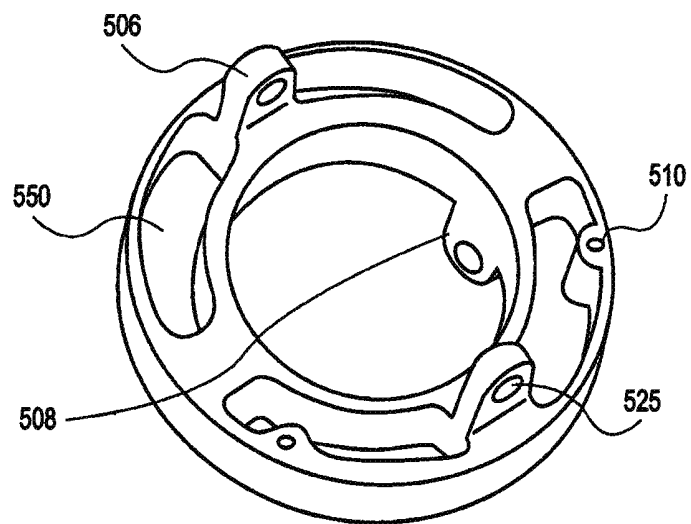


FIG. 18E

FIG. 19A

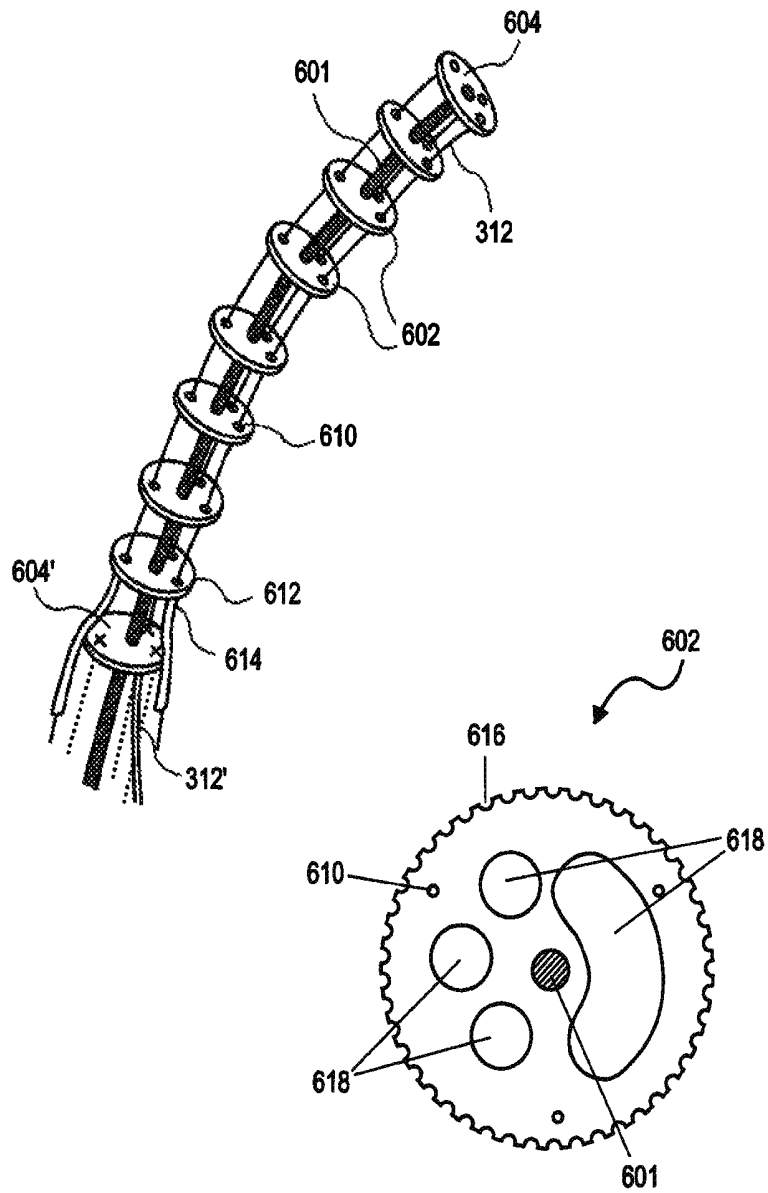


FIG. 19B

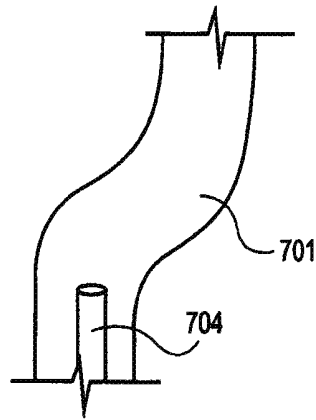


FIG. 20A

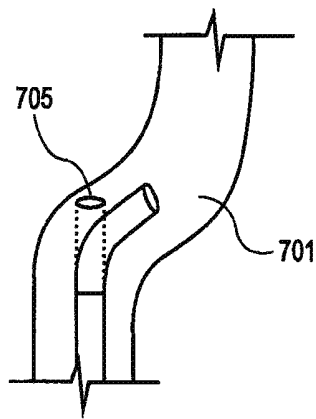


FIG. 20B

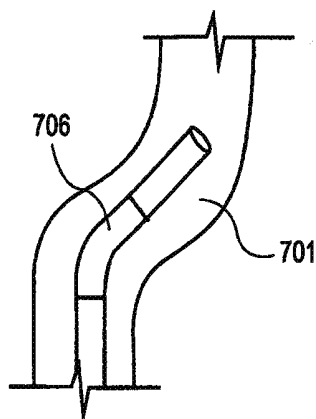


FIG. 20C

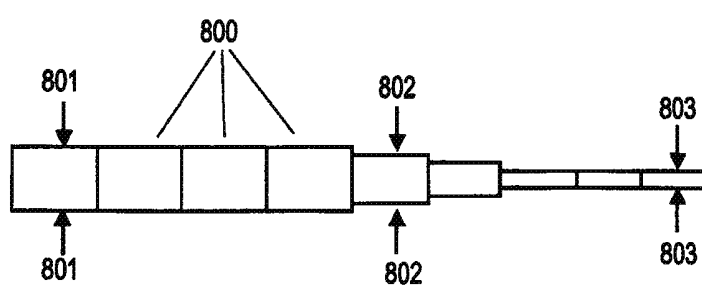


FIG. 21

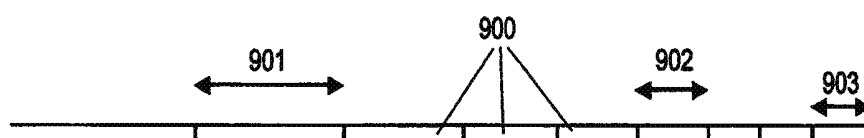


FIG. 22

APPARATUS AND METHOD FOR ENDOSCOPIC COLECTOMY

CROSS REFERENCE TO RELATED APPLICATIONS

This application is a divisional application of U.S. patent application Ser. No. 12/027,739 (filed Feb. 7, 2008; now U.S. Pat. No. 8,361,090 B2), which is a divisional application of U.S. patent application No. 10/327,370 (filed Dec. 20, 2002; now U.S. Pat. No. 7,338,505 B2), which claims the benefit of priority of U.S. Provisional Patent Application No. 60/347,674 (filed Jan. 9, 2002), which are all incorporated herein by reference in their entirety.

FIELD OF THE INVENTION

The present invention relates generally to surgical methods and apparatus. More particularly, it relates to methods and apparatus for performing endoscopic colectomy.

BACKGROUND OF THE INVENTION

Endoscopy studies the intraluminal aspects of hollow organs of the upper and lower intestine including the esophagus, stomach and the colon through cannulation of the lumen via the mouth or anus. Endoscopic polypectomy is presently limited to a submucosal resection. The endoscopist is often unable to completely resect a sessile polyp or lesion and therefore the patient is subjected to subsequent definitive surgery, i.e. resection of the base of the tumor. Endoscopic polypectomy can be used to debulk sessile masses but it is unable to resect mural disease. Incomplete resection of a sessile polyp may destroy the biopsy specimen and alter the relationship of the gross specimen given to the pathologist thereby resulting in the pathologist possibly providing incorrect or incomplete study results. The endoscopist is also unable to correct uncommon, but life threatening, procedural complications such as perforations. Other cases where resection is required are invasive tumors, perforation from different causes, inflammatory bowel disease, diverticulosis and others.

Surgical approaches for resecting diseased tissue are largely practiced by making large laparotomy incisions or using minimally invasive techniques such as laparoscopic surgery in which tissues are resected and repaired through small incisions.

There are numerous surgical devices enabling surgeons to resect diseased tissue and subsequently anastomose remaining tissue either through a conventional incision or using a laparoscope and making one or more relatively small incisions. Additionally, endoscopically assisted stapling devices are known which enable surgeons to remotely anastomose luminal structures such as the bowel. Endoscopically assisted bowel anastomosis nevertheless typically requires extraluminal assistance via a traditional laparotomy incision or use of a laparoscope.

Trends in surgery are towards minimally invasive procedures as evidenced by developments including laparoscopic cholecystectomy, laparoscopic appendectomy and laparoscopically assisted partial colectomies and hernia repairs. All of these minimally invasive procedures involve introducing a laparoscope through the abdominal wall and creating other associated openings to gain access to the peritoneal cavity in order to perform the necessary surgical procedure. Typically, general anesthesia is required. Endoscopically possible procedures include polypectomy, mucosectomy, and cauteriza-

tion. During "laparoscopic colectomy" today the colon is separated from its omentum laparoscopically and then the colon is exteriorized out of the abdominal cavity, through a laparotomy incision where the resection and anastomosis are performed extracorporeally.

Disadvantages of the laparoscopic method include the need to traverse the abdominal wall, increased operating time secondary to the lack of exposure for the procedure and possibly the need to convert to an "open" laparotomy in the course of performing the procedure.

Present stapling techniques in surgery are for the most part functionally adequate but limited. Devices exist including the GIA and EEA staplers which can be used to transect tissue in a linear or circular fashion, respectively, with subsequent anastomosis with staples. The linear GIA is relatively versatile. The EEA is primarily suited for lower colonic circular anastomosis after a lesion has been surgically removed (via laparotomy or laparoscopically) or during a colostomy take-down procedure.

The rigid post of the EEA stapler severely limits its use, as well as requiring that an open procedure be utilized. The steerable endoscopic stapler is useful in allowing for more bowel accessibility; however, it remains dependent upon transabdominal surgical exposure prior to utilization. While laparoscopic surgical instruments have been used for bowel anastomosis, in such procedures the bowel is exteriorized through the laparoscopic incision and anastomosed extracorporeally or in an augmented stapled side-to-side fashion.

U.S. Pat. Nos. 5,868,760 and 6,264,086 describe a method and apparatus for performing endoluminal resection of tissue, in particular for removal of diseased portions of a patient's colon. This purely endoluminal approach to colostomy does not fully address the surgical anatomy of the colon. As is well known, the colon and other viscera are connected and supported within the abdomen by the omentum, a membranous extension of the peritoneum that carries the blood supply to the colon. Resection of more than a small portion of the colon requires mobilization of the colon from the omentum and ligation or cauterization of the blood vessels supplying that portion of the colon. This aspect is not addressed by the endoluminal approach described; therefore it would be suitable for resecting only small portions of the colon.

Commonly owned and copending U.S. patent application Ser. Nos. 09/790,204 filed Feb. 20, 2001 (now U.S. Pat. No. 6,468,203); 09/969,927 filed Oct. 2, 2001; and 10/229,577 filed Aug. 27, 2002, describe steerable colonoscopes that uses serpentine motion to facilitate rapid and safe insertion of the colonoscope into a patient's colon. The technology described therein can also be used in conjunction with the methods and apparatus of the present invention to facilitate endoscopic colectomy or resection of any other part of the gastrointestinal system including, but not limited to, the esophagus, duodenum, jejunum and ileum or any other tubular organ like the bronchus. These patents and patent applications, and all other patents and patent applications referred to herein, are hereby incorporated by reference in their entirety.

SUMMARY OF THE INVENTION

In keeping with the foregoing discussion, the present invention takes the form of methods and apparatus for performing endoscopic colectomy that combine the advantages of the laparoscopic and endoluminal approaches. The diseased portion of the colon to be resected is identified using either laparoscopic and/or colonoscopic techniques or using another imaging modality. A colectomy device mounted on a colonoscope grasps the colon wall at two sites adjacent to a

diseased portion of the colon. Using laparoscopic techniques, the diseased portion of the colon is separated from the omentum and the blood vessels supplying it are ligated or cauterized. The colon wall is transected to remove the diseased portion and the excised tissue is removed using the laparoscope or drawn into the colectomy device for later removal upon withdrawal of the colonoscope. The colectomy device approximates the two ends of the colon and performs an end-to-end anastomosis. If the part to be resected is a tumor, prior to the resection, the edges of the segment to be resected will be stapled to seal it and prevent spillage of malignant cells to the healthy tissue.

The methods and apparatus of the present invention provide a number of benefits not realized by the prior art approaches to colectomy. As stated above, the purely endoluminal approach does not provide for separation of the colon from the omentum, which is necessary when resecting more than just a small portion of the colon wall. By combining laparoscopic techniques with a colonoscope-mounted colectomy device, the present invention overcomes this deficiency in the prior art allowing a more comprehensive approach to colectomy. Unlike prior art laparoscopic techniques, however, the colon does not need to be exteriorized for excision of the diseased portion or anastomosis of the remaining colon. The colonoscope-mounted colectomy device approximates the ends of the colon and performs an anastomosis from the interior of the lumen of the colon. The excised tissue can be drawn into the colectomy device for removal through the lumen of the colon along with the colonoscope or can be taken out by the laparoscope, which can be done through a very small incision in the patient's skin. The prior art approach also does not protect from leaking of malignant cells to the periphery. This idea will enable sealing of the tissue with staples at its ends to prevent such leakage. Optionally, it will be done with the help of a laparoscopic device that will serve as an anvil. Unlike the prior art procedure, the present invention will optionally use a balloon inflated in the lumen of the colon or any other resected organ before stapling, and by this assure the anastomosis will be ideal with the best possible approximation of the edges.

The use of colonoscopic techniques in the present invention provides another benefit not realized by a purely laparoscopic approach. Since colonoscopic examination is at present the most definitive diagnostic method for identifying diseases of the colon, locating the lesions through the exterior of the colon by laparoscopy or even by direct visualization can be somewhat problematic. Using the colonoscope to identify and isolate the diseased portion of the colon from within the lumen helps assure that the correct portions of the colon wall are excised and makes clean surgical margins without residual disease more assured as well.

In a preferred embodiment, the present invention utilizes a steerable colonoscope as described in U.S. patent application Ser. No. 09/790,204 (now U.S. Pat. No. 6,468,203); Ser. Nos. 09/969,927; and 10/229,577, which have been incorporated by reference. The steerable colonoscope described therein provides a number of additional benefits for performing endoscopic colectomy according to the present invention. The steerable colonoscope uses serpentine motion to facilitate rapid and safe insertion of the colonoscope into the patient's colon, which allows the endoscopic colectomy method to be performed more quickly and more safely. Beyond this however, the steerable colonoscope has the capability to create a three-dimensional mathematical model or map of the patient's colon and the location of any lesions identified during the initial examination. Lesions found during a previous examination by CT, MRI or any other imaging

technology can also be mapped onto the three-dimensional mathematical model of the colon. By generating a three-dimensional map of the colon, the system knows where each part of the endoscope is in the colon and will be able to localize the two parts of the dissecting and stapling system exactly in the desired location. During surgery, this information can be used to quickly and accurately return the colonoscope to the location of the identified lesions where the colonoscope-mounted colectomy device will be used to complete the endoscopic colectomy procedure.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a phantom drawing illustrating a diseased portion of the colon being separated from the omentum using laparoscopic techniques through a small incision in a patient's abdomen.

FIG. 2 is a cutaway drawing illustrating a steerable colonoscope with a colectomy device mounted thereon being inserted through the lumen of a patient's colon.

FIG. 3 is a cutaway drawing showing the gripping mechanism of the colonoscope-mounted colectomy device expanded within the lumen of the colon.

FIG. 4 illustrates the colon after the diseased portion has been excised and removed with the colonoscope-mounted colectomy device in position to approximate the transected ends of the colon.

FIG. 5 illustrates the colonoscope-mounted colectomy device performing an end-to-end anastomosis to complete the endoscopic colectomy procedure.

FIG. 6 shows a first embodiment of the steerable endoscope of the present invention.

FIG. 7 shows a second embodiment of the steerable endoscope of the present invention.

FIG. 8 shows a wire frame model of a section of the body of the endoscope in a neutral or straight position.

FIG. 9 shows the wire frame model of the endoscope body shown in FIG. 8 passing through a curve in a patient's colon.

FIG. 10 shows a representative portion of an alternative endoscopic body embodiment having multiple segments interconnected by joints.

FIG. 11 shows a partial schematic representation of the embodiment of FIG. 10 showing two segments being pivotable about two independent axes.

FIG. 12 shows a preferable endoscope embodiment having motorized segmented joints.

FIGS. 13A-13B show exploded isometric assembly views of two adjacent segments and an individual segment, respectively, from the embodiment shown in FIG. 12.

FIG. 14 shows a variation of the tendon driven endoscope of the present invention.

FIG. 15A shows the range of motion of a controllable segment of the present invention actuated by three tendons.

FIGS. 15B to 15F show the use of three tendons to actuate a controllable segment used in the endoscope of the present invention.

FIGS. 16A and 16B show the use of two tendons to actuate a controllable segment in the endoscope of the present invention.

FIGS. 16C and 16D show the use of four tendons to actuate a controllable segment in the endoscope of the present invention.

FIG. 17 shows a partial schematic representation of a single tendon bending a segment.

FIGS. 18A and 18B show an end view and a side view, respectively, of a vertebra-type control ring which may be used to form the controllable segments of the endoscope of the present invention.

FIG. 18C shows a side view of interconnected vertebra-type control rings used to form the controllable segments of the endoscope of the present invention.

FIGS. 18D and 18E show a side view and a perspective view, respectively, of another embodiment of a vertebra-type control ring.

FIG. 19A shows a perspective view of an endoscope device variation with the outer layers removed to reveal the control rings and backbone.

FIG. 19B shows an end view of a variation of the control ring for an endoscope of the present invention.

FIGS. 20A to 20C illustrate advancing the tendon driven endoscope of the present invention through a tortuous path.

FIG. 21 shows a variation of the tendon driven endoscope of the present invention that has segments of differing diameters.

FIG. 22 shows a variation of the tendon-driven endoscope of the present invention that has segments of different length.

DETAILED DESCRIPTION OF THE INVENTION

FIG. 2 is a cutaway drawing illustrating a steerable colonoscope 100 with a colectomy device 102 mounted thereon being inserted through the lumen of a patient's colon. As mentioned before, the same technique may apply for every other tubular shaped organ. Preferably, the steerable colonoscope 100 is constructed as described in U.S. patent application Ser. No. 09/790,204 (now U.S. Pat. No. 6,468,203); Ser. No. 09/969,927 (now U.S. Pat. No. 6,610,007); and Ser. No. 10/229,577 (now U.S. Pat. No. 6,858,005), with multiple articulating segments that are controlled to move with a serpentine motion that facilitates insertion and withdrawal of the colonoscope with a minimum of contact and stress applied to the colon walls. Additional details and various embodiments of the steerable colonoscope 100 are described below with reference to FIGS. 6-22. In addition, the control system of the steerable colonoscope 100 has the capability to construct a three-dimensional mathematical model or map of the colon as it advances through lumen under control of the operator. The three-dimensional mathematical model of the colon and the location and nature of any lesions identified in the course of an initial colonoscopic examination can be stored and used in performance of the endoscopic colectomy procedure. In alternate embodiments, the colectomy device 102 of the present invention may be mounted on a colonoscope of a different design and construction.

The colectomy device 102 can be permanently or removably mounted on the steerable colonoscope 100. The colectomy device 102 has a distal component 104 and a proximal component 106. The distal component 104 and the proximal component 106 each have an expandable member 108 and a gripping mechanism 110 for gripping the wall of the colon. The expandable member 108 may be an inflatable balloon or a mechanically expandable mechanism. The gripping mechanism 110 may comprise a plurality of circumferentially located ports within which attachment points 112, e.g., needles, hooks, barbs, etc., may be retractably positioned about an exterior surface of the expandable member 108. Alternatively, the gripping mechanism 110 may utilize a vacuum gripper through a plurality of circumferentially located ports around the distal component 104 and/or the proximal component 106 or other known gripping mechanisms. In the case of the vacuum gripper, gripping mechanism

110 is in fluid communication through the ports and through the colonoscope 100 to the proximal end of the colonoscope 100 to a vacuum pump (not shown). At least one, and optionally both, of the distal component 104 and the proximal component 106 are movable longitudinally with respect to the body of the steerable colonoscope 100. Rails, grooves or the like 114 may be provided on the body of the steerable colonoscope 100 for guiding the longitudinal movement of the distal component 104 and the proximal component 106.

In addition, the colectomy device 102 includes a surgical stapler 116 or other anastomosis mechanism. The surgical stapler 116 is carried on either the distal component 104 or the proximal component 106 and a stapler anvil 118 is carried on the other of these components. The surgical stapler 116 may be configured similarly to any number of conventional stapling devices which are adapted to actuate staples into tissue. Another option is that there is a stapler and an anvil on both components for stapling and sealing the edges. Optionally, the colectomy device 102 may include a cutting device and/or electrocautery and/or a laser device for transecting the colon wall. Optionally, the colectomy device 102 may also include a vacuum mechanism or the like for drawing the excised tissue into the colectomy device 102 for later removal along with the steerable colonoscope 100.

FIG. 2 shows the steerable colonoscope 100 with the expandable members 108 of the distal component 104 and the proximal component 106 in a contracted or deflated condition for easy passage through the lumen of the patient's colon. The control system of the steerable colonoscope 100 monitors the position of each segment of the colonoscope 100 as it is advanced within the colon and can signal to the operator when the segments carrying the distal component 104 and the proximal component 106 of the colectomy device 102 are correctly positioned with respect to a previously detected lesion in the colon. Alternatively, the control system of the steerable colonoscope 100 can be programmed to advance the colonoscope 100 automatically through the lumen of the colon and to stop it when the distal component 104 and the proximal component 106 of the colectomy device 102 are correctly positioned with respect to the lesion in the colon. Alternatively, the control system will be able to automatically guide and deliver the two components to the desired location after the colonoscope has been inserted to the colon.

FIG. 3 is a cutaway drawing showing the expandable members 108 of the distal component 104 and the proximal component 106 of the colonoscope-mounted colectomy device 102 expanded within the lumen of the colon so that the gripping mechanism 110 grips the wall of the colon. The distal component 104 and the proximal component 106 may be expanded through any number of expansion devices. For instance, they may be radially expanded upon spoke-like support structures or they may be configured to radially expand in a rotational motion until the desired expansion diameter is attained. At this point, with the diseased portion of the colon identified and isolated by the colonoscope-mounted colectomy device 102, the diseased portion is separated from the omentum and the blood vessels supplying it are ligated and/or cauterized using laparoscopic techniques. FIG. 1 is a phantom drawing illustrating a diseased portion of the colon being separated from the omentum using laparoscopic techniques through a small incision in a patient's abdomen.

Next, the diseased portion of the colon is excised by transecting the colon at the proximal and distal end of the diseased portion. The colon may be transected using laparoscopic techniques or using a cutting mechanism and/or electrocautery device mounted on the colectomy device 102. The excised tissue is removed using the laparoscope or drawn into

the colectomy device **102** for later removal upon withdrawal of the steerable colonoscope **100**. FIG. 4 illustrates the colon after the diseased portion has been excised and removed with the colonoscope-mounted colectomy device **102** in position to approximate the transected ends of the colon.

The remaining ends of the colon are approximated one to the other by moving the distal component **104** and/or the proximal component **106** longitudinally with respect to the body of the steerable colonoscope **100**, as shown by the arrows. Optionally, the proximal component **106** may be longitudinally translated towards the distal component **104** or both components **104**, **106** may be approximated simultaneously towards one another. The ends of the colon are stapled to one another to create an end-to-end anastomosis **120** using the surgical stapler **116** and stapler anvil **118** on the colectomy device **102**. Once the ends of the tissue have been approximated, staples or other fastening devices, e.g., clips, screws, adhesives, sutures, and combinations thereof, etc., may be actuated through the surgical stapler **116** such that they pierce both ends of the tissue against the stapler anvil **118**. FIG. 5 illustrates the colonoscope-mounted colectomy device performing an end-to-end anastomosis **120** to complete the endoscopic colectomy procedure. Once the anastomosis **120** is complete, the expandable members **108** of the distal component **104** and the proximal component **106** are deflated or contracted and the steerable colonoscope **100** and the colectomy device **102** are withdrawn from the patient's body. The expanded members will assure a very accurate end-to-end anastomosis and prevent stenosis that can happen as a result of inaccurate approximation of the two ends.

In an alternative method using the colonoscope-mounted colectomy device **102**, the diseased portion of the colon may be excised using a cutting device within the colectomy device **102** after the ends of the diseased portion have been approximated and anastomosed. The excised tissue is drawn into the colectomy device **102** and removed when the steerable colonoscope **100** is withdrawn from the patient.

In another alternative method, the colectomy procedure may be performed entirely from the endoluminal approach using the colonoscope-mounted colectomy device **102** without laparoscopic assistance. This method would be particularly advantageous for resection of small portions of the colon where it may not be necessary to mobilize an extended portion of the colon from the omentum to achieve successful approximation and anastomosis. The three-dimensional mapping capability of the steerable colonoscope **102** would be used to locate previously identified lesions without laparoscopic assistance.

Steerable Colonoscope

FIG. 6 shows a first embodiment of the steerable endoscope **100** of the present invention. The endoscope **100** has an elongate body **103** with a manually or selectively steerable distal portion **105** and an automatically controlled proximal portion **107**. The selectively steerable distal portion **105** can be selectively steered or bent up to a full 180 degree bend in any direction. A fiberoptic imaging bundle **113** and one or more illumination fibers **115** extend through the body **103** from the proximal end **111** to the distal end **109**. Alternatively, the endoscope **100** can be configured as a video endoscope with a miniaturized video camera, such as a CCD camera, positioned at the distal end **109** of the endoscope body **103**. The images from the video camera can be transmitted to a video monitor by a transmission cable or by wireless transmission. Optionally, the body **103** of the endoscope **100** may include one or two instrument channels **117**, **119** that may also be used for insufflation or irrigation. The body **103** of the endoscope **100** is highly flexible so that it is able to bend

around small diameter curves without buckling or kinking. When configured for use as a colonoscope, the body **103** of the endoscope **100** is typically from 135 to 185 cm in length and approximately 12-13 mm in diameter. The endoscope **100** can be made in a variety of other sizes and configurations for other medical and industrial applications.

A proximal handle **121** is attached to the proximal end **111** of the elongate body **103**. The handle **121** includes an ocular **124** connected to the fiberoptic imaging bundle **113** for direct viewing and/or for connection to a video camera **126**. The handle **121** is connected to an illumination source **128** by an illumination cable **134** that is connected to or continuous with the illumination fibers **115**. A first luer lock fitting **130** and a second luer lock fitting **132** on the handle **121** are connected to the instrument channels **117**, **119**.

The handle **121** is connected to an electronic motion controller **140** by way of a controller cable **136**. A steering control **122** is connected to the electronic motion controller **140** by way of a second cable **138**. The steering control **122** allows the user to selectively steer or bend the selectively steerable distal portion **105** of the body **103** in the desired direction. The steering control **122** may be a joystick controller as shown, or other known steering control mechanism. The electronic motion controller **140** controls the motion of the automatically controlled proximal portion **107** of the body **103**. The electronic motion controller **140** may be implemented using a motion control program running on a microcomputer or using an application-specific motion controller. Alternatively, the electronic motion controller **140** may be implemented using a neural network controller.

An axial motion transducer **150** is provided to measure the axial motion of the endoscope body **103** as it is advanced and withdrawn. The axial motion transducer **150** can be made in many possible configurations. By way of example, the axial motion transducer **150** in FIG. 6 is configured as a ring **152** that surrounds the body **103** of the endoscope **100**. The axial motion transducer **150** is attached to a fixed point of reference, such as the surgical table or the insertion point for the endoscope **100** on the patient's body. As the body **103** of the endoscope **100** slides through the axial motion transducer **150**, it produces a signal indicative of the axial position of the endoscope body **103** with respect to the fixed point of reference and sends a signal to the electronic motion controller **140** by telemetry or by a cable (not shown). The axial motion transducer **150** may use optical, electronic or mechanical means to measure the axial position of the endoscope body **103**. Other possible configurations for the axial motion transducer **150** are described below.

FIG. 7 shows a second embodiment of the endoscope **100** of the present invention. As in the embodiment of FIG. 6, the endoscope **100** has an elongate body **103** with a selectively steerable distal portion **105** and an automatically controlled proximal portion **107**. The steering control **122** is integrated into proximal handle **121** in the form of one or two dials for selectively steering the selectively steerable distal portion **105** of the endoscope **100**. Optionally, the electronic motion controller **140** may be miniaturized and integrated into proximal handle **121**, as well. In this embodiment, the axial motion transducer **150** is configured with a base **154** that is attachable to a fixed point of reference, such as the surgical table. A first roller **156** and a second roller **158** contact the exterior of the endoscope body **103**. A multi-turn potentiometer **160** or other motion transducer is connected to the first roller **156** to measure the axial motion of the endoscope body **103** and to produce a signal indicative of the axial position.

The endoscope **100** may be manually advanced or withdrawn by the user by grasping the body **103** distal to the axial

motion transducer **150**. Alternatively, the first roller **156** and/or second roller **158** may be connected to a motor **162** for automatically advancing and withdrawing the body **103** of the endoscope **100**.

FIG. **8** shows a wire frame model of a section of the body **103** of the endoscope **100** in a neutral or straight position. Most of the internal structure of the endoscope body **103** has been eliminated in this drawing for the sake of clarity. The endoscope body **103** is divided up into sections **1, 2, 3 . . . 10**, etc. The geometry of each section is defined by four length measurements along the a, b, c and d axes. For example, the geometry of section **1** is defined by the four length measurements $l_{1a}, l_{1b}, l_{1c}, l_{1d}$, and the geometry of section **2** is defined by the four length measurements $l_{2a}, l_{2b}, l_{2c}, l_{2d}$, etc. Preferably, each of the length measurements is individually controlled by a linear actuator (not shown). The linear actuators may utilize one of several different operating principles. For example, each of the linear actuators may be a self-heating NiTi alloy linear actuator or an electrorheological plastic actuator, or other known mechanical, pneumatic, hydraulic or electromechanical actuator. The geometry of each section may be altered using the linear actuators to change the four length measurements along the a, b, c and d axes. Preferably, the length measurements are changed in complementary pairs to selectively bend the endoscope body **103** in a desired direction. For example, to bend the endoscope body **103** in the direction of the a axis, the measurements $l_{1a}, l_{2a}, l_{3a} . . . l_{10a}$, would be shortened and the measurements $l_{1b}, l_{2b}, l_{3b} . . . l_{10b}$, would be lengthened an equal amount. The amount by which these measurements are changed determines the radius of the resultant curve.

In the selectively steerable distal portion **105** of the endoscope body **103**, the linear actuators that control the a, b, c and d axis measurements of each section are selectively controlled by the user through the steering control **122**. Thus, by appropriate control of the a, b, c and d axis measurements, the selectively steerable distal portion **105** of the endoscope body **103** can be selectively steered or bent up to a full 180° in any direction.

In the automatically controlled proximal portion **107**, however, the a, b, c and d axis measurements of each section are automatically controlled by the electronic motion controller **140**, which uses a curve propagation method to control the shape of the endoscope body **103**. To explain how the curve propagation method operates, FIG. **9** shows the wire frame model of a part of the automatically controlled proximal portion **107** of the endoscope body **103** shown in FIG. **8** passing through a curve in a patient's colon C. For simplicity, an example of a two-dimensional curve is shown and only the a and b axes will be considered. In a three-dimensional curve all four of the a, b, c and d axes would be brought into play.

In FIG. **9**, the endoscope body **103** has been maneuvered through the curve in the colon C with the benefit of the selectively steerable distal portion **105** (this part of the procedure is explained in more detail below) and now the automatically controlled proximal portion **107** resides in the curve. Sections **1** and **2** are in a relatively straight part of the colon C, therefore $l_{1a}=l_{1b}$, and $l_{2a}=l_{2b}$. However, because sections **3-7** are in the S-shaped curved section, $l_{3a}<l_{3b}$, $l_{4a}<l_{4b}$, and $l_{5a}<l_{5b}$, but $l_{6a}>l_{6b}$, $l_{7a}>l_{7b}$ and $l_{8a}>l_{8b}$. When the endoscope body **103** is advanced distally by one unit, section **1** moves into the position marked **1'**, section **2** moves into the position previously occupied by section **1**, section **3** moves into the position previously occupied by section **2**, etc. The axial motion transducer **150** produces a signal indicative of the axial position of the endoscope body **103** with respect to a fixed point of reference and sends the signal to the electronic

motion controller **140**. Under control of the electronic motion controller **140**, each time the endoscope body **103** advances one unit, each section in the automatically controlled proximal portion **106** is signaled to assume the shape of the section that previously occupied the space that it is now in. Therefore, when the endoscope body **103** is advanced to the position marked **1'**, $l_{1a}=l_{1ab}$, $l_{2a}=l_{2b}$, $l_{3a}=l_{3b}$, $l_{4a}<l_{4b}$, $l_{5a}<l_{5b}$, $l_{6a}<l_{6b}$, $l_{7a}>l_{7b}$, $l_{8a}>l_{8b}$, and $l_{9a}>l_{9b}$, and, when the endoscope body **103** is advanced to the position marked **1''**, $l_{1a}=l_{1b}$, $l_{2a}=l_{2b}$, $l_{3a}=l_{3b}$, $l_{4a}=l_{4b}$, $l_{5a}<l_{5b}$, $l_{6a}<l_{6b}$, $l_{7a}<l_{7b}$, $l_{8a}>l_{8b}$, $l_{9a}>l_{9b}$, and $l_{10a}>l_{10b}$. Thus, the S-shaped curve propagates proximally along the length of the automatically controlled proximal portion **107** of the endoscope body **103**. The S-shaped curve appears to be fixed in space, as the endoscope body **103** advances distally.

Similarly, when the endoscope body **103** is withdrawn proximally, each time the endoscope body **103** is moved proximally by one unit, each section in the automatically controlled proximal portion **107** is signaled to assume the shape of the section that previously occupied the space that it is now in. The S-shaped curve propagates distally along the length of the automatically controlled proximal portion **107** of the endoscope body **103**, and the S-shaped curve appears to be fixed in space, as the endoscope body **103** withdraws proximally.

Whenever the endoscope body **103** is advanced or withdrawn, the axial motion transducer **150** detects the change in position and the electronic motion controller **140** propagates the selected curves proximally or distally along the automatically controlled proximal portion **107** of the endoscope body **103** to maintain the curves in a spatially fixed position. This allows the endoscope body **103** to move through tortuous curves without putting unnecessary force on the wall of the colon C.

FIG. **10** shows a representative portion of an alternative endoscopic body embodiment **190** which has multiple segments **192** interconnected by joints **194**. In this embodiment, adjacent segments **192** can be moved or angled relative to one another by a joint **194** having at least one degree-of-freedom, and preferably having multiple degrees-of-freedom, preferably about two axes as shown here. As seen further in FIG. **4**, a partial schematic representation **196** of the embodiment **190** is shown where two segments **192** may be rotated about joint **194** about the two independent axes. The range of motion may be described in relation to spherical axes **198** by angles α and β .

As mentioned above, such a segmented body may be actuated by a variety of methods. A preferable method involves the use of electromechanical motors individually mounted on each individual segment to move the segments relative to one another. FIG. **12** shows a preferable embodiment **200** having motorized segmented joints. Each segment **192** is preferably comprised of a backbone segment **202**, which also preferably defines at least one lumen running through it to provide an access channel through which wires, optical fibers, air and/or water channels, various endoscopic tools, or any variety of devices and wires may be routed through. The backbone segment may be made of a variety of materials which are preferably biocompatible and which provide sufficient strength to support the various tools and other components, e.g., stainless steel. Although much of the description is to an individual segment **192**, each of the segments **192** are preferably identical, except for the segment (or first few segments) located at the distal tip, and the following description readily applies to at least a majority of the segments **192**.

A single motor, or multiple motors depending upon the desired result and application, may be attached to at least a

majority of the segments. An embodiment having a single motor on a segment is illustrated in FIG. 12 where an individual motor **204** is preferably attached to backbone **202** and is sufficiently small and compact enough so as to present a relatively small diameter which is comfortable and small enough for insertion into a patient without trauma. Motor **204**, which is shown here as being a small brushed DC motor, may be used for actuating adjacent segments **192** and may be controlled independently from other motors. Various motors, aside from small brushed DC motors, may also be used such as AC motors, linear motors, etc. Each motor **204** also preferably contains within the housing not only the electromechanical motor assembly EM itself, but also a gear reduction stage GR, and a position encoder PE. A gear reduction stage GR attached to the motor assembly EM will allow for the use of the motor **204** in its optimal speed and torque range by changing high-speed, low-torque operating conditions into a more useful low-speed, high-torque output. The position encoder PE may be a conventional encoder to allow the controlling computer to read the position of the segment's joint **194** by keeping track of the angular rotational movement of the output shaft of the motor **204**.

Each motor **204** has a rotatable shaft which extends from an end of the motor **204** to provide for the transmission of power to actuate the segments **192**. Upon this shaft, a spool **206** may be rotatably attached with a first end of the cable **208** further wound about the spool **206**. The cable **208** may then be routed from spool **206** through a channel **212** which is defined in the cable guide **210** and out through opening **214** (as seen in greater detail in FIGS. 13A-13B) to cable anchor **216**, to which the second end of the cable **208** is preferably attached, e.g., by crimping and/or soldering. The cable guide **210** serves to capture the cable **208** that is wound about the spool **206**. The cable anchor **216** is attached across a universal joint pivot **220** to an adjacent segment **192** via a pin **218** and may be shaped like a conventional electronic ring connector having a round section defining a hole therethrough for mounting to the segment **192** and an extension protruding from the anchor **216** for attaching the second end of the cable **208**. Cable **208** may comprise a wide variety of filaments, strands, wires, chains, braids, etc. any of which may be made of a wide variety of biocompatible materials, e.g., metals such as stainless steel, polymers such as plastics and Nylon, etc.

In operation, when the motor **204** is operated to spin the shaft in a first direction, e.g., clockwise, the spool **206** rotates accordingly and the cable **208** pulls in a corresponding direction on the adjacent segment **192** and transmits the torque to subsequently actuate it along a first axis. When the motor **204** is operated to spin the shaft in a second direction opposite to the first, e.g., counter-clockwise, the spool **206** again rotates accordingly and the cable **208** would then pull in the corresponding opposing direction on the adjacent segment **192** to subsequently transmit the torque and actuate it in the opposite direction.

FIGS. 13A and 13B show exploded isometric assembly views of two adjacent segments and an individual segment, respectively, from the embodiment shown in FIG. 12. As seen in FIG. 13A, backbone **202** is seen with the lumen **221**, which may be used to provide a working channel, as described above. Also seen are channel **212** defined in cable guide **210** as well as opening **214** for the cable **208** to run through. In interconnecting adjacent segments and to provide the requisite degree-of-freedom between segments, a preferable method of joining involves using the universal joint pivot **220**. However, other embodiments, rather than using a universal joint pivot **220**, may use a variety of joining methods, e.g., a flexible tube used to join two segments at their respective

centers, a series of single degree-of-freedom joints that may be closely spaced, etc. This particular embodiment describes the use of the universal joint pivot **220**. At the ends of backbone **202** adjacent to other segments, a pair of universal yoke members **224** may be formed with a pair of corresponding pin openings **226**. As the universal joint pivot **220** is connected to a first pair of yoke members **224** on one segment, a corresponding pair of yoke members **224** from the adjacent segment may also be attached to the joint pivot **220**.

As seen further in FIG. 13B, the universal joint pivot **220** is shown in this embodiment as a cylindrical ring having two sets of opposing receiving holes **228** for pivotally receiving corresponding yoke members **224**. The receiving holes **228** are shown as being spaced apart at 90.degree. intervals, however, in other variations, receiving holes may be spaced apart at other angles depending upon the desired degree-of-freedom and application. Also seen is an exploded assembly of spool **206** removed from motor **204** exposing drive shaft **205**. With motor **204** displaced from backbone **202**, the groove **230** is revealed as formed in the backbone **202**. This groove **230** may be depressed in backbone **202** to preferably match the radius of the motor **204** housing not only to help locate the motor **204** adjacent to backbone **202**, but also to help in reducing the overall diameter of the assembled segment. The motor **204** may be attached to the backbone **202** by various methods, e.g., adhesives, clamps, bands, mechanical fasteners, etc. A notched portion **232** may also be formed in the cable guide **210** as shown to help in further reducing segment diameter.

Prior to insertion into a patient, the endoscope **200** may optionally be configured to have a diagnostic check performed automatically. When the endoscope **200** is wound onto a drum, adjacent segments **192** will have a predetermined angle relative to one another, as determined initially by the diameter of the drum and the initial configuration of the storage unit in which the endoscope **200** may be positioned. During a diagnostic check before insertion, a computer may be configured to automatically sense or measure the angles between each adjacent segments **192**. If any of the adjacent segments **192** indicate a relative measured angle out of a predetermined acceptable range of angles, this may indicate a segment **192** being out of position and may indicate a potential point of problems during endoscope **200** use. Accordingly, the computer may subsequently sound an audible or visual alarm and may also place each of the segments **192** into a neutral position to automatically prevent further use or to prevent any trauma to the patient.

FIG. 14 shows a variation of the tendon driven endoscope **20** of the present invention. The endoscope **20** has an elongate body **21** with a manually or selectively steerable distal portion **24**, an automatically controlled portion **28**, and a flexible and passively manipulated proximal portion **22**, which may be optionally omitted from the device. The steerable distal portion **24** can be articulated by hand or with mechanical assistance from actuators. The automatically controlled portion **28** is segmented, and each segment is capable of bending through a full range of steerable motion. The distal portion **24** is also a controllable segment.

The selectively steerable distal portion **24** can be selectively steered or bent up to, e.g., a full 180.degree. bend in any direction **26**, as shown. A fiberoptic imaging bundle **40** and one or more illumination fibers **42** may extend through the body **21** from the proximal portion **22** to the distal portion **24**. Alternatively, the endoscope **20** may be configured as a video endoscope with a miniaturized video camera, such as a CCD or CMOS camera, positioned at the distal portion **24** of the endoscope body **21**. The images from the video camera can be

transmitted to a video monitor by a transmission cable or by wireless transmission where images may be viewed in real-time and/or recorded by a recording device onto analog recording medium, e.g., magnetic tape, or digital recording medium, e.g., compact disc, digital tape, etc. LEDs or other light sources could also be used for illumination at the distal tip of the endoscope.

The body **21** of the endoscope **20** may also include one or more access lumens **38** that may optionally be used for illumination fibers for providing a light source, insufflation or irrigation, air and water channels, and vacuum channels. Generally, the body **21** of the endoscope **20** is highly flexible so that it is able to bend around small diameter curves without buckling or kinking while maintaining the various channels intact. When configured for use as a colonoscope, the body **21** of the endoscope **20** may range typically from 135 to 185 cm in length and about 13-19 mm in diameter. The endoscope **20** can be made in a variety of other sizes and configurations for other medical and industrial applications.

The controllable portion **28** is composed of at least one segment **30**, and preferably several segments **30**, which are controllable via a computer and/or electronic controller (controller) **45** located at a distance from the endoscope **20**. Each of the segments **30** has tendons mechanically connected to actuators to allow for the controlled motion of the segments **30** in space. The actuators driving the tendons may include a variety of different types of mechanisms capable of applying a force to a tendon, e.g., electromechanical motors, pneumatic and hydraulic cylinders, pneumatic and hydraulic motors, solenoids, shape memory alloy wires, electronic rotary actuators or other devices or methods as known in the art. If shape memory alloy wires are used, they are preferably configured into several wire bundles attached at a proximal end of each of the tendons within the controller. Segment articulation may be accomplished by applying energy, e.g., electrical current, heat, etc., to each of the bundles to actuate a linear motion in the wire bundles which in turn actuate the tendon movement. The linear translation of the actuators within the controller may be configured to move over a relatively short distance, e.g., within a few inches or less such as ± 1 inch, to accomplish effective articulation depending upon the desired degree of segment movement and articulation.

It is preferable that the length of the insertable portion of the endoscope comprises controllable segments **30**, although a passive proximal portion **22** can also be used. This proximal portion **22** is preferably a flexible tubing member that may conform to an infinite variety of shapes, and may be made from a variety of materials such as thermoset and thermoplastic polymers which are used for fabricating the tubing of conventional endoscopes.

Each segment **30** preferably defines at least one lumen running throughout to provide an access channel through which wires, optical fibers, air and/or water channels, various endoscopic tools, or any variety of devices and wires may be routed. A polymeric covering, or sheath, **39** may also extend over the body of the endoscope **21** including the controllable portion **28** and steerable distal portion **24**. This sheath **39** can preferably provide a smooth transition between the controllable segments **30**, the steerable distal portion **24**, and the flexible tubing of proximal portion **22**.

A handle **32** may be attached to the proximal end of the endoscope. The handle **32** may include an ocular connected to the fiberoptic imaging bundle **42** for direct viewing. The handle **32** may otherwise have a connector **54** for connection to a video monitor, camera, e.g., a CCD or CMOS camera, or a recording device **52**. The handle **32** may be connected to an

illumination source **43** by an illumination cable **44** that is connected to or continuous with the illumination fibers **42**. Alternatively, some or all of these connections could be made at the controller **45**. Luer lock fittings **34** may be located on the handle **32** and connected to the various instrument channels.

The handle **32** may be connected to a motion controller **45** by way of a controller cable **46**. A steering controller **47** may be connected to the motion controller **45** by way of a second cable **48** or it may optionally be connected directly to the handle **32**. Alternatively, the handle may have the steering control mechanism integrated directly into the handle, e.g., in the form of a joystick, conventional disk controllers such as dials, pulleys or wheels, etc. The steering controller **47** allows the user to selectively steer or bend the selectively steerable distal portion **24** of the body **21** in the desired direction **26**. The steering controller **47** may be a joystick controller as shown, or other steering control mechanism, e.g., dual dials or rotary knobs as in conventional endoscopes, track balls, touchpads, mouse, or sensory gloves. The motion controller **45** controls the movement of the segmented automatically controlled proximal portion **28** of the body **21**. This controller **45** may be implemented using a motion control program running on a microcomputer or using an application-specific motion controller. Alternatively, the controller **45** may be implemented using, e.g., a neural network controller.

The actuators applying force to the tendons may be included in the motion controller unit **45**, as shown, or may be located separately and connected by a control cable. The tendons controlling the steerable distal portion **24** and the controllable segments **30** extend down the length of the endoscope body **21** and connect to the actuators. FIG. **14** shows a variation in which the tendons pass through the handle **32** and connect directly to the motion controller **45** via a quick-release connector **60**. In this variation, the tendons are part of the control cable **46**, although they could independently connect to the actuators, so long as the actuators are in communication with the controller **45**.

An axial motion transducer (also called a depth referencing device or datum) **49** may be provided for measuring the axial motion, i.e., the depth change, of the endoscope body **21** as it is advanced and withdrawn. The depth referencing device **49** can be made in many possible configurations. For example, the axial motion transducer **49** in FIG. **14** is configured as a ring **49** that may surround the body **21** of the endoscope **20**. The axial motion transducer **49** is preferably attached to a fixed point of reference, such as the surgical table or the insertion point for the endoscope **20** on the patient's body. As the body **21** of the endoscope **20** slides through the axial motion transducer **49**, it indicates the axial position of the endoscope body **21** with respect to the fixed point of reference and sends a signal to the electronic controller **45** by telemetry or by a cable. The axial motion transducer **49** may use optical, electronic, magnetic, radio frequency or mechanical methods to measure the axial position of the endoscope body **21**.

When the endoscope body **21** is advanced or withdrawn, the axial motion transducer **49** detects the change in position and signals the motion controller **45**. The controller can use this information to propagate the selected curves proximally or distally along the controllable portion **28** of the endoscope body **21** to keep the endoscope actively following the pathway selected by the user steering the distal portion **24**. The axial motion transducer **49** also allows for the incrementing of a current depth within the colon C by the measured change in depth. This allows the endoscope body **21** to be guided through tortuous curves without putting unnecessary force on the wall of the colon C.

FIG. 15A shows an example of the resulting segment articulation which may be possible through the use of two or three tendons to articulate the controllable segments, including the steerable distal section. FIG. 15A shows one example of a possible range of motion of a controllable segment of the present invention actuated, in this example, by three tendons. A segment in the relaxed, upright position **301** can be bent in virtually any direction relative to the x-y plane. The figure, as an illustrative example, shows a segment **302** that has been bent down and at an angle relative to its original position **301**. The angles α and β describe the bend assumed by the segment. Angle β gives the angle in the x-y plane, while α is the angle describing the motion in the x-z plane. In one variation, the controllable segments of the endoscope can bend through all 360° in the β angle and up to 90° in the α angle. An angle a greater than 90° would result in looping of the endoscope. In FIG. 15A, the segment is shown bent approximately 45° along angle α . The freedom of movement of a segment is, in part, determined by the articulation method, the size of the segment, the materials from which it is constructed, and the manner in which it is constructed, among others. Some of these factors are discussed herein.

The steerable distal portion, as well as the endoscope and the controllable segments are bendable but preferably not compressible or expansible. Thus, in FIG. 15A, the centerline **304** of the relaxed segment **301** is approximately the same length as the centerline **306** of the segment after bending **302**.

FIGS. 15B to 15F show the use of three tendons to actuate a controllable segment used in an endoscope of the present invention. The tendons shown in this example are all Bowden type cables **310** that have an internal cable **312** coaxially surrounded by a housing or sleeve **314** in which the cable is free to move. Bowden cables can be used to apply either tensile or compressive forces, i.e., they may be pushed or pulled, to articulate the endoscope and can be actuated remotely to deliver forces as desired at locations along the endoscope. Force from a tendon is exerted across or through the segment by attaching the tendon cable at the distal end of the segment **320** and the tendon housing **314** at the proximal end of the segment **322**. FIG. 15B shows a view of the top of the segment with three attachment sites for the tendon cables indicated **320**.

In one variation, three tendons are used to actuate each segment, including the steerable distal portion, although four or more tendons could be used. Three tendons can reliably articulate a segment in any direction without having to rotate the segment or endoscope about its longitudinal axis. The three cable tendons **312** are preferably attached at the distal end of the segment **320** close to the segment's edge, spaced equally apart. In FIG. 15B, tendons are attached at the two o'clock, six o'clock and ten o'clock positions. It is desirable to use fewer tendons, because of space concerns, since the tendons controlling each segment project proximally to the actuators. Thus, two tendons could be used to control a segment. It may also be desirable to include one or more biasing element, e.g., a spring, to assist in articulating a segment in three dimensions. In another variation, two tendons may be used to articulate a segment in three dimensional space by controlling motion in two directions while rotating the segment about its longitudinal axis.

FIG. 15C shows a relaxed segment with three tendons attached. The tendon sleeves **314** are shown attached to the proximal end of the segment **322** directly below the corresponding cable attachment sites. FIGS. 15D to 15F show this segment bent by each of the controlling tendons **310** separately.

As shown in FIG. 15D, applying tension by pulling on the first tendon **330** results in a bending in the direction of the first tendon **330**. That is, looking down on the top of the unbent segment (as in FIG. 15B), if the first tendon is attached at the six o'clock position, then pulling on just this tendon results in bending the segment towards the six o'clock position. Likewise, in FIG. 15E, putting tension only on a second tendon **332** attached at the two o'clock position results in bending the segment towards the two o'clock direction. Finally, pulling on the tendon in the ten o'clock position **334** bends the segment towards the ten o'clock direction. In all cases, the bending is continuous; the greater the tension applied, the further the bending (the α angle, in the x-z plane of FIG. 15A). A segment can be bent in any direction by pulling on individual tendons or a combination of two tendons. Thus, to bend the segment in the twelve o'clock direction, both the second **332** and the third **334** tendon could be pulled with equal force. Alternatively, first tendon **330** in the six o'clock position may be pushed either alone or in combination with second **332** and third tendons **334** being pulled to result in the same configuration.

FIGS. 16A and 16B show a variation in which a segment is articulated by two tendons and one biasing element. FIG. 16A shows a planar top view of the segment. The attachment sites for the biasing element **340** and the two tendons **320** are spaced around the perimeter of the distal end of the segment as shown. The tendons **320** may be attached at the two o'clock and ten o'clock positions, looking down on the top of the section, and the biasing element **340** is attached at the six o'clock position. FIG. 16B shows a perspective view of the segment in the unbent configuration. In this variation, the biasing element is configured to apply tension to the side of the segment such that it will bend towards the six o'clock position. The biasing element can be any element that can apply compressive or tensile forces across the segment, e.g., a spring, elastic element, a piston, etc. The segment is held in the neutral or unbent position shown in FIG. 16B by applying tension from both tendons **312**. Controlling the amount of tension applied by the tendons results in bending of the segment in three dimensional space. More than one biasing element could also be used with two or more tendons. For example, a biasing element could be located opposite each tendon.

Alternatively, if the tendon is a push-pull cable, and each tendon can apply compression as well as tension, then two tendons can control the motion of segment without any biasing element at all.

More than three tendons can also be used to control the bending of a segment. FIG. 16C shows a top planar view of a segment that is controlled by four tendons attached in the eleven o'clock, two o'clock, five o'clock and eight o'clock positions. As with the three-tendon embodiment, tension applied on one or a combination of the tendons results in shortening the side of the segment. Thus, if tension is applied only on the tendon attached distally at the eleven o'clock position **355**, the corresponding side of the tendon will shorten, and the segment will bend in the eleven o'clock direction.

In all these variations, the circumferential locations of the tendons and/or biasing elements are illustrative and are not intended to be limited to the examples described herein. Rather, they may be varied according to the desired effects as understood by one of skill in the art.

FIG. 17 shows a partial schematic representation of a single tendon bending a segment. For clarity, the other parts of a complete endoscope, including other tendons and segments, have been omitted from FIG. 17. Tension applied to a

tendon cable is transferred across the entire segment, resulting in bending. By using a Bowden cable **310** whose sleeve **314** is attached to the base **322** of the segment and also fixed at the proximal actuator end **403**, only the intended segment **401** is bent by applying tension to the tendon **312**, and more proximal segments are unaffected. The tendon is placed in tension by the actuator **410**, which is shown, in this variation, as a motor pulling on the tendon cable **312**.

Linked control rings may provide the flexible structure needed to construct the steerable distal portion and the controllable segments. Two examples of the types of control rings that may be utilized are shown. The first is shown in FIG. **18A** which shows a vertebra-type control ring that forms the controllable segments of the present invention. FIG. **18A** shows an end view of a single vertebra. Each ring-shaped vertebra **501** can define a central channel or aperture **504** or apertures that can collectively form the internal lumen of the device as previously described. The vertebrae may have two pairs of hinges; the first pair **506** projecting perpendicularly from a first face of the vertebra and a second pair **508**, located 90° around the circumference from the first pair, projecting perpendicularly away from the face of the vertebra on a second face of the vertebra opposite to the first face. The hinges shown in FIGS. **18A** and **18B** are tab-shaped, however other shapes may also be used.

The vertebra control ring in FIG. **18A** is shown with three holes **510** through the edge of the vertebra that may act, e.g., as attachment sites for the tendon cable **312** if the vertebra is the most distal vertebra in a segment, or as a throughway for a tendon cable that can actuate the segment in which the vertebra is used. These holes **510** can also be used to attach the sleeve of the Bowden-type tendon cable **314** when the vertebra is the most proximal control disk in a segment. Alternatively, rather than a hole **510**, the attachment sites could be a recess or other specialized shape. Although FIG. **18A** shows three holes **510**, the number of holes may depend upon the number of tendons used to control the segment to which the vertebra belongs. Since the holes **510** may be used as attachment sites for the tendons, there are as many holes as there are tendons controlling the segment.

The outer edge of the vertebra in FIG. **18A** may be scalloped to provide spaces **512** for tendon housings of tendons that control more distal segments and bypass the vertebra. These tendon bypass spaces preferably conform to the outer diameter of the tendons used. The number of tendon bypass spaces **512** may vary depending on the number of tendons. Also, the orientation of the tendon bypass spaces may be varied if it is desirable to vary the way in which the bypassing tendons are wound around the endoscope. For example, the spaces **512** in FIG. **18C** are oriented at an angle relative to the longitudinal axis of the vertebra, allowing the tendons to wind around the body of the endoscope as they project proximally. Furthermore, the tendon bypass spaces could be lubricated or composed of a lubricious material in order to facilitate free movement of the bypassing tendons across the segment, and prevent interference between the bending of the segment and the bypassing tendons.

FIGS. **18B** and **18C** show side views of the same vertebra as FIG. **18A**. The two pairs of hinge joints **508**, **506** are shown. Hinge joints **508**, **506** are preferably located 90° apart and extend axially so that the hinge joints can pivotally mate with hinge joints from adjacent vertebrae. This mating **520** with adjacent vertebrae is more clearly seen in FIG. **18C**. These hinges can be joined, pinned, or connected through the holes **525** as shown **522**. Alternatively, hinges may also be made from materials utilizing, e.g., thermoplastics, shape memory alloys, etc. Once hinged, each vertebra can rotate

relative to an adjoining vertebra in one axis. However, because vertebrae are hinged to each other in directions alternating by 90°, an assembly of multiple vertebrae is able to move in virtually any direction. The greater the number of vertebrae joined in this manner, the greater the range of motion. In one embodiment, two to ten vertebrae are used to comprise one segment, achieving a length of around 4 cm to 10 cm per segment. The dimensions of both the vertebrae and the hinge joints can be varied, e.g., longer hinge joints will have a greater bending radius when joined to another vertebra. Furthermore, the number of vertebrae per segment can vary, e.g. more than ten vertebrae could be used.

FIGS. **18D** and **18E** show another variation of a vertebra in sectional and perspective views, respectively. In FIGS. **18D** and **18E**, the tendons that bypass the segment may be contained within the body of the vertebra in a tendon bypassing space **550** rather than along the outer edge of the vertebra as shown in FIG. **18A**. The vertebra of FIGS. **18D** and **18E** show four tendon bypassing spaces **550**, and each space can hold approximately fifteen bypassing tendon sleeves. The number, shape and sizes of the tendon bypassing spaces can be varied. For example, a vertebra could have two tendon bypassing spaces that could hold more than thirty-five tendon sleeves. Moreover, the tendon bypassing space could also be located on the inside of the central aperture or lumen of the vertebra **504**.

Although FIG. **18D** shows tendon sleeves holding only a single tendon cable **560**, more than one tendon cable could be contained in a tendon housing or sleeve. For example, if three tendons articulate a segment, all three tendons could be contained in a single tendon housing. Such a combined tendon housing could further utilize lubrication to accommodate independent movement by individual tendon cables and/or could be divided into compartments that isolate the tendons within the housing.

FIG. **18E** also shows a perspective view of the hinge joints **506**, **508** that can pivotally mate with pairs of hinge joints from adjacent vertebrae. Although FIGS. **18A** and **18B** shows two pairs of hinge joints projecting axially, a single hinge joint on each face of the vertebra could also be used. Moreover, as long as the hinge joints can pivotally mate with adjacent vertebrae, the hinge joints can be located at different radial locations from the center of the vertebra. For example, the pairs of hinge joints shown in FIGS. **18A** to **18C** are located closer to the center of the vertebra than the hinge joints in FIGS. **18D** and **18E**.

FIG. **19A** and **19B** illustrate a second variation of control ring. The variation shown in the figure utilizes a flexible backbone **601** preferably made of a material that is relatively non-compressible and non-extensible, to which control rings **602** are attached at intervals. This structure allows bending in a continuous curve in any desired direction. FIG. **19A** shows a side view of one controllable segment of this variation with the outer layers removed to show the control rings and backbone. Multiple control rings **602** may be attached to the flexible backbone at regular intervals. Fewer or more control rings could be used to comprise a single segment depending upon the desired degree of articulation. The tendon cable **312** attaches to the most distal control ring of the segment **604**. As with the vertebra-type variation, this central backbone embodiment is shown actuated by three tendons **310** attached at sites equally spaced around the edge of the most distal control ring of the segment **604**. The tendon cables controlling the segment **312** pass through spaces or holes **610** defined in the control rings **602** through which they are free to move. These holes **610** could be lubricated, lined with a lubricious material or the control rings **602** may be composed of some

lubricious material to facilitate cable motion through the holes **610**. The tendon sleeve preferably attaches at a location **614** to the most proximal control ring in the segment **612**. When a tendon **312** is placed under tension, this force is distributed along the entire segment. Because the inner tendon cable **312** is freely slidable within the tendon sleeve **314**, and the tendon sleeve is fixed at both ends of the tendon **614**, pulling on the tendon cable causes bending only in the selected segment.

FIG. **19A** also shows the first control ring of a more proximal segment **604**. The tendons controlling the more distal segment may pass over the outside of the more proximal segments as they project proximally to the actuators. The outer edge of the control rings for the flexible backbone embodiment are shown with channels or tendon bypassing spaces **616** for bypassing tendons, as seen in FIG. **19B**. As with the vertebra-type control rings, these tendon bypassing spaces could also be located within the control ring, for example, in an enclosed tendon bypassing space.

FIG. **19B** shows an end view of control ring **602** which may be used with the flexible backbone embodiment of the endoscope. The center of the control ring contains a channel through which the flexible backbone **601** can be attached. A number of additional channels through the control ring **618** are also shown. These channels can be aligned with channels in neighboring control rings to form an internal lumen or channel for a fiber optic imaging bundle, illumination fibers, etc. as discussed above. Moreover, adjacent control rings may be spaced adjacently to one another at uniform or various distances depending upon the desired degree of bending or control. FIG. **19B** shows three equally spaced holes **610** through which the tendon cable can pass; these holes **610** could also be used as attachment sites for the tendon cable, e.g., when the control ring is the most distal control ring in the segment **604**, or for the tendon cable sleeve, e.g. when the control ring is the most proximal control ring in the segment **612**. These holes **610** could be shaped specifically to receive either the tendon end or the tendon sleeve. Control rings of other designs could be used for different regions of the segment, or for different segments.

FIGS. **20A** to **20C** illustrate a variation of the tendon driven endoscope navigating a tortuous path. The path **701** is shown in FIG. **20A**. This pathway may represent a portion of colon, for example. In FIG. **20A**, the distal tip of the device **704** approaches the designated bend. FIG. **20B** shows the distal tip being steered **705** to assume the appropriate curve. This steering could be performed manually by the user, e.g. a doctor, or automatically using an automatic detection method that could determine the proximity of the walls of the pathway. As described, the bending of the steerable tip is performed by placing tension on the tendon, or combination of tendons that results in the appropriate bending.

The device is then advanced again in FIG. **20C**; as it is advanced, the selected curve is propagated down the proximal length of the endoscope, so that the bend of the endoscope remains in relatively the same position with respect to the pathway **701**. This prevents excessive contact with the walls, and allows the endoscope to move more easily along the tortuous pathway **701**. The endoscope is in continuous communication with the motion controller, and the motion controller can monitor the location of the endoscope within the pathway, e.g., depth of insertion, as well as the selected bends or curves that define the pathway of the endoscope. Depth can be determined by, e.g., the axial motion transducer **49** previously described, or by more direct measurement techniques. Likewise, the shape of each segment could be determined by the tension applied to the tendons, or by direct measurement,

such as direct measurement of displacement of the tendon cables. The motion controller can propagate the selected shape of a segment at a specified location, or depth, within the body, e.g., by setting the lengths of the sides of more proximal segments equal to the corresponding lengths of the sides of more distal segments as the device is moved distally. The controller can also use this information to automatically steer the body of the endoscope, or for other purposes, e.g. creating a virtual map of the endoscope pathway for analytic use.

In addition to measuring tendon displacement, the motion controller can also adjust for tendon stretch or compression. For example, the motion controller can control the "slack" in the tendons, particularly in tendons that are not actively under tension or compression. Allowing slack in inactive tendons reduces the amount of force that is required to articulate more proximal segments. In one variation, the umbilicus at the distal end of the endoscope may contain space to allow slack in individual tendons.

The bending and advancing process can be done in a stepwise or continuous manner. If stepwise, e.g., as the tendon is advanced by a segment length, the next proximal segment **706** is bent to the same shape as the previous segment or distal steerable portion. A more continuous process could also result by bending the segment incrementally as the tendon is advanced. This could be accomplished by the computer control, for example when the segments are smaller than the navigated curve.

Controllable segments, including the steerable distal portion, can be selected to have different dimensions, e.g., different diameters or lengths, even within the same endoscope. Segments of different dimensions may be desirable because of considerations of space, flexibility and method of bending. For example, the more segments in an endoscope, the further it can be steered within a body cavity; however, more segments require more tendons to control the segments. FIGS. **21** and **22** illustrate two variations on tendon driven endoscopes.

FIG. **21** shows a tendon driven endoscope variation that has segments **800** of differing diameters. More distal segments may have a smaller diameter **803** than more proximal segments, e.g., **802**, **801**. The diameter of a typical endoscope could decrease from, e.g., 20 mm, down to, e.g., 12.5 mm. The endoscope shown in FIG. **21** appears telescoped, as the diameter decreases distally in a stepwise manner. This design would be responsive, e.g., to internal body structures that become increasingly narrow. This design would also help accommodate bypassing tendons from more distal segments as they proceed towards the proximal actuators because of the larger diameter of the more proximal segments. FIG. **21** shows four differently sized segments; however, virtually any number of differently sized segments could be used. Moreover, although the segments appear stepped in this variation, the outer surface may be gently tapered to present a smooth outer surface decreasing in diameter towards the distal end.

FIG. **22** shows another variation of the tendon driven endoscope that has segments of different lengths. Using segments of different lengths may require fewer overall segments **900** to construct an equivalent length of articulatable endoscope. As shown in FIG. **22**, more proximal segments **901** are increasingly longer than more distal, e.g., **902**, **903**, segments. For example, segment length could be decreased from 20 cm at a proximal segment down to 6 cm at a distal most segment. The lengths may be decreased incrementally segment to segment by a constant factor; alternatively, lengths may be decreased geometrically, exponentially, or arbitrarily depending upon the desired articulation. In practice this results in an "averaging" of curves by more distal segments as bends and turns are propagated proximally. In order to

accomplish this, the motion controller may be configured to accommodate the differently sized segments accordingly. Alternatively, endoscopes could be comprised of a combination of segments of different length and thickness, depending upon the application.

The tendons that articulate the segments are in mechanical communication with the actuators. However, it may be desirable to have the insertable distal portion of the endoscope be removable from the actuators and controller, e.g., for cleaning or disinfecting. A quick-release mechanism between the proximal end of the endoscope and the actuators is an efficient way to achieve an endoscope that is easily removable, replaceable or interchangeable. For example, the proximal ends of the tendons can be organized to allow predictable attachment to corresponding actuators. The tendons may be organized into a bundle, array, or rack. This organization could also provide other advantages to the endoscope, such as allowing active or passive control of the tendon slack. Furthermore, the proximal ends of each tendon can be modified to allow attachment and manipulation, e.g., the ends of the tendons may be held in a specially configured sheath or casing.

While the present invention has been described herein with respect to the exemplary embodiments and the best mode for practicing the invention, it will be apparent to one of ordinary skill in the art that many modifications, improvements and subcombinations of the various embodiments, adaptations and variations can be made to the invention without departing from the spirit and scope thereof.

What is claimed is:

1. An endoscopic device for approximating tissue within a hollow body organ, comprising:

an elongated body having a plurality of articulatable segments and a steerable distal portion, wherein each of the segments are configurable to assume a selected shape along an arbitrary path when the elongated body is advanced distally or proximally;

a first tissue approximation component positioned about the elongated body, wherein the first tissue approximation component is configured to radially expand into contact with a first region of tissue and releasably grip the first region of tissue via a plurality of tissue gripping regions circumferentially located about the first tissue approximation component; and

a second tissue approximation component positioned about the elongated body proximally of the first tissue approximation component, wherein the second tissue approximation component is configured to radially expand into contact with a second region of tissue and releasably grip the second region of tissue via a plurality of tissue gripping regions circumferentially located about the second tissue approximation component, wherein the first tissue approximation component and the second tissue approximation component are configured to approximate and securely fasten the first region of tissue to the second region of tissue.

2. The endoscopic device of claim 1 wherein the first and the second tissue approximation components each comprise a radially expandable ring.

3. The endoscopic device of claim 1 wherein the first and the second tissue approximation components each comprise a radially expandable balloon.

4. The endoscopic device of claim 1 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise vacuum ports.

5. The endoscopic device of claim 1 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise retractable fasteners.

6. The endoscopic device of claim 5 wherein the retractable fasteners are selected from the group consisting of needles, hooks, and barbs.

7. The endoscopic device of claim 1 wherein the first tissue approximation component is adapted to slide longitudinally towards the second tissue approximation component along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region of tissue is adjacent to the second region of tissue.

8. The endoscopic device of claim 1 wherein the second tissue approximation component is adapted to slide longitudinally towards the first tissue approximation component along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region of tissue is adjacent to the second region of tissue.

9. The endoscopic device of claim 1 wherein the first and the second tissue approximation components are each adapted to slide longitudinally towards one another along at least a portion of the elongated body within rails or grooves defined along the elongated body such that the first region of tissue is adjacent to the second region of tissue.

10. The endoscopic device of claim 1 wherein the first tissue approximation component or the second tissue approximation component contains a plurality of fasteners configured to fasten the first region of tissue to the second region of tissue.

11. The endoscopic device of claim 10 wherein the fasteners are selected from one of staples, clips, screws, adhesives, sutures, and combinations thereof.

12. The endoscopic device of claim 1 wherein the first tissue approximation component and the second tissue approximation component are configured to radially contract away from the first region of tissue and the second region of tissue respectively.

13. An endoscopic device for approximating tissue within a hollow body organ, comprising:

an elongated body having a plurality of articulatable segments and a steerable distal portion, wherein each of the segments are configurable to assume a selected shape along an arbitrary path when the elongated body is advanced distally or proximally;

a first tissue approximation component positioned about the elongated body, wherein the first tissue approximation component is configured to releasably grip a first region of tissue via a plurality of tissue gripping regions circumferentially located about the first tissue approximation component; and

a second tissue approximation component positioned about the elongated body proximally of the first tissue approximation component, wherein the second tissue approximation component is configured to releasably grip a second region of tissue via a plurality of tissue gripping regions circumferentially located about the second tissue approximation component,

wherein the first tissue approximation component and the second tissue approximation component are configured to approximate and securely fasten the first region of tissue to the second region of tissue and radially contract away from the first region of tissue and the second region of tissue respectively.

14. The endoscopic device of claim 13 wherein the first and the second tissue approximation components each comprise a radially contractible ring.

15. The endoscopic device of claim 13 wherein the first and the second tissue approximation components each comprise a radially contractible balloon.

16. The endoscopic device of claim 13 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise vacuum ports.

17. The endoscopic device of claim 13 wherein the plurality of tissue gripping regions on each of the first and the second tissue approximation components comprise retractable fasteners.

18. The endoscopic device of claim 13 wherein the first tissue approximation component or the second tissue approximation component contains a plurality of fasteners configured to fasten the first region of tissue to the second region of tissue.

* * * * *

专利名称(译)	用于内窥镜结肠切除术的装置和方法		
公开(公告)号	US8696694	公开(公告)日	2014-04-15
申请号	US13/729602	申请日	2012-12-28
[标]申请(专利权)人(译)	直观外科手术操作公司		
当前申请(专利权)人(译)	Intuitive Surgical公司运营, INC.		
[标]发明人	BELSON AMIR		
发明人	BELSON, AMIR		
IPC分类号	A61B1/00 A61B17/115 A61B17/00 A61B1/31 A61B17/32 A61B17/22 A61B A61B17/11 A61B17/08		
CPC分类号	A61B1/00147 A61B17/1114 A61B2019/5259 A61B2017/00557 A61B1/0055 A61B2017/1103 A61B2017/22054 A61B1/0058 A61B2017/22034 A61B1/31 A61B2017/003 A61B2034/2059 A61B17/00234 A61B17/1155 A61B2017/00296 A61B2017/00314 A61B2017/00349 A61B2017/00353 A61B2017/1132		
优先权	60/347674 2002-01-09 US		
其他公开文献	US20130116712A1		
外部链接	Espacenet USPTO		

摘要(译)

本文描述了用于内窥镜结肠切除术的装置和方法。具有第一和第二组织接近装置的结肠切除装置安装在彼此分离的结肠镜上。在结肠切除术装置的展开期间,结肠的患病部分位于组织接近装置之间。组织接近装置径向扩张,使得它们在与结肠的疾病部分相邻的两个部位处接触并抓握结肠壁。将病变部分与网膜分离,并使用腹腔镜进行横切,或将其拉入结肠镜中以便以后取出。然后在结肠镜上朝向彼此推动组织接近装置,以使结肠的两个自由边缘接近在一起,在那里它们使用组织接近装置作为外科吻合器固定到彼此,以产生端对端吻合。

