



(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:  
**09.01.2008 Bulletin 2008/02**

(51) Int Cl.:  
**A61B 18/14** (2006.01) **A61B 17/32** (2006.01)  
**A61B 18/00** (2006.01)

(21) Application number: **07012598.4**

(22) Date of filing: **27.06.2007**

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HU IE IS IT LI LT LU LV MC MT NL PL PT RO SE SI SK TR**  
Designated Extension States:  
**AL BA HR MK YU**

- **Miyazawa, Taro**  
**Hachioji-shi, Tokyo 192-8512 (JP)**
- **Okabe, Hiroshi**  
**Hachioji-shi, Tokyo 192-8512 (JP)**
- **Taniguchi, Kazunori**  
**Hachioji-shi, Tokyo 192-8512 (JP)**

(30) Priority: **04.07.2006 JP 2006184663**


(74) Representative: **von Hellfeld, Axel**  
**Wuesthoff & Wuesthoff**  
**Patent- und Rechtsanwälte**  
**Schweigerstrasse 2**  
**81541 München (DE)**

(71) Applicant: **OLYMPUS MEDICAL SYSTEMS CORP.**  
**Shibuya-ku**  
**Tokyo 151-0072 (JP)**

(72) Inventors:  
• **Masuda, Shinya**  
**Hachioji-shi, Tokyo 192-8512 (JP)**

(54) **Surgical instrument**

(57) A surgical instrument can grasp a living tissue (S) by first and second grasping members (25, 59), can cut the grasped tissue by ultrasonic vibration from a grasping surface (61) of an ultrasonic vibrating portion (31) in the second member, and can coagulate the cut portion of the tissue by high-frequency current between first and second electrode portions in the first and second members. A pressing portion (55) is provided in the first member to be in contact with the grasped tissue and presses the tissue in cooperation with the grasping surface of the vibrating portion. Each of the first and second electrode portions includes electrodes in both sides of the pressing portion. The electrodes of the first and second electrode portions cooperate to press the grasped tissue while the tissue is pressed by the pressing portion of the first member and the grasping surface of the vibrating portion.

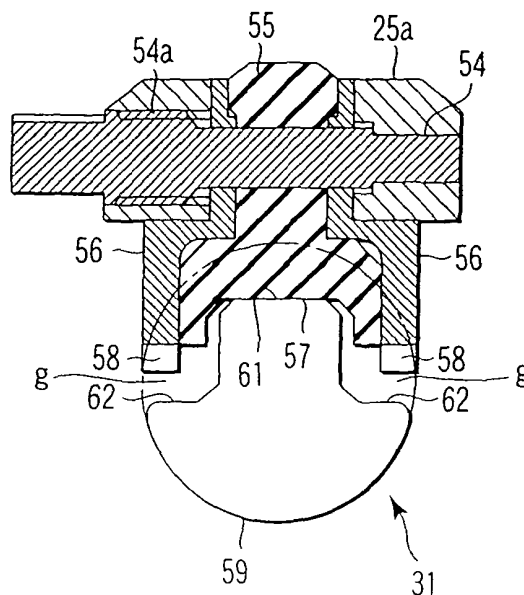

**FIG. 7**

## Description

**[0001]** The present invention relates to a surgical instrument, which grasps a living tissue, and coagulates and cuts the tissue by ultrasonic vibration and high-frequency current.

**[0002]** Each of an ultrasonic instrument using ultrasonic vibration and a high-frequency instrument using a high-frequency current is known as a surgical instrument.

An ultrasonic instrument can coagulate and cut a living tissue by heating the tissue with ultrasonic vibration. A high-frequency instrument can coagulate and cut a living tissue by touching an electrified electrode to the living tissue.

**[0003]** Surgical instruments which can treat a living tissue by using both ultrasonic vibration and high-frequency current are known by Jpn. Pat. Appln. KOKAI Publication Nos. 2003-79633, 2004-12987 and 2004-216180. In each of these surgical instruments, ultrasonic vibration generated by an ultrasonic transducer provided in an operation area is transmitted to a distal end portion of an ultrasonic probe through an ultrasonic vibration transmitting member, and a jaw is provided on the ultrasonic probe to be able to open and close to the probe. The jaw and the probe can grasp a living tissue between them. And, by supplying a high-frequency current from an externally provided high-frequency power supply to the ultrasonic probe, the tissue grasped between the ultrasonic probe and the jaw can be coagulated and cut by the high-frequency current.

**[0004]** The surgical instrument described in the Jpn. Pat. Appln. KOKAI Publication No. 2003-79633 has a round bar-shaped horn for generating ultrasonic vibration, and an open/close cover having an arc-shaped section and an electrode and provided on the horn to open and close thereto. A living tissue is grasped by the horn and cover, and coagulated and cut by the ultrasonic vibration from the horn and high-frequency current from the electrode of the cover. However, in this conventional surgical instrument, there is a problem that the living tissue cannot be grasped (compressed) by a strong force because the living tissue is grasped by the round bar-shaped horn and the arc-shaped sectioned open/close cover.

**[0005]** The surgical instrument described in each of the Jpn. Pat. Appln. KOKAI Publication Nos. 2004-129870 and 2004-216180 has a round bar-shaped horn for generating ultrasonic vibration, and a grasping member having an electrode and provided on the horn to open and close thereto. A living tissue is grasped by the horn and the grasping member, and coagulated and cut by the ultrasonic vibration from the horn and high-frequency current from the electrode of the grasping member. However, also in this conventional surgical instrument, there is a problem that the living tissue cannot be grasped (compressed) by a strong force because the living tissue is grasped by the round bar-shaped horn and the grasping member.

**[0006]** This invention is derived from the above described circumstances, and an object of this invention is to provide a surgical instrument which can coagulate and cut a desired living tissue by ultrasonic vibration and high-frequency current while surely grasping the desired living tissue by strong force, so that the cut portion of the desired living tissue can be surely and strongly sealed and a time needed from grasping the desired living tissue to coagulating, cutting, and sealing thereof can be shortened.

**[0007]** In order to achieve the above described object of this invention, a surgical instrument according to one aspect of the present invention, comprises: a first grasping member and second grasping member to open and close relative to each other; an ultrasonic vibrating portion which is provided in the second grasping member, which is connected to an ultrasonic transducer to generate ultrasonic vibration, and which has a grasping surface to be in contact with a living tissue grasped between the first grasping member and the second grasping member; a first high-frequency electrode portion provided in the first grasping member; and a second high-frequency electrode portion provided in the second grasping member to be independent of the first high-frequency electrode portion, wherein the surgical instrument can cut the living tissue grasped between the first grasping member and the second grasping member by the ultrasonic vibration from the grasping surface of the ultrasonic vibrating portion, and can further coagulate the cut portion of the living tissue by the high-frequency current between the first high-frequency electrode portion and the second high-frequency electrode portion. And, the surgical instrument is characterized in that: a pressing portion is further provided in the first grasping member, the pressing portion being in contact with the living tissue grasped between the first grasping member and the second grasping member, and pressing the living tissue in cooperation with the grasping surface of the ultrasonic vibrating portion; the first high-frequency electrode portion includes at least a pair of electrodes which are arranged in both sides of the pressing portion in the first grasping member; the second high-frequency electrode portion includes at least a pair of electrodes which are arranged in both sides of the pressing portion in the second grasping member to oppose to the electrodes of the first high-frequency electrode portion; and the electrodes of the first high-frequency electrode portion and the electrodes of the second high-frequency electrode portion cooperate with each other in the both sides of the pressing portion to press the living tissue grasped between the first grasping member and the second grasping member while the living tissue is pressed by the pressing portion of the first grasping member and the grasping surface of the ultrasonic vibrating portion.

**[0008]** In order to achieve the above described object of this invention, a surgical instrument according to another aspect of the present invention, comprises: a first grasping member and second grasping member to open

and close relative to each other; an ultrasonic vibrating portion which is provided in the second grasping member, which is connected to an ultrasonic transducer to generate ultrasonic vibration, and which has a grasping surface to be in contact with a living tissue grasped between the first grasping member and the second grasping member; a first high-frequency electrode portion provided in the first grasping member; and a second high-frequency electrode portion provided in the first grasping member to be independent of the first high-frequency electrode portion, wherein the surgical instrument can cut the living tissue grasped between the first grasping member and the second grasping member by the ultrasonic vibration from the grasping surface of the ultrasonic vibrating portion, and can further coagulate the cut portion of the living tissue by the high-frequency current between the first high-frequency electrode portion and the second high-frequency electrode portion. And, the surgical instrument is characterized in that: a pressing portion is further provided in the first grasping member, the pressing portion being in contact with the living tissue grasped between the first grasping member and the second grasping member, and pressing the living tissue in cooperation with the grasping surface of the ultrasonic vibrating portion; the first high-frequency electrode portion includes at least one electrode which is arranged in one side of the pressing portion in the first grasping member; the second high-frequency electrode portion includes at least one electrode which is arranged in the other side of the pressing portion in the first grasping member; and the at least one electrode of the first high-frequency electrode portion and the at least one electrode of the second high-frequency electrode portion cooperate with each other in the both sides of the pressing portion to press the living tissue grasped between the first grasping member and the second grasping member while the living tissue is pressed by the pressing portion of the first grasping member and the grasping surface of the ultrasonic vibrating portion.

**[0009]** Each of the surgical instrument according to one aspect of the present invention and characterized by comprising as described above and the surgical instrument according to another aspect of the present invention and characterized by comprising as described above, can coagulate and cut a desired living tissue by ultrasonic vibration and high-frequency current while surely grasping the desired living tissue by strong force, so that the cut portion of the desired living tissue can be surely and strongly sealed and a time needed from grasping the desired living tissue to coagulating, cutting, and sealing thereof can be shortened.

**[0010]** The invention can be more fully understood from the following detailed description when taken in conjunction with the accompanying drawings, in which:

FIG. 1 is a side view schematically showing the whole of a surgical instrument according to a first embodiment of the invention;

FIG. 2 is a longitudinal sectional view of an operation area of the surgical instrument of FIG. 1;

FIG. 3 is an enlarged sectional view of a distal end portion of the operation area of FIG. 2;

FIG. 4 is a transverse sectional view along a line of IV-IV in FIG. 2;

FIG. 5A is a plan view of a surgical treatment area of the surgical instrument of FIG. 1;

FIG. 5B is a longitudinal sectional view of the surgical treatment area of FIG. 5A;

FIG. 6A is a transverse sectional view along a line of VIA-VIA in FIG. 5B;

FIG. 6B is a transverse sectional view along a line of VIB-VIB in FIG. 5B;

FIG. 6C is a transverse sectional view along a line of VIC-VIC in FIG. 5B;

FIG. 7 is a transverse sectional view showing a state that a first grasping member of FIG. 6C is combined with a second grasping member;

FIG. 8 is a transverse sectional view showing a state that a living tissue is grasped by the first and second grasping members of the surgical treatment area of FIG. 7;

FIG. 9A is a longitudinal sectional view of a surgical treatment area of a surgical instrument according to a second embodiment of the invention;

FIG. 9B is a transverse sectional view along a line of IXB-IXB in FIG. 9A;

FIG. 10A is a longitudinal sectional view of a surgical treatment area of a surgical instrument according to a third embodiment of the invention;

FIG. 10B is a transverse sectional view along a line of XB-XB in FIG. 10A;

FIG. 11A is a longitudinal sectional view of a surgical treatment area of a surgical instrument according to a fourth embodiment of the invention;

FIG. 11B is a transverse sectional view along a line of XIB-XIB in FIG. 11A;

FIG. 12A is a schematic perspective view of a surgical treatment area of a surgical instrument according to a fifth embodiment of the invention;

FIG. 12B is a transverse sectional view showing a state that a living tissue is grasped by first and second grasping members of the surgical treatment area of FIG. 12A;

FIG. 13 is a schematic perspective view of a surgical treatment area of a surgical instrument according to a sixth embodiment of the invention;

FIG. 14A is a schematic perspective view of a surgical treatment area of a surgical instrument according to a seventh embodiment of the invention;

FIG. 14B is a transverse sectional view along a line of XIVB-XIVB in FIG. 14A;

FIG. 15 is a schematic transverse sectional view of a surgical treatment area of a surgical instrument according to an eighth embodiment of the invention;

FIG. 16 is a schematic perspective view of a surgical treatment area of a surgical instrument according to

a ninth embodiment of the invention;

FIG. 17 is a schematic transverse sectional view of a surgical treatment area of a surgical instrument according to a tenth embodiment of the invention;

FIG. 18 is a schematic transverse sectional view of a surgical treatment area of a surgical instrument according to an eleventh embodiment of the invention;

FIG. 19A is a schematic perspective view of a surgical treatment area of an example of a surgical instrument different from the conventional one; and

FIG. 19B is a schematic transverse sectional view along a line of XIXB-XIXB in FIG. 19A.

**[0011]** First, a surgical instrument according to a first embodiment of the present invention will be explained with reference to FIG. 1 to FIG. 8.

**[0012]** As shown in FIG. 1, a surgical instrument 10 has an operation area 11, an insertion area 12 which is attachable to and detachable from the insertion area 11, a transducer unit 13 which is detachably inserted into the insertion area 12 from the proximal end portion of the operation area 11.

**[0013]** The operation area 11 has an operation area main body 14 having a cylindrical casing 14a. The proximal end portion of the operation area main body 14 is provided with a transducer unit connector 15 to which the transducer unit 13 is connected. A fixed handle 16 is integrally provided to the outer circumferential surface of the casing 14a of the operation area main body 14.

**[0014]** A movable handle 18 is provided to the casing 14a of the operation area main body 14 with a pivot 17. A finger insertion hole 16a is formed in the fixed handle 16, and fingers excepting the thumb of one hand of an operator can be selectively inserted into the finger insertion hole 16a. A thumb insertion hole 18a is formed in the movable handle 18, and the thumb of the same hand of the operator can be inserted into the thumb insertion hole 18a. The casing 14a of the operation area main body 14 is further provided with a first electrode pin 19 and a second electrode pin 20, both of which project from the body and can be connected to a high-frequency power supplying device (not shown).

**[0015]** An insertion sheath 22 of the insertion area 12 is detachably connected to the distal end portion of the casing 14a of the operation area main body 14. The insertion sheath 22 includes a tubular member which is made of electrically conductive material and the outer surface of which is covered by an insulating layer 22b, and a holding member 22a which is provided at the distal end portion of the tubular member. The holding member 22a holds a surgical treatment area 23. The surgical treatment area 23 includes a first grasping member 25 which is pivotally supported by a pivot pin 24 to be rotationally movable in a direction crossing the longitudinal center line of the insertion sheath 22.

**[0016]** The transducer unit 13 includes a transducer casing 26 which can be detachably connected to the

transducer unit connecting part 15 of the operation area main body 14. A transducer for generating ultrasonic vibration is housed in the transducer casing 26. A unit connector 27 is provided at the distal end portion of the transducer casing 26. A C-shaped engaging ring 28 which is formed by cutting a part of a ring member is fit on the unit connector 27. The transducer unit 13 further includes a probe 29 as an ultrasonic vibration transmitting member. A fixing screw 30 which is detachably connected to the unit connector 27 is provided at the proximal end portion of the probe 29. The distal end portion of the probe 29 is configured as an ultrasonic vibrating portion 31. An electric cable 32 for generating ultrasonic vibration is extended from the proximal end of the transducer casing 26.

**[0017]** When the transducer casing 26 of the transducer unit 13 is fit into the transducer unit connector 15 of the operation area main body 14, the probe 29 of the transducer unit 13 is inserted into the tubular member of the insertion sheath 22, and the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 is projected forward from the holding member 22a of the insertion sheath 22. The ultrasonic vibrating portion 31 at the distal end portion of the probe 29 projected forward from the holding member 22a of the insertion sheath 22 cooperates with the first grasping member 25 to form the surgical treatment area 23.

**[0018]** Next, the internal structure of the operation area 11 will be explained with reference to FIGS. 2 to 4. FIG. 2 is a longitudinal sectional view of the operation area 11 of the surgical instrument 10 of FIG. 1. FIG. 3 is an enlarged sectional view of the distal end portion of the operation area 11 of FIG. 2. And, FIG. 4 is a transverse sectional view along a line of IV-IV in FIG. 2.

**[0019]** As shown in FIG. 2, the casing 14a of the operation area main body 14 is made of insulating material such as synthetic resin, and is provided with a second electrode mounting portion 33 on which the second electrode pin 20 is mounted. The second electrode pin 20 includes an intermediate portion, a projecting portion, and an internal connecting portion 20b. The intermediate portion is covered by an insulating cover 34. The projecting portion projects from the second electrode mounting portion 33 and is configured as an external connector 20a to which a plug (not shown) is connected. And, the internal connecting portion 20b is buried in the second electrode mounting portion 33 and is electrically connected to an internal ring-shaped connection terminal 35 of the casing 14a.

**[0020]** A female screw 36 is provided at the proximal end portion of the inner surface of the casing 14a, and the connection terminal 35 and a fixing ring 37 are fixed to the female screw 36. An electrically conductive cylinder 38 is provided in the inner space of the casing 14a such that the conductive cylinder 38 is encircled with and coaxial to the ring-shaped connection terminal 35, and the conductive cylinder 38 is electrically connected to the terminal 35. A ring-shaped probe holding member 39 is provided at the inner end portion of the conductive cyl-

inder 38, and the probe holding member 39 is made of electrically conductive and elastic material such as an electrically conductive silicone rubber. When the probe 29 of the transducer unit 13 is inserted into the tubular member of the insertion sheath 22 and the transducer casing 26 of the transducer unit 13 is fit into the transducer unit connector 15 of the operation area main body 14, the probe holding member 39 closely contacts the probe 29 to electrically connect the probe 29 with the second electrode pin 20.

**[0021]** A cylindrical slider mounting member 40 which is made of electrically insulating material is provided on the outer surface of the conductive cylinder 38.

**[0022]** As shown in FIG. 3, a connection cylinder 41 is detachably connected to the inner end portion of the slider mounting member 40 by a connection pin 42, and a main channel tube 42a into which the probe 29 is inserted is connected to the inner end portion of the connection cylinder 41. The main channel tube 42a is inserted into the tubular member of the insertion sheath 22. A cylindrical electrically conductive member 43 is provided at the proximal end portion of the tubular member. The conductive member 43 is electrically connected to a cylindrical electrically conductive extending portion 44 through an electrically conductive rubber 170, and the extending portion 44 covers the outer circumferential surface of the slider mounting member 40.

**[0023]** The first electrode pin 19 which projects from the casing 14a of the operation area main body 14 includes an intermediate portion 19a, an external connecting portion 19b, and a proximal end portion. The intermediate portion 19a is covered by an electrically insulating cover 45. The external connector 19b projects outward from the casing 14a and is connected to a plug (not shown). And, the proximal end portion has an internal connection pin 46 buried in the casing 14a.

**[0024]** As shown in FIG. 4, the midpoint of a contact plate 47 formed by bending a plate spring to substantially C-shape is fixed to the internal connection pin 46. Contacts 47a are provided on the both end portions of the contact plate 47, and the contacts 47a are elastically in contact with two diametrically separated portions on the outer circumferential surface of the conductive extending portion 44. That is, the first electrode pin 19 is electrically connected to the conductive extending portion 44 of the conductive member 43 through the contact plate 47, and further electrically connected from the conductive member 43 to the insertion sheath 22.

**[0025]** As shown in FIGS. 2 and 3, a slider 48 is provided on the outer circumferential surface of the slider mounting member 40 provided in the inner space of the casing 14a of the operation area main body 14, and the slider 48 is slidable in the longitudinal direction of the slider mounting member 40. The slider 48 is urged by a spring 49 toward the proximal end portion of the inner space of the casing 14a of the operation area main body 14. A connection pin 50 connects the slider 48 to the movable handle 18 pivotally connected to the casing 14a

of the operation area main body 14 by the pivot 17. By rotationally moving the movable handle 18, the slider mounting member 40 is moved forward and backward on the outer surface of the conductive cylinder 38, through the connection pin 50 and slider 48. This movement is transmitted to a drive rod 51 inserted in the tubular member of the insertion sheath 22, through the connection cylinder 41. That is, by moving the movable handle 18 in a direction indicated an arrow F, the drive rod 51 is moved forward in the tubular member of the insertion sheath 22.

**[0026]** Next, the surgical treatment area 23 will be explained with reference to FIGS. 5A to 7. FIG. 5A is a plan view of the surgical treatment area of the surgical instrument of FIG. 1. FIG. 5B is a longitudinal sectional view of the surgical treatment area of FIG. 5A. FIG. 6A is a transverse sectional view along a line of VIA-VIA in FIG. 5B. FIG. 6B is a transverse sectional view along a line of VIB-VIB in FIG. 5B. FIG. 6C is a transverse sectional view along a line of VIC-VIC in FIG. 5B. And, FIG. 7 is a transverse sectional view showing a state that a first grasping member 25 is combined with a second grasping member.

**[0027]** The first grasping member 25 which is pivotally fixed by the pivot pin 24 to the holding member 22a provided at the distal end portion of the tubular member of the insertion sheath 22, is curved a little to the left side from the center of the axis of the insertion sheath 22 in the plane view as shown in FIG. 5A, so as to easily grasp a living tissue. The first grasping member 25 includes a grasping member main body 25a pivotally supported by the holding member 22a, and an ultrasonic surgical treatment area member 25b located in the distal end side of the grasping member main body 25a. A connection pin 53 is provided at the proximal end portion of the grasping member main body 25a, and the distal end portion of the drive rod 51 in the tubular member of the insertion sheath 22 is connected to the connection pin 53.

**[0028]** The distal end portion of the grasping member main body 25a is bifurcated. The ultrasonic surgical treatment area member 25b is pivotally supported in the cut-out 51a of the bifurcated distal end portion of the grasping member main body 25a by a pivot pin 54 whose screw portion 54a is inserted into and fixed to the bifurcated distal end portion, and the ultrasonic surgical treatment area member 25b is rotational in a direction crossing the center of the insertion sheath 22. Therefore, the ultrasonic surgical treatment area member 25b is rotationally movable in the same direction as the first grasping member 25.

**[0029]** The ultrasonic surgical treatment area member 25b includes a pad member 55 forming a pressing portion, and a pair of first electrodes 56 provided symmetrically on both sides of the pad member 55. The pad member 55 is made of a low-friction material such as PTFE (polytetrafluoroethylene), and a square groove 57 is formed in its surface which is used to grasp a living tissue. A row of substantially sawtooth-like teeth 58 is formed

on the surface of each first electrode 56, which is used to grasp the living tissue. The row of teeth 58 makes the surface of each first electrode 56 grasp the living tissue without slipping. The row of teeth 58 projects further outward from the grasping surface of the pad member 55 in a direction crossing the grasping surface of the pad member 55.

**[0030]** The first grasping member 25 configured as described above faces the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 projected forward from the holding member 22a when the probe 29 of the transducer unit 13 is inserted into the insertion sheath 22. The ultrasonic vibrating portion 31 configures a second grasping member 59 which cooperates with the first grasping member 25 to grasp a living tissue. The second grasping member 59 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section at the distal end portion of the probe 29, into a non-circular cross section (a generally reversed T-shape) by a well-known machining such as forging, cutting, and the like. Specifically, a grasping surface 61 opposite to the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and a pair of second electrodes 62 opposite to the rows of teeth 58 of the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b are provided on the surface of the second grasping member 59 opposite to the first grasping member 25.

**[0031]** In the second grasping member 59, the pair of second electrodes 62 is located farther from the ultrasonic surgical treatment area member 25b of the first grasping member 25, than the grasping surface 61, and makes a step to the grasping surface 61. Further, each second electrode 62 forms a gap "g" to each row of teeth 58 of each first electrode 56 of the ultrasonic surgical treatment area member 25b, when the grasping surface 61 contacts the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25. This gap "g" prevents a short circuit between the first electrode 56 and second electrode 62.

**[0032]** That is, when the first grasping member 25 is pivotally moved in a direction where it approaches the second grasping member 59 (grasping operation), the grasping surface 61 of the second grasping member 59 contacts the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, but each second electrode 56 comes close to but faces each row of teeth 58 of each first electrode 56 of the ultrasonic surgical treatment area member 25b with the gap "g" therebetween.

**[0033]** When the first grasping member 25 is rotated around the pivot pin 24 in a direction where it approaches the second grasping member 59 by the operation of the drive rod 51 in the insertion sheath 22, and the first grasping member 25 is placed at a position to grasp a living

tissue in cooperation with the second grasping member 59, the bottom surface of the square groove 57 of the first grasping member 25 and the grasping surface 61 of the second grasping member 59 are in contact with each other to form a cut-join face, and the rows of teeth 58 of the pair of first electrodes 56 and the pair of second electrodes 62 are faced each other and placed in parallel to each other to form a pair of coagulate-join faces.

**[0034]** Since the cut-join face and the pair of coagulate-join faces extend in a direction orthogonal to the opening/closing direction of the first and second grasping members 25 and 59, the first and second grasping members 25 and 59 can provide a strong grasping force to a living tissue.

**[0035]** Further, since the cut-join face and the pair of coagulate-join faces are arranged to separate from each other in the direction orthogonal to the opening/closing direction of the first and second grasping members 25 and 59, the second grasping member 59 configured by the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 does not project from the first grasping member 25 in both sides thereof in the direction orthogonal to the above opening/closing direction. Therefore, the surgical treatment area 23 can be easily inserted into a narrow portion in a body cavity and can perform a treatment thereto.

**[0036]** Next, an operation of the surgical instrument 10 configured as described above will be explained.

**[0037]** For example, when performing a surgical treatment for the purpose of sealing a blood vessel in an abdominal cavity of a patient, the insertion area 12 of the surgical instrument 10 is inserted into the abdominal cavity of the patient through a trocar (not shown) inserted into an opening formed in an abdomen of the patient. Then, the surgical treatment area 23 at the distal end portion of the insertion area 12 is approached a part of the blood vessel where the surgical treatment will be performed.

**[0038]** When the movable handle 18 is not moved in the direction indicated by the arrow F in FIG. 2 with respect to the fixed handle 16, the drive rod 51 is retracted in the tubular member of the insertion sheath 22 by the urging force of the spring 49 in the casing 14a of the operation area main body 14 of the operation area 11, and the first grasping member 25 can be placed at the open position far from the second grasping member 59.

**[0039]** After placing the part of the blood vessel where the surgical treatment will be performed between the second grasping member 59 and the first grasping member 25 placed at the opening position, the movable handle 18 is pivotally moved in the direction indicated by the arrow F in FIG. 2 with respect to the fixed handle 16 of the operation area 11. At this time, the drive rod 51 connected to the slider holding member 40 through the connection cylinder 41 can be advanced in the tubular member of the insertion sheath 22 against the urging force of the spring 49 in the casing 14a of the operation area main body 14 of the operation area 11. The advanced drive

rod 51 pivotally moves the first grasping member 25 toward the second grasping member 59 around the pivot pin 24.

**[0040]** As a result, as shown in FIG. 8, a living tissue S of the part of the blood vessel where the surgical treatment will be performed is grasped between the first and second grasping members 25 and 59. That is, the tissue S is grasped in the cut-join face between the grasping surface 61 of the second grasping member 59 and the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and is also grasped in the coagulate-join faces between the pair of first electrodes 56 on both sides of the square groove 57 of the pad member 55 and the pair of second electrodes 62 on both sides of the grasping surface 61 of the second grasping member 59. In this time, since each of the cut-join face and coagulate-join faces extends in the direction orthogonal to the grasping direction of the first and second grasping members 25 and 59, the tissue S can be grasped by a strong force. Moreover, the rows of teeth 58 provided on the pair of first electrodes 56 prevents the tissue S from slipping and escaping from the grasping members.

**[0041]** When the ultrasonic transducer in the transducer casing 26 of the transducer unit 13 is driven in this state, the ultrasonic vibration generated by the ultrasonic transducer is transmitted to the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 through the probe 29, and the second grasping member 59 configured by the ultrasonic vibrating portion 31 is ultrasonically vibrated. This ultrasonic vibration generates a frictional heat in the part of the tissue S grasped between the grasping surface 61 of the second grasping member 59 and the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and this part of the tissue S is coagulated by the frictional heat, and cut further.

**[0042]** Next, a high-frequency current is applied from a not shown high-frequency power supply to the first electrode pin 19 of the operation area 11. The high-frequency current is led to the tubular member of the insertion sheath 22 through the contact plate 47, conductive extending portion 44, conductive rubber 170 and conductive member 43 in the casing 14a of the operation area main body 14 of the operation area 11, and reaches the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b of the first grasping member 25. The high-frequency current is further led from the pair of first electrodes 56 to the pair of second electrodes 62 of the second grasping member 59 through the tissue S, and returned from the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 forming the second grasping member 59 and the probe 29, to the above-mentioned high-frequency power supply, through the probe holding member 39, conductive cylinder 38, connection terminal 35 and second electrode pin 20 in the

casing 14a of the operation area main body 14 of the operation area 11.

**[0043]** The pair of the portions of the tissue S, where high-frequency current flows between the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b of the first grasping member 25 and the pair of second electrodes 62 of the second grasping member 59, is coagulated.

**[0044]** The tissue S grasped between the first grasping member 25 and the second grasping member 59 is cut at the portion grasped between the grasping surface 61 of the second grasping member 59 and the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and the pair of the portions of the tissue S grasped between the pair of second electrodes 62 of the second grasping member 59 and the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b of the first grasping member 25 is coagulated.

**[0045]** Since the tissue S is a part of the blood vessel to be surgically treated, the above-mentioned part of the blood vessel is cut at the portion grasped between the grasping surface 61 of the second grasping member 59 and the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and is coagulated, that is, sealed at the pair of the portions grasped between the pair of second electrodes 62 of the second grasping member 59 and the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b of the first grasping member 25.

**[0046]** When the first grasping member 25 grasps the tissue S in cooperation with the second grasping member 59, the grasping surface 61 of the second grasping member 59 makes a surface contact with the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25 and forms the cut-join face, and the rows of teeth 58 of the pair of first electrodes 56 of the ultrasonic surgical treatment area member 25b face the pair of second electrodes 62 of the second grasping member 59 in substantially parallel thereto and form the coagulate-join face, thereby the tissue S can be grasped by a sufficiently strong force. Therefore, the coagulation and cutting ability can be increased by using both ultrasonic vibration and high-frequency current, and the surgical treatment time in the surgical treatment area 23 can be reduced.

**[0047]** The ultrasonic vibration and the high frequency current be used at the same time. The ultrasonic vibration may be preferentially used when the cutting is prior to the coagulation, and the high-frequency current may be preferentially used when the coagulation is prior to the cutting.

**[0048]** Next, a surgical instrument according to a second embodiment of the invention will be explained with reference to FIGS. 9A and 9B. In the second embodi-

ment, the same components as those of the first embodiment described above with reference to FIG. 1 to FIG. 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0049]** FIG. 9A is a longitudinal sectional view of a surgical treatment area of the surgical instrument according to the second embodiment of the present invention. FIG. 9B is a transverse sectional view along a line of IXB-IXB in FIG. 9A.

**[0050]** In this embodiment, in a pair of first electrodes 73 on both sides of a pad member 72 in the ultrasonic surgical treatment area member 25b of a first grasping member 71, each of a pair of surface areas to face a pair of second electrodes 75 of a second grasping member 75 is inclined (to 45°, for example) to form an inclined surface 73a with respect to a line CL passing the center of the pad member 72 and extending along the pivotal movement direction of the first grasping member 71. A row of substantially sawtooth-like teeth 74 is formed at the outer end portion of the inclined surface 73a of each first electrode 73 to grasp a living tissue without slipping.

**[0051]** Further, in this embodiment, the second grasping member 75 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section (substantially an octagonal form), by a well-known machining such as forging, cutting and the like. The surface of the second grasping member 75 facing to the first grasping member 71 has a grasping surface 76 facing to the pad member 72 of the ultrasonic surgical treatment area member 25b of the first grasping member 71, and a pair of second electrodes 77 which faces the inclined surface 73a of the pair of first electrodes 73 of the ultrasonic surgical treatment area member 25b and which has inclined surfaces 77a inclined similarly to the inclined surfaces 73a.

**[0052]** When the grasping surface 76 of the second grasping member 75 contacts the facing surface of the pad member 72 of the ultrasonic surgical treatment area member 25b of the first grasping member 71, each inclined surface 77a of the pair of second electrodes 77 of the second grasping member 75 faces each inclined surface 73a of the pair of first electrodes 73 of the ultrasonic surgical treatment area member 25b of the first grasping member 71 with a gap "g" between them.

**[0053]** When the first grasping member 71 is pivotally moved around the pivot pin 24 in the direction in which the first grasping member 71 comes close to the second grasping member 75, and the first grasping member 71 is placed at a position where the first grasping member 71 grasps a living tissue in cooperation with the second grasping member 75 between them, the pad member 72 of the first grasping member 71 makes a surface contact with the grasping surface 76 of the second grasping member 75 and forms a cut-join face, and the inclined surfaces 73a of the pair of first electrodes 73 face the inclined surfaces 77a of the pair of second electrodes 77 in substantially parallel thereto and form a pair of coag-

ulate-join faces.

**[0054]** Since the cut-join face extends in a direction orthogonal to the opening/closing direction of the first and second grasping members 71 and 75, and each coagulate-join face is inclined (to 45° for example) to the direction orthogonal to the above opening/closing direction, the first and second grasping members 71 and 75 can provide a strong grasping force for the living tissue.

**[0055]** Further, since the cut-join face and the pair of coagulate-join faces are arranged to separate from each other in the direction orthogonal to the opening/closing direction of the first and second grasping members 71 and 75, the second grasping member 75 configured by the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 is not projected from the first grasping member 71 in its both sides in the direction orthogonal to the above opening/closing direction. Therefore, the surgical treatment area 23 can be easily inserted into a narrow portion of an abdominal cavity and treat it.

**[0056]** Next, a surgical instrument according to a third embodiment of the invention will be explained with reference to FIGS. 10A and 10B. In the third embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0057]** FIG. 10A is a longitudinal sectional view of a surgical treatment area of the surgical instrument according to a third embodiment of the invention. FIG. 10B is a transverse sectional view along a line of XB-XB in FIG. 10A.

**[0058]** In this embodiment, a pair of first electrodes 83 in both sides of a pad member 82 in the ultrasonic surgical treatment area member 25b of a first grasping member 81 is projected along and in parallel to a line CL passing the center of the pad member 82 and extending along the moving direction of the first grasping member 81. A row of substantially sawtooth-like teeth 84 is formed on each projected end surface of the pair of first electrodes 83 to grasp a living tissue without slipping.

**[0059]** Further, in this embodiment, a second grasping member 88 is provided by machining the ultrasonic vibrating portion 31, which has conventionally the circular cross section, at the distal end portion of the probe 29, into a non-circular cross section (rectangular), by a well-known machining such as forging, cutting, and the like. The surface of the second grasping member 85 which faces the first grasping member 81 has a grasping surface 86 which faces a pad member 82 of the ultrasonic surgical treatment area member 25b of the first grasping member 81, and a pair of second electrodes 87 which face the inside surfaces of the pair of first electrodes 83 of the ultrasonic surgical treatment area member 25b.

**[0060]** When the grasping surface 86 of the second grasping member 85 contacts the facing surface of the pad member 82 of the ultrasonic surgical treatment area member 25b of the first grasping member 81, each second electrode 87 of the second grasping member 85 fac-



es each inside surface of the pair of first electrodes 83 of the ultrasonic surgical treatment area member 25b of the first grasping member 81 with a gap "g" therebetween.

**[0061]** When the first grasping member 81 is pivotally moved around the pivot pin 24 in the direction in which the first grasping member 81 comes close to the second grasping member 85 and placed at a position where the first grasping member 81 grasps a living tissue in cooperation with the second grasping member 85, the pad member 82 of the first grasping member 81 makes a surface contact with the grasping surface 86 of the second grasping member 85 and forms a cut-join face, and the inside surfaces of the pair of first electrodes 83 face the pair of second electrodes 87 in substantially parallel thereto and form a pair of coagulate-join faces.

**[0062]** Since the cut-join face extends in the direction orthogonal to the opening/closing direction of the first and second grasping members 81 and 85, and the pair of coagulate-join faces extends in parallel to the above opening/closing direction, the first and second grasping members 81 and 85 can provide a strong grasping force for a living tissue.

**[0063]** Further, since the cut-join face and the pair of coagulate-join faces are separated from each other in the direction orthogonal to the opening/closing direction of the first and second grasping members 81 and 85, the second grasping member 85 configured by the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 does not project from the first grasping member 81 in its both sides in the direction orthogonal to the above opening/closing direction. Therefore, the surgical treatment area 23 can be easily inserted into a narrow portion in an abdominal cavity and treat it.

**[0064]** Next, a surgical instrument according to a fourth embodiment of the invention will be explained with reference to FIGS. 11A and 11B. In the fourth embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0065]** FIG. 11A is a longitudinal sectional view of a surgical treatment area of a surgical instrument according to a fourth embodiment of the invention. FIG. 11B is a transverse sectional view along a line of XIB-XIB in FIG. 11A.

**[0066]** In this embodiment, only a second grasping member 88 is different from the first embodiment. The second grasping member 88 is provided by machining the ultrasonic vibrating portion 31 which has a conventionally circular cross section, at the distal end portion of the probe 29, into a non-circular cross section (substantially a reversed T-shape), by a well-known machining such as forging, cutting, and the like. The cross section of the second grasping member 59 of the first embodiment shown in FIGS. 7 and 8 is also a reversed T-shape. But, the cross section of the second grasping member 88 of the fourth embodiment is slightly different from that

of the second grasping member 59 of the first embodiment. Specifically, a portion of the second grasping member 88 of the fourth embodiment, which project from the midpoint of the laterally extending surface of the second grasping member 88, the laterally extending surface facing the first grasping member 25, in the direction crossing the lateral direction, and which is inserted into the square groove 57 of the pad member 55 of the ultrasonic surgical treatment member 25b of the first grasping member 25, is formed to have a triangular shape having an acute angle at its projected end.

**[0067]** In the cross section of the facing surface of the second grasping member 88 of the fourth embodiment, the above described triangular portion forms a grasping surface 89, and a pair of portions extending laterally in both sides of the grasping surface 89 forms a pair of flat second electrodes 90 which face the pair of first electrodes 56 (the rows of teeth 58) of the ultrasonic surgical treatment area member 25b of the first grasping member 25.

**[0068]** When the first grasping member 25 is pivotally moved around the pivot pin 24 in the direction in which the first grasping member 25 comes close to the second grasping member 88 and a contact portion 25c of the grasping part main body 25a contacts a contact portion 22c of the holding member 22a at the distal end portion of the insertion sheath 22, a gap "h" is formed between the acute projected end of the grasping surface 89 of the second grasping member 88 and the bottom surface of the square groove 57 of the pad member 55 of the ultrasonic surgical treatment area member 25b of the first grasping member 25, and a gap "g" is formed between each second electrode 90 of the second grasping member 88 and each first electrode 56 (the row of teeth 58) of the ultrasonic surgical treatment area member 25b of the first grasping member 25.

**[0069]** When the first grasping member 25 is pivotally moved around the pivot pin 24 in the direction in which the first grasping member 25 comes close to the second grasping member 88 and placed at a position where the first grasping member 25 grasps a living tissue in cooperation with the second grasping member 88, the acute end of the grasping surface 89 of the second grasping member 88 extends to the bottom surface of the square groove 57 of the pad member 55 of the first grasping member 25 in a direction orthogonal to the center line of the pivot pin 24 of the first grasping member 25 and forms a cut-join line, and the pair of first electrodes 56 and the pair of second electrodes 90 face each other in substantially parallel to each other and form a pair of coagulate-join faces.

**[0070]** Since the cut-join line extends in the direction orthogonal to the center line of the pivot pin 24 of the first grasping member 25 and the pair of coagulate-join faces extends in the direction orthogonal to the opening/closing direction of the first and second grasping members 25 and 88, the first and second grasping members 25 and 88 can provide a strong grasping force for a living tissue.

**[0071]** Further, since the cut-join line and the pair of coagulate-join faces are separated from each other in the direction orthogonal to the opening/closing direction of the first and second grasping members 25 and 88, the second grasping member 88 configured by the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 does not project from the first grasping member 25 in both sides thereof in the direction orthogonal to the above opening/closing direction. Therefore, the surgical treatment area 23 can be easily inserted into a narrow portion in an abdominal cavity and treat it.

**[0072]** In this embodiment, since the acute end of the grasping surface 89 of the second grasping member 88 does not contact the bottom surface of the square groove 57 of the pad member 55 of the first grasping member 25, the bottom surface of the square groove 57 of the pad member 55 is not worn by the grasping surface 89 of the second grasping member 88, and the durability of this embodiment increases.

**[0073]** The cut-join line formed by making the acute end of the grasping surface 89 of the second grasping member 88 in contact with the bottom surface of the square groove 57 of the pad member 55 of the first grasping member 25 generates a large concentration of grasping force for a living tissue grasped between the grasping surface 89 of the second grasping member 88 and the bottom surface of the square groove 57 of the pad member 55 of the first grasping member 25.

**[0074]** Next, a surgical instrument according to a fifth embodiment of the invention will be explained with reference to FIGS. 12A and 12B. In the fifth embodiment, the same components as those of the first embodiment described above with reference to FIG. 1 to FIG. 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0075]** FIG. 12A is a schematic perspective view of a surgical treatment area of a surgical instrument according to a fifth embodiment of the invention. FIG. 12B is a transverse sectional view showing a state in which a living tissue is grasped by first and second grasping members of the surgical treatment area of FIG. 12A.

**[0076]** In this embodiment, a first grasping member 91 is formed like a flat plate. A pad member 92 having an arc-shaped cross section is provided at a mid portion of a flat grasping surface of the first grasping member 91 in a lateral direction thereof. A pair of first electrodes 93 is provided in both sides of the pad member 92 on the above grasping surface.

**[0077]** A second grasping member 94 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, a grasping surface 95 having a concave cross section is provided in a portion of the second grasping member 94 which faces the first grasping member 91, the grasping surface 95 corresponding to the pad member 92 of the first grasping member 91. A pair of

second electrodes 96 is provided at both edge portions of the grasping surface 95 in its cross section to face the pair of first electrodes 93 of the first grasping member.

**[0078]** When the first grasping member 91 is pivotally moved in the direction in which the first grasping member 91 comes close to the second grasping member 94 and placed at a position where the first grasping member 91 grasps a living tissue in cooperation with the second grasping member 94, the pad member 92 of the first grasping member 91 makes a surface contact with the grasping surface 95 of the second grasping member 88 and forms a curved cut-join face, and the acute ends of the pair of second electrodes 96 face the pair of first flat electrode 93 and form a pair of coagulate-join lines extending in a direction orthogonal to the center line of the pivotal movement of the first grasping member 91.

**[0079]** The pair of coagulate-join lines formed by the pair of first flat electrodes 93 of the first grasping member 91 and the acute ends of the pair of second electrodes 96 at the both side edges of the grasping surface 95 of the second grasping member 94, generates a large concentration of grasping force for the tissue S grasped by the pad member 92 of the first grasping member 91 and the grasping surface 95 of the second grasping member 94.

**[0080]** In this embodiment, the first grasping member 91 can be made more compact than the second grasping member 94 configured by the ultrasonic vibrating portion 31 at the distal end portion of the probe 29. Therefore, the surgical treatment area 23 can be easily inserted into a narrow portion in an abdominal cavity and treat it.

**[0081]** Next, a surgical instrument according to a sixth embodiment of the present invention will be explained with reference to FIG. 13. In the sixth embodiment, the same components as those of the first embodiment described above with reference to FIG. 1 to FIG. 8 will be denoted the same reference numerals and detailed explanation thereof will be omitted.

**[0082]** FIG. 13 is a schematic perspective view of a surgical treatment area of the surgical instrument according to the sixth embodiment of the present invention.

**[0083]** In this embodiment, a first grasping member 101 has a semicircular cross section, and a pad member 103 is buried in a rounded groove 102 made at the lateral center of the surface of the first grasping member 101, the surface facing a second grasping member 105. A pair of first flat electrodes 104 is provided in both sides of the pad member 103 on the facing surface of the first grasping member 101.

**[0084]** The second grasping member 105 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, a grasping surface 106 projecting toward the pad member 103 of the facing surface of the first grasping member 101 and a pair of second flat electrodes 107 arranged in both sides of the grasping

surface 106 and facing the pair of first flat electrodes 104 of the facing surface of the first grasping member 101 are provided on a part of the second grasping member 105 facing the first grasping member 101. The grasping surface 106 is shaped like waves gently continuing along the extending direction of the pad member 10.

**[0085]** When the first grasping member 101 is pivotally moved in the direction in which the first grasping member 101 comes close to the second grasping member 105 and placed at a position where the first grasping member 101 grasps a living tissue in cooperation with the second grasping member 105, the pad member 103 of the first grasping member 101 discontinuously contacts the gently continuing wave-shaped grasping surface 106 of the second grasping member 105 and forms a cut-join face, and the pair of second flat electrodes 107 face the pair of first flat electrodes 104 in parallel thereto and form a pair of coagulate-join faces which are extending in the direction orthogonal to the center line of the opening/closing direction of the first grasping member 101.

**[0086]** The above described cut-join face and pair of coagulate-join faces can provide a strong grasping force for the tissue between the first grasping member 101 and second grasping member 105. In this embodiment, it is unnecessary to provide a row of teeth for anti-slipping on each of the pair of first electrodes 104, and the pair of first electrodes 104 can minutely coagulate the tissue in cooperation with the pair of second electrodes 107.

**[0087]** Next, a surgical instrument according to a seventh embodiment of the invention will be explained with reference to FIGS. 14A and 14B. In the seventh embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0088]** FIG. 14A is a schematic perspective view of a surgical treatment area of the surgical instrument according to the seventh embodiment of the invention.

**[0089]** FIG. 14B is a transverse sectional view along a line of XIVB-XIVB in FIG. 14A.

**[0090]** In this embodiment, a first grasping member 111 has a cross section similar to a cross section of a saddle for riding a horse, and a pad member 113 is buried in a rounded groove 112 at the center of a surface of the first grasping member 111 in the lateral direction, the surface facing a second grasping member 115. In the opposite surface of the first grasping member 111, A pair of portions projected from both sides of the pad member 113 on the facing surface of the first grasping member 111 is configured as a pair of first electrodes 114.

**[0091]** The second grasping member 115 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, the surface of the second grasping member 115 which faces the first grasping member 111 is formed to have a cross section corresponding to

the facing surface of the first grasping member 111.

**[0092]** That is, a portion of the facing surface of the second grasping member 115, the portion corresponding to the pad member 113 on the facing surface of the first grasping member 111, is configured as a grasping surface 116 projecting toward the pad member 113 and having a rounded substantially triangular cross section, and a pair of portions of the facing surface of the second grasping member 115, the portions corresponding to the pair of first electrodes 114 of the facing surface of the first grasping member 111, is configured as a pair of concaved second electrodes 117 to receive the pair of first projecting electrodes 114.

**[0093]** When the first grasping member 111 is pivotally moved in a direction in which the first grasping member 111 comes close to the second grasping member 115 and placed at a position where the first grasping member 111 grasps a living tissue in cooperation with the second grasping member 115, the pad member 113 of the first grasping member 111 makes a line contact with the grasping surface 116 of the second grasping member 115 and forms a cut-join face, and the pair of first electrodes 114 contacts the pair of second electrodes 117 in a wide area and forms a pair of coagulate-join faces.

**[0094]** Next, a surgical instrument according to an eighth embodiment of the present invention will be explained with reference to FIG. 15. In the eighth embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0095]** FIG. 15 is a schematic transverse sectional view of a surgical treatment area of the surgical instrument according to the eighth embodiment of the present invention.

**[0096]** In this embodiment, a first grasping member 121 has an arc-shaped cross section. A pad member 122 is provided at the center of the arc-shape, and first and second electrodes 124 and 127 are provided on both sides of the pad member 122. The inner surface 123 of the first grasping member 121 faces a second grasping member 125.

**[0097]** The second grasping member 125 is configured by the rounded bar-shaped ultrasonic vibrating portion 31 at the distal end portion of the probe 29. The portion of the outer circumferential surface of the second grasping member 125 facing the inner surface 123 of the first grasping member 121 forms a grasping surface 126.

**[0098]** When the first grasping member 121 is pivotally moved in a direction in which the first grasping member 121 comes close to the second grasping member 125 and placed at a position where the first grasping member 121 grasps a living tissue in cooperation with the second grasping member 125, the pad member 122 of the first grasping member 121 makes a surface contact with the grasping surface 126 of the second grasping member 125 and forms a cut-join face, and the first electrode 124 and the second electrode 127 facing each other through

the pad member 122 form coagulate-join faces. The first electrode 124 and the second electrode 127 apply a high-frequency current to the living tissue grasped between the inner surface 123 of the first grasping member 121 and the grasping surface 126 of the second grasping member 125.

**[0099]** Next, a surgical instrument according to a ninth embodiment of the present invention will be described with reference to FIG. 16. In the ninth embodiment, the same components as those of the first embodiment described above with reference to FIG. 1 to FIG. 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0100]** FIG. 16 is a schematic perspective view of a surgical treatment area of the surgical instrument according to the ninth embodiment of the invention.

**[0101]** In this embodiment, a first grasping member 131 includes two independent parts. The two parts of the first grasping member 131 are pivotally connected to two surfaces of a holding member 22a having a triangular cross section, by pivots 132. Two edge portions of the two parts of the first grasping member 131 adjacent to each other are configured as pad members 133, and the inner surfaces of two edge portions of the two parts of the first grasping member 131 located away from each other are configured as first electrodes.

**[0102]** The second grasping member 135 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, a surface of the second grasping member 135 which faces the two parts of the first grasping member 131, is formed to correspond to the above described two surfaces of the holding member 22a having the triangular cross section.

**[0103]** A ridge portion of the triangular cross sectioned facing surface of the second grasping member 135, the ridge portion corresponding to the pad members 133 of the two adjacent edge portions of the first grasping member 131 is configured as a grasping surface 136, and the foot end portions of the triangular cross sectioned facing surface are configured as a pair of second electrodes 137.

**[0104]** When the two parts of the first grasping member 131 are pivotally moved to the second grasping member 135 in directions in which the two parts come close to the longitudinal center line 31a of the second grasping member 135 and placed at positions where the two parts grasp a living tissue in cooperation with the second grasping member 135, each of the pad members 133 of the two parts of the first grasping member 131 makes a surface contact with the grasping surface 136 of the second grasping member 135 and forms a cut-join face, and the first electrodes and the second electrodes 137 are faced each other and in parallel to each other, and form coagulate-join surfaces.

**[0105]** That is, since each of the opening/closing di-

rections of the two parts of the first grasping member 131 is a radial direction of the second grasping member 135 that is the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 and each of the pair of coagulate-join surfaces is formed in the direction orthogonal to each opening/closing direction, a strong grasping force can be proved for a living tissue on the pair of coagulate-join surfaces.

**[0106]** Next, a surgical instrument according to a tenth embodiment of the invention will be explained with reference to FIG. 17. In the tenth embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0107]** FIG. 17 is a schematic transverse sectional view of a surgical treatment area of the surgical instrument according to the tenth embodiment of the invention.

**[0108]** In this embodiment, only a second grasping member 138 is different from the first embodiment. The second grasping member 138 which grasps a living tissue in cooperation with the first grasping member 25, is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, the surface of the second grasping member 138, which faces the first grasping member 25, includes a grasping surface 139 configured by a projecting portion facing the square groove 57 of the pad member 55 of the first grasping member 25, and a pair of second electrodes 140 having flat surfaces facing the pair of first electrodes 56 (the rows of teeth 58) in both sides of the grasping surface 139. When the projected end of the grasping surface 139 contacts the bottom surface of the square groove 57 of the pad member 55 of the first grasping member 25, each of the pair of second electrodes 140 is placed at a position where a gap "g" is formed between each of the pair of second electrodes 140 and each of the pair of first electrodes 56 (the rows of teeth 58). Further, insulating layers 141 are formed by insulation coating on both sides of the projected grasping surface 139 of the second grasping member 138, but the second electrodes 140 are not insulated by insulation coating. Therefore, the areas of the pair of first electrodes 56 can be substantially the same as those of the pair of second electrodes 140 and a current density therebetween can be increased, and a living tissue grasped therebetween can be efficiently coagulated.

**[0109]** Next, a surgical instrument according to an eleventh embodiment of the present invention will be explained with reference to FIG. 18. In the eleventh embodiment, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0110]** FIG. 18 is a schematic transverse sectional view of a surgical treatment area of the surgical instru-

ment according to the eleventh embodiment of the invention.

**[0111]** In a first grasping member 151 of this embodiment, an insulating block 154 made of synthetic resin is further integrally provided on an outside of each of a pair of first electrodes 153 on both sides of a pad member 152. The insulating block 154 is projected in the grasping direction from the first electrode 153. A row of teeth 155 is formed in the projected end of the insulating block 154.

**[0112]** A second grasping member 156 which grasps a living tissue in cooperation with the first grasping member 151 is provided by machining the ultrasonic vibrating portion 31 which has conventionally a circular cross section, at the distal end portion of the probe 29, into a non-circular cross section, by a well-known machining such as forging, cutting, and the like. Specifically, the surface of the second grasping member 156, which faces the first grasping member 151, is configured to a cross section of isosceles trapezoidal. The distal end of the second grasping member 156 is configured as a grasping surface 157 which is to be in contact with the pad member 152 of the first grasping member 151, and two legs on both sides of the grasping surface 157 are configured as a pair of second electrodes 158 having a pair of inclined surfaces 158a which face the pair of first electrodes 153.

**[0113]** When the first grasping member 151 is pivotally moved in a direction in which the first grasping member 151 comes close to the second grasping member 156 and placed at a position where the first grasping member 151 grasps a living tissue in cooperation with the second grasping member 156, the pad member 152 of the first grasping member 151 contacts the grasping surface 157 of the second grasping member 156 and forms a cut-join face. The pair of first electrodes 153 of the first grasping member 151 faces the pair of second electrodes 158 of the second grasping member 156 and forms a pair of coagulate-join faces. In this embodiment, even if a force directing in a lateral direction is applied to the ultrasonic vibrating portion 31 at the distal end portion of the probe 29, the vibrating portion 31 does not directly contact the pair of first electrodes 153. Therefore, the durability of the ultrasonic vibrating portion 31 at the distal end portion of the probe 29 is increased.

**[0114]** Next, an example of a surgical instrument which is different from the conventional one will be explained with reference to FIGS. 19A and 19B. In this example, the same components as those of the first embodiment described above with reference to FIGS. 1 to 8 will be denoted by the same reference numerals and detailed explanation thereof will be omitted.

**[0115]** FIG. 19A is a schematic perspective view of a surgical treatment area of the example of the surgical instrument which is different from the conventional one.

**[0116]** FIG. 19B is a schematic transverse sectional view along a line of XIX-XIX in FIG. 19A.

**[0117]** In this example, a first grasping member 161 is a member having a rectangular cross section, and has a row of sawtooth-like teeth 162 on its grasping surface.

A groove 163 is formed at the center of the cross section of the first grasping member 161 and extends in its axial direction. A first electrode 164 is buried in the groove 163. A pad member 165 is provided on the grasping surface of the first grasping member 161.

**[0118]** A second grasping member 166 to grasp a living tissue in cooperation with the first grasping member 161 is configured by the ultrasonic vibrating portion 31 at the distal end portion of the round bar-shaped probe 29. A portion of the outer circumferential surface of the second grasping member 166, the portion facing the first grasping member 161, is configured as a grasping surface 167 at a point being in contact with the pad 165 of the first grasping member 161. The outer surface of the second grasping member 166, Both sides of the grasping surface 167 on the portion of the outer circumferential surface of the second grasping member 166, the portion facing the first grasping member 161, are configured as a pair of second arc-shaped electrodes 168 which face the first electrode 164.

**[0119]** When the first grasping member 161 is pivotally moved in a direction in which the first grasping member 161 comes close to the second grasping member 166 and grasps a living tissue in cooperation with the second grasping member 166, the row of teeth 162 on the grasping surface of the first grasping member 161 contacts the living tissue, the pad member 165 on the grasping surface of the first grasping member 161 partially contacts the grasping surface 167 of the second grasping member 166 and forms a cut-join face. The first electrode 164 of the first grasping member 161 faces the pair of second electrodes 168 of the second grasping member 166 and forms coagulate-join faces.

**[0120]** This invention is not limited to the embodiments described hereinbefore. This invention may be embodied in various forms by modifying various component members without departing from an aspect of the invention. Further, the various component members disclosed in the above described various embodiments may be properly combined with each other. For example, some component members may be deleted from all components members shown in each embodiment.

## Claims

1. A surgical instrument, comprising: a first grasping member (25, 71, 81, 91, 101, 111, 151) and second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156) to open and close relative to each other; an ultrasonic vibrating portion (31) which is provided in the second grasping member, which is connected to an ultrasonic transducer to generate ultrasonic vibration, and which has a grasping surface (61, 76, 86, 89, 95, 106, 116, 139, 157) to be in contact with a living tissue (S) grasped between the first grasping member and the second grasping member; a first high-frequency electrode portion (56, 73, 83, 93,

104, 114, 153) provided in the first grasping member; and a second high-frequency electrode portion (62, 75, 77, 87, 90, 96, 107, 117, 140, 158) provided in the second grasping member to be independent of the first high-frequency electrode portion, wherein the surgical instrument can cut the living tissue grasped between the first grasping member and the second grasping member by the ultrasonic vibration from the grasping surface of the ultrasonic vibrating portion, and can further coagulate the cut portion of the living tissue by the high-frequency current between the first high-frequency electrode portion and the second high-frequency electrode portion, the surgical instrument being **characterized in that:**

a pressing portion (55, 72, 82, 92, 103, 113, 152) is further provided in the first grasping member (25, 71, 81, 91, 101, 111, 151), the pressing portion being in contact with the living tissue (S) grasped between the first grasping member and the second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156), and pressing the living tissue in cooperation with the grasping surface (61, 76, 86, 89, 95, 106, 116, 139, 157) of the ultrasonic vibrating portion (31);

the first high-frequency electrode portion (56, 73, 83, 93, 104, 114, 153) includes at least a pair of electrodes which are arranged in both sides of the pressing portion (55, 72, 82, 92, 103, 113, 152) in the first grasping member (25, 71, 81, 91, 101, 111, 151);

the second high-frequency electrode portion (62, 75, 77, 87, 90, 96, 107, 117, 140, 158) includes at least a pair of electrodes which are arranged in the both sides of the pressing portion (55, 72, 82, 92, 103, 113, 152) in the second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156) to oppose to the electrodes of the first high-frequency electrode portion (56, 73, 83, 93, 104, 114, 153); and

the electrodes of the first high-frequency electrode portion (56, 73, 83, 93, 104, 114, 153) and the electrodes of the second high-frequency electrode portion (62, 75, 77, 87, 90, 96, 107, 117, 140, 158) cooperate with each other in the both sides of the pressing portion (55, 72, 82, 92, 103, 113, 152) to press the living tissue (S) grasped between the first grasping member (25, 71, 81, 91, 101, 111, 151) and the second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156) while the living tissue is pressed by the pressing portion of the first grasping member and the grasping surface (61, 76, 86, 89, 95, 106, 116, 139, 157) of the ultrasonic vibrating portion (31).

2. The surgical instrument according to claim 1, **characterized in that**

a distance from a longitudinal center line of the second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156) to the grasping surface (61, 76, 86, 89, 95, 106, 116, 139, 157) of the ultrasonic vibrating portion (31) provided in the second grasping member and a distance from the longitudinal center line of the second grasping member to each electrode of the second high-frequency electrode portion (62, 75, 77, 87, 90, 96, 107, 117, 140, 158) provided in the second grasping member are different from each other.

3. The surgical instrument according to claim 2, **characterized in that**

a gap (g) is provided between each of the electrodes of the first high-frequency electrode portion (56, 73, 83, 93, 104, 114, 153) and each of the electrodes of the second high-frequency electrode portion (62, 75, 77, 87, 90, 96, 107, 117, 140, 158) while the grasping surface (61, 76, 86, 89, 95, 106, 116, 139, 157) of the ultrasonic vibrating portion (31) provided in the second grasping member is closest to the pressing portion (55, 72, 82, 92, 103, 113, 152) of the first grasping member (25, 71, 81, 91, 101, 111, 151).

4. The surgical instrument according to claim 2 or 3, **characterized in that**

the distance from the longitudinal center line of the second grasping member (59, 75, 85, 88, 105, 115, 138, 156) to the grasping surface (61, 76, 86, 89, 106, 116, 139, 157) of the ultrasonic vibrating portion (31) provided in the second grasping member is longer than the distance from the longitudinal center line of the second grasping member to each electrode of the second high-frequency electrode portion (62, 77, 87, 90, 107, 117, 140, 158) provided in the second grasping member.

5. The surgical instrument according to any one of the claims 2 to 4, **characterized in that:**

the grasping surface (61, 139) of the ultrasonic vibrating portion (31) provided in the second grasping member (59, 138) and a part of the pressing portion (55) provided in the first grasping member (25), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other; the electrodes of the first high-frequency electrode portion (56) provided in the first grasping member (25) and the electrodes of the second high-frequency electrode portion (62, 140) provided in the second grasping member (59, 138) face to each other in the direction along which the first grasping member and the second grasping member open and close relative to each other; and

an extending direction of the grasping surface (61, 139) of the ultrasonic vibrating portion (31) provided in the second grasping member (59, 138) and an extending direction of each electrode of the second high-frequency electrode portion (62, 140) provided in the second grasping member are the same as to each other in a direction which is orthogonal to the opening and closing direction and which crosses the longitudinal center line of the second grasping member.

6. The surgical instrument according to any one of the claims 2 to 4, **characterized in that:**

the grasping surface (76) of the ultrasonic vibrating portion (31) provided in the second grasping member (75) and a part of the pressing portion (72) provided in the first grasping member (71), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other;  
the electrodes of the first high-frequency electrode portion (56) provided in the first grasping member (71) and the electrodes of the second high-frequency electrode portion (77) provided in the second grasping member (75) incline with respect to the opening and closing direction of the first and second grasping members; and  
the grasping surface (76) of the ultrasonic vibrating portion (31) provided in the second grasping member (75) extends in a direction which is orthogonal to the opening and closing direction and which crosses the longitudinal center line of the second grasping member.

7. The surgical instrument according to any one of the claims 2 to 4, **characterized in that:**

the grasping surface (86) of the ultrasonic vibrating portion (31) provided in the second grasping member (85) and a part of the pressing portion (82) provided in the first grasping member (81), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other;  
the electrodes of the first high-frequency electrode portion (83) provided in the first grasping member (81) and the electrodes of the second high-frequency electrode portion (87) provided in the second grasping member (85) oppose to each other in a direction which is orthogonal to the opening and closing direction and which crosses the longitudinal center line of the second grasping member;

the electrodes of the first high-frequency electrode portion (83) provided in the first grasping member (81) and the electrodes of the second high-frequency electrode portion (87) provided in the second grasping member (85) extend in the opening and closing direction of the first and second grasping members, and  
the grasping surface (86) of the ultrasonic vibrating portion (31) provided in the second grasping member (85) extends in a direction which is orthogonal to the opening and closing direction and which crosses the longitudinal center line of the second grasping member.

8. The surgical instrument according to any one of the claims 2 to 4, **characterized in that:**

the grasping surface (89) of the ultrasonic vibrating portion (31) provided in the second grasping member (88) and a part of the pressing portion (55) provided in the first grasping member (25), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other;  
the electrodes of the first high-frequency electrode portion (56) provided in the first grasping member (25) and the electrodes of the second high-frequency electrode portion (90) provided in the second grasping member (88) oppose to each other in the opening and closing direction of the first and second grasping members;  
the grasping surface (89) of the ultrasonic vibrating portion (31) provided in the second grasping member (88) has a triangular cross section which crosses the longitudinal center line of the second grasping member, an apex of the triangular cross section opposing to the pressing portion (55) of the first grasping member (25); and  
each electrode of the second high-frequency electrode portion (90) provided in the second grasping member (88) extends in the direction which is orthogonal to the opening and closing direction and which crosses the longitudinal center line of the second grasping member.

9. The surgical instrument according to claim 2 or 3, **characterized in that**

the distance from the longitudinal center line of the second grasping member (94) to the grasping surface (95) of the ultrasonic vibrating portion (31) provided in the second grasping member is shorter than the distance from the longitudinal center line of the second grasping member to each electrode of the second high-frequency electrode portion (96) provided in the second grasping member.

**10. The surgical instrument according to claim 9, characterized in that:**

the pressing portion (92) of the first grasping member (91) projects toward the grasping surface (95) of the ultrasonic vibrating portion (31) provided in the second grasping member (94); and  
the grasping surface (95) of the ultrasonic vibrating portion (31) provided in the second grasping member (94) is indented to receive the projecting pressing portion (92) of the first grasping member (91).

**11. The surgical instrument according to any one of the claims 2 to 4, characterized in that:**

the grasping surface (106) of the ultrasonic vibrating portion (31) provided in the second grasping member (105) and a part of the pressing portion (103) provided in the first grasping member (101), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other; the electrodes of the first high-frequency electrode portion (104) provided in the first grasping member (101) and the electrodes of the second high-frequency electrode portion (107) provided in the second grasping member (105) oppose to each other in the opening and closing direction of the first and second grasping members; and  
the grasping surface (106) of the ultrasonic vibrating portion (31) provided in the second grasping member (105) is waved in a direction which is orthogonal to the opening and closing direction and which is along the longitudinal center line of the second grasping member.

**12. The surgical instrument according to any one of the claims 2 to 4, characterized in that:**

the grasping surface (116) of the ultrasonic vibrating portion (31) provided in the second grasping member (115) and a part of the pressing portion (113) provided in the first grasping member (111), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other; the electrodes of the first high-frequency electrode portion (114) provided in the first grasping member (111) and the electrodes of the second high-frequency electrode portion (117) provided in the second grasping member (115) oppose

to each other in the opening and closing direction of the first and second grasping members; the first grasping member (111) includes a pair of further opposing parts in outer sides of the electrodes of the first high-frequency electrode portion (114) and the second grasping member (115) includes a pair of further opposing parts in outer sides of the electrodes of the second high-frequency electrode portion (117), the further opposing parts of the first grasping member and the further opposing parts of the second grasping member opposing to each other in the opening and closing direction of the first and second grasping members;

each of the further opposing parts of the first grasping member (111) inclines such that the each of further opposing parts goes away from the part of the pressing portion (113), the part opposing to the grasping surface (116) of the ultrasonic vibrating portion (31) provided in the second grasping member, in a direction which is orthogonal to the opening and closing direction and which is orthogonal to the longitudinal center line of the second grasping member (115), and approaches the opposing part of the pressing portion (113) in the opening and closing direction; and

each of the further opposing parts of the second grasping member (115) inclines such that the each of further opposing parts is farther away from the grasping surface (116) of the ultrasonic vibrating portion (31) in the direction which is orthogonal to the opening and closing direction and which is orthogonal to the longitudinal center line of the second grasping member, and approaches the grasping surface in the opening and closing direction.

**13. The surgical instrument according to any one of the claims 2 to 4, characterized in that:**

the grasping surface (157) of the ultrasonic vibrating portion (31) provided in the second grasping member (156) and a part of the pressing portion (152) provided in the first grasping member (151), the part opposing to the grasping surface of the ultrasonic vibrating portion, face to each other in a direction along which the first grasping member and the second grasping member open and close relative to each other; the electrodes of the first high-frequency electrode portion (153) provided in the first grasping member (151) and the electrodes of the second high-frequency electrode portion (158) provided in the second grasping member (156) incline with respect to the opening and closing direction of the first and second grasping members; the grasping surface (157) of the ultrasonic vi-



brating portion (31) provided in the second grasping member (156) curves in a cross section which crosses the longitudinal center line of the second grasping member; and  
 the part of the pressing portion (152) provided in the first grasping member (151), the part opposing to the grasping surface of the ultrasonic vibrating portion, curves in a cross section which crosses the longitudinal center line of the second grasping member, to follow the curvature of the cross section of the grasping surface of the ultrasonic vibrating portion.

14. The surgical instrument according to any one of the claims 1 to 13, **characterized in that** the ultrasonic vibrating portion (31) configures the second grasping member (59, 75, 85, 88, 94, 105, 115, 138, 156).

15. A surgical instrument, comprising: a first grasping member (121, 131) and second grasping member (125, 135) to open and close relative to each other; an ultrasonic vibrating portion (31) which is provided in the second grasping member, which is connected to an ultrasonic transducer to generate ultrasonic vibration, and which has a grasping surface (126, 136) to be in contact with a living tissue (S) grasped between the first grasping member and the second grasping member; a first high-frequency electrode portion (124, 137) provided in the first grasping member; and a second high-frequency electrode portion (127, 137) provided in the first grasping member to be independent of the first high-frequency electrode portion, wherein the surgical instrument can cut the living tissue grasped between the first grasping member and the second grasping member by the ultrasonic vibration from the grasping surface of the ultrasonic vibrating portion, and can further coagulate the cut portion of the living tissue by the high-frequency current between the first high-frequency electrode portion and the second high-frequency electrode portion, the surgical instrument being **characterized in that:**

a pressing portion (122, 133) is further provided in the first grasping member (121, 131), the pressing portion being in contact with the living tissue (S) grasped between the first grasping member and the second grasping member (125, 135), and pressing the living tissue in cooperation with the grasping surface (126, 136) of the ultrasonic vibrating portion (31);  
 the first high-frequency electrode portion (124, 137) includes at least one electrode which is arranged in one side of the pressing portion (122, 133) in the first grasping member (121, 131);  
 the second high-frequency electrode portion (127, 137) includes at least one electrode which

is arranged in the other side of the pressing portion (122, 133) in the first grasping member (121, 131); and

the at least one electrode of the first high-frequency electrode portion (124, 137) and the at least one electrode of the second high-frequency electrode portion (127, 137) cooperate with each other in the both sides of the pressing portion (122, 133) to press the living tissue (S) grasped between the first grasping member (121, 131) and the second grasping member (125, 135) while the living tissue (S) is pressed by the pressing portion of the first grasping member and the grasping surface (126, 136) of the ultrasonic vibrating portion (31).

16. The surgical instrument according to claim 15, **characterized in that**

the grasping surface (126) of the ultrasonic vibrating portion (31) and parts of the second grasping member (125) corresponding to the first and second high-frequency electrode portions (124, 127) of the first grasping member (121) configure a continuously curved surface in a cross section which crosses a longitudinal center line of the second grasping member, and

a part of the pressing portion (122) corresponding to the grasping surface (126) of the ultrasonic vibrating portion (31) and the first and second high-frequency electrode portions (124, 127) configure a continuously curved surface in a cross section which crosses the longitudinal center line of the second grasping member (125), the continuously curved surface in the cross section of the part of the pressing portion and the first and second high-frequency electrode portions following the continuously curved surface in the cross section of the grasping surface of the ultrasonic vibrating portion and the parts of the second grasping member.

17. The surgical instrument according to claim 15, **characterized in that**

a distance from a longitudinal center line (31a) of the second grasping member (135) to the grasping surface (136) of the ultrasonic vibrating portion (31) provided in the second grasping member and a distance from the longitudinal center line of the second grasping member to each of the parts of the second grasping member corresponding to the first and second high-frequency electrode portions (137, 137) of the first grasping member (131) are different from each other.

18. The surgical instrument according to claim 17, **characterized in that**

the grasping surface (136) of the ultrasonic vibrating portion (31) provided in the second grasping member (135) and the parts of the second grasping member

corresponding to the first and second high-frequency electrode portions (137, 137) of the first grasping member (131) configure two inclined surfaces (134, 134) in a cross section which crosses the longitudinal center line (31a) of the second grasping member (135), the two inclined surfaces (134, 134) inclining from a center of the grasping surface (136) in one direction along the opening and closing direction of the first and second grasping members; and the pressing portion (133) provided in the first grasping member (131) and the first and second high-frequency electrode portions (137, 137) of the first grasping member are inclined in both sides of a center of the pressing portion, the center corresponding to the center of the grasping surface (136), to follow the two inclined surfaces.

**19. The surgical instrument according to claim 18, characterized in that**

the distance from the longitudinal center line (31a) of the second grasping member (135) to the grasping surface (136) of the ultrasonic vibrating portion (31) provided in the second grasping member is longer than the distance from the longitudinal center line (31a) of the second grasping member (135) to each of the parts of the second grasping member corresponding to the first and second high-frequency electrode portions (137, 137) of the first grasping member (131).

**20. The surgical instrument according to claim 19, characterized in that**

the pressing portion (133) provided in the first grasping member (131) and the first and second high-frequency electrode portions (137, 137) of the first grasping member (131) are divided into two at the center of the pressing portion (133) corresponding to the center of the grasping surface (136).

5

10

15

20

25

30

35

40

45

50

55

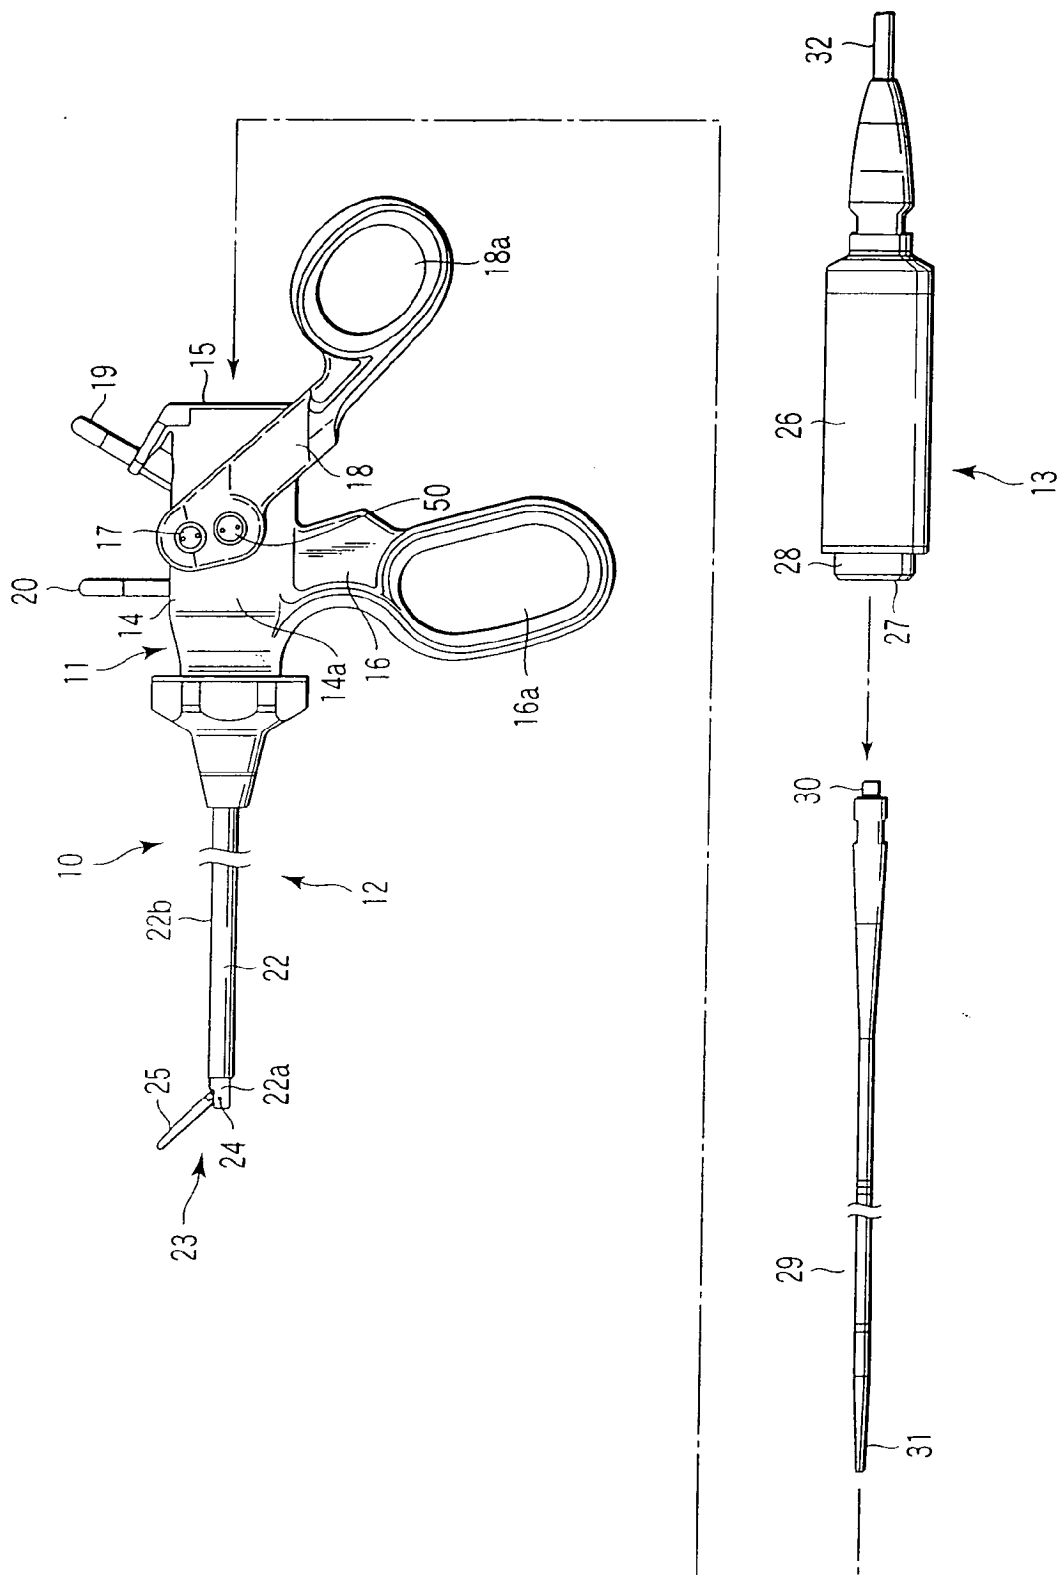


FIG. 1


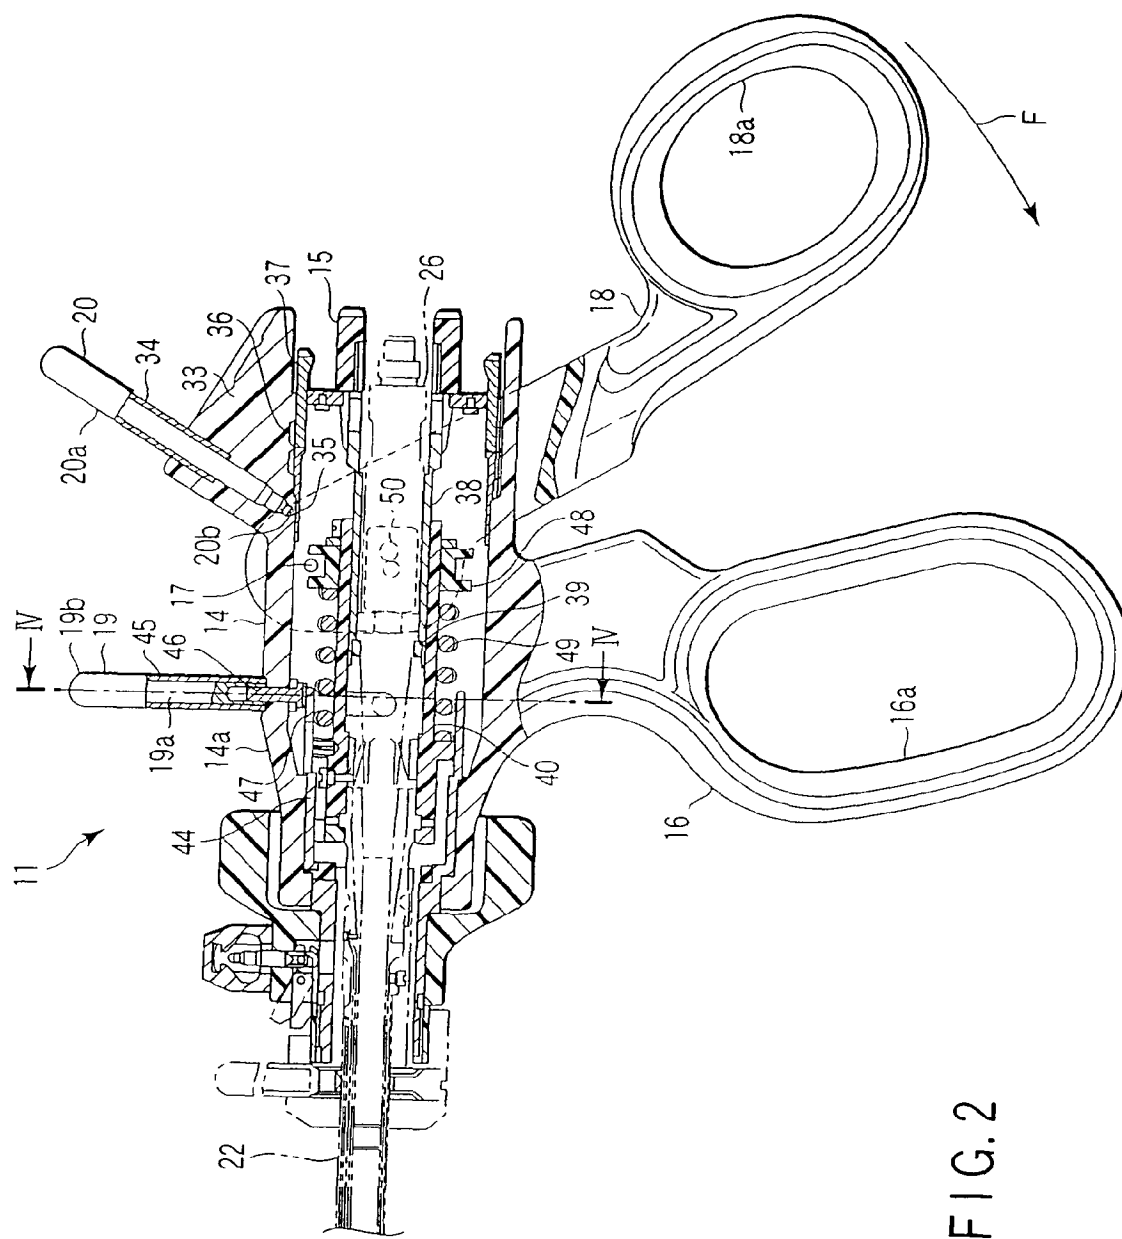


FIG. 2

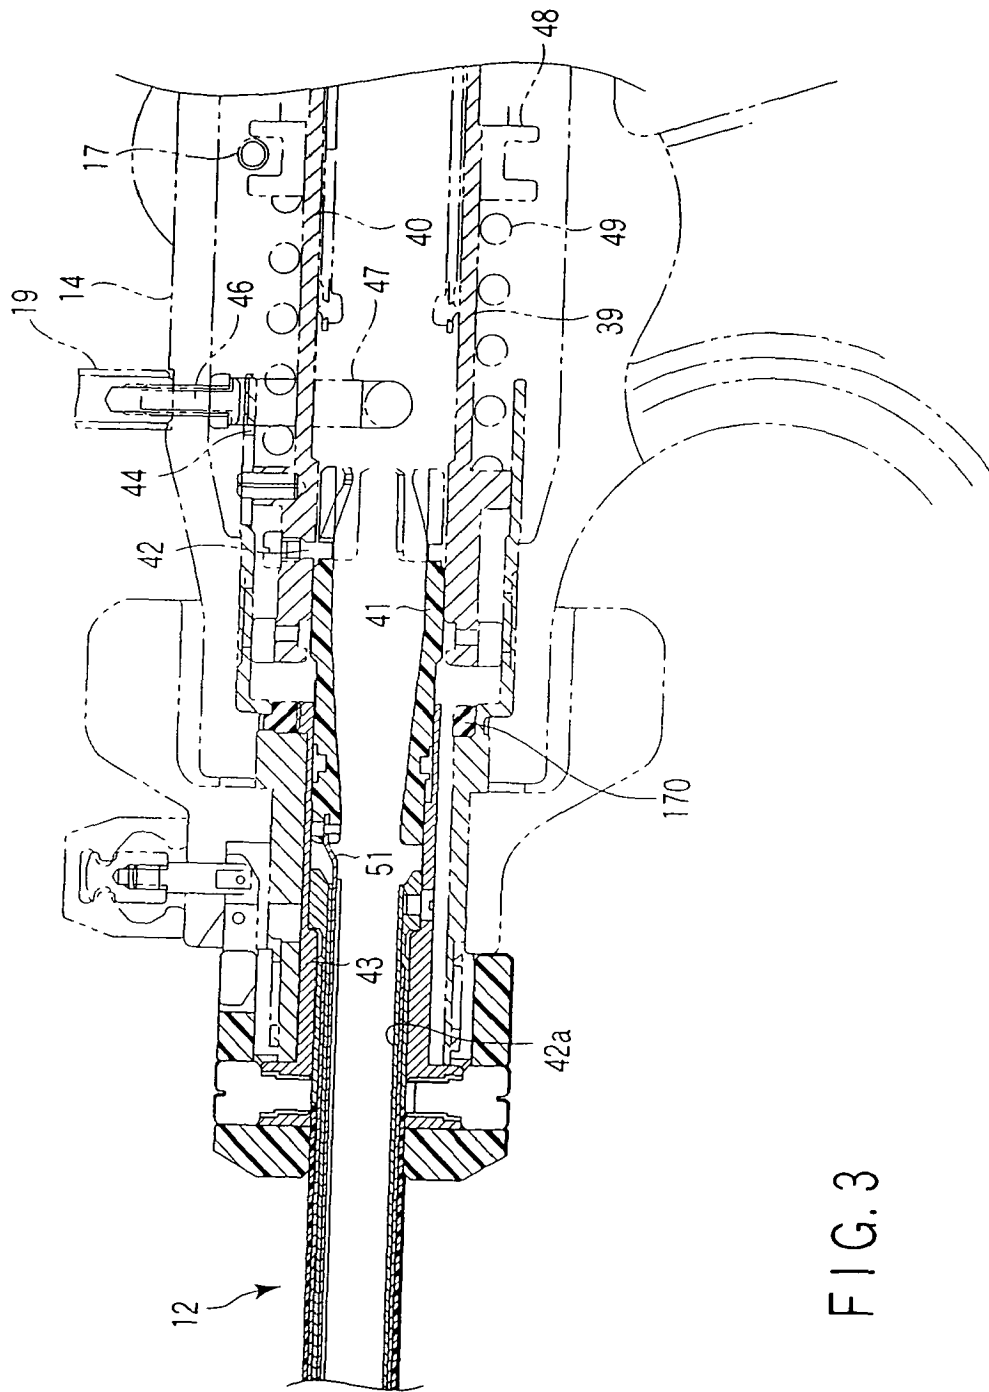

F1G.3

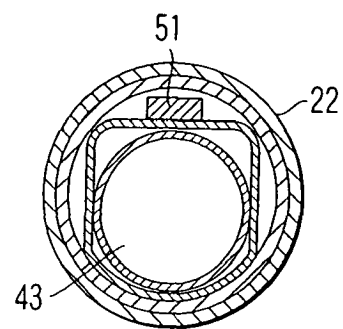


FIG. 6A

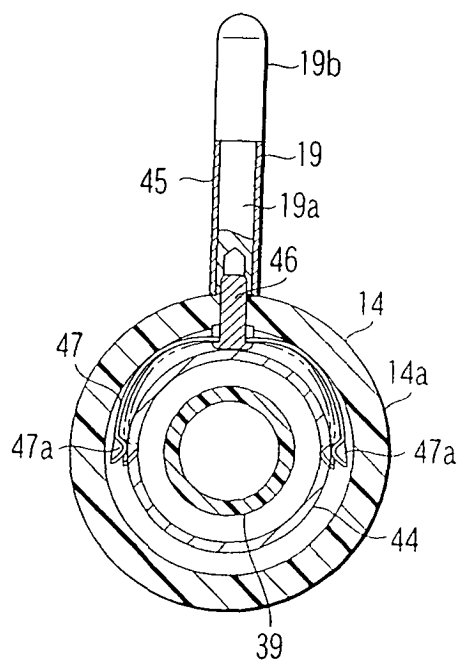


FIG. 4

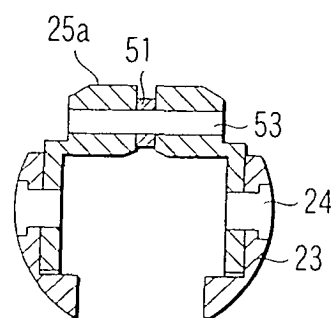


FIG. 6B

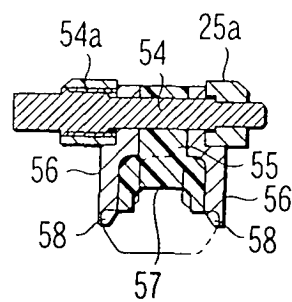


FIG. 6C

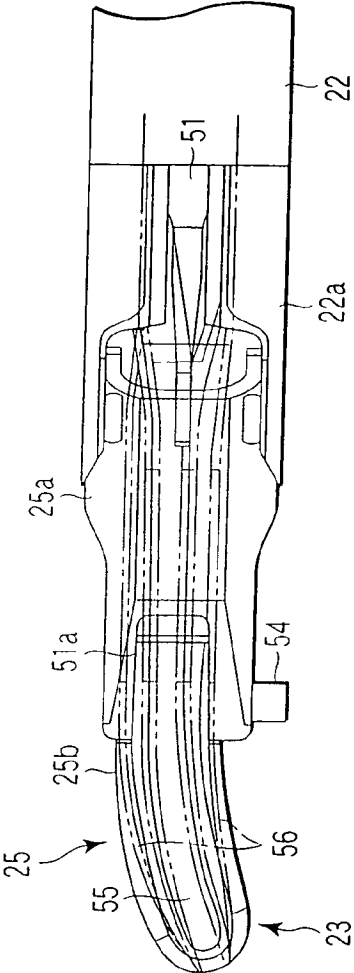


FIG. 5A

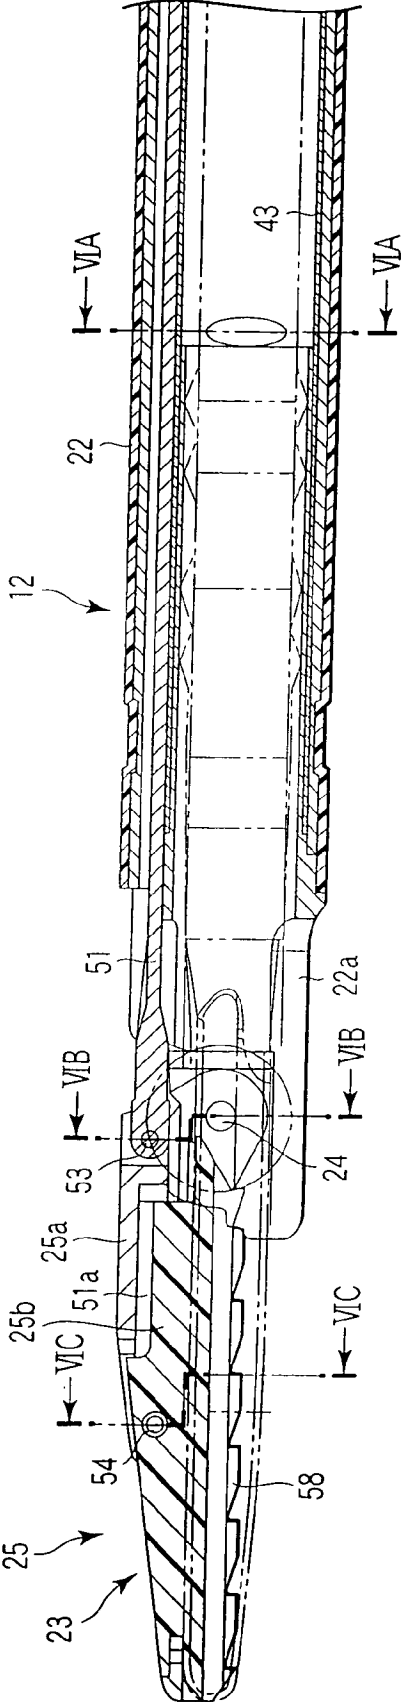


FIG. 5B

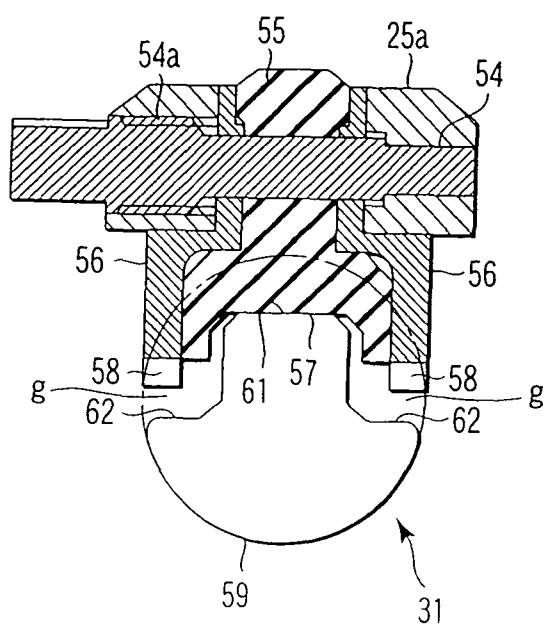


FIG. 7

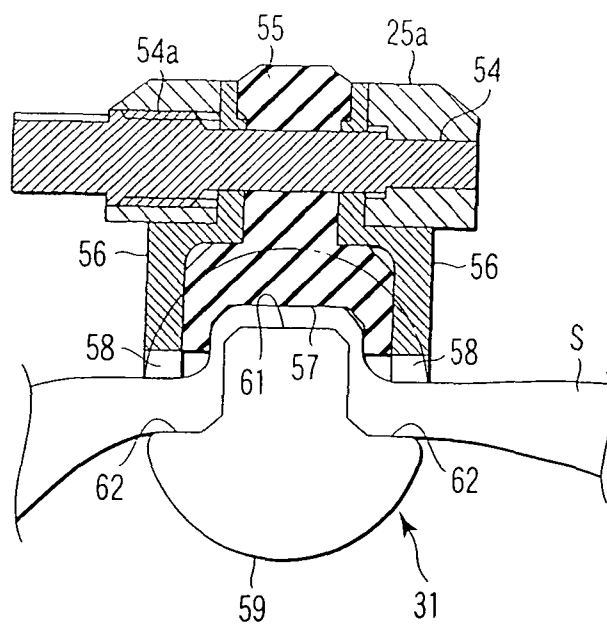


FIG. 8



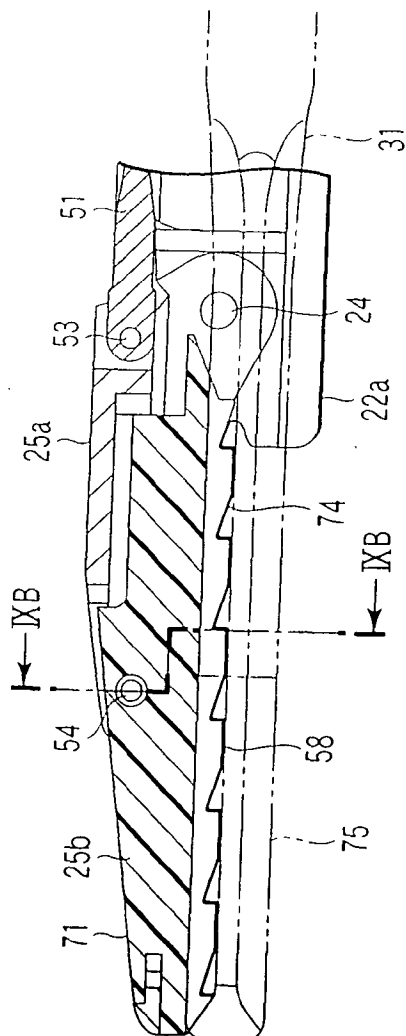


FIG. 9A

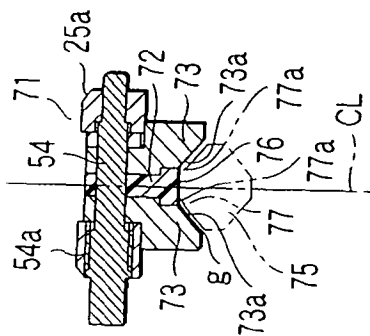


FIG. 9B

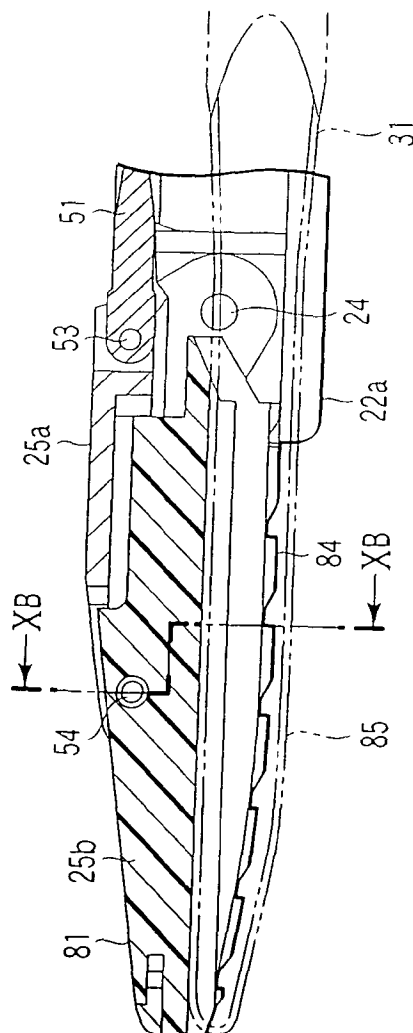


FIG. 10A

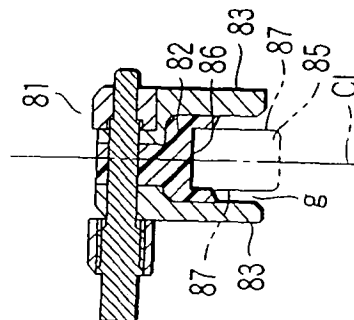


FIG. 10B

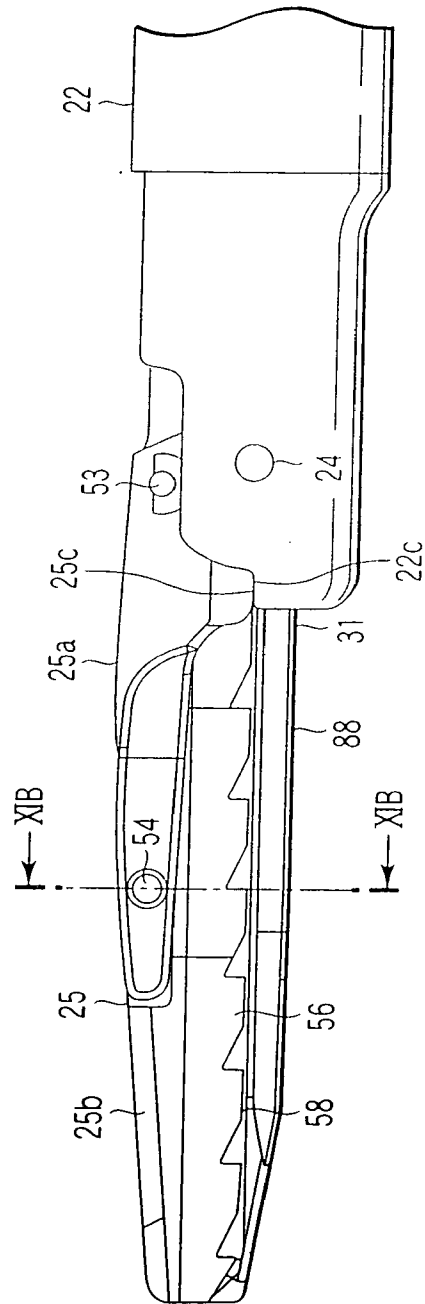


FIG. 11A

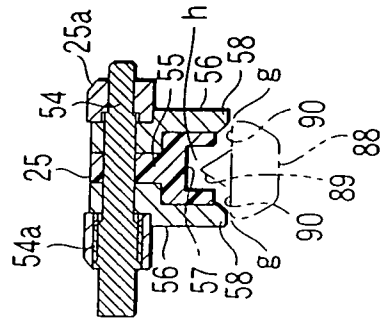


FIG. 11B

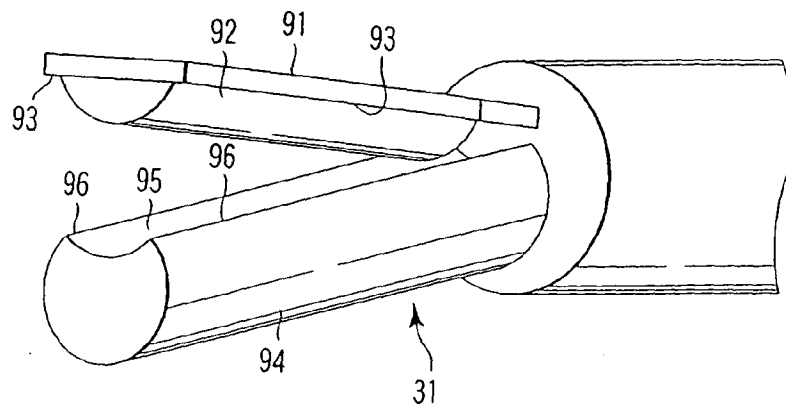


FIG. 12A

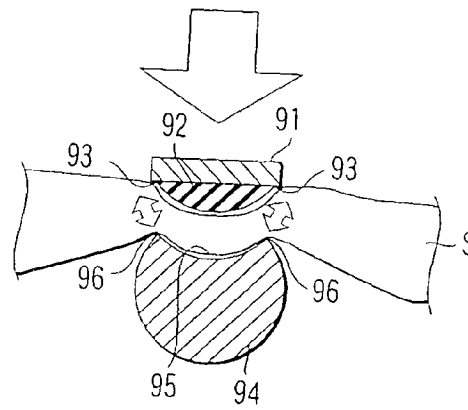


FIG. 12B

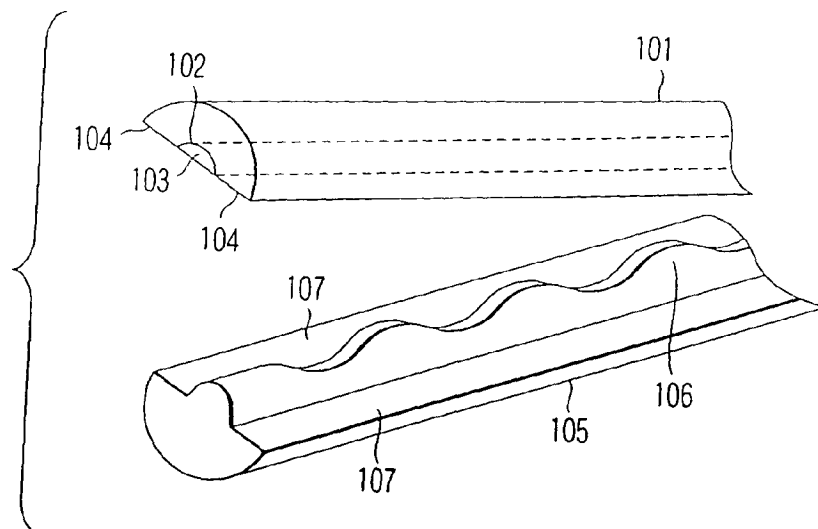
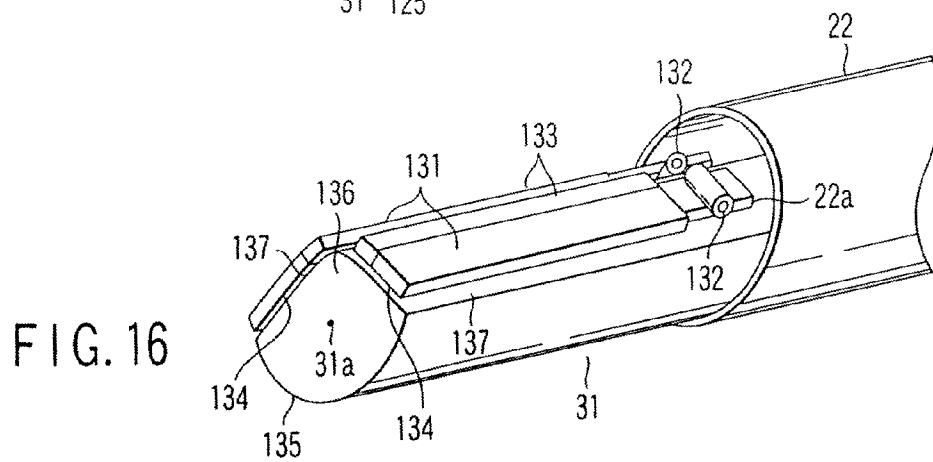
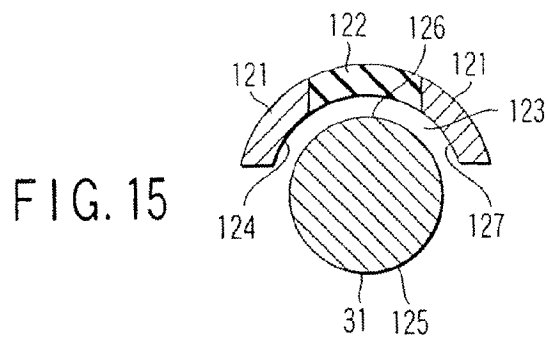
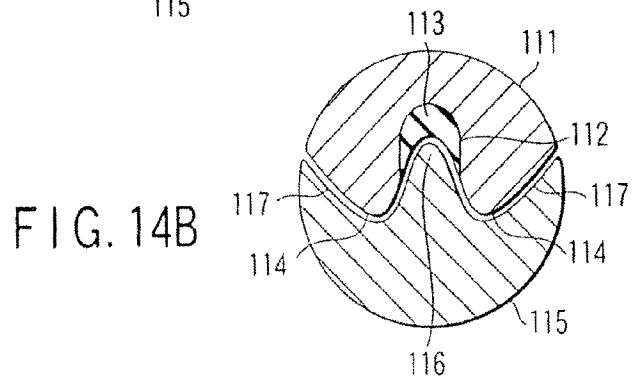
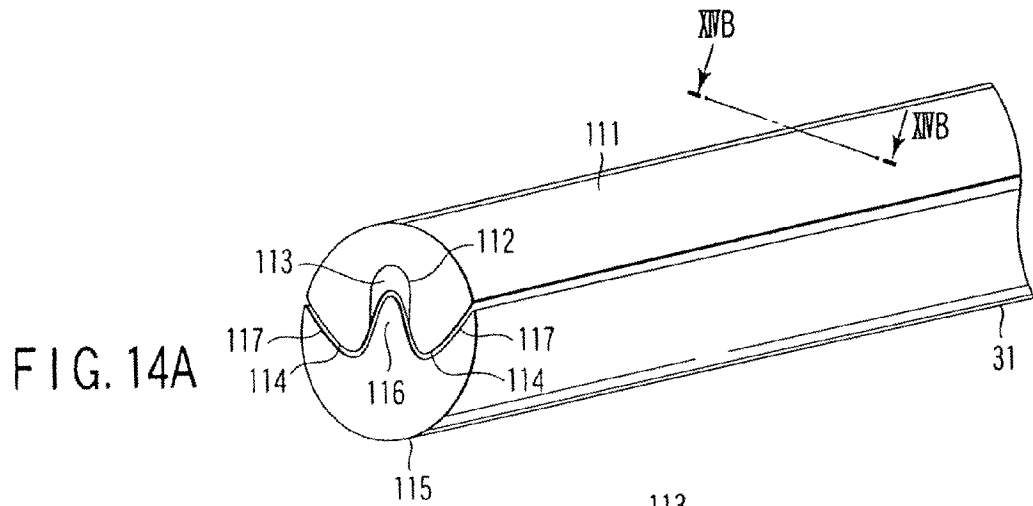


FIG. 13



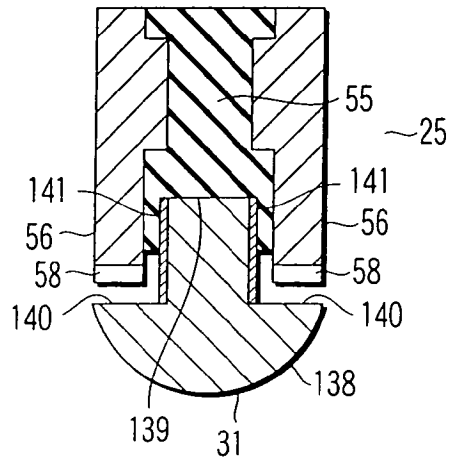


FIG. 17

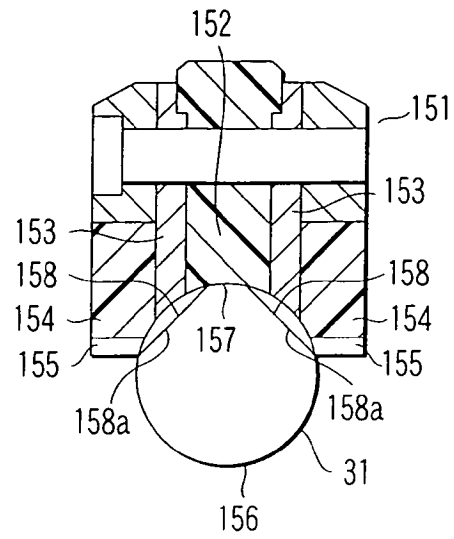


FIG. 18

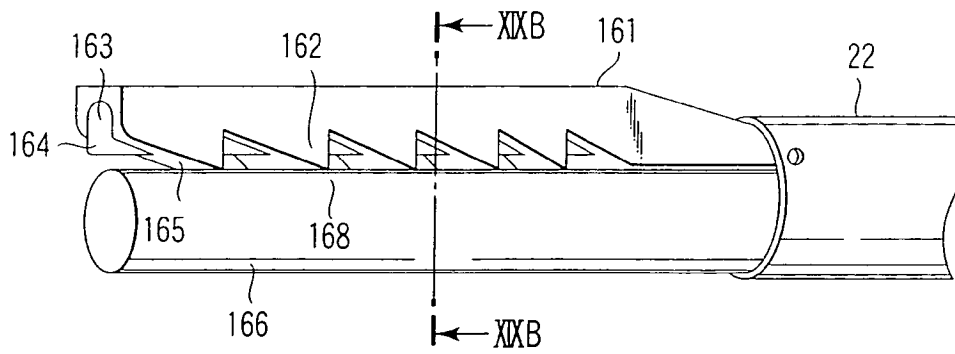


FIG. 19A

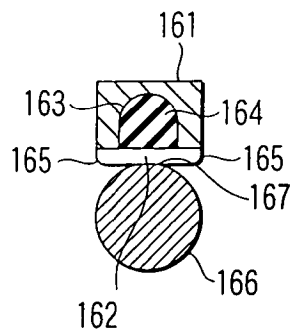


FIG. 19B



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 07 01 2598

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	WO 2005/122918 A (OLYMPUS CORP [JP]; MASUDA SHINYA [JP]; SHIMIZU KO [JP]; KIMURA KENICHI) 29 December 2005 (2005-12-29) * figures 13-20C *	1,2,5,9,14,15	INV. A61B18/14
Y		3	ADD. A61B17/32 A61B18/00
A		4,6-8,10-13,16-20	
	-& US 2006/259054 A1 (MASUDA SHINYA [JP] ET AL) 16 November 2006 (2006-11-16) * paragraphs [0052] - [0058], [0082] - [0097]; figures 13-20C *		
Y	US 2005/159745 A1 (TRUCKAI CSABA [US] ET AL) 21 July 2005 (2005-07-21) * paragraphs [0061], [0062], [0083], [0085]; figures 8,9,20 *	3	
A		1,2,4-20	
A	US 6 056 735 A (OKADA MITSUMASA [JP] ET AL) 2 May 2000 (2000-05-02) * column 35, line 8 - column 39, line 63; figures 53-62 *	1-20	TECHNICAL FIELDS SEARCHED (IPC) A61B
A	US 6 113 598 A (BAKER JAMES A [US]) 5 September 2000 (2000-09-05) * column 12, line 51 - column 14, line 66; figures 10-14C *	1-20	
A	US 6 083 223 A (BAKER JAMES A [US]) 4 July 2000 (2000-07-04) * abstract * * column 5, lines 46-67; figures 2-4C *	1-20	
P,L,X	JP 2007 050181 A (OLYMPUS MEDICAL SYSTEMS CORP) 1 March 2007 (2007-03-01) * figures 1-12 *	1-20	
	-/--		
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 31 October 2007	Examiner Fischer, Olivier
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

2

EPO FORM 1503 03/02 (P04C01)



European Patent  
Office

# EUROPEAN SEARCH REPORT

Application Number  
EP 07 01 2598

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
	-& US 2007/043297 A1 (MIYAZAWA TARO [JP]) 22 February 2007 (2007-02-22) -----		
			TECHNICAL FIELDS SEARCHED (IPC)
The present search report has been drawn up for all claims			
Place of search <b>Munich</b>		Date of completion of the search <b>31 October 2007</b>	Examiner <b>Fischer, Olivier</b>
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

2  
EPO FORM 1503 03/02 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT  
ON EUROPEAN PATENT APPLICATION NO.**

EP 07 01 2598

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.  
The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

31-10-2007

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 2005122918 A	29-12-2005	EP 1757242 A1 US 2006259054 A1	28-02-2007 16-11-2006
US 2006259054 A1	16-11-2006	EP 1757242 A1 WO 2005122918 A1	28-02-2007 29-12-2005
US 2005159745 A1	21-07-2005	NONE	
US 6056735 A	02-05-2000	NONE	
US 6113598 A	05-09-2000	NONE	
US 6083223 A	04-07-2000	NONE	
JP 2007050181 A	01-03-2007	US 2007043297 A1	22-02-2007
US 2007043297 A1	22-02-2007	JP 2007050181 A	01-03-2007



**REFERENCES CITED IN THE DESCRIPTION**

*This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.*

**Patent documents cited in the description**

- JP 2003079633 A [0003] [0004]
- JP 2004012987 A [0003]
- JP 2004216180 A [0003] [0005]
- JP 2004129870 A [0005]

专利名称(译)	手术器械		
公开(公告)号	<a href="#">EP1875875A1</a>	公开(公告)日	2008-01-09
申请号	EP2007012598	申请日	2007-06-27
[标]申请(专利权)人(译)	奥林巴斯医疗株式会社		
申请(专利权)人(译)	奥林巴斯医疗系统股份有限公司.		
当前申请(专利权)人(译)	奥林巴斯医疗系统股份有限公司.		
[标]发明人	MASUDA SHINYA MIYAZAWA TARO OKABE HIROSHI TANIGUCHI KAZUNORI		
发明人	MASUDA, SHINYA MIYAZAWA, TARO OKABE, HIROSHI TANIGUCHI, KAZUNORI		
IPC分类号	A61B18/14 A61B17/32 A61B18/00 A61N1/32		
CPC分类号	A61B17/320092 A61B18/1445 A61B2017/320093 A61B2017/320095 A61B2018/0019 A61B2018/00589 A61B2018/146 A61N1/328 A61N7/02		
优先权	2006184663 2006-07-04 JP		
其他公开文献	EP1875875B1		
外部链接	<a href="#">Espacenet</a>		

#### 摘要(译)

手术器械能够通过第一和第二抓握构件 ( 25,59 ) 抓住活组织 ( S ) , 能够通过超声波振动从第二构件中的超声波振动部分 ( 31 ) 的抓握表面 ( 61 ) 切割被抓取的组织并且, 可以通过第一和第二构件中的第一和第二电极部分之间的高频电流来凝结组织的切割部分。按压部分 ( 55 ) 设置在第一构件中以与抓握的组织接触并且与振动部分的抓握表面协作地按压组织。第一和第二电极部分中的每一个包括位于按压部分两侧的电极。当组织被第一构件的按压部分和振动部分的抓握表面按压时, 第一和第二电极部分的电极配合以按压被抓住的组织。

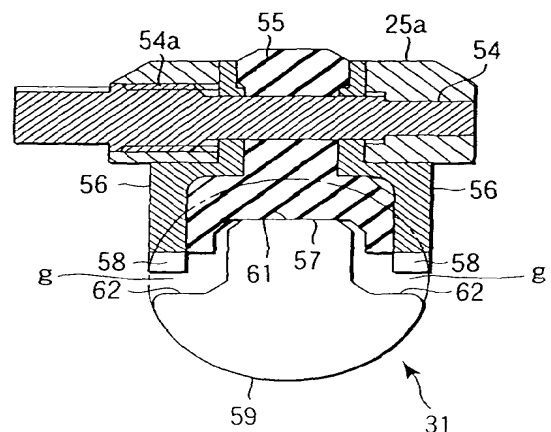


FIG. 7