



(11) **EP 3 162 318 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention
of the grant of the patent:
16.10.2019 Bulletin 2019/42

(51) Int Cl.:
A61B 90/00 ^(2016.01) **A61B 18/14** ^(2006.01)
G06F 3/01 ^(2006.01)

(21) Application number: **16195634.7**

(22) Date of filing: **19.10.2006**

(54) **AUXILIARY IMAGE DISPLAY AND MANIPULATION ON A COMPUTER DISPLAY IN A MEDICAL ROBOTIC SYSTEM**

HILFSBILDANZEIGE UND -MANIPULATION AUF EINER COMPUTERANZEIGE IN EINEM
MEDIZINISCHEN ROBOTISCHEN SYSTEM

MANIPULATION ET AFFICHAGE D'IMAGE AUXILIAIRE SUR UN ÉCRAN D'ORDINATEUR DANS
UN SYSTÈME ROBOTIQUE MÉDICAL

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI
SK TR**

(30) Priority: **20.10.2005 US 728450 P**

(43) Date of publication of application:
03.05.2017 Bulletin 2017/18

(62) Document number(s) of the earlier application(s) in
accordance with Art. 76 EPC:
06817132.1 / 1 937 176

(73) Proprietor: **Intuitive Surgical Operations, Inc.**
Sunnyvale, CA 94086 (US)

(72) Inventors:
• **HOFFMAN, Brian**
Sunnyvale, CA 94087 (US)

- **KUMAR, Rajesh**
Santa Clara, CA 94051 (US)
- **LARKIN, David**
Menlo Park, CA 94025 (US)
- **PRISCO, Giuseppe**
Mountain View, CA 94043 (US)
- **SWARUP, Nitish**
Sunnyvale, CA 94085 (US)
- **ZHANG, Guanghai G**
San Jose, CA 95129 (US)

(74) Representative: **MacDougall, Alan John Shaw et al**
Mathys & Squire LLP
The Shard
32 London Bridge Street
London SE1 9SG (GB)

(56) References cited:
WO-A1-2007/030173 US-A1- 2004 106 916
US-B1- 6 522 906

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

FIELD OF THE INVENTION

[0001] The present invention generally relates to medical robotic systems and in particular, to the displaying and manipulating of auxiliary images on a computer display in a medical robotic system.

BACKGROUND OF THE INVENTION

[0002] Medical robotic systems such as those used in performing minimally invasive surgical procedures offer many benefits over traditional open surgery techniques, including less pain, shorter hospital stays, quicker return to normal activities, minimal scarring, reduced recovery time, and less injury to tissue. Consequently, demand for minimally invasive surgery using medical robotic systems is strong and growing.

[0003] One example of a medical robotic system is the daVinci® Surgical System from Intuitive Surgical, Inc., of Sunnyvale, California. The daVinci® system includes a surgeon's console, a patient-side cart, a high performance 3-D vision system, and Intuitive Surgical's proprietary EndoWrist™ articulating instruments, which are modeled after the human wrist so that when added to the motions of the robotic arm assembly holding the surgical instrument, they allow at least a full six degrees of freedom of motion, which is comparable to the natural motions of open surgery.

[0004] The daVinci® surgeon's console has a high-resolution stereoscopic video display with two progressive scan cathode ray tubes ("CRTs"). The system offers higher fidelity than polarization, shutter eyeglass, or other techniques. Each eye views a separate CRT presenting the left or right eye perspective, through an objective lens and a series of mirrors. The surgeon sits comfortably and looks into this display throughout surgery, making it an ideal place for the surgeon to display and manipulate 3-D intra-operative imagery.

[0005] In addition to primary imagery being displayed on the display screen, it is also desirable at times to be able to concurrently view auxiliary information to gain better insight or to otherwise assist in the medical procedure being performed. The auxiliary information may be provided in various modes such as text information, bar graphs, two-dimensional picture-in-picture images, and two-dimensional or three-dimensional images that are registered and properly overlaid with respect to their primary image counterparts.

[0006] For auxiliary images, the images may be captured pre-operatively or intra-operatively using techniques such as ultrasonography, magnetic resonance imaging, computed axial tomography, and fluoroscopy to provide internal details of an anatomic structure being treated. This information may then be used to supplement external views of the anatomic structure such as captured by a locally placed camera.

[0007] Although there are a plethora of auxiliary information sources as well as manners of displaying that information, improvements in the display and manipulation of auxiliary images is still useful to better assist surgeons in performing medical procedures with medical robotic systems.

[0008] US 2004/106916 A1 describes a computer-assisted surgery system and method, for use during a medical procedure, which comprises: application logic operatively associated with said computer-assisted surgery system and operable to: receive information on an object of interest; track the position of a tool; determine a scalar distance between a current position of said tool and said object of interest; and provide an indication of said scalar distance to a user of said tool.

[0009] US 6,522,906 B1 describes systems and methods for performing robotically-assisted surgical procedures on a patient, which enable an image display device to provide an operator with auxiliary information related to the surgical procedure, in addition to providing an image of the surgical site itself. The systems and methods allow an operator to selectively access and reference auxiliary information on the image display device during the performance of a surgical procedure.

SUMMARY

[0010] The invention is defined by the appended claims.

[0011] Also herein described is a method for displaying auxiliary information including the effect of a therapeutic procedure as an overlay to or otherwise associated with an image of an anatomic structure being treated at the time by the procedure.

[0012] Also herein described is a method for displaying a user selected portion at a user specified magnification factor of a volume rendering of an auxiliary image of an anatomic structure as a registered overlay to a primary image of the anatomic structure on a computer display screen.

[0013] Also herein described is a medical robotic system having a master input device that may be used to manually register images in a three-dimensional space of a computer display.

[0014] Also herein described is a medical robotic system having a master input device that may be used to define cut-planes of a volume rendering of an anatomic structure in a three-dimensional space of a computer display.

[0015] Also herein described is a medical robotic system having a master input device that may be used to selectively modify portions or details of a volume rendering of an anatomic structure in a three-dimensional space of a computer display.

[0016] Also herein described is a medical robotic system having a master input device that may be used to vary display parameters for a rendering of an anatomic structure being displayed on a computer display screen.

[0017] Also herein described is a medical robotic system having a master input device that may be switched between an image capturing mode wherein the master input device controls movement of an image capturing device, and an image manipulating mode wherein the master input device controls display and manipulation of images captured by the image capturing device on a computer display screen.

[0018] Also herein described is a method for displaying a selected portion of an auxiliary image of an anatomic structure as an overlay to a primary image of the anatomic structure on a computer display screen, comprising: associating a movable window with a pointing device such that the movable window is positionable on the computer display screen using the pointing device; registering an auxiliary image of an anatomic structure with a primary image of the anatomic structure so as to be at a same position and orientation in a common reference frame; and displaying the primary image on the computer display screen, and a portion of the registered auxiliary image corresponding to the same screen coordinates as the movable window as an overlay to the primary image in the movable window.

[0019] Also herein described is a medical robotic system comprising: an image capturing device for capturing images; a robotic arm holding the image capturing device; a computer display screen; a master input device adapted to be manipulatable by an user in multiple degrees-of-freedom movement; and a processor configured to control movement of the image capturing device according to user manipulation of the master input device when the master input device is in an image capturing mode, and controlling the displaying of images derived from the captured images on the computer display screen according to user manipulation of the master input device when the master input device is in an image manipulating mode.

[0020] Features and advantages of the various aspects of the present invention will become apparent from the following description of its preferred embodiment, which description should be taken in conjunction with the accompanying drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0021]

FIG. 1 illustrates a top view of an operating room employing a medical robotic system utilizing aspects of the present invention.

FIG. 2 illustrates a block diagram of a medical robotic system utilizing aspects of the present invention.

FIG. 3 illustrates a laparoscopic ultrasound probe useful for a medical robotic system utilizing aspects of the present invention.

FIG. 4 illustrates a flow diagram of a method for displaying on a computer display screen an effect of a therapeutic procedure being applied by a therapeutic instrument to an anatomic structure, utilizing aspects of the present invention.

FIG. 5 illustrates an external view of an anatomic structure with a therapeutic instrument inserted in the anatomic structure for performing a therapeutic procedure.

FIG. 6 illustrates an internal view of an anatomic structure with a discernable therapeutic effect shown as captured by a therapy sensing device.

FIG. 7 illustrates a computer display screen displaying an effect of a therapeutic procedure registered to an anatomic structure being treated by the procedure, as generated by a method utilizing aspects of the present invention.

FIG. 8 illustrates a flow diagram of a method for displaying a selected portion of an auxiliary image of an anatomic structure in a user movable magnifying glass on a computer display screen, utilizing aspects of the present invention.

FIG. 9 illustrates a flow diagram of a method for displaying a manipulatable window of an internal view of an anatomic structure at a specified magnification factor, utilizing aspects of the present invention.

FIG. 10 illustrates an auxiliary image of an anatomic structure and concentric areas of the auxiliary image representing different magnification factors for display on a computer display screen in a magnifying glass by a method utilizing aspects of the present invention.

FIG. 11 illustrates a computer display screen with a primary image of an anatomic structure and an overlaid portion of an auxiliary image of the anatomic structure viewed in a magnifying glass lens as displayed by a method utilizing aspects of the present invention.

FIG. 12 illustrates a flow diagram of a method performed by a processor in a medical robotic system for manipulating objects displayed on a computer display screen utilizing aspects of the present invention.

DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT

[0022] **FIG. 1** illustrates, as an example, a top view of an operating room employing a medical robotic system. The medical robotic system in this case is a Minimally

Invasive Robotic Surgical ("MIRS") System 100 including a Console ("C") utilized by a Surgeon ("S") while performing a minimally invasive diagnostic or surgical procedure with assistance from one or more Assistants ("A") on a Patient ("P") who is reclining on an Operating table ("O").

[0023] The Console includes a Master Display 104 (also referred to herein as a "Display Screen" or "computer display screen") for displaying one or more images of a surgical site within the Patient as well as perhaps other information to the Surgeon. Also included are Master Input Devices 107, 108 (also referred to herein as "Master Manipulators"), one or more Foot Pedals 105, 106, a Microphone 103 for receiving voice commands from the Surgeon, and a Processor 102. The Master Input Devices 107, 108 may include any one or more of a variety of input devices such as joysticks, gloves, trigger-guns, hand-operated controllers, grippers, or the like. The Processor 102 is preferably a personal computer that may be integrated into the Console or otherwise connected to it in a conventional manner.

[0024] The Surgeon performs a medical procedure using the MIRS System 100 by manipulating the Master Input Devices 107, 108 so that the Processor 102 causes their respectively associated Slave Arms 121, 122 to manipulate their respective removably coupled and held Surgical Instruments 138, 139 (also referred to herein as "Tools") accordingly, while the Surgeon views three-dimensional ("3D") images of the surgical site on the Master Display 104.

[0025] The Tools 138, 139 are preferably Intuitive Surgical's proprietary EndoWrist™ articulating instruments, which are modeled after the human wrist so that when added to the motions of the robot arm holding the tool, they allow at least a full six degrees of freedom of motion, which is comparable to the natural motions of open surgery. Additional details on such tools may be found in commonly owned U.S. Pat. No. 5,797,900 entitled "Wrist Mechanism for Surgical Instrument for Performing Minimally Invasive Surgery with Enhanced Dexterity and Sensitivity". At the operating end of each of the Tools 138, 139 is a manipulatable end effector such as a clamp, grasper, scissor, stapler, blade, needle, needle holder, or energizable probe.

[0026] The Master Display 104 has a high-resolution stereoscopic video display with two progressive scan cathode ray tubes ("CRTs"). The system offers higher fidelity than polarization, shutter eyeglass, or other techniques. Each eye views a separate CRT presenting the left or right eye perspective, through an objective lens and a series of mirrors. The Surgeon sits comfortably and looks into this display throughout surgery, making it an ideal place for the Surgeon to display and manipulate 3-D intra-operative imagery.

[0027] A Stereoscopic Endoscope 140 provides right and left camera views to the Processor 102 so that it may process the information according to programmed instructions and cause it to be displayed on the Master Display 104. A Laparoscopic Ultrasound ("LUS") Probe

150 provides two-dimensional ("2D") ultrasound image slices of an anatomic structure to the Processor 102 so that the Processor 102 may generate a 3D ultrasound computer model or volume rendering of the anatomic structure.

[0028] Each of the Tools 138, 139, as well as the Endoscope 140 and LUS Probe 150, is preferably inserted through a cannula or trocar (not shown) or other tool guide into the Patient so as to extend down to the surgical site through a corresponding minimally invasive incision such as Incision 161. Each of the Slave Arms 121-124 includes a slave manipulator and setup arms. The slave manipulators are robotically moved using motor controlled joints (also referred to as "active joints") in order to manipulate and/or move their respectively held Tools. The setup arms are manually manipulated by releasing normally braked joints (also referred to as "setup joints") to horizontally and vertically position the Slave Arms 121-124 so that their respective Tools may be inserted into the cannulae.

[0029] The number of surgical tools used at one time and consequently, the number of slave arms being used in the System 100 will generally depend on the medical procedure to be performed and the space constraints within the operating room, among other factors. If it is necessary to change one or more of the tools being used during a procedure, the Assistant may remove the tool no longer being used from its slave arm, and replace it with another tool, such as Tool 131, from a Tray ("T") in the Operating Room.

[0030] Preferably, the Master Display 104 is positioned near the Surgeon's hands so that it will display a projected image that is oriented so that the Surgeon feels that he or she is actually looking directly down onto the surgical site. To that end, an image of the Tools 138, 139 preferably appear to be located substantially where the Surgeon's hands are located even though the observation points (i.e., that of the Endoscope 140 and LUS Probe 150) may not be from the point of view of the image.

[0031] In addition, the real-time image is preferably projected into a perspective image such that the Surgeon can manipulate the end effector of a Tool, 138 or 139, through its associated Master Input Device, 107 or 108, as if viewing the workspace in substantially true presence. By true presence, it is meant that the presentation of an image is a true perspective image simulating the viewpoint of an operator that is physically manipulating the Tools. Thus, the Processor 102 transforms the coordinates of the Tools to a perceived position so that the perspective image is the image that one would see if the Endoscope 140 was looking directly at the Tools from a Surgeon's eye-level during an open cavity procedure.

[0032] The Processor 102 performs various functions in the System 100. One important function that it performs is to translate and transfer the mechanical motion of Master Input Devices 107, 108 to their associated Slave Arms 121, 122 through control signals over Bus 110 so that the Surgeon can effectively manipulate their respective

Tools **138, 139**. Another important function is to implement the various methods described herein in reference to **FIGS. 4-12**.

[0033] Although described as a processor, it is to be appreciated that the Processor **102** may be implemented in practice by any combination of hardware, software and firmware. Also, its functions as described herein may be performed by one unit, or divided up among different components, each of which may be implemented in turn by any combination of hardware, software and firmware. When divided up among different components, the components may be centralized in one location or distributed across the System **100** for distributed processing purposes.

[0034] Prior to performing a medical procedure, ultrasound images captured by the LUS Probe **150**, right and left 2D camera images captured by the stereoscopic Endoscope **140**, and end effector positions and orientations as determined using kinematics of the Slave Arms **121-124** and their sensed joint positions, are calibrated and registered with each other.

[0035] Slave Arms **123, 124** may manipulate the Endoscope **140** and LUS Probe **150** in similar manners as Slave Arms **121, 122** manipulate Tools **138, 139**. When there are only two master input devices in the system, however, such as Master Input Devices **107, 108** in the System **100**, in order for the Surgeon to manually control movement of either the Endoscope **140** or LUS Probe **150**, it may be required to temporarily associate one of the Master Input Devices **107, 108** with the Endoscope **140** or the LUS Probe **150** that the Surgeon desires manual control over, while its previously associated Tool and Slave Manipulator are locked in position.

[0036] Although not shown in this example, other sources of primary and auxiliary images of anatomic structures may be included in the System **100**, such as those commonly used for capturing ultrasound, magnetic resonance, computed axial tomography, and fluoroscopic images. Each of these sources of imagery may be used pre-operatively, and where appropriate and practical, intra-operatively.

[0037] **FIG. 2** illustrates, as an example, a block diagram of the System **100**. In this system, there are two Master Input Devices **107, 108**. Master Input Device **107** controls movement of either a Tool **138** or a stereoscopic Endoscope **140**, depending upon which mode its Control Switch Mechanism **211** is in, and Master Input Device **108** controls movement of either a Tool **139** or a LUS Probe **150**, depending upon which mode its Control Switch Mechanism **231** is in.

[0038] The Control Switch Mechanisms **211** and **231** may be placed in either a first or second mode by a Surgeon using voice commands, switches physically placed on or near the Master Input Devices **107, 108**, Foot Pedals **105, 106** on the Console, or Surgeon selection of appropriate icons or other graphical user interface selection means displayed on the Master Display **104** or an auxiliary display (not shown).

[0039] When Control Switch Mechanism **211** is placed in the first mode, it causes Master Controller **202** to communicate with Slave Controller **203** so that manipulation of the Master Input **107** by the Surgeon results in corresponding movement of Tool **138** by Slave Arm **121**, while the Endoscope **140** is locked in position. On the other hand, when Control Switch Mechanism **211** is placed in the second mode, it causes Master Controller **202** to communicate with Slave Controller **233** so that manipulation of the Master Input **107** by the Surgeon results in corresponding movement of Endoscope **140** by Slave Arm **123**, while the Tool **138** is locked in position.

[0040] Similarly, when Control Switch Mechanism **231** is placed in the first mode, it causes Master Controller **108** to communicate with Slave Controller **223** so that manipulation of the Master Input **108** by the Surgeon results in corresponding movement of Tool **139** by Slave Arm **122**. In this case, however, the LUS Probe **150** is not necessarily locked in position. Its movement may be guided by an Auxiliary Controller **242** according to stored instructions in Memory **240**. The Auxiliary Controller **242** also provides haptic feedback to the Surgeon through Master Input **108** that reflects readings of a LUS Probe Force Sensor **247**. On the other hand, when Control Switch Mechanism **231** is placed in the second mode, it causes Master Controller **108** to communicate with Slave Controller **243** so that manipulation of the Master Input **108** by the Surgeon results in corresponding movement of LUS Probe **150** by Slave Arm **124**, while the Tool **139** is locked in position.

[0041] Before a Control Switch Mechanism effects a switch back to its first or normal mode, its associated Master Input Device is preferably repositioned to where it was before the switch. Alternatively, the Master Input Device may remain in its current position and kinematic relationships between the Master Input Device and its associated Tool Slave Arm readjusted so that upon the Control Switch Mechanism switching back to its first or normal mode, abrupt movement of the Tool does not occur. For additional details on control switching, see, e.g., commonly owned U.S. Pat. No. 6,659,939 entitled "Co-operative Minimally Invasive Telesurgical System".

[0042] A third Control Switch Mechanism **241** is provided to allow the user to switch between an image capturing mode and an image manipulating mode while the Control Switch Mechanism **231** is in its second mode (i.e., associating the Master Input Device **108** with the LUS Probe **150**). In its first or normal mode (i.e., image capturing mode), the LUS Probe **150** is normally controlled by the Master Input Device **108** as described above. In its second mode (i.e., image manipulating mode), the LUS Probe **150** is not controlled by the Master Input Device **108**, leaving the Master Input Device **108** free to perform other tasks such as the displaying and manipulating of auxiliary images on the Display Screen **104** and in particular, for performing certain user specified functions as described herein. Note however that although the LUS Probe **150** may not be controlled by the Master

Input Device 108 in this second mode of the Control Switch Mechanism 241, it may still be automatically rocked or otherwise moved under the control of the Auxiliary Controller 242 according to stored instructions in Memory 240 so that a 3D volume rendering of a proximate anatomic structure may be generated from a series of 2D ultrasound image slices captured by the LUS Probe 150. For additional details on such and other programmed movement of the LUS Probe 150, see commonly owned U.S. patent Application Ser. No. 11/447,668 entitled "Laparoscopic Ultrasound Robotic Surgical System," filed June 6, 2006.

[0043] The Auxiliary Controller 242 also performs other functions related to the LUS Probe 150 and the Endoscope 140. It receives output from a LUS Probe Force Sensor 247, which senses forces being exerted against the LUS Probe 150, and feeds the force information back to the Master Input Device 108 through the Master Controller 222 so that the Surgeon may feel those forces even if he or she is not directly controlling movement of the LUS Probe 150 at the time. Thus, potential injury to the Patient is minimized since the Surgeon has the capability to immediately stop any movement of the LUS Probe 150 as well as the capability to take over manual control of its movement.

[0044] Another key function of the Auxiliary Control 242 is to cause processed information from the Endoscope 140 and the LUS Probe 150 to be displayed on the Master Display 104 according to user selected display options. Examples of such processing include generating a 3D ultrasound image from 2D ultrasound image slices received from the LUS Probe 150 through an Ultrasound Processor 246, causing either 3D or 2D ultrasound images corresponding to a selected position and orientation to be displayed in a picture-in-picture window of the Master Display 104, causing either 3D or 2D ultrasound images of an anatomic structure to overlay a camera captured image of the anatomic structure being displayed on the Master Display 104, and performing the methods described below in reference to FIGS. 4-12.

[0045] Although shown as separate entities, the Master Controllers 202, 222, Slave Controllers 203, 233, 223, 243, and Auxiliary Controller 242 are preferably implemented as software modules executed by the Processor 102, as well as certain mode switching aspects of the Control Switch Mechanisms 211, 231, 241. The Ultrasound Processor 246 and Video Processor 236, on the other hand, may be software modules or separate boards or cards that are inserted into appropriate slots coupled to or otherwise integrated with the Processor 102 to convert signals received from these image capturing devices into signals suitable for display on the Master Display 104 and/or for additional processing by the Auxiliary Controller 242 before being displayed on the Master Display 104.

[0046] Although the present example assumes that each Master Input Device is being shared by only one pre-assigned Tool Slave Robotic Arm and one pre-as-

signed Image Capturing Device Robotic Arm, alternative arrangements are also feasible and envisioned to be within the full scope of the present invention. For example, a different arrangement wherein each of the Master Input Devices may be selectively associated with any one of the Tool and Image Capturing Device Robotic Arms is also possible and even preferably for maximum flexibility. Also, although the Endoscope Robotic Arm is shown in this example as being controlled by a single Master Input Device, it may also be controlled using both Master Input Devices to give the sensation of being able to "grab the image" and move it to a different location or view. Still further, although only an Endoscope and LUS Probe are shown in this example, other Image Capturing Devices such as those used for capturing camera, ultrasound, magnetic resonance, computed axial tomography, and fluoroscopic images are also fully contemplated within the System 100, although each of these Image Capturing Devices may not necessarily be manipulated by one of the Master Input Devices.

[0047] FIG. 3 illustrates a side view of one embodiment of the LUS Probe 150. The LUS Probe 150 is a dexterous tool with preferably two distal degrees of freedom. Opposing pairs of Drive Rods or Cables (not shown) physically connected to a proximal end of the LUS Sensor 301 and extending through an internal passage of Elongated Shaft 312 mechanically control pitch and yaw movement of the LUS Sensor 301 using conventional push-pull type action.

[0048] The LUS Sensor 301 captures 2D ultrasound slices of a proximate anatomic structure, and transmits the information back to the Processor 102 through LUS Cable 304. Although shown as running outside of the Elongated Shaft 312, the LUS Cable 304 may also extend within it. A Clamshell Sheath 321 encloses the Elongate Shaft 312 and LUS Cable 304 to provide a good seal passing through a Cannula 331 (or trocar). Fiducial Marks 302 and 322 are placed on the LUS Sensor 301 and the Sheath 321 for video tracking purposes.

[0049] FIG. 4 illustrates, as an example, a flow diagram of a method for displaying the effect of a therapeutic procedure or treatment on the Display Screen 104. In 401, a primary image of an anatomic structure is captured by an image capturing device. As an example, FIG. 5 illustrates a primary image which has been captured by the Endoscope 140 and includes an anatomic structure 501 and therapeutic instrument 511 that has been partially inserted into the anatomic structure 501 in order to perform a therapeutic procedure at a therapy site within the anatomic structure 501. In another application, the therapeutic instrument 511 may only need to touch or come close to the anatomic structure 501 in order to perform a therapeutic procedure.

[0050] The primary image may be captured before or during the therapeutic procedure. A primary image captured before the procedure is referred to as being a "pre-operative" image, and a primary image captured during the procedure is referred to as being an "intra-operative"

image. When the primary image is a pre-operative image, the image is generally not updated during the procedure, so that the method generally only employs one primary image. On the other hand, when the primary image is an intra-operative image, the image is preferably updated periodically during the procedure, so that the method employs multiple primary images in that case.

[0051] Pre-operative images are typically captured using techniques such as Ultrasonography, Magnetic Resonance Imaging (MRI), or Computed Axial Tomography (CAT). Intra-operative images may be captured at the surgical or therapeutic site by image capturing devices such as the stereoscopic Endoscope **140** or LUS Probe **150**, or they may be captured externally by techniques such as those used to capture the pre-operative images.

[0052] In **402** of **FIG. 4**, the therapeutic instrument is turned on, or otherwise activated or energized, so as to be capable of applying therapy to the anatomic structure within the patient. The instrument generally has a tip for applying the therapeutic energy to abnormal tissue such as diseased or damaged tissue. As one example of such a therapeutic procedure, Radio Frequency Ablation (RFA) may be used to destroy diseased tissue such as a tumor located in an anatomic structure such as the liver by applying heat to the diseased tissue site using an RFA probe. Examples of other procedures include High Intensity Focused Ultrasound (HIFU) and Cauterization. The therapeutic instrument may be one of the Tools **138**, **139** attached to Slave Arms **121**, **122** so that it may be moved to and manipulated at the therapy site through the master/slave control system by the Surgeon.

[0053] In **403**, an auxiliary image is generated, wherein the auxiliary image indicates the effect of the therapeutic procedure on the anatomic structure. The auxiliary image may be an actual image of the anatomic structure that has been provided by or generated from information captured by a sensing device which is capable of sensing the effect of the therapeutic procedure. Alternatively, the auxiliary image may be a computer model indicating the effect of the therapy, which may be generated using an empirically derived or otherwise conventionally determined formula of such effect.

In this latter case, the computer model is generally a volumetric shape determined by such factors as the geometry of the tip of the therapeutic instrument, the heat or energy level being applied to the anatomic structure by the tip of the therapeutic instrument, and the features of the surrounding tissue of a therapy site being subjected to the therapeutic procedure in the anatomic structure.

[0054] As an example of an auxiliary image provided or otherwise derived from information captured by a sensing device, **FIG. 6** illustrates a three-dimensional ultrasound image of an anatomic structure **601** which has been conventionally derived from two-dimensional ultrasound slices captured by the LUS probe **150**. In this example, an ablation volume **621** is shown which represents the effect of a therapeutic procedure in which a tip **613** of an RFA probe **612** is being applied to a tumor site

of the anatomic structure **601**. The growth of the ablation volume in this case is viewable due to changes in tissue properties from the heating and necrosis of the surrounding tissue at the tumor site.

[0055] In **404**, the primary and auxiliary images are registered so as to be of the same scale and refer to a same position and orientation in a common reference frame. Registration of this sort is well known. As an example, see commonly owned U.S. Patent No. 6,522,906 entitled "Devices and Methods for Presenting and Regulating Auxiliary Information on an Image Display of a Telesurgical System to Assist an Operator in Performing a Surgical Procedure".

[0056] In **405**, the primary image is displayed on the Display Screen **104** while the therapeutic procedure is being performed, with the registered auxiliary image preferably overlaid upon the primary image so that corresponding structures or objects in each of the images appear as the same size and at the same location and orientation on the Display Screen **104**. In this way, the effect of the therapeutic procedure is shown as an overlay over the anatomic structure that is being subjected to the procedure.

[0057] As an example, **FIG. 7** shows an exemplary Display Screen **104** in which an auxiliary image, distinguished as a dotted line for illustrative purposes, is overlaid over the primary image of **FIG. 5**. When the auxiliary image is provided by or derives from information captured by a sensing device, the therapy effect **521**, therapeutic instrument **512**, and instrument tip **513** is provided by or derived from the captured information. On the other hand, when the therapy effect **521** is generated as a volumetric shaped computer model using an empirically determined formula, the therapeutic instrument **512** and instrument tip **513** may be determined using conventional tool tracking computations based at least in part upon joint positions of its manipulating slave arm.

[0058] In **406** of **FIG. 4**, the method then checks whether the therapeutic instrument has been turned off. If it has, then this means that the therapeutic procedure is over, and the method ends. On the other hand, if the therapeutic instrument is still on, then the method assumes that the therapeutic procedure is still being performed, and proceeds in **407** to determine whether a new primary image has been captured. If no new primary image has been captured, for example, because the primary image is a pre-operative image, then the method jumps back to **403** to update the auxiliary image and continue to loop through **403-407** until the therapeutic procedure is determined to be completed by detecting that the therapeutic instrument has been turned off. On the other hand, if a new primary image has been captured, for example, because the primary image is an intra-operative image, then the method updates the primary image in **408** before jumping back to **403** to update the auxiliary image and continue to loop through **403-408** until the therapeutic procedure is determined to be completed by detecting that the therapeutic instrument has

been turned off.

[0059] FIG. 8 illustrates, as an example, a flow diagram of a method for displaying an auxiliary image of an anatomic structure as a registered overlay to a primary image of the anatomic structure at a user specified magnification in a window defined as the lens area of a magnifying glass whose position and orientation as displayed on the Display Screen 104 is manipulatable by the user using an associated pointing device.

[0060] In 801, the method starts out by associating the magnifying glass with the pointing device so that as the pointing device moves, the magnifying glass being displayed on the Display Screen 104 (and in particular, its lens which may be thought of as a window) moves in a corresponding fashion. The association in this case may be performed by "grabbing" the magnifying glass in a conventional manner using the pointing device, or by making the magnifying glass effectively the cursor for the pointing device. Since the Display Screen 104 is preferably a three-dimensional display, the pointing device is correspondingly preferably a three-dimensional pointing device with orientation indicating capability.

[0061] In 802, current primary and auxiliary images are made available for processing. The primary image in this example is captured by the Endoscope 140 and the auxiliary captured by the LUS Probe 150. However, other sources for the primary and auxiliary images are also usable and contemplated in practicing the invention, including primary and auxiliary images captured from the same source. As an example of this last case, a high resolution camera may capture images at a resolution greater than that being used to display images on a display screen. In this case, the high resolution image captured by the camera may be treated as the auxiliary image, and the downsized image to be displayed on the display screen may be treated as the primary image.

[0062] In 803, a user selectable magnification factor is read. The magnification factor is user selectable by, for example, a dial or wheel type control on the pointing device. Alternatively, it may be user selectable by user selection of item in a menu displayed on the Display Screen 104, or any other conventional user selectable parameter value scheme or mechanism. If the user fails to make a selection, then a default value is used, such as a magnification factor of 1.0.

[0063] In 804, the primary and auxiliary images are registered so as to be of the same scale and refer to a same position and orientation in a common reference frame so that corresponding structures and objects in the two images have the same coordinates.

[0064] In 805, the primary image is displayed on the Display Screen 104 such as a three-dimensional view of the anatomic structure, in which case, a portion of a two-dimensional slice of the auxiliary image of the anatomic structure may be displayed as an overlay in the lens of the magnifying glass. The portion of the two-dimensional slice in this case is defined by a window area having a central point that has the same position and orientation

of as the central point of the lens of the magnifying glass, and an area determined by the magnification factor so that the portion of the two-dimensional slice may be enlarged or reduced so as to fit in the lens of the magnifying glass. Since the position and orientation of the magnifying glass is manipulatable by the positioning device to any position in the three-dimensional space of the Display Screen 104, including those within the volume of the anatomic structure, the two-dimensional slice can correspond to any user selected depth within the anatomic structure. Unlike a physical magnifying glass, its view is not limited to inspecting only the exterior of the anatomic structure. For additional details on 805, see the description below in reference to FIG. 9.

[0065] In 806, the method then determines whether the magnifying glass command has been turned off by, for example, the user releasing a "grabbed" image of the magnifying glass, or otherwise switching off the association between the magnifying glass and the pointing device by the use of a conventional switch mechanism of some sort. If it has, then the method ends. On the other hand, if it has not, then the method jumps back to 802 and continues to loop through 802-806 until the magnifying glass command is detected to have been turned off. Note that each time the method loops through 802-806, updated versions, if any, of the primary and auxiliary images are processed along with updated values, if any, for the user selectable magnification factor. Thus, if the method proceeds through the looping in a sufficiently fast manner, the user will not notice any significant delay if the user is turning a dial or knob to adjust the magnification factor while viewing the anatomic structure at a selected position and orientation of the magnifying glass.

[0066] FIG. 9 illustrates, as an example, a flow diagram of a method for displaying an auxiliary image view of an anatomic structure at a specified magnification factor as an overlay to a primary image view of the anatomic structure in the lens of a user movable magnifying glass. As previously explained, this method may be used to perform 805 of FIG. 8.

[0067] In 901, the current position and orientation of a central point of the lens of the magnifying glass are determined in the three-dimensional space of the Display Screen 104. In 902, a two-dimensional slice of the registered volumetric model of the auxiliary image is taken from the perspective of that position and orientation, and a portion of the two-dimensional slice is taken as defined in an auxiliary view window having a central point preferably at that same position and orientation. The area of the auxiliary view window in this case is inversely proportional to that of the lens according to the current magnification factor for the magnifying glass. In 903, the portion of the two-dimensional slice defined by the auxiliary view window is then enlarged by the magnification factor so that it fits in the lens area of the magnifying glass, and in 904, the primary image of the anatomic structure is displayed on the Display Screen 104 with the enlarged

portion of the two-dimensional slice of the auxiliary image overlaid in the lens area of the magnifying glass being displayed on the Display Screen 104.


[0068] As a pictorially example of 901-904, in FIGS. 10-11, a two-dimensional slice 1001 of an auxiliary image of an anatomic structure is shown along with two circular windows 1021, 1022 on the two-dimensional slice as illustrated in FIG. 10. Each of the windows 1021, 1022 in this case corresponds in shape to and having a central point equal to that of a lens 1121 of a magnifying glass 1120 which is being displayed along with a primary image of an external view 1101 of the anatomic structure on the Display Screen 104 as illustrated in FIG. 11. In this example, the area of the window 1021 is equal to the area of the lens 1121, so that if the magnification factor was 1.0, then window 1021 would be selected for use in 902. On the other hand, the area of the window 1022 is less than the area of the lens 1121, so that if the magnification factor is greater than 1.0, then the window 1022 may be selected for use in 902. Note that although the lens 1121 of the magnifying glass 1120 is depicted as being circularly shaped, it may also have other common shapes for a magnifying glass, such as a rectangular shape.

[0069] FIG. 12 illustrates, as an example, a flow diagram of a method performed by a processor in a medical robotic system for manipulating image objects displayed on a computer display screen of the medical robotic system in response to corresponding manipulation of an associated master input device when the master input device is in an image manipulating mode.

[0070] As a preface to the method, the medical robotic system includes an image capturing device to capture images (such as either the Endoscope 140 or the LUS Probe 150); a robotic arm holding the image capturing device (such as the Slave Arm 123 or the Slave Arm 124 respectively holding the Endoscope 140 and the LUS Probe 150); a computer display screen (such as the Display Screen 104); a master input device adapted to be manipulatable by a user in multiple degrees-of-freedom movement (such as the Master Input Device 107 or the Master Input Device 108); and a processor (such as the Auxiliary Controller 242) that is configured to control movement of the image capturing device according to user manipulation of the master input device when the master input device is in an image capturing mode, and control the displaying of images derived from the captured images on the computer display screen according to user manipulation of the master input device when the master input device is in the image manipulating mode.

[0071] In 1201, the processor detects that the user has placed the master input device into its image manipulating mode. One way that this may be implemented is using a master clutch mechanism provided in the medical robotic system, which supports disengaging the master input device from its associated robotic arm so that the master input device may be repositioned. When this mode is activated by some mechanism such as the user depressing a button on the master input device, pressing

down on a foot pedal, or using voice activation, the associated robotic arm is locked in position, and a cursor

(nominally an iconic representation of a hand, e.g. ) is presented to the user on the computer display screen. When the user exits this mode, the cursor is hidden and control of the robotic arm may be resumed after readjusting its position if required.

[0072] In 1202, the processor determines whether a control input such as that generated by depressing a button on a conventional mouse has been activated by the user. The control input in this case may be activated by depressing a button provided on the master input device, or it may be activated by some other fashion such as squeezing a gripper or pincher formation provided on the master input device. For additional details on clutching, and gripper or pincher formations on a master input device, see, e.g., commonly owned U.S. Patent No. 6,659,939 entitled "Cooperative Minimally Invasive Telesurgical System". If the control input is not determined to be "on" (i.e., activated) in 1202, then the processor waits until it either receives an "on" indication or the image manipulating mode is exited.

[0073] In 1203, after receiving an indication that the control input is "on", the processor checks to see if the cursor is positioned on (or within a predefined distance to) an object being displayed on the computer display screen. If it is not, then in 1204, the processor causes a menu of user selectable items or actions to be displayed on the computer display screen, and in 1205, the processor receives and reacts to a menu selection made by the user.

[0074] Examples of user selectable menu items include: magnifying glass, cut-plane, eraser, and image registration. If the user selects the magnifying glass item, then an image of a magnifying glass is displayed on the computer display screen and the method described in reference to FIG. 8 may be performed by the processor. When the user is finished with the magnifying glass function, then the user may indicate exiting of the function in any conventional manner and the processor returns to 1202.

[0075] If the user selects the cut-plane item, then a plane (or rectangular window of fixed or user adjustable size) is displayed on the computer display screen. The master input device may then be associated with the plane so that the user may position and orientate the plane in the three-dimensional space of the computer display screen by manipulating the master input device in the manner of a pointing device. If the plane is maneuvered so as to intersect a volume rendering of an anatomic structure, then it functions as a cut-plane defining a two-dimensional slice of the volume rendering at the intersection. Alternatively, the master input device may be associated with the volume rendering of the anatomic structure, which may then be maneuvered so as to intersect the displayed plane to define the cut-plane. Association of the plane or volume rendering with the pointing

device may be performed in substantially the same manner as described in reference to the magnifying glass with respect to **801** of **FIG. 8**.

[0076] The two-dimensional slice may then be viewed either in the plane itself, or in a separate window on the computer display screen such as in a picture-in-picture. The user may further select the cut-plane item additional times to define additional two-dimensional slices of the volume rendering for concurrent viewing in respective planes or picture-in-picture windows on the computer display screen. So as not to clutter the computer display screen with unwanted cut-plane slices, a conventional delete function is provided so that the user may selectively delete any cut-planes and their corresponding slices. When the user is finished with the cut-plane function, then the user may indicate exiting of the function in any conventional manner and the processor returns to **1202**.

[0077] If the user selects the eraser item, then an eraser is displayed on the computer display screen. The master input device is then associated with the eraser so that the user may position and orientate the eraser in the three-dimensional space of the computer display screen by manipulating the master input device in the manner of a pointing device. Association of the eraser with the pointing device in this case may be performed in substantially the same manner as described in reference to the magnifying glass with respect to **801** of **FIG. 8**. If the eraser is maneuvered so as to intersect a volume rendering of an anatomic structure, then it functions to either completely or partially erase such rendering wherever it traverses the volume rendering. If partial erasing is selected by the user (or otherwise pre-programmed into the processor), then each time the eraser traverses the volume rendering, less detail of the anatomic structure may be shown. Less detail in this case may refer to the coarseness/fineness of the rendering, or it may refer to the stripping away of layers in the three-dimensional volume rendering. All such characteristics or options of the erasing may be user selected using conventional means. If the user inadvertently erases a portion of the volume rendering, a conventional undo feature is provided to allow the user to undo the erasure. When the user is finished with the erasing function, then the user may indicate exiting of the function in any conventional manner and the processor returns to **1202**.

[0078] In addition to an eraser function as described above, other spatially localized modifying functions are also contemplated and considered to be within the full scope of the present invention, including selectively sharpening, brightening, or coloring portions of a displayed image to enhance its visibility in, or otherwise highlight, a selected area. Each such spatially localized modifying function may be performed using substantially the same method described above in reference to the eraser function.

[0079] If the user selects the image registration item, then the processor records such selection for future action as described below in reference to **1212** before jump-

ing back to process **1202** again. Image registration in this case typically involves manually registering an auxiliary image of an object such as an anatomic structure with a corresponding primary image of the object.

[0080] As an alternative to the above described menu approach, icons respectively indicating each of the selectable items as described above may be displayed on the computer display screen upon entering image manipulating mode and selected by the user clicking on them, after which, the processor proceeds to perform as described above in reference to selection of their corresponding menu items.

[0081] Now continuing with the method described in reference to **FIG. 12**, after receiving an indication that the control input is on in **1201** and determining that the cursor is positioned on or near an object (not an icon) being displayed on the computer display screen in **1202**, the processor preferably changes the cursor from an iconic representation of a hand, for example, to that of a grasping hand to indicate that the object has been "grabbed" and is ready to be moved or "dragged" to another position and/or orientation in the three-dimensional space of the computer display screen through user manipulation of the master input device.

[0082] In **1206**, the processor then determines whether the user has indicated that a display parameter of the selected object is to be adjusted, and if the user has so indicated, in **1207**, the processor performs the display adjustment. As an example, a dial on the master input device may be turned by the user to indicate both that a display adjustment for a display parameter associated with dial is to be adjusted according to the amount of rotation of the dial on the selected object. Alternatively, if the master input device is equipped with a gripper, the gripper may be rotated so as to function as a dial. Examples of display parameters that may be adjusted in this manner include: brightness, contrast, color, and level of detail (e.g., mesh coarseness/fineness, or voxel size and/or opaqueness) of the selected object being displayed on the computer display screen.

[0083] The processor then proceeds to **1208** to determine whether the cursor has moved since "grabbing" the selected object after an affirmative determination in **1203**. If it has not moved, then the processor jumps back to **1202** since the user may only have wanted to adjust a display parameter of a selected object at this time. On the other hand, if the cursor has moved since "grabbing" the selected object, then in **1209**, the processor moves the selected object to the new cursor position. Since the cursor operates in the three-dimensional space of the computer display screen, when it moves "into" the display screen, it may indicate such movement by, for example, getting progressively smaller in size. Where the three-dimensional nature of the computer display screen is achieved through the use of right and left two-dimensional views of the object with disparities of common points between the two views indicating depth values, decreasing of the depth values for images of the cursor in the

right and left views indicates that the cursor is moving "into" the display screen.

[0084] Optionally, in **1210**, haptic feedback may be provided back to the master input device so that the user may sense reflected forces while the "grabbed" object is being moved in **1209**. As an example, user interactions with the object may be reflected haptically back to the user by associating a virtual mass and inertial properties with the object so that the user feels a reflected force when coming into contact with the object or when translating or rotating the object as it is accelerated/decelerated. The haptic feedback performed in this **1210** may only be performed for some types of objects and not for others, or it may take effect only in certain circumstances. Use of such haptic feedback may also be applied to the movement of the magnifying glass and/or the plane used for defining cut-planes as described above. In such cases, however, the haptic feedback may be restricted to only occurring after the magnifying glass or the plane enters into an anatomic structure of interest.

[0085] In **1211**, the processor determines whether the control input is still in an "on" state. If the control is still "on", then the processor jumps back to **1208** to track and respond to cursor movement. On the other hand, if the control has been turned off by, for example, the user releasing a button that was initially depressed to indicate that control was turned "on", then in **1212**, the processor performs a selected menu action.

[0086] For example, if the image registration item had been selected by the user in response to the processor displaying the menu in **1204** (or alternatively, the user clicking an icon indicating that item), then the object that has been moved is registered with another image of the object that is now aligned with and is being displayed on the computer display screen at the time so that they have the same coordinate and orientation values in a common reference frame such as that of the computer display screen. This feature facilitates, for example, manual registration of an auxiliary image of an anatomic structure (such as obtained using the LUS Probe 150) with a primary image of the anatomic structure (such as obtained using the Endoscope **140**). After the initial registration, changes to the position and/or orientation of the corresponding object in the primary image may be mirrored so as to cause corresponding changes to the selected object in the auxiliary image so as to maintain its relative position/orientation with respect to the primary image. When the user is finished with the image registration function, then the processor returns to **1202**.

[0087] Although the various aspects of the present invention have been described with respect to a preferred embodiment, it will be understood that the invention is entitled to full protection within the full scope of the appended claims.

Claims

1. A medical robotic system (100) comprising:

an image capturing device (150) for capturing images;
a robotic arm (124) holding the image capturing device (150);
a computer display screen (104);
a master input device (108) adapted to be manipulatable by a user in multiple degrees-of-freedom movement; and
a processor (102) configured to:

when the master input device (108) is in an image capturing mode, control movement of the image capturing device (150) according to user manipulation of the master input device (108); and

when the master input device (108) is in an image manipulating mode:

control the displaying of images derived from the captured images on the computer display screen (104) according to user manipulation of the master input device (108);

characterized by the processor (102) further configured to:

display one of the three-dimensional volumes and a two-dimensional window on the computer display screen (104);

manipulate a position and orientation of the window on the computer display screen (104) in response to user manipulation of the master input device (108); and

define a cut-plane by an intersection of the window with the three-dimensional volume so as to indicate a two-dimensional slice of the three-dimensional volume.

2. The medical robotic system (100) according to claim 1, wherein the two-dimensional slice is displayed in the window.

3. The medical robotic system (100) according to claim 1, wherein the two-dimensional slice is displayed in a picture-in-picture window of the computer display screen (104).

4. The medical robotic system (100) according to claim 1, wherein the processor (102) is further configured to display a user selectable number of two-dimensional windows on the computer display screen

(104), individually manipulate positions and orientations of the windows on the computer display screen (104) in response to user manipulation of the master input device (108), and define cut-planes by intersections of the manipulated windows with the three-dimensional volume so as to indicate corresponding two-dimensional slices of the three-dimensional volume.

5. The medical robotic system (100) according to claim 4, wherein the two-dimensional slices are displayed in corresponding picture-in-picture windows of the computer display screen (104). 5
6. The medical robotic system (100) according to claim 1, wherein the processor (102) is configured to display the two-dimensional window on the computer display screen (104) in response to user selection of an item included in a displayed menu on the computer display screen (104). 10 20
7. The medical robotic system (100) according to claim 1, wherein the processor (102) is configured to display the two-dimensional window on the computer display screen (104) in response to user selection of an icon being displayed on the display screen (104). 25
8. The medical robotic system (100) according to claim 7, wherein the icon is displayed in a periphery area of the computer display screen (104), and the processor (102) is further configured to interpret user mouse-type actions of clicking on the icon and dragging the icon away from the periphery area as a user selection of the icon. 30 35
9. The medical robotic system (100) according to claim 8, wherein the image capturing device (150) is an ultrasound probe (150) and the derived images are three-dimensional ultrasound images of an anatomic structure that are computer generated from two-dimensional ultrasound slices captured by the ultrasound probe (150). 40

Patentansprüche

1. Medizinisches Robotersystem (100), das Folgendes umfasst:

eine Bilderfassungsvorrichtung (150) zum Erfassen von Bildern;
einen Roboterarm (124), der die Bilderfassungsvorrichtung (150) hält;
einen Computerbildschirm (104);
eine Haupteingabevorrichtung (108), die dafür ausgelegt ist, von einem Benutzer in mehreren Freiheitsgraden bewegt werden zu können; und

einen Prozessor (102), der für Folgendes konfiguriert ist:

wenn sich die Haupteingabevorrichtung (108) in einem Bildaufnahmemodus befindet, Steuern der Bewegung der Bilderfassungsvorrichtung (150) gemäß einer Benutzerbedienung der Haupteingabevorrichtung (108); und
wenn sich die Haupteingabevorrichtung (108) in einem Bildbearbeitungsmodus befindet:

Steuern der Anzeige von Bildern, die von den aufgenommenen Bildern auf dem Computeranzeigebildschirm (104) abgeleitet wurden, gemäß einer Benutzerbedienung der Haupteingabevorrichtung (108);

dadurch gekennzeichnet, dass der Prozessor (102) ferner für Folgendes konfiguriert ist:

Anzeigen eines der dreidimensionalen Volumina und eines zweidimensionalen Fensters auf dem Computeranzeigebildschirm (104);

Manipulieren einer Position und Orientierung des Fensters auf dem Computeranzeigebildschirm (104) als Reaktion auf eine Manipulation der Haupteingabevorrichtung (108) durch den Benutzer; und
Definieren einer Schnittebene durch einen Schnitt des Fensters mit dem dreidimensionalen Volumen, um eine zweidimensionale Schicht des dreidimensionalen Volumens anzuzeigen.

2. Medizinisches Robotersystem (100) nach Anspruch 1, wobei die zweidimensionale Schicht in dem Fenster angezeigt wird.

3. Medizinisches Robotersystem (100) nach Anspruch 1, wobei die zweidimensionale Schicht in einem Bild-in-Bild-Fenster des Computerbildschirms (104) angezeigt wird.

4. Medizinisches Robotersystem (100) nach Anspruch 1, wobei der Prozessor (102) ferner für Folgendes konfiguriert ist: Anzeigen einer vom Benutzer wählbaren Anzahl von zweidimensionalen Fenstern auf dem Computeranzeigebildschirm (104), individuelles Manipulieren der Positionen und Ausrichtungen der Fenster auf dem Computeranzeigebildschirm (104) als Reaktion auf eine Benutzerhandhabung der Haupteingabevorrichtung (108) und Definieren

der Schnittebenen durch Schnittpunkte der manipulierten Fenster mit dem dreidimensionalen Volumen, um entsprechende zweidimensionale Schichten des dreidimensionalen Volumens anzuzeigen.

5. Medizinisches Robotersystem (100) nach Anspruch 4, wobei die zweidimensionalen Schichten in entsprechenden Bild-in-Bild-Fenstern des Computerbildschirms (104) angezeigt werden.

6. Medizinisches Robotersystem (100) nach Anspruch 1, wobei der Prozessor (102) dafür konfiguriert ist, das zweidimensionale Fenster auf dem Computeranzeigebildschirm (104) als Reaktion auf die Benutzerauswahl eines Elements anzuzeigen, das in einem angezeigten Menü auf dem Computeranzeigebildschirm (104) enthalten ist.

7. Medizinisches Robotersystem (100) nach Anspruch 1, wobei der Prozessor (102) dafür konfiguriert ist, das zweidimensionale Fenster auf dem Computeranzeigebildschirm (104) als Reaktion auf die Benutzerauswahl eines auf dem Anzeigebildschirm (104) angezeigten Symbols anzuzeigen.

8. Medizinisches Robotersystem (100) nach Anspruch 7, wobei das Symbol in einem Randbereich des Computeranzeigebildschirms (104) angezeigt wird, und der Prozessor (102) ferner dafür konfiguriert ist, die Mauseaktionen des Benutzers durch Klicken auf das Symbol und Ziehen des Symbols aus dem Peripheriebereich als eine Benutzerauswahl des Symbols zu interpretieren.

9. Medizinisches Robotersystem (100) nach Anspruch 8, wobei die Bilderfassungsvorrichtung (150) eine Ultraschallsonde (150) ist und die abgeleiteten Bilder dreidimensionale Ultraschallbilder einer anatomischen Struktur sind, die aus zweidimensionalen Ultraschallschichten computergeneriert werden, die von der Ultraschallsonde (150) erfasst werden.

Revendications

1. Système robotisé médical (100) comprenant :

un dispositif de capture d'image (150) destiné à capturer des images ;
un bras robotisé (124) tenant le dispositif de capture d'image (150) ;
un écran d'affichage d'ordinateur (104) ;
un dispositif d'entrée maître (108) conçu pour pouvoir être manipulé par un utilisateur dans un mouvement à plusieurs degrés de liberté de mouvement ; et
un processeur (102) configuré pour :

quand le dispositif d'entrée maître (108) est dans un mode de capture d'image, commander le mouvement du dispositif de capture d'image (150) selon la manipulation par l'utilisateur du dispositif d'entrée maître (108) ; et

quand le dispositif d'entrée maître (108) est dans un mode de manipulation d'image : commander l'affichage d'images dérivées des images capturées sur l'écran d'affichage d'ordinateur (104) selon la manipulation par l'utilisateur du dispositif d'entrée maître (108) ;

caractérisé en ce que le processeur (102) est configuré en outre pour :

afficher soit des volumes tridimensionnels soit une fenêtre bidimensionnelle sur l'écran d'affichage d'ordinateur (104) ;
manipuler une position et une orientation de la fenêtre sur l'écran d'affichage d'ordinateur (104) en réponse à la manipulation par l'utilisateur du dispositif d'entrée maître (108) ; et
définir un plan de coupe par une intersection de la fenêtre avec le volume tridimensionnel de manière à indiquer une tranche bidimensionnelle du volume tridimensionnel.

2. Système robotisé médical (100) selon la revendication 1, dans lequel la tranche bidimensionnelle est affichée dans la fenêtre.

3. Système robotisé médical (100) selon la revendication 1, dans lequel la tranche bidimensionnelle est affichée dans une fenêtre d'incrustation d'image de l'écran d'affichage d'ordinateur (104).

4. Système robotisé médical (100) selon la revendication 1, dans lequel le processeur (102) est configuré en outre pour afficher un nombre sélectionnable par l'utilisateur de fenêtres bidimensionnelles sur l'écran d'affichage d'ordinateur (104), manipuler individuellement des positions et des orientations des fenêtres sur l'écran d'affichage d'ordinateur (104) en réponse à la manipulation par l'utilisateur du dispositif d'entrée maître (108), et définir des plans de coupe par des intersections des fenêtres manipulées avec le volume tridimensionnel de manière à indiquer des tranches bidimensionnelles correspondantes du volume tridimensionnel.

5. Système robotisé médical (100) selon la revendication 4, dans lequel les tranches bidimensionnelles sont affichées dans des fenêtres d'incrustation d'image correspondantes de l'écran d'affichage d'ordinateur (104).

6. Système robotisé médical (100) selon la revendication 1, dans lequel le processeur (102) est configuré pour afficher la fenêtre bidimensionnelle sur l'écran d'affichage d'ordinateur (104) en réponse à la sélection par l'utilisateur d'un élément inclus dans un menu affiché sur l'écran d'affichage d'ordinateur (104). 5
7. Système robotisé médical (100) selon la revendication 1, dans lequel le processeur (102) est configuré pour afficher la fenêtre bidimensionnelle sur l'écran d'affichage d'ordinateur (104) en réponse à la sélection par l'utilisateur d'une icône étant affichée sur l'écran d'affichage (104). 10
8. Système robotisé médical (100) selon la revendication 7, dans lequel l'icône est affichée dans une zone périphérique de l'écran d'affichage d'ordinateur (104), et le processeur (102) est configuré en outre pour interpréter des actions de type souris par l'utilisateur de cliquage sur l'icône et de glissement de l'icône pour l'éloigner de la zone périphérique comme une sélection par l'utilisateur de l'icône. 15 20
9. Système robotisé médical (100) selon la revendication 8, dans lequel le dispositif de capture d'image (150) est une sonde échographique (150) et les images dérivées sont des images tridimensionnelles échographiques d'une structure anatomique qui sont générées par ordinateur à partir de tranches bidimensionnelles échographiques par la sonde échographique (150). 25 30

35

40

45

50

55

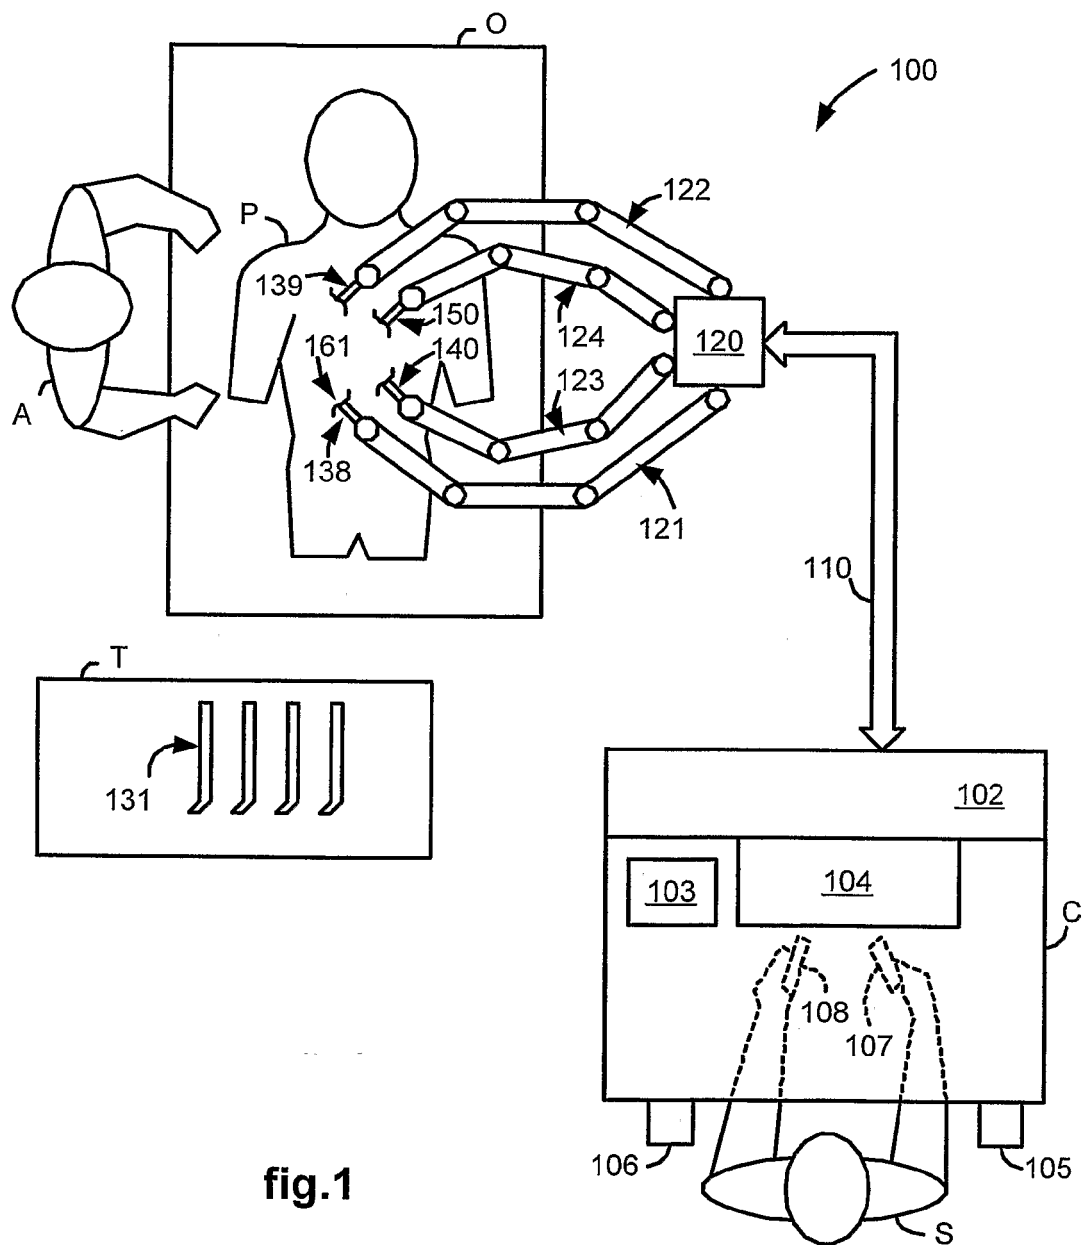


fig.1

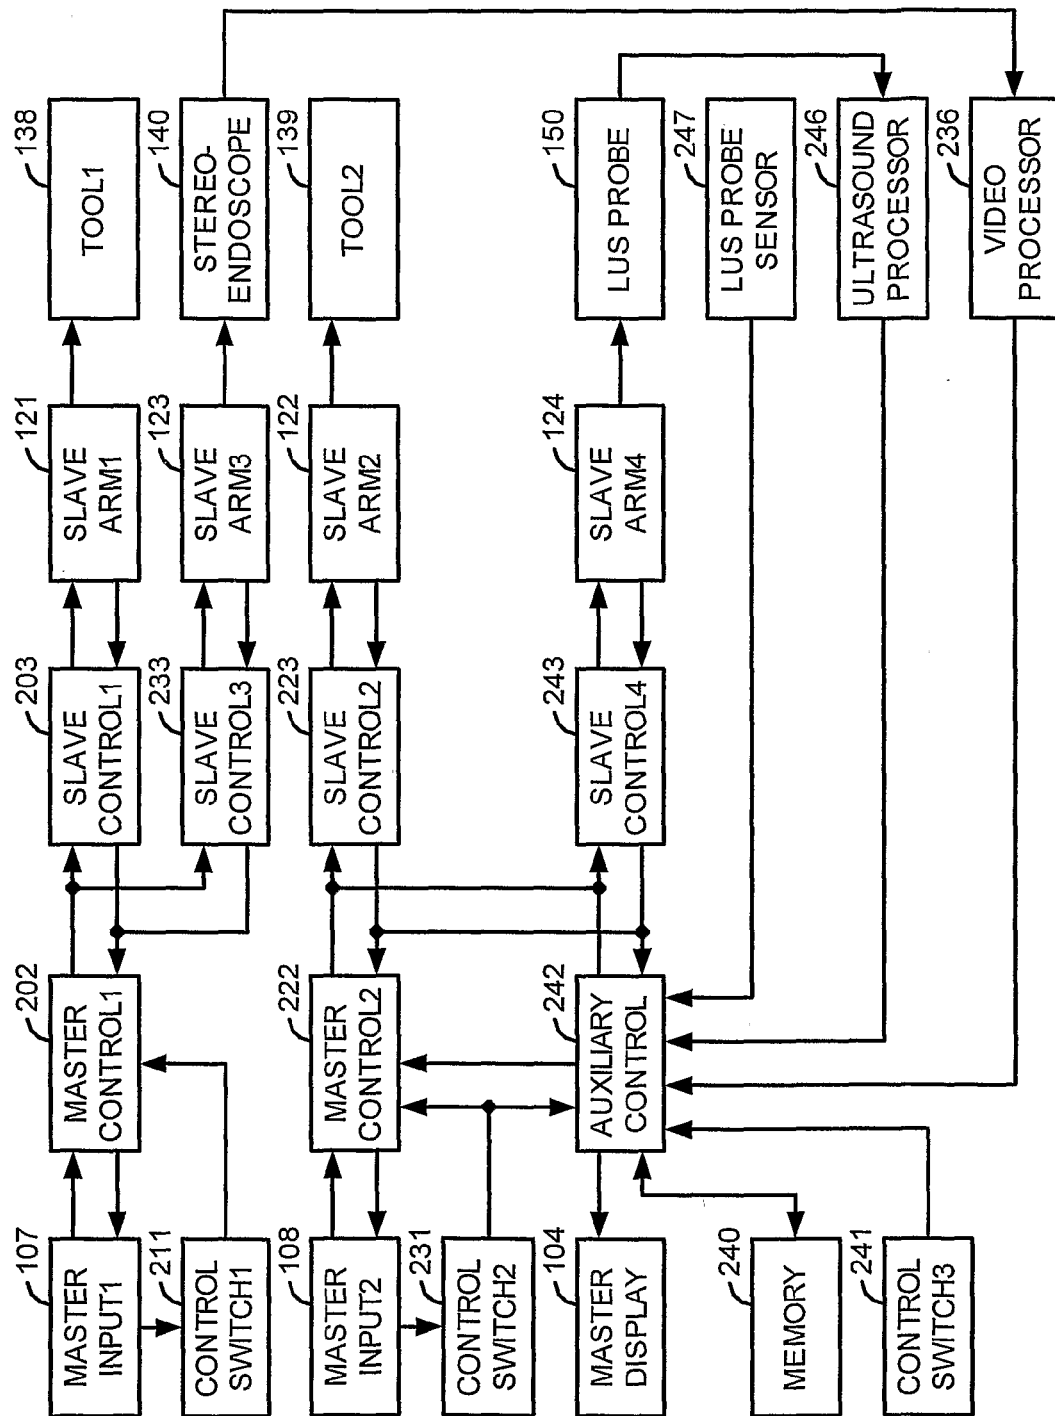


fig.2

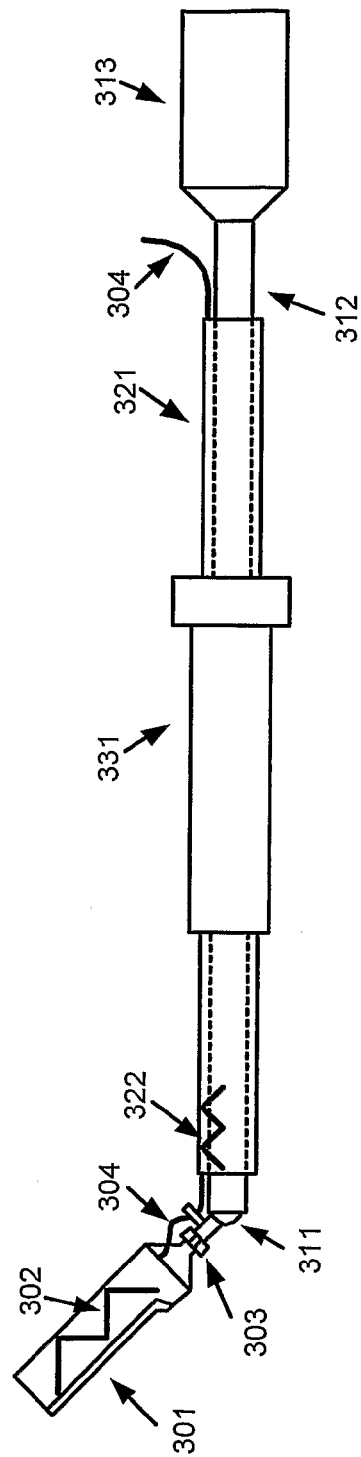


fig.3

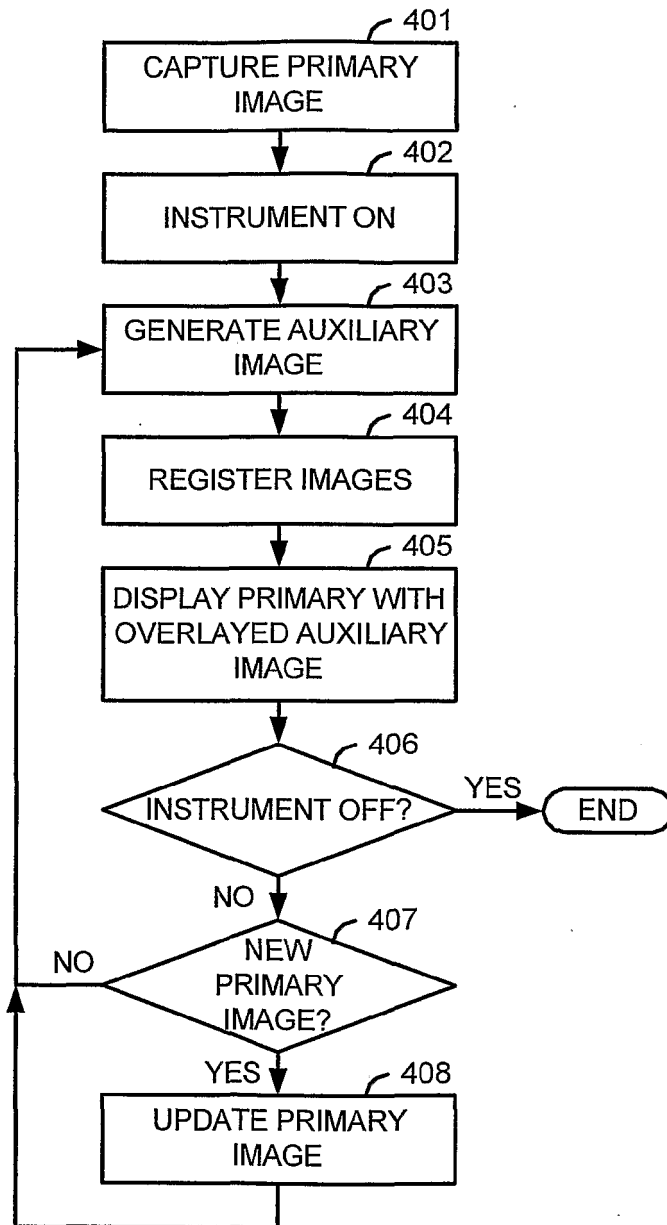


fig.4

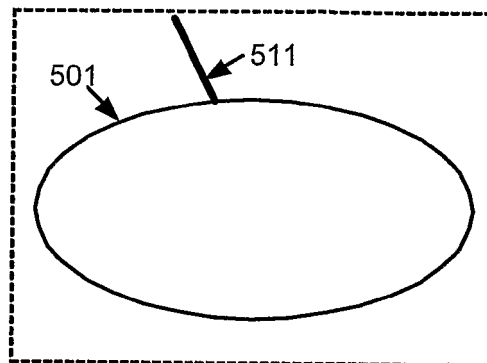


fig.5

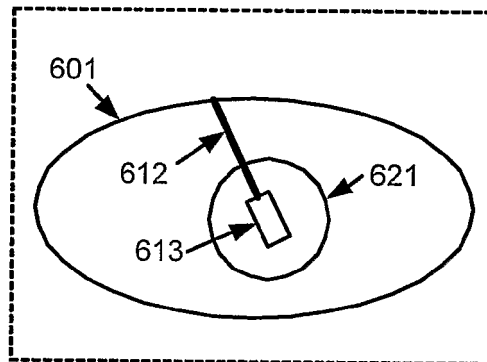


fig.6

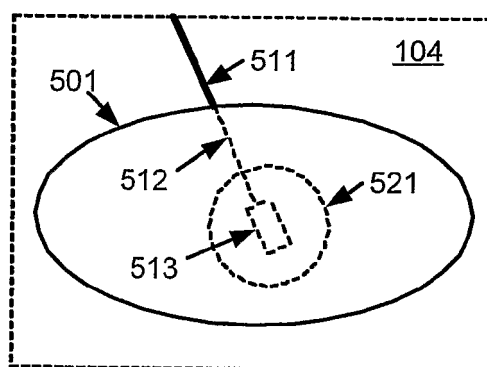


fig.7

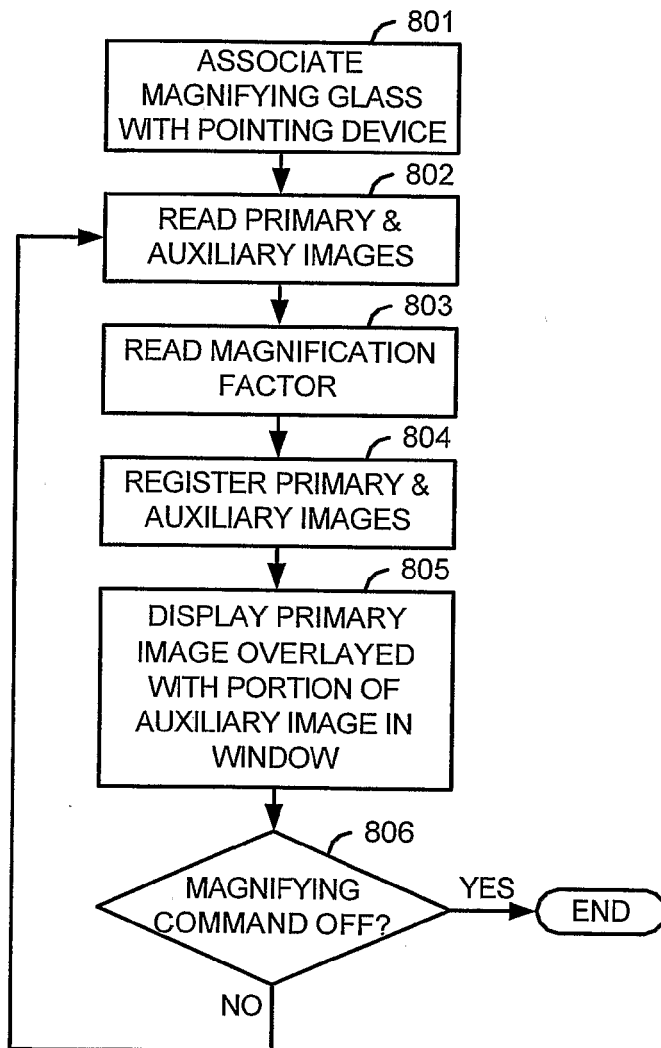


fig.8

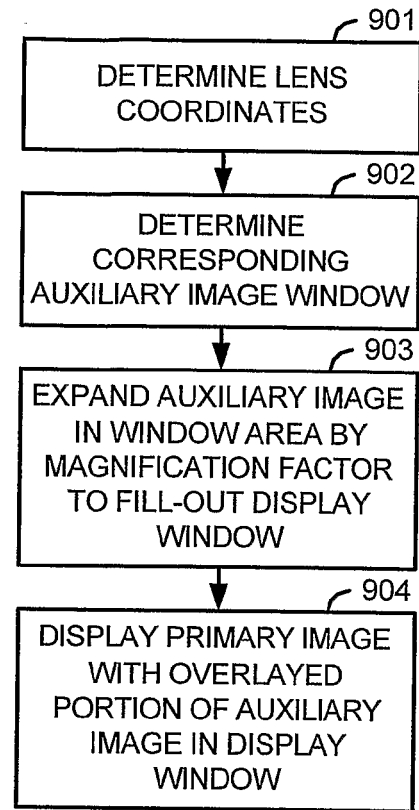


fig.9

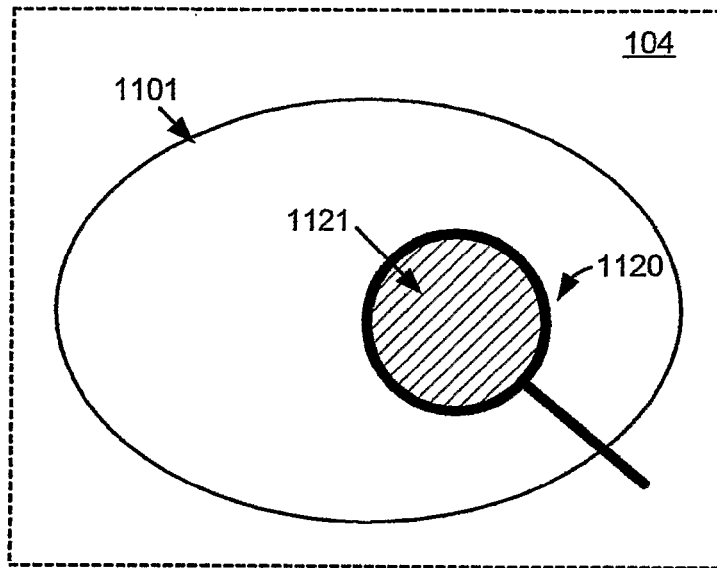


fig.11

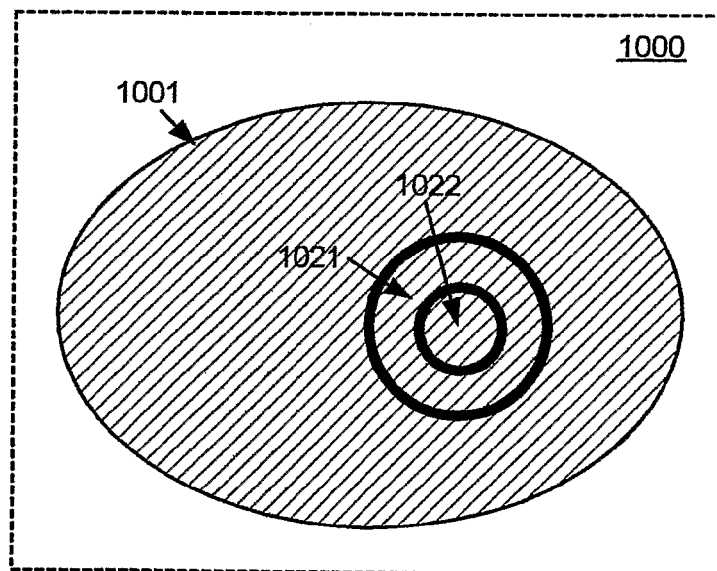


fig.10

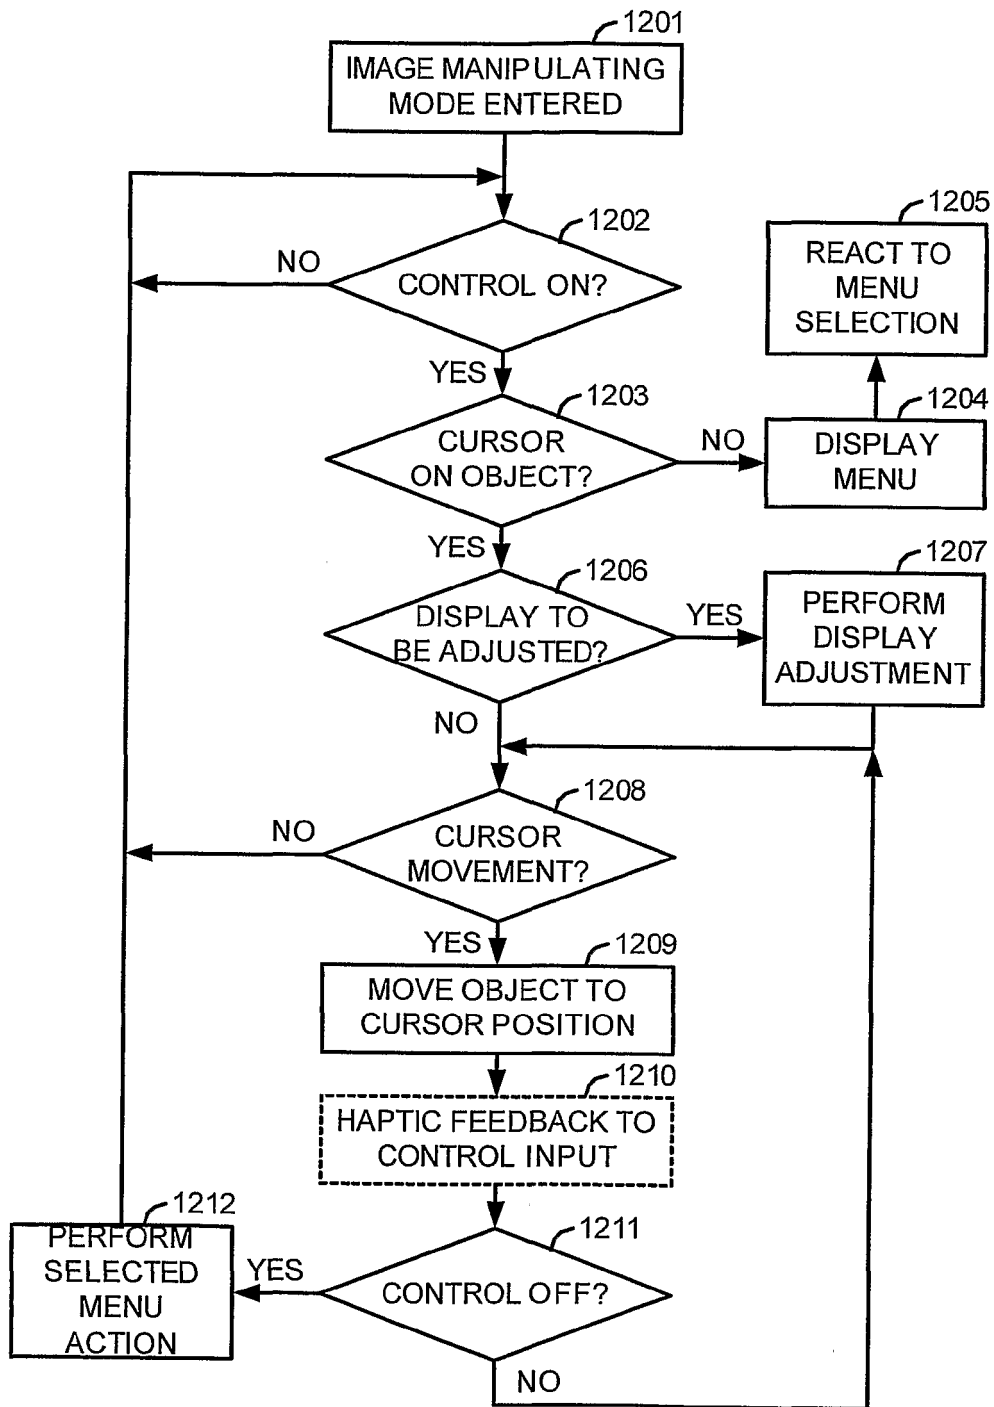


fig.12

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2004106916 A1 [0008]
- US 6522906 B1 [0009]
- US 5797900 A [0025]
- US 6659939 B [0041] [0072]
- US 44766806 A [0042]
- US 6522906 B [0055]

专利名称(译)	医疗机器人系统中计算机显示器上的辅助图像显示和操作		
公开(公告)号	EP3162318B1	公开(公告)日	2019-10-16
申请号	EP2016195634	申请日	2006-10-19
[标]申请(专利权)人(译)	直观外科手术操作公司		
申请(专利权)人(译)	Intuitive Surgical公司运营 , INC.		
当前申请(专利权)人(译)	Intuitive Surgical公司运营 , INC.		
[标]发明人	HOFFMAN BRIAN KUMAR RAJESH LARKIN DAVID PRISCO GIUSEPPE SWARUP NITISH ZHANG GUANGHUA G		
发明人	HOFFMAN, BRIAN KUMAR, RAJESH LARKIN, DAVID PRISCO, GIUSEPPE SWARUP, NITISH ZHANG, GUANGHUA G		
IPC分类号	A61B90/00 A61B18/14 G06F3/01		
CPC分类号	A61B18/1482 A61B34/10 A61B34/30 A61B34/37 A61B34/70 A61B34/71 A61B34/76 A61B90/36 A61B90/361 A61B90/37 A61B2090/101 A61B2090/364 A61B2090/374 A61B2090/3782 A61N7/022 G06F3/011 G06F3/016 G06F3/0346 G06F3/0481 G06F3/04817 G06F3/04842 G06F3/04845 G06F3 /04847 G06F3/0486 G06F2203/014 G06F2203/04804 G06F2203/04806 A61B1/00193 A61B1/04 A61B1/313 A61B5/055 A61B5/742 A61B18/12 A61B2018/00577 A61B2018/00595 A61B2018/00982 A61B2018/00994 A61B2090/378		
优先权	60/728450 2005-10-20 US PCT/US2006/040754 2006-10-19 WO		
其他公开文献	EP3162318A3 EP3162318A2		
外部链接	Espacenet		

摘要(译)

为了帮助外科医生执行医疗程序，外科医生通常在计算机显示屏上显示和操纵辅助图像，该辅助图像通常指示正被治疗的解剖结构的内部细节，并且通常由该解剖结构的外部视图补充主图像。外科医生可以将在第一模式下控制机械臂的主输入设备切换到第二模式，以便代替地用作鼠标状指示设备，以方便外科医生执行这种辅助信息的显示和操纵。

