



US 20050283079A1

(19) **United States**

(12) **Patent Application Publication** (10) **Pub. No.: US 2005/0283079 A1**

Steen et al.

(43) **Pub. Date:** **Dec. 22, 2005**

(54) **METHOD AND APPARATUS FOR MEDICAL
ULTRASOUND NAVIGATION USER
INTERFACE**

(76) Inventors: **Erik Normann Steen**, Moss (NO);
Rune Torkildsen, Foreidgrend (NO);
Ditlef Martens, Bergen (NO)

Correspondence Address:

DEAN D. SMALL (12553 + 1000)
ARMSTRONG TEASDALE LLP
ONE METROPOLITAN SQUARE, SUITE 2600
ST. LOUIS, MO 63102-2740 (US)

(21) Appl. No.: **10/926,547**

(22) Filed: **Aug. 26, 2004**

Related U.S. Application Data


(60) Provisional application No. 60/581,675, filed on Jun. 22, 2004.

Publication Classification

(51) **Int. Cl.⁷** **A61B 8/02**
(52) **U.S. Cl.** **600/447**

(57) ABSTRACT

In one embodiment, an ultrasound system is provided that includes a probe having a 2D array of transducers for acquiring ultrasound information along a plurality of scan lines through an object in real time. The scan lines are arranged to define volumetric data corresponding to a volume of interest (VOI) in a subject or patient. One such VOI may include the human heart or some portion of the human heart. The system includes a beamformer configured with scan parameter values that define the scan lines. An image buffer stores multiple data volumes acquired over time that are successively retrieved and processed by a display processor. The display processor accesses the data volumes stored in the image buffer successively to control generation of at least one of 2D and 3D renderings based on display parameters, wherein the display processor obtains from the image buffer a first data volume defined based on first scan parameter values, while the probe acquires ultrasound information for a second data volume that is entered into the image buffer. The second data volume is defined based on second scan parameter values. A navigation view presents in real time the renderings generated by the display processor with their corresponding 3D orientation. A navigator is provided that controls the display of the navigation view in real time such that, as the user adjusts a display parameter value to change a view plane, images presented in the navigation view are updated to reflect the view plane. A user interface is provided for adjusting the scan and display parameter values.

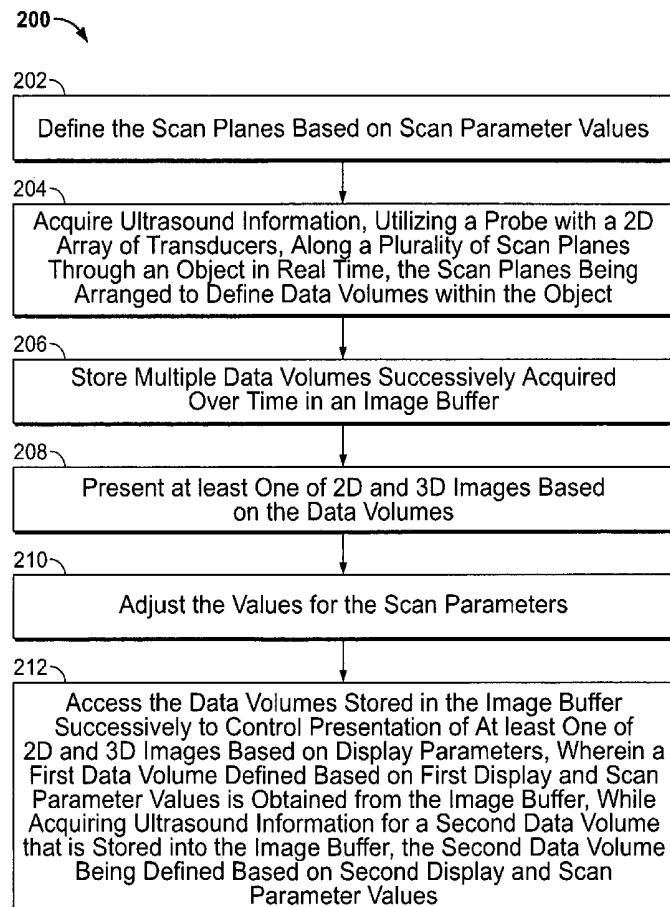

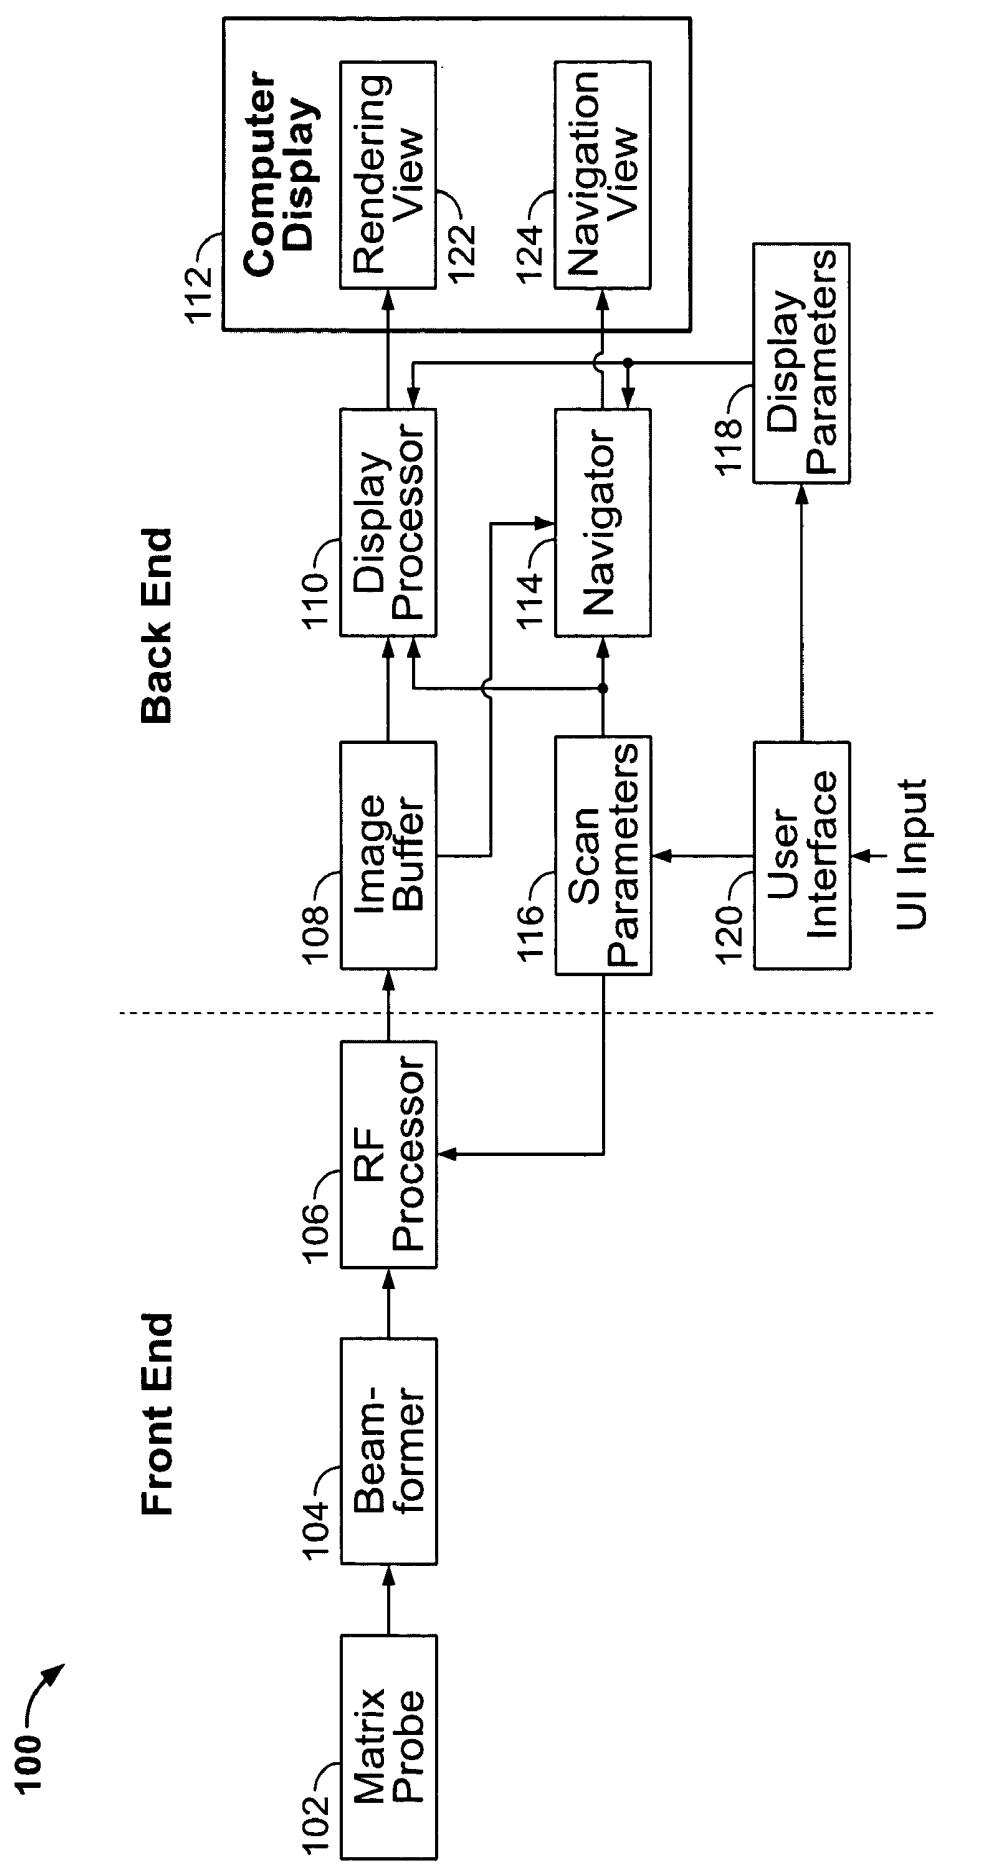


FIG. 1

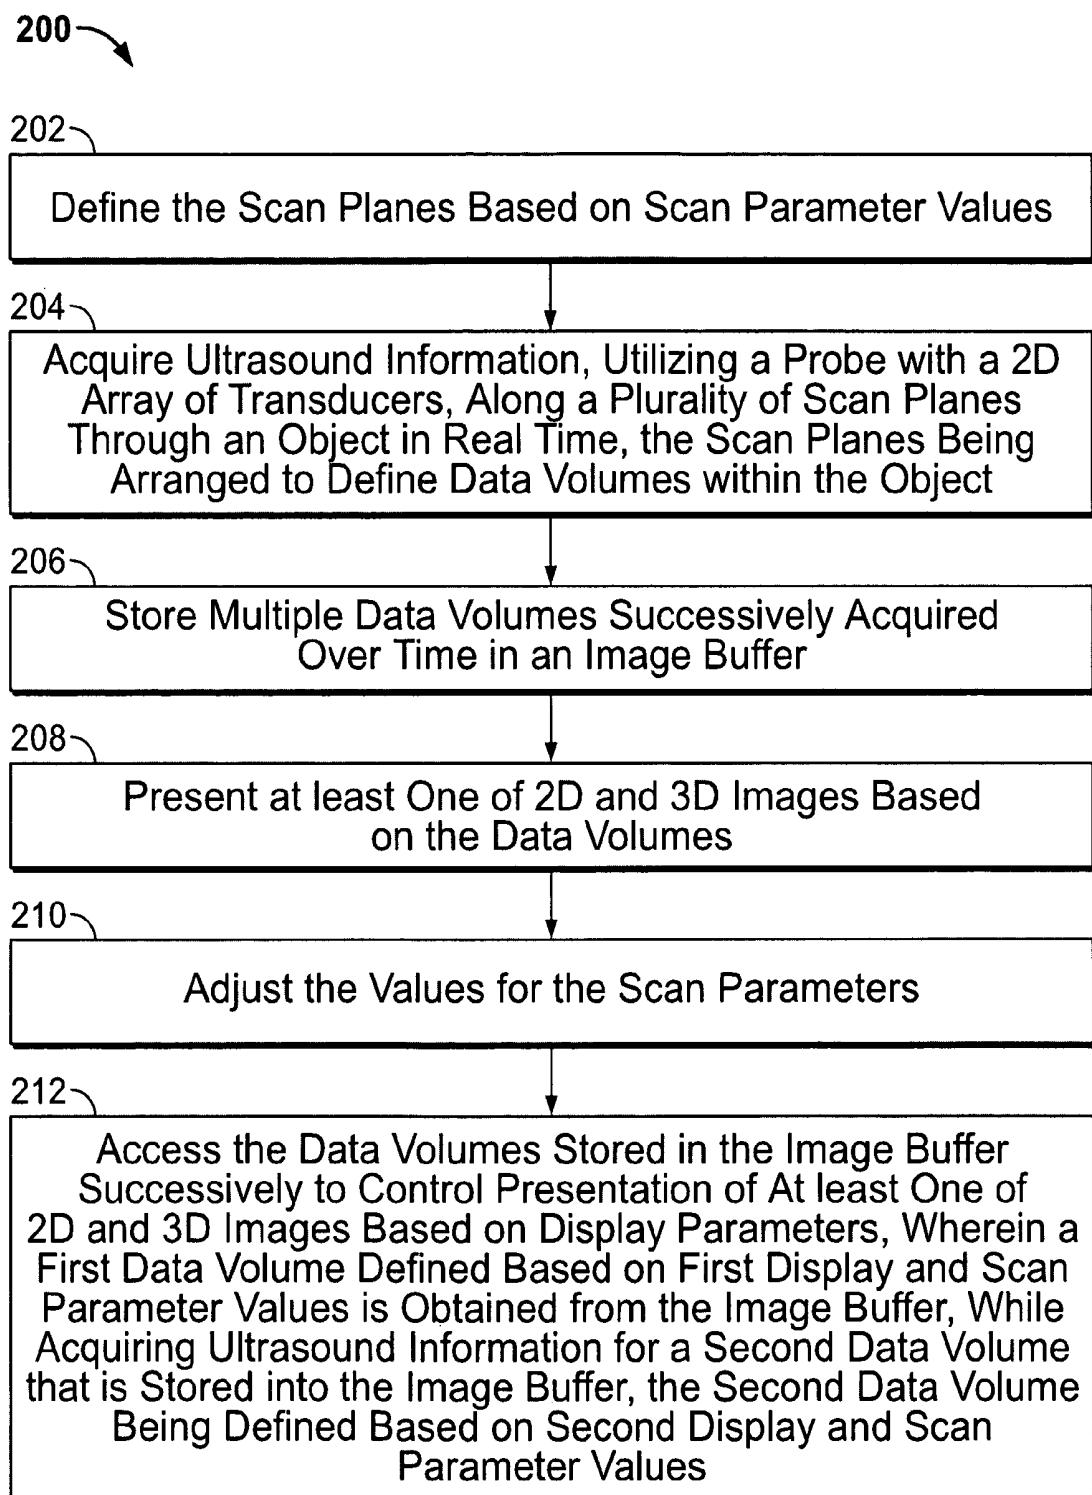
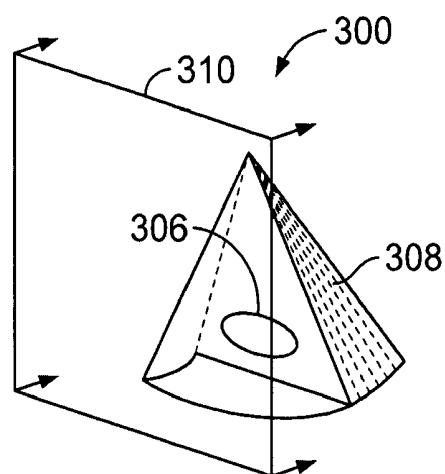
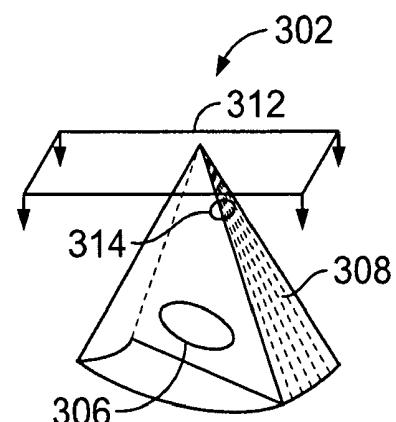
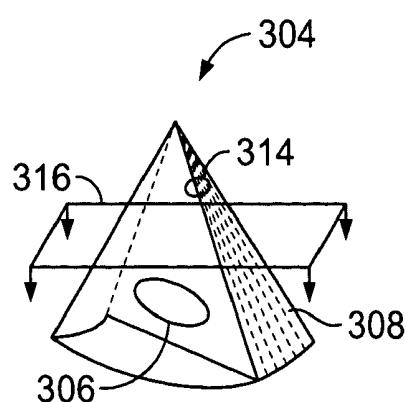
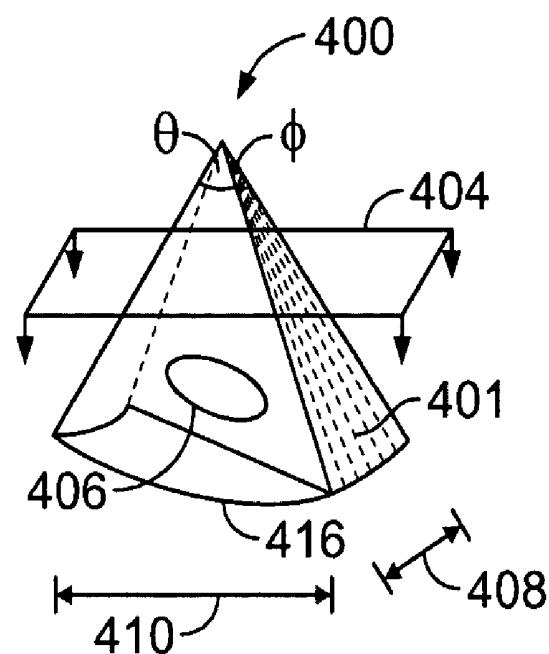
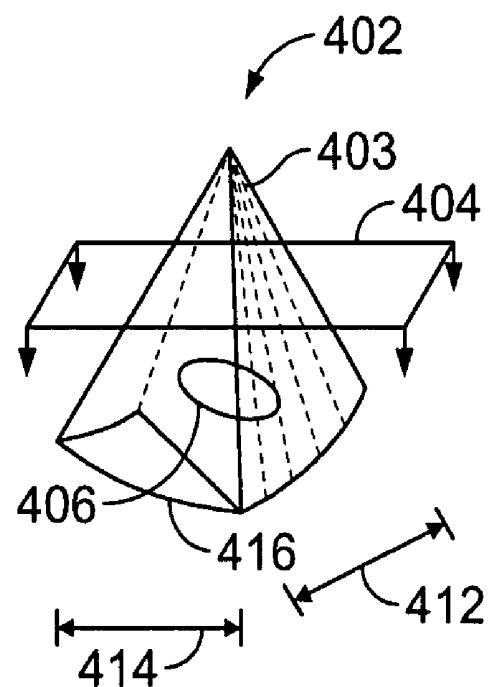
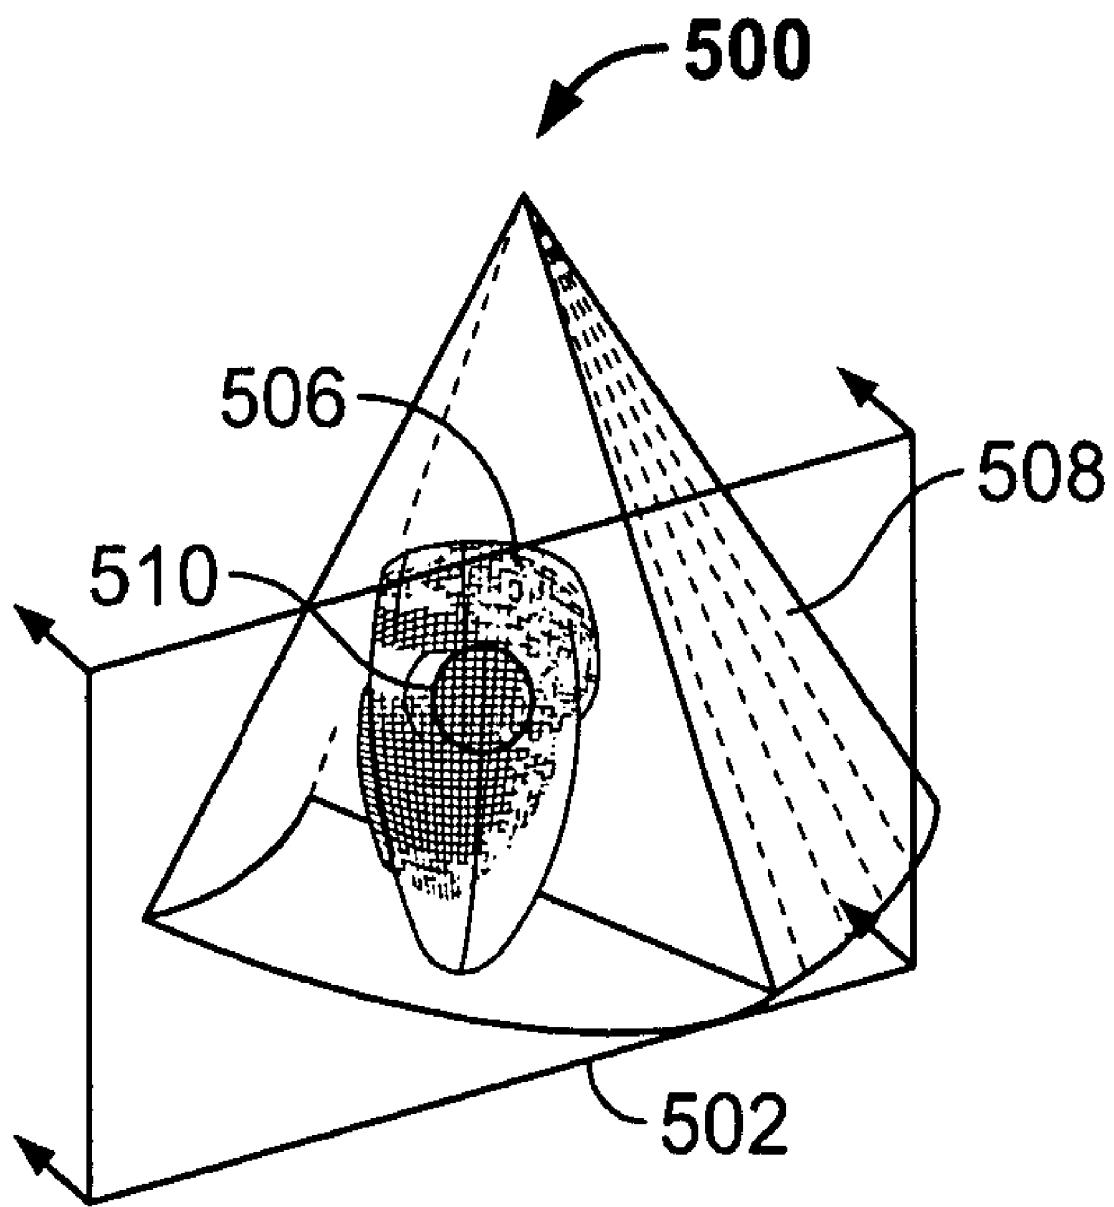


FIG. 2

**FIG. 3****FIG. 4****FIG. 5**

**FIG. 6****FIG. 7**

**FIG. 8**

METHOD AND APPARATUS FOR MEDICAL ULTRASOUND NAVIGATION USER INTERFACE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to and the benefit of the filing date of U.S. Provisional Application No. 60/581,675 filed on Jun. 22, 2004 and which is hereby incorporated by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] The present invention relates to diagnostic ultrasound methods and systems. In particular, the present invention relates to methods and systems for navigation in ultrasound data.

[0003] Numerous ultrasound methods and systems exist for use in medical diagnostics. Various features have been proposed to facilitate patient examination and diagnosis based on ultrasound images of the patient. For example, certain systems offer ultrasound volumetric imaging of an object, e.g. the human heart. To be useful, these systems require a navigator for orienting view planes within the volume data. Typically, the navigation of the view planes must be done after data acquisition.

[0004] Heretofore, ultrasound methods and systems were unable to acquire volumetric ultrasound data at the same time as an operator navigates in the volumetric data to generate 2D or 3D rendered images of the object.

[0005] A need exists for improved methods and systems that provide real time navigation in ultrasound volumetric data.

BRIEF DESCRIPTION OF THE INVENTION

[0006] One embodiment, an ultrasound system is provided that includes a probe having a 2D array of transducers for acquiring ultrasound information along a plurality of scan lines through an object in real time. The scan lines are arranged to define volumetric data corresponding to a volume of interest (VOI) in a subject or patient. One such VOI may include the human heart or some portion of the human heart. The system includes a beamformer configured with scan parameter values that define the scan lines. An image buffer stores multiple data volumes acquired over time that are successively retrieved and processed by a display processor. The display processor accesses the data volumes stored in the image buffer successively to control generation of at least one of 2D and 3D renderings based on display parameters, wherein the display processor obtains from the image buffer a first data volume defined based on first scan parameter values, while the probe acquires ultrasound information for a second data volume that is entered into the image buffer. The second data volume is defined based on second scan parameter values. A navigation view presents in real time the renderings generated by the display processor with their corresponding 3D orientation. A navigator is provided that controls the display of the navigation view in real time such that, as the user adjusts a display parameter value to change a view plane, images presented in the navigation view are updated to reflect the view plane. A user interface is provided for adjusting the scan and display parameter values.

[0007] In another embodiment, an ultrasound method is provided that acquires ultrasound information, utilizing a 2D array of transducers, along a plurality of scan lines through an object in real time, the scan lines being arranged to define data volumes within the object. The method includes defining the scan lines based on scan parameter values. The method stores multiple data volumes successively acquired over time in an image buffer, and includes adjustment of the values for the scan parameters. At least one of 2D and 3D images is presented based on the data volumes. The method accesses the data volumes stored in the image buffer successively to control presentation of the at least one of 2D and 3D images based on display parameters, wherein a first data volume defined based on first scan parameter values is obtained from the image buffer, while acquiring ultrasound information for a second data volume that is entered into the image buffer, the second data volume being defined based on second scan parameter values.

[0008] In yet another embodiment, an ultrasound system is provided that includes a probe having a 2D array of transducers for acquiring ultrasound information along a plurality of scan lines through an object in real time, the scan lines being arranged to define data volumes within the object. A beamformer having scan parameters that define the scan lines is provided, the scan parameters having parameter values. An image buffer stores multiple data volumes successively acquired over time. A display is provided for presenting at least one of 2D and 3D images based on the data volumes. A display processor accesses the data volumes stored in the image buffer successively to control presentation of the at least one of 2D and 3D images based on display parameters. A navigator is also provided that controls display of a navigation view in real time such that, as the user adjusts a display parameter value to change an orientation view, images presented on the display are updated to reflect the orientation view.

BRIEF DESCRIPTION OF THE DRAWINGS

[0009] FIG. 1 is a block diagram of an ultrasound system formed in accordance with an embodiment of the present invention.

[0010] FIG. 2 is a flowchart of an exemplary method supporting real time navigation of 2D and 3D rendering views produced and displayed from acquired volumetric data.

[0011] FIG. 3 is an illustration of a navigation view with a view plane looking into a volume from the left that may be produced by the system of FIG. 1.

[0012] FIG. 4 is an illustration of a navigation view with a view plane looking into the volume of FIG. 3 from the top.

[0013] FIG. 5 is an illustration of the navigation view of FIG. 4 with the view plane translated downwards.

[0014] FIG. 6 is an illustration showing a volume obtained with a selected width and elevation, the width and elevation selected through a user interface of the system of FIG. 1.

[0015] FIG. 7 is an illustration showing a changed volume obtained by changing the width and elevation for the volume of FIG. 6.

[0016] **FIG. 8** is an illustration of a navigation view of a heart as seen from a view plane selected by the user of the system of **FIG. 1**.

DETAILED DESCRIPTION OF THE INVENTION

[0017] **FIG. 1** is a block diagram of an ultrasound system **100** formed in accordance with an embodiment of the present invention. The ultrasound system **100** is configurable to acquire volumetric data corresponding to a volume of interest (VOI) in a subject or patient. One such VOI may include the human heart or some portion of the human heart. The ultrasound system **100** is configurable to acquire 3-dimensional (3D) volumes of data, each volume defined by an azimuth angle and elevation angle. The ultrasound system **100** includes a 2-dimensional (2D) array/matrix probe **102** that under the guidance of a beamformer **104** scans the VOI and acquires volumes of data at a rate of 15-30 volumes/sec, depending on the size of the volume (azimuth angle and elevation angle). The probe **102** receives backscattered echoes from the scanned object within the VOI and generates electrical receive signals that are combined in the beamformer **104** to form each beam/line within each scan plan. Multiple scan plans (differentiated by their elevation angle) combine to form a volume. The beamformer **104** outputs the beam information to an RF processor **106** that converts the beam information into ultrasound imaging data, e.g. B-mode information. The B-mode information generated from the RF processor **106** is stored in an image buffer **108**. The image buffer **108** is a ring buffer that stores each acquired volume at a rate depending upon the size of each volume. Each volume in the image buffer **108** is given a time stamp.

[0018] While B-mode information is stored in the image buffer **108**, previously stored B-mode information is retrieved and made available, a volume at a time, to a display processor **110** and a navigator **114**. The display processor **110** and the navigator **114** receive the same set of inputs, e.g. a set of scan parameters **116**, a set of display parameters **118**, and volume data from the image buffer **108** for processing. The image buffer **108** is a ring buffer in that the buffer **108** wraps around on itself. When the last storage location in the buffer **108** is reached, the beginning location in the buffer **108** is next addressed. Volumetric information is retrieved from the buffer **108** by the display processor **110** and the navigator **114** at a rate that prevents overwriting of information in the image buffer **108**.

[0019] The display processor **110** processes the volume information retrieved from the image buffer **108** to form a rendering such as, for example, a volume rendering or a slice (cut) plane rendering, that is displayed in a rendering view **122** of a computer display **112**. The rendering view **122** displays an image of the scanned object as would be seen from a desired orientation or view plane (direction of view) as determined by the display parameters **118**. The orientation or view plane from which the rendering view **122** is formed and displayed may be displayed to the user by a navigation view **124** in the computer display **112**. The navigator **114** generates and controls the navigation view **124** that is displayed on the computer display **112**. The navigation view **124** may show a high level view of the scanned object and the orientation or direction of view of the scanned object by positioning the scanned object with respect to a set of planes

or slices, such as a set of orthogonal planes or slices that form a Cartesian reference system.

[0020] The user through a user interface **120** may change the scan parameters **116** and/or the display parameters **118**. The navigator **114** controls the orientation shown in the navigation view **124** based on the values of the display parameters **118**. When changing the navigation view **124** by changing the display parameters **118**, the display of the rendering view **122** is correspondingly changed to show the scanned object as formed and seen from the new view direction and/or orientation. Thus, the user may navigate and change the direction of view and/or orientation of the scanned object as is displayed in the navigation view **124**, and in so doing, change the view of the scanned object that is displayed in the rendering view **122**. The display of the scanned object shown in rendering view **122** is aligned to agree and correspond with the new view orientation that is shown in the navigation view **124**. Direction of view (the navigation view **124**) may be changed while new volume data is being acquired and stored in the image buffer **108**. The user is able to navigate in real time the view or perspective being displayed of the scanned object while the object is being scanned. The lag time to see changes made in the display parameters **118** (changes in the viewing direction and/or orientation) update the rendering view **122** and the navigation view **124** depends on the time required to generate new renderings. Unlike changing the scan parameters **116**, changing the display parameters **118** does not affect the configuration of the beamformer **104**.

[0021] **FIG. 2** is a flowchart **200** of an exemplary method supporting real time navigation of 2D and 3D rendering views **122** produced and displayed in the computer display **112** from acquired volumetric data. At **202**, a plurality of scan planes is defined based on values assigned to the scan parameters **116**. The scan parameters **116** include such variables as, for example, scan depth, width (azimuth angle), elevation angle, number of beams (beam density) in elevation and in azimuth, number of samples/beam, and mode. The user may define the values for the scan parameters **116** through the user interface **120**, such as through the use of a keyboard, trackball, and/or mouse, and may update the scan parameters **116** in real time during the ultrasound scanning. New scan parameter values are provided to the display processor **110** and the navigator **114**. The lag time for seeing the effect of having changed the values of the scan parameters **116** is from 1 to 2 seconds, time being needed to configure the beamformer **104** with the new scan parameters **116**.

[0022] At **204**, ultrasound information is acquired by utilizing a probe with a 2D array of transducers to collect scan information along a plurality of scan plans through a scanned object. The scanning is performed in real time in that no manual repositioning of the probe is needed in order to acquire all the scan planes that form a data volume. Each scan plan of the volume is differentiated from another by the elevation angle of the beam lines producing the scan plan. The width of the scan plan is determined by an azimuth angle. A volume of scan data may be produced by varying the elevation angle of the scan to generate a plurality of scan planes through the scanned object at different elevations.

[0023] At **206**, multiple data volumes are successively stored as acquired over time in the image buffer **108**. As

related for **FIG. 1**, the image buffer **108** is a ring buffer with data volumes being extracted and used by the display processor **110** and the navigator **114** while data volumes are being stored in the image buffer **108**.

[0024] At **208**, the 2D or 3D rendering view **122** is presented in the computer display **112** as formed by the display processor **110** based on the scanned volume, the scan parameters **116**, and the display parameters **118**. At **210** the user may adjust the scan parameters **116** to obtain a wider or narrower scan of the scanned object, or to obtain a scan with a greater density of beams/lines in a scan plane or the elevation (number of scan planes per volume).

[0025] At **210**, the user adjusts the scan parameters **116** and, as the user makes adjustments, the effects of the adjustments as displayed in the rendering view **122** are presented **208** in the computer display **112**. The effects of the adjustments to the scan parameters **116** may be viewed in about 1 or 2 seconds from having entered the adjustments. The time of 1 or 2 seconds may be needed in order to reconfigure the beamformer **104** with the new scan parameters **116**, acquire and store new volume data in the image buffer **108**, retrieve and process the new volume data from the image buffer **108** by the display processor **110**, and present the updated rendering view **122** in the computer display **112**. When the user is satisfied with the size and quality of display of the scanned object in the rendering view **122**, the user may want to view the scanned object from a different direction and/or orientation.

[0026] At **212**, data volumes are successively accessed from the image buffer **108**, and with the current valuing of the scan parameters **116** and the display parameters **118**, the rendering view **122** and the navigation view **124** are displayed in the computer display **112**. The navigator **114** uses the display parameters **118** to define the orientation or direction of view (view plane) and to display the view plane as part of the navigation view **124** in the computer display **112**. The user may adjust the display parameters **118** through the user interface **120** similarly to how the scan parameters **116** are adjusted. Examples of display parameters may include view direction, rotation translation, tilt, zoom factor, and number of images viewed. Both the display processor **110** and the navigator **114** read the display parameters **118**. The navigator **114** produces a view plane or angle of view with a view of the scanned object in the navigation view **124**. The rendering view **122** may be an enlarged view of the scanned object in comparison to the scanned object shown in the navigation view **124**. The rendering view **122** and the navigation view **124** may each be displayed in a quadrant of the computer display **112**.

[0027] Real time navigation is obtained by successively accessing data volumes stored in the image buffer **108** and scan parameter values stored in **116** and presenting at least one of 2D and 3D images based on display parameters **118**, wherein each image that is displayed is defined based on separate display parameter values stored in display parameters **118**.

[0028] **FIG. 3** is an illustration of a navigation view **300** with a view plane **310** looking into a volume **308** from the left that may be produced by the system **100** of **FIG. 1**. The navigation view **300** shows an image of a heart valve **306** generated as seen from viewing into a volume **308** from the left. The view plane **310**, is shown as a table top with four

arrows for legs, and indicates to the user that the image of the heart valve **306** is produced by looking perpendicularly through the view plane **310** (perpendicularly through the table top) into the volume **308**. The image of the heart valve **306** may be formed by use of various techniques, such as slice (cut plane) imaging, surface rendering, and the like. The user may change the orientation of the view plane **310** with respect to the volume **308** by rotating and/or translating the view plane **310**. For example, the view plane **310** may be reoriented about the volume **308** to obtain a view plane **312** and view of the heart valve **306** as shown in **FIG. 4**.

[0029] **FIG. 4** is an illustration of a navigation view **302** with a view plane **312** looking into the volume **308** from the top. A translation and/or rotation of the view plane **310** of **FIG. 3** obtains the view plane **312** of **FIG. 4**. Shown in **FIG. 4** is an object **314** between the view plane **312** and the heart valve **306**. The view from the view plane **312** includes the object **314** which may obstruct the view of a portion of the heart valve **306**. The generated image of the heart valve **306** has the object **314** obstructing the view of the heart valve **306**. The obstructed view may be resolved by translating the view plane **312** downward as shown in **FIG. 5**.

[0030] **FIG. 5** is an illustration of the navigation view **302** of **FIG. 4** with the view plane **312** translated downward. The view plane **312** of navigation view **302** has been lowered down (translated downward) to be closer to the heart valve **306** in **FIG. 5**. The new view plane **316** is positioned below the obstructing object **314** to result in an image of the heart valve **306** that is no longer obstructed by the object **314**. By translating the view plane **312** downward to obtain the view plane **316**, the user has eliminated use of the volumetric scan data that contains the obstructing object **314** in forming the view or image of the heart valve **306**. The user may change the values of display parameters **118** through the use of the user interface **120** of **FIG. 1** to reorient the view plane **312**. Reorientation may result in a view of the heart valve **306** from a different angle and/or without obstructing objects within the view.

[0031] **FIG. 6** is an illustration **400** showing a volume **401** obtained with a selected width **410** (azimuth angle θ) and elevation **408** (elevation angle ϕ), the width **410** and elevation **408** selected by the user through the user interface **120** of the system **100** of **FIG. 1**. The volume **401** is determined from the width **410** (the azimuth angle θ) of a scan slice **416** and the elevation **408** (the elevation angle ϕ) for the scan slice **416**. **FIG. 6** shows a view plane **404** through which an image of a heart valve **406** is defined and displayed. When observing the display of the heart valve **406**, the user or sonographer may desire to display more of the heart valve **406** or more area surrounding the heart valve **406**, but with the view remaining unchanged. A larger view of the heart valve **406** may be obtained as shown in **FIG. 7**.

[0032] **FIG. 7** is an illustration **402** showing a changed volume **403** obtained by changing the width **410** and elevation **408** for the volume **401** of **FIG. 6**. In **FIG. 7**, a shortened width **414** and increased elevation **412** through which scan slices **416** are obtained is specified by the user to obtain the changed volume **403**. Without changing the view plane **404** of **FIG. 6**, a larger view of the heart valve **406** is obtained by increasing the volume **403** of the scan.

[0033] **FIG. 8** is an illustration of a navigation view **500** of a heart **506** as seen from a view plane **502** selected by the

user of the system 100 of **FIG. 1**. The heart 506 is shown with an aortic structure 510 facing the view plane 502. The image of the heart 506 in the navigation view 500 may be generated as a surface rendering. In an alternative embodiment, the image shown of the heart 506 may not be a generic surface model, but instead may be a calibrated model of a heart.

[0034] The system 100 may generate a model of a heart constructed from a plurality of polygons and position the heart model in the location of the heart 506. To be useful, the heart model is scaled based on data from the patient. Data may be manually measured or automatically determined to scale the size of the heart model based on actual size of the patient's heart. For example, the actual size of the patient's heart may be determined based on three landmarks in data (e.g. two points on the mitral ring and the aortic output) and apex. The generated heart model is positioned and oriented within the volume 508 according to the landmarks in the volume data. Thus, the navigation view 500 may show a heart 506 that is a calibrated scale model of the patient's heart positioned and oriented correctly within the volume 508. Corresponding to the view plane 502 of the navigation view 500, a rendering view (not shown in the figure) may show 2D or 3D images derived from the ultrasound scan data. The view plane 502 may intersect the heart model.

[0035] Exemplary embodiments of diagnostic ultrasound systems and methods are described above in detail. The systems and methods are not limited to the specific embodiments described herein, but rather, components of each system may be utilized independently and separately from other components described herein. Each system component can also be used in combination with other system components.

[0036] While the invention has been described in terms of various specific embodiments, those skilled in the art will recognize that the invention can be practiced with modification within the spirit and scope of the claims.

What is claimed is:

1. An ultrasound system, comprising:

a probe having a 2D array of transducers acquiring ultrasound information along a plurality of scan lines through an object in real time, said scan lines being arranged to define data volumes within the object;

a beamformer having scan parameters that define said scan lines, said scan parameters having parameter values;

an image buffer storing multiple data volumes successively acquired over time;

a display processor accessing said data volumes stored in said image buffer successively to control generation of at least one of 2D and 3D renderings based on display parameters, wherein said display processor obtains from said image buffer a first data volume defined based on first scan parameter values, while said probe acquires ultrasound information for a second data volume that is entered into said image buffer, said second data volume being defined based on second scan parameter values;

a navigation view presenting in real time the said renderings generated by said display processor with their corresponding 3D orientation;

a navigator controlling display of said navigation view in real time such that, as the user adjusts a display parameter value to change a view plane, images presented in said navigation view are updated to reflect said view plane; and

a user interface for adjusting said scan and display parameter values.

2. The ultrasound system of claim 1, wherein said user interface permits a user to adjust said scan parameters from said first parameter values to said second parameter values while viewing said at least one of 2D and 3D renderings based on volume data being acquired in real time.

3. The ultrasound system of claim 1, wherein said image buffer simultaneously stores at least one data volume defined by said first parameter values and at least one data volume defined by said second parameter values.

4. The ultrasound system of claim 1, wherein said image buffer is substantially simultaneously accessed by said display processor to read said data volumes from said image buffer and by said beamformer to write said data volumes to said image buffer.

5. The ultrasound system of claim 1, wherein said display presents at least one of volume rendered images, surface rendered images and cut plane images.

6. The ultrasound system of claim 1, further comprising a navigator controlling display of a navigation view indicating at least one of view planes, object models and landmarks relative to the said data volume, said navigation view being defined based on said data volume data, scan and display parameter values.

7. The ultrasound system of claim 1, wherein said probe continues to acquire new data volumes as display parameters values for said display parameters are changed.

8. The ultrasound system of claim 1, wherein a lag time after changing display parameter values before displaying updated images based on new display parameter values is no more than $\frac{1}{4}$ second.

9. The ultrasound system of claim 1, wherein a lag time after changing scan parameter values before displaying updated images based on new scan parameter values is no more than 2 seconds.

10. The ultrasound system of claim 1, wherein said image buffer stores a time stamp with each of said data volumes, said time stamp identifying a time at which said data volume was acquired.

11. An ultrasound method, comprising:

acquiring ultrasound information, utilizing a 2D array of transducers, along a plurality of scan lines through an object in real time, said scan lines being arranged to define data volumes within the object;

defining said scan lines based on scan parameters having scan parameter values;

storing multiple data volumes successively acquired over time in an image buffer;

adjusting said scan parameter values for said scan parameters;

presenting at least one of 2D and 3D images based on said data volumes; and

accessing said data volumes stored in said image buffer successively to control presentation of said at least one of 2D and 3D images based on display parameters, wherein a first data volume defined based on first scan parameter values is obtained from said image buffer, while acquiring ultrasound information for a second data volume that is entered into said image buffer, said second data volume being defined based on second scan parameter values.

12. The ultrasound method of claim 11, further comprising permitting a user to adjust said scan parameters from said first parameter values to said second parameter values while viewing 2D images being acquired in real time.

13. The ultrasound method of claim 11, further comprising simultaneously storing at least one data volume defined by said first parameter values and at least one data volume defined by said second parameter values.

14. The ultrasound method of claim 11, further comprising substantially simultaneously accessing said image buffer to read said data volumes from said image buffer and writing said data volumes to said image buffer.

15. The ultrasound method of claim 11, further comprising presenting at least one of volume rendered images, surface rendered images and cut plane images.

16. The ultrasound method of claim 11, further comprising controlling display of a navigation view indicating at least one of view planes, object models and landmarks relative to said data volume, said navigation view being defined based on said data volume, scan and display parameter values.

17. The ultrasound method of claim 11, further comprising continuing to acquire new data volumes as display parameters values for said display parameters are changed.

18. The ultrasound method of claim 11, wherein a lag time after changing display parameter values before displaying updated images based on new display parameter values is no more than $\frac{1}{4}$ second.

19. The ultrasound method of claim 11, wherein a lag time after changing scan parameter values before displaying updated images based on new scan parameter values is no more than 2 seconds.

20. The ultrasound method of claim 11, further comprising storing a time stamp with each of said data volumes, said time stamp identifying a time at which said data volume was acquired.

21. An ultrasound system, comprising:

a probe having a 2D array of transducers acquiring ultrasound information along a plurality of scan lines through an object in real time, said scan lines being arranged to define data volumes within the object;

a beamformer having scan parameters that define said scan lines, said scan parameters having parameter values;

an image buffer storing multiple data volumes successively acquired over time;

a display for presenting at least one of 2D and 3D images based on said data volumes;

a display processor accessing said data volumes stored in said image buffer successively to control presentation of said at least one of 2D and 3D images based on display parameters; and

a navigator controlling display of a navigation view in real time such that, as the user adjusts a display parameter value to change an orientation view, images presented on said display are updated to reflect said orientation view.

* * * * *

专利名称(译)	用于医学超声导航用户界面的方法和装置		
公开(公告)号	US20050283079A1	公开(公告)日	2005-12-22
申请号	US10/926547	申请日	2004-08-26
[标]申请(专利权)人(译)	STEEN ERIK TORKILDSEN RUNE MARTENS DITLEF		
申请(专利权)人(译)	STEEN ERIK TORKILDSEN RUNE MARTENS DITLEF		
当前申请(专利权)人(译)	通用电气公司		
[标]发明人	STEEN ERIK NORMANN TORKILDSEN RUNE MARTENS DITLEF		
发明人	STEEN, ERIK NORMANN TORKILDSEN, RUNE MARTENS, DITLEF		
IPC分类号	A61B8/14 A61B8/02		
CPC分类号	A61B8/0883 A61B8/14 A61B8/145 A61B8/4483 A61B8/463 G01S15/8993 A61B8/467 A61B8/483 G01S7/52074 G01S7/52085 A61B8/466 A61B8/461		
优先权	60/581675 2004-06-22 US		
其他公开文献	US7604595		
外部链接	Espacenet USPTO		

摘要(译)

在一个实施例中，提供了一种超声系统，其包括具有2D换能器阵列的探头，用于沿着穿过物体的多个扫描线实时采集超声信息。扫描线被布置成限定对应于受试者或患者中的感兴趣体积(VOI)的体积数据。一种这样的VOI可以包括人的心脏或人的心脏的某些部分。该系统包括配置有定义扫描线的扫描参数值的波束形成器。图像缓冲器存储随时间获取的多个数据量，这些数据量由显示处理器连续检索和处理。显示处理器连续访问存储在图像缓冲器中的数据量，以基于显示参数控制2D和3D渲染中的至少一个的生成，其中显示处理器从图像缓冲器获得基于第一扫描参数值定义的第一数据量，探针获取输入图像缓冲区的第二数据量的超声信息。基于第二扫描参数值定义第二数据量。导航视图实时呈现由显示处理器生成的渲染及其对应的3D方向。提供导航器，其实时控制导航视图的显示，使得当用户调整显示参数值以改变视平面时，导航视图中呈现的图像被更新以反映视图平面。提供用户界面以调整扫描和显示参数值。

