




US 20170202580A1

(19) **United States**(12) **Patent Application Publication**
YOSHIMINE(10) **Pub. No.: US 2017/0202580 A1**(43) **Pub. Date: Jul. 20, 2017**(54) **ULTRASONIC PROBE****Publication Classification**(71) Applicant: **OLYMPUS CORPORATION**, Tokyo
(JP)(51) **Int. Cl.**
A61B 17/56 (2006.01)
A61B 18/00 (2006.01)(72) Inventor: **Hideto YOSHIMINE**, Hachioji-shi (JP)(52) **U.S. Cl.**
CPC **A61B 17/56** (2013.01); **A61B 18/00**
(2013.01)(73) Assignee: **OLYMPUS CORPORATION**, Tokyo
(JP)(21) Appl. No.: **15/480,022**(22) Filed: **Apr. 5, 2017****Related U.S. Application Data**(63) Continuation of application No. PCT/JP2015/
076183, filed on Sep. 15, 2015.(30) **Foreign Application Priority Data**

Jan. 7, 2015 (JP) 2015-001839

(57) **ABSTRACT**

A curving section is always disposed in a projection plane of a probe main body section. The curving section includes a first bending surface which bends relative to a peripheral surface of the probe main body section to approach a longitudinal axis, thereby intersecting the longitudinal axis; a second bending surface which bends relative to the first bending surface toward a bending direction of the first bending surface and a direction away from the longitudinal axis; a third bending surface which bends relative to the second bending surface toward a direction to approach the longitudinal axis on a side reverse to the bending direction of the first bending surface, and extends toward an extension line of the first bending surface.

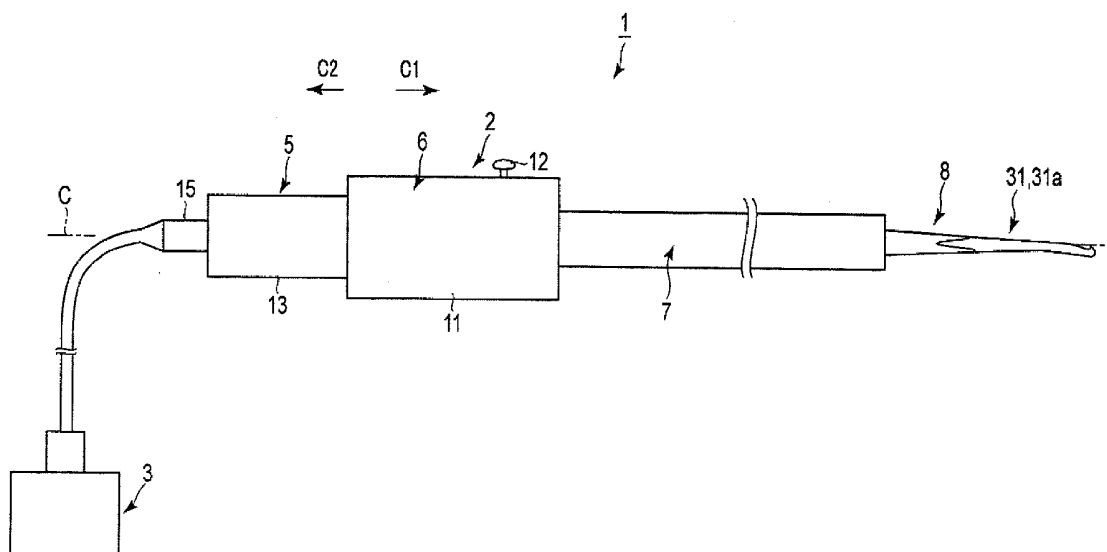

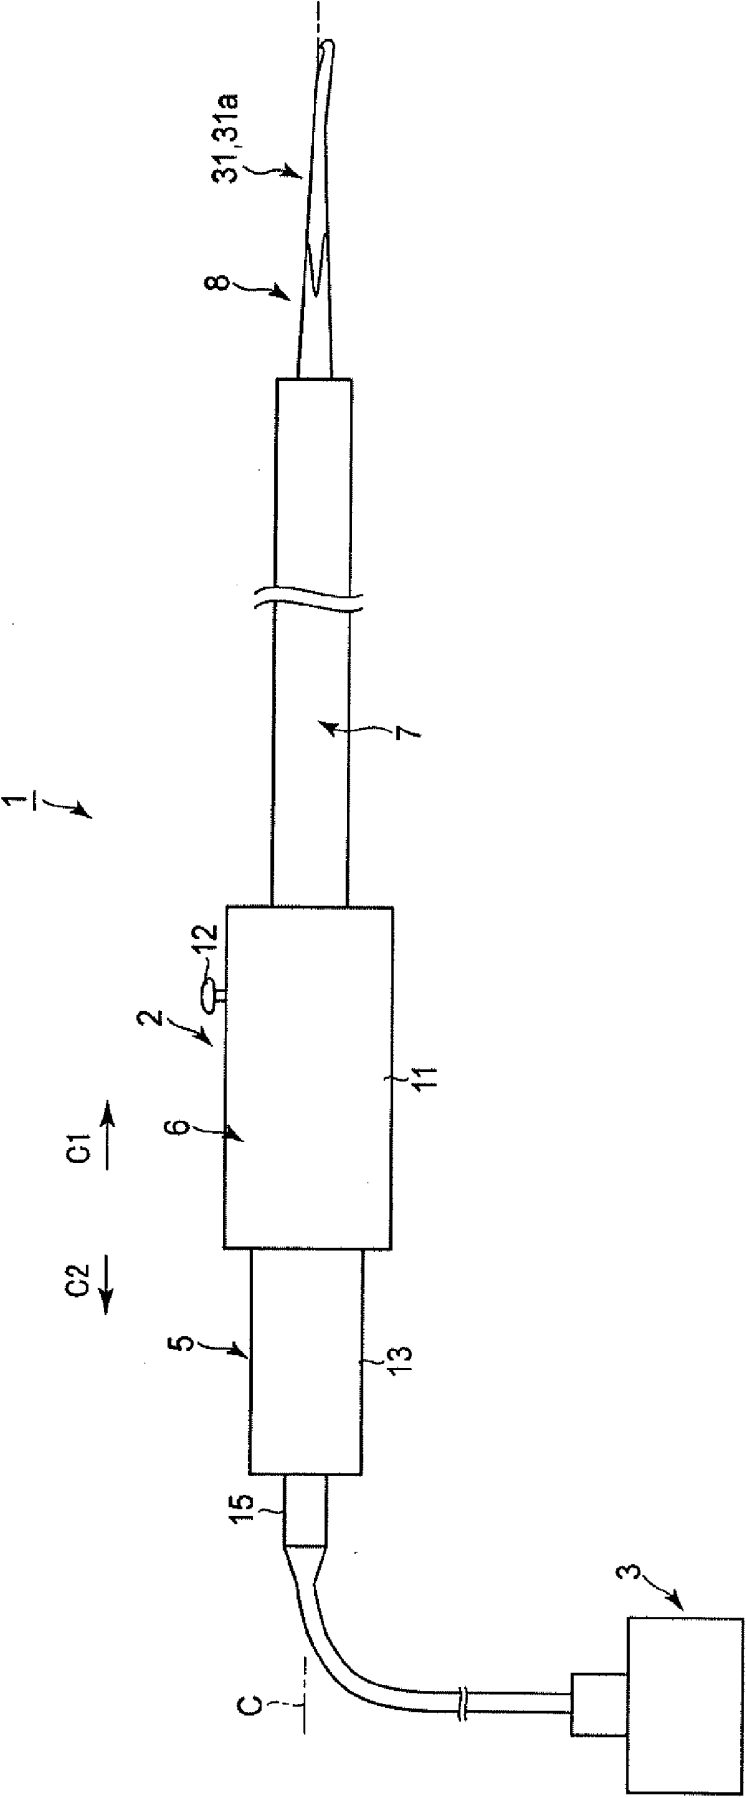


FIG.1


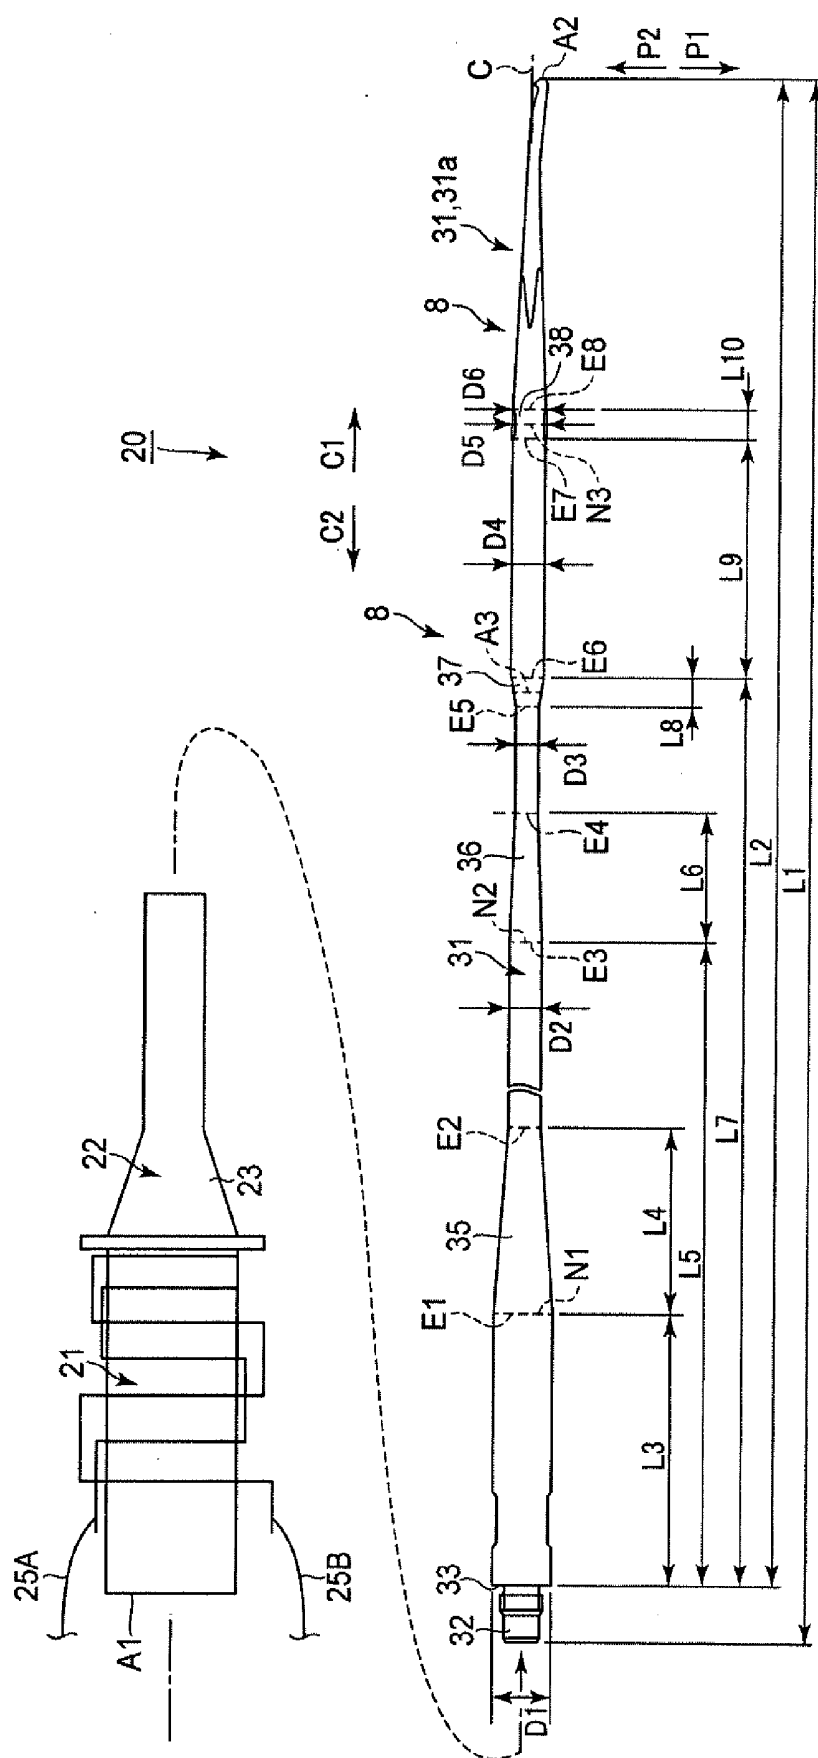


FIG. 2

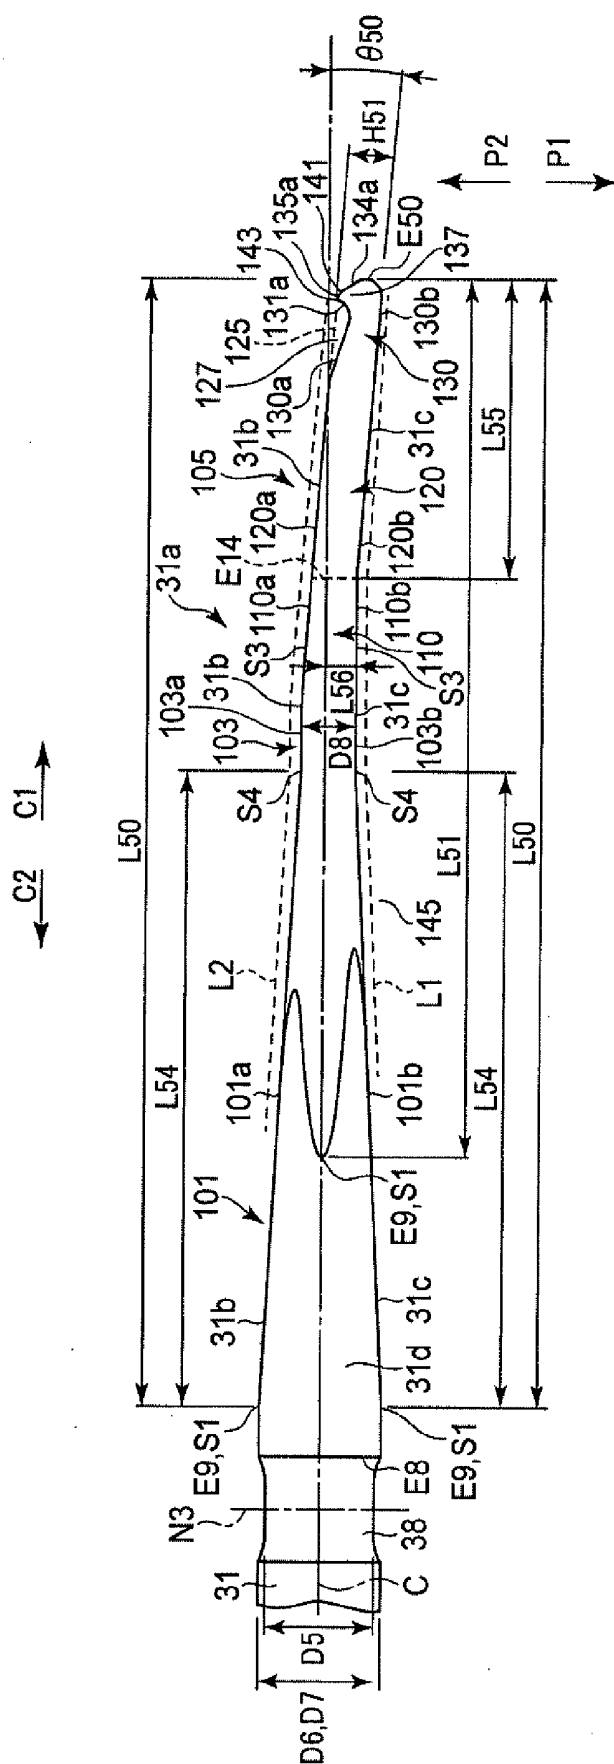

F1G.3

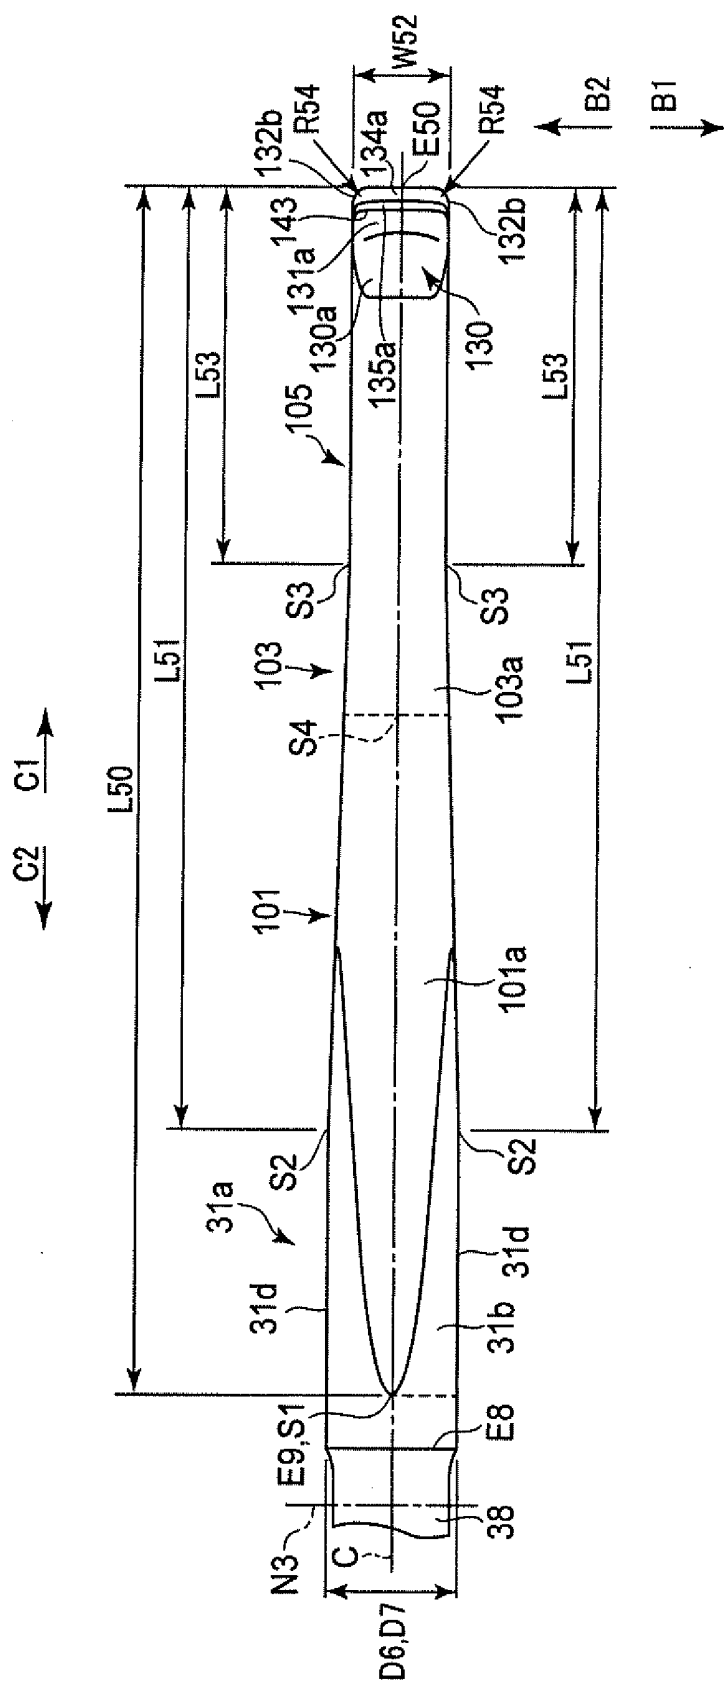


FIG. 4

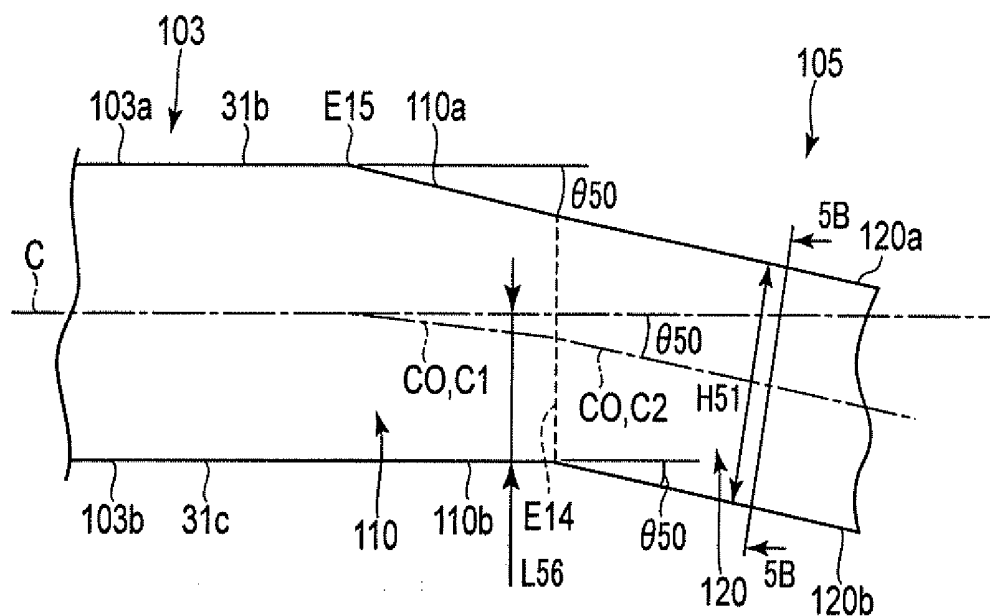


FIG. 5A

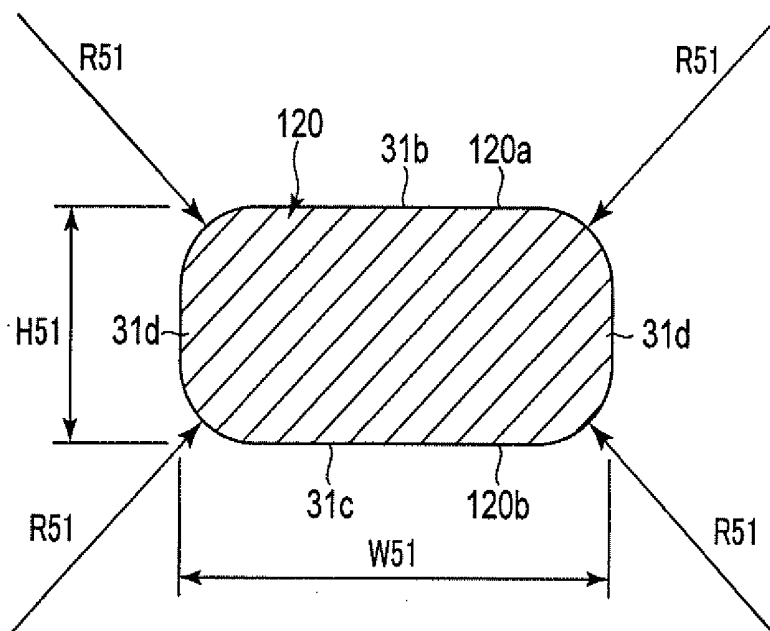


FIG. 5B

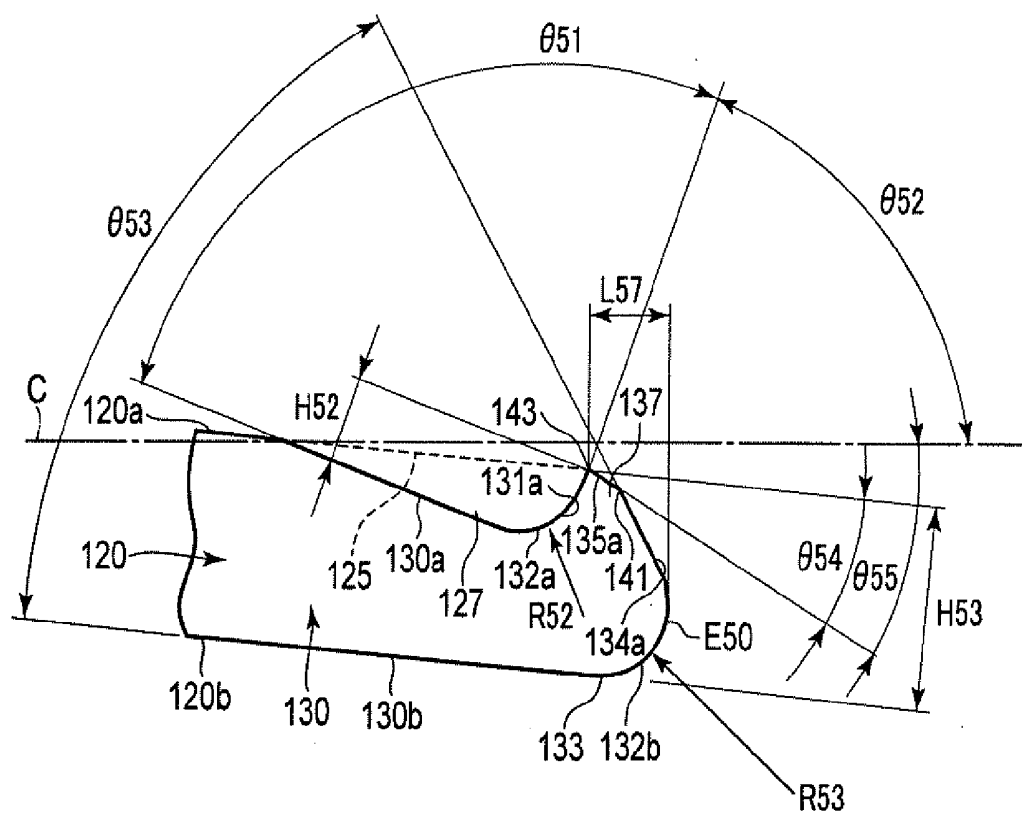


FIG. 6

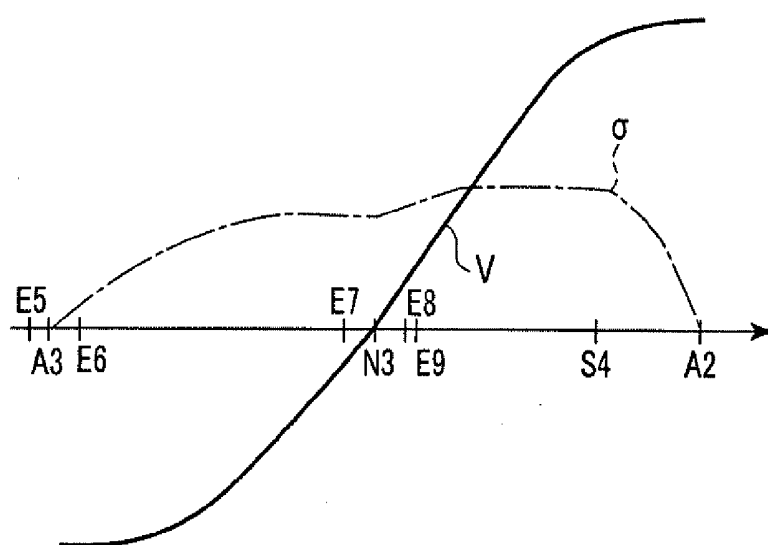


FIG. 7

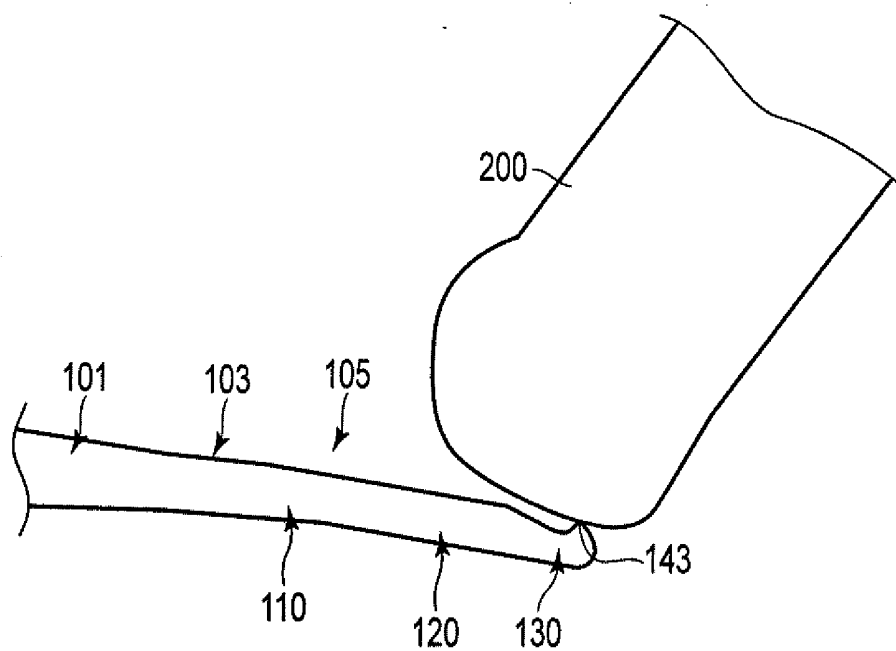


FIG. 8A

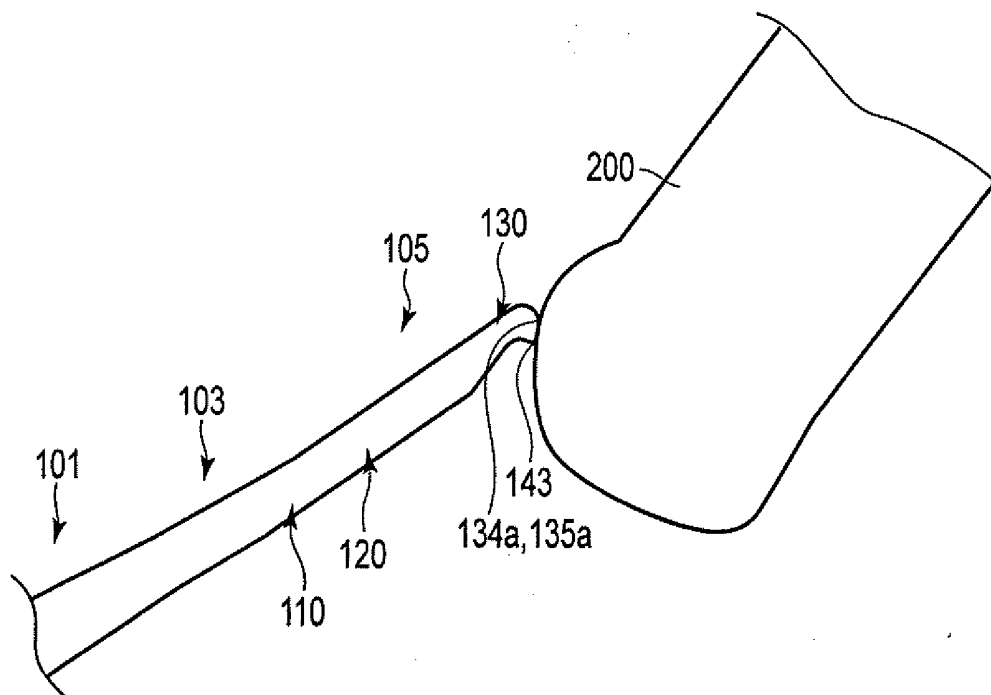


FIG. 8B

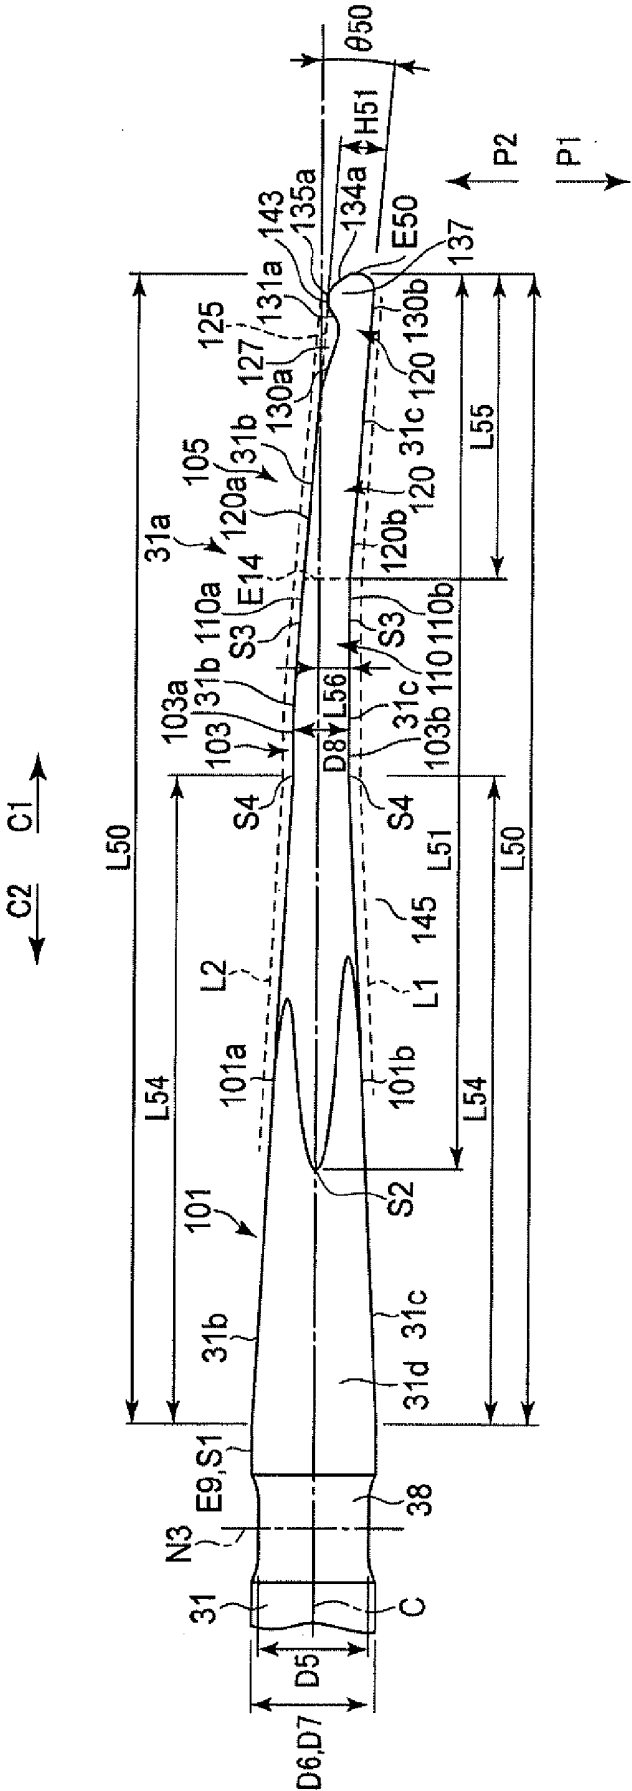


FIG. 9



FIG. 10

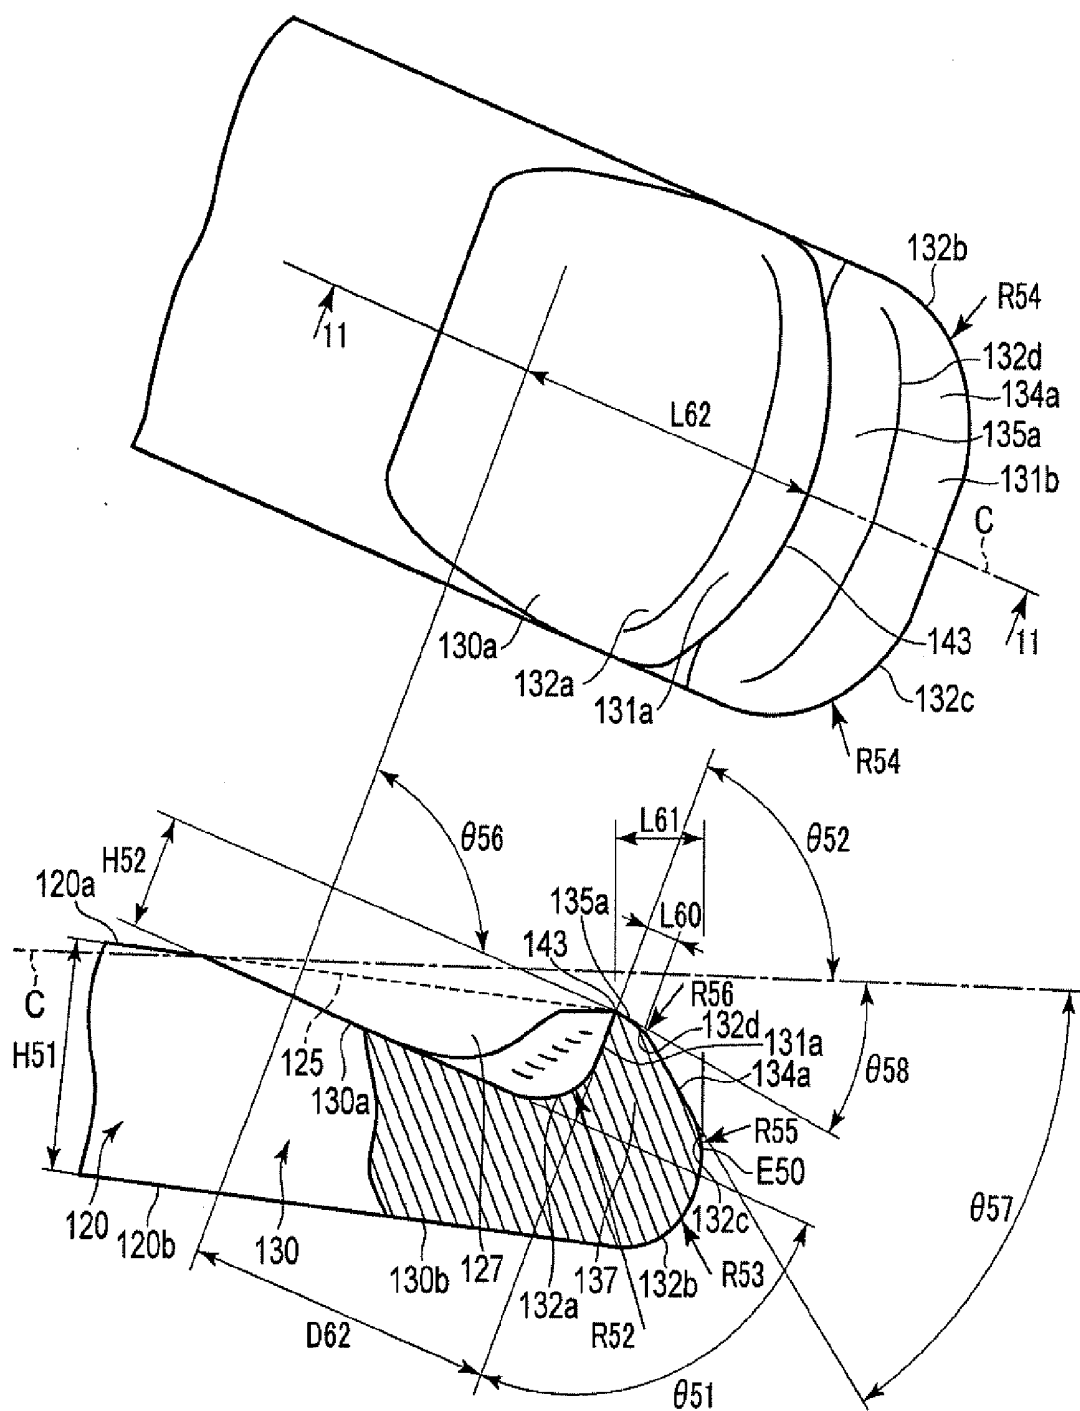


FIG. 11

ULTRASONIC PROBE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a Continuation Application of PCT Application No. PCT/JP2015/076183, filed Sep. 15, 2015 and based upon and claiming the benefit of priority from prior Japanese Patent Application No. 2015-001839, filed Jan. 7, 2015, the entire contents of all of which are incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention

[0003] The present invention relates to an ultrasonic probe to perform cutting of, for example, a hard bone tissue and a cartilage tissue by ultrasonic vibration.

[0004] 2. Description of the Related Art

[0005] In Jpn. Pat. Appln. KOKAI Publication No. 2005-152098, there is disclosed an ultrasonic treatment system including an ultrasonic probe (an ultrasonic horn). In this ultrasonic treatment system, an ultrasonic vibration generated in a vibration generating section (an ultrasonic vibration mechanism) is transmitted from a proximal toward a distal in the ultrasonic probe. In a distal portion of the ultrasonic probe, a scalpel portion is formed as a planar treating region.

[0006] In the scalpel portion, an outer surface of the ultrasonic probe is formed in an uneven state. The ultrasonic vibration is transmitted to the scalpel portion in a state where the scalpel portion is in contact with a treatment target, whereby an affected area is cut. The affected area is, for example, a bone or another hard tissue.

BRIEF SUMMARY OF THE INVENTION

[0007] According to an ultrasonic probe of one aspect of the invention, the ultrasonic probe for a knee joint transmits ultrasonic vibration to treat the knee joint by the ultrasonic vibration, the ultrasonic probe includes a probe main body section which is extended along a longitudinal axis and to which the ultrasonic vibration is transmitted from its proximal end to its distal end; and a curving section which has a central axis bending relative to the longitudinal axis of the probe main body section, is continuous with a distal portion of the probe main body section, and is bent relative to the probe main body section, wherein the curving section is always disposed in a projection plane of the probe main body section, when the probe main body section is seen along the longitudinal axis from the proximal end toward the distal end, the curving section includes: a treating section having a treating region and disposed in a distal portion of the curving section; a first bending surface which is continuous with the treating section, and bends relative to a peripheral surface of the probe main body section to approach the longitudinal axis, thereby intersecting the longitudinal axis; a second bending surface which is disposed in the treating section, and bends relative to the first bending surface toward a bending direction of the first bending surface and a direction away from the longitudinal axis; a third bending surface which is disposed in the treating section, bends relative to the second bending surface toward a direction to approach the longitudinal axis on a side reverse to the bending direction of the first bending surface, and extends toward an extension line of the first bending surface; and a first treating surface which is disposed in the

treating section, and bends relative to the third bending surface in the bending direction of the first bending surface, and the treating region is disposed in a continuous region of the third bending surface with the first treating surface, and is positioned on the extension line of the first bending surface or positioned on a side opposite to the longitudinal axis with respect a boundary that is the extension line of the first bending surface.

[0008] Advantages of the invention will be set forth in the description which follows, and in part will be obvious from the description, or may be learned by practice of the invention. Advantages of the invention may be realized and obtained by means of the instrumentalities and combinations particularly pointed out hereinafter.

BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING

[0009] The accompanying drawings, which are incorporated in and constitute a part of the specification, illustrate embodiments of the invention, and together with the general description given above and the detailed description of the embodiments given below, serve to explain the principles of the invention.

[0010] FIG. 1 is a view showing an ultrasonic treatment system according to a first embodiment of the present invention;

[0011] FIG. 2 is a view showing a constitution of a vibrating body unit;

[0012] FIG. 3 is a side view of a distal portion of a probe main body section according to the first embodiment;

[0013] FIG. 4 is a top plan view of the distal portion of the probe main body section according to the first embodiment;

[0014] FIG. 5A is an enlarged view around a sectional area decreasing portion shown in FIG. 3;

[0015] FIG. 5B is a cross-sectional view along the 5B-5B line shown in FIG. 5A;

[0016] FIG. 6 is an enlarged view around a treating section shown in FIG. 3;

[0017] FIG. 7 is a schematic view showing an amplitude of a longitudinally vibration and stress due to an ultrasonic vibration between a second distal vibration antinode and a most distal vibration antinode in a state where the vibrating body unit according to the first embodiment longitudinally vibrates in an predetermined frequency range;

[0018] FIG. 8A is a view showing one example of a treatment of the ultrasonic probe;

[0019] FIG. 8B is a view showing one example of a treatment of the ultrasonic probe;

[0020] FIG. 9 is a side view of a distal portion of a probe main body section according to a second embodiment; FIG. 10 is a top plan view of the distal portion of the probe main body section according to the second embodiment; and

[0021] FIG. 11 shows an enlarged view around a treating section shown in FIG. 10 and a cross-sectional view along the 11-11 line shown in FIG. 11.

DETAILED DESCRIPTION OF THE INVENTION

[0022] Hereinafter, embodiments of the present invention will be described in detail with reference to the drawings.

First Embodiment

[0023] A first embodiment will be described with reference to

[0024] FIG. 1, FIG. 2, FIG. 3, FIG. 4, FIG. 5A, FIG. 5B, FIG. 6, FIG. 7, FIG. 8A and FIG. 8B. It is to be noted that in parts of drawings, diagrammatic representation of members of parts is omitted or simplified for clarification of the diagrammatic representation. In FIG. 3, a range shown with a broken line F1 and a broken line F2 projects to a distal side with respect to a distal end of a sheath 7.

[0025] FIG. 1 is a view showing an ultrasonic treatment system 1 of the present embodiment. As shown in FIG. 1, the ultrasonic treatment system 1 includes an ultrasonic treatment instrument (a hand piece) 2, an energy control device 3, and a transducer unit 5. The ultrasonic treatment instrument 2 has a longitudinal axis C. Here, a direction parallel to the longitudinal axis C is a longitudinal axis direction. One side of the longitudinal axis direction is a distal side (an arrow C1 direction of FIG. 1), and a side opposite to the distal side is a proximal side (an arrow C2 direction of FIG. 1). The ultrasonic treatment instrument 2 of the present embodiment is, for example, for use in treating a knee joint by ultrasonic vibration.

[0026] The ultrasonic treatment instrument 2 includes a holding unit 6, the sheath 7, and an ultrasonic probe 8. The holding unit 6 includes a holding casing 11 to be held by an operator, and an energy operating button 12 that is an energy operation input section attached to the holding casing 11 and configured to be operated by the operator. The sheath 7 that is a hollow tubular member extending along the longitudinal axis C is coupled with the distal side of the holding unit 6. The ultrasonic probe (a vibration transmitting member) 8 is inserted through the sheath 7. It is to be noted that a distal portion of the ultrasonic probe 8 projects from a distal end of the sheath 7 toward the distal side. The ultrasonic probe 8 is, for example, an ultrasonic probe for the knee joint to which the ultrasonic vibration is transmitted to treat the knee joint by the ultrasonic vibration.

[0027] Furthermore, the transducer unit 5 having a transducer case 13 is coupled with the proximal side of the holding unit 6. The transducer unit 5 is connected to one end of a cable 15. The other end of the cable 15 is connected to the energy control device 3. The energy control device 3 is, for example, an energy treatment device. The energy control device 3 includes an electric power source, a conversion circuit to convert an electric power from the electric power source into a vibration generating electric power, a processor (a control section) including a CPU (central processing unit) or an ASIC (application specific integrated circuit), and a storage medium such as a memory. Inside the holding casing 11, there is disposed a switch (not shown) in which an ON/OFF state is changed by an input of an energy operation in the energy operating button 12. The switch is electrically connected to the processor of the energy control device 3 via a signal route extending through the transducer unit 5 and an inside of the cable 15. Furthermore, in the ultrasonic treatment system 1, a vibrating body unit 20 extends through an inside of the holding casing 11 and an inside of the transducer case 13.

[0028] FIG. 2 is a view showing a constitution of the vibrating body unit 20. As shown in FIG. 2, the vibrating body unit 20 includes the ultrasonic probe 8 mentioned above, an ultrasonic transducer 21 that is a vibration generating section constituted of piezoelectric elements, and a

relay transmitting member 22. The ultrasonic transducer 21 and the relay transmitting member 22 are arranged in the transducer case 13, and the relay transmitting member 22 is supported by the transducer case 13. The ultrasonic transducer 21 is attached to the relay transmitting member 22. Inside the holding casing 11, the ultrasonic probe 8 is connected to the distal side of the relay transmitting member 22. In the relay transmitting member 22, a sectional area changing portion 23 is disposed in which a sectional area perpendicular to the longitudinal axis C decreases toward the distal side. The sectional area changing portion (a horn portion) 23 is positioned on the distal side with respect to the ultrasonic transducer 21. The ultrasonic transducer 21 is connected to one end of each of electric wires 25A and 25B. The electric wires 25A and 25B extend through the inside of the cable 15, and the other end of the wire is connected to the energy control device 3.

[0029] The switch is switched to an ON state by the input of the energy operation in the energy operating button 12, whereby in the energy control device 3, the control section controls the conversion circuit, to supply the vibration generating electric power (a vibration generating current) to the ultrasonic transducer 21 through the electric wires 25A and 25B. Consequently, in the ultrasonic transducer 21, the ultrasonic vibration occurs, and the generated ultrasonic vibration is transmitted to the ultrasonic probe 8 via the relay transmitting member 22. In this case, an amplitude of the ultrasonic vibration is enlarged in the sectional area changing portion 23 of the relay transmitting member 22.

[0030] [Probe Main Body Section 31]

[0031] The ultrasonic probe 8 includes a probe main body section 31 extending along the longitudinal axis C. The probe main body section 31 substantially linearly extends along the longitudinal axis C which is an axial center. On the proximal side of the probe main body section 31, an engagement connecting portion 32 is provided. The engagement connecting portion 32 is engaged in an engagement groove (not shown) disposed in the relay transmitting member 22 (e.g., by screwing an external thread into an internal thread), whereby the probe main body section 31 is connected to the distal side of the relay transmitting member 22. Thus, the relay transmitting member 22 is connected to the probe main body section 31, whereby an abutment surface 33 formed at a proximal end of the probe main body section 31 abuts on the relay transmitting member 22. The ultrasonic vibration is transmitted from the relay transmitting member 22 to the probe main body section 31 through the abutment surface 33.

[0032] Thus, the ultrasonic vibration is transmitted to the probe main body section 31, whereby in the probe main body section 31 (the ultrasonic probe 8), the ultrasonic vibration is transmitted from the proximal toward the distal. In a state where the ultrasonic vibration is transmitted through the probe main body section 31, the vibrating body unit 20 performs a longitudinal vibration in a vibrating direction parallel to the longitudinal axis direction in an predetermined frequency range including an predetermined frequency. In this case, a vibration antinode (the most proximal vibration antinode) A1 that is one of vibration antinodes of the longitudinal vibration is positioned at a proximal end of the vibrating body unit 20 (a proximal end of the relay transmitting member 22), and a vibration antinode (the most distal vibration antinode) A2 that is one of the vibration antinodes of the longitudinal vibration is

positioned at a distal end of the vibrating body unit **20** (a distal end of the ultrasonic probe **8**). Here, the vibration antinode **A1** is positioned most proximally among the vibration antinodes of the longitudinal vibration, and the vibration antinode **A2** is positioned most proximally among the vibration antinodes of the longitudinal vibration. In a certain example, the vibrating body unit **20** is designed in a state of transmitting the ultrasonic vibration therethrough, thereby performing the longitudinal vibration at 47 kHz (the predetermined frequency), and the vibrating body unit actually longitudinally vibrates in the frequency range (the predetermined frequency range) of 46 kHz or more and 48 kHz or less.

[0033] The ultrasonic probe **8** has a total length **L1** from its distal end to its proximal end (a proximal end of the engagement connecting portion **32**) in the longitudinal axis direction. In the certain example, it is preferable that the total length **L1** is 183.1 mm. Furthermore, the ultrasonic probe **8** has a longitudinal dimension **L2** from the distal end to the abutment surface **33** (the proximal end of the probe main body section **31**) in the longitudinal axis direction. In the certain example, it is preferable that the longitudinal dimension **L2** is 177.1 mm.

[0034] In the probe main body section **31**, a horn portion (a first horn portion) **35** is disposed. In the horn portion **35**, the sectional area perpendicular to the longitudinal axis **C** decreases toward the distal side. The horn portion (a sectional area decreasing portion) **35** is positioned on the distal side with respect to the abutment surface **33**, and the probe main body section **31** has a longitudinal dimension **L3** from the abutment surface **33** to a proximal end (a vibration input end) **E1** of the horn portion **35** in the longitudinal axis direction. In the certain example, it is preferable that the longitudinal dimension **L3** is 29 mm. Furthermore, the horn portion (the first horn portion) **35** has a horn longitudinal dimension (a first horn longitudinal dimension) **L4** from the proximal end (the vibration input end) **E1** to a distal end (a vibration output end) **E2** in the longitudinal axis direction. In the certain example, it is preferable that the horn longitudinal dimension **L4** is 20 mm.

[0035] An outer diameter of the probe main body section **31** is kept to be substantially constant from the abutment surface **33** to the proximal end **E1** of the horn portion **35** in the longitudinal axis direction. Therefore, the probe main body section **31** has an outer diameter **D1** in the abutment surface **33** and at the proximal end **E1** of the horn portion **35**. In the certain example, it is preferable that the outer diameter **D1** is 7 mm. Furthermore, in the horn portion **35**, a sectional area decreases toward the distal side, and hence at the distal end **E2** of the horn portion **35**, the probe main body section **31** has an outer diameter **D2** smaller than the outer diameter **D1**. That is, in the horn portion **35**, the outer diameter of the probe main body section **31** decreases from the outer diameter **D1** to the outer diameter **D2** toward the distal side. In the certain example, it is preferable that the outer diameter **D2** is 3.8 mm.

[0036] In a state where the vibrating body unit **20** longitudinally vibrates in the predetermined frequency range (e.g., 46 kHz or more and 48 kHz or less), a vibration node **N1** that is one of vibration nodes of the longitudinal vibration is positioned at the proximal end **E1** of the horn portion **35** or in the vicinity of the proximal end **E1**, and each of the vibration antinodes of the longitudinal vibration is positioned away from the horn portion **35** in the longitudinal axis

direction. Consequently, in the horn portion **35** in which the sectional area decreases toward the distal side, the amplitude of the longitudinal vibration (the ultrasonic vibration) is enlarged. In the certain example, the longitudinal vibration in which the amplitude at the vibration antinode is 18 μm is transmitted to the proximal end **E1** of the horn portion **35**, and the amplitude of the longitudinal vibration in the horn portion **35** is enlarged. It is to be noted that in a state where the vibrating body unit **20** vertically vibrates at the predetermined frequency (e.g., 47 kHz) included in the predetermined frequency range, the vibration node **N1** is positioned at the proximal end **E1** of the horn portion **35**.

[0037] In the probe main body section **31**, a horn portion (a second horn portion) **36** is provided. In the horn portion **36**, the sectional area perpendicular to the longitudinal axis **C** decreases toward the distal side. The horn portion (a sectional area decreasing portion) **36** is positioned on the distal side from the horn portion (the first horn portion) **35**, and the probe main body section **31** has a longitudinal dimension **L5** from the abutment surface **33** to a proximal end (a vibration input end) **E3** of the horn portion **36** in the longitudinal axis direction. In the certain example, it is preferable that the longitudinal dimension **L5** is 88.1 mm. Furthermore, the horn portion (the second horn portion) **36** has a horn longitudinal dimension (a second horn longitudinal dimension) **L6** from the proximal end (the vibration input end) **E3** to a distal end (a vibration output end) **E4** in the longitudinal axis direction. In the certain example, it is preferable that the horn longitudinal dimension **L6** is 14 mm.

[0038] In the probe main body section **31**, the outer diameter is kept to be substantially constant from the distal end **E2** of the horn portion (the first horn portion) **35** to the proximal end **E3** of the horn portion (the second horn portion) **36** in the longitudinal axis direction. Therefore, the probe main body section **31** has the outer diameter **D2** at the proximal end **E3** of the horn portion **36**. That is, at the distal end **E2** of the horn portion **35** and the proximal end **E3** of the horn portion **36**, the outer diameter of the probe main body section **31** becomes the outer diameter **D2** and has about the same size. Furthermore, in the horn portion **36**, the sectional area decreases toward the distal side, and hence at the distal end **E4** of the horn portion **36**, the probe main body section **31** has an outer diameter **D3** that is smaller than the outer diameter **D2**. That is, in the horn portion **36**, the outer diameter of the probe main body section **31** decreases from the outer diameter **D2** to the outer diameter **D3** toward the distal side. In the certain example, it is preferable that the outer diameter **D3** is 2.7 mm.

[0039] In the state where the vibrating body unit **20** longitudinally vibrates in the predetermined frequency range (e.g., 46 kHz or more and 48 kHz or less), a vibration node **N2** that is one of the vibration nodes of the longitudinal vibration is positioned at the proximal end **E3** of the horn portion **36** or in the vicinity of the proximal end **E3**, and each of the vibration antinodes of the longitudinal vibration is positioned away from the horn portion **36** in the longitudinal axis direction. Consequently, in the horn portion **36** in which the sectional area decreases toward the distal side, the amplitude of the longitudinal vibration (the ultrasonic vibration) is enlarged. It is to be noted that in the state where the vibrating body unit **20** vertically vibrates at the predetermined frequency (e.g., 47 kHz) included in the predetermined frequency range, the vibration node **N2** is positioned at the proximal end **E3** of the horn portion **36**. Furthermore,

in the state where the vibrating body unit 20 vertically vibrates in the predetermined frequency range, the vibration node N2 is positioned on the distal side with respect to the vibration node N1.

[0040] In the probe main body section 31, a sectional area increasing portion 37 is provided. In the sectional area increasing portion 37, the sectional area perpendicular to the longitudinal axis C increases toward the distal side. The sectional area increasing portion 37 is positioned on the distal side with respect to the horn portion (the second horn portion) 36, and the probe main body section 31 has a longitudinal dimension L7 from the abutment surface 33 to a distal end (a vibration output end) E6 of the sectional area increasing portion 37 in the longitudinal axis direction. In the certain example, it is preferable that the longitudinal dimension L7 is 116.7 mm. Furthermore, the sectional area increasing portion 37 has an extending dimension L8 from a proximal end (a vibration input end) E5 to the distal end (the vibration output end) E6 in the longitudinal axis direction. The extending dimension L8 is small, and hence in the sectional area increasing portion 37, a distance from the proximal end E5 to the distal end E6 decreases.

[0041] In the probe main body section 31, the outer diameter is kept to be substantially constant from the distal end E4 of the horn portion (the second horn portion) 36 to the proximal end E5 of the sectional area increasing portion 37 in the longitudinal axis direction. Therefore, the probe main body section 31 has the outer diameter D3 at the proximal end E5 of the sectional area increasing portion 37. That is, at the distal end E4 of the horn portion 36 and the proximal end E5 of the sectional area increasing portion 37, the outer diameter of the probe main body section 31 becomes the outer diameter D3 and has about the same size. Furthermore, in the sectional area increasing portion 37, the sectional area increases toward the distal side, and hence at the distal end E6 of the sectional area increasing portion 37, the probe main body section 31 has an outer diameter D4 that is larger than the outer diameter D3. That is, in the sectional area increasing portion 37, the outer diameter of the probe main body section 31 increases from the outer diameter D3 to the outer diameter D4 toward the distal side. In the certain example, the outer diameter D4 is about the same as the outer diameter D2 at the proximal end E3 of the horn portion 36. In this case, it is preferable that the outer diameter D4 is 3.8 mm.

[0042] In the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, a vibration antinode A3 that is one of the vibration antinodes of the longitudinal vibration is positioned in the sectional area increasing portion 37. The vibration antinode A3 at which stress due to the ultrasonic vibration becomes zero is positioned in the sectional area increasing portion 37, and hence, also in the sectional area increasing portion 37 in which the sectional area increases toward the distal side, the amplitude of the longitudinal vibration (the ultrasonic vibration) hardly decreases. It is to be noted that in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, the vibration antinode A3 is positioned on the distal side with respect to the vibration node N2, and in the present embodiment, the vibration antinode A3 is positioned second distally among the vibration antinodes of the longitudinal vibration.

[0043] The probe main body section 31 includes a supported portion 38 by the sheath 7 via an elastic member (not

shown). The supported portion 38 is positioned on the distal side with respect to the sectional area increasing portion 37. The probe main body section 31 has a longitudinal dimension L9 from the distal end E6 of the sectional area increasing portion 37 to a proximal end E7 of the supported portion 38 in the longitudinal axis direction. In the certain example, it is preferable that the longitudinal dimension L9 is 24.1 mm. Furthermore, the supported portion 38 has an extending dimension L10 from the proximal end E7 to a distal end E8 in the longitudinal axis direction. The extending dimension L10 is small, and in the certain example, it is preferable that the extending dimension L10 is 3 mm.

[0044] In the probe main body section 31, the outer diameter is kept to be substantially constant from the distal end E6 of the sectional area increasing portion 37 to the proximal end E7 of the supported portion 38 in the longitudinal axis direction. Therefore, the probe main body section 31 has the outer diameter D4 at the proximal end E7 of the supported portion 38. That is, at the distal end E6 of the sectional area increasing portion 37 and the proximal end E7 of the supported portion 38, the outer diameter of the probe main body section 31 becomes the outer diameter D4 and has about the same size. In a proximal portion of the supported portion 38, the outer diameter of the probe main body section 31 decreases from the outer diameter D4 to an outer diameter D5. In the certain example, the outer diameter D5 is about 0.4 mm smaller than the outer diameter D4. In the supported portion 38, the outer diameter of the probe main body section 31 is kept to be substantially constant at the outer diameter D5 along a large part in the longitudinal axis direction. Further, in the distal portion of the supported portion 38, the outer diameter of the probe main body section 31 increases from the outer diameter D5 to an outer diameter D6. In consequence, the probe main body section 31 has the outer diameter D6 at the distal end E8 of the supported portion 38. The outer diameter D6 at the distal end E8 of the supported portion 38 is about the same as the outer diameter D4 at the proximal end E7 of the supported portion 38. Consequently, at the proximal end E7 and the distal end E8 of the supported portion 38, the sectional area of the probe main body section 31 which is perpendicular to the longitudinal axis C becomes about the same. In the certain example, it is preferable that the outer diameter D6 is 3.8 mm.

[0045] In the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, a vibration node N3 that is one of the vibration nodes of the longitudinal vibration is positioned in the supported portion 38. Consequently, the probe main body section 31 (the ultrasonic probe 8), which longitudinally vibrates, is also attached to the sheath 7 via the elastic member in the supported portion 38. Furthermore, the probe main body section is supported by the sheath 7 at the vibration node N3 of the longitudinal vibration, and hence in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, transmission of the ultrasonic vibration from the supported portion 38 to the sheath 7 is prevented. In the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, the vibration node (the most distal vibration node) N3 is positioned on the distal side with respect to the vibration node N2, and is positioned most distally among the vibration nodes of the longitudinal vibration. Furthermore, at the proximal end E7 and the distal end E8 of the supported

portion 38, the sectional area of the probe main body section 31 which is perpendicular to the longitudinal axis C becomes about the same, and hence in the supported portion 38, the amplitude of the longitudinal vibration hardly changes.

[0046] Furthermore, the distal end of the sheath 7 is positioned on the distal side with respect to the distal end E8 of the supported portion 38. Therefore, in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, the vibration node N3 positioned most distally among the vibration nodes is positioned inside the sheath 7. However, a distance between the distal end E8 of the supported portion 38 and the distal end of the sheath 7 in the longitudinal axis direction is small, and is about several mm in the certain example.

[0047] FIG. 3 and FIG. 4 are views showing a constitution of the distal portion of the ultrasonic probe 8. Here, a certain direction that is substantially perpendicular to (intersects) the longitudinal axis C is a first perpendicular direction (a direction of an arrow P1 in each of FIG. 2 and FIG. 3), and an opposite direction to the first perpendicular direction (a first intersecting direction) is a second perpendicular direction (a direction of an arrow P2 in each of FIG. 2 and FIG. 3). Furthermore, one of two directions which substantially perpendicular the longitudinal axis C (intersect) and are perpendicular to the first perpendicular direction (the first intersecting direction) and the second perpendicular direction (a second intersecting direction) is a first width direction (a direction of an arrow B1 in FIG. 4). Further, an opposite direction to the first width direction is a second width direction (a direction of an arrow B2 in FIG. 4). Here, FIG. 2 and FIG. 3 are views of the ultrasonic probe 8 seen from a first width direction side, and FIG. 4 is a view of the ultrasonic probe 8 seen from a second perpendicular direction side.

[0048] As shown in FIG. 3 and FIG. 4, the probe main body section 31 extends to a position located on the distal side with respect to the supported portion 38. That is, a distal end E9 of the probe main body section 31 is positioned on the distal side from the distal end E8 of the supported portion 38. However, a distance between the distal end E8 of the supported portion 38 and the distal end E9 of the probe main body section 31 in the longitudinal axis direction is small, and is about 0.6 mm in the certain example.

[0049] As described above, in the probe main body section 31, the amplitude of the longitudinal vibration is enlarged in the horn portion (the first horn portion) 35 and the horn portion (the second horn portion) 36, and the amplitude of the longitudinal vibration hardly changes in the sectional area increasing portion 37 and the supported portion 38. Due to the above-mentioned constitution, in the certain example, the longitudinal vibration of an amplitude of 80 μ m occurs at the distal end E6 of the probe main body section 31, in a case where the longitudinal vibration of an amplitude of 18 μ m at the vibration antinode is transmitted to the proximal end (the abutment surface 33) of the probe main body section 31.

[0050] [Distal Constituting Section 31a of Probe Main Body Section 31]

[0051] As shown in FIG. 1, the probe main body section 31 has a distal constituting section 31a which exposed toward outside from the distal end of the sheath 7. For example, a part located on a forward side with respect to the

distal end E8 of the supported portion 38 functions as the distal constituting section 31a.

[0052] As shown in FIG. 3, the distal constituting section 31a has a reference surface 31b including an after-mentioned blade tip portion 143, and an opposite surface 31c disposed on a side opposite to the reference surface 31b. The reference surface 31b is an upper surface of the probe main body section 31 and the opposite surface 31c is a lower surface of the probe main body section 31. The reference surface 31b and the opposite surface 31c are narrowed so that the probe main body section 31 tapers off toward a distal end E50 of the distal constituting section 31a. As shown in FIG. 3 and FIG. 4, on the reference surface 31b and the opposite surface 31c, a narrowing start position S1 is a position that is distant from the distal end E50 as much as a longitudinal dimension L50 in a longitudinal axis C direction. It is preferable that the longitudinal dimension L50 is 32 mm. The narrowing start position S1 is a continuous position of a proximal end of a tapered section 101 with the distal end E9 of the probe main body section 31, and is also a boundary position between the probe main body section 31 and the tapered section 101.

[0053] As shown in FIG. 3 and FIG. 4, in a circumferential direction of the probe main body section 31, the reference surface 31b and the opposite surface 31c are continuous with both side surfaces 31d of the probe main body section 31. As shown in FIG. 4, parts of the side surfaces 31d are narrowed to taper off toward the distal end E50. As shown in FIG. 3 and FIG. 4, on the side surfaces 31d, a narrowing start position S2 is a position that is distant as much as a longitudinal dimension L51 from the distal end E50 in the longitudinal axis C direction. It is preferable that the longitudinal dimension L51 is 25 mm. It is to be noted that parts of each side surface 31d is not narrowed, and as shown in FIG. 4, the narrowing end position S3 is a position that is distant as much as a longitudinal dimension L53 from the distal end E50. It is preferable that the longitudinal dimension L53 is 10 mm. Furthermore, between the narrowing start position S1 and the narrowing start position S2, the parts of the side surfaces 31d are not narrowed.

[0054] As shown in FIG. 3 and FIG. 4, the probe main body section 31 has the tapered section 101 (a sectional area decreasing portion), a relay extending section 103, and a curving section (a curved extending section) 105 which are provided in the distal constituting section 31a. A distal portion of the tapered section 101 is continuous with a proximal portion of the relay extending section 103, and a distal portion of the relay extending section 103 is continuous with a proximal portion of the curving section 105.

[0055] As shown in FIG. 3 and FIG. 4, it is preferable that a maximum outer diameter D7 of the tapered section 101 is 3.8 mm. It is preferable that a minimum outer diameter D8 of the tapered section 101 is 1.7 mm.

[0056] As shown in FIG. 3, a part 101a of the tapered section 101 is included in the reference surface 31b and is, for example, an upper surface of the tapered section 101. A part 101b of the tapered section 101 is included in the opposite surface 31c and is, for example, a lower surface of the tapered section 101. The parts 101a and 101b are narrowed from the narrowing start position S1 to the narrowing end position S4. The narrowing end position S4 is positioned forwardly from the narrowing start position S1. It is preferable that a longitudinal dimension L54 from the

narrowing start position S1 to the narrowing end position S4 is 18 mm. The parts 101a and 101b function as an after-mentioned narrowing region.

[0057] As shown in FIG. 3 and FIG. 4, the side surfaces 31d of the distal portion in the tapered section 101 are narrowed from the narrowing start position S2 to the narrowing end position S4.

[0058] The side surfaces 31d in the proximal portion of the tapered section 101 are not narrowed, and this length is a length from the narrowing start position S1 to the narrowing start position S2.

[0059] In the tapered section 101, the sectional area perpendicular to the longitudinal axis C decreases toward the distal side. In the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range (e.g., 46 kHz or more and 48 kHz or less), the vibration node (the most distal vibration node) N3 that is one of the vibration nodes of the longitudinal vibration is positioned in the supported portion 38 and positioned in the vicinity of a proximal end (E9) of the tapered section 101. Further, in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range, each of the vibration antinodes of the longitudinal vibration is positioned away from the tapered section 101 in the longitudinal axis direction. Consequently, in the tapered section 101 in which the sectional area decreases toward the distal side, the amplitude of the longitudinal vibration (the ultrasonic vibration) is enlarged. In the certain example, the distal end E50 longitudinally vibrates at 140 μ m to 150 μ m, in a case where the longitudinal vibration of an amplitude of 80 μ m at the vibration antinode is transmitted to the proximal end (E9) of the tapered section 101.

[0060] Furthermore, in the present embodiment, a dimension of the tapered section 101 from the proximal end (E9) to a distal end (S4) in the longitudinal axis direction is larger than a $\frac{1}{8}$ wavelength ($\lambda/8$) in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range. In the certain example, in the state where the vibrating body unit 20 longitudinally vibrates at 46 kHz or more and 48 kHz or less (the predetermined frequency range), a $\frac{1}{4}$ wavelength ($\lambda/4$) from the vibration node (the most distal vibration node) N3 to the distal end E50 that is the vibration antinode (the most distal vibration antinode) A2 is 34.4 mm or more and 35.2 mm or less. On the other hand, in this example, a dimension from the proximal end (E9) of the tapered section 101 to the narrowing end position S3 in the longitudinal axis direction is about 22 mm, and is larger than the $\frac{1}{8}$ wavelength in the state where the vibrating body unit 20 longitudinally vibrates at 46 kHz or more and 48 kHz or less (the predetermined frequency range). Furthermore, in the tapered section 101, it is preferable that the longitudinal dimension L54 between the proximal end (E9) and the narrowing end position S4 in the longitudinal axis direction is 17.9 mm or more and 18.1 mm or less.

[0061] Therefore, the longitudinal dimension L54 is also larger than the $\frac{1}{8}$ wavelength in the state where the vibrating body unit 20 longitudinally vibrates at 46 kHz or more and 48 kHz or less (the predetermined frequency range).

[0062] As shown in FIG. 3, the reference surface 31b and the opposite surface 31c in the relay extending section 103 are not narrowed but are arranged in parallel along the longitudinal axis C. As shown in FIG. 4, the side surfaces 31d in the distal portion of the relay extending section 103 are narrowed up from the narrowing end position S3 to the

narrowing end position S4. A length of the relay extending section 103 is a length from the narrowing end position S3 to the narrowing end position S4. This region functions as an after-mentioned parallel region.

[0063] As shown in FIG. 5A, the curving section 105 has a central axis C0 that bends relative to the longitudinal axis C that is the central axis of the probe main body section 31. The central axis C0 of the curving section 105 bends away from the longitudinal axis C (toward the downside) from the proximal portion of the curving section 105 toward a distal portion of the curving section 105. The central axis C0 linearly extends. Further, as shown in FIG. 3 and FIG. 5A, the curving section 105 is bent relative to the probe main body section 31 on the distal end of the probe main body section 31. The curving section 105 linearly bends away from the longitudinal axis C. The bent curving section 105 is always disposed in a projection plane of the probe main body section 31, when the probe main body section 31 is seen along the longitudinal axis C from the proximal end toward the distal end. As shown in FIG. 4, in the curving section 105, the side surfaces 31d are not narrowed and the curving section corresponds to a portion having the longitudinal dimension L53.

[0064] As shown in FIG. 3, FIG. 5A and FIG. 6, the curving section 105 has a sectional area decreasing portion 110, a sectional area uniform portion 120, and a treating section 130. A proximal portion of the sectional area decreasing portion 110 is continuous with the distal portion of the relay extending section 103. A proximal portion of the sectional area uniform portion 120 is continuous with a distal portion of the sectional area decreasing portion 110. A proximal portion of the treating section 130 is continuous with a distal portion of the sectional area uniform portion 120. The sectional area decreasing portion 110 is provided in the proximal portion of the curving section 105, the treating section 130 is continuous with the distal portion of the curving section 105, and the sectional area uniform portion 120 is interposed between the sectional area decreasing portion 110 and the treating section 130 and continuous with these. For example, a femur that is an affected area 200 in the knee joint is treated with the treating section 130.

[0065] As shown in FIG. 3 and FIG. 5A, a part 110a of the sectional area decreasing portion 110 is included in the reference surface 31b, and is, for example, an upper surface of the sectional area decreasing portion 110. The part 110a is narrowed into a tapered state. Specifically, the part 110a is linearly bent relative to the reference surface 31b in the relay extending section 103 in a direction to approach the longitudinal axis C (downwardly toward the longitudinal axis C). A bending angle $\theta 50$ is 5 degrees or more and 20 degrees or less.

[0066] As shown in FIG. 3 and FIG. 5A, a part 110b of the sectional area decreasing portion 110 is included in the opposite surface 31c and is, for example, a lower surface of the sectional area decreasing portion 110. The part 110b is disposed in parallel with the longitudinal axis C. It is preferable that a longitudinal dimension L56 between the part 110b and the longitudinal axis C is 0.95 mm.

[0067] As shown in FIG. 5A, due to the part 110a and the part 110b, the central axis C1 of the sectional area decreasing portion 110 which is included in the central axis C0 of the curving section 105 is linearly bent relative to the longitudinal axis C toward a direction away from the longitudinal axis C (downwardly from the longitudinal axis C).

[0068] As shown in FIG. 3 and FIG. 5A, the sectional area uniform portion 120 has a uniform thickness. As shown in FIG. 5A and FIG. 5B, it is preferable that a height H51 of the sectional area uniform portion 120 is 1.4 mm. It is preferable that a width W51 of the sectional area uniform portion 120 is 2.8 mm. In a periphery of the sectional area uniform portion 120, each corner radius R51 is 0.5 mm.

[0069] As shown in FIG. 5A, a part 120a of the sectional area uniform portion 120 is included in the reference surface 31b and is, for example, an upper surface of the sectional area uniform portion 120. The part 120a is continuous with the part 110a of the sectional area decreasing portion 110 included in the reference surface 31b, and is disposed on the same straight line as in the part 110a. Consequently, the part 120a is, similarly to the part 110a, linearly bent relative to the reference surface 31b in the relay extending section 103 toward a direction to approach the longitudinal axis C (downwardly toward the longitudinal axis C). A bending angle $\theta 50$ is 5 degrees or more and 20 degrees or less. As shown in FIG. 3 and FIG. 6, the part 120a extends up to the longitudinal axis C so that a distal portion of the part 120a intersects the longitudinal axis C.

[0070] As shown in FIG. 3 and FIG. 5A, the part 120a is continuous with the treating section 130, and functions as a first bending surface that bends relative to a peripheral surface of the probe main body section 31 to approach the longitudinal axis C, thereby intersecting the longitudinal axis C.

[0071] As shown in FIG. 3 and FIG. 5A, a part 120b of the sectional area uniform portion 120 is included in the opposite surface 31c, and is, for example, a lower surface of the sectional area uniform portion 120. The part 120a is continuous with the part 110b of the sectional area decreasing portion 110 included in the opposite surface 31c. The part 120b is linearly bent relative to the part 110b in the direction away from the longitudinal axis C (downwardly from the longitudinal axis C). A bending angle $\theta 50$ is 5 degrees or more and 20 degrees or less in the same manner as in the above-mentioned bending angles $\theta 50$. Consequently, the bending angles $\theta 50$ correspond to the bending angles of the part 110a and the circumferential surface of the sectional area uniform portion 120. In consequence, the part 120a is disposed in parallel with the part 120b. As shown in FIG. 3 and FIG. 6, a distal portion of the part 120b is positioned below the longitudinal axis C.

[0072] As shown in FIG. 5A, due to the part 120a and the part 120b, a central axis C2 of the sectional area uniform portion 120 which is included in the central axis C0 of the curving section 105 is linearly bent relative to the central axis C1 of the sectional area decreasing portion 110 toward the direction away from the longitudinal axis C (downwardly from the longitudinal axis C). A bending angle $\theta 50$ is 5 degrees or more and 20 degrees or less in the same manner as in the above-mentioned bending angles $\theta 50$. It is to be noted that the central axis C0 of the curving section 105 preferably bends at an angle of 5 degrees or more and 8 degrees or less relative to the longitudinal axis of the probe main body section 31. That is, it is preferable that the bending angle $\theta 50$ is 5 degrees or more and 8 degrees or less.

[0073] As shown in FIG. 3 and FIG. 5A, it is preferable that a longitudinal dimension L55 from the distal end E50 to a bending start position E14 of the opposite surface 31c is 8.5 mm. The bending start position E14 is a continuous region of the part 110b with the part 120b. Consequently, the

curving section 105 is formed on the basis of the bending start position E14. The longitudinal dimension L55 indicates a sum of a length of the sectional area uniform portion 120 and a length of the treating section 130.

[0074] In the bending of the curving section 105, the curving section 105 includes an upper surface which includes a circumferential surface of the blade tip portion 143 and an after-mentioned projecting portion 137 that are a treating region and which is bent relative to an upper surface of the probe main body section 31, and a lower surface which is disposed on a side opposite to the upper surface of the curving section 105 with respect to the central axis C0 of the curving section 105, and which is bent relative to a lower surface of the probe main body section 31. The upper surface of the curving section 105 includes, for example, the part 110a, the part 120a, and a part 130a on the reference surface 31b. The lower surface of the curving section 105 includes, for example, the part 110b, the part 120b, and a part 130b on the opposite surface 31c. The upper surface of the probe main body section 31 is, for example, the part 103a of the relay extending section 103. The part 103a is included in the reference surface 31b, and is, for example, the upper surface of the relay extending section 103. The lower surface of the probe main body section 31 is, for example, a part 103b of the relay extending section 103 and part 110b. The part 103b is included in the opposite surface 31c in the same manner as in the part 110b. The part 103b is a lower surface of the relay extending section 103. A bending start position E15 of the upper surface of the curving section 105 relative to the upper surface of the probe main body section 31 is a continuous region of the part 103a with the part 110a. The bending start position E14 of the lower surface of the curving section 105 relative to the lower surface of the probe main body section 31 is a continuous region of the part 110b with the part 120b. The bending start position E15 is positioned on the proximal side with respect to the bending start position E14. The probe main body section 31 and the curving section 105 vibrate in the predetermined frequency range in a state where the ultrasonic vibration is transmitted from the probe main body section 31 to the curving section 105. In the state where the probe main body section 31 and the curving section 105 are vibrated in the predetermined frequency range, the bending start positions E14 and E15 are positioned forwardly, i.e., positioned on the distal side of the curving section 105 with respect to the most distal vibration node.

[0075] As shown in FIG. 4, it is preferable that a width W52 of the treating section 130 is 2.8 mm in the same manner as in the width W51 of the sectional area uniform portion 120.

[0076] As shown in FIG. 3 and FIG. 6, the part 130a of the treating section 130 is included in the reference surface 31b, and is, for example, an upper surface of the treating section 130. The part 130a is linearly bent relative to the part 120a of the sectional area uniform portion 120 included in the reference surface 31b, in the direction away from the longitudinal axis C (downwardly from the longitudinal axis C). The part 130a is disposed in the treating section 130, and functions as a second bending surface that bends relative to the first bending surface, in a bending direction of the part 120a as the first bending surface and a direction away from the longitudinal axis C.

[0077] As shown in FIG. 3 and FIG. 6, the part 130a smoothly curves into a circular shape, and is continuous with

a part **131a** included in the reference surface **31b**. The part **131a** is disposed in the treating section **130**, and functions as a third bending surface that bends relative to the part **130a** as the second bending surface in a direction to approach the longitudinal axis C on a side reverse to the bending direction of the part **120a** as the first bending surface, and extends toward an extension line **125** of the part **120a** as the first bending surface. The part **131a** extends up to a position that is on the extension line **125** of the part **120a** or a position below the extension line **125**, toward the longitudinal axis C relative to the part **130a**. The part **131a** is, for example, the upper surface of the treating section **130**.

[0078] As shown in FIG. 6, in a high direction of a curved surface portion **132a** in the part **130a** and the part **131a**, a corner radius **R52** is 0.5 mm. In the curved surface portion **132a**, the part **131a** tilts at an angle $\theta 51$ relative to the part **130a**. The angle $\theta 51$ is 90 degrees. It is preferable that a height **H52** of the part **131a** relative to the part **130a** is 0.6 mm. An angle $\theta 52$ formed between the longitudinal axis C direction and the part **131a** is 55 degrees or more and 85 degrees or less. As shown in FIG. 6, due to the parts **130a** and **131a**, a concave portion **127** is formed in a distal portion of the reference surface **31b**.

[0079] As shown in FIG. 3 and FIG. 6, the part **130b** of the treating section **130** is included in the opposite surface **31c**, and is, for example, a lower surface of the treating section **130**. The part **130b** is continuous with the part **120b** of the sectional area uniform portion **120** included in the opposite surface **31c**, and is disposed on the same straight line as in the part **120b**. The part **130b** extends up to a region located forwardly from the curved surface portion **132a**. The part **130b** smoothly curves into a circular shape toward the longitudinal axis C and a rear side, and is continuous with a part **134a** included in the reference surface **31b**. The part **134a** is, for example, the upper surface of the treating section **130**.

[0080] As shown in FIG. 6, in a high direction of a curved surface portion **132b** in the part **130b** and the part **134a**, a corner radius **R53** is 0.5 mm. The part **134a** tilts at an angle $\theta 53$ relative to the part **130b**. The angle $\theta 53$ is 55 degrees. As shown in FIG. 4, in a width direction of the curved surface portion **132b**, a corner radius **R54** is 0.5 mm.

[0081] As shown in FIG. 6, a boundary point **133** between the part **130b** and the curved surface portion **132b** is a region which is most distant from the longitudinal axis C in the treating section **130**, in a radius direction of the probe main body section **31**. The boundary point **133** is positioned between the longitudinal axis C and the opposite surface **31c** in one region (e.g., **E9**) of the tapered section **101** having the maximum outer diameter **D7**, in the radius direction of the probe main body section **31**. That is, when the distal end is seen from the proximal end along the longitudinal axis C, the curving section **105** including the treating section **130** having the boundary point **133** is always disposed in the projection plane of the tapered section **101**.

[0082] As shown in FIG. 3 and FIG. 6, the part **134a** is bent rearward, and is continuous with a part **135a** included in the reference surface **31b**. This continuous region (a bent portion) functions as the blade tip portion **141**. The blade tip portion **141** is linearly formed along the width directions (the arrow **B2** direction) of the treating section **130**, and is an end portion between the part **134a** and the part **135a**. The part **135a** is, for example, the upper surface of the treating section **130**.

[0083] As shown in FIG. 6, the part **135a** is bent at an angle $\theta 54$ relative to the extension line **125**. The angle $\theta 54$ is 25 degrees. In other words, the part **135a** tilts at the angle $\theta 54$ relative to the central axis **C2** of the sectional area uniform portion **120**.

[0084] As shown in FIG. 3 and FIG. 6, the part **135a** is continuous with the part **131a**. The part **135a** tilts at an angle $\theta 55$ around a continuous region between the part **135a** and the part **131a** toward the part **134a** (away from the longitudinal axis C (downward)). The angle $\theta 55$ is 30 degrees or more and 45 degrees or less. The part **135a** functions as a first treating surface that bends relative to the part **131a** that is a third bending surface in the bending direction of the part **120a** that is a first bending surface. It is to be noted that in the present embodiment, the part **134a** is disposed forwardly with respect to the part **135a**, and functions as a second treating surface that bends relative to the part **135a** in the direction away from the longitudinal axis C.

[0085] As shown in FIG. 3 and FIG. 6, the continuous region between the part **135a** and the part **131a** functions as the blade tip portion **143**. Consequently, the part **135a** has the blade tip portion **143**. Further, the part **135a** bends relative to the blade tip portion **143** in the bending direction of the part **120a** and a direction away from the extension line **125** of the part **120a**, with on the blade tip portion **143** being a center. Furthermore, the parts **134a** and **135a** tilt relative to the longitudinal axis C.

[0086] As shown in FIG. 6, it is preferable that a longitudinal dimension **L57** in a longitudinal direction between the distal end **E50** formed in the curved surface portion **132b** and the blade tip portion **143** is 0.6 mm. As shown in FIG. 3, FIG. 4 and FIG. 6, the blade tip portion **143** is formed linearly along the width direction of the treating section **130**, and is an end portion of the part **131a** and the part **135a**. It is preferable that a height **H53** between the blade tip portion **143** and the boundary point **133** is 1.4 mm. The height **H53** is a height of a distal portion of the treating section **130** including the projecting portion **137** that will be described later, and is shorter than the width **W52** of the treating section **130**. It is preferable that the width **W52** is 2.8 mm as described above. A length of the part **135a** (the first treating surface) along the longitudinal axis C is 25% or more of the longitudinal dimension **L57** from the blade tip portion **143** (the treating region) to the distal end **E20** of the curving section **105**. The blade tip portion **143** is disposed at the highest position in the treating section **130**, the part **131a** and the part **135a**. As shown in FIG. 6, the part **135a** including the blade tip portion **143** is positioned on the extension line **125** of the part **120a** or below the extension line **125**. The blade tip portion **143** is disposed in a continuous region of the part **131a** as the third bending surface with the part **135a** as the first treating surface. As shown in FIG. 6, the blade tip portion **143** functions as a treating region positioned on the extension line **125** of the part **120a** as the first bending surface or positioned on a side opposite to the longitudinal axis C with respect to a boundary that is the extension line **125** of the part **120a** as the first bending surface. That is, the blade tip portion **143** is disposed at a position that is on the extension line **125** or a position below the extension line **125**.

[0087] As shown in FIG. 6, in the above-mentioned shape of the treating section **130**, the treating section **130** has the projecting portion **137** projecting toward a side reverse to a bending direction of the central axis **C0** of the curving

section 105 relative to the longitudinal axis C, and the blade tip portion 143 of the treating region disposed at the end of the projecting portion 137 and therefore disposed at the position reverse to the bending direction of the central axis C0 relative to the longitudinal axis C to treat the knee joint.

[0088] The projecting portion 137 is, for example, a regional portion surrounded with the curved surface portion 132a and the parts 131a, 135a and 134a. The curved surface portion 132a and the parts 131a, 135a and 134a constitute a circumferential surface of the projecting portion 137. The end of the projecting portion 137 is a continuous region of the part 131a with the part 135a. A maximum height of the projecting portion 137 is the height H52 of the part 131a relative the part 130a.

[0089] In the distal constituting section 31a, the probe main body section 31 has the tapered section 101, the relay extending section 103 and the curving section (the curved extending section) 105 as described above. When a view-point is changed, the ultrasonic probe 8 has a narrowed region, a parallel region and an intersecting region.

[0090] As shown in FIG. 3, the narrowed region is disposed in the distal portion of the probe main body section 31 and is tapered and narrowed toward the longitudinal axis C. The narrowed region has the parts 101a and 101b. The parts 101a and 101b are vertically symmetrically arranged about the longitudinal axis C, and have the same length, shape and tilt as each other. Consequently, a narrowing angle on an upper surface is the same as a narrowing angle on a lower surface. The probe main body section 31 including the narrowed region and the curving section 105 vibrate in the predetermined frequency range in a state where the ultrasonic vibration is transmitted from the probe main body section 31 including the narrowed region to the curving section 105. In the state where the probe main body section 31 including the narrowed region and the curving section 105 vibrated in the predetermined frequency range, the longitudinal dimension L54 is larger than a $\frac{1}{8}$ wavelength of the vibration. The narrowed region and the treating section 130 disposed on the distal side with respect to the narrowed region are arranged in a $\frac{1}{4}$ wavelength of the vibration.

[0091] As shown in FIG. 3 and FIG. 5A, a parallel region is disposed forwardly with respect to the distal portion of the probe main body section 31 and the narrowed region, is continuous with the narrowed region, and is parallel to the longitudinal axis C. The parallel region has, for example, the reference surface 31b and the opposite surface 31c in the relay extending section 103, and the opposite surface 31c in the sectional area decreasing portion 110. In other words, the parallel region has, for example, the parts 103a and 103b of the relay extending section 103 and the part 110b of the sectional area decreasing portion 110. The reference surface 31b (the part 103a) is an upper surface that is parallel to the longitudinal axis C. The opposite surface 31c (the parts 103b and 110b) are lower surfaces which are arranged on a side opposite to the upper surface with respect to the longitudinal axis C, are parallel to the longitudinal axis C, and are longer the upper surface. The part 103a and the part 103b are vertically symmetrically arranged about the longitudinal axis C, and have the same length and shape each other. The part 110b is provided, and hence the lower surface in the parallel region is longer than the upper surface in the parallel region, and extends to the distal side more than the upper surface in the parallel region.

[0092] As shown in FIG. 5A and FIG. 6, the intersecting region is disposed in the curving section 105, is continuous with the parallel region, and intersects the longitudinal axis C. The intersecting region has, for example, the reference surface 31b in the curving section 105. In other words, the intersecting region has the part 120a of the sectional area uniform portion 120.

[0093] As described above, the bent curving section 105 is always disposed in the projection plane of the probe main body section 31, when the probe main body section 31 is seen along the longitudinal axis C from its proximal end toward its distal end. Further, the part 101b is narrowed toward the longitudinal axis C. The continuous part 103b is continuous with the distal end of the part 101b and parallel to the longitudinal axis C, and the part 110b is continuous with the distal end of the part 103b and parallel to the longitudinal axis C. The parts 103b and 110b are always arranged in the projection plane of the probe main body section 31. The parts 120b and 130b are linearly bent in the direction away from the longitudinal axis C, but are always arranged in the projection plane of the probe main body section 31 in the same manner as in the parts 103b and 110b. Consequently, as shown in FIG. 3, a space 145 is formed on an opposite surface 31c side and in the projection plane of the probe main body section 31. The space 145 is positioned between the proximal end E9 (the proximal end of the part 101a) and the distal end of the part 130b in the longitudinal axis C direction, and positioned on the lateral side of the distal constituting section 31a of the probe main body section 31. The space 145 is disposed on a side reverse to the blade tip portion 143 with respect to the distal constituting section 31a of the probe main body section 31.

[0094] [Operation And Advantageous Effects]

[0095] Next, a function and an effect of the ultrasonic probe 8 of the present embodiment will be described.

[0096] For example, in a surgical operation under endoscope observation of, for example, the knee joint, an unshown port (opening) disposed to approach the affected area 200 is usually set at a predetermined position.

[0097] In the shape of the ultrasonic probe 8, when the ultrasonic probe 8 is seen from a proximal portion toward the distal portion of the ultrasonic probe 8 along the longitudinal axis of the ultrasonic probe 8, differently from the present embodiment, it is defined that the distal portion of the ultrasonic probe is bent relative to the proximal portion so that the distal portion of the ultrasonic probe 8 is always disposed outside the projection plane of the proximal portion of the ultrasonic probe. Further, it is defined that the treating section 130 is disposed in the distal portion. In this case, the port is usually narrow, a tubular member is thin, a cavity in the knee joint is narrow, and a circumferential surface of the femur is formed into a curved surface. Consequently, in the above-mentioned shape of the ultrasonic probe 8, inserting properties of the ultrasonic probe 8 to the tubular member and approaching properties of the treating region in the ultrasonic probe 8 to the affected area 200 would deteriorate. In the ultrasonic probe 8, a direction in which the affected area can be treated is determined in accordance with the vibrating direction. When the ultrasonic probe 8 does not come in contact with the affected area 200 in an appropriate state, an efficiency of the treatment deteriorates. Furthermore, the cavity is narrow, and the affected area is formed into the curved surface. Consequently, the above-mentioned shape of the ultrasonic probe 8 is not suitable to treat the

affected area 200 in the narrow cavity. Furthermore, in the above-mentioned shape of the ultrasonic probe 8, the probe would come in contact with an area other than the affected area to damage the area other than the affected area, before coming in contact with the affected area. Consequently, the ultrasonic probe is not suitable to treat the affected area in the narrow cavity.

[0098] In the present embodiment, the curving section 105 is bent relative to the probe main body section 31. When a distal end of the curving section 105 is seen from its proximal end along the longitudinal axis C direction, the curving section 105 including the treating section 130 having the boundary point 133 is always disposed in the projection plane of the tapered section 101. The part 120a as the first bending surface is bent relative to the circumferential surface of the probe main body section 31 to approach the longitudinal axis C, thereby intersecting with the longitudinal axis C. Further, the blade tip portion 143 that is the treating region is positioned on the extension line 125 of the part 120a as the first bending surface. Alternatively, the extension line 125 of the part 120a that is the first bending surface is the boundary, and the blade tip portion is positioned on the side opposite to the longitudinal axis C with respect to the boundary. The blade tip portion 143 is linearly formed along the width direction of the treating section 130.

[0099] Consequently, even when a cavity between the femur and a tibia is narrow and a lower surface of the femur is formed into a curved surface, the affected area 200 can appropriately be treated with the ultrasonic probe 8 in accordance with the shape of the ultrasonic probe 8. Furthermore, the affected area is not limited to the knee joint, and in a narrow cavity of a joint (e.g., a shoulder joint) other than the knee joint, the affected area 200 can appropriately be treated with the ultrasonic probe 8 in accordance with the shape of the ultrasonic probe 8. Furthermore, as shown in FIG. 8A and FIG. 8B, it is possible to improve the approaching properties of the blade tip portion 143 as the treating region in the ultrasonic probe 8 to the femur that is the affected area 200, and it is possible to improve the treatment efficiency to the affected area 200. Especially, even when the probe main body section 31 is obliquely approached to the affected area 200, the blade tip portion 143 tilts, and hence the treatment efficiency can improve. Furthermore, in the present embodiment, as shown in FIG. 8A and FIG. 8B, by rotating the probe main body section 31 around the axis of the probe main body section 31 and changing an orientation of the blade tip portion 143, it is possible to easily treat any regions of the femur and to improve the treatment efficiency and the treatment quality. In the case where the affected area 200 is present in an innermost area of a cruciate ligament, the blade tip portion 143 can easily approach the affected area 200.

[0100] The central axis of the curving section 105 bends at an angle of five degrees or more and eight degrees or less relative to the longitudinal axis C of the probe main body section 31. Consequently, even when the port is narrow and the tubular member is thin, the inserting properties of the probe main body section 31 into the tubular member can improve in the probe main body section 31 having the curving section 105, as long as the probe main body section 31 is inserted into the tubular member. Furthermore, the probe main body section 31 having the curving section 105 can be inserted through the tubular member in accordance with a degree of the curve of the curving section 105, and

during the insertion, the curving section 105 does not have to abut on an inner peripheral surface of the tubular member. Further, as shown in FIG. 8A and FIG. 8B, it is possible to improve the approaching properties of the blade tip portion 143 as the treating region in the ultrasonic probe 8 to the femur that is the affected area 200, and it is possible to improve the treatment efficiency to the affected area 200. In the present embodiment, as shown in FIG. 8A and FIG. 8B, by rotating the ultrasonic probe 8 around the axis of the probe main body section 31 and changing the orientation of the blade tip portion 143, it is possible to easily treat any regions of the femur and to improve the treatment efficiency and a treatment quality. In a case where the affected area 200 is present in the innermost area of the cruciate ligament, the blade tip portion 143 can easily approach the affected area 200.

[0101] The blade tip portion 143 that is the treating region is disposed at a position on a side reverse to the bending direction of the central axis C0 of the curving section 105. Consequently, the blade tip portion 143 can always be disposed within a projection area of the probe main body section 31. When the probe main body section 31 is inserted into the thin tubular member, the blade tip portion 143 can be prevented from abutting on the inner peripheral surface of the tubular member. Furthermore, it is possible to improve the approaching properties of the blade tip portion 143 even to any regions of the femur.

[0102] The treating section 130 is a thin distal portion of the curving section 105. A height of the distal portion of the treating section 130 is shorter than a width of the treating section 130, and hence strength of the treating section 130 can be acquired in a state where the treating section 130 is thin. The strength is acquired, and hence even when an amplitude V of the longitudinal vibration is enlarged in the tapered section 101, the treating section 130 can be prevented from breaking. Furthermore, in the state where the breakage is prevented, the hard affected area 200, e.g., a bone or the like can be treated by use of the enlarged amplitude V of the longitudinal vibration. Furthermore, the treating section 130 is thin, and hence the treating section 130 can easily approach the affected area 200.

[0103] The bending start position E15 is positioned on the proximal side with respect to the bending start position E14. Consequently, the space 145 can be formed as an escaping portion, and hence the approaching properties to the affected area 200 can improve in the narrow cavity. Specifically, for example, the lower surface of the femur as the affected area 200 is treated. When the space 145 is formed, for example, the opposite surface 31c can be prevented from abutting on an upper surface of the tibia which faces the lower surface of the femur. That is, the area other than the affected area 200 can be prevented from being unintentionally treated, and prevented from being damaged. Further, the ultrasonic probe 8 can easily access the affected area 200 even in the narrow space. Furthermore, the distal portion of the curving section 105 can be thinned and lightened, and the treatment efficiency in the narrow cavity can improve.

[0104] The bending start positions E14 and E15 are positioned on a distal portion side of the curving section 105 with respect to the most distal vibration node N3. Consequently, the amplitude V of the longitudinal vibration which is enlarged in the tapered section 101 can be transmitted to the blade tip portion 143, and the treatment efficiency can improve.

[0105] The distal portion of the probe main body section 31 can be tapered by the narrowed region, the parallel region and the intersecting region, and the approaching properties can improve. Furthermore, the space 145 as the escaping portion can be formed, and hence the treatment efficiency in the narrow cavity can improve. Specifically, it is defined that, for example, the lower surface of the femur of the affected area 200 is treated. Thus, the space 145 is formed, so that, for example, the opposite surface 31c can be prevented from abutting on the upper surface of the tibia which faces the lower surface of the femur. That is, the area other than the affected area 200 can be prevented from being unintentionally treated, and can be prevented from being damaged. Further, the ultrasonic probe 8 can easily access the affected area 200 even in the narrow space. Furthermore, the distal portion of the curving section 105 can be thinned and lightened, and the treatment efficiency in the narrow cavity can improve.

[0106] In a case where the affected area 200 is hard as in, for example, the bone, it is necessary to enlarge the amplitude V of the longitudinal vibration. In the present embodiment, the amplitude V of the longitudinal vibration can securely be enlarged by the tapered section 101 including the narrowed region.

[0107] The part 135a including the blade tip portion 143 tilts at the angle $\theta 55$ relative to the longitudinal axis C toward the part 134a with the blade tip portion 143 being a center. Consequently, when the probe main body section 31 advances and retreats along the longitudinal axis C direction, for example, a side surface of the affected area 200 which is in the form of a curved surface can be treated by the part 135a including the blade tip portion 143.

[0108] The part 134a including the blade tip portions 141 and the part 135a including the blade tip portions 143 may cut the affected area 200. The affected area 200 is cut by the parts 134a and 135a, so that a region abraded by the blade tip portions 141 and 143 is prevented from being only concaved and a stepped area is prevented from being formed in the circumferential surface of the affected area 200.

[0109] The part 131a, the part 135a and the part 134a form the blade tip portions 141 and 143, i.e., blade tip portions is formed in two steps. Consequently, in the present embodiment, it is possible to acquire thickness and strength of the treating section 130 as compared with a case where only one blade tip portion located on. Furthermore, a length of the first treating surface is 25% or more of the longitudinal dimension L57 from the blade tip portion 143 to the distal end of the curving section 105. Consequently, it is possible to acquire thickness and strength of the treating section 130. Thus, the strength is acquired, and hence even when the amplitude V of the longitudinal vibration is enlarged in the tapered section 101, it is possible to prevent breakage of the treating section 130. Further, in the state where the breakage is prevented, it is possible to treat the hard affected area 200, e.g., the bone or the like by use of the enlarged amplitude V of the longitudinal vibration.

[0110] In the present embodiment, the tapered section 101 and the relay extending section 103 are arranged, and a predetermined length is acquired. Consequently, even when the amplitude is enlarged, it is possible to prevent stress from being concentrated on a predetermined region of the distal constituting section 31a of the probe main body section 31, and it is possible to disperse the stress in the whole distal constituting section 31a of the probe main body section 31.

[0111] FIG. 7 shows the amplitude V of the longitudinal vibration and stress σ due to the ultrasonic vibration, between the second distal vibration antinode A3 and the most distal vibration antinode A2 in a state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range. In FIG. 7, an abscissa shows a position in a longitudinal axis direction and an ordinate shows the amplitude V and the stress σ . Furthermore, in FIG. 7, a solid line shows change of the amplitude V of the longitudinal vibration and a one-dot chain line shows change of the stress σ . As shown in FIG. 7, in a state where the vibrating body unit 20 longitudinal vibrates in the predetermined frequency range, the tapered section 101 is positioned on the distal side with respect to the most distal vibration node N3, and the amplitude V of the longitudinal vibration is enlarged in the tapered section 101. For example, the longitudinal vibration in which the amplitude at the vibration antinode is 80 μm is enlarged into the longitudinal vibration in which the amplitude at the vibration antinode is 140 μm or more and 150 μm or less by the tapered section 101. Furthermore, the stress σ due to the ultrasonic vibration increases at the vibration node and in a portion in which a sectional area perpendicular to a transmitting direction of the ultrasonic vibration decreases, and the stress becomes zero at the vibration antinode. Therefore, as shown in FIG. 7, the stress σ increases between the vibration node N3 and the narrowing end position S4 that is a distal end of the tapered section 101.

[0112] Here, in the present embodiment, a dimension from the proximal end (E9) of the tapered section 101 to the narrowing end position S4 in the longitudinal axis direction is larger than a $\frac{1}{8}$ wavelength ($\lambda/8$) in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range. Further, in the tapered section 101, the longitudinal dimension L54 between the proximal end (E9) and the narrowing end position S4 in the longitudinal axis direction is also larger than the $\frac{1}{8}$ wavelength in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range. The dimension from the proximal end (E9) of the tapered section 101 to the narrowing end position S4 in the longitudinal axis direction increases, so that the stress σ due to the ultrasonic vibration is kept to be substantially uniform along the total length between the vibration node N3 and the narrowing end position S4 of the tapered section 101. That is, between the vibration node N3 and the narrowing end position S4 of the tapered section 101, the stress is effectively prevented from locally increasing (i.e., generation of a peak is effectively prevented). For example, in a certain example, even when the longitudinal vibration (of, e.g., 80 μm) in which the amplitude at the vibration antinode increases is transmitted to the proximal end (E9) of the tapered section 101, the stress σ is kept to be substantially uniform at about 300 Mpa between the vibration node N3 and the narrowing end position S4 of the tapered section 101 in the state where the vibrating body unit 20 longitudinally vibrates in the predetermined frequency range (e.g., 46 kHz or more and 48 kHz or less). That is, in the present embodiment, the stress is prevented from locally increasing up to about 700 Mpa between the vibration node N3 and the narrowing end position S4 of the tapered section 101 (e.g., at the narrowing end position S4 that is the distal end of the tapered section 101). The stress σ is prevented from locally increasing, and

hence it is possible to effectively prevent the ultrasonic probe 8 from breaking due to the ultrasonic vibration.

[0113] In the present embodiment, in the case where the hard affected area 200, e.g., the bone or the like is treated with the ultrasonic probe 8 by use of the ultrasonic vibration, it is necessary to enlarge the amplitude V of the longitudinal vibration in the tapered section 101, and it is necessary to press the blade tip portion 143 onto the affected area 200. During the treatment, the tapered section 101 including the narrowed region and the curving section 105 would break due to the enlarged amplitude V and pressing. In the present embodiment, the longitudinal dimension L54 is larger than the $\frac{1}{8}$ wavelength in the state where the vibrating body unit 20 of the ultrasonic probe 8 longitudinally vibrates. The narrowed region and the treating section 130 are arranged in a $\frac{1}{4}$ wavelength in the state where the vibrating body unit 20 longitudinally vibrates. Consequently, the stress is dispersed in the longitudinal dimension L54, that is, the stress is prevented from locally increasing as described above. Furthermore, the stress decreases in the relay extending section 103 and the curving section 105. Therefore, it is possible to effectively prevent the ultrasonic probe 8 from breaking due to the ultrasonic vibration, and the enlargement of the amplitude V is compatible with the prevention of the breakage.

[0114] In the present embodiment, the probe main body section 31 is formed so that any stepped areas are not formed, and the distal constituting section 31a of the probe main body section 31 is only narrowed.

[0115] Consequently, it is possible to inhibit generation of cavitation, and it is possible to prevent the cavitation from disturbing an observation view field when the affected area 200 is treated, in other words, an operator's visibility can improve. Further, it is possible to prevent the cavitation from damaging the affected area 200, and it is possible to prevent the cavitation from damaging the probe main body section 31 and the distal constituting section 31a. The corners R51 are formed in the periphery of the sectional area uniform portion 120, the corner R52 is formed in the curved surface portion 132a, and the corner R53 and the corner R54 are formed in the curved surface portion 132b of the part 130b. Consequently, in the sectional area uniform portion 120 and the curved surface portion 132b, it is possible to inhibit the generation of the cavitation and it is possible to prevent the cavitation from damaging the affected area 200.

[0116] Furthermore, in the above description, even when the sectional area uniform portion 120, the curved surface portion 132a and the curved surface portion 132b come in contact with the affected area 200, the corners R51, R52, R53 and R54 can prevent damages on the affected area 200. A curved surface portion of the corner radius R51 may be formed along ranges F1 and F2 of FIG. 3 in the longitudinal axis direction. That is, the curved surface portion of the corner radius R51 extends from the distal end of the ultrasonic probe 8 to the tapered section 101 in the longitudinal axis direction, and is formed in a projecting portion (an exposed portion) of the ultrasonic probe 8 from the distal end of the sheath 7.

Second Embodiment

[0117] In the present embodiment, differences from the first embodiment will only be described with reference to FIG. 9, FIG. 10 and FIG. 11.

[0118] It is preferable that a total length L1 is 183.2 mm.

[0119] It is preferable that a longitudinal dimension L2 is 177.2 mm. A longitudinal dimension L53 is preferably 10 mm.

[0120] As shown in FIG. 9 and FIG. 11, in a curved surface portion 132a, for example, a corner radius R52 is 0.4 mm. It is preferable that a height H52 of a part 131a relative to a part 130a is 0.7 mm.

[0121] As shown in FIG. 11, in the width direction of a curved surface portion 132b, a corner radius R54 of each curved surface portion 132b is 1 mm. As shown in FIG. 11, an angle $\theta 56$ formed between a part 135a and a perpendicular direction perpendicular to a planar direction of the part 130a is 70 degrees. It is preferable that a longitudinal dimension L60 of the part 135a is 0.2 mm.

[0122] As shown in FIG. 11, the curved surface portion 132b is curved smoothly in a circular shape along a longitudinal axis C and toward the rear, and is continuous with a part 134a included in the reference surface 31b. In a high direction of a curved portion 132c between the curved surface portion 132b and the part 134a, a corner radius R55 is 0.4 mm. The part 134a is bent at an angle $\theta 57$ relative to the longitudinal axis C. The angle $\theta 57$ is 55 degrees.

[0123] As shown in FIG. 11, the part 134a is curved smoothly in a circular shape along the longitudinal axis C and toward the rear, and is continuous with the part 135a. In a high direction of a curved portion 132d between the part 134a and the part 135a, a corner radius R56 is 0.4 mm. The part 135a is bent at an angle $\theta 58$ relative to the longitudinal axis C. The angle $\theta 58$ is 25 degrees.

[0124] As shown in FIG. 11, it is preferable that a longitudinal dimension L61 in a longitudinal direction between a distal end E50 formed in the curved surface portion 132b and a blade tip portion 143 is 0.6 mm.

[0125] As shown in FIG. 11, the part 135a is bent relative to the blade tip portion 143 in a bending direction of a part 120a about on the blade tip portion 143 so that the whole surface of the part 135a including the blade tip portion 143 is disposed on an extension line 125 of the part 120a. Alternatively, the part 135a is bent relative to the blade tip portion 143 in the bending direction of the part 120a about the blade tip portion 143 so that the whole surface of the part 135a including the blade tip portion 143 is positioned on a side opposite to the longitudinal axis C with respect to a boundary that is the extension line 125 of the part 120a. That is, the whole surface of the part 135a including the blade tip portion 143 is disposed on the same plane as the extension line 125 or on a plane below the extension line 125.

[0126] As shown in FIG. 11, each of the part 131a and the part 135a including the blade tip portion 143 is formed into a circular shape. In this case, it is preferable that a longitudinal dimension L62 between a central position to form a circle of the blade tip portion 143 and the blade tip portion 143 is 2 mm. The central position is formed on a part 130a side.

[0127] In the present embodiment, it is possible to obtain effects similar to those of the first embodiment. In the present embodiment, the blade tip portion 141 is omitted, and the curved portions 132c and 132d can further inhibit generation of cavitation. Each of the part 131a and the part 135a including the blade tip portion 143 is formed into the circular shape. Consequently, treating properties to an affected area 200 can improve.

[0128] Although the embodiments, etc. of the present invention have been described above, the present invention

is not limited to the above-described embodiments, etc., and, needless to say, various modifications can be made without departing from the spirit of the invention.

1. An ultrasonic probe comprising:

a probe main body section which is extended along a longitudinal axis and to which ultrasonic vibration is transmitted from its proximal end to its distal end; and
a curving section which is disposed on a distal side with respect to the probe main body section, curves relative to the probe main body section in a first intersecting direction, and extends in a longitudinal axis direction, in a case where a direction intersecting the longitudinal axis is defined as the first intersecting direction and a side opposite to the first intersecting direction is defined as a second intersecting direction, the curving section having a first bending surface facing the side of the second intersecting direction; and

a treating section which is disposed on a distal side relative to the curving section and configured to cut a treatment target, the treating section having a blade tip portion projecting toward the second intersecting direction side, and a concave portion interposed between the first bending surface and the blade tip portion in the longitudinal axis direction and concaved on the side of the first intersecting direction which is defined by a second bending surface bending and extending relative to the first bending surface in the first intersecting direction and facing the second intersecting direction side and a third bending surface bending and extending relative to the second bending surface in the second intersecting direction and facing the second intersecting direction side,

wherein the blade tip portion is positioned on an extension line on which the first bending surface is extended on the distal side or positioned on the first intersecting direction side relative to the extension line of the first bending surface.

2. The ultrasonic probe according to claim 1,

wherein the wherein a central axis of the curving section is bent at an angle of 5 degrees or more and 8 degrees or less relative to the longitudinal axis of the probe main body section.

3. (canceled)

4. The ultrasonic probe according to claim 1 wherein the curving section has:

a lower surface facing the first intersecting direction side, and

a start position at which the first bending surface starts bending relative to the longitudinal axis on the first intersecting direction side is positioned on a proximal side with respect to a start position at which the lower surface starts bending relative to the longitudinal axis on the first intersecting direction side.

5. The ultrasonic probe according to claim 1,

wherein a height of the blade tip portion of the treating section is shorter than a width of the treating section.

6. (canceled)

7. The ultrasonic probe according to claim 1, comprising, between the probe main body section and the curving section,

a narrowed region tapered and narrowed toward the longitudinal axis; and

a parallel region which is disposed on a distal side with respect to the narrowed region, is continuous with the narrowed region, and is parallel to the longitudinal axis.

8. The ultrasonic probe according to claim 7,

wherein the parallel region has:

an upper surface which is parallel to the longitudinal axis; and

a lower surface which is disposed on a side opposite to the upper surface with respect to the longitudinal axis, is parallel to the longitudinal axis, and is longer than the upper surface.

9-11. (canceled)

12. The ultrasonic probe according to claim 1,

wherein a central axis of the curving section is bent at an angle of 5 degrees or more and 20 degrees or less relative to the longitudinal axis of the probe main body section.

13. An ultrasonic treatment instrument comprising:

the ultrasonic probe according to claim 1; and

a transducer unit connected to the ultrasonic probe.

* * * * *

专利名称(译)	超声波探头		
公开(公告)号	US20170202580A1	公开(公告)日	2017-07-20
申请号	US15/480022	申请日	2017-04-05
[标]申请(专利权)人(译)	奥林巴斯株式会社		
申请(专利权)人(译)	OLYMPUS CORPORATION		
当前申请(专利权)人(译)	OLYMPUS CORPORATION		
[标]发明人	YOSHIMINE HIDETO		
发明人	YOSHIMINE, HIDETO		
IPC分类号	A61B17/56 A61B18/00		
CPC分类号	A61B18/00 A61B17/56 A61B17/1675 A61B17/320068 A61B2017/320071 A61B2017/320072 A61B2017/320074 A61B2017/320089 A61B2018/00565 A61B2017/00402		
优先权	2015001839 2015-01-07 JP		
外部链接	Espacenet USPTO		

摘要(译)

弯曲部分总是设置在探头主体部分的投影平面中。弯曲部分包括第一弯曲表面，该第一弯曲表面相对于探头主体部分的外周表面弯曲以接近纵向轴线，从而与纵向轴线相交；第二弯曲表面，其相对于第一弯曲表面朝向第一弯曲表面的弯曲方向和远离纵向轴线的方向弯曲；第三弯曲表面，其相对于第二弯曲表面朝向在与第一弯曲表面的弯曲方向相反的一侧上接近纵向轴线的方向弯曲，并且朝向第一弯曲表面的延伸线延伸。

