



US006569163B2

(12) **United States Patent**
Hata et al.

(10) **Patent No.: US 6,569,163 B2**
(45) **Date of Patent: May 27, 2003**

(54) **WIRELESS ELECTROSURGICAL ADAPTER
UNIT AND METHODS THEREOF**

(56) **References Cited**

U.S. PATENT DOCUMENTS

(75) Inventors: **Cary Hata**, Tustin, CA (US); **Ji Zhang**,
Burnaby (CA)
(73) Assignee: **Quantumcor, Inc.**, Irvine, CA (US)
(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 0 days.

3,845,771 A	*	11/1974	Vise	606/49
4,510,939 A	*	4/1985	Brennan et al.	128/639
4,878,493 A	*	11/1989	Pasternak et al.	607/99
5,242,440 A	*	9/1993	Shippert	606/30
5,885,281 A	*	3/1999	Urueta	606/45
6,423,059 B1	*	7/2002	Hanson et al.	606/41
6,436,116 B1	*	8/2002	Spitz et al.	606/170

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **09/957,375**

JP 2001-17385 * 1/2001

(22) Filed: **Sep. 20, 2001**

* cited by examiner

(65) **Prior Publication Data**

US 2002/0128644 A1 Sep. 12, 2002

Primary Examiner—Joseph Pelham

(57) **ABSTRACT**

Related U.S. Application Data

(63) Continuation-in-part of application No. 09/803,284, filed on
Mar. 9, 2001.


(51) **Int. Cl.**⁷ **A61B 18/14**

(52) **U.S. Cl.** **606/41; 606/45; 606/49;**
606/50

(58) **Field of Search** 606/1, 27-32,
606/34, 37, 42, 45, 49

A wireless adapter unit that couples to an electrosurgery instrument comprising at least one surface electrical contact for contactably coupling the electrosurgical instrument to a remote power source through a coupling mechanism, wherein the coupling mechanism comprises an insulated electrical conductor running through a surgeon's glove and/or a surgeon's gown.

23 Claims, 13 Drawing Sheets

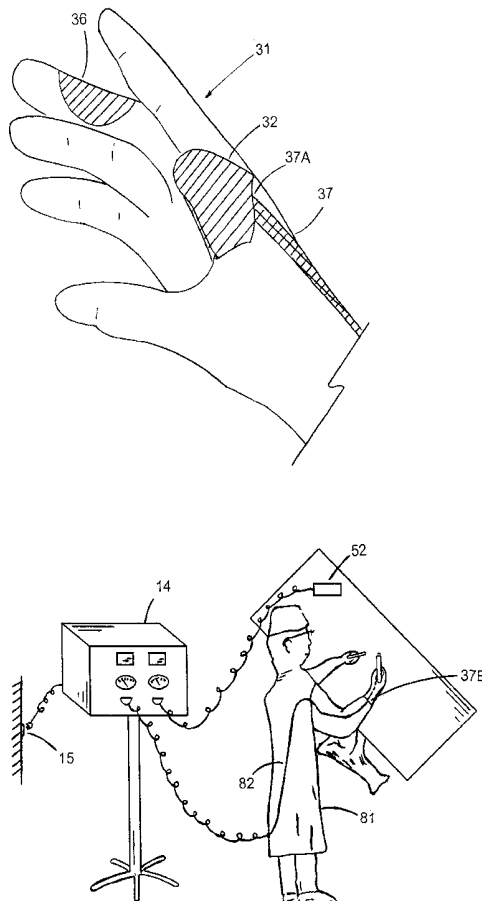

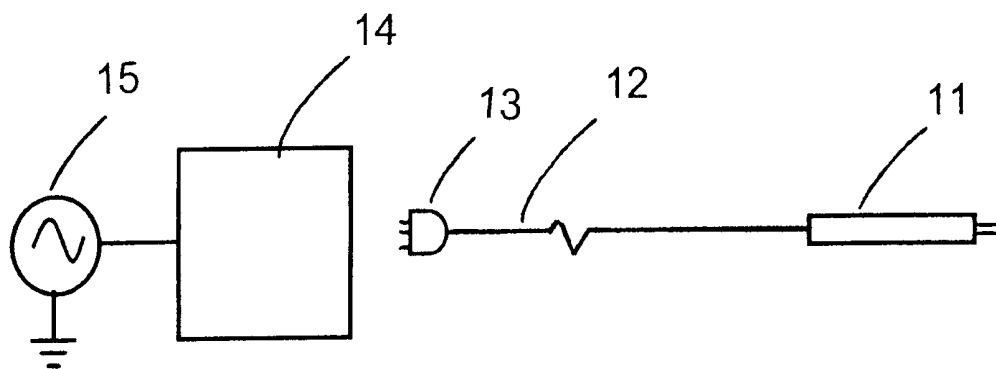


FIG. 1
(Prior Art)

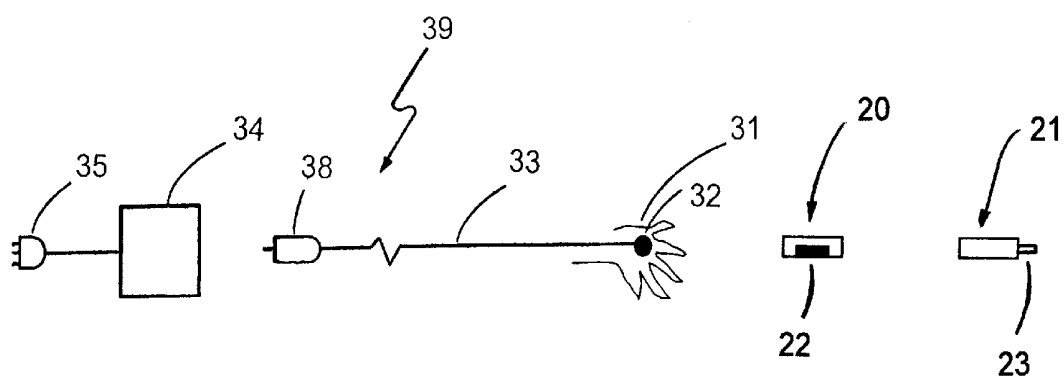
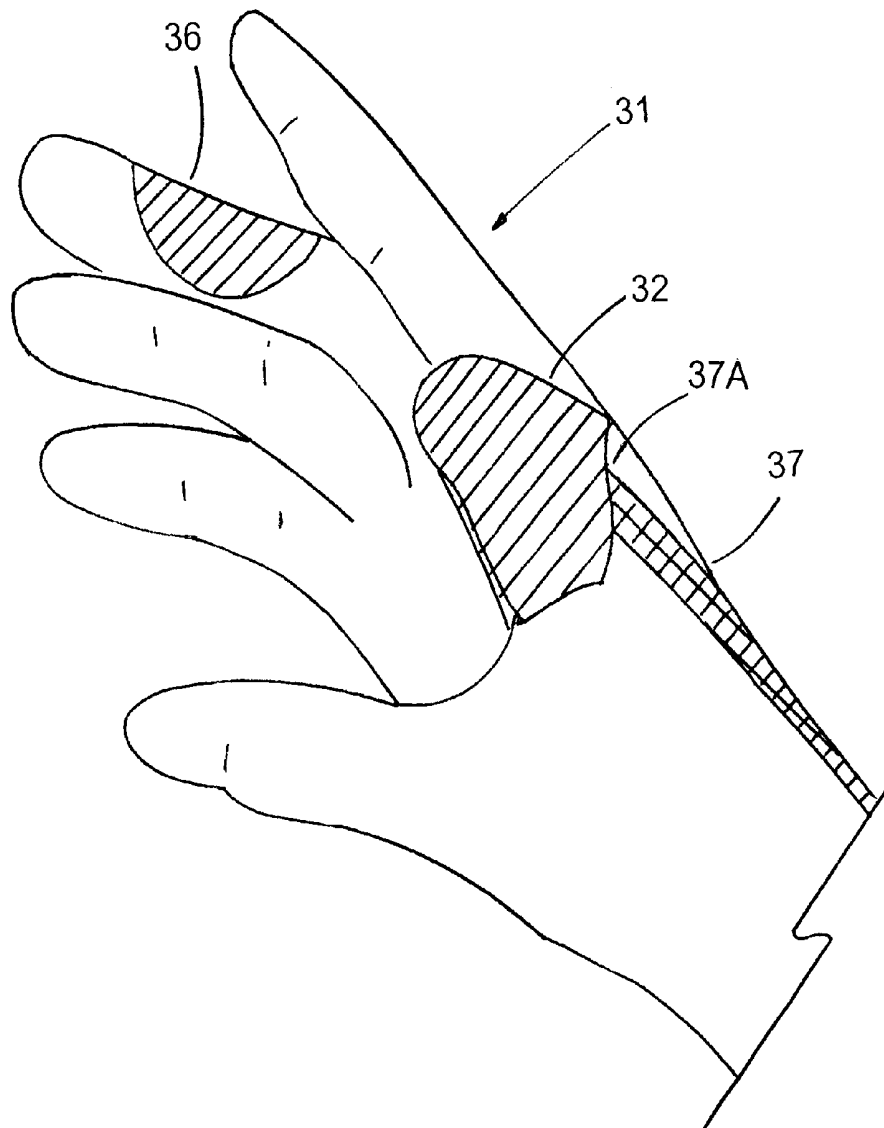
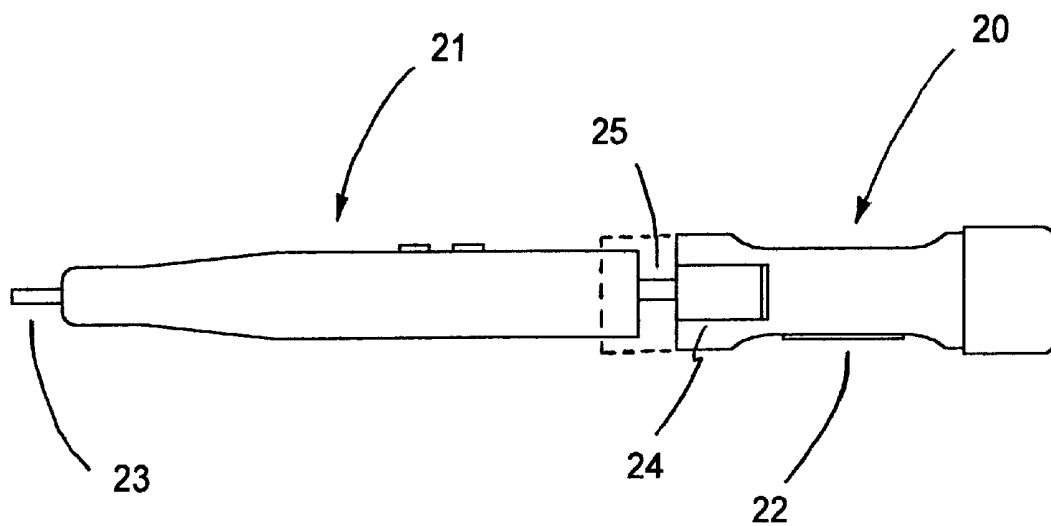
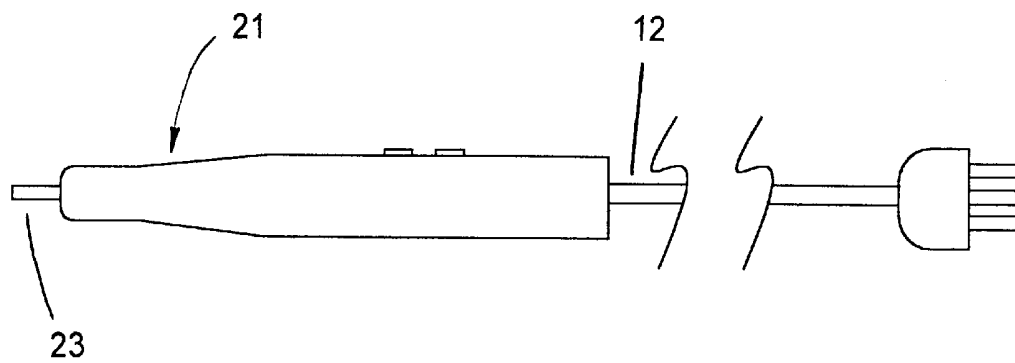
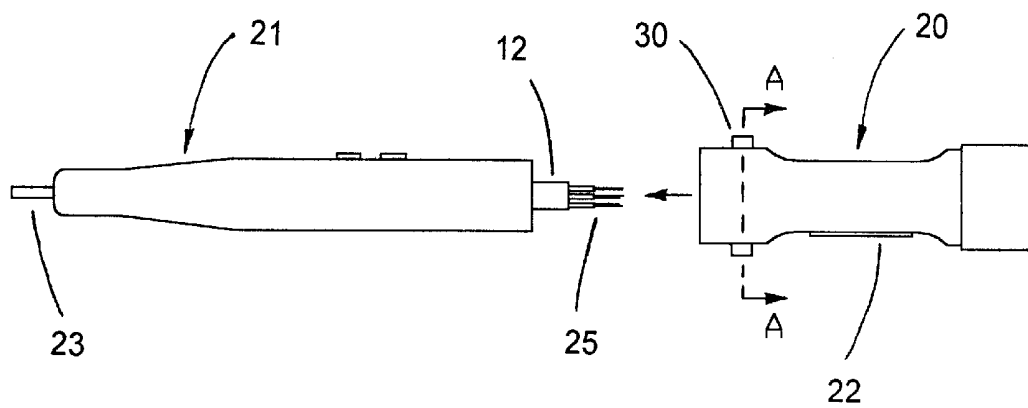



FIG. 2

**FIG. 3**

**FIG. 4**

**FIG. 4A**

**FIG. 4B**

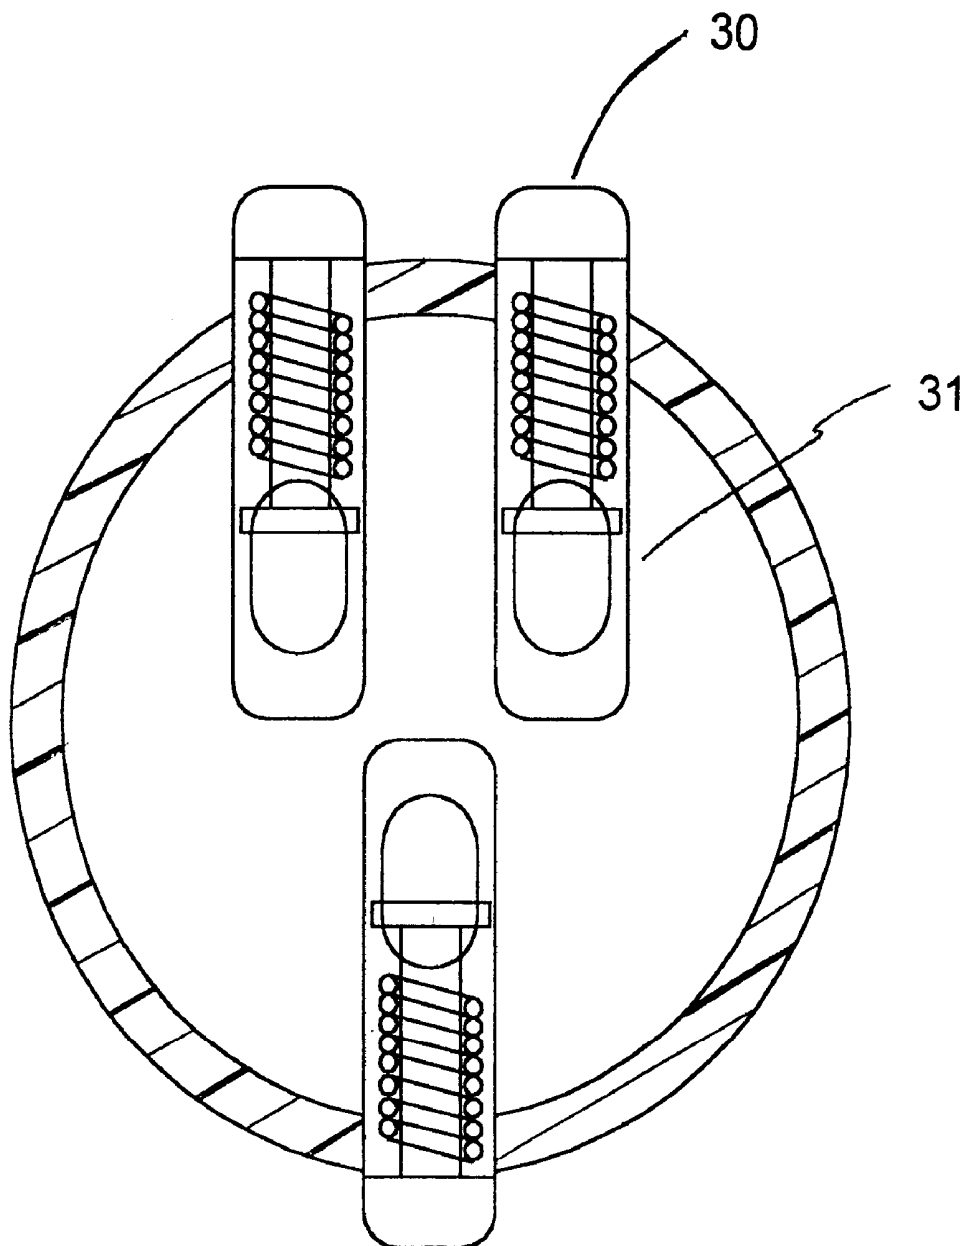**FIG. 4C**

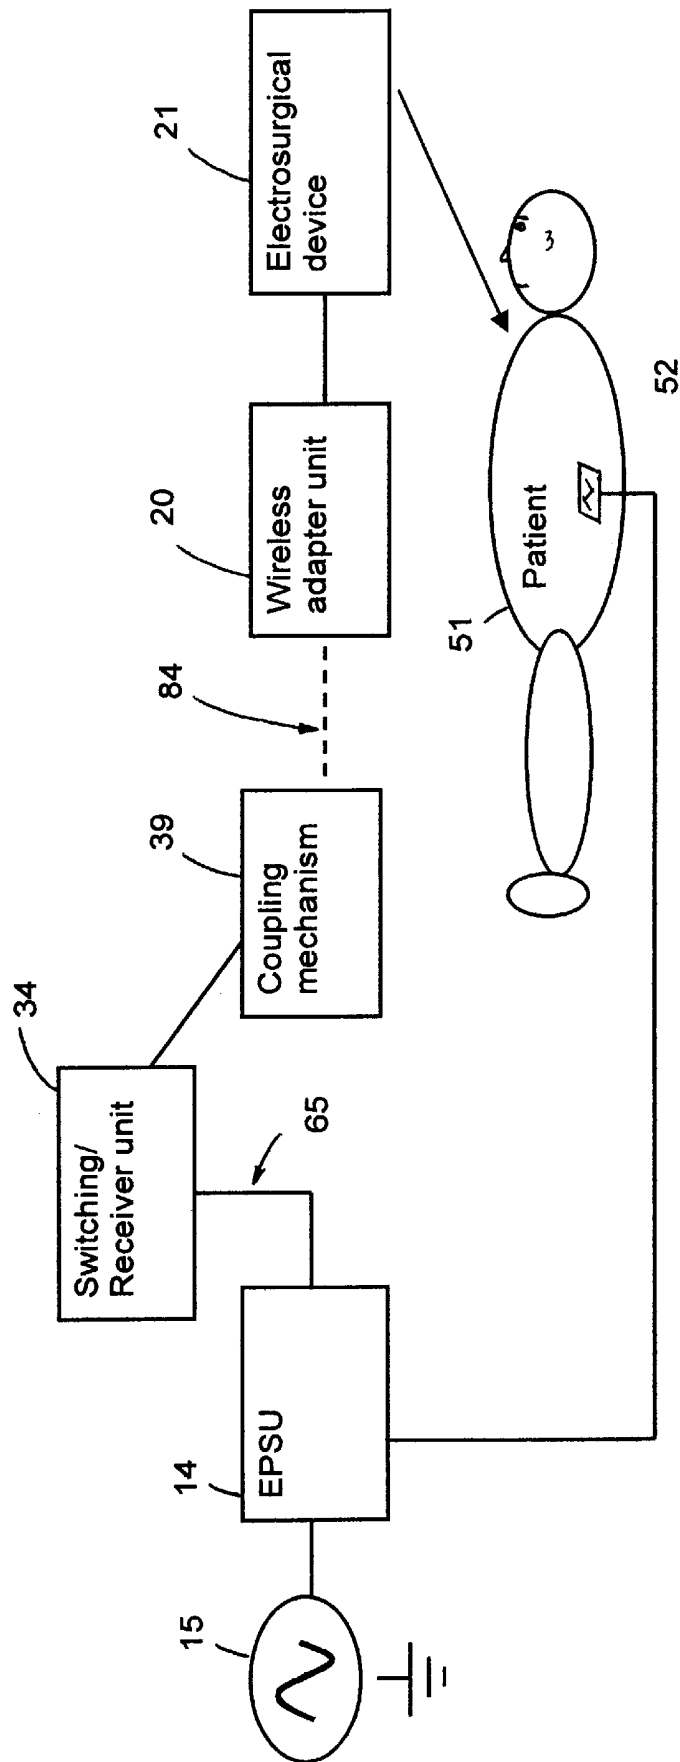
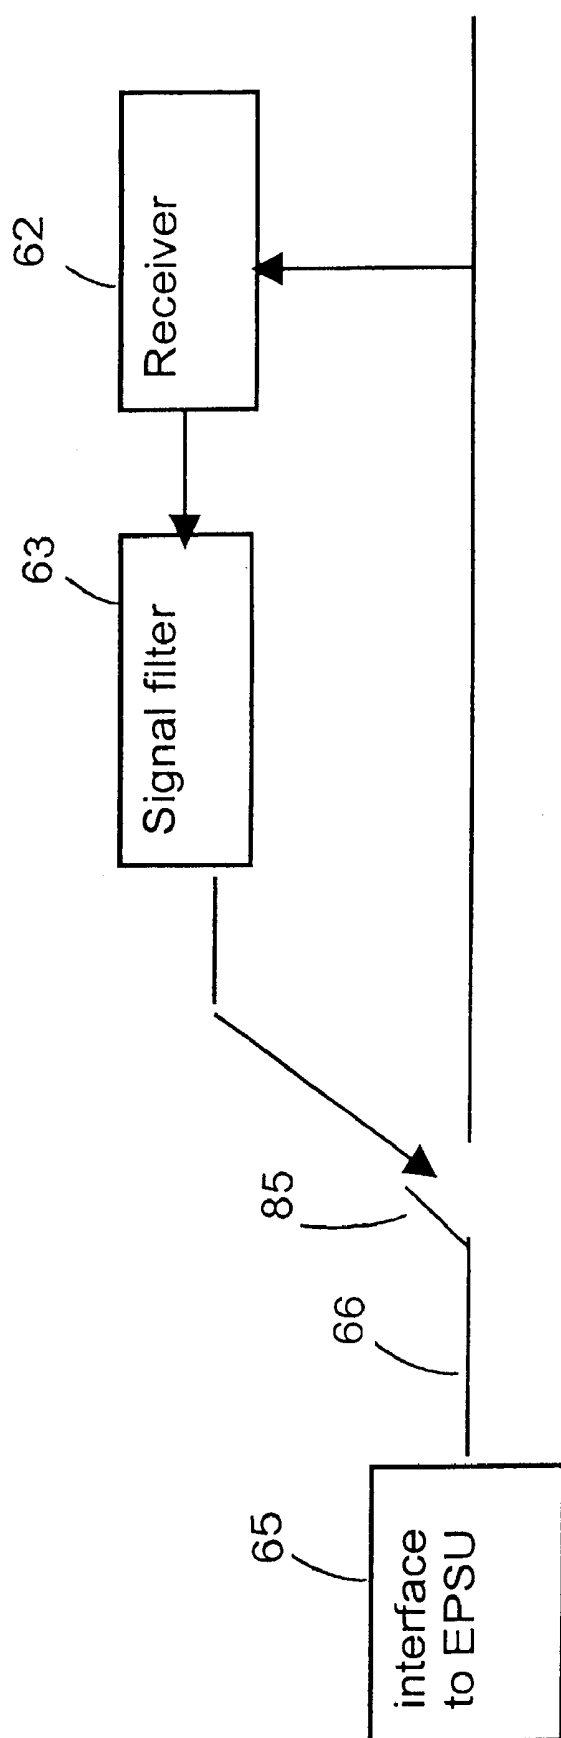


FIG. 5

**FIG. 6**

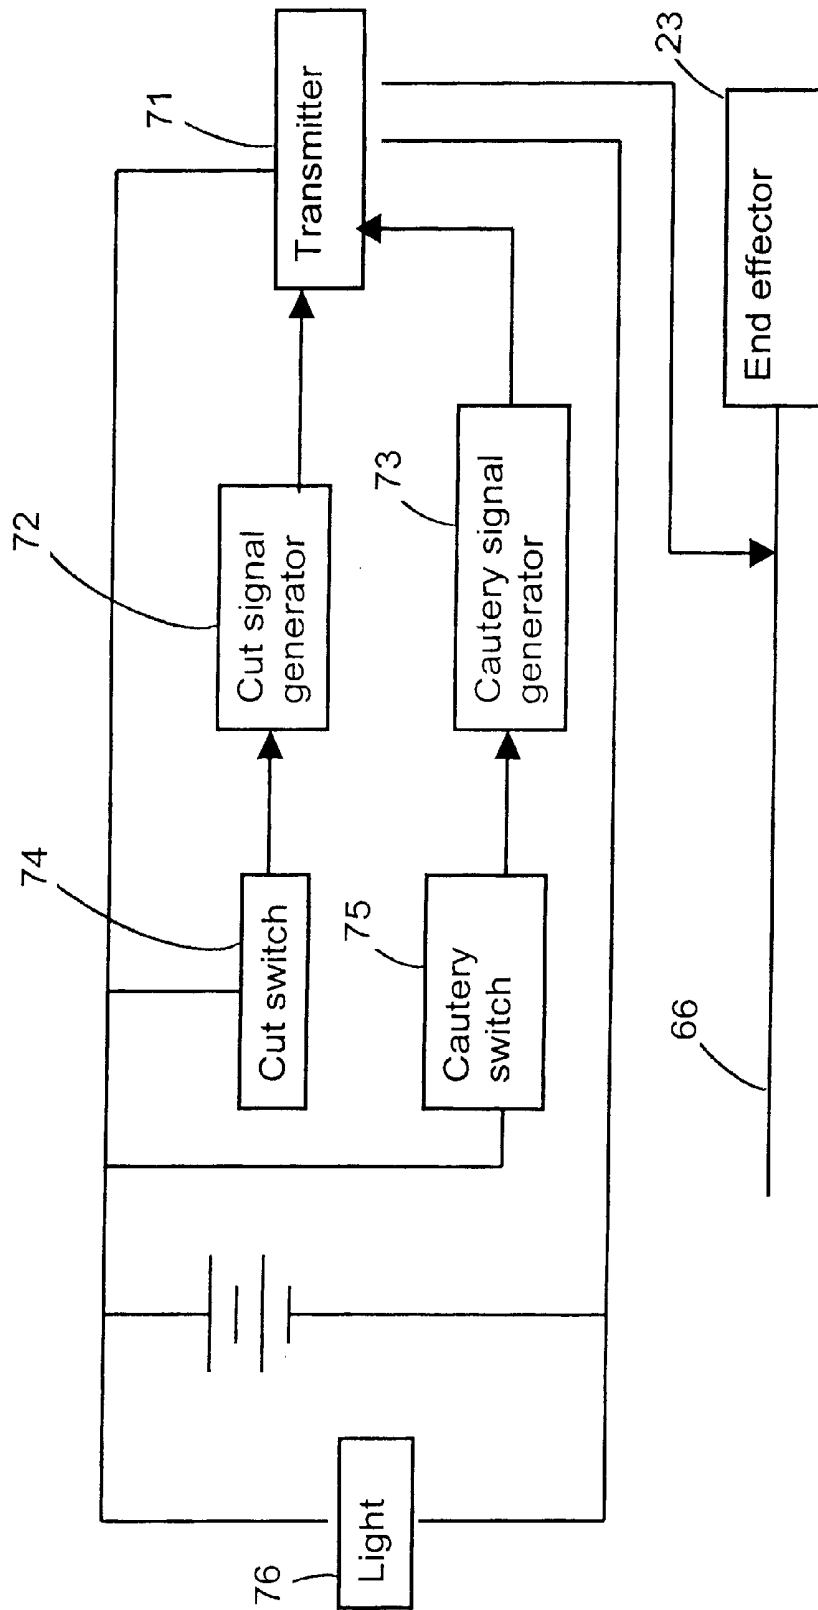


FIG. 7

(A) User indication:

(a) Cut operation



(b) Coagulation operation



(B) Transmitter function:



(C) Receiver receives after coupling and amplifying:



(D) Receiver timing circuitry receives:



FIG. 8

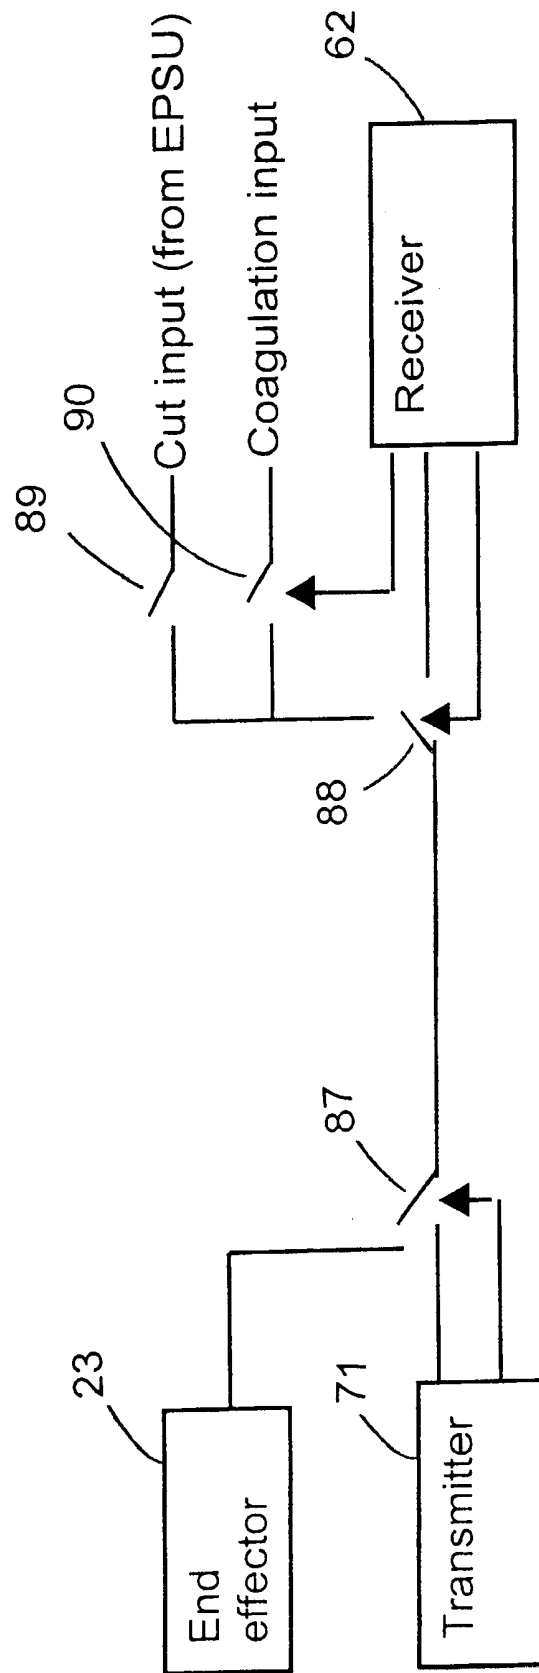


FIG. 9

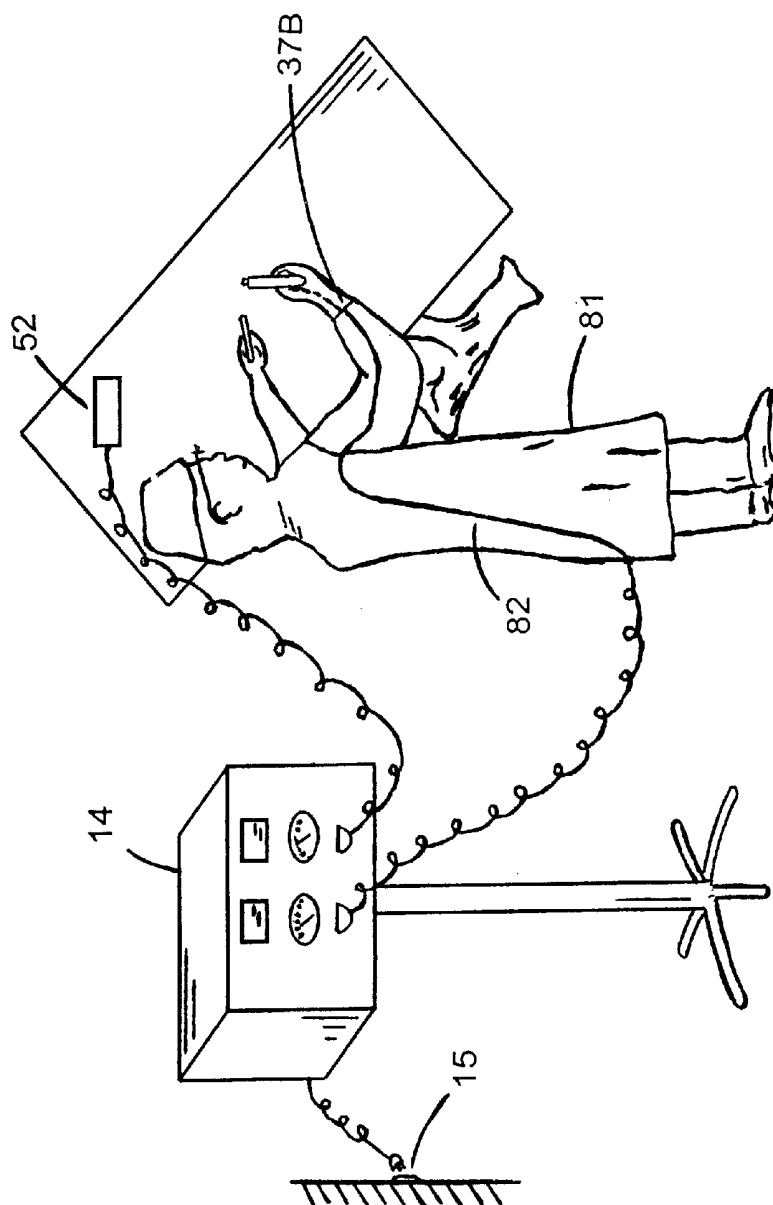


FIG. 10

WIRELESS ELECTROSURGICAL ADAPTER UNIT AND METHODS THEREOF

CROSS-REFERENCE TO RELATED APPLICATIONS

This application is a continuation-in-part of U.S. patent application Ser. No. 09/803,284 filed Mar. 9, 2001, entire contents of which are incorporated herein by reference.

FIELD OF THE INVENTION

The present invention generally relates to improved electrosurgical devices and methods for use. More particularly, this invention relates to a remotely wired adapter unit that can be coupled with an electrosurgical device for use as tool for ablating, cutting, or coagulating tissues via a wireless instrument with high frequency energy.

BACKGROUND OF THE INVENTION

Electrosurgical devices are used in nearly every operating room today. Electrocautery systems are used as a substitute for a mechanical, sharp blade for the purposes of cutting tissue or coagulation. An electrosurgical device may be used in open-chest surgeries or in minimally invasive endoscopic operations. Known electrosurgical instruments include, for example, monopolar blades, bipolar forceps, bipolar scissors, monopolar hooks, monopolar scissors, bipolar endocutters, electric coagulators, or the like. Each of those instruments has an electrosurgical end effector which is adapted to treat tissue through application of electrosurgical energy to tissue which is brought in contact with the electrosurgical end effector. Most known electrosurgical instruments are connected by electrical cords or wires to electrosurgical generators.

In general, the terms for electrosurgery, electrocautery, radiosurgery, diathermy, endothermy and radiofrequency heating have all been used to refer to tissue application of radiofrequency electricity to obtain a desired effect. In its classic meaning, electrocautery is defined as the use of electricity to heat an object, which is then touched to the tissue to singe vessels. Electrosurgery usually uses radiofrequency electricity to generate heat in the tissue itself rather than applying heat from an outside source.

It has been noticed by surgeons that the standard electrocautery instrument is inconvenient for them to use due to the attached wire or electrical cord. The wire could become tangled on the cautery instrument or on another object, and can be troublesome to their hand motion, make cautery awkward and less efficient. The electrical cord is also a nuisance in that it requires monitoring and careful placement to ensure that it remains sterile during surgical operations. Some surgeons have developed innovative methods for hanging or suspending the electrical cords, facilitating use of the electrosurgical devices and reducing the interference of the cords. For example, Weber et al. described a novel, yet simple, electrosurgical suspension apparatus that facilitate the performance of excision and repair, Mohs micrographic surgery, cosmetic surgery, and other forms of dermatologic surgery in *Dermatology Surgery* 2000;26:142-145.

It has been noted that certain tasks, such as laparoscopic cautery, would benefit from the application of cautery without the use of another instrument such as cautery obturator. Furthermore, a surgeon has noted that he cannot always see as clearly as he would like while cutting in non-lapascopic surgeries.

The prior art of surgical cautery is mainly performed electrically with a monopolar or bipolar cautery instrument.

The instrument transforms hospital available AC power into low current electricity, high frequency waveforms to cut through tissue and/or coagulate tissue. The attached electrical conducting wire or cord remains an unnecessary troublesome problem. This also applies to non-surgery electrical instruments.

An apparent form of the cordless electrosurgical device is a battery-powered cautery instrument or handpiece. U.S. Pat. No. 5,792,138 to Shipp discloses a cordless battery-operated electrocautery unit for use in surgical procedures. Though the battery-powered handpiece shows cordless advantages, the power may drift and the cautery efficiency demands constant battery exchange or recharge. The battery itself also increases the weight of the instrument.

Another alternative form of the cordless electrosurgical instruments is a specifically designed trocar or trocar adapter. U.S. Pat. No. 5,961,514 to Long et al. discloses a cordless electrosurgical instrument that is adapted to fit through a trocar which includes an electrosurgical adapter with at least a first electrical contact positioned in and extending axially along the elongated aperture, an electrical conductor, an external conductor, an outer housing and an electrical cord attached to it.

Electrosurgical generators supply electrical energy to the electrosurgical instruments through electrical cords. The cordless electrosurgical instrument as disclosed in U.S. Pat. No. 5,961,514 still requires a specially designed trocar having an attached electrical cord connected to a generator. Furthermore, the Long et. al. device needs an extra hand to engage the trocar or trocar adapter to the cordless instrument, which is not a contactably coupling technique and the device applies only to laparoscopic procedures.

Therefore, there is an unmet clinical need for integrating the power and signal source into a surgeon's gloves and/or gown as a remotely wired system while the actual cautery or ablation is done with a cordless instrument. The technology that is readily applicable on a wireless instrument could apply to any cautery instrument, ablation handpiece, any electrosurgery apparatus, or the like.

SUMMARY OF THE INVENTION

In general, it is an object of the present invention to provide a wireless adapter unit for contactably coupling an electrosurgical device to a remote power source. In one preferred embodiment, a remotely wired adapter unit comprises at least one surface electrical contact for contactably coupling the electrosurgical device to the remote power source through a coupling mechanism. In another preferred embodiment, the coupling mechanism further comprises a glove having at least one electrically conductive patch zone located at an outer surface of the glove for contactably coupling the wireless adapter unit to the remote power source. The glove may further comprise an insulated glove conductor having a first end and a second end, the first end of said insulated glove conductor being connected to one of the at least one electrically conductive patch zone of the glove and the second end of said insulated glove conductor being coupled to said remote power source.

In another embodiment, the wireless adapter system further comprises a gown having an insulated gown conductor, the insulated gown conductor being positioned between the second end of the insulated glove conductor and said remote power source.

In still another embodiment, the wireless adapter unit further comprises a signal transmitter and the remote power source comprises a switching/receiver unit, wherein signals

transmitted from said transmitter are received by the switching/receiver unit adapted for switching the power on. The signals may be transmitted either by short range radio-frequency transmission method or by capacitively coupled signal transmission method.

A method for performing a cordless electrosurgery operation, the method comprises contactably coupling a wireless adapter unit along with an electrosurgical device to a remote power source through a coupling mechanism on a surgeon's glove, a surgeon's gown, and the like.

BRIEF DESCRIPTION OF THE DRAWINGS

Additional objects and features of the present invention will become more apparent and the invention itself will be best understood from the following Detailed Description of the Exemplary Embodiments, when read with reference to the accompanying drawings.

FIG. 1 is an example of prior art electrosurgical device systems.

FIG. 2 is a wireless electrosurgery instrument system with a wireless adapter unit attaching to the proximal end of the electrosurgical device, constructed in accordance with the principles of the present invention.

FIG. 3 is a surgeon's glove serving as a coupling mechanism adapted for coupling the wireless adapter unit which is coupled to the electrosurgery device and to a remote power source.

FIG. 4 is the wireless adapter unit coupled to an electrosurgical device.

FIG. 4A is an electrosurgical instrument cut off at its cable cord.

FIG. 4B is an electrosurgical instrument with its internal wire exposed to be coupled to a wireless adapter unit.

FIG. 4C is a cross-sectional view of the wireless adapter unit from FIG. 4B depicting spring-loaded wire contacts to couple each of the wires originating from the cut electrosurgical device.

FIG. 5 is a schematic diagram illustrating the operating mode of the current wireless electrosurgery instrument system.

FIG. 6 is a switching/receiver unit for the wireless adapter unit coupled to the electrosurgical instrument.

FIG. 7 is a detailed block diagram including an end effector for the wireless electrosurgery instrument.

FIG. 8 is a dual function signals transmission and receiving sequence.

FIG. 9 is a block diagram of switches and basic system elements for dual cut and coagulation functions.

FIG. 10 is a perspective view of a simulated electrosurgery operation using the wireless electrosurgery device system of the present invention.

DETAILED DESCRIPTION OF THE EXEMPLARY EMBODIMENTS

Referring to FIGS. 1 to 10, what is shown is an embodiment of the wireless electrosurgical device system comprising a wireless adapter unit that can be coupled to an electrosurgical instrument, a coupling mechanism and a remote power source.

FIG. 1 shows an example of prior art electrosurgical device systems. Currently surgical cautery is mainly performed electrically with a monopolar cautery instrument, though bipolar cautery instruments are also used occasion-

ally. The prior art instrument transforms hospital available AC power (100 to 250VAC approximately, dependent upon the country) into low current electricity, high frequency (including radiofrequency) waveforms to cut through and/or to coagulate tissue. The cutting and coagulating waveforms are delivered to the tissue through a cautery scalpel that plugs into the cautery power supply through a standard cautery interface. There is a switch on the cautery scalpel that a practitioner or surgeon uses to close the appropriate circuit for either cutting or coagulation. Typically, a wired cautery instrument 11 with its attached wire or electrical cord 12 and a connector 13 is plugged into a standard electrosurgery power supply (EPSU) 14 or indirectly connected to a remote power source 15. The standard electrosurgery power supply in this invention can be a high frequency power generator, such as a radiofrequency generator.

FIG. 2 shows an electrosurgery instrument system constructed in accordance with the principles of the present invention. The remotely wired electrosurgical device system comprises a wireless adapter unit 20 having a transmitter and a remote power source 15, and the adapter unit 20 being connected through a cable cord of an electrosurgery instrument 21, wherein the wireless adapter unit 20 comprises at least one surface electrical contact 22 for contactably coupling the electrosurgical instrument to the remote power source through a coupling mechanism 39. The term "contactably coupling" as referred in this invention is defined as coupling two electrical contact elements by contacting without plugging or connection. U.S. Pat. No. 5,961,514 discloses a cordless electrosurgical instrument that uses a trocar or trocar adapter as a coupling element for power supply, wherein the trocar or trocar adapter needs to plug into the electrosurgery instrument using an extra hand. Loose wires from the trocar adapter become a troublesome problem to the surgeon. On the contrary, the wireless adapter unit of the present invention has neither loose wire to interfere with the surgeon's hand motions nor does it contain a battery-pack. The wireless adapter unit of the present invention connects with the commercially available electrosurgical device such as a cautery instrument to create a wireless electrosurgical system.

In one embodiment, the coupling mechanism 39 may comprise a surgery glove 31 to be worn by a surgeon for performing electrosurgery on a patient and a plug 38 to be connected to a switching/receiver 34, which is electrically connected through an end plug 35 to and becomes an additional component of the generator 14 and remote power source 15. In one preferred embodiment, the switching/receiver may be enclosed within an EPSU 14 or otherwise stand-alone. The surgery glove 31 has at least one electrically conductive patch zone 32 located at an outer surface of the glove for "contactably coupling" the wireless instrument to the remote power source through an attached conductor wire 33. As shown in FIG. 3 for an alternate bipolar electrocautery operation, a second electrically conductive patch zone 36 on the glove surface may be provided for contactably coupling a second of the at least one surface electrical contact 22 of the wireless adapter unit which is connected to a bipolar instrument, to the remote power source 15 as a returning conductor wire.

In FIG. 4, the electrosurgical instrument 21 is coupled to the wireless adapter unit 20 through a cable cord 25 with its plug inserted into a receptacle 24. The electrosurgical instrument may also comprise an end effector 23, the end effector being electrically coupled to one of the at least one surface electric contact 22 through a first internal conducting wire

within the instrument (not shown). Therefore, a complete circuit is established by a returning electrode **52** normally placed contactably under the patient and returning the current to the standard electrosurgery power supply unit (EPSU) **14**. In a bipolar instrument, the end effector **23** further comprises a returning electrode which is connected through a second internal conducting wire within the instrument to a second of the at least one surface electrical contact **22** for contactably coupling the wireless instrument to the remote power source through the coupling mechanism **39**. The coupling mechanism **39**, that may comprise at least one conducting wire, may be disposable or sterilized for re-use.

The end effector may include the distal portion of an electrosurgery instrument, such as bipolar forceps, bipolar scissors, a monopolar hook, monopolar scissors, bipolar endocutters, an electric coagulator, or the like. The instrument may be a scalpel that has an actuator mounted on said scalpel, the actuator being adapted for activating and deactivating the remote power source. Typically a small battery, such as an AAA size battery is optionally included in the end effector for light bulb use and for activating the feedback circuit.

In one embodiment as depicted in FIG. 4A, the electrosurgical instrument **21** may be a modified version of the prior art wired cautery instrument **11**, whereas the attached wire or electrical cord **12** onto the prior art cautery instrument **11** has been cut off configured for electrically coupling to the wireless adapter unit **20**. FIG. 4B illustrates the cut-off electrical cord **12** with its internal wires **25**—i.e., positive, negative, and ground—and the wireless adapter unit **20** to be coupled. FIG. 4C shows the cross-section of the wireless adapter unit **20** with contact openings **31** for the internal wires **25** that are stripped of their insulation. The spring-loaded plug **30** is pulled up while the stripped wire is inserted, and the plug is subsequently released to clamp down the wire. This is performed on all the internal wires **25** to create an electrical coupling between the electrical surgical instrument **21** and the wireless adapter unit **20**. In another embodiment, the receptacle **24** is configured to electrically couple the electrical cord **12** to the cable cord **25** on the wireless adapter unit **20**.

FIG. 3 shows a surgeon's glove serving as a coupling mechanism **39** adapted for coupling the electrosurgery instrument **21** through the wireless adapter unit **20** to a remote power source **15**. The glove may comprise at least an insulated glove conductor **37** having a first end **37A** and a second end **37B**, the first end of the insulated glove conductor being connected to the electrically conductive patch zone **32** of the glove and the second end of the insulated glove conductor being coupled to the remote power source optionally through the EPSU **14**.

In one preferred embodiment, the device system further comprises a gown **81** (as shown in FIG. 10) having an insulated gown conductor **82**, the insulated gown conductor being positioned between the second end **37B** of the insulated glove conductor **37** and the remote power source **15** through the EPSU **14**. For example, a monopolar electrosurgery instrument with cautery power delivered from a standard electrosurgery power supply unit to which the wireless adapter unit interface, to the wireless adapter unit **20** through an insulated conductor attached to the surgeon's glove and gown. The insulated conductor could be built into the glove and/or gown or attached on top of it with glue, Velcro® tape or other fixation technique. The insulated gown conductor could be right-handed, left-handed or both-handed. Typically the insulated conducting wires could be placed inside or outside of the gloves or gown.

The remotely wired electrosurgical device system of the present invention consists at least one of the following elements: an end effector that may contact the tissue for electrosurgery operation in either a monopolar fashion or a bipolar fashion, a control circuitry, signaling mechanism, light and driving circuit, and power source.

FIG. 5 shows a schematic diagram illustrating the operating mode of the current wireless electrosurgery instrument. A patient **51** has a returning electrode **52** for returning the electrical current back to the standard electrosurgery power supply unit (EPSU) **14**. The EPSU has typically a plurality of ports to receive electricity from the power source and the return current from the patient's ground, as well as the output ports (for example, three banana jacks in the standard model) to which the coupling mechanism **39** interfaces. This same interface is used to connect to the switching/receiver unit **34**. The wireless adapter unit **20** is remotely wired to the EPSU **14** by a coupling mechanism **39** in a "contactably coupling" fashion **84**. The switching/receiver unit **34** receives the signal from a transmitter **71** mounted at or adjacent the wireless adapter unit **20**.

The switching/receiver unit as shown in FIG. 6 comprises a receiver for the signals sent from the electronics in the wireless instrument either through RF or IR methods or along the line. The signals received are filtered through a signal filter **63** to activate the receiver relay **85** for power supply from the main power line **66** to the end effector. The interface **65** to EPSU is positioned between the EPSU **14** and the switching/receiver unit **34**.

FIG. 7 shows a detailed block diagram including an end effector **23** for the wireless electrosurgery instrument **21**. In a preferred embodiment for dual cut and cautery functions, a transmitter subsystem **71** emits the signals for a desired cutting or cautery function to the switching/receiver unit **34**. A light **76** is generally provided for the surgeon to better see the surgical site. After receiving and filtering the signal, the switching/receiver unit **34** then energize the circuits necessary to power oscillators attached to the main power line **66** for supplying the power to the end effector **23** of the wireless adapter unit **20**. At least two of the push-button switches are located at the electrosurgical device for different functions, such as cut, cautery or coagulation. In general, a cut switch **74** or a cautery switch **75** is depressed to activate a cut signal generator **72** or a cautery signal generator **73**, followed by transmitting the signal to the switching/receiver unit **34** for power energizing.

Several communicating/signaling methods for activating the end effector of the wireless electrosurgery instrument are available. The communicating/signaling method of the present invention may be selected from a group consisting of (a) infrared transmission, (b) short range radio frequency signaling, and (c) monopolar end effector using capacitive coupling of signals. Other communication/signal transmission methods, such as voice activation, sound, ultrasound, light, laser, foot-switching activation, or the like are also applicable in the present invention.

Infra-Red Transmission

The infrared transmission technique used infrared LEDs to transmit light pulses to perform the signaling and communication. Different signals for cutting, coagulating, inactive, or other function are made by varying the flashing frequency or other timing characteristics.

This communication could be done at very short range from one or several LEDs, possibly being arranged to form an optimized spreading of the light power, aimed at a receiver on the surgeon's glove. At the expense of power and the risk of line-of-sight blocking of the signal, this commu-

nication could also be done over a greater distance from a transmitter on top of the instrument to a receiver in a line-of-sight unobstructed location somewhere else in the operating suite.

The receiver (a phototransistor or other infra-red sensitive device) transduces the signal into something understandable by a microprocessor or other electronic circuitry. These electrical signals are then interpreted and the appropriate switches closed to turn on the desired electrosurgery operation.

This method of signaling has the limitations of interference by blocking of the signal forcing the transmitter to be close to the receiver, and through this limitation the necessity for extra wiring (including the receiver) being attached to the surgeon's arm.

Short Range RF Transmission

The short range RF transmission technique would work in much the same way but would instead use a RF transmitter located in the wireless electrosurgery instrument to transmit commands to a receiver. The receiver could be located on the surgeon's gown or elsewhere in the operating suite. The size and range of the antennae necessary would vary with the frequency permissible by the hospital and appropriate international standards. A good example of a system using short range RF transmission is a Bluetooth wireless mouse for a PC computer.

This would be an improvement over the infrared technique for its ability to communicate with an out-of-sight receiver, but would have the disadvantage of RF emissions in an operating room restricting the frequencies and the power levels being used. It would be possible to place the receiver somewhere on the operating table or close to the surgeon's hands for convenient signal transmission to the switching/receiver unit. In this application, transmitter must be a part of the wireless instrument. Antennae for receiving signals could be a second wire attached to the surgeon's gown.

Monopolar Cautery Using Capacitive Coupling of Signals

Another alternative is the one which integrates the signal and power delivery into the same conductor. This eliminates the requirement of a second set of wires on the user and the inconvenience of positioning them and maintaining appropriate orientations.

The transmitter in the wireless instrument in the user's hands and the receiver at the EPSU are now connected directly through a single conductor. The transmitter consists of circuitry to create voltage pulses of different time lengths depending on which task, for example, cut or coagulate, that the user wishes to perform.

These voltage pulses are sent along the single conductor to the receiver. Normally this would be ineffective as the transmitter being monopolar is effectively floating relative to the receiver. To get around this and create the illusion of a common basis (similar to ground but not electrically so), the signal is instead capacitively coupled to the receiver. The capacitor serves as a differentiator removing all DC content and passing only the AC. This transmitted signal is then reduced to two pulse spikes, one negative and one positive, framing the amount of time that the transmitter transmitted. The pulses are then massaged into regular electrical signals (e.g. at TTL levels) acceptable to timing circuitry, which calculates the time between the pulses and determines the user's intent. Once cut or coagulation is determined, the appropriate action is carried out.

Other transmission/communication methods are also applicable in the present invention. Two different frequencies are used to indicate the different operations. Receiver

contains electronics to determine which frequency broadcast would still use capacitive coupling and switches to protect the electronics. One needs to choose frequencies wisely. It generally uses a frequency much greater than 60 Hz to avoid the 60 Hz hums. Shielded cable could be used for most of the length to limit radiation.

Operating Mode

This operating mode is shown in FIG. 8 where the user indicates a cut and then a coagulate operation. " t_1 " indicates the time for cut signal, and " t_2 " indicates the time for coagulation signal. Note that these signals could be on the order of microseconds or less and as such the operations are separated as they would most likely not occur so close together in time.

The operating sequence as shown in FIG. 8 includes (A) user indication; (B) transmitter function; (C) receiver receiving after coupling and amplifying; and (D) receiver timing and processing circuitry receiving. The time required to indicate each operation mode could vary provided that there is still a sufficient difference in time length between the two signal types. After receiving and interpreting its orders, the selected operation would be carried out for a period of time, a number of multiples of the signaling time chosen to be long enough to achieve efficiency of operation and to remove noticeable and inconvenient delays from the user, and short enough so as to be turned off when no longer desired. This can be seen to form each operation into a packet of time consisting of signaling, delay to setup, operation, and delay to reset.

To avoid the problem of variation between clock oscillators (these are generally small, but crystal and other clock oscillators can have tolerances of a percent or two) creating skew problems or preventing proper use of the cautery due to inexact timing, the exact time taken for each of these pulses would be arranged between the transmitter and receiver in a calibration procedure at the start of any operation and before use. In the calibration procedure the transmitter sends to the receiver pulses for cutting, coagulation and for the amount of time that the operation will take place—the "on-time". The receiver receives each of these, measures them and stores for future comparison the amount of time each takes. This will facilitate coordination between the receiver and transmitter, removing the possibility of the transmitter circuitry being connected to (not isolated from) the conductor when the cautery waveform is applied.

It is important for the control circuitry to be isolated from the cautery waveforms due to the waveforms' high voltages (about 300 to 1500VDC) and high frequencies, which are enough to destroy circuit components. Although it is unlikely to be dangerous, it is probably best that the patient is isolated from the control signals. To evade unwanted exposure for the components and the patient, a method of separating the signals from the cautery was devised using electrically controlled mechanical relays and a timing scheme to isolate the two groups. This is shown in FIG. 8.

In FIG. 9, the transmitter 71 and receiver 62 are shown having outputs to various relays 87, 88, 89, 90. The transmitter controls a relay 87 that switches contact with the monopole between the transmitter and the cautery blade, an end effector 23. The receiver controls two relays: one relay that controls the type of cautery input (either cutting 89 or coagulation 90) and another relay 88 that switches monopole contact between the receiver and the cautery input.

Normally the relays are set to make the connection between the transmitter and receiver. After the user indicates their desired function and the transmitter transmits it, the transmitter activates relay 87 to connect up the end effector.

Simultaneously, the valid timing signal is received at the receiver 62 and the receiver disconnects itself and connects one of the cut or coagulation inputs to the monopole direct to the end effector, and from there the signal passes into the patient.

After the pre-arranged "on time" (set during the calibration period), the receiver disconnects the cautery signal input and the transmitter reconnects itself to the monopole. The transmitter then waits for the user to give more input and the receiver waits for the transmitter to send a signal. Or should the user be holding the switch indicating an operation, the process begins again immediately. There is no confusion here for the receiver as to when to begin as the transmitter drives the process entirely.

It is unlikely but possible that noise could be substantial enough to be received as a pulse into the system. It would then set off a counter to await the next pulse. Thus there needs to be a method of determining when a pulse is legitimate or not. An error correction scheme could be set up using the time lengths stored from the calibration procedure as normal points and allow some variation in time from these.

FIG. 10 shows a perspective view of a simulated operation using the wireless electrosurgery device system of the present invention. A surgeon who holds a electrosurgery instrument 21 connected to a wireless adapter unit has a coupling mechanism 39 comprising a glove 31 and/or a gown 81 of the present invention. The electrosurgery operation would become a complete circuit only when both the electrosurgery instrument contacts a patient who has a return electrode and the surgeon sends out a signal from the transmitter to activate the main power line through the EPSU 14.

The key advantage of the present invention over the prior art is its relative safety. The remotely wired electrosurgical device system of the present invention can only be activated by a surgeon or operator who has the coupling mechanism on his surgical glove and/or surgical gown. It is apparent that someone who picks up the instrument and depresses the transmitter button will not activate the instrument. This serves as a safety protection that is not available in other electrosurgical apparatus.

From the foregoing, it should now be appreciated that an improved wireless electrosurgery instrument having a coupling mechanism through a surgeon's glove and/or surgeon's gown has been disclosed. While the invention has been described with reference to a specific embodiment, the description is illustrative of the invention and is not to be construed as limiting the invention. Various modifications and applications may occur to those skilled in the art without departing from the true spirit and scope of the invention as described by the appended claims.

What is claimed is:

1. A remotely wired electrosurgical device system comprising a wireless adapter unit having a transmitter subsystem, and said wireless adapter unit connected to an electrosurgical instrument with a push-button switch mounted at or adjacent to said electrosurgical instrument and a remote power source comprising a switching receiver unit for power energizing, the transmitter subsystem emitting a signal by depressing said push-button switch to the switching receiver unit for energizing the power source, wherein the wireless adapter unit comprises at least one surface electrical contact for contactably coupling the wireless adapter unit connected to the electrosurgical instrument to the remote power source through a coupling mechanism.

2. The remotely wired electrosurgical device system of claim 1, wherein the coupling mechanism further comprises

a glove having at least one electrically conductive patch zone located at an outer surface of the glove for contactably coupling the wireless adapter unit to the remote power source.

3. The remotely wired electrosurgical device system of claim 2, wherein the glove comprises an insulated glove conductor having a first end and a second end, the first end of said insulated glove conductor being connected to one of the at least one electrically conductive patch zone of the glove and the second end of said insulated glove conductor being coupled to said remote power source.

4. The remotely wired electrosurgical device system of claim 1, wherein the electrosurgical instrument coupled to the wireless adapter unit comprises an end effector, said end effector being electrically coupled to one of the at least one surface electric contact through a first internal conducting wire within the instrument.

5. The remotely wired electrosurgical device system of claim 1, wherein the remote power source is a radio-frequency power generator.

6. The remotely wired electrosurgical device system of claim 4, wherein the end effector is selected from a group consisting of monopolar blade, bipolar forceps, bipolar scissors, a monopolar hook, monopolar scissors, bipolar endocutters, and an electric coagulator.

7. The remotely wired electrosurgical device system of claim 1, wherein the wireless adapter unit is coupled to an electrosurgical instrument such as a scalpel that has an actuator mounted on said scalpel, the actuator being adapted for activating and deactivating the remote power source through the said wireless adapter unit.

8. The remotely wired electrosurgical device system of claim 3, wherein the glove further comprises a second insulated glove conductor having a first end and a second end, the first end of said insulated glove conductor being connected to one of the at least one electrically conductive patch zone of the glove and the second end of said insulated glove conductor being coupled to said remote power source.

9. The remotely wired electrosurgical device system of claim 2, wherein the device system further comprises a gown having an insulated gown conductor, the insulated gown conductor being positioned between the second end of the insulated glove conductor and said remote power source.

10. The remotely wired electrosurgical device system of claim 1, wherein the wireless adapter unit of the electrosurgical instrument further comprises a signal transmitter and the remote power source comprises a switching/receiver unit, and wherein signals transmitted from said transmitter are received by the switching/receiver unit adapted for switching the power on.

11. The remotely wired electrosurgical device system of claim 10, wherein the signals are transmitted by infrared transmission method.

12. The remotely wired electrosurgical device system of claim 10, wherein the signals are transmitted by short range RF transmission method.

13. The remotely wired electrosurgical device system of claim 10, wherein the signals are transmitted by capacitively coupled signal transmission method.

14. A method for performing a cordless electrosurgery operation, the method comprising contactably coupling an electrical surgical instrument and a remote power source through a wireless adapter unit connected to the proximal end of the electrical surgical instrument and by a coupling mechanism mounted on a surgeon's glove, the wireless adapter unit comprising a transmitter subsystem emitting a signal for either cutting or cautery, wherein the transmitter

11

subsystem sends out a signal to activate the power source depending on energy needs of cutting or cautery.

15 15. The method according to claim 14, wherein the coupling mechanism further comprises an electrically conductive patch zone located at an outer surface of the surgeon's glove for contactably coupling the wireless adapter unit of the electrosurgical instrument to the remote power source.

10 16. The method according to claim 15, wherein the coupling mechanism further comprises a gown having an insulated gown conductor, the insulated gown conductor being positioned between the electrically conductive patch zone of the glove and said remote power source for contactably coupling the wireless adapter unit of the electrosurgical instrument to the remote power source.

15 17. The method according to claim 14, wherein the signal is transmitted by infrared transmission method.

18. The method according to claim 14, wherein the signal is transmitted by short range RF transmission method.

20 19. The method according to claim 14, wherein the signal is transmitted by capacitively coupled signal transmission method.

20 20. The method according to claim 14, wherein the signal is by ultrasound signal transmission method.

25 21. The method according to claim 14, wherein the signal is transmitted by voice activation transmission method.

12

22. The method according to claim 14, wherein the step of sending out the signal is activated by foot-switching activation method.

23. A method for performing a cordless electrosurgery operation using an electrosurgical device system, wherein the device system comprises a wireless adapter unit having a transmitter subsystem, and said wireless adapter unit connected to an electrosurgical instrument with a push-button switch mounted at or adjacent to said electrosurgical instrument and a remote power source comprising a switching receiver unit for power energizing, and wherein the wireless adapter unit comprises at least one surface electrical contact for contactably coupling the wireless adapter unit to the remote power source through a coupling mechanism, the method comprising:

15 contactably coupling the wireless adapter unit connected to the electrosurgical instrument and the remote power source through the coupling mechanism mounted on a surgeon's glove;

depressing the push-button switch for sending out a signal from the transmitter subsystem to the switching receiver unit; and applying the wireless adapter unit connected to the electrosurgical instrument to contact a patient for performing the cordless electrosurgery operation.

* * * * *

专利名称(译)	无线电外科适配器单元及其方法		
公开(公告)号	US6569163	公开(公告)日	2003-05-27
申请号	US09/957375	申请日	2001-09-20
[标]申请(专利权)人(译)	HATA CARY 张骥		
申请(专利权)人(译)	HATA CARY 张骥		
[标]发明人	HATA CARY ZHANG JI		
发明人	HATA, CARY ZHANG, JI		
IPC分类号	A61B18/14		
CPC分类号	A61B18/14		
其他公开文献	US20020128644A1		
外部链接	Espacenet USPTO		

摘要(译)

一种无线适配器单元，其耦合到电外科器械，所述电外科器械包括至少一个表面电触点，用于通过耦合机构将电外科器械可接触地耦合到远程电源，其中，所述耦合机构包括穿过外科医生手套的绝缘导体和/或外科医生的礼服。

