

(19)



(11)

**EP 2 561 350 B1**

(12)

**EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:  
**28.06.2017 Bulletin 2017/26**

(51) Int Cl.:  
**G01N 33/48 (2006.01) G01N 33/537 (2006.01)**

(21) Application number: **10848598.8**

(86) International application number:  
**PCT/US2010/028683**

(22) Date of filing: **25.03.2010**

(87) International publication number:  
**WO 2011/119163 (29.09.2011 Gazette 2011/39)**

**(54) METHOD AND SYSTEM FOR ANALYZING A BLOOD SAMPLE**

VERFAHREN UND SYSTEM ZUR ANALYSE EINER BLUTPROBE

PROCÉDÉ ET SYSTÈME PERMETTANT D'ANALYSER UN ÉCHANTILLON DE SANG

(84) Designated Contracting States:  
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO SE SI SK SM TR**

(56) References cited:  
**US-A- 5 616 501 US-A- 5 616 501**  
**US-A1- 2006 160 229 US-A1- 2007 105 230**  
**US-A1- 2009 076 736 US-A1- 2010 075 369**

(30) Priority: **24.03.2010 US 730977**

- **STEINKAMP J A: "FLOW CYTOMETRY", REVIEW OF SCIENTIFIC INSTRUMENTS, AIP, MELVILLE, NY, US, vol. 55, no. 9, 1 September 1984 (1984-09-01), pages 1375-1400, XP000652545, ISSN: 0034-6748, DOI: 10.1063/1.1137948**
- **STEWART C C ET AL: "RESOLVING LEUKOCYTES USING AXIAL LIGHT LOSS", CYTOMETRY, vol. 10, no. 4, 1989, pages 426-432, XP002718817, ISSN: 0196-4763**
- **SCHWARZ H P ET AL: "Phospholipid composition of blood plasma, erythrocytes, and "ghosts" in sickle cell disease.", CLINICAL CHEMISTRY SEP 1977, vol. 23, no. 9, September 1977 (1977-09), pages 1548-1550, XP002718818, ISSN: 0009-9147**

(43) Date of publication of application:  
**27.02.2013 Bulletin 2013/09**

(73) Proprietor: **Beckman Coulter, Inc. Brea, CA 92821 (US)**

- (72) Inventors:
- **GODEFROY, Christophe, P. Miramar, FL 33027 (US)**
  - **RILEY, John, Steven Miami, FL 33196 (US)**
  - **VIDAL, Patricio, J. Miami, FL 33196 (US)**

(74) Representative: **Boult Wade Tennant Verulam Gardens 70 Gray's Inn Road London WC1X 8BT (GB)**

**EP 2 561 350 B1**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

## Description

### BACKGROUND

#### Field of the Invention

**[0001]** This invention relates in general to the methods and systems for analyzing the blood samples using a particle analyzer, and more particularly to determining reticulocytes and hard-to-ghost cells.

#### Background

**[0002]** Each year, millions of Americans are affected by blood diseases. Examples of blood pathologies include various hematological malignancies, such as leukemias and lymphomas, hemoglobinopathies, which encompass a number of anemias of genetic origin, such as thalassemia, Cooley's Disease, and sickle-cell anemia (HbS disease), as well as various clotting and bleeding disorders. Blood abnormality can also be a secondary consequence associated with other conditions, such as HIV/AIDS, malignant tumors, and autoimmune disorders. Most of these conditions have significant morbidity and mortality and commonly cause severe pain in the affected patient. Early diagnosis of these disorders is critical so patients who have the disease can receive proper treatment and disease management.

**[0003]** Blood is a specialized bodily fluid that delivers necessary substances, such as nutrients and oxygen, to the body's cells and transports waste products away from those same cells. The predominant cell in blood is the erythrocyte, i.e., red blood cell or red cell. In a peripheral blood smear, erythrocytes derive their reddish color from protein hemoglobin, and usually appear round or oval with a pale-staining center region. Their biconcave morphology increases the cell's surface area and facilitates diffusion of oxygen and carbon dioxide from the cell. A typical erythrocyte has a lifespan of about 120 days.

**[0004]** Erythrocytes develop from nucleated precursor cells in the bone marrow. Immature erythrocytes, i.e., reticulocytes, have organelles that contribute to an increased hemoglobin content and gas-carrying capacity. Reticulocytes can be recognized in peripheral blood smears when a special stain is used to stain their polyribosome or ribonucleic acid (RNA). Under typical conditions, reticulocytes account for about 1-2% of red blood cells in a sample. However, during certain periods of physical need, the reticulocyte count may increase.

**[0005]** Blood tests can be used to determine physiological and biochemical states, such as disease, mineral content, drug effectiveness, and organ function. In confirming or helping to confirm the diagnosis of diseases such as, for example, various forms of anemia or acute internal hemorrhage, the determination of reticulocytes can be of critical importance.

**[0006]** Automated reticulocyte analysis can be done using a particle analyzer such as a flow cytometer or

hematology analyzer. Example particle analyzers include, the UniCel® DxH 800 System from Beckman Coulter and XT-2000 from Sysmex Corporation. The preparation of a blood sample for cytometric flow or hematology analysis generally involves taking a whole blood sample and performing one or both the steps of incubating the sample of blood with a vital stain such as New Methylene Blue (NMB) and diluting the blood sample with a hypotonic acid that clears hemoglobin. The staining precipitates RNA within the erythrocytes. Diluting with a hypotonic acid clears hemoglobin, leaving the stained RNA within the cells. The process of removing hemoglobin is commonly referred to as "ghosting." The blood sample, or portion of it, is then subjected to analysis in a flow cell of a particle analyzer. Typically, cells in a sheath fluid pass through a point in the flow cell, one by one, where they are interrogated by one or more beams of light. Several measurements are generated for each passing cell. The interrogation of a single cell is referred to as a cell event. Commonly recorded measurements per cell event include, forward light scatter, axial light loss, and fluorescence. Some particle analyzers also collect a direct current impedance (DC) measurement which is a measure of how much impedance is exerted by a cell. The DC measurement, which is obtained from applying the maximum current such that the cell membrane is not permeated and no current flows through the cell, is also known as Coulter volume or volume.

### 30 SUMMARY OF THE INVENTION

**[0007]** The present application is directed towards the analysis of particle analyzer data. The present invention is defined in the claims. In one embodiment, an automated method of enumerating hard-to-ghost cells which are defined as cells that retain at least 30% of their original hemoglobin content following mixing with a ghosting reagent in a blood cell sample comprises: mixing a blood cell sample with a nucleic acid stain and a ghosting reagent to remove hemoglobin from red blood cells, thereby generating a ghosted blood cell sample; passing the ghosted blood cell sample through a cytometric flow cell; analyzing the ghosted blood cell sample in the cytometric flow cell by using light scatter and axial light loss measurements thereby generating event data comprising an axial light loss and a light scatter measurement for each cell; differentiating hard-to-ghost cells in the ghosted blood cell sample from other cells using the analysis by the event data comprising an axial light loss measurement and a light scatter measurement for each cell; and enumerating the hard-to-ghost cells.

**[0008]** Further features and advantages of the present invention, as well as the structure and operation of various embodiments thereof, are described in detail below with reference to the accompanying drawings. It is noted that the invention is not limited to the specific embodiments described herein. Such embodiments are presented herein for illustrative purposes only. Additional em-

bodiments will be apparent to persons skilled in the relevant art(s) based on the teachings contained herein.

#### BRIEF DESCRIPTION OF THE DRAWINGS

##### [0009]

FIG. 1 is a view of event data from analysis of a blood sample using a flow cytometer, in two-dimensions. FIG. 2 illustrates steps in analyzing immature reticulocytes in a blood sample according to an embodiment of the present invention.

FIG. 3 shows further details of the preprocessing step shown in FIG. 2, according to an embodiment of the present invention.

FIG. 4 shows further details of the measuring step shown in FIG. 2, according to an embodiment of the present invention.

FIGS. 5(A) and 5(B) are two-dimensional views of event data from the analysis of a blood sample. FIG. 5(B) is a view of the event data shown in FIG. 5(A) with the hard-to-ghost cell population removed.

FIG. 6 shows the same event population shown in FIG. 5(A), but using axial light loss (ALL) and UMALS instead of the conventional DC and UMALS.

FIGS. 7 (A-C) show several two-dimensional views illustrating event data with varying capability to identify the hard-to-ghost cell population.

FIG. 8 shows further details of the measuring step shown in FIG. 2, according to another embodiment of the present invention.

FIG. 9 is a system for evaluating immature reticulocytes according to an embodiment of the present invention.

FIG. 10(A) shows a three-dimensional view of the event data from the analysis of a blood sample from a healthy individual. Hard-to-ghost cells 1010, mature red blood cells 1020, and reticulocytes 1030 are distinctly differentiated in the view.

FIG. 10(B) shows a three-dimensional view of the event data from the analysis of a blood sample from a patient diagnosed with sickle cell anemia. Hard-to-ghost cells 1010, mature red blood cells 1020, and reticulocytes 1030 are distinctly differentiated in the view.

FIG. 10(C) shows a three-dimensional view of the event data from the analysis of a blood sample from a patient diagnosed with Thalassemia. Hard-to-ghost cells 1010, mature red blood cells 1020, and reticulocytes 1030 are distinctly differentiated in the view.

FIG. 11 illustrate an average % of "hard-to-ghost" cells in blood samples drawn from healthy individuals.

FIG. 12 illustrate an average % of "hard-to-ghost" cells in blood samples drawn from patients suffering from various diseases.

[0010] The features and advantages of the present invention will become more apparent from the detailed description set forth below when taken in conjunction with the drawings. In the drawings, like reference numbers generally indicate identical, functionally similar, and/or structurally similar elements. Generally, the drawing in which an element first appears is indicated by the leftmost digit(s) in the corresponding reference number.

#### 10 DETAILED DESCRIPTION

[0011] The present invention relates to particle analysis data processing. While the present invention is described herein with reference to illustrative embodiments for particular applications, it should be understood that the invention is not limited thereto. Those skilled in the art with access to the teachings herein will recognize additional modifications, applications, and embodiments within the scope thereof and additional fields in which the invention would be of significant utility.

#### Overview

[0012] As described in the background section above, the automated ability to determine the distribution of red blood cells in a blood sample is a vital capability for several applications. The methods and systems disclosed herein yield an improved automated measure of cell populations in a blood sample. In one embodiment, the hard-to-ghost cells are differentiated and enumerated using methods provided herein.

[0013] Exemplary environments in which this invention may be practiced include particle analyzers, such as Beckman Coulter's UniCel® DxH 800 System. The UniCel® DxH 800 System, for example, uses the Coulter proprietary Volume, Conductivity, and LightScatter (VCS) technology to evaluate hydrodynamically focused cells within a flow cell. VCS uses three independent energy sources that work in concert with each other for cell measurement: a low frequency direct current power source to measure volume; a high frequency power source to measure conductivity, and a laser light source to measure scatter. The volume measurement is performed using the Coulter principle of electrical impedance to physically measure the volume that the entire cell displaces in an isotonic diluent. This method accurately sizes all cell types regardless of their orientation in the light path. Alternating current in the radio frequency (RF) range short circuits the bipolar lipid layer of a cell's membrane, allowing the energy to penetrate the cell. This powerful method is used to collect information about cell size and internal structure, including chemical composition and nuclear volume. A laser and multiple-angle light scatter detectors provide information about a cell's internal structure, granularity, and surface morphology. In addition, VCS devices use the highly accurate DC measurement of volume to obtain other measurements that are adjusted for cell size from conductivity and scatter.

It should be noted, however, that the teachings in this disclosure are not limited to devices using VCS technology.

**[0014]** FIG. 1 shows a two-dimensional scatter plot of a blood sample based on event data generated from measurements of blood using a particle analyzer. Each data point appearing in the scatter plot is based on selected measurements obtained from one cell event, i.e., the interrogation of an individual cell by an electric current and a laser beam in the flow cell. Event data populations of different cell types commonly found in a blood sample are shown in the scatter plot. In general, sufficient separation exists between the populations of red cells as a whole (i.e., erythrocytes 102 and reticulocytes 104), platelets 108, and white cells 106, that known techniques allow for gating the red cell population as a whole, for example, based on the area defined by lines 122 and 124. Gating refers to the process of filtering selected measurements from multi-parameter data, for example, as described above, separating red cells (erythrocytes and reticulocytes), platelets and white blood cells by testing the measurements generated for each cell event against known threshold values. For example, line 124 can be a threshold volume value and line 122 can be a threshold light scatter value, where cell events with volume measurements above line 124 and light scatter (often used in the form of log of light scatter) value less than line 122 correspond to either erythrocytes or reticulocytes. In existing systems, the reticulocyte population can also be gated, for example, by a line such as line 130. The events to the right of line 130 are reticulocytes, whereas the events to the left of line 130 are mature red cells.

### Analyzing Reticulocytes

**[0015]** In one aspect, methods for analyzing reticulocytes in a blood sample are presented. FIG. 2 is a flow-chart of steps in evaluating reticulocytes according to an embodiment of the present invention. In step 202, a blood sample is prepared for analysis in a particle analyzer. Preparation can include ghosting the blood sample and/or staining the sample with a suitable dye or stain. FIG. 3 illustrates preparation step 202 in further detail, according to one embodiment. In step 302, the blood sample can be combined with a vital stain to further delineate reticulocytes. For example, a non-fluorochrome dye that precipitates intracellular ribonucleic acid (RNA) of the reticulocyte can be used. Examples of suitable stains include, but are not limited to, New Methylene Blue (known as Reagent A of the Coulter Retic Pak™), Oxazine 750, and Brilliant Cresyl Blue. RNA, having been precipitated, will have higher density which will enhance the delineation of the RNA content in each cell. Using a non-fluorescent dye to measure reticulocytes has the added advantage to allow the blood sample to be further analyzed for other constituents by utilizing a fluorescent dye, if desired. Examples of suitable fluorescent dyes

include, but are not limited to, thiazole orange and polymethine. Additional preparatory steps are possible in various embodiments of the present invention. For example, in some embodiments a fluorescent dye can be combined with the blood sample to measure additional properties of the sample using a fluorescence measure.

**[0016]** To further effectuate the examination of a composition of a blood sample, the blood sample can be combined with a reagent such as, for example, a reticulocyte ghosting solution having potassium thiocyanate and sulfuric acid (step 304). This type of ghosting reagent can be obtained as a commercial product known as Reagent B of the Coulter Retic Pak™. Other ghosting reagents known to those skilled in the art can be used. The ghosting process releases the hemoglobin in red blood cells, resulting in ghosted cell. The term "ghosted cell", as used herein, refers to a red blood cell that has more than 70% of its hemoglobin content removed. Preferably, the cell has more than 90% and even more preferred has more than 95% of the hemoglobin removed. In other words, the ghosted cell retains less than 30% of its original hemoglobin. The reduction of the hemoglobin content enhances the definition of the reticulum to permit cytometric flow determination of the reticulocytes. More specifically, the reduction in hemoglobin content of the red blood cells enables the differentiation of the reticulocytes from the mature RBC when measuring by a non-fluorescent method comprising light scatter and DC.

**[0017]** In addition to facilitating the release of hemoglobin, the ghosting process can also sphere the red blood cells giving the cells a more regular shape, and thereby permitting more predictable light scatter measurements. The native reticulocyte has an irregular shape which produces unpredictable light scatter information when subjected to a light beam. The spherizing of the red blood cell provides reproducible light scatter information which forms the basis for determining the reticulocytes in the sample. In some embodiments, it might be advantageous to combine the blood sample with a spherizing agent. The spherizing agent is used in an amount effective to cause the reticulated erythrocytes and red blood cells to isovolumetrically sphere to eliminate orientation artifacts in analysis of the reticulocytes. In some embodiments, the spherizing reagent is a zwitterionic surfactant which isovolumetrically spheres the red blood cells. Examples of spherizing agents suitable for the present invention include, but are not limited to, lauroamidopropylbetaine, cocoamidopropylbetaine and cocoamidodisulfobetaine.

**[0018]** It has been previously found that the ghosting process is affected by temperature. Temperatures below 55°F. appear to retard the ghosting process and longer time periods are necessary to permit the ghosting process to occur. In some embodiments, the blood sample will be mixed with the ghosting solution at a temperature of at least 55° for approximately 30 seconds. In one embodiment, ghosting of blood sample will be conducted at 106° F. (41° C.).

**[0019]** In some embodiments, the pH of the ghosting solution should be not higher than 3.0. In one embodiment, the pH of the ghosting solution is approximately 1.0 to 2.0. In addition, it appears that the acidic ghosting solution solubilizes the hemoglobin and facilitates its removal from the blood cell. It has been noted that when utilizing potassium thiocyanate, sulfuric acid is the preferred acid to be utilized in the combination. The preferred concentration for the potassium thiocyanate is approximately from 1.0 to 6.0 grams per liter, and for the sulfuric acid is approximately from 0.7 to 3.0 grams per liter.

**[0020]** The osmotic pressure of the ghosting solution should be controlled so that there is a rapid, but controlled swelling of the blood cell. The osmotic pressure of the ghosting solution should be at least about 75 milliosmoles. The osmotic pressure causes the blood cell to swell and release the hemoglobin within thirty (30) seconds of mixing with the ghosting solution. If the osmotic pressure is less than about 75 milliosmoles, then the blood cell will not retain an intact cell membrane and will lyse. More specifically, lower osmotic pressure results in red cells that are damaged so that reticulocyte enumeration is not reliable. If the osmotic pressure is not sufficient, the blood cells will retain hemoglobin which will obscure reticulocyte differentiation. In some embodiments, the osmotic pressure of the ghosting solution will range from about 75 to about 110 milliosmoles. In other embodiments, the osmotic pressure of the ghosting solution will be in the range of about 82 to about 105 milliosmoles.

**[0021]** Returning to FIG. 2, in step 204, the blood sample is analyzed using a particle analyzer. In one embodiment, the particle analyzer is a hematology analyzer. For example, the blood sample, or a portion of it, is introduced into the particle analyzer. Under hydrodynamic pressure, the blood sample flows, cell by cell, through a flow cell. Within the flow cell, several parameters of the individual cells are measured. For example, particle analyzers using the VCS technology can perform the volumetric sizing of a cell, conductivity of a cell, and light scatter, simultaneously for each cell. FIG. 4 is a flowchart of step 204 in further detail, according to an embodiment of the present invention.

**[0022]** In step 402, the blood sample prepared in step 202, is introduced into a flow cell for analysis. In step 404, in one embodiment, the sample is interrogated by energy from three independent sources as it flows, cell by cell, through an interrogation point in the flow cell. In step 406, the light scatter measurement is recorded for each cell event. As the RNA content decreases with the maturity of the reticulocyte, it can be expected that the light scatter measurement decreases. Several measurements of light scatter can be available, for example, and without limitation, include forward light scatter measurements. Forward scatter measures the light that passes through the cell being interrogated and that is deflected from the axis of the beam of light. Examples of forward light scatter include, but are not limited to, lower median

angle light scatter (LMALS), upper median angle light scatter (UMALS), and low angle light scatter (LALS). The LMALS refers to light scattered at an 9°-19° angle from the axis of the beam, UMALS refers to light scattered at an 20°-43° angle from the axis of the beam, and LALS refers to light scattered at approximately 5.1° angle from the axis of the beam. Another light scatter measurement, side angle light scatter (SALS), can measure light scattered at 90° angle. In some embodiments, the analyses of blood sample will include a measurement of axial light loss (ALL). ALL is the amount of light lost at about 0° to 0.5° angle relative to the axis of the beam.

**[0023]** In step 408, another measurement that is indicative of reticulocyte maturity is collected. For example, in one embodiment of the present invention, the size of the cell can be measured. The size of the cell is known to decrease with the maturity of the reticulocyte, in general, as the RNA content decreases. As an example, the size of the cell, or cell volume, can be measured using the DC measurement. The peak amplitude of the DC pulse is a function of cell volume. Other measurements indicative of reticulocyte maturity, including direct or indirect ways of measuring the volume of the cell, can be used in this step. For example, fluorescence measurement to indicate the amount of RNA in the cell, or other modes of measuring cell volume can be used. As another example, forward scatter can also be used to indicate cell size.

**[0024]** Returning to FIG. 2, in step 206 a reticulocyte population is identified from the entire cell event population. Scatter plots of the event data, using various axis, help identify blood cell distribution patterns. As an example, the event data can be visualized in a scatter plot, such as, for example, FIG. 1, where the light scatter is on the x-axis and volume (DC) is on the y-axis. As indicated earlier with respect to FIG. 1, the reticulocyte population 104 can be identified separately from erythrocytes 102, platelets 108 and white cells 106. The accuracy of the reticulocyte population is dependent particularly on how definitively line 130 separating the reticulocytes from the red cells can be determined. For example, in one embodiment, while line 130 can be superimposed on the scatter plot 100 based on threshold light scatter and volume measurement values derived empirically from previous collections of measurements, line 130 can fail to correctly separate erythrocytes 102 from reticulocytes (104), particularly with regard to cell events that lie in close proximity to line 130 in scatter plot 100.

**[0025]** Returning yet again to FIG. 2, in step 207, one or more reticulocyte measures can be reported. In one embodiment the reticulocyte fraction is reported as the ratio of a predetermined number of regions defined on the mapping function to the entire red blood cell population. In another embodiment reticulocytes can be reported as a percentage or absolute number. Reporting involves outputting one or more measurements to a display or other output device such as a computer file.

### Detecting Hard-to-Ghost Cells

**[0026]** In one aspect, the method of the present invention allows for the accuracy of reticulocyte detection that is reported to be improved with having more accurate sample data based on which to compute reticulocyte information. It has been observed, in some blood samples, that after the initial ghosting process some cells remain that were either not ghosted or were only partially ghosted, i.e., "hard-to-ghost" cells. For the purposes of the present invention, the term "hard-to-ghost cell" will refer to a cell which has retained at least 30% of its original hemoglobin content. In other words, the hard-to-ghost cell has less than 70% of its original hemoglobin removed. Preferably, the cell has more than 50% and even more preferred has more than 70% of the original hemoglobin content. The ghosting process, for example, by combining a hypotonic acid solution with the blood sample, is intended to clear hemoglobin from the cells. Without ghosting or with inefficient ghosting (i.e., when the cells lose less than 30% of their hemoglobin content), erythrocytes may not clearly differentiate from reticulocytes. Another view of the difference from ghosted cells compared to hard-to-ghost cells can be seen in FIG. 6 which shows population 610 of the hard-to-ghost cells being positioned in upper portion of the scatter plot of axial light loss versus UMALS. When hard-to-ghost cells are present in the blood sample, and the blood sample is analyzed using light scatter and DC, the differentiation of the reticulocytes from the mature red cells can fail because the hard-to-ghost cell population is dense and is generally positioned within the reticulocyte region. Some embodiments of the present involve detecting hard-to-ghost cells in the total population of blood cells.

**[0027]** FIGS. 5(A) and 5(B) show the contrast presented in scatter plots of the same event data with and without hard-to-ghost cell events, using conventional light scatter or upper medium angle light scatter (UMALS), and DC axis. In FIG. 5(A) the scatter plot includes hard-to-ghost cell events. The boundary 510 shows the location of a hard-to-ghost cell event population. FIG. 5(B) shows the same event population after hard-to-ghost cell events, including the population defined by boundary 510, are removed. In both FIGS. 5(A) and 5(B), the events below boundary 530 correspond to platelets and the events to the right of boundary 520 correspond to white blood cells. As can be seen by the location of the boundary 510, the hard-to-ghost cell event population spans the separation of the mature red blood cell population and the reticulocyte population, thereby making it difficult to clearly distinguish between mature red blood cells and reticulocytes. In contrast, when the hard-to-ghost cell event population is removed, as shown in FIG. 5(B), a clear boundary 511 can be defined between the mature red blood cells and reticulocytes. A visual comparison of FIGS. 5(A) and 5(B) illustrates the difficulty in identifying and separating the mature red cells from reticulocytes when hard-to-ghost cells are present.

**[0028]** In this embodiment, the axial light loss measurement enables the discrimination of the hard-to-ghost population from the rest of the sample. It has been unexpectedly found by the inventors of the present invention that the same event population that cannot identify the hard-to-ghost population based on the conventionally used light scatter measurement, can now distinguish the population using an axial light loss measurement. For example, FIG. 6 shows the same event population shown in FIG. 5(A), but using axial light loss (ALL) and UMALS instead of the conventional DC and UMALS. Using ALL, hard-to-ghost cell events can be clearly identified, as shown by the area within the boundary 610.

**[0029]** FIGS. 7(A-C) illustrate the hard-to-ghost cell event removal of another blood sample using ALL in an embodiment of the present invention. Scatter plot 710 shows the generally used UMALS and DC. In scatter plot 710, hard-to-ghost cells are present (as shown within boundary 711), but cannot be clearly distinguished from other red blood cells. However, when the same data is shown in scatter plot 720, having axial light loss (ALL) and UMALS as axis, the ability to detect hard-to-ghost cells is vastly improved. Based on ALL, the hard-to-ghost population 721 is clearly discernible from the other event populations.

**[0030]** In one embodiment of the present invention, the cell events corresponding to the hard-to-ghost population can be filtered-out, and the remaining cell events can be displayed in scatter plot, for example such as 730, using UMALS axis and DC axis. Filtering-out cell events corresponding to the hard-to-ghost population can be accomplished by gating the hard-to-ghost population either, automatically based on, for example, threshold ALL and UMALS values determined empirically, or with manual operator assistance. A visual comparison of scatter plots 730 and 710 illustrates the clearer distinction between the mature red blood cell population to the left of boundary 731 and the reticulocyte population to the right of boundary 731.

**[0031]** As shown in FIG. 6 (specifically the area within boundary 610) and FIGS. 7(A-C) (specifically the area within boundary 721), when using ALL, hard-to-ghost cells can be identified as a distinct population from other populations such as mature red blood cells, reticulocytes, platelets and white blood cells. The hard-to-ghost cells generally display a higher ALL than other blood cell types except for white blood cells. White blood cells can be distinguished due to their high light scatter measurements relative to other blood cell types. The high ALL of the hard-to-ghost cell population can be attributed to the relatively high light absorption of hemoglobin. At a laser wavelength of 488nm (the wavelength used in the particle analyzer that yielded results shown in FIGS. 5(A), 5(B), 6 and 7(A-C)) hemoglobin displays very high optical absorption that leads to a high level of ALL. In general, hemoglobin shows increased absorption of light when the light is between 400-500nm wavelength.

**[0032]** Detection of the hard-to-ghost cells in a blood

sample being analyzed can be accomplished by the embodiment of the present invention shown in FIG. 8. In FIG. 8, step 202 of FIG. 2 is further dissected to include steps to detect hard-to-ghost cells. In step 802, a prepared blood sample, i.e., a sample having been ghosted and stained, can be introduced to a flow cell for analysis. In step 804, the sample is interrogated, cell by cell, using measurements including a light beam as explained with respect to FIG. 2 above. In step 806, the ALL measurement is collected, along with one or more light scatter measurements in step 810. Descriptions of the light scatter measurement can be found above with respect to FIG. 2.

**[0033]** In one embodiment, once the hard-to-ghost cells are detected, this event data can be used to more accurately analyze reticulocytes. For example, the hard-to-ghost cell population can be filtered out using the ALL values of the reticulocyte events, as in step 812. In this embodiment, the event data will be available for further analysis for determining reticulocyte information or any other red cell information, as in step 814. In general, the removal of the hard-to-ghost cell event population would increase the accuracy of most parameters reported concerning red blood cells and/or reticulocytes. Calculation and reporting of reticulocyte information is described above with respect to FIG. 2.

#### Enumerating Hard-to-Ghost Cells

**[0034]** One aspect of the present invention is concerned with enumerating the hard-to-ghost cells in the blood sample. It has been unexpectedly discovered by the inventors of the present invention that there exists a correlation between the hard-to-ghost cell population in a blood sample and a blood pathology. Specifically, it has been found that the number of hard-to-ghost cells is increased in analyzed blood samples collected from patients suffering from various diseases, examples of which include, but are not limited to, diseases such as hemoglobinopathies, (e.g., sickle cell anemia and Thalassemia), hematological malignancies (e.g., leukemias and lymphomas), clotting and bleeding disorders, as well as HIV/AIDS, malignant tumors, and autoimmune disorders. In addition, further information can be obtained about these diseases when comparing the position of the hard-to-ghost cells in the scattergram to normal samples. Returning to FIG. 8, following the detection, hard-to-ghost cells can be enumerated, as in step 813. Counting or enumerating of cells is a well-established technique for well-defined cell populations, such as the presently defined hard-to-ghost cells. In one embodiment the hard-to-ghost fraction is reported as the ratio of hard-to-ghost cells to the entire red blood cell population. In another embodiment hard-to-ghost cells can be reported as a percentage or absolute number. Said value can be used as a research use only (RUO) parameter, or can be developed into an *in vitro* diagnostic (IVD) parameter. FIGS. 10 (A-C) illustrate the difference in size of hard-to-ghost

cell populations 1010 in blood samples derived from a healthy individuals (FIG. 10(A)) and from patients suffering from sickle cell anemia (FIG. 10(B)) and Thalassemia (FIG. 10(C)). As illustrated by the FIGS. 10(A) and 11, the % hard-to-ghost cells of a total RBC population is negligible, i.e., less than about 0.01% in blood samples donated by healthy individuals. It has also been determined that blood samples from patients suffering from a number of certain pathologies contain an increased population of hard-to-ghost cells (illustrated in FIG. 12). Such pathologies include renal failure, liver cancer, HIV, sickle cell anemia, and thalassemia. The % hard-to-ghost cells of a total RBC population in a blood sample of a patient with a certain diagnosed disease state is increased at least 10-fold from the hard-to-ghost cell population size of a healthy individual. In some blood samples, the hard-to-ghost cell population of a patient suffering from a disease or disorder is at least 100-fold greater than that of a healthy individual. The discovery of this trend by the inventors of the present invention can be useful in determining existence of abnormal population of hard-to-ghost cells, which may further be related to a presence of certain pathologies.

**[0035]** Alternate methods can be employed to enumerate hard-to-ghost cells. More particularly, one skilled in the art can analyze a blood sample by ghosting the sample and measuring cell by cell hemoglobin of the blood cell sample using light scatter measurement as known to those skilled in the art. Those cells which have at least 30% of the original hemoglobin are considered hard-to-ghost cells. In other words, the hard-to-ghost cells will have greater light scatter than a ghosted cells in the scattergram. In this alternate method, one skilled in the art could also employ a fluorescent dye to differentiate the reticulocytes from the hard-to-ghost cells.

**[0036]** It will be understood by a skilled artisan that the environments in which this invention can be practiced, such as flow cytometers and hematology analyzers, can be programmed to report a numerical value for hard-to-ghost cell population. This numerical value can be correlated to a biochemical and/or a physiological state of an individual. For example, a threshold value can be set for % hard-to-ghost cell of total red blood cells in a blood sample that corresponds to the number of hard-to-ghost cells present in a healthy individual. When a number of hard-to-ghost cells in a blood sample derived from a patient exceeds such threshold value, a disease state can be suspected and the blood sample can be reported, warranting further diagnostic evaluation of the patient. A physician assessing the blood count result will determine the appropriate further testing based on patient's symptoms, general health status, disease or disorder, gender, and age. In one embodiment, a blood sample can be reported for further evaluation if % hard-to-ghost cell in a blood sample exceeds the threshold value by at least 10-fold. In another embodiment, a blood sample can be reported for further evaluation if % hard-to-ghost cell in a blood sample exceeds the threshold value by at least

100-fold.

### System to determine blood cell information

**[0037]** FIG. 9 shows a system to analyze blood samples according to an embodiment of the present invention. A particle analyzer 910 is coupled using link 940 to a computer 901. Computer 901 is optionally coupled using link 950 to a display 920, and/or an external storage device 921. Computer 901 can include a processor 902, a memory 903, an internal storage 904, an input module 905, an output module 906, and a reticulocyte module 907. Reticulocyte module 907 can include a detector module 961, an analyzer module 963, a differentiator module 965, and a reporter module 967.

**[0038]** Particle analyzer 910 can include a hematology analyzer, flow cytometer, or similar device that is capable of interrogating a blood sample with the use of a beam of light. A blood sample is prepared an input to particle analyzer 910 for analysis. The event data generated by particle analyzer 910 is communicated to computer 901, over the link 940. Link 940 can be a device-internal connection such as peripheral component interconnect (PCI) bus, or a network connection. The events generated by the analysis of blood samples in particle analyzer 910 can be communicated to computer 901 in real-time or in batch-mode.

**[0039]** The event data, subsequent to any processing within computer 901, is then presented to a user on display 920, or stored in external storage device 921. For example, scatter plots generated by processing within computer 901 can be presented to the user using display 920. Processed event data can also be stored for later analysis and display. External storage device 921 can include a hard drive, or other type of portable storage.

**[0040]** Processor 902 can execute instructions that enable the processing of modules 905, 906 and 907. Internal memory 903 provides the temporary memory required for such processing, and internal storage 904 can provide for the temporary or intermediate storage of data and results associated with such processing. Internal storage 904 can also store control logic based on instructions and/or program code of modules including the component modules of reticulocyte module 907, in the forms including computer readable program code.

**[0041]** Input module 905 receives the event data generated by particle analyzer 910. Input module 905 can include any processing that is required to transform the input event data from particle analyzer 910, to a format understood by reticulocyte module 907. Output module 906 collects the event data processed by reticulocyte module 907, performs any conversion necessary, and outputs to either display 920 or storage 920, using link 950. Link 950 can be an device-internal connection such as PCI, or a network connection. Display 920 can be a display device that is customized for the viewing of particle analyzer data, a generic display, or any other means capable of outputting results of the particle analysis.

**[0042]** The detector module 961 can include the instructions for determining measurements or parameters of cell events as they pertain to side scatter including UMALS, forward scatter, axial light loss, and DC. Note that every embodiment of the present invention may not have access to all of the measurements above. There may be some configuration required on particle analyzer 910 to enable the collection of all of the above measurements.

**[0043]** Analyzer module 963 includes the instructions for identifying the reticulocyte population and/or a hard-to-ghost cell population, and isolating that population from other types of blood cells. In another embodiment, analyzer module 963 can include instructions to filter-out the cell events corresponding to hard-to-ghost cells, as explained above. In yet another embodiment, analyzer module 963 can include instructions for enumerating the hard-to-ghost cell population.

**[0044]** Differentiator module 965 can include instructions that cause the computer to determine the immature reticulocyte information of the sample being analyzed. For example, the reticulocyte event population identified using module 963, may now be investigated using both, the light scatter measurement as well as a second reticulocyte maturity measurement such as volume, to differentiate the mature from the immature reticulocytes.

**[0045]** Reporter module 967 includes the instruction enabling computer 901 to display scatter plots to display 920, and also to report useful quantifications of the reticulocytes in the blood sample. The reticulocyte fraction or the reticulocyte percentage are some quantifications that can be reported by reporter module 967. Reporter module 967 can also include instructions to report information about hard-to-ghost cell populations.

**[0046]** In this disclosure, methods were disclosed that can improve the accuracy of blood sample analysis through measures such as the reticulocyte fraction and hard-to-ghost cells. The disclosed methods yield substantial improvements over the current methods and can lead to significant improvements in the detection and treatment of a number of blood pathologies. Persons skilled in the art will understand that the techniques disclosed herein can be applicable for cell types other than erythrocytes as described here.

### Claims

1. A method of detecting hard-to-ghost cells, which are defined as cells that retain at least 30% of their original hemoglobin content following mixing with a ghosting reagent, in a blood sample comprising:
  - (a) mixing the blood sample with a ghosting reagent to remove hemoglobin from red blood cells, thereby generating a ghosted blood sample;
  - (b) evaluating the ghosted blood sample in a cy-

- tometric flow cell by a detection comprising an axial light loss measurement and a light scatter measurement, thereby generating event data comprising an axial light loss and a light scatter measurement for each cell; and
- (c) identifying hard-to-ghost cells using the event data comprising an axial light loss measurement and a light scatter measurement for each cell.
2. The method of claim 1, wherein the identification of the hard-to-ghost cells using the axial light loss measurement comprises comparing the axial light loss measurement against a first threshold and a light scatter measurement against a second threshold, wherein the hard-to-ghost cells are identified as having an axial light loss measurement greater than the first threshold and a light scatter measurement lower than the second threshold.
3. The method of claim 1, wherein the light scatter measurement comprises or is selected from upper median angle light scatter (UMALS), lower median angle light scatter (LMALS), and low angle light scatter (LALS).
4. The method of claim 1, further comprising collecting direct current impedance measurements.
5. The method of claim 1 used for enumerating hard-to-ghost cells in a blood sample and further comprising:
- (d) enumerating the hard-to-ghost cell population using the event data comprising an axial light loss measurement and a light scatter measurement for each cell; and
- (e) reporting the hard-to-ghost cell population in the blood sample.
6. The method of claim 5, wherein reporting the hard-to-ghost cell population includes reporting a ratio of the hard-to-ghost cell population to total red blood cells or reporting a % hard-to-ghost cells of total red blood cell population.
7. The method of claim 1 used for detecting an abnormal population of hard-to-ghost cells in a patient sample, comprising:
- (a) mixing a blood sample from the patient with a ghosting reagent to remove hemoglobin from red blood cells, thereby generating a ghosted blood sample;
- (b) evaluating the ghosted blood sample in a cytometric flow cell by a detection comprising an axial light loss measurement and a light scatter measurement, thereby generating event data comprising an axial light loss and a light scatter measurement for each cell;
- (c) identifying hard-to-ghost cells using axial light loss measurement and a light scatter measurement of the event data;
- (d) enumerating the hard-to-ghost cell population using the axial light loss measurement and a light scatter measurement; and
- (e) determining existence of abnormal population of hard-to-ghost cells when the number of hard-to-ghost cells exceeds a threshold value.
8. The method of claim 7, wherein the abnormal population of hard-to-ghost cells is associated with hemoglobinopathy, optionally wherein hemoglobinopathy comprises sickle cell anemia or thalassemia.
9. The method of claim 1 used for analyzing a blood sample, comprising:
- (a) mixing the blood sample with a ghosting reagent to remove hemoglobin from red blood cells, thereby generating a ghosted blood sample;
- (b) measuring the ghosted blood sample in a cytometric flow cell by a detection comprising an axial light loss measurement and a light scatter measurement to generate event data comprising an axial light loss measurement and a light scatter measurement for each cell;
- (c) identifying a hard-to-ghost cell population using the event data, based on said axial light loss measurement and a light scatter measurement;
- (d) filtering-out the hard-to-ghost cell population from said event data; and
- (e) analyzing the event data without the hard-to-ghost cell population to identify blood cell distribution patterns.
10. A computer readable medium storing instructions wherein said instructions when executed cause at least one processor to analyze a blood sample using a method comprising:
- (a) generating event data comprising an axial light loss measurement and a light scatter measurement for each cell based on a detection comprising an axial light loss measurement and a light scatter measurement of a ghosted blood sample in a cytometric flow cell; and
- (b) identifying a hard-to-ghost cell population which are defined as cells that retain at least 30% of their original hemoglobin content following mixing with a ghosting reagent, using the event data, based on said axial light loss measurement and light scatter measurement.
11. The computer readable medium of claim 10, wherein

the method further comprises:

- (c) filtering-out the hard-to-ghost cell population from said event data; and
- (d) analyzing the event data without the hard-to-ghost cell population to identify blood cell distribution patterns; or wherein the method further comprises:

- (c) enumerating the hard-to-ghost cell population using the axial light loss measurement and a light scatter measurement; and
- (d) determining existence of abnormal population of hard-to-ghost cells when the number of hard-to-ghost cells exceeds a threshold value; or wherein the method further comprises:

- (c) enumerating the hard-to-ghost cell population using the axial light loss measurement and light scatter measurement; and
- (d) reporting the hard-to-ghost cell population in the blood sample.

**12.** A system for analyzing a blood sample, comprising:

- at least one processor;
- a particle analyzer coupled to the at least one processor and comprising a cytometric flow cell;
- a detector module coupled to the at least one processor and configured to generate event data comprising an axial light loss measurement and a light scatter measurement for each cell based on a detection comprising an axial light loss measurement and a light scatter measurement of a ghosted blood sample in the flow cell; and
- an analyzer module coupled to the at least one processor and configured to identify a hard-to-ghost cell population which is defined as cells that retain at least 30% of their original hemoglobin content following mixing with a ghosting reagent using the event data, based on said axial light loss measurement and light scatter measurement.

**13.** The system of claim 12, wherein the analyzer module is further configured to enumerate the hard-to-ghost cell population using the axial light loss measurement and a light scatter measurement; or wherein the analyzer module is further configured to:

- filter-out the hard-to-ghost cell population from said event data; and
- analyze the event data without the hard-to-ghost

cell population to identify blood cell distribution patterns.

**14.** An automated method of enumerating hard-to-ghost cells which are defined as cells that retain at least 30% of their original hemoglobin content following mixing with a ghosting reagent, in a blood cell sample comprising:

- (a) mixing a blood cell sample with a nucleic acid stain and a ghosting reagent to remove hemoglobin from red blood cells in the blood cell sample, thereby generating a ghosted blood cell sample;
- (b) passing the ghosted blood cell sample through a cytometric flow cell;
- (c) analyzing the ghosted blood cell sample in the cytometric flow cell by using light scatter and axial light loss measurements thereby generating event data comprising an axial light loss and a light scatter measurement for each cell
- (d) differentiating hard-to-ghost cells in the ghosted blood cell sample from other cells using the analysis by the event data comprising an axial light loss measurement and a light scatter measurement for each cell ; and
- (e) enumerating the hard-to-ghost cells.

**15.** The method of claim 14, wherein mixing of the blood sample with the nucleic acid-staining dye and the ghosting reagent is performed separately; or wherein the stain is fluorescent or non-fluorescent, or further comprising determining an existence of an abnormal population of hard-to-ghost cells by comparing the number of hard-to-ghost cells in the blood cell sample to a threshold value and reporting the number of hard-to-ghost cells that exceeds the threshold value.

**Patentansprüche**

**1.** Verfahren zum Erkennen von Hart- bis Ghost-Zellen, die als Zellen definiert werden, die in einer Blutprobe mindestens 30 % ihres ursprünglichen Hämoglobingehalts erhalten, nachdem sie mit einem Ghost-Reagenz vermischt wurden; umfassend:

- (a) das Vermischen der Blutprobe mit einem Ghost-Reagenz, um Hämoglobin aus roten Blutzellen zu entfernen und so eine Ghost-Blutprobe zu erzeugen;
- (b) die Auswertung der Ghost-Blutprobe in einer zytometrischen Flusszelle durch eine Erkennung, umfassend eine Axiallichtverlustmessung und eine Streulichtmessung, wodurch Ereignisdaten erzeugt werden, die einen Axiallichtverlust und eine Streulichtmessung für jede Zelle

- umfassen; und  
(c) die Identifizierung von Hart- bis Ghost-Zellen mithilfe der Ereignisdaten, die eine Axiallichtverlustmessung und eine Streulichtmessung für jede Zelle verwenden.
2. Das Verfahren nach Anspruch 1, wobei die Identifizierung der Hart- bis Ghost-Zellen mithilfe der Axiallichtverlustmessung den Vergleich der Axiallichtverlustmessung mit einem ersten Grenzwert und einer Streulichtmessung mit einem zweiten Grenzwert umfasst, wobei die Hart- bis Ghost-Zellen identifiziert werden als solche Zellen, bei denen die Axiallichtverlustmessung höher ist als der erste Grenzwert und die Streulichtmessung niedriger als der zweite Grenzwert.
3. Das Verfahren nach Anspruch 1, wobei die Streulichtmessung Folgendes umfasst oder aus den Folgenden ausgewählt ist: oberer Medianstreulichtwinkel (engl.: upper median angle light scatter, UMALS), unterer Medianstreulichtwinkel (engl.: lower median angle light scatter, LMALS) und niedriger Streulichtwinkel (engl. low angle light scatter, LALS).
4. Das Verfahren nach Anspruch 1, weiter umfassend die Erfassung direkter Stromimpedanzmessungen.
5. Das Verfahren nach Anspruch 1, verwendet für die Auszählung der Hartbis Ghost-Zellen in einer Blutprobe, und weiterhin umfassend:
- (d) die Auszählung der Hart- bis Ghost-Zellpopulation mithilfe der Ereignisdaten, die eine Axiallichtverlustmessung und eine Streulichtmessung für jede Zelle umfassen; und  
(e) den Bericht der Hart- bis Ghost-Zellpopulation in der Blutprobe.
6. Das Verfahren nach Anspruch 5, wobei das Erfassen in einem Bericht der Hart- bis Ghost-Zellpopulation den Bericht über ein Verhältnis der Hart- bis Ghost-Zellpopulation zur Gesamtzahl der roten Blutkörperchen oder einen Bericht mit einem Prozentsatz an Hart- bis Ghost-Zellen an der Gesamtzahl der roten Blutkörperchen enthält.
7. Das Verfahren nach Anspruch 1, verwendet für das Erkennen einer anormalen Population von Hart- bis Ghost-Zellen in einer Blutprobe, umfassend:
- (a) das Vermischen einer Blutprobe eines Patienten mit einem Ghost-Reagenz, um Hämoglobin aus roten Blutzellen zu entfernen und so eine Ghost-Blutprobe zu erzeugen;  
(b) die Auswertung der Ghost-Blutprobe in einer zytometrischen Flusszelle durch eine Erkennung, umfassend eine Axiallichtverlustmessung
- und eine Streulichtmessung, wodurch Ereignisdaten erzeugt werden, die einen Axiallichtverlust und eine Streulichtmessung für jede Zelle umfassen;  
(c) die Identifizierung von Hart- bis Ghost-Zellen mithilfe einer Streulichtmessung für die Ereignisdaten;  
(d) die Auszählung der Hart- bis Ghost-Zellpopulation mithilfe der Axiallichtverlustmessung und einer Streulichtmessung; und  
(e) das Bestimmen des Vorliegens einer anormalen Population von Hart- bis Ghost-Zellen, wenn die Anzahl der Hart- bis Ghost-Zellen einen Grenzwert überschreitet.
8. Das Verfahren nach Anspruch 7, wobei die anormale Population der Hart- bis Ghost-Zellen mit einer Hämoglobinopathie verbunden ist, wobei die Hämoglobinopathie optional eine Sichelzellenanämie oder Thalassämie umfasst.
9. Das Verfahren aus Anspruch 1, verwendet für die Analyse einer Blutprobe, umfassend:
- (a) das Vermischen der Blutprobe mit einem Ghost-Reagenz, um Hämoglobin aus roten Blutzellen zu entfernen und so eine Ghost-Blutprobe zu erzeugen;  
(b) das Messen der Ghost-Blutprobe in einer zytometrischen Flusszelle durch eine Erkennung, umfassend eine Axiallichtverlustmessung und eine Streulichtmessung zur Erzeugung von Ereignisdaten, die einen Axiallichtverlust und eine Streulichtmessung für jede Zelle umfassen;  
(c) die Identifizierung einer Hart- bis Ghost-Zellpopulation mithilfe der Ereignisdaten basierend auf der besagten Axiallichtverlustmessung und Streulichtmessung;  
(d) das Herausfiltern der Hart- bis Ghost-Zellpopulation aus den besagten Ereignisdaten; und  
(e) die Analyse der Ereignisdaten ohne die Hart- bis Ghost-Zellpopulation, um Verteilungsmuster für Blutkörperchen zu identifizieren.
10. Computerlesbares Medium zur Speicherung von Anweisungen, wobei die genannten Anweisungen bei ihrer Ausführung mindestens einen Prozessor dazu veranlassen, eine Blutprobe mithilfe eines Verfahrens zu analysieren, das Folgendes umfasst:
- (a) das Erzeugen von Ereignisdaten einschließlich einer Axiallichtverlustmessung und einer Streulichtmessung für jede Zelle auf der Basis einer Feststellung umfassend eine Axiallichtverlustmessung und eine Streulichtmessung einer Ghost-Blutprobe in einer zytometrischen Flusszelle; und  
(b) die Identifizierung einer Hart- bis Ghost-Zell-

population, die als Zellen definiert werden, die mindestens 30 % ihres ursprünglichen Hämoglobingehalts nach dem Mischen mit einem Ghost-Reagenz erhalten, unter Verwendung der Ereignisdaten, die auf besagter Axiallichtverlustmessung und Streulichtmessung beruhen.

11. Das computerlesbare Medium nach Anspruch 10, wobei das Verfahren weiterhin umfasst:

(c) das Herausfiltern der Hart- bis Ghost-Zellpopulation aus den besagten Ereignisdaten; und  
(d) die Analyse der Ereignisdaten ohne die Hart- bis Ghost-Zellpopulation, um Verteilungsmuster für Blutkörperchen zu identifizieren; oder wobei das Verfahren weiterhin Folgendes umfasst:

(c) die Auszählung der Hart- bis Ghost-Zellpopulation mithilfe der Axiallichtverlustmessung und einer Streulichtmessung;  
und

(d) das Bestimmen des Vorliegens einer anormalen Population von Hart- bis Ghost-Zellen, wenn die Anzahl der Hart- bis Ghost-Zellen einen Grenzwert überschreitet, oder wobei das Verfahren weiterhin Folgendes umfasst:

(c) die Auszählung der Hart- bis Ghost-Zellpopulation mithilfe der Axiallichtverlustmessung und der Streulichtmessung;  
und

(d) den Bericht der Hart- bis Ghost-Zellpopulation in der Blutprobe.

12. System zur Analyse einer Blutprobe, umfassend:

mindestens einen Prozessor;  
einen Partikelanalysator, der mit dem mindestens einen Prozessor gekoppelt ist, und eine zytometrische Flusszelle umfasst;

ein Detektormodul, das mit dem mindestens einen Prozessor gekoppelt und dazu konfiguriert ist, Ereignisdaten einschließlich einer Axiallichtverlustmessung und einer Streulichtmessung für jede Zelle auf der Basis einer Feststellung umfassend eine Axiallichtverlustmessung und eine Streulichtmessung einer Ghostblutprobe in einer zytometrischen Flusszelle zu erzeugen; und

ein Analysatormodul, das mit dem mindestens einen Prozessor gekoppelt und dazu konfiguriert ist, eine Hart- bis Ghost-Zellpopulation, die als Zellen definiert werden, die mindestens 30 % ihres ursprünglichen Hämoglobingehalts nach dem Mischen mit einem Ghostreagenz er-

halten, unter Verwendung der Ereignisdaten, die auf besagter Axiallichtverlustmessung und Streulichtmessung beruhen, zu identifizieren.

13. Das System nach Anspruch 12, wobei das Analysatormodul weiter konfiguriert ist, die Hart- bis Ghost-Zellpopulation mithilfe der Axiallichtverlustmessung und einer Streulichtmessung auszuzählen; oder wobei das Analysatormodul weiter konfiguriert ist, um:

die Hart- bis Ghost-Zellpopulation aus den besagten Ereignisdaten herauszufiltern; und die Ereignisdaten ohne die Hart- bis Ghost-Zellpopulation zu analysieren, um Verteilungsmuster für Blutkörperchen zu identifizieren.

14. Automatisiertes Verfahren zum Auszählen von Hart- bis Ghost-Zellen, die als Zellen definiert werden, die in einer Blutzellprobe mindestens 30 % ihres ursprünglichen Hämoglobingehalts erhalten, nachdem sie mit einem Ghost-Reagenz vermischt wurden; umfassend:

(a) das Vermischen einer Blutzellprobe mit einer Nukleinsäurefärbung und einem Ghost-Reagenz, um Hämoglobin aus roten Blutkörperchen in der Blutzellprobe zu entfernen und so eine Ghost-Blutzellprobe zu erzeugen;

(b) das Weiterleiten der Ghost-Blutzellprobe durch eine zytometrische Flusszelle;

(c) die Analyse der Ghost-Blutprobe in einer zytometrischen Flusszelle mithilfe von Axiallichtverlust- und Streulichtmessung, wodurch Ereignisdaten erzeugt werden, die einen Axiallichtverlust und eine Streulichtmessung für jede Zelle umfassen

(d) das Differenzieren der Hart- bis Ghost-Zellpopulation in der Ghost-Blutzellenprobe aus anderen Zellen mithilfe der Analyse durch die Ereignisdaten, die eine Axiallichtverlustmessung und eine Streulichtmessung für jede Zelle umfassen; und

(e) das Auszählen der Hart- bis Ghost-Zellen.

15. Das Verfahren nach Anspruch 14, wobei das Mischen der Blutprobe mit der Nukleinsäure-Färbesubstanz und dem Ghost-Reagenz einzeln durchgeführt wird; oder wobei die Färbung fluoreszierend oder nicht fluoreszierend ist, oder weiterhin umfassend die Bestimmung des Vorliegens einer anormalen Population von Hart- bis Ghost-Zellen durch Vergleich der Anzahl von Hart- bis Ghost-Zellen in der Blutzellprobe mit einem Grenzwert und Berichten der Anzahl der Hart- bis Ghost-Zellen, die den Grenzwert übersteigen.

## Revendications

1. Procédé de détection de cellules difficiles à fantômiser, qui sont définies comme étant des cellules qui conservent au moins 30 % de leur teneur originale en hémoglobine à la suite d'un mélange avec un réactif de fantômisation, dans un échantillon de sang, comprenant :
  - (a) le mélange de l'échantillon de sang avec un réactif de fantômisation pour éliminer l'hémoglobine des globules rouges, en générant de ce fait un échantillon de sang fantômisé ;
  - (b) l'évaluation de l'échantillon de sang fantômisé dans une cellule de flux cytométrique par une détection comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière, en générant de ce fait des données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule ; et
  - (c) l'identification des cellules difficiles à fantômiser en utilisant les données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule.
2. Procédé selon la revendication 1, dans lequel l'identification des cellules difficiles à fantômiser en utilisant la mesure de perte de lumière axiale comprend la comparaison de la mesure de perte de lumière axiale vis-à-vis d'un premier seuil et d'une mesure de dispersion de lumière vis-à-vis d'un deuxième seuil, dans lequel les cellules difficiles à fantômiser sont identifiées comme ayant une mesure de perte de lumière axiale supérieure au premier seuil et une mesure de dispersion de lumière inférieure au deuxième seuil.
3. Procédé selon la revendication 1, dans lequel la mesure de dispersion de lumière comprend ou est choisie parmi une dispersion de lumière à angle médian supérieur (UMALS), une dispersion de lumière à angle médian inférieur (LMALS), et une dispersion de lumière à angle faible (LALS).
4. Procédé selon la revendication 1, comprenant en outre le recueil de mesures d'impédance de courant continu.
5. Procédé selon la revendication 1, utilisé pour le dénombrement de cellules difficiles à fantômiser dans un échantillon de sang et comprenant en outre :
  - (d) le dénombrement de la population de cellules difficiles à fantômiser en utilisant les données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion
- de lumière pour chaque cellule ; et
- (e) l'établissement d'un rapport de la population de cellules difficiles à fantômiser dans l'échantillon de sang.
5. Procédé selon la revendication 5, dans lequel l'établissement d'un rapport de la population de cellules difficiles à fantômiser inclut l'établissement d'un rapport d'une proportion de la population de cellules difficiles à fantômiser par rapport aux globules rouges totaux ou l'établissement d'un rapport d'un pourcentage de cellules difficiles à fantômiser de la population totale de globules rouges.
7. Procédé selon la revendication 1, utilisé pour détecter une population anormale de cellules difficiles à fantômiser dans un échantillon d'un patient, comprenant :
  - (a) le mélange d'un échantillon de sang provenant du patient avec un réactif de fantômisation pour éliminer l'hémoglobine des globules rouges, en générant de ce fait un échantillon de sang fantômisé ;
  - (b) l'évaluation de l'échantillon de sang fantômisé dans une cellule de flux cytométrique par une détection comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière, en générant de ce fait des données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule ;
  - (c) l'identification des cellules difficiles à fantômiser en utilisant une mesure de perte de lumière axiale et une mesure de dispersion de lumière des données d'événement ;
  - (d) le dénombrement de la population de cellules difficiles à fantômiser en utilisant la mesure de perte de lumière axiale et une mesure de dispersion de lumière ; et
  - (e) la détermination de l'existence d'une population anormale de cellules difficiles à fantômiser lorsque le nombre de cellules difficiles à fantômiser dépasse une valeur seuil.
8. Procédé selon la revendication 7, dans lequel la population anormale de cellules difficiles à fantômiser est associée à une hémoglobinopathie, éventuellement dans lequel l'hémoglobinopathie comprend une anémie drépanocytaire ou une thalassémie.
9. Procédé selon la revendication 1, utilisé pour analyser un échantillon de sang, comprenant :
  - (a) le mélange de l'échantillon de sang avec un réactif de fantômisation pour éliminer l'hémoglobine des globules rouges, en générant de ce fait un échantillon de sang fantômisé ;

- (b) la mesure de l'échantillon de sang fantômisé dans une cellule de flux cytométrique par une détection comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour générer des données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule ;
- (c) l'identification d'une population de cellules difficiles à fantômiser en utilisant les données d'événement, sur la base de ladite mesure de perte de lumière axiale et d'une mesure de dispersion de lumière ;
- (d) l'extraction par filtrage de la population de cellules difficiles à fantômiser desdites données d'événement ; et
- (e) l'analyse des données d'événement sans la population de cellules difficiles à fantômiser pour identifier des motifs de distribution de cellules sanguines.
10. Support lisible par un ordinateur stockant des instructions, dans lequel lesdites instructions, lorsqu'elles sont exécutées, amènent au moins un processeur à analyser un échantillon de sang en utilisant un procédé comprenant :
- (a) la génération de données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule sur la base d'une détection comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière d'un échantillon de sang fantômisé dans une cellule de flux cytométrique ; et
- (b) l'identification d'une population de cellules difficiles à fantômiser qui sont définies comme étant des cellules qui conservent au moins 30 % de leur teneur originale en hémoglobine à la suite d'un mélange avec un réactif de fantômisation, en utilisant les données d'événement, sur la base de ladite mesure de perte de lumière axiale et de ladite mesure de dispersion de lumière.
11. Support lisible par ordinateur selon la revendication 10, dans lequel le procédé comprend en outre :
- (c) l'extraction par filtrage de la population de cellules difficiles à fantômiser desdites données d'événement ; et
- (d) l'analyse des données d'événement sans la population de cellules difficiles à fantômiser pour identifier des motifs de distribution de cellules sanguines ; ou dans lequel le procédé comprend en outre :
- (c) le dénombrement de la population de
- cellules difficiles à fantômiser en utilisant la mesure de perte de lumière axiale et une mesure de dispersion de lumière ; et
- (d) la détermination de l'existence d'une population anormale de cellules difficiles à fantômiser lorsque le nombre de cellules difficiles à fantômiser dépasse une valeur seuil ; ou dans lequel le procédé comprend en outre :
- (c) le dénombrement de la population de cellules difficiles à fantômiser en utilisant la mesure de perte de lumière axiale et une mesure de dispersion de lumière ; et
- (d) l'établissement d'un rapport de la population de cellules difficiles à fantômiser dans l'échantillon de sang.
12. Système pour analyser un échantillon de sang, comprenant :
- au moins un processeur ;  
un analyseur de particules couplé à l'au moins un processeur et comprenant une cellule de flux cytométrique ;  
un module détecteur couplé à l'au moins un processeur et conçu pour produire des données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule sur la base d'une détection comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière d'un échantillon de sang fantômisé dans la cellule de flux ; et  
un module analyseur couplé à l'au moins un processeur et conçu pour identifier une population de cellules difficiles à fantômiser qui est définie comme étant des cellules qui conservent au moins 30 % de leur teneur originale en hémoglobine à la suite d'un mélange avec un réactif de fantômisation, en utilisant les données d'événement, sur la base de ladite mesure de perte de lumière axiale et de ladite mesure de dispersion de lumière.
13. Système selon la revendication 12, dans lequel le module analyseur est en outre conçu pour dénombrer la population de cellules difficiles à fantômiser en utilisant la mesure de perte de lumière axiale et une mesure de dispersion de lumière ; ou dans lequel le module analyseur est en outre conçu pour :
- extraire par filtrage la population de cellules difficiles à fantômiser desdites données d'événement ; et

analyser les données d'événement sans la population de cellules difficiles à fantômiser pour identifier des motifs de distribution de cellules sanguines.

5

- 14.** Procédé automatisé de dénombrement de cellules difficiles à fantômiser, qui sont définies comme étant des cellules qui conservent au moins 30 % de leur teneur originale en hémoglobine à la suite d'un mélange avec un réactif de fantômisation, dans un échantillon de sang, comprenant :

10

(a) le mélange d'un échantillon de cellules sanguines avec une teinture d'acide nucléique et un réactif de fantômisation pour éliminer l'hémoglobine des globules rouges dans l'échantillon de cellules sanguines, en générant de ce fait un échantillon de cellules sanguines fantômisées ;

15

(b) le passage de l'échantillon de cellules sanguines fantômisées à travers une cellule de flux cytométrique ;

20

(c) l'analyse de l'échantillon de cellules sanguines fantômisées dans la cellule de flux cytométrique en utilisant des mesures de dispersion de lumière et de perte de lumière axiale, en générant de ce fait des données d'événement comprenant une mesure de perte de lumière axiale et une mesure dispersion de lumière pour chaque cellule

25

(d) la différenciation des cellules difficiles à fantômiser dans l'échantillon de cellules sanguines fantômisées par rapport aux autres cellules en utilisant l'analyse par les données d'événement comprenant une mesure de perte de lumière axiale et une mesure de dispersion de lumière pour chaque cellule ; et

30

35

(e) le dénombrement des cellules difficiles à fantômiser.

- 15.** Procédé selon la revendication 14, dans lequel le mélange de l'échantillon de sang avec le colorant de teinture d'acide nucléique et le réactif de fantômisation est effectué séparément ; ou dans lequel la teinture est fluorescente ou non fluorescente, ou comprenant en outre la détermination de l'existence d'une population anormale de cellules difficiles à fantômiser en comparant le nombre de cellules difficiles à fantômiser dans l'échantillon de cellules sanguines à une valeur seuil et en faisant le rapport du nombre de cellules difficiles à fantômiser qui dépasse la valeur seuil.

40

45

50

55



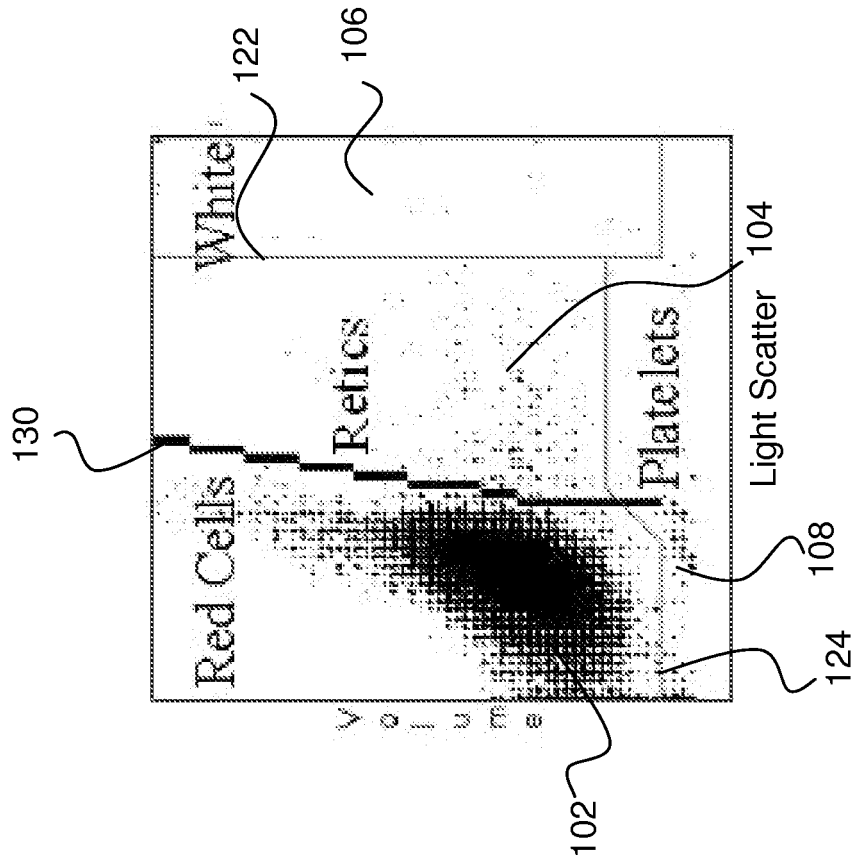



FIG. 1

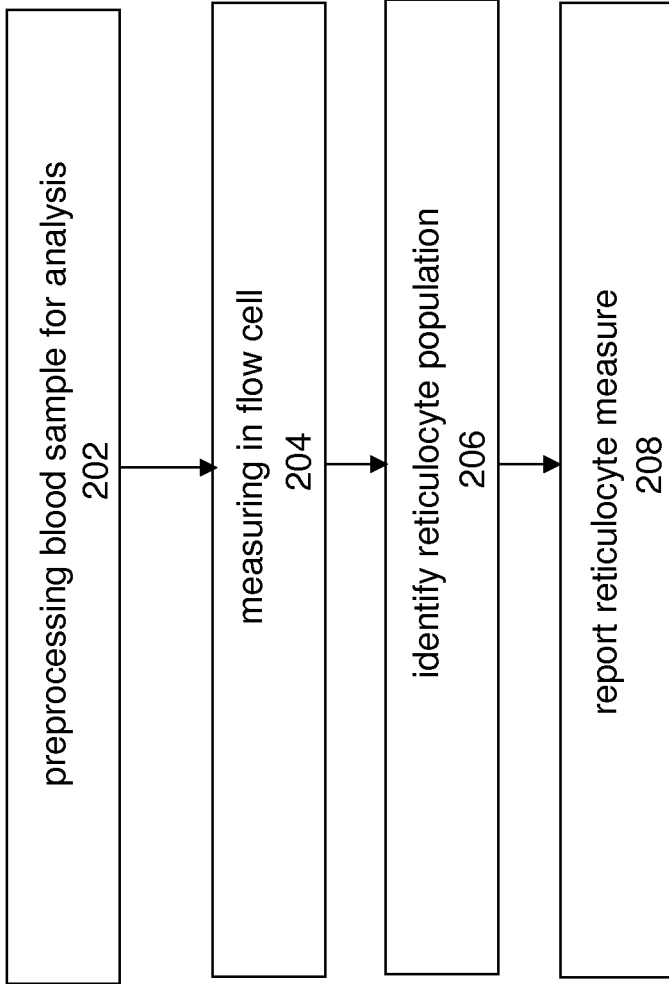

**FIG. 2**

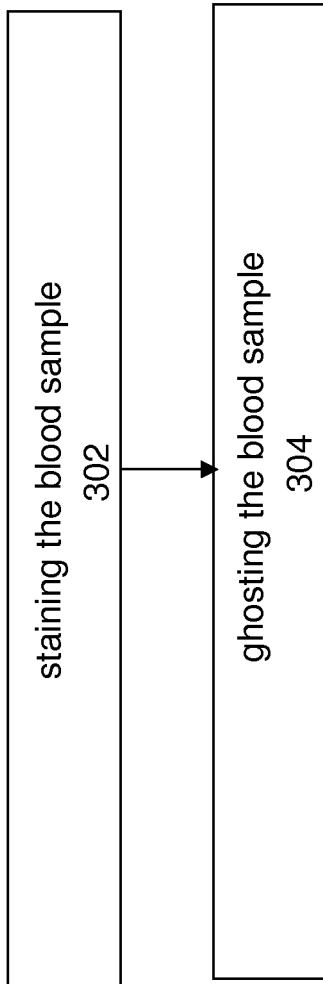

**FIG. 3**

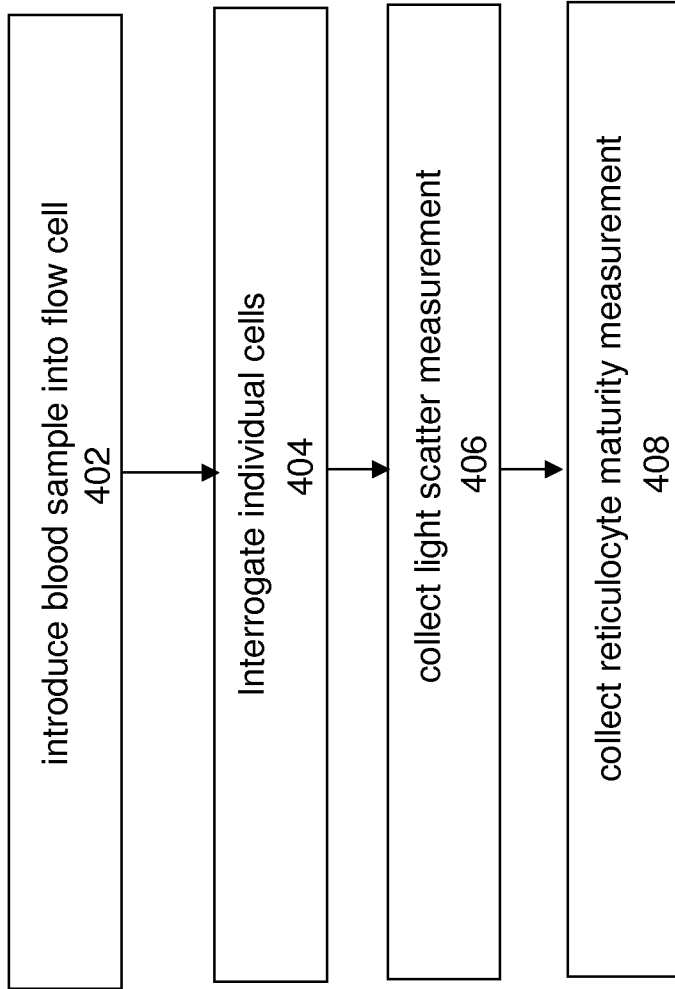

**FIG. 4**

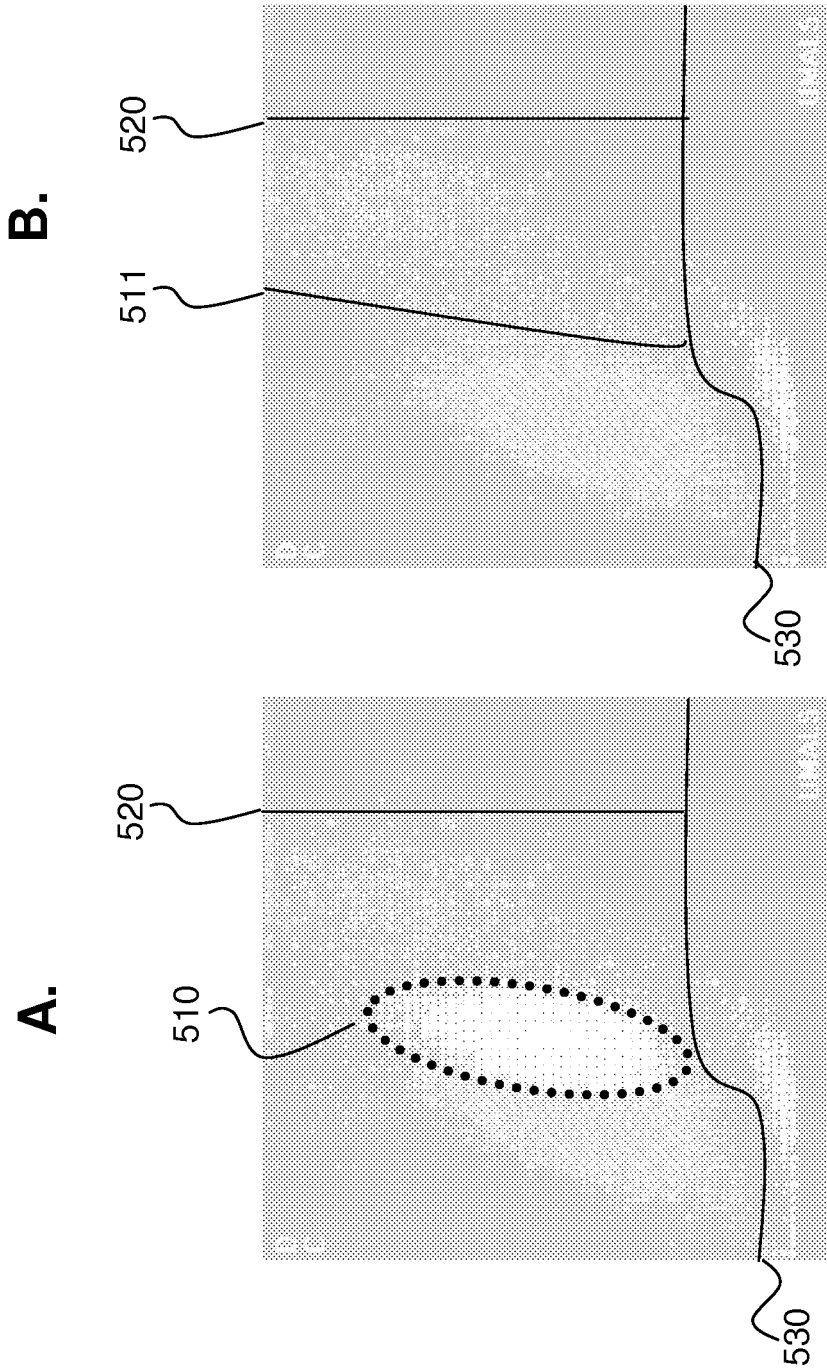


FIG. 5

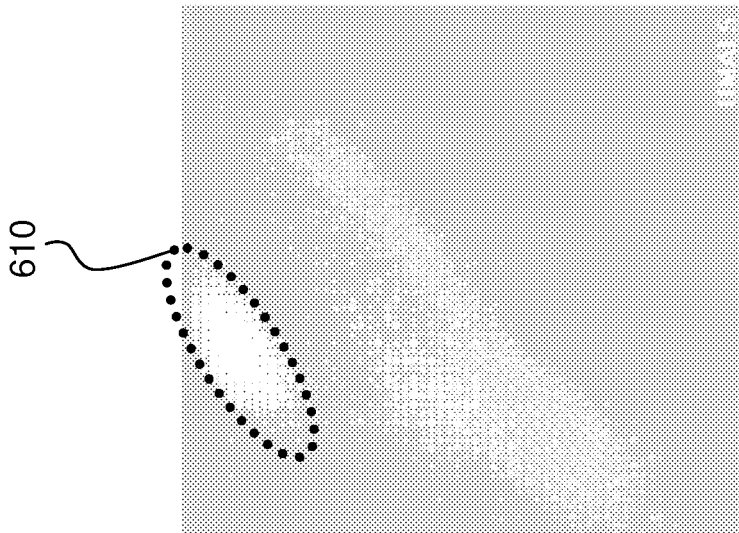


FIG. 6


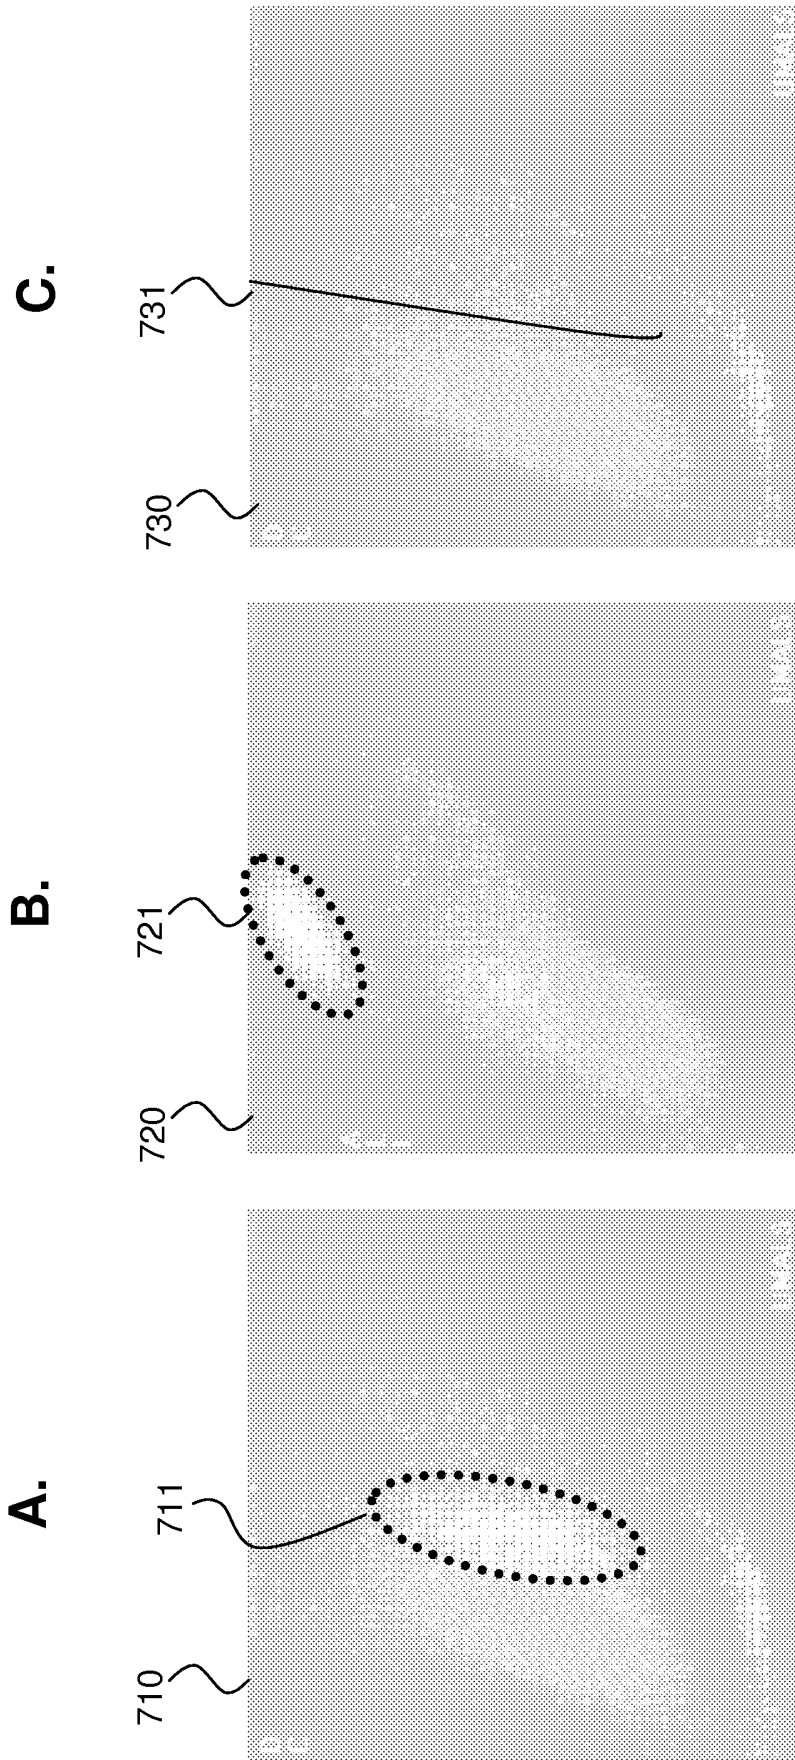


FIG. 7

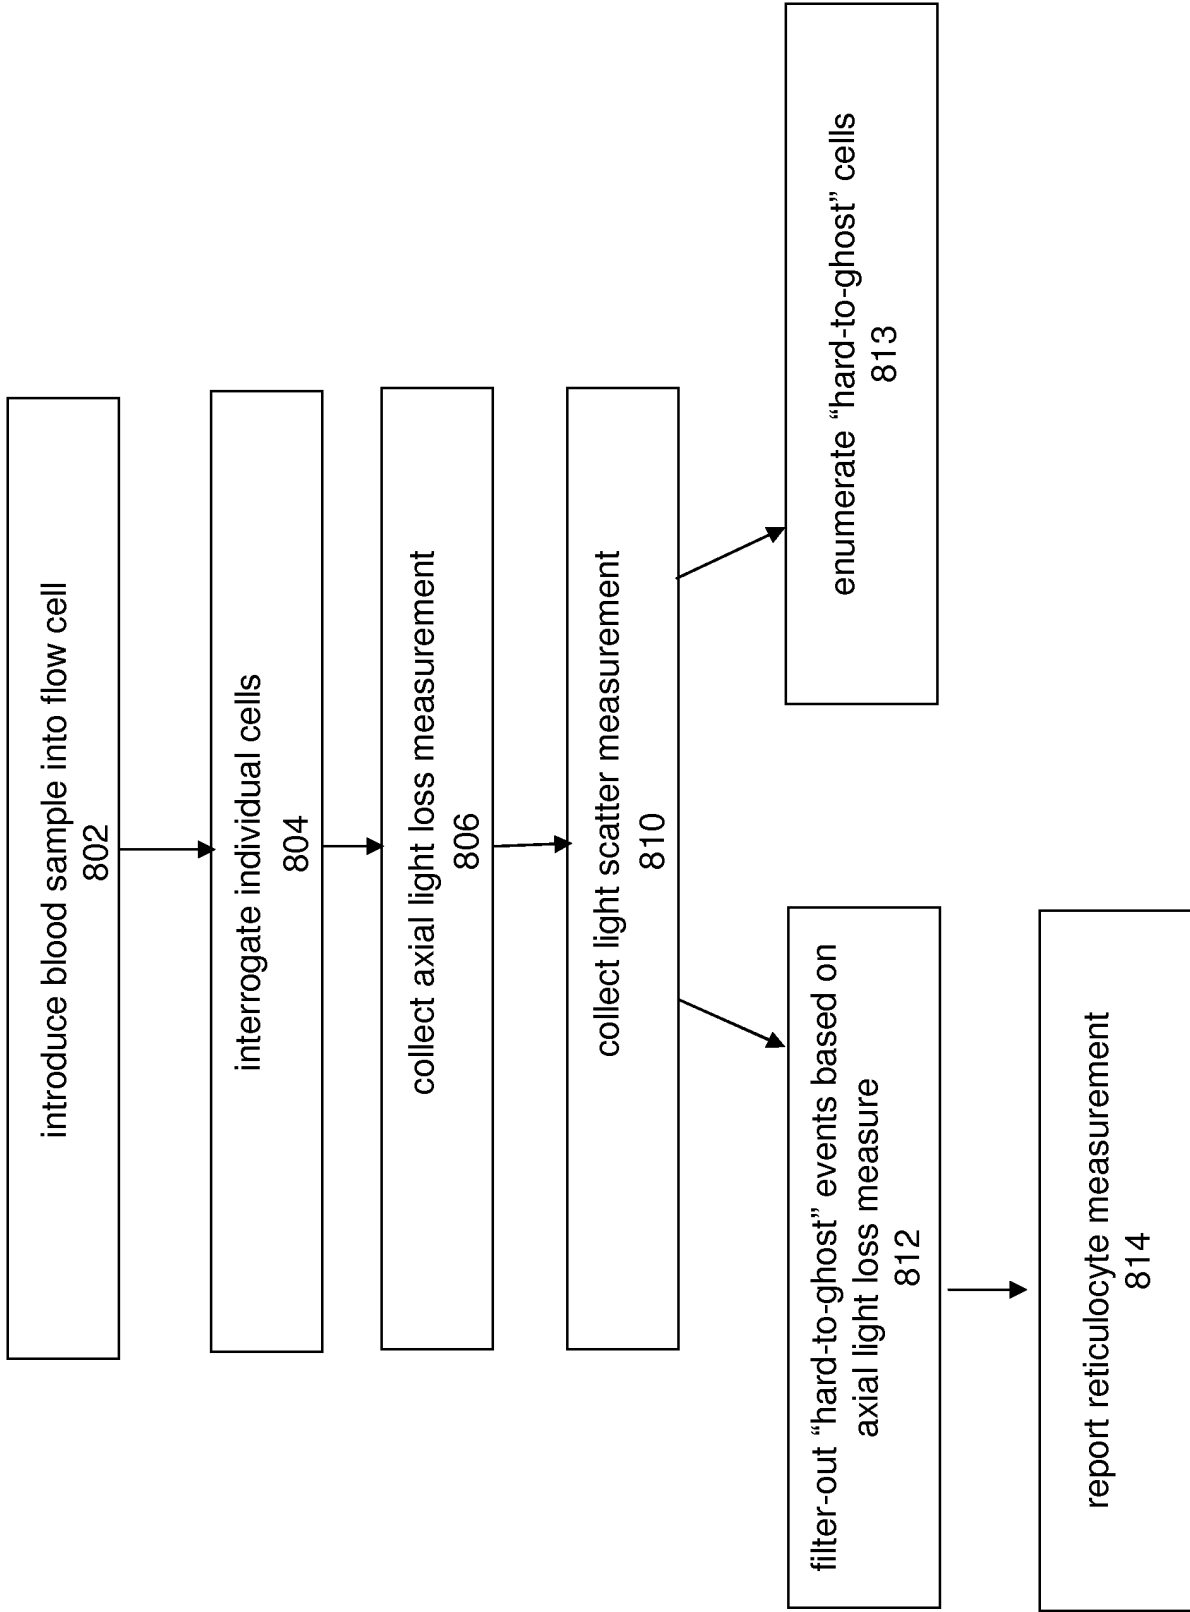

**FIG. 8**

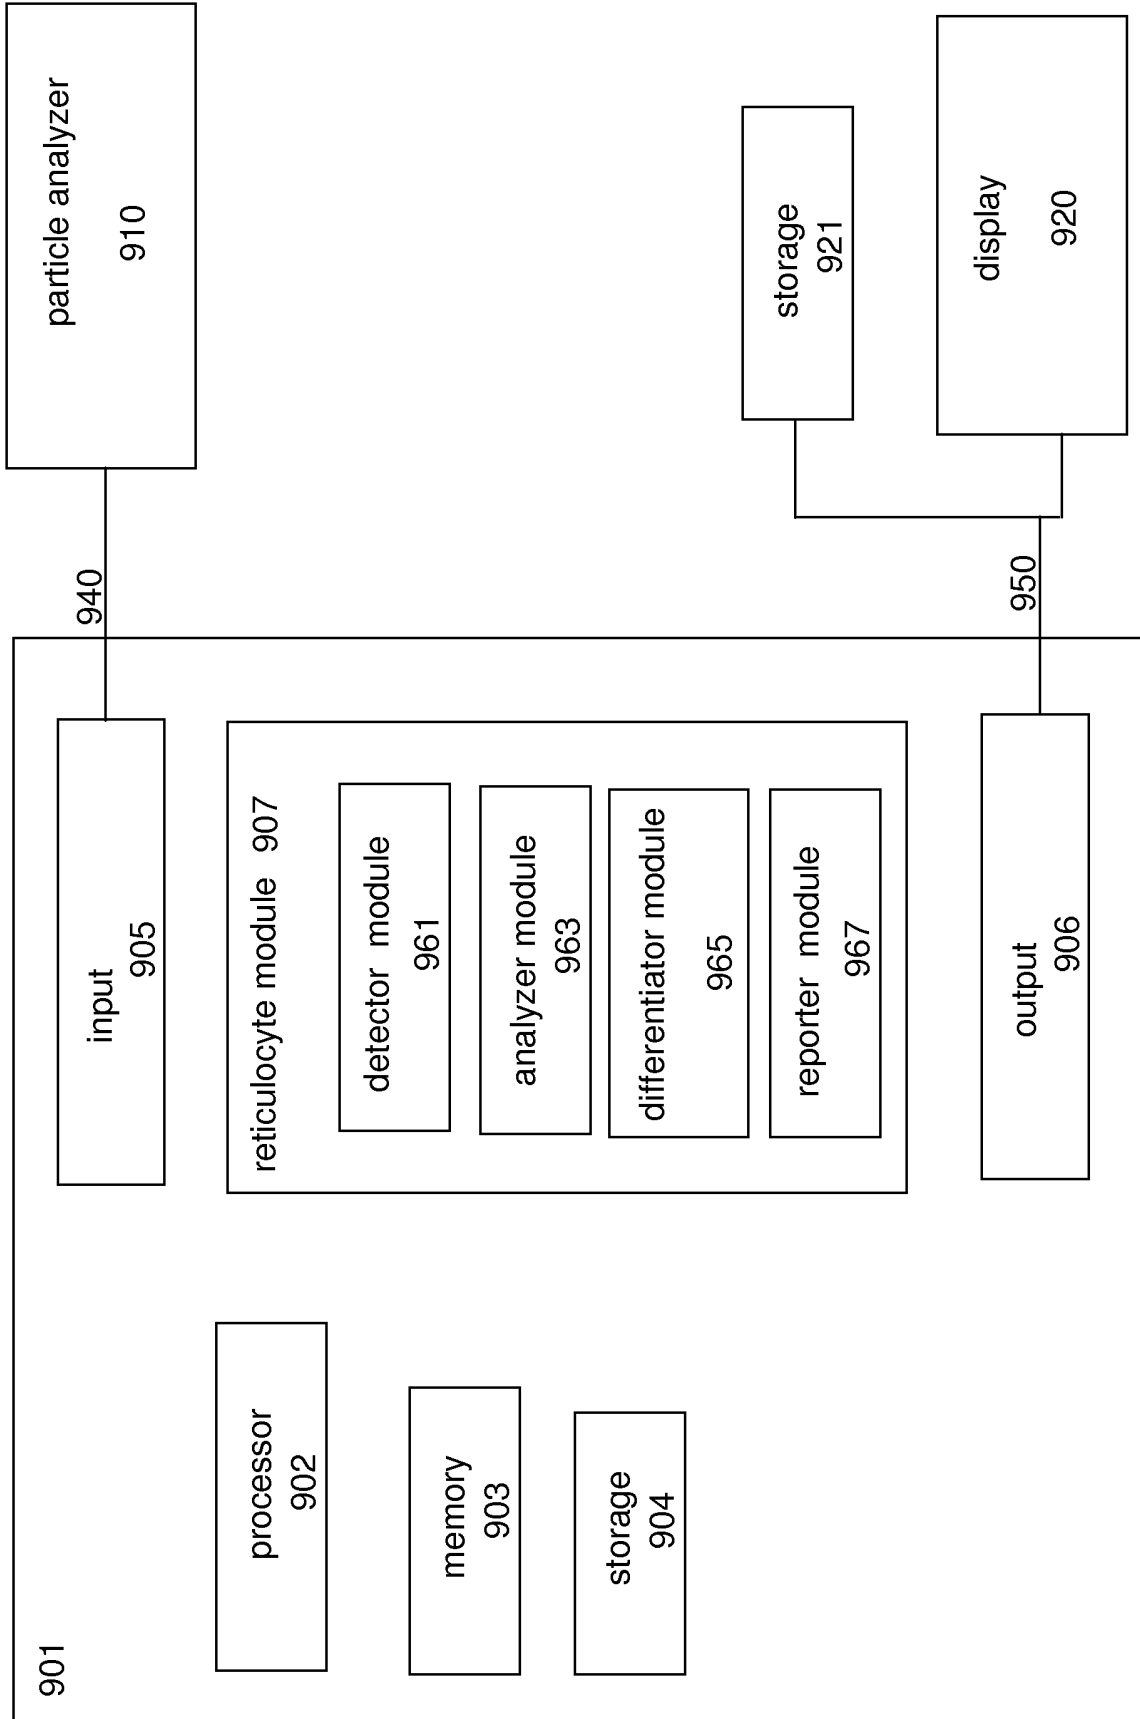


FIG. 9

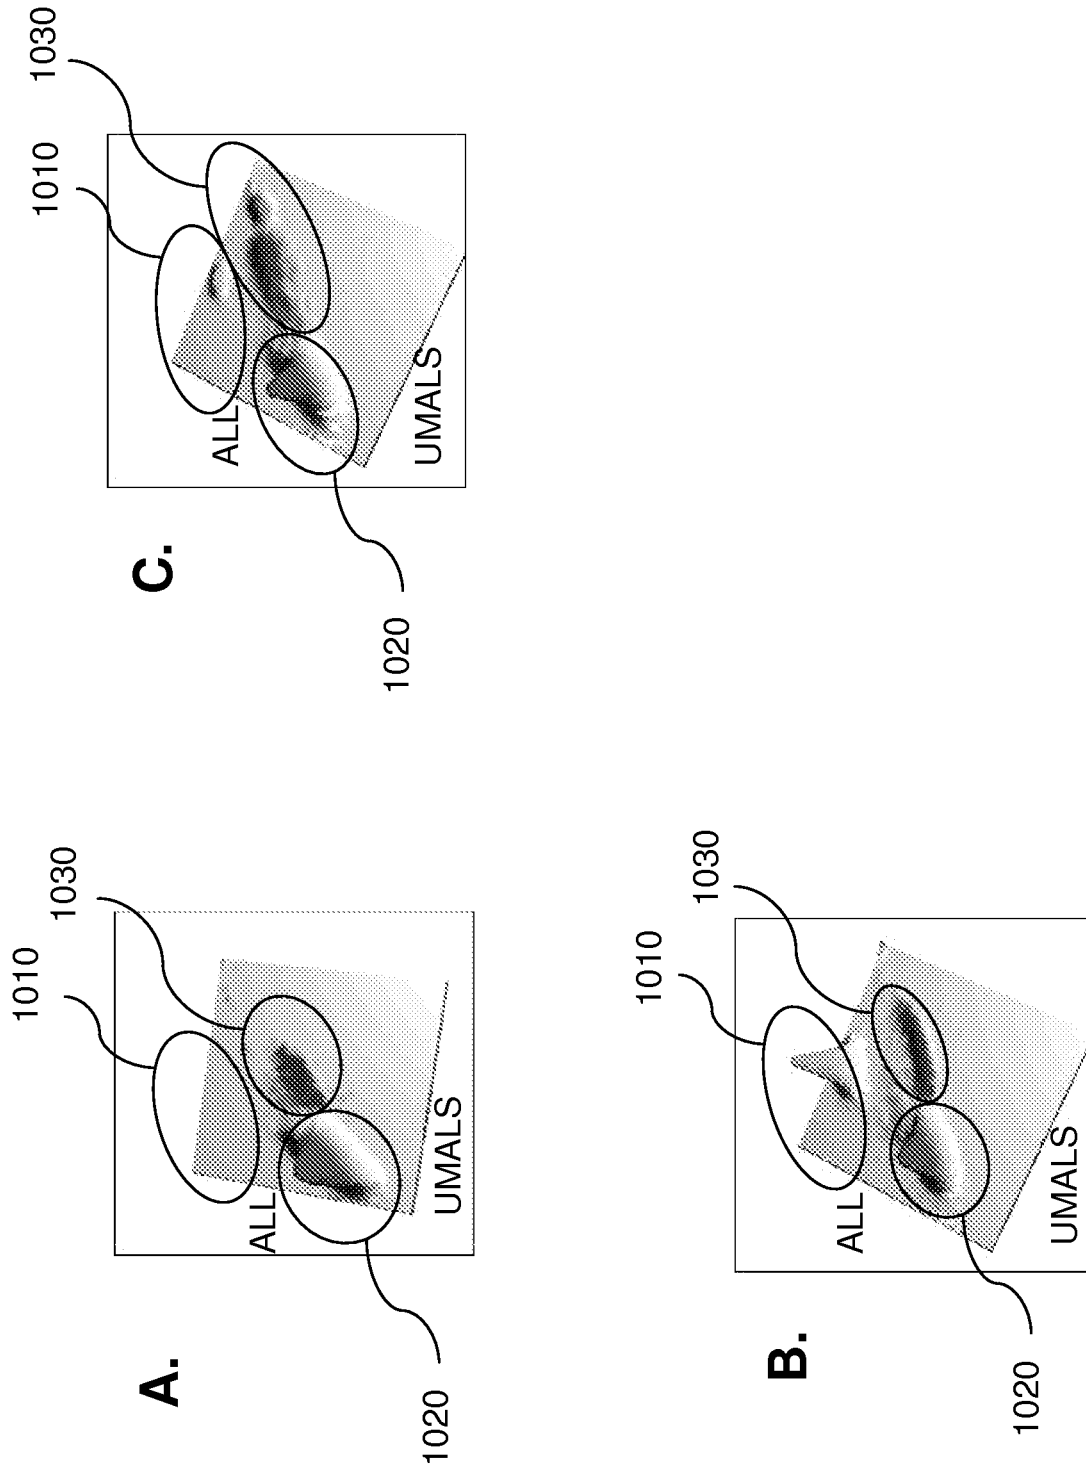


FIG. 10

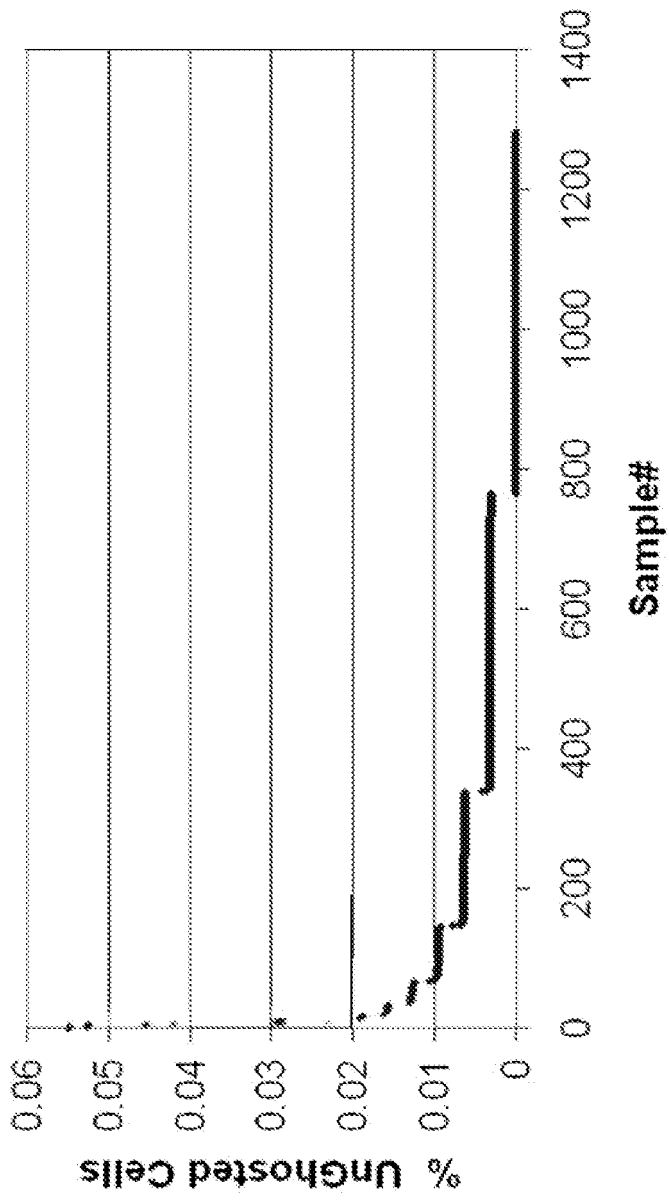


FIG. 11



专利名称(译)	用于分析血液样本的方法和系统		
公开(公告)号	<a href="#">EP2561350B1</a>	公开(公告)日	2017-06-28
申请号	EP2010848598	申请日	2010-03-25
[标]申请(专利权)人(译)	贝克曼考尔特公司		
申请(专利权)人(译)	BECKMAN COULTER , INC.		
当前申请(专利权)人(译)	BECKMAN COULTER , INC.		
[标]发明人	GODEFROY CHRISTOPHE P RILEY JOHN STEVEN VIDAL PATRICIO J		
发明人	GODEFROY, CHRISTOPHE, P. RILEY, JOHN, STEVEN VIDAL, PATRICIO, J.		
IPC分类号	G01N33/48 G01N33/537		
CPC分类号	G01N33/5094 G01N15/1459 G01N33/537 G01N2015/1006 Y10T436/25125		
代理机构(译)	博尔特WADE TENNANT		
优先权	12/730977 2010-03-24 US		
其他公开文献	EP2561350A4 EP2561350A1		
外部链接	<a href="#">Espacenet</a>		

摘要(译)

公开了用于分析血液样品的方法，系统和计算机程序产品。一个实施例是检测和计数血液样本中的难以幽灵细胞的方法。另一个实施方案是分析血液样品中的网状细胞的方法。还提供了使用血液计数参数的方法。

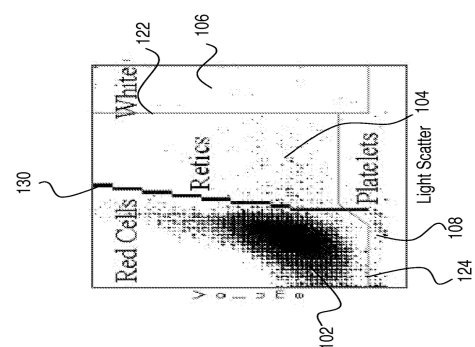


FIG. 1