



(11) **EP 2 857 837 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
25.07.2018 Bulletin 2018/30

(51) Int Cl.:
G01N 33/558 ^(2006.01) **G01N 33/532** ^(2006.01)
G01N 33/543 ^(2006.01)

(21) Application number: **13798097.5**

(86) International application number:
PCT/KR2013/004843

(22) Date of filing: **31.05.2013**

(87) International publication number:
WO 2013/180533 (05.12.2013 Gazette 2013/49)

(54) **FREEZE-DRIED CONJUGATE AND KIT FOR IMMUNOCHROMATOGRAPHIC POINT-OF-CARE TESTING AND A METHOD USING THE KIT**

LYOPHILISATIONSKONJUGAT UND KIT FÜR IMMUNCHROMATOGRAPHISCHE POC-TESTS UND DEREN VERWENDUNG

CONJUGUÉ LYOPHILISÉ DESTINÉ À DES TESTS EFFECTUÉS SUR LES LIEUX DE SOINS PAR IMMUNO-CHROMATOGRAPHIE, NÉCESSAIRE DE DOSAGE IMMUNOLOGIQUE L'UTILISANT, ET PROCÉDÉ D'ANALYSE UTILISANT LE NÉCESSAIRE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **HWANG, Hee Young**
Suwon-si
Gyeonggi-do 443-380 (KR)
- **LEE, Hyo Keun**
Suwon-si
Gyeonggi-do 443-472 (KR)

(30) Priority: **31.05.2012 KR 20120058708**

(43) Date of publication of application:
08.04.2015 Bulletin 2015/15

(74) Representative: **Finnie, Isobel Lara et al**
Haseltine Lake LLP
Lincoln House, 5th Floor
300 High Holborn
London WC1V 7JH (GB)

(73) Proprietor: **SD Biosensor Inc.**
Suwon-si, Gyeonggi-do 443-702 (KR)

(72) Inventors:

- **CHOI, Hyoung Gil**
Seongnam-si
Gyeonggi-do 463-030 (KR)
- **HONG, Sung Yub**
Yongin-si
Gyeonggi-do 446-559 (KR)

(56) References cited:
WO-A1-94/01775 **WO-A2-02/14869**
WO-A2-2006/065118 **WO-A2-2006/083367**
WO-A2-2010/104937 **JP-A- 2010 256 012**
KR-B1- 100 455 298 **KR-B1- 100 506 165**
KR-B1- 100 671 825 **KR-B1- 100 747 412**
US-A- 5 611 973 **US-A1- 2001 039 059**
US-A1- 2008 090 305

EP 2 857 837 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[Technical Field]

5 **[0001]** The present invention relates to a freeze-dried conjugate structure for immunochromatography, an immunoassay kit comprising the freeze-dried conjugate structure and an immunochromatographic strip, and a method for qualitatively or quantitatively analyzing an analyte in a sample using the immunoassay kit.

[Background Art]

10 **[0002]** An immunochromatographic assay, also known as a rapid test method, is a method capable of qualitatively and quantitatively analyzing a trace analyte within a short time using an antigen-antibody reaction and has been used to diagnose or detect various diseases and in various fields, including medical, agricultural, livestock, food, military and environmental fields. This immunochromatographic assay is typically performed using either an assay strip comprising a reaction material, which can change in response to the analyte to be detected, or an assay device comprising the assay strip mounted in a plastic case. FIG. 1 is a cross-sectional view of a conventional assay strip which is used in the immunochromatographic assay. As shown in FIG. 1, the conventional assay strip includes: a sample pad for receiving a liquid sample; a conjugate pad containing a conjugate, obtained by conjugating a label, which generates a signal that can be sensed visually or by a sensor to a ligand such as an antigen or an antibody; a porous membrane pad having immobilized thereon a binding substance (antibody or antigen) that binds specifically to an analyte in the sample and/or the conjugate; and an absorbent pad for finally receiving the liquid sample. These functional pads are connected to each other in the above order while partially overlapping each other, and attached to a solid support so that they are continuously arranged. In the case that the assay strip is used in a form being mounted in the plastic case, a sample introduction port for dropping the sample onto a position corresponding to the sample pad is formed on the case, and an observation window for observing assay results is formed at a position corresponding to the binding agent immobilized on the porous membrane pad. In the immunochromatographic assay that is performed using this assay strip, when a liquid sample is dropped onto the sample pad, it moves through the conjugate pad and the porous membrane pad by a capillary phenomenon, and is finally received in the absorbent pad. Herein, the conjugate in the conjugate pad also moves together with the liquid sample, and if the analyte to be detected is present in the sample, the conjugate will bind to the binding agent on the porous membrane pad through the analyte (generally referred to as a "sandwich reaction"), or the conjugate and the analyte competitively bind to the binding agent (generally referred to as "competition reaction"), and thus the presence of the analyte in the sample can be sensed visually or by a sensor.

25 **[0003]** However, this conventional assay strip has a problem in that the liquid sample that moves by a capillary phenomenon does not uniformly bind to the dry conjugate immobilized on the conjugate pad, and thus there may be a variation between the assay strips, suggesting that the accuracy and reproducibility of the quantitative analysis of the sample can be reduced.

30 **[0004]** In addition, in a method employing liquid reagents, which is frequently used in biochemical assays, the accuracy and reproducibility of sample analysis can be improved by mixing liquid reagents at a specific ratio in well-plate. However, when liquid reagents including an antibody and an antigen are stored for a long period of time, the affinity of antigen-antibody reactions will be reduced, or the antigen and the antibody will be denatured, suggesting that the liquid reagents are problematic in terms of stability. For this reason, liquid reagents can be cold- or freeze-stored in order to improve their long-term stability, but the cold- or freeze-stored liquid reagents are difficult to use in various measurement sites for point-of-care testing such as rapid testing.

35 **[0005]** Accordingly, the present inventors have made extensive efforts to increase the stability of a conjugate and improve the accuracy and reproducibility of sample analysis, and as a result, have developed a freeze-dried conjugate bead and a sample pretreatment device including the same, in which the freeze-dried conjugate bead has high long-term storage stability and is allowed to react uniformly with a sample in the sample pretreatment device to provide a reaction product, which has a size and concentration suitable for quantitative analysis and is subjected into an assay device, thereby completing the present invention.

40 **[0006]** US 2001/039059 A1 discloses that in an immunochromatographic device the detector antibody may be provided in the form of lyophilized beads, placed within the fluid path upstream from the membrane, such that the bead dissolves in the fluid.

45 **[0007]** US 2008/090305 A1 discloses a test device/method for detecting the presence or quantifying the concentration of an analyte in a biological fluid, comprising: a test strip disposed within a housing, and a test well disposed within the housing between the sample port and the test strip.

50 **[0008]** WO 94/01775 A1 discloses a target-specific labeling complex comprising: an enzyme bound to a specific binding substance; and dye molecules complexed to the conjugate in an amount sufficient to impart a visually discernable color to the complex while leaving an active site of the specific binding substance available for binding to a target molecule.

5 [0009] WO 02/14869 A2 discloses an immunoassay device comprising: (a) a chromatographic assay strip, said strip contains a sample receiving zone, a test zone and an absorption zone; (b) a solubilizing assay reagent having a selected labeled antibody to the hydrophobic analyte in the biological solution; (c) a second antibody to the analyte immobilized in the test zone of the chromatographic strip, said second antibody capable of binding to the analyte in the analyte/antibody complex and forming a sandwich, such that detection of the label in the test zone shows the presence and/or concentration of the analyte.

[0010] WO 2006/065118 A2 discloses a gold labelled EBV protein, preferably in powder form, in particular as lyophilised powder and also in combination with an immunochromatographic device.

10 [Disclosure]

[Technical Problem]

15 [0011] It is an object of the present invention to provide a freeze-dried conjugate structure for immunochromatography, comprising a first conjugate comprising a first label for signal detection and a first ligand that reacts with an analyte, wherein the first label and the first ligand are physically or chemically linked to each other, and the conjugate structure is formed by rapidly freezing a dispersion, in which the first conjugate at a predetermined concentration is dispersed in a solvent, in the form of drops having a uniform volume, followed by freeze-drying, thereby removing the solvent, wherein the space occupied by the solvent in the freeze-dried drops forms a porous space by removing the solvent.

20 [0012] This object is provided as defined in claim 1.

[0013] Another object of the present invention is to provide an immunoassay kit comprising the above freeze-dried conjugate structure and an immunochromatographic strip.

[0014] This other object is provided as defined in claim 6.

25 [0015] Still another object of the present invention provides a method for qualitatively or quantitatively analyzing an analyte in a sample using the above immunoassay kit, the method comprising: simultaneously or sequentially adding a buffer and a sample to a conjugate structure and simultaneously or sequentially performing the dissolution of the conjugate structure and a reaction between the conjugate and the sample; loading a material resulting from the preceding step onto an immunochromatographic strip and allowing the loaded material to migrate along the strip; and determining the presence or absence and intensity of a signal generated from a first label on a test line.

30 [0016] This still another object is provided as defined in claim 13.

[Technical Solution]

35 [0017] In order to achieve the above objects, the present invention provides a freeze-dried conjugate structure for immunochromatography, comprising a first conjugate comprising a first label for signal detection and a first ligand that reacts with an analyte, wherein the first label and the first ligand are physically or chemically linked to each other, and the conjugate structure is formed by rapidly freezing a dispersion, in which the first conjugate at a predetermined concentration is dispersed in a solvent, in the form of drops having a uniform volume of 5 - 30 μ l, followed by freeze-drying, thereby removing the solvent, wherein the space occupied by the solvent in the freeze-dried drops forms a porous space by removing the solvent, wherein the conjugate structure has a porosity of 70 - 90%.

40 [0018] As used herein, the term "immunochromatography" refers to an assay method that uses a combination of the immune reaction principle based on an antigen-antibody reaction and the chromatographic principle in which a sample and a reagent are moved along a medium by a mobile phase. Briefly, the antibody or antibody to be analyzed are dispensed and immobilized on a porous membrane in advance, and when blood sample migrates from one end of the membrane to the immobilized antibody or antigen, the reaction with the antigen or antibody in the sample is observed. In a general sense, the term "immune reaction" refers to an antigen-antibody reaction, but in a broader sense in the present invention, it is meant to include not only an antigen-antibody reaction, but also a reaction between a receptor and a ligand binding specifically thereto. Also, not limited thereto, it includes reactions between materials that specifically recognize each other, such as an enzyme-substrate reaction.

45 [0019] A label may be used so that the antigen-antibody reaction can be easily detected visually or using a sensor. In addition, a ligand capable of binding specifically to an analyte may be used in a state linked to the label so that the label can bind to the analyte to be detected. As used herein, the term "conjugate" refers to a conjugate of the label with the ligand. The label and the ligand can be physically or chemically linked to each other. Specifically, the label and the ligand can be linked to each other by passive adsorption, or the label can be modified to have a reactive group and can be covalently linked to the ligand, but is not limited thereto. In addition, linkage between the label and the ligand can be performed using any method known to those skilled in the art.

5 [0020] As used herein, the term "label" refers to a substance that generates a signal that can be sensed visually or using a sensor. Examples of the label that is used in the present invention include, but are not limited to, latex particles, gold particles, colored polystyrene microparticles, enzymes, fluorescent dyes, conductive polymers, or magnetic particles. In addition, the signal can be generated by the intrinsic characteristic (such as luminescence) of the label, or external stimulus such as fluorescence.

10 [0021] As used herein, the term "ligand" refers to a substance that binds specifically to a specific substance. For example, an antibody binding specifically to an antigen, or a ligand binding specifically to a specific receptor acts as a ligand to each other in a broader sense. In addition, any substance may be used as the ligand in the present invention, as long as it shows the above-described characteristics. In the context of the present invention, the term "ligand" refers to a substance that binds specifically to a specific substance as described above, unless it is specified as a ligand that binds specifically to a specific receptor.

15 [0022] The conjugate can be prepared by preparing a solution containing a predetermined concentration of the label and a solution containing a predetermined concentration of the ligand, mixing these solutions together, and allowing the mixed solution to react for a predetermined time. Herein, the concentrations of the solutions and the mixing ratio between the solutions can be determined in view of the binding ratio between the label and the ligand. The binding of the ligand to the label may be the binding of one ligand to one label, the binding of a plurality of ligands to one label, or the binding of a plurality of labels to one ligand. A specific binding ratio is not critical to the present invention, but is preferably maintained at a constant ratio. The binding ratio can change depending on the kinds of label and ligand and can be estimated in view of the relative size thereof and the number of binding sites. For example, when a latex bead having a size of several microns is used as the label and an antibody is used as the ligand, a plurality of antibodies can be bound to one latex bead. Preferably, in order to allow a uniform number of antibodies to bind to the surface of each latex bead, the concentrations and mixing ratio of the antibody and latex solutions can be controlled so that the antibodies are bound to the surface of the latex to saturate, but the scope of the present invention is not limited thereto.

20 [0023] As described above, a solution containing a predetermined concentration of the conjugate can be obtained by mixing solutions containing predetermined concentrations of the label and the ligand, respectively, and allowing the mixed solution to react. The conjugate solution is in the form of a dispersion in which the conjugate molecule is uniformly dispersed in a solution at a predetermined concentration.

25 [0024] The conjugate solution may further contain another conjugate molecule, which comprises a label for signal detection and a ligand that reacts with a reporter molecule immobilized on a control line, so that the conjugate molecule can be used as an internal control. The additional conjugate can be prepared as a uniform dispersion in the same manner as the method for preparing the above-described conjugate and may be mixed with the above-described conjugate solution. The label that is used in the additional conjugate molecule may be the same as or different from that in the above conjugate. The above terms and those for the internal control will be discussed in detail later.

30 [0025] In the present invention, for easy storage and uniform reactivity with a sample, the "freeze-dried conjugate structure" can be prepared by rapidly freezing a dispersion of the conjugate in the form of drops having a uniform volume, and freeze-drying the frozen drops. Specifically, a dispersion of conjugate molecules dispersed uniformly in a solvent at a predetermined concentration can be frozen by spraying drops of the dispersion, which have a uniform volume, so as to come into contact with an extremely-low-temperature liquid refrigerant. Herein, the drops of the dispersion are rapidly frozen to provide solid spheres having a uniform size. The extremely-low-temperature liquid refrigerant that is used in the present invention may be a liquid having an evaporation point between -270 and -180°C. For example, it may be liquid nitrogen, liquid helium, liquid oxygen, liquid hydrogen or the like and may be selected in view of cost and safety. Preferably, it may be liquid nitrogen or liquid helium, but is not limited thereto.

35 [0026] The immunochromatography in the present invention can be used in qualitative or quantitative analysis. In order to use the freeze-dried conjugate structure in quantitative analysis, each of the conjugate structures can be prepared to include a specific number of conjugate molecules. As described above, this preparation can be performed by preparing a uniform dispersion containing the conjugate at a predetermined concentration, and spraying drops of the dispersion, which have a uniform volume, into an extremely-low-temperature liquid refrigerant so as to be rapidly frozen. In order to spray the uniform conjugate dispersion in the form of drops having a uniform volume, a dispenser may be used. When the dispenser is used, the dispersion can be sprayed in the form of drops having a uniform volume, and the variation in the volume of the drops can be minimized. Herein, the volume of the dispersion drops being sprayed can be controlled by controlling the nozzle hole size and dispensing pressure of the dispenser. In addition, the size of the conjugate drops can be controlled depending on the composition and viscosity of the conjugate solution, the dropping rate and amount of the solution, and the surface tension of the drops. The solution drop may be a sphere having a volume of 5-30 μl and a diameter of 0.5-5 mm, but is not limited thereto.

40 [0027] The rapidly frozen conjugate structure can further be freeze-dried to provide a freeze-dried conjugate structure. In the freeze drying process, the solvent is removed from the frozen conjugate structure, and thus the structure becomes porous. The porous freeze-dried conjugate structure prepared as described above can be rapidly dissolved in a buffer so that it can react uniformly with a sample. The freeze drying process can be performed using a freeze dryer, and the

cooling temperature in the freeze dryer may be -20°C or lower. Preferably, the cooling temperature may be -40°C or below, but is not limited thereto. The freeze drying time and temperature can be changed depending on the characteristics of the sample to be dried. The prepared freeze-dried conjugate structure has a porosity of 70-90% and can be completely dissolved in a buffer immediately or within 5 seconds after the start of the dissolution process.

5 [0028] In another aspect, the present invention provides an immunoassay kit comprising the above-described freeze-dried conjugate structure and an immunochromatographic strip.

[0029] As used herein, the term "immunoassay" refers to a method of detecting an analyte using a specific immune reaction such as an antigen-antibody reaction. Herein, immunochromatography can be performed using the chromatographic principle. Immunochromatographic analysis is performed while an analyte-containing sample is moved with a mobile phase through a medium by a capillary phenomenon. Thus, as the medium for immunochromatography, a strip can be prepared and used. The detailed elements and functions of this immunochromatographic strip will be described later.

10 [0030] As described above, immunochromatography is based on the chromatographic principle in which a mobile phase with an analyte moves along a medium. Thus, in order to perform an immunoassay using an immunochromatographic strip, a mobile phase for moving an analyte-containing sample along the strip is required. Thus, the immunoassay kit of the present invention may further include a buffer. The buffer functions not only as a mobile phase for moving a sample along the immunochromatographic strip, but also as a solvent for dissolving the conjugate. If necessary, it may also function as a diluent for diluting a sample. In addition, the immunoassay kit may further include a component for lysing blood cells such as red blood cells in order to analyze whole blood. As the buffer, a conventional buffer, such as 20 10 mM to 1 M phosphate buffered solution (PBS), a nonionic or amphoteric surfactant or a mixture thereof, may be used without limitation. The buffer can be suitably selected depending on the kind of desired reaction such as an antigen-antibody reaction.

[0031] Preferably, when the immunoassay kit of the present invention is used, a sample is allowed to react with a uniform solution of the freeze-dried conjugate structure in a buffer before the sample is injected into an immunochromatographic column in order to ensure a uniform reaction between the conjugate and the sample, and then may be analyzed using the assay strip.

25 [0032] For storage of the freeze-dried conjugate structure, it may be provided together with a chamber comprising a cap, which is provided for its dissolution in a buffer and its reaction with a sample. A buffer and a sample may be added directly to the freeze-dried conjugate structure kept in the chamber comprising the cap, so that the conjugate structure can be dissolved and can react uniformly with the sample. When the chamber is used, the freeze-dried conjugate structure can be stored in a state in which it is covered with the cap, the freeze-dried conjugate structure itself and/or a mixture thereof with a buffer and a sample can be stored without contamination. Preferably, the chamber may be conical in shape so that a reaction mixture solution can be easily loaded onto the strip using a device such as a pipette without being lost, but is not limited thereto.

30 [0033] Because the freeze-dried conjugate structure is one obtained by freezing the dispersion of the conjugate at a predetermined concentration as drops having a uniform volume, followed by freeze-drying the frozen drops, the structure has a constant content of the conjugate molecule, and thus is suitable for use in the quantitative analysis of an analyte.

[0034] In addition, the immunoassay kit may further comprise, as an internal control, a second freeze-dried conjugate structure comprising a second conjugate which comprises a second label for signal detection and a second ligand that reacts with a reporter molecule, in which the second freeze-dried conjugate structure is provided according to the same principle and preparation method as those for the above-described freeze-dried conjugate structure. As described above, the internal control can be provided by adding the second conjugate structure to the conjugate dispersion during the preparation of the freeze-dried conjugate structure to make a single structure. Alternatively, the second freeze-dried conjugate structure may be separately prepared using the same method as described above and may be added to a mixture of a sample and the conjugate. The internal control and the reporter molecule will be described later.

35 [0035] The immunochromatographic strip may comprise a porous membrane pad, which has formed thereon a test line for capturing an analyte in a sample, and an absorbent pad which is provided at one end of the porous membrane pad and serves to provide a driving force for transferring the analyte.

[0036] To detect an analyte in a sample, either a ligand capable of binding specifically to the analyte to selectively capture the analyte, or the same substance as the analyte, or an analogue thereof, which detect the analyte by inducing a competitive reaction with the analyte, is immobilized as a ligand on the porous membrane pad to form a "test line". On the test line of the immunochromatographic strip of the present invention, either a substance capable of binding to an analyte in a sample, or the same substance as the analyte, or an analogue thereof, which can induce a competitive reaction with the analyte, may be immobilized as a third ligand. The type of third ligand can be selected depending on the type of immunoassay used. The type of immunoassay will be described later. Like the ligand included in the conjugate, the second ligand, which reacts with the reporter molecule, and the third ligand that binds to an analyte in a sample, may be, for example, an antigen, an antibody, a receptor or a ligand that binds specifically to the receptor.

40 [0037] As a medium along which a mobile phase and a sample migrate, a porous membrane pad is used so that the

mobile phase and the sample can be moved by a capillary phenomenon. At one end of the porous membrane pad, an absorbent pad that provides a driving force for transferring a sample is located. The absorbent pad may be located so that it partially overlaps the porous membrane pad. The membrane that is used in the present invention may be a nitrocellulose membrane, a glass fiber membrane, a polyethersulfone (PES) membrane, a cellulose membrane, a nylon membrane, or a combination of two or more thereof. Preferably, a nitrocellulose membrane having a pore size of 5-15 μm may be used in the present invention, but is not limited thereto.

[0038] The immunochromatographic strip may further comprise a solid backing plate. The solid backing plate may be made of a plastic material. When the strip is attached onto the solid backing plate, it can have increased durability and can be easily handled and stored. In addition, the solid backing plate makes it easy to mount the strip in an outer case. Examples of a plastic material that may be used for the solid backing plate include, but are not limited to, a polypropylene film, a polyester film, a polycarbonate film, an acrylic film and the like.

[0039] The immunochromatographic strip may be mounted in a case unit. A lower case may comprise a plurality of guides and/or strip support portions, which function to place and fix or press the immunochromatographic strip at a suitable position. An upper case may have guides and strip support portions at positions corresponding to the guides and strip support portions of the lower case. In other words, the guides and/or the strip support portions may be formed only in the lower case or formed in both the upper case and the lower case. The upper case may have a sample introduction port and an observation window for detecting a signal from the label at a position corresponding to the test line. The sample introduction port may be formed in the form of a hole or a slit at one end of the porous membrane, which is opposite to the absorbent pad, enough separated therefrom, with respect to the test line, so that a sample can migrate along the membrane. The observation window may be formed at a location corresponding to the test line of the porous membrane and/or a location including the test line and the control line (if formed) so as to have a size sufficient for observing the test line and/or the control line visually or using a sensor. The size and shape of the observation window are not limited, as long as the test line and/or the control line can be observed through the observation window.

[0040] The upper and lower cases may be made of a conventional plastic material, for example, polycarbonate or acrylonitrile butadiene styrene (ABS), but are not limited thereto. The upper and lower cases can be manufactured separately and coupled to each other through conventional means such as coupling grooves and coupling protrusions. In some cases, the upper and lower cases may be manufactured in an integral form.

[0041] When the immunoassay kit of the present invention is used, an analyte bound to the first conjugate, that is, an analyte bound to the first label through the first ligand, is captured on the test line by the third ligand binding specifically thereto, and the presence or absence, amount, or both, of the analyte in the sample can be determined by measuring a signal generated from the first label on the test line. In other words, the analyte can be qualitatively analyzed based on the presence or absence of a signal generated from the first label on the test line, and can also be quantitatively analyzed by measuring the intensity of a signal generated from the first label on the test line.

[0042] Thus, the immunochromatographic strip may further comprise, before or after the test line, a control line for determining whether the sample migrated. The control line may be formed by immobilizing a reporter molecule before or after the test line on the porous membrane at a suitable distance from the test line.

[0043] As used herein, the term "control line" refers to a portion that generates a constant signal regardless of the type of sample or the concentration of an analyte in a sample. The control line can be formed by a method similar to the method for forming the test line. For example, the control line can be formed by immobilizing a ligand substance that does not bind to the substance to be analyzed and, at the same time, can bind specifically to and capture the ligand of the second conjugate, which is included as an internal control in the mixture of the sample and the conjugate and is moved along the porous membrane together with the sample by a mobile phase, to emitting a constant signal regardless of the concentration and presence or absence of the analyte in the sample. A ligand that may be used for the control line is termed "reporter molecule" herein. Examples of a reporter molecule that is used in the present invention include anti-rabbit IgG, anti-chicken IgY, streptavidin, etc. The sizes and positions of the test line and the control line can be suitably selected depending on the antigen-antibody reaction used and the like. Whether the sample migrated can be determined based on the presence or absence of a signal emitted from the control line, and the quantitative analysis of the analyte can be performed by comparing the intensity of the signal of the test line with the intensity of the signal of the control line.

[0044] Immunoassays can be largely classified, according to principle, into two categories: a sandwich assay and a competitive or inhibition assay. In the case of the sandwich assay, the first ligand of the conjugate first immunologically reacts with an analyte in a sample to form an immune complex. The immune complex is moved along the immunochromatographic strip by a mobile phase and immune-specifically binds to and is captured by the test line having immobilized thereon a third ligand that binds specifically to the analyte. On the other hand, in the case of the competitive or inhibition assay, a third ligand that binds specifically to the first ligand of the conjugate is immobilized on the test line of the porous membrane. The third ligand may be the same substance as an analyte in a sample, or an analogue thereof, but any substance may be used as the third ligand without limitation, as long as it can bind to the first ligand competitively with the analyte. Because the intensity of a signal generated from the label of the conjugate captured by the test line through

an immune reaction is proportional or inversely proportional to the concentration of the analyte in the sample, the presence or absence of the analyte can be qualitatively analyzed based on whether the signal is positive or negative, and the analyte can be quantitatively analyzed by comparing the intensity of the signal with the standard colorimetric system or the internal control.

5 [0045] In still another aspect, the present invention provides a method for qualitatively or quantitatively analyzing an analyte in a sample using the above immunoassay kit, the method comprising: simultaneously or sequentially adding a buffer and a sample to a conjugate structure and simultaneously or sequentially performing the dissolution of the conjugate structure and a reaction between the conjugate and the sample; loading a material resulting from the preceding step onto an immunochromatographic strip and allowing the loaded material to migrate along the strip; and determining the presence or absence and intensity of a signal generated from a first label on a test line.

10 [0046] The principle in which an analyte in a sample is qualitatively and/or quantitatively analyzed using the immunoassay kit of the present invention is as described above.

15 [0047] The immunoassay method of the present invention can be performed in the following manner. First, the conjugate structure is dissolved in a buffer, after which a sample is added to and uniformly mixed with the solution, and the mixture is allowed to react for a predetermined time. Alternatively, a buffer and a sample may be simultaneously added to the conjugate structure so that the conjugate structure is dissolved and, at the same time, can react with an analyte in the sample. Preferably, the conjugate structure is completely dissolved in a buffer to form a uniform dispersion of the conjugate molecules, and a sample is added to the dispersion so as to immunologically react with an analyte in the sample. However, the order in which the conjugate structure, buffer and the sample are mixed or reacted with each other is not limited, as long as the conjugate structure can be completely dissolved so that the conjugate molecules can be dissolved uniformly in the solution and react sufficiently with the sample to form an immune complex. Then, the solution containing the immune complex resulting from the dissolution and immune reaction step are loaded on the immunochromatographic strip and allowed to migrate along the strip, after which the qualitative or quantitative analysis of an analyte in the sample can be performed by determining the presence or absence and intensity of a signal generated from the first label on the test line.

20 [0048] As the solution containing the analyte that migrates along the porous membrane of the strip becomes more uniform, the migration speed of the mobile phase and the antigen-antibody reaction time become more constant, and thus the accuracy of sample analysis can be increased. Thus, the assay method of the present invention, which comprises mixing a sample with a uniform solution of the conjugate in a buffer, allowing the mixture to react sufficiently, loading the reaction mixture on the immunochromatographic strip and allowing the loaded mixture to migrate along the strip, is suitable for increasing the accuracy of analysis.

25 [0049] In an Example of the present invention, the assay method of the present invention and a conventional assay method employing an immunoassay strip further comprising a conjugate pad having a conjugate adsorbed thereon were performed, and the results of the assay methods were compared with each other. As a result, it was shown that more highly reproducible results could be obtained in the analysis of glycated hemoglobin using the method of the present invention (Table 1). Further, it was shown that the glycated hemoglobin concentration and the measured intensity of a signal in quantitative analysis were highly linearly correlated with each other (FIG. 6).

30 [0050] Examples of the sample that is used in the immunoassay of the present invention include all biological samples, including whole blood, blood cells, serum, plasma, bone marrow, sweat, urine, tears, saliva, skin, mucosa and hair, which are isolated from mammals, preferably humans. For example, the sample may be blood. The blood sample may be blood cell-free serum or plasma. When whole blood is used, a buffer containing a component capable of lysing blood cells may be used.

35 [0051] The immunoassay method of the present invention is useful for the analysis of blood glucose levels and the diagnosis of diseases using whole blood as a sample. Examples of the diseases include malaria antigen (Ag), AIDS, hepatitis C, hepatitis B, syphilis, gastric ulcer-causing microorganisms, cancer markers (AFP, PSA, CEA), tuberculosis, SAS, dengue fever, and leprosy. Preferably, the analyte may be glycated hemoglobin, but is not limited thereto.

40 [0052] According to a specific embodiment of the present invention, the concentration of glycated hemoglobin in blood can be measured by using blood as a sample, immobilizing anti-glycated hemoglobin antibody as the second ligand on the test line, and measuring the intensity of a signal generated from the label of the conjugate captured by the test line. For example, the measurement can be performed using a spectrophotometer as a sensor, but the detection method is not limited thereto. The concentration of glycated hemoglobin is generally expressed as the percentage of the glycated hemoglobin concentration relative to the total hemoglobin concentration. The percentage of the glycated hemoglobin concentration (HbA1c) relative to the total hemoglobin concentration (TotalHb) can be calculated using the following equation. When the percentage of the glycated hemoglobin concentration is 3-6.5%, the sample is judged to be normal, and when the percentage is 6.5-20%, the sample is diagnosed as diabetes.

$$HbA1c(\%) = \frac{HbA1c(g/dL)}{TotalHb(g/dL)} \times 100$$

5

[0053] In order to measure the concentrations of hemoglobin and glycated hemoglobin in human red blood cells, a step of lysing red blood cells is required. Like the conventional analysis of glycated hemoglobin, the assay method of the present invention may comprise a pretreatment step of lysing red blood cells. The lysis of red blood cells can be performed simultaneously with the conjugate-sample reaction by adding a blood cell lysis buffer to a liquid buffer that is used in the sample pretreatment step. Thus, the kit of the present invention is highly useful as a point-of-care testing kit.

10

[0054] Hereinafter, the present invention will be described in detail with reference to the accompanying drawings.

[0055] FIG. 3 is an exploded perspective view of an immunoassay device according to an embodiment of the present invention; FIG. 4 is a photograph of a freeze-dried conjugate according to the present invention; and FIG. 5 sequentially shows the steps of an immunoassay method according to the present invention. As shown in FIGS. 3 and 5, the immunoassay device according to the present invention comprises: at least one membrane strip comprising a porous membrane having formed thereon a test line which has immobilized thereon a binding agent (antigen, antibody or ligand) that binds to a detectable analyte in a sample and/or a conjugate by an immune specific reaction, that is, an antigen-antibody reaction, in order to qualitatively or quantitatively analyze the analyte by an immunochromatographic assay; an upper case covering the upper part of the membrane strip and having a sample introduction port and an observation window; a lower case covering the lower part of the membrane strip and having a sample reservoir; and a sample pretreatment device (FIG. 5) which contains a freeze-dried conjugate comprising the conjugate and serves to mix the sample, a liquid buffer and the conjugate with each other and introduce the mixture into the sample reservoir. Alternatively, the immunoassay device may consist only of the membrane strip and the sample pretreatment device.

15

20

25

[Advantageous Effects]

[0056] Because a sample is subjected to immunochromatography after reacting uniformly with a freeze-dried conjugate structure separately prepared according to the present invention externally, quantitative analysis can be performed with high reproducibility and linearity depending on a concentration compared to a conventional assay method which is performed using an immunochromatographic strip comprising a conjugate pad prepared by adsorbing a conjugate.

30

[0057] In addition, the freeze-dried conjugate structure of the present invention can be provided in a state in which it is received in a chamber additionally comprising a cap. Thus, it can be stored without contamination and is easy to carry. In addition, the freeze-dried conjugate structure can be rapidly and uniformly dissolved so that it is immediately allowed to react with a mixture of a buffer and a sample and the reaction product can be analyzed by an immunoassay kit. Thus, it is suitable for use in point-of-care testing.

35

[Description of Drawings]

[0058]

40

FIG. 1 is a cross-sectional view of an assay strip which is used in a conventional immunochromatographic assay. FIG. 2 is an exploded perspective view of a conventional immunoassay device.

FIG. 3 is an exploded perspective view of an immunoassay device according to an embodiment of the present invention.

45

FIG. 4 shows the shape of a freeze-dried conjugate bead according to an embodiment of the present invention.

FIG. 5 shows a perspective view of a sample pretreatment device and an immunoassay method according to an embodiment of the present invention. Specifically, FIG. 5(A) shows a sample pretreatment device, which is a chamber equipped with a cap and containing a freeze-dried conjugate bead. FIG. 5(B) shows an immunoassay method employing the sample pretreatment device.

50

FIG. 6 shows a comparison of the results of quantitative analysis of glycated hemoglobin, performed using immunoassay devices according to the Example of the present invention and the Comparative Example. The diamonds indicate the measurement values obtained by the immunoassay device according to the Example of the present invention, and the squares indicate the measurement values obtained by a conventional immunoassay device according to the Comparative Example.

55

Fig. 7 shows changes of measured values for glycated hemoglobin depending on a volume of a freeze-dried conjugate bead according to an embodiment of the present invention.

[Mode for Invention]

[0059] Hereinafter, the present invention will be described in further detail with reference to examples. It is to be understood, however, that these examples are for illustrative purposes only and are not intended to limit the scope of the present invention.

Example 1: Analysis of glycated hemoglobin using freeze-dried conjugate bead

A. Preparation of antibody-immobilized nitrocellulose pad

[0060] A monoclonal antibody to glycated hemoglobin was diluted in 0.1 M phosphate buffered solution (PBS) at a concentration of 1 mg/ml, and then sprayed onto the test line position of a nitrocellulose pad (width: 25 mm; pore size: 10-12 μm) using a dispenser. Meanwhile, anti-rabbit immunoglobulin G antibody obtained by inoculating rabbit immunoglobulin G into a mouse was diluted in 0.1 M PBS at a concentration of 1 mg/ml, sprayed onto the control line position of the nitrocellulose pad and dried in an incubator at 37°C so as to be immobilized. On the portion excluding the antibody-immobilized portion of the nitrocellulose pad, a PBS containing 0.05 wt% bovine serum albumin, 4 wt% sucrose and 0.0625 wt% ionic surfactant was sprayed to block and dried in an incubator at 30°C for 60-120 minutes. The resulting nitrocellulose pad was attached to a polypropylene backing plate having an adhesive applied thereon, and then an absorbent pad (Millipore, USA) was attached onto the nitrocellulose pad so that it overlapped by 1 mm.

B. Preparation of freeze-dried conjugate beads comprising antibody-latex conjugate

[0061] A conjugate solution was prepared in the following manner. First, each of anti-glycated hemoglobin monoclonal antibody and rabbit immunoglobulin G was added at various concentrations to 1 ml of an aqueous solution of latex in 0.1 M MES (2-(N-morpholino)ethanesulfonic acid) buffer (pH 6.0), and then allowed to react in an incubator at 37°C for 1 hour. Each of the resulting conjugate solutions was centrifuged once at 12,000 rpm, and the supernatant was removed, thus removing unreacted antibody. To the remaining material, a buffer containing 1wt% bovine serum albumin was added and allowed to react for 24 hours, so that the unreacted latex surface was blocked with the bovine serum albumin. The buffer used was 0.1 M PBS containing, in addition to 1 wt% bovine serum albumin, 0.5 wt% sucrose, 1 wt% PEG (polyethylene glycol), 1 wt% PVA (polyvinyl alcohol) and the like.

[0062] The resulting conjugate-containing solution was added dropwise to liquid nitrogen using a dispenser in the form of a drop having a volume of 20 μl so that it was rapidly frozen. This rapid freezing process was repeated to obtain conjugate beads which were then freeze-dried in a freeze dryer for 20 hours.

C. Manufacture of immunoassay device

[0063] The strip prepared in step A was mounted in a lower case, and then covered with an upper cover, thereby manufacturing an immunoassay strip device (FIG. 3) according to an embodiment of the present invention. Each of the freeze-dried conjugate beads (FIG. 4) prepared in step B was placed in a pretreatment device (FIG. 5) which was then covered with a cap. The manufactured immunoassay strip device and the pretreatment device were dehumidified, sealed, packaged in single pouches and stored.

Comparative Example 1: Preparation of conventional assay strip comprising conjugate pad

A. Preparation of antibody-immobilized nitrocellulose pad

[0064] An antibody-immobilized nitrocellulose pad was prepared in the same manner as described in step A of Example 1.

B. Preparation of antibody-latex conjugate pad

[0065] An antibody-latex conjugate solution was prepared in the same manner as described in step B of Example 1. The prepared conjugate solution was applied to the glass fiber pad shown in FIG. 1 at a density of 10 $\mu\text{l}/25\text{ mm}^2$ using a dispenser. The pad having the antibody-latex conjugate applied thereto was frozen rapidly with liquid nitrogen, and then dried in a freeze dryer for 20 hours, and the dried pad was cut to a size of 7 mm \times 30 mm.

[0066] The resulting conjugate pad was attached to a polypropylene backing plate having an adhesive applied thereon so that 1 mm of the conjugate pad overlapped the lower side of the nitrocellulose pad attached to the backing plate.

C. Manufacture of immunoassay device

[0067] Pads, including the nitrocellulose pad and conjugate pad prepared in steps A and B of Comparative Example 1, were arranged as shown in FIG. 1 so that they overlapped each other. The arrangement was mounted in a lower case and covered with an upper case, thereby manufacturing an immunoassay strip device (FIG. 2) according to the Comparative Example. The manufactured immunoassay strip device was dehumidified, sealed, packaged in a single pouch and stored.

Test Example 1: Comparison of measurement performance for glycated hemoglobin between assay strips employing conjugate pad and freeze-dried conjugate bead, respectively

[0068] In order to compare performance between the assay strips prepared in Example 1 and Comparative Example 1, the level of glycated hemoglobin in 10 blood samples was measured 10 times for each sample using each assay strip. Also, the level of glycated hemoglobin in each of the 10 blood samples used in the above measurement was measured using an automated testing system (Variant II Turbo; Bio-Rad Laboratories, Hercules, CA, USA) and compared with the measurement results obtained using the assay strips prepared in Examples 1 and Comparative Example 1. The measurement results obtained using the prepared assay strips were expressed as numerical values using a spectrophotometer capable of measuring the intensity of light in the specific regions of the membrane, including the test line and the control line. From the numerical values measured in the test line and the control line by the spectrophotometer, the glycated hemoglobin level (HbA1c %) was calculated. The results of the calculation are shown in Table 1 below.

Table 1: Comparison of performance for measurement of glycated hemoglobin

Sample No.	Automated testing system	Example		Comparative Example	
	Average of measurements	Average of measurements	CV%	Average of measurements	CV%
Sample 1	5.6%	5.4%	2.3	5.2%	9.7
Sample 2	6.5%	6.6%	3.1	5.6%	9.5
Sample 3	7.4%	7.2%	3.4	6.5%	7.6
Sample 4	7.9%	8.0%	2.5	8.3%	5.0
Sample 5	8.7%	8.8%	3.8	8.5%	5.5
Sample 6	9.5%	9.3%	2.6	9.7%	3.0
Sample 7	5.4%	5.4%	2.9	5.8%	4.8
Sample 8	6.1%	6.1%	2.6	6.7%	2.4
Sample 9	7.2%	7.1%	3.2	7.6%	5.1
Sample 10	7.9%	8.1%	3.2	7.6%	5.9

[0069] As can be seen in Table 1 above, the measurement values obtained using the assay strip prepared in Example 1 had high reproducibility (low coefficient of variation; CV%) compared to the measurement values obtained using the assay strip prepared in Comparative Example 1. In addition, when the measurement values were compared with the measurement values obtained by the automated testing system, it could be seen that the measurement values obtained using the assay strip of Example 1 had a low variation compared to the measurement values obtained using the assay strip of Comparative Example 1. In other words, it was shown that the use of the method for measuring glycated hemoglobin using the assay strip of the present invention showed high accuracy and reproducibility compared to the use of the conventional method.

Test Example 2: Comparison of the ability to quantitatively analyzing glycated hemoglobin between immunoassay devices employing conjugate pad and freeze-dried conjugate bead, respectively

[0070] In order to compare the ability to quantitative analysis between the immunoassay devices manufactured in Example 1 and Comparative Example 1, 12 blood samples containing various concentrations of glycated hemoglobin were analyzed. In addition, the level of glycated hemoglobin in each of the 12 samples used in the above analysis was measured using an automated testing system (Variant II; Bio-Rad Laboratories, Inc) as described in Test Example 1, and its relationship with the glycated hemoglobin concentration was analyzed. The results of the analysis are shown in

FIG. 6. In FIG. 6, the diamonds indicate the signal values (intensities) measured by the immunoassay device manufactured in Example 1 of the present invention, and the squares indicate the signal values (intensities) measured by the immunoassay device manufactured in Comparative Example 1. As can be seen in FIG. 6, the measurement values obtained by the immunoassay device of the present invention were proportional to the concentration of glycosylated hemoglobin and had high linearity over a wide concentration range including a range in which diabetes can be diagnosed ($R^2=0.996$). On the other hand, the measurement values obtained by the immunoassay device of Comparative Example 1, similar to a conventional immunoassay device, showed a tendency to be generally proportional to the concentration of glycosylated hemoglobin, but had low linearity ($R^2=0.919$), and particularly showed an unreliable low linearity for the samples containing glycosylated hemoglobin at a concentration of 5-8%, which includes 6.5%, a standard for diagnosing diabetes ($R^2=0.747$; data not shown). The glycosylated hemoglobin concentrations and measurement values for the samples used in the concentration dependence test are summarized in Table 2 below.

Table 2: Comparison of the ability to quantitatively analyze glycosylated hemoglobin

Sample No.	HbA1c	A (◆)	B (■)
Sample 1	5.1%	0.85709	0.74213
Sample 2	5.4%	0.87160	0.77635
Sample 3	6.6%	0.93709	0.78221
Sample 4	6.7%	0.93586	0.79454
Sample 5	7.1%	0.96748	0.80414
Sample 6	8.0%	1.01602	0.93555
Sample 7	9.5%	1.09534	0.99538
Sample 8	11.1%	1.18901	1.02154
Sample 9	11.0%	1.18645	1.00212
Sample 10	5.6%	0.89845	0.75455
Sample 11	6.1%	0.91795	0.80114
Sample 12	6.8%	0.96111	0.85412

A: immunoassay device (Example 1) of the present invention; B: conventional immunoassay device (Comparative Example 1).

Test Example 3: Change in glycosylated hemoglobin measurement value depending on the volume of the drop of a freeze-dried conjugate

[0071] In order to confirm that in the preparation of a freeze-dried conjugate structure uniformity in the volume of drops is closely related to quantitative analysis ability, six different freeze-dried conjugate structures, each being made with drops having a uniform volume of 5 μl , 10 μl , 15 μl , 20 μl , 25 μl , or 30 μl , were prepared and the quantitative analysis of glycosylated hemoglobin was performed. Five samples having different glycosylated hemoglobin concentrations were in turn applied to the six different freeze-dried conjugate structures, and then the levels of glycosylated hemoglobin were measured. Table 3 below shows the glycosylated hemoglobin values of the samples and the measured values from the respective freeze-dried conjugate structures applied thereto. Also, the resulting plot is shown in Fig. 7.

Table 3: Glycated hemoglobin measurement values according to the volume of the drop of a freeze-dried conjugate

HbA1c%	5 μ l	10 μ l	15 μ l	20 μ l	25 μ l	30 μ l
5.4%	0.7245	0.7845	0.8241	0.8716	0.8944	0.9123
7.2%	0.8124	0.8874	0.9214	0.96748	0.9541	1.001
9.5%	0.9841	1.015	1.0135	1.09534	1.1121	1.1231
11.4%	1.0245	1.1112	1.1231	1.18901	1.2234	1.2234
13.8%	1.0844	1.1945	1.2121	1.2752	1.2955	1.3454

[0072] As can be seen in Table 3 and Fig. 7, in a freeze-dried conjugate structure made with drops having a uniform volume, there was a high degree of linear correlation between the glycated hemoglobin concentration and the glycated hemoglobin values. It was also confirmed through the test that in samples at the same concentration level, the glycated hemoglobin values slightly increases as the volume of the drops of the freeze-dried conjugate increases. The results show that the use of a freeze-dried conjugate structure made with drops having a uniform volume between 5-30 μ l helps enhance the accuracy and reproducibility of the quantitative analysis of an immunoassay kit, thereby allowing more accurate qualitative and quantitative assays.

[0073] Meanwhile, it was also found that in a freeze-dried conjugate structure made with drops having different volumes, the intensity of the signal may be affected not only by the concentration of glycated hemoglobin in samples, but even by the volume of the drops of the freeze-dried conjugate. For example, a sample having a glycated hemoglobin concentration of 11.4% showed a glycated hemoglobin value of 1.1231 when a freeze-dried conjugate structure having a volume of 15 μ l was employed, and the same glycated hemoglobin value (1.1231) was obtained in a sample having a glycated hemoglobin concentration of 9.5% employing a freeze-dried conjugate structure having a volume of 30 μ l. This suggests that if a freeze-dried conjugate structure is made with drops having different volumes, the accuracy of sample analysis cannot be guaranteed because it is unclear from what samples measurement values were obtained. This further suggests that the accuracy and reproducibility of the quantitative analysis may be reduced if a freeze-dried conjugate structure made with drops having different volumes is employed.

Claims

1. A freeze-dried conjugate structure for immunochromatography, comprising a first conjugate comprising a first label for signal detection and a first ligand that reacts with an analyte, wherein the first label and the first ligand are physically or chemically linked to each other, and the conjugate structure is formed by rapidly freezing a dispersion, in which the first conjugate at a predetermined concentration is dispersed in a solvent, in the form of drops having a uniform volume of 5-30 μ l, followed by freeze-drying, thereby removing the solvent, wherein the space occupied by the solvent in the freeze-dried drops forms a porous space by removing the solvent, wherein the conjugate structure has a porosity of 70-90%.
2. The freeze-dried conjugate structure of claim 1, further comprising a second conjugate comprising a second label for signal detection and a second ligand that reacts with a reporter molecule, in which the second label and the second ligand are physically or chemically linked to each other, and the second label is the same as or different from the first label.
3. The freeze-dried conjugate structure of claim 1, wherein the ligand is an antigen, an antibody, a receptor or a ligand of the receptor.
4. The freeze-dried conjugate structure of claim 1, wherein the rapid freezing is performed by adding the dispersion dropwisely to a liquid having an evaporation point between -270°C and -180°C.
5. The freeze-dried conjugate structure of claim 1, wherein the rapid freezing is performed by adding the drops having a uniform volume using a dispenser.

6. An immunoassay kit comprising the freeze-dried conjugate structure of any one of claims 1 to 5 and an immunochromatographic strip.
7. The immunoassay kit of claim 6, further comprising a buffer which serves as either a solvent for dissolving the conjugate or a mobile phase for chromatography.
8. The immunoassay kit of claim 6, further comprising a freeze-dried conjugate structure comprising a second conjugate comprising a second label for signal detection and a second ligand that reacts with a reporter molecule, wherein the second label and the second ligand are physically or chemically linked to each other, and the conjugate structure is formed by rapidly freezing a dispersion, in which the second conjugate is dispersed in a solvent, in the form of drops having a uniform volume, followed by freeze-drying, thereby removing the solvent, wherein the space occupied by the solvent in the freeze-dried drops forms a porous space by removing the solvent.
9. The immunoassay kit of claim 6, wherein the immunochromatographic strip comprises a porous membrane pad, which has formed thereon a test line for capturing an analyte in a sample, and an absorbent pad which is provided at one end of the porous membrane pad and serves to provide a driving force for transferring the analyte.
10. The immunoassay kit of claim 9, wherein the test line has immobilized thereon a third ligand that binds specifically to the analyte in the sample.
11. The immunoassay kit of claim 10, wherein the analyte bound to the first label by the first ligand is captured by the third ligand on the test line, and the presence, amount, or both, of the analyte in the sample is determined by measuring a signal generated from the first label on the test line.
12. The immunoassay kit of claim 9, wherein the immunochromatographic strip further comprises, before or after the test line, a control line for determining whether the sample migrated, in which the control line has immobilized thereon a reporter molecule.
13. A method for qualitatively or quantitatively analyzing an analyte in a sample using the immunoassay kit of claim 6, the method comprising:
- simultaneously or sequentially adding a buffer and a sample to a conjugate structure and simultaneously or sequentially performing the dissolution of the conjugate structure and a reaction between the conjugate and the sample;
- loading a material resulting from the preceding step onto an immunochromatographic strip and allowing the loaded material to migrate along the strip; and
- determining the presence or absence and intensity of a signal generated from a first label on a test line.

40 Patentansprüche

1. Gefriergetrocknete Konjugatstruktur für Immunchromatographie, umfassend ein erstes Konjugat, das eine erste Markierung zur Signaldetektion und einen ersten Liganden umfasst, der mit einem Analyten reagiert, wobei die erste Markierung und der erste Ligand physikalisch oder chemisch miteinander verknüpft sind, und wobei die Konjugatstruktur durch rasches Gefrieren einer Dispersion gebildet wird, in welcher das erste Konjugat in einer vorbestimmten Konzentration in einem Lösemittel in Form von Tropfen dispergiert ist, die ein gleichmäßiges Volumen von 5 bis 30 μ l aufweisen, gefolgt von einem Gefrietrocknen, wodurch das Lösemittel entfernt wird, wobei der Raum, der von dem Lösemittel in den gefriergetrockneten Tropfen eingenommen wird, einen porösen Raum bildet, indem das Lösemittel entfernt wird, wobei die Konjugatstruktur eine Porosität von 70 bis 90 % aufweist.
2. Gefriergetrocknete Konjugatstruktur nach Anspruch 1, ferner umfassend ein zweites Konjugat, das eine zweite Markierung zur Signaldetektion und einen zweiten Liganden umfasst, der mit einem Reportermolekül reagiert, wobei die zweite Markierung und der zweite Ligand physikalisch oder chemisch miteinander verknüpft sind, und wobei die zweite Markierung die gleiche wie die erste Markierung oder von dieser verschieden ist.
3. Gefriergetrocknete Konjugatstruktur nach Anspruch 1, wobei der Ligand ein Antigen, ein Antikörper, ein Rezeptor oder ein Ligand des Rezeptors ist.

EP 2 857 837 B1

4. Gefriergetrocknete Konjugatstruktur nach Anspruch 1, wobei das rasche Gefrieren durchgeführt wird, indem die Dispersion tropfenweise zu einer Flüssigkeit zugesetzt wird, die einen Verdampfungspunkt zwischen -270 °C und -180 °C aufweist.
5. Gefriergetrocknete Konjugatstruktur nach Anspruch 1, wobei das rasche Gefrieren durchgeführt wird, indem die Tropfen, die ein gleichmäßiges Volumen aufweisen, unter Verwendung eines Dispensers zugesetzt werden.
6. Immunassay-Kit, umfassend die gefriergetrocknete Konjugatstruktur nach einem der Ansprüche 1 bis 5 und einen immunchromatographischen Streifen.
7. Immunassay-Kit nach Anspruch 6, ferner umfassend einen Puffer, der entweder als Lösemittel zum Lösen des Konjugats oder als mobile Phase für die Chromatographie dient.
8. Immunassay-Kit nach Anspruch 6, ferner umfassend eine gefriergetrocknete Konjugatstruktur, umfassend ein zweites Konjugat, das eine zweite Markierung zur Signaldetektion und einen zweiten Liganden umfasst, der mit einem Reportermolekül reagiert, wobei die zweite Markierung und der zweite Ligand physikalisch oder chemisch miteinander verknüpft sind, und wobei die Konjugatstruktur durch rasches Gefrieren einer Dispersion gebildet wird, in welcher das zweite Konjugat in einem Lösemittel in Form von Tropfen dispergiert ist, die ein gleichmäßiges Volumen aufweisen, gefolgt von einem Gefrieren, wodurch das Lösemittel entfernt wird, wobei der Raum, der von dem Lösemittel in den gefriergetrockneten Tropfen eingenommen wird, einen porösen Raum bildet, indem das Lösemittel entfernt wird.
9. Immunassay-Kit nach Anspruch 6, wobei der immunchromatographische Streifen ein Kissen aus einer porösen Membran, auf dem eine Testlinie zum Einfangen eines Analyten in einer Probe gebildet ist, und ein Absorptionsmittelkissen umfasst, das an einem Ende des Kissens aus einer porösen Membran vorgesehen ist und dazu dient, eine Antriebskraft zum Transferieren des Analyten bereitzustellen.
10. Immunassay-Kit nach Anspruch 9, wobei auf der Testlinie ein dritter Ligand immobilisiert ist, der spezifisch an den Analyten in der Probe bindet.
11. Immunassay-Kit nach Anspruch 10, wobei der Analyt, der durch den ersten Liganden an die erste Markierung gebunden ist, durch den dritten Liganden auf der Testlinie eingefangen wird, und wobei das Vorhandensein, die Menge oder beides des Analyten in der Probe bestimmt wird, indem ein Signal gemessen wird, das von der ersten Markierung auf der Testlinie erzeugt wird.
12. Immunassay-Kit nach Anspruch 9, wobei der immunchromatographische Streifen vor oder nach der Testlinie ferner eine Kontrolllinie umfasst, um zu bestimmen, ob die Probe migriert ist, wobei auf der Kontrolllinie ein Reportermolekül immobilisiert ist.
13. Verfahren zum qualitativen oder quantitativen Analysieren eines Analyten in einer Probe unter Verwendung des Immunassay-Kits nach Anspruch 6, wobei das Verfahren umfasst:
 - gleichzeitiges oder sequenzielles Zusetzen eines Puffers und einer Probe zu einer Konjugatstruktur und gleichzeitiges oder sequenzielles Durchführen der Lösung der Konjugatstruktur und einer Reaktion zwischen dem Konjugat und der Probe;
 - Laden eines aus dem vorhergehenden Schritt resultierenden Materials auf einen immunchromatographischen Streifen und Ermöglichen, dass das geladene Material entlang des Streifens migriert; und
 - Bestimmen des Vorhandenseins oder der Abwesenheit und der Intensität eines Signals, das von einer ersten Markierung auf einer Testlinie erzeugt wird.

Revendications

1. Une structure de conjugué lyophilisée pour l'immuno-chromatographie, comprenant un premier conjugué comprenant un premier marqueur pour la détection de signal et un premier ligand qui réagit avec un analyte, dans lequel le premier marqueur et le premier ligand sont physiquement ou chimiquement liés l'un à l'autre, et la structure conjuguée est formée en congelant rapidement une dispersion, dans laquelle le premier conjugué à une concentration prédéterminée est dispersé dans un solvant, sous forme de gouttes ayant un volume uniforme de $5 - 30\text{ }\mu\text{l}$, suivi d'une


EP 2 857 837 B1

lyophilisation, éliminant ainsi le solvant, dans lequel l'espace occupé par le solvant dans les gouttes lyophilisées forme un espace poreux en éliminant le solvant, dans lequel la structure conjuguée à une porosité de 70 à 90 %.


- 5 2. La structure de conjugué lyophilisé selon la revendication 1, comprenant en outre un second conjugué comprenant un second marqueur pour la détection du signal et un second ligand qui réagit avec une molécule rapportrice, dans lequel le second marqueur et le second ligand sont physiquement ou chimiquement liés l'un à l'autre, et le deuxième marqueur est identique ou différent du premier marqueur.
- 10 3. La structure de conjugué lyophilisé selon la revendication 1, dans laquelle le ligand est un antigène, un anticorps, un récepteur ou un ligand du récepteur.
- 15 4. La structure de conjugué lyophilisé selon la revendication 1, dans laquelle la congélation rapide est effectuée en ajoutant goutte à goutte la dispersion à un liquide ayant un point d'évaporation compris entre -270° C et -180° C.
- 20 5. La structure de conjugué lyophilisé selon la revendication 1, dans laquelle la congélation rapide est réalisée en ajoutant les gouttes ayant un volume uniforme en utilisant un distributeur.
- 25 6. Un kit de dosage immunologique comprenant la structure conjuguée lyophilisée de l'une quelconque des revendications 1 à 5 et une bande immunochromatographique.
- 30 7. Le kit de dosage immunologique selon la revendication 6, comprenant en outre un tampon qui sert de solvant pour dissoudre le conjugué ou une phase mobile pour la chromatographie.
- 35 8. Le kit de dosage immunologique selon la revendication 6, comprenant en outre une structure conjuguée lyophilisée comprenant un second conjugué comprenant un second marqueur pour la détection du signal et un second ligand qui réagit avec une molécule rapportrice, dans laquelle le second marqueur et le second ligand sont physiquement ou chimiquement liés l'un à l'autre, et la structure conjuguée est formée en congelant rapidement une dispersion, dans laquelle le second conjugué est dispersé dans un solvant, sous forme de gouttes ayant un volume uniforme, suivi d'une lyophilisation, éliminant ainsi le solvant, dans lequel l'espace occupé par le solvant dans les gouttes lyophilisées forme un espace poreux en éliminant le solvant.
- 40 9. Le kit de dosage immunologique selon la revendication 6, dans lequel la bande immunochromatographique comprend un tampon à membrane poreuse, sur lequel est formée une ligne d'essai pour capturer un analyte dans un échantillon, et un tampon absorbant qui est fourni à une extrémité du tampon à membrane poreuse et sert à fournir une force motrice pour transférer l'analyte.
- 45 10. Le kit de dosage immunologique selon la revendication 9, dans lequel la ligne d'essai a immobilisé sur celle-ci un troisième ligand qui se lie spécifiquement à l'analyte dans l'échantillon.
- 50 11. Le kit de dosage immunologique selon la revendication 10, dans lequel l'analyte lié au premier marqueur par le premier ligand est capturé par le troisième ligand sur la ligne d'essai, et la présence, la quantité, ou les deux, de l'analyte dans l'échantillon est déterminée par la mesure d'un signal généré à partir du premier marqueur sur la ligne d'essai.
- 55 12. Le kit de dosage immunologique selon la revendication 9, dans lequel la bande immunochromatographique comprend en outre, avant ou après la ligne d'essai, une ligne de contrôle pour déterminer si l'échantillon a migré, dans lequel la ligne de contrôle a immobilisé une molécule rapportrice.
13. Un procédé d'analyse qualitative ou quantitative d'un analyte dans un échantillon en utilisant le kit de dosage immunologique de la revendication 6, le procédé comprenant :
 - additionner simultanément ou séquentiellement un tampon et un échantillon à une structure conjuguée et la réalisation simultanée ou séquentielle de la dissolution de la structure conjuguée et d'une réaction entre le conjugué et l'échantillon ;
 - charger une matière résultant de l'étape précédente sur une bande immunochromatographique et laisser migrer le matériau chargé le long de la bande ; et
 - déterminer la présence ou l'absence et l'intensité d'un signal généré à partir d'un premier marqueur sur une ligne d'essai.

[FIG. 1]


conventional assay strip

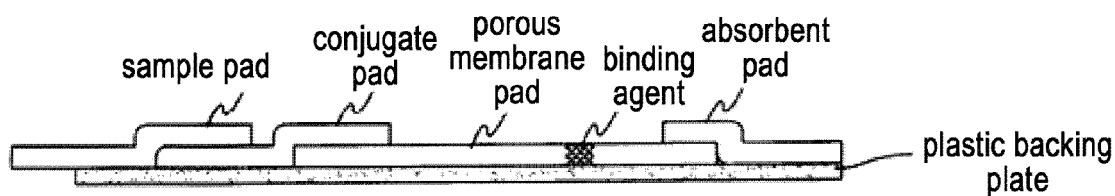


[FIG. 2]

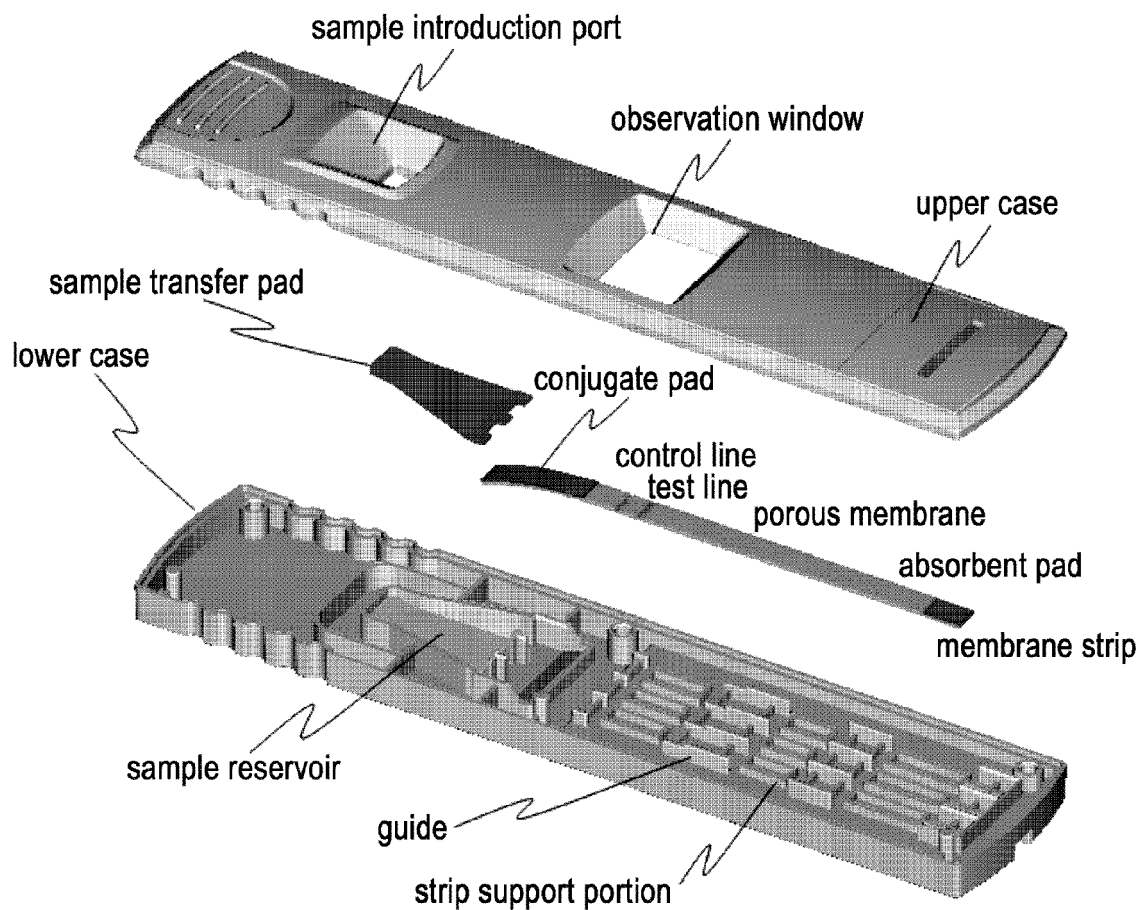


[FIG. 3]

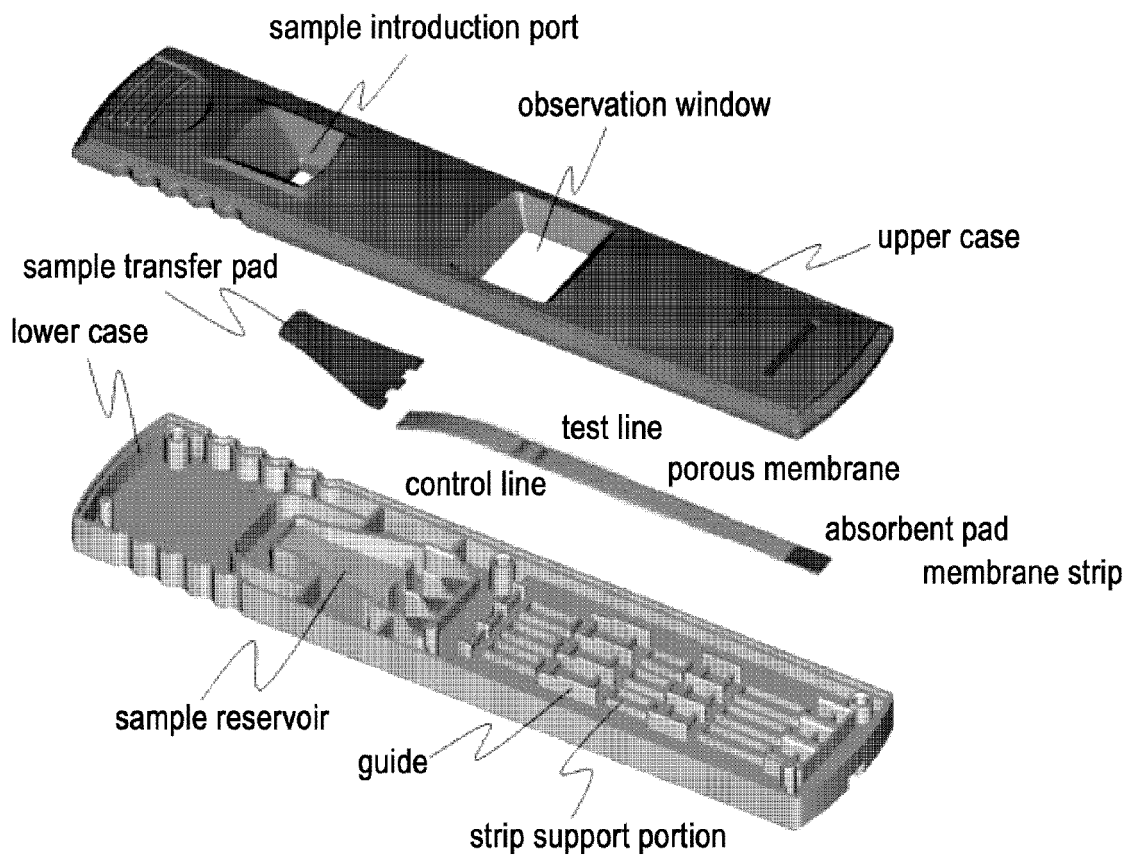


[FIG. 4]

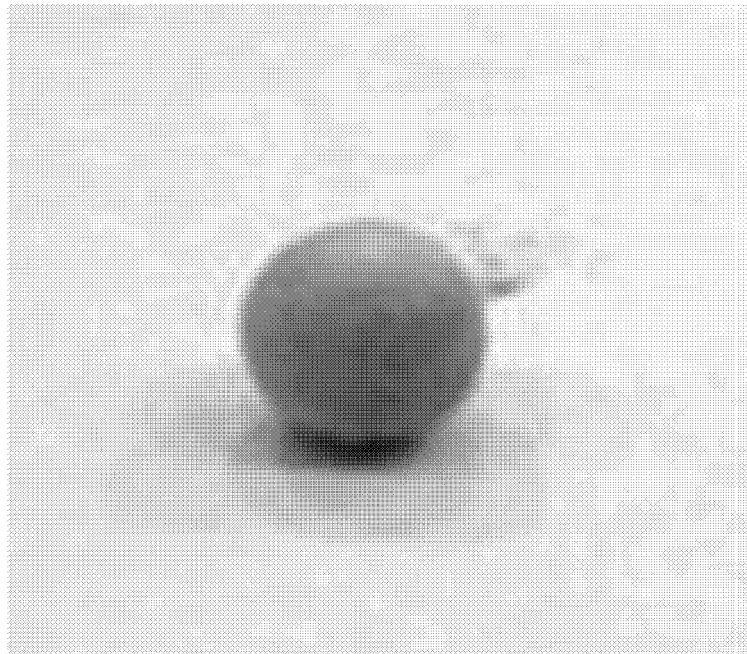


[FIG. 5]

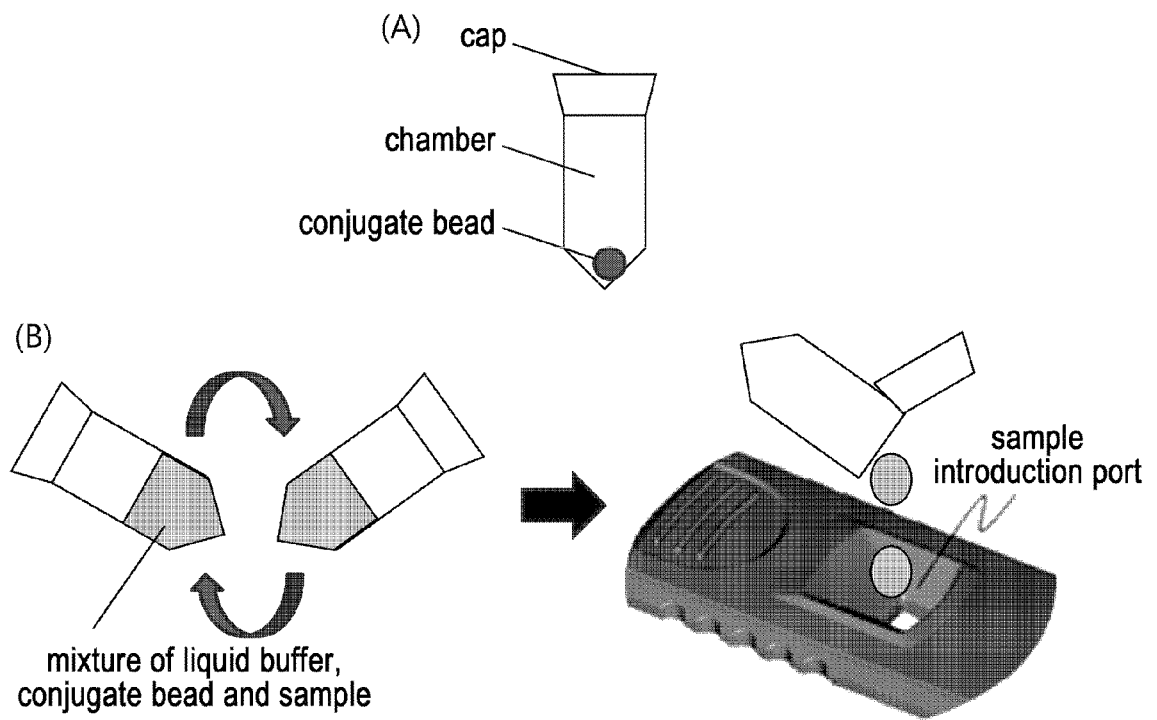

[FIG. 6]

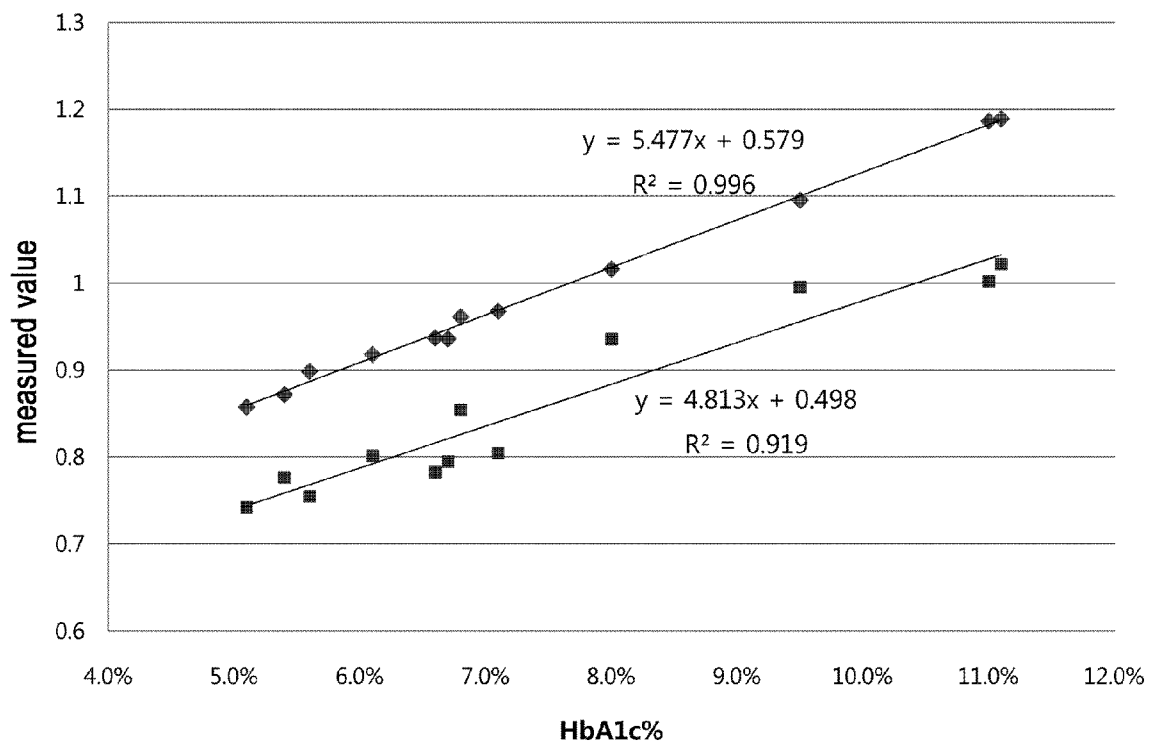

[FIG. 7]

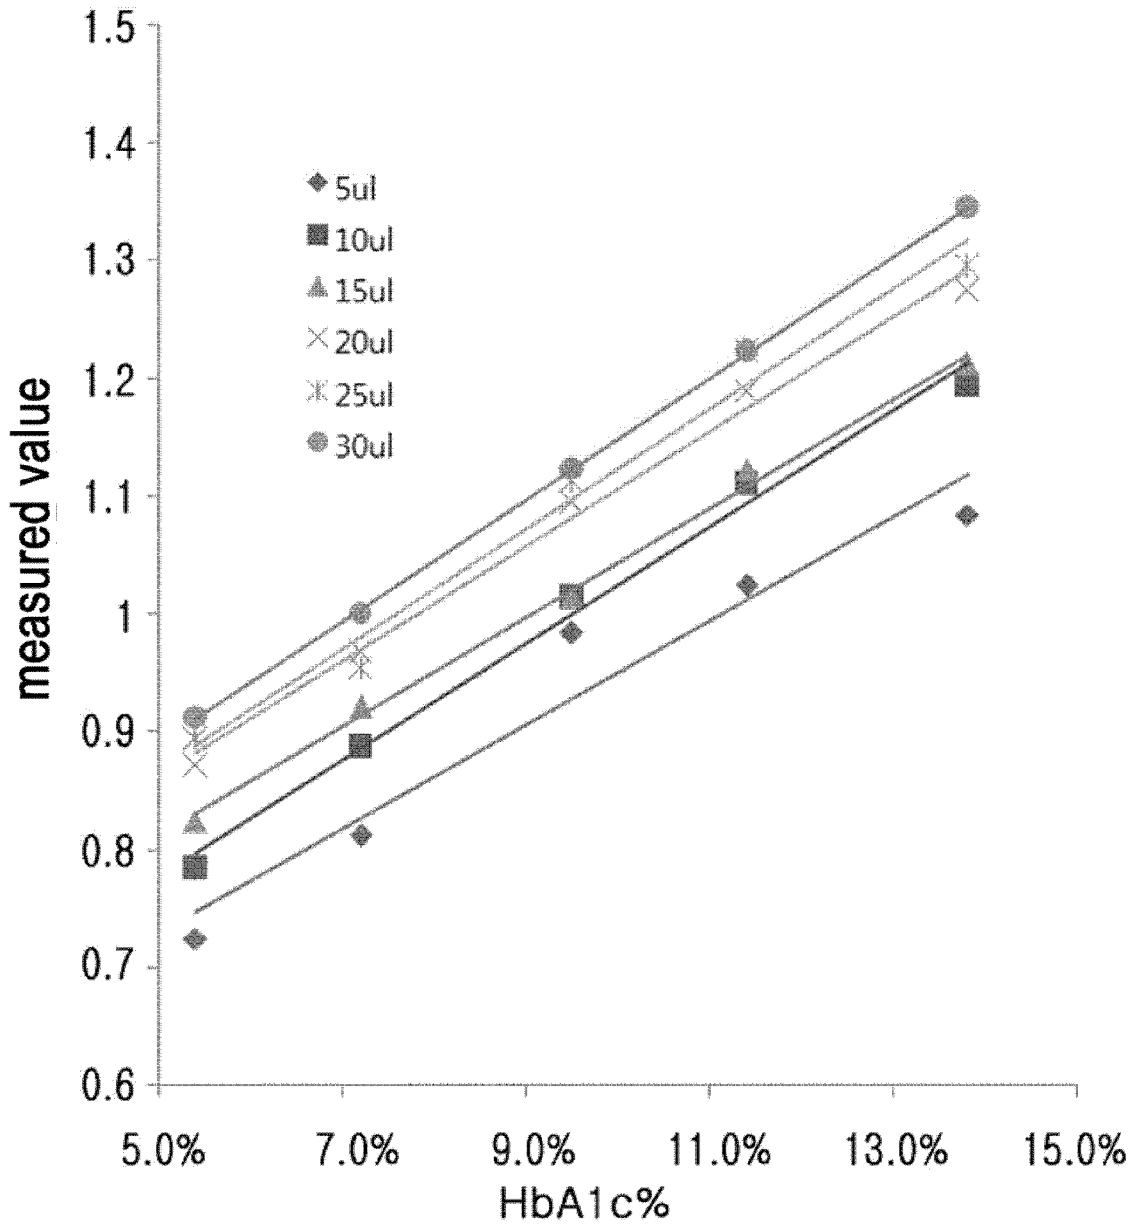

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 2001039059 A1 [0006]
- US 2008090305 A1 [0007]
- WO 9401775 A1 [0008]
- WO 0214869 A2 [0009]
- WO 2006065118 A2 [0010]

专利名称(译)	用于免疫色谱图即时检验的冷冻干燥的缀合物和试剂盒以及使用该试剂盒的方法		
公开(公告)号	EP2857837B1	公开(公告)日	2018-07-25
申请号	EP2013798097	申请日	2013-05-31
[标]申请(专利权)人(译)	SD生物传感器		
申请(专利权)人(译)	SD生物传感器INC.		
当前申请(专利权)人(译)	SD生物传感器INC.		
[标]发明人	CHOI HYOUNG GIL HONG SUNG YUB HWANG HEE YOUNG LEE HYO KEUN		
发明人	CHOI, HYOUNG GIL HONG, SUNG YUB HWANG, HEE YOUNG LEE, HYO KEUN		
IPC分类号	G01N33/558 G01N33/532 G01N33/543		
CPC分类号	G01N33/5436 G01N33/49 G01N33/532 G01N33/538 G01N33/558 G01N33/723 G01N33/90		
优先权	1020120058708 2012-05-31 KR		
其他公开文献	EP2857837A1 EP2857837A4		
外部链接	Espacenet		

摘要(译)

本发明涉及用于免疫层析的冷冻干燥的缀合物结构，包含冷冻干燥的缀合物结构和免疫层析条的免疫测定试剂盒，以及使用免疫测定试剂盒定性或定量分析样品中的分析物的方法。因为样品在与根据本发明单独制备的冷冻干燥的缀合物结构外部均匀反应后进行免疫层析，所以可以以高重复性和线性度进行定量分析，这取决于与使用常规测定方法进行的浓度相比的浓度。免疫层析条带，其包含通过吸附缀合物制备的缀合物垫。另外，本发明的冷冻干燥的缀合物结构可以在其被容纳在另外包括帽的腔室中的状态下提供。因此，它可以在没有污染的情况下储存并且易于携带。另外，冷冻干燥的缀合物结构可以快速和均匀地溶解，以使其立即与缓冲液和样品的混合物反应，并且可以通过免疫测定试剂盒分析反应产物。因此，它适用于即时检验。

$$HbA1c(\%) = \frac{HbA1c(g/dL)}{TotalHb(g/dL)} \times 100$$