



(11)

EP 2 205 968 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
20.11.2013 Bulletin 2013/47

(51) Int Cl.:
G01N 33/48 (2006.01) G01N 33/53 (2006.01)

(21) Application number: **08836072.2**

(86) International application number:
PCT/US2008/078636

(22) Date of filing: **02.10.2008**

(87) International publication number:
WO 2009/046227 (09.04.2009 Gazette 2009/15)

(54) MODULAR POINT-OF-CARE DEVICES AND USES THEREOF

MODULARE POC-VORRICHTUNGEN UND IHRE VERWENDUNG

DISPOSITIFS MODULAIRES À UTILISER SUR PLACE ET LEURS UTILISATIONS

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MT NL NO PL PT
RO SE SI SK TR**

(30) Priority: **02.10.2007 US 997460 P**

(43) Date of publication of application:
14.07.2010 Bulletin 2010/28

(60) Divisional application:
13178059.5 / 2 657 699

(73) Proprietor: **Theranos, Inc.**
Palo Alto, CA 94304 (US)

(72) Inventors:
• **BURD, Tammy**
San Jose, CA 95125 (US)
• **GIBBONS, Ian**
Portola Valley, CA 94028 (US)
• **HOLMES, Elizabeth A.**
Palo Alto, CA 94301 (US)
• **FRENZEL, Gary**
Mountain View, CA 94040 (US)
• **NUGENT, Anthony Joseph**
Dublin, CA 94568 (US)

(74) Representative: **Cole, William Gwyn et al**
avidity IP
Kestrel House
Falconry Court
Baker's Lane
Epping, Essex CM16 5DQ (GB)

(56) References cited:
WO-A1-2004/112602 WO-A2-2005/072145
WO-A2-2007/002579 US-A1- 2002 039 723
US-A1- 2003 175 993 US-A1- 2007 224 084
US-B1- 6 291 249

- **GIBBONS I ET AL: "Patient-side immunoassay system with a single-use cartridge for measuring analytes in blood." September 1989 (1989-09), CLINICAL CHEMISTRY SEP 1989 LNKD-PUBMED:2776311, VOL. 35, NR. 9, PAGE(S) 1869 -1873 , XP009137830 ISSN: 0009-9147 * page 1868 - page 1870 ***
- **VON LODE P: "Point-of-care immunotesting: Approaching the analytical performance of central laboratory methods" CLINICAL BIOCHEMISTRY, ELSEVIER INC, US, CA LNKD-DOI:10.1016/J.CLINBIOCHEM.2005.03.008, vol. 38, no. 7, 1 July 2005 (2005-07-01), pages 591-606, XP004974179 ISSN: 0009-9120**

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 2 205 968 B1

Description**[0001]****BACKGROUND OF THE INVENTION**

[0002] The discovery of a vast number of disease biomarkers and the establishment of miniaturized medical systems have opened up new avenues for the prediction, diagnosis and monitoring of treatment of diseases in a point-of-care setting. Point-of-care systems can rapidly deliver test results to medical personnel, other medical professionals and patients. Early diagnosis of a disease or disease progression can allow medical personnel to begin or modify therapy in a timely manner.

[0003] Multiplexed biomarker measurement can provide additional knowledge of the condition of a patient. For example, when monitoring the effects of a drug, three or more biomarkers can be measured in parallel. Typically, microtiter plates and other similar apparatuses have been used to perform multiplexed separation-based assays. A microtiter plate (for example, a 384 well microtiter plate) can perform a large number of assays in parallel.

[0004] In a Point-of-Care (POC) device, the number of assays that can be performed in parallel is often limited by the size of the device and the volume of the sample to be analyzed. In many POC devices, the number assays performed is about 2 to 10. A POC device capable of performing multiplexed assays on a small sample would be desirable.

[0005] A shortcoming of many multiplexed POC assay devices is the high cost of manufacturing the components of the device. If the device is disposable, the high cost of the components can make the manufacturing of a POC device impractical. Further, for multiplexed POC devices that incorporate all of the necessary reagents onboard of the device, if any one of those reagents exhibit instability, an entire manufactured lot of devices may have to be discarded even if all the other reagents are still usable.

[0006] When a customer is interested in a customizing a POC device to a particular set of analytes, manufacturers of multiplexed POC assay systems are often confronted with a need to mix-and-match the assays and reagents of the device. A multiplexed POC assay suitable to each customer can be very expensive, difficult to calibrate, and difficult to maintain quality control.

[0007] POC methods have proven to be very valuable in monitoring disease and therapy (for example, blood glucose systems in diabetes therapy, Prothrombin Time measurement in anticoagulant therapy using Warfarin). By measuring multiple markers, it is believed that complex diseases (such as cancer) and therapies such as multi-drug therapy for cancer can be better monitored and controlled.

[0008] WO 2007/002579 discloses devices and methods for point of care instruments. Gibbons I et al., Clin. Chem., 35/9, 1869-1873, September 1989 discusses a patient-side immunoassay system with a single-use cartridge for measuring analytes in blood. US 2007/224084 discloses portable medical devices that allow real-time detection of analytes from a biological fluid and which are useful for providing point-of-care testing for a variety of medical applications.

SUMMARY OF THE INVENTION

[0009] Thus, there remains an unmet need for alternative designs of POC devices. A desirable design provides modular capture surfaces and assay incubation elements. Furthermore, modular capture surfaces and assay incubation elements need to be integrated into POC disposables suited for just-in-time (JIT) manufacturing methods. It would be desirable to provide a customizable POC device at a practical cost to user and the manufacturer. The present invention addresses these needs and provides related advantages as well.

[0010] In an aspect, a cartridge is disclosed for automated detection of an analyte in a bodily fluid sample comprising: an array of addressable assay units configured to run a chemical reaction that yields a detectable signal indicative of the presence or absence of the analyte; and an array of addressable reagent units, wherein an individual addressable reagent unit of the array is addressed to correspond to an individual addressable assay unit of the array of assay units, and wherein the individual reagent unit is configured to be calibrated in reference to the corresponding individual assay unit before the arrays are assembled on the cartridge and wherein the individual assay unit of the array of addressable assay units and the individual reagent unit of the array of addressable reagent units are configured to be movable into fluid communication such that reagents for running the chemical reaction are brought to contact with the portion of the sample in the assay unit. The device can further comprise a sample collection unit configured to receive the bodily fluid sample.

[0011] In another aspect, a cartridge is disclosed for automated detection of an analyte in a bodily fluid sample comprising: a sample collection unit configured to receive the bodily fluid sample; an array of assay units configured to receive a portion of the sample from the sample collection unit and run a chemical reaction that yields a detectable signal indicative of the presence of the analyte in the sample; and an array of reagent units containing reagents for running the chemical reaction; wherein an individual assay unit of the array of assay units and an individual reagent unit of the

array of reagents units are configured to be movable into fluid communication such that reagents for running the chemical reaction are brought to contact with the bodily fluid sample in the assay unit.

[0012] An individual reagent unit can be configured to receive a movable assay unit. In some embodiments, the individual assay unit comprises an assay tip. In some embodiments, the individual assay unit is configured to run an immunoassay.

[0013] The bodily fluid sample can be a blood sample. In some instances, a sample collection unit is configured to receive a volume of the bodily fluid sample about 50, 20, 10, 5 or 3 microliters or less. In an instance, the sample collection unit is configured to receive a volume of the bodily fluid sample equivalent to a single drop of blood.

[0014] A cartridge as described herein can comprise a pretreatment unit configured to retrieve a portion of the bodily fluid sample for running the chemical reaction to detect the analyte and the pretreatment unit can be configured to retrieve plasma from whole blood sample received in the sample collection unit.

[0015] In an aspect, a system is described herein for automated detection of an analyte in a bodily fluid sample comprising: a cartridge as described herein; and a detection assembly for detecting the detectable signal indicative of the presence or absence of the analyte. The system can further comprise a programmable mechanical device configured to move the individual assay unit from a first location to a second location. In some instances, a system comprises a fluid transfer device. The fluid transfer device can be a pipette and can be automated. A system can also comprise a communication assembly for transmitting a protocol based on the analyte to be detected. In some instances, a system herein comprises a heating block configured to receive an individual assay unit and can also comprise a magnetic block, for example, that can be used for separation of red cells from the sample.

[0016] In another aspect, a system is disclosed for automated detection of a plurality of analytes in a bodily fluid sample, comprising: a fluidic device comprising: a sample collection unit configured to contain the bodily fluid sample; an array of assay units, wherein an individual assay unit of said array of assay units is configured to run a chemical reaction that yields a signal indicative of an individual analyte of said plurality of analytes being detected; and an array of reagent units, wherein an individual reagent unit of said array of reagent units contains a reagent; and a fluid transfer device comprising a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit, and wherein said fluid transfer device comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from the sample collection unit and the reagent from the individual reagent unit into the individual assay unit. In some embodiments, the configuration of the processor to direct fluid transfer effects a degree of dilution of the bodily fluid sample in the array of assay units to bring signals indicative of the plurality of analytes being detected within a detectable range, such that said plurality of analytes are detectable with said system.

[0017] In some instances, a bodily fluid sample comprises at least two analytes that are present at concentrations that differ by at least 2, 5, 10, 15, 50, or 100 orders of magnitude. The degree of dilution of the bodily fluid sample can bring the signals indicative of the at least two analytes within the detectable range.

[0018] A system herein can further comprise a detector configured to detect signal intensities of the detectable range. An exemplary detector is a photomultiplier and a detectable range of the detector can be about 20 to about 10 million counts.

[0019] In some embodiments, wherein the individual head of a fluid transfer device is configured to adhere to the individual assay unit. The individual assay unit can provide an immunoassay reaction site. In some instances, the individual assay unit is a pipette tip. The fluid transfer device can be a pipette such as an air-displacement pipette. The fluid transfer device can also comprises a motor in communication with the programmable processor, wherein the motor can move said plurality of heads based on a protocol from said programmable processor.

[0020] In another aspect, a system is described herein for automated detection of a plurality of analytes in a plasma portion of a whole blood sample, comprising: a device configured to automatically receive and process the whole blood sample to yield the plasma portion, from which a detectable signal indicative of the presence or absence of the analyte of interest is generated onboard the device; and a detection assembly for detecting the detectable signal indicative of the presence or absence of the analyte.

[0021] In an aspect, provided herein is a method of detecting an analyte in a bodily fluid sample comprising: providing a bodily fluid sample to a cartridge as described herein; allowing said sample to react within at least one assay unit; and detecting said detectable signal generated from said analyte collected in said sample of bodily fluid. The bodily fluid sample can be blood and the method can comprise retrieving plasma from the blood.

[0022] In an aspect as provided herein, a method of on-demand assembly of a cartridge for automated detection of an analyte in a bodily fluid sample, wherein the cartridge comprises a housing, said housing comprising: an array of addressable assay units, wherein an individual assay unit of the array is configured to run a chemical reaction that yields a detectable signal indicative of the presence or absence of the analyte; and an array of addressable reagent units, wherein an individual reagent unit of the array is addressed to correspond to the individual assay unit, said method comprises: (i) placing according to the analyte to be detected an array of addressable assay units, wherein an individual assay unit of the array is configured to run a chemical reaction that detects an analyte of interest ordered by said end user, into the housing; (ii) placing according to the analyte to be detected an array of reagent units, wherein an individual

reagent unit of the array corresponds to the individual assay unit, into the housing; and (iii) securing the arrays of (i) and (ii) within the housing of the cartridge. The method can comprise selecting an analyte to be detected. In some embodiments, the method comprises sealing the cartridge. In an embodiment, the method comprises labeling the cartridge with a readable label indicating the analyte to be detected, for example with a bar code or RFID.

[0023] In an aspect, a method is provided for automated detection of a plurality of analytes in a bodily fluid sample, comprising: providing the bodily fluid sample to a fluidic device, wherein the fluidic device comprises: a sample collection unit configured to contain the bodily fluid sample; an array of assay units, wherein an individual assay unit of said array of assay units is configured to run a chemical reaction that yields a signal indicative of an individual analyte of said plurality of analytes being detected; and an array of reagent units, wherein an individual reagent unit of said array of reagent units contains a reagent; engaging the individual assay unit using a fluid transfer device; transferring the bodily fluid sample from the sample collection unit to the individual assay unit using the fluid transfer device; and transferring the reagent from the individual reagent unit to the individual assay unit, thereby reacting the reagent with the bodily fluid sample to yield the signal indicative of the individual analyte of the plurality of analytes being detected.

[0024] In an embodiment, the fluid transfer device comprises a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit; and wherein said fluid transfer device comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from the sample collection unit and the reagent from the individual reagent unit into the individual assay unit. The method can further comprise providing instructions to the programmable processor, wherein the instructions can direct the step of transferring the bodily fluid sample to the individual assay unit.

[0025] In an embodiment, the step of transferring the bodily fluid sample effects a degree of dilution of the bodily fluid sample in the individual assay unit to bring the signal indicative the individual analyte of the plurality of analytes being detected within a detectable range. The bodily fluid sample can comprise at least two individual analytes that are present at concentrations that differ by at least 2, 5, 10, 15, 50, or 100 orders of magnitude. In some instances, the degree of dilution of the bodily fluid sample brings the signals indicative of the at least two individual analytes within the detectable range. In an embodiment, the detectable range is about 1000 to about 1 million counts per second using a photomultiplier.

[0026] In an embodiment, the reagent in the individual reagent unit is an enzyme substrate for an immunoassay and the method can further comprise repeating the step of transferring the reagent from the individual reagent unit after the reaction to yield the signal indicative of the individual analyte of the plurality of analytes being detected is complete, thereby creating a second reaction to yield a second signal indicative of the individual analyte. An intensity of the signal and a second intensity of the second signal indicative of the individual analyte can be averaged to calculate the final intensity of the signal indicative of the individual analyte.

[0027] In an aspect, a method is described herein of measuring a volume of a liquid sample, comprising: reacting a known quantity of a control analyte in a liquid sample with a reagent to yield a detectable signal indicative of the control analyte; and comparing said detectable signal with an expected detectable signal, wherein the expected signal is indicative of an expected volume of the liquid sample, and wherein said comparison provides a measurement of said volume of said liquid sample being measured. In some instances, the control analyte is not normally present in said liquid sample in a detectable amount. The method can comprise verifying the volume of said liquid sample when the measurement of the volume of the sample is within about 50% of the expected volume of the liquid sample. In an embodiment, the method further comprises: reacting a bodily fluid sample containing a target analyte with a reagent to yield a detectable signal indicative of the target analyte; and measuring the quantity of the target analyte in the bodily fluid sample using an intensity of said detectable signal indicative of the target analyte and the measurement of said volume of said liquid sample. The liquid sample and the bodily fluid sample can be the same sample and the control analyte does not react with the target analyte in the bodily fluid sample. In some instances, the liquid sample and the bodily fluid sample are different liquid samples. The control analyte can be, for example, fluorescein-labeled albumin, fluorescein labeled IgG, anti-fluorescein, anti-digoxigenin, digoxigenin-labeled albumin, digoxigenin-labeled IgG, biotinylated proteins, non-human IgG.

[0028] In another aspect, a method of retrieving plasma from a blood sample is provided herein that comprises: mixing a blood sample in the presence of magnetizable particles in a sample collection unit, wherein the magnetizable particles comprise an antibody capture surface for binding to non-plasma portions of the blood sample; and applying a magnetic field above a plasma collection area to the mixed blood sample to effect suspension of the non-plasma portions of the blood sample on top of the plasma collection area. In some instances, the sample collection unit is a capillary tube. The blood sample can be less than about 20 microliters and the plasma retrieved can be less than about 10 microliters. In some instances, the blood sample is not diluted. In some instance, mixing occurs in the presence of antibodies unbound to a solid surface. The mixing can comprise mixing by syringe action.

[0029] Also described is a method of using automated immunoassay for detecting an analyte present in plasma portion of a whole blood sample, comprising: providing a whole blood sample to a device that is configured to automatically receive and process on board the whole blood sample to yield the plasma portion, from which a detectable signal indicative of the presence or absence of the analyte of interest is generated on board; detecting said signal that is

indicative of the presence or absence of the analyte in said bodily fluid sample; and transmitting result of (b) to an end user. The immunoassay can be an ELISA. In some instances, the result is transmitted wirelessly.

[0030] In some embodiments, a method as described herein is carried out in a system as described herein.

BRIEF DESCRIPTION OF THE DRAWINGS

[0031] Many novel features of the invention are set forth with particularity in the appended claims. A better understanding of the features and advantages of the invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which many principles of the invention are utilized, and the accompanying drawings of which:

[0032] Figure 1 illustrates an exemplary device of the invention comprising assay units, reagents unit, and other modular components of the device.

[0033] Figure 2 illustrates two side-cut away views of the exemplary device of Figure 1 comprising cavities in the housing of the device shaped to accommodate an assay unit, a reagent unit, and a sample tip.

[0034] Figure 3A demonstrates an exemplary assay unit that comprises a small tip or tubular formation.

[0035] Figure 3B demonstrates an example of a sample tip as described herein.

[0036] Figures 4A and 4B illustrate two examples of a reagent unit comprising a cup.

[0037] Figure 5 demonstrates an example of a system comprising a device and a fluid transfer device.

[0038] Figure 6 illustrates an exemplary system of the invention comprising a heating block for temperature control and a detector.

[0039] Figure 7 demonstrates an exemplary a system wherein a patient delivers blood to a device and then the device is inserted into a reader.

[0040] Figure 8 illustrates the process flow of building a system for assessing the medical condition of a patient.

[0041] Figures 9A through 9E demonstrate an example of a plasma separation method wherein a whole blood sample has been aspirated into a sample tip and a magnetic reagent is mixed and suspended with the sample, then a magnetic field is applied to the whole blood sample and magnetic reagent mixture. Separated blood plasma sample can then be distributed into a well of a device.

[0042] Figure 10 demonstrates an exemplary method of a control assay as described herein comprising a known quantity of control analyte.

[0043] Figure 11 illustrates a thin film, for example, contamination, within the tip when a liquid is expelled and another liquid aspirated.

[0044] Figure 12 illustrates a calibration curve correlating an assay unit and a reagent unit for conducting an assay for VEGFR2.

[0045] Figure 13 illustrates a calibration curve correlating results for an assay unit and a reagent unit for conducting an assay for P1GF in a system, as measured with a luminometer.

[0046] Figure 14 illustrates CRP concentration plotted against the assay signal (photon counts) and the data fitted to a 5-term polynomial function to generate a calibration function.

[0047] Figure 15 shows a fit was achieved between a model and the values of the parameters Smax, C0.5 and D as described herein.

[0048] Figure 16 displays data according to the dilution used to achieve the final concentration in an assay tip.

[0049] Figure 17 illustrates the normalized assay response (B/B_{max}) is plotted against the log normalized concentration ($C/C_{0.5}$) for relative dilutions: 1:1 (solid line), 5:1 (dashed line), and 25:1 (dotted line).

[0050] Figures 18 and 19 illustrate a similar example as Figure 17 at different normalized concentrations.

[0051] Figure 20 demonstrates the assay response for a control analyte after the steps of: removal of the detector antibody, washing the assay, and adding a substrate, as read in a spectro-luminometer for 0.5 s.

[0052] Figure 21 demonstrates the results of an assay that was evaluated by measuring photons produced over about 10 s in a system herein.

DETAILED DESCRIPTION OF THE INVENTION

[0053] The embodiments and aspects of the invention described herein pertain to devices, systems, and methods for automated detection of an analyte in a sample of bodily fluid. The invention is capable of detecting and/or quantifying analytes that are associated with specific biological processes, physiological conditions, disorders or stages of disorders, or effects of biological or therapeutic agents.

Devices

[0054] In an aspect of the invention, a device for automated detection of an analyte in a bodily fluid sample comprises

an array of addressable assay units configured to run a chemical reaction that yields a detectable signal indicative of the presence or absence of the analyte, and an array of addressable reagent units, each of which is addressed to correspond to one or more addressable assay units in said device, such that individual reagent units can be calibrated in reference to the corresponding assay unit(s) before the arrays are assembled on the device.

[0055] In another aspect of the invention, a device for automated detection of an analyte in a bodily fluid sample comprises an array of assay units configured to run a chemical reaction that yields a detectable signal indicative of the presence of the analyte, and an array of reagent units containing reagents for running the chemical reaction, wherein at least one of the assay units and at least one of the reagent units are movable relative to each other within the device such that reagents for running the chemical reaction are automatically brought to contact with the bodily fluid sample in the assay unit.

[0056] In an embodiment of a device of the invention, the array of assay units or reagent units can be addressed according to the chemical reaction to be run by the configured assay unit. In another embodiment, at least one of the assay units and at least one of the reagent units are movable relative to each other within the device such that reagents for running the chemical reaction are automatically brought to contact with the bodily fluid sample in the assay unit.

[0057] In one embodiment, the device of the invention is self-contained and comprises all reagents, liquid- and solid-phase reagents, required to perform a plurality of assays in parallel. Where desired, the device is configured to perform at least 2, 3, 4, 5, 6, 7, 8, 9, 10, 20, 30, 40, 50, 100, 200, 500, 1000 or more assays. One or more control assays can also be incorporated into the device to be performed in parallel if desired.

[0058] The assays can be quantitative immunoassays and can be conducted in a short period of time. Other assay type can be performed with a device of the invention including, but not limited to, measurements of nucleic acid sequences and measurements of metabolites, such as cholesterol. In some embodiments, the assay is completed in no more than one hour, preferably less than 30, 15, 10, or 5 minutes. In other embodiments, the assay is performed in less than 5 minutes. The duration of assay detection can be adjusted accordingly to the type of assay that is to be carried out with a device of the invention. For example, if needed for higher sensitivity, an assay can be incubated for more than one hour or up to more than one day. In some examples, assays that require a long duration may be more practical in other POC applications, such as home use, than in a clinical POC setting.

[0059] Any bodily fluids suspected to contain an analyte of interest can be used in conjunction with the system or devices of the invention. Commonly employed bodily fluids include but are not limited to blood, serum, saliva, urine, gastric and digestive fluid, tears, stool, semen, vaginal fluid, interstitial fluids derived from tumorous tissue, and cerebrospinal fluid.

[0060] A bodily fluid may be drawn from a patient and provided to a device in a variety of ways, including but not limited to, lancing, injection, or pipetting. As used herein, the terms subject and patient are used interchangeably herein, and refer to a vertebrate, preferably a mammal, more preferably a human. Mammals include, but are not limited to, murines, simians, humans, farm animals, sport animals, and pets. In one embodiment, a lancet punctures the skin and withdraws a sample using, for example, gravity, capillary action, aspiration, or vacuum force. The lancet may be part of the device, or part of a system, or a stand alone component. Where needed, the lancet may be activated by a variety of mechanical, electrical, electromechanical, or any other known activation mechanism or any combination of such methods. In another embodiment where no active mechanism is required, a patient can simply provide a bodily fluid to the device, as for example, could occur with a saliva sample. The collected fluid can be placed in the sample collection unit within the device. In yet another embodiment, the device comprises at least one microneedle which punctures the skin. 3

[0061] The volume of bodily fluid to be used with a device is generally less than about 500 microliters, typically between about 1 to 100 microliters. Where desired, a sample of 1 to 50 microliters, 1 to 40 microliters, 1 to 30 microliters, 1 to 10 microliters or even 1 to 3 microliters can be used for detecting an analyte using the device.

[0062] In an embodiment, the volume of bodily fluid used for detecting an analyte utilizing the subject devices or systems is one drop of fluid. For example, one drop of blood from a pricked finger can provide the sample of bodily fluid to be analyzed with a device, system or method described herein.

[0063] A sample of bodily fluid can be collected from a subject and delivered to a device of the invention as described hereinafter.

[0064] In an embodiment, the arrays of assay and reagent units are configured to be a set of mix-and-match components. The assay units can comprise at least one capture surface capable of reacting with an analyte from the sample of bodily fluid. The assay unit may be a tubular tip with a capture surface within the tip. Examples of tips of the invention are described herein. A reagent unit typically stores liquid or solid reagents necessary for conducting an assay that detect a give analyte. Each individual assay and reagent unit can be configured for assay function independently. To assemble a device, the units can be assembled in a just-in-time fashion for use in integrated cartridges.

[0065] Separate components, both liquid and solid phase, can be made and then be tested for performance and stored. In an embodiment, the assembly of the device is carried out in on-demand fashion at a manufacturing location. The device can be modular and include components such as a housing that is generic for all assays, assay units, such as tips, and reagent units, such as a variety of frangible or instrument operable containers that encapsulate liquid reagents.

In some instances, an assembled device is then tested to verify calibration (the relation of the system response to known analyte levels). Assay devices can be assembled from a library of premanufactured and calibrated elements on demand. In some embodiments, fluidic pathways within a device can be simple and obviate any chance of trapping bubbles and providing an efficient way to wash away excess labeled reagents in reagent excess assays such as ELISAs.

[0066] A housing for a device of the invention can be made of polystyrene or another moldable or machinable plastic and can have defined locations to place assay units and reagent units. In an embodiment, the housing has means for blotting tips or assay units to remove excess liquid. The means for blotting can be a porous membrane, such as cellulose acetate, or a piece bibulous material such as filter paper.

[0067] In some embodiments, at least one of the components of the device may be constructed of polymeric materials. Non-limiting examples of polymeric materials include polystyrene, polycarbonate, polypropylene, polydimethylsiloxanes (PDMS), polyurethane, polyvinylchloride (PVC), polysulfone, polymethylmethacrylate (PMMA), acrylonitrile-butadiene-styrene (ABS), and glass.

[0068] The device or the subcomponents of the device may be manufactured by variety of methods including, without limitation, stamping, injection molding, embossing, casting, blow molding, machining, welding, ultrasonic welding, and thermal bonding. In an embodiment, a device is manufactured by injection molding, thermal bonding, and ultrasonic welding. The subcomponents of the device can be affixed to each other by thermal bonding, ultrasonic welding, friction fitting (press fitting), adhesives or, in the case of certain substrates, for example, glass, or semi-rigid and non-rigid polymeric substrates, a natural adhesion between the two components.

[0069] An exemplary device as described herein is illustrated in Figure 1. The device **100** is also sometimes referred to herein as a cartridge **100**. The device **100** comprises a housing **130** with locations to accommodate assay units **121** and reagent units **103, 122, 124, 125**. In the exemplary embodiment of Figure 1, assay units **121** occupy a center row of the housing **130** of the device **100**. The assay units **121** can optionally include at least one calibration unit **126**. In an example, the assay units **121** are similar to pipette tips and are referred to as assay tips **121** and the calibration units **126** are referred to as calibration tips **126** herein, however, the assay units **121** can be of any shape and size as are accommodated broadly by a device **100** as described herein. The assay units **121** and calibration units **126** are exemplary assay units **121** and are described in more detail herein. The assay units **121** in Figure 1 can comprise a capture surface and are capable, for example, of performing a chemical reaction such as nucleic acid assays and immunoassays. The assay units **121** can be assembled into the housing according to instructions or the assays that a user wishes to perform on a sample.

[0070] As shown in Figure 1, the housing of the device **100** can comprise a sample collection unit **110** configured to contain a sample. A sample, such as a blood sample, can be placed into the sample collection unit **110**. A sample tip **111** (for example, a pipette tip that couples to a fluid transfer device as described in more detail herein) can occupy another portion of the housing **130**. When an assay is to be run the sample tip **111** can distribute the sample to pretreatment reagent units or pretreatment units **103, 104, 105, 106, 107**, or assay units **121**. Exemplary pretreatment units **103, 104, 105, 106, 107** include but are not limited to: mixing units **107**, diluent or dilution units **103, 104**, and, if the sample is a blood sample, plasma removal or retrieval units **105, 106**. The pretreatment units **103, 104, 105, 106, 107** can be the same type of unit or different types of units. Other pretreatment units **103, 104, 105, 106, 107** as are necessary to run a chemical reaction can be incorporated into device **100** as would be obvious to one skilled in the art with knowledge of this disclosure. The units **103, 104, 105, 106, 107** can contain various amounts of reagents or diluents, flexible to whatever is needed to run the assay on the current cartridge **100**.

[0071] Often, the assay units **121** can be manufactured separately from the housing **130** and then inserted into the housing **130** with pick-and-place methods. The assay units **121** can fit snugly into the housing **130** or can fit loosely into the housing **130**. In some embodiments, the housing **130** is manufactured such that it holds the reagent units **103, 122, 124, 125** and/or assay units **121** snugly in place, for example during shipping or manipulation a cartridge. Reagents units **103, 122, 124, 125** are shown in Figure 1 that contain a conjugate reagent **122** (for example, for use with an immunoassay), a wash reagent **125** (for example, to wash said conjugate from capture surfaces), and a substrate **124** (for example, an enzyme substrate). Other embodiments of the device **100** and the components in the example in Figure 1 are described herein. Reagent units **103, 122, 124, 125** can be manufactured and filled separately from the housing **130** and then placed into the housing **130**. In this way, a cartridge **100** can be built in a modular manner, therefore increasing the flexibility of the cartridge **100** to be used for a variety of assays. Reagents in a reagent unit **103, 122, 124, 125** can be chosen according to the assay to be run. Exemplary reagents and assays are described herein.

[0072] A device, such as the example shown in Figure 1, can also comprise other features as may be needed to run a chemical reaction. For example, if the assay units **121** are assay tips **121** as described herein, the device can comprise tip touch-off pads **112** to remove excess sample or reagent from an assay tip **121** or a sample tip **111** after fluid transfer, for example, by a system as described herein. The housing **130** can also comprise units or areas **101, 102** within the device **100** for placing a used tip or unit, for example, in order to avoid cross-contamination of a sample tip **111** or assay unit **121**. In Figure 1, the device **100** comprises a sample tip **111** for transferring a sample between units of the device **100**. The device **100** as illustrated in Figure 1 also comprises a pretreatment tip **113** for transferring a sample that has

been pretreated in a unit of the device **100** to other units of a device **100** to perform a chemical reaction. For example, the sample tip **111** can be used to remove a blood sample from the sample collection unit **110** and transfer the blood sample to pretreatment units **103, 104, 105, 106, 107** as described. Red cells can be removed from the blood sample in the pretreatment units **103, 104, 105, 106, 107** and the pretreatment tip **113** can then be used to collect the blood plasma from the pretreatment units **103, 104, 105, 106, 107** and transfer the blood plasma to another pretreatment unit (for example, a diluent unit) **103, 104, 105, 106, 107** and/or to at least one assay unit **121**. In an embodiment, a sample tip **111** is the sample collection unit **110**. In another embodiment, the sample collection unit **110** is similar to a well and is configured to contain a sample as received by a user.

[0073] Assay units **121** and reagent units **103, 122, 124, 125** as shown in Figure 1 can be addressable to indicate the location of the units on the cartridge **100**. For example, a column of the cartridge **100** as shown in Figure 1 can contain an assay unit **121** to run an assay configured to detect C-reactive protein, and the column can contain corresponding reagent units **103, 122, 124, 125** for that assay in the same column, wherein the units are addressed to correspond to each other. For example, the addresses can be entered and stored in a computer system, and the cartridge **100** can be given a label, such as a bar code. When the bar code of the cartridge **100** is scanned for use, the computer system can send the addresses of the units to a system, such as those described herein, to transfer the fluids and run a reaction according to the addresses entered into the computer. The addresses can be part of a protocol sent to operate the system. The addresses can be in any configuration and can be altered if need be to change the protocol of running an assay, which in turn can offer a change in assay protocol or steps to a user of the cartridge that has not been typically available in prior art POC devices. In some embodiments, the housing **130** and units are configured in a 6 by 8 array of units as shown in Figure 1. The layout of the units can be of any format, for example, rectangular arrays or random layouts. A cartridge **100** can comprise any number of units, for example between 1 and about **500**. In some embodiments, a cartridge **100** has between 5-100 units. As an example as shown in Figure 1, the cartridge **100** has 48 units.

[0074] Two side cut-away views of the exemplary device **200** of Figure 1 are illustrated in Figures 2A and 2B. A cavity can be shaped in a housing **220** of a device to accommodate assay units (for example, assay tips) **201** in a vertical orientation (housing horizontal) with their bosses toward the top of the device **200**. As shown in Figure 2, a cavity can also be shaped to accommodate a reagent unit **210, 212** or a sample collection unit or tip **202**. There may be features in the housing **220** to capture the units precisely and hold them securely. Such features can also be designed to operate with a mechanism for moving the tips, such as tip pick-up and drop-off. In another embodiment, the sample collection unit comprises a bendable or breakable element that serves to protect a small collection tube during shipment and to hold a plunger device in place within a capillary. Also shown in Figure 2A are two exemplary embodiments of reagent units **210, 212** as are described herein. The bottom of the housing **220** can be configured to collect waste liquids, for example, wash reagents after use that are transferred back through a hole in the housing **220** to the bottom. The housing **220** can comprise an absorbent pad to collect waste fluids. The assay units **201** and sample units **202** can be positioned to fit through a cavity of the housing **220** of the device **200** and extend beyond an inner support structure. The reagent units **210, 212** fit snugly into the housing as is shown in Figure 2 and do not extend beyond the inner support structure. The housing **220** and the areas in which the assay units **201** and reagents units **210, 212** can be held and positioned may adapt a variety of patterns.

[0075] In some embodiments, each tip provides for a single assay and can be paired with or corresponded to an appropriate reagent, such as required reagents for running the designated assay. Some tips provide for control assay units and have known amounts of analyte bound to their capture surfaces either in the manufacturing process or during the performance of an assay. In case of a control assay unit, the unit is configured to run a control assay for comparison. The control assay unit may comprise, for example, a capture surface and analyte that are in a solid or liquid state.

[0076] In many embodiments, the device holds all reagents and liquids required by the assay. For example, for a luminogenic ELISA assay the reagents within the device may include a sample diluent, a detector conjugate (for example, three enzyme-labeled antibodies), a wash solution, and an enzyme substrate. Additional reagents can be provided as needed.

[0077] In some embodiments, reagents can be incorporated into a device to provide for sample pretreatment. Examples of pretreatment reagents include, without limitation, white cell lysis reagents, reagents for liberating analytes from binding factors in the sample, enzymes, and detergents. The pretreatment reagents can also be added to a diluent contained within the device.

[0078] An individual reagent unit can be configured to receive a movable assay unit. In some embodiments, the individual assay unit comprises an open ended hollow cylindrical element comprising a capture surface and a reaction cuvette. A cylindrical assay unit can be referred to as an assay tip herein. In some embodiments, the individual assay unit is configured to run an immunoassay. An assay unit **301** that comprises a small tip or tubular formation is shown in Figure 3A. In some instances, the tip **301** is configured to provide an interior cylindrical capture surface **311** and a boss **321** capable of engaging with the housing of device. In some instances, the boss **321** and the tip **301** is configured to engage with a mechanism of moving the tip **301** such as a system as described herein or for example, a fluid transfer device. An assay tip **301** as shown in Figure 3A can comprise an opening **331** at the bottom of the tip. The opening **331**

can be utilized for transferring fluids or reagents in and out of an assay unit **301**. In an embodiment, an assay unit **301** as described is or is similar to a pipette tip with the improvement that the assay unit **301** comprises a capture surface **311** configured to detect an analyte in a sample.

[0079] The tip **301** can be manufactured by an injection-molded process. In an embodiment, the tip **301** is made of a clear polystyrene for use with chemiluminescence assays. As shown in Figure 3A, an exemplary tip **301** comprises a boss (shown as the larger top half of the tip **301**), which can engage with a housing and can engage, for example, with tapered elements of a fluid transfer device and/or pipetting devices so as to form a pressure-tight seal. Also shown in Figure 3A, the exemplary tip **301** comprises a smaller cylindrical part. In many embodiments, an assay capture surface is contained within the smaller cylindrical part. The assay capture surface can be anywhere within the tip **301** or on the outside of the tip **301**. The surface of the tip **301** can be of many geometries including, but not limited to, tubular, cubic, or pyramidal. In chemiluminescence and fluorescence-based assays, the tip **301** can serve as a convenient means to present the assay product to the assay optics.

[0080] Figure 3B demonstrates an exemplary sample collection unit **302** comprising a sample tip **302**. The sample tip **302** as shown in Figure 3B can also be separate from a sample collection unit **302** and used to transfer sample from the sample collection units to other units on a device as described herein. The sample tip as shown in Figure 3B comprises a boss **322** as described herein to couple the tip **302** with a housing of a device and a fluid transfer device. The sample tip **302** also comprises an opening **332** to allow the transfer of fluids or samples in and out of the sample tip. In some embodiments, the sample tip **302** is of the same shape as an assay tip **301**. In other embodiments (such as those shown in Figures 3A and 3B), the sample tip **302** is a different shape than the assay tip **301**.

[0081] In an embodiment, one function of a tip is to enable samples and liquid reagents to be brought into contact with the capture surface of the assay unit. The movement can occur by a variety of means including, but not limited to, capillary action, aspiration, and controlled pumping. The small size of the tips enables rapid control of the required temperature for a chemical reaction. Heat transfer and/or maintenance can be carried out by simply placing the tip in a temperature controlled block.

[0082] In some embodiments, the tip is able to contain about 1 to 40 microliters of fluid. In a further embodiment, the tip is able to contain about 5 to 25 microliters of fluid. In an embodiment, the tip contains 20 microliters of fluid. In some instances, a tip can contain 1 microliter of fluid or less. In other instances, a tip can contain up to 100 microliters.

[0083] Where desired, the end of the tip can be blotted onto an absorbent material (for example incorporated into a disposable cartridge) prior to introduction of the next assay component to avoid contamination with a small amount of sample and/or reagent. Due to physical forces, any liquid drawn into a subject tip can be held at any desired location with minimal risk of the liquid draining out, even when held in a vertical orientation.

[0084] The assay unit (for example, an assay tip) can be coated with assay capture reagents prior to use, using similar fluidics as in the assay (for example, controlled capillary or mechanical aspiration).

[0085] A capture surface (also referred to herein as a reaction site) can be formed by a binding antibody or other capture reagents bound covalently or by adsorption to the assay unit. The surface can then be dried and maintained in dry condition until used in an assay. In an embodiment, there is a reaction site for each analyte to be measured.

[0086] In an embodiment, the assay unit can be moved into fluid communication with the reagent unit and/or a sample collection unit, such that a reagent or sample can interact with a reaction site where bound probes can detect an analyte of interest in the bodily fluid sample. A reaction site can then provide a signal indicative of the presence or concentration of the analyte of interest, which can then be detected by a detection device described herein.

[0087] In some embodiments, the location and configuration of a reaction site is an important element in an assay device. Most, if not all, disposable immunoassay devices have been configured with their capture surface as an integral part of the device.

[0088] In one embodiment, a molded plastic assay unit is either commercially available or can be made by injection molding with precise shapes and sizes. For example, the characteristic dimension can be a diameter of 0.05 - 3 mm or can be a length of 3 to 30 mm. The units can be coated with capture reagents using method similar to those used to coat microtiter plates but with the advantage that they can be processed in bulk by placing them in a large vessel, adding coating reagents and processing using sieves, holders, and the like to recover the pieces and wash them as needed.

[0089] The assay unit can offer a rigid support on which a reactant can be immobilized. The assay unit is also chosen to provide appropriate characteristics with respect to interactions with light. For example, the assay unit can be made of a material, such as functionalized glass, Si, Ge, GaAs, GaP, SiO₂, SiN₄, modified silicon, or any one of a wide variety of gels or polymers such as (poly)tetrafluoroethylene, (poly)vinylidenedifluoride, polystyrene, polycarbonate, polypropylene, PMMA, ABS, or combinations thereof. In an embodiment, an assay unit comprises polystyrene. Other appropriate materials may be used in accordance with the present invention. A transparent reaction site may be advantageous. In addition, in the case where there is an optically transmissive window permitting light to reach an optical detector, the surface may be advantageously opaque and/or preferentially light scattering.

[0090] A reactant immobilized at the capture surface can be anything useful for detecting an analyte of interest in a sample of bodily fluid. For instance, such reactants include, without limitation, nucleic acid probes, antibodies, cell

membrane receptors, monoclonal antibodies and antisera reactive with a specific analyte. Various commercially available reactants such as a host of polyclonal and monoclonal antibodies specifically developed for specific analytes can be used.

[0091] One skilled in the art will appreciate that there are many ways of immobilizing various reactants onto a support where reaction can take place. The immobilization may be covalent or noncovalent, via a linker moiety, or tethering them to an immobilized moiety. Non-limiting exemplary binding moieties for attaching either nucleic acids or proteinaceous molecules such as antibodies to a solid support include streptavidin or avidin/biotin linkages, carbamate linkages, ester linkages, amide, thioester, (N)-functionalized thiourea, functionalized maleimide, amino, disulfide, amide, hydrazone linkages, and among others. In addition, a silyl moiety can be attached to a nucleic acid directly to a substrate such as glass using methods known in the art. Surface immobilization can also be achieved via a Poly-L Lysine tether, which provides a charge-charge coupling to the surface.

[0092] The assay units can be dried following the last step of incorporating a capture surface. For example, drying can be performed by passive exposure to a dry atmosphere or via the use of a vacuum manifold and/or application of clean dry air through a manifold.

[0093] In many embodiments, an assay unit is designed to enable the unit to be manufactured in a high volume, rapid manufacturing processes. For example, tips can be mounted in large-scale arrays for batch coating of the capture surface into or onto the tip. In another example, tips can be placed into a moving belt or rotating table for serial processing. In yet another example, a large array of tips can be connected to vacuum and/or pressure manifolds for simple processing.

[0094] In an embodiment, an assay unit can be operably coupled with a fluid transfer device. The fluid transfer device can be operated under automatic control without human interaction. In assay units comprising tips, the control of the installed height of a disposable liquid tip relies on the tapered interference attachment of the tip to the liquid dispenser. A fluid transfer device can engage the tip. In some instances, the immersion length of a tip in liquid to be transferred must be known to minimize the liquid contact with the outside of the tip which may be uncontrolled. In order to couple or adhere a tip to the fluid transfer device a hard stop can be molded at the bottom of the tapered connector which engages the nozzle of the dispenser. An air tight seal can be made by an o-ring that is half way up the taper or in the flat bottom of the nozzle. By separating the seal function of the tip from the controlled height of the tip both can be separately adjusted. The modular device and fluid transfer device can enable many assays to be performed in parallel.

[0095] The reagent units of a device can store reagents that are required to perform a given chemical reaction for detecting a given analyte of interest. Liquid reagents can be dispensed into small capsules that can be manufactured from a variety of materials including, without limitation, plastic such as polystyrene, polyethylene, or polypropylene. In some embodiments, the reagent units are cylindrical cups. Two examples of a reagent unit **401**, **402** comprising a cup are shown in Figures 4A and 4B. Where desired, the units **401**, **402** fit snugly into cavities in a housing of a device. The units **401**, **402** can be sealed on the open surface to avoid spilling the reagents **411**, **412** onboard. In some embodiments, the seal is an aluminized plastic and can be sealed to the cup by thermal bonding. A unit can be of any shape as is necessary to contain a reagent. For example, a cylindrical shaped reagent unit **401** is shown in Figure 4A, and the reagent unit contains a liquid reagent **411**. A different shaped reagent unit **402** is illustrated in Figure 4B also contain a liquid reagent **412**. Both exemplary reagent units **401**, **402** comprise optional slight modifications near the top surface that allow the units **401**, **402** to fit snugly into a housing of a device as described herein.

[0096] In many embodiments of the invention the reagent units are modular. The reagent unit can be designed to enable the unit to be manufactured in a high volume, rapid manufacturing processes. For example, many reagent units can be filled and sealed in a large-scale process simultaneously. The reagent units can be filled according to the type of assay or assays to be run by the device. For example, if one user desires different assays than another user, the reagent units can be manufactured accordingly to the preference of each user, without the need to manufacture an entire device. In another example, reagent units can be placed into a moving belt or rotating table for serial processing.

[0097] In another embodiment, the reagent units are accommodated directly into cavities in the housing of a device. In this embodiment, a seal can be made onto areas of housing surrounding the units.

[0098] Reagents according to the present invention include without limitation wash buffers, enzyme substrates, dilution buffers, conjugates, enzyme-labeled conjugates, DNA amplifiers, sample diluents, wash solutions, sample pre-treatment reagents including additives such as detergents, polymers, chelating agents, albumin-binding reagents, enzyme inhibitors, enzymes, anticoagulants, red-cell agglutinating agents, antibodies, or other materials necessary to run an assay on a device. An enzyme-labeled conjugate can be either a polyclonal antibody or monoclonal antibody labeled with an enzyme that can yield a detectable signal upon reaction with an appropriate substrate. Non-limiting examples of such enzymes are alkaline phosphatase and horseradish peroxidase. In some embodiments, the reagents comprise immunoassay reagents. In general, reagents, especially those that are relatively unstable when mixed with liquid, are confined separately in a defined region (for example, a reagent unit) within the device.

[0099] In some embodiments, a reagent unit contains approximately about 5 microliters to about 1 milliliter of liquid. In some embodiments, the unit may contain about 20-200 microliters of liquid. In a further embodiment, the reagent unit contains 100 microliters of fluid. In an embodiment, a reagent unit contains about 40 microliters of fluid. The volume of liquid in a reagent unit may vary depending on the type of assay being run or the sample of bodily fluid provided. In an

embodiment, the volumes of the reagents do not have to be predetermined, but must be more than a known minimum. In some embodiments, the reagents are initially stored dry and dissolved upon initiation of the assay being run on the device.

[0100] In an embodiment, the reagent units can be filled using a siphon, a funnel, a pipette, a syringe, a needle, or a combination thereof. The reagent units may be filled with liquid using a fill channel and a vacuum draw channel. The reagent units can be filled individually or as part of a bulk manufacturing process.

[0101] In an embodiment, an individual reagent unit comprises a different reagent as a means of isolating reagents from each other. The reagent units may also be used to contain a wash solution or a substrate. In addition, the reagent units may be used to contain a luminogenic substrate. In another embodiment, a plurality of reagents are contained within a reagent unit.

[0102] In some instances, the setup of the device enables the capability of pre-calibration of assay units and the reagent units prior to assembly of disposables of the subject device.

Systems

[0103] In an aspect, a system of the invention comprises a device comprising assay units and reagent units comprising reagents (both liquid and solid phase reagents). In some embodiments, at least one of the whole device, an assay unit, a reagent unit, or a combination thereof is disposable. In a system of the invention, the detection of an analyte with a device is operated by an instrument. The instrument, device, and method offer an automated detection system. The automated detection system can be automated based upon a defined protocol or a protocol provided to the system by a user.

[0104] In an aspect, a system for automated detection of an analyte in a bodily fluid sample comprises a device or cartridge, and a detection assembly or detector for detecting the detectable signal indicative of the presence or absence of the analyte.

[0105] In an embodiment, the user applies a sample (for example, a measured or an unmeasured blood sample) to the device and inserts the device into the instrument. All subsequent steps are automatic, programmed either by the instrument (hard wired), the user, a remote user or system, or modification of the instrument operation according to a identifier (for example, a bar code or RFID on the device).

[0106] Examples of different functions of that can be carried out using a system of the invention include, but are not limited to, dilution of a sample, removal of parts of a sample (for example, red blood cells (RBCs)), reacting a sample in an assay unit, adding liquid reagents to the sample and assay unit, washing the reagents from the sample and assay unit, and containing liquids during and following use of the device. Reagents can be onboard the device in a reagent unit or in a reagent unit to be assembled onto the device.

[0107] An automated system can detect a particular analyte in a biological sample (for example, blood) by an enzyme-linked immunosorbent assay (ELISA). The system is amenable to multiplexing and is particularly suited for detecting an analyte of interest present in a small volume of a whole blood sample (for example, 20 microliters or less). The system can also detect analytes in different dilutions of a single sample, allowing different sensitivities to be tested on the same device, when desired. All reagents, supplies, and wastes can be contained on the device of the system.

[0108] In use, a sample from a subject is applied to the assembled device and the device is inserted into an instrument. In an embodiment, an instrument can begin processing the sample by some combination of removal of red cells (blood sample), dilution of the sample, and movement of the sample to the assay unit. In an embodiment with multiplexed assays, a plurality of assay units are used and a portion of the sample is moved to individual assay units in sequence or in parallel. Assays can then be performed by a controlled sequence of incubations and applications of reagents to the capture surfaces.

[0109] An exemplary fluid transfer device is comprised of any component required to perform and/or read the assay. Example components include, but are not limited to, pumps to aspirate and eject accurately known fluid volumes from wells or units of the device, at least one translational stage for improving the precision and accuracy of the movement within the system, a detector to detect an analyte in an assay unit, and temperature regulation means to provide a regulated temperature environment for incubation of assays. In an embodiment of the invention, the instrument controls the temperature of the device. In a further embodiment, the temperature is in the range of about 30-40 degrees Celsius. In some embodiments, the temperature control by the system can comprise active cooling. In some instances, the range of temperature is about 0-100 degrees Celsius. For example, for nucleic acid assays, temperatures up to 100 degrees Celsius can be achieved. In an embodiment, the temperature range is about 15-50 degrees Celsius. A temperature control unit of the system can comprise a thermoelectric device, such as a Peltier device.

[0110] Cartridges, devices, and systems as described herein can offer many features that are not available in existing POC systems or integrated analysis systems. For example, many POC cartridges rely on a closed fluidic system or loop to handle small volumes of liquid in an efficient manner. The cartridges and fluidic devices described herein can have open fluid movement between units of the cartridge. For example, a reagent can be stored in a unit, a sample in a sample collection unit, a diluent in a diluent unit, and the capture surface can be in an assay unit, wherein in one state of cartridge,

none of the units are in fluid communication with any of the other units. Using a fluid transfer device or system as described herein, the units do not have to be in fluid communication with each other in a state. The units can be movable relative to each other in order to bring some units into fluid communication. For example, a fluid transfer device can comprise a head that engages an assay unit and moves the assay unit into fluidic communication with a reagent unit.

[0111] The devices and systems herein can provide an effective means for high throughput and real-time detection of analytes present in a bodily fluid from a subject. The detection methods may be used in a wide variety of circumstances including identification and quantification of analytes that are associated with specific biological processes, physiological conditions, disorders or stages of disorders. As such, the systems have a broad spectrum of utility in, for example, drug screening, disease diagnosis, phylogenetic classification, parental and forensic identification, disease onset and recurrence, individual response to treatment versus population bases, and monitoring of therapy. The subject devices and systems are also particularly useful for advancing preclinical and clinical stage of development of therapeutics, improving patient compliance, monitoring ADRs associated with a prescribed drug, developing individualized medicine, outsourcing blood testing from the central laboratory to the home or on a prescription basis, and monitoring therapeutic agents following regulatory approval. The devices and systems can provide a flexible system for personalized medicine. Using the same system, a device can be changed or interchanged along with a protocol or instructions to a programmable processor of the systems to perform a wide variety of assays as described. The systems and devices herein offer many features of a laboratory setting in a desk-top or smaller size automated instrument.

[0112] In some embodiments a patient may be provided with a plurality of devices to be used for detecting a variety of analytes. A subject may, for example, use different fluidic devices on different days of the week. In some embodiments the software on the external device associating the identifier with a protocol may include a process to compare the current day with the day the fluidic device is to be used based on a clinical trial for example. In another embodiment, the patient is provided different reagent units and assay units that can be fit into a housing of a device interchangeably. In yet another embodiment, as described the patient does not need a new device for each day of testing, but rather, the system can be programmed or reprogrammed by downloading new instructions from, e.g. an external device such as a server. If for example, the two days of the week are not identical, the external device can wirelessly send notification to the subject using any of the methods described herein or known in the art to notify them of the proper device and/or proper instructions for the system. This example is only illustrative and can easily be extended to, for example, notifying a subject that a fluidic device is not being used at the correct time of day.

[0113] For example, a cartridge as illustrated in Figure 1 can comprise a variety of assay units and reagent units. The assay units can comprise a capture surface according to an analyte to be detected. The assay units can then be assembled with the rest of the device in a just-in-time fashion. In many prior art POC devices, the capture surface is integral to the device and if the capture surface is incorrect or not properly formed, the whole device is bad. Using a device as described herein, the capture surface and/or assay unit can be individually quality controlled and customized independently of the reagent units and the housing of the device.

[0114] Reagent units can be filled with a variety of reagents in a similar just-in-time fashion. This provides flexibility of the device being customizable. In addition, the reagent units can be filled with different volumes of reagents without affecting the stability of a device or the chemical reactions to be run within the device. Coupled with a system as described with a fluid transfer device, the devices and units described herein offer flexibility in the methods and protocols of the assays to be run. For example, a batch of similar devices containing the same reagents can be given to a patient pool for a clinical trial. Half way through the clinical trial, a user identifies that the assay could be optimized by changing the dilution of the sample and the amount of reagent provided to the assay unit. As provided herein, the assay can be changed or optimized by only changing the instructions to a programmable processor of the fluid transfer device. For example, the batch of cartridges in the patient pool had excess diluent loaded on the cartridge. The new protocol demands four times as much diluent as the previous protocol. Due to the methods and systems provided herein, the protocol can be changed at a central server and sent to all the systems for executing the methods with the devices without having to provide new devices to the patient pool. In other words, a POC device and system as described herein can offer much of the flexibility of a standard laboratory practice where excess reagents and often excess sample are often available.

[0115] In some instances, wherein the units of the cartridge are separate, devices and systems provide flexibility in construction of the systems described herein. For example, a cartridge can be configured to run 8 assays using an array of assay units and an array of reagent units. Due to the features of the cartridge as described herein, the same housing, or a housing of the same design can be used to manufacture a cartridge with up to 8 different assays than the previous cartridge. This flexibility is difficult to achieve in many current POC device designs because of the closed systems and fluid channels, and therefore the devices may not be modular or as easy to assemble as described.

[0116] Currently, a need exists for the detecting more than one analyte where the analytes are present in widely varying concentration range, for example, one analyte is in the pg/ml concentration range and another is in the ug/ml concentration range. The system as described herein has the ability to simultaneously assay analytes that are present in the same sample in a wide concentration range. Another advantage for being able to detect concentrations of different analytes present in a wide concentration range is the ability to relate the ratios of the concentration of these analytes to

safety and efficacy of multiple drugs administered to a patient. For example, unexpected drug-drug interactions can be a common cause of adverse drug reactions. A real-time, concurrent measurement technique for measuring different analytes would help avoid the potentially disastrous consequence of adverse drug-drug interactions.

[0117] Being able to monitor the rate of change of an analyte concentration and/or or concentration of PD or PK markers over a period of time in a single subject, or performing trend analysis on the concentration, or markers of PD, or PK, whether they are concentrations of drugs or their metabolites, can help prevent potentially dangerous situations. For example, if glucose were the analyte of interest, the concentration of glucose in a sample at a given time as well as the rate of change of the glucose concentration over a given period of time could be highly useful in predicting and avoiding, for example, hypoglycemic events. Such trend analysis has widespread beneficial implications in drug dosing regimen. When multiple drugs and their metabolites are concerned, the ability to spot a trend and take proactive measures is often desirable.

[0118] Accordingly, the data generated with the use of the subject fluidic devices and systems can be utilized for performing a trend analysis on the concentration of an analyte in a subject.

[0119] Often, 8 assays on the same cartridge may require different dilutions or pre-treatments. The range of dilution can be substantial between assays. Many current POC devices offer a limited range of dilution and therefore a limited number of assays that can be potentially carried out on the POC device. However, a system and/or cartridge as described herein can offer a large range of dilutions due to the ability of to serially dilute a sample. Therefore, a large number of potential assays can be performed on a single cartridge or a plurality of cartridges without modifying the detector or reading instrument for the assays.

[0120] In an example, a system as provided herein is configured to run multiple (e.g., five or more) different target analyte detection assays. In order to bring the expected analyte concentration within the range of detection of an immunoassay as described herein and commonly used in the POC field, a sample must be diluted e.g., 3:1, 8:1, 10:1, 100:1, and 2200:1, to run each of the five assays. Because the fluid transfer device is able to hold and move fluid within the device, serial dilutions can be performed with a system as described herein to achieve these five different dilutions and detect all five different target analytes. As described above, the protocol for performing the assays is also capable of being adjusted without modifying the device or the system.

[0121] In a laboratory setting with traditional pipetting, typically larger volumes of sample are used than in a POC setting. For example, a laboratory may analyze a blood sample withdrawn from the arm of a patient in a volume in the milliliter range. In a POC setting, many devices and users demand that the process is fast, easy and/or minimally invasive, therefore, small samples (on the order of a volume in the microliter range) such as one obtained by a fingerstick) are typically analyzed by a POC device. Because of the difference in sample, current POC devices can lose flexibility in running an assay that is afforded in a laboratory setting. For example, to run multiple assays from a sample, a certain minimum volume can be required for each assay to allow for accurate detection of an analyte, therefore putting some limits on a device in a POC setting.

[0122] In another example, a system and/or fluid transfer device as described herein provides a great deal of flexibility. For example, the fluid transfer device can be automated to move an assay unit, an assay tip, or an empty pipette from one unit of the device to a separate unit of the device, not in fluid communication with each other. In some instances, this can avoid cross-contamination of the units of a device as described. In other instances, it allows for the flexibility of moving several fluids within a device as described into contact with each other according to a protocol or instructions. For example, a cartridge comprising 8 different reagents in 8 different reagent units can be addressed and engaged by a fluid transfer device in any order combination as is instructed by a protocol. Therefore, many different sequences can be run for any chemical reaction to run on the device. Without changing the volume of the reagents in the cartridge or the type of reagents in the cartridge, the assay protocol can be different or modified without the need for a second cartridge or a second system.

[0123] For example, a user orders a cartridge with a specific type of capture surface and specific reagents to run an assay to detect an analyte (for example, C-reactive protein (CRP)) in a sample. The protocol the user originally planned for may require 2 washing steps and 3 dilution steps. After the user has received the device and system, the user has decided that the protocol should actually have 5 washing steps and only 1 dilution step. The devices and systems herein can allow the flexibility for this change in protocol without having to reconfigure the device or the system. In this example, only a new protocol or set of instructions are needed to be sent to the programmable processor of the system or the fluid transfer device.

[0124] In another example, a system as provided herein is configured to run five different target analyte detection assays, wherein each assay needs to be incubated at a different temperature. In many prior art POC devices, incubation of multiple assays at different temperatures is a difficult task because the multiple assays are not modular and the capture surfaces cannot be moved relative to the heating device. In a system as described herein, wherein an individual assay unit is configured to run a chemical reaction, an individual assay unit can be place in an individual heating unit. In some embodiments, a system comprises a plurality of heating units. In some instances, a system comprises at least as many heating units as assay units. Therefore, a plurality of assays can be run as a plurality of temperatures.

[0125] Systems and devices as described herein can also provide a variety of quality control measures not previously available with many prior art POC devices. For example, because of the modularity of a device, the assay units and reagents units can be quality controlled separately from each other and/or separately from the housing and/or separately from a system or fluid transfer device. Exemplary methods and systems of quality control offered by the systems and devices herein are described.

[0126] A system as described can run a variety of assays, regardless of the analyte being detected from a bodily fluid sample. A protocol dependent on the identity of the device may be transferred from an external device where it can be stored to a reader assembly to enable the reader assembly to carry out the specific protocol on the device. In some embodiments, the device has an identifier (ID) that is detected or read by an identifier detector described herein. The identifier detector can communicate with a communication assembly via a controller which transmits the identifier to an external device. Where desired, the external device sends a protocol stored on the external device to the communication assembly based on the identifier. The protocol to be run on the system may comprise instructions to the controller of the system to perform the protocol, including but not limited to a particular assay to be run and a detection method to be performed. Once the assay is performed by the system, a signal indicative of an analyte in the bodily fluid sample is generated and detected by a detection assembly of the system. The detected signal may then be communicated to the communications assembly, where it can be transmitted to the external device for processing, including without limitation, calculation of the analyte concentration in the sample.

[0127] In some embodiments, the identifier may be a bar code identifier with a series of black and white lines, which can be read by an identifier detector such as a bar code reader, which are well known. Other identifiers could be a series of alphanumeric values, colors, raised bumps, or any other identifier which can be located on a device and be detected or read by an identifier detector. The identifier detector may also be an LED that emits light which can interact with an identifier which reflects light and is measured by the identifier detector to determine the identity of a device. In some embodiments the identifier may comprise a storage or memory device and can transmit information to an identification detector. In some embodiments a combination of techniques may be used. In some embodiments, the detector is calibrated by used of an optical source, such as an LED.

[0128] In an example, a bodily fluid sample can be provided to a device, and the device can be inserted into a system. In some embodiments the device is partially inserted manually, and then a mechanical switch in the reader assembly automatically properly positions the device inside the system. Any other mechanism known in the art for inserting a disk or cartridge into a system may be used. In some embodiments, manual insertion may be required.

[0129] In some embodiments a method of automatically selecting a protocol to be run on a system comprises providing a device comprising an identifier detector and an identifier; detecting the identifier; transferring said identifier to an external device; and selecting a protocol to be run on the system from a plurality of protocols on said external device associated with said identifier.

[0130] In an aspect, a system for automated detection of a plurality of analytes in a bodily fluid sample is disclosed that comprises: a fluidic device (such as those described herein) comprising: a sample collection unit configured to contain the bodily fluid sample; an array of assay units, wherein an individual assay unit of said array of assay units is configured to run a chemical reaction that yields a signal indicative of an individual analyte of said plurality of analytes being detected; and an array of reagent units, wherein an individual reagent unit of said array of reagent units contains a reagent. The system further comprises a fluid transfer device comprising a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit, and wherein said fluid transfer device comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from the sample collection unit and the reagent from the individual reagent unit into the individual assay unit. For example, an individual assay unit comprises a reagent and is configured is to run a chemical reaction with that reagent.

[0131] In some instances, the configuration of the processor to direct fluid transfer effects a degree of dilution of the bodily fluid sample in the array of assay units to bring signals indicative of the plurality of analytes being detected within a detectable range, such that said plurality of analytes are detectable with said system. In an example, the bodily fluid sample comprises at least two analytes that are present at concentrations that differ by at least 2, 5, 10, 15, 50, or 100 orders of magnitude. In an example the bodily fluid sample is a single drop of blood. In an embodiment, the concentrations of at least two analytes present in a sample differs by up to 10 orders of magnitude (for example, a first analyte is present at 0.1 pg/mL and a second analyte is present at 500 ug/mL. In another example, some protein analytes are found at concentrations of greater than 100 mg/mL, which can extend the range of interest to about twelve orders of magnitude.

[0132] A degree of dilution of the bodily fluid sample can bring the signals indicative of the at least two analytes within the detectable range. In many instances, a system further comprises a detector, such as a photomultiplier (PMT). With a photomultiplier, for example, a detectable range of the detector can be about 10 to about 10 million counts per second. Each count corresponds to a single photon. In some instances, PMTs are not 100% efficient and the observed count rate may be slightly lower than, but still close to, the actual number of photons reaching the detector per unit time. In some instances, counts are measured in about ten intervals of about one second and the results are averaged. In some embodiments, ranges for assays are 1000 - 1,000,000 counts per second when using a PMT as a detector. In some

instances, count rates as low as 100 per second and count rates as high as 10,000,000 are measurable. The linear response range of PMTs (for example, the range where count rate is directly proportional to number of photons per unit time) can be about 1000-3,000,000 counts per second. In an example, an assay has a detectable signal on the low end of about 200-1000 counts per second and on the high end of about 10,000-2,000,000 counts per second. In some instances for protein biomarkers, the count rate is directly proportional to alkaline phosphatase bound to the capture surface and also directly proportional to the analyte concentration. Other exemplary detectors include avalanche photodiodes, avalanche photodiode arrays, CCD arrays, super-cooled CCD arrays. Many other detectors have an output that is digital and generally proportional to photons reaching the detector. The detectable range for exemplary detectors can be suitable to the detector being used.

[0133] An individual head of a fluid transfer device can be configured to adhere to the individual assay unit. The fluid transfer device can be a pipette, such as an air-displacement pipette. The fluid transfer device can be automated. For example, a fluid transfer device can further comprise a motor in communication with a programmable processor and the motor can move the plurality of heads based on a protocol from the programmable processor. As described, an individual assay unit can be a pipette tip, for example, a pipette tip with a capture surface or reaction site.

[0134] Often times, in a POC device, such as the systems and devices described herein, the dilution factor must be estimated and reasonably precise. For example, in environments where non-expert users operate the system there needs to be ways of ensuring a dilution of a sample.

[0135] As described herein, a fluid transfer device can affect a degree of dilution of a sample to provide accurate assay results. For example, a programmable fluid transfer device can be multi-headed) to dilute or serially dilute samples as well as provide mixing of a sample and diluent. A fluid transfer device can also provide fluid movement in POC devices.

[0136] As described, the systems and devices herein can enable many features of the flexibility of laboratory setting in a POC environment. For example, samples can be collected and manipulated automatically in a table top size or smaller device or system. A common issue in POC devices is achieving different dilution ranges when conducting a plurality of assays, wherein the assays may have significantly different sensitivity or specificity. For example, there may be two analytes in a sample, but one analyte has a high concentration in the sample and the other analyte has a very low concentration. As provided, the systems and devices herein can dilute the sample to significantly different levels in order to detect both analytes. For example, if the analyte is in a high concentration, a sample can be serially diluted to the appropriate detection range and provided to a capture surface for detection. In the same system or device, a sample with an analyte in a low concentration may not need to be diluted. In this manner, the assay range of the POC devices and systems provided herein can be expanded from many of the current POC devices.

[0137] A fluid transfer device can be part of a system that is a bench-top instrument. The fluid transfer device can comprise a plurality of heads. Any number of heads as is necessary to detect a plurality of analytes in a sample is envisioned for a fluid transfer device of the invention. In an example, a fluid transfer device has about eight heads mounted in a line and separated by a distance. In an embodiment, the heads have a tapered nozzle that engages by press fitting with a variety of tips, such as assay unit or sample collection units as described herein. The tips can have a feature that enables them to be removed automatically by the instrument and disposed into in a housing of a device as described after use. In an embodiment, the assay tips are clear and transparent and can be similar to a cuvette within which an assay is run that can be detected by an optical detector such as a photomultiplier tube.

[0138] In an example, the programmable processor of a system can comprise instructions or commands and can operate a fluid transfer device according to the instructions to transfer liquid samples by either withdrawing (for drawing liquid in) or extending (for expelling liquid) a piston into a closed air space. Both the volume of air moved and the speed of movement can be precisely controlled, for example, by the programmable processor.

[0139] Mixing of samples (or reagents) with diluents (or other reagents) can be achieved by aspirating components to be mixed into a common tube and then repeatedly aspirating a significant fraction of the combined liquid volume up and down into a tip. Dissolution of reagents dried into a tube can be done in similar fashion. Incubation of liquid samples and reagents with a capture surface on which is bound a capture reagent (for example an antibody) can be achieved by drawing the appropriate liquid into the tip and holding it there for a predetermined time. Removal of samples and reagents can be achieved by expelling the liquid into a reservoir or an absorbent pad in a device as described. Another reagent can then be drawn into the tip according to instructions or protocol from the programmable processor.

[0140] In an example as illustrated in Figure 11, a liquid **1111** previously in a tip **1101** can leave a thin film **1113** within the tip **1101** when expelled. Therefore, a system can use the action of the leading (for example uppermost) portion of the next liquid **1112** to scour the previously present liquid **1111** from the tip **1101**. The portion of the subsequent liquid contaminated with the liquid previously present **1113** can be held within the top of the tip **1101** where it does not continue to interact with the capture surface **1102**. The capture surface **1102** can be in a defined area of the tip **1101** such that the previous liquid **1111** does not react with the capture surface **1102**, for example as shown in Figure 11, the capture surface **1102** occupies a defined portion of the cylindrical part of the tip **1101** not extending all the way up to the boss of the tip. In many instances, incubation time is short (for example 10 minutes) and separation of the contaminated zone of liquid is relatively large (> 1 mm) so diffusion or the active components of the contaminated portion of liquid **1113**

does not occur rapidly enough react with the capture surface **1102** during the incubation. For many high sensitivity assays, there is a requirement to remove one reagent or wash the capture surface (for example, a detector antibody which is labeled with the assay signal generator). In an example, a fluid transfer device of a system described herein can provide washing by adding further removal and aspiration cycles of fluid transfer, for example, using a wash reagent.

In an example, four wash steps demonstrated that the unbound detector antibody in contact with the capture surface is reduced by a factor of better than 10^6 -fold. Any detector antibody non-specifically bound to the capture surface (highly undesirable) can also be removed during this wash process.

[0141] Extension of the range of an assay can be accomplished by dilution of the sample. In POC assay systems using disposable cartridges containing the diluent there is often a practical limit to the extent of dilution. For example, if a small blood sample is obtained by fingerstick (for example, about 20 microliters) is to be diluted and the maximum volume of diluent that can be placed in a tube is 250 microliters, the practical limit of dilution of the whole sample is about 10-fold. In an example herein, a system can aspirate a smaller volume of the sample (for example about 2 microliters) making the maximum dilution factor about 100-fold. For many assays, such dilution factors are acceptable but for an assay like that of CRP (as described in the examples herein) there is a need to dilute the sample much more. Separation-based ELISA assays can have an intrinsic limitation in the capacity of the capture surface to bind the analyte (for example about a few hundred ng/ml for a typical protein analyte). Some analytes are present in blood at hundreds of micrograms/ml. Even when diluted by 100-fold, the analyte concentration may be outside the range of calibration. In an exemplary embodiment of a system, device, and fluid transfer device herein, multiple dilutions can be achieved by performing multiple fluid transfers of the diluent into an individual assay unit or sample collection unit. For example, if the concentration of an analyte is very high in a sample as described above, the sample can be diluted multiple times until the concentration of the analyte is within an acceptable detection range. The systems and methods herein can provide accurate measurements or estimations of the dilutions in order to calculate the original concentration of the analyte.

[0142] In an embodiment, a system herein can move a liquid sample and move an assay unit. A system can comprise a heating block and a detector. In order to move a liquid sample, a system may provide aspiration-, syringe-, or pipette-type action. In an exemplary embodiment, a fluid transfer device for moving a liquid sample is a pipette and pipette head system. The number of pipette devices required by the system can be adjusted according to the type of analyte to be detected and the number of assays being run. The actions performed by the pipette system can be automated or operated manually by a user.

[0143] Figure 5 demonstrates an example of a fluid transfer device **520** and system **500** as described herein. The fluid transfer device system can move eight different or identical volumes of liquid simultaneously using the eight different heads **522**. For example, the cartridge (or device as described herein) **510** comprises eight assay units **501**. Individual assay units **501** are configured according to the type of assay to be run within the unit **501**. Individual assay units **501** may require a certain volume of sample. An individual head **522** can be used to distribute a proper amount of sample to an individual assay unit **501**. In this example, each head **522** corresponds to an addressed individual assay unit **501**.

[0144] The fluid transfer device mechanism **520** can also be used to distribute reagents from the reagent units. Different types of reagents include a conjugate solution, a wash solution, and a substrate solution. In an automated system, the stage **530** on which the device **510** sits can be moved to move the device **510** relative to the positioning of the assay units **501** and heads **522** and according to the steps necessary to complete an assay as demonstrated in Figure 5. Alternatively, the heads **522** and tips **501** or the fluid transfer device **520** can be moved relative to the position of the device **510**.

[0145] In some embodiments, a reagent is provided in dry form and rehydrated and/or dissolved during the assay. Dry forms include lyophilized materials and films coated on surfaces.

[0146] A system can comprise a holder or engager for moving the assay units or tips. An engager may comprise a vacuum assembly or an assembly designed to fit snugly into a boss of an assay unit tip. For example, a means for moving the tips can be moved in a manner similar to the fluid transfer device heads. The device can also be moved on a stage according to the position of an engager or holder.

[0147] In an embodiment, an instrument for moving the tips is the same as an instrument for moving a volume of sample, such as a fluid transfer device as described herein. For example, a sample collection tip can be fit onto a pipette head according to the boss on the collection tip. The collection tip can then be used to distribute the liquid throughout the device and system. After the liquid has been distributed, the collection tip can be disposed, and the pipette head can be fit onto an assay unit according to the boss on the assay unit. The assay unit tip can then be moved from reagent unit to reagent unit, and reagents can be distributed to the assay unit according to the aspiration- or pipette-type action provided by the pipette head. The pipette head can also perform mixing within a collection tip, assay unit, or reagent unit by aspiration- or syringe-type action.

[0148] A system can comprise a heating block for heating the assay or assay unit and/or for control of the assay temperature. Heat can be used in the incubation step of an assay reaction to promote the reaction and shorten the duration necessary for the incubation step. A system can comprise a heating block configured to receive an assay unit of the

invention. The heating block can be configured to receive a plurality of assay units from a device of the invention. For example, if 8 assays are desired to be run on a device, the heating block can be configured to receive 8 assay units. In some embodiments, assay units can be moved into thermal contact with a heating block using the means for moving the assay units. The heating can be performed by a heating means known in the art.

[0149] An exemplary system **600** as described herein is demonstrated in Figure 6. The system **600** comprises a translational stage **630** onto which a device **610** (or cartridge in this example) is placed either manually or automatically or a combination of both. The system **600** also comprises a heating block **640** that can be aligned with the assay units **611** of the device **610**. As shown in Figure 6, the device **610** comprises a series of 8 assay units **611** and multiple corresponding reagent units **612**, and the heating block **640** also comprises an area **641** for at least 8 units to be heated simultaneously. Each of the heating areas **641** can provide the same or different temperatures to each individual assay unit **611** according to the type of assay being run or the type of analyte being detected. The system **600** also comprises a detector (such as a photomultiplier tube) **650** for detection of a signal from an assay unit **611** representative of the detection of an analyte in a sample.

[0150] In an embodiment, a sensor is provided to locate an assay unit relative to a detector when an assay is detected.

[0151] In an embodiment, the detector is a reader assembly housing a detection assembly for detecting a signal produced by at least one assay on the device. The detection assembly may be above the device or at a different orientation in relation to the device based on, for example, the type of assay being performed and the detection mechanism being employed. The detection assembly can be moved into communication with the assay unit or the assay unit can be moved into communication with the detection assembly.

[0152] In many instances, an optical detector is provided and used as the detection device. Non-limiting examples include a photodiode, photomultiplier tube (PMT), photon counting detector, avalanche photo diode, or charge-coupled device (CCD). In some embodiments a pin diode may be used. In some embodiments a pin diode can be coupled to an amplifier to create a detection device with a sensitivity comparable to a PMT. Some assays may generate luminescence as described herein. In some embodiments chemiluminescence is detected. In some embodiments a detection assembly could include a plurality of fiber optic cables connected as a bundle to a CCD detector or to a PMT array. The fiber optic bundle could be constructed of discrete fibers or of many small fibers fused together to form a solid bundle. Such solid bundles are commercially available and easily interfaced to CCD detectors.

[0153] A detector can also comprise a light source, such as a bulb or light emitting diode (LED). The light source can illuminate an assay in order to detect the results. For example, the assay can be a fluorescence assay or an absorbance assay, as are commonly used with nucleic acid assays. The detector can also comprise optics to deliver the light source to the assay, such as a lens or fiber optics.

[0154] In some embodiments, the detection system may comprise non-optical detectors or sensors for detecting a particular parameter of a subject. Such sensors may include temperature, conductivity, potentiometric signals, and amperometric signals, for compounds that are oxidized or reduced, for example, O_2 , H_2O_2 , and I_2 , or oxidizable/reducible organic compounds.

[0155] A device and system may, after manufacturing, be shipped to the end user, together or individually. The device or system of the invention can be packaged with a user manual or instructions for use. In an embodiment, the system of the invention is generic to the type of assays run on different devices. Because components of the device can be modular, a user may only need one system and a variety of devices or assay units or reagent units to run a multitude of assays in a point-of-care environment. In this context, a system can be repeatedly used with multiple devices, and it may be necessary to have sensors on both the device and the system to detect such changes during shipping, for example. During shipping, pressure or temperature changes can impact the performance of a number of components of the present system, and as such a sensor located on either the device or system can relay these changes to, for example, the external device so that adjustments can be made during calibration or during data processing on the external device. For example, if the temperature of a fluidic device is changed to a certain level during shipping, a sensor located on the device could detect this change and convey this information to the system when the device is inserted into the system by the user. There may be an additional detection device in the system to perform these tasks, or such a device may be incorporated into another system component. In some embodiments information may be wirelessly transmitted to either the system or the external device, such as a personal computer or a television. Likewise, a sensor in the system can detect similar changes. In some embodiments, it may be desirable to have a sensor in the shipping packaging as well, either instead of in the system components or in addition thereto. For example, adverse conditions that would render an assay cartridge or system invalid that can be sensed can include exposure to a temperature higher than the maximum tolerable or breach of the cartridge integrity such that moisture penetration.

[0156] In an embodiment, the system comprises a communication assembly capable of transmitting and receiving information wirelessly from an external device. Such wireless communication may be Bluetooth or RTM technology. Various communication methods can be utilized, such as a dial-up wired connection with a modem, a direct link such as a T1, ISDN, or cable line. In some embodiments, a wireless connection is established using exemplary wireless networks such as cellular, satellite, or pager networks, GPRS, or a local data transport system such as Ethernet or token

ring over a local area network. In some embodiments the information is encrypted before it is transmitted over a wireless network. In some embodiments the communication assembly may contain a wireless infrared communication component for sending and receiving information. The system may include integrated graphic cards to facilitate display of information.

[0157] In some embodiments the communication assembly can have a memory or storage device, for example localized RAM, in which the information collected can be stored. A storage device may be required if information can not be transmitted at a given time due to, for example, a temporary inability to wirelessly connect to a network. The information can be associated with the device identifier in the storage device. In some embodiments the communication assembly can retry sending the stored information after a certain amount of time.

[0158] In some embodiments an external device communicates with the communication assembly within the reader assembly. An external device can wirelessly or physically communicate with a system, but can also communicate with a third party, including without limitation a patient, medical personnel, clinicians, laboratory personnel, or others in the health care industry.

[0159] An exemplary method and system is demonstrated in Figure 7. In the example of Figure 7, a patient delivers a blood sample to a device as described herein and then the device is inserted into a reader, wherein the reader can be desktop system capable of reading an analyte in the blood sample. The reader can be a system as described herein. The reader can be a bench-top or desk-top system and can be capable of reading a plurality of different devices as described herein. The reader or system is capable of carrying out a chemical reaction and detecting or reading the results of the chemical reaction. In the example in Figure 7, a reader is automated according to a protocol sent from an external device (for example, a server comprising a user interface). A reader can also send the results of the detection of the chemical reaction to the server and user interface. In an exemplary system, the user (for example, medical personnel such as a physician or researcher) can view and analyze the results as well as decide or develop the protocol used to automate the system. Results can also be stored locally (on the reader) or on the server system. The server can also host patient records, a patient diary, and patient population databases.

[0160] Figure 8 illustrates the process flow of building a system for assessing the medical condition of a subject. The patient inputs personal data and or measurements from a device, reader, and/or system as described herein into a database as may be present on a server as described. The system can be configured to display the personal data on a patient station display. In some embodiments, the patient station display is interactive and the patient can modify inputted data. The same or a different database contains data from other subjects with a similar medical condition. Data from the other subjects can be historical data from public or private institutions. Data from other subjects may also be internal data from a clinical study.

[0161] Figure 8 also illustrates the flow of data from reader collection data that includes the data from the subject to a server that is connected over a public network. The server can manipulate the data or can just provide the data to a user station. The patient data may also be input to the server separately from the data pertaining to a medical condition that is stored in a database. Figure 8 also demonstrates a user station display and the flow of information to medical personnel or a user. For example, using the exemplary process flow of Figure 8, a patient at home can input a bodily fluid sample into a cartridge of the invention as described herein and place it in a system or reader as described herein. The patient can view the data from the system at a patient station display and/or modify or input new data into the process flow. The data from the patient can then travel over a public network, such as the internet, for example, in an encrypted format, to a server comprising a network interface and a processor, wherein the server is located at a central computing hub or in a clinical trial center. The server can use medical condition data to manipulate and understand the data from the user and then send the results over a public network as described to a user station. The user station can be in a medical office or laboratory and have a user station display to display the results of the assay and manipulation of the patient data to the medical personnel. In this example, the medical personnel can receive results and analysis of a sample from a patient from a test that the patient administered in an alternate location such as the patient's home. Other embodiments and example of systems and components of systems are described herein.

[0162] In some embodiments the external device can be a computer system, server, or other electronic device capable of storing information or processing information. In some embodiments the external device includes one or more computer systems, servers, or other electronic devices capable of storing information or processing information. In some embodiments an external device may include a database of patient information, for example but not limited to, medical records or patient history, clinical trial records, or preclinical trial records. An external device can store protocols to be run on a system which can be transmitted to the communication assembly of a system when it has received an identifier indicating which device has been inserted in the system. In some embodiments a protocol can be dependent on a device identifier. In some embodiments the external device stores more than one protocol for each device. In other embodiments patient information on the external device includes more than one protocol. In some instances, the external server stores mathematical algorithms to process a photon count sent from a communication assembly and in some embodiments to calculate the analyte concentration in a bodily fluid sample.

[0163] In some embodiments, the external device can include one or more servers as are known in the art and commercially available. Such servers can provide load balancing, task management, and backup capacity in the event

of failure of one or more of the servers or other components of the external device, to improve the availability of the server. A server can also be implemented on a distributed network of storage and processor units, as known in the art, wherein the data processing according to the present invention reside on workstations such as computers, thereby eliminating the need for a server.

[0164] A server can includes a database and system processes. A database can reside within the server, or it can reside on another server system that is accessible to the server. As the information in a database may contains sensitive information, a security system can be implemented that prevents unauthorized users from gaining access to the database.

[0165] One advantage of some of the features described herein is that information can be transmitted from the external device back to not only the reader assembly, but to other parties or other external devices, for example without limitation, a PDA or cell phone. Such communication can be accomplished via a wireless network as disclosed herein. In some embodiments a calculated analyte concentration or other patient information can be sent to, for example but not limited to, medical personnel or the patient.

[0166] Accordingly, the data generated with the use of the subject devices and systems can be utilized for performing a trend analysis on the concentration of an analyte in a subject.

[0167] Another advantage as described herein is that assay results can be substantially immediately communicated to any third party that may benefit from obtaining the results. For example, once the analyte concentration is determined at the external device, it can be transmitted to a patient or medical personnel who may need to take further action. The communication step to a third party can be performed wirelessly as described herein, and by transmitting the data to a third party's hand held device, the third party can be notified of the assay results virtually anytime and anywhere. Thus, in a time-sensitive scenario, a patient may be contacted immediately anywhere if urgent medical action may be required.

[0168] By detecting a device based on an identifier associated with a fluidic device after it is inserted in the system, the system allows for fluidic device-specific protocols to be downloaded from an external device and run. In some embodiments an external device can store a plurality of protocols associated with the system or associated with a particular patient or group of patients. For example, when the identifier is transmitted to the external device, software on the external device can obtain the identifier. Once obtained, software on the external device, such as a database, can use the identifier to identify protocols stored in the database associated with the identifier. If only one protocol is associated with the identifier, for example, the database can select the protocol and software on the external device can then transmit the protocol to the communication assembly of the system. The ability to use protocols specifically associated with a device allows for any component of a device of the invention to be used with a single system, and thus virtually any analyte of interest can be detected with a single system.

[0169] In some embodiments multiple protocols may be associated with a single identifier. For example, if it is beneficial to detect from the same patient an analyte once a week, and another analyte twice a week, protocols on the external device associated with the identifier can also each be associated with a different day of the week, so that when the identifier is detected, the software on the external device can select a specific protocol that is associated with the day of the week.

[0170] In some embodiments a patient may be provided with a plurality of devices to use to detect a variety of analytes. A subject may, for example, use different devices on different days of the week. In some embodiments the software on the external device associating the identifier with a protocol may include a process to compare the current day with the day the device is to be used based on a clinical trial for example. If for example, the two days of the week are not identical, the external device can wirelessly send notification to the subject using any of the methods described herein or known in the art to notify them that an incorrect device is in the system and also of the correct device to use that day. This example is only illustrative and can easily be extended to, for example, notifying a subject that a device is not being used at the correct time of day.

[0171] The system can also use a networking method of assessing the medical condition of a subject. A system of communicating information may or may not include a reader for reading subject data. For example, if biomarker data is acquired by a microfluidic point-of-care device, the values assigned to different individual biomarkers may be read by the device itself or a separate device. Another example of a reader would be a bar code system to scan in subject data that has been entered in an electronic medical record or a physician chart. A further example of a reader would consist of an electronic patient record database from which subject data could be directly obtained via the communications network. In this way, the efficacy of particular drugs can be demonstrated in real-time, thus justifying reimbursement of the therapy.

[0172] Noncompliance with a medical treatment, including a clinical trial, can seriously undermine the efficacy of the treatment or trial. As such, in some embodiments the system of the present invention can be used to monitor patient compliance and notify the patient or other medical personnel of such noncompliance. For example, a patient taking a pharmaceutical agent as part of medical treatment plan can take a bodily fluid sample which is assayed as described herein, but a metabolite concentration, for example, detected by the system may be at an elevated level compared to a known profile that will indicate multiple doses of the pharmaceutical agent have been taken. The patient or medical personnel may be notified of such noncompliance via any or the wireless methods discussed herein, including without

limitation notification via a handheld device such a PDA or cell phone. Such a known profile may be located or stored on an external device described herein.

[0173] In an embodiment, the system can be used to identify sub-populations of patients which are benefited or harmed by a therapy. In this way, drugs with varying toxicity that would otherwise be forced from the market can be saved by allocating them only to those who will benefit.

Methods

[0174] The devices and methods of the invention provide an effective means for real-time detection of analytes present in a bodily fluid from a subject. The detection methods may be used in a wide variety of circumstances including identification and quantification of analytes that are associated with specific biological processes, physiological conditions, disorders, stages of disorders or stages of therapy. As such, the devices and methods have a broad spectrum of utility in, for example, drug screening, disease diagnosis, phylogenetic classification, parental and forensic identification, disease onset and recurrence, individual response to treatment versus population bases, and monitoring of therapy. The devices and methods are also particularly useful for advancing preclinical and clinical stage of development of therapeutics, improving patient compliance, monitoring ADRs associated with a prescribed drug, individualized medicine, outsourcing blood testing from the central laboratory to the residence of the patient. The device can be employed on a prescription basis, utilized by pharmaceutical companies for monitoring therapeutic agents following regulatory approval or utilized for payors outsourcing blood tests from a central lab.

[0175] Accordingly, in an embodiment, the present invention provides a method of detecting an analyte in a bodily fluid sample comprising providing a blood sample to a device or system of the invention, allowing the sample to react within at least one assay unit of the device, and detecting the detectable signal generated from the analyte in the blood sample.

[0176] Figure 1 demonstrates an exemplary embodiment of a device of the invention comprising at least one assay unit and at least one reagent unit. The assay units (for example, designated as sample tips and calibrator tips in Figure 1) can contain a capture surface and the reagent units can contain items such as conjugates, washes, and substrates. The device exemplified in Figure 1 also comprises a whole blood sample collection tip, a plasma sample collection tip, a blood input well, a beads well or plasma separation well, a tip touch-off or blotting pad, a dilution well, a diluted plasma sample well or plasma diluent well, collection tip disposal areas.

[0177] In an embodiment, a method comprises performing an Enzyme-linked Immunosorbent Assay (ELISA). In an example as described in this paragraph, a sample is provided to a sample collection unit of a device as described herein. The device is then inserted into a system, wherein system detects the type of cartridge or device that is inserted. The system can then communicate with an external device to receive a set of instructions or protocol that allow the system to perform the desired assay or assays of the cartridge. The protocol can be sent to the programmable processor of a fluid transfer device of the system. In an example, the fluid transfer device engages a sample tip of the cartridge and picks up a certain volume of the sample from the sample collection unit and moves it to a pretreatment unit where red blood cells are removed. The plasma of the sample can then be aspirated into a plasma tip or any assay tip by the fluid transfer device according to the protocol. The tip containing the plasma can then pick up a diluent to dilute the sample as is necessary for the assays to be run. Many different dilutions can be carried by using serial dilutions of the sample. For example, each assay tip or assay unit can contain a sample of a different dilution. After the sample is aspirated into an assay unit by the fluid transfer device, the assay unit can then be incubated with the sample to allow any target analyte present to attach to the capture surface. Incubations as described in this example can be at the system or room temperature for any period of time, for example 10 minutes, or can in a heating device of the system as described herein. The assay unit can engage a reagent unit addressed with a reagent corresponding to the assay to be run in each individual assay unit that have a capture surface for that assay. In this example, the first reagent is a detector solution of an ELISA, for example, comprising a detector antibody such as a labeled anti-protein antibody different than the capture surface. The detector solution is then aspirated out of the assay unit and then a wash solution can be aspirated into the assay unit to remove any excess detector solution. Multiple wash steps can be used. The final reagent to be added is an enzymatic substrate which causes the bound detector solution to chemiluminesce. The enzymatic substrate is then expelled from the assay unit and the results of the assay are read by a detector of the system. At each step as described, incubations can occur as necessary as described herein. In this example, the entire process after putting the cartridge into the system is automated and carried out by a protocol or set of instructions to the programmable system.

[0178] One exemplary method proceeds with delivering a blood sample into the blood input well. The sample can then be picked up by a collection tip and inserted into the plasma separation well. Alternatively, the blood can be deposited directly into a well containing a blood separator. For example, plasma separation can be carried out by a variety of methods as described herein. In this example, plasma separation proceeds using magnetizable beads and antibodies to remove the components of the blood that are not plasma. The plasma can then be carried by a plasma collection tip as to not contaminate the sample with the whole blood collection tip. In this example, the plasma collection tip can pick-

up a predetermined amount of diluent and dilute the plasma sample. The diluted plasma sample is then distributed to the assay units (sample tips) to bind to a capture surface. The assay units can be incubated to allow for a capture reaction to be carried out. The assay unit then can be used to collect a conjugate to bind with the reaction in the assay unit. The conjugate can comprise an entity that allows for the detection of an analyte of interest by a detector, such as an optical detector. Once conjugate has been added to the assay unit, the reaction can be incubated. In an exemplary method using an exemplary device of Figure 1, a reagent unit containing a wash for the conjugate is then accessed by the assay unit (sample tip) to remove any excess conjugate that can interfere with any analyte detection. After washing away excess conjugate, a substrate can be added to the assay unit for detection. In addition, in the example of Figure 1 and this method, a calibrator tip assay unit can be used to carry out all of the methods described in this paragraph except the collection and distribution of the sample. Detection and measurements using the calibrator tip assay unit can be used to calibrate the detection and measurements of the analyte from the sample. Other processes and methods similar to those used in this example are described hereinafter.

[0179] Any bodily fluids suspected to contain an analyte of interest can be used in conjunction with the system or devices of the invention. For example, the input well or sample collection unit in the example of Figure 1 can collect or contain any type of commonly employed bodily fluids that include, but are not limited to blood, serum, saliva, urine, gastric and digestive fluid, tears, stool, semen, vaginal fluid, interstitial fluids derived from tumorous tissue liquids extracted from tissue samples, and cerebrospinal fluid. In an embodiment, the bodily fluid is blood and can be obtained by a fingerstick. In an embodiment, the bodily fluid sample is a blood plasma sample.

[0180] A bodily fluid may be drawn from a patient and distributed to the device in a variety of ways including, but not limited to, lancing, injection, or pipetting. In one embodiment, a lancet punctures the skin and delivers the sample into the device using, for example, gravity, capillary action, aspiration, or vacuum force. The lancet may onboard the device, or part of a reader assembly, or a stand alone component. Where needed, the lancet may be activated by a variety of mechanical, electrical, electromechanical, or any other known activation mechanism or any combination of such methods. In another embodiment where no active mechanism is required, a patient can simply provide a bodily fluid to the device, as could occur, for example, with a saliva sample. The collected fluid can be placed into a collection well or unit of the device. In some embodiments, there is a user activated lancet and sample collecting capillary within the device.

[0181] The volume of bodily fluid to be used with a method or device described herein is generally less than about 500 microliters, further can be between about 1 to 100 microliters. Where desired, a sample of 1 to 50 microliters, 1 to 40 microliters, 1 to 30 microliters, 1 to 10 microliters or even 1 to 3 microliters can be used for detecting an analyte using the subject fluidic device. In an embodiment, the sample is 20 microliters.

[0182] In an embodiment, the volume of bodily fluid used for detecting an analyte utilizing the devices, systems, or methods is one drop of fluid. For example, one drop of blood from a pricked finger can provide the sample of bodily fluid to be analyzed with a device, system, or method of the invention.

[0183] In some embodiments, the bodily fluids are used directly for detecting the analytes present in the bodily fluid without further processing. Where desired, however, the bodily fluids can be pre-treated before performing the analysis with a device. The choice of pre-treatments will depend on the type of bodily fluid used and/or the nature of the analyte under investigation. For instance, where the analyte is present at low level in a sample of bodily fluid, the sample can be concentrated via any conventional means to enrich the analyte. Methods of concentrating an analyte include but are not limited to drying, evaporation, centrifugation, sedimentation, precipitation, and amplification. Where the analyte is a nucleic acid, it can be extracted using various lytic enzymes or chemical solutions or using nucleic acid binding resins following the accompanying instructions provided by manufacturers. Where the analyte is a molecule present on or within a cell, extraction can be performed using lysing agents including but not limited to anticoagulants such as EDTA or heparin, denaturing detergent such as SDS or non-denaturing detergent such as Thesit, sodium deoxylate, triton X-100, and tween-20.

[0184] In an embodiment, the subject collects a sample of bodily fluid with a syringe. The sample can enter the syringe through a capillary tube. In an embodiment measuring an analyte in a blood sample, the subject performs a fingerstick and touches the outer end of the glass capillary to the blood so that blood is drawn by capillary action and fills the capillary with a volume. In some instances, the sample volume is known. In some embodiments, the sample volume is in the range of about 5 - 20 microliters or other volume ranges as described herein.

[0185] In another embodiment, a method and system is provided to obtain a plasma sample substantially free of red blood cells from a blood sample. When conducting an assay, the analytes are often contained in the blood plasma, and the red blood cells can interfere with a reaction.

[0186] Often, when measuring a blood sample, the analytes of interest are in the serum or plasma. For clinical purposes, the final reported concentration of multiple blood tests often needs to relate to the concentration of blood serum or blood plasma in a diluted sample. In many cases, blood serum or blood plasma is the test medium of choice in the lab. Two operations may be necessary prior to running an assay, dilution and red blood cell removal. Blood samples vary significantly in the proportion of the sample volume occupied by red cells (the hematocrit which varies from about 20 - 60%). Furthermore, in a point-of-care environment when assay systems are operated by non-expert personnel, the volume of

sample obtained may not be that which is intended. If a change in volume is not recognized, it can lead to error in the reported analyte concentrations.

[0187] In related but separate embodiment, the present invention provides a method of retrieving plasma from a blood sample is provided that comprises mixing a blood sample in the presence of magnetizable particles in a sample collection unit, wherein the magnetizable particles comprise an antibody capture surface for binding to non-plasma portions of the blood sample, and applying a magnetic field above a plasma collection area to the mixed blood sample to effect suspension of the non-plasma portions of the blood sample on top of the plasma collection area, thereby retrieving the plasma from a blood sample.

[0188] In order to process blood samples, the device or system of the invention may include a magnetic reagent or object which binds to red cells and enables magnetic removal of red cells from plasma. The reagent can be provided in lyophilized form but also can be present as a liquid dispersion. A reagent comprised of magnetizable particles (for example, about 1 micrometer in size) can be coated with an antibody to a red cell antigen or to some adaptor molecule. In some embodiments, the reagent also contains unbound antibodies to red cell surface antigens, which may be unlabeled or labeled with an adaptor moiety (such as biotin, digoxigenin, or fluorescein). In an embodiment analyzing a blood sample, the red blood cells in a diluted sample co-agglutinate with the magnetizable particles aided by a solution phase antibody. Alternatively, a lectin that recognizes a red cell surface carbohydrate can be used as a co-agglutination agent. Sometimes, combinations of red cell agglutinating agents are used. Alternatively, a device of the invention can comprise a blood filter, such as a pad of glass fiber, to aid in the separation of red blood cells from a sample.

[0189] When blood is mixed with a magnetic reagent, a co-agglutination can occur in which many, if not all, of the red cells form a mixed agglutinate with the magnetizable particles. The reagent dissolution and mixing process is driven by repeated aspiration using a tip or collection tip of the invention or a pipette-like tip. After the magnetizable mass has formed, the mass can be separated from the blood plasma by use of a magnet to hold the mass in place as plasma is allowed to exit the tip. In an embodiment, the plasma exits the tip by gravity in a vertical orientation, while the magnet holds the mass in place. In another embodiment, the plasma exits the tip by vacuum or pressure means, while the mass is held within the tip. The plasma can be deposited into a well, another collection tip, or assay unit of the invention.

[0190] An example of a plasma separation method of the invention is demonstrated in Figures 9A through 9E. In Figure 9A, a whole blood sample **901** has been aspirated into a sample tip **910** as described herein, for example in the amount of about 20 microliters. The whole blood sample **901** is then deposited into a separation well **920** (for example, a well containing magnetic beads or particles) of an example device. Figure 9B illustrates a method of suspending and mixing a magnetic reagent in the whole blood sample **902** in a separation well (for example, magnetic bead particles and free binding molecules). Figure 9C demonstrates a 10 microliter air slug **930** that can be used to prevent loss from the tip **910**. The mixed whole blood sample and magnetic reagent **902** are incubated for several seconds (for example, 60 to 180 seconds) to allow an agglutination reaction to occur.

[0191] Figure 9D demonstrates the application of a magnetic field **940** to the whole blood cell and magnetic reagent mixture **902**. The magnetic field **940** can be applied by a magnetic collar **942** that is incorporated with a system or with any magnetic means known in the art. The magnetic field **940** attracts any particles that have adhered to the magnetic reagent. In this way, the plasma **903**, which does not adhere with the magnetic reagent, can be separated from non-plasma portions of a whole blood sample.

[0192] Figure 9E demonstrates a method of distributing a blood plasma sample **903**, as separated by the magnetic reagent described herein, into a well or unit **950** of a device as described herein. The blood plasma sample **903** can also be distributed to a collection tip or assay unit, as well as any other sort of assay device as obvious to one skilled in the art. In Figure 9E, the magnetic field **940** is shown to move with the tip **910** distributing the blood plasma sample **903**. In this example, 5 to 8 microliters of plasma have been removed from a 20 microliter whole blood sample. 1 to 99% of a whole blood sample can be plasma separated using a method of the invention. In an embodiment, 25 to 60% of the volume of the whole blood sample is plasma that can be separated.

[0193] Other exemplary steps of a method as described can be completed. In order to move the blood plasma sample to another well or unit, a capillary plasma collection tip (which can be operated by a robotic system or any other system of the invention) collects the blood plasma sample by capillary and aspiration force. Another step can comprise distributing the plasma sample in a diluent, and the sample can then be diluted by the diluent. The diluted blood plasma sample can then be collected by the collection tip in a predetermined volume. The diluted blood plasma sample can then be mixed and distributed into a well or unit of a device to be distributed to one or a plurality of assay units of a device of the invention. The sample can also be distributed into any other type of device, such as a microtiter plate, as would be obvious to those skilled in the art.

[0194] The example process demonstrated in Figures 9A through 9E can be used with other devices and systems, other than those disclosed herein. For example, a fluid transfer tip can contain the agglutinated mass and the plasma could be deposited into a microtiter plate. Other devices and systems as would be obvious to those skilled in the art could be utilized to execute the example blood plasma separation as disclosed herein.

[0195] The sample of bodily fluid can also be diluted in a variety of other manners, such as using a sample collection

device capable of dilution. The housing of the sample collection device can comprise a tube. In the tube, two moveable seals can contain a volume of a diluent. In a preferable embodiment, the volume of the diluent is predetermined, e.g., in about the range of 50 microliters to 1 milliliter, preferably in the range of about 100 microliters to 500 microliters.

[0196] In an aspect, a method for automated detection of a plurality of analytes in a bodily fluid sample is provided that comprises: providing the bodily fluid sample to a fluidic device, wherein the fluidic device comprises: a sample collection unit configured to contain the bodily fluid sample; an array of assay units, wherein an individual assay unit of said array of assay units is configured to run a chemical reaction that yields a signal indicative of an individual analyte of said plurality of analytes being detected; and an array of reagent units, wherein an individual reagent unit of said array of reagent units contains a reagent. The method can also comprise engaging the individual assay unit using a fluid transfer device. Continuing the method, bodily fluid sample can be transferred from the sample collection unit to the individual assay unit using the fluid transfer device and the reagent from the individual reagent unit can be transferred to the individual assay unit, thereby reacting the reagent with the bodily fluid sample to yield the signal indicative of the individual analyte of the plurality of analytes being detected. In some embodiments, the fluid transfer device comprises a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit; and wherein said fluid transfer device comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from the sample collection unit and the reagent from the individual reagent unit into the individual assay unit.

[0197] In some instances, instructions are provided to the programmable processor, for example, by a user, a subject, or the manufacturer. Instructions can be provided from an external device, such as a personal electronic device or a server. The instructions can direct the step of transferring the bodily fluid sample to the individual assay unit. For example, the step of transferring the bodily fluid sample can affect a degree of dilution of the bodily fluid sample in the individual assay unit to bring the signal indicative the individual analyte of the plurality of analytes being detected within a detectable range. In some examples, the degree of dilution of the bodily fluid sample brings the signals indicative of the at least two individual analytes within a detectable range as described herein.

[0198] Pattern recognition techniques can be used to determine if the detection of an analyte or a plurality of analytes by a method as described herein is within or outside a certain range. For example, detectable signals outside the reportable range can be rejected. The certain range can be established during calibration of a fluidic device the reagent and assay units. For example, the range is established when a device is assembled in a just-in-time fashion.

[0199] In some instances, if the detectable signal of an analyte as detected with a lower dilution factor or degree of dilution exceeds that for a higher dilution factor, the lower dilution result can be rejected as invalid. In most instances, concentrations of an analyte in a sample as derived from signals from samples with different degrees of dilution get lower as the degree of dilution becomes greater. If this does happen, an assay result can be verified. The systems, devices, and methods herein provide the flexibility of quality control rules such as those described that many POC devices cannot offer. The systems, devices, and methods provide many of the quality control features as would be expected in a laboratory setting.

[0200] In an embodiment, a sample is diluted in a ratio that is satisfactory for both high sensitivity and low sensitivity assays. For example, a dilution ratio of sample to diluent can be in the range of about 1:10,000 - 1:1. The device can enable a sample to be diluted into separate locations or extents. The device can also enable the sample to be subject to serial dilutions. In further instances, serial dilution within the device or system can dilute the sample up to 10,000,000,000:1.

[0201] In embodiments, a sample containing an analyte for detection can be moved from a first location to a second location by aspiration-, syringe-, or pipette-type action. The sample can be drawn into the reaction tip by capillary action or reduced atmospheric pressure. In some embodiments, the sample is moved to many locations, including an array of assay units of a device of the invention and different wells in the housing of a device of the invention. The process of moving the sample can be automated by a system of the invention, as described herein.

[0202] The assay units and/or collection tips containing the sample can also be moved from a first location to a second location. The process of moving an assay unit or a collection tip can be automated and carried out by a user-defined protocol.

[0203] In an embodiment, the assay units are moved to collect reagent from a reagent unit of the invention. In many embodiments, movement of an assay unit is automated. Aspiration-, syringe-, or pipette-type action can be used to collect reagent from a reagent unit into an assay unit.

[0204] Once a sample has been added to an assay unit that comprises a capture surface, the entire unit can be incubated for a period of time to allow for a reaction between the sample and the capture surface of the assay unit. The amount of time needed to incubate the reaction is often dependent on the type of assay being run. The process can be automated by a system of the invention. In an embodiment, the incubation time is between 30 seconds and 60 minutes. In another embodiment, the incubation time is 10 minutes.

[0205] An assay unit can also be incubated at an elevated temperature. In an embodiment, the assay unit is incubated at temperature in a range of about 20 to 70 degrees Celsius. The assay unit can be inserted into a heating block to

elevate the temperature of the assay unit and/or the contents of the assay unit.

[0206] In an embodiment of a method of the invention, a conjugate is added to the assay unit after a sample has been added to the unit. The conjugate can contain a molecule for labeling an analyte captured by a capture surface in the assay unit. Examples of conjugates and capture surface are described hereinafter. The conjugate can be a reagent contained within a reagent unit. The conjugate can be distributed to the assay unit by aspiration-, syringe-, or pipette-type action. Once a conjugate has been distributed to an assay unit, the assay unit can be incubated to allow the conjugate to react with an analyte within the assay unit. The incubation time can be determined by the type of assay or the analyte to be detected. The incubation temperature can be any temperature appropriate for the reaction.

[0207] In an aspect, a method of calibrating a device for automated detection of an analyte in a bodily fluid sample is provided. A device can comprise an array of addressable assay units configured to run a chemical reaction that yields a detectable signal indicative of the presence or absence of the analyte, and an array of addressable reagent units, each of which is addressed to correspond to one or more addressable assay units in said device, such that individual reagent units are calibrated in reference to the corresponding assay unit(s) before the arrays are assembled on the device. The device is calibrated by calibrating the assay units and reagent units before they are assembled on the device. The device can then be assembled using the calibrated components, making the device, and a method and system that utilize the device, modular components.

[0208] Calibration can be pre-established by measuring the performance of assay reagents, such as conjugates, before the assay units and reagent unit are assembled in a device of the invention. Calibration information and algorithms can be stored on a server linked wirelessly to the assay system. Calibration can be performed in advance or retrospectively by assays performed in replicate systems at a separate location or by using information obtained when the assay system is used.

[0209] In an aspect, a control material can be used in a device or system to measure or verify the extent of dilution of a bodily fluid sample. For example, another issue of solid-phase based assays such as ELISA is that an assay uses a solid-phase reagent that is difficult to quality control without destruction of its function. The systems and methods herein provide methods to determine the dilution achieved in a POC system using a disposable device with automated mixing and/or dilution.

[0210] In an embodiment, a method provides retrospective analysis, for example, by use of a server in real time to analyze data prior to reporting results. For example, an assay can be performed and a control assay can be run in parallel to the assay. The control assay provides a measurement of an expected dilution of the sample. In some examples, the control assay can verify the dilution of the sample and thus, dilution of a sample for the assay or plurality of assays run within the system can be considered accurate.

[0211] A method of measuring a volume of a liquid sample can comprise: reacting a known quantity of a control analyte in a liquid sample with a reagent to yield a detectable signal indicative of the control analyte; and comparing an intensity of said detectable signal with an expected intensity of said detectable signal, wherein the expected intensity of said signal is indicative of an expected volume of the liquid sample, and wherein said comparison provides a measurement of said volume of said liquid sample being measured. In many instances, the control analyte is not present in said liquid sample in a detectable amount.

[0212] In an embodiment, a method can further comprise verifying the volume of said liquid sample when the measurement of the volume of the sample is within about 50% of the expected volume of the liquid sample.

[0213] For example, a method utilized a device or system described herein can further comprise: reacting a bodily fluid sample containing a target analyte with a reagent to yield a detectable signal indicative of the target analyte; and measuring the quantity of the target analyte in the bodily fluid sample using an intensity of said detectable signal indicative of the target analyte and the measurement of said volume of said liquid sample. The liquid sample and the bodily fluid sample can be the same sample. In some embodiments, the control analyte does not react with the target analyte in the bodily fluid sample, therefore providing not interacting with detection of the target analyte.

[0214] In some instances, the liquid sample and the bodily fluid sample are different liquid samples. For example, a control liquid, such as water, and a blood sample. Or in another example, a saliva sample and a blood sample.

[0215] A control analyte can be, without limitation, fluorescein-labeled albumin, fluorescein labeled IgG, anti-fluorescein, anti-digoxigenin, digoxigenin-labeled albumin, digoxigenin-labeled IgG, biotinylated proteins, non-human IgG. Other exemplary control analytes can be obvious to one skilled in the art. In an embodiment, the control analyte does not occur in a human bodily fluid sample.

[0216] In a POC system as described herein configured to detect a plurality of analytes within a sample, the system can have capabilities to dilute and mix liquids. In many instances, an automated system or user can use a control assay to measure the dilution actually achieved and factor that dilution into the system calibration. For example, a control analyte can be never found in the sample of interest and dried into a reagent unit. The quantity of the dried control analyte can be known and mixed with a sample in the reagent unit. The concentration of analyte can be measured to indicate the volume of sample and any dilution performed on the sample.

[0217] Examples of control analytes for an immunoassay include, but are not limited to: fluorescein-labeled protein,

biotinylated protein, fluorescein-labeled, Axlexa™-labeled, Rhodamine-labeled, Texas Red-labeled, immunoglobulin. For example the labeling can be achieved by having at least two haptens linked per molecule of protein. In some embodiments, 1-20 haptens are linked per molecule of protein. In a further embodiment, 4-10 haptens are linked per molecule of protein. Many proteins have large numbers of free amino groups to which the haptens can be attached. In many instances, hapten-modified proteins are stable and soluble. Also, haptens such as fluorescein and Texas Red are sufficiently large and rigid that antibodies with high affinity can be made (for example, a hapten is large enough to fill the antibody binding site). In some embodiments, haptens can be attached to proteins using reagents, such as fluorescein isothiocyanate, and fluorescein carboxylic acid NHS ester to create control analytes in which the part recognized by the assay system is the hapten.

[0218] In some embodiments, a method utilizes dried control analyte. In some examples, a dried control analyte avoids dilution of the sample and can make the control analyte more stable. Dried control analyte can be formulated so it dissolves rapidly and/or completely on exposure to a liquid sample. In some embodiments, a control analyte can be an analyte for which antibodies with high affinity. In some instances, a control analyte can be an analyte that has no cross reaction with any endogenous sample component. Additionally, for example, the analyte can be inexpensive and/or easy to make. In some embodiments, the control analyte is stable over the lifetime of the device or system described herein. Exemplary carriers used to create analytes with covalently linked haptens include proteins such as, but not limited to: albumin, IgG, and casein. Exemplary polymer carriers used to create novel analytes with covalently linked haptens include, but are not limited to: Dextran, Poly-vinylpyrrolidone. Exemplary excipients used to formulate and stabilize control analytes include, but are not limited to: sucrose, salts, and buffers (such as sodium phosphate and tris chloride).

[0219] A control analyte and method as described herein can be used in a variety of ways including the examples described herein. For example, a method can measure a volume of a sample. In some embodiments, a method measures dilution or a dilution factor or a degree of dilution of a sample. In some instances, a method provides a concentration of the control analyte in a sample. In a system or device described herein to detect a plurality of analytes, measurements from a method herein using a control analyte can be used to verify or describe measurements of target analytes. For example, a fluid transfer device with multiple heads may be used to distribute liquid into a plurality of assay units, including a control unit. In some instances, it can be assumed that liquid amount distributed into the plurality of units is the same or similar between the individual units. In some embodiments, a method described herein with a control analyte can be used to verify that the correct volume of sample has been collected or utilized within a device or system. In another embodiment, a method verifies the correct volume of diluent has been provided to the sample. Also, the dilution factor or degree of dilution can also be verified. In yet another embodiment, a method with a control analyte verifies the correct volume of diluted sample has been distributed to the plurality of units.

[0220] Figure 10 demonstrates an exemplary method of a control assay as described herein comprising a known quantity of control analyte. A unit **1010** before assembly into a cartridge can be filled with a solution **1001** comprising a known mass of control analyte **1002**. The liquid of the solution can be removed and the unit **1010** dried to leave the control analyte **1002** in the unit **1010**. The unit **1010** can then be inserted into a device and transported for use. When the unit **1010** is used and receives a sample or diluent **1003**, the sample **1003** can be delivered in an expected volume and mixed with the dried control analyte **1002** within the unit **1010** to create a control solution **1004** with an expected concentration. The control solution **1004** can be optionally diluted. In an embodiment, the control analyte **1002** can be detected by the same manners as a target analyte in the device. The control analyte concentration in the control solution **1004** is measured. The measurement of the concentration can be used to calculate the volume of the sample **1003** added to create the control solution **1004**. In this manner, a user can compare the measured volume of the sample **1003** with the expected volume of the sample **1003**.

[0221] In an example, red blood cells can be removed from a blood sample. However, if some red blood cells remain, or red blood cells are not removed from a blood sample, a method with a control analyte can be used to correct for effects from red blood cells in the blood sample. Because hematocrit can vary significantly (for example, from 20 - 60% of the total volume of a sample), the quantity of an analyte in a fixed or expected volume (v) of blood can be a function of the hematocrit (H expressed here as a decimal fraction). For example, the quantity of analyte with a concentration C in plasma is $C \cdot v \cdot (1-H)$. Thus the quantity for a sample with hematocrit 0.3 is 1.4 times that for a sample with hematocrit 0.5. In an exemplary embodiment, undiluted blood can be dispensed into a device as described and red cells can be removed. A control analyte concentration in the plasma fraction can then be measured to estimate the volume of sample plasma and determine the hematocrit.

[0222] In some embodiments, unbound conjugate may need to be washed from a reaction site to prevent unbound conjugates from producing inaccurate detection. The limiting step of many immunoassays is a washing step. The compromise of minimum carryover and high sensitivity is dependent on the wash removal of unbound conjugate. The wash step can be severely limited in a microtiter plate format due to the difficulty of removing the wash liquid from a well (for example, by automatic means). An assay unit device and system of the invention can have a number of advantages in the way liquids are handled. An advantage may be an improvement in the signal to noise ratio of an assay.

[0223] Removal of the conjugate can be difficult if conjugates are sticking to the edges of the assay units of a device

if, for example, there is not an excess of a wash solution.

[0224] A wash of the conjugate can occur by either pushing the wash solution from above or drawing the wash solution up and expelling the liquid similar to the loading of the sample. The washing can be repeated as many times as necessary.

[0225] When using a wash buffer in an assay, the device can store the wash buffer in reagent units and the assay unit can be brought into fluid communication with the wash. In an embodiment, the wash reagent is able to remove unbound reagent from the assay units by about 99, 99.9, or 99.999% by washing. In general, a high washing efficiency resulting in a high degree of reduction of undesired background signals is preferred. Washing efficiency is typically defined by the ratio of signal from a given assay to the total amount of signal generated by an assay with no wash step and can be readily determined by routine experimentation. It can be generally preferred to increase the volume of washing solution and time of incubation but without sacrificing the signals from a given assay. In some embodiments, washing is performed with about 50 ul to about 5000 ul of washing buffer, preferably between about 50 ul to about 500 ul washing buffer, for about 10 to about 300 seconds.

[0226] Additionally, it can be advantageous to use several cycles of small volumes of wash solution which are separated by periods of time where no wash solution is used. This sequence allows for diffusive washing, where labeled antibodies diffuse over time into the bulk wash solution from protected parts of the assay unit such as the edges or surfaces where it is loosely bound and can then be removed when the wash solution is moved from the reaction site.

[0227] In many embodiments, the last step is to distribute an enzymatic substrate to detect the conjugate by optical or electrical means. Examples of substrates are described hereinafter.

[0228] For example, the reagent in the individual reagent unit of a device herein can be an enzyme substrate for an immunoassay. In another embodiment, the step of transferring the substrate reagent from the individual reagent unit can be repeated after a reaction at the capture site. For example, enzymatic substrate is transferred to a reaction site and incubated. After measuring the assay signal produced, used substrate can be removed and replaced with fresh substrate and the assay signal remeasured. A signal indicative of the individual analyte being can be detected using a system as described herein from both the first and the second application of substrate. The second substrate is usually the same as the original substrate. In an embodiment, the second substrate is transferred to a reaction site from a second reagent unit of a device herein. In another embodiment, the second substrate is transferred to a reaction site from the same reagent unit as the original substrate. Transferring a second substrate thereby creates a second reaction to yield a second signal indicative of the individual analyte. The intensity of the original signal and a second intensity of the second signal can be compared to calculate the final intensity of the signal indicative of the individual analyte and whether the assay was properly conducted.

[0229] In an embodiment, the intensities of the multiple signals can be used for quality control of an assay. For example, if the signals differ by 20%, 30%, 40%, 50%, 60%, 70%, 80%, 90%, 100% or more, the assay results may be disregarded.

[0230] In an embodiment, a method as described herein comprises re-loading sample and or detector-conjugate (enzyme-labeled antibody) and or the enzyme substrate and sample to rectify or confirm an assay signal or to use as an internal control. For example, re-use of an assay tip or unit as described can be provided to verify function and/or to add further sample or control materials obtain a second signal.

[0231] In some instances, a method of re-loading a substrate to an enzyme unit is enabled by the ability of a system as described herein to automatically to transfer liquid samples and reagents into the assay units. Some assays do not require the system to deliver a result immediately or on a schedule, therefore, a control method as described offers an opportunity to possibly enhance the reliability of the results. A response observed following iterations of adding an enzyme substrate can be used to verify the initial response or to calculate spike recovery.

[0232] Experiments have shown that by adding a second enzyme substrate to an assay unit, the reproducibility of results can be maintained. In some embodiments, a control method provides replicate analyses using an assay unit gave a response significantly lower than that expected.

[0233] With any control methods described herein, there are numerous possible errors that can be accounted for or postulated from executing a control method. Exemplary assay errors include, but are not limited to, improper manufacturing of an assay unit or device, improper aspiration of a sample and/or one or more reagents, an assay unit is not positioned properly relative to the photomultiplier during detection, and a missing assay unit in the device or system.

[0234] In some embodiments, the present invention provides a method of obtaining pharmacological data useful for assessing efficacy and/or toxicity of a pharmaceutical agent from a test animal utilizing the subject fluidic devices or systems.

[0235] When using laboratory animals in preclinical testing of a pharmaceutical agent, it is often necessary to kill the test subject to extract enough blood to perform an assay to detect an analyte of interest. This has both financial and ethical implications, and as such it may be advantageous to be able to draw an amount of blood from a test animal such that the animal does not need to be killed. In addition, this can also allow the same test animal to be tested over several different time points, thus allowing for a more effective evaluation of the effects of an agent on single animals. On average, the total blood volume in a mouse, for example, is 6-8 mL of blood per 100 gram of body weight. A benefit of the current invention is that only a very small volume of blood is required to perform preclinical trials on mice or other small laboratory

animals. In some embodiments between about 1 microliter and about 50 microliters are drawn. In an embodiment between about 1 microliter and 10 microliters are drawn. In preferred embodiments about 5 microliters of blood are drawn.

[0236] A further advantage of keeping the test animal alive is evident in a preclinical time course study. When multiple mice, for example, are used to monitor the levels of an analyte in a test subject's bodily fluid over time, the added variable of using multiple subjects is introduced into the trial. When, however, a single test animal can be used as its own control over a course of time, a more accurate and beneficial preclinical trial can be performed.

[0237] In some embodiments a method of automatically monitoring patient compliance with a medical treatment using the subject devices or systems is provided. The method comprises the steps of allowing a sample of bodily fluid to react with assay reagents in a device to yield a detectable signal indicative of the presence of an analyte in said sample; detecting said signal with said device; comparing said signal with a known profile associated with said medical treatment to determine if said patient is compliant or noncompliant with said medical treatment; and notifying a patient of said compliance or noncompliance.

[0238] In another embodiment, the system and methods of the invention provide a means of discovering new biomarkers and/or validating by association of trends in such markers with disease and therapy outcomes.

[0239] In another embodiment, the system and methods of the invention can identify trends in biomarker levels and daily patient diary information over time that can be used to adjust a drug dose to an optimal level for particular patients (for example, adaptive dose-ranging).

[0240] In some embodiments noncompliance may include taking an improper dose of a pharmaceutical agent including without limitation multiple doses or no dose, or may include inappropriately mixing pharmaceutical agents. In preferred embodiments a patient is notified substantially immediately after the signal is compared with a known profile.

[0241] A patient or subject of a clinical trial may forget to take a bodily fluid sample for analysis as described herein. In some embodiments a method of alerting a patient to test a sample of bodily fluid using a device as described herein comprises providing a protocol to be run on said device, said protocol located on an external device, associated with said patient, and comprising a time and date to test said sample of bodily fluid; and notifying patient to test said bodily fluid on said date and time if said sample has not been tested. In some embodiments a patient can be notified wirelessly as described herein. Compliance with therapeutic regimes can be improved by use of prompts on a display and obtaining responses from patients (for example, by way of a touch-screen).

[0242] A patient may be provided with a device when procuring a prescription of drugs by any common methods, for example, at a pharmacy. Likewise, a clinical trial subject may be provided with such devices when starting a clinical trial. The patient or subject's contact information, including without limitation cell phone, email address, text messaging address, or other means of wireless communication, may at that time be entered into the external device and associated with the patient or subject as described herein, for example, in a database. Software on the external device may include a script or other program that can detect when a signal generated from a detection device has not yet been sent to the external device, for example at a given time, and the external device can then send an alert notifying the patient to take a bodily fluid sample.

[0243] In one embodiment, the system is provided directly to a consumer and is used in lifestyle and/or athletic management. Relevant lifestyle and exercise data can be input and measurements of parameters indicative of muscle damage, anaerobic metabolism (for example, lactic acid) can be measured. In some embodiments, the system can be sufficiently small to be portable.

[0244] In another embodiment, the system is particularly suited for measurement of markers in the blood of small animals such as rats and mice that are commonly used in pre-clinical work. Such animals only have a small volume of blood and so assay systems requiring very small volumes of sample are particularly useful, especially in longitudinal studies where several samples from a single animal are needed in rapid succession. These considerations can be especially important when several analytes need to be measured in parallel.

[0245] In one embodiment, the system includes a convenient way to package the several elements required for multiple complex assays in a secure form for shipping. For example, assay elements click fit into a housing.

Assays

[0246] A variety of assays may be performed on a fluidic device according to the present invention to detect an analyte of interest in a sample. A wide diversity of labels is available in the art that can be employed for conducting the subject assays. In some embodiments labels are detectable by spectroscopic, photochemical, biochemical, electrochemical, immunochemical, or other chemical means. For example, useful nucleic acid labels include the radioisotopes ³²P, ³⁵S, fluorescent dyes, electron-dense reagents, enzymes, etc. A wide variety of labels suitable for labeling biological components are known and are reported extensively in both the scientific and patent literature, and are generally applicable to the present invention for the labeling of biological components. Suitable labels include radionucleotides, enzymes, substrates, cofactors, inhibitors, fluorescent moieties, chemiluminescent moieties, bioluminescent labels, or colorimetric labels. Reagents defining assay specificity optionally include, for example, monoclonal antibodies, polyclonal antibodies, pro-

teins, nucleic acid probes or other polymers such as affinity matrices, carbohydrates or lipids. Detection can proceed by any of a variety of known methods, including spectrophotometric or optical tracking of radioactive, fluorescent, or luminescent markers, or other methods which track a molecule based upon size, charge or affinity. A detectable moiety can be of any material having a detectable physical or chemical property. Such detectable labels have been well-

[0247] In some embodiments the label is coupled directly or indirectly to a molecule to be detected such as a product, substrate, or enzyme, according to methods well known in the art. As indicated above, a wide variety of labels are used, with the choice of label depending on the sensitivity required, ease of conjugation of the compound, stability requirements, available instrumentation, and disposal provisions. Non-radioactive labels are often attached by indirect means. Generally, a receptor specific to the analyte is linked to a signal generating moiety. Sometimes The analyte receptor is linked to an adaptor molecule (such as biotin or avidin) and the assay reagent set includes a binding moiety (such as a biotinylated reagent or avidin) that binds to the adaptor and to the analyte. The analyte binds to a specific receptor on the reaction site. A labeled reagent can form a sandwich complex in which the analyte is in the center. The reagent can also compete with the analyte for receptors on the reaction site or bind to vacant receptors on the reaction site not occupied by analyte. The label is either inherently detectable or bound to a signal system, such as a detectable enzyme, a fluorescent compound, a chemiluminescent compound, or a chemiluminogenic entity such as an enzyme with a luminogenic substrate. A number of ligands and anti-ligands can be used. Where a ligand has a natural anti-ligand, for example, biotin, thyroxine, digoxigenin, and cortisol, it can be used in conjunction with labeled, anti-ligands. Alternatively, any haptenic or antigenic compound can be used in combination with an antibody.

[0248] In some embodiments the label can also be conjugated directly to signal generating compounds, for example, by conjugation with an enzyme or fluorophore. Enzymes of interest as labels will primarily be hydrolases, particularly phosphatases, esterases and glycosidases, or oxidoreductases, particularly peroxidases. Fluorescent compounds include fluorescein and its derivatives, rhodamine and its derivatives, dansyl groups, and umbelliferone. Chemiluminescent compounds include dioxetanes, acridinium esters, luciferin, and 2,3-dihydrophthalazinediones, such as luminol.

[0249] Methods of detecting labels are well known to those of skilled in the art. Thus, for example, where the label is radioactive, means for detection include scintillation counting or photographic films as in autoradiography. Where the label is fluorescent, it may be detected by exciting the fluorochrome with light of an appropriate wavelength and detecting the resulting fluorescence by, for example, microscopy, visual inspection, via photographic film, by the use of electronic detectors such as digital cameras, charge coupled devices (CCDs) or photomultipliers and phototubes, or other detection device. Similarly, enzymatic labels are detected by providing appropriate substrates for the enzyme and detecting the resulting reaction product. Finally, simple colorimetric labels are often detected simply by observing the color associated with the label. For example, conjugated gold often appears pink, while various conjugated beads appear the color of the bead.

[0250] In some embodiments the detectable signal may be provided by luminescence sources. Luminescence is the term commonly used to refer to the emission of light from a substance for any reason other than a rise in its temperature. In general, atoms or molecules emit photons of electromagnetic energy (e.g., light) when then move from an excited state to a lower energy state (usually the ground state). If exciting cause is a photon, the luminescence process is referred to as photoluminescence. If the exciting cause is an electron, the luminescence process can be referred to as electroluminescence. More specifically, electroluminescence results from the direct injection and removal of electrons to form an electron-hole pair, and subsequent recombination of the electron-hole pair to emit a photon. Luminescence which results from a chemical reaction is usually referred to as chemiluminescence. Luminescence produced by a living organism is usually referred to as bioluminescence. If photoluminescence is the result of a spin-allowed transition (e.g., a single-singlet transition, triplet-triplet transition), the photoluminescence process is usually referred to as fluorescence. Typically, fluorescence emissions do not persist after the exciting cause is removed as a result of short-lived excited states which may rapidly relax through such spin-allowed transitions. If photoluminescence is the result of a spin-forbidden transition (e.g., a triplet-singlet transition), the photoluminescence process is usually referred to as phosphorescence. Typically, phosphorescence emissions persist long after the exciting cause is removed as a result of long-lived excited states which may relax only through such spin-forbidden transitions. A luminescent label may have any one of the above-described properties.

[0251] Suitable chemiluminescent sources include a compound which becomes electronically excited by a chemical reaction and may then emit light which serves as the detectible signal or donates energy to a fluorescent acceptor. A diverse number of families of compounds have been found to provide chemiluminescence under a variety of conditions. One family of compounds is 2,3-dihydro-1,4-phthalazinedione. A frequently used compound is luminol, which is a 5-amino compound. Other members of the family include the 5-amino-6,7,8-trimethoxy- and the dimethylamino[ca]benz analog. These compounds can be made to luminesce with alkaline hydrogen peroxide or calcium hypochlorite and base.

Another family of compounds is the 2,4,5-triphenylimidazoles, with lophine as the common name for the parent product. Chemiluminescent analogs include para-dimethylamino and -methoxy substituents. Chemiluminescence may also be obtained with oxalates, usually oxalyl active esters, for example, p-nitrophenyl and a peroxide such as hydrogen peroxide, under basic conditions. Other useful chemiluminescent compounds that are also known include -N-alkyl acridinum esters and dioxetanes. Alternatively, luciferins may be used in conjunction with luciferase or lucigenins to provide bioluminescence.

[0252] The term analytes as used herein includes without limitation drugs, prodrugs, pharmaceutical agents, drug metabolites, biomarkers such as expressed proteins and cell markers, antibodies, serum proteins, cholesterol and other metabolites, polysaccharides, nucleic acids, biological analytes, biomarkers, genes, proteins, or hormones, or any combination thereof. Analytes can be combinations of polypeptides, glycoproteins, polysaccharides, lipids, and nucleic acids.

[0253] Of particular interest are biomarkers are associated with a particular disease or with a specific disease stage. Such analytes include but are not limited to those associated with autoimmune diseases, obesity, hypertension, diabetes, neuronal and/or muscular degenerative diseases, cardiac diseases, endocrine disorders, metabolic disorders, inflammation, cardiovascular diseases, sepsis, angiogenesis, cancers, Alzheimer's disease, athletic complications, and any combinations thereof.

[0254] Of also interest are biomarkers that are present in varying abundance in one or more of the body tissues including heart, liver, prostate, lung, kidney, bone marrow, blood, skin, bladder, brain, muscles, nerves, and selected tissues that are affected by various disease, such as different types of cancer (malignant or non-metastatic), autoimmune diseases, inflammatory or degenerative diseases.

[0255] Also of interest are analytes that are indicative of a microorganism, virus, or Chlamydiaceae. Exemplary microorganisms include but are not limited to bacteria, viruses, fungi and protozoa. Analytes that can be detected by the subject method also include blood-born pathogens selected from a non-limiting group that consists of *Staphylococcus epidermidis*, *Escherichia coli*, methicillin-resistant *Staphylococcus aureus* (MSRA), *Staphylococcus aureus*, *Staphylococcus hominis*, *Enterococcus faecalis*, *Pseudomonas aeruginosa*, *Staphylococcus capitis*, *Staphylococcus warneri*, *Klebsiella pneumoniae*, *Haemophilus influenzae*, *Staphylococcus simulans*, *Streptococcus pneumoniae* and *Candida albicans*.

[0256] Analytes that can be detected by the subject method also encompass a variety of sexually transmitted diseases selected from the following: gonorrhea (*Neisseria gonorrhoeae*), syphilis (*Treponema pallidum*), chlamydia (*Chlamydia trachomatis*), nongonococcal urethritis (*Ureaplasma urealyticum*), yeast infection (*Candida albicans*), chancroid (*Haemophilus ducreyi*), trichomoniasis (*Trichomonas vaginalis*), genital herpes (HSV type I & II), HIV I, HIV II and hepatitis A, B, C, G, as well as hepatitis caused by TTV.

[0257] Additional analytes that can be detected by the subject methods encompass a diversity of respiratory pathogens including but not limited to *Pseudomonas aeruginosa*, methicillin-resistant *Staphylococcus aureus* (MSRA), *Klebsiella pneumoniae*, *Haemophilus influenzae*, *Staphylococcus aureus*, *Stenotrophomonas maltophilia*, *Haemophilus parainfluenzae*, *Escherichia coli*, *Enterococcus faecalis*, *Serratia marcescens*, *Haemophilus parahaemolyticus*, *Enterococcus cloacae*, *Candida albicans*, *Moraxiella catarrhalis*, *Streptococcus pneumoniae*, *Citrobacter freundii*, *Enterococcus faecium*, *Klebsella oxytoca*, *Pseudomonas fluorescens*, *Neisseria meningitidis*, *Streptococcus pyogenes*, *Pneumocystis carinii*, *Klebsella pneumoniae*, *Legionella pneumophila*, *Mycoplasma pneumoniae*, and *Mycobacterium tuberculosis*.

[0258] Listed below are additional exemplary markers according to the present invention: Theophylline, CRP, CKMB, PSA, Myoglobin, CA125, Progesterone, TxB2, 6-keto-PGF-1- α , and Theophylline, Estradiol, Lutenizing hormone, Triglycerides, Tryptase, Low density lipoprotein Cholesterol, High density lipoprotein Cholesterol, Cholesterol, IGFR.

[0259] Exemplary liver markers include without limitation LDH, (LD5), (ALT), Arginase 1 (liver type), Alpha-fetoprotein (AFP), Alkaline phosphatase, Alanine aminotransferase, Lactate dehydrogenase, and Bilirubin. [00260] Exemplary kidney markers include without limitation TNF α Receptor, Cystatin C, Lipocalin-type urinary prostaglandin D, synthetase (LPGDS), Hepatocyte growth factor receptor, Polycystin 2, Polycystin 1, Fibrocystin, Uromodulin, Alanine, aminopeptidase, N-acetyl-B-D-glucosaminidase, Albumin, and Retinol-binding protein (RBP).

[0260] Exemplary heart markers include without limitation Troponin I (TnI), Troponin T (TnT), CK, CKMB, Myoglobin, Fatty acid binding protein (FABP), CRP, D-dimer, S-100 protein, BNP, NT-proBNP, PAPP-A, Myeloperoxidase (MPO), Glycogen phosphorylase isoenzyme BB (GPBB), Thrombin Activatable Fibrinolysis Inhibitor (TAFI), Fibrinogen, Ischemia modified albumin (IMA), Cardiotrophin-1, and MLC-I (Myosin Light Chain-I).

[0261] Exemplary pancreas markers include without limitation Amylase, Pancreatitis-Associated protein (PAP-1), and Regeneratin proteins (REG).

[0262] Exemplary muscle tissue markers include without limitation Myostatin.

[0263] Exemplary blood markers include without limitation Erythropoietin (EPO).

[0264] Exemplary bone markers include without limitation, Cross-linked N-telopeptides of bone type I collagen (NTx) Carboxyterminal cross-linking telopeptide of bone collagen, Lysyl-pyridinoline (deoxypyridinoline), Pyridinoline, Tartrate-resistant acid phosphatase, Procollagen type I C propeptide, Procollagen type I N propeptide, Osteocalcin (bone gla-protein), Alkaline phosphatase, Cathepsin K, COMP (Cartilage Oligimeric Matrix Protein), Osteocrin Osteoprotegerin

(OPG), RANKL, sRANK, TRAP 5 (TRACP 5), Osteoblast Specific Factor 1 (OSF-1, Pleiotrophin), Soluble cell adhesion molecules, sTfR, sCD4, sCD8, sCD44, and Osteoblast Specific Factor 2 (OSF-2, Periostin).

[0265] In some embodiments markers according to the present invention are disease specific. Exemplary cancer markers include without limitation PSA (total prostate specific antigen), Creatinine, Prostatic acid phosphatase, PSA complexes, Prostate-specific gene-1, CA 12-5, Carcinoembryonic Antigen (CEA), Alpha fetoprotein (AFP), hCG (Human chorionic gonadotropin), Inhibin, CAA Ovarian C1824, CA 27.29, CA 15-3, CAA Breast C1924, Her-2, Pancreatic, CA 19-9, Carcinoembryonic Antigen, CAA pancreatic, Neuron-specific enolase, Angiostatin DcR3 (Soluble decoy receptor 3), Endostatin, Ep-CAM (MK-1), Free Immunoglobulin Light Chain Kappa, Free Immunoglobulin Light Chain Lambda, Herstatin, Chromogranin A, Adrenomedullin, Integrin, Epidermal growth factor receptor, Epidermal growth factor receptor-Tyrosine kinase, Pro-adrenomedullin N-terminal 20 peptide, Vascular endothelial growth factor, Vascular endothelial growth factor receptor, Stem cell factor receptor, c-kit/KDR, KDR, and Midkine.

[0266] Exemplary infectious disease conditions include without limitation: Viremia, Bacteremia, Sepsis, and markers: PMN Elastase, PMN elastase/ al-PI complex, Surfactant Protein D (SP-D), HBVc antigen, HBVs antigen, Anti-HBVc, Anti-HIV, T-suppressor cell antigen, T-cell antigen ratio, T-helper cell antigen, Anti-HCV, Pyrogens, p24 antigen, Muramyl-dipeptide.

[0267] Exemplary diabetes markers include without limitation C-Peptide, Hemoglobin Alc, Glycated albumin, Advanced glycosylation end products (AGEs), 1,5-anhydroglucitol, Gastric Inhibitory Polypeptide, Glucose, Hemoglobin, ANGPTL3 and 4.

[0268] Exemplary inflammation markers include without limitation Rheumatoid factor (RF), Antinuclear Antibody (ANA), C-reactive protein (CRP), Clara Cell Protein (Uteroglobin).

[0269] Exemplary allergy markers include without limitation Total IgE and Specific IgE.

[0270] Exemplary autism markers include without limitation Ceruloplasmin, Metallothioneine, Zinc, Copper, B6, B12, Glutathione, Alkaline phosphatase, and Activation of apo-alkaline phosphatase.

[0271] Exemplary coagulation disorders markers include without limitation b-Thromboglobulin, Platelet factor 4, Von Willebrand factor.

[0272] In some embodiments a marker may be therapy specific. COX inhibitors include without limitation TxB2 (Cox-1), 6-keto-PGF-1-alpha (Cox 2), 11-Dehydro-TxB-1a (Cox-1).

[0273] Other markers of the present include without limitation Leptin, Leptin receptor, and Procalcitonin, Brain S100 protein, Substance P, 8-Iso-PGF-2a.

[0274] Exemplary geriatric markers include without limitation, Neuron-specific enolase, GFAP, and S100B.

[0275] Exemplary markers of nutritional status include without limitation Prealbumin, Albumin, Retinol-binding protein (RBP), Transferrin, Acylation-Stimulating Protein (ASP), Adiponectin, Agouti-Related Protein (AgRP), Angiopoietin-like Protein 4 (ANGPTL4, FIAF), C-peptide, AFABP (Adipocyte Fatty Acid Binding Protein, FABP4)

Acylation-Stimulating Protein (ASP), EFABP (Epidermal Fatty Acid Binding Protein, FABP5), Glicentin, Glucagon, Glucagon-Like Peptide-1, Glucagon-Like Peptide-2, Ghrelin, Insulin, Leptin, Leptin Receptor, PYY, RELMs, Resistin, and sTfR (soluble Transferrin Receptor).

[0276] Exemplary markers of Lipid metabolism include without limitation Apo-lipoproteins (several), Apo-A1, Apo-B, Apo-C-II, Apo-D, Apo-E.

[0277] Exemplary coagulation status markers include without limitation Factor I: Fibrinogen, Factor II: Prothrombin, Factor III: Tissue factor, Factor IV: Calcium, Factor V: Proaccelerin, Factor VI, Factor VII: Proconvertin, Factor VIII: Anti-hemolytic factor, Factor IX: Christmas factor, Factor X: Stuart-Prower factor, Factor XI: Plasma thromboplastin antecedent, Factor XII: Hageman factor, Factor XIII: Fibrin-stabilizing factor, Prekallikrein, High-molecular-weight kininogen, Protein C, Protein S, D-dimer, Tissue plasminogen activator, Plasminogen, a2-Antiplasmin, Plasminogen activator inhibitor 1 (PAI1).

[0278] Exemplary monoclonal antibodies include those for EGFR, ErbB2, and IGF1R.

[0279] Exemplary tyrosine kinase inhibitors include without limitation Ab1, Kit, PDGFR, Src, ErbB2, ErbB 4, EGFR, EphB, VEGFR1-4, PDGFRb, FLT3, FGFR, PKC, Met, Tie2, RAF, and TrkA.

[0280] Exemplary Serine/Threonine Kinase Inhibitors include without limitation AKT, Aurora A/B/B, CDK, CDK (pan), CDK1-2, VEGFR2, PDGFRb, CDK4/6, MEK1-2, mTOR, and PKC-beta.

[0281] GPCR targets include without limitation Histamine Receptors, Serotonin Receptors, Angiotensin Receptors, Adrenoreceptors, Muscarinic Acetylcholine Receptors, GnRH Receptors, Dopamine Receptors, Prostaglandin Receptors, and ADP Receptors.

[0282] Described herein is a method of monitoring more than one pharmacological parameter useful for assessing efficacy and/or toxicity of a therapeutic agent. For example, a therapeutic agent can include any substances that have therapeutic utility and/or potential. Such substances include but are not limited to biological or chemical compounds such as simple or complex organic or inorganic molecules, peptides, proteins

(e.g. antibodies) or a polynucleotides (e.g. anti-sense). A vast array of compounds can be synthesized, for example polymers, such as polypeptides and polynucleotides, and synthetic organic compounds based on various core structures,

and these can also be included as therapeutic agents. In addition, various natural sources can provide compounds for screening, such as plant or animal extracts, and the like. It should be understood, although not always explicitly stated that the agent is used alone or in combination with another agent, having the same or different biological activity as the agents identified by the inventive screen. The agents and methods also are intended to be combined with other therapies.

For example, small molecule drugs are often measured by mass-spectrometry which can be imprecise. ELISA (antibody-based) assays can be much more accurate and precise.

[0283] Physiological parameters include without limitation parameters such as temperature, heart rate/pulse, blood pressure, and respiratory rate. Pharmacodynamic parameters include concentrations of biomarkers such as proteins, nucleic acids, cells, and cell markers. Biomarkers could be indicative of disease or could be a result of the action of a drug. Pharmacokinetic (PK) parameters include without limitation drug and drug metabolite concentration. Identifying and quantifying the PK parameters in real time from a sample volume is extremely desirable for proper safety and efficacy of drugs. If the drug and metabolite concentrations are outside a desired range and/or unexpected metabolites are generated due to an unexpected reaction to the drug, immediate action may be necessary to ensure the safety of the patient. Similarly, if any of the pharmacodynamic (PD) parameters fall outside the desired range during a treatment regime, immediate action may have to be taken as well.

[0284] Being able to monitor the rate of change of an analyte concentration or PD or PK parameters over a period of time in a single subject, or performing trend analysis on the concentration, PD, or PK parameters, whether they are concentrations of drugs or their metabolites, can help prevent potentially dangerous situations. For example, if glucose were the analyte of interest, the concentration of glucose in a sample at a given time as well as the rate of change of the glucose concentration over a given period of time could be highly useful in predicting and avoiding, for example, hypoglycemic events. Such trend analysis has widespread beneficial implications in drug dosing regimen. When multiple drugs and their metabolites are concerned, the ability to spot a trend and take proactive measures is often desirable.

[0285] Described herein is a business method of assisting a clinician in providing an individualized medical treatment. A business method can comprise post prescription monitoring of drug therapy by monitoring trends in biomarkers over time. The business method can comprise collecting at least one pharmacological parameter from an individual receiving a medication, said collecting step is effected by subjecting a sample of bodily fluid to reactants contained in a fluidic device, which is provided to said individual to yield a detectable signal indicative of said at least one pharmacological parameter; and cross referencing with the aid of a computer medical records of said individual with the at least one pharmacological parameter of said individual, thereby assisting said clinician in providing individualized medical treatment.

[0286] The devices, systems, and methods herein allow for automatic quantification of a pharmacological parameter of a patient as well as automatic comparison of the parameter with, for example, the patient's medical records which may include a history of the monitored parameter, or medical records of another group of subjects. Coupling real-time analyte monitoring with an external device which can store data as well as perform any type of data processing or algorithm, for example, provides a device that can assist with typical patient care which can include, for example, comparing current patient data with past patient data. Therefore, also described herein is a business method which effectively performs at least part of the monitoring of a patient that is currently performed by medical personnel.

EXAMPLE 1

[0287] In this example, a device, method, and system of the invention are used to perform an assay for human VEGFR2. The example demonstrates a type of assay that can be performed at the point of care. The capture surface of an assay unit can be coated onto the assay unit according to the assay, this example a VEGFR2 assay. The inner surface of the assay unit (made from injection molded polystyrene similar to example in Figure 3A) was exposed to a succession of coating reagents by aspiration and pneumatic ejection. Twenty microliters of each coating reagents were drawn into assay units and incubated at room temperature for 10 minutes. The coating reagents used in this example are, as used in succession, Neutravidin (20ug/mL) in Carbonate-Bicarbonate buffer (pH 9), biotinylated "Capture antibody" (a monoclonal antibody directed to VEGFR2 at 20ug/mL) in Tris buffered saline, (pH 8), and a "fixative" reagent containing 3% bovine serum albumin in Tris-buffered saline. After the succession of coatings, the assay units were dried by exposure to dry air and stored desiccated.

[0288] Samples for analysis are then distributed to the assay unit diluted in a solution of 50 mM tris-buffer (pH 8) containing bovine serum albumin and isotonic sucrose for 20 minutes. In a reagent unit comprising a conjugate, a solution of Alkaline phosphatase (bovine intestine)-labeled monoclonal antibody directed to VEGFR2 (binding to a distinct epitope to the antibody of the capture surface) at 250 ng/mL in a stabilizer reagent from Biostab is provided to the assay unit for 10 minutes. After the conjugate has been allowed to bind with the complex of the analyte bound to the capture surface, the assay unit was washed with a solution contained in a reagent unit (commercially available wash buffer from Assay Designs). The assay unit was washed 5 times. Then the assay unit was moved to collect and mix with another reagent contained in a different reagent, a solution of a commercially available luminogenic substrate for alkaline phosphatase

(KPL Phosphaglo), and incubated for 10 minutes. The reaction of the assay in the assay unit was then detected by a detector assembly of the invention.

[0289] Figure 12 demonstrates the VEGFR2 assay response using the method of the example. The x axis scale is VEGFR2 concentration (pg/mL); the y scale is relative luminescence (counts). The curve was used to calibrate the modular assay unit and reagent units.

EXAMPLE 2

[0290] An assay for human PIGF was performed using the assay units and reagent units of the invention and read in a commercial instrument. In parallel, an assay using the same reagents was done in prototype disposable cartridges (as described below) in a prototype reader. Analyte concentrations were 0, 4, 80 and 400 pg/mL respectively. The measurements illustrated in Figure 13 were used to calibrate an assay unit and reagent unit necessary for conducting an assay for human PIGF.

EXAMPLE 3

[0291] Magnetizable beads are 1.3 um diameter BioMag magnetic particles from Bangs Laboratories. Beads are coated (by the manufacturer) with anti-Rabbit IgG. Beads are dispersed at 14 mg/mL in tris-buffered sucrose (or, alternatively, tris buffered saline) containing 3% bovine serum albumin and rabbit anti-human red blood cell IgG, from CedarLane at ≥ 1.15 mg/mL. Aliquots (10 uL of this dispersion were dispensed into conical tubes and lyophilized (frozen in liquid N₂ and lyophilized for approximately 24 hrs. at -70°C) prior to insertion into a slot in the cartridge housing. The rabbit antibody binds both to the red cells and to the anti-rabbit IgG-coated beads and forms a co-agglutinate of beads and red cells.

[0292] The lyophilized magnetizable bead pellet was re-suspended by adding 20 uL of whole blood then aspirating and dispensing at least 8 times (approximately 1.5 min) into a conical tube.

[0293] Blood was separated by placing the tip (in a vertical orientation) in a strong, horizontally oriented magnetic field. Typically 8 uL of essentially red cell free plasma with no observable hemolysis was recovered from a 20 ul blood sample (70% yield). Recovery of analytes (compared to plasma not exposed to the magnetic separation) was close to 100% for Protein-C, VEGF, PIGF, Insulin, GIP and GIP-1.

EXAMPLE 4

[0294] Serial dilution of a sample for analyses of an analyte can be carried out in a system as described herein. C-reactive protein (CRP) is an acute-phase marker. Normal levels are in the high ng/mL to low ug/ml range. In any acute disease process, the human liver produces CRP and levels in blood can increase to hundreds of ug/ml. CRP has presented issues for prior art POC analytic systems because of the wide dynamic range of analyte to be measured ($> 10^5$ -fold).

[0295] A system as described herein comprising a fluid transfer device and a cartridge or device with arrays of assay and reagent units was developed. Assay tips having monoclonal anti-CRP bound to their inner surface were mounted in cartridge together with a detector-antibody solution (alkaline-phosphatase labeled monoclonal anti-CRP (having a different epitope specificity than that on the tips), a wash solution and a chemiluminogenic alkaline phosphatase (PhosphaGLOTM) substrate from KPL.

[0296] To assay CRP, the cartridges were loaded with pre-diluted solutions of CRP used without further dilution. The cartridges were processed by a system. Successively the CRP solution (10 uL), detector antibody (12 uL) were drawn into the tips incubated for 10 min at 34 °C then discarded. The tips were washed by four aspirations of 20 uL wash solution before 15 uL of substrate was aspirated into the tips. After 10 min at 37 °C, light emission was measured by the instrument for 5 s. CRP concentration was plotted against the assay signal (photon counts) and the data fitted to a 5-term polynomial function as shown below to generate a calibration function as shown in Figure 14.

EXAMPLE 5

[0297] An experiment was then executed using serial dilutions of a sample containing highly concentrated analyte to obtain an unambiguous assay response in a system and device as described herein. Solutions of CRP (20 uL) were loaded into cartridges and serially diluted by the instrument (to dilutions of 1: 50, 250, 750 and 1500-fold respectively). The diluted solutions were then processed as in Example 4. When the diluted CRP concentration exceeded the calibration range of the assay (300 ng/mL), a downward response was seen (as shown below; data from two instruments).

[0298] The response as shown in Figure 15 can be modeled using a modification of the Scatchard binding isotherm ($S/S_{\max} = C/(C + C_{0.5})$). The modification assumes that the response of the assay is linearly proportional to the con-

centration of the detector antibody, as is the case in this example (data not shown). Any carry-over of CRP in the diluted sample into the next reagent (detector antibody) will react rapidly with the reagent rendering it incapable of binding to antigen bound to the solid phase antibody. The reduction in effective concentration is reduced in proportion to the CRP carried-over and can be accounted for with a factor $(D - C*f)/D$.

[0299] Therefore, $S = S_{max} * (C / (C + C_{0.5})) * (D - C*f) / D$, wherein S is the assay signal, S_{max} is the maximum signal (corresponding to zero carry-over), C is the concentration of analyte, $C_{0.5}$ is the concentration for half-maximal signal (no carry-over), D is the detector antibody concentration, and f is the fractional carryover.

[0300] Values used to fit the data, were derived by optimizing each of the four parameters below using the technique of minimization of least square differences between the data and the model fit. As can be seen in Figure 15, an excellent fit was achieved and the values of the parameters S_{max} , $C_{0.5}$ and D (see table 2) are close to the values that can be estimated from the maximum signal reached, the observed $C_{0.5}$ and the known detector antibody concentration. This model estimated the extent of carry-over as 0.034% (decimal 3.83E-04).

Table 1: Best fit parameters to model describing biphasic CRP assay response

Parameter	Value	Units
S_{max}	7.24E+05	Counts
$C_{0.5}$	5.02E+01	ng/mL
D	5.72E+00	ng/mL
f	3.83E-04	

[0301] Data can be then be viewed according to the dilution used to achieve the final concentration in each assay tip, and for each dilution level the responses fit to the same response showing that the dilutions are accurate and precise as shown in Figure 16.

[0302] The model as described herein can be used to compute responses for any given dilution and set up algorithms to ensure that the analyte concentration in any tip within the calibration range. Graphic means of representing the data are shown in Figure 17, wherein the normalized assay response (B/B_{max}) is plotted against the log normalized concentration ($C/C_{0.5}$) for relative dilutions: 1:1 (solid line), 5:1 (dashed line), and 25:1 (dotted line). Figures 18 and 19 illustrate a similar example as Figure 17 at different normalized concentrations. Simple pattern recognition algorithms can be used to identify valid data for high concentration samples. For example, for most of the dose-response, the signal decreases with dilution. When signal for any dilution equal or exceed that of the next higher dilution, the lower dilution result is rejected. In another example, concentrations derived by using the calibration function shown in Example 4, should correspond within some system imprecision with the known dilutions. If the calculated concentration for a low dilution is lower than would correspond with those for higher dilutions, the lower dilution result can be rejected.

[0303] When the assay dose-response approaches a maximum, the slope of the concentration ($\Delta C / \Delta S$) versus signal increases. For assays in which the relative variation in signal ($\Delta S / S$) is essentially constant (for example some instances of the system as described) this translates to a bigger variation in the calculated concentration result at higher concentrations. As provided herein, dilution or serial dilution can provide a concentration precision as achieved by immunoassays at signal levels significantly greater (for example, > 10-fold) higher than the blank (zero analyte) signal but not close to the maximum signal (for example < 0.3*Max. signal). Serial dilution can allow the assay signal to be in this range.

[0304] By making several estimates of the analyte concentration from different dilutions, an average value can be obtained. An average value can also be achieved by making replicate measurements at a single dilution level. In some instances, a serial dilution approach as offered by the methods, systems, and device described herein can often eliminate errors due to non-linearity of dilution due to (for example) matrix effects from the sample.

EXAMPLE 6

[0305] Fluorescein is a well-known chemical and high affinity antibodies are known which are specific for the molecule. By attaching several fluorescein moieties to a protein such as albumin, an artificial analyte is created that can be measured by ELISA. The example herein is set up on a microtiter plate to show the feasibility of such an assay and is easily translatable to a device or system of the invention as described herien.

[0306] Anti-fluorescein monoclonal antibody was attached to wells of 384-well microtiter plates to create a capture surface. An assay is performed by adding a series of solutions to the wells and incubating at room temperature for 10 min at each stage when necessary. 30 ul of known concentrations of a commercially available preparation of fluorescein-labeled bovine albumin (sample) with a ratio of about five fluoresceins per molecule were added to the wells. After mechanical removal of the sample, 30 ul of alkaline phosphatase-labeled anti-fluorescein (detector antibody) was added

at a concentration of 100 ng/ml. After removal of the detector antibody, the wells were washed three times 40 μ l of wash solution ("Wash Buffer" Cat# 80-1351 [Assay Designs, Ann Arbor, Michigan] diluted 1:20 before use). PhosphaGLO™ (40 μ L) substrate was then added and the assay response was then read in an M5 spectro-luminometer for 0.5 s. The assay response is shown in Figure 20.

[0307] Fluorescein-labeled albumin (5 μ L at various concentrations up to 80 ng/mL) dissolved in Tris-buffered saline containing bovine albumin at 3 mg/mL (buffer) was placed in polypropylene tubes and dried by exposure to low humidity air overnight. Complete drying was verified by weighing many tubes before and after drying and verifying the appropriate weight loss and a near-constant final weight was achieved. The analyte was recovered by adding 5 μ L water, 20 μ L human serum and 180 μ L buffer and mixing. Control experiments were made by mixing 5 μ L aliquots of analyte solution with 20 μ L serum and 180 μ L buffer.

[0308] Analyte recovery was measured using the assay as described herein. As shown below, the recovery of assay signal (and analyte) is essentially quantitative at all concentrations. It can be desirable to have good recovery (>90%), which is precise (<2% CV in recovery). In some instances, the assay dose-response is linear over the range of interest by having a low concentration of analyte and excess of the reagents. For example, a linear assay dose-response can be achieved by having sufficient capacity for antigen binding on the capture surface such that even at the highest level of analyte only a moderate proportion (for example, < 30%) of sites are occupied at the end of the binding reaction. As described herein, for analytes in the ng/mL range and assays with short incubation times (< say 30 m) this condition is achieved with capture surfaces coated as described previously. In another example, sufficient concentration of detector antibody such that the concentration is not significantly depleted during the detector antibody incubation (for example, < 30% of the reagent binds to the surface at the highest antigen levels), and this condition can be satisfied by use of detector antibody concentrations in about 5 to 100 ng/mL. In yet another example, a linear assay dose-response can be achieved by having development of a signal less than the linear response of the detector (for example, a PMT with up to about 4 million photons per second). As described herein, systems and methods can fall within this range. In yet another example, a linear assay dose-response can be achieved by development of a signal sufficiently high as to be precisely measured (for example, photon count rates greater than about 1,000 per second).

[0309] Assay tips (as described herein) were coated by aspiration of the following succession of reagents: 20 μ L 5 μ g/mL Rabbit anti-fluorescein (Molecular Probes # A6413) in carbonate buffer pH 9, 20 μ L 3% bovine albumin in tris-buffered saline pH 8, and 20 μ L 2.5 μ g/mL bovine albumin labeled with fluorescein (Sigma-Aldrich A9771), each followed by incubation for 10 m and ejection of liquid. The tips were then washed three times by aspiration of bovine albumin in tris-buffered saline pH 8 followed by incubation 3% bovine albumin in tris-buffered saline pH 8. Tips were then dried as described herein. These tips were used to assay samples containing goat anti-fluorescein by incubation of 20 μ L aliquots of the following solutions in sequence: goat anti-fluorescein (sample) in tris-buffered saline pH 8 containing 3% BSA, alkaline phosphatase labeled Rabbit-anti-goat fluorescein at 100 ng/mL in Stabilzyme™ (a commercially available solvent), washing four times with Wash Buffer, and PhosphaGLO™ alkaline phosphatase chemiluminogenic substrate, each with an incubation at room temperature for 10 min. The assay was evaluated by measuring photons produced over about 10s in the instrument using a photomultiplier tube in Molecular Devices M5 luminometer by placing each tip in a custom-modified frame which fits the instrument microtiter plate stage and the results are demonstrated in Figure 21. In this example, Figure 21 shows a linear response similar to that in Figure 20.

Table 2: Configurations of assays for candidate control analytes

Capture surface reagent 1	Capture surface reagent 2	Analyte	Detector: APase-labeled
Anti-fluorescein		Fluorescein-labeled albumin	Anti-fluorescein
Anti-fluorescein	Fluorescein-labeled albumin	Anti-fluorescein (species X)	Anti X-Ig
Avidin		Biotinylated-species X-IgG	Anti X-Ig
Anti-biotin	Biotin-labeled albumin		Anti-biotin or Streptavidin
Anti-digoxin	Digoxin-labeled albumin		Anti-digoxin
Fluorescein-labeled albumin		Anti-fluorescein (species X)	Anti-X-Ig
Anti-biotin	Biotinylated anti-fluorescein	Anti-fluorescein (species X)	Anti-X-Ig

EXAMPLE 7

[0310] This example illustrates the predictability of response from an immunoassay for CRP using assay tips as described herein following initial addition of reagents, removal of the reaction product, washing the tips then reintroduction of some or all assay components. The assay sequence was: tips were incubated in prototype instruments at 34C for 10 min in succession with (1) sample (CRP 0.3, 3, 30, 150 and 300 ug/mL), diluted by the instrument 500 then 2000-fold (2) alkaline phosphatase labeled rabbit anti-goat IgG ["Dab"] (5 ng/mL) then washed three times and (3) with Phospha-GLO™ alkaline phosphatase chemiluminogenic substrate ["Substrate"]. The experiment was performed on several instruments which also read the proton production rate over 10 seconds after step 3. Final (in tip) CRP concentrations were 0.15, 0.6, 1.5, 6, 15, 60, 75, 300 and 600 ng/mL and glow levels ranged from 2,000 to 600,000 counts/0.5 sec. In some experiments, after step (3) in the assay, the reaction product was discarded and variously steps 3 (diamonds and solid line), steps 2 + 3 (squares and dashed line), or steps 1 + 2 + 3 (triangles and dotted line) were repeated and the results are presented as re-processed assay signal versus original assay signal as shown in Figure 22.

[0311] The re-processed assay signals were linearly related (proportional) to the original assay signal. The second substrate addition gave a higher signal relative to the original whereas reprocessed assays in which Dab and substrate were both introduced or those where sample, Dab and substrate were all reintroduced gave lower signals than the original. In an example using this method, all steps in an assay sequence can be examined for quality control to understand if they went as expected according to the expected relationship between the first and subsequent iterations of assay steps.

[0312] For example as described herein, if an assay step has not happened properly, then the assay result can either be rejected as incorrect or the later iterations of the assay result can be used as the appropriate assay response.

[0313] An immunoassay for C-reactive protein was performed in a system as described herein. Six equivalent assay tips were incubated in succession with sample (200 ng/mL CRP), alkaline phosphatase labeled rabbit anti-goat IgG then washed and incubated with PhosphaGLO™ alkaline phosphatase chemiluminogenic substrate. Incubations were for 10 min at 34C. The experiment was performed on three instruments which also read the proton production rate over 10 seconds. On average about 40,000 counts (photons) per 0.5 second read time were detected. In this example, the glow level on tips one and two on instrument three gave clearly different results as shown in Table 3. The instrument was then used to wash the tips and to introduce fresh PhosphaGLO™ substrate (aspiration 2). Results are presented as ratios of glow rate for each tip to the average for the six tips on each respective instrument. After the second aspiration, tips one and two gave results in line with the other four in instrument three indicating that whatever problem had been responsible for low signal in tips one and two had been rectified.

Table 3: Recovery of appropriate signal from malfunctioning tips

	Signal, Ratio to average			
Instrument #	1	2	3	3
Aspiration #	1	1	1	2
Tip #				
1	1.002	0.988	0.460	1.043
2	0.848	1.045	0.917	0.929
3	0.959	0.893	1.141	1.035
4	1.062	1.067	1.103	1.028
5	1.049	0.981	1.171	1.022
6	1.079	1.025	1.207	0.942
CV, %	8.6	6.2	28.3	5.0

Claims

1. A cartridge for automated detection of an analyte in a bodily fluid sample comprising:

an array of addressable assay units configured to run a chemical reaction that yields a detectable signal indicative of the presence or absence of the analyte; and
an array of addressable reagent units, wherein an individual addressable reagent unit of the array is addressed

to correspond to an individual addressable assay unit of the array of assay units, wherein the individual reagent unit is configured to be calibrated in reference to the corresponding individual assay unit before the arrays are assembled on the cartridge, and wherein the individual assay unit of the array of addressable assay units and the individual reagent unit of the array of addressable reagent units are configured to be movable into fluid communication such that reagents for running the chemical reaction are brought to contact with the portion of the sample in the assay unit.

2. The cartridge of claim 1 wherein:

- (a) the individual reagent unit is configured to receive a movable assay unit;
- (b) the individual assay unit comprises an assay tip;
- (c) the individual assay unit is configured to run an immunoassay; or
- (d) the bodily fluid sample is a blood sample.

3. The cartridge of claim 1 further comprising:

(a) a sample collection unit configured to:

- (i) receive the bodily fluid sample;
- (ii) receive a volume of the bodily fluid sample of about 50 microliters or less; or
- (iii) receive a volume of the bodily fluid sample that is a single drop of blood; or

(b) a pretreatment unit configured to retrieve a portion of the bodily fluid sample for running the chemical reaction to detect the analyte, and optionally wherein the bodily fluid sample is a whole blood sample and the portion is plasma;

4. A system for automated detection of an analyte in a bodily fluid sample comprising:

- a. a cartridge of claim 1; and
- b. a detection assembly:

- (i) for detecting the detectable signal indicative of the presence or absence of the analyte;
- (ii) configured to detect signal intensities brought within the detectable range by dilution of the bodily fluid sample;
- (iii) configured to detect signal intensities over about 1000 to about 1 million counts per second using a photomultiplier.

5. The system of claim 4 further comprising:

- (a) a programmable mechanical device configured to move the individual assay unit from a first location to a second location;
- (b) a communication assembly for transmitting a protocol based on the analyte to be detected;
- (c) a heating block configured to receive the individual assay unit; or
- (d) a magnetic block.

6. The system of claim 4 further comprising a fluid transfer device wherein the fluid transfer device:

- (a) is a pipette, and optionally wherein the pipette is an air-displacement pipette;
- (b) is automated; or
- (c) comprises a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit, and comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from a sample collection unit and the reagent from the individual reagent unit into the individual assay unit; and optionally

- (i) wherein the configuration of the processor to direct fluid transfer effects a degree of dilution of the bodily fluid sample in the array of assay units to bring signals indicative of the plurality of analytes being detected within a detectable range, such that said plurality of analytes are detectable with said system; or

(ii) wherein the fluid transfer device further comprises a motor in communication with the programmable processor.

7. The system of claim 4, wherein:

- (a) the bodily fluid sample comprises at least two analytes that are present at concentrations that differ by at least 2 orders of magnitude;
- (b) the bodily fluid sample comprises at least two analytes that are present at concentrations that differ by at least 5 orders of magnitude;
- (c) a degree of dilution of the bodily fluid sample brings the signals indicative of at least two analytes within the detectable range;
- (d) the bodily fluid sample is less than about 50 μ l;
- (e) the bodily fluid sample is a single drop of blood;
- (f) an individual head of a fluid transfer device is configured to adhere to the individual assay unit;
- (g) said individual assay unit provides an immunoassay reaction site; or
- (h) said individual assay unit is a pipette tip.

8. A method of detecting an analyte in a bodily fluid sample collected from a subject comprising:

- a. providing a bodily fluid sample to the cartridge of claim 1;
- b. allowing said sample to react within at least one assay unit; and
- c. detecting said detectable signal generated from said analyte collected in said bodily fluid sample.

9. The method of claim 8, wherein the bodily fluid sample is blood and the method further comprises retrieving plasma from the blood.

10. A system for automated detection of an analyte in a plasma portion of a whole blood sample, comprising:

- a. a cartridge of claim 1, where said cartridge is further configured to automatically receive and process the whole blood sample to yield the plasma portion, from which a detectable signal indicative of the presence or absence of the analyte of interest is generated onboard the cartridge;
- and
- b. a detection assembly for detecting the detectable signal indicative of the presence or absence of the analyte.

11. A method of on-demand assembly of a cartridge of claim 1, wherein the cartridge comprises a housing, said method comprising:

- (i) placing according to the analyte to be detected the array of addressable assay units, wherein the individual assay unit of the array is configured to run a chemical reaction that detects an analyte of interest ordered by said end user, into the housing;
- (ii) placing according to the analyte to be detected the array of reagent units, into the housing; and
- (iii) securing the arrays of (i) and (ii) within the housing of the cartridge.

12. The method of claim 11 further comprising:

- (a) selecting an analyte to be detected;
- (b) sealing the cartridge; or
- (c) labeling the cartridge with a readable label indicating the analyte to be detected, and optionally wherein the readable label is a bar code or RFID.

13. A method for automated detection of a plurality of analytes in a bodily fluid sample collected from a subject, comprising:

- a. providing the bodily fluid sample to the cartridge of claim 1;
- b. engaging the individual assay unit using a fluid transfer device;
- c. transferring the bodily fluid sample from a sample collection unit to the individual assay unit using the fluid transfer device; and
- d. transferring a reagent from the individual reagent unit to the individual assay unit, thereby reacting the reagent with the bodily fluid sample to yield the signal indicative of the individual analyte of the plurality of analytes being

detected.

14. The method of claim 13, wherein:

- (a) the fluid transfer device comprises a plurality of heads, wherein an individual head of the plurality of heads is configured to engage the individual assay unit; and wherein said fluid transfer device comprises a programmable processor configured to direct fluid transfer of the bodily fluid sample from the sample collection unit and the reagent from the individual reagent unit into the individual assay unit, optionally further comprising providing instructions to the programmable processor, optionally wherein the instructions direct the step of transferring the bodily fluid sample to the individual assay unit;
- (b) the step of transferring the bodily fluid sample effects a degree of dilution of the bodily fluid sample in the individual assay unit to bring the signal indicative the individual analyte of the plurality of analytes being detected within a detectable range;
- (c) the bodily fluid sample comprises at least two individual analytes that are present at concentrations that differ by at least 2 orders of magnitude;
- (d) the bodily fluid sample comprises at least two individual analytes that are present at concentrations that differ by at least 5 orders of magnitude;
- (e) the degree of dilution of the bodily fluid sample brings the signals indicative of the at least two individual analytes within a detectable range;
- (f) the degree of dilution of the bodily fluid sample is detected with a photomultiplier and the at least two individual analytes are in a range of about 1000 to about 1 million counts per second;
- (g) the bodily fluid sample is less than about 50 μ l;
- (h) the bodily fluid sample is a single drop of blood; or
- (i) the reagent in the individual reagent unit is an enzyme substrate for an immunoassay, optionally further comprising repeating the step of transferring the reagent from the individual reagent unit after the reaction to yield the signal indicative of the individual analyte of the plurality of analytes being detected is complete, thereby creating a second reaction to yield a second signal indicative of the individual analyte, and optionally wherein an intensity of the signal and a second intensity of the second signal indicative of the individual analyte are averaged to calculate the final intensity of the signal indicative of the individual analyte.

15. A method of measuring a volume of a sample of a biological fluid collected from a subject, comprising:

- a. reacting a known quantity of a control analyte in said sample with a reagent to yield a detectable signal indicative of the quantity of the control analyte, wherein said reacting step occurs in a cartridge of claim 1; and
- b. comparing said detectable signal with an expected detectable signal, wherein the expected signal is indicative of an expected volume of the sample, and wherein said comparison provides a measurement of said volume of said sample being measured;

optionally further comprising:

- (a) verifying the volume of said sample when the measurement of the volume of the sample is within about 50% of the expected volume of the sample;
- (b)
 - (i) reacting said sample containing a target analyte with a reagent to yield a detectable signal indicative of the target analyte; and
 - (ii) measuring the quantity of the target analyte in the sample based on of said detectable signal indicative of the target analyte and the measurement of said volume of said liquid sample; or (c)
 - (i) mixing the sample in the presence of magnetizable particles in a sample collection unit, wherein the magnetizable particles comprise an antibody capture surface for binding to non-plasma portions of the sample; and
 - (ii) applying a magnetic field above a plasma collection area to the mixed sample to effect suspension of the non-plasma portions of the sample on top of the plasma collection area, optionally wherein
 - (1) the sample is a blood sample;
 - (2) the sample collection unit is a capillary tube;
 - (2) the sample is less than about 50 microliters;

- (3) the plasma retrieved is less than about 10 microliters;
- (4) the sample is not diluted;
- (5) the mixing occurs in the presence of antibodies unbound to a solid surface;
- (6) the mixing comprises mixing by syringe action; or
- (7) the method is carried out in a system of claim 4 or 8; or

(d) transmitting result of the comparison to an end user, and optionally wherein the result is transmitted wirelessly; and optionally wherein:

- (a) the control analyte is normally not present in said sample in a detectable amount;
- (b) a liquid sample and the bodily fluid sample are the same sample;
- (c) the control analyte does not react with a target analyte in the bodily fluid sample;
- (d) a liquid sample and the bodily fluid sample are different liquid samples;
- (e) the control analyte is selected from the group consisting of: albumin, fluorescein, IgG, protein C, fluorescein-labeled albumin, fluorescein labeled IgG, anti-fluorescein, anti-digoxigenin, digoxigenin-labeled albumin, digoxigenin-labeled IgG, biotinylated proteins, and non-human IgG;
- (f) the reaction is an immunoassay;
- (g) the reaction is an ELISA; or
- (h) the method is carried out in a system of claim 4 or 8.

Patentansprüche

1. Kassette zur automatischen Erfassung eines Analyten in einer Körperflüssigkeitsprobe, welche Folgendes umfasst:

eine Anzahl von adressierbaren Assayeinheiten, die so ausgebildet sind, dass eine chemische Reaktion erfolgt, die ein feststellbares Signal erzeugt, das das Vorhandensein oder das Fehlen eines Analyten anzeigt, und eine Reihe von adressierbaren Reagenzeinheiten, wobei eine einzelne adressierbare Reagenzeinheit der Reihe so adressiert ist, dass sie einer einzelnen adressierbaren Assayeinheit der Reihe von Assayeinheiten entspricht, wobei die einzelne Reagenzeinheit so ausgebildet ist, dass sie in Bezug auf die einzelne Assayeinheit kalibrierbar ist, bevor die Reihen in der Kassette angeordnet werden, und wobei die einzelne Assayeinheit der Reihe von adressierbaren Assayeinheiten und die einzelne Reagenzeinheit der Reihe von adressierbaren Reagenzeinheiten so konfiguriert sind, dass sie in eine fließende Kommunikation bewegbar sind, derart, dass die Reagenzien zur Ausführung der chemischen Reaktion in Kontakt mit einem Teil der Probe in der Assayeinheit gebracht werden.

2. Kassette nach Anspruch 1, wobei

- (a) die einzelne Reagenzeinheit so ausgebildet ist, dass sie eine bewegliche Assayeinheit aufnimmt,
- (b) die einzelne Assayeinheit eine Assayspitze enthält,
- (c) die einzelne Assayeinheit so ausgebildet ist, dass sie ein Immunoassay ausführt, oder
- (d) die Körperflüssigkeitsprobe eine Blutprobe ist.

3. Kassette nach Anspruch 1, welche ferner umfasst:

(a) eine Probensammeleinheit, die ausgebildet ist, um

- (i) die Körperflüssigkeitsprobe aufzunehmen,
- (ii) ein Volumen der Körperflüssigkeitsprobe von etwa 50 Mikrolitern oder weniger aufzunehmen, oder
- (iii) ein Volumen der Körperflüssigkeitsprobe aufzunehmen, die ein einzelner Blutstropfen ist, oder

(b) eine Vorbehandlungseinheit, die so ausgebildet ist, dass sie einen Teil der Körperflüssigkeitsprobe zur Ausführung der chemischen Reaktion erhält, um den Analyten zu erfassen und optional, wobei die Körperflüssigkeitsprobe eine vollständige Blutprobe und der Teil Plasma ist.

4. System zur automatischen Erfassung eines Analyten in einer Körperflüssigkeitsprobe, welches Folgendes umfasst:

a. eine Kassette nach Anspruch 1, und

b. eine Erfassungsanordnung:

- (i) zur Erfassung eines feststellbaren Signals, das das Vorhandensein oder das Fehlen eines Analyten anzeigt,
- (ii) die so ausgebildet ist, dass Signalintensitäten erfasst werden, die durch Verdünnung der Körperflüssigkeitsprobe in einen erfassbaren Bereich gebracht sind,
- (iii) die so ausgebildet ist, dass sie Signalintensitäten erfasst, die über 1000 - 1 Million Zählungen pro Sekunde unter Verwendung eines Fotomultipliers liegen.

5. System nach Anspruch 4, welches ferner umfasst:

- (a) eine programmierbare mechanische Einrichtung, die so ausgebildet ist, dass sie die einzelne Assayeinheit von einer ersten Stelle zu einer zweiten Stelle bewegt,
- (b) eine Kommunikationsanordnung zur Übertragung eines Protokolls, das auf dem zu erfassenden Analyten basiert,
- (c) einen Wärmeblock, der so ausgebildet ist, dass er die einzelne Assayeinheit aufnimmt, oder
- (d) einen magnetischen Block.

6. System nach Anspruch 4, welches ferner eine Einrichtung zur Flüssigkeitsübertragung enthält, wobei die Einrichtung zur Flüssigkeitsübertragung

- (a) eine Pipette ist und optional, bei der die Pipette eine Luftverdrängungspipette ist,
- (b) automatisch arbeitet, oder
- (c) eine Mehrzahl von Köpfen enthält, wobei ein einzelner Kopf der Mehrzahl von Köpfen so ausgebildet ist, dass dieser die einzelne Assayeinheit aufnimmt und einen programmierbaren Prozessor enthält, der so ausgebildet ist, dass er einen Flüssigkeitstransfer der Körperflüssigkeitsprobe von einer Probensammeleinheit und den Reagenz von einer einzelnen Reagenzeinheit in die einzelne Assayeinheit steuert, und optional

- (i) bei der die Konfiguration des Prozessors so ausgebildet ist, dass der Flüssigkeitstransfer einen Grad der Verdünnung der Körperflüssigkeitsprobe in der Reihe von Assayeinheiten bewirkt, um Signale, die in Bezug auf die Mehrzahl von Analyten, die zu erfassen sind, indikativ sind, in einen erfassbaren Bereich zu bringen, derart, dass die Mehrzahl der Analyten mit dem System erfassbar werden, oder
- (ii) wobei die Flüssigkeitstransfereinrichtung ferner einen Motor in Kombination mit einem programmierbaren Prozessor enthält.

7. System nach Anspruch 4, wobei

- (a) die Körperflüssigkeitsprobe wenigstens zwei Analyten enthält, die in Konzentrationen vorliegen, die sich um wenigstens zwei Größenordnungen unterscheiden,
- (b) die Körperflüssigkeitsprobe wenigstens zwei Analyten enthält, die in Konzentrationen vorliegen, die sich um wenigstens fünf Größenordnungen unterscheiden,
- (c) ein Grad der Verdünnung der Körperflüssigkeitsprobe die Signale, die für die wenigstens zwei Analyten indikativ sind, in einen erfassbaren Bereich bringt,
- (d) die Körperflüssigkeitsprobe kleiner als etwa 50 Mikroliter ist,
- (e) die Körperflüssigkeitsprobe ein einzelner Blutstropfen ist,
- (f) ein einzelner Kopf einer Flüssigkeitstransfereinrichtung so konfiguriert ist, dass dieser an der einzelnen Assayeinheit anhängt,
- (g) die einzelne Assayeinheit eine Immunoassay-Reaktionsstelle hat, oder
- (h) die einzelne Assayeinheit eine Pipettenspitze ist.

8. Verfahren zur Feststellung eines Analyten in einer Körperflüssigkeitsprobe, die von einem Subjekt genommen ist, das Folgendes umfasst:

- a. Bereitstellen einer Körperflüssigkeitsprobe in einer Kassette nach Anspruch 1,
- b. Zulassen der Reaktion der Probe mit wenigstens einer Assayeinheit, und
- c. Erfassen des detektierbaren Signals, das von dem Analyten erzeugt ist, der in der Körperflüssigkeitsprobe gesammelt ist.

9. Verfahren nach Anspruch 8, wobei die Körperflüssigkeitsprobe Blut ist und das Verfahren ferner das Abtrennen von Plasma aus dem Blut umfasst.

10. System zur automatischen Erfassung eines Analyten in einem Plasmateil einer vollständigen Blutprobe, welches Folgendes umfasst:

- a. eine Kassette nach Anspruch 1, wobei die Kassette ferner so konfiguriert ist, dass sie automatisch die vollständige Blutprobe aufnimmt und verarbeitet, um den Plasmateil zu erhalten, aus dem auf der Kassette ein detektierbares Signal erzeugt wird, das für das Vorhandensein oder das Fehlen des interessierenden Analyten indikativ ist, und
- b. eine Erfassungsanordnung zur Erfassung des detektierbaren Signals, das für das Vorhandensein oder das Fehlen des Analyten in indikativ ist, vorgesehen ist.

11. Verfahren zur Erstellung einer Kassette nach Anspruch 1 nach Bedarf, wobei die Kassette ein Gehäuse aufweist, und das Verfahren Folgendes umfasst:

- (i) Anordnen der Reihe von adressierbaren Assayeinheiten gemäß dem Analyten, der zu erfassen ist, in dem Gehäuse, wobei die einzelne Assayeinheit der Reihe so konfiguriert ist, dass eine chemische Reaktion erzeugt wird, die einen interessierenden Analyten erfasst, der vom Endnutzer abgefragt wird,
- (ii) Anordnen der Reihe von Reagenzeinheiten im Gehäuse gemäß dem zu erfassenden Analyten, und
- (iii) Sichern der Reihe von (i) oder (ii) innerhalb des Gehäuses der Kassette.

12. Verfahren nach Anspruch 11, welches ferner Folgendes umfasst:

- (a) Auswahl eines zu erfassenden Analyten,
- (b) Versiegeln der Kassette, oder
- (c) Kennzeichnen der Kassette mit einem lesbaren Label, das für den zu erfassenden Analyten indikativ ist, und optional, wobei das lesbare Label ein Barcode oder RFID ist.

13. Verfahren zur automatischen Erfassung einer Mehrzahl von Analyten in einer Körperflüssigkeitsprobe, die von einem Subjekt gesammelt ist, welches Folgendes umfasst:

- a. Bereithalten der Körperflüssigkeitsprobe für eine Kassette nach Anspruch 1,
- b. Erfassung der einzelnen Assayeinheit unter Verwendung einer Flüssigkeitsübertragungseinrichtung,
- c. Übertragen der Körperflüssigkeitsprobe von einer Probensammeleinheit zu einer einzelnen Assayeinheit unter Verwendung der Flüssigkeitsübertragungseinrichtung, und
- d. Übertragen eines Reagenz der einzelnen Reagenzeinheit zur einzelnen Assayeinheit, wobei das Reagenz mit der Körperflüssigkeitsprobe reagiert, um ein Signal zu erhalten, das für den einzelnen Analyten der Mehrzahl von zu erfassenden Analyten indikativ ist.

14. Verfahren nach Anspruch 13, wobei

- (a) die Flüssigkeitsübertragungseinrichtung eine Mehrzahl von Köpfen enthält, wobei ein einzelner Kopf der Mehrzahl von Köpfen so gebildet ist, dass er die einzelne Assayeinheit erfasst, und wobei die Flüssigkeitsübertragungseinrichtung einen programmierbaren Prozessor enthält, der so ausgeführt ist, dass er eine Flüssigkeitsübertragung der Körperflüssigkeitsprobe von der Probensammeleinheit ausführt und das Reagenz von der einzelnen Reagenzeinheit in die einzelne Assayeinheit durchführt, und optional ferner Instruktionen für den programmierbaren Prozessor bereitstellt, und insbesondere, wobei die Instruktionen den Schritt der Übertragung der Körperflüssigkeitsprobe zur einzelnen Assayeinheit bewirken,
- (b) der Schritt der Überführung der Körperflüssigkeitsprobe einen Grad der Verdünnung der Körperflüssigkeitsprobe in der einzelnen Assayeinheit enthält, um das Signal, das für die einzelnen Analyten der Mehrzahl von Analyten indikativ ist, in einen detektierbaren Bereich zu bringen,
- (c) die Körperflüssigkeitsprobe wenigstens zwei einzelnen Analyten enthält, die in Konzentrationen vorhanden sind, die sich um wenigstens zwei Größenordnungen unterscheiden,
- (d) die Körperflüssigkeitsprobe wenigstens zwei einzelnen Analyten enthält, die bei Konzentrationen vorhanden sind, die sich um wenigstens fünf Größenordnungen unterscheiden,
- (e) der Grad der Verdünnung der Körperflüssigkeitsprobe die Signale, die für wenigstens zwei einzelne Analyten indikativ sind, in einen detektierbaren Bereich bringt,

(f) der Grad der Verdünnung der Körperflüssigkeitsprobe mit einem Fotomultiplier erfasst wird und die wenigstens zwei einzelnen Analyten in einem Bereich von etwa 1000 bis etwa 1 Million Zählungen pro Sekunde liegen,
 (g) die Körperflüssigkeitsprobe kleiner als etwa 50 Mikroliter ist,
 (h) die Körperflüssigkeitsprobe ein einzelner Blutstropfen ist, oder
 (i) das Reagenz in der einzelnen Reagenzeinheit ein Enzymsubstrat für ein Immunoassay ist, insbesondere ferner die Wiederholung des Schrittes umfasst, das Reagenz von der einzelnen Reagenzeinheit zu übertragen, nachdem die Reaktion zur Erzeugung des Signals, das für die einzelnen Analyten der Mehrzahl von Analyten, die zu detektieren sind, ausgeführt ist, wobei eine zweite Reaktion zur Ermittlung eines zweiten Signals erfolgt, das für einen einzelnen Analyten indikativ ist und insbesondere, wobei eine Intensität des Signals und eine zweite Intensität des zweiten Signals, das für den einzelnen Analyten indikativ ist, gemittelt wird, um die schließliche Intensität des Signals, das für die einzelnen Analyten indikativ ist, zu errechnen.

15. Verfahren zur Messung eines Volumens einer Probe einer biologischen Flüssigkeit, die von einem Subjekt genommen ist, welches umfasst:

- a. Reagieren einer bekannten Menge eines Kontrollanalyten in der Probe mit einem Reagenz, um ein detektierbares Signal zu erhalten, das für eine Menge des Kontrollanalyten indikativ ist, wobei der Reaktionsschritt in eine Kassette nach Anspruch 1 erfolgt, und
- b. Vergleichen des detektierbaren Signals mit einem erwarteten detektierbaren Signal, wobei das erwartete Signal für ein erwartetes Volumen der Probe indikativ ist, und wobei der Vergleich eine Messung des Volumens der zu messenden Probe ist,

insbesondere welches ferner umfasst:

- (a) Verifizieren des Volumens der Probe, wenn die Messung des Volumens der Probe innerhalb etwa 50% des erwarteten Volumens der Probe liegt,
- (b)

- (i) Reagieren der Probe, die einen Zielanalyten aufweist mit einem Reagenz, um ein erfassbares Signal zu erhalten, das für die Zielanalyten indikativ ist, und
- (ii) Messen der Menge des Zielanalyten in der Probe auf Basis des detektierbaren Signals, das für den Zielanalyten und die Messung des Volumens der Flüssigkeitsprobe indikativ ist, oder

(c)

- (i) Mischen der Probe bei Vorhandensein von magnetisierbaren Partikeln in einer Probensammeleinheit, wobei die magnetisierbaren Partikel eine Antikörpererfassungsfläche enthalten, um an Nichtplasmateile der Probe zu binden, und
- (ii) Aufbringen eines magnetischen Feldes oberhalb einer Plasmasammelstelle auf die gemischten Probe, um eine Suspension der Nichtplasmateile der Probe an der Oberseite des Plasmasammelbereichs zu bewirken, insbesondere wobei

- (1) die Probe ein Blutprobe ist,
- (2) die Probensammeleinheit eine Kapillarröhre ist,
- (2) die Probe kleiner als etwa 50 Mikroliter ist,
- (3) das erhaltene Plasma kleiner als etwa 10 Mikroliter ist,
- (4) die Probe nicht verdünnt ist,
- (5) die Mischung bei Vorhandensein von ungebundenen Antikörpern auftritt, welche nicht an einer festen Oberfläche gebunden sind,
- (6) die Mischung das Mischen durch eine Spritzenaktion umfasst,
- (7) das Verfahren in einem System nach den Ansprüchen 4 oder 8 ausgeführt wird, oder

(d) die Resultate des Vergleichs an einen Endnutzer übermittelt werden und optional, wobei das Resultat drahtlos übertragen wird und insbesondere, wobei

- (a) der Kontrollanalyt normalerweise nicht in einer erfassbaren Menge in der Probe vorhanden ist,
- (b) eine Flüssigkeitsprobe und die Körperflüssigkeitsprobe die gleiche Probe sind,
- (c) der Kontrollanalyt nicht mit einem Zielanalyten in der Körperflüssigkeitsprobe reagiert,
- (d) eine Flüssigkeitsprobe und die Körperflüssigkeitsprobe unterschiedliche Flüssigkeitsproben sind,

- (e) der Kontrollanalyt aus einer Gruppe ausgewählt ist, die Folgendes umfasst: Albumin, Fluorescein, IgG, C-Protein, Fluorescingelabeltes Albumin, Fluorescingelabeltes IgG, Anti-Fluorescein, Anti-Digoxigenin, Digoxigeningelabeltes Albumin, Digoxigeningelabeltes IgG, biotinyliertes Protein und nicht humanes IgG,
 (f) die Reaktion ein Immunoassay ist,
 (g) die Reaktion ein ELISA ist, oder
 (h) das Verfahren ausgeführt wird in einem System der Ansprüche 4 oder 8.

Revendications

1. Cartouche destinée à la détection automatisée d'un analyte dans un échantillon de fluide corporel comprenant :

un ensemble d'unités de dosage adressables configuré pour exécuter une réaction chimique qui génère un signal détectable indicatif de la présence ou de l'absence de l'analyte ; et
 un ensemble d'unités de réactifs adressables, dans laquelle une unité de réactif adressable individuelle de l'ensemble est adressée pour correspondre à une unité de dosage adressable individuelle de l'ensemble des unités de dosage, dans laquelle l'unité de réactif individuelle est configurée pour être calibrée en référence à l'unité de dosage individuelle correspondante avant que les ensembles ne soient assemblés sur la cartouche et dans laquelle l'unité de dosage individuelle de l'ensemble des unités de dosage adressables et l'unité de réactif individuelle de l'ensemble des unités de réactif adressables sont configurées pour être mobiles pour réaliser une communication fluïdique, de telle sorte que les réactifs destinés à exécuter la réaction chimique soient amenés en contact avec la partie de l'échantillon dans l'unité de dosage.

2. Cartouche selon la revendication 1, dans laquelle :

- (a) l'unité de réactif individuelle est configurée pour recevoir une unité de dosage mobile ;
- (b) l'unité de dosage individuelle comprend une pointe de dosage ;
- (c) l'unité de dosage individuelle est configurée pour exécuter un dosage immunologique ; ou
- (d) l'échantillon de fluide corporel est un échantillon de sang.

3. Cartouche selon la revendication 1, comprenant en outre :

- (a) une unité de collecte d'échantillon configurée pour :

- (i) recevoir l'échantillon de fluide corporel ;
- (ii) recevoir un volume de l'échantillon de fluide corporel approximativement égal ou inférieur à 50 microlitres ; ou
- (iii) recevoir un volume de l'échantillon de fluide corporel qui est une seule goutte de sang ; ou

- (b) une unité de prétraitement configurée pour récupérer une partie de l'échantillon de fluide corporel pour exécuter la réaction chimique pour détecter l'analyte, et dans laquelle optionnellement l'échantillon de fluide corporel est un échantillon de sang complet et dans laquelle la partie est du plasma.

4. Système pour la détection automatisée d'un analyte dans un échantillon de fluide corporel comprenant :

- (a) une cartouche selon la revendication 1 ; et
- (b) un assemblage de détection :

- (i) pour la détection du signal détectable indicatif de la présence ou de l'absence de l'analyte ;
- (ii) configuré pour détecter des intensités de signal amenées à être détectable à l'intérieur de la plage par une dilution de l'échantillon de fluide corporel ;
- (iii) configuré pour détecter des intensités de signal comprises entre environ 1000 et environ 1 million de comptes par seconde en utilisant un photomultiplicateur.

5. Système selon la revendication 4, comprenant en outre :

- (a) un dispositif mécanique programmable configuré pour déplacer l'unité de dosage individuelle à partir d'un premier emplacement jusqu'à un second emplacement ;

- (b) un assemblage de communication destiné à transmettre un protocole basé sur l'analyte à détecter ;
- (c) un bloc de chauffage configuré pour recevoir l'unité de dosage individuelle ; ou
- (d) un bloc magnétique.

6. Système selon la revendication 4, comprenant en outre un dispositif de transfert de fluide, dans lequel le dispositif de transfert de fluide :

- (a) est une pipette, et dans lequel optionnellement la pipette est une pipette à déplacement d'air ;
- (b) est automatisé ; ou
- (c) comprend une pluralité de têtes, dans lequel une tête individuelle de la pluralité de têtes est configurée pour venir en prise avec l'unité de dosage individuelle, et comprend un processeur programmable configuré pour diriger un transfert de fluide de l'échantillon de fluide corporel en provenance d'une unité de collecte d'échantillons, et le réactif en provenance de l'unité de réactif individuelle, dans l'unité de dosage individuelle ;

et optionnellement :

- (i) dans lequel la configuration du processeur pour diriger le transfert de fluide réalise un degré de dilution de l'échantillon de fluide corporel dans l'ensemble d'unités de dosage pour obtenir des signaux indicatifs de la pluralité d'analytes détectés à l'intérieur d'une plage détectable, de telle sorte que ladite pluralité d'analytes soient détectables avec ledit système ; ou
- (ii) dans lequel le dispositif de transfert de fluide comprend en outre un moteur en communication avec le processeur programmable.

7. Système selon la revendication 4, dans lequel :

- (a) l'échantillon de fluide corporel comprend au moins deux analytes qui sont présents à des concentrations qui diffèrent de 2 ordres de grandeur au moins ;
- (b) l'échantillon de fluide corporel comprend au moins deux analytes qui sont présents à des concentrations qui diffèrent de 5 ordres de grandeur au moins ;
- (c) un degré de dilution de l'échantillon de fluide corporel permet d'obtenir des signaux indicatifs de deux analytes au moins à l'intérieur de la plage détectable ;
- (d) l'échantillon de fluide corporel est inférieur à 50 μ l environ ;
- (e) l'échantillon de fluide corporel est une seule goutte de sang ;
- (f) une tête individuelle d'un dispositif de transfert de fluide est configurée pour adhérer à l'unité de dosage individuelle ;
- (g) ladite unité de dosage individuelle fournit un site de réaction de dosage immunologique ; ou
- (h) ladite unité de dosage individuelle est une pointe pour pipette.

8. Procédé de détection d'un analyte dans un échantillon de fluide corporel collecté chez un sujet comprenant :

- (a) la fourniture d'un échantillon de fluide corporel à la cartouche selon la revendication 1 ;
- (b) la possibilité dudit échantillon de réagir à l'intérieur d'au moins une unité de dosage ; et
- (c) la détection dudit signal détectable généré à partir dudit analyte collecté dans ledit échantillon de fluide corporel.

9. Procédé selon la revendication 8, dans lequel l'échantillon de fluide corporel est du sang et le procédé comprend en outre la récupération du plasma contenu dans le sang.

10. Système de détection automatisée d'un analyte dans une partie de plasma d'un échantillon de sang complet, comprenant :

- (a) une cartouche selon la revendication 1, dans lequel ladite cartouche est configurée en outre pour recevoir et pour traiter de manière automatique l'échantillon de sang complet pour obtenir la partie de plasma, à partir de laquelle un signal détectable indicatif de la présence ou de l'absence de l'analyte d'intérêt, est généré dans la cartouche ; et
- (b) un assemblage de détection pour détecter le signal détectable indicatif de la présence ou de l'absence de l'analyte.

11. Procédé d'assemblage à la demande d'une cartouche selon la revendication 1, dans lequel la cartouche comprend un boîtier, ledit procédé comprenant :

- (i) le placement dans le boîtier, selon l'analyte à détecter, de l'ensemble des unités de dosage adressable, dans lequel l'unité de dosage individuelle de l'ensemble est configurée pour exécuter une réaction chimique qui détecte un analyte qui présente un intérêt commandée par ledit utilisateur final ;
- (ii) le placement dans le boîtier, selon l'analyte à détecter, de l'ensemble d'unités de réactifs ; et
- (iii) la fixation des ensembles (i) et (ii) à l'intérieur du boîtier de la cartouche.

12. Procédé selon la revendication 11, comprenant en outre :

- (a) la sélection d'un analyte à détecter ;
- (b) le scellage de la cartouche ; ou
- (c) l'étiquetage de la cartouche avec une étiquette lisible qui indique l'analyte à détecter, et dans lequel optionnellement l'étiquette lisible est un code-barres ou un RFID.

13. Procédé de détection automatisée d'une pluralité d'analytes dans un échantillon de fluide corporel collecté chez un sujet comprenant :

- (a) la fourniture de l'échantillon de fluide corporel à la cartouche selon la revendication 1 ;
- (b) la mise en prise de l'unité de dosage individuelle en utilisant un dispositif de transfert de fluide ;
- (c) le transfert de l'échantillon de fluide corporel à partir d'une unité de collecte d'échantillons jusqu'à l'unité de dosage individuelle en utilisant le dispositif de transfert de fluide ; et
- (d) le transfert d'un réactif à partir de l'unité de réactif individuelle jusqu'à l'unité de dosage d'analyse, en faisant réagir de ce fait le réactif avec l'échantillon de fluide corporel pour obtenir le signal indicatif de l'analyte individuel de la pluralité d'analytes détectés.

14. Procédé selon la revendication 13, dans lequel :

- (a) le dispositif de transfert de fluide comprend une pluralité de têtes, dans lequel une tête individuelle de la pluralité de têtes est configurée pour se mettre en prise avec l'unité de dosage individuelle ; et dans lequel ledit dispositif de transfert de fluide comprend un processeur programmable configuré pour diriger le transfert de fluide de l'échantillon de fluide corporel à partir de l'unité de collecte d'échantillons et du réactif à partir de l'unité de réactif individuelle dans l'unité de dosage individuelle, comprenant en outre optionnellement l'apport d'instructions au processeur programmable, dans lequel optionnellement les instructions dirigent le transfert de l'échantillon de fluide corporel jusqu'à l'unité de dosage individuelle ;
- (b) l'étape de transfert de l'échantillon de fluide corporel réalise un degré de dilution de l'échantillon de fluide corporel dans l'unité de dosage individuelle pour fournir le signal indicatif de l'analyte individuel de la pluralité d'analytes détectés à l'intérieur d'une plage détectable ;
- (c) l'échantillon de fluide corporel comprend au moins deux analytes individuels qui sont présents à des concentrations qui diffèrent d'au moins 2 ordres de grandeur ;
- (d) l'échantillon de fluide corporel comprend au moins deux analytes individuels qui sont présents à des concentrations qui diffèrent d'au moins 5 ordres de grandeur ;
- (e) le degré de dilution de l'échantillon de fluide corporel permet d'obtenir des signaux indicatifs d'au moins deux analytes individuels à l'intérieur d'une plage détectable ;
- (f) le degré de dilution de l'échantillon de fluide corporel est détecté au moyen d'un photomultiplicateur et les au moins deux analytes individuels au moins se situent dans une plage comprise entre environ 1000 et environ 1 million de comptes par seconde ;
- (g) l'échantillon de fluide corporel est inférieur à 50 μ l environ ;
- (h) l'échantillon de fluide corporel est une seule goutte de sang ; ou
- (i) le réactif dans l'unité de réactif individuelle est un substrat d'enzyme d'un dosage immunologique, comprenant en outre optionnellement la répétition de l'étape du transfert du réactif à partir de l'unité de réactif individuelle une fois que la réaction destinée à obtenir le signal indicatif de l'analyte individuel de la pluralité d'analytes détectés, a pris fin, en créant de ce fait une seconde réaction destinée à obtenir un second signal indicatif de l'analyte individuel, et dans lequel optionnellement une intensité du signal et une seconde intensité du second signal indicatif de l'analyte individuel, sont moyennées pour calculer l'intensité finale du signal indicatif de l'analyte individuel.

15. Procédé destiné à mesurer un volume d'un échantillon de fluide biologique collecté chez un sujet, comprenant :

(a) la réaction d'une quantité connue d'un analyte de contrôle dans ledit échantillon avec un réactif pour obtenir un signal détectable indicatif de la quantité d'analyte de contrôle, dans lequel ladite étape de réaction se produit dans une cartouche selon la revendication 1 ; et

(b) la comparaison dudit signal détectable à un signal détectable escompté, dans lequel le signal escompté est indicatif d'un volume escompté de l'échantillon, et dans lequel ladite comparaison fournit une mesure dudit volume dudit échantillon mesuré ;

comprenant optionnellement en outre :

(a) la vérification du volume dudit échantillon lorsque la mesure du volume de l'échantillon est comprise à environ 50 % du volume escompté de l'échantillon ;

(b)

(i) la réaction dudit échantillon qui contient un analyte cible avec un réactif pour obtenir un signal détectable indicatif de l'analyte cible ; et

(ii) la mesure de la quantité d'analyte cible dans l'échantillon sur la base dudit signal détectable indicatif de l'analyte cible et de la mesure dudit volume dudit échantillon de liquide ; ou

(c)

(i) le mélange de l'échantillon en présence de particules pouvant être aimantées dans une unité de collecte d'échantillons, dans lequel les particules pouvant être aimantées comprennent une surface de capture d'anticorps pour se lier à des parties non plasmiques de l'échantillon ;

et

(ii) l'application d'un champ magnétique, au-dessus de la zone de collection de plasma, à l'échantillon mélangé pour réaliser la suspension des parties non plasmiques de l'échantillon sur la zone de collecte de plasma, dans lequel optionnellement :

(1) l'échantillon est un échantillon de sang ;

(2) l'unité de collecte d'échantillon est un tube capillaire ;

(3) l'échantillon est inférieur à 50 microlitres environ ;

(4) le plasma récupéré est inférieur à 10 microlitres environ ;

(5) l'échantillon n'est pas dilué ;

(6) le mélange se produit en présence d'anticorps non liés à une surface solide ;

(7) le mélange comprend le mélange suite à une action de seringue ; ou

(8) le procédé est exécuté dans un système selon la revendication 4 ou la revendication 8 ; ou

(d) la transmission du résultat de la comparaison à un utilisateur final, et dans lequel optionnellement le résultat est transmis de manière sans fil ;

et dans lequel optionnellement :

(a) l'analyte de contrôle n'est normalement pas présent dans ledit échantillon en une quantité détectable ;

(b) un échantillon de liquide et l'échantillon de fluide corporel sont le même échantillon ;

(c) l'analyte de contrôle ne réagit pas avec un analyte cible dans l'échantillon de fluide corporel ;

(d) un échantillon de liquide et l'échantillon de fluide corporel sont des échantillons de liquide différents ;

(e) l'analyte de contrôle est choisi parmi le groupe constitué par : l'albumine, la fluorescéine, l'IgG, la protéine C, l'albumine marquée à la fluorescéine, l'IgG marquée à la fluorescéine, l'anti-fluorescéine, l'anti-digoxigénine, l'albumine marquée à la digoxigénine, l'IgG marquée à la digoxigénine, des protéines combinées à la biotine, et l'IgG non humaine ;

(f) la réaction est un dosage immunologique ;

(g) la réaction est un ELISA ; ou

(h) le procédé est exécuté dans un système selon la revendication 4 ou la revendication 8.

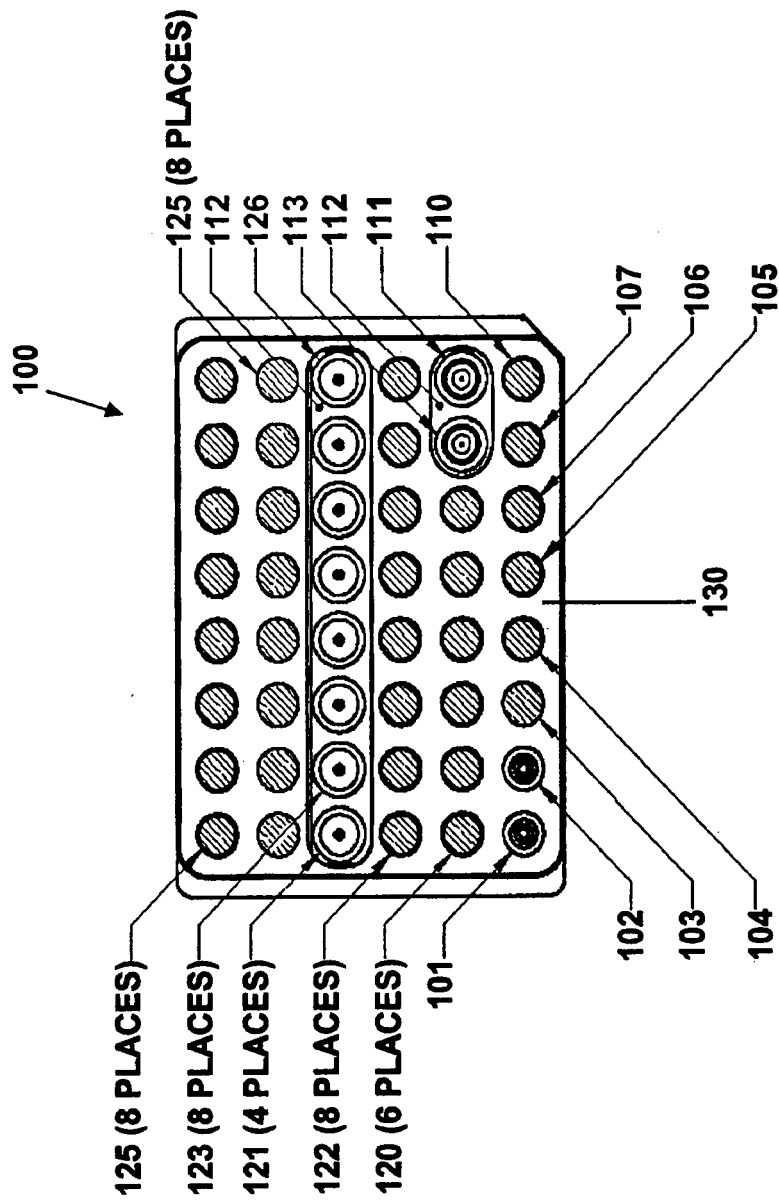


FIGURE 1

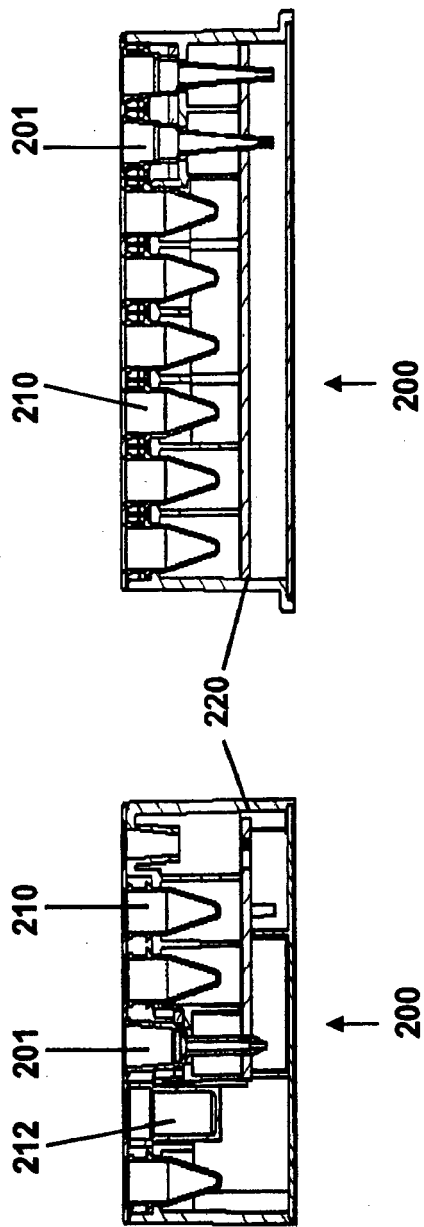


FIGURE 2

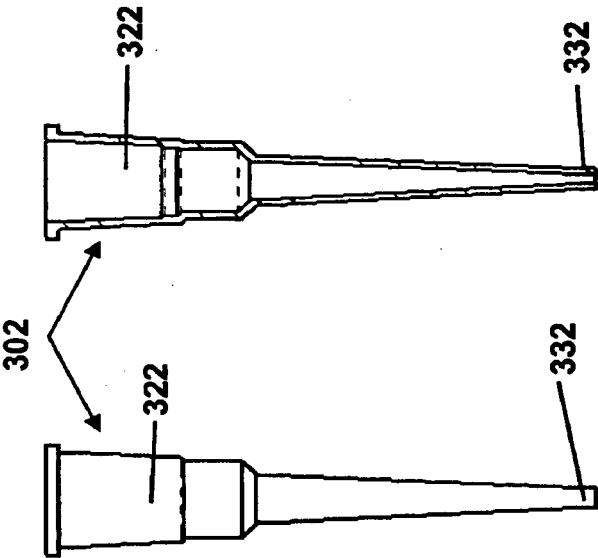


FIGURE 3B

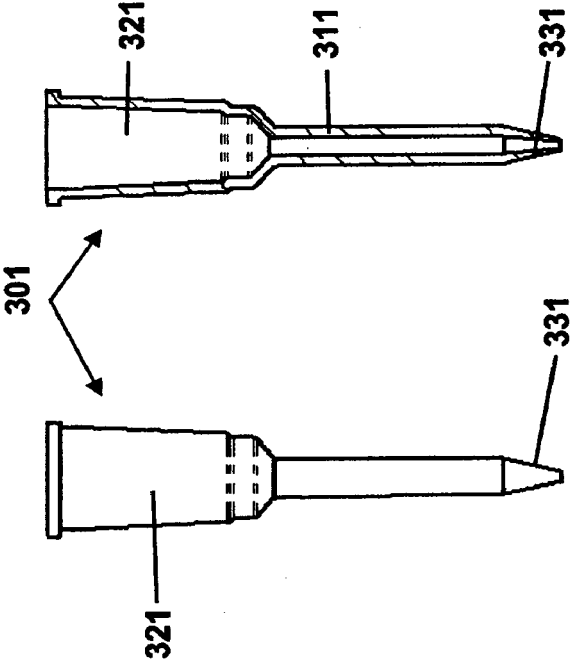


FIGURE 3A

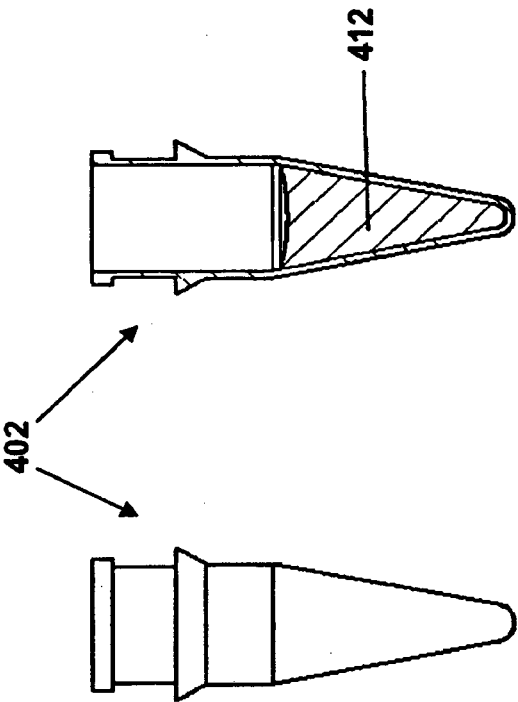


FIGURE 4B

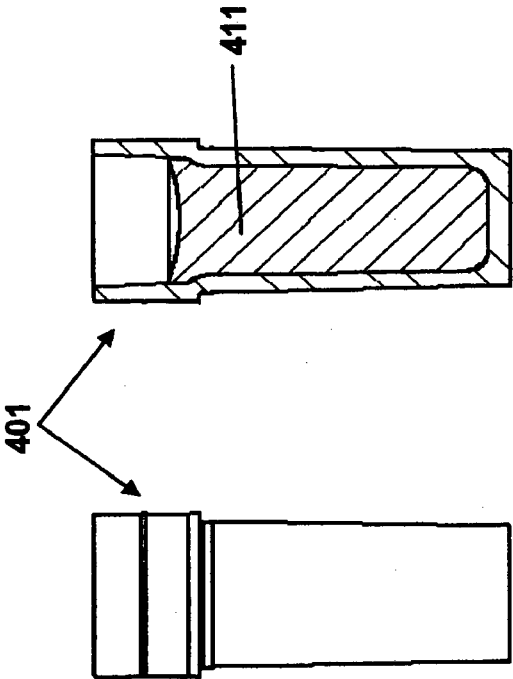


FIGURE 4A

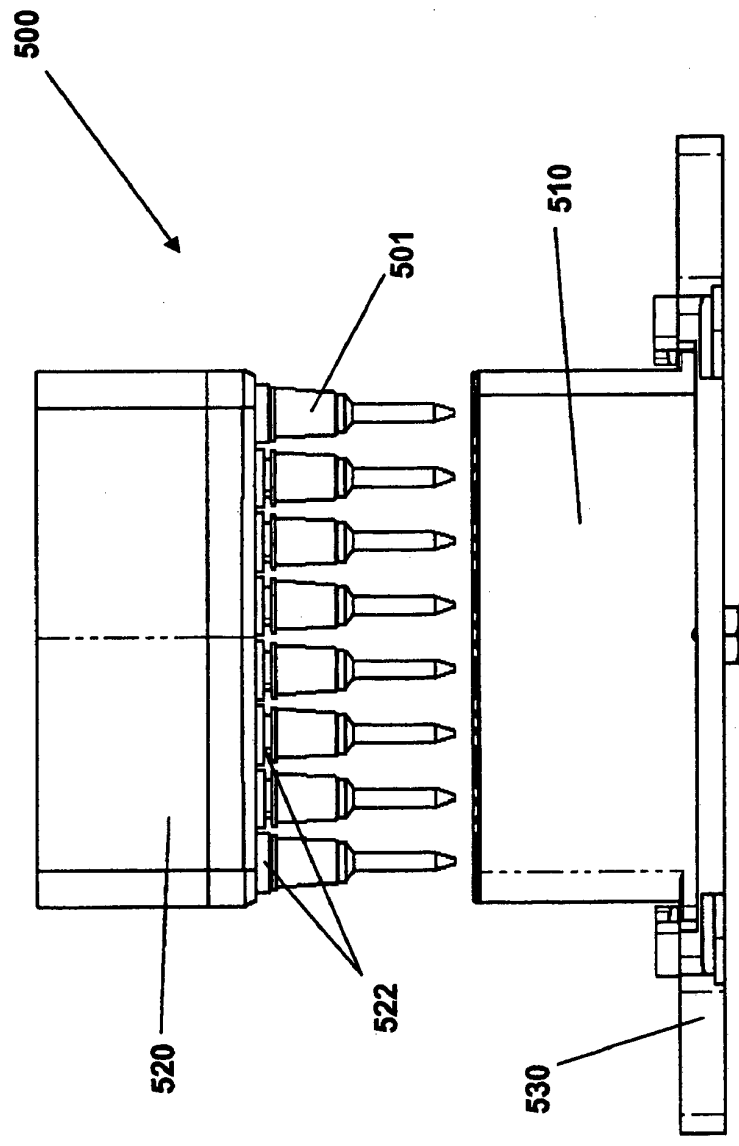


FIGURE 5

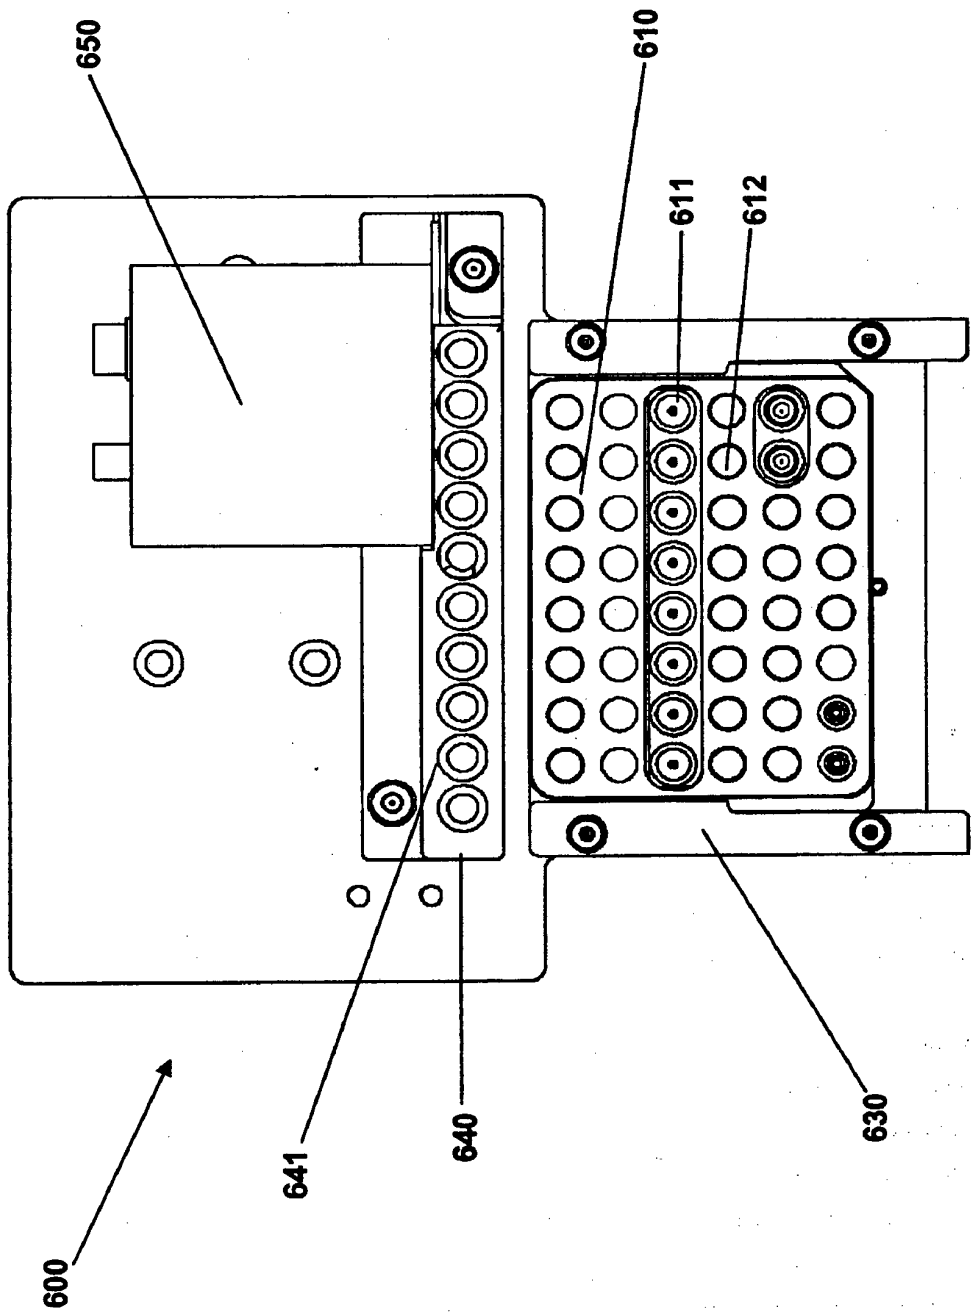


FIGURE 6

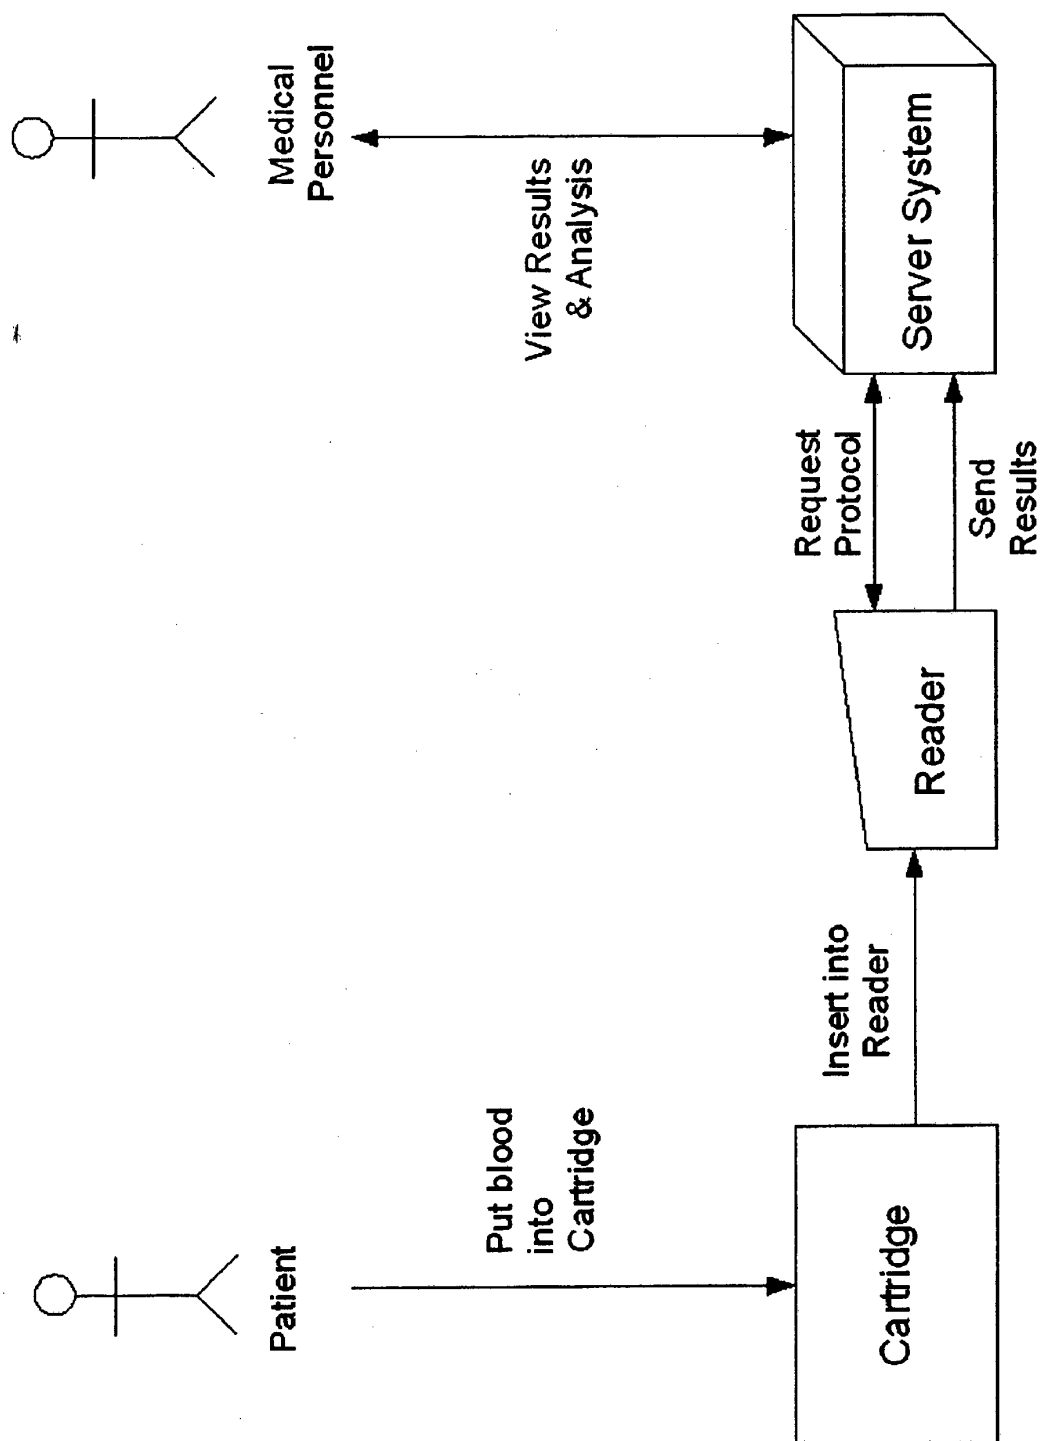


FIGURE 7

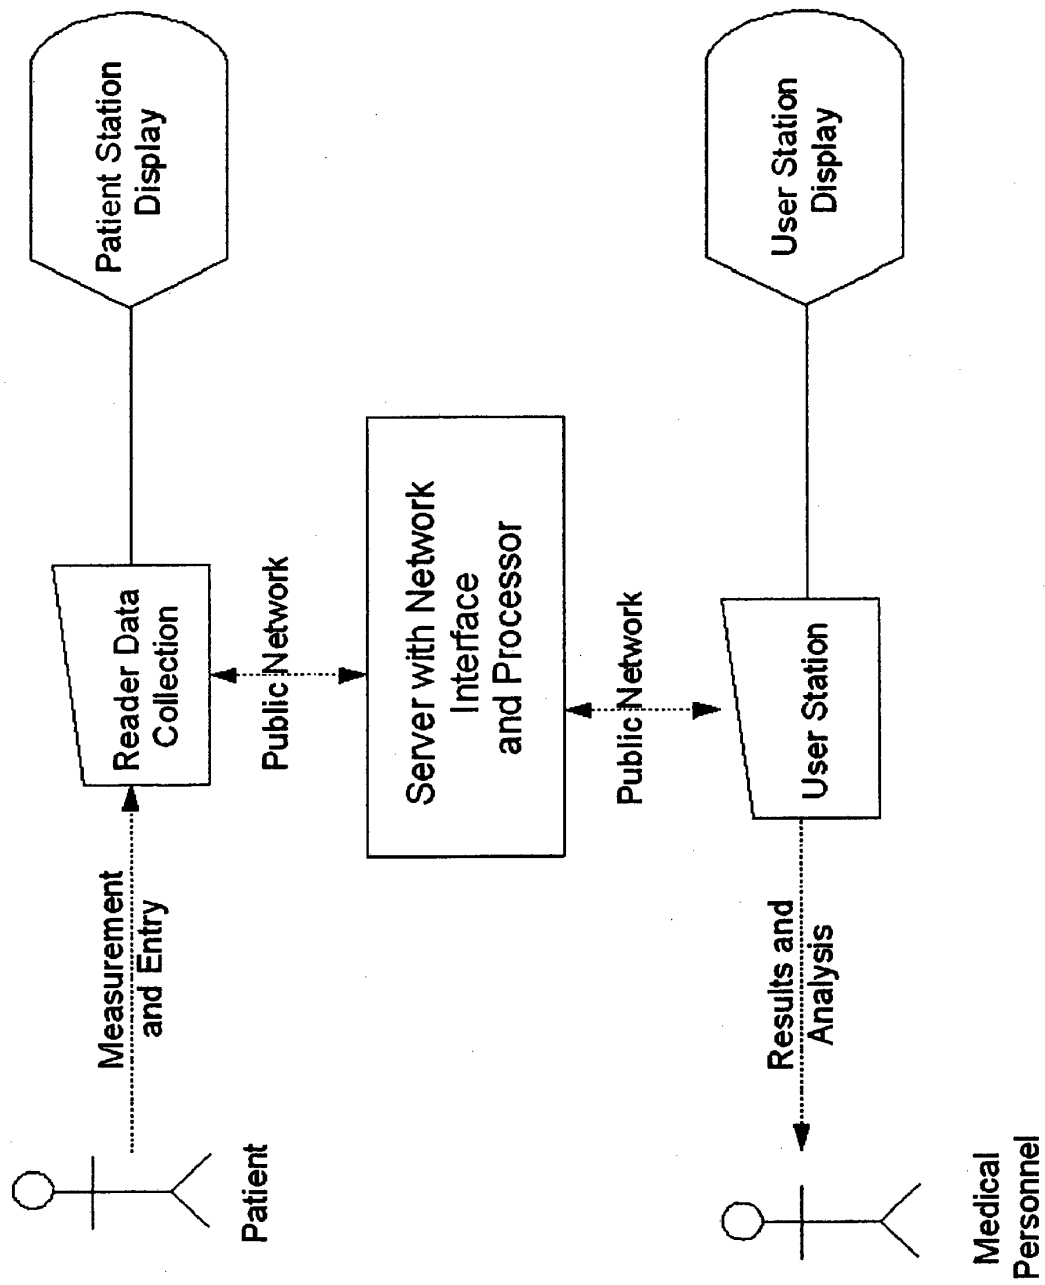


FIGURE 8

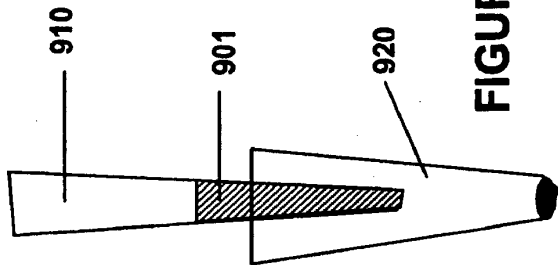


FIGURE 9A

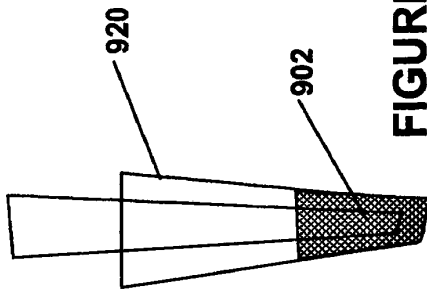


FIGURE 9B

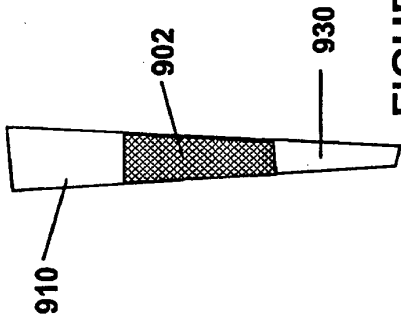


FIGURE 9C

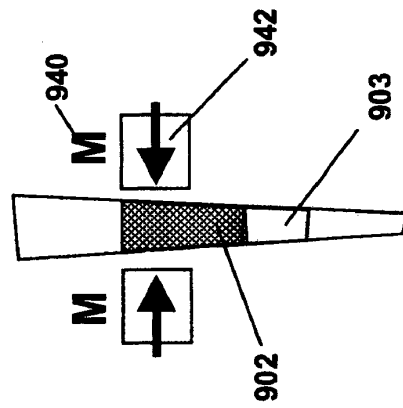


FIGURE 9D

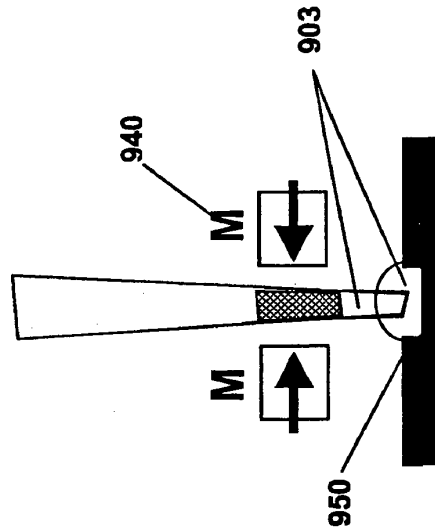


FIGURE 9E

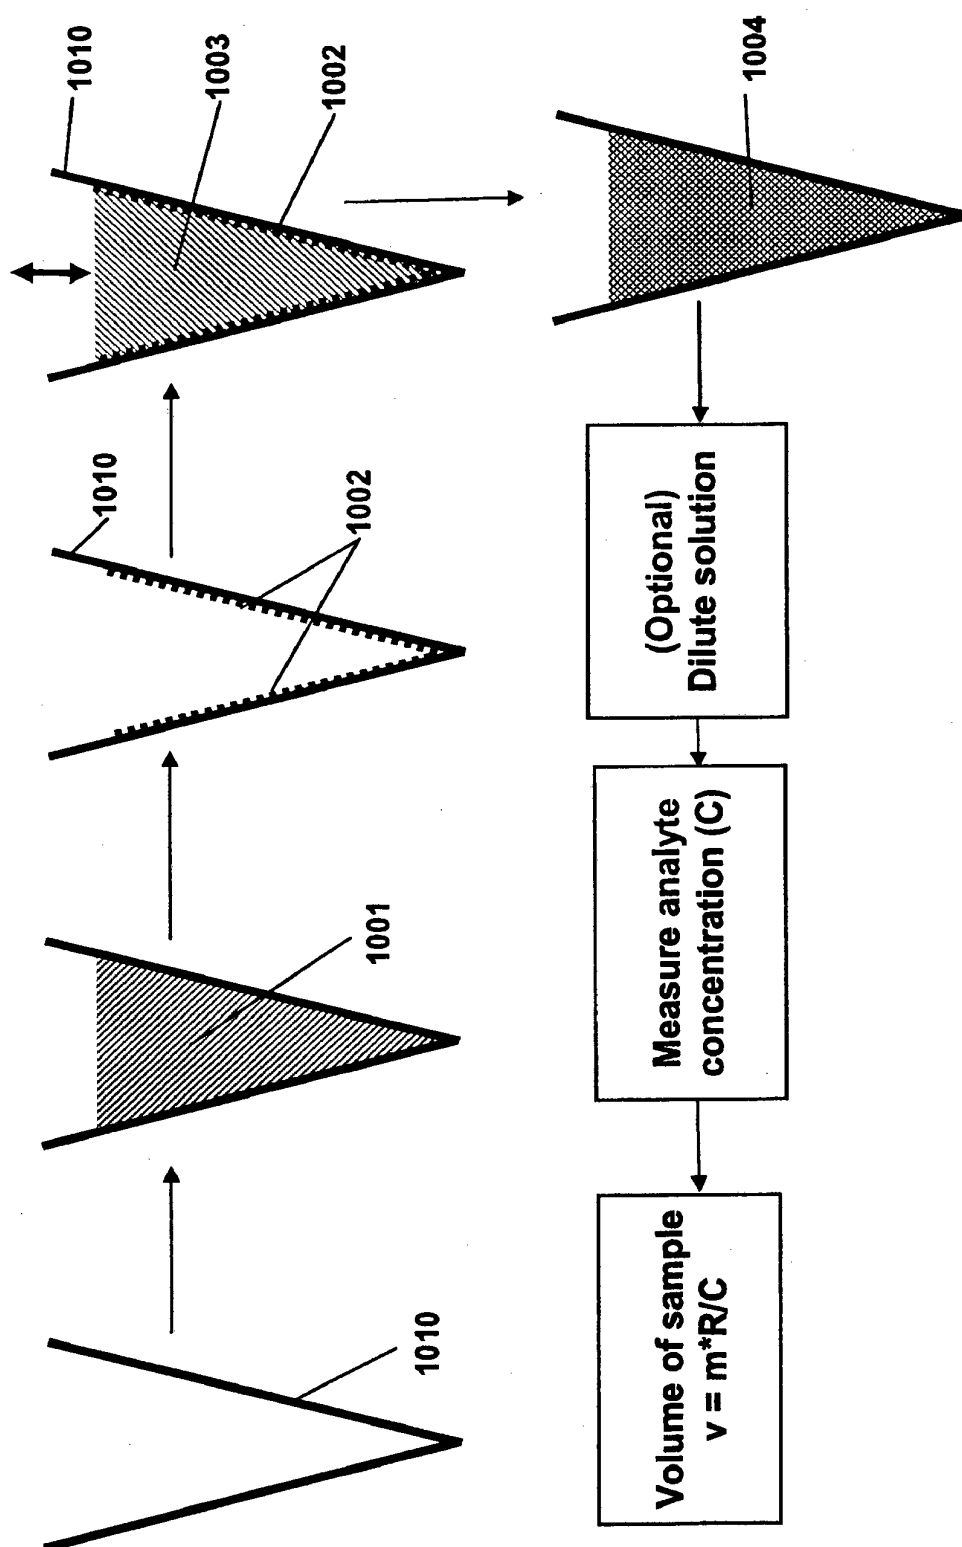


FIGURE 10

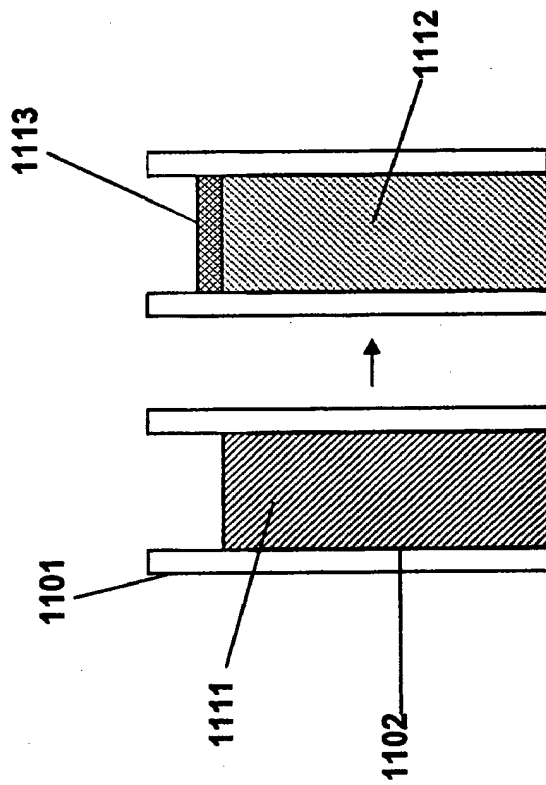


FIGURE 11

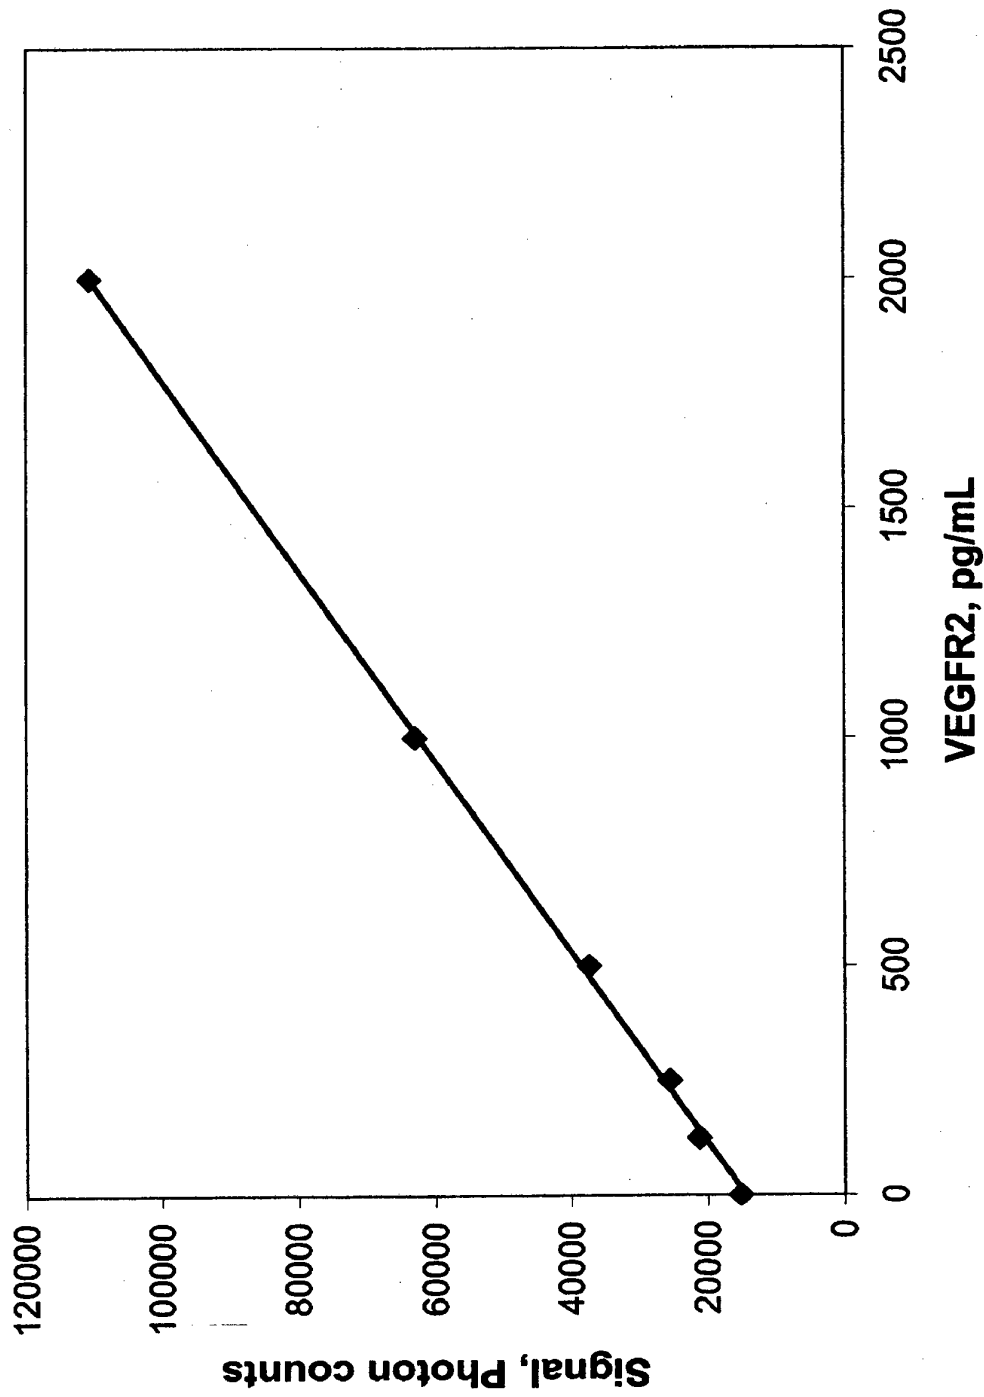


FIGURE 12

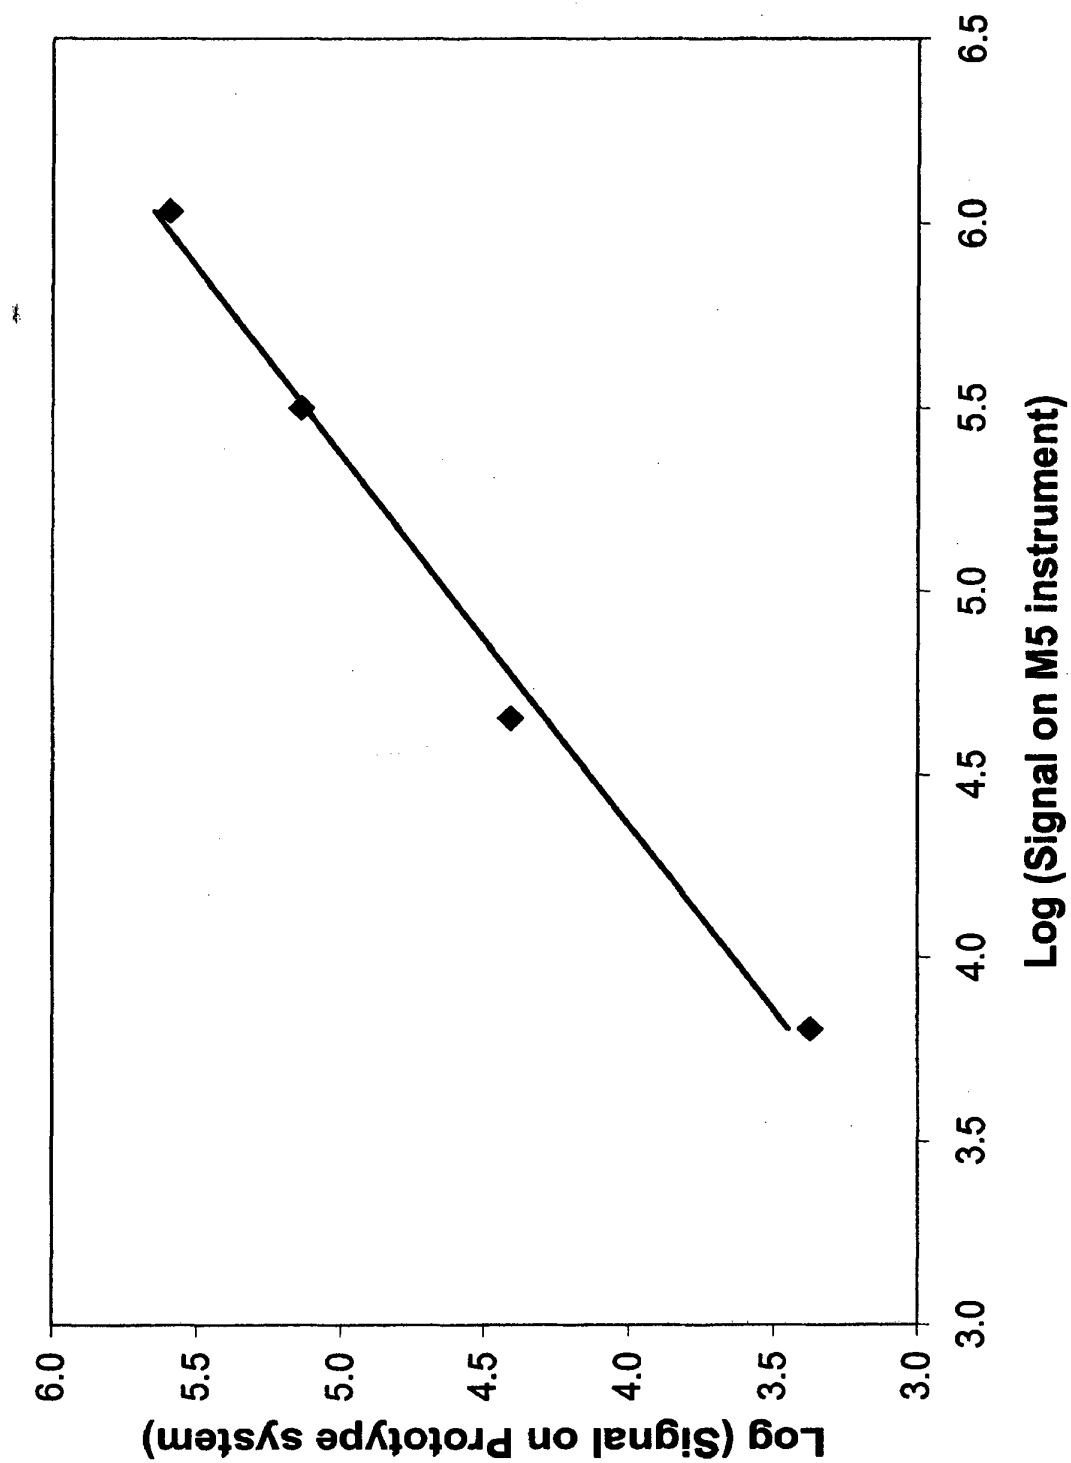
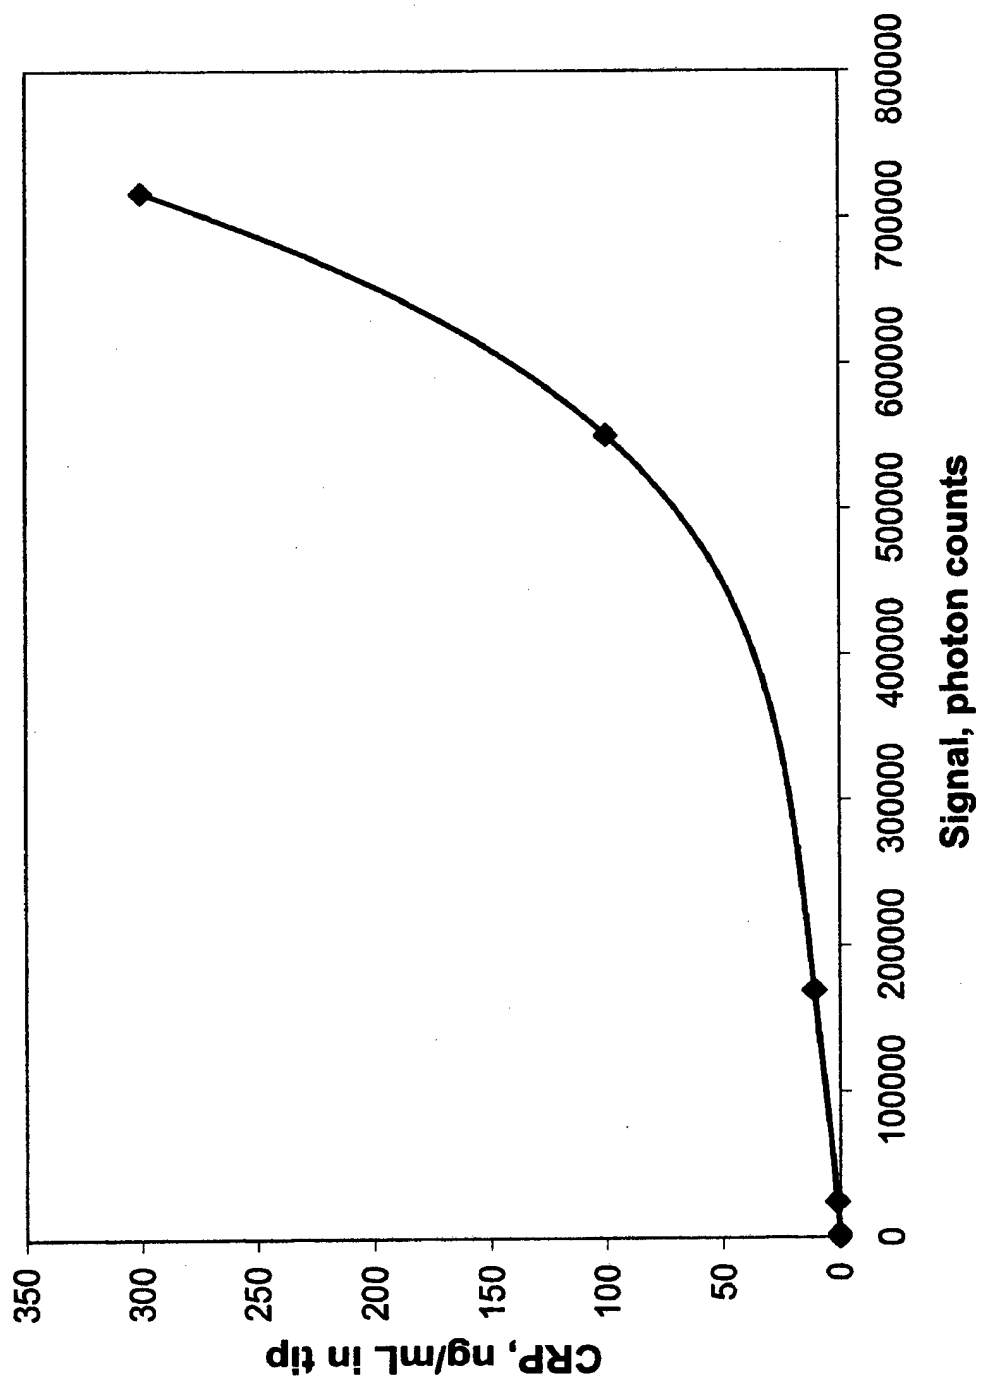


FIGURE 13

**FIGURE 14**

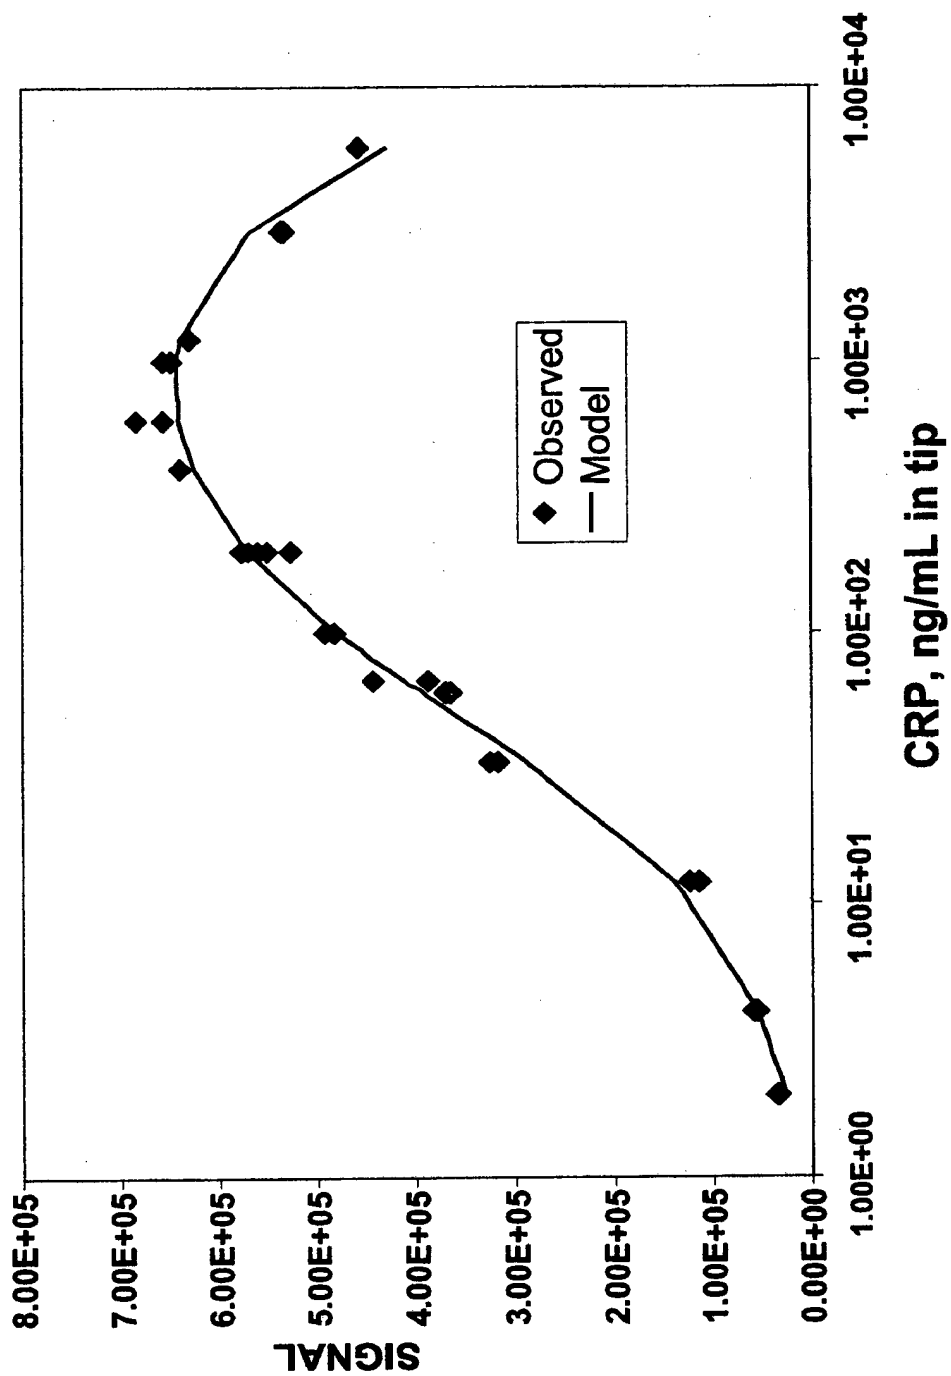


FIGURE 15

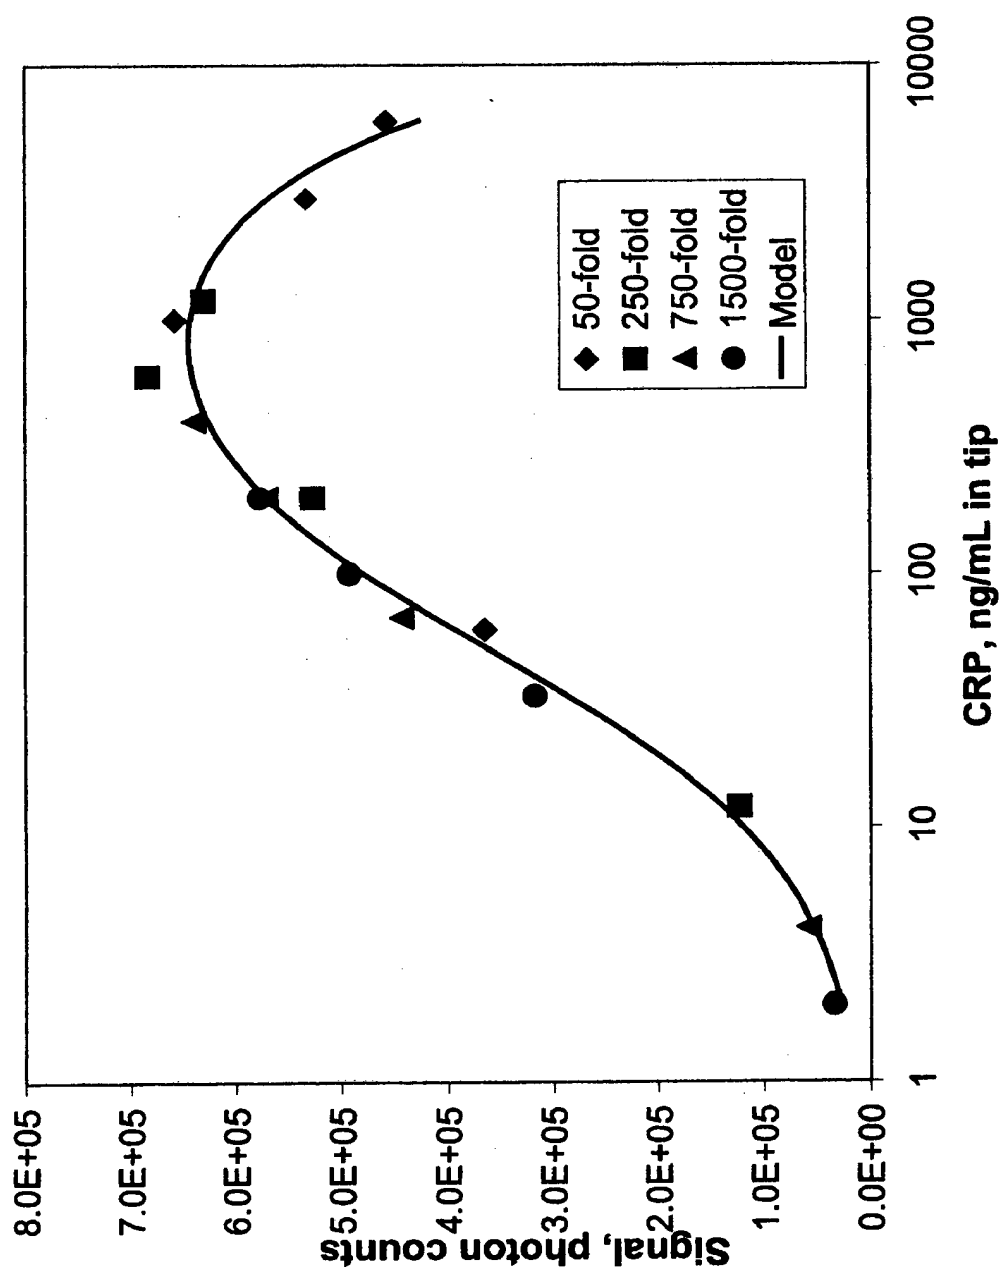


FIGURE 16

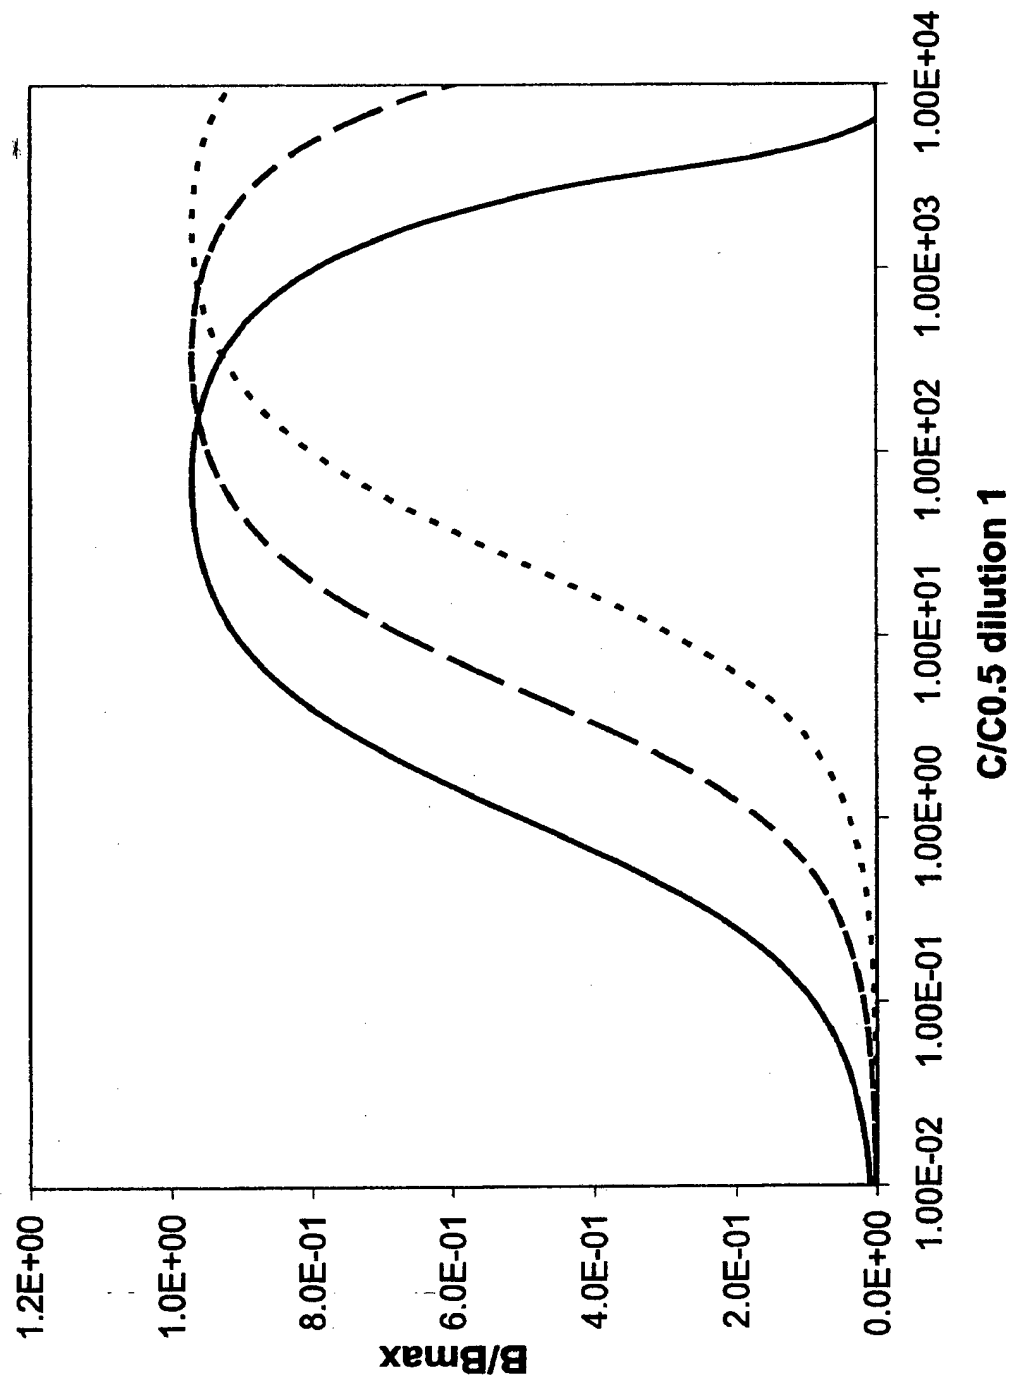


FIGURE 17

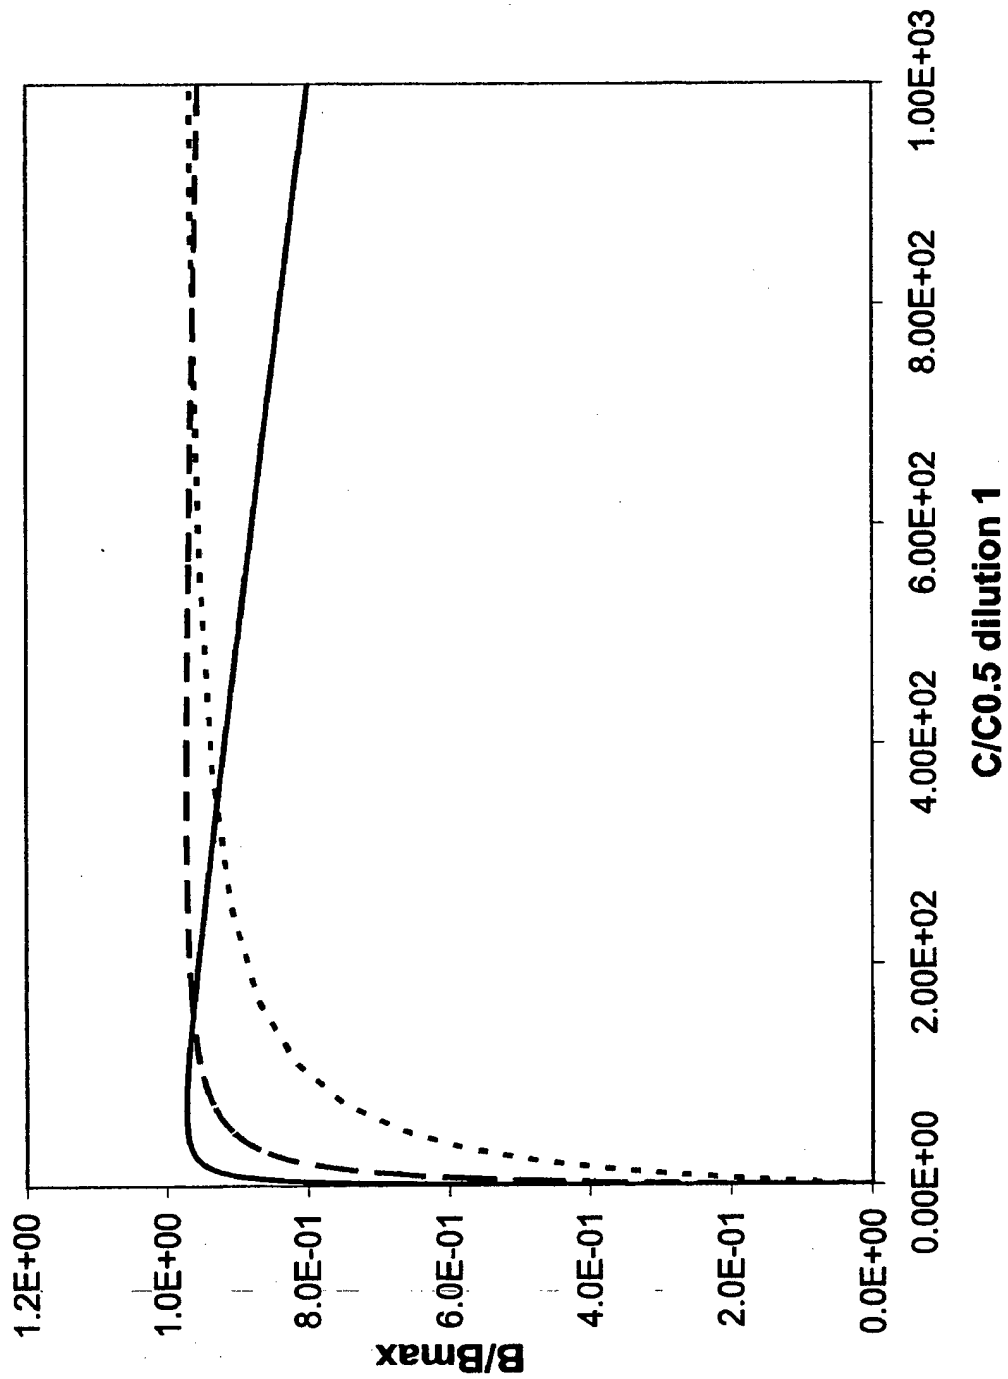


FIGURE 18

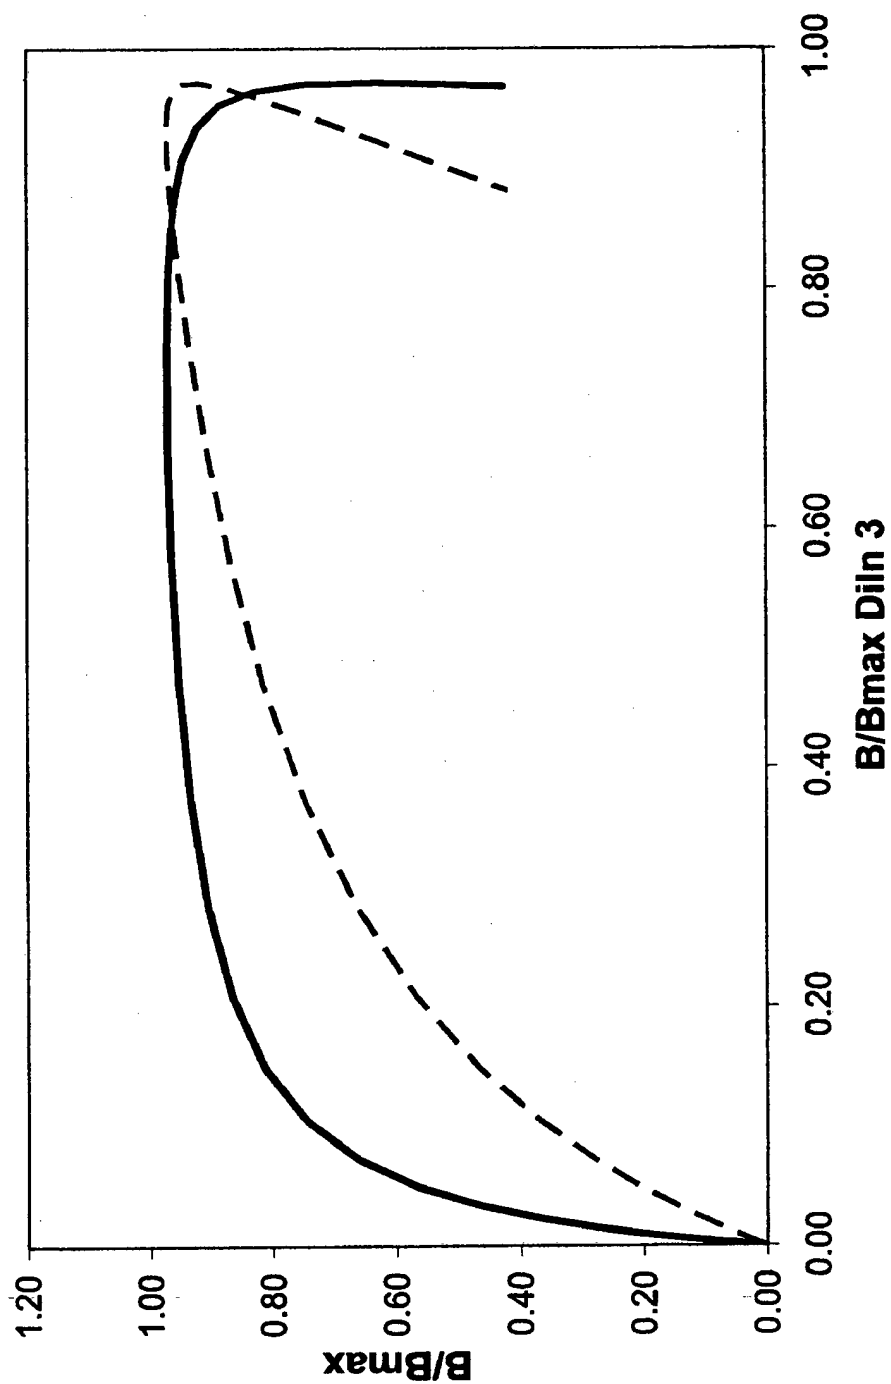


FIGURE 19

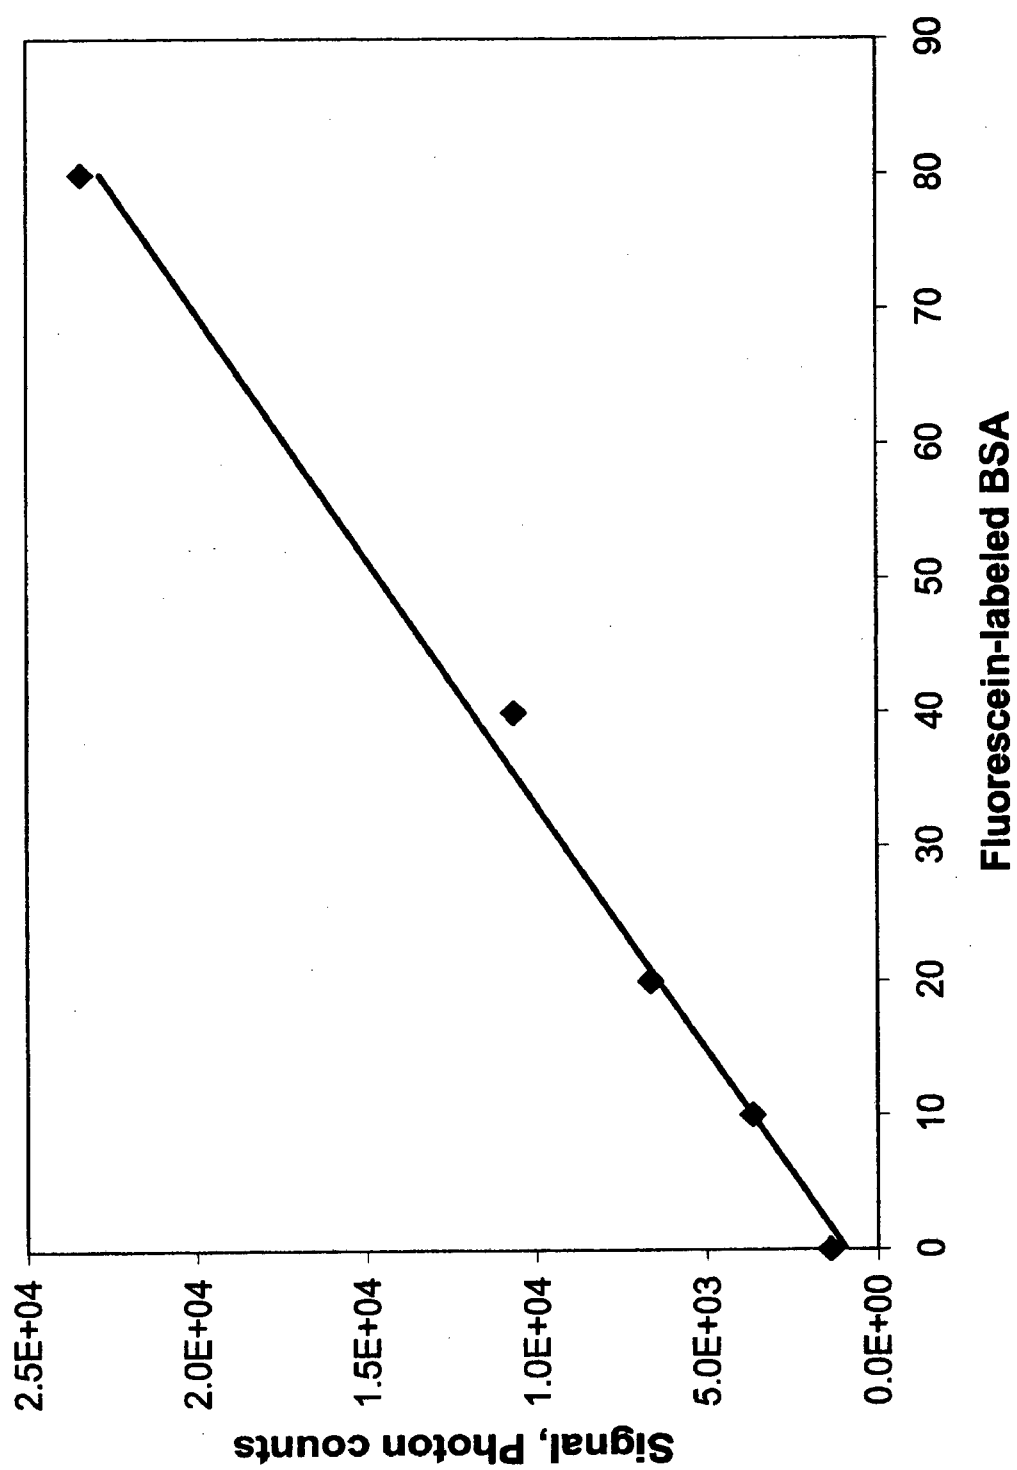


FIGURE 20

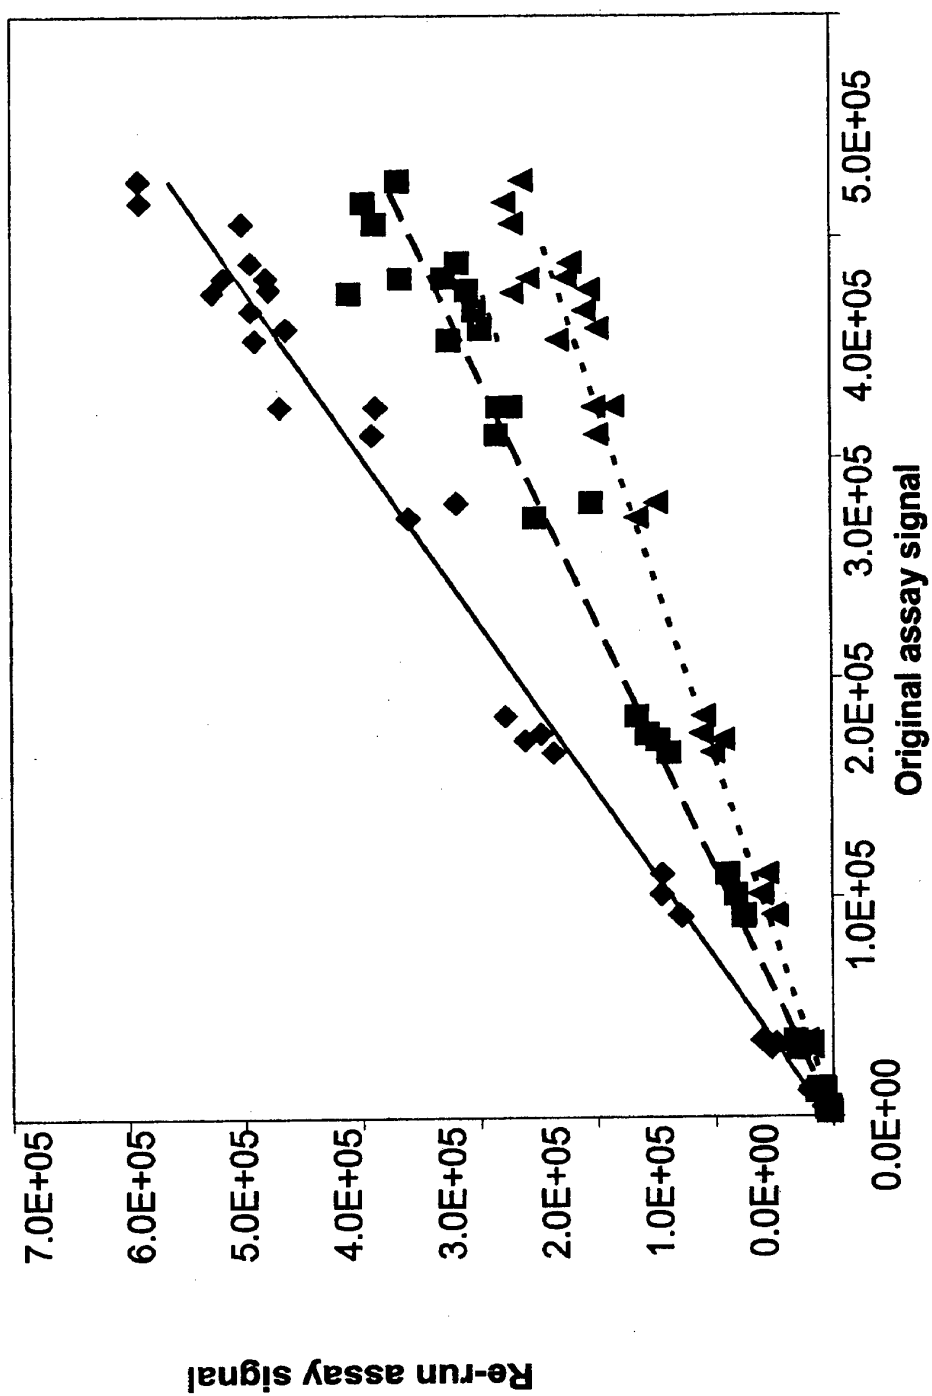


FIGURE 21

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 2007002579 A [0008]
- US 2007224084 A [0008]

Non-patent literature cited in the description

- **GIBBONS I et al.** *Clin. Chem.*, September 1989, vol. 35 (9), 1869-1873 [0008]

专利名称(译)	模块化护理点设备及其用途		
公开(公告)号	EP2205968B1	公开(公告)日	2013-11-20
申请号	EP2008836072	申请日	2008-10-02
[标]申请(专利权)人(译)	赛拉诺斯股份有限公司		
申请(专利权)人(译)	THERANOS INC.		
当前申请(专利权)人(译)	THERANOS INC.		
[标]发明人	BURD TAMMY GIBBONS IAN HOLMES ELIZABETH A FRENZEL GARY NUGENT ANTHONY JOSEPH		
发明人	BURD, TAMMY GIBBONS, IAN HOLMES, ELIZABETH A. FRENZEL, GARY NUGENT, ANTHONY JOSEPH		
IPC分类号	G01N33/48 G01N33/53		
CPC分类号	B01J19/0046 B01J2219/00283 B01J2219/00292 B01J2219/00315 B01J2219/00369 B01J2219/00371 B01J2219/00385 B01J2219/00466 B01J2219/00495 B01J2219/005 B01J2219/00693 B01J2219/00702 B01L3/021 B01L3/0262 B01L3/5025 B01L3/527 B01L2200/04 B01L2200/0689 B01L2200/141 B01L2200/148 B01L2300/0654 B01L2300/0829 B01L2300/1805 B01L2400/043 G01N35/028 G01N2035/0097 A61B10/0038 A61B10/0045 A61B10/0051 A61B10/0058 A61B10/007 A61B10/02 A61B2010/0074 A61B2010/0077 B01L9/543 G16H10/40 G01N33/5302 G01N33/54386 G01N2333/4737 G01N2333/71 Y10T29/49826 Y10T436/25375 C12M1/02 C12M1/266 G01N33/48 G01N33/50 G01N33/5091 G01N33/53 G01N35/02 G01N35/08 G01N35/10 G01N37/00 A61B5/15 A61B5/150755 A61B5/151 B01L7/52 B01L7/5255 G01N1/38 G01N33/5304 G01N33/54326 G01N33/54366 G01N33/56966 G01N33/57484 G01N33/6803 G01N33/94 G01N35/00732 G01N35/00871 G01N35/1065 G01N35/1074 G01N2035/00237 G01N2035/00851 G01N2035/00881 G01N2035/1032 G01N2035/1034 G01N2035/1048 G01N2333/475 G01N2333/912 G01N2333/91205 G01N2333/9129 G01N2800/26 G01N2800/60		
代理机构(译)	COLE , WILLIAM格温		
优先权	60/997460 2007-10-02 US		
其他公开文献	EP2205968A1 EP2205968A4		
外部链接	Espacenet		

摘要(译)

本发明提供了在护理点使用的装置和系统。本发明的方法装置涉及自动检测体液中的分析物。该装置的部件是模块化的，以允许使用所公开的方法用于各种医疗应用的灵活性和稳健性。

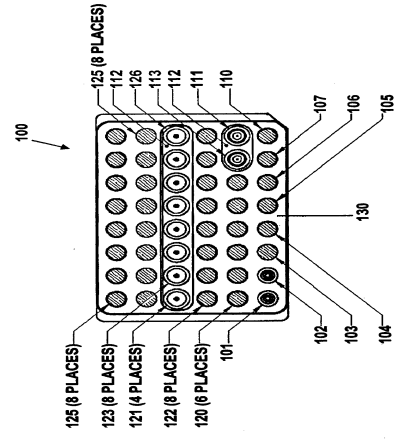


FIGURE 1