

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
11 September 2009 (11.09.2009)

(10) International Publication Number
WO 2009/111254 A2

(51) International Patent Classification:
G01N 33/53 (2006.01)

(21) International Application Number:
PCT/US2009/035222

(22) International Filing Date:
26 February 2009 (26.02.2009)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/067,756 29 February 2008 (29.02.2008) US

(71) Applicant (for all designated States except US):
BIOMEDOMICS, INC. [US/US]; 6 Davis Drive, Research Triangle Park, NC 27709-2076 (US).

(72) Inventor; and

(75) Inventor/Applicant (for US only): **WANG, Xue-Feng** [US/US]; 6 Davis Drive, Research Triangle Park, NC 27709-2076 (US).

(74) Agent: **JOYNER, Charles**; 7515 Johnson Mill Rd., Bahama, NC 27503 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ,

CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- of inventorship (Rule 4.17(iv))

Published:

- without international search report and to be republished upon receipt of that report (Rule 48.2(g))



WO 2009/111254 A2

(54) Title: A RAPID AND SENSITIVE METHOD FOR QUANTITATIVE DETERMINATION OF THE LEVEL OF HEP-ARIN-PF4 COMPLEX INDUCED IMMUNOGLOBULIN ANTIBODIES

(57) Abstract: Disclosed herein is a lateral flow immuno-assay system capable of rapidly, cost effectively, and quantitatively detecting and assessing the level of HIT antibodies in body fluids of a patient. Also taught are methods for employing the system to assist in diagnosis of HIT, and for screening or detecting a changing titer of HIT antibodies in the body fluids of a patient to determine susceptibility toward HIT.

A RAPID AND SENSITIVE METHOD FOR QUANTITATIVE
DETERMINATION OF THE LEVEL OF HEPARIN - PF4 COMPLEX
INDUCED IMMUNOGLOBULIN ANTIBODIES

BACKGROUND OF THE INVENTION

5 An animal's immune system provides a stream of protein molecules know as antibodies that circulate through the animal's blood stream. When large toxin molecules or microorganisms, known as antigens, enter the blood stream, the immune system, through a complex biochemical sequence, recognizes that the antigens are foreign to the animal's system, and hence, a threat. In response to
10 the invasion of antigens, the immune system rapidly produces "customized" antibodies that attach themselves to the specific site on the antigen. The attached antibodies act as markers to identify the antigens or other material produced by the immune system, which in turn destroy the antigens.

 Because antibodies are extremely specific; selective; and sensitive, and
15 relatively easy to generate, scientists have recognized that they can be the basis for a variety of useful tests known as immunoassays. In its basic form, an immunoassay for a specific antigen involves allowing a test sample of material of unknown composition, an analyte, to come in contact with immobilized antibodies that bind to the specific antigen. If the antigen is present, it will bind, *i.e.* conjugate,
20 with the antibodies and also become immobilized. The immobilized antibodies are washed to remove any free analyte, and then treated with labeled antibodies that bind to a different site on the antigen than the immobilized antibodies. If the antigen in question was present in the analyte, it will now be conjugated to the labeled antibodies and also to the immobilized antibodies. Presence of the antigen
25 can be detected by sensing the label.

 Typically, labels have distinct signatures detectable by electromagnetic radiation absorption, emission, or both. A particularly useful technique is to use labels that are florescent. That is, they absorb electromagnetic radiation above the frequency range of visible light then instantly emit visible light. The strength of the
30 absorption or emission can be directly correlated to the amount of label, and hence the antibody being observed. Alternatively, a label detectable by electronic means

may be used. For example, the label may impede a radio frequency signal and the amount of impedance detected by electronic means.

Thus, Immunoassays are tests that take advantage of the specific binding of an antibody to its antigen and are discussed and illustrated in most University level
5 biochemistry textbooks. For example, see L. Nelson, *et al.*, *Lehninger Principles of Biochemistry*, 3rd Ed., 231 – 233, Worth, NY (2000) and L. Stryer, *Biochemistry*, 4th Ed., 60 – 63, W. H. Freeman, NY (1995). The main characteristic of immunological techniques is the appropriate labeling of the antibody or the antigen. This label helps create a signal that correlates with the immunoreaction and allows the
10 detection of the analyte of interest. In laboratory assays, various wash steps are required to remove free labeled or unlabeled reactants and allow the detection of the analyte by the bound and labeled reactants. Test results may be quantified by comparison to a calibration curve established by a previously run series of assays using known amounts of analyte.

15 A widely practiced form of immunoassay is the enzyme-linked immunosorbent assay (ELISA); *supra*, Nelson, *et al.*, and Stryer. There are many variations of ELISA's, most of which require multiple steps and a moderate to extensive skill level to execute. However, one category of immunoassay, *i.e.* the well-known lateral flow immunoassay (LFIA), of which home pregnancy tests are an
20 example, are simple, typically requiring only one step, and requiring no technical sophistication to perform. Thus, LFIA can be easily performed by non-trained users and used on-site during sample collection. The simplicity of the tests paired with their quick return of results (2–15 minutes), means that testing is cost-effective. LFIA represent an appropriate point-of-care (POC) and field-use technology that
25 can be applied to a broad range of applications. Despite the advantages of LFIA, they are often limited to simple screening applications. This is because LFIA's, in their present form, are not easily quantifiable and are not sensitive enough for certain applications.

Each year millions of patients, about a third of those hospitalized, are
30 exposed to heparin. About 1% to 5% of these heparin-exposed patients develop a severe complication known as heparin-induced thrombocytopenia often referred to as "HIT". Venous or arterial thrombosis is among the effects of HIT, and in patients

suffering from acute thrombosis, HIT may be fatal. After discontinuation of heparin in patients with HIT, the platelet levels generally return to normal. Therefore, timely and accurate diagnosis of HIT can alleviate pain and even prevent death. See Arapally *et al*, *N Engl J Med*, 355; 8: 809.

5 The immunoglobulin antibodies, such as IgG, IgA, IgE, or IgM antibodies, that develop after five or more days of heparin therapy appear to cause HIT. These antibodies differ from those associated with other forms of drug-induced thrombocytopenia in that, in the presence of optimal concentrations of heparin, they activate blood platelets. This activation causes the platelets to release the contents
10 of their storage granules and to undergo membrane changes that create sites for the binding of a coagulation factor, fibrinogen, normally present in plasma (B. H. Chong, et al., *Br. J. Haematol.*, **64**: 347 (1986)). Heparin first binds to platelet factor 4 (PF4), which arises during heparin treatment, to form a highly immunogenic complex on the surface of platelets. Next, in susceptible patients, immunoglobulin,
15 *e.g.* IgG, IgA, IgE, or IgM antibodies to the antigenic heparin-PF4 complex develop that bind with the complex to activate platelets *via* Fc receptors on the surface of the platelets (M. F. Cooney, *Critical Care Nurse*, **26**, 6: 30(2006)).

Several HIT diagnostic procedures and assays are reported in the art, but each has drawbacks that limits its use in accurately, rapidly, reliably, and cost
20 effectively diagnosing the risk of HIT. For example, US patent 5,972,717 teaches an ELISA type immunoassay. However, while ELISA procedures and assays are suited for laboratory environments, they are not well suited for POC use because of their complexity and the requirement for skilled operators. In practice, an ELISA requires 3-4 hours of skilled technician time and typically involves turnaround times
25 of one day to one week.

SUMMARY OF THE INVENTION

There is a need for a sensitive, accurate, reliable, quantitative, cost effective, rapid, and easy to use assay for point of care application to assist in the diagnosis
30 of HIT, and the invention described herein fulfills that need in all its aspects. The present HIT immuno-flow type assay in its various forms includes, but is not limited to, lateral flow immuno-assays and flow-through assays.

A first aspect is a method wherein the level of heparin - PF4 complex induced immunoglobulin antibodies in a patient is determined by direct measurement with a point-of-care immuno-flow assay system, in particular, a lateral-flow immunoassay system. A first embodiment of the first aspect is a method of quantitatively determining a body fluid level, *e.g.* blood, or component thereof, of heparin - PF4 complex induced immunoglobulin, *e.g.*, IgG, IgA, IgE, or IgM antibodies by a point-of-care lateral-flow immunoassay system. A second embodiment of the first aspect is a method for detecting a changing titer of heparin - PF4 complex induced immunoglobulin antibodies in a patient by multiple applications over time of the first embodiment.

A second aspect of the invention is a point-of-care immuno-flow assay system, in particular, a lateral-flow immunoassay, for quantitatively measuring, directly or indirectly, heparin - PF4 complex induced immunoglobulin antibodies level in a patient. A first embodiment of this aspect is an immuno-flow assay system for directly determining body fluid, *e.g.* blood, or component thereof, level of heparin - PF4 complex induced immunoglobulin antibodies in a patient. A second embodiment is a point-of-care lateral-flow immunoassay system for quantitatively determining, directly or indirectly, in a body fluid, *e.g.* blood, or component thereof, level of heparin - PF4 complex induced immunoglobulin antibodies in the patient.

20 BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 schematically depicts the elements assay strip of the lateral-flow immunoassay system of the invention.

Figure 2 schematically depicts the assay strip of the invention at the completion of the assay.

25 Figure 3 schematically depicts a lateral-flow immunoassay system reader with associated equipment.

DETAILED DESCRIPTION OF THE INVENTION

LFIA's are widely known in the scientific and patent literature relating to diagnostic assays. See, David Carlberg, "Lateral-flow Assays: Designing for

Automation,” *IVD Technology*, (Cover Story) May 1999. Compared with other immunoassay formats such as ELISA’s, the major advantages of LFIA’s are their ease of use, because aside from the dispensing of the sample, no additional sample or reagent handling steps are usually necessary. In a lateral-flow assay system, antibody-antigen reactions, as well as the removal of excess reactants, takes place by chromatographic separation driven by capillary forces. The detector reagent (i.e., the labeled antibody) and the sample wick through the pads or membranes of the test strip. At a capture line, *i.e. test line*, the detector reagent interacts with the capture reagent, which has been immobilized on the membrane. The test result is then evaluated visually, typically by two lines—a test line and a reference line.

When a patient is being treated with heparin, *e.g.* as part of a surgical procedure, the assay system of the present invention is a convenient means of monitoring the patient’s blood, or other body fluid, level of heparin - PF4 complex induced immunoglobulin antibodies to determine if the patient has HIT or is susceptible to HIT. The LFIA and associated device taught herein, because of simplicity, robustness, and rapid completion time are well suited for point of care clinical use.

As used herein, the term “point of care” (POC) refers to a medical diagnostic procedure (as well as the means for its executing) that is particularly adapted for use in the immediate vicinity of the patient being treated. For example, during a surgical procedure, the present invention may be conveniently employed within the operating room in order to fully capitalize on its ease of use and rapid turn-around time. However, the skilled artisan will appreciate that the POC assay of the present invention may also be used to advantage in a wide variety of other settings. For example, it may be used in large central clinical laboratories and well as small physician office and community hospital laboratories. Further, it is well suited for military medicine in a field environment.

Relative to other immunoassays for antibodies which indicate possible onset of HIT, the present invention uniquely combines the attributes of fast turnaround (<30 minutes), quantitative capability, high sensitivity, and cost effectiveness. The combination of these benefits makes practical the new applications of: 1) pre-

screening patients for HIT antibodies prior to administering heparin in the current clinical setting and 2) tracking a changing titer of HIT antibodies

Pre-screening is generally not done with today's slow turnaround and costly tests. However, patients may carry antibodies from heparin exposure in previous hospital stays; their records and/or personal memory or knowledge may not record such exposure. The time to onset of thrombocytopenia after the initiation of heparin in patients with no previous heparin exposure or remote exposure (more than 100 days) normally occurs 5-10 days after heparin exposure, and thus the ELISA test is normally five days after heparin exposure. However, thrombocytopenia it may occur in hours in a patient with a history of recent (last 100 days) exposure to Heparin from a previous hospital stay (Arapally et al, N ENGL J MED 355; 8: 809). The rapid, cost effective, quantitative POC assay of the present invention may be used for pre-screening patients to avoid HIT by reliably informing the attending physician of the level of circulating HIT antibodies. That is, the attending physician may choose not to prescribe heparin if the HIT antibody level is above a certain point.

As a cost effective and rapid turnaround, yet *quantitative*, POC test, the assay system of the invention can be employed as a daily or more frequent *series*, to inform physicians of a changing concentration of HIT antibodies which are approaching but have not reached the numeric (optical density) value considered to be a HIT "positive" test. Physicians would be enabled to take appropriate corrective action, e.g. switching to alternative anticoagulants, prior to a positive test confirming HIT onset. Moreover, the *rate* of change discernable from multiple rapid turnaround tests is informative and similarly actionable information for physicians. Finally, the rapid, quantitative and low cost test series could enable physicians to track the rising titer prior to or concurrent with observation of clinical indications of HIT rather than following such observation, as is the current clinical practice (*Vide supra*, Arapally et al, 813, regarding current clinical practice), again potentially enabling earlier corrective action.

The skilled artisan will appreciate that a quantitative assay may also be used as a qualitative or semi-quantitative assay. The present invention may be used in a qualitative mode to answer the simple question, "Are *any* HIT antibodies detected in the sample?" with a simple, positive or negative answer. Likewise, if

any HIT antibodies are detected, the present invention can return a semi-quantitative response such as “a small amount, a moderate amount, a large amount, or an extremely large amount. There may be occasions when less than a full quantitative reading will suffice.

5 For the following description of the invention, readers will find it convenient to have Figures 1 - 3 before them.

Figure 1 is a schematic depiction of the assay strip LFIA **01** of lateral-flow immunoassay system of the present invention. LFIA **01** comprises a rigid or semi-rigid backing **03**, *e.g.* plastic or glass, which supports membrane layer **05**, that is an inert,
10 fibrous material capable of supporting movement of liquids by capillary action, and under certain conditions, binding biologically derived molecules such as proteins or antibodies. An example of such a fibrous material is nitrocellulose, which is widely used as LFIA membrane material. Optionally, membrane layer **05** may be comprised of one or more layers that may be of the same or different compositions. In the art of lateral-flow
15 immunoassay systems, a strip of membrane, *e.g.* membrane layer **05**, on a plastic support is often referred to as a “card” and membrane cards of various compositions are commercially available.

Membrane layer **05** is zoned into functional areas referred to herein as sample pad **07**, conjugate zone **09**, test line **11**, reference line **13**, and wicking pad **15** arrayed in
20 the order shown in Figures 1 and 2. Conjugate zone **09** and test line **11**, test line **11** and reference line **13**, and reference line **13** and wicking pad **15** are separated by flow zones. Optionally, sample pad **07** may be enhanced with features that promote the efficiency and accuracy of binding in LFIA **01**. For example, sample pad **07** may be
25 fitted with a blood preparation means so that whole blood may be converted to a form more amenable for LFIA analysis such as serum. If a body fluid other than blood is the sample, analogous preparation means may be employed to make that fluid amenable for LFIA analysis. Additionally, sample pad **07** may be supplied with preserving, stabilizing, flow promoting, and buffering agents. Sample pad **07** may be layered on top of membrane layer **05** or may be integrated into this membrane.

30 Conjugate zone **09** contains a means for labeling HIT antibodies that may be present in the sample for which LFIA **01** is intended to assay, so that the labeled

antibodies can be detected optically or electronically at the conclusion of the assay. Conjugate zone **09** is supplied with labeled molecules of an antibody binding ligand, such as recombinant protein A affixed with a label, "labeled protein A **19**" (shown symbolically in Figures 1 and 2 as "**A***"). The label is detectable by emission or
5 absorption of electromagnetic radiation, electronic means, other means employed in the immuno-assay art, such as enzyme labeling and substrate development. Suitable labels include materials that fluoresce, phosphoresce, or otherwise emit or absorb radiation. Conveniently, intensely colored, *e.g.* nano scale latex or gold, particles are useful as labels in the present invention. Optionally, conjugate zone **09** may be integrated into
10 sample pad **07**.

Test line **11** and reference line **13** are zones delineated on the fibrous material that comprises membrane layer **05**. Immobilized on the strip of membrane layer **05** that forms test line **11** is heparin - PF4 complex **21** capable of reacting with the immunoglobulin HIT antibodies **20** that may be present in the sample of body fluid, such
15 as blood, or a component thereof, subjected to assay using LFIA **01**. The immunoglobulin HIT antibodies **20** (represented in Figure 1 as "**Y_{HIT}**") may be typically IgG, IgA, IgE, or IgM induced by heparin-PF4 complexes in the body of a patient.

Immobilized on the strip of membrane layer **05** that forms reference line **13** is a second antibody binding ligand capable of reacting with antibody binding ligand in
20 conjugate zone **09** (as noted above, "labeled protein A **19**"). Thus, reference line **13** is comprised of a) antibodies that bind to protein A, b) antibodies that recognize antibodies bound to the labeled protein A, or c) a ligand that binds directly or indirectly the label and are designated collectively herein as "binding reagent A **22**." In Figure 1, label binding reagent A **22** is noted as "**Y_A**".

25 The assay using LFIA **01** is initiated by placing onto sample pad **07** (indicated in Figure 1 by the heavy arrow) a sample, typically a drop, of body fluid, such as blood, or a component thereof, *e.g.* plasma and serum, hereinafter "sample **23**", suspected of containing immunoglobulin HIT antibodies **20**. As the liquid components of sample **23** flow by capillary action into the region of conjugate zone **09**, immunoglobulin HIT
30 antibodies **20** contained in the sample conjugatively bind to the molecules of labeled protein A **19** to form antibody complexes **25** (shown symbolically in Figure 1 as "**Y_{HIT}A***"). That is, antibody complexes **25** are comprised of immunoglobulin HIT antibodies **20**

bound to molecules of labeled protein A **19**. Antibody complexes **25** move out of conjugate zone **09** by capillary action through membrane **05** and advance toward test line **11** (schematically illustrated in Figure 1 by a dashed arrow).

In Figure 3, complexes **25** have migrated to test line **11**, where they become
5 bound to units of heparin - PF4 complex **21** and are trapped as antibody complexes **27** at test line **11**. In Figure 2, antibody complex **27** is symbolically represented as "H-PF4-Y_{HIT}A*". Thus, at test line 11 complex **27** may be detected by the visualization of labels that were part of antibody complexes **25**

Those molecules of labeled protein A **19** that do not bind to test line **11** continue
10 to move through membrane layer **05** to the reference line **13**. As noted above, immobilized at reference line **13** are ligands that can directly or indirectly bind the label **22** that are capable of binding to molecules of a labeled protein A **19** to form complex **28** shown as "A*-Y_A" in Figure 2. Therefore, labeled protein A **19** that not conjugated to immunoglobulin HIT antibodies **20** in sample **23** to form antibody complexes **25**, and
15 hence, immobilized at test line **11**, are now immobilized at reference line **13** in complexes **28**.

Absorption or emission of electromagnetic radiation or enzymatic detection at reference line **13** indicates that the test has been completed and is valid. For example, appearance of the label affixed to labeled protein A **19** at reference line **13** and also
20 appearance of the label at test line **11** indicates that the test is complete and there is some immunoglobulin HIT antibodies **20** in the sample. Conversely, no appearance of the label at test line **11**, but appearance at reference line **13**, indicates there is no immunoglobulin HIT antibodies **20** in the sample or the amount is below the sensitivity of the assay. No appearance of the label at either test line **11** or reference line **13** indicates
25 either the assay is not complete or it is faulty in some manner and should be repeated. Any materials not immobilized at test line **11** or at reference line **13** continue to move through membrane layer **05** and are absorbed into wicking pad **15**. At this point, the assay is fully developed and may be analyzed.

Conveniently, LFIA **01** may be housed in a cassette that protects it and facilitates
30 its handling and analysis. Such protective cassette, usually constructed of a polymeric material, are provided as an integral part most commercially available LFIA units, and

the utility of a protective cassette is widely taught in the technical and patent literature. Typically, a LFIA protective cassette provides at least one port for introducing a sample to be assayed and one or more windows for viewing and reading test and reference lines. For example, see David Carlberg, "Lateral-flow Assays: Designing for Automation,"
5 *IVD Technology*, (Cover Story) May 1999. A LFIA protective cassette may also be configured to facilitate proper orientation in an electro-optical reader. Further, a LFIA protective cassette may be imprinted with useful indicia, such as directions for use, warnings, and bar codes for identification.

A series of samples having identical volume with varying, but known, amounts
10 immunoglobulin HIT antibodies **20** are assayed using the LFIA 01 described above. A curve or standardized chart defining the relationship of the amount of immunoglobulin HIT antibodies **20**, present in the samples and the level of absorption or radiation detected at the test line is established. The result of an assay of a sample having an unknown amount of immunoglobulin HIT antibodies **20** is compared with the
15 standardized chart to determine the amount of analyte in the sample thereby enabling the LFIA of the present invention to quantitatively determine the level of immunoglobulin antibodies in a sample of a given volume.

Figure 3 schematically depicts a means for reading, *i.e.* analyzing, the developed assay. The developed assay may be read by visual comparison of the density of the
20 test line with a standardization chart described above. However, reading by an electro-optical device schematically illustrated in Figure 3 and described below is much preferred because of the greater sensitivity and consistency offered by such devices. Further, such electro-optical devices may be configured to yield a digital output that may serve as an input to other computer systems for long term storage and extensive data
25 analysis.

Turning to Figure 3, electro-optical reader **102** is comprised of electro-optical sensor **104** in communication with electronic signal processor **106**, which in turn is optionally in communication with interpretation means **108**. A developed LFIA **01** (described above and illustrated in Figures 1 -2) is inserted into electro-optical sensor
30 **104** of reader **102** where a source of electromagnetic radiation, typically light source **110**, illuminates the test line **11** (Figures 1 - 2) of LFIA **01**. Typically, LFIA **01** will be housed in a protective cassette, which assists in optimally orienting the LFIA **01** within

electro-optical sensor **104**. Light source **110** may be an emitter of IR, visible, or UV light. Light absorbed by the test line **11** is directly proportional to the density of the test line, and thus, proportional to the amount of the immunoglobulin antibodies (shown as **20** in Figure 1) that were present in the test sample (**23** in Figure 1). Therefore, the light
5 reflected from the test line **11** is indirectly proportional to the light absorbed. That is, the more light absorbed by test line **11**, the less light is reflected.

To receive electromagnetic radiation reflected from test line **11** is an electromagnetic radiation detector **112**. If the electromagnetic radiation is light, *e.g.* IR, visible, or UV, the detector **112** might be a photo cell, camera, CCD line scanner, or
10 other light sensing device positioned to sense light reflected from test line **11**. Detector **112** may be comprised of a single or multiple units, and it includes any associated electronic circuitry such as power supplies, amplifiers, and data processing units. Conveniently, lens **114a** focuses light onto test line **11** while lens **114b** focuses the light reflected from test line **11** onto detector **112**. In cases where the detection mode is fluorescence,
15 detector **112** receives light that fluoresces from test line **11** rather than reflected light. Further, in the fluorescence mode, the light illuminating test line **11** may be in the visible or UV range.

Detector **112** is in communication with signal processor **106**. For example, detector **112** generates an electric voltage proportional to the light it senses, and that
20 voltage is transmitted by a suitable means such as shielded cable to signal processor **106**. Signal processor **106** converts the voltage, *i.e.* the signal, received from detector **112** into a form that can be perceived by human senses. Typically, signal processor **106** displays the signal from detector **112** in a visual analog or digital form, *e.g.* a meter, digital numerical readout, or printer.

25 The display from signal processor **106** may be read directly by a human operator and compared with a previously prepared calibration chart (described above) to determine the amount of immunoglobulin antibodies **20** in the sample of blood. Optionally, signal processor **106** may be in communication with interpretation means **108**, which is a data processing means, *e.g.* a computer, that may be programmed to
30 automate the process of reading the output from signal processor **106** and comparing that reading with a calibration chart to determine the level of immunoglobulin antibodies **20**.

Interpretation means **108** may be programmed to signal the health care providers by visual and / or audio means **116** that there is a rising titer of immunoglobulin antibodies **20**. Interpretation means **108** can store results of multiple tests over time, which is a useful data base for both patient care and medical research. Further, as a particular advantage, when the results are recorded in digital form, such result can be sent by electronic means **118** in “real time” *via*, phone or internet, directly to consulting health care providers even if they are at remote locations.

Any means known in the art for detecting labels on antibodies such as detection of electromagnetic absorption, emission, or both; or detection by electronic means may be used in the invention. For example, labels that absorb visible light may be visualized directly by eye or indirectly by an electro-optical device are frequently employed as are labels that are fluorescent under UV light or visible light. In some applications, phosphorescent labels may be employed.

Biosensors are devices that detect an analyte that combines a biological component (*e.g.* tissue, enzymes, antibodies, and nucleic acids) with a physicochemical element (*e.g.* optical or piezoelectric) in association with electronic circuitry. Biosensors can be related to nanotechnology such as nanotube based sensing. Herein biosensors and associated components are collectively referred to as “electronic means of analyte detection.”

In addition to determining the level of heparin –PF4 complex induced immunoglobulin antibodies the assay of the present invention may be configured to concurrently quantitatively detect one or more other bio-markers in the body fluid of a patient. Examples of such bio-markers include, but are not limited to antibodies, DNA, proteins, toxins, and complex factors. For example, the assay may be configured to concurrently detect level of D-dimer.

Preparation and employment of the invention will be further understood from the following non-limiting examples. The reader will find it helpful to refer to Figures 1 - 3 as well as the corresponding description of those figures presented above.

EXAMPLES

Summary

A mixture of modified PF4 is incubated with heparin to form a PF4 heparin complex, hereafter referred to as the "Complex," which is striped onto a supported nitrocellulose membrane such as membrane **05** where it binds to form a test line, such as test line **11**. A clinical sample of a body fluid, such as blood, or a component thereof, is applied to a sample pad, e.g. sample pad **07**, comprising reaction conditioning reagents. Antibodies within the sample are labeled by the rehydration of recombinant protein A affixed to colored latex particles also contained on the sample pad or in a separate conjugation pad zone, e.g., conjugation zone **09**. The labeled sample migrates across the nitrocellulose membrane. If the sample contains anti-complex antibodies, these antibodies bind to the complex and a measurable signal is produced in proportion to the concentration of antibodies specific for the complex. Antibodies not captured at the test line are subsequently captured by molecules of protein A at the reference line, e.g. reference line **13**, or they migrate and onto an absorbent pad material, e.g. wicking pad **15**.

EXAMPLE 1

Preparation of the Complex:

Heparin (HP), 40 ul of 1000 U/mL, in phosphate buffered saline (PBS, Fisher Scientific PN: BP665-1) is mixed with 94 ul of PF4 (1.4 mg/mL, HPF, BioMedomics) and 56 ul of water, then incubated at room temperature for 30 minutes to yield the Complex mixture. The Complex mixture is then mixed with stabilizing agents by adding 4 ul of 50% sucrose (Fisher PN: S5) with 4 ul of 25% trehalose (Sigma PN:T9449) and 2 ul of 1M TAPS buffer (Sigma PN: T5441, pH 9.0).

EXAMPLE 2

Preparation of the Membrane

The Complex mixture described above is striped onto a Millipore Hi-Flow mylar backed nitrocellulose membrane (25 mm wide, SHF0900425) affixed to an adhesive backed card (polystyrene 59 mm by 305 mm from GML or equivalent) at

.075 ul/mm using an Imagene Isoflow striper (or equivalent) at 45 mm/second under conditions described by the manufacturer's user manual to create a test line, The test line is proximal to the sample pad at a position to be determined by the cassette holder assembly and, if employed, corresponding position for a reader..

- 5 Simultaneously, a reference reagent comprising of 0.25 mg/mL of recombinant protein A (Repligen PN: rPA-50) is mixed with 1% sucrose/0.5% trehalose/10 mM TAPS pH 9.0 (as was done with the Complex mixture) and striped at .075ul/mm at 45 mm/second at the same time as the Complex, but at a position upstream of the test line as designated by the reader and/or cassette holder assembly to create a
10 reference line. The striped membrane is then baked at 56°C for one week.

EXAMPLE 3

Preparation of the Protein A Latex Particles

- Dark blue carboxy-latex particles, "beads," (Bangs Beads, DC02B, 0.33 micron or equivalent), 10% in 100 ul, are covalently coupled by washing the beads
15 with 50 mM MES (Sigma PN:M3885) pH 4.5, adding 1 mL of a fresh preparation of 10 mg/mL EDAC (Sigma PN:E1769) in 50 mM MES, pH 4.5, incubating for 30 minutes at room temperature. The resulting material is pelleted in a centrifuge at 13.4K x g for 5 minutes, the pellets washed with 50 mM MES pH 4.5, re-suspend (with sonication in water bath using Branson desktop sonicator) with 1 ml of
20 0.65mg/mL recombinant protein A in 1x PBS, vortex, sonicate, and, finally, incubated at RT overnight. Next, 100 ul of 10% BSA (Proliant Biologicals PN: 68100 or equivalent)/100xTE (Fisher PN: BP1338), is vortex sonicated, and incubated at RT for at least 1 hour. The beads are centrifuged to form pellets, which are washed with 1 mL PBS. The wash step is repeated three times to
25 remove unbound protein A and excess blocker ingredients. After re-suspending the recombinant protein A (rPA) beads in 1 mL of 4% sucrose/0.05% sodium azide (Sigma), they are stored under refrigeration until needed.

EXAMPLE 4

Preparation of Sample Pad

- 30 A glass fiber pad (Ahlstrom 8964 or equivalent) is saturated with a mixture of 1% ethylenediamine tetrakis(propoxylate-block-ethoxylate) tetrol (Sigma PN:

4335539) surfactant, 0.8% sodium casein (Sigma PN:C8654), and 5x TE. The resulting product is maintained at 56°C until dry. Once dry, a mixture of 2.5% v/v of the rPA beads (prepared above) in a solution of 5% sucrose/2.5% trehalose/5x TE is prepared and sprayed onto the sample pad proximal to one end at 3 ul/mm using
5 the Imogene Isoflow airbrush set to 4-5 psi at a height of 5-7 mm at a dispense rate of 75 mm/second. The labeled sample pads are dried overnight at 56°C, and stored in desiccated bags.

EXAMPLE 5

Preparation of Strips

10 After baking, the Complex striped nitrocellulose cards are assembled into the test strips by adding the labeled protein A samples pads. This can be done by removing the release liner from the lower portion of the adhesive backed card proximal to the test line side containing the Complex, and firmly pressing the
sample pad onto the adhesive area whereby 2 mm of the sample pad overhangs
15 onto the striped nitrocellulose cards. An absorbent pad, such as Ahlstrom 222 is cut, the release liner removed from the adhesive card backing proximal to the reference line striped on the nitrocellulose, and pressed onto the adhesive backing whereby 2 mm of the absorbent pad overhangs the nitrocellulose membrane. The test card can now be cut into convenient size test strips, usually 4-5 mm depending
20 upon the plastic cassette housings employed, using a Kinematic Matrix Model # 2360 (Terra Haute, CA) guillotine cutter or equivalent.

EXAMPLE 6

Assembly of Assay System

25 Test strips are placed into plastic cassette holders usually custom designed for the particular reader. The cut test strips are taken and placed in the lower portion of the cassette with the sample pad side at the bottom of the cassette. The top portion of the plastic housing is positioned over the test strip whereby the sample chamber is above the lower portion of the sample pad and the top is pressed into place. The assay is ready to use and can be stored and desiccated in
30 polyfoil bags until needed at room temperature. Note also that a blood separation membrane may be employed above the sample pad to filter whole blood cells

thereby conveniently allowing plasma to flow onto the pad. Separation membranes are commercially available, *e.g.* from Millipore, and are commonly used by those skilled in the art.

EXAMPLE 7

5

Testing and Assay Usage

The clinical sample is brought to room temperature. The plastic housing containing the test strip is placed onto a flat surface at room temperature. After adding 75 ul (or other volume depending upon the width of the test strip) to the sample well, a timer is started, and the test results read at 30 minutes. If a visual
10 test line can be seen anytime after about 5 minutes, the test is considered positive. The test results should not be read past 40 minutes because results will change due to sample evaporation.

What is claimed is:

1. A method of assisting in the diagnosis of heparin induced thrombocytopenia, in a patient, comprising quantitatively determining if a body fluid level of heparin – PF4 complex induced immunoglobulin antibodies in the patient is above a predetermined range using a point-of-care immuno-flow assay system.
5
2. The method of Claim 1 wherein the body fluid is blood or a component thereof.
3. The method of Claim 1 wherein the immunoglobulin antibodies are IgG, IgA, IgE, or IgM antibodies.
- 10 4. The method of Claim 1 wherein the immuno-flow assay system is a lateral flow immuno-assay system.
5. The method of Claim 1 wherein the immuno-flow assay system is a flow through immuno-assay system.
- 15 6. A method of screening a patient for susceptibility to heparin induced thrombocytopenia comprising determining by means of a point-of-care immuno-flow assay system:
 - a) if heparin – PF4 complex induced immunoglobulin antibodies are present in a body fluid of the patient, and
 - b) if the antibodies are present in the body fluid, quantitatively determining
20 the level of the antibodies.
7. The method of Claim 6 wherein the body fluid is blood or a component thereof.
8. The method of Claim 6 wherein the immunoglobulin antibodies are IgG, IgA, IgE, or IgM antibodies.
- 25 9. The method of Claim 6 wherein the immuno-flow assay system is a lateral flow immuno-assay system.

10. The method of Claim 6 wherein the immuno-flow assay system is a flow through immuno-assay system.

11. A method for assisting a physician in assessing a patient's vulnerability to heparin induced thrombocytopenia in a patient being administered heparin or a heparin containing medication comprising:

a) determining a changing titer of heparin – PF4 complex induced immunoglobulin antibodies, judged by a physician to be indicative of a patient's vulnerability, or

b) determining the rate of change of the titer of heparin – PF4 complex induced immunoglobulin antibodies as a function of time, judged by a physician to be indicative of a patient's vulnerability,

by making multiple assays of a body fluid level of heparin – PF4 complex induced immunoglobulin antibodies in the patient over a period of time using a rapid, cost effective, quantitative immuno-flow assay system,

12. The method Claim 11 wherein the body fluid is blood or a component thereof.

13. The method of Claim 11 wherein the immunoglobulin antibodies are IgG, IgA, IgE, or IgM antibodies.

14. The method of Claim 11 wherein the immuno-flow assay system is a lateral flow immuno-assay system.

15. The method of Claim 11 wherein the immuno-flow assay system is a flow through immuno-assay system.

16. A point-of-care immuno-flow assay system for quantitatively determining the body fluid level of heparin - PF4 complex induced immunoglobulin antibodies in a patient.

17. The system of Claim 16 wherein the body fluid is blood or a component thereof.

18. The system of Claim 16 where in the immunoglobulin antibodies are IgG, IgA, IgE, or IgM antibodies.

19. The method of Claim 16 wherein the immuno-flow assay system is a lateral flow immuno-assay system.

5 20. The method of Claim 16 wherein the immuno-flow assay system is a flow through immuno-assay system.

21. The system of Claim 16 that uses electromagnetic radiation absorption, emission, or both as detection means.

10 22. The system of Claim 16 wherein electromagnetic detection means is fluorescence

23. The system of Claim 16 that uses biosensors in association with electronic circuitry as detection means.

24. The system of Claim 23 wherein the biosensors are related to nanotechnology.

15 25 The system of Claim 24 wherein nanotechnology is based on nanotube sensing.

26. A point-of-care lateral flow immuno-assay system for quantitatively determining the level of heparin – PF4 complex induced immunoglobulin antibodies in a body fluid of a patient comprising:

20 a) a linear, membrane of an inert, fibrous material capable of supporting movement of liquids by capillary action and which in turn, is supported by a backing,

25 wherein the membrane from proximal end to distal end is zoned into a sample pad, a conjugate zone, a test line, a reference line, and a wicking pad each optionally separated from its adjacent zone by a flow zone,

b) a means of binding a light absorbing label to heparin – PF4 complex induced immunoglobulin antibodies passing through the conjugate zone, wherein the antibodies were present in a sample of the body fluid on the sample pad,

5 c) a means of immobilizing on the membrane along the test line, heparin – PF4 complex capable of conjugatively binding to heparin – PF4 complex induced immunoglobulin antibodies bound to a light absorbing label passing into the test line,

10 wherein the light absorbing label facilitates the visibility of antibodies bound to heparin – PF 4 complex immobilized at the test line.

27. The system of Claim 26 wherein the body fluid is blood or a component thereof.

28. The system of Claim 26 wherein visibility of the antibodies is facilitated by an electro-optical reading device.

15 29. The system of Claim 26 for quantitatively determining the body fluid level of heparin - PF4 complex induced immunoglobulin antibodies and concurrently, quantitatively determining the body fluid levels of one or more other bio-markers in a patient.

20 30. The system of Claim 29 for concurrently determining the level of heparin - PF4 complex induced immunoglobulin antibodies and the level of D-dimer.

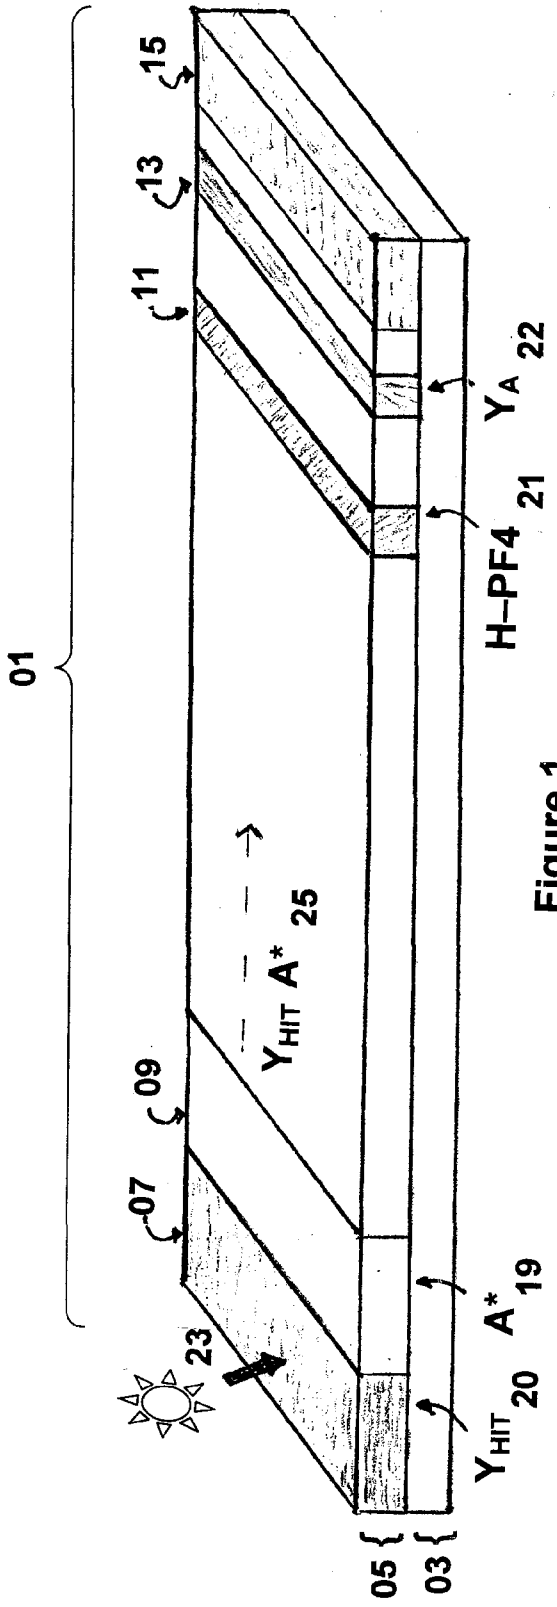


Figure 1

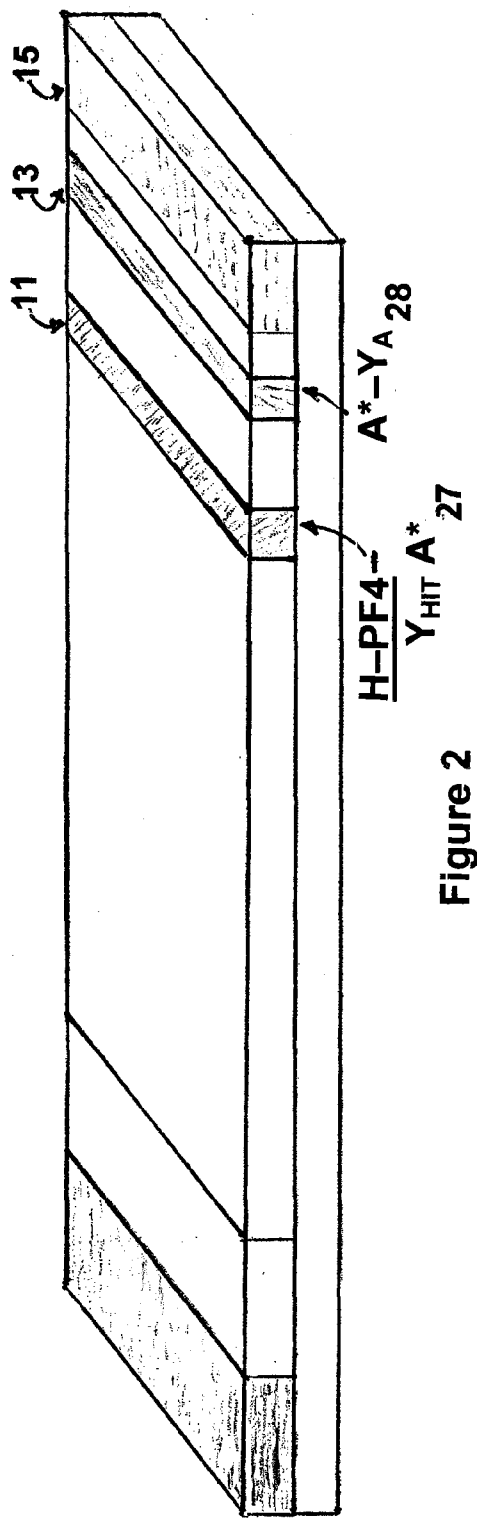


Figure 2

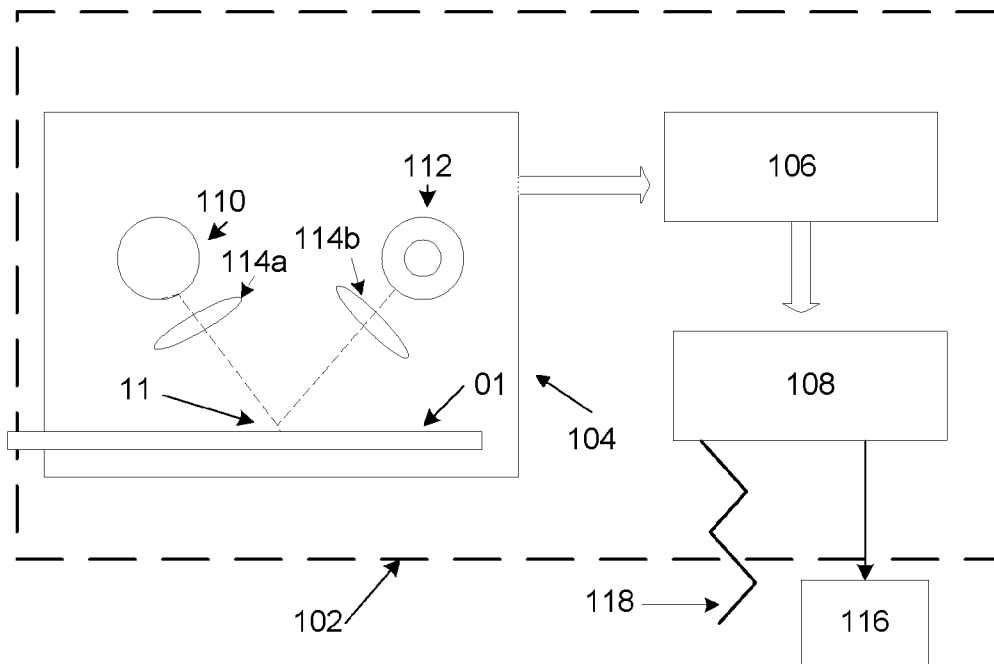


Figure 3

专利名称(译)	一种快速，灵敏的定量测定肝素-PF4复合物诱导免疫球蛋白抗体水平的方法		
公开(公告)号	EP2265948A2	公开(公告)日	2010-12-29
申请号	EP2009717826	申请日	2009-02-26
[标]申请(专利权)人(译)	BIOMEDOMICS		
申请(专利权)人(译)	BIOMEDOMICS INC.		
当前申请(专利权)人(译)	BIOMEDOMICS INC.		
[标]发明人	WANG XUE FENG		
发明人	WANG, XUE-FENG		
IPC分类号	G01N33/53 G01N33/543		
CPC分类号	G01N33/86 G01N2333/522 G01N2400/40 G01N2800/222 Y10S435/97		
优先权	61/067756 2008-02-29 US		
其他公开文献	EP2265948A4		
外部链接	Espacenet		

摘要(译)

本文公开了一种侧流免疫测定系统，其能够快速，成本有效且定量地检测和评估患者体液中HIT抗体的水平。还教导了使用该系统辅助HIT诊断，以及筛选或检测患者体液中HIT抗体滴度变化以确定对HIT易感性的方法。